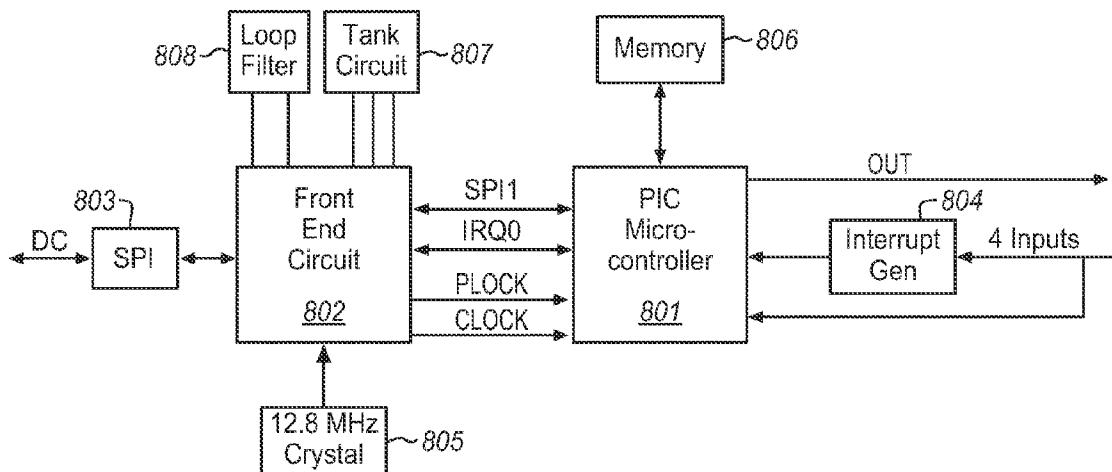




(86) Date de dépôt PCT/PCT Filing Date: 2013/02/07
(87) Date publication PCT/PCT Publication Date: 2013/08/15
(45) Date de délivrance/Issue Date: 2020/03/10
(85) Entrée phase nationale/National Entry: 2014/07/31
(86) N° demande PCT/PCT Application No.: US 2013/025077
(87) N° publication PCT/PCT Publication No.: 2013/119764
(30) Priorité/Priority: 2012/02/10 (US61/597,338)

(51) Cl.Int./Int.Cl. G01M 11/02(2006.01)
(72) Inventeurs/Inventors:
WIDMAN, MICHAEL F., US;
AGARWAL, NAVEEN, US
(73) Propriétaire/Owner:
JOHNSON & JOHNSON VISION CARE, INC., US
(74) Agent: NORTON ROSE FULBRIGHT CANADA
LLP/S.E.N.C.R.L., S.R.L.

(54) Titre : PROCEDE ET APPAREIL PERMETTANT DE MESURER LE FRONT D'ONDE D'UN DISPOSITIF
OPHTALMIQUE
(54) Title: METHOD AND APPARATUS FOR MEASURING THE WAVEFRONT OF AN OPHTHALMIC DEVICE



(57) Abrégé/Abstract:

This invention provides for a method and a wavefront measuring apparatus used to measure, in one or continuous measurements, one or more ophthalmic devices directly on a forming mandrel, in non-hydrated state and in a much faster way with high spatial resolution.

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2013/119764 A1

(43) International Publication Date
15 August 2013 (15.08.2013)(51) International Patent Classification:
G01M 11/02 (2006.01)

(21) International Application Number:

PCT/US2013/025077

(22) International Filing Date:

7 February 2013 (07.02.2013)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/597,338 10 February 2012 (10.02.2012)

(71) Applicant: **JOHNSON & JOHNSON VISION CARE, INC.** [US/US]; 7500 Centurion Parkway, Jacksonville, Florida 32256 (US).(72) Inventors: **WIDMAN, Michael F.**; 2864 Claire Lane, Jacksonville, Florida 32223 (US). **AGARWAL, Naveen**; 5869 Alamosa Circle, Jacksonville, Florida 32258 (US).(74) Agents: **JOHNSON, Philip S.** et al.; Johnson & Johnson, One Johnson & Johnson Plaza, New Brunswick, New Jersey 08933 (US).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,

[Continued on next page]

(54) Title: METHOD AND APPARATUS FOR MEASURING THE WAVEFRONT OF AN OPHTHALMIC DEVICE

(57) **Abstract:** This invention provides for a method and a wavefront measuring apparatus used to measure, in one or continuous measurements, one or more ophthalmic devices directly on a forming mandrel, in non-hydrated state and in a much faster way with high spatial resolution.

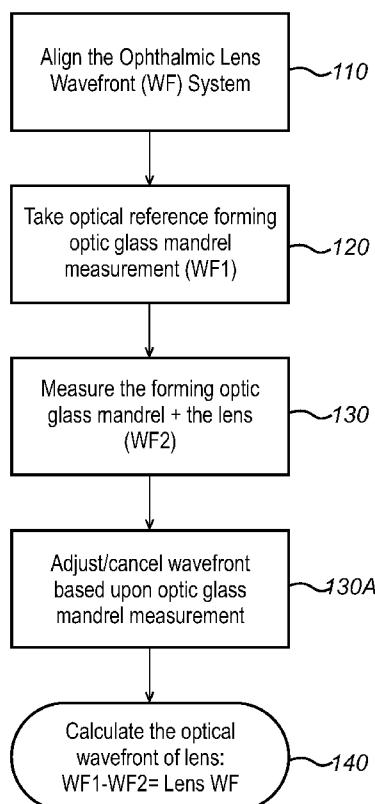FIG. 1
Process Map



WO 2013/119764 A1

Declarations under Rule 4.17:

- as to the identity of the inventor (Rule 4.17(i))
- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) **Designated States** (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

METHOD AND APPARATUS FOR MEASURING THE WAVEFRONT OF AN OPHTHALMIC DEVICE

FIELD OF USE

5 This invention describes a method and apparatus for obtaining accurate optical measurements of an ophthalmic device using an optical digital wavefront sensor and without contacting said ophthalmic device. More specifically, the apparatus uses an optical digital wavefront metrology technique to obtain simultaneous measurements of intensity and phase of the transmitted wavefront in one or more continuous
10 measurements.

BACKGROUND OF THE INVENTION

It has been known to measure the physical properties of contact lenses using various devices and methods, i.e. optical metrology. Conventionally, optical metrology involves directing an incident beam at an optical object, measuring the resulting diffracted beam, and analyzing the diffracted beam to determine various characteristics, such as the profile of the structure. However, traditional ophthalmic lenses are often made by cast molding, in which a monomer material is deposited in a cavity defined between optical surfaces of opposing mold parts. To prepare a lens using such mold parts, an uncured hydrogel lens formulation is placed between a plastic disposable front
15 curve mold part and a plastic disposable back curve mold part.
20 curve mold part and a plastic disposable back curve mold part.

The front curve mold part and the back curve mold part are typically formed via injection molding techniques wherein melted plastic is forced into highly machined steel tooling with at least one surface of optical quality.

The front curve and back curve mold parts are brought together to shape the lens

5 according to desired lens parameters. The lens formulation is subsequently cured, for example by exposure to heat and light, thereby forming a lens. Following cure, the mold parts are separated and the lens is removed from the mold parts for said conventional optical metrology. However, the nature of the injection molding processes and equipment make it difficult to form custom lenses specific to a particular patient's eye or

10 a particular application. Consequently, in prior descriptions, methods and apparatus for forming customized lenses via the use of free-form techniques have been described, such as in WO 2009/025848 and WO 2009/025845. An important aspect of these techniques is that a lens is produced in a novel manner where one of two lens surfaces is formed in a free-form fashion without cast molding, lathing or other tooling.

15 A free formed surface and base may include a free flowing fluent media included in the free formed surface. This combination results in a device sometimes referred to as a lens precursor. Fixing radiation and hydration treatments may typically be utilized to convert a Lens Precursor into an ophthalmic lens.

A freeform lens created in this manner may need to be measured in order to

20 ascertain the physical parameters of the lens. Therefore, new apparatus and methods are needed for measuring a lens formed from a precursor.

SUMMARY OF THE INVENTION

Accordingly, the present invention is directed to methods and apparatus for using a non-contact optical instrument for determining the measurement of an ophthalmic device, for example a dry contact lens that includes an UV-cured lens that has no moisture present in the lens, by using optical digital wavefront technology. Some key advantages of the present invention may include one or more of: a much faster way to obtain accurate measurements of dry contact lenses through single shot and real-time optical measurement, direct visualization of intensity and wavefront, a high dynamic range, a high spatial resolution as directly related to CCD camera resolution, vibration-insensitivity, and cost efficiency.

The present invention provides apparatus for measuring a physical characteristic of an ophthalmic device, the apparatus comprising:

an optic mandrel for forming an ophthalmic device using free-form technology; said optic mandrel comprising an optical effect;

15 a lens cancellation system comprising one or more lenses to collectively cancel said optical mandrel's optical effect;

an emitter functional to emit a wavelength of radiation in a direction towards the ophthalmic device;

a sensor functional to detect a transmitted wavefront based upon the emitted wavelength, wherein the transmitted wavefront's intensity and phase will be different based upon a physical characteristic of said ophthalmic device, and

a processor in logical communication with one or both of the emitter and the sensor; wherein the processor is programmed to transmit a logical signal based upon the reflecting wavefront's intensity and phase.

The apparatus may measure more than one physical characteristic. Preferably, the 5 apparatus obtains wavefront measurements of an ophthalmic device.

As used herein, the term "emitter" may mean "light source".

The optic mandrel, the lens cancellation system, the emitter and the sensor may be aligned. Preferably, the lens cancellation system, the emitter and the sensor are mounted on a rail. The rail may be a vertical rail, preferably a vertical optical rail.

10 In the apparatus, the sensor may comprise a digital wavefront camera. The digital wavefront camera may be capable of moving to change or vary continuously a distance along an optical axis of transmission of two or more intensity profiles. The digital wavefront camera may be vibration insensitive. The digital wavefront camera may further comprise a beam splitter to cause a production of a second image at a different 15 position along the optical axis of transmission. Alternatively or in addition, the digital wavefront camera may further comprise one or more magnification lenses dependant on the diaphragm in a light source and the working distance between the light source and the digital wavefront camera.

The apparatus may further comprise a kinematic mount for placement of said 20 optical mandrel for proper alignment with the lens cancellation system and the emitter. In addition, the apparatus may further comprise a vacuum for holding the mandrel fixture and the kinematic mount.

The apparatus may further comprise a top aperture and a bottom aperture, wherein said top aperture is slightly smaller than the bottom aperture and placed on top of the mandrel fixture without contacting said mandrel to create a physical barrier by limiting the light beam passing through defining a boundary condition for a solution of an 5 intensity transport equation. The top aperture may be changed to cover a different field of view. The bottom aperture may also be changed to further improve a dynamic range of measurement.

The lens cancellation system used in the apparatus described herein may comprise an assembly comprising three lenses inside of a tube, wherein a light beam can pass 10 through each of said lenses. The assembly may be placed perpendicularly to the rail. The light beam may be placed perpendicularly to the rail. The three lens cancellation system may include one or more of: an asphere lens, a plano-convex lens and a plano-concave lens to cancel out one or both of: defocus, and spherical aberrations of the forming optic mandrel which subsequently allows light coming out of the mandrel to be 15 collimated.

The processor may function in real time to generate one or more continuous wavefront measurements of said ophthalmic device.

The emitted radiation may be a high quality light beam with a monochromatic wavelength. The emitted radiation may comprise a monochromatic wavelength of from 20 about 630nm to about 635nm.

The present invention also provides a method of obtaining wavefront measurements of an ophthalmic device, the method comprising;
aligning an ophthalmic lens wavefront system,

taking an optical measurement of a forming optic mandrel and storing that intensity measurement of a forming optic mandrel as an intensity reference file, taking an optical measurement of a forming glass mandrel with a lens that may have been formed on it and storing that intensity file, using software in a processor capable of subtracting one intensity file from at least one other intensity file to obtain a value for an optical wavefront of a lens in real time.

The ophthalmic lens wavefront system used in the method of the present invention may comprise any of the apparatus described herein.

BRIEF DESCRIPTION OF THE DRAWINGS

15 Fig. 1 illustrates method steps that may be used to implement the present invention.

Fig. 2 illustrates apparatus components that may be useful in implementing the present invention comprising digital optical wavefront technology.

Fig. 3, Fig. 3A, & Fig. 3B illustrate exemplary kinematic mount apparatus components that may be useful in implementing the present invention.

20 Fig. 4 illustrates an example of mandrel wavefront optical cancellation, as opposed to no mandrel wavefront optical cancellation.

Fig. 4A illustrates an example of a dry lens wavefront after mandrel wavefront optical cancellation.

Fig. 5 illustrates additional method steps that may be used to implement the present invention.

DETAILED DESCRIPTION OF THE INVENTION

The present disclosure provides for methods and apparatus for obtaining an 5 optical wavefront measurement of an ophthalmic device. In the following sections, detailed descriptions of the invention will be given. The description of both preferred and alternative embodiments though thorough are exemplary only, and it is understood to those skilled in the art that variations, modifications, and alterations may be apparent. It is therefore to be understood that the exemplary embodiments do not limit the broadness 10 of the aspects of the underlying invention as defined by the claims.

GLOSSARY

As used herein, the term “comprising” encompasses “including” as well as “consisting” and “consisting essentially of” *e.g.* an apparatus “comprising” X may consist exclusively of X or may include something additional *e.g.* X + Y.

15 “Fluent lens reactive media” as used herein means a reactive mixture that is flowable in either its native form, reacted form, or partially reacted form and, a portion or all reactive media may be formed upon further processing into a part of an ophthalmic lens.

“Free-form” as used herein refers to a surface that is formed by crosslinking of a 20 reactive mixture via exposure to actinic radiation on a voxel by voxel basis, with or without a fluent media layer, and not shaped according to a cast mold, lathe, or laser ablation.

“Lens forming mixture” and sometimes referred as “reactive mixture” or “RMM”

(reactive monomer mixture) herein refers to a monomer or prepolymer material which may be crosslinked to form an ophthalmic lens. Lens-forming mixtures may comprise one or more additives such as: UV blockers, tints, photoinitiators or catalysts, and other additives one might desire in an ophthalmic lenses such as, contact or intraocular lenses.

5 “Lens precursor” as used herein, refers to a composite object consisting of a lens precursor form and a fluent lens reactive mixture in contact with the lens precursor form. For example, the fluent lens reactive media may be formed in the course of producing a lens precursor form within a volume of reactive mixture. Separating the lens precursor form and adhered fluent lens reactive media from a volume of reactive mixture used to 10 produce the lens precursor form may generate a lens precursor. Additionally, a lens precursor may be converted to a different entity by either the removal of significant amounts of fluent lens reactive mixture or the conversion of a significant amount of fluent lens reactive media into non-fluent, incorporated material.

“Lens precursor form” as used herein, means a non-fluent object with at least one 15 optical quality surface which is consistent with being incorporated, upon further processing, into an ophthalmic lens.

“Ophthalmic lens” as used herein and sometimes referred to as “ophthalmic device” or “lens” refers to any ophthalmic device that resides in or on the eye. These devices can provide optical correction or may be cosmetic. For example, the term “lens” can refer to 20 a contact lens, intraocular lens, overlay lens, ocular insert, optical insert or other similar device through which vision is corrected or modified, or through which eye physiology is cosmetically enhanced (e.g., iris color) without impeding vision. The preferred lenses of

the invention may be soft contact lenses made from silicone elastomers or hydrogels, which include but are not limited to silicone hydrogels, and fluorohydrogels.

Measurements of one or more ophthalmic devices may be taken in its unhydrated lens state, and on a mandrel on which, a lens may be formed using free-form technology.

5 Included in the present disclosure are a digital wavefront camera and an objective lens. Also included, may be a mandrel fixture which may be mounted on a kinematic mounting device assembly that may include a three-lens mandrel cancellation system inside of a tube, a bottom aperture underneath, a mandrel fixture and a top aperture that is placed directly on top of the glass mandrel without making physical contact, a light
10 source, a pinhole, diaphragm, and an asphere lens located in the bottom part of the apparatus. All of these components may be mounted perpendicularly to a vertical optical rail and adjusted, until the output beam from a light source is parallel with a rail and may be collimated as it exits the forming optic mandrel. Collimating light may be a parallel beam of light that has a flat wavefront, which means that the intensity of light does not
15 change along an optical axis (referred to as “z direction”).

A series of steps may be implemented to measure the free-formed unhydrated ophthalmic lenses. First, an optical measurement of a forming optic glass mandrel may be taken in transmission mode without a lens on it to obtain the optical wavefront of a base mandrel. That wavefront data may subsequently be stored as a reference file. A
20 lens may subsequently be made on the same exact mandrel fixture which may be mounted onto said kinematic mount assembly. Subsequently, an optical measurement of a forming optic glass mandrel with a lens on it may be taken, in transmission mode and that wavefront data file may also be stored. The two data files may be subtracted from

each other, thereby giving an optical wavefront measurement of a lens in transmission.

Measurements may be made in transmission mode, but alternatively or in addition taking a measurement in reflective mode may be equally possible.

Referring now to **Fig. 1**, is a flow chart that illustrates method steps that may be used to obtain an optical wavefront of a lens. Various steps may include one or more of: aligning an ophthalmic lens wavefront (WF) system **110**, followed by taking an optical wavefront measurement of a forming optic glass mandrel and storing that wavefront data as a reference file (wavefront 1) **120**, followed by taking an optical wavefront measurement of a forming optic glass mandrel with a lens that may have been formed on that particular optic and storing that wavefront data file (wavefront 2) **130**, followed by subtracting a wavefront 2 file from a wavefront 1 file and obtaining a value for an optical wavefront of an ophthalmic lens **140**.

Referring now to **Fig. 2**, a side view of an exemplary wavefront measurement system mounted perpendicularly to a vertical optical rail **255** is depicted. A light source **200** may act as a reference for remaining components when aligning an apparatus and may be placed approximately 125mm from a vertical optical rail **255**. An overall objective purpose of aligning an apparatus may be so a collimated light beam may be produced parallel to a rail **255** when it exits a forming optic glass mandrel **235**. A light source **200**, which may have a wavelength of about 633 nm, may contain various optical elements inside and generate a high quality light beam. However, wavelength may vary, 633nm is described herein for illustrative purposes but any other monochromatic wavelength may be used. A pinhole **205**, which adjusts the diameter of the light beam, may restrict an uncollimated beam of light. An aspheric focusing lens **210** subsequently

focuses a beam of light and collimates it. Before a collimated beam enters a mandrel cancellation optical system **220**, there may be a bottom aperture **215** that may sit directly above an aspheric focusing lens **210** and may be mounted either independently or to the bottom of a “LP1A” (Axis adjustable) stage **265**. An adjustable bottom aperture **215** 5 controls a diameter of a collimated light coming from an aspheric focusing lens **210**. A purpose of a bottom aperture **215** may be to restrict a field of view to allow a homogenous and uniform intensity profile and prevent saturation of a digital wavefront camera (also referred hereon as “DWC”) **250**.

Just above a bottom aperture **215** may be a kinematic mounting device **225**, which 10 may contain a tube inside of it comprising a series of lenses, which may collectively form a mandrel cancellation optical system **220**. For example, a set of three lenses may be used: an asphere lens, a plano-convex lens, and a plano-concave lens. A purpose of a mandrel cancellation optical system **220** may be to cancel out both defocus and spherical aberration of a forming optic glass mandrel **235**, which subsequently allows light coming 15 out of a mandrel **235** to be collimated. Where there are three lenses of a mandrel cancellation optical system **220**, the power and distances between the three lenses may be designed in such a way to cancel out an optical effect of a mandrel **235** in a 10mm field of view, thereby causing the DWC to detect a flat wavefront. Otherwise, an optical effect of a mandrel **235** may introduce errors in calculation of a lens wavefront upon 20 subtracting. Directly above a mandrel cancellation optical system **220** may be a kinematic mounting device **225** for the mandrel fixture **230** which may be mounted on top.

Referring now to both, **Fig. 3** and **Fig. 3A**, **Fig. 3** a schematic view of an exemplary kinematic mounting device assembly **325** is depicted. **Fig. 3A** represents a top view of a kinematic mounting device assembly **325**. A forming optic assembly glass mandrel fixture **330** may be held in place by two adjuster ball pins **315** (only one of which is illustrated in **Fig. 3**) and a plunger **310**. A plunger **310** rides in a grove that may have a spring **320** behind it, which may be captivated by spring pin assembly screw **340** representing a spring pin assembly **345**. A plunger **310** may move in and out freely, engaging a mandrel fixture **330** in a notch **355**. A notch **355** may keep a mandrel fixture **330** clocked in a desired position when a spring **320** pushes a plunger **310** into a notch **355**. A spring pin assembly **345** via a plunger **310**, pushes a mandrel fixture **330** towards the left (in **Fig. 3**), an edge of which subsequently impinges on adjuster ball pins **315**. Adjustment of either of adjuster ball pins **315**, may adjust an entire X,Y position of a mandrel fixture **330**. Height and level of a mandrel fixture **330** may be adjusted by adjusting screws **305** and locating balls **300**. A vacuum **350** may be applied to a space between a mandrel fixture **330** and a kinematic mount **325**. A vacuum **350** holds a mandrel fixture **330** down onto the balls **300**, but not to a point that a spring **320** and plunger **310** may be inhibited from pushing a mandrel fixture **330** against adjuster ball pins **315**. A forming optic glass mandrel **335** may be positioned on a mandrel fixture **330**. Different geometries of a kinematic mounting device **325** may be used.

Referring now to **Fig. 3B**, represents a broken view of a kinematic mounting device **325** and an encapsulating lens tube **360** that houses three lenses of a mandrel cancellation optical system. Also illustrated, may be a location of a mandrel cancellation

optical system contained inside of a kinematic mount **325**. The kinematic mounting device **325** may comprise a locking nut **327**.

Referring back to **Fig. 2**, a top aperture **240** may be attached to a rail **255** directly above a mandrel fixture **230**. A top aperture **240** may be placed directly on top of a 5 mandrel fixture **230** as close to a forming optic glass mandrel **235** without actually physically touching it. Different geometries of a top aperture **240** may be used. A top aperture **240**, which may be slightly smaller than a bottom aperture **215**, may restrict a diameter of a collimated light beam exiting a forming optic glass mandrel **235**, causing a **DWC 250** only to get intensity from a collimated light in only a certain zone restricted by 10 a top aperture **240**. A top aperture **240** diameter may be changed to cover a different field of view. A purpose of a top aperture, may be to create a physical barrier by limiting light to pass through only that aperture which defines a boundary condition for a solution of an intensity transport equation, which assumes that an intensity of light outside of a diameter of a top aperture **240** may be equal to zero. An adjustable top aperture **240**, or various 15 combinations of a top aperture **240** and bottom aperture **215** may be used to improve a dynamic range of measurement.

An objective lens **245** may sit directly above a top aperture **240** and a **DWC 250** may be attached to an objective lens **245**. A **DWC 250** may be mounted on an X, Y stage **260**. Alternatively, a rotation stage may be mounted here. Inside of a **DWC** there may 20 be a beam splitter which may cause a second intensity image at a fixed distance along the optical axis of transmission from a first intensity image to be formed. Distance between two images may be changed to another fixed value or varied continuously using a movable camera. A working distance between a **DWC 250** and a diaphragm in a light

source **200** may be dependent upon an objective camera lens magnification used. An objective lens camera magnification may be .333 and working distance may be 69 mm.

There may be three alignment positions of a DWC **250**. First, a DWC **250** and objective lens **245** may be positioned on a vertical optical rail **255** in position 1. In 5 position 1, an objective lens **245** images a top aperture **240** in a DWC **250**, which produces a first image in focus, referred to as image 1. Second, a DWC **250** and objective lens **245** may be positioned down on a vertical optical rail **255** in position 2, in which image 1 becomes fuzzy. In position 2, a beam splitter in a DWC **250** may subsequently cause a production of a second image, referred to as image 2. Finally, a 10 DWC **250** and objective lens **245** may be subsequently positioned in between image 1 and image 2, in a final position. In a final position, image 1 and image 2 may be both equally fuzzy.

Referring now to both **Fig. 4** and **Fig. 4A**, **Fig. 4** is an example of a computer generated optical wavefront of a reference without mandrel optical cancellation **400** and 15 an optical wavefront of a reference mandrel with mandrel optical cancellation **410**. **Fig. 4A** illustrates an example of a computer generated wavefront of a dry lens obtained after removing a mandrel optical wavefront **420**. After a system has been aligned, a first measurement taken may be an optical reference measurement of a glass mandrel without 20 a lens on it, shown as example **410**. That data may be referred to as wavefront 1 and may be stored. A second optical measurement may subsequently be taken of a glass mandrel with a lens on it and that data which is referred to as wavefront 2, may be stored. Finally, wavefront 1 may be digitally subtracted from wavefront 2 to yield a lens wavefront, shown as an example in **420**.

Referring now to **Fig. 5**, represents a picture diagram **500** to illustrate a process by which the wavefront measurement **540** may be done through acquisition of image 1 **520** and image 2 **530** from a DWC **510**. During a measurement, two intensity images, image 1 **520** and image 2 **530** may be obtained. The software utilized may be referred to as

5 Getwave software (version 1.0.9) designed by Phaseview. However, other software may be used that performs the same function. For illustration purposes, image 1 **520** may be referred to as intensity distribution 1 and image 2 **530** as intensity distribution 2. These two intensity distribution images may subsequently be used in a calculation, which may be made inside of software, based upon the difference between the two images.

10 Subsequently, an optical wavefront may be constructed for a measurement. More specifically, software utilizes a generic equation, which may be referred to as the *intensity transport equation*, the equation which is:

$$-\kappa \frac{\partial \phi_z}{\partial r} I_z(r) = \underbrace{I_z(r) \nabla^2 \phi_z(r)}_{\text{Curvature}} + \underbrace{\nabla I_z(r) \cdot \nabla \phi_z(r)}_{\text{Slope}}$$

15 The intensity transport equation may be implemented in such a way by using a particular algorithm, to allow for a measurement of a glass mandrel or a glass mandrel with a lens on it and to collect intensity data from both measurements. Intensity data may subsequently be converted into an optical wavefront. An optical wavefront describes a path of light in terms of a light's intensity and phase. A wavefront may be measured in terms of one or more of: Zernike coefficients, as peak to valley ("PTV"), and wavefront 20 root mean square ("RMS"), as compared to flat wave. Subsequent to wavefront calculations for both a reference measurement of a glass mandrel without a lens (wavefront 1) and a measurement of a glass mandrel with a lens (wavefront 2); two

wavefront files, wavefront 2 and wavefront 1, may be subtracted from one another to obtain a value for an optical wavefront of a lens.

Conclusion

The present disclosure, as described above and as further defined by the claims 5 below, provides methods and apparatus for measuring physical characteristics of one or more ophthalmic devices.

CLAIMS:

1. Apparatus for measuring a physical characteristic of an ophthalmic device, the apparatus comprising:

an optic mandrel for forming an ophthalmic device using free-form technology; said optic mandrel comprising an optical effect;

a lens cancellation system comprising more than one lens to collectively cancel said optical mandrel's optical effect, wherein said lens cancellation system comprises an assembly comprising three lenses inside of a tube, wherein a light beam can pass through each of said lenses and may be placed perpendicularly to a rail, wherein said three lens cancellation system can include one or more of: an asphere lens, a plano-convex lens and a plano-concave lens to cancel out one or both of: defocus, and spherical aberrations of the forming optic mandrel which subsequently allows light coming out of the mandrel to be collimated;

an emitter functional to emit a wavelength of radiation in a direction towards the ophthalmic device;

a sensor functional to detect a transmitted wavefront based upon the emitted wavelength, wherein the transmitted wavefront's intensity and phase will be different based upon a physical characteristic of said ophthalmic device, and

a processor in logical communication with one or both of the emitter and the sensor; wherein the processor is programmed to transmit a logical signal based upon the reflecting wavefront's intensity and phase.

2. The apparatus of claim 1 wherein the optic mandrel, the lens cancellation system, the emitter and the sensor are aligned.

3. The apparatus of claim 1 or claim 2 wherein the optic mandrel, the lens cancellation system, the emitter and the sensor are mounted on a rail, preferably the rail is a vertical optical rail.
4. The apparatus of any one of claim 1-3 wherein the sensor comprises a digital wavefront camera, optionally the digital wavefront camera is capable of moving to change or vary continuously a distance along an optical axis of transmission of two or more intensity profiles, optionally the digital wavefront camera is vibration insensitive, optionally the digital wavefront camera further comprises a beam splitter to cause a production of a second image at a different position along the optical axis of transmission, optionally the digital wavefront camera further comprises one or more magnification lenses dependant on the diaphragm in a light source and the working distance between the light source and the digital wavefront camera.
5. The apparatus of any one of claims 1-4 further comprising a kinematic mount for placement of said optical mandrel for proper alignment with the lens cancellation system and the emitter, optionally further comprising a vacuum for holding the mandrel fixture and the kinematic mount.
6. The apparatus of any one of claims 1-5 further comprising a top aperture and a bottom aperture, wherein said top aperture is slightly smaller than the bottom aperture and placed on top of the mandrel fixture without contacting said mandrel to create a physical barrier by limiting the light beam passing through defining a boundary condition for a solution of an intensity transport equation.
7. The apparatus of Claim 6 wherein said top aperture can be changed to cover a different field of view.
8. The apparatus of Claim 6 or claim 7 wherein said bottom aperture can also be changed to further improve a dynamic range of measurement.

9. The apparatus of any one of claims 1-8 wherein the processor functions in real time to generate one or more continuous wavefront measurements of said ophthalmic device.

10. The apparatus of any one of claims 1-9 wherein the emitted radiation is a high quality light beam with a monochromatic wavelength.

11. The apparatus of any one of claims 1-10 wherein the emitted radiation comprises a monochromatic wavelength of from about 630nm to about 635mm.

12. A method for obtaining wavefront measurements of an ophthalmic device, the method comprising;

aligning an ophthalmic lens wavefront system, wherein the ophthalmic lens wavefront system comprises the apparatus of any one of claims 1 to 11,

taking an optical measurement of a forming optic mandrel and storing that intensity measurement of a forming optic mandrel as an intensity reference file,

taking an optical measurement of a forming glass mandrel with a lens that may have been formed on it and storing that intensity file,

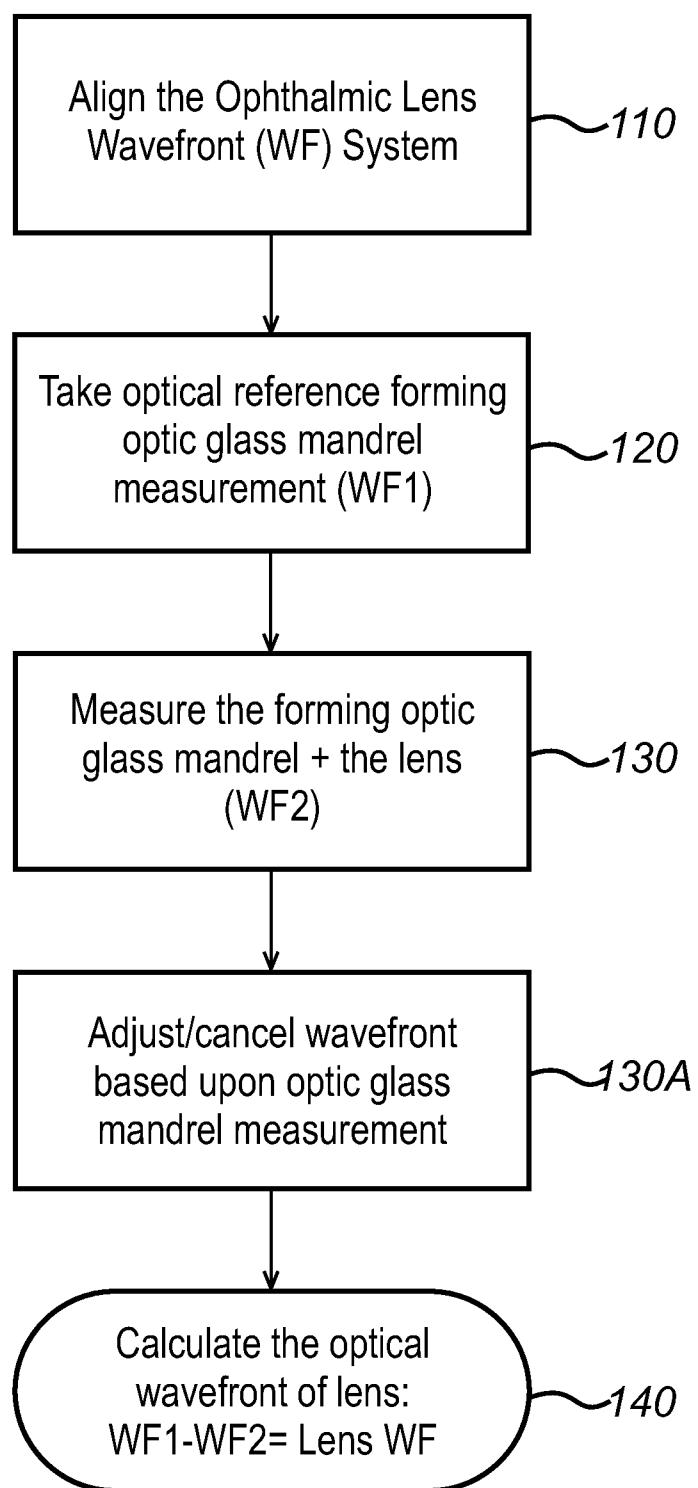
using software in a processor capable of subtracting one intensity file from at least one other intensity file to obtain a value for an optical wavefront of a lens in real time.

13. The method of claim 12 further comprising the processor implementing an intensity transport equation and an algorithm.


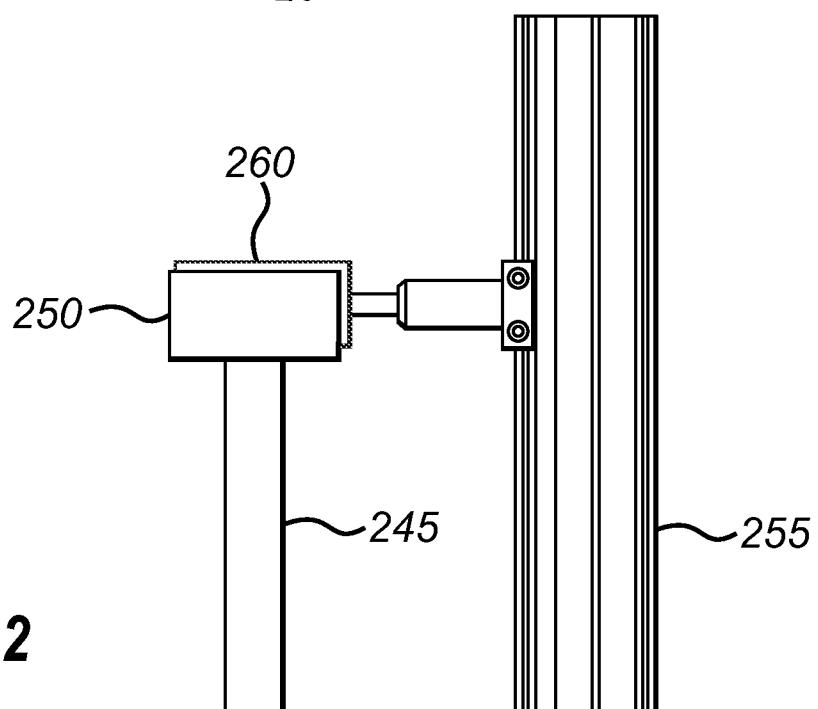
14. The method of claim 12 or claim 13 wherein intensity data may subsequently be converted into an optical wavefront and preferably wherein the optical wavefront describes a path of light in terms of a light's intensity and phase.

FIG. 1

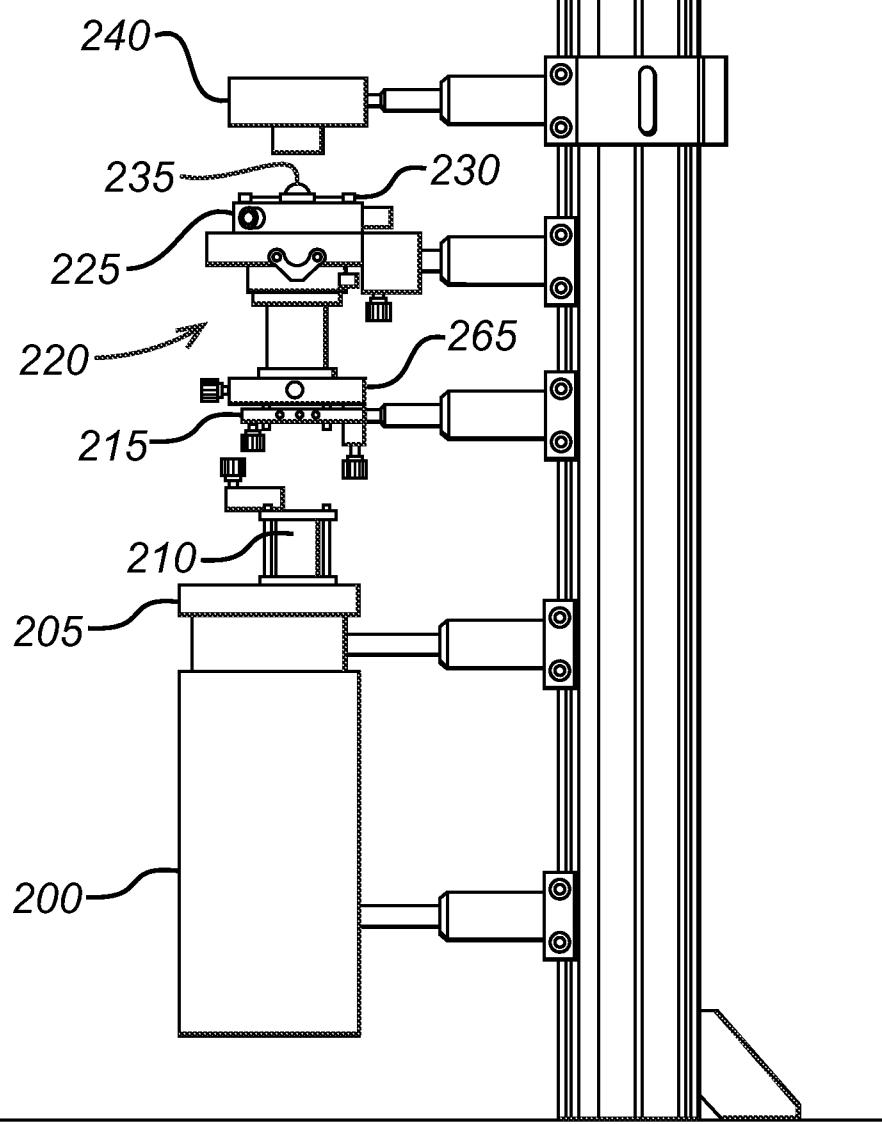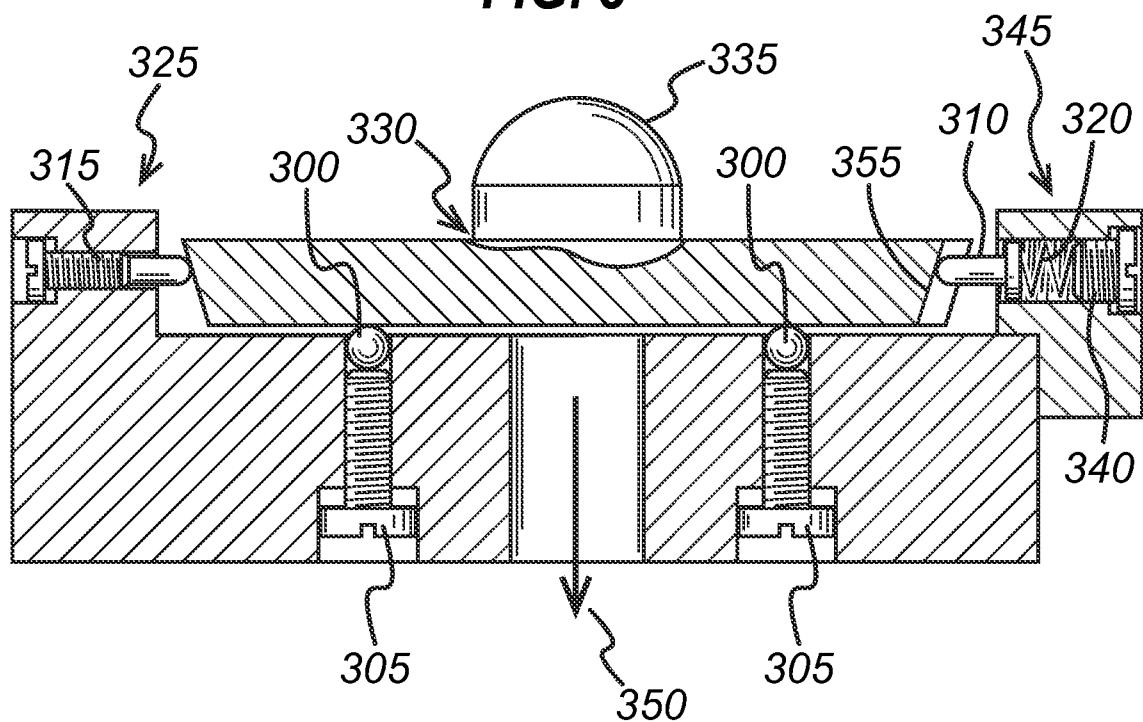
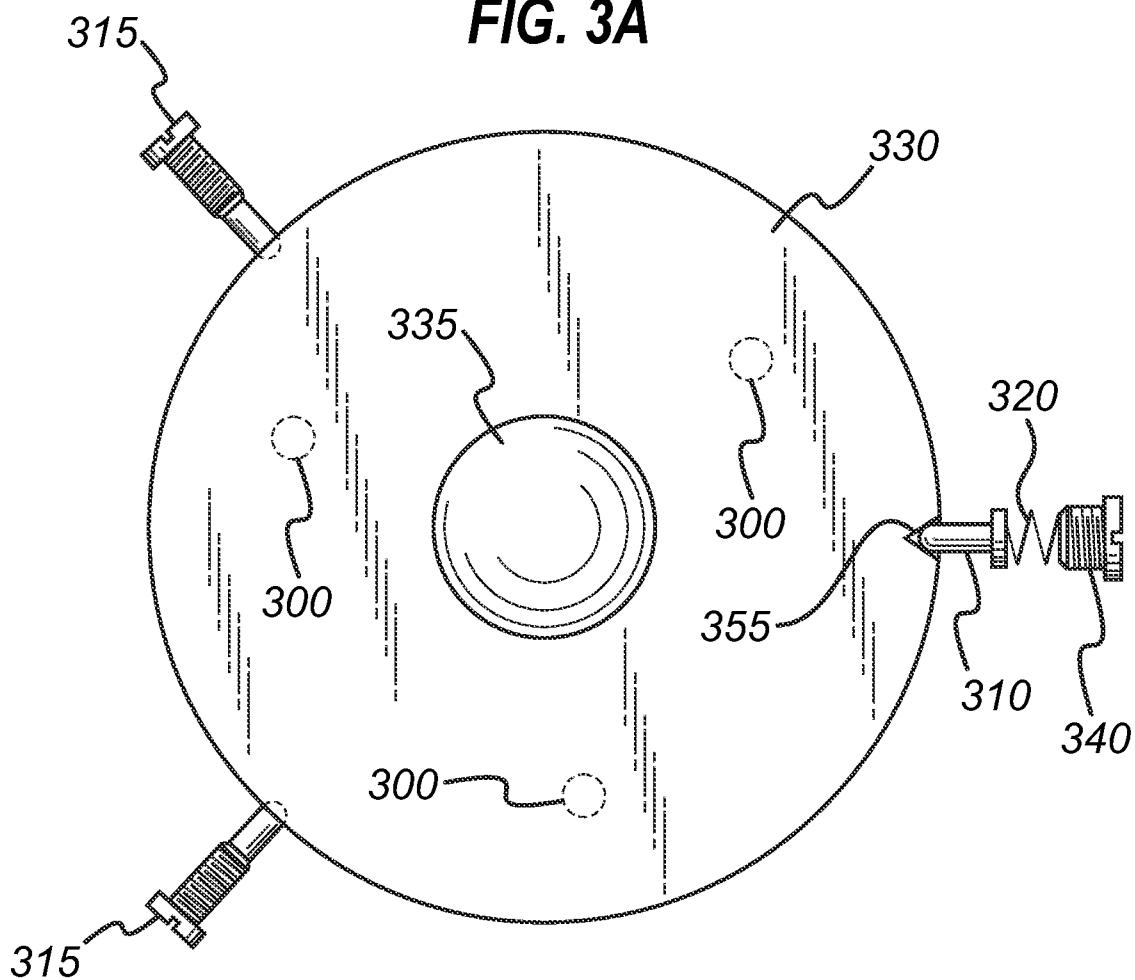
Process Map



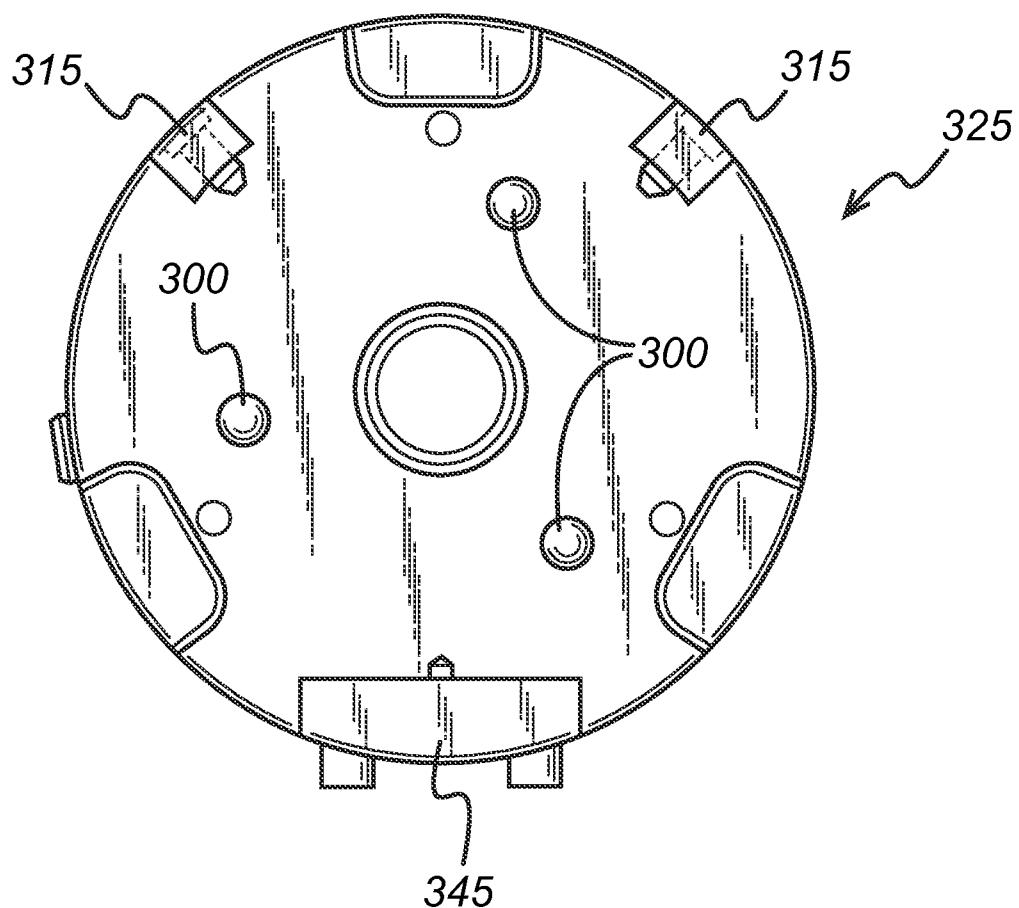
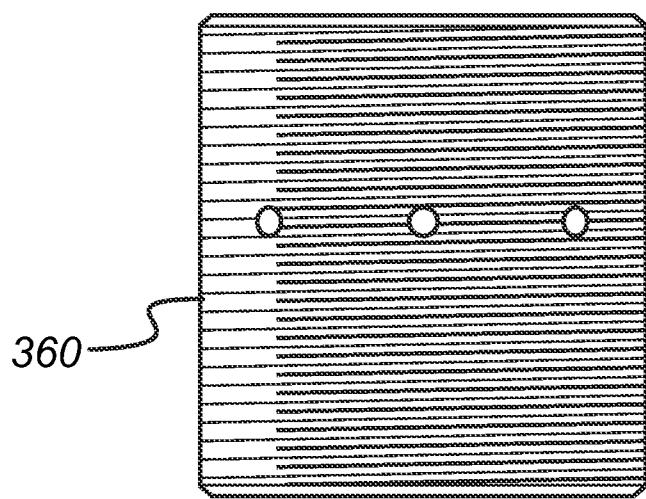
2/8

**FIG. 2**

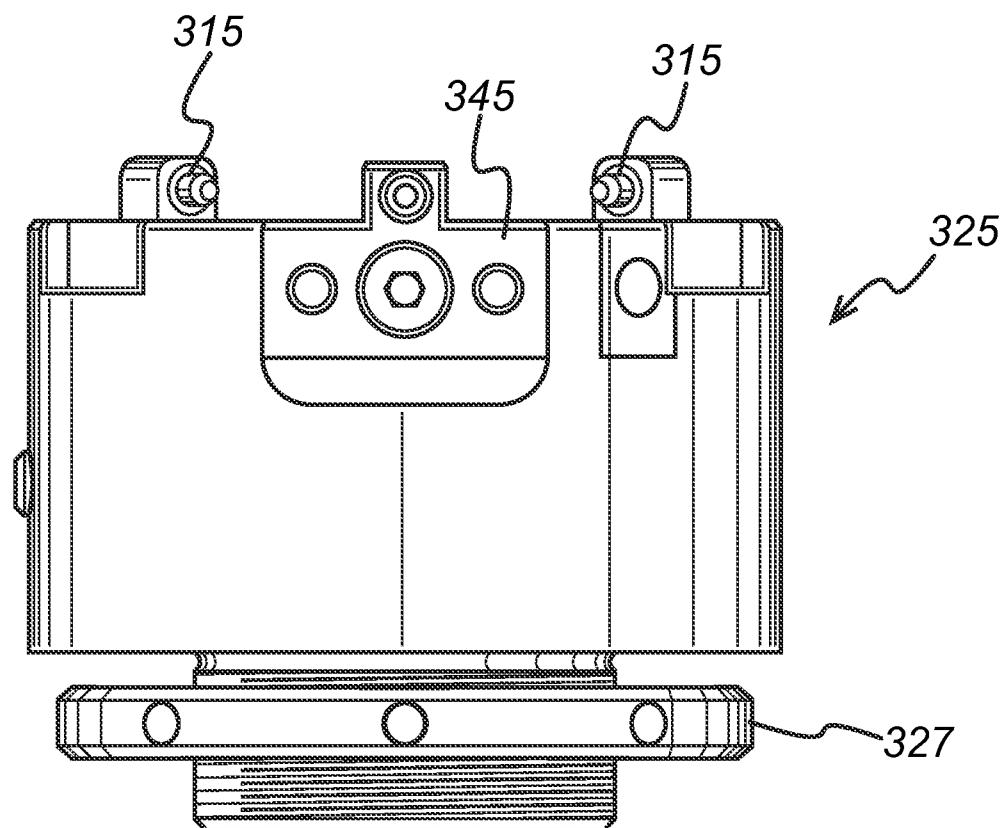
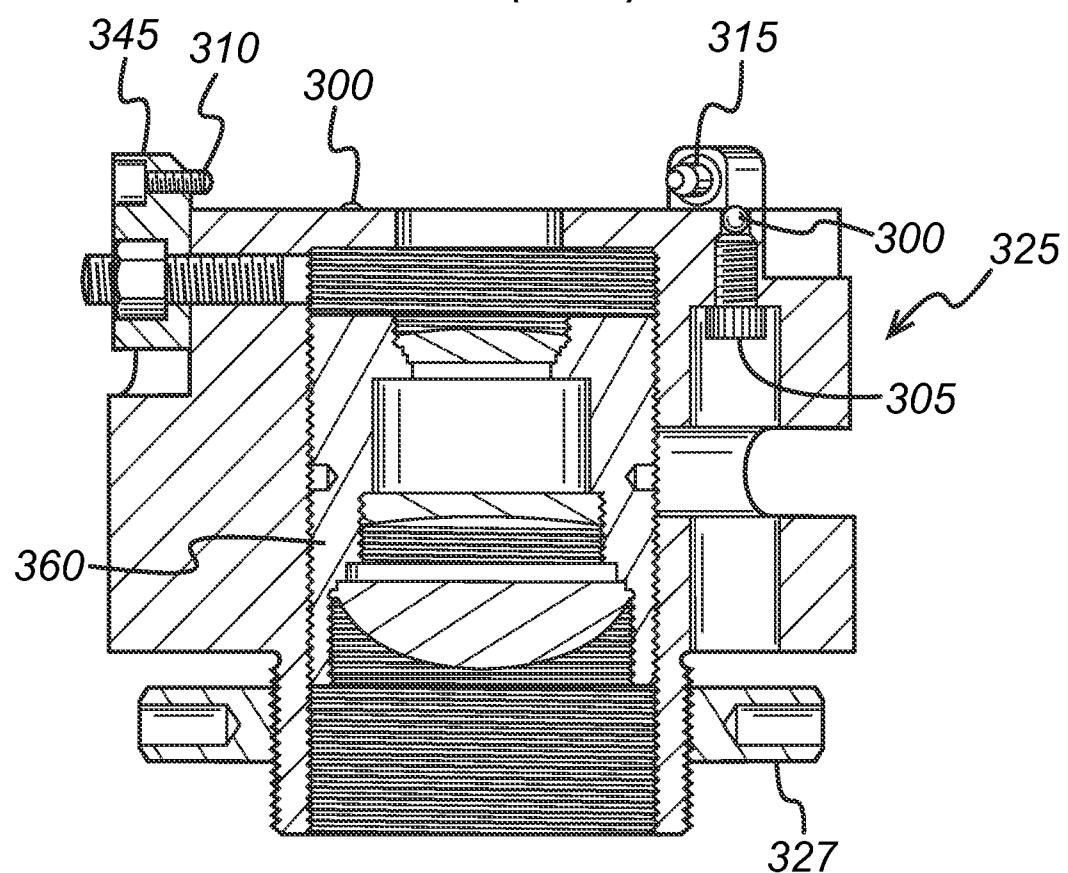
3/8

FIG. 3**FIG. 3A**

4/8


**FIG. 3B**

5/8

**FIG. 3B (contd)**


6/8

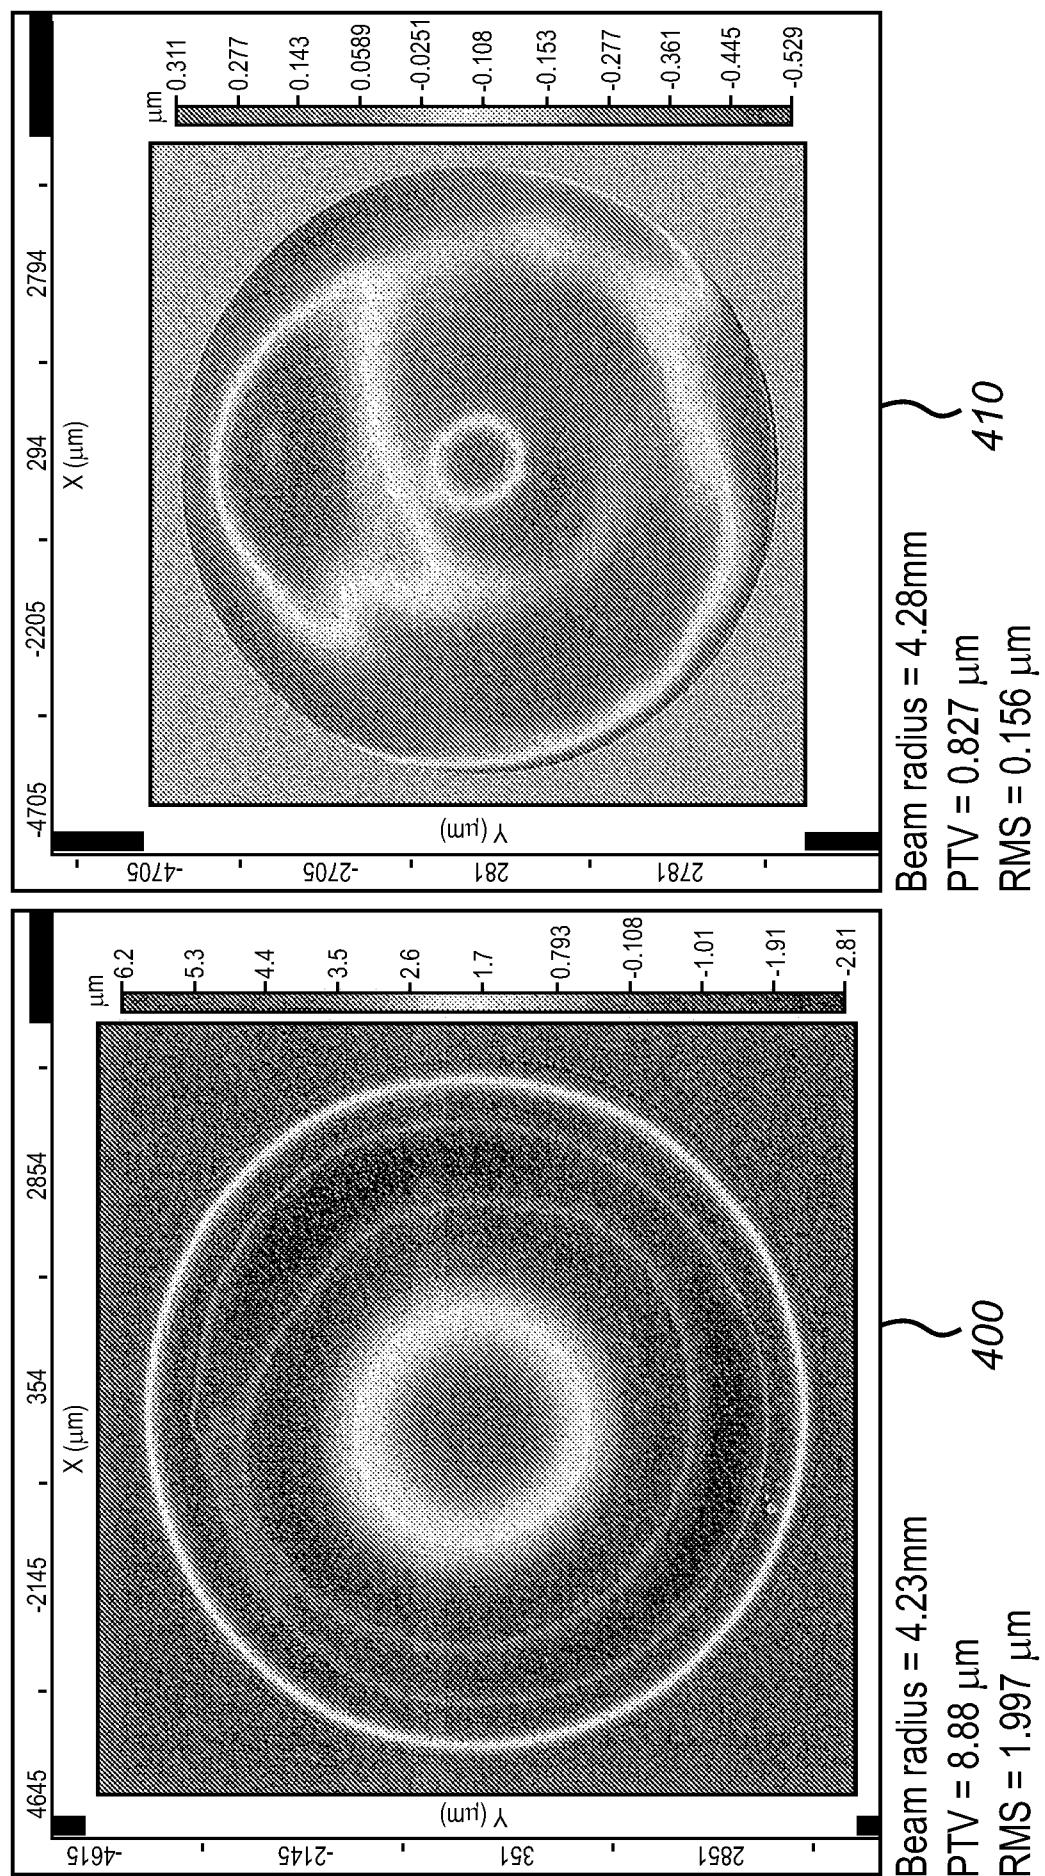FIG. 4 Mandrel Optical Cancellation



7/8

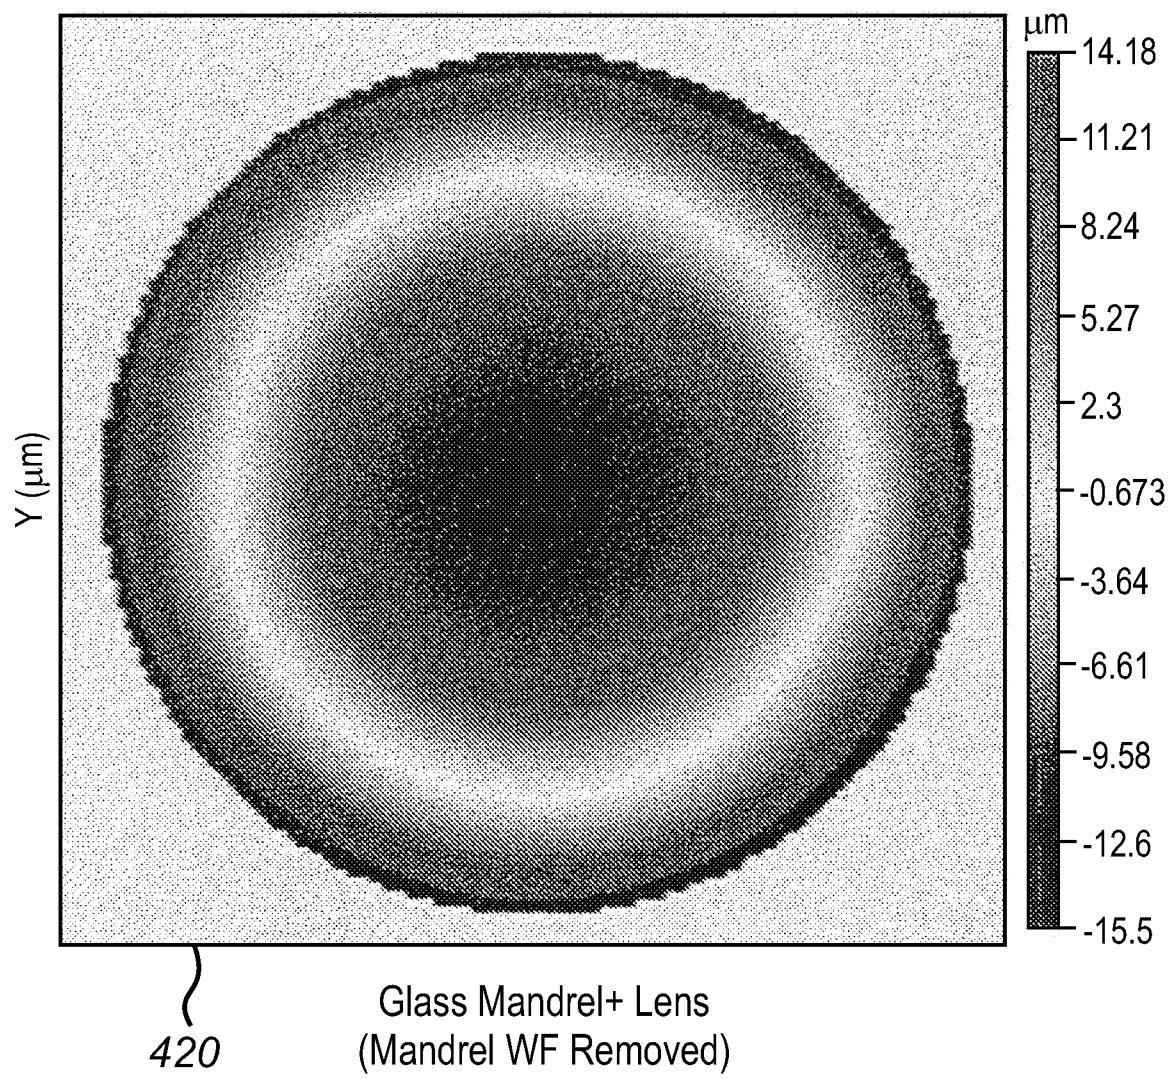FIG. 4A
Custom Optic WF Measurement



8/8

