



(51) International Patent Classification:

A61F 2/24 (2006.01) A61L 27/56 (2006.01)
A61L 27/48 (2006.01)

(21) International Application Number:

PCT/US2012/040529

(22) International Filing Date:

1 June 2012 (01.06.2012)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/492,324 1 June 2011 (01.06.2011) US
13/485,823 31 May 2012 (31.05.2012) US

(71) Applicant (for all designated States except US): **W.L. GORE & ASSOCIATES, INC.** [US/US]; 555 Paper Mill Road, Newark, DE 19711 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **BRUCHMAN, William, C.** [US/US]; 2616 S. Lantis Lane, Camp Verde, AZ 86322 (US). **HARTMAN, Cody, L.** [US/US]; 2307 N. Talkington Dr., Flagstaff, AZ 86001 (US).

(74) Agents: **FORDENBACHER, Paul** et al.; W.L. Gore & Associates, Inc., 551 Paper Mill Road, P.O. Box 9206, Newark, DE 19714-9206 (US).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) Title: DURABLE MULTI-LAYER HIGH STRENGTH POLYMER COMPOSITE SUITABLE FOR IMPLANT AND ARTICLES PRODUCED THEREFROM

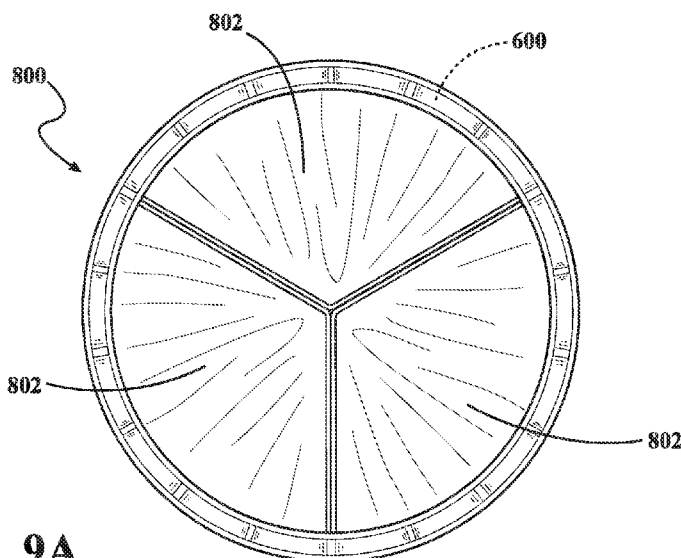**FIG. 9A**

(57) Abstract: A thin, biocompatible, high-strength, composite material is disclosed that is suitable for use in various implanted configurations. The composite material maintains flexibility in high-cycle flexural applications, making it particularly applicable to high-flex implants such as heart pacing lead or heart valve leaflet. The composite material includes at least one porous expanded fluoropolymer layer and an elastomer substantially filling substantially all of the pores of the porous expanded fluoropolymer.



**DURABLE MULTI-LAYER HIGH STRENGTH POLYMER COMPOSITE
SUITABLE FOR IMPLANT AND ARTICLES PRODUCED THEREFROM**

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation-in-part application of co-pending United States Patent Application Serial No. 13/078,774 filed April 1, 2011, and also claims priority to provisional application Serial No. 61/492,324 filed June 1, 2011.

BACKGROUND

Field

[001] This disclosure relates to materials used in medical implants. More particularly, the disclosure relates to a biocompatible material suitable for use in high-cycle flexural applications including artificial heart valves.

Background

[002] Artificial heart valves preferably should last at least ten years in vivo. To last that long, artificial heart valves should exhibit sufficient durability for at least four hundred million cycles or more. The valves, and more specifically heart valve leaflets, must resist structural degradation including the formation of holes, tears, and the like, as well as adverse biological consequences including calcification and thrombosis.

[003] Fluoropolymers, such as expanded and non-expanded forms of polytetrafluoroethylene (PTFE), modified PTFE, and copolymers of PTFE, offer a number of desirable properties, including excellent inertness and superior biocompatibility, and, therefore make ideal candidate materials. PTFE and expanded PTFE (ePTFE) have been used to create heart valve leaflets. It has been shown, however, that PTFE stiffens with repeated flexure, which can lead to unacceptable flow performance. Failure due to formation of holes and tears in the material has also been observed. A variety of polymeric materials have previously been employed as prosthetic heart valve leaflets. Failure of these leaflets due to stiffening and hole formation occurred within two years of implant. Efforts to improve

leaflet durability by thickening the leaflets resulted in unacceptable hemodynamic performance of the valves, that is, the pressure drop across the open valve was too high.

[004] As such, it remains desirable to provide a biocompatible artificial heart valve design that lasts at least ten years in vivo by exhibiting sufficient durability for at least about four hundred million cycles of flexure or more.

SUMMARY

[005] According to embodiments, an implantable article is provided for regulating blood flow direction in a human patient. Such an article may include, but is not limited to, a cardiac valve or a venous valve

[006] In one embodiment, the implantable article includes a leaflet comprising a composite material with at least one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the at least one fluoropolymer layer, wherein the composite material comprises less than about 80% fluoropolymer by weight.

[007] In other exemplary embodiments, the implantable article includes a leaflet having a thickness and formed from a composite material having more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer, wherein the leaflet has a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 5.

[008] In other exemplary embodiments, the implantable article includes a support structure; a leaflet supported on the support structure, the leaflet having a thickness and formed from a composite material having more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer, wherein the leaflet has a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 5.

[009] In other exemplary embodiments, the implantable article includes a leaflet cyclable between a closed configuration for substantially preventing blood flow through the implantable article and an open configuration allowing blood flow through the implantable article. The leaflet is formed from a plurality of fluoropolymer layers and having a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of

less than about 5. The leaflet maintains substantially unchanged performance after actuation of the leaflet at least 40 million cycles.

[010] In other exemplary embodiments, the implantable article includes a leaflet cyclable between a closed configuration for substantially preventing blood flow through the implantable article and an open configuration allowing blood flow through the implantable article. The implantable article also includes a cushion member located between at least a portion of the support structure and at least a portion of the leaflet, wherein the cushion member is formed from a plurality of fluoropolymer layers and having a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 5. The leaflet maintains substantially unchanged performance after actuation of the leaflet at least 40 million cycles.

[011] In exemplary embodiments, a method is provided for forming a leaflet of an implantable article for regulating blood flow direction in a human patient, which includes the steps of: providing a composite material having more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer; and bringing more than one layer of the composite material into contact with additional layers of the composite material by wrapping a sheet of the composite material with a starting and ending point defined as an axial seam adhered to itself.

[012] In exemplary embodiments, an implantable article is provided for regulating blood flow direction in a human patient, which includes a polymeric leaflet having a thickness of less than about 100 μm .

[013] In another embodiment, the implantable article includes a generally annular shaped support structure having a first end and an opposite second end. The first end of the support structure has a longitudinally extending post. A sheet of leaflet material extends along an outer periphery of the support structure and forms first and second leaflets extending along on opposite sides of the post. A cushion member is coupled to the post and provides a cushion between the post and the leaflets to minimize stress and wear on the leaflets as the leaflets cycle between open and closed positions.

BRIEF DESCRIPTION OF THE DRAWINGS

[014] The accompanying drawings are included to provide a further understanding of the invention and are incorporated in and constitute a part of this specification, illustrate exemplary embodiments of the invention, and together with the description serve to explain the principles of the invention.

[015] Figures 1A, 1B, 1C, and 1D are front, side and top elevational views, and a perspective view, respectively, of a tool for forming a heart valve leaflet, in accordance with an embodiment;

[016] Figure 2A is a perspective view of a cushion pad being stretched over a leaflet tool, in accordance with an embodiment;

[017] Figure 2B is a perspective view of a release layer being stretched over the cushion pad covered leaflet tool in Figure 2A, in accordance with an embodiment;

[018] Figures 3A, 3B and 3C are top, side and front elevational views illustrating a step in the formation of a valve leaflet, in which the leaflet tool covered by the cushion pad and release layer (shown in Figures 2A and 2B, respectively) is positioned over a composite material for cutting and further assembly, in accordance with an embodiment;

[019] Figure 4 is a top elevational view of a tri-leaflet assembly prior to cutting excess leaflet material, in accordance with an embodiment;

[020] Figure 5A is a perspective view of the tri-leaflet assembly and a base tool, in accordance with an embodiment;

[021] Figure 5B is a perspective view of the tri-leaflet assembly and base tool aligned and assembled to form a base tool assembly, in accordance with an embodiment;

[022] Figure 6A is a flattened plane view of a stent frame or support structure, in accordance with an embodiment;

[023] Figure 6B is a flattened plane view of the support structure covered in a polymer coating, in accordance with an embodiment;

[024] Figures 7A, 7B and 7C are scanning electron micrograph images of expanded fluoropolymer membranes used to form the valve leaflets, in accordance with an embodiment;

[025] Figure 8 is a perspective view of a valve assembly, in accordance with an embodiment;

[026] Figures 9A and 9B are top elevational views of the heart valve assembly of Figure 8 shown illustratively in closed and open positions, respectively, in accordance with an embodiment;

[027] Figure 10 is a graph of measured outputs from a heart flow pulse duplicator system used for measuring performance of the valve assemblies;

[028] Figures 11A and 11B are a graph and data chart of measured outputs from a high rate fatigue tester used for measuring performance of the valve assemblies;

[029] Figures 12A and 12B are graphs of measured outputs from the heart flow pulse duplicator system taken while testing valve assemblies according to and embodiment at zero cycles and after about 207 million cycles, respectively;

[030] Figures 13A and 13B are graphs of measured outputs from the heart flow pulse duplicator system taken while testing valve assemblies in accordance with embodiments at about 79 million cycles and after about 198 million cycles, respectively;

[031] Figure 14 is a perspective view of a mandrel for manufacturing a heart valve assembly, in accordance with an embodiment;

[032] Figure 15 is a perspective view of a valve frame for a heart valve, in accordance with an embodiment;

[033] Figure 16 is a perspective view of the valve frame of Figure 15 nested together with the mandrel Figure 14, in accordance with an embodiment;

[034] Figure 17 is a perspective view of a molded valve, in accordance with an embodiment;

[035] Figure 18 is a perspective view of a molded valve, showing an attachment member for reinforcing a bond between adjacent valve leaflets and a post of a valve frame, in accordance with an embodiment;

[036] Figure 19 is a perspective view of a valve frame, in accordance with an embodiment;

[037] Figure 20 is a perspective view of the valve frame of Figure 19 with posts that are cushion-wrapped, in accordance with an embodiment;

[038] Figure 21 is a perspective view of a stereolithography-formed mandrel, in accordance with an embodiment;

[039] Figure 22 is a perspective view of the cushion-wrapped valve frame of Figure 20 mounted onto the mandrel of Figure 21, in accordance with an embodiment;

[040] Figure 23 is a perspective view of a valve having valve leaflets coupled to and supported on the cushion-wrapped valve frame of Figure 20, in accordance with an embodiment

[041] Figure 24 is a perspective view of a non-collapsible stent frame or support structure, in accordance with an embodiment;

[042] Figure 25 is a perspective view of a laminated stent frame, in accordance with an embodiment;

[043] Figure 26A is a perspective view of the tri-leaflet assembly, base tool, stent frame encapsulated within a composite strain relief and sewing ring, in accordance with an embodiment;

[044] Figure 26B is a perspective view of a tri-leaflet assembly, in accordance with an embodiment;

[045] Figure 27 is a perspective view of a valve, in accordance with an embodiment;

[046] Figure 28 is a perspective view of a valve and fixture, in accordance with an embodiment;

[047] Figure 29 is a perspective view of a valve, fixture, and press, in accordance with an embodiment;

[048] Figure 30 is a perspective view of a completed valve, in accordance with an embodiment;

[049] Figure 31 is a perspective view of a non-collapsible stent frame or support structure of Figure 24 with a cushion member covering a perimeter of the structure, in accordance with an embodiment;

[050] Figure 32 is a perspective view of a completed valve having leaflets coupled to and supported on a frame or support structure with a cushion member covering a perimeter of the support structure, a strain relief, and a sewing flange, in accordance with an embodiment;

[051] Figure 33A is a perspective view of a collapsible stent frame or support structure of Figure 6A with a cushion member covering the regions of the structure to which leaflets are attached, in accordance with an embodiment;

[052] Figure 33B is a flattened plane view of the support structure of Figure 6A with a polymer coating encapsulating the cushion members, in accordance with an embodiment;

[053] Figure 34 is a perspective view of the collapsible stent frame and cushion members of Figures 33A and 33B with leaflet material wrapped as cylinder over the exterior of the frame with three axial slits, in accordance with an embodiment;

[054] Figure 35 is a perspective view of Figure 34 with three tabs of leaflet material internalized to stent frame through individual openings, in accordance with an embodiment;

[055] Figure 36 is a perspective view of a completed valve having leaflets coupled to and supported on a collapsible frame with a cushion member at leaflet attachment sites of structure and a strain relief, in accordance with an embodiment;

[056] Figure 37 is a graph of leaflet thickness and numbers of layers for a single composite material, in accordance with embodiments;

[057] Figure 38 is a graph comparing the leaflet thickness and numbers of layers for two different composite materials, in accordance with embodiments;

[058] Figure 39 is a sample graph of leaflet thickness and number of layers with boundaries defined for hydrodynamic performance, minimum number of layers, minimum strength, maximum composite thickness, and maximum percentage of fluoropolymer, in accordance with embodiments;

[059] Figure 40 is a graph of leaflet thickness and number of layers with boundaries defined for hydrodynamic performance, minimum number of layers, minimum strength, maximum composite thickness, and maximum percentage of fluoropolymer for the leaflet configurations of Examples 1, 2, 3, A, B, 4A, 4B, 4C, 5, 6, 7, & 8, in accordance with embodiments;

[060] Figure 41A is a graph of leaflet thickness and number of layers depicting general trends of improved durability observed during accelerated wear testing;

[061] Figure 41B is a graph of leaflet thickness and number of layers depicting general trends of reduced durability observed during accelerated wear testing;

[062] Figure 42 is a graph of hydrodynamic performance data (EOA and regurgitant fraction) comparing two valves, in accordance with embodiments;

[063] Figure 43 is Table 4, which is a table of performance data for example valves, in accordance with embodiments; and

[064] Figure 44 is Table 6, which is a table of performance data for example valves, in accordance with embodiments.

DETAILED DESCRIPTION OF THE ILLUSTRATED EMBODIMENTS

[065] Definitions for some terms used herein are provided below in the Appendix.

[066] The embodiments presented herein address a long-felt need for a material that meets the durability and biocompatibility requirements of high-cycle flexural implant applications, such as heart valve leaflets. It has been observed that heart valve leaflets formed from porous fluoropolymer materials or, more particularly, from ePTFE containing no elastomer suffer from stiffening in high-cycle flex testing and animal implantation.

[067] In one embodiment, described in greater detail below, the flexural durability of porous fluoropolymer heart valve leaflets was significantly increased by adding a relatively high-percentage of relatively lower strength elastomer to the pores. Optionally, additional layers of the elastomer may be added between the composite layers. Surprisingly, in embodiments wherein porous fluoropolymer membranes are imbibed with elastomer the presence of the elastomer increased overall thickness of the leaflet, the resulting increased thickness of the fluoropolymer members due to the addition of the elastomer did not hinder or diminish flexural durability. Further, after reaching a minimum percent by weight of elastomer, it was found that fluoropolymer members in general performed better with increasing percentages of elastomer resulting in significantly increased cycle lives exceeding 40 million cycles in vitro, as well as by showing no signs of calcification under certain controlled laboratory conditions.

[068] A material according to one embodiment includes a composite material comprising an expanded fluoropolymer membrane and an elastomeric material. It should be readily appreciated that multiple types of fluoropolymer membranes and multiple types of elastomeric materials can be combined while within the spirit of the present embodiments. It should also be readily appreciated that the elastomeric material can include multiple elastomers, multiple types of non-elastomeric components, such as inorganic fillers, therapeutic agents, radiopaque markers, and the like while within the spirit of the present embodiments.

[069] In one embodiment, the composite material includes an expanded fluoropolymer material made from porous ePTFE membrane, for instance as generally described in U.S. Patent No. 7,306,729.

[070] The expandable fluoropolymer, used to form the expanded fluoropolymer material described, may comprise PTFE homopolymer. In alternative embodiments, blends of PTFE, expandable modified PTFE and/or expanded copolymers of PTFE may be used. Non-limiting examples of suitable fluoropolymer materials are described in, for example, U.S. Patent No. 5,708,044, to Branca, U.S. Patent No. 6,541,589, to Baillie, U.S. Patent No. 7,531,611, to Šabol et al., U.S. Patent Application No. 11/906,877, to Ford, and U.S. Patent Application No. 12/410,050, to Xu et al.

[071] The expanded fluoropolymer of the present embodiments may comprise any suitable microstructure for achieving the desired leaflet performance. In one embodiment, the expanded fluoropolymer may comprise a microstructure of nodes interconnected by fibrils, such as described in U.S. Patent No. 3,953,566 to Gore. In one embodiment, the microstructure of an expanded fluoropolymer membrane comprises nodes interconnected by fibrils as shown in the scanning electron micrograph image in Figure 7A. The fibrils extend from the nodes in a plurality of directions, and the membrane has a generally homogeneous structure. Membranes having this microstructure may typically exhibit a ratio of matrix tensile strength in two orthogonal directions of less than 2, and possibly less than 1.5.

[072] In another embodiment, the expanded fluoropolymer may have a microstructure of substantially only fibrils, such as, for example, depicted in Figure 7B and 7C, as is generally taught by U.S. Patent No. 7,306,729, to Bacino. Figure 7C is a higher magnification of the expanded fluoropolymer membrane shown in

Figure 7B, and more clearly shows the homogeneous microstructure having substantially only fibrils. The expanded fluoropolymer membrane having substantially only fibrils as depicted in Figures 7B and 7C, may possess a high surface area, such as greater than $20\text{m}^2/\text{g}$, or greater than $25\text{m}^2/\text{g}$, and in some embodiments may provide a highly balanced strength material having a product of matrix tensile strengths in two orthogonal directions of at least $1.5 \times 10^5 \text{ MPa}^2$, and/or a ratio of matrix tensile strengths in two orthogonal directions of less than 2, and possibly less than 1.5.

[073] The expanded fluoropolymer of the present embodiments may be tailored to have any suitable thickness and mass to achieve the desired leaflet performance. In some cases, it may be desirable to use a very thin expanded fluoropolymer membrane having a thickness less than $1.0 \mu\text{m}$. In other embodiments, it may be desirable to use an expanded fluoropolymer membrane having a thickness greater than $0.1 \mu\text{m}$ and less than $20 \mu\text{m}$. The expanded fluoropolymer membranes can possess a specific mass less than about $1\text{g}/\text{m}^2$ to greater than about $50\text{g}/\text{m}^2$.

[074] Membranes according to embodiments can have matrix tensile strengths ranging from about 50 MPa to about 400 MPa or greater, based on a density of about $2.2 \text{ g}/\text{cm}^3$ for PTFE.

[075] Additional materials may be incorporated into the pores or within the material of the membranes or in between the layers of the membranes to enhance desired properties of the leaflet. Composites according to one embodiment can include fluoropolymer membranes having thicknesses ranging from about $500 \mu\text{m}$ to less than $0.3 \mu\text{m}$.

[076] The expanded fluoropolymer membrane combined with elastomer provides the elements of the present embodiments with the performance attributes required for use in high-cycle flexural implant applications, such as heart valve leaflets, in at least several significant ways. For example, the addition of the elastomer improves the fatigue performance of the leaflet by eliminating or reducing the stiffening observed with ePTFE-only materials. In addition, it reduces the likelihood that the material will undergo permanent set deformation, such as wrinkling or creasing, that could result in compromised performance. In one embodiment, the elastomer occupies substantially all of the pore volume or space

within the porous structure of the expanded fluoropolymer membrane. In another embodiment the elastomer is present in substantially all of the pores of the at least one fluoropolymer layer. Having elastomer substantially filling the pore volume or present in substantially all of the pores reduces the space in which foreign materials can be undesirably incorporated into the composite. An example of such foreign material is calcium. If calcium becomes incorporated into the composite material, as used in a heart valve leaflet, for example, mechanical damage can occur during cycling, thus leading to the formation of holes in the leaflet and degradation in hemodynamics.

[077] In one embodiment, the elastomer that is combined with the ePTFE is a thermoplastic copolymer of tetrafluoroethylene (TFE) and perfluoromethyl vinyl ether (PMVE), such as described in U.S. Patent No. 7,462,675. As discussed above, the elastomer is combined with the expanded fluoropolymer membrane such that the elastomer occupies substantially all of the void space or pores within the expanded fluoropolymer membrane. This filling of the pores of the expanded fluoropolymer membrane with elastomer can be performed by a variety of methods. In one embodiment, a method of filling the pores of the expanded fluoropolymer membrane includes the steps of dissolving the elastomer in a solvent suitable to create a solution with a viscosity and surface tension that is appropriate to partially or fully flow into the pores of the expanded fluoropolymer membrane and allow the solvent to evaporate, leaving the filler behind.

[078] In another embodiment, a method of filling the pores of the expanded fluoropolymer membrane includes the steps of delivering the filler via a dispersion to partially or fully fill the pores of the expanded fluoropolymer membrane;

[079] In another embodiment, a method of filling the pores of the expanded fluoropolymer membrane includes the steps of bringing the porous expanded fluoropolymer membrane into contact with a sheet of the elastomer under conditions of heat and/or pressure that allow elastomer to flow into the pores of the expanded fluoropolymer membrane.

[080] In another embodiment, a method of filling the pores of the expanded fluoropolymer membrane includes the steps of polymerizing the elastomer within the pores of the expanded fluoropolymer membrane by first filling the pores with a prepolymer of the elastomer and then at least partially curing the elastomer.

[081] After reaching a minimum percent by weight of elastomer, the leaflets constructed from fluoropolymer materials or ePTFE generally performed better with increasing percentages of elastomer resulting in significantly increased cycle lives. In one embodiment, the elastomer combined with the ePTFE is a thermoplastic copolymer of tetrafluoroethylene and perfluoromethyl vinyl ether, such as described in U.S. Patent No. 7,462,675, and other references that would be known to those of skill in the art. For instance, in another embodiment shown in Example 1, a leaflet was formed from a composite of 53% by weight of elastomer to ePTFE and was subjected to cycle testing. Some stiffening was observed by around 200 million test cycles, though with only modest effect on hydrodynamics. When the weight percent of elastomer was raised to about 83% by weight, as in the embodiment of Example 2, no stiffening or negative changes in hydrodynamics were observed at about 200 million cycles. In contrast, with non-composite leaflets, i.e. all ePTFE with no elastomer, as in the Comparative Example B, severe stiffening was apparent by 40 million test cycles. As demonstrated by these examples, the durability of porous fluoropolymer members can be significantly increased by adding a relatively high-percentage of relatively lower strength elastomer to the pores of the fluoropolymer members. The high material strength of the fluoropolymer membranes also permits specific configurations to be very thin.

[082] Other biocompatible polymers which may be suitable for use in embodiments may include but not be limited to the groups of urethanes, silicones(organopolysiloxanes), copolymers of silicon-urethane, styrene/isobutylene copolymers, polyisobutylene, polyethylene-co-poly(vinyl acetate), polyester copolymers, nylon copolymers, fluorinated hydrocarbon polymers and copolymers or mixtures of each of the foregoing.

[083] Leaflets constructed from a composite material comprising less than about 55% fluoropolymer by weight can be assembled in a variety of configurations based on desired laminate or leaflet thickness and number of layers of composite. The thickness of the composite is directly related to the percentage of fluoropolymer by weight and membrane thickness. Using a range of membrane thickness from about 300 nm to more than 3,556 nm and a range of percentage of fluoropolymer by weight from 10 to 55, for example, allowed the formation of composite thicknesses ranging from 0.32 μm to more than 13 μm .

[084] The relationship between the leaflet thickness and number of composite layers is shown illustratively in a graph in Figure 37, wherein two leaflet configurations, indicated as A and B, are shown. In one embodiment, these configurations A and B may be constructed from a single composite. In another embodiment, there may be a generally linear relationship between leaflet thickness and number of layers, wherein $Y = mX$; in which Y = leaflet thickness, m = slope, and X = number of layers. The slope (m) or ratio of leaflet thickness to number of layers is equal to the composite thickness. Therefore, doubling the number of layers from 20 to 40 for configurations A and B, for example, has the result of doubling the thickness from 40 μm to 80 μm . It should be appreciated that the slope of the line or even the shape of the graph of leaflet thickness versus number of composite layers can vary depending on the amount of elastomer between the layers and the uniformity of the layers.

[085] When the percentage of fluoropolymer by weight for the same membrane is reduced, the thickness of the composite is increased. As shown in Figure 38, this increase in composite thickness is indicated by the increased slope of the dotted line relative to the solid line from the previous embodiment. In the embodiment illustrated by the dotted line, a reduction of the percentage of fluoropolymer by weight for the same membrane by about half results in about an increase in thickness of the composite by about two, which is reflected in the increased slope of the dotted line. Therefore, a leaflet as depicted by configuration C in Figure 38 can either have the same number of layers as configuration A or the same leaflet thickness as configuration B by varying the percentage of fluoropolymer by weight.

[086] In determining what configurations of percent fluoropolymer by weight, composite thickness, and number of layers influenced both hydrodynamic as well as durability performance, boundaries were observed, as best shown by the graph in Figure 39. There are five boundaries that generally define suitable leaflet configurations that have been observed thus far. The first boundary is defined by acceptable hydrodynamic performance set forth by ISO guidance document for cardiovascular implants (5840:2005) defining limits of EOA and regurgitant fraction for a given valve size. Typically, leaflets with a thickness greater than 100 μm formed from these composites perform near these limits of acceptability. The

second boundary is a minimum number of layers (10) as observed by durability failures further illustrated by the examples provided. Similarly, the third boundary is a maximum ratio of leaflet thickness to number of layers or composite thickness of 5 μm . Generally, low layer numbers built from thick composites performed poorly when compared to high layer numbers of either the same percent fluoropolymer by weight and leaflet thickness. The fourth boundary is defined by the minimum number of layers of a given composite which is determined by the strength required to resist fluoropolymer creep during hydrodynamic loading of the leaflet when the valve is closed during the cardiac cycle. The strength of the laminate is measured by a dome burst test, where typically a burst pressure of least 207 KPa is required to ensure the leaflets maintain their shape and function. The fifth boundary is defined by the maximum percent fluoropolymer by weight (55%) required to significantly increase cyclic durability. In Figure 40, a graph illustrating these boundaries is shown with the leaflet configurations of all the examples provided to further illustrate these discoveries.

[087] The maximum number of layers of a given composite may be determined by the desired leaflet thickness. It has been observed that as leaflet thickness increases, the hydrodynamic performance behavior for a given valve geometry decreases while the bending character improves. "Hydrodynamic performance" generally refers to the combination of EOA and regurgitant fraction plotted on a Cartesian coordinate system in two dimensions for a given valve size as depicted in Figure 42. "Bending character" generally refers to the qualitative amount of wrinkles and/or creases developed with in the leaflet structure during deformations induced by cyclic opening and closing. Conversely, as leaflet thickness is decreased, the hydrodynamic performance behavior for a given geometry increases while the bending character is reduced. This observation of differences in bending character as a function of leaflet thickness is further illustrated with examples of two valves with 13 μm and 130 μm leaflet thicknesses, referred to as valve 42A and valve 42B, respectively. A graph of hydrodynamic performance data (EOA and regurgitant fraction) comparing these two valves is shown in Figure 42 where minimizing the regurgitant fraction and maximizing the EOA is desirable.

[088] It has been observed that thin film materials exposed to large cyclic deformations over long durations are generally susceptible to wrinkles and creases.

It is also generally known by those skilled in the art that durability of thin materials exposed to large cyclic deformations over long durations is reduced as a result of such wrinkles and creases that can be formed during the duty cycle.

[089] Therefore, it was surprising when leaflets of similar thickness (about 16 μm) which were constructed from ultra thin composites (0.32 μm) and had five times the number of layers (about 50) versus conventional leaflets had the desirable bending behavior only previously achieved by leaflets having thicknesses of 75 μm or greater. Additionally, when comparing durability of low number of layers of composites to high number of layers, the high number of layers typically out-perform the low number of layers constructs by orders of magnitude using number of duty cycles as a comparison. A valve with fifty layers and 16 μm thick leaflets was shown to have significantly fewer wrinkles and creases than a six layer construction of the approximately the same thickness.

[090] Comparing leaflets of about the same thickness in cross section with 4, 9, 26, 50, & 21 layers respectively, it was appreciated that the increase in the number of layers facilitates both the ability of the laminate to take a smaller bend radius as well as accommodate a tight curvature by storing length of individual layers through localized buckling.

[091] General trends that have been observed by varying the thickness and number of layers are illustrated in the graphs in Figures 41A and 41B and are further supported by the examples provided.

[092] The following non-limiting examples are provided to further illustrate embodiments. It should also be readily appreciated that other valve frame designs may be used other than those illustrated in the examples below and accompanying figures.

[093] **Example 1**

[094] Heart valve leaflets according to one embodiment were formed from a composite material having an expanded fluoropolymer membrane and an elastomeric material and joined to a metallic balloon expandable stent using an intermediate layer of FEP, as described by the following process:

[095] 1) A thick, sacrificial tooling cushion pad or layer was formed by folding a ePTFE layer over upon itself to create a total of four layers. The ePTFE layer was about 5 cm (2") wide, about 0.5mm (0.02") thick and had a high degree of

compressibility, forming a cushion pad. Referring to Figures 1 and 2, the cushion pad 200 was then stretched (Figure 2) onto a leaflet tool, generally indicated at 100. The leaflet tool 100 has a leaflet portion 102, a body portion 104 and a bottom end 106. The leaflet portion 102 of the leaflet tool 100 has a generally arcuate, convex end surface 103. The cushion pad 200 was stretched and smoothed over the end surface 103 of the leaflet portion 102 of the leaflet tool 100 by forcing the leaflet tool 100 in the direction depicted by the arrow (Figure 2A). A peripheral edge 202 of the cushion pad 200 was stretched over the bottom end 106 of the leaflet tool 100 and twisted to hold the cushion pad 200 in place (Figure 2B).

[096] 2) Referring to Figure 2B, a release layer 204 was then stretched over the leaflet portion 102 of the leaflet tool 100 which in the previous step was covered with the cushion pad 200. In one embodiment, the release layer 204 was made from a substantially nonporous ePTFE having a layer of fluorinated ethylene propylene (FEP) disposed along an outer surface or side thereof. The release layer 204 was stretched over the leaflet tool 100 such that the FEP layer faced toward the cushion pad 200 and the substantially nonporous ePTFE faced outwardly or away from the cushion pad 200. The release layer was about 25 μm thick and of sufficient length and width to allow the release layer 204 to be pulled over the bottom end 106 of the leaflet tool 100. As with the cushion pad 200 in the previous step, a peripheral edge 206 of the release layer 204 was pulled toward the bottom end 106 of the leaflet tool 100 and then twisted onto the bottom end 106 of the leaflet tool 100 to retain or hold the release layer 204 in place. The FEP layer of the release layer 204 was then spot-melted and thereby fixedly secured to the cushion pad 200, as required, by the use of a hot soldering iron.

[097] 3) The processes of Steps 1) and 2) were repeated to prepare three separate leaflet tools, each having a cushion pad covered by a release layer.

[098] 4) A leaflet material according to one embodiment was formed from a composite material comprising a membrane of ePTFE imbibed with a fluoroelastomer. A piece of the composite material approximately 10 cm wide was wrapped onto a circular mandrel to form a tube. The composite material was comprised of three layers: two outer layers of ePTFE and an inner layer of a fluoroelastomer disposed therebetween. The ePTFE membrane was manufactured according to the general teachings described in U.S. Patent No. 7,306,729. The

fluoroelastomer was formulated according to the general teachings described in U.S. Patent No. 7,462,675. Additional fluoroelastomers may be suitable and are described in U.S. Publication No. 2004/0024448.

[0099] The ePTFE membrane had the following properties: thickness = about 15 μm ; MTS in the highest strength direction = about 400 MPa; MTS strength in the orthogonal direction = about 250 MPa; Density = about 0.34 g/cm^3 ; IBP = about 660 KPa.

[0100] The copolymer consists essentially of between about 65 and 70 weight percent perfluoromethyl vinyl ether and complementally about 35 and 30 weight percent tetrafluoroethylene.

[0101] The percent weight of the fluoroelastomer relative to the ePTFE was about 53%.

[0102] The multi-layered composite had the following properties: thickness of about 40 μm ; density of about 1.2 g/cm^3 ; force to break/width in the highest strength direction = about 0.953 kg/cm; tensile strength in the highest strength direction = about 23.5 MPa (3,400 psi); force to break/width in the orthogonal direction = about 0.87 kg/cm; tensile strength in the orthogonal direction = about 21.4 MPa (3100 psi), IPA bubble point greater than about 12.3 MPa, Gurley Number greater than about 1,800 seconds, and mass/area = about 14 g/m^2 .

[0103] The following test methods were used to characterize the ePTFE layers and the multi-layered composite.

[0104] The thickness was measured with a Mutitoyo Snap Gage Absolute, 12.7 mm (0.50") diameter foot, Model ID-C112E, Serial # 10299, made in Japan. The density was determined by a weight/volume calculation using an Analytical Balance Mettler PM400 New Jersey, USA. The force to break and tensile strengths were measured using an Instron Model #5500R Norwood, MA, load cell 50 kg, gage length = 25.4 cm, crosshead speed = 25 mm/minute (strain rate = 100% per minute) with flat faced jaws. The IPA Bubble Point was measured by an IPA bubble point tester, Pressure Regulator Industrial Data Systems Model LG-APOK, Salt Lake City, UT, USA, with a Ramp Rate of 1.38 KPa/s (0.2 psi/s), 3.14 cm^2 test area. The Gurley Number was determined as the time in seconds for 100 cm^3 of air to flow through a 6.45 cm^2 sample at 124 mm of water pressure using a Gurley Tester, Model #4110, Troy, NY, USA.

[0105] Unless otherwise noted, these test methods were used to generate the data in subsequent examples.

[0106] Layers of the composite material, each having two outer layers of ePTFE and an inner layer of a fluoroelastomer disposed therebetween, was wrapped onto a mandrel having a diameter of about 28 mm (1.1") such that the higher strength direction of the membrane was oriented in the axial direction of the mandrel. In one embodiment, four layers of the composite material were wrapped in a non-helical, generally circumferential fashion onto the mandrel. The composite material had a slight degree of tackiness that allowed the material to adhere to itself. While still on the mandrel, the composite material was slit longitudinally generally along the mandrel long axis to form a sheet about 10 cm (4") by about 90 mm (3.5").

[0107] 5) The resulting sheet of leaflet material (or composite material from Step 4) was then cut and wrapped onto the leaflet tool 100 having a cushion pad 200 covered by a release layer 204. More specifically, as shown in Figures 3A – 3C, the leaflet material 300 was placed onto a flat cutting surface. The leaflet tool 100 with the cushion pad 200 and release layer 204 was then aligned onto the leaflet material 300 approximately as shown. Four slits 302, 304, 306, 308 were then formed in the leaflet material 300 with a razor blade. One pair of slits 302, 304 extends from one side of the leaflet tool 100 and terminates at one edge 300a of the leaflet material 300, and the other pair of slits 306, 308 extends from an opposite side of the leaflet tool 100 and terminates at an opposite edge 300b of the leaflet material 300. The slits 302, 304, 306, 308 were spaced apart from the leaflet portion 102 of the leaflet tool 100. The slits 302, 304, 306, 308 did not protrude under the leaflet tool 100. It should be appreciated that the widths of the individual slits are shown not to scale. The slits 302, 304, 306, 308 in the leaflet material 300 resulted in the formation of a folding portion 310, a pair of straps 312, 314 and excess material of leaflet material 315. The folding portions 310 were then folded in the general direction indicated by the arrows 316 in Figure 3 and smoothed over the leaflet tool 100, which was covered by the cushion pad 200 and the release layer 204 in the previous steps.

[0108] 6) The leaflet material 315 was then stretched and smoothed over the leaflet portion 102, particularly the end surface 103 of the leaflet tool 100. The Steps 4) and 5) were repeated to form three separate leaflet assemblies. The three leaflet assemblies 402, 404, 406 were then clamped together to form a tri-leaflet assembly

400, as shown in Figure 4. Shown are the three separate leaflet assemblies 402, 404, 406, each having an excess material of leaflet material 315 extending generally radially beyond the periphery of the tri-leaflet assembly 400.

[0109] 7) A base tool was then provided having cavities for engaging the end surfaces of the leaflet tools of the tri-leaflet assembly and trimming the excess leaflet area to form three leaflets. Referring to Figure 5A, the base tool is generally indicated at 500 and extends longitudinally between an end 501 and an opposite bottom end 503. Three concave cavities 502, 504, 506 are formed in the end 501 of the base tool 500. Each concave cavity 502, 504, 506 is formed to match fit or nestingly seat the end surface 103 of one of the three leaflet assemblies 402, 404, 406. Three radially extending elements 508, 510, 512 extend outwardly from the end of the base tool 500. Each element 508, 510, 512 is disposed between an adjacent pair of concave cavities 502, 504, 506.

[0110] The base tool 500 was then prepared having a compression pad and a release layer (not shown) similar to how the leaflet tool was prepared in Steps 1 and 2. As described for each leaflet tool in Steps 1 and 2, the compression pad and the release layer were similarly stretched and affixed to the base tool 500 to form a base tool assembly.

[0111] 8) Referring to Figure 5B, the base tool assembly (illustrated for convenience as the base tool 500 without showing the cushion pad and the release layer) and the tri-leaflet assembly, generally indicated at 400, were then generally axially aligned together so that the end surface (not shown) of each leaflet tool 100 was seated into one of the concave cavities (not shown) in the end 501 of the base tool, generally indicated at 500, to form a combined tool assembly.

[0112] 9) A metallic balloon expandable stent was then fabricated. A tube of 316 stainless steel having a wall thickness of about 0.5mm (0.020") and a diameter of about 2.5cm (1.0") was laser cut. A pattern was cut into the tube to form an annular-shaped cut stent frame or support structure, which is generally indicated at 600 and shown illustratively in a flat, plane view in Figure 6a. The support structure 600, includes a plurality of small closed cells 602, a plurality of large closed cells 604, and a plurality of leaflet closed cells 606. Note that one of the plurality of leaflet closed cells 606 appears as an open cell in Figure 6A due to the flat plane view. The

cells 602, 604, 606 are generally arranged along rows forming the annular shape of the support structure 600.

[0113] 10) Polymeric materials were then adhered to the laser cut stent frame. First, a sacrificial compression layer of ePTFE membrane was wrapped without overlap onto a mandrel (not shown) having a diameter of about 2.5 cm (1.0"). The sacrificial compression layer of ePTFE membrane had a thickness of about 0.5 mm (0.02") and a width of about 10 cm (4"), and was compliant and compressible to provide a soft, sacrificial compression layer.

[0114] 11) Four layers of a substantially nonporous, ePTFE film were then wrapped onto the mandrel on top of the compression layer membrane. The substantially nonporous, ePTFE film had a thickness of about 25 μm (0.001"), was about 10 cm (4") wide and had a layer of FEP on one side. The substantially nonporous, ePTFE film was wrapped with the FEP facing away from the mandrel. The substantially nonporous, ePTFE film had the properties of the release layer previously described in Step 2).

[0115] 12) A thin film of type 1 (ASTM D3368) FEP was constructed using melt extrusion and stretching. An additional 10 layers of this type 1 (ASTM D3368) FEP film was added to the mandrel, which was previously wrapped in the compression layer membrane in Step 10 and the four layers of substantially nonporous, ePTFE film in Step 11. The type 1 (ASTM D3368) FEP film was about 40 μm (0.0016") thick and was about 7.7 cm (3") wide.

[0116] 13) The wrapped mandrel was then heat treated in an air convection oven at about 320 °C for about 5 minutes and allowed to cool.

[0117] 14) The support structure (indicated at 600 in Figure 6A) was then placed onto the heat treated and wrapped mandrel. Two additional layers of type 1 (ASTM D3368) FEP film (provided in Step 12) were then wrapped onto the support structure, which was previously placed on the wrapped mandrel.

[0118] 15) The wrapped mandrel and the support structure supported thereon were then heat treated in an air convection oven at about 320 °C for about 10 minutes and allowed to cool, forming a polymeric-coated support structure.

[0119] 16) The polymeric-coated support structure was then trimmed with a scalpel to form a trimmed stent frame, which is generally indicated at 700 and shown illustratively in a flat, plane view in Figure 6B. More specifically, in one manner, the

polymeric coating was trimmed about 2 mm (0.08") past the edges of the support structure (600, Figure 6A) to form a variety of edge profiles 708. In another manner, the polymeric coating was allowed to span entire cells to form a web in each cell. In either case, the support structure 600 was fully encapsulated within a polymeric coating 702 to form the trimmed stent frame 700. The trimmed stent frame 700 includes a plurality of leaflet openings 704 corresponding in number and generally in shape to the plurality of leaflet closed cells 606 (Figure 6A). Further, a slit 706 is formed in the polymeric coating 702 of each of the small closed cells as shown in Figure 6B. Specifically, each slit 706 is linear and generally parallel to a longitudinal center axis (not shown) of the annular-shaped support structure 600.

[0120] 17) The trimmed stent frame was then placed onto the combined tool assembly from Step 8. The leaflet portions (102) of the leaflet tools were aligned to the leaflet openings (704 in Figure 6B) in the trimmed stent frame. The three excess leaflet material areas (315 in Figure 4) were pulled through the leaflet openings of the stent frame. Each of the three pairs of straps (312, 314 in Figure 3A) was pulled through one of the slits (706 in Figure 6B) and wrapped around the trimmed stent frame. Each pair of straps were wrapped in opposing directions relative to each other. The six straps were then heat tacked to the trimmed stent frame using a hot soldering iron.

[0121] 18) The combined tool assembly (Step 8) and the trimmed stent frame having the wrapped and heat tacked straps were then mounted into a rotary chuck mechanism. The rotary chuck mechanism was then adjusted to apply a light, longitudinal compressive load. The excess leaflet material areas (315 in Figure 4) were then heat tacked to the base tool (500 in Figure 5) using a hot soldering iron.

[0122] 19) The combined tools of Step 18 were then wrapped with an additional 2 layers of type 1 (ASTM D3368) FEP film (from Step 12). Three additional layers of the composite (Step 4) were then overwrapped and tacked down to the trimmed stent frame.

[0123] 20) In preparation for a final heat treat, release and sacrificial layers of a compression tape and compression fiber were applied both circumferentially and longitudinally to the assembly from Step 19. The compression tape/fiber contact and compress the assembly both circumferentially and longitudinally during the subsequent heat treat. A sacrificial layer of compression tape was circumferentially

wrapped in a helical fashion onto the assembly from Step 19. This compression tape had the properties of the sacrificial compression layer of ePTFE previously described in Step 10. An ePTFE compression fiber was then tightly wrapped onto the compression tape. Approximately 100 turns of the compression fiber were circumferentially applied in a closely spaced helical pattern. The ePTFE compression fiber was about 1 mm (0.04") in diameter and was structured to shrink longitudinally when sufficiently heated. The clamped assembly was then removed from the rotary chuck mechanism. Three layers of sacrificial compression tape were then wrapped in a longitudinal fashion around the assembly. Approximately 20 wraps of the compression fiber was then longitudinally wrapped over the longitudinal compression tape.

[0124] 21 The assembly from Step 20 was then heat treated in an air convection oven at about 280°C for about 90 minutes and then room temperature water quenched. This heat treatment step facilitates the flow of the thermoplastic fluoroelastomer into the pores of the ePTFE membrane used to create the leaflet material described in step 4.

[0125] 22) The sacrificial compression tapes/fibers were then removed. The polymeric materials were trimmed to allow the leaflet and base tools to be separated. The stent polymeric layers were then trimmed to allow removal of the stent frame with the attached leaflets. The leaflets were then trimmed, resulting in a valve assembly as shown in Figure 8 and generally indicated at 800.

[0126] The resulting valve assembly 800, according to one embodiment, includes leaflets 802 formed from a composite material with at least one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the at least one fluoropolymer layer. Each leaflet 802 is movable between a closed position, shown illustratively in Figure 9A, in which blood is prevented from flowing through the valve assembly, and an open position, shown illustratively in Figure 9B, in which blood is allowed to flow through the valve assembly. Thus, the leaflets 802 of the valve assembly 800 cycle between the closed and open positions generally to regulate blood flow direction in a human patient,

[0127] The performance of the valve leaflets in each valve assembly was characterized on a real-time pulse duplicator that measured typical anatomical

pressures and flows across the valve, generating an initial or “zero fatigue” set of data for that particular valve assembly. The valve assembly was then transferred to a high-rate fatigue tester and was subjected to approximately 207 million cycles. After each block of about 100 million cycles, the valve was then returned to the real-time pulse duplicator and the performance parameters re-measured.

[0128] The flow performance was characterized by the following process:

[0129] 1) The valve assembly was potted into a silicone annular ring (support structure) to allow the valve assembly to be subsequently evaluated in a real-time pulse duplicator. The potting process was performed according to the recommendations of the pulse duplicator manufacturer (ViVitro Laboratories Inc., Victoria BC, Canada)

[0130] 2) The potted valve assembly was then placed into a real-time left heart flow pulse duplicator system. The flow pulse duplicator system included the following components supplied by VSI Vivitro Systems Inc., Victoria BC, Canada: a Super Pump, Servo Power Amplifier Part Number SPA 3891; a Super Pump Head, Part Number SPH 5891B, 38.320 cm² cylinder area; a valve station/fixture; a Wave Form Generator, TriPack Part Number TP 2001; a Sensor Interface, Part Number VB 2004; a Sensor Amplifier Component, Part Number AM 9991; and a Square Wave Electro Magnetic Flow Meter, Carolina Medical Electronics Inc., East Bend, NC, USA.

[0131] In general, the flow pulse duplicator system uses a fixed displacement, piston pump to produce a desired fluid flow through the valve under test.

[0132] 3) The heart flow pulse duplicator system was adjusted to produce the desired flow, mean pressure, and simulated pulse rate. The valve under test was then cycled for about 5 to 20 minutes.

[0133] 4) Pressure and flow data were measured and collected during the test period, including ventricular pressures, aortic pressures, flow rates, and pump piston position. Shown illustratively in Figure 10 is a graph of typical data outputs from the heart flow pulse duplicator system.

[0134] 5) Parameters used to characterize the valve and to compare to post-fatigue values are pressure drop across the open valve during the positive pressure portion of forward flow, effective orifice area, and regurgitant fraction.

[0135] Following characterization, the valve assembly was then removed from the flow pulse duplicator system and placed into a high-rate fatigue tester. A Six Position Heart Valve Durability Tester, Part Number M6 was supplied by Dynatek, Galena, MO, USA and was driven by a Dynatek Delta DC 7000 Controller. This high rate fatigue tester displaces fluid through a valve assembly with a typical cycle rate of about 780 cycles per minute. During the test, the valve assembly can be visually examined using a tuned strobe light. The pressure drop across the closed valve can also be monitored as displayed in Figures 11A and 11B. Shown in Figures 11A and 11B is a typical data set verifying that the high-rate fatigue tester was producing consistent pressure wave forms.

[0136] The valve assembly was continuously cycled and periodically monitored for visual and pressure drop changes. After approximately 200 million cycles, the valve assembly was removed from the high-rate tester and returned to the real-time pulse duplicator. The pressure and flow data were collected and compared to the original data collected.

[0137] Shown in Figure 12A is a screen shot displaying typical measured data outputs from the real-time heart flow pulse duplicator system. Shown are Ventricular Pressures, Aortic Pressures and Flow Rate. The initial or zero fatigue data for a particular valve is shown illustratively in Figure 12A. The same measurements were taken and data were collected for the same particular valve after 207 million cycles. The 207 million cycle data for the particular valve is shown illustratively in Figure 12B. Both sets of measurements were taken at 5 liters per minute flow rate and 70 cycles per minute rate. Comparing Figures 12A and 12B, it should be readily appreciated that the waveforms are substantially similar, indicating no substantial change in the valve leaflet performance after about 207 million cycles. Pressure drop, effective orifice area (EOA), and regurgitant fraction measured at zero and 207 million cycles are summarized in Table 1 below.

Table 1

Number of cycles (Million)	Pressure Drop (mm Hg)	EOA (cm ²)	Regurgitant Fraction (%)
0	5.7	2.78	12.7
207	7.7	2.38	9.6

[0138] Generally, it was observed that the valve leaflets constructed according to the embodiments described herein exhibited no physical or mechanical degradation, such as tears, holes, permanent set and the like, after 207 million cycles. As a result, there was also no observable change or degradation in the closed and open configurations of the valve leaflets even after 207 million cycles.

[0139] **Example 2**

[0140] A heart valve having polymeric leaflets joined to a rigid metallic frame was constructed according to the following process:

[0141] A mandrel 900 was machined from PTFE having a shape shown in Figure 14. The mandrel 900 has a first end 902 and an opposite second end 904, and extends longitudinally therebetween. The mandrel 900 has an outer surface 910 having three (two shown) generally arcuate, convex lobes 912, each generally for forming leaflets (not shown) of a finished valve assembly (not shown). The outer surface 910 also includes a frame seating area 920 for positioning a valve frame (930 in Figure 15) relative to the convex lobes 912 prior to formation of leaflets onto the valve frame.

[0142] As shown in Figure 15, a valve frame 930 was laser cut from a length of 316 stainless steel tube with an outside diameter of about 25.4mm and a wall thickness of about 0.5mm in the shape shown in Figure 15. In the embodiment shown, the valve frame 930 extends axially between a bottom end 932 and an opposite top end defined generally by a plurality of axially extending, generally spire shaped posts 934 corresponding to the number of leaflets in the intended finished valve assembly (not shown). In the specific embodiment shown, three posts 934 are formed in the valve frame 930.

[0143] Two layers of an about 4 μ m thick film of FEP (not shown) was wrapped around the valve frame 930 and baked in an oven for about 30 minutes at about 270°C and allowed to cool. The resulting covered valve frame (for clarity, shown uncovered and indicated at 930) was then slid onto the mandrel 900 so that the complementary features between the valve frame 930 and mandrel 900 are nested together, as shown in Figure 16.

[0144] A leaflet material was then prepared having a membrane layer of ePTFE imbibed with a fluoroelastomer. More specifically, the membrane layer of ePTFE was manufactured according to the general teachings described in U.S. Patent No. 7,306,729. The ePTFE membrane was tested in accordance with the methods described in the Appendix. The ePTFE membrane had a mass per area of about 0.57 g/m^2 , a porosity of about 90.4%, a thickness of about $2.5 \text{ }\mu\text{m}$, a bubble point of about 458 KPa, a matrix tensile strength of about 339 MPa in the longitudinal direction and about 257 MPa in the transverse direction. This membrane was imbibed with the same fluoroelastomer as described in Example 1. The fluoroelastomer was dissolved in Novec HFE7500, 3M, St Paul, MN, USA in an about 2.5% concentration. The solution was coated using a mayer bar onto the ePTFE membrane (while being supported by a polypropylene release film) and dried in a convection oven set to about 145°C for about 30 seconds. After two coating steps, the resulting composite material of ePTFE/fluoroelastomer had a mass per area of about 3.6 g/m^2 .

[0145] The composite material (not shown) was then wound around the assembled mandrel 900 and valve frame 930. In one embodiment, a total of 20 layers of the ePTFE/fluoroelastomer composite was used. Any excess composite material that extended beyond the ends of mandrel 900 were twisted and pressed lightly against the ends 902, 904 of the mandrel 900.

[0146] The composite material wrapped mandrel was then mounted in a pressure vessel so that a vent port 906 (Figure 14) in the base or second end 904 of the mandrel 900 was plumbed to atmosphere. The vent port 906 extends from the second end 904 axially through the mandrel 900 and communicates to a generally orthogonally extending vent port 908 that extends through the outer surface 910 of the mandrel 900. The vent ports 906, 908, in addition to other vent ports which may be provided in the mandrel as needed (not shown), allow trapped air between the composite material and the mandrel to escape during the molding process.

[0147] About 690 KPa (100 psi) of nitrogen pressure was applied to the pressure vessel, forcing the ePTFE/fluoroelastomer composite against the mandrel 900 and the valve frame 930. Heat was applied to the pressure vessel until the temperature inside the vessel reached about 300°C , about 3 hours later. The heater was turned off and the pressure vessel was allowed to cool to room

temperature overnight. This process thermally bonded the layers of ePTFE/fluoroelastomer composite to each other and to the FEP coating on the valve frame 930. The pressure was released and the mandrel was removed from the pressure vessel.

[0148] The ePTFE/fluoroelastomer composite was trimmed circumferentially in two places: first, at the bottom end 932 of the valve frame 930, and second, near the top end of the valve frame 930 along a circle generally intersecting near the mid-point of each post 934. The resulting valve assembly 940 consisting of the valve frame 930 and the trimmed composite material was separated from and slid off the mandrel. The molded valve assembly 940, as shown in Figure 17, includes the valve frame 930 and a plurality of leaflets 950 formed from the trimmed composite material. In one embodiment, the valve assembly 940 included three leaflets. In another embodiment, each leaflet 950 in the valve assembly 940 was approximately 40 μm thick.

[0149] To help control the degree of opening of the valve, adjacent leaflets about each post were bonded together. As shown in Figure 18, the adjacent leaflets 950a, 950b were wrapped around the post 934 and bonded together to form a seam 954. The seam 954 had a depth 956 extending to at least about 2mm from the post 934. To support the bond between the adjacent leaflets 950a, 950b, an attachment member 952 was fixedly secured to inner surfaces of the adjacent leaflets 950a, 950b thereby bridging the seam 954 between the adjacent leaflets 950a, 950b. As shown in Figure 18, the attachment member 952 was generally rectangular. It should be appreciated, however, that other shapes for the attachment member may be utilized. The attachment member 952 was formed from the same type of composite material used to form the leaflets 950. The attachment member 952 was fixedly secured to the inner surfaces of the adjacent leaflets 950a, 950b using the fluoroelastomer solution previously described. These steps were repeated for the other pairs of adjacent leaflets of the valve assembly.

[0150] The performance and durability of the valve leaflets in this example were analyzed in the same manner as described in Example 1. The valve assembly was initially characterized on the same real-time pulse duplicator as described in Example 1 that measured typical anatomical pressures and flows across the valve, generating an initial or "zero fatigue" set of data for that particular valve assembly.

The valve was then subjected to accelerated testing as in Example 1. After about 79 million cycles, the valve was removed from the high rate fatigue tester and the hydrodynamic performance again characterized as in Example 1. The valve was removed finally at about 198 million cycles. Pressure drop, EOA and regurgitant fraction measured at about 79 million cycles and about 198 cycles are summarized in Table 2 below.

[0151] Figures 13A and 13B display similar results for a similar valve. Figure 13A is a graph of measured data output from the heart flow pulse duplicator system taken after about 79 million cycles. The same measurements were taken for the similar valve after about 198 million cycles, a graph of which is shown illustratively in Figure 13B. Both sets of measurements were taken at about 4 liters per minute flow rate and about 70 cycles per minute rate. Comparing Figures 13A and 13B, it should be again appreciated that the waveforms are significantly similar, indicating no substantial change in the valve leaflet performance after about 198 million cycles. Pressure drop, effective orifice area (EOA), and regurgitant fraction measured at 0, about 79, and about 198 million cycles are summarized in Table 2 below. These data indicate no substantial change in the valve leaflet performance after about 198 million cycles.

Table 2

Number of Cycles (Million)	Pressure Drop (mm Hg)	EOA (cm ²)	Regurgitant Fraction (%)
0	6.8	2.56	7.8
79	5.4	2.58	10.25
198	4.4	2.60	10.1

[0152] **Example 3**

[0153] A heart valve having polymeric leaflets joined to a rigid metallic frame was constructed according to the following process:

[0154] A valve support structure or frame 960 was laser cut from a length of 316 stainless steel tube with an outside diameter of about 25.4mm and a wall thickness of about 0.5mm in the shape shown in Figure 19. In the embodiment shown, the frame 960 extends axially between a bottom end 962 and an opposite top end defined generally by a plurality of axially extending, generally spire shaped

posts 964 corresponding to the number of leaflets in the intended finished valve assembly (not shown). A parabolically shaped top edge 968 extends between adjacent posts 964. In the specific embodiment shown, three posts 964 and three top edges 968 form the top end of the frame 960. The corners of the frame that would be in contact with the leaflet material were rounded using a rotary sander and hand polished. The frame was rinsed with water and then plasma cleaned using a PT2000P plasma treatment system, Tri-Star Technologies, El Segundo, CA, USA.

[0155] In one embodiment, a cushion member is provided between at least a portion of the frame and at least a portion of the leaflet to minimize stress related to direct contact between the frame and the leaflet. A composite fiber of ePTFE and silicone was created by first imbibing an ePTFE membrane with silicone MED-6215 (NuSil, Carpinteria, CA, USA), slitting it to a width of about 25 mm, and rolling into a substantially round fiber. The ePTFE used in this fiber was tested in accordance with the methods described in the Appendix. The ePTFE membrane had a bubble point of about 217 KPa, a thickness of about 10 μm , a mass per area of about 5.2 g/m^2 , a porosity of about 78%, a matrix tensile strength in one direction of about 96 MPa, and a matrix tensile strength of about 55 MPa in an orthogonal direction. The composite fiber 966 was wrapped around each of the posts 964 of the frame 960 as shown in Figure 20.

[0156] A mandrel 970 was formed using stereolithography in a shape shown in Figure 21. The mandrel 970 has a first end 972 and an opposite second end 974, and extends longitudinally therebetween. The mandrel 970 has an outer surface 980 having three (two shown) generally arcuate, convex lobes 982, each generally for forming leaflets (not shown) of a finished valve assembly (not shown). The outer surface 980 also includes a frame seating area 984 for positioning the frame (960 in Figure 19) relative to the convex lobes 982 prior to formation of the valve leaflets onto the valve frame.

[0157] The mandrel 970 was then spray coated with a PTFE mold release agent. Four layers of the ePTFE membrane previously described in this example were wrapped around the mandrel. MED-6215 was wiped onto the ePTFE and allowed to wet into and substantially fill the pores of the ePTFE. Excess MED-6215 was blotted off and the frame 960 with the composite fiber 966 wrapped posts 964 was positioned on the mandrel 970 along the frame seating area 984, as shown in

Figure 22. Silicone MED-4720, NuSil, Carpinteria, CA, USA was placed along the top edges 968 of the frame 960 and along the posts 964 of the frame 960 to create a strain relief within the leaflet (not shown). Eight additional layers of ePTFE were wrapped around the frame 960 and mandrel 970. Additional MED-6215 was wiped onto the ePTFE and allowed to wet into and substantially fill the pores of the ePTFE. Another 8 layers of ePTFE were wrapped around the frame 960 and mandrel 970. These layers form a blotter to absorb any excess silicone during the molding process and were removed after the silicone had cured.

[0158] Silicone rubber forms (not shown) molded with one surface exactly matching the inverse shape of the mandrel surface were previously fabricated for each of the 3 leaflet-forming features. These forms were spray coated with PTFE mold release and then mated to the matching feature of the mandrel. Approximately 50 wraps of an ePTFE fiber (not shown) were wound around the silicone forms to apply generally radial pressure to the valve against the mandrel.

[0159] This assembly was then placed in an oven at about 100°C for about 1 hour to cure the silicone. After cooling, the fiber and silicone forms were removed, the 8 layers of blotter ePTFE were peeled away and discarded, and the resulting valve (not shown) was slid off of the mandrel. The posts were trimmed using wire cutters and the excess length of leaflet material and excess length of material at the base of the frame was carefully trimmed using scissors to form a completed valve assembly, which is shown and generally indicated at 990 in Figure 23. Thus, in one embodiment, the valve assembly 990 was formed having the frame or support structure 960; a plurality of leaflets 992 supported on the support structure 960 and movable between open and closed positions to regulate blood flow through the valve assembly 990; and a composite fiber 966 wrapped post 964 located between at least a portion of the support structure 960 and at least a portion of each leaflet 992 to minimize stress in the leaflets due to the coupling and/or proximity of the leaflets to the support structure. In another embodiment, the cushion member is formed from a composite material with at least one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores, as described above.

[0160] It should be appreciated that support structures other than as specifically shown in the figures may be utilized. Further, cushion members may be utilized anywhere along the support structure as necessary to minimize stress in the

leaflets due to the coupling and/or proximity of the leaflets to the support structure. For example, cushion member(s) may be coupled to the support structure along the parabolically shaped top edge.

[0161] It should also be appreciated that the cushion members may be formed as sheets and wrapped around desired locations along the support structure, or be formed from fibers of various cross sectional shapes and sizes.

[0162] It should also be appreciated that the cushion members may be formed as tubes and slid over the ends of the support structure, or be slit longitudinally and positioned around the desired location along the support structure.

[0163] The leaflets of the complete valve assembly were measured and determined to have an average thickness at the center of each leaflet of about 120 μm .

[0164] The valve assembly was then characterized for flow performance and subjected to accelerated testing as in Example 1. After each block of about 50 million cycles, the valve assembly was removed from the high rate fatigue tester and the hydrodynamic performance again characterized as in Example 1. The valve assembly was removed finally at about 150 million cycles and demonstrated acceptable performance and no hole formation.

[0165] Comparative Example A

[0166] Six valves were constructed in the manner of Example 1 with the exception that the elastomer was not incorporated. The ePTFE material was the same as that described in Example 1, but it was not imbibed with the fluoroelastomer copolymer and was instead coated with a discontinuous layer of FEP copolymer that served as a thermoplastic adhesive. Valves were constructed as in Example 1 with each leaflet comprising 3 layers of membrane resulting in a final leaflet thickness averaging about 20 μm . After hydrodynamic characterization, the valves were mounted in the Dynatek accelerated tester described in Example 1. By about 40 million cycles, edge delamination and hole formation in the leaflets was observed and the test was stopped.

[0167] Comparative Example B

[0168] Two valves were constructed in the manner of Example 1 but did not incorporate the elastomer portion of the embodiments. The material employed was thin ePTFE membrane possessing properties similar to the following: a mass per

area of about 2.43 g/m^2 , a porosity of about 88%, an IBP of about 4.8 KPa, a thickness of about $13.8 \text{ }\mu\text{m}$, a matrix tensile strength in one direction of about 662 MPa, and a matrix tensile strength of about 1.2 MPa in the orthogonal direction. The ePTFE membrane was tested in accordance with the methods described in the Appendix. Ten layers of the membrane were placed in alternating directions onto a stack and then placed on the tooling as described in Example 1. The tooling was then exposed to about 350°C in a convection air oven for about 25 minutes, removed and quenched in a water bath. The three pieces of tooling were then inserted into the stent frame and the leaflets bonded to the valve assembly with FEP as in Example 1.

[0169] Each valve was subjected to high-rate fatigue testing using the real-time heart flow pulse duplicator system, as described above. After about 30 million cycles on one valve and about 40 million cycles on another valve, visual degradation, including stiffening and deformation, was observed and measurable decrease in performance was noted. In addition to the visual and measurable degradation in performance, Table 3 below summarizes the pressure drop, effective orifice area (EOA), and regurgitant fraction measured after about 40 million cycles.

Table 3

Number of Cycles (Millions)	Pressure Drop (mm Hg)	EOA (cm^2)	Regurgitant Fraction (%)
0	3.9	3.11	8.1
40×10^6	6.5	2.85	14.1

[0170] The material properties of the following non-limiting examples are provided in FIG. 42, Table 4, for reference to the individual descriptions, wherein like parts from the previous exemplary embodiments are enumerated with like prime numerals.

[0171] **Example 4a**

[0172] In exemplary embodiments, a heart valve having polymeric leaflets formed from a composite material having an expanded fluoropolymer membrane and an elastomeric material and joined to a semi-rigid, non-collapsible metallic frame, and further a having strain relief and sewing ring was constructed according to the following process:

[0173] A valve frame was laser machined from a length of MP35N cobalt chromium tube hard tempered with an outside diameter of 26.0 mm and a wall thickness of 0.6 mm in the shape shown illustratively and generally indicated at 1000 in Figure 24. The frame 1000 was electro-polished resulting in 0.0127 mm material removal from each surface and leaving the edges rounded. The frame 1000 was exposed to a surface roughening step to improve adherence of leaflets to the frame 1000, without degrading fatigue durability performance. The frame 1000 was cleaned by submersion in an ultrasonic bath of acetone for approximately five minutes. The entire metal frame surface was then subjected to a plasma treatment using methods commonly known to those having ordinary skill in the art. This treatment also served to improve the wetting of the fluorinated ethylene propylene (FEP) adhesive.

[0174] FEP powder (Daikin America, Orangeburg N.Y.) was then applied to the frame. More specifically, the FEP powder was stirred to form an airborne "cloud" in an enclosed blending apparatus, such as a standard kitchen type blender, while the frame is suspended in the cloud. The frame was exposed to the FEP powder cloud until a uniform layer of powder was adhered to the entire surface of the frame. The frame was then subjected to a thermal treatment by placing it in a forced air oven set to 320°C for approximately three minutes. This caused the powder to melt and adhere as a thin coating over the entire frame. The frame was removed from the oven and left to cool to room temperature.

[0175] The strain relief and sewing ring were attached to the frame in the following manner. A 23mm diameter cylindrical mandrel was wrapped with a single layer of Kapton® (El DuPont de Nemours, Inc., Wilmington, DE) polyimide film and held in place by an adhesive strip of Kapton® tape over the length of the overlapping seam. One wrap of a two layer laminate consisting of an ePTFE membrane laminated to a 25.4 µm thick layer of fluoroelastomer, as described in Example 1, was wrapped with the high strength of the membrane aligned along a direction generally parallel with the axis of the Kapton®-covered mandrel with no substantial overlap at the seam. The frame was aligned coaxially over the wrapped mandrel. An additional wrap of the two layer laminate was wrapped onto the mandrel encapsulating the entire frame with the seam oriented 180° from the seam of the single inner wrap. The four layer laminate was end cut about 135 mm from the base

of the frame encapsulated within. The four layer laminate was hand rolled axially in the toward the base of the frame until the 135 mm length of material formed an approximate 3 mm outer diameter ring adjacent to the base of the frame. The four layer laminate was end cut approximately 20 mm from the top of the frame and the assembly was compression wrapped helically with two sacrificial layers of ePTFE membrane imbibed with a polyimide, four layers of unsintered ePTFE membrane, and approximately one hundred wraps of an ePTFE fiber. The entire assembly was subjected to a thermal treatment by placing it in a forced air oven set to 280°C for five minutes and returned to room temperature by immediate water quench upon removal from the oven. The sacrificial layers were removed and the four layer laminate at the top end of the frame trimmed to allow about a 2 mm length to extend beyond the perimeter of the top of the frame. The mandrel and Kapton were then removed from the interior of the frame resulting in the frame assembly, generally indicated at 1010 in Figure 25, having the strain relief 1012 and sewing ring 1014 with the frame 1000 laminated within.

[0176] A single female mold or base tool, shown illustratively and indicated at 50 in Figure 5a, is provided with concave cavities (502, 504, 506) generally defining the shape of the tri-leaflet. Three male molds or leaflet tools (100) are provided with end surfaces (103) corresponding in shape and contour with the concave cavities in the base tool. The leaflet tools are pivotally coupled to each other, which helps to maintain relative axial and rotational spacing as depicted in the tri-leaflet assembly (400) in Figure 5a. The base and leaflet tools are wrapped with a single layer of unsintered ePTFE membrane to form a cushioning layer and then a single layer of substantially nonporous ePTFE membrane with FEP on one side is used to adhere the membranes together and onto the mandrels with a soldering iron. The sacrificial layers ensure that all the mating surfaces between the base and leaflet tools have a cushioning layer when compressed together; an additional function is as a release layer to prevent the leaflet material from adhering to the tools. The base and leaflet tools are initially combined to create a single cylindrical structure or combined tool assembly, as depicted in Figure 5b, to facilitate leaflet construction and attachment to the frame with the strain relief and sewing ring component via a tape wrapping process, as discussed in detail below.

[0177] A leaflet material was then prepared. A membrane of ePTFE was manufactured according to the general teachings described in US Patent 7,306,729. The ePTFE membrane had a mass per area of 1.15 g/m^2 , a bubble point of 79.7 MPa, a thickness of about 1016 nm, a matrix tensile strength of 410.9 MPa in the longitudinal direction and 315.4 MPa in the transverse direction. This membrane was imbibed with a fluoroelastomer, as described above in Example 1. The fluoroelastomer was dissolved in Novec HFE7500 (3M, St Paul, MN) in a 2.5% concentration. The solution was coated using a mayer bar onto the ePTFE membrane (while being supported by a polypropylene release film) and dried in a convection oven set to 145°C for 30 seconds. After 2 coating steps, the final ePTFE/fluoroelastomer or composite had a mass per area of 4.08 g/m^2 , 28.22 % fluoropolymer by weight, a dome burst strength of 15.9 KPa, and thickness of $1.93 \text{ }\mu\text{m}$.

[0178] Three layers of the leaflet or composite material was wrapped around the combined tool assembly with an elastomer rich side of the composite facing away from the tools. In exemplary embodiments, the composite material is oriented to have a predetermined matrix tensile strength along a direction generally parallel with the longitudinal axis of the combined tool assembly. More specifically, the predetermined matrix tensile strength is about 410 MPa.

[0179] Referring to Figures 26a and 26b, the frame assembly 1010 was positioned co-axially onto the combined tool assembly, generally indicated at 1020, over the three inner wraps of the composite material. The frame assembly 1010 was also aligned rotationally to match the features of the base tool 500', as depicted in Figure 26a. Twenty-three additional layers of the composite material were wrapped around the combined tool assembly 1020 with the elastomer rich side of each layer facing toward the tools previously wrapped by the three aforementioned layers of composite material. In exemplary embodiments, the additional layers of the composite material were each oriented to have a predetermined matrix tensile strength along a direction generally parallel with the longitudinal axis of the combined tool assembly. In one embodiment, the predetermined matrix tensile strength was about 410 MPa. The leaflet tools 100' were then removed from underneath the twenty-six layer composite laminate tube.

[0180] Each of the leaflet tools 100' was then moved rotatably about its respective end pivot, as depicted in Figure 26b, to allow the composite laminate tube 1015 from the previous step to be positioned between the leaflet tools 100'. The leaflet tool assembly was coaxially aligned to the base tool 500' and the leaflet tools 100' rotated inwardly toward each other to compress the twenty-six layer composite laminate tube onto the female tri-leaflet mold surface configuration of the base tool 500'. The combined tool assembly comprising the leaflet and base tools, composite laminate, strain relief, frame, and sewing ring was then mounted between fixed and translational portions of a fixture. Both radial and axial compression were applied by radially clamping the leaflet tools 100' while simultaneously applying an axial load with the translational end of the fixture.

[0181] The combined tool assembly was then compression wrapped helically with two sacrificial layers of compliant ePTFE membrane imbibed with a polyimide, four layers of un-sintered ePTFE membrane, and approximately one hundred wraps of an ePTFE fiber. The entire assembly was removed from the lathe and placed in a clamping fixture to maintain axial compression while subjected to a thermal treatment by placing it in a forced air oven set to about 280°C for about 30 minutes. The assembly was removed from the oven and brought back to room temperature via immediate water quench. The sacrificial layers, leaflet and base tools were removed leaving a fully adhered valve in a closed three dimensional form.

[0182] The excess leaflet material was trimmed with scissors from the top of the frame posts to the common triple point of each leaflet to create three commissures or coapting surface regions as depicted in Figure 27. The leaflets were opened with an ePTFE mandrel tapered from 10 mm to 25 mm. The annular sewing ring 1014 at the base of the frame 1000 was molded into a flange by placing the frame assembly 1010 between corresponding halves 1030a, 1030b of a fixture, as illustrated in Figures 28 and 29 and placing the assembly in an ultrasonic compression welder (not shown), such as a model #8400 ultrasonic compression welder made by Branson ultrasonics, Danbury CT. A weld time of about 0.8 seconds, hold time of about 3.0 seconds, and pneumatic pressure of about 0.35 MPa was applied to the assembly. The ultrasonic welding process was performed twice to create a sewing ring flange thickness of approximately 2 mm with an outer

diameter of 33 mm. The final valve assembly is shown illustratively and generally indicated at 1100 in Figure 30.

[0183] The final leaflet was comprised of 28.22 % fluoropolymer by weight with a thickness of 50.3 μm . Each leaflet had 26 layers of the composite and a ratio of thickness/number of layers of 1.93 μm .

[0184] The resulting valve assembly 1100 includes leaflets 1102 formed from a composite material with more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer. Each leaflet 1102 is movable between a closed position, shown illustratively in Figures 30A, in which blood is substantially prevented from flowing through the valve assembly, and an open position, shown illustratively in Figure 30B, in which blood is allowed to flow through the valve assembly. Thus, the leaflets 1102 of the valve assembly 1100 cycle between the closed and open positions generally to regulate blood flow direction in a human patient.

[0185] The hydrodynamic performance was measured prior to accelerated wear testing. The performance values were; EOA = 1.88 cm^2 and regurgitant fraction = 10.86 %. No observable damage has been recorded during durability testing with the number of cycles nearing 100 million.

[0186] **Example 4b**

[0187] In exemplary embodiments, a heart valve was constructed with a valve frame, strain relief, sewing ring, and first three layers of composite material, as described above in Example 4a, and utilizing a leaflet material comprising a final composite having a mass per area of 11.80 g/m^2 , 9.74% fluoropolymer by weight, a dome burst strength of 17.3 KPa, and thickness of 5.78 μm after the coating steps.

[0188] Six additional layers of the composite material were wrapped around the combined molds of Figure 26a with the membrane orientation as described in Example 4a.

[0189] The assembly was molded, thermally processed, and trimmed as described in Example 4a.

[0190] The final leaflet was comprised of 9.74% fluoropolymer by weight with a thickness of 52.0 μm . Each leaflet had 9 layers of the composite material and a ratio of thickness/number of layers of 5.78 μm .

[0191] The hydrodynamic performance was measured prior to accelerated wear testing. The performance values were; EOA = 2.05 cm^2 and regurgitant fraction = 11.71 %. Observable damage was recorded as frame detachment during durability testing at about 6 million cycles.

[0192] **Example 4c**

[0193] In exemplary embodiments, a heart valve was constructed with a valve frame that was laser machined and coated with FEP, as described above in Example 4a, and further provided with a cushion member attached to the perimeter of the frame adjacent to leaflets regions to minimize stress related to direct contact between the frame and the leaflet.

[0194] A 0.5 mm thick ePTFE fiber was helically wrapped onto a 1.143 mm mandrel with a pitch that eliminated space between wraps. Two layers of $2.54 \text{ }\mu\text{m}$ FEP film was wrapped over ePTFE fiber coils and was then subjected to a thermal treatment by placing it in a forced air oven set to 320°C for approximately three minutes. The material was brought back to room temperature via air cooling at room temperature. The ePTFE fiber formed a contiguous coil tube once removed from the mandrel. The coiled tube was cut into three 125 mm lengths and slit axially leaving only 5 mm intact as a coiled tube. Each of the three lengths was slid onto FEP-coated frame to form the frame 1000' having the cushion member 1030 attached thereto for minimizing stress related to direct contact between the frame 1000' and the leaflet (not shown), as depicted in Figure 31.

[0195] A valve frame, strain relief, sewing ring, leaflet material, and first layer of composite material were prepared, as described in Example 4a, encapsulating the cushion members and frame. The leaflet material was prepared such that after the coating steps, the final composite had a mass per area of 25.48 g/m^2 , 8.91% fluoropolymer by weight, a dome burst strength of 31.7 KPa, and thickness of $13.08 \text{ }\mu\text{m}$.

[0196] Three additional layers of the composite material were wrapped around the combined molds with the membrane orientation, as described in Example 4a.

[0197] The assembly was molded with cushion members, thermally processed, and trimmed as described in Example 4a to form the final valve assembly 1100' having the frame 1000' and the cushion member 1030 attached thereto for

minimizing stress related to direct contact between the frame 1000' and the leaflets 1102', as depicted in Figure 32.

[0198] The final leaflet was comprised of 8.91% fluoropolymer by weight with a thickness of 52.3 μm . Each leaflet had 4 layers of the composite and a ratio of thickness/number of layers of 13.08 μm .

[0199] The hydrodynamic performance was not measured prior to accelerated wear testing. Observable damage was recorded as a hole formation in leaflet during durability testing at about 12.4 million cycles.

[0200] **Example 5**

[0201] In exemplary embodiments, a heart valve was constructed having a valve frame, strain relief, sewing ring, leaflet material, and first three layers of composite material were prepared, as described in Example 4a, and further having the final leaflet described immediately below.

[0202] Fifteen additional layers of the composite material were wrapped around the combined molds and with the membrane orientation as described in Example 4a.

[0203] The assembly was molded, thermally processed, and trimmed as described in Example 4a.

[0204] The final leaflet was comprised of 9.74% fluoropolymer by weight with a thickness of 98.3 μm . Each leaflet had 18 layers of the composite and a ratio of thickness/number of layers of 5.46 μm .

[0205] The hydrodynamic performance was measured prior to accelerated wear testing. The performance values were; EOA = 1.73 cm^2 and regurgitant fraction = 11.71 %. Observable damage was recorded as frame detachment and leaflet delamination during durability testing at about 100 million cycles.

[0206] **Example 6**

[0207] In exemplary embodiments, a heart valve was constructed having a valve frame, cushion layer, strain relief, and sewing ring were prepared, as described in Example 4c, and further having the final leaflet as described immediately below.

[0208] A leaflet material was then prepared. The ePTFE membrane had a mass per area of 0.31 g/m^2 , a bubble point of 0.11 MPa, a thickness of about 127 nm, a matrix tensile strength of 442.0 MPa in the longitudinal direction and 560.0 MPa in the transverse direction. This membrane was imbibed with a fluoroelastomer

as described in Example 4a. After the coating steps, the final ePTFE/fluoroelastomer or composite had a mass per area of 1.04 g/m^2 , 29.9 % fluoropolymer by weight, a dome burst strength of 9.9 KPa, and thickness of $0.52 \text{ }\mu\text{m}$.

[0209] Ninety-five layers of the composite was wrapped around the combined molds with the membrane oriented such that the matrix tensile strength of 442 MPa is oriented axially and the elastomer rich side of the membrane facing toward the molds as described in Example 4a.

[0210] The assembly was molded, thermally processed, and trimmed as described in Example 4a.

[0211] The final leaflet was comprised of 29.00 % fluoropolymer by weight with a thickness of $49.7 \text{ }\mu\text{m}$. Each leaflet had 95 layers of the composite and a ratio of thickness/number of layers of $0.52 \text{ }\mu\text{m}$.

[0212] The hydrodynamic performance was measured prior to accelerated wear testing. The performance values were; EOA = 2.19 cm^2 and regurgitant fraction = 9.7 %. No observable damage has been recorded during durability testing.

[0213] **Example 7**

[0214] In other exemplary embodiments, a heart valve having polymeric leaflets was formed from a composite material having an expanded fluoropolymer membrane and an elastomeric material; joined to a metallic balloon expandable stent frame; and was constructed according to the following process:

[0215] A metallic balloon expandable stent frame was laser machined from a length of MP35N alloy annealed tube with an outside diameter of 26.00 mm and a wall thickness of 0.60 mm. A pattern was cut into the tube to form a cylindrically-shaped cut stent frame, also referred herein as a support structure, as illustrated and generally indicated at 600 in the flat plane view of Figure 6a. The support structure 600, includes a plurality of small closed cells 602, a plurality of large closed cells 604, and a plurality of leaflet closed cells 606. Note that one of the plurality of leaflet closed cells 606 appears as an open cell in Figure 6A due to the flat plane view. The cells 602, 604, 606 are generally arranged along rows forming the annular shape of the support structure 600.

[0216] The surface of the metallic frame was prepared as described in Example 4a.

[0217] An ePTFE laminate was attached to the frame with a strain relief, in a manner similar to Example 4c. A 24mm diameter cylindrical mandrel was wrapped with a single layer of Kapton® polyimide film (DuPont) and held in place by an adhesive strip of Kapton® tape over the length of the overlapping seam. Two layers of a substantially nonporous ePTFE having a layer of FEP disposed along an outer surface or side thereof was wrapped with the FEP facing away from the mandrel surface; two layers of FEP, 3.6 μm thick, were then wrapped over this. The metallic balloon expandable stent frame was aligned coaxially over the wrapped mandrel. An additional two layers of FEP were wrapped over the stent on the mandrel encapsulating the stent and strain relief. Two layers of a substantially porous ePTFE were wrapped over the FEP followed by an additional three layers of FEP wrapped over ePTFE. The entire assembly was subjected to a thermal treatment by placing it in a forced air oven set to 375°C for twenty minutes and returned to room temperature by immediate water quench upon removal from the oven. The laminate was trimmed from regions of the frame to expose three windows for leaflet attachment as depicted in Figure 33b.

[0218] A leaflet material was then prepared as described in Example 6. The ePTFE membrane had a mass per area of 0.29 g/m^2 , a bubble point of 0.11 MPa, a thickness of about 158 nm, a matrix tensile strength of 434.0 MPa in the longitudinal direction and 646.0 MPa in the transverse direction. This membrane was imbibed with a fluoroelastomer as described in Example 4a. After the coating process, the final ePTFE/ fluoroelastomer composite had a mass per area of 0.94 g/m^2 , 30.3 % fluoropolymer by weight, a dome burst strength of 4.14KPa, and thickness of 0.44 μm .

[0219] Seventeen layers of the composite was wrapped around a 26mm mandrel. The composite was oriented so that the matrix tensile strength of 434 MPa was placed axially and the elastomer rich side of the membrane was facing toward the mandrel as described in Example 4a.

[0220] The subassembly containing the frame and strain relief was positioned on the mandral over the 17 layers. An additional 40 layers of composite were wrapped, sandwiching the frame between both layers of composite creating a total of 57 layers of composite. The mandrel, leaflet layers, and frame were covered by an impermeable layer and sealed at both ends. Using a pressure vessel, the assembly

was heated to about 285°C at 75psi for about 23 minutes and then allowed to cool to room temperature while under pressure. The valve assembly was removed from the mandrel. The free edge of the leaflet was created by slicing the laminate in an arc at each of the three leaflet closed cells 606 on the frame freeing the leaflet to open and close under fluid pressure. The leaflets were molded into final shape using leaflet molding tools described in FIGs. 5A-5B. Each of the leaflet molding tools was coaxially aligned to the base tool to allow for a cover to be applied to the exterior of the frame.

[0221] A frame cover material was then prepared as described in Example 6. The ePTFE membrane had a mass per area of 0.86 g/m², a bubble point of 0.11 MPa, a thickness of about 900 nm, a matrix tensile strength of 376.0 MPa in the longitudinal direction and 501.0 MPa in the transverse direction. This membrane was imbibed with a fluoroelastomer as described in Example 4a. After the coating process, the final ePTFE/ fluoroelastomer composite had a mass per area of 7.05 g/m², 14.1 % fluoropolymer by weight, a dome burst strength of 13.1KPa, and thickness of 3.28 µm.

[0222] Fifteen layers of the composite was wrapped around the valve frame while being held in the shape set tooling. The composite was oriented so that the matrix tensile strength of 501 MPa was placed axially and the elastomer rich side of the membrane was facing toward the mandrel as described in Example 4a. The final cover was comprised of 14.1 % fluoropolymer by weight with a thickness of 49.2 µm.

[0223] The assembly was molded, thermally processed in an open atmosphere convection oven at 250 °C for 1 hour. The valve was then removed from the molding tooling.

[0224] The final leaflet was comprised of 30.3 % fluoropolymer by weight with a thickness of 25.0 µm. Each leaflet had 57 layers of the composite and a ratio of thickness/number of layers of 0.44 µm.

[0225] A plurality of longitudinally extending slits 1302 were formed in the tube 1300 resulting in the formation of a plurality of tabs 1304. The slits can be formed by any suitable method known to those having ordinary skill in the art, such as by cutting with a blade.

[0226] The leaflet tools (not shown) were then slid out from underneath the tube 1300.

[0227] The three tabs 1304 created by forming the slits 1302 in the tube 1300 were then fed inwardly through respective windows or cells formed in the frame, as depicted in Figure 35. Each of the leaflet tools was coaxially aligned to the base tool to allow the inwardly fed tabs 1304 of the tube 1300 from the previous step to be positioned and compressed between the leaflet tools and the female tri-leaflet mold surface configuration of the base tool. The combined tool assembly comprising the leaflet and base tools, composite or leaflet material, and frame was then mounted between fixed and translational portions of a fixture. Both radial and axial compression were applied by radially clamping the leaflet tools while simultaneously applying an axial load with the translational end of the fixture.

[0228] The assembly was molded, thermally processed, and trimmed as described in Example 4a. The final valve assembly having the metallic balloon expandable stent frame 600", cushion members 1030", and leaflets 704" is shown in Figure 36.

[0229] The final leaflet was comprised of 33.70% fluoropolymer by weight with a thickness of 16.0 μm . Each leaflet had fifty layers of the composite and a ratio of thickness/number of layers of 0.32 μm .

[0230] The hydrodynamic performance was measured prior to use. The performance values were; EOA = 2.0 cm^2 and regurgitant fraction = 15.7 %. No observable damage has been recorded during durability testing.

[0231] Following construction and testing, the valve was sent to Carmeda Corporation (Carmeda AB, Stockholm Sweden) for heparin coating. After coating, the completed valve was mounted on a balloon catheter and crushed to a reduced diameter of 20French using a mechanical iris crushing apparatus. The catheter-mounted valve was forwarded to Sterigenics corp. (Salt lake city UT) for ethylene oxide sterilization. Using sterile technique the valve was inserted through a 20F sheath into the surgically exposed iliac artery of an anesthetized 4 month old, 25Kg Ramboulet sheep. The catheter was advanced through the inferior vena cava, through the right atrium and into the pulmonary artery trunk. It was deployed over the native pulmonary valve and actuated by pressurizing the balloon catheter to 4 atmospheres. Following angiogram and pressure measurements, the catheter was withdrawn and the animal recovered. The valve, referred below as the explanted

valve, remained in place for one month, replacing the function of the native pulmonary valve.

[0232] The hydrodynamic performance of the explanted valve was measured after explant and compared with a control valve. The explanted valve was explanted, fixed in formalin solution, digested in sodium hydroxide, rinsed in ethanol, acetone and distilled water prior to testing. The control valve was a duplicate of the explanted valve that was compressed to the delivery diameter, redeployed on a balloon catheter and tested. Each valve was tested under both aortic and pulmonary flow conditions in a ViVitro real time tester. No degradation in hemodynamic performance was observed.

[0233] The performance values for the explanted and control valves are listed in Table 5.

Table 5

Aortic conditions, 70 bpm, 5 liter/min, 125/89 peak bp			
	Pressure Drop (mm Hg)	EOA (cm ²)	Closing volume (ml)
Control	8.9	1.99	4.12
Explanted valve	6.8	2.12	2.69
Pulmonary conditions, 70 bpm, 5 liter/min, 26/15 peak bp			
Control	9.5	1.82	2.25
Explanted	8.9	1.76	2.25

[0234] **Example 8**

[0235] In exemplary embodiments, a heart valve having polymeric leaflets joined to a rigid metallic frame was constructed according to the following process:

[0236] A valve support structure or frame 960 was laser cut from a length of 316 stainless steel tube with an outside diameter of 25.4mm and a wall thickness of 0.5mm in the shape shown in Figure 19. In the embodiment shown, the frame 960 extends axially between a bottom end 962 and an opposite top end defined generally by a plurality of axially extending, generally spire shaped posts 964 corresponding to

the number of leaflets in the intended finished valve assembly (not shown). A parabolically shaped top edge 968 extends between adjacent posts 964. In the specific embodiment shown, three posts 964 and three top edges 968 form the top end of the frame 960. The corners of the frame that would be in contact with the leaflet material were rounded using a rotary sander and hand polished. The frame was rinsed with water and then plasma cleaned using a PT2000P plasma treatment system, Tri-Star Technologies, El Segundo, CA, USA.

[0237] A cushion member is provided between at least a portion of the frame and at least a portion of the leaflet to minimize stress related to direct contact between the frame and the leaflet. A composite fiber of ePTFE and silicone was created by first imbibing an ePTFE membrane with silicone MED-6215 (NuSil, Carpinteria, CA, USA), slitting it to a width of 25 mm, and rolling into a substantially round fiber. The ePTFE used in this fiber was tested in accordance with the methods described in the Appendix. The ePTFE membrane had a bubble point of 217 KPa, a thickness of 10 μm , a mass per area of 5.2 g/m^2 , a porosity of 78%, a matrix tensile strength in one direction of 96 MPa, and a matrix tensile strength of 55 MPa in an orthogonal direction. The composite fiber 966 was wrapped around each of the posts 964 of the valve frame 960 as shown in Figure 20.

[0238] A mandrel 970 was formed using stereolithography in a shape shown in Figure 21. The mandrel 970 has a first end 972 and an opposite second end 974, and extends longitudinally therebetween. The mandrel 970 has an outer surface 980 having three (two shown) generally arcuate, convex lobes 982, each generally for forming leaflets (not shown) of a finished valve assembly (not shown). The outer surface 980 also includes a frame seating area 984 for positioning the valve frame (960 in Figure 19) relative to the lobes 982 prior to formation of the valve leaflets onto the valve frame.

[0239] The mandrel 970 was then spray coated with a PTFE mold release agent. Four layers of ePTFE membrane were wrapped around the mandrel. The ePTFE membrane was tested in accordance with the methods described in the Appendix. The ePTFE membrane had a mass per area of 0.57 g/m^2 , a porosity of 90.4%, a thickness of about 2.5 μm , a bubble point of 458 KPa, a matrix tensile strength of 339 MPa in the longitudinal direction and 257 MPa in the transverse direction. MED-6215 was wiped onto the ePTFE and allowed to wet into and

substantially fill the pores of the ePTFE. Excess MED-6215 was blotted off and the valve frame 960 with the composite fiber 966 wrapped posts 964 was positioned on the mandrel 970 along the frame seating area 984, as shown in Figure 22. Silicone MED-4720, NuSil, Carpinteria, CA, USA was placed along the top edges 968 of the frame 960 and along the posts 964 of the frame 960 to create a strain relief within the leaflet (not shown). Thirty additional layers of the same ePTFE were wrapped around the frame 960 and mandrel 970. Additional MED-6215 was wiped onto the ePTFE and allowed to wet into and substantially fill the pores of the ePTFE. 8 layers of ePTFE membrane were wrapped around the frame 960 and mandrel 970. The ePTFE used was tested in accordance with the methods described in the Appendix. The ePTFE membrane had a bubble point of 217 KPa, a thickness of 10 μm , a mass per area of 5.2 g/m^2 , a porosity of 78%, a matrix tensile strength in one direction of 96 MPa, and a matrix tensile strength of 55 MPa in an orthogonal direction. These layers absorbed any excess silicone during the molding process and were removed after the silicone had cured.

[0240] Silicone rubber forms (not shown) molded with one surface exactly matching the inverse shape of the mandrel surface were previously fabricated for each of the 3 leaflet-forming features. These forms were spray coated with PTFE mold release and then mated to the matching feature of the mandrel. Approximately 50 wraps of an ePTFE fiber (not shown) were wound around the silicone forms to apply generally radial pressure to the valve against the mandrel.

[0241] This assembly was then placed in an oven at 100°C for 1 hour to cure the silicone. After cooling, the fiber and silicone forms were removed, the 8 layers of blotter ePTFE were peeled away and discarded, and the resulting valve (not shown) was slid off of the mandrel. The posts were trimmed using wire cutters and the excess length of leaflet material and excess length of material at the base of the frame was carefully trimmed using scissors to form a completed valve assembly, which is shown and generally indicated at 990 in Figure 23. Thus, in one embodiment, the valve assembly 990 was formed having the frame or support structure 960; a plurality of leaflets 992 supported on the support structure 960 and movable between open and closed positions to regulate blood flow through the valve assembly 990; and a cushion member 1030 located between at least a portion of the support structure 960 and at least a portion of each leaflet 992 to minimize stress in

the leaflets due to the coupling and/or proximity of the leaflets to the support structure. In another embodiment, the cushion member is formed from a composite material with at least one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores, as described above.

[0242] It should be appreciated that support structures other than as specifically shown in the figures may be utilized. Further, cushion members may be utilized anywhere along the support structure as necessary to minimize stress in the leaflets due to the coupling and/or proximity of the leaflets to the support structure. For example, cushion member(s) may be coupled to the support structure along the parabolically shaped top edge.

[0243] It should also be appreciated that the cushion members may be formed as sheets and wrapped around desired locations along the support structure, or be formed from fibers of various cross sectional shapes and sizes.

[0244] It should also be appreciated that the cushion members may be formed as tubes and slid over the ends of the support structure, or be slit longitudinally and positioned around the desired location along the support structure.

[0245] The leaflets of the complete valve assembly were measured and determined to have an average thickness at the center of each leaflet of about 48 μm .

[0246] The final leaflet was comprised of 24.00% fluoropolymer by weight with a thickness of 48.0 μm . Each leaflet had 48 layers of the composite and a ratio of thickness/number of layers of 1.07 μm .

[0247] The hydrodynamic performance was measured prior to accelerated wear testing. The performance values were; EOA = 2.4 cm^2 and regurgitant fraction = 12.5 %. No observable damage has been recorded during durability testing with the number of cycles of about 150 million.

[0248] The hydrodynamic performance of the valves described in Examples 4a, 4b, 5, 6, 7, and 8 was characterized on a real-time pulse duplicator that measured typical anatomical pressures and flows across the valve, generating an initial or "zero fatigue" set of data for that particular valve assembly.

[0249] Following flow performance characterization, the valve assemblies were then removed from the flow pulse duplicator system and placed into a high-rate fatigue or durability tester. The valves were continuously monitored to ensure they

held pressure when closed and to assess when any damage in the form of frame detachment, tears, holes, or delamination occurred. Where appropriate, the hydrodynamic performance of valves were again measured post durability testing at about 100 million cycles and recorded.

[0250] The results of the performance characterizations are listed in FIG. 43, Table 6.

[0251] The data presented in Examples 4a, 4b, 4c, 5, 6, 7 & 8 and summarized in Tables 4, 5 and 6 support the observation of general durability and hydrodynamic performance trends associated with different leaflet configurations when thickness, percent fluoropolymer by weight, and number of layers are varied. The number of Examples presented support these observations by allowing comparisons to be made when differences due to frame type and cushion members are used in the individual valve construction.

[0252] Examples 4b and 4c are configurations where leaflet thickness and percent fluoropolymer by weight are equal and illustrate that low layer numbers lead to reduced durability. The failure mode of Example 4b of frame detachment was mitigated by using a cushion member which in turn doubled the time to failure, however the failure mode switched from frame detachment to hole formation within the leaflet. Both Examples 4a and 4b had durability failures well below what is acceptable.

[0253] Examples 4b and 5 provide a comparison where percent fluoropolymer by weight is held constant and a difference in layer number and therefore leaflet thickness are measured. Both Examples have the same valve construction without the cushion members which have been shown above to mitigate frame detachment. The effect of doubling the number of layers from 9 to 18 and therefore increasing the leaflet thickness from about 52 μm to about 98 μm improved the number of cycles to frame detachment by nearly an order of magnitude from 12 million to 100 million.

[0254] Example 4a, which again is of similar construction to Examples 4b, where leaflet thickness of about 50 μm is held constant and varying the percent fluoropolymer by weight from about 10 % for Example 4b to about 30 % for Example 4a enabled the creation of a thinner composite and therefore many more layers (26) for the same leaflet thickness. Although some free edge delamination has been observed for Example 4a near the high strain region of the triple point, the valve is

still viable as determined by hydrodynamic characterization with 100 million cycles accrued as shown in Table 5.

[0255] In examples 6 and 7, the improved bending behavior of these thin and high layer configurations generally indicate that improved durability follows when compared to lower layer number constructions due to the reduction in creases and wrinkles thought the duty cycle as illustrated in Figures 41A and 41B.

[0256] Additionally, Example 8 illustrates that similar durability can be achieved with different elastomers of high layer configurations as demonstrated by Examples 6 and 7.

[0257] It will be apparent to those skilled in the art that various modifications and variations can be made in the present embodiments without departing from the spirit or scope of the embodiments. Thus, it is intended that the present embodiments cover the modifications and variations of this invention provided they come within the scope of the appended claims and their equivalents.

APPENDIX

[0258] As used in this application, matrix tensile strength refers to the tensile strength of a porous fluoropolymer specimen under specified conditions. The porosity of the specimen is accounted for by multiplying the tensile strength by the ratio of density of the polymer to the density of the specimen.

[0259] As used herein the term "membrane" refers to a porous fluoropolymer article, "composite" refers to imbibed porous fluoropolymers, and a "leaflet" is a component of an implantable article for regulating blood flow direction. Leaflets of the present embodiments are one or more layers of a composite.

[0260] The term "imbibe" used herein refers to any process used to at least partially fill pores with a secondary material.

[0261] For porous fluoropolymer leaflets having pores substantially filled with elastomer, the elastomer can be dissolved or degraded and rinsed away using an appropriate solvent in order to measure desired properties.

[0262] As the term "elastomer" is used herein it defines a polymer, mixture of polymers, or mixture of one or more polymers with one or more non-polymeric components that has the ability to be stretched to at least 1.3 times its original length and to retract rapidly to approximately its original length when released. The term "elastomeric" is intended to describe a property whereby a polymer displays stretch and recovery properties similar to an elastomer, although not necessarily to the same degree of stretch and/or recovery.

[0263] As the term "thermoplastic" is used herein it defines a polymer that softens when exposed to heat and returns to its original condition when cooled to room temperature. Such a polymer can be made to soften, flow or take on new shapes, without significant degradation or alteration of the polymer's original condition, by the application of heat or heat and pressure. In contrast to a thermoplastic polymer, a "thermoset" polymer is hereby defined as a polymer that solidifies or "sets" irreversibly when cured. A determination of whether a polymer is a "thermoplastic" polymer within the meaning of the present embodiments can be made by slowly elevating the temperature of a stressed specimen and watching for deformation. If the polymer can be made to soften, flow, or take on a new shape, without significant degradation or alteration of the polymer's original chemical condition, then the polymer is considered to be a thermoplastic. If only small

amounts of material are available it may be necessary to use a hot stage microscope for this determination.

[0264] One measure of the quality of a valve is the effective orifice area (EOA), which can be calculated as follows: $EOA(\text{cm}^2) = Q_{\text{rms}} / (51.6 * (\Delta P)^{1/2})$ where Q_{rms} is the root mean square systolic/diastolic flow rate (cm^3/s) and ΔP is the mean systolic/diastolic pressure drop (mmHg).

[0265] Another measure of the hydrodynamic performance of a valve is the regurgitant fraction, which is the amount of fluid or blood regurgitated through the valve divided by the stroke volume.

[0266] As used in this application, the surface area per unit mass, expressed in units of m^2/g , was measured using the Brunauer-Emmett-Teller (BET) method on a Coulter SA3100 Gas Adsorption Analyzer, Beckman Coulter Inc. Fullerton CA, USA. To perform the measurement, a sample was cut from the center of the expanded fluoropolymer membrane and placed into a small sample tube. The mass of the sample was approximately 0.1 to 0.2 g. The tube was placed into the Coulter SA-Prep Surface Area Outgasser (Model SA-Prep, P/n 5102014) from Beckman Coulter, Fullerton CA, USA and purged at about 110°C for about two hours with helium. The sample tube was then removed from the SA-Prep Outgasser and weighed. The sample tube was then placed into the SA3100 Gas adsorption Analyzer and the BET surface area analysis was run in accordance with the instrument instructions using helium to calculate the free space and nitrogen as the adsorbate gas.

[0267] Bubble point and mean flow pore size were measured according to the general teachings of ASTM F31 6-03 using a capillary flow Porometer, Model CFP 1500AEXL from Porous Materials, Inc., Ithaca NY, USA. The sample membrane was placed into the sample chamber and wet with SilWick Silicone Fluid (available from Porous Materials Inc.) having a surface tension of about 20.1 dynes/cm. The bottom clamp of the sample chamber had an about 2.54 cm diameter hole. Using the Capwin software version 7.73.012 the following parameters were set as specified in the table below.

[0268] <u>Parameter</u>	<u>Set Point</u>
[0269] Maxflow (cm^3/m)	200000
[0270] Bubflow(cm^3/m)	100

[0271] F/PT (old bubltime)	50
[0272] Minbpress (PSI)	0
[0273] Zerotime (sec)	1
[0274] V2incr(cts)	10
[0275] Preginc (cts)	1
[0276] Pulse delay(sec)	2
[0277] Maxpre (PSI)	500
[0278] Pulse width (sec)	0.2
[0279] Mineqtime (sec)	30
[0280] Presslew (cts)	10
[0281] Flowslew (cts)	50
[0282] Eqiter	3
[0283] Aveiter	20
[0284] Maxpdif (PSI)	0.1
[0285] Maxfdif (PSI)	50
[0286] Sartp(PSI)	1
[0287] Sartf (cm ³ /m)	500

[0288] Membrane thickness was measured by placing the membrane between the two plates of a Käfer FZ1000/30 thickness snap gauge Käfer Messuhrenfabrik GmbH, Villingen-Schwenningen, Germany. The average of the three measurements was reported.

[0289] The presence of elastomer within the pores can be determined by several methods known to those having ordinary skill in the art, such as surface and/or cross section visual, or other analyses. These analyses can be performed prior to and after the removal of elastomer from the leaflet.

[0290] Membrane samples were die cut to form rectangular sections about 2.54 cm by about 15.24 cm to measure the weight (using a Mettler-Toledo analytical balance model AG204) and thickness (using a Käfer Fz1000/30 snap gauge). Using these data, density was calculated with the following formula: $\rho = m/w \cdot l \cdot t$, in which: ρ = density (g/cm³): m = mass (g), w = width (cm), l = length (cm), and t = thickness (cm). The average of three measurements was reported.

[0291] Tensile break load was measured using an INSTRON 122 tensile test machine equipped with flat-faced grips and a 0.445 kN load cell. The gauge length

was about 5.08 cm and the cross-head speed was about 50.8 cm/min. The sample dimensions were about 2.54 cm by about 15.24 cm. For longitudinal measurements, the longer dimension of the sample was oriented in the highest strength direction. For the orthogonal MTS measurements, the larger dimension of the sample was oriented perpendicular to the highest strength direction. Each sample was weighed using a Mettler Toledo Scale Model AG204, then the thickness measured using the Käfer FZ1000/30 snap gauge. The samples were then tested individually on the tensile tester. Three different sections of each sample were measured. The average of the three maximum loads (i.e., peak force) measurements was reported. The longitudinal and transverse matrix tensile strengths (MTS) were calculated using the following equation: $MTS = (\text{maximum load/cross-section area}) \cdot (\text{bulk density of PTFE} / (\text{density of the porous membrane}))$, wherein the bulk density of the PTFE was taken to be about 2.2 g/cm^3 . Flexural stiffness was measured by following the general procedures set forth in ASTM D790. Unless large test specimens are available, the test specimen must be scaled down. The test conditions were as follows. The leaflet specimens were measured on a three-point bending test apparatus employing sharp posts placed horizontally about 5.08 mm from one another. An about 1.34 mm diameter steel bar weighing about 80 mg was used to cause deflection in the y (downward) direction, and the specimens were not restrained in the x direction. The steel bar was slowly placed on the center point of the membrane specimen. After waiting about 5 minutes, the y deflection was measured. Deflection of elastic beams supported as above can be represented by : $d = F \cdot L^3 / 48 \cdot EI$, where F (in Newtons) is the load applied at the center of the beam length, L (meters), so $L = 1/2$ distance between suspending posts, and EI is the bending stiffness (Nm). From this relationship the value of EI can be calculated. For a rectangular cross-section: $I = t^3 \cdot w / 12$, where I = cross-sectional moment of inertia, t = specimen thickness (meters), w = specimen width (meters). With this relationship, the average modulus of elasticity over the measured range of bending deflection can be calculated.

WHAT IS CLAIMED IS:

1. An implantable article for regulating blood flow direction in a human patient, comprising:
a leaflet having a thickness and formed from a composite material having more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer, the leaflet having a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 5.
2. The implantable article as set forth in claim 1, wherein the ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 3.
3. The implantable article as set forth in claim 1, wherein the ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 1.
4. The implantable article as set forth in claim 1, wherein the ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 0.5.
5. The implantable article as set forth in claim 1, wherein the EOA across the implantable article for regulating blood flow direction is maintained within 10% of the pre-cycling value after 40 million cycles.
6. The implantable article as set forth in claim 1, wherein the leaflet is devoid of edge delamination or hole formation after 40 million cycles.
7. The implantable article as set forth in claim 1, wherein the leaflet has at least 10 layers and a composite material comprising less than about 50% fluoropolymer by weight.
8. The implantable article as set forth in claim 7, wherein the leaflet has a thickness less than 100 μm .

9. The implantable article as set forth in claim 8, wherein the leaflet has a bending modulus of less than about 100 MPa.
10. An implantable article for regulating blood flow direction in a human patient, the article comprising:
 - a leaflet cyclable between a closed configuration for substantially preventing blood flow through the implantable article and an open configuration allowing blood flow through the implantable article, the leaflet being formed from a plurality of fluoropolymer layers and having a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 5, the leaflet maintaining substantially unchanged performance after actuation of the leaflet to at least 40 million cycles.
11. The implantable article as set forth in claim 10, wherein the leaflet remains substantially impermeable after actuation of the leaflet to at least 40 million cycles.
12. The implantable article as set forth in claim 11, wherein the leaflet remains substantially impermeable after actuation of the leaflet to at least 40 million cycles *in vivo*.
13. The implantable article as set forth in claim 10, wherein the leaflet is operatively coupled to a support frame and movable between the closed and open configurations relative to the support frame.
14. The implantable article as set forth in claim 13, wherein the support frame is selectively diametrically adjustable for endovascular delivery and deployment at a treatment site.
15. The implantable article as set forth in claim 10, wherein the performance of the leaflet remains substantially unchanged after compacting and expanding prior to cycling of the leaflet.

16. The implantable article as set forth in claim 10, wherein the performance of the leaflet remains substantially unchanged after endovascular delivery of the implantable article.
17. The implantable article as set forth in claim 10, wherein the leaflet encompasses a radiopaque element.
18. A method of forming a leaflet of an implantable article for regulating blood flow direction in a human patient, the method comprising:
 - providing a composite material having more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer; and
 - bringing more than one layer of the composite material into contact with additional layers of the composite material by wrapping a sheet of the composite material with a starting and ending point defined as an axial seam adhered to itself.
19. The method as set forth in claim 18, wherein the sheet of the composite material is wrapped generally radially with the starting and ending point defined as the axial seam adhered to itself.
20. The method as set forth in claim 19, wherein the sheet of the composite material is substantially contiguous.
21. The method as set forth in claim 18, wherein the sheet of the composite material has a ratio of leaflet thickness (μm) to number of layers of fluoropolymer of less than about 5.
22. An implantable article for regulating blood flow direction in a human patient, the article comprising a polymeric leaflet having a thickness of less than about 100 μm .

23. The implantable article as set forth in claim 22, wherein the leaflet is formed from a composite material having more than one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the more than one fluoropolymer layer.

24. The implantable article as set forth in claim 23, wherein the leaflet includes at least 10 layers of the composite material.

25. An implantable article for regulating blood flow direction in a human patient, comprising:

a leaflet comprising a composite material having at least one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores of the at least one fluoropolymer layer, the composite material comprising less than about 80% fluoropolymer by weight.

26. The implantable article as set forth in claim 25, wherein the composite material comprises less than about 70% fluoropolymer by weight.

27. The implantable article as set forth in claim 25, wherein the composite material comprises less than about 60% fluoropolymer by weight.

28. The implantable article as set forth in claim 25, wherein the composite material comprises less than about 50% fluoropolymer by weight.

29. The implantable article as set forth in claim 25, wherein the composite material further includes a layer of the elastomer.

30. The implantable article as set forth in claim 29, wherein the elastomer is a fluoroelastomer.

31. The implantable article as set forth in claim 30, wherein the elastomer is a TFE/PMVE copolymer.

32. The implantable article as set forth in claim 31, wherein the copolymer comprises essentially of between about 40 and 80 weight percent perfluoromethyl vinyl ether and complementally 60 and 20 weight percent tetrafluoroethylene.
33. The implantable article as set forth in claim 29, wherein the fluoropolymer is PTFE.
34. The implantable article as set forth in claim 29, wherein the PTFE is ePTFE.
35. The implantable article as set forth in claim 34, wherein the at least one fluoropolymer layer has a matrix tensile strength in at least one direction greater than about 96 MPa.
36. The implantable article as set forth in claim 25, wherein the elastomer is a fluoroelastomer.
37. The implantable article as set forth in claim 36, wherein the elastomer is a TFE/PMVE copolymer.
38. The implantable article as set forth in claim 37, wherein the copolymer comprises essentially of between about 40 and 80 weight percent perfluoromethyl vinyl ether and complementally about 60 and 20 weight percent tetrafluoroethylene.
39. The implantable article as set forth in claim 25, wherein the fluoropolymer is PTFE.
40. The implantable article as set forth in claim 38, wherein the PTFE is ePTFE.
41. The implantable article as set forth in claim 39, wherein the at least one fluoropolymer layer has a matrix tensile strength in at least one direction greater than about 96 MPa.

42. The implantable article as set forth in claim 25, wherein the leaflet has a thickness of less than about 350 μm .
43. The implantable article as set forth in claim 25, wherein the leaflet has a thickness of less than about 300 μm .
44. The implantable article as set forth in claim 25, wherein the leaflet has a thickness of less than about 200 μm .
45. The implantable article as set forth in claim 25, wherein the leaflet has a thickness of less than about 100 μm .
46. The implantable article as set forth in claim 25, wherein the leaflet has a thickness of less than about 50 μm .
47. The implantable article as set forth in claim 25, wherein the leaflet has a thickness of less than about 25 μm .
48. The implantable article as set forth in claim 25, wherein the EOA across the implantable article for regulating blood flow direction is maintained within about 10% after about 40 million cycles.
49. The implantable article as set forth in claim 25, wherein a regurgitant fraction across the implantable article for regulating blood flow direction is maintained below about 15% after about 40 million cycles.
50. The leaflet as set forth in claim 25, wherein the leaflet is devoid of edge delamination or hole formation after about 40 million cycles.
51. A method of forming the composite material of the implantable article of claim 25, the method comprising the steps of:
dissolving an elastomer in a solvent suitable to create a solution to substantially fill the pores of the membrane;

substantially fill the pores of the membrane; and
allowing the solvent to evaporate so that the elastomer remains in
substantially all of the pores of the membrane.

52. A method of forming the composite material of the implantable article of claim 25, the method comprising the step of delivering the elastomer via a dispersion to substantially fill the pores of the at least one fluoropolymer layer.

53. A method of forming the composite material of the implantable article of claim 25, the method comprising the step of bringing the at least one fluoropolymer layer into contact with a sheet of the elastomer under conditions of heat or pressure that allow elastomer to substantially fill the pores of the at least one fluoropolymer layer.

54. A method of forming the composite material of the implantable article of claim 25, the method comprising the step of polymerizing the elastomer within the pores of the at least one fluoropolymer layer.

55. The implantable article as set forth in claim 34, wherein the composite material comprises less than about 50% fluoropolymer by weight.

56. An implantable article for regulating blood flow direction in a human patient, the implantable article comprising:

a support structure;
a leaflet supported on the support structure and movable between open and closed positions to regulate blood flow through the implantable article; and
a cushion member located between at least a portion of the support structure and at least a portion of the leaflet, wherein the cushion member is formed from a composite material with at least one fluoropolymer layer having a plurality of pores and an elastomer present in substantially all of the pores.

57. The implantable article as set forth in claim 56, wherein the cushion member includes expanded fluoropolymer.

58. The implantable article as set forth in claim 56, wherein the cushion member is formed as a fiber.

59. The implantable article as set forth in claim 56, wherein the cushion member is formed as a sheet.

60. The implantable article as set forth in claim 56, wherein the cushion member is formed as a tube.

61. The implantable article as set forth in claim 58, wherein the cushion member is wrapped generally helically about the at least a portion of the support structure to provide a cushion between the at least a portion of the support structure and the leaflet.

62. The implantable article as set forth in claim 56, wherein the support structure includes a longitudinally extending post about which a portion of the leaflet is wrapped to secure the leaflet to the support structure.

63. The implantable article as set forth in claim 58, wherein the fluoropolymer layer of the cushion member is formed from porous ePTFE.

64. The implantable article as set forth in claim 63, wherein the cushion member is formed as a fiber.

65. The implantable article as set forth in claim 64, wherein the fiber is wrapped generally helically about the post to provide a cushion between the post and the portion of the leaflet wrapped about the post.

66. The implantable article as set forth in claim 64, wherein the fiber is formed from a sheet of ePTFE having a plurality of pores and an elastomer present in substantially all of the pores.

67. An implantable article for regulating blood flow direction in a human patient, the implantable article comprising:

a generally annular shaped support structure, the support structure having a first end and an opposite second end, the first end having a longitudinally extending post;

a sheet of leaflet material extending along an outer periphery of the support structure and forming a first leaflet and a second leaflet each extending along opposite sides of the post; and

a cushion member coupled to the post to provide a cushion between the post and the leaflets.

68. The implantable article as set forth in claim 67, wherein the cushion member is a fiber formed from a sheet of ePTFE having a plurality of pores and an elastomer present in substantially all of the pores.

69. An implantable article for regulating blood flow direction in a human patient, the implantable article comprising:

a leaflet comprising a composite material having at least one fluoropolymer layer having a plurality of pores and an elastomer substantially filling the pores of the at least one fluoropolymer layer, the composite material comprising less than about 80% fluoropolymer by weight.

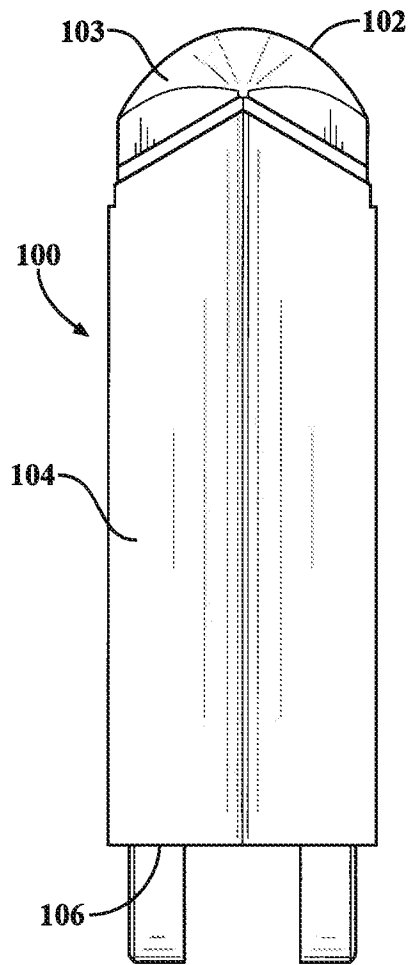


FIG. 1A

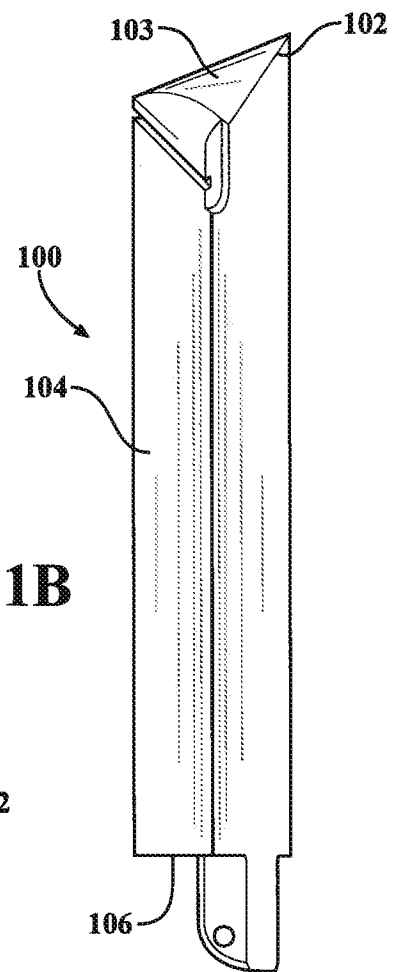


FIG. 1B

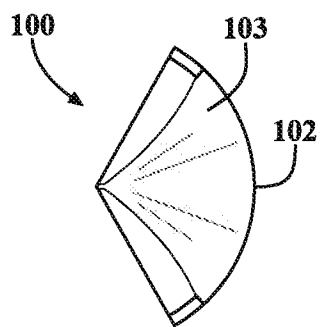


FIG. 1C

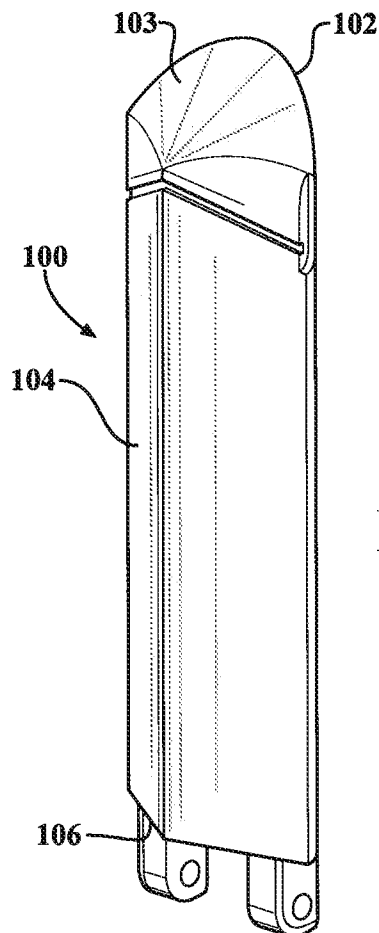


FIG. 1D

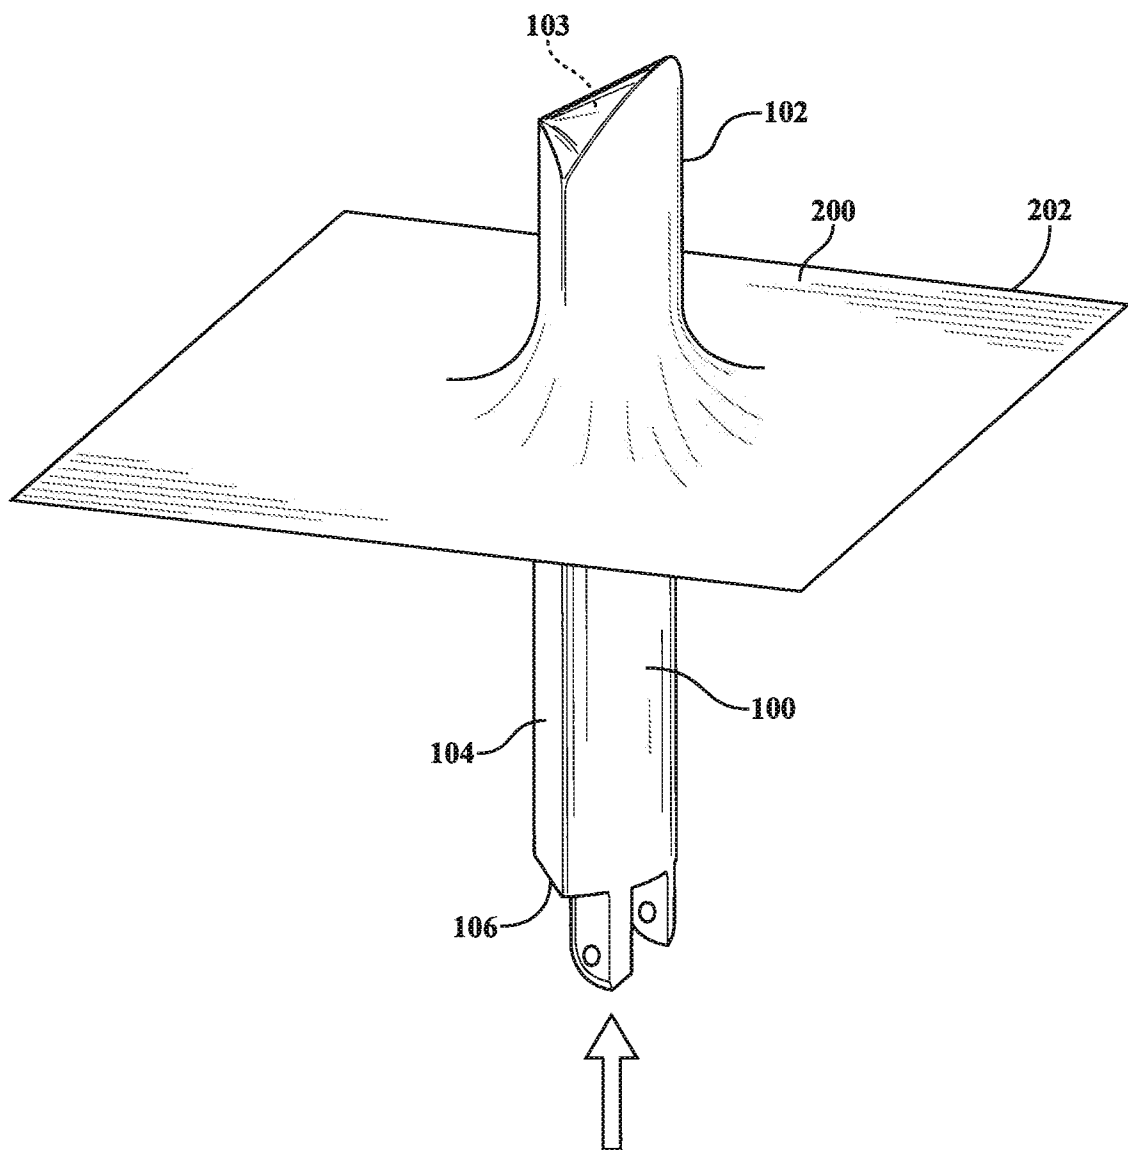


FIG. 2A

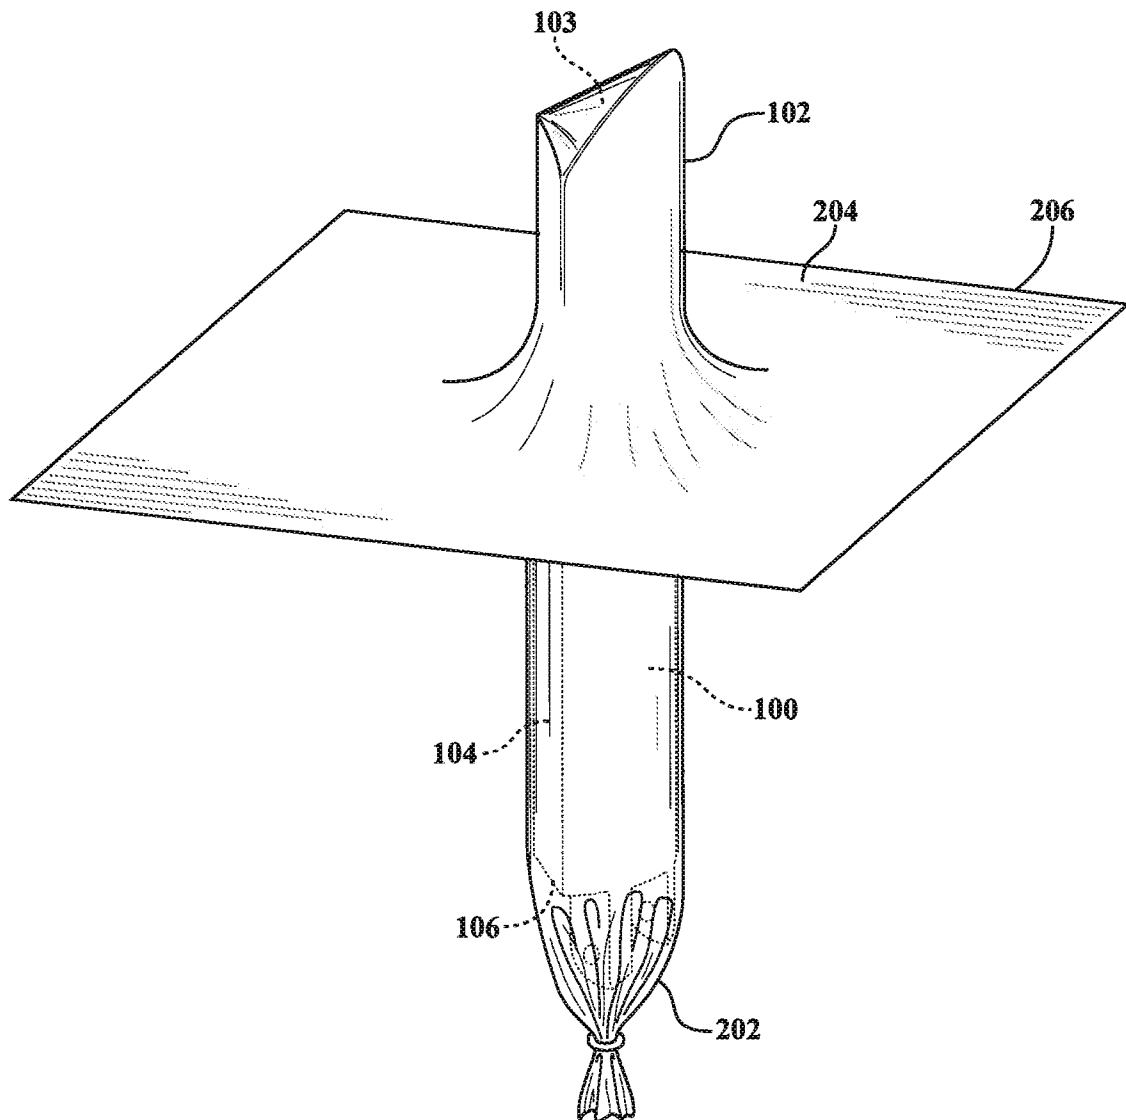
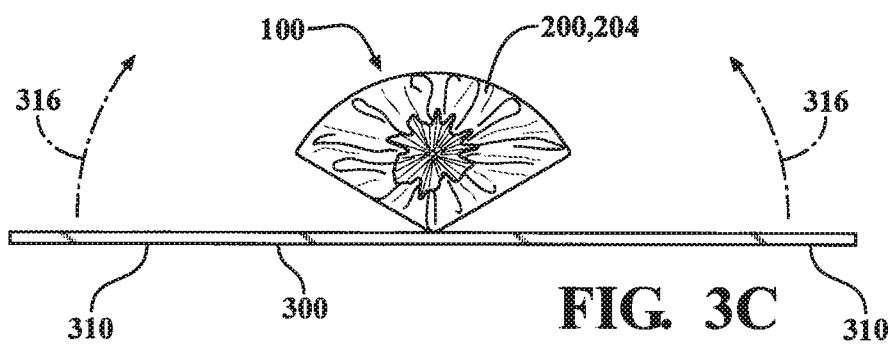
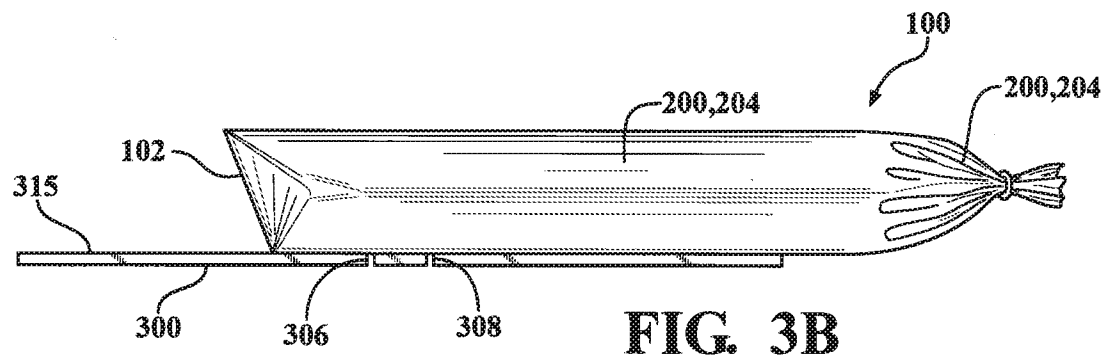
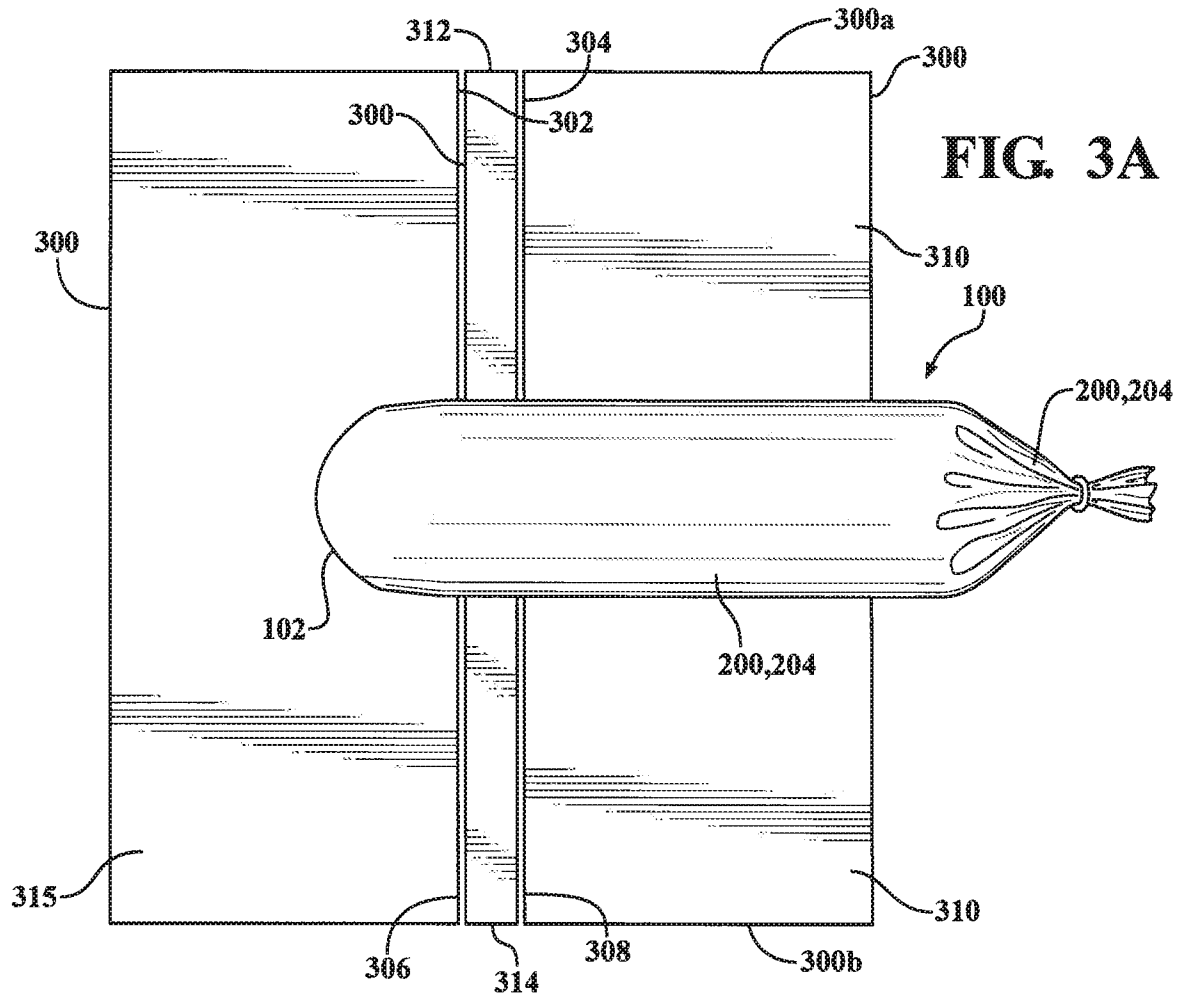
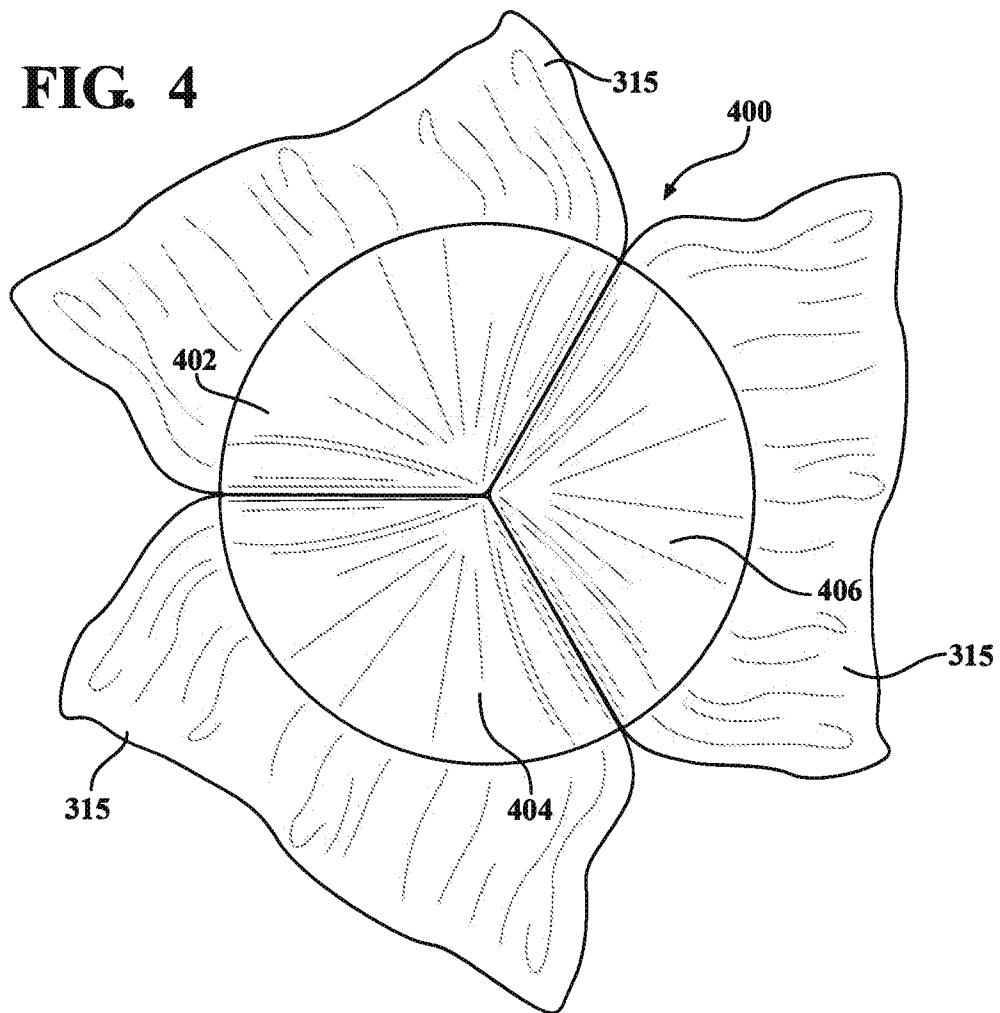


FIG. 2B





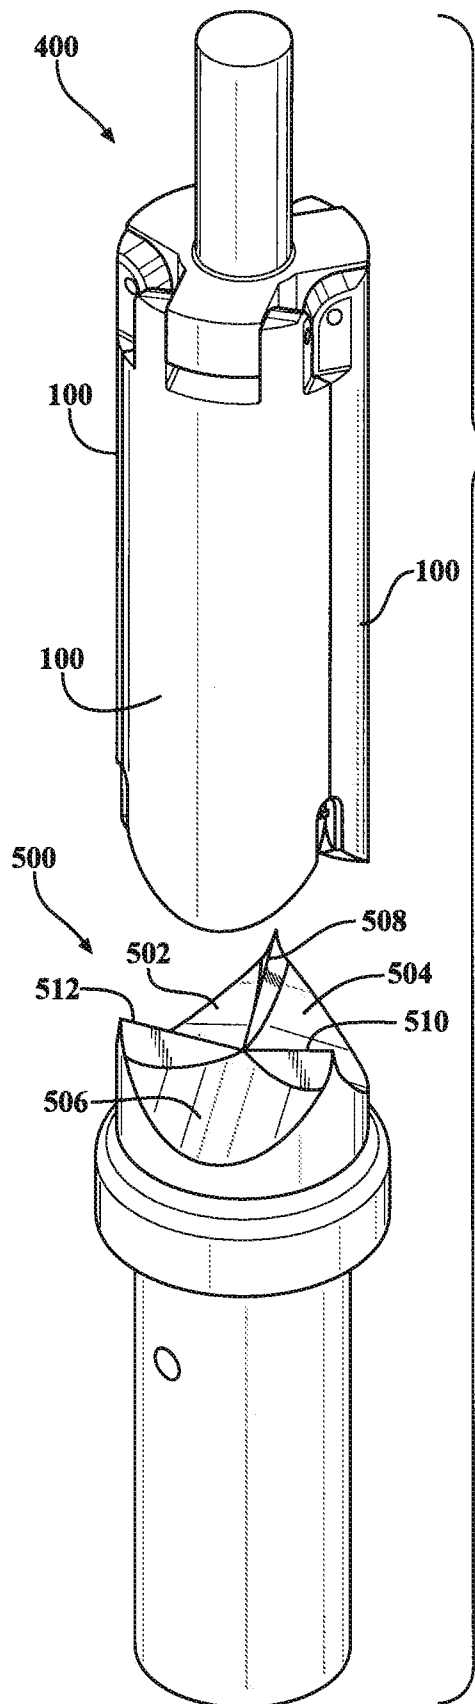


FIG. 5A

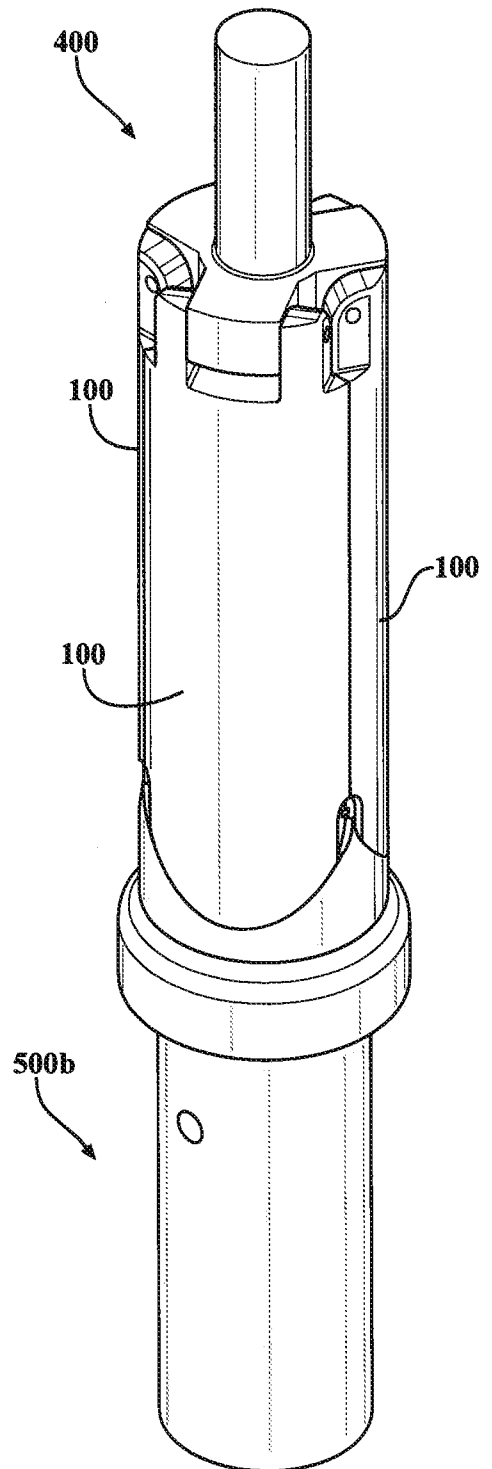


FIG. 5B

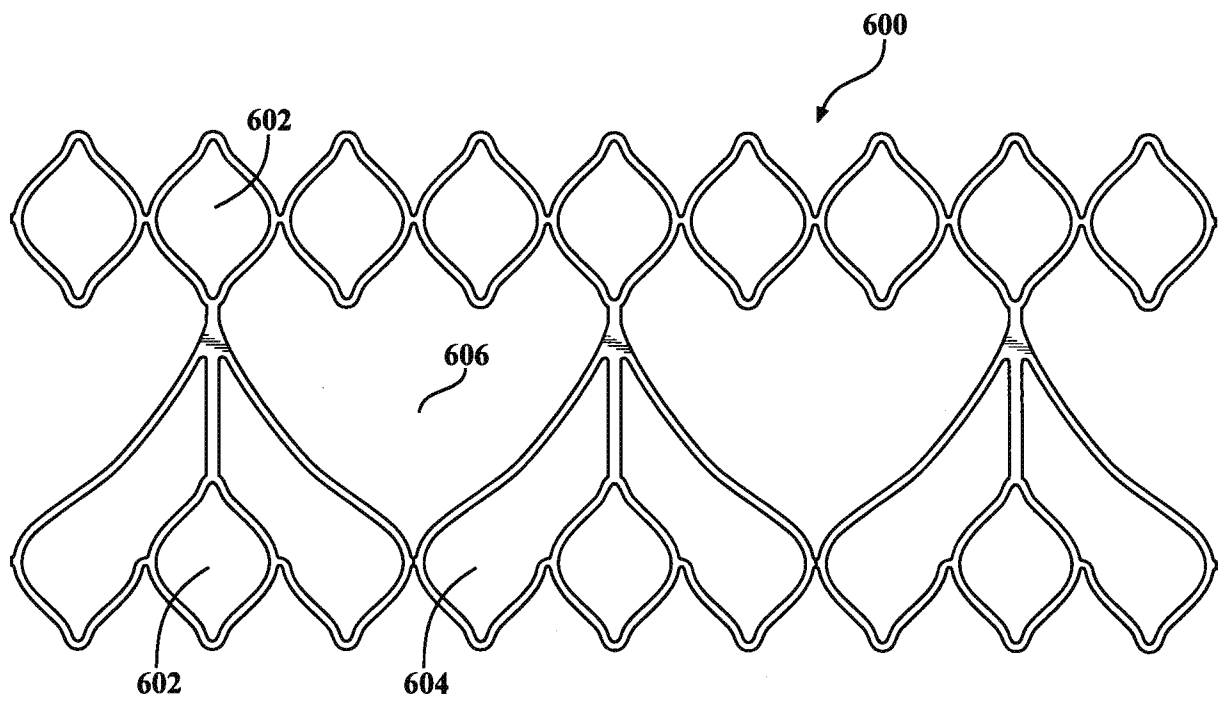


FIG. 6A

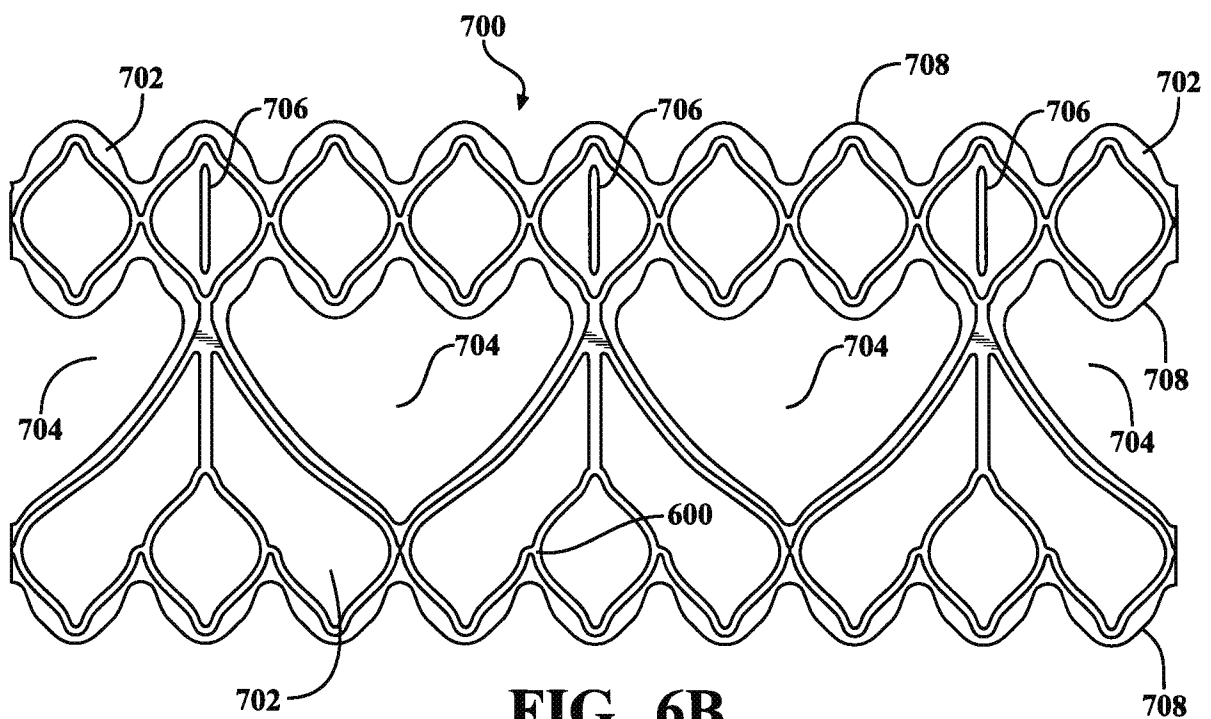


FIG. 6B

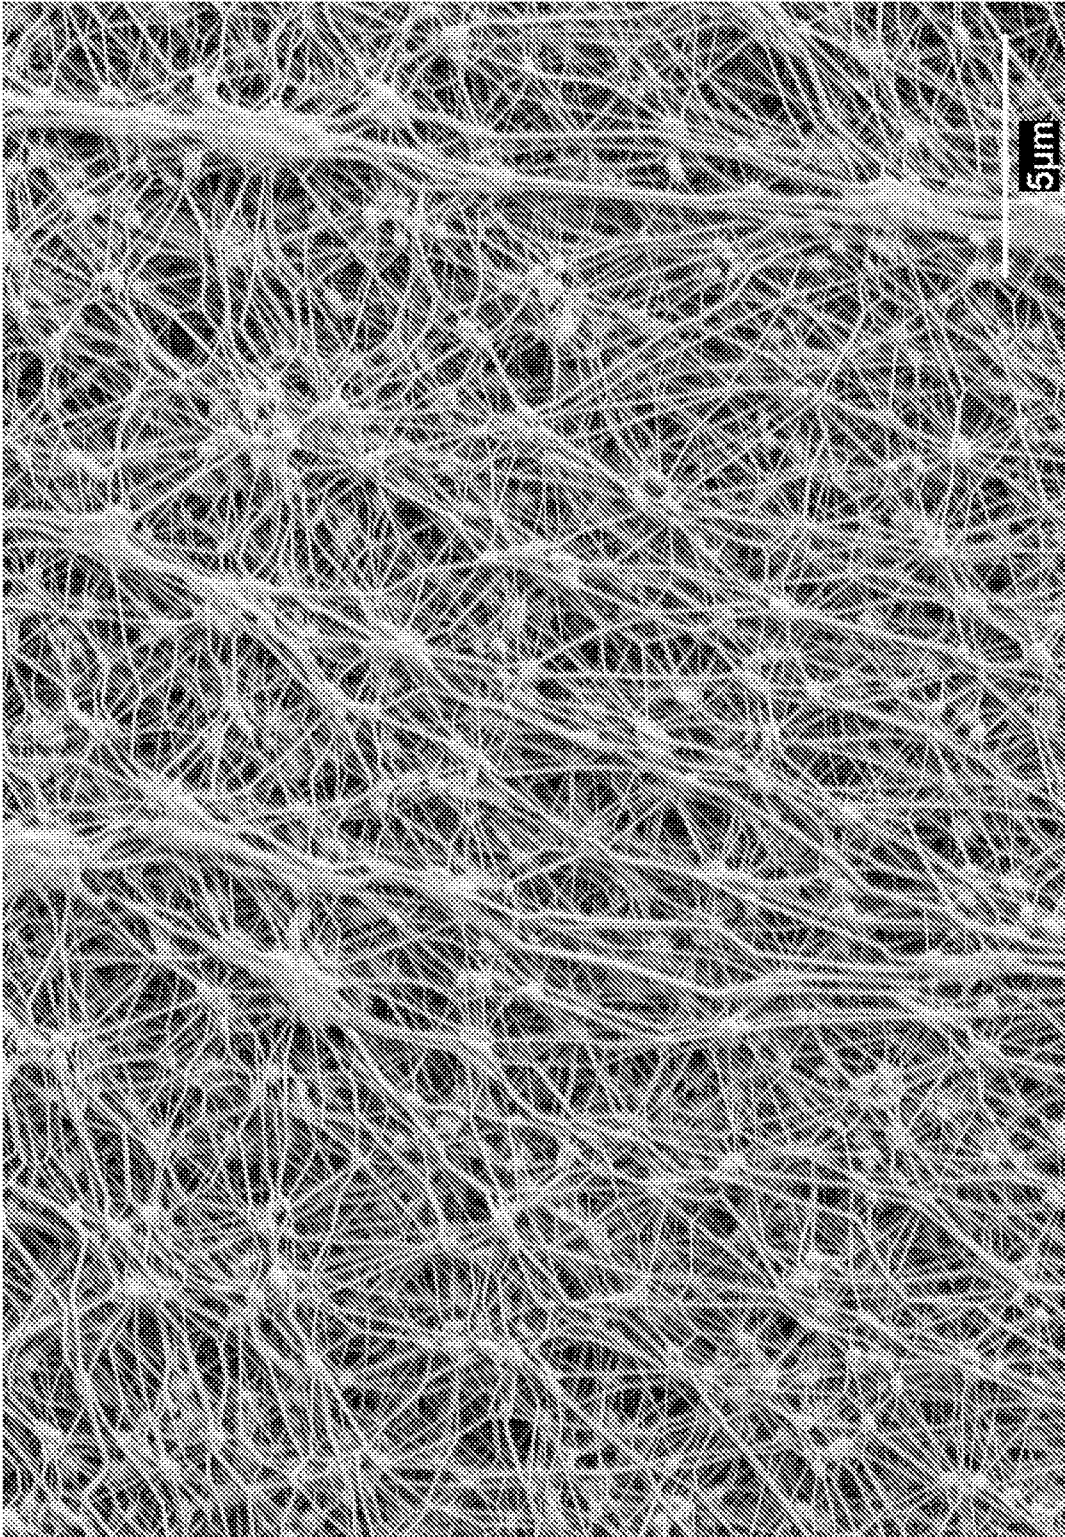


FIG. 7A

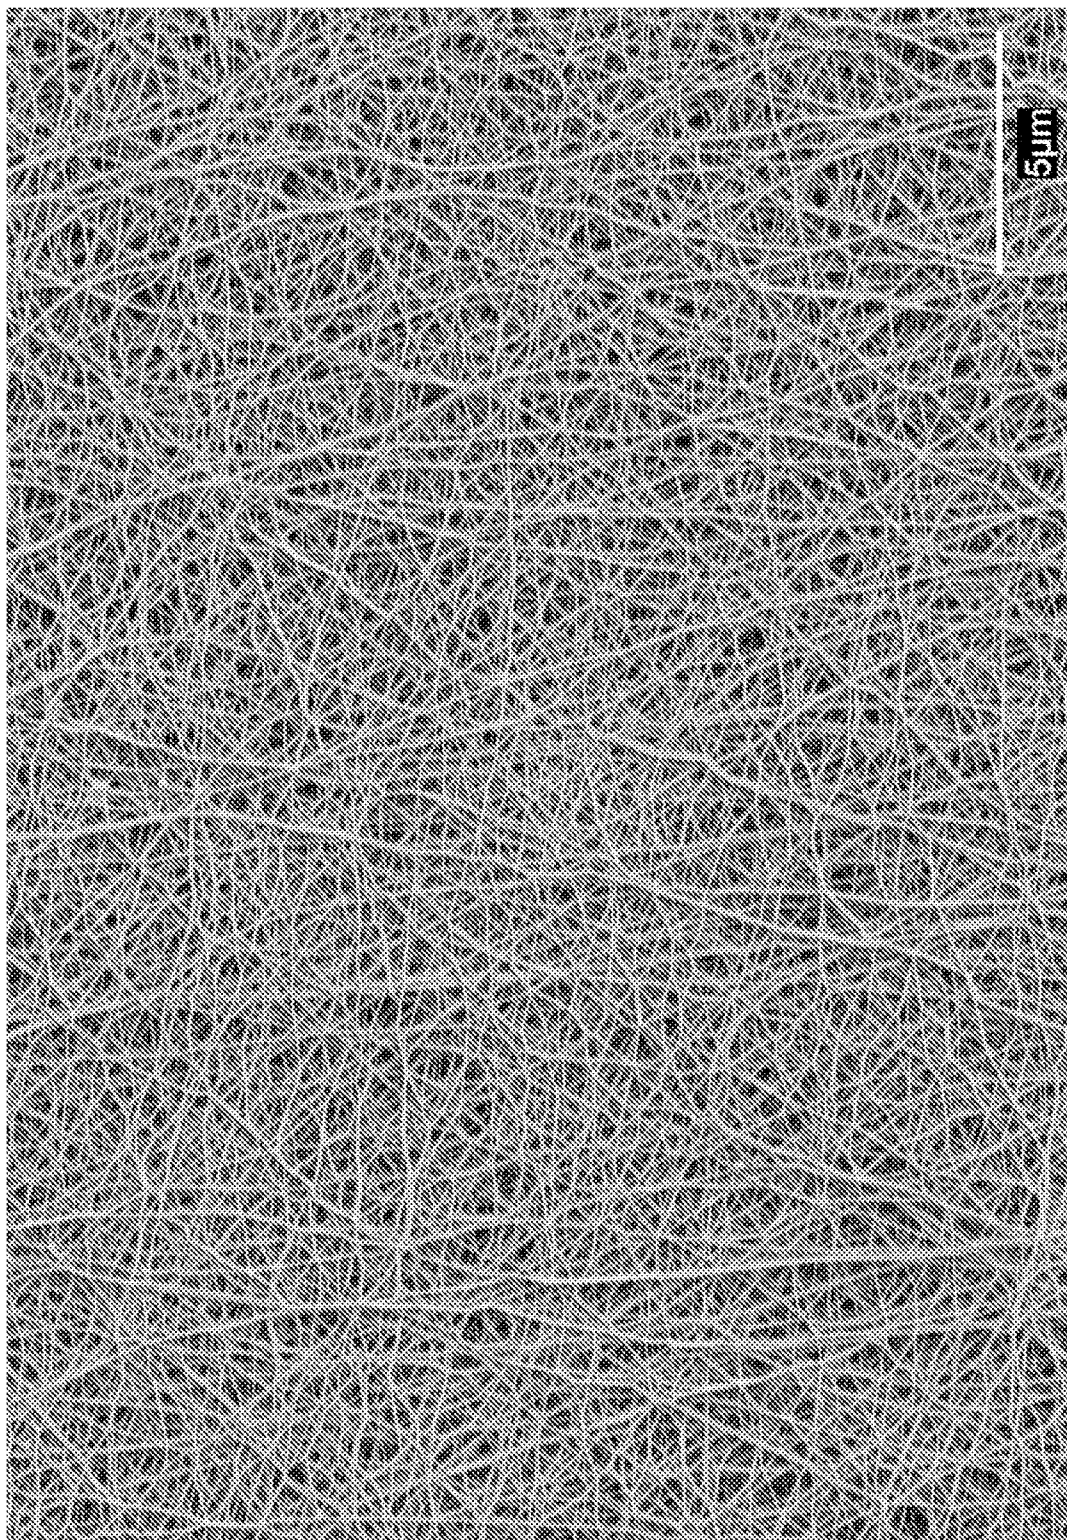


FIG. 7B

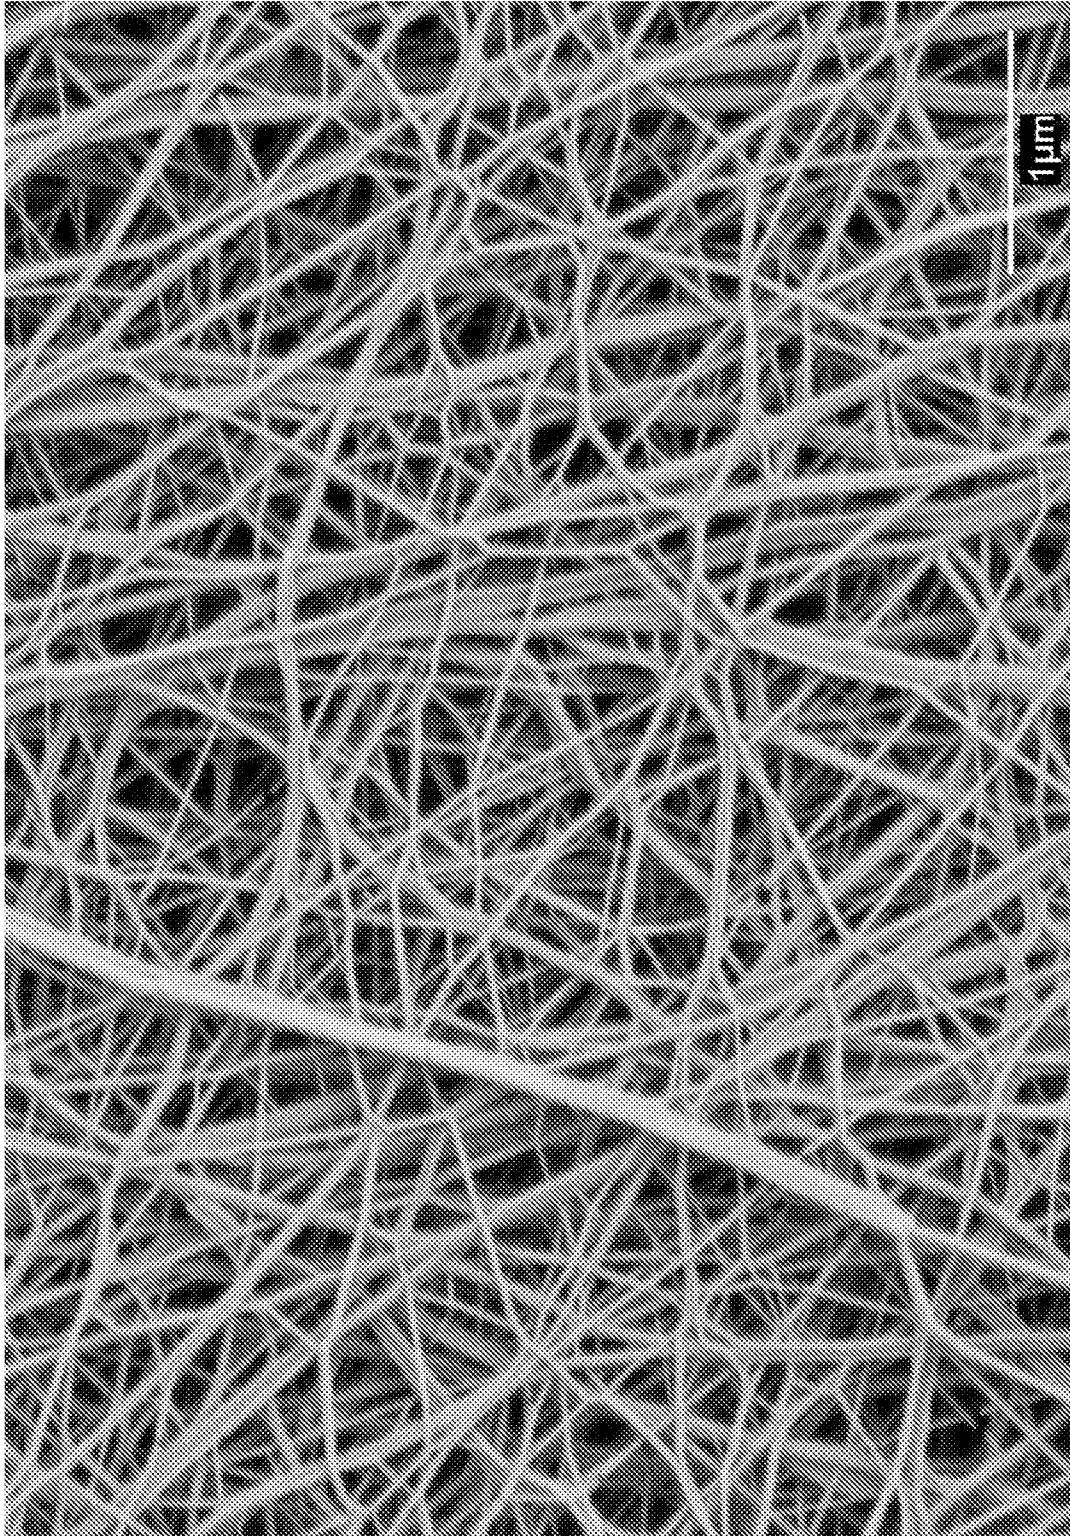


FIG. 7C

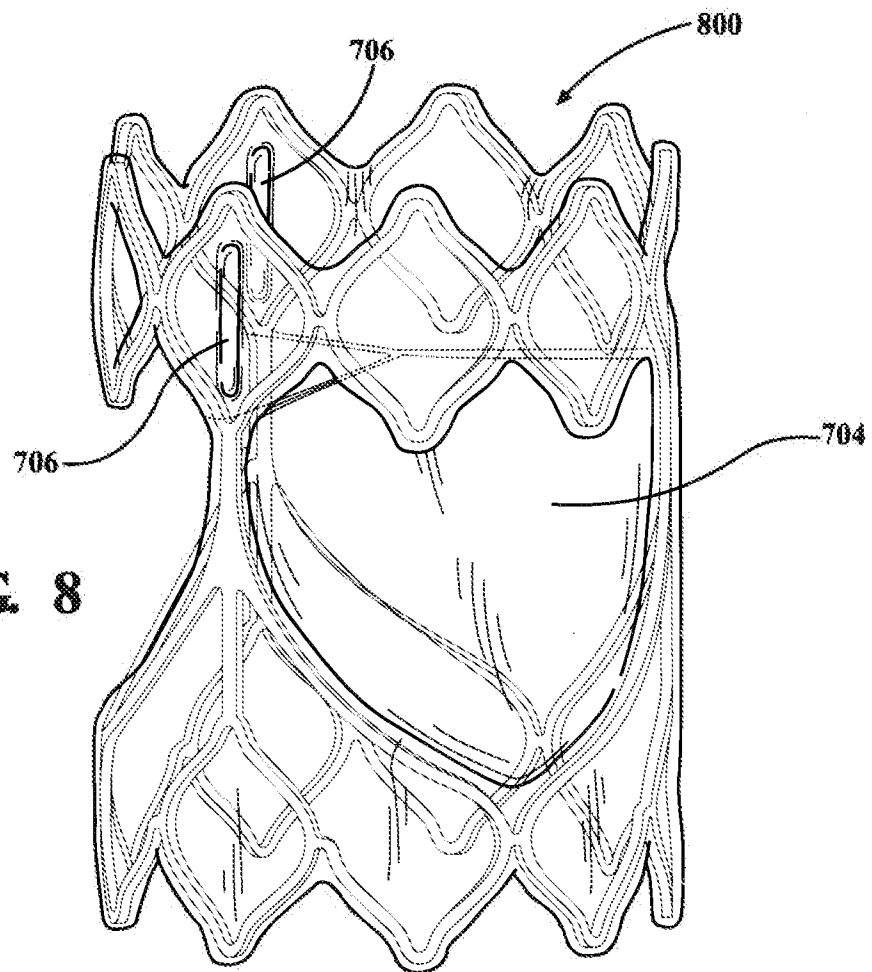


FIG. 8

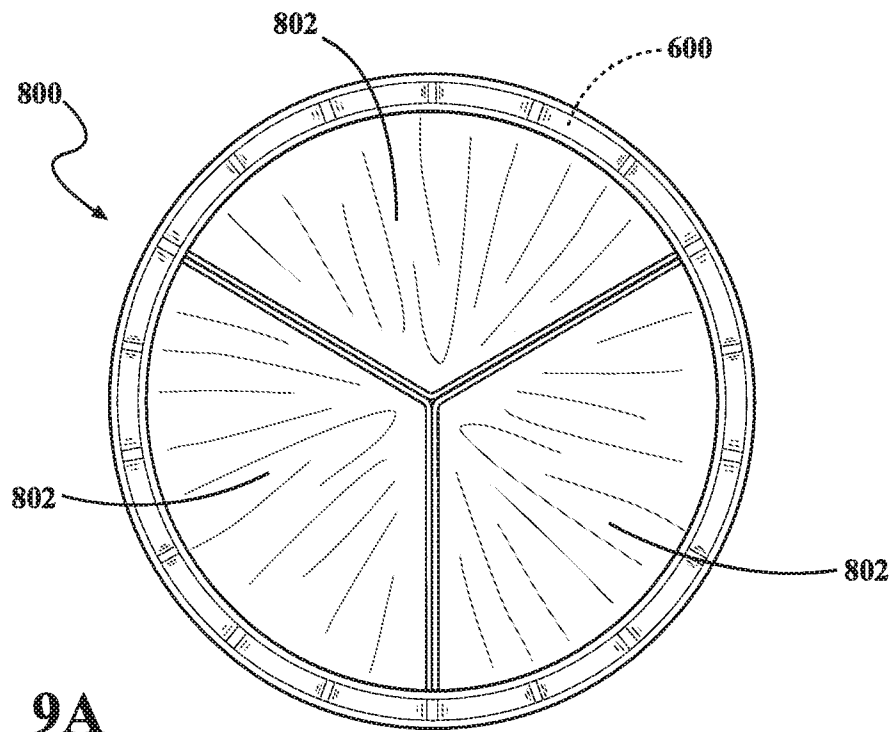


FIG. 9A

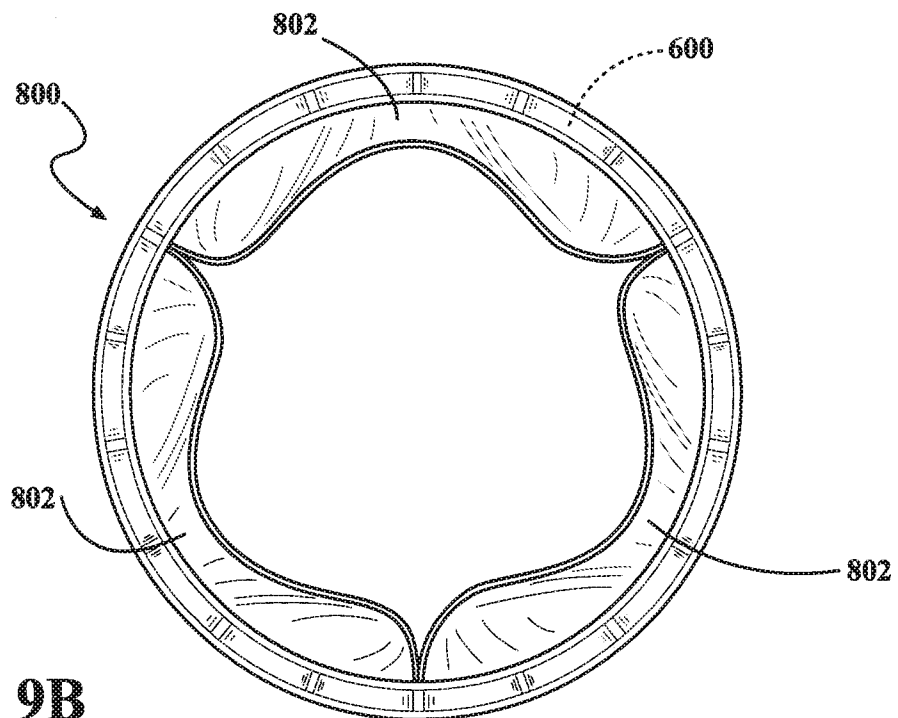


FIG. 9B

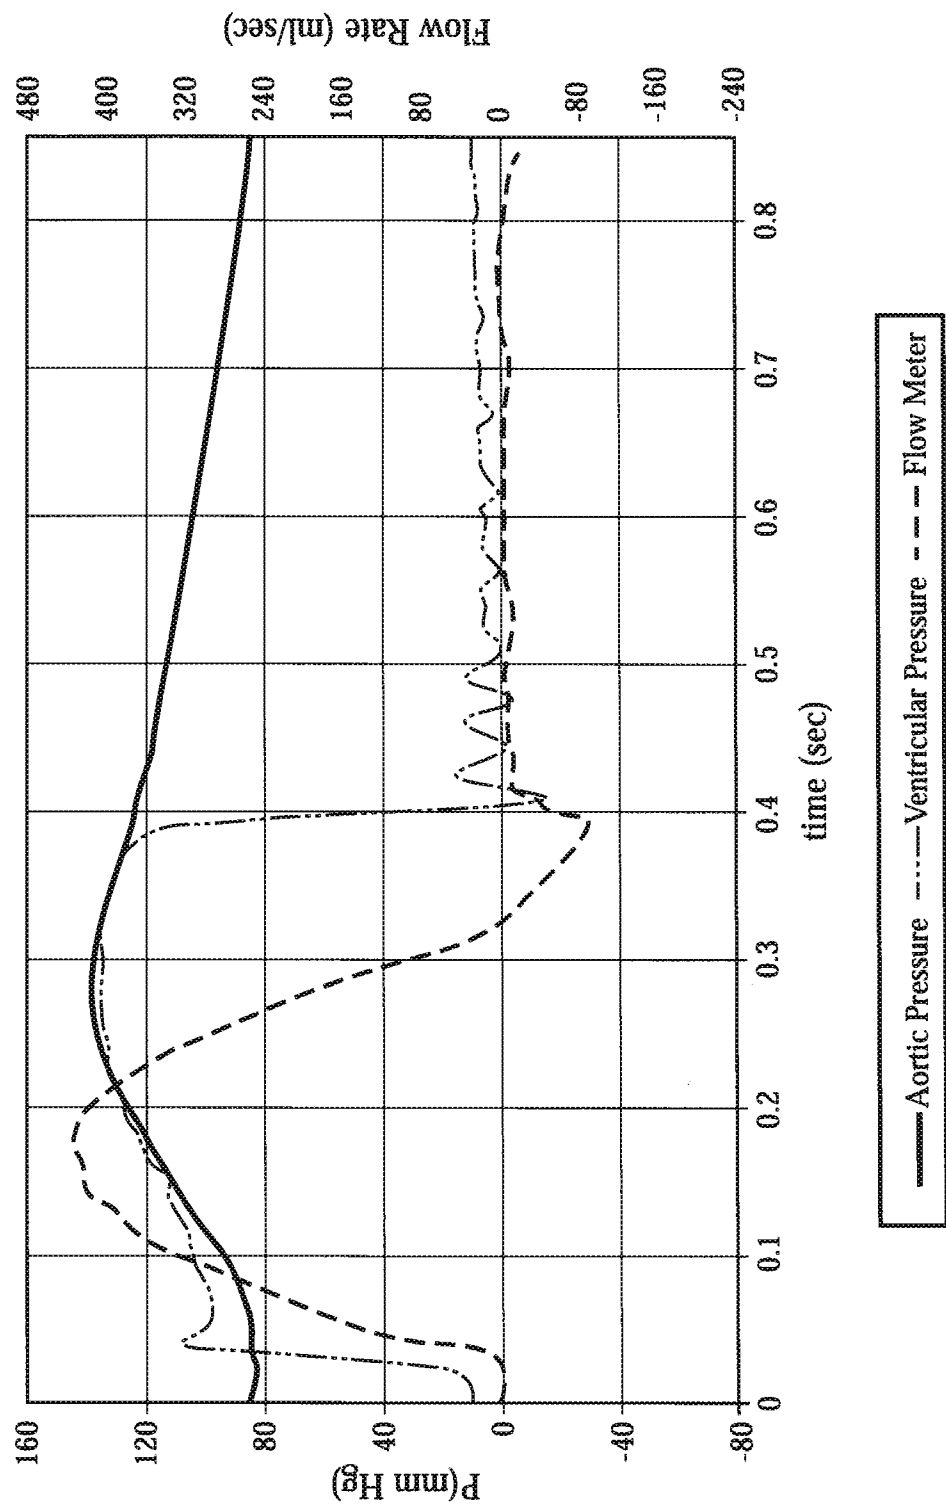


FIG. 10

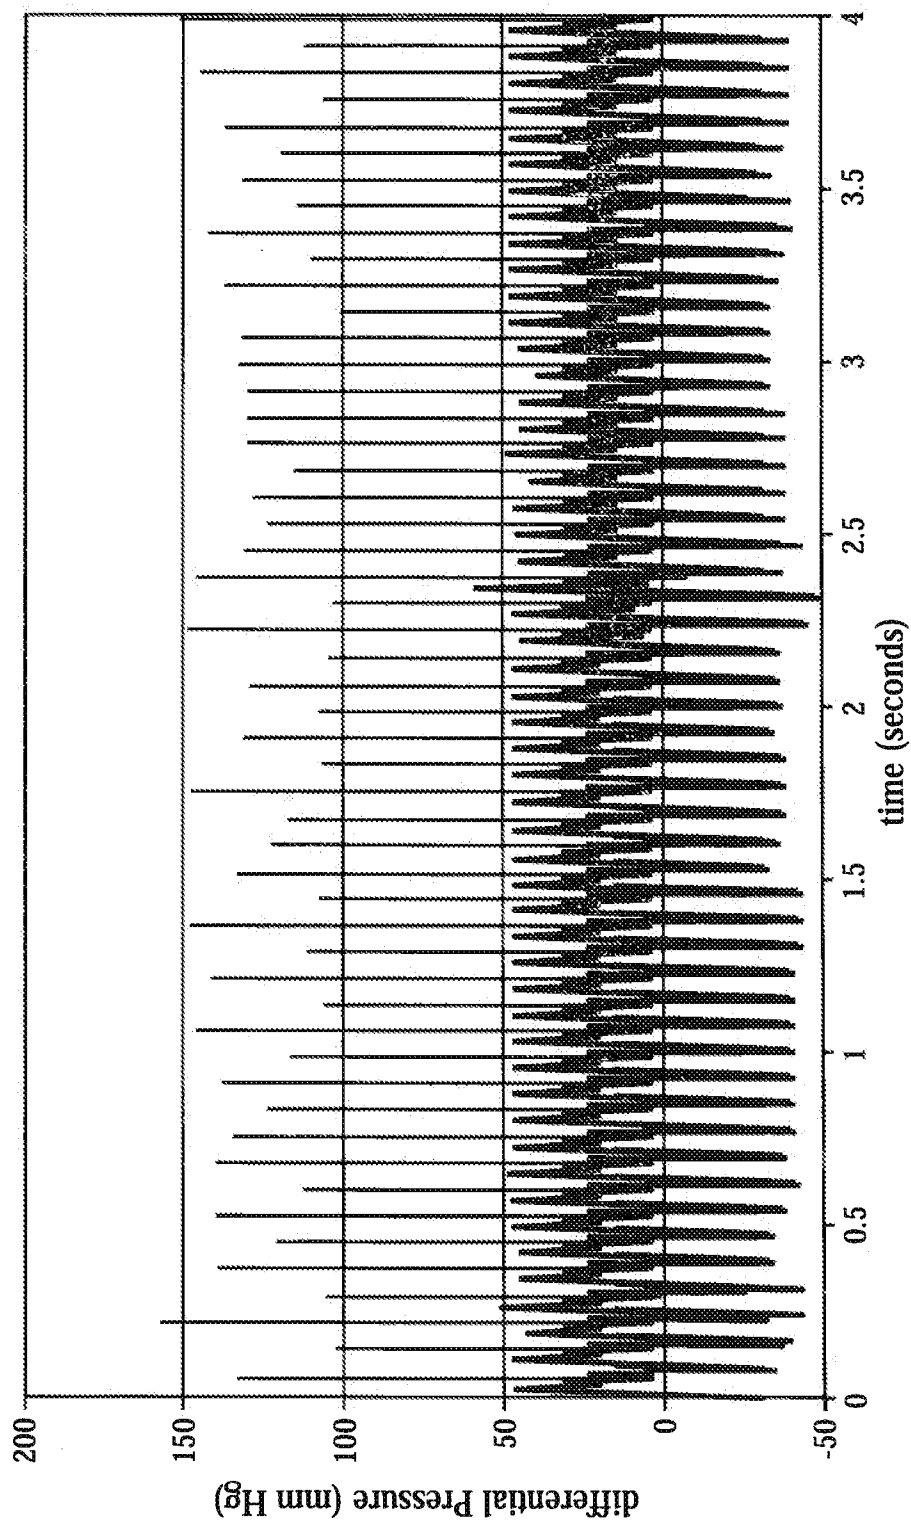
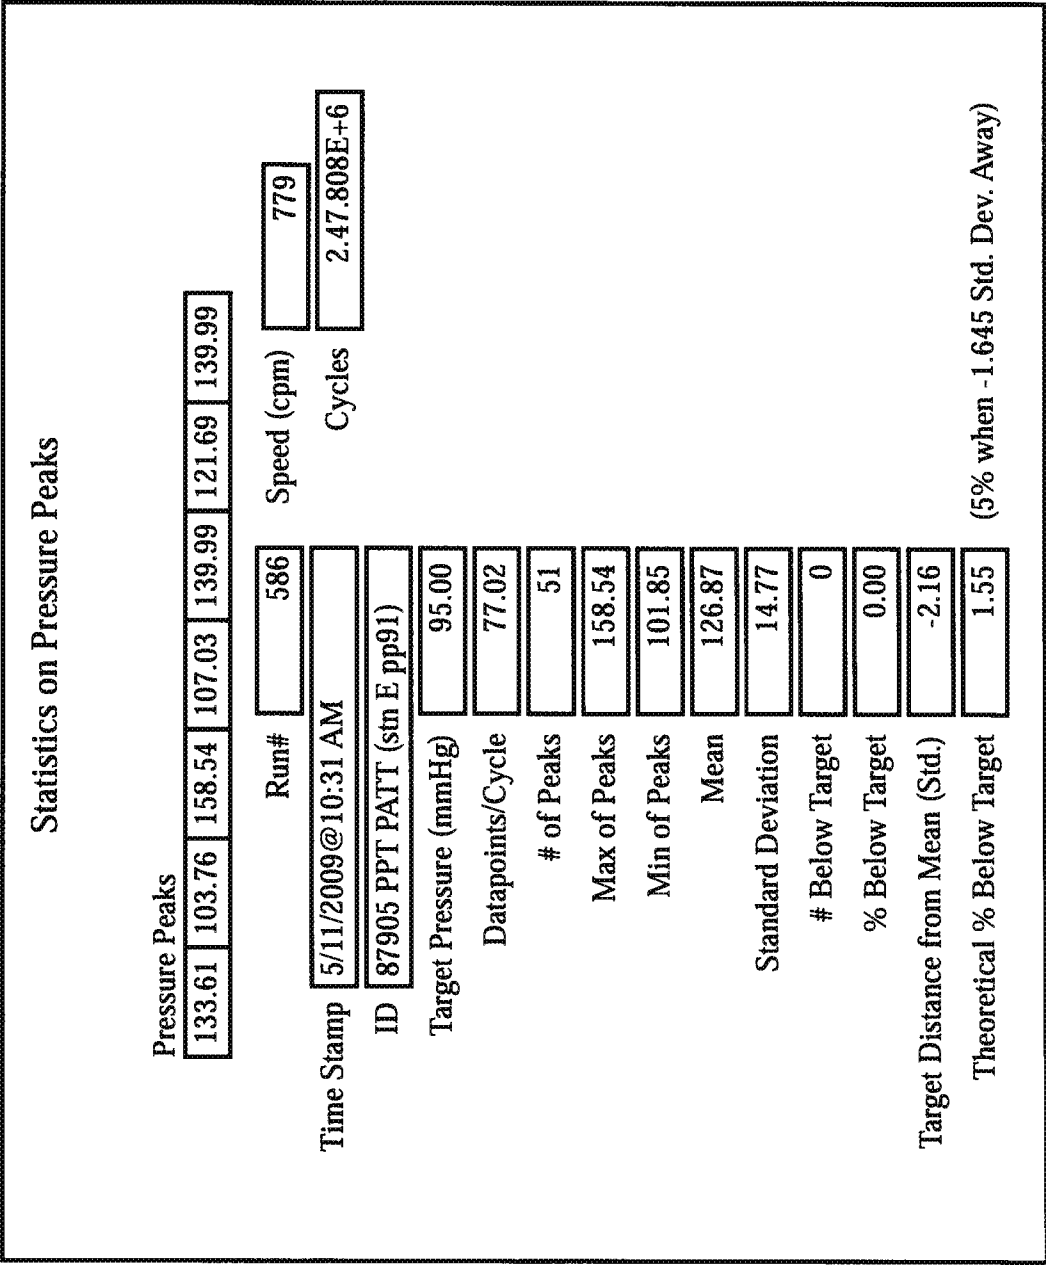


FIG. 11A

FIG. 11B



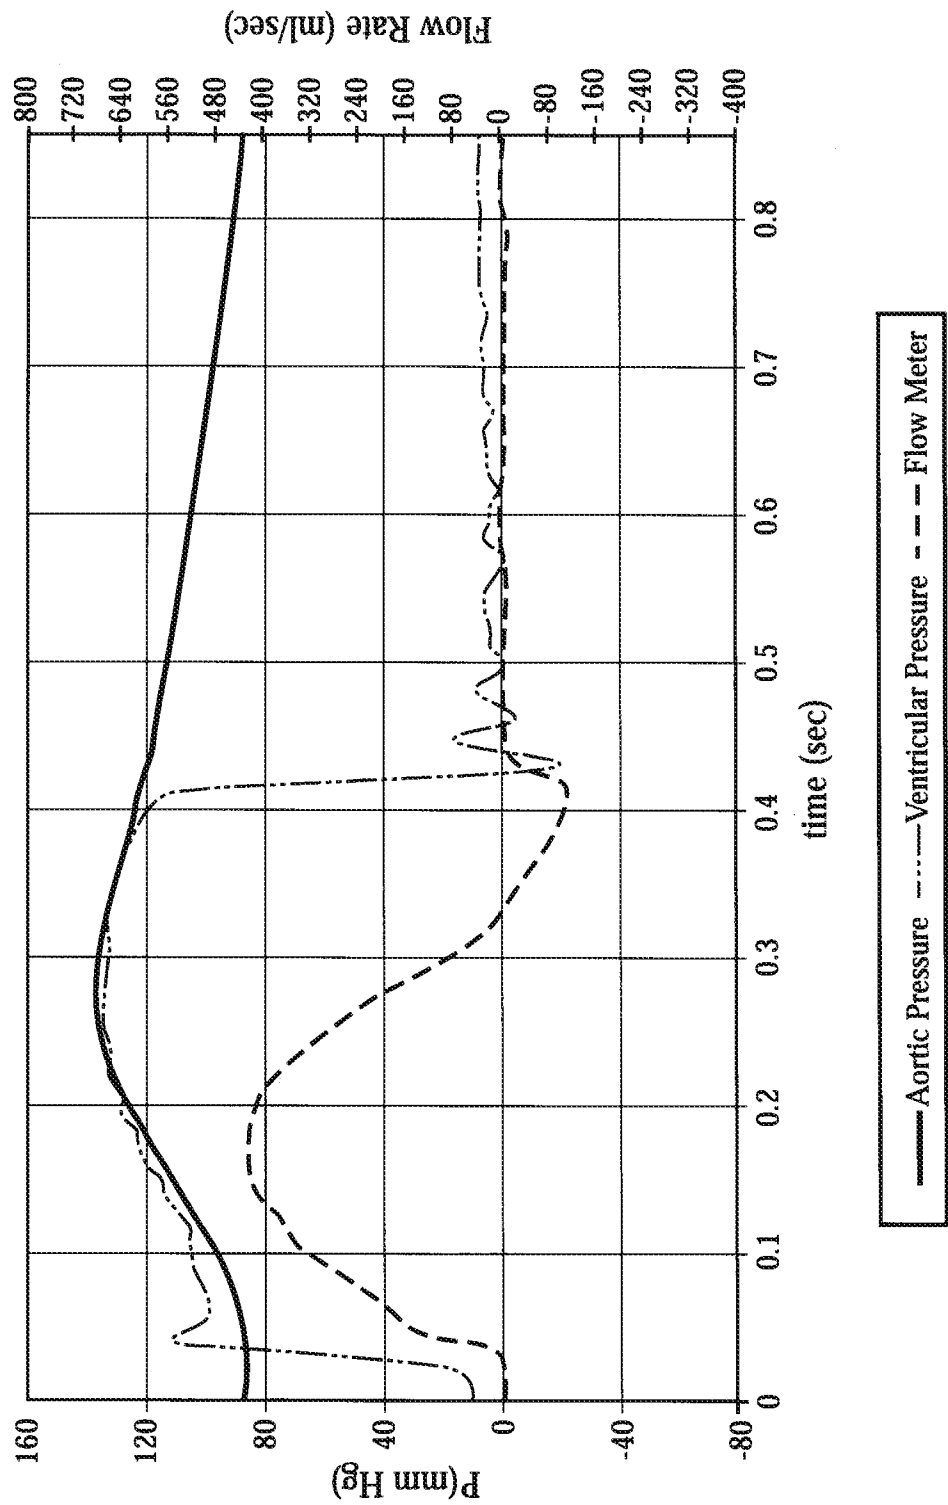


FIG. 12A

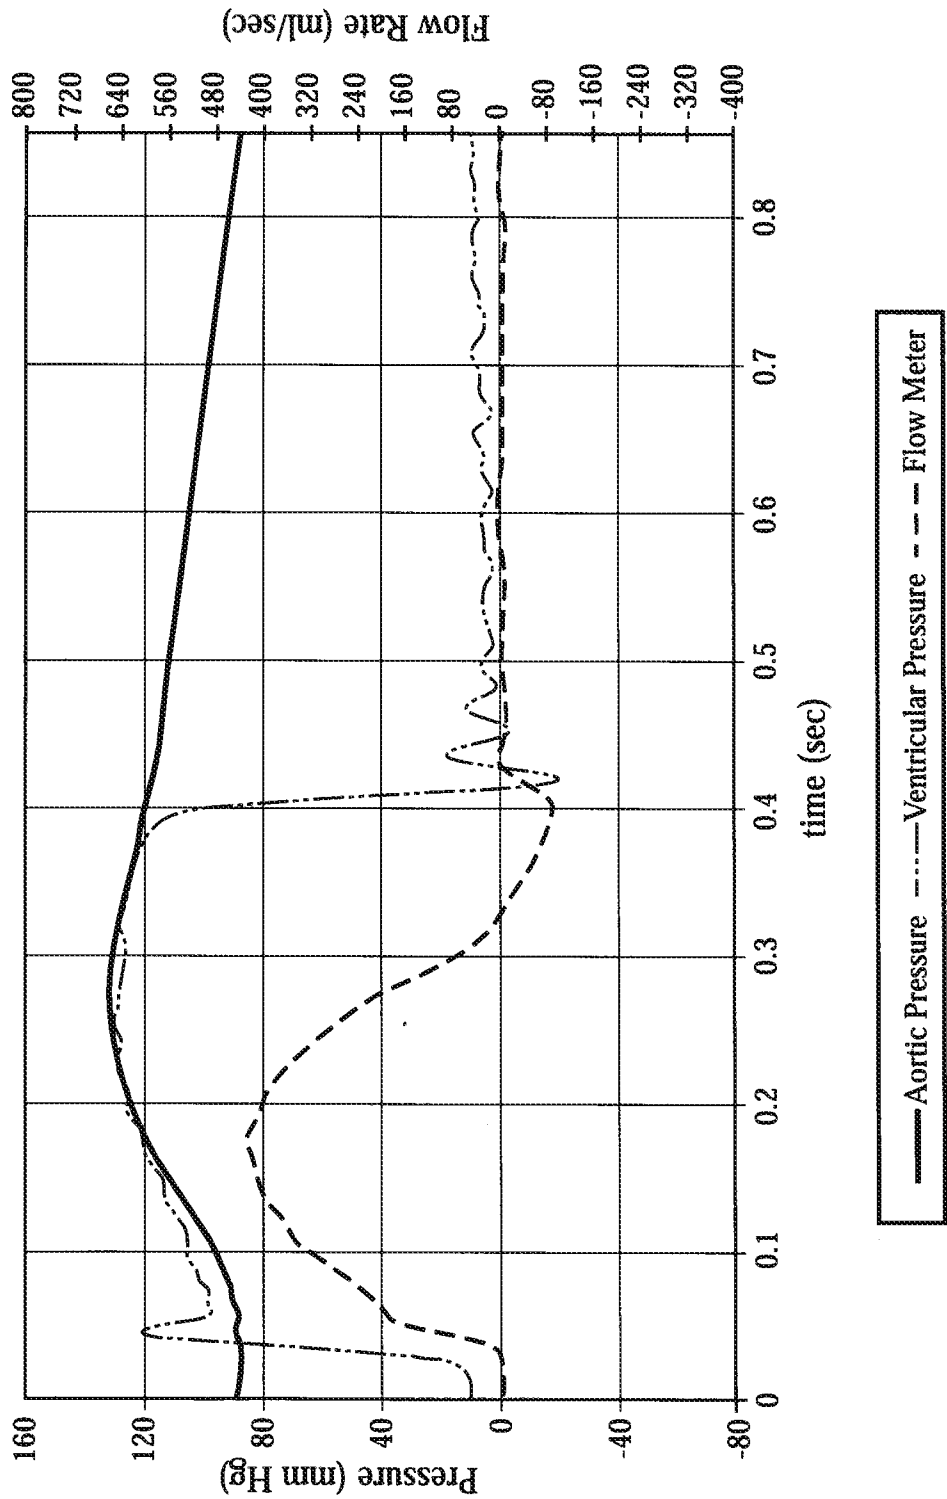


FIG. 12B


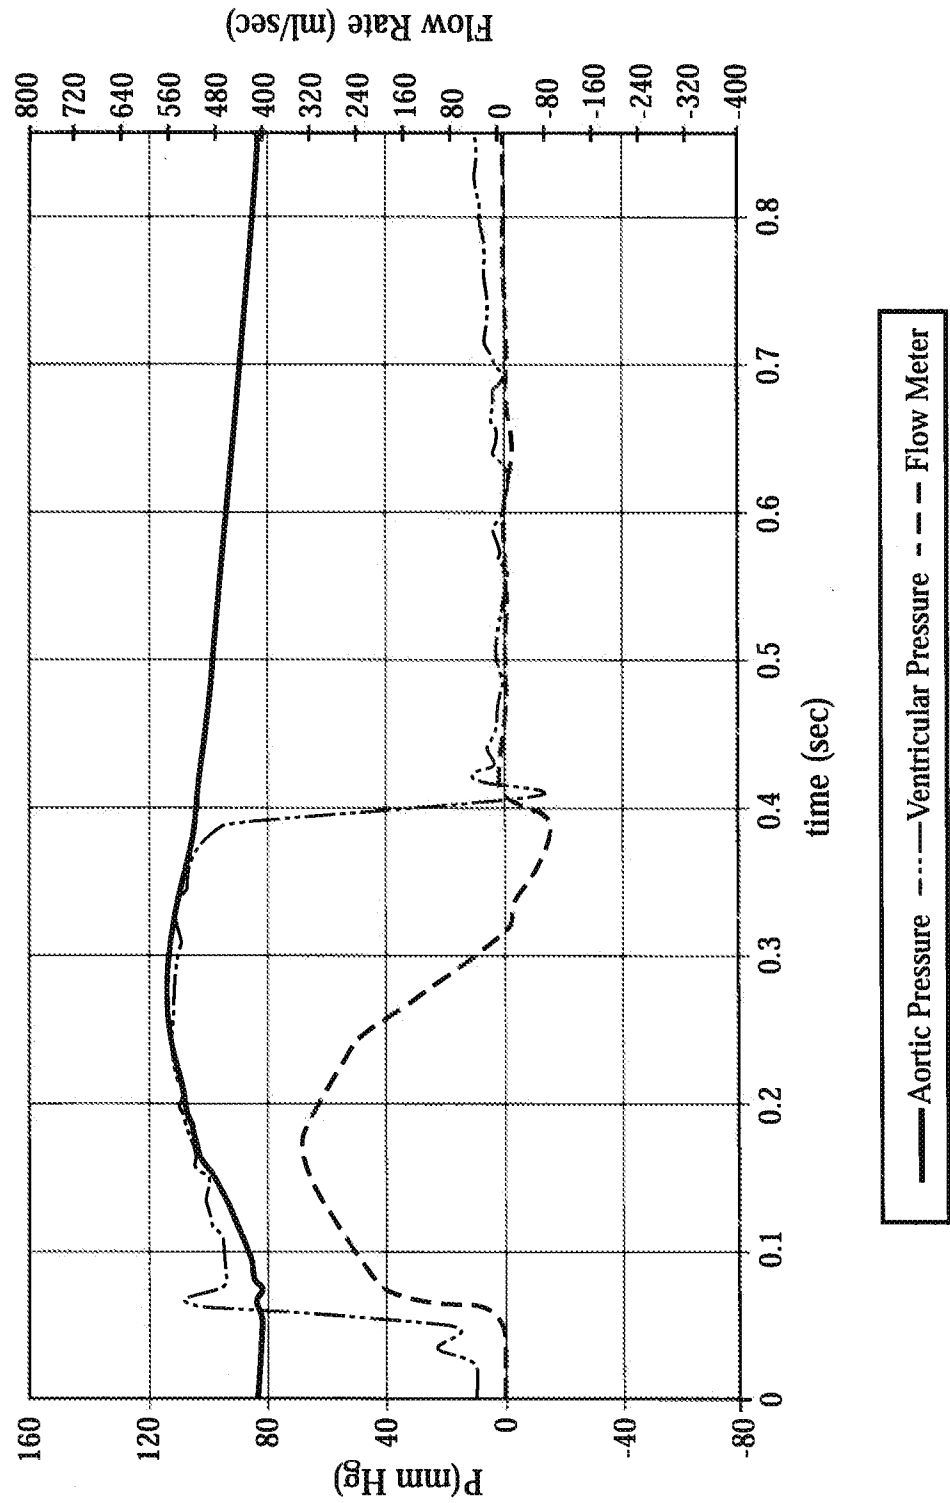


FIG. 13A

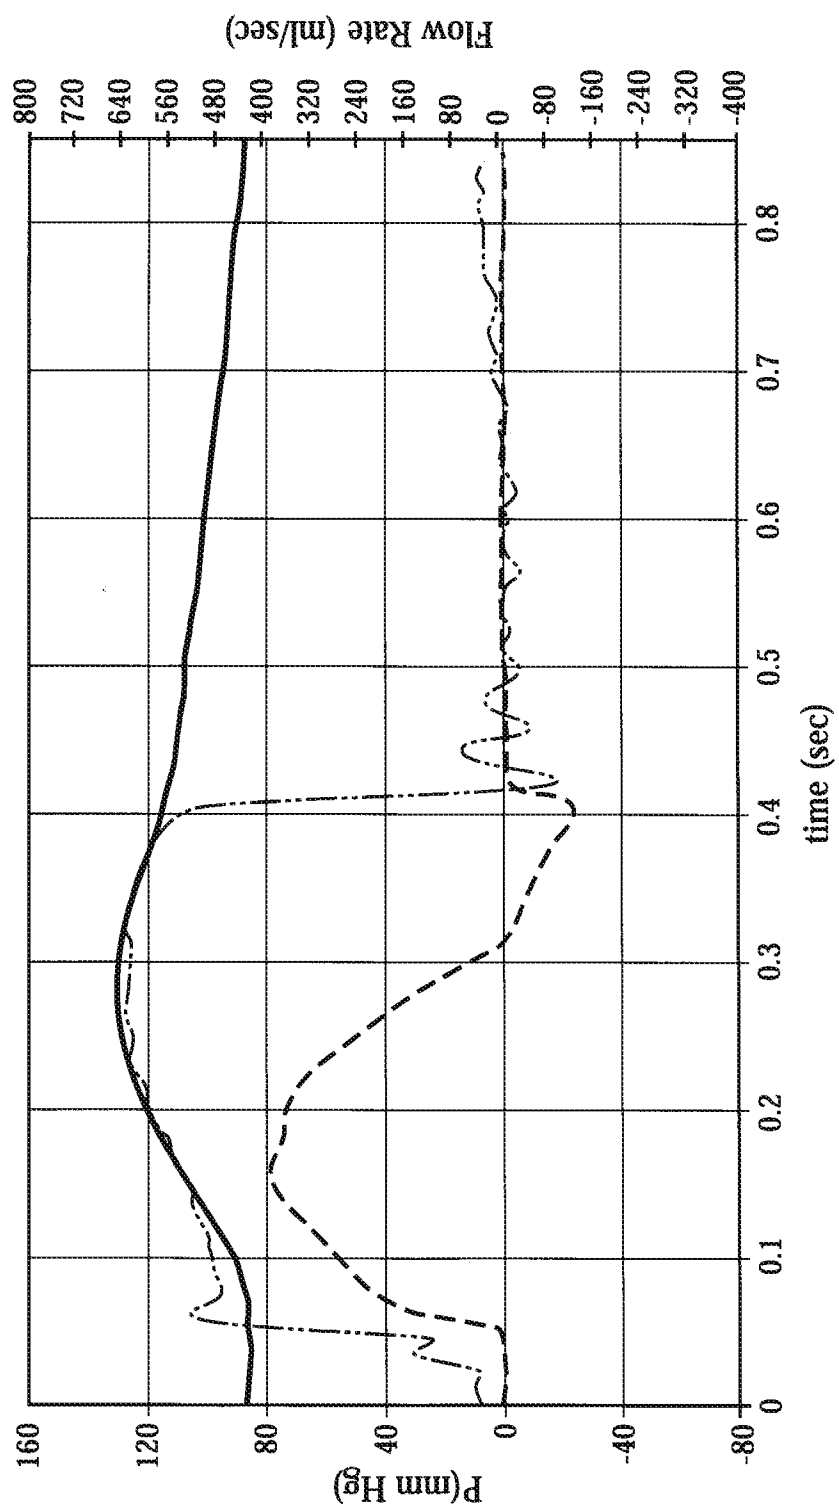

— Aortic Pressure Ventricular Pressure - - - Flow Meter

FIG. 13B

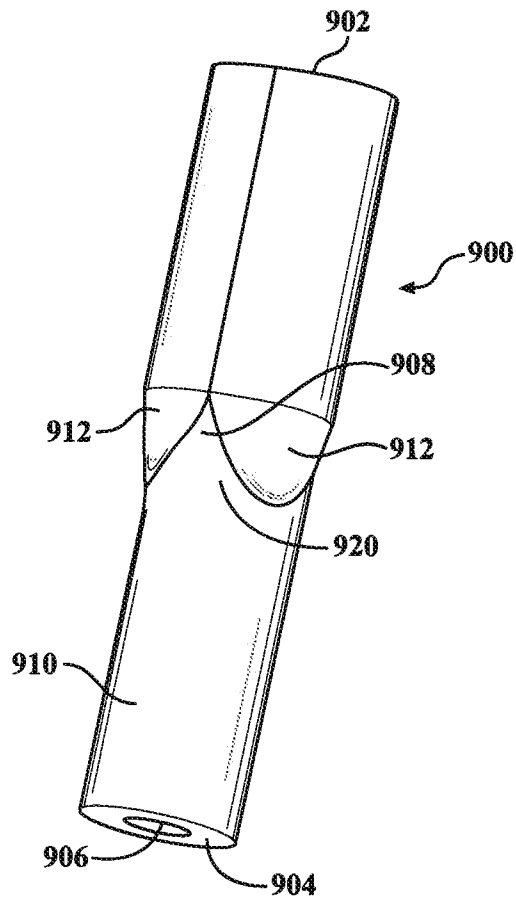


FIG. 14

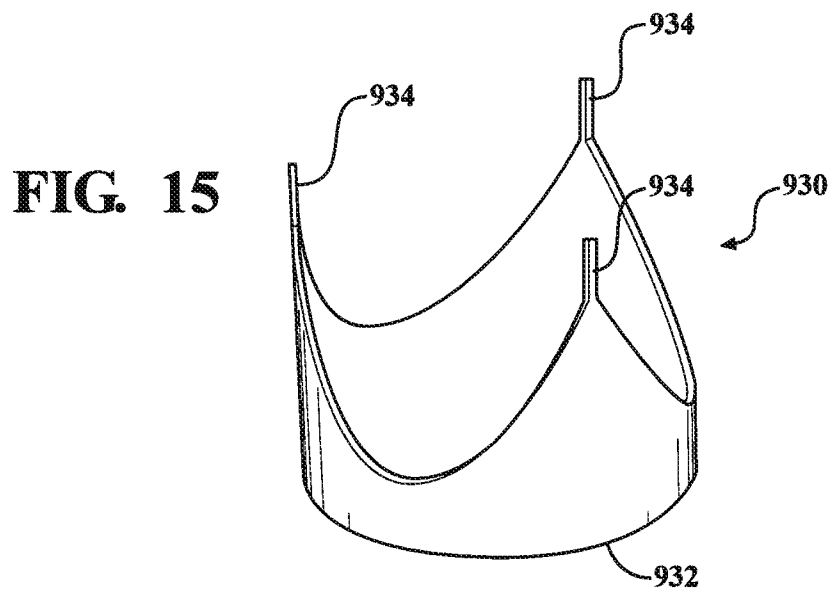


FIG. 15

FIG. 16

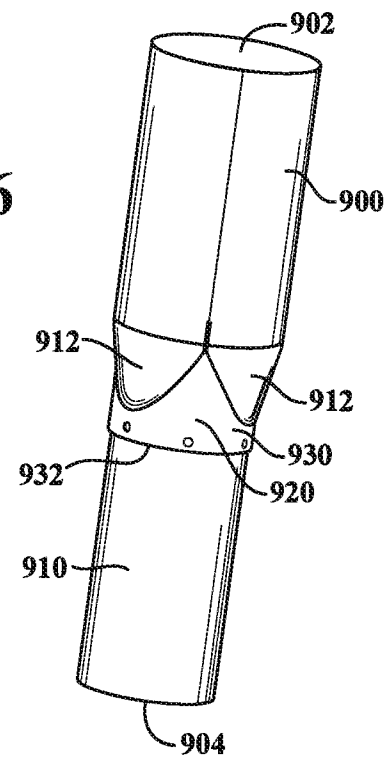


FIG. 17

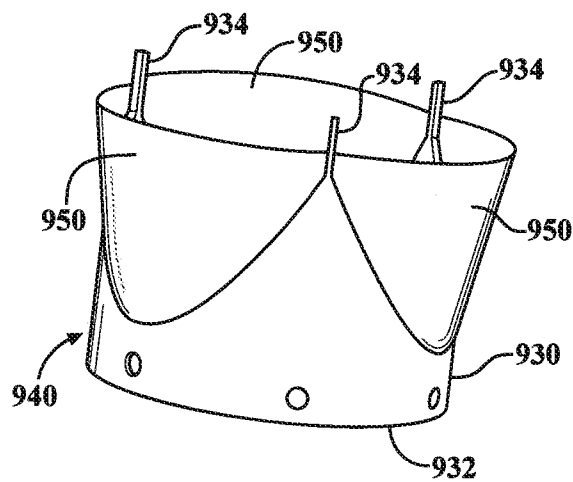


FIG. 18

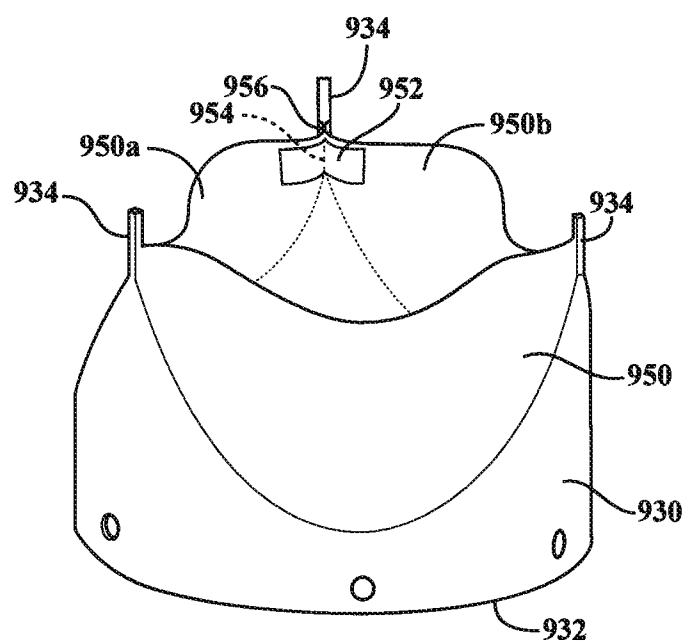


FIG. 19

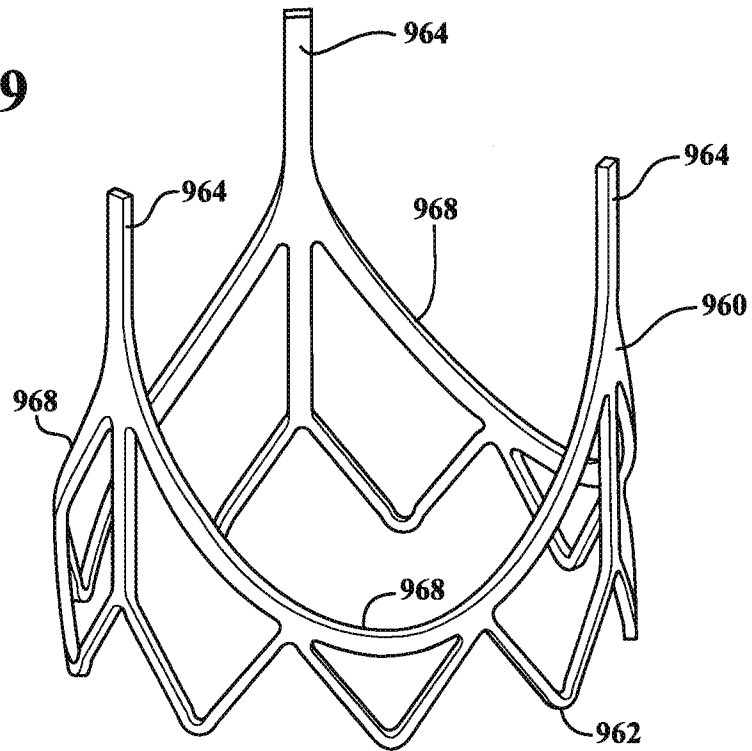


FIG. 20

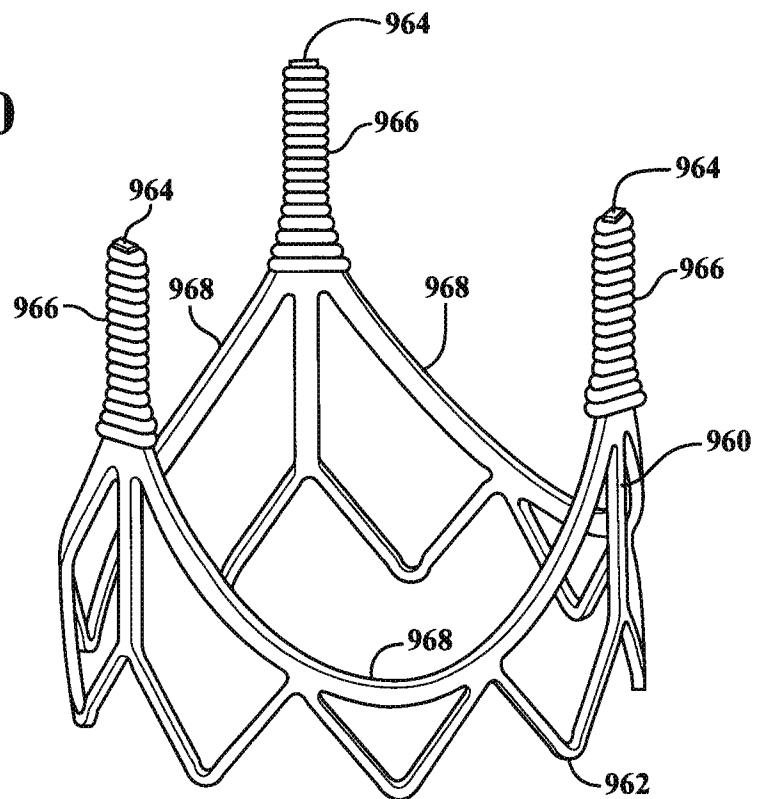


FIG. 21

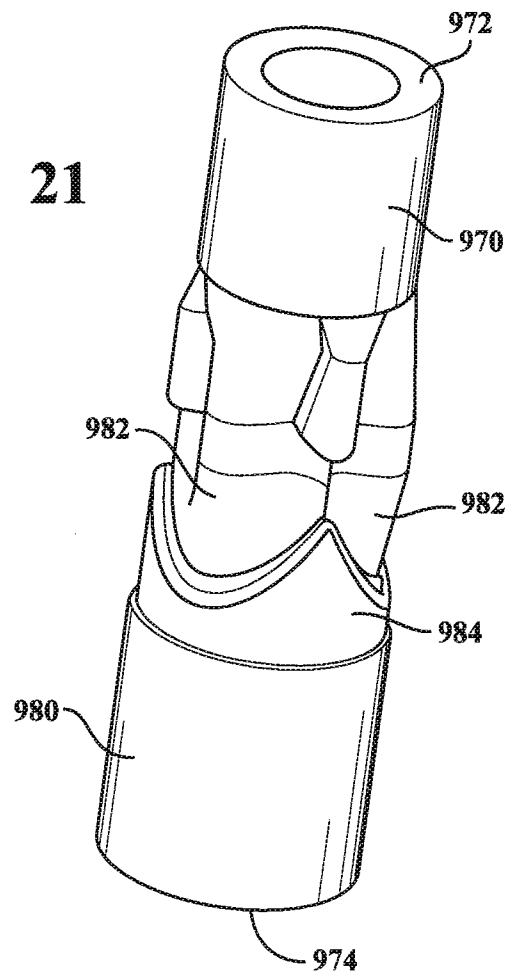
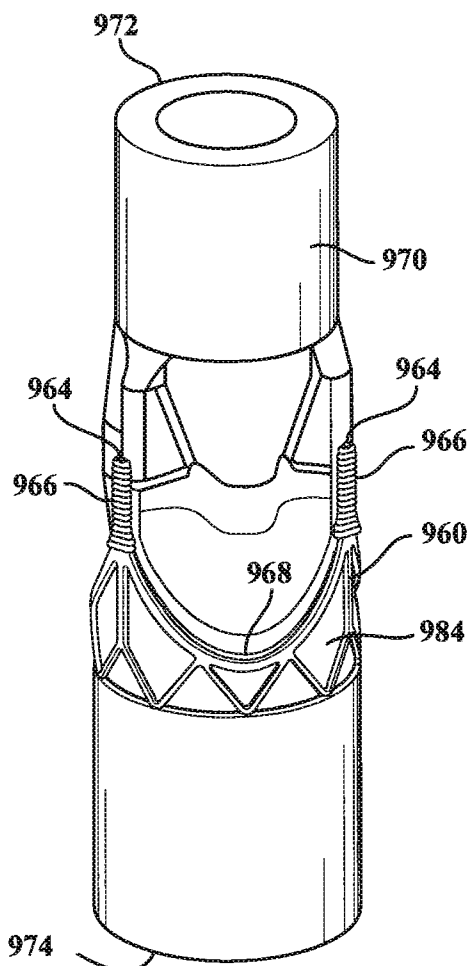


FIG. 22



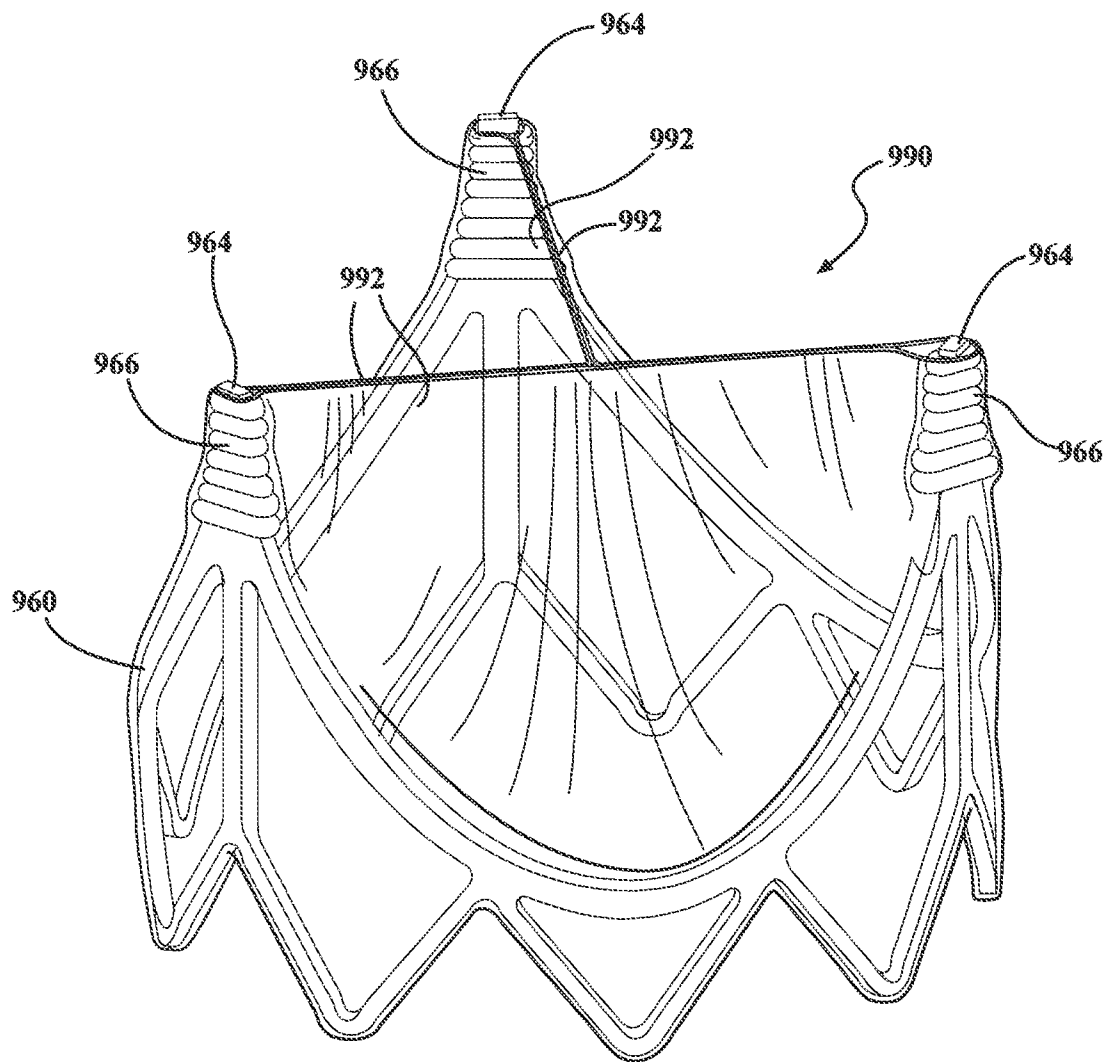


FIG. 23

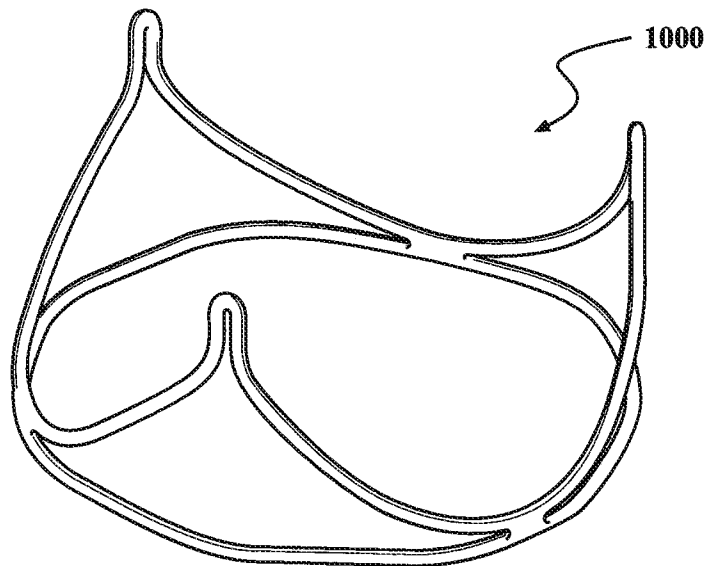


FIG. 24

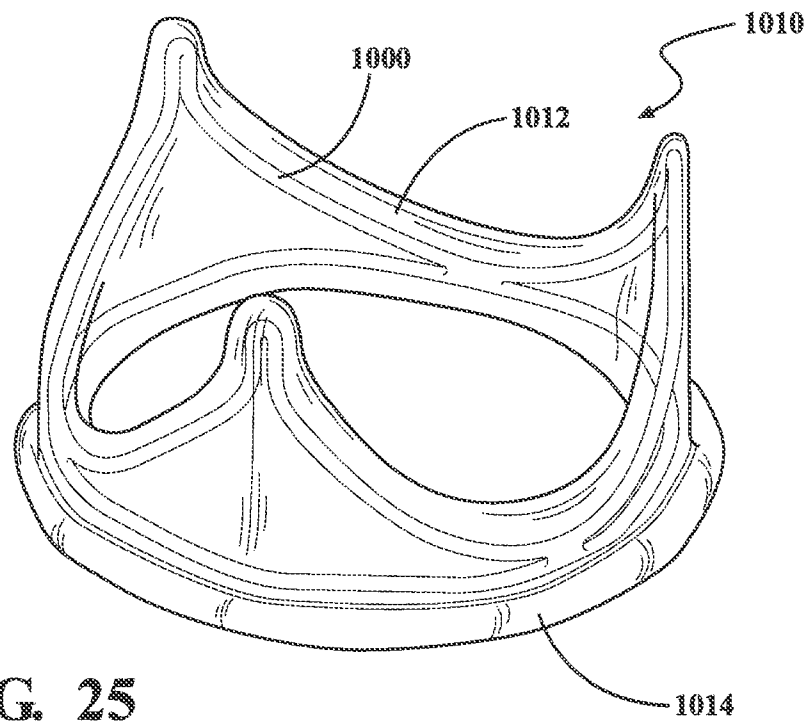


FIG. 25

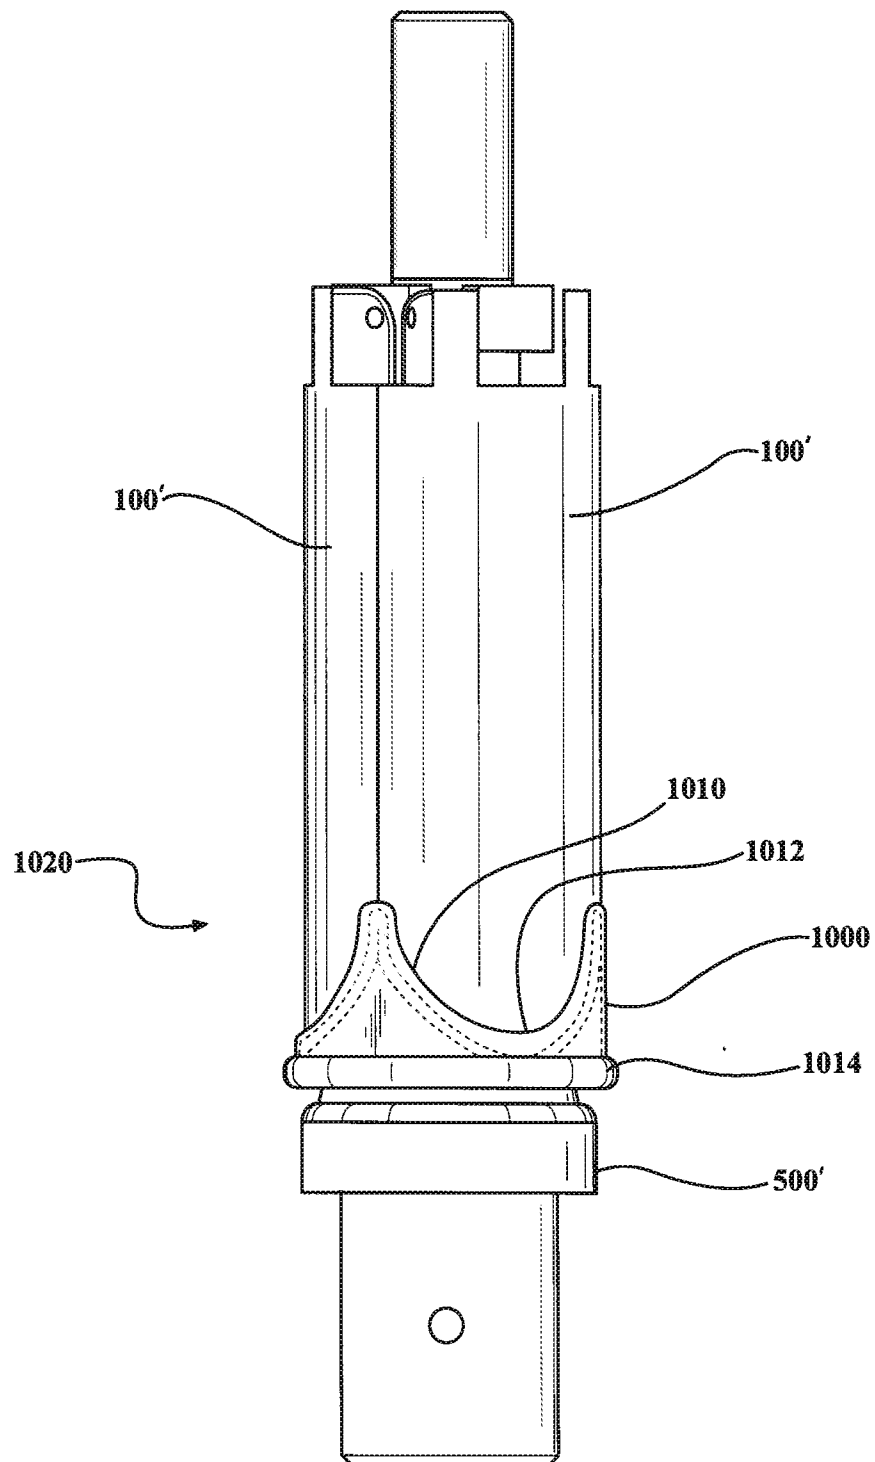


FIG. 26A

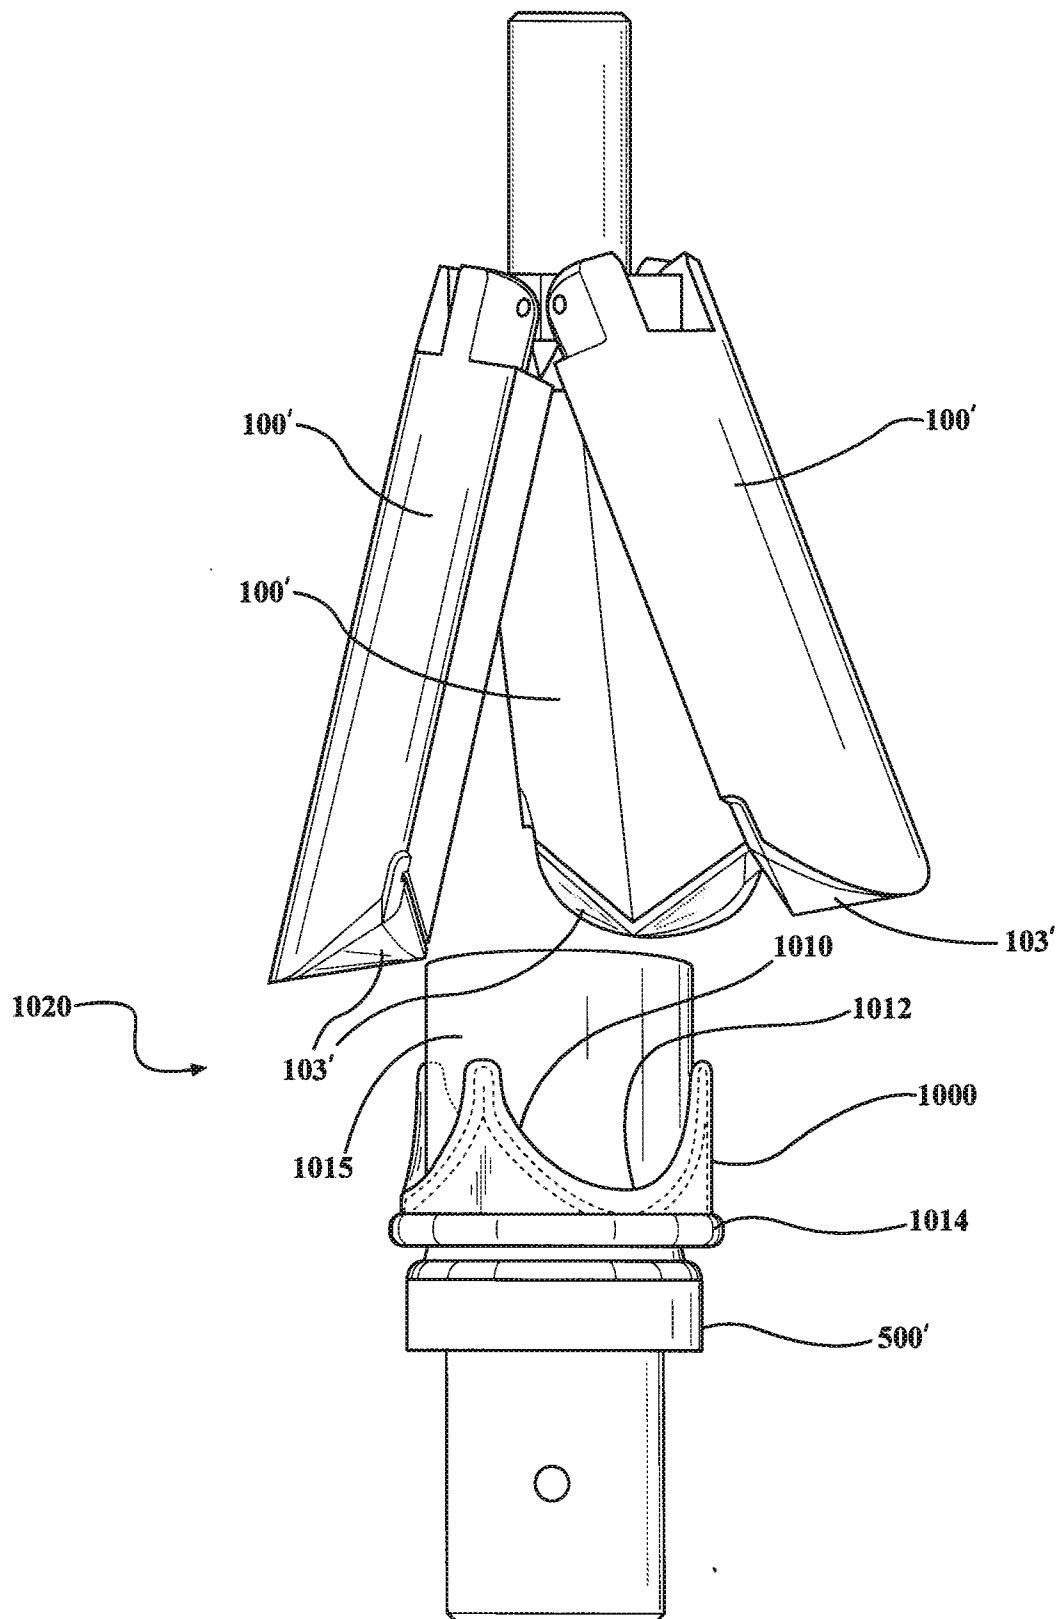


FIG. 26B

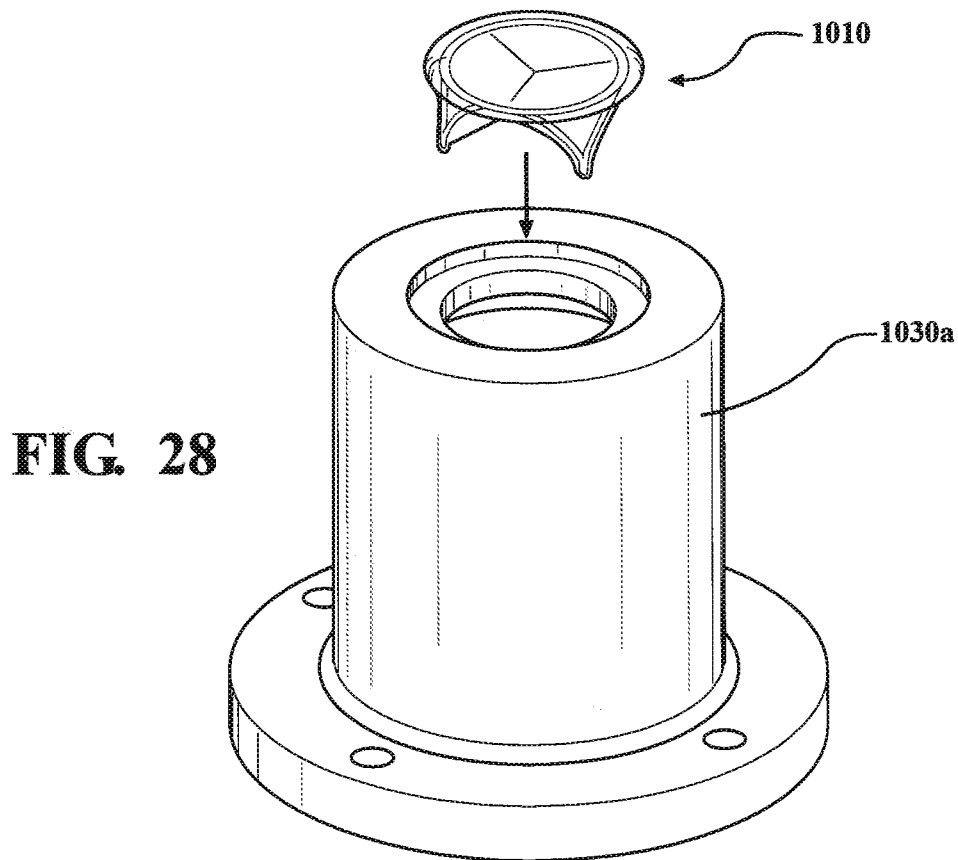
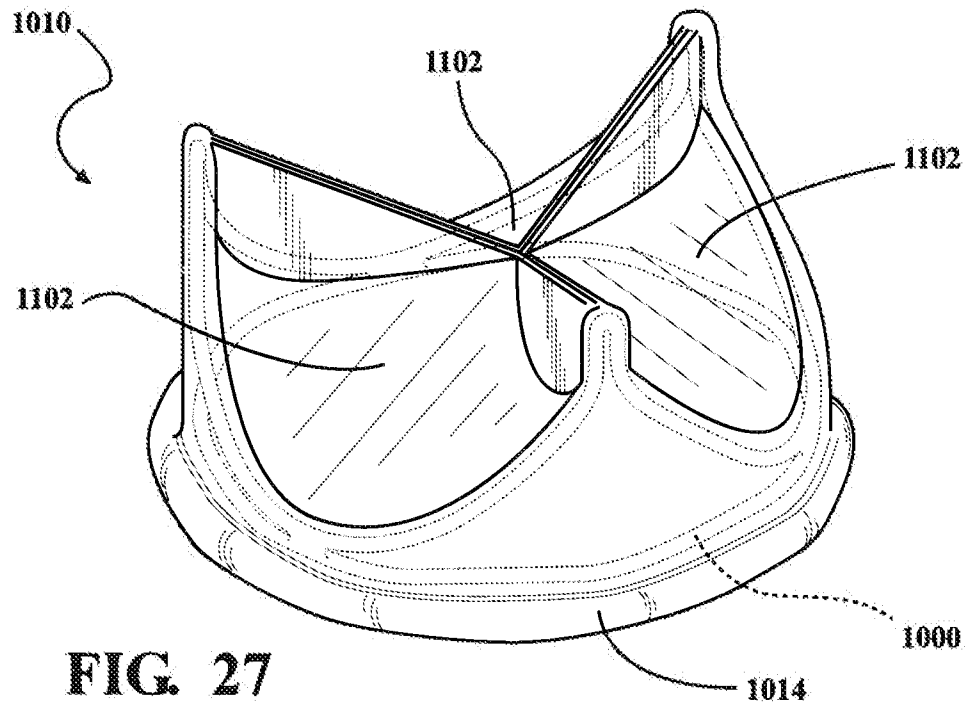


FIG. 29

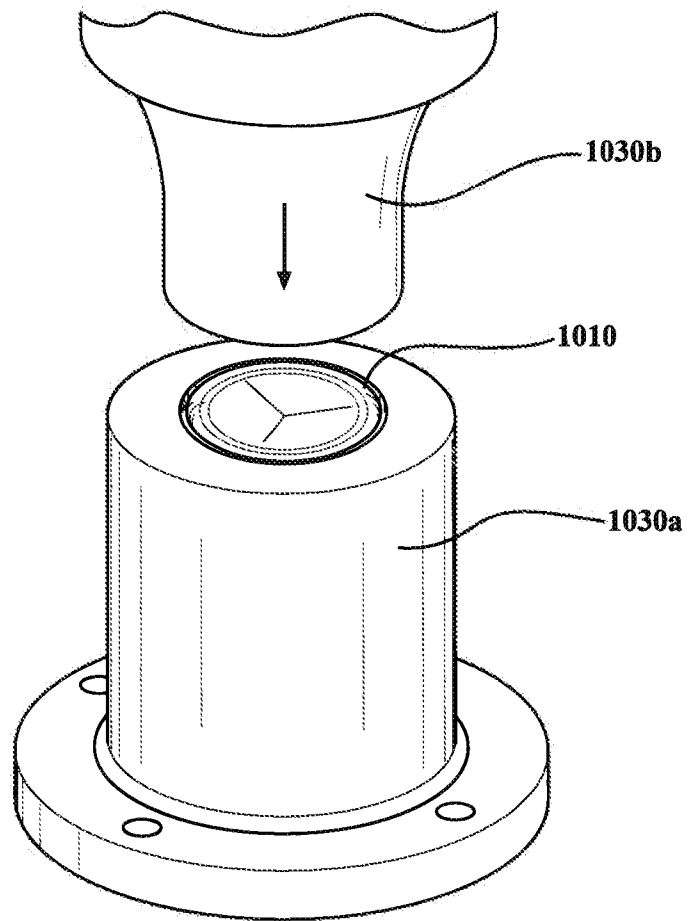


FIG. 30

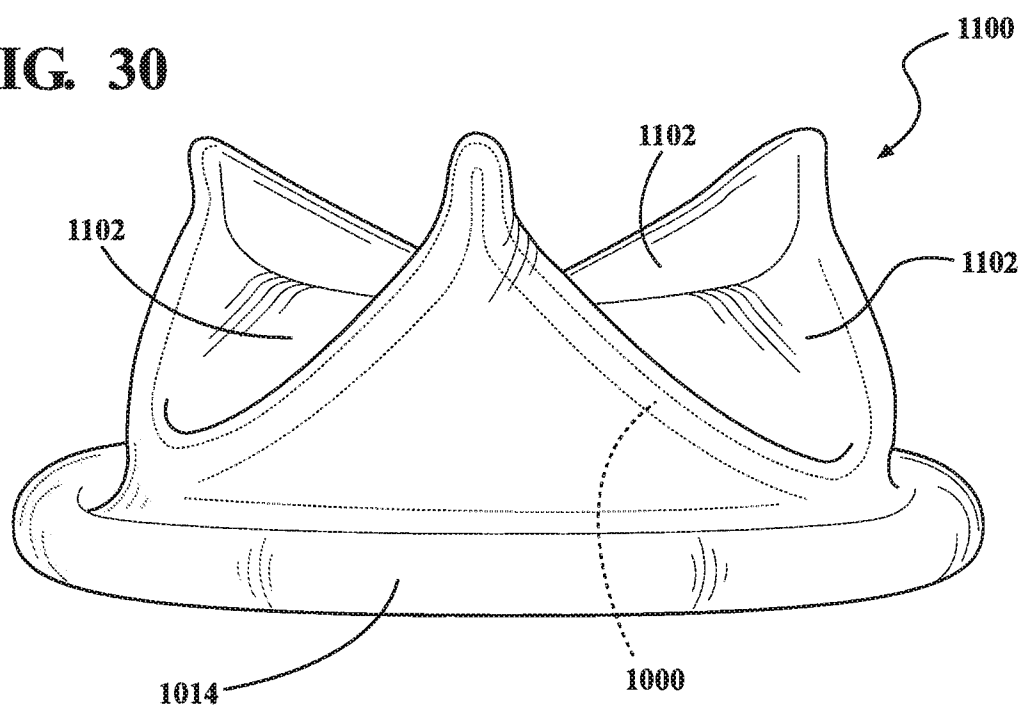


FIG. 31

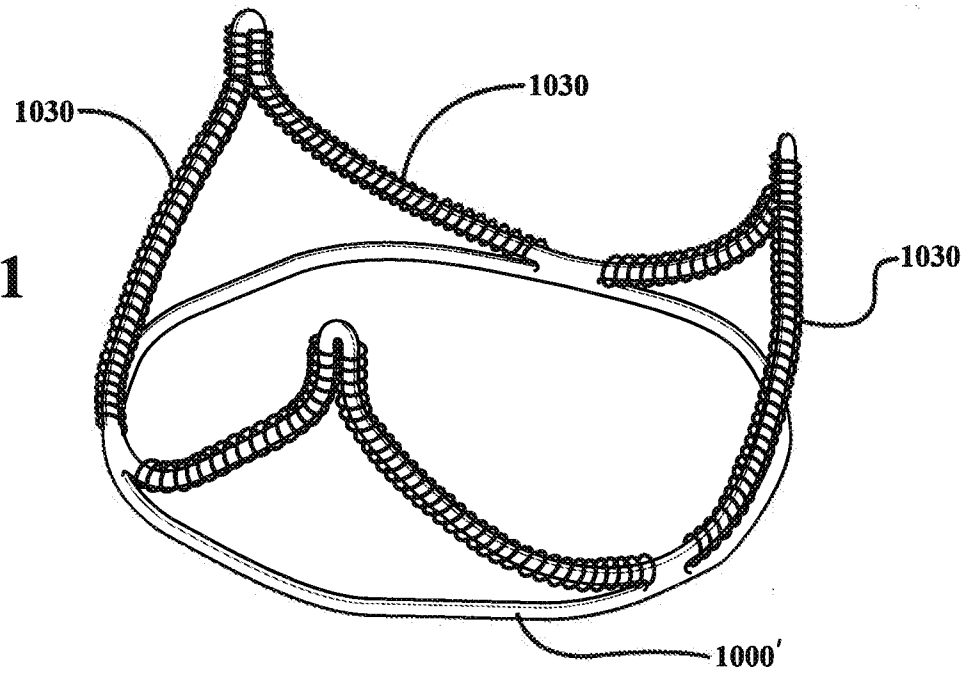


FIG. 32

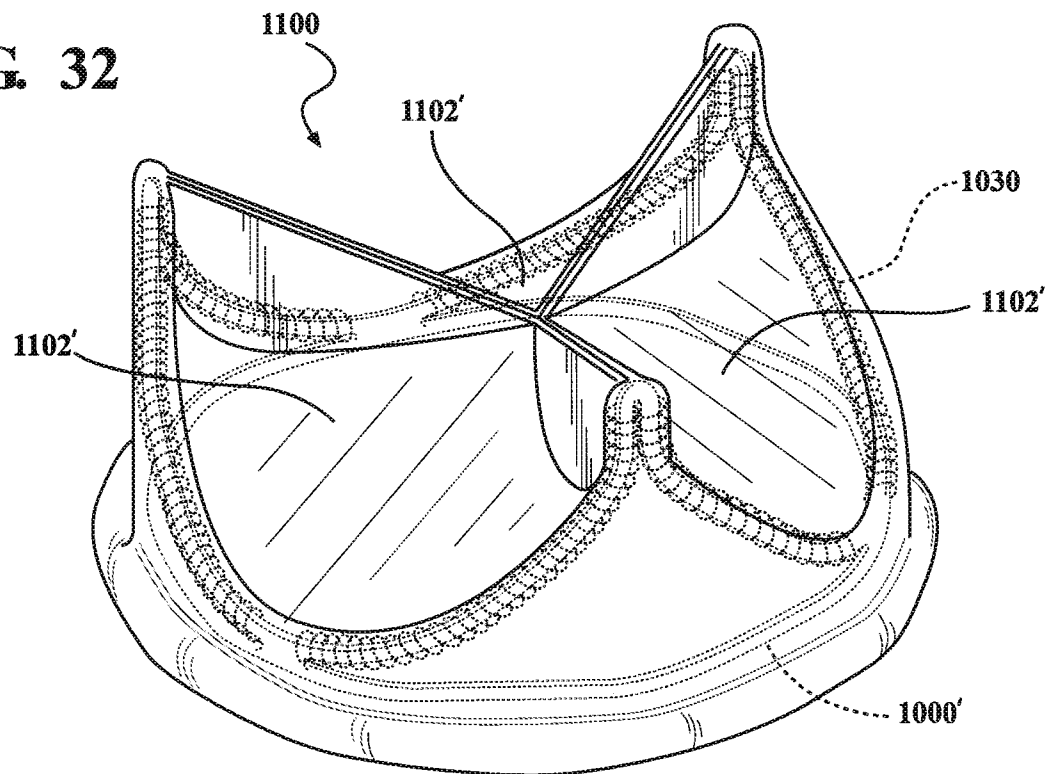


FIG. 33A

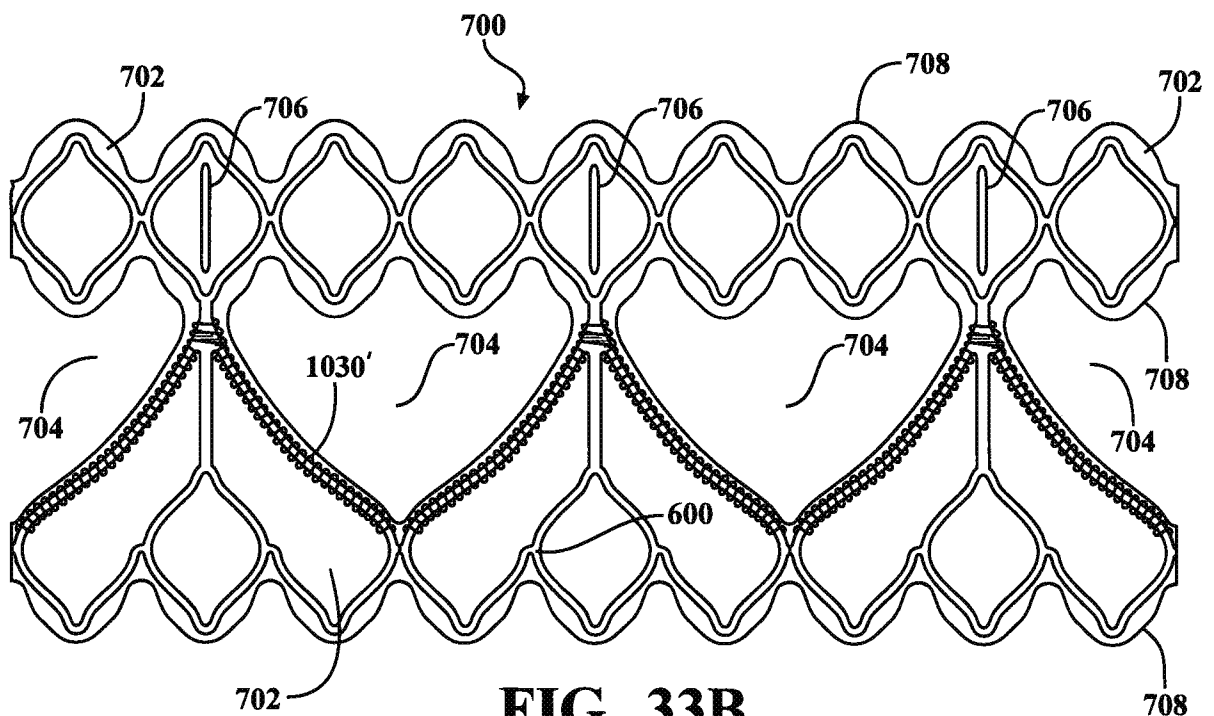
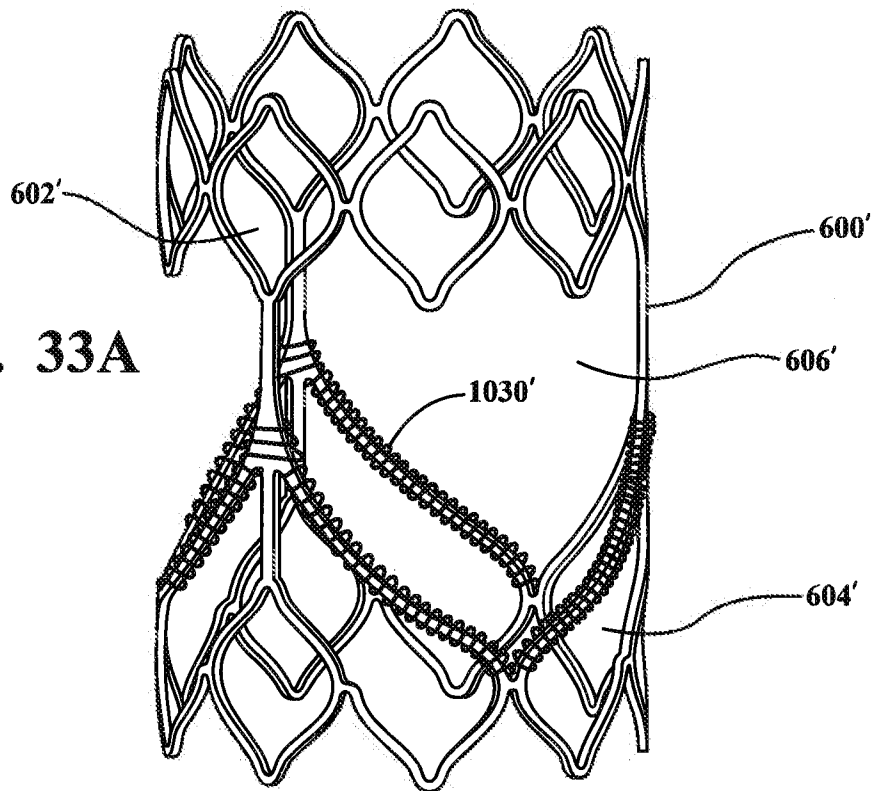


FIG. 33B

FIG. 34

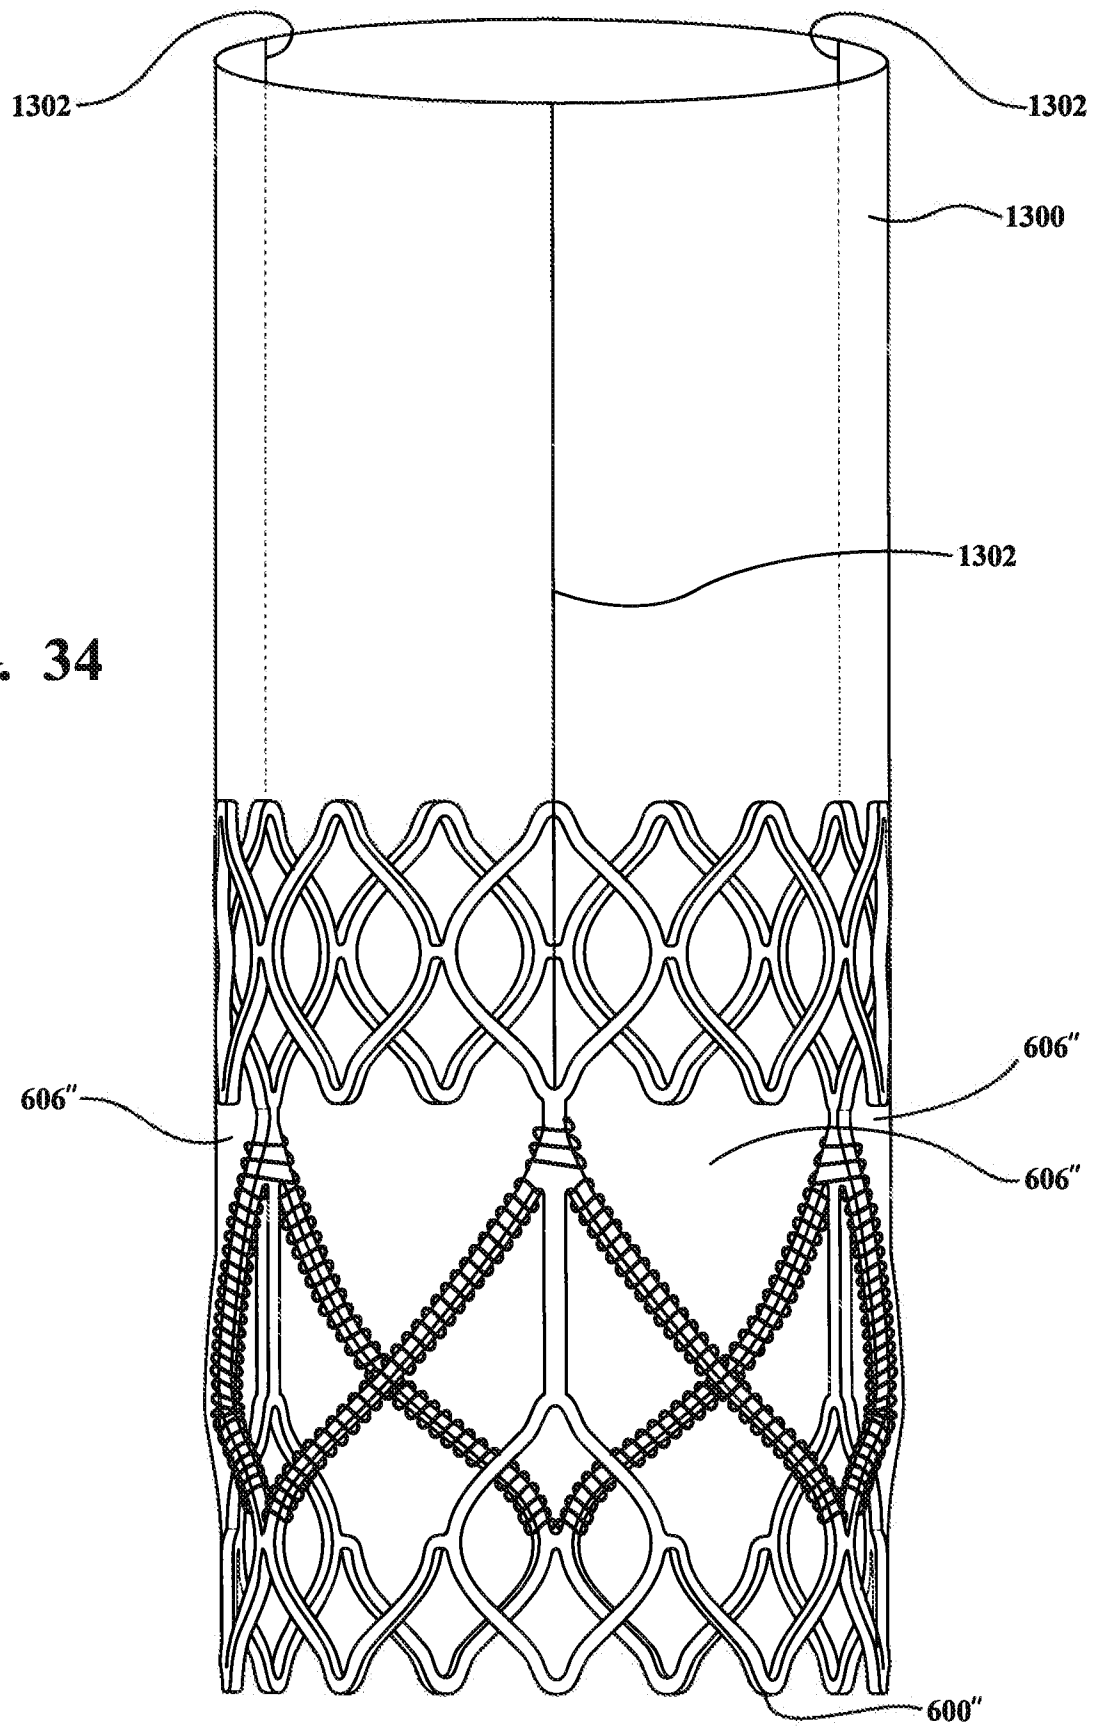
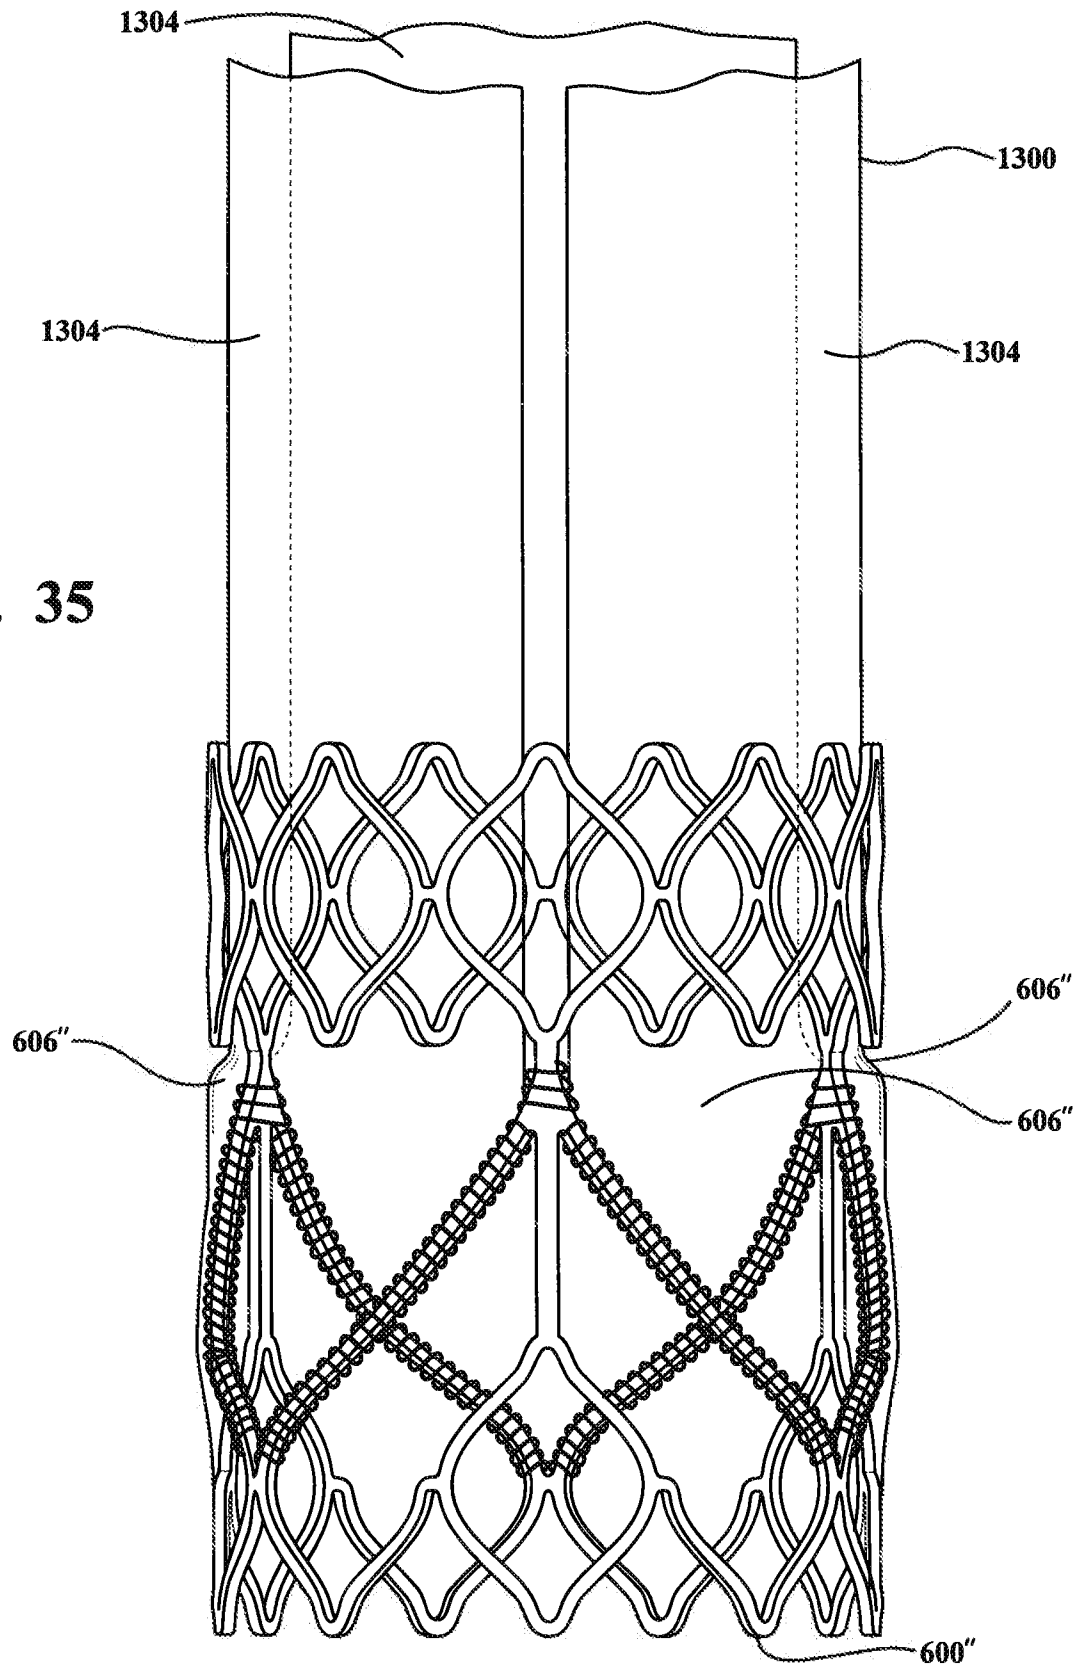


FIG. 35



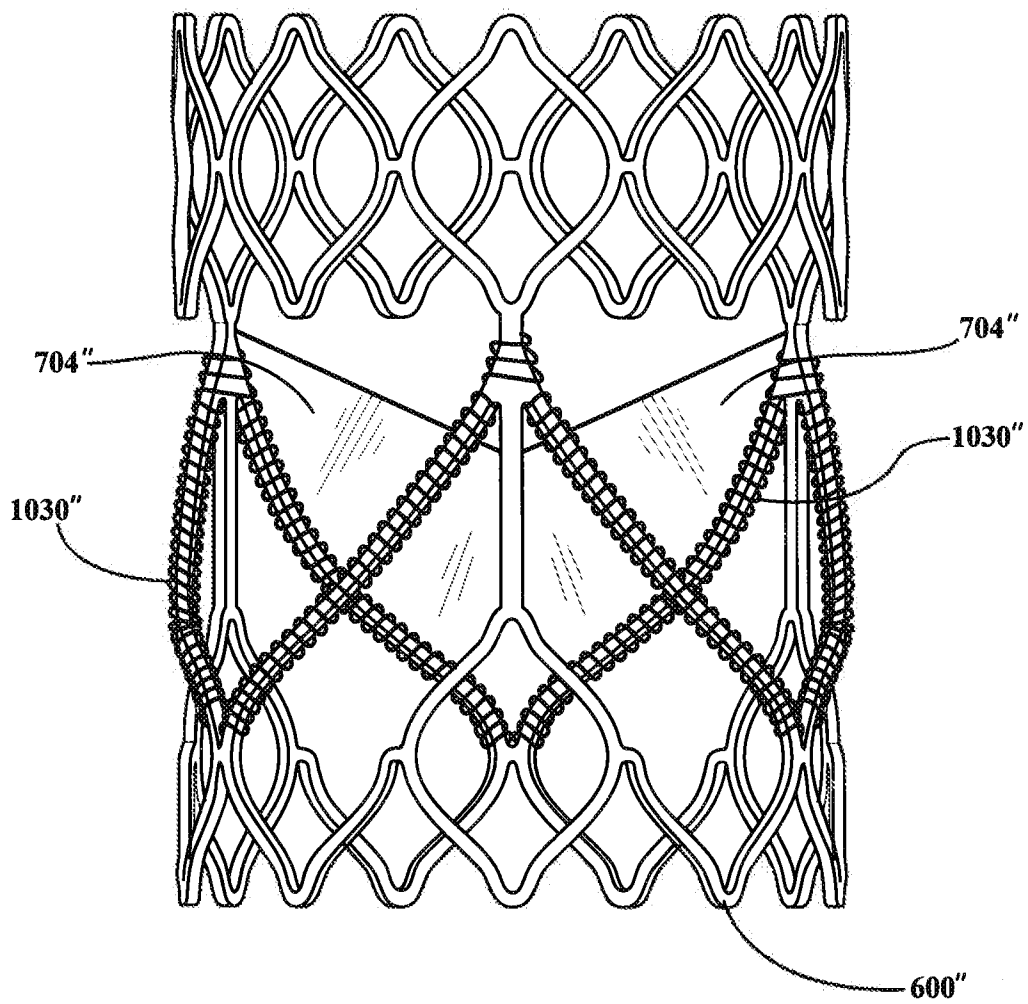


FIG. 36

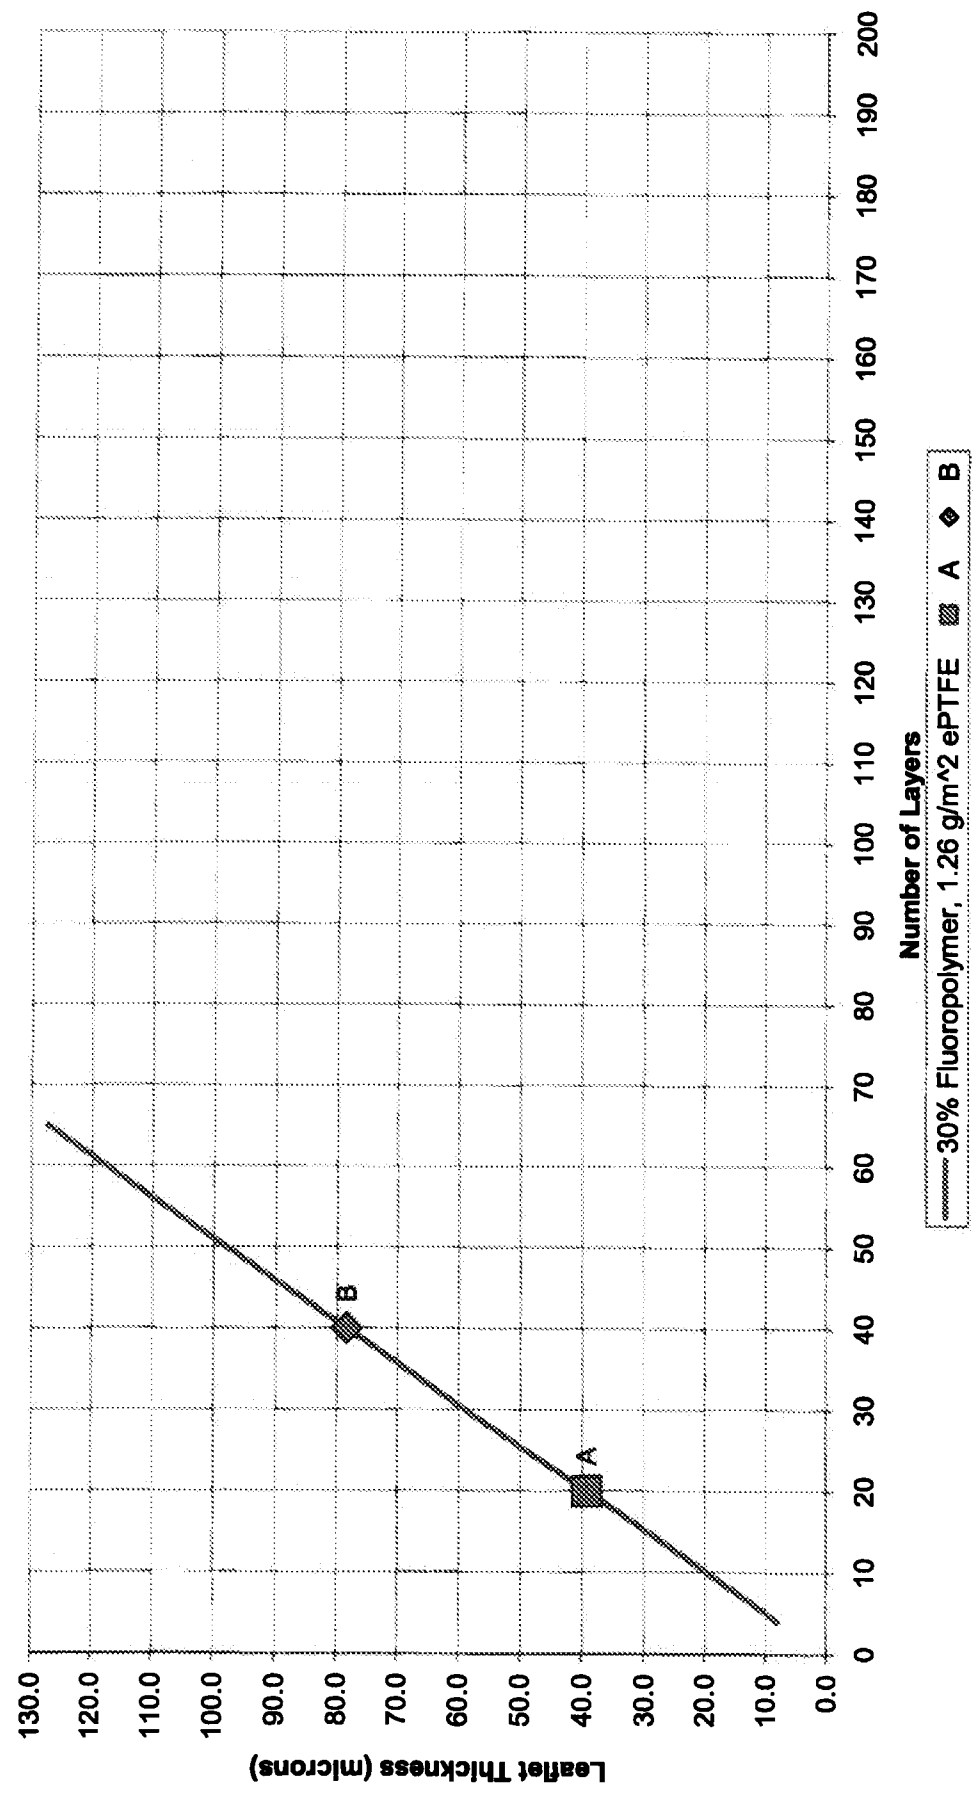


FIG. 37

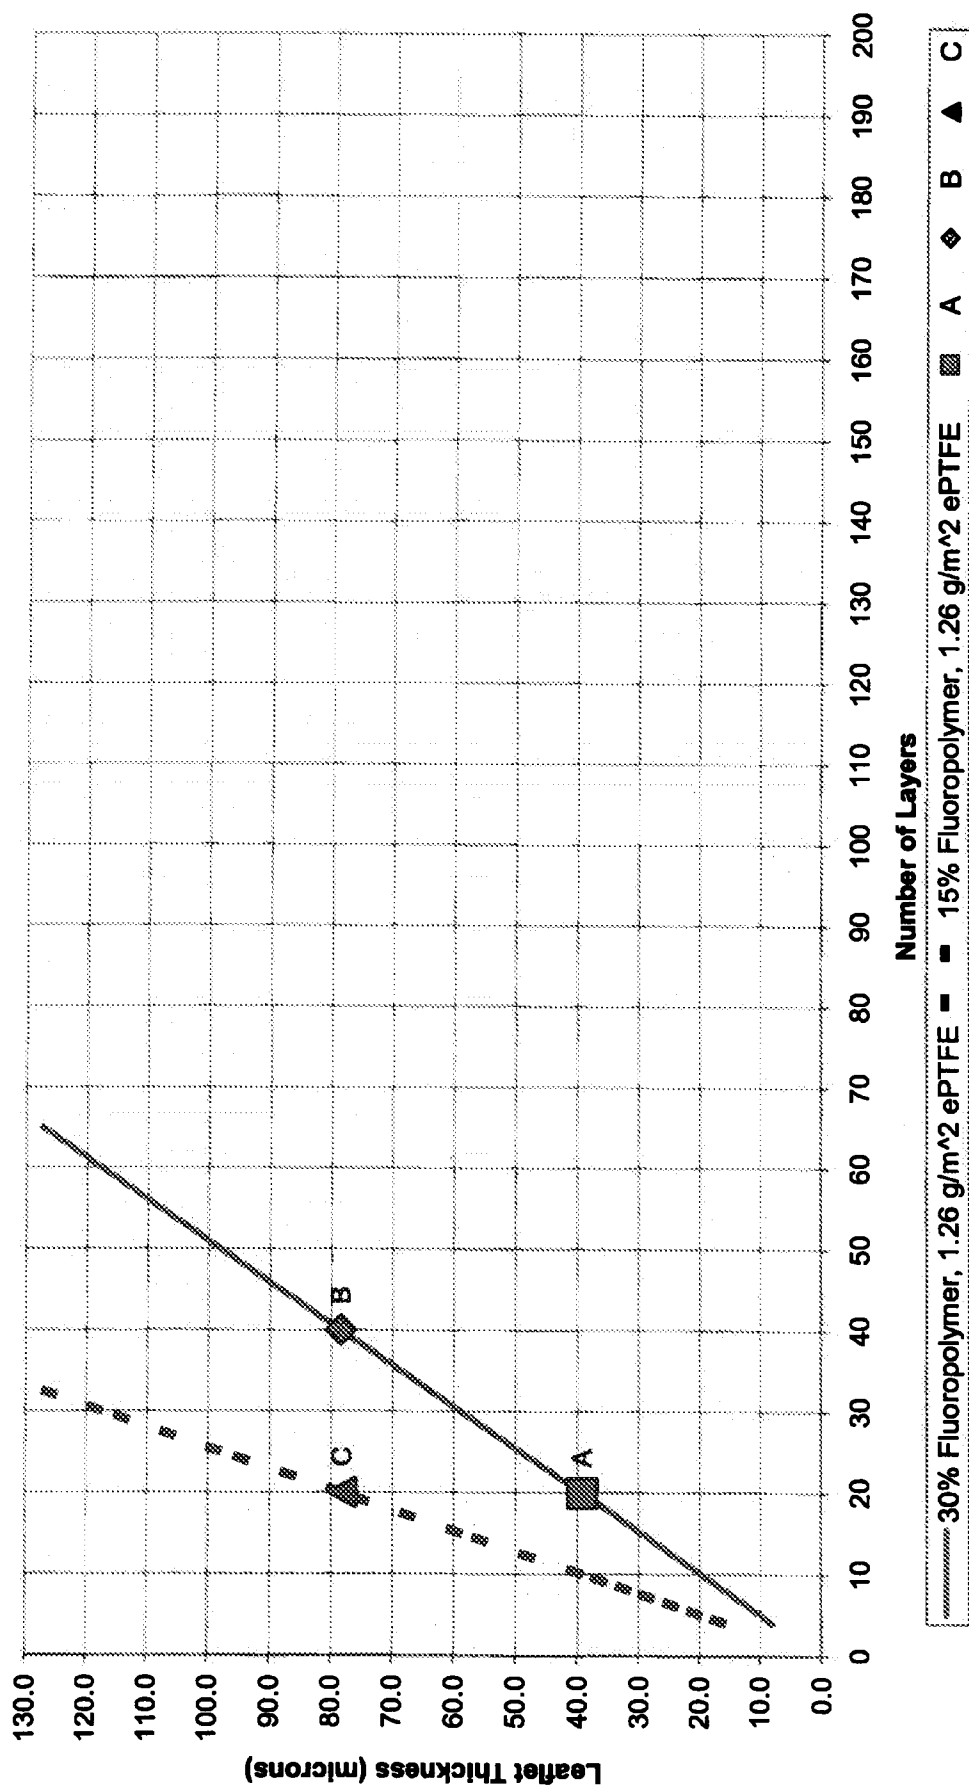


FIG. 38

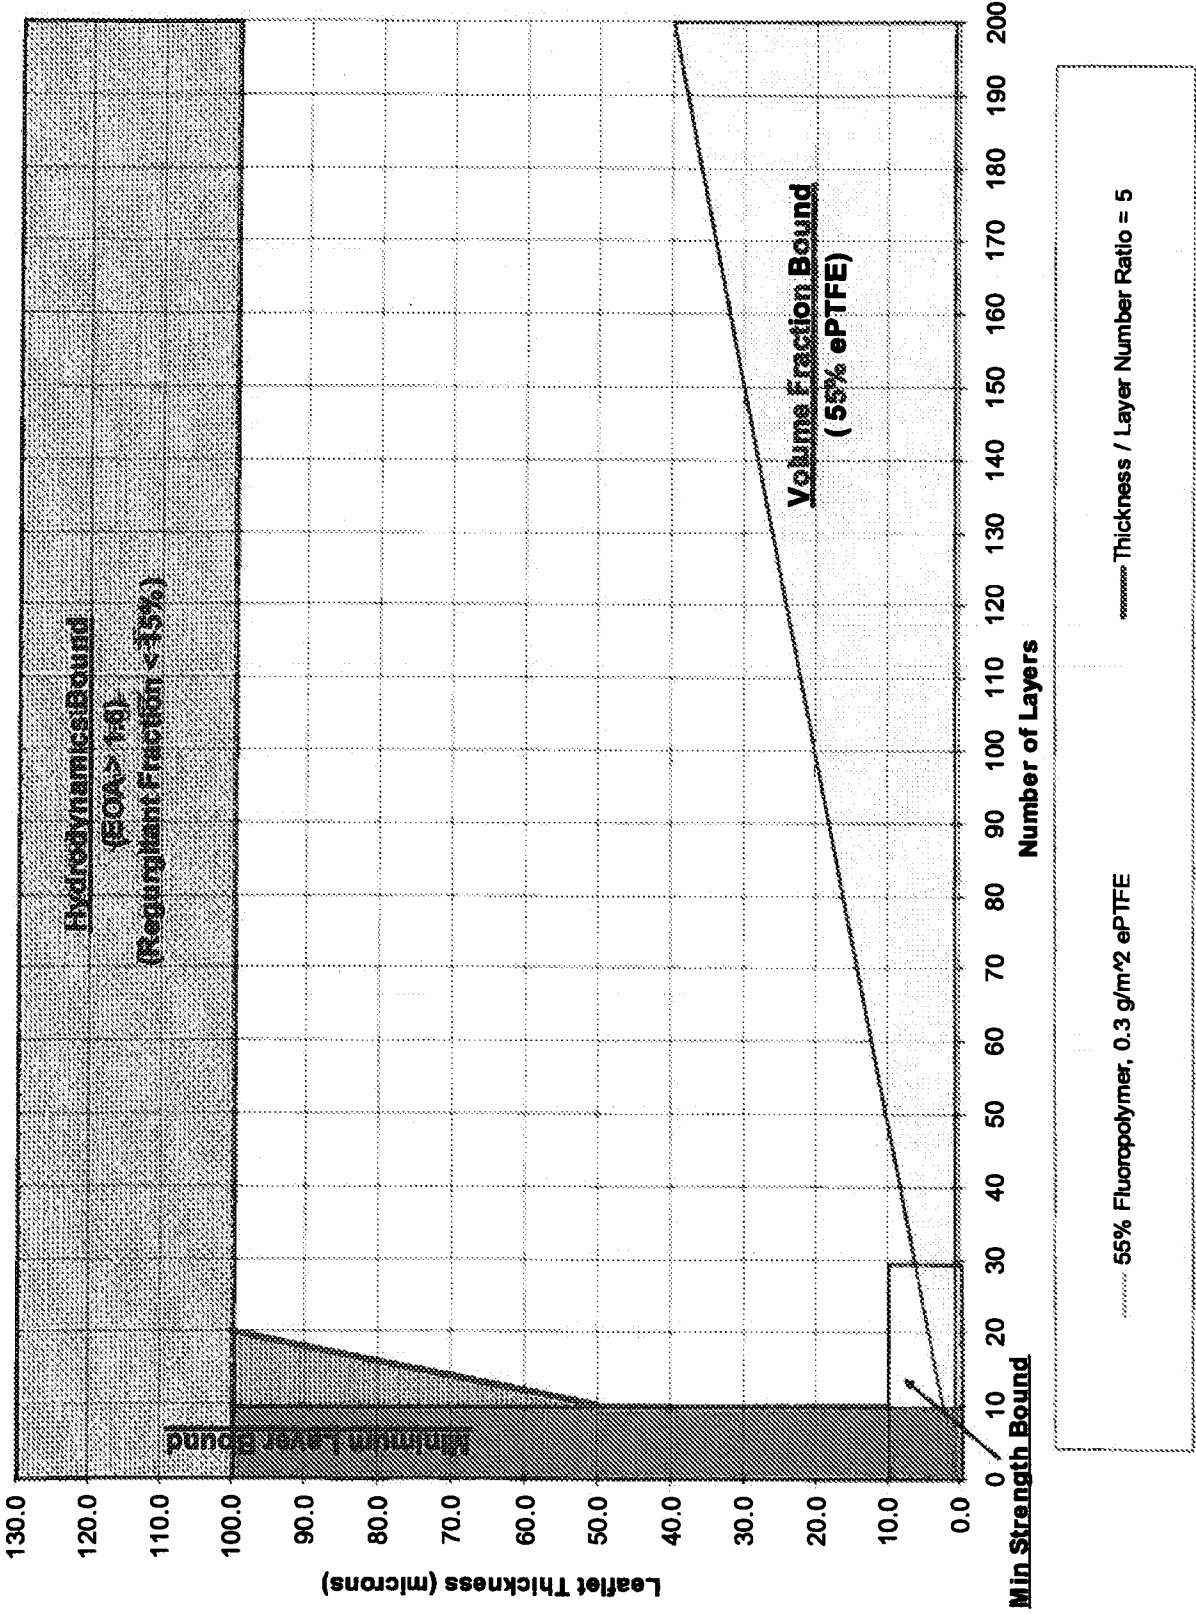


FIG. 39

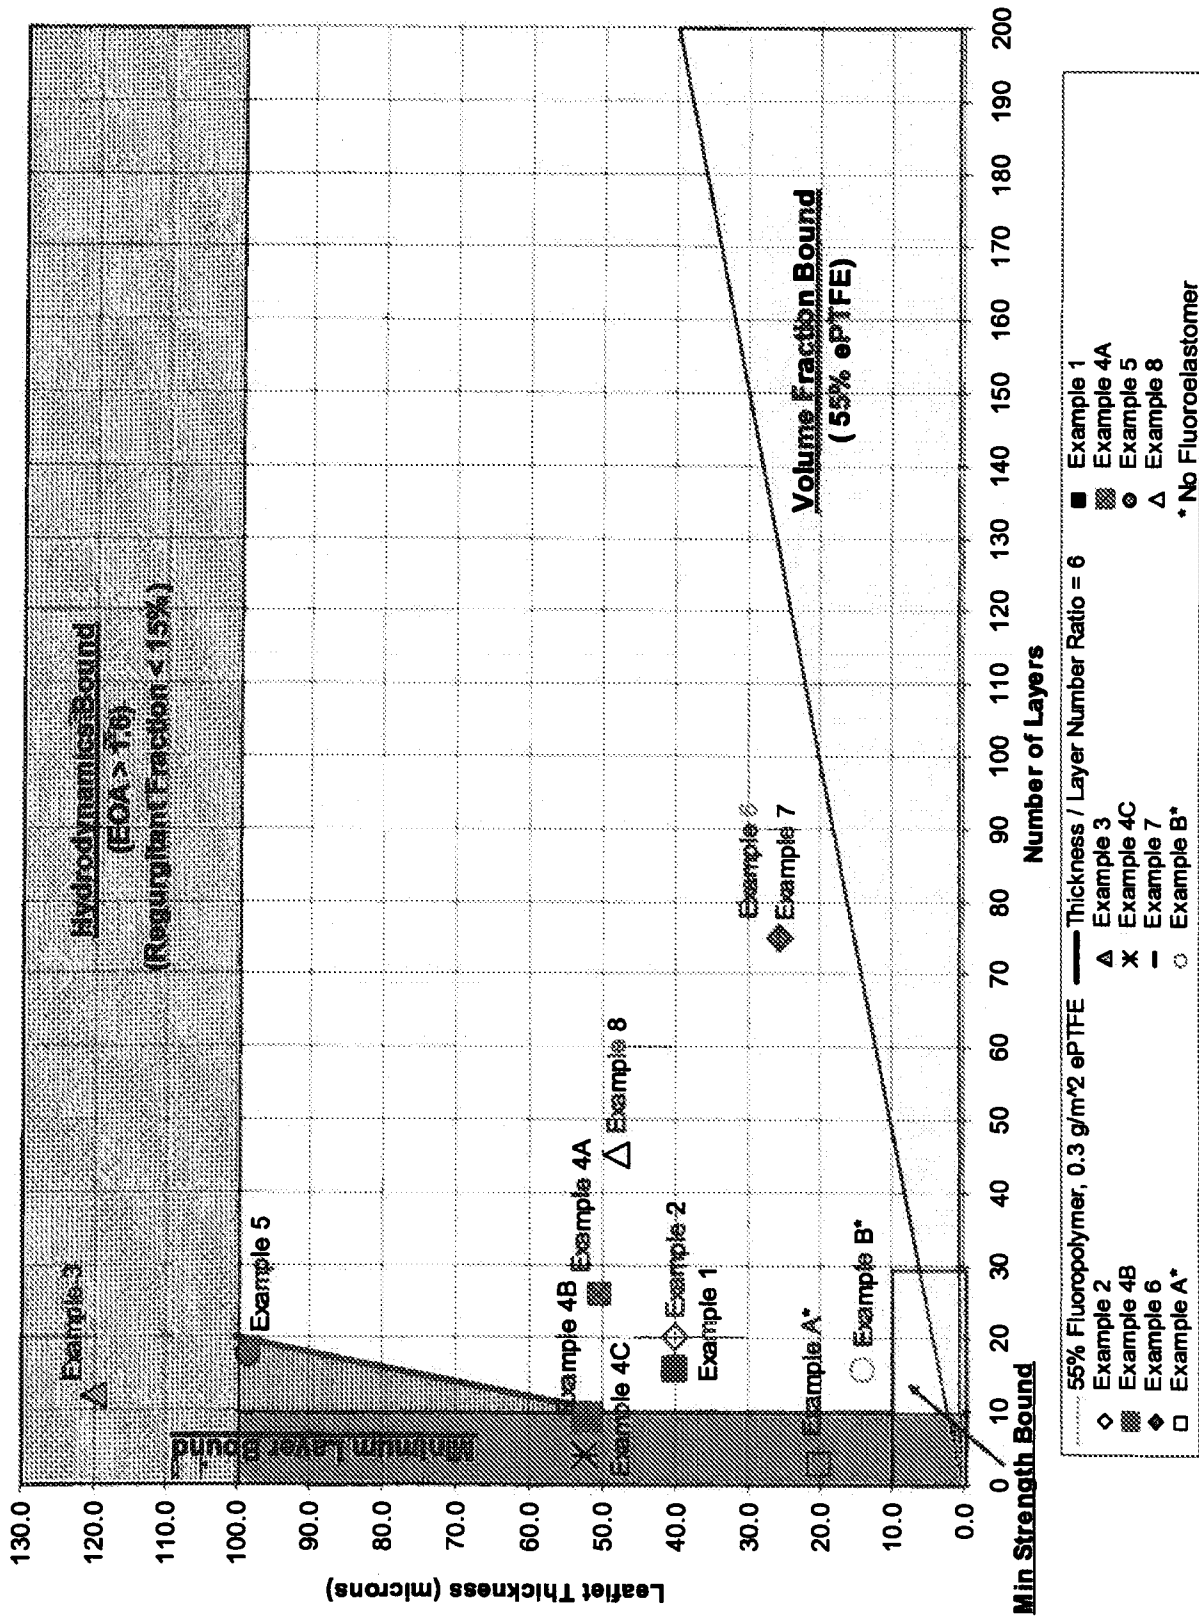


FIG. 40

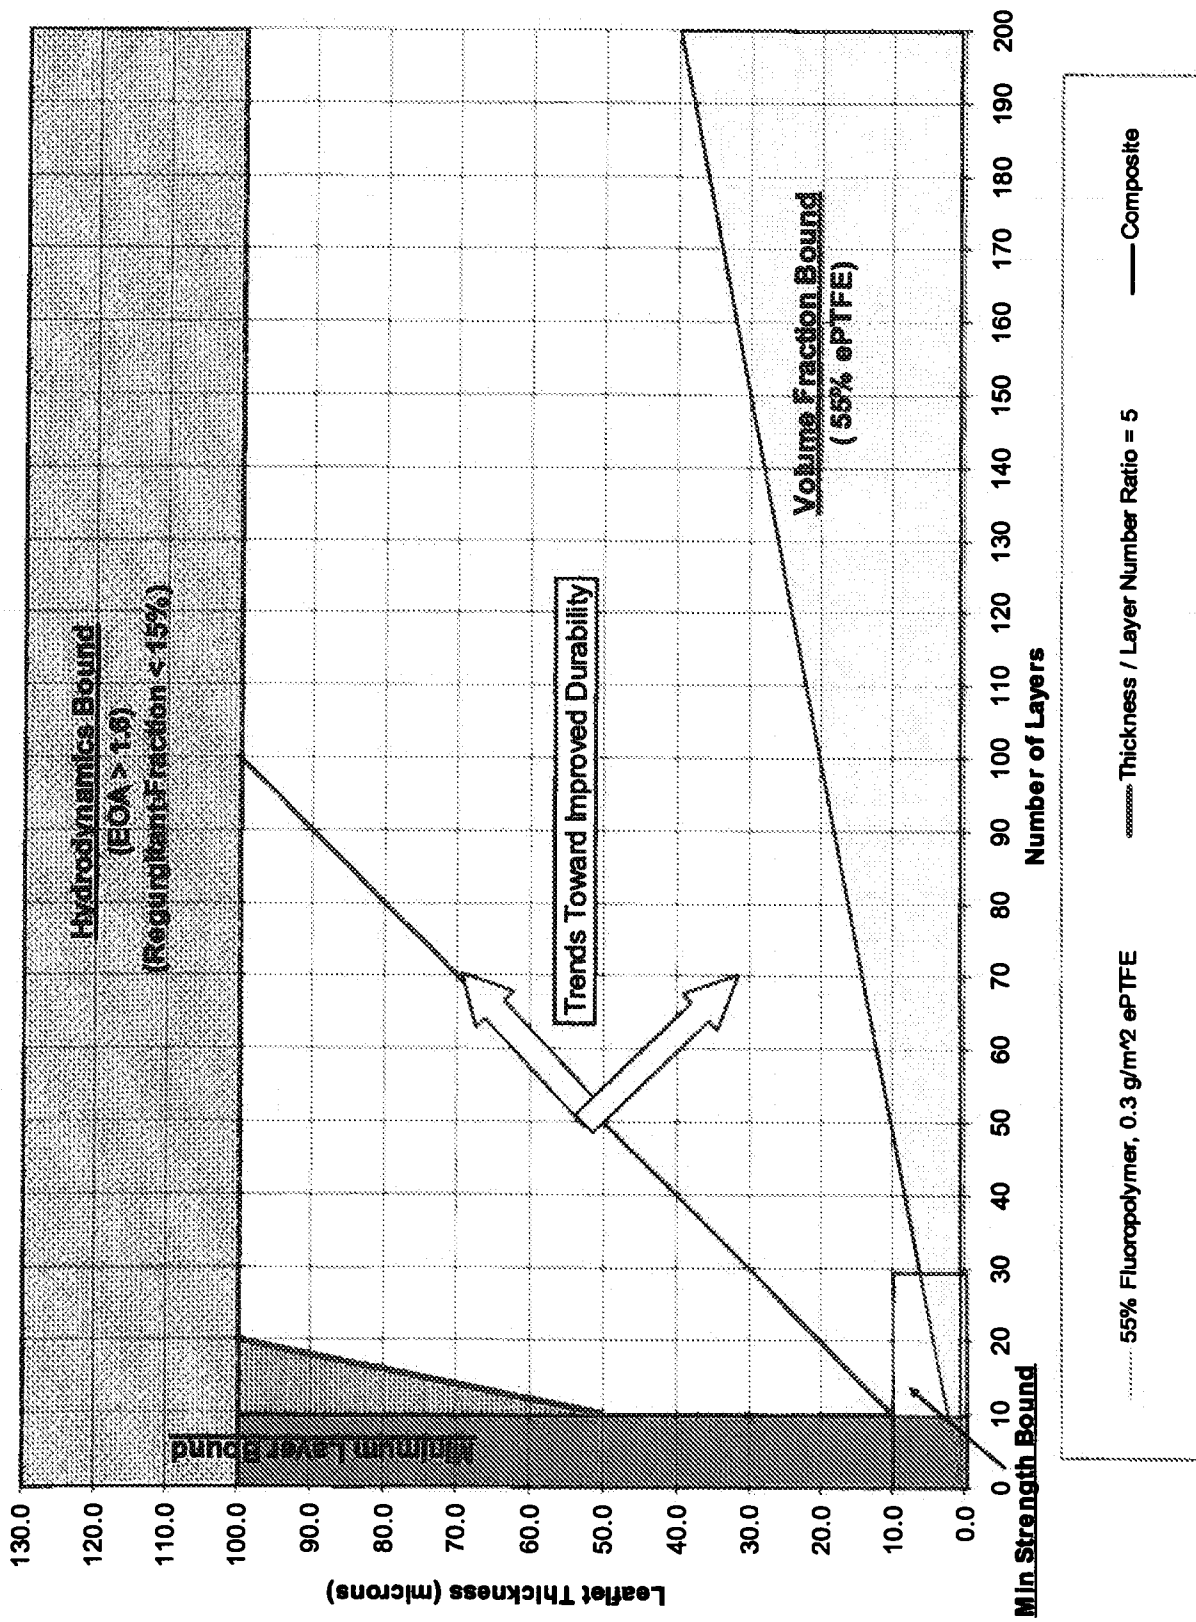


FIG. 41A

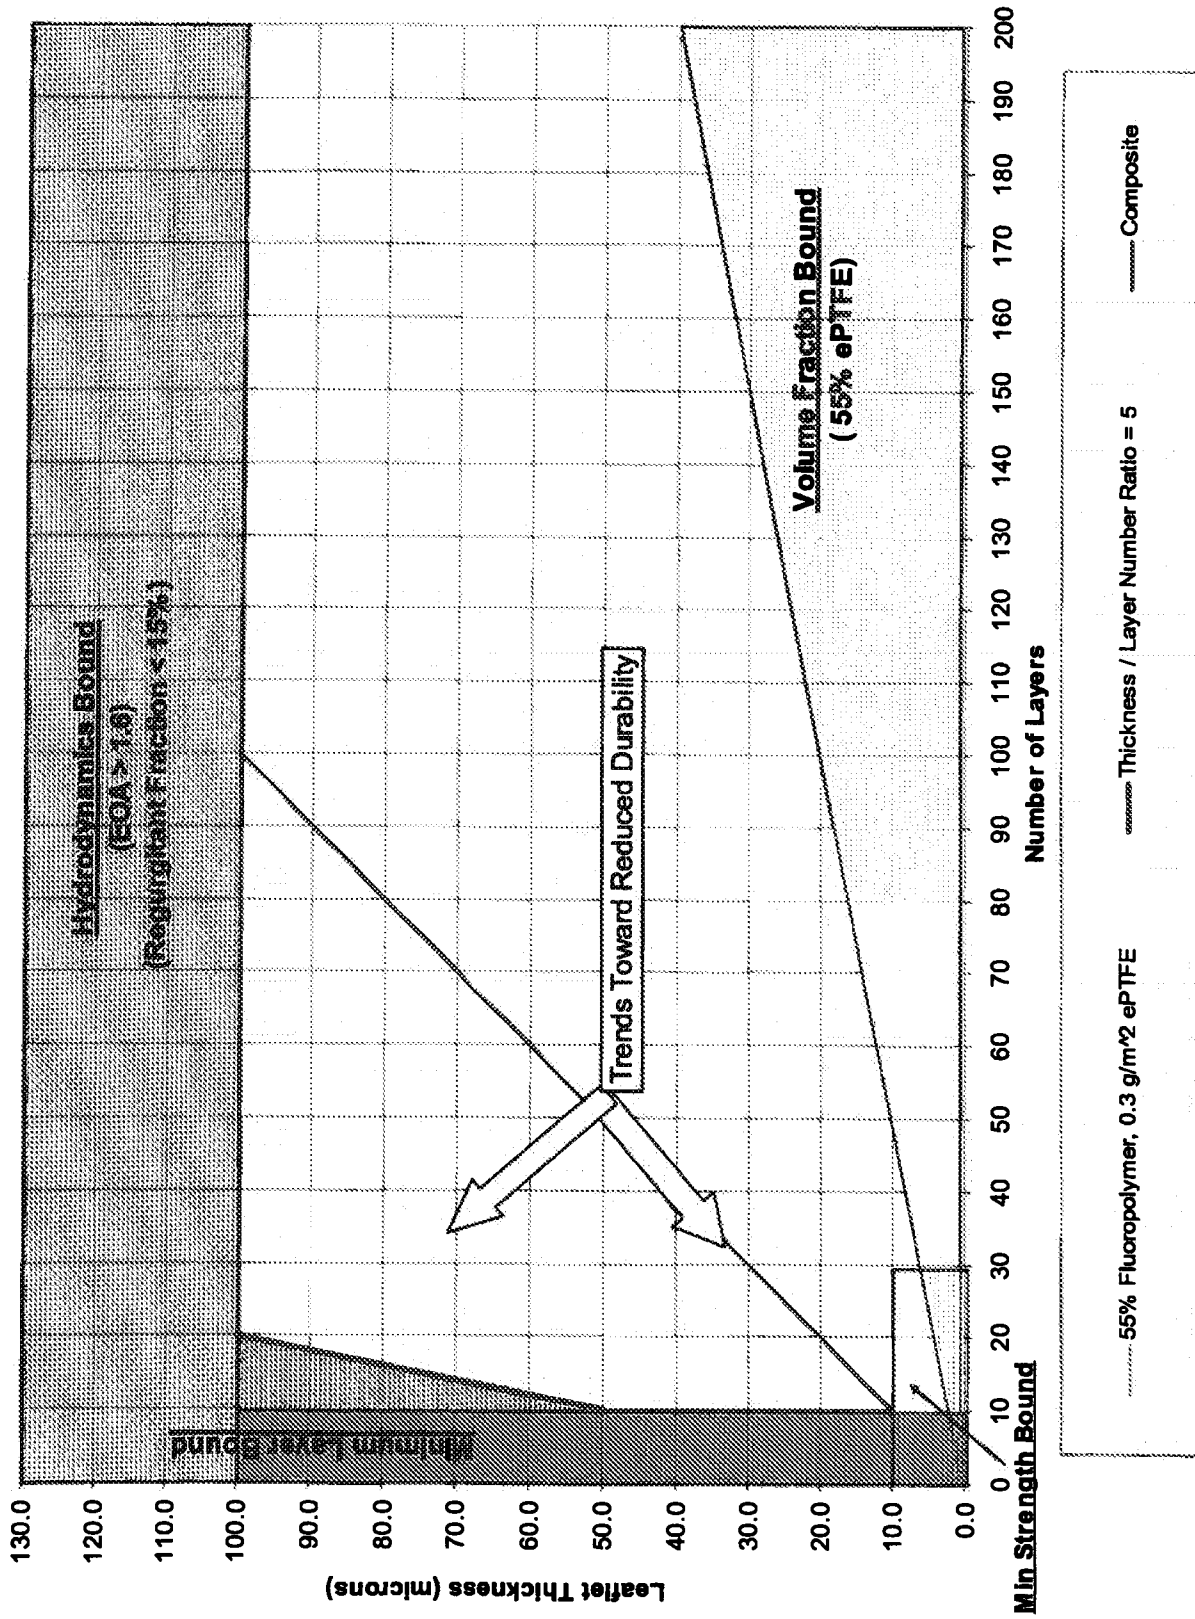


FIG. 41B

RF vs EOA

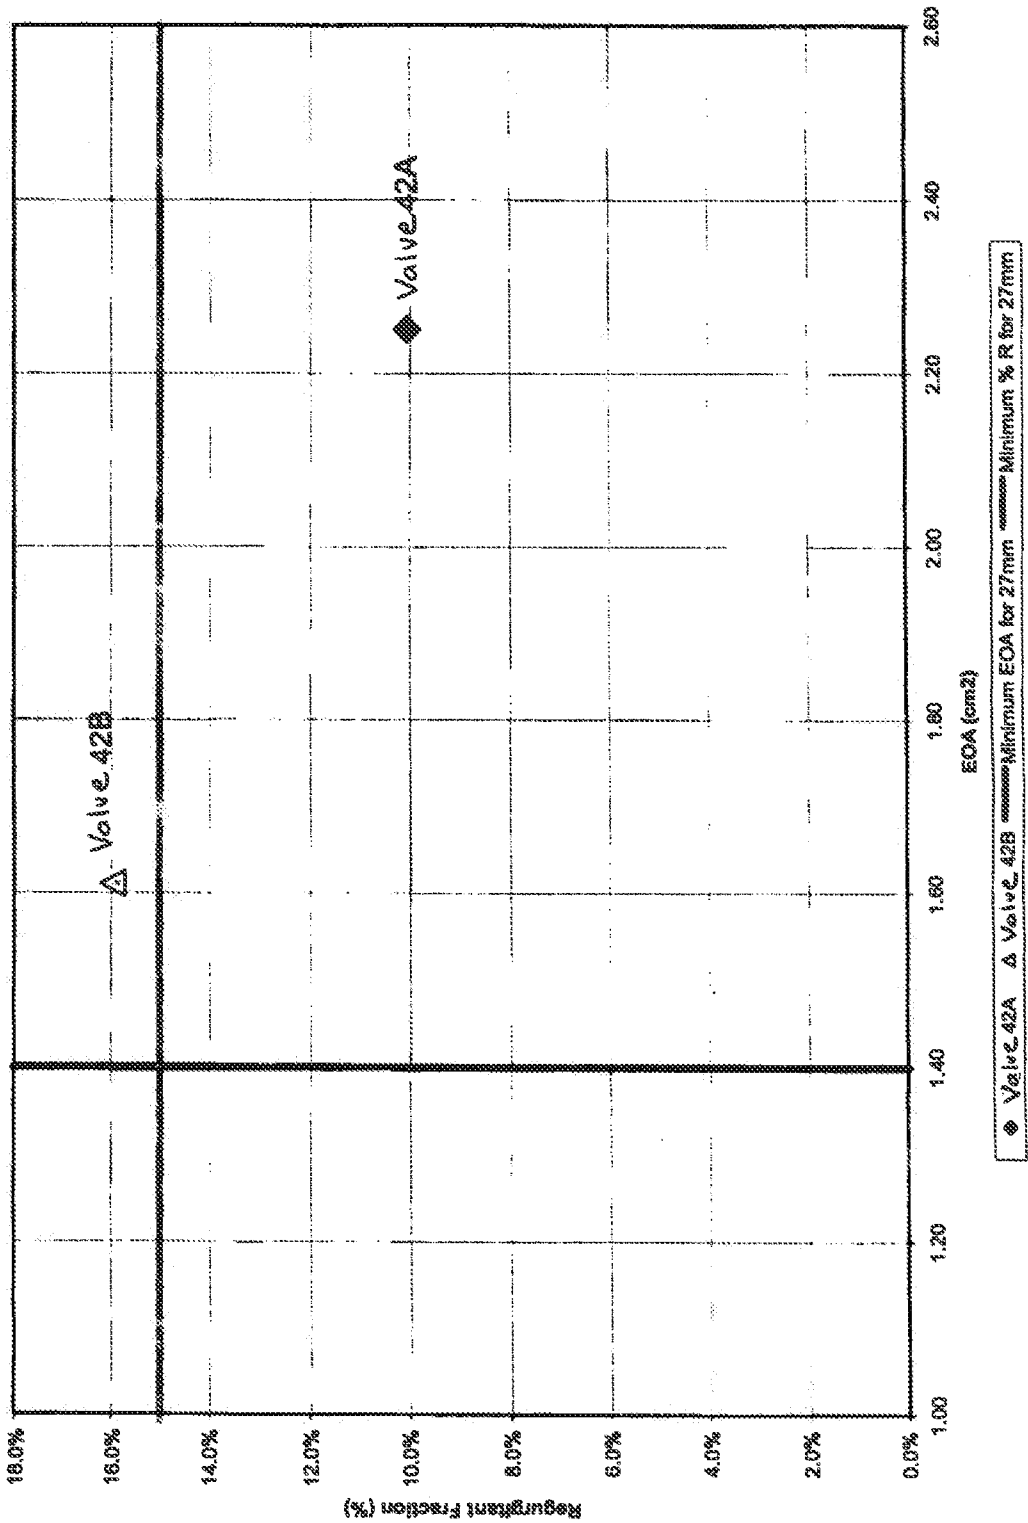


FIG. 42

Table 4

Example Number	Example 4a	Example 4b	Example 4c	Example 5	Example 6	Example 7	Example 8
Frame Type	non-collapsible	non-collapsible	Non-collapsible	non-collapsible	non-collapsible	collapsible	non-collapsible
Cushion Layer	No	No	Yes	No	Yes	Yes	Yes
Leaflet Thickness (μm)	50.3	52.0	52.3	98.3	49.7	25.0	48.0
Volume Fraction (% ePTFE)	28.22	9.74	8.91	9.74	29.9	25.0	24.00
Elastomeric Material	PMVE	PMVE	PMVE	PMVE	PMVE	PMVE	Silicone
Number of Layers	26	9	4	18	95	57	45
(Thickness) / (# of Layers)	1.93	5.78	13.08	5.46	0.52	0.44	1.07
Membrane Properties:							
Mass / Area (g/m^2)	1.15	1.15	2.27	1.15	0.31	0.29	0.57
Thickness (nm)	1016	1016	3556	1016	127	158	2500
MTS in MD (MPa)	410.9	410.9	319.4	410.9	442.0	434.0	339
MTS in TD (MPa)	315.4	315.4	407.3	315.4	560.0	646.0	257
Bubble Point (MPa)	79.7	79.7	101.5	79.7	0.11	0.11	0.46
Density (g/cm^3)	1.059	1.059	0.637	1.059	0.400	0.400	0.221
Composite Properties:							
Thickness (μm)	1.93	5.78	13.08	5.46	0.52	0.44	1.07
Mass / Area (g/m^2)	4.08	11.8	25.48	11.80	1.04	0.94	N/A
Volume Fraction (% ePTFE)	28.22	9.74	8.91	9.74	29.9	30.3	24.00
Dome Burst (KPa)	15.9	17.3	31.7	17.3	4.8	4.14	N/A

FIG. 43

Table 6

Example Number	Example 4a	Example 4b	Example 4c	Example 5	Example 6	Example 7	Example 8
Collapsible Frame	No	No	No	No	No	Yes	No
Effective Orifice Area (EOA, cm ²)							
Compaction & Expansion	Pre 1.88	2.05	N/A	1.73	2.19	2.10	2.4
	Post N/A	N/A	N/A	N/A	N/A	2.20	N/A
At removal	2.17 @100million	Failed @ 6 million	Failed @ 12.4 million	2.109 @100million	2.04, @100million	2+ million cycles in animal	2.4 @150million
Regurgitant Fraction (RF, %)							
Compaction & Expansion	Pre 10.86	11.71	N/A	11.71	9.70	25.9	12.5
	Post N/A	N/A	N/A	N/A	N/A	22.0	N/A
At removal	15.66 @100million	Failed @ 6 million	Failed @ 12.4 million	9.50 @100million	13.7, @100million	2+ million cycles in animal	28.0 @150million
Construction & Leaflet Failures Observed							
Frame Detachment		X		X			
Leaflet			X				
Hole							
Tear							
Delaminate				X			

FIG. 44

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2012/040529

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61F2/24 A61L27/48 A61L27/56
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61F A61L

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 6 776 604 B1 (CHOBOTOV MICHAEL V [US] ET AL) 17 August 2004 (2004-08-17) column 7, line 6 - line 9 column 15, line 39 - line 47 -----	1-17
A	EP 0 773 971 A1 (GORE & ASS [US]) 21 May 1997 (1997-05-21) paragraphs [0002], [0015], [0023], [0026] -----	1-17
A	WO 2007/016251 A2 (COOK INC [US]) 8 February 2007 (2007-02-08) paragraphs [0044], [0088], [0089], [0092] ----- -/-	1-17



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

7 November 2012

Date of mailing of the international search report

14/11/2012

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Franz, Volker

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2012/040529

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 2006/000763 A2 (UNIV GLASGOW [GB]; WHEATLEY DAVID JOHN [GB]) 5 January 2006 (2006-01-05) page 58, line 13 - line 17 page 25, line 11 - line 13 page 22, line 18 - line 24 -----	1-17
X	WO 98/26731 A2 (ATRIUM MEDICAL CORP [US]) 25 June 1998 (1998-06-25) page 7, line 17 page 8, line 2 page 8, line 19 - line 24 -----	18-24
A	WO 02/100454 A1 (SCIMED LIFE SYSTEMS INC [US]) 19 December 2002 (2002-12-19) page 22, line 1 - line 8 page 4, line 2 - line 14 -----	18-24
X	EP 0 293 090 A2 (BAXTER TRAVENOL LAB [US]) 30 November 1988 (1988-11-30)	25-50,69
Y	page 2, line 50 page 3, line 55 - page 4, line 7 -----	56-68
Y	EP 0 150 608 A1 (SHILEY INC [US]) 7 August 1985 (1985-08-07) claim 1 -----	56-68
A	WO 2009/149462 A2 (EDWARDS LIFESCIENCES CORP [US]; HARITON ILIA [IL]; BENICHO NETANEL [I]) 10 December 2009 (2009-12-10) paragraphs [0065], [0078]; figure 25 -----	56-68
A	US 2003/055495 A1 (PEASE MATTHEW L [US] ET AL) 20 March 2003 (2003-03-20) paragraph [0050] -----	56-68

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2012/040529

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☒ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☒ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

This International Searching Authority found multiple (groups of) inventions in this international application, as follows:

1. claims: 1-17

A prosthetic valve comprising a leaflet made of several porous fluoropolymer layers with an elastomer filling the pores. The ratio of thickness in microns to number of layers is less than 5. This group of claims is directed towards solving the technical problem how to improve durability of a valve leaflet without compromising mechanical properties.

2. claims: 18-24

Method of forming a leaflet for a prosthetic heart valve, comprising the steps of wrapping a sheet of composite material onto itself, forming an axial seam. This group of claims is directed towards solving the problem how to manufacture a composite material in an alternative way.

3. claims: 25-55, 69

Leaflet for a heart valve comprising a composite of porous fluoropolymer with elastomer filling the pores, wherein the composite comprises less than 80% fluoropolymer by weight. This group of claims is directed towards solving the problem how to select the composition for a leaflet in an alternative way.

4. claims: 56-68

A prosthetic valve with a leaflet fixed to a support structure and a cushion between support structure and leaflet. This group of claims is directed towards solving the technical problem how to minimize wear between support structure and valve leaflet.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2012/040529

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 6776604	B1	17-08-2004	US 6776604 B1 17-08-2004
		US 2004224047 A1	11-11-2004
EP 0773971	A1	21-05-1997	AU 1430795 A 22-02-1996
		CA 2192457 A1	08-02-1996
		DE 69419265 D1	29-07-1999
		DE 69419265 T2	05-01-2000
		EP 0773971 A1	21-05-1997
		JP H10503538 A	31-03-1998
		US 5641566 A	24-06-1997
		US 5645915 A	08-07-1997
		WO 9603457 A1	08-02-1996
WO 2007016251	A2	08-02-2007	US 2007027535 A1 01-02-2007
		WO 2007016251 A2	08-02-2007
WO 2006000763	A2	05-01-2006	WO 2006000763 A2 05-01-2006
		WO 2006000776 A2	05-01-2006
WO 9826731	A2	25-06-1998	AU 727411 B2 14-12-2000
		AU 5898498 A	15-07-1998
		CA 2273887 A1	25-06-1998
		EP 0971643 A2	19-01-2000
		EP 2298241 A2	23-03-2011
		JP 2002510985 A	09-04-2002
		WO 9826731 A2	25-06-1998
WO 02100454	A1	19-12-2002	AT 303170 T 15-09-2005
		CA 2450160 A1	19-12-2002
		DE 60205903 D1	06-10-2005
		DE 60205903 T2	08-06-2006
		EP 1399200 A1	24-03-2004
		JP 4401165 B2	20-01-2010
		JP 2005505317 A	24-02-2005
		US 2003017775 A1	23-01-2003
		US 2006264138 A1	23-11-2006
		WO 02100454 A1	19-12-2002
EP 0293090	A2	30-11-1988	CA 1302897 C 09-06-1992
		EP 0293090 A2	30-11-1988
		JP 1046468 A	20-02-1989
		US 4816339 A	28-03-1989
EP 0150608	A1	07-08-1985	AU 566778 B2 29-10-1987
		AU 3717884 A	04-07-1985
		CA 1229202 A1	17-11-1987
		DE 3471879 D1	14-07-1988
		EP 0150608 A1	07-08-1985
		ES 8608850 A1	16-12-1986
		JP 1504264 C	28-06-1989
		JP 60158858 A	20-08-1985
		JP 63052899 B	20-10-1988
		MX 157676 A	08-12-1988
		US 4629459 A	16-12-1986
		ZA 8410032 A	27-08-1986
WO 2009149462	A2	10-12-2009	CA 2728231 A1 10-12-2009
		CN 202105047 U	11-01-2012

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2012/040529

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		EP 2323591 A2	25-05-2011
		JP 2011522634 A	04-08-2011
		US 2010036484 A1	11-02-2010
		US 2011319991 A1	29-12-2011
		WO 2009149462 A2	10-12-2009

US 2003055495	A1	20-03-2003	NONE
