



(12) **United States Design Patent**
Okada et al.

(10) **Patent No.:** **US D1,069,123 S**
(45) **Date of Patent:** **** Apr. 1, 2025**

- (54) **EYE TESTING APPARATUS AND EQUIPMENT**
- (71) Applicant: **TOPCON CORPORATION**, Tokyo (JP)
- (72) Inventors: **Hiroyuki Okada**, Tokyo (JP); **Takeo Aoki**, Tokyo (JP); **Yasuhisa Kaneda**, Tokyo (JP)
- (73) Assignee: **TOPCON CORPORATION**, Tokyo (JP)
- (**) Term: **15 Years**
- (21) Appl. No.: **29/827,098**

- (22) Filed: **Feb. 17, 2022**
- (51) **LOC (15) Cl.** **24-02**
- (52) **U.S. Cl.**
USPC **D24/172**
- (58) **Field of Classification Search**
USPC D24/170, 172, 185-187, 231, 232, 140, D24/158-160, 120, 184, 137; D15/199; D16/100, 130, 136, 200, 300
CPC A61B 3/024; A61B 3/113; A61B 3/028; A61B 3/112; A61B 3/14; A61B 3/00; A61B 3/0008; A61B 3/18; A61B 3/11; A61B 5/163; A61B 5/6821; G02B 27/0172; G02B 27/0025; G02B 27/0012; G02B 27/0093
See application file for complete search history.

- (56) **References Cited**
U.S. PATENT DOCUMENTS
D341,541 S * 11/1993 Ichiyoshi D10/46
5,474,066 A * 12/1995 Grolman A61B 3/165
600/401
D390,662 S * 2/1998 Cooper D24/172
D394,505 S * 5/1998 Hayashi D24/172
5,838,424 A * 11/1998 Wawro A61B 3/02
351/200

(Continued)

FOREIGN PATENT DOCUMENTS

JP D1744030 * 5/2023

OTHER PUBLICATIONS

NW500 Non-Mydriatic Retinal Camera. 2023. Site visited Feb. 15, 2024. [chrome-extension://efaidnbmnnnibpcajpegglefindmkaj/https://cdn.brandfolder.io/I6S47VV/at/5mhkhwjrzmsx6tksfzmm96/NW500_brochure.pdf] (Year: 2023).*

(Continued)

Primary Examiner — Justin M Jonaitis
Assistant Examiner — Maheen Khurshid
(74) *Attorney, Agent, or Firm* — Muncy, Geissler, Olds & Lowe, P.C.


(57) **CLAIM**

The ornamental design for an eye testing apparatus and equipment as shown and described.


DESCRIPTION

FIG. 1 is a top, front, and right side perspective view of an eye testing apparatus and equipment showing our new design;
FIG. 2 is a bottom, front, and right side perspective view thereof;
FIG. 3 is a bottom, back, and left side perspective view thereof;
FIG. 4 is a front view thereof;
FIG. 5 is a back view thereof;
FIG. 6 is a top plan view thereof;
FIG. 7 is a bottom plan view thereof;
FIG. 8 is a right side elevational view thereof;
FIG. 9 is a left side elevational view thereof; and,
FIG. 10 is a reference view showing the eye testing apparatus and equipment in an alternate position.
In the drawings, the broken lines depict portions of the eye testing apparatus and equipment that form no part of the claimed design.


1 Claim, 10 Drawing Sheets

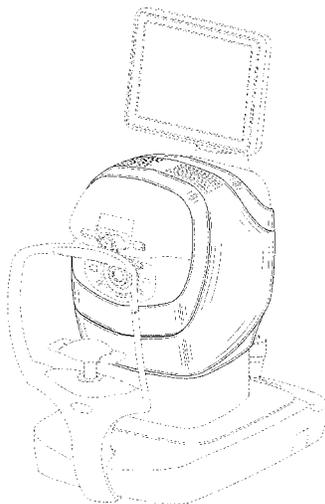


F I G. 1

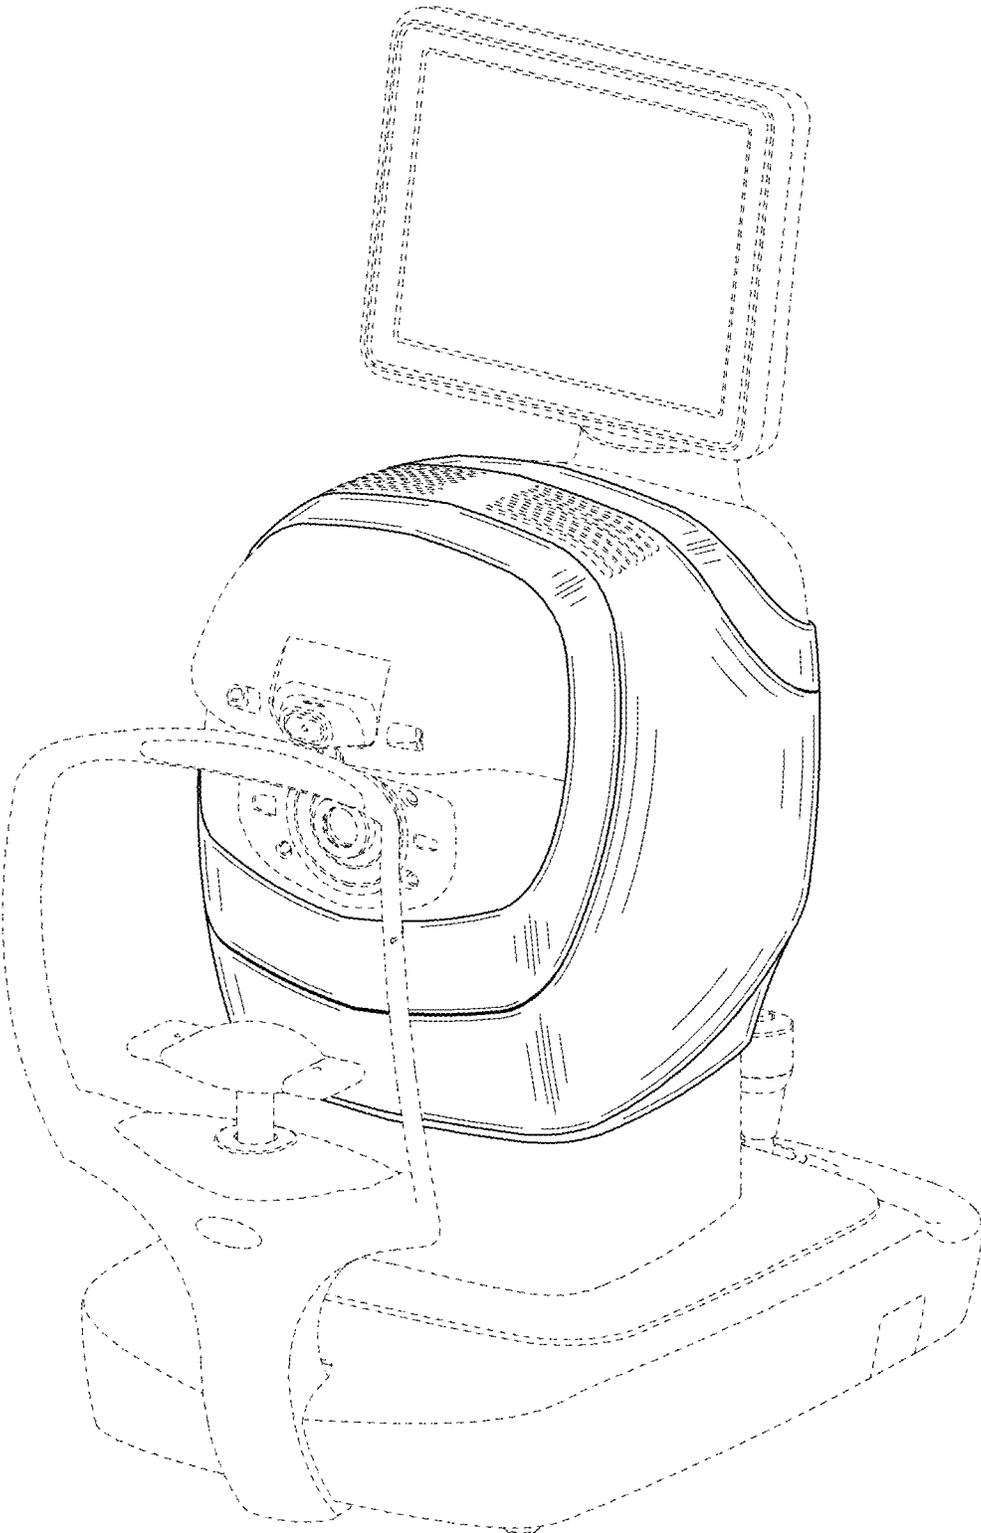


F I G. 2

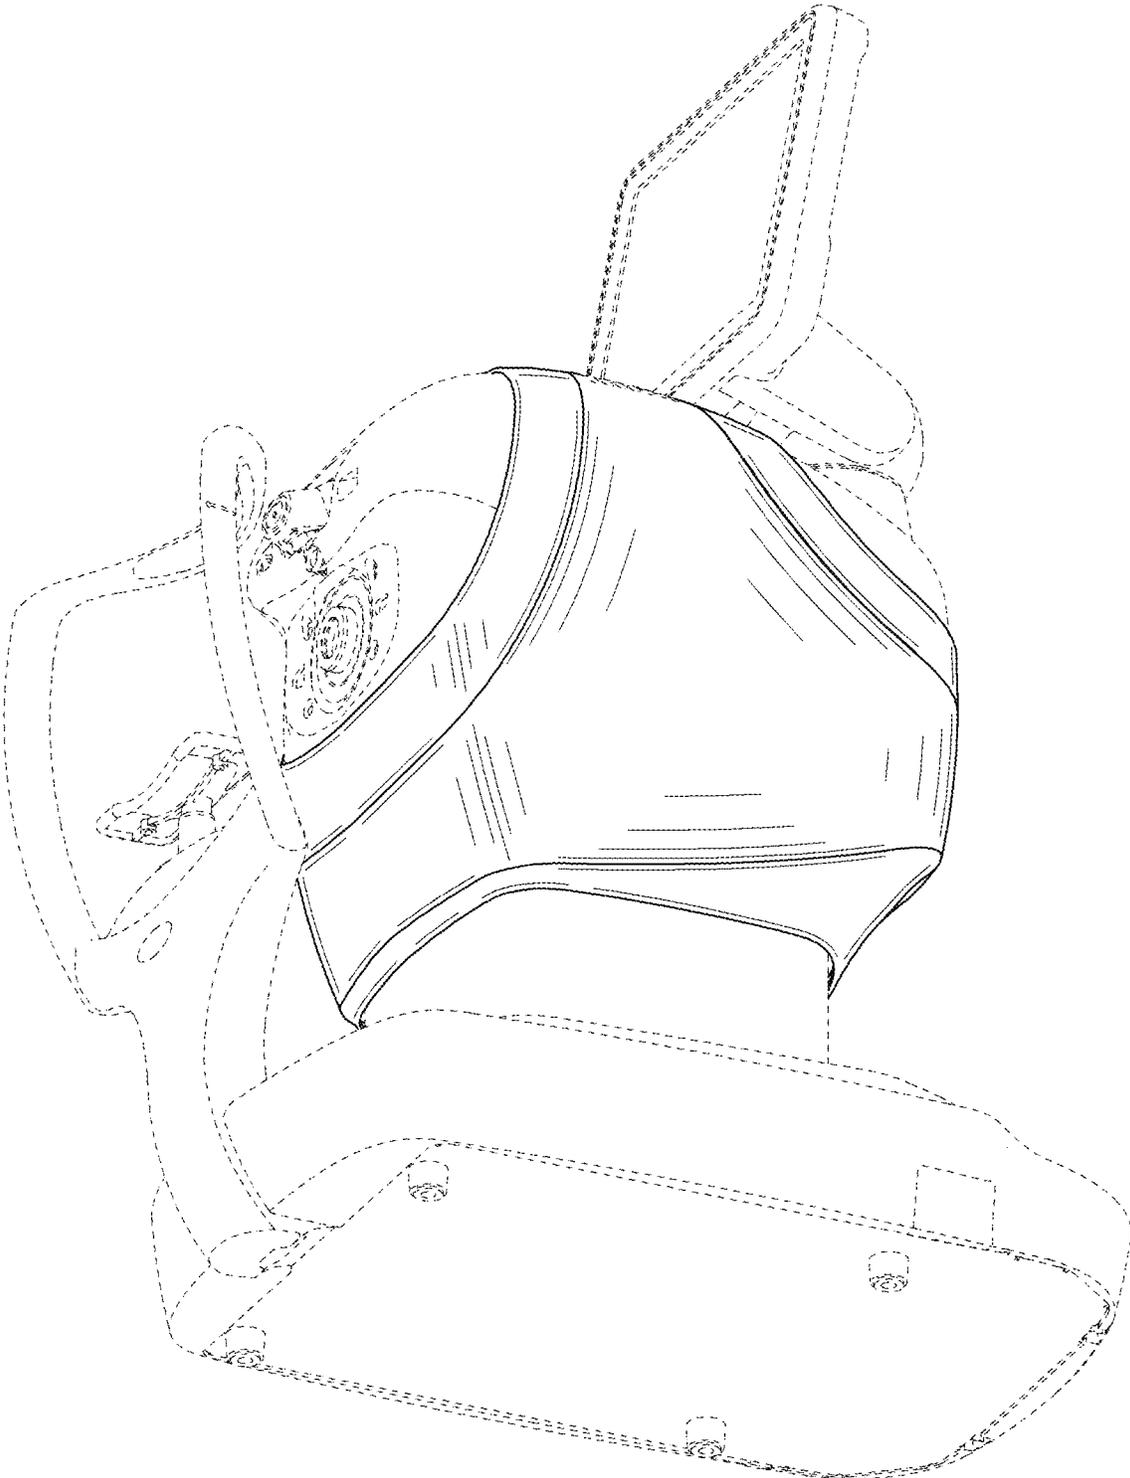


F I G. 3

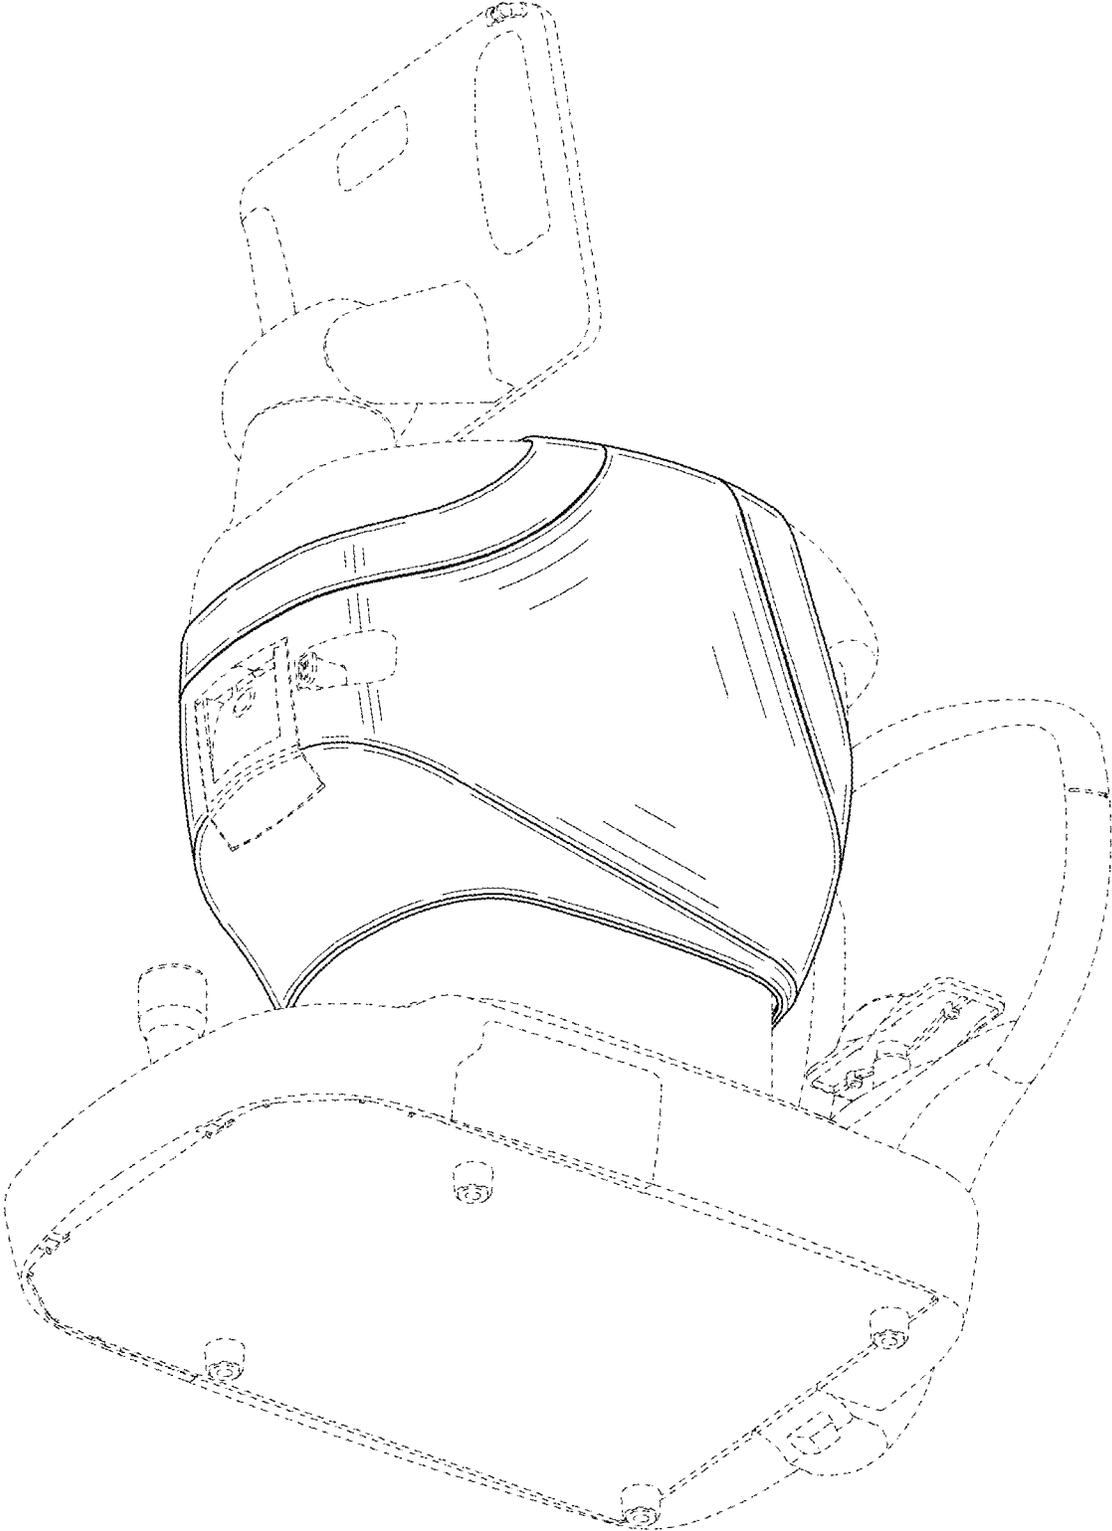

F I G. 4

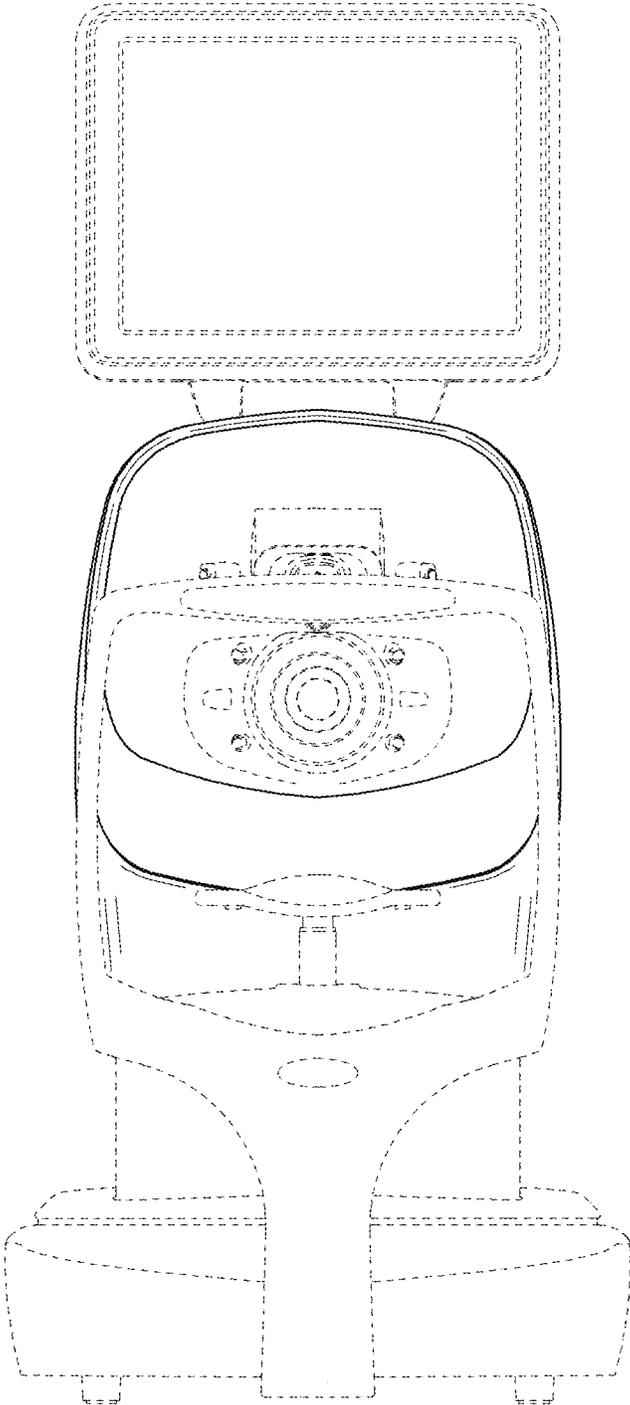

F I G. 5

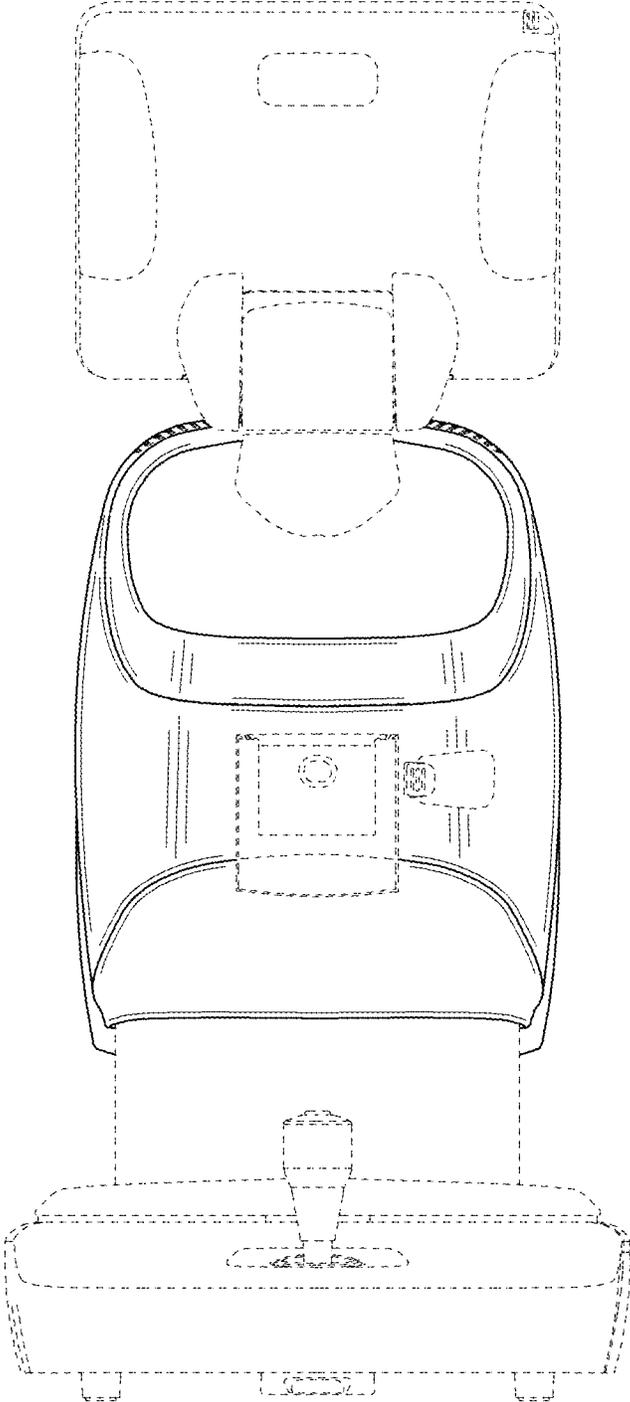

F I G. 6



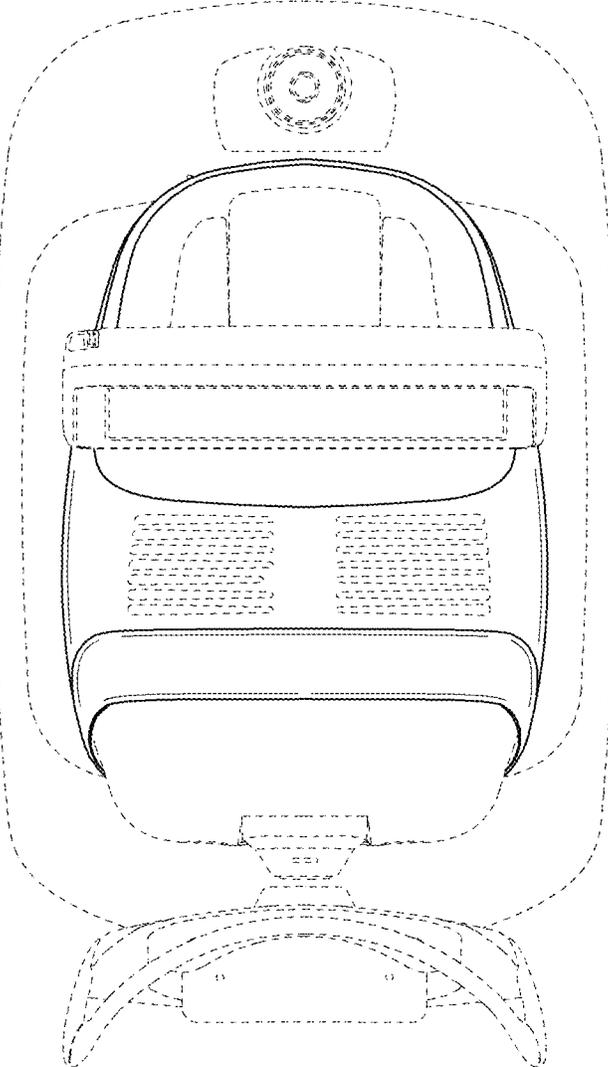



FIG. 7

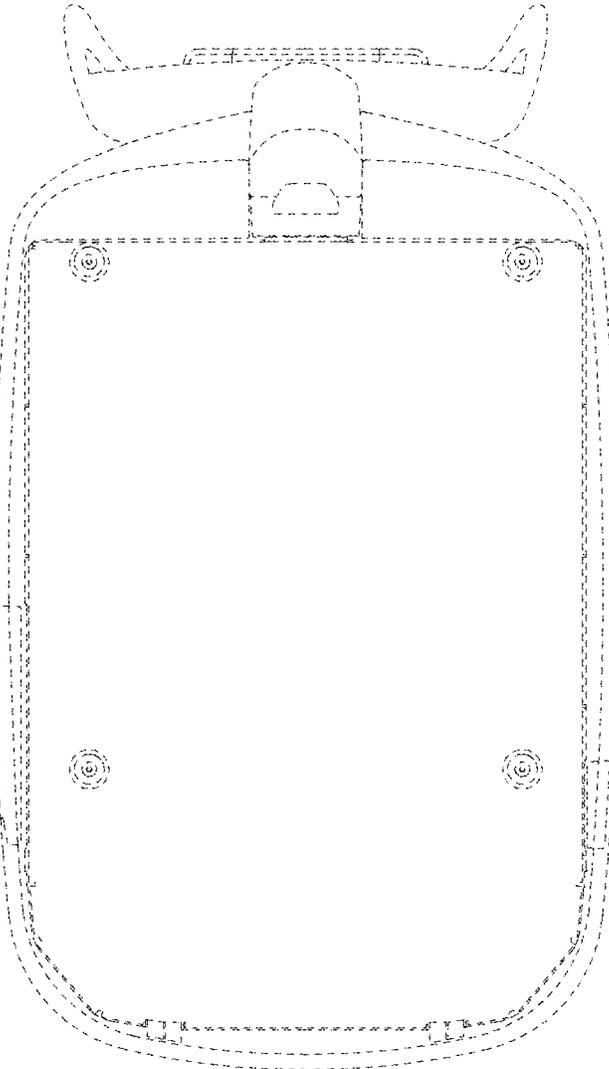

F I G. 8

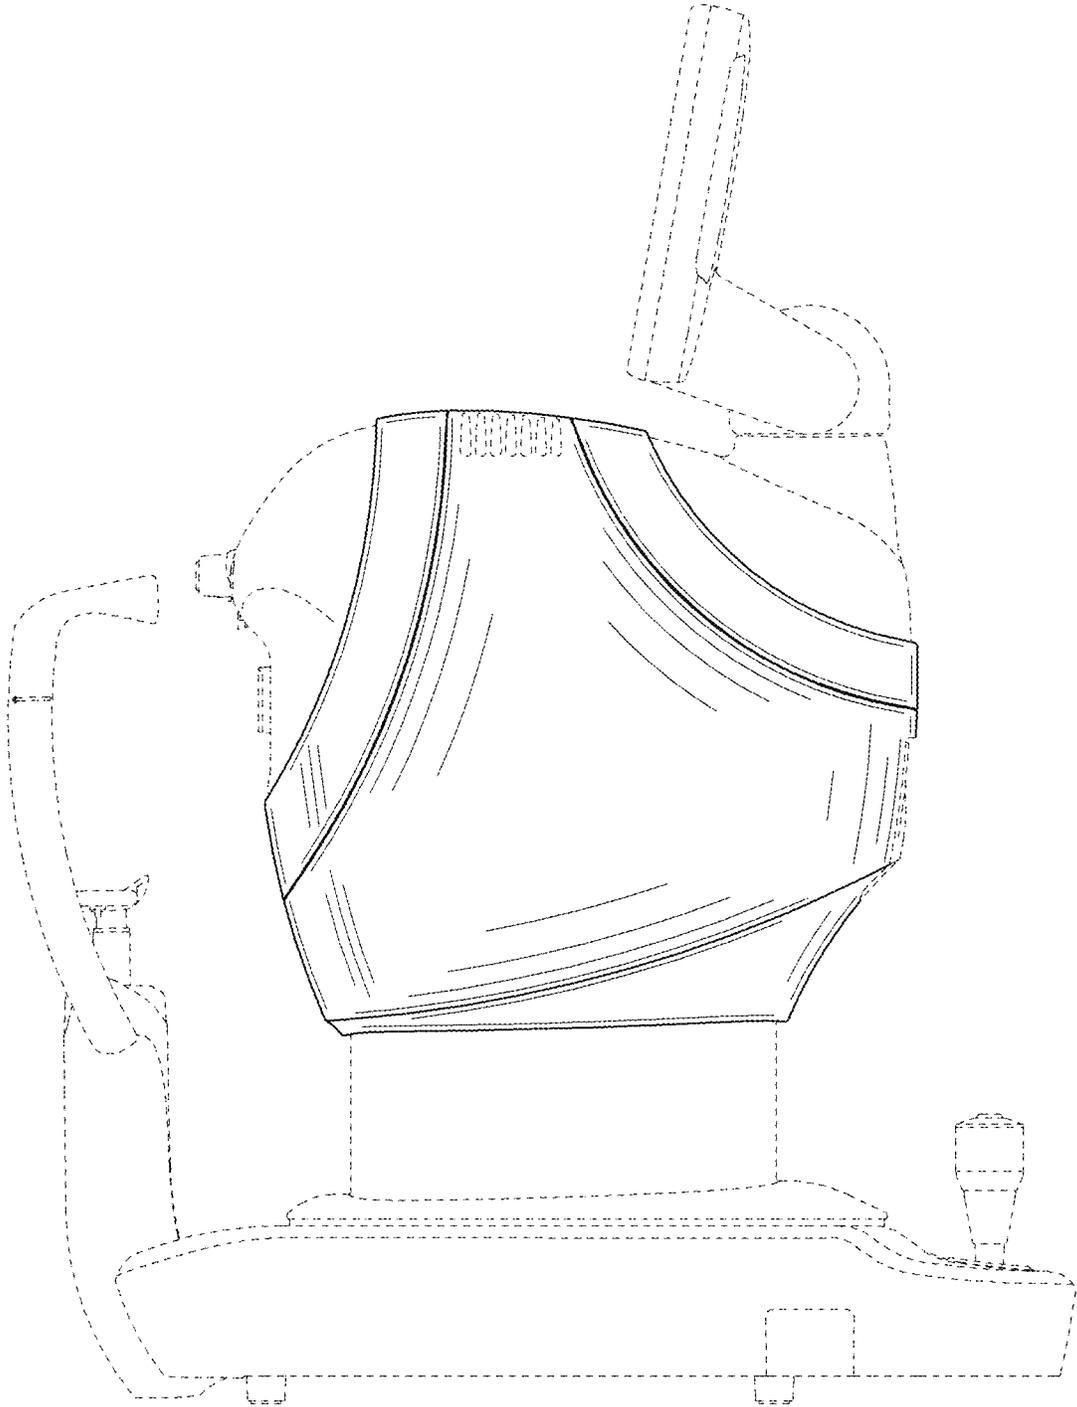

F I G. 9

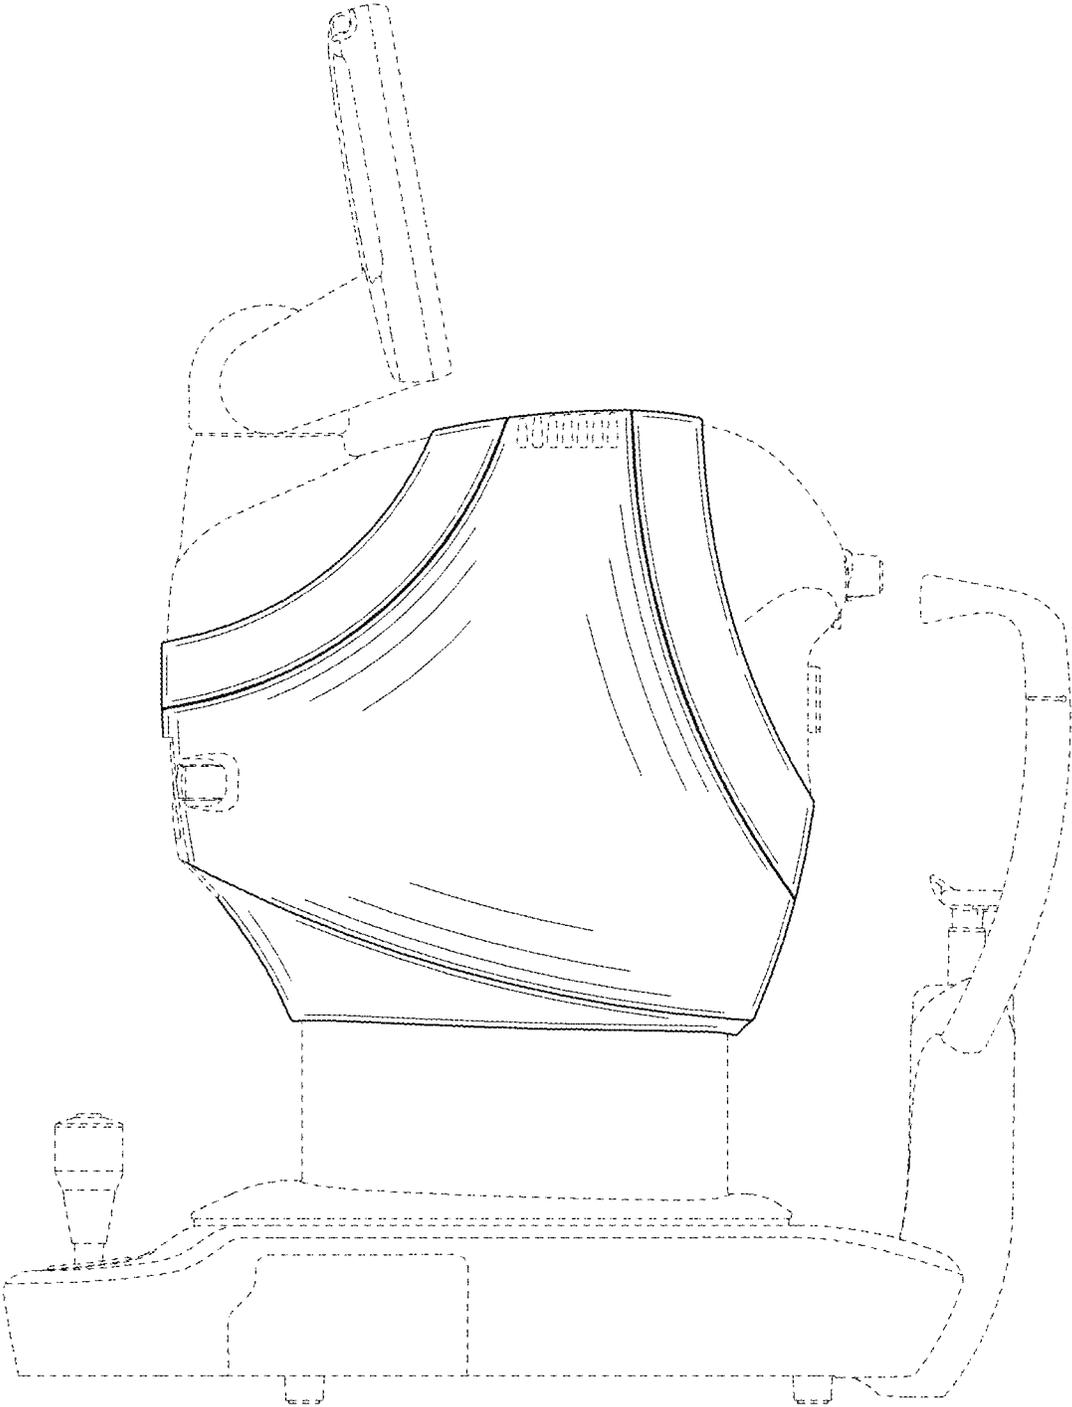

F I G. 10

