

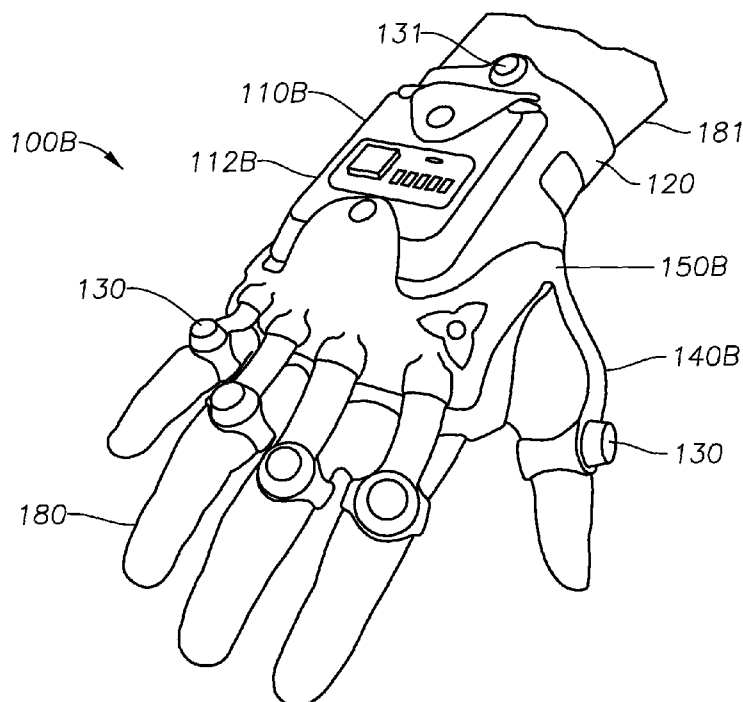


- (51) International Patent Classification:
A61H 1/00 (2006.01) *B25J 11/00* (2006.01)
A63B 23/16 (2006.01)
- (21) International Application Number:
PCT/US2013/040701
- (22) International Filing Date:
13 May 2013 (13.05.2013)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/645,682 11 May 2012 (11.05.2012) US
13/892,269 11 May 2013 (11.05.2013) US
- (71) Applicant: UNIVERSITY OF TENNESSEE RE-
SEARCH FOUNDATION [US/US]; UT Health Science
Center, 910 Madison Avenue, Suite 827, Memphis, TN
38163 (US).
- (72) Inventors: YU, Liu; University of Tennessee Health Sci-
ence Center, 910 Madison Avenue, Suite 827, Memphis,
TN 38163 (US). NELSON, Randall, J.; University of
Tennessee Health Science Center, 910 Madison Avenue,
Suite 827, Memphis, TN 38163 (US).

- (74) Agent: BREWER, Peter, L.; Baker Donelson, 265 Brook-
view Centre Way, Suite 600, Knoxville, TN 37919 (US).
- (81) Designated States (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,
NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU,
RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ,
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,
ZM, ZW.
- (84) Designated States (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
ML, MR, NE, SN, TD, TG).

[Continued on next page]

- (54) Title: PORTABLE HAND REHABILITATION DEVICE



(57) Abstract: A therapeutic device for improv-
ing voluntary control of paretic muscles in a pa-
tient extremity is provided. The therapeutic device
is designed to be portable and may be strapped
onto a patient's wrist or ankle. The device em-
ploys a plurality of micro-motors configured to
deliver vibratory sensations to a patient extremity
as somatosensory inputs. Each micro-motor is di-
mensioned to reside on a patient's respective fin-
ger or along their foot. The therapeutic device
also includes a micro-processor programmed to
actuate the micro-motors for designated times and
in pre-programmed sequences, and a housing con-
taining the micro-processor. A method of using
somatosensory input as a functional guidance to
improve motor function in a patient extremity is
also provided.

**Declarations under Rule 4.17:**

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))

— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

Published:

— with international search report (Art. 21(3))

PORTABLE HAND REHABILITATION DEVICE

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Serial No. 61/645,682 filed as a provisional application on May 11, 2012. That application was entitled “Portable Hand Rehabilitation Device,” and is incorporated herein in its entirety by reference.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

[0002] Not applicable.

THE NAMES OF THE PARTIES TO A JOINT RESEARCH AGREEMENT

[0003] Not applicable.

BACKGROUND OF THE INVENTION

Field of the Invention

[0004] The present invention relates to rehabilitative devices. More specifically, the invention relates to a portable device for enhancing motor function in paretic extremities, such as the hands of a stroke victim.

Technology in the Field of the Invention

[0005] Many individuals in the United States suffer from limited motor function in their extremities. This may be due to any of several causes. Some individuals may, for example, have suffered a stroke. The term “stroke” is a lay term that typically refers to a condition wherein the blood supply to an area of the brain is temporarily cut off. This is referred to as an “ischemic stroke.”

[0006] In an ischemic stroke, a clot interrupts blood flow to a part of the brain. When blood fails to get through the brain, the oxygen supply to the affected area is cut off, causing brain cells to die. The

longer the brain is without blood, the more severe the damage will be. Where the portion of the brain that controls movement of the upper extremities is damaged, the individual may be left in a state of partial paralysis, or paresis.

[0007] Some strokes are referred to as “hemorrhagic.” A hemorrhagic stroke occurs when a blood vessel in the brain itself ruptures. This produces bleeding into the brain matter, causing damage to surrounding brain cells.

[0008] Regardless of the type, stroke is the most common cause of disability in the United States. There are approximately 650,000 new and 180,000 recurrent strokes each year in the United States. About a quarter of stroke survivors are considered permanently disabled. Stroke patient rehabilitation is a billion dollar industry in the United States.

[0009] Individuals may also lose function in one or more extremities as a result of an injury. Such injuries may occur due to a car accident, a diving accident, a fall, or other trauma. In these instances, the individual’s cervical spine and nerves may be injured, again producing paresis in the hands. Additionally, such trauma can produce brain injury.

[0010] In addition to these events, some individuals may develop partial upper paralysis as a result of a medical condition. Examples of such conditions include amyotrophic lateral sclerosis (ALS), hypokalemic periodic paralysis, cerebral palsy, or other diseases. Finally, some individuals may suffer some degree of paresis due to brain injury caused by an explosion or accident incident to work or military duty.

[0011] When any of these conditions of partial paralysis occur, the individual is left with limited motor function in their arms. The most common disability among the numerous stroke survivors is weakness of the hand. Such individuals have difficulty performing routine tasks such as eating, turning off a light, manipulating a remote control, typing, or countless other activities that most people take for granted.

[0012] In many instances, individuals with limited motor function will undergo therapy. Such therapy may take place at a rehabilitation facility or at a medical office. Some patients undergo

expensive rehab through the use of so-called robots. Such therapy tends to be expensive. In other instances, a daily regimen of home-based rehabilitation is prescribed to achieve hand and finger functional recovery. However, home-based programs are sometimes limited by the motivation of the patient and the patient's desire or ability to use proper techniques.

[0013] Therefore, a need exists for a hand rehabilitation device that will efficiently improve hand function in stroke patients and injury victims at home or other remote location. Further, a need exists for a home-based device that provides somatosensory, or touch-based, signals as functional guidance during rehabilitation. Still further, a need exists for a portable device that does not rely upon percutaneous electrical stimulation or implant and that engages the patient's brain.

BRIEF SUMMARY OF THE INVENTION

[0014] A portable rehabilitation device for chronic neurological disorders, including stroke and traumatic brain injuries, is provided herein. The device is used for patient therapy to improve control of paretic muscles in a patient extremity.

[0015] In one embodiment, the therapeutic device comprises a plurality of micro-motors. Each micro-motor is configured to deliver a vibratory sensation to selected extremity points. An example of extremity points is the patient's fingers. The micro-motors provide vibratory input to the extremity points.

[0016] Each micro-motor is dimensioned to reside on a patient's respective finger or, in one embodiment, along the patient's foot or toes. In one arrangement, five micro-motors are provided for each device, representing the usual number of digits on a patient's hand. In another arrangement, twelve micro-motors are provided. These represent one micro-motor on the dorsal side of each finger, one micro-motor on the ventral side of each finger, and a micro-motor positioned on each of the dorsal and ventral sides of the patient's wrist.

[0017] The device also includes a power source. The power source is in electrical communication with each of the micro-motors. The power source may be, for example, one or more batteries or a USB cable. In the latter instance, the USB cable may be plugged into a portable processing unit such

as a laptop or a personal digital assistant. The processing unit, in turn, may be programmed to allow the patient or a health care provider to select a regimen of treatment to be delivered by the micro-motors.

[0018] The therapeutic device also includes a micro-processor, or controller. The micro-processor is programmed to actuate the micro-motors for designated times and sequences. The micro-processor may be pre-programmed to offer a variety of different times and sequences to increase patient interest and challenge. The micro-processor may communicate with each of the micro-motors through either a wired or through a wireless signal.

[0019] The device also includes a housing. The housing supports and protects the micro-processor and the batteries. The micro-processor may communicate with the batteries and the micro-motors through a printed circuit board. Where the micro-processor communicates with micro-motors wirelessly, then the housing will also include a transmitter for sending a wireless signal such as through the use of Blue Tooth or Wi-Max.

[0020] Preferably, the therapeutic device also has a power switch. The power switch allows the patient or a health care assistant to manually activate and de-activate the controller and micro-motors. This extends battery life. In addition, the therapeutic device also preferably includes a light source. The light source is arranged on the housing to deliver visual input to the patient when a micro-motor is vibrating.

[0021] In a preferred embodiment, each of the plurality of micro-motors is dimensioned to reside on a patient's finger. The device may then further include a glove for supporting each of the micro-motors adjacent to the patient's respective fingers. A strap may be provided for supporting the housing on the patient's wrist. The strap may be embedded in the glove. Alternatively, the housing is embedded in the glove itself without need of a separate strap. Alternatively still, no separate housing is used, but the micro-processor and associated electronics are embedded in the glove through so-called flex-electronics.

[0022] A method of using somatosensory input as a functional guidance to improve motor function in a patient extremity is also presented herein. In the method, the patient responds to both light and vibratory signals initiated by the controller. In this way, the patient receives somatosensory input guidance for motor tasks, requiring active brain engagement. Vibratory input combined with optional visual input provides go-cues and stop-cues for the patient.

[0023] The method includes securing a therapeutic device around a patient's wrist. The therapeutic device is constructed in accordance with the device described generally above, in its various embodiments. The method also includes initiating a first cycle of vibratory inputs from the micro-motors according to the programming of the micro-processor. The method then includes monitoring patient movement of the extremity points in response to the vibratory inputs of the respective micro-motors.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] So that the manner in which the present invention can be better understood, certain illustrations, charts, photographs and/or flow charts are appended hereto. It is to be noted, however, that the drawings illustrate only selected embodiments of the inventions and are therefore not to be considered limiting of scope, for the inventions may admit to other equally effective embodiments and applications.

[0025] Figure 1A is a perspective view of a portable hand rehabilitation device according to the present invention, in one embodiment. An illustrative control unit and glove are shown, along with wires extending from the control unit and into the glove.

[0026] Figure 1B is a perspective view of a portable hand rehabilitation device according to the present invention, in an alternate embodiment. An illustrative control unit and glove are again shown.

[0027] Figure 2A provides a pair of control units and wires of the rehabilitation device of Figure 1A. One unit is for a patient's left hand, while the other unit is for a patient's right hand. In both units, wires are seen extending from the control units to respective micro-motors.

[0028] Figure 2B provides a pair of control units and wires of the rehabilitation device of Figure 1B. One unit is for a patient's left hand, while the other unit is for a patient's right hand. In both units, wires are seen extending from the control units to respective micro-motors.

[0029] Figure 3A offers an exploded view of the control unit of Figure 2A. Selected components within the housing are seen, including a printed circuit board, a micro-controller, an LED and a pair of batteries.

[0030] Figure 3B offers an exploded view of the control unit of Figure 2B. Selected components within the housing are seen, including a printed circuit board, a micro-controller, a plurality of LED lights and a pair of batteries.

[0031] Figure 4 provides perspective views of a micro-motor, in one aspect. Four separate drawings are designated as "A," "B," "C," and "D."

[0032] The drawings designated as "A" and "B" represent the top and bottom portions of a micro-motor housing, respectively.

[0033] The drawing designated as "C" provides the bottom housing with a vibratory device resting therein.

[0034] The drawing designated as "D" shows the top and bottom portions of the housing connected together to form the micro-motor. The vibratory device and leads reside therein.

[0035] Figure 5 is a flow chart showing steps for performing a method for providing neuro-electrical stimulation of a patient's upper extremities, in one embodiment. The method uses somatosensory input as a functional guidance to improve motor function.

DETAILED DESCRIPTION OF CERTAIN EMBODIMENTS

[0036] **Figure 1A** is a perspective view of a portable rehabilitation device **100A** according to the present invention, in one embodiment. The device **100A** shown in the illustrative embodiment of **Figure 1A** generally includes a control unit **110A**. The control unit **110A** defines a micro-processor

(seen at **111** in **Figure 3A**) and associated circuitry held within a housing **112A**. The housing **112A**, in turn, is optionally secured to a patient's wrist (not shown) or other extremity using a strap **120** or other securing means.

[0037] In one embodiment the microprocessor is the MSP430F2013 provided by Texas Instruments, Inc. of Plano, Texas. However, any suitable microprocessor may be used that allows a patient to activate and control cycles for somatosensory inputs.

[0038] The rehabilitation device **100A** also includes a plurality of micro-motors **130**. The micro-motors **130** are transducers that convert electrical energy into mechanical energy. In one aspect, the micro-motors **130** are so-called coin vibration motors, such as the C1020B00F81 motor of Jinlong Machinery & Electronics Co. of Wenzhou, Zhejiang, China and Brooklyn, New York. In the view of **Figure 1A**, only a portion of one micro-motor **130** is visible, it being understood that the micro-motors **130** are embedded in the fingers of a glove **150A**.

[0039] The rehabilitation device **100A** further includes electrical wires **140**. The wires **140** transmit electric current from a battery (shown at **170** in **Figure 3A**) within the housing **112A** to each of the micro-motors **130**. Separate positive and negative wires extend from the housing **112A** to each of the micro-motors **130**. Electrical current is transmitted through the wires **140** according to signals sent by the microprocessor **111**.

[0040] In the arrangement of **Figure 1A**, the rehabilitation device **100A** is a hand rehabilitation device. This means that the rehabilitation device **100A** is configured to deliver somatosensory input to a patient's hand. In this instance, the strap **120** is configured and dimensioned to secure the housing **120** to a patient's wrist. This also means that the micro-motors **130** are placed along the patient's fingers.

[0041] To support the micro-motors **130** on the patient's fingers, a glove **150A** is provided. In the illustrative arrangement of **Figure 1A**, the glove **150A** is a right-hand glove. It is understood that a second hand rehabilitation device **100A** may be provided along with a left-hand glove (not shown). In either instance, the micro-motors **130** may be embedded within the glove **150A** along either the dorsal side or the ventral side of the patient's fingers.

[0042] It is noted that the term “finger” as used herein includes the thumb. It is also noted that the glove **150A** preferably leaves the finger tips exposed to enable mobility and to facilitate tactile sensation.

[0043] **Figure 2A** is a perspective view of a pair of hand rehabilitation devices **100A** (without gloves). Each device **100A** includes a control unit. One control unit, designated as **110A-L**, includes wires **130** configured to deliver signals to micro-motors **130** on a patient's left hand; a second control unit, designated as **100A-R**, includes wires **130** configured to deliver signals to micro-motors **130** on a patient's right hand. The micro-motors are individually designated as **132**, **133**, **134**, **135** and **136**. Micro-motors **132** are designed to reside within the glove **150A** adjacent to a patient's thumb (not shown), while micro-motors **133**, **134**, **135** and **136** are dimensioned to reside within the glove **150A** adjacent to the patient's four respective fingers (also not shown).

[0044] Control signals are provided from the control units **110A-L**, **110A-R** to the micro-motors **132**, **133**, **134**, **135**, **136** in pre-programmed sequences and for designated times. For example, a control signal may be sent to a first micro-motor, e.g., **132**, to cause it to vibrate for 10 seconds. During this time, the patient will respond to the vibratory input by wiggling, rotating, flexing, or otherwise exercising the extremity point corresponding to that micro-motor **132**. Thereafter, the signal is terminated. After a dead period of, for example, 4 seconds, a new control signal may be sent to a second micro-motor, e.g., **134**, to cause it to vibrate for 10 seconds; then, that control signal will be terminated and a new dead period of, say, 5 seconds will follow. This cycle may be continued for each micro-motor **132**, **133**, **134**, **135**, **136** until control signals have been sent to each micro-motor for, say, three cycles.

[0045] Each control unit **110A-L**, **110A-R** includes a housing **112A**. In the illustrative arrangement of **Figure 2A**, the housing **112A** has a generally rectangular profile. However, it is understood that the geometry of the housing **112A** is not significant so long as it is small enough to be portable and, preferably, to be worn immediately on an extremity. The extremity may be a wrist or ankle. The housing **112A** includes a base **114** having openings or slots **124**. The slots **124** receive and support the strap **120**.

[0046] The straps **120** in **Figure 2A** are ideally dimensioned to wrap around the patient's left and right wrists, respectively. The straps **120** will include any securing means (not shown) for securing the housings **112A** to the patient's respective wrists. Such securing means may be buckles, clips, hook-and-loop materials, snaps, magnets, or other items well known for securing clothing, bandages or straps.

[0047] Each rehabilitation device **100A** includes a light **104**. The light **104** may be, for example, a red light-emitting diode (LED). The LED light **104** comes on whenever a control signal is being sent from the control unit **110A** to a micro-motor **130**. Illumination of the light **104** indicates the occurrence of vibration generated by one of the five micro-motors **132, 133, 134, 135, 136**. The LED light **104** may be manually overridden (turned off) using a switch **106**. This allows vibratory input only to guide patient tasks.

[0048] Each rehabilitation device **100A** also includes a reset button **105**. The reset button **105** allows the patient or a health care assistant to restart vibration and light cycles for the devices **100A**.

[0049] **Figure 3A** offers an exploded view of the control unit **110A** of the devices **100A** of **Figure 2A**. Various components are seen, including the housing **112A**, the reset button **105** and the light **104A**.

[0050] **Figure 3A** also shows a power switch **160**. The power switch **160** allows the patient or a health care assistant to turn the rehabilitation device **100A** off when the device **100A** is not in operation. This, in turn, conserves battery power. The power switch **160** extends through an opening **1** in the housing **112A**.

[0051] The device **100A** runs on a power source. Preferably, the power source comprises one or more batteries, such as AA batteries **170**. In this way, the device **100A** is highly portable. However, the invention does not preclude the use of a power pack and power cord.

[0052] Various openings are provided in the housing **112A** of the device **100A**. Opening **115** accommodates the reset button **105**; opening **114A** accommodates the light **104A**; and opening **116A** accommodates the LED switch **106A**.

[0053] A printed circuit board **162** resides within the housing **112A**. The printed circuit board **162** provides electrical communication between various electrical components. Outputs **164** extend from the printed circuit board **162** to deliver control signals from the micro-processor **111** to the micro-motors **130**.

[0054] The printed circuit board **162** is supported by the base **114**. Openings **163** are provided along corners of the printed circuit board **162** for landing on corresponding sockets **113** in the base **114** and for receiving attachment screws (not shown). The base **114** includes the slots **124** for receiving the strap **120** of **Figure 1A**. The base **114** also includes a battery case **127** for receiving AA batteries **170**. Finally, the base **114** offers an opening **165** through which electrical leads **172**, **174** pass. The electrical leads **172**, **174** provide electrical communication between the batteries **170** and the printed circuit board **162**.

[0055] It is noted that in the arrangement of **Figure 3A**, the batteries **170** reside under the base **114**. A battery case cover **175** is provided to secure the batteries **170** in place under the base **114**. For purposes of this disclosure, such an arrangement is considered storing the batteries **170** within the housing **112A**.

[0056] **Figure 4** provides perspective views of a micro-motor **430**, in one aspect. Four separate drawings are designated as “A,” “B,” “C,” and “D.”

[0057] The drawings designated as “A” and “B” represent top **432** and bottom **434** portions of a micro-motor housing, respectively. The top **432** and bottom **434** portions are designed to mate together in order to form a shell for holding a vibratory device **436**.

[0058] The drawing designated as “C” shows the bottom portion **434** of the housing. Here, a vibratory device **436** has been placed therein. Wires **438** extend from the vibratory device **436** and out of the bottom portion **434** of the housing. In operation, the wires **438** will connect to the circuitry of the printed circuit board **162**.

[0059] The drawing designated as “D” shows the top **432** and bottom **434** portions of the housing connected together. This represents the complete micro-motor **430**. The micro-motor **430** may be, for

example, a so-called coin motor or pancake motor having a diameter of 8 to 16 mm and a thickness of 3 to 8 mm. The micro-motor **130** may have a rated voltage of about 1.5 to 5.0 volts, and an operational speed of about 5,000 to 20,000 rpm or, more preferably, 7,500 to 11,000 rpm.

[0060] The micro-motor **436** is intended to be in electrical communication with a controller, such as micro-processor **111**. As noted, a micro-processor **111** resides within the housing **112A** of the control unit **110A**. The micro-processor **111** is arranged to transmit signals to the micro-motors (shown in **Figure 2A** as micro-motors **132**, **133**, **134**, **135** and **136**) and the light **104A** in cycles. For example, a first vibratory signal may be sent to a first micro-motor **132**, and a first light signal may be simultaneously sent to the light **104A**. This causes the first micro-motor **132** and the light **104A** to illuminate simultaneously. The light **104A** will stay illuminated for as long as the first micro-motor **132** is vibrating, providing the patient with somatosensory input.

[0061] During this time, the patient will move the finger that is receiving vibrations from the first micro-motor **132**. Motion will continue for as long as the micro-motor **132** is vibrating and the light **104A** is illuminated. After a designated period of time, such as 5 seconds or 10 seconds, the signals will be discontinued, causing the first micro-motor **132** to no longer vibrate and causing the light **104A** to no longer illuminate. Thereafter, a short dead period will be introduced where no vibrations and no illumination take place. The patient will rest during the dead period, and await a next signal.

[0062] After the dead period, a next set of signals will be sent by the micro-processor **111**. For example, a second vibratory signal may be sent to micro-motor **136**, with a corresponding light signal being sent to the light **104A**. This new set of signals may take place for a period of, for example, three to eight seconds, during which time the patient will move or exercise the finger associated with micro-motor **136**. Thereafter, a second dead period will be introduced. Each dead period may be, for example, from 2 to 10 seconds or, more preferably, about 4 seconds.

[0063] It is noted that the light switch **106A** allows the patient or health care attendant to override the illumination of the light **104A** during vibration cycles. This introduces a level of difficulty to the patient during rehabilitation. The patient must then rely solely upon tactile sensation to know when to begin exercising an extremity part. To introduce further complexity, the micro-processor **111** may be

programmed such that vibratory periods are random as between the micro-motors **132**, **133**, **134**, **135**, **136**. Furthermore, the times for vibratory periods may be different, such that a first signal is, for example, 6 seconds; a second signal is 8 seconds; a third signal is 2 seconds; a fourth signal is 10 seconds; and a fifth signal is 5 seconds. Dead periods between these signals may also be varied, such as between 2 and 8 seconds. In this way, the patient is challenged to concentrate on the tactile and, optionally, visual stimulation for exercise.

[0064] The micro-processor **111** is pre-programmed to conduct a number of therapy cycles. In one aspect, the patient or physical therapist communicates with the micro-processor **111** through a so-called smart phone or a tablet, such as the iPhone[®] or the iPad[®] offered by Apple, Inc. of Cupertino, California. The communication may be through Bluetooth or other wireless communication system using an application on the smart phone or tablet. The application, or “App,” allows the patient or his or her therapist to select a cycle and a level of difficulty.

[0065] In one aspect, the degree of current to a particular micro-motor **130** may be varied. As the patient improves, the degree of current may be reduced, causing vibratory input to be more subtle. This further increases the level of difficulty.

[0066] The portable rehabilitation device **100A** of **Figure 1A** presents one embodiment for a rehabilitation device. In this embodiment, five micro-motors **130** are provided, with each micro-motor **130** arranged to provide vibratory stimulation to a selected finger. However, additional micro-motors **130** may be provided to increase stimulation.

[0067] **Figure 1B** is a perspective view of a portable rehabilitation device **100B** according to the present invention, in an alternate embodiment. The device **100B** shown in **Figure 1B** represents a more advanced embodiment. Here, two micro-motors **130** are placed along each finger **180**, preferably on the dorsal side and on the ventral side of each finger **180**. In addition, two micro-motors **131** are placed along a wrist **181**, with one micro-motor **131** being on the dorsal side and the other being on the ventral side of the wrist **181**. In this way stimuli may be delivered not only to the fingers **180**, but also to the wrist **181**. Stimuli are delivered on each side of the fingers and wrist to increase somatosensory input.

[0068] As with the device **100A**, the portable rehabilitation device **100B** shown in **Figure 1B** includes a control unit **110B**. The control unit **110B** defines a micro-processor (seen at **111** in **Figure 3B**) and associated circuitry held within a housing **112B**. The housing **112B**, in turn, is secured to the patient's wrist **181** (or, alternatively, ankle) using a brace **120B** or other securing means.

[0069] In one embodiment the microprocessor is the MSP430-F2013 provided by Texas Instruments, Inc. of Plano, Texas. This is an ultra-low power controller that features a 16-bit RISC CPU, 16-bit registers, and constant generators that contribute to code efficiency. A digitally controlled oscillator (DCO) allows wake-up from low-power modes to active mode in less than 1 μ s. However, any suitable micro-processor may be used that allows a patient to activate and control cycles for somatosensory input.

[0070] As noted, the rehabilitation device **100B** also includes a plurality of micro-motors **130**. The micro-motors **130** may be designed in accordance with the micro-motors **130** / **430** described above in connection with **Figures 2A** and **4**. In this respect, the micro-motors **130** are transducers that convert electrical energy into mechanical energy. Cycles of mechanical energy are generated by the micro-motors **130**, forming vibrations.

[0071] The rehabilitation device **100B** further includes electrical wires (seen at **140** in **Figure 2B**). The wires **140** transmit electric current from batteries (shown at **170** in **Figure 3B**) within the housing **112B** to each of the micro-motors **130**. In the arrangement of **Figure 1B**, the wires **140** are encased within insulated channels of a glove **150B**. Electrical current is transmitted through the channels according to signals sent by the micro-processor **111**.

[0072] It is noted here that the glove **150B** of **Figure 1B** covers only a portion of the hand and fingers. In this instance, the glove **150B** is really more of a skeleton. The skeleton design increases comfort to the patient and is easier to don and doff. For purposes of the present disclosure, the term "glove" includes any support structure for carrying a hand rehabilitation device **100B**. Preferably, the support structure includes an elastic material that is sewn into a middle posterior portion of the glove **150B**. This allows more of a "one size fits all" or "two sizes fits all" approach.

[0073] **Figure 2B** is a perspective view of a pair of hand rehabilitation devices **100B**. Each device **100B** includes a micro-processor (seen at **111** in **Figure 3B**). The micro-processors **111** reside within

and are part of a control unit. One control unit, designated as **110B-L**, includes wires **140** configured to deliver vibratory signals to micro-motors **130** on a patient's left hand; a second control unit, designated as **110B-R**, includes wires **130** configured to deliver vibratory signals to micro-motors **130** on a patient's right hand. The micro-motors are individually designated as **132**, **133**, **134**, **135** and **136**. Micro-motors **132** are designed to reside along the glove **150B** adjacent to a patient's thumb (not shown in **Figure 2B**), while micro-motors **133**, **134**, **135** and **136** are dimensioned to reside within the glove **150B** adjacent to the patient's fingers (also not shown).

[0074] It is noted in the arrangement of **Figure 2B** that the micro-motors **132**, **133**, **134**, **135**, **136** are arranged in pairs. As discussed above, the micro-motors are arranged in pairs so that mechanical stimuli may be beneficially delivered to a patient's fingers on opposing sides of each respective finger.

[0075] Signals are provided from the micro-processors **111** in the control units **110B-L**, **110B-R** to the micro-motors **132**, **133**, **134**, **135**, **136** in pre-programmed sequences and for designated times. For example, a control signal may be sent to a first micro-motor pair, e.g., **132**, to cause the pair to vibrate for 10 seconds. During this time, the patient will wiggle, rotate, flex, or otherwise exercise the finger associated with the micro-motor pair. Thereafter, the signal is terminated. After a dead period of, for example, 4 seconds, a new control signal may be sent to a second micro-motor pair, e.g., **135**, to cause the micro-motors to vibrate for 10 seconds; then, that control signal will be terminated and a new dead period of, for example, 6 seconds will follow. This cycle may be continued for each micro-motor pair **132**, **133**, **134**, **135**, **136** until control signals have been sent to each micro-motor pair for, say, five cycles.

[0076] As noted, each micro-processor, or controller **111**, resides within a housing **112B**. In the illustrative arrangement of **Figure 2B**, the housing **112B** has a generally rectangular profile. However, it is understood that the geometry of the housing **112B** is not significant so long as it is small enough to be portable and, preferably, to be worn immediately on an extremity. The extremity may be a wrist or ankle. The housing **112B** includes a base **114** and may have openings or slots **124** that receive a strap **120**. More preferably, the housing **112B** is embedded into the brace **120** for the device **100B** as shown in the embodiment of **Figure 1B**.

[0077] The rehabilitation devices **100B-L** and **100B-R** include the light **104A** and the override switch **106A** as described above in connection with **Figure 2A**. However, the rehabilitation devices **100B-L**, **100B-R** also include a bank of lights **104B**. The individual lights in the bank of lights **104B** may also be, for example, red light-emitting diodes (LED's). Each LED light **104B** corresponds to a micro-motor pair **130**. In addition, an override switch **106B** is provided for each light in the bank of lights **104B**.

[0078] In the rehabilitation device **100B**, the patient is presented with a choice of using no lights, using one light **104A**, or using the bank of lights **104B**. When using the bank of lights **104B**, the patient has the choice of overriding one, two, three or four of the lights **104B** using switches in a bank of override switches **104B**.

[0079] Where the patient chooses to use only the single light **104A** in a rehabilitation device **110B**, the patient will turn the switches in the bank of override switches **106B** to an "off" position. This overrides the lights in the bank of lights **104B** to keep them from being illuminated when control signals are sent to a micro-motor **130**. The rehabilitation devices **100B-L**, **100B-R** then operate in the same manner as described above for the rehabilitation devices **100A-L**, **100A-R**. Somatosensory input will include illumination of single lights **104A** in the rehabilitation devices **110B** when any micro-motor **130** is vibrating.

[0080] Where the patient chooses to use the lights in the bank of lights **104B**, the patient will turn the single switch **106A** in each rehabilitation device **100B-L**, **100B-R** to an "off" position. This overrides the single lights **104A** and keeps them from illuminating when control signals are being sent to the pairs of micro-motors **130**. The rehabilitation devices **100B-L** and **100B-R** then offer visual input for the patient in the form of either sequenced or random illumination of selected lights in the bank of lights **104B**.

[0081] In operation, an LED light in the bank of lights **104B** is illuminated when a control signal is sent from the micro-processor **111** to a selected pair of micro-motors **130**. Stated another way, illumination of a light **104B** indicates the occurrence of vibration generated by one of the five micro-

motor pairs **132, 133, 134, 135, 136**. Of interest, the illuminated light corresponds in position in the housing **112B** to a micro-motor pair **130**.

[0082] It is again noted that selected lights in the bank of lights **104B** may be turned off by turning a corresponding override switch in the bank of switches **106B** to an "off" position. This allows only vibratory input, increasing the level of challenge to the patient in his or her rehabilitation process.

[0083] Each rehabilitation device **100B** also includes a reset button **105**. The reset button **105** allows the patient or a health care assistant to restart vibration and light cycles for the devices **100B**.

[0084] **Figure 3B** offers an exploded view of a control unit **110B** of the devices **100B** of **Figure 2B**. Various components are seen, including the micro-processor **111**, the reset button **105** and the lights **106A, 106B**. Additional features include the power switch **160** and the batteries **170**. Still additional features include opening **115** for the reset button **105**; opening **114A** for the single light **104A**; and opening **116A** for the single LED switch **106A**. Additional openings include openings **114B** for the bank of lights **104B** and openings **116B** for the bank of override switches **106B**.

[0085] Additional features of the control unit **110B** are generally in accordance with the control unit **110A**, except for offering the bank of lights **104B** and the bank of override switches **106B**, and except for the use of micro-motor pairs **132, 133, 134, 135, 136**. Accordingly, additional details concerning the control unit **110B** need not be repeated. However, it is noted that dorsal and ventral micro-motors may optionally be separately programmed during for exercise.

[0086] The rehabilitation devices **100A, 100B** operate to improve motor function in a patient by providing vibratory stimulation in the fingers along with visual prompting. Medical research in the neurosciences field suggests that physical stimulation improves somatosensory input, which in turn enhances motor recovery in stroke patients. Further, using vibration as a trigger (go cue), the devices facilitate brain engagement, which is believed to be more efficient in promoting motor recovery than using somatosensory input as passive stimulation only.

[0087] Studies have suggested that somatosensory-related activation levels in SI are modulated by the context within which tactile stimuli are delivered. Vibro-tactile stimuli may be active or may be

passive. Vibro-tactile stimuli presented during active frequency discrimination are associated with enhanced SI activity when compared to that elicited by passive vibro-tactile input. Active use of the combination of tactile and visual stimuli enhances attentional control over perceptual selection. It is believed that activity of SI neurons differs, depending on functional significance of somatosensory inputs.

[0088] It has been observed by the applicants herein that hand/wrist movements that are guided by somatosensory inputs initiate faster and reach target with greater success rates when compared with movements guided by visual input alone. Therefore, the present invention employs somatosensory inputs as active guidance of motor tasks in the form of a portable device. In contrast to expensive robot-aided therapy that is usually offered in rehabilitation centers, the devices herein offer a portable, cost-efficient instrument for long-term home-based rehabilitation.

[0089] During hand rehabilitation, the housing will be attached to the patient's wrist. The micro-motors will be positioned along individual fingers, wrists and/or palmar pads. The controller is programmed to provide a timing and sequence of vibrations among the micro-motors that enables improved motor function. The controller may be re-programmed as needed to offer increased challenge to the patient during recovery. In one aspect, current is reduced to decrease the level of vibratory stimulation, thereby increasing the challenge to the patient during rehabilitation.

[0090] The vibro-somatosensory inputs delivered by the micro-motors can be used as the go-cue and/or stop signal, depending on the design of the rehabilitation task. The vibratory inputs can also serve as a somatosensory feedback when coupled with hand movements for stroke victims.

[0091] The therapeutic device described herein provides an active functional task-guidance during rehabilitation to mobilize a larger number of neural elements. Such neural elements may include both central and peripheral structures to facilitate hand function. The device emphasizes patients' attention during rehabilitation, which is important in effective functional recovery of a deficit hand. The device may be applied to the lower extremity of the patient as well. In this instance, the glove may be modified to serve as a sock.

[0092] In one aspect, the housing includes a USB connection that allows data gathered concerning use of the device to be uploaded to a computer as a digital file. Uploading may take place, for example, at a doctor's office or a rehabilitation center. Alternatively, uploading may be done on a patient's computer or hand-held device, and then sent via electronic mail to a health care provider. This confirms that the rehabilitation device is actually being used by the patient and helps the provider, the carrier, or CMS establish benchmarks. In one aspect, the USB connection also allows the micro-processor to be re-programmed to create different sequences of vibratory and/or light sequences.

[0093] **Figure 5** is a flow chart showing steps for performing a method **500** for providing neuro-electrical stimulation of a patient's upper extremities, in one embodiment. The method **500** uses somatosensory input as a functional guidance to improve motor function.

[0094] In one embodiment, the method **500** first includes attaching a therapeutic device to a patient's extremity. This is seen in Box **510**. The extremity is preferably the patient's wrist, but may alternatively be an ankle. The therapeutic device is arranged such that at least one micro-motor is placed along a corresponding patient digit (or extremity point). Where the therapeutic device is attached to the patient's wrist, the micro-motors will be placed along the fingers (including the thumb).

[0095] In one aspect, the micro-motors are positioned in pairs. This means that micro-motors are placed on opposing sides of a patient's respective fingers. This increases the tactile stimuli to the patient.

[0096] The method **500** next includes activating the therapeutic device. This is provided in Box **520**. Activating the therapeutic device generates a sequence of control signals that are sent to the various micro-motors. The micro-motors, in turn, vibrate to deliver vibratory somatosensory inputs to the patient. Activating the therapeutic device may be done by pressing a reset button.

[0097] The control signals are sent by a micro-processor as discussed above. Times for delivering control signals may be adjusted, and times for dead periods between control signals may vary.

[0098] The method **500** further includes the optional step of turning a switch to an "on" position. This is indicated at Box **530**. When the switch is in the "on" position, a light is illuminated during the

time that a micro-motor is vibrating. In this way, the patient also receives visual as well as somatosensory inputs.

[0099] The method **500** also comprises monitoring patient movement of digits in response to the vibratory and optional visual inputs. This is seen at Box **540**. Monitoring may mean assistance and encouragement offered by a physical therapist or attendant. Alternatively or in addition, monitoring may mean evaluation by the patient himself or herself. Alternatively or in addition, monitoring may mean recording therapy cycles and transmitting those to a health care provider or an insurance entity.

[00100] The method **500** also includes resetting the therapeutic device. This is shown at Box **550**. Resetting the therapeutic device initiates a new cycle of vibratory and, optionally, visual inputs. The new cycle of vibratory inputs provides a different sequence of control signals, a different duration of control signals, or both. Resetting may also be done by pressing a reset button.

[00101] Optionally, the method **500** includes selecting lights from a bank of lights on the therapeutic device. This is given at Box **560**. The selected lights will illuminate when a corresponding micro-motor is vibrating.

[00102] While it will be apparent that the inventions herein described are well calculated to achieve the benefits and advantages set forth above, it will be appreciated that the inventions are susceptible to modification, variation and change without departing from the spirit thereof.

CLAIMS

1. A portable therapeutic device for improving voluntary control of paretic muscles in a patient extremity, comprising:
 - a plurality of micro-motors configured to deliver a vibratory sensation to selected patient extremity points as vibratory inputs;
 - a housing;
 - a light source arranged on the housing to deliver visual input to the patient when a micro-motor is vibrating;
 - a micro-processor residing within the housing and programmed to send control signals to actuate the micro-motors and light source for designated times and sequences in order to form cycles of somatosensory inputs;
 - a manual override switch for selectively preventing the light source from illuminating during cycles of somatosensory inputs; and
 - a reset button for initiating a new cycle of somatosensory inputs in response to manual resetting.
2. The therapeutic device of claim 1, further comprising:
 - one or more batteries residing within the housing for providing power; and
 - a power switch for manually activating and de-activating power to the micro-processor.
3. The therapeutic device of claim 1, wherein:
 - the extremity points are fingers such that each of the plurality of micro-motors is dimensioned to reside on a patient's finger; and
 - the device further comprises a glove for supporting each of the micro-motors adjacent to the patient's respective fingers.
4. The therapeutic device of claim 1, wherein:
 - each of the plurality of micro-motors is dimensioned to reside on a patient's foot; and

the device further comprises a sock for supporting each of the micro-motors along the patient's foot.

5. The therapeutic device of claim 1, wherein the controller communicates with each of the micro-motors through either a wired or a wireless signal.

6. The therapeutic device of claim 1, wherein:
the cycles of somatosensory inputs comprise at least a first cycle and a second cycle; and
the second cycle of vibratory inputs provides a different sequence of control signals, a different duration of control signals, or both, relative to the first cycle.

7. The therapeutic device of claim 1, wherein:
the extremity points are fingers such that each of the plurality of micro-motors is dimensioned to reside on a patient's finger;
the plurality of micro-motors comprises pairs of micro-motors such that a pair of micro-motors resides on opposing sides of each of the patient's fingers;
the device further comprises a pair of micro-motors placed on the dorsal and ventral sides of the patient's wrist, respectively; and
the cycles of somatosensory inputs comprise cycles of vibratory and light inputs delivered and corresponding to the patient's fingers and wrist.

8. The therapeutic device of claim 1, wherein:
the housing containing the light source, the micro-processor and the batteries defines a control unit; and
the control unit is dimensioned to reside along the patient's wrist.

9. The therapeutic device of claim 1, further comprising:
a glove for supporting each of the micro-motors adjacent to the patient's respective fingers.

10. The therapeutic device of claim 9, wherein the control unit is embedded into the glove proximate the patient's wrist.
11. The therapeutic device of claim 7, further comprising:
 - a bank of lights corresponding to the pairs of micro-motors such that a light is illuminated when a control signal is sent to vibrate a corresponding pair of micro-motors.
12. The therapeutic device of claim 11, further comprising:
 - a bank of override switches having switches that correspond to the lights in the bank of lights and to the pairs of micro-motors for selectively preventing a light from illuminating during cycles of somatosensory inputs.
13. The therapeutic device of claim 11, further comprising:
 - a memory for storing patient use events.
14. A method of using somatosensory input as a functional guidance to improve motor function in a patient extremity, comprising:
 - securing a therapeutic device around a patient's wrist, the therapeutic device comprising:
 - a plurality of micro-motors configured to deliver a vibratory sensation to a patient extremity points as vibratory inputs, with each micro-motor being dimensioned to reside on a patient's respective finger,
 - a housing,
 - a light source arranged on the housing to deliver visual input to the patient when a micro-motor is vibrating, and
 - a micro-processor residing within the housing and programmed to send control signals to actuate the micro-motors and light source for designated times and sequences in order to form cycles of somatosensory inputs;
 - initiating a first cycle of vibratory inputs from the micro-motors according to the programming of the micro-processor; and

monitoring patient movement of the extremity points in response to the vibratory inputs of the respective micro-motors.

15. The method of claim 14, further comprising:

pressing a reset button on the housing in order to initiate a second cycle of vibratory inputs after completing the first cycle.

16. The method of claim 14, further comprising:

placing an override switch along the housing in an “on” position so that the light source illuminates when a micro-motor is vibrating; and

receiving visual feedback from the light source during the first cycle;

and wherein the therapeutic device further comprises:

one or more batteries residing within the housing for providing power, and

a power switch for manually activating and de-activating power to the micro-processor.

17. The method of claim 16, wherein:

the therapeutic device further comprises a glove for supporting each of the micro-motors adjacent to the patient’s respective fingers;

the cycles of somatosensory inputs comprise at least a first cycle and a second cycle; and

the second cycle of vibratory inputs provides a different sequence of control signals, a different duration of control signals, or both, relative to the first cycle.

18. The method of claim 16, wherein:

the plurality of micro-motors comprises pairs of micro-motors such that a first pair of micro-motors resides on opposing sides of each of the patient's fingers;

the device further comprises a pair of micro-motors placed on the dorsal and ventral sides of the patient's wrist, respectively; and

the cycles of somatosensory inputs comprise cycles of vibratory inputs delivered to the patient's fingers and wrist.

19. The method of claim 18, wherein:

the therapeutic device further comprises a bank of lights corresponding to the pairs of micro-motors such that a light is illuminated when a control signal is sent to vibrate a corresponding pair of micro-motors, and a bank of override switches having switches that correspond to the lights in the bank of lights and to the pairs of micro-motors for selectively preventing a light from illuminating during cycles of somatosensory inputs; and

the method further comprises placing at least one of the override switches along the bank of switches in an “on” position so that the light sources corresponding to that at least one override switch illuminate when corresponding micro-motors are vibrating; and

receiving visual feedback from the corresponding light sources during the first cycle.

20. A portable therapeutic device for improving voluntary control of paretic muscles in a patient's upper extremity, comprising:

a plurality of micro-motors configured to deliver a vibratory sensation to the patient's fingers as vibratory inputs, wherein the micro-motors are arranged in pairs placed along opposing sides of each finger;

a glove dimensioned to fit onto the patient's hand and supporting each of the micro-motors adjacent to the patient's respective fingers;

a light source placed along the glove to deliver visual input to the patient when a micro-motor is vibrating;

a micro-processor embedded in the glove and programmed to send control signals to actuate the micro-motors and light source for designated times and sequences in order to form cycles of somatosensory inputs;

a manual override switch for selectively preventing the light source from illuminating during cycles of somatosensory inputs; and

a reset button for initiating a new cycle of somatosensory inputs in response to manual resetting.

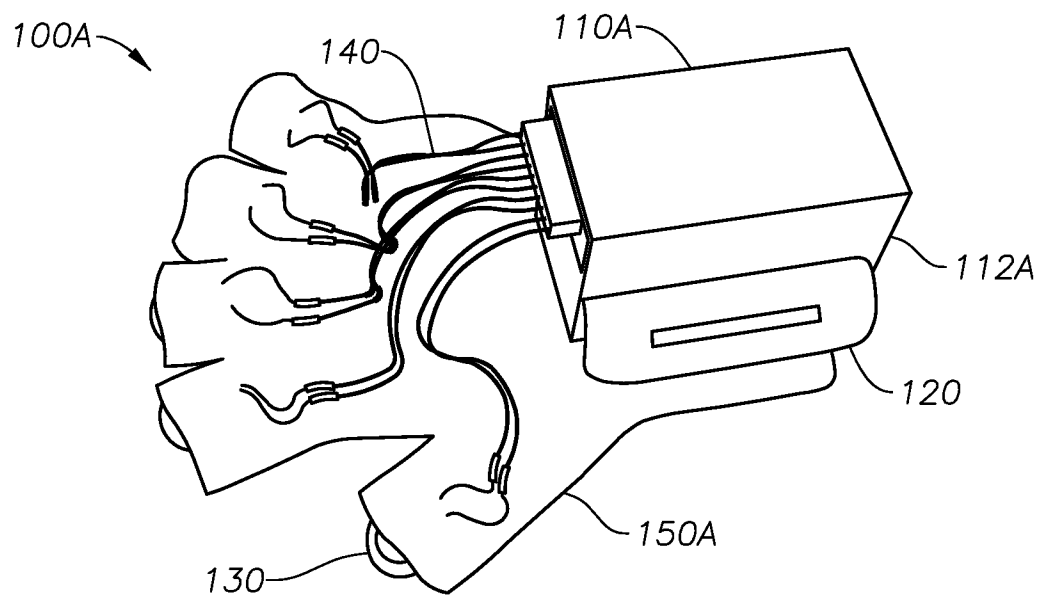
$1/8$ 

FIG. 1A

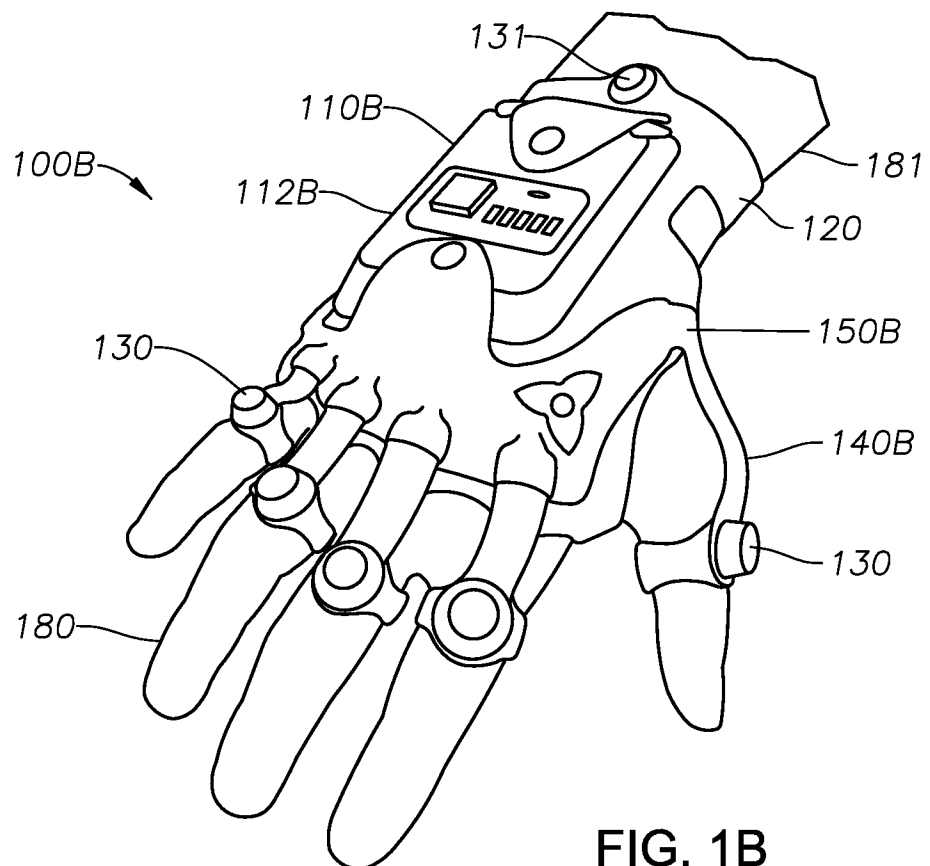


FIG. 1B

2/8

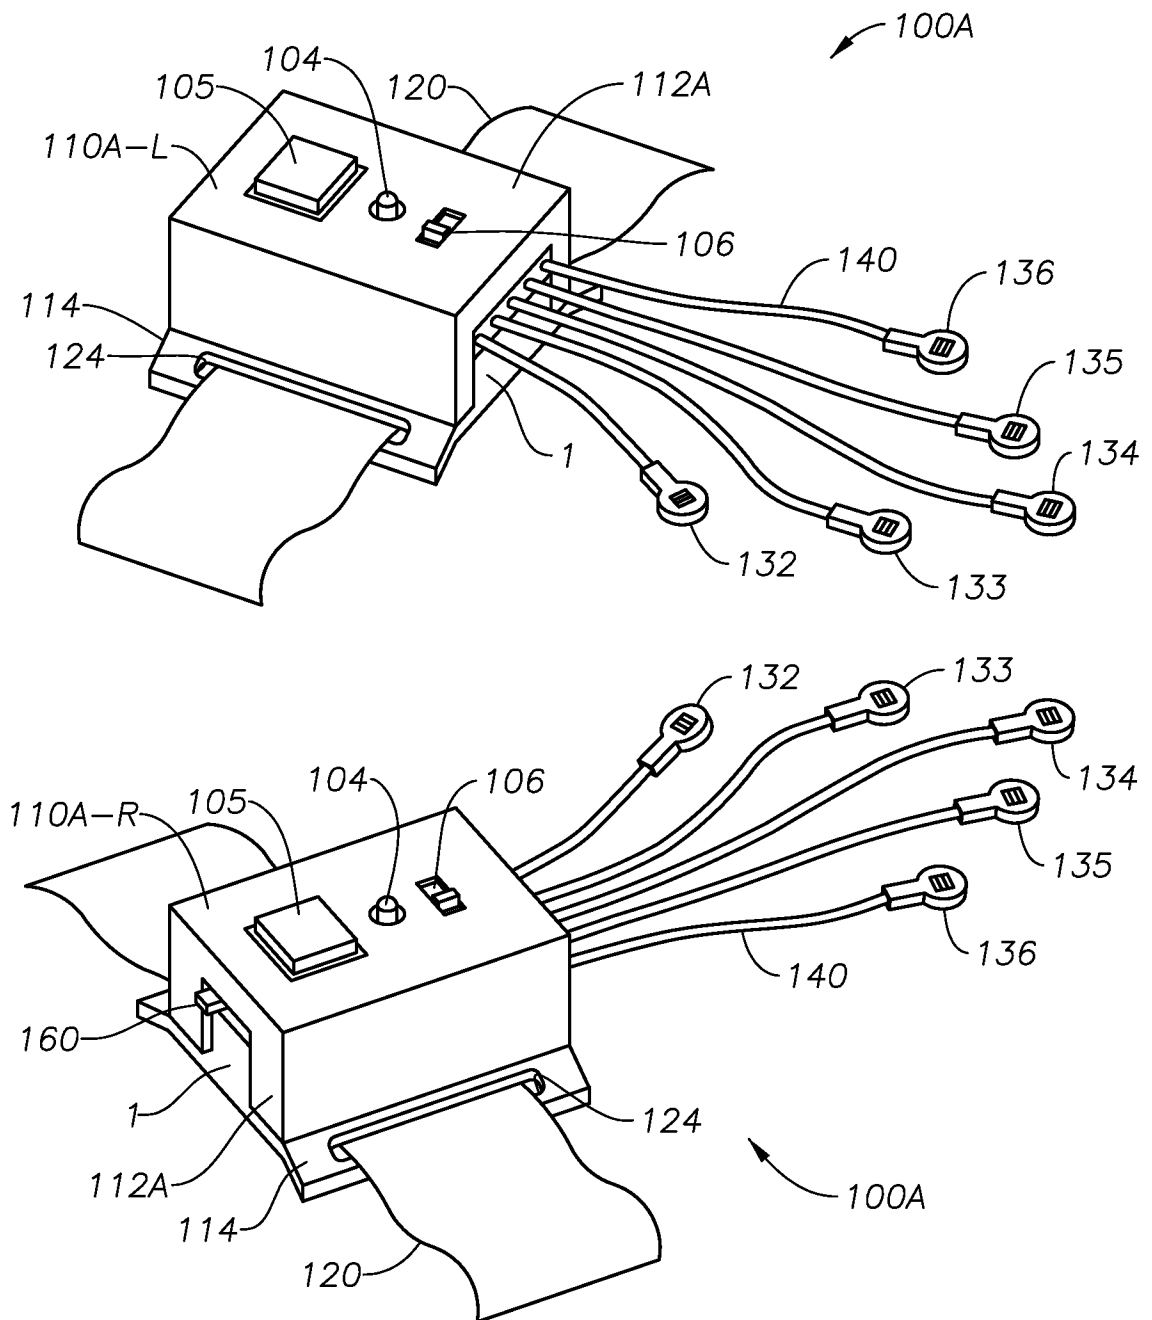


FIG. 2A

3/8

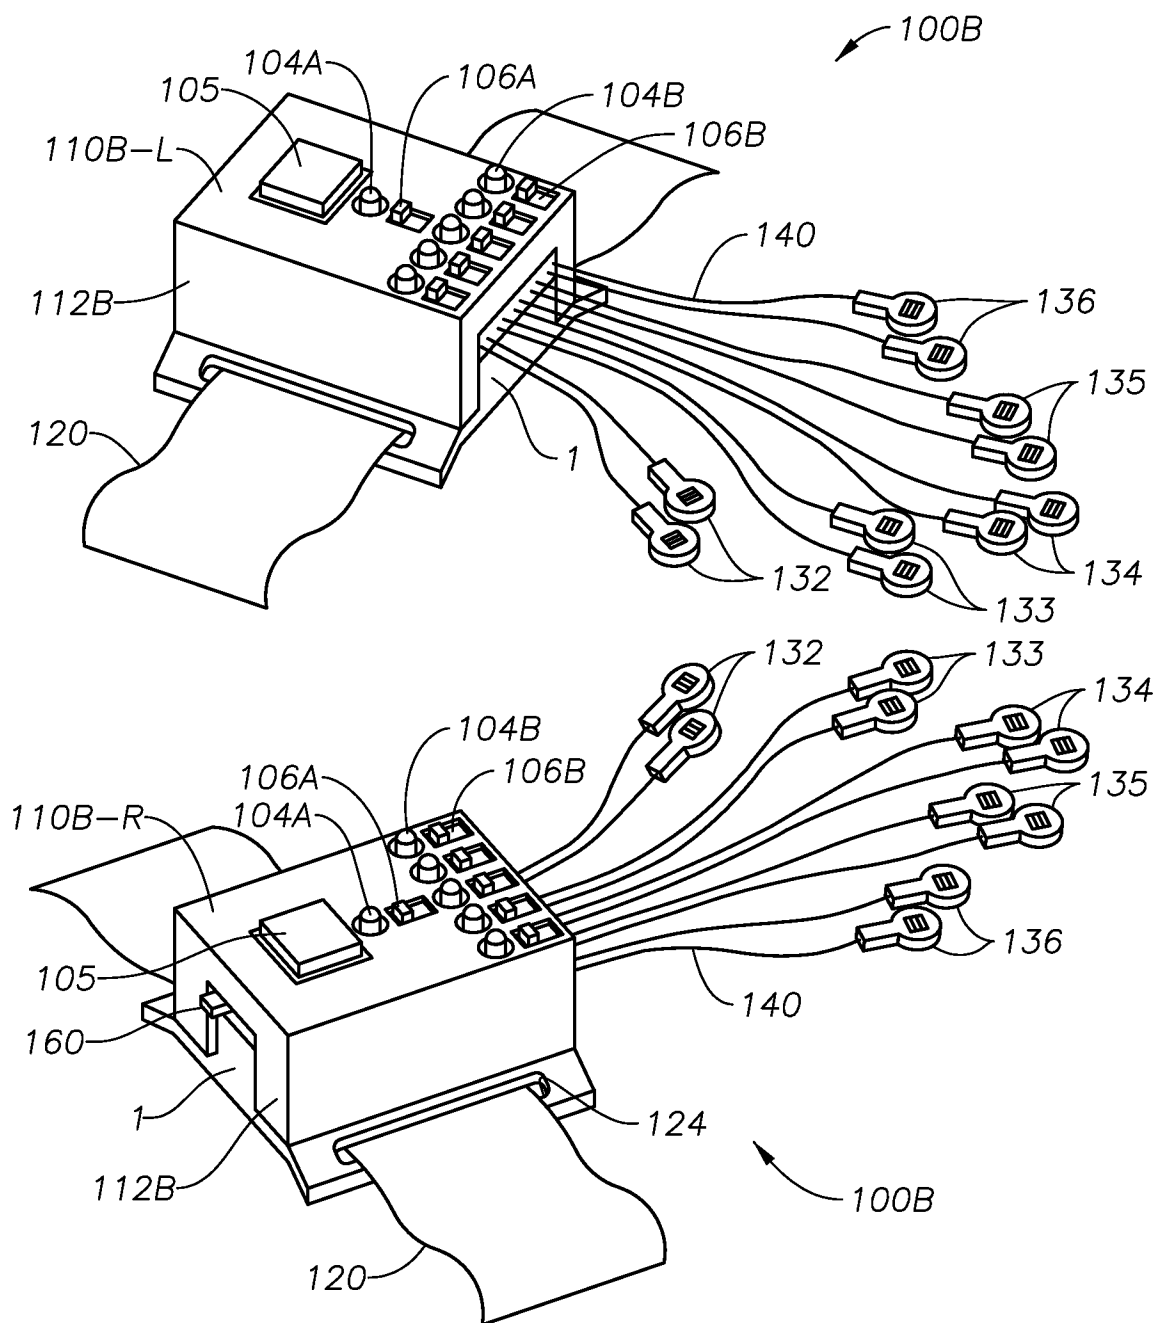


FIG. 2B

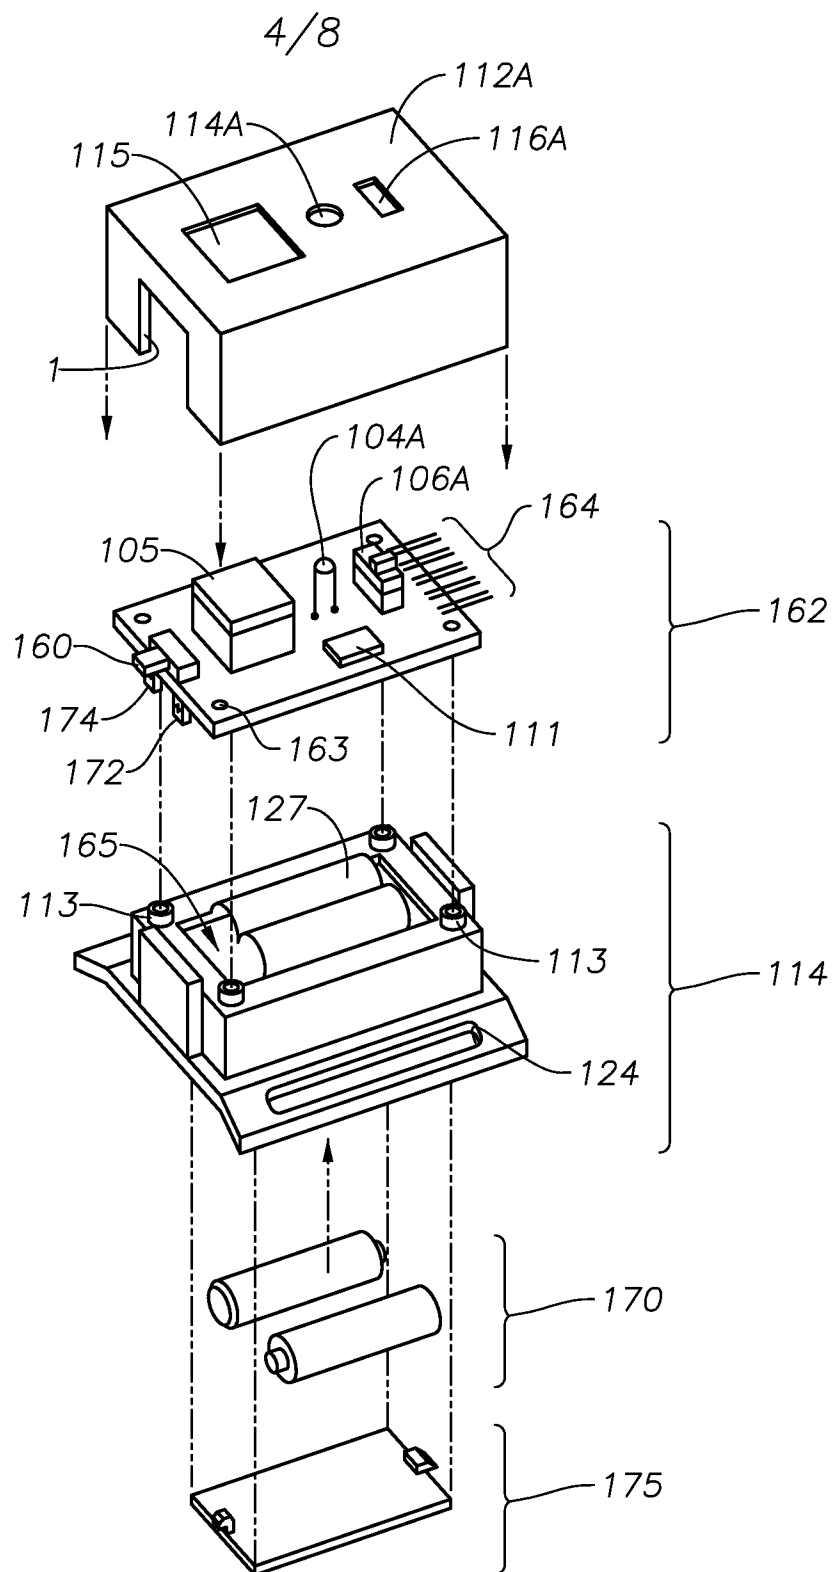


FIG. 3A

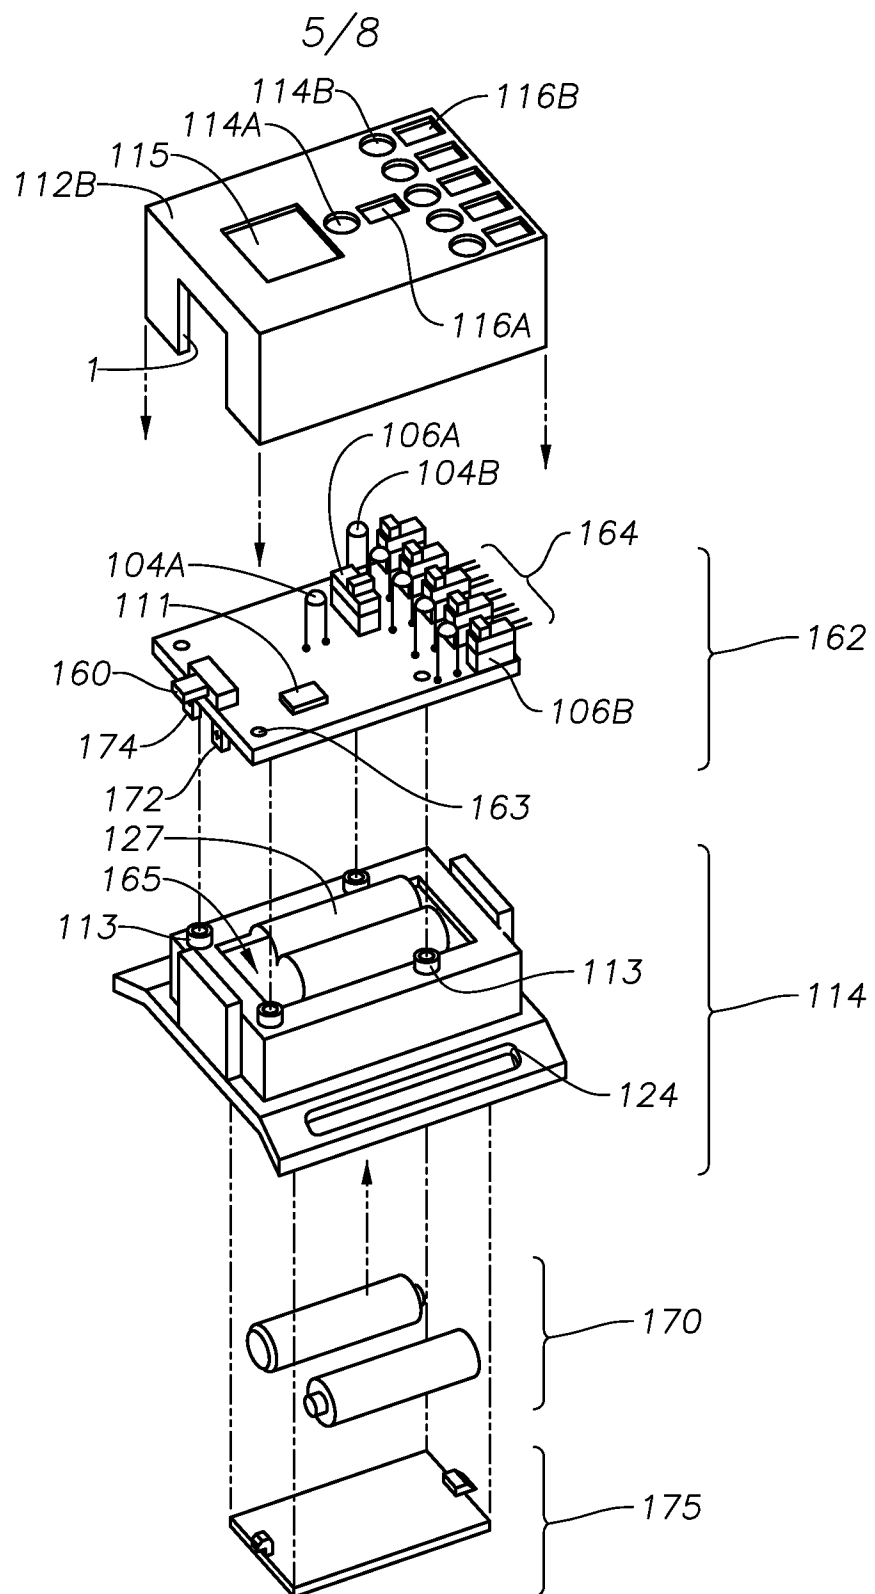


FIG. 3B

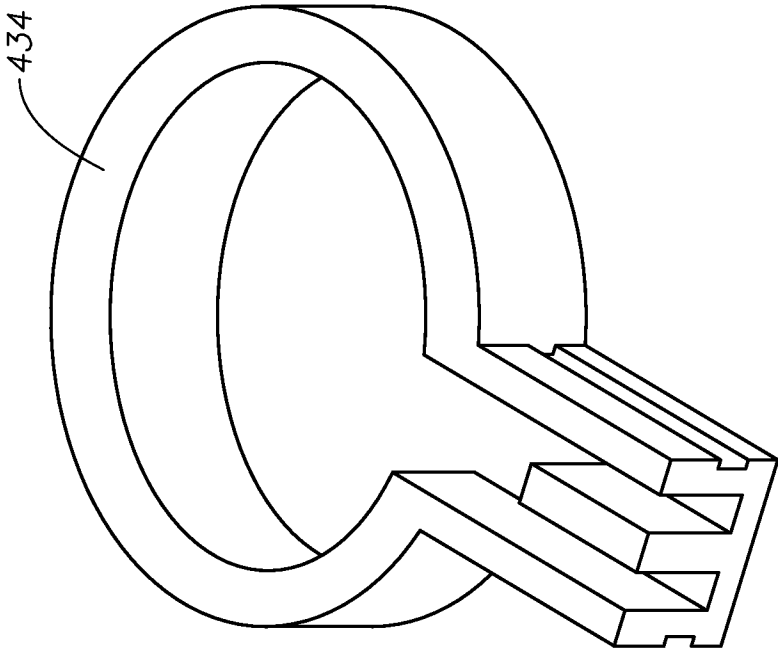


FIG. 4B

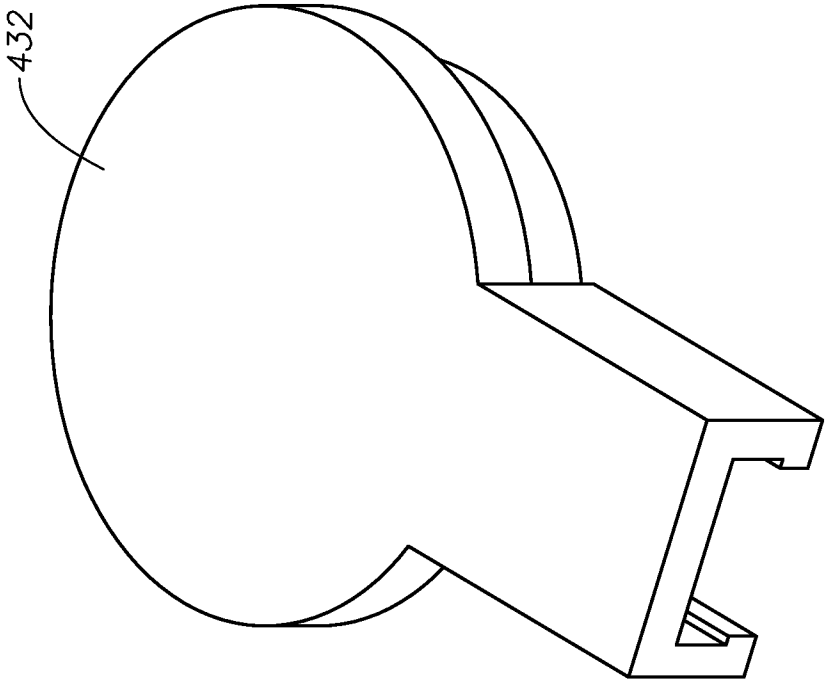


FIG. 4A

7/8

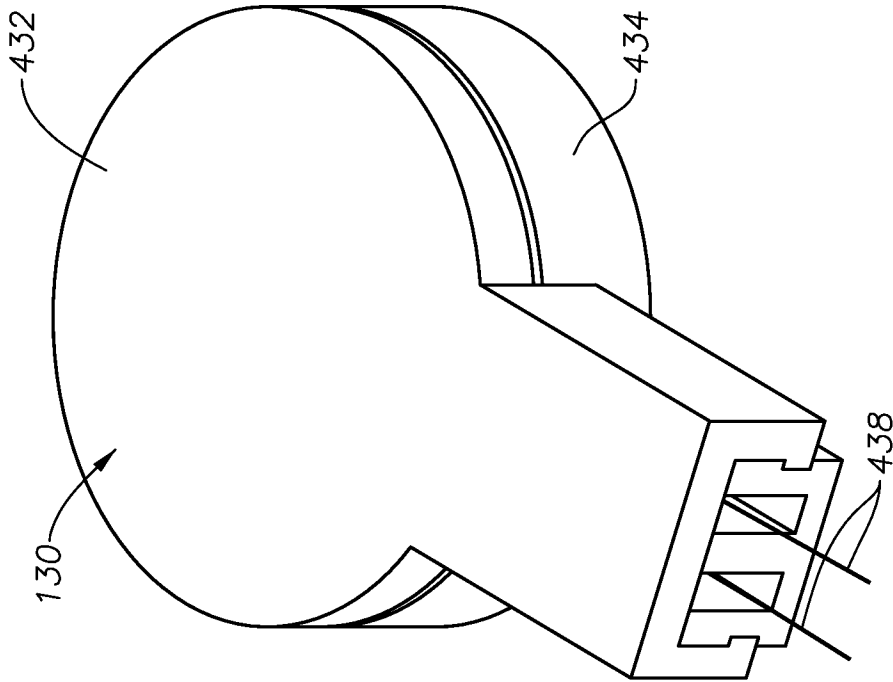


FIG. 4D

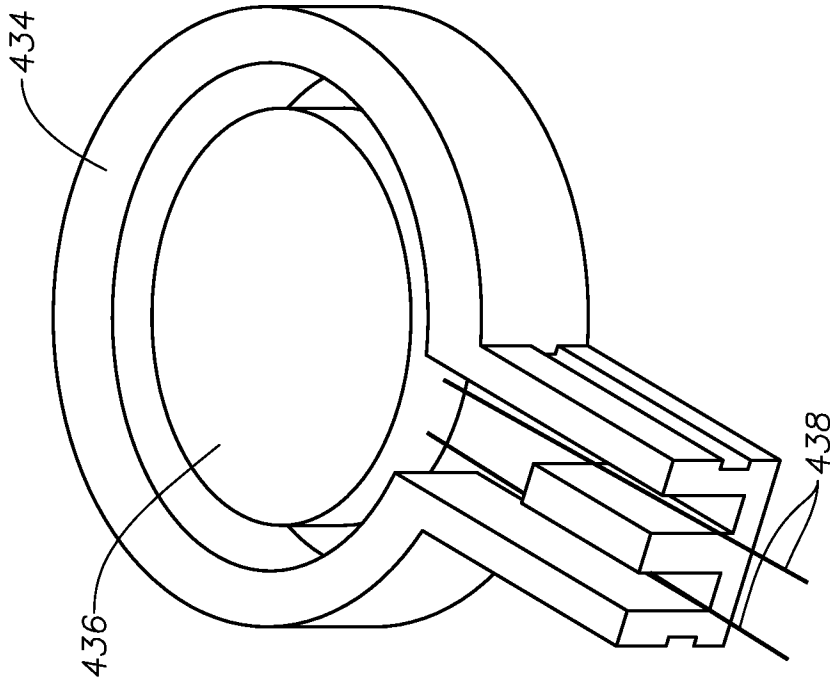


FIG. 4C

8/8

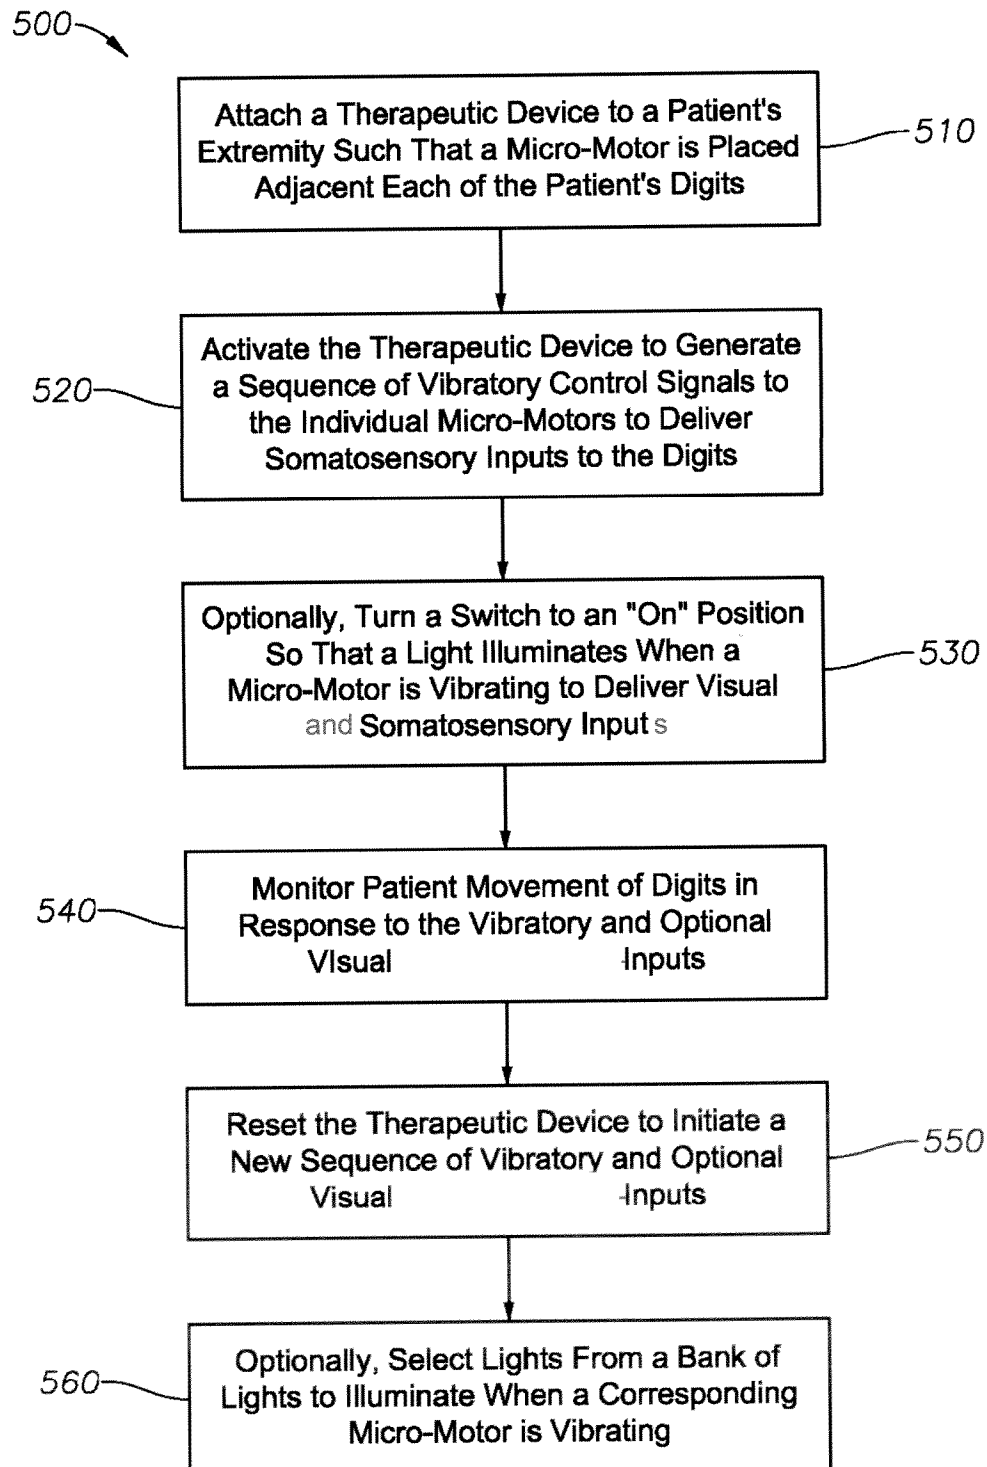


FIG. 5

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2013/040701**A. CLASSIFICATION OF SUBJECT MATTER****A61H 1/00(2006.01)i, A63B 23/16(2006.01)i, B25J 11/00(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61H 1/00; A61H 23/02; A61H 23/06; A61N 1/08; A61H 7/00; A61H 1/02; A61H 11/00; A63B 23/16; B25J 11/00

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: hand, vibration, rehabilitation, extremity, articulate, joint

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 1974710 A1 (TSAI, SHEN-HAI) 1 October 2008 See paragraphs [0018]-[0023]; and figure 1.	1-13,20
A	WO 2010-033055 A1 (HANDMEDIC HB) 25 March 2010 See page 5, line 21 - page 7, line 13; and figure 1.	1-13,20
A	US 4558704 A (PETROFSKY, JERROLD S.) 17 December 1985 See column 4, lines 21-39; column 5, lines 1-57; and figure 2.	1-13,20
A	US 5601529 A (WOLLMAN, MATT J.) 11 February 1997 See column 3, line 13 - column 5, line 61; and figure 1.	1-13,20
A	WO 2011-117901 A1 (IDROGENET S.R.L.) 29 September 2011 See claims 1-11; and figure 1.	1-13,20



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

16 September 2013 (16.09.2013)

Date of mailing of the international search report

16 September 2013 (16.09.2013)

Name and mailing address of the ISA/KR

Korean Intellectual Property Office
189 Cheongsu-ro, Seo-gu, Daejeon Metropolitan City,
302-701, Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

CHANG Bong Ho

Telephone No. +82-42-481-3353



INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2013/040701

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 14-19
because they relate to subject matter not required to be searched by this Authority, namely:
Claims 14 to 19 pertain to a method for treatment of the human body and thus relate to a subject matter which this ISA is not required to search, under Article 17(2)(a)(i) of the PCT and Rule 39.1(iv) of the Regulations under the PCT.
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/040701

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 1974710 A1	01/10/2008	None	
WO 2010-033055 A1	25/03/2010	None	
US 04558704 A	17/12/1985	EP 0145504 A3 JP 60-153856 A	09/09/1987 13/08/1985
US 05601529 A	11/02/1997	WO 96-32915 A1	24/10/1996
WO 2011-117901 A1	29/09/2011	CA 2794193 A1 CN 102811690 A EP 2549971 A1 JP 2013-529937 A US 2013-0072829 A1	29/09/2011 05/12/2012 30/01/2013 25/07/2013 21/03/2013