



- (51) **International Patent Classification:**
A61M 5/315 (2006.01) *A61M 5/24* (2006.01)
- (21) **International Application Number:**
PCT/EP2014/055129
- (22) **International Filing Date:**
14 March 2014 (14.03.2014)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
1304575.2 14 March 2013 (14.03.2013) GB
61/782,225 14 March 2013 (14.03.2013) US
- (71) **Applicant:** **NORTON HEALTHCARE LIMITED**
[GB/GB]; Ridings Point, Whistler Drive, Castleford, York-
shire WF10 5HX (GB).
- (72) **Inventors:** **CAMMISH, Neil**; 14 Blyton Lane, Salford
Greater, Manchester M7 3BR (GB). **HORLOCK, Mark**;
18 Mayfield Close, Timperley, Cheshire WA15 7TE (GB).
- (74) **Agent:** **COTTAM, David William**; Teva UK Limited,
Global Patent Group, Field House, Station Approach, Har-
low Essex CM20 2FB (GB).
- (81) **Designated States** (*unless otherwise indicated, for every
kind of national protection available*): AE, AG, AL, AM,


AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.

- (84) **Designated States** (*unless otherwise indicated, for every
kind of regional protection available*): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments (Rule 48.2(h))

(54) **Title:** DISPENSING MECHANISM FOR A MEDICAL DEVICE

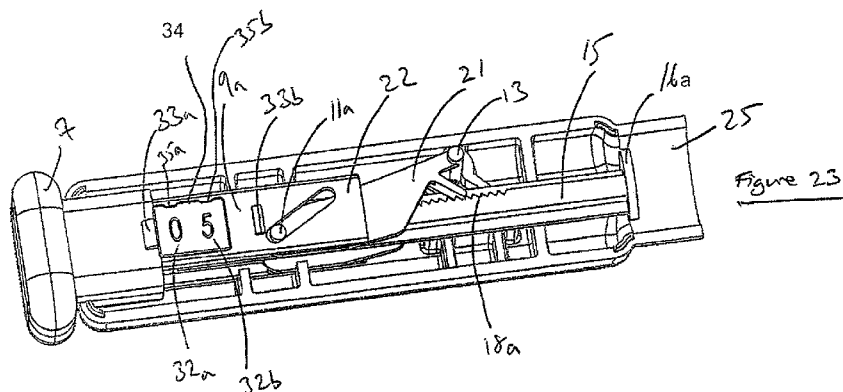

(57) **Abstract:** A dispensing mechanism for administering a dosage of a medicament includes dosage setting means (7) for setting the dosage of a medicament to be administered; expelling means (15) for expelling a medicament from a medicament container; and coupling means (21) operatively coupled with the dosage setting means (7) and the expelling means (15), wherein the coupling means (21) is arranged to convert displacement of the dosage setting means (7) into a displacement of the expelling means (15) in a first direction, wherein the expelling means (15) includes a ratchet means (18a, 18b), and wherein the mechanism includes a first and a second independently moveable resisting pawl (14a, 14b) means facing a common side of the ratchet means (18), the first and the second resisting pawl means (14a, 14b) being configured to engage with the ratchet means (18a, 18b) and resist displacement of the expelling means (15) in a second direction opposite to said first direction.

Dispensing Mechanism for a Medical Device

The present invention relates to a dispensing mechanism for administering a dosage of a medicament. The present invention also relates to a medical device comprising a dispensing mechanism, an injection device comprising a dispensing mechanism and an inhaler comprising a dispensing mechanism.

Medical devices for administering medicament are known, for example liquid solutions or powders can be delivered to a user or patient using injection devices or powder inhalers respectively.

One such medical device for administering a liquid solution is an injection device comprising a dispensing mechanism in which the dosage to be administered may be set by a dosage button moveable by a user or patient. A subsequent further movement of the dosage button, typically in the proximal direction of the device, i.e. in a direction towards an injection site of the device on the patient's skin, serves to inject the medicament using a ram to displace a plunger in a vial or cartridge of liquid medicament. A needle is typically attached to the cartridge in order to allow a subcutaneous delivery of the medicament. The dispensing mechanism ensures that a controlled and accurate dose may be administered.

However, such drive mechanisms often include several interacting component parts and thus packaging the components within a medical device that is optimal in size to carry and simplicity to use can be difficult. In addition, it cannot always be readily determined by a user of the device whether the correct dosage has been fully administered.

The present invention aims to alleviate at least to a certain extent at least one of the problems of the prior art.

According to a first aspect of the invention, there is provided a dispensing mechanism for administering a dosage of a medicament, the mechanism comprising: a dosage setting means, element, part or parts for setting a dose of medicament to be administered; expelling means, element part of parts for expelling a medicament from a medicament container; a coupling means, element, part of parts operatively coupled with the dosage setting means and the expelling means, wherein the coupling means is arranged to convert displacement of the dosage setting means into a displacement of the expelling means in a first direction, wherein the expelling means or coupling means includes a ratchet means, element, part or

parts, and wherein the mechanism includes a first and a second independently moveable resisting pawl means or pawls facing a common side of the ratchet means, the first and the second resisting pawl means being configured to engage with the ratchet means and resist displacement of the expelling means in a second direction opposite to said first direction.

- 5 Advantageously, such a mechanism provides a compact arrangement and control of the expelling means. The resisting pawl means advantageously prevents movement of the expelling means during dose setting.

The dosage setting means may comprise a push button or other component which can be manually manipulated by a user.

- 10 Optionally, the ratchet means comprises a first and a second set of teeth, the first set of teeth being arranged to engage with the first resisting pawl means and the second set of teeth being arranged to engage with the second resisting pawl means.

- The first and second sets of teeth are optionally each arranged in rows. The rows are optionally parallel and may be spaced from one another. The teeth preferably comprise
15 peaks and valleys. The ridges of the peaks of each set of teeth are aligned transverse to the longitudinal axis of the expelling means. The teeth are preferably equally spaced in each row of teeth. The heights of the teeth are preferably equal.

- Each tooth preferably comprises a front planar face and a rear planar face. The front planar face is preferably arranged proximally, i.e. nearer the point of contact with a patient's skin, in
20 use, in the mechanism. The front face is preferably inclined at a smaller angle to a plane extending parallel to a side of the body of the mechanism or device and the rear face of each tooth being inclined at a relatively larger angle to said plane.

- The engaging faces are preferably the faces of the teeth against which the pawls may act to resist movement. The engaging faces are preferably the rear faces of the teeth in each row
25 of teeth.

The pawls may be orientated with their free, ratchet-engaging ends angled towards a first, proximal end of the mechanism.

Optionally, the dosage setting means is linearly displaceable in a direction substantially parallel to the longitudinal axis of the expelling means.

- 30 Optionally, the dosage setting means is rotationally displaceable about an axis substantially parallel to the longitudinal axis of the expelling means.

Optionally, the dosage setting means is displaceable both axially and rotationally about an axis parallel to the longitudinal axis of the expelling means, for example where a screw thread arrangement is provided.

5 Optionally, the first and/or second resisting pawl means comprise(s) or are formed with a part of a body of the mechanism.

Optionally, the mechanism may be formed of a plastics material, a metallic material or a combination of both.

Optionally, the teeth pitch in each of the first set of teeth and the second set of teeth is substantially equal.

10 Optionally, engaging faces of the second set of teeth are arranged offset from engaging faces of the first set of teeth on the ratchet means. Preferably, the offset is in the longitudinal direction of the expelling means.

15 Optionally, the engaging faces of the teeth in the first set of teeth are offset a distance of half the tooth pitch, i.e. half the distance between adjacent engaging faces from the teeth of the second set of teeth. Preferably, the offset is in the longitudinal direction of the expelling means.

20 Optionally, the resisting pawls are offset in the longitudinal direction of the expelling means. Optionally, the ratchet comprises a single set of teeth engageable with the resisting pawls. This allows for an alternative arrangement in order to achieve fine dosages. Optionally, the offset of the resisting pawls may be, for example, 0.5 or 1.5 times the pitch or distance between adjacent teeth in the ratchet.

Advantageously, by arranging the teeth or pawls so that only one pawl engages with an engaging face of one of the two sets of teeth at any one time, finer doses can be dispensed whilst the component features remain the same size.

25 Optionally, the expelling means comprises a longitudinal member.

Optionally, the expelling means is formed with ribs, or protrusions to be received in or be guided in corresponding recesses or channels. This ensures smooth motion of the expelling means.

30 Optionally, the first and second resisting pawl means are formed on opposing parts of a body of the mechanism. This reduces the number of components and can provide strength to the resisting pawls.

Optionally, the body may be formed of two half-shells.

A dispensing mechanism is also provided, wherein the first and the second resisting pawl means are aligned in a substantially common plane. Alternatively, the first and the second
5 resisting pawls means could be aligned offset with the teeth in the ratchet being in alignment.

Optionally, the first resisting pawl means is aligned adjacent the second resisting pawl means.

Optionally, the coupling means comprises a drive means or driver comprising a pair of drive
10 pawls engageable in said ratchet means for displacing said expelling means.

Optionally, the drive pawls are arranged in adjacent alignment or may be offset corresponding to the offset of the resisting pawls.

Optionally, the coupling includes a guide slot in which a follower on the drive means is received and configured such that the drive means is moved as a result of movement of the
15 dosage setting means. Optionally, the driver is caused to rotate about a pivot in order to engage the drive pawls with the teeth in the ratchet and produce motion of the expelling means.

Alternative coupling means may include gears or thread arrangements in order to produce a displacement of the expelling means upon movement of the dosage means.

20 Optionally, the expelling means comprises a ram means.

According to a second aspect of the invention, there is provided a dispensing mechanism for administering a dosage of a medicament, the mechanism comprising: a body; and dosage setting means, element, part of parts for setting the dosage of a medicament to be
25 administered, the dosage setting means being moveable in a first direction for setting the dose and in a second direction for administering the dose, wherein the mechanism further comprises an indication element, the indication element being arranged to be displaced by a predetermined movement of the dosage setting means; and wherein the indication element is arranged such that the indication element remains unmoved relative to said body of the
30 mechanism during at least part of said movement of the dosage setting means.

In this way, the indication element can provide a static indication to a user for at least part of the motion of the dosage setting means. This can serve to facilitate operation of the mechanism or device by a user.

Optionally, the indication element is movable within a guide channel. Advantageously, this
5 maintains the orientation of the indication element.

Optionally, the indication element is slidingly supported in or on the body.

Optionally, the dosage setting means is movable in an axial direction substantially parallel to the longitudinal axis of the body.

Optionally, the indication element is formed as a planar element, preferably as a generally
10 rectangular plate or element.

Optionally, the dosage setting means is rotatable about the longitudinal axis of the body.

Optionally, the dosage setting means is operative coupled to a first and a second engagement means, elements or parts, the first engagement means and the second engagement means being engageable with the indication element such that upon
15 engagement, movement of the dosage setting means causes displacement of the indication element.

The engagement means are preferably formed to engage with the indication element in order to move it with corresponding movement of the dosage setting means.

Optionally, the engagement elements are arranged spaced from one another at a distance
20 greater than a length of the indication element. This then provides a degree of lost motion of the indication element relative to the dosage setting element.

Optionally, resisting means, elements or parts are provided, the resisting means being arranged to resist movement of the indication element relative to movement of the dosage setting means. This prevents movement of the indication element until a predetermined
25 movement of the dosage setting means has been made.

Optionally, the resisting means comprises a protrusion receivable in a corresponding recess. The protrusion may be provided on the body or dosage setting element or on the indication element or vice versa, for example. This provides a degree of mechanical resistance without additional parts.

30 Optionally, the resisting means comprises a protrusion receivable in a corresponding recess.

Optionally, the mechanism includes an aperture through which at least a portion of the indication element is exposed, in use, to a user.

Optionally, the indication element comprises tactile and/or visual indications. This may include Braille or other types of tactile indications and/or visual indications such as lights or printed numbers. The indications may indicate the state of the mechanism or device, e.g. whether a dose is ready to be administered or if a dose needs to be set.

Optionally, the indication element is moved directly by the dosage setting means. The indication element may be in direct contact with the dosage setting means.

Optionally, the indication element is moved indirectly by the dosage setting means.

10

According to a third aspect of the invention, there is provided a dispensing mechanism for administering a dosage of a medicament, the mechanism comprising: a body; dosage setting means, element, part or parts for setting the dosage of a medicament to be administered, the dosage setting means being moveable in a first direction for setting the dose and in a second direction for administering the dose; and an indication element, the indication element being arranged to be displaced by a predetermined movement of the dosage setting means; and wherein the mechanism further includes conversion means, element, part of parts configured, during displacement of the indication element, to convert a movement of the dosage setting means of a first magnitude into a movement of the indication element of a second magnitude, and wherein said first magnitude of movement is different to said second magnitude of movement.

20

In this way, the degree of movement of the indication element can be configured to be different in magnitude to that of the dosage setting means.

Optionally, the first magnitude of movement is greater than the second magnitude of movement. In this way, a small movement of the dosage setting means can cause a larger movement of the indication element.

25

Optionally, the first magnitude of movement is smaller than the second magnitude of movement. As such, the indication element can be arranged to move a shorter distance than the movement of the dosage setting means.

Optionally, the conversion means is configured to move the indication element during all movement of the dosage setting means. The conversion means may be in constant contact

30

with the dosage setting means or in constantly coupled thereto, for example through an intermediate component.

Optionally, the indication element remains unmoved relative to the body of the mechanism during at least part of said movement of the dosage setting means.

- 5 Optionally, the indication element is movable within a guide channel.

Optionally, the indication element is slidingly supported in or on the body.

Optionally, the dosage setting means is movable in an axial direction substantially parallel to the longitudinal axis of the body.

Optionally, the dosage setting means is rotatable about the longitudinal axis of the body.

- 10 Optionally, the conversion means comprises a first and a second engagement means operatively coupled to the dosage setting means, the first engagement means and the second engagement means being engageable with the indication element such that upon engagement, movement of the dosage setting means causes displacement of the indication element.

- 15 Optionally, the engagement elements are arranged spaced from one another at a distance greater than a length of the indication element.

Optionally, the conversion means comprises a lever.

Optionally, the lever acts about a fulcrum operatively coupled to the dosage setting means. The relative magnitudes of movement of the dosage setting means and indication element
20 may be configured by the relative lengths of the lever either side of the fulcrum.

Optionally, the lever is resiliently flexible. In this way dimensional tolerances may be accounted for as the lever may flex if movement of the dosage setting means is greater than the space in which the lever is located.

Optionally, the lever is pivotally attached to said body.

- 25 Optionally, the lever is formed integrally with said body. This can serve to reduce manufacturing costs and reduce the number of parts in the mechanism. The lever could alternatively be any part of the body, indicator or dose setting means, for example.

Optionally, resisting means are provided, the resisting means being arranged to resist movement of the indication element relative to movement of the dosage setting means.

Optionally, the resisting means comprises a protrusion receivable in a corresponding recess.

Optionally, the mechanism includes an aperture through which at least a portion of the indication element is exposed, in use, to a user.

Optionally, the indication element comprises tactile and/or visual indications.

- 5 Optionally, the indication element is moved directly by the dosage setting means.

Optionally, the indication element is moved indirectly by the dosage setting means.

According to a fourth aspect of the invention, there is provided a dispensing mechanism for administering a dosage of a medicament, the mechanism comprising: a dosage setting
10 means, element, part or parts for setting a dose of medicament to be administered; expelling means, element, part of parts for expelling a medicament from a medicament container; a coupling means, element, part or parts operatively coupled with the dosage setting means and the expelling means, wherein the coupling means is arranged to convert displacement of the dosage setting means into a displacement of the expelling means in a first direction,
15 wherein the coupling means includes a ratchet means, element or part or parts comprises a first and a second ratchet wheels, and wherein the mechanism includes a first and a second independently moveable resisting pawl means facing the ratchet means, the first and the second resisting pawl means being configured to engage with the first and second ratchet wheels respectively and resist displacement of the expelling means in a second direction
20 opposite to said first direction.

Advantageously, such a mechanism provides a compact arrangement and control of the expelling means. The resisting pawl means advantageously prevents movement of the expelling means during dose setting.

Optionally, the first ratchet wheel comprises a first set of teeth and the second ratchet wheel
25 comprises a second set of teeth, the first set of teeth being arranged to engage with the first resisting pawl means and the second set of teeth being arranged to engage with the second resisting pawl means.

Optionally, engaging faces of the second set of teeth are arranged rotationally offset from engaging faces of the first set of teeth on the ratchet means. Each of the first and second
30 ratchet wheels may have teeth provided around their entire circumference. The first and second ratchet wheels preferably share a common rotational axis.

Optionally, the dosage setting means is linearly displaceable in a direction substantially parallel to the longitudinal axis of the expelling means.

Optionally, the dosage setting means is rotationally displaceable about an axis substantially parallel to the longitudinal axis of the expelling means.

- 5 Optionally, the first and/or second resisting pawl means comprise(s) a part of a body of the mechanism.

Optionally, the angular teeth pitch in each of the first set of teeth and the second set of teeth is substantially equal.

- 10 Optionally, the engaging faces of the teeth in the first set of teeth are offset by an angle of rotation of half the angle of rotation between adjacent engaging faces from the teeth of the second set of teeth.

Optionally, the expelling means comprises a longitudinal member.

Optionally, the first and second resisting pawl means are formed on opposing parts of a body of the mechanism.

- 15 Optionally, the first and the second resisting pawl means are aligned in a substantially common plane.

Optionally, the first resisting pawl means is aligned adjacent the second resisting pawl means.

- 20 Optionally, the coupling means comprises a drive means comprising a pair of drive pawls engageable in said ratchet means for rotation of said ratchet wheel. The drive pawls may be spaced from one another to align either side of the expelling means.

Optionally, the drive pawls are arranged in adjacent alignment.

- 25 Optionally, the coupling includes a guide slot in which a follower on the drive means is received and configured such that the drive means is moved as a result of movement of the dosage setting means.

- 30 Optionally, the ratchet means comprises a gear wheel engageable with a corresponding set of teeth on the expelling means. The gear wheel preferably shares a common axis of rotation with the ratchet wheels. The teeth on the expelling means are preferably formed as a rack of teeth. The rotation of the gear wheel preferably results in axial movement of the expelling means.

Optionally, the first and second ratchet wheels are arranged either side of said gear wheel.

Optionally, the diameter of the gear wheel is smaller than the diameter of each of the ratchet wheels. The ratchet wheels may be aligned either side of the expelling means. The gear wheel and ratchet wheel may be formed integrally as a single piece.

5 Optionally, the expelling means comprises a ram means.

Any one or more of the first to fourth aspects of the invention or any optional feature thereof may be combined. Advantages of the features are applicable to different aspects and embodiments of the invention.

10 According to a fifth aspect of the invention, there is provided a medical device comprising a dispensing mechanism according to any of the first to fourth aspects of the invention and any optional feature thereof.

Optionally, the medical device may comprise a medicament container such glass vial, cartridge or foil pack and/or a receiving part for such a medicament container.

15 According to a sixth aspect of the invention, there is provided an injection device comprising a dispensing mechanism according to any of the first to fourth aspects of the invention and any optional feature thereof.

According to a seventh aspect of the invention, there is provided an inhaler comprising a dispensing mechanism according to any of the first to fourth aspects of the invention and any optional feature thereof.

20

The present invention will now be described by way of an exemplary embodiment, with reference to the accompanying drawings, in which:

Figure 1 shows a perspective view of a medical device with a dispensing mechanism comprising a dosage button in a depressed state;

25 Figure 2 shows a perspective view of the medical device of Figure 1 with a dosage button in a withdrawn state;

Figure 3 shows a first side perspective view of the medical device of Figure 1 with part of the outer body removed with the dosage button in a depressed state;

30 Figure 4 shows a first side perspective view of the medical device of Figure 1 with part of the outer body removed with the dosage button in a withdrawn state;

Figure 5 shows a first side perspective view of a drive pawl of the medical device of Figure 1;

Figure 6 shows a second side perspective view of the medical device of Figure 1 with part of the outer body removed with the dosage button in a depressed state;

5 Figure 7 shows a second side perspective view of the medical device of Figure 1 with part of the outer body removed with the dosage button in a withdrawn state;

Figure 8 shows a second side perspective view of a drive pawl of the medical device of Figure 1;

Figure 9 shows a perspective side view of the medical device of Figure 1 without a cartridge holder;

10 Figure 10 shows a cutaway view through the body of the medical device as shown in Figure 9 showing a rear view of a ratchet arrangement;

Figure 11 shows a cutaway view through the body of the medical device as shown in Figure 9, with the ratchet removed and showing the underside of the drive pawl;

15 Figures 12 and 14 show cross-sections A-A and B-B respectively of the medical device as marked in Figure 13 with the dosage button in a depressed state;

Figures 15 and 17 show cross-sections C-C and D-D respectively of the medical device as marked in Figure 16 with the dosage button in a withdrawn state;

Figure 18a shows a side view of the ratchet of the medical device as shown in Figure 1;

Figure 18b shows a detail view A as circled in the ratchet view shown in Figure 18a;

20 Figure 19a shows a plan view along the length of the ratchet as shown in Figure 18a;

Figure 19b shows a detail view B as circled in the ratchet view as shown in Figure 19a;

Figure 20 shows a perspective view of the ratchet as shown in Figure 18a;

Figure 21 shows a perspective side view of a medical device with an indicator window with a dosage button in a depressed state;

25 Figure 22 shows a perspective side view of the medical device with an indicator window with the dosage button in a withdrawn state;

Figure 23 shows a perspective view of the medical device shown in Figure 21 with part of the outer body removed;

Figure 24 shows a side view of the medical device as shown in Figure 21 marking cross-section E-E;

Figure 25 shows a cross-sectional view E-E of Figure 21 showing the dosage button in an initial depressed state;

- 5 Figure 26 shows a cross-section view E-E of Figure 21 showing the dosage button in an initial retracted state;

Figure 27 shows a cross-section view E-E of Figure 21 showing the dosage button in an intermediate retracted state;

- 10 Figure 28 shows a cross-section view E-E of Figure 21 showing the dosage button in an fully retracted state;

Figure 29 shows a medical device with an alternative dosage button in a depressed state;

Figure 30 shows the medical device of Figure 29 with the dosage button in a rotated and retracted state;

- 15 Figure 31 shows the medical device of Figure 29 with the dosage button in a rotated and depressed state;

Figure 32 shows an external perspective view of a further medical device with the dosage button in a withdrawn state;

Figure 33 shows a partial cross-section through the device as shown in Figure 32;

- 20 Figure 34 shows an external perspective view of the device of Figure 32 with the dosage button on a depressed state;

Figure 35 shows a partial cross-section through the device as shown in Figure 33;

Figures 36 to 39 show the medical device of Figures 32 and 33 in partial stages of assembly;

Figure 40 shows a view of a further medical device comprising an alternative dispensing mechanism with part of the body removed with a push button in a depressed state;

- 25 Figure 41 shows a further view the medical device of Figure 40 with the push button in a retracted state;

Figure 42 shows a view of the coupling means and expelling means of the dispensing mechanism shown in Figures and 41; and

Figure 43 shows a view of a rotary ratchet of the expelling means of the dispensing mechanism of Figure 42.

Figure 1 shows a perspective view of a medical device including a dispensing mechanism generally indicated 1. The medical device 1 comprises an elongate body 2 with a substantially square cross-section with rounded edges between adjacent sides. However, it is envisaged that the body 2 may be formed in any suitable shape, for example with a circular cross-section or with varying cross section along the length of the device 1.

The size and the form of the body 2 may be designed to facilitate being held in a user or patient's hand. The surface may be provided with surface protrusions or knurling or any other such surface texture to facilitate gripping of the device 1.

At a first, proximal end 3a of the body 2, i.e. the end nearest an injection site of a user in use, a cartridge receptacle 4 is attached, for example by a bonded or clipped engagement, to the body 2, for holding a medicament cartridge or carpule. The cartridge receptacle 4 is formed generally as a truncated cone and may be made transparent in order that a user may inspect the contents of the medicament cartridge to obtain a visual indication of the quantity of medicament remaining. The medicament cartridge may be filled with a liquid medicament, for example insulin.

A removable and disposable needle (not shown) may be attached to the cartridge receptacle 4 or to a threaded engagement 5 provided on the outer surface of a cylindrical part at the proximal end of the cartridge which, as shown in Figure 1, extends through the end of the cartridge receptacle 4. A typical needle comprises a rear needle part for puncturing a plastic stopper 6 provided at the proximal end of the medicament cartridge. The needle also comprises a forward needle part. In use, the forward needle part may be inserted subcutaneously into a patient so that medicament may be injected from the medicament cartridge into a patient.

At a second, distal end 3b of the body 2 of device 1, i.e. the end, in use, furthest from an injection site of a user, a dosage setting means or element is provided in the form of a push button 7. In the embodiment, the push button has a similar, generally square, cross-sectional shape to that of the body 2 of the device 1. However, different shapes and arrangements of the dosage means are envisaged. The dosage means 7 is typically sized to be gripped between a finger and thumb of a user. Figure 1 shows the push button 7 in a depressed, i.e. pushed-in state relative to the body 2 of the device 1.

The push button 7 may be pulled out away from the body 2 in a first distal direction in order to set a dose and pushed in towards the body 2 in a second proximal direction in order to administer a dose of medicament.

5 In Figure 2, the push button is shown in a first, pulled-out state, with the device ready to deliver a dose. The push button 7 comprises a drive shaft 8 connecting the push button to a drive mechanism within the body of the device.

The body 2, in the embodiment, is formed of two half-shells 2a, 2b. The body 2 is generally formed of a plastics material, which may be injection moulded or produced by any other suitable manufacturing technique.

10 Figure 3 shows the device 1 with one of the half-shells 2b removed to expose the internal drive mechanism of the device 1.

Within the body 2 of the device 1, an expelling means, element or part is provided in the form of a longitudinal drive rod 15. The rod 15 is linear in form and serves as a ratchet or ratchet means, with an upper surface comprising two sets of ratchet teeth 18a, 18b
15 extending along at least part of the length of the rod 15. The teeth are orientated such that their lands, valleys or ridges of the peaks run transverse to the longitudinal direction of the device.

In the exemplary embodiment described herein, the teeth of one of the sets of ratchet teeth are offset from the teeth of the other set of ratchet teeth. However, it should be noted that
20 such an 'offset' arrangement is only a preferred embodiment of the present invention.

The sets of ratchet teeth in this example are separated by a longitudinal planar divider 24. The longitudinal rear side of the rod 15 is planar with a central protruding guide rib 20. Corresponding channels and support rails 23a, 23b are formed within the body 2 to receive the rod 15 and the guide rib 20 and allow linear movement thereof along the longitudinal axis
25 of the device 1.

At the proximal end of the rod 15, the rod comprises an engagement ram 16a in the form of a circular disc. The ram 16a is formed and sized such that, in use, the ram 16a can engage with and displace a plunger 17 in a medicament cartridge received in the cartridge receptacle 4.

30 A coupling means, element, part or mechanism is provided to couple the dosage setting element with the expelling element. In the embodiment, the coupling means includes a first coupling element 22 connected to the push button 5 via a shaft 8. In the embodiment, the

first coupling element 22 is formed integrally with the shaft 8. However, it is envisaged that the coupling element 22 could be operatively coupled to the push button 7 and/or shaft via a sprung or biased coupling so as to be moveable relative thereto.

The coupling element 22 comprises a pair of spaced planar sections of which only the upper planar section 9a is visible in Figure 3. However, a corresponding lower planar section is formed with the lower side of the shaft of the push button 7. The spaced planar sections 9a are perpendicular to the plane of the surface on which the ratchet teeth are provided. In the upper planar section 9a of the coupling element 22, a diagonal slot 10a is provided. The diagonal slot 10a extends diagonally in a direction across the body of the device.

10 The coupling further comprises a drive means or driver 21 which, as shown more clearly in Figure 5, comprises a pair of parallel and spaced planar arms 12a, 12b connected via a transverse web 16b towards a proximal end thereof. Each of the planar arms 12a, 12b comprises a circular protrusion or follower of which only the upper protrusion 11a is visible in Figures 3 to 4.

15 The circular protrusion 11a of the upper planar arm 12a is received in the diagonal guide slot 10a of the upper planar section 9a of the coupling element. Although not shown, a corresponding circular protrusion is formed on the lower planar arm 12b and is received in a corresponding diagonal guide slot 10a in the lower planar section of the coupling element 22.

20 The underside of the upper planar section 9a of the coupling element 22 is supported on and slides atop of the upper planar arm 12a of the driver 21.

The driver 21 comprises a pair of drive pawls 14a, 14b extending from the web 16b. A gap is provided between the drive pawls 14a, 14b which fits around the divider 24 between the two sets of ratchet teeth 18a, 18b. The drive pawls are independently flexible about their connection with the driver 21.

The driver 21 comprises a cylindrical portion 13a which is pivotally located in a corresponding hole in the body 2 of the device 1. The cylindrical portion is rotatably engaged with the hole in the body 2 such that the driver 21 may rotate about the axis of the cylindrical portion, which acts therefore as a pivot axis.

30 The drive pawls 14a, 14b are arranged such that they can engage with a tooth respectively of each of the sets of ratchet teeth 18, although due to the offset in the sets of teeth, the drive pawls 14a, 14b do not necessarily contact the same part of a tooth in a respective set of teeth. For example, with an offset arrangement of the two sets of teeth in the drive rod,

one drive pawl may be in engagement with a rear face of a tooth and the other drive pawl may be atop a ridge or peak of a tooth in the adjacent set of teeth. The drive pawls 14a, 14b of the driver 21 are angled towards the proximal end 3a of the body 2 of device 1. However, embodiments are envisaged where the teeth in each set of teeth are in adjacent alignment.

- 5 Figure 4 shows a further view of the device 1 as shown in Figure 3 with the push button 7 in a retracted or withdrawn position.

As can be seen in Figure 3 and 4, in the depressed state of the push button 7, the engagement protrusion 11a of the driver 22 is located at one end, the distal end, of the diagonal slot 10a of the coupling element 22. In the withdrawn position of the push button 7, the engagement
10 protrusion 11a of the driver 22 is located at the other end, the proximal end, of the diagonal slot 10a of the coupling element 22. This change of position is achieved by the engagement protrusion 11a sliding in the diagonal slot 11a as the push button 7 is moved in a direction along the longitudinal axis of the device.

Because of the diagonal orientation of the slot 11a in the coupling element, the movement of
15 the engagement protrusion 11a, which is formed with the driver 21, causes the driver 21 to rotate about the pivot point formed by the engagement of the cylindrical protrusion 13 of the driver 21 engaged in the body 2 of the device 1.

As the driver 21 is rotated clockwise about the pivot axis 13 by the push button 7 being depressed, one of the pawls 14a, 14b engages with at least one rear face of a tooth on one
20 of the sets of ratchet teeth 18a such that the longitudinal rod 15 is displaced in a direction towards the distal end of the device.

Figures 6, 7 and 8 show reverse side perspective views respectively of the views shown in Figures 3, 4 and 5.

In Figure 6, the device 1 is shown with the push button 7 in a depressed state. The
25 longitudinal drive rod 15 can be seen showing the upper side thereof in which the two sets of ratchet teeth 18a, 18b are provided separated by divider 24. The upper and lower drive pawls 14a, 14b can be engaged with teeth respectively in the first and second sets of ratchet teeth 18a, 18b, although as described above, due to the offset of the teeth in the two sets of teeth 18a, 18b, the drive pawls 14a, 14b do not necessarily contact the same portion of a
30 tooth in a respective set of teeth.

Figure 7 shows the device 1 with the push button 7 in a withdrawn state. As can be seen from Figure 6, with the push button 7 in a depressed state or position, the driver 21 has been rotated about the pivot axis 13 thus engaging at least one of the drive pawls 14a, 14b with at

least one rear face of a tooth of a set of ratchet teeth 18a, 18b and causing the drive rod 15 to be displaced in a proximal direction.

The drive pawls 14a, 14b are formed to allow a degree of flexing relate to the web 16b.

Figure 9 shows a view of the device 1 with the push button 7 in a depressed state. The device 1 is shown with the cartridge receptacle 4 removed. An aperture 25 can be seen in the proximal end 3a of the body 2 in which the drive rod 15 may extend in use to engage with the stopper of a medicament cartridge (not shown).

Figure 10 shows a view of the device 1 with a cut-out in the body 2. Through the cut-out, the drive rod 15 may be seen. Either side of the drive rod 15, the upper and lower arms 12a, 12b of the driver are located. The upper and lower drive pawls 14a, 14b can also be seen.

Spaced from the upper and lower drive pawls 14a, 14b, in the proximal direction of the body 2 of the device 1, a pair of resistance or resisting pawls 26a, 26b is provided. The resistance pawls 26a, 26b are formed with or attached to the body 2 of the device 1.

Figure 11 shows a further cut-away view of the body 2 of the device 1, but with the drive rod 15 removed. Here, the arrangement of the resistance pawls 26a, 26b and drive pawls 14a, 14b can be seen.

The resistance pawls 26a, 26b are angled in a direction towards the proximal end 3a of the body 2 of device 1. The resistance pawls are flexible to a certain degree with respect to the body 2 of the device 1.

The upper resistance pawl 26a can engage with the upper set of teeth 18a on the longitudinal rod 15, with the lower resistance pawl 26b engageable with the lower set of teeth 18b on the longitudinal rod 15. Due to the offset of the teeth between the teeth in one set of ratchet teeth to the teeth in the other set of ratchet teeth in this embodiment, the resistance pawls 26a, 26b may not contact the same part of a tooth in each of the first and second sets of ratchet teeth 18a, 18b.

The resistance pawls 26a, 26b serve to resist or prevent movement of the longitudinal rod 15 in a direction away from the proximal end 3a of the body 2 of device 1, by engaging the rear faces of the ratchet teeth 18a, 18b.

The operation of the device 1 will now be described with reference to Figures 12 and 14, which show cross sections A-A and B-B along the parallel longitudinal planes shown in Figure 13.

Figures 12 and 14 show the device 1 with the push button 7 in a depressed state. A medicament cartridge 27 is shown within the cartridge receptacle 4. A plunger 17 is provided within the medicament cartridge 27 which can be moved by engagement and displacement of the ram 16a of the longitudinal or drive rod 15, which serves to expel the medicament from the cartridge 27. Figure 14 is a lower side view of the device 1 and the description of the upper side as shown in Figure 12 is equally applicable to the lower side.

The upper resistance pawl 26a and the distal edge thereof can be seen engaged with a rear face of a tooth of the upper set of ratchet teeth 18a on the longitudinal drive rod 15.

The upper drive pawl 14a can also be seen engaged with a rear face of a tooth of the upper set of ratchet teeth 18a on the longitudinal or drive rod 15.

In order to set a dose, a user must withdraw the push button 7 in a direction away from the cartridge receptacle 4, i.e. in a distal direction with respect to the body 2 of device 1.

As the push button 7 is withdrawn, as has been described in relation to Figures 3 to 8, the sliding or engagement protrusion 11a on the upper drive arm 12a of the driver, which is located in the diagonal slot 10a of the coupling element 22, slides in the slot, causing the driver 21 to rotate in an anti-clockwise direction about the pivot axis 13. During this movement, due to the offset of the sets of ratchet teeth 18a, 18b, one of the resistance pawls 26a, 26b acts to resist movement of the drive rod 15 in a distal direction by engagement with the rear face of the tooth.

As the driver 21 rotates, one of the drive pawls 14a, 14b slides from between a space or valley between two longitudinally adjacent peaks of two teeth, over the front tooth face and ridge of a tooth such that it proceeds to be located in the longitudinally adjacent space or valley between successive teeth. The other of the drive pawls also moves, but due to the offset in the sets of ratchet teeth 18a, 18b does not necessarily end up on the same part of a tooth. At this stage, the push button is then in a retracted state as shown in Figures 15 and 17 which show cross sections D-D and C-C along the parallel longitudinal planes shown in Figure 16.

Upon the subsequent displacement of the dosage setting means 7 towards the proximal end 3a of the body 2 of device 1, the sliding protrusion 11a moves along the slot 10a in the coupling 22. As a result, the driver 21 rotates in a clockwise direction about the pivot point 13. One of the drive pawls 14a, 14b on the driver 21, normally a drive pawl positioned behind a peak of a tooth, engages with the rear face of the tooth in the set of ratchet teeth 18a, 18b in which it is located such that the longitudinal rod is displaced upon further

movement of the dosage setting means in an axial direction in order to administer a dosage of medicament.

This operation, i.e. the continued withdrawal and subsequent depression of the push button 7, serves to move the drive pawls 14a, 14b successively into subsequent valleys or spaces between the teeth and drive the drive rod 15 towards the proximal end 3a of the body 2 of device 1. After the drive pawl reaches the surface 28a, 28b after the last tooth of the drive rod 15, no further displacement can be made.

The resistance pawls 26a, 26b are fixed to the body 2 of the device 1 and serve to resist or prevent movement of the drive rod ("expelling means") 15 in a direction opposite to the administering direction, i.e. in a direction towards the proximal end 3a of the body 2 of device 1. This ensures a consistent displacement of the drive rod 15 in the proximal direction only and prevents backlash or displacement of the drive rod 15 in the distal direction.

All of the sets of ratchet teeth 18a, 18b are provided on a common side of the drive rod 15 and therefore all the resistance pawls 26a, 26b and drive pawls 14a, 14b are arranged to face a common side of the drive rod.

As the drive rod 15 is displaced in the proximal direction of the device 1, the resistance pawls 26a, 26b slide over the ratchet teeth 18a, 18b on the drive rod 15.

Figures 18a, 19a, 20, show more detailed side, plan and perspective views of a drive rod 15 having offset sets of teeth.

The drive rod 15 comprises two sets of ratchet teeth 18a, 18b separated by a divider 24. The two sets of ratchet teeth 18a, 18b are offset, i.e. engaging faces of the upper set of ratchet teeth 18a, are offset from the engaging faces of the lower set of ratchet teeth 18b in a direction parallel to the longitudinal axis of the drive rod 15. This can be more clearly seen in details A and B shown in Figures 18b and 19b.

As shown in Figure 18b, each tooth has a ridge or peak 29c, a sliding front face 29a over which the pawls slide and an engagement rear face 29d as well a valley centre 29b. The teeth in each set of ratchet teeth 18a, 18b on opposing sides of the expelling means are equally spaced from one another. The offset between the two sets of ratchet teeth 18a, 18b in the embodiment is equal to half the spacing between adjacent teeth in either of the first or second sets of ratchet teeth 18a, 18b.

In the embodiments described, the upper and lower resistance pawls 26a, 26b are arranged in adjacent alignment. Similarly, the upper and lower drive pawls 14a, 14b are also arranged

in adjacent alignment. Due to the offset of the two sets of ratchet teeth 18a, 18b on the drive rod 15, when driving the driver 21, as described above, during each sequence of withdrawing the push button 7 and subsequently depressing the push button 7, only one set of resistance pawl 26a and drive pawl 14a engage fully with one set of the ratchet teeth, i.e. only one of the drive pawls 14a causes the drive rod 15 to be displaced and only one of the corresponding resistance pawls 26a prevents return movement of the drive rod 15. During a subsequent sequence, the other set of drive pawl 14b and resistance pawl 26b fully engages with the other set of ratchet teeth 18b, and so on.

Accordingly, the offset of the ratchet teeth 18a, 18b provides a ratchet with finer resolution of movement, which is equal to the distance between the valley of one tooth in one of the sets of ratchet teeth 18a and the valley of an adjacent tooth in the other of the sets of ratchet teeth 18b. This offset is shown in Figure 19b at item 30.

It follows that movement of the drive rod 15 in the embodiment described proceeds in smaller increments than if no offset were to be provided between the two sets of ratchet teeth 18a, 18b. This enables a finer dose or volume of medicament to be administered with the device 1 as a result of movement or displacement of the drive rod 15.

The offset in the case of a drive rod 15 with offset sets of ratchet teeth 18a, 18b may be adjusted according to requirements. For example, a drive rod 15 may be chosen with a larger tooth pitch in the sets of ratchet teeth in order to administer a large dosage during each cycle of movement. Conversely, a smaller pitch could be chosen. The other components however generally remain the same.

As previously mentioned, a drive rod 15 where the sets of ratchet teeth are in alignment is also envisaged. In such an embodiment, both drive pawls and resistance pawls would be in engagement with corresponding parts of teeth in each set of teeth at the same time in order to drive the expelling means and resist movement of the expelling means in the distal direction of the device.

With all of these embodiments, providing the ratchet teeth 18a, 18b on a single, common side of the drive rod 15 enables a more compact and simple device construction to be achieved.

As an alternative to offset teeth on the drive rod 15, the adjacent ratchet teeth may be aligned with the drive pawls offset from one another. Indeed, a single set of ratchet teeth can be provided which can engage with each of the drive pawls and each of the resistance pawls.

It is envisaged that other coupling mechanisms may be provided to displace the drive rod and the present invention should not be considered limited to the exemplary coupling mechanism as shown in the Figures.

Figures 21 and 22 show a further embodiment of the device 1 having an indicator element 34 visible through a display window or aperture 31 provided in a surface of the body 2 of the device. Figures 21 and 22 have drive mechanisms configured to drive a drive rod 15 as described above in relation to Figures 1 to 20. However, the indicator element 34 and display window 31 arrangement of Figures 21 and 22 may be applied to devices with different drive mechanisms, including inhaler devices (not shown).

Figure 21 shows the device 1 with the push button 7 in a depressed state. In this position of the push button 7, a first state indicator 32a of "0" provided on the indicator element 34 is visible in the window 31. This first state indicator 32a could for example indicate to a user that no dosage has been set by the push button 7.

Figure 22 shows the device 1 with the push button 7 in a withdrawn or retracted state. In this position of the push button 7, a second state indicator 32b of "5" provided on the indicator element 34 is visible through the window 31. This second state indicator 32b could for example indicate to a user that a dosage of 5 units has been set for administration. Of course, other indications of state could be provided such as arrows or other visual or tactile markers or characters.

Figure 23 shows a view of the device 1 with part of the body removed to show the internal drive mechanism and also the mechanism to move the indicator element 34. The drive mechanism includes a driver 21 rotatable about a pivot axis 13. The driver 21 includes a protrusion 11a which engages through a diagonal, linear slot in a coupling element 22. The driver 21 drives a drive rod 15 provided with sets of ratchet teeth 18a, 18b. The drive rod 15 comprises a ram 16a which can be extended or displaced through an aperture 25 in order to displace a plunger in a medicament container such as an insulin cartridge (not shown). The function of such a mechanism has already been described in relation to Figures 1 to 20 and will not be described further here.

The coupling 22 includes a planar surface 9a, as described above. The surface 9a is provided with distal and proximal protrusions 33a, 33b, which are spaced apart a distance greater than the axial length of the indicator element 34, which is disposed in the body 2 between said protrusions 33a, 33b.

A protrusion 35c is provided along an edge of the window 31, the protrusion 35c being configured to engage with each of two spaced indents 35a, 35b located along an edge of the indicator element 34 parallel to the direction of movement of the indicator element 34. When engaged with either of the indents 35a, 35b, the protrusion 35c acts to inhibit free axial linear movement of the indicator element 34, which in this embodiment is formed as a substantially rectangular planar element.

The indents 35a, 35b and the protrusion 35c combine with protrusions 33a, 33b on the body 2 to form motion conversion means, the function of which will now be described with reference to Figures 25 to 28 which are sectional views through section E-E as shown in Figure 24.

When the push button 7 of the device is fully depressed into the body 2 of the device, as shown in Figure 25, the indicator element 34 is positioned with its distal edge engaged with protrusion 33a towards the rear or distal end of the device body 2. The indication "0" is shown in the window 31, represented by the dashed outline.

Upon initial withdrawal of the push button 7, as shown in Figure 26, the indicator element 34 remains stationary relative to the body 2 of the device thanks to protrusion 35c along the edge of window 31 engaging with rearmost indent 35a of the indicator element 34. This engagement acts to resist axial movement of the indicator element 34 relative to the body 2 such that the indicator element 34 slides over the surface of the coupling 22 when during an initial movement of the push button 7 and, as there is no movement of the indicator element 34 relative to the body 2, the indication "0" remains visible to a user through window 31, indicating, for example, that the dosage has not yet been set.

Upon further withdrawal of the push button 7, as shown in Figure 27, the proximal protrusion 33b engages with the proximal edge of the indicator element 34, which causes the indicator element 34 to be displaced in a distal axial direction of the body 2 of the device, in doing so overcoming the resistance provided by the engagement of the protrusion 35c and distal indent 35a, such that the indication "0" 32a begins to move out of visibility in the window 31.

Figure 28 shows the fully retracted position of the push button 7. Here it can be seen that the proximal protrusion 33b on the coupling 22 maintains its engagement with the indicator element 34 thereby completing the axial movement of the indicator element 34 to bring indication "5" 32b into visibility in the display window 31. This could for example indicate to a user that the dosage has been correctly set and the push button 7 could be depressed in order to administer the dose. In this final fully withdrawn position of the push button 7, the

protrusion 35c along the edge of window 31 becomes engaged with the foremost indent 35b on the edge of the indicator element 34.

Upon subsequent depression of the push button 7 in order to administer a dose, the indicator element 34 again initially remains stationary relative to the body 2 due to the resistance of protrusion 35c being engaged with the foremost indent 35b on the edge of the indicator element 34 such that the indication "5" 32b remains visible in the window 31 during an initial movement of the push button 7. This could, for example, indicate to a user that the dose has not yet been fully administered.

Similarly as when the push button 7 is withdrawn, upon continued depression of the push button 7, the distal protrusion 33a on the coupling 22 engages with the corresponding distal edge of the indicator element 34 thereby to move it in the proximal direction relative to the body 2 of the device such that the indication "0" 32a is again displayed in the window 31 and protrusion 35c again engages with rearmost protrusion 35a on the edge of the indicator element 34.

Although in the embodiment, the indicator element 34, here in the form of a sliding indicator, has been provided with indents 35a, 35b at each end of travel, it is also envisaged to provide a protrusion on the edge of the sliding indicator 34 which engages with corresponding indents provided on a corresponding edge of the window 31.

It will be understood that the mechanism provides a magnitude of displacement of the indication element 34 which is different to (i.e. less than) the magnitude of displacement of the dosage setting means. In the embodiment, the spacing of the protrusions 33a, 33b on the surface 9a of coupling 22 provides a relative or "lost motion" movement between the push button 7 and the indicator element 34. This allows the indications 32a, 32b to remain visible and unchanged during phases of the operation of the device. This can lead to improved operation of the device as the displayed indications 32a, 32b remain consistent and unchanged.

While in the embodiment, an axially moveable push button 7 has been shown to provide drive of the mechanism, other forms of dosage setting means may be provided such as a dial, rotatable about the longitudinal axis of the device while still embodying the above-described arrangement of the indicator element 34. An example of such a dosage setting means with a rotating dial 36 on a cylindrical body 37 is shown in Figures 29 to 31 in a fully screwed in position in Figure 29, a fully retracted, i.e. screwed-out position in Figure 30 and a fully depressed position in Figure 31.

A further embodiment of a device 1 is shown in Figures 32 to 39 comprising a different indicator element arrangement. Externally, the device 1 is formed similarly to the embodiments described above, comprising a body 2, a cartridge receiver 4, a cartridge with a threaded portion 5 for receiving an injection needle, a push button or dosage means 7 and a window or aperture 31. Through the window 31, an indication, here the number "5" is visible, which is on an indicator element 42.

Figure 33 shows a cross-section through the device shown in Figure 32. The dispensing mechanism is similar to that shown in Figures 1 to 31 and comprises a driver 21 with drive pawl 14a, 14b and resistance pawls 26a, 26b arranged to engage with ratchet teeth 18a, 18b on a drive rod 15.

A coupling element 38 is provided, which comprises a diagonal slot 10a within which a protrusion 11a is received. These parts function similarly to the coupling element 22 described in relation to Figures 1 to 31 in order to set a dose with the push means 7 and administer a dose. The dosage and administering functions will accordingly not be described further here.

In contrast to the device of Figures 1 to 31, as shown in Figure 33, the coupling element 38 comprises a rectangular aperture 43. Along one edge of the aperture, an opening 45 is provided in which a conversion means in the form of lever 39 is positioned. The lever 39 extends through the opening 45 into the aperture 43 from a pivoted connection 40 on the body 2 located outside the aperture 43.

The indicator element 42 is provided with a pair of spaced protrusions, represented by the dashed lines 41a, 41b. The protrusions 41a, 41b extend from the rear surface or underside of the indicator element 42 (not shown in Figures 33 or 35) and are positioned towards either end of the indicator element 42 in the longitudinal direction of the device. When assembled, the protrusions 41a, 41b extend into the aperture 43 such that they are positioned either side of the distal end of the lever 39, i.e. the end of the lever 39 furthest from the pivoted connection 40, such that the indicator element 42 rests atop the lever 39.

Figure 33 shows the device with the push button 7 in a retracted position. Here it can be seen that the lever 39 is in contact with the rearmost or distal protrusion 41b of the indicator element 42 and is orientated such that the lever 39 is angled towards the distal end of the body 2.

Figure 34 shows an external view of the device of Figures 32 and 33 when the push button 7 is in a fully depressed position. In this position, the indicator element 42 now shows the

indication "0". As has been described in relation to Figures 28 to 31, the indication "0" can be used to indicate to a user that no dose has been set and the indication "5" can be used to indicate that a dose of 5 units has been set, for example.

As can be seen in Figure 35, with the push button 7 in a fully depressed state, the rectangular aperture 43 has been axially displaced in the proximal direction of the device relative to the position of the rectangular aperture 43 of the device in the state shown in Figure 33. It can be seen that the opening 45 in the side of the aperture 43 has therefore also moved in a corresponding towards the proximal end of the body 2. As the lever 39 is pivotally attached to a fixed pivot 40 on the body of the device, the movement of the aperture 43 and the opening 45 therein causes rotation of the lever 39 about the pivot 40. As the distance between the pivot 40 and the opening 45 is less than the distance between the opening 45 and the distal end of the lever 39, it can be appreciated that a movement of the aperture 43 results in a movement of the distal end of the lever 39 of a greater magnitude, which moves the indicator element 42, via the protrusions 41a, 41b, a corresponding distance. Thus it can be seen that the opening 45 acts as a fulcrum 43.

The relative lengths of the lever 39 between the pivot 40 and the fulcrum 43 and the length between the fulcrum 43 and the distal end of the lever 39, or its point of contact with the protrusions 41a, 41b of the indication element 42, may be selected to produce a desired magnitude of movement of the indication element 42 relative to the dosage setting means 7.

As shown in Figure 35, in the depressed state of the push button 7, the distal end of the lever 39 is in contact with the protrusion 41a of the indicator element 42 towards the proximal end of the body 2 and has moved the indicator element 42 such that the indication "0" is now visible in the aperture or window 31 as shown in Figure 34.

The lever 39 acts to convert a movement of a first magnitude of the push button 7 or coupling 38 into a movement of a second, greater magnitude of the indicator element 42. In a device with limited space, the lever 39 can provide a greater movement and functionality of the indicator element 42 than if the movement of the indicator element 42 was limited only to the same magnitude or degree of movement of the push button 7. For example, a 4mm movement of the indicator element 42 can result from just a 2mm axial movement of the push button 7, thereby providing a "gained motion" effect.

It will be understood however, that the opening 45 or fulcrum 43 and lever 39 may be arranged with a shorter distance between the opening 45 and the distal end of the lever 39 than the distance between the pivoted end 40 of the lever 39 and the opening 45 such that a

smaller magnitude of movement of the indicator element 42 is achieved relative to the magnitude of movement of the push button 7.

As a further alternative, the lever 39 may be formed of a resiliently flexible material such that when the indicator element 42 reaches the limit of its movement, if the lever 39 should be caused to rotate further, for example if the manufacturing tolerances of the lever 39 are such that it is slightly longer or wider than necessary or if the fulcrum 43 or opening 45 position is not precisely located, the lever 39 will flex to prevent damage to itself or to the indicator element 42.

Figures 36 to 39 show some assembly steps of the device with the lever. Figure 36 shows the body, driver 21 and drive rod 15 located in the body 2. The body 2 is formed with a circular aperture 40 for receiving a support 44 of the lever 39.

Figure 37 shows the support 44 of the lever 39 located in the aperture 40. The lever 39 is pivotable about the axis of the circular aperture 44. Although shown in Figure 37 as a separate part in the embodiment, the lever 39 could be formed integrally with the body 2, yet still able to pivot.

Figure 38 shows the device with the coupling 38 attached to the push button 7 fitted. The lever 39 can be seen located in the opening 45 provided along one longitudinal side of the rectangular aperture 43.

Finally, Figure 39 shows the indicator element 42 positioned atop the coupling 38 and hence lever 39. The indicator element 42 is formed with the lever-engagable protrusions 41a, 41b underneath, which were shown and described in relation to Figures 33 and 35.

The indicator element 42 is shown provided with indents 46a, 46b, which have a similar function to the indents 35a, 35b described in relation to Figure 23 and 25 to 28 to resist free motion of the indicator element 42.

Although not shown in the Figures, it is envisaged that instead of a lever 39, the conversion means could comprise geared or threaded components, with the gearing or threading being chosen or configured such that a predetermined magnitude of movement of the indicator element 34 is achieved for a predetermined differing magnitude of movement of the push button 7.

In each of the aforementioned embodiments, the dosage setting means 7 could be indirectly or directly coupled to the indication element 34, 42. The indicator element 34, 42 is typically constrained within a channel or guide elements to limit the lateral movement thereof.

Figure 40 shows an alternative dispensing mechanism provided in a device 1. The device 1 includes a medicament container in the form of a cartridge receptacle 4. Within the cartridge receptacle 4, a cartridge is contained with a screw thread 5 at the proximal end to receive a needle.

Similarly to the embodiments shown in Figures 1 to 39, the dispensing mechanism comprises a dosage setting means in the form of a push button 7. The dosage setting means is formed with a shaft 8 connecting the push button 7 with a plate 38 in which a diagonal slot 52a is formed similarly to the embodiments of Figures 1 to 39. Accordingly, this aspect of the embodiment will not be described in further detail.

An expelling means 51 is provided in the form of a ram with a circular disc 52 to engage with the plunger of a cartridge in order to dispense a liquid medicament therefrom.

A drive element 48 is provided. The drive element 48 comprises an arm 48a connected towards the proximal end thereof to a pivot point 49 formed in the body 55 of the mechanism. At the distal end of the drive element of driver, a circular protrusion or follower 52a is provided which engages with the diagonal slot 10a in the plate 38 of the dosage setting means 7.

The drive element 48 comprises a further pair of arms 48b which extend from the distal end of the driver 48 in the proximal direction of the mechanism and device and angled relative the arm 48a connected to the pivot point 49. Each of the pair of arms 48b comprises at their proximal, free ends, a drive pawl 48c.

The expelling means 51 comprises a rack of teeth 54 which are formed to engage with the teeth 47c of a drive wheel 47. The drive wheel 47 has a central section 47c formed as a gear wheel which engages with the teeth 54 of the rack of the expelling means 51.

The drive wheel 47 is formed with two ratchet wheels 47a, 47b at either end. The ratchet wheels 47a, 47b have a larger diameter to the diameter of the central gear wheel 47c. The teeth of the ratchet wheels are offset relative to one another, i.e. the faces of the teeth in one ratchet wheel are offset from the faces of the teeth in the other ratchet wheel. Similarly to the embodiments described in relation to Figures 1 to 39, this can provide a finer movement and thus dosage.

Biasing pawls 50 are formed with the body 55 and are angled in the proximal direction of the device. Two such biasing pawls are provided. One upper biasing pawl engages with one of the ratchet wheels 47a and the other, lower biasing pawl engages with the other of the ratchet wheels 47b. It can therefore be seen that these biasing pawls 50 serve to prevent anticlockwise (as seen in Figures 40m, 41) rotation of the drive wheel and can therefore be seen to act similarly to the biasing pawls described in relation to Figures 1 to 39. The biasing pawls 50 face a common side of the ratchet wheels provided on the drive wheel.

Figure 40 shows the device 1 with the push button 7 in a depressed position. As can be seen from Figures 40 and 41, upon withdrawal of the push button 7 into the withdrawn position as shown in Figure 41, the protrusion 52a on the driver 48 follows the diagonal slot 10a such that the driver 48 is caused to rotate anticlockwise about the pivot point 49. In so doing, the drive pawls 48c slide over the teeth in the ratchet wheels 47a, 47b, thus moving into successive valleys formed by the ratchet teeth. The biasing pawls 50 prevent rotation of the drive wheel in an anticlockwise direction during this movement of the drive pawls.

Upon the subsequent depressing of the push button 7 in the axial proximal direction, the driver 48 is caused to rotate about the pivot point 49. Due to the offset of the ratchet teeth in the ratchet wheels 47a, 47b, only one of the drive pawls 47a, 47b engages fully with an engaging face of one of the ratchet wheels 47a, 47b and rotates the ratchet wheel 47 about its axis 56 in a clockwise direction as viewed in Figure 41.

As the drive wheel 47 rotates, the gear teeth 47c, which are engaged with the rack of teeth 54 on the expelling means 51, rotate causing the expelling means to be displaced in an axial direction to deliver or administer a dose from the cartridge.

Figure 42 shows the expelling means 51, driver 48 and drive wheel 47. Due to the larger relative diameters of the ratchet wheels 47a, 47b to the size of the gear wheel 47c on the drive wheel 47, the expelling means sits between the drive arms 48c of the driver 48. This again allows for a more compact arrangement of components.

Figure 43 shows a view of the drive wheel 47. Each ratchet wheel 47a, 47b shares the same axis of rotation as the central gear wheel 47c located therebetween. The ratchet wheels 47a, 47b may be formed integrally with the gear wheel 47c.

As with the embodiments of Figures 1 to 39, the drive pawls could be offset rather than the ratchets on the drive wheel, with the ratchets of the drive wheel being in alignment.

Various modifications may be made to the embodiments described without departing from the scope of the invention as defined in the accompanying claims. Furthermore, a skilled

person will note that, though the terms “upper” and “lower” are used throughout the description for ease of reference to the figures, these terms are interchangeable with other differentiating terms for similar or identical features such as “first” and “second”, for example.

CLAIMS

1. A dispensing mechanism for administering a dosage of a medicament, the mechanism comprising:
 - a body; and
 - dosage setting means for setting the dosage of a medicament to be administered, the dosage setting means being moveable in a first direction for setting the dosage and in a second direction for administering the dosage,
 - wherein the mechanism further comprises an indication element, the indication element being arranged to be displaced by a predetermined movement of the dosage setting means; and
 - wherein the indication element is configured to remain unmoved relative to said body of the mechanism during at least part of said movement of the dosage setting means.
2. A dispensing mechanism as claimed in claim 1, wherein the indication element is movable within a guide channel.
3. A dispensing mechanism as claimed in claim 1 or 2, wherein the indication element is slidingly supported in, on or by the body.
4. A dispensing mechanism as claimed in any of claims 1 to 3, wherein the dosage setting means is operatively coupled to conversion means in the form of a first and a second engagement means, the first engagement means and the second engagement means being independently engageable with the indication element such that upon engagement movement of the dosage setting means causes displacement of the indication element.
5. A dispensing mechanism as claimed in claim 4, wherein the engagement means are arranged spaced apart a distance greater than the longitudinal length of the indicator element.
6. A dispensing mechanism as claimed in claim 5, wherein the engagement means are protrusions formed as part of the dose setting means.
7. A dispensing mechanism as claimed in any of the preceding claims, wherein the dosage setting means is linearly displaceable in a direction substantially parallel to the longitudinal axis of the body.

8. A dispensing mechanism as claimed in any of claims 1 to 6, wherein the dosage setting means is rotatable about an axis substantially parallel to the longitudinal axis of the body.

5

9. A dispensing mechanism as claimed in any of the preceding claims, further comprising resisting means arranged to resist movement of the indication element relative to movement of the dosage setting means.

10

10. A dispensing mechanism as claimed in claim 9, wherein the resisting means comprises a protrusion receivable in one or more corresponding recesses.

11

11. A dispensing mechanism as claimed in any of the preceding claims, wherein the mechanism includes an aperture through which at least a portion of the indication element is exposed to a user.

15

12. A dispensing mechanism as claimed in any of the preceding claims, wherein the indication element comprises tactile and/or visual indications.



20


13. A dispensing mechanism as claimed in any of the preceding claims, wherein the indication element is moved directly by the dosage setting means.


14. A dispensing mechanism as claimed in any one of claims 1 to 12, wherein the indication element is moved indirectly by the dosage setting means.




25




15. A medical device comprising a dispensing mechanism according to any of the preceding claims.


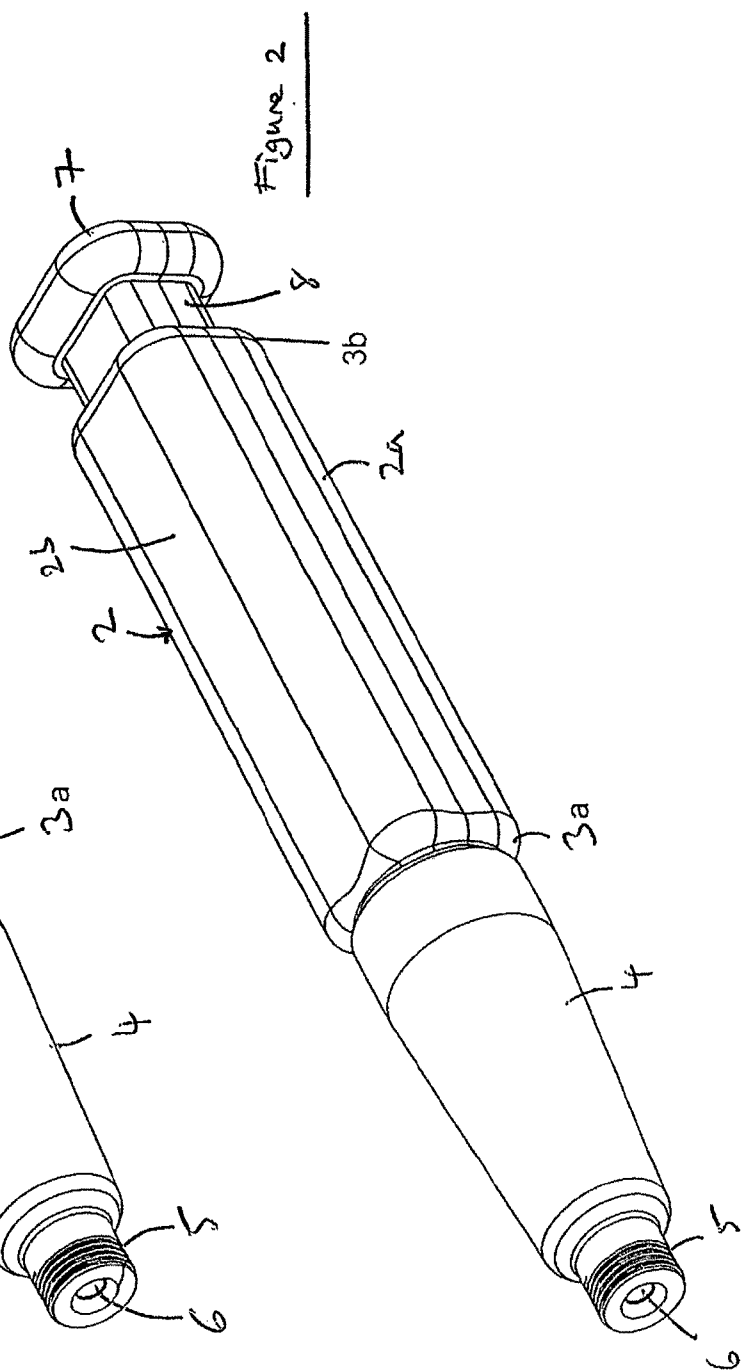
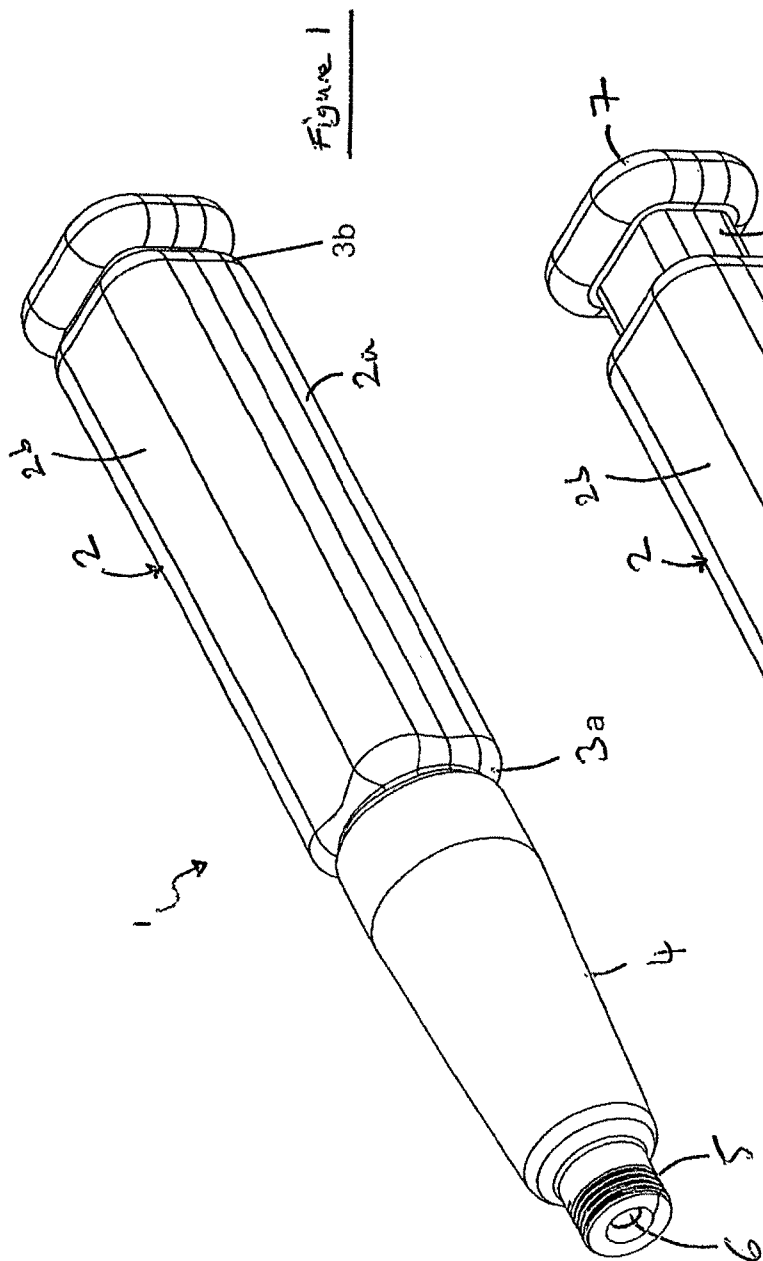


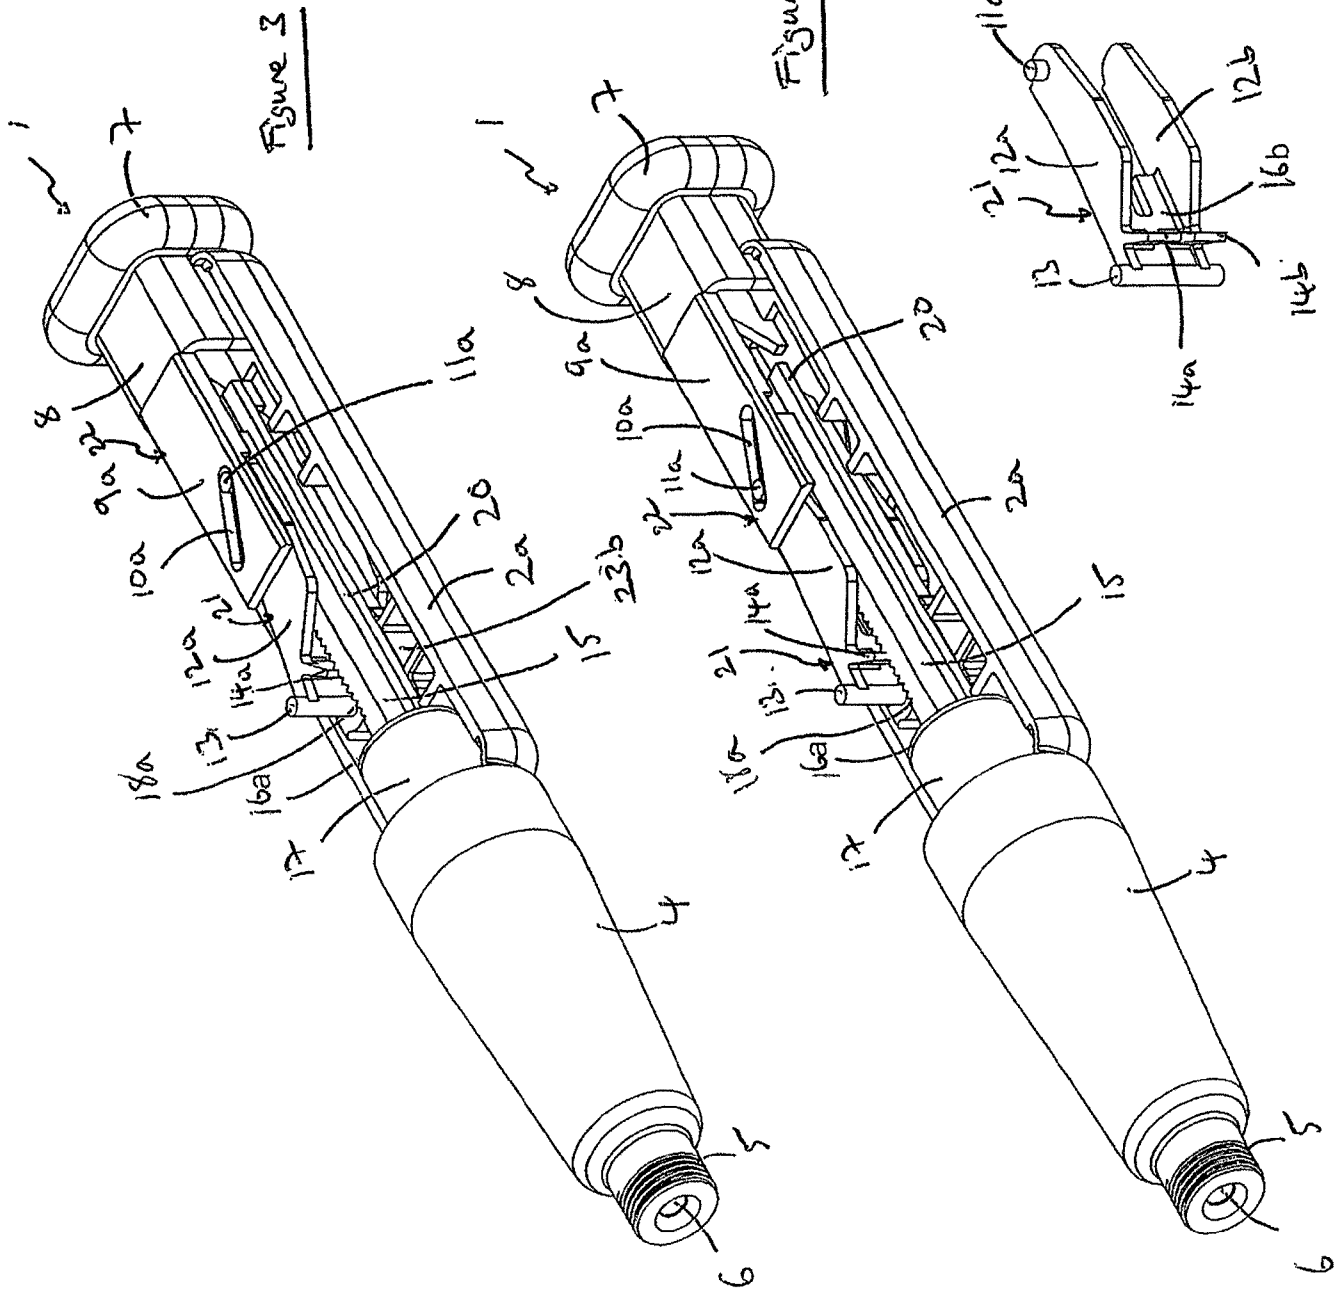



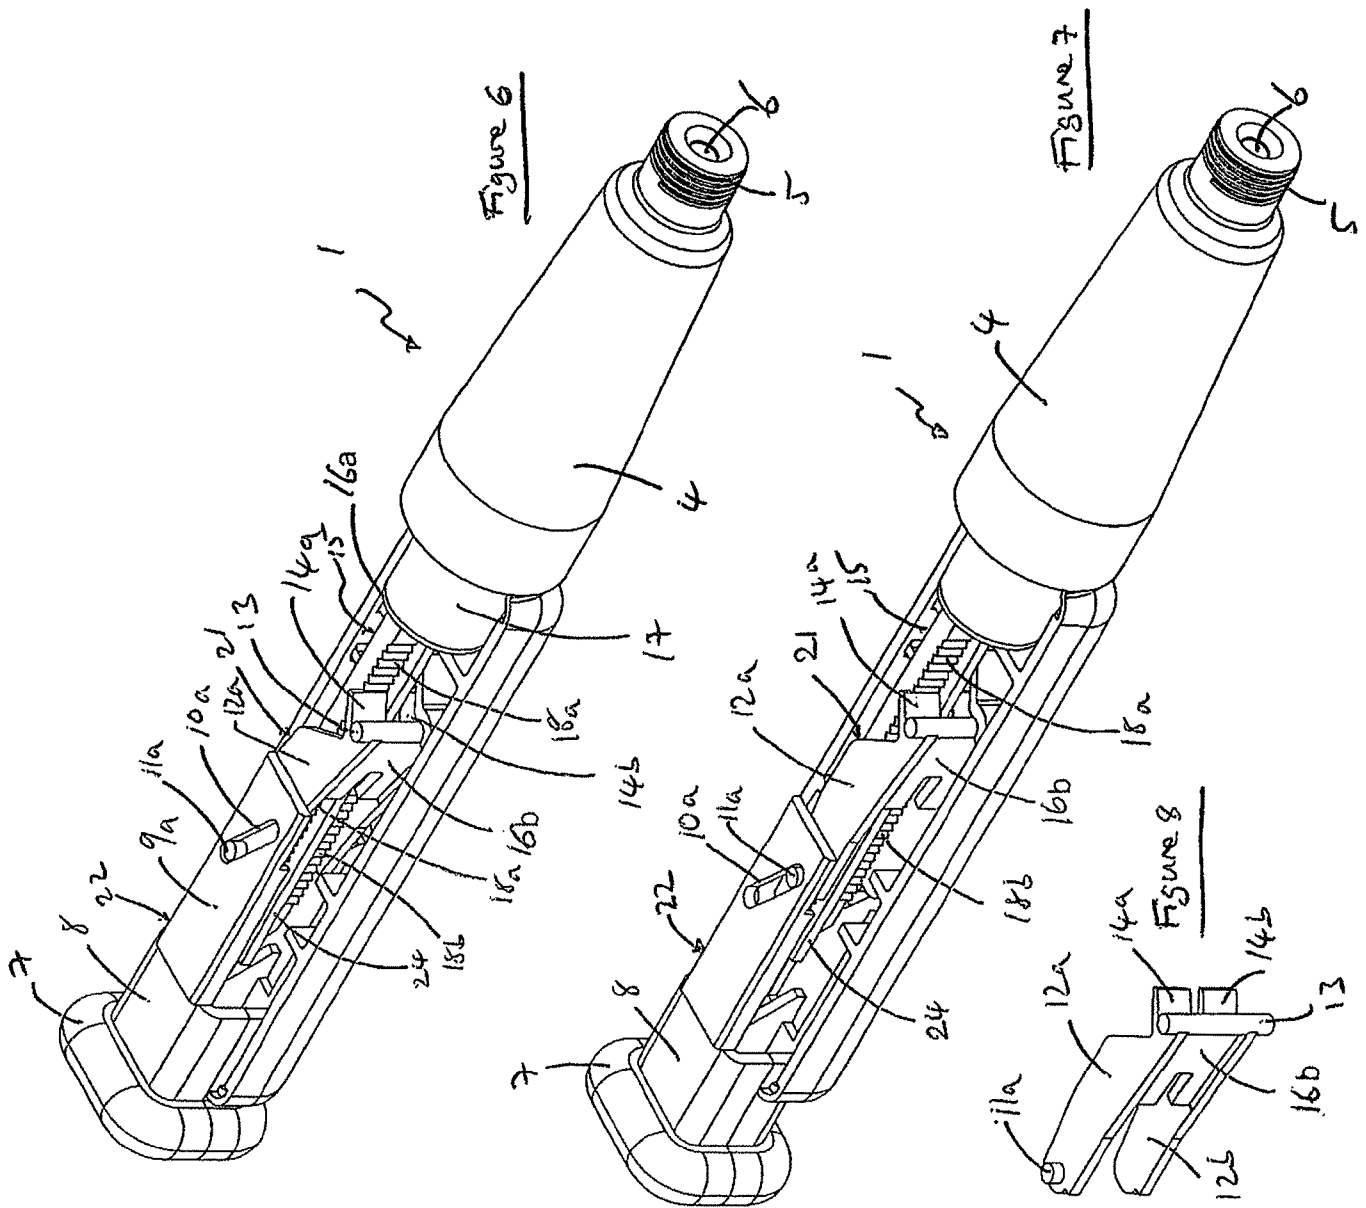


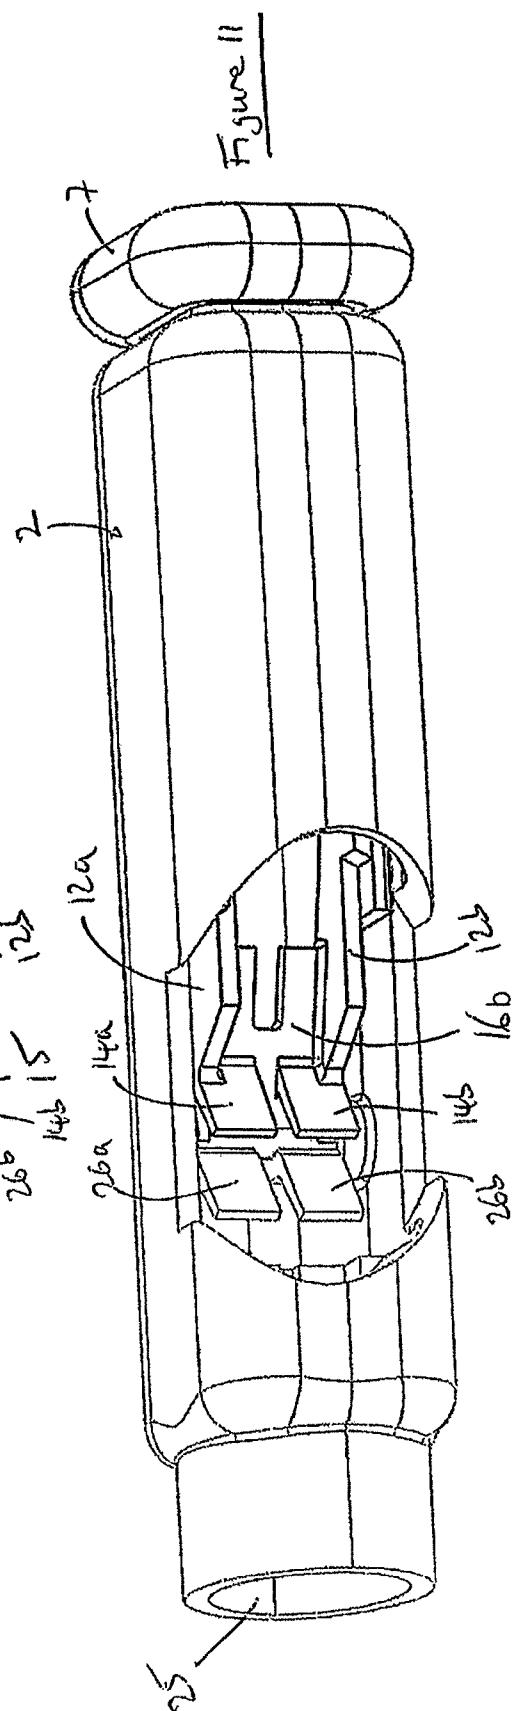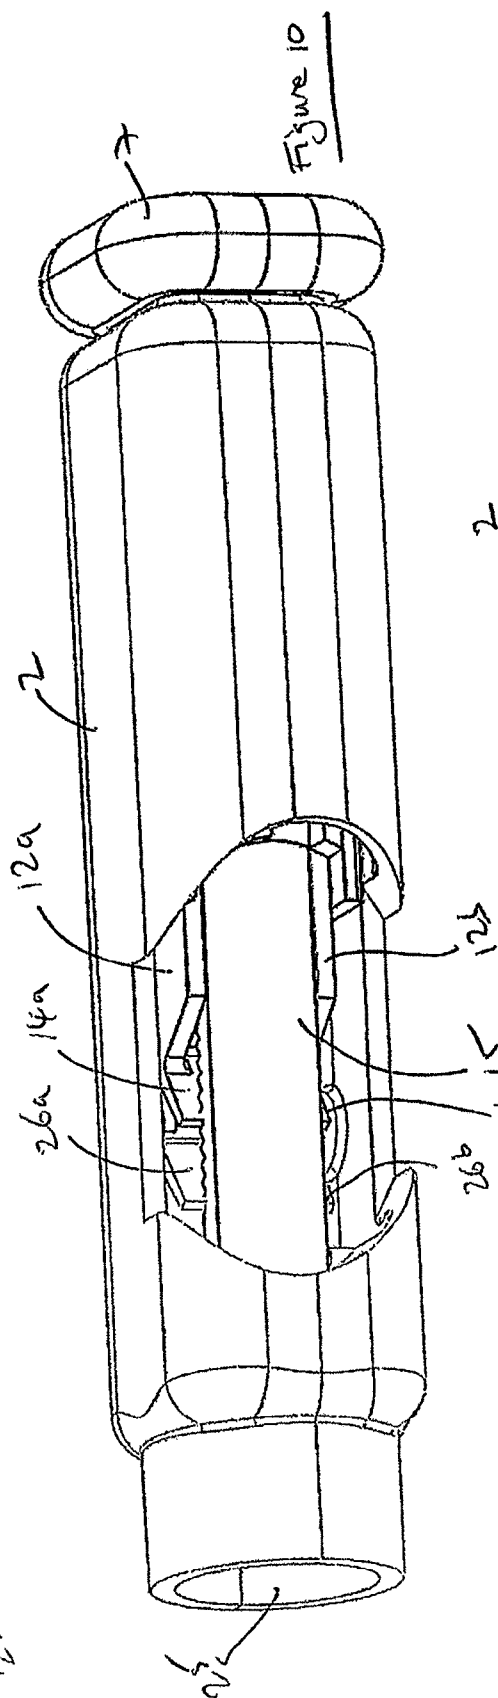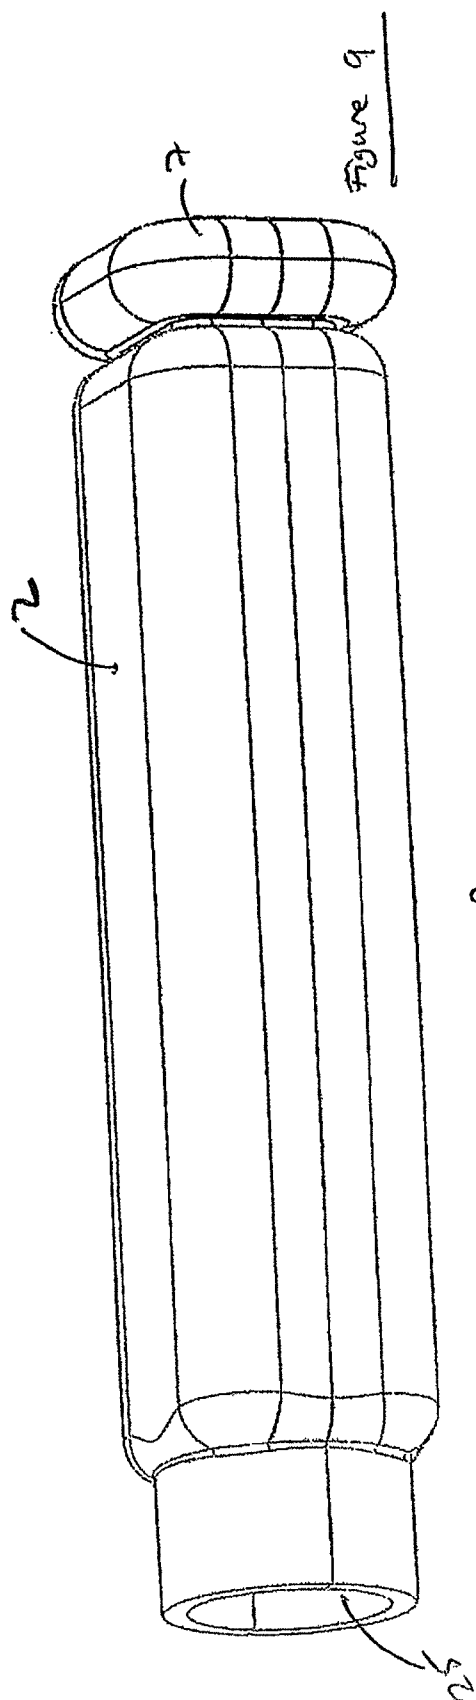


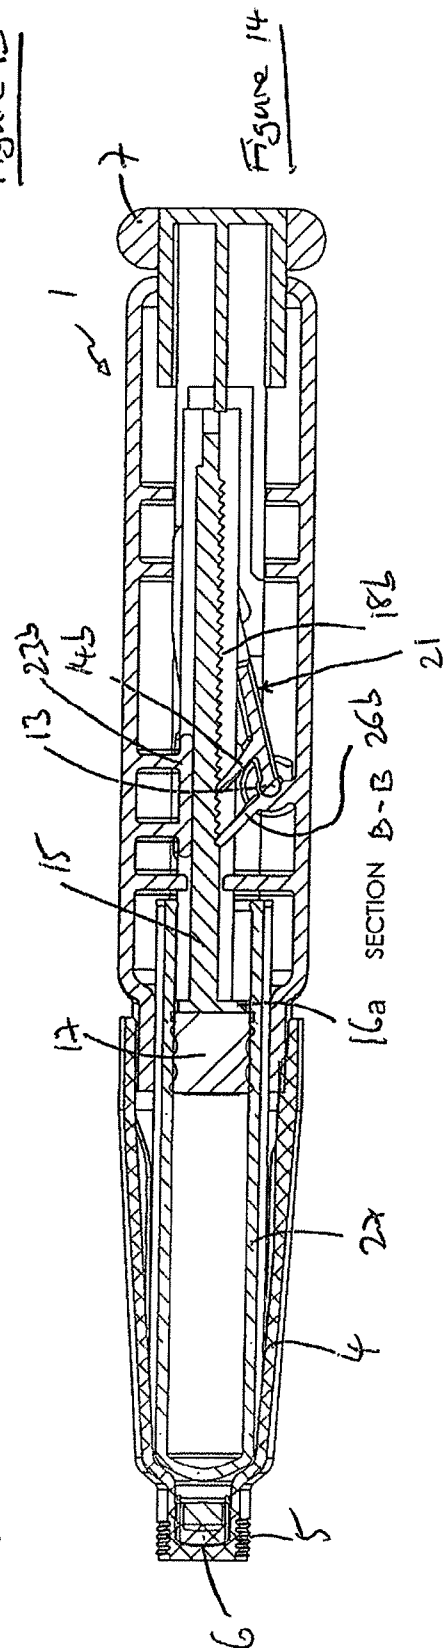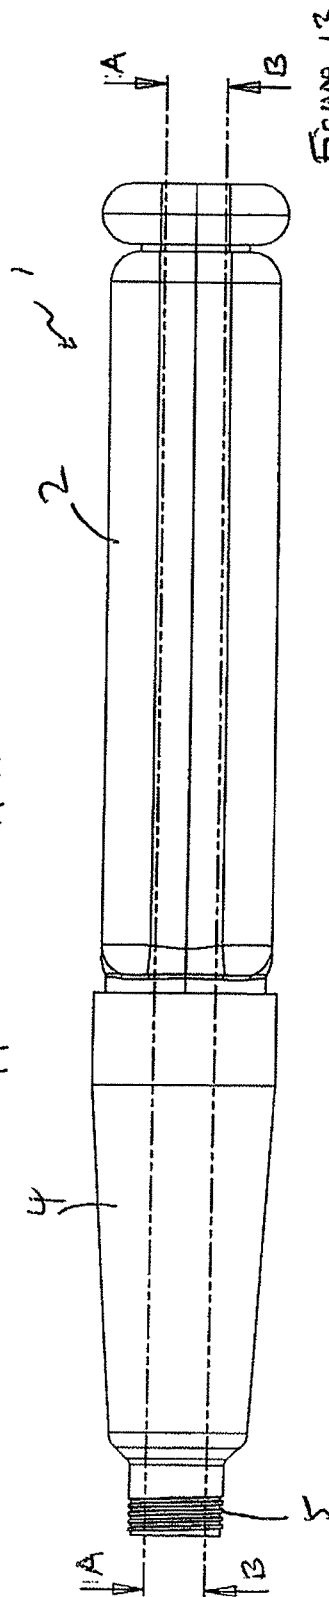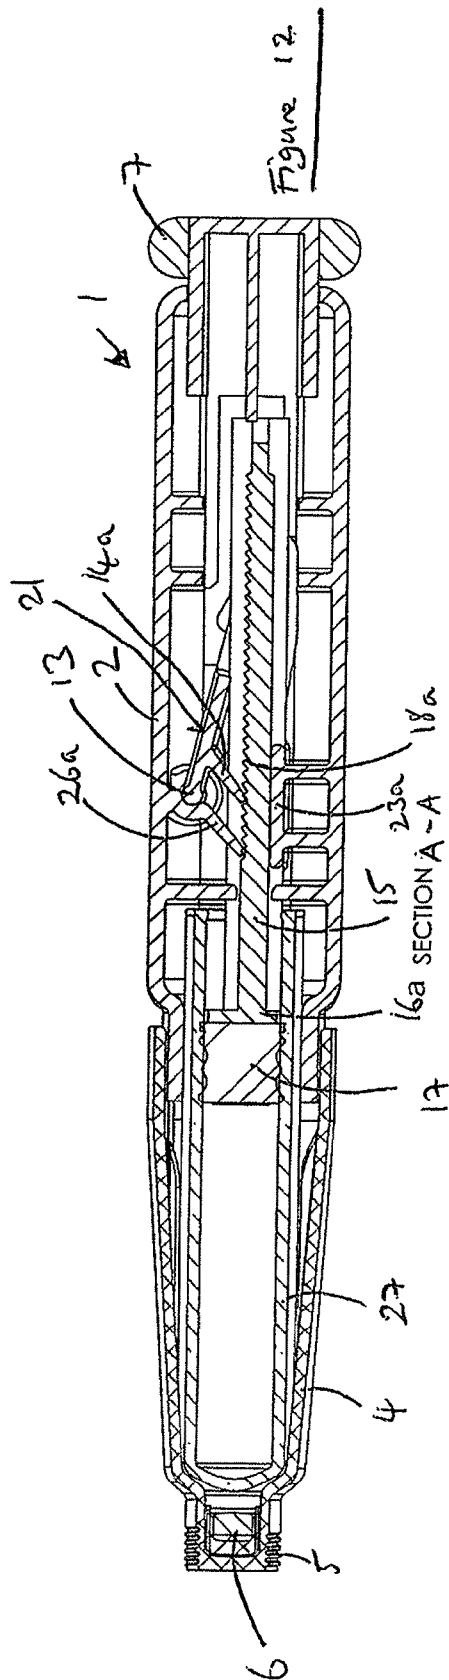

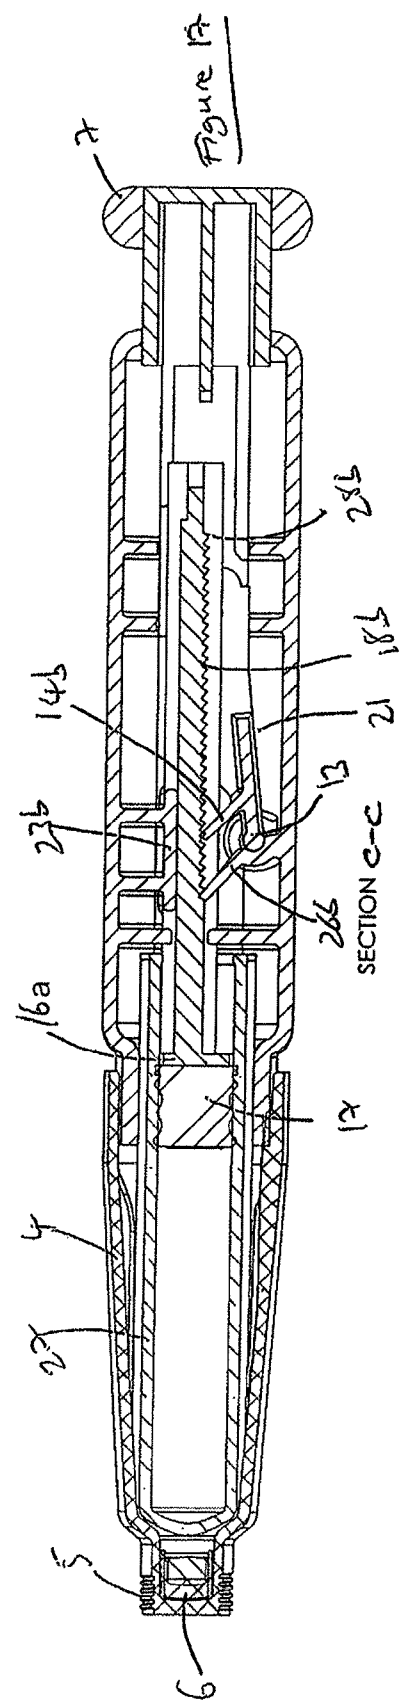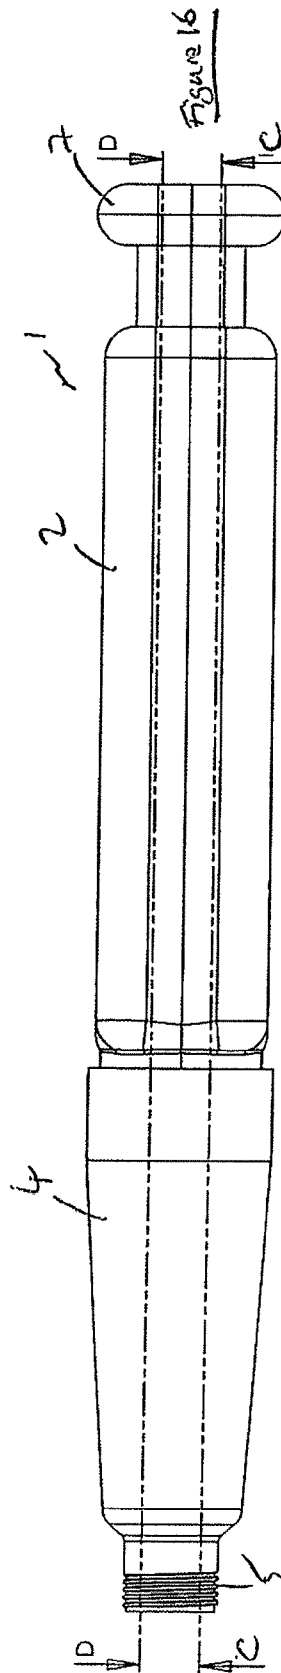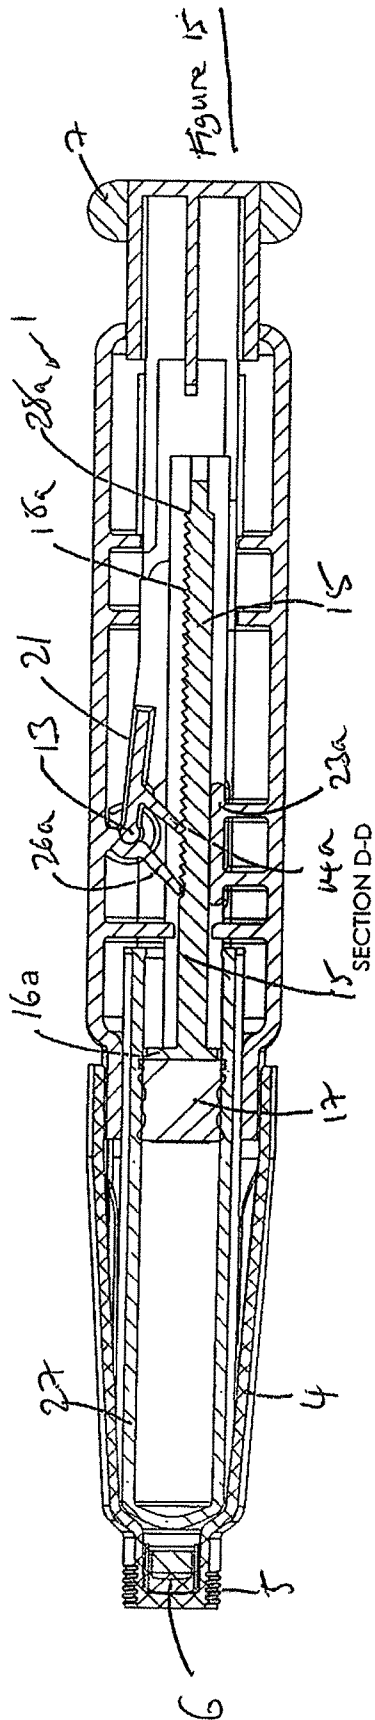

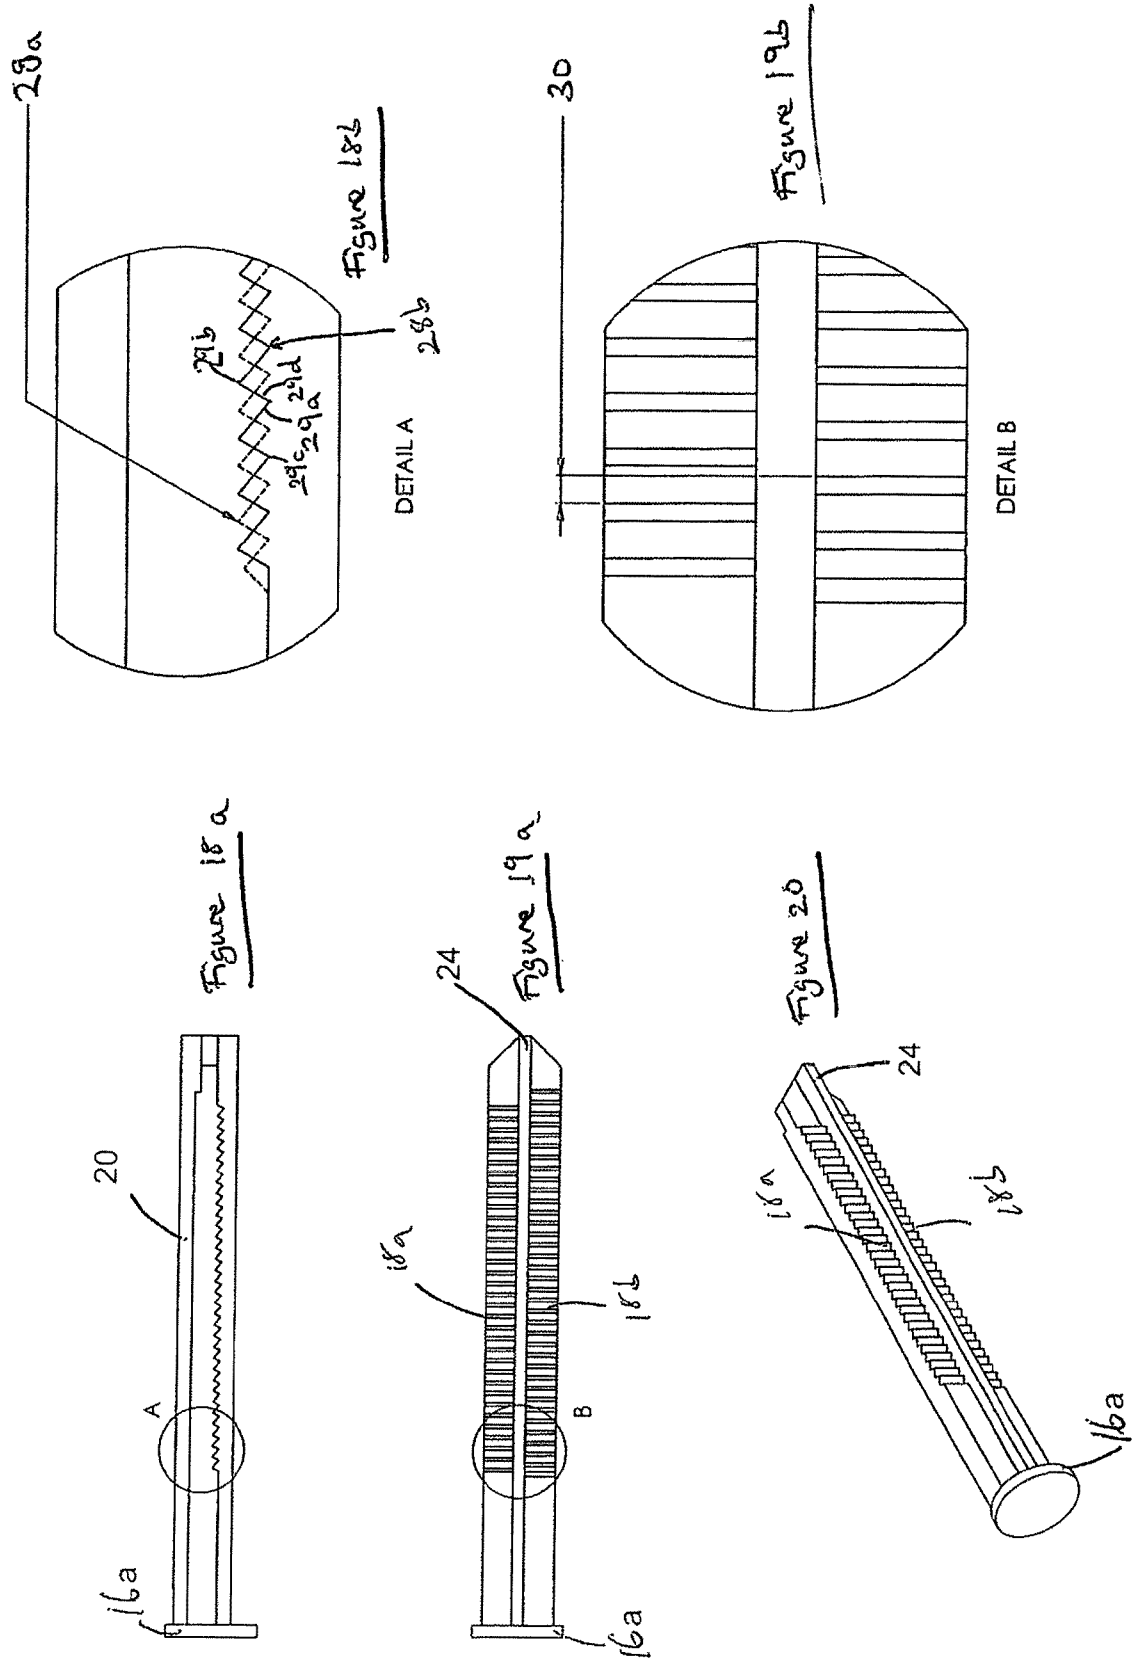

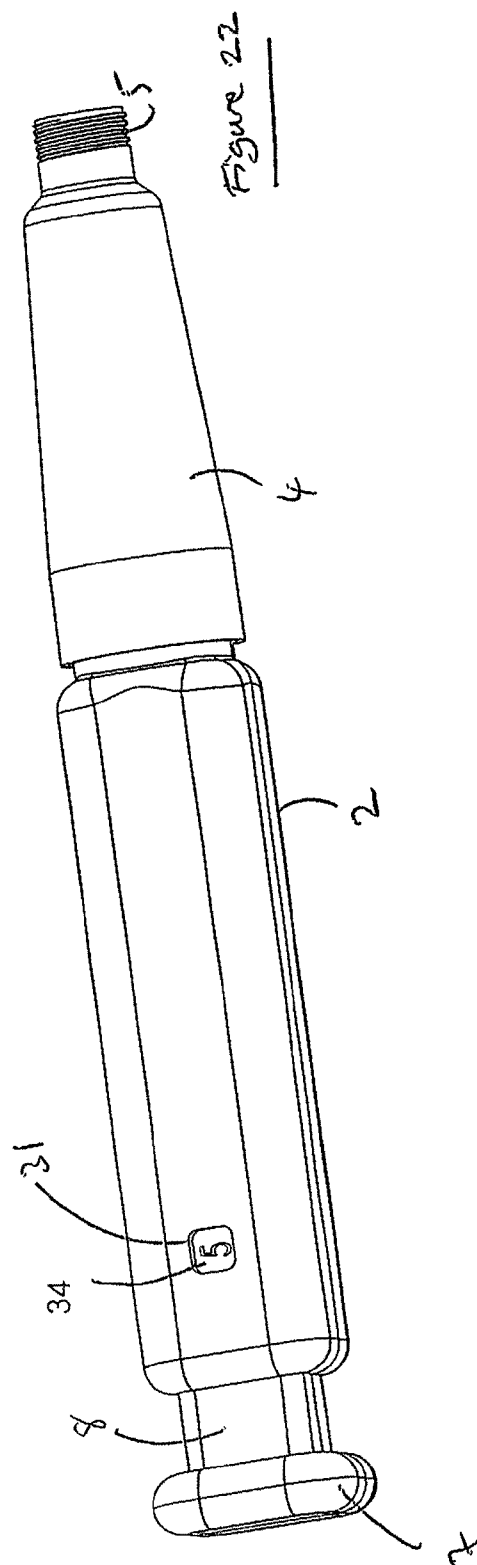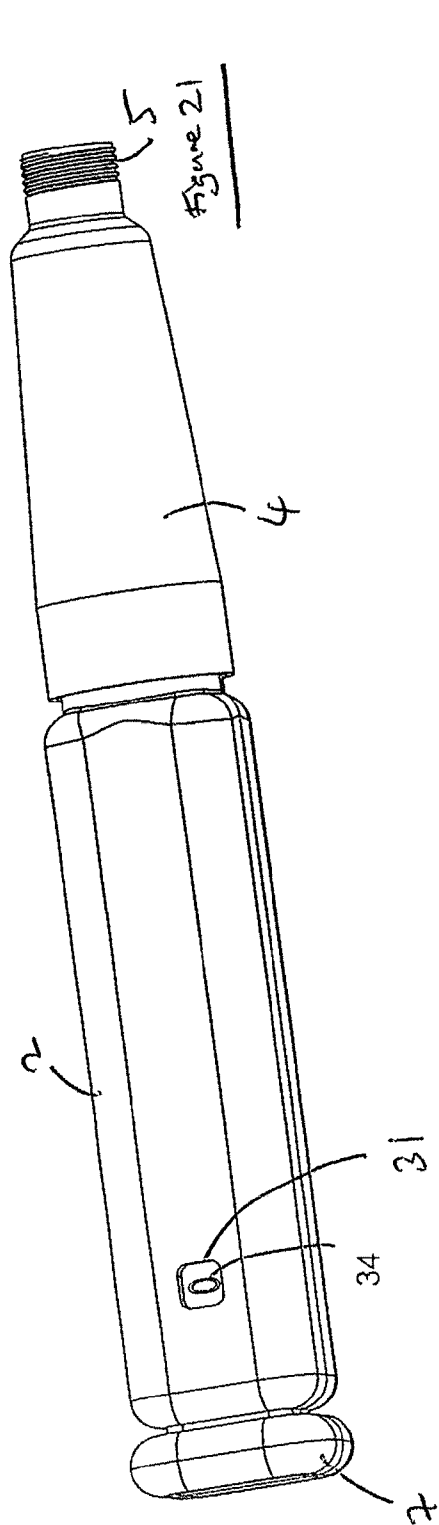

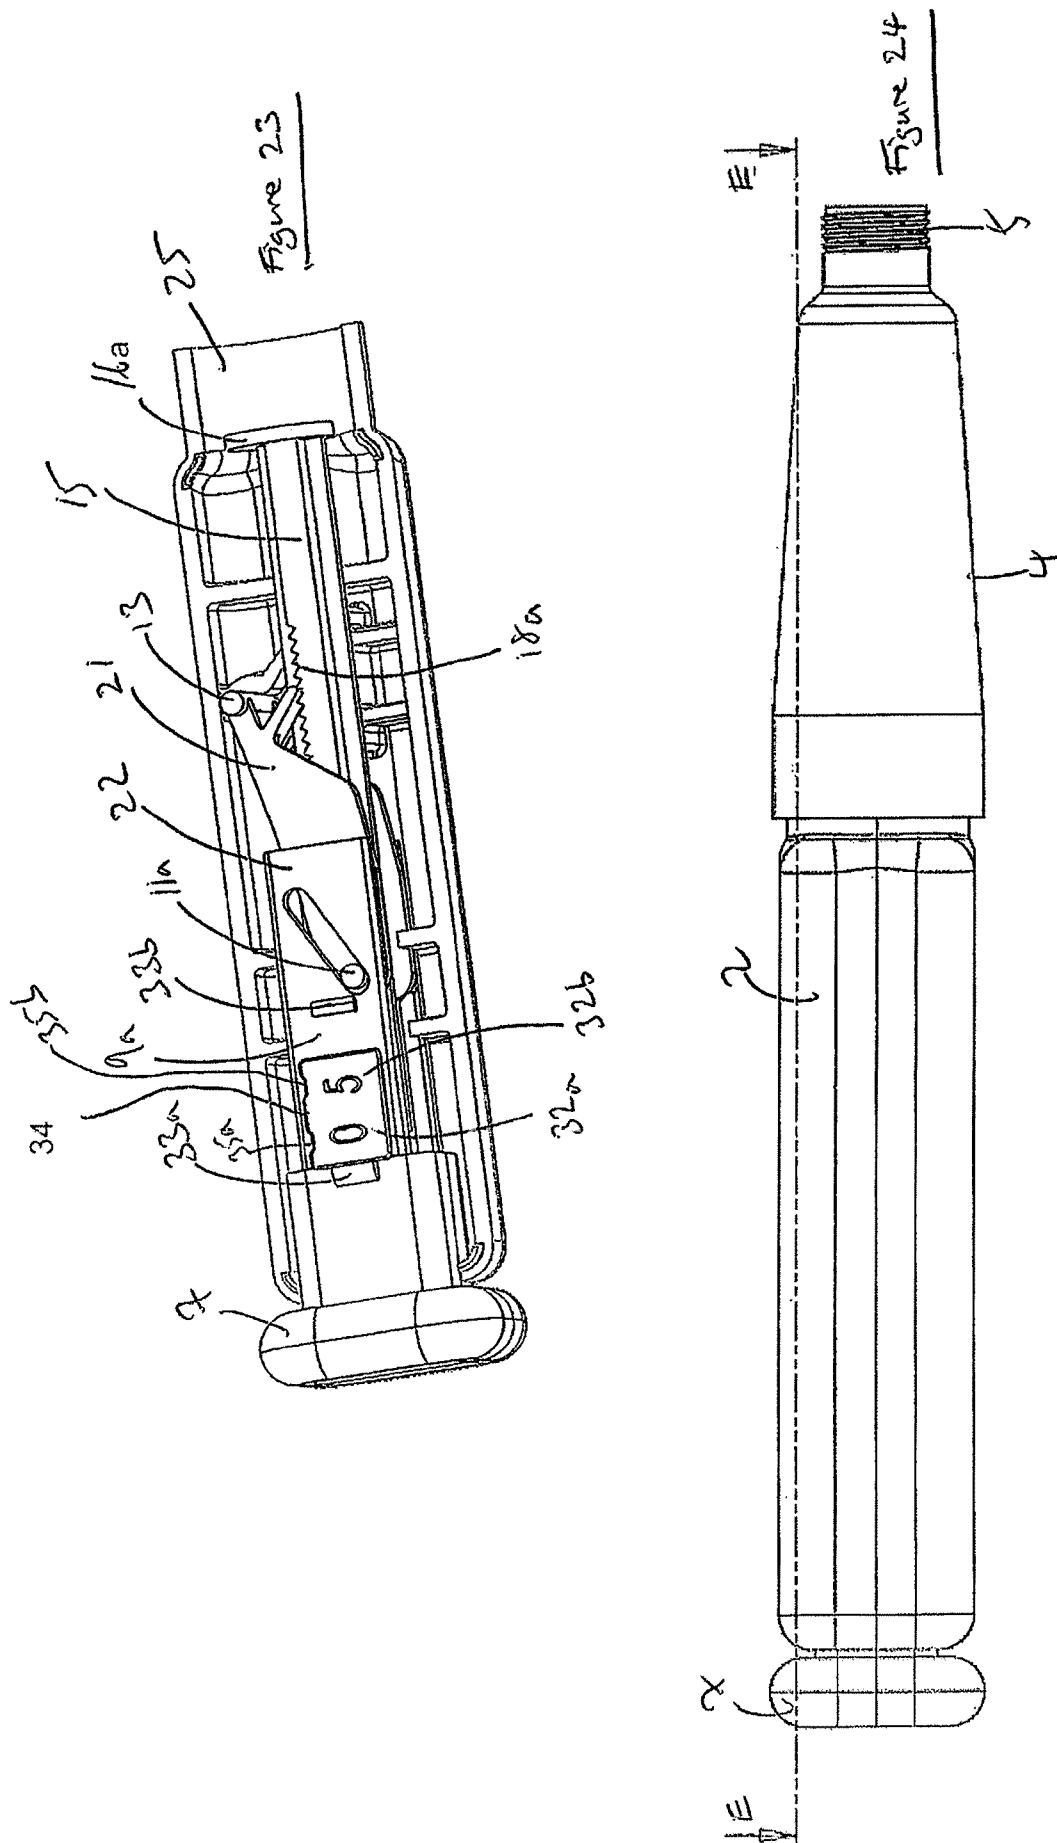

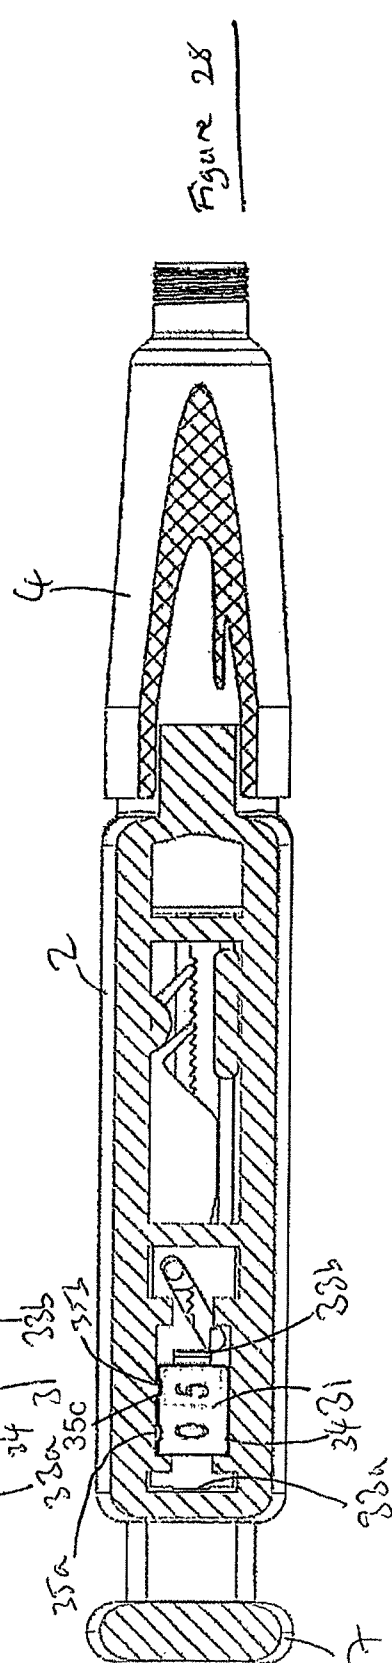
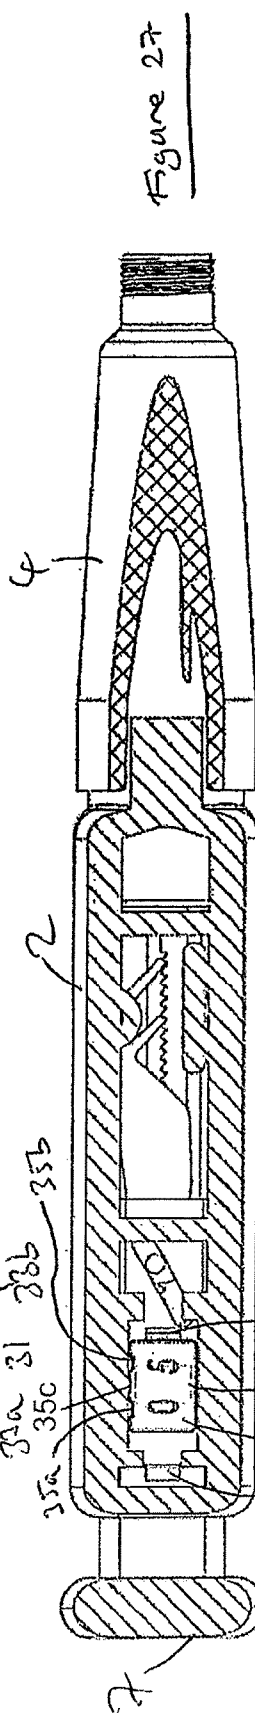
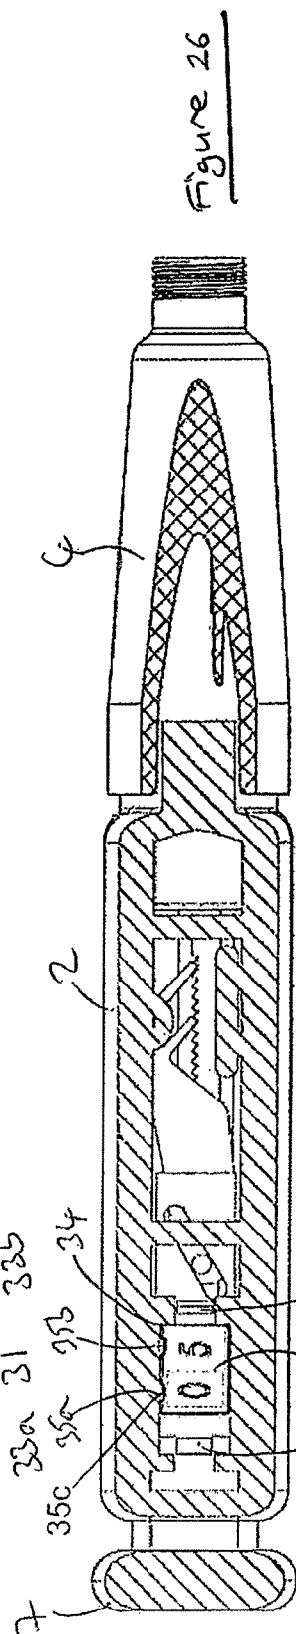
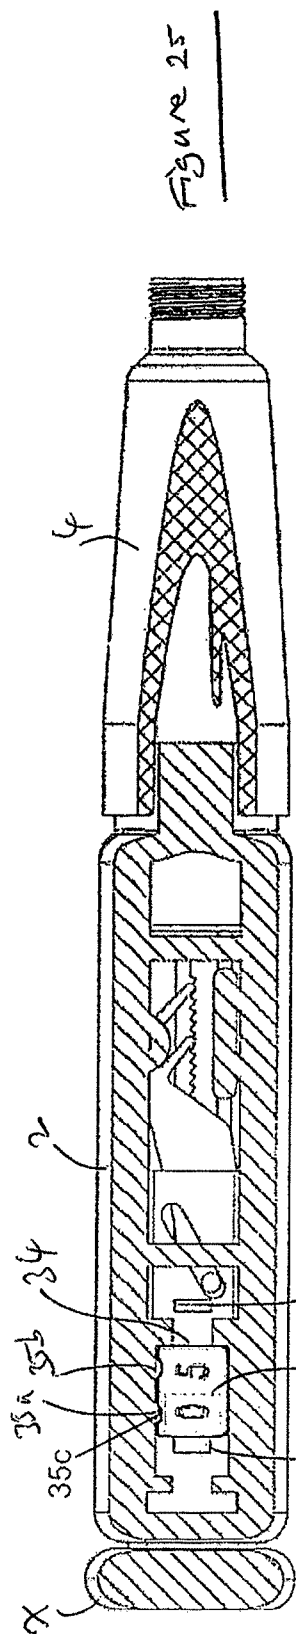


Figure 29

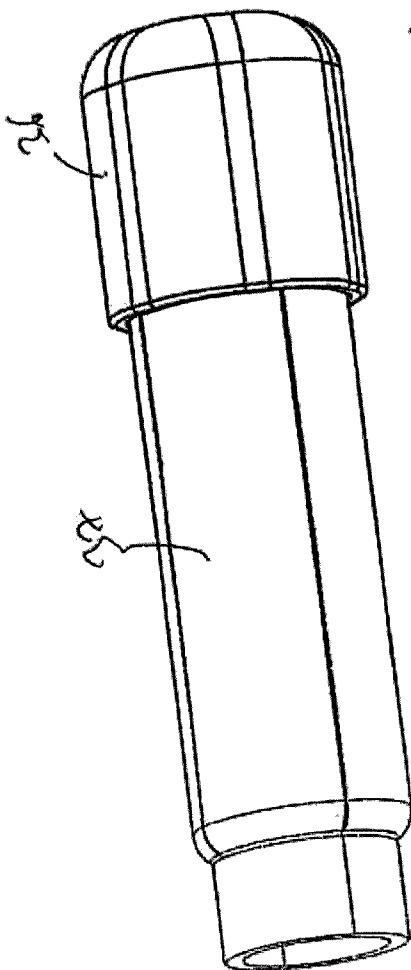


Figure 30










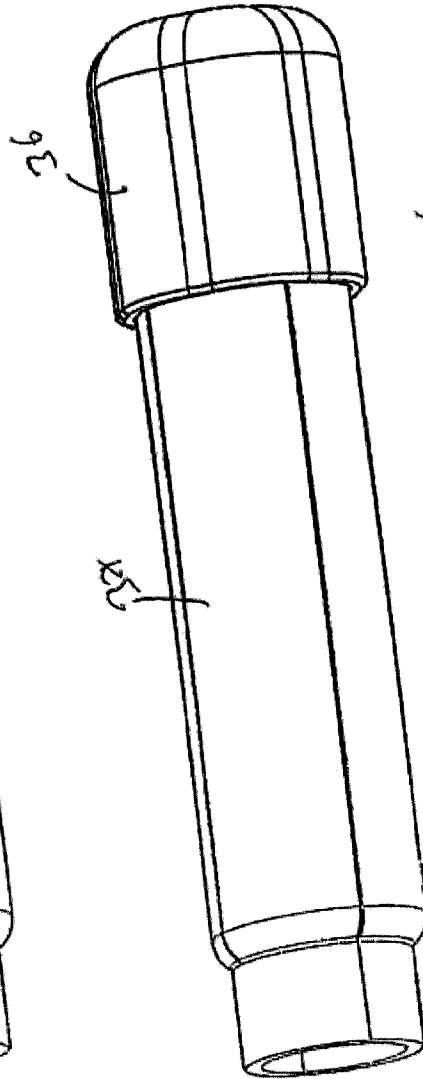



Figure 31

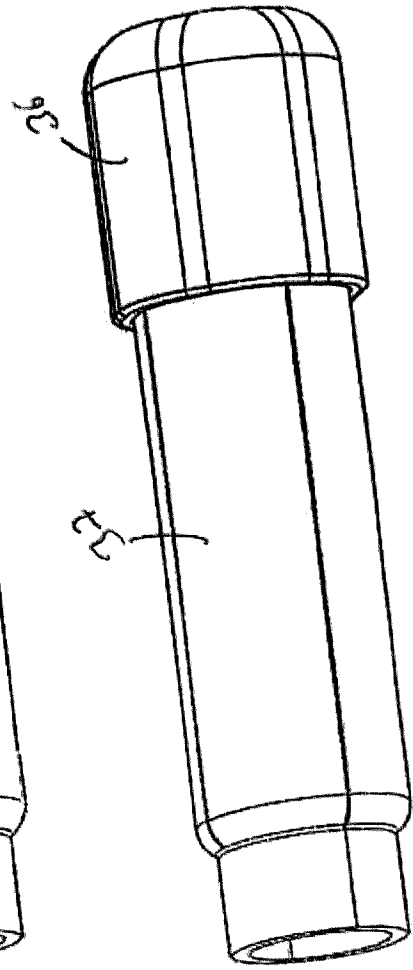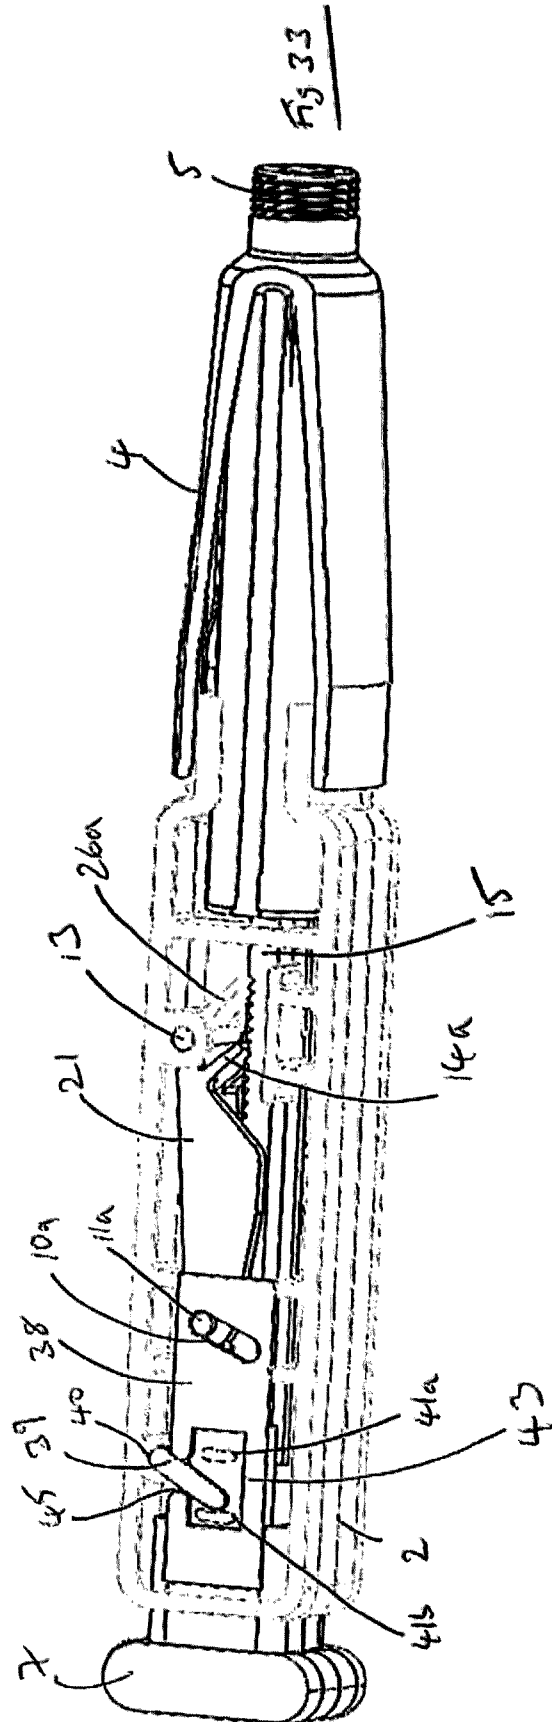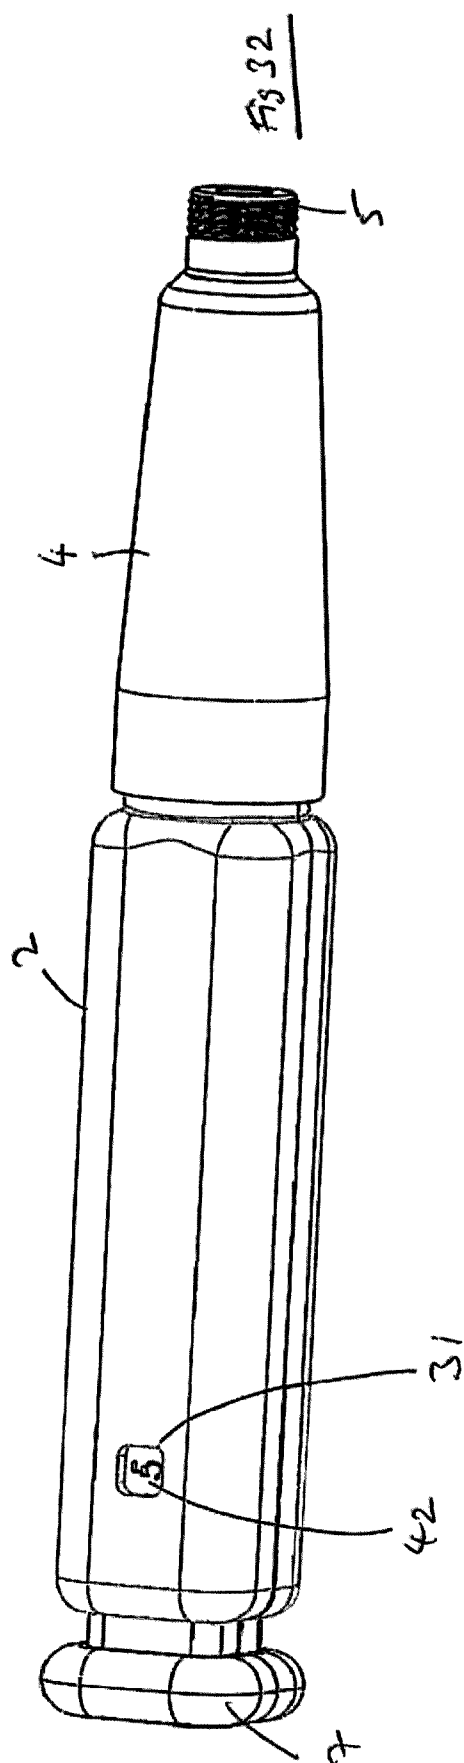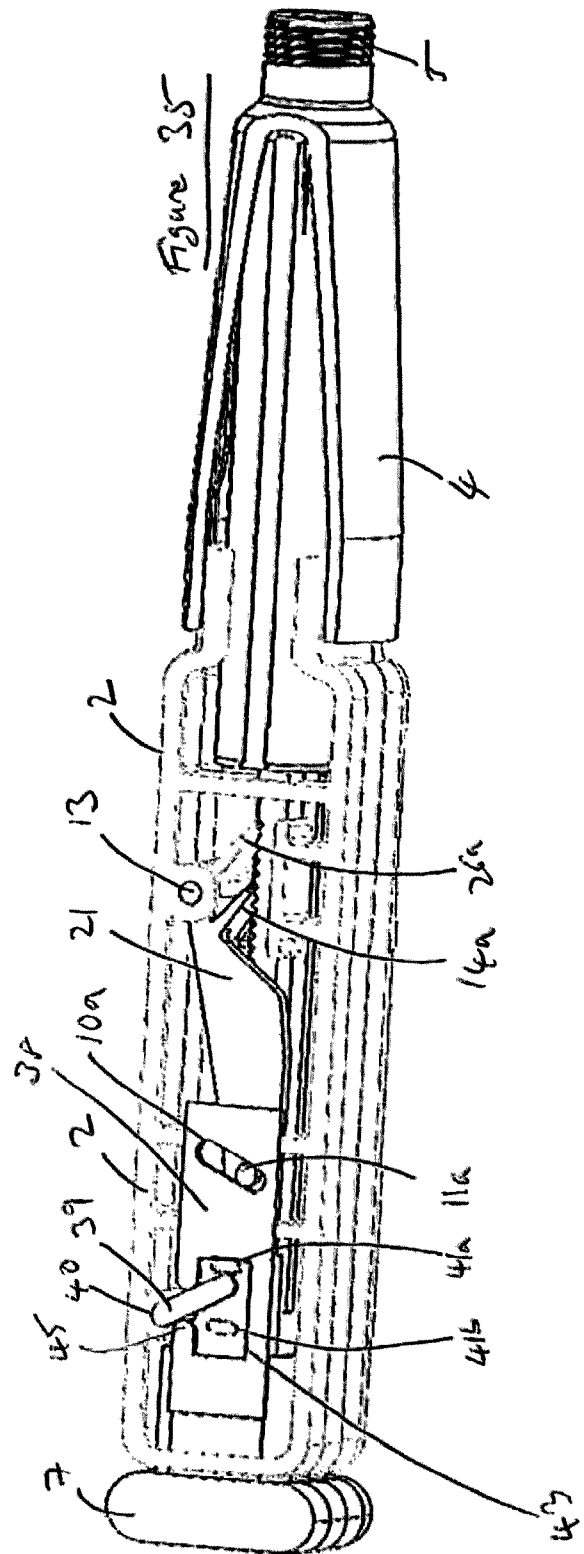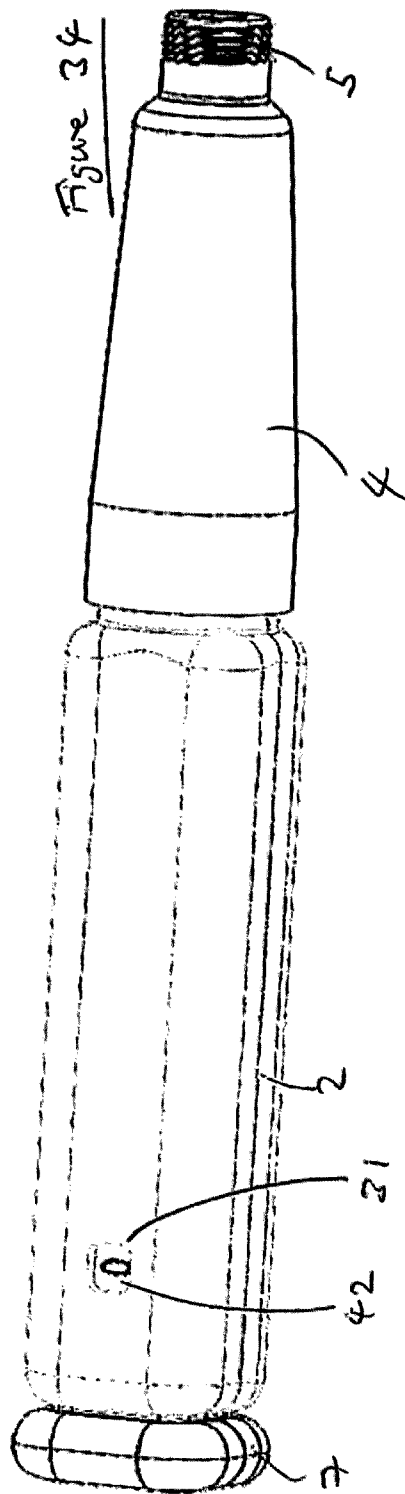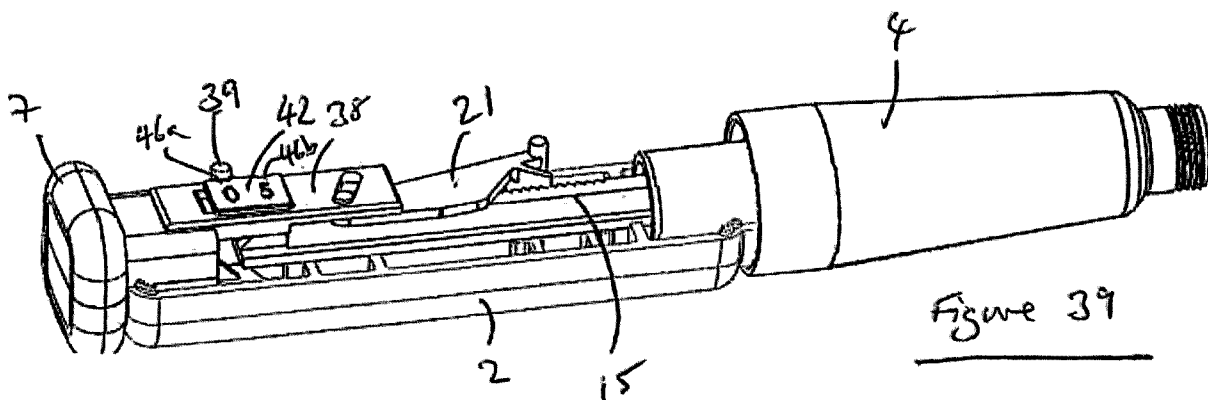

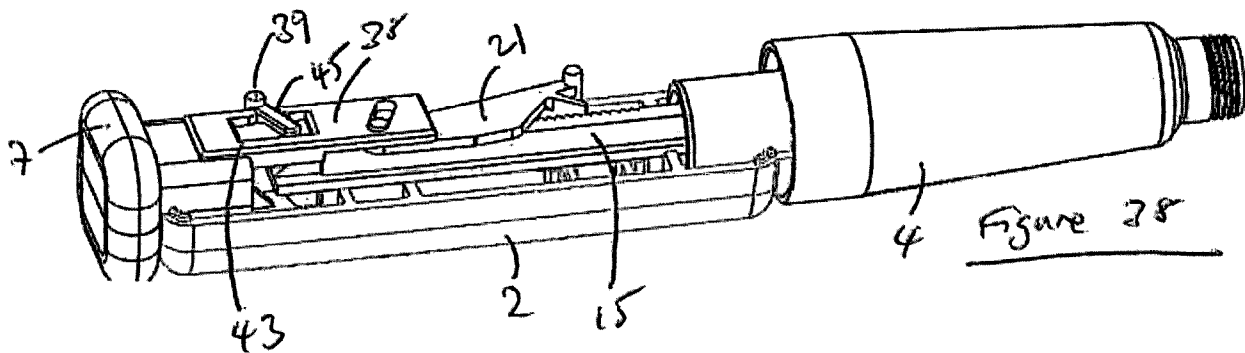

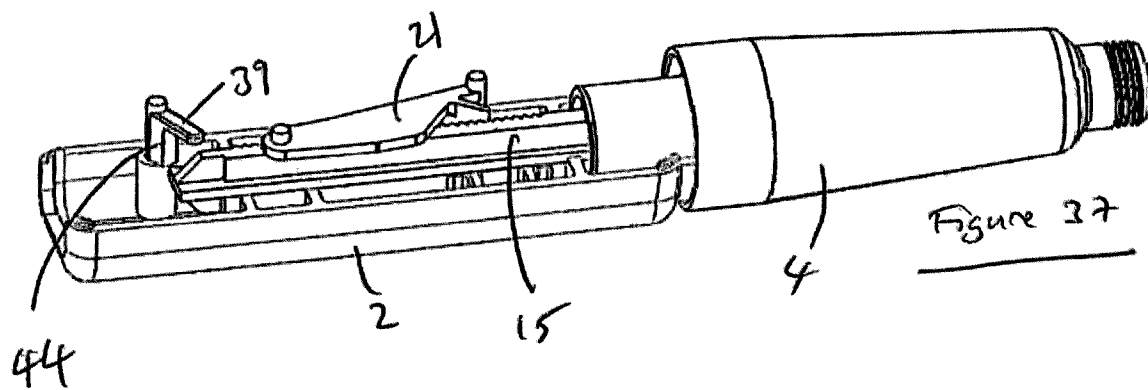

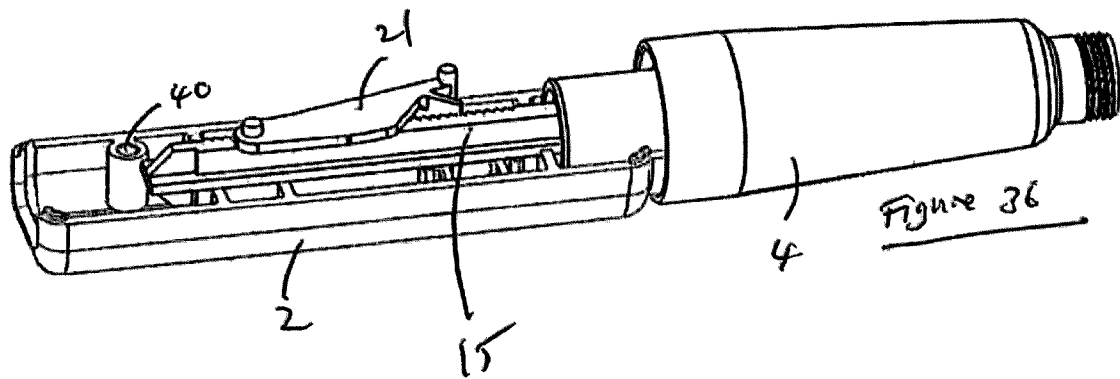

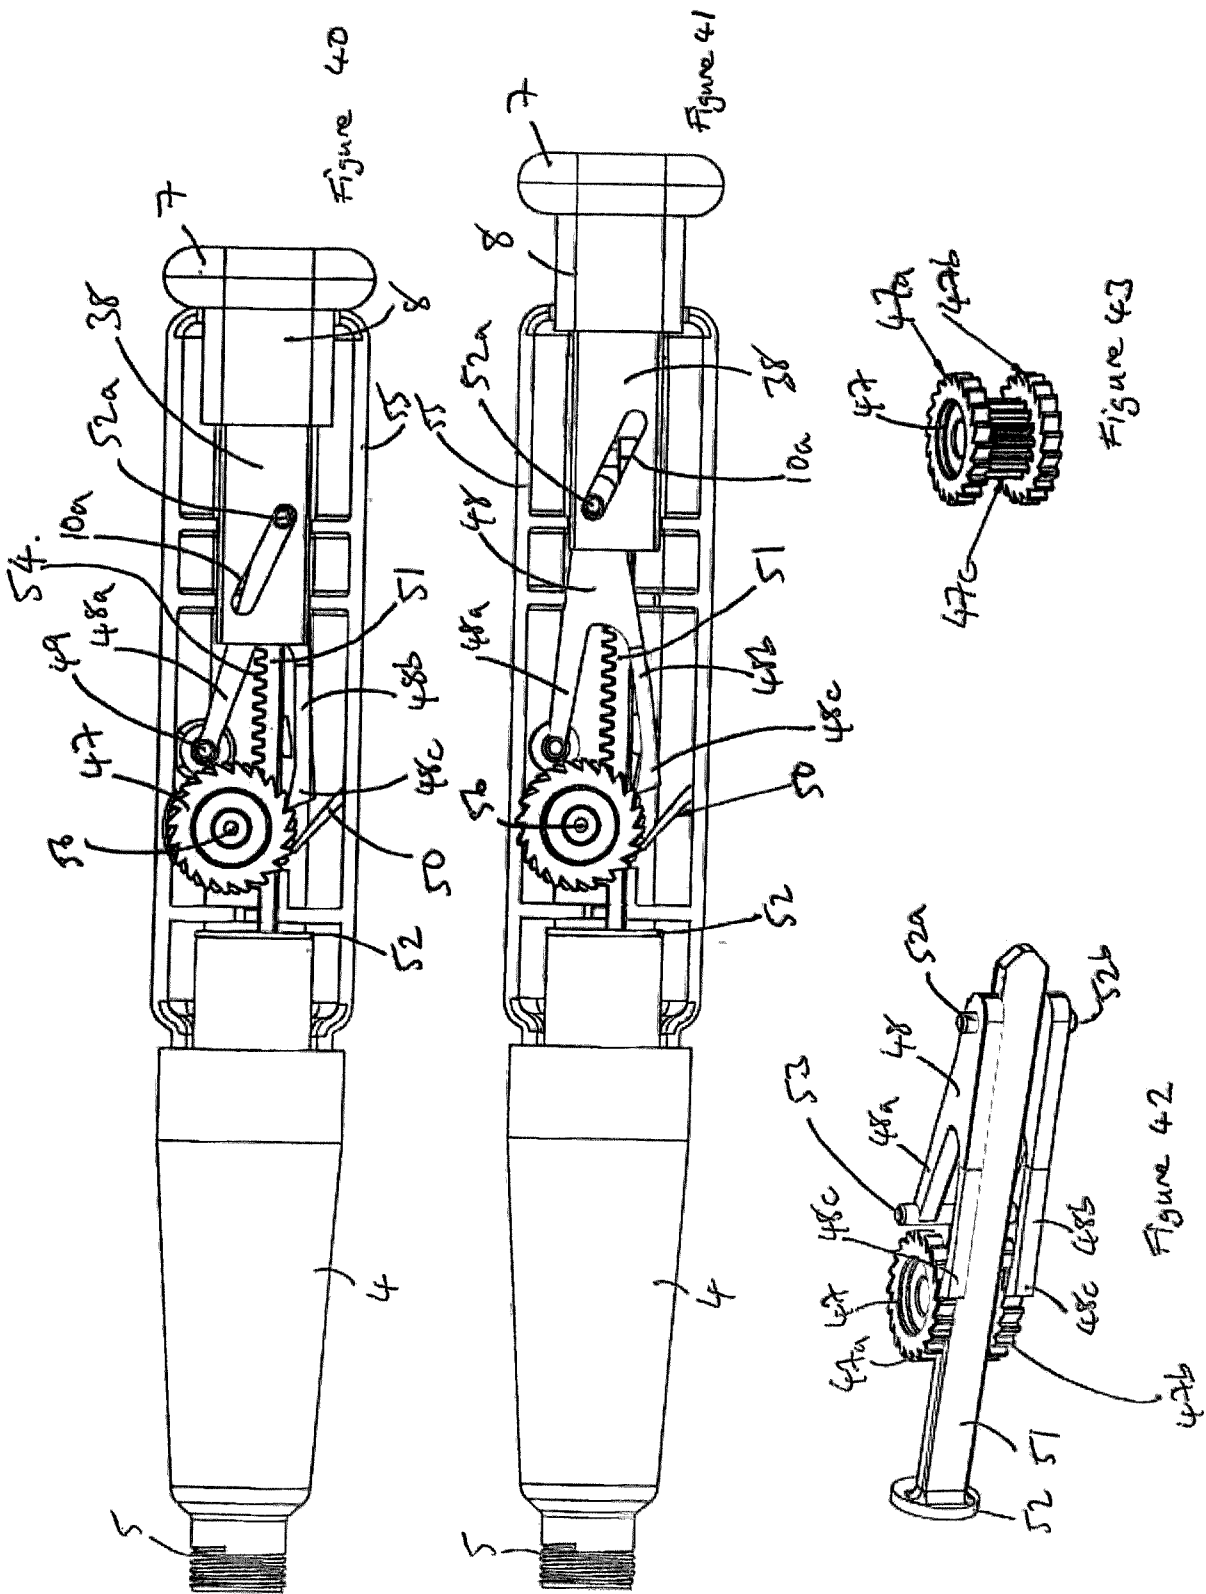

INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2014/055129

A. CLASSIFICATION OF SUBJECT MATTER

INV. A61M5/315 A61M5/24
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 03/057285 A2 (OWEN MUMFORD LTD [GB]; MARSHALL JEREMY [GB]; HOLMAN RURY REGINALD [GB]) 17 July 2003 (2003-07-17) figures 1, 5a-b page 1, lines 16-21 page 6, line 19 - page 7, line 3 -----	1-3,7,8, 15
X	EP 2 123 317 A1 (SANOFI AVENTIS DEUTSCHLAND [DE]) 25 November 2009 (2009-11-25) figures 4, 13, 13a-c paragraphs [0001], [0123] -----	1-8,11, 14,15
X	EP 1 923 083 A1 (SANOFI AVENTIS DEUTSCHLAND [DE]) 21 May 2008 (2008-05-21) figure 1 paragraphs [0001], [0055], [0058], [0059] -----	1,7-10, 12,13,15



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

9 July 2014

Date of mailing of the international search report

18/07/2014

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Herz, Markus

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2014/055129

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 03057285	A2	17-07-2003	EP 1463550 A2 06-10-2004
			EP 1690561 A2 16-08-2006
			JP 4550424 B2 22-09-2010
			JP 2005514120 A 19-05-2005
			US 2005090782 A1 28-04-2005
			WO 03057285 A2 17-07-2003
EP 2123317	A1	25-11-2009	AR 073447 A1 10-11-2010
			AU 2009250106 A1 26-11-2009
			CA 2724763 A1 26-11-2009
			CN 102099073 A 15-06-2011
			EP 2123317 A1 25-11-2009
			EP 2303369 A1 06-04-2011
			JP 5271411 B2 21-08-2013
			JP 2011520537 A 21-07-2011
			KR 20110022607 A 07-03-2011
			NZ 589316 A 29-06-2012
			RU 2010151981 A 27-06-2012
			TW 201010752 A 16-03-2010
			US 2012010575 A1 12-01-2012
			UY 31833 A 05-01-2010
			WO 2009141067 A1 26-11-2009
EP 1923083	A1	21-05-2008	AR 063830 A1 18-02-2009
			AR 063836 A1 25-02-2009
			AU 2007321447 A1 22-05-2008
			AU 2007321449 A1 22-05-2008
			BR PI0719069 A2 03-12-2013
			CA 2669374 A1 22-05-2008
			CA 2669379 A1 22-05-2008
			CL 2007003300 A1 27-06-2008
			CL 2007003301 A1 27-06-2008
			CN 101610804 A 23-12-2009
			CN 101622023 A 06-01-2010
			CO 6210736 A2 20-10-2010
			CO 6210737 A2 20-10-2010
			CR 10769 A 25-05-2009
			CR 10770 A 23-07-2009
			DK 2091599 T3 25-03-2013
			EC SP099333 A 30-06-2009
			EC SP099334 A 30-06-2009
			EG 25189 A 17-10-2011
			EP 1923083 A1 21-05-2008
			EP 2081622 A1 29-07-2009
			EP 2091599 A1 26-08-2009
			EP 2392372 A2 07-12-2011
			ES 2401354 T3 18-04-2013
			GT 200900131 A 25-05-2011
			GT 200900132 A 08-08-2011
			HK 1140154 A1 30-08-2013
			HK 1140436 A1 10-01-2014
			HN 2009000998 A 12-10-2011
			HN 2009001000 A 21-09-2012
			IL 198747 A 31-12-2012
			IL 198750 A 31-10-2012
			JP 5286275 B2 11-09-2013
			JP 5427607 B2 26-02-2014
			JP 2010509958 A 02-04-2010

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/EP2014/055129

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		JP 2010522577 A	08-07-2010
		KR 20090080560 A	24-07-2009
		KR 20090082489 A	30-07-2009
		MA 30884 B1	02-11-2009
		MA 30885 B1	02-11-2009
		ME 00589 A	20-12-2011
		MY 148971 A	28-06-2013
		MY 149575 A	13-09-2013
		NZ 576964 A	27-05-2011
		NZ 577007 A	27-05-2011
		PE 12032008 A1	24-09-2008
		PE 12042008 A1	29-09-2008
		PT 2091599 E	05-03-2013
		RU 2009122952 A	27-12-2010
		RU 2009123008 A	27-12-2010
		SI 2091599 T1	30-04-2013
		SV 2009003263 A	27-10-2009
		SV 2009003264 A	27-10-2009
		TW 200833383 A	16-08-2008
		TW 200833387 A	16-08-2008
		UA 96167 C2	10-10-2011
		US 2010094206 A1	15-04-2010
		US 2010094207 A1	15-04-2010
		US 2012172816 A1	05-07-2012
		US 2012289929 A1	15-11-2012
		UY 30721 A1	03-07-2008
		UY 30722 A1	03-07-2008
		WO 2008058666 A1	22-05-2008
		WO 2008058668 A1	22-05-2008
		ZA 200903077 A	28-04-2010
		ZA 200903129 A	31-03-2010
