



US00D979080S

(12) **United States Design Patent** (10) **Patent No.:** **US D979,080 S**
Jalinous (45) **Date of Patent:** **** Feb. 21, 2023**

(54) **MRI TOWER COIL STAND**
(71) Applicant: **Reza Jalinous**, Winchester, MA (US)
(72) Inventor: **Reza Jalinous**, Winchester, MA (US)
(**) Term: **15 Years**
(21) Appl. No.: **29/696,437**

D788,310 S * 5/2017 Takeuchi D24/158
D804,031 S * 11/2017 Hsu D24/158
10,542,890 B2 * 1/2020 Yang A61B 5/055
D880,700 S * 4/2020 Sun D24/158
D890,927 S * 7/2020 Chong D24/158
2018/0263547 A1 * 9/2018 Settles A61B 5/055
2020/0081081 A1 * 3/2020 Yang A61B 5/055
2021/0072330 A1 * 3/2021 Berendt, Jr. G01R 33/341
2021/0077828 A1 * 3/2021 Wang A61N 5/1077

(22) Filed: **Jun. 27, 2019**
(51) **LOC (14) Cl.** **24-01**
(52) **U.S. Cl.**
USPC **D24/200; D24/184**
(58) **Field of Classification Search**
USPC D24/158-159, 184-186, 200
CPC A61B 5/055; A61B 6/03; G01R 33/34007;
G01R 33/341; G01R 33/34084; G01R
33/34; G01R 33/64; G01R 33/3657;
G01R 33/365
See application file for complete search history.

OTHER PUBLICATIONS

MRI Tower Cil Stand. Jaltron-llc-coils. Retrieved on Apr. 6, 2021.
Retrieved from the Internet: <https://www.jaltron-coils.com/mri-tower-coil-stand>.*

* cited by examiner

Primary Examiner — Wan Laymon
(74) *Attorney, Agent, or Firm* — David J. Connaughton, Jr.; Justin Tringer; Lambert Shortell & Connaughton

(57) **CLAIM**

The ornamental design for a MRI tower coil stand, as shown and described.

(56) **References Cited**


U.S. PATENT DOCUMENTS

D112,023 S 11/1938 Martinsson
4,634,980 A * 1/1987 Mistic G01R 33/34007
324/318
D318,330 S 7/1991 Doty
D357,069 S 4/1995 Plahn
D407,820 S * 4/1999 Sullenberger D24/184
D571,920 S 6/2008 Juliana
D607,712 S 1/2010 Kelleghan
D667,118 S * 9/2012 Wodecki D24/159
D689,612 S * 9/2013 Braswell, Jr. D24/158
D699,359 S 2/2014 Lindekugel
D742,535 S 11/2015 Wu
9,456,764 B2 * 10/2016 Burke A61B 5/055
D770,635 S 11/2016 Cole
D770,992 S 11/2016 Tauchi
D776,822 S 1/2017 McKinley

DESCRIPTION

FIG. 1 is an isometric view of the front of the MRI tower coil stand, which embodies my design;
FIG. 2 is a side view thereof;
FIG. 3 is a side view thereof;
FIG. 4 is a side view thereof;
FIG. 5 is a side view thereof;
FIG. 6 is a top plan view thereof; and,
FIG. 7 is a bottom plan view thereof.
The broken line in the drawings is included for the purpose of illustrating portions of the MRI tower coil stands and forms no part of the claimed design.

1 Claim, 7 Drawing Sheets

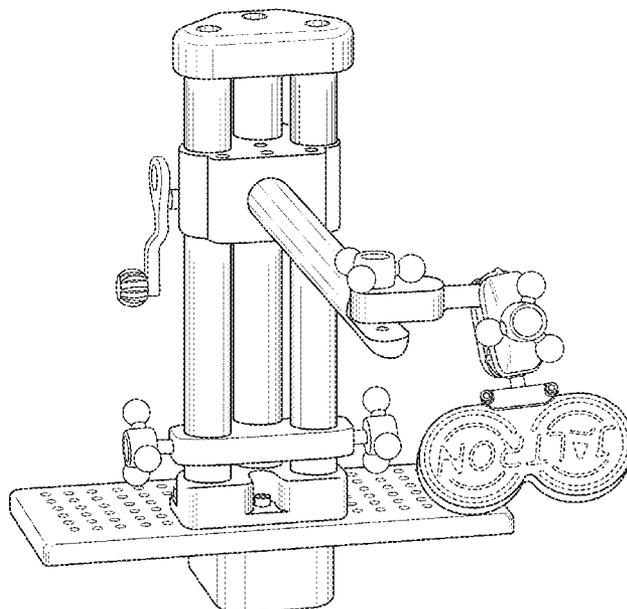

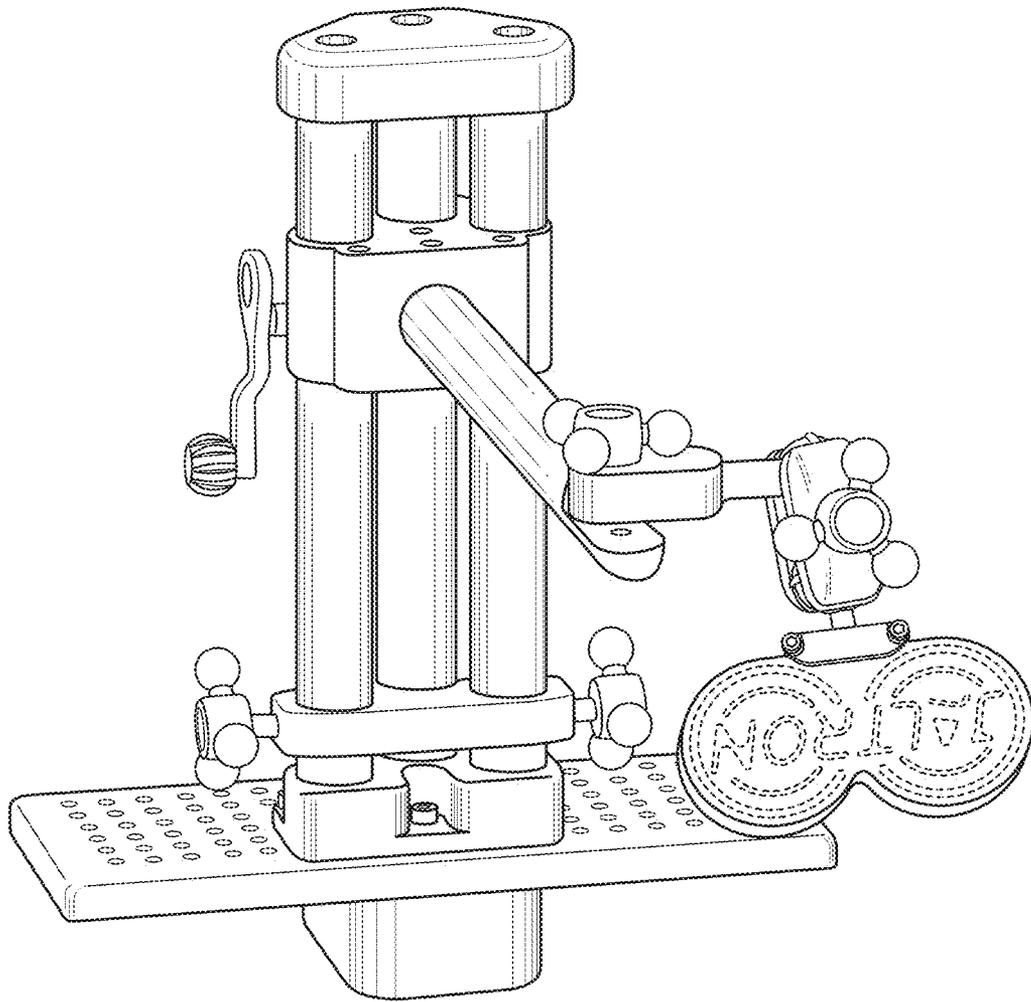


Fig. 1

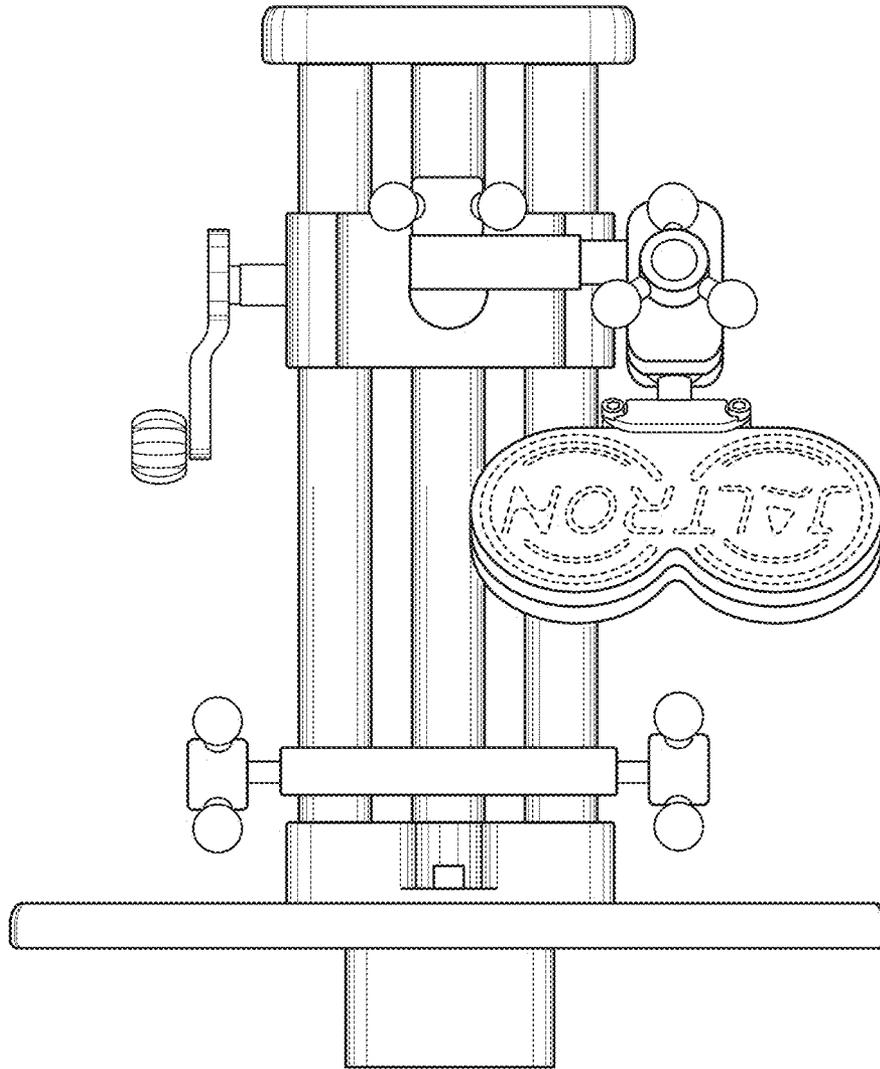


Fig. 2

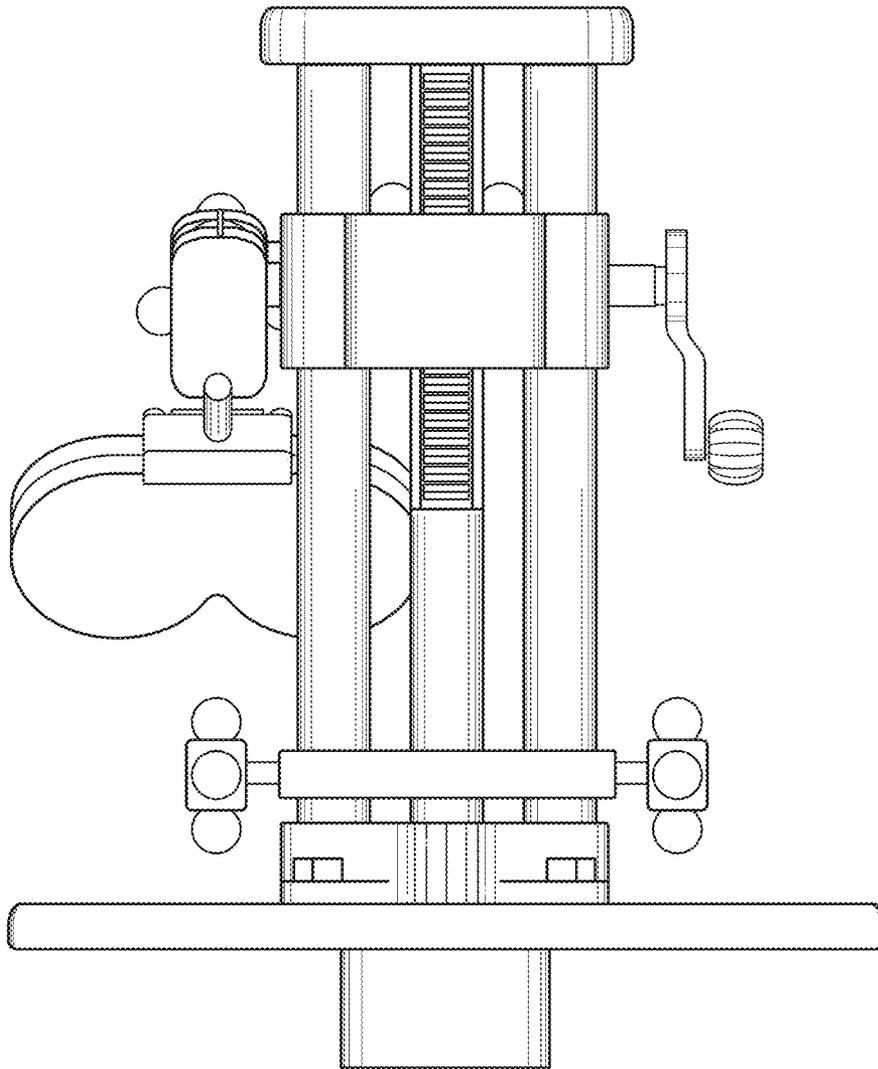


Fig. 3

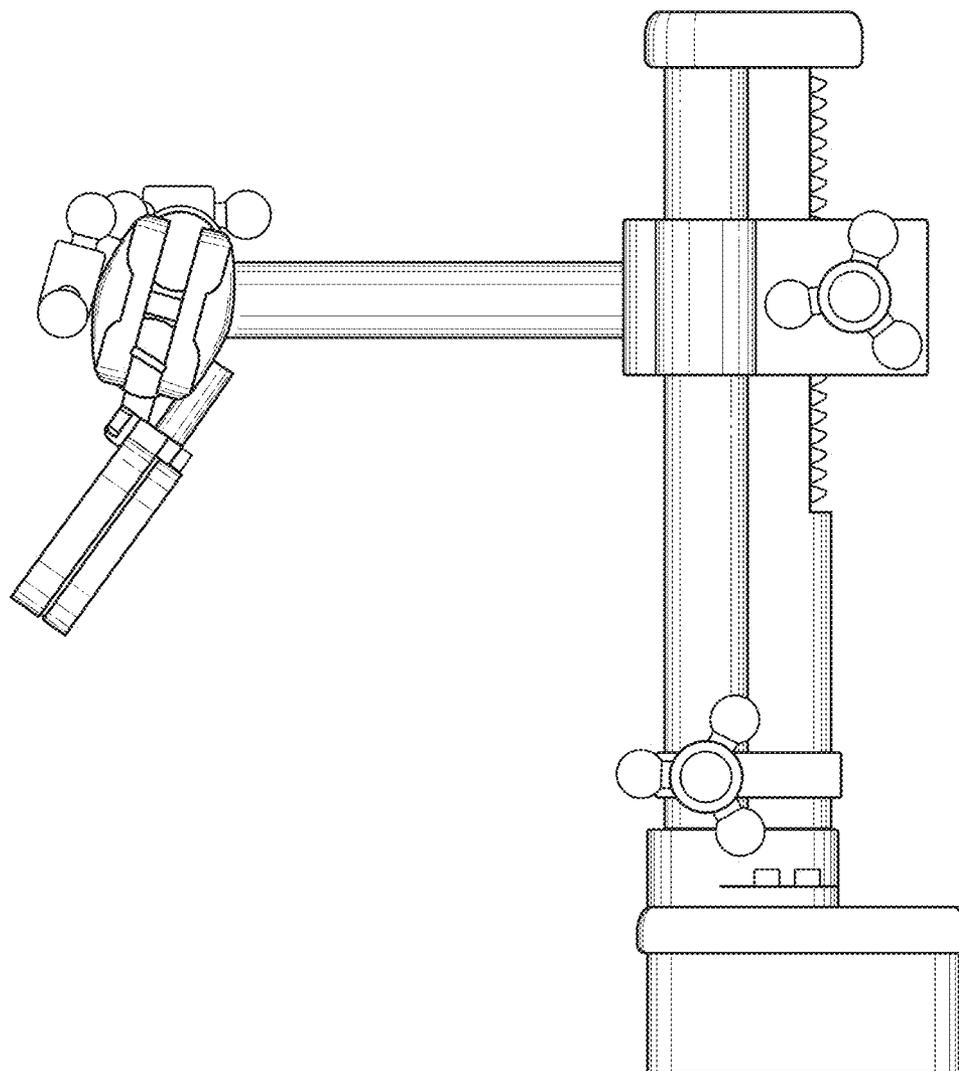


Fig. 4

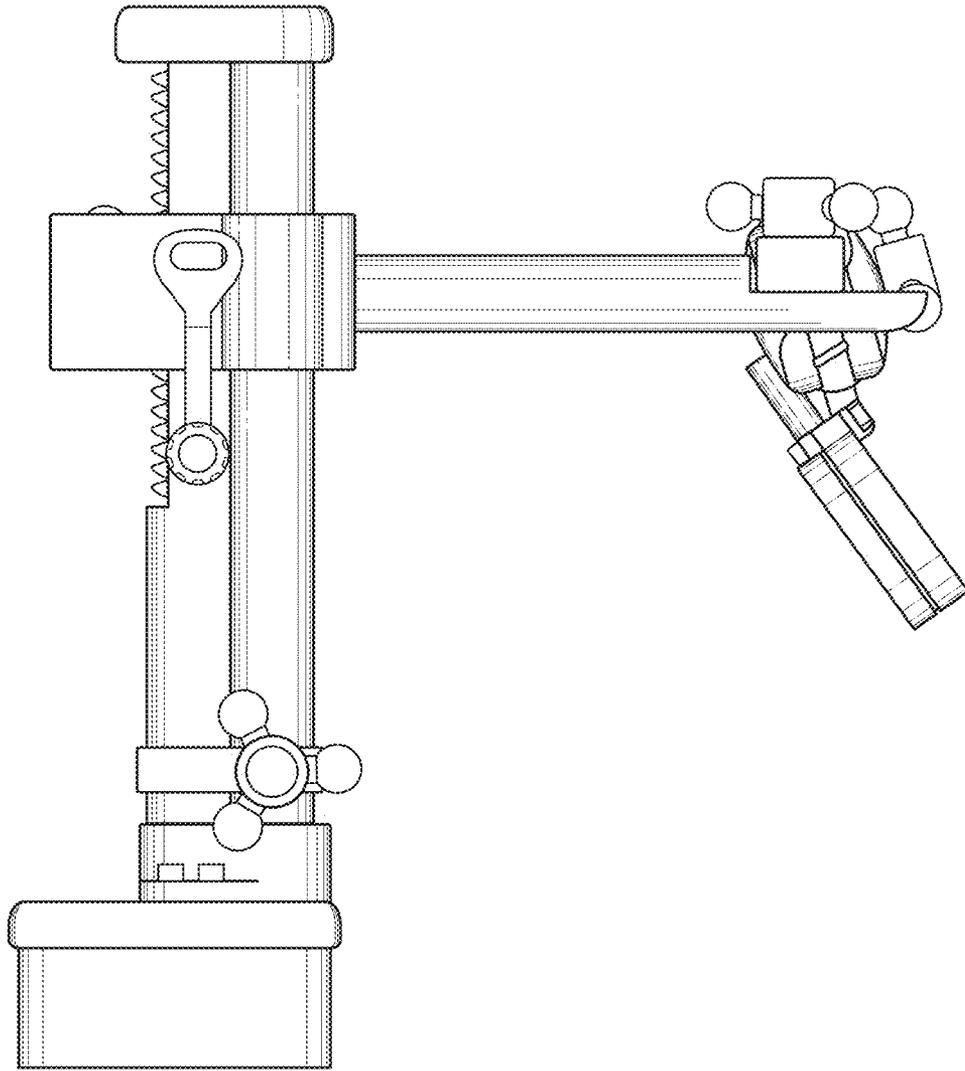


Fig. 5

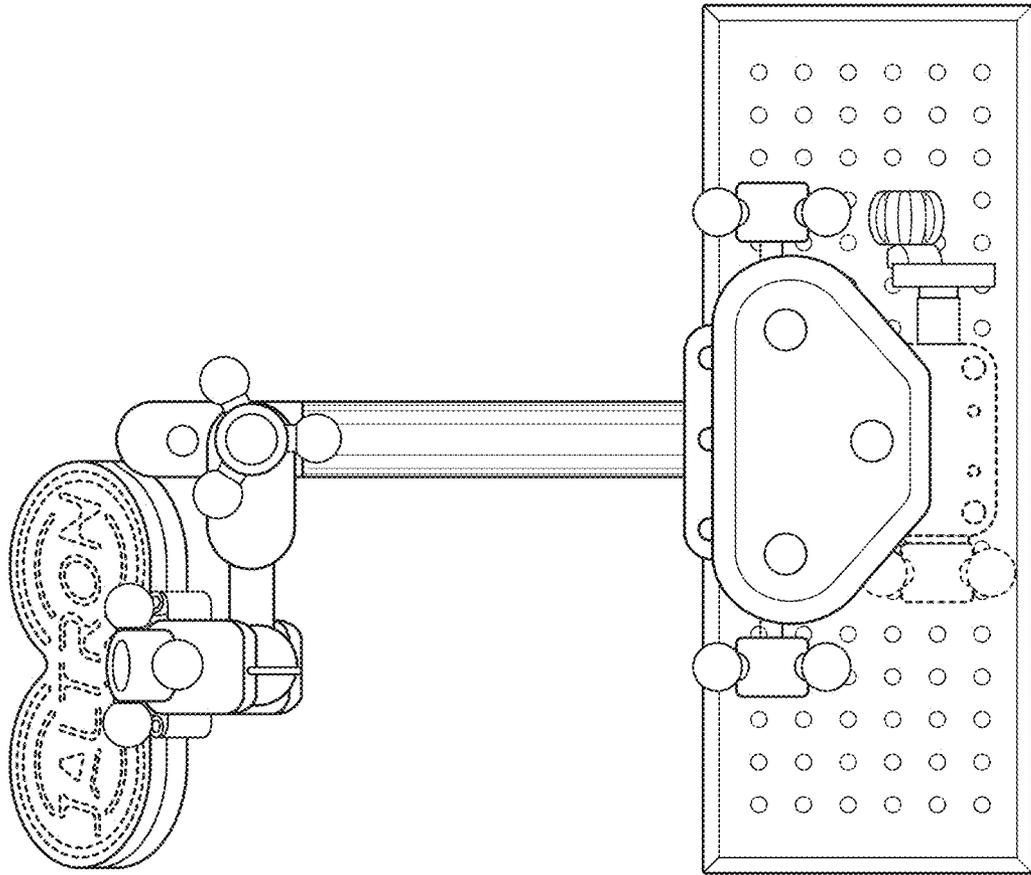


Fig. 6

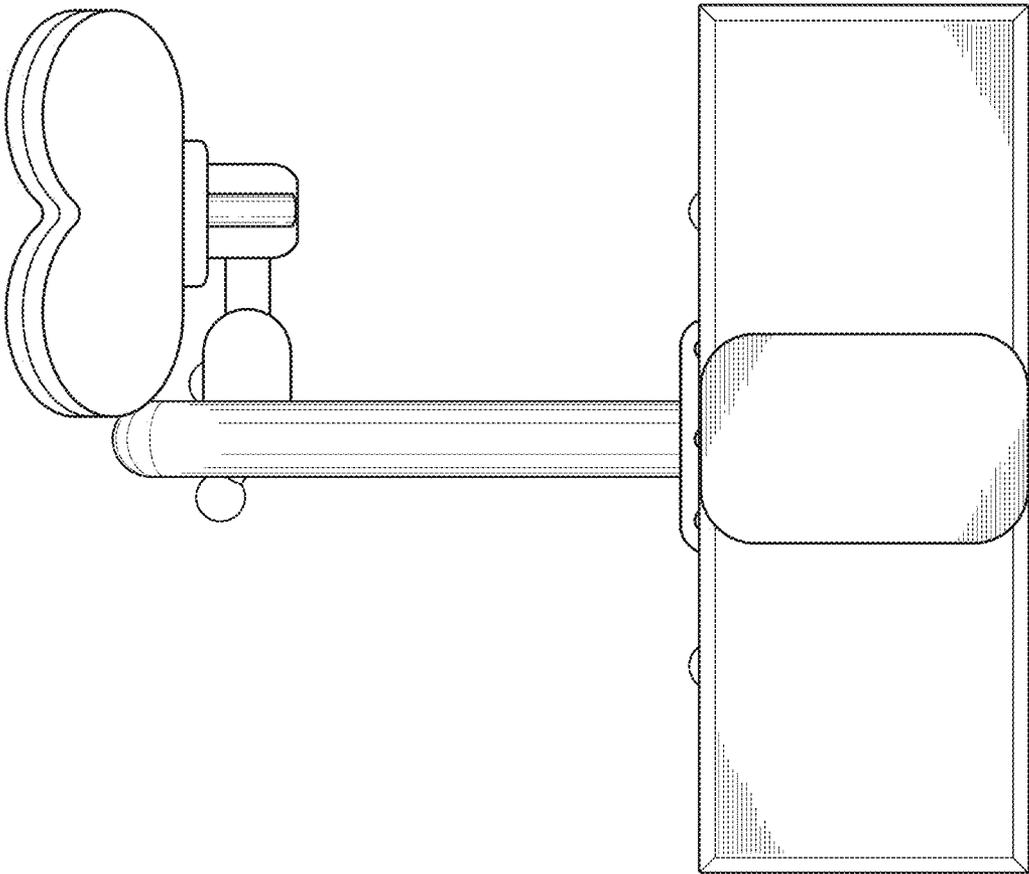


Fig. 7