



(22) Date de dépôt/Filing Date: 2006/11/01
 (41) Mise à la disp. pub./Open to Public Insp.: 2007/05/17
 (45) Date de délivrance/Issue Date: 2010/04/13
 (30) Priorité/Priority: 2005/11/17 (US11/281,751)


(51) Cl.Int./Int.Cl. *A61B 19/00* (2006.01),
A61F 9/007 (2006.01), *A61M 1/00* (2006.01)

(72) Inventeurs/Inventors:
 ARTSYUKHOVICH, ALEXANDER N., US;
 BOUKHNY, MIKHAIL, US;
 GORDON, RAPHAEL, US;
 SORENSEN, GARY P., US;
 THOE, DAVID, US;
 SVETIC, RALPH E., US;
 YADLOWSKY, MICHAEL, US

(73) Propriétaire/Owner:
 ALCON, INC., CH

(74) Agent: KIRBY EADES GALE BAKER

(54) Titre : CASSETTE DE DONNEES CHIRURGICALES
 (54) Title: SURGICAL CASSETTE

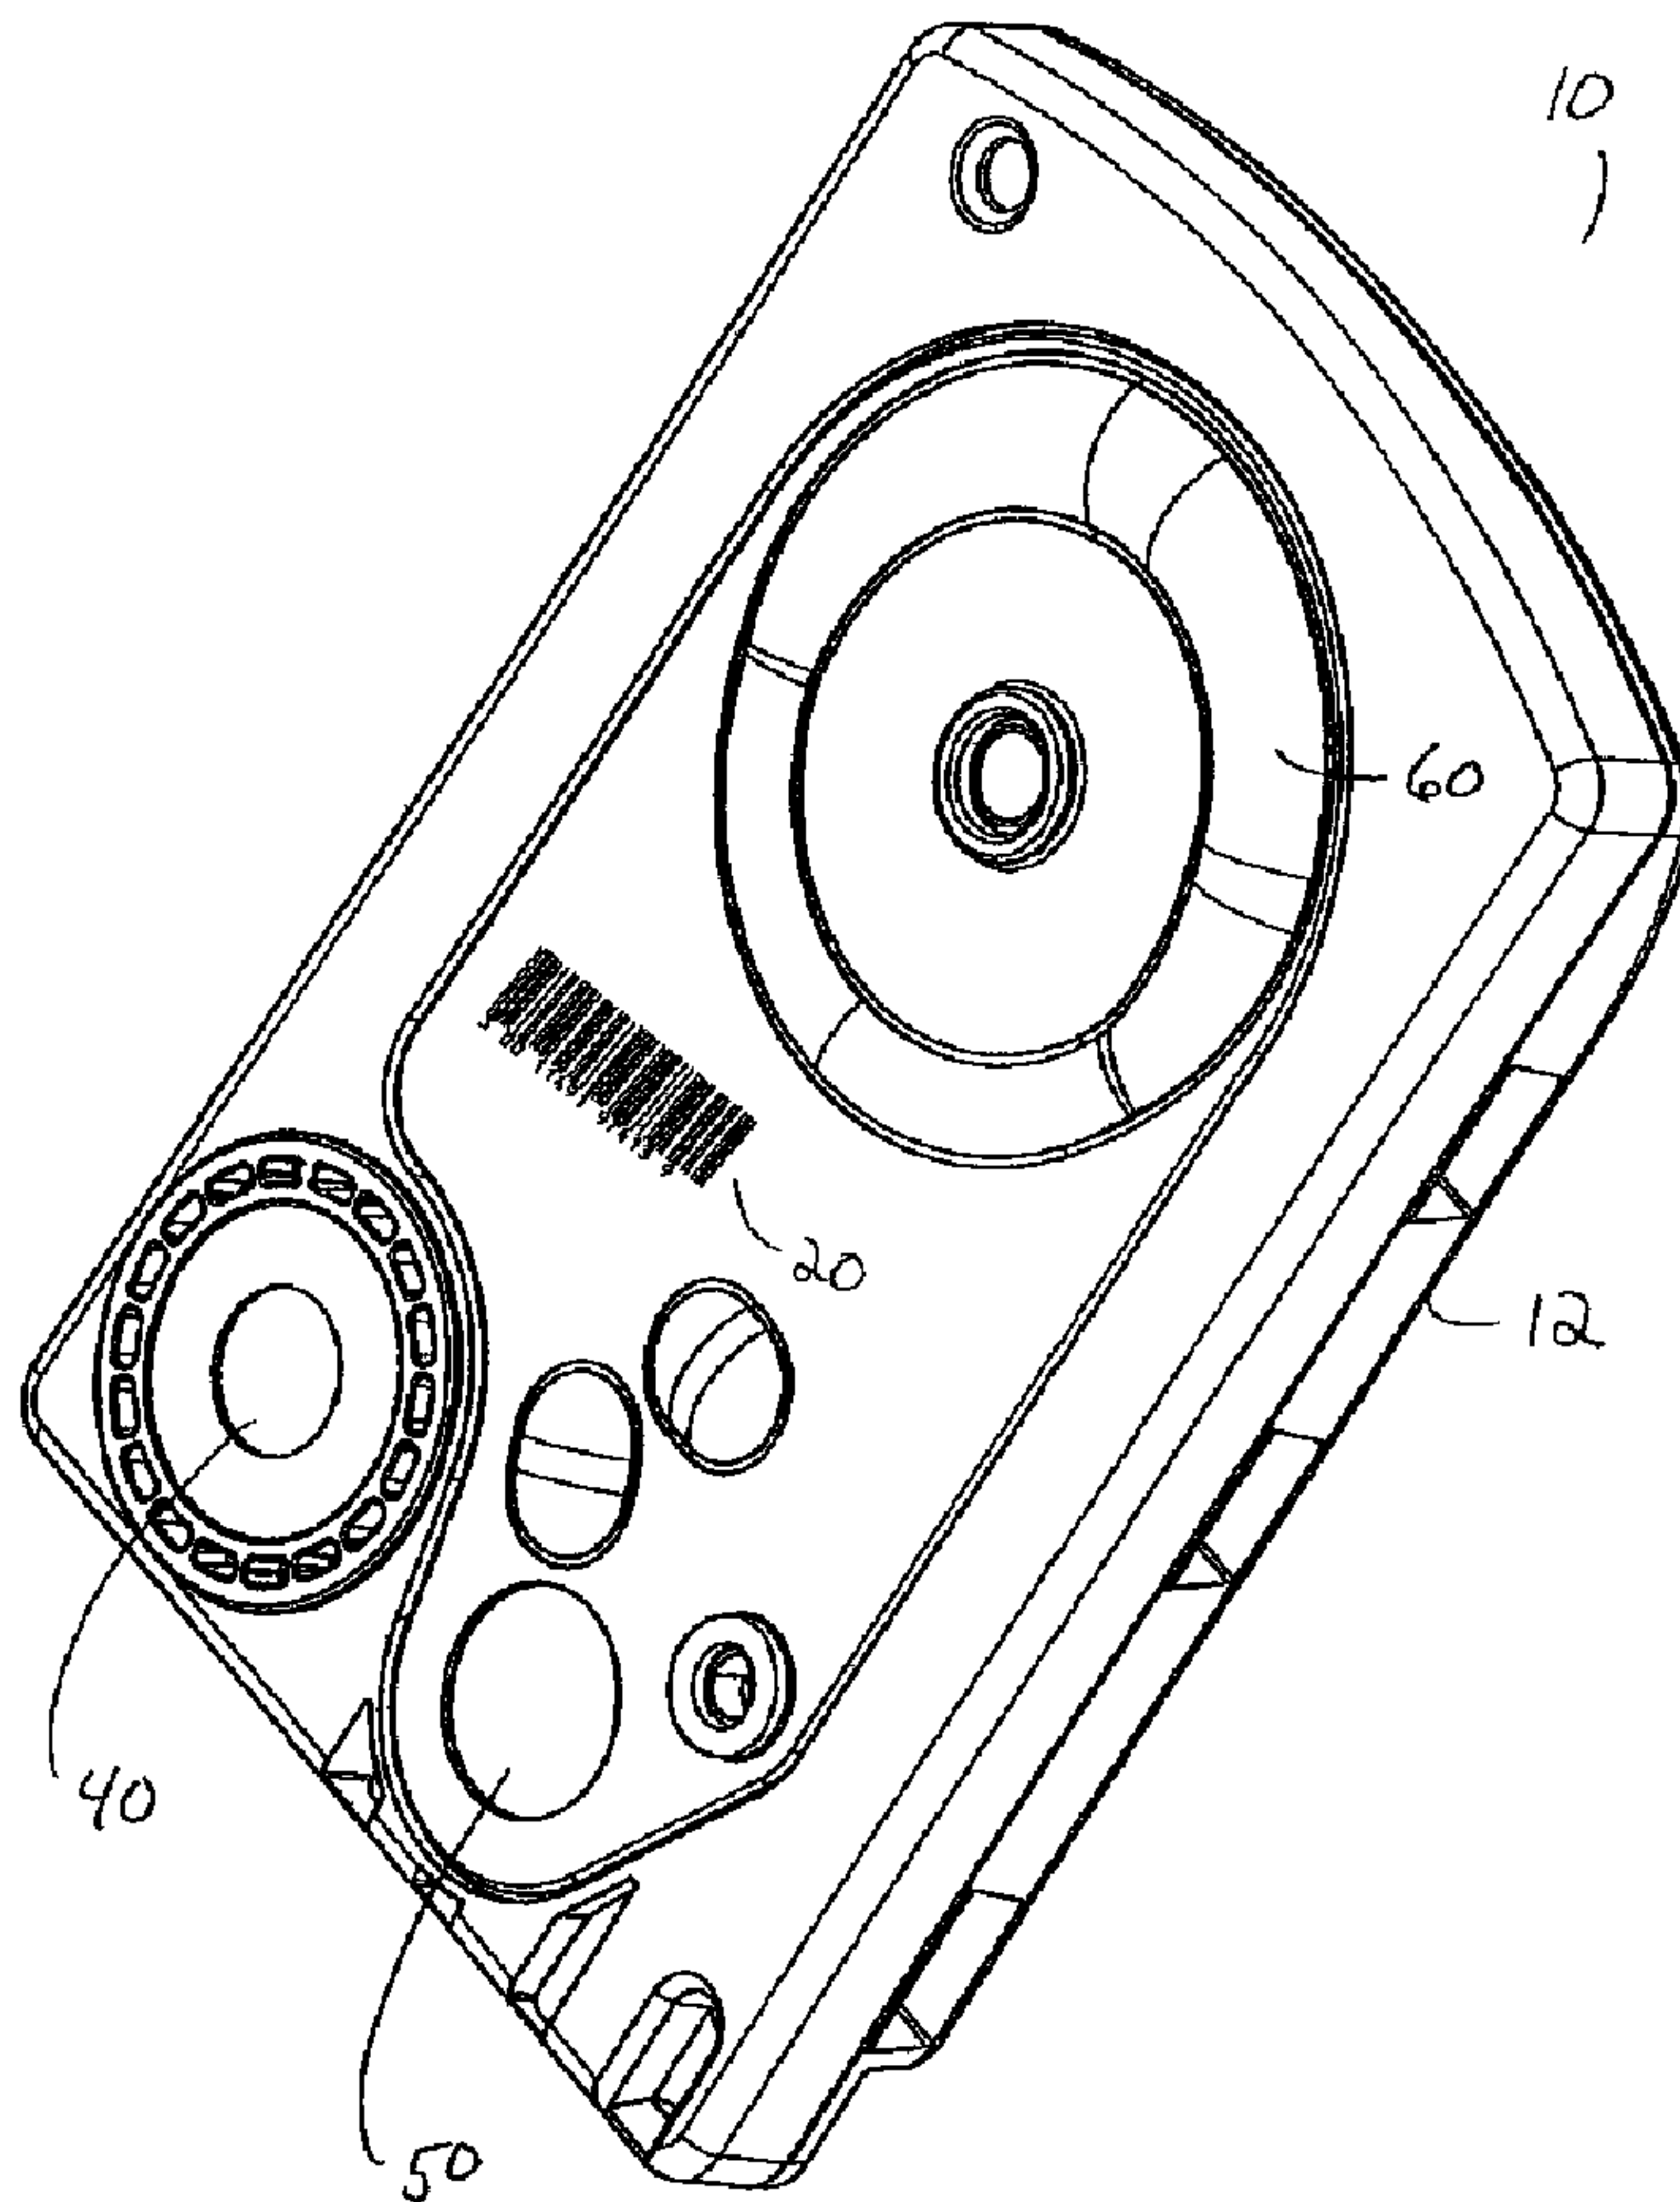

(57) Abrégé/Abstract:

A surgical system and cassette, the cassette having an identification method that is specific to the cassette. Suitable methods include bar coding or Radio Frequency Identification ("RFID"). Cassette information that may be encoded include features such as

(57) Abrégé(suite)/Abstract(continued):

lot number and performance characteristics, such as pressure sensor calibration data, flow and pressure data and any other performance characteristics of the cassette captured during testing of the cassette at manufacture.

Abstract of the Disclosure

A surgical system and cassette, the cassette having an identification method that is specific to the cassette. Suitable methods include bar coding or Radio Frequency Identification ("RFID"). Cassette information that may be encoded include features such as lot number and performance characteristics, such as pressure sensor calibration data, flow and pressure data and any other performance characteristics of the cassette captured during testing of the cassette at manufacture.

SURGICAL CASSETTE

Background of the Invention

5

This invention relates generally to the field of surgical cassettes and more particularly to an identification system for surgical cassettes.

The use of cassettes with surgical instruments to help manage irrigation and aspiration flows into and out of a surgical site is well-known. See, for example, U.S. Patent Nos. 10 4,493,695, 4,627,833 (Cook), 4,395,258 (Wang, et al.), 4,713,051 (Steppe, et al.), 4,798,850 (DeMeo, et al.), 4,758,238, 4,790,816 (Sundblom, et al.), 5,267,956, 5,364,342 (Beuchat), 6,036,458 (Cole, et al.) and 6,059,544 (Jung et al.).

The fluidic performance of the surgical instrument is substantially affected by the 15 fluidic performance of the cassette. As a result, current surgical instrumentation and cassettes are designed to work as an integral system, with the fluidic performance of the cassette designed to optimize the fluidic performance of the entire surgical system. Recent advances made in surgical instrumentation now allow the surgeon to manually or automatically control the operating parameters of the surgical instrumentation to a very fine degree. Specialized 20 cassettes have been developed to allow the surgeon to capitalize on the advance control afforded by modern surgical instrumentation. The operating parameters of the surgical instrumentation, however, must be adjusted depending upon the cassette being used. One system, disclosed in U.S. Patent No. 6,059,544 (Jung, et al.), has a cassette with a series of frangible tabs that can be used to allow the instrument to recognize the type of cassette being 25 used. While such a system works very well, and has been commercially successful, the cassette identification system disclosed in this reference identifies only the type of cassette installed in the surgical console, and does not provide any information as to the performance characteristics of the specific cassette. Other ophthalmic surgical instruments contain embedded memory chips or other ID methods that allow the surgical console to recognize the 30 instrument and adjust the console automatically to appropriate operating parameters. None of these systems; however, is capable of recognizing a specific cassette or instrument and adjusting the surgical console for the unique performance characteristics of a specific cassette or instrument.

Accordingly, a need exists for a cassette identification system that identifies the performance parameters for each specific cassette.

Brief Summary of the Invention

5

The present invention improves upon the prior art by providing a surgical system and cassette, the cassette having an identification method that is specific to the cassette. Suitable methods include bar coding or Radio Frequency Identification ("RFID"). Cassette information that may be encoded include features such as lot number and performance characteristics, such as pressure sensor calibration data, flow and pressure data and any other performance characteristics of the cassette captured during testing of the cassette at manufacture.

Accordingly, one objective of the present invention is to provide a surgical cassette that can be readily identified by the surgical instrument in which the cassette is used.

15

Another objective of the present invention is to provide a surgical system that recognizes information that is cassette specific.

Still another objective of the present invention is to provide a cassette encoded with information specific to the cassette.

20

These and other advantages and objectives of the present invention will become apparent from the detailed description and claims that follow.

Brief Description of the Drawing

FIG. 1 is a perspective view of a surgical console that may be used with the system of the present invention.

25

FIG. 2 is a perspective view of a first embodiment of a cassette suitable for use with the present invention.

FIG. 3 is a perspective view of a first embodiment of a cassette suitable for use with the present invention.

30

Detailed Description of the Preferred Embodiments

As best seen in FIG. 1, surgical console 100 generally contains cassette receiving portion 110 that may contain reader 120. Console 100 may be any suitable surgical console, such as the INFINTI[®] Surgical System commercially available from Alcon Laboratories, Fort Worth, Texas. As best seen in FIG. 2, cassette 10 that may be used with the present invention generally contains bar code 20 placed in a location corresponding to optical reader 120 when cassette 10 is placed within cassette receiving portion 110 of console 100. One skilled in the art will recognize that reader 120 may be a bar code reader, a CCD camera, a CMOS sensor or other suitable optical reader. Bar code 20 may be printed on housing 12 in any suitable location and in any suitable color designed to perform optimally with reader 120. By way of example, bar code 20 may be printed on pressure sensor 40. In this way, if pressure sensor 40 is an optical pressure sensor, reader 120 can be used both for cassette 10 identification and as part of pressure sensor 40. Cassette 10 may be any suitable irrigation/aspiration cassette, such as the INFINTI[®] Fluid Management System commercially available from Alcon Laboratories, Fort Worth, Texas. Alternatively, as seen in FIG. 3, cassette 10' may contain, within or on housing 12', a non-optical means, such as an acoustic or a hard wired or wireless communication device, with microcomputer or RFID chip 30 being one specific example, that is read by detector or receiver 130 in console 100, appropriate microcomputer or RFID chips and detectors/receivers being well-known in the art.

During manufacture of cassettes 10 and 10', information specific to each individual cassette can be recorded into bar code 20 or chip 30. Such information can include lot number, manufacture date, component part tracking information and similar information about cassettes 10 and 10'. In addition, cassettes 10 and 10' may be tested during manufacture and the specific operating performance of individual cassettes 10 and 10' can be recorded and included in the information provided in bar code 20 or chip 30. Such information can include calibration data for aspiration pressure sensors 40 and 40', irrigation pressure sensors 50 and 50', the performance characteristics of peristaltic pump tubes 60 and 60', such characteristics possibly including vacuum rise time, maximum vacuum and flow resistance and being unique to each individual cassette 10 or 10'. Such information can be transferred to surgical console 100 through bar code 20 or chip 30 so that the software contained within console 100 can make automatically, appropriate adjustments in the

operating parameters of console 100 to help assure optimum performance of surgical console 100 and cassettes 10 and 10'.

This description is given for purposes of illustration and explanation. It will be apparent to those skilled in the relevant art that changes and modifications may be made to
5 the invention described above without departing from its scope or spirit.

Claims

1. A surgical system, comprising:
 - a) a surgical console having a cassette receiving portion;
 - b) a cassette sized and shaped to be received in the cassette receiving
5 portion of the surgical console, the cassette comprising:
 - a housing;
 - a means for identifying the cassette and storing information about the
cassette readable by the console;
 - an optical aspiration pressure sensor on the exterior of the housing;
 - 10 c) the surgical console having a detector, so that information contained
within the identifying means can be detected or received by the detector when the
cassette is received by the cassette receiving portion of the surgical console; and
the information contained within the identifying means located in or on the
cassette identifies fluidic performance characteristics specific to the operation of the
15 cassette, unique to each individual cassette and captured during testing of the cassette
at manufacture and software contained within the console adapted to automatically
make appropriate adjustments in the operating parameters of the console, in response
to detecting said information, to help assure optimum performance of the surgical
console in combination with an individual cassette, said fluidic performance
20 characteristics are selected from:
 - calibration data for the optical aspiration pressure sensor, calibration data for
irrigation pressure sensors, the performance characteristics of peristaltic pump tubes,
vacuum rise time for the peristaltic pump tubes, maximum vacuum and flow
resistance for the peristaltic pump tubes.
- 25 2. The system of claim 1, wherein the identifying means is an optical means,
located on the cassette, and wherein the detector is an optical reader located on the
cassette receiving portion of the surgical console.
3. The system of claim 2, wherein the identifying means comprises a bar code.

4. The system of claim 2, wherein the identifying means comprises an optical means located on the optical aspiration pressure sensor.
5. The system of claim 1, wherein the identifying means is a non-optical means, located in or on the cassette, and wherein the detector is located in the surgical console.
6. The system of claim 5, wherein the identifying means comprises a microcomputer chip, or a Radio Frequency Identification (RFID) chip.
7. A surgical cassette sized and shaped to be received in a cassette receiving portion of a surgical console, the cassette comprising:
- 10 a housing;
- a means for identifying the cassette and storing information about the cassette readable by the console;
- an optical aspiration pressure sensor on the exterior of the housing;
- wherein the surgical console has a detector, so that information contained
- 15 within the identifying means can be detected or received by the detector when the cassette is received by the cassette receiving portion of the surgical console; and
- the information contained within the identifying means located in or on the cassette identifies fluidic performance characteristics specific to the operation of the cassette, unique to each individual cassette and captured during testing of the cassette
- 20 at manufacture,
- said fluidic performance characteristics are selected from:
- calibration data for the optical aspiration pressure sensor, calibration data for irrigation pressure sensors, the performance characteristics of peristaltic pump tubes, vacuum rise time for the peristaltic pump tubes, maximum vacuum and flow
- 25 resistance for the peristaltic pump tubes.
8. The cassette of claim 7, wherein the identifying means additionally identifies encoded individual cassette identification data, including lot number, manufacture date, component part tracking information.

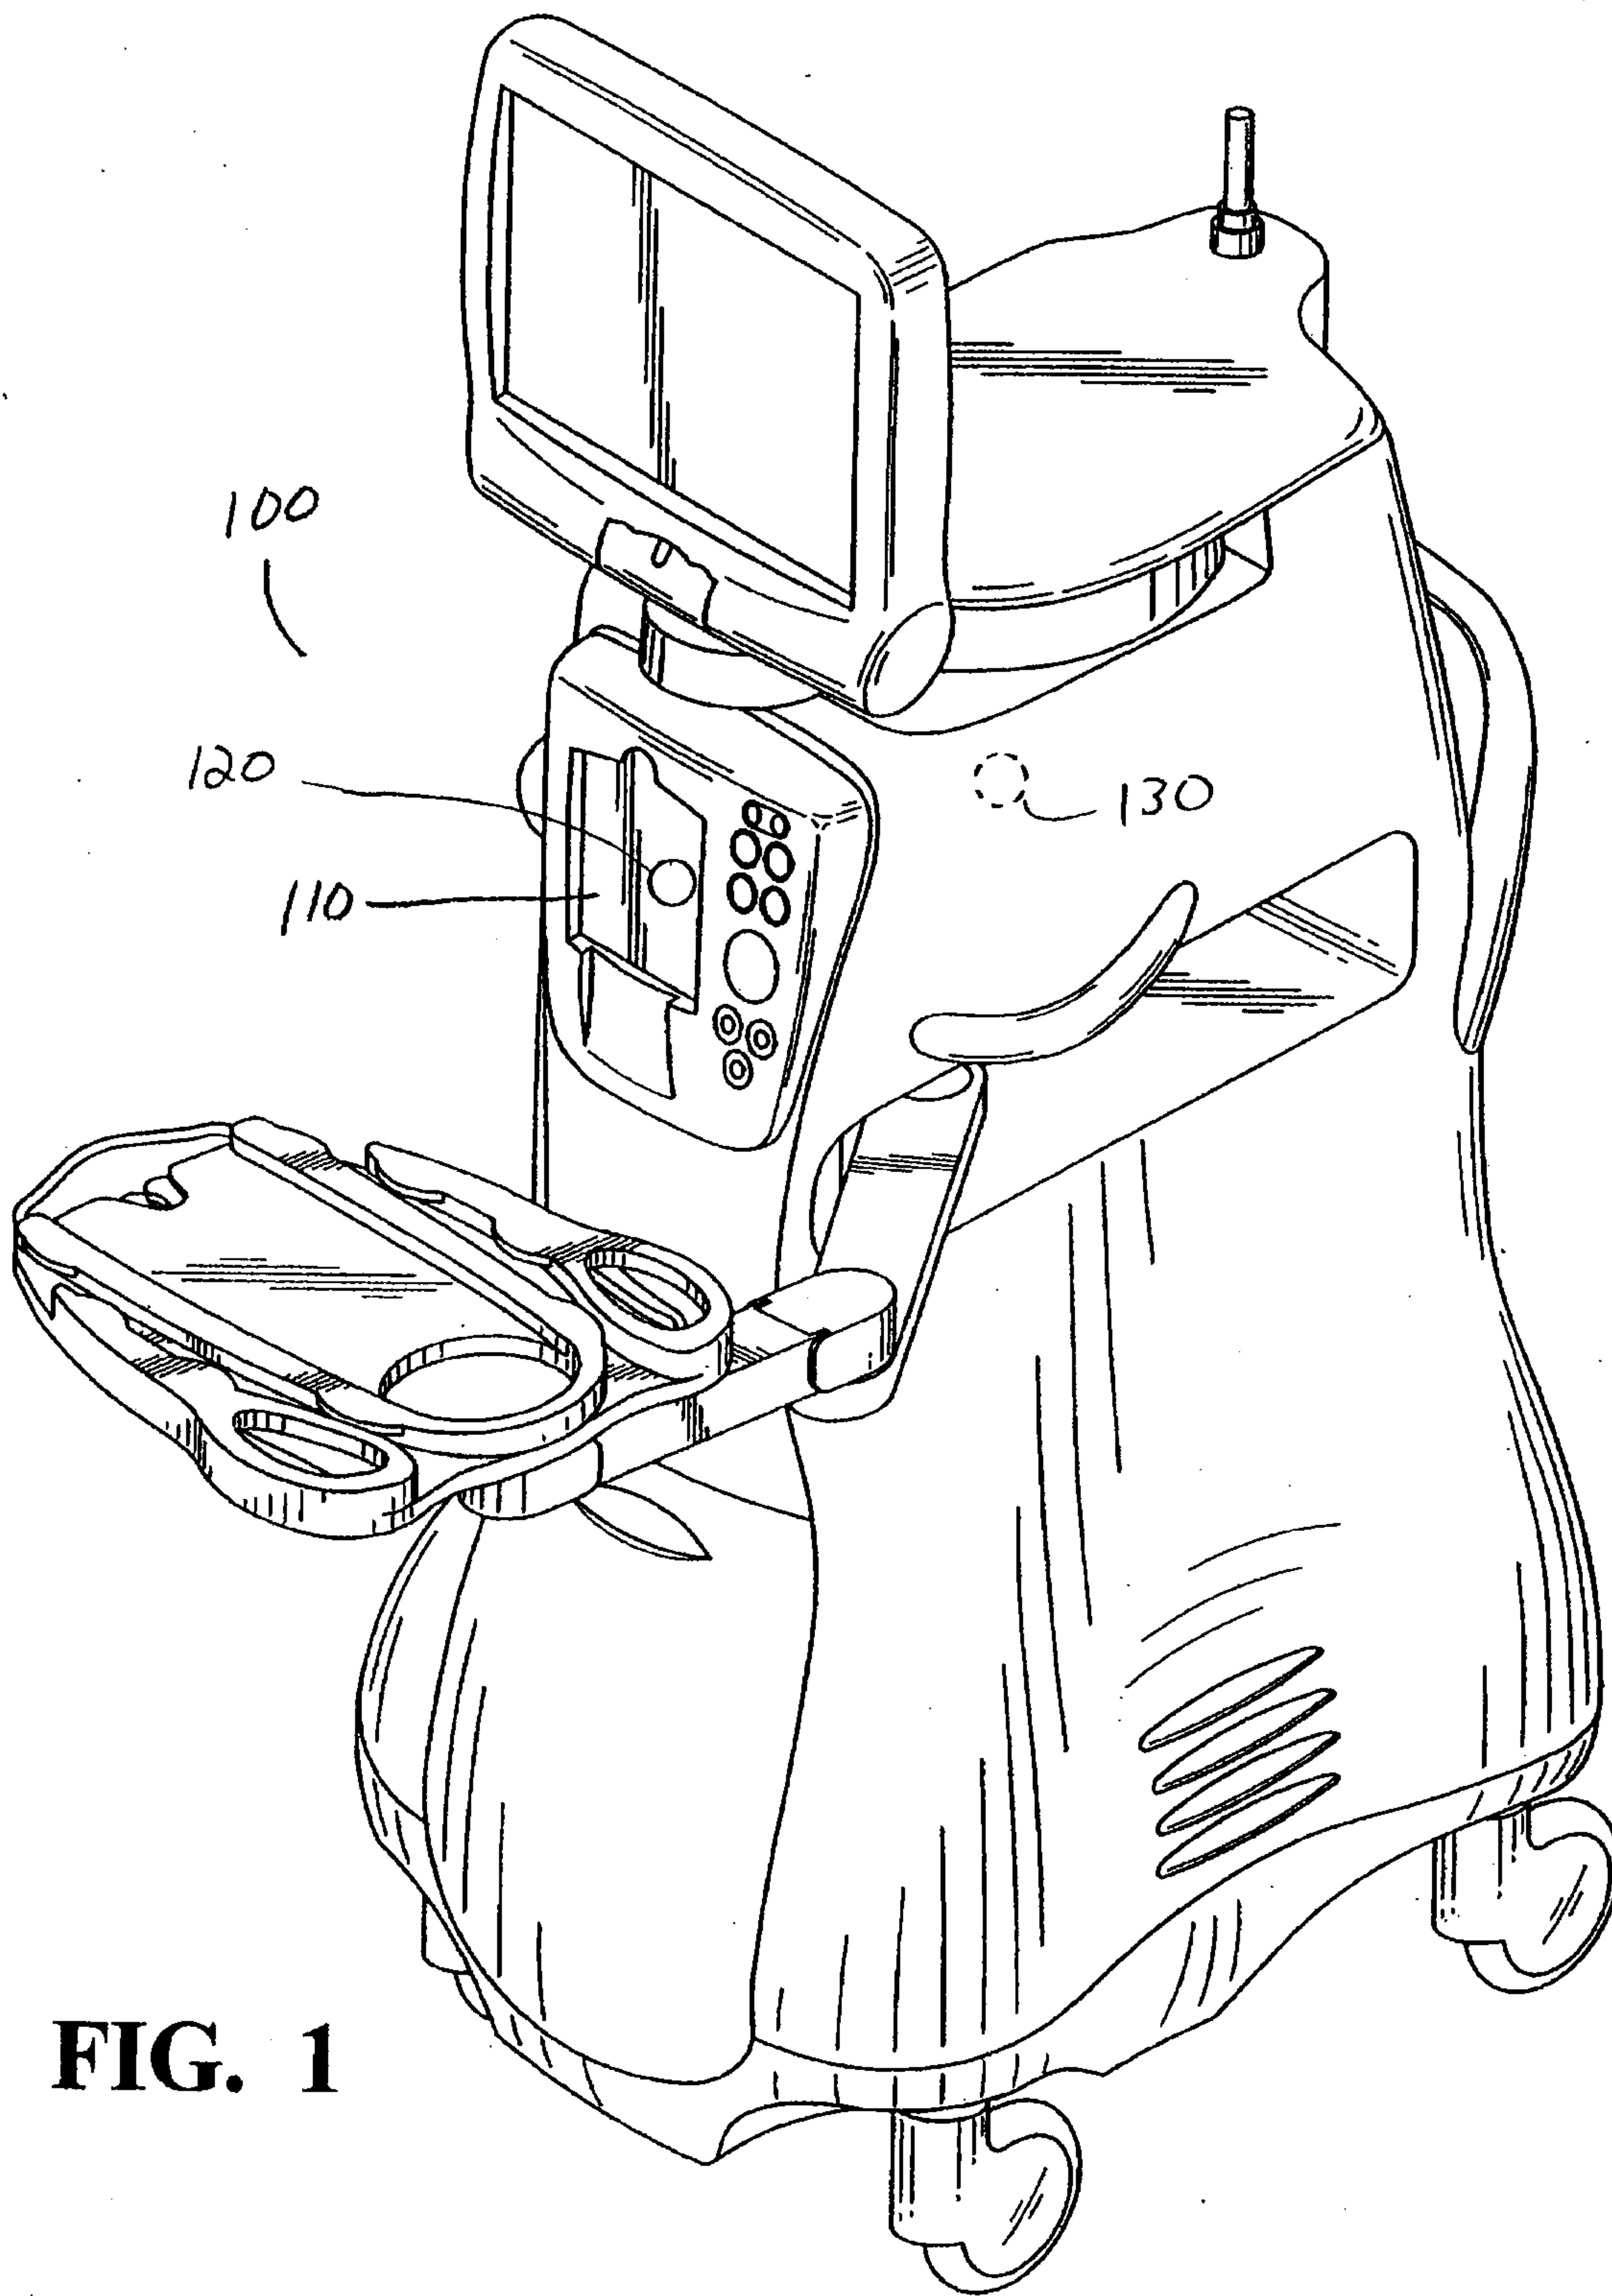


FIG. 1

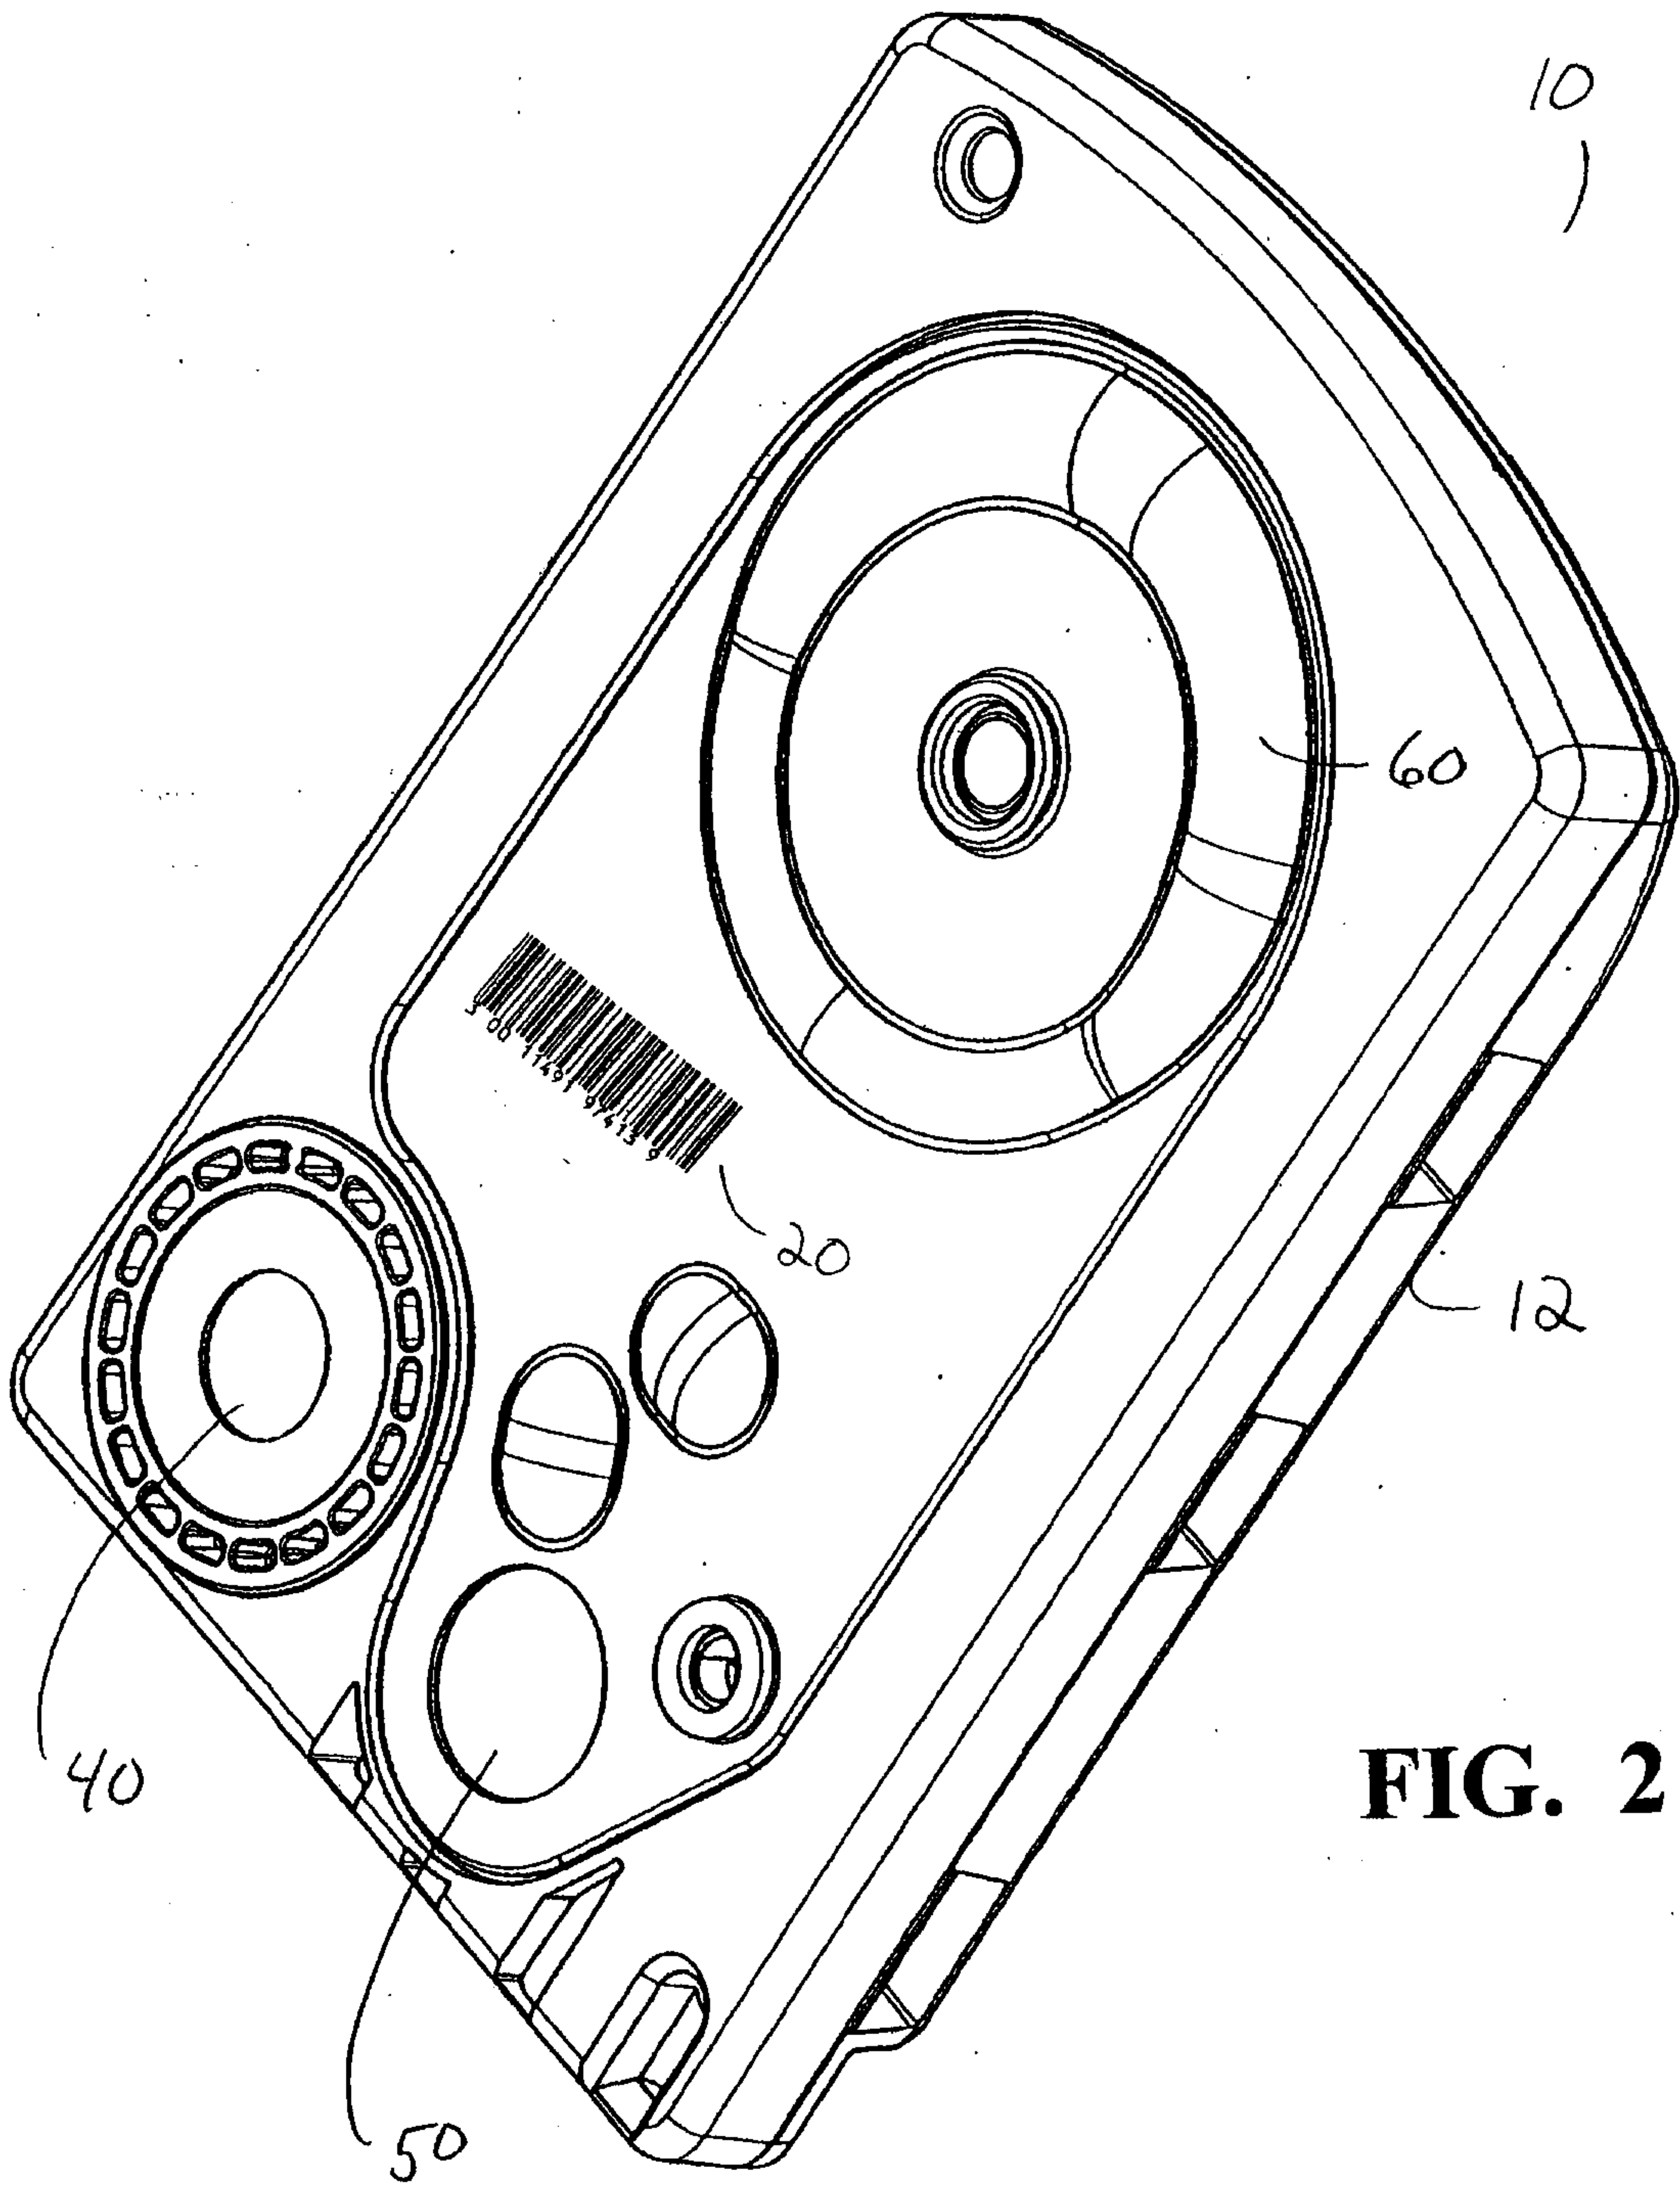


FIG. 2

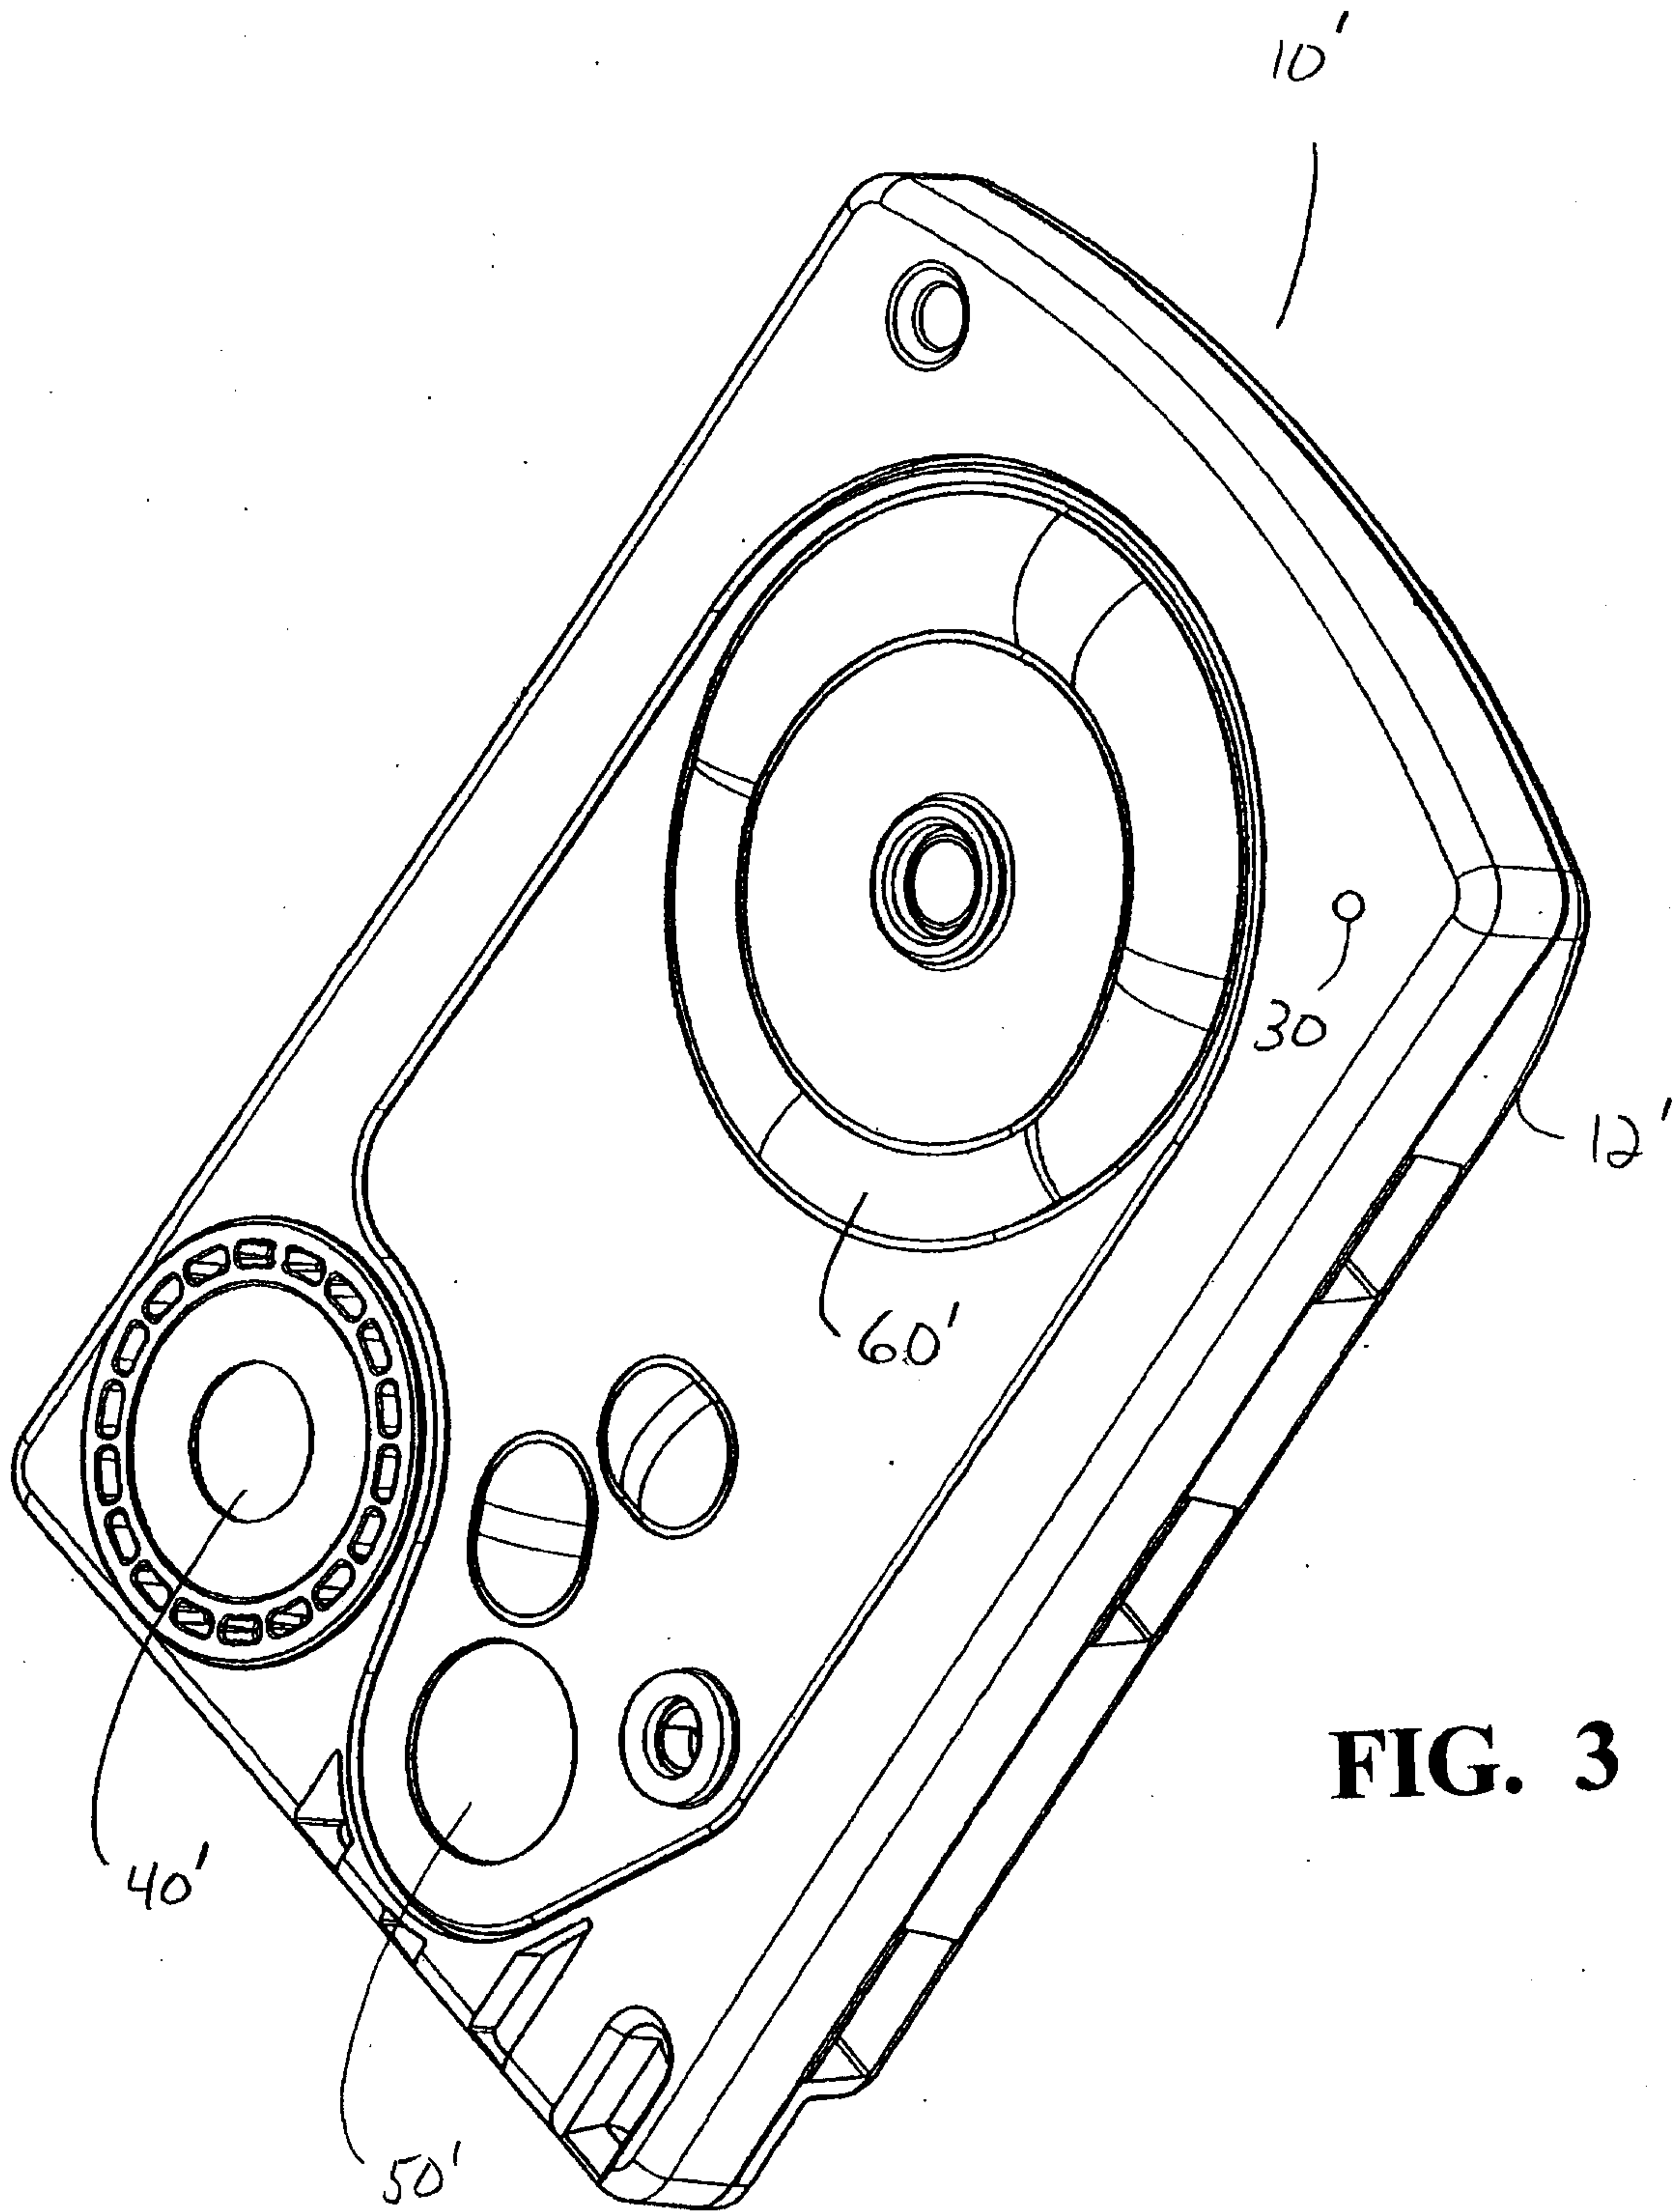


FIG. 3

