

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
26 June 2003 (26.06.2003)

PCT

(10) International Publication Number
WO 03/051214 A1

(51) International Patent Classification⁷: **A61B 18/02**

(21) International Application Number: PCT/US02/39936

(22) International Filing Date:
13 December 2002 (13.12.2002)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
10/024,899 18 December 2001 (18.12.2001) US

(71) Applicant: **SCIMED LIFE SYSTEMS, INC.** [US/US];
One SciMed Place, Maple Grove, MN 55311 (US).

(72) Inventor: **LAFONTAINE, Daniel, M.**; 11400 Fifth Avenue North, Plymouth, MN 55441 (US).

(74) Agent: **SCHAEFER, Stephen, R.**; Fish & Richardson P.C., P.A., 60 South Sixth Street, Suite 3300, Minneapolis, MN 55402 (US).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZM, ZW.


(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: CRYO-TEMPERATURE MONITORING

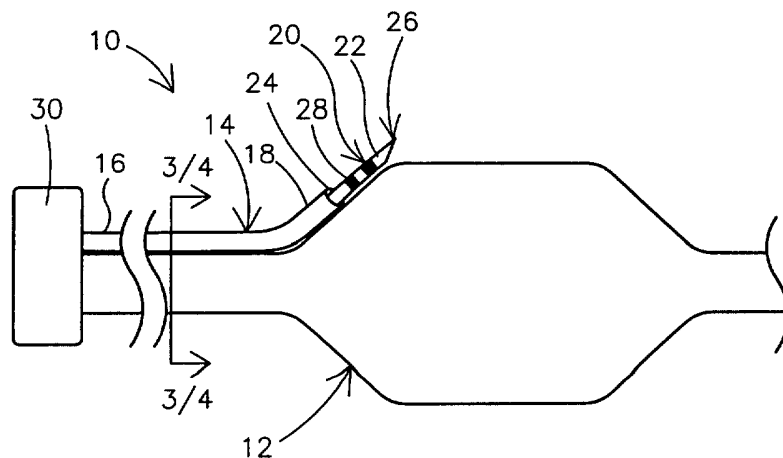

(57) Abstract: Devices and methods for cold-treating lesions within the body. A temperature monitoring device for use with a cryo therapy apparatus may include a cryo therapy apparatus, one or more tubular members coupled to the cryo therapy apparatus, and a temperature monitoring member coupled to the tubular member. The temperature monitoring member may comprise a retractable needle, an infrared sensor, an ultrasound transmitter, or a stent having a plurality of spikes.



WO 03/051214 A1

CRYO-TEMPERATURE MONITORING

Background of the Invention

1. Field of the Invention

The present invention pertains generally to the field of cryo therapy. More particularly, the present invention pertains to cryo balloon therapy catheters for use in causing cold-induced necrosis.

2. Description of the Related Art

A number of medical conditions may be treated using ablative techniques or devices. Ablative techniques, generally, result in the necrosis of abnormal tissue at an area of interest. Ablation of the abnormal tissue may result in an efficacious treatment for a medical condition. For example, atrial fibrillation may be the result of abnormal electrical activity in the left atrium and the pulmonary vein, and may be treatable by ablation of the abnormal tissue within the left atrium and/or the pulmonary vein.

Atrial fibrillation is a serious medical condition that is the result of abnormal electrical activity within the heart. This abnormal activity may occur at regions of the heart including the sino-atrial (SA) node, the atrioventricular (AV) node, the bundle of His, or within other areas of cardiac tissue. Moreover, atrial fibrillation may be caused by abnormal activity within a isolated focal center within the heart. It is believed that these foci can originate within the pulmonary vein, particularly the superior pulmonary veins.

Minimally invasive techniques have been described that use ablation catheters to target the pulmonary vein with the hope of ablating foci having abnormal electrical activity. The techniques typically are characterized by application of energy to cause lesions within the foci or other areas possessing abnormal electrical activity.

Some ablation devices utilize radio frequency (RF) energy for ablation, including the device disclosed in U.S. Patent No. 6,024,740 to Lesh et al. The RF energy devices may be used to ablate an area of interest with heat. The use of RF energy for ablation may, however, lead to untoward healing responses such as collagen build up at the area of interest after treatment. Moreover, RF ablation of within an atrium may decrease atrial output. A need, therefore, exists for ablative devices and methods that include improved healing responses.

An alternative treatment strategy has been developed that uses cooling energy for ablation. This method, termed cryoplasty or cryo balloon therapy, may be used to cool the lesion to freeze a portion of the affected area. For example, cryo balloon therapy may be used to freeze a lesion within a blood vessel that might otherwise lead to restenosis or recoil.

In addition to its potential utility in preventing and slowing restenosis and addressing recoil, cryo balloon therapy may be used for ablation techniques. For example, cryo balloon therapy may be efficacious in varicose vein treatment of incompetent valves, valvular disease, mitral valve regurgitation therapy, atrial fibrillation, gastric reflux disease, gastro esophageal reflux disease, GURD, esophageal disease, cancer treatment including stomach or uterine cancer, etc.

Uses of cryo balloon therapy include cold-induced necrosis of cells within the body. When the target area is located within the heart or pulmonary vasculature, it may be important to precisely control the cryo balloon therapy catheter to necrosis only the desired tissue. Precise temperature regulation may be required to necrosis target tissues while minimizing damage to healthy tissue. Moreover, precise temperature monitoring

may be useful in target areas that have an uneven surface, such as trabeculae within the heart. A need, therefore, exists for cryoplasty catheters with precise temperature monitoring capabilities.

Brief Summary of the Invention

5 The present invention pertains to a refinement to cryo therapy catheters that may incorporate some of the needs described above. More particularly, the present invention comprises a temperature monitoring device for use with a cryo balloon therapy catheters. The temperature monitoring device may be coupled to a cryo therapy catheter and may be used to measure temperature while performing a medical procedure, for example cryo
10 balloon therapy or cryoplasty. The temperature monitoring device may comprise a tubular member having a temperature monitoring member coupled thereto.

 The temperature monitoring member may comprise a retractable needle slidably disposed within a lumen of the tubular member. Alternatively, the temperature monitoring member comprises an infrared optic sensor, an ultrasound transmitter, or a
15 sheath that encircles the cryo therapy apparatus having a plurality of thermal spikes. In addition, one or more tubular members may be disposed about the cryo therapy apparatus in an array.

Brief Description of the Several Views of the Drawings

Figure 1 is a plan view of a cryo therapy apparatus including a retractable needle;

20 Figure 2 is an alternate cryo therapy apparatus including an infrared sensor;

 Figure 3 is a cross-sectional view of a quartet array arrangement of tubular members;

Figure 4 is a cross-sectional view of an octet array arrangement of tubular members;

Figure 5 is a second alternate embodiment of a cryo therapy apparatus including an ultrasound transmitter;

5 Figure 6 is a detailed view of an arrangement of the tubular members shown in Figure 5;

Figure 7 is a third alternate embodiment of a cryo therapy apparatus including a plurality of thermal spikes;

Figure 8 is a fourth alternate embodiment of a cryo therapy apparatus.

10 Detailed Description of the Invention

The following description should be read with reference to the drawings wherein like reference numerals indicate like elements throughout the several views. The detailed description and drawings represent select embodiments and are not intended to be limiting.

15 Figure 1 is a plan overview of a temperature monitoring device 10 for use with a cryo therapy apparatus 12 according to an embodiment of the invention. Temperature monitoring device 10 may include a tubular member 14 having a temperature monitoring member 20 coupled thereto. Temperature monitoring member 20 may be used to measure temperature while performing a medical procedure, for example cryo therapy,
20 cryo balloon therapy, or cryoplasty.

Tubular member 14 includes a proximal end 16 and a distal end 18. Tubular member 14 may be coupled to cryo therapy apparatus 12, for example along the length or proximate an external surface of cryo therapy apparatus 12. Tubular member 14 may be

comprised of materials including, but not limited to, metals, stainless steel, nickel alloys, nickel-titanium alloys, thermoplastics, high performance engineering resins, fluorinated ethylene propylene (FEP), polymer, polyethylene (PE), polypropylene (PP), polyvinylchloride (PVC), polyurethane, polytetrafluoroethylene (PTFE), polyether-ether ketone (PEEK), polyimide, polyamide, polyphenylene sulfide (PPS), polyphenylene oxide (PPO), polysulfone, nylon, perfluoro (propyl vinyl ether) (PFA), combinations thereof, or other suitable materials.

Cryo therapy apparatus 12 is substantially similar to analogous devices (cryo therapy apparatuses, cryoplasty catheters, etc.) disclosed within U.S. Patent No. 5,868,735 to Lafontaine and U.S. Patent Application Serial No. 09/849,892 to Lafontaine, the entire disclosures of which are hereby incorporated by reference. Briefly, cryo therapy apparatus 12 may include a shaft with a cryoplasty device (e.g., a cryoplasty balloon) disposed at a distal end thereof. The shaft may include an inflation tube, a drain tube, and may further comprise an outer sheath defining an annular lumen between the outer sheath and the shaft. The annular lumen may be sealed such that a vacuum may be maintained therein. The cryoplasty device may include a single balloon or multiple balloons (i.e., a first balloon within a second balloon).

In use, coolant may pass through the inflation lumen into the cryoplasty device. The cryoplasty device may then be used for heat transfer with an area of interest. Coolant may be removed from the cryoplasty device through the drain tube following heat transfer.

Temperature monitoring member 20 may comprise a retractable thermocoupled needle 22 slidably disposed within a lumen 24 of tubular member 14. According to this

embodiment, the inside diameter of tubular member 14 is sized appropriately for having temperature monitoring member 20 disposed within lumen 24. Thermocoupled retractable needle 22 is understood to include temperature sensing means that measure temperature in a manner that is quantifiable by a clinician. Alternatively, retractable
5 needle 22 may include a temperature sensor coupled thereto. Retractable needle 22 may include a sharpened distal point 26 and at least one marker band 28. Distal point 26 may be adapted to penetrate and/or cut into tissue during a medical procedure.

From Figure 1 it can be appreciated that temperature monitoring member 20 (and others described below) have a length along the longitudinal axis and extends away from
10 cryo therapy apparatus 12 along the longitudinal axis. Moreover, an angle may be defined between temperature monitoring member 20 and cryo therapy apparatus 12. This angle may be about 90°, acute, or obtuse. It can also be seen in Figure 1 that the length of temperature monitoring member 20 that extends from cryo therapy apparatus is greater than its width (measured along the axis perpendicular to the longitudinal axis).

15 Marker band 24 may produce a relatively bright image on a fluoroscopy screen during a medical procedure. This relatively bright image aids the user of marker band 24 in determining the location of temperature monitoring member 20. Marker band 24 may comprise a number of radiopaque materials including, but not limited to, gold, platinum, and plastic material loaded with a radiopaque filler. Temperature monitoring member 20
20 may further comprise additional marker bands or may comprise a marker band disposed at a different location. For example, marker band 24 may comprise a first marker band (e.g., marker band 24) a fixed distance from distal point 22 of temperature monitoring member 20. A second marker band may be disposed on temperature monitoring member

20 proximally a distance that is approximately equal to the distance the first marker band is from distal point 22.

Proximal end 16 of tubular member 14 may be connected to a manifold 30. Manifold 30 comprises means for controlling temperature monitoring member 20. More specifically, manifold 30 may comprise means for quantifying temperature as measured
5 by, for example, thermocoupled needle 20. Means for quantifying temperature may include an analog temperature reading or display, a digital temperature reading or display, a connector for coupling to a computerized system for measuring temperature, a computerized system for processing other data, and combinations thereof.

10 In use, temperature monitoring device 10 may be advanced to an area of interest. The area of interest may be, for example, an artery including the pulmonary artery, a vein including the pulmonary vein, a blood vessel, the heart, trabeculae within the heart, a body organ, or other areas where cryoplasty may prove beneficial. Cryo therapy apparatus 12 may be used to cool the area of interest while temperature monitoring
15 member 20 may be used to quantify temperature by inserting distal point 26 into tissue at the area of interest. In an embodiment, distal point 26 may contact the surface of the tissue at the area of interest or it may penetrate and/or cut into the tissue to measure temperature below the surface. Marker band 28 may be used to determine the location of distal point 26 during heat transfer. Accurately determining the location of distal point 26
20 may allow more precise cooling and prevent possible tissue damage due to over-cooling. Alternatively, the needles may have pre-determined depth marker band/stops which allow tissue penetration to a fixed depth such as 1-3mm, etc.

Figure 2 is a plan view of an alternate temperature monitoring device 110 according to an embodiment of the invention. Temperature monitoring device 110 is substantially similar to temperature monitoring device 10 except that temperature monitoring member 120 comprises an infrared or optic sensor 132. At least a portion of
5 infrared or optic sensor 132 may be disposed within a lumen of tubular member 114, i.e., the equivalent of lumen 24 of tubular member 14. Alternatively, infrared or optic sensor 132 may be disposed proximate distal end 218 of tubular member 214.

Temperature monitoring device 110 may be used to measure temperature at an area of interest by detecting infrared energy at the area of interest with infrared sensor 32.
10 Quantification of infrared energy may comprise a measurement of heat and/or temperature. Manifold 30 comprises means for quantifying temperature. For example, manifold 30 may comprise means for quantifying infrared energy.

Cooling may result in the formation of ice or ice balls adjacent cryo therapy apparatus 12 and/or the treatment site. As a result, alternative temperature monitoring
15 members may be used. For example, in order to monitor or otherwise visualize ice or ice ball formation, optical sensing may be used. Optic sensing may be looking at the ice ball visually by color change or appearance of ice. Other methods may be used as described herein to monitor ice formation as well as methods known to those in the art.

Figure 3 and Figure 4 depict a plan overview of arrangements of tubular members
20 14 taken through section 3/4-3/4 of Figure 1 and depicting additional tubular members 14. More than one tubular member 14 may be disposed about cryo therapy apparatus 12 in an array. Four tubular members 14 may be disposed about cryo therapy apparatus 12 in a quartet array as shown in Figure 3. Similarly, Figure 4 depicts eight tubular members 14,

evenly spaced between, and disposed about cryo therapy apparatus 12 in an octet array. Although Figure 3 and Figure 4 depict arrangements of tubular member 14, it should be understood that any of the tubular members, temperature monitoring devices, and analogous structures disclosed herein may be substituted without departing from the spirit
5 of the invention.

Figure 5 is a plan view of an alternate temperature monitoring device 210 according to an embodiment of the invention. Temperature monitoring device 210 is substantially similar to temperature monitoring device 10 except that temperature monitoring member 220 comprises an ultrasound transmitter 234. Similar to what is
10 disclosed above, at least a portion of ultrasound transmitter 234 may be disposed within a lumen of tubular member 214 or ultrasound transmitter 234 may be disposed at distal end 218 of tubular member 214.

Temperature monitoring device 210 may be used to measure temperature at an area of interest by transmitting ultrasound energy from ultrasound transmitter 234.
15 Manifold 30 may comprise means for quantifying temperature including means for accumulating ultrasound images, ultrasound energy, and other ultrasound data. Analysis of ultrasound images, ultrasound energy, and other ultrasound data may provide an indirect measurement of temperature. For example, an ultrasound image may be used to view a phase change within the area of interest. The phase change may indicate a
20 quantifiable level of cooling.

Figure 6 is a detailed view of a tubular members 214 taken through line 6-6 of Figure 5 and depicting addition tubular members 214. In an embodiment, tubular members 214 may be disposed about cryo therapy apparatus 12 in an array. In an

exemplary embodiment, the array may be a circular array. The circular array may enable a user to more precisely measure temperature and determine the location of temperature monitoring device 210. In addition, tubular members 214 may be arranged in a quartet or octet array as disclosed above, and tubular members 14 and 114 may also be arranged in a
5 circular array.

Figure 7 is a plan view of an alternate temperature monitoring device 310 according to an embodiment of the invention. Temperature monitoring device 310 is substantially similar to temperature monitoring device 10 with a number of refinements described below.

10 Tubular member 314 comprises a sheath that, encircles cryo therapy apparatus 12. Temperature monitoring member 320 comprises a stent 36 disposed at distal end 318 of tubular member 314. Stent 36 may further comprise a plurality of thermal spikes 38. Stent 36 is comprised of a shape memory alloy (e.g., nickel-titanium alloy). Alternatively, stent 36 may be comprised of materials similar to those listed above
15 including metals and polymers.

Thermal spikes 38 may be capable of measuring temperature at an area of interest. According to this embodiment, thermal spikes 38 may be coupled to manifold 30 such that a user may quantify temperature. Manifold 30 may comprise means for quantifying temperature including those listed above.

20 In addition, thermal spikes 38 may be used to facilitate heat transfer to an area of interest. For example, trabeculae within the heart may not allow cryo therapy apparatus 12 to evenly cool the heart. The result may be uneven or incomplete heat transfer. Thermal spikes 38 may be capable of reaching, contacting, and penetrating surfaces of an

area of interest. For example, thermal spikes 38 may be capable of contacting trabeculae within the heart and may, thus, facilitate heat transfer to these areas.

In an embodiment, stent 36 may be collapsed at body temperature and be expanded when cooled. A collapsed state at body temperature will minimize the outside
5 diameter of stent 36, which may facilitate delivery of temperature monitoring device 310 to an area of interest. Cooling, for example cooling initiated by cryo therapy apparatus 12, may expand stent 36 in order to move thermal spikes 38 proximate the area of interest.

Figure 8 illustrates another alternative temperature monitoring device 410.
10 Device 410 includes cryo therapy apparatus 412 coupled to manifold 30 essentially as described above. In addition, tubular member 414 may be coupled to cryo therapy apparatus 412. For example, tubular member 414 may be disposed at least partially within cryo therapy apparatus 12 or within the shaft portion of cryo therapy apparatus 12. When disposed within cryo therapy apparatus 12, tubular member 414 may be
15 substantially coaxial with or proximate an interior wall of apparatus 12.

Temperature monitoring member 420 may be disposed within tubular member 441 and may extend into cryo therapy apparatus 12. In an alternative embodiment, temperature monitoring member 420 may be disposed within cryo therapy apparatus 12 without the use of tubular member 441. For example, temperature monitoring member
20 420 may be disposed within the shaft of cryo therapy apparatus 12.

Temperature monitoring member 420 includes an optical imaging apparatus 434 including an emitter 440 and a detector 442. Emitter 440 is adapted and configured to emit energy (e.g., light, infrared energy, ultrasonic energy, etc.) from within cryo therapy

apparatus. Detector 442 is adapted to collect data by detecting energy. A number of different arrangements of emitters and/or detectors may be used without departing from the spirit of the invention.

Cryo therapy apparatus 412 is essentially the same in form and function as cryo
5 therapy apparatus 12 but further includes an inner cooling chamber 444 and an outer
cooling chamber 446. A dual-chamber cooling apparatus (such as apparatus 412) may
provide additional safety or cooling advantages. For example, outer cooling chamber 446
may prevent loss of coolant into the body if inner cooling chamber 444 failed. It can be
appreciated that the dual chamber cooling apparatus 412 can be substituted into any of the
10 other embodiments described herein.

Numerous advantages of the invention covered by this document have been set
forth in the foregoing description. It will be understood, however, that this disclosure is,
in many respects, only illustrative. Changes may be made in details, particularly in
matters of shape, size, and arrangement of steps without exceeding the scope of the
15 invention. The invention's scope is, of course, defined in the language in which the
appended claims are expressed.

CLAIMS

What is claimed is:

1. A temperature monitoring device for use with a cryo therapy apparatus,
comprising:

5 a cryo therapy apparatus;
a tubular member coupled to the cryo therapy apparatus; and
a temperature monitoring member coupled to the tubular member.

2. The temperature monitoring device according to claim 1, wherein the
10 temperature monitoring member is coupled to the cryo therapy apparatus in a quartet
array.

3. The temperature monitoring device according to claim 1, wherein the
temperature monitoring member is coupled to the cryo therapy apparatus in a octet array.

15 4. The temperature monitoring device according to claim 1, wherein the
temperature monitoring member is coupled to the cryo therapy apparatus in a circular
array.

20 5. The temperature monitoring device according to claim 1, wherein the
tubular member further comprises a proximal end, a distal end, and a lumen extending
therethrough.

6. The temperature monitoring device according to claim 5, wherein the temperature monitoring member comprises a retractable needle slidably disposed within the lumen of the tubular member.

5 7. The temperature monitoring device according to claim 6, wherein the retractable needle further comprises a marker band.

8. The temperature monitoring device according to claim 1, wherein the temperature monitoring member comprises an infrared sensor.

10

9. The temperature monitoring device according to claim 1, wherein the temperature monitoring member comprises an ultrasound transmitter.

10. The temperature monitoring device according to claim 1, wherein the
15 temperature monitoring member comprises an expandable stent having a plurality of thermal spikes.

11. The temperature monitoring device according to claim 11, wherein the stent comprises nickel-titanium alloy.

20

12. A temperature monitoring device for use with a cryo therapy apparatus, comprising:

a cryo therapy apparatus;

a plurality of tubular members coupled to the cryo therapy apparatus, the tubular members each coupled to a temperature monitoring member and arranged in an array; and

wherein the temperature monitoring member can measure the temperature at an area of interest while the cryoplasty device cools the area of interest.

5

13. The temperature monitoring device according to claim 12, wherein the tubular member further comprises a proximal end, a distal end, and a lumen extending therethrough.

10

14. The temperature monitoring device according to claim 13, wherein the temperature monitoring member comprises a retractable needle slidably disposed within the lumen of the tubular member.

15

15. The temperature monitoring device according to claim 14, wherein the retractable needle further comprises a marker band.

16. The temperature monitoring device according to claim 12, wherein the temperature monitoring member comprises an infrared sensor.

20

17. The temperature monitoring device according to claim 12, wherein the temperature monitoring member comprises an ultrasound transmitter.

18. The temperature monitoring device according to claim 12, wherein the temperature monitoring members are arranged in a quartet array.

19. The temperature monitoring device according to claim 12, wherein the
5 temperature monitoring members are arranged in an octet array.

20. The temperature monitoring device according to claim 12, wherein the temperature monitoring members are arranged in a circular array.

10 21. The temperature monitoring device according to claim 12, wherein the temperature monitoring member an expandable stent having a plurality of thermal spikes.

22. The temperature monitoring device according to claim 21, wherein the stent comprises nickel-titanium alloy.

15

23. A method of monitoring the temperature of an area of interest during a cryoplasty procedure, comprising the steps of:

providing a temperature monitoring device including a cryo therapy apparatus, a tubular member coupled to the cryo therapy apparatus, the tubular member including a
20 temperature monitoring member;

advancing the temperature monitoring device to an area of interest;

cooling the area of interest with the cryo therapy apparatus; and

measuring temperature at the area of interest with the temperature monitoring member.

24. The method according to claim 23, wherein the tubular member further
5 comprises a proximal end, a distal end, and a lumen extending therethrough.

25. The method according to claim 24, wherein the temperature monitoring member comprises a retractable needle slidably disposed within the lumen of tubular member.

10

26. The method according to claim 25, wherein the retractable needle further comprises a marker band.

27. The method according to claim 26, wherein the step of measuring
15 temperature with the temperature monitoring member includes penetrating the area of interest with the retractable needle.

28. The method according to claim 23, wherein the temperature monitoring member comprises an infrared sensor.

20

29. The method according to claim 28, wherein the step of measuring temperature with the temperature monitoring member includes detecting infrared energy at the area of interest.

30. The method according to claim 23, wherein the temperature monitoring member comprises an ultrasound transmitter.

5 31. The method according to claim 30, wherein the step of measuring temperature with the temperature monitoring member includes irradiating the area of interest with ultrasound energy.

32. The method according to claim 23, wherein the temperature monitoring
10 member an expandable stent having a plurality of thermal spikes.

33. The method according to claim 32, wherein the step of measuring temperature with the temperature monitoring member includes penetrating the area of interest with the thermal spike.
15

34. The method according to claim 32, wherein the stent comprises nickel-titanium alloy.

35. A temperature monitoring device for use with a cryo therapy apparatus,
20 comprising:

a cryo therapy apparatus;

a tubular member coupled to the cryo therapy apparatus; and

a temperature monitoring member coupled to the tubular member, the temperature monitoring member having a length extending from the cryo therapy apparatus along a longitudinal axis and a width; and

wherein the length of the temperature monitoring member extending away from
5 the cryo therapy apparatus along the longitudinal axis is larger than the width.

36. The temperature monitoring device in accordance with claim 35, wherein the temperature monitoring member extends from the cryo therapy apparatus at an angle.

10 37. The temperature monitoring device in accordance with claim 36, wherein the angle is about 90°.

38. The temperature monitoring device in accordance with claim 36, wherein the angle is acute.

15

39. The temperature monitoring device in accordance with claim 36, wherein the angle is obtuse.

40. A temperature monitoring device for use with a cryo therapy apparatus,
20 comprising:

a cryo therapy apparatus; and

a temperature monitoring member coupled to the cryo therapy apparatus, wherein at least a portion of the temperature monitoring member is disposed within the cryo therapy apparatus.

5 41. A temperature monitoring device for use with a cryo therapy apparatus, comprising:

an elongate shaft having a distal end;

a cooling chamber disposed at the distal end of the shaft;

10 a temperature monitoring member coupled to the shaft, wherein at least a portion of the temperature monitoring member is disposed within the cooling chamber.

42. The temperature monitoring device in accordance with claim 41, wherein the cooling chamber includes an outer cooling chamber and an inner cooling chamber.

FIG. 1

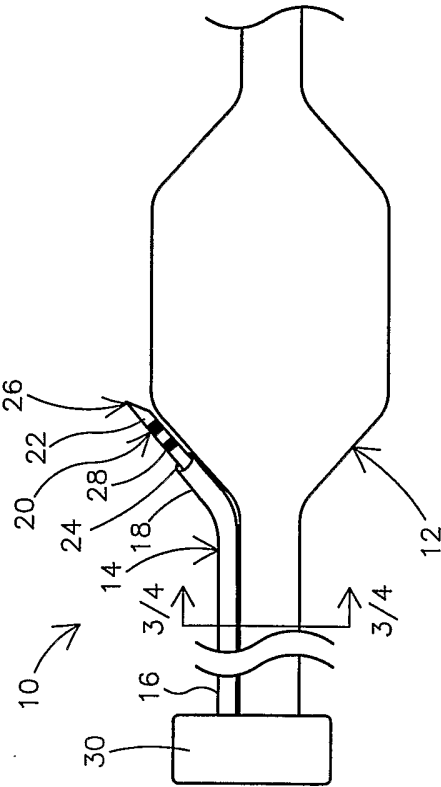


FIG. 2

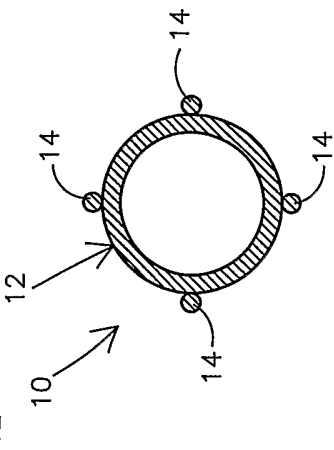
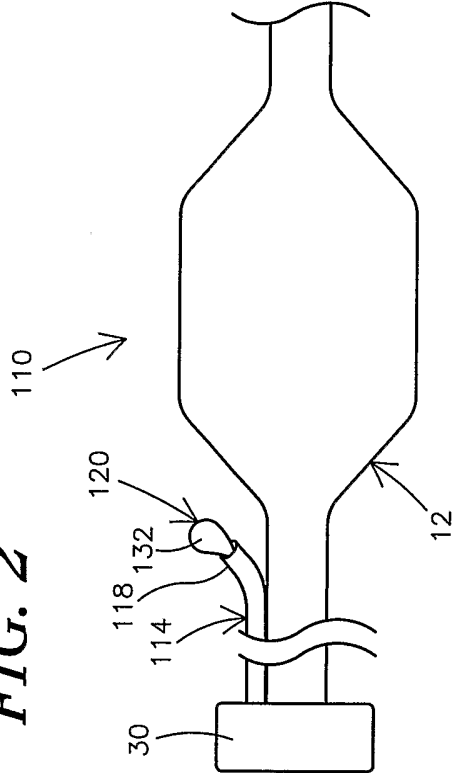


FIG. 3

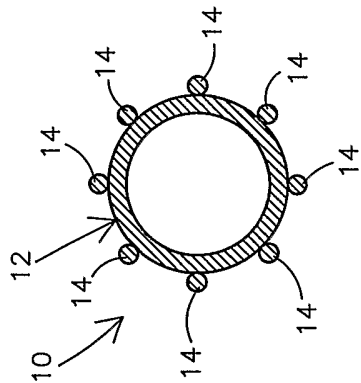


FIG. 4

FIG. 5

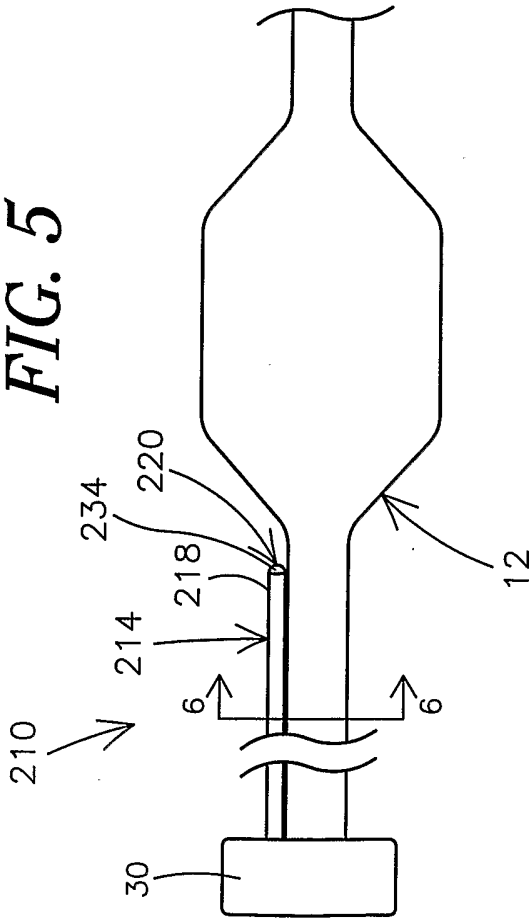


FIG. 6

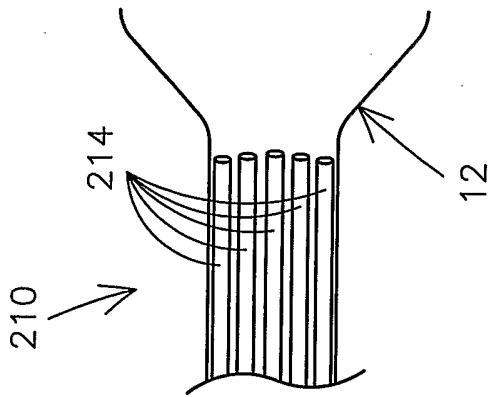
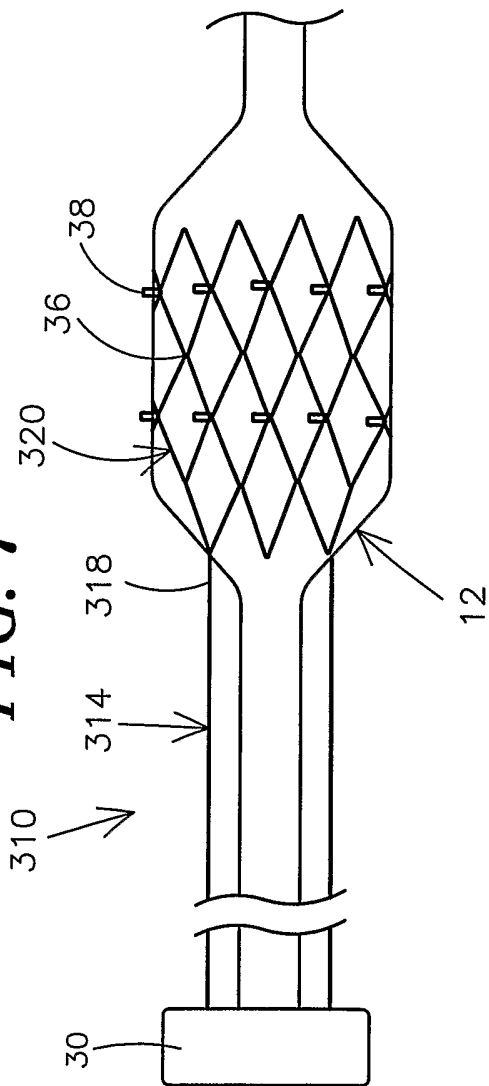


FIG. 7



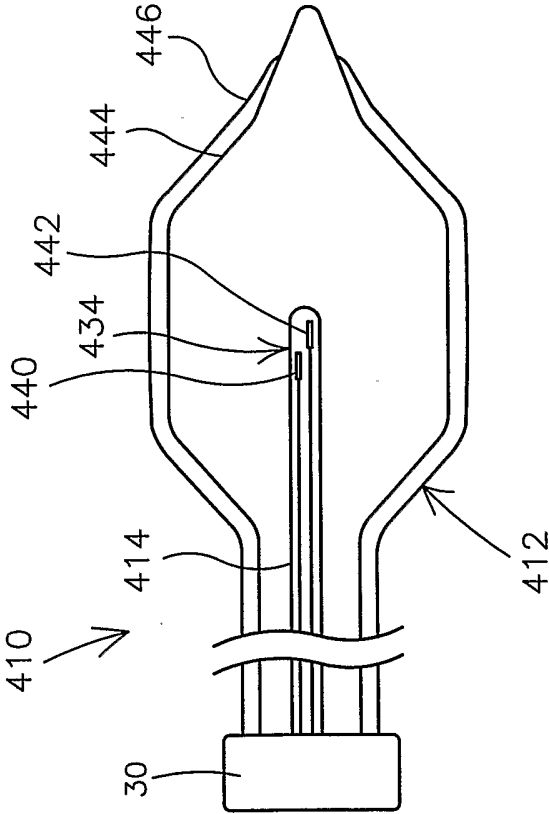


FIG. 8

INTERNATIONAL SEARCH REPORT

In national Application No

F... S 02/39936

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61B18/02

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 01 22897 A (NOVASYS MEDICAL INC) 5 April 2001 (2001-04-05) page 8, line 6 - line 22; figure 1 page 18, line 1 - line 9; figure 3 page 18, line 24 - page 19, line 7 page 21, line 1 - line 3 ---	1,2,5-7, 10, 12-15,21
X	WO 00 47121 A (KORPAN NIKOLAI ;ZHARKOV JAROSLAV (UA)) 17 August 2000 (2000-08-17) abstract; figure 2 ---	40
A	---	41
X	DE 197 24 082 A (TRICUMED GMBH) 10 December 1998 (1998-12-10) claim 1; figure ---	41
Y	---	42
	--- -/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

° Special categories of cited documents:

A document defining the general state of the art which is not considered to be of particular relevance

E earlier document but published on or after the international filing date

L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

O document referring to an oral disclosure, use, exhibition or other means

P document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

& document member of the same patent family

Date of the actual completion of the international search

7 April 2003

Date of mailing of the international search report

14/04/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Ducreau, F

INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 02/39936

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y A	US 5 220 927 A (ASTRAHAN MELVIN A ET AL) 22 June 1993 (1993-06-22) column 8, line 10 - line 22; figures 1,5	1,5-7, 35-39 12-15, 35,40,41
Y	--- US 5 868 735 A (LAFONTAINE DANIEL M) 9 February 1999 (1999-02-09) cited in the application column 2, line 49 - column 3, line 14; figures 1-3	1,5-7
Y A	--- FR 2 403 063 A (KI GI) 13 April 1979 (1979-04-13) page 4, line 28 - line 39; figure 1	35-39 1,12
Y A	--- WO 00 47118 A (JAYARAMAN SWAMINATHAN) 17 August 2000 (2000-08-17) page 7, line 1 - line 26; figure 10	42 40,41
A	--- US 5 562 720 A (RICHTMAN ROXANNE L ET AL) 8 October 1996 (1996-10-08) column 7, line 53 - line 61; figure 1	1,4,12
A	--- US 5 057 106 A (MCQUEENEY JAMES F ET AL) 15 October 1991 (1991-10-15) column 7, line 43 - line 46; figure 1 -----	40,41

INTERNATIONAL SEARCH REPORT

national application No.
PCT/US 02/39936**Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)**

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 22-34
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

 In ai Application No
 101/US 02/39936

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
WO 0122897	A	05-04-2001	AU	7735200 A		30-04-2001
			EP	1244392 A1		02-10-2002
			WO	0122897 A1		05-04-2001
WO 0047121	A	17-08-2000	AT	409715 B		25-10-2002
			AT	409716 B		25-10-2002
			AT	409585 B		25-09-2002
			AT	409453 B		26-08-2002
			AT	409454 B		26-08-2002
			AT	20399 A		15-03-2002
			WO	0047121 A2		17-08-2000
			EP	1083838 A2		21-03-2001
			AT	57199 A		15-03-2002
			AT	74199 A		15-02-2002
			AT	75399 A		15-01-2002
			AT	76799 A		15-01-2002
DE 19724082	A	10-12-1998	DE	19724082 A1		10-12-1998
US 5220927	A	22-06-1993	US	4967765 A		06-11-1990
			EP	0462302 A1		27-12-1991
			US	5344435 A		06-09-1994
			US	5249585 A		05-10-1993
US 5868735	A	09-02-1999	EP	0910295 A1		28-04-1999
			WO	9838934 A1		11-09-1998
			US	6290696 B1		18-09-2001
			US	2002032438 A1		14-03-2002
FR 2403063	A	13-04-1979	FR	2403063 A1		13-04-1979
WO 0047118	A	17-08-2000	WO	0047118 A1		17-08-2000
			AU	2679799 A		29-08-2000
			EP	1158906 A1		05-12-2001
			JP	2002536106 T		29-10-2002
US 5562720	A	08-10-1996	US	5277201 A		11-01-1994
			US	5443470 A		22-08-1995
			US	5443463 A		22-08-1995
			AT	216274 T		15-05-2002
			AU	679271 B2		26-06-1997
			AU	7931494 A		04-05-1995
			CA	2173851 A1		20-04-1995
			DE	69430435 D1		23-05-2002
			DE	69430435 T2		14-11-2002
			EP	0723467 A1		31-07-1996
			ES	2174880 T3		16-11-2002
			JP	9503689 T		15-04-1997
			WO	9510326 A1		20-04-1995
			US	5643304 A		01-07-1997
			AT	164503 T		15-04-1998
			AU	4105293 A		29-11-1993
			CA	2117900 A1		11-11-1993
			DE	69317776 D1		07-05-1998
			DE	69317776 T2		10-09-1998
			EP	0637943 A1		15-02-1995
			FI	945112 A		31-10-1994
			IL	105523 A		10-01-1997

INTERNATIONAL SEARCH REPORT

Int	Patent Application No
P	S 02/39936

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5562720	A	JP 7506033 T	06-07-1995
		NO 944072 A	26-10-1994
		WO 9321846 A1	11-11-1993
		US 6041260 A	21-03-2000
		US 5713942 A	03-02-1998
		AT 230284 T	15-01-2003
		AU 6625594 A	08-11-1994
		CA 2159483 A1	27-10-1994
		DE 69431950 D1	06-02-2003
		EP 0693955 A1	31-01-1996
		JP 8508912 T	24-09-1996
		WO 9423794 A1	27-10-1994
		AU 7671594 A	14-03-1996
		WO 9605776 A1	29-02-1996
US 5057106	A	US 4700716 A	20-10-1987
	15-10-1991	AU 3696989 A	12-12-1989
		EP 0415997 A1	13-03-1991
		WO 8911311 A1	30-11-1989
		EP 0385978 A1	12-09-1990
		WO 8902292 A1	23-03-1989
		US 4776086 A	11-10-1988