




US 20070179607A1

(19) **United States**(12) **Patent Application Publication****Hodorek et al.**(10) **Pub. No.: US 2007/0179607 A1**(43) **Pub. Date: Aug. 2, 2007**(54) **CARTILAGE RESURFACING IMPLANT**(22) Filed: **Jan. 31, 2006**(75) Inventors: **Robert A. Hodorek**, Warsaw, IN (US);
Antony J. Lozier, Warsaw, IN (US);
Cheryl R. Blanchard, Warsaw, IN (US)**Publication Classification**(51) **Int. Cl.**
A61F 2/30 (2006.01)(52) **U.S. Cl.** **623/14.12; 623/23.51; 623/23.5**

Correspondence Address:

John F. Hoffman, Esq.
BAKER & DANIELS LLP
111 East Wayne Street, Suite 800
Fort Wayne, IN 46802 (US)(57) **ABSTRACT**

A cartilage resurfacing implant is provided for replacing cartilage of an articulating portion of a bone at a skeletal joint having opposed joint surfaces. The cartilage resurfacing implant includes a body having a bearing surface and a bone interface. The bearing surface is able to support articulation with an opposing joint surface.

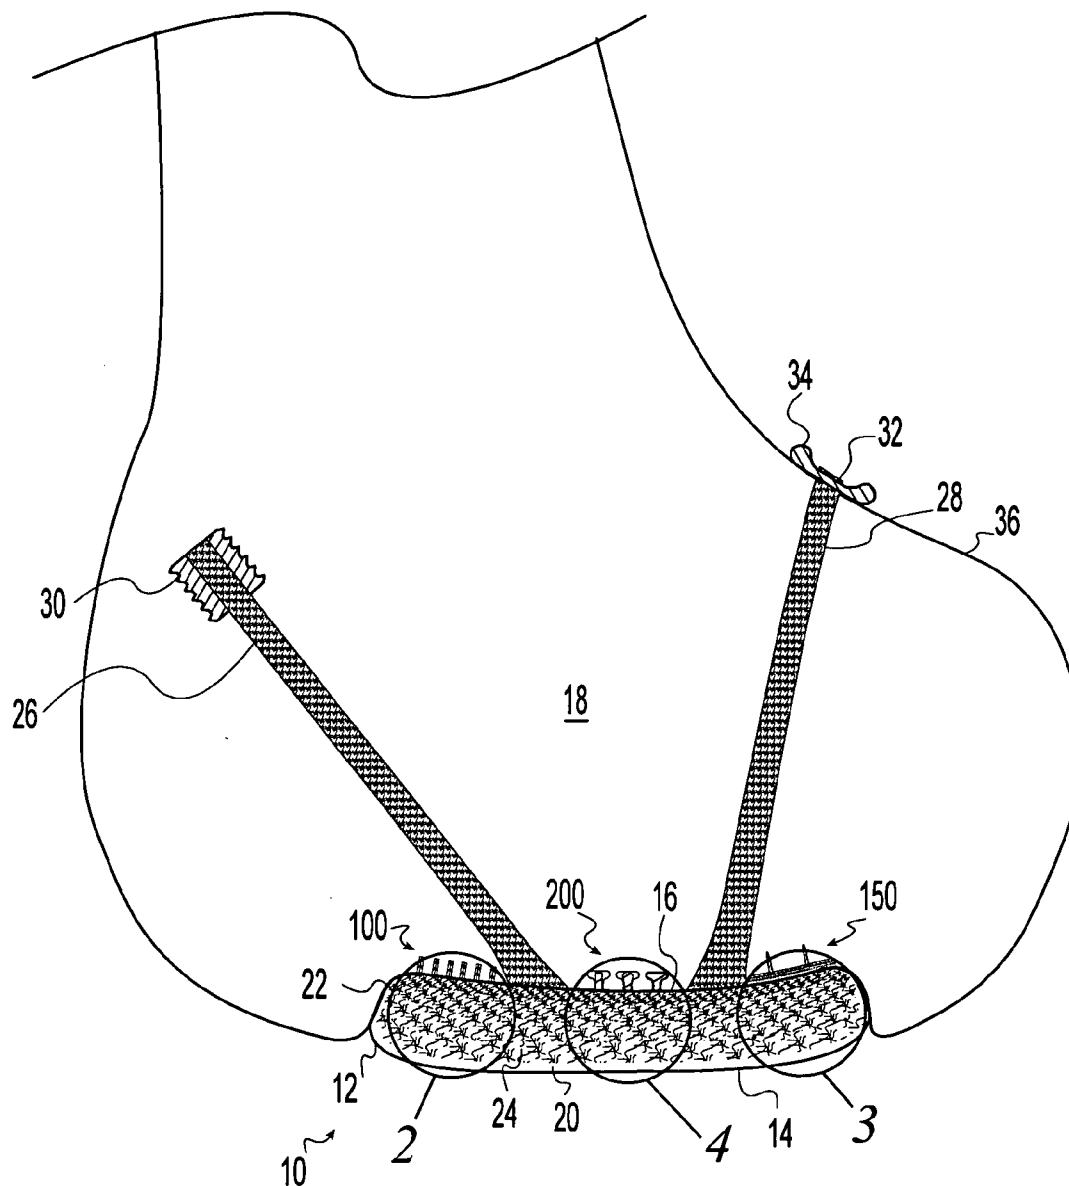(73) Assignee: **Zimmer Technology, Inc.**(21) Appl. No.: **11/344,265**

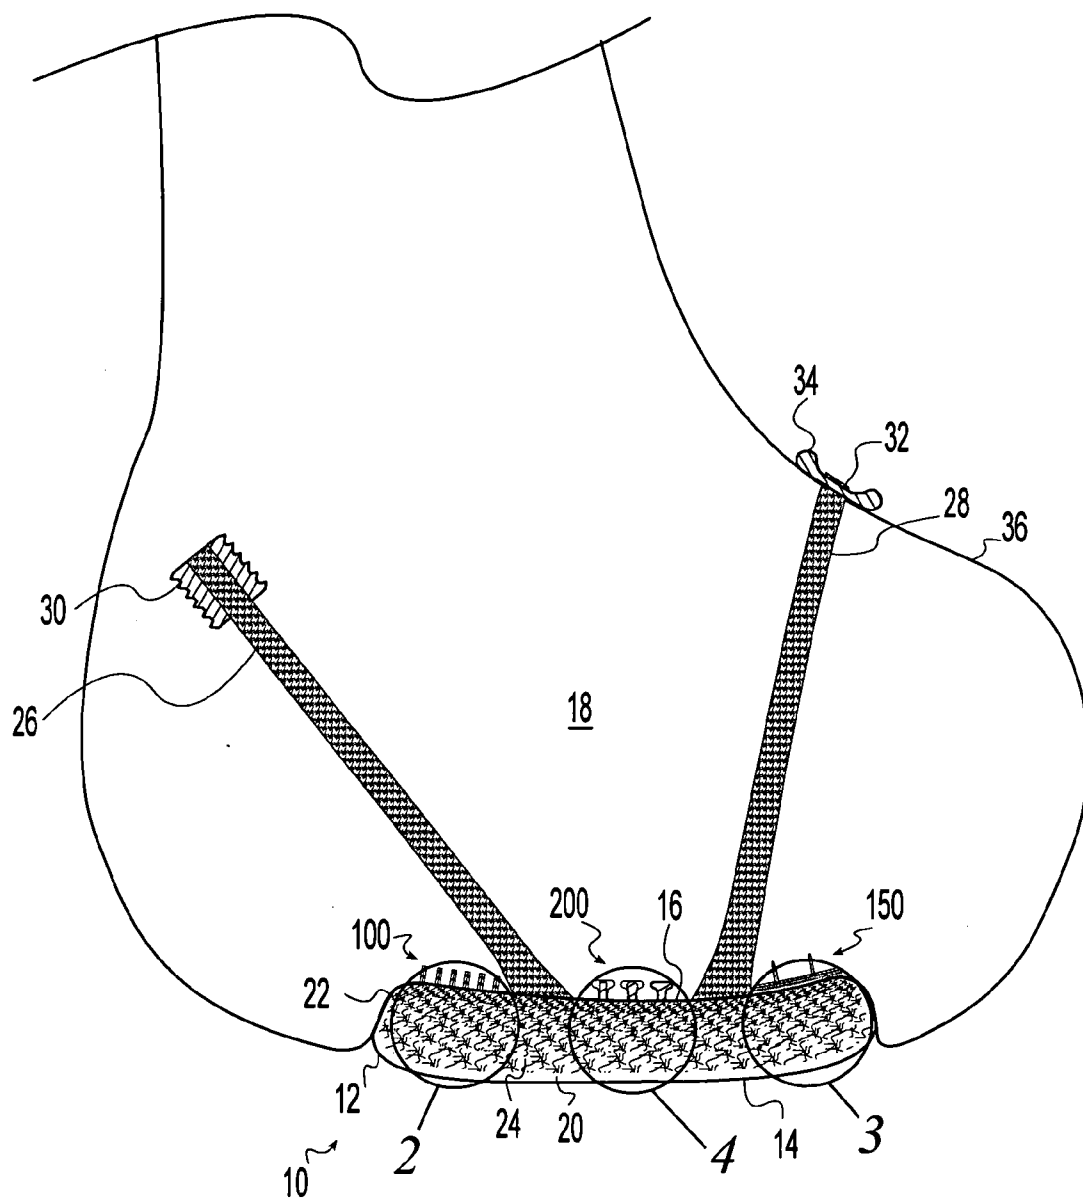


Fig. 1

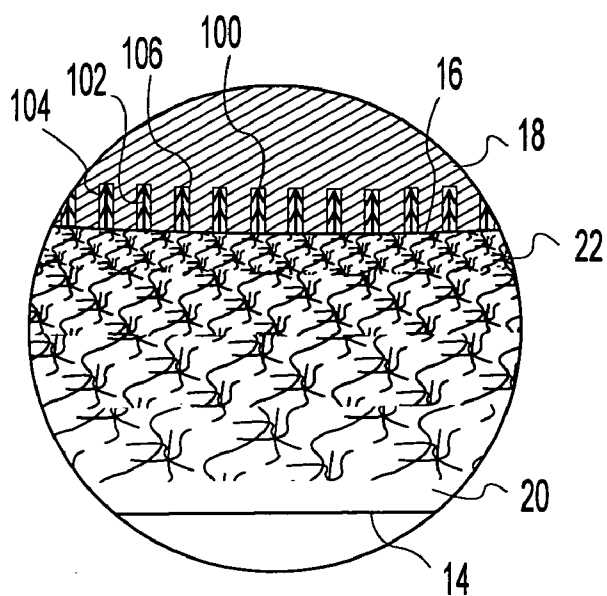


Fig. 2

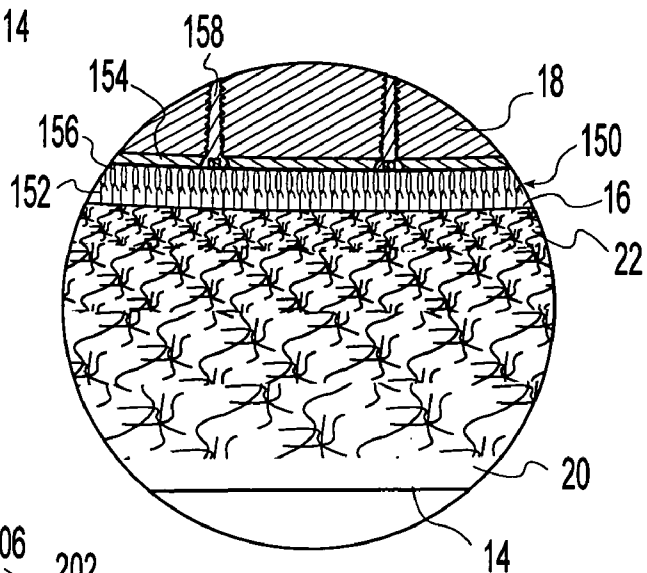


Fig. 3

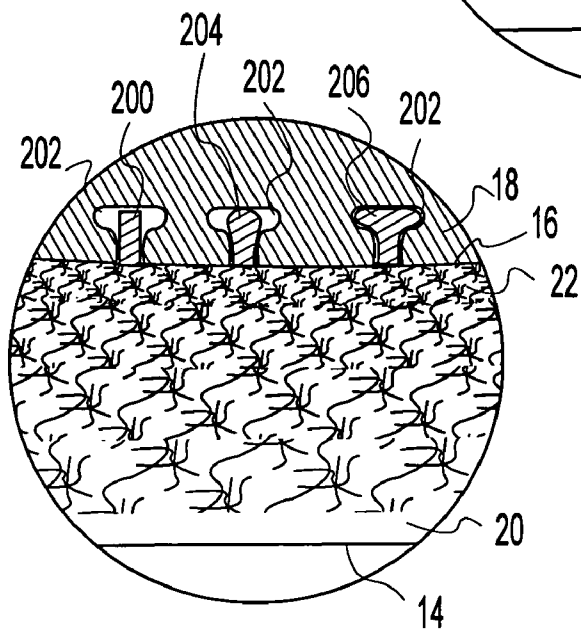


Fig. 4

CARTILAGE RESURFACING IMPLANT

FIELD OF THE INVENTION

[0001] The invention relates to implants for skeletal joints. In particular, the invention relates to implants for repairing cartilage defects in the articular surface of skeletal joints.

BACKGROUND

[0002] Degenerative and traumatic damage to the articular cartilage of skeletal joints can result in pain and restricted motion. Prosthetic joint replacement surgery is frequently utilized to alleviate the pain and restore joint function. During this surgery, one or more of the articulating surfaces of the joint are replaced with prosthetic bearing components. The replacement components typically include a portion for anchoring the implant adjacent to the joint and a portion for articulating with opposing joint surfaces. For example, during knee replacement surgery, an incision is made into the knee joint to expose the joint. Portions of the articular surfaces of the tibia and femur are removed and artificial joint components are positioned to replace the removed portions. In a total knee replacement, all of the articulating compartments of the joint are replaced with prosthetic components. However, often only one compartment of the knee joint, typically the medial compartment, is impaired. In a unicondylar knee replacement, only the damaged compartment is repaired with prosthetic bearing components. In an even less invasive approach, where the damage is limited to isolated defects in the articular cartilage, it has been proposed to replace just the articular cartilage in the immediate vicinity of the defect.

SUMMARY

[0003] The present invention provides a cartilage resurfacing implant for replacing cartilage of an articulating portion of a bone at a skeletal joint having opposed joint surfaces. The cartilage resurfacing implant includes a body having a bearing surface and a bone interface. The bearing surface is able to support articulation with an opposing joint surface.

[0004] In one aspect of the invention, the implant includes a flexible body.

[0005] In another aspect of the invention, the implant includes a plurality of reinforcing fibers embedded in the body and extending from the bone interface to define a bone attachment.

[0006] In another aspect of the invention, the implant includes a plurality of reinforcing fibers embedded in the body and extending from the bone interface to define flexible cables securable to the bone.

[0007] In another aspect of the invention, the implant includes a plurality of reinforcing fibers embedded in the body and extending from the bone interface to define slender bristles distributed across the bone interface able to spread the fixation load evenly over the bone interface.

[0008] In another aspect of the invention, the implant includes a plurality of reinforcing fibers embedded in the body and extending from the bone interface to define one component of a hook-and-loop fastener arrangement.

[0009] In another aspect of the invention, the implant includes a plurality of expandable pegs projecting from the bone interface.

BRIEF DESCRIPTION OF THE DRAWINGS

[0010] Various examples of the present invention will be discussed with reference to the appended drawings. These drawings depict only illustrative examples of the invention and are not to be considered limiting of its scope.

[0011] FIG. 1 is a side sectional view of an articulating bone end repaired with an illustrative cartilage resurfacing implant according to the present invention;

[0012] FIG. 2 is a detailed view of the cartilage resurfacing implant of FIG. 1;

[0013] FIG. 3 is a detailed view of the cartilage resurfacing implant of FIG. 1; and

[0014] FIG. 4 is a detailed view of the cartilage resurfacing implant of FIG. 1.

DESCRIPTION OF THE ILLUSTRATIVE EXAMPLES

[0015] Embodiments of a cartilage resurfacing implant include a body having a bearing surface and a bone interface. The implant may function as a replacement for damaged or diseased cartilage of a skeletal joint to sustain continued joint function. The implant may be used to replace a portion of any skeletal joint including, but not limited to, joints of the hip, knee, shoulder, spine, elbow, wrist, ankle, jaw, and digits. The implant may be configured to replace a relatively small defect within the joint, an entire compartment of the joint, or the total joint.

[0016] The bearing surface may be made of any material suitable for articulation with natural or prosthetic opposing bearing surfaces. Preferably the bearing material is resilient to facilitate intraoperative flexing, cutting, and/or otherwise shaping of the bearing surface to fit a surgical site. The bearing surface may include polyolefins, polyesters, polyimides, polyamides, polyacrylates, polyketones, and/or other suitable materials. For example the bearing surface may include ultrahigh molecular weight polyethylene. The bearing surface may include a hydrogel having a three dimensional network of polymer chains with water filling the void space between the macromolecules. The hydrogel may include a water soluble polymer that is crosslinked to prevent its dissolution in water. The water content of the hydrogel may range from 20-80%. The high water content of the hydrogel results in a low coefficient of friction for the bearing due to hydrodynamic lubrication. Advantageously, as loads increase on the bearing component, the friction coefficient decreases as water forced from the hydrogel forms a lubricating film. The hydrogel may include natural or synthetic polymers. Examples of natural polymers include polyhyaluronic acid, alginate, polypeptide, collagen, elastin, polylactic acid, polyglycolic acid, chitin, and/or other suitable natural polymers and combinations thereof. Examples of synthetic polymers include polyethylene oxide, polyethylene glycol, polyvinyl alcohol, polyacrylic acid, polyacrylamide, poly(N-vinyl-2-pyrrolidone, polyurethane, polyacrylonitrile, and/or other suitable synthetic polymers and combinations thereof.

[0017] The bone interface provides an anchor for the implant. The bone interface may be defined by a unitary body or by a substrate embedded in the body. A substrate may be solid or porous. The bearing surface may attach to the substrate by bonding, mechanical fasteners, porous interdigitation, and/or other suitable attachment methods. For example, the substrate may include an open porous structure in which a portion of the bearing surface is integrated to attach the bearing surface to the substrate. The substrate may be configured to be cemented in place, to be press-fit in place, to receive tissue ingrowth, and/or to be anchored to tissue in any other suitable tissue anchoring configuration. For example, the substrate may include an open porous structure for placement adjacent to body tissue to receive tissue ingrowth to anchor the implant adjacent the tissue. A porous structure may be configured to promote hard and/or soft tissue ingrowth. The porous structures may be in form of an open cell foam, a woven structure, a grid, agglomerated particles, and/or other suitable structures and combinations thereof.

[0018] The substrate may include any suitable material including, but not limited to, metals, polymers, ceramics, hydrogels and/or other suitable materials and combinations thereof. For example, a polymer substrate may include resorbable and/or non-resorbable polymers. Examples of resorbable polymers include polylactic acid polymers, polyglycolic acid polymers, and/or other suitable resorbable polymers. Examples of non-resorbable polymers include polyolefins, polyesters, polyimides, polyamides, polyacrylates, polyketones, and/or other suitable non-resorbable polymers. A metal substrate may include titanium, tantalum, stainless steel, and/or other suitable metals and alloys thereof. Preferably the substrate is relatively rigid to provide a suitable surface for hard tissue ingrowth. For example, the substrate may include a porous tantalum material having a structure similar to that of natural trabecular bone. Such a material is described in U.S. Pat. No. 5,282,861 entitled "Open Cell Tantalum Structures For Cancellous Bone Implants And Cell And Tissue Receptors". The material is fabricated by vapor depositing tantalum into a porous matrix. The substrate may include protruding pegs or other bone engaging features to further enhance the connection of the substrate to tissue.

[0019] The cartilage resurfacing implant may have a relatively high stiffness near a bone interface to enhance fixation of the implant to the rigid bone surface and a relatively low stiffness near the bearing surface to provide a compliant surface able to move with surrounding natural cartilage tissue. The implant may include a stiffness gradient from relatively high near the bone interface to relatively low near the bearing surface to gradually distribute stresses from the articulating surface to the bone interface and improve its delamination resistance. The cartilage resurfacing implant may include a unitary porous body. The body may include a separate porous substrate joined to the bearing surface. The implant may include a graded porosity that varies from relatively low porosity and high stiffness near the bone interface to relatively high porosity and low stiffness near the bearing surface. For example, a substrate, or a unitary body, may include a porous metal having relatively small pores near the bone interface and relatively large pores toward the bearing surface. Alternatively the substrate, or unitary body, may have uniform or randomly sized pores that vary in the number of pores, or pore density, such that

there is a relatively low pore density and high stiffness near the bone interface and a relatively high pore density and low stiffness toward the bearing surface.

[0020] The cartilage resurfacing implant may include a crosslinked polymer structure that has higher crosslinking and stiffness near the bone interface and relatively low crosslinking and stiffness near the articular surface. For example, the implant may include a hydrogel that varies from highly crosslinked to lightly crosslinked to define a stiffness gradient.

[0021] The cartilage resurfacing implant may include fibrous reinforcement within the implant body that includes a relatively high percentage of fiber reinforcement near the bone interface to increase the strength and stiffness near the bone and a relatively low percentage of fiber reinforcement near the bearing surface. The fiber reinforcement may have a varying composition from relatively strong fibers near the bone interface to relatively less strong fibers near the articular surface. For example, metal fibers near the bone interface may transition to high strength polymer fibers away from the bone interface to hydrogel fibers at the bearing surface. A unitary porous metal layer may be included for immediate contact with the bone. The reinforcing fibers may project away from the bone interface toward the bone to form fibrous anchors. For example, fibers imbedded in the implant may extend from the back of the implant to form cables for securing the implant to a bone. The cables may be secured in tunnels in the bone or extend to an outer surface of the bone. The cables may be secured with screws, pins, clips, clamps, buttons and/or other fixation members.

[0022] In another example, fibers imbedded in the implant may extend from the back of the implant to form slender bristles distributed across the bone interface. For example, the bristles may be distributed to spread the fixation load evenly over the bone interface. This is especially helpful where the implant is flexible to conform to the shape of the bone at the bone interface as it provides many fixation points to stabilize the flexible implant. For example, the bristles may be distributed in any suitable number from 1-100 per square inch of bone interface. Preferably the bristles number 4-20 per square inch. Even more preferably the bristles number 9-16 per square inch. The bristles may have any cross-sectional shape and size but are preferably generally cylindrical and have diameters in the range of 0.010-0.125 inches. More preferably the bristles have diameters in the range of 0.020-0.070 inches and still more preferably the bristles have diameters in the range of 0.030-0.050 inches. The bristles may be pressed directly into the bone to attach the implant to the bone. Alternatively, the bristles may be pressed into predrilled holes. The bristles may have a roughened or projecting surface to enhance their grip on the bone. For example, the bristles may be abrasive grit blasted, plasma sprayed, barbed, and/or otherwise roughened. The bristles may be porous to enhance their grip on the bone by bone ingrowth into pores. For example, the bristles may include porous metals, ceramics, polymers, and/or other suitable porous materials. For example, the bristles may include porous tantalum having a structure similar to natural trabecular bone.

[0023] In another example, fibers imbedded in the implant may extend from the back of the implant to form one component of a hook and loop fastener arrangement. For

example, the fibers may form hooks and/or loops on the back of the implant. A mating component may be pre-attached to the bone. For example, a mounting base including hooks and/or loops may be installed on the bone and the implant pressed against the mounting base to join the implant to the bone. The mounting base may be attached to the bone with adhesives, screws, staples, and/or other suitable fastening methods. For example, the mounting base may be in the form of a thin, flexible layer of loops attached to the bone with screws and hooks may project from the bone interface of the implant to engage the loops.

[0024] In another example, one or more pegs may extend from the back of the implant to engage one or more holes formed in the bone. The pegs may include expandable pegs. For example, expandable pegs may include heat expandable, fluid expandable, and/or otherwise expandable pegs that expand after insertion into the bone. The pegs may expand in width or diameter to grip the bone. The pegs may expand by deploying barbs to grip the bone. For example, partially or fully dehydrated hydrogel pegs may extend from the back of the implant. As the pegs absorb fluid from the surgical site and surrounding tissues, the pegs may expand to fill the holes and grip the bone. As the pegs press against the walls of the holes they form a strong frictional engagement. The pegs may also deform to positively engage the natural porosity of the bone in the walls of the holes. The positive engagement may be further enhanced by forming the holes with a larger diameter inside the bone than at the hole entrance. The hydrogel pegs may expand to at least partially take on the shape of the hole and thus form a positive engagement with the bone. For example, the bone holes may be undercut with a small entry diameter and a larger diameter deeper into the bone. The pegs may deploy barbs upon fluid expansion. In another example, the pegs may include a heat activated expansion mechanism. For example, the pegs may include a shape memory alloy that deploys barbs in the presence of heat from the patient's body. For example, the pegs and/or barbs may be made of shape memory alloy that transforms from a first shape prior to insertion to a second, deployed shape, after exposure to patient body temperature. The pegs may be fiber reinforced to enhance their tensile strength. For example, fibers from the implant may extend into the pegs.

[0025] The cables, bristles, hook and loop fasteners, and/or expanding pegs may be formed integrally with the implant or as separate elements subsequently attached to the implant.

[0026] The bearing surface may be formed by casting, injection molding, compression molding, machining, and/or other suitable forming processes and combinations thereof. For example, the bearing surface may be compression or injection molded into a porous substrate such that the bearing surface interdigitates with the substrate and is thereby joined to it.

[0027] The attachment of the cartilage resurfacing implant to the bone may be enhanced by the use of adhesives including fibrin glue, cyanoacrylate, epoxy, bone cement, and/or other suitable adhesives introduced at the bone interface. The attachment of the cartilage resurfacing implant to the bone may be enhanced by the use of bone growth inducing and/or conducting substances including bone paste, bone chips, bone growth proteins, bone growth peptides,

bone marrow aspirate, stem cells, bone attachment proteins, bone attachment peptides, and/or other suitable bone growth promoting substances introduced at the bone interface.

[0028] The cartilage resurfacing implant may be provided in a variety of sizes and shapes to facilitate its use in repairing differently sized and shaped cartilage defects. Alternatively, the implant may be provided in a generic form that may be intraoperatively cut to the desired shape and size.

[0029] The drawing shows an illustrative cartilage resurfacing implant **10** according to the present invention. The illustrative implant **10** is shown in use to resurface a portion of a femoral articulating surface at a knee joint. However, it is within the scope of the invention for the cartilage resurfacing implant **10** to be configured to replace any amount of any bearing surface in any skeletal joint. The implant **10** includes a body **12** having a bearing surface **14** engageable with an opposing joint surface for joint articulation. The implant **10** includes a bone interface **16** engageable with the bone **18**. The illustrative implant **10** includes a fiber reinforced hydrogel structure having a fiber free region **20** adjacent to the bearing surface **14** and a highly fiber reinforced region **22** adjacent to the bone interface **16**. The fibers **24** are distributed in a gradient of increasing fiber density from relatively less dense near the bearing surface **14** to relatively more dense near the bone interface **16**. The implant **10** is produced by embedding a fibrous preform into the hydrogel during formation of the hydrogel.

[0030] The implant **10** forms several attachments to the bone **18**. A pair of cables **26**, **28** extends from the bone interface **16** into the bone **18** to form localized connections to the bone. The cables **26**, **28** preferably are formed from fibers that interdigitate into the implant body **12** and form a portion of the fibrous reinforcement of the body **12**. One of the cables **26** is anchored to the bone **18** by a screw **30** threadably engaged with and embedded in the bone. The other cable **28** is anchored to the bone **18** by suspending an eyelet **32** formed in the end of the cable over a button **34** disposed against the cortical surface **36** of the bone **18**. The bone interface **16** of the implant **10** includes distributed fixation to more uniformly distribute the dislocation forces over the bone interface **16**. The distributed fixation includes a portion including bristles **100** embedded in the bone **18**, another portion including a hook and loop fastener **150**, and another portion including expanding pegs **200** embedded in the bone. The cables **26**, **28**, bristles **100**, hook and loop fastener **150**, and pegs **200** may each be used singly as the only form of fixation for the implant **10** to the bone **18** or in any combination of fasteners.

[0031] The bristles **100** are shown in more detail in FIG. 2. In the illustrative implant **10**, the bristles **100** project from the bone interface **16**. Each bristle **100** includes a main shaft **102** and barbs **104** extending outwardly from the main shaft **102**. The bristles are pressed into holes **106** drilled in the bone **18** and the barbs **104** grip the sides of the holes **106**. In the illustrative implant **10**, the bristles **100** are extensions of stiff fibers embedded in the implant body **12**.

[0032] The hook and loop fastener **150** is shown in more detail in FIG. 3. In the illustrative implant **10**, hooks **152** project from the bone interface **16** and are formed as extensions of stiff fibers embedded in the implant body **12**. A mounting base **154** includes loops **156** engageable with

the hooks. Bone screws **158** extend through the mounting base **154** and into the bone **18** to secure the mounting base **154** to the bone **18**.

[0033] The pegs **200** are shown in more detail in FIG. 4. In the illustrative implant **10**, each peg **200** is formed as a fiber reinforced extension of the fiber reinforced hydrogel body **12** of the implant **10**. The pegs **200** are molded as an integral part of the body **12**. The pegs **200** are inserted into holes **202** formed in the bone **18**. In the illustrative example, each hole **202** is undercut to have a larger diameter inside the bone **18** than at the surface of the bone **18**. As the pegs **200** absorb fluid from the surgical site, the hydrogel swells causing the pegs **200** to fill at least a portion of the hole **202** and lock the implant **10** in place on the bone **18**. One of the pegs **204** in FIG. 4 is shown expanded to partly fill a hole **202**. This is illustrative of a peg **204** that is in the process of expanding or one that has limited expansion potential due to the nature of its hydrogel composition and/or expansion restraint introduced by fiber reinforcement of the peg **204**. Another of the pegs **206** in FIG. 4 is shown fully expanded to fill the undercut hole **202**.

[0034] In a cartilage resurfacing surgical procedure, a cartilage defect is identified on the articular surface of a bone. The defect may be relatively small and affect only a small area of the articular surface or the defect may be relatively large, or there may be a large number of defects, and affect the entire articular surface. The damaged portion of the articular surface is removed by abrading, cutting, scraping, drilling, and/or any other suitable process. A cartilage resurfacing implant **10** is selected to fit the prepared site. The implant **10** may be provided in a form that is cut or otherwise reformed intraoperatively to fit the prepared site. Fixation holes are formed in the bone, if necessary, and the implant **10** is applied to the prepared site.

[0035] Although examples of a cartilage resurfacing implant and its use have been described and illustrated in detail, it is to be understood that the same is intended by way of illustration and example only and is not to be taken by way of limitation. The invention has been illustrated in use to replace a portion of a damaged femoral articular surface at a knee joint. However, the cartilage resurfacing implant may be configured to replace any amount of any articular surface at any skeletal joint. Accordingly, variations in and modifications to the cartilage resurfacing implant and its use will be apparent to those of ordinary skill in the art, and the following claims are intended to cover all such modifications and equivalents.

What is claimed is:

1. A cartilage resurfacing implant for replacing articular cartilage of an articulating portion of a bone at a skeletal joint having articulating opposed joint surfaces, the cartilage resurfacing implant comprising:

a flexible body having a bearing surface and a bone interface, the bearing surface being able to support articulation with an opposing joint surface, the body being sufficiently flexible to conform to the shape of the bone in vivo.

2. The cartilage resurfacing implant of claim 1 wherein the body is flexibly deformable in response to normal joint articulation to conform to the opposed joint surfaces.

3. The cartilage resurfacing implant of claim 1 further comprising a plurality of reinforcing fibers embedded in the

body, the reinforcing fibers extending from the bone interface to define a bone attachment.

4. The cartilage resurfacing implant of claim 3 wherein the body has a relatively higher stiffness near the bone interface and a relatively lower stiffness near the bearing surface.

5. The cartilage resurfacing implant of claim 4 wherein the body defines a stiffness gradient varying from relatively high near the bone interface to relatively low near the bearing surface.

6. The cartilage resurfacing implant of claim 5 wherein the body comprises a porous substrate defining a pore gradient varying from relatively small pores near the bone interface to relatively large pores near the bearing surface.

7. The cartilage resurfacing implant of claim 5 wherein the body comprises a porous substrate that varies from a relatively low pore density near the bone interface to a relatively high pore density near the bearing surface.

8. The cartilage resurfacing implant of claim 5 wherein the body comprises a crosslinked polymer structure that varies from more highly crosslinked near the bone interface to less highly crosslinked near the articular surface.

9. The cartilage resurfacing implant of claim 8 wherein the body comprises a crosslinked hydrogel.

10. The cartilage resurfacing implant of claim 3 wherein the body comprises a hydrogel.

11. The cartilage resurfacing implant of claim 5 wherein the reinforcing fibers comprise a percentage of the body composition that varies from a relatively high percentage of fiber reinforcement near the bone interface to a relatively low percentage of fiber reinforcement near the bearing surface.

12. The cartilage resurfacing implant of claim 5 wherein the reinforcing fibers comprise differing strengths of fibers that vary from relatively strong fibers near the bone interface to relatively less strong fibers near the articular surface.

13. The cartilage resurfacing implant of claim 12 wherein the body comprises metal fibers near the bone interface, high strength polymer fibers between the bone interface and bearing surface, and hydrogel fibers near the bearing surface.

14. The cartilage resurfacing implant of claim 3 wherein fibers extend from the bone interface to define flexible cables securable to the bone.

15. The cartilage resurfacing implant of claim 3 wherein fibers extend from the bone interface to define slender bristles distributed across the bone interface able to spread the fixation load evenly over the bone interface.

16. The cartilage resurfacing implant of claim 15 wherein the bristles comprise a main shaft and barbs extending outwardly from the main shaft to engage the bone.

17. The cartilage resurfacing implant of claim 3 wherein fibers extend from the bone interface to define one component of a hook-and-loop fastener arrangement.

18. The cartilage resurfacing implant of claim 17 wherein the fibers define hooks, the cartilage resurfacing implant further comprising a separate loop component able to be pre-installed on the bone and defining loops engageable with the hooks.

19. The cartilage resurfacing implant of claim 3 wherein the bone attachment comprises expandable pegs projecting from the bone interface.

20. The cartilage resurfacing implant of claim 19 wherein the pegs comprise an at least partially dehydrated hydrogel expandable by contact with body fluids.

21. The cartilage resurfacing implant of claim 19 wherein the pegs comprise heat expandable pegs.

22. The cartilage resurfacing implant of claim 3 further comprising an adhesive selected from the group consisting of fibrin glue, cyanoacrylate, epoxy, and bone cement.

23. The cartilage resurfacing implant of claim 3 further comprising a bone growth substance selected from the group consisting of bone paste, bone chips, bone growth proteins, bone growth peptides, bone marrow aspirate, stem cells, bone attachment proteins, and bone attachment peptides.

24. The cartilage resurfacing implant of claim 1 further comprising a set of similarly constructed bodies varying in size and shape selectable to repair differently sized and shaped cartilage defects.

25. The cartilage resurfacing implant of claim 1 wherein the body is intraoperatively shapable to a desired shape and size.

26. A cartilage resurfacing implant for replacing articular cartilage of an articulating portion of a bone at a skeletal joint having articulating opposed joint surfaces, the cartilage resurfacing implant comprising:

a body having a bearing surface and a bone interface, the bearing surface being able to support articulation with an opposing joint surface; and

a plurality of reinforcing fibers embedded in the body, the reinforcing fibers extending from the bone interface to define flexible cables securable to the bone.

27. A cartilage resurfacing implant for replacing articular cartilage of an articulating portion of a bone at a skeletal joint having articulating opposed joint surfaces, the cartilage resurfacing implant comprising:

a body having a bearing surface and a bone interface, the bearing surface being able to support articulation with an opposing joint surface; and

a plurality of reinforcing fibers embedded in the body, the reinforcing fibers extending from the bone interface to define slender bristles distributed across the bone interface able to spread the fixation load evenly over the bone interface.

28. The cartilage resurfacing implant of claim 27 wherein the bristles comprise a main shaft and barbs extending outwardly from the main shaft to engage the bone.

29. A cartilage resurfacing implant for replacing articular cartilage of an articulating portion of a bone at a skeletal joint having articulating opposed joint surfaces, the cartilage resurfacing implant comprising:

a body having a bearing surface and a bone interface, the bearing surface being able to support articulation with an opposing joint surface; and

a plurality of reinforcing fibers embedded in the body, the reinforcing fibers extending from the bone interface to define one component of a hook-and-loop fastener arrangement.

30. The cartilage resurfacing implant of claim 29 wherein the fibers define hooks, the cartilage resurfacing implant further defining a separate loop component able to be pre-installed on the bone and defining loops engageable with the hooks.

31. A cartilage resurfacing implant for replacing articular cartilage of an articulating portion of a bone at a skeletal joint having articulating opposed joint surfaces, the cartilage resurfacing implant comprising:

a body having a bearing surface and a bone interface, the bearing surface being able to support articulation with an opposing joint surface; and

a plurality of expandable pegs projecting from the bone interface, the pegs expandable in response to implantation adjacent to the bone.

32. The cartilage resurfacing implant of claim 31 wherein the pegs comprise fluid expandable pegs.

33. The cartilage resurfacing implant of claim 32 wherein the pegs comprise an at least partially dehydrated hydrogel expandable by contact with body fluids.

34. The cartilage resurfacing implant of claim 33 wherein reinforcing fibers from the body extend into the pegs.

35. The cartilage resurfacing implant of claim 31 wherein the pegs comprise expanding barbs.

36. The cartilage resurfacing implant of claim 31 wherein the pegs comprise heat expandable pegs.

37. The cartilage resurfacing implant of claim 31 wherein the pegs comprise a shape memory alloy.

* * * * *