

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
27 March 2003 (27.03.2003)

PCT

(10) International Publication Number
WO 03/024349 A1

(51) International Patent Classification⁷: A61B 18/18

(21) International Application Number: PCT/US02/28488

(22) International Filing Date:
5 September 2002 (05.09.2002)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
09/947,658 5 September 2001 (05.09.2001) US
60/356,390 12 February 2002 (12.02.2002) US
60/368,177 27 March 2002 (27.03.2002) US

(63) Related by continuation (CON) or continuation-in-part (CIP) to earlier applications:

US	09/947,658 (CIP)
Filed on	5 September 2001 (05.09.2001)
US	60/356,390 (CIP)
Filed on	12 February 2002 (12.02.2002)
US	60/368,177 (CIP)
Filed on	27 March 2002 (27.03.2002)

(71) Applicant (for all designated States except US): TIS-SUELINK MEDICAL, INC. [US/US]; Suite 400, One Washington Center, Dover, NH 03820 (US).

(72) Inventors; and


(75) Inventors/Applicants (for US only): MCCLURKEN, Michael, E. [US/US]; 26 Deer Meadow Road, Durham, NH 03824 (US). LIPSON, David [US/US]; 131 Pheasant Brook Road, North Andover, MA 01845 (US). LUZZI, Robert [US/US]; 4 Cragmere Heights Road, Exeter, NH 03833 (US). OYOLA, Arnold, E. [US/US]; 49 Nottingham Road, Raymond, NH 03077 (US). WILSON, Jonathan, E. [US/US]; 8 Carpenter Street, Amesbury, MA 01913 (US). MAURER, Christopher, W. [US/US]; 500 Broadway #2154, Malden, MA 02148 (US). GREELEY, Roger, D. [US/US]; 126 Spring Street, Portsmouth, NH 03801 (US).

(74) Agent: BRUESS, Steven, C.; Merchant & Gould P.C., P.O. Box 2903, Minneapolis, MN 55402-0903 (US).

(81) Designated States (national): AE, AG, AL, AM, AT (utility model), AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA,

[Continued on next page]

(54) Title: FLUID-ASSISTED MEDICAL DEVICES, SYSTEMS AND METHODS

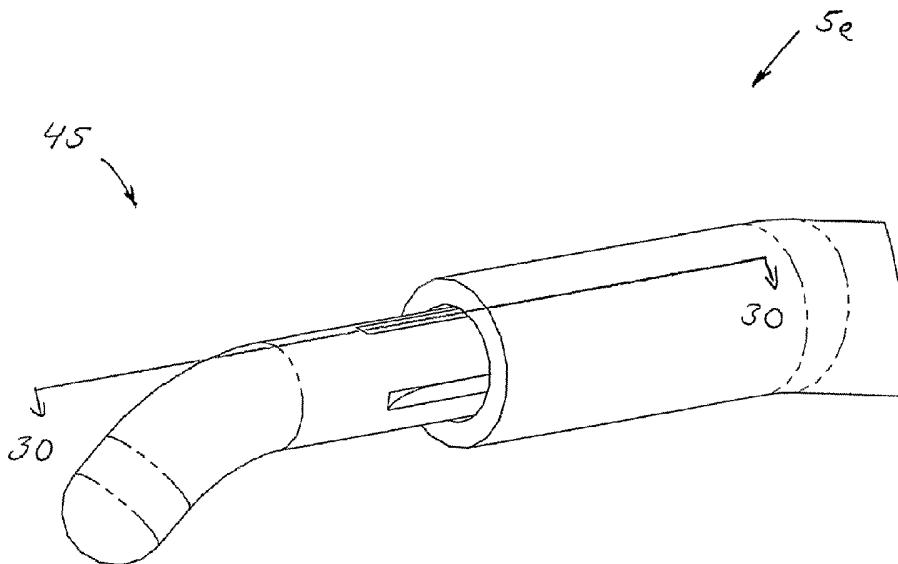

WO 03/024349 A1

(57) Abstract: Surgical devices, systems and methods for treating tissue are provided. Also provided are systems for treating tissue and methods of treating tissue. An exemplary surgical device comprises a handle (20a) having a proximal end and a distal end; a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end; an electrode tip (45), at least a portion of the electrode tip extending distally beyond the distal end of the shaft, the electrode tip extending distally beyond the distal end of the shaft comprising a spherical end surface portion (25) and a cylindrical side surface portion, the spherical end surface portion located distal to the cylindrical side surface portion and comprising at least a portion of the distal end surface of the surgical device; and a fluid passage directed to provide a fluid towards the cylindrical side portion of the electrode tip.



CH, CN, CO, CR, CU, CZ (utility model), CZ, DE (utility model), DE, DK (utility model), DK, DM, DZ, EC, EE (utility model), EE, ES, FI (utility model), FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SI, SK (utility model), SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),

European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

FLUID-ASSISTED MEDICAL DEVICES, SYSTEMS AND METHODS

This application is being filed as a PCT International Patent application in the name of TissueLink Medical, Inc. (a U.S. national corporation), for the 5 designation of all countries except the US, and Michael E. McClurken, David Lipson, Robert Luzzi, Arnold E. Oyola, Jonathan E. Wilson, Christopher W. Maurer, and Roger D. Greeley (all US citizens), for the designation of the United States only, on 5 September 2002.

10

Cross Reference to Related Applications

This patent application is related to United States Patent Application Serial Nos. 60/356,390, filed February 12, 2002, and 60/368,177, filed March 27, 2002, both now pending. This patent application is also related to United States Patent Application Serial No. 09/947,658, filed September 5, 2001, now pending, which is 15 a continuation-in-part of United States Patent Application Serial No. 09/797,049, filed March 1, 2001, now pending, which is a continuation of United States Patent Application Serial No. 60/187,114, filed March 6, 2000. This patent application is also related to United States Patent Application Serial No. 09/668,403, filed 20 September 22, 2000, now pending. This patent application incorporates the entire disclosure of each patent application herein by reference to the extent they are consistent.

Field

This invention relates generally to the field of medical devices, systems and 25 methods for use upon a body during surgery. More particularly, the invention relates to electrosurgical devices, systems and methods for use upon tissues of a human body during surgery, particularly open surgery and minimally invasive surgery such as laparoscopic surgery.

30

Background

Electrosurgical devices configured for use with a dry tip use electrical energy, most commonly radio frequency (RF) energy, to cut tissue or to cauterize blood vessels. During use, a voltage gradient is created at the tip of the device, thereby inducing current flow and related heat generation in the tissue. With sufficiently 35 high levels of electrical energy, the heat generated is sufficient to cut the tissue and, advantageously, to stop the bleeding from severed blood vessels.

Current dry tip electrosurgical devices can cause the temperature of tissue being treated to rise significantly higher than 100 °C, resulting in tissue desiccation,

tissue sticking to the electrodes, tissue perforation, char formation and smoke generation. Peak tissue temperatures as a result of RF treatment of target tissue can be as high as 320 °C, and such high temperatures can be transmitted to adjacent tissue via thermal diffusion. Undesirable results of such transmission to adjacent 5 tissue include unintended thermal damage to the tissue.

Using saline according to the present invention to couple RF electrical energy to tissue inhibits such undesirable effects as sticking, desiccation, smoke production and char formation. One key factor is inhibiting tissue desiccation, which occurs when tissue temperature exceeds 100 °C and all of the intracellular water boils 10 away, leaving the tissue extremely dry and much less electrically conductive. However, an uncontrolled or abundant flow rate of saline can provide too much cooling at the electrode/tissue interface. This cooling reduces the temperature of the target tissue being treated, and the rate at which tissue thermal coagulation occurs is determined by tissue temperature. This, in turn, can result in longer treatment time 15 to achieve the desired tissue temperature for treatment of the tissue. Long treatment times are undesirable for surgeons since it is in the best interest of the patient, physician and hospital, to perform surgical procedures as quickly as possible.

RF energy delivered to tissue can be unpredictable and often not optimal when using general-purpose generators. Most general-purpose RF generators have 20 modes for different waveforms (e.g. cut, coagulation, or a blend of these two) and device types (e.g. monopolar, bipolar), as well as power levels that can be set in watts. However, once these settings are chosen, the actual power delivered to tissue and associated heat generated can vary dramatically over time as tissue impedance changes over the course of RF treatment. This is because the power delivered by 25 most generators is a function of tissue impedance, with the power ramping down as impedance either decreases toward zero or increases significantly to several thousand ohms. Current dry tip electrosurgical devices are not configured to address a change in power provided by the generator as tissue impedance changes or the associated effect on tissue and rely on the surgeon's expertise to overcome this 30 limitation.

Summary of the Invention

In certain embodiments, a system for treating tissue is provided. The system comprises radio frequency power provided from a power source at a power level; an 35 electrically conductive fluid provided from a fluid source at a fluid flow rate; and an electrosurgical device configured to provide the radio frequency power and the electrically conductive fluid to the tissue.

In certain embodiments the conductive fluid is an indicator of tissue temperature. The conductive fluid can relate the tissue temperature to boiling, an amount of boiling, or an onset of boiling of the conductive fluid.

The conductive fluid can cool the tissue or dissipate heat from the tissue.

5 Alternately or additionally, the conductive fluid dissipates heat from at least one of the tissue and the conductive fluid by a boiling of at least a portion of the fluid.

For other embodiments, at least one of the radio frequency power level and the flow rate of the conductive fluid is used to effect a boiling of the electrically conductive fluid. Furthermore, in some embodiments, the effect on boiling may 10 comprise at least one of initiating, increasing, decreasing and eliminating boiling of the electrically conductive fluid.

For other embodiments, the electrically conductive fluid functions to limit the temperature of the tissue at the tissue surface to about a boiling temperature of the electrically conductive fluid.

15 Generally, the electrically conductive fluid protects the tissue from desiccation. In some embodiments, the conductive fluid protects the tissue from desiccation by boiling at least a portion of the electrically conductive fluid. In other embodiments, the electrically conductive fluid protects the tissue from desiccation by boiling at least a portion of the conductive fluid at a temperature below the 20 temperature of tissue desiccation.

For some embodiments, the electrically conductive fluid is provided to the tissue at the tissue surface and the radio frequency power is also provided to the tissue at the tissue surface. The radio frequency power reaches below the tissue surface into the tissue via (through) the electrically conductive fluid at the tissue 25 surface.

At least one of the radio frequency power level and the conductive fluid flow rate can be adjusted based on a boiling of the conductive fluid. Furthermore, for other embodiments, adjusting at least one of the radio frequency power level and the conductive fluid flow rate based on a boiling of the conductive fluid comprises one 30 of initiating, increasing, decreasing and eliminating boiling of the electrically conductive fluid.

In certain embodiments, a method for treating tissue is provided comprising providing radio frequency power at a power level; providing an electrically conductive fluid at a fluid flow rate; and providing an electrosurgical device 35 configured to provide the radio frequency power with the electrically conductive fluid to the tissue.

Still further, a system for treating tissue is provided, the system comprising radio frequency power provided from a power source at a power level; an

electrically conductive fluid provided from a fluid source at a fluid flow rate; an electrosurgical device configured to provide the radio frequency power and the conductive fluid to the tissue; and a fluid coupling which couples the tissue and the electrosurgical device, the coupling comprising the conductive fluid.

5 In certain embodiments the fluid coupling is an indicator of tissue temperature. The fluid coupling can function as an indicator of tissue temperature by using boiling; an amount of boiling; or an onset of boiling of the fluid coupling.

For other embodiments, the fluid coupling cools the tissue or dissipates heat from the tissue. The fluid coupling can dissipate heat from at least one of the tissue 10 and the fluid coupling by a boiling of at least a portion of the fluid coupling. For other embodiments, the fluid coupling can limit the temperature of the tissue at the tissue surface to close to a boiling temperature of the fluid coupling.

The fluid coupling can protect the tissue from desiccation. In some 15 embodiments, the fluid coupling protects the tissue from desiccation by boiling at least a portion of the fluid coupling. In other embodiments, the fluid coupling protects the tissue from desiccation by boiling at least a portion of the fluid coupling at a temperature which protects the tissue from desiccation.

For other embodiments, at least one of the radio frequency power level and the conductive fluid flow rate is used to effect a boiling of the fluid coupling. 20 Furthermore, in some embodiments, the effect on boiling may be at least one of initiating, increasing, decreasing and eliminating boiling of the fluid coupling.

The conductive fluid can be provided to the tissue at the tissue surface, and the radio frequency power can also be provided to the tissue at the tissue surface. The radio frequency power can be provided to an area below the tissue surface via 25 (through) the fluid coupling at the tissue surface.

In certain embodiments, a method for treating tissue is provided, the method comprising providing radio frequency power at a power level; providing an electrically conductive fluid at a fluid flow rate; providing an electrosurgical device configured to provide the radio frequency power and the electrically conductive 30 fluid to the tissue; and forming a fluid coupling which couples the tissue and the electrosurgical device. The fluid coupling comprises conductive fluid.

The fluid coupling can be used as an indicator of tissue temperature. This can be done by boiling; an amount of boiling of the fluid coupling; or an onset of boiling of the fluid coupling.

35 For some embodiments, the fluid coupling is used to cool the tissue or dissipate heat from the tissue by transferring heat to the fluid coupling. The fluid coupling can dissipate heat from at least one of the tissue and the fluid coupling by a boiling of at least a portion of the fluid coupling.

For other embodiments, at least one of the radio frequency power level and the conductive fluid flow rate is adjusted based on a boiling of the fluid coupling. Furthermore, for other embodiments, adjusting at least one of the radio frequency power level and the conductive fluid flow rate based on a boiling of the fluid

5 coupling comprises one of initiating, increasing, decreasing and eliminating boiling of the fluid coupling.

For other embodiments, the temperature of the tissue at the tissue surface is limited to about a boiling temperature of the fluid coupling.

10 For other embodiments, the tissue is protected from desiccation with the fluid coupling. Furthermore, for other embodiments, the tissue is protected from desiccation with the fluid coupling by a boiling of at least a portion of the fluid coupling. Furthermore, for other embodiments, the tissue is protected from desiccation with the fluid coupling by a boiling of at least a portion of the fluid coupling at a temperature which protects the tissue from desiccation.

15 The method for treating tissue can further comprise providing the conductive fluid to the tissue at the tissue surface; and providing the radio frequency power to the tissue at the tissue surface and below the tissue surface into the tissue through the fluid coupling.

With regards to specific devices, in certain embodiments a surgical device
20 for treating tissue is provided comprising a handle having a proximal end and a distal end; a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end; an electrode tip, at least a portion of the electrode tip extending distally beyond the distal end of the shaft, the electrode tip extending distally beyond the distal end of the shaft comprising a spherical end
25 surface portion and a cylindrical side surface portion, the spherical end surface portion located distal to the cylindrical side surface portion and comprising at least a portion of the distal end surface of the surgical device; and a fluid passage directed to provide a fluid towards the cylindrical side portion of the electrode tip.

In other embodiments, a surgical device for treating tissue is provided
30 comprising a handle having a proximal end and a distal end; a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end; an electrode tip, at least a portion of the electrode tip extending distally beyond the distal end of the shaft, the electrode tip extending distally beyond the distal end of the shaft comprising a neck portion and an enlarged head portion, the
35 enlarged head portion located distal to the neck portion and comprising at least a portion of a distal end surface of the surgical device; and a fluid passage directed to provide a fluid towards the enlarged head portion of the electrode tip.

In still other embodiments, a device for treating tissue is provided comprising a handle having a proximal end and a distal end; a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end; an electrode tip, the electrode tip comprising a spherical end surface portion and a cylindrical side surface portion, the spherical end surface portion located distal to the cylindrical side surface portion and comprising at least a portion of the distal end surface of the device; a fluid passage connectable to a fluid source; and a plurality of fluid outlet openings in fluid communication with the fluid passage, the fluid outlet openings positioned to provide a fluid from the fluid source around the cylindrical side surface portion of the electrode tip.

In still other embodiments, a device for treating tissue is provided comprising a handle having a proximal end and a distal end; a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end; an electrode tip comprising a rounded distal end surface portion configured to blunt dissect tissue and a side surface portion configured to seal tissue from at least one of the flow of bodily fluids and air, the side surface portion having a surface area greater than the surface area of the distal end surface portion; a fluid passage connectable to a fluid source; and at least one fluid outlet opening in fluid communication with the fluid passage, the fluid outlet opening positioned to provide a fluid from the fluid source to the side surface portion of the electrode tip and proximal the distal end surface portion.

In other embodiments, a device for treating tissue is provided comprising a first electrode tip spaced from a second electrode tip, the first and second electrode tips being connectable to different terminals of a radio frequency generator to generate electrical current flow therebetween; at least one fluid passage connectable to a fluid source; at least one fluid outlet opening in fluid communication with the fluid passage, the fluid outlet opening configured to provide a fluid from the fluid source to at least one of a tissue surface and at least one of the first and second electrode tips; and the first and second electrode tips configured to slide over and seal tissue in the presence of a fluid provided from the fluid outlet opening and an electrical current provided from the electrode tips.

Additional methods for treating tissue may also comprise providing tissue having a tissue surface; providing radio frequency power at a power level; providing an electrically conductive fluid at a fluid flow rate; providing an surgical device configured to simultaneously provide the radio frequency power and the electrically conductive fluid to tissue; providing the electrically conductive fluid to the tissue at the tissue surface; forming a fluid coupling comprising the electrically conductive fluid which couples the tissue and the surgical device; providing the radio frequency

power to the tissue at the tissue surface and below the tissue surface into the tissue through the fluid coupling; sealing the tissue against at least one of the flow of bodily fluids and air by at least one of shrinking collagen and coagulating blood in the tissue; and blunt dissecting the tissue.

5 In other embodiments, methods for treating tissue may also comprise providing tissue having a tissue surface; providing radio frequency power at a power level; providing an electrically conductive fluid at a fluid flow rate; providing an surgical device configured to simultaneously provide the radio frequency power and the electrically conductive fluid to tissue, the surgical device comprising a first 10 electrode tip and a second electrode tip; providing the electrically conductive fluid to the tissue at the tissue surface; forming a fluid coupling comprising the electrically conductive fluid which couples the tissue and the surgical device; providing the radio frequency power to the tissue at the tissue surface and below the tissue surface into the tissue through the fluid coupling; sliding the first electrode tip and the 15 second electrode tip over the tissue surface; and sealing the tissue against at least one of the flow of bodily fluids and air by at least one of shrinking collagen and coagulating blood in the tissue.

Brief Description Of The Drawings

20 To better understand and appreciate the invention, refer to the following detailed description in connection with the accompanying drawings, hand and computer generated:

25 FIG. 1 is a block diagram showing one embodiment of a control system of the invention, and an electrosurgical device;

30 FIG. 2 is a schematic graph that describes the relationship between RF power to tissue (P), flow rate of saline (Q), and tissue temperature (T) when heat conduction to adjacent tissue is considered;

35 FIG. 3 is schematic graph that describes the relationship between RF power to tissue (P), flow rate of saline (Q), and tissue temperature (T) when heat conduction to adjacent tissue is neglected;

40 FIG. 4 is a schematic graph that describes the relationship between RF power to tissue (P), flow rate of saline (Q), and tissue temperature (T) when the heat required to warm the tissue to the peak temperature (T) 68 is considered;

45 FIG. 5 is a graph showing the relationship of percentage saline boiling and saline flow rate (cc/min) for an exemplary RF generator output of 75 watts;

50 FIG. 6 is a schematic graph that describes the relationship of load impedance (Z, in ohms) and generator output power (P, in watts), for an exemplary generator output of 75 watts in a bipolar mode;

FIG. 7 is a schematic graph that describes the relationship of time (t, in seconds) and tissue impedance (Z, in ohms) after RF activation;

FIG. 8 is a schematic perspective view of a cannula which may be used with an electrosurgical device according to the present invention;

5 FIG. 9 is a schematic exploded perspective view of an assembly of an electrosurgical device according to the present invention;

FIG. 10 is a schematic longitudinal cross-sectional side view of the tip and shaft of the device of FIG. 9 taken along line 10-10 of FIG. 12;

10 FIG. 11 is a schematic close-up longitudinal cross-sectional side view of the tip portion of the device bounded by circle 45 shown in FIG. 10 taken along line 10-10 of FIG. 12;

FIG. 12 is a schematic distal end view of the tip portion of the device bounded by circle 45 shown in FIG. 10;

15 FIG. 13 is a schematic side view of the tip and shaft of the device of FIG. 9 with a fluid coupling to a tissue surface of tissue;

FIG. 14 is a schematic close-up cross-sectional side view of an alternative tip portion;

FIG. 15 is a schematic close-up section side view of the tip portion of FIG. 14 taken along line 15-15 of FIG. 14;

20 FIG. 16 is a schematic close-up cross-sectional side view of the tip portion of FIG. 14 disposed in a tissue crevice;

FIG. 17 is a schematic graph of impedance Z versus time t showing changes in impedance represented by impedance spikes;

FIG. 18 is a schematic graph of the impedance Z versus boiling of fluid %;

25 FIG. 19 is schematic close-up cross-sectional view of the sleeve taken along line 19-19 of FIG. 15;

FIG. 20 is a schematic close-up perspective view of an alternative tip portion;

30 FIG. 21 is a schematic close-up section side view of the tip portion of FIG. 20 taken along line 21-21 of FIG. 20;

FIG. 22 is a schematic close-up cross-sectional side view of the tip portion of FIG. 20 disposed in a tissue crevice;

FIG. 23 is a schematic close-up front perspective view of the electrode for the tip portion of FIG. 20;

35 FIG. 24 is a schematic close-up rear perspective view of the electrode for the tip portion of FIG. 20;

FIG. 25 is a schematic close up cross-sectional view of a porous electrode with recesses;

FIG. 26 is schematic close up cross-sectional view of an electrode with semi-circular recesses;

FIG. 27 is schematic close up cross-sectional view of an electrode with V-shaped recesses;

5 FIG. 28 is schematic close up cross-sectional view of an electrode with U-shaped recesses;

FIG. 29 is a schematic close-up perspective view of an alternative tip portion;

10 FIG. 30 is a schematic close-up section side view of the tip portion of FIG. 29 taken along line 30-30 of FIG. 29;

FIG. 31 is a schematic close-up front perspective view of the electrode for the tip portion of FIG. 29;

FIG. 32 is a schematic close-up rear perspective view of the electrode for the tip portion of FIG. 29;

15 FIG. 33 is a schematic close-up perspective view of an alternative tip portion;

FIG. 34 is a schematic close-up section side view of the tip portion of FIG. 33 taken along line 34-34 of FIG. 33;

20 FIG. 35 is a schematic close-up front perspective view of the electrode for the tip portion of FIG. 33;

FIG. 36 is a schematic close-up rear perspective view of the electrode for the tip portion of FIG. 33;

FIG. 37 is a schematic close-up perspective view of an alternative tip portion;

25 FIG. 38 is a schematic close-up section side view of the tip portion of FIG. 37 taken along line 38-38 of FIG. 37;

FIG. 39 is a schematic close-up perspective view of an alternative tip portion;

30 FIG. 40 is a schematic close-up section side view of the tip portion of FIG. 39 taken along line 40-40 of FIG. 39;

FIG. 41 is a schematic close-up front posterior perspective view of the electrode for the tip portion of FIG. 39;

FIG. 42 is a schematic close-up front anterior perspective view of the electrode for the tip portion of FIG. 39;

35 FIG. 43 is a schematic side view of the tip portion of FIG. 39 with a fluid coupling to a tissue surface of tissue;

FIG. 44 is a schematic front view of the tip portion of FIG. 39 with a fluid coupling to a tissue surface of tissue;

FIG. 45 is a schematic side view of the tip portion of FIG. 39 with a fluid coupling to a tissue surface of tissue;

FIG. 46 is a schematic exploded perspective view of an assembly of an alternative electrosurgical device according to the present invention;

5 FIG. 47 is a schematic close-up cross-sectional side view of the tip portions of FIG. 46 assembled with a fluid coupling to a tissue surface of tissue;

FIG. 48 is a schematic close-up cross-sectional side view of the tip portions of FIG. 46 assembled with an alternative fluid coupling to a tissue surface of tissue;

10 FIG. 49 is a schematic exploded perspective view of an assembly of an alternative electrosurgical device according to the present invention;

FIG. 50 is a schematic close-up cross-sectional side view of the tip portions of FIG. 49 assembled with a fluid coupling to a tissue surface of tissue;

FIG. 51 is a schematic exploded perspective view of an assembly of an alternative electrosurgical device according to the present invention;

15 FIG. 52 is a schematic close-up perspective side view of a distal end portion of the device of FIG. 51;

FIG. 53 is a schematic close-up cross-sectional side view of a distal end portion of the device of FIG. 51 assembled with a fluid coupling to a tissue surface of tissue;

20 FIG. 54 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

FIG. 55 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

25 FIG. 56 is a schematic close-up perspective view of the arms of the device of FIG. 55;

FIG. 57 is a schematic close-up perspective view of a distal end portion of the device of FIG. 55;

FIG. 58 is a schematic close-up perspective view of a distal end portion of the device of FIG. 55;

30 FIG. 59 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

FIG. 60 is a schematic close-up perspective view of the arms of the device of FIG. 59;

35 FIG. 61 is a schematic close-up perspective view of a distal end portion of the device of FIG. 59;

FIG. 62 is a schematic close-up perspective view of a distal end portion of the device of FIG. 59;

FIG. 63 is a schematic close-up perspective view of a distal end portion of an alternative electrosurgical device according to the present invention;

FIG. 64 is a schematic close-up perspective view of a distal end portion of the device of FIG. 63 with tissue;

5 FIG. 65 is a schematic close-up perspective view of the arms of an alternative electrosurgical device according to the present invention;

FIG. 66 is a schematic close-up perspective view of a distal end portion of the arms of the device of FIG. 65 with the collar removed;

10 FIG. 67 is a schematic close-up perspective view of a distal end portion of the device of FIG. 65;

FIG. 68 is a schematic close-up perspective view of a distal end portion of the device of FIG. 65 with one arm removed;

15 FIG. 69 is a schematic close-up perspective view of the collar of the device of FIG. 65;

FIG. 70 is a schematic close-up perspective view of a distal end portion of an alternative electrosurgical device according to the present invention;

FIG. 71 is a schematic close-up perspective view of a distal end portion of one of the arms of the device of FIG. 70;

20 FIG. 72 is a schematic close-up perspective view of a distal end portion of an alternative electrosurgical device according to the present invention;

FIG. 73 is a schematic close-up side view of a distal end portion of the device of FIG. 72;

25 FIG. 74 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

FIG. 75 is a schematic perspective view of a handle portion of the device of FIG. 74 assembled with various components;

FIG. 76 is a schematic close-up side view of a portion of the assembly of FIG. 75;

30 FIG. 77 is a schematic close-up side view of a portion of the assembly of FIG. 75;

FIG. 78 is a schematic partial cross-sectional front perspective view of the electrical connections for the device of FIG. 74;

FIG. 79 is schematic partial cross-sectional rear perspective view of the electrical connections for the device of FIG. 74;

35 FIG. 80 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

FIG. 81 is a schematic side view of a handle portion of the device of FIG. 80 assembled with various components;

FIG. 82 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

FIG. 83 is a schematic perspective view of a handle portion of the device of FIG. 82 assembled with various components;

5 FIG. 84 is a schematic side view of a handle portion of the device of FIG. 82 assembled with various components;

FIG. 85 is a schematic side view of a handle portion of the device of FIG. 82 assembled with various components;

10 FIG. 86 is a schematic side view of a handle portion of the device of FIG. 82 assembled with various components;

FIG. 87 is a schematic perspective view of an alternative electrosurgical device according to the present invention;

FIG. 88 is a schematic perspective view of a handle portion of the device of FIG. 87;

15

FIG. 89 is a schematic side view of a handle portion of the device of FIG. 87;

FIG. 90 is a schematic perspective view of a handle portion an alternative electrosurgical device according to the present invention; and

FIG. 91 is a schematic side view of the handle portion of FIG. 90.

20 FIG. 92 is a schematic perspective view of a handle portion an alternative electrosurgical device according to the present invention; and

FIG. 93 is a schematic side view of the handle portion of FIG. 92.

Detailed Description

25 Throughout the present description, like reference numerals and letters indicate corresponding structure throughout the several views, and such corresponding structure need not be separately discussed. Furthermore, any particular feature(s) of a particular exemplary embodiment may be equally applied to any other exemplary embodiment(s) of this specification as suitable. In other 30 words, features between the various exemplary embodiments described herein are interchangeable as suitable, and not exclusive.

The invention provides devices, systems and methods that preferably improve control of tissue temperature at a tissue treatment site during a medical procedure. The invention is particularly useful during surgical procedures upon 35 tissues of the body, where it is desirable to coagulate and shrink tissue, to occlude lumens of blood vessels (e.g. arteries, veins), airways (e.g. bronchi, bronchioles), bile ducts and lymphatic ducts.

The invention includes electrosurgical procedures, which preferably utilize RF power and electrically conductive fluid, to treat tissue. Preferably, a desired tissue temperature range is achieved by adjusting parameters, such as conductive fluid flow rate, that affect the temperature at the tissue/electrode interface.

5 Preferably, the device achieves a desired tissue temperature by utilizing a desired percentage boiling of the conductive solution at the tissue/electrode interface.

In one embodiment, the invention provides a control device, the device comprising a flow rate controller that receives a signal indicating power applied to the system, and adjusts the flow rate of conductive fluid from a fluid source to an 10 electrosurgical device. The invention also contemplates a control system comprising a flow rate controller, a measurement device that measures power applied to the system, and a pump that provides fluid at a selected flow rate.

The invention will be discussed generally with reference to FIG. 1. FIG. 1 shows a block diagram of one exemplary embodiment of a system of the invention. 15 Preferably, as shown in FIG. 1, an electrically conductive fluid 24 is provided from a fluid source 1 through a fluid line 2 to a pump 3, which has an outlet fluid line 4a that is connected as an input fluid line 4b, to electrosurgical device 5. In a preferred embodiment, the outlet fluid line 4a and the input fluid line 4b are flexible and are made from a polymeric material, such as polyvinylchloride (PVC) or polyolefin (e.g. 20 polypropylene, polyethylene) and the conductive fluid comprises a saline solution. More preferably, the saline comprises sterile, and even more preferably, normal saline. Although the description herein will specifically describe the use of saline as the fluid 24, other electrically conductive fluids, as well as non-conductive fluids, can be used in accordance with the invention.

25 For example, in addition to the conductive fluid comprising physiologic saline (also known as "normal" saline, isotonic saline or 0.9% sodium chloride (NaCl) solution), the conductive fluid may comprise hypertonic saline solution, hypotonic saline solution, Ringers solution (a physiologic solution of distilled water containing specified amounts of sodium chloride, calcium chloride, and potassium chloride), lactated Ringer's solution (a crystalloid electrolyte sterile solution of distilled water containing specified amounts of calcium chloride, potassium chloride, sodium chloride, and sodium lactate), Locke-Ringer's solution (a buffered isotonic solution of distilled water containing specified amounts of sodium chloride, potassium chloride, calcium chloride, sodium bicarbonate, magnesium chloride, and 30 dextrose), or any other electrolyte solution. In other words, a solution that conducts electricity via an electrolyte, a substance (salt, acid or base) that dissociates into electrically charged ions when dissolved in a solvent, such as water, resulting 35 solution comprising an ionic conductor.

While a conductive fluid is preferred, as will become more apparent with further reading of this specification, the fluid 24 may also comprise an electrically non-conductive fluid. The use of a non-conductive fluid is less preferred to that of a conductive fluid as the non-conductive fluid does not conduct electricity. However, 5 the use of a non-conductive fluid still provides certain advantages over the use of a dry electrode including, for example, reduced occurrence of tissue sticking to the electrode of the device 5 and cooling of the electrode and/or tissue. Therefore, it is also within the scope of the invention to include the use of a non-conducting fluid, such as, for example, dionized water.

10 Returning to FIG. 1, energy to heat tissue is provided from energy source, such as an electrical generator 6 which preferably provides RF alternating current energy via a cable 7 to energy source output measurement device, such as a power measurement device 8 that measures the RF alternating current electrical power. In one exemplary embodiment, preferably the power measurement device 8 does not 15 turn the power off or on, or alter the power in any way. A power switch 15 connected to the generator 6 is preferably provided by the generator manufacturer and is used to turn the generator 6 on and off. The power switch 15 can comprise any switch to turn the power on and off, and is commonly provided in the form of a footswitch or other easily operated switch, such as a switch 15a mounted on the 20 electrosurgical device 5. The power switch 15 or 15a may also function as a manually activated device for increasing or decreasing the rate of energy provided from the surgical device 5. Alternatively, internal circuitry and other components of the generator 6 may be used for automatically increasing or decreasing the rate of energy provided from the surgical device 5. A cable 9 preferably carries RF energy 25 from the power measurement device 8 to the electrosurgical device 5. Power, or any other energy source output, is preferably measured before it reaches the electrosurgical device 5.

30 For the situation where capacitance and induction effects are negligibly small, from Ohm's law, power **P**, or the rate of energy delivery (e.g. joules/sec), may be expressed by the product of current times voltage (i.e. $I \times V$), the current squared times resistance (i.e. $I^2 \times R$), or the voltage squared divided by the resistance (i.e. V^2/R); where the current **I** may be measured in amperes, the voltage **V** may be measured in volts, the electrical resistance **R** may be measured in ohms, and the power **P** may be measured in watts (joules/sec). Given that power **P** is a function of 35 current **I**, voltage **V**, and resistance **R** as indicated above, it should be understood, that a change in power **P** is reflective of a change in at least one of the input variables. Thus, one may alternatively measure changes in such input variables

themselves, rather than power **P** directly, with such changes in the input variables mathematically corresponding to a changes in power **P** as indicated above.

As to the frequency of the RF electrical energy, it is preferably provided within a frequency band (i.e. a continuous range of frequencies extending between 5 two limiting frequencies) in the range between and including about 9 kHz (kilohertz) to 300 GHz (gigahertz). More preferably, the RF energy is provided within a frequency band in the range between and including about 50 kHz (kilohertz) to 50 MHz (megahertz). Even more preferably, the RF energy is provided within a frequency band in the range between and including about 200 kHz (kilohertz) to 2 10 MHz (megahertz). Most preferably, RF energy is provided within a frequency band in the range between and including about 400 kHz (kilohertz) to 600 kHz (kilohertz). Further, it should also be understood that, for any frequency band identified above, the range of frequencies may be further narrowed in increments of 1 (one) hertz anywhere between the lower and upper limiting frequencies.

15 While RF electrical energy is preferred, it should be understood that the electrical energy (i.e., energy made available by the flow of electric charge, typically through a conductor or by self-propagating waves) may comprise any frequency of the electromagnetic spectrum (i.e. the entire range of radiation extending in frequency from 10^{23} hertz to 0 hertz) and including, but not limited to, gamma rays, 20 x-rays, ultraviolet radiation, visible light, infrared radiation, microwaves, and any combinations thereof.

With respect to the use of electrical energy, heating of the tissue is preferably performed by means of resistance heating. In other words, increasing the 25 temperature of the tissue as a result of electric current flow through the tissue, with the electrical energy being absorbed from the voltage and transformed into thermal energy (i.e. heat) via accelerated movement of ions as a function of the tissue's electrical resistance.

Heating with electrical energy may also be performed by means of dielectric heating (capacitance). In other words, increasing the temperature of the tissue 30 through the dissipation of electrical energy as a result of internal dielectric loss when the tissue is placed in a varying electric field, such as a high-frequency (e.g. microwave), alternating electromagnetic field. Dielectric loss is the electrical energy lost as heat in the polarization process in the presence of the applied electric field. In the case of an alternating current field, the energy is absorbed from the 35 alternating current voltage and converted to heat during the polarization of the molecules.

However, it should be understood that energy provided to heat the tissue may comprise surgical devices other than electrosurgical devices, energy sources other

than generators, energy forms other than electrical energy and mechanisms other than resistance heating. For example, providing thermal energy to the tissue from energy source with a difference (e.g. higher) in temperature. Such may be provided, for example, to the tissue from a heated device, which heats tissue through direct 5 contact with the energy source (conduction), heats through contact with a flowing fluid (convection), or from a remote heat source (radiation).

Also, for example, providing energy to the tissue may be provided via 10 mechanical energy which is transformed into thermal energy via accelerated movement of the molecules, such as by mechanical vibration provided, for example, by energy source such as a transducer containing a piezoelectric substance (e.g., a quartz-crystal oscillator) that converts high-frequency electric current into vibrating ultrasonic waves which may be used by, for example, an ultrasonic surgical device.

Also, for example, providing energy to the tissue may be provided via 15 radiant energy (i.e. energy which is transmitted by radiation/waves) which is transformed into thermal energy via absorption of the radiant energy by the tissue. Preferably the radiation/waves comprise electromagnetic radiation/waves which include, but is not limited to, radio waves, microwaves, infrared radiation, visible light radiation, ultraviolet radiation, x-rays and gamma rays. More preferably, such radiant energy comprises energy with a frequency of 3×10^{11} hertz to 3×10^{16} hertz 20 (i.e. the infrared, visible, and ultraviolet frequency bands of the electromagnetic spectrum). Also preferably the electromagnetic waves are coherent and the electromagnetic radiation is emitted from energy source such as a laser device.

A flow rate controller 11 preferably includes a selection switch 12 that can 25 be set to achieve desired levels of percentage fluid boiling (for example, 100%, 98%, 80% boiling). Preferably, the flow rate controller 11 receives an input signal 10 from the power measurement device 8 and calculates an appropriate 30 mathematically predetermined fluid flow rate based on percentage boiling indicated by the selection switch 12. In a preferred embodiment, a fluid switch 13 is provided so that the fluid system can be primed (e.g. air eliminated) before turning the generator 6 on. The output signal 16 of the flow rate controller 11 is preferably sent to the pump 3 motor to regulate the flow rate of conductive fluid, and thereby provide an appropriate fluid flow rate which corresponds to the amount of power being delivered.

In one exemplary embodiment, the invention comprises a flow rate controller 35 11 that is configured and arranged to be connected to a source of RF power (e.g. generator 6), and a source of fluid (e.g. fluid source 1), for example, a source of conductive fluid. The device of the invention receives information about the level of RF power applied to an electrosurgical device 5, and adjusts the flow rate of the

fluid 24 to the electrosurgical device 5, thereby controlling temperature at the tissue treatment site.

In another exemplary embodiment, elements of the system are physically included together in one electronic enclosure. One such embodiment is shown by 5 enclosure within the outline box 14 of FIG 1. In the illustrated embodiment, the pump 3, flow rate controller 11, and power measurement device 8 are enclosed within an enclosure, and these elements are connected through electrical connections to allow signal 10 to pass from the power measurement device 8 to the flow rate controller 11, and signal 16 to pass from the flow rate controller 11 to the pump 3. 10 Other elements of a system can also be included within one enclosure, depending upon such factors as the desired application of the system, and the requirements of the user.

The pump 3 can be any suitable pump used in surgical procedures to provide saline or other fluid at a desired flow rate. Preferably, the pump 3 comprises a 15 peristaltic pump. With a rotary peristaltic pump, typically a fluid 24 is conveyed within the confines of a flexible tube (e.g. 4a) by waves of contraction placed externally on the tube which are produced mechanically, typically by rotating rollers which squeeze the flexible tubing against a support intermittently. Alternatively, with a linear peristaltic pump, typically a fluid 24 is conveyed within the confines of 20 a flexible tube by waves of contraction placed externally on the tube which are produced mechanically, typically by a series of compression fingers or pads which squeeze the flexible tubing against a support sequentially. Peristaltic pumps are generally preferred for use as the electro-mechanical force mechanism (e.g. rollers driven by electric motor) does not make contact the fluid 24, thus reducing the 25 likelihood of inadvertent contamination.

Alternatively, pump 3 can be a "syringe pump", with a built-in fluid supply. With such a pump, typically a filled syringe is located on an electro-mechanical force mechanism (e.g. ram driven by electric motor) which acts on the plunger of the syringe to force delivery of the fluid 24 contained therein. Alternatively, the syringe 30 pump may comprise a double-acting syringe pump with two syringes such that they can draw saline from a reservoir (e.g. of fluid source 1), either simultaneously or intermittently. With a double acting syringe pump, the pumping mechanism is generally capable of both infusion and withdrawal. Typically, while fluid 24 is being expelled from one syringe, the other syringe is receiving fluid 24 therein from 35 a separate reservoir. In this manner, the delivery of fluid 24 remains continuous and uninterrupted as the syringes function in series. Alternatively, it should be understood that a multiple syringe pump with two syringes, or any number of syringes, may be used in accordance with the invention.

Furthermore, fluid 24, such as conductive fluid, can also be provided from an intravenous (IV) bag full of saline (e.g. of fluid source 1) that flows under the influence (i.e. force) of gravity. In such a manner, the fluid 24 may flow directly to the electrosurgical device 5, or first to the pump 3 located there between.

- 5 Alternatively, fluid 24 from a fluid source 1 such as an IV bag can be provided through an IV flow controller that may provide a desired flow rate by adjusting the cross sectional area of a flow orifice (e.g. lumen of the connective tubing with the electrosurgical device 5) while sensing the flow rate with a sensor such as an optical drop counter. Furthermore, fluid 24 from a fluid source 1 such as an IV bag can be
- 10 provided through a manually or automatically activated device such as a flow controller, such as a roller clamp, which also adjusts the cross sectional area of a flow orifice and may be adjusted manually by, for example, the user of the device in response to their visual observation (e.g. fluid boiling) at the tissue treatment site or a pump.
- 15 Similar pumps can be used in connection with the invention, and the illustrated embodiments are exemplary only. The precise configuration of the pump 3 is not critical to the invention. For example, pump 3 may include other types of infusion and withdrawal pumps. Furthermore, pump 3 may comprise pumps which may be categorized as piston pumps, rotary vane pumps (e.g. axial impeller, centrifugal impeller), cartridge pumps and diaphragm pumps. In some embodiments, the pump 3 can be substituted with any type of flow controller, such as a manual roller clamp used in conjunction with an IV bag, or combined with the flow controller to allow the user to control the flow rate of conductive fluid to the device. Alternatively, a valve configuration can be substituted for pump 3.
- 20 Furthermore, similar configurations of the system can be used in connection with the invention, and the illustrated embodiments are exemplary only. For example, the fluid source 1 pump 3, generator 6, power measurement device 8 or flow rate controller 11, or any other components of the system not expressly recited above, may comprise a portion of the electrosurgical device 5. For example, in one exemplary embodiment the fluid source 1 may comprise a compartment of the electrosurgical device 5 which contains fluid 24, as indicated at reference character 1a. In another exemplary embodiment, the compartment may be detachably connected to the electrosurgical device 5, such as a canister which may be attached via threaded engagement with the device 5. In yet another exemplary embodiment, the compartment may be configured to hold a pre-filled cartridge of fluid 24, rather than the fluid directly.
- 25
- 30
- 35

Also for example, with regards to alternative for the generator 6, an energy source, such as a direct current (DC) battery used in conjunction with inverter

5 circuitry and a transformer to produce alternating current at a particular frequency, may comprise a portion of the electrosurgical device 5, as indicated at reference character 6a. In one embodiment the battery element of the energy source may comprise a rechargeable battery. In yet another exemplary embodiment, the battery element may be detachably connected to the electrosurgical device 5, such as for recharging. The components of the system will now be described in further detail. From the specification, it should be clear that any use of the terms "distal" and "proximal" are made in reference from the user of the device, and not the patient.

10 The flow rate controller 11 controls the rate of flow from the fluid source 1. Preferably, the rate of fluid flow from the fluid source 1 is based upon the amount of RF power provided from the generator 6 to the electrosurgical device 5. In other words, as shown in FIG. 2, preferably there is a relationship between the rate of fluid flow **Q** and the RF power **P** indicated by the Y- and X-axes of the schematic graph, respectively. More precisely, as shown in FIG. 2, the relationship between the rate 15 of fluid flow **Q** and RF power **P** may be expressed as a direct, linear relationship. The flow rate **Q** of conductive fluid 24, such as saline, interacts with the RF power **P** and various modes of heat transfer away from the target tissue, as described herein.

20 Throughout this disclosure, when the terms "boiling point of saline", "vaporization point of saline", and variations thereof are used, what is actually referenced for explanation purposes, is the boiling point of the water (i.e. 100°C) in the saline solution given that the difference between the boiling point of normal saline (about 100.16°C) and the boiling point of water is negligible.

25 FIG. 2 shows a schematic graph that describes the relationship between the flow rate of saline, RF power to tissue, and regimes of boiling as detailed below. Based on a simple one-dimensional lumped parameter model of the heat transfer, the peak tissue temperature can be estimated, and once tissue temperature is estimated, it follows directly whether it is hot enough to boil saline. The total RF electrical power **P** that is converted into heat can be defined as:

$$30 \quad P = \Delta T/R + \rho c_p Q_l \Delta T + \rho Q_b h_v \quad (1)$$

where **P** = the total RF electrical power that is converted into heat.

35 Conduction. The term $[\Delta T/R]$ in equation (1) is heat conducted to adjacent tissue, represented as 70 in FIG. 2, where:

$\Delta T = (T - T_\infty)$ the difference in temperature between the peak tissue temperature (T) and the normal temperature (T_∞) of the body tissue (°C). Normal temperature of the body tissue is generally 37 °C; and

5 $R =$ Thermal resistance of surrounding tissue, the ratio of the temperature difference to the heat flow (°C/watt).

10 This thermal resistance can be estimated from published data gathered in experiments on human tissue (see for example, Phipps, J.H., "Thermometry studies with bipolar diathermy during hysterectomy," *Gynaecological Endoscopy*, 3:5-7 (1994)). As described by Phipps, Kleppinger bipolar forceps were used with an RF power of 50 watts, and the peak tissue temperature reached 320 °C. For example, using the energy balance of equation (1), and assuming all the RF heat put into tissue is conducted away, then R can be estimated:

15

$$R = \Delta T/P = (320-37)/50 = 5.7 \approx 6 \text{ °C/watt}$$

20 However, it is undesirable to allow the tissue temperature to reach 320 °C, since tissue will become desiccated. At a temperature of 320 °C, the fluid contained in the tissue is typically boiled away, resulting in the undesirable tissue effects described herein. Rather, it is preferred to keep the peak tissue temperature at no more than about 100 °C to inhibit desiccation of the tissue. Assuming that saline boils at about 100 °C, the first term in equation (1) ($\Delta T/R$) is equal to $(100 - 37)/6 = 10.5$ watts. Thus, based on this example, the maximum amount of heat conducted to adjacent tissue without any significant risk of tissue desiccation is 10.5 watts.

25 Referring to FIG. 2, RF power to tissue is represented on the X-axis as **P** (watts) and flow rate of saline (cc/min) is represented on the Y-axis as **Q**. When the flow rate of saline equals zero ($Q = 0$), there is an "offset" RF power that shifts the origin of the sloped lines **76**, **78**, and **80** to the right. This offset is the heat conducted to adjacent tissue. For example, using the calculation above for bipolar forceps, this offset RF power is about 10.5 watts. If the power is increased above this level with no saline flow, the peak tissue temperature can rise well above 100 °C, resulting in tissue desiccation from the boiling off of water in the cells of the tissue.

30 Convection. The second term $[\rho c_p Q_l \Delta T]$ in equation (1) is heat used to warm up the flow of saline without boiling the saline, represented as **72** in FIG. 2, where:

ρ = Density of the saline fluid that gets hot but does not boil (approximately 1.0 gm/cm³);
 c_p = Specific heat of the saline (approximately 4.1 watt-sec/gm-°C);
 Q_l = Flow rate of the saline that is heated (cm³/sec); and
5 ΔT = Temperature rise of the saline. Assuming that the saline is heated to body temperature before it gets to the electrode, and that the peak saline temperature is similar to the peak tissue temperature, this is the same ΔT as for the conduction calculation above.

10 The onset of boiling can be predicted using equation (1) with the last term on the right set to zero (no boiling) ($\rho Q_b h_v = 0$), and solving equation (1) for Q_l leads to:

$$Q_l = [P - \Delta T/R]/\rho c_p \Delta T \quad (2)$$

15 This equation defines the line shown in FIG. 2 as the line of onset of boiling
 76.

Boiling. The third term [$\rho Q_b h_v$] in equation (1) relates to heat that goes into converting the water in liquid saline to water vapor, and is represented as 74 in FIG. 2, where:

20 Q_b = Flow rate of saline that boils (cm³/sec); and
 h_v = Heat of vaporization of saline (approximately 2,000 watt-sec/gm).
 A flow rate of only 1 cc/min will absorb a significant amount of heat if it is
 25 completely boiled, or about $\rho Q_b h_v = (1) (1/60) (2,000) = 33.3$ watts. The heat
 needed to warm this flow rate from body temperature to 100 °C is much less, or
 $\rho c_p Q_l \Delta T = (1) (4.1) (1/60) (100 - 37) = 4.3$ watts. In other words, the most
 significant factor contributing to heat transfer from a wet electrode device can be
 fractional boiling. The present invention recognizes this fact and exploits it.

30 Fractional boiling can be described by equation (3) below:

$$Q_l = \frac{\{P - \Delta T/R\}}{\{\rho c_p \Delta T + \rho h_v Q_b / Q_l\}} \quad (3)$$

35 If the ratio of Q_b/Q_l is 0.50 this is the 50% boiling line 78 shown in FIG. 2.
 If the ratio is 1.0 this is the 100% boiling line 80 shown in FIG. 2.

As indicated previously in the specification, using a fluid to couple energy to tissue inhibits such undesirable effects as sticking, desiccation, smoke production and char formation, and that one key factor is inhibiting tissue desiccation, which

occur if the tissue temperature exceeds 100 °C and all the intracellular water boils away, leaving the tissue extremely dry and much less electrically conductive.

As shown in FIG. 2, one control strategy or mechanism which can be employed for the electrosurgical device 5 is to adjust the power **P** and flow rate **Q**

5 such that the power **P** used at a corresponding flow rate **Q** is equal to or less than the power **P** required to boil 100% of the fluid and does not exceed the power **P** required to boil 100% of the fluid. In other words, this control strategy targets using the electrosurgical device 5 in the regions of FIG. 2 identified as $T < 100$ °C and $T = 100$ °C, and includes the 100% boiling line 80. Stated another way, this control
10 strategy targets not using the electrosurgical device 5 only in the region of FIG. 2 identified as $T >> 100$ °C.

Another control strategy that can be used for the electrosurgical device 5 is to operate the device 5 in the region $T < 100$ °C, but at high enough temperature to shrink tissue containing Type I collagen (e.g., walls of blood vessels, bronchi, bile
15 ducts, etc.), which shrinks when exposed to about 85 °C for an exposure time of 0.01 seconds, or when exposed to about 65 °C for an exposure time of 15 minutes. An exemplary target temperature/time for tissue shrinkage is about 75 °C with an exposure time of about 1 second. As discussed herein, a determination of the high end of the scale (i.e., when the fluid reaches 100 °C) can be made by the phase
20 change in the fluid from liquid to vapor. However, a determination at the low end of the scale (e.g., when the fluid reaches, for example, 75 °C for 1 second) requires a different mechanism as the temperature of the fluid is below the boiling temperature and no such phase change is apparent. In order to determine when the fluid reaches a temperature that will facilitate tissue shrinkage, for example 75 °C, a
25 thermochromic material, such as a thermochromic dye (e.g., leuco dye), may be added to the fluid. The dye can be formulated to provide a first predetermined color to the fluid at temperatures below a threshold temperature, such as 75 °C, then, upon heating above 75 °C, the dye provides a second color, such as clear, thus turning the fluid clear (i.e. no color or reduction in color). This color change may be gradual,
30 incremental, or instant. Thus, a change in the color of the fluid, from a first color to a second color (or lack thereof) provides a visual indication to the user of the electrosurgical device 5 as to when a threshold fluid temperature below boiling has been achieved. Thermochromic dyes are available, for example, from Color Change Corporation, 1740 Cortland Court, Unit A, Addison, IL 60101.

35 It is also noted that the above mechanism (i.e., a change in the color of the fluid due to a dye) may also be used to detect when the fluid reaches a temperature which will facilitate tissue necrosis; this generally varies from about 60 °C for an exposure time of 0.01 seconds and decreasing to about 45 °C for an exposure time of

15 minutes. An exemplary target temperature/time for tissue necrosis is about 55 °C for an exposure time of about 1 second.

In order to reduce coagulation time, use of the electrosurgical device 5 in the region $T = 100$ °C of FIG. 2 is preferable to use of the electrosurgical device 5 in the 5 region $T < 100$ °C. Consequently, as shown in FIG. 2, another control strategy which may be employed for the electrosurgical device 5 is to adjust the power P and flow rate Q such that the power P used at a corresponding flow rate Q is equal to or more than the power P required to initiate boiling of the fluid, but still less than the power P required to boil 100% of the fluid. In other words, this control strategy 10 targets using the electrosurgical device 5 in the region of FIG. 2 identified as $T = 100$ °C, and includes the lines of the onset of boiling 76 and 100% boiling line 80. Stated another way, this control strategy targets use using the electrosurgical device 5 on or between the lines of the onset of boiling 76 and 100% boiling line 80, and 15 not using the electrosurgical device 5 in the regions of FIG. 2 identified as $T < 100$ °C and $T >> 100$ °C.

For consistent tissue effect, it is desirable to control the saline flow rate so that it is always on a “line of constant % boiling” as, for example, the line of the onset of boiling 76 or the 100% boiling line 80 or any line of constant % boiling located in between (e.g. 50% boiling line 78) as shown in FIG. 2. Consequently, 20 another control strategy that can be used for the electrosurgical device 5 is to adjust power P and flow rate Q such that the power P used at a corresponding flow rate Q targets a line of constant % boiling.

It should be noted, from the preceding equations, that the slope of any line of constant % boiling is known. For example, for the line of the onset of boiling 76, 25 the slope of the line is given by $(\rho c_p \Delta T)$, while the slope of the 100% boiling line 80 is given by $1/(\rho c_p \Delta T + \rho h_v)$. As for the 50% boiling line 78, for example, the slope is given by $1/(\rho c_p \Delta T + \rho h_v 0.5)$.

If, upon application of the electrosurgical device 5 to the tissue, boiling of the fluid is not detected, such indicates that the temperature is less than 100 °C as 30 indicated in the area of FIG. 2, and the flow rate Q must be decreased to initiate boiling. The flow rate Q may then decreased until boiling of the fluid is first detected, at which time the line of the onset of boiling 76 is transgressed and the point of transgression on the line 76 is determined. From the determination of a point on the line of the onset of boiling 76 for a particular power P and flow rate Q , 35 and the known slope of the line 76 as outlined above (i.e. $1/\rho c_p \Delta T$), it is also possible to determine the heat conducted to adjacent tissue 70.

Conversely, if upon application of the electrosurgical device 5 to the tissue, boiling of the fluid is detected, such indicates that the temperature is approximately

equal to 100 °C as indicated in the areas of FIG. 2, and the flow rate **Q** must be increased to reduce boiling until boiling stops, at which time the line of the onset of boiling 76 is transgressed and the point of transgression on the line 76 determined. As with above, from the determination of a point on the line of the onset of boiling 76 for a particular power **P** and flow rate **Q**, and the known slope of the line 76, it is also possible to determine the heat conducted to adjacent tissue 70.

With regards to the detection of boiling of the fluid, such may be physically detected by the user (e.g. visually by the naked eye) of the electrosurgical device 5 in the form of either bubbles or steam evolving from the fluid coupling at the 10 electrode/tissue interface. Alternatively, such a phase change (i.e. from liquid to vapor or vice-versa) may be measured by a sensor which preferably senses either an absolute change (e.g. existence or non-existence of boiling with binary response such as yes or no) or a change in a physical quantity or intensity and converts the change into a useful input signal for an information-gathering system. For example, 15 the phase change associated with the onset of boiling may be detected by a pressure sensor, such as a pressure transducer, located on the electrosurgical device 5. Alternatively, the phase change associated with the onset of boiling may be detected by a temperature sensor, such as a thermistor or thermocouple, located on the electrosurgical device 5, such as adjacent to the electrode. Also alternatively, the 20 phase change associated with the onset of boiling may be detected by a change in the electric properties of the fluid itself. For example, a change in the electrical resistance of the fluid may be detected by an ohm meter; a change in the amperage may be measured by an amp meter; a change in the voltage may be detected by a volt meter; and a change in the power may be determined by a power meter.

25 Yet another control strategy which may be employed for the electrosurgical device 5 is to eliminate the heat conduction term of equation (1) (i.e. $\Delta T/R$). Since the amount of heat conducted away to adjacent tissue can be difficult to precisely predict, as it may vary, for example, by tissue type, it may be preferable, from a control point of view, to assume the worst case situation of zero heat conduction, 30 and provide enough saline so that if necessary, all the RF power could be used to heat up and boil the saline, thus providing that the peak tissue temperature will not go over 100 °C a significant amount. This situation is shown in the schematic graph of FIG. 3.

35 Stated another way, if the heat conducted to adjacent tissue 70 is overestimated, the power **P** required to intersect the 100% boiling line 80 will, in turn, be overestimated and the 100% boiling line 80 will be transgressed into the $T >> 100$ °C region of FIG. 2, which is undesirable as established above. Thus, assuming the worse case situation of zero heat conduction provides a “safety factor”

to avoid transgressing the 100% boiling line **80**. Assuming heat conduction to adjacent tissue **70** to be zero also provides the advantage of eliminating the only term from equation (1) which is tissue dependent, i.e., depends on tissue type. Thus, provided ρ , c_p , ΔT , and h_v are known as indicated above, the equation of the line for any line of constant % boiling is known. Thus, for example, the 98% boiling line, 80% boiling line, etc. can be determined in response to a corresponding input from the selection switch **12**. In order to promote flexibility, it should be understood that the input from the selection switch preferably may comprise any percentage of boiling. Preferably the percentage of boiling may be selected in single percent increments (i.e. 100%, 99%, 98%, etc.).

Upon determination of the line of the onset of boiling **76**, the 100% boiling line **80** or any line of constant % boiling there between, it is generally desirable to control the flow rate **Q** so that it is always on a particular line of constant % boiling for consistent tissue effect. In such a situation, the flow rate controller **11** will adjust the flow rate **Q** of the fluid **24** to reflect changes in power **P** provided by the generator **6**, as discussed in greater detail below. For such a use the flow rate controller **11** may be set in a line of constant boiling mode, upon which the % boiling is then correspondingly selected.

As indicated above, it is desirable to control the saline flow rate **Q** so that it is always on a line of constant % boiling for consistent tissue effect. However, the preferred line of constant % boiling may vary based on the type of electrosurgical device **5**. For example, if with use of the device **5**, shunting through saline is not an issue, then it can be preferable to operate close to or directly on, but not over the line of the onset of boiling, such as **76a** in FIG. 3. This preferably keeps tissue as hot as possible without causing desiccation. Alternatively, if with use of the device **5** shunting of electrical energy (e.g. from one jaw to an opposing jaw of certain copulative bipolar devices) through excess saline is an issue, then it can be preferable to operate along a line of constant boiling, such as line **78a** in FIG. 3, the 50% line. This simple proportional control will have the flow rate determined by equation (4), where **K** is the proportionality constant:

$$Q_l = K \times P \quad (4)$$

In essence, when power **P** goes up, the flow rate **Q** will be proportionately increased. Conversely, when power **P** goes down, the flow rate **Q** will be proportionately decreased.

The proportionality constant **K** is primarily dependent on the fraction of saline that boils, as shown in equation (5), which is equation (3) solved for **K** after eliminating **P** using equation (4), and neglecting the conduction term ($\Delta T/R$):

$$5 \quad K = \frac{1}{\{\rho c_p \Delta T + \rho h_v Q_b / Q_l\}} \quad (5)$$

Thus, the present invention provides a method of controlling boiling of fluid, such as a conductive fluid, at the tissue/electrode interface. In a preferred embodiment, this provides a method of treating tissue without use of tissue sensors, 10 such as temperature or impedance sensors. Preferably, the invention can control boiling of conductive fluid at the tissue/electrode interface and thereby control tissue temperature without the use of feedback loops.

In describing the control strategy of the present invention described thus far, focus has been drawn to a steady state condition. However, the heat required to 15 warm the tissue to the peak temperature (**T**) may be incorporated into equation (1) as follows:

$$P = \Delta T/R + \rho c_p Q_l \Delta T + \rho Q_b h_v + \rho c_p V \Delta T / \Delta t \quad (6)$$

20 where $\rho c_p V \Delta T / \Delta t$ represents the heat required to warm the tissue to the peak temperature (**T**) **68** and where :

ρ = Density of the saline fluid that gets hot but does not boil (approximately 1.0 gm/cm³);
 25 c_p = Specific heat of the saline (approximately 4.1 watt-sec/gm-°C);
 V = Volume of treated tissue
 ΔT = ($T - T_\infty$) the difference in temperature between the peak tissue temperature (**T**) and the normal temperature (T_∞) of the body tissue (°C). Normal temperature of the body tissue is generally 37 °C; and
 30 Δt = ($t - t_\infty$) the difference in time to achieve peak tissue temperature (**T**) and the normal temperature (T_∞) of the body tissue (°C).

The inclusion of the heat required to warm the tissue to the peak temperature (**T**) in the control strategy is graphically represented at **68** in FIG. 4. With respect to 35 the control strategy, the effects of the heat required to warm the tissue to the peak temperature (**T**) **68** should be taken into account before flow rate **Q** adjustment being undertaken to detect the location of the line of onset of boiling **76**. In other words, the flow rate **Q** should not be decreased in response to a lack of boiling before at

least a quasi-steady state has been achieved as the location of the line of onset of boiling 76 will continue to move during the transitory period. Otherwise, if the flow rate Q is decreased during the transitory period, it may be possible to decrease the flow Q to a point past the line of onset of boiling 76 and continue past the 100% boiling line 80 which is undesirable. In other words, as temperature (T) is approached the heat 68 diminishes towards zero such that the lines of constant boiling shift to the left towards the Y-axis.

FIG. 5 is an exemplary graph of flow rate Q versus % boiling for a situation where the RF power P is 75 watts. The percent boiling % is represented on the X-axis, and the saline flow rate Q (cc/min) is represented on the Y-axis. According to this example, at 100 % boiling the most desirable predetermined saline flow rate Q is 2 cc/min. Also according to this example, flow rate Q versus % boiling at the remaining points of the graft illustrates a non-linear relationship as follows:

15 Table 1 – % Boiling and Flow Rate Q (cc/min) at RF Power P of 75 watts

	0%	17.4
	10%	9.8
	20%	6.8
	30%	5.2
20	40%	4.3
	50%	3.6
	60%	3.1
	70%	2.7
	80%	2.4
25	90%	2.2
	100%	2.0

Typical RF generators used in the field have a power selector switch to 300 watts of power, and on occasion some have been found to be selectable up to 400 watts of power. In conformance with the above methodology, at 0% boiling with a corresponding power of 300 watts, the calculated flow rate Q is 69.7 cc/min and with a corresponding power of 400 watts the calculated flow rate Q is 92.9 cc/min. Thus, when used with typical RF generators in the field, a fluid flow rate Q of about 100 cc/min or less with the present invention is expected to suffice for the vast majority of applications.

As discussed herein, RF energy delivery to tissue can be unpredictable and vary with time, even though the generator has been “set” to a fixed wattage. The schematic graph of FIG. 6 shows the general trends of the output curve of a typical

general-purpose generator, with the output power changing as load (tissue plus cables) impedance Z changes. Load impedance Z (in ohms) is represented on the X-axis, and generator output power P (in watts) is represented on the Y-axis. In the illustrated embodiment, the electrosurgical power (RF) is set to 75 watts in a bipolar mode. As shown in the figure, the power will remain constant as it was set as long as the impedance Z stays between two cut-offs, low and high, of impedance, that is, for example, between 50 ohms and 300 ohms in the illustrated embodiment. Below load impedance Z of 50 ohms, the power P will decrease, as shown by the low impedance ramp **28a**. Above load impedance Z of 300 ohms, the power P will decrease, as shown by the high impedance ramp **28b**. Of particular interest to saline-enhanced electrosurgery is the low impedance cut-off (low impedance ramp **28a**), where power starts to ramp down as impedance Z drops further. This change in output is invisible to the user of the generator and not evident when the generator is in use, such as in an operating room.

15 FIG. 7 shows the general trend of how tissue impedance generally changes with time for saline-enhanced electrosurgery. As tissue heats up, the temperature coefficient of the tissue and saline in the cells is such that the tissue impedance decreases until a steady-state temperature is reached upon which time the impedance remains constant. Thus, as tissue heats up, the load impedance Z decreases, 20 potentially approaching the impedance Z cut-off of 50 ohms. If tissue is sufficiently heated, such that the low impedance cut-off is passed, the power P decreases along the lines of the low impedance ramp **28a** of FIG. 6.

Combining the effects shown in FIG. 6 and FIG. 7, it becomes clear that when using a general-purpose generator set to a "fixed" power, the actual power 25 delivered can change dramatically over time as tissue heats up and impedance drops. Looking at FIG. 6, if the impedance Z drops from 100 to 75 ohms over time, the power output would not change because the curve is "flat" in that region of impedances. If, however, the impedance Z drops from 75 to 30 ohms one would transgress the low impedance cut-off and "turn the corner" onto the low impedance 30 ramp **28a** portion of the curve and the power output would decrease dramatically.

According to one exemplary embodiment of the invention, the control device, such as flow rate controller 11, receives a signal indicating the drop in actual power delivered to the tissue and adjusts the flow rate Q of saline to maintain the tissue/electrode interface at a desired temperature. In a preferred embodiment, the 35 drop in actual power P delivered is sensed by the power measurement device 8 (shown in FIG. 1), and the flow rate Q of saline is decreased by the flow rate controller 11 (also shown in FIG. 1). Preferably, this reduction in saline flow rate Q allows the tissue temperature to stay as hot as possible without desiccation. If the

control device was not in operation and the flow rate **Q** allowed to remain higher, the tissue would be over-cooled at the lower power input. This would result in decreasing the temperature of the tissue at the treatment site.

The flow rate controller 11 of FIG. 1 can be a simple “hard-wired” analog or

5 digital device that requires no programming by the user or the manufacturer. The flow rate controller 11 can alternatively include a processor, with or without a storage medium, in which the determination procedure is performed by software, hardware, or a combination thereof. In another embodiment, the flow rate controller 11 can include semi-programmable hardware configured, for example, using a

10 hardware descriptive language, such as Verilog. In another embodiment, the flow rate controller 11 of FIG. 1 is a computer, microprocessor-driven controller with software embedded. In yet another embodiment, the flow rate controller 11 can include additional features, such as a delay mechanism, such as a timer, to automatically keep the saline flow on for several seconds after the RF is turned off

15 to provide a post-coagulation cooling of the tissue or “quench,” which can increase the strength of the tissue seal. Also, in another embodiment, the flow rate controller 11 can include a delay mechanism, such as a timer, to automatically turn on the saline flow several seconds before the RF is turned on to inhibit the possibility of undesirable effects as sticking, desiccation, smoke production and char formation.

20 Also in another embodiment, the flow rate controller 11 can include a low level flow standby mechanism, such as a valve, which continues the saline flow at a standby flow level (which prevents the flow rate from going to zero when the RF power is turned off) below the surgical flow level ordinarily encountered during use of the electrosurgical device 5.

25 An exemplary electrosurgical device of the present invention which may be used in conjunction with the system of the present invention is shown at reference character 5a in FIG. 9, and more particularly in FIGS. 9-13. While various electrosurgical devices of the present invention are described with reference to use with the remainder of the system of the invention, it should be understood that the

30 description of the combination is for purposes of illustrating the remainder of the system of the invention only. Consequently, it should be understood that the electrosurgical devices of the present invention can be used alone, or in conjunction with the remainder of the system of the invention, or that a wide variety of electrosurgical devices can be used in connection with the remainder of the system

35 of the invention. The electrosurgical devices disclosed herein are preferably further configured for both open and laparoscopic surgery. For laparoscopic surgery, the devices are preferably configured to fit through either a 5 mm or 12 mm trocar cannula.

As shown in FIG. 8, electrosurgical device **5a** may be used in conjunction with a cannula as illustrated at reference character **19**, during laparoscopic surgery such as, for example, a laparoscopic cholecystectomy. Cannula **19** comprises a proximal portion **19a** separated from a distal portion **19b** by an elongated rigid shaft portion **19c**. Proximal portion **19a** of cannula **19** preferably comprises a head portion **19d** connected to rigid shaft portion **19c**, preferably by threaded engagement. Most importantly, cannula **19** has a working channel **19e** which extends through head portion **19d** and shaft portion **19c** from proximal portion **19a** to distal portion **19b** of cannula **19**. In one particular embodiment, during insertion 5 into cannula **19**, electrosurgical device **5a** is configured to enter the proximal end of working channel **19e**, move along the channel **19e** distally, and then be extended from the distal end of the working channel **19e**. In the same embodiment, during retraction from cannula **19**, electrosurgical device **5a** is configured to enter the distal end of working channel **19e**, move along the channel **19e** proximally, and then be 10 removed from the proximal end of working channel **19e**.

15

Referring back to FIG. 9, as shown electrosurgical device **5a** comprises a monopolar electrosurgical device. As shown in FIG. 9, electrosurgical device **5a** preferably includes a rigid, self-supporting, hollow shaft **17**, a proximal handle comprising mating handle portions **20a**, **20b** and a tip portion as shown by circle **45**. Handle **20a**, **20b** is preferably made of a sterilizable, rigid, non-conductive material, such as a polymer (e.g. polycarbonate). As shown in FIGS. 10 and 11, tip portion **45** includes a contact element preferably comprising an electrode **25** which, as shown, comprises a solid ball having a smooth, uninterrupted surface. Also as shown in FIGS. 10 and 11, tip portion **45** also comprises a sleeve **82** having a 20 uniform diameter along its longitudinal length, a spring **88** and a distal portion of shaft **17**. As shown in FIG. 10, the longitudinal axis **31** of the tip portion **45** may be configured at an angle **A** relative to the longitudinal axis **29** of the proximal remainder of shaft **17**. Preferably the longitudinal axis **31** of the tip portion **45** is 25 configured at an angle **A** of about 5 degrees to 90 degrees relative to the longitudinal axis **29** of the proximal remainder of shaft **17**. More preferably, the longitudinal axis **31** of tip portion **45** is configured at an angle **A** of about 8 degrees to 45 degrees relative to the longitudinal axis of **29** of the proximal remainder of shaft **17**.

30

As shown in FIGS. 10 and 11, for electrosurgical device **5a**, electrode **25** generally has a spherical shape with a corresponding spherical surface, a portion **42** of which is exposed to tissue **32** (less than 180 degrees and more specifically about 100-120 degrees) at the distal end of device **5a**. When electrode **25** is in the form of a sphere, the sphere may have any suitable diameter. However, the sphere 35 preferably has a diameter in the range between and including about 1 mm to about 7

mm. Although, it has been found that when a sphere is larger than about 4 mm and less than about 2 mm tissue treatment can be adversely effected (particularly tissue treatment time) due to an electrode surface that is respectively either to large or to small. Thus, more preferably the sphere has a diameter in the range between and 5 including about 2.5 mm to about 3.5 mm. Even more preferably, the sphere has a diameter of about 3 mm.

It is understood that shapes other than a sphere can be used for the contact element. Examples of such shapes include oblong or elongated shapes. However, as shown in FIGS. 10 and 11, preferably a distal end surface of electrosurgical 10 device 5a always provides a blunt, rounded surface which is non-pointed and non-sharp as shown by electrode 25.

As shown in FIGS. 10 and 11, electrode 25, is preferably located in a cavity 81 of a cylindrical sleeve 82 providing a receptacle for electrode 25. Among other things, sleeve 82 guides movement of the electrode 25. Among other things, sleeve 15 82 also functions as a housing for retaining the electrode 25.

Also as shown in FIG. 11, a portion 44 of the electrode 25, is retained within the cavity 81 while another portion 43 extends distally through the fluid outlet opening provided by circular fluid exit hole 26. Also as shown, sleeve 82 is connected, preferably via welding with silver solder, to the distal end 53 of shaft 17.

20 For device 5a, electrode 25, sleeve 82 and shaft 17 preferably comprise, and more preferably at least essentially consists of, an electrically conductive metal, which is also preferably non-corrosive, and more particularly stainless steel. Other metals include copper, titanium, gold, silver and platinum. Furthermore, shaft 17 preferably comprises thick walled stainless steel hypo-tubing.

25 As for cavity 81, the internal diameter of cavity 81 surrounding the electrode 25, is preferably slightly larger than the diameter of the sphere, typically by about 0.25 mm. This permits the sphere to freely rotate within the cavity 81. Consequently, cavity 81 of sleeve 82 also preferably has a diameter in the range of about 1 mm to about 7 mm.

30 As best shown in FIGS. 11 and 12, in order to retain the electrode 25, within the cavity 81 of sleeve 82, preferably the fluid exit hole 26, which ultimately provides a fluid outlet opening, of cavity 81 at its distal end 83 comprises a distal pinched region 86 which is reduced to a size smaller than the diameter of the electrode 25, to inhibit escape of the electrode 25 from the sleeve 82. More 35 preferably, the fluid exit hole 26 comprises a diameter smaller than the diameter of the electrode 25.

As best shown in FIG. 12, the fluid exit hole 26 preferably has a diameter smaller than the diameter of the electrode 25, which can be accomplished by at least

one crimp 84 located at the distal end 83 of the sleeve 82 which is directed towards the interior of the sleeve 82 and distal to the portion 44 of the electrode 25 confined in cavity 81. Where one crimp 84 is employed, the crimp 84 may comprise a single continuous circular rim pattern. In this manner, the contact element portion 5 extending distally through the fluid outlet opening (i.e. electrode portion 43) provided by fluid exit hole 26 has a complementary shape to the fluid outlet opening provided by fluid exit hole 26, here both circular.

However, as shown in FIG. 12, the crimp 84 may also comprise a discontinuous circular rim pattern where the crimp 84 is interrupted by at least one 10 rectangular hole slot 85 formed at the distal end 83 of the sleeve 82. Thus, the fluid outlet opening located at the distal end of the device 5a may comprise a first portion (e.g. the circular fluid exit hole portion 26) and a second portion (e.g. the slot fluid exit hole portion 85). As shown in FIG. 12, preferably, crimp 84 comprises at least 15 four crimp sections forming a circular rim pattern separated by four discrete slots 85 radially located there between at 90 degrees relative to one another and equally positioned around the fluid outlet opening first portion. Slots 85 are preferably used to provide a fluid outlet opening or exit adjacent the electrode 25, when the electrode 25 is fully seated (as discussed below) and/or when the electrode 25 is not in use (i.e. not electrically charged) to keep surface portion 42 of the electrode surface of 20 electrode 25 wet. Preferably, slots 85 have a width in the range between and including about 0.1 mm to 1 mm, and more preferably have a width in the range between and including about 0.2 mm to 0.3 mm. As for length, slots 85 preferably have a length in the range between and including about 0.1 mm to 1 mm, and more preferably have a length in the range between and including about 0.4 mm to 0.6 25 mm.

As shown in FIG. 12, the contact element portion extending distally through the fluid outlet opening (i.e. electrode portion 43) extends distally through the fluid outlet opening first portion (e.g. the circular fluid exit hole portion 26) and does not extend distally through the fluid outlet opening second portion (e.g. the slot fluid 30 exit hole portion 85). In this manner an edge 91 of the slot 85 remains exposed to tissue 32 to provide a tissue separating edge as discussed below.

It should be understood that the particular geometry of fluid outlet opening provided by the fluid exit hole located at the distal end of the device 5a to the electrode, is not critical to the invention, and all that is required is the presence of a 35 fluid exit hole which provides fluid 24 as required. For example, the fluid exit hole 26 may comprise an oval shape while electrode 25, comprises a different shape, such as a round shape.

As shown in FIG. 12, in addition to slot 85 providing a fluid exit, at least one edge 91 of slot 85 may provide a tissue separating edge adjacent a blunt surface (e.g. surface portion 42 of the electrode 25) which may be used for blunt dissection when the electrosurgical device 5a is manipulated, particularly by rotating (e.g. twirling), 5 abrading or impacting. When edge 91 is used in such regard, it is preferred that the edge comprise a sharp edge with a sharp angle which has not been rounded by, for example, a fillet.

Turning to the proximal end of the tip (comprising the electrode 25, spring 88 and sleeve 82) of the device 5a and electrode 25, as shown in FIG. 11, preferably 10 the portion of the sleeve 82 proximal to the electrode 25, also has a proximal pinched region 87 which retains the electrode 25 in the cavity 81 of the sleeve 82 and inhibits escape of the electrode 25 from the cavity 81 of the sleeve 82, such as a diameter smaller than the diameter of the electrode 25.

While distal pinched region 86 and proximal pinched region 87 may be used 15 solely to support the electrode 25, in its position of use, the electrode may be further supported by a compression spring 88 as shown in FIG. 11. The use of spring 88 is preferred to provide a variable length support within the working length of the spring 88 for overcoming manufacturing tolerances (e.g. length) between the fixed supports (i.e. pinched regions 86 and 87) of the sleeve 82. As for maintaining 20 proper location of the spring 88, sleeve 82 also comprises a lumen 89 as shown in FIG. 11 (i.e. the cavity of an elongated hollow structure, such as a tube or tube like structure; typically cylindrical) which, in addition to providing a direct passage for fluid, provides a guide tube for spring 88. Furthermore, the surface portion 60 of electrode 25, which contacts the spring 88 may comprise a flat surface rather than a 25 curvilinear surface to better seat the spring against the electrode 25.

In addition to the above, spring 88 provides a multitude of functions and 30 advantages. For example, the configuration of the distal pinched region 86, proximal pinched region 87 and spring 88 offers the ability to move the electrode 25, distally and proximally within sleeve 82. As shown in FIG. 11, spring 88 is located proximal to the electrode 25 between a first load bearing surface comprising the electrode surface 60 and a second load bearing surface comprising the distal end 53 of shaft 17. In this manner, spring 88 can be configured to provide a decompression force to seat the electrode 25 against the distal pinched region 86, in this case the perimeter edge 92 of crimp 84, prior to use of the electrosurgical device 5a.

35 Conversely, upon application of the electrode 25, of the device 5a against the surface 22 of tissue 32 with sufficient force to overcome the compression force of the spring 88, spring 88 compresses and the electrode 25 retracts proximally away from distal pinched region 86, in this case perimeter edge 92 of crimp 84, changing

the position thereof. In the above manner, the contact element comprising electrode 25 is retractable into the cavity 81 of the housing provided by sleeve 82 upon the application of a proximally directed force against surface 42 of the portion 43 of the electrode 25 extending distally beyond the distal opening 26 located at the distal end 5 83 of the housing and spring 88 functions as a retraction biasing member.

By making the electrode 25, positionable in the above manner via spring 88, in various embodiments the electrosurgical device 5a can be provided with a damper mechanism which dampens the force of the electrode 25 on tissue 32 being treated.

Furthermore, in various embodiments the electrosurgical device 5a, an 10 electrode 25 which can be positioned as outlined above can comprise a fluid flow rate adjustment mechanism which incrementally increases the area of the fluid exit hole 26 and the corresponding fluid flow rate in response to the incremental proximal retraction of the electrode 25. In such an instance the electrode 25 functions as a valve in regulating flow of the fluid 24 through fluid exit hole 26.

15 In various embodiments, spring 88 may be used in conjunction with the distal pinched region 86 (e.g. crimp 84 comprising a single continuous circular pattern) to provide a fluid seal between the electrode 25 and the distal pinched region 86 which stops fluid flow from the electrosurgical device 5a. In this manner, the electrosurgical 5a device may be used to provide both a wet electrode and dry 20 electrode (i.e. when the fluid flow is on and off, respectively) with the energy and fluid provided sequentially in addition to simultaneously. The incorporation of a dry electrode function into the device of the current invention may be desirable to provide a mechanism for electrosurgical cutting.

Furthermore, in various embodiments of electrosurgical device 5a, an 25 electrode 25 which can be positioned as outlined above can comprise a declogging mechanism which retracts to provide access for unclogging fluid exit holes, such as fluid exit holes 26 and 85, which may become flow restricted as a result of loose debris (e.g. tissue, blood) becoming lodged therein. For example, when a biasing force, such as from a handheld cleaning device (e.g. brush) or from pushing the 30 distal tip against a hard surface such as a retractor, is applied to surface 42 of electrode 25 which overcomes the compression force of the spring 88 causing the spring 88 to compress and the electrode 25 to retract, the tip of the handheld cleaning device may be extended into the fluid exit hole 26 for cleaning the fluid exit hole 26, perimeter edge 92, slot 85 and edge 91. Stated another way, an 35 electrode 25, which can be positioned as outlined, provides a method for declogging a fluid exit hole by increasing the cross-sectional area of the fluid exit hole to provide access thereto.

Also, in various embodiments of the electrosurgical device **5a**, the spring **88** comprises an electrical conductor, particularly when the electrode **25**, is retracted to a non-contact position (i.e. not in contact) with the sleeve **82**.

5 In other embodiments, proximal pinched region **87** may comprise one or more crimps similar to distal pinched region **86**, such that electrode **25** is retained in sleeve **82** both distally and proximally by crimps. Also, in other embodiments, sleeve **82** may be disposed within shaft **17** rather than being connected to the distal end **53** of shaft **17**. Also, in still other embodiments, sleeve **82** may be formed unitarily (i.e. as a single piece or unit) with shaft **17** as a unitary piece.

10 As best shown in FIGS. 10 and 11, the electrode **25** is retained in the sleeve **82** such that a portion **43** of the electrode **25** extends distally beyond distal end **83** of the sleeve **82**. As shown, preferably the surface **42** of this exposed portion **43** of the electrode **25** is blunt and does not comprise any sharp corners. Also, the portion **43** of the electrode **25** which extends distally beyond the distal end **83** of the sleeve **82** 15 is controlled by the shape of the fluid exit hole **26** in sleeve **82** in relation to the shape of the electrode **25**. In other words, the portion **43** of the electrode **25** which extends distally beyond the distal end **83** of the sleeve **82** is controlled by the contact of the electrode surface with the edge **92**.

20 As shown in FIGS. 10 and 11, in locations where shaft **17** and sleeve **82** are electrically conductive (for device **5a**, preferably shaft **17** and sleeve **82** are completely electrically conductive and do not comprise non-conductive portions), preferably an electrical insulator **90** (i.e. comprising non-conductive or insulating material) preferably surrounds shaft **17** and sleeve **82** along substantially its entire exposed length (e.g. the portion outside the confines of the handle **20**), terminating a 25 short distance (e.g. at the proximal onset of the crimp **84** or less than about 3 mm) from distal end **83** of the sleeve **82**. Insulator **90** preferably comprises a shrink wrap polymer tubing.

30 As with the other electrosurgical devices described within, a input fluid line **4b** and a power source, preferably comprising generator **6** preferably providing RF power via cable **9**, are preferably fluidly and electrically coupled, respectively, to the tip portion **45** of the electrosurgical device **5a**.

35 As indicated above, device **5a** comprises a monopolar device. In other words, a first electrode, often referred to as the active electrode, comprises an electrode of the electrosurgical device **5a** (e.g. electrode **25**) while a second electrode, often referred to as the indifferent or return electrode, comprises a ground pad dispersive electrode located on the patient, typically on the back or other suitable anatomical location. Preferably, both electrodes are electrically coupled to the generator **6** to form an electrical circuit. Preferably the active electrode is

coupled to the generator 6 via a wire conductor from insulated wire cable 9 to the outer surface 18 of the shaft 17 within the confines of the handle 20a, 20b, typically through a switch 15a.

In other embodiments, the shaft 17 may be made of an electrical non-conducting material except for a portion at its distal end 53 that comes in contact with sleeve 82. This portion of shaft 17 that contacts the sleeve 82 should be electrically conducting. In this embodiment, the wire conductor from insulated wire cable 9 extends to this electrically conducting portion of shaft 17. In still other embodiments, the shaft 17 may completely comprise a non-conducting material as where the wire conductor from insulated wire cable 9 extends directly to the sleeve 82.

With respect to the fluid coupling, fluid 24 from the fluid source 1 for use with electrosurgical device 5a preferably is communicated from fluid source 1 through a flexible, polyvinylchloride (PVC) outlet fluid line 4a to a flexible, polyvinylchloride (PVC) inlet fluid line 4b connected to the electrosurgical device 5a. The outlet fluid line 4a and the inlet fluid line 4b are preferably connected via a male and female mechanical fastener configuration, preferably comprising a Luer-Lok® connection from Becton, Dickinson and Company. The lumen of the inlet line is then preferably interference fit over the outside diameter of the shaft 17 to provide a press fit seal there between. Additionally an adhesive may be disposed there between to strengthen the seal. Fluid 24 is then communicated down the lumen 23 of the shaft 17 through the lumen 89 and cavity 81 of the sleeve 82 where it is expelled from around and on the exposed surface 42 of the electrode 25. This provides a wet electrode for performing electrosurgery.

As shown in FIG. 13, during use of electrosurgical device 5a, typically a fluid coupling 30 preferably comprising a discrete, localized web and more preferably comprising a triangular shaped web or bead portion providing a film of fluid 24 is provided between the surface 22 of the tissue 32 and electrode 25. When the user of electrosurgical device 5a places the electrode 25 at a tissue treatment site and moves the electrode 25 across the surface 22 of the tissue 32, fluid 24 is expelled around and on the surface 42 of the electrode 25 at the distal end 83 of the sleeve 82 and onto the surface 22 of the tissue 32 via coupling 30. The fluid 24, in addition to providing an electrical coupling between the electrosurgical device 5a and the tissue 32, lubricates the surface 22 of the tissue 32 and facilitates the movement of electrode 25 across the surface 22 of the tissue 32. During movement of the electrode 25, the electrode 25 typically slides across the surface 22 of the tissue 32, but also may rotate as the electrode 25 moves across the surface 22 of the tissue 32. Typically the user of the electrosurgical device 5a slides the electrode

across the surface 22 of the tissue 32 back and forth with a painting motion while using the fluid 24 as, among other things, a lubricating coating. Preferably the thickness of the fluid 24 between the distal end surface of the electrode 25 and the surface 22 of the tissue 32 at the outer edge of the coupling 30 is in the range

5 between and including about 0.05 mm to 1.5 mm. More preferably, the fluid 24 between the distal end surface of the electrode 25 and the surface 22 of the tissue 32 at the outer edge of the coupling 30 is in the range between and including about 0.1 mm to 0.3 mm. Also preferably, in certain embodiments, the distal end tip of the electrode 25 contacts the surface 22 of tissue 32 without any fluid 24 in between.

10 Another exemplary electrosurgical device of the present invention which may be used in conjunction with the system of the present invention is shown at reference character 5b in FIGS 14-16. In this embodiment, electrical insulator 90 preferably terminates proximally to the sleeve 82 where sleeve 82 is connected to the distal end 53 of shaft 17. In certain embodiments where the sleeve 82 is formed 15 unitary with the shaft 17, the electrical insulator 90 preferably terminates proximally to proximal pinched region 87. In this manner, in addition to the spherical surface portion 42 of the electrode 25 and the narrowing surface portion 41, here conical, of the sleeve 82 being used for treating tissue 32 when exposed thereto, a cylindrical surface 40 of a cylindrical portion 39 of the sleeve 82 and a broadening surface portion 47 of broadening portion 54, here both conical, of the sleeve 82 also function 20 as electrode surfaces for treating tissue. Thus, the electrode exposed to tissue 32 now comprises a cylindrical surface portion 40 and a broadening surface portion 47 in addition to the spherical surface portion 42 and the narrowing surface portion 41, with the cylindrical surface portion 40 substantially increasing the surface area of 25 the electrode. As a result, the electrode 25 now also comprises surfaces which are parallel and perpendicular to the longitudinal axis 31 of the tip portion 45, and more particularly sleeve 82, of the electrosurgical device 5b. In the above manner, front end use (e.g. surfaces 41 and 42), sideways use (e.g. surface 40 and 47) or oblique use (e.g. surfaces 40, 41 and 42) of the electrosurgical device 5b is facilitated.

30 In the above manner, the tip portion 45 now comprises a first tissue treating surface (e.g. distal end spherical surface 42) and a second tissue treating surface (e.g. side surface 40). As discussed above, preferably the first tissue treating surface is configured for blunt dissection while the second tissue treating surface is configured for coagulation. Additionally, tip portion 45 also comprises a third tissue treating 35 surface (e.g. surface 41) located between the first tissue treating surface (e.g. surface 42) and a second tissue treating surface (e.g. surface 40). Furthermore, tip portion 45 also comprises a fourth tissue treating surface (e.g. surface 47) located proximal and adjacent to surface 40.

With device **5a**, when the electrode **25**, is placed directly in contact with surface **22** of tissue **32**, it may be possible for the tissue **32** to occlude fluid flow from the fluid exit holes **26**, **85** located at the distal end of the device **5a**.

Consequently, for device **5b** fluid exit holes **93**, **94** may be located in the cylindrical side portion **39** of the sleeve **82**, either proximal or adjacent to the electrode **25**, and either in addition to or as an alternative to fluid exit holes **26**, **85**.

As shown in FIGS. **14** and **15**, at least one fluid exit hole **93** is preferably formed in the cylindrical longitudinal side surface **40** and through the wall of side portion **39** of the sleeve **82** adjacent to electrode **25** when electrode **25** is fully seated. Furthermore, preferably at least one fluid exit hole **94** is formed in the cylindrical side portion **39** of the sleeve **82** proximal to electrode **25** when electrode **25** is fully seated.

Preferably, holes **93**, **94** each comprise more than one hole which are equally spaced radially in a circular pattern around the longitudinal axis **31** of the tip portion **45**, and more particularly sleeve **82**. More preferably, holes **93**, **94** each comprise four discrete holes equally spaced 90 degrees around the cylindrical side portion **39** of the sleeve **82**. Preferably holes **93**, **94** have a diameter in the range between and including about 0.1 mm to 1.0 mm, and more preferably have a length in the range between and including about 0.2 mm to 0.6 mm. Electrode **25** which can be positioned as outlined above can comprise not only a valve for regulating fluid flow from the fluid exit holes, such as fluid exit hole **26**, but also comprise a valve which while opening one fluid flow exit simultaneously closes another fluid flow exit. For example, as electrode **25** retracts proximally, fluid exit hole **26** is opened while fluid exit hole **93** is closed. Stated another way, an electrode **25** which can be positioned as outlined above can provide a mechanism for altering the size and/or location of the fluid exit holes during use of the electrosurgical device **5b** which may be necessary, for example, to direct fluid to a particular tissue location or balance fluid flow among the fluid exit outlets.

Thus, as shown in FIGS. **14** and **15**, surfaces **40**, **41** and **47** of the sleeve **82**, and surface **42** of electrode **25** are all active electrode surfaces and can provide electrical energy to tissue **32**. Portions of this combined electrode surface can be wet by fluid flow from holes **26**, **94** or **93**, as well as from the hole slots **85** in the crimp **84** adjacent the electrode **25**.

The holes **94**, **93** in the cylindrical sleeve **82** of the overall electrode surface are intended to assure that fluid **24** is provided to the smooth, less rough, atraumatic sides of the electrode that are used to produce tissue coagulation and hemostasis (e.g. surfaces **40** and **47**) rather than blunt dissection (e.g. surfaces **41** and **42**). The

most distal portion of the device may have a more rough, but also wetted, electrode surface that can blunt dissect as well as coagulate tissue.

The electrode configuration shown in FIGS. 14 and 15 is particularly useful to a surgeon performing a liver resection. Once the outer capsule of the liver is 5 scored with a dry bovie blade along the planned line of resection the distal tip of tip portion 45 is painted back and forth along the line, resulting in coagulation of the liver parenchyma. As the tissue is coagulated under and around the electrode surfaces 40, 41 and 42, the electrode is used to blunt dissect into the coagulated parenchyma, with the edge 91 of the slots 85 around the crimp 84 providing 10 roughness elements that aid in disrupting the tissue 32 and enabling the parting of the tissue 32.

As shown in FIG. 16, the device 5b can be used deeply in a crevice 97 of tissue 32 to blunt dissect the tissue 32 and coagulate it at the same time. Blunt dissection is preferred over sharp dissection, such as with a blade or scissors, since 15 blunt dissection is less likely to tear or damage the larger blood vessels or other vessels. Once identified by blunt dissection, larger vessels can be safely clipped, tied with suture or sealed with some other device. If the larger vessels are not thus first "skeletonized" without being damaged by blunt dissection, they may bleed profusely and require much more time to stop the bleeding. The device can also be 20 used to coagulate first without simultaneous blunt dissection, and then blunt dissect in a separate step.

This technique can also be used on other parenchymal organs such as the pancreas, the kidney, and the lung. In addition, it may also be useful on muscle tissue and subcutaneous fat. Its use can also extend to benign tumors, cysts or other 25 tissue masses found in the urological or gynecological areas. It would also enable the removal of highly vascularized tumors such as hemangiomas.

In FIG. 16 the zone 99 identifies the part of the electrode that has the ability to blunt dissect and coagulate, and the zone 98 identifies the part that is intended primarily for coagulation and hemostasis. The line 100 indicates the depth of the 30 zone of tissue that is coagulated, typically from 3 mm to 5 mm deep.

For the devices disclosed herein, the presence of various fractions of boiling can be visually estimated by the naked eye, or by detecting changes in electrical impedance. FIG. 17 shows a plot of electrical impedance Z versus time t . The impedance spikes 101 shown in FIG. 17 occur at a frequency of about 1 cycle per 35 second and with an amplitude that is on the same order as the baseline impedance. This frequency is shown in FIG. 17 as the interval 102 between successive impedance spikes. Impedance is directly measurable by dividing the voltage by the current as previously described. The use of electrical impedance to detect the onset

of tissue dessication when impedance rises dramatically as a result of being heated to the point of smoking and charring, but not to detect the presence of boiling, is described above. As shown in FIG 17, the impedance **Z** may change from a level of about 100 ohms with no boiling, to a level of about 400 ohms or more with a large 5 fraction of the conductive fluid boiling. The percentages of boiling shown are exemplary as are the levels of impedance.

Shown in FIG. 18 is the qualitative nature of the boiling as the % boiling increases, indicated by the small figures for each of five exemplary "regimes" of boiling. In each small figure a portion of the tip of the tip portion **45** of the device 10 **5a** is shown in close proximity to tissue **32**. As boiling begins in regime **104**, there are few small bubbles **37** of vapor in the conductive fluid **24**, here saline, of coupling **30**. As the percentage of boiling increases at regime **106** there are a larger number of small bubbles **37**. As the percentage boiling increases further at regime **107**, the bubbles **37** become much larger. At even higher percentage boiling at regime **108** 15 intermittent threads of saline form and are quickly boiled off. Finally, at the highest level of regime **109**, drops **36** of saline are instantly boiled upon contacting the hot surface **22** of the tissue **32** and arcing occurs from the metal to the tissue **32**.

Returning to FIGS. 14 and 15, fluid outlet openings are provided by substantially linear through holes **93**, **94** which provide conductive fluid **24** to the 20 treatment site. However, in an alternative embodiment, as shown in FIG. 19, fluid outlet openings in the sleeve **82** may be provided by holes in the form of tortuous and interconnected pathways **59**, which are formed in a material pervious to the passage of fluid **24**, therethrough, such as a porous material. The discrete, linear through holes **93**, **94** may be either supplemented with or replaced by a plurality of 25 tortuous, interconnected pathways **59** formed in the porous material which, among other things, provides porous surfaces **40**, **41** and **47** to more evenly distribute fluid flow and provide the conductive fluid **24** to tissue **32** at the treatment site. According to the invention, all or a portion of the sleeve **82** may comprise a material pervious to the passage of fluid **24** therethrough as disclosed herein.

30 In certain embodiments, the contact element, here electrode **25** may also comprise a material pervious to the passage of fluid **24**, therethrough, such as a porous material (e.g. metal, polymer or ceramic) to provide the tortuous pathways **59**. In these embodiments, the porous structure of the electrode **25** allows fluid **24** to not only pass around electrode **25** on the outer porous surface **42** to be expelled, but 35 also allows fluid **24** to pass through the electrode **25**, to be expelled. According to the invention, all or a portion of the electrodes or any particular electrodes for treating tissue **32** may comprise a material pervious to the passage of fluid **24** therethrough as disclosed herein.

Where the contact element and sleeve provide electrodes for treating tissue and compromise a porous material, preferably the porous material further comprises porous metal. Porous sintered metal is available in many materials (such as, for example, 316L stainless steel, titanium, Ni-Chrome) and shapes (such as cylinders, 5 discs, plugs) from companies such as Porvair, located in Henderson, NC.

Porous metal components can be formed by a sintered metal powder process or by injection molding a two-part combination of metal and a material that can be burned off to form pores that connect (open cell) to each other. With sintering, for example, typically solid particles of material are placed in a mold under heat and 10 pressure such that the outer surface of the particles soften and bond to one another with the pores comprising the interstices between the particles. Alternatively, when porosity is formed by burning off material, it is not the interstice between the particles which provides the porosity as with sintering, but rather a partial 15 evisceration of the material generally provided by the removal of a component with a lower melt temperature than the burn off temperature.

While the electrode provided by contact element and/or sleeve preferably comprises an electrically conductive material such as metal, a non-electrically conductive porous contact element and/or sleeve, such as porous polymers and ceramics, can be used to replace an electrically conductive contact element and/or 20 sleeve. While the porous polymers and ceramics are generally non-conductive, they may also be used to conduct the RF energy through the porous polymer and ceramic thickness and porous surface to the tissue to be treated by virtue of conductive fluid 24 contained within the plurality of interconnected tortuous pathways 59.

Preferably the tortuous passages in the porous materials have a pore size 25 (cross-sectional dimension) in the range between and including about 2.5 micrometers (0.0025 mm) to 500 micrometers (0.5 mm) and more preferably has pore size in the range between and including about 10 micrometers (0.01 mm) to 120 micrometers (0.12 mm). Even more preferably, the porous material has a pore 30 size in the range between and including about 20 micrometers (0.02 mm) to 80 micrometers (0.08 mm).

In addition to possibly providing a more uniform distribution of fluid 24, the porous materials also may provide other advantages. For example, when the 35 electrode surfaces, such as surfaces 40, 41, 42 and 47, in contact with the surface 22 of tissue 32 are porous and dissipate fluid 24, the tissue 32 is less apt to stick to the surfaces 40, 41, 42 and 47 of the electrode as compared to the situation where the surfaces 40, 41, 42 and 47 are not porous. In addition, by providing fluid 24 to surfaces 40, 41, 42 and 47 through tortuous pathways 59, heated and/or electrified fluid 24 can now be provided more uniformly to surfaces 40, 41, 42 and 47, which

may result in a wider tissue treatment region as compared to when the surfaces are not porous.

Preferably the porous material provides for the wicking (i.e. drawing in of fluid by capillary action or capillarity) of the fluid 24 into the pores of the porous material. In order to promote wicking of the fluid 24 into the pores of the porous material, preferably the porous material, and in particular the surface of the tortuous pathways, is hydrophilic. The porous material may be hydrophilic with or without post treating (e.g. plasma surface treatment such as hypercleaning, etching or micro-roughening, plasma surface modification of the molecular structure, surface 5 chemical activation or crosslinking), or made hydrophilic by a coating provided thereto, such as a surfactant.

Though not preferable, it is not necessary that fluid coupling 30 of fluid 24 be present in between the metal electrode surfaces (e.g. 40, 41, 42) and tissue 32 at all locations of tissue treatment and there may be points of direct tissue contact by 10 the electrode surfaces without any fluid coupling 30 therebetween. In such an instance, the convective cooling of the metal electrode by flowing saline is often sufficient to keep the metal electrode and tissue contacting the metal electrode at or below a temperature of 100 °C. In other words, heat may be also first dissipated from the tissue 32 to the electrodes by conduction, then dissipated from the 15 electrodes to the fluid 24 by convection.

Preferably the relationship between the material for electrodes particularly their surfaces (e.g. 40, 41, 42, 47), and fluid 24 throughout the various embodiments should be such that the fluid 24 wets the surface of the electrodes to form a continuous thin film coating thereon (for example, see FIG. 19A) and does not form 20 isolated rivulets or circular beads (e.g. with a contact angle, θ greater than 90 degrees) which freely run off the surface of the electrode. Contact angle, θ , is a quantitative measure of the wetting of a solid by a liquid. It is defined geometrically 25 as the angle formed by a liquid at the three phase boundary where a liquid, gas and solid intersect. In terms of the thermodynamics of the materials involved, contact angle θ involves the interfacial free energies between the three phases given by the 30 equation $\gamma_{LV} \cos \theta = \gamma_{SV} - \gamma_{SL}$ where γ_{LV} , γ_{SV} and γ_{SL} refer to the interfacial energies of the liquid/vapor, solid/vapor and solid/liquid interfaces, respectively. If the contact angle θ is less than 90 degrees the liquid is said to wet the solid. If the 35 contact angle θ is greater than 90 degrees the liquid is non-wetting. A zero contact angle θ represents complete wetting. Thus, preferably the contact angle is less than 90 degrees.

For clarification, while it is known that the contact angle θ may be defined by the preceding equation, in reality contact angle θ is determined by a various

models to an approximation. According to publication entitled "Surface Energy Calculations" (dated September 13, 2001) from First Ten Angstroms (465 Dinwiddie Street, Portsmouth, Virginia 23704), there are five models which are widely used to approximate contact angle θ and a number of others which have

5 small followings. The five predominate models and their synonyms are: (1) Zisman critical wetting tension; (2) Girifalco, Good, Fowkes, Young combining rule; (3) Owens, Wendt geometric mean; (4) Wu harmonic mean; and (5) Lewis acid/base theory. Also according to the First Ten Angstroms publication, for well-known, well characterized surfaces, there can be a 25% difference in the answers provided

10 for the contact angle θ by the models. Also for clarification, any one of the five predominate models above which calculates a contact angle θ within a particular range of contact angles θ or the contact angle θ required of a particular embodiment of the invention should be considered as fulfilling the requirements of the embodiment, even if the remaining four models calculate a contact angle θ which

15 does not fulfill the requirements of the embodiment.

The effects of gravity and surface tension tend to wick the fluid **24**, here saline, around the circumference of the cylindrical sleeve **82** to preferably cover the entire active electrode surface. More specifically, the effects of gravity and surface tension on fluid **24** which is located on the electrode surfaces may be modeled by the

20 Bond number N_{BO} . Bond number N_{BO} measures the relationship of gravitational forces to surface tension forces and may be expressed as:

$$N_{BO} = \text{gravitational force/surface tension force}$$

$$N_{BO} = \rho L^2 g / \sigma$$

where:

25 ρ = Density of the saline fluid (approximately 1.0 gm/cm³);
 L = droplet diameter (cm)
 g = Gravitational acceleration (980 cm/s²)
 σ = Surface tension (approximately 72.8 dynes/cm @ 20° C)

30 For a Bond number $N_{BO} = 1$, the droplet diameter is equal to about .273 cm or about 2.7 mm, which is in the same order of magnitude as the preferred size of the electrode. For the purposes of the present invention, preferably Bond number N_{BO} for a droplet of fluid **24** on a surface of the electrode **25** is preferably less than 1.

Another tip portion of an exemplary electrosurgical device **5c** of the present

35 invention which may be used in conjunction with the system of the present invention is shown at reference character **45** in FIGS **20-24**. As best shown in FIGS. **20** and **21**, the separate sleeve **82** of embodiments **5a** and **5b** has been eliminated from tip portion **45** of device **5c**. Consequently, the contact element, still preferably

comprising an electrode 25, is assembled directly with the shaft 17. Electrode 25 is preferably assembled (e.g. mechanically connected via press fit, mechanical connector, threaded, welded, adhesively bonded) adjacent the distal end 53 of shaft 17. In certain embodiments, the electrode 25 preferably is detachably assembled to 5 the shaft 17 such that it may be removed from the shaft 17, preferably manually by human hand, so that the shaft 17 may be used with multiple different contact elements/electrodes, or the shaft 17 may be reusable and used with disposable contact elements/electrodes.

As shown in FIGS. 20-24, electrode 25 preferably comprises an enlarged 10 head portion comprising a spherical portion 43 and a corresponding spherical surface portion 42 located at the distal end of the device 5c which provided a smooth, blunt contour outer surface. More specifically, as shown, the spherical portion 43 and spherical surface portion 42 further provide a domed, hemisphere (i.e. less than a full sphere) and hemispherical surface portion comprising preferably 15 about 180 degrees.

Also as shown in FIGS. 20-24, the enlarged head portion of electrode 25 preferably also comprises a cylindrical portion 39 and a corresponding cylindrical surface portion 40 located proximal and adjacent to the spherical portion 43 and spherical surface portion 42, respectively.

20 Further continuing with FIGS. 20-24, electrode 25 preferably comprises a connector portion, preferably comprising a shank 46, which connects the remainder of the electrode 25 to the shaft 17. Among other things, the connector portion of the electrode 25 is preferably configured to form a connection with a mating connector portion of the shaft 17. As shown, preferably the shank portion 46 is configured to 25 extend into cavity 50 of shaft 17 which comprises a cylindrical receptacle and provides the mating connector portion for shank 46. More preferably, surface 48 of the shank portion 46 is configured to mate against and form an interference fit with surface 52 of cavity 50 to provide the connection.

Continuing with FIGS. 20-24, shank portion 46 is preferably cylindrical and 30 located proximal and adjacent to a neck portion 56. As shown, here neck portion 56 also comprises a cylindrical portion 57 (having a corresponding cylindrical surface portion 58) located proximal and adjacent to a broadening portion 54 (having a corresponding broadening surface portion 47). Here broadening portion 54 and corresponding broadening surface portion 47 are both spherical, and more 35 specifically comprise a domed, hemisphere and hemispherical surface portion comprising preferably about 180 degrees, located proximal and adjacent to the cylindrical portion 39 and cylindrical surface portion 40.

As shown in FIGS. 20-24, the cylindrical portion 57 of neck portion 56 preferably has a cross-sectional dimension, here diameter, greater than the cross-sectional dimension, here also diameter, of the shank 46. In this manner, in certain embodiments, the proximal end of the neck portion 56 may be located adjacent and in contact with the distal end 53 of shaft 17.

Also as shown in FIGS. 20-24, electrode 25 comprises at least one recess 64 which provides an elongated fluid flow channel for the distribution of fluid 24. The use of device 5c, and in particular recesses 64, for the distribution of fluid 24 is generally preferred to the fluid exit holes 93, 94 of device 5b in particularly deep tissue crevices 97 where tissue 32 can occlude fluid flow from the fluid exit holes located in the cylindrical portion 39 of the electrode 25.

As shown, electrode 25 preferably comprises a plurality of longitudinally directed recesses 64 and, more specifically, four recesses 64 equally spaced 90 degrees around the shank 46 and/or neck portion 56, both proximal of cylindrical portion 39. As best shown in FIG. 24, in certain embodiments, the recess 64 may comprise a first side wall 64a, a second opposing side wall 64b, and a bottom wall 64c.

In use, when tissue 32 overlies and occludes the fluid outlet opening 55 of recess 64 for a portion of its longitudinal length, thus inhibiting fluid 24 from exiting therefrom, fluid 24 from recess 64 may still be expelled from the electrosurgical device 5c after flowing longitudinally in the channel 64 to a remote location where the channel 64 is unoccluded and uninhibited to fluid flow exiting therefrom.

However, in certain instances, it may be possible that the recess 64 may be occluded by tissue 32 completely along its longitudinal length, thus completely inhibiting fluid flow from exiting through opening 55. In order to overcome this problem, at least a portion of the electrode 25 may comprise a material pervious to the passage of fluid 24, therethrough, such as a porous material described above.

As shown in FIG. 25, in another embodiment of the electrosurgical device of the present invention, as shown at reference character 5d in FIG. 25, the walls 64a, 64b of recess 64, surface 48 of the shank portion 46, and/or the surfaces of the neck portion 56 of electrode 25 may be porous and connected by a plurality of tortuous pathways 59 in the porous material. Consequently, rather than flowing out of recess 64 from a direct fluid outlet opening 55, which may be occluded by tissue 32, the fluid 24 may exit indirectly from recess 64 by first flowing through tortuous pathways 59 of the electrode 25 from side walls 64a, 64b of the recess 64 and then exit the electrode 25 from surface 58, which may be in unoccluded by tissue 32. Alternatively, if adjacent surface 58 of the electrode 25 is also occluded by tissue 32, the fluid 24 may continue to flow through tortuous pathways 59 of electrode 25 and

exit electrode 25 from a surface 64a, 64b of a recess 64 or surface such as 40, 42, 47 or 58 which may be in unoccluded by tissue 32.

Where the electrode 25 comprises a porous material, recess 64 may be either supplemented with or replaced by the plurality of tortuous, interconnected passages 59 formed in the porous material as shown in FIG. 25, with porous surfaces such as 40, 42, 47 or 58 to more evenly distribute fluid flow and provide conductive fluid 24 to the tissue treatment site. All or a portion of the electrodes can be porous according to the invention.

In other embodiments of the invention, recess 64 may comprise cross-sectional shapes other than rectangular shapes. For example, as shown in FIGS. 26-28 recess 64 comprises a semi-circular shape, a V-shape, or a U-shape respectively, or any combination thereof.

Returning to FIG. 21, in order to facilitate direct fluid communication of recess 64 with lumen 23 of shaft 17, preferably recesses 64 of device 5c are initiated 15 within the confines of shaft 17. In other words, within the cavity 50 of shaft 17 proximal to distal end 53. Preferably the configuration of the recesses 64 as provided by geometry (e.g. width, depth) and/or the material and/or surface treatment of the electrode 25 may be arranged such that surface tension will act to retain fluid collected in the recess 64 where the force of gravity is acting to remove 20 the fluid from the recess 64. However, while it is desirable that a certain predetermined amount of surface tension act to retain fluid collected in the recess 64 in the presence of gravity, the surface tension must be balanced against the inhibition of fluid flow from the recess 64.

As indicated above, the use of device 5c, and in particular recesses 64, for 25 the distribution of fluid 24 is generally preferred to the fluid exit holes 93, 94 of device 5b in particularly deep tissue crevices 97 where tissue 32 can occlude fluid flow from the fluid exit holes 93, 94 located in the cylindrical portion 39 of the electrode 25. Also, since holes 93, 94 are not presented with a declogging mechanism, such as provided for such as fluid exit holes 26 and 85, holes such as 30 93, 94 that can be simply occluded by ordinary tissue/electrode contact will sooner or later become irreversibly clogged.

As shown in FIG. 21, with device 5c fluid outlet openings 73 are provided by the structure of the electrode 25 (i.e. recesses 64) at the distal end 53 of the shaft 17 which are protected and sheltered from contact and occlusion from surface 22 of tissue 32. Fluid outlet openings 73 of device 5c are protected from occlusion from surface 22 of tissue 32 as the structure of device 5c defining the openings 73 is at 35 least partially configured for non-contact with surface 22 of tissue 32. More specifically, here the structure of the device defining the openings 73 is completely

configured for non-contact with surface 22 of tissue 32. Stated another way, the openings 73 are provided on the device 5c at a location removed from the tissue surface 22. Also, as shown, openings 73 are particularly sheltered from occlusion from surface by 22 of tissue 32 by a portion of the shaft 17. Also as shown, when 5 openings 73 are formed substantially perpendicular to the surface 22 of tissue 32 and thus turned away from direct contact with surface 22 of tissue 32.

Another tip portion of an exemplary electrosurgical device 5e of the present invention which may be used in conjunction with the system of the present invention is shown at reference character 45 in FIGS. 29-32. As best shown in FIGS. 31 and 10 32, the broadening portion 54 has been eliminated and the cylindrical portion 39 has an equal cross-sectional dimension, here diameter, with the neck portion 56. Conversely, for device 5c, the cylindrical portion 39 has a cross-sectional dimension, there also diameter, greater than the cross-sectional dimension, there also diameter, of the neck portion 56.

15 Also as shown in FIGS. 31 and 32, the cylindrical portion 39 further comprises a rectilinear (straight) cylindrical portion 39a having a rectilinear cylindrical surface portion 40a and a curvilinear cylindrical portion 39b having a curvilinear cylindrical surface portion 40b. As shown, device 5e comprises the shape of a hockey stick. The cylindrical portion 39 for device 5c may be similarly 20 arranged.

Another tip portion of an exemplary electrosurgical device 5f of the present invention which may be used in conjunction with the system of the present invention is shown at reference character 45 in FIGS 33-36. As best shown in FIGS. 35 and 25 36, the cylindrical portion 39 has a cross-sectional dimension, here diameter, less than the cross-sectional dimension, here also diameter, of the neck portion 56. As shown the neck portion 56 is located proximal and adjacent to a narrowing portion 49 with a corresponding narrowing surface portion 51, here both conical.

Also as shown in FIG. 34, the cylindrical portion 39 further comprises a rectilinear cylindrical portion 39a having a rectilinear cylindrical surface portion 40a 30 and a curvilinear cylindrical portion 39b having a curvilinear cylindrical surface portion 40b. Furthermore, as shown, the cylindrical portion 39, and more specifically at least one of the rectilinear cylindrical portion 39a and the curvilinear cylindrical portion 39b, comprises a portion of a hook. Preferably, as shown both the rectilinear cylindrical portion 39a and the curvilinear cylindrical portion 39b 35 comprise portions of a hook. As shown in FIGS. 35 and 36, the hook further comprises an L-hook.

Another tip portion of an exemplary electrosurgical device 5g of the present invention which may be used in conjunction with the system of the present invention

is shown at reference character 45 in FIGS 37-38. As shown, for device 5g the cylindrical portion 39, and more specifically both the rectilinear cylindrical portion 39a and the curvilinear cylindrical portion 39b comprise portions of a hook. Also as shown in FIGS. 37 and 38, the hook further comprises an J-hook.

5 Another tip portion of an exemplary electrosurgical device 5h of the present invention which may be used in conjunction with the system of the present invention is shown at reference character 45 in FIGS 39-42. As shown in FIGS. 39 and 40, electrode 25 preferably comprises a finger portion 65 (preferably comprising cylindrical portion 39 and cylindrical surface portion 40) having a distal end
10 (preferably comprising a spherical portion 43 and spherical surface portion 42) which, among other things, is configured for blunt dissection or electrosurgical dissection of tissue 32. Electrosurgical dissection occurs when tension or force is applied to tissue while also applying RF energy. The RF energy heats the tissue, thereby weakening it, and the tissue yields or breaks where desired. Surgeons may
15 refer to this type of dissection with a hook-type electrode as "hook and cook". Furthermore, finger portion 65 is also preferably configured to function as a hook, particularly the anterior (i.e. front) surface portion 66 of finger portion 65 which is configured, among other things, to engage and restrain tissue 32.

As shown, finger portion 65 is rectilinear and forms an L-hook with an angle
20 of about 90 degrees relative to the longitudinal axis 31 of the tip portion 45, particularly shank 45. However, finger portion may be formed at angles other than 90 degrees. For example, finger portion 65 may be formed at any angle in the range between and including about 60 degrees relative to the tip portion 45 to about 180 degrees relative to the tip portion 45, or any other range of angles or particular angle
25 inclusive therein (e.g. 75°, 105°, 120°, 135°, 180°, 90°-135°, 90°-180°).

Among other things, electrode 25 preferably comprises a knuckle portion 61 comprising a rounded protuberance having a raised prominence on the posterior (back) surface portion 62 of the electrode 25. Also as shown, knuckle portion 61 also comprises a rounded protuberance having a raised prominence on the lateral
30 surface portion 75 of the electrode 25. Among other things, posterior knuckle surface portion 62 and lateral knuckle surface portion 75 formed by knuckle portion 61 are configured for coagulation and stasis (e.g. hemostasis, aerostasis) of tissue 32.

Key to device 5g is the cross-sectional dimension of the knuckle Z to the cross-section dimension of the finger F. When comparing the functions of blunt or
35 electrosurgical dissection and coagulation/hemostasis, the coagulation/hemostasis portion of the electrode 25 preferably comprises a greater surface area than the blunt or electrosurgical dissection portion of the electrode 25.

As shown in FIG. 36, preferably the cross-sectional dimension **Z**, of the knuckle portion **61** is greater than cross-section dimension **F** of the finger portion **65**. Here, as shown, the cross-sectional dimensions **Z** and **F** comprise diameters. However, in other embodiments where the cross-sectional dimension **Z** and/or **F** could not properly be considered to comprise a diameter, the cross-sectional dimension **Z** and/or **F** could comprise a width or thickness.

Preferably, the cross-sectional dimension **Z** of the knuckle portion **61** is in the range between and including about 1.6 to 3.3 times greater than the cross-section dimension **F** of the finger portion **65**, with typical dimensions comprising the ratios of 2.5 mm to 1.5 mm (1.6 times) and 2.5 mm to 0.75 mm (3.3 times). Even more preferably, the cross-sectional dimension **Z** of the knuckle portion **61** is in the range between and including about 2 to 2.5 times greater than the cross-section dimension **F** of the finger portion **65**, with typical dimensions comprising the ratios of 2.5 mm to 1.25 mm (2 times) and 2.5 mm to 1 mm (2.5 times).

From the above dimensions, the ratio of the surface area of the knuckle portion **61** to the surface area of the distal end (e.g. surface **42**) of the finger portion **65** may be determined to an approximation using a formula for half the area of a sphere. For the above dimensions, preferably the surface area of the knuckle portion **61** is in the range between and including about 2.8 times to 11 times greater than the surface area the distal end of the finger portion **65**. More preferably, the surface area of the knuckle portion **61** is in the range between and including about 4 times to 6.2 times greater than the surface area the distal end of the finger portion **65**.

Also as shown in FIGS. 39 and 40, neck portion **56** preferably comprises a cylindrical portion **57** located proximal and adjacent to a spatula portion **67**. As shown, spatula portion **67** comprises a substantially flat anterior surface portion **69** of electrode **25**. In certain embodiments, electrode **25** may comprise one, any combination of, or all of the features of finger portion **65**, knuckle portion **61** and spatula portion **67**.

Turning to use of the devices, similar to device **5b**, device **5c** is particularly useful to a surgeon performing a liver resection. Once the outer capsule of the liver is scored with a dry bovie blade along the planned line of resection the distal tip of tip portion **45** is painted back and forth along the line, with radio frequency power and the flow of fluid **24** on, resulting in coagulation of the liver parenchyma. Once the tissue is coagulated under and around the electrode surface **42** and, as the device **5c** enters a crevice **97**, surface **40**, surface **42** of electrode **25** is used to blunt dissect the coagulated parenchyma. Blunt dissection of the coagulated parenchyma is performed by continuous abrading or splitting apart of the parenchyma with the substantially the same back and forth motion as coagulation and with the device **5c**.

being held substantially in the same orientation as for coagulation of the liver parenchyma. However, with blunt dissection, the surgeon typically applies more force to the tissue. In various embodiments, once the liver parenchyma is coagulated, blunt dissection may be performed with or without the radio frequency power (i.e. on or off) and/or with or without the presence of fluid 24.

5 In addition to liver resections, device 5h are particularly useful to a surgeon performing a laparoscopic cholecystectomy (abbr. "lap chole") for the case of, for instance, either acute cholecystitis or an intrahepatic gallbladder in that the device provides multi-functional uses. More particularly, device 5h is useful to the surgeon 10 for coagulation and dissection of an inflamed serosal layer of tissue 32 between the liver and gallbladder, which may include tough, fibrous, highly vascular connecting tissue between the organs.

15 For coagulation, device 5h may be positioned in at least three different orientations. For the first orientation, as shown in FIG. 43, coagulation may be performed with posterior knuckle surface portion 62 formed by knuckle portion 61. Similar to device 5c, coagulation with device 5h is performed with radio frequency power and the flow of fluid 24 on. Preferably power is applied in the coagulation mode of the generator and at a power level in the range between and including about 10 watts to 60 watts. More preferably, the power level is in the range between and 20 including about 20 watts to 50 watts. Even more preferably, the power level is in the range between and including about 30 watts to 40 watts. With respect to motion of surface portion 62 during coagulation, coagulation may be performed with surface portion 62 stationary, or with a painting motion by moving surface portion 62 back and forth substantially along the longitudinal axis 29 or laterally side to 25 side.

30 For the second orientation, as shown in FIG. 44, coagulation may be performed with a combination of lateral knuckle surface portion 75 formed by knuckle portion 61 and cylindrical surface portion 40, and more specifically a lateral cylindrical surface portion of cylindrical surface portion, of finger portion 65. For the third orientation, as shown in FIG. 45, coagulation may be performed also with another combination of knuckle portion 61 and finger portion 65. As shown in FIG. 35, coagulation may be performed with a posterior cylindrical surface portion of cylindrical surface portion 40 and a posterior surface of knuckle portion 61. In the various orientations, coagulation may be used to stop active bleeding (e.g. such as a spleen injury comprising a splenic capsule tear) or pre-coagulation of tissue before dissection for bloodless surgery.

Where the surgeon has pre-coagulated the tissue 32, the surgeon may dissect the tissue 32 with simultaneous mechanical traction (i.e. the process of drawing or

pulling of the tissue 32 with a mechanical device) with anterior (i.e. front) surface portion 66 of finger portion 65 which is configured, among other things, to engage and restrain tissue 32. More specifically, the surgeon may hook the tissue 32 for dissection against the surface portion 66 of finger portion 65 and apply traction to the tissue 32, then dissect the tissue 32.

5 Since the tissue 32 has been coagulated, dissection may be performed with or without the radio frequency power (i.e. on or off) and/or with or without the presence of fluid 24. Where the tissue 32 is dissected without fluid 24, but with the radio frequency power on and with the generator set to the coagulation mode, the 10 process of dissecting may be referred to as "hook and cook" in the art. While dissecting in this manner is fast, it suffers from the problems of significant arcing, the production of smoke and char, and the possibility of inadvertent perforation of the gall bladder wall. Alternatively, dissecting without the radio frequency power on may eliminate the problems of arcing, the production of smoke and char, and the 15 possibility of inadvertent perforation, but may result in bleeding if the tissue 32 is not sufficiently coagulated. In order to overcome the aforementioned issues, dissection of the tissue 32 with traction may be performed similar to coagulation (i.e. in the presence of both radio frequency power and fluid 24). However, this alternative typically requires more time than "hook and cook".

20 With regards to the sequence of events for dissect the tissue 32 with traction and using the "hook and cook" technique (i.e. without fluid 24), the surgeon first engages the tissue 32 on the surface portion 66 of finger portion 65. The surgeon then applies traction to the engaged tissue 32. Once complete, the surgeon checks for proper position then applies the radio frequency power. Upon application of the 25 radio frequency power, the tissue 32 yields, separates and breaks. The surgeon then turns the radio frequency power off. This process may then be repeated numerous times as the surgeon incrementally dissects tissue 32 along a length in step-wise fashion.

30 Certain embodiments of the invention may be particularly configured for bipolar devices. For example, an exemplary bipolar electrosurgical device of the present invention which may be used in conjunction with the system of the present invention is shown at reference character 5i in FIGS. 46-48. With a bipolar device, the ground pad electrode located on the patient is eliminated and replaced with a 35 second electrical pole as part of the device. An alternating current electrical circuit is then created between the first and second electrical poles of the device. Consequently, alternating current no longer flows through the patient's body to the ground pad electrode, but rather through a localized portion of tissue preferably between the poles of the bipolar device.

In certain embodiments, an exemplary bipolar surgical device of the present invention may comprise, among other things, multiple, substantially parallel, arms. As shown in FIG. 46, electrosurgical device **5i** preferably includes two arms comprising rigid, self-supporting, hollow shafts **17a**, **17b**, a proximal handle 5 comprising mating handle portions **20a**, **20b** and arm tip portions as shown by circles **45a**, **45b**. In this embodiment, shafts **17a**, **17b** preferably comprise thick walled hypo-tubing. In this manner, the shafts **17a**, **17b** have sufficient rigidity to maintain their form during use of the device without kinking or significant bending.

Preferably the arms of device **5i** (comprising shafts **17a**, **17b**) are retained in position relative to each other by a mechanical coupling device comprising a collar **95** and inhibited from separating and/or rotating relative to each other. Collar **95** preferably comprises a polymer (e.g. acrylonitrile-butadiene-styrene or polycarbonate) and is preferably located on the distal portion of the arms. More preferably, the collar **95** is located proximal the distal ends **53a**, **53b** of the shafts **17a**, **17b**. Preferably the collar **95** comprises two apertures **96a**, **96b**, preferably comprising opposing C-shapes, configured to receive a portion of the shafts **17a**, **17b** which are preferably snap-fit therein. Once the collar **95** is connected to the shafts **17a**, **17b**, preferably by a snap-fit connection, the collar **95** may be configured to slide along the length of the shafts **17a**, **17b** as to adjust or vary the location of the collar **95** on the shafts **17a**, **17b**. Alternatively, the location of the collar **95** may be fixed relative to the shafts **17a**, **17b** by welding, for example.

Device **5i** comprises a first arm tip portion **45a** and a second arm tip portion **45b**. As shown, preferably both first arm tip portion **45a** and second arm tip portion **45b** are each individually configured identical to tip portion **45** of device **5a**. As a result, device **5i** has two separate, spatially separated (by empty space) contact elements preferably comprising electrodes **25a**, **25b**.

As shown in FIG. 47, when device **5i** is in use electrodes **25a**, **25b** are laterally spaced adjacent tissue surface **22** of tissue **32**. Electrodes **25a**, **25b** are connected to a source of alternating electrical current and alternating current electrical field is created between electrodes **25a** and **25b**. In the presence of alternating current, the electrodes alternate polarity between positive and negative charges with current flow from the positive to negative charge.

Similar to device **5a**, for device **5i** fluid **24** is communicated from a fluid source **1** within the lumens **23a**, **23b** of the shafts **17a**, **17b** through the lumens **89a**, **89b** and cavities **81a**, **81b** of the sleeves **82a**, **82b** where it is expelled from around and on the surface **42a**, **42b** of the electrodes **25a**, **25b**.

As with use of device **5a**, with use of device **5i** fluid couplings **30a**, **30b** preferably comprising discrete, localized webs and more preferably comprising a

triangular shaped web or bead portion providing a film of fluid 24 is provided between the surface 22 of the tissue 32 and the electrodes 25a, 25a. When the user of electrosurgical device 5i places the electrodes 25a, 25b at a tissue treatment site and moves the electrodes 25a, 25b across the surface 22 of the tissue 32, fluid 24 is 5 expelled around and on the surfaces 42a, 42b of the electrodes 25a, 25b at the distal ends 83a, 83b of the sleeves 82a, 82b and onto the surface 22 of the tissue 32 via couplings 30a, 30b. At the same time, RF electrical energy, shown by electrical field lines 130, is provided to the tissue 32 at the tissue surface 22 and below the tissue surface 22 into the tissue 32 through the fluid couplings 25a, 25b.

10 As with device 5a, the fluid 24, in addition to providing an electrical coupling between the electrosurgical device 5i and the tissue 32, lubricates the surface 22 of the tissue 32 and facilitates the movement of electrodes 25a, 25b across the surface 22 of the tissue 32. During movement of the electrodes 25a, 25b the electrodes 25a, 25b typically slide across the surface 22 of the tissue 32, but also 15 may rotate as the electrodes 25a, 25b move across the surface 22 of the tissue 32. Typically the user of the electrosurgical device 5i slides the electrodes 25a, 25b across the surface 22 of the tissue 32 back and forth with a painting motion while using the fluid 24 as, among other things, a lubricating coating. Preferably the thickness of the fluid 24 between the distal end surface of the electrodes 25a, 25b 20 and the surface 22 of the tissue 32 at the outer edge of the couplings 30a, 30b is in the range between and including about 0.05 mm to 1.5 mm. More preferably, the fluid 24 between the distal end surface of the electrodes 25a, 25b and the surface 22 of the tissue 32 at the outer edge of the coupling 30a, 30b is in the range between and including about 0.1 mm to 0.3 mm. Also preferably, in certain embodiments, 25 the distal end tip of the electrode 25 contacts the surface 22 of tissue 32 without any fluid 24 in between.

As shown in FIG. 48, the fluid coupling for device 5i may comprise a conductive fluid bridge 27 between electrodes 25a, 25b which rests on the surface 22 of the tissue 32 and forms a shunt between the electrodes 25a, 25b. Given this 30 scenario, a certain amount of RF energy may be diverted from going into the tissue 32 and actually pass between the electrodes 25a, 25b via the conductive fluid bridge 27. This loss of RF energy may slow down the process of coagulating tissue and producing the desired hemostasis or aerostasis of the tissue.

In order to counteract the loss of energy through bridge 27, once enough 35 energy has entered the bridge 27 to boil the fluid 24 of bridge 27, the loss of RF energy correspondingly decreases with the loss of the bridge 27. Preferably energy is provided into the fluid 24 of the bridge 27 by means of heat dissipating from tissue 32.

Thus, where a high % boiling of the conductive fluid 24 of the bridge 24 is created, the loss of RF energy through the bridge 27 may either be reduced or eliminated because all the fluid 24 of bridge 27 boils off or a large fraction of boiling creates enough disruption in the continuity of the bridge 27 to disrupt the 5 electrical circuit through the bridge 27. Thus, one control strategy of the present invention is to reduce the presence of a conductive fluid shunt by increasing the % boiling of the conductive fluid.

Another embodiment of a bipolar device is shown at 5j in FIGS. 49 and 50. Similar to device 5i, electrosurgical device 5j preferably includes two arms 10 comprising rigid, self-supporting, shafts 17a, 17b, a proximal handle comprising mating handle portions 20a, 20b and first and second arm tip portions as shown by circles 45a, 45b. However, as shown in FIG. 50, unlike device 5i, for device 5j the shafts 17a, 17b may comprise solid rods (i.e. do not have lumens) which provide for electrical connection to a power source but do not have lumens for providing 15 conductive fluid through the sleeves 82a, 82b. Rather conductive fluid 24 is preferably provided by means of a lumen 122 of a separate fluid line 120, preferably comprising either a metal (e.g. stainless steel hypo-tubing) or polymer (e.g. PVC tubing) material, extending distally and substantially parallel to the arms along side shafts 17a, 17b. In order to minimize the risk of clogging of the lumen 122 at the 20 distal end outlet opening 124 of the fluid line 120, as shown, preferably the distal end 126 of the fluid line 120 is located proximal and adjacent to the distal end of the device 5j and more preferably, proximal to spherical surface portions 42a, 42b of electrodes 25a, 25b, or other tissue treating surfaces of electrodes as the electrode configurations vary.

25 Also as shown for device 5j, the outlet opening 124 for the fluid line 120 is preferably spaced uniformly between electrodes 25a, 25b such that conductive fluid 24 expelled from the outlet opening 124 may form a fluid coupling comprising the a bridge 27 between the tissue surface 22 and the surface 42a, 42b of each of the electrodes 25a, 25b. If a collar 95 is used with device 5j preferably the collar 30 contains a third C-shaped aperture to accommodate fluid line 120 there through.

In certain embodiments, at least a portion of the length of the two arms (comprising the shafts 17a, 17b and sleeves 82a, 82b) or the two arms and fluid line 120 of device 5j may be located and housed within the cavity 132, typically a lumen, of an elongated hollow tubular enclosure 128 as shown in FIG. 49. The elongated 35 tubular enclosure 128 may or may not be connected to the handle portions 20a, 20b. Where the tubular enclosure is not connected to the handle portions 20a, 20b, similar to collar 95, the tubular enclosure 128 may be configured to slide along the length of the shafts 17b, 17c as to adjust or vary the location of the enclosure 128 on

the shafts 17a, 17b or, alternatively, may be fixed relative to the shafts 17a, 17b by welding, for example.

The elongated tubular enclosure 128 may comprise, for example a wrapping, such as shrink wrap polymer film or shrink wrap polymer tubing, which may be 5 formed and located with the surface of cavity 132 against insulators 90a, 90b upon the application of heat thereto. In this manner, the elongated members shafts 17a, 17b or the shafts 17a, 17b and fluid line 120, are retained in position relative to each other and inhibited from separating relative to each other.

Another embodiment of a bipolar device is shown at 5k in FIGS. 51-53. As 10 shown in FIGS. 51 and 53, electrosurgical device 5k preferably includes a housing comprising mating handle portions 20a, 20b and mating elongated shaft portions 134a, 134b forming a hollow shaft. As best shown in FIG. 51, shaft portions 134a, 134b, preferably comprise two semi-circular elongated portions which are connected to handle portions 20a, 20b, respectively, preferably as part of a unitary (i.e. single 15 piece) polymer molding.

As best shown in FIG. 53, electrodes 25a, 25b are preferably assembled directly with shaft portions 134a, 134b adjacent the distal end of shaft portions 134a, 134b. As shown, preferably electrodes 25a, 25b are mechanically assembled adjacent the distal end of shaft portions 134a, 134b via a spool configuration. More 20 specifically, preferably electrodes 25a, 25b comprise locking portions comprising proximal circular flange portions 136a, 136b and distal circular flange portions 138a, 138b separated and connected by circular spindles 140a, 140b there between which form the respective spool configurations.

The circular recesses 142a, 142b formed between the proximal circular 25 flange portions 136a, 136b and distal circular flange portions 138a, 138b provides a receptacle for receiving semi-circular interlocking tab portions 144a, 144b of distal end portions 146a, 146b of shaft portions 134a, 134b.

During assembly, the interlocking tab portions of one of the shaft portions are first located in a portion of the recesses 142a, 142b of electrodes 25a, 25b. In 30 other words, for example, electrodes 25a, 25b may be first assembled with semi-circular interlocking tab portions 144a of distal end portion 146a of shaft portion 134a which then occupy a first semi-circular portion of circular recesses 142a, 142b. Then, once the electrodes 25a, 25b have been properly seated with respect to the first shaft portion, here 134a, the interlocking tab portions of the second shaft 35 portion, here 144b of shaft 134b, are located in the remaining semi-circular portion of circular recesses 142a, 142b. After the electrodes 25a, 25b have been properly seated with respect to both shaft portions 134a, 134b and all remaining components are properly located, the shaft portions 134a, 134b and handle portions 20a, 20b

may be assembled to one another by use of, for example an adhesive (e.g. cyanoacrylate) or welding.

As best shown in FIG. 53, electrodes **25a**, **25b** of device **5k** preferably comprise spherical portions **43a**, **43b** and a corresponding spherical surface portions **42a**, **42b** located at the distal end of the device which provided a smooth, blunt contour outer surface. More specifically, as shown, the spherical portions **43a**, **43b** and spherical surface portion **42a**, **42b** further provide a domed, hemisphere (i.e. less than a full sphere) and hemispherical surface portion comprising preferably about 180 degrees. Also as shown in FIG. 53, electrodes **25a**, **25b** preferably also 10 comprise cylindrical portions **39a**, **39b** and a corresponding cylindrical surface portions **40a**, **40b** located proximal and adjacent to the spherical portions **43a**, **43b** and spherical surface portions **42a**, **42b**, respectively.

Electrodes **25a**, **25b** of device **5k** are preferably coupled to the generator **6** via wire conductors **38a**, **38b** of insulated wires **21a**, **21b**. At their distal ends, 15 conductors **38a**, **38b** may be coupled to electrodes **25a**, **25b** by means of first being inserted into the lumens **148a**, **148b** of hollow metal tubes **150a**, **150b**, such as hypo-tubes, then crimping the tubes **150a**, **150b**. The tubes **150a**, **150b** are then preferably inserted and retained in proximal end receptacles **152a**, **152b** of electrodes **25a**, **25b** by an interference fit. Alternatively, tubes **150a**, **150b** may be 20 eliminated and wire conductors **38a**, **38b** may be coupled to electrodes **25a**, **25b** by welding, soldering, mechanical fasteners or other suitable methods.

For device **5k** conductive fluid **24** is preferably provided by means of a lumen **122** of a separate fluid line **120**, preferably comprising either a metal (e.g. stainless steel hypo-tubing) or polymer (e.g. PVC tubing) material, extending 25 distally and substantially parallel within the lumen of the shaft comprising shaft portions **134a**, **134b**.

Similar to device **5j**, in order to minimize the risk of clogging of the lumen **122** at the distal end outlet opening **124** of the fluid line **120**, as shown, preferably the distal end **126** of the fluid line **120** is located proximal to the distal end of the 30 device **5k** and more preferably, proximal to spherical surface portions **42a**, **42b** and cylindrical surface portions **40a**, **40b** of electrodes **25a**, **25b**, or other tissue treating surfaces of electrodes as the electrode configurations vary.

Also similar to device **5j**, for device **5k** the outlet opening **124** for the fluid line **120** is preferably spaced uniformly between electrodes **25a**, **25b** such that 35 conductive fluid **24** expelled from the outlet opening **124** may form a fluid coupling comprising the a bridge **27** between the tissue surface **22** and the surface **42a**, **42b** of each of the electrodes **25a**, **25b**.

The effect of the bipolar devices of the present invention on tissue may be varied by changing the separation distance between the contact elements.

Consequently, as shown in FIG. 54, in contrast to certain other embodiments which the separation distance is unadjustable, bipolar device **5l** provides an adjustment 5 mechanism for changing the separation distance (either increasing or decreasing) between the electrodes **25a**, **25b**. As shown in FIG. 54, the changing of the separation distance between the electrodes **25a**, **25b** is provided by a scissors type adjustment mechanism with two arms **117a**, **117b** hinged relative to one another in the middle on a pivot **110** preferably comprising a pin. Device **5l** may also comprise 10 a latching mechanism **111** which incrementally fixes the position of the electrodes **25a**, **25b** relative to one another during tissue treatment by increasing or decreasing the separation distance.

Furthermore, as shown, the arms **117a**, **117b** themselves are preferably hinged on pivots **110a** and **110b**, also preferably comprising pins, which divide the 15 arms **117a**, **117b** into proximal arm portions **118a**, **118b** and distal arm portions **112a**, **112b**. Distal arm portions **112a**, **112b** are preferably connected by a linkage **113** which keeps distal arm portions **112a**, **112b** and electrodes **25a**, **25b** substantially parallel to one another with use of the device **5l**. As shown, linkage 20 **113** comprises a bar **114** fixed to distal arm portion **112b** and having an elongated opening **116** therein. Linkage also comprises a pin **115** fixed to distal arm portion **112a** which moves along and within the opening **116** during use of the device **5l** with the changing of the separation distance between electrodes **25a**, **25b**. For device **5l**, tip portions **45a**, **45b** may particularly comprise the configuration disclosed with device **5i**.

25 Another embodiment of a bipolar device is shown at **5m** in FIGS. 55-58. As best shown in FIGS. 55 and 56 and similar to device **5i**, electrosurgical device **5m** preferably includes two stationary, immobile arms comprising rigid, self-supporting, hollow shafts **17a**, **17b**. Shafts **17a**, **17b** for device **5m** preferably comprise thick walled hypo-tubing providing sufficient rigidity to maintain their form during use of 30 the device without kinking or significant bending. In certain embodiments, shafts **17a**, **17b** may be hand malleable.

35 As shown throughout FIGS. 55-58 and similar to device **5i**, preferably the arms of device **5m** (comprising shafts **17a**, **17b**) are retained in position relative to each other by a mechanical coupling device comprising a collar **95** and inhibited from separating relative to each other. Also as shown throughout FIGS. 55-58, collar **95** is preferably located on a distal portion of the arms. More preferably, the collar **95** is located adjacent the distal ends **53a**, **53b** of the shafts **17a**, **17b**. As best shown in FIGS. 57 and 58, preferably the collar **95** comprises two apertures **96a**,

96b, shown as comprising C-shapes, configured to receive a distal end portion of the shafts arms. Once the collar 95 is mechanically connected to the shafts 17a, 17b, preferably by a snap-fit or slide-through connection, the location of the collar 95 may be further fixed relative to the shafts 17a, 17b by, for example, adhesive bonding the collar 95 to shaft insulators 90a, 90b. Such adhesive bonding may be accomplished, for example, either by use of a separate adhesive or autogenic bonding of the collar 95 to the insulators 90a, 90b by, for example, welding such as ultrasonic welding.

10 Collar 95 comprises an electrically insulating (dielectric) material. In some embodiments, the electrically insulating material for collar 95 may comprise a polymer, either thermoplastic or thermoset, reinforced or unreinforced, filled or unfilled. Exemplary polymer materials include, but are not limited to, polyacetal (POM), polyamide (PA), polyamideimide (PAI), polyetheretherketone (PEEK), polyetherimide (PEI), polyethersulfone (PES), polyimide (PI), polyphenylenesulfide (PPS), polyphthalamide (PPA), polysulfone (PSO), polytetrafluoroethylene (PTFE) and syndiotactic polystyrene (SPS). More preferably, the electrically insulating polymer comprises either a liquid crystal polymer and, more particularly, an aromatic liquid crystal polyester which is reinforced with glass fiber, such as Vectra® A130 from Ticona, or Ultem® 10% glass filled polyetherimide from the 15 General Electric Company. Exemplary reinforcement materials for polymers include, but are not limited to, glass fibers and boron fibers. Exemplary filler materials for polymers include mica, calcium carbonate and boron nitride. Reinforcement materials for the polymer material may be preferable for increased strength while filler materials may be preferable for increased heat resistance and/or 20 thermal conductivity. Still other electrically insulating materials for collar 95 may a 25 ceramic such as boron nitride.

As discussed above with reference to device 5i and FIG. 48, the fluid coupling to tissue for device 5i may comprise a conductive fluid bridge 27 between electrodes 25a, 25b which rests on the surface 22 of the tissue 32 and forms a shunt 30 between the electrodes 25a, 25b. As discussed above, a certain amount of RF energy may be diverted from going into the tissue 32 and actually pass between the electrodes 25a, 25b via the conductive fluid bridge 27. This loss of RF energy may slow down the process of coagulating tissue and producing the desired hemostasis or aerostasis of the tissue. Also as discussed above, the loss of RF energy through the 35 bridge 27 may either be reduced or eliminated because all the fluid 24 of bridge 27 boils off or a large fraction of boiling creates enough disruption in the continuity of the bridge 27 to disrupt the electrical circuit through the bridge 27. Thus, as indicated above one control strategy of the present invention is to reduce the

presence of a conductive fluid shunt by increasing the % boiling of the conductive fluid.

Rather than increasing the % boiling of the conductive fluid bridge 27 to reduce the presence of a fluid shunt between the electrodes 25a, 25b, in certain

5 applications it may be advantageous to provide the electrosurgical device with a dam between the electrodes 25a, 25b which reduces, and preferably prevents, the formation of the conductive fluid bridge 27 between the electrodes 25a, 25b.

As best shown in FIGS. 57 and 58, collar 95 of device 5m preferably further includes a substantially flat, blade-shaped electrical insulator spacer portion 154

10 located laterally between the electrodes 25a, 25b. In addition to keeping the electrodes 25a, 25b separated at a predetermined minimum separation distance (as dictated by the thickness of spacer portion 154), spacer portion 154 also provides a dam between electrodes 25a, 25b which reduces, and preferably prevents, the formation of the conductive fluid bridge 27 between the electrodes 25a, 25b.

15 Also as best shown in FIGS. 57 and 58, the distal end surface 156 of spacer portion 154 preferably follows the contour of the adjacent distal end surfaces 158a, 158b of the electrodes 25a, 25b such that the distal end surface 156 of spacer portion 154 is substantially flush, and preferably flush, with the adjacent distal end surfaces 158a, 158b of electrodes 25a, 25b. In this manner, the spacer portion 156 and the electrodes 25a, 25b are better configured to slide along the surface of tissue given there are no raised or recessed edges created between the distal end surface 156 of spacer portion 154 and the adjacent distal end surfaces 158a, 158b of the electrodes 25a, 25b which could impair sliding movement.

Similar to device 5c, electrodes 25a, 25b of device 5m are preferably assembled adjacent the distal ends 53a, 53b of shafts 17a, 17b by connector portions, preferably comprising shank portions 46a, 46b which connect the remainder of the electrodes 25a, 25b to shafts 17a, 17b. Among other things, the connector portion of the electrodes 25a, 25b are preferably configured to form a connection with a mating connector portion of the shafts 17a, 17b. Also similar to device 5c, preferably shank portions 46a, 46b of device 5m are configured to extend into cavities 50a, 50b of shafts 17a, 17b which comprise cylindrical receptacles and provide the mating connector portions for shank portions 46a, 46b. Also similar to device 5c, preferably surfaces 48a, 48b of shank portions 46a, 46b of device 5m are configured to mate against and form an interference fit with surfaces 52a, 52b of cavities 50a, 50b to provide the connection.

Similar to device 5c, shank portions 46a, 46b of device 5m are preferably cylindrical and located proximal and adjacent to neck portions 56a, 56b. As best shown in FIGS. 57 and 58, neck portions 56a, 56b comprise cylindrical portions

57a, 57b preferably having a cross-sectional dimension, here diameter, greater than the cross-sectional dimension, here also diameter, of shank portions 46a, 46b. In this manner, similar to device 5c, in certain embodiments, the proximal end of neck portions 56a, 56b of device 5m may be located adjacent and in contact with distal 5 ends 53a, 53b of shafts 17a, 17b.

As best shown in FIGS. 57 and 58, similar to recess 64 of device 5c, electrodes 25a, 25b of device 5m preferably comprises at least one recess 63a, 63b which provides an elongated fluid flow channel and outlet for the distribution of fluid 24.

10 Electrodes 25a, 25b of device 5m preferably comprise an enlarged head portion. Each enlarged head portion preferably comprises a side hemispherical portion 160a, 160b with a hemispherical surface comprising preferably about 180 degrees. As best shown in FIGS. 57 and 58, preferably the hemisphere portions 160a, 160b are arranged facing away from one another in outwardly facing opposing 15 relation on opposite sides of the device. The hemispherical portions 160a, 160b are preferably located laterally of transversely orientated cylindrical medial transition portions 162a, 162b which preferably provide the smooth transition between the hemispherical portions 160a, 160b and spacer portion 154 of collar 95. As shown electrodes 25a, 26b and spacer portion 154 may comprise abutting flat surfaces 20 164a, 164b which are arranged facing towards and opposing one another. In alternative embodiments, medial transition portions 162a, 162b of electrodes 25a, 25b may be eliminated resulting in the head portion of electrodes 25a, 25b comprising just hemispherical portions 160a, 160b with a hemispherical surfaces comprising preferably about 180 degrees.

25 In certain embodiments spacer portion 154 may comprise a thickness in the range between and including about 0.5 mm to 10 mm, or in any 0.1 mm increment or range therebetween, to provide a separation distance between the electrodes 25a, 25b of such. For example, spacer portion 154 comprises a thickness in the range between and including about 1.5 mm to 4 mm.

30 As an alternative to adjusting the separation distance between the electrodes 25a, 25b by changing the thickness of the spacer portion 154, portions of electrodes 25a, 25b may be coated with an thin (e.g. 0.01 to 0.5 mm) electrically insulating coating comprising, for example, a polymer or ceramic material. As shown in FIGS. 59-62, a portion of the electrodes 25a, 25b for device 5n, here the neck portions 56a, 35 56b, medial transition portions 162a, 162b and approximately half of each hemisphere portion 160a, 160b of the enlarged head portion are shown with an electrically insulating coating 166 thereon. As a result, the active tissue treating electrode surface is now limited to about quarter-sphere surfaces 168a, 168b and the

separation distance between the tissue treating electrode surfaces has been increased by the thickness of the medial transition portions **162a**, **162b** of electrodes **25a**, **25b**.

Another embodiment of a bipolar device is shown at **5o** in FIGS. 63-64.

Similar to device **5n**, the active tissue treating electrode surface of electrodes **25a**,

5 **25b** may be limited to about quarter-sphere surfaces **168a**, **168b** (about 90 degrees) with the other surfaces of the electrode extending from the distal end of shaft insulators **90a**, **90b** having electrically insulating coating **166** thereon. However, different from device **5n**, the enlarged head portion of the electrodes **25a**, **25b** of device **5o** comprise two substantially circular spheres (i.e. except where they join to 10 neck portions **56a**, **56b**). The spheres may have any suitable diameter. However, the spheres preferably have a diameter in the range between and including about 0.5 mm to about 7 mm. More preferably the spheres have a diameter in the range between and including about 1.0 mm to about 4 mm. Even more preferably, the spheres have a diameter in the range between and including about 1.5 mm to about 3 15 mm. Where coating **166** is not located thereon, the active electrical surface of the spheres is about 260 degrees.

Also different from device **5n**, collar **95** of device **5o** does not include spacer portion **154**. With device **5o**, electrodes **25a**, **25b** are separated by an air gap therebetween. As a result, as shown in FIG. 64, when electrodes **25a**, **25b** of device 20 **5o** are pressed against the surface **22** of tissue **32** and the tissue **32** against electrodes **25a**, **25b** compresses and forms recesses **170a**, **170b**, device **5o** is configured to allow tissue **32** located adjacent the gap **172** between the electrodes **25a**, **25b** to form a tissue protuberance **174** there into with downward slopes into the recess **170a**, **170b**. Since fluid **24** which may exist between the electrodes **25a**, **25b** will tend to 25 flow with gravity down the slopes of the tissue protuberance **174** and into the adjoining recesses **170a**, **170b**, the possibility of formation of a conductive fluid bridge **27** between electrodes **25a**, **25b** is reduced. Furthermore, even if a conductive fluid bridge **27** were to form between the electrodes **25a**, **25b** (e.g. where electrodes **25a**, **25b** of device **5o** are not pressed against tissue **32** 30 significantly enough to form recesses **170a**, **170b**, the coating **166** on the inner facing surfaces of the electrodes **25a**, **25b** reduces the possibility such a bridge would be electrified by electrodes **25a**, **25b** directly.

Another embodiment of a bipolar device is shown at **5p** in FIGS. 65-69. As best shown in FIG. 66, the electrodes **25a**, **25b** now comprise a hollow metal tubes. 35 More specifically, the distal end portion of the tubes comprise about a 90 degree bend (within about \pm 5 degrees) forming two right angle elbows and which curves the distal end portions towards each other as they extend distally. Furthermore, the

distal ends of the tubes are arranged facing towards and opposing one another. Consequently, the electrodes 25a, 25b are substantially mirror images of each other.

As shown in FIG. 66, collar 95 has been removed to better show that preferably the electrodes 25a, 25b comprise circular, stainless steel hypo-tubing.

- 5 Where the electrodes 25a, 25b comprise separate pieces from shafts 17a, 17b, electrodes 25a, 25b of device 5p are preferably connected to shafts 17a, 17b by interference fit of the inner diameter of the shafts 17a, 17b with the inner diameter of the electrodes 25a, 25b. However, in order to minimize the number of components and assembly thereof, preferably a single piece of continuous tubing 10 provides both the shaft and the electrode. In other words, as shown, preferably the electrodes 25a, 26b are provided by the same piece of tubing used for shafts 17a, 17b.

As best shown in FIGS. 67-69, preferably device 5p includes a collar 95 which includes an electrical insulator spacer portion 154 located laterally between the electrodes 25a, 25b. Furthermore, spacer portion 154 preferably includes at least one recess 176a, 176b which provides an elongated fluid flow channel and a portion of the fluid passage for the distribution of fluid 24 from openings 178a, 178b. As shown, both the distal end openings 180a, 180b of the tubes and openings 178a, 178b of recesses 176a, 176b are positioned at a location substantially inaccessible to 20 direct contact with tissue or otherwise configured away from direct contact with tissue as to not become occluded by tissue with use of device 5p.

Preferably spacer portion 154 includes protrusions 182a, 182b, and more specifically semi-circular protrusions configured to fit into distal end openings 180a, 180b and at least partially occlude openings 180a, 180b. In this manner electrodes 25a, 25b are retained from movement relative to spacer 154, as well as the rest of collar 95.

In certain embodiments, in order that heat may be transferred away from electrodes 25a, 25b by spacer portion 154, preferably the material for collar 95 has a thermal conductivity k_{tc} at 300°K (Kelvin) equal or greater than about 0.01 30 watt/cm°K. More preferably, the material for collar 95 has a thermal conductivity k_{tc} at 300°K (Kelvin) equal or greater than about 0.16 watt/cm°K. Even more preferably, the material for collar 95 has a thermal conductivity k_{tc} at 300°K (Kelvin) equal or greater than about 0.35 watt/cm°K.

The use of openings 178a, 178b of recesses 176a, 176b for the distribution 35 of fluid 24 may be preferred to at least one fluid exit opening 184a, 184b which may be provided on the distal end side of electrodes 25a, 25b proximal to the distal end (see FIG. 66), particularly in deep tissue crevices where tissue can occlude fluid flow from openings 184a, 184b. However, as shown in FIGS. 70-71 for device 5q,

where fluid exit openings 184a, 184b are positioned at a location substantially inaccessible to direct contact with tissue or otherwise configured away from direct contact with tissue as to not become occluded by tissue (such as slots shown on the inner side wall of the electrodes 25a, 25b adjacent the inner radius of the elbow 5 bend and distal end of the electrode), the openings 184a, 184b may be equally effective as openings 178a, 178b.

More particularly, as shown, openings 184a, 184b in FIG. 70-71, for example, are closer to the inner radius of elbow bend than the other radius of the elbow bend, which aids in reducing occlusion by tissue. However, in other 10 embodiments, the fluid exit openings 184a, 186a may be closer to the outer radius of elbow bend than the inner radius of the elbow bend, as shown in FIG. 66. Still, in other embodiments, the fluid exit openings 184a, 186a may be equidistant the outer radius of elbow bend and the inner radius of the elbow bend, as shown in FIG. 73.

Another embodiment of a bipolar device is shown at 5r in FIGS. 72-73. As 15 shown the distal end of spacer portion 154 includes a recess 186 configured to allow tissue 32 to form a tissue protuberance 174 there into to reduce the possibility of formation of a conductive fluid bridge 27 between electrodes 25a, 25b as discussed above.

One or more of the devices of the present invention may include assemblies 20 which control power and/or fluid flow to the tissue treating portion of the device. The ability to control the flow of fluid from the device may provide certain advantages over a device not so equipped. These advantages include reducing the amount of fluid at the tissue treatment site and the likelihood of having to apply suction to the treatment site to remove fluid.

25 For device 5s in FIGS. 74-79, a single multi-positional, multi-functional switch and valve assembly 190 comprises a switch button 192. Button 192 protrudes through an aperture 194 formed in handle portions 20a, 20b. Button 192 is preferably integrally connected via a single piece polymer molding to a proximally extending switch arm 196 which provides a portion of a fluid flow 30 control mechanism, preferably formed when interacting with handle portion 20a to turn the flow of fluid 24 to the tissue treating portion of the device on (full flow, i.e. unregulated flow at full flow rate through the tubing) and off (no flow).

More specifically, the fluid flow control mechanism of switch/valve assembly 190 is provided with the changing the separation distance between the proximal end portion 198 of switch arm 196 and wall section 200 of handle portion 20a as switch arm 196 is moved proximally and distally along track 206 formed and defined by apertures 208 of ribs 210 of handle portion 20a in response to button 192 being moved proximally and distally in switch button aperture 194.

As shown in FIG. 76, fluid line 4b is located between proximal end portion 198 of switch arm 196 and wall section 200 of handle portion 20a. As button 192 and switch arm 196 are moved proximally by hand force, thus decreasing separation distance between proximal end portion 198 of switch arm 196 and wall section 200 of handle portion 20a, fluid line 4b is externally squeezed and compressed therebetween and its lumen correspondingly occluded to decrease, and preferably completely stop, the fluid flow rate. As exhibited by the above fluid flow control mechanism, preferably the mechanism does not make contact with fluid 24, thus reducing the likelihood of inadvertent contamination.

Continuing with FIG. 76, preferably the fluid flow control mechanism of switch/valve assembly 190 comprises a mechanism which holds the arm 196 in a fixed, locked position while compressing and occluding fluid line 4b. As shown, preferably the locking mechanism comprises a locking tab 202 of handle portion 20a which holds arm 196 in its locked rearward position by engaging a distal end portion 204 of switch arm 196.

Locking tab 202 is disengaged from distal end portion 204 of switch arm 196 by depressing button 192. Upon depressing button 192, the distal end portion 204 of switch arm also separates from tab 202 and tab 202 disengages from distal end portion 204. As best shown in FIG. 77, simultaneously switch arm 196 is forced distally by the decompression of resilient fluid line 4b such that tab 202 enters detent 212. Preferably switch arm 196 is also forced distally by decompression of a linear spring 228 which biases proximal movement of arm 196 to the switch's off position against fluid line 4b with compression thereof, and, with decompression thereof, helps return the switch 192 to its on position upon arm 196 being disengaged from tab 202. As shown, spring 228 is supported on arm 196 by circular post 234 and is compressed between a flange 238 located at the base of post 234 and one of ribs 210. Upon distal end portion 204 of arm 196 disengaging from tab 202, button 192 and switch arm 196 may travel distally until tab 202 engages the proximal end 214 of detent 212.

Once the flow of fluid 24 has resumed, switch button 192 of switch/valve assembly 190 may now be depressed to activate the flow of electric current to electrodes 25a, 25b. As discussed above, electrodes 25a, 25b are preferably coupled to the generator 6 via wire conductors 38a, 38b of insulated wires 21a, 21b. Here, for example, the active and return electrodes comprise electrodes 25a, 25b.

As shown in FIGS. 78-79, electrode 25a is directly coupled to generator 6 without any additional inclusion of an on/off switch with an associated control circuit therebetween. However, in addition to being directly coupled to generator 6, the electrical coupling of electrode 25b to generator 6 now includes the presence of

two separated electrical contacts 216 and 218 which, in the open position, create an open control circuit between electrode 25b and generator 6. The wiring of this electrical control circuit with the generator 6 is known in the art and discussed briefly below.

5 As best shown in FIGS. 77-79, contacts 216 and 218 are disposed on a platform 222 partially underling switch button 192 and arm 196. As best shown in FIG. 78, contact 216 comprises a domed contact which overlies contact 218. In the open, or undepressed, position, contact 216 remains separated from underlying contact 218 by virtue of the domed configuration of contact 216, thus resulting in an
10 open control circuit between electrode 25b and generator 6. However, when switch button 192 of switch/valve assembly 190 is in its depressed position, post 220 in turn depresses dome contact 216 into contact with contact 218, thus closing the control circuit between electrode 25b and generator 6. The presence of the closed control circuit formed with wire 21c is then sensed by generator 6 through a low
15 voltage sensor which then provides the set power to electrodes 25a, 25b.

When a depression force is removed from switch button 192, contact 216 returns to its pre-depression domed position as a result of its resiliency or elastic memory, thus returning switch button 192 to its undepressed position and reopening the control circuit between electrode 25b and generator 6. The presence of the open
20 control circuit is then sensed by the generator which then stops providing power to electrodes 25a, 25b. Alternatively, where switch button 192 is not used and the physician chooses to activate electrodes 25a, 25b with a foot pedal switch, the set electrical power to the electrodes 25a, 25b only flows directly through contact 218 to complete the electrical circuit.

25 It should be understood that switch/valve assembly 190 is configured such that electrical current cannot be provided to electrodes 25a, 25b while the flow of fluid 24 is off. As shown in FIG. 77, when switch button 192 and switch arm 196 are in their proximal position, post 220 does not overlie domed contact 216. Consequently, if switch button 192 is depressed, post 220 merely makes contact
30 with platform 222 and the electrical circuit between electrodes 25a, 25b and generator 6 remains opened.

35 It should also be understood that in the case of a single main fluid passage which may branch into multiple secondary passages, preferably switch/valve assembly 190 acts on the main fluid passage to reduce complexity. As shown in FIGS. 76-77, preferably switch/valve assembly 190 is located proximal of splitter 240.

In other embodiments one or more of the devices of the present invention may include a separate power switch and fluid flow valve assemblies rather than part

of a single multi-positional switch/valve assembly. As shown in FIGS. 80-81, device **5t** comprises a switch assembly **224** for turning power on and off to the tissue treating portion of the device and a valve assembly **226** for turning fluid flow on (full flow) and off (no flow) to the tissue treating portion of the device.

5 As best shown in FIG. 81, switch button **230** of switch assembly **224** turns fluid flow on and off in substantially the same manner as switch button **192** of switch/valve assembly **190** (i.e. with distal and proximal movement). However, unlike device **5s**, proximal end portion **198** of switch arm **196** of device **5t** includes a roller wheel **236** to aid with compression and decompression of fluid line **4b**.

10 With regards to power, switch button **232** of valve assembly **226** turns power on and off in substantially the same manner as switch button **192** of switch/valve assembly **190** (i.e. in depressed and unpressed positions). However, unlike switch/valve assembly **190**, with valve assembly **226** power can be turned on and off independently of fluid flow. In other words, switch button **232** of valve assembly 15 **226** can be in the power “on” position while switch button **230** of switch assembly **224** is in the fluid flow “off” position. Thus, the device **5t** can be configured to operate as dry electrosurgical device without fluid **24** being provided simultaneously from the tissue treating portion of the device.

15 In yet another embodiment, as shown in FIGS. 82-86, the second valve assembly for turning fluid flow on and off to the tissue treating portion of the device may comprise a roller pinch clamp assembly. As best shown in FIGS. 83-86, device **5u** includes a roller pinch clamp assembly **242** and, more specifically, an inclined ramp roller pinch clamp assembly (as opposed to a parallel acting clamp).

20 As best shown in FIGS. 84-85, the clamp includes a housing provided by handles **20a**, **20b**, a roller wheel **244** having a wheel center axis **246** and a guide pin hub. As shown, the guide pin hub is provided by pair of opposing, integrally formed, cylindrical trunnions **248a**, **248b**, but may also be provided by a separately formed pin. Trunnions **248a**, **248b** are contained within and move along a track **250** preferably provided and defined by opposing trunnion channels **252a**, **252b** formed 25 between wheel upper guide surfaces **254a**, **254b** and wheel lower guide surfaces **256a**, **256b** extending longitudinally and parallel inward from the side wall portions of the handles **20a**, **20b**. As shown, wheel upper guide surfaces **254a**, **254b** are provided by a lip portion of the handles **20a**, **20b** which partially define aperture **258** through which roller wheel partially extends while wheel lower guide surfaces **256a**, 30 **256b** are provided by ribs **260a**, **260b**.

35 Handles **20a**, **20b** also preferably provide tubing guide surfaces **272a**, **272b** which at least a portion of which provide a clamping surface against which plastic tubing **4b** is clamped by roller **244**. As best shown in FIGS. 84-85, tubing guide

surfaces 272a, 272b are provided by ribs 270a, 270b. In use, fluid line 4b is externally squeezed and compressed between the outer perimeter surface 262 of roller wheel 244 and at least a portion of tubing guide surfaces 272a, 272b. In this embodiment, preferably surface 262 is serrated.

5 Trunnions 248a, 248b support the movement of roller wheel 244 in two opposing directions, here proximally and distally, along track 250. As best shown in FIGS. 85-86, the separation distance between the outer perimeter surface 262 of roller wheel 244 and tubing guide surfaces 272a, 272b changes throughout the proximal and distal travel of roller wheel 244 along track 250. More specifically, 10 the separation distance between the outer perimeter surface 262 of roller wheel 244 and tubing guide surfaces 272a, 272b is greater between the outer perimeter surface 262 of roller wheel 244 and distal end portions 274a, 274b of tubing guide surfaces 272a, 272b provided by distal end portions 264a, 264b of ribs 270a, 270b than between the outer perimeter surface 262 of roller wheel 244 and proximal end 15 portions 276a, 276b of tubing guide surfaces 272a, 272b provided by proximal end portions 266a, 266b of ribs 270a, 270b.

As shown in FIGS. 84-85, when axis 246 of roller wheel 244 is opposing distal end portions 274a, 274b of tubing guide surfaces 272a, 272b, preferably the separation distance is configured such that the tubing 4b may be uncompressed and 20 the lumen of tubing 4b completely open for full flow therethrough. Conversely, as shown in FIG. 86, when axis 246 of roller wheel 244 is opposing proximal end portions 276a, 276b of tubing guide surfaces 272a, 272b preferably the separation distance is configured such that the tubing 4b is compressed and the lumen of tubing 4b is completely blocked so that the flow of fluid through tubing 4b is prevented.

25 Distal end portions 274a, 274b of tubing guide surfaces 272a, 272b are separated from proximal end portions 276a, 276b of tubing guide surfaces 272a, 272b by transition surfaces 278a, 278b which are provided by transition rib portion 268a, 268b of ribs 270a, 270b. Preferably compression of tubing initially begins 30 between transition surfaces 278a, 278b and the outer perimeter surface 262 of roller wheel 244 and increases as wheel 244 moves proximally along proximal end portions 276a, 276b of tubing guide surfaces 272a, 272b. With this configuration, consideration may be given to eliminating at least that portion of distal end portions 274a, 274b of tubing guide surfaces 272a, 272b that do not contribute to 35 compression of the tubing 4b. However, given that of distal end portions 274a, 274b of tubing guide surfaces 272a, 272b guide tubing 4b to splitter 240, such may not be desirable.

As shown in FIGS. 84-86, both transition surfaces 278a, 278b and proximal end portions 276a, 276b of tubing guide surfaces 272a, 272b provide sloped

inclining surfaces proximally along their respective lengths which decreases the separation distance between the outer perimeter surface **262** of roller wheel **244** and the tubing guide surfaces **272a**, **272b** as the wheel **244** moves proximally. As shown, preferably the transition surfaces **278a**, **278b** and proximal end portions **276a**, **276b** of tubing guide surfaces **272a**, **272b** have different slopes such that the separation distance decreases at a faster rate along transition surfaces **278a**, **278b** as compared to proximal end portions **276a**, **276b** of tubing guide surfaces **272a**, **272b**. In this manner, compression of tubing **4b** is non-linear along the length of travel of wheel **244** with a majority of the compression occurring between roller wheel **244** and transition surfaces **278a**, **278b**. More preferably, the lumen of tubing **4b** is completely blocked when roller wheel **244** is compressing the tubing **4b** against the proximal portion of transition surfaces **278a**, **278b**, and the added compression of the tubing **4b** along proximal end portions **276a**, **276b** of tubing guide surfaces **272a**, **272b** provides an additional safety to assure complete blocking of the lumen even where there are variations in the tubing, such as the size of the lumen.

It should be realized that, due to the slope of the transition rib portion **268a**, **268b**, as the roller wheel **244** moves proximally relative to transition surfaces **278a**, **278b** the lumen of tubing **4b** is blocked incrementally. Thus, in addition to providing an on/off mechanism, the roller pinch clamp assembly **242** can also be used to regulate the fluid flow rate between two non-zero flow values. It should also be realized that the roller pinch clamp assembly **242** of the device may be used in series conjunction with another roller pinch clamp assembly which is typically provided as part of an IV set (i.e. IV bag, IV bag spike, drip chamber, connecting tubing, roller clamp, slide clamp, luer connector). When used in this manner, the roller pinch clamp assembly of the IV set may be used to achieve a primary (major) adjustment for fluid flow rate, while the roller pinch clamp assembly **242** of the device may be used to achieve a secondary (more precise minor) adjustment for the fluid flow rate.

In another embodiment, as shown in FIGS. 87-89 for device **5v**, the roller pinch clamp assembly **242** may include a cover **280** which at least partially closes aperture **258** and/or conceals roller wheel **244**. Among other things, cover **280** reduces the possibility of undesirable foreign fluid (e.g. blood and other bodily fluids) from entering into the confines of handle **20a**, **20b** through aperture **258**. Furthermore, cover **280** reduces the exposure of the internal mechanics of the roller pinch clamp assembly **242**. In this manner, cover **280** reduces the possibility of foreign objects (e.g. practitioner's rubber gloves) from entering into the confines of handle **20a**, **20b** through aperture **258** and getting snagged, for example, between the trunnions **248a**, **248b** and track **250**.

As shown in FIGS. 88-89, preferably cover 280 overlies and moves distally and proximally with roller wheel 244, and is configured to provide a switch button portion 282 when wheel 244 is covered within semi-circular receptacle 284 and inaccessible to direct manipulation. Preferably cover 280 is configured to

5 substantially close aperture 258 regardless of the position of the wheel 244, preferably by means of a distal shield portion 286 and a proximal shield portion 288. Preferably, distal shield portion 286 and a proximal shield portion 288 each have a length equal to or greater than the length of aperture 258 minus the length of switch button portion 282.

10 Also as shown, preferably cover 280 comprises a distal guide portion 290 and a proximal guide portion 292 located beneath distal shield portion 286 and a proximal shield portion 288 on opposing sides of wheel 244. As shown proximal guide portion 292 and distal shield portion 286 both comprise rectangular guide pins and preferably move along a track 250 similarly to wheel 244. Wheel 244 partially

15 extends into receptacle 284 which has a slightly larger diameter than wheel 244.

With movement of switch button portion 282 proximally by a proximal directed force apply by, for example, a finger, the inner surface 294 of distal guide portion 290 makes contact with surface 262 of wheel 244 and pushes wheel proximally. Conversely, with movement of switch button portion 282 distally by a

20 distally directed force apply by, for example, a finger, the inner surface 296 of proximal guide portion 292 makes contact with outer surface 262 of wheel 244 and pushes wheel distally. In this embodiment, the surface 262 of wheel 244 is preferably smooth and wheel 244 preferably comprises a self-lubricating polymer material such as polyacetal.

25 In another embodiment, as shown in FIGS. 90-91 for device 5w, the switch button portion 282 of cover 280 may include side portions 298 which cover the opposing sides of wheel 244. However, unlike embodiment 5v, a portion of the cover 280 for device 5w is not contained in or directly guided by track 250 as distal guide portion 290 and proximal guide portion 292 have been eliminated. While the

30 cover 280 for embodiment 5w still applies directional force to wheel 244 to move wheel 244, cover 280 now is joined to wheel 244 and conveyed along track 250 by trunnions 248a, 248b of wheel 244. As shown, cover 280 includes two opposing C-shaped apertures 300 which provided wheel hub receptacles for trunnions 248a, 248b. As shown, trunnions 248a, 248b are located in apertures 300.

35 Thus, with movement of switch button portion 282 proximally by a proximal directed force, the inner surface 302 of cover 280 defining apertures 300 makes contact with cylindrical side surface 304 of trunnions 248a, 248b and pushes wheel proximally. Conversely, with movement of switch button portion 282 distally by a

distally directed force, the inner surface 302 of cover 280 defining apertures 300 also makes contact with cylindrical side surface 304 of trunnions 248a, 248b and pushes wheel distally.

In another embodiment, as shown in FIGS. 92-93 for device 5x, the switch 5 button portion 282 of cover 280 has been eliminated. Thus, roller wheel 244 is now exposed and may be acted on directly rather than through switch button portion 282.

While the various embodiments of switch assemblies described above have predominately been described with reference to bipolar devices, it should be understood that the various switch assemblies may be equally adaptable to other 10 fluid-assisted medical devices such as the monopolar devices of the present invention.

Bipolar devices 5i-5x are particularly useful as non-coaptive tissue sealers given they do not grasp tissue. Devices 5i-5x are particularly useful to surgeons to achieve hemostasis after dissecting through soft tissue as part of hip or knee 15 arthroplasty. The tissue treating portions can be painted over the raw, oozing surface 22 of tissue 32 to seal the tissue 32 against bleeding, or focused on individual larger bleeding vessels to stop vessel bleeding.

Devices 5i-5x are also useful to stop bleeding from the surface of cut bone tissue as part of any orthopaedic procedure that requires bone to be cut. Bipolar 20 devices 5i-5x are particularly useful for these applications over a monopolar device 5a as a much greater surface area 22 of tissue 32 may be treated in an equivalent period of time and with better controlled depth of the treatment.

As is well known, bone, or osseous tissue, is a particular form of dense 25 connective tissue consisting of bone cells (osteocytes) embedded in a matrix of calcified intercellular substance. Bone matrix mainly contains collagen fibers and the minerals calcium carbonate, calcium phosphate and hydroxyapatite. Among the many types of bone within the human body are compact bone and cancellous bone. Compact bone is hard, dense bone that forms the surface layers of bones and also the shafts of long bones. It is primarily made of haversian systems which are covered by 30 the periosteum. Compact bone contains discrete nutrient canals through which blood vessels gain access to the haversian systems and the marrow cavity of long bones. For example, Volkmann's canals which are small canals found in compact bone through which blood vessels pass from the periosteum and connect with the blood vessels of haversian canals or the marrow cavity. Bipolar devices as disclosed 35 herein may be particularly useful to treat compact bone and to provide hemostasis and seal bleeding vessels (e.g. by shrinking to complete close) and other structures associated with Volkmann's canals and Haversian systems.

In contrast to compact bone, cancellous bone is spongy bone and forms the bulk of the short, flat, and irregular bones and the ends of long bones. The network of osseous tissue that makes up the cancellous bone structure comprises many small trabeculae, partially enclosing many intercommunicating spaces filled with bone marrow. Consequently, due to their trabecular structure, cancellous bones are more amorphous than compact bones, and have many more channels with various blood cell precursors mixed with capillaries, venules and arterioles. Bipolar devices as disclosed herein may be particularly useful to treat cancellous bone and to provide hemostasis and seal bleeding structures such as the above micro-vessels (i.e. 5 capillaries, venules and arterioles) in addition to veins and arteries. Such devices may be particularly useful for use during orthopaedic knee, hip, shoulder and spine 10 procedures (e.g. arthroplasty).

During a knee replacement procedure, the condyle at the distal epiphysis of the femur and the tibial plateau at the proximal epiphysis of the tibia are often cut 15 and made more planer with saw devices to ultimately provide a more suitable support structure for the femoral condylar prosthesis and tibial prosthesis attached thereto, respectively. The cutting of these long bones results in bleeding from the cancellous bone at each location. In order to seal and arrest the bleeding from the cancellous bone which has been exposed with the cutting of epiphysis of each long 20 bone, the bipolar devices disclosed herein may be utilized. Thereafter, the respective prostheses may be attached.

Turning to a hip replacement procedure, the head and neck of the femur at the proximal epiphysis of the femur is removed, typically by cutting with a saw device, and the intertrochanteric region of the femur is made more planer to provide a 25 more suitable support structure for the femoral stem prosthesis subsequently attached thereto. With respect to the hip, a ball reamer is often used to ream and enlarge the acetabulum of the innominate (hip) bone to accommodate the insertion of an acetabular cup prosthesis therein, which will provide the socket into which the head of the femoral stem prosthesis fits. The cutting of the femur and reaming of the 30 hip bone results in bleeding from the cancellous bone at each location. In order to seal and arrest the bleeding from the cancellous bone which has been cut and exposed, the bipolar devices disclosed herein may be utilized. Thereafter, as with the knee replacement, the respective prostheses may be attached.

The bipolar devices disclosed herein may be utilized for treatment of 35 connective tissues, such as for shrinking intervertebral discs during spine surgery. Intervertebral discs are flexible pads of fibrocartilaginous tissue tightly fixed between the vertebrae of the spine. The discs comprise a flat, circular capsule roughly an inch in diameter and about 0.25 inch thick, made of a tough, fibrous

outer membrane called the annulus fibrosus, surrounding an elastic core called the nucleus pulposus.

Under stress, it is possible for the nucleus pulposus to swell and herniate, pushing through a weak spot in the annulus fibrosus membrane of the disc and into the spinal canal. Consequently, all or part of the nucleus pulposus material may protrude through the weak spot, causing pressure against surrounding nerves which results in pain and immobility.

The bipolar devices disclosed herein may be utilized to shrink protruding and herniated intervertebral discs which, upon shrinking towards normal size, reduces the pressure on the surrounding nerves and relieves the pain and immobility. The devices disclosed herein may be applied via posterior spinal access under surgeon control for either focal shrinking of the annulus fibrosus membrane.

Where a intervertebral disc cannot be repaired and must be removed as part of a discectomy, the devices disclosed herein may be particularly useful to seal and arrest bleeding from the cancellous bone of opposing upper and lower vertebra surfaces (e.g. the cephalad surface of the vertebral body of a superior vertebra and the caudad surface of an inferior vertebra). Where the disc is removed from the front of the patient, for example, as part of an anterior, thoracic spine procedure, the devices disclosed herein may also be particularly useful to seal and arrest bleeding from segmental vessels over the vertebral body.

The bipolar devices disclosed herein may be utilized to seal and arrest bleeding of epidural veins which bleed as a result of the removal of tissue around the dural membrane during, for example a laminectomy or other neurosurgical surgery. The epidural veins may start bleeding when the dura is retracted off of them as part of a decompression. Also during a laminectomy, the devices disclosed herein, may be used to seal and arrest bleeding from the vertebral arch and, in particular the lamina of the vertebral arch.

One or more of the features of the previously described system can be built into a custom RF generator. This embodiment can provide one or more advantages. For example, this type of system can save space and reduce overall complexity for the user. This system can also enable the manufacturer to increase the power delivered into low impedance loads, thereby further reducing the time to achieve the desired tissue effects. This changes the curve of FIG. 5, by eliminating or reducing the slope of the low impedance ramp **28a** of power versus impedance.

Alternatively, for situations where the high impedance ramp **28b** may be exceeded with use of the devices of the present invention, it may be desirable to provide an impedance transformer **224** in a series circuit configuration between the electrode(s) of the device **5** and the power output of generator **6**. Consequently, the

impedance transformer 224 may be provided with the device 5, the generator 6 or any of the wire connectors (e.g. wire 21) connecting device 5 and generator 6.

Impedance transformer 224 is configured to match the load impedance provided to generator 6 such that it is within the working range of the generator 6 and, more

5 preferably in the working range between the low and high cut-offs.

To effectively treat thick tissues, it can be advantageous to have the ability to pulse the RF power on and off. Under some circumstances, the temperature deep in tissue can rise quickly past the 100 °C desiccation point even though the electrode/tissue interface is boiling at 100 °C. This manifests itself as “popping,” as

10 steam generated deep in the tissue boils too fast and erupts toward the surface. In one embodiment of the invention, a switch is provided on the control device or custom generator to allow the user to select a “pulse” mode of the RF power.

Preferably, the RF power system in this embodiment is further controlled by software.

15 In some embodiments, it can be desirable to control the temperature of the conductive fluid before it is released from the electrosurgical device. In one embodiment, a heat exchanger is provided for the outgoing saline flow to either heat or chill the saline. The heat exchanger may be provided as part of the electrosurgical device or as part of another part of the system, such as within the

20 enclosure 14. Pre-heating the saline to a predetermined level below boiling reduces the transient warm-up time of the device as RF is initially turned on, thereby reducing the time to cause coagulation of tissue. Alternatively, pre-chilling the saline is useful when the surgeon desires to protect certain tissues at the electrode/tissue interface and treat only deeper tissue. One exemplary application of

25 this embodiment is the treatment of varicose veins, where it is desirable to avoid thermal damage to the surface of the skin. At the same time, treatment is provided to shrink underlying blood vessels using thermal coagulation. The temperature of the conductive fluid prior to release from the surgical device can therefore be controlled, to provide the desired treatment effect.

30 In another embodiment, the flow rate controller is modified to provide for a saline flow rate that results in greater than 100% boiling at the tissue treatment site. For example, the selection switch 12 of the flow rate controller 11 (shown in FIG. 1) can include settings that correspond to 110%, 120% and greater percentages of boiling. These higher settings can be of value to a surgeon in such situations as

35 when encountering thick tissue, wherein the thickness of the tissue can increase conduction away from the electrode jaws. Since the basic control strategy neglects heat conduction, setting for 100% boiling can result in 80% of 90% boiling, depending upon the amount of conduction. Given the teachings herein, the switch of

the flow rate controller can accommodate any desirable flow rate settings, to achieve the desired saline boiling at the tissue treatment site.

Some embodiments of the invention can provide one or more advantages over current electrosurgical techniques and devices. For example, the invention 5 preferably achieves the desired tissue effect (for example, coagulation, cutting, and the like) in a fast manner. In a preferred embodiment, by actively controlling the flow rate of saline, both in quantity (Q vs. P) and location (for example, using gutters to direct fluid distally to tissue, using holes to direct flow of fluid, or other similar methods) the electrosurgical device can create a hot non-desiccating 10 electrode/tissue interface and thus a fast thermally induced tissue coagulation effect.

The use of the disclosed devices can result in significantly lower blood loss during surgical procedures such as liver resections. Typical blood loss for a right hepatectomy can be in the range of 500 – 1,000 cubic centimeters. Use of the devices disclosed herein to perform pre-transection coagulation of the liver can 15 result in blood loss in the range of 50 – 300 cubic centimeters. Such a reduction in blood loss can reduce or eliminate the need for blood transfusions, and thus the cost and negative clinical consequences associated with blood transfusions, such as prolonged hospitalization and a greater likelihood of cancer recurrence. Use of the device can also provide improved sealing of bile ducts, and reduce the incidence of 20 post-operative bile leakage, which is considered a major surgical complication.

The invention can, in some embodiments, deliver fast treatment of tissue without using a temperature sensor built into the device or a custom special-purpose generator. In a preferred embodiment, there is no built-in temperature sensor or other type of tissue sensor, nor is there any custom generator. Preferably, the 25 invention provides a means for controlling the flow rate to the device such that the device and flow rate controller can be used with a wide variety of general-purpose generators. Any general-purpose generator is useable in connection with the fluid delivery system and flow rate controller to provide the desired power; the flow rate controller will accept the power and constantly adjust the saline flow rate according 30 to the control strategy. Preferably, the generator is not actively controlled by the invention, so that standard generators are useable according to the invention. Preferably, there is no active feedback from the device and the control of the saline 35 flow rate is "open loop." Thus, in this embodiment, the control of saline flow rate is not dependent on feedback, but rather the measurement of the RF power going out to the device.

For purposes of the appended claims, the term "tissue" includes, but is not limited to, organs (e.g. liver, lung, spleen, gallbladder), highly vascular tissues (e.g. liver, spleen), soft and hard tissues (e.g. adipose, areolar, bone, bronchus-associated

lymphoid, cancellous, chondroid, chordal, chromaffin, cicatricial, connective, elastic, embryonic, endothelial, epithelial, erectile, fatty, fibrous, gelatinous, glandular, granulation, homologous, indifferent, interstitial, lymphadenoid, lymphoid, mesenchymal, mucosa-associated lymphoid, mucous, muscular, myeloid, 5 nerve, osseous, reticular, scar, sclerous, skeletal, splenic, subcutaneous) and tissue masses (e.g. tumors).

While preferred embodiments of the present invention have been described, it should be understood that various changes, adaptations and modifications can be made therein without departing from the spirit of the invention and the scope of the 10 appended claims. The scope of the invention should, therefore, be determined not with reference to the above description, but instead should be determined with reference to the appended claims along with their full scope of equivalents. Furthermore, it should be understood that the appended claims do not necessarily comprise the broadest scope of the invention which the Applicant is entitled to 15 claim, or the only manner(s) in which the invention may be claimed, or that all recited features are necessary.

All publications and patent documents cited in this application are incorporated by reference in their entirety for all purposes.

We claim:

1. A surgical device for treating tissue comprising:
 - a handle having a proximal end and a distal end;
 - 5 a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end;
 - an electrode tip, at least a portion of the electrode tip extending distally beyond the distal end of the shaft, the electrode tip extending distally beyond the distal end of the shaft comprising a spherical end surface portion and a cylindrical side surface portion, the spherical end surface portion located distal to the cylindrical side surface portion and comprising at least a portion of the distal end surface of the surgical device; and
 - 10 a fluid passage directed to provide a fluid towards the cylindrical side portion of the electrode tip.
- 15 2. The device according to claim 1 wherein:
 - the fluid passage directed to expel a fluid towards the cylindrical side portion of the electrode tip expels the fluid from an opening at the distal end of the shaft.
- 20 3. The device according to claim 2 wherein:
 - the opening at the distal end of the shaft is located between the electrode tip and the distal end of the shaft.
4. The device according to claim 2 wherein:
 - 25 the opening at the distal end of the shaft is orientated away from direct contact with tissue.
5. The device according to claim 2 wherein:
 - 30 the opening at the distal end of the shaft is sheltered from direct contact with tissue.
6. The device according to claim 5 wherein:
 - 35 the opening at the distal end of the shaft is sheltered from direct contact with tissue by the shaft.
7. The device according to claim 1 wherein:

the fluid passage directed to expel a fluid towards the cylindrical side portion of the electrode tip is also directed to expel the fluid towards the spherical end surface portion of the electrode tip.

- 5 8. The device according to claim 1 wherein:
the fluid passage directed to expel a fluid towards the cylindrical side portion of the electrode tip is also directed to expel the fluid distally along the cylindrical side portion of the electrode tip.
- 10 9. The device according to claim 1 wherein:
the fluid passage directed to expel a fluid towards the cylindrical side portion of the electrode tip is also directed to expel the fluid away from direct contact with tissue.
- 15 10. The device according to claim 1 wherein:
the fluid passage is partially provided by a longitudinally directed elongated recess formed in the electrode tip.
11. The device according to claim 1 wherein:
20 the electrode tip has a length and is straight along its length.
12. The device according to claim 1 wherein:
at least a portion of the cylindrical side surface portion of the electrode tip comprises a curved cylindrical side surface portion.
- 25 13. The device according to claim 11 wherein:
the curved cylindrical side surface portion comprises at least a portion of a hook.
- 30 14. The device according to claim 1 wherein:
at least a portion of the cylindrical side surface portion of the electrode tip comprises a straight cylindrical side surface portion.
15. The device according to claim 14 wherein:
35 the straight cylindrical side surface portion comprises at least a portion of a hook.

16. The device according to claim 1 wherein:
the electrode tip comprises a hook.
17. The device according to claim 16 wherein:
5 the hook comprises an L-shaped hook.
18. The device according to claim 16 wherein:
the hook comprises an J-shaped hook.
- 10 19. The device according to claim 1 wherein:
the electrode tip further comprises a knuckle portion comprising a rounded
protuberance.
- 15 20. The device according to claim 19 wherein:
the electrode tip knuckle portion has a knuckle portion width;
the electrode tip cylindrical portion has a cylindrical portion width; and
the knuckle portion width is greater than the cylindrical portion width.
21. The device according to claim 1 wherein:
20 a contact angle (θ) of the fluid on a surface of the electrode tip is less than 90
degrees.
22. The device according to claim 1 wherein:
the fluid on a surface of the electrode tip has a contact angle (θ) of less than
25 90 degrees.
23. The device according to claim 1 wherein:
the fluid provides a film on a surface of the electrode tip.
- 30 24. A surgical device for treating tissue comprising:
a handle having a proximal end and a distal end;
a shaft extending distally beyond the distal end of the handle, the shaft
having a proximal end and a distal end;
an electrode tip, at least a portion of the electrode tip extending distally
- 35 beyond the distal end of the shaft, the electrode tip extending distally beyond the
distal end of the shaft comprising a neck portion and an enlarged head portion, the
enlarged head portion located distal to the neck portion and comprising at least a
portion of a distal end surface of the surgical device; and

a fluid passage directed to provide a fluid towards the enlarged head portion of the electrode tip.

25. A device for treating tissue comprising:
 - 5 a handle having a proximal end and a distal end;
 - a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end;
 - 10 an electrode tip, the electrode tip comprising a spherical end surface portion and a cylindrical side surface portion, the spherical end surface portion located distal to the cylindrical side surface portion and comprising at least a portion of the distal end surface of the device;
 - 15 a fluid passage connectable to a fluid source; and
 - a plurality of fluid outlet openings in fluid communication with the fluid passage, the fluid outlet openings positioned to provide a fluid from the fluid source around the cylindrical side surface portion of the electrode tip.
26. The device according to claim 25 wherein:
 - the plurality of fluid outlet openings are positioned proximal to the cylindrical side surface portion of the electrode tip.
- 20 27. The device according to claim 26 wherein:
 - the plurality of fluid outlet openings comprise openings at the distal end of the shaft.
- 25 28. The device according to claim 26 wherein:
 - the plurality of fluid outlet openings comprise four equally spaced openings at the distal end of the shaft.
29. The device according to claim 25 wherein:
 - 30 the plurality of fluid outlet openings are positioned around the cylindrical side surface portion of the electrode tip.
30. The device according to claim 29 wherein:
 - the plurality of fluid outlet openings are provided by four equally spaced openings positioned around the cylindrical side surface portion of the electrode tip.
- 35 31. A surgical device for treating tissue comprising:
 - a handle having a proximal end and a distal end;

a shaft extending distally beyond the distal end of the handle, the shaft having a proximal end and a distal end;

an electrode tip comprising a rounded distal end surface portion configured to blunt dissect tissue and a side surface portion configured to seal tissue from at least one of the flow of bodily fluids and air, the side surface portion having a surface area greater than the surface area of the distal end surface portion;

5 a fluid passage connectable to a fluid source; and

at least one fluid outlet opening in fluid communication with the fluid passage, the fluid outlet opening positioned to provide a fluid from the fluid source to the side surface portion of the electrode tip and proximal the distal end surface portion.

10

32. A tissue sealing device comprising:

a first electrode tip spaced from a second electrode tip, the first and second electrode tips being connectable to different terminals of a radio frequency generator to generate electrical current flow therebetween;

15 at least one fluid passage connectable to a fluid source;

at least one fluid outlet opening in fluid communication with the fluid passage, the fluid outlet opening configured to provide a fluid from the fluid source to at least one of a tissue surface and at least one of the first and second electrode tips; and

20 the first and second electrode tips configured to slide over and seal tissue in the presence of a fluid provided from the fluid outlet opening and an electrical current

25 provided from the electrode tips.

33. The device according to claim 32 wherein:

the at least one fluid outlet opening is located between the first electrode tip and the second electrode tip.

30

34. The device according to claim 32 wherein:

the at least one fluid outlet opening is configured to provide the fluid between the first electrode tip and the second electrode tip.

35. 35. The device according to claim 32 wherein:

the at least one fluid outlet opening is configured to provide the fluid to tissue between the first electrode tip and the second electrode tip.

36. The device according to claim 32 wherein:
the first electrode tip provides a first electrode tip distal end surface of the device;
the second electrode tip provides a second electrode tip distal end surface of the device; and
the at least one fluid outlet opening is located proximal to both distal end surfaces.

5

37. The device according to claim 32 wherein:
the first electrode tip provides a first electrode tip distal end surface of the device;
the second electrode tip provides a second electrode tip distal end surface of the device; and
the at least one fluid outlet opening is located adjacent to both distal end surfaces.

10

38. The device according to claim 32 wherein:
the at least one fluid outlet opening further comprises at least a first fluid outlet opening and a second fluid outlet opening;
the first fluid outlet opening is configured to provide the fluid to the first electrode tip; and
the second fluid outlet opening is configured to provide the fluid to the second electrode tip.

15

39. The device according to claim 38 wherein:
the first electrode tip provides a first electrode tip distal end surface of the device;
the second electrode tip provides a second electrode tip distal end surface of the device;
the first fluid outlet opening is located proximal to the first electrode tip distal end surface of the device; and
the second fluid outlet opening is located proximal to the second electrode tip distal end surface of the device.

20

40. The device according to claim 38 wherein:
the first electrode tip provides a first electrode tip distal end surface of the device;

25

the second electrode tip provides a second electrode tip distal end surface of the device;

the first fluid outlet opening is located adjacent to the first electrode tip distal end surface of the device; and

5 the second fluid outlet opening is located adjacent to the second electrode tip distal end surface of the device.

41. The device according to claim 38 wherein:

the first electrode tip provides a first electrode tip distal end surface of the 10 device;

the second electrode tip provides a second electrode tip distal end surface of the device;

the first fluid outlet opening is located on the first electrode tip distal end surface of the device; and

15 the second fluid outlet opening is located on the second electrode tip distal end surface of the device.

42. The device according to claim 38 wherein:

the first fluid outlet opening is positioned at a location substantially 20 inaccessible to direct contact with the tissue; and

the second fluid outlet opening is positioned located at a location substantially inaccessible to direct contact with the tissue.

43. The device according to claim 32 wherein:

25 the first electrode tip is separated from the second electrode tip by a separation distance; and

the separation distance between the first electrode tip and second electrode tip is adjustable.

30 44. The device according to claim 32 wherein:

the first electrode tip is separated from the second electrode tip by a separation distance; and

the separation distance between the first electrode tip and second electrode tip is at least one of incrementally increasable and decreasable by a latching 35 mechanism.

45. The device according to claim 32 wherein:
the first electrode tip is separated from the second electrode tip by a
separation distance; and
the separation distance between the first electrode tip and second electrode
5 tip is unadjustable.

46. The device according to claim 32 wherein:
an electrical insulator is located between the first electrode tip and the second
electrode tip.

10 47. The device according to claim 46 wherein:
a portion of the electrical insulator provides a portion of the fluid passage.

48. The device according to claim 46 wherein:
15 a portion of the electrical insulator provides a dam between the first electrode
tip and the second electrode tip.

49. The device according to claim 46 wherein:
the electrical insulator provides an electrical insulator distal end surface of
20 the device;
the first electrode tip provides a first electrode tip distal end surface of the
device adjacent a first portion of the electrical insulator distal end surface of the
device;
the second electrode tip provides a second electrode tip distal end surface of
25 the device adjacent a second portion of the electrical insulator distal end surface of
the device;
the first electrode tip distal end surface of the device adjacent the first portion
of the electrical insulator distal end surface of the device is substantially flush with
the first portion of the electrical insulator distal end surface of the device;
30 the second electrode tip distal end surface of the device adjacent the second
portion of the electrical insulator distal end surface of the device is substantially
flush with the second portion of the electrical insulator distal end surface of the
device; and
whereby the transition between the electrical insulator distal end surface of
35 the device and the first and second electrode tip distal end surfaces is substantially
smooth and to provide for sliding of the first and second electrode tips along a tissue
surface.

50. The device according to claim 32 wherein:
the first electrode tip is separated from the second electrode tip by an electrical insulator.
- 5 51. The device according to claim 32 wherein:
the first electrode tip and the second electrode tip are held in position relative to each other by a collar.
- 10 52. The device according to claim 32 wherein:
the first electrode tip and the second electrode tip are connected by a linkage.
53. The device according to claim 32 wherein:
the first electrode tip and the second electrode tip are substantially parallel.
- 15 54. The device according to claim 32 wherein:
the first electrode tip and the second electrode tip are substantially the same shape.
55. The device according to claim 32 wherein:
20 the first electrode tip and the second electrode tip are substantially mirror images of each other.
56. The device according to claim 32 wherein:
the first electrode tip comprises a first electrode tip spherical surface; and
25 the second electrode tip comprises a second electrode tip spherical surface.
57. The device according to claim 56 wherein:
the first electrode tip spherical surface comprises at least a portion of a first electrode tip distal end surface of the device; and
30 the second electrode tip spherical surface comprises at least a portion of a second electrode tip distal end surface of the device.
58. The device according to claim 56 wherein:
the first electrode tip spherical surface comprises at least a portion of a side
35 surface of the first electrode tip; and
the second electrode tip spherical surface comprises at least a portion of a side surface of the second electrode tip.

59. The device according to claim 58 wherein:
the first electrode tip spherical surface and the second electrode tip spherical surface are on opposite sides of the device.
- 5 60. The device according to claim 56 wherein:
the first electrode tip spherical surface comprises a hemi-spherical surface less than 180 degrees; and
the second electrode tip spherical surface comprises a hemi-spherical surface less than 180 degrees; and
- 10 61. The device according to claim 56 wherein:
the first electrode tip spherical surface comprises a hemi-spherical surface of about 180 degrees; and
the second electrode tip spherical surface comprises a hemi-spherical surface of about 180 degrees.
- 15 62. The device according to claim 56 wherein:
the first electrode tip spherical surface comprises a hemi-spherical surface greater than 180 degrees; and
the second electrode tip spherical surface comprises a hemi-spherical surface greater than 180 degrees; and
- 20 63. The device according to claim 56 wherein:
the first electrode tip spherical surface is provided by a first electrically conductive ball; and
the second electrode tip spherical surface is provided by a second electrically conductive ball.
- 25 64. The device according to claim 32 wherein:
the first electrode tip comprises a first electrode tip cylindrical surface; and
the second electrode tip comprises a second electrode tip cylindrical surface.
- 30 65. The device according to claim 32 wherein:
the first electrode tip comprises a first electrode tip cylindrical surface located proximal to a first electrode tip spherical surface; and
the second electrode tip comprises a second electrode tip cylindrical surface located proximal to a second electrode tip spherical surface.

66. The device according to claim 32 wherein:
 - the first electrode tip comprises a first electrode tip cylindrical surface located medial to a first electrode tip spherical surface; and
 - the second electrode tip comprises a second electrode tip cylindrical surface located medial to a second electrode tip spherical surface.
- 5
67. The device according to claim 32 wherein:
 - the first electrode tip comprises a first electrode tip first cylindrical surface located proximal to a first electrode tip second cylindrical surface; and
 - 10
 - the second electrode tip comprises a second electrode tip first cylindrical surface located proximal to a second electrode tip second cylindrical surface.
68. The device according to claim 32 wherein:
 - the first electrode tip comprises a first electrode tip first cylindrical surface transverse to a first electrode tip second cylindrical surface; and
 - 15
 - the second electrode tip comprises a second electrode tip first cylindrical surface transverse to a second electrode tip second cylindrical surface.
69. The device according to claim 32 wherein:
 - 20
 - the first electrode tip comprises a neck portion and an enlarged head portion relative to the neck portion, the enlarged head portion located distal to the neck portion and comprising at least a portion of a first electrode tip distal end surface of the device; and
 - the second electrode tip comprises a neck portion and an enlarged head portion relative to the neck portion, the enlarged head portion located distal to the neck portion and comprising at least a portion of a second electrode tip distal end surface of the device.
- 25
70. The device according to claim 69 wherein:
 - 30
 - the first electrode tip head portion comprises a sphere of greater than 180 degrees; and
 - the second electrode tip head portion comprises a sphere of greater than 180 degrees.
- 35
71. The device according to claim 32 wherein:
 - the first electrode tip comprises a first electrode tip hollow metal tube;
 - the second electrode tip comprises a second electrode tip hollow metal tube;
 - and

the first and second electrode tip hollow metal tubes having a bend which curves the tips towards each other as they extend distally.

72. The device according to claim 71 wherein:
5 the first electrode tip hollow metal tube bend is about 90 degrees; and
the second electrode tip hollow metal tube bend is about 90 degrees.

73. The device according to claim 71 wherein:
the first electrode tip hollow metal tube provides at least one first electrode
10 tip hollow metal tube fluid outlet opening; and
the second electrode tip hollow metal tube provides at least one second
electrode tip hollow metal tube fluid outlet opening.

74. The device according to claim 73 wherein:
15 the first electrode tip hollow metal tube has a first electrode tip hollow metal
tube distal end;
the second electrode tip hollow metal tube has a second electrode tip hollow
metal tube distal end;
the first electrode tip hollow metal tube fluid outlet opening is located at the
20 distal end of the first electrode tip hollow metal tube; and
the second electrode tip hollow metal tube fluid outlet opening is located at
the distal end of the second electrode tip hollow metal tube.

75. The device according to claim 73 wherein:
25 the first electrode tip hollow metal tube has a first electrode tip hollow metal
tube distal end;
the second electrode tip hollow metal tube has a second electrode tip hollow
metal tube distal end;
the first electrode tip hollow metal tube fluid outlet opening is located
30 adjacent the distal end of the first electrode tip hollow metal tube; and
the second electrode tip hollow metal tube fluid outlet opening is located
adjacent the distal end of the second electrode tip hollow metal tube.

76. The device according to claim 73 wherein:
35 the first electrode tip hollow metal tube has a first electrode tip hollow metal
tube distal end;
the second electrode tip hollow metal tube has a second electrode tip hollow
metal tube distal end;

the first electrode tip hollow metal tube fluid outlet opening is located proximal to the distal end of the first electrode tip hollow metal tube; and

the second electrode tip hollow metal tube fluid outlet opening is located proximal to the distal end of the second electrode tip hollow metal tube.

5

77. The device according to claim 73 wherein:

the first electrode tip hollow metal tube fluid outlet opening is positioned at a location substantially inaccessible to direct contact with the tissue; and

10 the second electrode tip hollow metal tube fluid outlet opening is positioned at a location substantially inaccessible to direct contact with the tissue.

78. The device according to claim 71 wherein:

15 the first electrode tip hollow metal tube provides at least one first electrode tip hollow metal tube fluid outlet opening, the bend has an inner bend radius and an outer bend radius and at least a portion of the first electrode tip hollow metal tube fluid outlet opening is closer to the inner bend radius than the outer bend radius;

20 the second electrode tip hollow metal tube and provides at least one second electrode tip hollow metal tube fluid outlet opening, and bend has an inner bend radius and an outer bend radius and at least a portion of the second electrode tip hollow metal tube fluid outlet opening is closer to the inner bend radius than the outer bend radius.

79. The device according to claim 71 wherein:

25 the first electrode tip hollow metal tube provides at least one first electrode tip hollow metal tube fluid outlet opening, the bend has an inner bend radius and an outer bend radius and at least a portion of the first electrode tip hollow metal tube fluid outlet opening is closer to the outer bend radius than the inner bend radius;

30 the second electrode tip hollow metal tube and provides at least one second electrode tip hollow metal tube fluid outlet opening, and bend has an inner bend radius and an outer bend radius and at least a portion of the second electrode tip hollow metal tube fluid outlet opening is closer to the outer bend radius than the inner bend radius.

80. The device according to claim 71 wherein:

35 the first electrode tip hollow metal tube provides at least one first electrode tip hollow metal tube fluid outlet opening, the bend has an inner bend radius and an outer bend radius and at least a portion of the first electrode tip hollow metal tube

fluid outlet opening is equidistant between the outer bend radius than the inner bend radius;

the second electrode tip hollow metal tube and provides at least one second electrode tip hollow metal tube fluid outlet opening, and bend has an inner bend radius and an outer bend radius and at least a portion of the second electrode tip hollow metal tube fluid outlet opening is equidistant between the outer bend radius than the inner bend radius.

5 81. The device according to claim 32 further comprising:
10 a housing having a housing distal end, the first electrode tip and the second electrode tip extending distally beyond the housing distal end.

82. The device according to claim 81 wherein:
15 the housing having a housing distal end comprises a shaft having a shaft distal end; and
the first electrode tip and the second electrode tip extending distally beyond the shaft distal end.

83. The device according to claim 32 further comprising:
20 a first housing having a first housing distal end, the first electrode tip extending distally beyond the first housing distal end; and
a second housing having a second housing distal end, the second electrode tip extending distally beyond the second housing distal end.

25 84. The device according to claim 83 wherein:
the first housing further comprises a first housing cavity, the first electrode tip retractable into the first housing cavity; and
the second housing further comprises a second housing cavity, the second electrode tip retractable into the second housing cavity.

30 85. The device according to claim 83 wherein:
the first housing further comprises a first housing distal end opening, the first electrode tip extending distally beyond the first housing distal end opening; and
the second housing further comprises a second housing distal end opening,
35 the second electrode tip extending distally beyond the second housing distal end opening.

86. The device according to claim 85 wherein:
the first housing distal end opening further comprises a first housing distal end fluid outlet opening; and
the second housing distal end opening further comprises a second housing distal end fluid outlet opening.

87. The device according to claim 86 wherein:
the first housing distal end fluid outlet opening is configured to provide the fluid to the first electrode tip; and
the second housing distal end fluid outlet opening is configured to provide the fluid to the second electrode tip.

88. The device according to claim 32 further comprising:
a first shaft having a first shaft distal end, the first electrode tip extending distally beyond the first shaft distal end; and
a second shaft having a second shaft distal end, the second electrode tip extending distally beyond the second shaft distal end.

89. The device according to claim 88 wherein:
the first shaft further comprises a first shaft distal end opening, the first electrode tip extending distally beyond the first shaft distal end opening; and
the second shaft further comprises a second shaft distal end opening, the second electrode tip extending distally beyond the second shaft distal end opening.

90. The device according to claim 89 wherein:
the first shaft distal end opening further comprises a first shaft distal end fluid outlet opening; and
the second shaft distal end opening further comprises a second shaft distal end fluid outlet opening.

91. The device according to claim 90 wherein:
the first shaft distal end fluid outlet opening is configured to provide the fluid to the first electrode tip; and
the second shaft distal end fluid outlet opening is configured to provide the fluid to the second electrode tip.

92. The device according to claim 32 wherein:
the first electrode tip is part of a first arm; and

the second electrode tip is part of a second arm;

93. The device according to claim 92 wherein:
the first arm and the second arm are immobile relative to each another.

5

94. The device according to claim 92 wherein:
the first arm and the second arm are movable relative to each other.

10

95. The device according to claim 92 wherein:
the first arm includes a pivot; and
the second arm includes a pivot.

15

96. The device according to claim 92 further comprising:
a handle having a proximal end and a distal end; and
the first arm and the second arm extend distally beyond the distal end of the handle.

20

97. The device according to claim 92 wherein:
the first arm comprises a first shaft having a first shaft distal end and the first electrode tip is located distal to the first shaft distal end; and
the second arm comprises a second shaft having a second shaft distal end and the second electrode tip is located distal to the second shaft distal end.

25

98. The device according to claim 97 wherein:
the first shaft has a first shaft fluid passage, the first shaft fluid passage configured to provide the fluid to the first electrode tip; and
the second shaft has a second fluid passage, the second shaft fluid passage configured to provide the fluid to the second electrode tip;

30

99. The device according to claim 32 further comprising:
a valve assembly to control a flow of the fluid.

100. The device according to claim 32 further comprising:
a handle; and
35 the valve assembly is located in the handle.

101. The device according to claim 99 wherein:
the valve assembly is configured to turn the flow of the fluid on and off.

102. The device according to claim 99 wherein:
the valve assembly is configured to adjust the flow of the fluid between two non-zero flow rates.
- 5 103. The device according to claim 99 wherein:
the valve assembly is configured to at least one of increase and decrease the flow of the fluid.
- 10 104. The device according to claim 99 wherein:
the fluid passage is partially provided within a plastic tubing; and
the valve assembly comprises a roller clamp assembly, the roller clamp assembly having a wheel configured to roll along the plastic tubing to at least partially open and close the fluid passage.
- 15 105. The device according to claim 104 wherein:
the wheel rolls proximally and distally.
106. The device according to claim 99 wherein:
the fluid passage is partially provided within a plastic tubing; and
20 the valve assembly comprises an arm, the arm configured to move in a first direction and a second direction, the first direction to compress the plastic tubing to at least partially close the fluid passage and a second direction to decompress the plastic tubing to at least partially open the fluid passage.
- 25 107. The device according to claim 106 wherein:
the arm moves proximally and distally.
108. The device according to claim 99 wherein:
the fluid passage is partially provided within a plastic tubing; and
30 the valve assembly comprises mechanism configured to compress the plastic tubing to at least partially close the fluid passage.
109. The device according to claim 99 wherein:
the fluid passage is partially provided within a plastic tubing and
35 the switch assembly comprises mechanism configured to pinch the plastic tubing to at least partially close the fluid passage.

110. The device according to claim 32 further comprising:
 - a switch assembly to control power, the switch assembly having on and off positions.
 - 5 a valve assembly to control a flow of the fluid, the valve having on and off positions;
 - a mechanism which prevents the switch assembly from being in the on position while the valve assembly is in the off position.
111. A method for treating tissue comprising:
 - 10 providing tissue having a tissue surface;
 - providing radio frequency power at a power level;
 - providing an electrically conductive fluid at a fluid flow rate;
 - providing an surgical device configured to simultaneously provide the radio frequency power and the electrically conductive fluid to tissue;
 - 15 providing the electrically conductive fluid to the tissue at the tissue surface;
 - forming a fluid coupling comprising the electrically conductive fluid which couples the tissue and the surgical device;
 - providing the radio frequency power to the tissue at the tissue surface and below the tissue surface into the tissue through the fluid coupling;
 - 20 sealing the tissue against at least one of the flow of bodily fluids and air; and blunt dissecting the tissue.
112. The method of treating tissue according to claim 111 wherein:
 - 25 the tissue comprises soft tissue.
113. The method of treating tissue according to claim 111 wherein:
 - 25 the tissue comprises organ tissue.
114. The method of treating tissue according to claim 113 wherein:
 - 30 the organ tissue comprises liver tissue.
115. The method of treating tissue according to claim 113 wherein:
 - 30 the organ tissue comprises lung tissue.
- 35 116. The method of treating tissue according to claim 113 wherein:
 - 35 the organ tissue comprises spleen tissue.

117. The method of treating tissue according to claim 113 wherein:
the organ tissue comprises gallbladder tissue.
118. The method of treating tissue according to claim 111 wherein:
5 the tissue comprises a vessel.
119. The method of treating tissue according to claim 118 wherein:
the vessel comprises a blood vessel.
- 10 120. A method for treating tissue comprising:
providing tissue having a tissue surface;
providing radio frequency power at a power level;
providing an electrically conductive fluid at a fluid flow rate;
providing an surgical device configured to simultaneously provide the radio
15 frequency power and the electrically conductive fluid to tissue, the surgical device
comprising a first electrode tip and a second electrode tip;
providing the electrically conductive fluid to the tissue at the tissue surface;
forming a fluid coupling comprising the electrically conductive fluid which couples
the tissue and the surgical device;
20 providing the radio frequency power to the tissue at the tissue surface and
below the tissue surface into the tissue through the fluid coupling;
sliding the first electrode tip and the second electrode tip over the tissue
surface; and
sealing the tissue against at least one of the flow of bodily fluids and air.
25
121. The method of treating tissue according to claim 120 wherein:
the tissue comprises soft tissue.
122. The method of treating tissue according to claim 120 wherein:
30 the tissue comprises hard tissue.
123. The method of treating tissue according to claim 120 wherein:
the tissue comprises osseous tissue.
- 35 124. The method of treating tissue according to claim 120 wherein:
the tissue comprises bone tissue.

125. The method of treating tissue according to claim 124 wherein:
the bone tissue comprises compact bone tissue.

126. The method of treating tissue according to claim 124 wherein:
5 the bone tissue comprises cancellous bone tissue.

127. The method of treating tissue according to claim 124 wherein:
the bone tissue comprises long bone tissue.

- 10 128. The method of treating tissue according to claim 124 wherein:
the bone tissue comprises femur bone tissue.

129. The method of treating tissue according to claim 124 wherein:
the bone tissue comprises tibia bone tissue.

- 15 130. The method of treating tissue according to claim 124 wherein:
the bone tissue comprises innominate bone tissue.

131. The method of treating tissue according to claim 124 wherein:
20 the bone tissue comprises vertebra bone tissue.

132. The method of treating tissue according to claim 120 wherein:
the tissue comprises connective tissue.

- 25 133. The method of treating tissue according to claim 120 performed as part of an
orthopaedic surgical procedure.

134. The method of treating tissue according to claim 120 performed as part of the
group consisting of knee, hip, shoulder and spinal surgical procedures.

- 30 135. The method of treating tissue according to claim 120 wherein:
the tissue comprises a vessel.

136. The method of treating tissue according to claim 135 wherein:
35 the vessel comprises a blood vessel.

137. The method of treating tissue according to claim 120 wherein:
the bodily fluid comprises blood.

FIG. 1

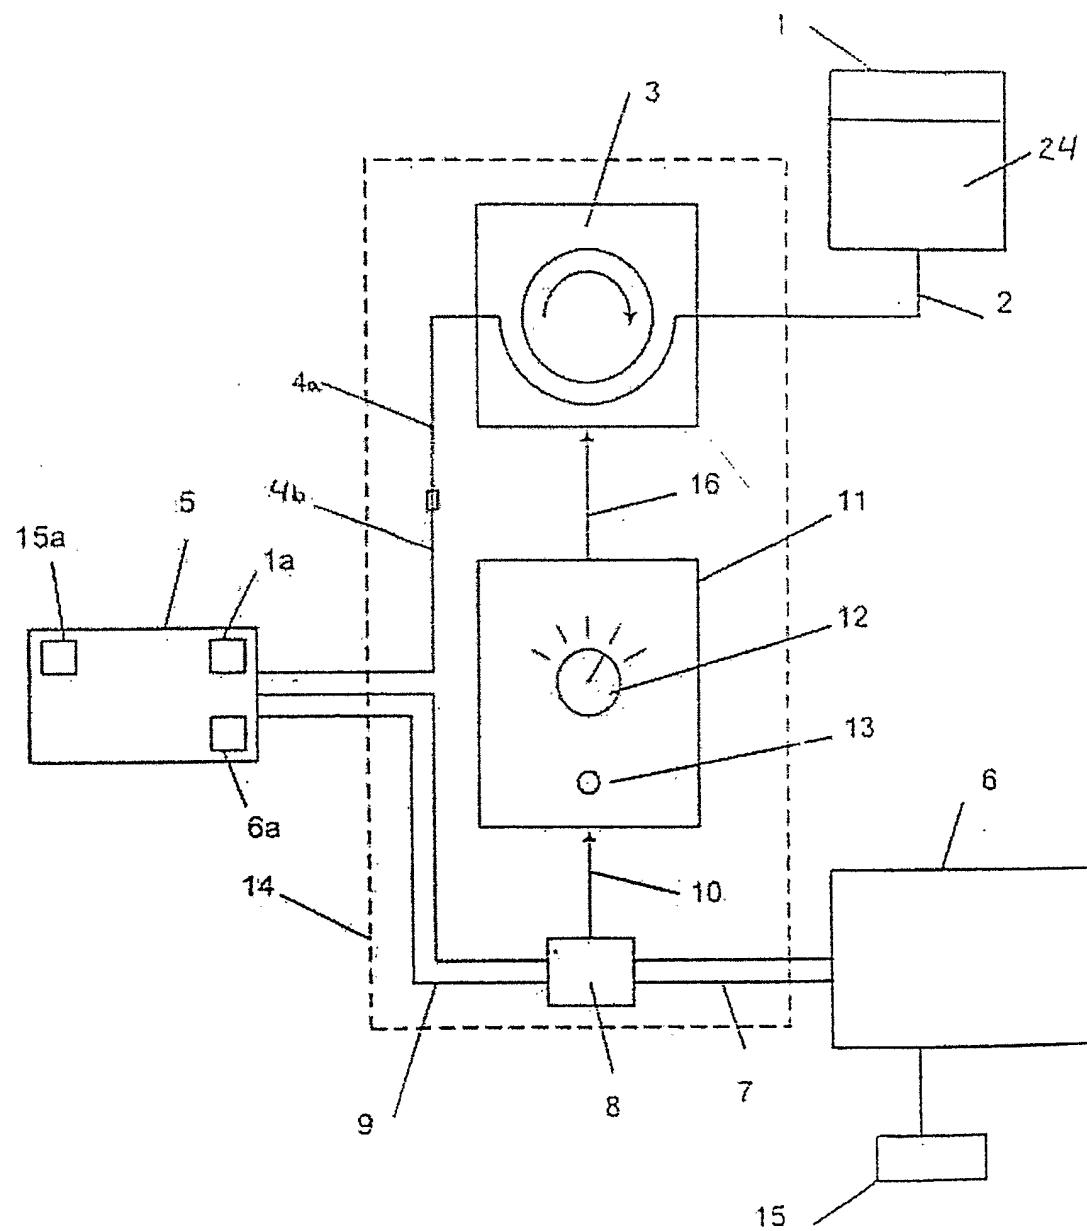


FIG. 2

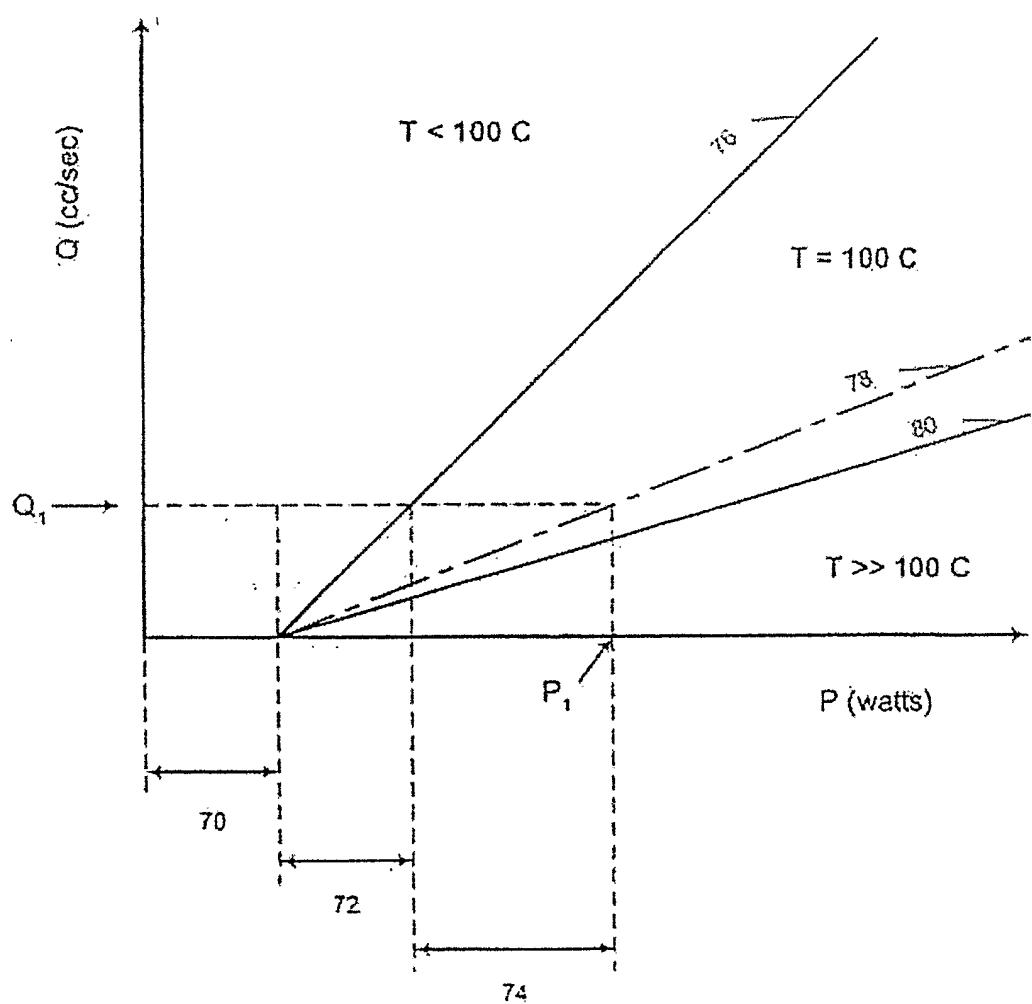


FIG. 3

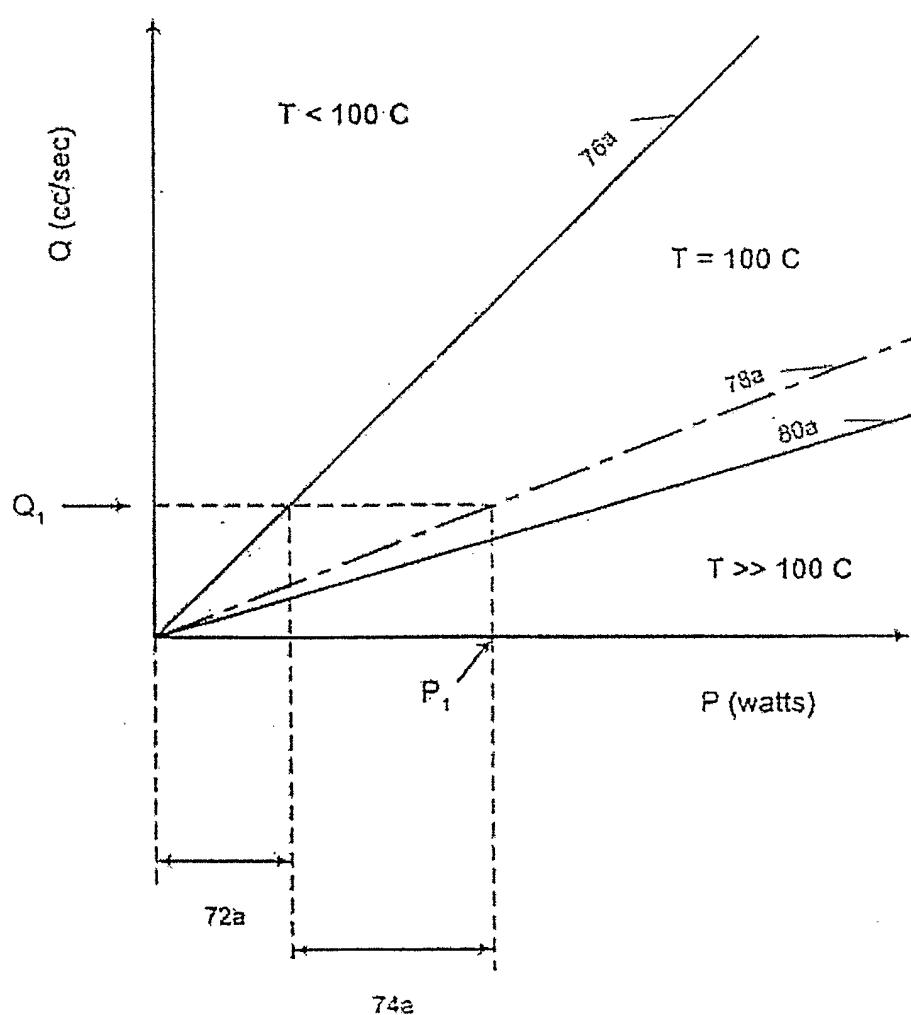


FIG. 4

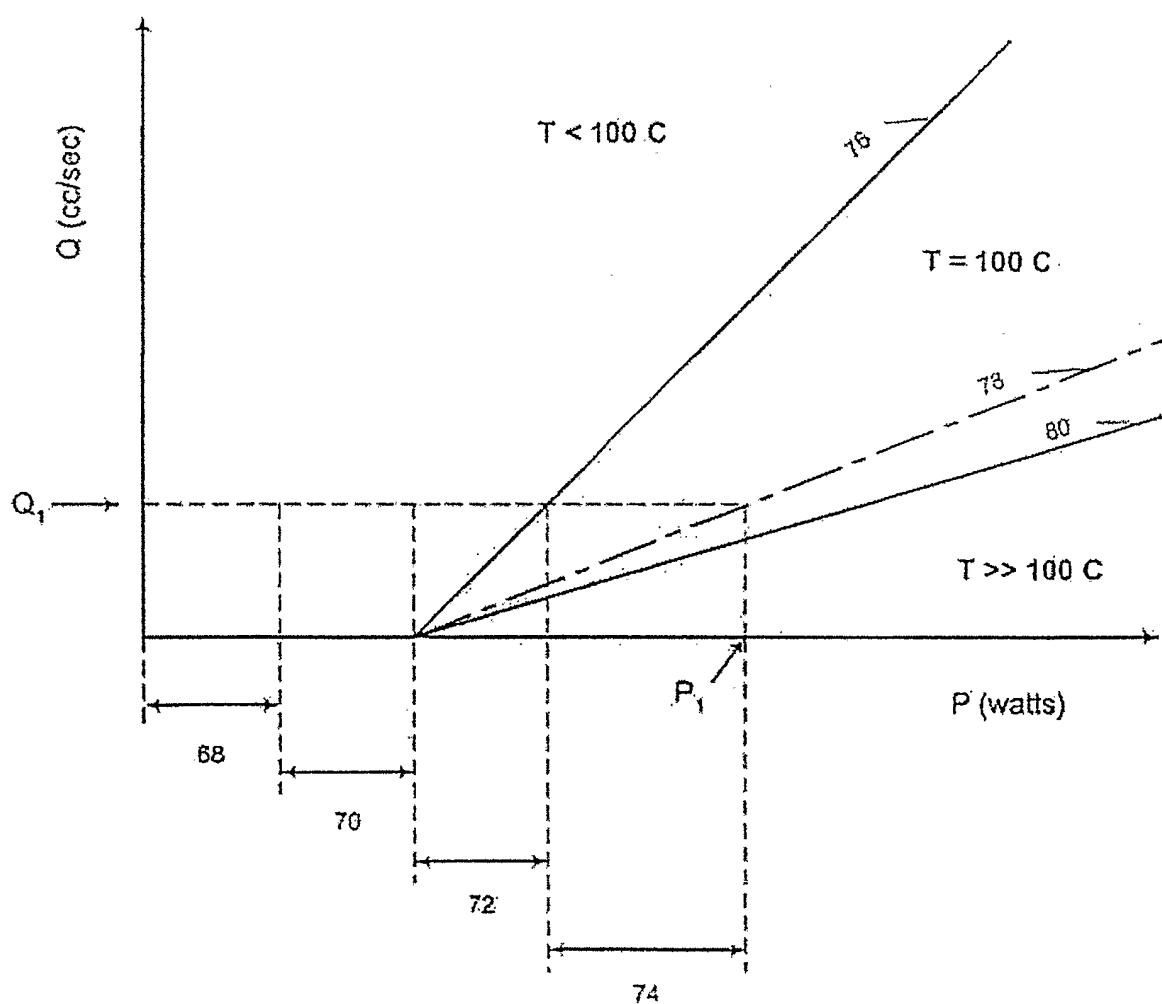


FIG. 5

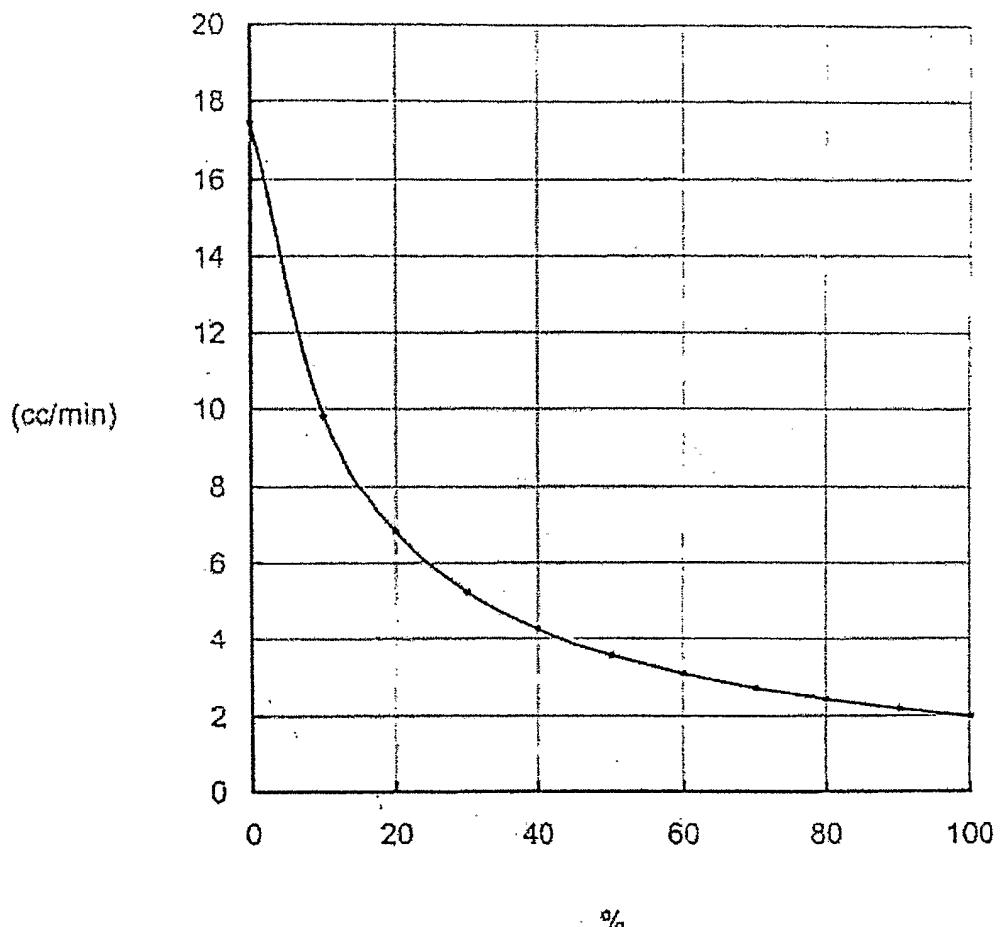


FIG. 6

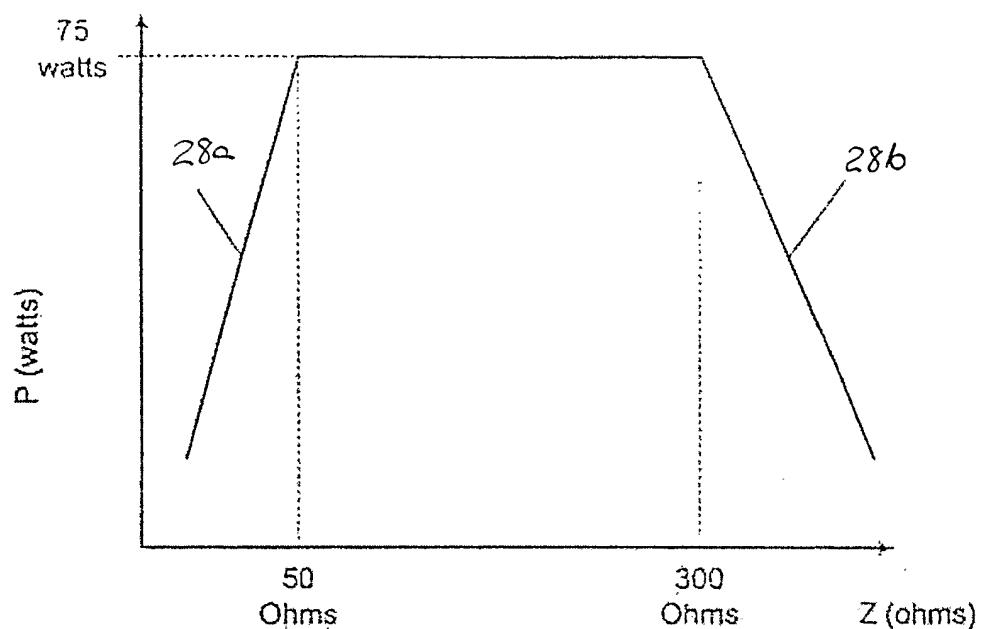
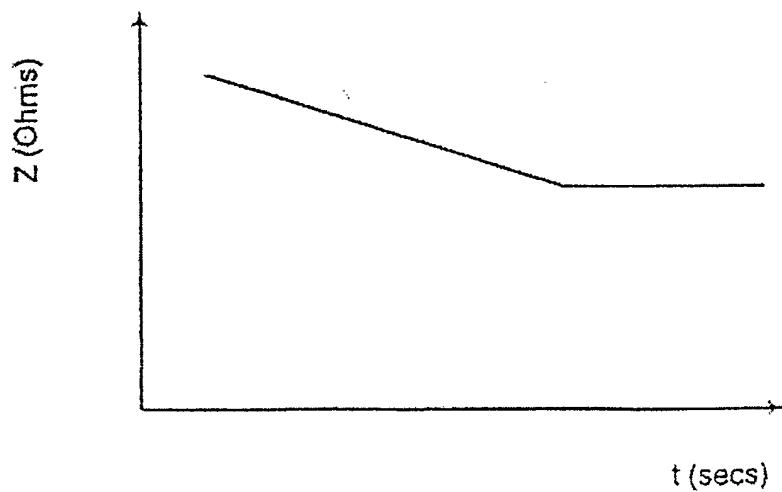


FIG. 7



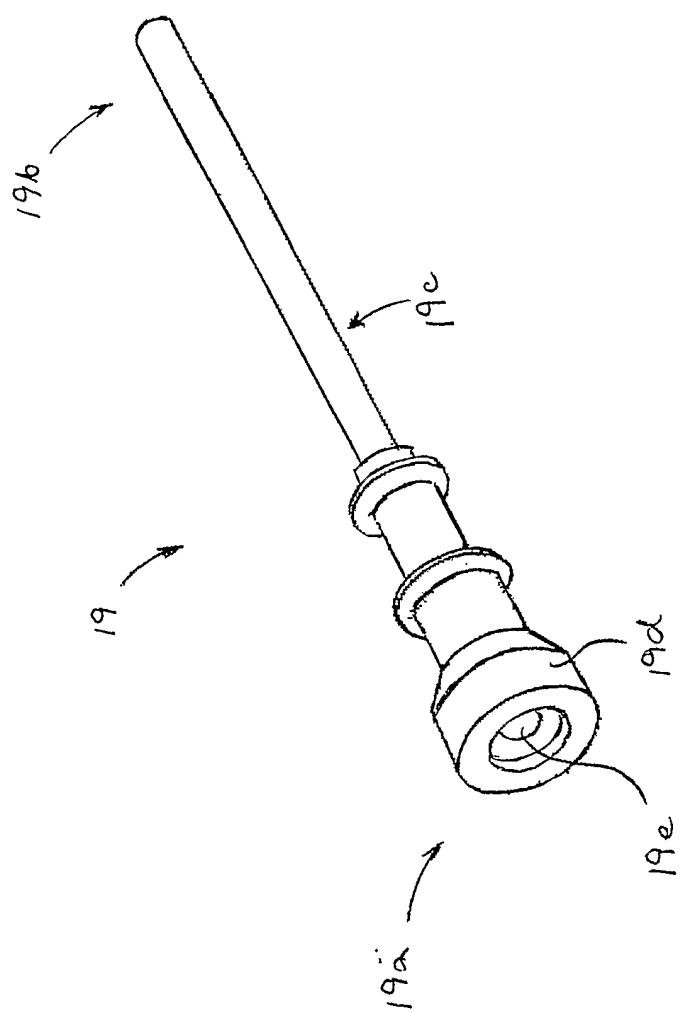
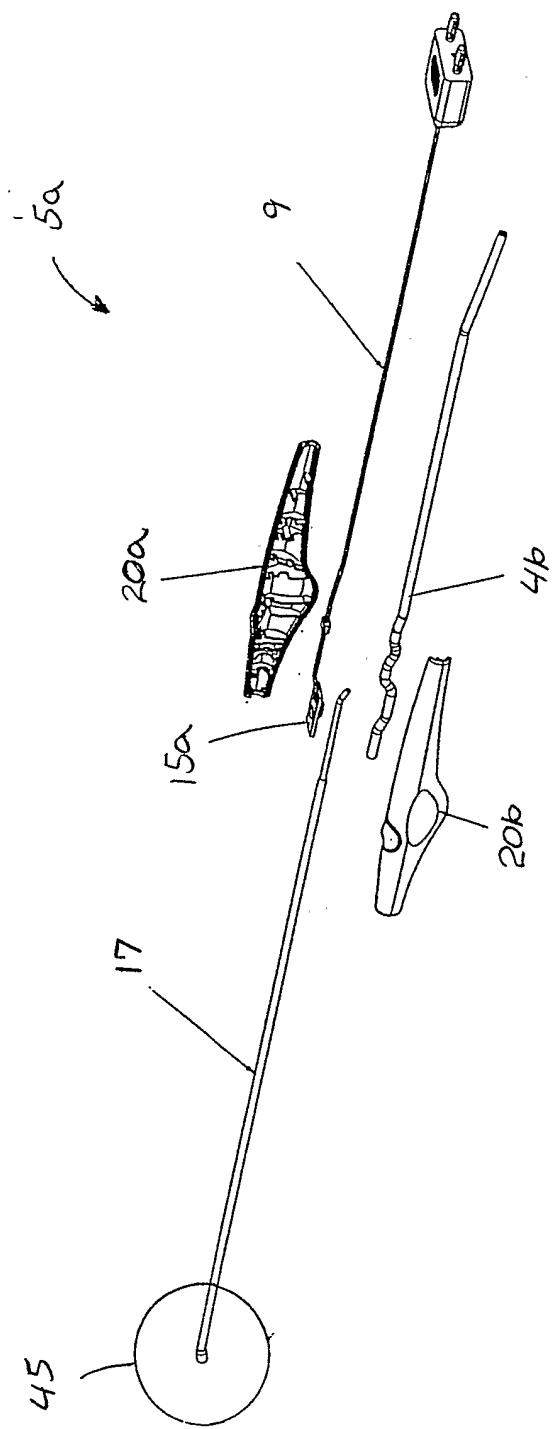
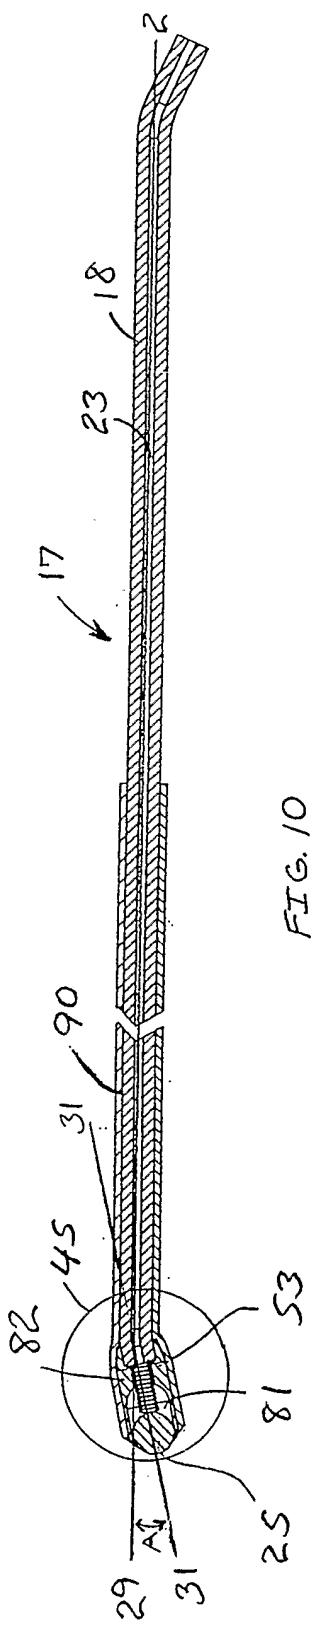
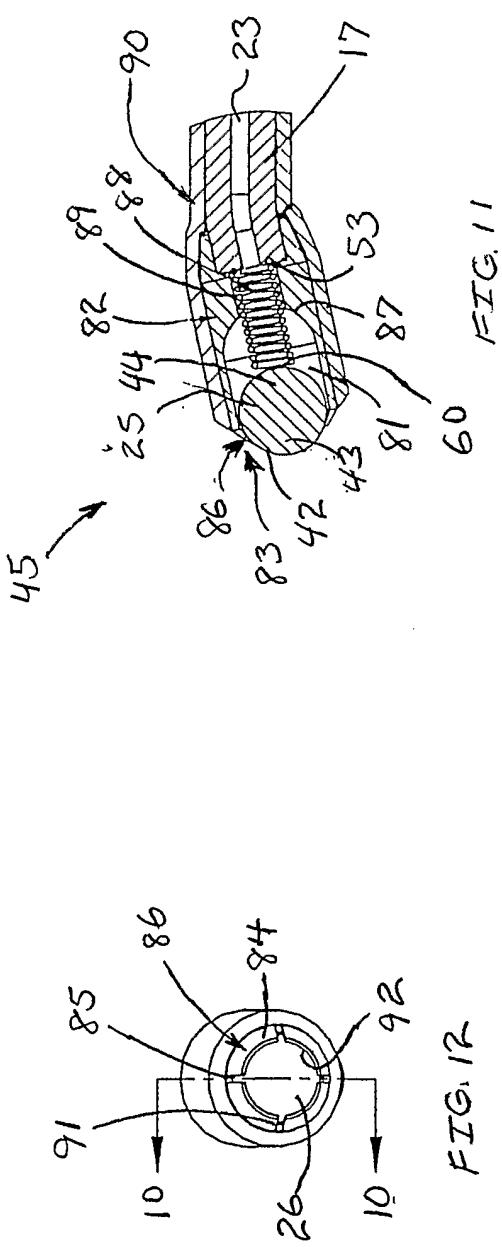


FIG. 8





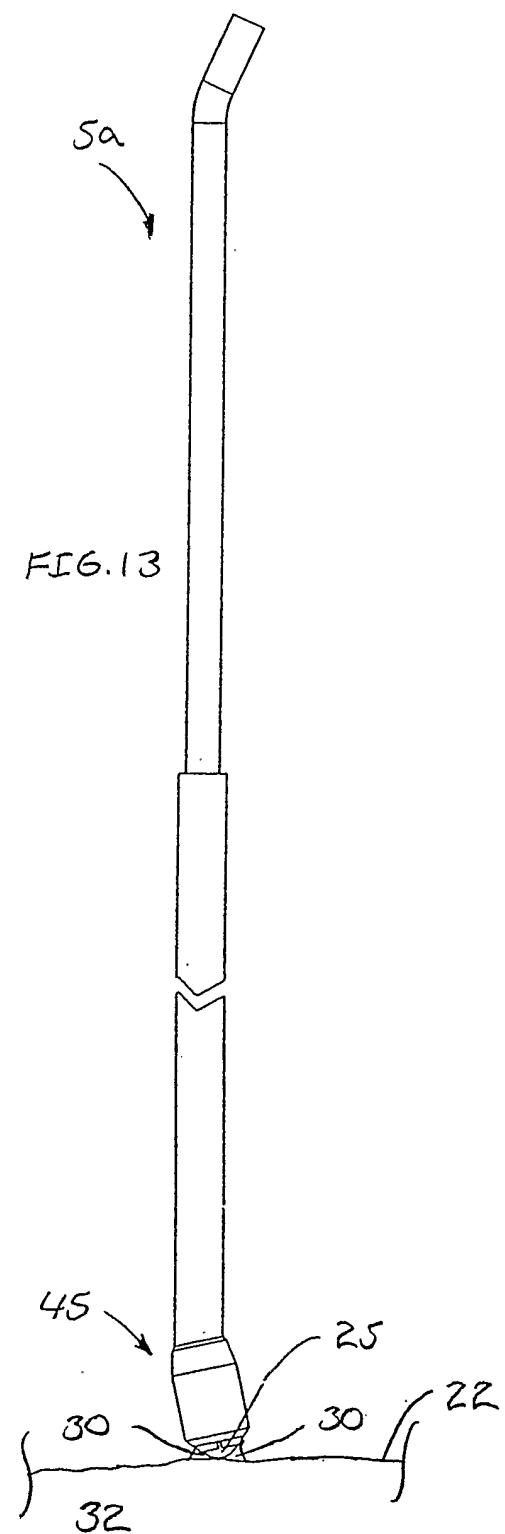


FIG. 15

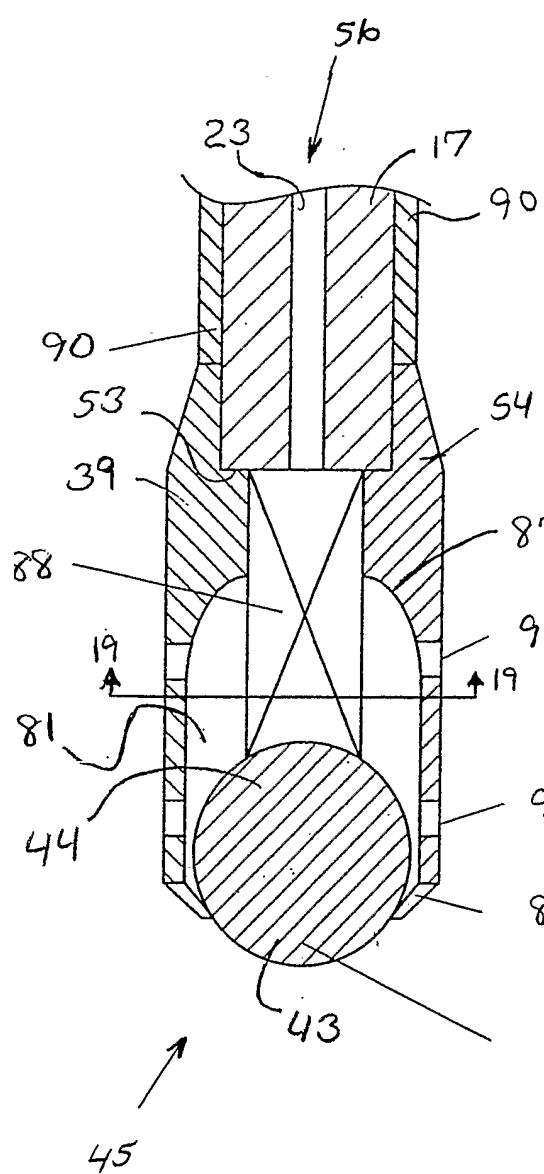


FIG. 14

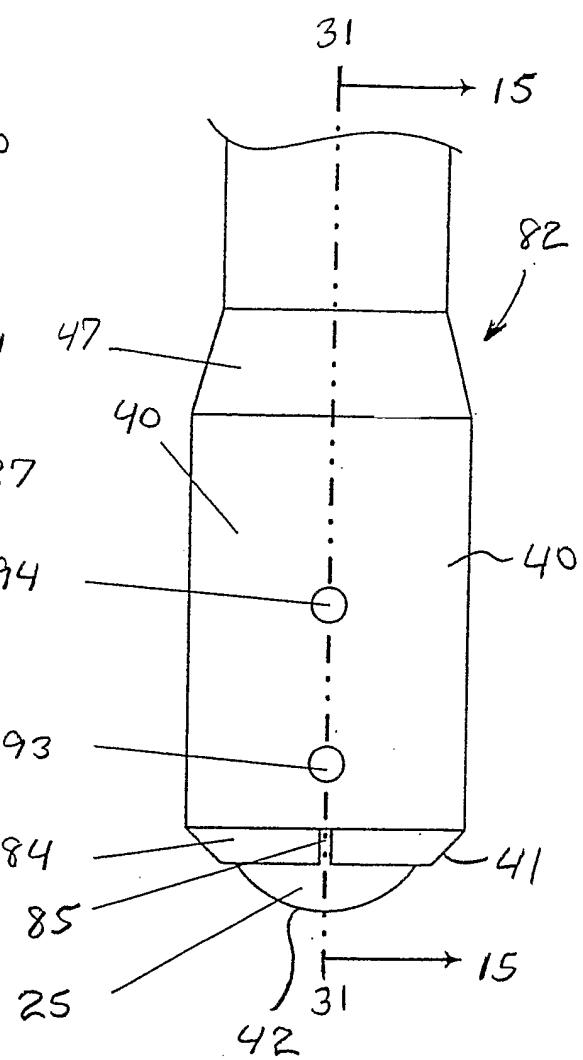


FIG. 16

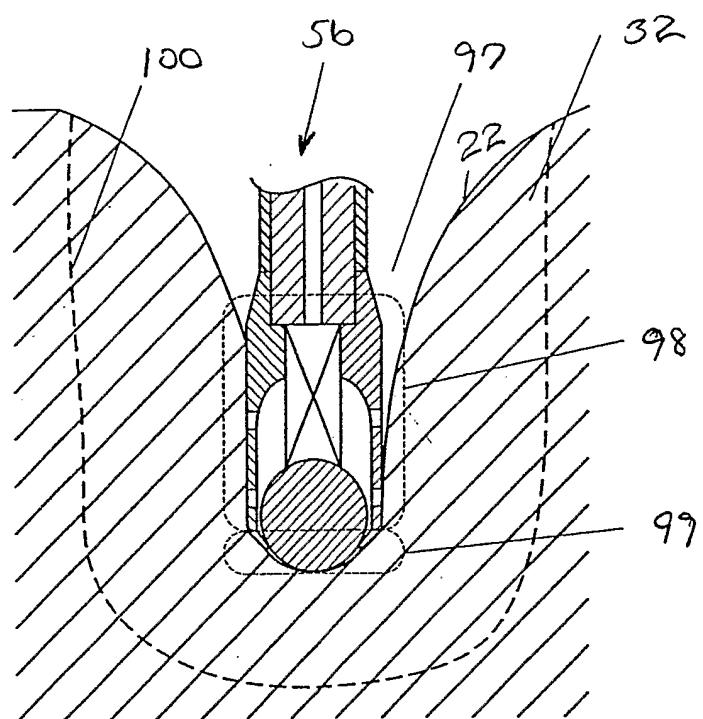


FIG. 17

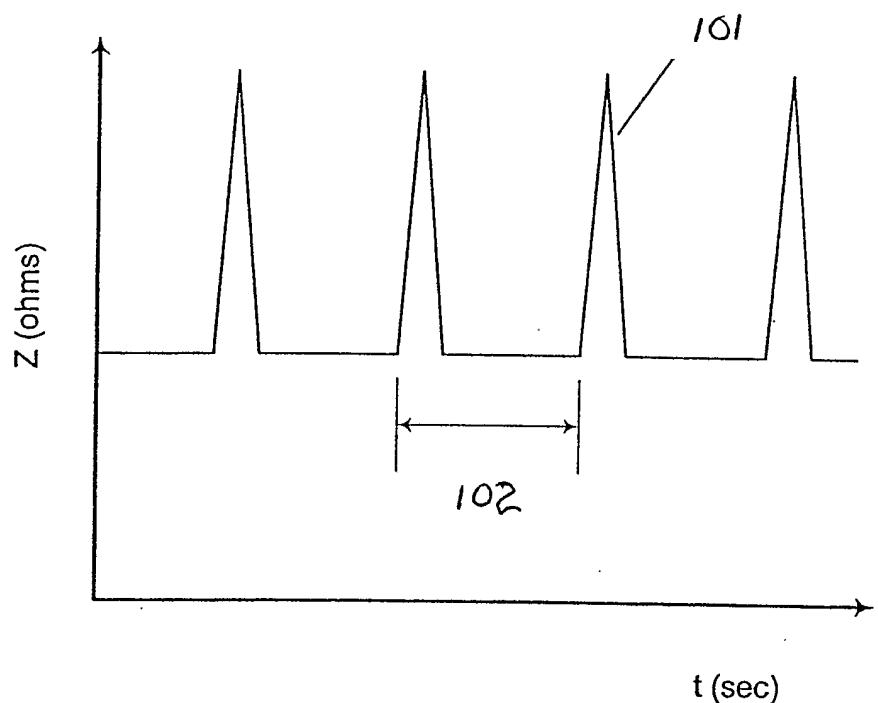
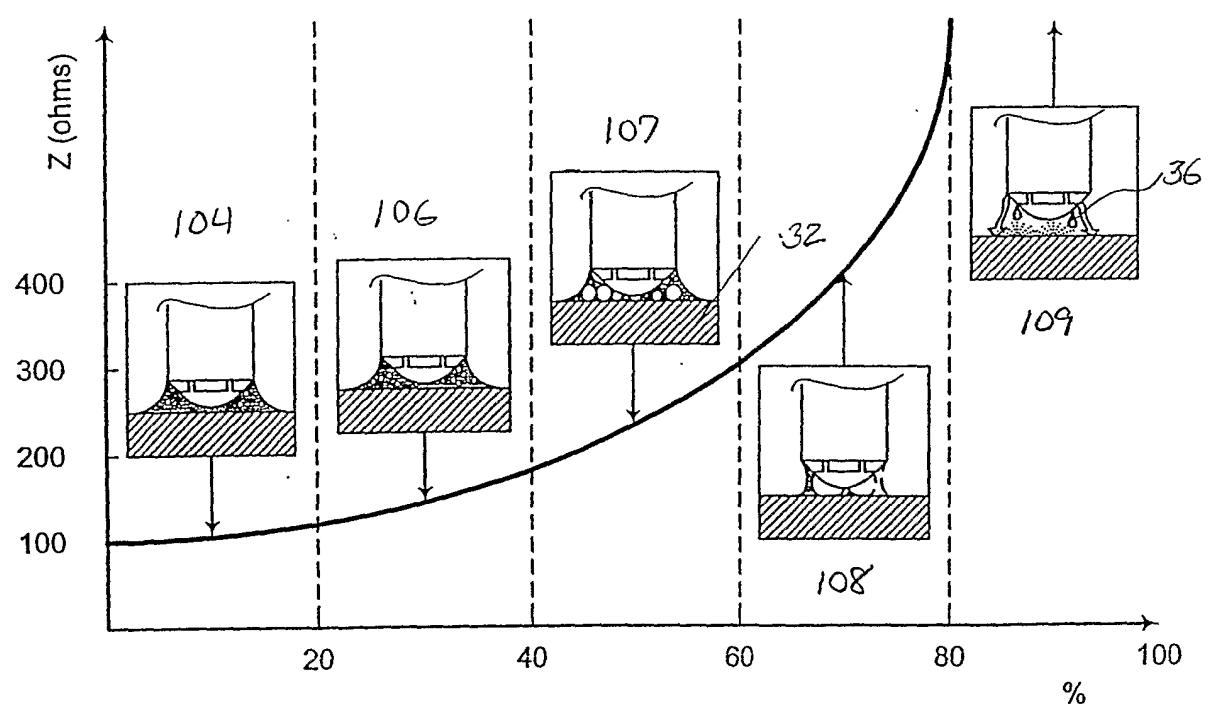


FIG. 18



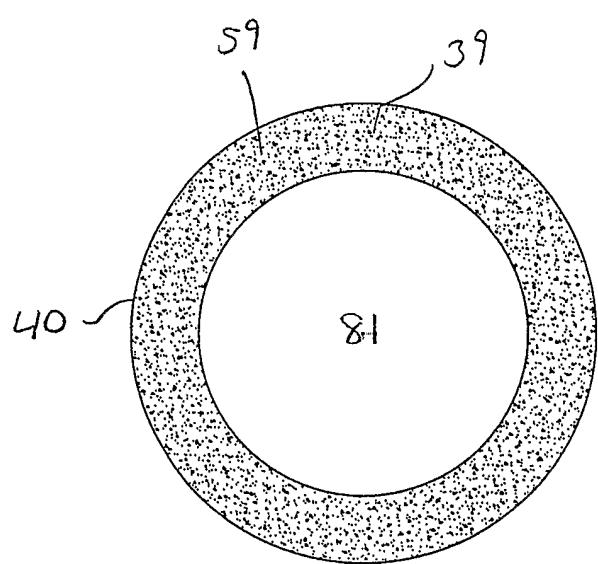
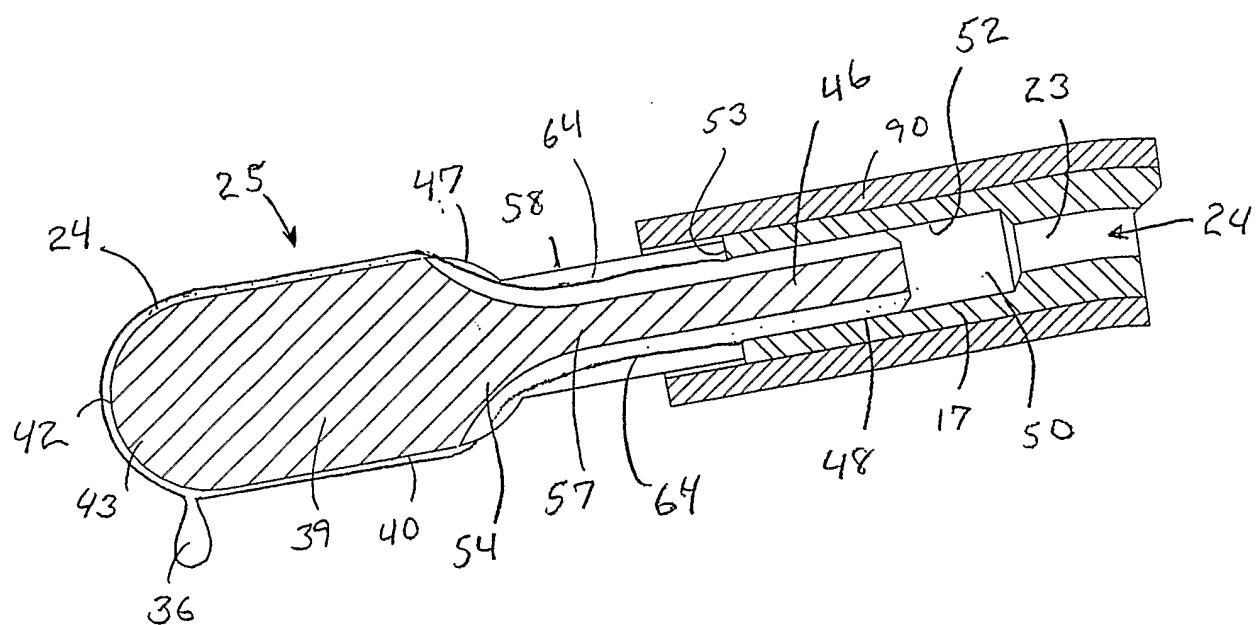
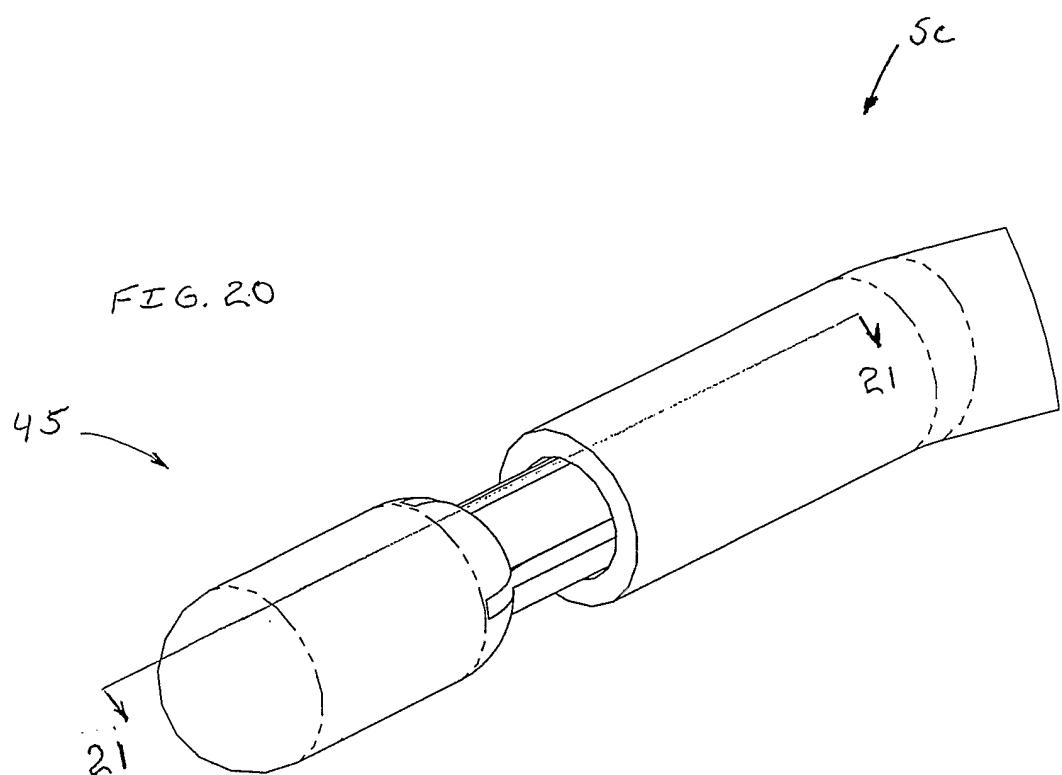


FIG. 19



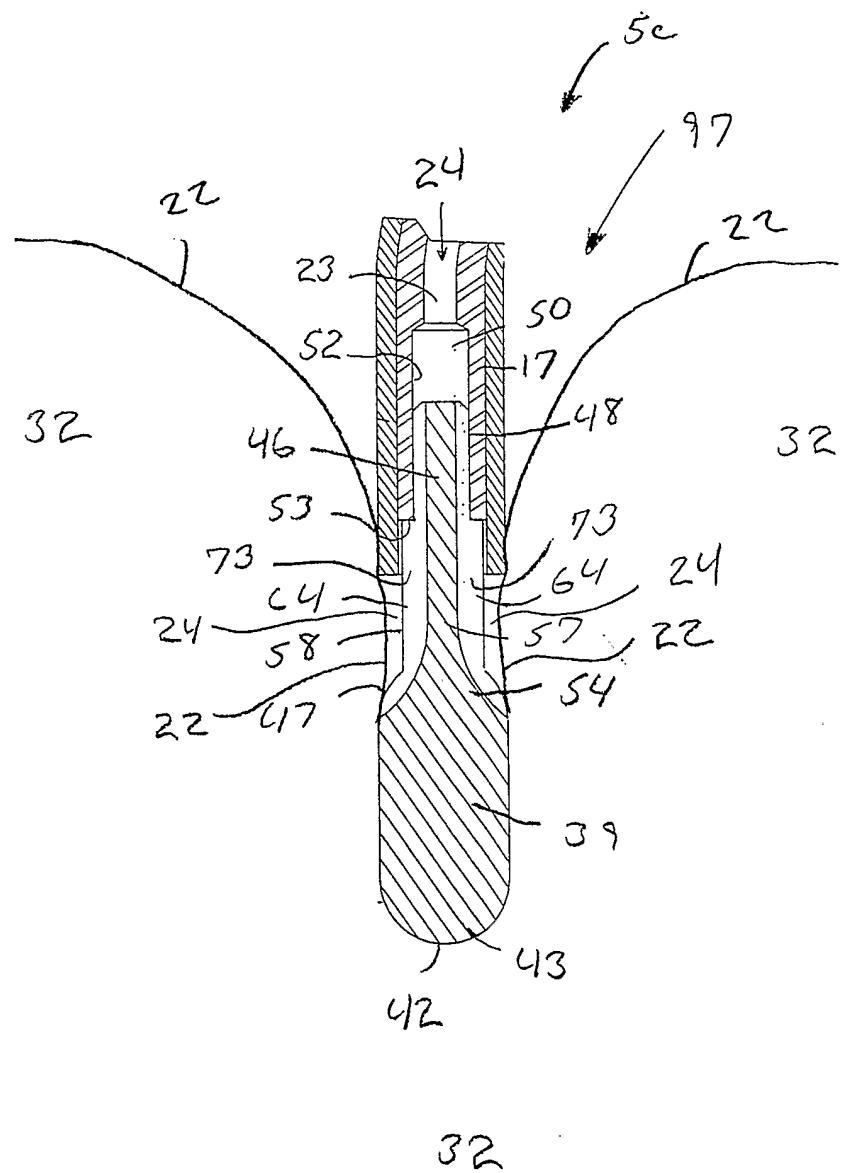


FIG. 22

FIG. 23

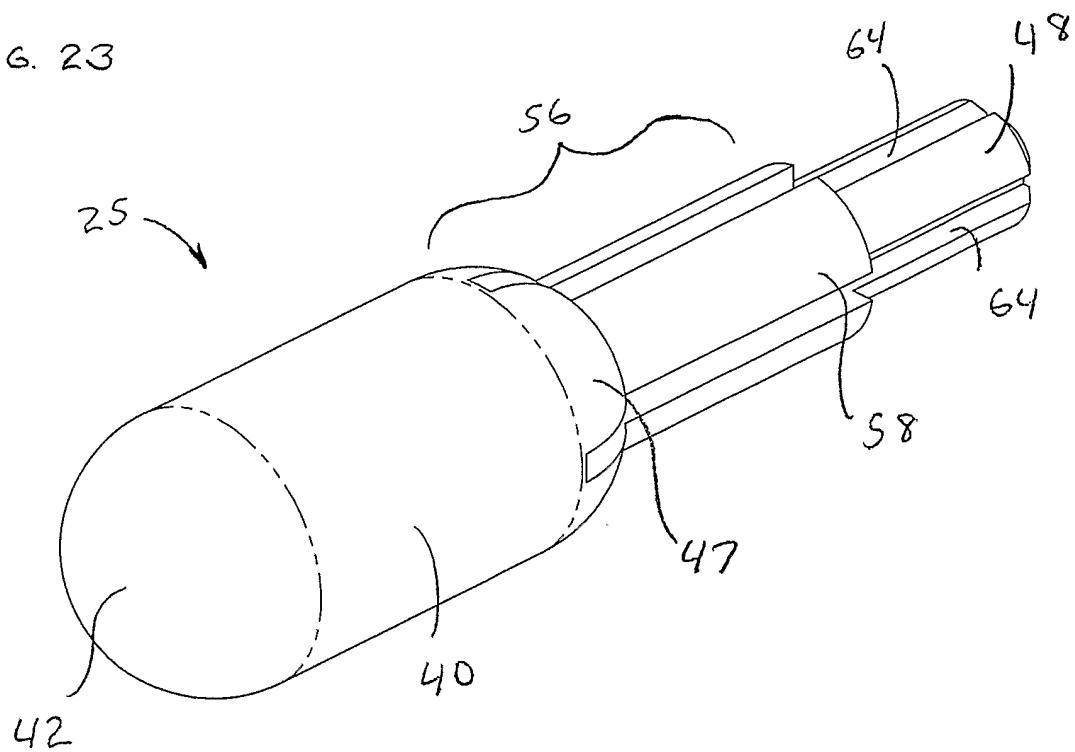
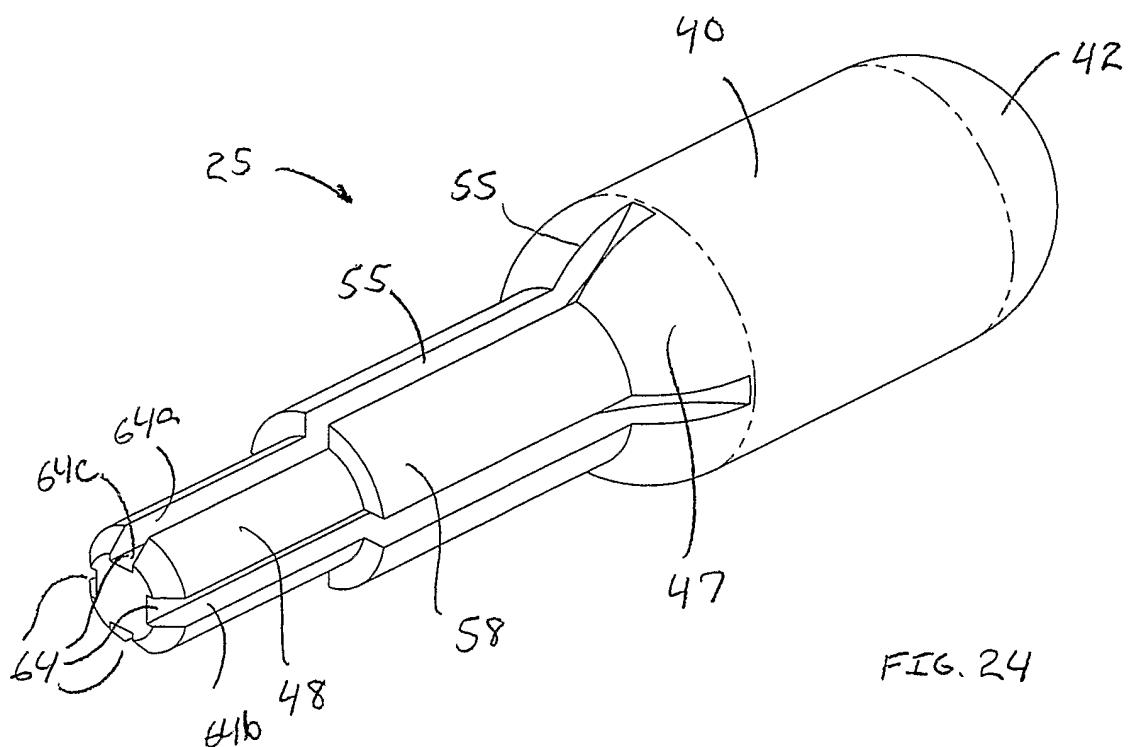


FIG. 24



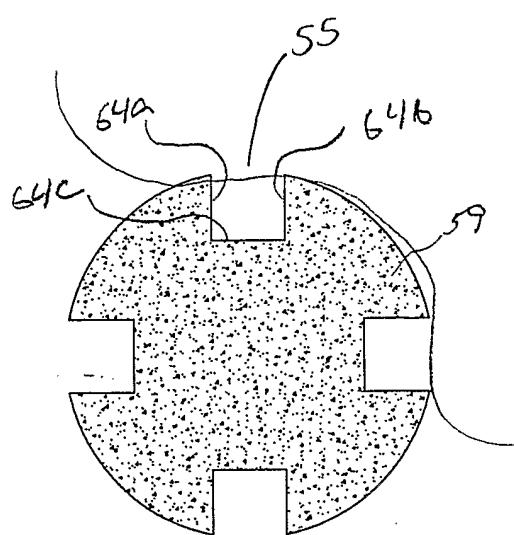


FIG. 25

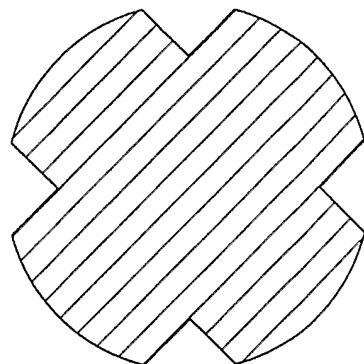


FIG. 27

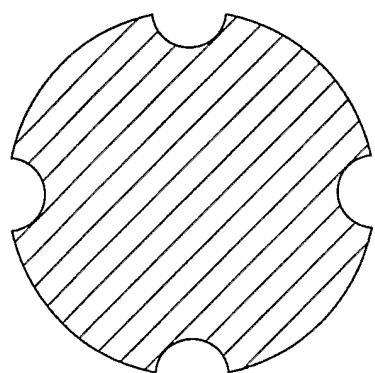


FIG. 26

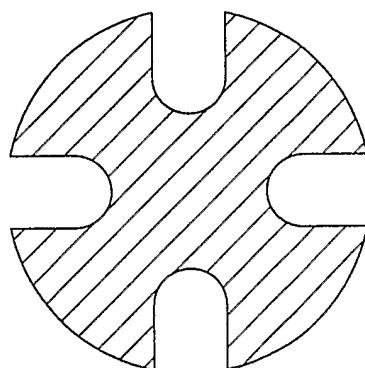


FIG. 28

FIG 29

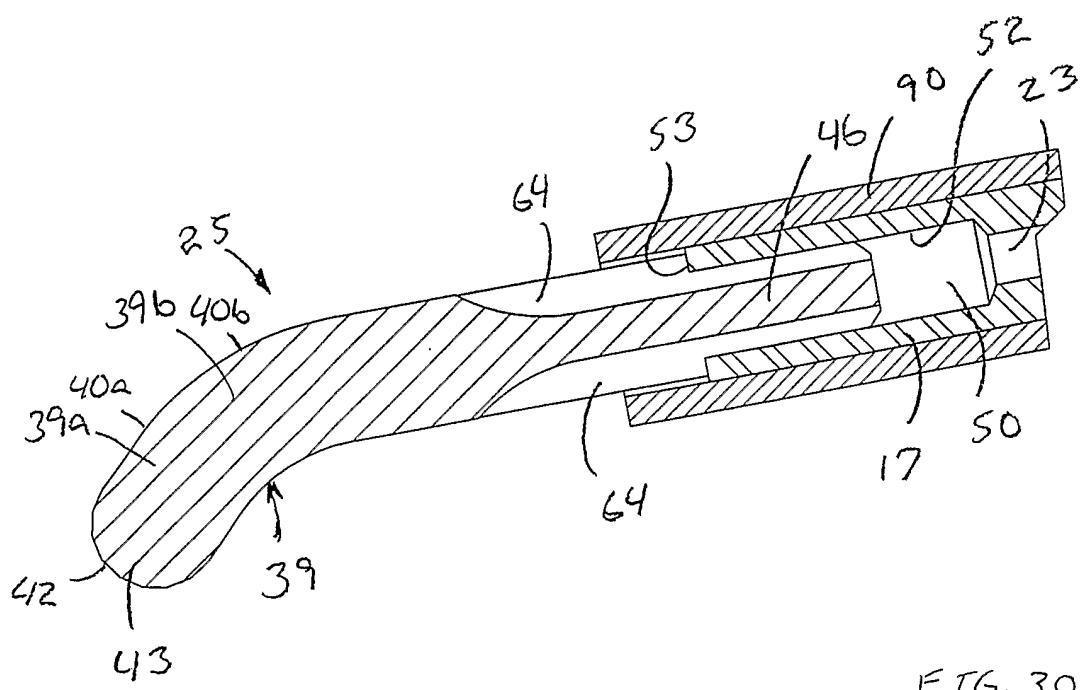
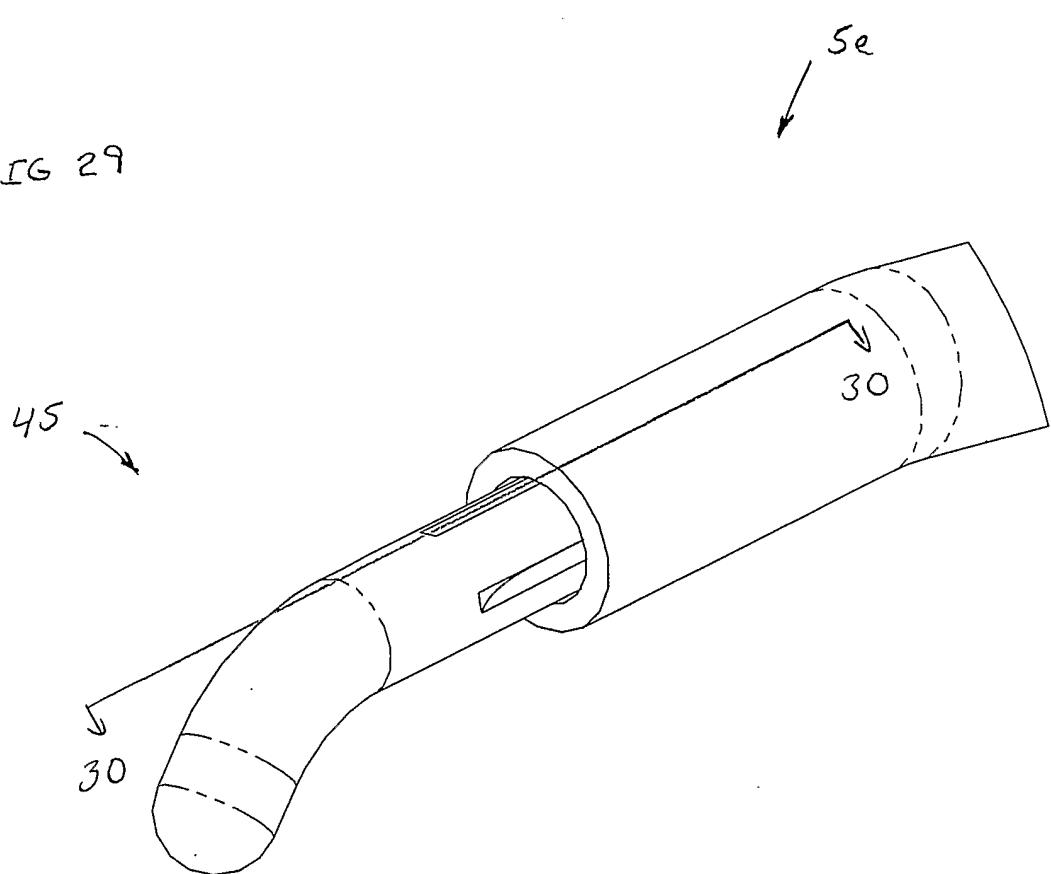


FIG. 30

FIG 6. 31

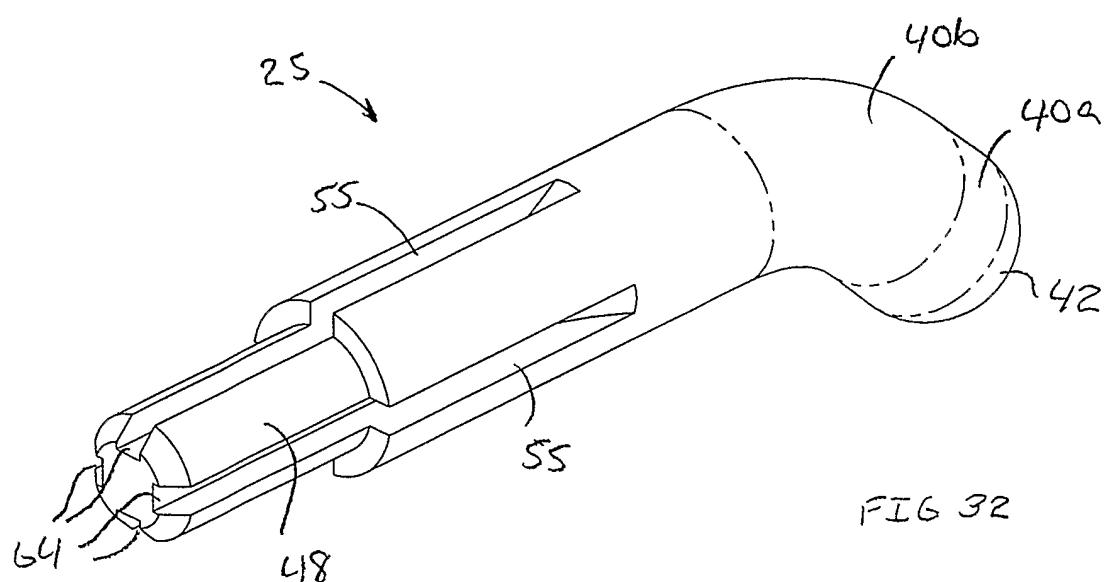
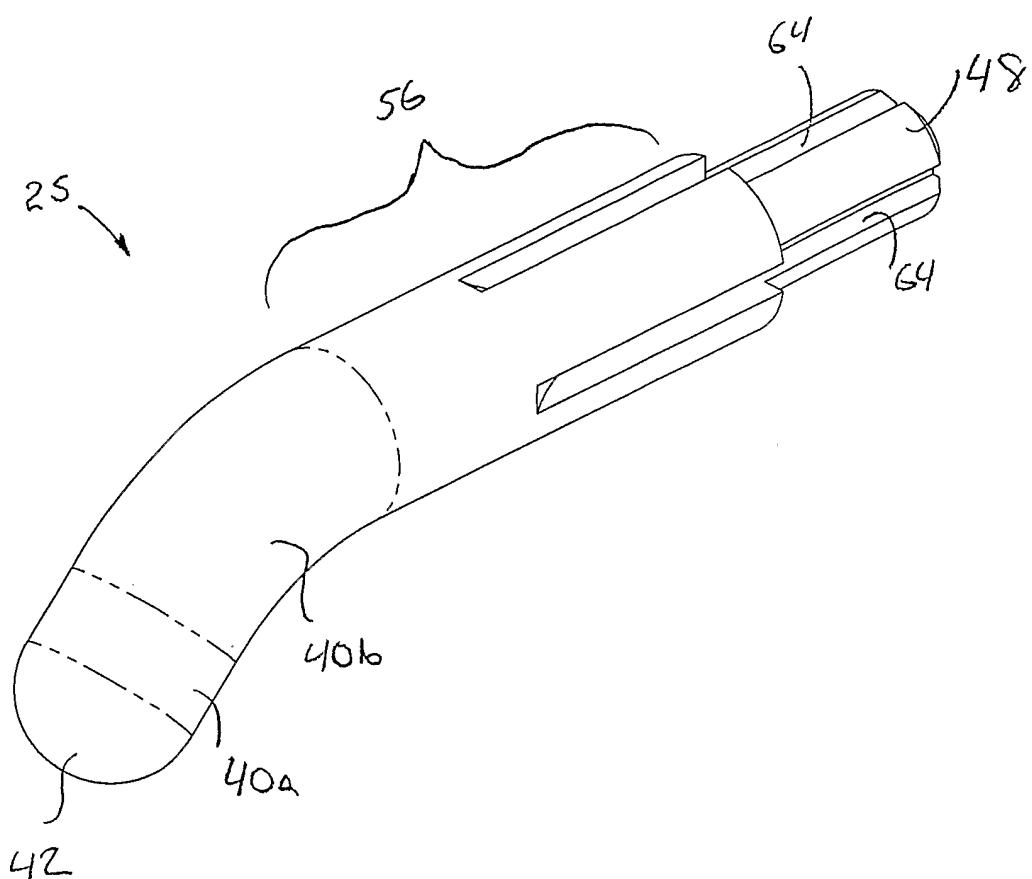


FIG 32

FIG. 33

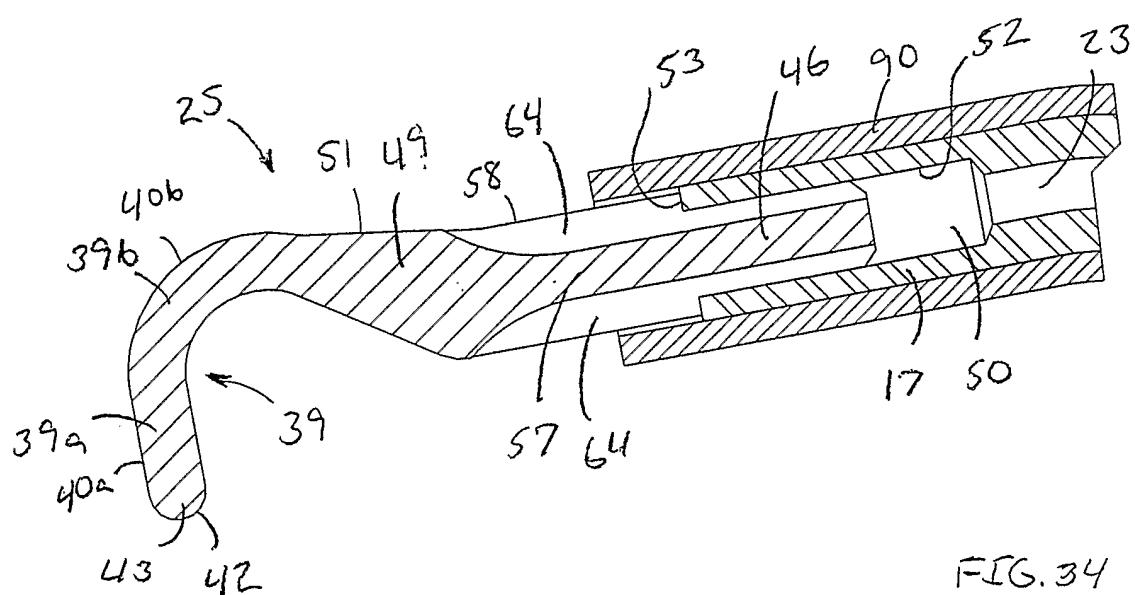
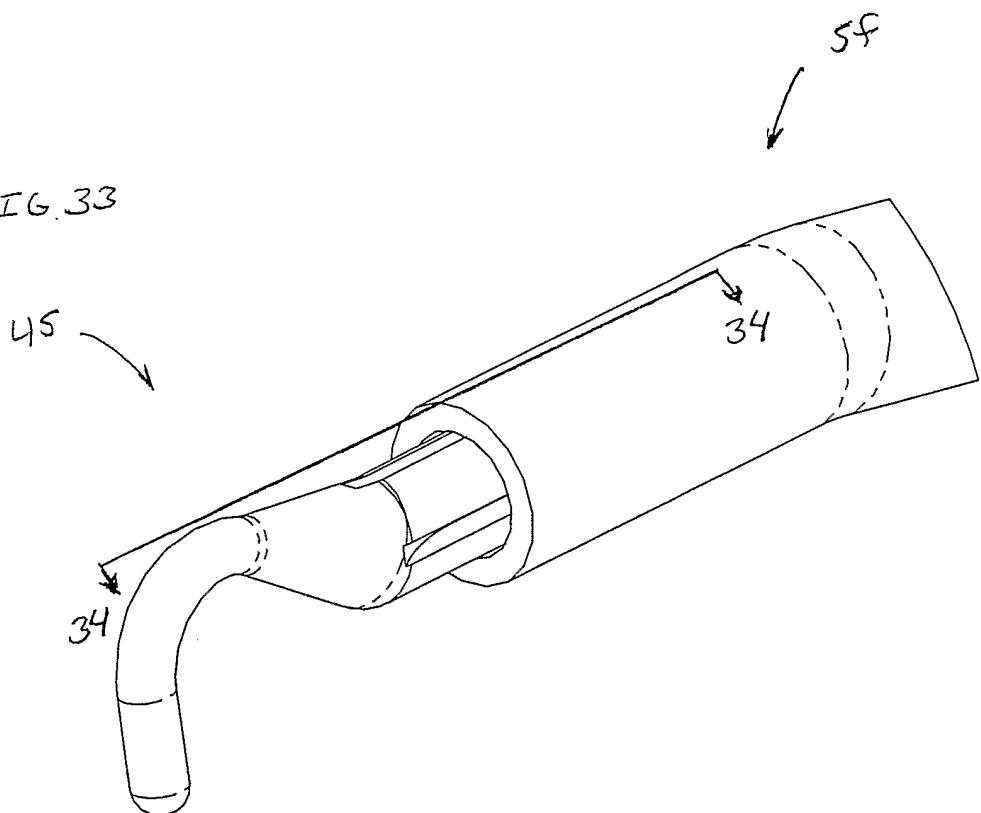


FIG. 34

FIG. 35

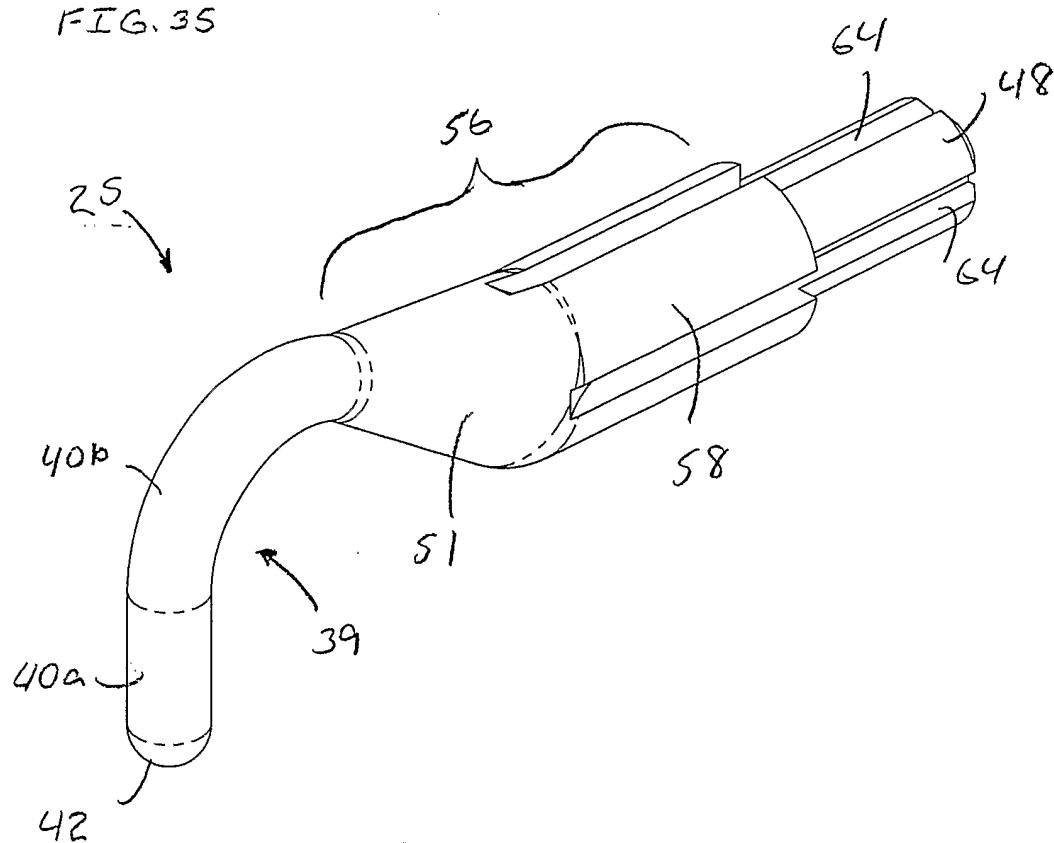
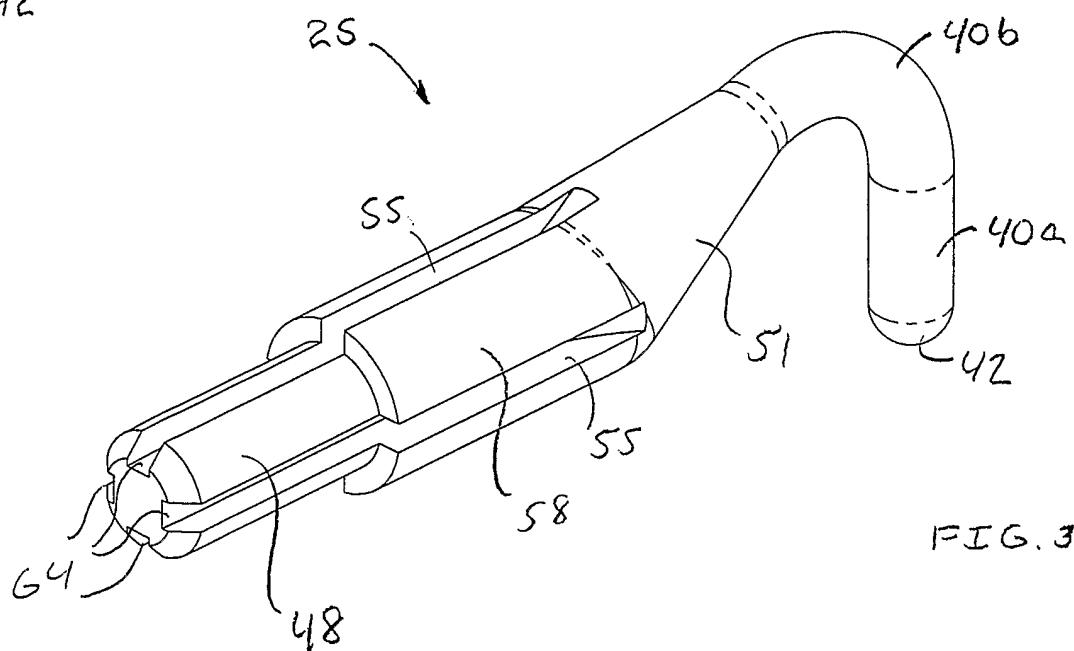


FIG. 36



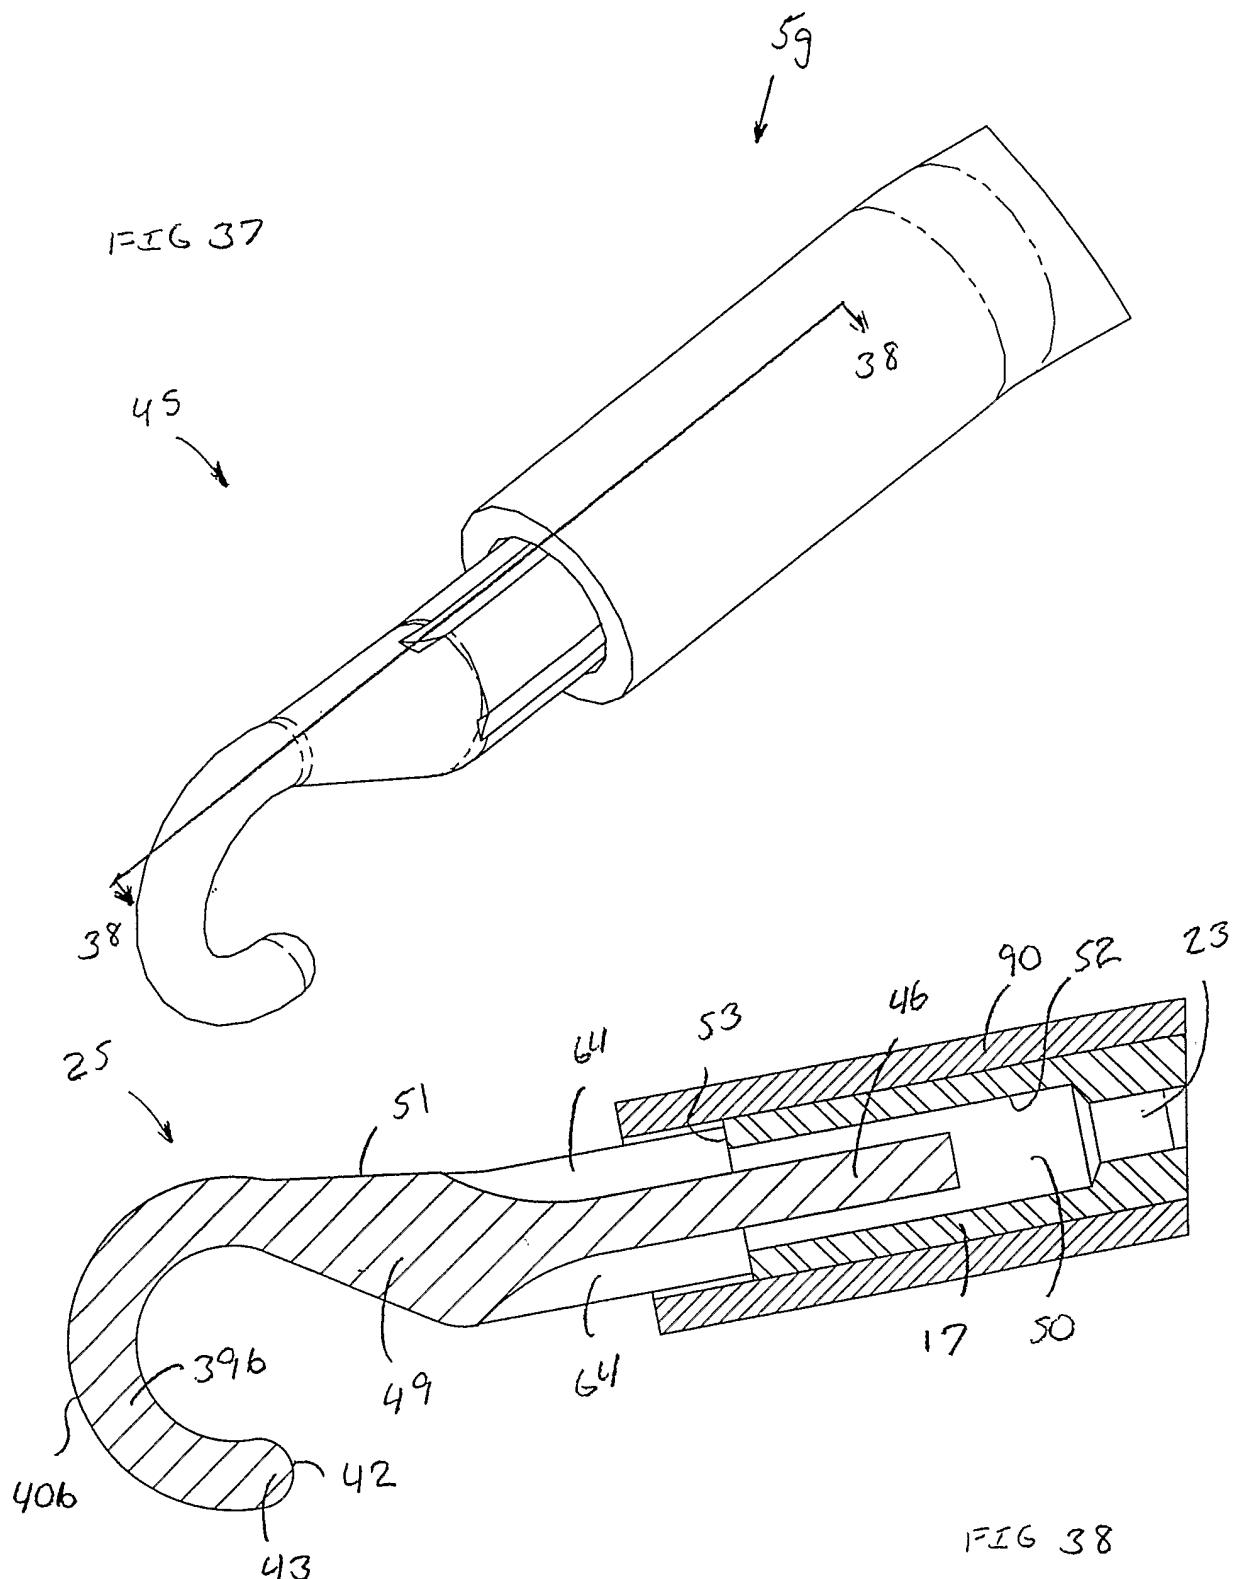


FIG. 39

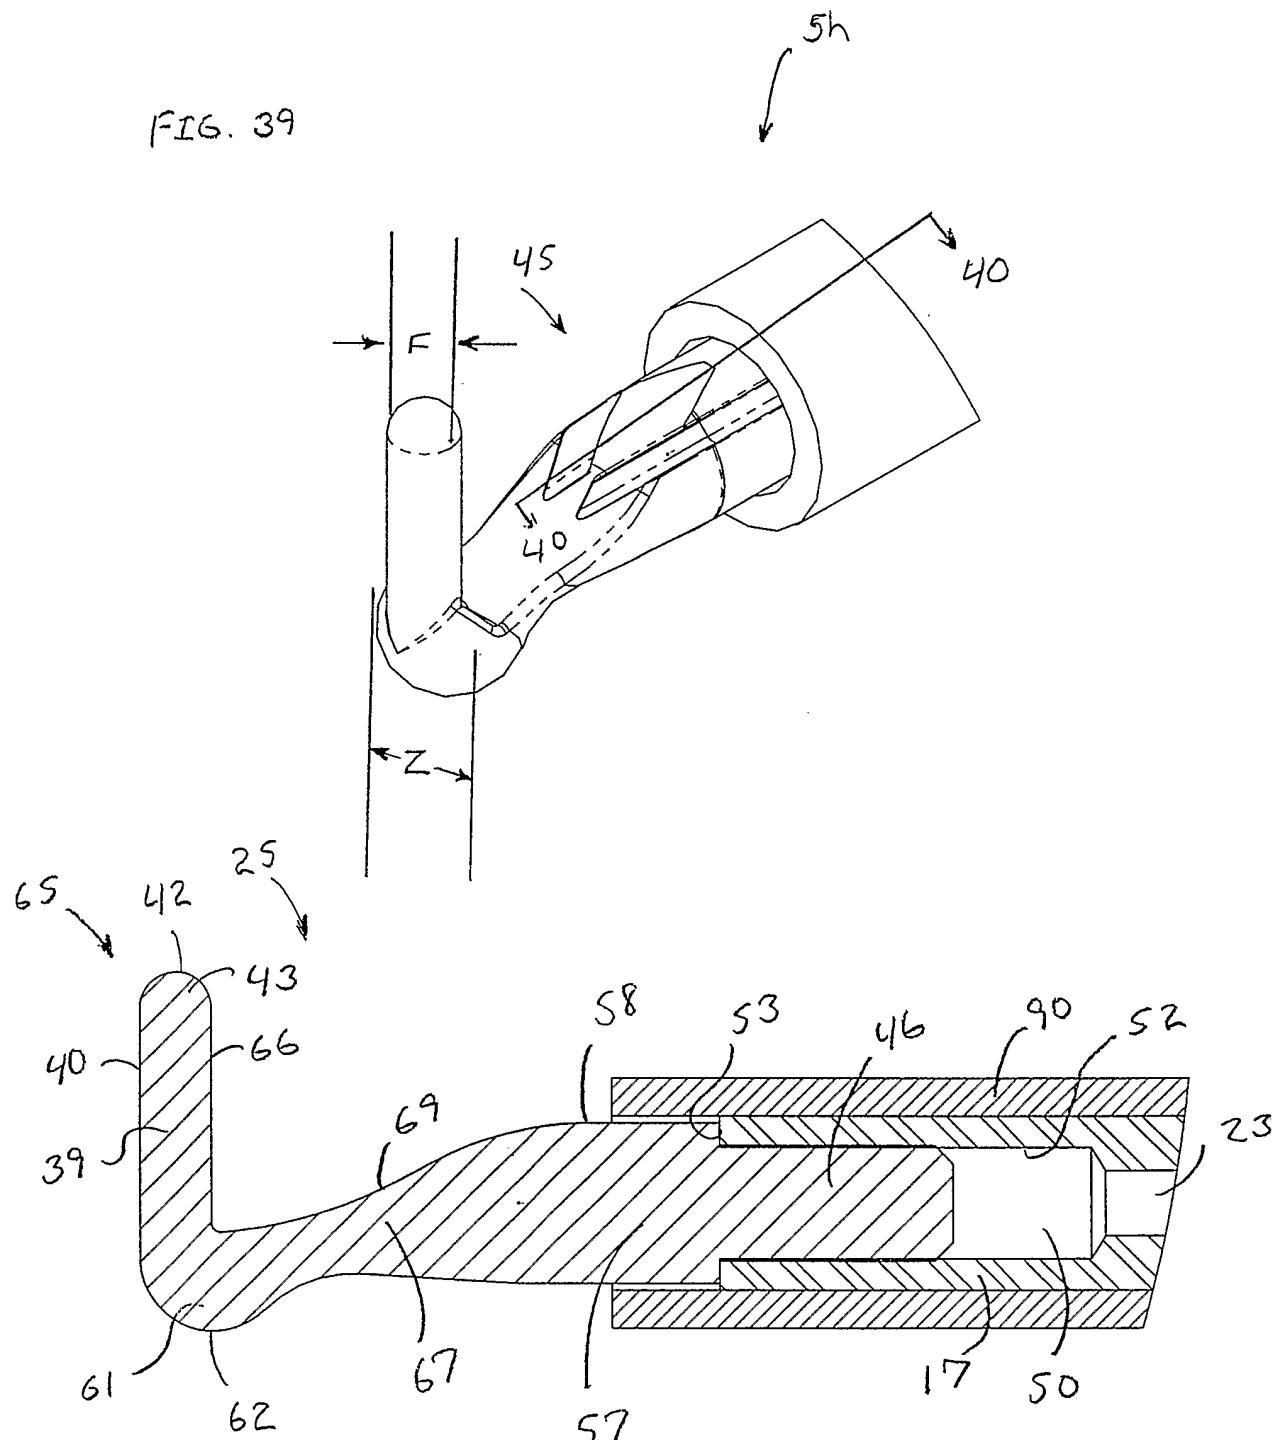


FIG 40

FIG. 41

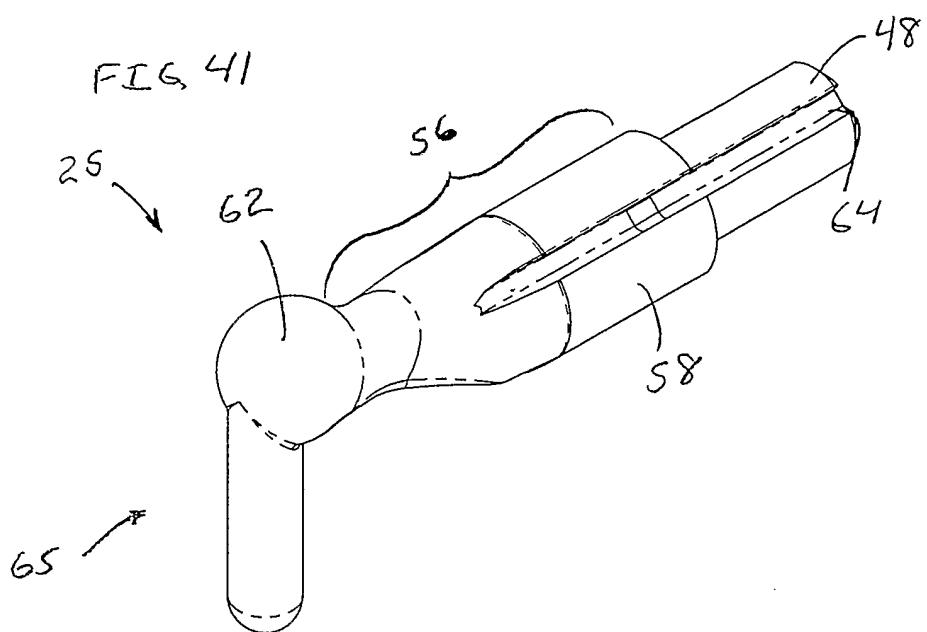
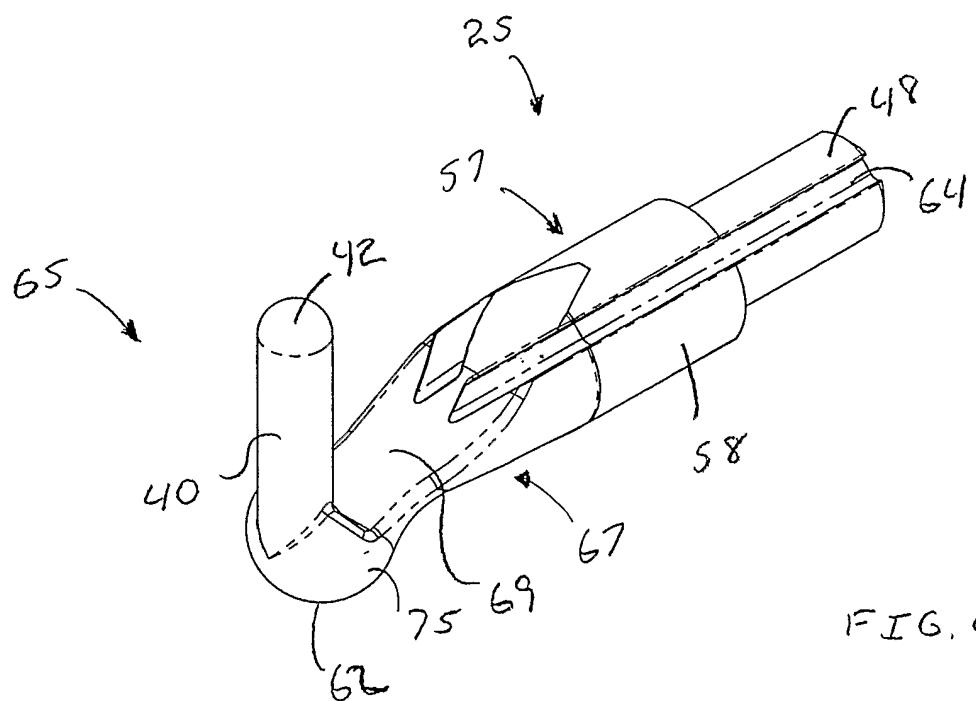


FIG. 42



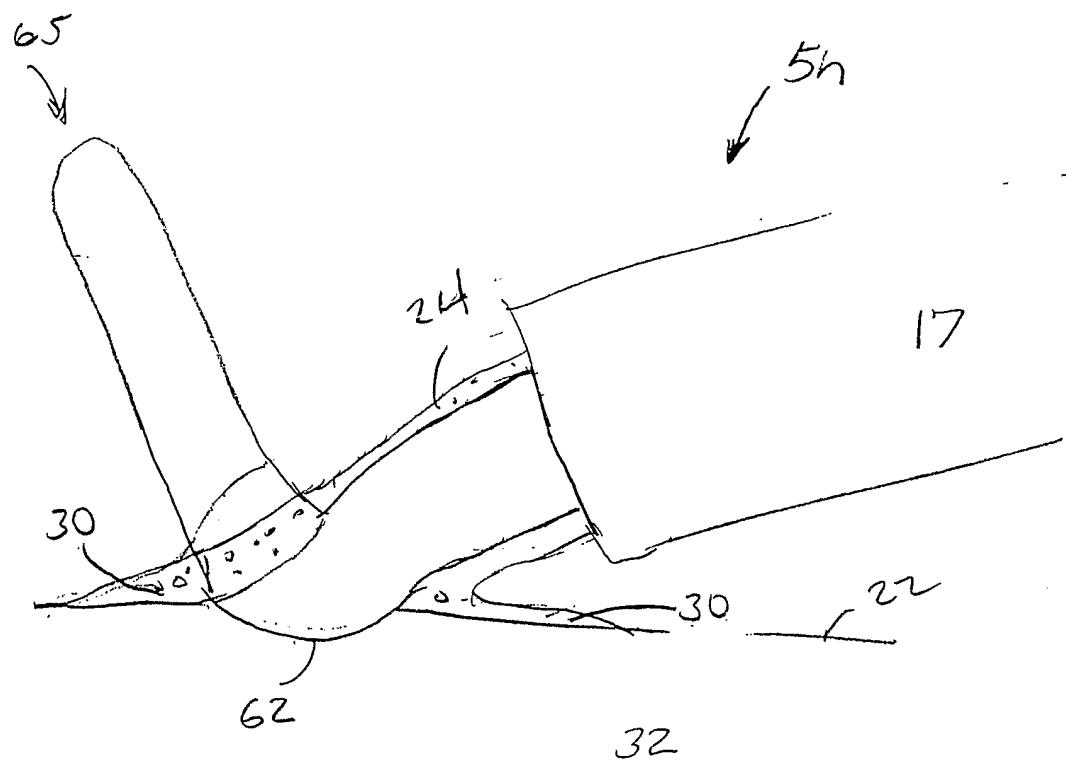


FIG. 43

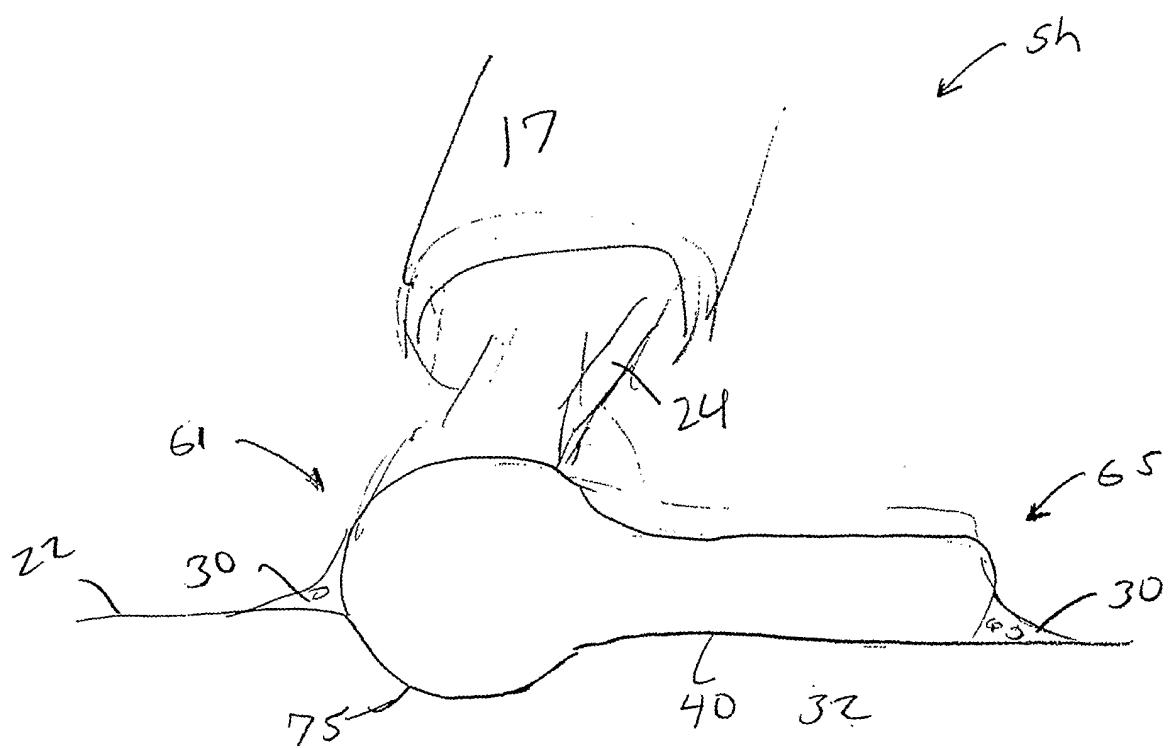


FIG. 44

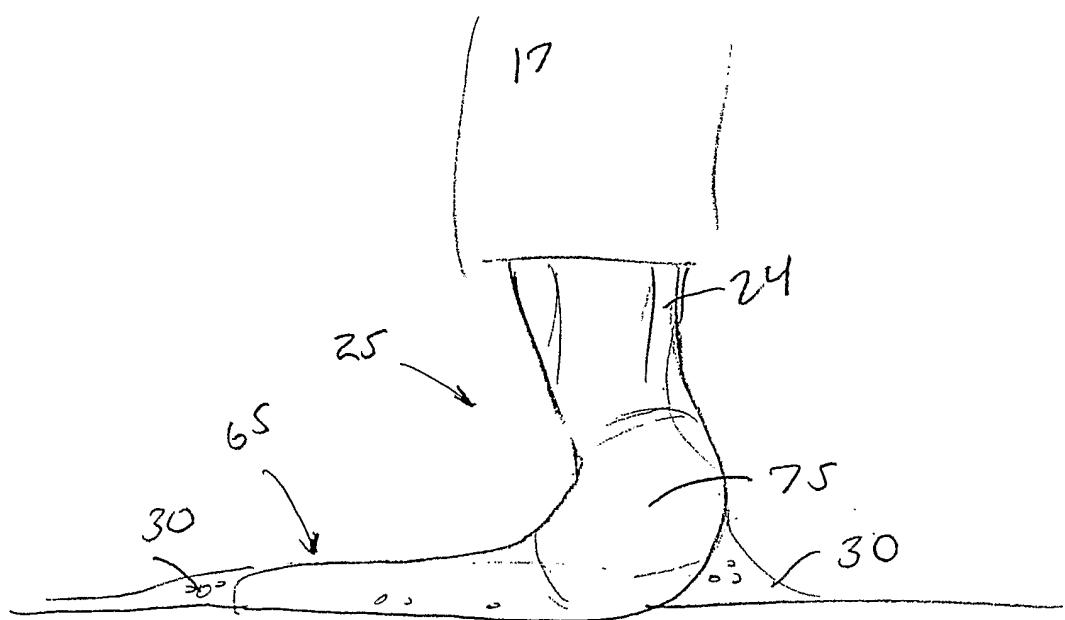
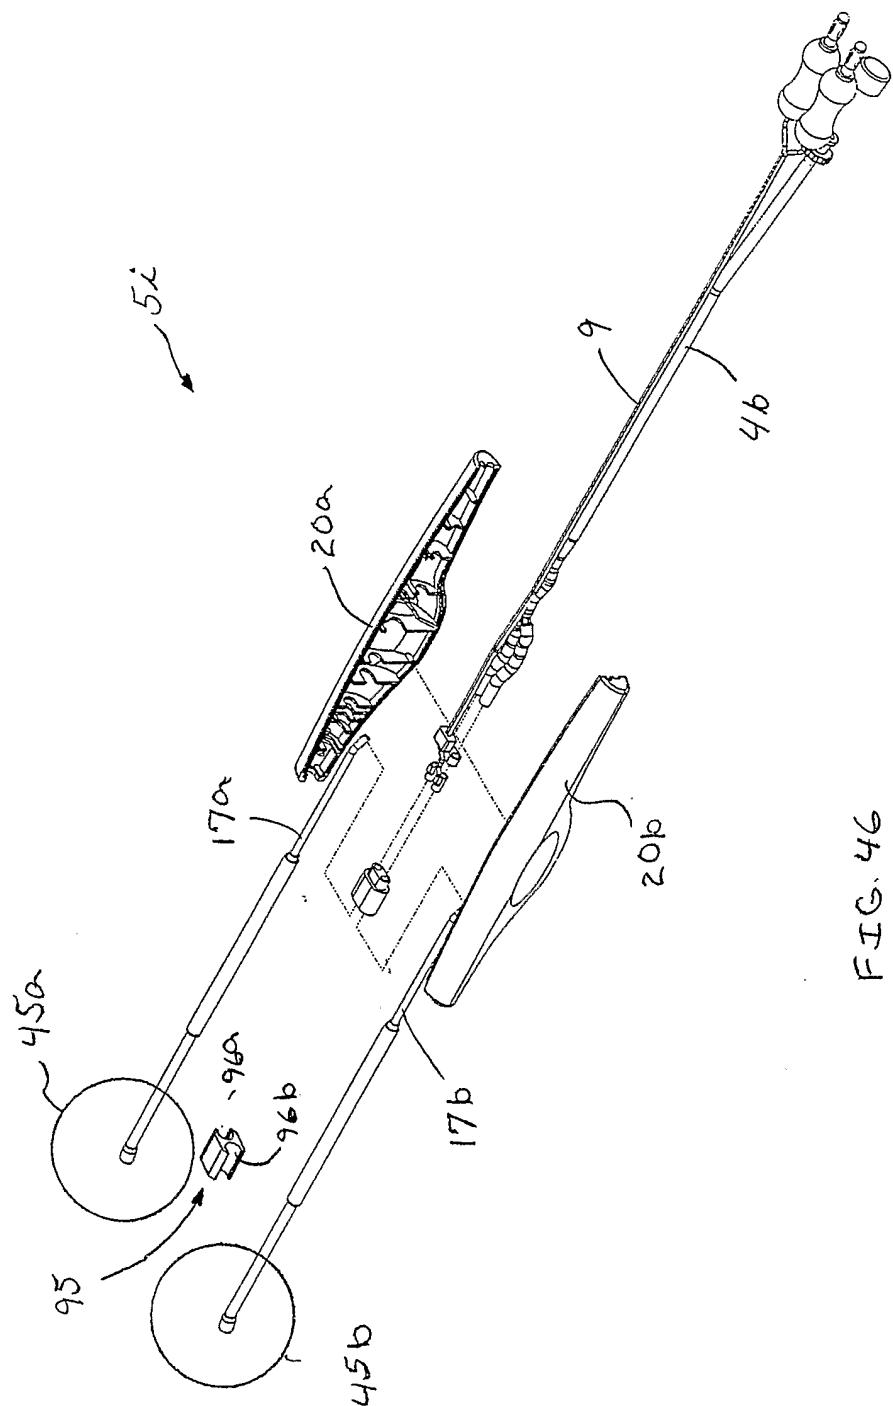


FIG. 45



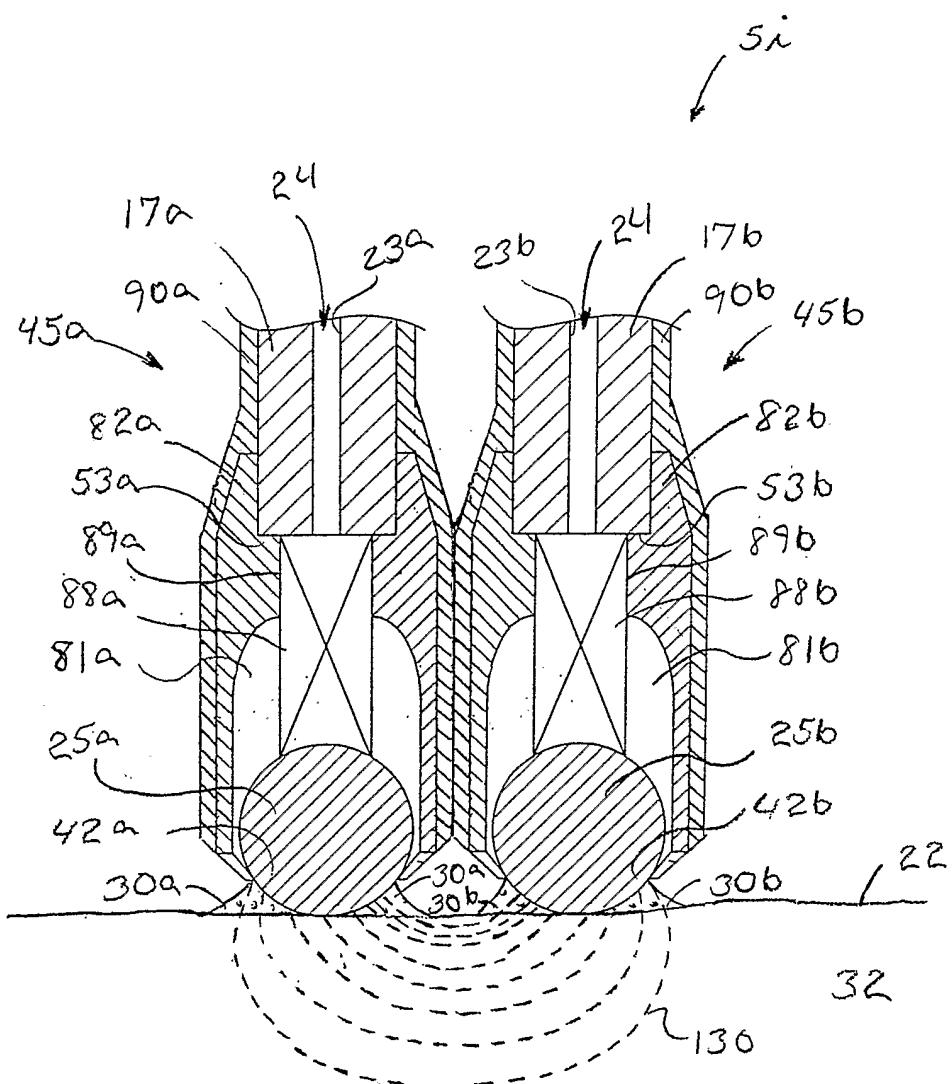


FIG. 47

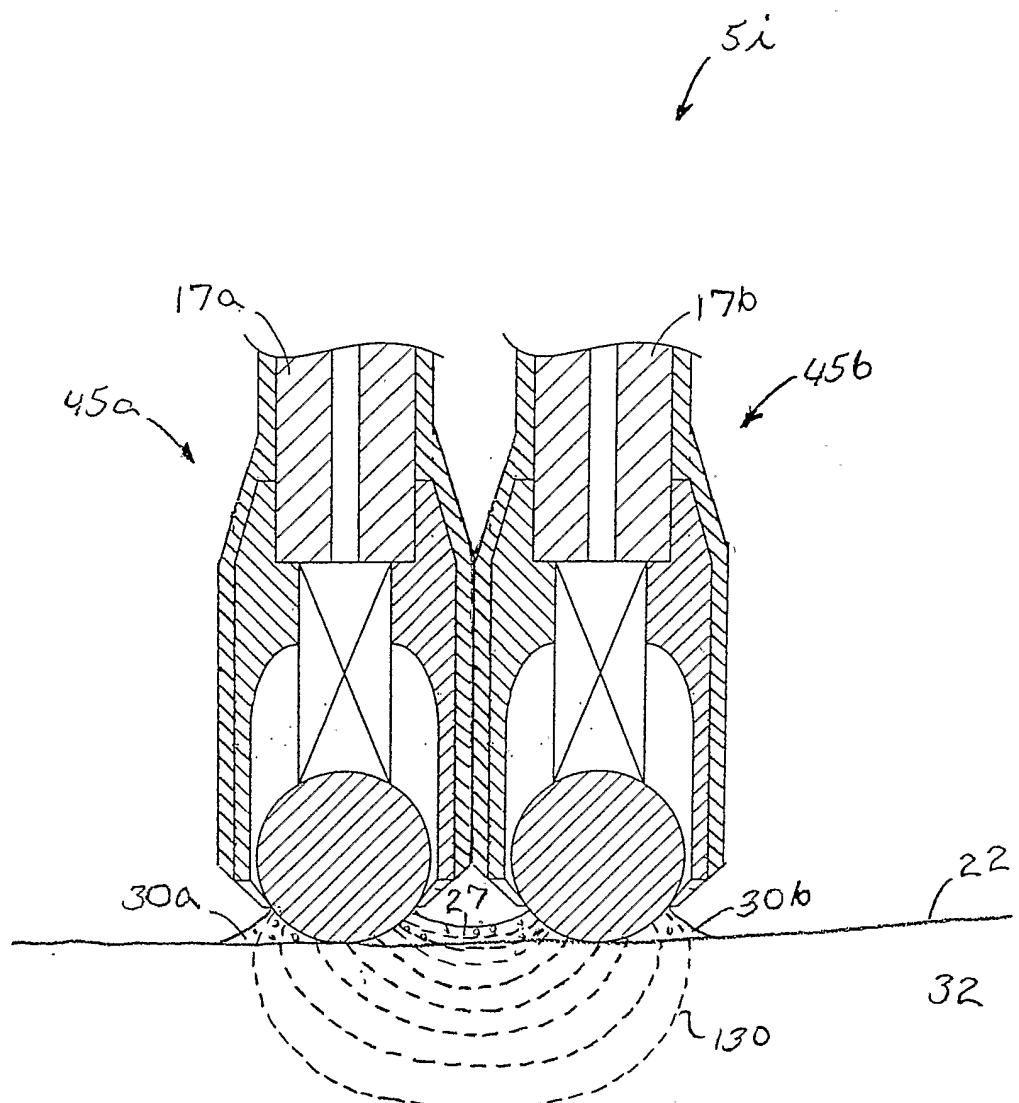


FIG. 48

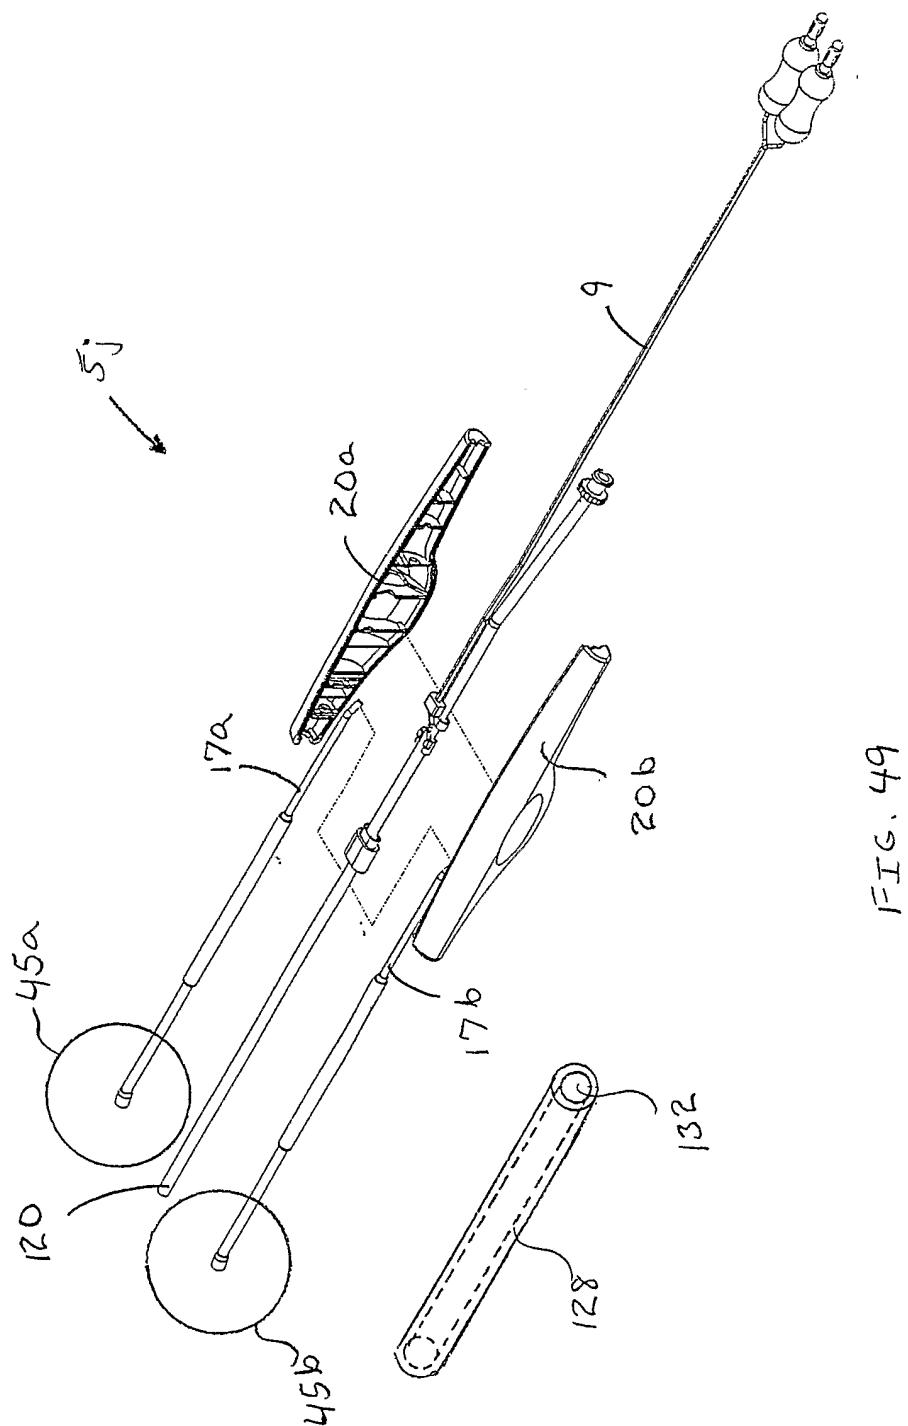
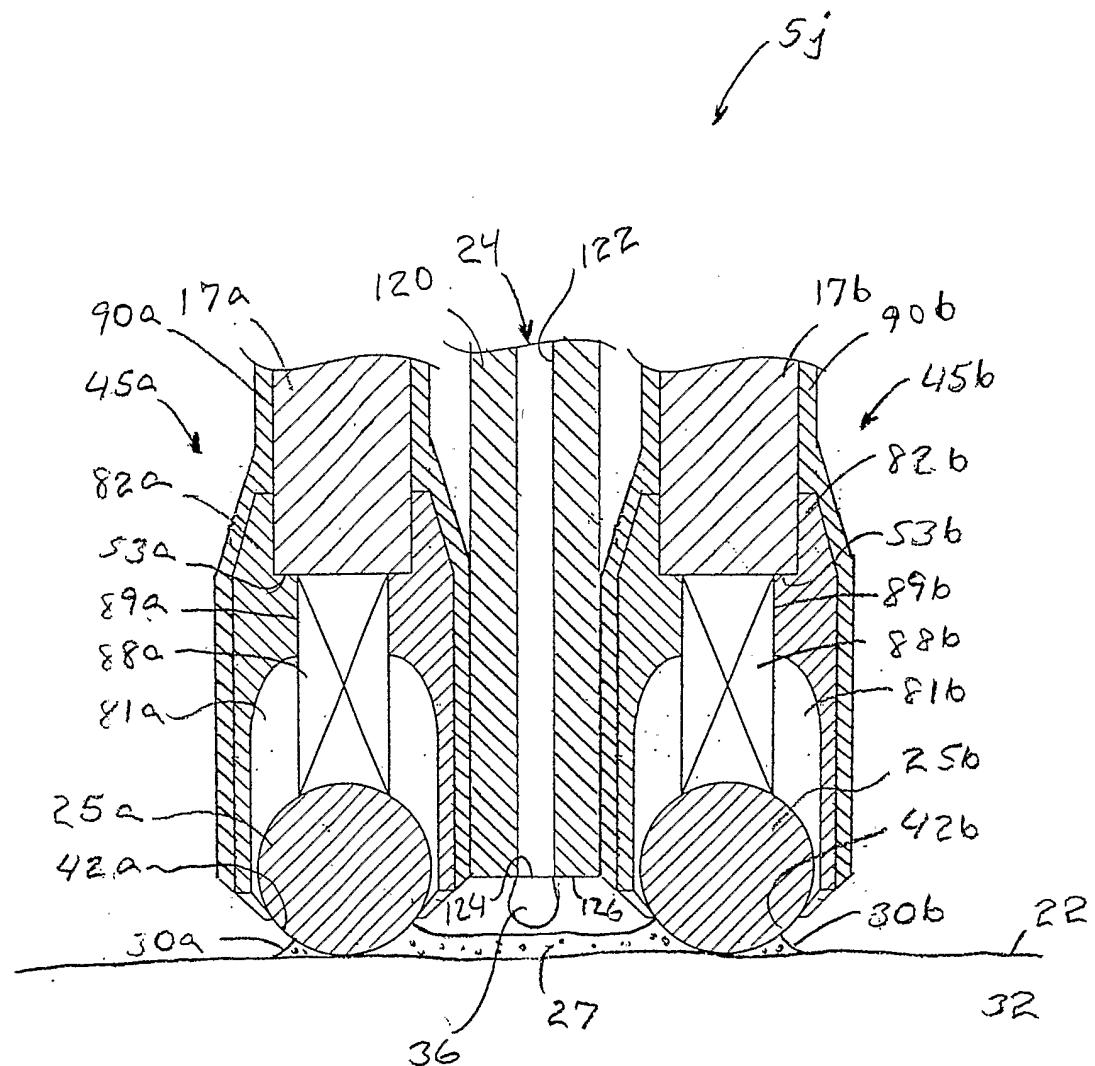


FIG. 49



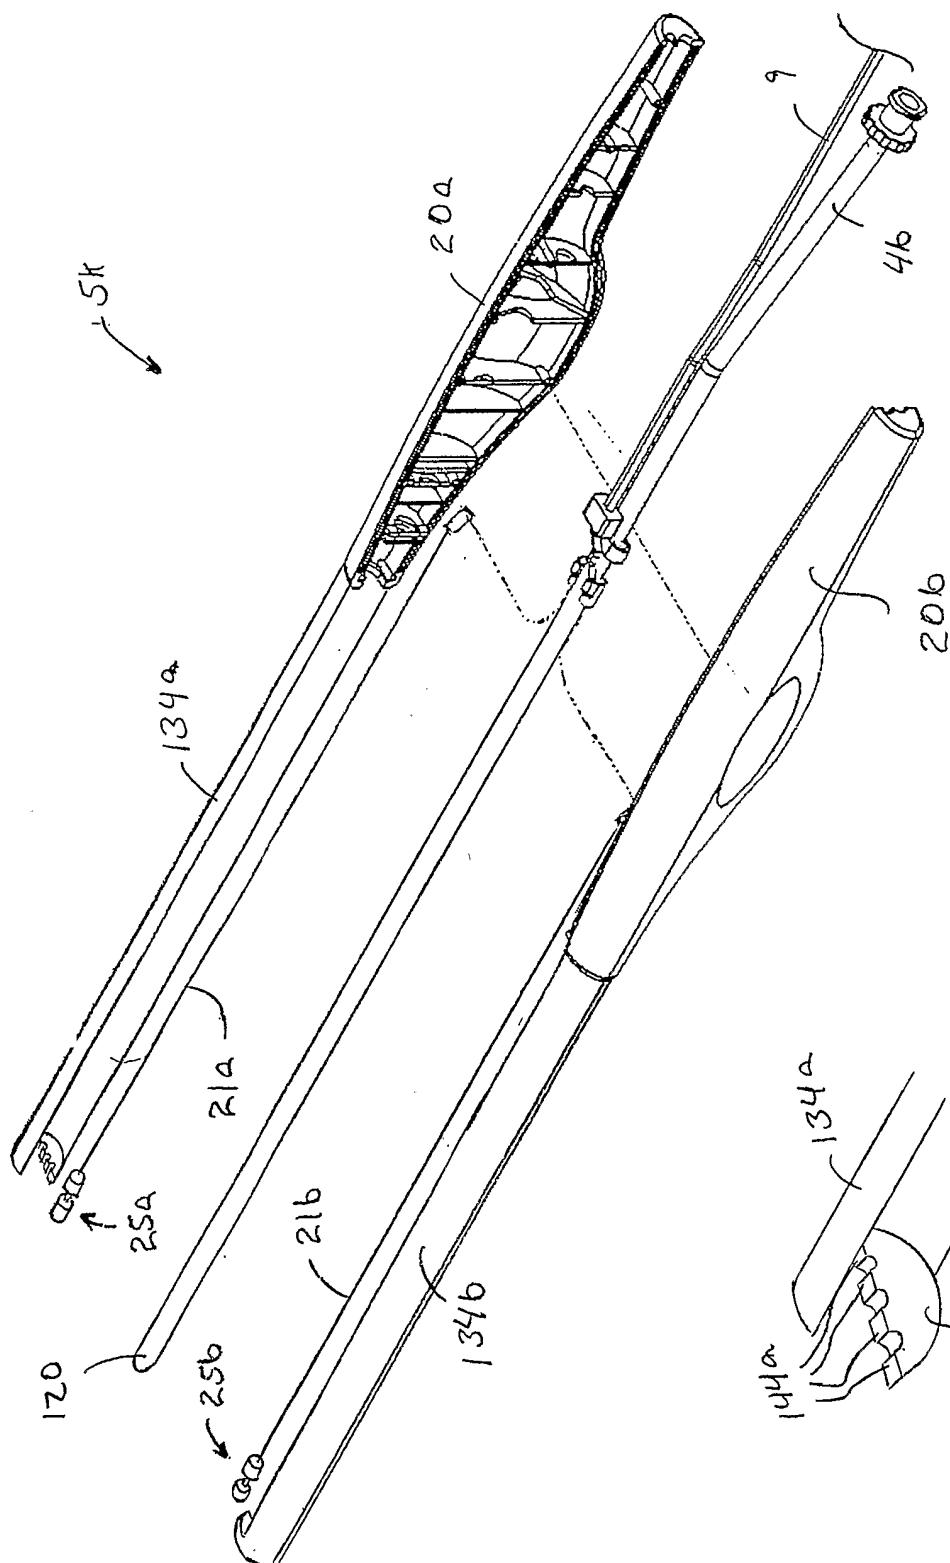


FIG 51

FIG. 52

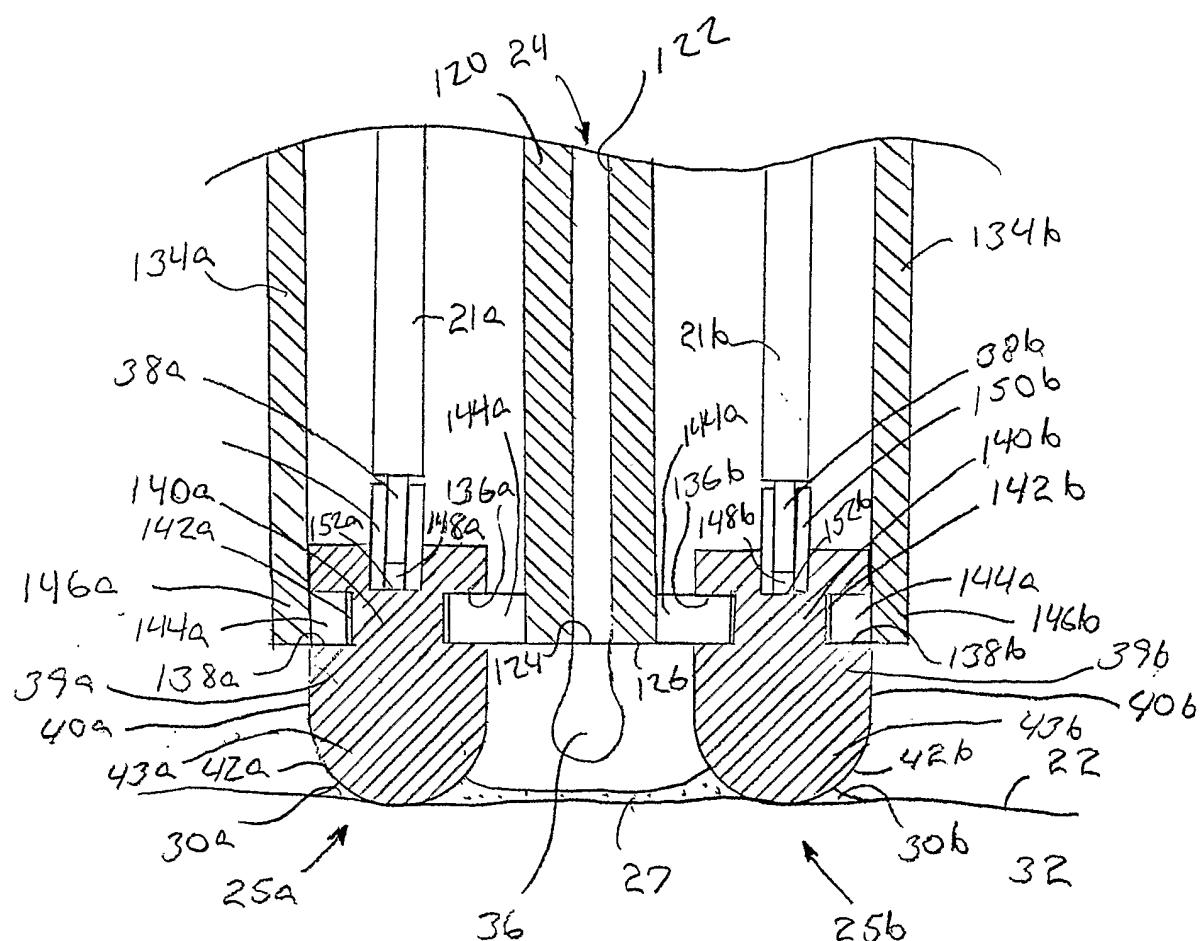
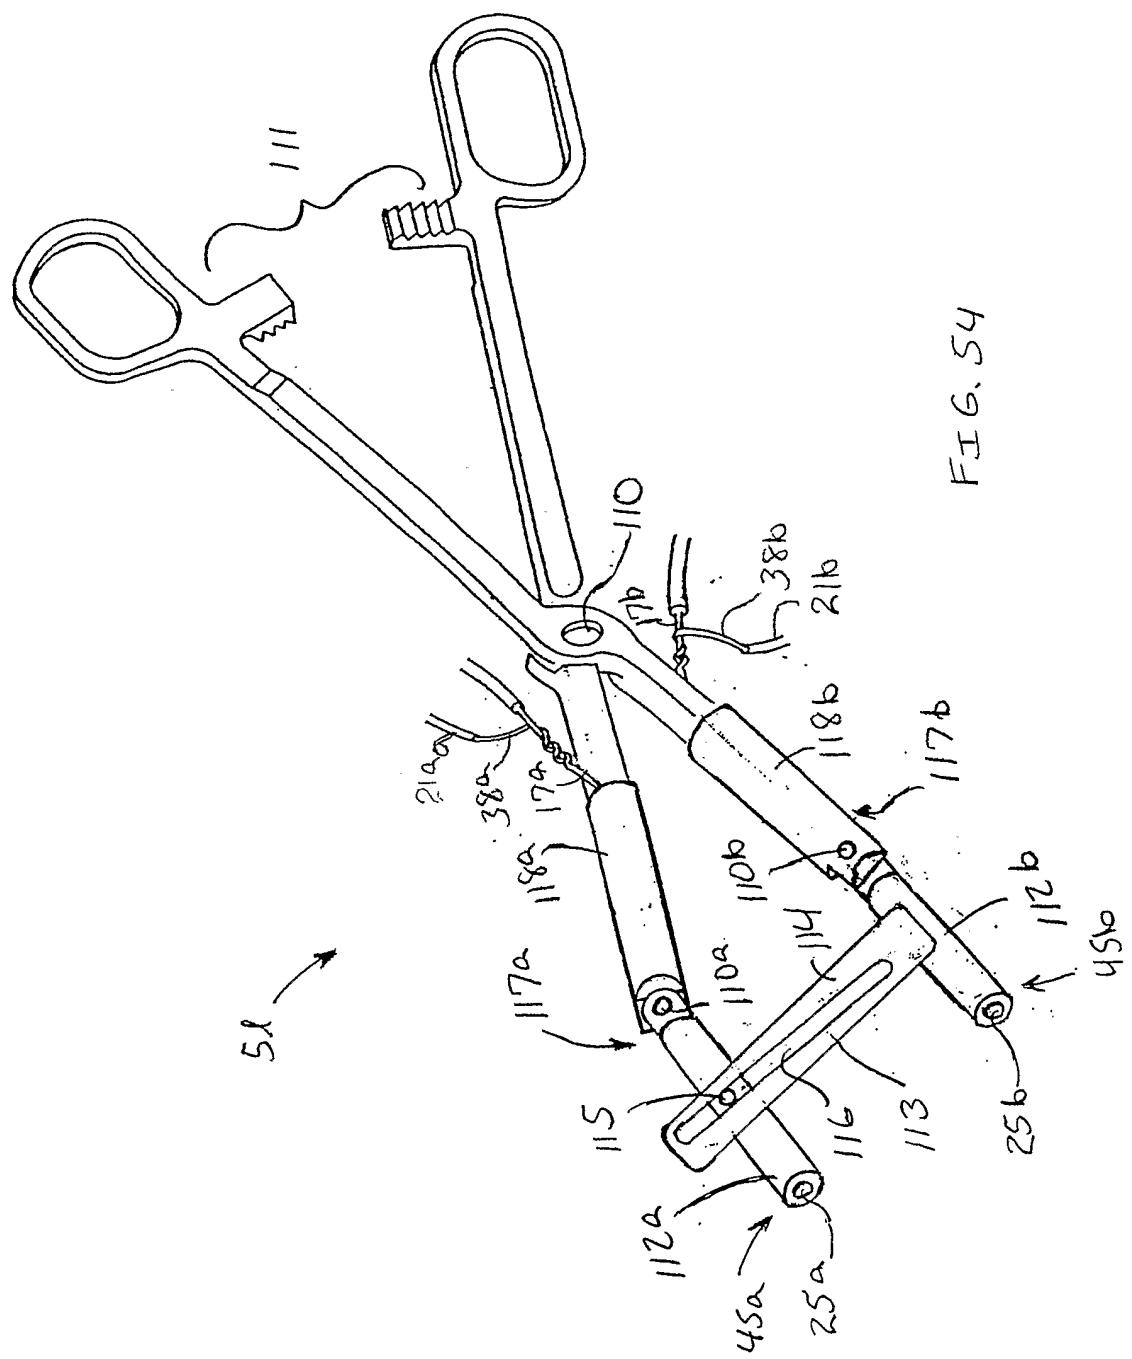
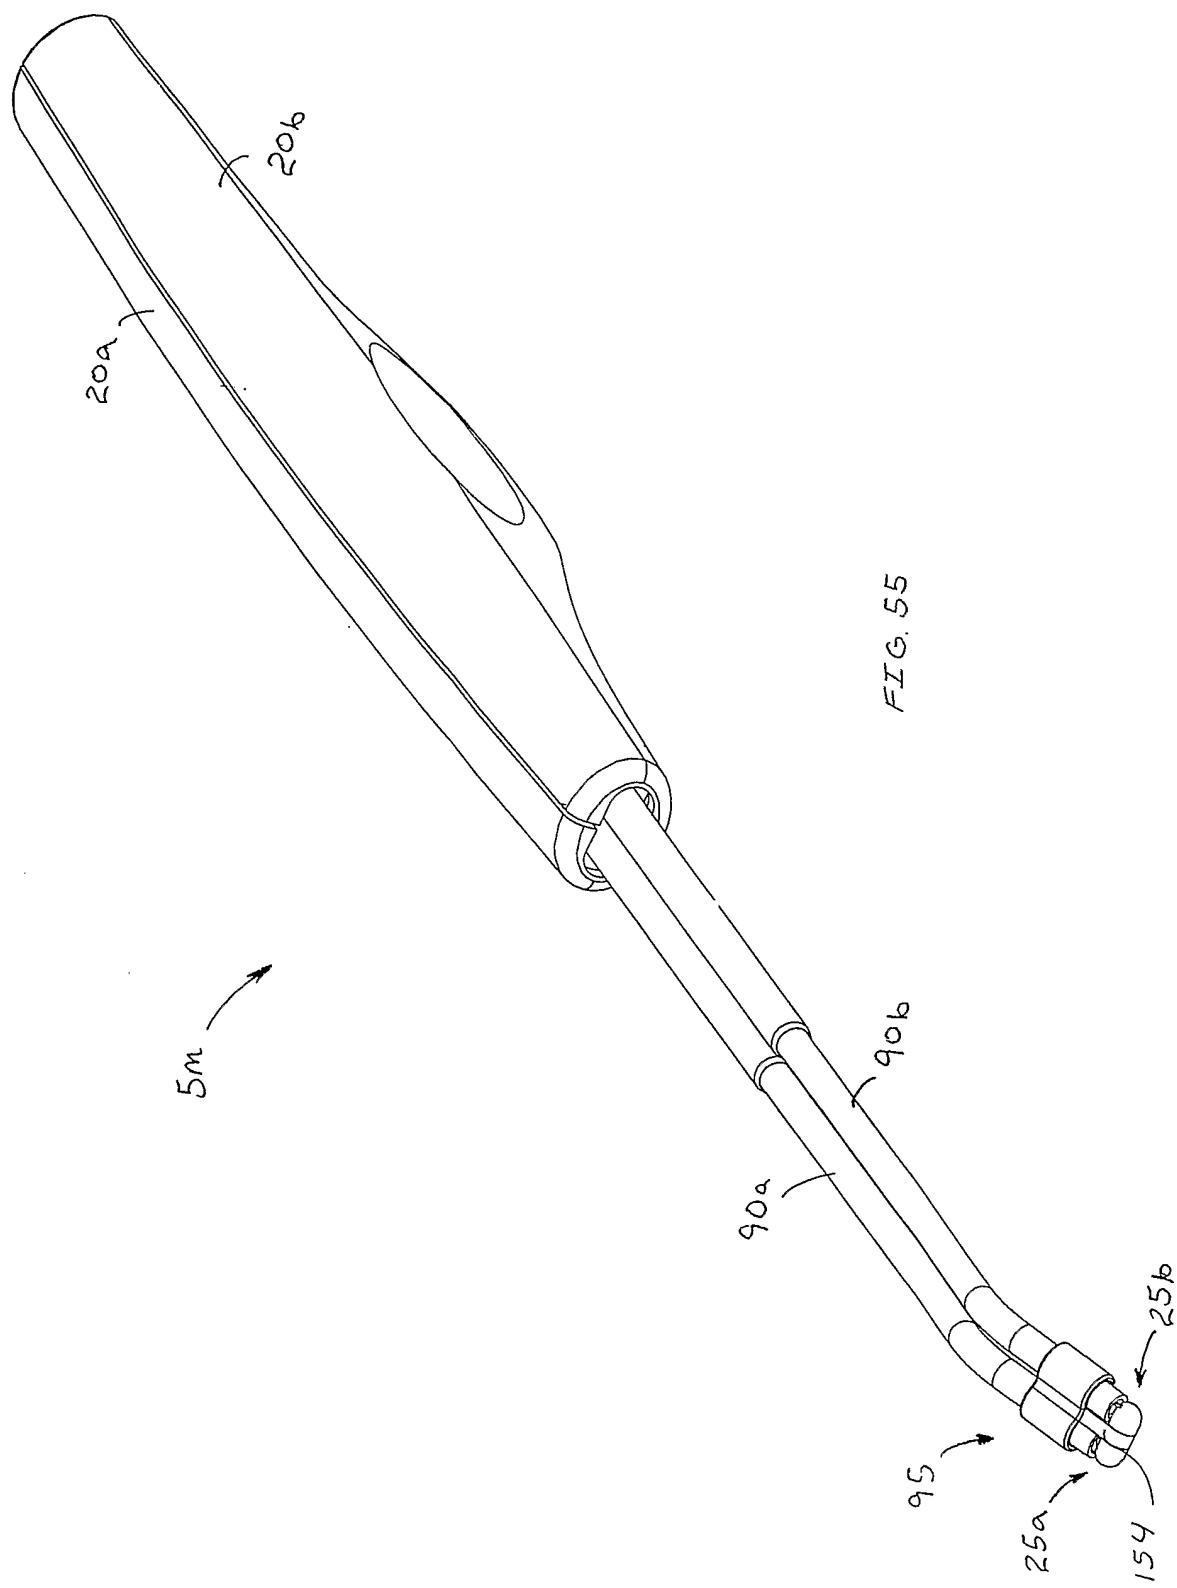
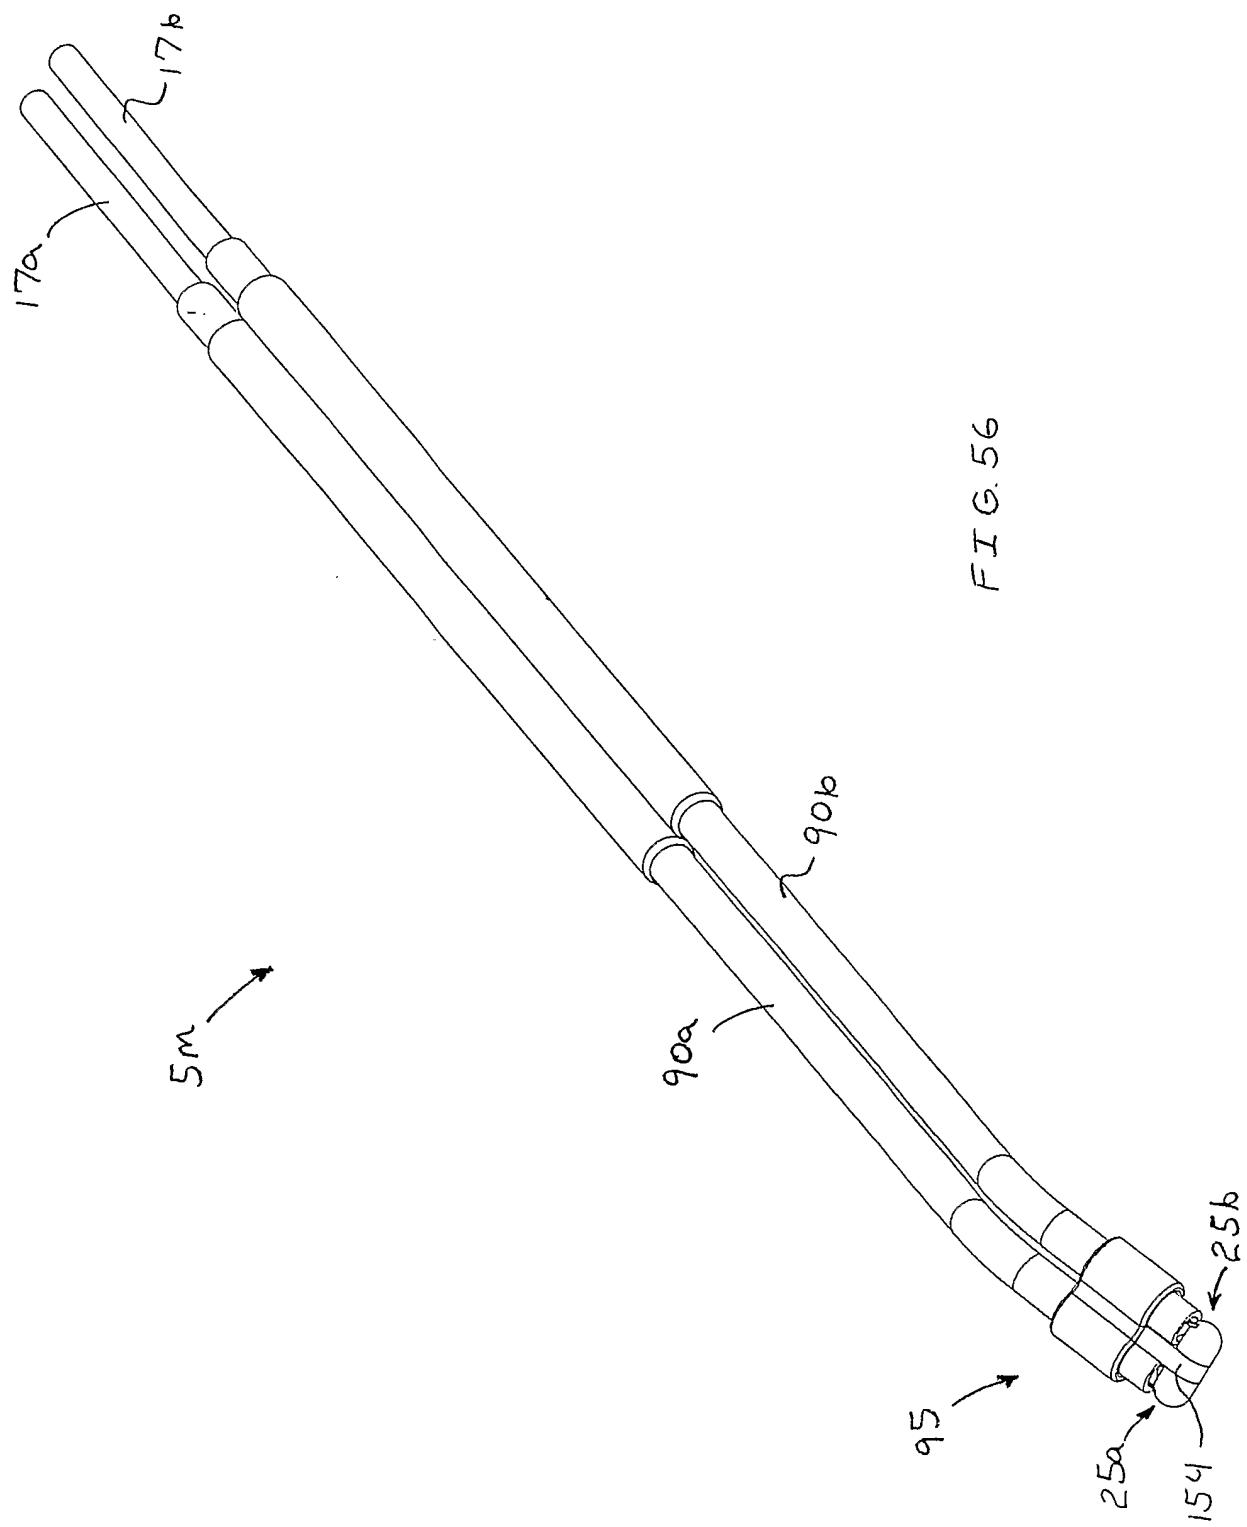


FIG 53







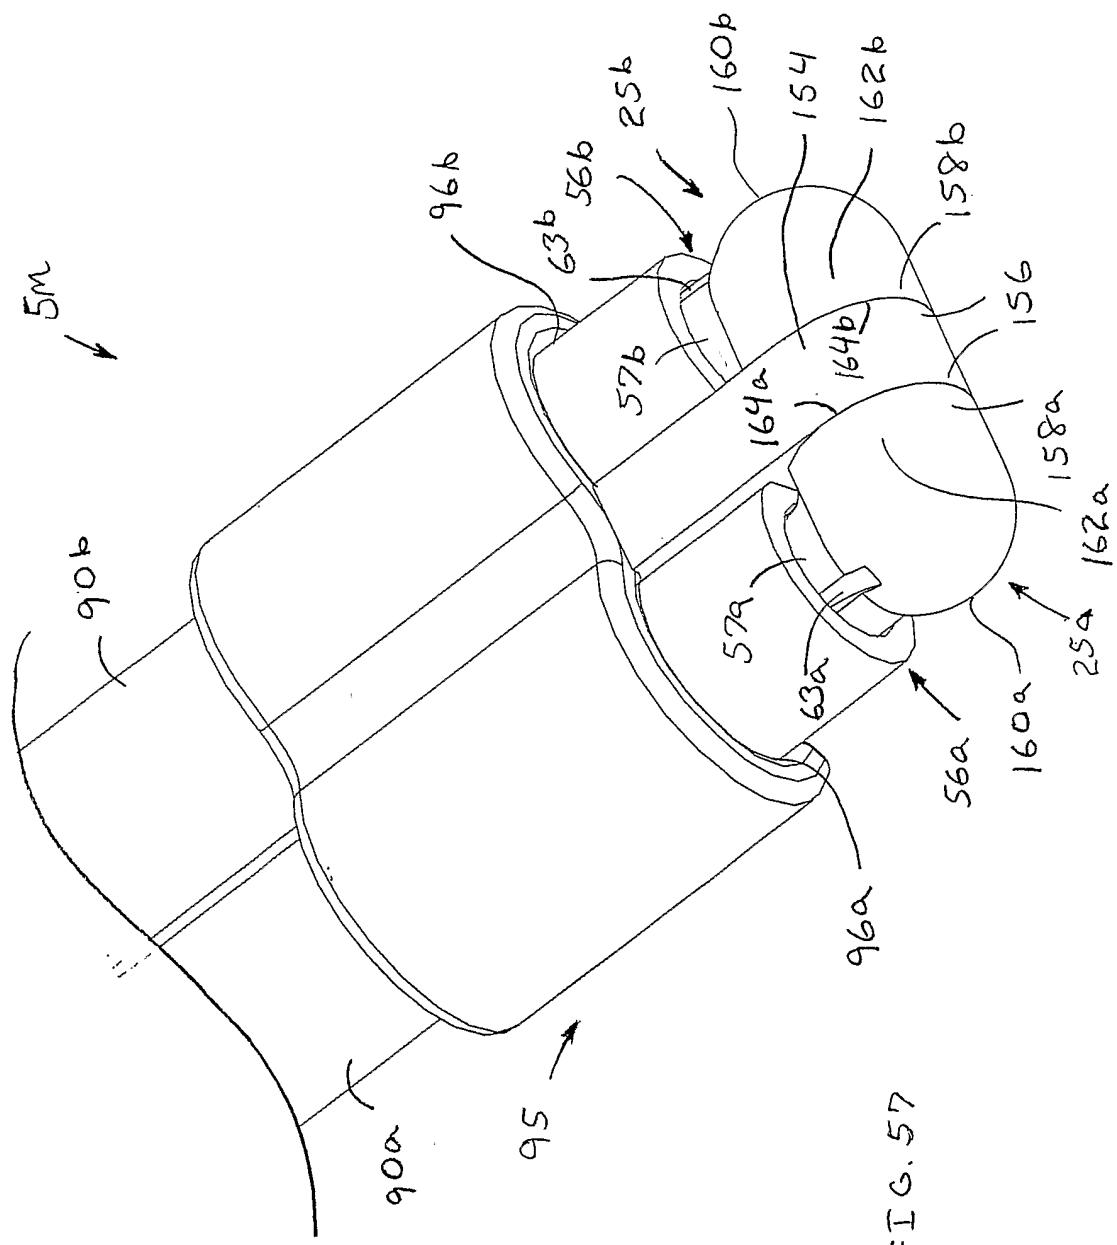


FIG. 57

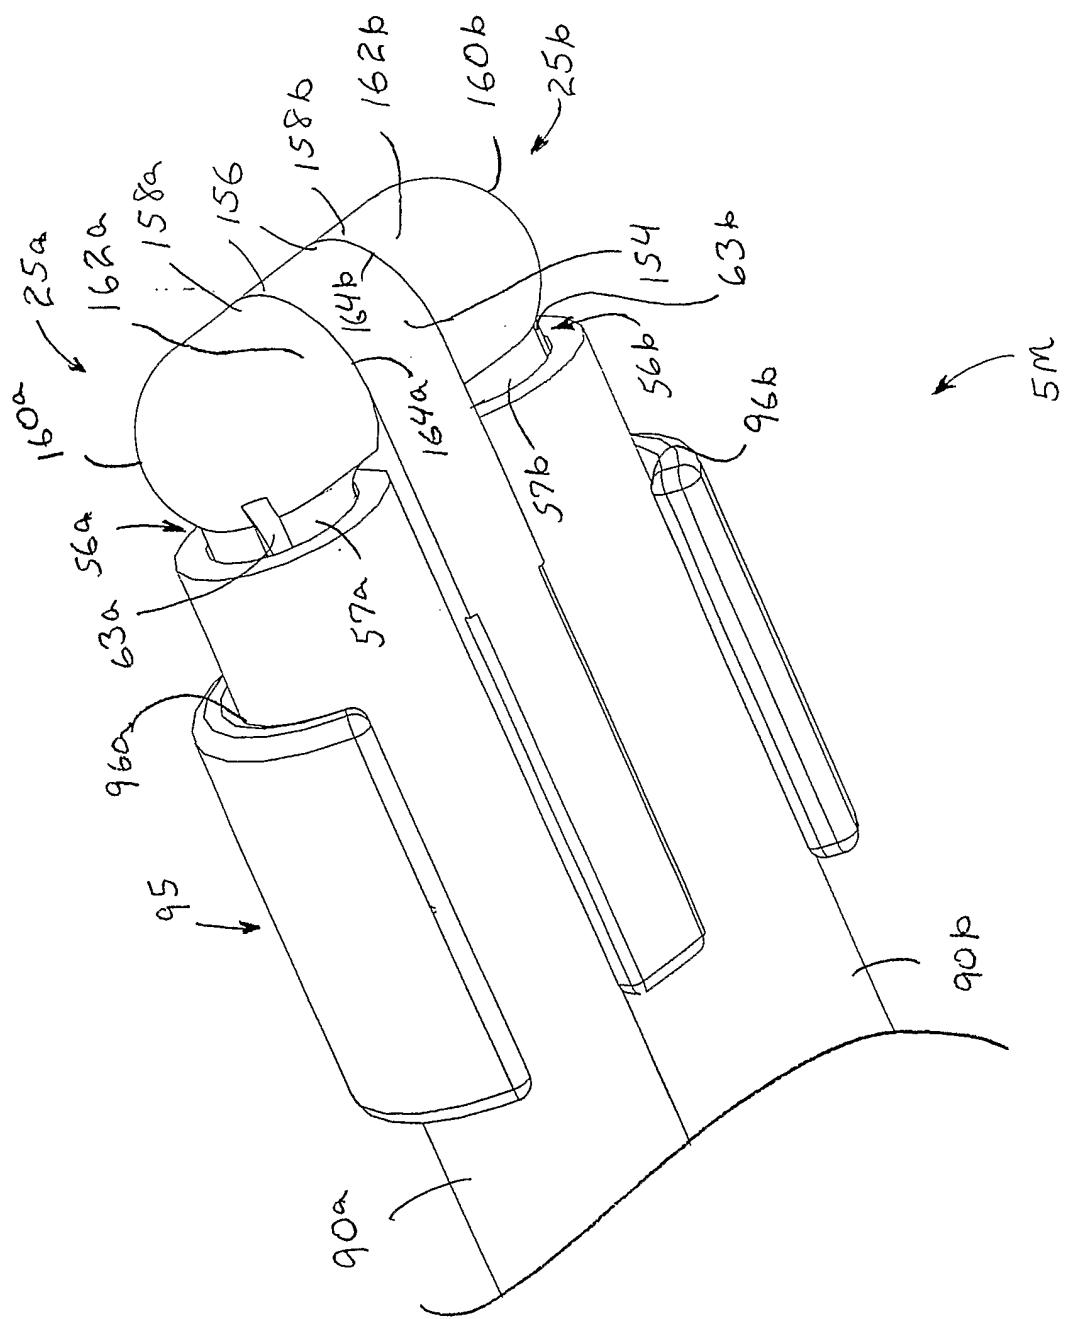
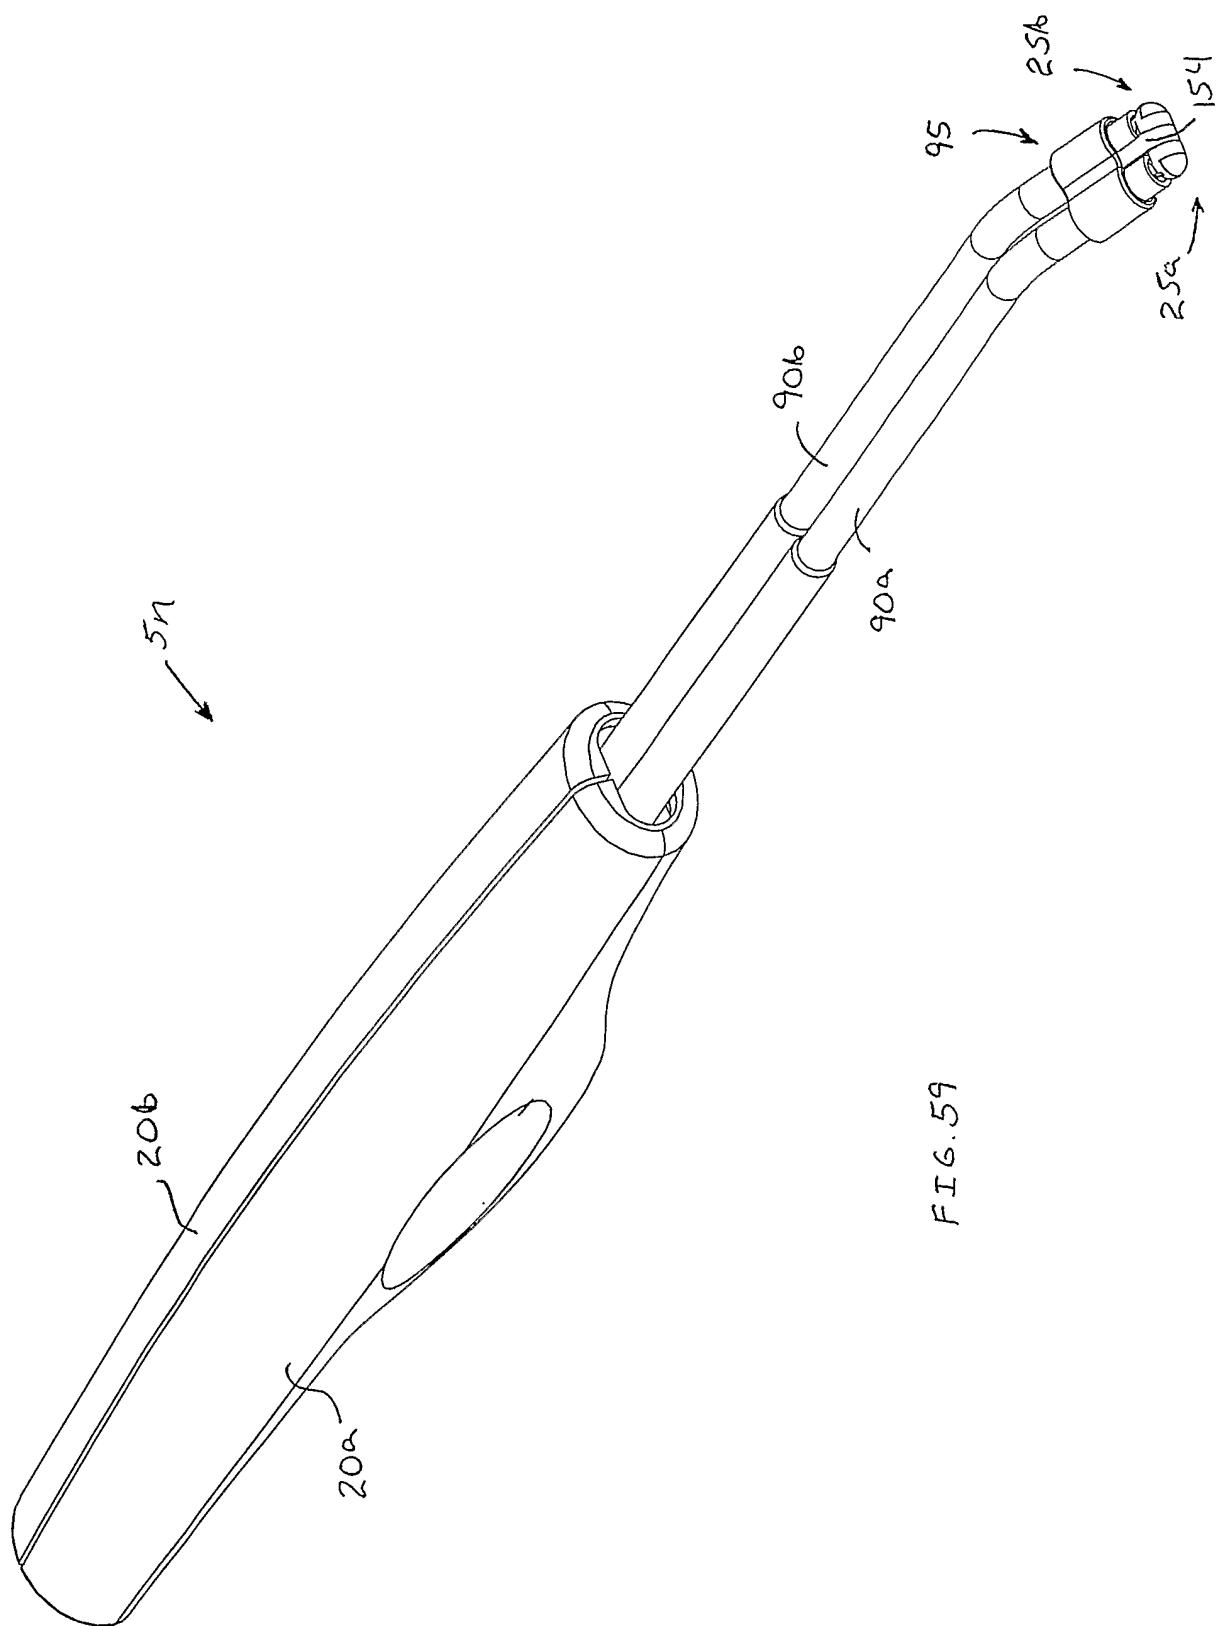
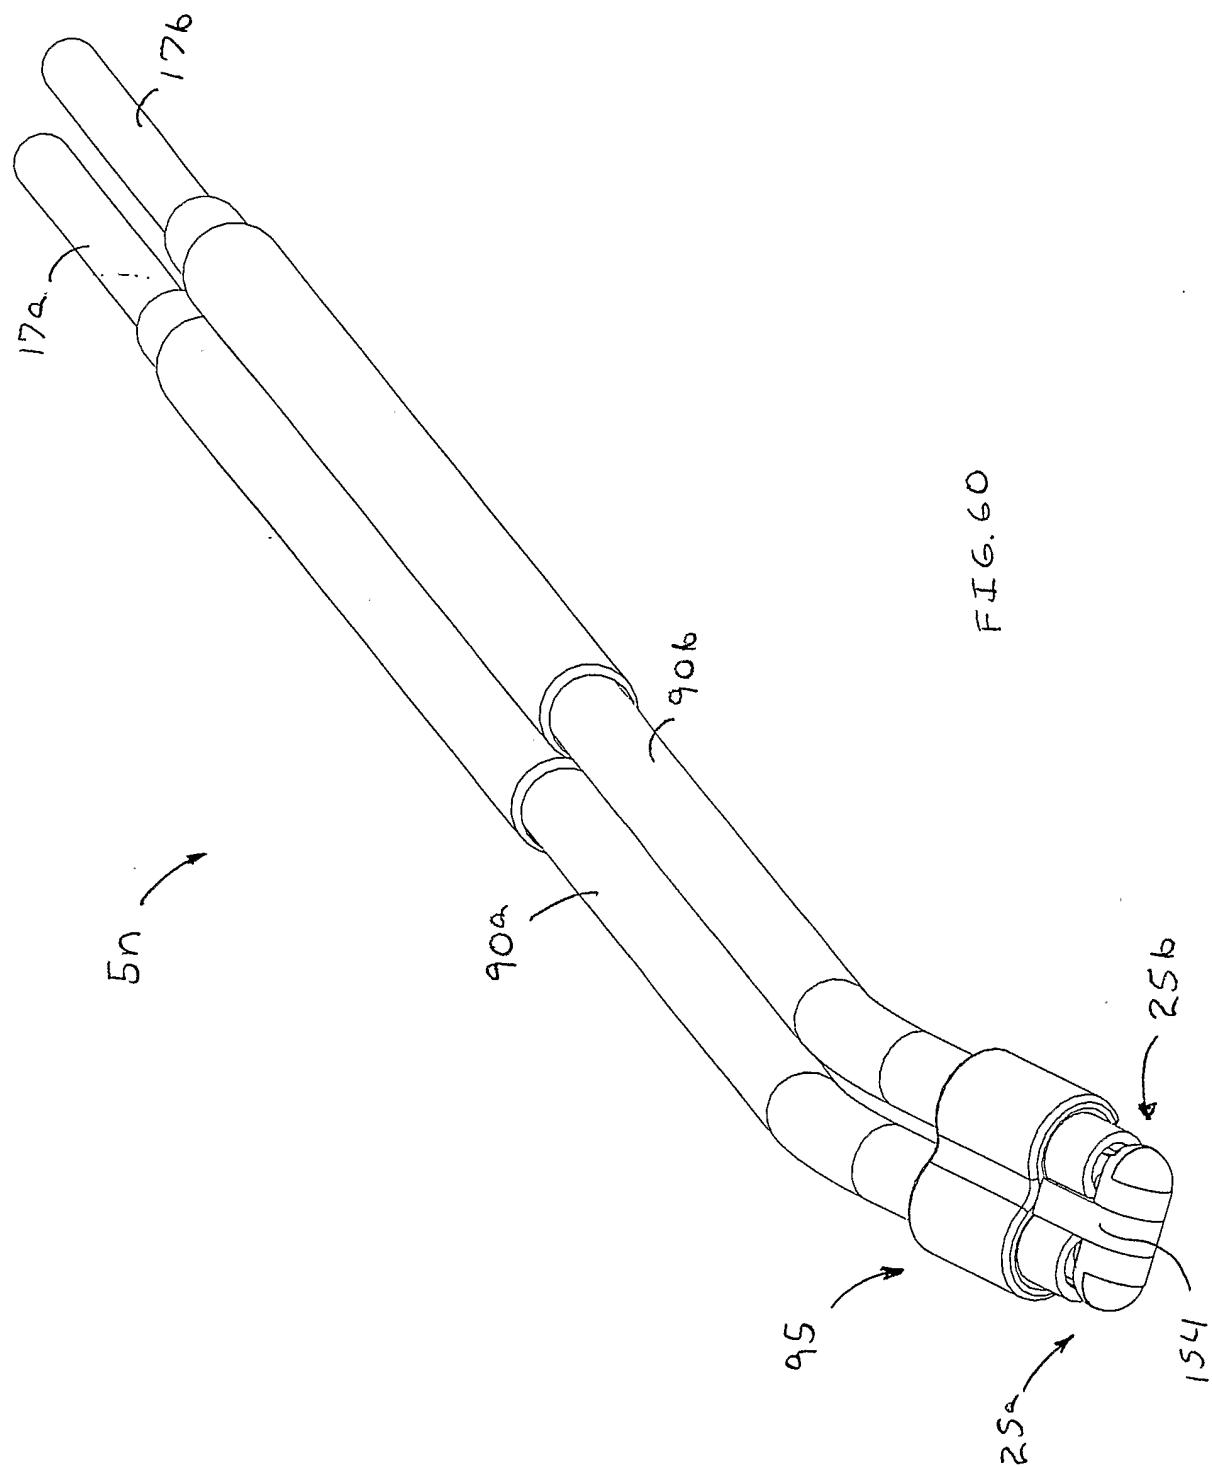


FIG. 58





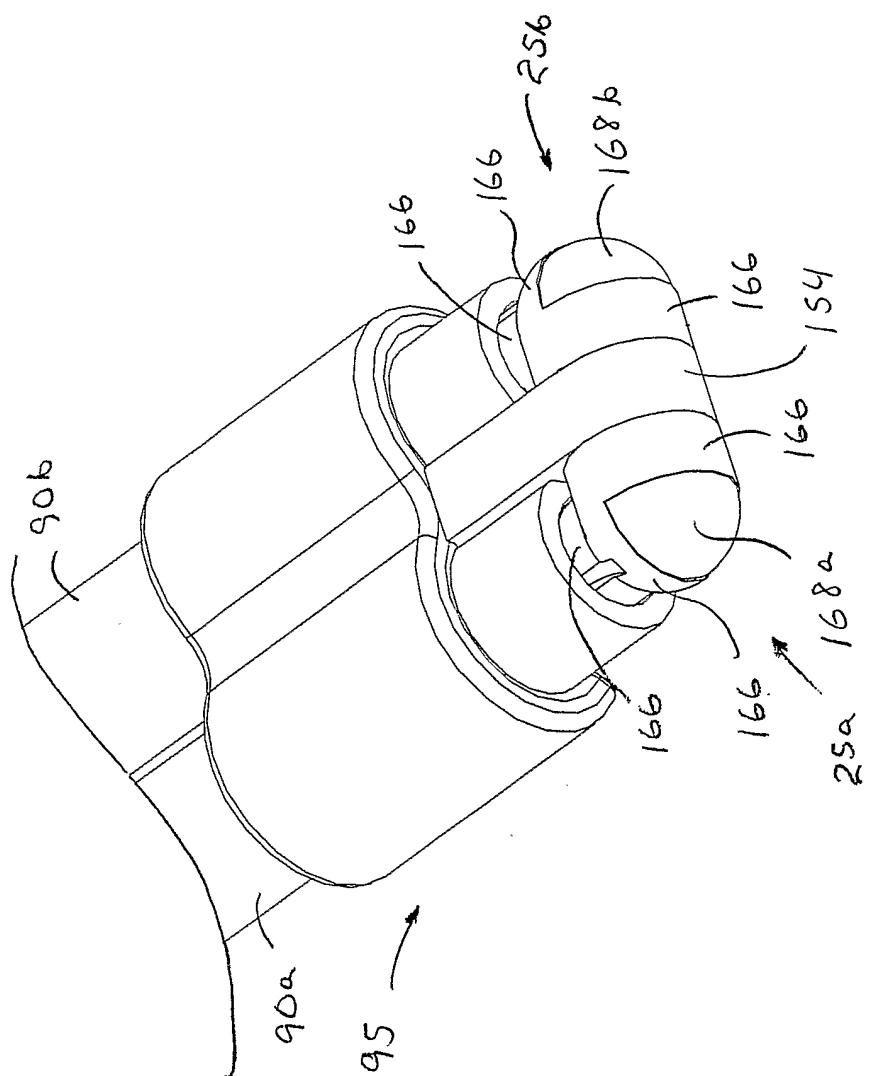


FIG. 61

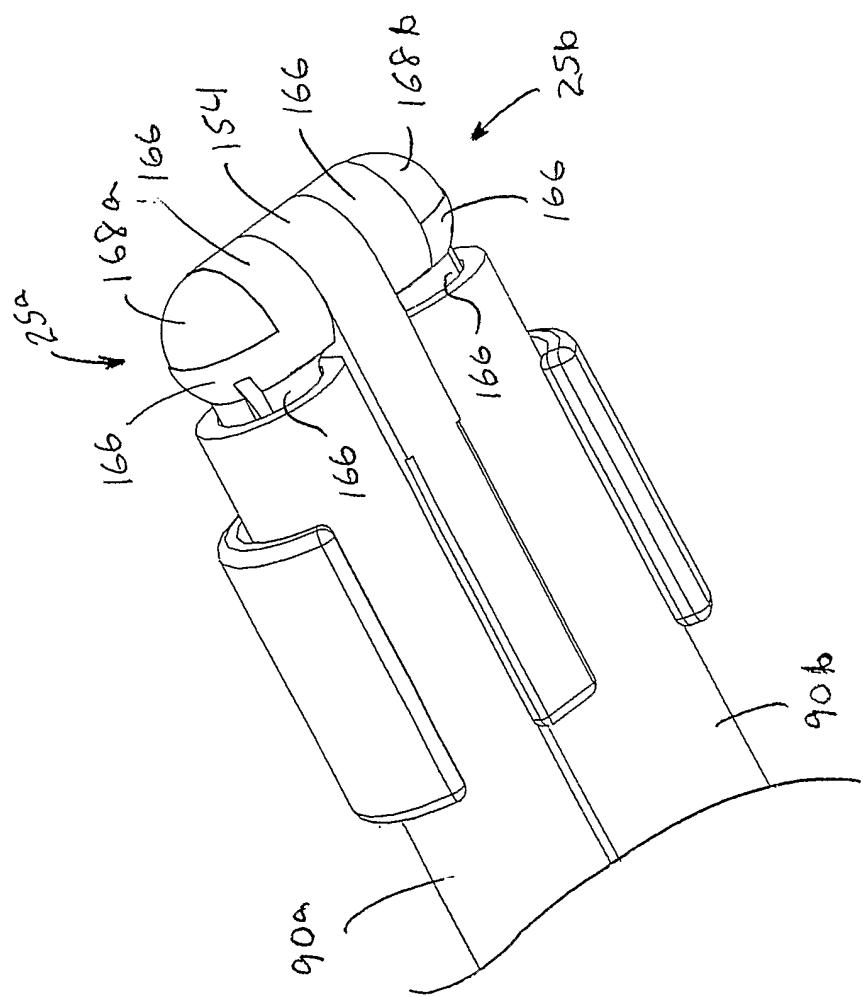


FIG. 62

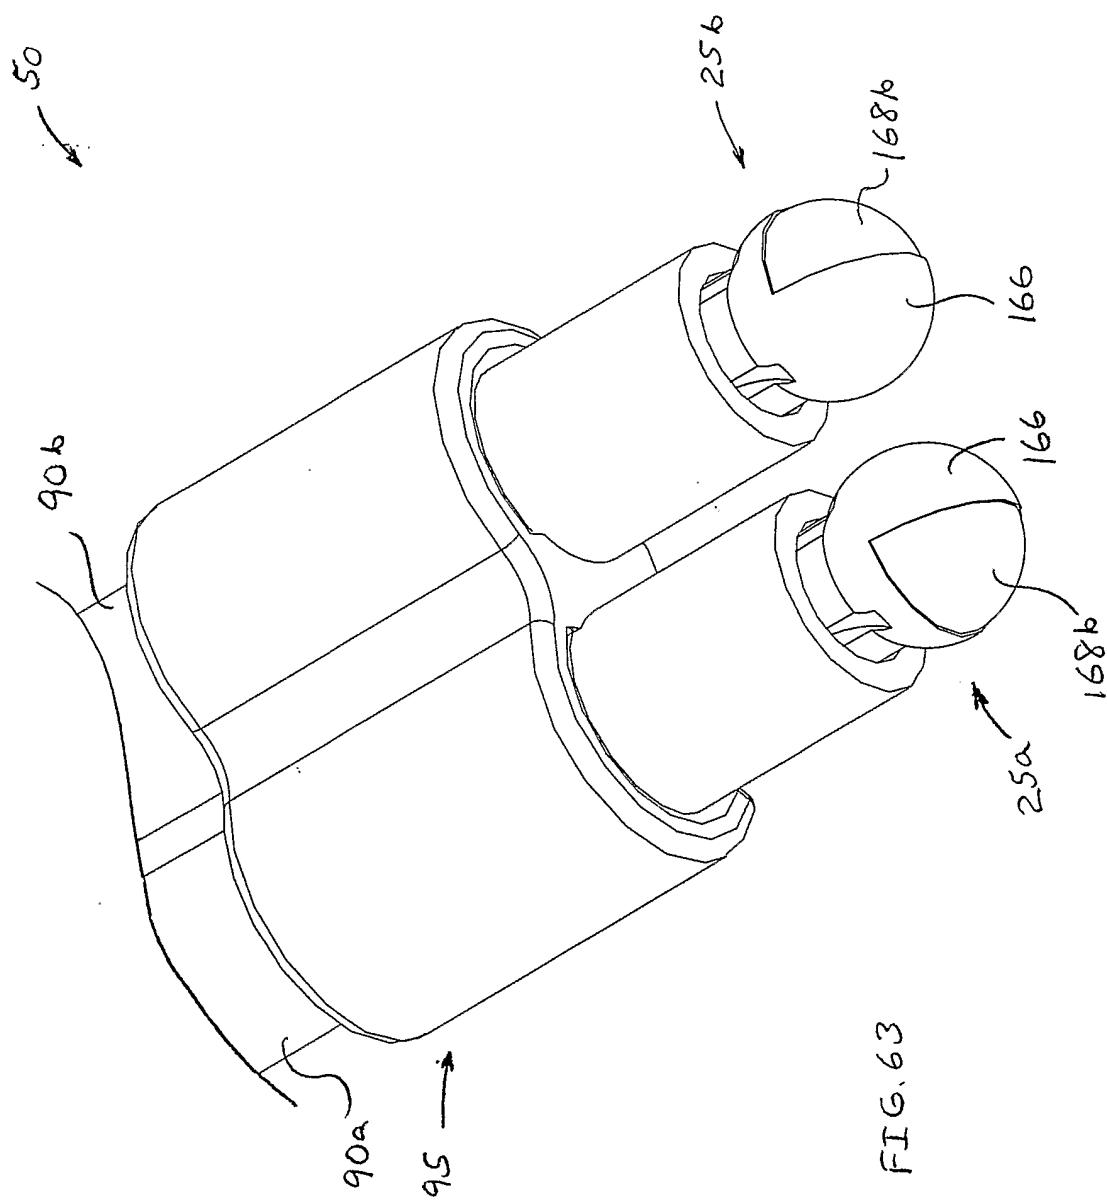


FIG. 63

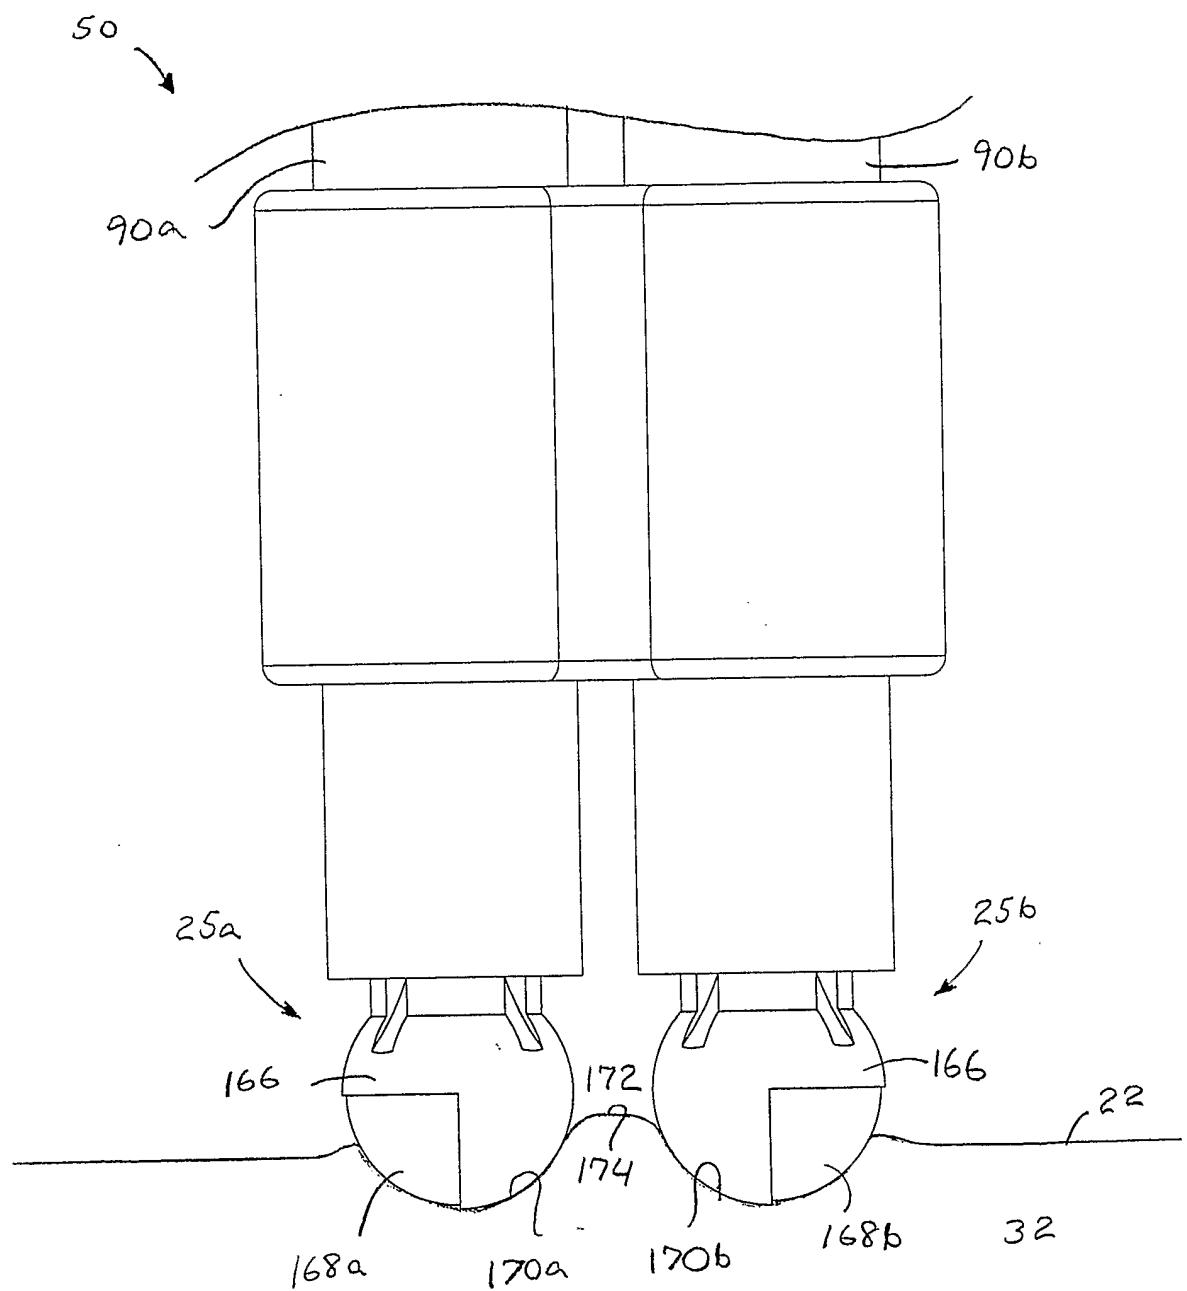
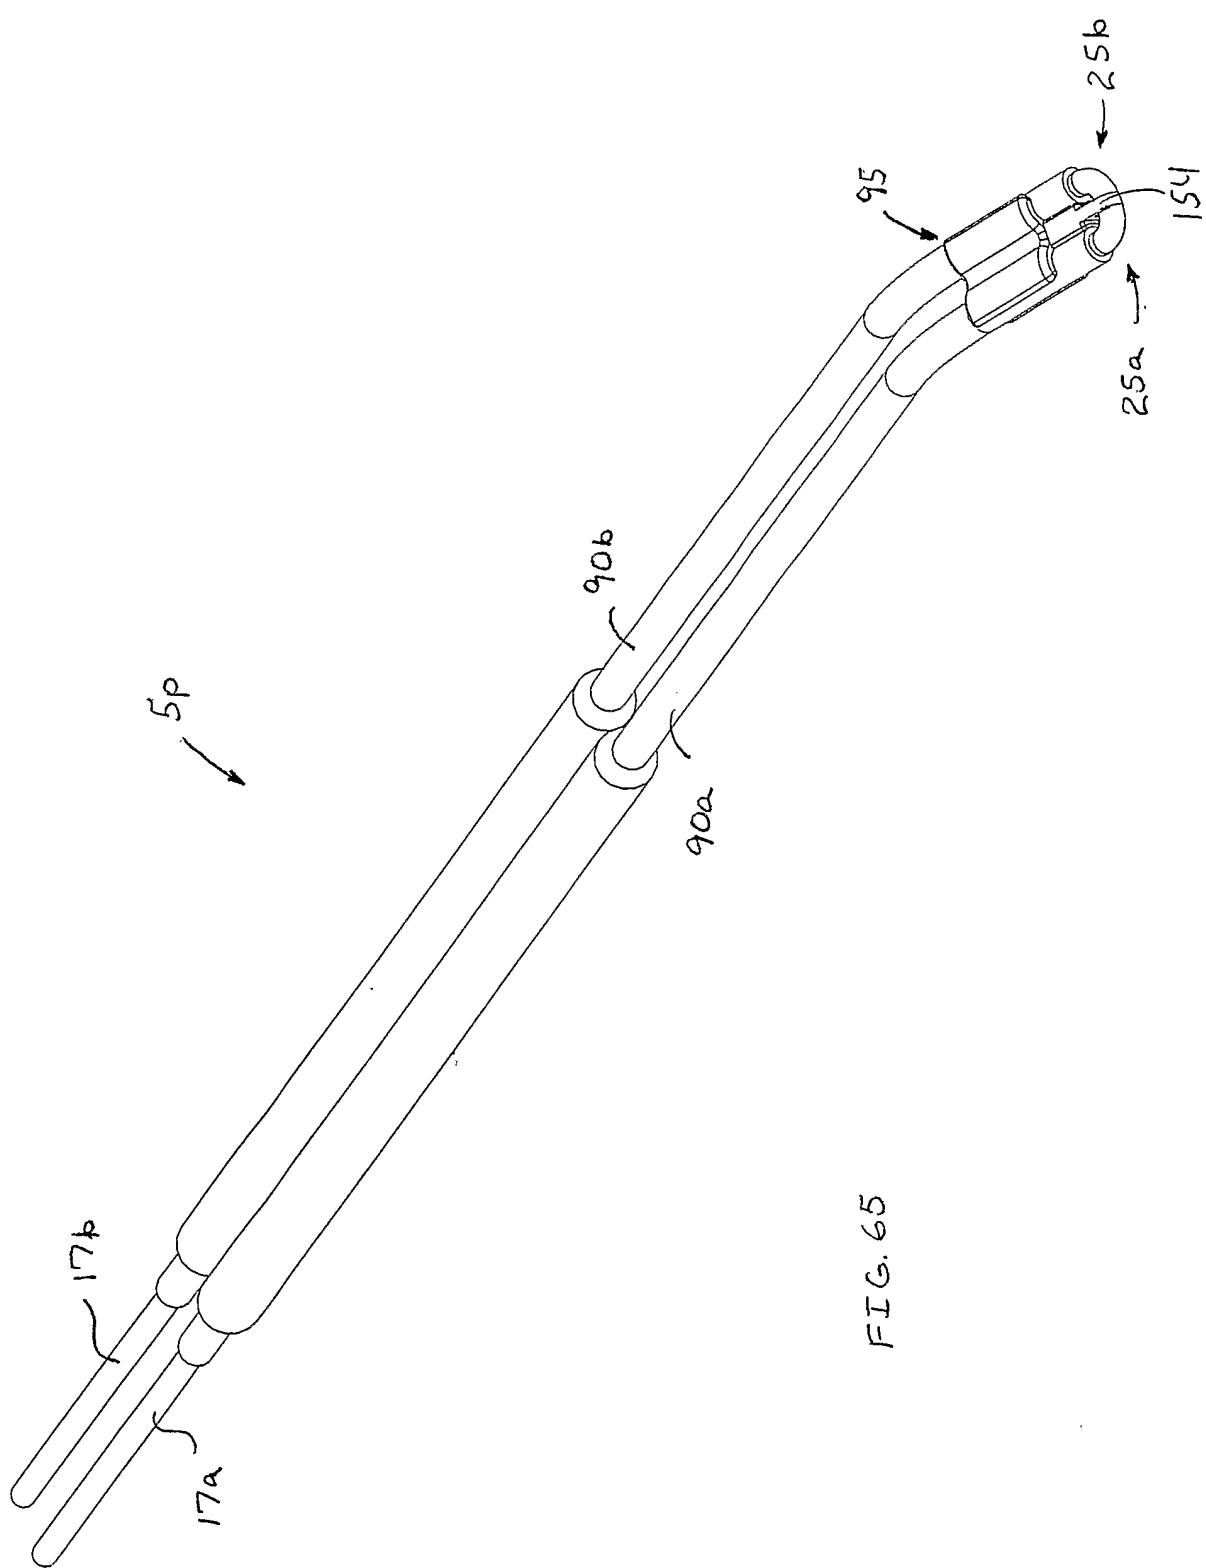


FIG. 64



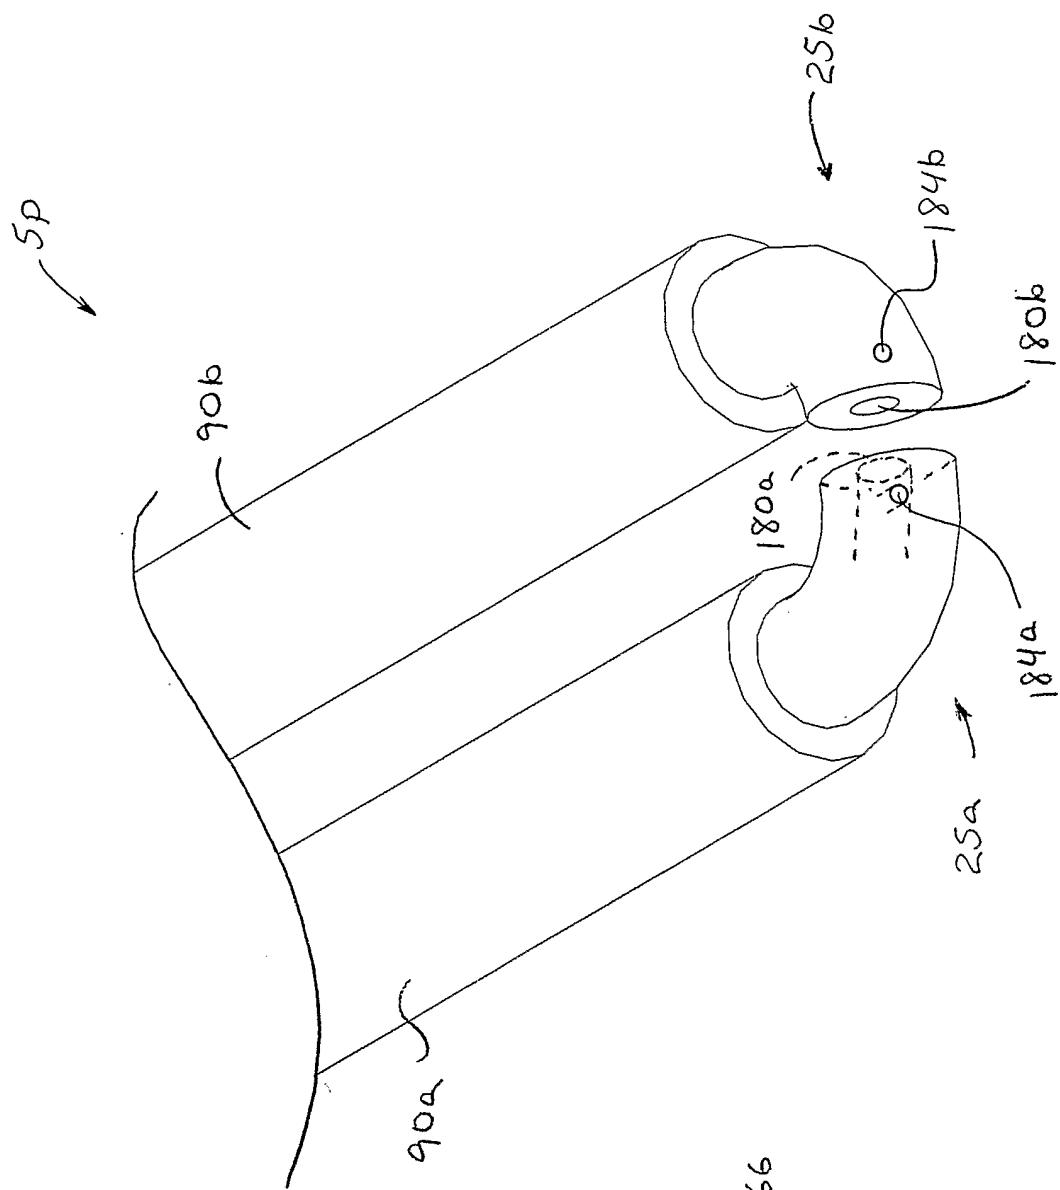
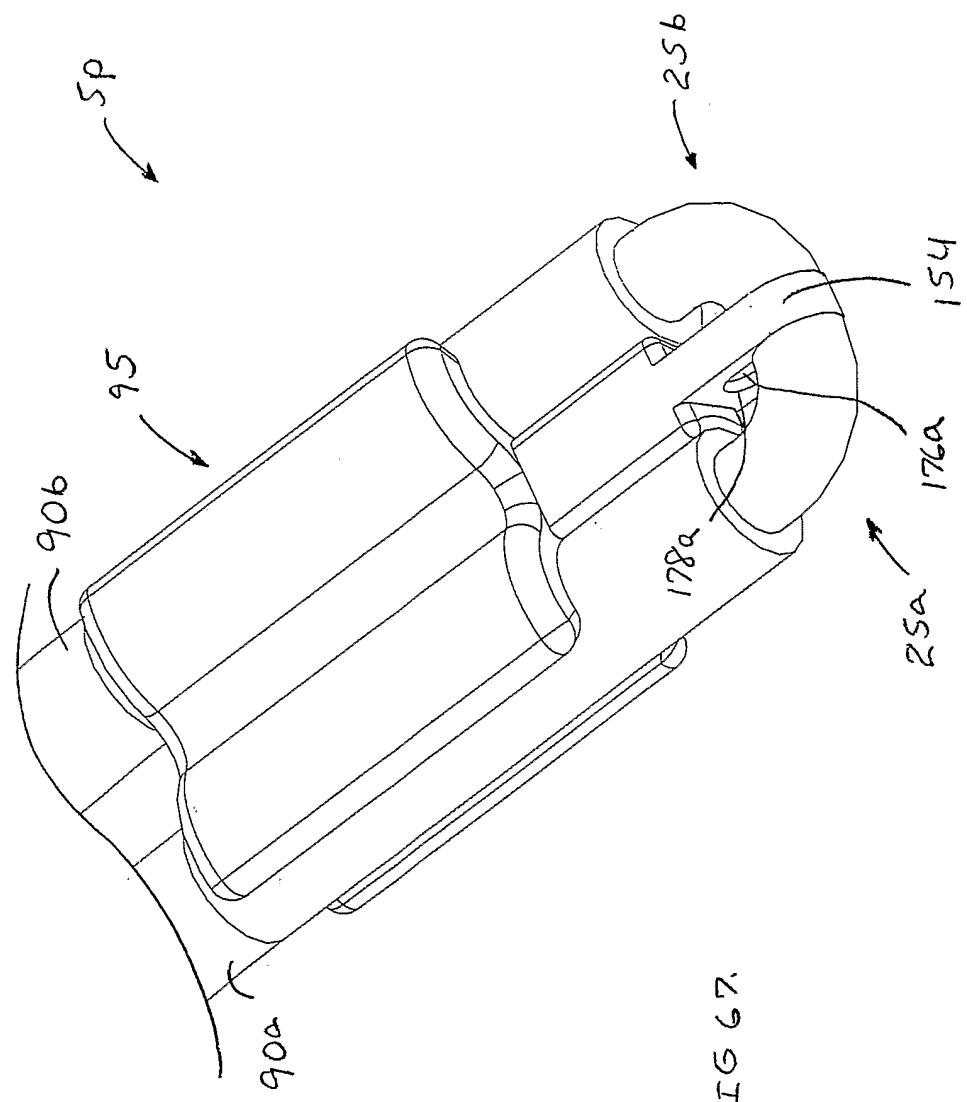


FIG. 66



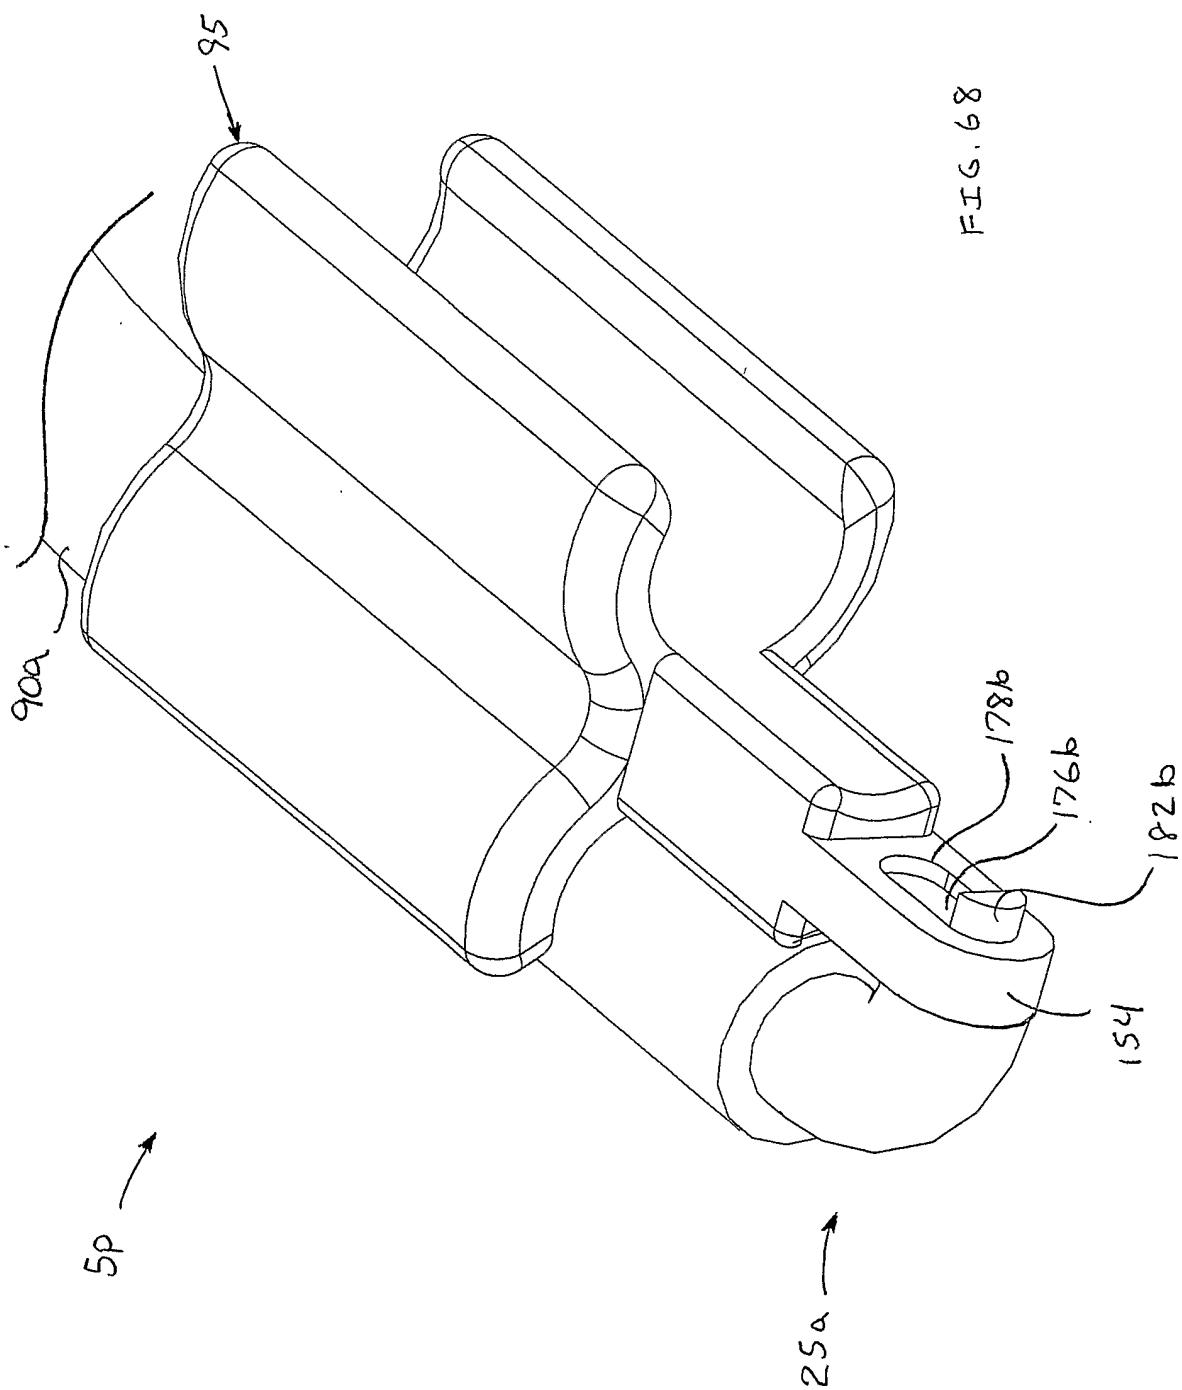
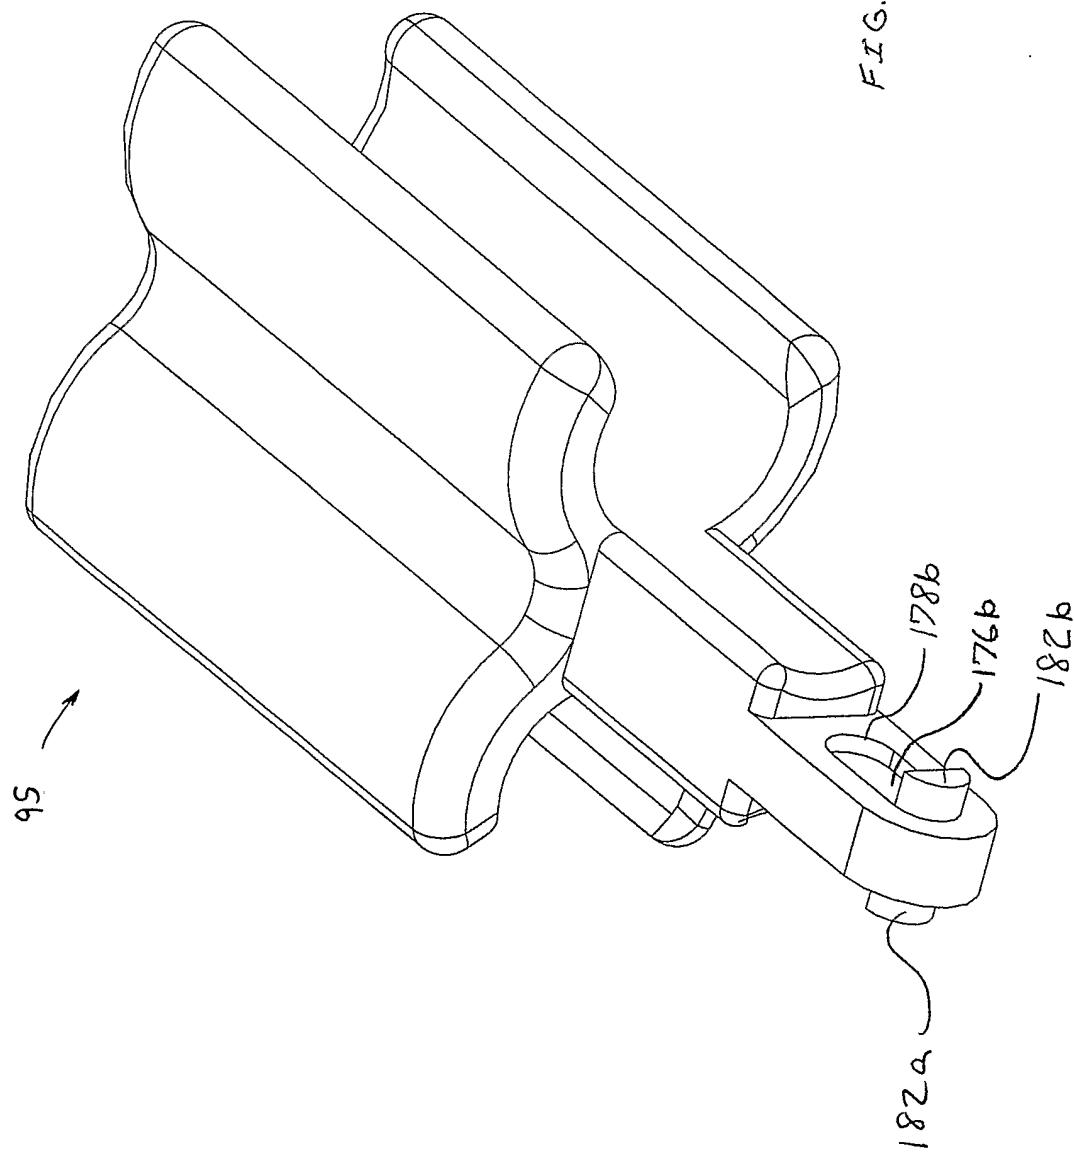


FIG. 69



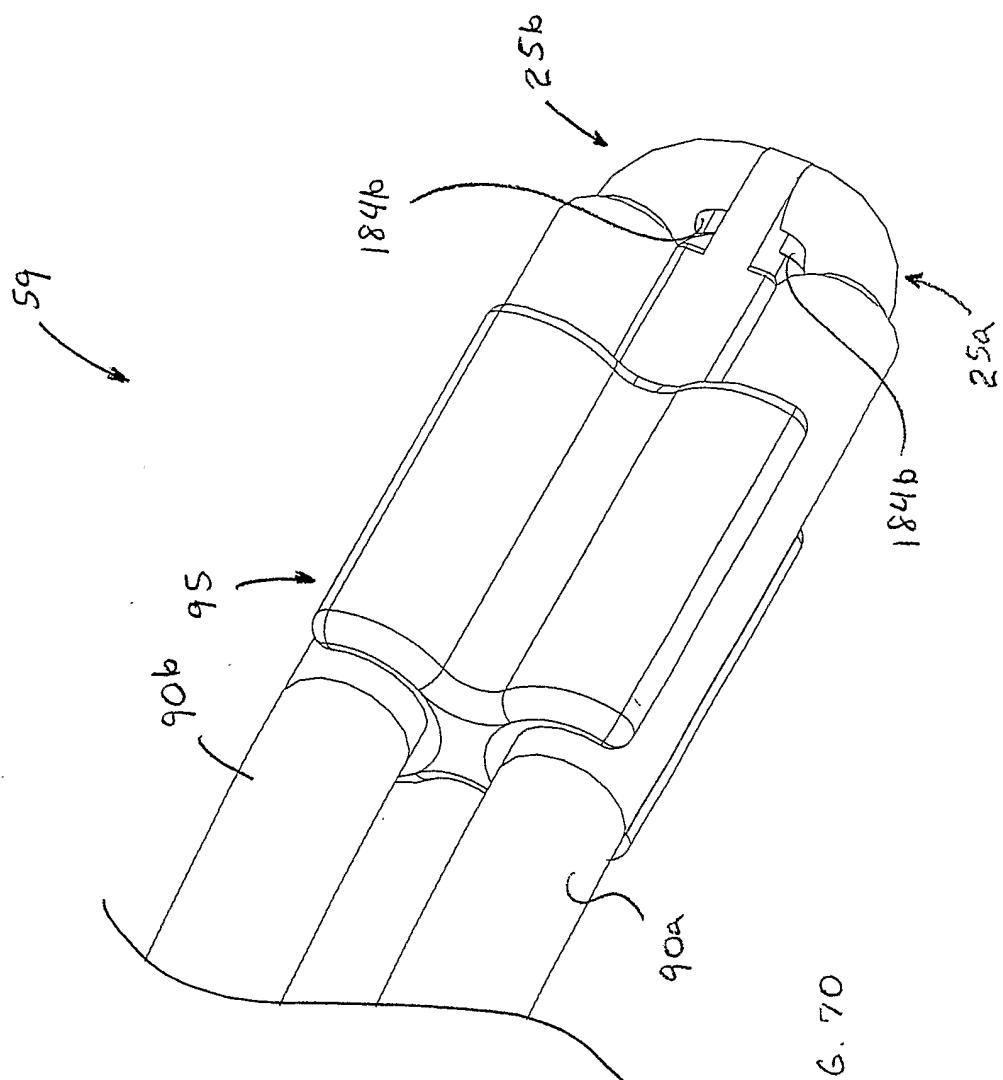
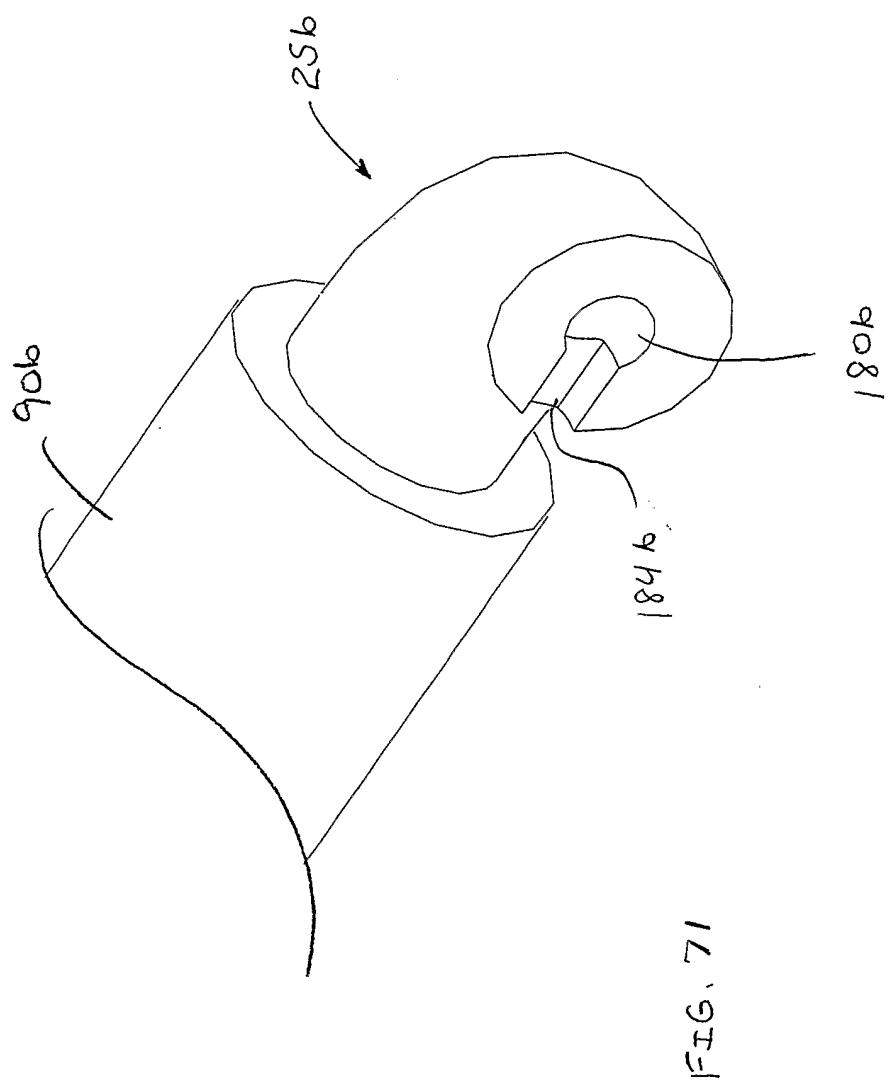
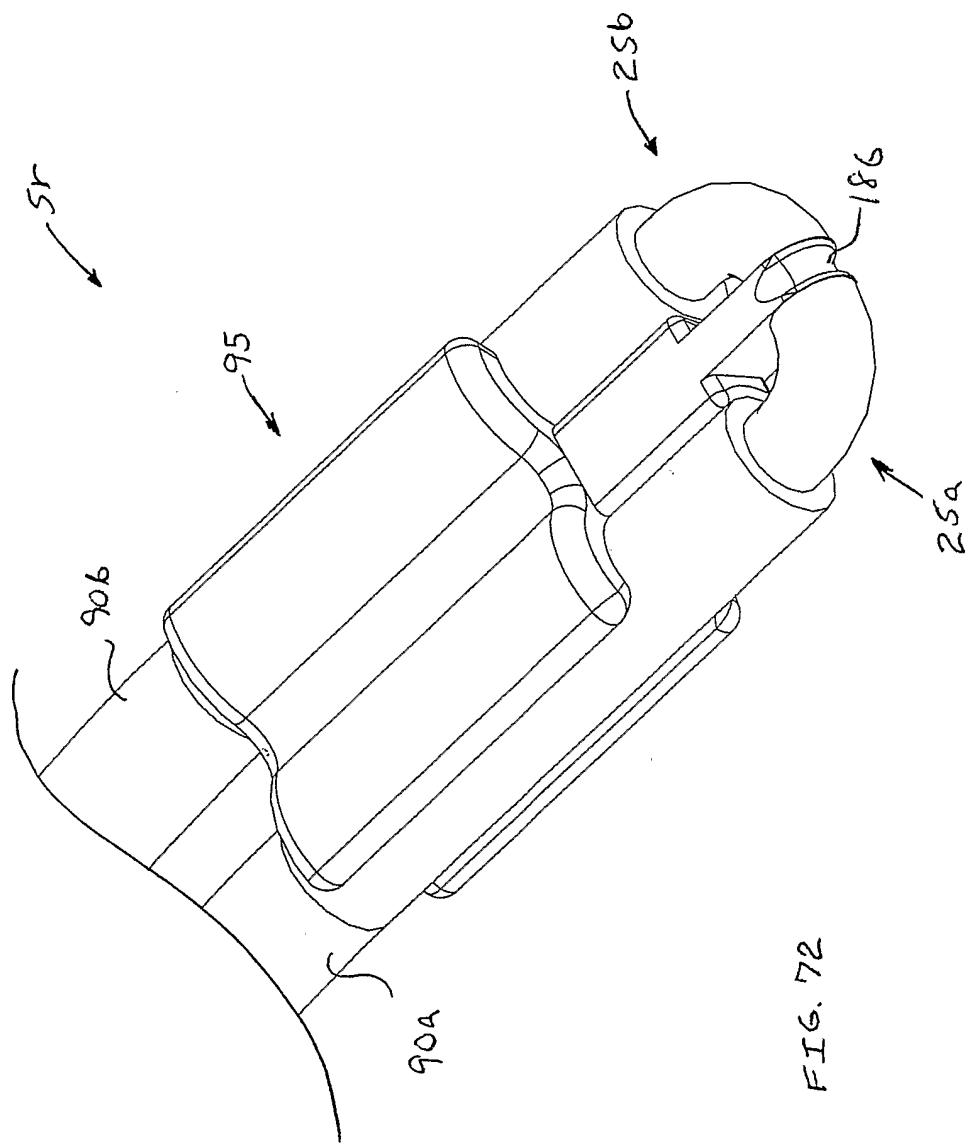
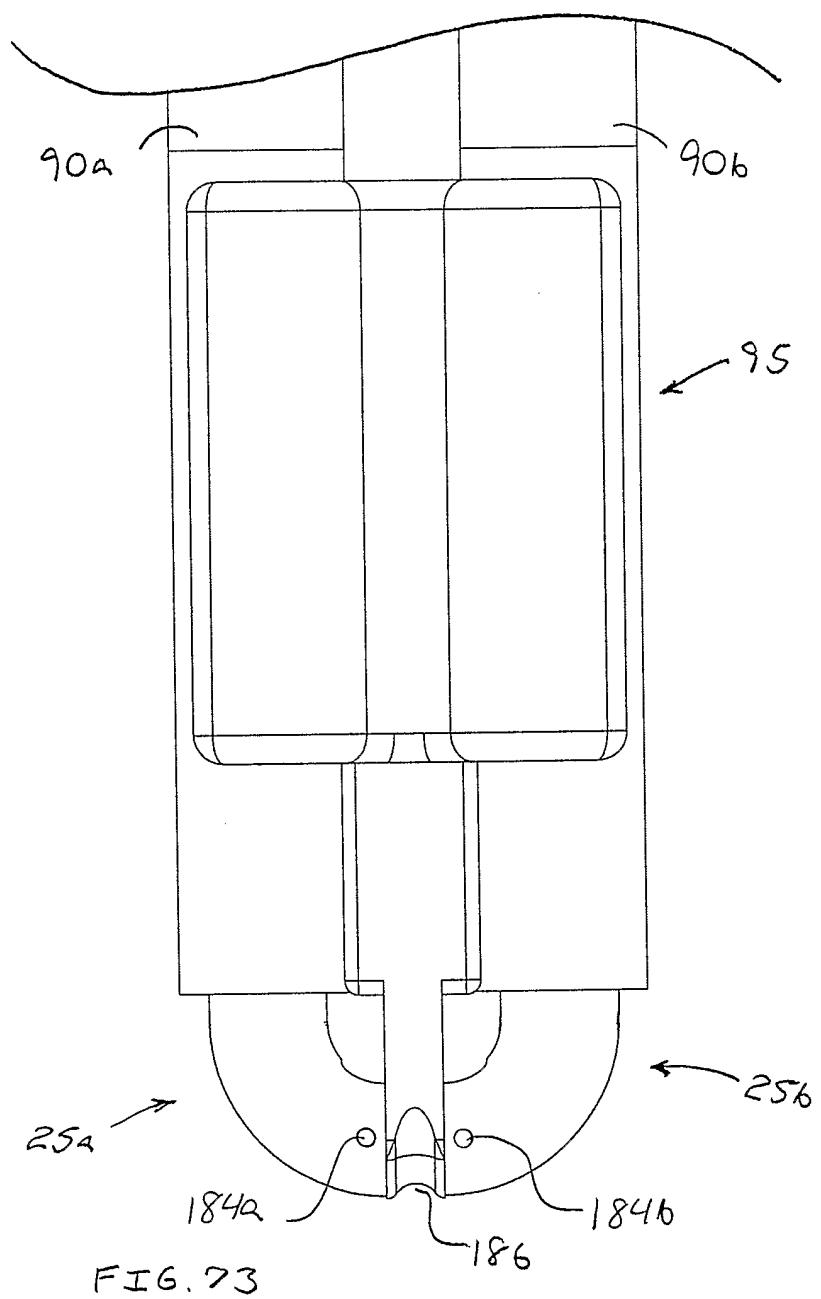
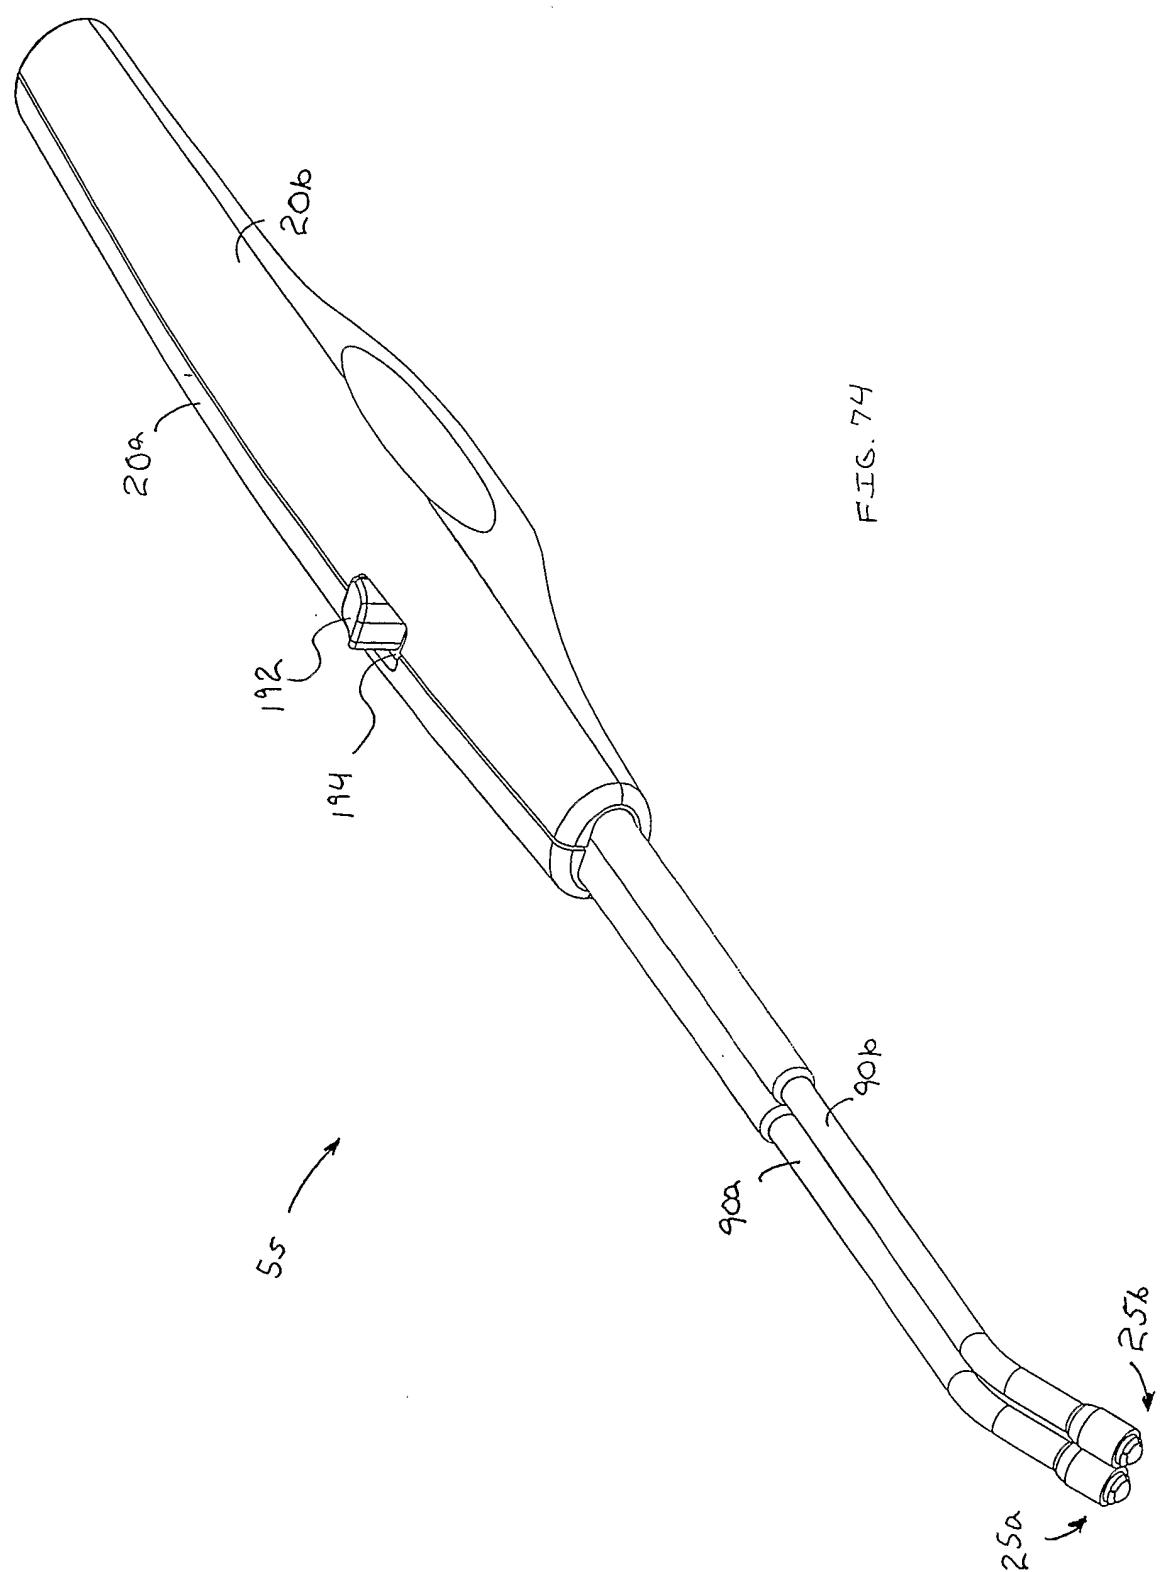



FIG. 70











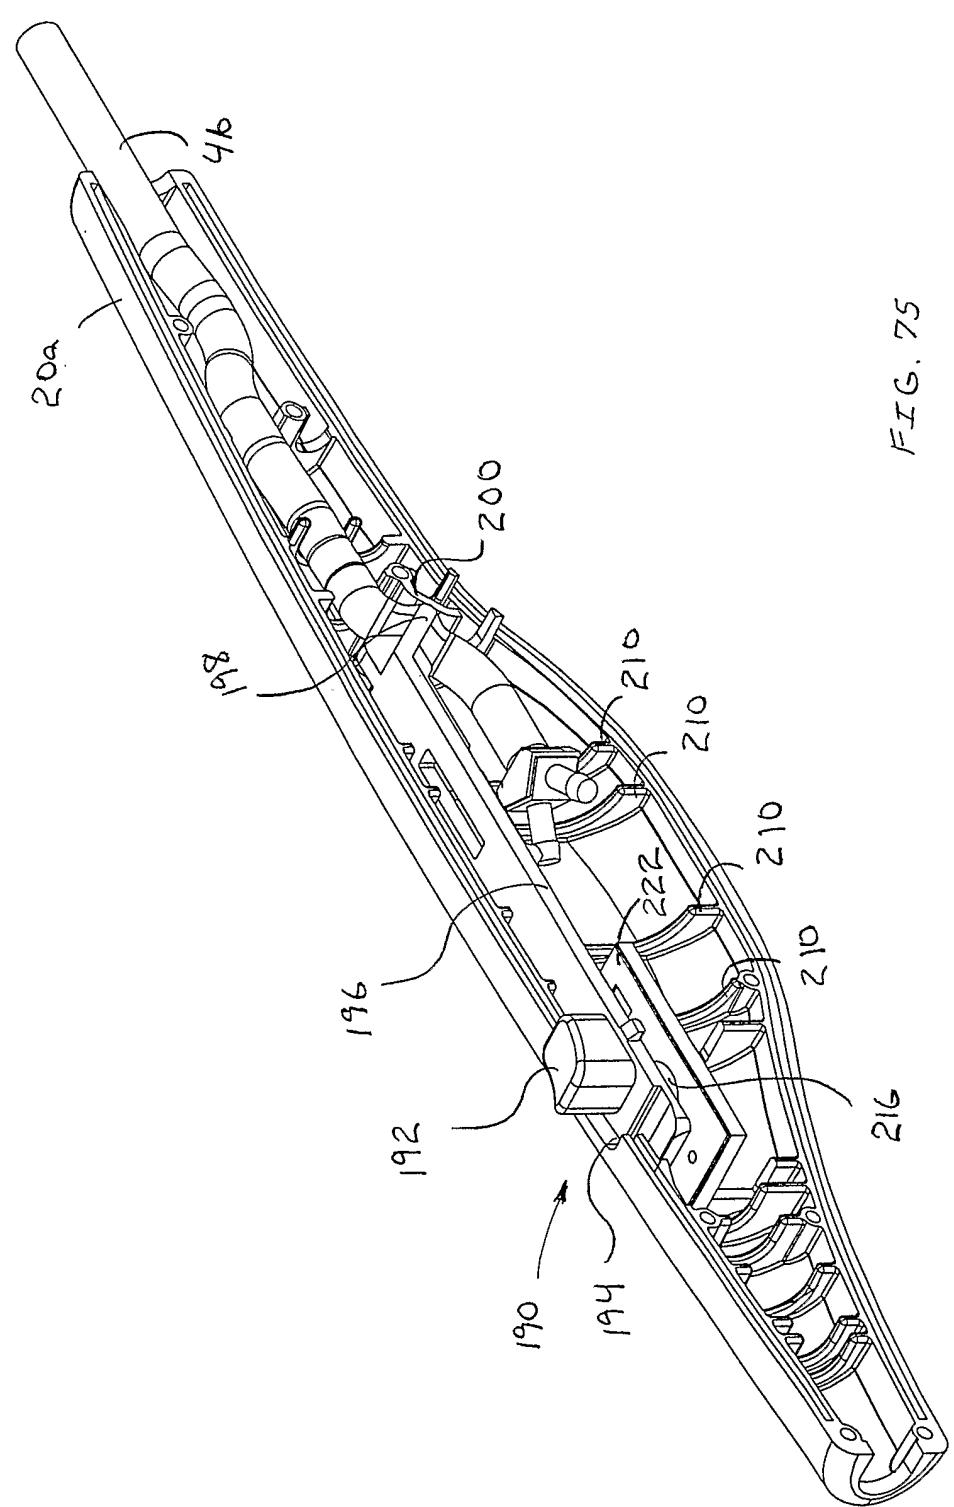

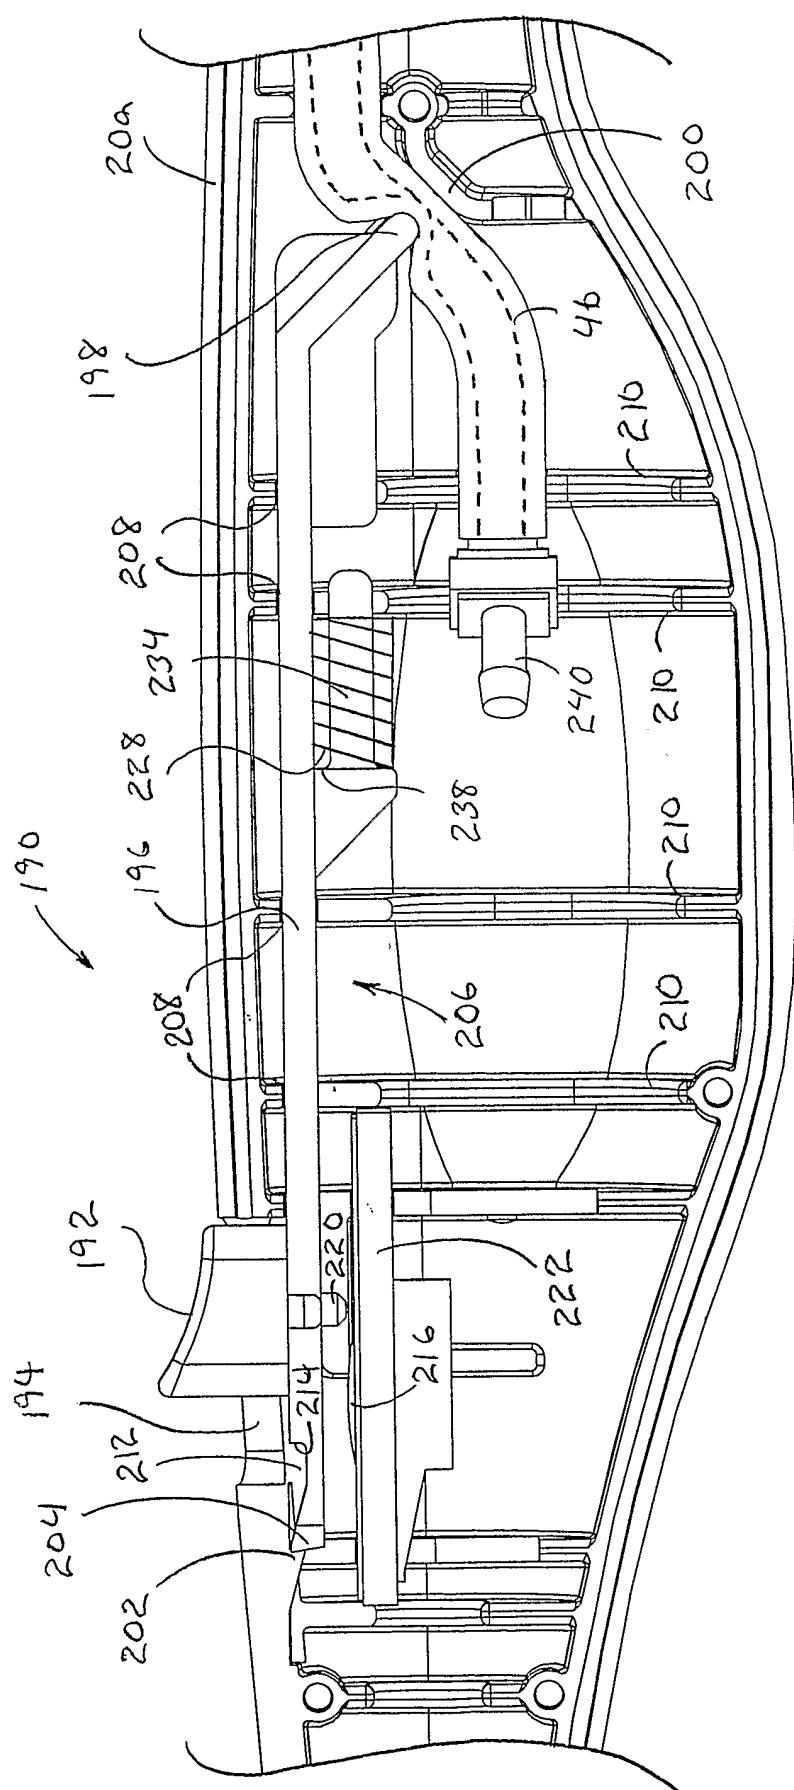

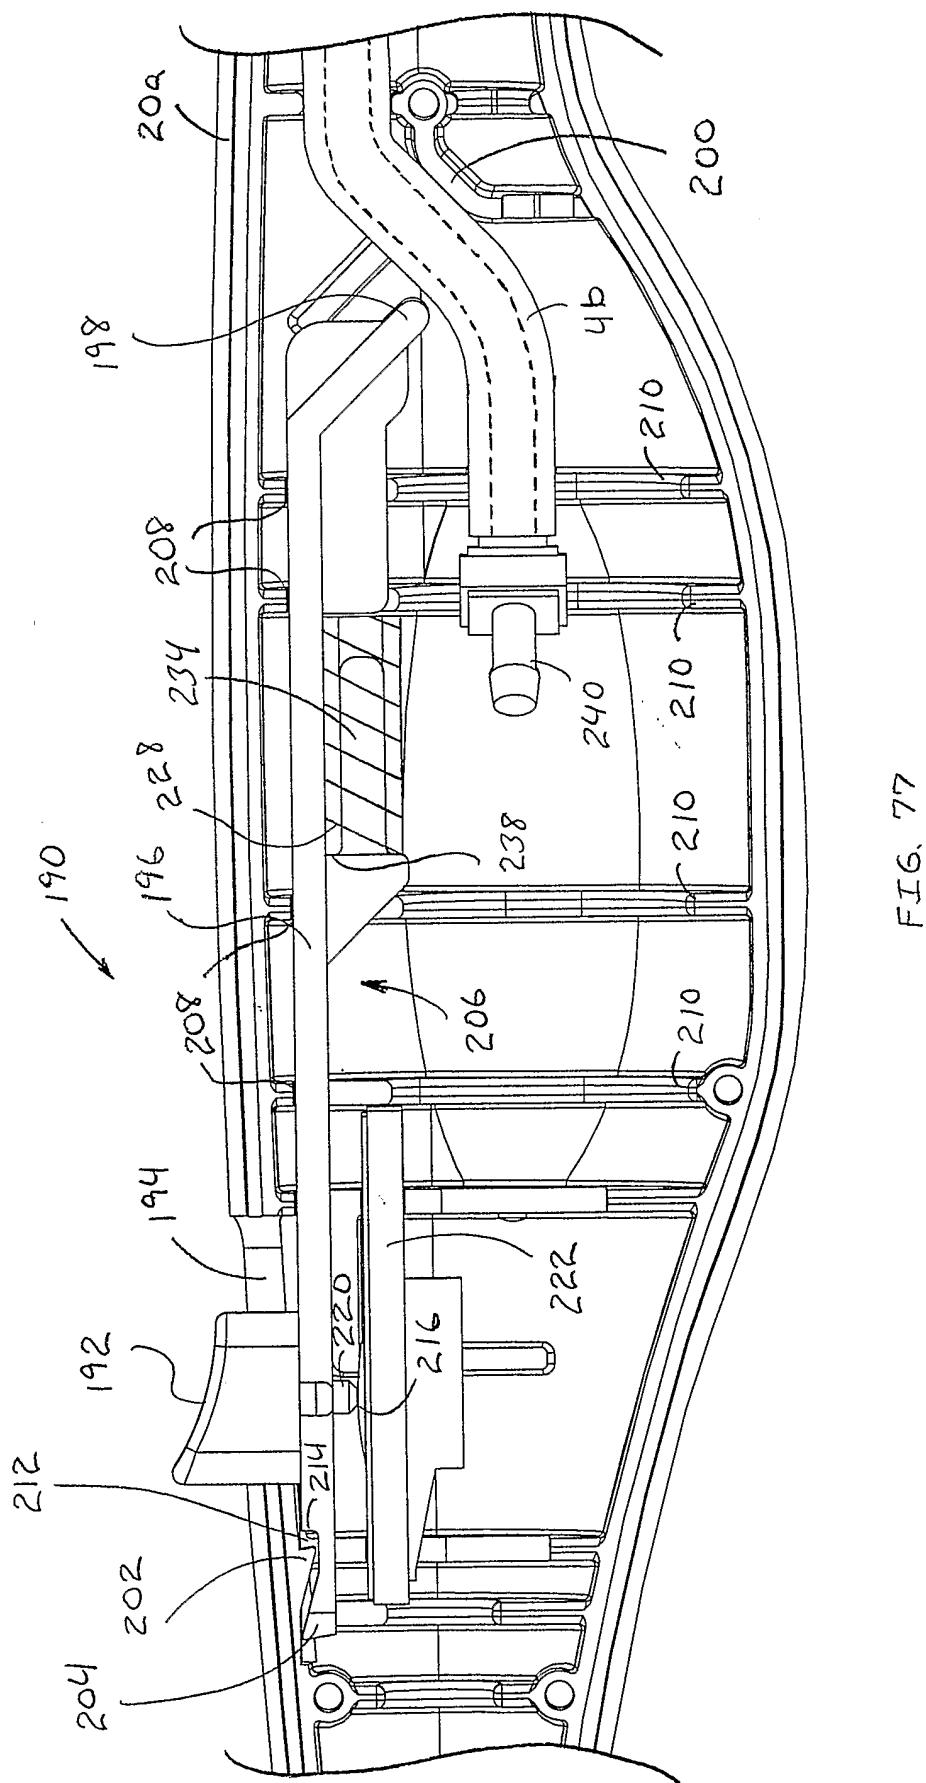

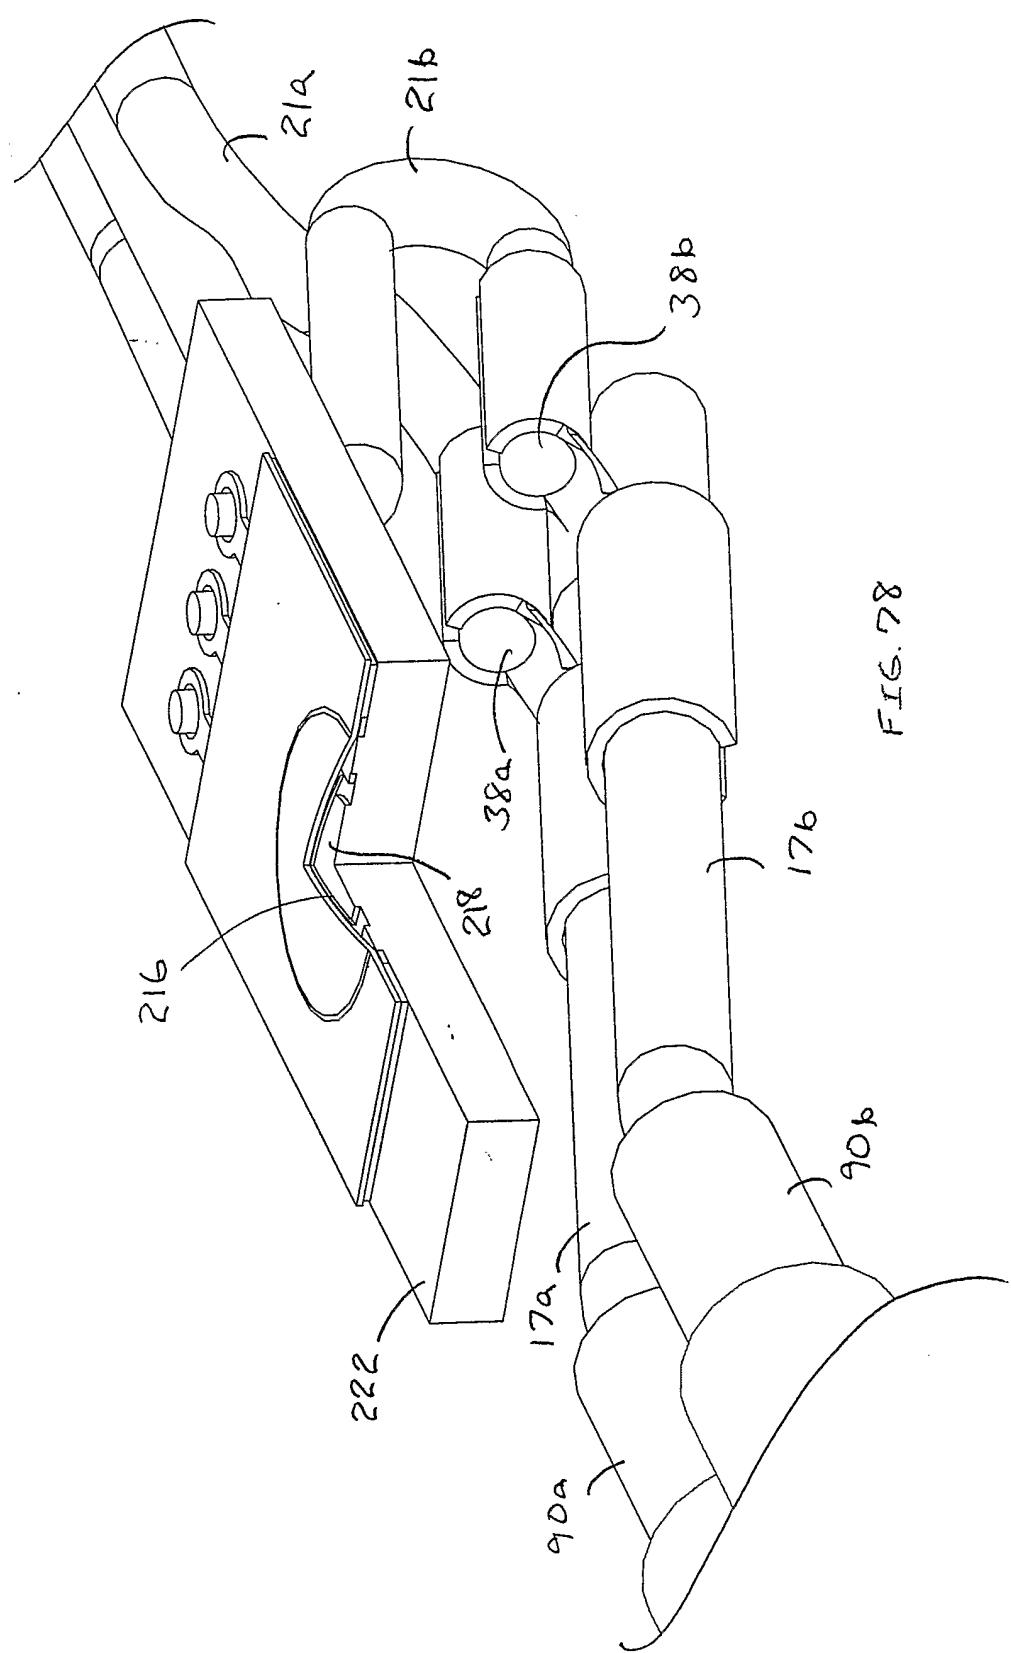
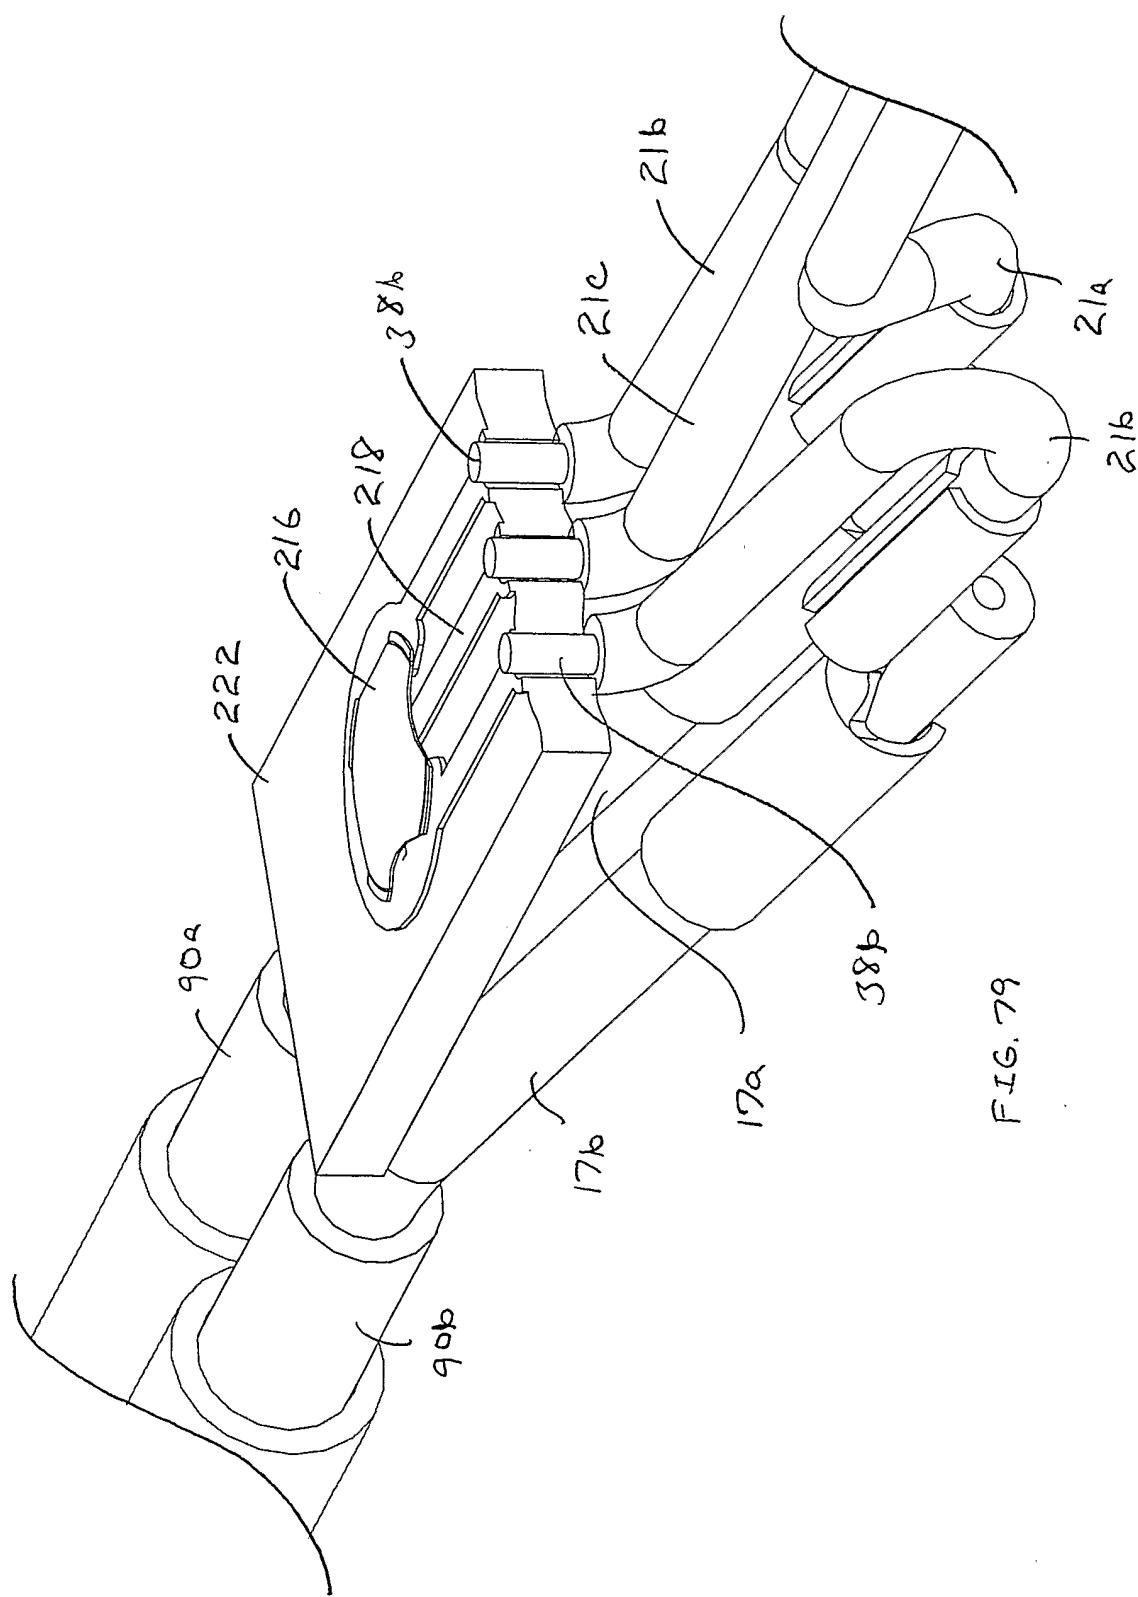
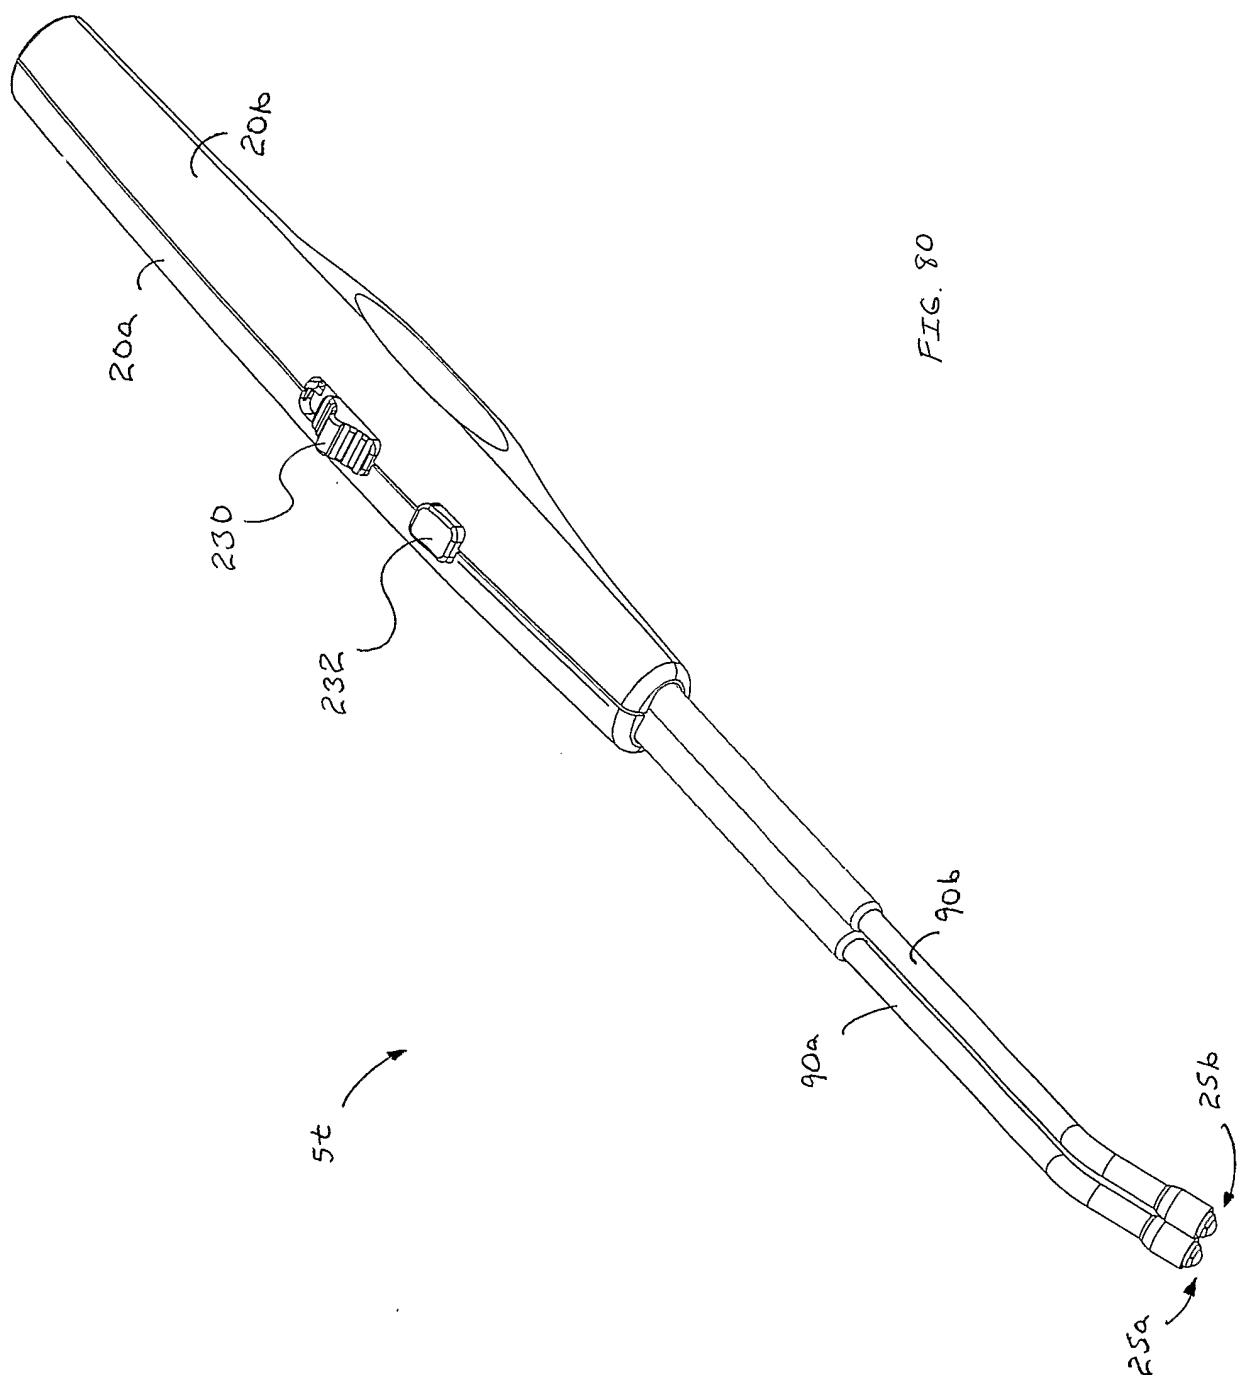


FIG. 78





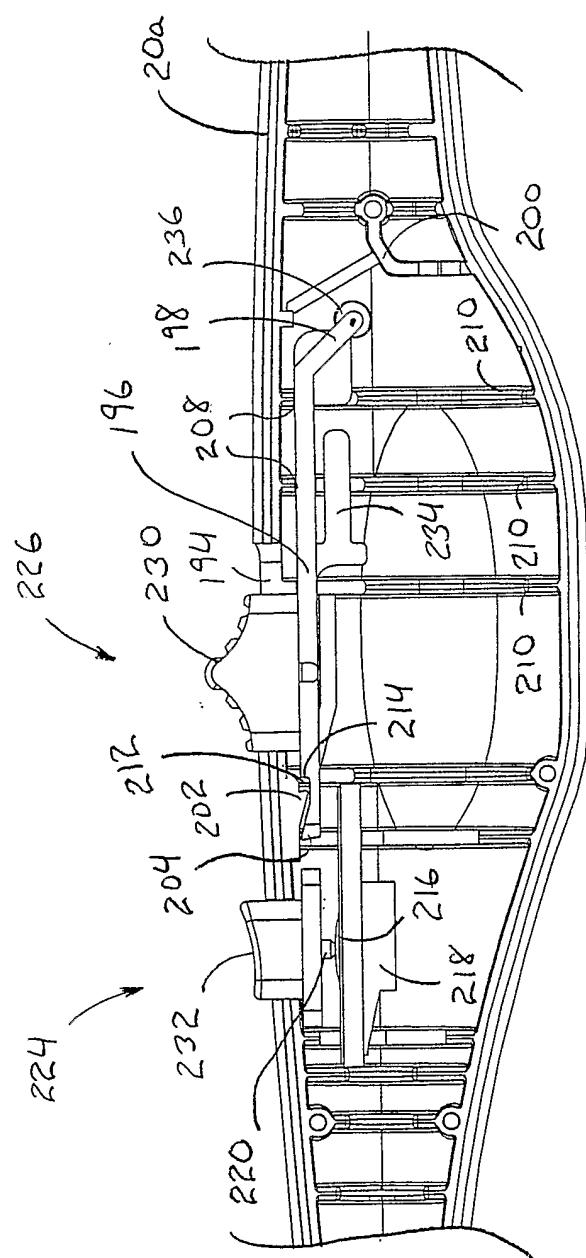
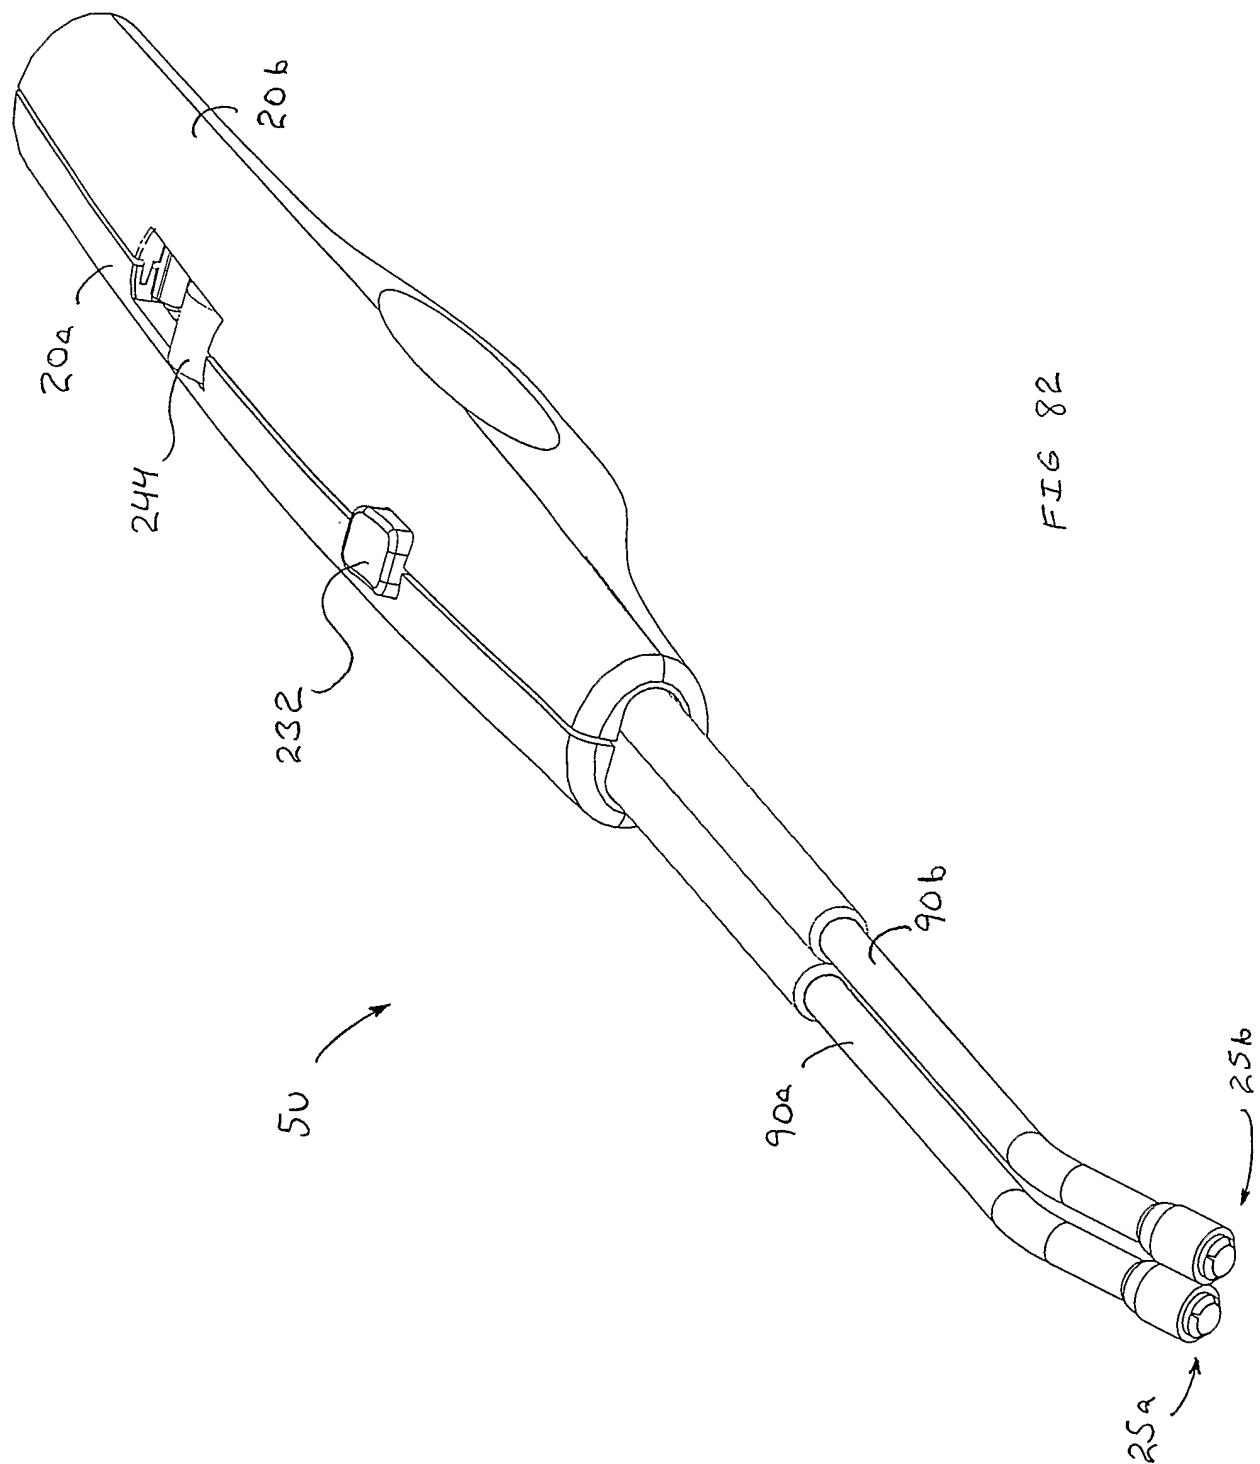


FIG. 81



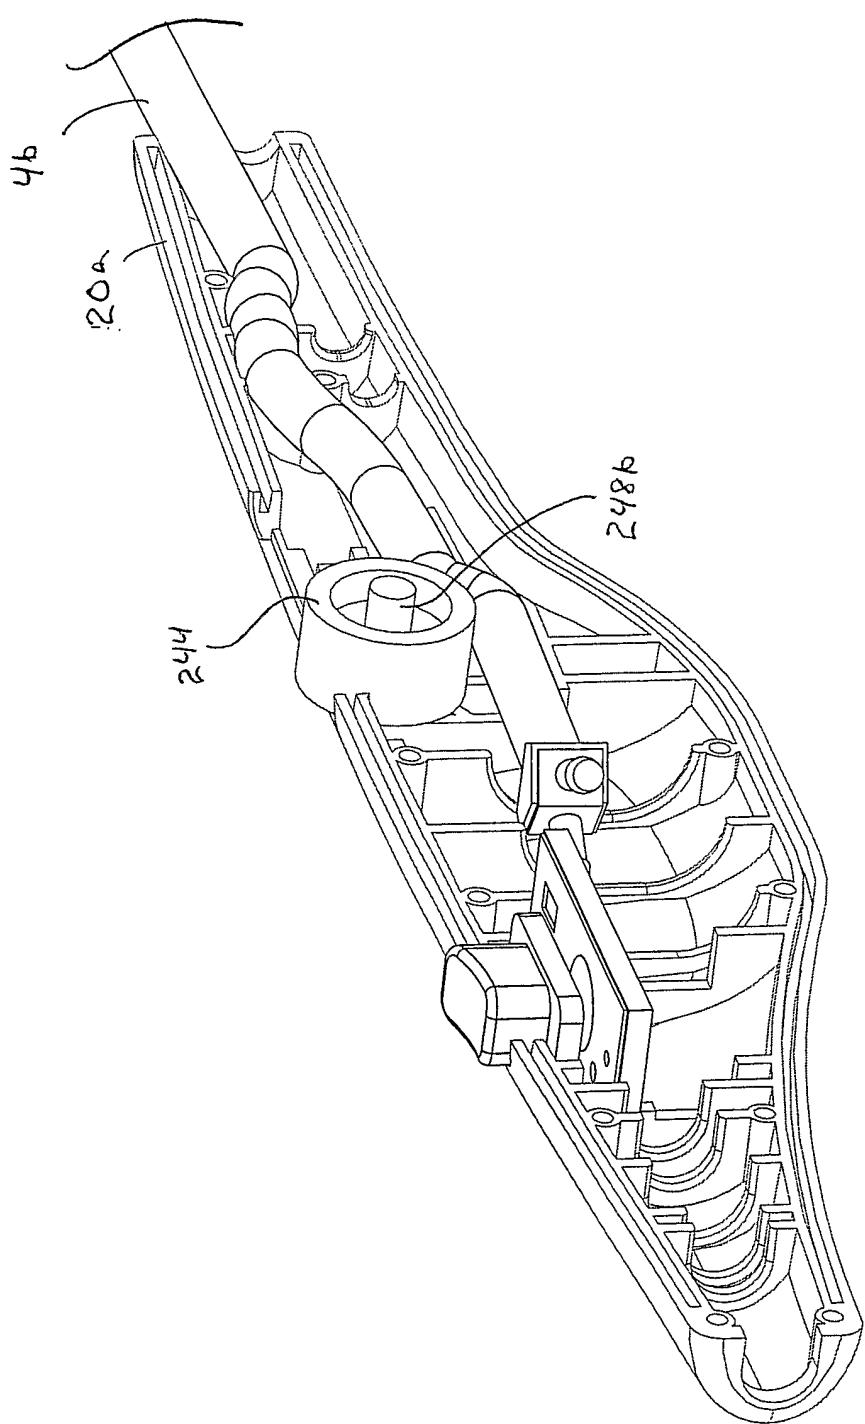


FIG. 83

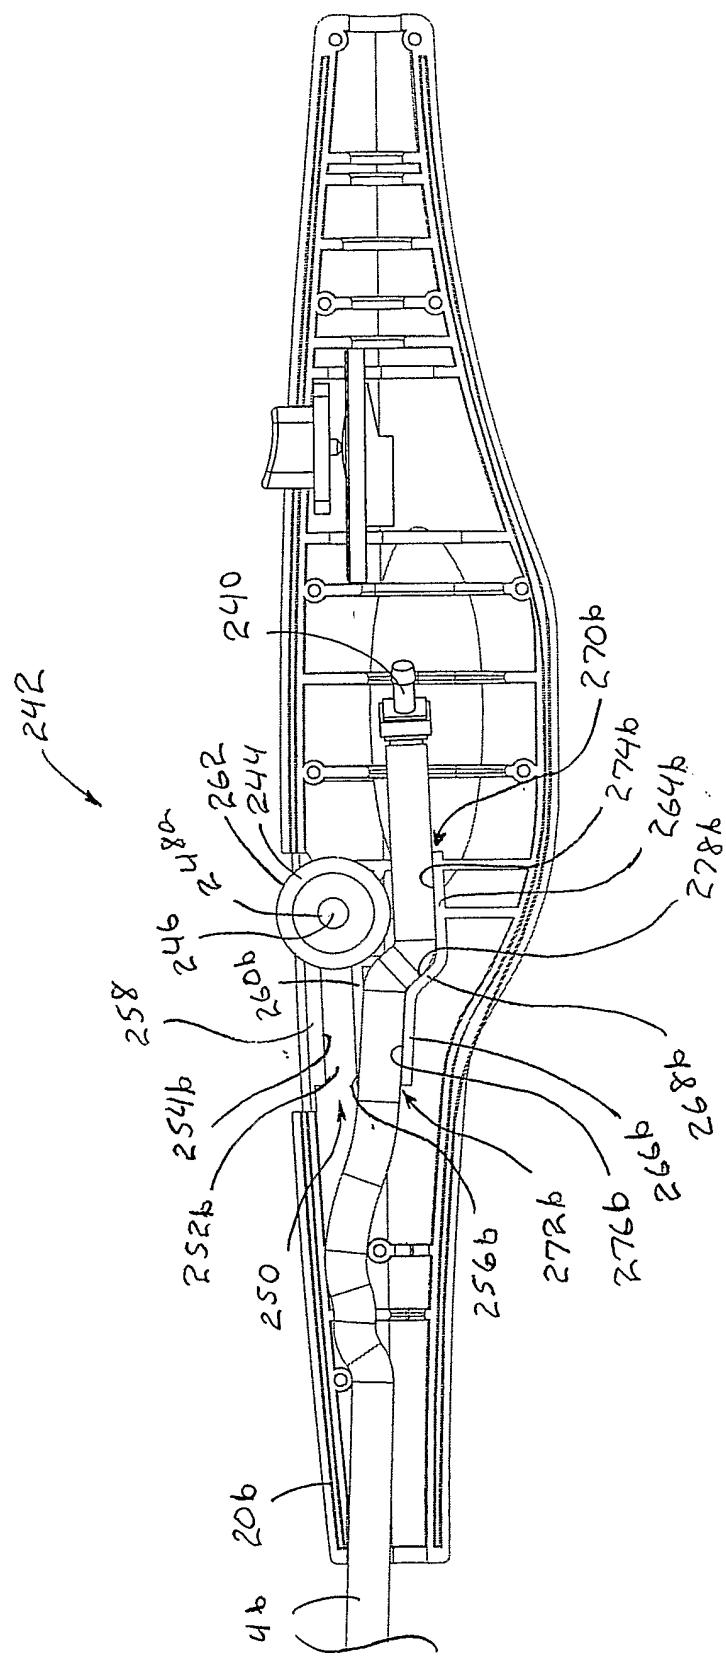
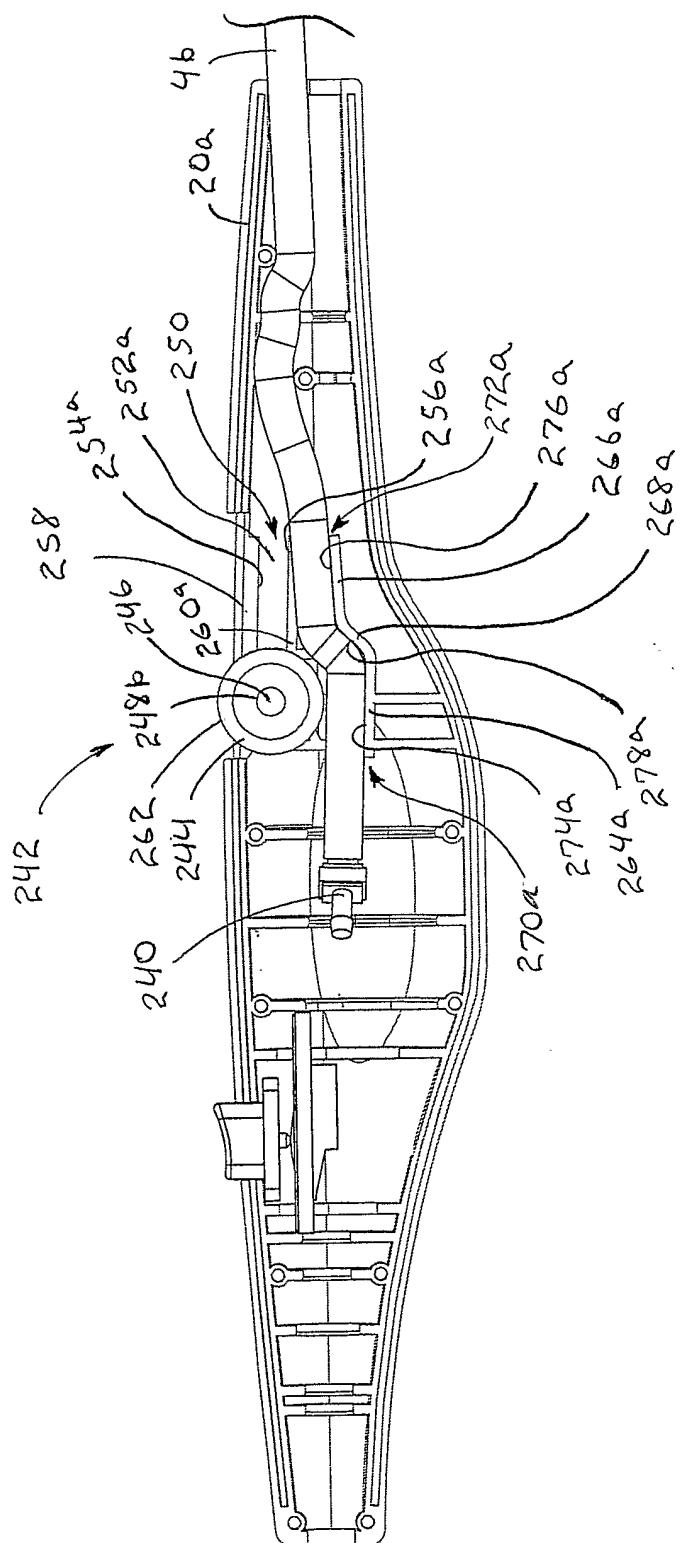
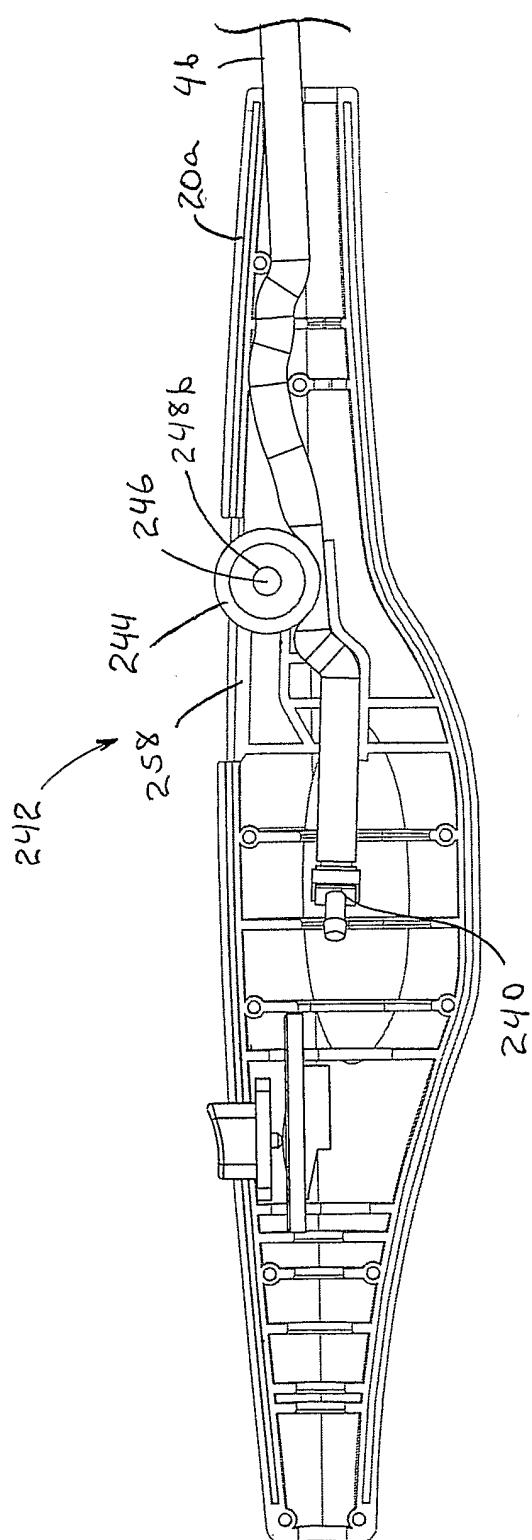


FIG. 84





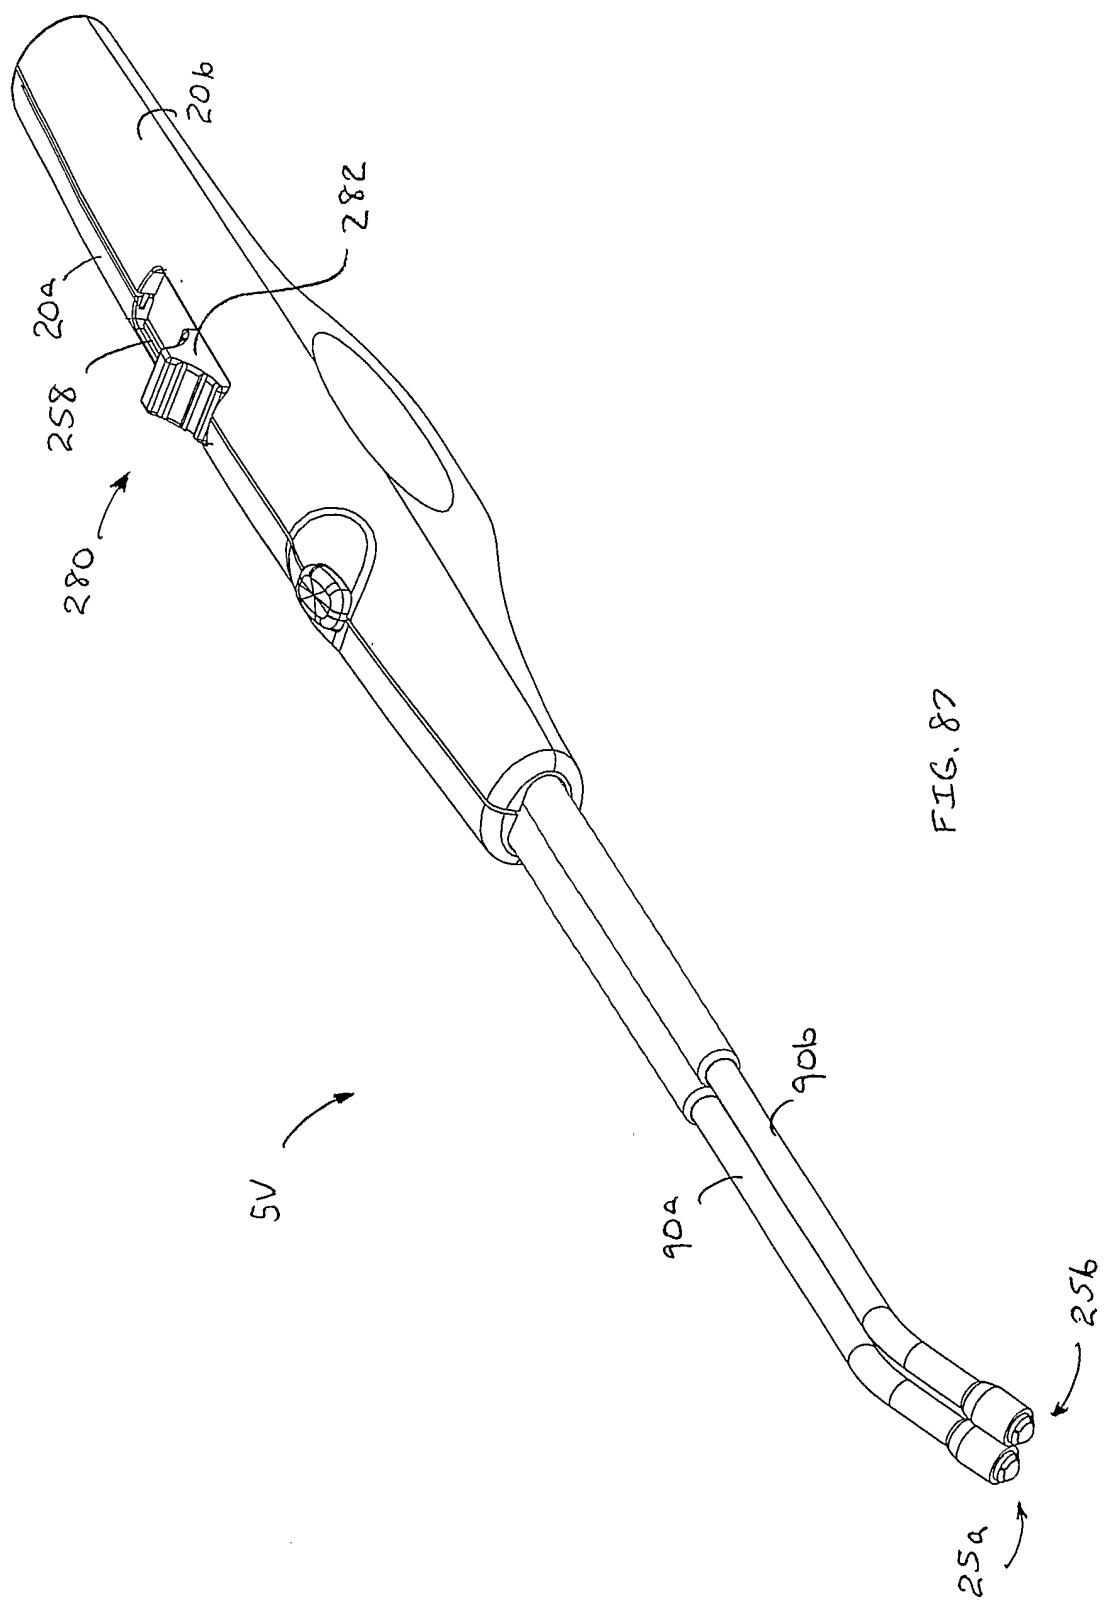
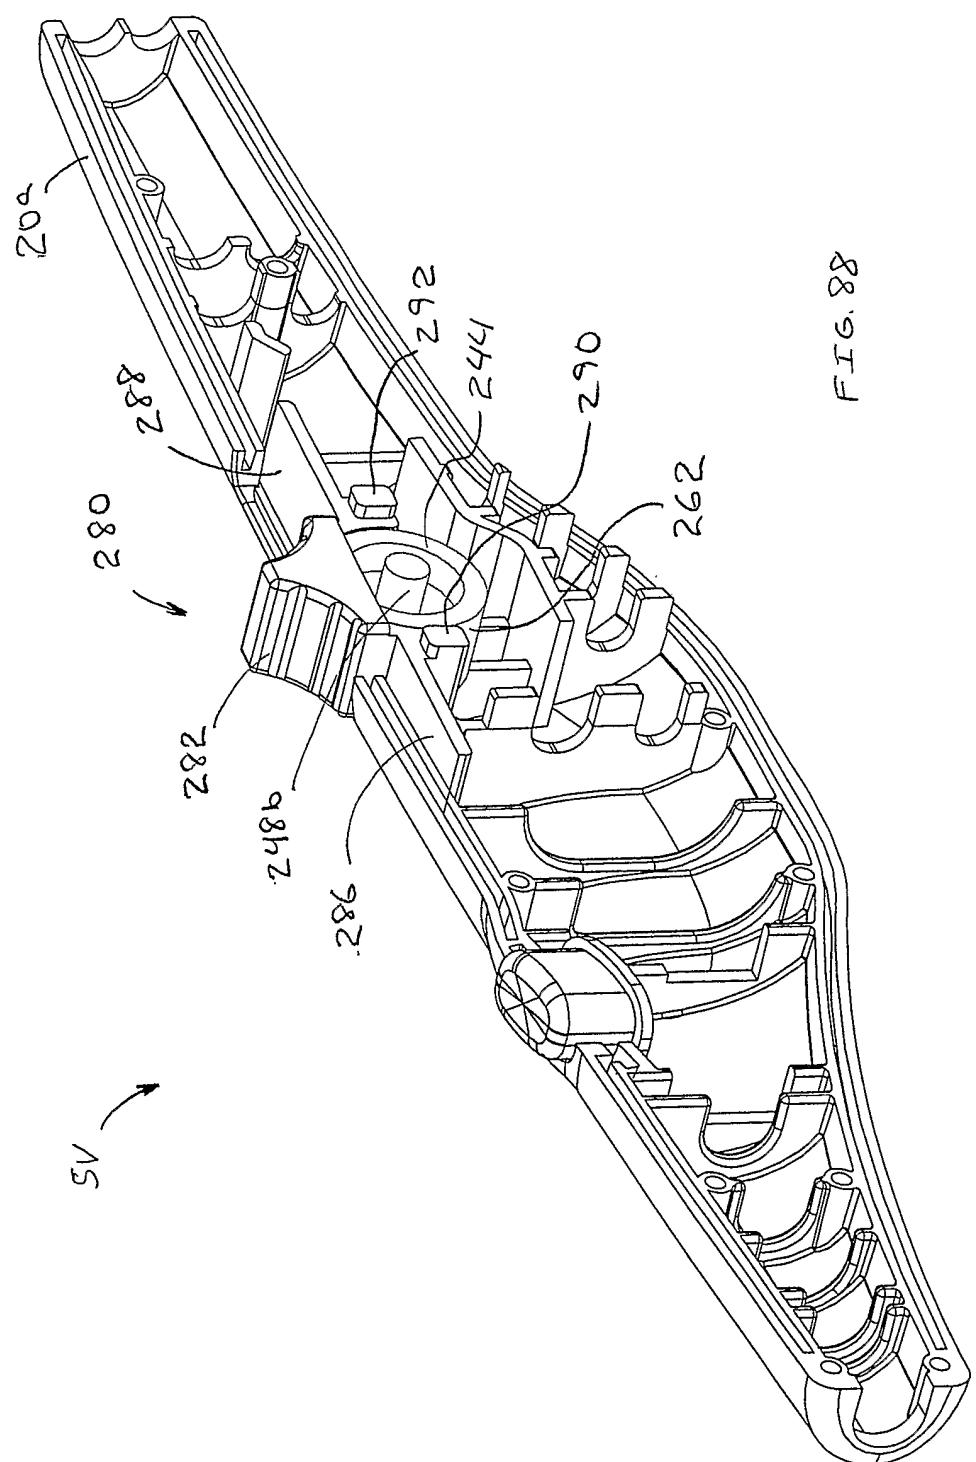


FIG. 87



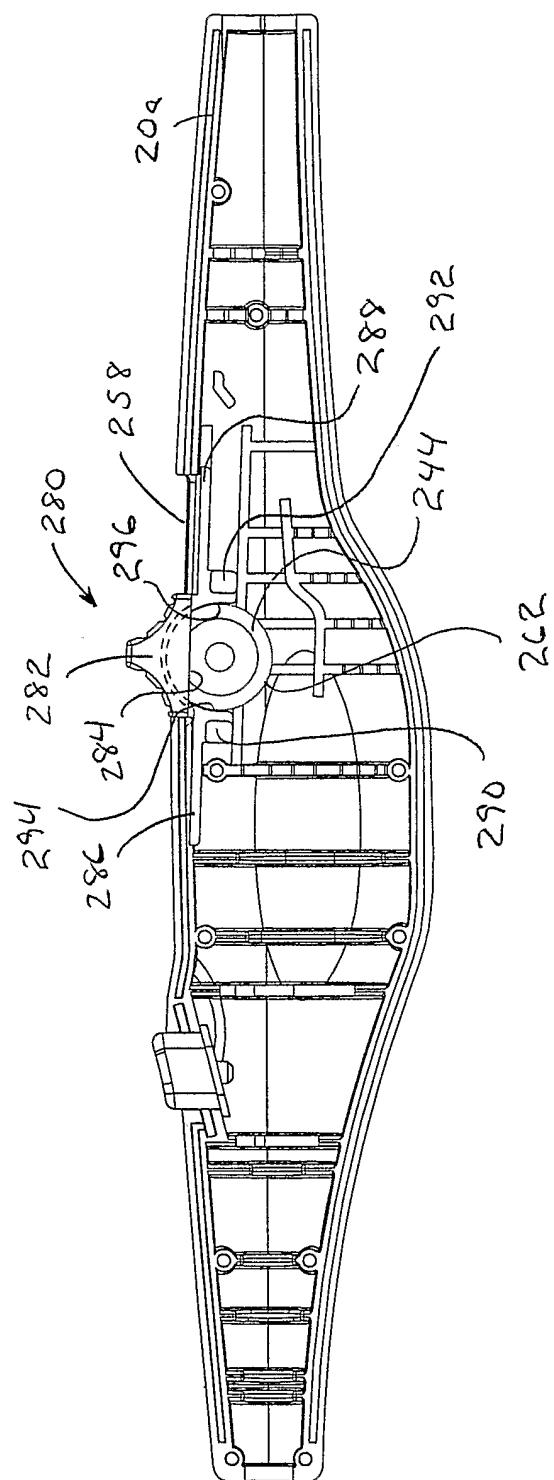
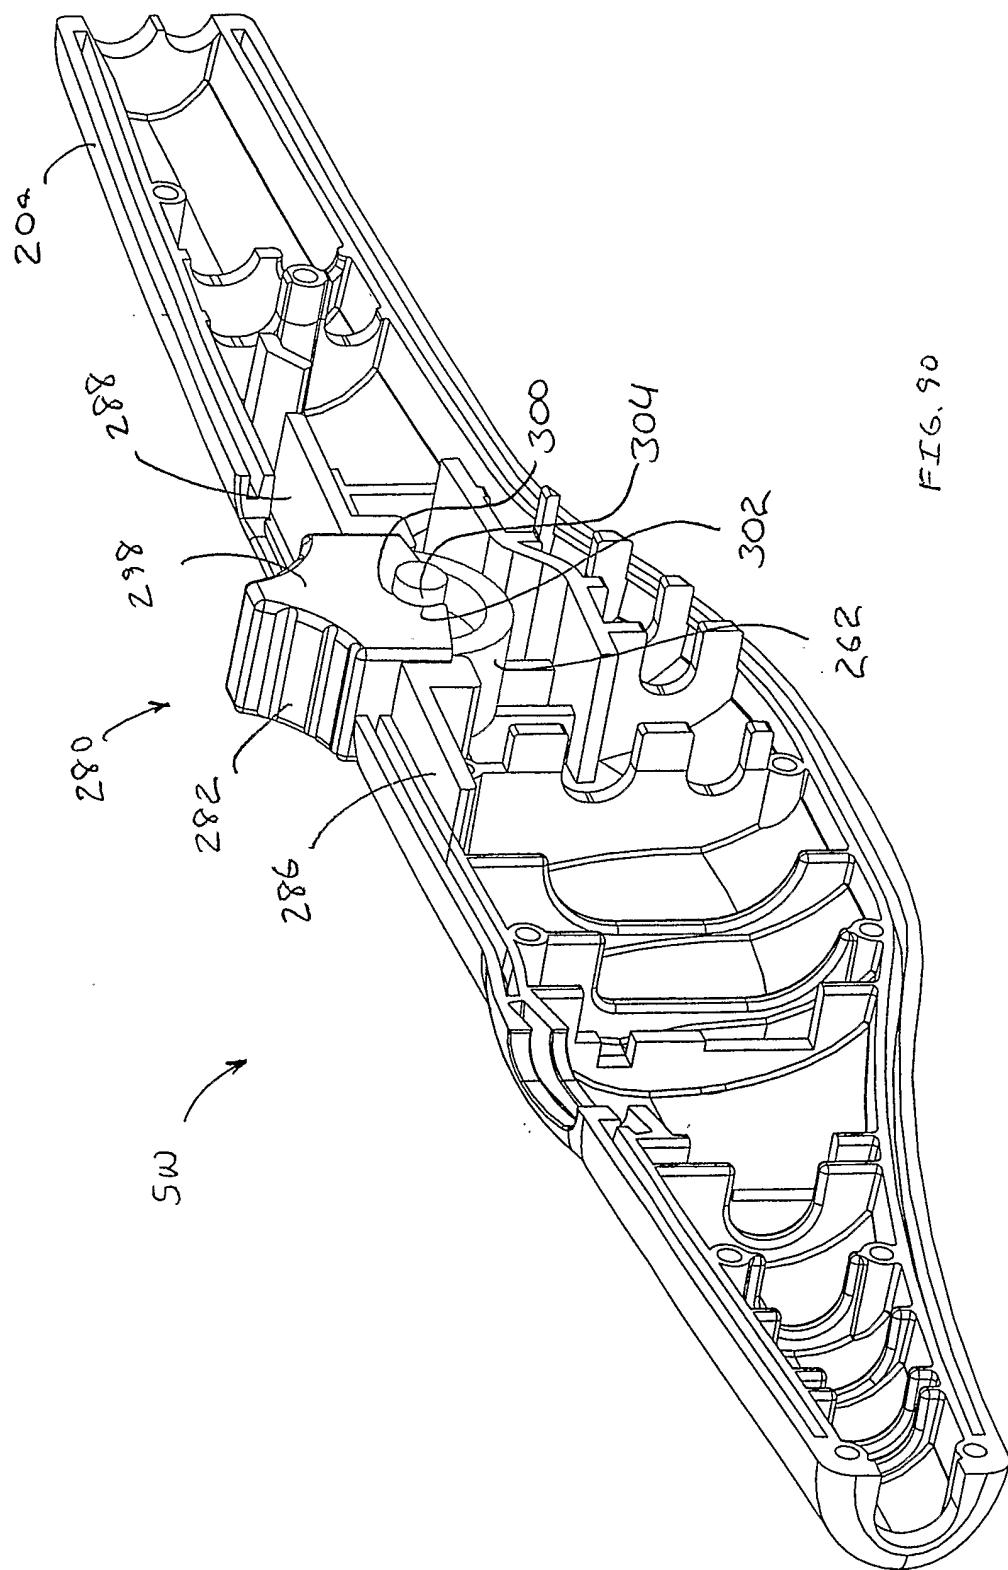


FIG. 89



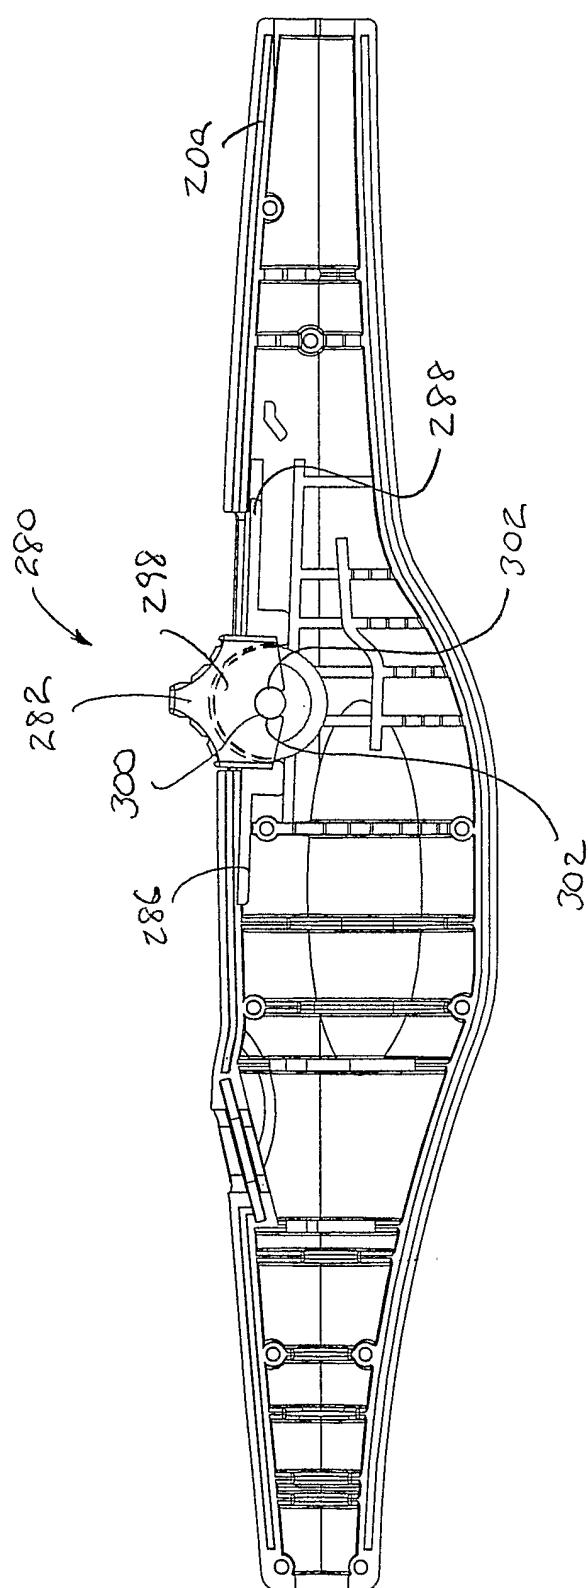
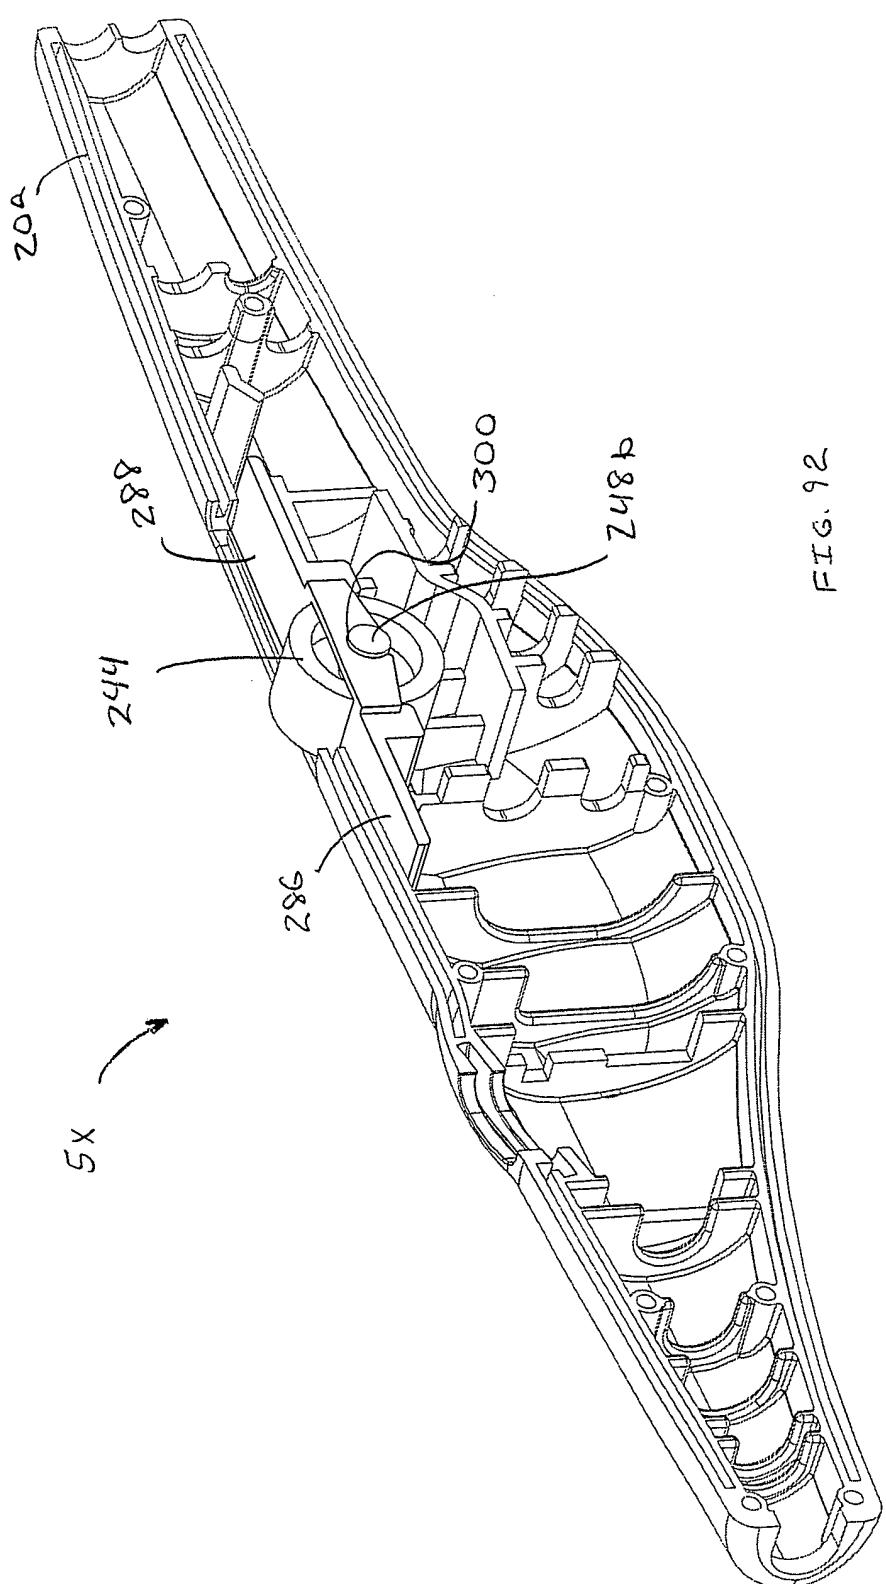


FIG. 91



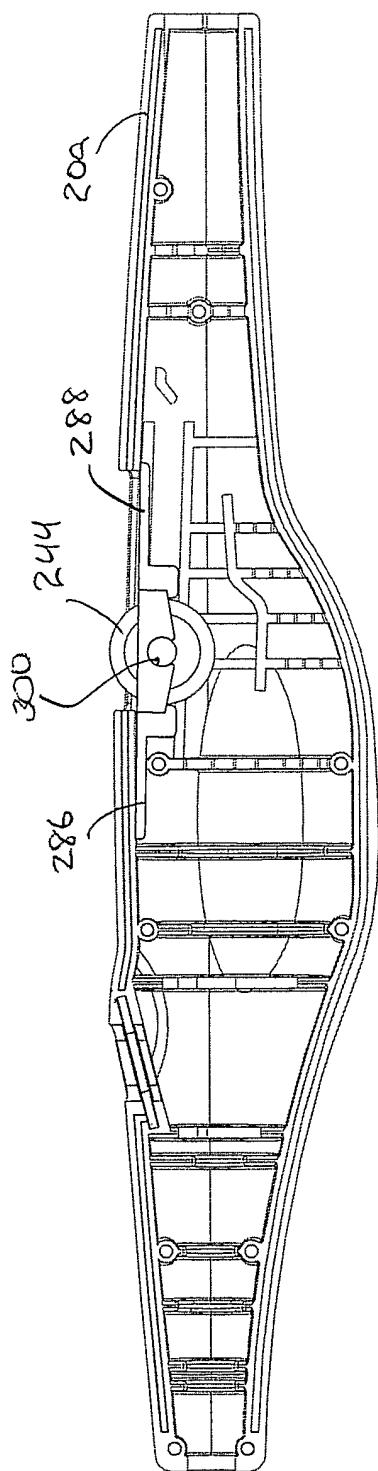


FIG. 93

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US02/28488

A. CLASSIFICATION OF SUBJECT MATTER

IPC(7) : A 61 B 18/18

US CL : 606/034

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 606/034, 27-32, 35, 38, 39, 41, 42

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 6,024,733 A (EGGERS et al.) 15 February 2000, see entire document.	1-137

<input type="checkbox"/>	Further documents are listed in the continuation of Box C.	<input type="checkbox"/>	See patent family annex.
*	Special categories of cited documents:	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A"	document defining the general state of the art which is not considered to be of particular relevance	"X"	document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E"	earlier application or patent published on or after the international filing date	"Y"	document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&"	document member of the same patent family
"O"	document referring to an oral disclosure, use, exhibition or other means		
"P"	document published prior to the international filing date but later than the priority date claimed		

Date of the actual completion of the international search

21 October 2002 (21.10.2002)

Date of mailing of the international search report


13 DEC 2002

Name and mailing address of the ISA/US

Commissioner of Patents and Trademarks
Box PCT
Washington, D.C. 20231

Facsimile No. (703)305-3230

Authorized officer


Linda C. Dvorak

Telephone No. 703/3080858