



US0D1031995S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,031,995 S**  
**Mézière et al.** (45) **Date of Patent:** **\*\* Jun. 18, 2024**

(54) **DIAGNOSTIC APPARATUS**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **bioMérieux**, Marcy l'Etoile (FR)  
(72) Inventors: **Cyril Mézière**, Villeurbanne (FR);  
**Philippe Marbaix**, La  
Balme-les-Grottes (FR); **Enrico Balatri**,  
Florence (IT)

EM 002755611-0001 \* 8/2015  
EM 003530823-0001 \* 12/2016  
EM 003531342-0001 \* 12/2016

(Continued)

OTHER PUBLICATIONS

Meril Diagnostics, AutoQuant 100 Amara, Nov. 8, 2018, Merillife.com, Retrieved from internet: <https://www.merillife.com/medical-devices/diagnostics/biochemistry/autoquant-100-amara> (Year: 2023).\*

(Continued)

(73) Assignee: **bioMérieux**, Marcy l'Etoile (FR)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/809,071**

(22) Filed: **Sep. 24, 2021**

*Primary Examiner* — Jennifer L Rempfer

*Assistant Examiner* — Edward P Jones

(74) *Attorney, Agent, or Firm* — Volpe Koenig

(30) **Foreign Application Priority Data**

Mar. 26, 2021 (EM) ..... 008475636-0001  
Mar. 31, 2021 (EM) ..... 008481923-0001

(57) **CLAIM**

The ornamental design for a diagnostic apparatus, as shown and described.

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/186**

**DESCRIPTION**

(58) **Field of Classification Search**  
USPC ..... D24/107, 232, 234, 216, 231  
CPC .. G01N 33/53; G01N 33/50; G01N 33/56966;  
G01N 33/5302; B01L 7/00  
See application file for complete search history.

The patent or application file contains at least one drawing executed in color. Copies of this patent or patent application publication with color drawings will be provided by the Office upon request and payment of the necessary fee.

FIG. 1 is a front perspective view of the diagnostic apparatus according to our design;  
FIG. 2 is a rear perspective view thereof;  
FIG. 3 is a front view thereof;  
FIG. 4 is a rear view thereof;  
FIG. 5 is a bottom view thereof;  
FIG. 6 is a top view thereof;  
FIG. 7 is a bottom perspective view thereof; and,  
FIG. 8 is a right-side view thereof, the left-side view being a mirror image thereof.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D330,596 S \* 10/1992 Frenkel ..... D24/186  
D378,782 S \* 4/1997 LaBarbera ..... D24/231  
D381,756 S \* 7/1997 Ohnuma ..... D24/231  
D523,153 S \* 6/2006 Akashi ..... D10/81  
D735,883 S \* 8/2015 Bauer ..... D24/234  
D818,146 S \* 5/2018 Tanaka ..... D24/216  
D854,187 S \* 7/2019 Meindl ..... D24/232  
D854,703 S \* 7/2019 Juhlin ..... D24/216

(Continued)

**1 Claim, 8 Drawing Sheets**  
**(8 of 8 Drawing Sheet(s) Filed in Color)**



(56)

**References Cited**

U.S. PATENT DOCUMENTS

D890,361 S \* 7/2020 Nüesch ..... D24/232  
D962,473 S \* 8/2022 Wu ..... D24/232

FOREIGN PATENT DOCUMENTS

EM 003763754-0002 \* 2/2017  
EM 005796547-0001 \* 10/2018  
GB 9003763754-0001 \* 2/2017

OTHER PUBLICATIONS

Boditech, Automated Immunoassay Analyzer with the all-in-one cartridge system, Jul. 6, 2018, Retrieved from internet: <https://www.boditech.co.kr/en/product/instruments/id/2> (Year: 2018).\*

Randox, Fully Automated Batch Immunoanalyzer, Jul. 24, 2019, <https://www.randox.com>, Retrieved from internet: <https://www.randox.com/ibms19/> (Year: 2019).\*

GMI Trusted Laboratory Solutions, Lab Companion ISS-7100 / ISS-7100R Stackable Incubated Shaker, 2023, Lab Companion, Retrieved from internet: <https://www.gmi-inc.com/product/lab-companion-iss-7100-iss-7100r-stackable-incubated-shaker/> (Year: 2023).\*

BioMérieux, bioMérieux announces CEmarking of Vidas® Kube™, the . . . , Dec. 20, 2022, Retrieved from internet: [https://www.biomerieux-diagnostics.com/sites/clinic/files/news-event-press-release/pr\\_biomerieux\\_vidas\\_kube\\_20221220.pdf](https://www.biomerieux-diagnostics.com/sites/clinic/files/news-event-press-release/pr_biomerieux_vidas_kube_20221220.pdf) (Year: 2022).\*

\* cited by examiner



FIG. 1



FIG. 2

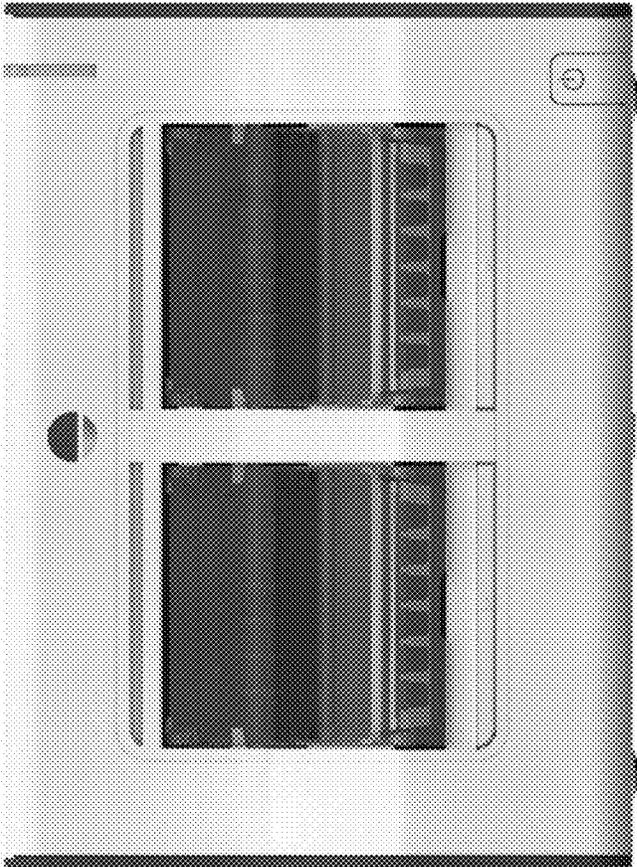


FIG. 3

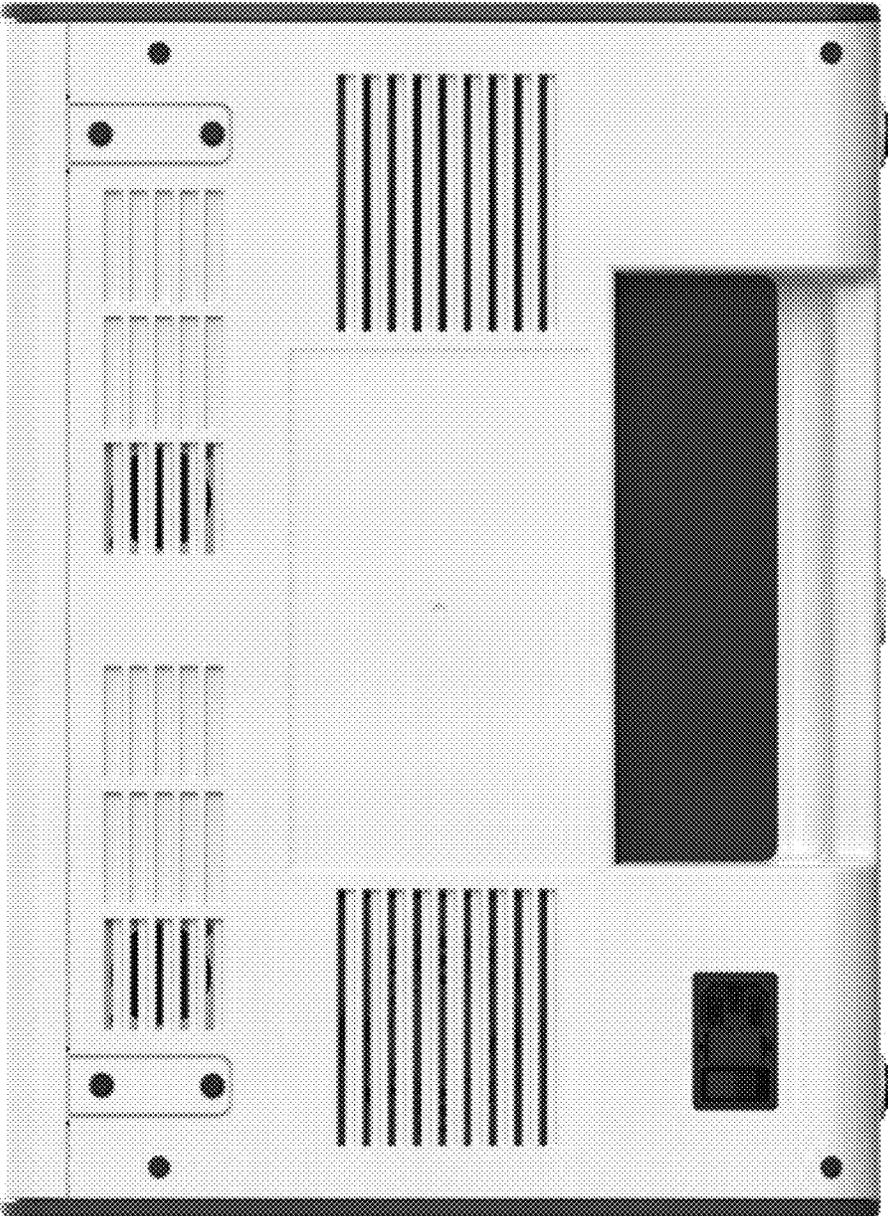
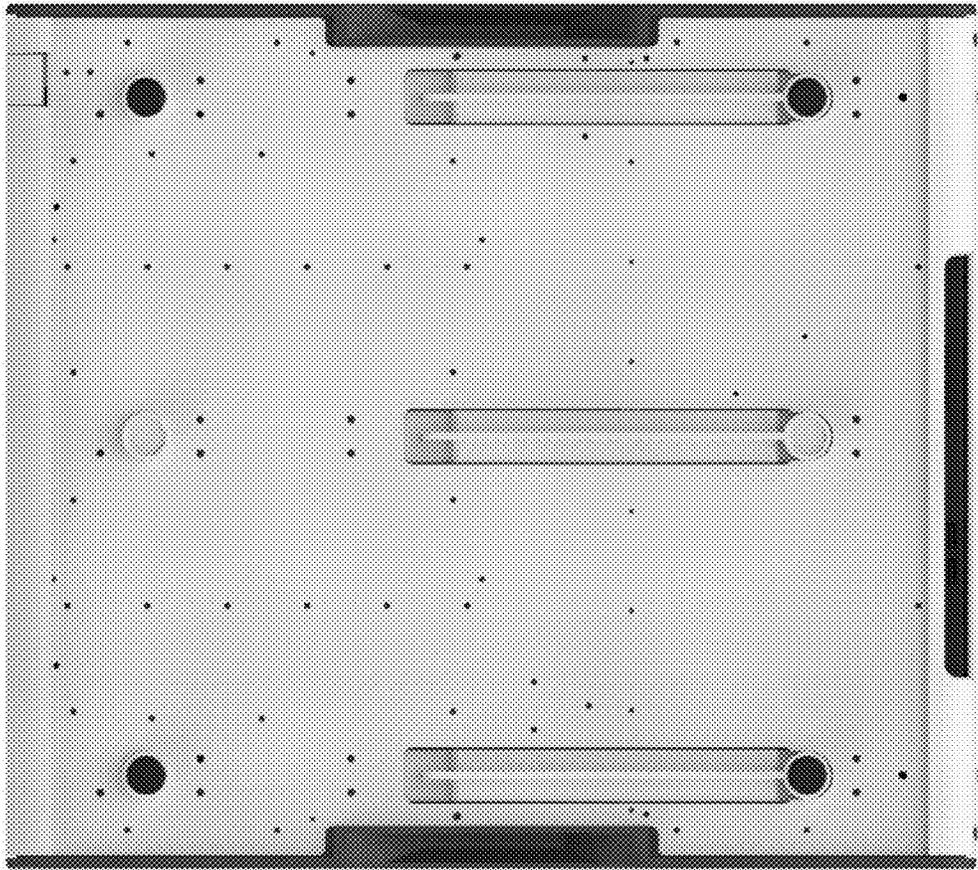


FIG. 4

FIG. 5



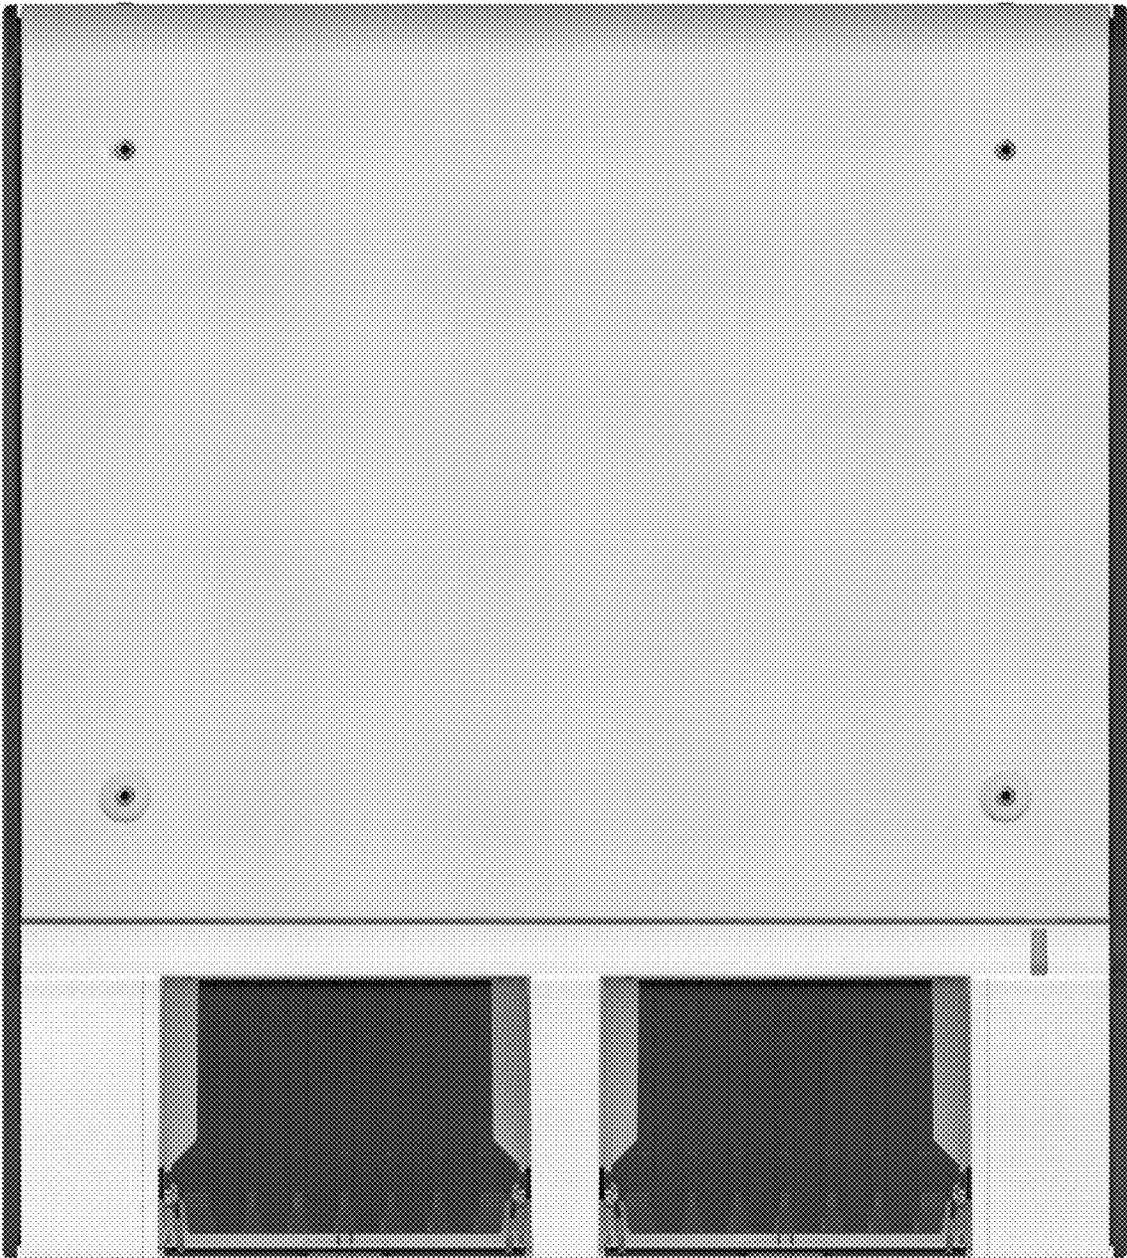


FIG. 6

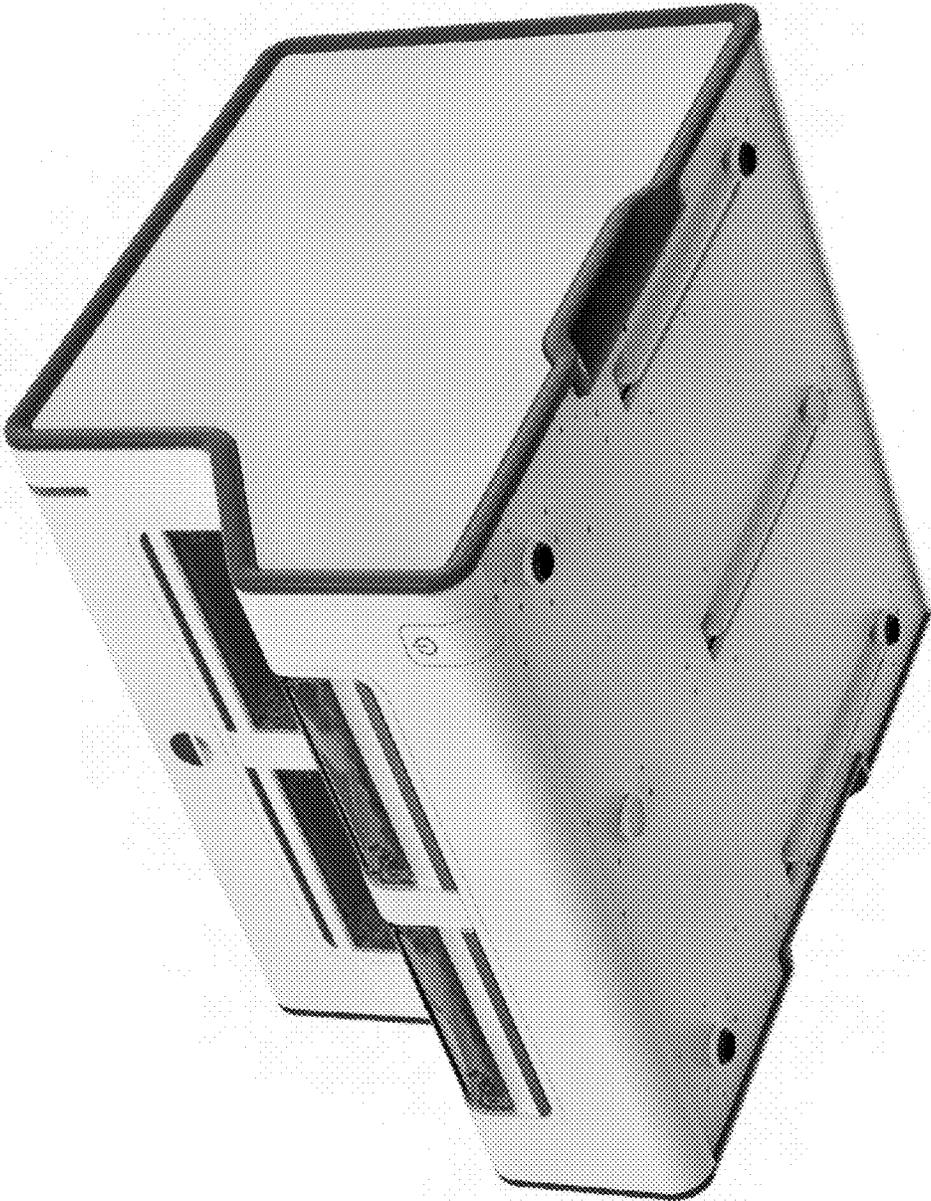


FIG. 7

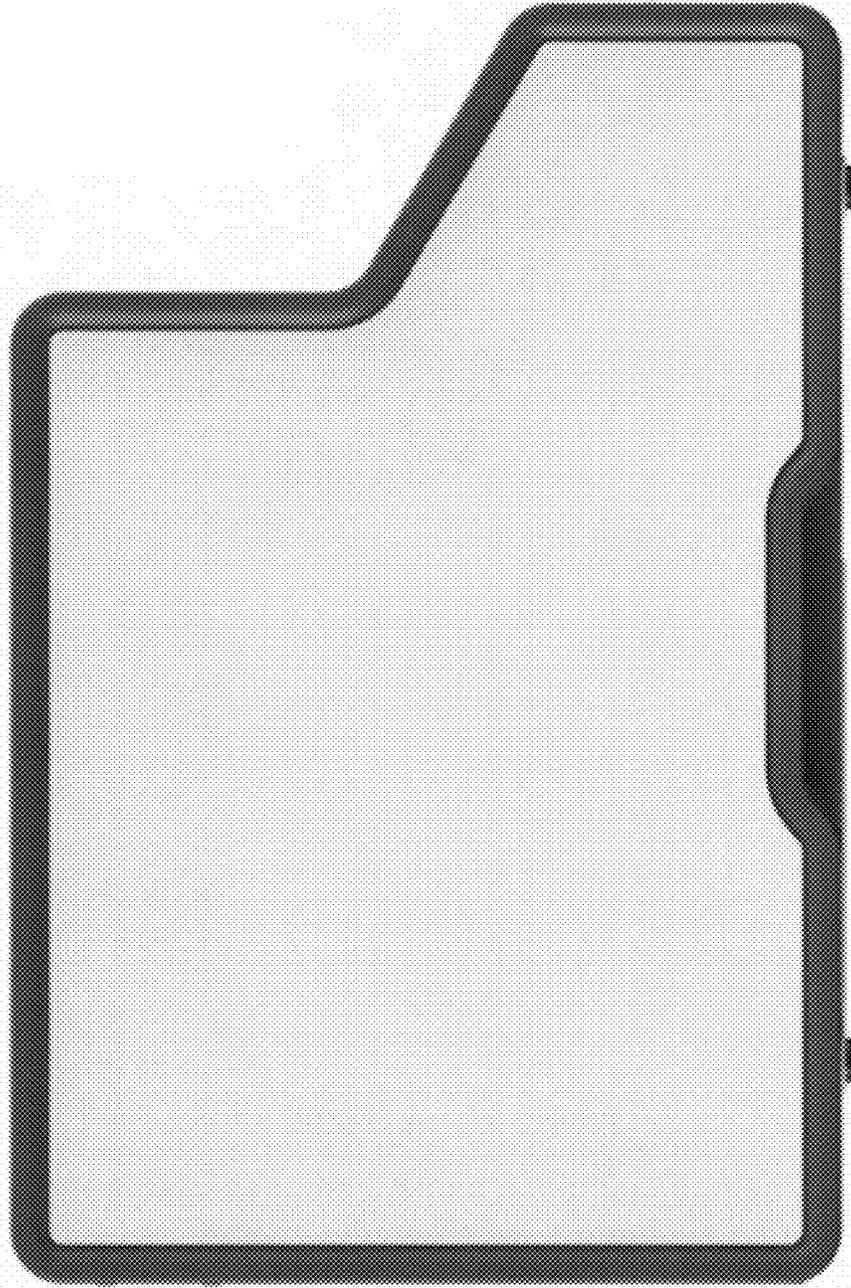


FIG. 8