



(11) **EP 2 364 662 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
14.09.2011 Bulletin 2011/37

(51) Int Cl.:
A61B 18/14 ^(2006.01) **A61B 18/12** ^(2006.01)
A61B 18/00 ^(2006.01)

(21) Application number: **10192580.8**

(22) Date of filing: **31.03.2009**

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL
PT RO SE SI SK TR**
Designated Extension States:
AL BA RS

(30) Priority: **31.03.2008 US 41045 P**
31.03.2008 US 40994 P
31.03.2008 US 41012 P
31.03.2008 US 40980 P
31.03.2008 US 40828 P
31.03.2008 US 40890 P
31.03.2008 US 40957 P
18.11.2008 US 115756 P

(62) Document number(s) of the earlier application(s) in
accordance with Art. 76 EPC:
09728455.8 / 2 265 196

(71) Applicant: **APPLIED MEDICAL RESOURCES
CORPORATION**
Rancho Santa Margarita, CA 92688 (US)

(72) Inventors:
• **Falkenstein, Zoran**
Rancho Santa Margarita, CA 92688 (US)
• **Cappello, Christopher J.**
Central City, CO 80427-0485 (US)
• **Johnson, Gary M.**
Mission Viejo, CA 92692 (US)
• **Gianneschi, Benjamin A.**
Orange, CA 92866 (US)
• **Tran, Oliva J.**
Torrance, CA 90501 (US)

- **Wixey, Matthew A.**
Rancho Santa Margarita, CA 92688 (US)
- **Pravongviengkham, Kennii**
Garden Grove
CA 92843 (US)
- **Pravong, Boun**
Corona, CA 92879 (US)
- **Yawata, Haruyasu**
Hungtington Beach, CA 92646 (US)
- **Brustad, John R.**
Dana Point, CA 92629 (US)
- **Cohen, Adam J.**
Worcester, MA 10602 (US)
- **Hilal, Nabil**
Laguna Niguel, CA 92677 (US)
- **Becerra, Matthew M.**
Foothill Ranch, CA 92610 (US)
- **Pingleton, Edward D.**
San Juan Capistrano, CA 92675 (US)
- **Hilal, Said S.**
Cota de Caza, CA 92679 (US)
- **Hart, Charles C.**
Summerville, SC 29483-8949 (US)
- **Wikoff, Chris R.**
Newport Beach, AL 92663 (US)

(74) Representative: **Fitchett, Stuart Paul**
Saunders & Dolleymore LLP
9 Rickmansworth Road
Watford
Hertfordshire WD18 0JU (GB)

Remarks:

This application was filed on 25-11-2010 as a
divisional application to the application mentioned
under INID code 62.

(54) **Electrosurgical system with a switching mechanism**

(57) Phase end point determination is provided to automatically halt the application of energy to tissue. Prior to the application of energy, the phase end point determination is identified by measuring the product of permittivity and conductivity of the tissue to be treated. An electrosurgical system can include an electrosurgical generator, a feedback circuit or controller, and an electrosurgical tool. The feedback circuit can provide an elec-

troscopy endpoint by determining the phase end point of a tissue to be treated. The electrosurgical system can include more than one electrosurgical tool for different electrosurgical operations and can include a variety of user interface features and audio/visual performance indicators. The electrosurgical system can also power conventional bipolar electrosurgical tools and direct current surgical appliances.

EP 2 364 662 A1

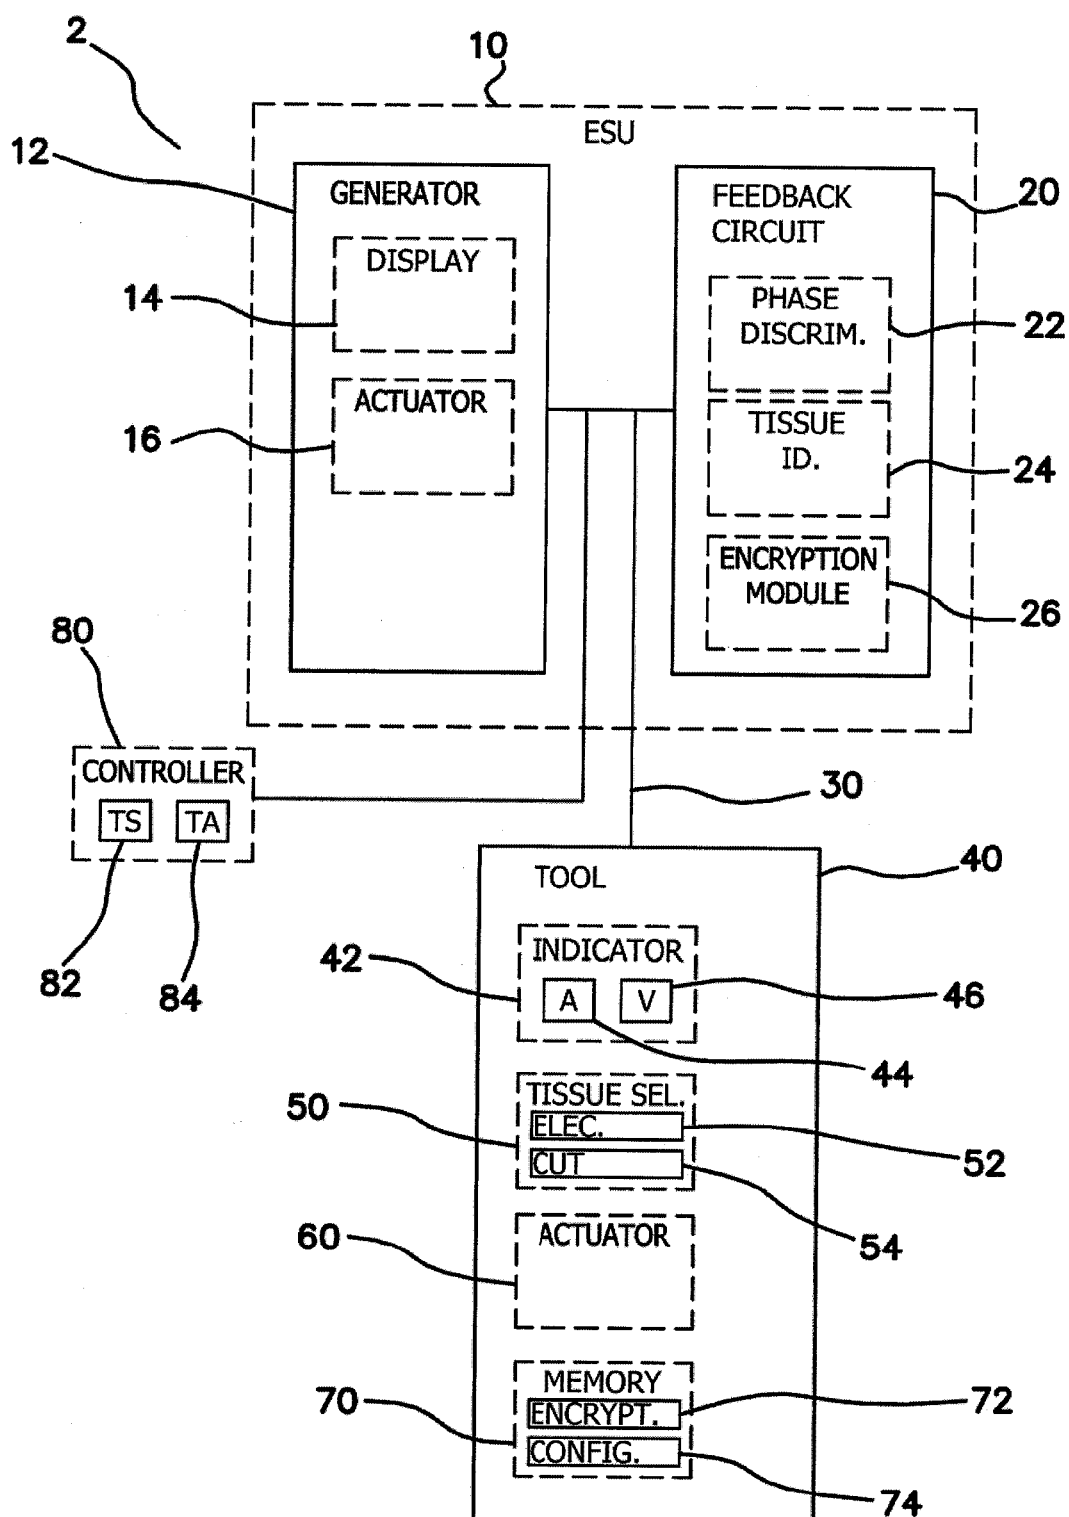


FIG. 1A

Description

Background

Field

[0001] The present application relates generally to electrosurgical systems and methods. More specifically, the present application relates to determination of an electrosurgery endpoint using phase shift monitoring.

Discussion of the Relevant Art

[0002] Surgical procedures often involve cutting and connecting bodily tissue including organic materials, musculature, connective tissue and vascular conduits. For centuries, sharpened blades and sutures have been mainstays of cutting and reconnecting procedures. As bodily tissue, especially relatively highly vascularized tissue is cut during a surgical procedure, it tends to bleed. Thus, medical practitioners such as surgeons have long sought surgical tools and methods that slow or reduce bleeding during surgical procedures.

[0003] More recently, electrosurgical tools have become available that use electrical energy to perform certain surgical tasks. Typically, electrosurgical tools are hand tools such as graspers, scissors, tweezers, blades, needles, and other hand tools that include one or more electrodes that are configured to be supplied with electrical energy from an electrosurgical generator including a power supply. The electrical energy can be used to coagulate, fuse, or cut tissue to which it is applied. Advantageously, unlike typical mechanical blade procedures, application of electrical energy to tissue tends to stop bleeding of the tissue.

[0004] Electrosurgical tools typically fall within two classifications: monopolar and bipolar. In monopolar tools, electrical energy of a certain polarity is supplied to one or more electrodes on the tool. A separate return electrode is electrically coupled to a patient. Monopolar electrosurgical tools can be useful in certain procedures, but can include a risk of certain types of patient injuries such as electrical burns often at least partially attributable to functioning of the return electrode. In bipolar electrosurgical tools, one or more electrodes is electrically coupled to a source of electrical energy of a first polarity and one or more other electrodes is electrically coupled to a source of electrical energy of a second polarity opposite the first polarity. Thus, bipolar electrosurgical tools, which operate without separate return electrodes, can deliver electrical signals to a focused tissue area with a reduced risk of patient injuries.

[0005] Even with the relatively focused surgical effects of bipolar electrosurgical tools, however, surgical outcomes are often highly dependent on surgeon skill. For example, thermal tissue damage and necrosis can occur in instances where electrical energy is delivered for a relatively long duration or where a relatively high-power

electrical signal is delivered even for a short duration. The rate at which a tissue will achieve the desired coagulation or cutting effect upon the application of electrical energy varies based on the tissue type and can also vary based on pressure applied to the tissue by an electrosurgical tool. However, even for a highly experienced surgeon, it can be difficult for a surgeon to assess how quickly a mass of combined tissue types grasped in an electrosurgical instrument will be fused a desirable amount.

[0006] Attempts have been made to reduce the risk of tissue damage during electrosurgical procedures. For example, previous electrosurgical systems have included generators that monitor an ohmic resistance or tissue temperature during the electrosurgical procedure, and terminated electrical energy once a predetermined point was reached. However, these systems have had shortcomings in that they have not provided consistent results at determining tissue coagulation, fusion, or cutting endpoints for varied tissue types or combined tissue masses. These systems can also fail to provide consistent electrosurgical results among use of different tools having different tool and electrode geometries. Typically, even where the change is a relatively minor upgrade to tool geometry during a product's lifespan, the electrosurgical generator must be recalibrated for each tool type to be used, a costly, time consuming procedure which can undesirably remove an electrosurgical generator from service.

Summary

[0007] In view of at least the foregoing shortcomings of the previous electrosurgical systems, there is a need in the art to improve control of electrosurgical procedures to enhance consistency of electrosurgical results among electrosurgical tools and tissue types. Accordingly, there is a need for an improved electrosurgical system that can accurately assess an electrical energy application endpoint for a desired electrosurgical procedure. There is also a need for an electrosurgical system that monitors tissue properties during the electrosurgical procedure to assess the energy application endpoint. There is also a need for an improved electrosurgical system that can rapidly accommodate various electrosurgical tools with minimal impact on surgical outcome. To address some or all of these needs and provide various additional advantages as discussed below in greater detail, various embodiments, methods, systems, and apparatuses for electrosurgical procedures are provided.

[0008] In various embodiments, methods and apparatuses for bloodless dissection of connective and vascular tissue are provided. The various methods and apparatuses described herein can be used in minimally invasive surgery, particularly laparoscopic surgery.

[0009] At the same time, various embodiments of the surgical tools described herein can include different electrode configurations. I.e., while in one embodiment only

the lower jaw is utilized to provide both coagulation and cutting functions, another embodiment can also employ the upper jaw element to be used in the coagulation and/or cutting process. In yet another embodiment, each jaw element can carry multiple electrode elements, greatly increasing the functionality of the tool. A specific electrode arrangement can allow for tools that are more suitable for particular surgical procedures.

[0010] Another aspect of the surgical tools described herein relates to activation and deactivation of one or multiple electrodes, based on the position of the jaw elements. This position-based actuation allows, for example, activation of the upper jaw electrodes only in a near-closed position of the tool (or, in other embodiments, in an opened or near-opened position of the tool). In some embodiments, electrical switches in the jaw element driving mechanism can be positioned in a hand-piece of the surgical tool to selectively activate and deactivate one or multiple electrodes based on a position of the jaw elements. In other embodiments, the activation and deactivation can be performed by sliding contacts that are assembled in the hand-piece.

[0011] Yet another aspect of the surgical tools described herein is the automated switching from coagulation to cutting, enabled by use of a multi-electrode generator. Here, a tissue feedback mechanism triggers both switching from one set of coagulation electrodes (applied with voltages appropriate for coagulation) to another set of cutting electrodes (applied with voltages appropriate for cutting). As such, each individual tool electrode can be relayed through a bus-bar connection to any polarity of choice of the power supply. In addition, tool position switches in the hand tool can provide with logic switching for the population of different coagulation and/or cutting settings, depending on the specific tool position.

[0012] In certain embodiments, an electrosurgical tool is provided comprising a first jaw, a second jaw, a first electrode, a second electrode, and a third electrode. The second jaw is pivotable with respect to the first jaw. The first electrode is positioned on the first jaw. The second electrode is positioned on the first jaw. The third electrode is positioned on the first jaw. The electrosurgical tool can be selectively configurable in a coagulation configuration such that at least one of the first, second, and third electrodes is electrically coupled with a source of electrical energy having a first polarity and at least one other of the electrodes is electrically coupled with a source of electrical energy having a second polarity generally opposite the first polarity and in a cutting configuration such that one of the first, second, and third electrodes is electrically coupled with a source of electrical energy having a cutting voltage and at least one other of the electrodes is configured to be a return electrode.

Brief Description of the Drawings

[0013] The present inventions may be understood by reference to the following description, taken in connec-

tion with the accompanying drawings in which the reference numerals designate like parts throughout the figures thereof.

[0014] Figure 1A is a schematic block diagram of an embodiment of electrosurgical system.

[0015] Figure 1B is a schematic block diagram of another embodiment of electrosurgical system.

[0016] Figure 2A is a perspective view of components of one embodiment of an electrosurgical system.

[0017] Figure 2B is a perspective view of components of one embodiment of an electrosurgical system.

[0018] Figure 2C is a perspective view of components of one embodiment of electrosurgical system.

[0019] Figure 3A is a perspective view of an electrosurgical unit for use in an electrosurgical system.

[0020] Figure 3B is a front view of the electrosurgical unit of Figure 3A.

[0021] Figure 3C is a rearview of the electrosurgical unit of Figure 3A.

[0022] Figure 4 is a block diagram of a fusion or welding process of an electrosurgical unit.

[0023] Figure 5A is a perspective view of an embodiment of laparoscopic sealer/divider.

[0024] Figure 5B is a disassembled view of a laparoscopic sealer/divider of Figure 1A.

[0025] Figures 6A-6C are views of an actuator of the laparoscopic sealer/divider of Figure 5A.

[0026] Figure 7 is a top cross-sectional view of an actuator of a laparoscopic sealer/divider of Figure 5A.

[0027] Figures 8A-8D are views of a shaft assembly of a laparoscopic sealer/divider of Figure 5A.

[0028] Figures 9A-9C are views of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0029] Figures 10A-10G are cross-sectional side views of a laparoscopic sealer/divider of Figure 5A.

[0030] Figures 11-1 and 11-2 are perspective views of a controller of a laparoscopic sealer/divider of Figure 5A.

[0031] Figure 12A is a side view of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0032] Figures 12B-12C are graphical representations of exemplary vessel sealing pressures provided by a laparoscopic sealer/divider of Figure 5A.

[0033] Figures 13-1, 13-2 and 13-3 are top level views of an electrode configuration of a laparoscopic sealer/divider of Figure 5A.

[0034] Figure 14 is a top level view of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0035] Figure 15 is a side view of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0036] Figures 16-1 and 16-2 are views of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0037] Figure 17A is a perspective view of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0038] Figure 17B is a perspective view of an actuator of a laparoscopic sealer/divider of Figure 5A.

[0039] Figures 18-1, 18-2 and 18-3 are views of portions of a shaft assembly of a laparoscopic sealer/divider of Figure 5A.

[0040] Figures 19-1 and 19-2 are views of a jaw assembly of a laparoscopic sealer/divider of Figure 5A.

[0041] Figure 20 is a perspective view of an embodiment of surgical tool for use in a laparoscopic surgical procedure.

[0042] Figure 21 is a perspective drawing of the distal end of an exemplary tissue fusion/cutting devices.

[0043] Figures 22A-D are schematic drawings of various embodiments of distal end configurations for an electrosurgical bloodless tissue dissection device.

[0044] Figures 23A-C are schematic drawings of active electrode switching circuitries in the hand tools.

[0045] Figure 24 is a schematic drawing of the inside of the hand-piece, illustrating the embodiment of active electrode switching mechanism based on the opening of the jaw elements.

[0046] Figure 25 depicts another embodiment of an active electrode switching mechanism, also based on the opening of the jaw elements.

[0047] Figure 26 depicts an embodiment of a passive switching mechanism, also based on the opening of the jaw elements.

[0048] Figure 27 depicts another embodiment of a passive switching mechanism, based on both the opening and closing of the jaw elements.

[0049] Figure 28 depicts a schematic circuitry that connects five electrodes through relays to a bus bar which is relayed to a measurement circuit, or an electrosurgical power plant.

[0050] Figure 29 schematically illustrates one embodiment of a method for substantially bloodless dissection of biological tissue.

Detailed Description

[0051] The following description is provided to enable any person skilled in the art to make and use the surgical tools and perform the methods described herein and sets forth the best modes contemplated by the inventors of carrying out their inventions. Various modifications, however, will remain apparent to those skilled in the art. It is contemplated that these modifications are within the scope of the present disclosure.

Electrosurgical System

[0052] Figure 1A illustrates a schematic diagram of an electrosurgical system 2. The electrosurgical system 2 can comprise an electrosurgical unit (ESU) 10 and an electrosurgical tool 40. The electrosurgical tool 40 can be electrically coupled to the electrosurgical unit 10. In some embodiments, an electronic coupler 30 such as an electrical wire, wire bundle, or cable can electrically couple the electrosurgical tool 40 to the ESU 10. In some embodiments, the electrosurgical system 2 can optionally further comprise an external tool controller 80.

[0053] With continued reference to Figure 1A, the electrosurgical unit 10 can comprise a generator 12 and a

feedback circuit 20. The generator 12 can include an actuator 16 such as a power supply and a signal processor configured to generate a radiofrequency (RF) electrosurgical signal. The generator 12 can further comprise a display 14. The display 14 can be configured to indicate the status of the electrosurgical system 2, including, among other information, the status of the actuator 16 and the status of the electrosurgical tool 40 electrically coupled to the electrosurgical unit 10.

[0054] With continued reference to Figure 1A, the feedback circuit 20 of the ESU 10 can comprise a phase discriminator 22, a tissue identifier 24, and an encryption module 26. In some embodiments, the phase discriminator 22 can be electrically coupled to the tissue identifier 24. The phase discriminator 22 can be configured to receive information from the electrosurgical tool 40 electrically coupled to the ESU 10. In some embodiments, the information from the electrosurgical tool 40 comprises information regarding an applied voltage and a supplied current to the electrosurgical tool, and the phase discriminator 22 can be configured to calculate a phase difference between the applied voltage and the supplied current. The encryption module 26 can be configured to transmit and receive data formatted in an encrypted protocol. The encrypted protocol can be one of several commercially-available encryption protocols, or, in some embodiments can be a purpose developed encryption protocol.

[0055] With continued reference to Figure 1A, In some embodiments, the feedback circuit 20 can be one or more integrated circuits, printed circuit boards, or other processor collocated with the generator 12 within an integrated ESU 10. As illustrated in Figure 1B, In other embodiments, the feedback circuit 20' can be electrically coupled to a stand-alone generator 12' to form an ESU 10'. The tool 40 can be electrically coupled to the feedback circuit 20'. Other aspects of electrosurgical systems having a stand-alone generator 12' and feedback circuit 20' can be substantially similar to systems having an integrated ESU discussed with respect to Figure 1A.

[0056] With continued reference to Figure 1A, the tool 40 can comprise an indicator 42, a tissue selector 50, an actuator 60, and a memory 70. In some embodiments, the indicator 40 can comprise an audio indicator 44 such as a speaker, a chime, a clicker device, or another audio generation device. In some embodiments, the indicator 40 can comprise a visual indicator 46 such as a lamp, an LED, a display, a counter, or another visual indication device. In some embodiments, the visual indicator 46 comprises a multi-color LED. In some embodiments, the tool 40 comprises both an audio indicator 44 and a visual indicator 46.

[0057] The tissue selector 50 can comprise an electrode assembly 52 and a cutting tool 54. In various embodiments, various electrode assemblies can be configured to perform a desired electrosurgical procedure such as, for example, coagulation, cutting, or fusion, on a particular tissue. In some embodiments, the electrode as-

sembly 52 can be configured for use as a vascular sealer. In other embodiments, the electrode assembly 52 can be configured for use as a bariatric stapler. In still other embodiments, the electrode assembly 52 can be configured for use as a tissue cutting device. In some embodiments, the cutting tool 54 can be a mechanical element such as a stationary or moveable blade or sharpened edge. In other embodiments, the cutting tool 54 can be an electrosurgical element such as an energizable wire or filament.

[0058] With continued reference to Figure 1A, the actuator 60 can be operatively coupled to the tissue selector 50 to selectively select tissue. For example, in some embodiments, the tissue selector 50 can include a jaw-based grasper, and the actuator can comprise an actuation mechanism to selectively move the grasper from an open position to a closed position. In other embodiments, it is contemplated that other tissue selectors can be used in the electrosurgical system 2. In some embodiments, the actuator 60 can also be configured to selectively energize the electrodes. For example, the actuator 60 can comprise a switch or button on the tool.

[0059] With continued reference to Figure 1A, the tool 40 can further comprise a memory 70. In some embodiments, the memory 70 comprises an encryption module 72 and a configuration device module 74. The encryption module 72 can be configured to facilitate an encrypted information exchange with the encryption module 26 on ESU 10. The configuration device module 74 can store operational parameter information about the tool 40. For example, in some embodiments, the configuration device module 74 can store information regarding the electrode assembly, the number of uses and total operational time of use of the tool, and other operational parameters.

[0060] With continued reference to Figure 1A, the electrosurgical system 2 can further comprise an external tool controller 80 electrically coupling the ESU 10 to the tool 40. In some embodiments, the external tool controller 80 comprises a tool selector 82 such as a switch. The external tool controller 80 can allow for multiple devices to connect thereto. A tool selector 82 allows selection of one of the multiple devices to be energized. For example the tool selector 82 can comprise a dial, switch, or toggle. The tool actuator 84 can selectively electrically couple the selected tool 40 with the ESU 10. 3

[0061] With reference to Figure 2A, an exemplary embodiment of electrosurgical system 102 is illustrated including an ESU 110, and an electrosurgical fusion tool 120. The electrosurgical fusion tool 120 can be electrically coupled to the ESU 110 by an electrical coupler 130 such as with a cabled connection to a tool port 112 on the ESU 110. In the illustrated embodiment, the electrosurgical fusion tool 120 comprises a tissue sealer and divider, as discussed in further detail below with respect to Figures 5A-19. The electrosurgical fusion tool 120 comprises visual indicators 122 such as multi-color LEDs positioned there on to apprise a user of the status of the tool. In other embodiments, the electrosurgical fusion tool

120 can be electrically coupled to a generator or a different electrosurgical unit. In some embodiments, a manual controller such as a hand of foot switch can be electrically coupled to the ESU 110 or the electrosurgical fusion tool 122 to allow selective control of the tool.

[0062] With reference to Figure 2B, an exemplary embodiment of electrosurgical system 202 is illustrated including an ESU 210, and an electrosurgical tool 220. The electrosurgical tool 220 can be electrically coupled to the ESU 210 such as with a cabled connection to a tool port 212 on the ESU 210. In the illustrated embodiment, the electrosurgical tool 220 comprises an electric cutting and coagulation tool, as discussed in further detail below with respect to Figures 20-29. The electrosurgical tool 220 comprises visual indicators 222 such as multi-color LEDs positioned there on to apprise a user of the status of the tool. In other embodiments, the electrosurgical tool 220 can be electrically coupled to a generator or a different electrosurgical unit. In some embodiments, a manual controller such as a hand of foot switch can be electrically coupled to the ESU 210 or the electrosurgical fusion tool 222 to allow selective control of the tool.

[0063] With reference to Figure 2C, an exemplary embodiment of electrosurgical system 2302 is illustrated including an ESU 310, and an electrosurgical tool 320. The electrosurgical tool 320 can be electrically coupled to the ESU 310 such as with a cabled connection to a tool port 312 on the ESU 310. The electrosurgical tool 320 comprises visual indicators 322 such as multi-color LEDs positioned thereon to apprise a user of the status of the tool. In other embodiments, the electrosurgical tool 320 can be electrically coupled to a generator or a different electrosurgical unit. In some embodiments, a manual controller such as a hand of foot switch can be electrically coupled to the ESU 310 or the electrosurgical tool 322 to allow selective control of the tool.

Integrated Electrosurgical Unit

[0064] With reference to Figures 3A-3C, of electrosurgical unit 410 is illustrated in perspective, front, and rear views. The electrosurgical unit 410 can be an integrated ESU as discussed above with respect to Figure 1A, and can comprise a generator and a feedback circuit. In some embodiments, the housing or console of the electrosurgical unit 410 can be sized and configured to fit on a standard operating room cart or storage rack. In some embodiments, the housing or console of the electrosurgical unit 410 can be configured to be stackable with other surgical electrical equipment.

[0065] With reference to Figures 3A-3B, a perspective view of the electrosurgical unit 410 is illustrated. In the illustrated embodiment, the electrosurgical unit 410 comprises two dedicated tool ports 412, one bipolar tool port 414, and one electrical power port 416. In other embodiments, electrosurgical units can comprise different numbers of ports. For example, in some embodiments, an electrosurgical unit can comprise more or fewer than two

dedicated teleports 412, more or fewer than one bipolar tool port 414, and more or fewer than one power port 416.

[0066] With continued reference to Figures 3A-3B, each dedicated tool port 412 is configured to be coupled to electrosurgical tool having a memory, as described above with respect to Figure 1A. Thus the dedicated tool ports 412 can be electrically coupled to the feedback circuit of the electrosurgical unit 410 as well as the generator. In some embodiments, the dedicated tool ports 412 can comprise multi-pin connectors comprising a plurality of electrical connection pins or pin receptacles. In some embodiments, the connectors can comprise more than 10, for example 20 pins or pin receptacles. As discussed above with respect to Figure 1A, and discussed in further detail below, the dedicated tool ports 412 can be configured for encrypted transmission and reception of data from an electrically coupled electrosurgical tool.

[0067] With continued reference to Figures 3A-3B, the bipolar tool port 414 can include a plug configured to receive a conventional bipolar electrosurgical tool. The bipolar tool port 414 can be coupled to the generator of the electrosurgical unit 410. In some embodiments, the bipolar tool port 414 is not coupled to the feedback circuit of the electrosurgical unit 410. Thus, advantageously, the electrosurgical unit 410 can energize both specialized electrosurgical tools, as described in further detail here and, conventional bipolar electrosurgical tools. Accordingly, the electrosurgical unit 410 can be used in place of a standalone bipolar electrosurgical generator without requiring additional rack or cart space in a surgical workspace.

[0068] With continued reference to Figures 3A-3B, the electrical power port 416 can be coupled to the generator of the electrosurgical unit 410. The electrical power port 416 can be configured to supply direct current. For example, in some embodiments, the electrical power port 416 can provide approximately 12 Volts DC. The electrical power port 416 can be configured to power a surgical accessory, such as a respirator, pump, light, or another surgical accessory. Thus, advantageously, in addition to replacing electrosurgical generator for standard bipolar tools, the electrosurgical unit 410 can also replace a surgical accessory power supply. In some embodiments, replacing presently-existing generators and power supplies with the electrosurgical unit 410 can reduce the amount of storage space required on storage racks cards or shelves in the number of mains power cords required in a surgical workspace.

[0069] With continued reference to Figures 3A-3B, the electrosurgical unit 410 can comprise a display 420. In some embodiments, the display can comprise a multiline display capable of presenting text and graphical information such as for example an LCD panel display, which, in some embodiments can be illuminated via backlight or sidelight. In some embodiments, the display 420 can comprise a multi-color display that can be configured to display information about a particular tool electrically coupled to the electrosurgical unit 410 and a color that cor-

responds to a standard color associated with a surgical procedure (such as, for example cutting operations displayed in yellow text and graphics, fusion or welding operations displayed in purple, and coagulation displayed in blue, bloodless dissection operations can be displayed in yellow and blue). In some embodiments, as discussed in further detail below, the display can be configured to simultaneously indicate status data for a plurality of tools electrically coupled to the electrosurgical unit 410. In some embodiments, a user can toggle the display 420 between presenting status of multiple electrically connected tools and status of a single electrically connected tool.

[0070] With continued reference to Figures 3A-3B, the electrosurgical unit can comprise a user interface such as, for example a plurality of buttons 422. The buttons 422 can allow user interaction with the electrosurgical unit such as, for example, requesting an increase or decrease in the electrical energy supplied to one or more tools coupled to the electrosurgical unit 410. In other embodiments, the display 420 can be a touch screen display thus integrating data display and user interface functionalities. In some embodiments, the electrosurgical unit 410 can comprise an audible indicator, such as a speaker or chime to alert a user of a possible error, the termination of electrical energy supplied, or other conditions. In some embodiments, the electrosurgical unit 410 can be configured such that the audible indicator can sound a particular sound during cutting operations, a different sound during fusion or welding operations, and another distinct sound during coagulation operations to provide audible feedback to a user.

[0071] With reference to Figure 3C, a rearview of the electrosurgical unit 410 is illustrated. In the illustrated embodiment, the rear of the electrosurgical unit 410 includes a rear panel 430. The rear panel 430 can include various ports, such as a controller port 432 configured to be electrically coupled to an external controller such as a foot pedal controller, as described above with respect to Figure 1A. The rear panel 430 can also include a grounding lug. In other embodiments, one or more controller ports and/or the grounding lug can be located on another face of the electrosurgical unit 410, for example on the front face or a side face. The rear face of the electrosurgical unit 410 can include a power module 440 including a mains power port configured to be plugged into an AC power mains such as a wall socket and a master power switch for powering the electrosurgical unit 410 on and off. In other embodiments, the master power switch can be positioned on another face of the electrosurgical unit 410, for example on the front face or a side face. The rear phase of the electrosurgical unit 410 can also include a heat exchange feature, such as, for example slots, a grill, or a plurality of louvers 450. In other embodiments, the heat exchange feature can be positioned on another face of the electrosurgical unit 410, for example on the front face or a side face. The heat exchange feature can enhance air or other fluid cooling of the generator, the

feedback circuit, and other electrical components housed within the electrosurgical unit 410 console.

Electrosurgical Systems and Processes

[0072] Electrosurgical systems and processes in various embodiments apply monopolar or bipolar high-frequency electrical energy to a patient during surgery. Such systems and processes are particularly adapted for laparoscopic and endoscopic surgeries, where spatially limited access and visibility call for simple handling, and are used to fuse blood vessels and weld other biological tissue and in one aspect to cut, dissect and separate tissue/vessels. In particular embodiments, the systems and processes include the application of RF energy to mechanically compressed tissue to (a) desiccate the tissue, and (b) to denature collagens (type I-III) and other proteins, which are abundant in most biological tissue. As heating of collagens to an appropriate temperature causes them to unfold, shrink or denature, the system enables the sealing of capillaries and blood vessels during surgery for permanent occlusion of the vessels. As described in greater detail below, as an example, arteries up to seven millimeters can be occluded and dissected by radio frequency (RF) energy and mechanical pressure.

[0073] When concurrently applying controlled high-frequency electrical energy to the compressed tissue, the tissue is compressed with a relatively high pressure (about 10-20 kg/cm²), and the tissue is supplied with sufficient electrical energy to denature proteins and remove sufficient water in the tissue. During this process, the applied voltages are sufficiently reduced to avoid electrical arcing (typically < 200V RMS).

[0074] When applying electrical energy in the described manner stated above, the tissue quickly moves through the following fusion/welding process. Starting at body temperature the tissue (a) heats quickly, leading to (b) cell rupture, expelling of juices (mainly water and salt ions), (c) unraveling and "activation" of collagens and elastin in the blood vessels at about 60-650 C, and (d) desiccation of the vessel. Here, the desiccation process can be seen by the release of water in form of steam where the vessel temperature has reached about 1000 C. The reduction of water in presence of unraveled collagen and elastin strands leads to formation of bonds between collagen strands, leading to a strong and elastic seal of the tissue. As confirmed by measurements, the strongest (highest burst pressure) vessel fusions are obtained when the vessels have been heated to at least 70° C, pressurized with about 10-20 kg/cm², and then desiccated by about 40-50% of their original water content.

[0075] Electrically, the tissue can be characterized during the fusion process by its impedance, which is typically starting at 10-100 Ohms purely ohmic resistance. During the fusion process, the purely ohmic resistance reduces by 20-50% before it increases by two orders of

magnitude. As the resistance approaches a final value, the impedance of the tissue gradually increases in capacitive behavior with a phase shift of about 20 degrees. The tissue will exhibit a pronounced capacitive behavior at the end of the fusion process with a phase shift of about 40 degrees, even though the ohmic component will remain nearly unchanged during this phase.

[0076] As previously described and described throughout the application, the electrosurgical generator ultimately supplies RF energy to a connected electrosurgical tool. The electrosurgical generator ensures that the supplied RF energy does not exceed specified parameters and detects faults or error conditions. In various embodiments, however, an electrosurgical tool provides the commands or logic used to appropriately apply RF energy for a surgical procedure. An electrosurgical tool includes memory having commands and parameters that dictate the operation of the tool in conjunction with the electrosurgical generator. For example, in a simple case, the generator can supply the RF energy but the connected tool decides how much energy is applied. The generator however does not allow the supply of RF energy to exceed a set threshold even if directed to by the connected tool thereby providing a check or assurance against a faulty tool command.

[0077] In one embodiment, each tool comes with an integrated circuit that provides tool authentication, configuration, expiration, and logging. Connection of tools into the receptacles or ports initiates a tool verification and identification process. Tool authentication in one embodiment is provided via a challenge-response scheme and/or a stored secret key also shared by the controller. Other parameters have hash keys for integrity checks. Usages are logged to the controller and/or to the tool integrated circuit. Errors in one embodiment can result in unlogged usage. In one embodiment, the log record is set in binary and interpreted with offline tools or via the controller.

[0078] In one embodiment, connection of a standard bipolar tool into the standard bipolar outlet will not actively check the tool. However, the controller recognizes a connection so that the information on the bipolar outlet can be displayed on the monitor or user interface of the unit. The display reserves a field for the bipolar outlet before the outlet is activated. In one embodiment, the controller uses time measurement components to monitor a tool's expiration. Such components utilize polling oscillators or timers, real-time calendar clocks and are configured at boot time. Timer interrupts are handled by the controller and can be used by scripts for timeouts. Logging also utilizes timers or counters to timestamp logged events.

[0079] The tool in one embodiment has memory integrated with or removable from the tool. A tool algorithm or script within the tool's memory is loaded into a script interpreter of the generator. The script provides commands and parameters readying the tool for use when connected to the generator. Upon activation of a switch coupled to the tool, the controller detects the switch clo-

sure, and authenticates the tool, checks the tool's expiration status, and initializes internal data structures representing the receptacle's tool. A subsequent activation of the tool switch initiates an event that causes the script to direct the generator to supply RF energy. The controller logs the usage to both the tool and the generator. When the tool is disconnected from the receptacle of the generator, the controller resets the information associated with the receptacle. The controller constantly monitors the generator for proper operation. Unrecoverable errors and faults are announced and further operation of the system is prevented. All faults are stored in the controller's memory and/or the tool's memory.

[0080] Data from a specific procedure (e.g., from power-up to power-down) is stored on each tool. The tool additionally holds the data from a procedure, i.e., the number of tool uses, the power setting and faults. Each tool in one embodiment holds the information from all other tools as well. Tool memory includes but is not limited to the following parameters: serial number of generator, time stamp, tissue assessment and endpoint setting for each tool use, cut, coagulation, weld, power setting, duration of RF and endpoint (auto stop, fault, manual stop, etc.).

[0081] The generator logs usage details in an internal log that is down loadable. The generator has memory for storage of code and machine performance. The generator has reprogrammable memory that contains instructions for specific tool performance. The memory for example retains a serial number and tool use parameters. The generator stores information on the type of tools connected. Such information includes but is not limited to a tool identifier, e.g., a serial number of a connected tool, along with a time stamp, number of uses or duration of use of the connected tool, power setting of each and changes made to the default setting. The memory in one embodiment holds data for about two months or about 10,000 tool uses and is configured to overwrite itself as needed.

[0082] In one embodiment, the controller includes a state machine interpreter module that parses tool scripts. Tool scripts represent a tool process for a specific or given tool. The tool scripts are stored on memory connected to or integrated with a tool, the controller or a combination thereof. The state machine interpreter module responds to specific events, such as a switch activation/de-activation, tool positions or exceeding measurement thresholds. The module upon response controls the output of RF energy and/or electrode activation. In one embodiment, an interpreter module is provided for each tool input receptacle. The controller detects tool events and forwards the detected event to the appropriate interpreter module. The module in turn requests actions of the controller based on the detected event which provides output to the connected tool associated with the appropriate tool input receptacle and also the appropriate interpreter module.

[0083] In one embodiment, the controller has a specific

or predetermined fixed tool script for a specific input receptacle. As such, only this tool script is used for the tool connected to the particular input receptacle. The interpreter module includes an event detector and a script parser. The event detector receives and identifies tool events, such as a switch activation/de-activation event or a measurement event (e.g., phase threshold exceeded). The event detector formulates requests to the controller to control RF output, output selection and/or selection of outputs, changes to the display and audio tones. Other events detected include detecting hand and foot switches, jaw switches, phase over and phase under-after-over events, shorts and opens, tool script states. The script parser interprets the tool scripts. Keywords in the scripts assist the script parser to extract operational commands and data for tool operation based on a detected event identified by the event detector. In addition to the voltage, current, etc. set points, a tool script specifies the RF source as from the CUT or the COAG source. The script also specifies which electrodes get connected to RF+, RF-, or allowed to float. Because the script controls the electrode configuration, and can set thresholds that trigger events, a script can completely reconfigure tool during its use.

[0084] The script controls the voltage and current output settings as well as sequences of voltage and current settings. For example the permittivity and conductivity of blood vessels is the same independent of size. A small blood vessel will fuse very rapidly while a large vessel may take several seconds. Applying a large amount of current to a small vessel may cause excess tissue damage, while using a small amount of current will take an unacceptably long time to perform the fusion function. So to modify tool performance the script can initially command a small amount of RF current, and if fusion endpoint is not reached in less than one second, a high current is commanded to speed the fusion of a large vessel. Another script usage to modify tool performance to switch from one operation (coagulation) to another operation (cut) is to reconfigure the tool electrodes and ESG output to simplify a multistep process such as fuse and cut. When the clinician starts the process the script will first setup the unit for the fusion, measure the tissue phase angle that indicates the fusion endpoint. RF power is then turned on until the fusion endpoint is reached. The unit will then turn off RF power and beep to indicate that fusion is complete. The unit then switches the electrodes to the cut configuration, sets the RF output for cut, and restarts the RF output. The cut operation is stopped by the clinician when the cut is completed.

[0085] Referring to Figure 4, an overview of tool operations is provided. A tool connected to the electrosurgical generator is verified 601. The endpoint is determined 602. The tool applies energy 603, e.g., RF energy, and continues until an endpoint is reached or an error condition is detected. Upon determination of an endpoint being reached or exceeded 604, the tool is deactivated (e.g., application of energy is stopped) ending the process.

[0086] Based on the tool algorithm for the connected tool, the tool verification and determination of an end point can vary. In particular, a tool short is determined by measuring resistance at a tissue contacting surface of the tool. If the resistance is less than ten (10) Ohms, a tool short condition is recognized. In accordance with various embodiments, the product of measured tissue permittivity and conductivity or an initial phase shift is utilized to determine the end point for a connected tool.

[0087] In accordance with various embodiments, phase shift and/or a phase rate of change is measured throughout the process to determine if an endpoint is reached or exceeded. Also, timeout parameters, e.g., a timer or counter reaching or exceeding a set time limit, or a fault condition stops or interrupts the process even if the determined end point is not reached or exceeded.

Handheld Electrosurgical Tools

[0088] As described generally above and described in further detail below, various handheld electrosurgical tools can be used in the electrosurgical systems described herein. For example, electrosurgical graspers, scissors, tweezers, probes, needles, and other instruments incorporating one, some, or all of the aspects discussed herein can provide various advantages in an electrosurgical system. Various embodiments electrosurgical tool are discussed below. It is contemplated that one, some, or all of the features discussed generally below can be included in any of the embodiment of tool discussed below. For example, it can be desirable that each of the tools described below include a memory for interaction with a feedback circuit as described above. However, in other embodiments, the tools described below can be configured to interact with a standard bipolar power source without interaction of a tool memory. Furthermore, although it is contemplated that certain aspects of these embodiments can be combined with certain aspects of other electrosurgical tools within the scope of this application. Certain aspects of these electrosurgical tools are discussed generally herein, and in more detail with respect to various embodiments below.

[0089] As discussed above with respect to Figures 1A and 1B, and electrosurgical tool can desirably include a memory. The memory can include an encryption module and a configuration device module. The configuration device module can store certain types of tool data. For example the configuration device module can store operational parameters for the tool, including software to be transferred to an electrosurgical unit upon successful electrical connection to the electrosurgical unit. These operational parameters can include data regarding various electrosurgical procedures to be performed by the tool and corresponding energy level ranges and durations for these operations, data regarding electrode configuration of a tool, and data regarding switching between electrodes to perform different electrosurgical procedures with the tool. Advantageously, unlike prior art elec-

trosurgical systems, changes to tool profiles and periodic tool updates can be rapidly made without downtime to electrosurgical generators, as the software for tool operation can reside in electrosurgical tool itself, rather than the generator. Accordingly, updates can be made during tool production.

[0090] The configuration device module can further store a data log comprising, for example, a record of information of each previous tool use. For example, in some embodiments, the data log can contain timestamp data including an electrosurgical unit identifier, a log of electrosurgical procedures performed by the tool, and a log of durations and energies applied to the tool. In some embodiments, it can be desirable that use of a particular tool is limited to a maximum usage period or number of procedures, especially where electrosurgical tool has not been configured for sterilization and reuse. Accordingly, in some embodiments, the configuration device module can be configured to prevent operation of a tool after a predetermined usage or number of procedures. In some embodiments, a tool can comprise a mechanical lockout in addition to or in place of the data log, such as a break-away single-use connector to reduce the possibility of unintended reuse.

[0091] In some embodiments, it is desirable that the tool communicate with the electrosurgical unit through an encrypted protocol. Accordingly, the memory can further store an encryption module, or encryption key to facilitate this encrypted communication.

[0092] As discussed above with respect to figures 18 and one be, it can be desirable that an electrosurgical tool for use in the electrosurgical system includes one or more audio and/or visual indicators. In some embodiments, the electrosurgical tool can include an array of LEDs, or a multi-color LED assembly such as a three-color LED assembly capable of generating many combined colors. The visual indicator can be configured to illuminate with a color corresponding to the type of electrosurgical procedure performed by the tool. Were a tool is configured to perform multiple different types of electrosurgical procedures, desirably the visual indicator updates to reflect the currently-selected electrosurgical procedure. Thus, advantageously, a user can tell, while watching the surgical field, what type of electrosurgical procedure the tool is configured to perform.

Electrosurgical Fusion Tool

[0093] With reference to Figures 5A-5B, one embodiment of a hand held laparoscopic sealer/divider or fusion tool 1100 is provided. In the illustrated embodiment, the sealer/divider comprises a handle assembly 1110, an elongate shaft 1120 extending from the handle assembly 1110, and a jaw assembly 1130 positioned on the elongate shaft 1120 opposite the handle assembly 1110. The elongate shaft 1120 has a proximal end and a distal end defining a central longitudinal axis therebetween. In the illustrated embodiment, the handle assembly 1110 com-

prises a pistol-grip like handle. The elongate shaft 1120 and the jaw assembly 1130, in one embodiment, are sized and shaped to fit through a 5mm diameter trocar cannula or access port. In other embodiments, the elongate shaft and jaw assembly can be sized and configured to fit through trocar cannulae or access ports having other standard, or non-standard sizes. In Figure 5A, the handle assembly 1110 is shown in a first or initial position in which the jaws are open.

[0094] With reference to Figures 5A-6C, the handle assembly 1110 comprises a stationary handle 1112 and an actuation handle 1114 movably coupled to the stationary handle. In the illustrated embodiment, the stationary handle 1112 comprises a housing formed of right 1112R and left handle 1112L frames. In other embodiments, the stationary handle 1112 can be a single component, or can be a housing formed of more than two pieces. In the illustrated embodiment, the actuation handle 1114 is slidably and pivotally coupled to the stationary housing, as discussed in further detail below. In operation, the actuation handle 1114 can be manipulated by a user, e.g., a surgeon to actuate the jaw assembly, for example, selectively opening and closing the jaws.

[0095] With continued reference to Figures 6A-6B, in the illustrated embodiment, the actuation handle 1114 is coupled to the stationary handle 1112 to form a force regulation mechanism 1200 coupling the handle assembly 1110 to the jaw assembly 1130. Desirably, the force regulation mechanism 1200 can be configured such that in a closed configuration, the jaw assembly 1130 delivers a gripping force between the first jaw 1132 and the second jaw 1134 between a predetermined minimum force and a predetermined maximum force.

[0096] With continued reference to Figures 6A-6B, in the illustrated embodiment, the actuation handle 1114 is coupled to the stationary handle 1112 at two sliding pivot locations 1202, 1204 to form the force regulation mechanism 1200. The actuation handle 1114 has a first end 1116 including a gripping surface formed thereon, and a second end 1118 opposite the first end 1116. In the illustrated embodiment, the actuation handle 1114 is coupled to a pin 1206 adjacent the second end 1118. In some embodiments, the actuation handle 1114 can be integrally formed with a protrusion extending therefrom defining a pin surface, while in other embodiments, a pin can be press-fit into an aperture in the actuation handle. The 1206 pin can be contained within slots in the stationary handle 1112, such as corresponding slots formed in the right and left handle frames 1112R, 1112L of the stationary handle housing. These slots can allow the sliding pin 1206 to move over a predetermined range. In some embodiments, the slots can be configured to define a desired actuation handle path as the actuation handle is moved from the first position corresponding to open jaws to a second position corresponding to closed jaws. For example, the illustrated embodiment includes generally linear slots formed in the stationary handle 1112 at an angle from the central longitudinal axis of the elongate shaft

1120. In other embodiments, the slots can be formed generally parallel to the central longitudinal axis. In some embodiments, the slots can be curvilinear.

[0097] In the illustrated embodiment, the force regulation mechanism 1200 includes a biasing member such as a trigger spring 1208 that biases the pin in a proximal direction towards the rear of the pin slots in the right and left handle frames (see, for example, Figure 6B). The trigger spring 1208 and the actuation handle 1114 can pivot freely or unhindered at their attachment point 1202. The biasing member 1208 can be preloaded to a predetermined force. In operation, as a predetermined force is exerted on the actuation handle 1114, a biasing force exerted by the trigger spring 1208 is overcome, and the second end 1118 of the actuation handle 1114 can translate generally distally, guided by the pin in the slots.

[0098] While the illustrated embodiment includes a pin-in-slot arrangement coupling one pivot point of the actuation handle to the stationary handle, in other embodiments, it is contemplated that other connections can be formed. For example, in some embodiments, a slot can be formed in the actuation handle and a mating projection can be formed in the stationary handle. Furthermore, while the illustrated embodiment includes a tension coil spring forming the biasing member, in other embodiments, other biasing members are contemplated. For example, the biasing member can comprise a compression spring, a torsion spring, an elastomeric band, a fluid-filled shock absorbing unit, or another suitable biasing device.

[0099] With continued reference to Figures 6A-6B, in the illustrated embodiment, the actuation handle 1114 is slidably and pivotably coupled to the stationary handle 1112 at a location between the first and second ends 1116, 1118 of the actuation handle. An actuation member such as a pull block 1250 can be coupled to the actuation handle. In the illustrated embodiment, an actuation path of the pull block 1250 is defined by rails formed in the right and left handle frames 1112L, 1112R. When the actuation handle 1114 is moved proximally, the pull block 1250 also moves, effectively closing the jaws thereby clamping any tissue between the jaws. In the illustrated embodiment, the rails guide the pull block 1250 to slide proximally and distally while limiting movement in other directions. In other embodiments, various other guide members such as a pin-in-slot arrangement can define the actuation path of the actuation member.

[0100] As illustrated, the pull block 1250 comprises a generally rectangular prismatic structure having a generally open top and bottom faces and a substantially closed proximal end. The actuation handle 1114 can extend through the top and bottom faces of the pull block 1250. An edge of the actuation handle 1114 can bear on the proximal end of the pull block 1250 such that movement of the actuation handle 1114 relative to the stationary handle can move the pull block 1250 generally longitudinally along the actuation path defined by the rails. A distal end of the pull block 1250 can be coupled with

an actuation shaft such as an actuation tube, bar, or rod, which can extend longitudinally along the elongate shaft of the sealer/divider. Thus, in operation, movement of the actuation handle 1114 from the first position to the second position translates the pull block 1250 longitudinally within the stationary housing, which correspondingly translates the actuation rod generally linearly along the longitudinal axis with respect to the elongate shaft. Movement of this actuation tube can control relative movement of the jaws in the jaw assembly.

[0101] With continued reference to Figures 6A and 6B, in some embodiments, the sealer/divider can include a latch mechanism 1260 to maintain the actuation handle 1114 in the second position with respect to the stationary handle. In the illustrated embodiment, the actuation trigger comprises an extended latch arm 1262 which can engage a matching latch 1264 contained within actuation handle 1112 for holding the actuation trigger at a second or closed position. In other embodiments, it is contemplated that the one portion of the latch mechanism can be formed on a portion of the actuation handle 1114 adjacent the second end of the actuation handle 1114, and a mating portion of the latch mechanism can be formed on the actuation handle 1112. In still other embodiments, it is contemplated that the a portion of the latch mechanism can be formed on the pull block 1250 and a mating portion of the latch mechanism can be formed on the stationary housing.

[0102] In some embodiments, the jaw assembly 1130 of the sealer/divider comprises an advanceable cutting blade 1400 (Figure 8B) that can be coupled to a blade actuator such as a blade trigger 1402 positioned on the handle assembly 1110. A blade actuation mechanism 1404 can operatively couple the blade trigger to the cutting blade. In the illustrated embodiment, the blade trigger 1402 is positioned on a proximal surface of the handle assembly such that it can be easily operated in a pistol-grip fashion. As illustrated, the blade actuation mechanism 1404 comprises a pivoting blade advancement link that transfers and reverses the proximal motion of the blade trigger 1402 to a blade actuation shaft assembly coupled to the cutting blade. In other embodiments, the blade trigger 1402 can be positioned elsewhere on the actuation handle 1112 such as on a distal surface of the actuation handle 1112 such that distal movement of the blade trigger 1402 can advance the cutting blade distally without transfer of advancement directions via a linkage. In operation, a user can move the blade trigger 1402 proximally to advance the cutting blade 1400 from a retracted position to an extended position. The blade actuation mechanism 1404 can include a biasing member such as a blade return spring 1406 to biases the blade advancement lever distally within the actuator and thereby bias the cutting blade 1400 into the retracted position.

[0103] With reference to Figure 6C, the handle assembly also comprises a wire harness 1500. The wire harness 1500, in certain embodiments, comprises six insulated individual electrical wires or leads contained within

a single sheath. As illustrated, the wire harness 1500 can exit the housing of the actuation handle 1112 at a lower surface thereof and can run generally upwards along the interior of the actuation handle 1112. In other embodiments, other wire routings can be made. For example, in some embodiments, the wire harness 1500 can exit a lower portion of the proximal surface of the actuation handle 1112. The wires within the harness can provide electrical communication between the sealer/divider and an electrosurgical generator and/or accessories thereof, as discussed above.

[0104] In certain embodiments of sealer/divider, inside the actuation handle 1112, two of the leads are attached to rotational coupling clips 1502 configured to allow infinite rotation of the jaw assembly 1130, as discussed in greater detail below, two of the other leads are attached to a visible indicator 1504, such as a multi-colored LED, and the remaining two leads are attached to a switch 1506. In some embodiments, the switch 1506 is connected to a user manipulated activation button and is activated when the activation button is depressed. In one aspect, once activated, the switch 1506 completes a circuit by electrically coupling the two leads together. As such, an electrical path is then established from an electrosurgical generator to the actuator to supply radio frequency power to one of the two leads attached to the rotational coupling clips 1502.

[0105] Referring now to Figure 7, the handle assembly is coupled to a rotational shaft assembly 1600. In certain embodiments, coupling of the handle assembly to the rotational shaft assembly 1600 is configured to allow infinite 360 degree rotation of the jaw assembly 1130 with respect to the handle assembly. In the illustrated embodiment, the handle assembly 1110 connects to the shaft 1120 at five locations or connections providing a continuous 360 degree rotation of the entire shaft while simultaneously allowing complete actuation of the actuation handle 1114, e.g., sealing and/or dividing of the vessel. As illustrated, the first two connections are rotational coupling clips 1502 which make contact with the rotational shaft assembly at the actuation tube and conductive sleeve. The next area of engagement or the third connection is a rotational hub assembly 1602 which is located between the two rotational coupling clips 1502.

[0106] With continued reference to Figure 7, the rotational shaft assembly 1600 is desirably contained within the right and left handle frames such that proximal and distal movement of the jaw assembly 1130 with respect to the handle assembly 1110 is prevented while allowing for rotational movement. For example, inwardly-extending flanges can be formed on the actuation handle 1112 that interfere with proximal and distal movement of the rotational hub assembly 1602, rotational coupling clips 1502, or other components of the rotational shaft assembly 1600. The fourth connection is at a plurality of threaded nuts 1604 and the pull block 1250. The fifth connection is between the blade lever 1608 and a rear blade shaft 1606. The rotation shaft assembly 1600 can also com-

prises a rotation knob 1610 which is fixed to the outer cover tube. The rotation knob 1610 allows the surgeon to rotate the shaft of the device while gripping the handle. While the rotational shaft assembly 1600 is illustrated as having five connection locations with the actuation handle 1112, in some embodiments, a rotational shaft assembly can have fewer connection locations, such as for example, 1, 2, 3, or 4 connection locations. In still other embodiments, it can be desirable that a rotational shaft assembly has more than 5 connection locations, such as, for example 6, 7, 8, or more than 8 connection locations.

[0107] Desirably, the rotational shaft assembly 1600 provides the vessel sealer/divider with continuous 360 degree rotation throughout operation of the electrosurgical instrument. By using rotational coupling clips 1502 for the electrical connections to the shaft, the shaft can operate, e.g., deliver RF energy, at any orientation or rotation of the jaw assembly 1130 relative to the handle assembly. Thus, advantageously, the surgeon is provided more surgical options for the placement and activation of the sealer/divider. Advantageously, with a rotational shaft assembly 1600, the wires and electrical and mechanical connections, as such, do not interfere with continuous, infinite rotation of the shaft. To maintain a bipolar connection through the rotational shaft assembly 1600, one of the electrical connections is electrically isolated from other conductive portions of the shaft.

[0108] As discussed in further detail below, in some embodiments, the sealer/divider can be configured to grasp with a gripping force within a predetermined range. In one embodiment, an overall tolerance stack-up over the length of the shaft can be controlled so that the force applied to the jaw assembly 1130 from the handle assembly can be maintained accurately within the predetermined range. The overall length of the shaft 1120 can be controlled by using threaded nuts 1604 and a threaded coupling. The threaded nuts 1604 can be adjusted to tightly control the length of the elongate shaft 1120. The length is controlled by maintaining the location of the threaded nuts 1604 in relation to the hub portions of the shaft. In the illustrated embodiment, attached to the distal end of the actuation tube is a threaded coupling. Attached to the threaded coupling are two threaded nuts, which are configured to engage with the pull block 1250. The pull block 1250 engages with the threaded nuts 1604 which are attached to the rear of the actuation tube, causing the actuation tube to move proximally. The described interaction can also be reversed so that the threaded nuts 1604 and coupling are attached to an outer cover tube rather than the actuation tube. In other embodiments, other length adjustment mechanisms can be used to control the overall tolerance stack-up such as a lock screw to selectively secure the position of the pull block 1250 at a desired location relative to the actuation tube or toothed ratchet interfaces defining set distance relationships between the pull block and the actuation tube. In other embodiments, a length adjustment mechanism can

be positioned at the distal end of the elongate shaft, e.g., where the elongate shaft interfaces with the jaw assembly 1130.

[0109] Referring to Figures 8A-8D, the elongate shaft 1120 can comprise a plurality of actuation members extending therethrough. In the illustrated embodiment, the elongate shaft comprises an actuation tube 1122 coupling the jaw assembly 1130 with the handle assembly 1110 and a blade actuation shaft assembly 1124 coupling the blade trigger 1402 with the cutting blade. In some embodiments, the blade actuation shaft assembly 1124 comprises a two-piece shaft having a proximal portion and a distal portion. The proximal portion of the blade shaft assembly can terminate at a proximal end at an interface node 1126. In the illustrated embodiment, the interface node 1126 comprises a generally spherical protrusion portion which is adapted to engage the blade advancing lever. In other embodiments, the interface node can comprise other geometries such as cubic or rectangular prismatic protrusions. In the illustrated embodiment, the proximal portion of the blade shaft is operatively coupled to the distal portion of the blade shaft assembly 1124. The distal portion of the blade shaft can comprise a mount at its distal end for attachment of the cutting blade. In the illustrated embodiment, the mount comprises at least one heat stake post. In certain embodiments, both the proximal and distal portions of the blade shaft are at least partially positioned within a generally tubular section of the actuation tube 1122. (see, e.g., Figure 8C).

[0110] As discussed above with respect to length adjustment of the elongate shaft 1120, in the illustrated embodiment attached to the distal end of the actuation tube 1122 is a threaded coupling 1150 (Figure 8D). As illustrated, attached to the threaded coupling 1150 are two thread nuts 1604, which are configured to engage with the pull block 1250. In the illustrated embodiment, the actuation tube 1122 is housed within an outer cover tube. While the actuation tube 1122 is illustrated as a generally tubular member that can be nested within the outer cover tube 1126, and that can have a blade actuation shaft 1124 nested within it, in other embodiments, a non-tubular actuation member can be used, for example, a shaft, a rigid band, or a link, which, in certain embodiments can be positioned generally parallel to the blade actuation shaft within the outer cover tube.

[0111] With continued reference to Figure 8A, in the illustrated embodiment, attached to the distal end of the outer cover tube 1126 is the rotational shaft assembly 1600. The rotational shaft assembly 1600 comprises two mating hubs 1602 and a conductive sleeve 1610. In the illustrated embodiment, the hubs 1602 snap together, engaging with the outer cover tube. In other embodiments, the hubs can be of a monolithic construction and configured to interface with mating features on the outer cover tube. The conductive sleeve 1610 can be attached to the proximal portion of the assembled hubs after they are attached to the outer cover tube. When the conductive sleeve 1610 is attached to the rear of the assembled

hubs 1602, the sleeve 1610 traps the exposed end of an isolated wire 1612 (see Figure 8D). In the illustrated embodiment, the isolated wire 1612 extends from its entrapment point under the conductive sleeve through a slot in the actuation tube 1122 and then inside a protective sleeve 1614. The protective sleeve 1614 and isolated wire 1612 extend distally inside the actuation tube 1122, towards the jaw assembly 1130. In other embodiments, the isolated wire can be formed integrally with a protective sheath and no separate protective sleeve is present in the actuation tube.

[0112] With reference to Figures 9A-9C, attached to the distal end of the elongate shaft 1120 is the jaw assembly 1130. In certain embodiments, the jaw assembly 1130 comprises a lower jaw 1134, upper jaw 1132, upper conductive assembly 1142, lower nonconductive spacer 1144, and jaw pivot pin 1146. In the illustrated embodiments, the jaw pivot pin 1146 pivotally couples the upper and lower jaws 1132, 1134 and allows the upper jaw 1132 to pivot relative to the lower jaw 1134. In other embodiments, other pivotal couplings are contemplated. As illustrated, the proximal portion of the upper jaw 1132 extends through the lower jaw 1134 and into a hole in the actuation tube 1122.

[0113] In some embodiments, one jaw can be fixed with respect to the elongate shaft 1120 such that the opposing jaw pivots with respect to the fixed jaw between an open and a closed position. For example, in the illustrated embodiment, the proximal portion of the lower jaw 1134 extends inside the cover tube 1126 and is crimped in place, fixing the jaw assembly 1130 to the rotation shaft assembly 1600. Thus, in the illustrated embodiment, the upper jaw 1132 is moveable with respect to a fixed lower jaw 1134. In other embodiments, both jaws can be pivotally coupled to the elongate shaft such that both jaws can pivot with respect to each other.

[0114] Attached to the upper jaw 1132 is the upper conductive assembly 1142, which comprises a nonconductive portion 1702 and a conductive pad 1704 (see Figure 9B). The nonconductive portion 1702 isolates the conductive pad 1704 from the upper jaw 1132, likewise isolating it from the rest of the shaft assembly 1120. The isolated wire 1612 can be routed to electrically couple the conductive pad 1704 on the upper jaw 1132 to the wiring harness 1500 in the handle assembly 1110. In the illustrated embodiment, the isolated wire 1612 extends from the distal end of the protective sleeve which is housed at the proximal end of the lower jaw and extends into the upper jaw 1132. The upper jaw 1132 can have a slot positioned to receive the isolated wire. The isolated wire 1612 then extends through a hole in the upper jaw 1132 and drops into a slot in the nonconductive portion. The isolated wire then extends to the distal end of the nonconductive portion and drops through to the conductive pad (see Figure 8D).

[0115] The jaw assembly 1130 can include one or more nonconductive space maintaining members such as spacers 1144 to reduce the risk that electrodes on the

upper jaw 1132 and lower jaw 1134 can come into direct contact and create a short. In the illustrated embodiment, the lower nonconductive spacer 1144 is housed inside the u-groove portion of the lower jaw and contains space maintaining protrusions which prevent the conductive pad from contacting the lower jaw (see Figure 9C).

[0116] Turning now to some of the operational aspects of the electrosurgical instruments described herein, once a vessel 1030 or tissue bundle has been identified for sealing, the upper and lower jaws are placed around the tissue (see Figure 10A). The actuation handle 1114 is squeezed moving the actuation handle 1114 proximally with respect to the actuation handle 1112 (see Figure 10B). As the actuation handle 1114 moves proximally it pushes the pull block 1250 along the rails in the right and left handle frames. The pull block 1250 engages with the threaded nuts 1604 which are attached to the rear of the actuation tube 1122, causing the actuation tube 1122 to move proximally. Proximal movement of the actuation tube pivots the upper jaw 1132, coupled to the pull tube, towards the lower jaw, effectively clamping the tissue (see Figure 10C). The force applied to the tissue by the upper jaw is translated through the pull tube and pull block 1250 to the actuation handle 1114. Once the preloaded force has been overcome, the actuation handle 1114 will begin to move the sliding pin 1206 distally (see Figure 10D). When the preload on the trigger spring has been overcome, the actuation handle 1114 pivot point shifts from the sliding pin 1206 to the rear portion of the pull block 1250 where it contacts the actuation trigger. The sliding pin 1206 can advance distally because the preloaded force on the trigger spring 1208 has been overcome.

[0117] The continued manipulation of the actuation handle 1114 pivots the actuation handle 1114 to a location where the actuation handle 1114 engages with the latch mechanism 1260 in the right and left handle frames that maintains the trigger in the engaged position and prevents the trigger from returning to an opened position. When the engaged position is reached and nothing is present between the upper and lower jaws 1132, 1134, the trigger spring is extended to a distance that ensures that the force applied to the electrodes of the jaw assembly 1130 is near the lower end of the force range required for optimal vessel sealing. When a large, e.g., maximum, amount of tissue is placed in the jaws, the actuation handle 1114 extends the trigger spring 1208 a greater distance. However, the trigger spring 1208 ensures that the maximum amount of force applied does not exceed the maximum end of the force range used for optimal vessel sealing. From the engaged position, sealing radio frequency energy is applied to the tissue by depressing the power activation button. Once the tissue has been sealed, the actuation trigger can be reopened by continuing proximal advancement to a position that allows the actuation trigger's finger portion to disengage from the latch portions of the left and right handle frames. (See Figures 10A-10F))

[0118] The floating dual pivoting mechanism including a sliding pin 1206 and a pull block 1250 described above desirably provides a minimum force, optimal for sealing vessels and tissue, is maintained regardless of the amount of substance contained between the upper and lower jaws. This mechanism also reduces the risk that an extremely large amount of force is applied to the tissue. If too much force is applied to a vessel or tissue bundle, potential damage could occur. Thus, if a very small vessel or thin tissue bundle is clamped within the jaw, the instrument applies the minimum amount of force required to obtain a good tissue weld. The same is true with a very large vessel or tissue bundle. Since the travel of the jaw can vary greatly depending on tissue thickness, the force applied by the jaw is adjustable. It is desired that the instrument be self-adjusting and automatic (no action from the user). The floating dual pivot mechanism described below provides the self-adjustment, applying a specific range of force along the length of the electrode.

[0119] Once the actuation handle 1114 has been depressed to a predetermined force range for optimal vessel sealing, it will engage the matching latch of the right and left handle frames, locking the actuation trigger from moving further distally (See Figure 10E). At this point the user can depress the activation button, applying the appropriate energy to the tissue for proper sealing.

[0120] Once the tissue has been sealed, the user can actuate the blade trigger 1402. When the blade trigger 1402 is moved proximally, the blade lever pivots, forcing the front and rear blade shafts and cutting blade 1400 to move distally. The cutting blade advances forward and divides the sealed portion of the tissue (see Figure 10F). When the user releases the blade trigger 1402, the blade spring resets the cutting blade to its original position. When the blade trigger 1402 has been returned to its original or initial position the user can continue to squeeze the actuation handle 1114 to open the upper jaw. Continued proximal movement of the actuation handle 1114 will disengage the actuation handle 1114 from the latch mechanism 1260 of the right and left handle frames by biasing the extended arm portion 1262 of the actuation trigger upwards, over the end of the latch, to a position where the trigger can be released (see Figure 10G).

[0121] The electrosurgical instrument is connectable to an electrosurgical generator specifically configured to apply the proper amount of energy to the tissue when the activation button is depressed, such as the electrosurgical generator described above. With reference to Figure 11, the instrument is also connectable to an intermediate control unit 1800 in conjunction with an electrosurgical generator. The intermediate control unit 1800 can monitor the tissue sealing and ensure that the proper amount of sealing energy is applied to the tissue. The control unit 1800 in one aspect can have a set of cables configured to plug into most typical electrosurgical generators. The control unit also has a port for connecting the wiring harness 1500 plug from the instrument (see Figure 11).

[0122] With continued reference to Figure 11, in certain embodiments, the non-sterile power controller interfaces with the sterile vessel sealer/divider through a cord extending from the sealer/divider beyond the sterile field and plugged into the controller. In one aspect, the controller regulates and/or distributes power from a non-sterile reusable power supply to which the controller is attached or integrated. In some embodiments, the controller can be configured for a single use to maintain sterility of the surgical environment. In order to prevent reuse of the non-reusable controller, the cord of the electrosurgical tool, once plugged into the non-sterile controller cannot be removed. This connection permanently couples the sterile and non-sterile portions, preventing the user from being able to disconnect the controller for reuse in unintended surgical procedures or purposes. (see Figure 11)

[0123] In grasping jaw assemblies such as the jaw assembly 1130 of the electrosurgical tool, the gripping force generated between the jaws can vary along the length of the jaws from a relative maximum F_{max} near the proximal end to a relative minimum F_{min} near the distal end. In some embodiments, the electrosurgical tool can be configured such that the forces are optimized along the length of the active electrode portions of the jaws, a predetermined force range for vessel sealing is maintained. A predetermined maximum amount of force utilized to obtain a proper vessel seal is desirably not exceeded at the proximal end of the active electrodes (closest to the pivot). In addition a gripping force at the distal most ends of the active electrodes is desirably greater than a predetermined minimum amount of force for optimal vessel sealing. Desirably, the gripping force generated at every point along the jaw assembly 1130 is within the range defined by the predetermined maximum force and the predetermined minimum force to achieve optimal sealing. (See Figure 12A).

[0124] In some embodiments, the electrode width to form vessel seals is between about 0.25 mm and about 1.5 mm. In other embodiments, the electrode width is desirably between about 0.4 mm and about 1 mm. In other embodiments, the electrode width is preferably between about 0.6 mm and 0.8 mm. In some embodiments, the electrode width is approximately 0.75 mm. With an electrode of 0.75 mm, and the sufficient pressure for this type of electrode to achieve a vessel seal is approximately 3 pounds (see Figures 12B and 12C). However it can be seen from Figure 12C that a force range of approximately 0.4 pound to 2.3 kg on a 0.75 mm electrode can maintain burst pressures greater than 15 psi. In some embodiments, the jaw and electrode arrangement desirably can maintain a pressure of between 3 and 39 kg/cm², more desirably 10-30 kg/cm², and preferably approximately 23 kg/cm². Embodiments having different electrode widths can have different force ranges. In order to maximize sealing surface area while still maintaining the electrode configuration described above, in some embodiments, multiple rows of 0.75 mm electrodes

may be provided (see Figure 12C).

[0125] In some embodiments, electrode geometry on the conductive pads of the jaw assembly 1130 ensures that the sealing area completely encloses the distal portion of the blade cutting path. Single linear electrodes could cause vessel leakage when only a portion of a vessel is sealed. In one embodiment, the electrodes positioned on the jaw assembly 1130 comprise a single u-shaped electrode 1902 surface on each of the upper and lower jaws. Each u-shaped electrode can comprise generally parallel linear legs 1910 extending from a proximal end of the conductive pad of the jaw towards the distal end and a curved connector 1912 at the distal end extending from one leg to the opposite leg. Desirably, the u-shaped electrodes can completely encompass the distal end of the blade cutting path. In other embodiments, to provide a greater sealing area, two or more spaced u-shaped electrode surfaces on both the upper and lower jaws can be provided (see Figure 13). In some embodiments, the electrodes 1904 can be connected at the distal ends to create a completely enclosed seal (see Figure 13). In certain embodiments one or multiple bridge members 1908 between the u-shaped electrode 1906 surfaces can further ensure that the sealing area completely encloses the distal portion of the blade cutting path.

[0126] In some embodiments, for some surgical procedures the outer shape of the jaws 1130' can be curved such that the distal ends of the jaws are offset with respect to the longitudinal axis from the proximal ends of the jaws to improve visibility for a user such as a surgeon. In embodiments with curved jaws, the u-shaped electrodes can also be provided in a curved fashion while still maintaining proper electrode width and spacing (see Figure 14).

[0127] With reference to Figure 15, in certain embodiments, the electrosurgical device can include a tissue dissector formed on the jaw assembly 1130". Advantageously, this integrated tissue dissector can facilitate dissection of non-vascular tissue either bluntly or electrosurgically, without having to exchange the vessel sealer/divider with another instrument. Thus, this multiple tool functionality can advantageously facilitate quicker surgical procedures. The reduced number of tool exchanges can be especially advantageous in laparoscopic procedures or procedures with relatively limited access as tool exchanges can be time consuming in these surgical environments.

[0128] With continued reference to Figure 15, in some embodiments, one of the jaws of the jaw assembly 1130" can have an extended distal end distally beyond the distal end of the other jaw (see Figure 15). In the illustrated embodiment, the lower jaw 1134" can have an extended distal end. Advantageously, in embodiments where the lower jaw 1134" is pivotally fixed to the elongate shaft, this extended arrangement can facilitate stability of the lower jaw during dissection. In other embodiments, the upper jaw 1132 can have an extended distal end, allowing the tissue dissector to be pivoted during the dissection operation by movement of the actuation

handle 1114. In some embodiments, the extended distal end can be tapered in shape such that the distal end is relatively short and narrow compared to relatively more proximal portions of the jaw. Advantageously, this tapered shape allows the distal end to access tissue positioned in relatively confined environments while reducing the risk that adjacent tissue is contacted.

[0129] With reference to Figures 16-1 and 16-2, In some embodiments, both jaws of the jaw assembly 1130" are tapered laterally and/or in height along the length of the jaw's electrode portions, or at least part of the electrode portions. In these embodiments, the jaw assembly 1130" has a low-profile distal end which can be used for tissue dissection. Advantageously, the low-profile distal end can also enhance access of the jaw assembly 1130" to relatively confined surgical environments.

[0130] With reference to Figures 17A and 17B, in certain embodiments, a cutting/coagulating electrode can be disposed on an exterior surface of the jaw assembly 1130 to provide tissue dissection. In some embodiments, the cut/coagulation electrode is located on the jaw at, for example, the distal end on the outer surface of either the upper or lower jaw (see Figure 17A). Desirably, the electrode 1920 can be electrically isolated or insulated from other components of the jaw assembly 1130, providing an active electrode for the bi-polar instrument. As such, an isolated wire can extend from the cut/coagulation electrode 1920 to the proximal end of the elongate shaft 1120 (similar to the isolated wire extending from the conductive pad on the upper jaw) to electrically couple the cut/coagulation electrode to the wiring harness 1500 of the electrosurgical tool in the handle assembly. In some embodiments, the isolated wire can extend within a protective sleeve within the outer cover tube of the elongate shaft. In other embodiments, the isolated wire can be integrally formed with a protective sheath. The isolated wire also in one aspect is coupled to a rotational connection, e.g., a rotational clip, similar to the isolated wire extending for the conductive pad.

[0131] With reference to Figure 17B, the cut/coagulation electrode in one aspect can be selectively activated by at least one actuation button 1922, 1924 or switch on the handle assembly 1110. In some embodiments, the handle assembly can comprise a cut button 1922 to actuate the electrode with a tissue cutting electrosurgical signal and a coagulation button 1924 to actuate the electrode with a tissue coagulating electrosurgical signal. For example, in Figure 17B, separate cut and coagulation buttons are illustrated on the actuator adjacent a tissue sealing button to actuate the electrodes on inner surfaces of the jaws. In other embodiments, a single, multifunction switch or button can actuate the cut/coagulation electrode in the desired configuration. In still other embodiments, the cut/coagulation electrode can be configured to receive only a cutting or only a coagulation electrosurgical signal, and a single corresponding actuation button or switch can be used to selectively actuate the electrode.

[0132] The vessel sealer/divider can use thin metallic tubes and small diameter machined rods for the internal elongated components used to actuate jaws such as the actuation tube and the blade actuation shaft. However, such components can be costly and in some embodiments, manufacturing and materials costs can be desirably reduced through the use of elongate injection molded plastic components. As discussed above with respect to the blade actuation shaft 1124, in some embodiments, costs and manufacturing difficulties can be reduced further through the use of an elongated shaft formed of two mating polymer shaft sections 1124a, 1124b such as a proximal or rear shaft portion and a distal or front shaft portion. In some embodiments, the two shaft portions 1124a, 1124b can be connected by interlocks 1960, e.g., projections on one shaft section or component mating with corresponding slots on the other shaft section, to maintain concentricity and prevent unnecessary movement in their axial direction (see Figure 18-1, 18-2 and 18-3). In other embodiments, other mating structures can be formed on the two mating shaft portions. For example, one of the shaft portions can be formed with one or more barbs thereon and the other shaft portion can be formed with a recess configured to receive and retain the barbs. In still other embodiments, the two mating shaft portions can be adhered with a chemical adhesive or epoxy, either in addition to, or in place of interlocks formed on the shaft portions.

[0133] With reference to Figures 19-1 and 19-2, in certain embodiments, the elongate shaft 1120 of the electrosurgical tool can be configured such that the outer surface thereof does not translate proximally and distally during actuation of the jaw assembly 1130 by the actuation handle 1114. In other embodiments, moving the outer shaft component can be used to open and close the jaws and provide a proper clamping force without manipulating the handle assembly. However, moving the outer shaft component can also cause the vessel sealer/divider to move in relation to a trocar seal and thus potentially complicating a gas seal between the sealer/divider and the insufflated body cavity. As such, it can be desirable that the outer most shaft components remaining stationary throughout a surgical procedure. As such, in certain embodiments, the elongate shaft maintains the moving components (e.g., the pull tube and the blade actuation shaft) on the inside of a stationary outer cover tube (which may also have a dielectric coating or insulating sleeve). With continued reference to Figures 19-1 and 19-2, as illustrated, the stationary outer cover tube is connected to the stationary portion of the jaws, while the pull tube is connected to the moving portion of the jaws (e.g., the upper jaw). Thus, as the jaw assembly 1130 is actuated from an open position (Figure 19-1) to a closed position (Figure 19-2), the pull tube translates longitudinally proximally while the outer cover sleeve remains stationary.

[0134] As discussed above with respect to the electrosurgical system, in certain embodiments the electrosur-

gical tool can comprise a memory such as a tool ID chip mounted on a small PCB. In some embodiments, the PCB can be disposed on or in the actuation handle 1112. In other embodiments, the PCB and chip can be integrated in the plug of the wiring harness. The PCB and chip can be molded with a tool-specific pattern. The tool ID chip and PCB can be electrically connected into the wiring harness and plug of the electrosurgical tool. A "spacer" between the plug and the tool ID chip, can allow the use of the same connector for all tools. In some embodiments, the spacer can have the same shape for all tools on the plug side, and a tool-specific pattern on the chip side such that during assembly there is a reduced risk that a PCB for one type of electrosurgical tool can be assembled into a different type of electrosurgical tool.

[0135] As discussed above with respect to the electrosurgical system, when the plug is inserted into the generator, the encrypted tool information stored in the memory is verified. General information (serial number of tool and generator) are exchanged, and the tool-specific software is uploaded into the generator. With completion of each tool use, tool-specific information (connections to generator, individual tool uses, errors, etc.) can be communicated, if needed, and stored in memory of the generator, the tool chip or both. In exemplary embodiment, the generator's memory is sized to hold data for about two months while the tool chip's memory can hold data for one surgical procedure.

[0136] As discussed above with respect to the electrosurgical system, in some embodiments, the electrosurgical fusion tool can be used in a system which monitors various operational parameters and determines a radiofrequency endpoint based on phase angle.

[0137] Although the present invention has been described in certain specific aspects, many additional modifications and variations would be apparent to those skilled in the art. It is therefore to be understood that the present invention may be practiced otherwise than specifically described, including various changes in the size, shape and materials, without departing from the scope and spirit of the present invention. Thus, embodiments of the present invention should be considered in all respects as illustrative and not restrictive.

Electrosurgical Dissection Tool

[0138] Laparoscopic surgical procedures typically require the dissection of connective or vascular tissue. Depending on factors such as tissue type, size, location and condition of the specific tissue, different tools and techniques can be used to perform a specific procedure. The choice of an individual tool can be based on functionality combined with a desire that the selected tool provide relatively little traumatic damage to the surrounding tissue. As an example, the dissection of connective tissue is usually performed by mechanical or electrosurgical cutting, whereas the dissection of vascular tissue typically relies on ligating techniques employing clips or staplers

followed by a mechanical cut. Consequently, a typical laparoscopic procedure including dissection of both connective tissue and vascular tissue calls for multiple tools being consecutively exchanged through trocar access ports to the surgical site. This tool exchange increases both the cost and time of the surgical procedure. It is hence desirable to provide multi-functional tools that can greatly reduce the number of tool exchanges during laparoscopic procedures.

[0139] Referring now to Figure 20, in the illustrated embodiment, a bloodless tissue-dissecting tool 2101 comprises a proximal hand-piece 2102 that connects through a shaft 2103 to a distal end-piece 2104. Activation of the trigger 2105 on the hand-piece 2102 allows closing and opening of the jaw elements 2106, 2107 on the distal end-piece 2104 so that tissue can be clamped between the upper 2106 and lower 2107 jaw elements.

[0140] With continued reference to Figure 20, in some embodiments, the tool 2101 can be configured to be electrically coupled to an electrosurgical generator. For example, in some embodiments, the tool 2101 can include an integrated power cord, or a socket or other connector adapted to receive a power cord. At least a portion of the tool can be selectively energized through actuation of a control or switch on the electrosurgical generator. For example, in some embodiments, the tool can be energized with a handswitch or a footswitch on or coupled to the electrosurgical generator.

[0141] With reference to Figure 21, an exemplary prior art electrosurgical device is illustrated. Electrosurgical tissue sealing devices that include a mechanical cutter can be used to first electrosurgically coagulate and then mechanically cut through a variety of tissue types. Certain harmonic tissue dividers can also be used to coagulate and/or to dissect a variety of tissue, ranging from connective to highly vascular tissue, such as organs.

[0142] As schematically depicted in Figure 21, prior-art electrosurgical tissue dissectors include a lower jaw forming a first electrode 2201 and an upper jaw forming a second electrode 2202. In the prior art devices, the two jaw elements - or electrodes 2201, 2202 - supply a relatively large amount of pressure to the tissue. High pressure with simultaneous application of electrical energy to the compressed tissue can be used to permanently occlude very large blood vessels by electrosurgical vessel fusion. After the electrical fusion process has been completed, the tissue can be separated by advancing a mechanical blade 2203.

[0143] In contrast to the prior art electrosurgical devices, with reference to Figure 22A, one embodiment of an electrosurgical tool that can be configured in either an electrosurgical coagulation state or an electrosurgical cutting state is shown. In the illustrated embodiment, a lower jaw element 2301 comprises a first coagulating electrode 2302, a second coagulating electrode 2303, and an electrosurgical cutting electrode 2304. Each of the electrodes can be electrically isolated from each other by insulating members 2305. The upper jaw 2306 is not

energized in this embodiment, but is merely used to press tissue against the lower jaw element 2301.

[0144] With the electrode arrangement illustrated in Figure 22A, tissue that is in contact with the lower jaw element 2301 can be coagulated by electrically coupling each of the two coagulation electrodes 2302, 2303 with the corresponding outlet of a bipolar electrosurgical unit. Here, the two coagulation electrodes 2302 and 2303 can be supplied with electrical energy having opposite polarities. In some embodiments, it can be desirable that the supplied electrical energy has a potential difference of no more than 200V to reduce the risk of arcing and that electrode 2302 and 2303 have the same contact area with the tissue. The latter ensures the same electrosurgical effect for both electrodes.

[0145] With continued reference to Figure 22A, after the two coagulation electrodes 2302, 2303 have achieved substantial hemostasis within the coagulated tissue volume, the tissue can be electrosurgically cut by applying energy to an electrosurgical cutting electrode 2304. During the electrosurgical cutting operation, the two coagulation electrodes 2302, 2303 can be electrically coupled to a corresponding outlet or outlets of a bipolar electrosurgical unit to function as return electrodes. Here, the potential difference between the cutting electrode 2304 and the two return electrodes 2302 and 2303 can desirably be between approximately 300-500V, while the two return electrodes can desirably be substantially equipotential.

[0146] With continued reference to Figure 22A, in some embodiments, it can be desirable that the relative contact area of the electrodes with the tissue is much smaller for the cutting electrode 2304 than for the return electrodes 2302, 2303. For example, in some embodiments, desirably the cutting electrode can have a contact area that is between approximately 1 % and 20% as large as a contact area of one of the return electrodes 2302, 2303. More desirably, the cutting electrode can have a contact area that is between about 5% and 10% as large as a contact area of one of the return electrodes 2302, 2303. In one embodiment, the cutting electrode can have a contact area that is approximately 10% as large as a contact area of one of the return electrodes 2302, 2303. This relative proportion between cutting area sizes lead to a relatively high current density (and hence high power density) in tissue close to the cutting electrode, which facilitates localized vaporization, or electrosurgical cutting of the tissue.

[0147] With continued reference to Figure 22A, an additional aspect of the illustrated electrode arrangement is that the lower jaw 2301 can be used for both coagulation and cutting, regardless of whether the jaws are in an opened or closed position. This multiple functionality is advantageous when using the tool to spot-coagulate tissue, or to dissect tissue by configuring the tool in a cutting state and brushing the tool against the tissue.

[0148] Another embodiment of electrode arrangement for a surgical tool is illustrated in Figure 22B. In the illus-

trated embodiment, the upper jaw 2306' is not only used to press tissue against the lower jaw element 2301, but it also includes an upper electrode 2307 disposed thereon which can be supplied with electrical energy. Tissue can be coagulated by supplying the two lower coagulation electrodes 2302, 2303 with a first electrical polarity, and the upper electrode 2307 with a second, opposing polarity from a bipolar electrosurgical unit. Again, it is desirable that when configured for coagulation, the potential difference between the upper electrode 2307 and the two lower electrodes 2302, 2303 does not exceed 200V to reduce the risk of arcing to the tissue and that electrode 2307 has the same contact area with the tissue as the combined surface area of electrodes 2302 and 2303. The latter ensures the same electrosurgical effect for both electrode sides.

[0149] With continued reference to Figure 22B, after hemostasis of the tissue between the upper electrode 2306' and the two lower electrodes 2302, 2303 has been substantially achieved, the tissue can be electrosurgically cut by supplying the electrosurgical cutting electrode 2304 with electrical energy. The upper coagulation electrode 2307 on the upper jaw 2306' can be configured as a return electrode by electrically coupling it with the corresponding outlet of a bipolar electrosurgical unit.

[0150] With continued reference to Figure 22B, when the surgical tool is configured as a electrosurgical cutting device, desirably the potential difference between the cutting electrode 2304 and the return electrode 2307 is between approximately 300-500V. In some embodiments, it can be desirable that the contact area of the electrodes with the tissue is much smaller for the cutting electrode 2304 than with the return electrode 2307 on the upper jaw 2306'. For example, in some embodiments, desirably the cutting electrode can have a contact area that is between approximately 1% and 20% as large as a contact area of the return electrode 2307. More desirably, the cutting electrode can have a contact area that is between about 5% and 10% as large as a contact area of the return electrode 2307. In one embodiment, the cutting electrode can have a contact area that is approximately 10% as large as a contact area of the return electrode 2307. This relative sizing can lead to relatively high current density (and hence high power density) in the tissue close to the cutting electrode 2304, which facilitates localized vaporization, or electrosurgical cutting of the tissue. With the surgical tool distal end of Figure 22B having electrodes 2302, 2303, 2304, 2307 as described above, only tissue between the two jaw elements can be coagulated and/or cut. Thus, unlike the embodiment of Figure 22A, the tool illustrated in Figure 22B is not configured to be used by employing the lower electrode only.

[0151] Another embodiment of electrode arrangement for a surgical tool is illustrated in Figure 22C. In the illustrated embodiment, the upper jaw 2306" includes an upper electrode 2307', but also shows two cutting electrodes 2304 and 2309 that are sandwiched between two coagulation electrodes 2302 and 2303. In difference to

the embodiment shown in Figure 22B, both coagulation and cutting is distinguished for cases where the hand tool (and hence the jaw members) are fully opened or not fully opened. With a fully opened tool, tissue can be coagulated by applying the two lower coagulation electrodes 2302 and 2303 with opposing polarities, and will be cut by applying cutting electrode 2304 with the first and both electrodes 2302 and 2303 to the second polarity. In difference, a not fully opened tool will coagulate tissue by applying both lower coagulation electrodes 2302 and 2303 with one polarity and electrode 2307' to the opposing one, while cutting occurs between electrode 309 and return electrode 2307'. Again, it is desirable that when configured for coagulation, the potential difference between the two lower electrodes 2302 and 2303 (tool fully open) or the upper electrode 2307' and the two lower electrodes 2302, 2303 (tool not fully open) does not exceed 200V to reduce the risk of arcing to the tissue.

[0152] The separation of cutting electrodes 2304 and 309 facilitates cutting of tissue that is positioned within the upper and lower jaw elements (not fully opened), or cutting of tissue in contact with the bottom side of the tool. The separation prevents inadvertent cutting of tissue.

[0153] Another embodiment of electrode arrangement for a surgical tool is illustrated in Figure 22D where the upper jaw 2306''' includes two separate electrodes 2307'' and 2308. In this configuration, the upper jaw element 2306''' can be used to press tissue against the lower jaw element 2301, but can also supply electrical energy.

[0154] With continued reference to Figure 22D, the electrodes 2302, 2303, 2307'', 2308 can be selectively configured to a coagulation state. By supplying the coagulation electrodes 2302, 2303 on the lower jaw 2301 and the two coagulation electrodes 2307'', 2308 on the upper jaw 2306''' with alternating polarities, tissue within the jaws can be coagulated. For example, in one possible coagulation state configuration, one coagulation electrode 2302 on the lower jaw 2301, and one coagulation electrode 2308 on the upper jaw 2306''' can be electrically coupled to a source of electrical energy having a first polarity. The other coagulation electrode 2303 on the lower jaw 2301, and the other coagulation electrode 2307'' on the upper jaw 2306''' can be electrically coupled to a source of electrical energy having a second polarity generally opposite the first polarity. While this is an illustrative example, it is contemplated that other combinations of connections of the electrodes 2302, 2303, 2307'', 2308 with electrical energy sources are possible to configure the tool in a coagulation state. It can be desirable that the contact area of the opposing coagulation electrode(s) are the same to provide the same electrosurgical effect for both electrode sides.

[0155] With continued reference to Figure 22D, after homeostasis of the tissue between the upper electrodes 2307'', 2308 and the two lower electrodes 2302, 2303 by application of electrical energy with the electrodes in the coagulation state, the tissue can be electrosurgically cut.

The distal end of the surgical tool can be configured into a cutting state by supplying the electrosurgical cutting electrode 2304 with electrical energy. In various embodiments, one, some, or all of the other electrodes 2302, 2303, 2307", 2308 can be configured to function as return electrodes when the tool is in a cutting state by electrically coupling them with the corresponding outlet of a bipolar electrosurgical unit.

[0156] With continued reference to Figure 22D, when the tool is configured in a cutting state, the potential difference between the cutting electrode and the return electrode is desirably between approximately 300-500V. Further, it can be desirable that the relative contact area of the electrodes with the tissue is much smaller for the cutting electrode 2304 than for any of the return electrodes 2302, 2303, 2307", 2308 or combinations thereof. For example, in some embodiments, desirably the cutting electrode 2304 can have a contact area that is between approximately 1% and 20% as large as a contact area of one of the return electrodes. More desirably, the cutting electrode can have a contact area that is between about 5% and 10% as large as a contact area of one of the return electrodes. In one embodiment, the cutting electrode can have a contact area that is approximately 10% as large as a contact area of one of the return electrodes. Just as with the embodiment illustrated and described with respect to Figure 22A, the electrode arrangement illustrated in the embodiment of Figure 22D can be used to spot-coagulate tissue, or to dissect the tissue when "brushing" the tool against it in a cutting mode.

[0157] The practicality of the tool configurations of Figures 22A through 22D can be further enhanced by selective activation and/or deactivation of the selected electrodes. In some embodiments, this selective activation and deactivation can be performed by operator-depressed electrical switches such as wired or wireless hand or foot operated switches, or switches positioned on the hand-piece. The electrosurgical unit will then address specific electrodes, depending on how far the jaws are opened and closed.

[0158] Figure 23A illustrates a schematic circuit diagram for an electrode arrangement as given in Figure 22A. Here, activation of a single-pole electrical switch 401 connects the outer coagulating electrodes 2302, 2303 to opposing polarities, while the center "cutting" electrode 2304 remains disengaged. This setting configures the electrodes in a coagulation state. Alternately, activation of a double-pole electrical switch 402 supplies the center "cutting" electrode 2304 with electrical energy having a first polarity, and the outer return electrodes 2302, 2303 with electrical energy having a second polarity generally opposing the first polarity. This setting configures the electrodes in a cutting state. As a result, the tool can be used for electrosurgical coagulation and/or cutting, and hence can perform the bloodless dissection of tissue.

[0159] Figure 23B illustrates a schematic power supply circuit that can be used for the electrode arrangement

shown in Figure 22B. In the illustrated embodiment, activation of a double-pole electrical switch 2403 connects the two outer coagulating electrodes 2302, 2303 on the lower jaw to a supply of electrical energy of a first polarity, and the coagulating electrode 2307 on the upper jaw to a supply of electrical energy of a second polarity substantially opposite the first polarity. With the switch 2403 in this position, the cutting electrode 2304 remains disengaged. This setting configures the electrodes of the surgical tool in a coagulation state. Alternately, activation of a single-pole electrical switch 2404 allows the lower jaw electrodes 2302, 2303 to be used for coagulation. The electrode on the upper jaw 2307 and the cutting electrode 2304 remain disengaged in this alternate coagulation configuration. To dissect tissue after it has been coagulated, a separate electrode outlet 2405 on an electrosurgical generator is used to address the cutting electrode 2304. Desirably, the cutting electrode is supplied with voltages of 300-500V with respect to the two return electrodes 2302, 2303 on the lower jaw.

[0160] Figure 23C illustrates a schematic power supply circuit that can be used to address the electrode arrangement of Figure 22D. In the illustrated embodiment, activation of a double-pole electrical switch 2406 connects the two coagulating electrodes 2302, 2303, 2307", 2308 on both the lower and upper jaw to sources of electrical energy having opposing polarities. The cutting electrode 2304 remains disengaged. This setting can be used to configure the electrodes of a surgical tool in a coagulation state to coagulate tissue that is clamped between the upper and lower jaw element. Alternately, in other embodiments, a second coagulation double-pole switch 2407 can be implemented to separate the activation of the upper and lower jaws such that one or both jaws can be selectively actuated during a coagulation state. To utilize the lower jaw of the tool for electrosurgical cutting of coagulated tissue, activation of the cutting double-pole switch 2408 connects the cutting electrode 2304 to a source of electrical energy having a first polarity and the two return electrodes 2302, 2303 to a source of electrical energy having a second polarity substantially opposite the first polarity. The voltage supplied by the generator for this setting is desirably between approximately 300-500V to facilitate electrosurgical cutting. In the illustrated embodiment, the electrodes 2307", 2308 on the upper jaw element remain unaddressed during electrosurgical cutting.

[0161] As discussed in more detail above, the activation (or deactivation) of specific electrodes can configure the tool in a coagulation state or a cutting state. In certain embodiments, the selective activation and deactivation of specific electrodes can be facilitated by push-buttons, switches, or other electrical switching devices mounted on the hand-piece of the laparoscopic tool, or wired or wireless switches. In other embodiments, the selective activation and deactivation of specific electrodes can be facilitated by switches or other electrical switching devices that are incorporated into the handle mechanism of

the hand-piece to switch at various positions of the jaw elements.

[0162] Regarding the circuit shown in Figure 23A, referring to the tool shown in Figure 22A, switching devices mounted on the hand-piece can be used to allow a user to selectively configure the electrodes on the tool. Switch 2401 can be a hand-activated switching device mounted on the hand-piece that can be selectively activated to configure the electrodes of the tool in a coagulation state. Switch 2402 can be a hand-activated switching device mounted on the hand-piece that can be selectively activated to configure the electrodes of the tool in a cutting state. In another embodiment, switches 2401, 2402 can be incorporated into the handle mechanism to such that the tool is automatically switched from a coagulation state to a cutting state at a predetermined position of the clamping members.

[0163] One benefit of switching the electrodes from a coagulation state to a cutting state at different positions of the jaw elements (e.g., open and nearly closed jaws) can be seen with respect to the embodiment of Figure 23B. In certain embodiments, switches 2403 and 2404 can be incorporated within the handle of the surgical tool for self-switching based on the position of the trigger mechanism, rather than on the outside of the hand tool for hand-activation. In one embodiment, switch 2403 can be disengaged and switch 2404 engaged in a fully open jaw element position. Thus, with the jaw elements fully opened, the switches 2403, 2404 can be configured such that only the lower jaw element can be used for spot coagulation. In this embodiment when the trigger of the hand-piece is actuated to move the jaw elements closed from the fully opened jaw position, switch 2404 is disengaged and 2403 simultaneously engaged. Thus, with the jaw elements moved into a partially-closed configuration, the tool can be used to coagulate or cut tissue that is clamped between the upper and lower jaw element.

[0164] In the described embodiment, the electrode switches are automatically actuated as the jaw elements are closed. Although the described embodiment includes a switch point between a coagulation state and a cutting state upon commencement of closure from the jaws fully opened position, other embodiments can have different switching positions. For example, with this automatic switching, the switches 2403, 2404 can be configured such that the electrodes are activated and deactivated at any position in an opening or closing cycle. In other embodiments, a surgical tool can include the electrode configuration of Figure 22B and the switching circuit of Figure 23B with the switches 2403, 2404 configured for manual actuation, such as by positioning on the tool hand-piece.

[0165] Similarly, in certain embodiments, a surgical tool having the electrode configuration of Figure 22D with the switching circuit of Figure 23C can have the switches 2406, 2408 incorporated into the trigger mechanism for automatic switching between a coagulation state and a cutting state at certain jaw element positions. In certain

embodiments, it can also be desirable to incorporate the second coagulation switch 2407 into the trigger mechanism of the hand-piece, disengaging the electrodes on the upper jaw element in predetermined jaw position such as a fully opened jaw position. This switching arrangement of the second coagulation switch 2407 allows for example to spot-coagulate tissue using the lower jaw element without inadvertently touching tissue with the electrodes on the upper jaw element. In other embodiments, it can be desirable for the second coagulation switch 2407 to be positioned on the hand-piece to be manually actuated by a user, allowing a user to selectively engage and disengage the electrodes on the upper jaw element. In other embodiments, all of the switches 2406, 2407, 2408 of the switching circuit of Figure 23C can be positioned on the hand-piece of the surgical tool to be manually actuated by the user.

[0166] With reference to Figure 24, one configuration of tool switching is illustrated. In the illustrated embodiment, electrical contacts are incorporated both into the hand-piece 2501 and the trigger 2502. For example, as illustrated, the hand-piece 2501 includes a first electrical contact 2504, a second electrical contact 2506, and a third electrical contact 2507 positioned therein. In the illustrated embodiment, the trigger 2502 includes a first electrical contact 2503 and a second electrical contact 2505. All of the electrical contacts 2503, 2504, 2505, 2506, 2507 are positioned to engage and disengage one another at predetermined relative positions of the trigger 2502 and the hand-piece 2501.

[0167] With continued reference to Figure 24, as shown, the first contact 2503 on the trigger 2502 engages the first contact 2504 on the hand-piece 2501 when the jaws are in a fully opened position, but the first contacts 2503, 2504 are disconnected when the trigger 2502 is moved from the open position to close the jaws. In the illustrated embodiment, with the jaws in the fully opened position, the second contact 2505 on the trigger 2502 engages the second contact 2506 on the hand-piece 2501. But, the second contacts 2505, 2506 are disconnected when the trigger 2502 is moved from the open position to close the jaws. As the jaws are closed further, the second contact 2505 on the trigger 2502 becomes engaged with the third contact 2507 on the hand-piece 2501, and the first contact 2503 on the trigger engages the second contact 2506 on the hand-piece 2501. This engagement allows switching of the polarity of the contacts 2507 as the hand-piece is closed further. As a result, and with reference to Figure 22B, the switching mechanism in Figure 24 allows for activation of the upper electrode 2307 and a lower coagulating electrode 2303 with opposing polarities in a fully open jaw position. With progressive tissue desiccation, the jaws start to close, and the upper electrode 2307 becomes electrically disengaged (by disconnecting contact 2503 and 2504 in Figure 24), whereas the lower electrode 2303 is switched to the same polarity as the second electrode 2302 (by connecting contact 2505 from 2506 to contact 2507 in Figure 24).

In a separate step, the desiccated tissue between the upper and lower jaw elements can now be electrosurgically dissected.

[0168] With reference to Figure 25, another embodiment of a switching mechanism is illustrated with the jaw members in a fully opened position. In the illustrated embodiment, concentric contact strips are disposed on the hand-piece and opposing contact pins are mounted on the trigger. In other embodiments, contact pins can be mounted on the hand-piece and contact strips positioned on the trigger. In the illustrated embodiment, trigger movement allows the pin contacts (which are connected to specific electrodes) to be supplied with electrical energy at certain tool positions. In some embodiments, the polarity of a single pin (i.e., the same electrode) might change as the jaws are opened or closed.

[0169] One contact strip and pin arrangement is illustrated in Figure 25 for an electrode configuration of Figure 3b. In the illustrated embodiment, pin 2601 is electrically coupled to the electrode 2307 (Figure 22B) on the upper jaw member and is disengaged. As illustrated, pin 2602 is electrically coupled to one of the coagulating electrodes 2302, 2303 (Figure 22B) on the lower jaw. As illustrated, pin 2602 is engaged as the trigger is moved from the "fully-open" position to a partially closed position. With further advancement of trigger, pin 2602 changes to the same polarity as the second coagulating electrode so that both can be used as return electrodes for cutting.

[0170] While both Figure 24 and Figure 25 show active switching mechanisms in the hand tool (where active electrodes can be switched), which allows the tools to be used with "conventional" electrosurgical generators, Figure 26 shows a configuration for passive switching. Here, a momentary switch 2701 is mounted in the handle and is closed by a trigger 2702 when lever 2703 is brought into the "fully open" position.

[0171] Similarly, Figure 27 shows the incorporation of two momentary switches 2801 and 2802 that are closed by trigger 2803 and 2804 in the "tool fully open" and "tool fully closed" position, respectively. The closing of the momentary switches as shown in Figures 26 and 27 is then used for logic switching of multi-electrode generators, as described in the following.

[0172] Figure 28 shows a schematic of a multi-electrode switching power supply for directly connecting individual tool electrodes (such as all individual electrodes in Figures 22A through 22D) to an internal RF power source. Instead of switching two polarities of an external electrosurgical unit to different electrodes with active switches in the hand tools, this arrangement facilitates population of individually-connected electrodes with different polarities by switching within the power supply. Depending on the tool position, as determined by tool position switches shown in Figures 26 and 27, the electrodes can be populated differently as determined by pre-determined logic. As such, the five electrode connection points 2901 through 2905 are connected to a relay bank

2906 to a bus bar 2907. Through selected switching of all relays in the relay bank 2906, each outlet point 2901 through 2905 can be independently and/or concurrently connected to the plant connection points 2908 and 2909, respectively. The plant connection points 2908 and 2909 themselves can be connected through the relay bank 2910 to the two outlets of a tissue measurement circuit 2911, or a RF plant 2912.

[0173] With reference to Figure 29, in certain embodiments, methods of using an electrosurgical tool for substantially bloodless tissue dissection are schematically illustrated. The illustrated method includes a positioning step 2952, a tissue assessment step 2954, an applying-electrical-energy-to-coagulate step 2956, a tissue measurement step 2958, a switching step 2960, and an applying-electrical-energy-to-cut step 2962. In the positioning step 2952 an electrosurgical tool having a plurality of electrodes being configurable in one of a coagulation configuration and a cutting configuration is positioned adjacent to tissue to be dissected. In certain embodiments, the electrosurgical tool comprises aspects of the electrosurgical tools discussed herein and illustrated in Figures 20 and 22-27.

[0174] In the tissue assessment step 2954, a measurement signal is applied to the tissue by the coagulation electrodes to determine a future trigger level to switch from coagulation to cutting. This determination can be achieved by measuring the product of conductivity and permittivity of the tissue, pointing to the desired electrical phase shift switching level for the respective tissue. For example, in some embodiments, desirable cutting switching levels occur at 10 degrees to 40 degrees. More desirably, the preferred switching level for blood vessels is between 10 to 30 degrees phase shift, while for highly vascular tissue (such as organs) it is rather between 20 to 40 degrees.

[0175] In the applying-electrical-energy-to-coagulate step 2956, electrical energy is applied to the electrosurgical tool in a coagulation configuration to achieve hemostasis in the tissue. In various embodiments discussed herein, electrode configurations for coagulation are provided. For example, applying electrical energy to the electrosurgical tool in the coagulation configuration can comprise supplying one of a plurality of electrodes with electrical energy having a first polarity and supplying another of the plurality of electrodes with electrical energy having a second polarity generally opposite the first polarity. Desirably, a potential difference between the electrode having the first polarity and the electrode having the second polarity is no more than approximately 200 V.

[0176] During the coagulation process of the tissue the phase shift between applied voltage and incurred current is measured concurrently in step 2958 to provide feedback of the coagulation status. Once the pre-determined switching level is reached, the process will proceed to the switching step 2960.

[0177] In the switching step 2960, as discussed above, some embodiments of electrosurgical tool can comprise

a handle assembly including a switching mechanism. This switching mechanism can selectively configure the electrosurgical tool in either the coagulation configuration or the cutting configuration depending on a position of a trigger of the handle assembly. As discussed above, in some embodiments the switching mechanism can be configured such that with the electrosurgical tool in an open position, the electrodes are configured in the coagulation configuration. The switching mechanism can further be configured such that when the electrosurgical tool is moved towards a closed position, the electrodes are configured in the cutting configuration. In other embodiments, switching of the configuration of electrodes from the coagulation configuration to the cutting configuration can occur at different predetermined positions of the trigger of the handle assembly. In yet another embodiment, the switching can occur within a multi-electrode power supply as shown in Figure 28.

[0178] In the applying-electrical-energy-to-cut step 2962, electrical energy is applied to the electrosurgical tool in a cutting configuration to dissect the tissue. In various embodiments discussed herein, electrode configurations for cutting are provided. For example, applying electrical energy to the electrosurgical tool in the cutting configuration can comprise supplying one of a plurality of electrodes with electrical energy and configuring another of the plurality of electrodes as a return electrode. Desirably, a potential difference between the cutting electrode and the return electrode is between approximately 300 V and approximately 500 V.

[0179] Although this application discloses certain preferred embodiments and examples, it will be understood by those skilled in the art that the present inventions extend beyond the specifically disclosed embodiments to other alternative embodiments and/or uses of the invention and obvious modifications and equivalents thereof. Further, the various features of these inventions can be used alone, or in combination with other features of these inventions other than as expressly described above. Thus, it is intended that the scope of the present inventions herein disclosed should not be limited by the particular disclosed embodiments described above, but should be determined only by a fair reading of the following claims.

Claims

1. An electrosurgical tool having a proximal end and a distal end, the tool comprising:

a distal end-piece positioned at the distal end of the tool comprising:

a first jaw element,
a second jaw element, the first and second jaw elements movable relative to one another between an open position and a

closed position; and
a plurality of electrodes disposed on at least one of the first jaw element and the second jaw element, the plurality of electrodes selectively configurable in one of a coagulation configuration and a cutting configuration;
an elongate shaft having a distal end connected to the distal end-piece and a proximal end;
a handle assembly positioned at the proximal end of the tool and connected to the proximal end of the elongate shaft, the handle assembly comprising;
a hand-piece; and
a trigger pivotally coupled to the hand-piece and operably coupled to the distal end-piece such that movement of the trigger relative to the hand-piece moves the first and second jaw elements relative to one another; and
a switching mechanism electrically coupled to the distal end-piece to selectively configure the plurality of electrodes in one of the coagulation configuration and the cutting configuration.

2. The electrosurgical tool of Claim 1, wherein the switching mechanism is operable by movement of the trigger relative to the hand-piece such that movement of the trigger selectively configures the plurality of electrodes in one of the coagulation configuration and the cutting configuration.

3. The electrosurgical tool of Claim 2, wherein the switching mechanism configures the plurality of electrodes in the coagulation configuration when the first jaw element and the second element are in the open position.

4. The electrosurgical tool of Claim 2, wherein the switching mechanism configures the plurality of electrodes in the cutting configuration when the first jaw element and the second jaw element are moved from the open position towards the closed position.

5. The electrosurgical tool of Claim 2, wherein the switching mechanism comprises:

a first electrical contact, a second electrical contact, and a third electrical contact all positioned on the hand-piece; and
a fourth electrical contact and a fifth electrical contact positioned on the trigger.

6. The electrosurgical tool of Claim 5, wherein the first electrical contact, second electrical contact, third electrical contact, fourth electrical contact, and fifth

electrical contact are positioned to engage and dis-engage one another at predetermined relative positions of the trigger and the hand-piece.

7. The electrosurgical tool of Claim 5, wherein when the first jaw element and the second jaw element are in an open position, the fourth electrical contact on the trigger engages the first electrical contact on the hand-piece, and the fifth electrical contact on the trigger engages the second electrical contact on the hand-piece. 5
10

8. The electrosurgical tool of Claim 5, wherein when the first jaw element and the second jaw element are between the open position and the closed position, the fourth electrical contact on the trigger engages the second electrical contact on the hand-piece, and the fifth electrical contact on the trigger engages the third electrical contact on the hand-piece. 15
20

9. The electrosurgical tool of Claim 2, wherein the switching mechanism comprises a plurality of contact strips disposed on the hand-piece, and a plurality of contact pins mounted on the trigger. 25

10. The electrosurgical tool of Claim 9, wherein the plurality of pins comprises two pins. 30


11. The electrosurgical tool of Claim 9, wherein the plurality of contact strips comprises two concentric contact strips. 35

12. The electrosurgical tool of Claim 1, wherein the switching mechanism comprises a single pole electrical switch and a double pole electrical switch. 40

13. The electrosurgical tool of Claim 1, wherein the switching mechanism comprises a first double pole electrical switch and a second double pole electrical switch. 45

14. The electrosurgical tool of Claim 13, wherein the switching mechanism further comprises a third double pole electrical switch. 50

15. The electrosurgical tool of Claim 1, wherein the switching mechanism comprises a multi-electrode switching power supply. 55

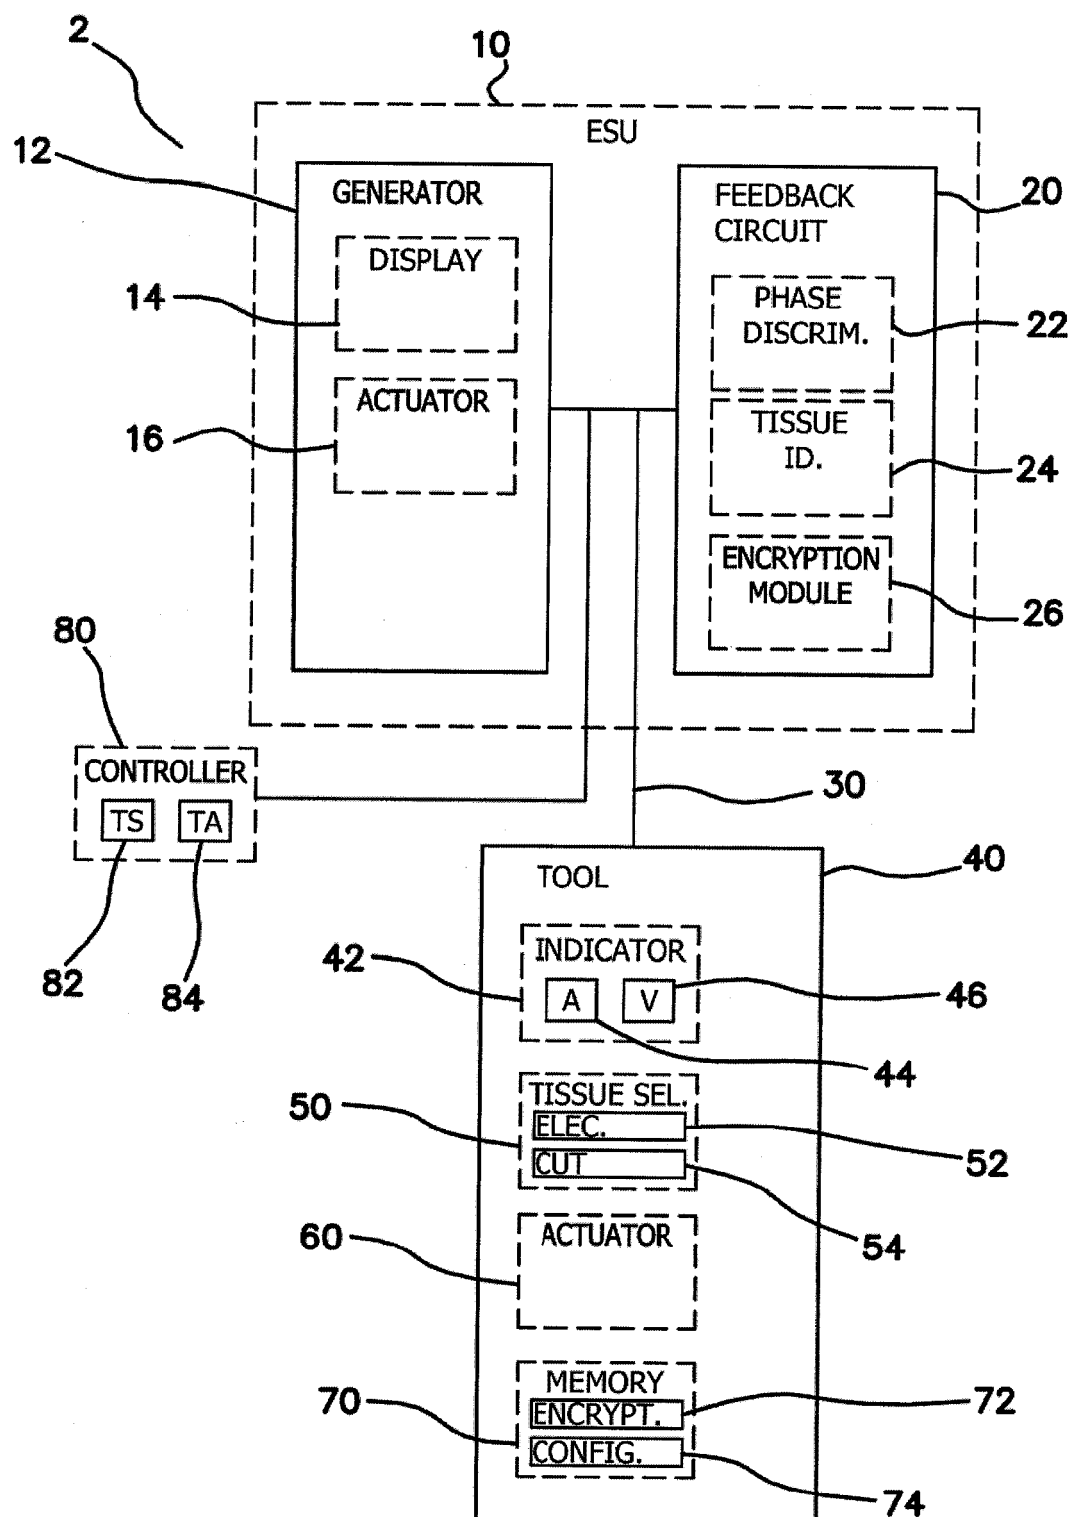**FIG. 1A**

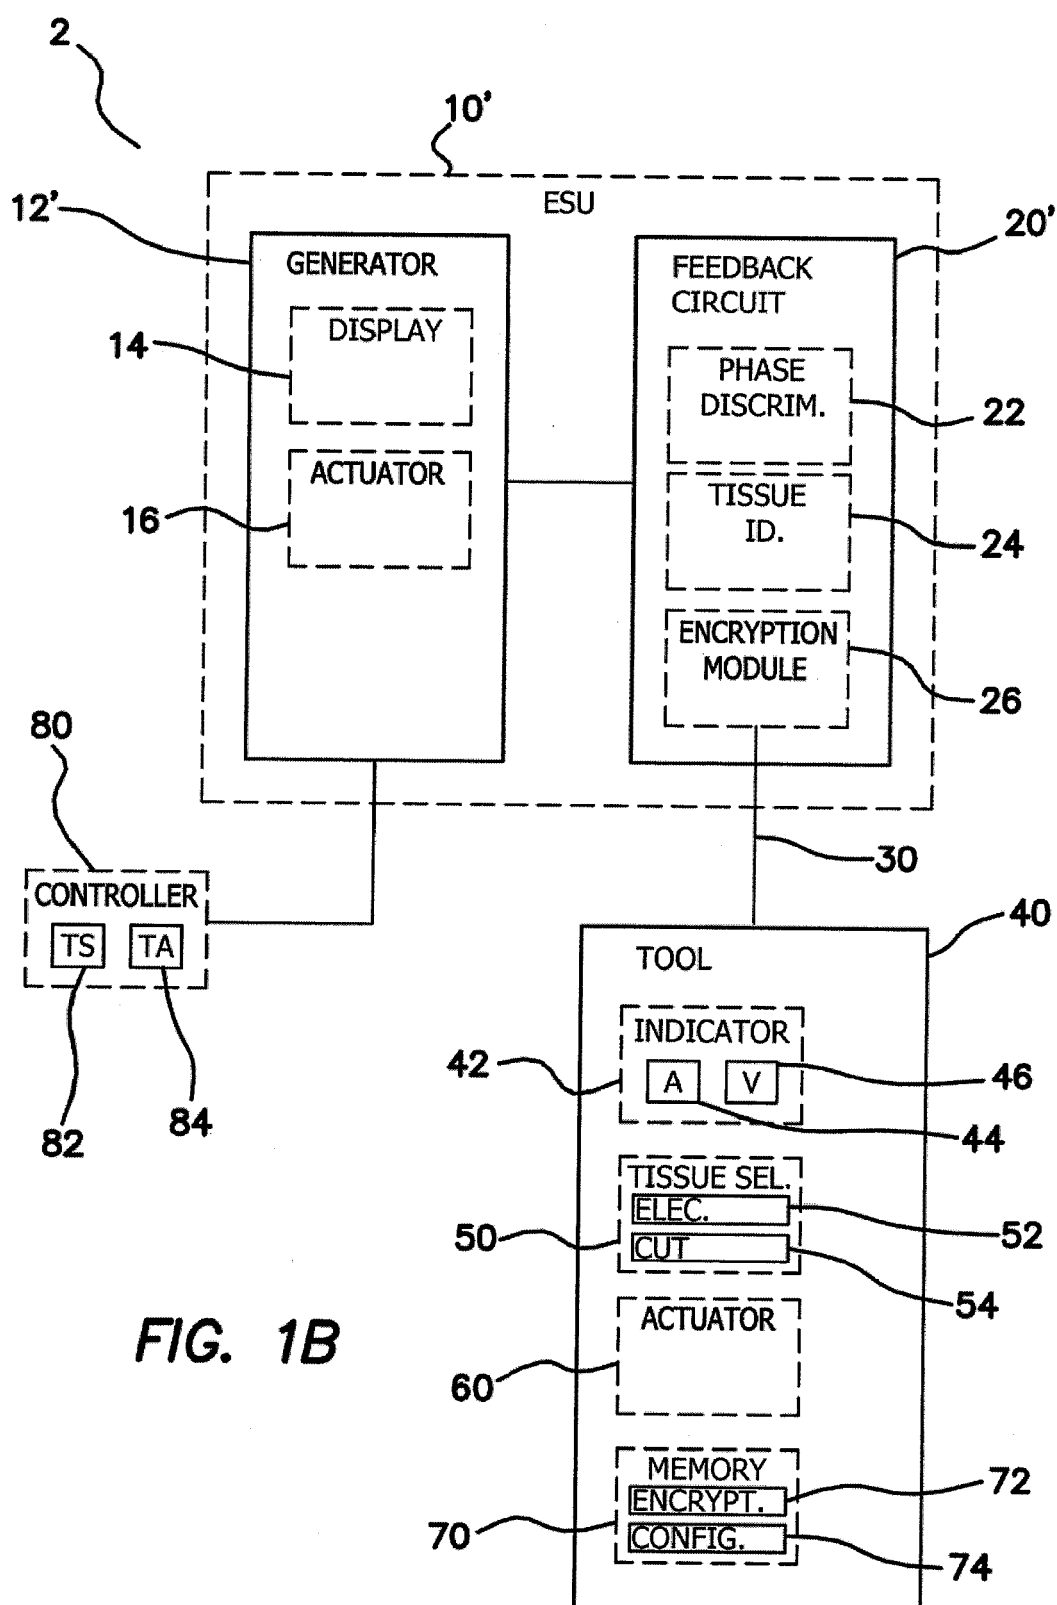


FIG. 1B

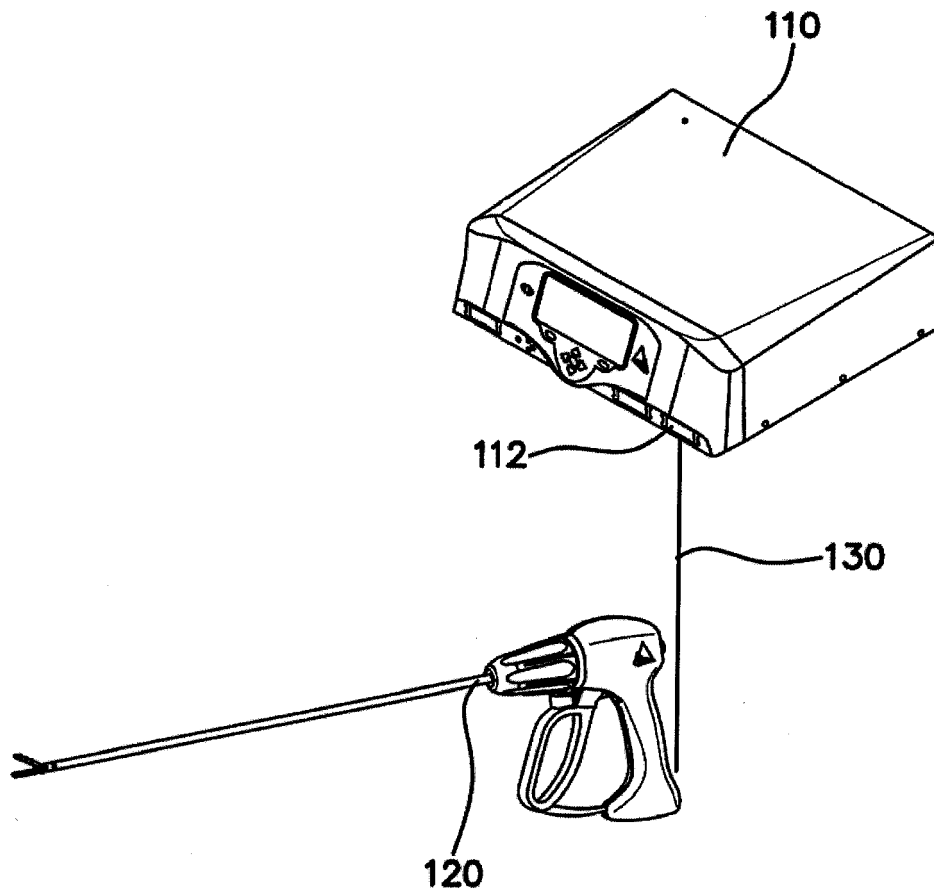


FIG. 2A

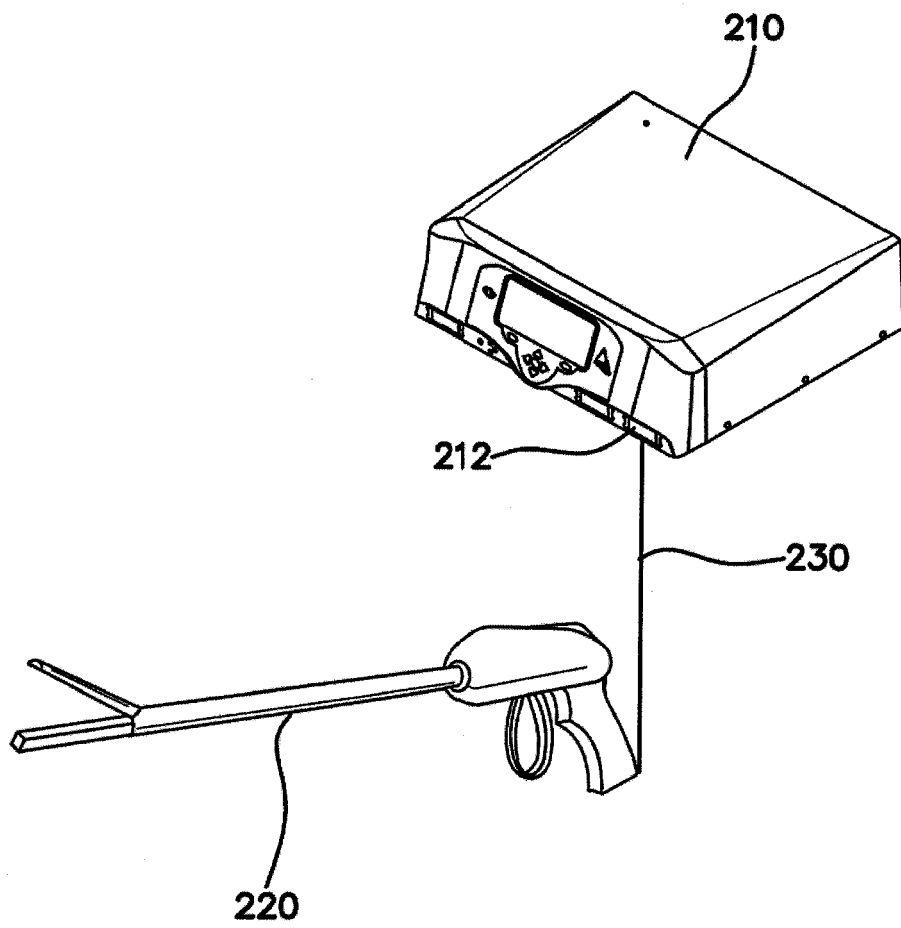


FIG. 2B

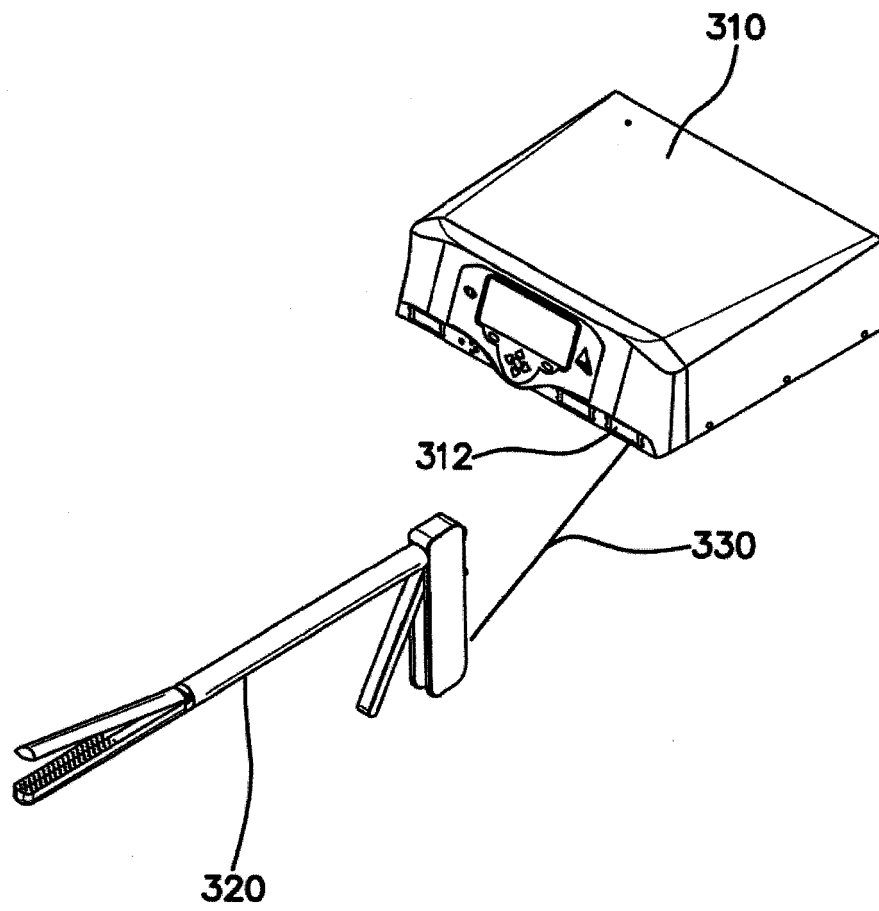


FIG. 2C

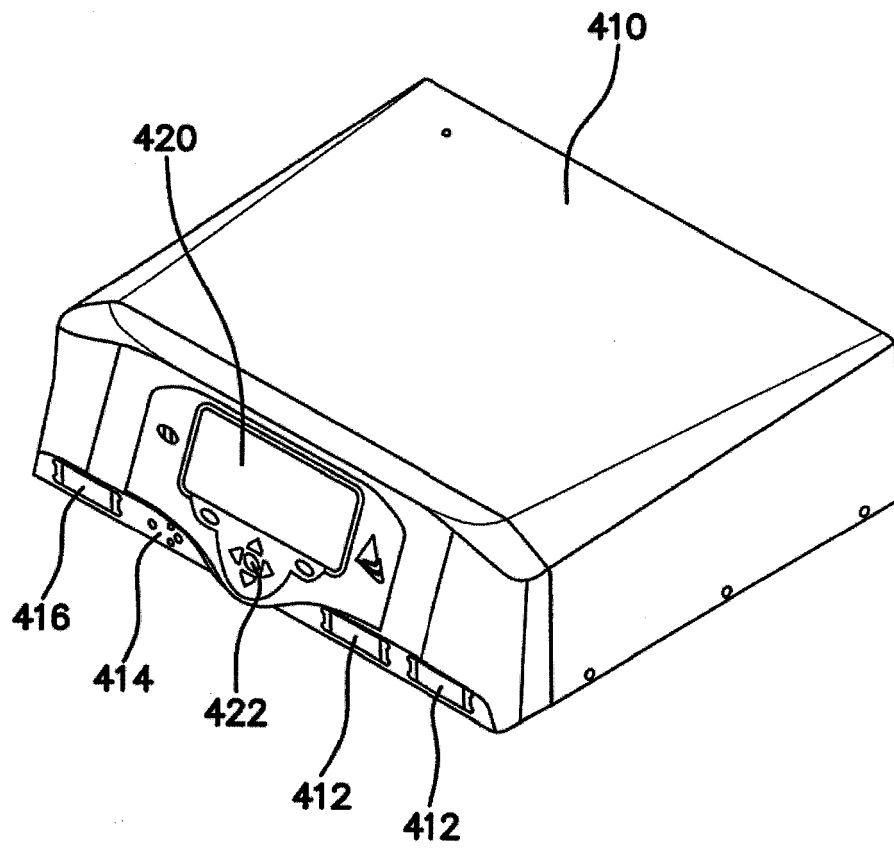


FIG. 3A

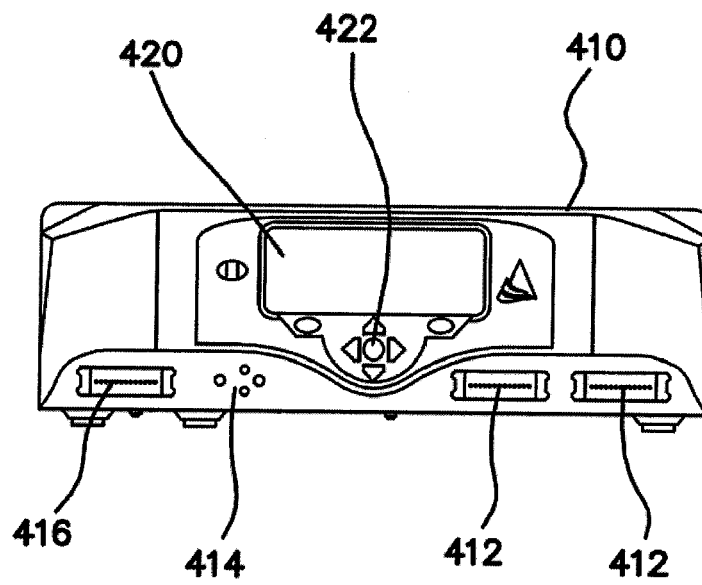


FIG. 3B

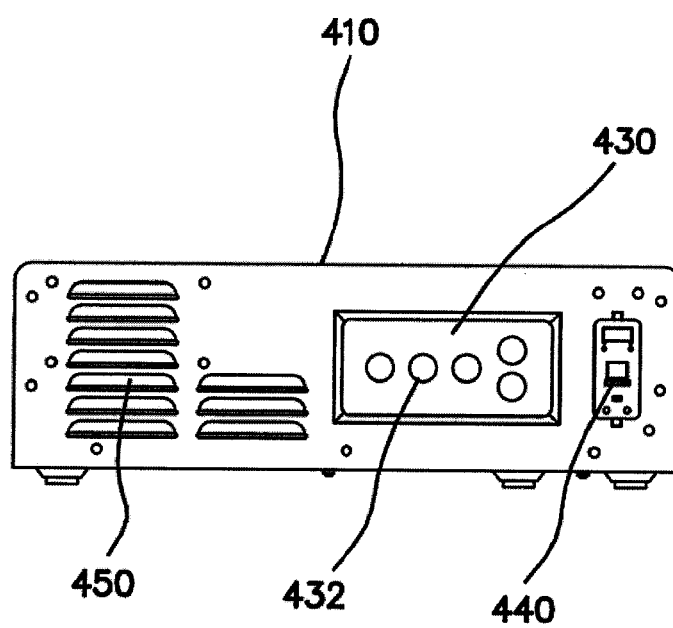


FIG. 3C

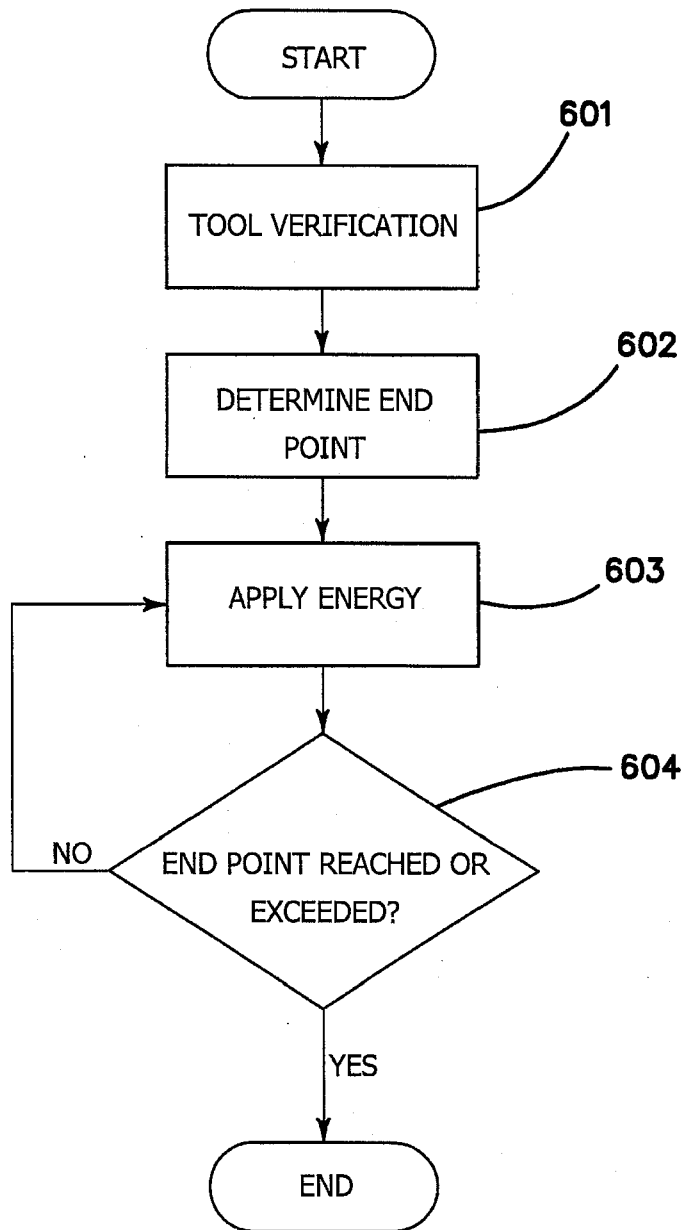


FIG. 4

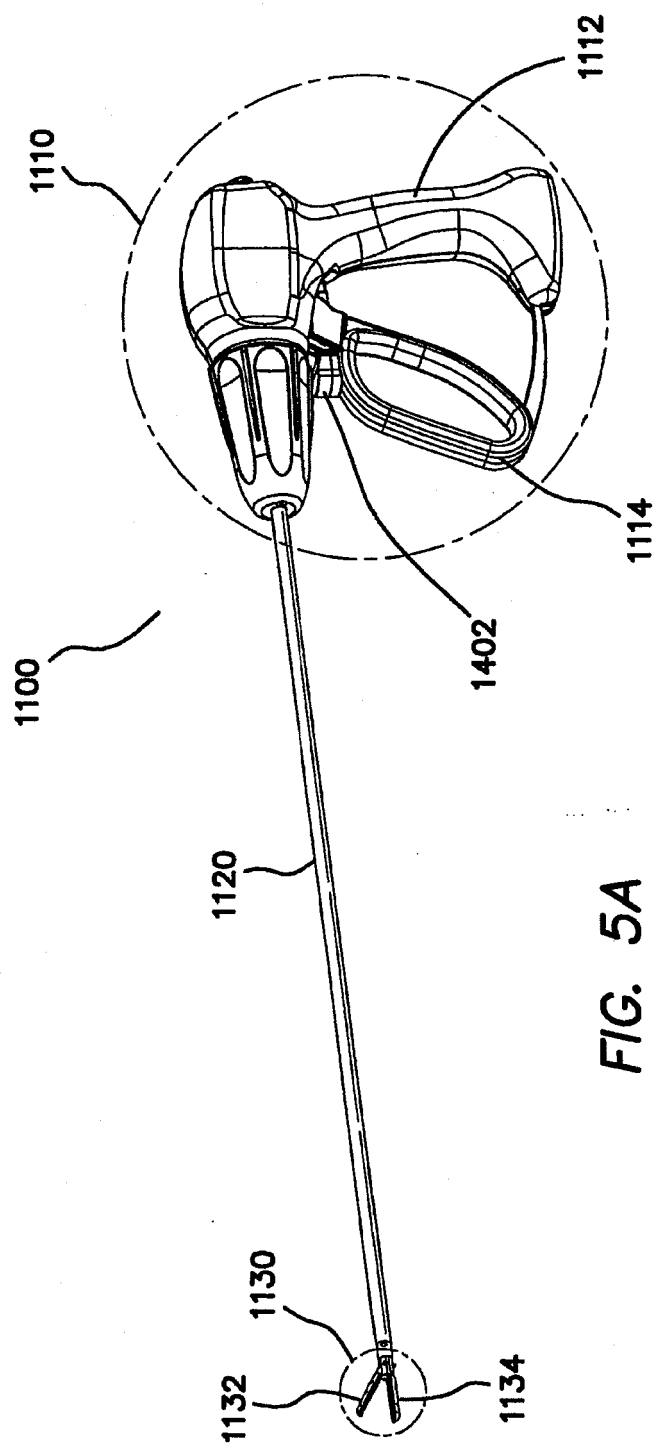
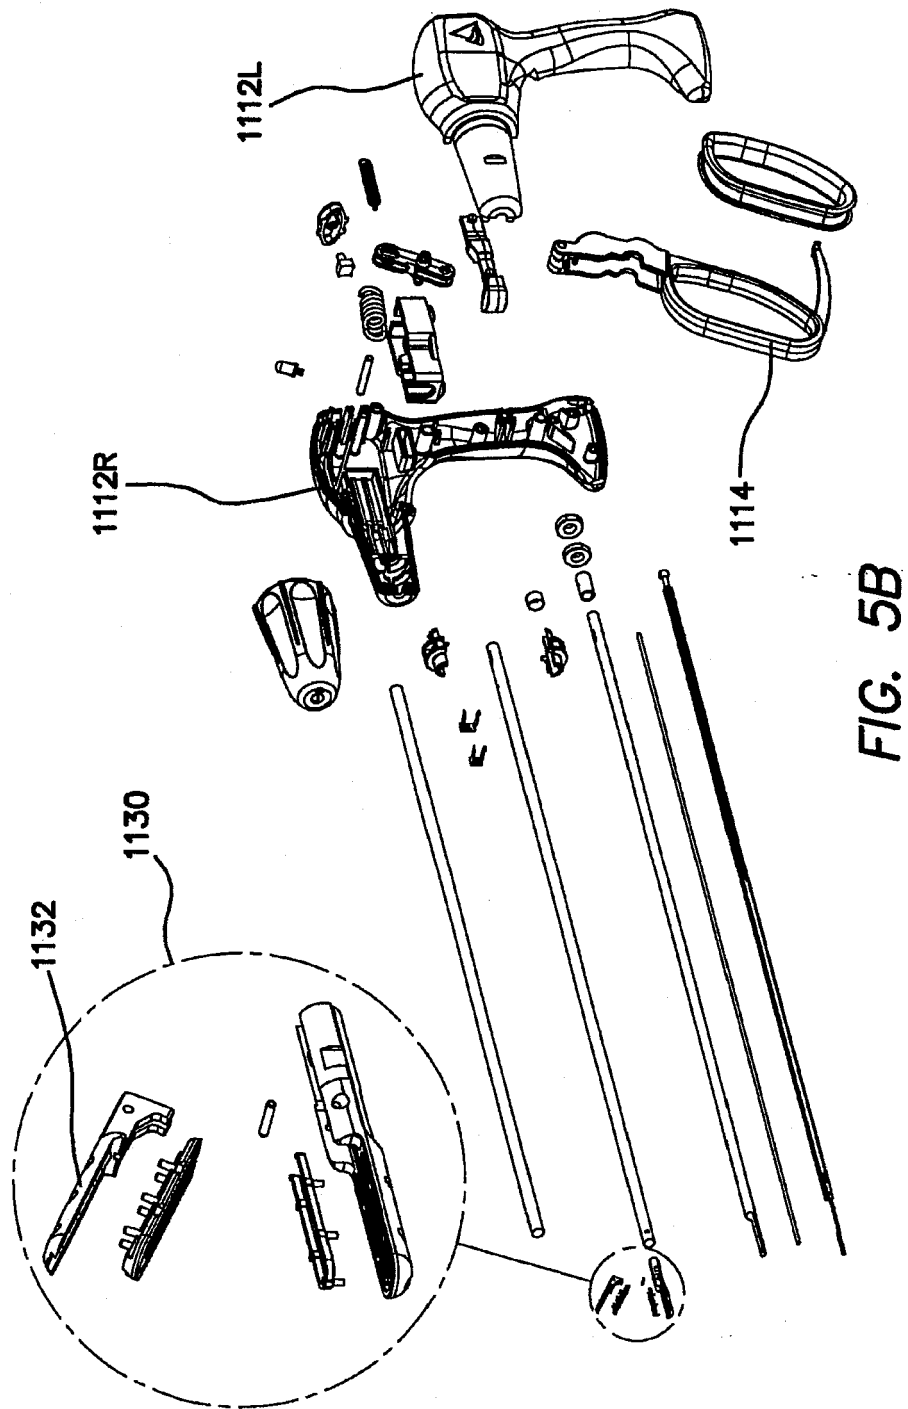


FIG. 5A



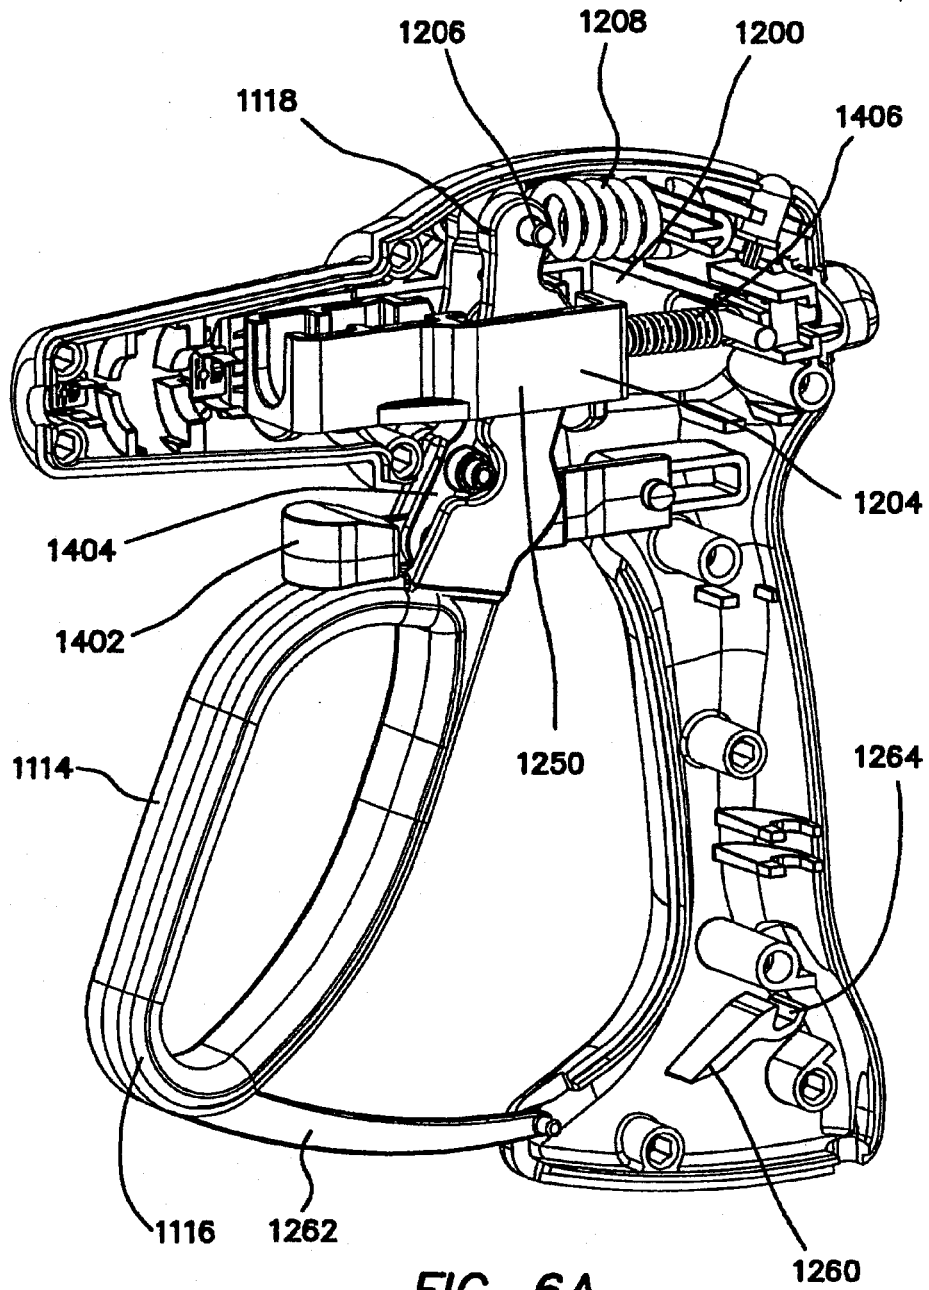


FIG. 6A

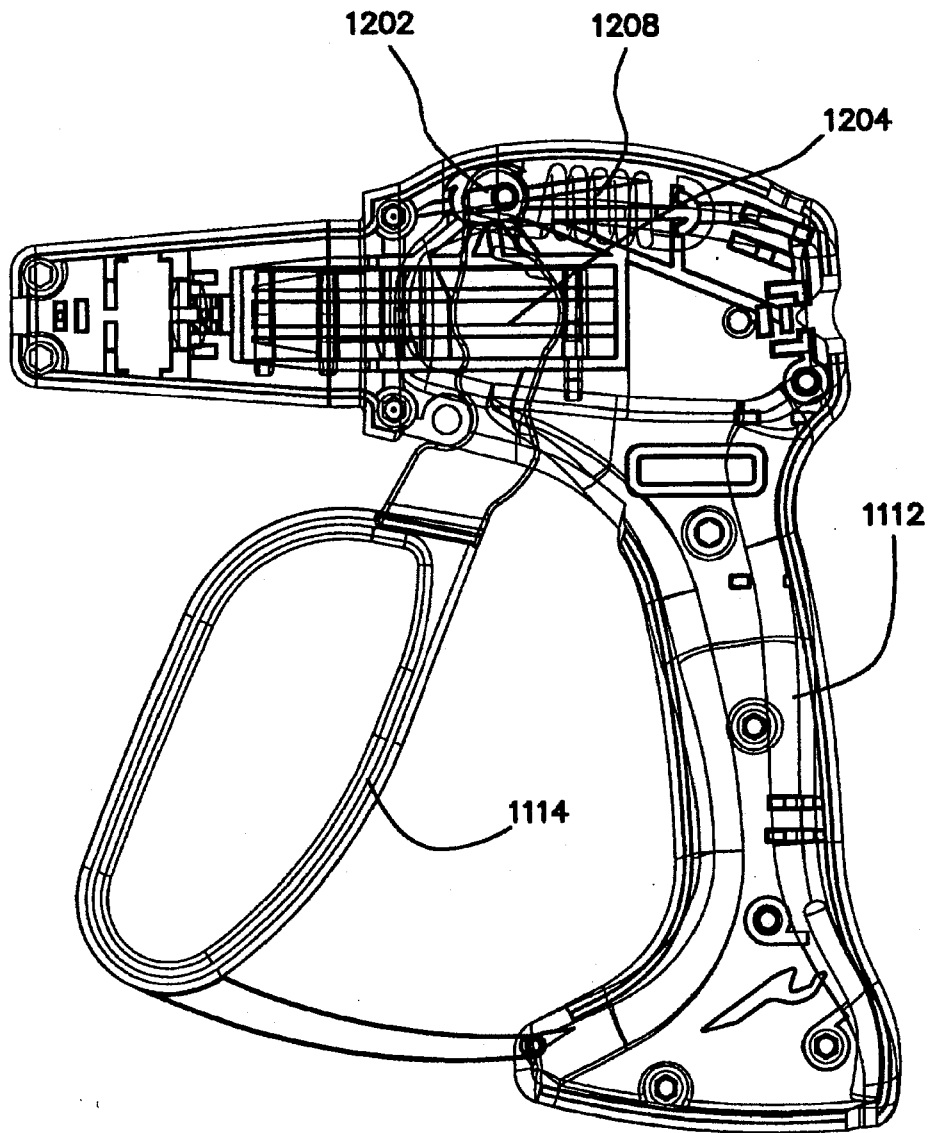


FIG. 6B

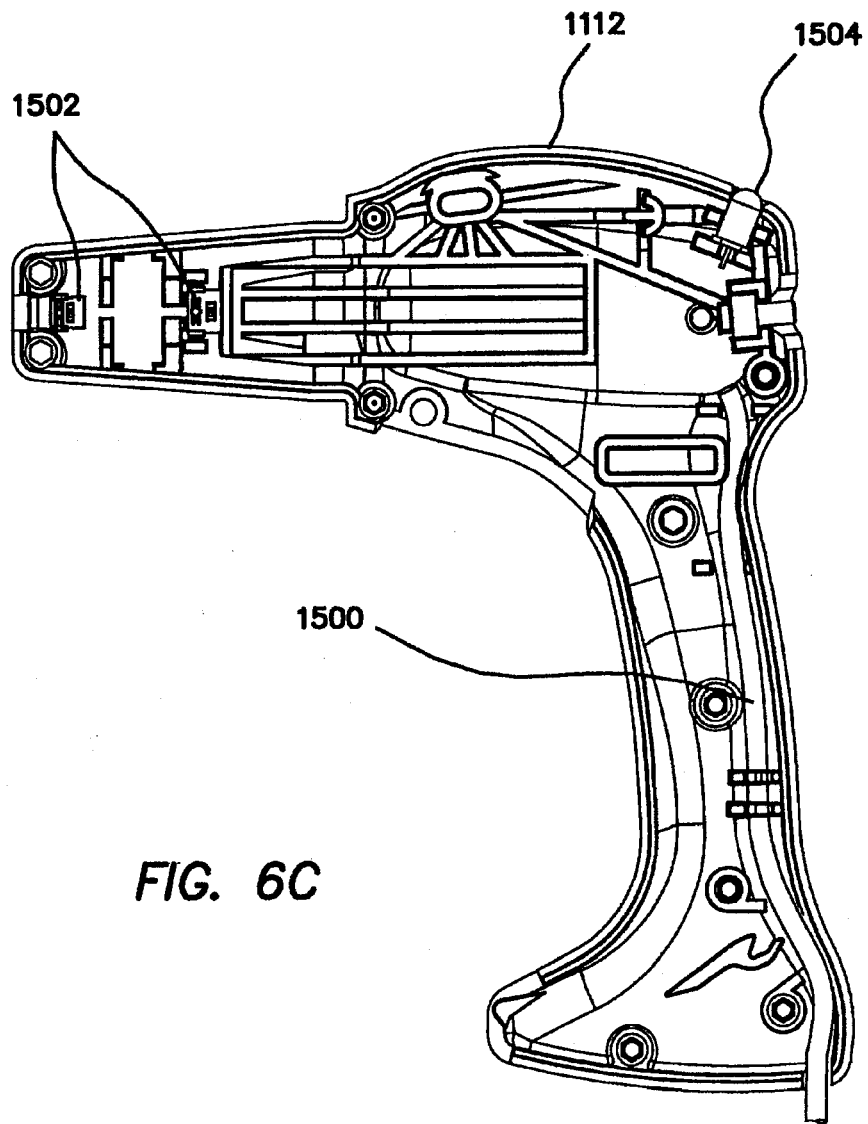


FIG. 6C

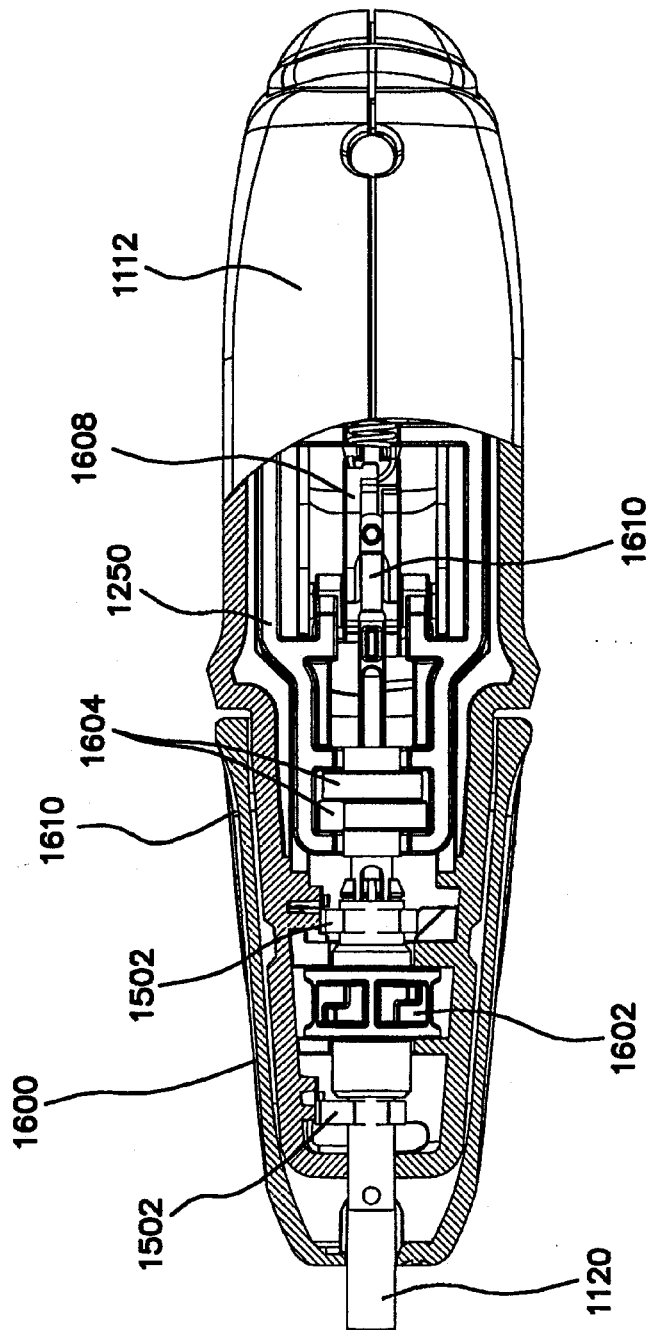


FIG. 7

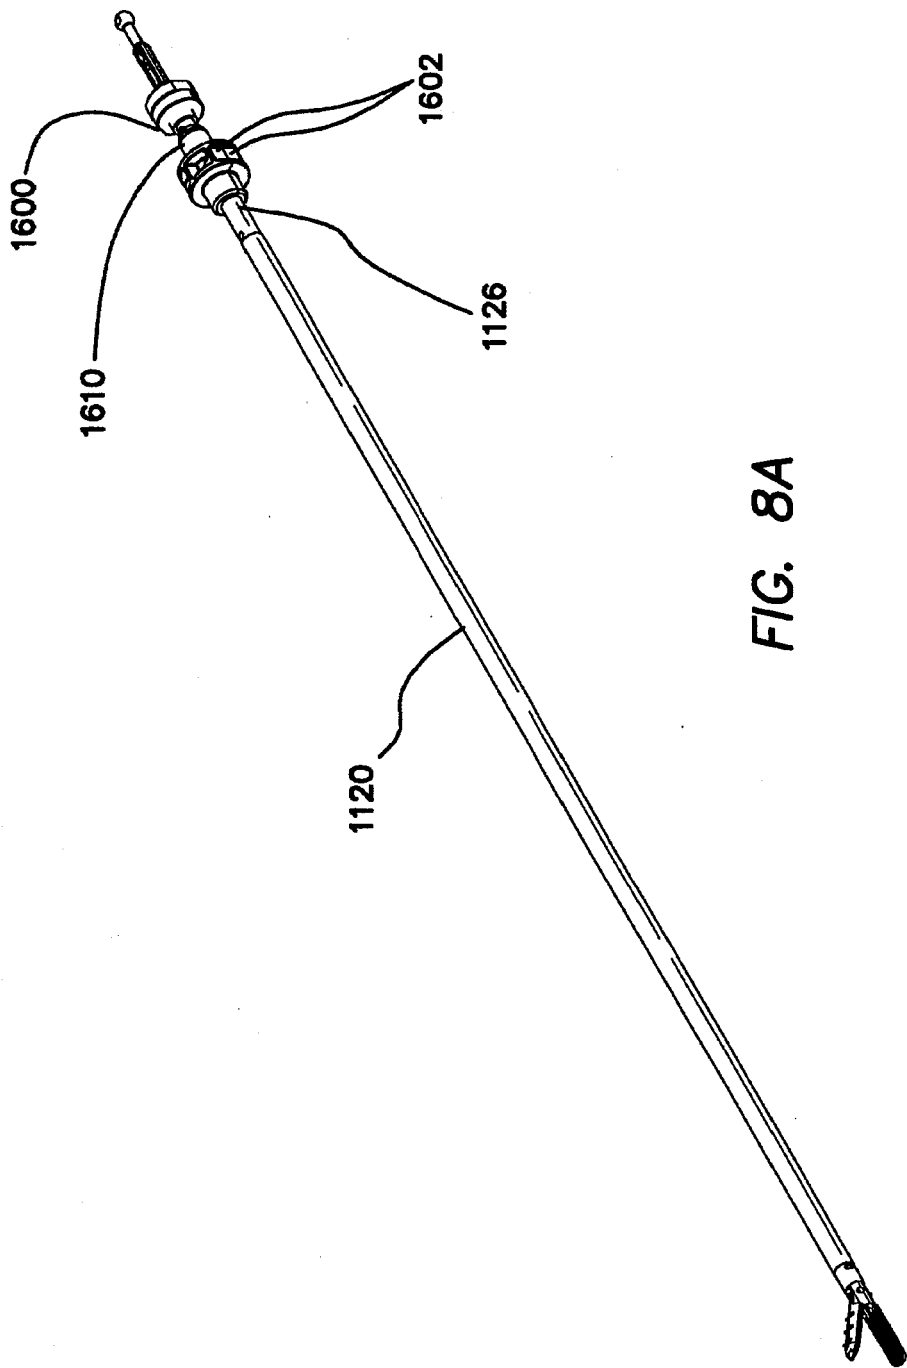


FIG. 8A

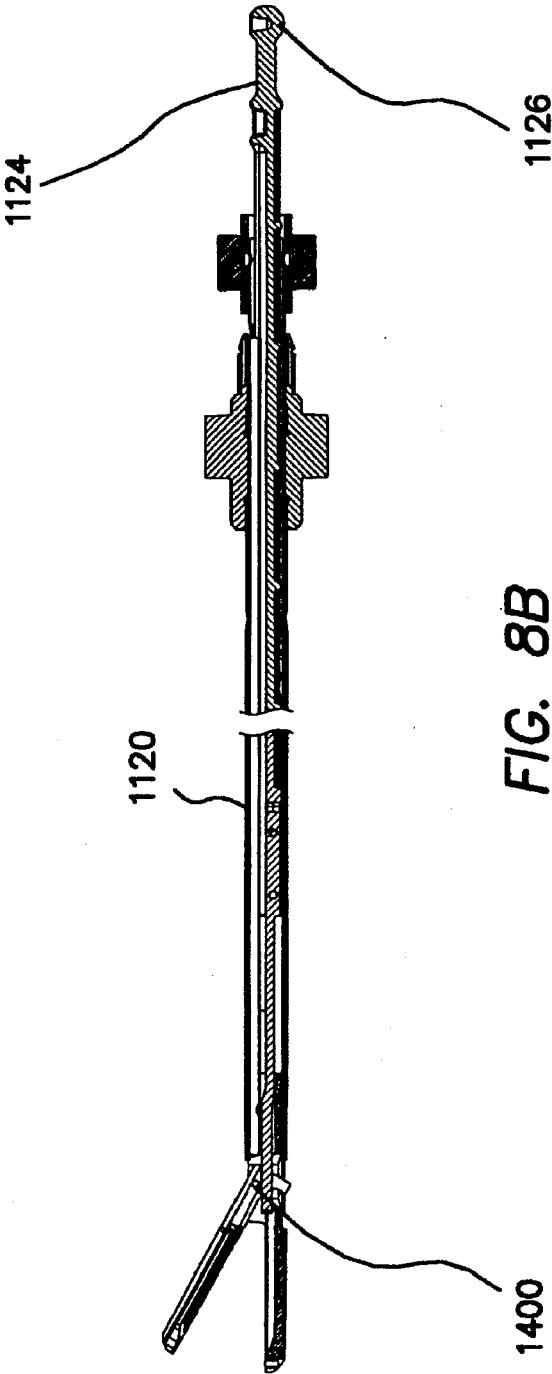


FIG. 8B

FIG. 8C-1

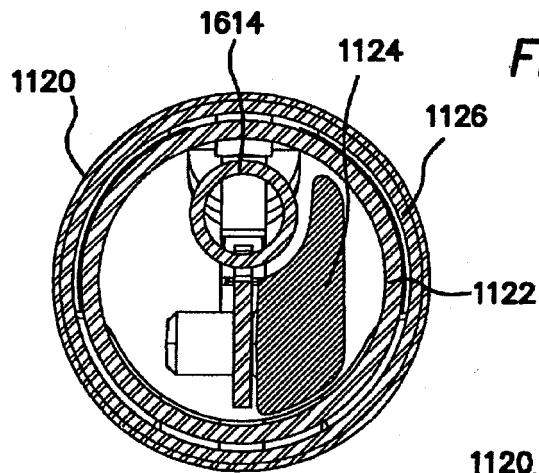


FIG. 8C-2

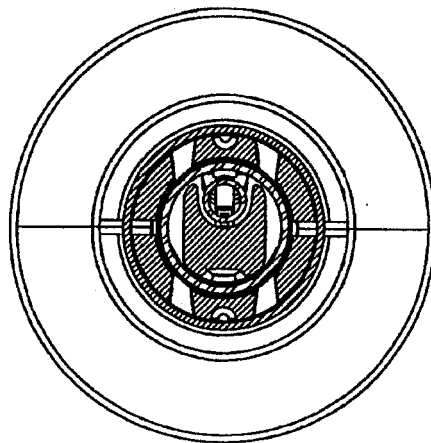
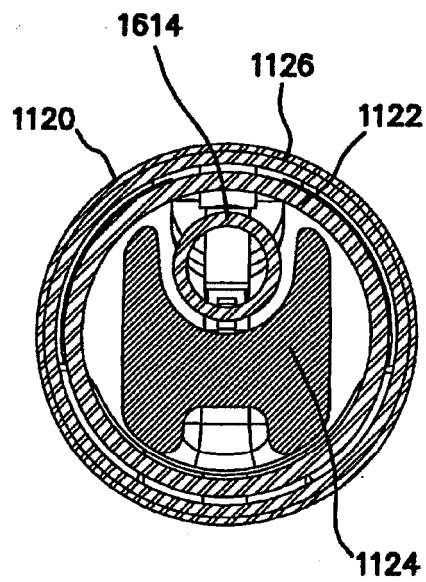


FIG. 8C-3

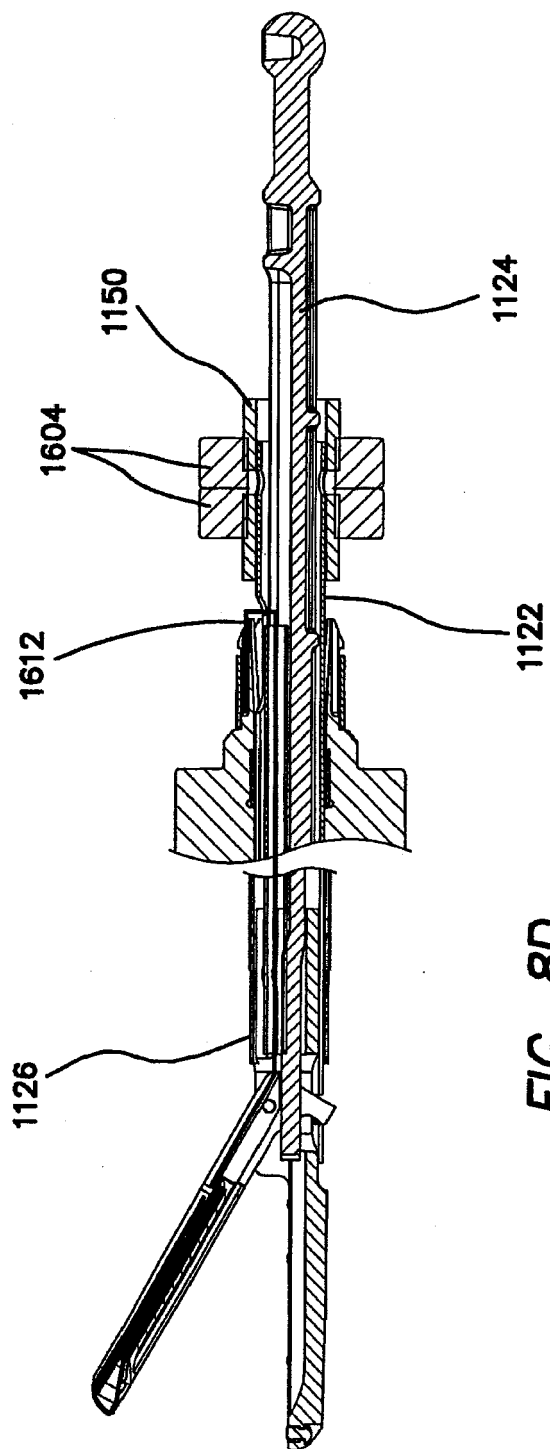


FIG. 8D

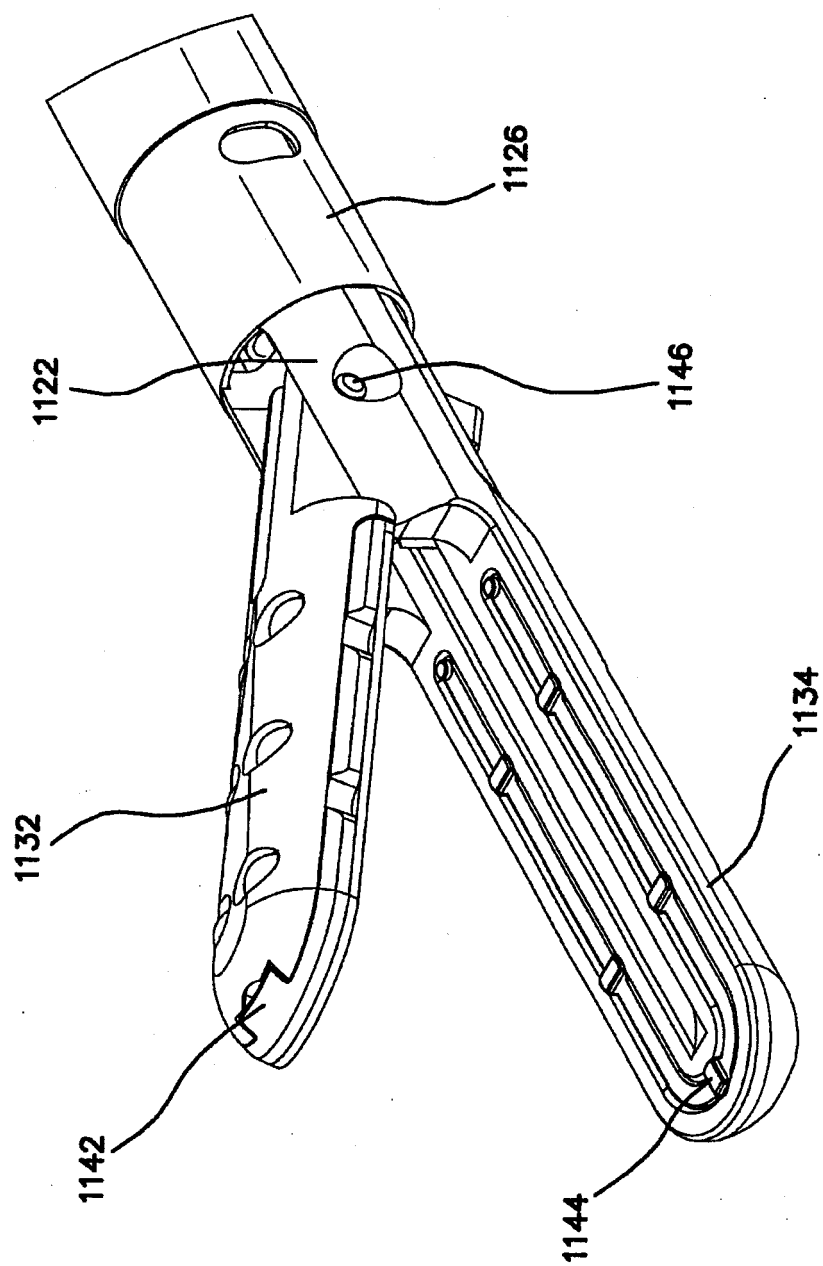


FIG. 9A

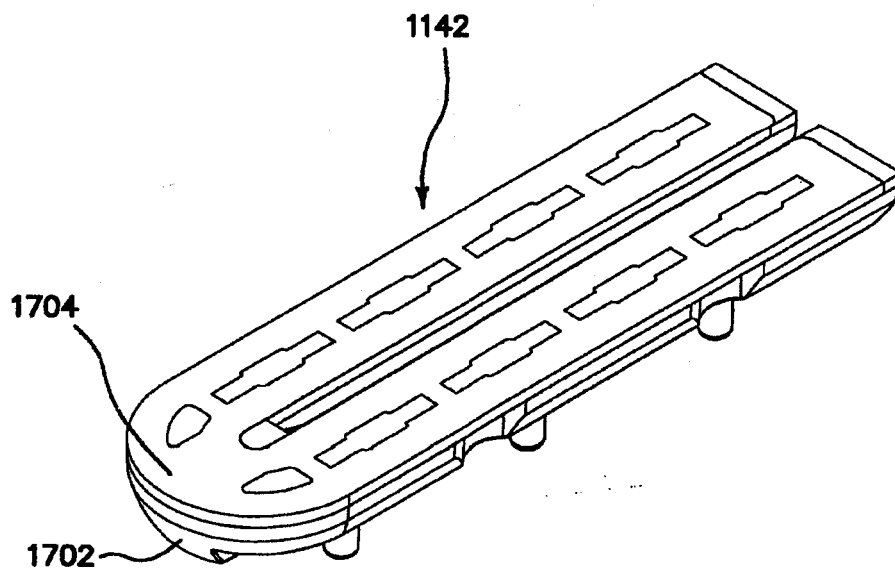
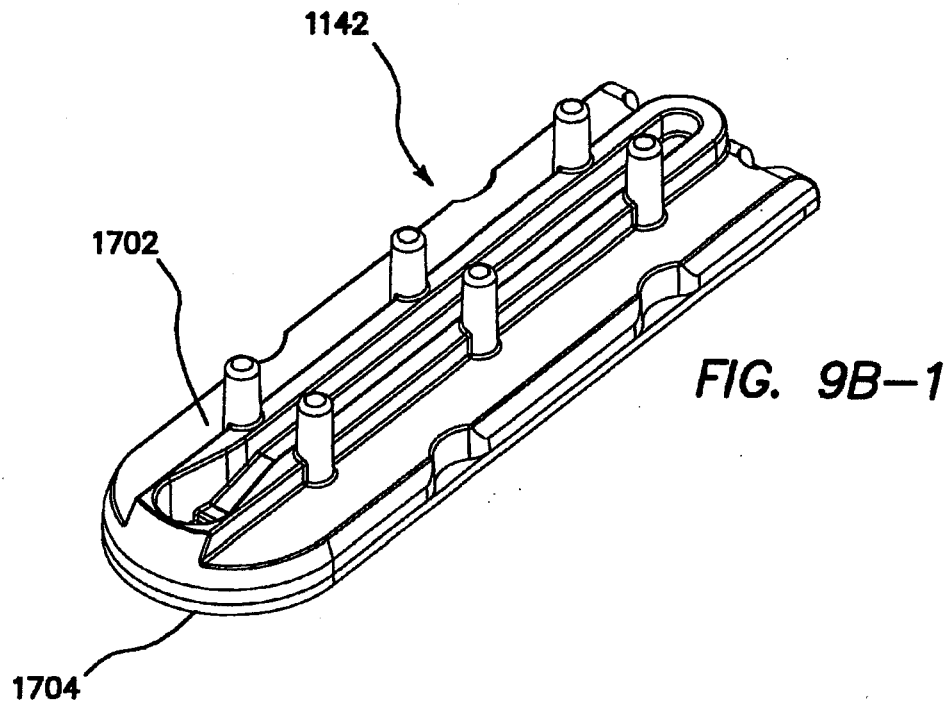
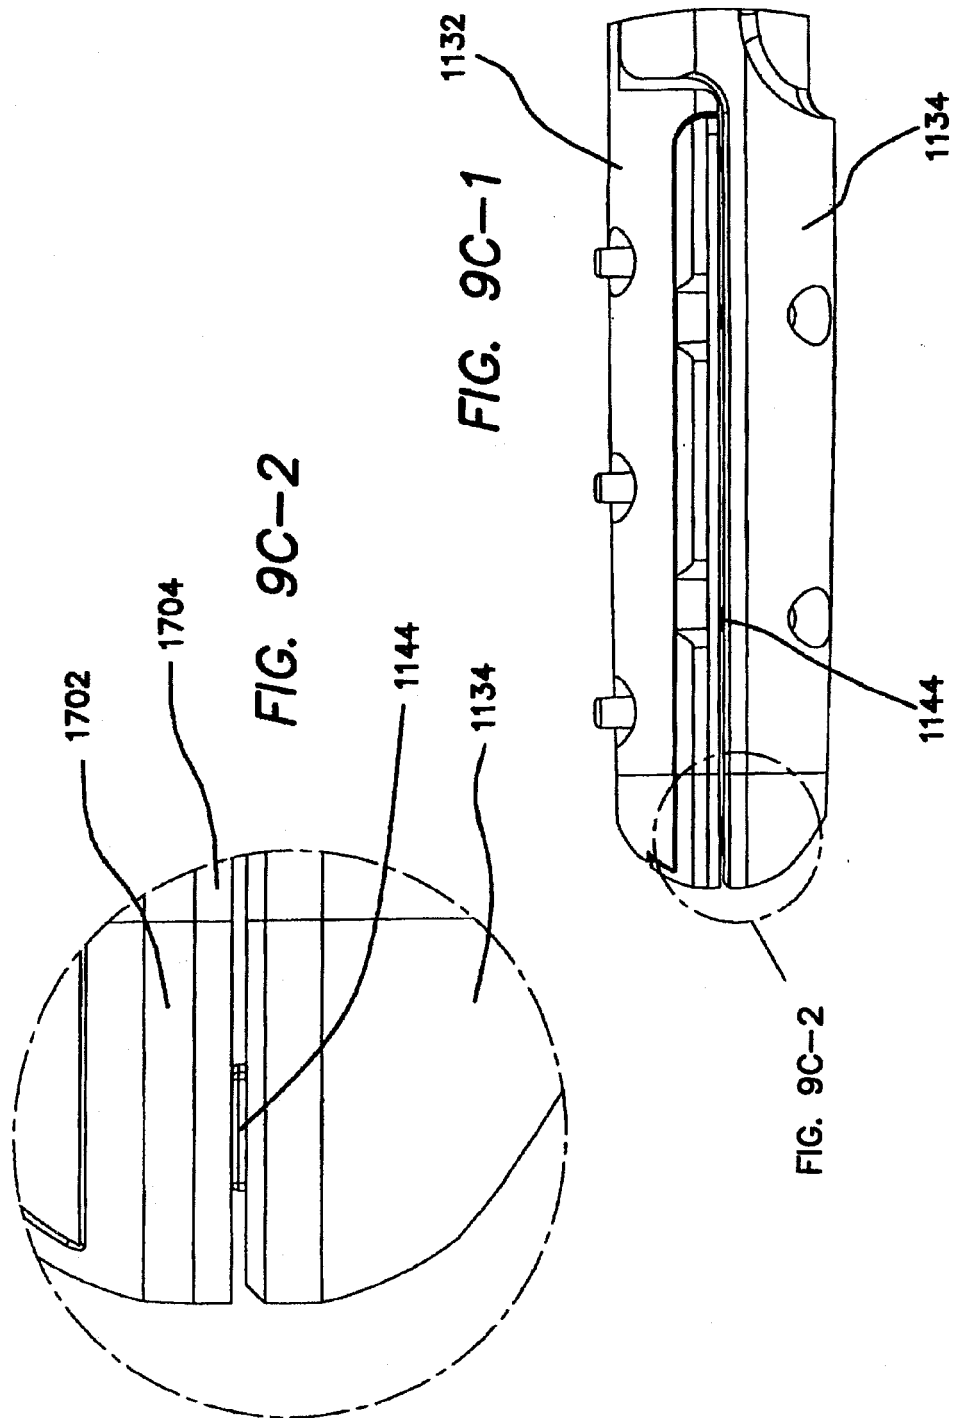


FIG. 9B-2



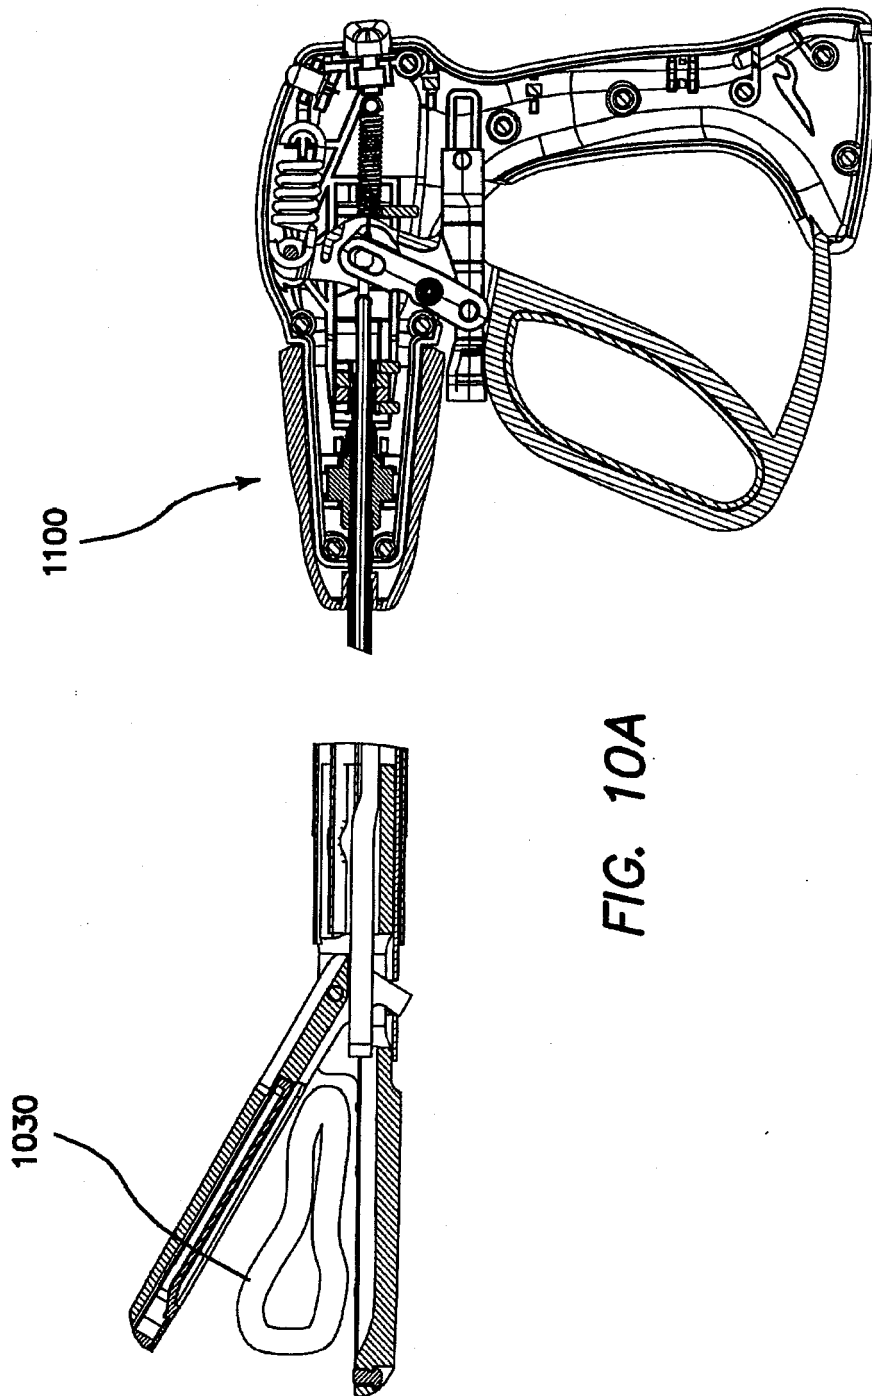
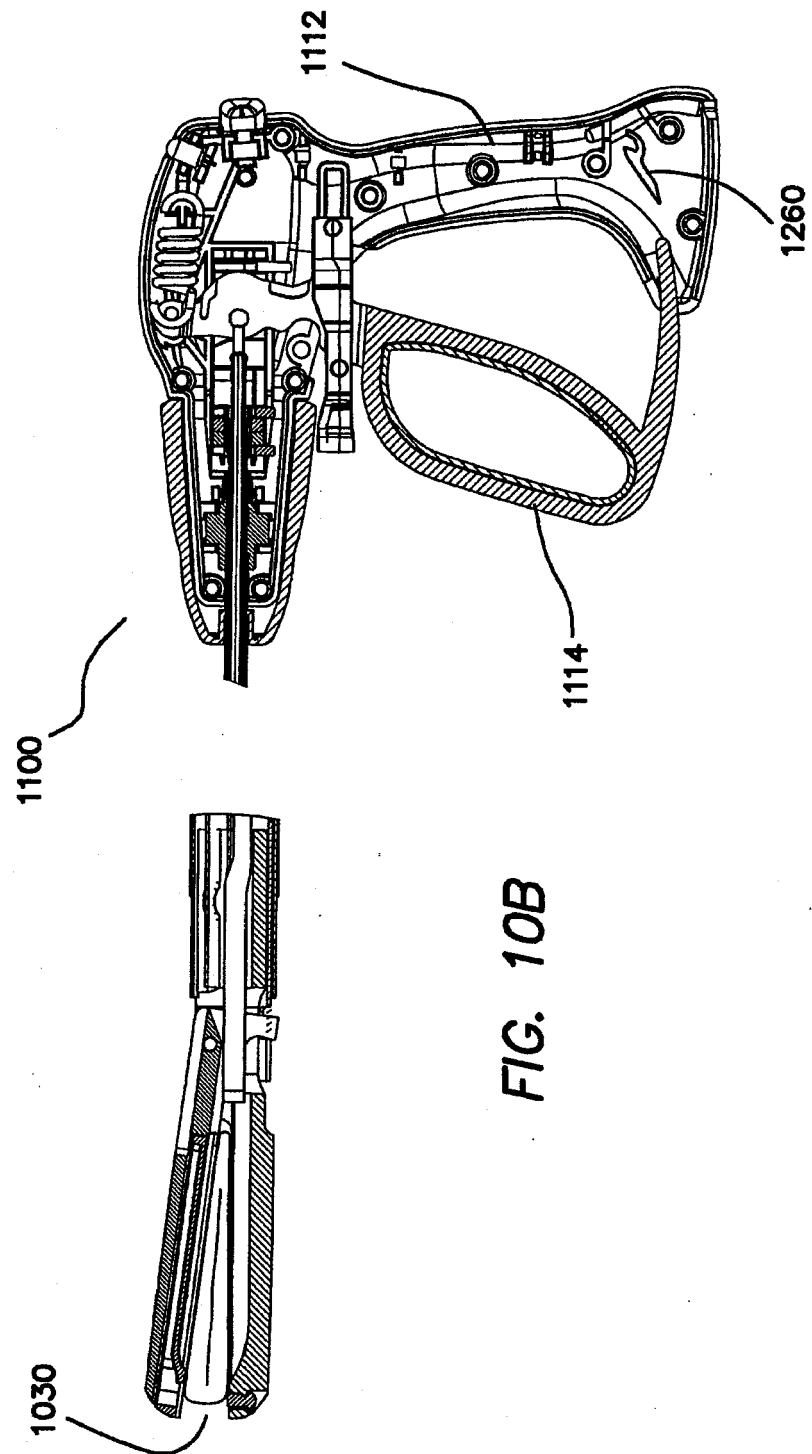
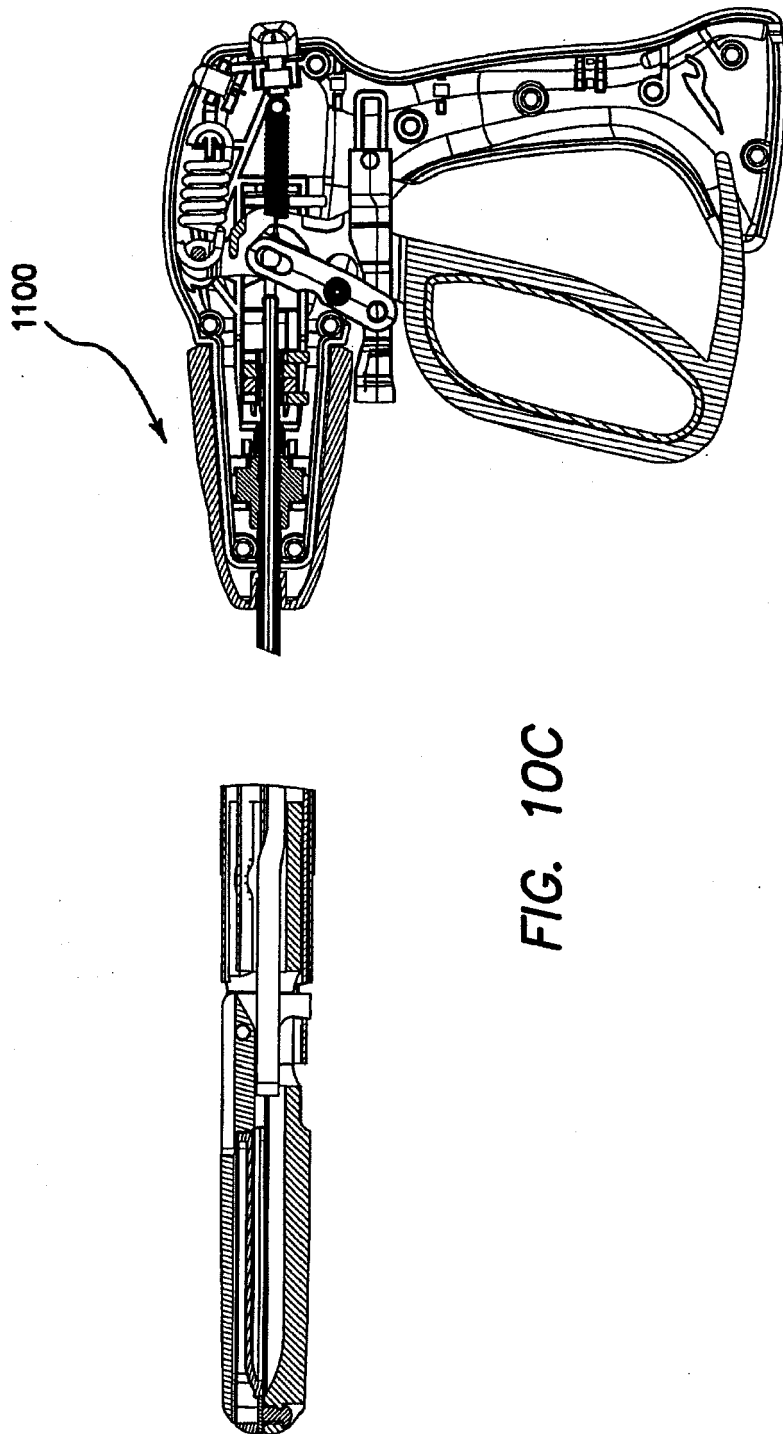
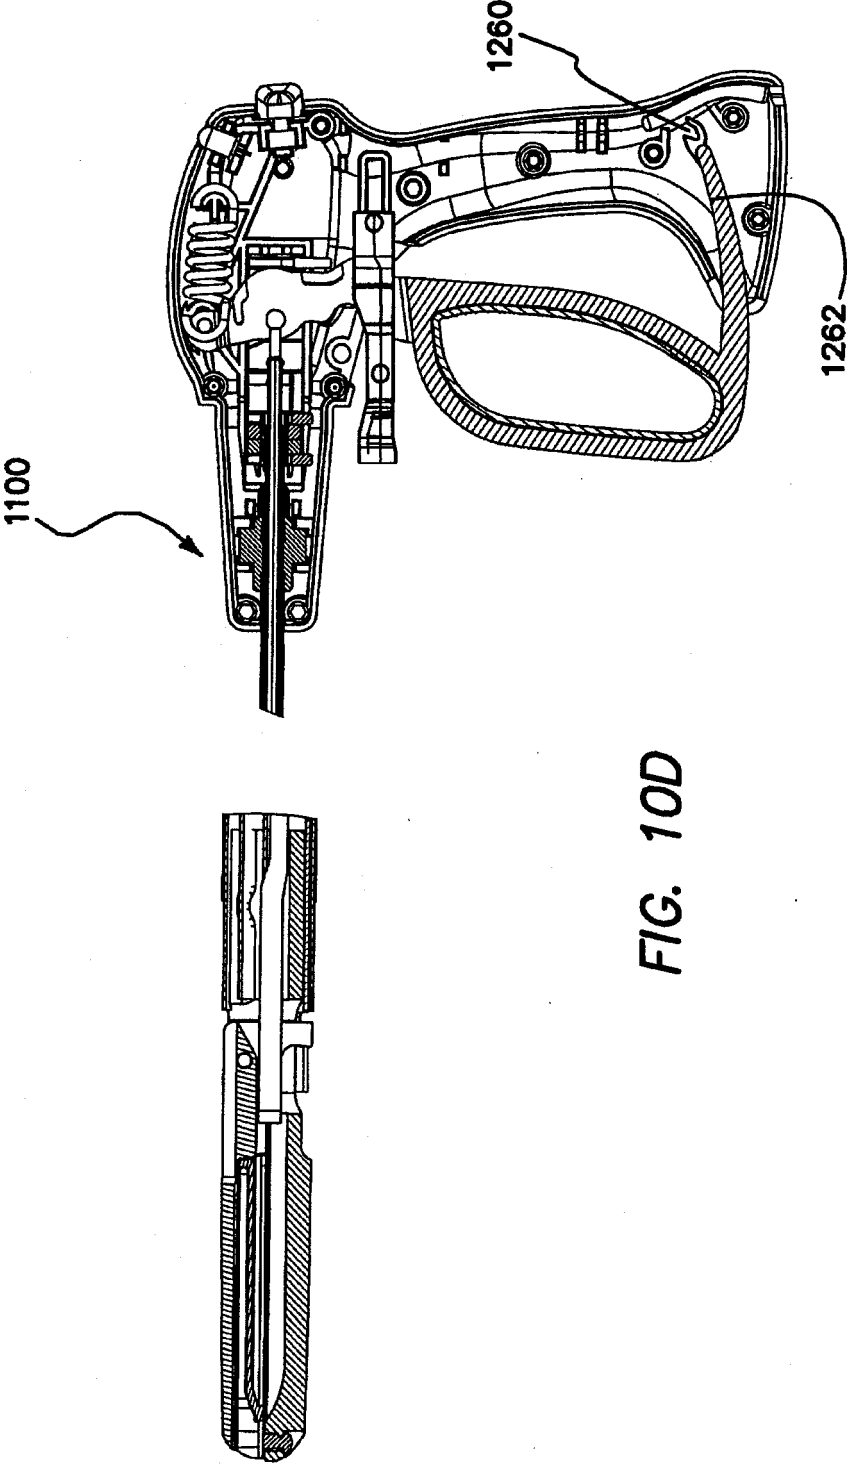


FIG. 10A







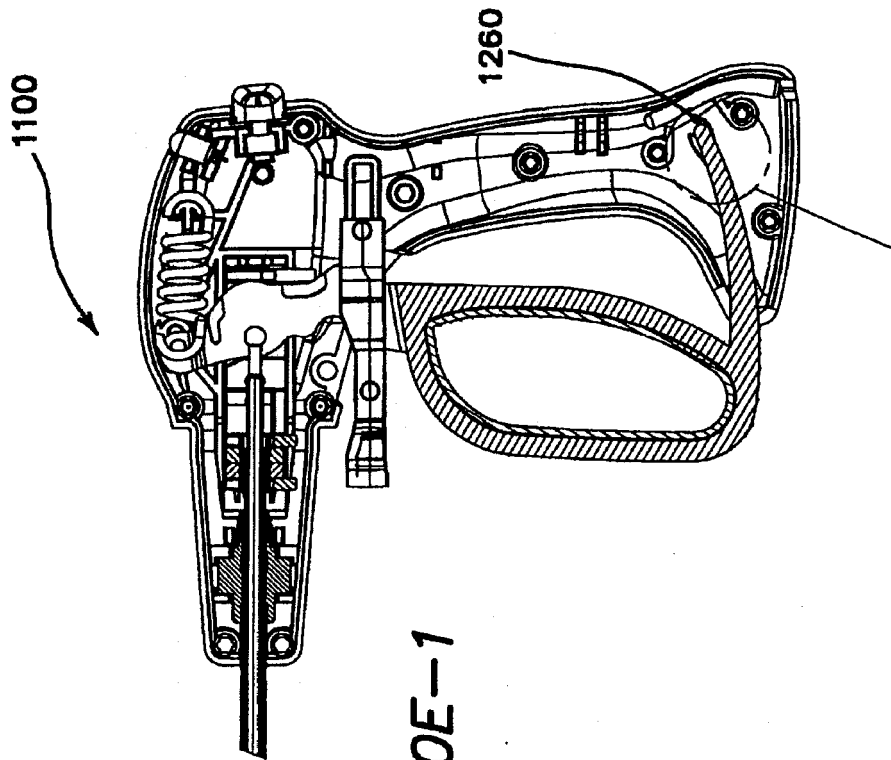


FIG. 10E-1

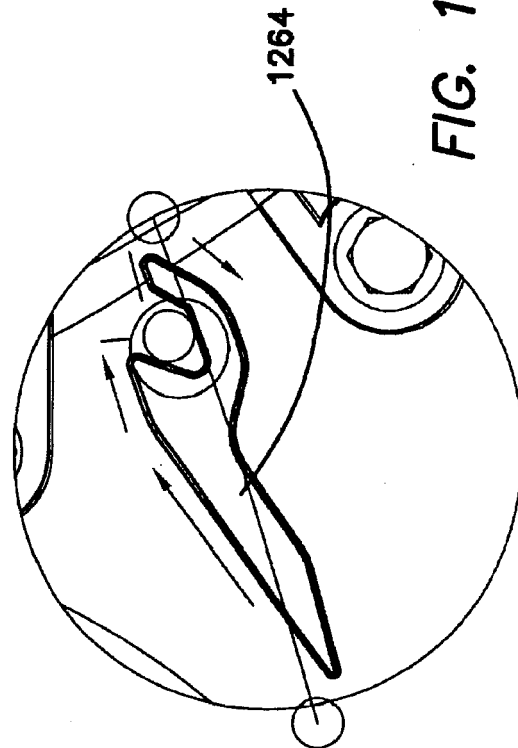



FIG. 10E-2

FIG. 10E-2

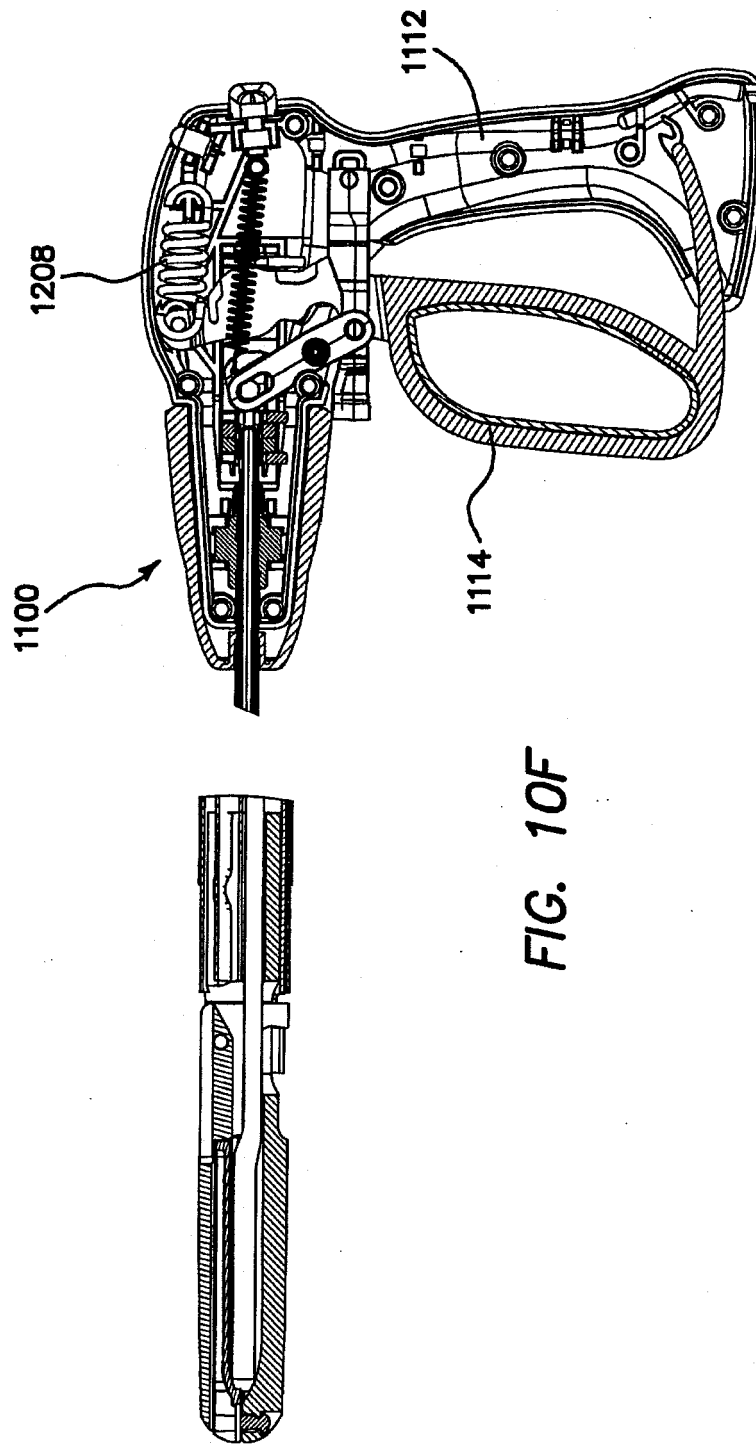
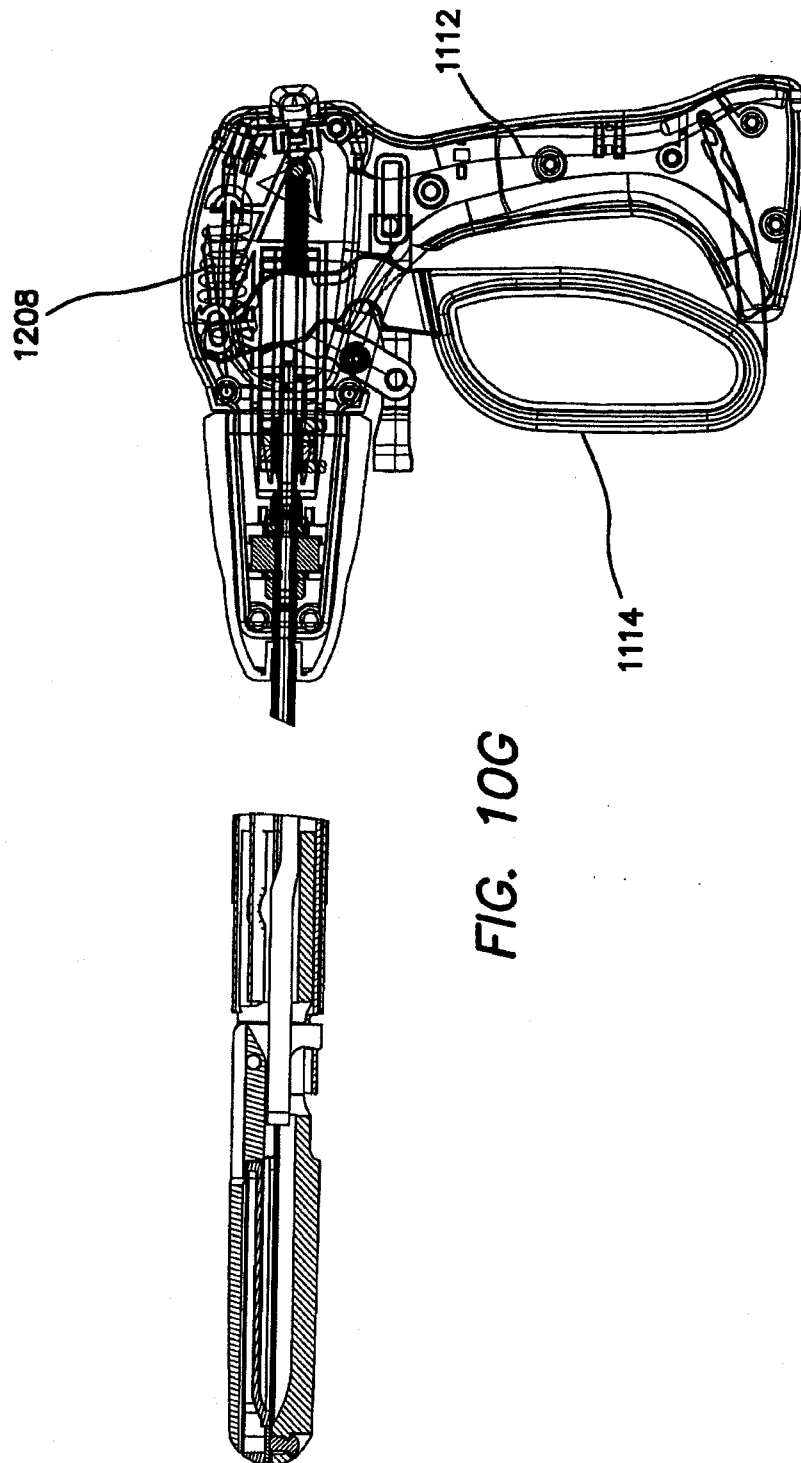
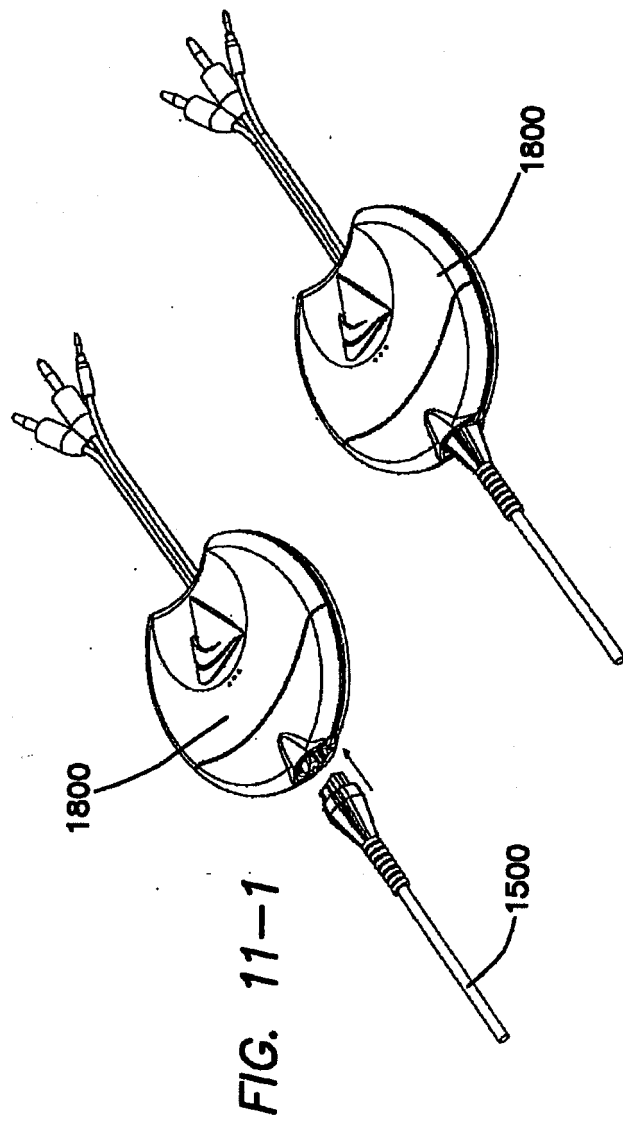


FIG. 10F





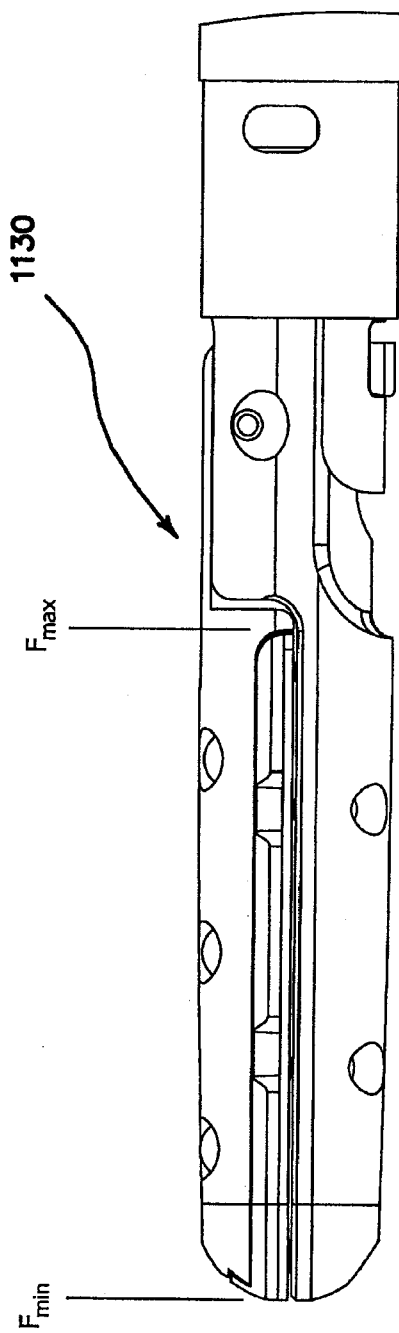


FIG. 12A

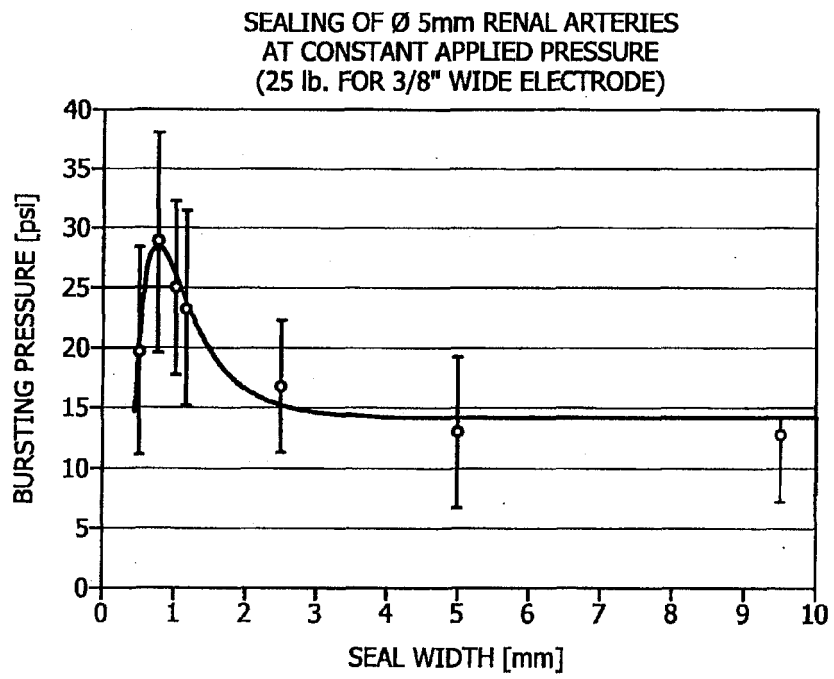


FIG. 12B

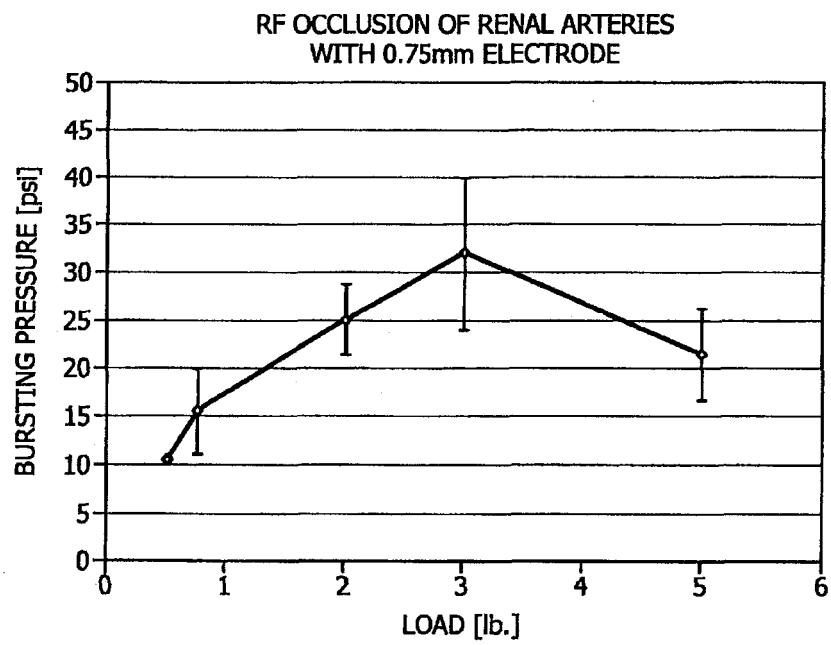


FIG. 12C

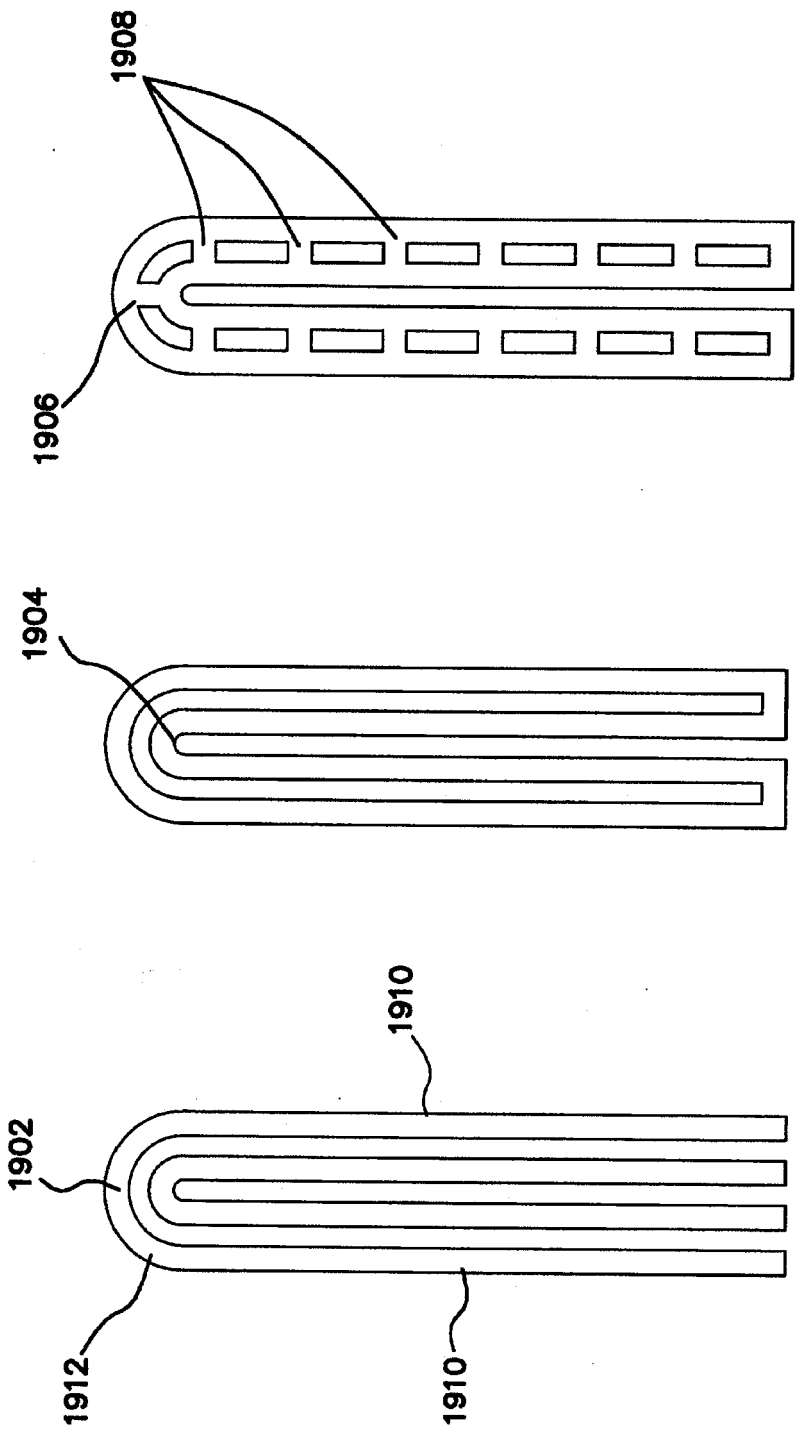


FIG. 13-3

FIG. 13-2

FIG. 13-1

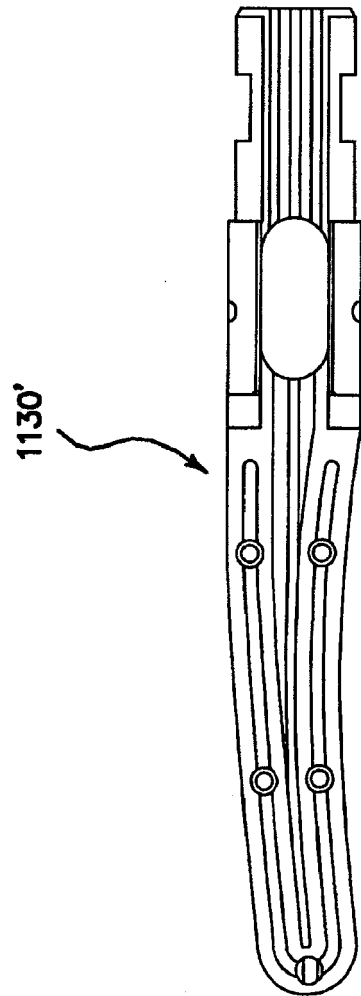


FIG. 14

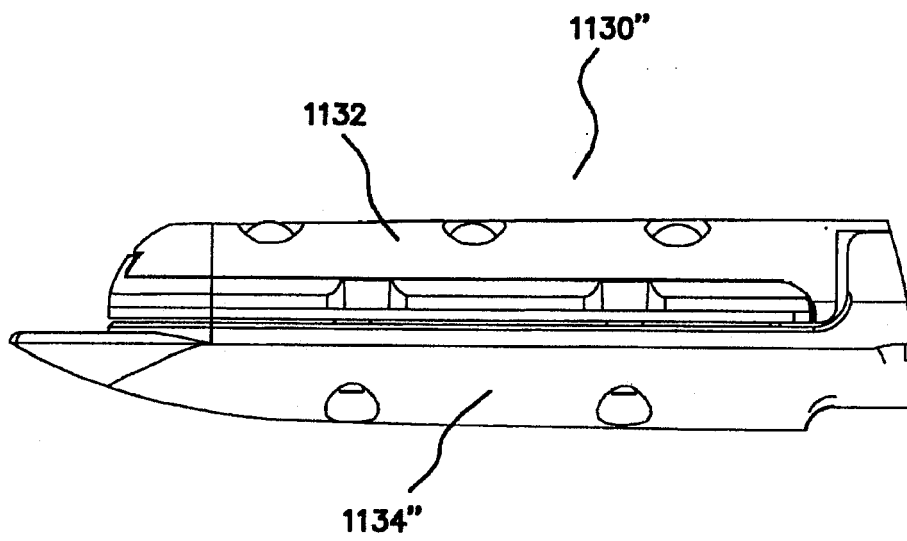


FIG. 15

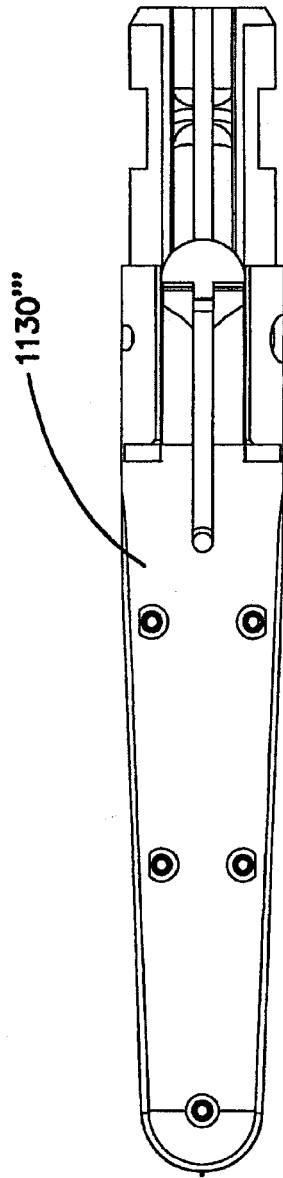


FIG. 16-1

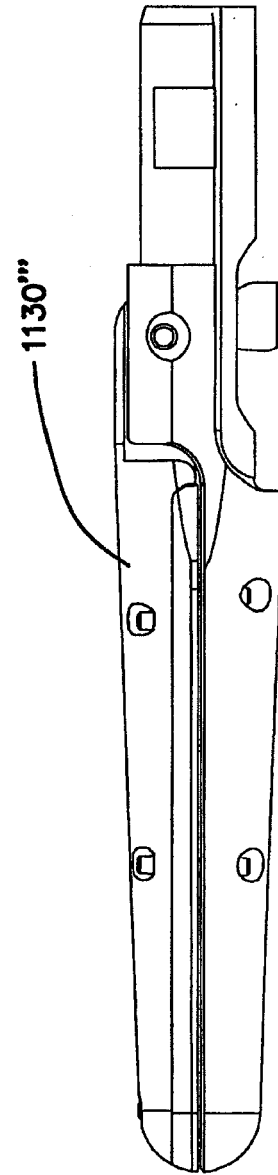
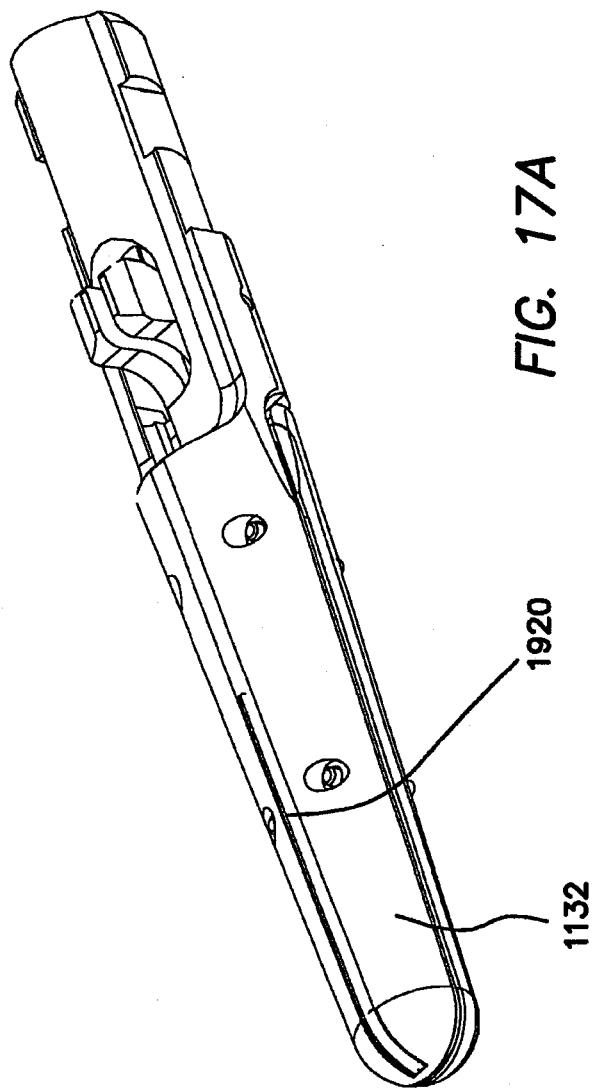


FIG. 16-2



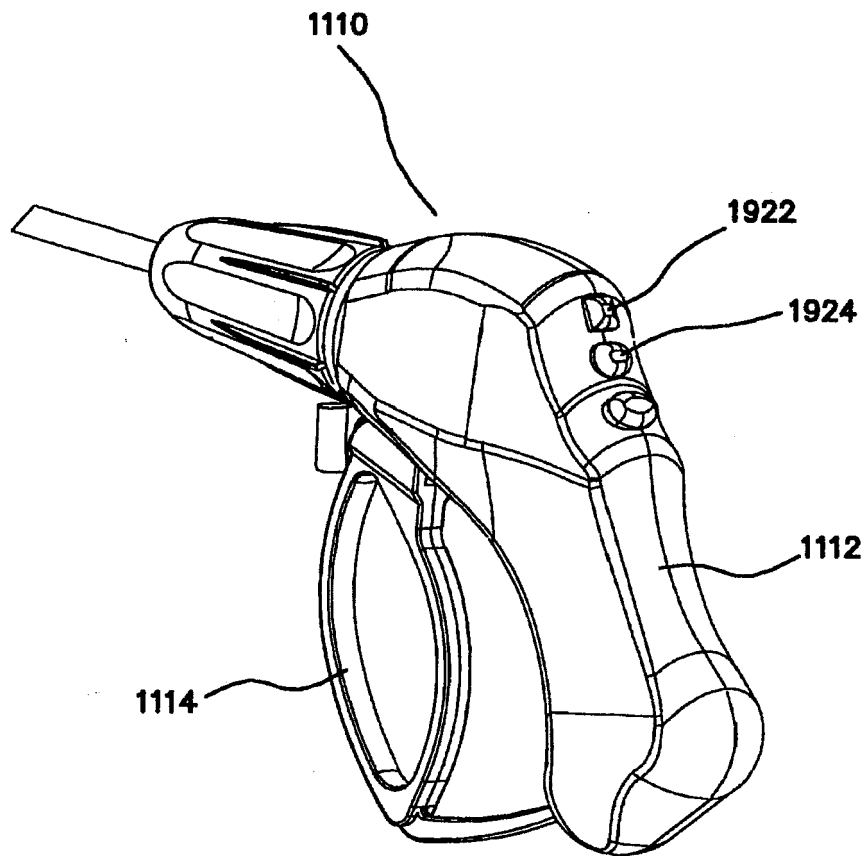
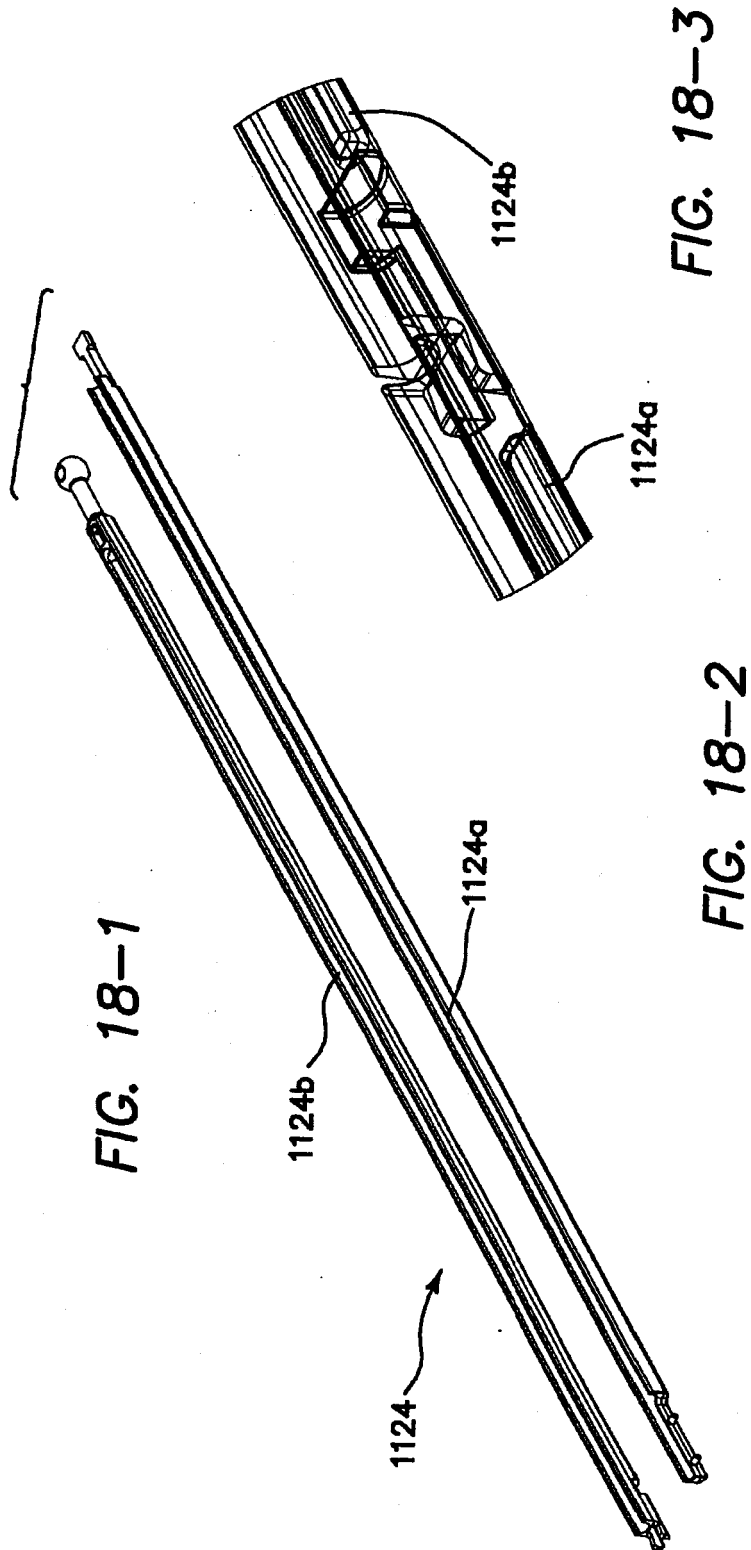
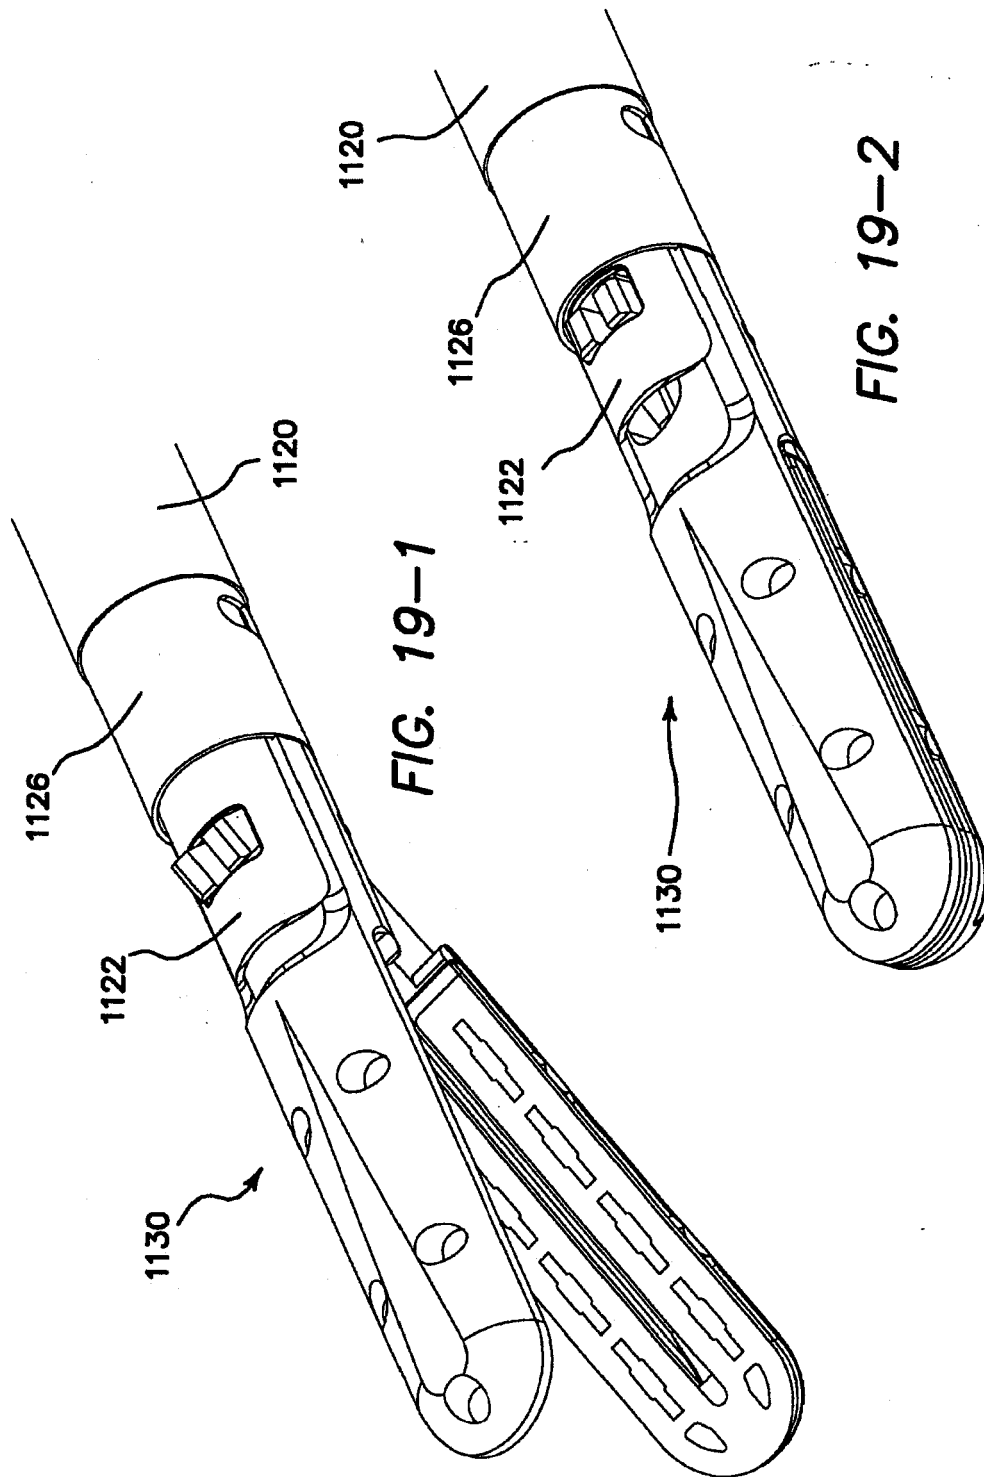


FIG. 17B





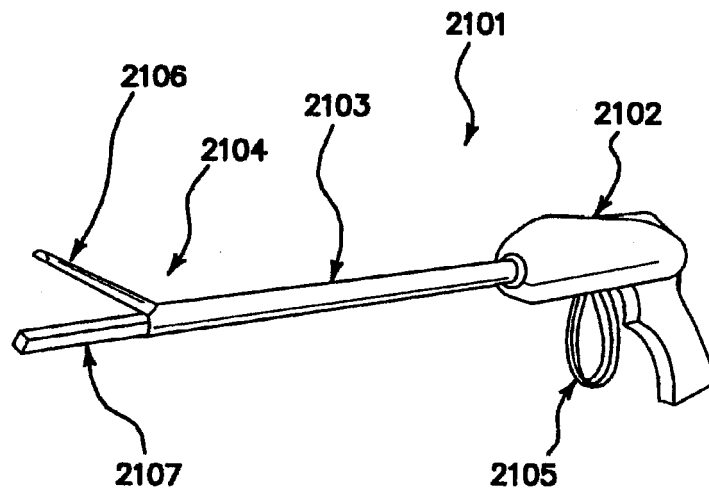


FIG. 20

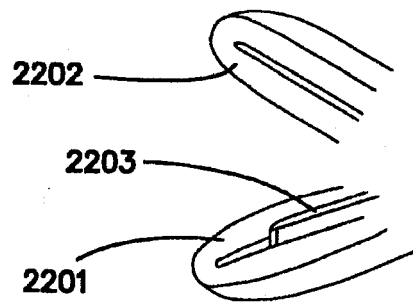


FIG. 21

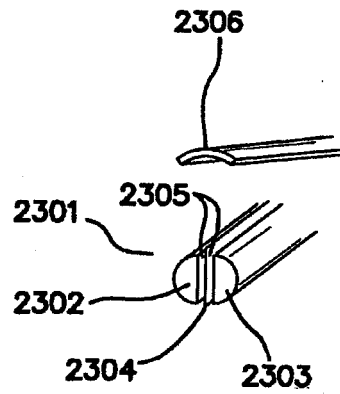


FIG. 22A

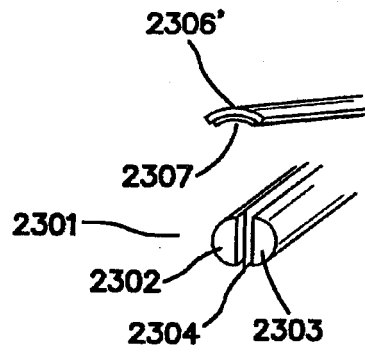


FIG. 22B

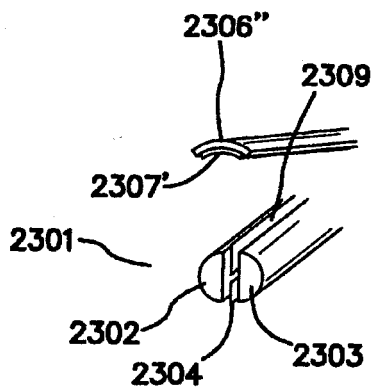


FIG. 22C

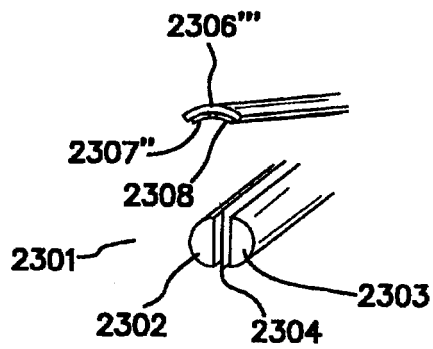
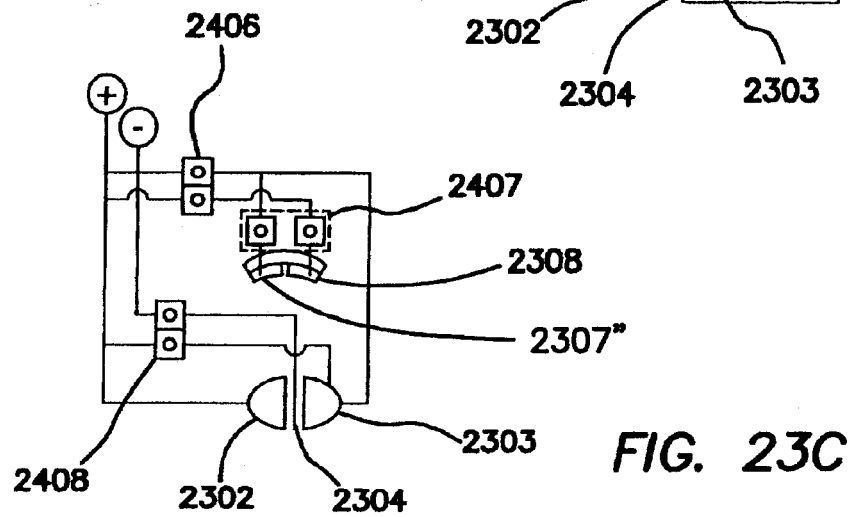
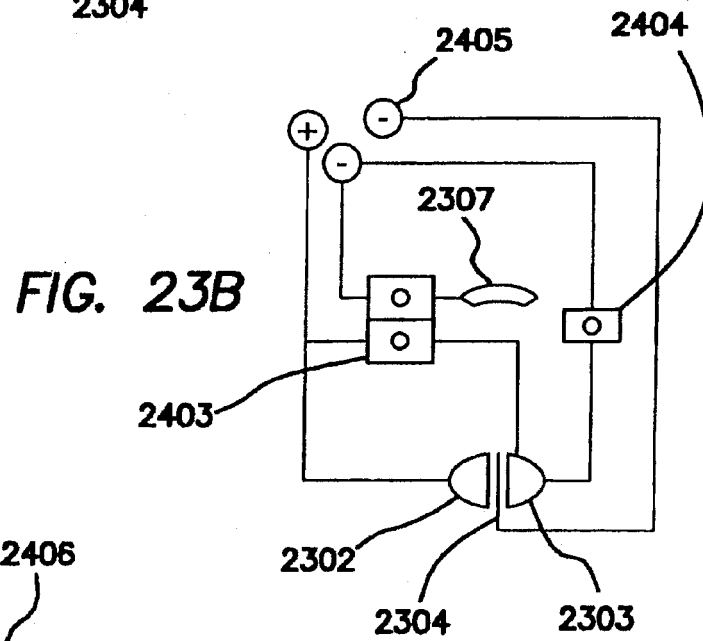
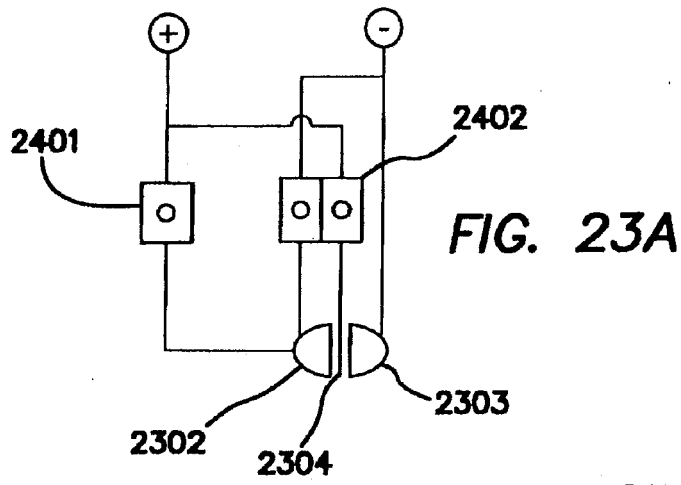


FIG. 22D



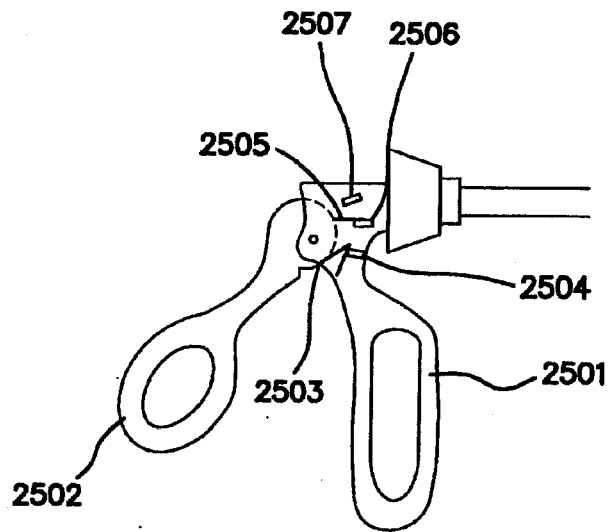


FIG. 24

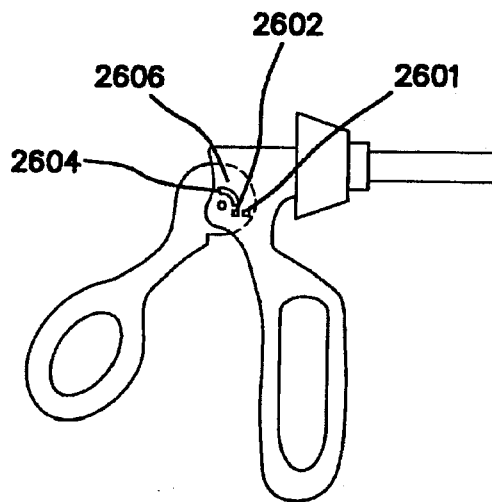


FIG. 25

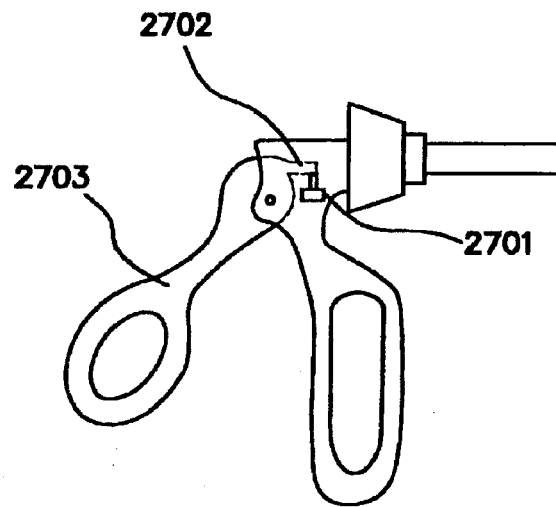


FIG. 26

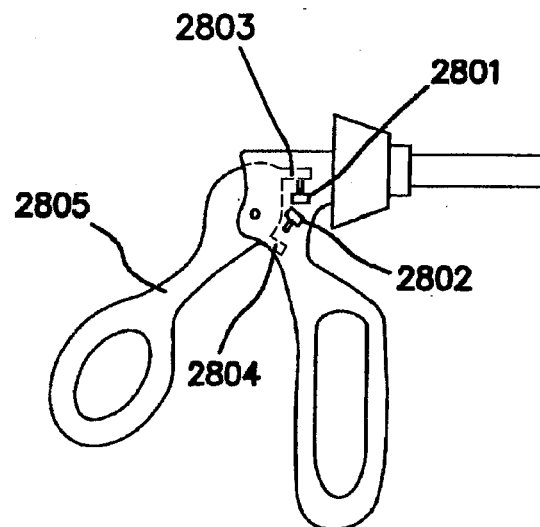


FIG. 27


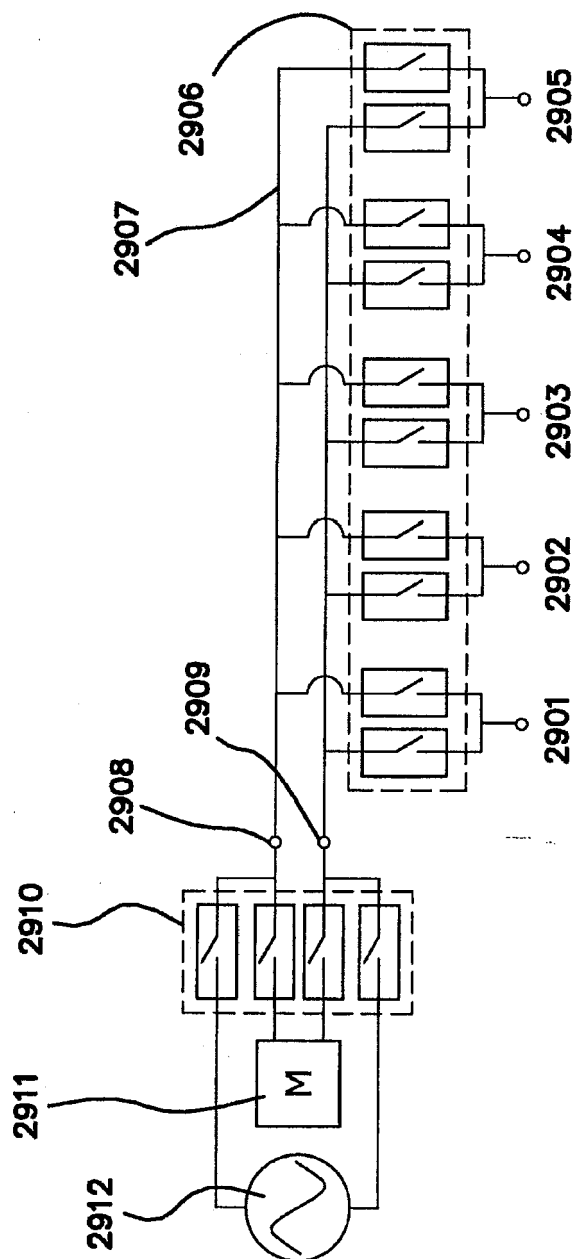


FIG. 28



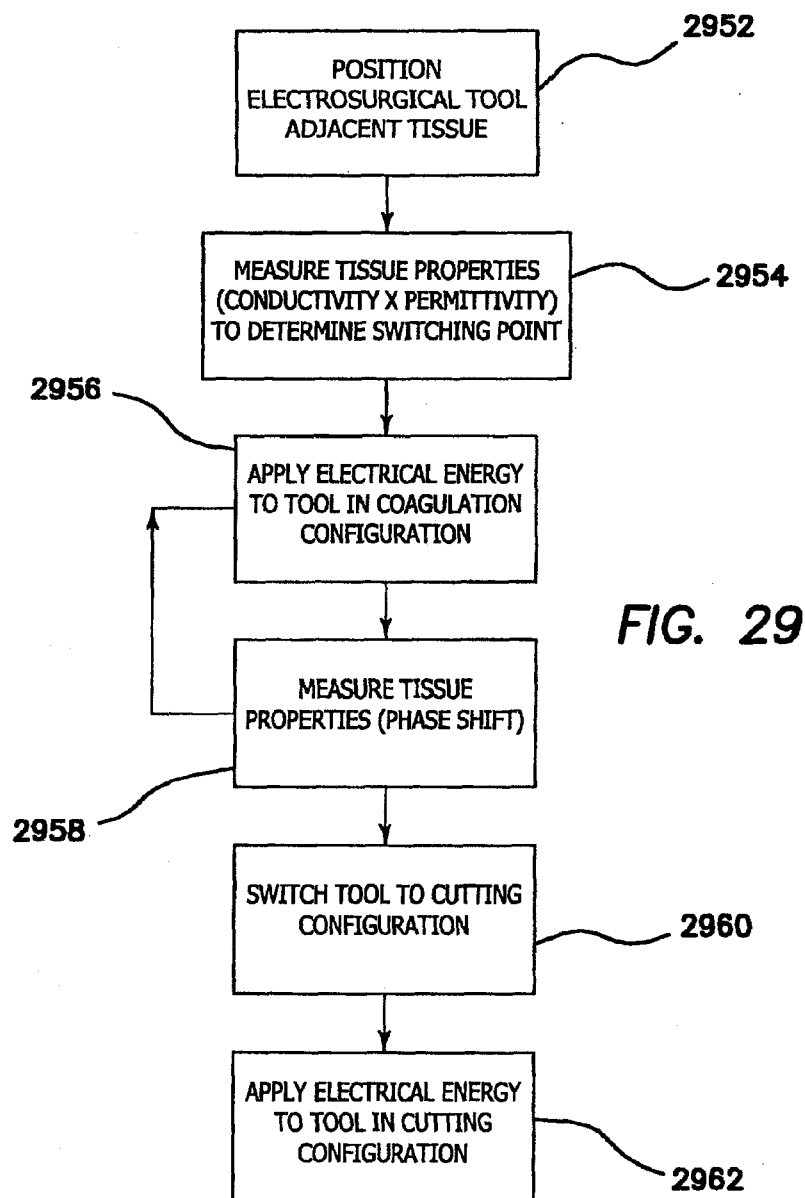

EUROPEAN SEARCH REPORT

Application Number
EP 10 19 2580

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (IPC)
X	US 6 270 497 B1 (SEKINO NAOMI [JP] ET AL) 7 August 2001 (2001-08-07) * column 5, lines 23-35; figures 1,3A-3C,14,15 * * column 12, lines 44-64 * * column 13, lines 23-46 * * column 14, line 34 - column 15, line 28; figures 18,19 * * column 14, lines 20-32; figure 17 * -----	1-15	INV. A61B18/14 ADD. A61B18/12 A61B18/00
X	US 2004/006340 A1 (LATTERELL SCOTT T [US] ET AL) 8 January 2004 (2004-01-08) * paragraphs [0027] - [0029], [0032]; figures 4,5,7 * -----	1	
A	US 5 234 427 A (OHTOMO NAOKI [JP] ET AL) 10 August 1993 (1993-08-10) * the whole document * -----	1-15	
A	WO 2006/125558 A1 (ERBE ELEKTROMEDIZIN [DE]; SCHNITZLER UWE [DE]) 30 November 2006 (2006-11-30) * the whole document * -----	1-15	TECHNICAL FIELDS SEARCHED (IPC) A61B
The present search report has been drawn up for all claims			
Place of search Munich		Date of completion of the search 21 July 2011	Examiner Monogiou, Efstratia
CATEGORY OF CITED DOCUMENTS X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document			

 1
EPO FORM 1503 03.82 (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 10 19 2580

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-07-2011

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 6270497 B1	07-08-2001	JP 4225624 B2	18-02-2009
		JP 2000135222 A	16-05-2000
US 2004006340 A1	08-01-2004	US 2004049185 A1	11-03-2004
US 5234427 A	10-08-1993	DE 69025849 D1	18-04-1996
		DE 69025849 T2	05-09-1996
		EP 0423757 A1	24-04-1991
		JP 2021833 C	26-02-1996
		JP 3133443 A	06-06-1991
		JP 7041044 B	10-05-1995
WO 2006125558 A1	30-11-2006	CN 101180003 A	14-05-2008
		DE 102005024221 A1	07-12-2006
		EP 1895924 A1	12-03-2008
		JP 2008541806 A	27-11-2008
		US 2009076504 A1	19-03-2009