



(86) Date de dépôt PCT/PCT Filing Date: 2016/01/14
(87) Date publication PCT/PCT Publication Date: 2016/07/21
(85) Entrée phase nationale/National Entry: 2017/06/29
(86) N° demande PCT/PCT Application No.: US 2016/013456
(87) N° publication PCT/PCT Publication No.: 2016/115379
(30) Priorité/Priority: 2015/01/14 (US62/103,485)

(51) Cl.Int./Int.Cl. *A61M 15/00* (2006.01)
(71) Demandeur/Applicant:
RESPIRA THERAPEUTICS, INC., US
(72) Inventeurs/Inventors:
CURTIS, ROBERT M., US;
DEATON, DAN, US;
HANNON, JAMES, US;
SMYTH, HUGH, US;
XU, ZHEN, US;
DONOVAN, MARTIN, US;
GIBBONS, AILEEN, US
(74) Agent: OYEN WIGGS GREEN & MUTALA LLP

(54) Titre : PROCÉDES ET DISPOSITIFS DE DISPERSION DE POUDRE
(54) Title: POWDER DISPERSION METHODS AND DEVICES

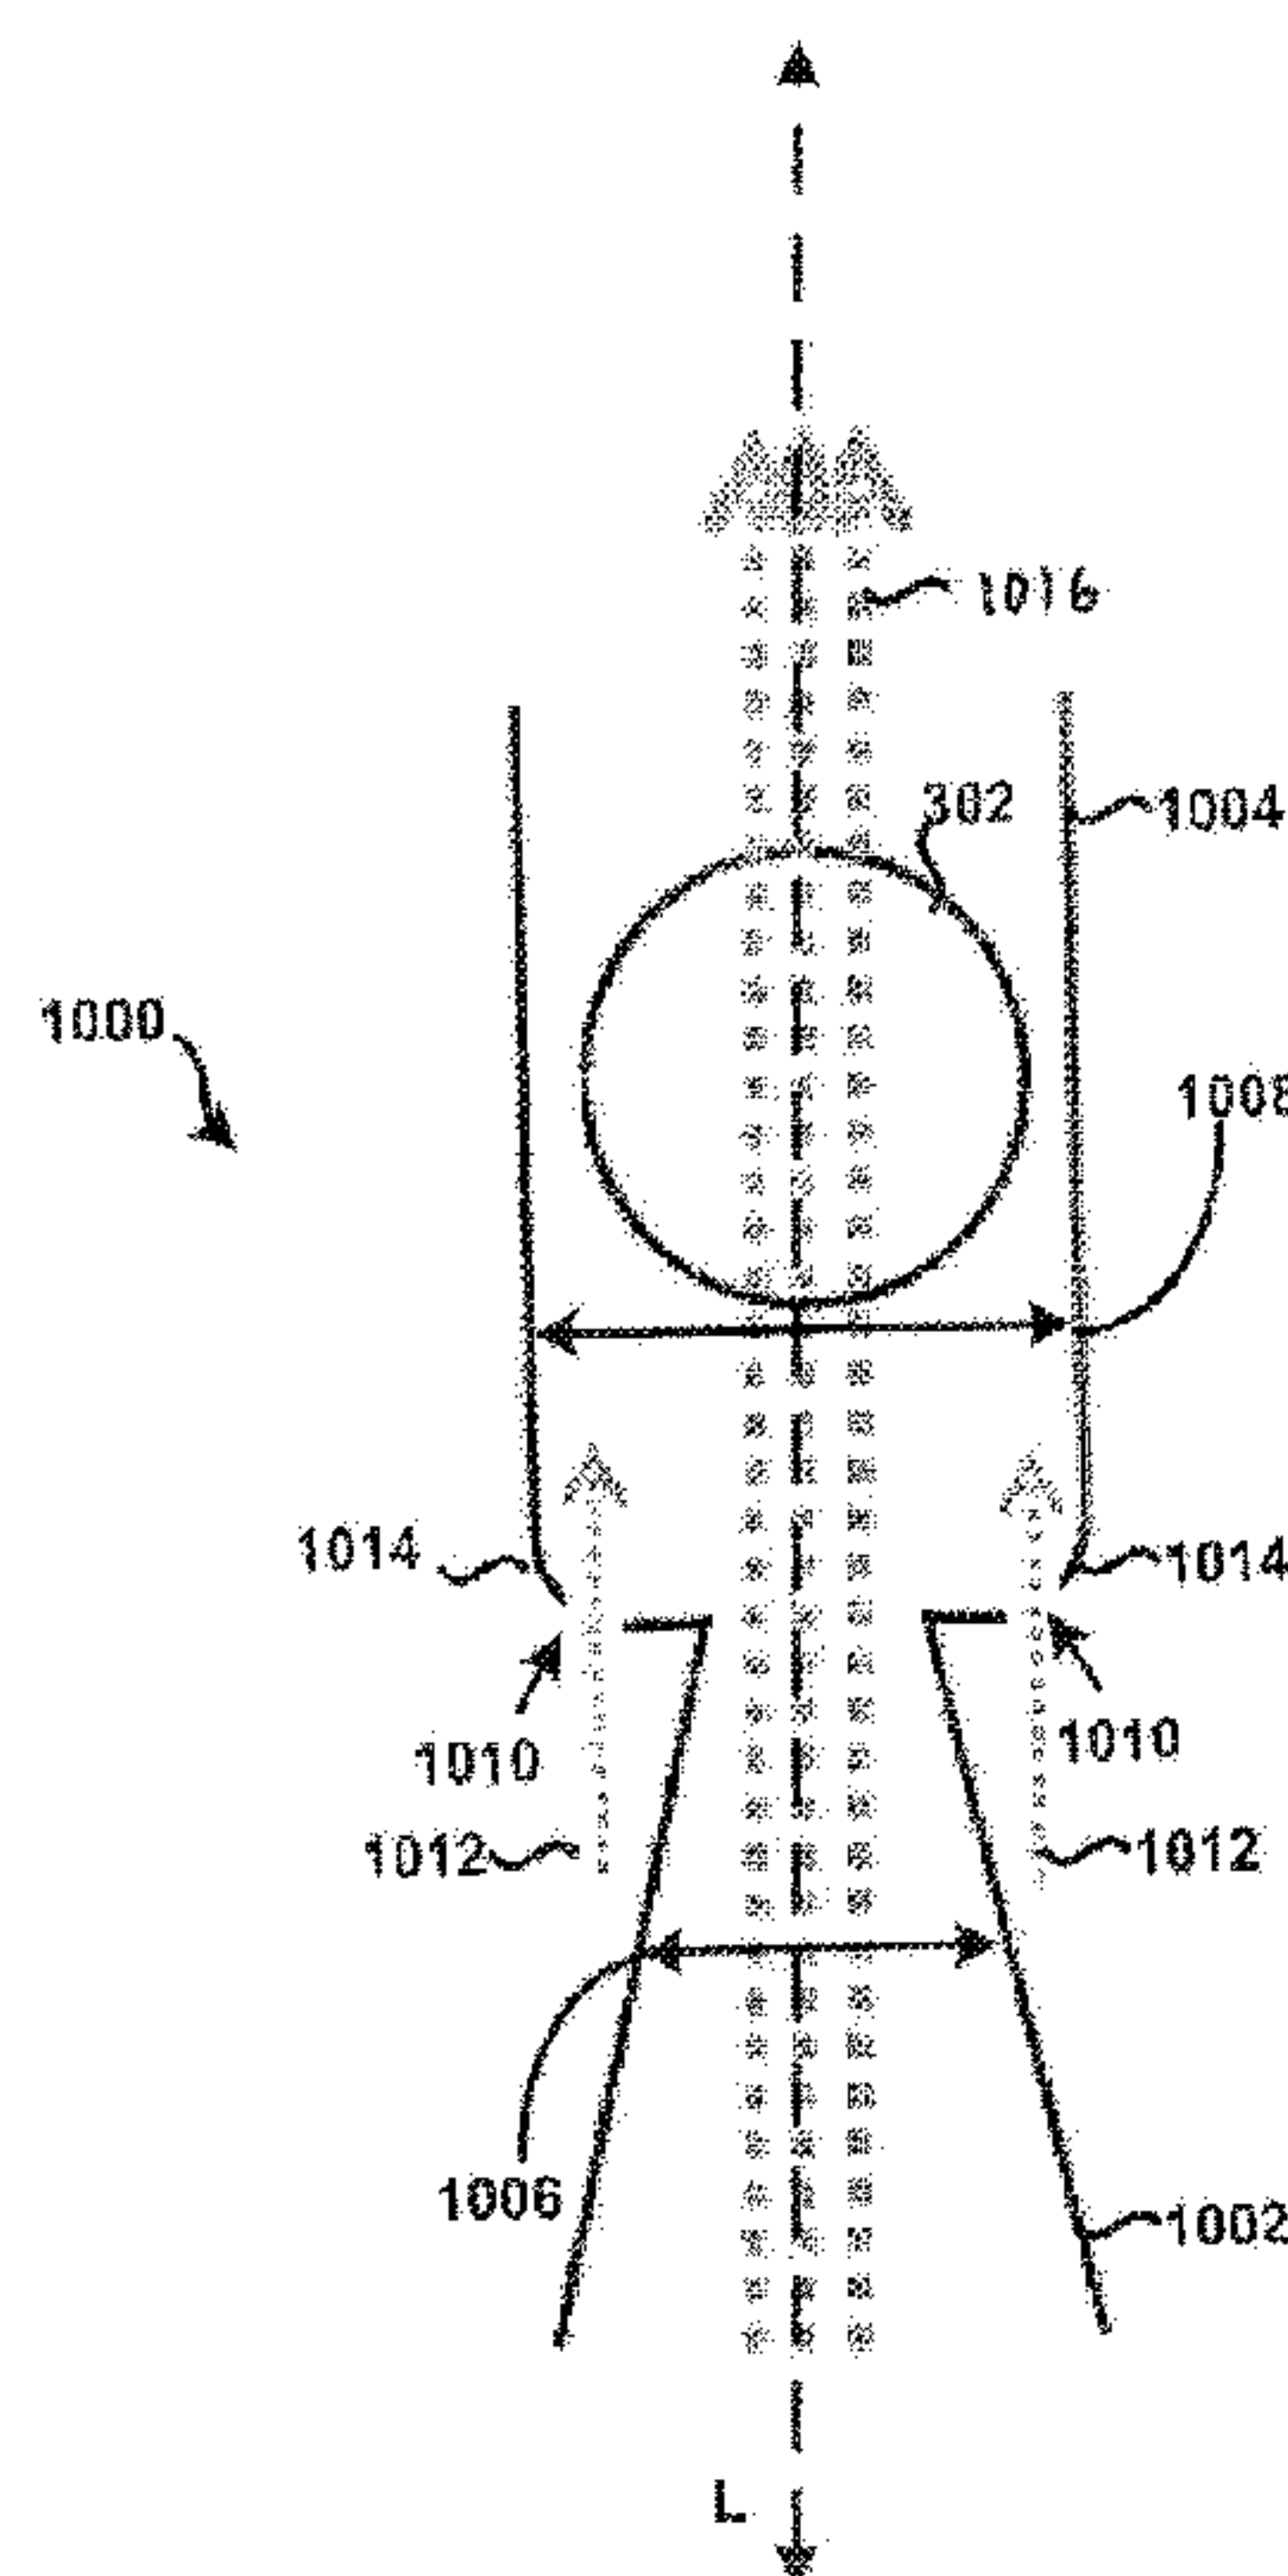


FIG. 10

(57) **Abrégé/Abstract:**

A dry powder inhaler includes a powder storage element configured to hold a powdered medicament and an inlet channel receives powdered medicament from the powder storage element that is entrained in an airflow. The inlet channel has a first diameter and defines an opening. The inhaler includes a dispersion chamber that receives the airflow and the powdered medicament from the opening. The dispersion chamber has a second diameter. The inhaler includes an actuator housed within the dispersion chamber. The actuator oscillates within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament entrained by the airflow passing through the dispersion chamber. A ratio between the first diameter and the second diameter is between about 0.40 and 0.60 such that an audible sound is produced as the actuator oscillates. The inhaler includes an outlet channel through which the airflow and powdered medicament exit the inhaler.



(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
21 July 2016 (21.07.2016)

(10) International Publication Number
WO 2016/115379 A1

(51) International Patent Classification:
A61M 15/00 (2006.01)

(21) International Application Number:
PCT/US2016/013456

(22) International Filing Date:
14 January 2016 (14.01.2016)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
62/103,485 14 January 2015 (14.01.2015) US

(71) Applicant: **RESPIRA THERAPEUTICS, INC.** [US/US];
#107, 5901 Indian School Road, Albuquerque, New Mexico 87110 (US).

(72) Inventors: **CURTIS, Robert M.**; 12 Black Mesa, Santa Fe, New Mexico 87506 (US). **DEATON, Dan**; 3212 Righters Mill Way, Apex, North Carolina 27539 (US). **HANNON, James**; Unit 3303, 6501 San Antonio Drive NE, Albuquerque, New Mexico 87109 (US). **SMYTH,**

Hugh; 1802 Basin Ledge, West Lake Hills, Texas 78746 (US). **XU, Zhen**; A106, 3901 Indian School Road NE, Albuquerque, New Mexico 87110 (US). **DONOVAN, Martin**; 2338 Sea Palm Dr., El Paso, Texas 79936 (US). **GIBBONS, Aileen**; Apt 2A, 337 E 54th Street, New York, New York 10022 (US).

(74) Agents: **SPINK, Torrey D.** et al.; Eighth Floor, Two Embarcadero Center, San Francisco, California 94111 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH,

[Continued on next page]

(54) Title: POWDER DISPERSION METHODS AND DEVICES

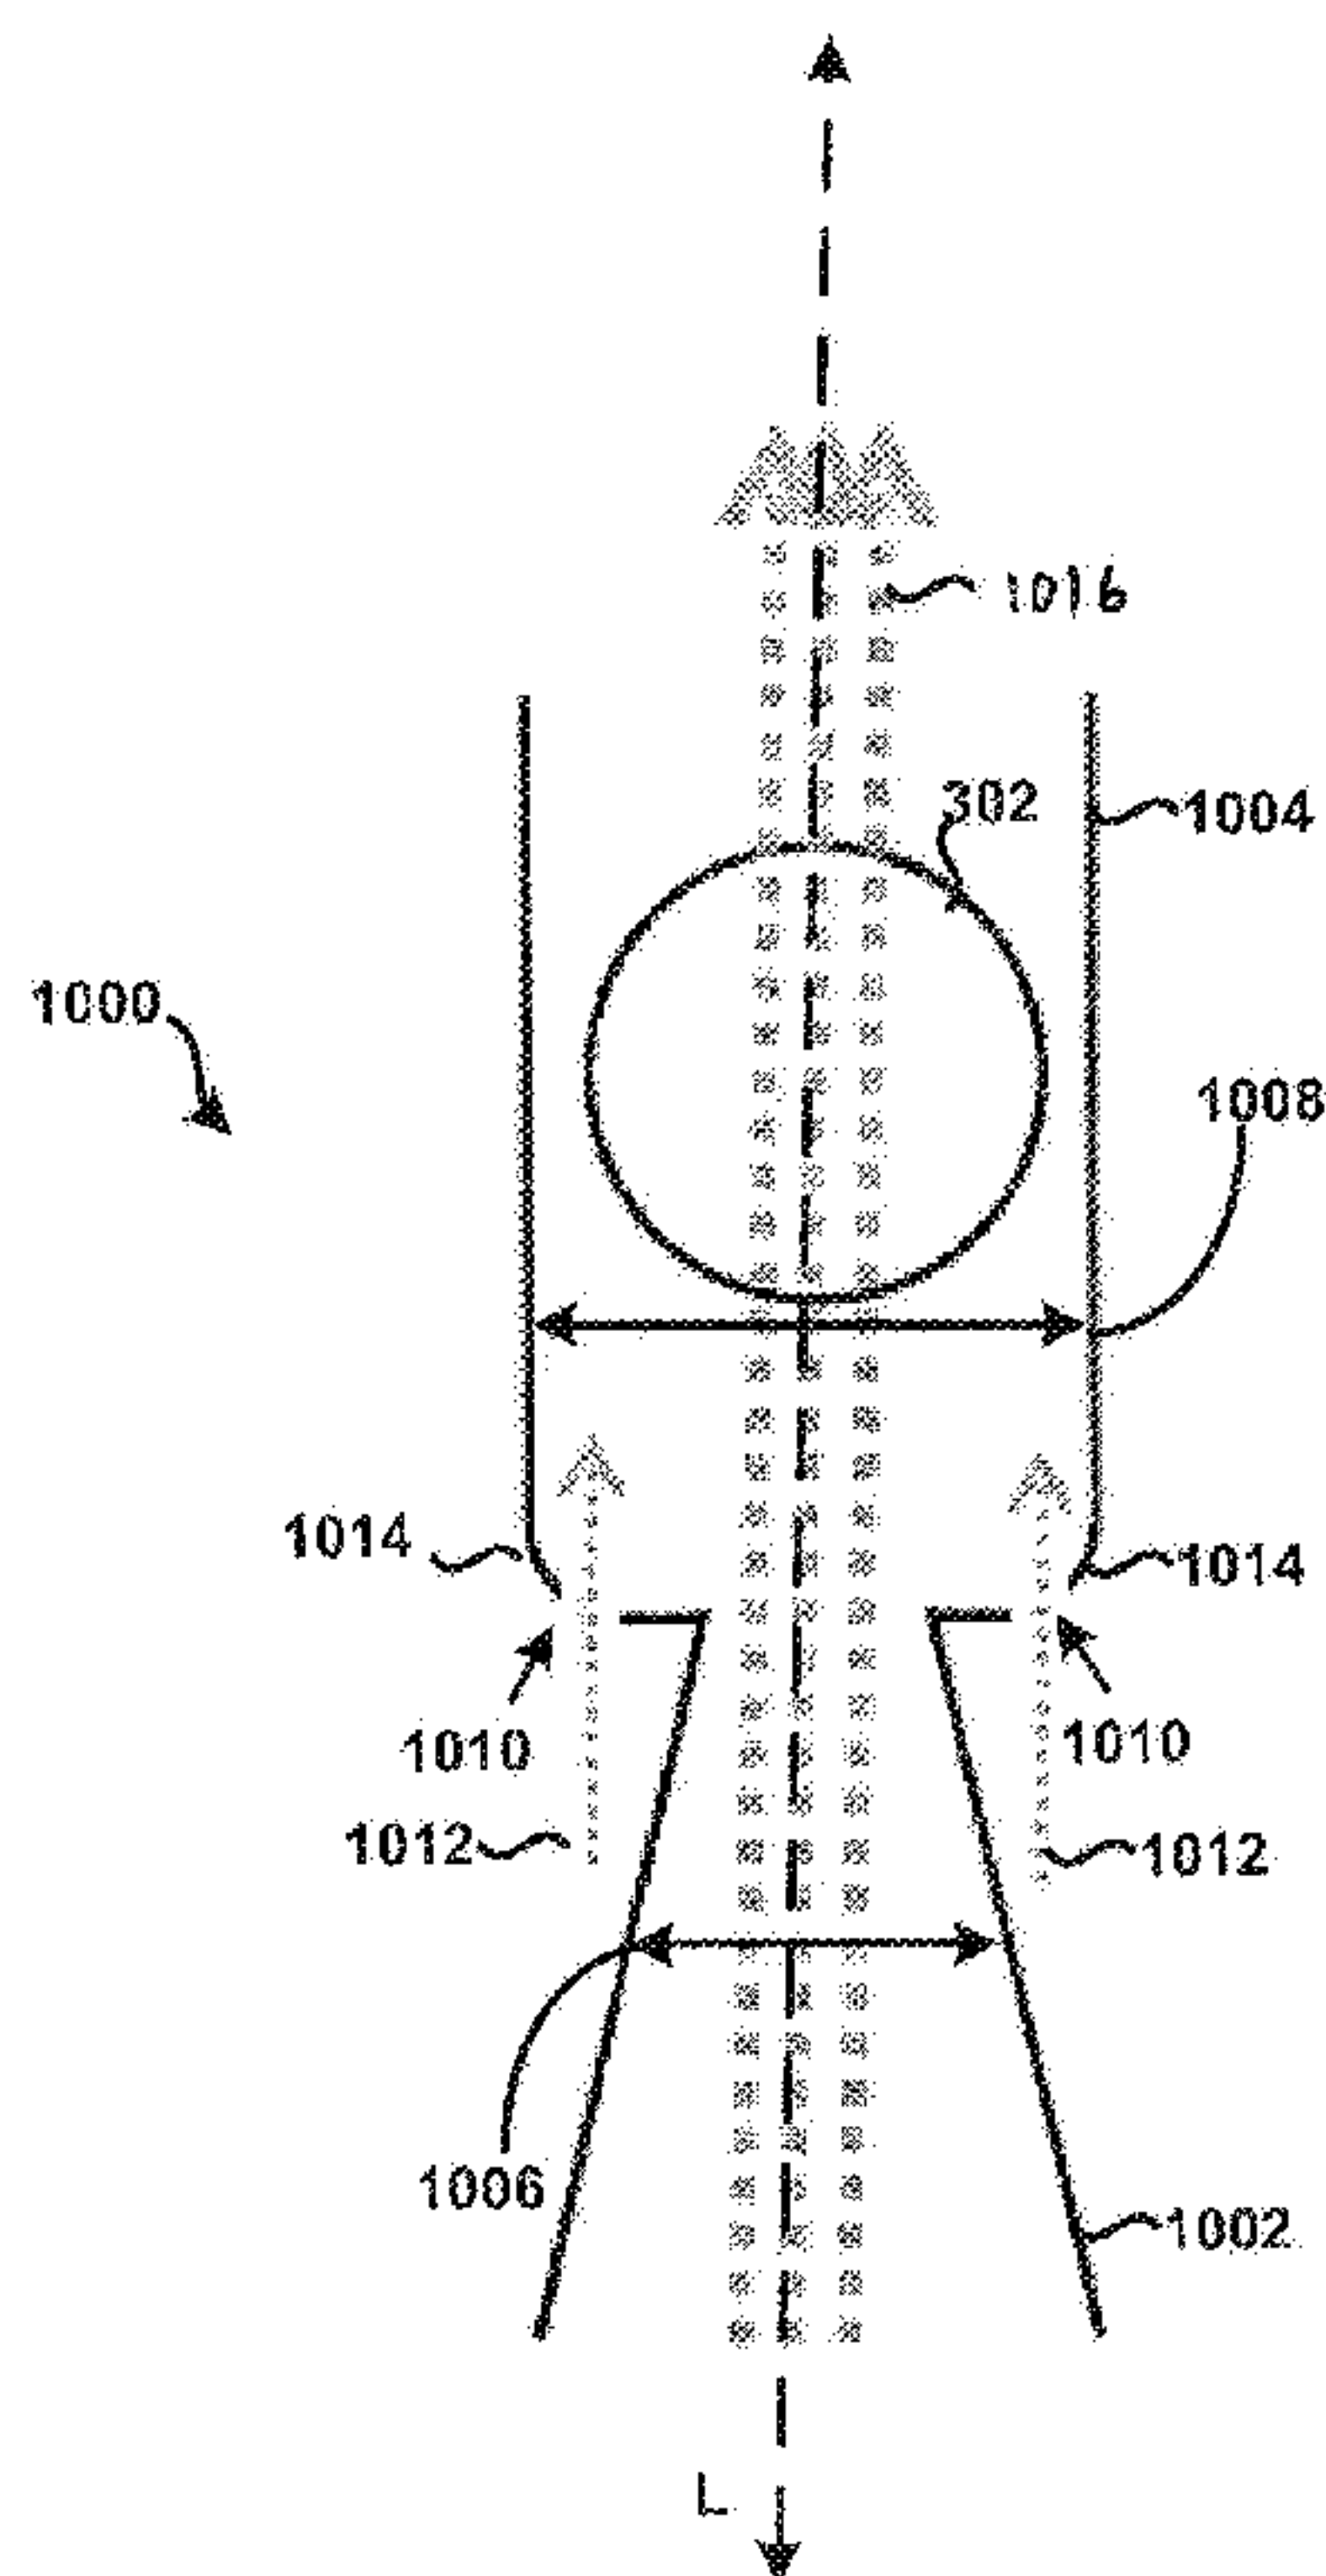


FIG. 10

(57) Abstract: A dry powder inhaler includes a powder storage element configured to hold a powdered medicament and an inlet channel receives powdered medicament from the powder storage element that is entrained in an airflow. The inlet channel has a first diameter and defines an opening. The inhaler includes a dispersion chamber that receives the airflow and the powdered medicament from the opening. The dispersion chamber has a second diameter. The inhaler includes an actuator housed within the dispersion chamber. The actuator oscillates within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament entrained by the airflow passing through the dispersion chamber. A ratio between the first diameter and the second diameter is between about 0.40 and 0.60 such that an audible sound is produced as the actuator oscillates. The inhaler includes an outlet channel through which the airflow and powdered medicament exit the inhaler.

WO 2016/115379 A1

GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Declarations under Rule 4.17:
— *as to the identity of the inventor (Rule 4.17(i))*
Published:
— *with international search report (Art. 21(3))*

POWDER DISPERSION METHODS AND DEVICES

CROSS-REFERENCE TO RELATED APPLICATION

[0001] This application claims priority to U.S. Provisional Patent Application No. 62/103,485, filed on January 14, 2015, entitled “POWDER DISPERSION METHODS AND DEVICES,” the entirety of which is hereby incorporated by reference for all purposes.

5 [0002] This application is related to U.S. Nonprovisional Patent Application No. 13/773,325, filed on 21 February 2013, entitled “INHALER TO DELIVER SUBSTANCES FOR PROPHYLAXIS OR PREVENTION OF DISEASE OR INJURY CAUSED BY THE INHALATION OF BIOLOGICAL OR CHEMICAL AGENTS,” the entirety of which is hereby incorporated by reference for all purposes.

10 [0003] This application is related to U.S. Nonprovisional Patent Application No. 13/776,546, attorney docket number 93933-863197, filed on 25 February 2013, entitled “POWDER DISPERSION DEVICES AND METHODS,” the entirety of which is hereby incorporated by reference for all purposes.

15 [0004] This application is related to U.S. Nonprovisional Patent Application No. 13/776,558, attorney docket number 93933-863196, filed on 25 February 2013, entitled “POWDER DISPERSION DEVICES AND METHODS,” the entirety of which is hereby incorporated by reference for all purposes.

BACKGROUND

[0005] In the field of dry powder inhalers, there is generally a trade-off between performance, as defined by the efficiency of the nominal or loaded dose in the inhaler that is delivered to the lung, and device complexity, in terms of the internal geometry, specifically, the powder flow path that the dose travels as it exits the device. In many instances, inhalers with relatively uncomplicated flow paths may be characterized by poor efficiency, as generally less than 30% of the nominal dose is delivered to the deep lung. Alternatively, inhalers with relatively more complex internal flow paths, may provide increased efficiency, such as less than or equal to 40% of the nominal dose, though the increased complexity of the internal flow path may lead to

20
25

increased deposition within the inhaler, effectively lowering the overall dose delivered to the patient and contaminating the device. In addition, most dry powder inhalers available today have no means of providing feedback to the user that they have used the device correctly. Incorrect use may cause poor inhaler performance.

5

SUMMARY

[0006] This Summary does not in any way limit the scope of the claimed subject matter.

[0007] The present disclosure is directed to a powder dispersion mechanism that is compact, breath-actuated, provides audio feedback, and that is effective or sufficient at promoting efficient particle dispersion across a range of doses such as from, for example, low microgram doses to
10 doses requiring many milligrams. Accordingly, in some embodiments, a powder dispersion mechanism is disclosed that employs an actuator contained within a dispersion chamber. An actuator is an element in the inhaler that may oscillate, generally linearly in certain embodiments, along an axis of the dispersion chamber when the patient inhales through the device, such that the actuator does not require an energy source other than a patient's inspiratory maneuver to
15 function. This actuator may take various forms or shapes including a sphere, ball, or bead-like shape. However, the actuator is not limited to this and may take any appropriate shape that results in oscillation. In some embodiments, the powder dispersion mechanism may include a predominantly straight flow path, and may be breath-actuated. This may be referred to as "passive" actuator activation or actuation. During actuator oscillation the actuator may make an
20 audible sound that could provide feedback for the user of the inhaler. However, the present disclosure is not so limiting. For example, actuator activation may be "active," where an external energy source is coupled with the patient's inhalation flow stream to induce actuator oscillation. One or more features of the inhaler may be such that a flow profile is generated within the dispersion chamber that prevents or at least minimizes unintended deposition or
25 accumulation of powder within the chamber.

[0008] In an aspect, a dry powder inhaler is disclosed. The dry powder inhaler may include a first chamber that is adapted to receive an aerosolized powdered medicament from an inlet channel. A volume of the first chamber may be equal to, greater than or less than the volume of the inlet channel. The dry powder inhaler may include a dispersion chamber that is adapted to
30 receive at least a portion of the aerosolized powdered medicament from the first chamber. The dispersion chamber may hold an actuator that is movable within the dispersion chamber along a

longitudinal axis. The dry powder inhaler may include an outlet channel through which air and powdered medicament exit the inhaler to be delivered to a patient. A geometry of the inhaler may be such that a flow profile is generated within the dispersion chamber that causes the actuator to oscillate along the longitudinal axis, enabling the oscillating actuator to effectively
5 disperse powdered medicament received in the dispersion chamber for delivery to the patient through the outlet channel. During actuator oscillation the actuator may generate an audible sound intended for feedback to the user.

[0009] In an aspect, a dry powder inhaler system is disclosed. The dry powder inhaler system may include a receptacle containing an amount of powdered medicament. The dry powder
10 inhaler system may include an inlet channel that is adapted to receive air and powdered medicament from the receptacle. The dry powder inhaler system may include a first chamber that is adapted to receive air and powdered medicament from the inlet channel. A volume of the first chamber may be equal to, greater or less than the volume of the inlet channel. The dry powder inhaler system may include a dispersion chamber that is adapted to receive air and
15 powdered medicament from the first chamber. The dispersion chamber may hold an actuator that is movable within the dispersion chamber along a longitudinal axis. The dry powder inhaler system may include an outlet channel through which air and powdered medicament exit the dispersion chamber to be delivered to a patient. A geometry of the system may be such that a flow profile is generated within the system that causes the actuator to oscillate along the
20 longitudinal axis, enabling the oscillating actuator to effectively disperse powdered medicament received in the dispersion chamber for delivery to the patient through the outlet channel. During actuator oscillation the actuator may generate an audible sound intended for feedback to the user.

[0010] In an aspect, a method for aerosolizing a powdered medicament is disclosed. The method may include providing an inhaler comprising a first chamber, and a dispersion chamber,
25 the dispersion chamber containing an actuator that is movable within the dispersion chamber along a longitudinal axis, and an outlet channel. The method may include inducing air flow through the outlet channel to cause air and powdered medicament to enter into the first chamber through the inlet channel into the dispersion chamber, and to cause the actuator to oscillate within the dispersion chamber to effectively disperse powdered medicament passing through the
30 first chamber and the dispersion chamber to be entrained by the air and delivered to the patient through the outlet channel.

[0011] In another aspect a dry powder inhaler is provided. The inhaler may include a powder storage element configured to hold a powdered medicament and an inlet channel configured to receive powdered medicament from the powder storage element that is entrained in an airflow. The inlet channel may have a first diameter and may define an opening. The inhaler may also include a dispersion chamber that is adapted to receive the airflow and the powdered medicament from the opening of the inlet channel. The dispersion chamber may have a second diameter. The inhaler may further include an actuator housed within the dispersion chamber. The actuator may be configured to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament passing through the dispersion chamber to be entrained by the airflow. A ratio between the first diameter and the second diameter may be between about 0.40 and 0.66 such that an audible sound is produced as the actuator oscillates. The inhaler may also include an outlet channel through which the airflow and powdered medicament exit the inhaler for delivery to a patient.

[0012] In another aspect, the dry powder inhaler may include a powder storage element configured to hold a powdered medicament and an inlet channel configured to receive powdered medicament from the powder storage element that is entrained in an airflow. The inlet channel may define an opening. The inhaler may include a dispersion chamber that is adapted to receive the airflow and the powdered medicament from the opening of the inlet channel. The dispersion chamber may have a length. The inhaler may further include a bead housed within the dispersion chamber. The bead may be configured to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament passing through the dispersion chamber to be entrained by the airflow. The bead may have a diameter such that the length of the dispersion chamber is between about 2 and 3.5 times larger than the diameter of the bead such that an audible sound is produced as the bead oscillates. The inhaler may also include an outlet channel through which the airflow and powdered medicament exit the inhaler for delivery to a patient.

[0013] In another aspect, the dry powder inhaler may include a powder storage element configured to hold a powdered medicament and an inlet channel configured to receive powdered medicament from the powder storage element that is entrained in an airflow. The inlet channel may have a first diameter and may define an opening. The inhaler may also include a dispersion chamber that is adapted to receive the airflow and the powdered medicament from the opening of

the inlet channel. The dispersion chamber may have a second diameter and a length. The inhaler may further include a bead housed within the dispersion chamber. The bead may be configured to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament passing through the dispersion chamber to be entrained by the airflow.

5 The bead may have a third diameter. A ratio between the first diameter and the second diameter may be between about 0.40 and 0.66 and the length may be between about 2 and 3.5 times larger than the third diameter such that an audible sound is produced as the bead oscillates. The inhaler may also include an outlet channel through which the airflow and powdered medicament exit the inhaler for delivery to a patient.

10 **[0014]** In another aspect, the dry powder inhaler may include a powder storage element configured to hold a powdered medicament and a conical frustum shaped inlet channel configured to receive powdered medicament from the powder storage element that is entrained in an airflow. The inhaler may also include a dispersion chamber that is adapted to receive the airflow and the powdered medicament from the opening of the inlet channel. The inhaler may

15 further include an actuator housed within the dispersion chamber. The actuator may be configured to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament passing through the dispersion chamber to be entrained by the airflow. The inhaler may also include an outlet channel through which the airflow and powdered medicament exit the inhaler for delivery to a patient.

20 **[0015]** In another aspect, the dry powder inhaler may include a powder storage element configured to hold a powdered medicament and an inlet channel configured to receive powdered medicament from the powder storage element that is entrained in an airflow. The inhaler may also include a dispersion chamber that is adapted to receive the airflow and the powdered medicament from the opening of the inlet channel. The airflow may be substantially coaxial

25 with a longitudinal axis of the dispersion chamber. The inhaler may further include an actuator housed within the dispersion chamber. The actuator may be configured to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the powdered medicament passing through the dispersion chamber to be entrained by the airflow. The inhaler may also include an outlet channel through which the airflow and powdered medicament exit the inhaler

30 for delivery to a patient. Although not so limited, an appreciation of the various aspects of the present disclosure may be gained from the following discussion in connection with the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

- [0016] FIG. 1 shows a cross-section of a first example tubular body.
- [0017] FIG. 2 shows the tubular body of FIG. 1 in multiple views.
- [0018] FIG. 3 shows a bead positioned within a chamber of the tubular body of FIG. 1.
- 5 [0019] FIG. 4 shows a first view of an example powder dispersion device in cross-section.
- [0020] FIG. 5 shows a perspective view of the device of FIG. 4.
- [0021] FIG. 6 shows a second view of the device of FIG. 4 in cross-section.
- [0022] FIG. 7 shows a third view of the device of FIG. 4 in cross-section.
- [0023] FIG. 8 shows the device of FIG. 4 incorporated into an existing inhaler system.
- 10 [0024] FIG. 9 shows the device of FIG. 4 in multiple configurations.
- [0025] FIG. 10 shows a cross-section of a second example tubular body.
- [0026] FIG. 11 shows a cross-section of a third example tubular body.
- [0027] FIG. 12 shows a cross-section of a fourth example tubular body.
- [0028] FIG. 13 shows a cross-section of a fifth example tubular body.
- 15 [0029] FIG. 14 shows a cross-section of a sixth example tubular body.
- [0030] FIG. 15 shows a cross-section of a seventh example tubular body.
- [0031] FIG. 16A shows a back view of non-circular inlet geometry.
- [0032] FIG. 16B shows a cross-section of the non-circular inlet geometry of FIG. 16A.
- [0033] FIG. 17 bead sound level plot for different chamber lengths.
- 20 [0034] FIGs. 18A and 18B show a bead sound comparison for different inlet channel and chamber diameters.
- [0035] FIGs. 19A-19C show bead position plots to determine chamber end contact for inlet diameters of 2.72mm.
- [0036] FIGs. 20A-20C show bead position plots to determine chamber end contact for inlet
25 diameters of 3.10mm.
- [0037] FIG. 21 shows one embodiment of chamber ribs.
- [0038] FIG. 22 shows one embodiments of bead retention features.
- [0039] FIG. 23 shows an embodiment having two beads in a chamber.
- [0040] FIG. 24 shows an embodiment of a DPI with capsule piercing and powder feed
30 element from a Plastiap RS01 inhaler.
- [0041] FIG. 25 shows a cross section of the DPI of FIG. 24.

[0042] FIG. 26 shows the aerosol performance of a DPI of FIG. 24.

[0043] FIG. 27 shows drug deposition within the DPI of FIG. 24 at different flow rates.

[0044] FIG. 28A shows a tightly-spaced grid structure used in experiment testing swirling flow according to embodiments.

5 [0045] FIG. 28B shows a 2-piece grid structure used in experiment testing swirling flow according to embodiments.

DETAILED DESCRIPTION

[0046] The present disclosure relates to the field of pulmonary drug or medicament delivery, and more specifically to dry powder inhalers that deliver a powder or medicament into the lungs
10 of a patient. Such a powder dispersion mechanism may comprise of an actuator positioned within a chamber that is arranged and configured to induce a sudden, rapid, or otherwise abrupt expansion of a flow stream upon entering the chamber. During actuator oscillation the actuator may make an audible sound or response that could provide feedback to the user of the inhaler. Characteristics of the audible response may be adjusted based on various geometric properties of
15 an inhaler, as well as material selection. Additionally, at least the chamber may be formed to exhibit one or more features that prevent or at least minimize the accumulation or build-up of powder in the chamber with the actuator. This may advantageously prevent the delivery of a macro dose of powder to a patient that may occur when an unintended deposit or residue of powder is broken-up or released during use. An actuator is an element in the inhaler that may
20 oscillate, generally linearly in certain embodiments, along an axis of the dispersion chamber when the patient inhales through the device, such that the actuator does not require an energy source other than a patient's inspiratory maneuver to function. This actuator may take various forms or shapes including a sphere, ball, or bead-like shape. However, the actuator is not limited to this and may take any appropriate shape that results in oscillation.

25 [0047] Embodiments provide dry powder inhalers configured to produce an audible sound or feedback while delivering acceptable aerosol performance. The audible feedback is sufficiently loud that a user of the inhaler may be alerted when inhalations meet or exceed a minimum amount of flow. Suitable audio sound may be obtained by configuring a ratio ($d_{\text{inlet}}/d_{\text{chamber}}$) of an internal diameter of an inlet (d_{inlet}) of the inhaler to an internal diameter of a dispersion
30 chamber of the inhaler (d_{chamber}) to be within a certain range, by configuring a ratio ($l_{\text{chamber}}/d_{\text{bead}}$) of a length of the dispersion chamber (l_{chamber}) relative to a diameter of the actuator or bead

(d_{bead}) of the inhaler to be within a certain range or by certain combinations of both ($d_{\text{inlet}}/d_{\text{chamber}}$) and ($l_{\text{chamber}}/d_{\text{bead}}$). These ratios may be specifically selected so that they provide an acceptable audio sound while also ensuring proper aerosol performance (so that the powder can reach the deep lung).

5 [0048] Referring now to **FIG. 1**, a cross-section of a first example tubular body **100** having an inlet **102** and a dispersion chamber **104** is shown according to the principles of the present disclosure. In this example, a fluid flow path of the inlet **102** is defined by a first internal diameter **106**, and a fluid flow path of the chamber **104** is defined by a second internal diameter **108**. Although shown approximately constant in **FIG. 1**, at least one of the first internal
10 diameter **106** and the second internal diameter **108** may vary in dimension as defined with respect to a longitudinal axis **L** of the tubular body **100**. Further, one or more apertures may be formed within the tubular body **100** at particular locations to allow a secondary air supply to enter the tubular body **100** during use to prevent or at least minimize the unintended accumulation or build-up of powder within the tubular body **100** for example the apertures **1310**
15 in **FIG 13**. Additionally, or alternatively, one or more internal surfaces of the tubular body **100** may be formed to exhibit rounded or curved features to prevent or at least minimize the unintended accumulation or build-up of powder within the tubular body **100**. In addition to providing desirable fluid flow characteristics, as discussed further below, such configurable internal features or dimensions of the tubular body may be defined so as to provide for a draft
20 angle for injection molding. In some embodiments, an injection molding technique or process may be used to fabricate at least the tubular body **100** of the present disclosure, including like features or elements discussed in further detail below. Other embodiments are possible.

[0049] For example, the first internal diameter **106** may taper inwardly, towards and as measured with reference to the longitudinal axis **L**, beginning approximately at a reference point
25 **L1** of the longitudinal axis **L** and ending approximately at a reference point **L2** of the longitudinal axis **L**. Other embodiments are possible. For example, the first internal diameter **106** may taper inwardly towards the longitudinal axis **L** beginning approximately at the reference point **L2**, and ending approximately at the reference point **L1**. . In another embodiment, the second internal diameter **108** may taper inwardly towards the longitudinal axis **L** beginning
30 approximately at the reference point **L3** and ending approximately at the reference point **L2**. Still other embodiments are possible.

[0050] For example, it is contemplated that an internal structural profile of at least one of the inlet **102** and the chamber **104** may be defined, as desired, such as to obtain or otherwise realize particular fluid flow characteristics within the tubular body **100**. For example, as depicted in **FIG. 1**, the tubular body **100** may be arranged and configured such that a sudden flow stream expansion may occur when the relatively “small” cross-sectional fluid flow path of or defined by the inlet **102** opens abruptly into a “larger” cross-sectional fluid flow path of or defined by the chamber **104**. In this example, high-energy forces may develop within the chamber **104**. In one aspect, this may be due to relatively “low” pressure regions induced by relatively “high” velocity fluid entering the chamber **104**, where a portion of the flow stream detaches and recirculation eddies may occur. Other mechanisms may contribute to the development of high-energy fluid flow within the chamber **104** as well. Further, such high-energy fluid flow, along with mechanical impact forces, may disrupt and aerosolize medicament powder agglomerates within the chamber **104** to provide for more effective deposition of medicament into the lungs of a patient. Still other embodiments of the example tubular body **100** are possible as well. For example, in some embodiments, a difference between the reference point **L1** of the longitudinal axis **L** and the reference point **L2** may approach zero (0). In this example, the tubular body **100** may consist only of the chamber **104**. Here, instead of an “inlet tube,” the tubular body **100** may consist of an “inlet hole”.

[0051] The geometry of the inlet to the dispersion chamber plays a critical role in the resistance of the inhaler. The resistance (R) is a relationship between the pressure drop across the device at a given flow and is defined as $R = \frac{\sqrt{\Delta P}}{Q}$ where ΔP is the pressure drop across the device (cm H₂O) and Q is the flow (LPM) at the given ΔP . One embodiment includes a conical or conical frustrum inlet **1002** of **FIG. 10**. Experiments have shown that a conical frustrum inlet significantly reduces the resistance of the inhaler compared to a tube or inlet hole geometry. An experiment was conducted comparing different inlet geometries with the same inlet **106** and dispersion chamber diameter **108** as defined in **FIG. 1**: (1) conical frustrum inlet, (2) tubular inlet, and (3) inlet hole. The inlet diameter **106** was 2.72 mm and the chamber diameter **108** was 5.89 mm and a 4 mm spherical bead was used as the actuator. The length of the chamber from **L2** to **L3** as shown in **FIG. 1** was 10mm. The conical frustrum inlet was shown to have a significantly lower resistance than the tubular inlet and inlet hole design as shown in **TABLE 1**. The geometry of the inlet shape at reference point **L2** in **FIG. 1** can be non-circular in shape

such as: triangular, square, polygon, or elliptical. For example, a first distal shape at **L1** may taper to a smaller second proximal shape at **L2**. In some embodiments, the first shape and the second shape may be the same and in other embodiments the first shape and the second shape may be different. A tapering inlet with a square geometry at **L2** is illustrated in **FIG. 16A**. **FIG. 16A** shows a front view of an inlet chamber **1602** and a dispersion chamber **1604** according to one embodiment. A distal opening of inlet chamber **1602** is shown as a circular opening, but may be any other shape. The inlet chamber **1602** tapers, as seen in the side cross-sectional view of **FIG. 16B**, to a smaller shape **1606** near the dispersion chamber **1604**. Referring again to **FIG. 16A**, smaller shape **1606** may be any shape, such as a square, rectangle, circle, or triangle.

Another experiment was conducted comparing the resistance of several different tapering inlets with varying geometries at reference point **L2** in **FIG 1**. The geometry at reference point **L1** in **FIG 1** was a circle while the geometry at reference point **L2** in **FIG 1** was varied to include an equilateral triangle, square, ellipse, and circle. The inlet area was held constant to match that of a circular inlet diameter of 3.30 mm which results in an open area of 8.55 mm². A 4 mm spherical bead was used as an actuator in the chamber, the chamber diameter **108** was 5.89mm, and the length of the chamber was 10mm for this test. The results are shown in **TABLE 2**, the square inlet had 10% lower resistance than the circular inlet. It was noted that the square inlet produced a similar audio sound from the actuator in terms of volume to the circular inlet. There may be added benefits to non-circular inlet shape designs to the dispersion chamber such as increased turbulence for better dispersion of powders. Lowering the resistance of the chamber is important because it increases the flow through the chamber for a given pressure drop. Increasing the flow may in turn increase the speed and/or frequency of the actuator oscillations which could be an important characteristic for efficient powder dispersion.

TABLE 1

Geometry	Resistance (<i>cm H₂O</i>) ^{0.5} /LPM
Conical Frustum	0.178
Tubular	0.242
Inlet hole	0.238

TABLE 2

Inlet shape	Resistance ($cm\ H_2O$) ^{0.5} /LPM
Circle	0.131
Equilateral triangle	0.284
Square	0.115
Ellipse	0.122

[0052] Referring now additionally to **FIG. 2**, the tubular body **100** of **FIG. 1** is shown in multiple views. In particular, the tubular body **100** of **FIG. 1** is shown in perspective view **202**, side view **204**, and cross-section view **206**. In this example, the cross-section view **206** is taken along an axis **A-A** of the side view **204**. Additionally, and as illustrated in **FIG. 1**, the fluid flow path of or defined by the inlet **102** is coaxially aligned with the fluid flow path of or defined by the chamber **104**. This is in contrast with a substantially “off-axis” alignment of the inlet **102** and the chamber **104**, illustrated conceptually in **FIG. 2** by a finite angle **B** defined with respect to the longitudinal axis **L**. A coaxial alignment may provide a number of advantages over such an “off-axis” alignment, such as facilitating or otherwise assisting in the development of high-energy forces within the chamber **104**. The coaxial alignment may further enable the efficient transfer of powder into the chamber **104**. However, other embodiments are possible. For example, in some embodiments, a central longitudinal axis of the inlet **102** may be at least slightly offset yet parallel to a central longitudinal axis of the chamber **104**. Other benefits and/or advantages associated with the alignment of the inlet **102** and the chamber **104** may be understood from the preceding description provided in connection with **FIGS. 1-2**, and from the following description provided in connection with **FIGS. 3-14**. Although the inlet may be “off-axis” in alignment, the principal component of flow is in the axial direction. Furthermore, swirling or centrifugal flow into the inlet is detrimental to the oscillation of the bead. An experiment was performed using an embodiment as illustrated in **FIG. 25**. This embodiment has air inlets that are tangential to flow through the chamber **104** and they are shaped to induce a swirling or tangential flow which promotes capsule emptying. A grid is in place **2406** and it acts as a flow straightener similar to a honeycomb flow straightener. Two different grids were tested (1) a tightly-spaced grid **2800** of **FIG. 28A** and (2) simple 2-piece grid structure **2802** as shown in **FIG. 28B**. The tightly-spaced grid **2800** straightens and aligns the flow in axial direction

similar to a honeycomb flow straightener used in wind tunnels. The tightly-spaced grid **2800** aligns the flow along the axis **204** shown in **FIG. 2**. The simple 2-piece grid **2802** provides little to no straightening of the flow. It was found that using the simple 2-piece grid **2802** prevented a spherical bead from oscillating under any flow conditions. The bead remained hovering near the inlet and did not oscillate.

[0053] For example, referring now additionally to **FIG. 3**, an actuator which could be shaped as a spherical bead **302** may be positioned within the chamber **104** of the tubular body **100** of **FIGS. 1-2**. In this example, the bead **302** may be approximately spherical, at least on the macroscale, and oscillate in a manner similar to that described in U.S. Application No. 13/469,963, filed 11 May 2012, and entitled “Bead-Containing Dry Powder Inhaler,” the complete disclosure of which is herein incorporated by reference. In some embodiments the actuator may be aspherical, or other shapes which may improve oscillation characteristics of the actuator. Further, a relationship between the diameter **304** of the actuator or bead **302**, the first internal diameter **106** of the inlet **102**, and the second internal diameter **108** of the chamber **104** may be of the form: $(d_{\text{bead}})^2 = (d_{\text{inlet}}) (d_{\text{chamber}})$. where d_{bead} and d_{inlet} and d_{chamber} are of similar order of magnitude. For example, in one embodiment d_{bead} may be about 4.00 mm, d_{chamber} may be about 5.89 mm, and d_{inlet} may be about 2.72 mm within manufacturing tolerance. In this example, a length of the chamber **104**, l_{chamber} , such as defined by a distance approximately between the reference point **L2** and the reference point **L3** of the longitudinal axis **L** (see **FIG. 1**), may be 2 to 3.5 times the diameter **304** of the bead **302**.

[0054] In some embodiments, a diameter of the bead **302** may be within a range of about 0.5 mm to about 15 mm. In some embodiments, a preferred diameter of the bead **302** may be within a range of about 1.5 mm to about 6 mm. Still other embodiments are possible. In some embodiments, a preferred ratio of the internal diameter **106** of the inlet **102** to that of the chamber **104** ($d_{\text{inlet}}/d_{\text{chamber}}$) may be within a range of about 0.40 to about 0.66 with a preferred range of 0.46-0.60, and even more preferred range of 0.50 – 0.60 or 0.53 – 0.60. In some embodiments, it may be preferred that the length of the chamber **104**, l_{chamber} , is about 2 times to about 5 times the diameter of the bead **302**. In other embodiments, it may be preferred that the length of the chamber **104**, l_{chamber} , is about 2 to about 3.5 times the diameter of the bead **302**. In other embodiments, it may be preferred that the length of the chamber **104**, l_{chamber} , is about 2 to about 2.5 times the diameter of the bead **302**.

[0055] In example embodiments, the length of the chamber **104** may determine whether the actuator **302** freely oscillates, without physical interaction with ends of the chamber **104**. Actuator oscillation that frequently impacts the chamber ends may not be desirable as it may generate particulate matter which can inhaled by the patient. In this manner, the length of the chamber **104** may facilitate free oscillation of the actuator **302**. A substantially “freely” oscillating actuator **302** may even more effectively disrupt and aerosolize powder agglomerates within the chamber **104**, as passed from the source, to provide for more effective deposition of medicament into the lungs of a patient.

[0056] For example, a study was performed to evaluate the length of the chamber **104** and to determine whether a particular length of chamber **104** would allow the actuator, a spherical bead **302**, to “freely” oscillate within the chamber **104**. In particular, using a device similar to the device **400**, a spherical bead actuator of fixed diameter, about 4 mm, was used across the study. The length of the chamber however was varied as 1.5x, 2.0x, 3.0x, 3.5x, 4.0x, and 9.8x diameter of the bead. In this manner, the study included evaluating at least six different device configurations. In general, it was found that oscillation of the bead within the chamber was similar for lengths up to and including 3.5x diameter of the spherical bead, yet varied for lengths 4.0x and 9.8x diameter of the bead. For example, a similar flow rate through the device was needed to allow the spherical bead to “freely” oscillate within the chamber at least for chamber lengths of 2.0x and 3.0x diameter of the bead. However, a “higher” flow rate was needed to allow the bead to “freely” oscillate within the chamber for a chamber length of 4.0x diameter of the bead. Further the spherical bead did not appear to “freely” oscillate within the chamber for a chamber length of 9.8x diameter of the spherical bead, for any flow rate through the device. At this chamber length, the spherical bead may not be fully influenced by the negative pressure field formed at the inlet of the device by the airflow through the sudden diameter expansion. Other mechanisms may be possible as well.

[0057] In another example, a study was performed to evaluate the length of the chamber **104** and to determine whether a particular diameter of the spherical bead actuator **302**, for a fixed length of the chamber **104**, would allow the actuator **302** to “freely” oscillate within the chamber **104**. In particular, using a device similar to the device **400**, a chamber of fixed length and diameter, about 10 mm length and about 6 mm diameter, was used across the study. The diameter of the spherical bead however was varied as 3.7 mm, 4 mm, and 4.7 mm. In this

manner, the study included evaluating at least three different bead configurations. In general, it was found that oscillation of the bead within the chamber for a 4 mm bead did “freely” oscillate within the chamber at a first particular flow rate. At this flow rate for this device configuration, a distinct audible sound produced by oscillation of the bead within the chamber may be observed.

5 Operation and characteristics of the device **400** having a 4 mm bead diameter is discussed in further detail below.

[0058] Further, it was found that oscillation of the spherical bead within the chamber for a 3.7 mm bead did “freely” oscillate within the chamber **104** at or about the first particular flow rate. However, a flow rate greater than the first particular flow rate was needed to observe an audible

10 sound similar to the distinct audible sound produced by oscillation of the spherical bead within the chamber for the 4 mm bead. Here, a greater flow rate may be required to produce the audible sound due to a reduced effective cross-sectional area of the 3.7 mm bead, as compared to the 4 mm bead. Other mechanisms may be possible as well. Further, it was found that oscillation of the bead within the chamber for a 4.7 mm bead did not “freely” oscillate within the chamber at

15 or about the first particular flow rate. Here, the effective cross-sectional area of the 4.7 mm bead may be too large such as to prohibit “free” oscillation within the chamber. Other mechanisms may be possible as well.

[0059] As described above, the actuator when oscillating can make an audible sound. The sound resulting from the oscillation of the actuator can be utilized as feedback to the user of the

20 inhaler to confirm they have performed the inhalation maneuver correctly. In general the volume of actuator sound increases with flow, which can encourage the user to perform a deep forceful inhalation. The sound of the actuator is strongly related to the length of the chamber and the preferred range is 2.0-3.5X the bead diameter, with 2 to about 2.5X the diameter of the actuator **302** being most preferred. Experiments have shown that for chamber lengths less than 2.0X the

25 actuator diameter the actuator oscillates freely but does not produce any significant sound. An experiment was performed to compare the sound from an oscillating bead with a chamber length of 1.5X and 2.5X bead diameter. The chambers for both used $d_{\text{bead}} = 4\text{mm}$, $d_{\text{inlet}} = 2.72\text{mm}$ $d_{\text{chamber}} = 5.89\text{mm}$. The sound of 1.5 and 2.5X chamber length was recorded using a microphone and analyzed as shown in **FIG. 17**. The 2.5X chamber length produced an audible sound from

30 bead oscillation from 1-4kPa. The audible sound level in general increased with the pressure and flow through the chamber. The 1.5X chamber length showed minimal increase in audible sound

from 1-4kPa compared to the 2.5X chamber length. A further experiment was performed to evaluate the sound of a bead using different ($d_{\text{inlet}}/d_{\text{chamber}}$) ratios. Two chambers were tested with $d_{\text{chamber}} = 5.89$ mm, and $l_{\text{chamber}} = 10$ mm, one had an inlet diameter of 2.72 mm and the other 3.10 mm resulting in 0.46 and 0.53 ($d_{\text{inlet}}/d_{\text{chamber}}$) ratios respectively. The level of the audible sound resulting from the oscillating bead was recorded at 1, 2, and 4kPa using a microphone. As shown in **FIGs. 18A and 18B**, the sound profile vs. time over roughly 20 seconds from the larger inlet ($d_{\text{inlet}}/d_{\text{chamber}} = 0.53$) of **FIG. 18B** was both louder and more consistent at 1, 2, and 4kPa. The smaller inlet to chamber ratio (0.46) of **FIG. 18A** showed significant periods of little sound resulting in an intermittent sound. A louder and more consistent sound is desirable for the audio feedback to the user. An intermittent sound such as that exhibited by ($d_{\text{inlet}}/d_{\text{chamber}} = 0.46$) may provide confusing feedback to the user as the sound is intermittent. The sound from bead oscillation could be used to provide valuable user feedback alerting the user that they have achieved the flow necessary for aerosol delivery. In some embodiments the sound of the bead could be analyzed by a microphone incorporated in the inhaler to determine if the patient reached a minimum flow rate for a period of time. This sound from the microphone could be processed and provide useful information to the patient and train them to achieve the necessary flow rate and time of inhalation for proper use of the inhaler. Furthermore this mechanism could be utilized as a patient compliance monitoring system to report when the inhaler was used and if the patient achieved the flow rate and volume necessary for powder delivery.

[0060] Continuing with the above dimensional example, the length of the chamber **104** may thus be about 10 mm for a 4 mm diameter bead. In this example, and when the ratio relationship between the diameters of the bead **302**, the inlet **102**, and the chamber **104** is observed, the bead **302** may oscillate within the chamber **104** generally without experiencing continuous physical collisions with either end of the chamber **104**. An experiment was performed to determine the frequency of bead collision with the ends of the chamber. Two clear chambers were machined from acrylic for use with a 4 mm bead ($d_{\text{chamber}} = 5.89$ mm, $l_{\text{chamber}} = 10$ mm, $d_{\text{inlet}} = 2.72$ mm and 3.10 mm) and the bead motion was recorded at 1200 frames/second for 5 seconds using a high speed camera. The video was analyzed to track the bead through the entire video. The center of the bead was plotted for all frames as seen in **FIGs. 19A-C** and **FIGs. 20A-C**. **FIGs. 19A-C** show pressure drops of 1, 2, and 4 kPa, respectively. **FIGs. 20A-C** show pressure drops of 1, 2, and 4 kPa, respectively. A polygon (**1900a-c** and **2000a-c** in **FIGs. 19A-C** and **FIGs. 20A-C**,

respectively) was drawn such that if the center of the bead was inside the polygon no contact is made with the ends of the chamber. It was found through high speed video observation bead never made contact with either end of the chamber from 1-4kPa pressure drop for either inlet size. Such an arrangement may further facilitate development of high energy forces within the chamber **104** to more efficiently disrupt and aerosolize medicament powder agglomerates within the chamber **104** for more effective deposition of medicament into the lungs of a patient. Such an arrangement may further facilitate development of high energy forces within the chamber **104** to more efficiently disrupt and aerosolize medicament powder agglomerates within the chamber **104** for more effective deposition of medicament into the lungs of a patient.

[0061] In general, high-energy forces may refer to dispersive forces that may strip drug from the bead **302**, and deaggregation or deagglomeration forces that may break-up or break-apart aggregates in powder fed into the chamber **104**. Here, the terms deaggregation or deagglomeration, and aggregation or agglomeration may be used interchangeably. The high-energy forces may be generated by the bead **302** when rapidly oscillating within the chamber **104** via formation of turbulence and eddies within the chamber **104**, compression and decompression zones within the chamber **104**, and the like. In some instances the bead may be spinning on its axis as well as oscillating along the axial length of the chamber. This may more effectively disrupt and aerosolize powder agglomerates within the chamber through the Magnus effect exerted by the spinning bead. The Magnus effect is a generation of a sidewise force on a spinning cylindrical or spherical solid immersed in a fluid (liquid or gas) when there is relative motion between the spinning body and the fluid.

[0062] When a DPF (Dry Powder Formulation) is passed through the chamber **104** containing the bead **302**, which is oscillating “rapidly” such as, for example, at a frequency greater than about 10 Hz, these high frequency oscillations of the bead **302** may produce high-energy forces within the chamber **104**. This may disrupt agglomerates of drug particles that may be held together at least by cohesive forces, such as by van der Waals forces, static electrical forces, etc. Additionally, physical collisions between the bead **302**, when rapidly oscillating, and potentially aggregated or agglomerated powder particles as they pass through the chamber **104** may promote de-aggregation of the agglomerates. The oscillation frequency may typically be between about 1 to about 1,000 Hz, and may preferably be between about 10 to about 500 Hz, although other

frequencies may also occur. However, in some cases, the oscillation frequency could be up to about 2,000 Hz.

[0063] As mentioned above, the example bead **302** disposed within the example chamber **104** may oscillate in a manner similar to that described in U.S. Application No. 13/469,963, filed 11 May 2012, entitled “Bead-Containing Dry Powder Inhaler.” However, in accordance with the present disclosure, the bead **302** may not include a pre-coated powder on its surface. Rather, powder may be separately introduced into the chamber **104** from a receptacle or powder storage element, such as dose containment or dosing chamber which can include but is not limited to capsules, reservoir, and blisters, or other temporary holding compartment or region, or from another dry powder inhaler, as described further below. With this configuration, the powder may be initially placed into a dose containment chamber. When a patient inhales from a mouthpiece, air may be drawn through the dose containment chamber which moves the powder into the chamber **104**, where it encounters the bead **302** oscillating primarily along the longitudinal axis **L** (see e.g., **FIG. 3**).

[0064] In some embodiments, however, the bead **302** may be coated with drug. This may act as a detachment platform for the drug coated on its surface, as well as a dispersion mechanism for drug formulation located and introduced upstream of the bead. For example, for a combination drug product, such as delivering two or more drugs in a single inhalation maneuver, where one drug is delivered in a larger dose, such as an inhaled corticosteroid, than the other drug, such as a long-acting beta-agonist, the lower dose drug may be coated onto the surface of the bead **302**, while the larger dose drug is located in a dose containment container, such as a capsule, blister, reservoir, etc., upstream of the chamber **104** containing the drug-coated bead. Thus, during inhalation, oscillation of the bead **302** may serve as a detachment platform to the drug adhered to its surface, and as a dispersion mechanism to the powder that is located upstream.

[0065] Additionally, the bead **302** may be coated with a layer of durable material. An example of such a material may include, but is not limited to, gelatin, sugars, any pharmaceutically acceptable film coating materials, including polymers, metallic coatings, anti-static coatings, plasma coatings, etc. This may be beneficial for example when bead material can erode or fragment. In this example, the layer thickness may depend on the density of the material to be added, such that the addition of the coated layer does not eliminate or substantially

impair or inhibit the ability of the bead **302** to oscillate within the chamber **104**. The bead may have various surface finish ranging from R_a (μm) 0.012 – 50, where R_a is the average surface roughness. The surface finish may affect bead motion and in turn may improve the dispersion and aerosolization of powder agglomerates within the chamber.

5 **[0066]** Using the bead **302** as a dispersion mechanism may provide a number of advantages. For example, by employing the oscillating bead in a chamber in the capacity of a dispersion engine, large doses such as, for example, about 1 mg to about 25 mg or greater, may be delivered by delivering them in capsule or blister or reservoir dose containers. However, it will be appreciated that smaller doses may also be delivered. For example, doses greater than about 1
10 μg of active drug may be delivered. In some cases, the active drug may be blended with a carrier, such as lactose. Also, when the bead **302** is not coated with drug and used as a dispersion mechanism, there is no retention mechanism required to hold the bead **302** tightly within the inhaler, decreasing the complexity of the DPF. Still further, using the bead **302** as a dispersion mechanism may require no additional or complicated processing steps for the DPF
15 formulations, as the powder may be produced by traditionally employed methods, particle engineered formulations may also be used.

[0067] Additionally, the bead **302** in the present disclosure may oscillate generally within the center of the chamber **104**, along the longitudinal axis **L**, where physical contact between the bead **302** and inner walls of the chamber **104**, and possibly ends of the chamber **104**, may occur
20 infrequently, if at all. This type of dispersion mechanism may be beneficial as collisions between walls of the chamber **104** and the bead **302** could serve to rub powder onto either the surface of the bead **302** or inner walls of the chamber **104** when powder is caught there during a physical collision, thereby decreasing an amount of powder available for transfer into the lungs of a patient. Alternatively the frequent collision of the bead **302** with the walls of the chamber
25 **104** may act to scrub off any drug adhered to the wall(s), thus increasing an amount of powder available for transfer into the lungs of a patient.

[0068] Referring still to **FIGS. 1-3**, and as mentioned above, alignment of the inlet **102** and the chamber **104**, may provide significant advantages over inhalers having an “off-axis” alignment. In particular, the tubular body **100** of the present disclosure may produce an
30 approximately symmetrical flow stream expansion that drives oscillation of the bead **302**. Such a configuration may enable a powder dispersion device, or dry powder inhaler, incorporating

aspects of the tubular body **100**, to be constructed with minimal bulk. For example, the chamber **104** in example embodiments of the present disclosure may be modeled as a cylinder of the dimensions detailed above (e.g., $d_{\text{chamber}} \sim 5.89 \text{ mm}$, $l_{\text{chamber}} \sim 10 \text{ mm}$) for a similar 4 mm bead. Accordingly, a maximum volume occupied by the chamber **104** is about 272 cubic mm based on the expression $V_{\text{cylinder}} = \pi r^2 l$.

[0069] Referring now to **FIGS. 4-5**, an example powder dispersion device or inhaler **400** is shown in accordance with the principles of the present disclosure. In particular, **FIG. 4** shows a first view of the device **400** of **FIG. 4** in cross-section. **FIG. 5** shows a perspective view of the device **400** of **FIG. 4**. The device **400** may generally incorporate aspects of the example tubular body **100** described above in connection with **FIGS. 1-3**. Additionally, or alternatively, the device **400** may generally incorporate aspects of one or more of the tubular bodies described below in connection with **FIGS. 10-14**. For example, the device **400** may include a first housing **402** comprising the inlet **102** and the chamber **104** of the tubular body **100**. Additionally, although not expressly shown, the bead **302** may be positioned within the chamber **104**, such as shown in **FIG. 3**. The device **400** may further include a second housing **404** comprising a sheath flow channel **406** that surrounds and is not in fluid connection with a primary or main powder flow channel **408**. In some embodiments, the first housing **402** may be integrally formed with the second housing **404**. In one embodiment, the chamber **104** and the main powder flow channel **408** may have at least one common structural dimension, such as internal diameter for example. Additionally, the second housing **404** may itself comprise of, be coupled to, or otherwise incorporated within, a mouthpiece adapted to be placed within the mouth of a patient, or in a nasal adapter adapted to conform to the nostrils of a patient. The device **400** may further include a plurality of flow bypass channels **410** that are formed within the second housing **404**. The flow bypass channels **410** may be in fluid connection with the sheath flow channel **406**.

[0070] The device **400** may further include a dosing chamber **412**, a retaining member **416**, and a piercing member **418** disposed at an end of the chamber opposite the inlet **102**. The piercing member **418** may puncture or otherwise perforate a capsule, blister, or powder reservoir **414** as arranged or positioned within the dosing chamber **412**. In general, the retaining member **416** may include at least one opening or aperture sized to permit air and powdered or otherwise aerosolized medicament to pass through the retaining member **416**, and to prevent the possibility of the bead **302** from exiting the chamber **104**. At least one opening or aperture may, in some

embodiments, be arranged and configured (e.g., diameter, pattern, symmetry, etc.) to maintain desired air flow characteristics with the device **400**, such that the bead **302** may disrupt and aerosolize medicament powder agglomerates within the chamber **104** to provide for more effective deposition of medicament into the lungs of a patient.

5 **[0071]** In one example, referring specifically to **FIG. 4**, a patient may prime the device **400** by puncturing the capsule, blister, or transfer of a dose from a powder reservoir **414**, and then inhale, drawing air through the chamber **104** which in turn draws the DPF from the dosing chamber **412** into the adjacent chamber **104** via the inlet **102**, where the bead **302** is rapidly oscillating, creating high-energy forces that may strip drug from the surface of carrier particles in
10 the DPF, or when the bead **302** is drug-covered, and/or de-agglomerate drug powder aggregates and drug-on-drug aggregates. Drug particles may then be deposited in lungs and airways of a patient from the primary or main powder flow channel **408** based on direction of air flow through the device such as shown in **FIG. 4**. Such a “self-dosing” scenario may be useful for effectively dispensing both traditional binary or ternary DPF formulations, drug and carrier/excipient
15 particles, and pure drug-powder formulations where there are no carrier particles are present. Other embodiments having similar effects are possible, as discussed further below.

[0072] In general, the resistance to flow of the device **400** may be adjusted by altering the geometry and/or arrangement of at least one of the inlet **102**, the bead **302**, the sheath flow channel **406**, the main powder flow channel **408**, and the flow bypass channel(s) **410**.
20 Additionally, as shown in **FIG. 5**, the flow bypass channels **410** may be located radially around the body of the second housing **404**, and fluidly connected to the sheath flow channel **406**. In some embodiments however, the device **400** may not include any flow bypass channels. In one embodiment, the flow bypass channels **410** may comprise a bypass channel where air is drawn into it via multiple individual side holes or channels located radially around the body of the
25 second housing **404**. However, other embodiments are possible. For example, the flow bypass channels **410** may comprise of different numbers and diameters of individual channels and entry points into the sheath flow channel **406**. Further, one or more of the flow bypass channels **410** may be parallel through the main powder flow channel **408**, or may be in fluid connection with, and then diverge from, the main powder flow channel **408**. Still other embodiments are possible.

30 **[0073]** One or more of the bypass channels **410** may be “opened” or “closed” such as by removal or insertion of a resilient material therein to “unplug” or “plug” the same. This may

result in changes in the overall resistance of the device **400**, thereby influencing flow rate through the device **400**. For example, a person may inhale through a “high” resistance inhaler with a lower inspiratory flow rate than they would through a “low” resistance inhaler, despite inhaling with the same inhalation effort. In this manner, the device **400** may be “tuned” to respond “optimally” to the needs of a patient. In other words, the device **400** in accordance with the present disclosure may be tailored to suit particular patient needs. For example, resistance of the device **400** may be approximately inversely proportional to diameter of the bead **302**. Thus, for a “larger” diameter bead **302**, one or more of the flow bypass channels **410** may be “closed” to increase resistance of the device such that a patient may receive a proper dose of medicament irrespective of possibly diminished inhalation capacity. Further, it is contemplated that the flow bypass channels **410** when “opened” may at least partially prevent or at least minimize the accumulation or build-up of powder in areas where non-laminar flow, such as flow eddies for example, may be present. Various other possible configurations or arrangements for such housing apertures are described in further detail below in connection with at least **FIGS. 10-14**.

[0074] Referring now to **FIG. 6**, a second view of the device **400** of **FIG. 4** is shown in cross-section. In this example, the device **400** is coupled to a mouthpiece **604** of an inhaler **602** by a coupling **606**, thereby allowing powder to flow through the inhaler **602** as during “normal” operation, and then into the chamber **104** containing the bead **302** (see also **FIG. 3**). In particular, a piercing member **612** may puncture or otherwise perforate a DPF containing capsule, blister, or powder reservoir **614** as contained within a dosing chamber **616** of the inhaler **602**. Powder may then be caused to flow through the inhaler **602** into the chamber **104** containing the bead **302** via the mouthpiece **604** and coupling **606**. The bead **302** may then disrupt and aerosolize DPF powder agglomerates within the chamber **104** to provide for more effective deposition of medicament into the lungs of a patient in a manner such as described above.

[0075] In general, the coupling **606** may be a rigid or flexible coupling formed of any material, or combination thereof, such as thermoplastic/thermosetting plastics, metals, glasses, elastomers, etc., and may be coupled to the mouthpiece **604** of the inhaler **602** on a first end **608**, and to the device **400** on a second end **610**. Here, it may be preferred that the material has surface properties that minimize the attraction of powder particles. The coupling **606** may be permanently fastened to, such as being integrally formed therewith, at least one of the inhaler

602 and the device 400, or may be removably fastened with least one of the inhaler 602 and the device 400. For example, the coupling 606 may be fastened to the inhaler 602 by one of a “snap-fit” or a “pressure-fit” or a “twist-to-fit” mechanism, etc., such as in a “quick” connect/disconnect implementation. Still other embodiments are possible. For example, it will be appreciated that the device 400 may not be limited to being “clipped” or otherwise “coupled” to other inhalers. Further, aspects of the present disclosure may be used in combination with any type of DPF dose containment system, and may not be limited to a capsule, blister, or reservoir dose containment systems.

[0076] As discussed above in connection with FIG. 4, a patient may prime the device 400 by puncturing the capsule, blister, or powder reservoir 414, and then inhale, drawing the powder from the dosing chamber 412 into the adjacent chamber 104 via the inlet 102, where the bead 302 is rapidly oscillating, creating high-energy forces that may strip drug from the surface of carrier particles (e.g., when the bead 302 is drug-covered), and/or de-agglomerate powder aggregates. Drug particles may then be deposited in lungs and airways of a patient from the primary or main powder flow channel 408 based on direction of air flow through the device such as shown in FIG. 4. Such a “self-dosing” scenario may at least be useful for effectively dispensing both traditional binary or ternary DPF formulations, drug and carrier/excipient particles, and pure drug-powder formulations where there are no carrier particles are present. Other embodiments are however possible.

[0077] For example, referring now specifically to FIG. 7, a “forced-dosing” scenario is described in accordance with the present disclosure. In particular, a third view of the device 400 of FIG. 4 is shown in cross-section in FIG. 7. In this example, a coupling 702 is shown that is removably coupled to the first housing 402 of the device 400. The coupling 702 includes an inlet 704 that is removably coupled to an air source 706. In one embodiment, an individual other than a patient may prime the device 400 by puncturing a capsule, blister, or reservoir 708 of the coupling 702 using a piercing member 710. The source 706 may then be employed to force air through the device 400, drawing powder from the reservoir 708 into the adjacent chamber 104 via the inlet 102, where the bead 302 is rapidly oscillating, creating high-energy forces that may strip drug from the surface of carrier particles (e.g., when the bead 302 is drug-covered), and/or de-agglomerate powder aggregates. Drug particles may then be deposited in lungs and airways

of the patient from the primary or main powder flow channel **408** based on direction of air flow through the device such as shown in **FIG. 7**.

[0078] Such a “forced-dosing” scenario may be beneficial when, for example, emergency treatment of unconscious or otherwise unresponsive personnel may be necessary. For example, the device **400** may enable a responder to administer treatment agent to the lungs of a patient. Additionally, the second housing **404** may itself comprise of, be coupled to, or otherwise incorporated within, a mouthpiece adapted to be placed within the mouth of a patient, or in a nasal adapter adapted to conform to the nostrils of a patient. In the example of **FIG. 7**, the second housing **404** of the device **400** may be securely positioned within or on the mouth or nasal passages of a patient. With air expelled from the lungs of a responder into the inlet **604**, the device **400** may be activated or actuated such as to deposit a treatment agent into the lungs and airways of the patient. In this example, the source **706** corresponds to the lungs of an individual. Other embodiments are possible. For example, in some embodiments the source **706** may comprise of a ventilation bag, mechanical ventilator, mechanical pump, etc. Still other embodiments are possible.

[0079] At least **FIG. 6-7** illustrate a scenario in which the example device **400** is coupled to, or fitted onto, an external feature of a dose containment system or powder source. Other embodiments are however possible. For example, referring now to **FIG. 8**, a scenario is illustrated in which the example device **400** is coupled to, or fitted onto, an internal feature of a dose containment system or powder source. In particular, the device **400** may replace a powder dispersion mechanism internal to an existing inhaler. An example of an existing inhaler may include the HandiHaler®, Twisthaler®, Turbuhaler®, Novolizer®, Plastiape RS01®, Turbospin® dry powder inhalers and others. Other embodiments are possible.

[0080] For example, a typical dose containment system or powder source **712** may generally include a dose module **714** that holds a portion of DPF, a powder dispersion module **716**, and a mouthpiece module **718** that would in practice be used to deliver a dose of the DPF to a patient. In general, the powder dispersion module **716** may exhibit a tortuous path the DPF needs to navigate between its introduction into the flow path and release from the mouthpiece module **718**. The tortuous path may possibly deaggregate DPF aggregates to some degree, but may also add flow resistance. In accordance with the principles of the present disclosure, the dose containment system or powder source **712** may be modified to replace the powder dispersion

module **716** with the device **400**, or subassemblies of the device **400**, including an inlet, chamber with a bead, and an outlet similar to the device **400**. Further, this may or may not include the second housing **404** of the device **400**, where an existing element of an inhaler being modified may instead be used. In this example, the device **400** may enhance the efficiency of de-
5 aggregation of DPF of the dose containment system or powder source **712**, and may lower the resistance to flow within the dose containment system or powder source **712**. Other benefits and advantages are possible as well.

[0081] Referring now to **FIG. 9**, a simplified, conceptual, example schematic diagram of the example device **400** of **FIG. 4** in multiple configurations is shown. In particular, the chamber
10 **104** of the device **400** is shown in a series configuration **902** with another chamber **104**, and in a parallel configuration **904** with another chamber **104**. In this example, it is contemplated that multiple drugs in each their own (e.g., two or more) dispersion chambers (e.g., in addition to other elements of the example device **400** as desired) configured in accordance with the principles of the present disclosure may be coupled in series or parallel. Further, it is
15 contemplated that any desired series/parallel combination may also be formed. For example, the series configuration **902** may be coupled in series with the parallel configuration **904**. In another example, the parallel configuration **904** may be coupled in series with a single particular chamber **104**, and etc.

[0082] In addition, it is contemplated that the type and configuration of the bead **302** may
20 vary in the context of **FIG. 9**. For example, when multiple ones of the chamber **104** are connected in series and/or parallel, one or more of the respective dispersion chambers may have similar bead sizes, different bead sizes, similar bead materials, different bead materials, and etc. Further, it is contemplated that any desired series/parallel combination may be formed. In general, type and configuration of the bead **302** may vary as desired.

[0083] Such an implementation may be beneficial in many respects. For example, for
25 combination therapies, one drug may pass through a particular dispersion chamber and another other drug may pass through a separate dispersion chamber, or both drugs can pass through the same dispersion chamber. Additionally, “downstream” of the dispersion chambers may merge into a single dispersion chamber, or be kept separate throughout the length of the device **400**,
30 such that the powders do not mix until they are emitted from the device. Still other benefits and/or advantages are possible as well.

[0084] Referring now to **FIG. 10**, a cross-section of a second example tubular body **1000** having an inlet **1002** and a dispersion chamber **1004** is shown according to the principles of the present disclosure. In many aspects, the second example tubular body **1000** is similar to at least the tubular body **100** of **FIG. 1**. For example, a fluid flow path of the inlet **1002** is defined by a first internal diameter **1006** that varies or tapers along a longitudinal axis **L**, and a fluid flow path of the dispersion chamber **1004** is defined by a second internal diameter **1008**. Further, one or more apertures **1010** are formed within the tubular body **1000** at particular locations to allow a secondary supply of air or air flow **1012** (sometimes referred to as “chase air”) to enter the tubular body **1000** during its use, to prevent or at least minimize the unintended accumulation or build-up of powder within the tubular body **1000**. In particular, it will be appreciated that air flowing through the one or more apertures **1010** may advantageously prevent or at least minimize the unintended accumulation or build-up of powder within internal edges or corners **1014** of the tubular body **1000** that are substantially adjacent the inlet **1002**, because the force of that air would push powder away from the corners **1014** into the primary air stream **1016** for subsequent deposition into the lungs of a patient in a manner similar to that as discussed above. Among other things, this may advantageously increase the efficiency of powder deposition into the lungs of a patient, prevent build-up of powder that can dislodge in subsequent uses of the chamber as a multi-dose inhaler device resulting in a super-dose to be delivered to the patient, and/or prevent undesired waste of powder.

[0085] Additionally, or alternatively, the corners **1014** of the tubular body **1000** may be formed to exhibit rounded or curved surfaces to prevent or at least minimize the unintended accumulation or build-up of powder within the tubular body **100**. **FIG. 14** in particular shows the corners **1014** of the tubular body **1000** formed to exhibit rounded or curved surfaces, without the apertures **1010**. Other embodiments are possible. For example, **FIG. 15** in particular shows corners **1015** of the tubular body **1000** that are formed to exhibit rounded or curved surfaces on an end of the tubular body **1000** opposite corners **1014**. Further, apertures **1017** are formed within the tubular body **1000** near or adjacent the corners **1015**. It is contemplated that any feature or element discussed as being near or adjacent the inlet **1002** may additionally, or alternatively, be formed on an end of the tubular body **1000** opposite of the inlet **1002**, such as shown in **FIG. 15**. This principle is applicable to each respective tubular body discussed in the context of the present disclosure. Further, the configuration and particular geometry of the

corners **1015** and/or the apertures **1017** need not necessarily be the same as that exhibited by the corners **1014** and/or apertures **1010**. For example, the tubular body **1000** as shown in **FIG. 15** may have a first portion **1019** configured similar to that shown in **FIG. 12**, whereas a second portion **1021** may be configured as shown in **FIG. 15**. Still many other embodiments are possible.

[0086] It will be appreciated that such rounded or curved surfaces may more effectively prevent powder from accumulating or adhering to portions of the corners **1014** when compared to other profiles that have a sharp transition between surfaces, such as the stepped-edge profile shown in **FIG. 1**. In addition to providing desirable fluid flow characteristics, one or both of the apertures **1010** and the rounded corners **1014** may further facilitate efficient and effective fabrication of the tubular body **1000** by injection molding for example.

[0087] In the example of **FIG. 10**, the secondary air flow **1012** comprises air flowing through the apertures **1010** and into the dispersion chamber **1004** in a substantially or approximately parallel direction to the primary air stream **1016**. Many other embodiments are possible. For example, referring now to **FIG. 11**, a cross-section of the second example tubular body **1000** is shown whereby the apertures **1010** are formed such that the secondary air flow **1012** comprises air flowing through the one or more apertures **1010** and into the dispersion chamber **1004** in a substantially or approximately perpendicular direction to the primary air stream **1016**. The benefits associated with the secondary air flow **1012** are similar to that described above in connection with **FIG. 10**.

[0088] Further, it is contemplated that the tubular body **1000** may be fabricated to exhibit the arrangement or configuration of the apertures **1010** as shown in **FIG. 10** together with the arrangement or configuration of the apertures **1010** as shown in **FIG. 11**. In either case, that is, in scenarios where the tubular body **1000** is fabricated to incorporate the apertures **1010** as shown in **FIG. 10** or **FIG. 11**, or where the tubular body **1000** is fabricated to incorporate the apertures **1010** as shown in both **FIG. 10** and **FIG. 11**, it is contemplated that the diameter of the apertures **1010** (i.e., when circular, however, other polygonal apertures are contemplated) in addition to the spatial arrangement of the apertures **1010** may be defined so that the desired fluid flow characteristics of the tubular body **1000** are realized. For example, the apertures **1010** may be defined within the tubular body **1000** so as to exhibit a specific pattern or symmetry that facilitates deposition of powder into the lungs of a patient, in tandem with preventing or at least

minimizing the accumulation or build-up of powder in or near the corners **1014** of the tubular body **1000**. Further, it is contemplated that the apertures **1010** may be formed or defined by means other than an injection molding technique for example.

[0089] For example, referring now to **FIG. 12**, a cross-section of the second example tubular body **1000** is shown whereby the body of the inlet **1002** and the body of the dispersion chamber **1004** are not integral, but rather are separate pieces so that apertures **1010** are formed by a gap(s) between the body of the inlet **1002** and the body of the dispersion chamber **1004**, when those two pieces are generally coupled together. In this example, the apertures **1010** are formed such that the secondary air flow **1012** comprises air flowing through the apertures **1010** and into the dispersion chamber **1004** in a substantially or approximately off-axis direction in reference to the primary air stream **1016** and/or the longitudinal axis **L**. It is contemplated that such a multi-piece arrangement or configuration may take many different forms, where a particular multi-piece arrangement or configuration may be implementation-specific, and/or possibly fabrication-method-specific, and so thus may evolve as requirements or specifications, and possibly fabrication technologies or techniques, evolve.

[0090] For example, referring now to **FIG. 13**, at least a cross-section of a third example tubular body **1300** having an inlet **1302** and a dispersion chamber **1304** is shown according to the principles of the present disclosure. In many aspects, the tubular body **1300** is similar to at least the tubular body **1000** of **FIG. 10**. For example, a fluid flow path of the inlet **1302** is defined by an internal diameter **1306** that varies or tapers along a longitudinal axis **L**, and a fluid flow path of the dispersion chamber **1304** is defined by an internal diameter **1308**. Further, the body of the inlet **1302** and the body of the dispersion chamber **1304** are not integral, but rather are separate pieces so that one or more apertures **1310** are formed by a gap(s) between the body of the inlet **1302** and the body of the dispersion chamber **1304** when those two pieces are generally coupled together. More specifically, the dispersion chamber **1304** is formed to exhibit notches **1312**, and when the body of the inlet **1302** and the body of the dispersion chamber **1304** are generally coupled, the apertures **1310** are formed as gaps between the body of the inlet **1302** and the body of the dispersion chamber **1304**. In general, it is contemplated that the notches **1312** may be defined as desired so that the apertures **1310** exhibit a specific shape, pattern, and/or symmetry that facilitates deposition of powder into the lungs of a patient, in tandem with preventing or at

least minimizing the accumulation or build-up of powder in or near internal surfaces of the mated assembly as shown in **FIG. 13**, and in particular the dispersion chamber **1304**.

[0091] The features or aspects of the present disclosure may be beneficial and/or advantageous in many respects. For example, to help minimize the buildup or accumulation of powder within at least the above-described dispersion chambers, it is contemplated that the outside corners of the inlet surface of the chamber may be formed so that “small” amounts of air are allowed to flow into the outermost corner via a gap/holes at the outermost edge of the inlet surface and the chamber cylinder. The dimension of the gap or gaps may be critical so as to allow sufficient air to flow into the outermost corner to minimize or prevent powder buildup, essentially sweeping away or causing the powder trapped there by the eddies not to build up in the first place. The flow though still is low enough not to alter the linear oscillation characteristics of the bead, and the negative pressure field that is present in the chamber that draws the bead back toward the inlet when air flows into the main inlet to the chamber, and is above the level needed to make the bead oscillate. The “corner air flow” can be via holes in the corner, or via a designed-in gap caused by the design of the mating parts that make up the cylinder. It is contemplated that less than about 25% of the main flow, less than about 10% of the main, less than about 5% of the main flow, or less about than about 1% of the main flow may prevent powder buildup in the corners, depending on the characteristics of the powder deposited in the corners and the physical properties and components thereof.

[0092] Additional features could further improve the disruption and dispersion of powder agglomerates within the chamber by the bead. The additional features may include ribs **2102** in the chamber of inhaler **2100** as shown in **FIG. 21** that would restrict the circumferential movement of the bead limiting the bead to axial movements. This may increase the speed and frequency of the bead oscillation in the chamber. In addition the retention feature **2216** that keeps the bead from exiting the chamber could be constructed from a wing as shown in cross section in **FIG. 22**. The wing as a retention feature **2216** could have several benefits to the design such as lowering inhaler resistance and increasing bead speed and or frequency among other possible benefits. In some embodiments, two or more beads **2304** may be placed in a single chamber as shown in **FIG. 23**, this may improve the disruption and dispersion of powder agglomerates within the chamber.

[0093] A specific embodiment of the inhaler **2400** has been created using the Plastiap RS01 dry powder inhaler (Plastiap S.p.a, Italy) as the dose containment and delivery system. This embodiment utilizes the capsule piercing and dose delivery system from a Plastiap RS01 to feed powder into the chamber with the oscillating actuator, a spherical bead as seen in **FIGs. 24-25**.

After piercing a capsule **2402**, air flows through inlet passages **2404** and the pierced capsule **2402** is lifted from the piercing chamber **2408** and rotates about its axis to efficiently empty the capsule **2402**. The aerosolized powder exiting the rotating capsule **2402** flows through a grid that serves as a flow straightening element **2406** and is fed into the chamber with the oscillating spherical bead. The design utilizes a conical frustum inlet from the Plastiap RS01 inhaler to the inlet diameter **106**. Experiments using a Next Generation Impactor (NGI) with this design have shown an emitted fine particle fraction (%FPF, with a fine particle cutoff $<5.3\mu\text{m}$) greater than 70% with several different active pharmaceutical ingredients (API). Emitted fine particle fraction (%FPF) is defined as the fraction of emitted mass below a cutoff diameter divided by the emitted mass from the inhaler. An experiment was performed testing this embodiment at 2 and 4 kPa with 20mg 20% Vardenafil (HCl)₂ in a lactose blend. This inhaler **2400** used $d_{\text{bead}} = 4.00$ mm, $d_{\text{inlet}} = 2.72$ mm, $d_{\text{chamber}} = 5.89$ mm, $l_{\text{chamber}} = 10$ mm, with 2 bypass channels open which resulted in a resistance = $0.104(\text{cm H}_2\text{O}^{0.5}/\text{LPM})$. Results show that this embodiment achieved similar aerosol performance at 2 and 4 kPa as shown in **FIG. 26**.

[0094] Typically drug powder deposition on the inhaler device components in dry powder inhalers changes with air flow rate. An experiment was conducted using the embodiment exhibited in **FIG. 24** and **FIG. 25**. This inhaler used $d_{\text{bead}} = 4.00$ mm, $d_{\text{inlet}} = 2.72$ mm, $d_{\text{chamber}} = 5.89$ mm, $l_{\text{chamber}} = 10$ mm, with 2 bypass channels which resulted in a resistance = $0.104(\text{cm H}_2\text{O}^{0.5}/\text{LPM})$. The inhaler was loaded with 20 mg of 20% Vardenafil (HCl)₂ and the amount of drug deposited in the capsule containment **2400**, dispersion chamber **104** and bead **304**, and mouthpiece **406** components as shown in **FIG. 27**. The inhaler was tested at 60 and 150 LPM (4 and 24 kPa respectively). Surprisingly the drug deposition by % mass was largely unchanged in the dispersion chamber **104**, bead **304**, and mouthpiece **408** sections despite a 250% increase in inhaler flow as shown in **TABLE 4**.

TABLE 4

Inhaler portion	60LPM	150LPM
Capsule containment	14.6%	8.1%

Chamber and bead	2.1%	1.7%
Mouthpiece	6.2%	6.3%

[0095] Although the subject matter has been described in language specific to structural features and/or methodological acts, it is to be understood that the subject matter defined in the appended claims is not necessarily limited to the specific features or acts described above.

- 5 Rather, the specific features and acts described above are disclosed as example forms of implementing the claims.

WHAT IS CLAIMED IS:

- 1 1. A dry powder inhaler, comprising:
2 a powder storage element configured to hold a powdered medicament;
3 an inlet channel configured to receive powdered medicament from the powder
4 storage element that is entrained in an airflow, the inlet channel having a portion with a first
5 diameter and defining an opening;
6 a dispersion chamber that is adapted to receive the airflow and the powdered
7 medicament from the opening of the inlet channel, the dispersion chamber having a second
8 diameter;
9 an actuator housed within the dispersion chamber, the actuator being configured
10 to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the
11 powdered medicament entrained in the airflow passing through the dispersion chamber, wherein
12 a ratio between the first diameter and the second diameter is between about 0.40 and 0.60 such
13 that an audible sound is produced as the actuator oscillates; and
14 an outlet channel through which the airflow and powdered medicament exit the
15 inhaler for delivery to a patient.
- 1 2. The dry powder inhaler according to claim 1, wherein:
2 the dispersion chamber has a length;
3 the actuator has a diameter, and
4 the length of the dispersion chamber is between about 2 and 3.5 times larger than
5 the diameter of the actuator such that an audible sound is produced as the actuator oscillates.
- 1 3. The dry powder inhaler according to claim 1, wherein the opening is non-
2 circular.
- 1 4. The dry powder inhaler according to claim 1, wherein the geometry of the
2 inhaler is such that a flow profile is generated within the dispersion chamber that substantially
3 prevents accumulation or deposits of the powdered medicament to internal surfaces of the
4 dispersion chamber.
- 1 5. The dry powder inhaler according to claim 1, wherein the airflow is
2 substantially coaxial with a longitudinal axis of the dispersion chamber.
- 1 6. The dry powder inhaler according to claim 1, wherein the powdered
2 medicament is packaged in one or more blisters, one or more capsules, or one or more reservoirs.

1 7. The dry powder inhaler according to claim 5, further comprising a
2 piercing member configured to puncture the one or more blisters or the one or more capsules.

1 8. The dry powder inhaler according to claim 1, wherein internal corners of
2 the inhaler have curved surfaces to minimize build-up of the powdered medicament within the
3 inhaler.

1 9. The dry powder inhaler according to claim 1, wherein the actuator
2 comprises one or more beads.

1 10. The dry powder inhaler according to claim 1, wherein the inlet channel is
2 conical frustum shaped.

1 11. The dry powder inhaler according to claim 1, wherein the dispersion
2 chamber defines at least one aperture configured to receive chase air separate from the airflow
3 entering in through the inlet channel.

1 12. A dry powder inhaler, comprising:
2 a powder storage element configured to hold a powdered medicament;
3 an inlet channel configured to receive powdered medicament from the powder
4 storage element that is entrained in an airflow, the inlet channel defining an opening;
5 a dispersion chamber that is adapted to receive the airflow and the powdered
6 medicament from the opening of the inlet channel, the dispersion chamber having a length;
7 a bead housed within the dispersion chamber, the bead being configured to
8 oscillate within the dispersion chamber when exposed to the airflow so as to deaggregate the
9 powdered medicament entrained by the airflow passing through the dispersion chamber, the bead
10 having a diameter, wherein the length of the dispersion chamber is between about 2 and 3.5
11 times larger than the diameter of the bead such that an audible sound is produced as the bead
12 oscillates; and
13 an outlet channel through which the airflow and powdered medicament exit the
14 inhaler for delivery to a patient.

1 13. The dry powder inhaler according to claim 12, wherein the dispersion
2 chamber has a first end and a second end, and wherein the bead rarely contacts the first end or
3 the second end while oscillating.

1 14. The dry powder inhaler according to claim 12, wherein the bead is
2 configured to spin along an axis while oscillating along the length of the dispersion chamber.

1 15. The dry powder inhaler according to claim 12, wherein the bead has a
2 surface finish having an average roughness of between 0.012 and 50 μm .

1 16. The dry powder inhaler according to claim 12, wherein the dispersion
2 chamber comprises one or more ribs configured to restrict circumferential movement of the bead
3 such that motion of the bead is substantially limited to axial movement along the length of the
4 dispersion chamber.

1 17. The dry powder inhaler according to claim 12, wherein the bead comprises
2 a second powdered medicament adhered thereto.

1 18. The dry powder inhaler according to claim 12, wherein the diameter of the
2 bead is between about 0.5 and 15 mm.

1 19. The dry powder inhaler according to claim 12, wherein the geometry of
2 the inhaler is such that a flow profile is generated within the dispersion chamber that
3 substantially prevents accumulation or deposits of the powdered medicament to internal surfaces
4 of the dispersion chamber.

1 20. The dry powder inhaler according to claim 12, wherein the inlet channel is
2 tapered from a first position to a smaller second position.

1 21. The dry powder inhaler according to claim 20, wherein the dispersion
2 chamber defines at least one aperture configured to receive chase air separate from the airflow
3 entering in through the inlet channel.

1 22. A dry powder inhaler, comprising:
2 a powder storage element configured to hold a powdered medicament;
3 an inlet channel configured to receive powdered medicament from the powder
4 storage element that is entrained in an airflow, the inlet channel having a portion with a first
5 diameter and defining an opening;

6 a dispersion chamber that is adapted to receive the airflow and the powdered
7 medicament from the opening of the inlet channel, the dispersion chamber having a second
8 diameter and a length;

9 a bead housed within the dispersion chamber, the bead being configured to
10 oscillate within the dispersion chamber when exposed to the airflow to deaggregate the
11 powdered medicament entrained by the airflow passing through the dispersion chamber, the bead
12 having a third diameter, wherein a ratio between the first diameter and the second diameter is

13 between about 0.40 and 0.66 and the length is between about 2 and 3.5 times larger than the third
14 diameter such that an audible sound is produced as the bead oscillates; and

15 an outlet channel through which the airflow and powdered medicament exit the
16 inhaler for delivery to a patient.

1 23. The dry powder inhaler according to claim 22, further comprising a
2 retaining member disposed at an end of the dispersion chamber opposite the inlet channel, the
3 retaining member configured to maintain the bead within the dispersion chamber while
4 permitting the airflow to flow to the outlet channel.

1 24. The dry powder inhaler according to claim 23, wherein the retaining
2 member comprises a wing.

1 25. The dry powder inhaler according to claim 22, wherein the powdered
2 medicament is contained within a capsule, and wherein the inhaler further comprises a piercing
3 member configured to puncture the capsule and a rotating mechanism configured to rotate the
4 punctured capsule to empty the powdered medicament from the punctured capsule.

1 26. The dry powder inhaler according to claim 22, wherein the inlet channel is
2 conical frustum shaped.

1 27. The dry powder inhaler according to claim 22, wherein the geometry of
2 the inhaler is such that a flow profile is generated within the dispersion chamber that
3 substantially prevents accumulation or deposits of the powdered medicament to internal surfaces
4 of the dispersion chamber.

1 28. The dry powder inhaler according to claim 22, wherein the dispersion
2 chamber defines at least one aperture configured to receive chase air separate from the airflow
3 entering in through the inlet channel.

1 29. A dry powder inhaler, comprising:
2 a powder storage element configured to hold a powdered medicament;
3 a conical or pyramid frustum shaped inlet channel configured to receive powdered
4 medicament from the powder storage element that is entrained in an airflow;
5 a dispersion chamber that is adapted to receive the airflow and the powdered
6 medicament from the opening of the inlet channel;

7 an actuator housed within the dispersion chamber, the actuator being configured
8 to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the
9 powdered medicament entrained by the airflow passing through the dispersion; and

10 an outlet channel through which the airflow and powdered medicament exit the
11 inhaler for delivery to a patient.

1 30. A dry powder inhaler, comprising:

2 a powder storage element configured to hold a powdered medicament;

3 an inlet channel configured to receive powdered medicament from the powder
4 storage element that is entrained in an airflow;

5 a dispersion chamber that is adapted to receive the airflow and the powdered
6 medicament from the opening of the inlet channel, wherein the airflow is substantially coaxial
7 with a longitudinal axis of the dispersion chamber;

8 an actuator housed within the dispersion chamber, the actuator being configured
9 to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the
10 powdered medicament entrained by the airflow passing through the dispersion chamber; and

11 an outlet channel through which the airflow and powdered medicament exit the
12 inhaler for delivery to a patient.

1 31. A dry powder inhaler, comprising:

2 a powder storage element configured to hold a powdered medicament;

3 an inlet channel configured to receive powdered medicament from the powder
4 storage element that is entrained in an airflow, the inlet channel defining an opening, wherein the
5 inlet channel comprises a flow straightener;

6 a dispersion chamber that is adapted to receive the airflow and the powdered
7 medicament from the opening of the inlet channel;


8 an actuator housed within the dispersion chamber, the actuator being configured
9 to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the
10 powdered medicament entrained by the airflow passing through the dispersion chamber and

11 an outlet channel through which the airflow and powdered medicament exit the
12 inhaler for delivery to a patient.

1 32. The dry powder inhaler according to claim 31, wherein the flow

2 straightener comprises a grid that is positioned across an opening of the inlet channel.

- 1 33. A dry powder inhaler, comprising:
2 a powder storage element configured to hold a powdered medicament;
3 an inlet channel configured to receive powdered medicament from the powder
4 storage element that is entrained in an airflow, the inlet channel defining an opening, wherein the
5 inlet channel tapers from a first distal shape to a smaller second proximal shape;
6 a dispersion chamber that is adapted to receive the airflow and the powdered
7 medicament from the opening of the inlet channel;
8 an actuator housed within the dispersion chamber, the actuator being configured
9 to oscillate within the dispersion chamber when exposed to the airflow to deaggregate the
10 powdered medicament entrained by the airflow passing through the dispersion chamber; and
11 an outlet channel through which the airflow and powdered medicament exit the
12 inhaler for delivery to a patient.
- 1 34. The dry powder inhaler according to claim 33, wherein the first distal
2 shape and the second proximal shape are different.
- 1 35. The dry powder inhaler according to claim 33, wherein the first distal
2 shape and the second proximal shape are the same.
- 1 36. The dry powder inhaler according to claim 33, wherein the second
2 proximal shape comprises a rectangle.

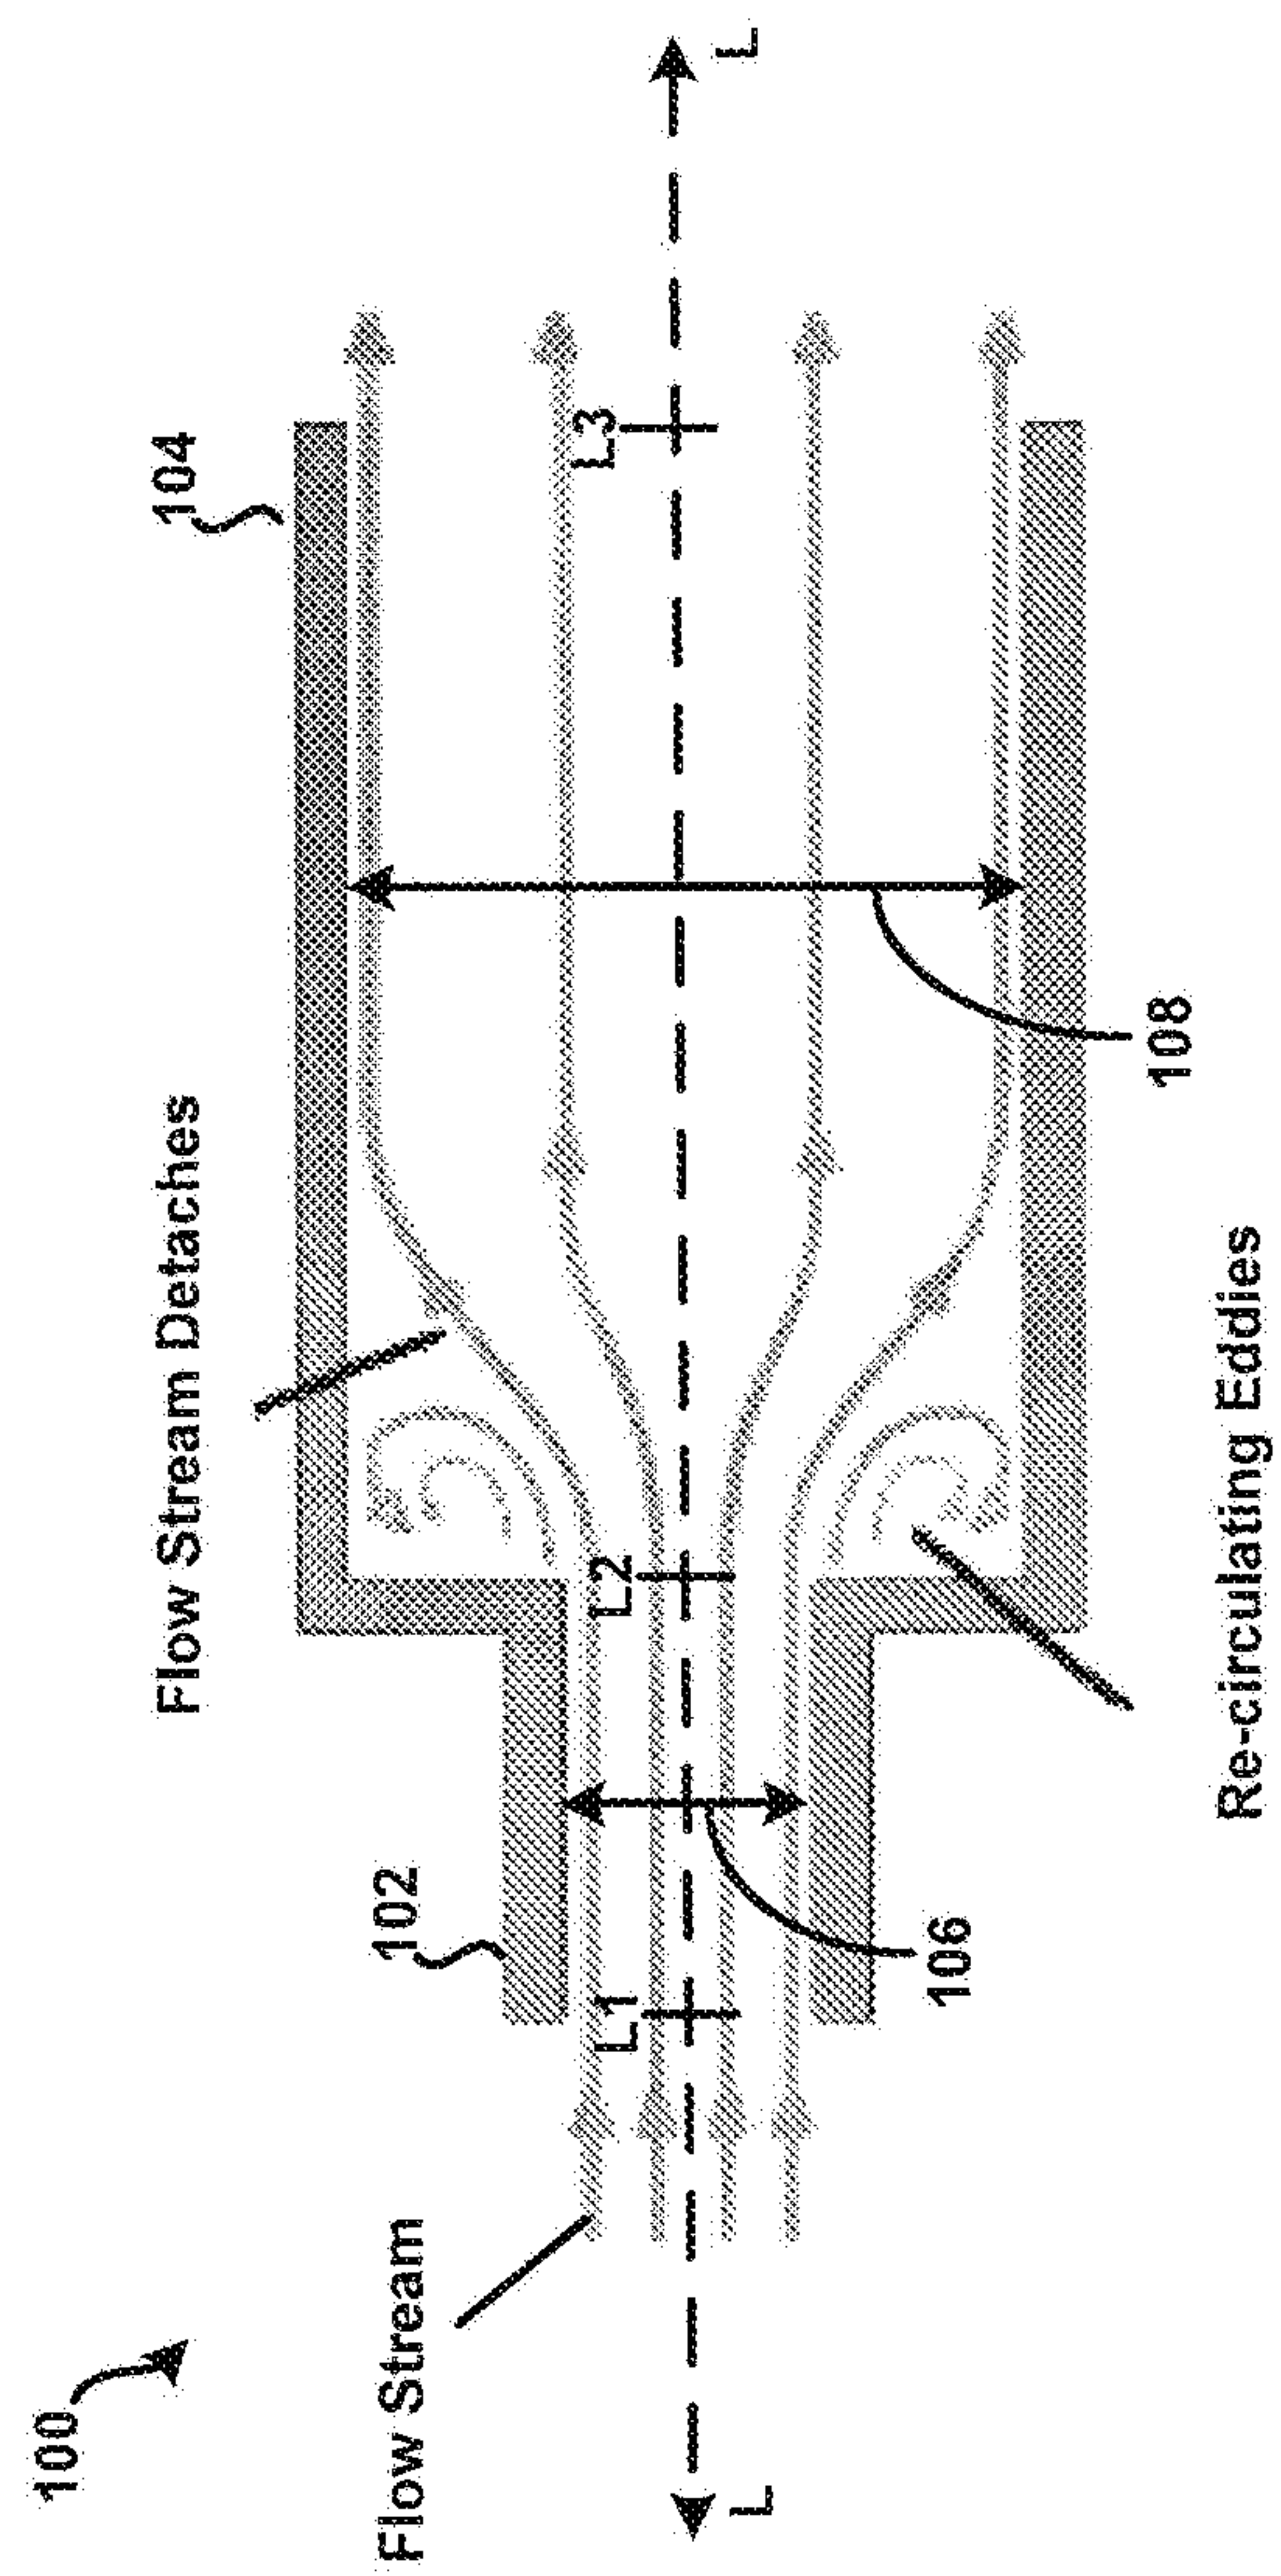

१७६

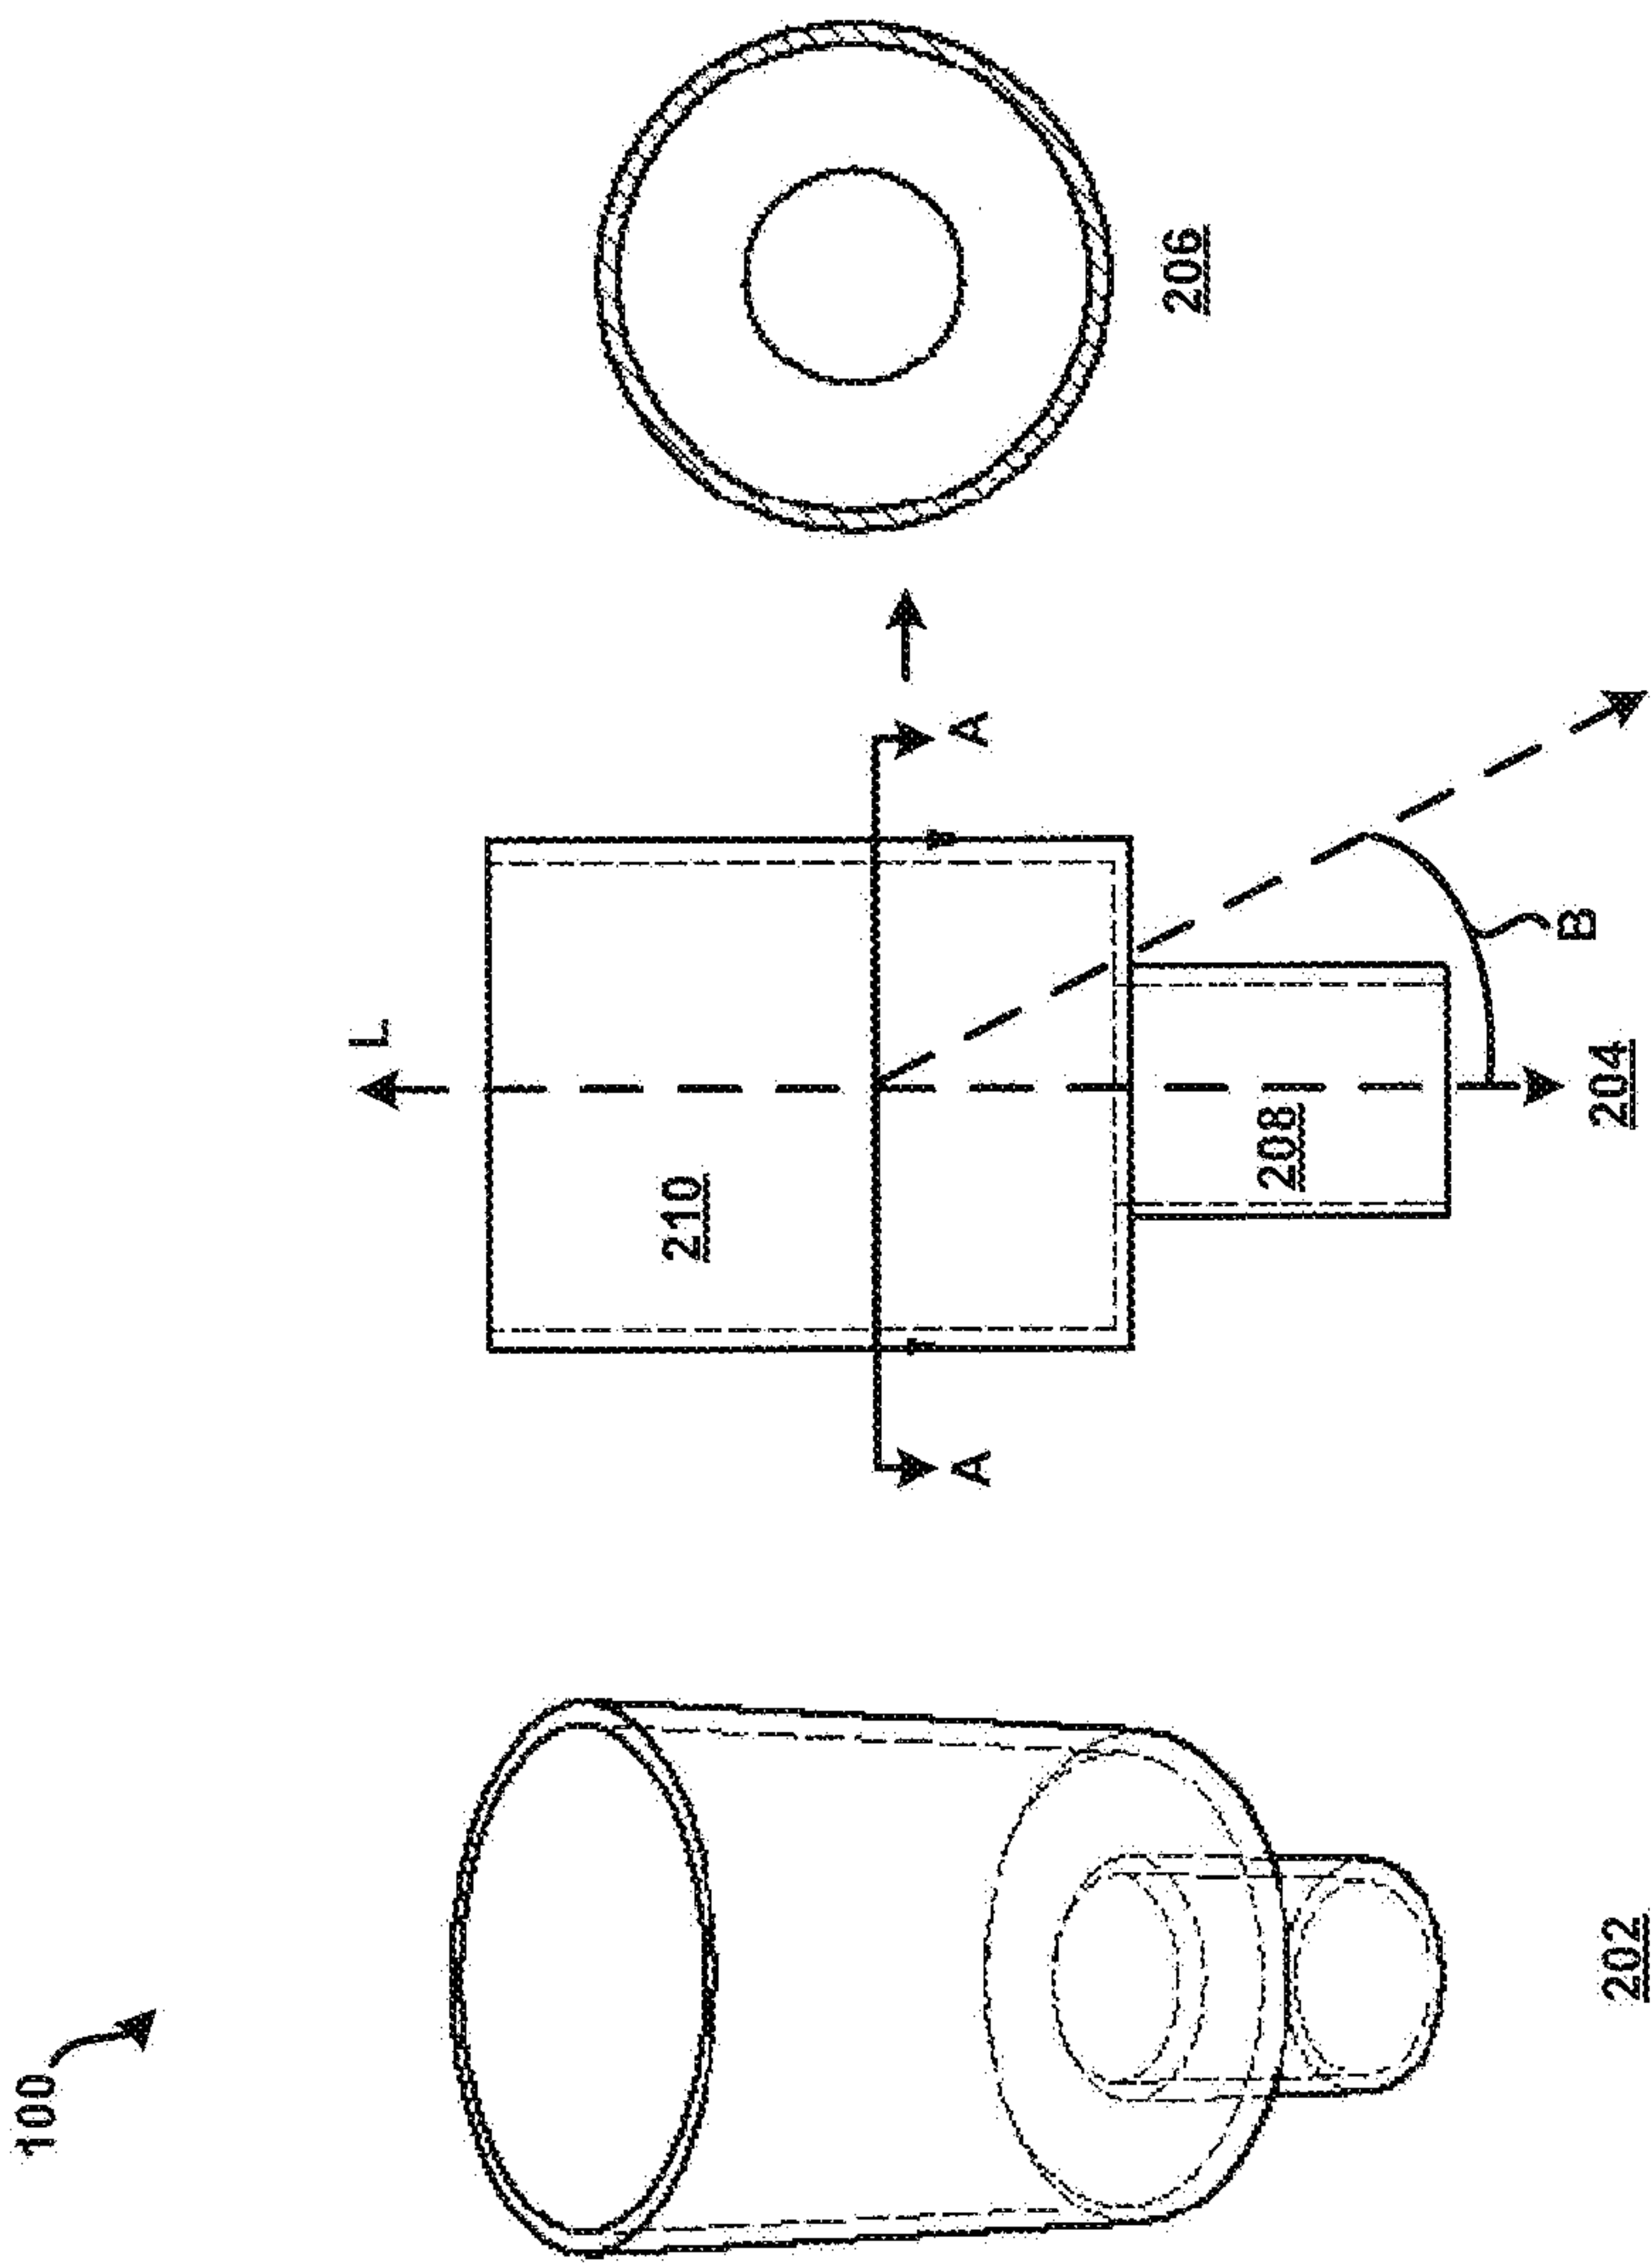


FIG. 2

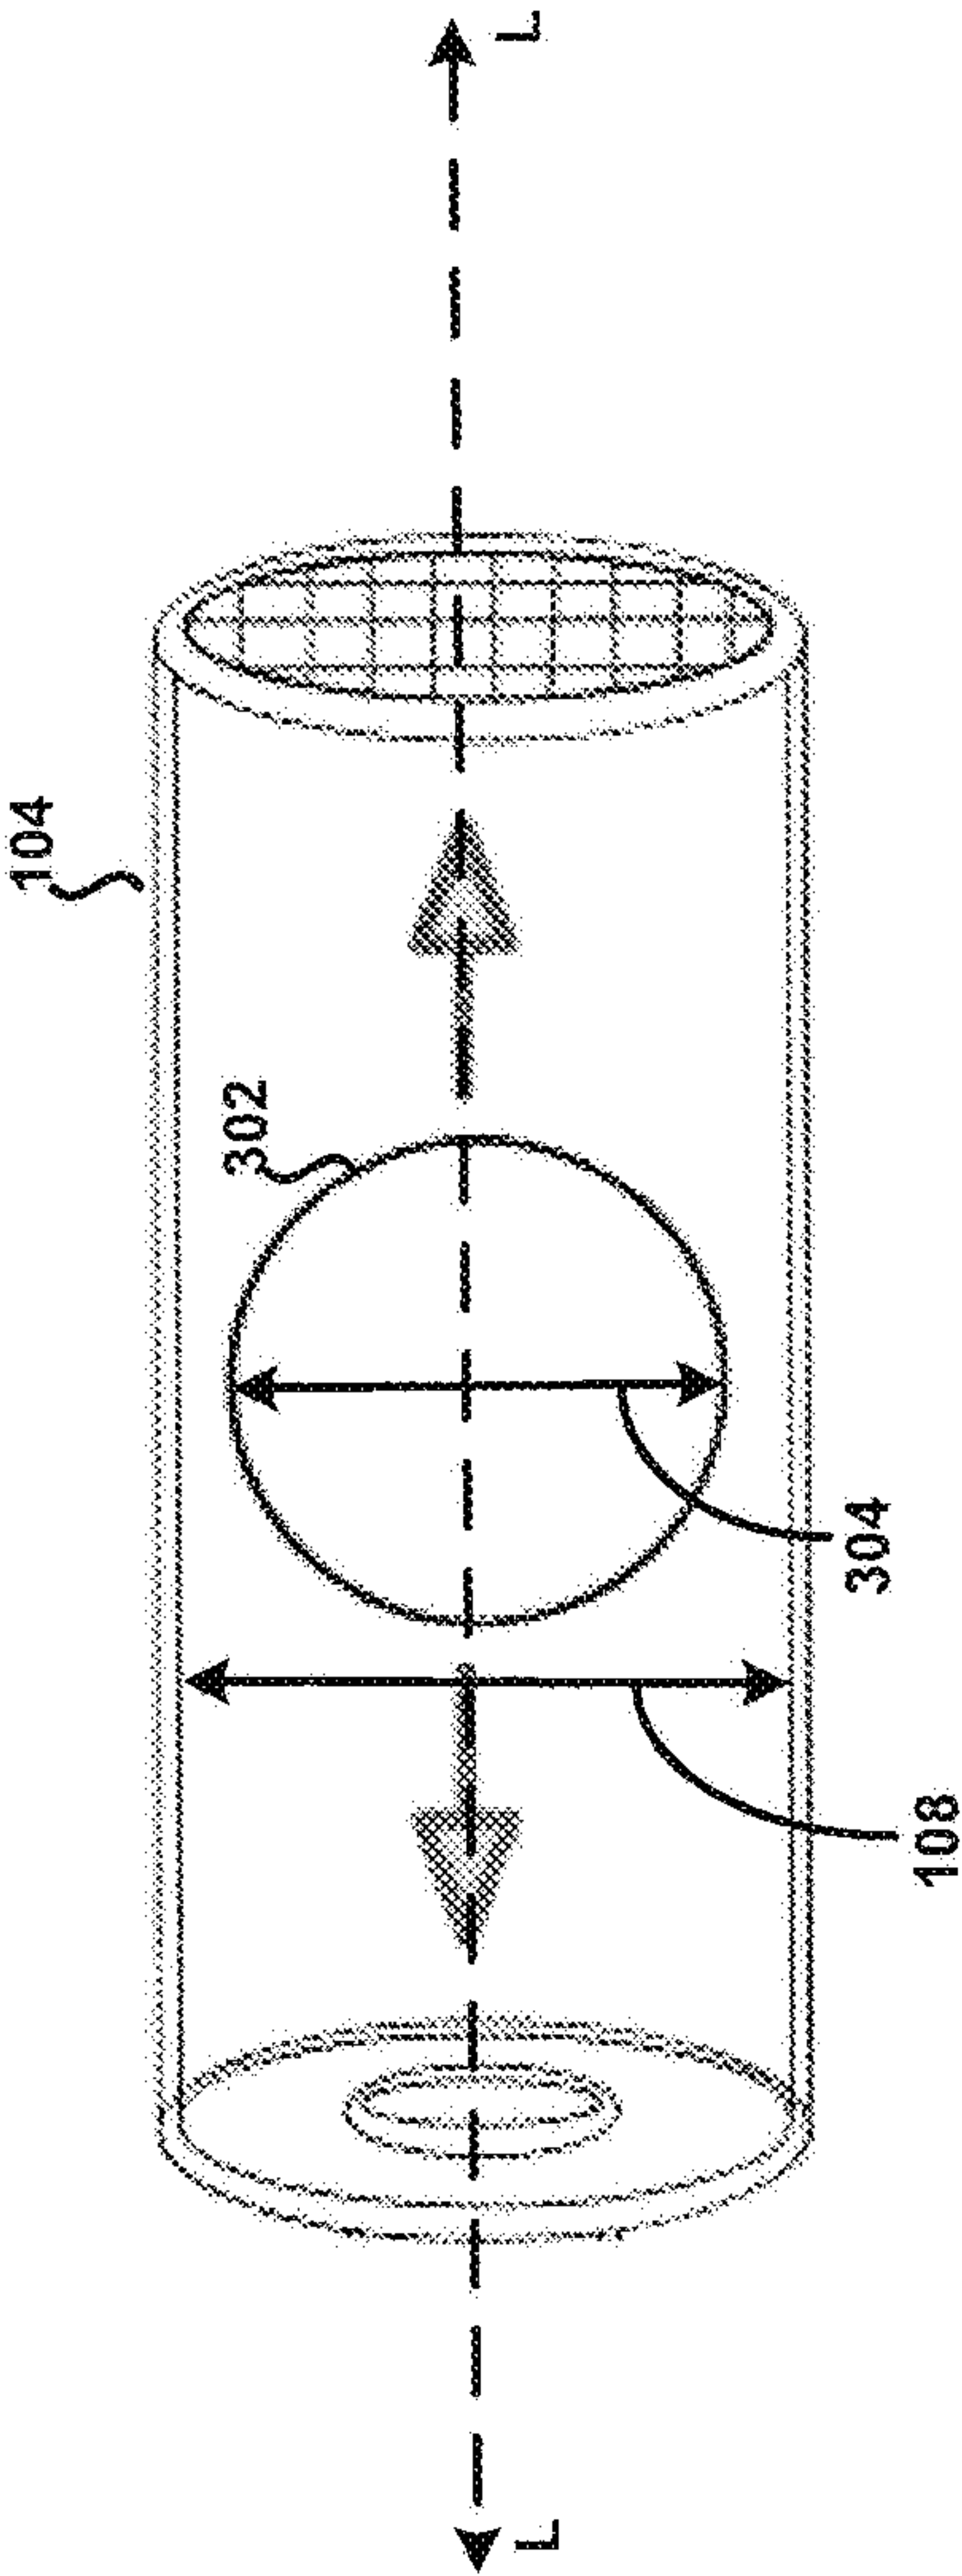


FIG. 3

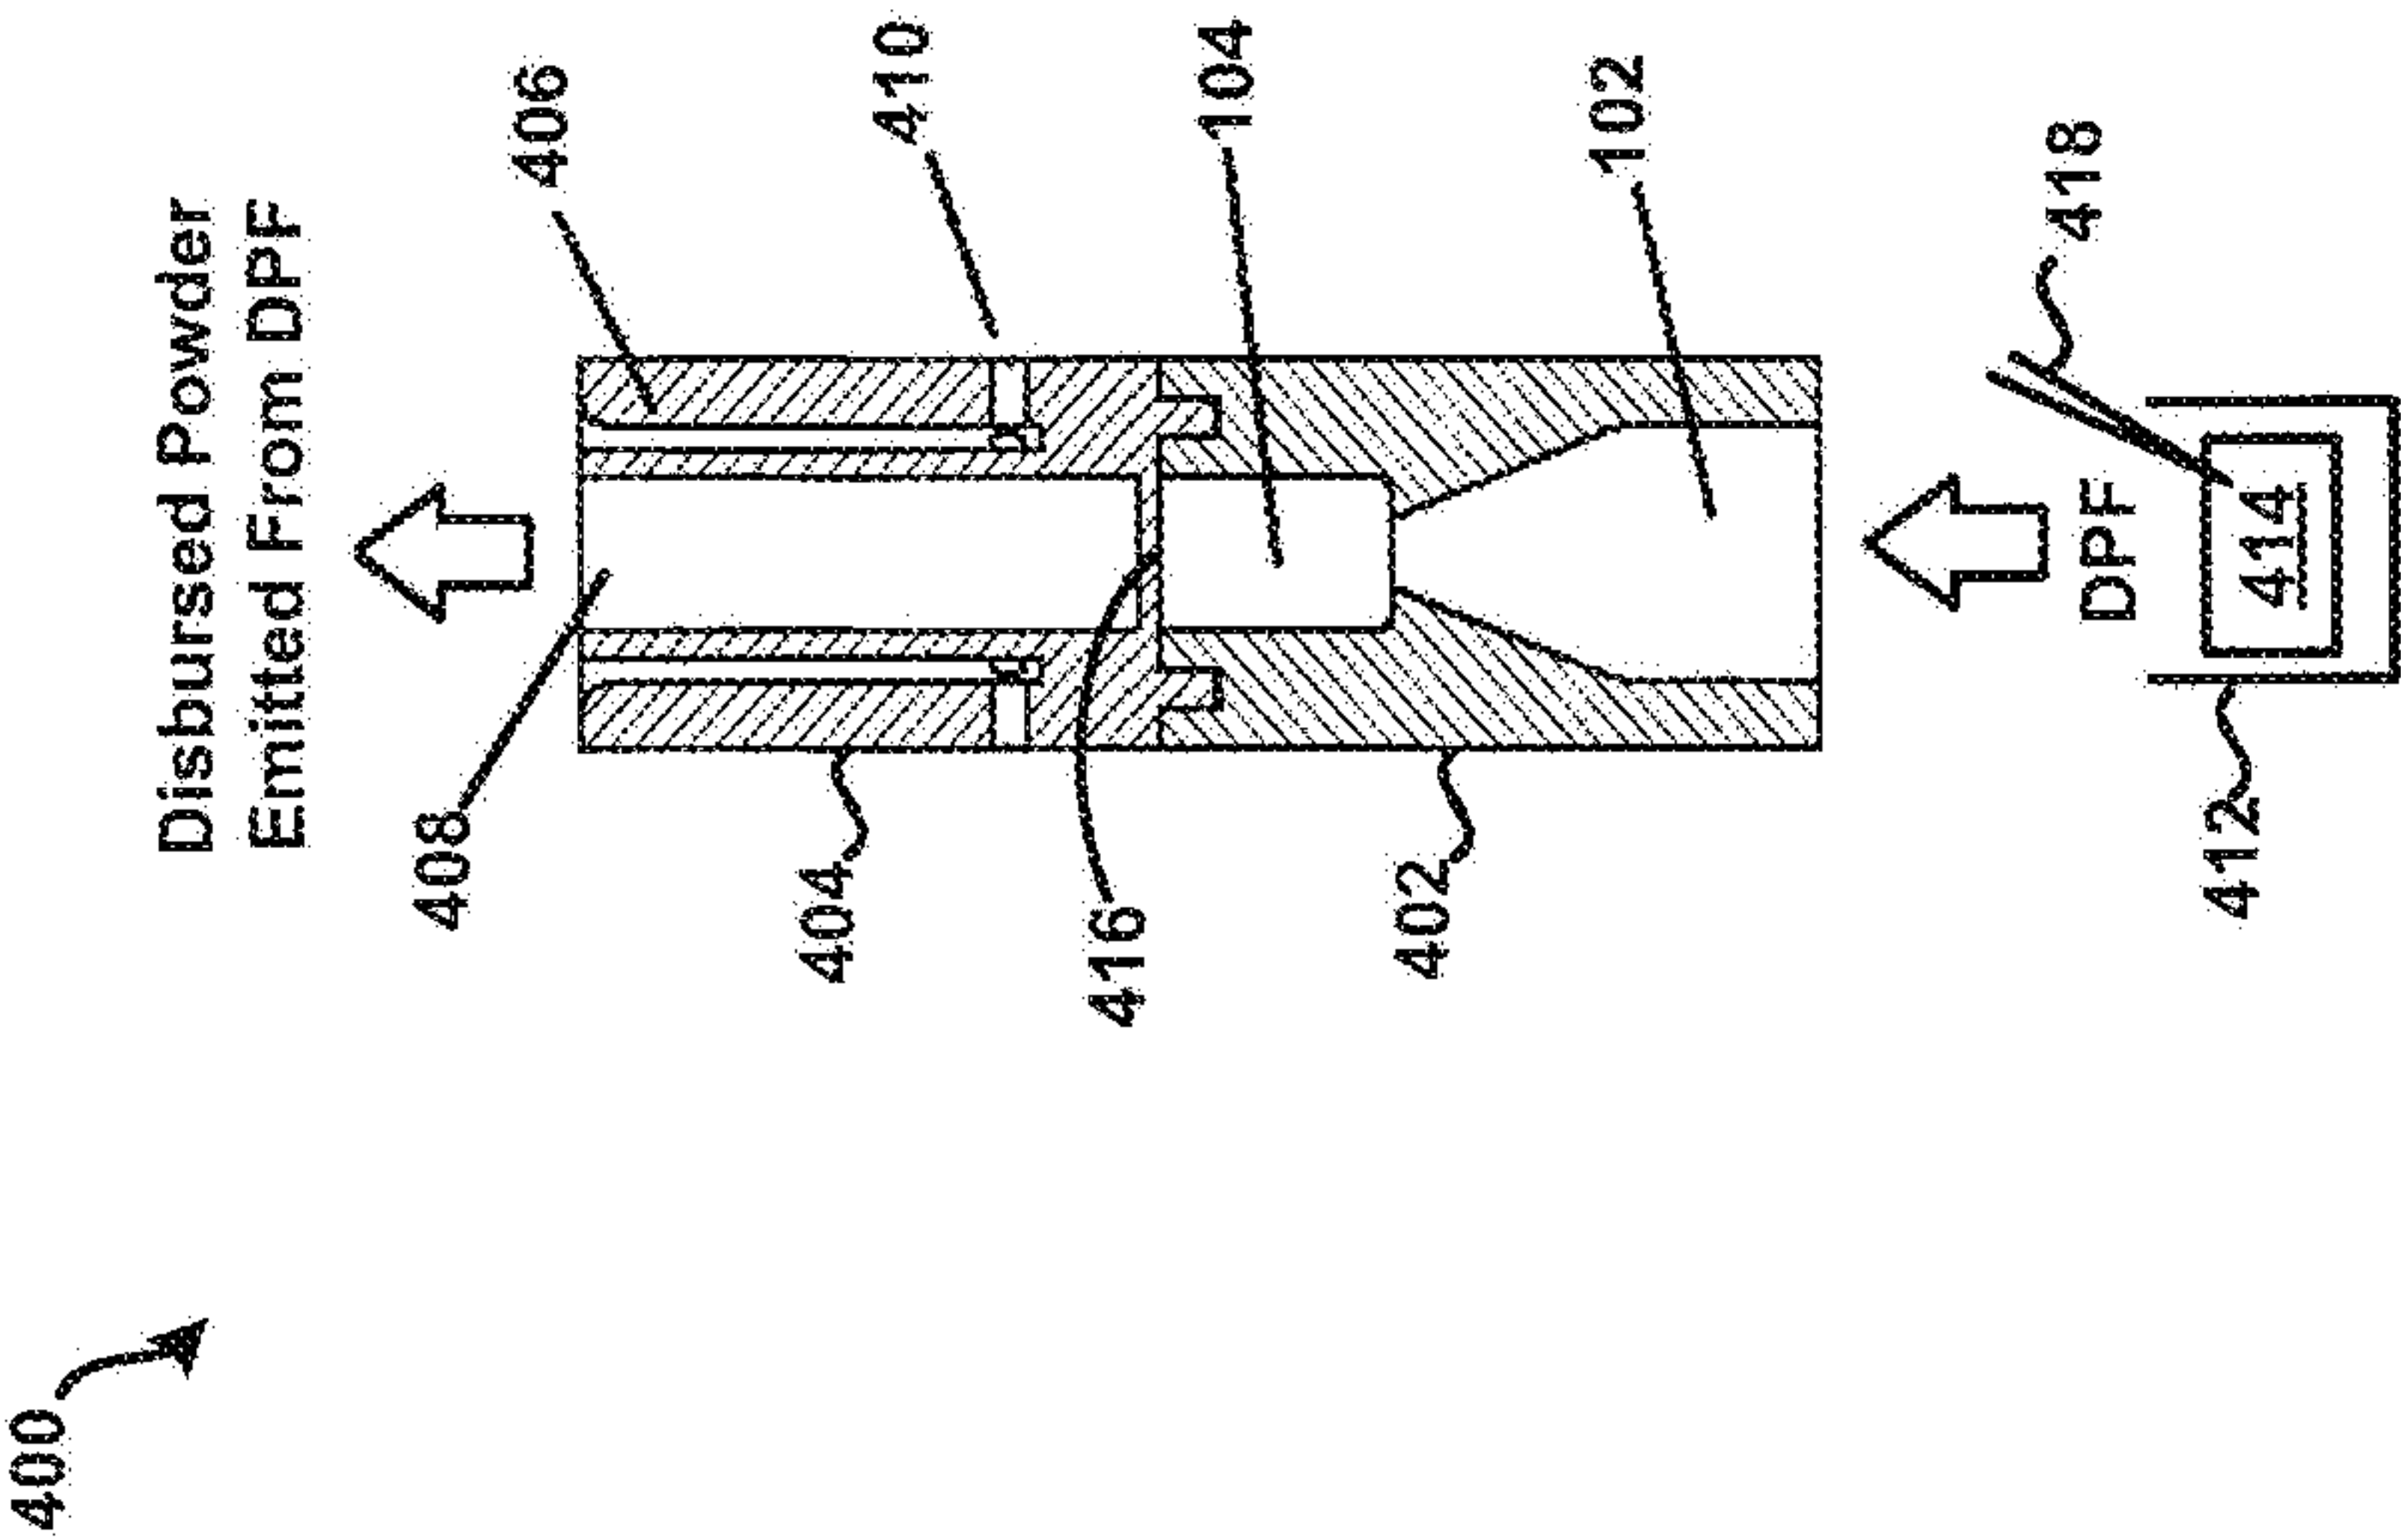


FIG. 4


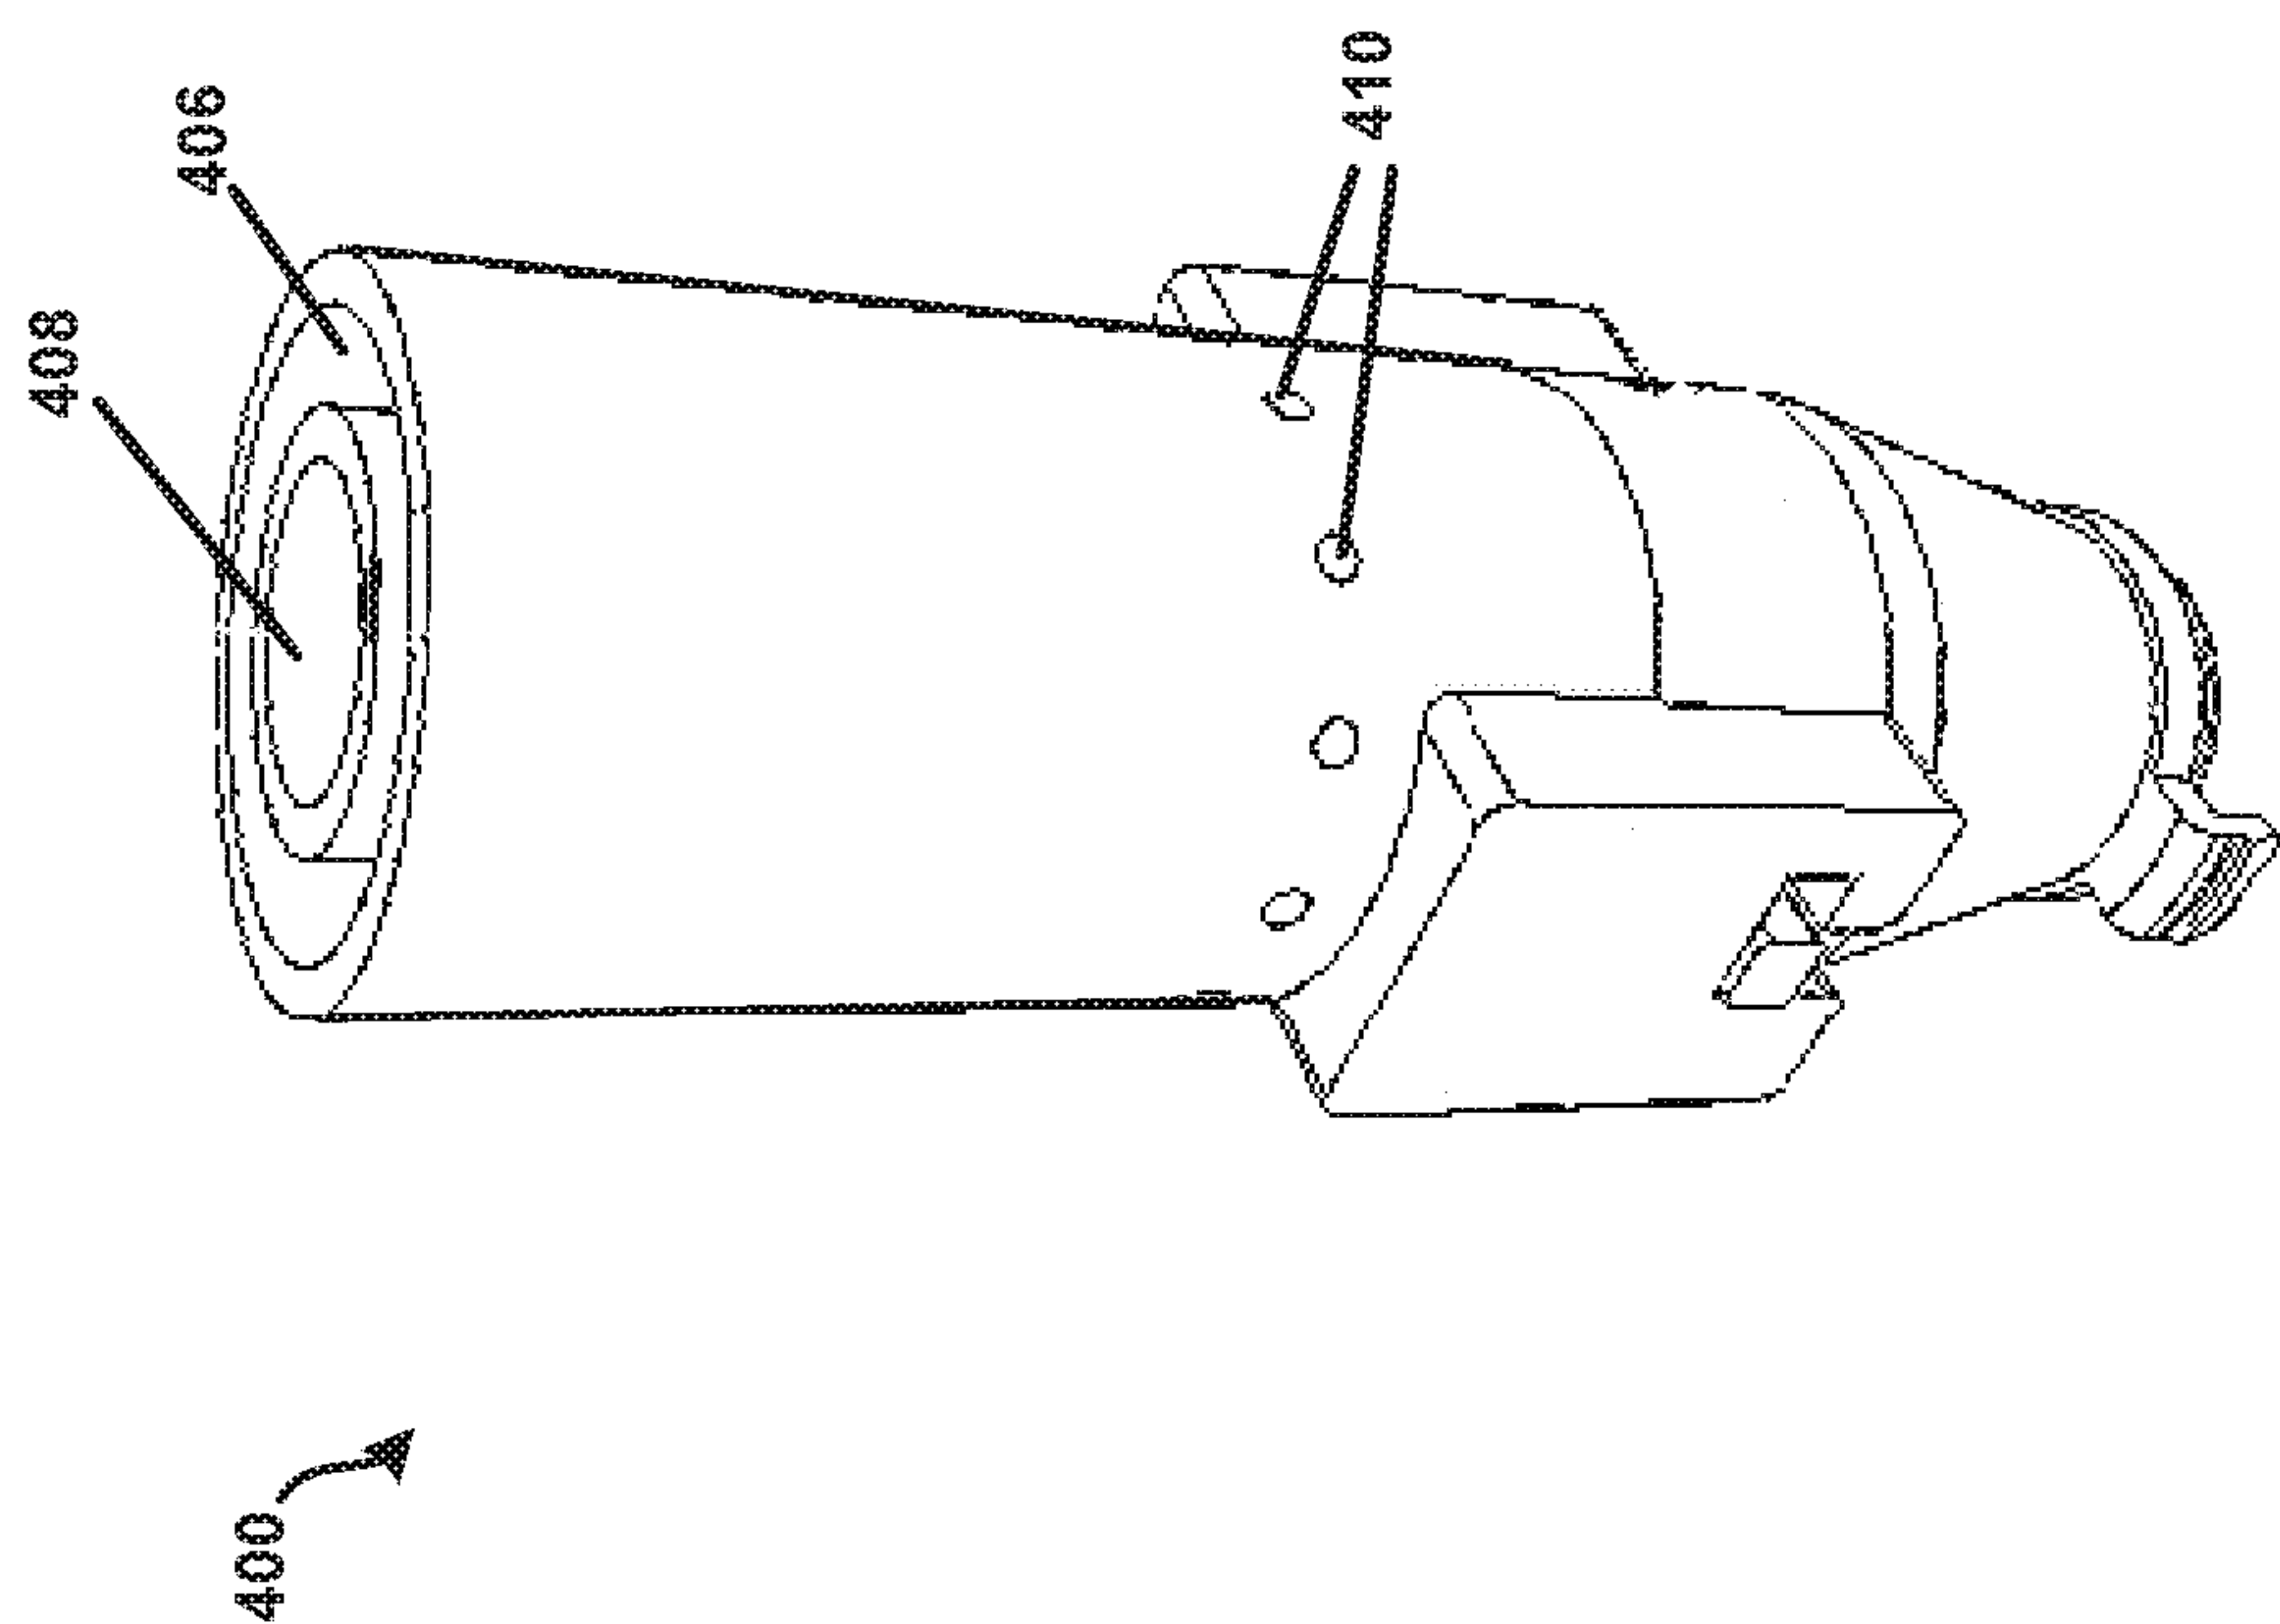


FIG. 5

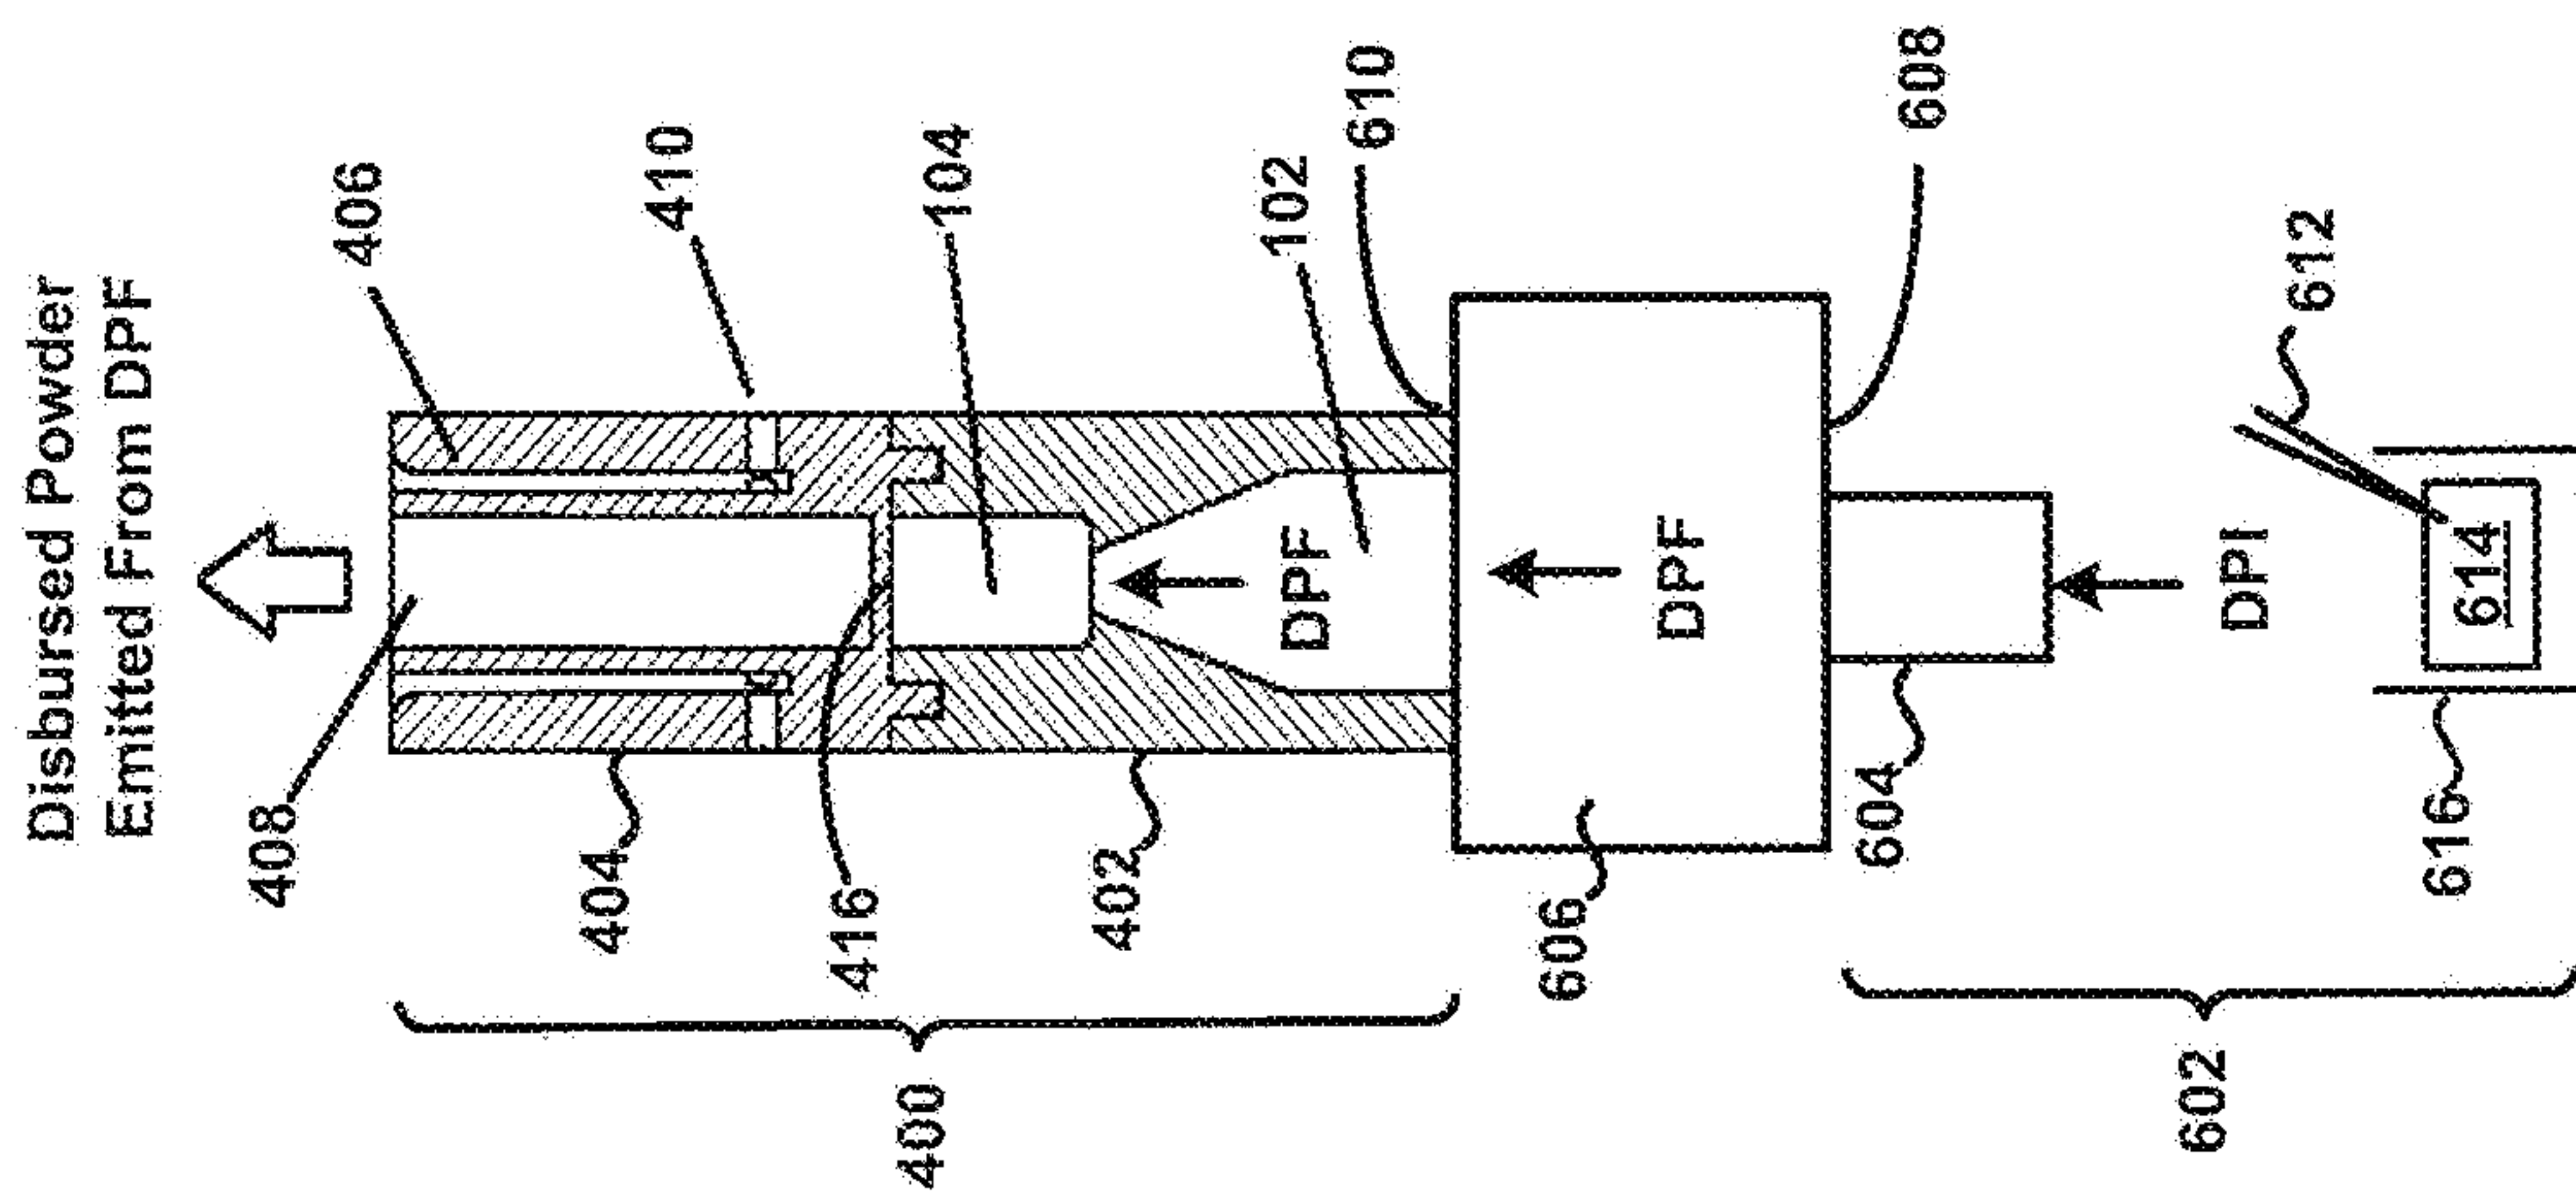

6
G
—
L

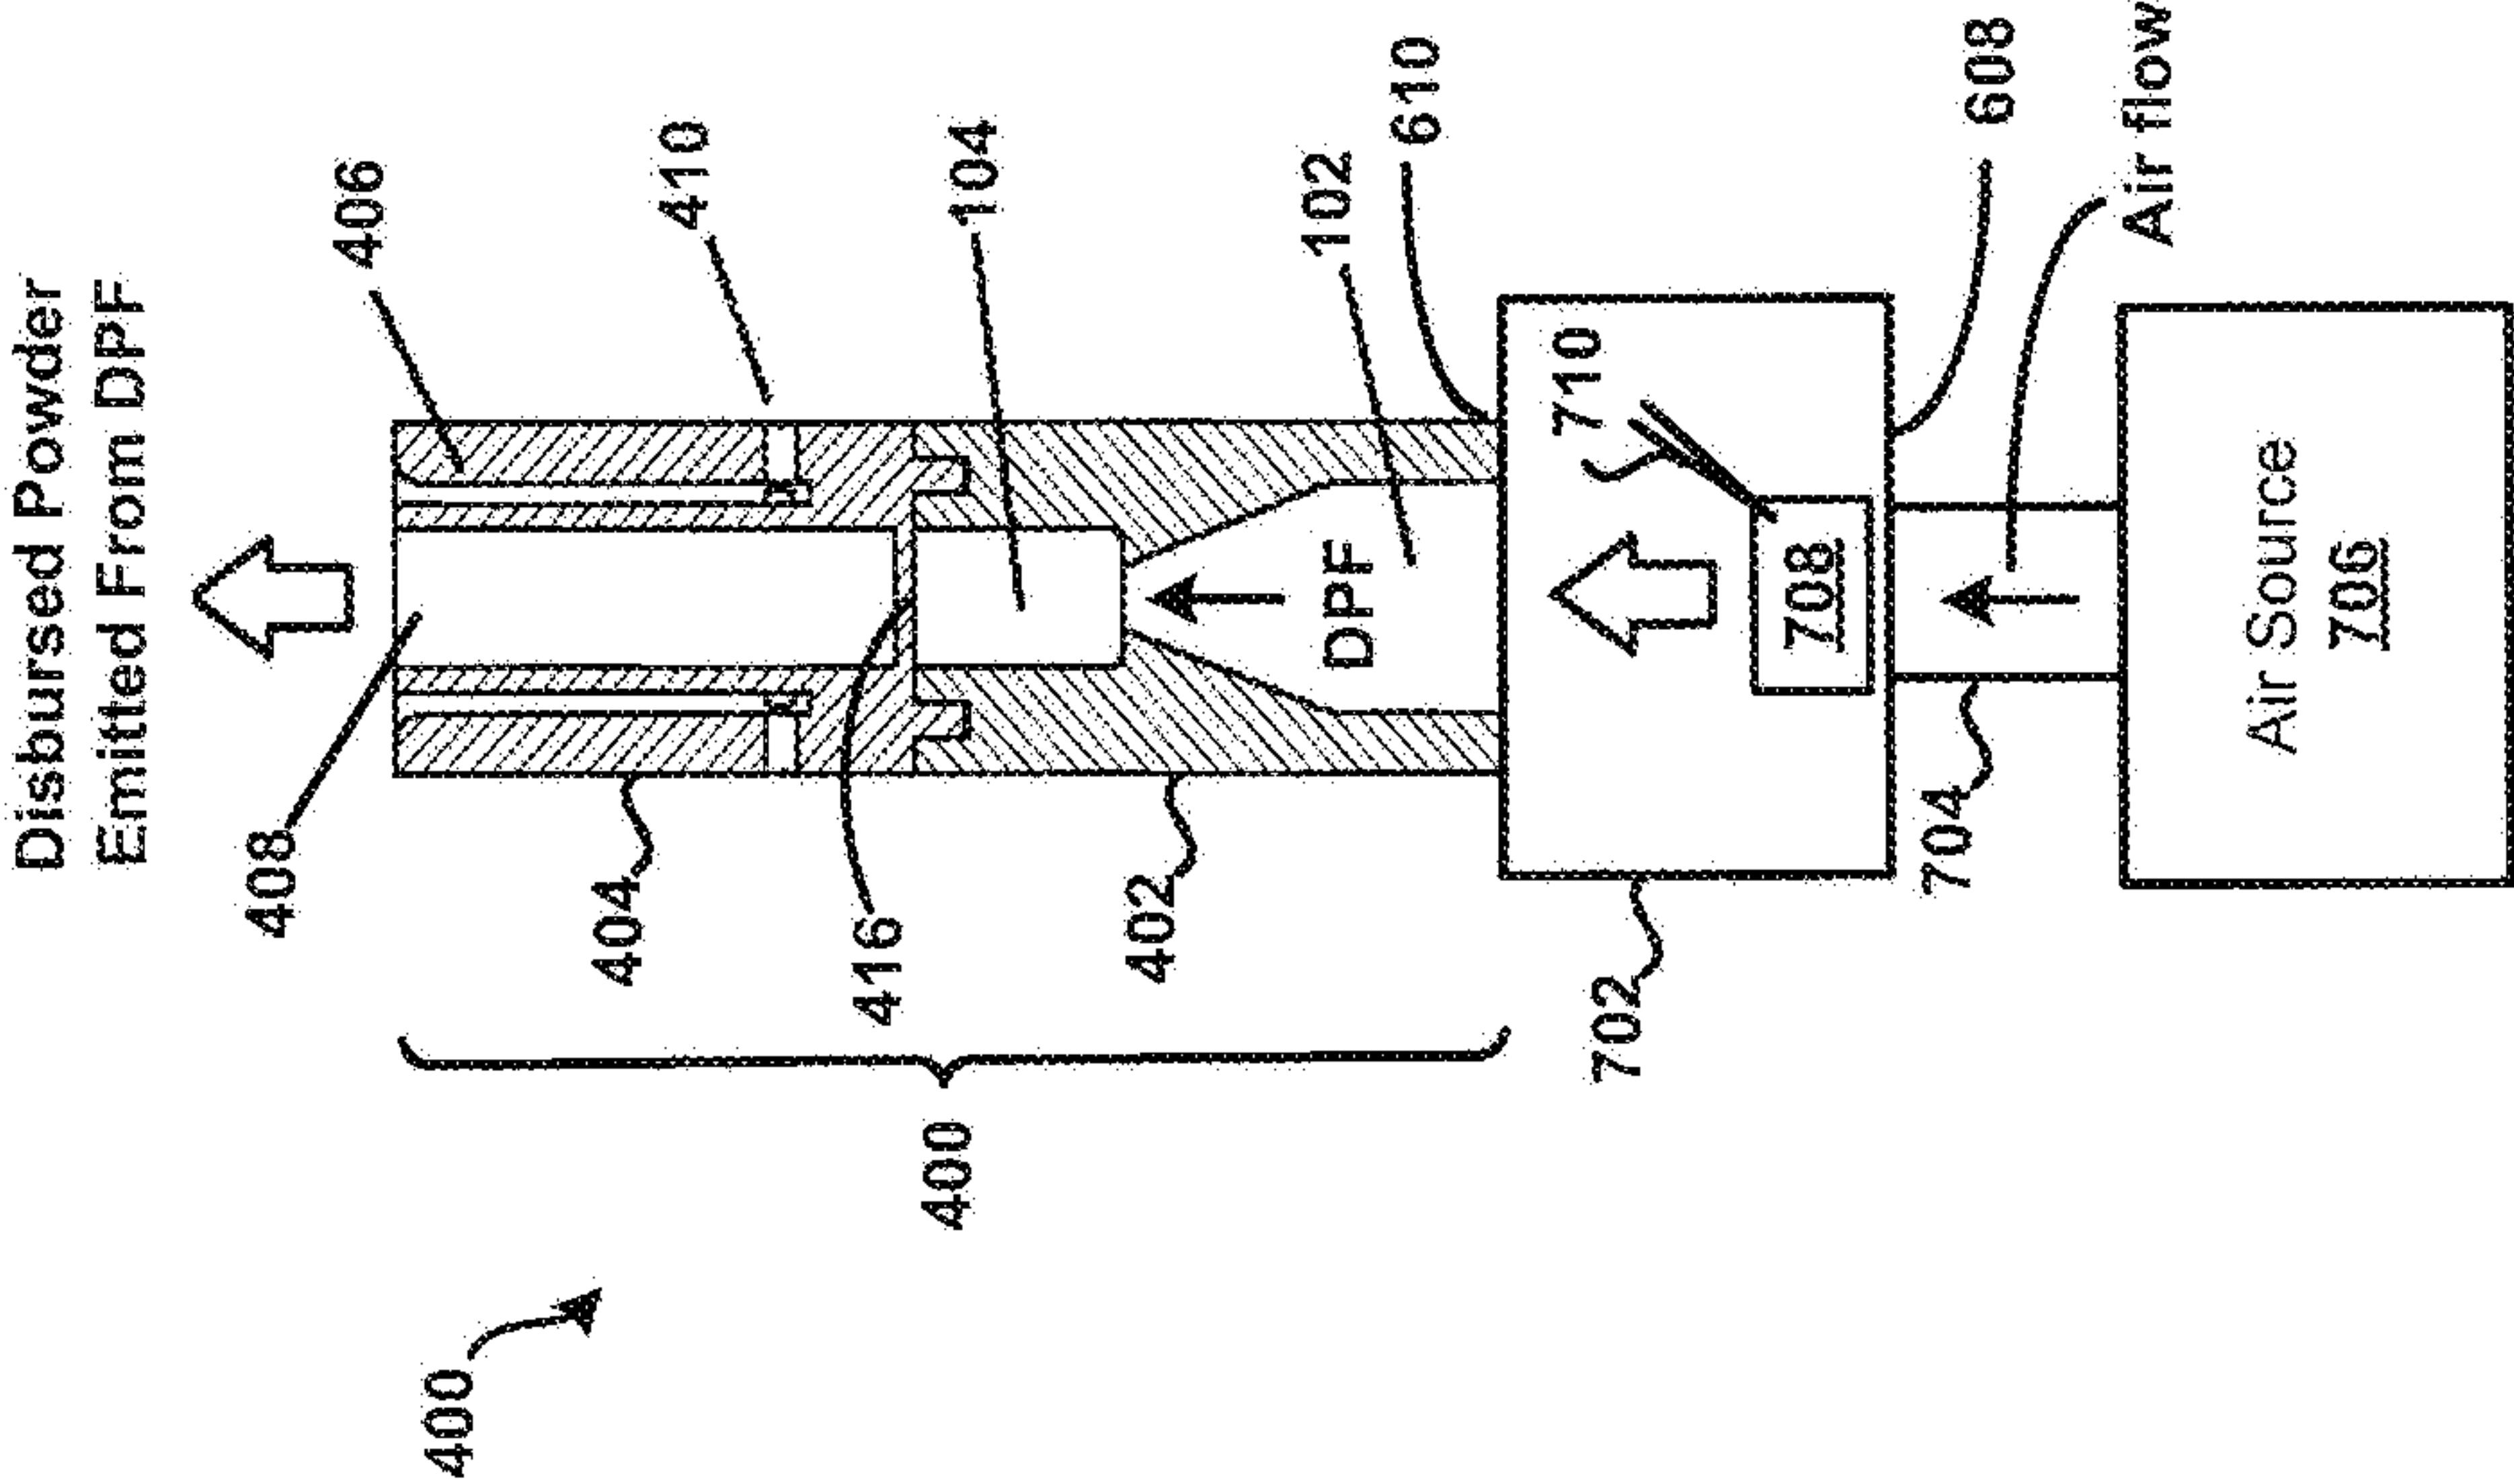


FIG. 7

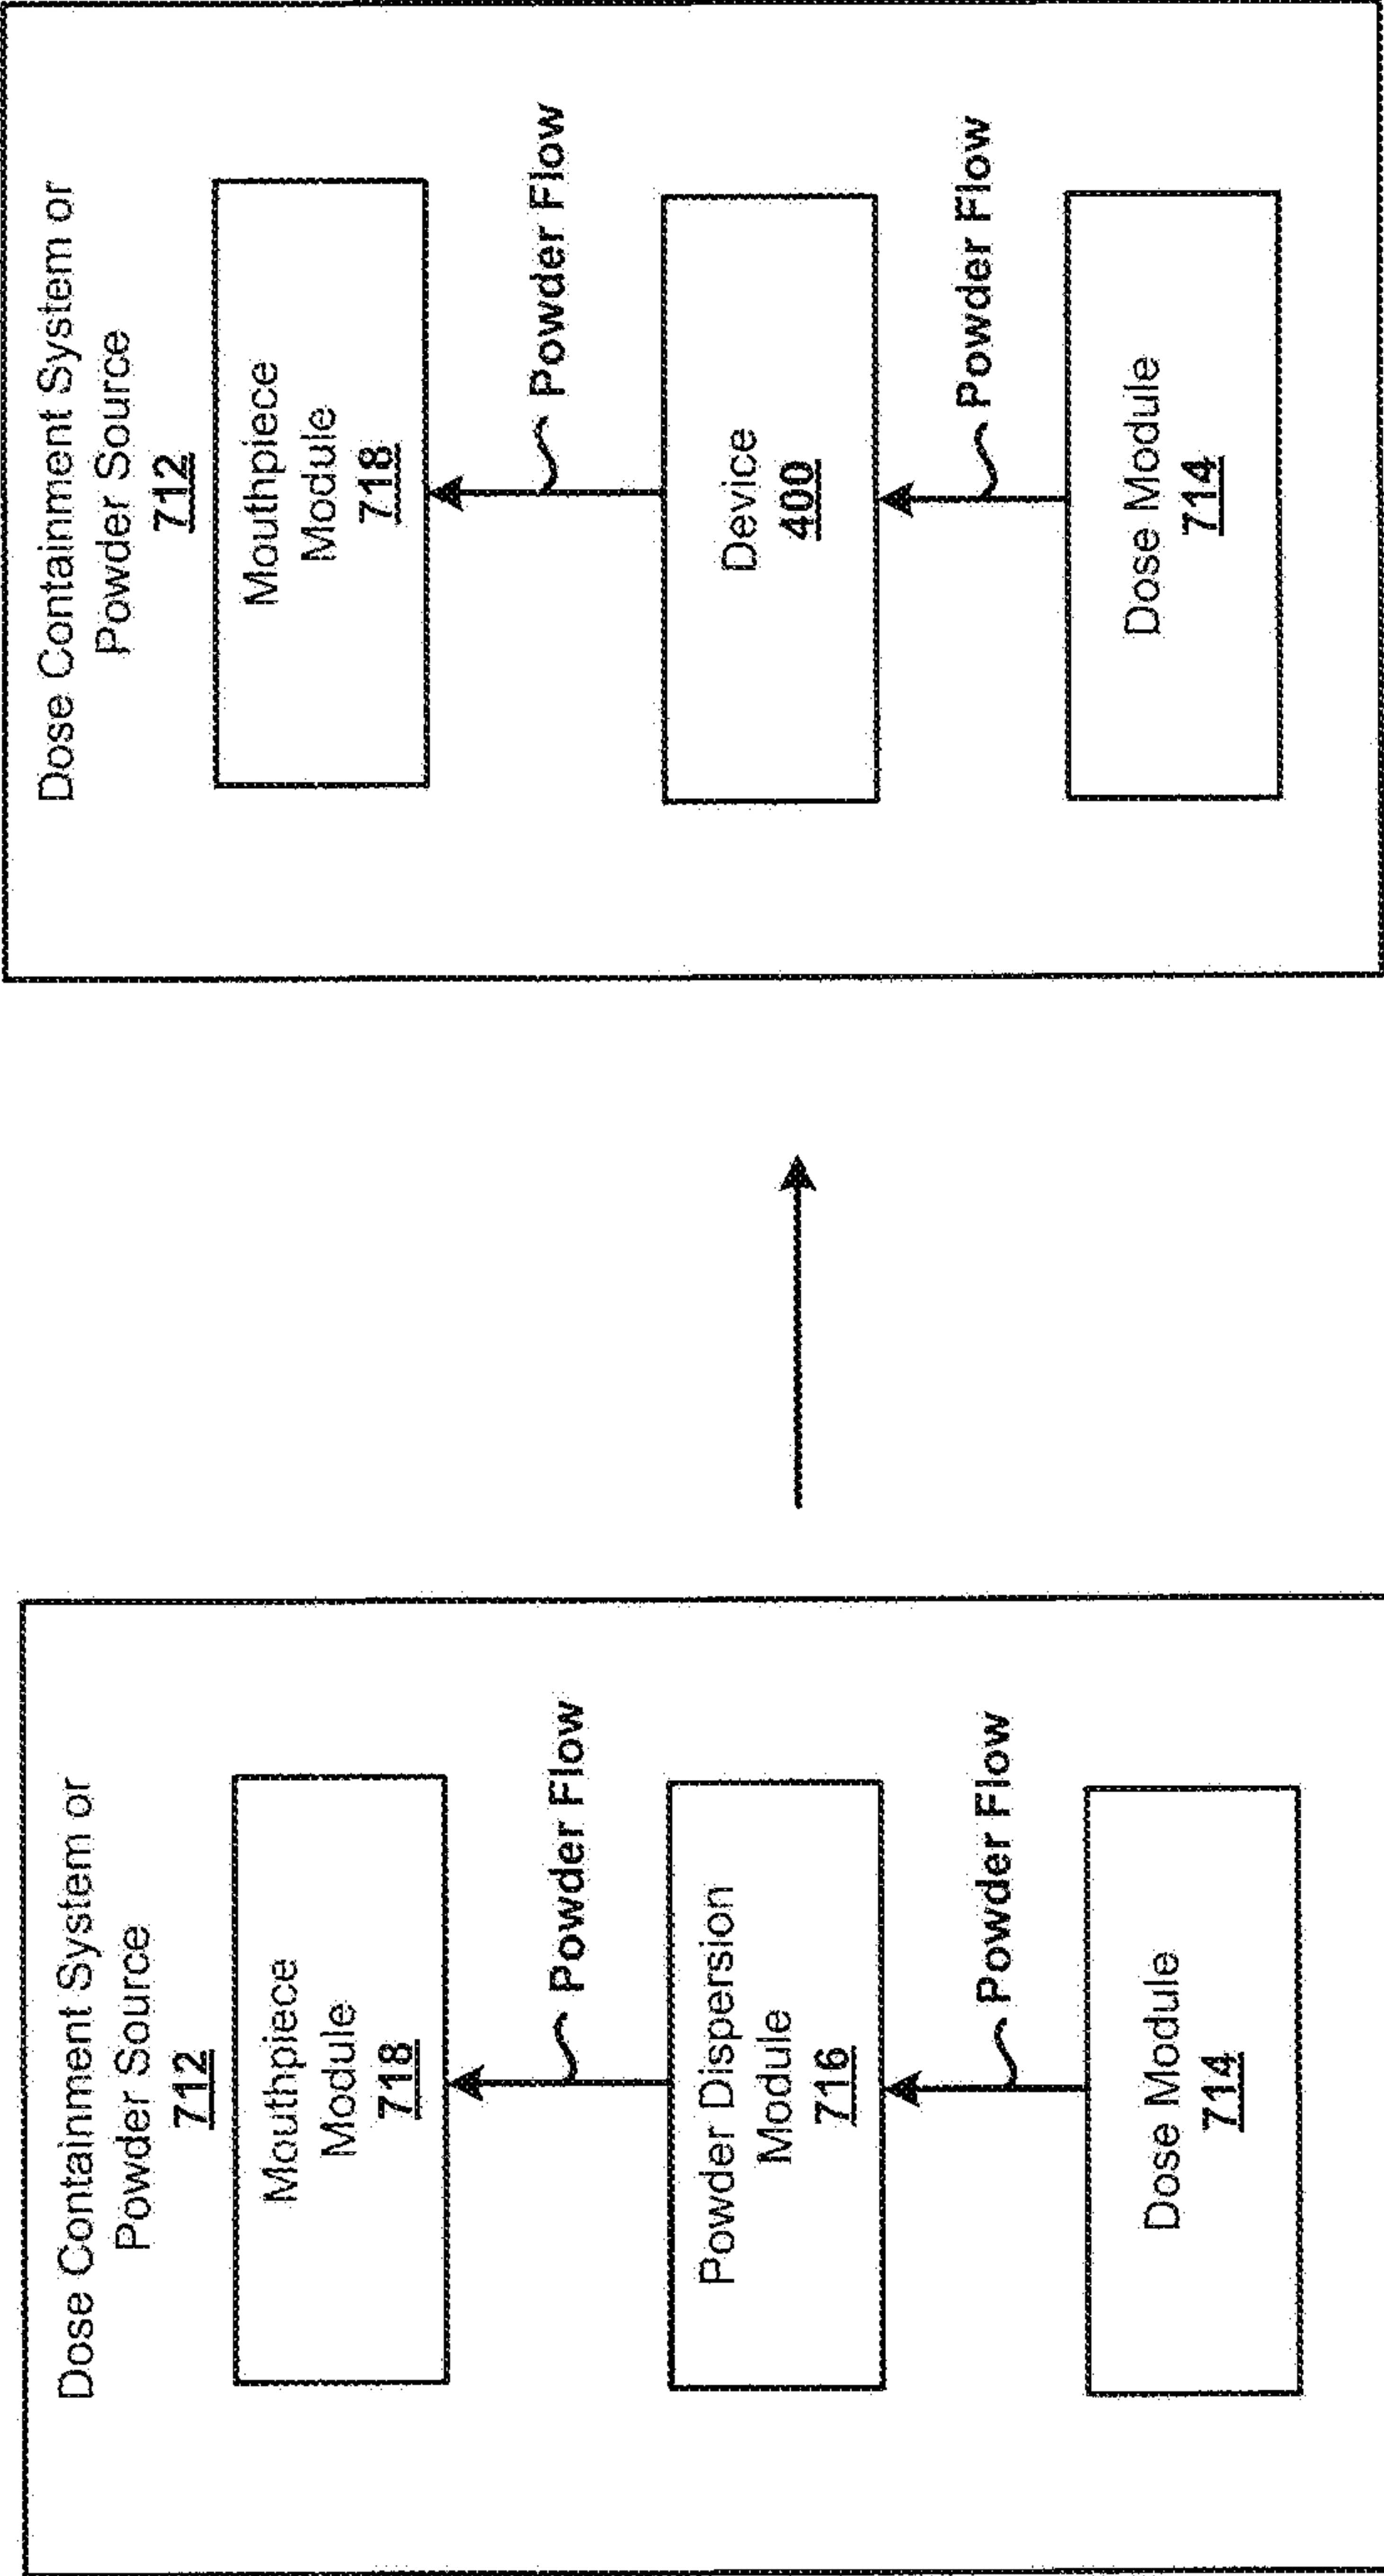


FIG. 8

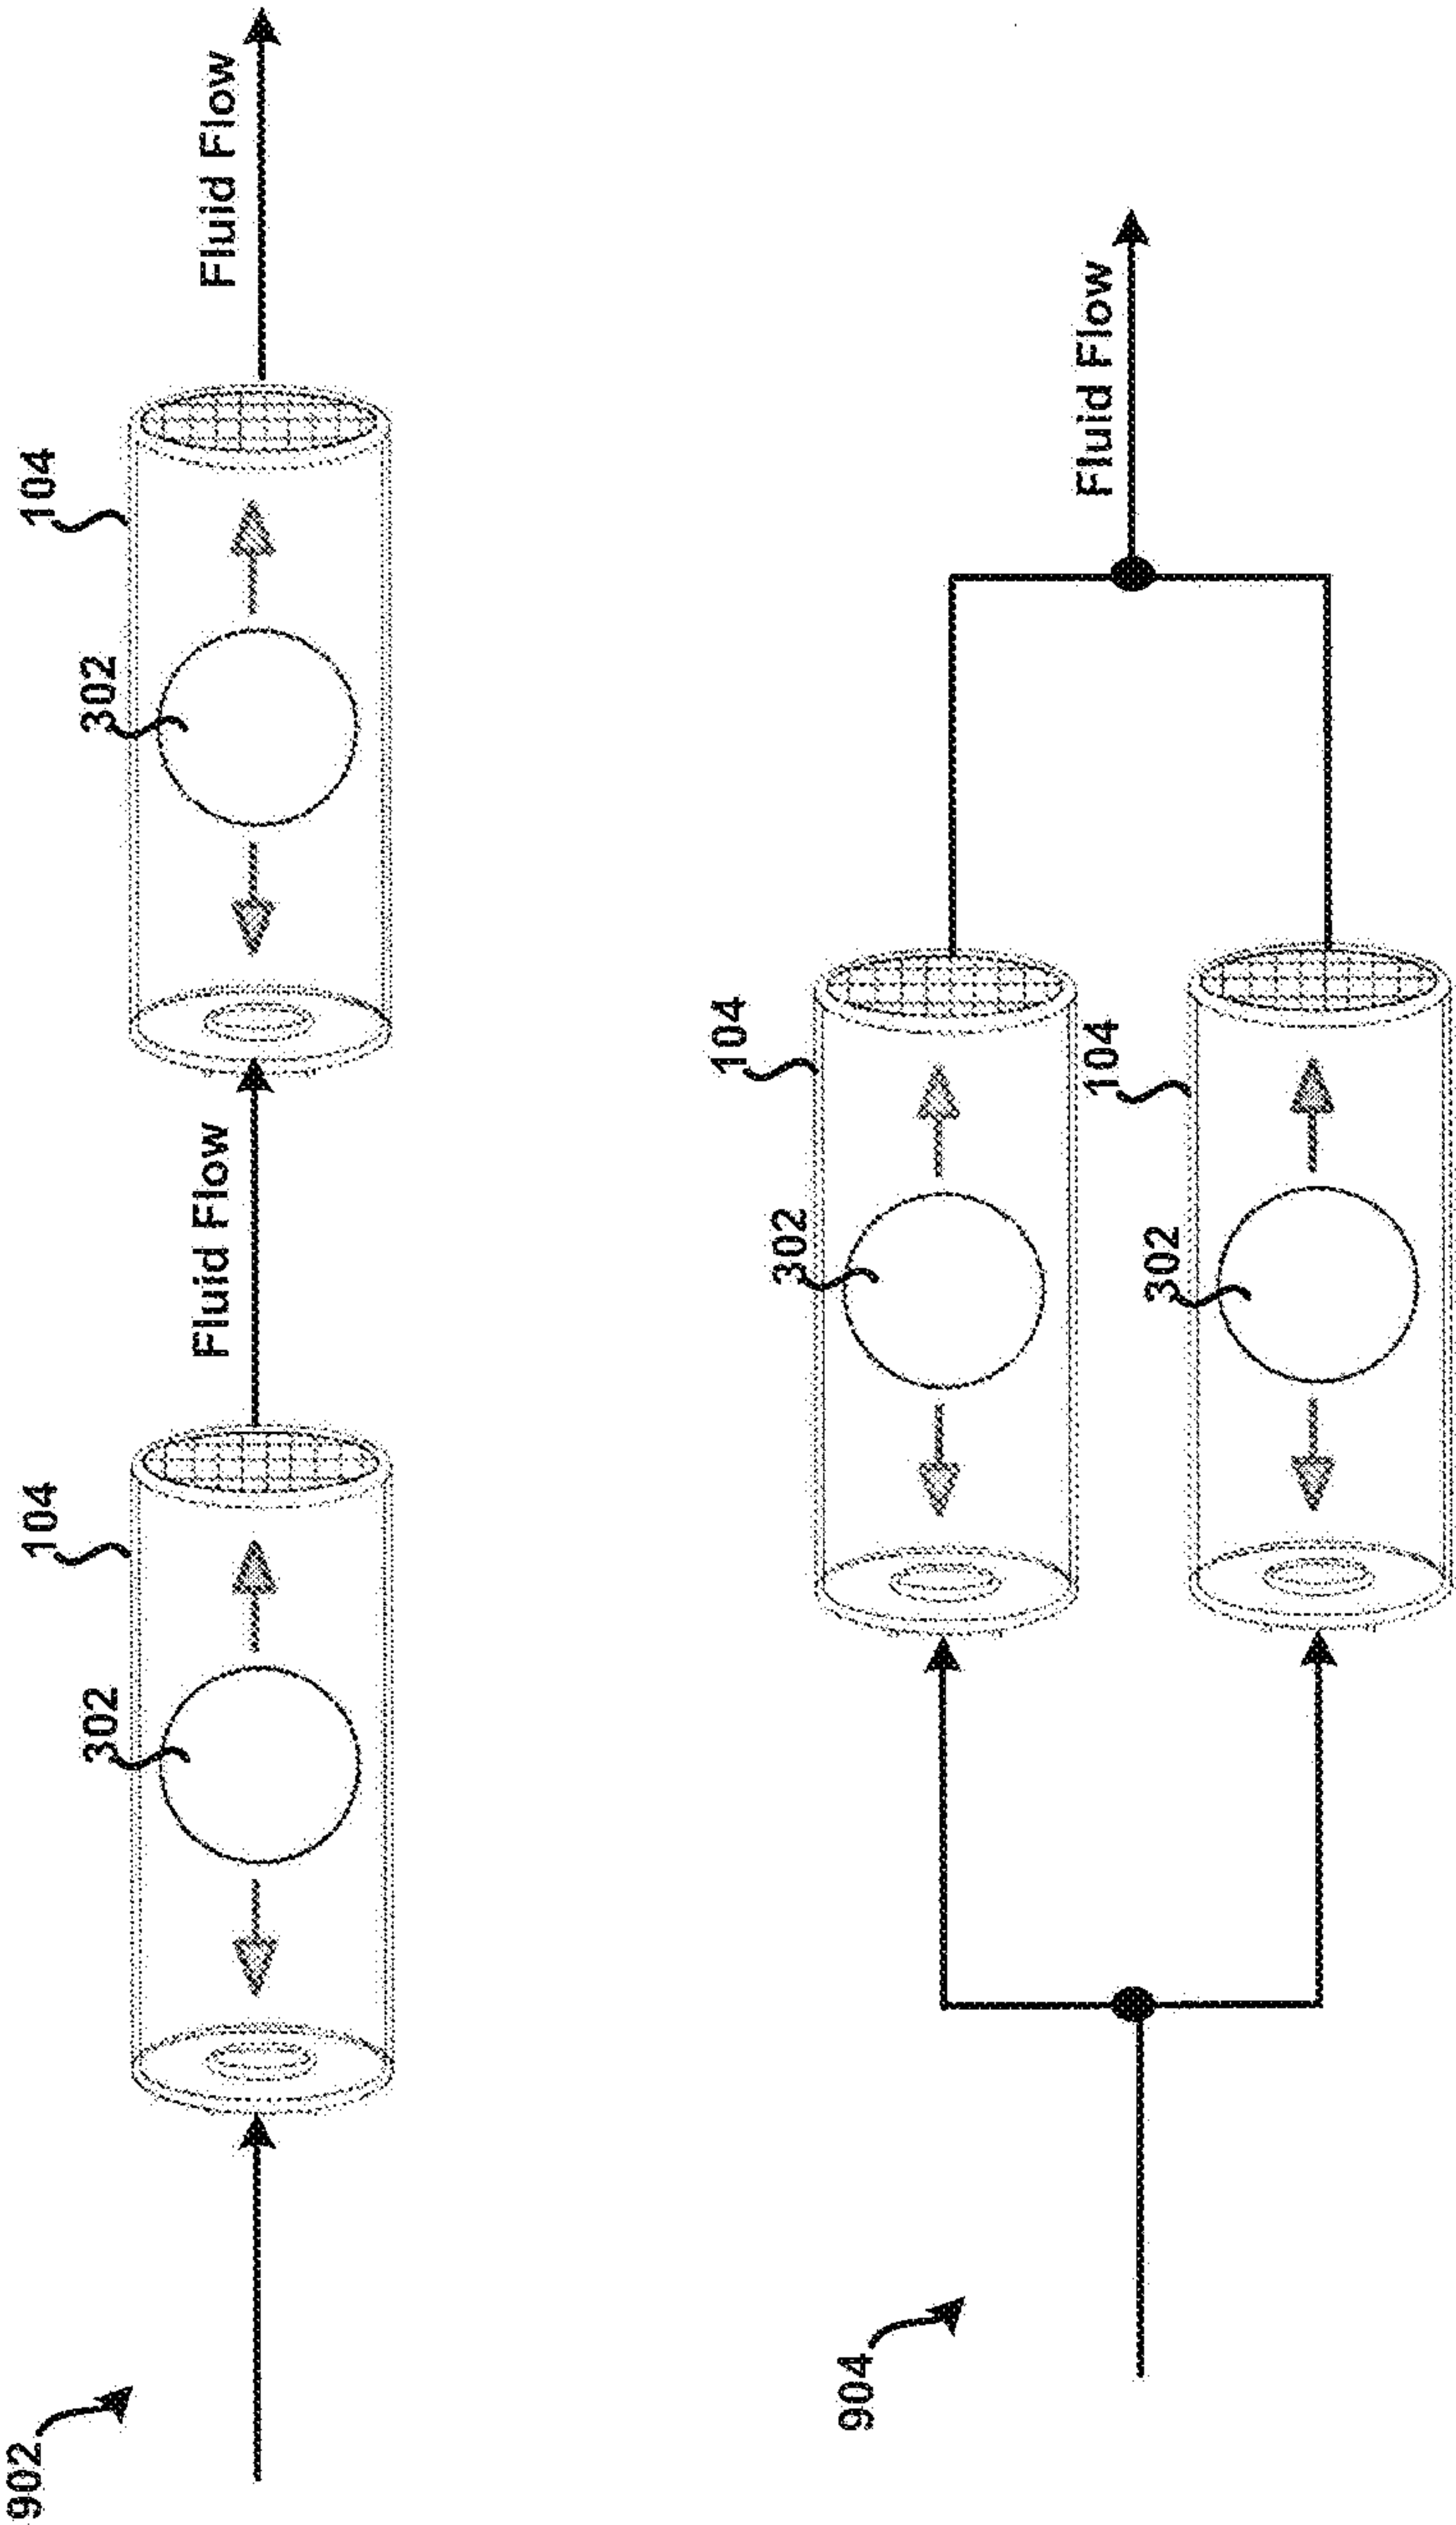


FIG. 9

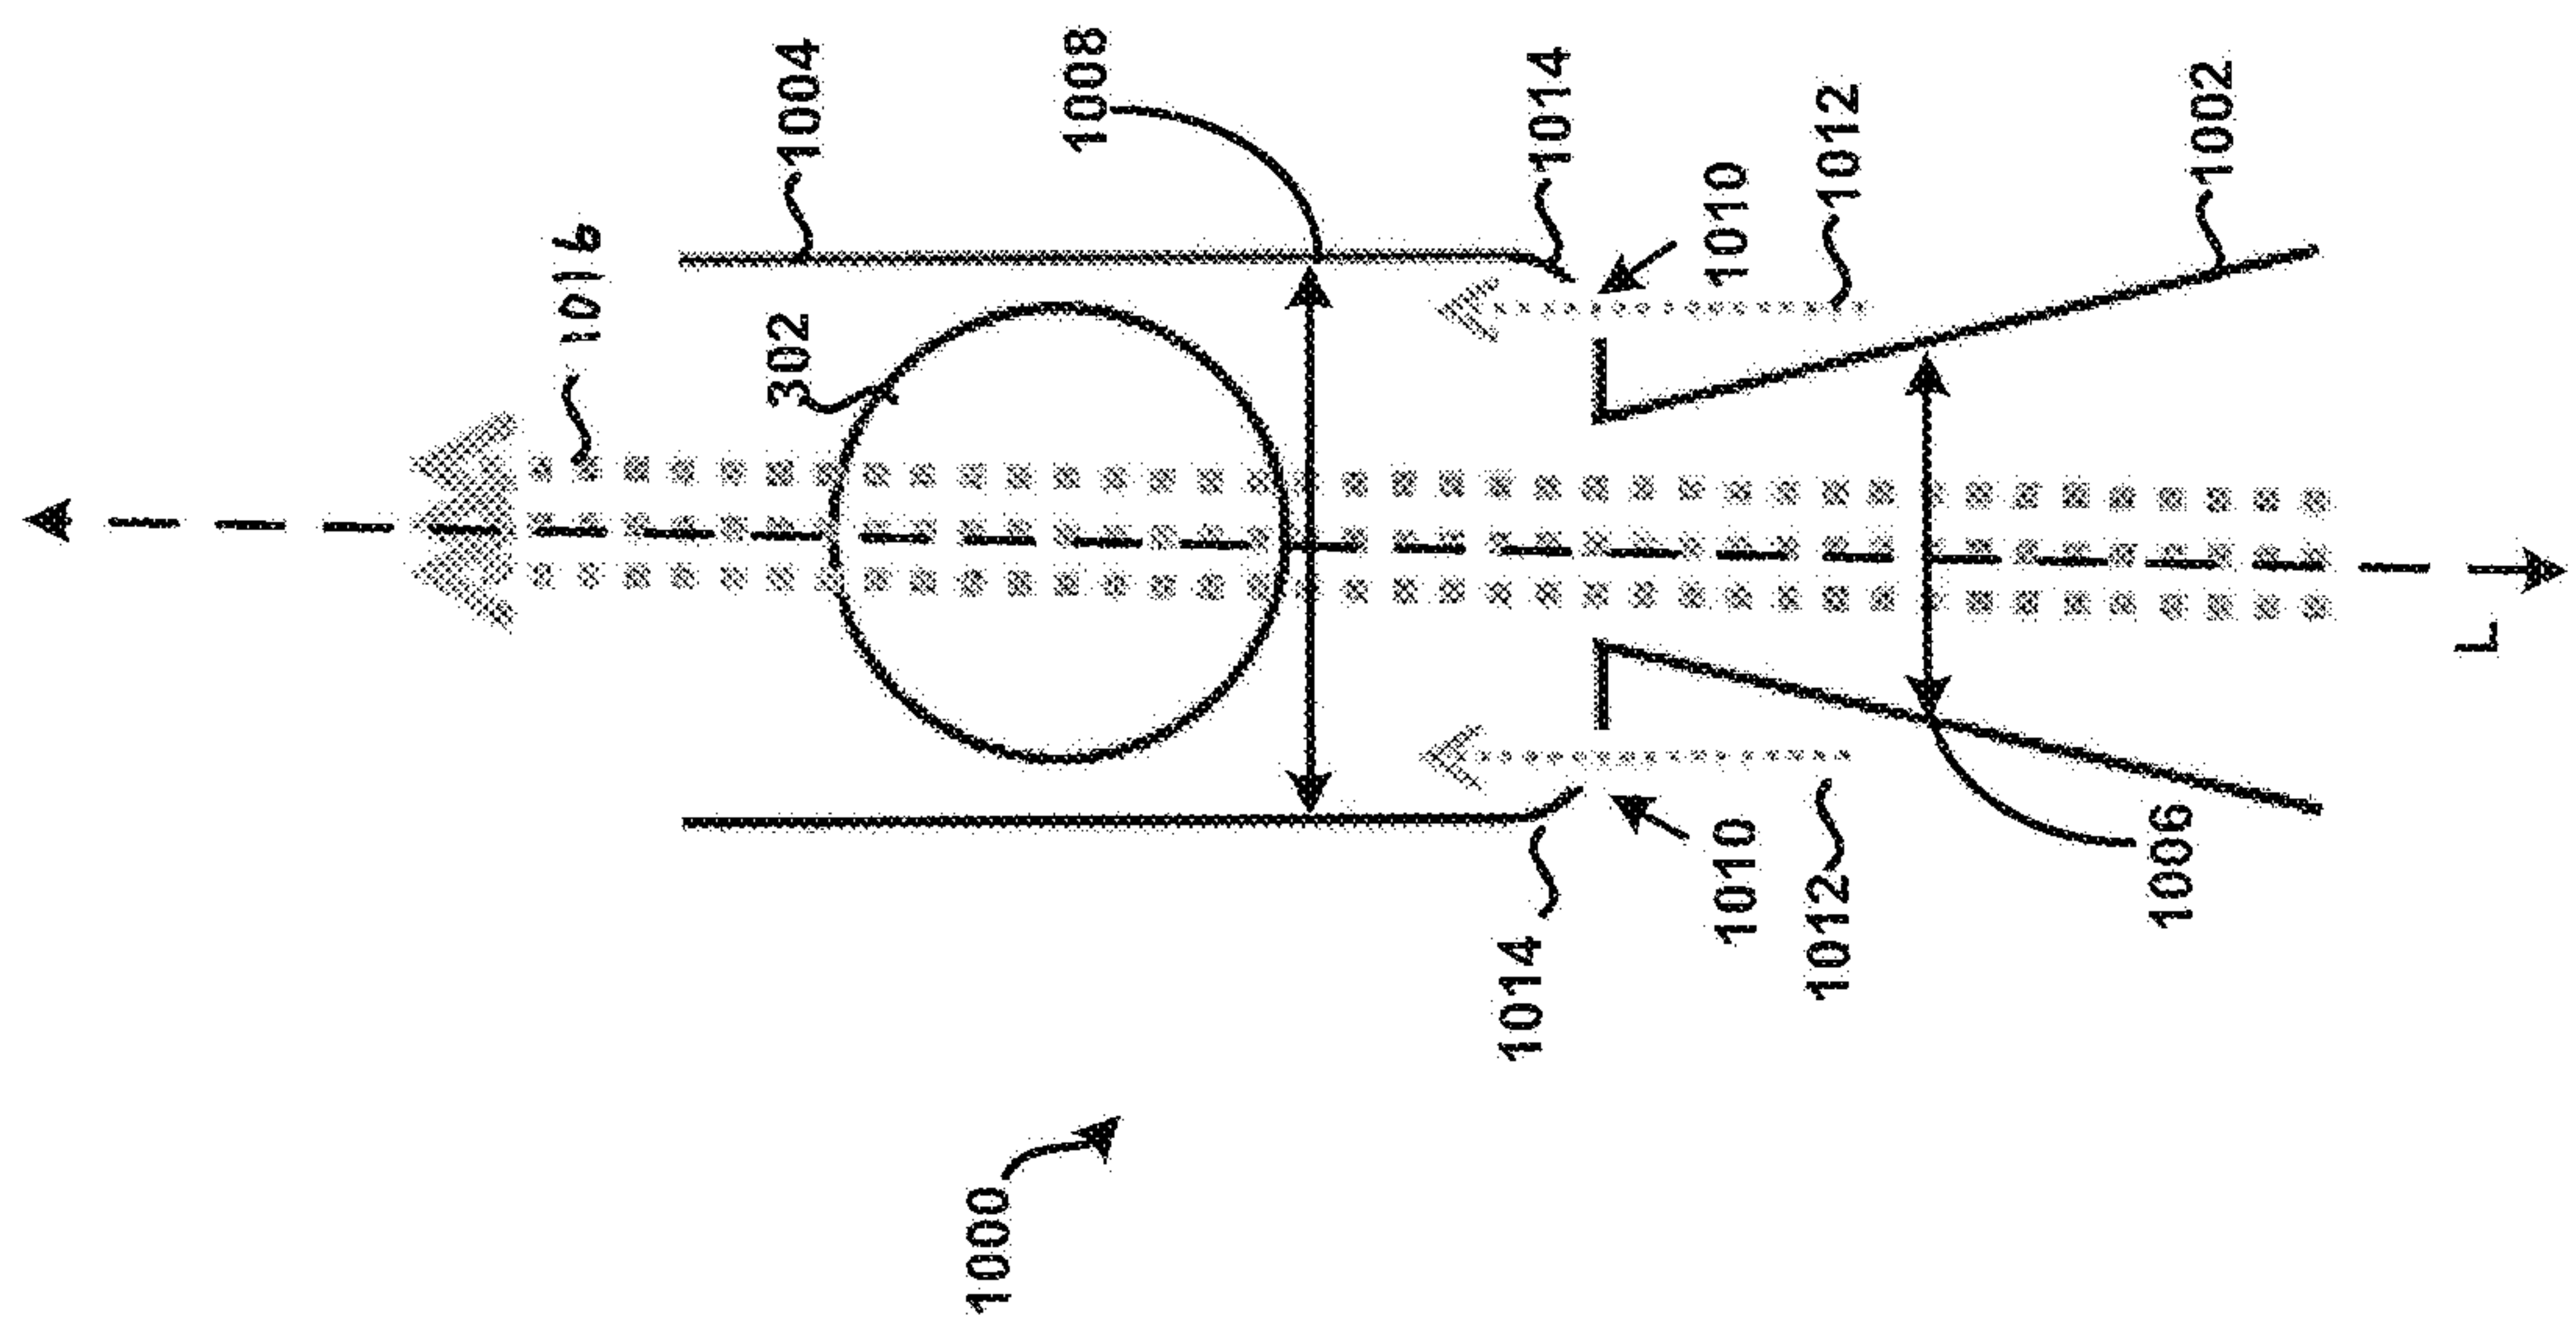


FIG. 10

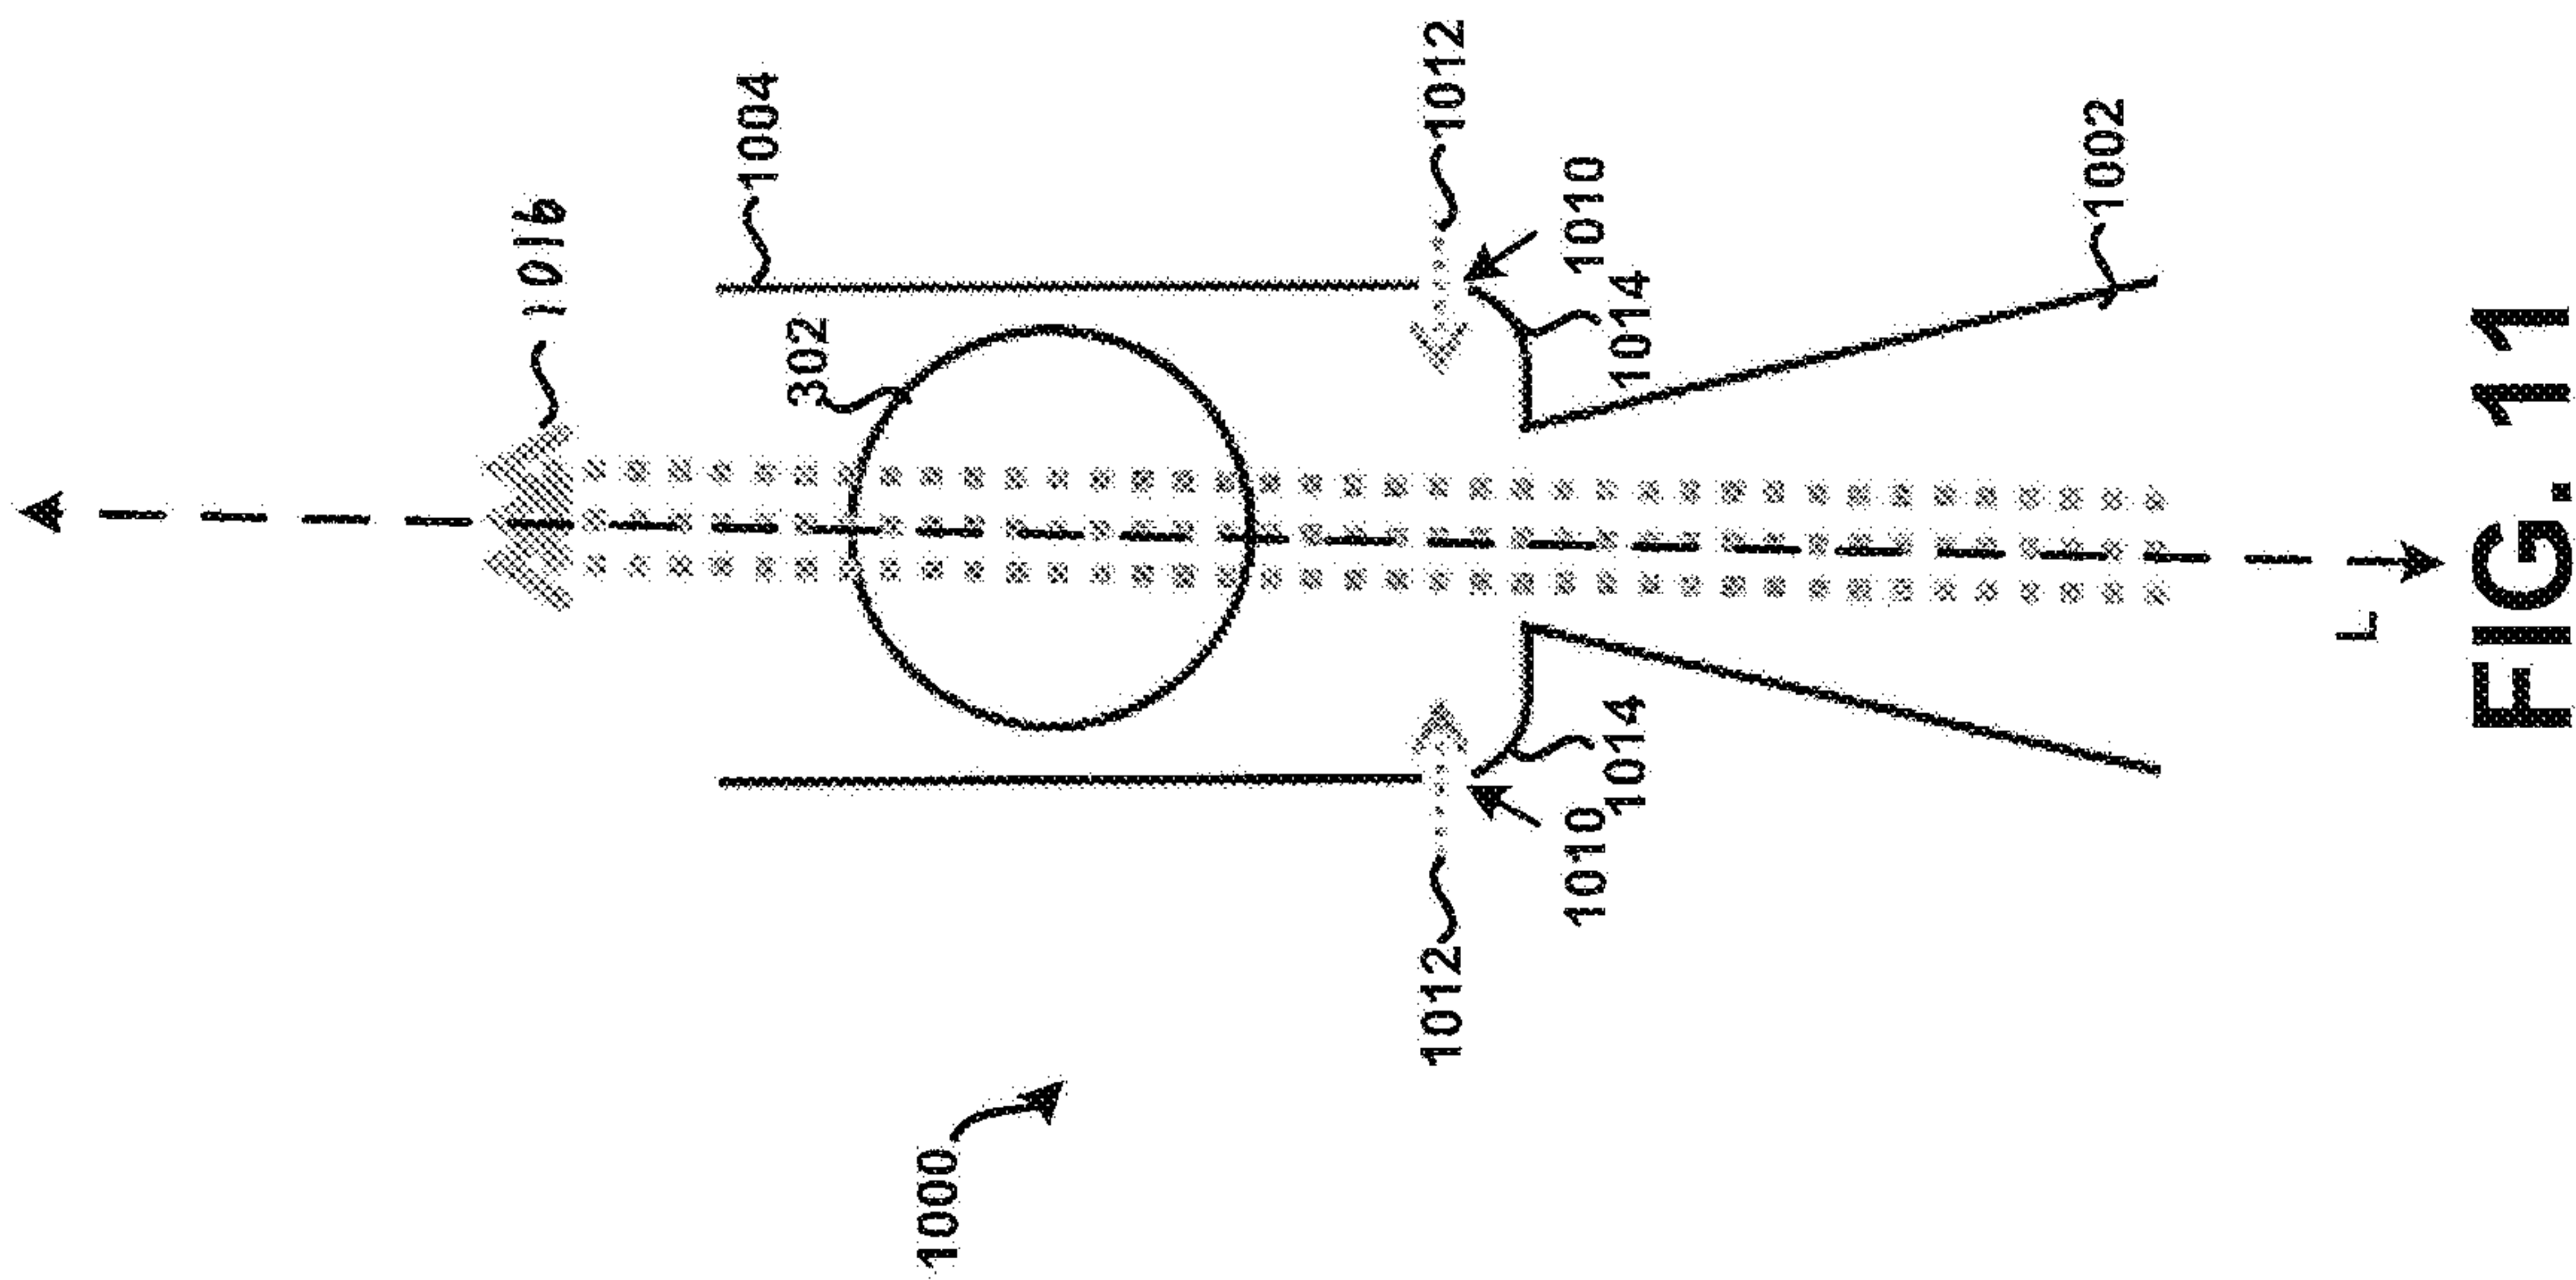


FIG. 11

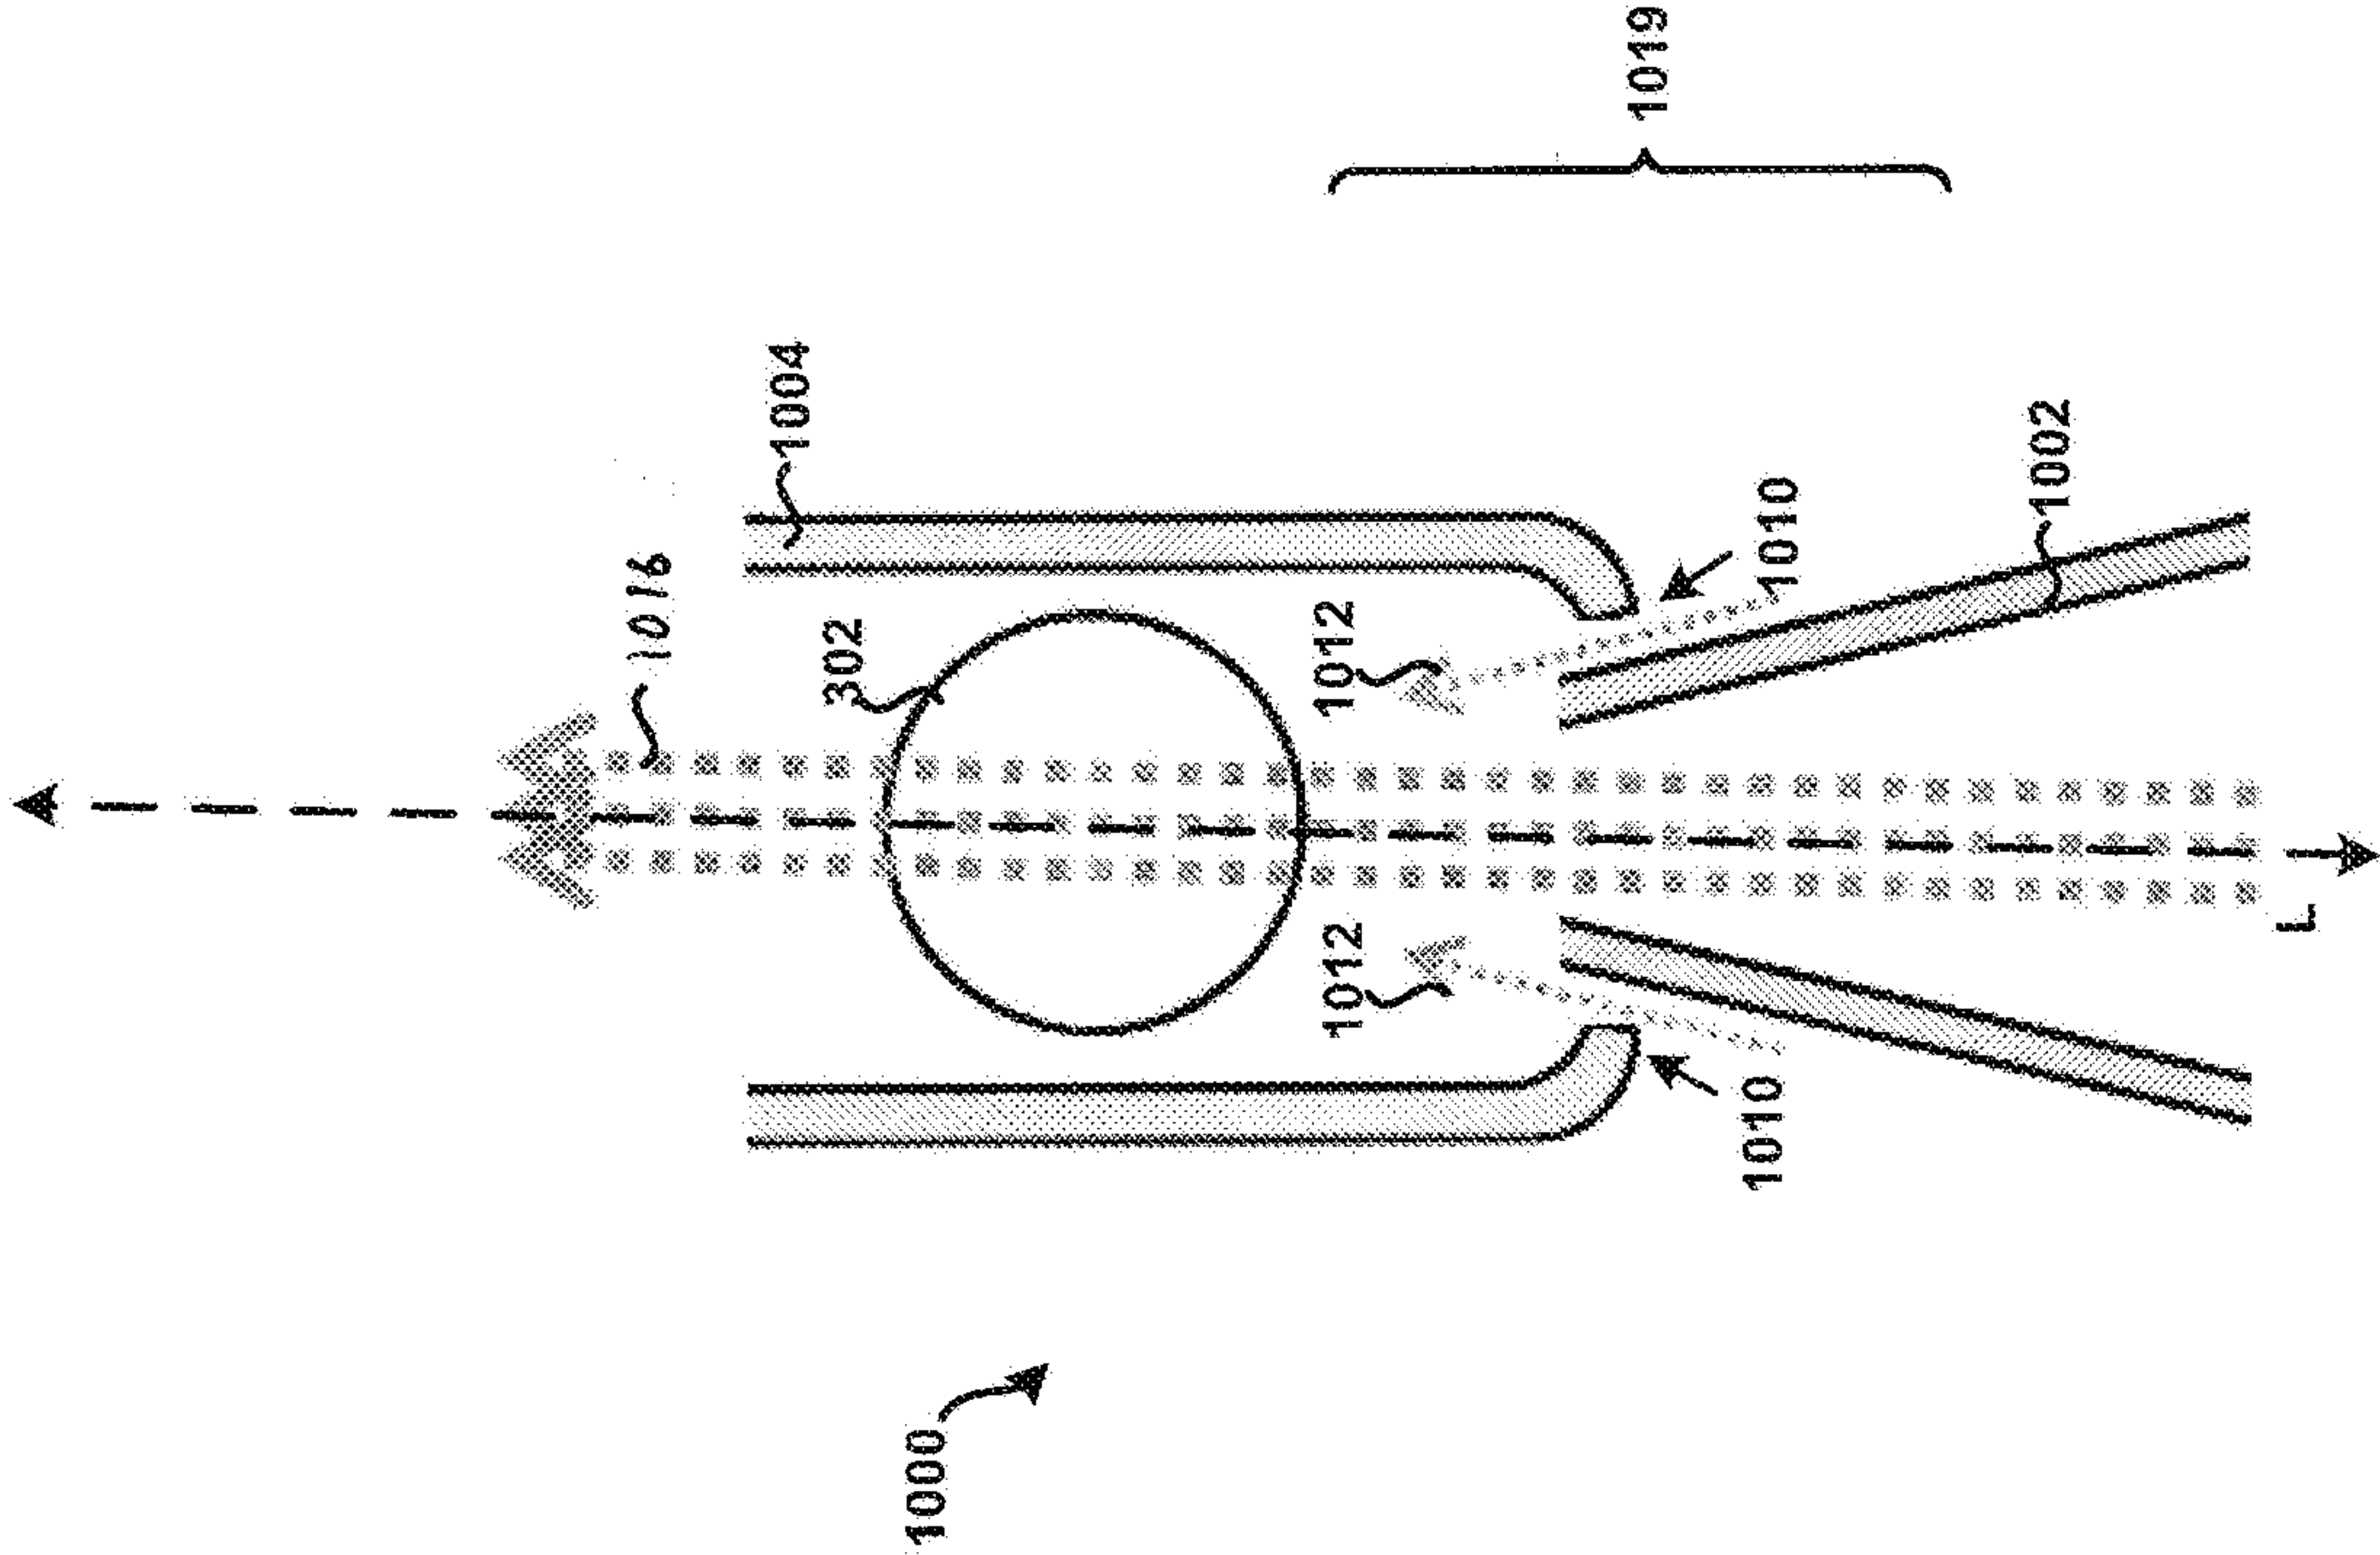


FIG. 12

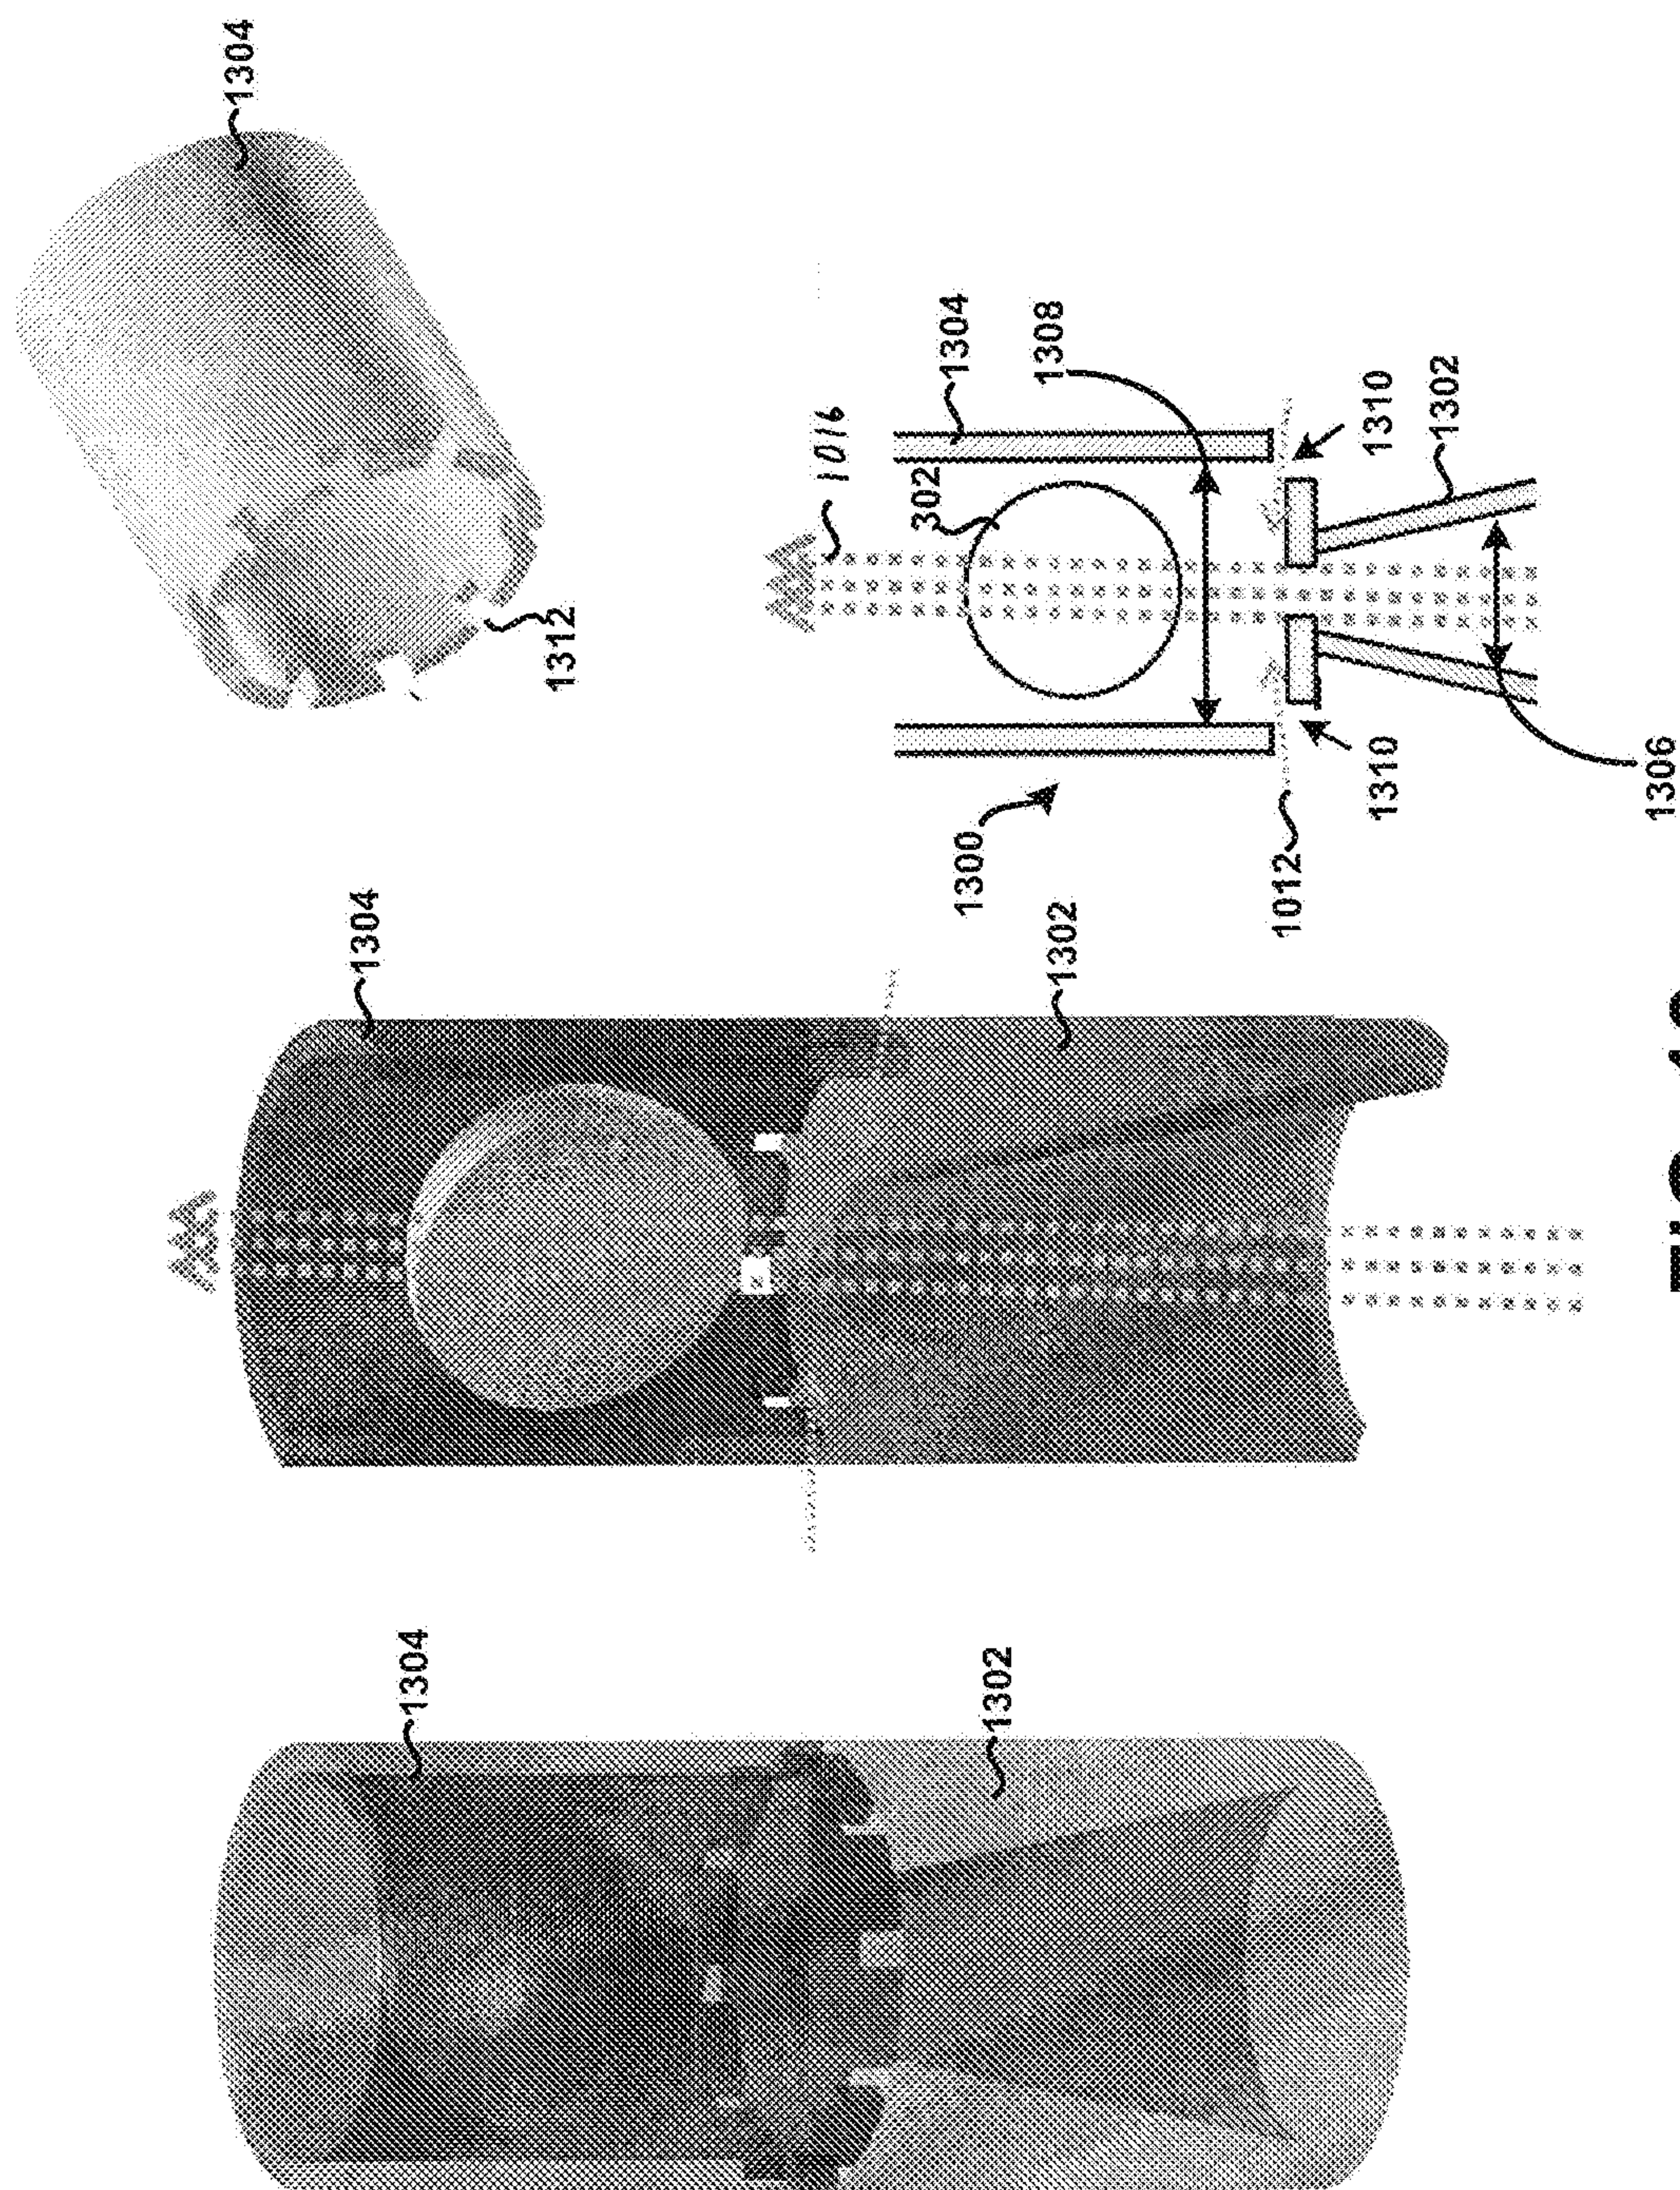


FIG. 13

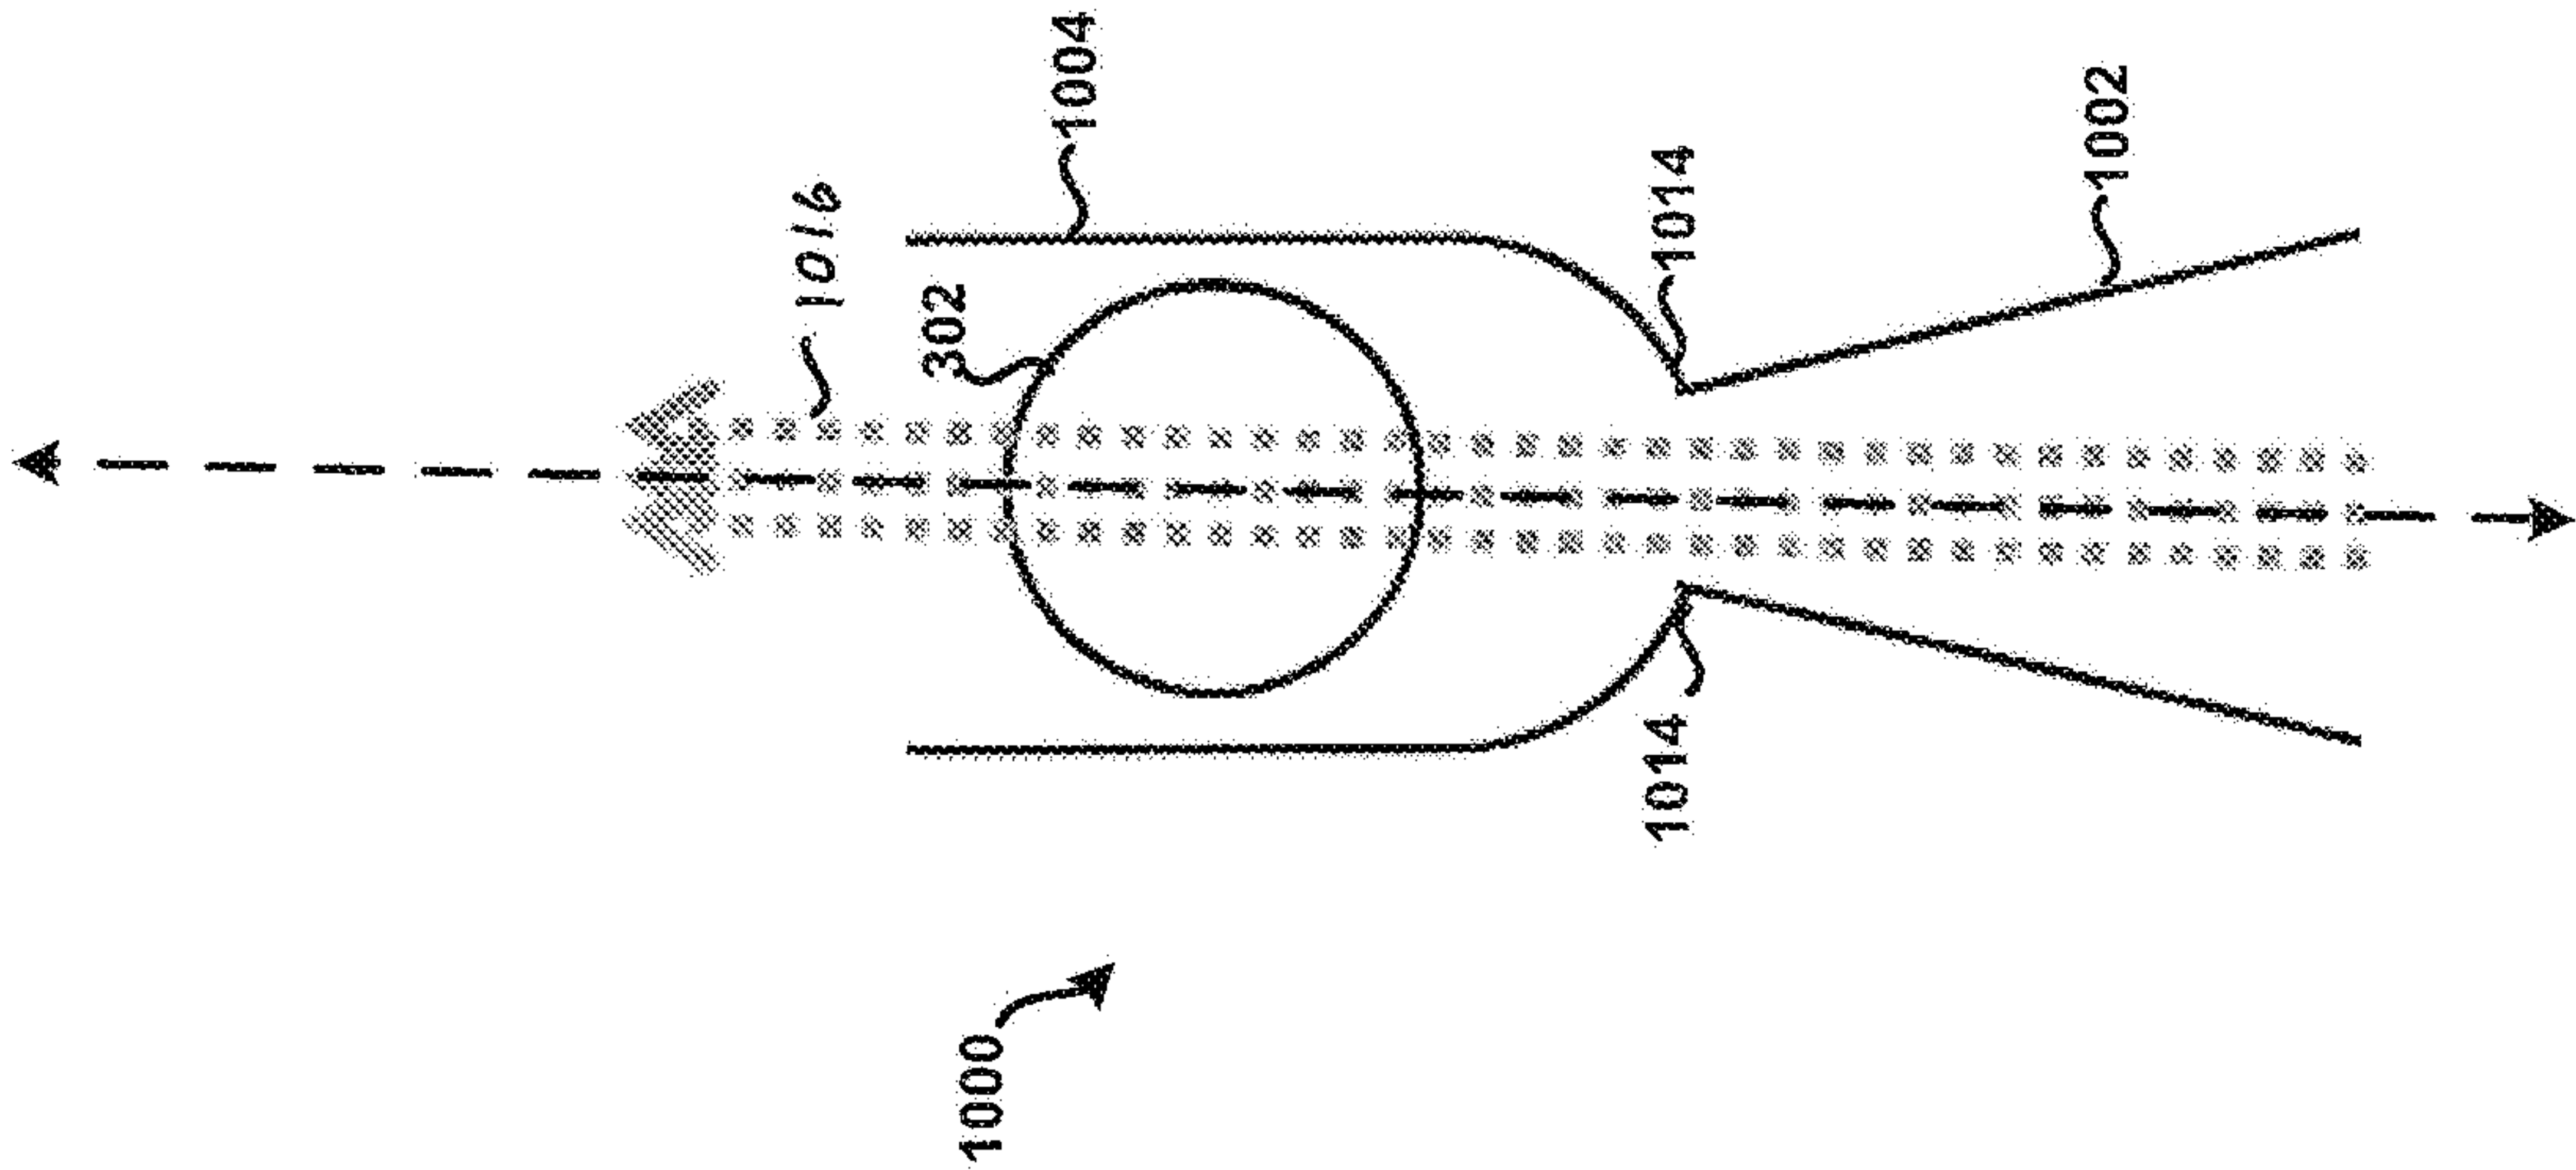


FIG. 14

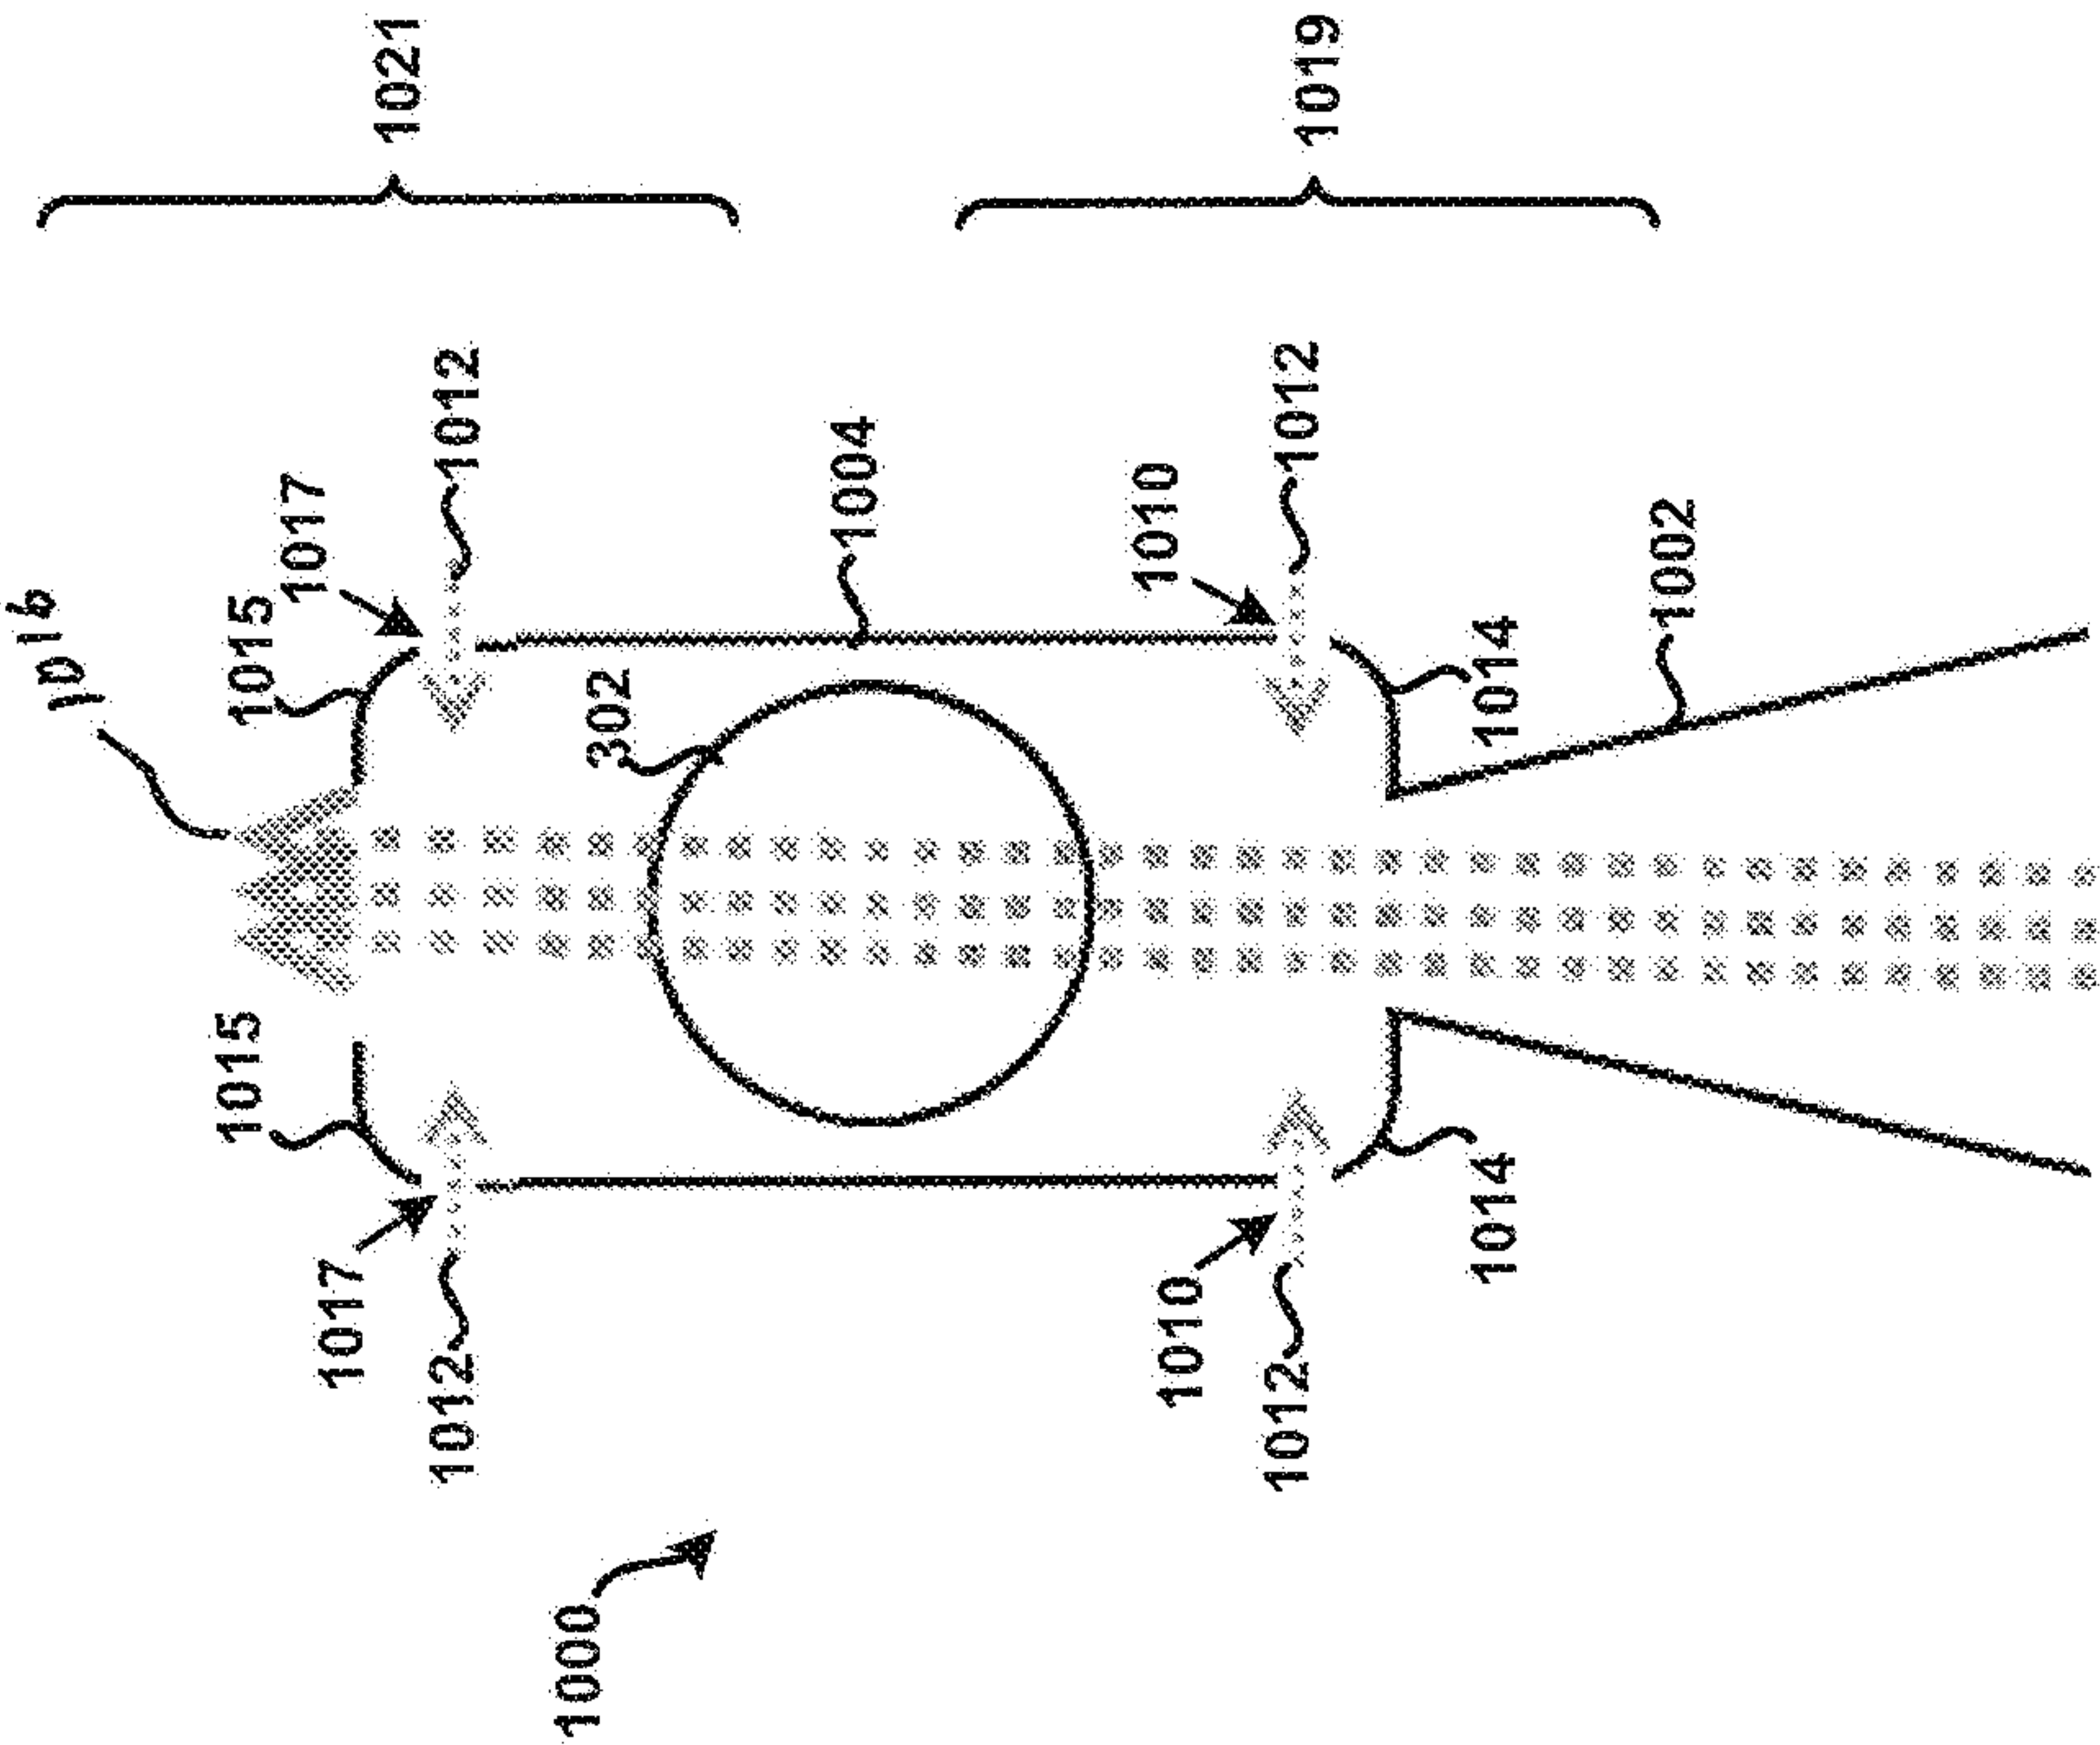


FIG. 15

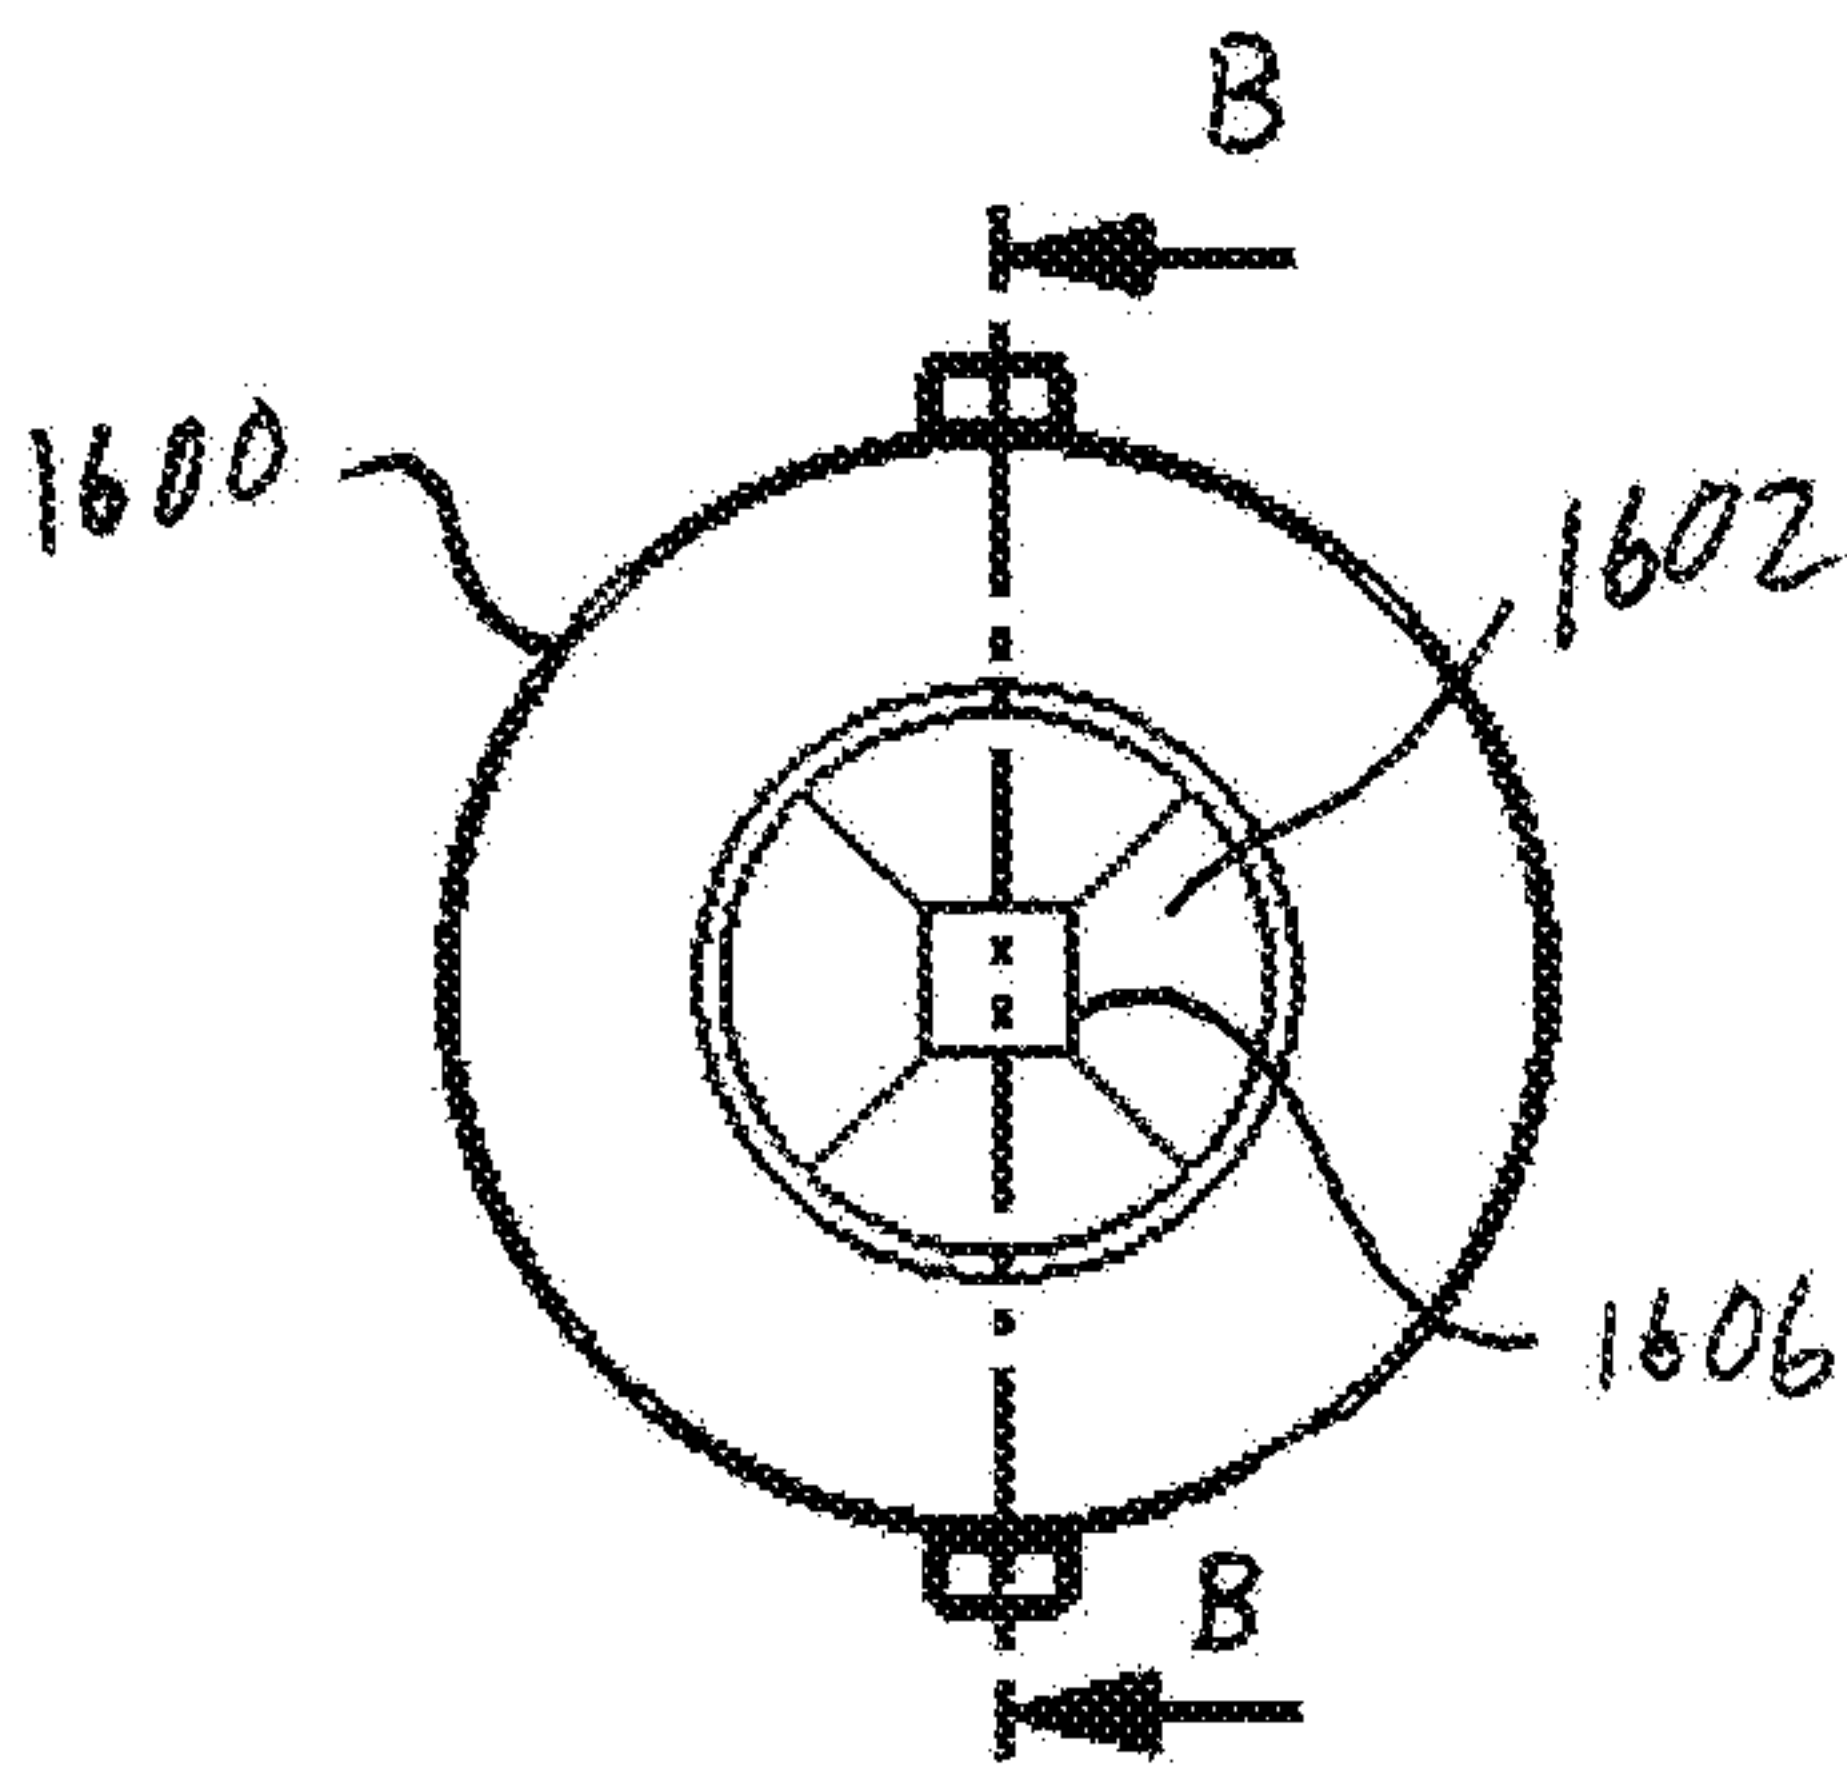


FIG. 16A


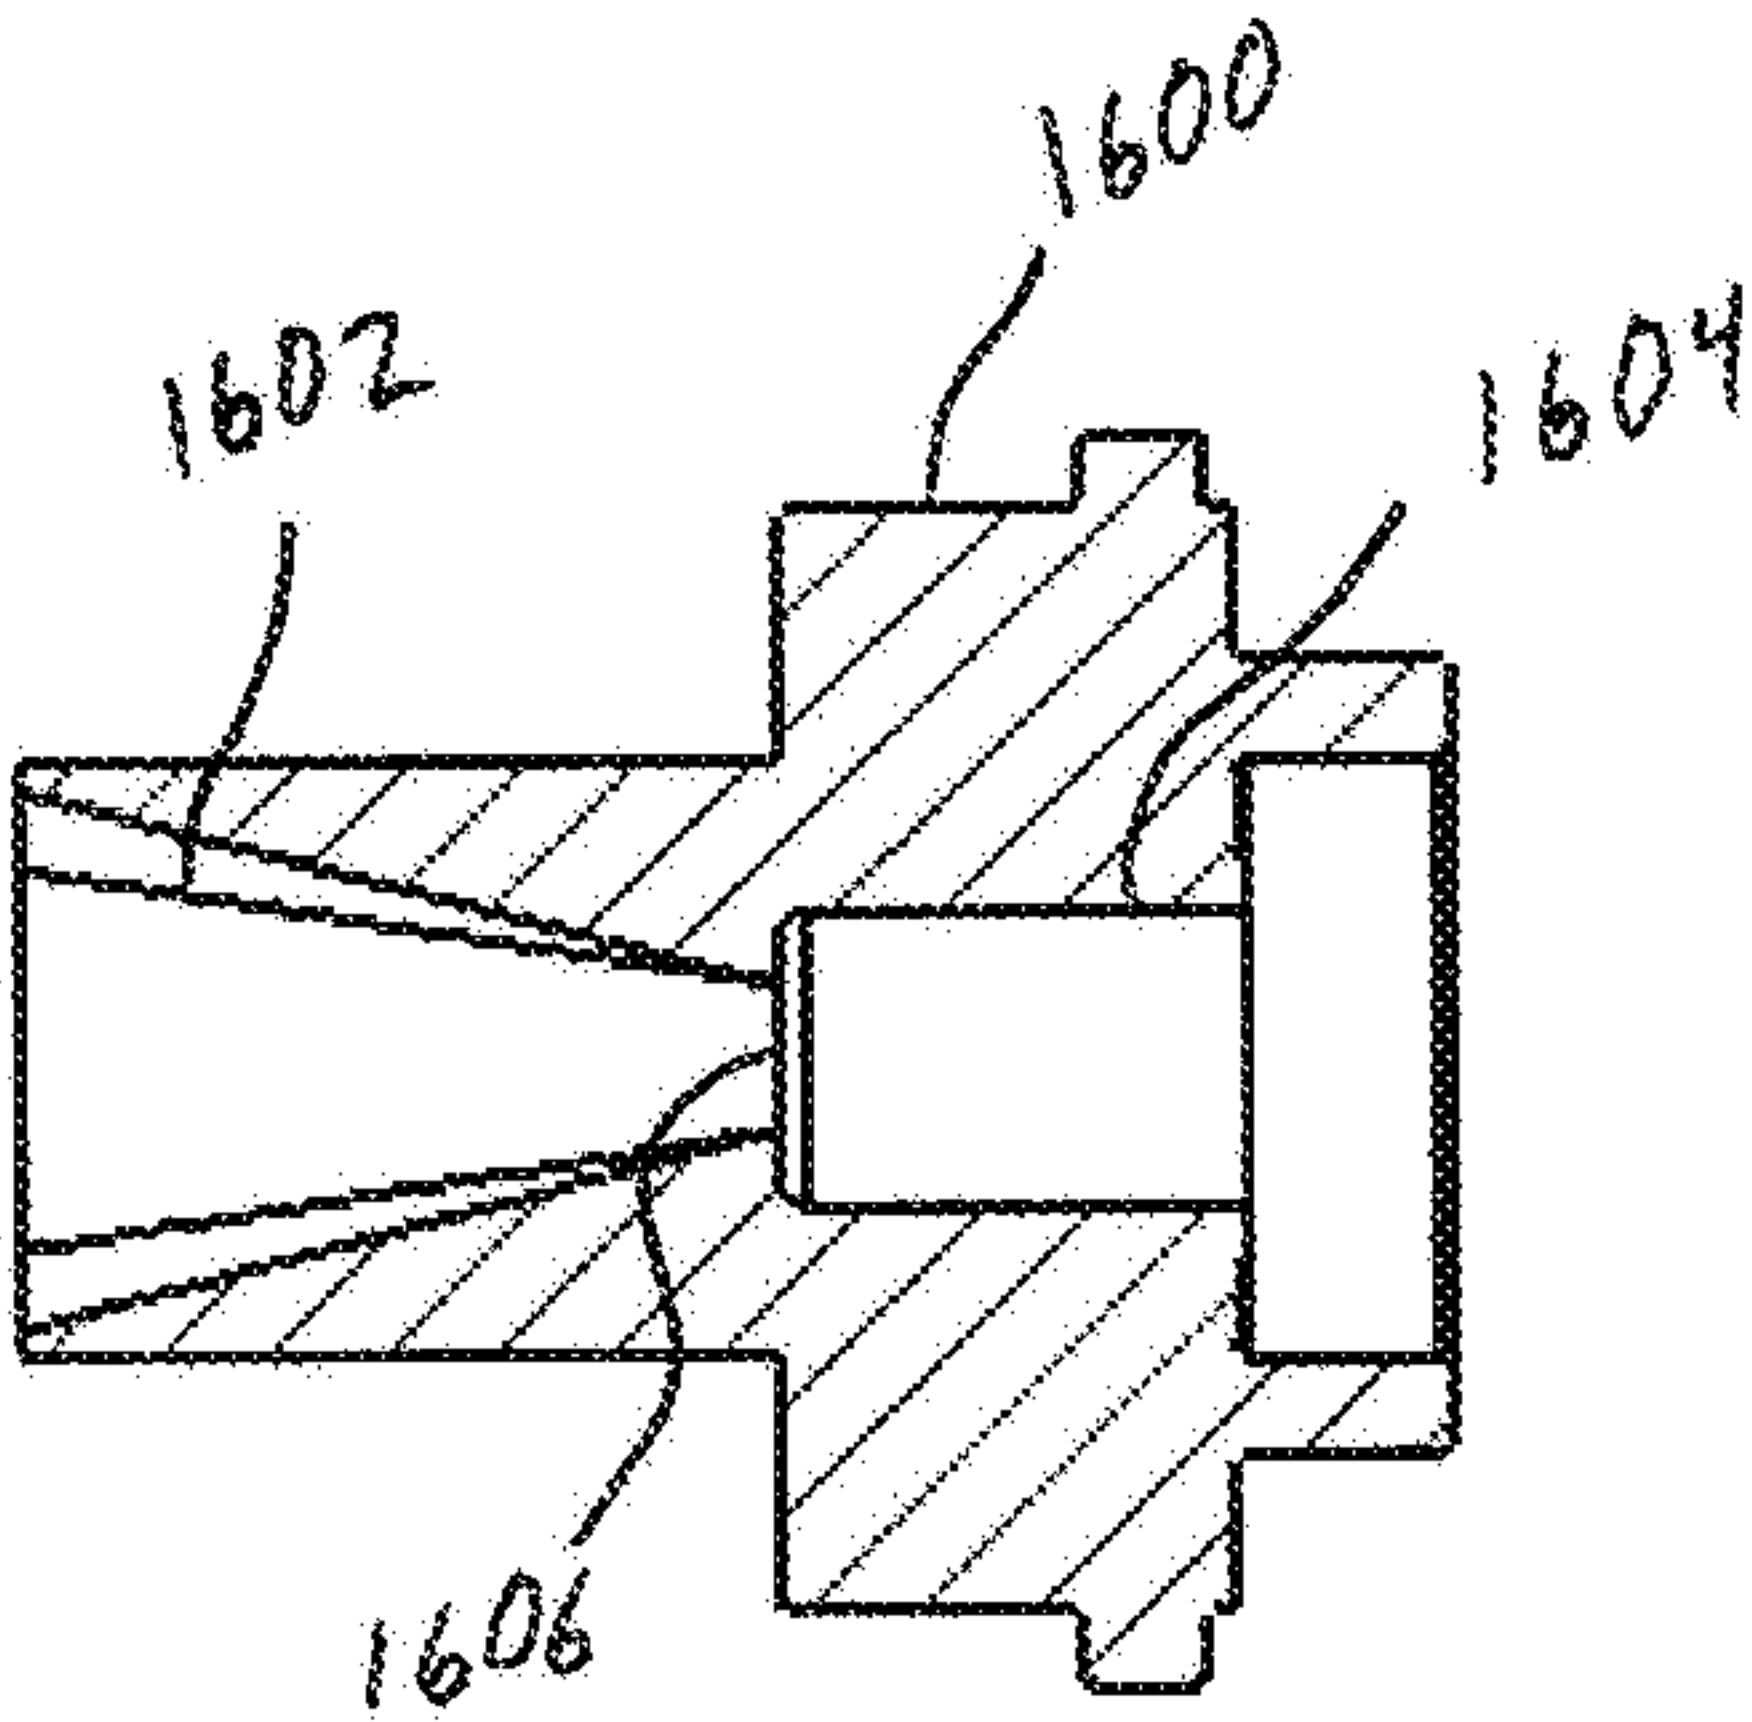


FIG. 16B

17/31

FIG. 17

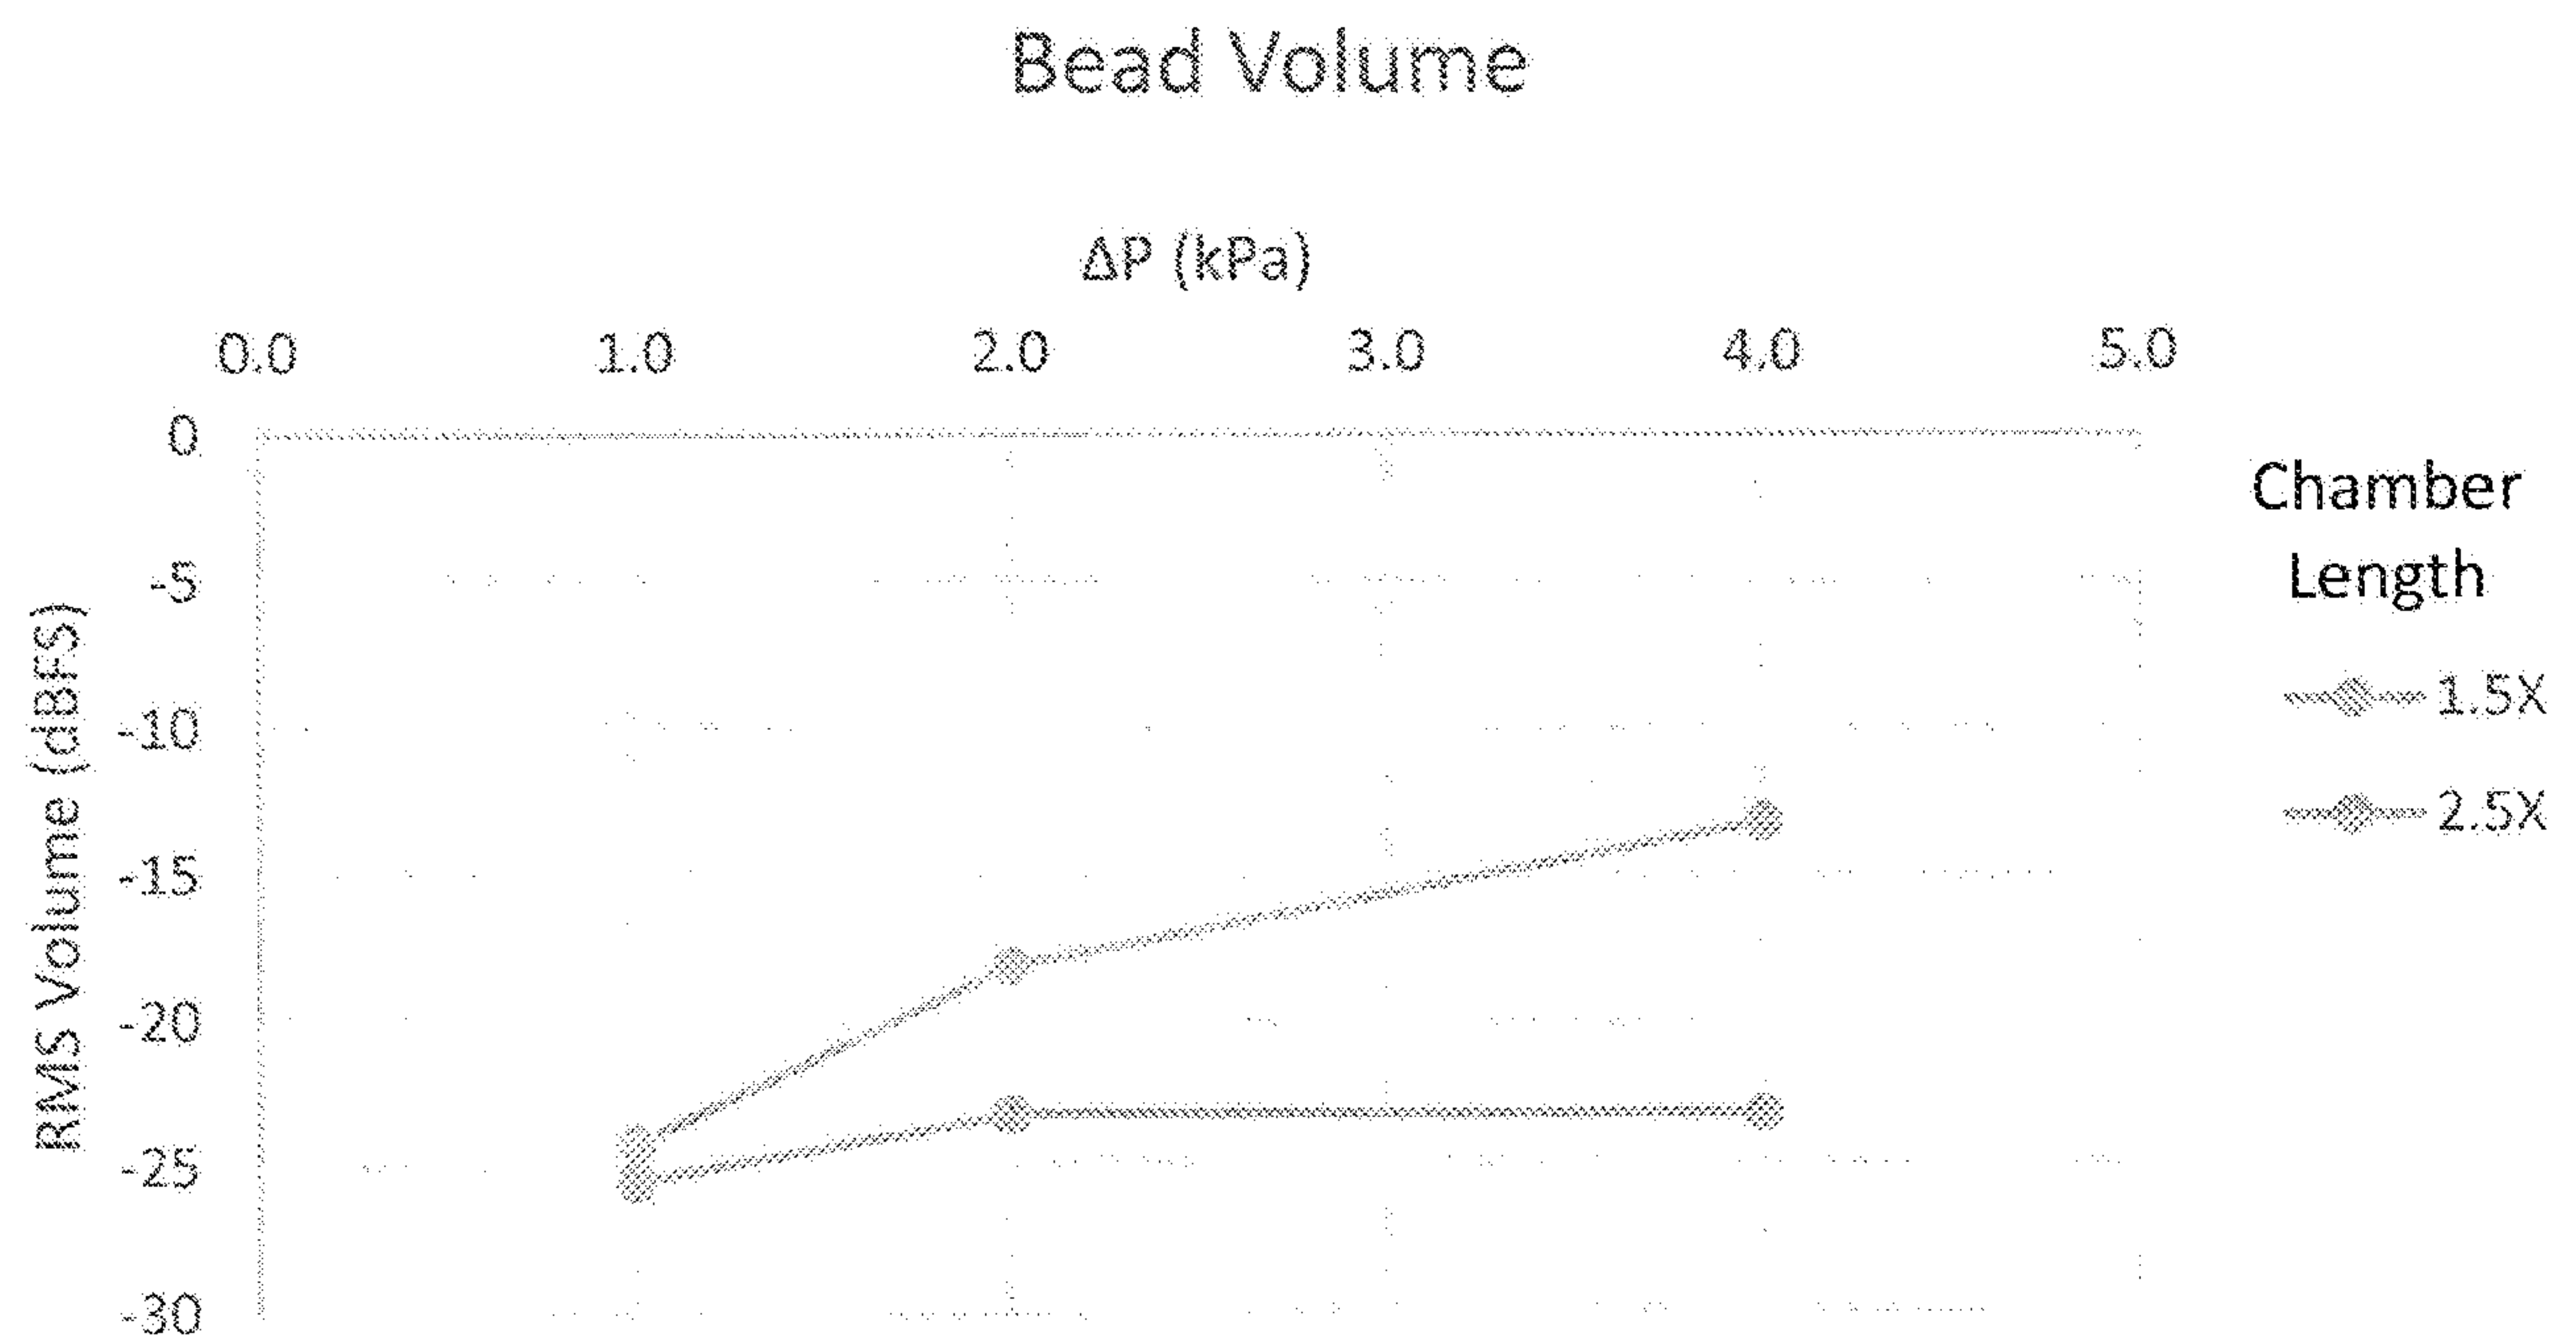

18/31

2.72mm Inlet - 4kPa

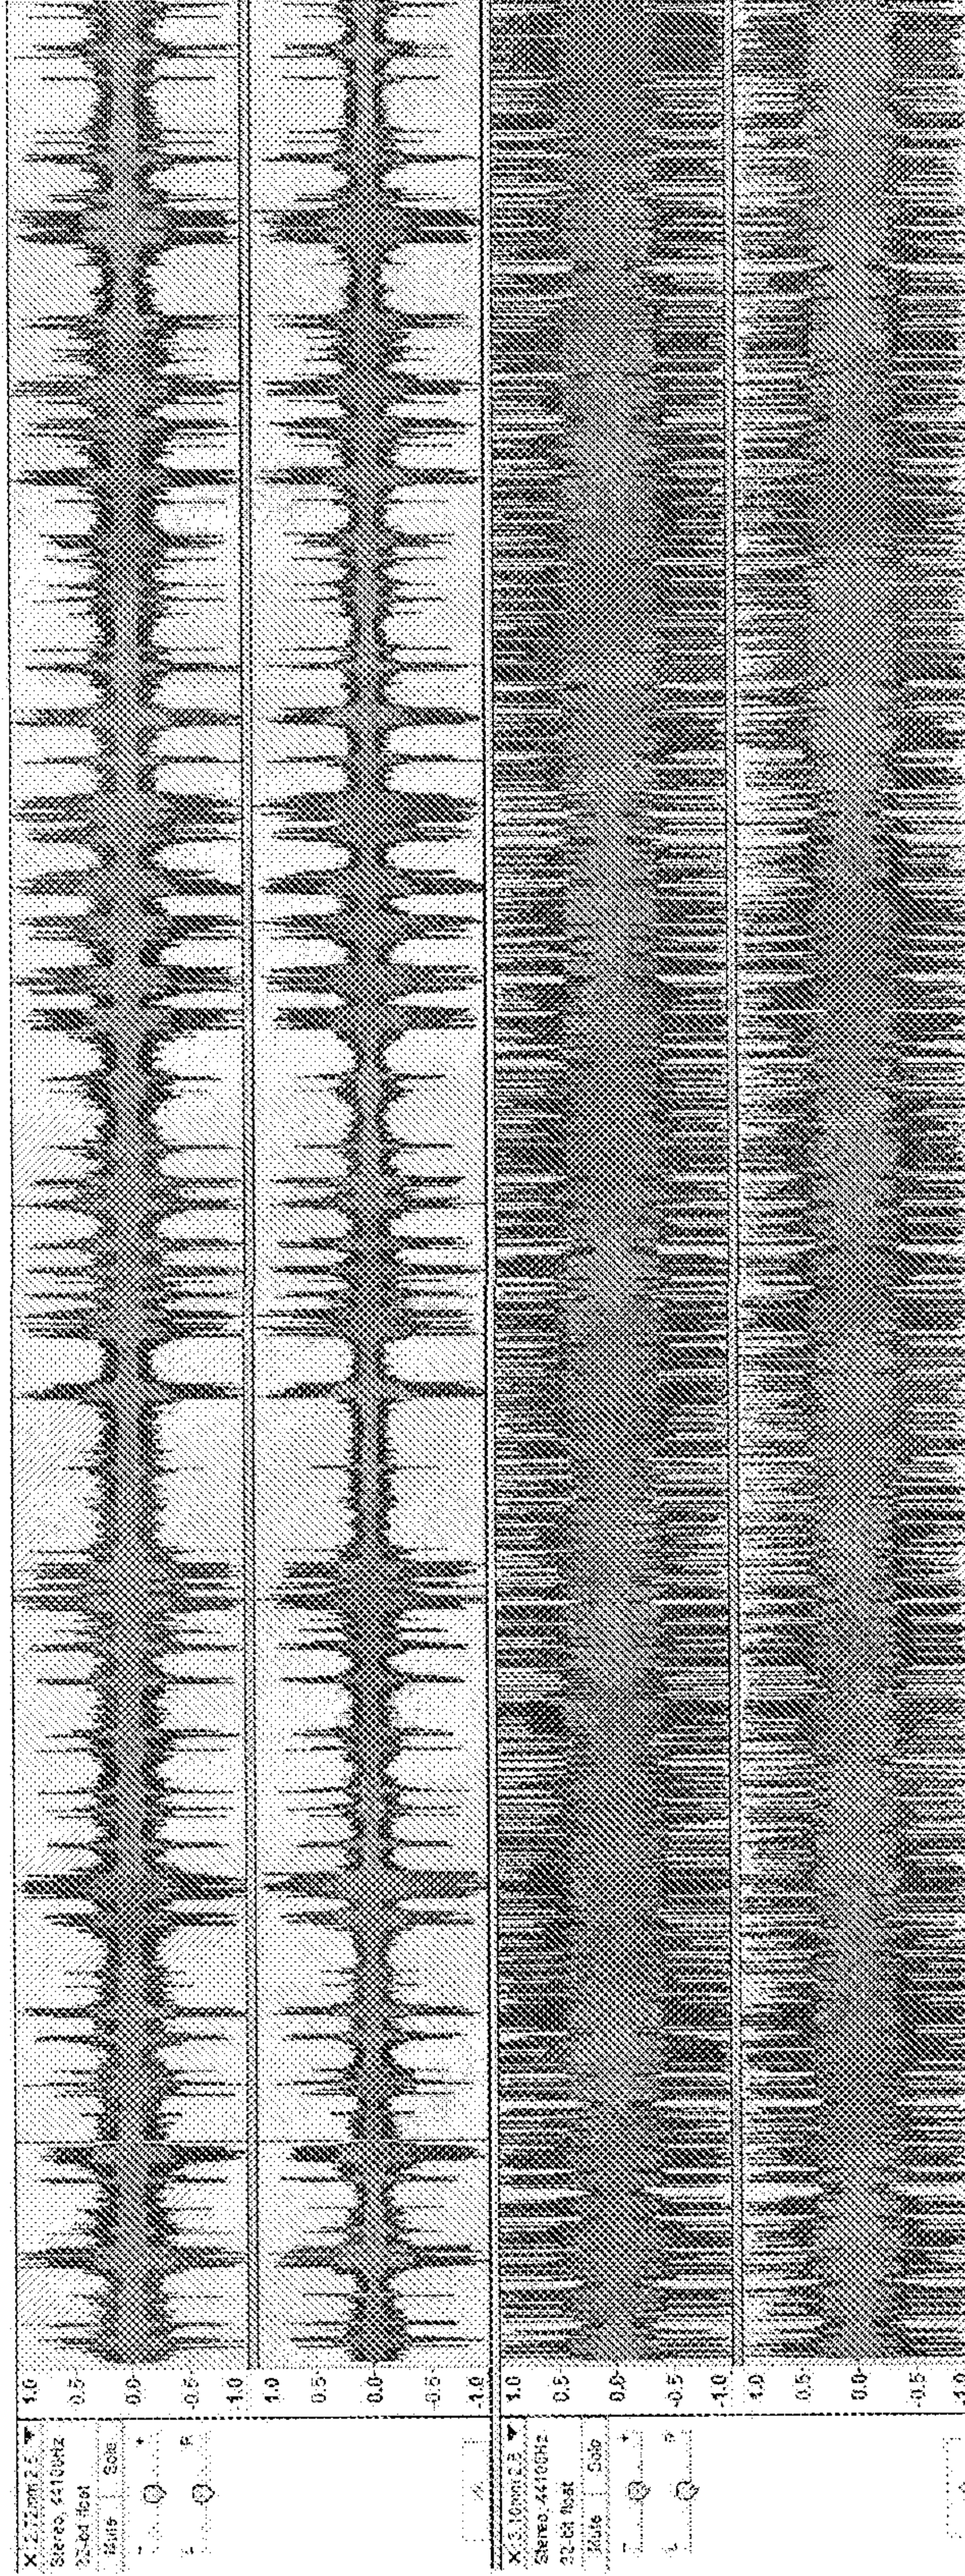



FIG. 18A

FIG. 18B

3.10mm Inlet - 4kPa

FIG. 19A

1kPa

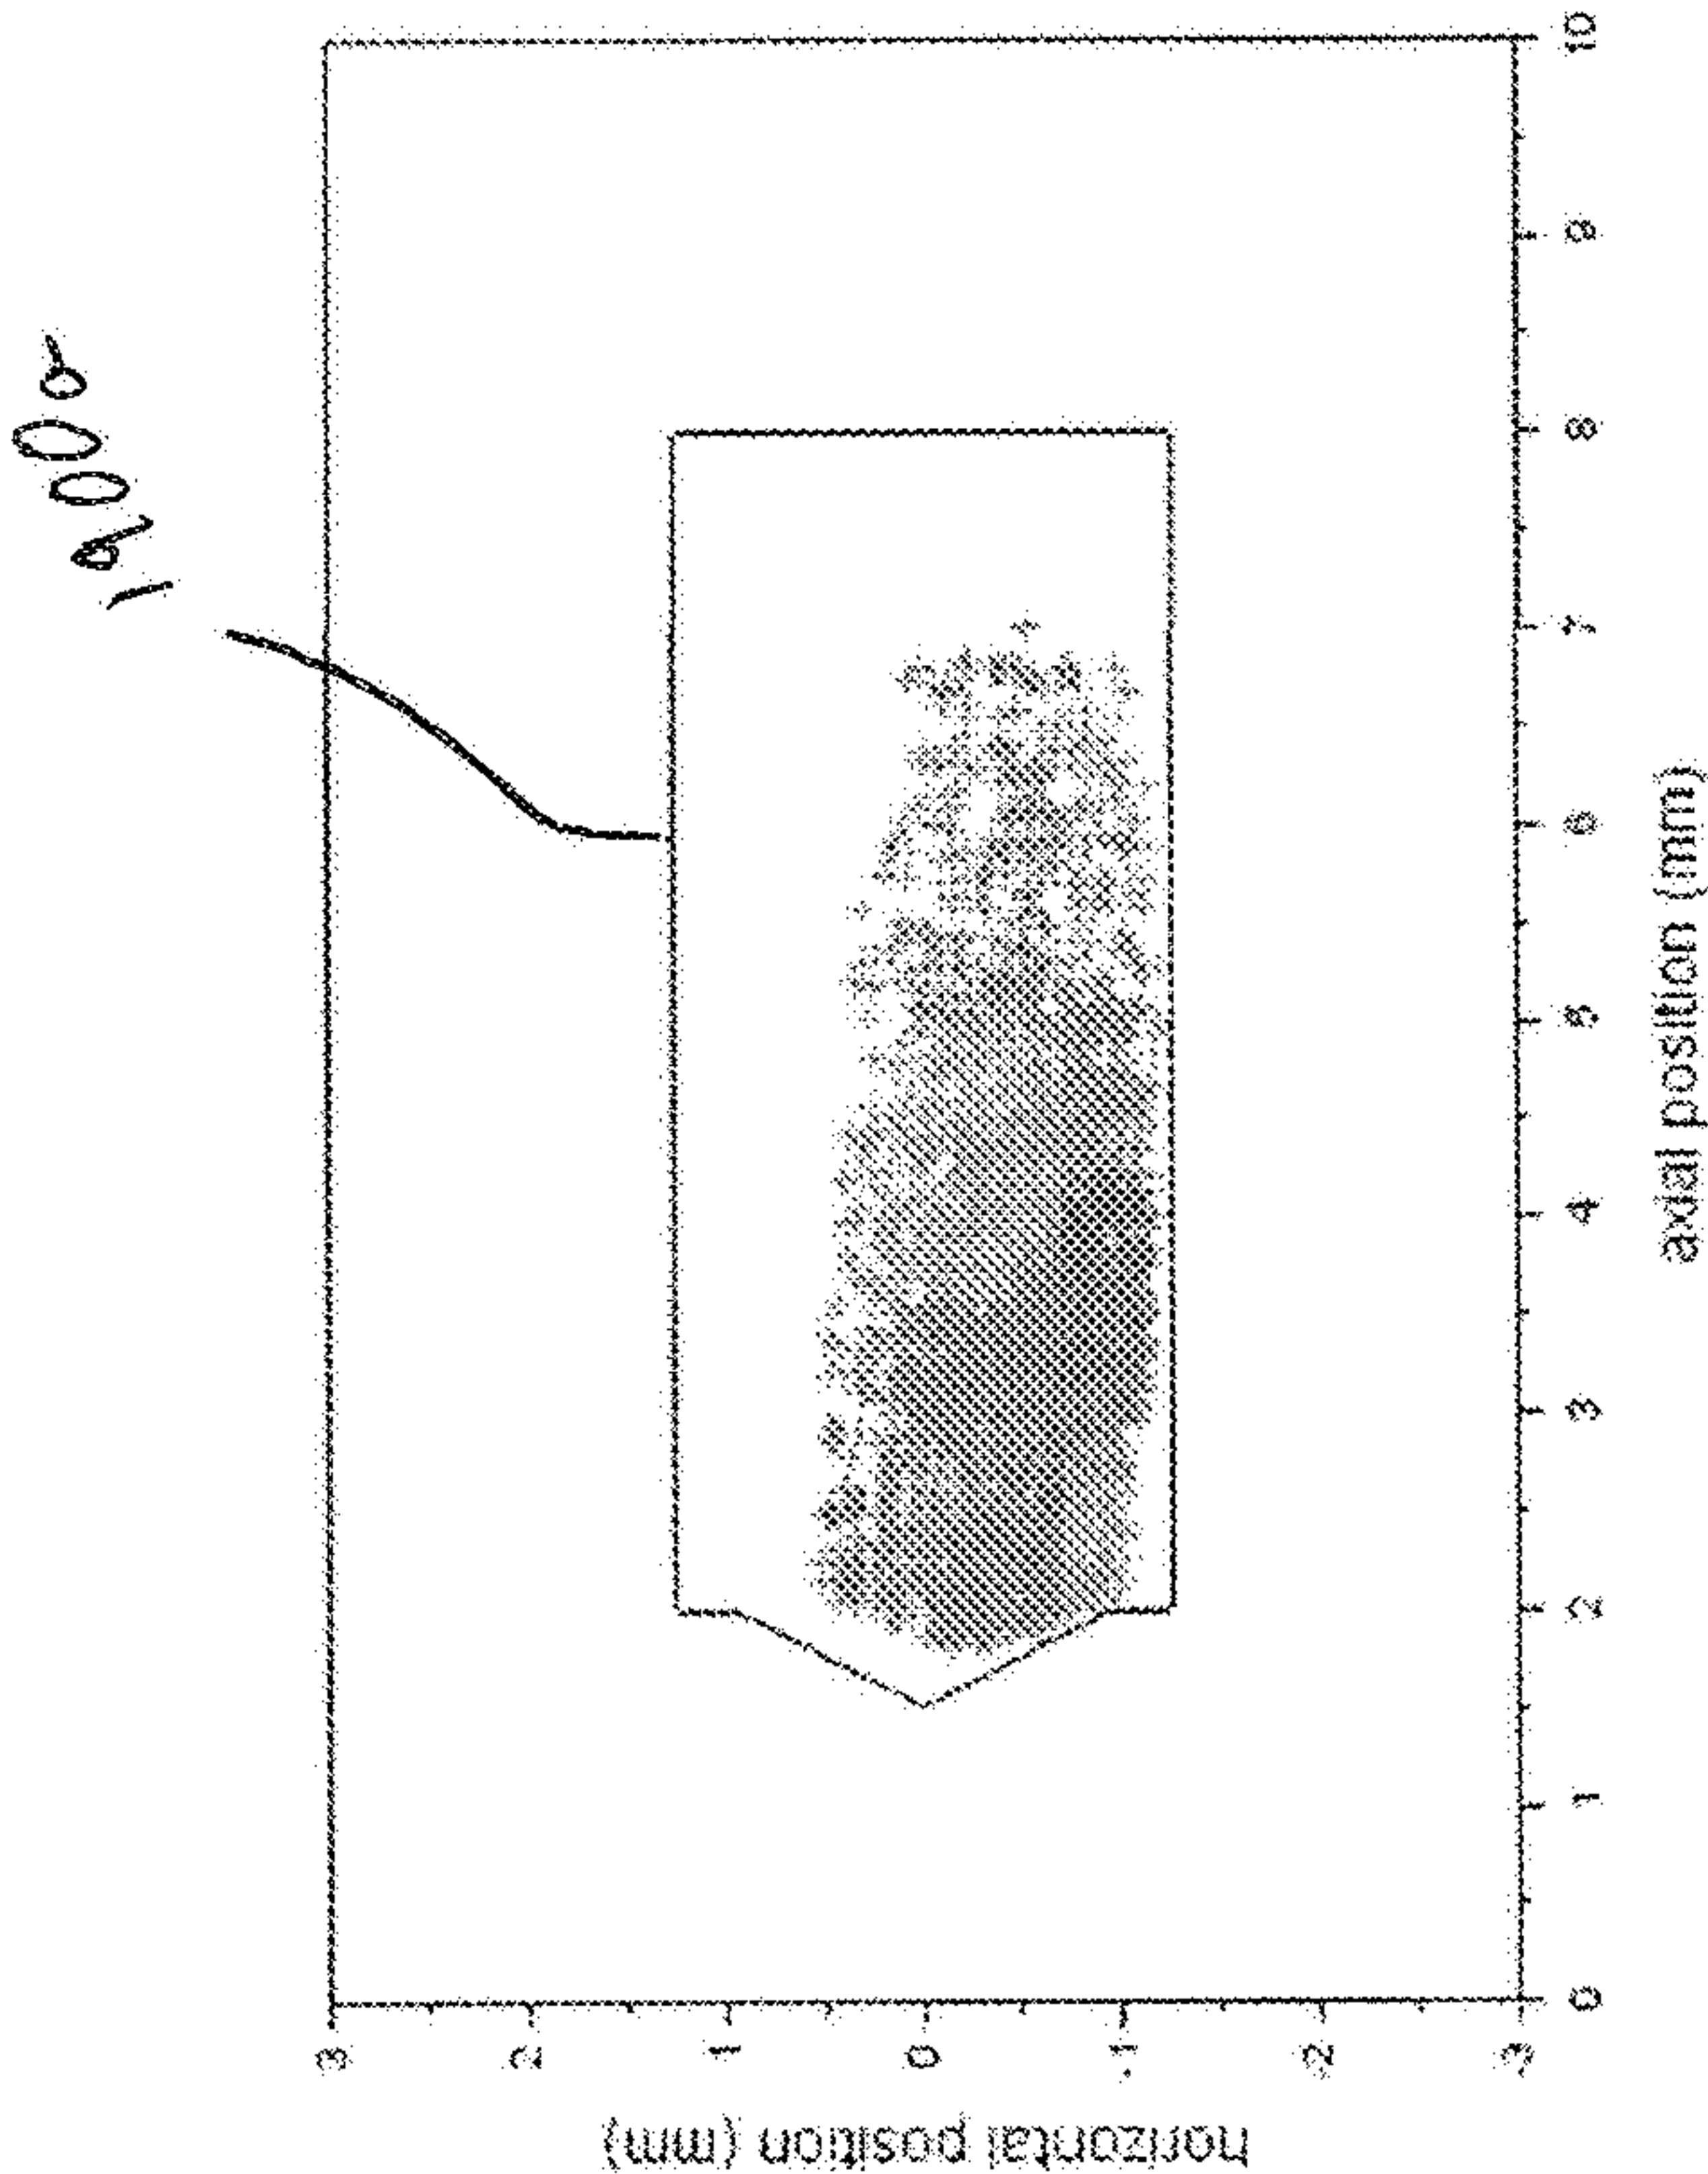



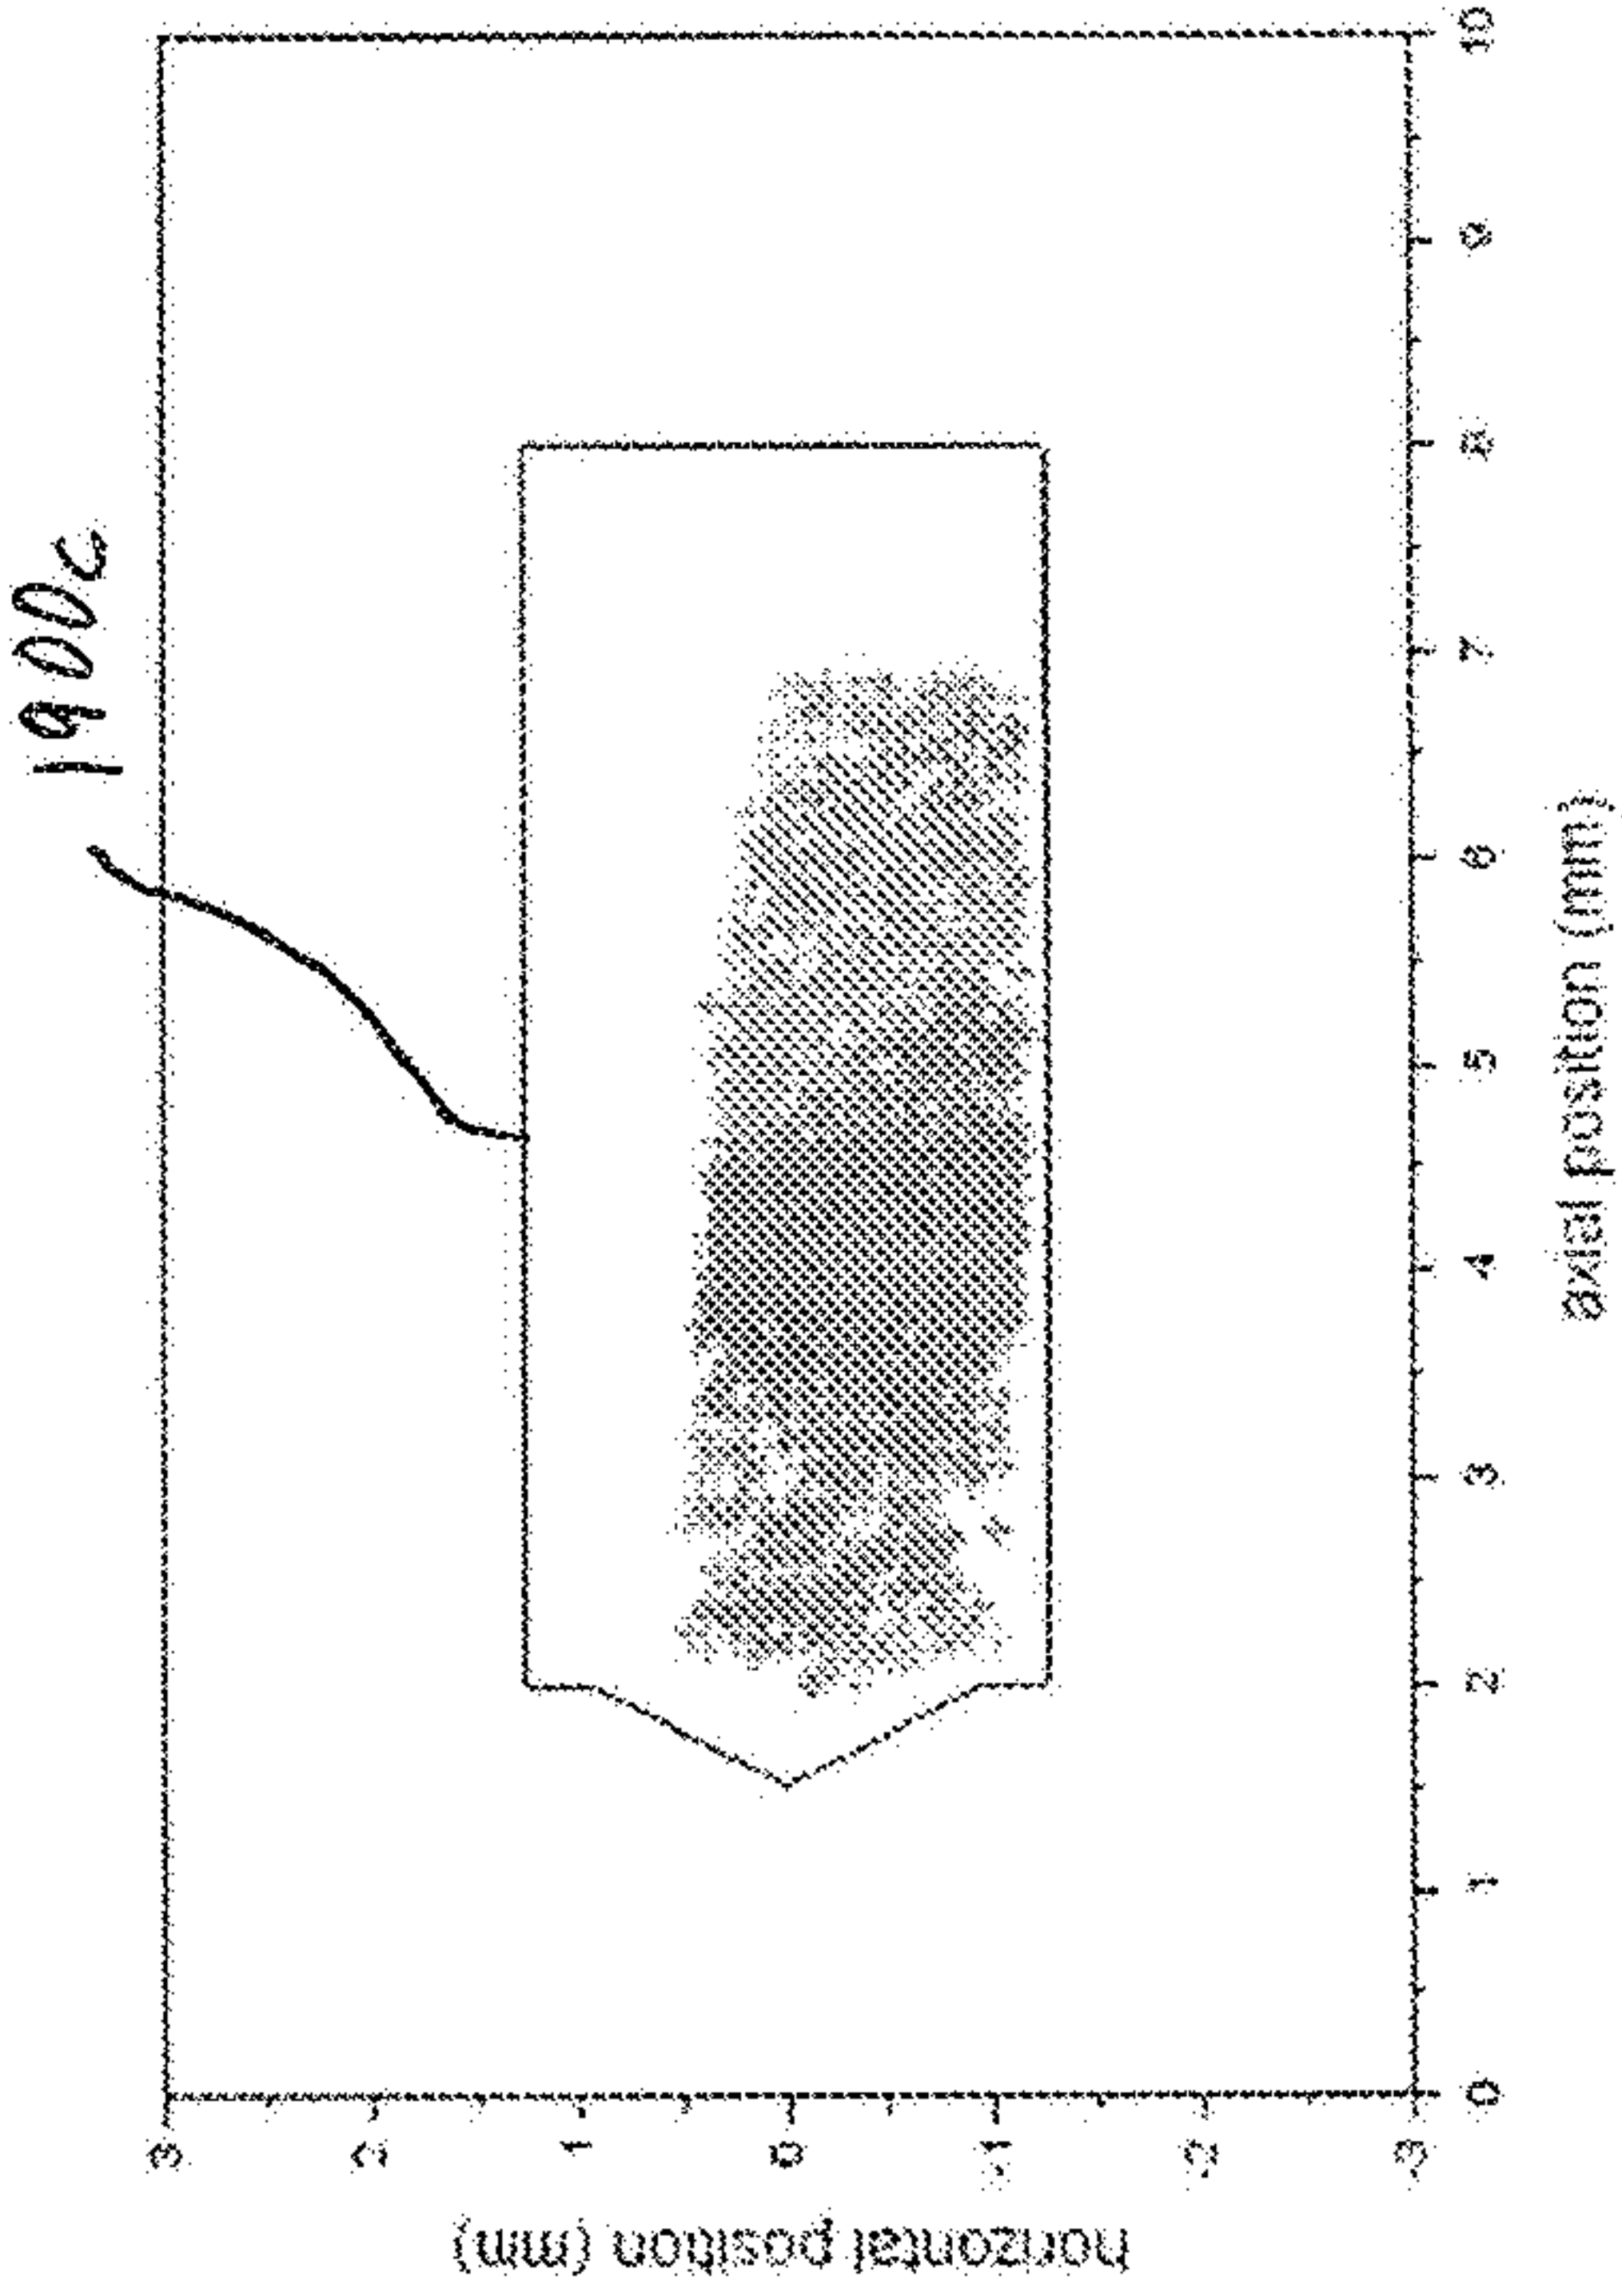


FIG. 20A

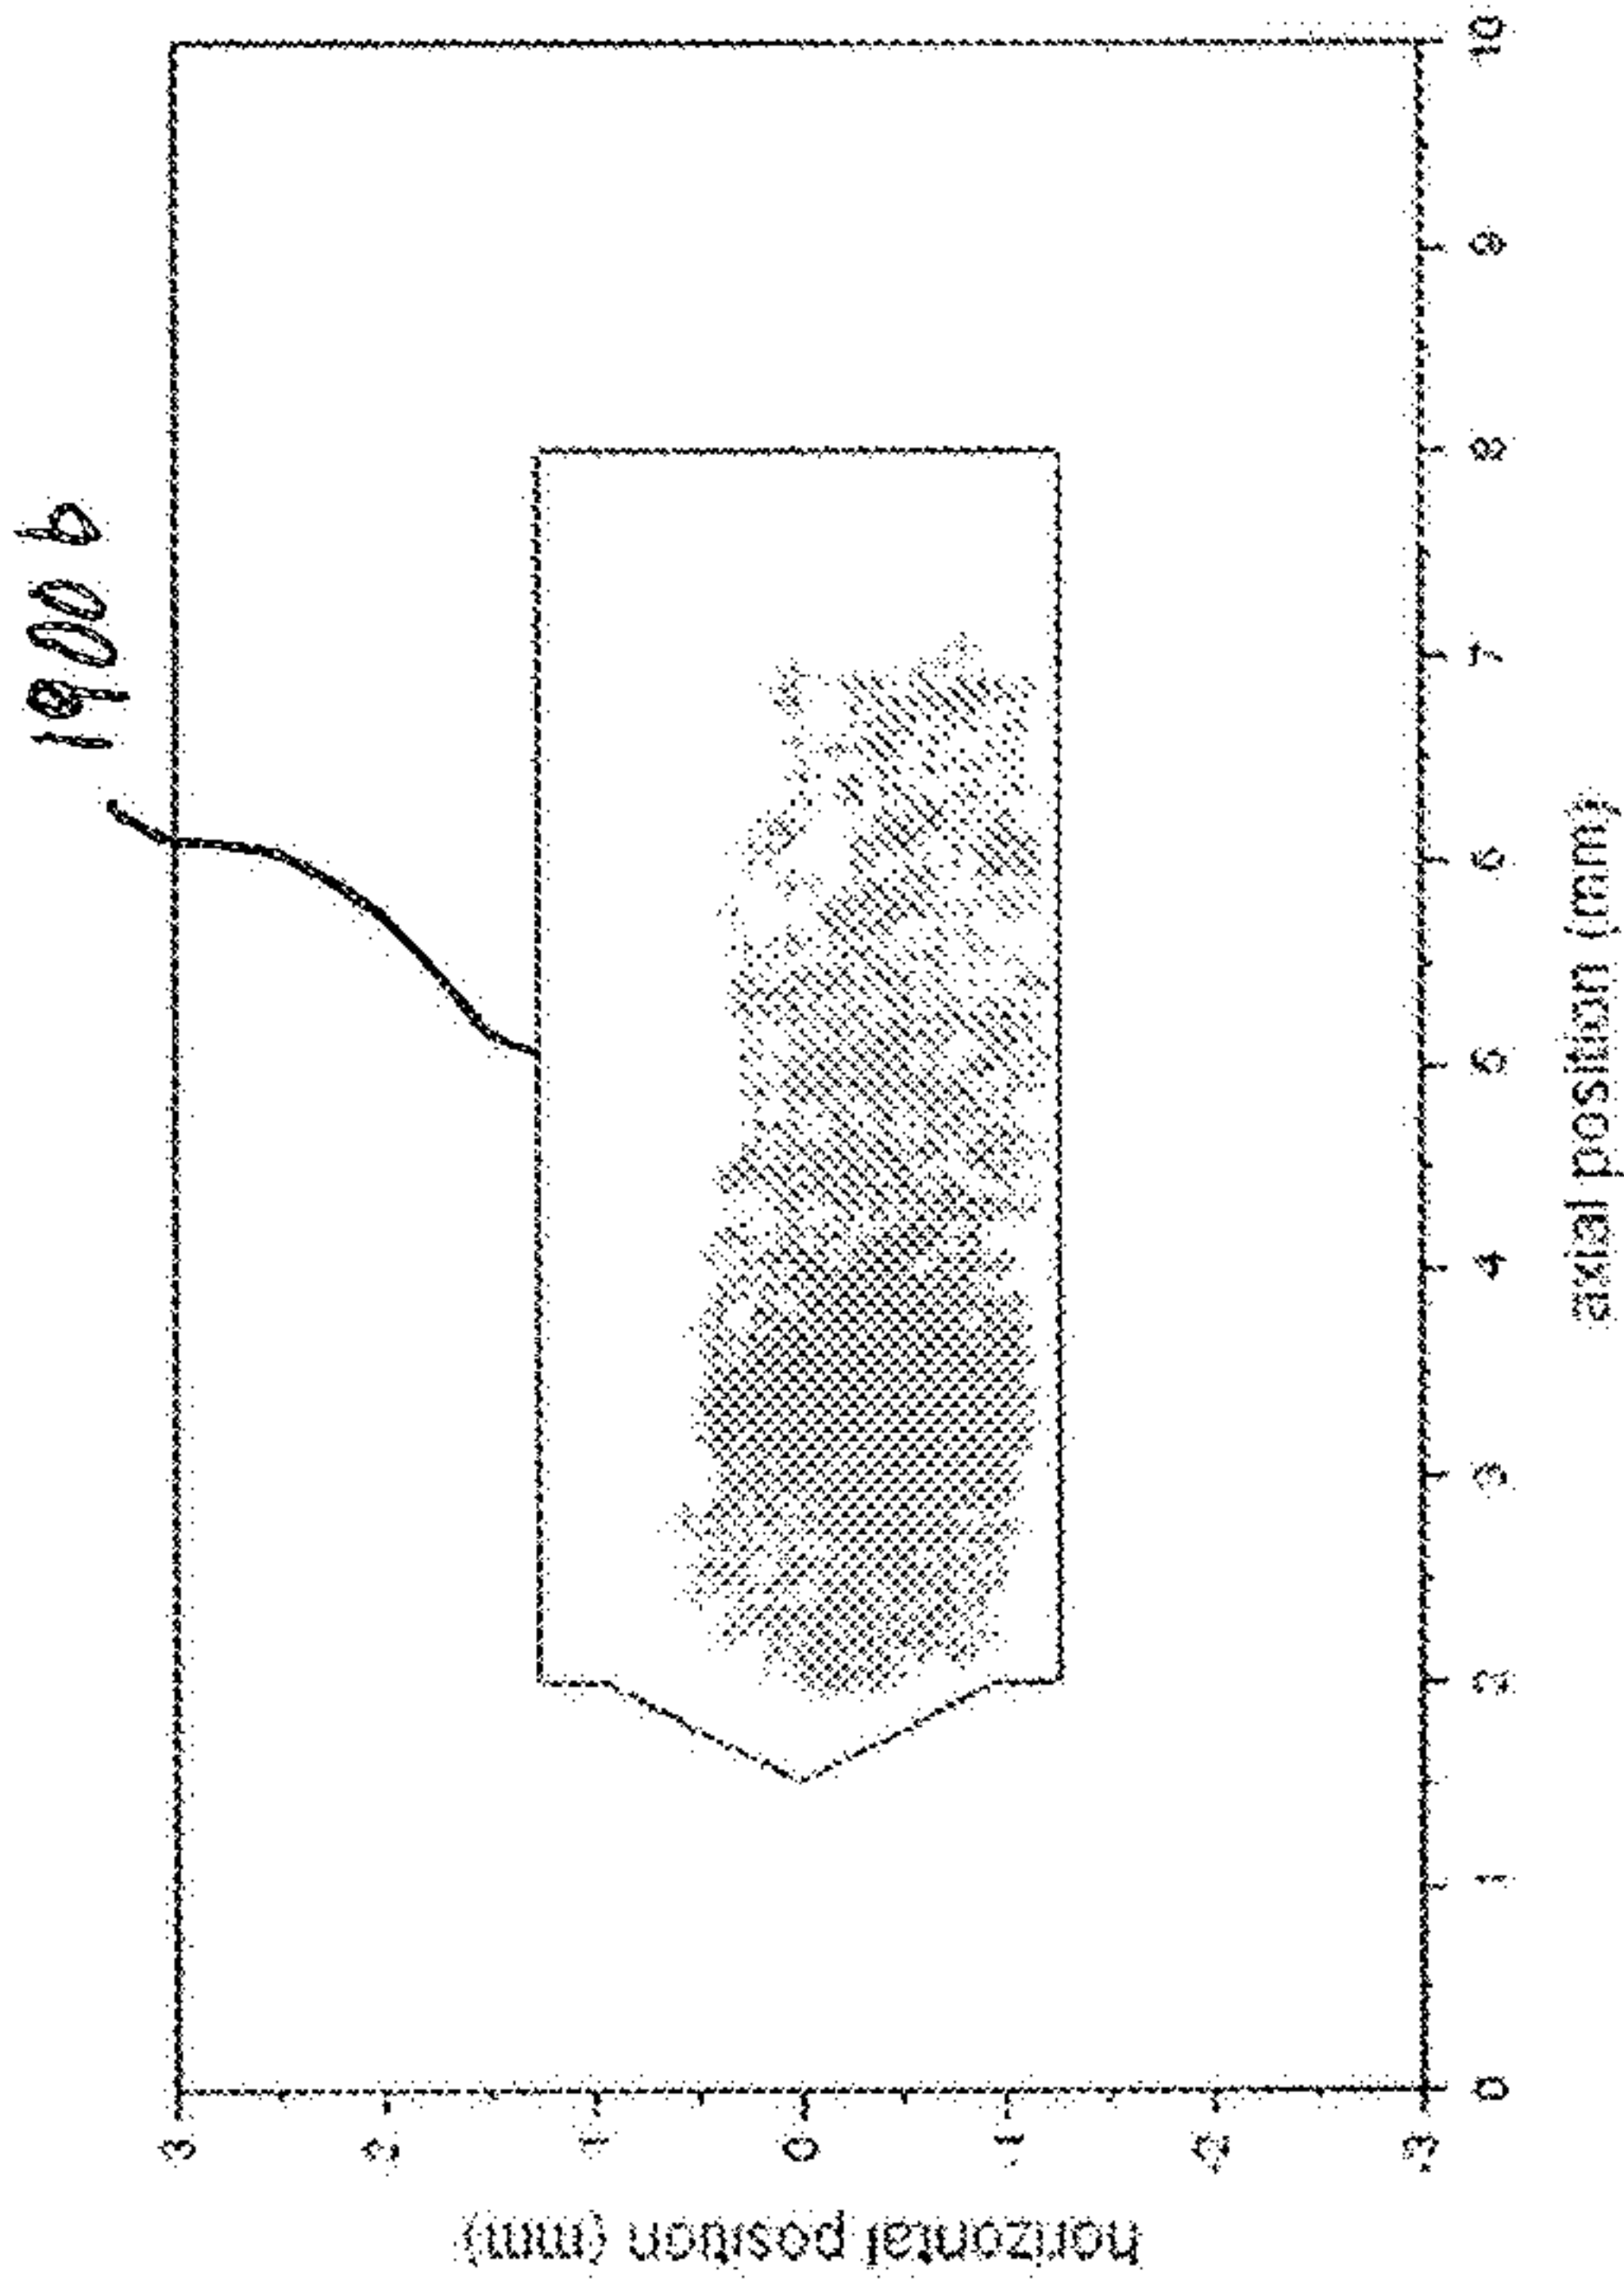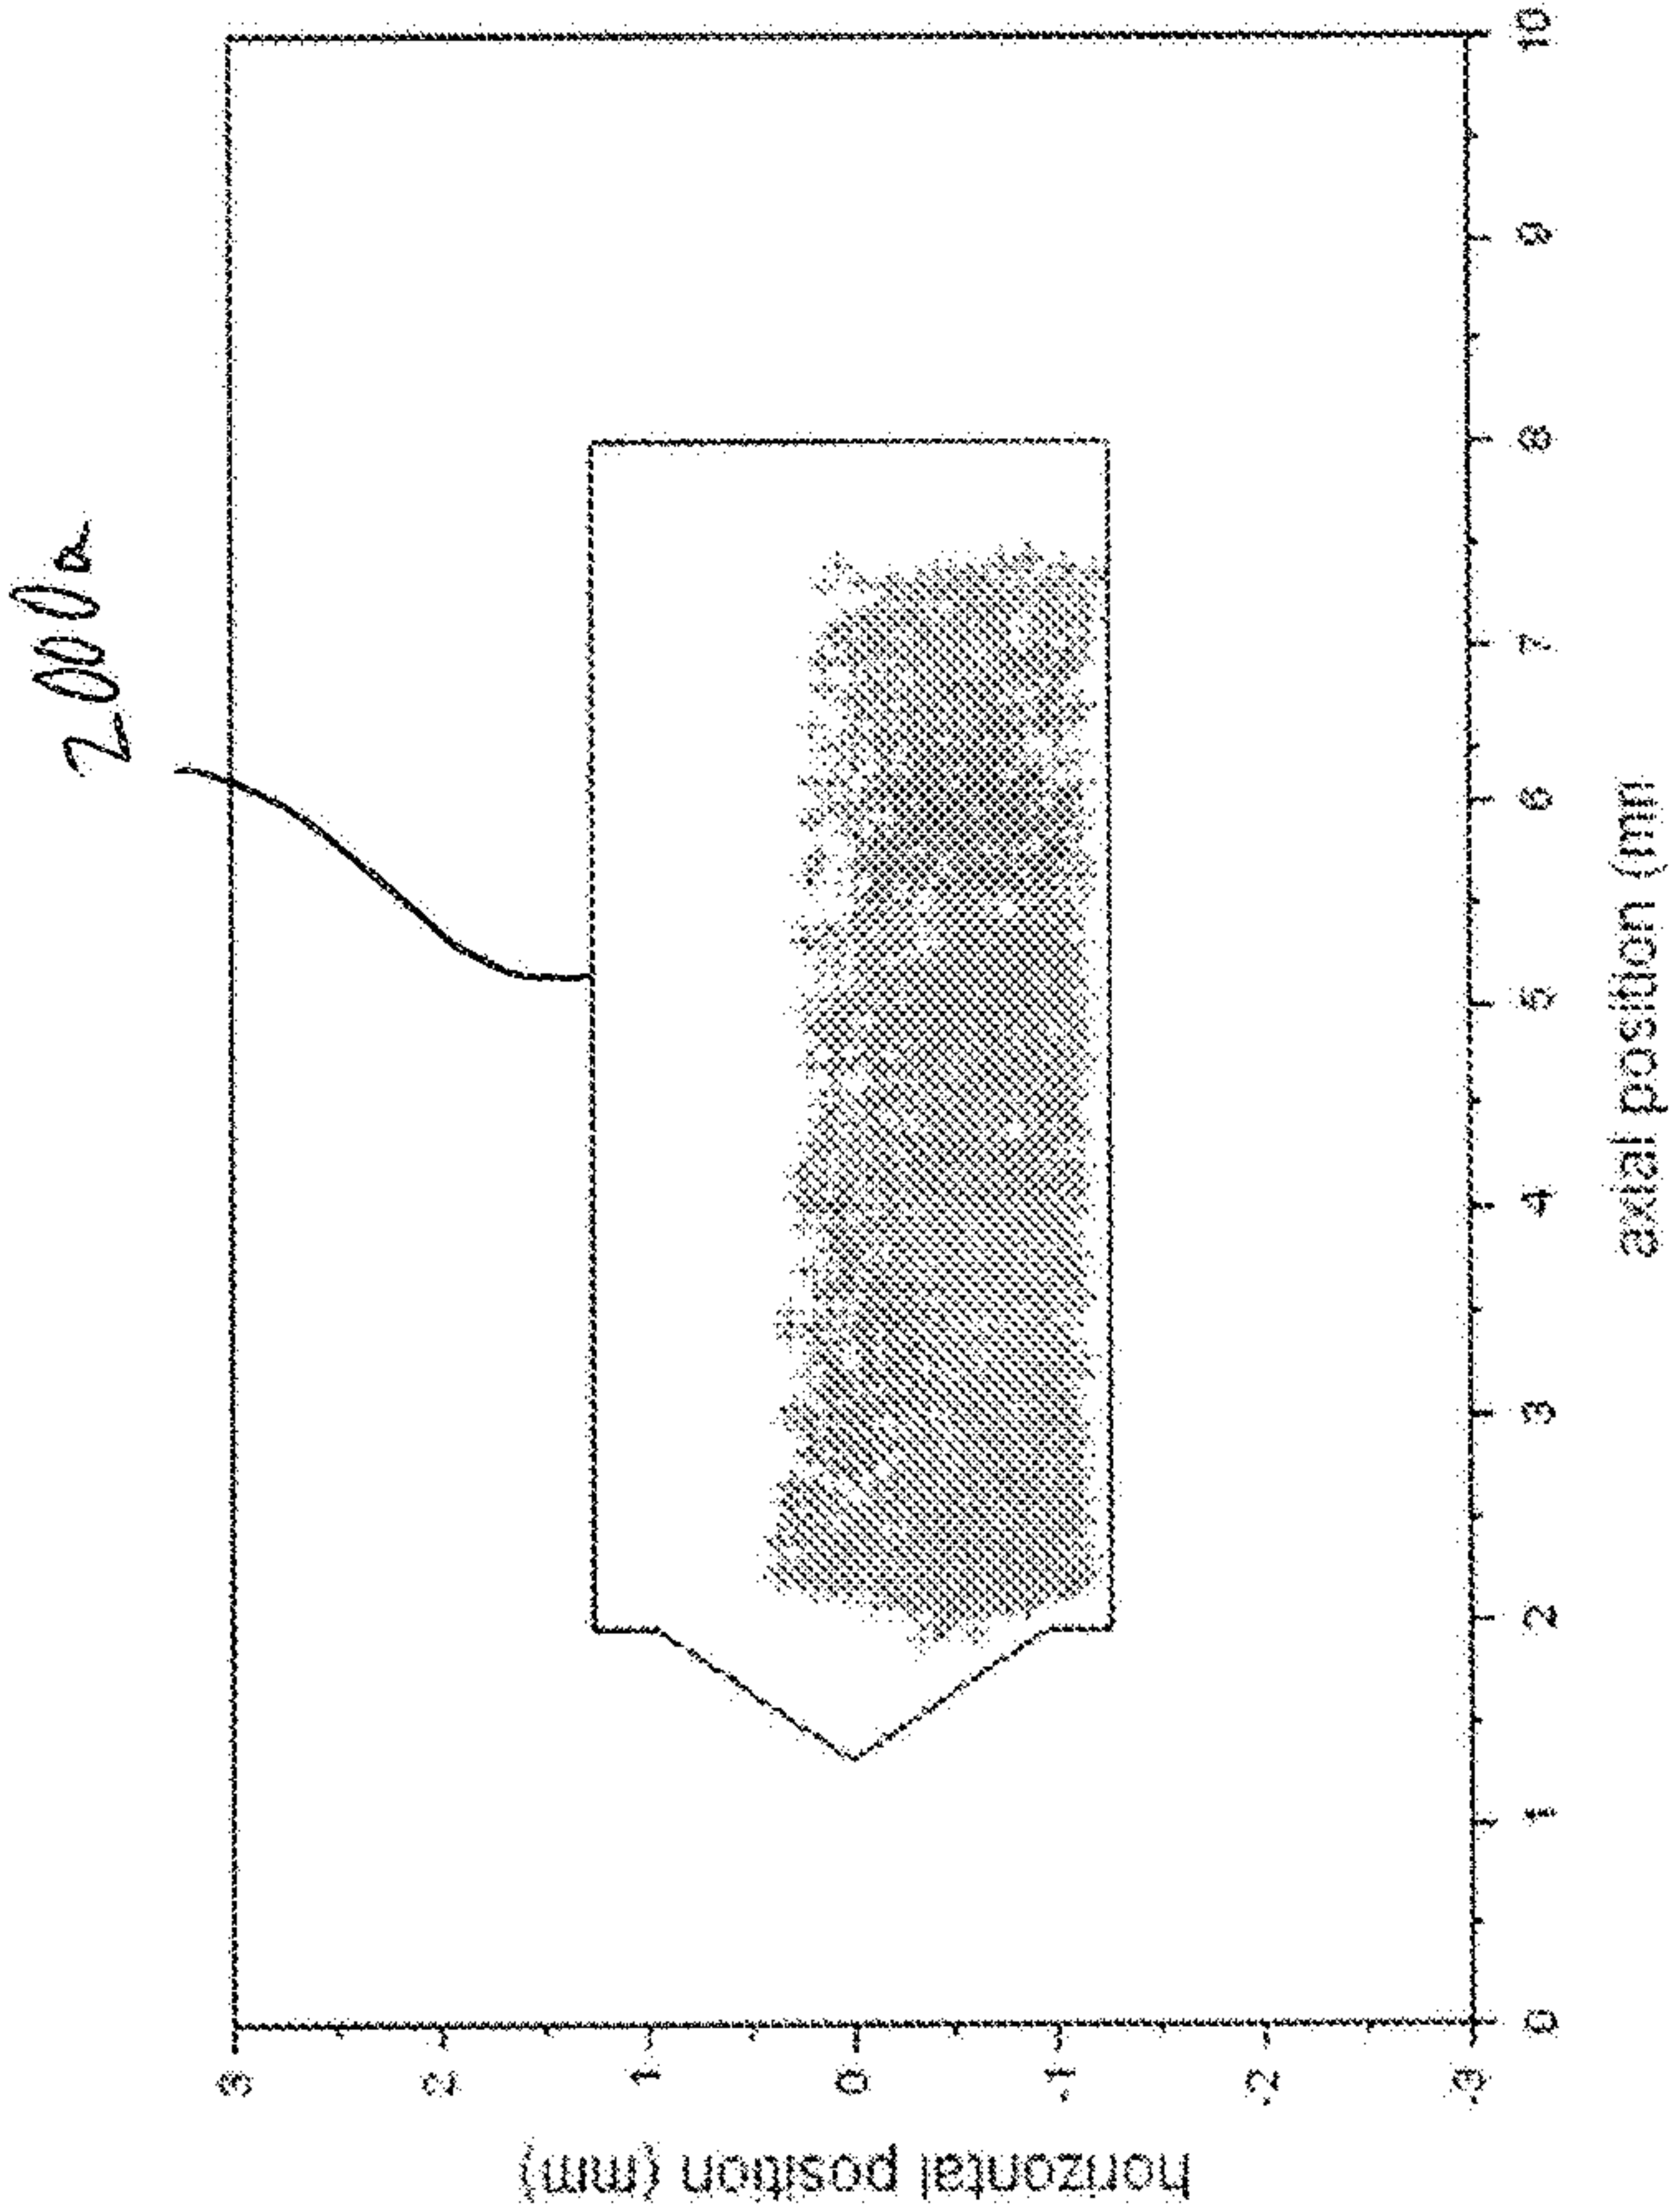

1 kPa

FIG. 20B



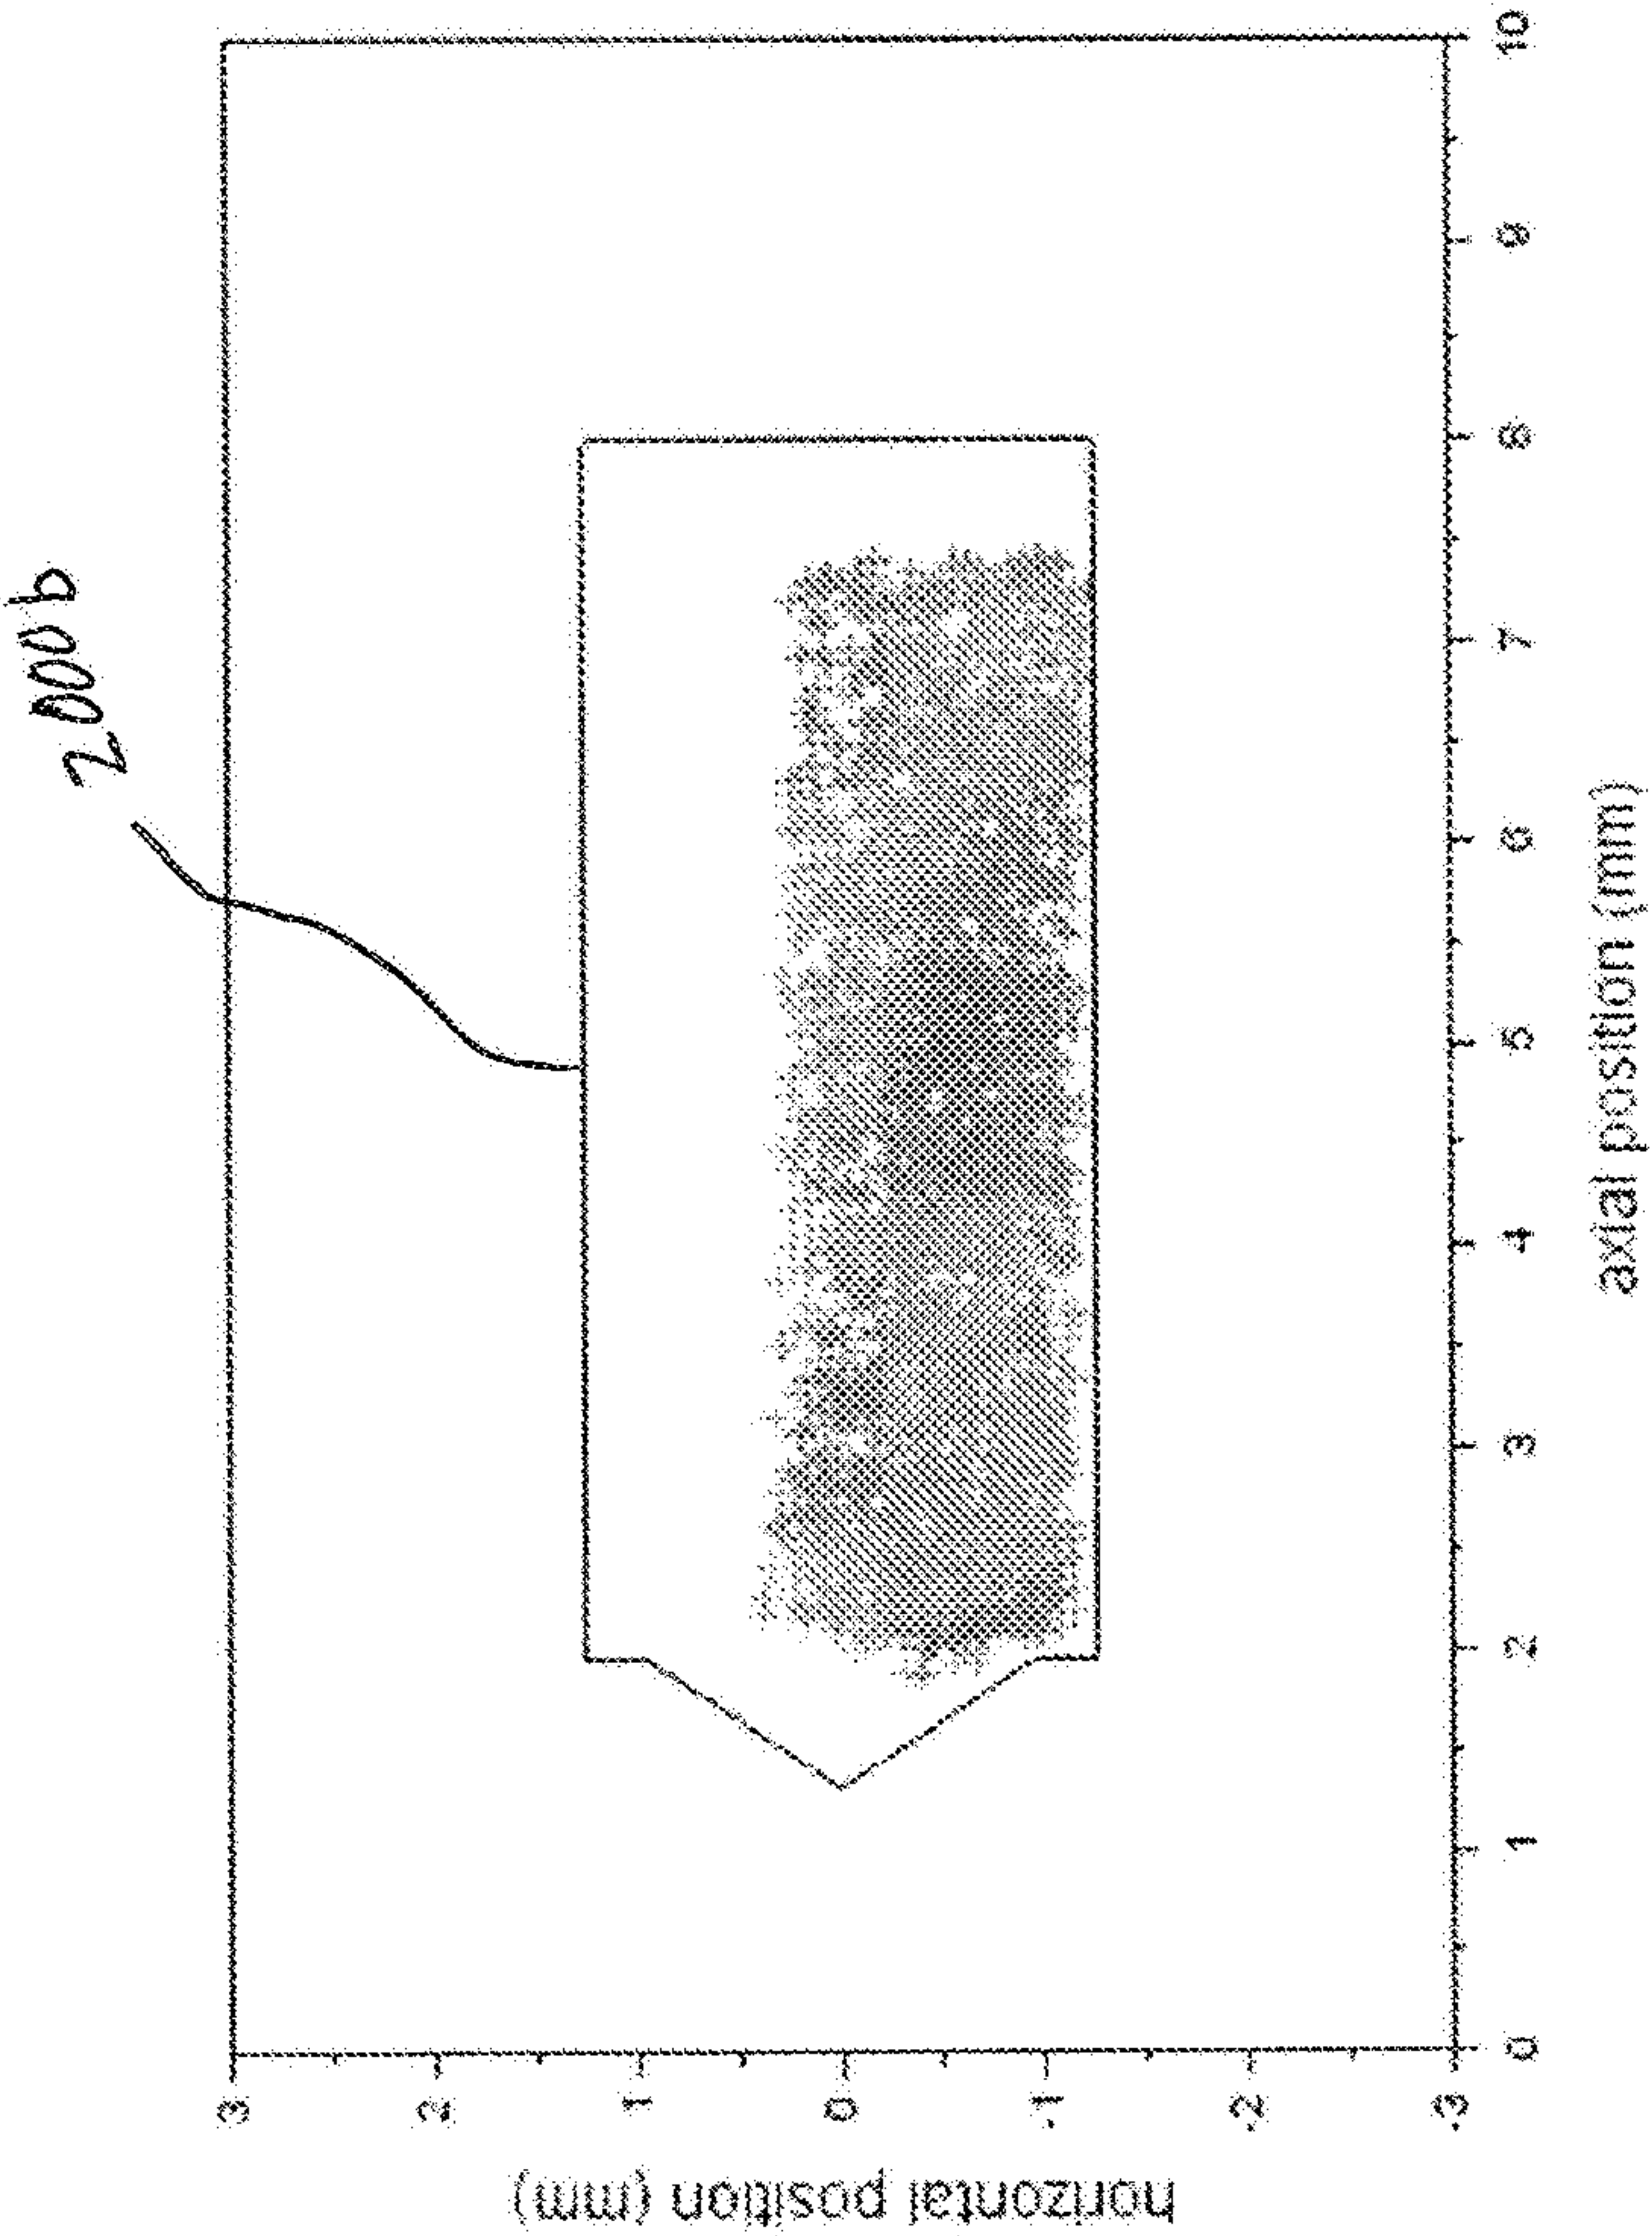


FIG. 20C

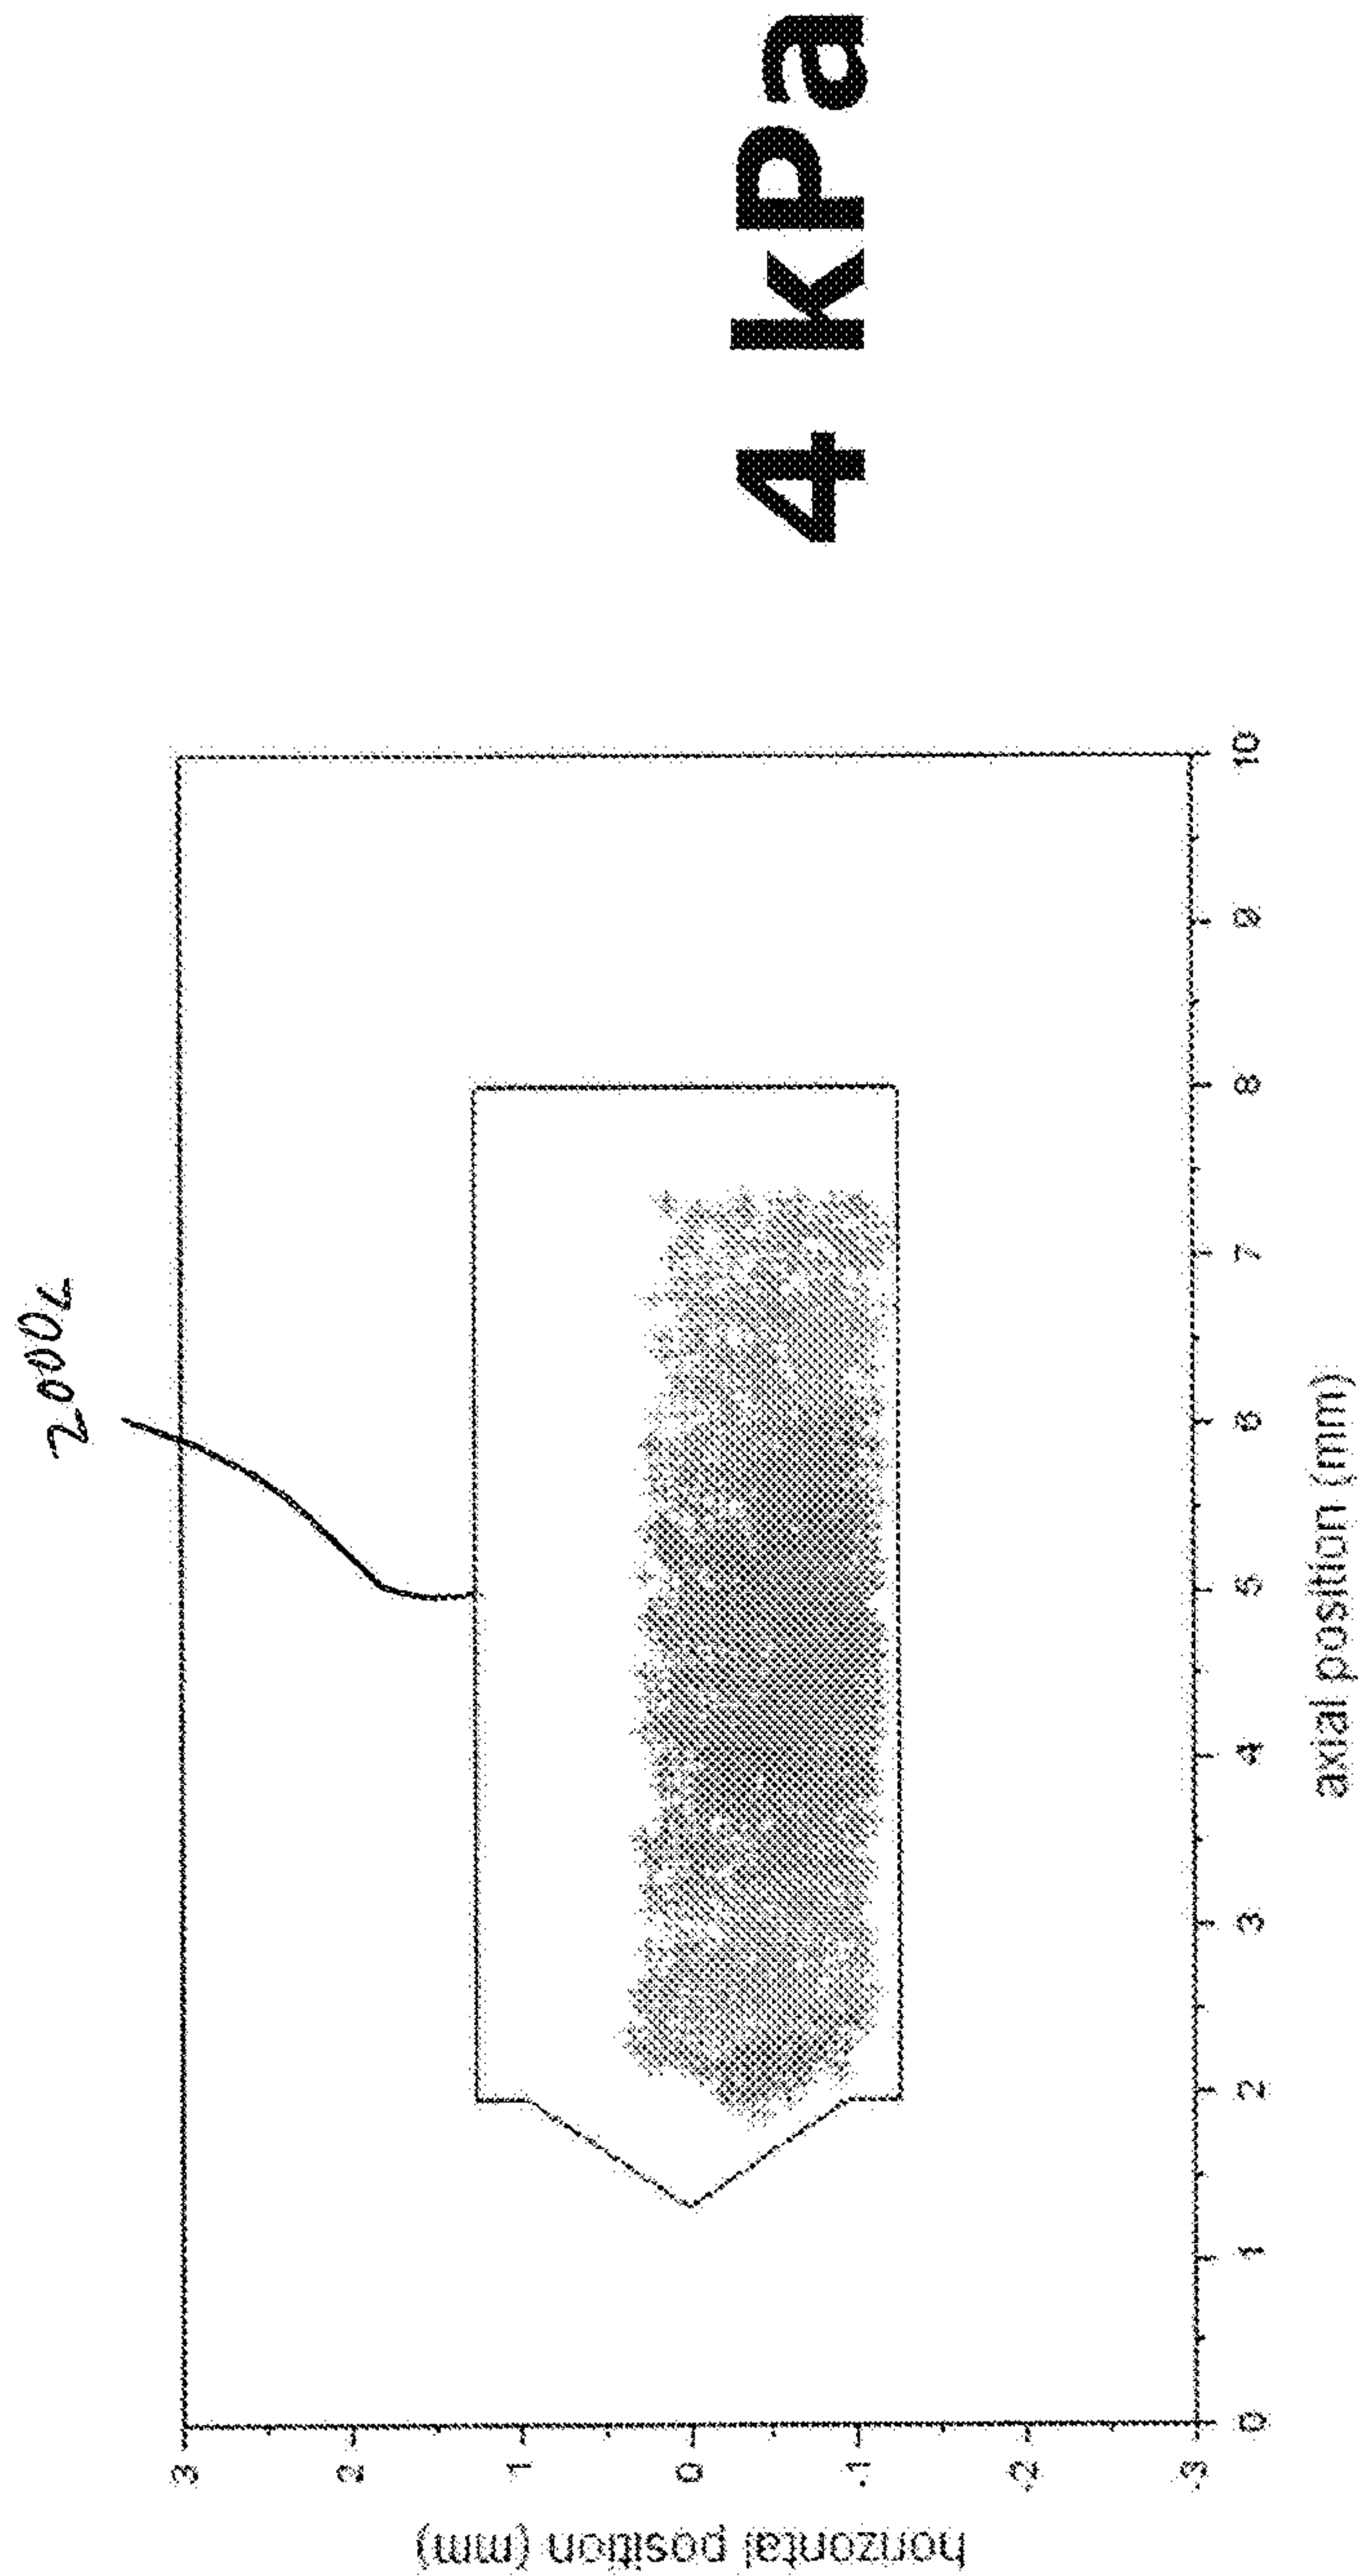

24/31

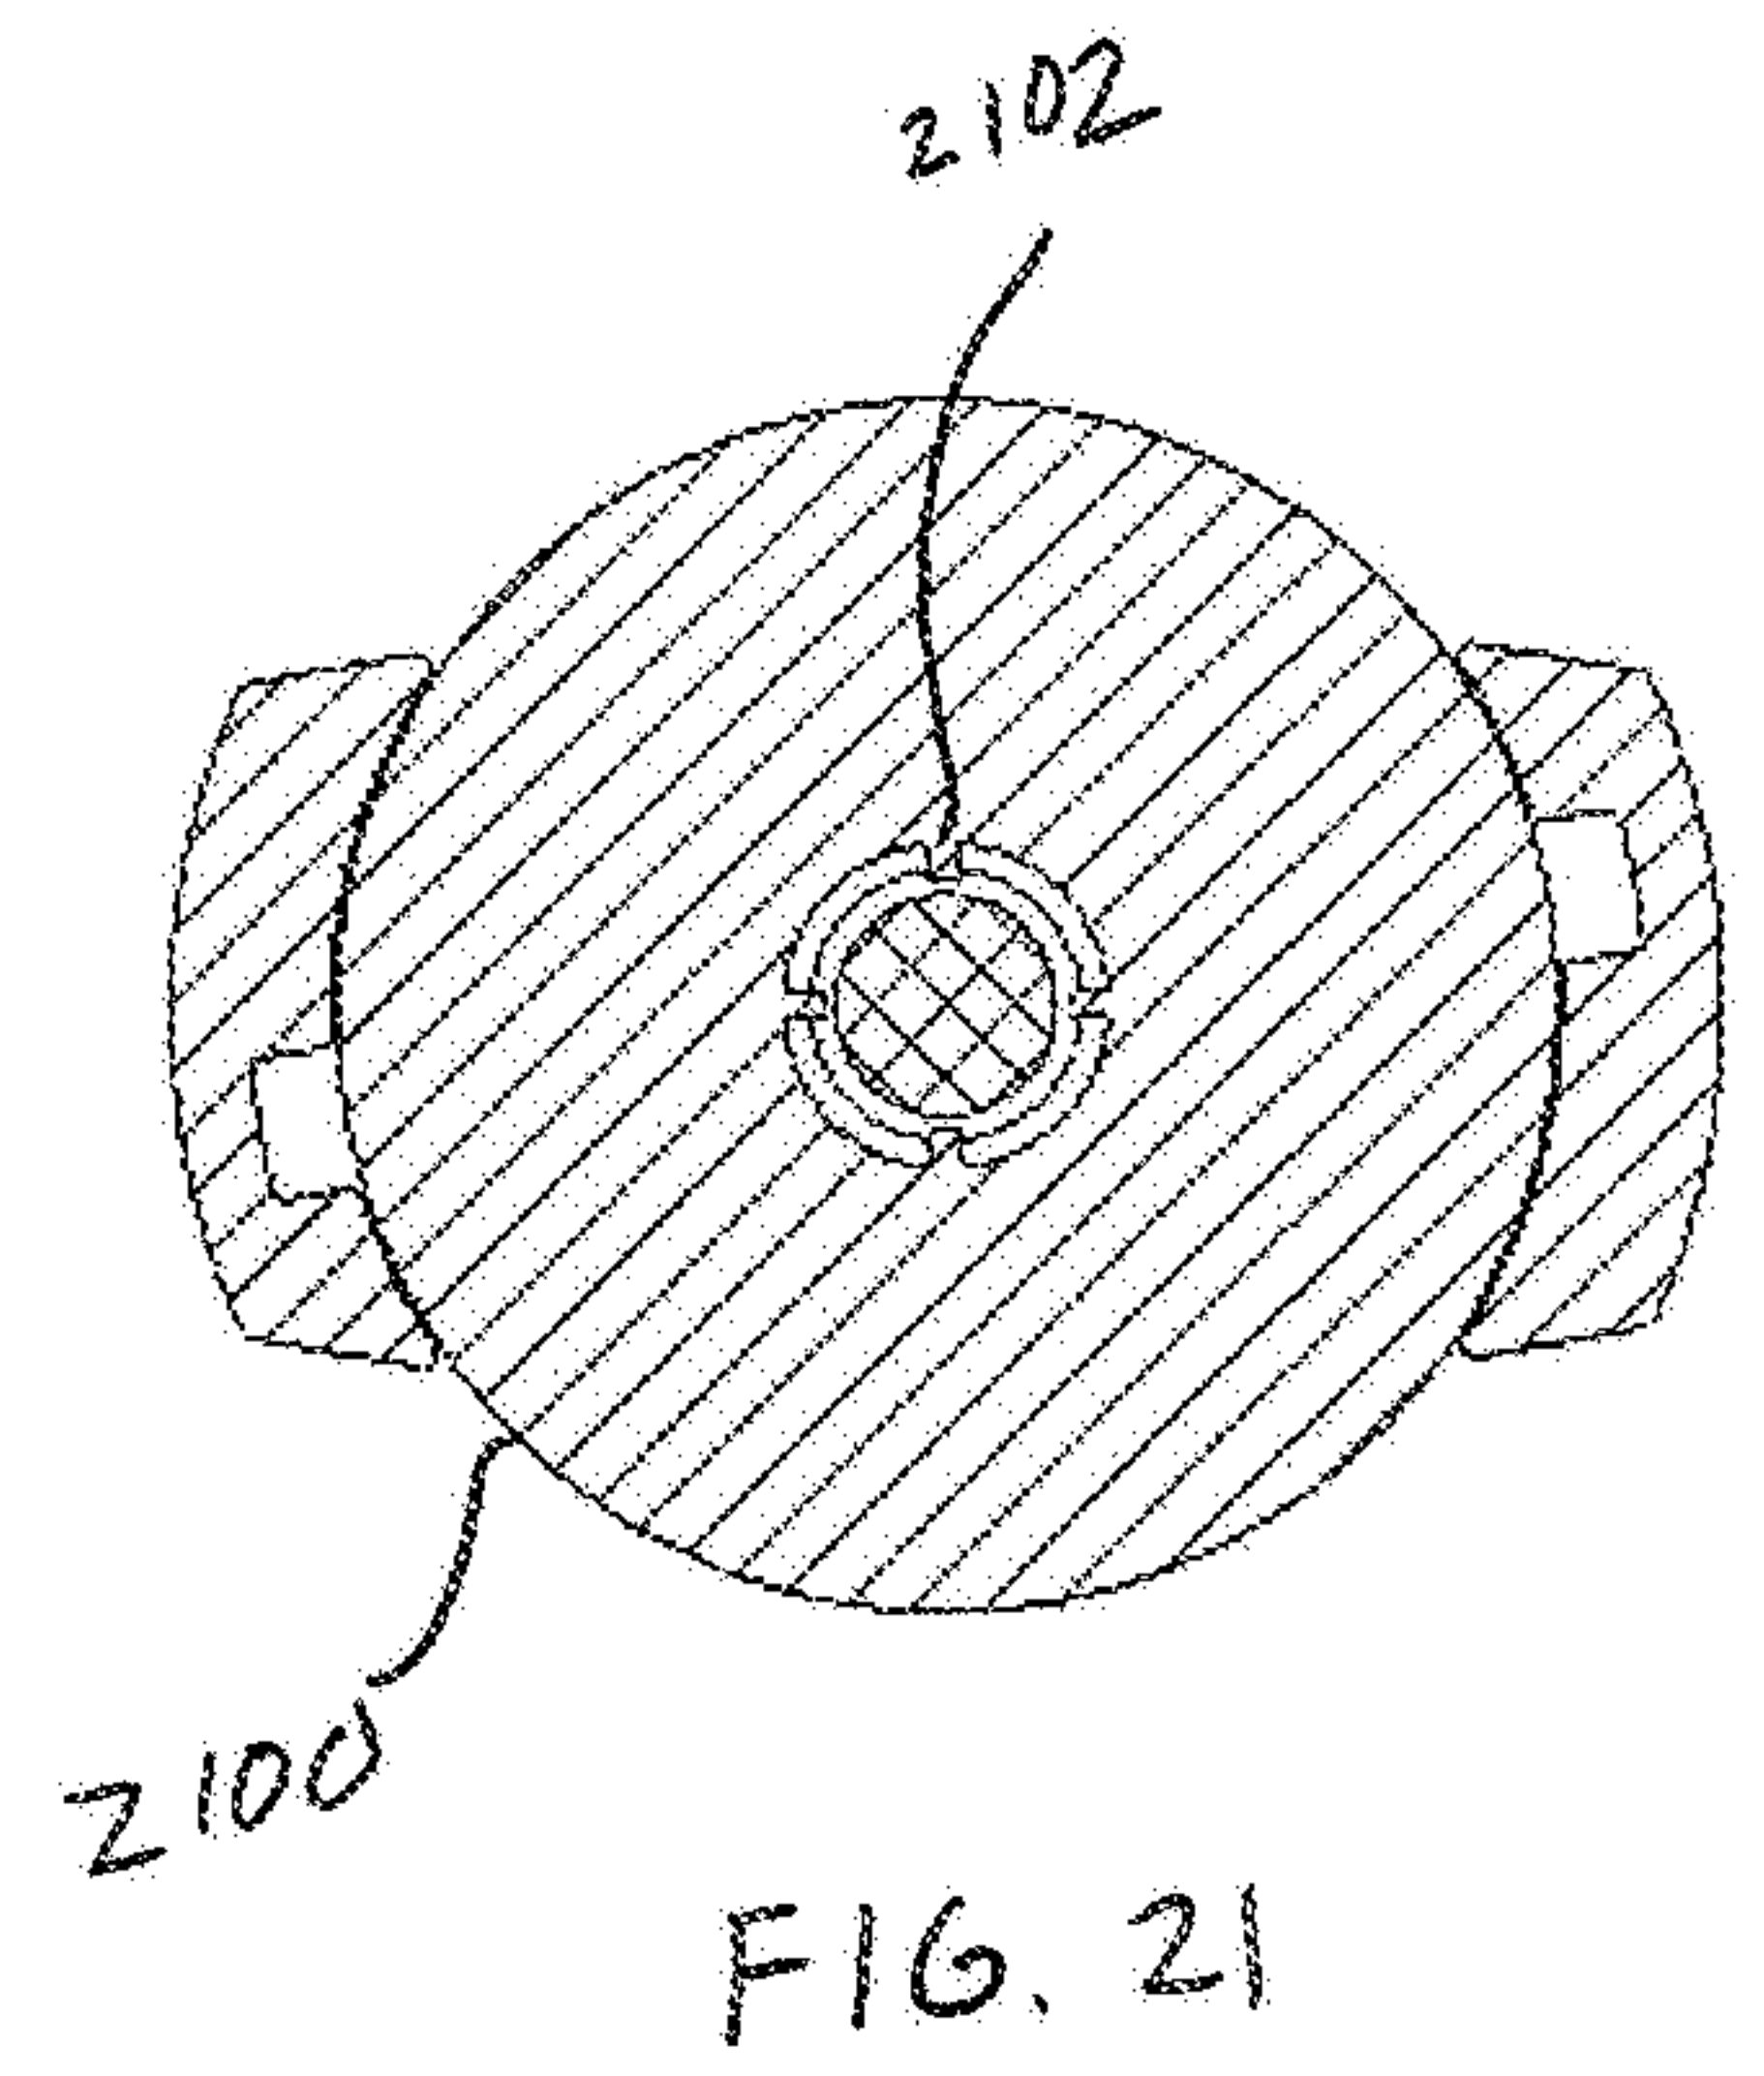

25/31

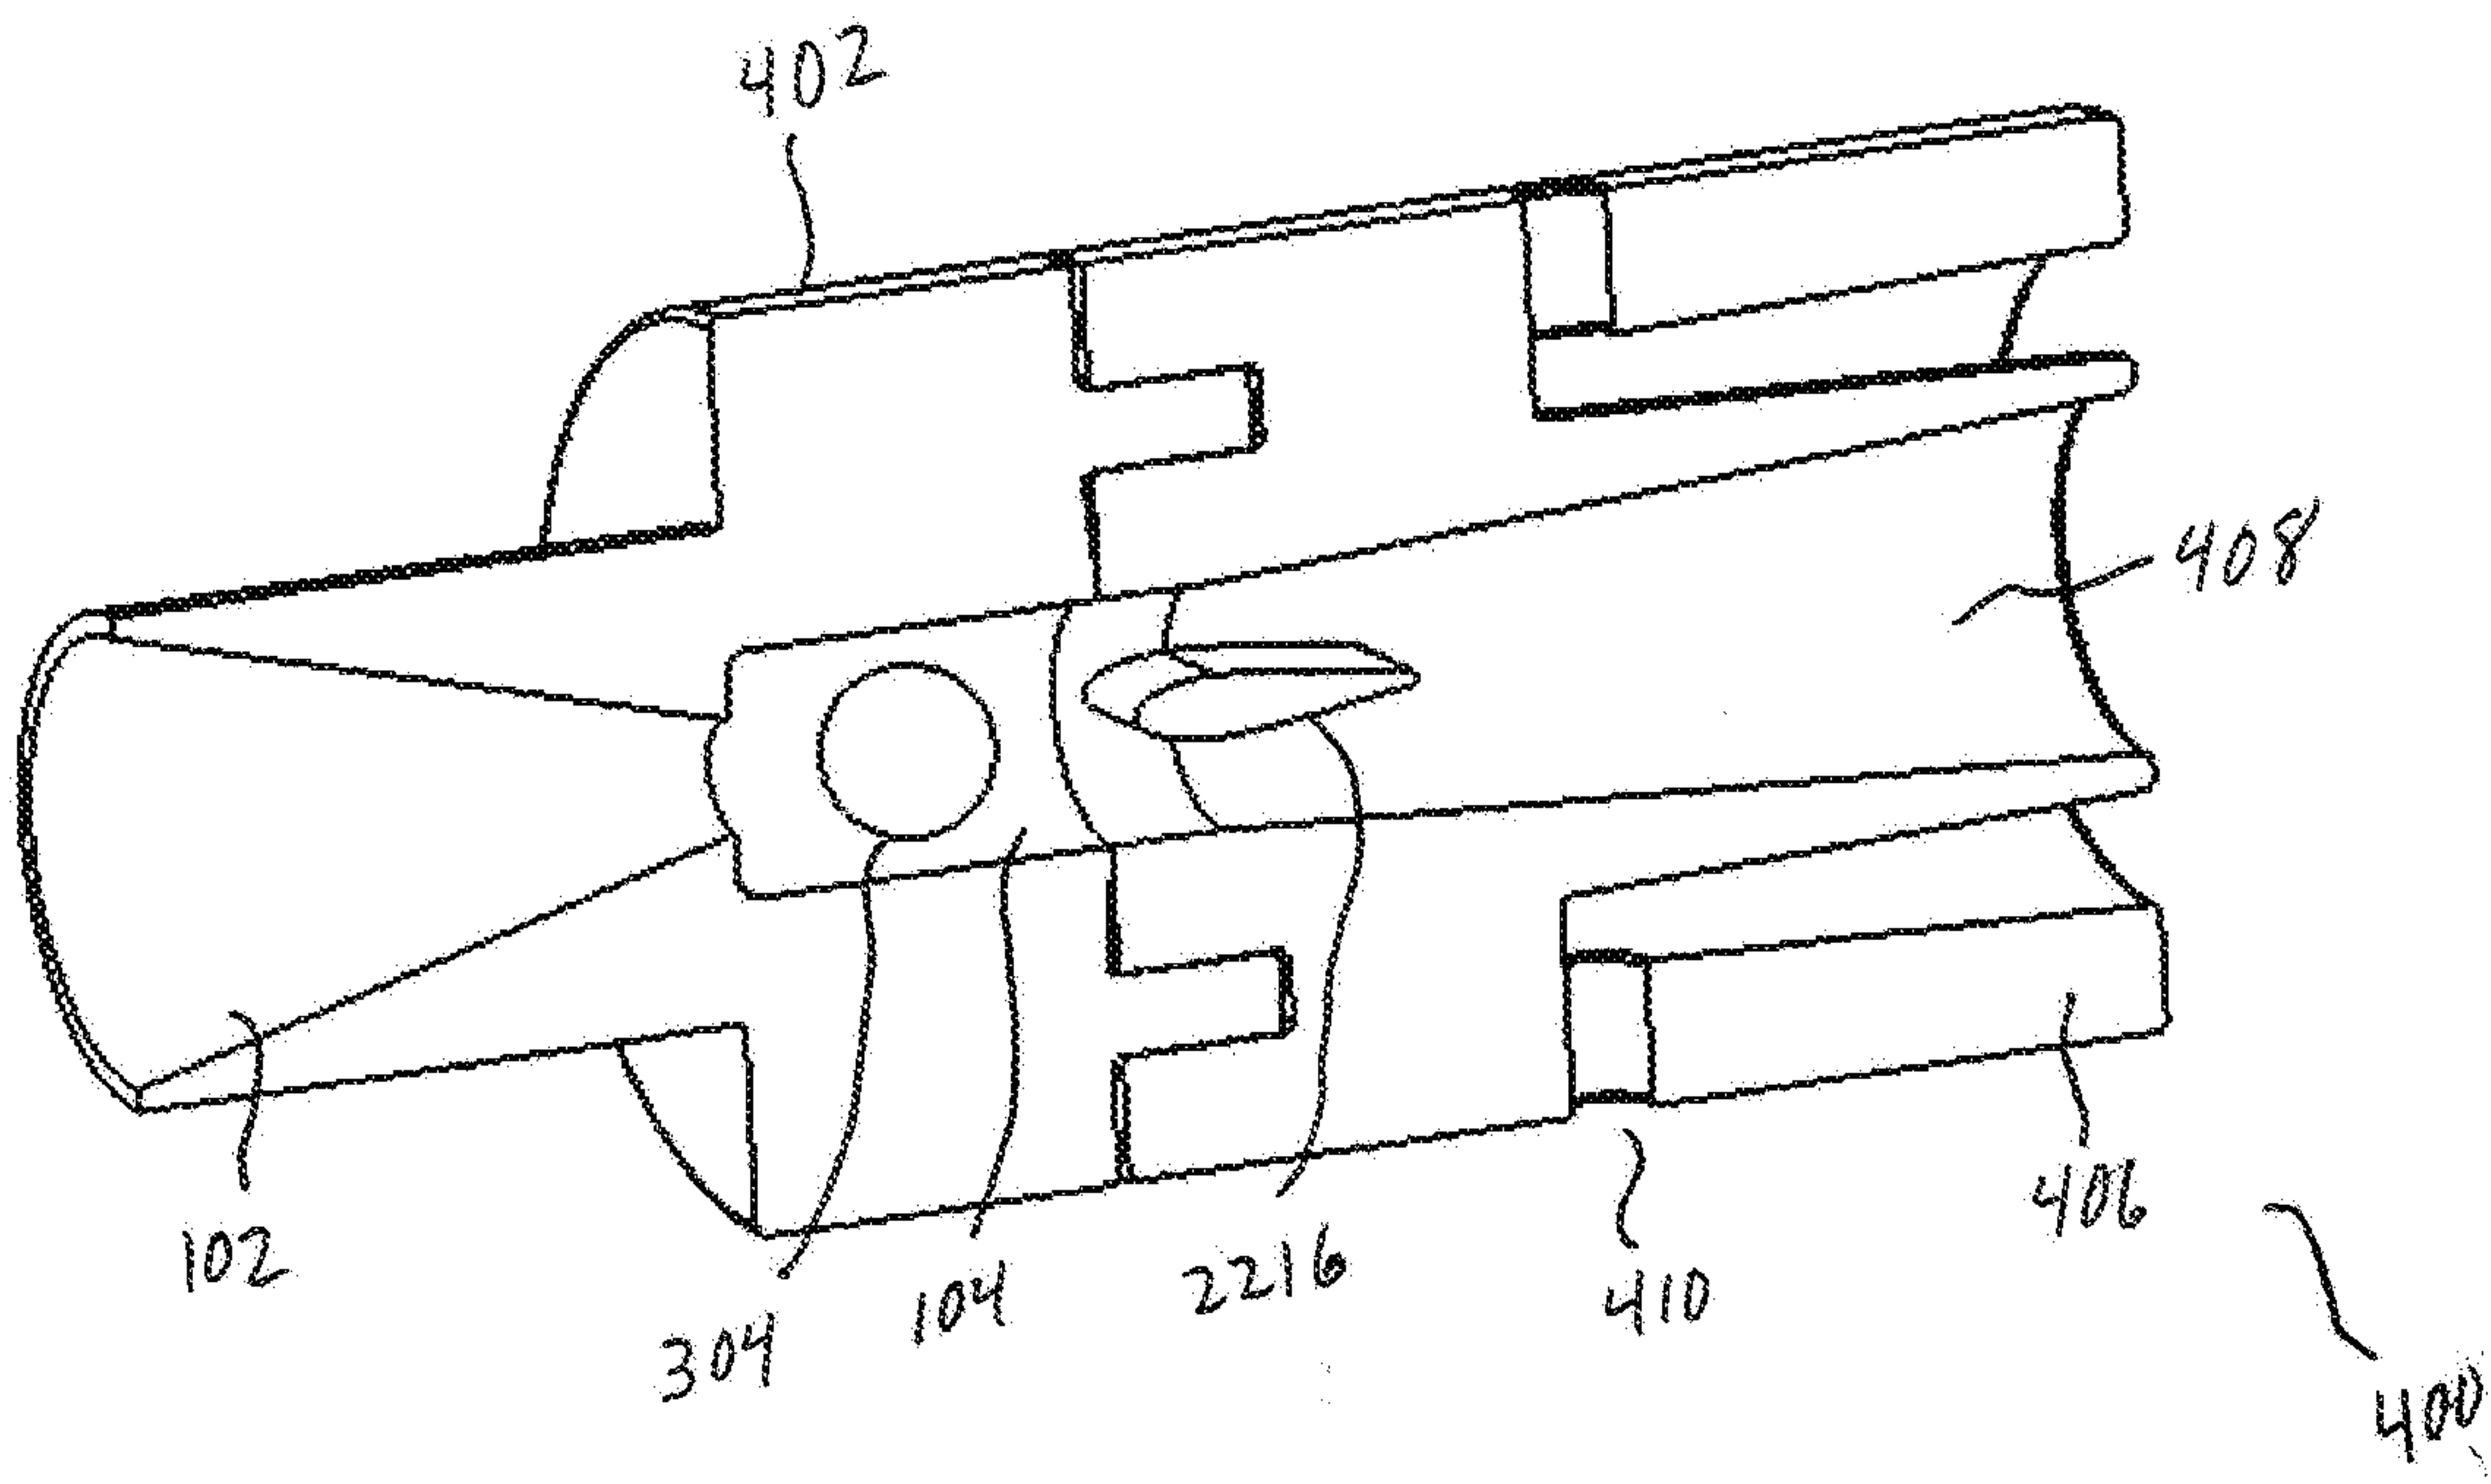


FIG. 22

26/31

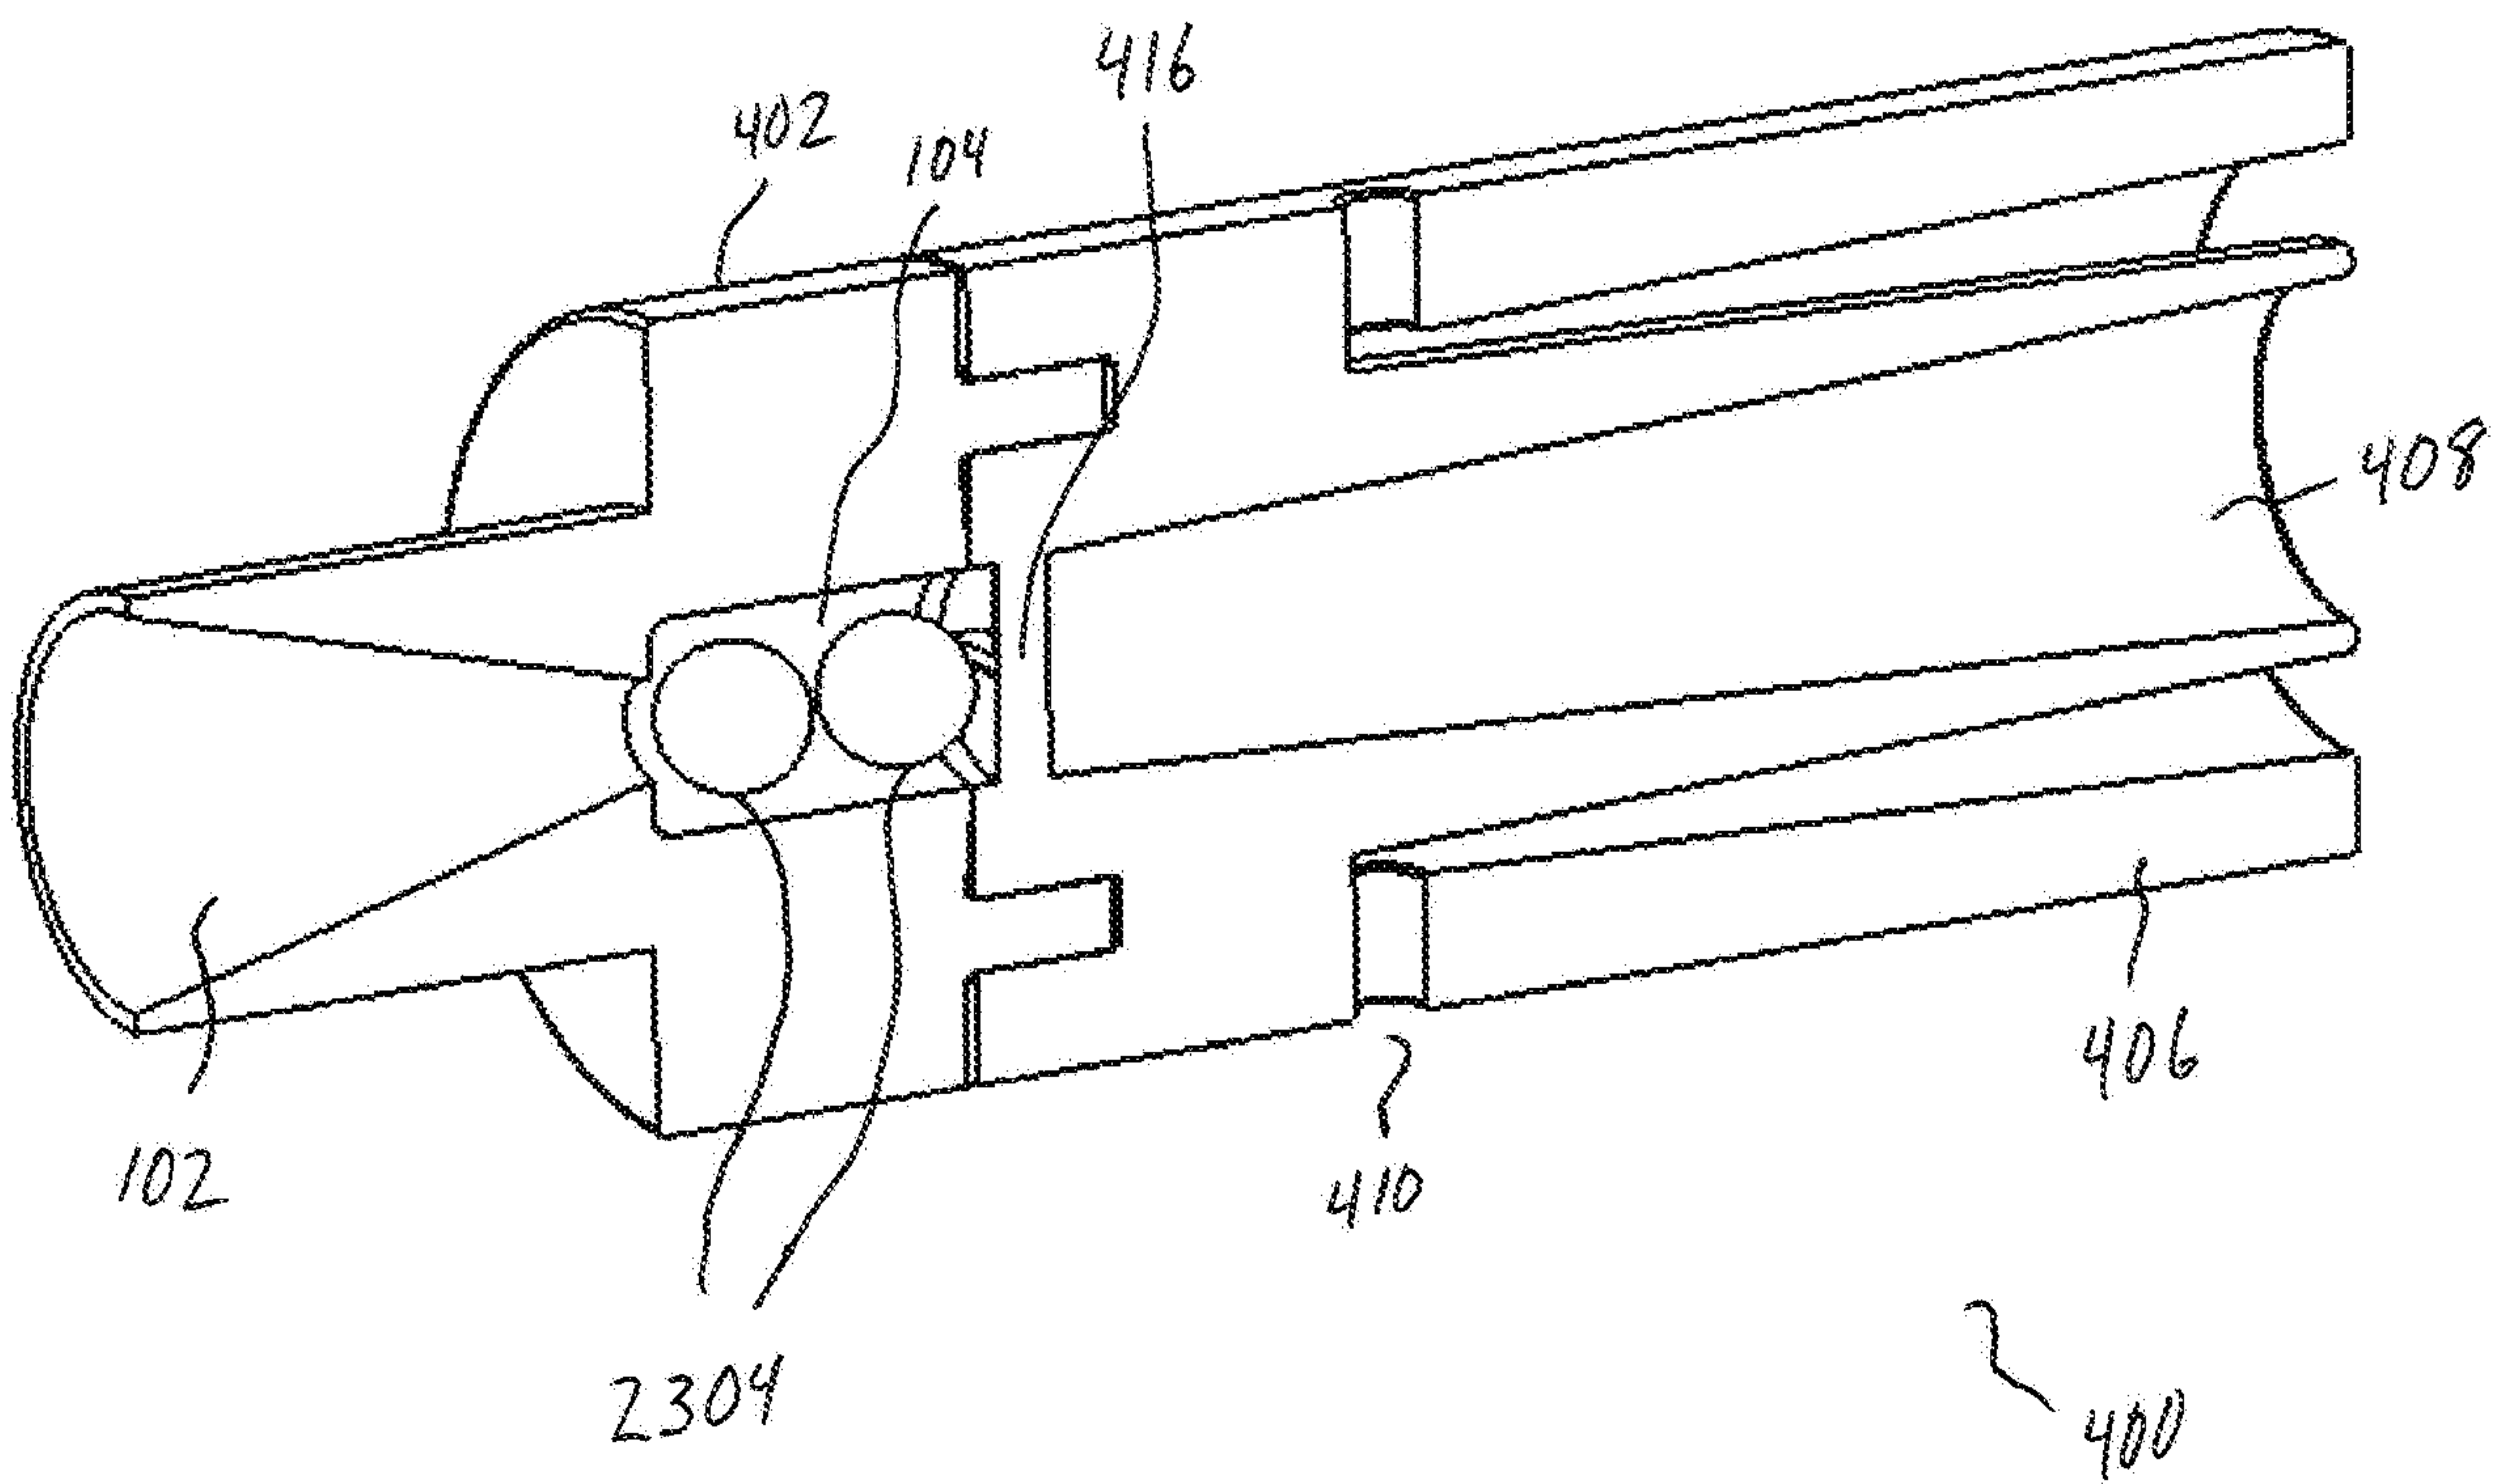


FIG. 23

27/31


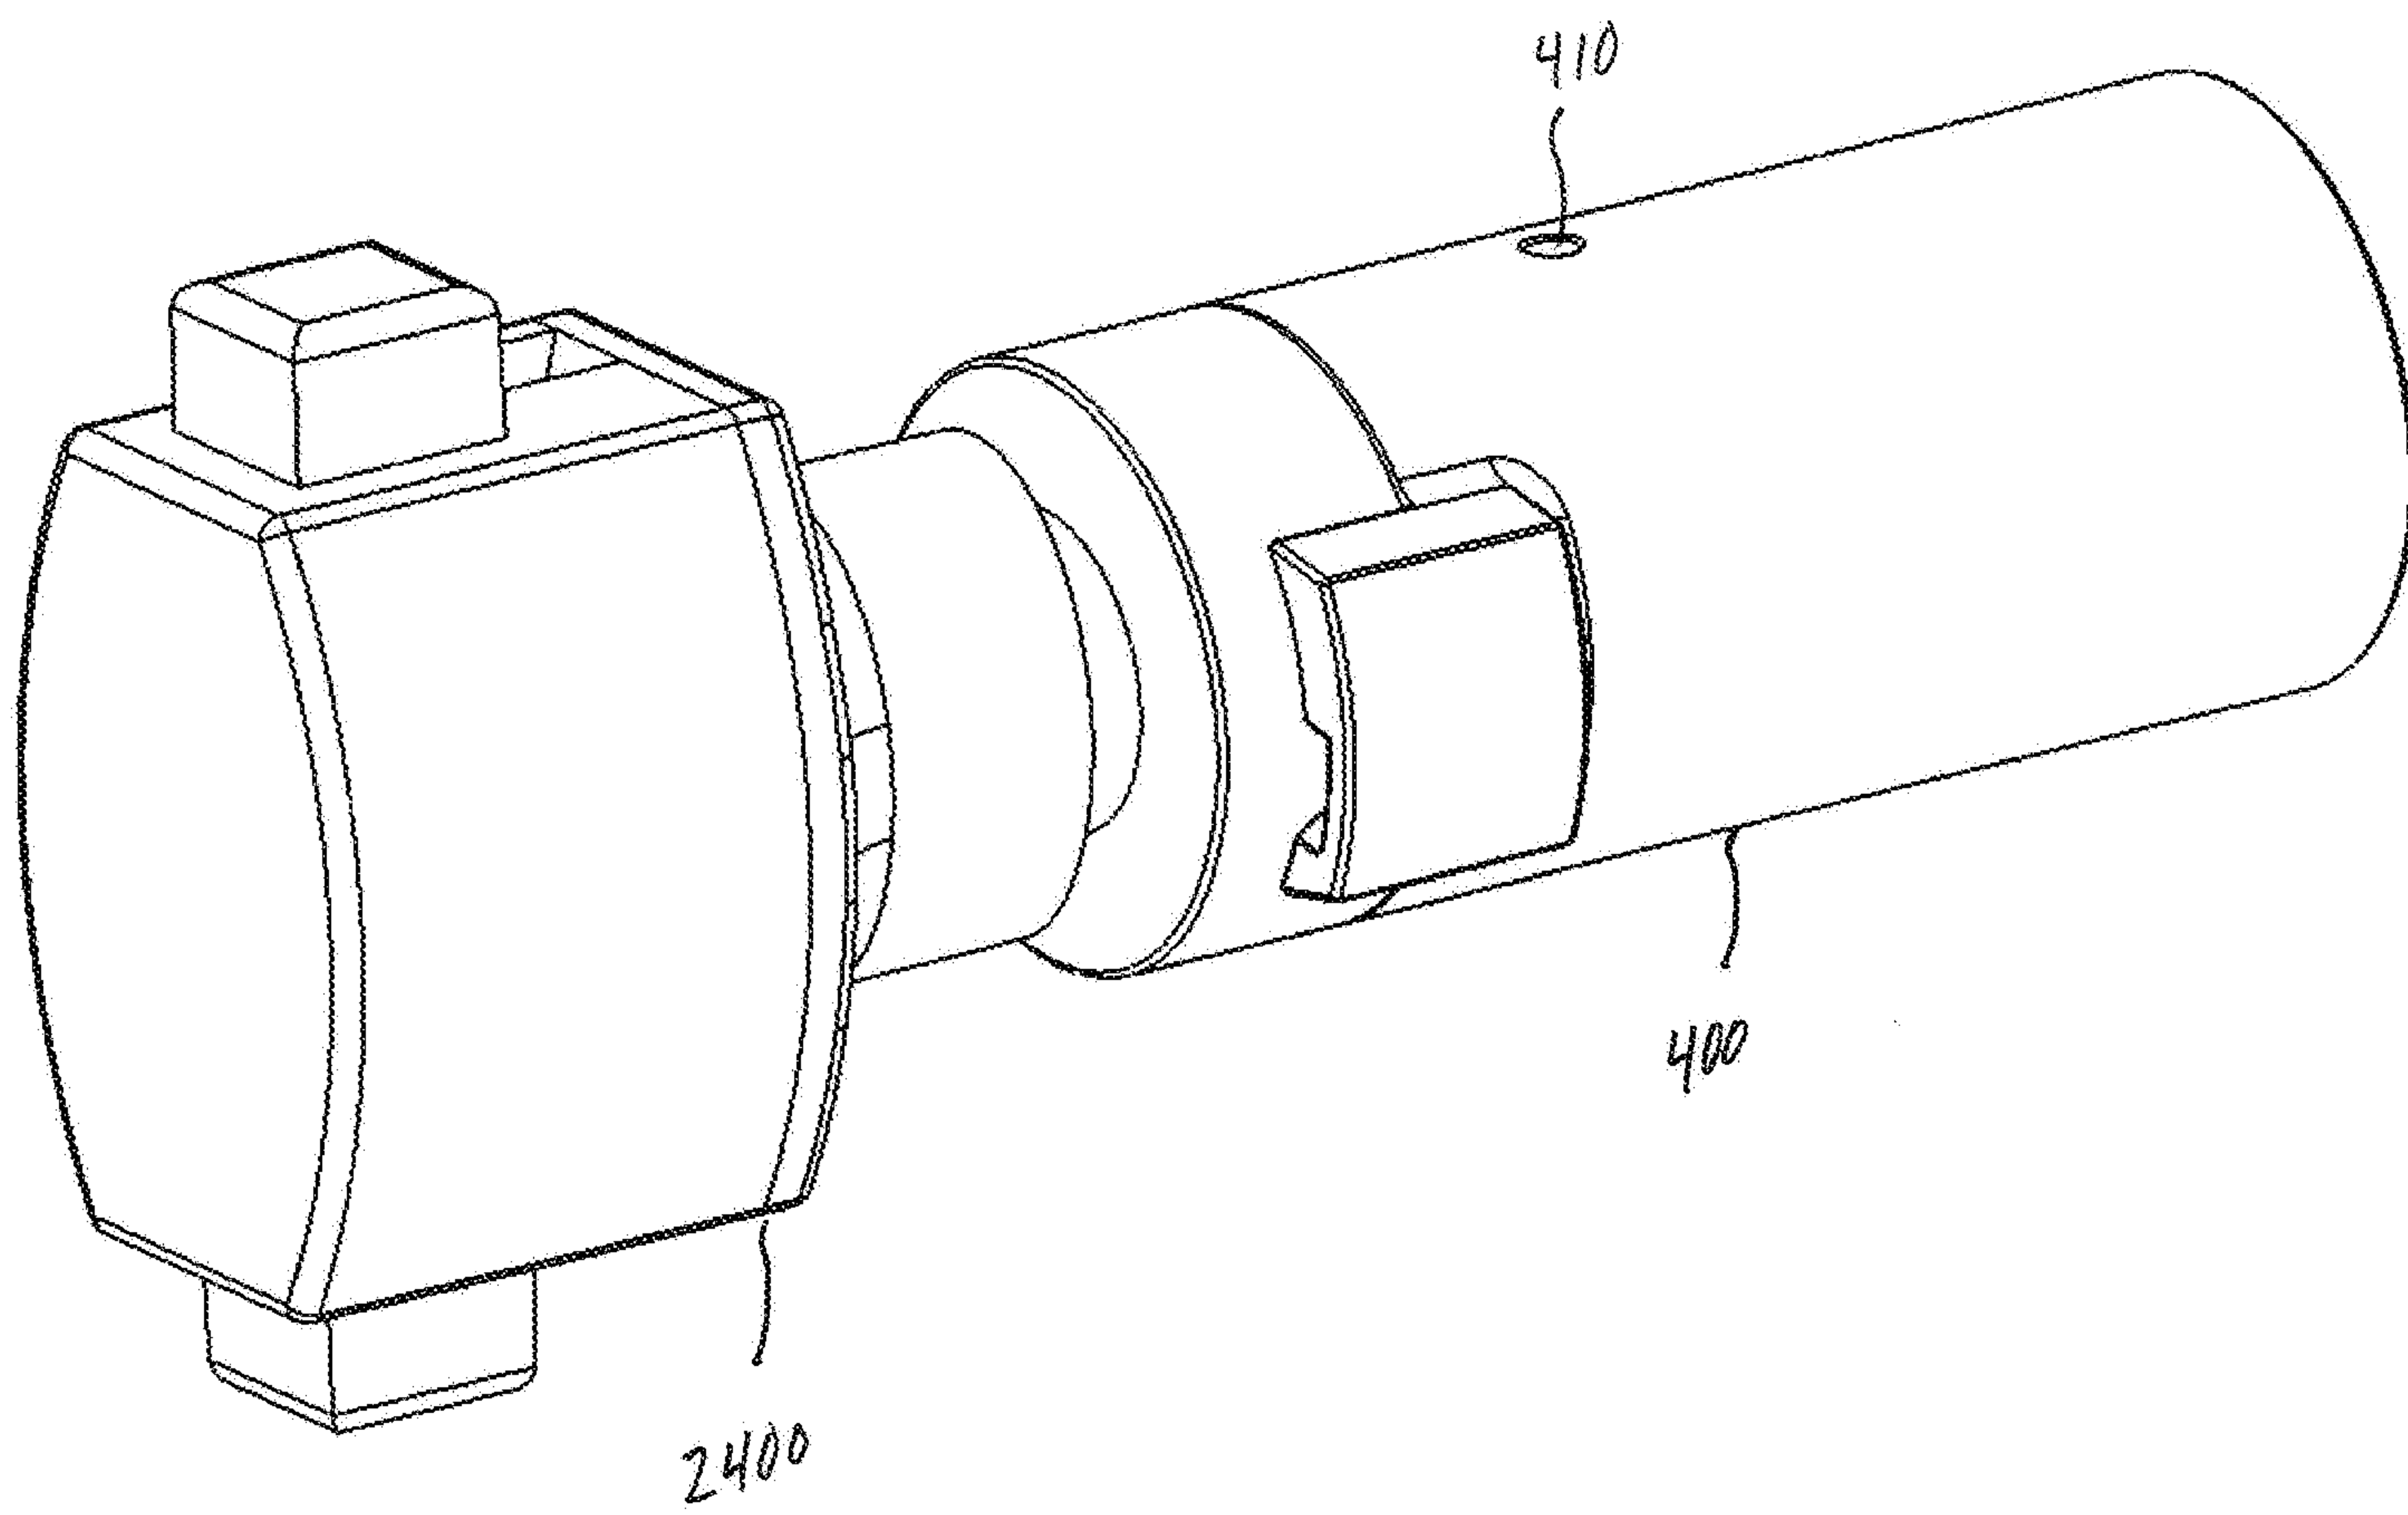


FIG. 24

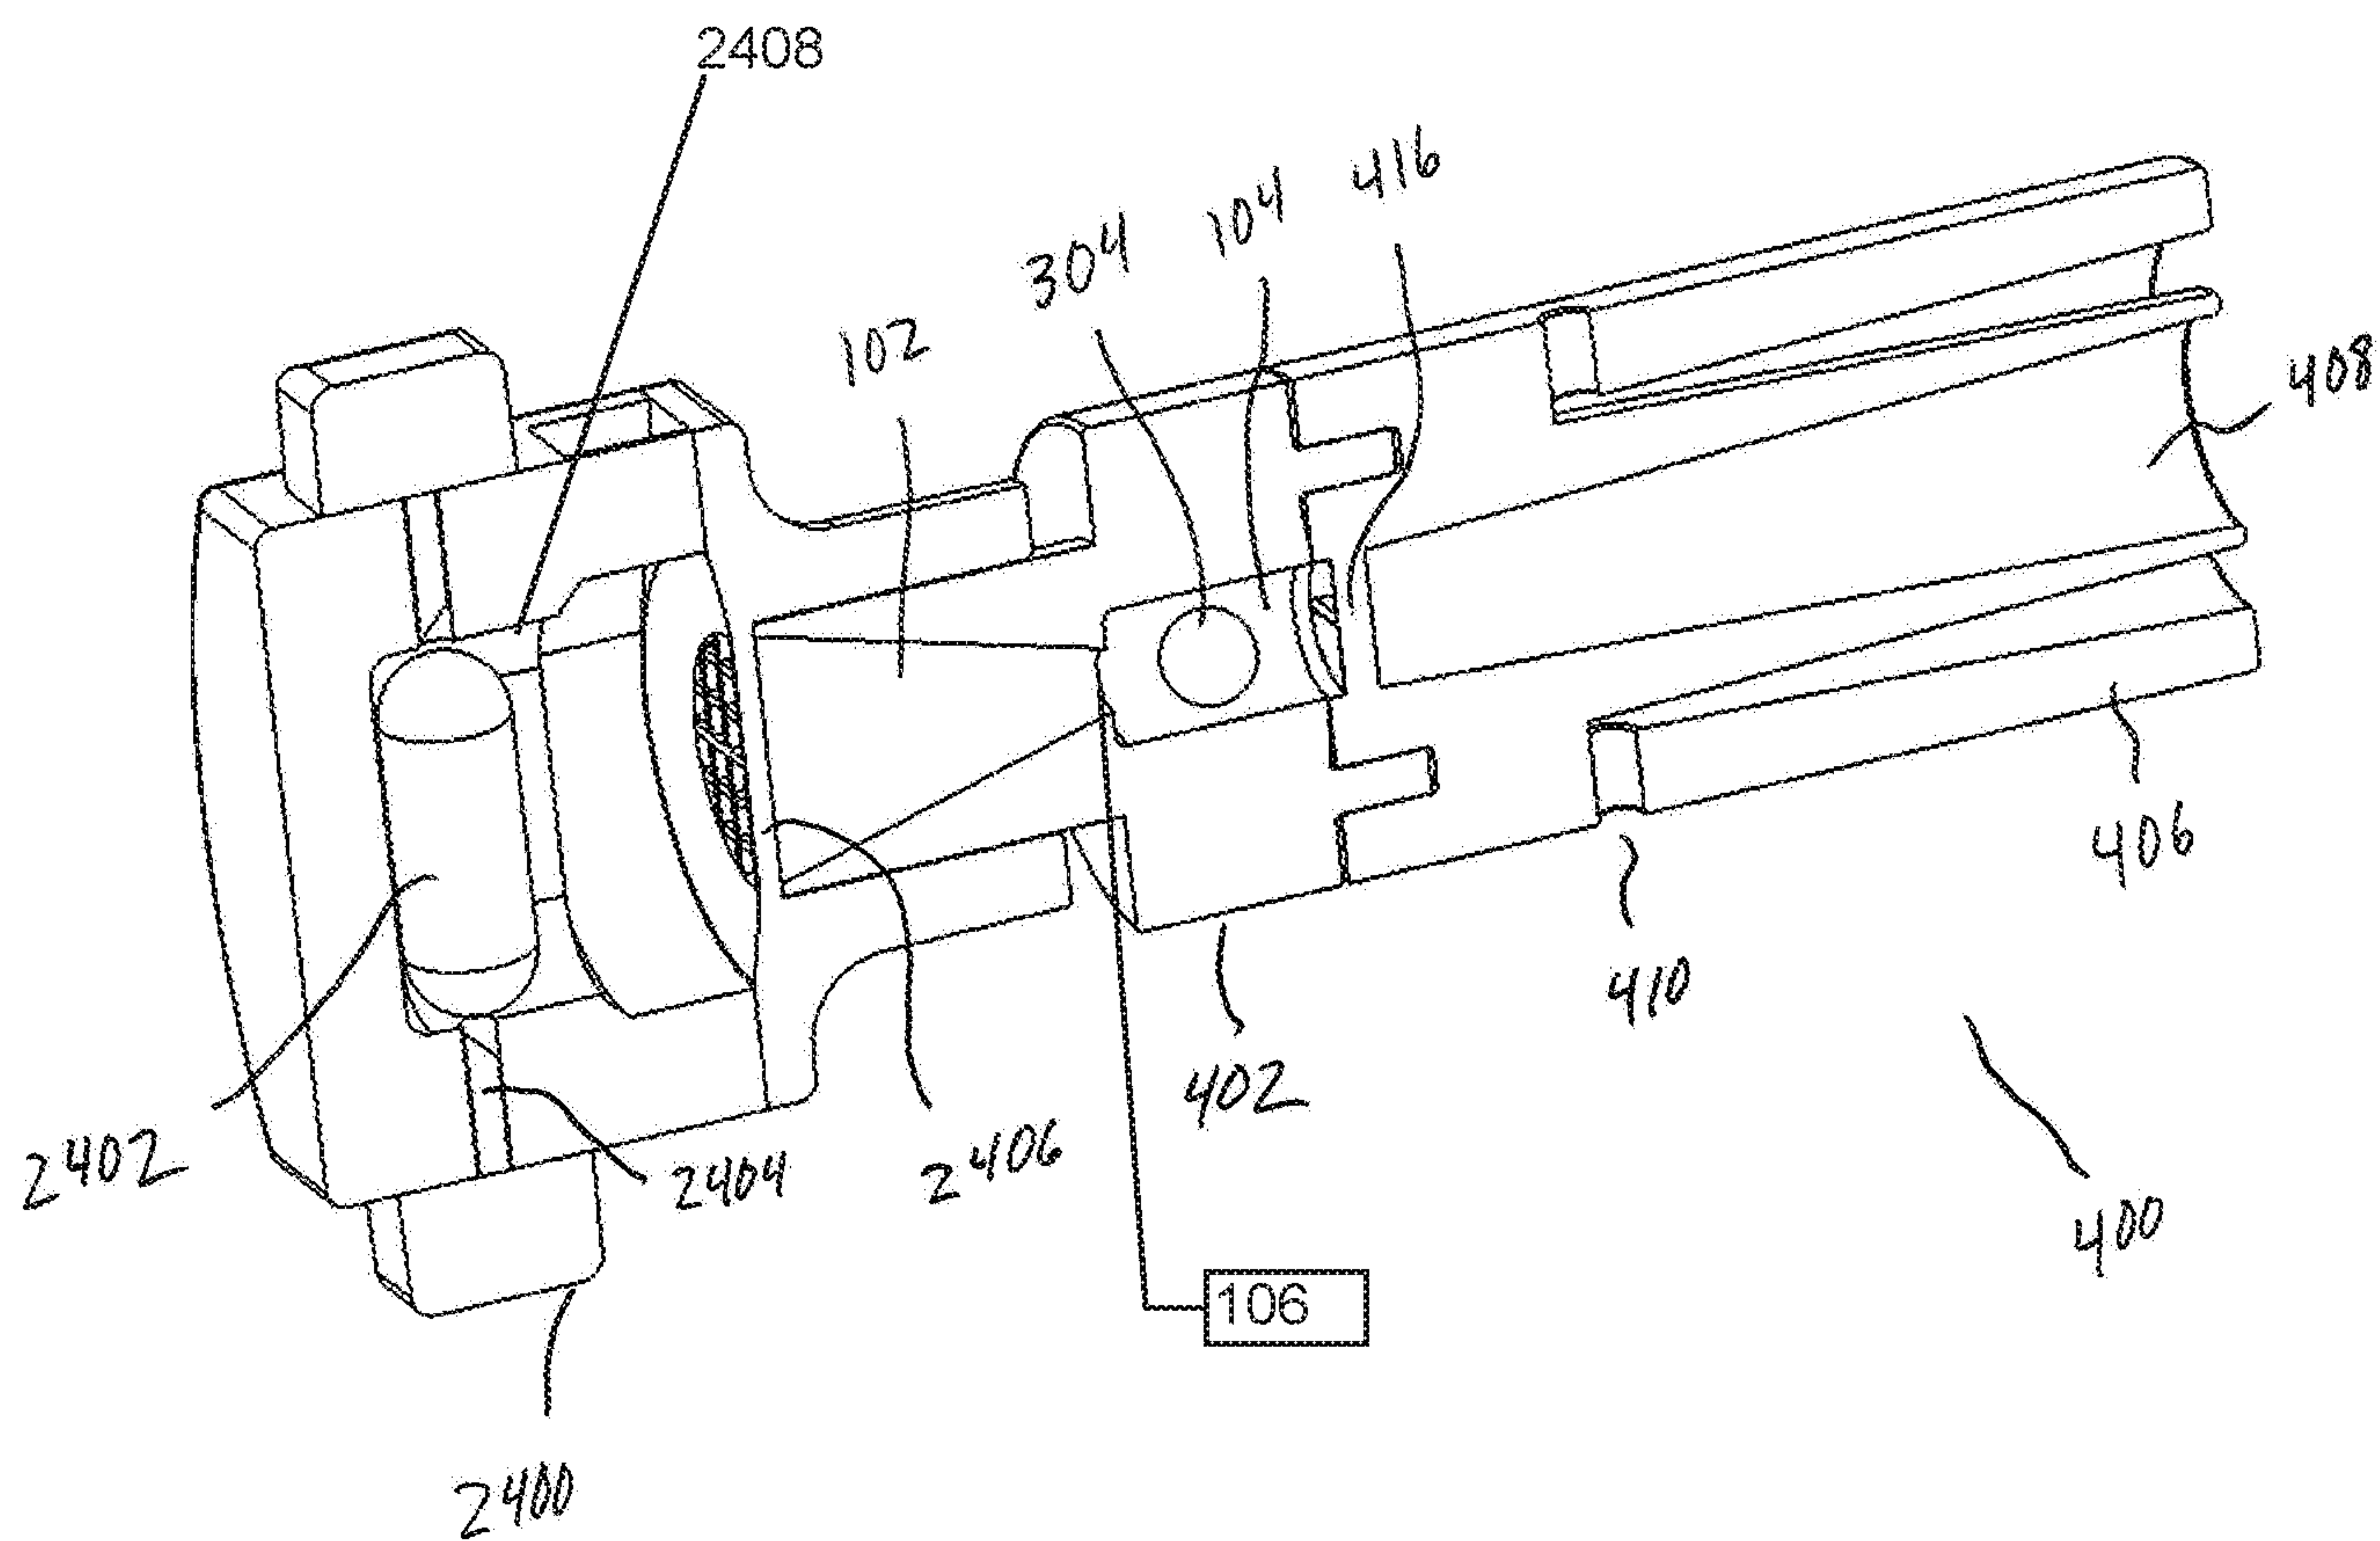

29/31

Summary of 20%Var(HCl)2-Inhalac250 Plastiapex-AB Aerosol Performance

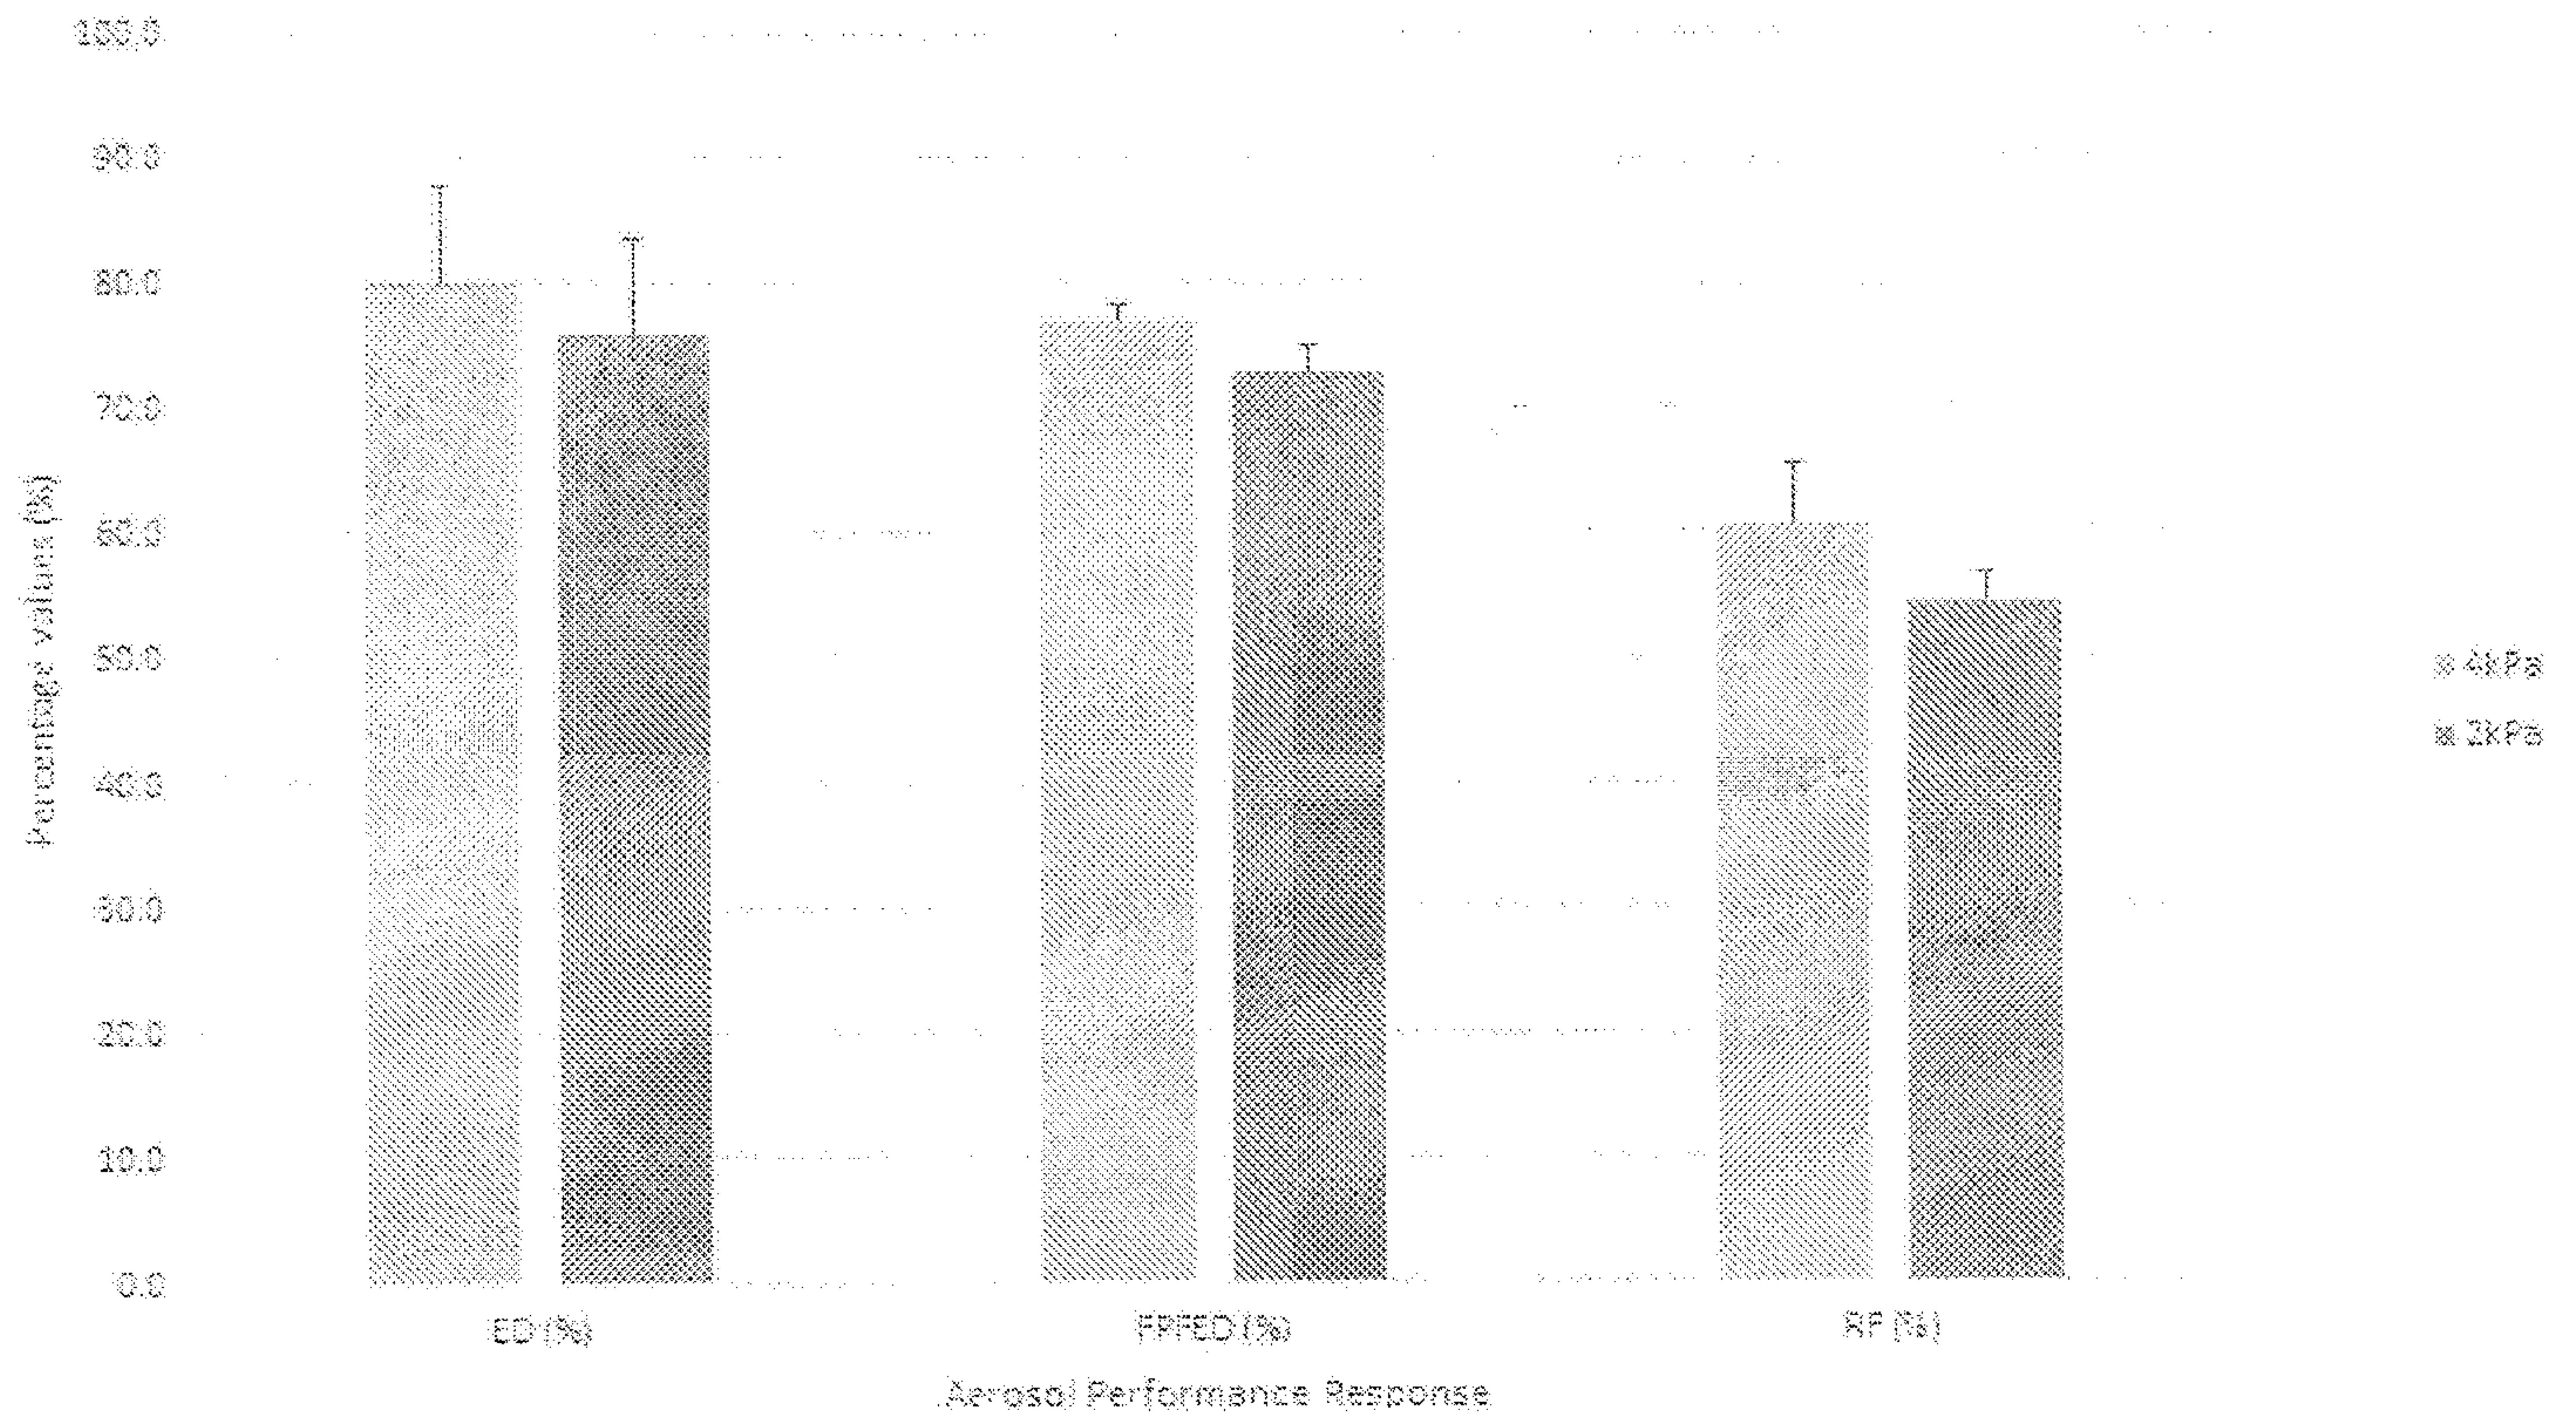


FIG. 26

30/31

P-AOS - Low vs High Flow Device Deposition

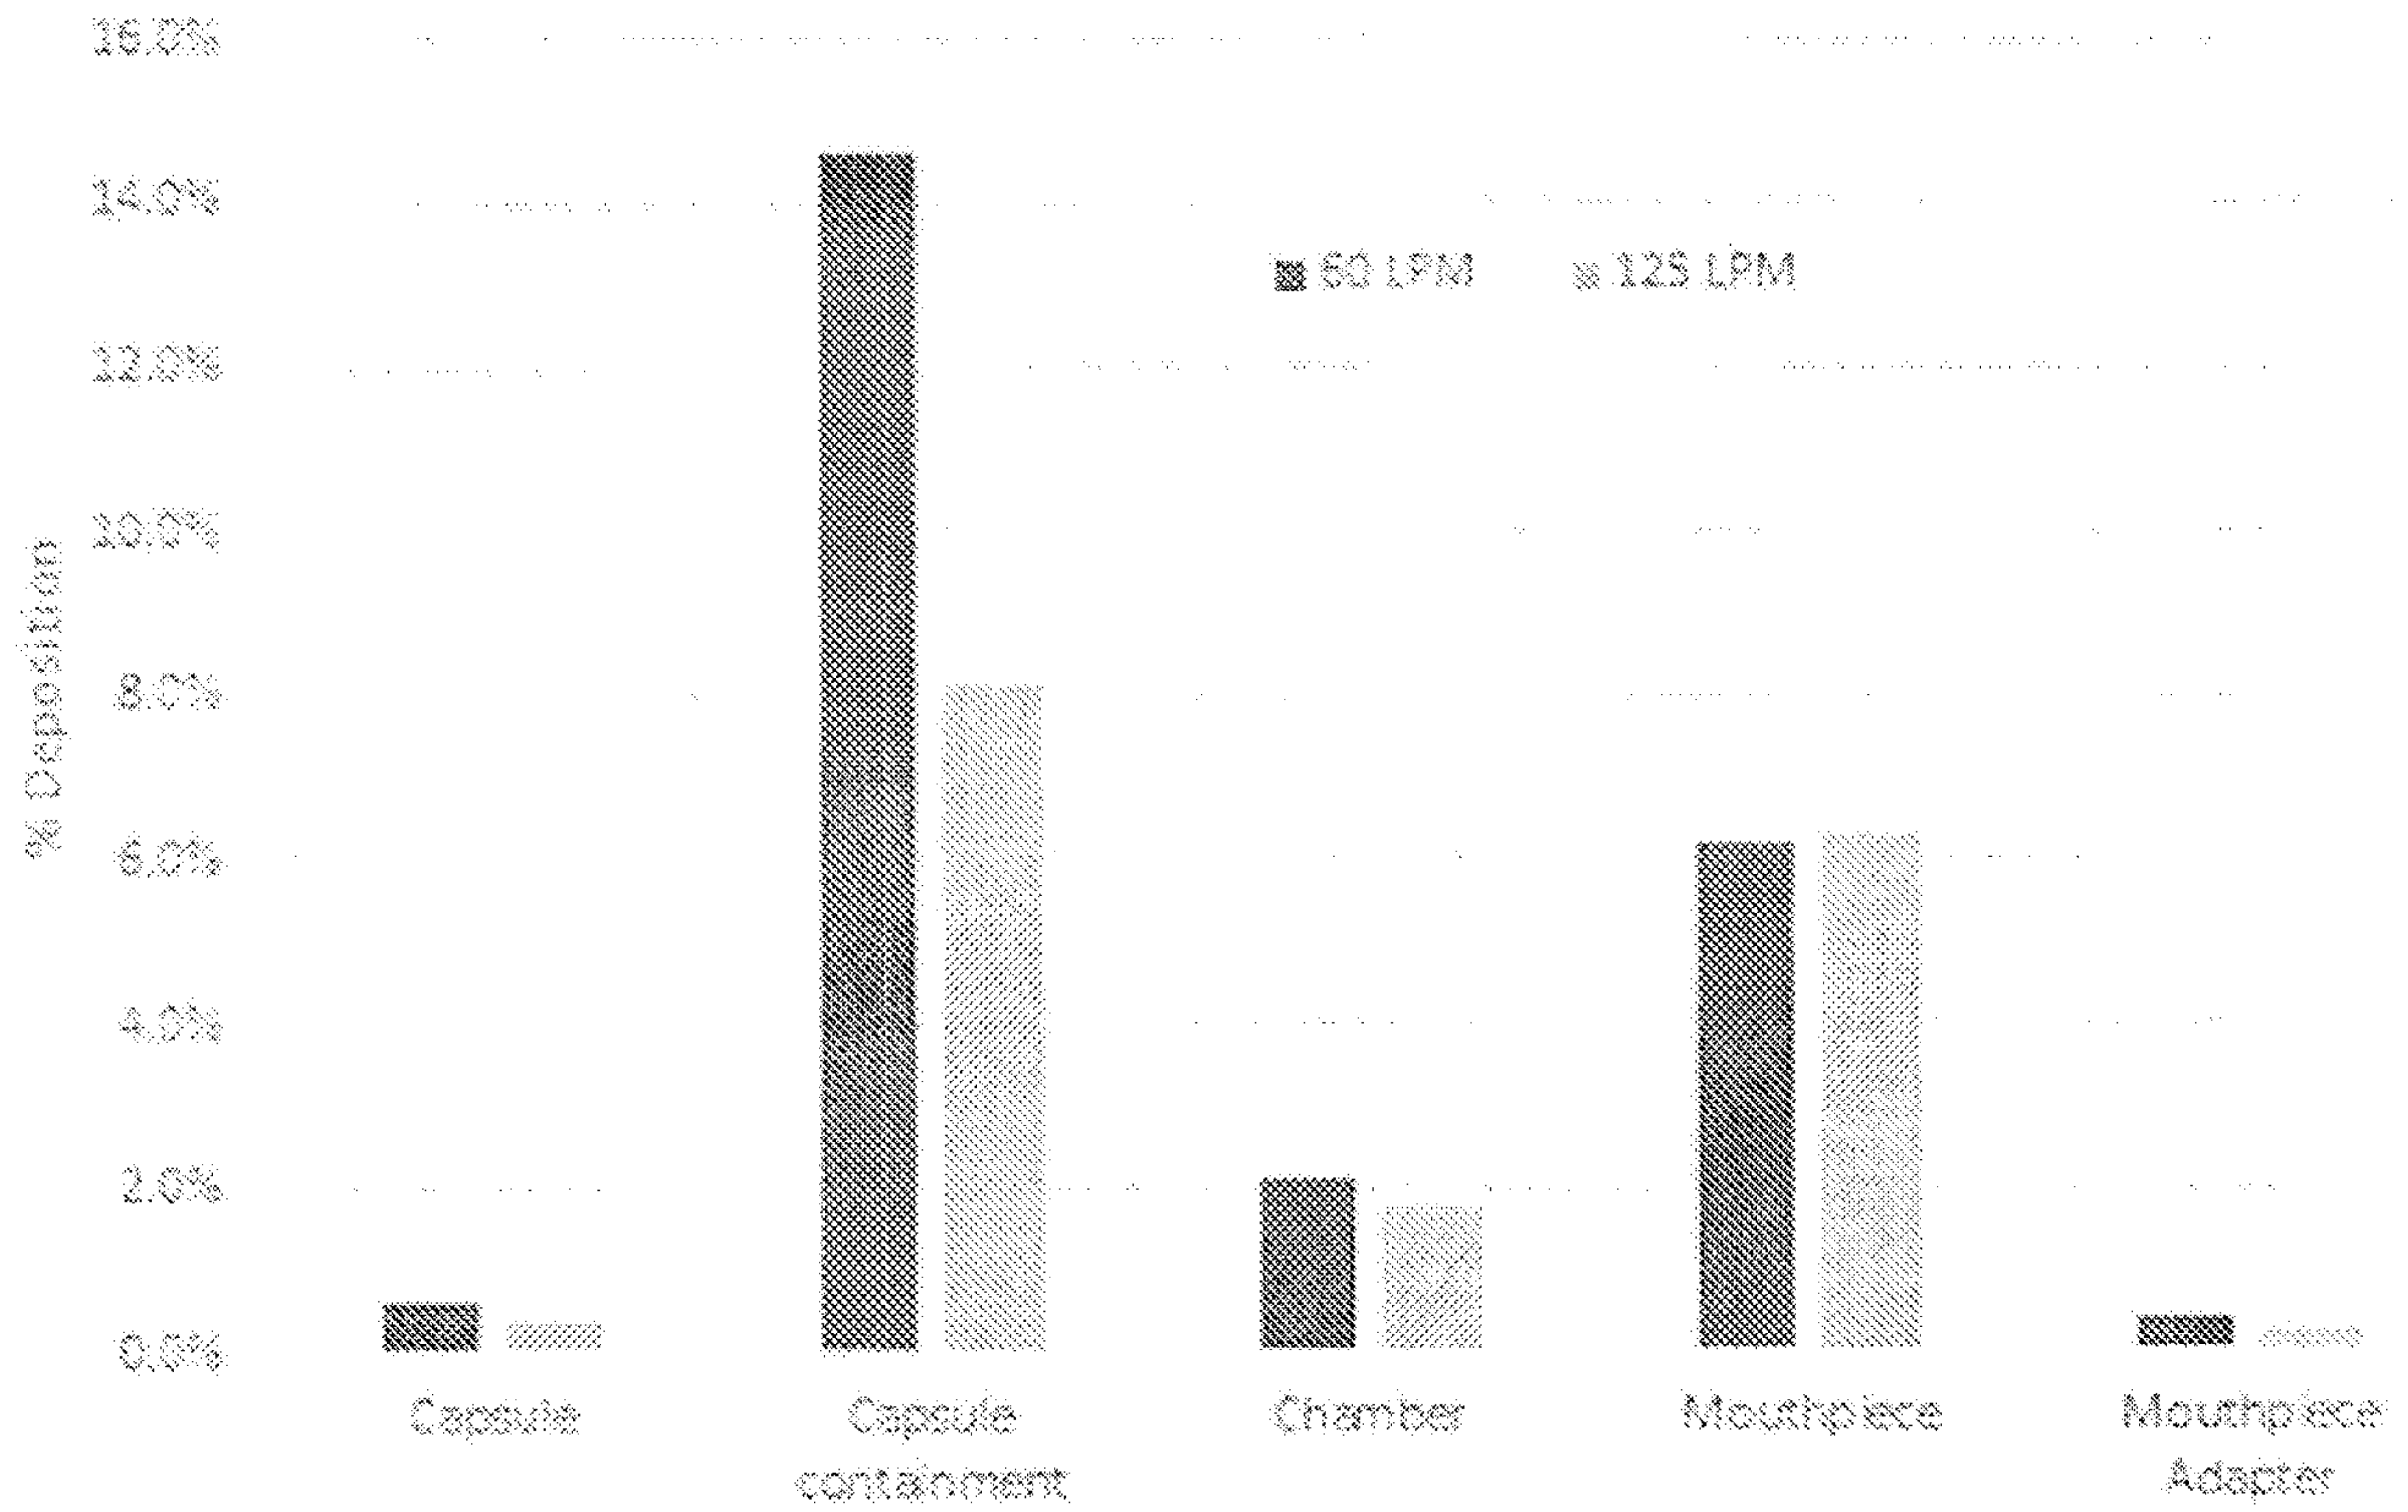


FIG. 27

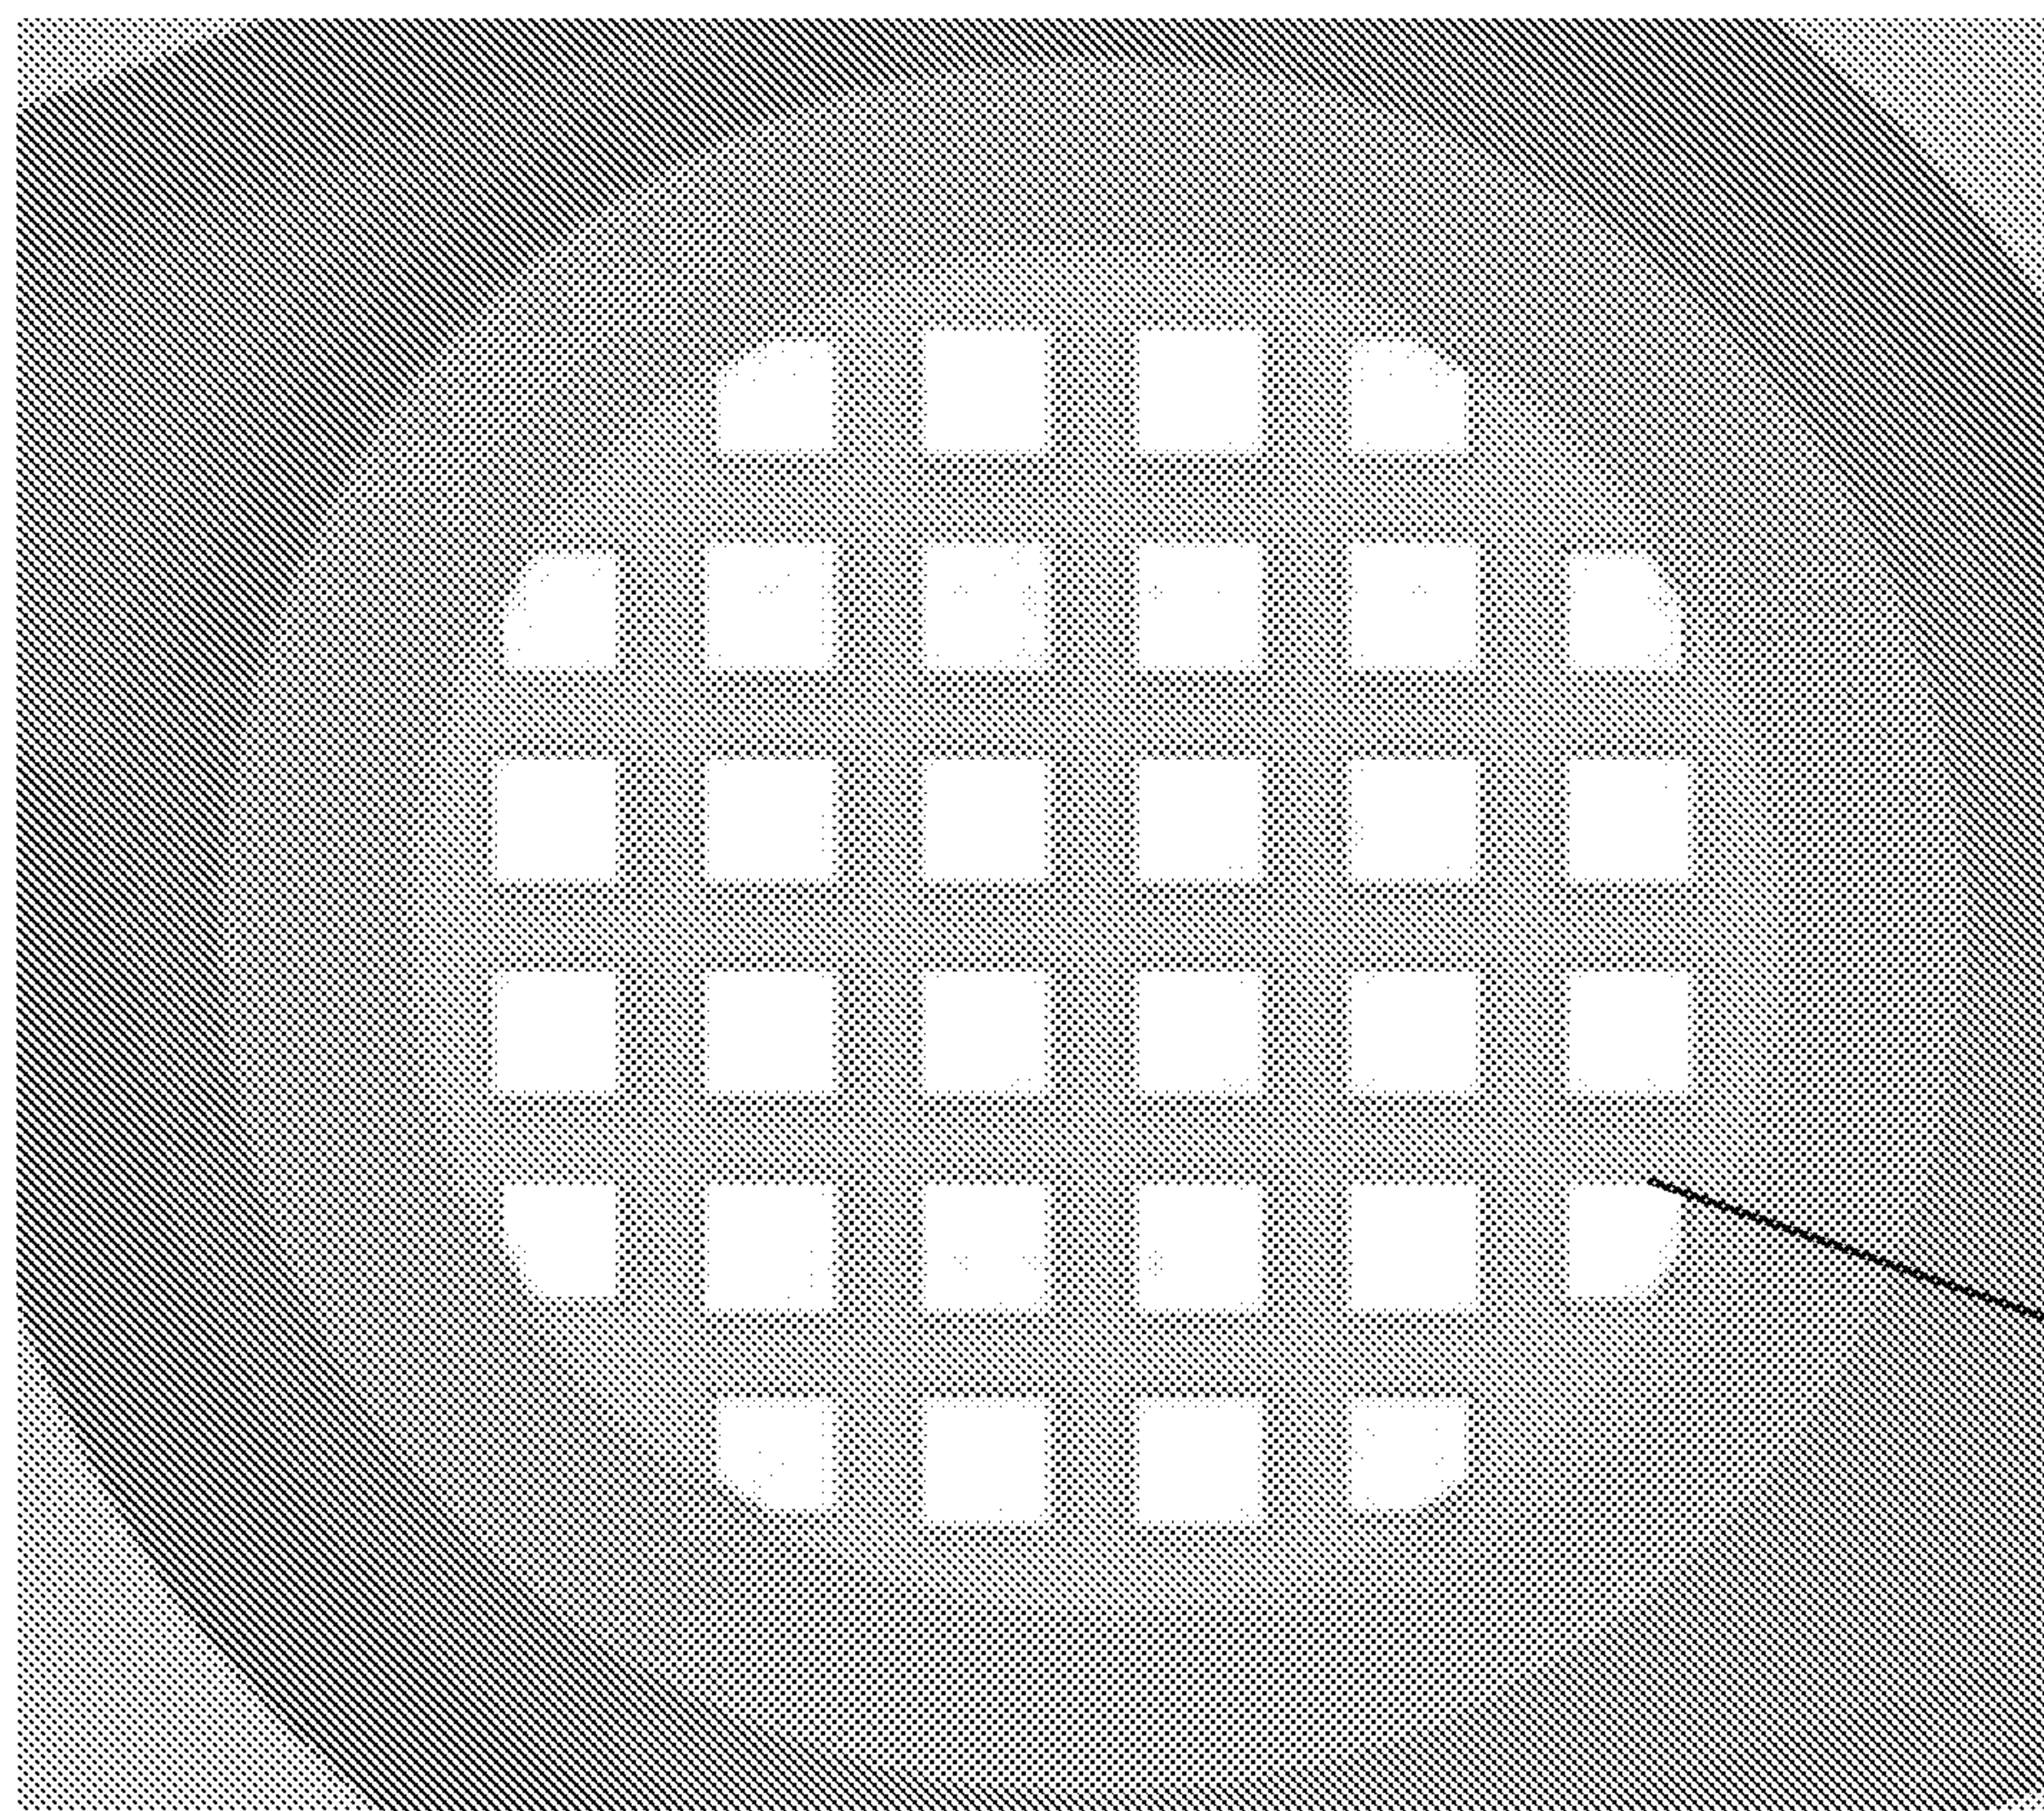


FIG. 28A

2800

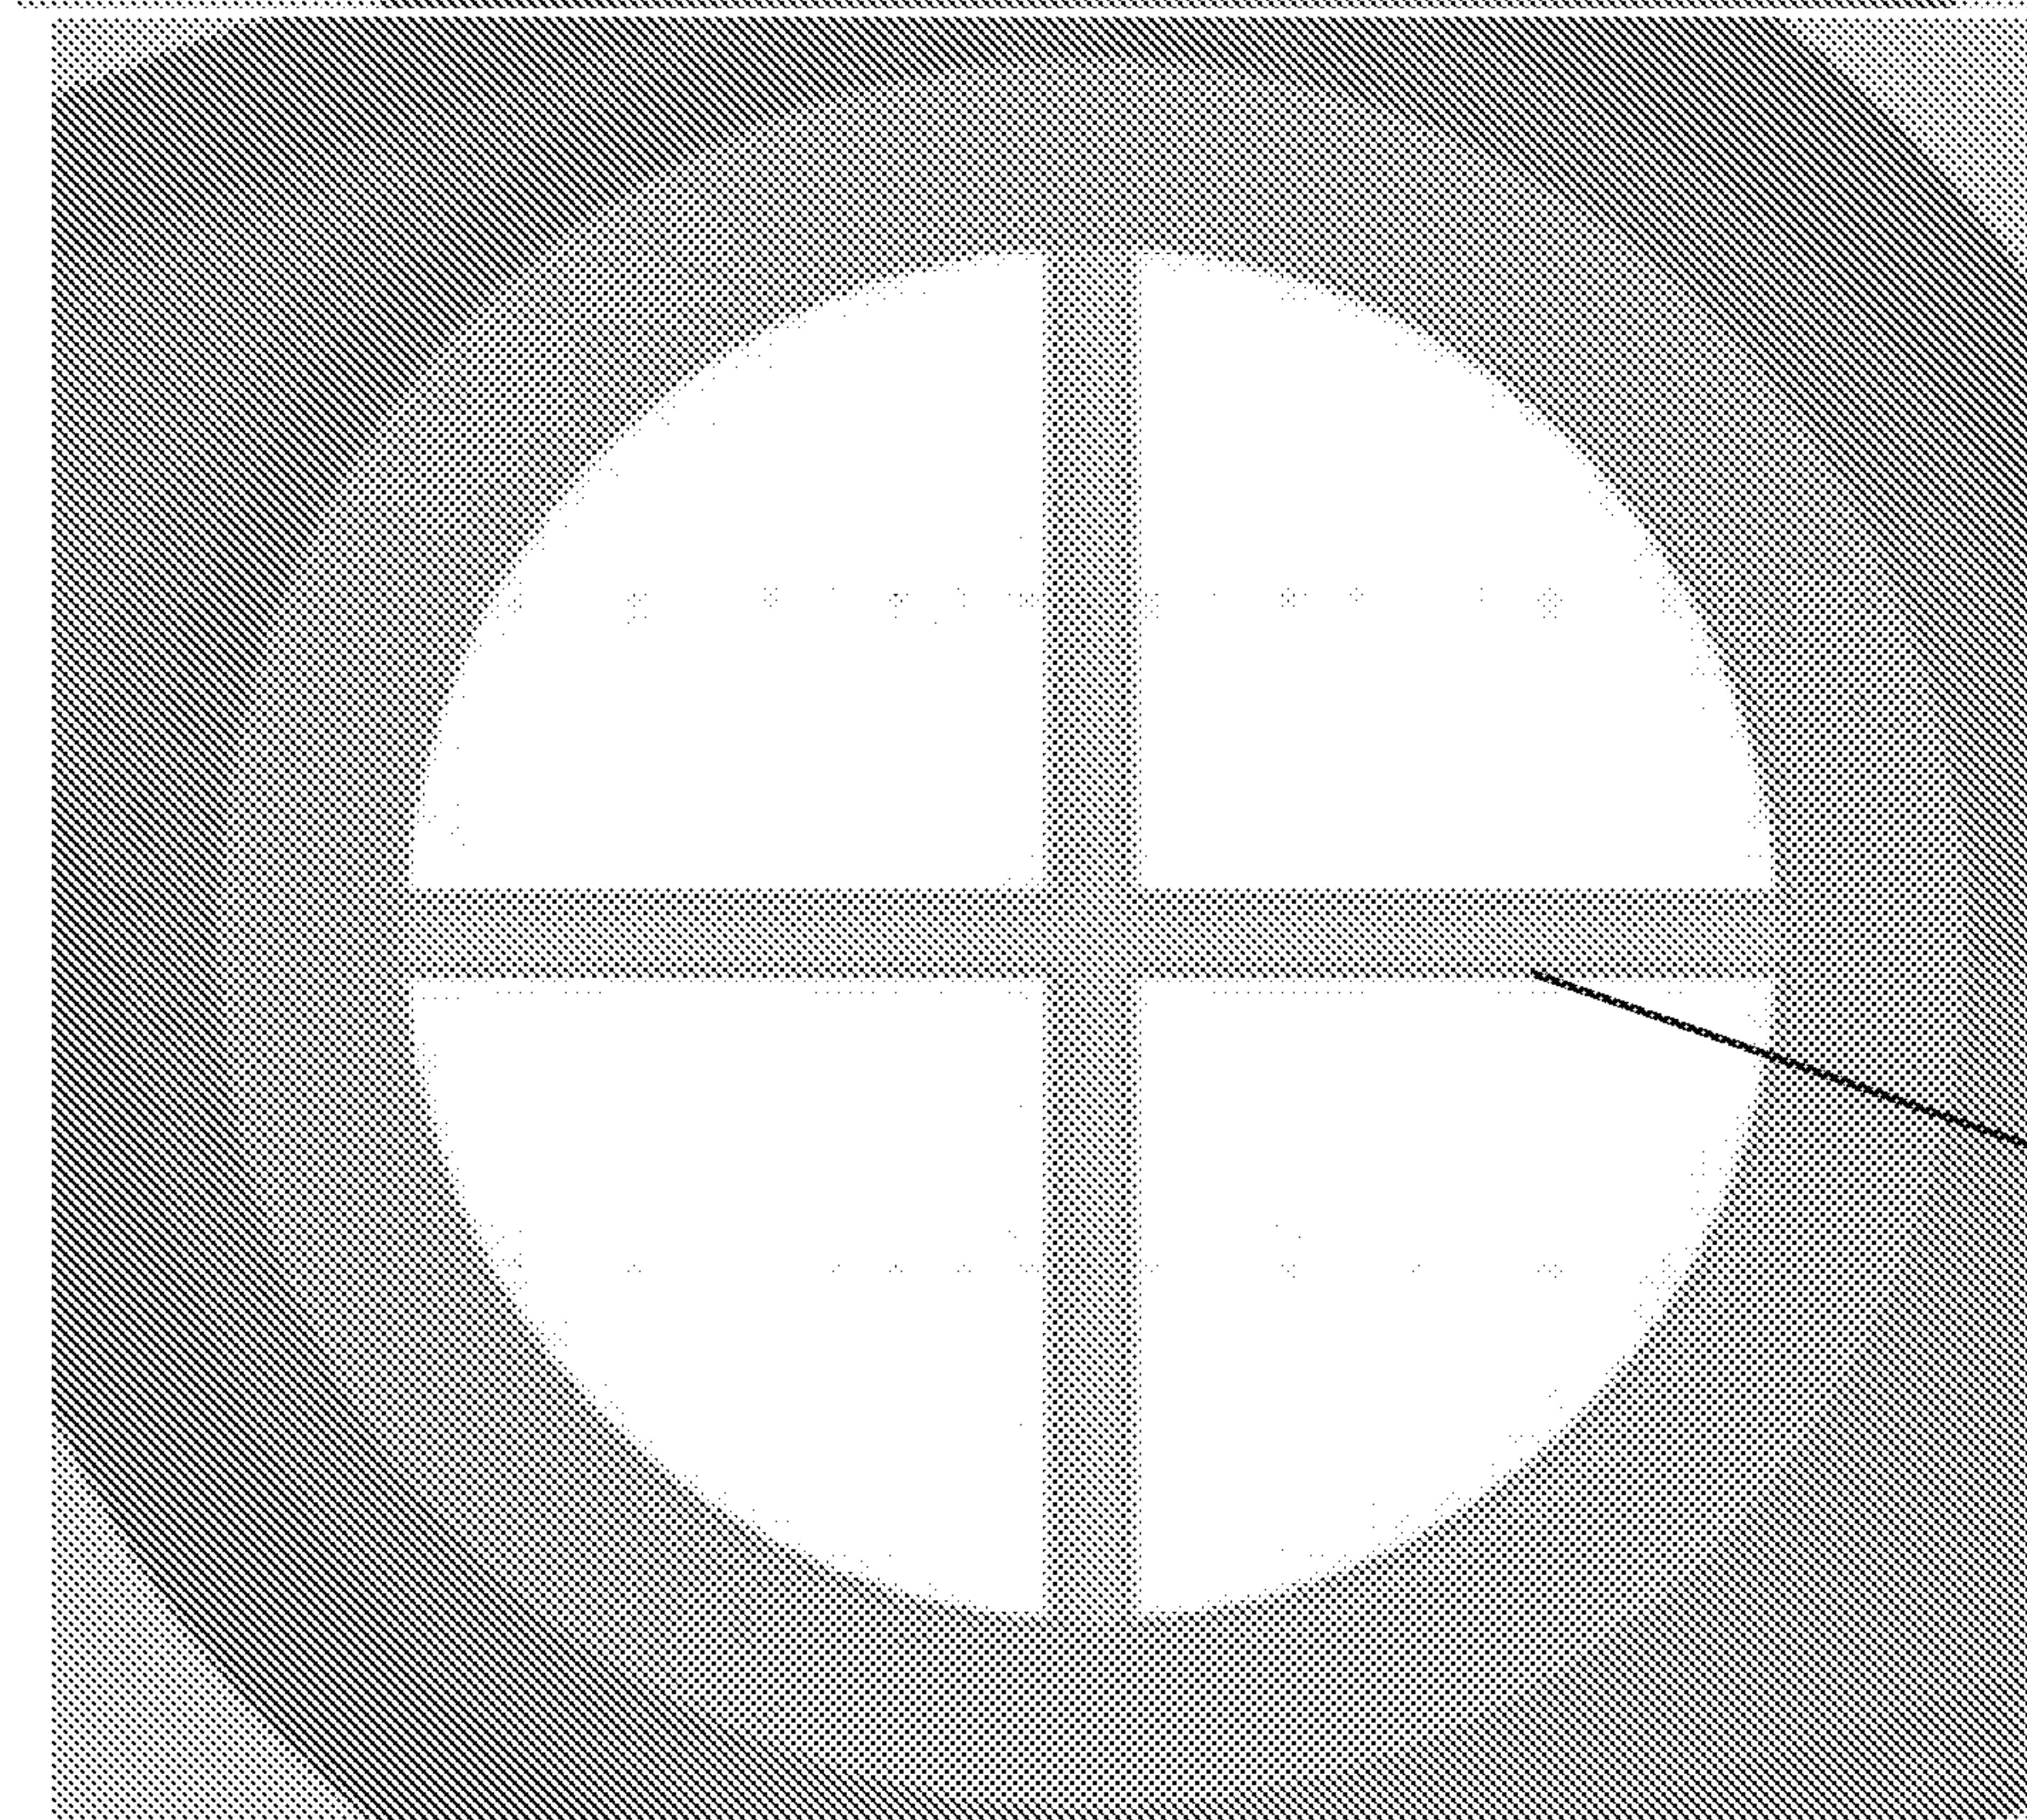


FIG. 28B

2802

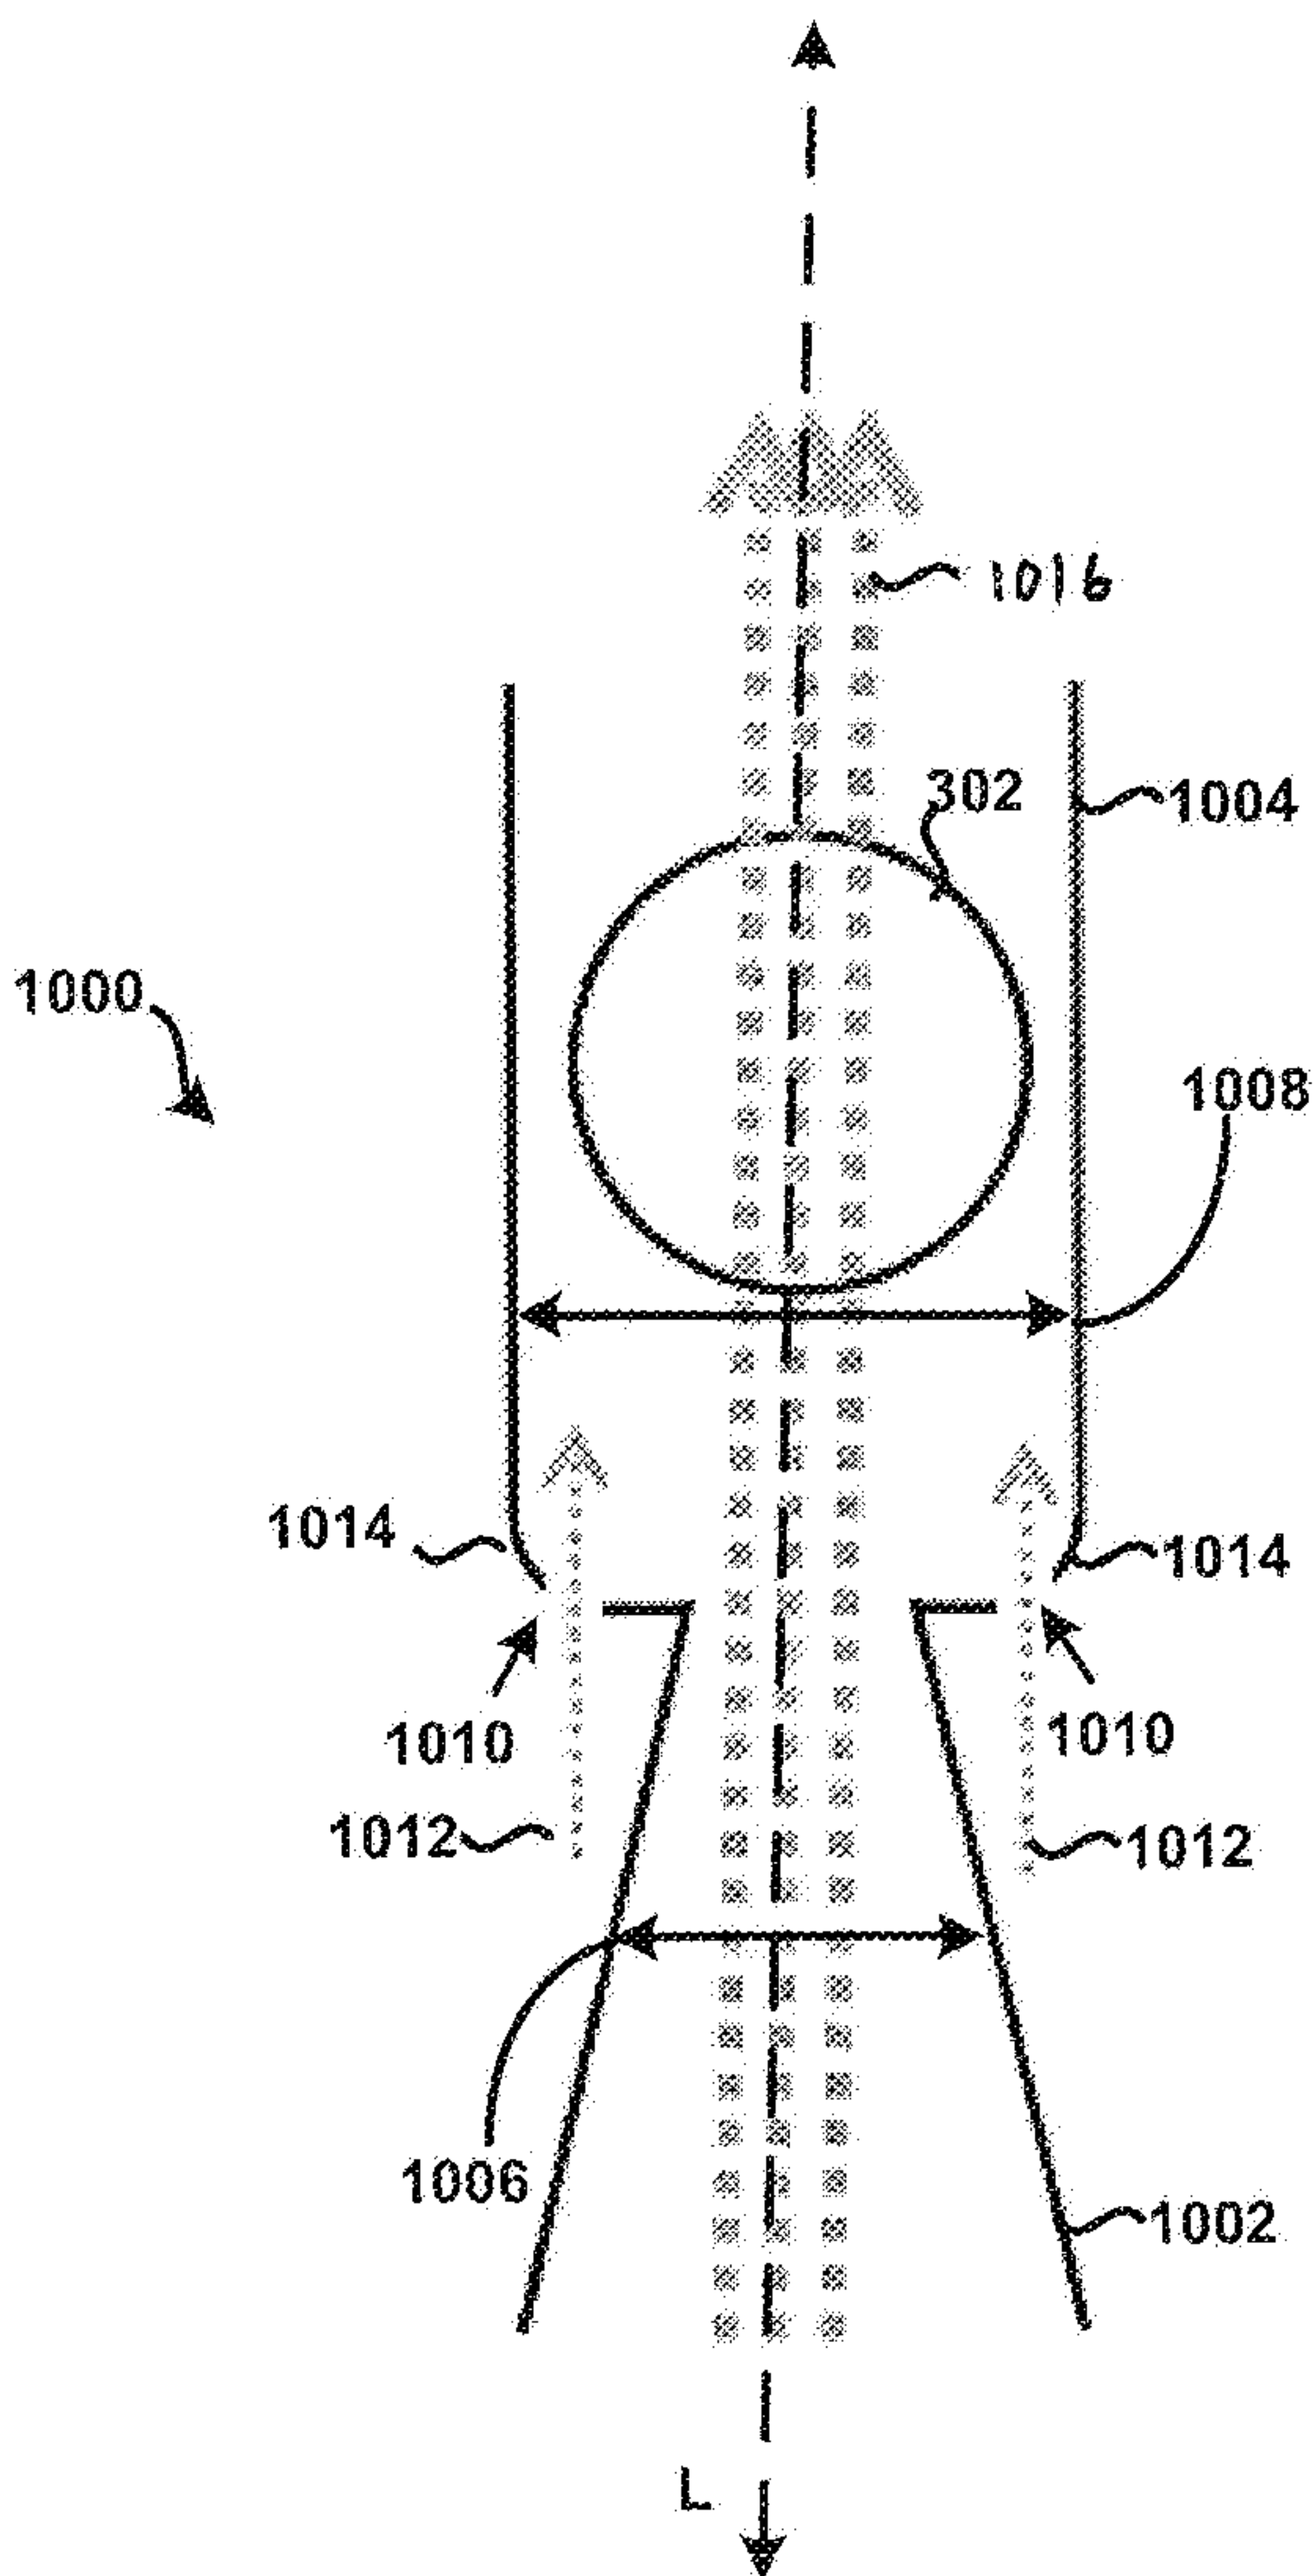


FIG. 10