



(51) International Patent Classification:

A61B 6/06 (2006.01) G21K 1/02 (2006.01)
A61N 5/10 (2006.01) G21K 1/04 (2006.01)

(21) International Application Number:

PCT/US2017/038256

(22) International Filing Date:

20 June 2017 (20.06.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/502,472 05 May 2017 (05.05.2017) US

(71) Applicant: ZAP SURGICAL SYSTEMS, INC. [US/US];
590 Taylor Way, San Carlos, California 94070 (US).

(72) Inventors: WILBUR, Raymond; c/o Zap Surgical Sys-
tems, 590 Taylor Way, San Carlos, California 94070 (US).
ACHKIRE, Younes; c/o Zap Surgical Systems, 590 Tay-

lor Way, San Carlos, California 94070 (US). BIRANG,
Manush; c/o Zap Surgical Systems, 590 Taylor Way, San
Carlos, California 94070 (US).

(74) Agent: SHURTZ, Kenneth R. et al.; Kilpatrick Townsend
and Stockton LLP, Mailstop: IP Docketing-22, 1100
Peachtree Street, Suite 2800, Atlanta, Georgia 30309 (US).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,
HR, HU, ID, IL, IN, IR, IS, JO, JP, KE, KG, KH, KN, KP,
KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(54) Title: REVOLVING RADIATION COLLIMATOR

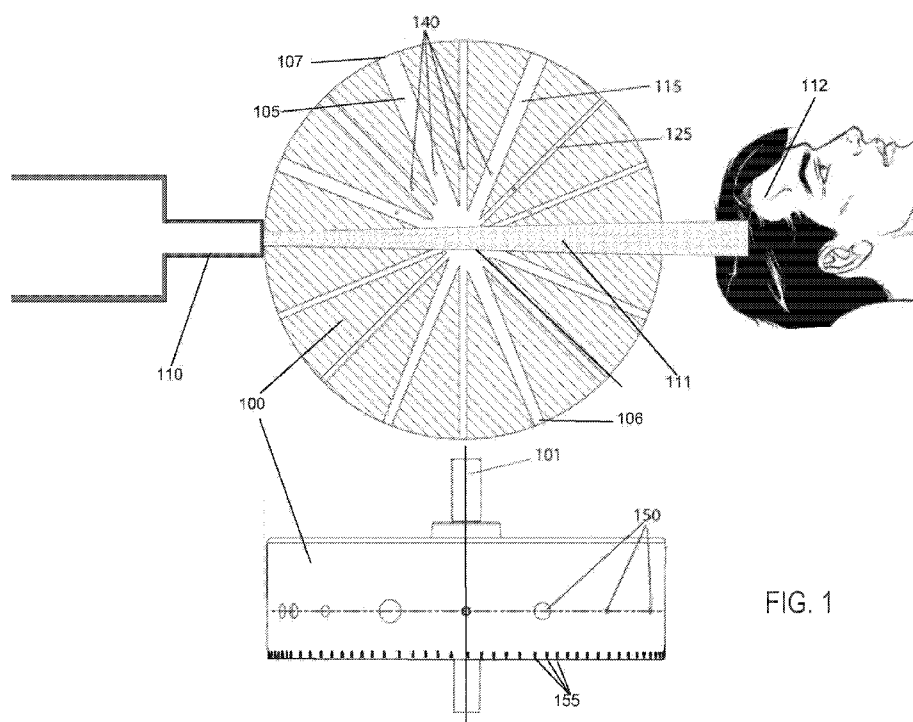


FIG. 1

(57) Abstract: Devices, systems and method that allow for delivery of therapeutic radiation beams of differing sizes or shapes during a radiation treatment are provided herein. Such devices can include a rotatable collimator body having multiple collimator channels of differing size or shape defined therein, the channels extending through the collimator body substantially perpendicular to the axis of rotation. The collimator body can include markers thereon to facilitate detection of an alignment position by a sensor of a control system to allow the collimator body to be rapidly and accurately moved between alignment positions to facilitate delivery of differing therapy beams during a treatment.



(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

REVOLVING RADIATION COLLIMATOR

CROSS-REFERENCES TO RELATED APPLICATIONS

- 5 **[0001]** This application claims the benefit of priority of U.S. Provisional Application No. 62/502,472 filed May 5, 2017, the entire contents of which are incorporated herein by reference.

BACKGROUND

[0002] The overarching goal of the collimator system is to deliver a beam of radiation produced by a source (for example a LINAC) to a target (for example a tumor in a patient's
10 brain). Because it is desirable to irradiate a tumor, but generally not desirable to irradiate surrounding healthy tissue, the size and the shape of each beam is of critical importance. In order to control the shape (for example diameter or 2D cross sectional area) of a beam of radiation, a collimator is used. A collimator is generally a piece of dense radiopaque metal that substantially blocks a beam of radiation except where a formed or machined hole allows the
15 radiation to be transmitted through. A larger radiation footprint may be produced by the radiation source (for example a LINAC or cobalt), but only those particles aligned to pass through the collimator will be permitted through to reach the target, the excess being absorbed or scattered internally. In addition to the tubular channels of machined or formed collimators, another pre-existing type is called a multi-leaf collimator. These conventional designs are very
20 complex, bulky and expensive. One example is a "Multi Leaf Collimator" using multiple thin tungsten plates moving in and out of the beam path to generate the desired beam exposure shape during treatment. This complex mechanism is prone to mechanical failure.

[0003] Different size and shape radiation treatment targets require different size and shape beams of radiation. There exists a need for systems and methods that allow for radiation beams
25 to be changed in a rapid and predictable manner. There is further a need for such systems to remain small, reliable and low cost.

BRIEF SUMMARY

[0004] The invention relates to the field of radiation therapy, and in particular, to collimator systems and associated methods of controlling the size and shape of radiation treatment beams during radiation therapy.

5 [0005] In a first aspect, the invention pertains to a radiation collimator assembly that includes a rotatable collimator body or collimator wheel having multiple collimator channels defined therein. In some embodiments, the collimator channels extend longitudinally perpendicular to the rotational axis of the collimator wheel, extending from the perimeter of the wheel, passing through the center and out to the opposite perimeter of the wheel. The collimator wheel is at least
10 partly surrounded by a collimator shield, excepting at least the portion having the selected collimator channel that is aligned with the radiation source and the patient target to allow passage of the radiation beam therethrough. In some embodiments, the posterior, LINAC-facing portion of the collimator wheel is ensheathed in shielding to prevent stray radiation from passing through non-selected collimator channels. The collimator shield is fabricated from a suitable
15 radiation absorptive material, typically tungsten or tungsten alloy, so as to block and absorb any scattered radiation emitted from orifices of non-aligned channels.

[0006] In another aspect, the collimator body is motorized and precisely indexed for rapid and exacting computer-controlled positioning of the selected collimator channel geometry with the radiation source, thereby delivering a desired beam shape to the precise dimensions required at
20 the target. By using a revolving collimator wheel, multiple sizes of the beam may be utilized during one treatment, quickly and automatically switching between two or more selected collimators.

[0007] These collimation assemblies have the advantage of being rapidly changeable by computer control, while remaining small, reliable in their simplicity and low in cost. Moreover,
25 such assemblies can utilize a single motor to switch between select one or more collimator channels. The aspects of the invention described herein allow for a more reliable radiation collimator that can quickly and precisely change X-ray exposure from 1 mm to 30 mm diameter at isocenter, and can function more reliably than many prior art collimators. Such collimator

assemblies enable rapid, automated (motorized and computer controlled) changing of beam aperture in the service of therapeutic radiation delivery, for example to treat brain tumors.

[0008] The collimator systems described herein allow for beam collimation without requiring use of a conventional block collimator and/or multi-leaf collimator system, such as those
5 commonly used in conventional radiation treatment systems, which are bulky and prone to mechanical malfunction over time.

[0009] In one aspect, an exemplary radiation collimator assembly includes a radiation source and a collimator wheel rotatable about a rotational axis thereof. The collimator wheel has multiple collimator channels that include a first and second collimator channel defined within the
10 collimator wheel that are arranged substantially perpendicular to the rotational axis of the collimator wheel. The collimator can include additional channels, for example three or more channels. The collimator can include any number of channels desired (e.g. 2, 3, 4, 5, 6, 7, 8, 9, 10 channels or more). In some embodiments, each of the first and second collimator channels pass through a center of the collimator wheel through which the rotational axis extends.

15 Preferably, at least some of the collimator channels are of differing sizes and/or shapes. In some embodiments, the multiple collimator channels are distributed at regular intervals along the collimator wheel.

[0010] In another aspect, the first and second collimator channels are selectable by rotationally moving the collimator wheel to align one of the first and second collimator channels with the
20 radiation source. Selective rotation of the collimator wheel can be facilitated by a motor and control unit operably coupled to the wheel. In some embodiments, the collimator assembly includes a motor operably coupled with the collimator wheel so as to rotate the collimator wheel about the rotational axis; and a control unit operably coupled with the motor to control rotation of the collimator wheel to a collimator position corresponding to alignment of a selected
25 collimator channel with the radiation source. In some embodiments, the control unit is communicatively coupled with one or more sensors configured to detect the collimator position. The one or more sensors can include one or more encoder readers and the collimator wheel includes multiple markers positioned thereon so that detection of a marker corresponds to alignment of a corresponding collimator channel.

[0011] In another aspect, radiation treatment systems utilizing such collimator assemblies are provided herein. An exemplary treatment system can include a radiation collimator assembly, such as described above, that is configured to deliver a radiation beam from a radiation source through one or more selected collimator channels of the collimator wheel to a target within a patient. Such a system can include a motor operably coupled with the collimator wheel so as to rotate the collimator wheel about the rotational axis and a control unit operably coupled with the motor to control rotation of the collimator wheel to positions corresponding to alignment of one or more selected collimator channel with the radiation source. The control unit is configured to rotate the collimator wheel to align one or more selected collimator channels with the radiation source, the one or more selected collimator channels corresponding to one or more desired therapy beams.

[0012] In another aspect, the treatment system includes a collimator shield. The collimator shield can be configured to surround at least a portion of the collimator body during delivery of therapy so as to block radiation from non-aligned collimator channels while allowing passage of a therapy beam from the selected, aligned collimator channel. In some embodiments, the collimator shield substantially surrounds a portion of the collimator wheel facing the radiation source except for the entry orifice of the selected, aligned collimator channel. In some embodiments, the collimator shield substantially surrounds the collimator body except for an aperture at an apex of the shield through which includes the exit orifice of the selected aligned collimator channel is exposed as well as a passage at the inlet orifice of the aligned channel to allow entry of the radiation beam through the selected channel. While a conically shaped shield is depicted in the embodiments presented herein, it is appreciated that the collimator shield could be formed in various different shapes so long as the shield allows radiation to pass through the selected, aligned channel while blocking radiation emitted from non-selected channels.

[0013] In yet another aspect, the treatment system can include an alignment verification mechanism. Such a verification feature can include an optical alignment feature, such as an optical laser light mechanism that directs a laser light beam through the selected collimator channel and detects the laser light beam emanating from an exit orifice. In some embodiments, the treatment system further includes one or more imaging devices for monitoring a patient during treatment.

[0014] In some embodiments, the collimator includes a collimator body having a pivot feature about which the collimator body is rotatable about a pivotal axis and multiple collimator channels extending through the collimator body, each being substantially perpendicular to the pivotal axis about which the collimator body is revolved. In some embodiments, each of the multiple collimator channels intersects the pivotal axis.

[0015] In another aspect, methods of delivering therapy beams of differing size and/or shape to a target in a patient during therapy are provided herein. An exemplary method includes selecting a first collimator channel from multiple collimator channels in a collimator body, the selected first collimator channel corresponding to a desired first therapy beam. The collimator body is rotatable within the treatment system along a rotational axis of the collimator body and the multiple collimator channels differ in size and/or shape and extend substantially perpendicular to the rotational axis. Next, the collimator body is rotated along the rotational axis until the selected first collimator channel is aligned with the radiation source, then a first particle beam is transmitted from a radiation source through the selected first collimator channel so as to direct the desired first therapy beam to the target within the patient. Such methods can further include selecting a second collimator channel in the collimator body, the selected second collimator channel corresponding to a desired second therapy beam differing from the first therapy beam in size and/or shape. The collimator body is then rotated along the rotational axis until the selected second collimator channel is aligned with the radiation source and then a second particle beam is transmitted from the radiation source through the selected second collimator channel so as to direct the desired second therapy beam to the target within the patient. In some embodiments, rotating the collimator body until the selected first collimator channel is aligned comprises rotating the collimator body until a sensor of a control unit of the system detects a marker disposed on the collimator body indicating a collimator position that corresponds to alignment of the first collimator channel. Such methods can further include validating alignment of the first collimator channel with the radiation source by transmitting a laser light beam through the collimator channel and detecting the laser light beam emitted from an exit aperture of the first collimator channel.

[0016] Various aspects and details of the invention can be further understood by referring to the exemplary embodiments depicted in the figures and the description provided below.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] FIG. 1 shows a cross section of an example revolving collimator wheel having collimator channels passing therethrough.

[0018] FIG. 2 shows an example revolving collimator wheel mounted upon a conical shield, the collimator wheel having magnetic encoder trackers that sense when the wheel has been brought into a desired collimator position.

[0019] FIG. 3 shows the apex of an example conical shield, including the exit openings of the collimator channels of the collimator wheel and cameras for monitoring the patient.

[0020] FIG. 4 shows an example collimator wheel and associated motor configured to drive between positions, and a linear accelerator that passes radiation through the collimator wheel and associated features.

[0021] FIG. 5 shows another example conical shield surrounding a periphery of the collimator wheel to cover orifices of non-aligned channels.

DETAILED DESCRIPTION

[0022] The invention relates generally to radiation treatment systems and methods of use, in particular collimator systems provide selective control and delivery of collimated beams of radiation.

[0023] FIG. 1 shows a cross sectional view of a revolving collimator wheel 100 having collimator channels 140 passing therethrough. Collimator wheel 100 has longitudinally extending channels or collimator channels 105, 115 and 125 defined therein, for example machined through the body of collimator wheel 100. The figure shows multiple other channels that are not labeled for the sake of clarity of the drawing. The collimator channels may be of various sizes, diameters or shapes. In some embodiments, each collimator channel is of a different diameter. For example, as shown in FIG. 1, collimator channel 105 is of larger bore than collimator channel 115, which is of larger bore than collimator channel 125. Each collimator channel extends from a radiation entrance aperture 106 to an exit aperture 107. In

some embodiments, the size of the entrance aperture 106 is smaller than that of the exit aperture 107 to facilitate delivery of maximal radiation doses at the margins of the target that the radiation ultimately strikes. The collimator wheel 100 is rotated so that a selected collimator channel is aligned with a radiation source 110 to allow passage of a particle radiation beam 111 through the selected channel, thereby providing a desired therapy beam to a target 112 in the patient. In a side profile of collimator wheel 100 shown at the bottom of FIG. 1, the entrance and exit apertures 150 are visible about the circumference collimator wheel 100 turns on axis 101. In this example, collimator wheel 100, couples with a 50:1 reduction gearbox and electric motor. In some embodiments, channel 105 and exit aperture 107 are round. It is appreciated that in alternative embodiments, the channels may be of any size or shape, for example square. Collimator wheel 100 can be formed of any suitable material, for example machined from a titanium alloy. While collimator wheel 100 is shown as being oriented vertically relative to the surface on which the patient rests, it is appreciated that the collimator wheel 100 could be configured in any orientation so long as the treatment beams passing through the collimator channels are directed to the target. Further, while the collimator wheel is shown as having eight collimator channels it is appreciated that such collimator wheels could include more or fewer collimator channels.

[0024] FIG. 2 shows a cross section of a revolving collimator wheel 200 mounted upon a collimator shield 210, and rotating between collimator positions on axis 205. In this embodiment, the collimator shield 210 substantially ensheaths the portion of the collimator wheel facing the radiation source so as to prevent radiation from entering non-aligned collimator channels. The rotational position of the collimator wheel can be precisely controlled by a control system by use of one or more sensors or encoders that monitor the position of the collimator wheel 200, for example by detecting markers disposed on the periphery of the collimator wheel. In this embodiment, the position of the collimator wheel is precisely monitored by encoder reader heads 215 and 216, which track a thin tapelike encoder strip affixed to the inner rim 214 of collimator wheel 100, adjacent to the path of reader heads 215 and 216. The control system detects signals produced by precisely placed changes in the electromagnetic interaction between the encoders and the encoder strip. Using this combination of encoder strip affixed to internal rim 214 and encoder reader heads, the control system senses when the wheel has been brought into the desired collimator position. Also shown in the cross section of collimator shield 210 is a

LINAC head 230, which is the source of the radiation delivered to the entrance aperture of a selected collimator. In some embodiments, an ion chamber is included in the collimator shield between the LINAC head 230 and collimator wheel 200. Alternative positional encoder schemes could include mechanical stops such as gear teeth and divots, and/or optically sensed position markers.

[0025] In one aspect, the collimator assembly and control system described above are incorporated into a treatment system. The control system includes a processor configured to facilitate controlled rotation of the collimator wheel to select positions corresponding to alignment of a selected collimator channel with the radiation source, the selected collimator channel corresponding to a desired treatment beam. In some embodiments, the treatment system includes a user interface that allows a treating physician to select one or more treatment beams associated with one or more collimator channels. In other embodiments, the control system automatically determine one or more collimator channels corresponding to a selected course of treatment.

[0026] FIG. 3 shows the apex of the conical shield, including the exit openings of the collimator channels and cameras for monitoring the patient. Collimator wheel 300 is visible edge-on, including selected channel exit aperture 305 and other apertures that are not identified and thus not aligned with the LINAC (underlying and not visible). Motor 315 turns collimator wheel 305 to a selected position in which the desired aperture is aligned with the LINAC. In some embodiments, the system includes one or more cameras to, for example cameras 310, positioned to permit the patient to be monitored while undergoing radiation treatment. Encoder interpretation computer subsystem 320 receives signals from encoder reader heads (see FIG. 2) to compute the precise rotational position of collimator wheel 300, and hence the position of any of the selectable collimator channels. For example, in a feedback loop, motor control computer subsystem 330 serves to activate motor 315 until encoders indicate that the selected collimator is aligned with the LINAC. In one aspect, the system is configured to change the collimator wheel position between multiple positions associated with select collimator channels during therapy so as to differing sizes of treatment beams to the target.

[0027] FIG. 4 shows a cross-sectional view of the collimator wheel in the context of the motor that drives between positions and a linear accelerator that passes radiation through an aligned collimator channel and associated features.

[0028] As shown, collimator wheel 449 has selected and aligned channel 451 with exit aperture 452 and entrance aperture 450. Collimator shield 410 surrounds the collimator wheel 449 along the portion facing the radiation source to allow passage of the particle beam through the inlet and exit orifices of channel 451 while preventing radiation from entering non-aligned channels. In this embodiment, collimator wheel 449 is selectively turned into the desired position via shaft 453 with bushing 434, shaft 453 being connected with gearbox 444 via coupling bracket and base 420. Gearbox 44 is coupled to and driven by motor 445, and provides a reduction in revolutions at a pre-defined ratio, permitting very fine control of the degree to which the collimator wheel is turned and aligned with the radiation source, the LINAC head 460 and distal margin of LINAC body 461. The pre-defined ratio can be 10:1, 20:1, 30:1, 40:1, 50:1, 60:1, 70:1, 80:1, 90:1 or any ratio suitable for a given geometry of the collimator wheel and treatment system and desired resolution of adjustment. In this embodiment, energy exiting LINAC head 460 enters sealed ion chamber 403 which permits monitoring of dose, dose rate and field symmetry by virtue of the fact that radiation that enters the ion chamber will produce a measureable ionization current that is proportional to the x-ray beam intensity.

[0029] In this embodiment, mechanical alignment is optimized using optical beam techniques. This has the advantage of maximizing the transfer of radiation from the ion chamber 403 into entrance aperture 450. For this purpose, the system includes laser shield mount holding laser 416, the beam from which is bent at a right angle by mirror 415 and directed into diaphragm iris lens 419 after which the laser light passes through shield bore 421 defined in shield 410 to reach the beam path right angle optical mirror 422. Because the beam path right angle optical mirror 422 is reflective to light but transparent to radiation, a properly aligned collimator can be detected by a laser beam being emitted from exit aperture 452 of collimator 451, while maintaining functionality of the primary radiation delivery alignment, a function useful in initial validation and verification of each machine.

[0030] FIG. 5 shows another example system with the same or similar collimator wheel and associated components shown in FIG. 1 and a conical collimator shield 510 that substantially

surrounds the periphery of the collimator wheel so as to block and absorb radiation emitted from orifices of non-aligned collimator channels while allowing passage of a particle beam 111 from the radiation source 110 through the selected, aligned collimator channel to provide a desired therapy beam to the target 112. In this embodiment, the collimator shield 510 covers any orifices of non-aligned channels. In some embodiments, the shield can cover less than all orifices of non-aligned channels. It is appreciated that in any of the embodiments herein, the shield can include multiple shield components to cover orifices of non-aligned channels and is not required to be a unitary component. Various configurations of the shield can be realized in accordance with the concepts described herein.

[0031] While these components are shown in a particular arrangement in this example, it is appreciated that alternative configurations could be realized utilizing various other means of rotating the collimator wheel as would be understood by one of skill in the art. In addition, it is appreciated that certain elements could be omitted, such as the cameras, ion chamber and optical beam alignment features, while still retaining certain advantageous aspects of the invention described above.

[0032] In the foregoing specification, the invention is described with reference to specific embodiments thereof, but those skilled in the art will recognize that the invention is not limited thereto. Various features and aspects of the above-described invention can be used individually or jointly. Further, the invention can be utilized in any number of environments and applications beyond those described herein without departing from the broader spirit and scope of the specification. The specification and drawings are, accordingly, to be regarded as illustrative rather than restrictive. It will be recognized that the terms “comprising,” “including,” and “having,” as used herein, are specifically intended to be read as open-ended terms of art.

WHAT IS CLAIMED IS:

1. A radiation collimator assembly comprising:
a radiation source; and
a collimator wheel rotatable about a rotational axis thereof, the collimator wheel having a plurality of collimator channels, the plurality of collimator channels including at least:
a first collimator channel defined within the collimator wheel, and
a second collimator channel defined within the collimator wheel,
wherein the first and second collimator channels are arranged substantially perpendicular to the rotational axis of the collimator wheel.
2. The radiation collimator assembly of claim 1 wherein each of the first and second collimator channels pass through a center of the collimator wheel through which the rotational axis extends.
3. The radiation collimator assembly of any preceding claim, wherein the first and second collimator channels are of differing sizes and/or shapes.
4. The radiation collimator assembly of any preceding claim, wherein the plurality of collimator channels are distributed at regular intervals along the collimator wheel.
5. The radiation collimator assembly of any preceding claim, wherein the plurality of collimator channels comprise three or more collimator channels.
6. The radiation collimator assembly of any preceding claim, wherein the first and second collimator channels are selectable by rotationally moving the collimator wheel to align one of the first and second collimator channels with the radiation source.
7. The radiation collimator assembly of any preceding claim, further comprising:
a motor operably coupled with the collimator wheel so as to rotate the collimator wheel about the rotational axis; and

a control unit operably coupled with the motor to control rotation of the collimator wheel to a collimator position corresponding to alignment of a selected collimator channel with the radiation source.

8. The radiation collimator assembly of claim 7 wherein the control unit is communicatively coupled with one or more sensors configured to detect the collimator position.

9. The radiation collimator assembly of claim 8 wherein the one or more sensors comprise one or more encoder readers and the collimator wheel includes a plurality of markers positioned corresponding to alignments of the plurality of collimator channels.

10. A radiation treatment system comprising:
the radiation collimator assembly of claim 1, wherein the collimator assembly is configured to deliver a radiation beam from the radiation source through one or more selected collimator channels of the collimator wheel to a target within a patient;
a motor operably coupled with the collimator wheel so as to rotate the collimator wheel about the rotational axis; and
a control unit operably coupled with the motor to control rotation of the collimator wheel to positions corresponding to alignment of one or more selected collimator channel with the radiation source.

11. The radiation treatment system of claim 10, wherein the control unit is configured rotate the collimator wheel to align one or more selected collimator channels of the plurality with the radiation source, the one or more selected collimator channels corresponding to one or more desired therapy beams.

12. The radiation treatment system of claim 10 or 11, further comprising:
a collimator shield substantially surrounding at least a portion of the collimator wheel facing the radiation source that includes non-aligned collimator channels to inhibit passage of radiation through non-aligned collimator channels while allowing passage of a particle beam through the selected, aligned collimator channel.

13. The radiation treatment system of any of claim 10 through 12, further comprising one or more imaging devices for monitoring a patient during treatment.

14. The radiation treatment system of any of claim 10 through 13, further comprising: an optical beam alignment feature configured to monitor or validate alignment of the selected collimator channel with the radiation source.

15. A collimator comprising:
a collimator body having a pivot feature about which the collimator body is rotatable about a pivotal axis; and
a plurality of collimator channels extending through the collimator body;
wherein each of the plurality of collimator channels are substantially perpendicular to the pivotal axis about which the collimator body is revolved.

16. The collimator of claim 15 wherein each of the plurality of collimator channels intersects the pivotal axis.

17. A method of treating a patient with a radiation beam from a radiation source of a treatment system, the method comprising:

selecting a first collimator channel from a plurality of collimator channels in a collimator body, the selected first collimator channel corresponding to a desired first therapy beam, wherein the collimator body is rotatable within the treatment system along a rotational axis of the collimator body and the plurality of collimator channels differ in size and/or shape and extend substantially perpendicular to the rotational axis;

rotating the collimator body along the rotational axis thereof until the selected first collimator channel is aligned with the radiation source; and

transmitting a first particle beam from the radiation source through the selected first collimator channel so as to direct the desired first therapy beam to the target within the patient.

18. The method of claim 17, further comprising:

selecting a second collimator channel from the plurality of collimator channels in the collimator body, the selected second collimator channel corresponding to a desired second therapy beam differing from the first therapy beam in size and/or shape;

rotating the collimator body along the rotational axis until the selected second collimator channel is aligned with the radiation source; and

transmitting a second particle beam from the radiation source through the selected second collimator channel so as to direct the desired second therapy beam to the target within the patient.

19. The method of claim 17 or 18, wherein rotating the collimator body until the selected first collimator channel is aligned comprises rotating the collimator body until a sensor of a control unit of the system detects a marker disposed on the collimator body indicating a collimator position that corresponds to alignment of the first collimator channel.

20. The method of any of claim 17 through 19, further comprising:

validating alignment of the first collimator channel with the radiation source by transmitting a laser light beam through the collimator channel and detecting the laser light beam emitted from an exit aperture of the first collimator channel.

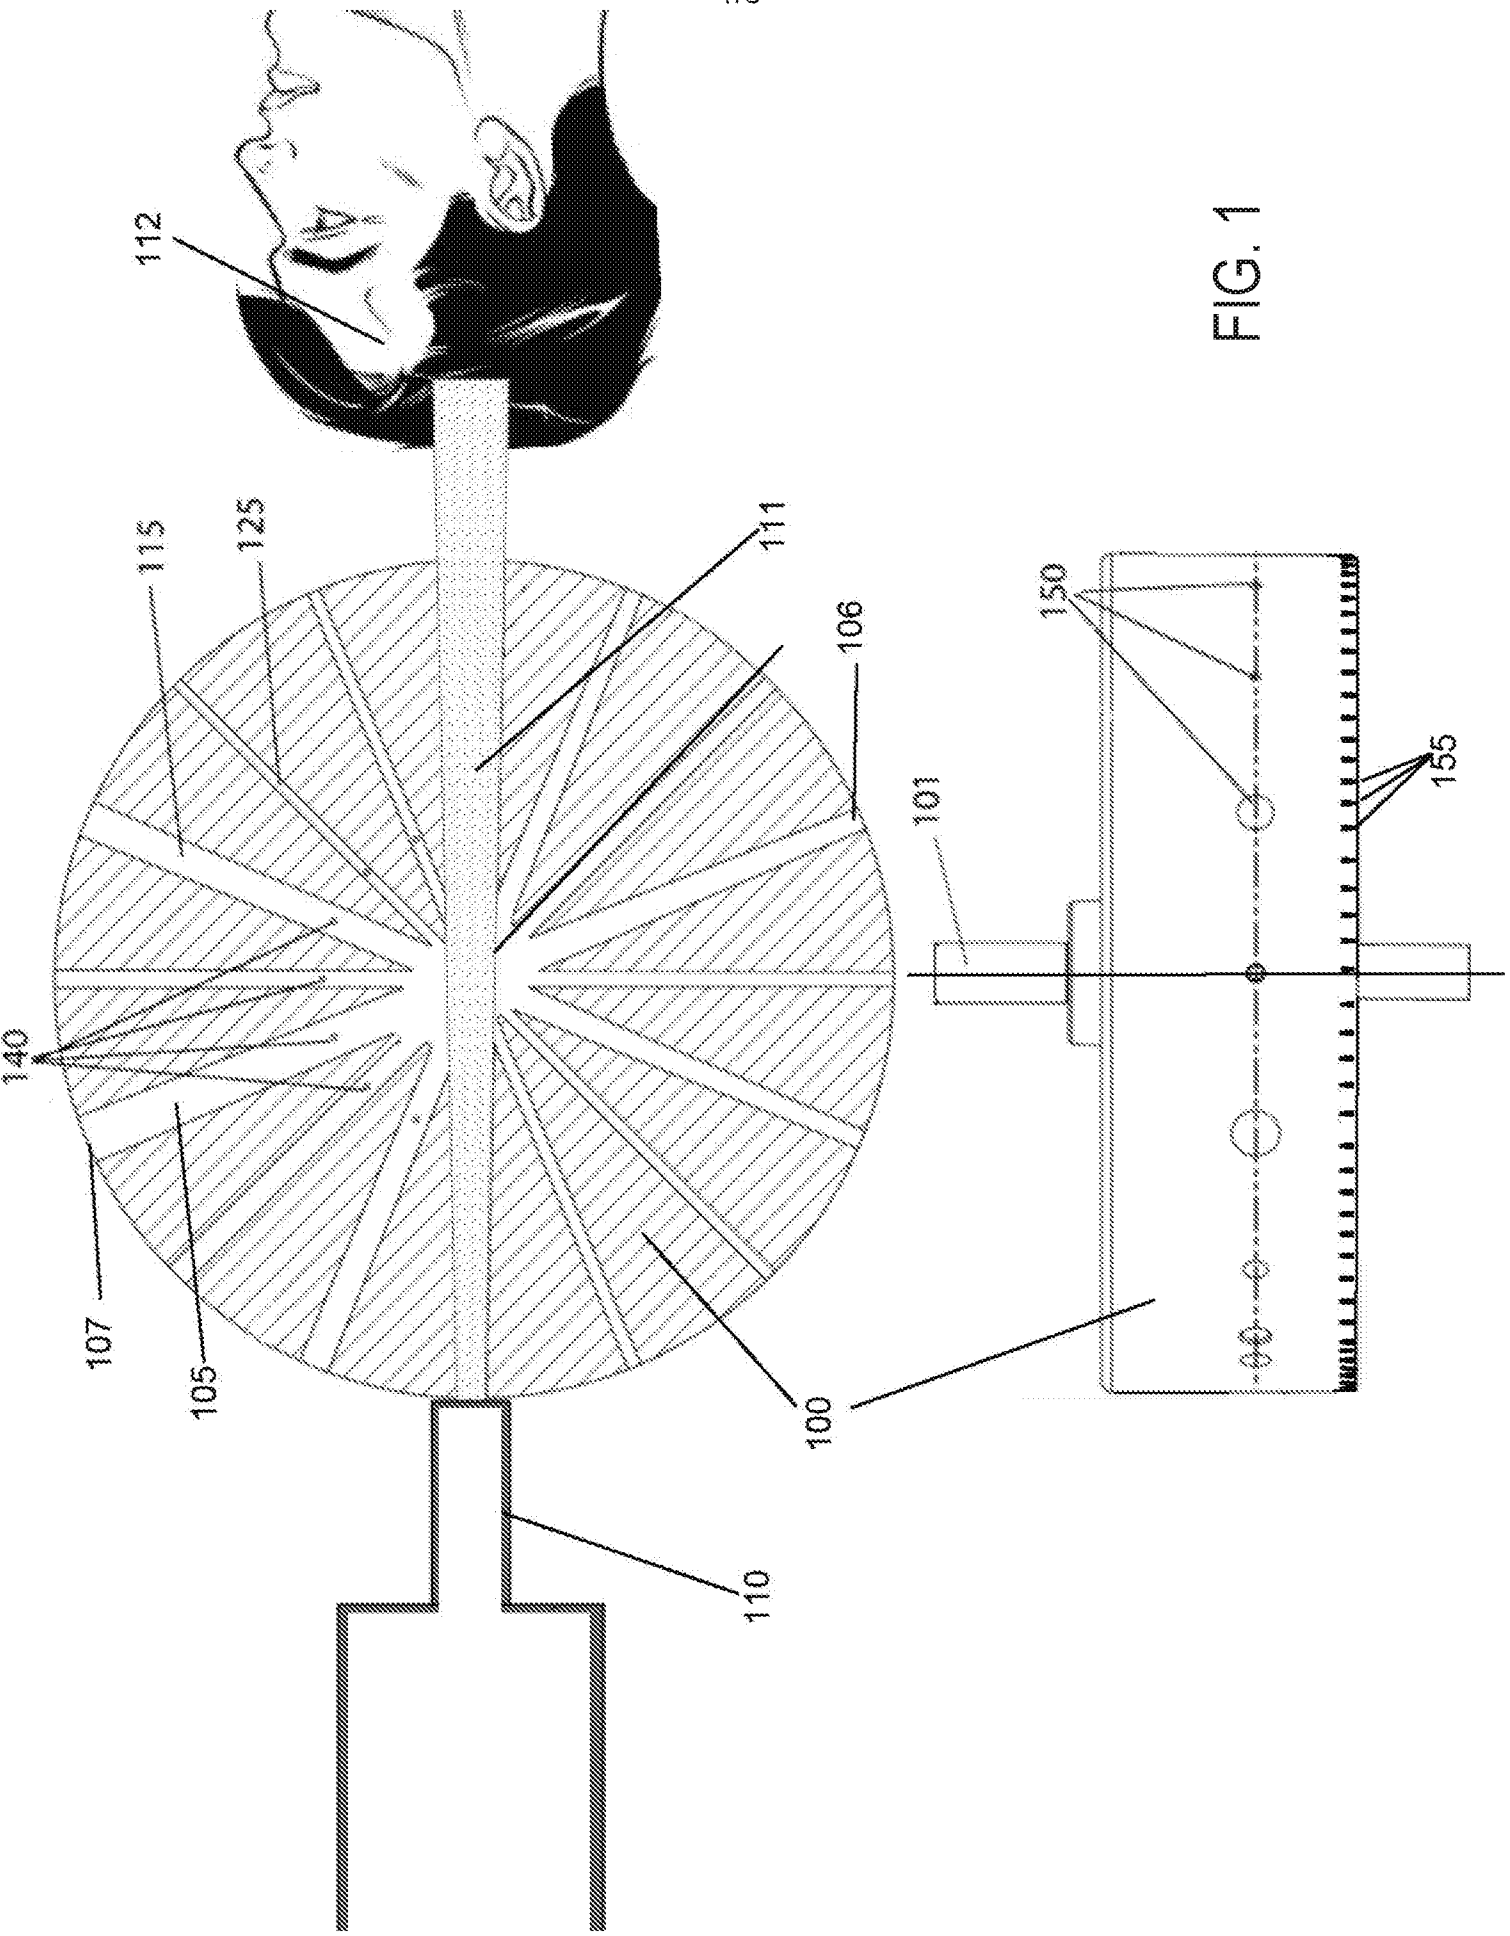


FIG. 1

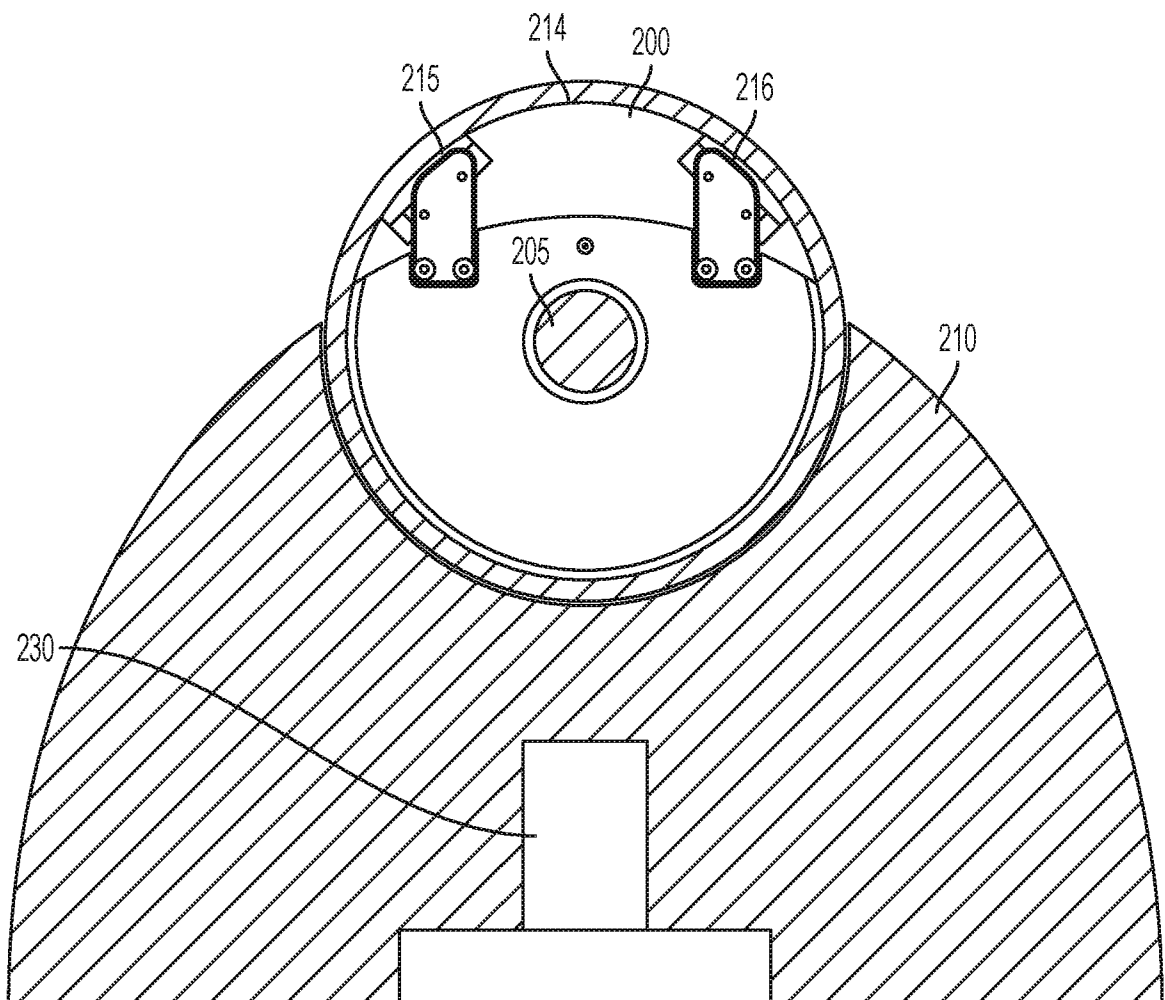


FIG. 2

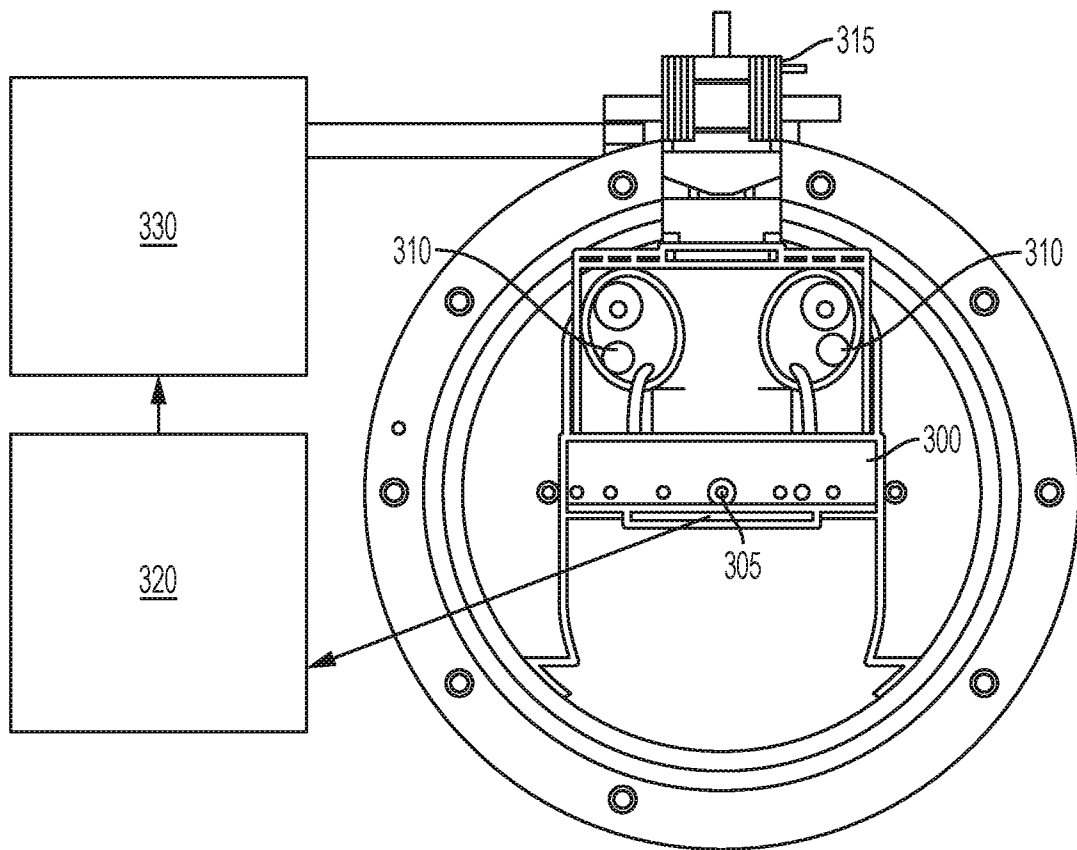


FIG. 3


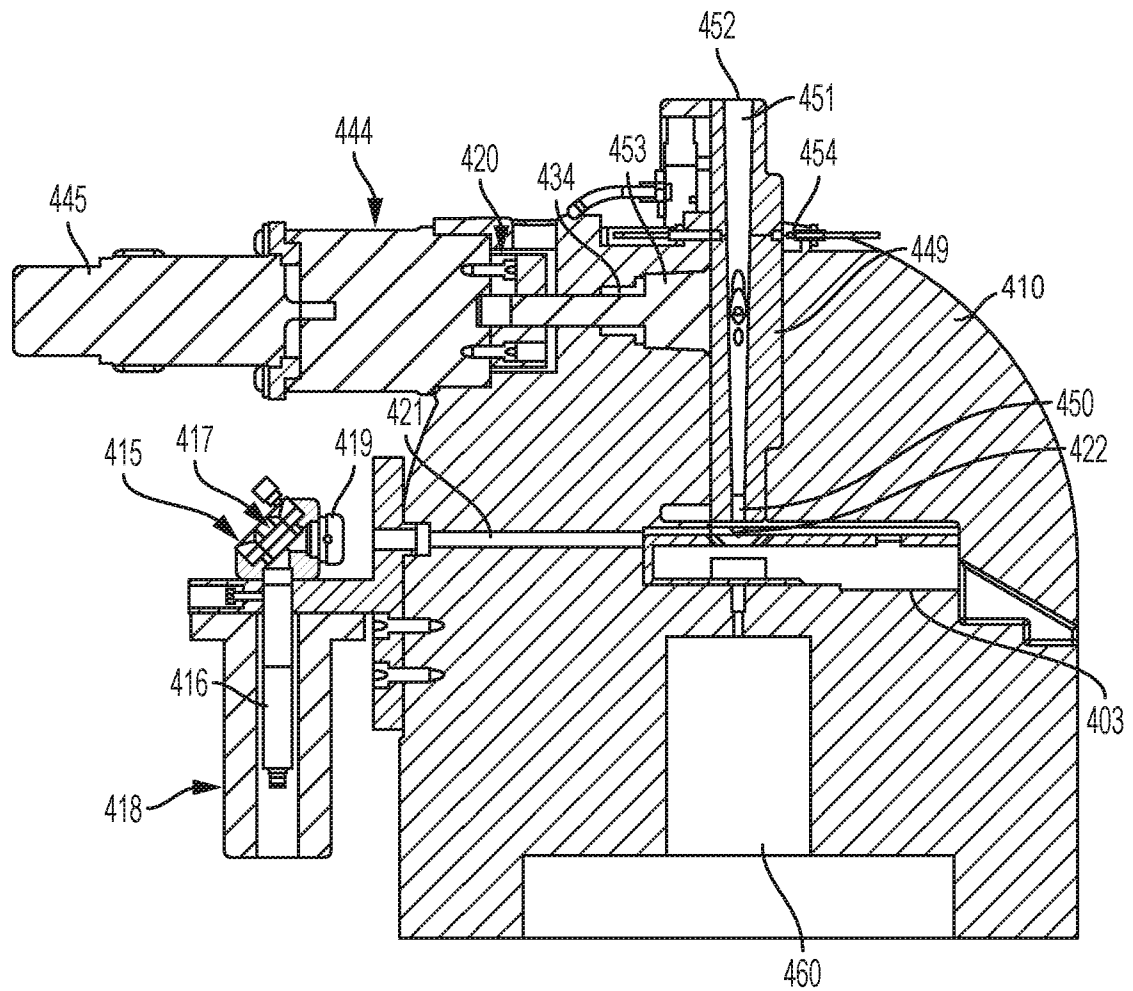


FIG. 4

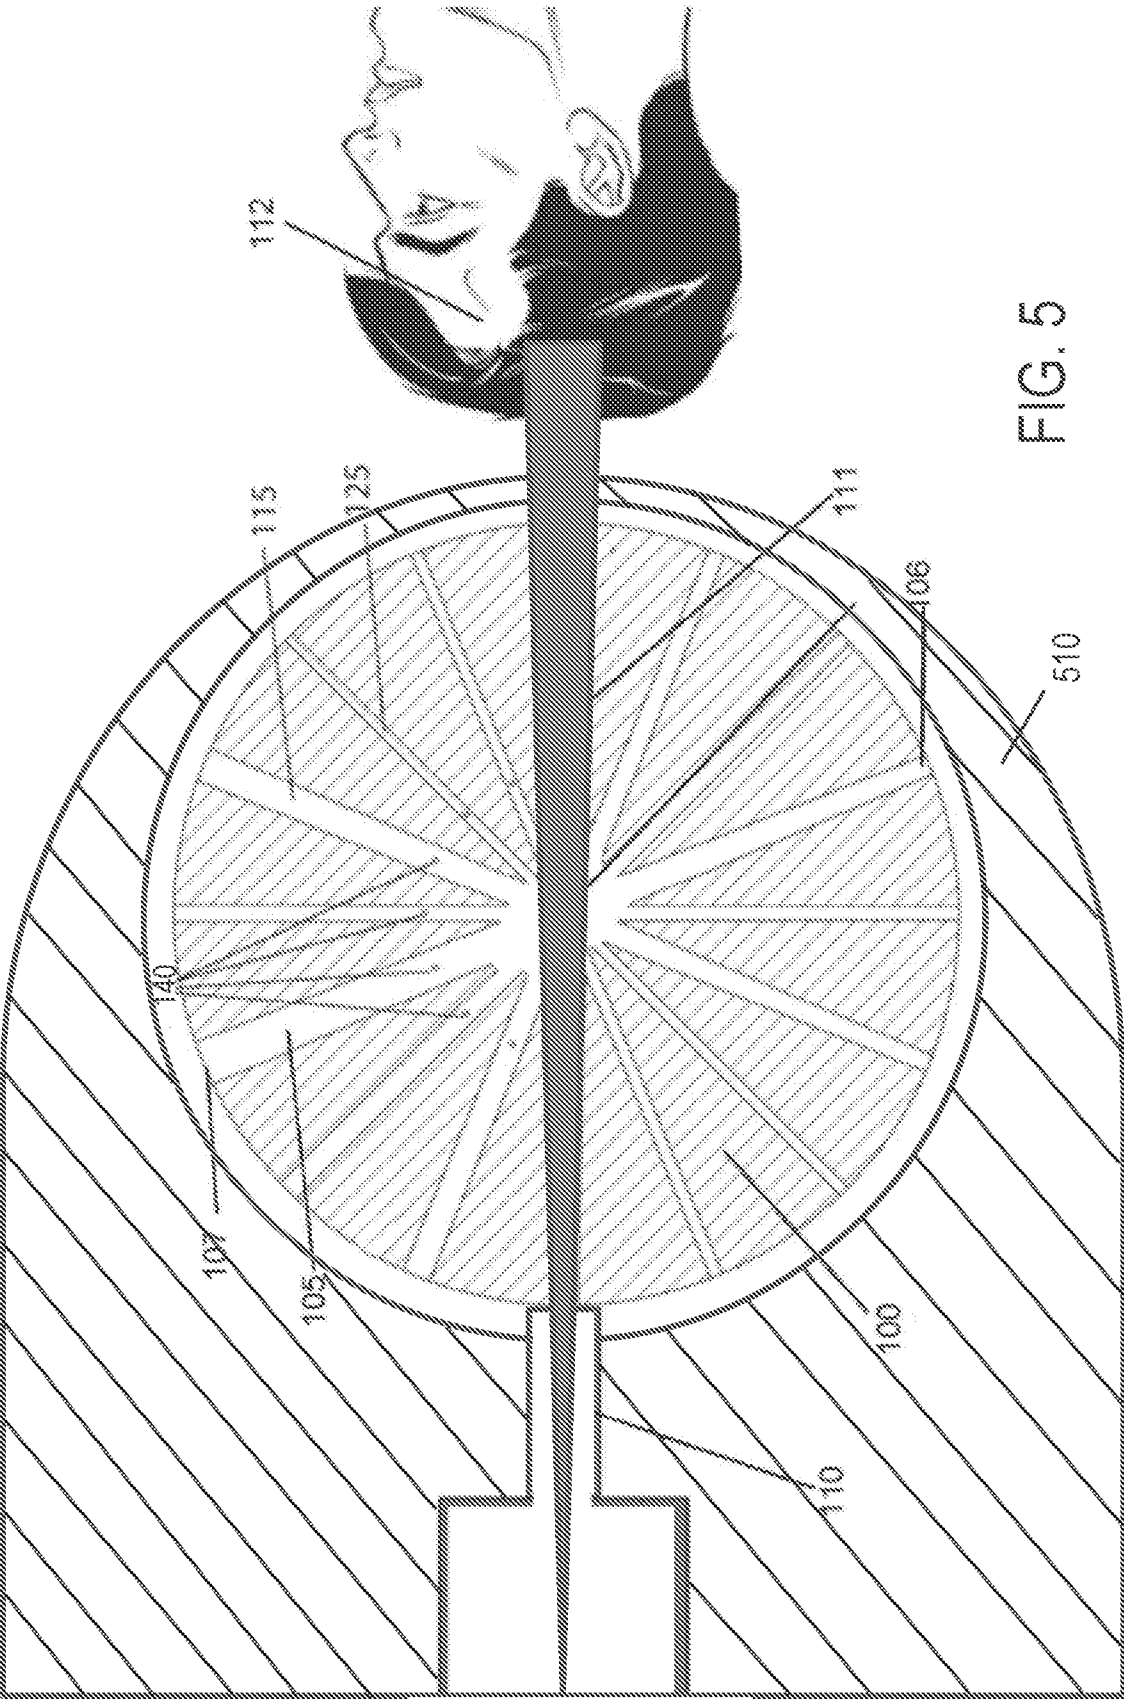

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2017/038256

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 6/06; A61N 5/10; G21K 1/02; G21K 1/04 (2017.01)

CPC - A61B 6/06; A61N 5/10; A61N 5/103; A61N 5/1031; A61N 5/1042; A61N 5/1045; A61N 5/1064; A61N 5/1065; A61N 2005/1087; A61N 2005/1088; A61N 2005/1095; G02B 6/002; G21K 1/02; G21K 1/04; G21K 1/043; G21K 1/046 (2017.02)

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

USPC - 250/492.3; 250/492.1; 250/505.1; 378/65; 378/145; 378/147; 378/149; 378/150; 378/160; 600/1 (keyword delimited)

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2013/0136239 A1 (ARIBEX, INC.) 30 May 2013 (30.05.2013) entire document	1-3, 10-12, 15-19
A	US 9,014,341 B2 (GE MEDICAL SYSTEMS GLOBAL TECHNOLOGY COMPANY LLC) 21 April 2015 (21.04.2015) entire document	1-3, 10-12, 15-19
A	WO 2013/180883 A1 (INDIANA UNIVERSITY RESEARCH AND TECHNOLOGY CORPORATION) 05 December 2013 (05.12.2013) entire document	1-3, 10-12, 15-19
A	US 4,266,135 A (KUWIK et al) 05 May 1981 (05.05.1981) entire document	1-3, 10-12, 15-19
A	US 9,208,918 B2 (NEUROLOGICA CORP.) 08 December 2015 (08.12.2015) entire document	1-3, 10-12, 15-19
A	US 2013/0261430 A1 (UHLEMANN et al) 03 October 2013 (03.10.2013) entire document	1-3, 10-12, 15-19

☐ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

21 August 2017

Date of mailing of the international search report

11 SEP 2017

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, VA 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Blaine R. Copenheaver

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2017/038256

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☒ Claims Nos.: 4-9, 13, 14, 20
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.