



(51) International Patent Classification:

G01N 30/06 (2006.01) C01G 23/047 (2006.01)
G01N 30/72 (2006.01) B01J 20/02 (2006.01)
G01N 27/64 (2006.01) C07K 1/14 (2006.01)
G01N 33/68 (2006.01)

(21) International Application Number:

PCT/US2015/065696

(22) International Filing Date:

15 December 2015 (15.12.2015)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/094,421 19 December 2014 (19.12.2014) US

(71) Applicant: UNIVERSITY OF HOUSTON SYSTEM
[US/US]; 4800 Calhoun Road, Houston, TX 77004 (US).(72) Inventors: VARGHESE, Oomman, K.; 2100 Welch
Street #C310, Houston, TX 77019 (US). WIJERATNE,
Aruna; 1200 Happy Hollow Road, Apt. 211, West Lafay-
ette, IN 47906 (US). PAULOSE, Maggie; 2100 Welch
Street, #C310, Houston, TX 77019 (US). AHIABU, Ivy;

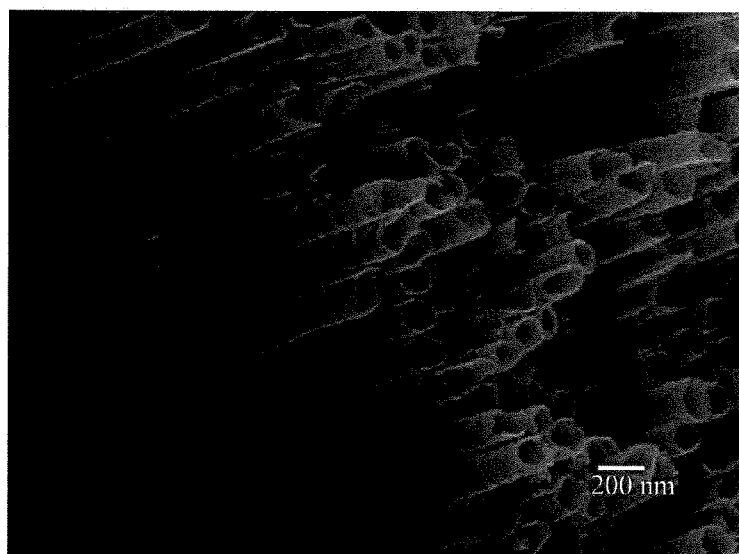
6446 Rutgers, Houston, TX 77005 (US). GREIS, Ken-
neth, D.; 7 Greene Street, Fort Thomas, KY 41075 (US).
WIJESUNDARA, Dharshana; 2627 Woodridge Cove
Dr., Houston, TX 77087 (US). CHU, Wei-kan; 2607
Lakecrest Drive, Pearland, TX 77584 (US).

(74) Agents: BORRELLI, Sara, K. et al.; Jackson Walker
L.L.P., 2323 Ross Avenue, Suite 600, Dallas, TX 75201
(US).(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG,
MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM,
PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC,
SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ,

[Continued on next page]

(54) Title: HIGHLY ORDERED TITANIA NANOTUBE ARRAYS FOR PHOSPHOPROTEOMICS

Figure 2



(57) Abstract: Titania nanotube arrays are useful for phosphopeptide enrichment and separation. These highly ordered titania nanotube arrays are a low cost and highly effective alternative to the use of liquid chromatography mass spectrometry (LC-MS) methods using mesoporous titania beads or particles. The highly ordered TiO₂ nanotubes are grown on surfaces coated with Ti metal, or preferably on Ti wires, by methods that preferably include anodic oxidation.



TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report (Art. 21(3))*

HIGHLY ORDERED TITANIA NANOTUBE ARRAYS FOR PHOSPHOPROTEOMICS

BACKGROUND

[0001] This disclosure pertains to phosphoproteomics or the study of phosphoproteomes in cellular systems and particularly to the use of titania nanotube arrays for separation and evaluation of phosphoproteomes.

[0002] Phosphoproteomic analysis offers a unique view of cellular function and regulation in biological systems by providing global measures of a key cellular regulator in the form of protein phosphorylation. Understanding the phosphorylation changes between normal and diseased cells or tissues offers a window into the mechanism of disease and thus potential targets for therapeutic intervention.

[0003] Reversible protein phosphorylation is a central regulatory mechanism for normal biological function and cellular homeostasis, while dysregulation of phosphorylation can lead to the initiation and propagation of a variety of diseases. As such, studies aimed at understanding the dynamics of phosphorylation on a global scale in control versus disease conditions have come to the forefront of biological research as the research community attempts to understand the underlying cellular mechanisms of disease with the goal of providing new targets for therapeutic intervention. Currently, methods employing liquid chromatography coupled with tandem mass spectrometry (LC-MS/MS) have become increasingly popular to study protein flux in various cellular systems and their various post translation modifications such as protein phosphorylation. The subset of proteins that are phosphorylated are referred to as phosphoproteomes. For evaluations on proteomes or phosphoproteomes using LC-MS/MS techniques, studies are performed by analyzing their respective peptide solutions generated from various proteolytic digestion strategies. This strategy is referred to as “bottom-up” proteomics. It employs separation of peptides based on their hydrophobic nature using liquid chromatography and analyzing the peptides eluting from LC-columns using mass spectrometry for their identity and quantity. Their respective proteins can then be related to the identified peptides with a variety of available database search algorithms. Such MS based proteomics methods are popular due to (1) high sensitivity, (2) ability to fragment peptides in millisecond time frames, and (3) the

ability to identify biochemically modified peptides along with the peptide sequence, thus allowing studies on phosphoproteomes .

[0004] The global study of cellular phosphorylation of proteins, commonly called phosphoproteomics, is typically done by first digesting the proteins into specific peptides followed by separation, identification and quantification of the peptides by liquid chromatography coupled with mass spectrometry (LC-MS). The success of these methods is highly dependent on the investigator's ability to effectively separate or enrich the phosphopeptides from non-phosphorylated peptides. This enrichment is required for several reasons: (1) many phosphorylated proteins are in low abundance compared to the total cellular protein and hence, their detection from a complex cellular mixture may be compromised due to the dynamic range of total proteins available; (2) phosphorylation site occupancy on many protein is often at a low stoichiometry (typically <5% but for phosphotyrosine it can be less than 0.1%) thus further diminishing the amount of phosphorylated peptide available for detection; (3) when using electrospray ionization (ESI) mass spectrometry, phosphopeptides are prone to ionization suppression in the positive ion mode when they are analyzed simultaneously with non-phosphorylated peptides. Given these challenges, the research community continually strives to developed ways to enhance the detection and quantification of the phosphopeptides.

[0005] For phosphopeptide enrichment, a variety of metal chelation and metal oxide affinity materials have shown great promise with titanium dioxide (TiO₂) having emerged as the most popular and widely utilized material. This is due in part to the observed robustness and tolerance of TiO₂ towards various reagents, including buffers, salts and detergents that are commonly used in biological protein preparations. This metal oxide, either as spherical porous beads or nano-composite material in powder form, has demonstrated high efficacy for enrichment via capture of the phosphate group of phosphopeptides in a bridging bidentate configuration between proximal TiO₂ groups on the surface of the material. This interaction can be disrupted by high pH elution and the enriched phosphopeptides can be further evaluated by mass spectrometry.

[0006] While TiO₂ enrichment represents one of the current best available options for phosphopeptide enrichment, it is not without some significant limitations. First, due to the

similar chemical structure of peptides containing aspartic or glutamic acids compared to phosphorylated peptides, considerable levels of acidic peptides are also captured by TiO_2 . This can be partially overcome by including competing additives (e.g. dihydroxybenzoic acid, glycolic acid) in the binding and wash buffers to compete away some of the acidic peptide binding. Secondly, optimization of the amount of TiO_2 material needed for a given protein extraction has proven to be challenging based on reports indicating that the efficiency of phosphopeptide capture is highly depending on having the correct ratio of TiO_2 to peptides. This means that the optimum ratio must be determined empirically for each sample set thus having a significant impact on the general utility of the method. Another significant challenge is the practical handling of the currently available materials. Typical use of these materials for phosphopeptide enrichments involves preparation of a slurry suspension of the “powdery” material in an appropriate buffer. The material is then packed into micro columns or used as solid phase media in optimized/controlled amounts to capture phosphopeptides. Practical considerations such as weighing out the desired amount of material, transfer of precise amounts from the slurry suspension into each sample and removing the material after eluting the phosphopeptides all add to the variability between experiments.

[0007] Finally, the most commonly used material for these studies (TitansphereTM TiO_2 Bulk Material-beads, GL Sciences Inc., Japan) is only available in one format as highly porous and spherical beads (Figure 1) with limited options for further optimization for phosphopeptide enrichment. Controlling the “peptide-to- TiO_2 beads ratio” that is decided by the surface area of TiO_2 beads has been shown to be a crucial factor in effectively separating the sub-stoichiometric phosphopeptides from the “non-phosphopeptides.” That means the amount (in milligrams) of beads utilized has a significant effect on the number of phosphopeptides identified per milligram of protein. However, the porosities or cavities of the beads are irregular in nature (see Figure 1), indicating these beads provide minimal control of the surface regularity and the surface area.

[0008] TiO_2 bulk material beads with improved phosphopeptide separation efficiency are yet to be reported. This could be due to the minimal surface manipulation opportunities that this type of TiO_2 material provides.

[0009] In recent years, titania nanotube arrays grown by anodic oxidation have emerged as a useful material for a wide variety of applications including: gas sensing, dye sensitized solar cells, hydrogen generation by water photoelectrolysis, organic electronics, microfluidics, molecular filtration, drug delivery, and tissue engineering. Being a highly ordered nanostructure with enormous surface area, titania nanotube arrays have also been investigated for phosphopeptide separation. For example, 250 nm long nanotube arrays, fabricated by anodizing titanium foils in aqueous hydrofluoric acid electrolyte, have been reported as a substrate for surface-assisted laser desorption/ionization mass spectroscopy (SALDI MS). A tryptic digest of β -casein was used it was illustrated that phosphopeptides could be selectively trapped on titania nanotubes. In addition, titania thin nanotube array films prepared on glass and patterned in 'S' shape have recently been reported for phosphopeptide enrichment and found to be useful for differential expression analysis of endogenous phosphopeptides between ovarian cancer patients and healthy woman. Despite these different studies, the ability of these materials to serve as alternative and perhaps superior options to the current standard materials used for phosphoproteomic research has not been confirmed or even explored in detail.

[0010] What is needed, therefore, is a new material form of porous TiO_2 that (1) can readily be immobilized on a given surface (metal or glass), (2) has the ability to be readily quantified in terms of the active surface area, (3) can be manipulated for controlled or variable pore sizes, and most importantly (4) is capable of separating phosphopeptides from their respective "non-phosphorylated" counterparts.

SUMMARY

[0011] The present disclosure pertains to highly ordered titania nanotube arrays for use in phosphopeptide separation and enrichment. These arrays have the prominent advantage of having the ability to immobilize TiO_2 nano tubes on a given surface with the ability to control the active surface area. In preferred embodiments, the highly ordered titania nanotube arrays are radially aligned titanium dioxide nanotubes (TNTs) on titanium wire (Ti-wire).

[0012] The nanotubes can be grown on Ti surfaces using a simple electrochemical process called anodic oxidation that is known for its simplicity and industrial viability. TiO_2 nanotubes have potential in a wide variety of applications, such as in sensors (e.g. hydrogen sensors), in dye sensitized solar cells, in hydrogen generation by water photoelectrolysis, in organic electronics, in microfluidics, in molecular filtration, in drug delivery, and in tissue engineering. The unique self-assembled nanoarchitecture has remarkable utility in CO_2 and water vapor conversion to hydrocarbon fuels, and also in highly efficient solar cells.

[0013] While fabrication of TNT arrays using anodic oxidation is known for its simplicity, cost effectiveness, and industrial viability, the primary advantage of using TNTs on titanium wire for phosphopeptide enrichment is that the surface area can be readily standardized in terms of the length of the wire. One can thus cut the wire into desired lengths to precisely and reproducibly generate the required active surface area for a given phosphopeptide enrichment method. Moreover, the nanotubes grown on wires do not mix into the solution or make colloidal dispersions and hence, in contrast to commonly used TitansphereTM TiO beads, nanotubes-on-wire architecture carries the added benefit of avoiding practical difficulties in separating beads from the solvent medium after elution of the phosphopeptides. In the present disclosure, the efficacy of radially aligned titania nanotubes grown on titanium wire was explored in comparison with the widely used, but expensive TitansphereTM TiO Bulk Material-beads in order to understand if this material could be a low cost alternative for practical use in phosphoproteomic research. It was shown that radially aligned TNTs grown on Ti-wire surfaces are highly suitable for isolating phosphopeptides. Peptides generated from a standard phosphoprotein (α -casein) and mouse liver complex tissue extracts were used. The architecture performed at a comparable level to the standard TitansphereTM TiO_2 Bulk Material-beads, while this medium possesses other desirable attributes mentioned above.

[0014] An example of preferred embodiments of highly ordered TiO₂ nanotubes is shown in Figure 2. Figure 2 shows a tilted surface view of the TiO₂ nanotube array, revealing the ordered porous architecture. As noted above, Figure 1 shows SEM images of the Titansphere™ TiO₂ Bulk Material-beads, illustrating the spherical morphology associated with the beads and their porosity. Figure 3 shows a schematic representation of bidentate interaction of phosphopeptide with TiO₂. Without wanting to be bound by theory, bidentate coordination of hydroxyl groups to positively polarized Ti(IV) on TiO₂ colloidal surface is likely the mode of action that accounts for preferential capture and enrichment of phosphorylated peptides. Previous studies have shown the adsorption of phosphate ions on thin films of colloidal TiO₂ using in situ internal reflection infrared spectroscopy. Similar Langmuir binding constants were also observed for phosphate ions and bidentate ligand species such as oxalate and catechol onto colloidal TiO₂ at low pH (2.3)—inferring bidentate ligation of phosphorylated peptides on to TiO₂ as the mechanism for selective capture of phosphopeptides.

[0015] Although the pore openings in commercially available Titansphere™ TiO₂ Bulk Material-beads are more or less uniformly distributed, the pore size (depth and diameter) is randomly distributed, which limits the opportunities to further optimize the surface area to enhance phosphopeptide enrichment. In contrast, TNTs on Ti wire are highly ordered, with definite pore size and distribution as evident from the SEM images in Figures 3 – 5. The ability to readily control both the length and porosity of TNTs make them useful for further improving how phosphopeptide enrichment is performed in phosphoproteomics profiling workflows. Although titania nanotubes can be grown on various substrates such as titanium, glass, and silicon having different shapes, the practically useful substrates and architectures are those that provide robustness in phosphopeptide enrichment and ease in determining and optimizing the surface area for effective phosphoproteomics profiling. Radially aligned titania nanotubes grown on wire is such an architecture where surface area of nanotubes can be readily standardized in terms of length of the wire so that a user having an idea of the surface area per unit length of the wire can easily cut and use a wire length that provide the desired surface area. Growth of nanotubes on cylindrical shapes such as wires and pipes has been reported, but the utility of these surfaces for phosphopeptide enrichment has not been demonstrated. Thus, the goal of the present study is to provide an insight on the potential of TNTs on Ti-wire as a viable alternative to Titansphere™ TiO₂ Bulk Material-beads for phosphopeptide separations.

[0016] Accordingly, described herein is a material useful for phosphopeptide separation that comprises highly ordered TiO_2 nanotubes grown on Ti metal surfaces. In preferred embodiments, the TNTs are radially aligned on Ti-wire having a variable, optimized length. Anodization of Ti wires per conditions similar to those given below results in the growth of highly ordered nanotubes pointing radially outward from the surface. The highly ordered TiO_2 nanotube array can be immobilized on a surface or made in the form of a self-standing membrane. In preferred methods of using these nanotube arrays, a sample suspected of containing one or more phosphopeptides is exposed to the nanotube arrays which bind the phosphopeptides and separate them from the sample. The separated phosphopeptides are then released from the nanotube arrays and may be subjected to further analysis and identification using any suitable method such as sequencing and a database search.

BRIEF DESCRIPTION OF THE DRAWINGS

[0017] Figure 1 shows a SEM image of a commercially available mesoporous TiO₂ bulk material bead.

[0018] Figure 2 shows a SEM image of a tilted surface view of an example of a TiO₂ nanotube array.

[0019] Figure 3 shows a schematic of bidentate interaction of phosphopeptide with TiO₂.

[0020] Figure 4 shows (A) a cross-sectional SEM image of an as-anodized Ti wire sample showing a titania nanotube layer (having a thickness of about 15 μm) covering the titanium wire (having a diameter of about 0.25 mm) and (B) a schematic representation of the orientation of the nanotubes on the surface of the wire substrate.

[0021] Figure 5 shows SEM images of (A) a side view of a Ti wire covered with TiO₂ nanotubes, with a higher magnification shown in the inset, (B) a side view of nanotubes (having a length of about 10 μm) attached to the Ti wire substrate, (C) a magnified lateral view of the nanotubes, and (D) a view of the top surface of the nanotubes, with a view of the bottom surface of the nanotubes detached from the wire substrate shown in the inset.

[0022] Figure 6 shows SEM images of nanotubes and a rift caused by stress at (A) a magnification of 78.73 K X and (B) a magnification of 50.00 K X.

[0023] Figure 7 shows (A) a high resolution transmission electron microscope (HRTEM) image of a nanotube grown on Ti wire, (B) a HRTEM image of the polycrystalline lattice, and (C) selected area diffraction pattern (SAD) from a few nanotubes showing reflections from anatase phase of titania.

[0024] Figure 8 shows a glancing angle X-ray diffractometer (GAXRD) pattern obtained from a single wire coated with nanotubes.

[0025] Figure 9 shows XPS survey spectrum from a titania nanotube film covered Ti wire, with insets showing high resolution scans of the O 1s and Ti 2p peaks.

[0026] Figure 10 shows a schematic of an experimental workflow for Matrix assisted laser desorption ionization mass spectrometry (MALDI-MS) analysis of tryptic peptides of a phosphoprotein standard, α -casein, 500 μ g was digested using trypsin, to compare phosphopeptide separation of commercially available bulk material beads and examples of a Ti-wire surface grown with TiO₂ nanotubes.

[0027] Figure 11 shows (A) MALDI-mass spectrum of α -casein tryptic peptides, between m/z range 1500-2100, indicating the prominent peptide, 8-HQGLPQEVLENLLR-22 (SEQ ID NO: 1) at m/z 1760.05, less prominent phosphorylated peptide, 104-YKVPQLEIVPN(pS)AEER-119 (SEQ ID NO: 2) at m/z 1952.07, and infinitesimally small response for the phosphorylated peptide 106-VPQLEIVPN(pS)AEER-119 (SEQ ID NO: 3) at m/z 1660.94; and MALDI-mass spectrum of α -casein tryptic peptides, between m/z range 1500-2100, after phosphopeptide separation using (B) commercially available bulk material beads and (C) an example Ti-wire surface grown with TiO₂ nanotubes.

[0028] Figure 12 shows a schematic of an experimental workflow for liquid chromatography-mass spectrometry/tandem mass spectrometry (LC-MS/MS) analysis and identification of mouse liver proteome tryptic peptides to compare phosphopeptide separation capacity of commercially available bulk material beads ("Beads") and examples of Ti-wire surface grown with TiO₂ nanotubes ("Wires").

[0029] Figure 13 shows bar-graphs representing, with unique and high confidence (>95%): (I) average number of phosphopeptides, (II) average number of phosphoproteins, (III) average number of Ser-phosphopeptides, and (IV) average number of Thr-phosphopeptides.

DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

[0030] The present disclosure relates to titania nanotube arrays useful for phosphopeptide enrichment and separation. These highly ordered titania nanotube arrays are a low cost and highly effective alternative to the use of liquid chromatography mass spectrometry (LC-MS) methods using mesoporous titania beads or particles. These beads or particles are expensive and their irregular pore structure offers very limited opportunities for surface manipulation for any further improvement in performance.

[0031] In a preferred embodiment, radially aligned nanotubes were grown by anodic oxidation of titanium wires and their performance was compared to widely used commercially available bulk mesoporous titania beads. Peptides generated from a standard phosphoprotein, α -casein, as well as mouse liver complex tissue extracts were used for the comparison. Example titania nanotubes of length about 10 to about 20 μm , with a pore diameter of about 110 nm and a wall thickness of about 20 nm, demonstrated their capacity to perform on par with the commercially available beads, with further indications that the nanotubes having optimum dimensions could outperform the commercially available phosphopeptide enrichment materials. However, other titania nanotubes having other lengths, pore diameters, and wall thicknesses may also be used, since the optimum dimensions for maximum separation capacity may be outside the ranges recited above. For example, the lengths of the titania nanotubes may range from about 100 nm to about 500 μm , and the pore diameter may range from about 10 nm to about 400 nm.

[0032] Thus, the highly porous nature of the commercially available bulk material, which has been effective for phosphopeptide separation, is also achieved in preferred embodiments of the highly ordered TiO_2 nanotubes grown on Ti metal surfaces. In preferred examples, TiO_2 nanotubes coated on Ti-wires were tested for their capacity for phosphopeptide enrichment, and compared to the phosphopeptide separation capacity of the commercially available bulk material beads as a reference. Ti-wires were chosen for nanotube growth because their quantity and effective surface area for phosphopeptide binding could be simply and appropriately tuned based on the wire length. Ideally, controlled/optimized amounts of TiO_2 -beads for improved phosphopeptide separation and detection should be used. Thus, instead of controlling the weight of small sample amounts of bulk material beads, the length of Ti-wires

bearing titania nanotubes are readily optimized for phosphopeptide separation. Furthermore, the nanotubes coated on Ti wires are immobile, so they do not mix into the solution, hence providing the added benefit of avoiding practical difficulties in separating beads from solvent media. The nanotube array can be immobilized on any suitable solid surface, or it may be utilized without any surface immobilization as a self-stranding membrane. In preferred embodiments, the Ti wire has a diameter from about 0.01 mm to about 1 mm. In additional preferred embodiments, the Ti wire has a diameter of about 0.25 mm.

[0033] In additional preferred embodiments, the titania nanotubes are not grown on Ti wires. Rather, they are grown inside a container such as a vial. The inside of the container is first coated with titanium, then the titanium is anodized to form the TiO_2 nanotubes. Phosphorylated proteins placed inside the container would then attach to the inside of the container.

[0034] Experiments demonstrate that the highly ordered titania nanotube arrays grown on Ti surfaces are highly suitable for isolating phosphopeptides. The arrays perform at an appreciable level as compared to bulk material beads while also possessing other desirable attributes. Importantly, the nanotube dimensions can be further varied in length and diameter, thus one can precisely tune the parameters to further optimize their functionality. In addition, the nanotube-on-wire geometry of preferred embodiments facilitates the use of “length of the wire” as a way to easily assess the surface area for phosphopeptide separation experiments and thus eliminate the need for weighing precisely very small amounts of enrichment material or the variability associated with using slurry suspensions of material as in the case of beads. Furthermore, the nanotube arrays may be made available at a much lower cost than the present commercially available materials. The TNTs on Ti wire embodiments are shown to offer similar efficacy for phosphopeptide enrichment compared to the current best approach, while at the same time offering an enhanced ease-of-use. It should be noted that titania nanotubes are not the only nanotubes expected to show these advantages. For example, nanotubes made of oxides of alloys of titanium and zinc oxide may also be useful.

EXAMPLE 1. MATERIALS, PREPARATION, AND CHARACTERIZATION OF TiO₂ NANOTUBES ON Ti WIRE

[0035] Guanidine:hydrogen chloride (GHCl), ammonium bicarbonate (NH₄HCO₃), Phosphatase inhibitor cocktail 2 (cat. no. P5726), dithiothreitol (DTT), iodoacetamide (IAA), formic acid (HCOOH, FA), trifluoroacetic acid (TFA), α -casein from bovine milk (cat. no. C6780, α s-casein minimum 70%), acetonitrile (CHROMASOLV®, for HPLC, gradient-grade, >99.9%), water (CHROMASOLV®-Plus, for HPLC), α -cyano-4-hydroxycinnamic acid (CHCA), and glycolic acid were purchased from Sigma-Aldrich (St. Louis, MO). For proteomics sample preparation work-flow, deionized water was obtained from an in-house Milli-Q system (Millipore, Bedford, MA). All centrifugation steps were completed in an IEC Micromax RF microfuge at 14,600 RCF (Relative Centrifugal Force). Modified trypsin was obtained from Promega (Madison, WI). Oligo R3 reversed-phase material was obtained from Applied Biosystems (Foster City, CA). For the packing of Oligo R3 reversed phase material, Bio-select extraction columns (reversed phase C4) were obtained from GRACE-VYDAC (W.R. Grace & Co., Deerfield, IL). For TiO₂-chromatography using “beads”, Titansphere TiO₂-beads were obtained from GL Sciences Inc. For TiO₂-chromatography using “wires”, titanium wire of diameter 0.25 mm (99.7% pure) purchased from Sigma Aldrich was used. The electrolyte for anodization of the wire consisted of ammonium fluoride (ACS reagent, 98%, Sigma Aldrich) and ethylene glycol (anhydrous, 99.8%, Sigma Aldrich) and deionized water.

[0036] Ammonium hydroxide (trace-metal grade, assay: 20-22% as NH₃) was obtained from Fisher Scientific (Hampton, NJ) for phosphopeptide elution during TiO₂-chromatography. Whole mouse liver samples were dounce homogenized in the presence of both protease and phosphatase inhibitor cocktails (Jarrold et al. 2005). Protein concentrations were also determined using NIT[™] (Non-Interfering[™]) Protein Assay-Kit purchased from G-BIOSCIENCES.

[0037] The Ti wire (diameter ~0.25 mm) was cut into ~25 mm length and degreased by sonication in acetone and then in isopropanol. The degreased wires were again cleaned sequentially in water and Micro-90, isopropanol and acetone and dried with nitrogen gas. Anodization was conducted at room temperature in an electrolyte consisting of 0.3 wt% NH₄F, 2

vol% H₂O in Ethylene Glycol. The titanium wire was used as anode and platinum foil as cathode. The anodization was performed for 4 h with 60 V applied between the electrodes. The anodized wires were washed and sonicated in isopropanol to remove debris formed on the surface of the nanotubes during the anodization process. The cleaned samples were annealed at 530 °C in oxygen for 3 h (Varghese et al. 2003).

[0038] The morphology of the nanotubes on Ti wire was studied using a field emission scanning electron microscope (FESEM; LEO 15125). The crystal structure was identified using a high resolution transmission electron microscope (HRTEM; JEOL 2010) and glancing angle x-ray diffractometer (GAXRD; Rigaku, Smartlab, Cu K-alpha). An array of three nanotube coated wire was used for GAXRD measurements. The incident angle was 0.5°. The x-ray photoelectron spectroscopy (XPS; Physical Electronics, model 5700) was used to determine the composition of the samples.

[0039] In order to understand the phosphopeptide separation efficiency of the titania nanotube arrays relative to the most utilized material in the field, TiO₂-chromatography was performed in parallel using, (1) the most popularly used and commercially available Titansphere™ TiO₂ Bulk Material-beads as a reference material (“Beads”) and, 2) Ti-wire pieces grown with TiO₂ nanotubes (“Wires”), on a standard phosphoprotein, α -casein and also on mouse liver lysates, to illustrate their phosphopeptide separation capacity, and their applicability in studying complex biological proteomes, respectively. Surfaces of Ti “wire” pieces were modified with TiO₂-nanotubes (see Figure 4), and the wires were particularly chosen so that they could be readily cut into pieces so that effective surface area can be simply be controlled by specific lengths.

[0040] Anodization of titanium wires per the conditions given above resulted in the growth of highly ordered nanotubes pointing radially outward from the surface. The SEM image of the cross section of a nanotube-covered Ti wire sample (diameter ~ 0.25 mm) is given in Figure 4(A) and an expanded view of the nanotubes on the wire surface is schematically represented in Figure 4(B). The growth and self-organization of the nanotubes take place during the anodization process and, without wanting to be bound by theory, are believed to be due to the interplay between electric field assisted oxidation of titanium metal and chemical dissolution as

well as electric field assisted dissolution of the oxide. An alternate model suggests a stress induced displacement of material rather than field assisted dissolution as responsible for the anodic growth of porous structures. Nevertheless, the nanotubes are grown more or less perpendicular to the substrate surface by consuming the metal and converting into oxide regardless of the growth conditions.

[0041] The anodization of titanium in organic electrolytes such as ethylene glycol generally produces anodization debris in the form of particles or nanowires or bunched/broken tubes on the surface of the sample. To remove the debris from the surface of the nanotubes, the wire samples were subjected to ultrasonic agitation at 35 kHz as used normally for other substrates. However, the nanotube films peeled during sonication due to the stress at the oxide/metal interface. The problem was eliminated by performing the ultrasonication at 130 kHz at a reduced power level for 1 to 2 hours. The resulting films were heat treated in oxygen ambient at 530 °C for stoichiometric TiO₂ formation and crystallization (Varghese et al. 2003).

[0042] The low magnification SEM images of a heat treated nanotube coated wire sample are shown in Figure 5(A) and the high magnification images of the nanotubes are given in Figures 5(B)-5(D). The nanotube coating appeared like the bark of a tree (see Figure 5(A) inset) with crevices formed between groups of nanotubes. Studies showed that the crevices were primarily formed during the growth of the nanotubes and not during heat treatment. The images in Figure 6(A) and 6(B) give a closer view of the rift between nanotubes. The nanotubes grown using ethylene glycol electrolyte in planar substrates have a more or less hexagonal close packed geometry. Such a configuration cannot be maintained in a cylindrical substrate geometry especially when the radius is small. The lateral stress across the nanotube film increases as the nanotube length increases and as a result partition is formed between nanotubes to relieve the stress. These observations and conclusions are consistent with those previously reported in which cracks were observed in TNT films on wire substrates. Nonetheless, the nanotubes were not detached from the substrate, rather their alignment changed in the partition region. The nanotubes between the crevices were closely packed as evident from the side and top views of the nanotubes given in Figure 5(B)-5(D). The close packing is maintained from the bottom of the nanotube (see Figure 5(D) inset) to the top. Nanotubes of length about 10 to 20 μm, pore

diameter ~110 nm and wall thickness ~20 nm (measured from SEM images) were used for the study.

[0043] In order to understand the structure and composition of the heat treated nanotubes on wire substrates, HRTEM, GAXRD and XPS studies were performed. Figure 7(A) shows the HRTEM images of a nanotube mechanically separated from the wire substrate. The high resolution image of a nanotube region given in Figure 7(B) shows the polycrystalline lattice. The selected area diffraction pattern (SAD) from a few nanotubes (Figure 7(C)) revealed reflections from anatase phase of titania. GAXRD patterns obtained from a sample of three nanotube coated wires (Figure 8) confirmed that the nanotubes consisted of anatase phase of titania. No other phase was found in the samples. This result was further substantiated by XPS studies. The XPS survey spectrum given in Figure 9 shows the peaks of titanium, oxygen and carbon only. The high resolution scans of O1s and Ti2P peaks are given in the inset. The carbon peak is centered at ~288 eV, which can be attributed to C-O bonds. It is likely that this peak arises from the carbon left on the surface after the burning of the organic electrolyte during heat treatment in oxygen ambient. The stoichiometry of the nanotubes was not estimated as XPS does not provide the composition accurately for nanoporous samples. Nonetheless, significant deviation is not expected from stoichiometry as the pristine oxide samples were heat treated in oxygen ambient. In short, the nanotubes composed of pure titanium dioxide in anatase phase.

EXAMPLE 2. TRYPSIN DIGESTION, DESALTING OF TRYPTIC PEPTIDES, AND SEPARATION OF PHOSHOPEPTIDES USING TIO2-CHROMATOGRAPHY

[0044] As reported previously (Wijeratne et al. 2013), 500 µg aliquots of protein were precipitated with 8 volumes of cold acetone (-20 °C) in 1.5 mL Eppendorf tubes. After centrifugation (14,600 RCF, 5 min), supernatants were discarded and pellets were washed three times using -20 °C acetone (100 µL for each wash). Sample tubes were then kept open in a fume-hood for 2 min to ensure any residual acetone vaporization. The pellets were reconstituted in 3 M Guanidine:HCl in 100 mM NH₄HCO₃ (90 µL) containing phosphatase inhibitor cocktail (2 µL). The solutions were subsequently reduced with DTT (1 mM final concentration, incubated at 37 °C, for 45 min) and then alkylated with iodoacetamide (5.5 mM final concentration, incubated at 37 °C, for 30 min). The solutions were finally diluted with ddH₂O to 1 mL before trypsin-based

digestion. 100 μg of modified trypsin was dissolved in 300 μL of 0.1 M NH_4HCO_3 , and 10 μg aliquots were added into each 500 μg protein sample (i.e. 1:50 weight ratio). Samples were then incubated overnight at 37 $^\circ\text{C}$, and the digestion was quenched by adding 20 μL of formic acid (to bring the pH of solutions to less than 5). After centrifugation, the supernatants were recovered for further processing. Similarly, 500 μg of bovine α -casein was subjected to trypsin digestion for qualitative comparison of phosphopeptide separation using Titansphere TiO_2 Bulk Material-beads (“beads”) and Ti-wire surface grown with TiO_2 nanotubes (“wires”).

[0045] Oligo R3 reversed-phase material was dispersed in ACN/ H_2O /TFA 70/29.9/0.1 (v/v/v) to make a 60 mg/mL slurry as previously described (Wijeratne, et al. 2013; Thingholm, et al. 2008), and divided into 500 μL aliquots each containing 30 mg of Oligo R3 beads in 1.5 mL Eppendorf tubes. The beads prepared for peptide desalting by sequential vortex, spin and removal of the supernatant followed by two wash steps using 200 μL of 0.1% TFA in MilliQH $_2\text{O}$. Peptide solutions were added onto washed Oligo R3 beads and incubated for 30 min at room-temperature using end-over-end rotation. GRACE-VYDAC BIOSELECT-C4 columns (CAT. NO. 214SPE1000) were adapted onto an extraction manifold (Waters Manifold, Massachusetts, USA), washed sequentially with 1) ACN (500 μL), 2) ACN/TFA/ H_2O 70/0.1/29.9 (v/v/v, 200 μL), 3) 0.1% TFA (500 μL) and 4) dd H_2O (500 μL), and then packed with peptide-bound Oligo R3 beads by a gentle application of vacuum into the extraction manifold vacuum chamber. Subsequently, the peptide-bound beads were washed with 500 μL dd H_2O and eluted by sequentially passing 200 μL of ACN/TFA/ H_2O 90/0.1/9.9 (v/v/v) for one time and then 200 μL of ACN/TFA/ H_2O 70/0.1/29.9 (v/v/v) for two times. All elution fractions were collected into 1.5 mL Eppendorf tubes. Prior to TiO_2 -chromatography, these elution fractions were subjected to vacuum centrifugation for complete dryness.

[0046] Phosphopeptide separation of the peptide mixtures was carried out using an optimized strategy adapted from previous reports ((Wijeratne, et al. 2013; Thingholm, et al. 2008; Li, et al. 2009), and was performed in triplicate using identical protein samples for each TiO_2 -chromatographic method. In using the “beads” for phosphopeptide separation, briefly for each replicate, TitansphereTM TiO_2 beads were dispersed in ACN/ H_2O /TFA 80/15/5 (v/v/v) to make a 100 $\mu\text{g}/\mu\text{L}$ slurry and then divided into 5 μL aliquots each containing 500 μg of TiO_2 beads in 0.5 mL Eppendorf tubes. Each vial was subjected to a vortex and spin with supernatants

discarded, followed by 2 additional wash steps using 200 μ L of 0.1% TFA in MilliQH₂O. Dried peptide mixtures (500 μ g) were reconstituted in 200 μ L of 1 M glycolic acid in ACN/H₂O/TFA 80/15/5 (v/v/v), and loaded onto the pre-washed Titansphere TiO₂-beads. The peptides were allowed to interact with the TiO₂ for 30 min at room temperature using end-over-end rotation. The TiO₂ beads were then sequentially washed with 400 μ L ACN/H₂O/TFA 80/15/5 (v/v/v) with a spin and removal of the supernatant followed by an additional 400 μ L wash with the same solvent. Finally the phosphopeptides captured on the TiO₂-beads were eluted 1 time with 200 μ L of 5% NH₄OH. In using the “wires” for phosphopeptide separation, briefly for each replicate, Ti-wire pieces (4 x 0.5 cm, i.e. 2.0 cm in length) grown with TiO₂ nanotubes were placed inside 0.5 mL Eppendorf tubes and subjected to similar washing steps. Following reconstitution of dried peptide mixtures (500 μ g) in 200 μ L of 1 M glycolic acid in ACN/H₂O/TFA 80/15/5 (v/v/v), peptide mixtures were loaded onto the pre-washed Ti-wire pieces grown with TiO₂ nanotubes. TiO₂ “wires” with loaded peptides were then sequentially washed with 400 μ L ACN/H₂O/TFA 80/15/5 (v/v/v) with a spin and removal of the supernatant followed by an additional 400 μ L wash with the same solvent. Finally the phosphopeptides captured on the TiO₂-“wires” were also eluted 1 time with 200 μ L of 5% NH₄OH. The NH₄OH elution fractions were dried by vacuum centrifugation prior to nanoLC-MS/MS analysis. For the standard phosphopeptide mixture obtained from α -casein trypsin digestion, 2.5 μ L aliquots of the elution fractions were removed from each sample, desalted by ZipTip(C-18 μ) as described by the manufacturer (Millipore) and evaluated by Matrix-assisted Laser Desorption Ionization – Time of Flight – Mass Spectrometry (MALDI-TOF-MS) to qualitatively investigate phosphopeptide separation.

[0047] MALDI-MS analysis was performed on a 4800 MALDI-TOF/TOFTM instrument (AB Sciex, Foster city, CA). Mass spectra were obtained in positive ion reflector mode. MALDI-matrix solution was prepared by dissolving α -cyano-4-hydroxy-cinnamic acid (CHCA, 5 mg) in 10 mM ammonium phosphate (monobasic) in ACN/FA/H₂O 60/0.1/39.9 (v/v/v, 1 mL). In order to perform MALDI-MS analyses, desalted (using Oligo R3 reversed phase material or ZipTipTM(C-18 μ)) and isolated peptides in solution (0.5 μ L) were mixed with MALDI-matrix solution (1 μ L), and spots were placed on a calibrated MALDI plate.

[0048] For the qualitative evaluation of phosphopeptide separation capacity of highly ordered TiO₂ nanotubes on Ti-Metal “wires” prepared, phosphopeptide separation experiments were first performed using a standard phosphoprotein, α -casein. As illustrated in Figure 10, tryptic digest from 500 μ g of α -casein was first separated into two identical aliquots, i.e. 250 μ g each, and subjected to OligoR3 based desalting as described in the methods. Prior to performing TiO₂-chromatography, for comparison purposes, a MALDI-mass spectrum (or an MS “finger print”) was obtained for desalted α -casein tryptic digest (Figure 11(A)). During the TiO₂-chromatography step, the desalted tryptic digests were pretreated with both “beads” and “wires”. After washing the captured phosphopeptides and eluting them with ammonia solutions as described in methods, MALDI-mass spectra (or MS “fingerprints”) were obtained (Figures 11(B) from beads and 11(C) from wires). In analyzing the mass spectral regions (m/z 1500 to 2100), after performing TiO₂-chromatography either using “beads” or “wires” on α -casein tryptic digests, the phosphopeptides, 106-VPQLEIVPN(pS)AEER-119 (SEQ ID NO: 3) and 104-YKVPQLEIVPN(pS)AEER-119 (SEQ ID NO: 2) represented by m/z values at 1661.01 and 1952.20, are markedly abundant from both TiO₂-treatments (Figures 11(B) and 11(C)) compare to before TiO₂ treatment (Figure 11(A)). In Figure 11(A), the most abundant peptide response for the α -casein tryptic peptide before TiO₂-treatment is, 8-HQGLPQEVLENLLR-22 (SEQ ID NO: 1) (m/z 1760.05). The responses at m/z 1660.94 and 1952.07 are either infinitesimally small or relatively low in abundance, respectively. This qualitative illustration demonstrates that TiO₂ nanotubes, grown on pieces of Ti-metal wire can be used to enrich phosphopeptides in a comparable manner to TiO₂ beads.

EXAMPLE 3. PHOSPHOPEPTIDE SEPARATION CAPACITY FOR PHOSPHOPROTEOMES OF COMPLEX TISSUE SAMPLES

[0049] In real biological protein samples or proteomes, it is known that phosphorylation is sub-stoichiometric or very low in abundance. Thus, separation of phosphopeptides from a purified standard phosphoprotein sample like the test case with α -casein may have different dynamics to that of a complex digestion derived from a tissue extract. Hence, the capacity of the highly ordered TiO₂ nanotubes in phosphopeptide separation for studying complex phosphoproteomes derived from tissue extracts was also compared with respect to the widely used TitansphereTM TiO₂ Bulk Material-beads.

[0050] Nano-LC-MS/MS analyses were performed on a TripleTOFTM 5600 (ABSciex, Toronto, ON, Canada) coupled to an Eksigent (Dublin, CA) nanoLC.ultra nanoflow system. Dried phosphopeptide samples were reconstituted in FA/H₂O 0.1/99.9 (v/v) and loaded onto IntegraFrit Trap Column (outer diameter of 360 μ m, inner diameter of 100, and 25 μ m packed bed) from New Objective, Inc. (Woburn, MA) at 2 μ l/min in FA/H₂O 0.4/99.2 (v/v) for 10 min to desalt and concentrate the samples. For the chromatographic separation of peptides, the trap-column was switched to align with the analytical column, Acclaim PepMap100 (inner diameter of 75 μ m, length of 15 cm, C18 particle sizes of 3 μ m and pore sizes of 100 Å) from Dionex-Thermo Fisher Scientific (Sunnyvale, CA). The peptides were eluted using a varying mobile phase (MP) gradient from 95% phase A (FA/H₂O 0.4/99.6, v/v) to 40% phase B (FA/ACN 0.4/99.6, v/v) for 70 min, from 40% phase B to 85% phase B for 5 min and then keeping the same MP-composition for 5 more minutes at 300 nL/min.

[0051] Nano-LC mobile phase was introduced into the mass spectrometer using a NANOSpray[®] III Source (AB Sciex, Toronto, On, Canada). Ion source gas 1 (GS1) was zero grade air while ion source gas 2 (GS2) and curtain gas (CUR) were both nitrogen. The “gas settings” were kept at 7, 0 and 25 respectively in vendor specified arbitrary units. Interface heater temperature and ion spray voltage was kept at 150 °C, and at 2.3 kV. The mass spectrometer method was operated in positive ion mode set to go through 4156 cycles for 90 minutes, where each cycle consisted of one TOF-MS scan (0.25 s accumulation time, in a 400 to 1600 m/z window) followed by twenty information dependent acquisition (IDA) mode MS/MS-scans on the most intense candidate ions selected from initially performed TOF-MS scan during each cycle, having a minimum of 150 counts. Each product ion scan was operated under vendor specified high-sensitivity mode with an accumulation time of 0.05 secs and a mass tolerance of 50 mDa. Former MS/MS-subjected candidate ions were excluded for 10 s after its first occurrence, and data were recorded using Analyst[®]-TF (1.5.1) software.

[0052] The nano-LC-MS/MS data (*.wiff file) from the enriched phosphopeptides were analyzed for peptide/protein identification using ProteinPilotTM software (version 4.2, revision 1297) that integrates the ParagonTM algorithm, searched against a SwissProt database of *Mus Musculus* protein sequences on a local 12-processor server. A custom “sample-type” was selected that specifies variable biological modifications as specified defaults in the ProteinPilot

software. The vendor defined phosphorylation emphasis on serine/threonine/tyrosine was also used as a special factor. The resulting *.group files were then used to generate a spreadsheet as a peptide summary report. Only those phosphopeptides identified with a minimum of 95% confidence in identity (calculated by probability algorithms of ProteinPilot™ software), and phosphorylation as a modification were selected as viable phosphopeptide identifications. Unique phosphopeptides were then selected based on sequence, modifications, and mass to charge ratio (m/z-value) using available software tools on Microsoft Excel. Tools made available by Microsoft Excel were used to determine the number of unique phosphopeptides for each replicate and each TiO₂-chromatography method employed.

[0053] In order to examine the capability of TiO₂ nanotubes for phosphopeptide separation in proteomes of complex samples, it was hypothesized that the number of high confidence (>95%) unique phosphopeptides identified using LC-MS/MS and database search algorithms is representative of the phosphopeptide separation capacity in a single phosphopeptide isolation. Hence, an experimental workflow, as depicted in Figure 12, was implemented and analyzed for unique phosphopeptide identifications. More specifically, from a single pool of mouse liver lysate, as described in the methods, six identical protein solutions (500 µg each) were sequentially subjected for protein precipitation, trypsin digestion, OligoR3 based desalting and phosphopeptide separation using TiO₂-chromatography. In performing TiO₂-chromatography with “beads”, 500 µg equivalents of Titansphere™ TiO Bulk Material-beads were used. For the “wires”, 2 cm (0.5 cm x 4) of Ti-wire pieces grown with highly ordered TiO₂ nanotubes were used. The surface area of Titansphere™ TiO Bulk Material-beads given by the manufacturer is 100 m²/g and therefore, the surface area of 500 µg beads is about 0.05 m². The surface area of the nanotubes (pore diameter ~ 110 nm, wall thickness ~ 20 nm and length about 15 µm) on a 2 cm long wire of diameter 0.25 mm was calculated using a method reported elsewhere (Varghese, et al. 2009; Shankar, et al. 2007) and is about 0.01 m². Thus, the Titansphere™ TiO beads used were having surface area about 5 times the surface area of nanotubes. For comparison purposes, triplicate of 1 µg equivalent tryptic digests from mouse liver proteome, were also analyzed using LC-MS/MS, so that “non-phosphopeptide separation” was compared to phosphopeptide separation by either “beads” or “wire” based TiO₂-chromatography methods. It was assumed that 1 µg equivalent of tryptic digest analysis in LC-MS from a mouse liver could be used to illustrate the sub-stoichiometric nature of

phosphopeptides, and comparison of phosphopeptides identified in such an analysis is illustrative of the separation capacity in using either TiO₂-chromatography methodologies. Nevertheless, following all LC-MS/MS analyses/runs of each sample, as described in the methods, each LC-MS/MS run was subjected to database searches to identify high confidence (>95%) unique phosphopeptides. The confidence values were assigned for phosphopeptide identifications from the Paragon probabilistic algorithms used in ProteinPilot search software.

The average number of high confidence phosphopeptides (Paragon plus algorithm assigned confidence >95%) identified and their average number of representative phosphoproteins were presented as bar-graphs, Figure 13 (I & II) for each “beads” and “wire” TiO₂-chromatography. In each graph represented in Figure 13, 1—“No Separation” represents the number of phosphopeptides identified in analyzing 1 µg equivalent of tryptic digest using LC-MS/MS with no TiO₂-chromatography performed, 2—“Separation with Beads”, and 3—“Separation with Wires” represent number of phosphopeptides identified in analyzing 500 µg equivalent of tryptic digest using LC-MS/MS with TiO₂-chromatography performed using, Titansphere™ TiO₂ Bulk Material-beads and Ti-wire surface grown with TiO₂ nanotubes, respectively. In inspecting Figure 13 (I & II), it is apparent that, although the surface area is lower, “wires” carry appreciable capacity (average number of phosphopeptides detected, 486.67 ± 8.41) to isolate phosphopeptides in reference to that observed when spherical “beads” are utilized (average number of phosphopeptides detected, 541.00 ± 12.50). In performing TiO₂-chromatography for phosphoproteomics studies, it has been well understood that phosphopeptides identified are phosphorylated mostly at serine (Ser or S) and then at threonine (Thr or T) amino acid residues. Thus, the average unique number of high confidence S-phosphopeptides and T-phosphopeptides identified were also plotted as bar-graphs—Figure 13 (III & IV) for evaluation. It is evident that the “wires” carry a more or less similar capacity to isolate Ser-phosphorylated peptides (390.33 ± 3.67) and Thr-phosphorylated peptides (18.65 ± 1.66), compared to peptides identified with Ser-phosphorylation (460.67 ± 11.86) and Thr-phosphorylation (13.88 ± 2.18) when “beads” are employed. Overall, these results demonstrate that the highly ordered TiO₂ nano tubes immobilization on Ti-metal wires carry significant potential as an alternate medium that can be utilized for mass spectrometry based phosphoproteomics workflows.

WHAT IS CLAIMED IS:

1. A method for isolation of phosphopeptides in a sample, comprising:
growing ordered TiO₂ nanotubes on a Ti surface, wherein the nanotubes point outward from the Ti surface, to produce an ordered TiO₂ nanotube array;
contacting the ordered TiO₂ nanotube array with the sample to produce bound phosphopeptides attached to the ordered TiO₂ nanotube array; and
releasing the bound phosphopeptides from the ordered TiO₂ nanotube array to produce isolated phosphopeptides.
2. The method of claim 1, wherein the ordered TiO₂ nanotubes have a length of about 100 nm to about 500 μ m and a pore diameter of about 10 nm to about 400 nm.
3. The method of claim 1, wherein the ordered TiO₂ nanotubes have a length of about 10 to about 20 μ m, a pore diameter of about 110 nm, and a wall thickness of about 20 nm.
4. The method of claim 1, wherein the ordered TiO₂ nanotubes are grown on the Ti surface by anodic oxidation.
5. The method of claim 1, wherein the Ti surface is a Ti wire and wherein the nanotubes point radially outward from the Ti wire.
6. The method of claim 5, wherein the Ti wire has a diameter of about 0.01 mm to about 1 mm.
7. The method of claim 5, wherein the Ti wire has a diameter of about 0.25 mm.
8. The method of claim 1, wherein the ordered TiO₂ nanotube array is immobilized on the Ti surface.
9. The method of claim 1, wherein the Ti surface is an internal surface of a container, and wherein the internal surface of the container has been coated with Ti.

10. The method of claim 1, wherein the Ti surface is a surface coated with Ti, and wherein the surface is metal, glass, silicon, plastic, or rubber.
11. A device for isolation of phosphopeptides in a sample, comprising:
an ordered TiO₂ nanotube array comprising ordered TiO₂ nanotubes grown on a Ti surface, wherein the nanotubes point outward from the Ti surface; and
a container for phosphopeptide isolation, wherein the ordered TiO₂ nanotube array is located within the container, and wherein the sample is placed in the container to contact the ordered TiO₂ nanotube array.
12. The device of claim 11, wherein the ordered TiO₂ nanotubes have a length of about 100 nm to about 500 μ m and a pore diameter of about 10 nm to about 400 nm.
13. The device of claim 11, wherein the ordered TiO₂ nanotubes have a length of about 10 to about 20 μ m, a pore diameter of about 110 nm, and a wall thickness of about 20 nm.
14. The device of claim 11, wherein the Ti surface is a Ti wire and wherein the nanotubes point radially outward from the Ti wire.
15. The device of claim 14, wherein the Ti wire has a diameter of about 0.01 mm to about 1 mm.
16. The device of claim 14, wherein the Ti wire has a diameter of about 0.25 mm.
17. The device of claim 11, wherein the ordered TiO₂ nanotube array is immobilized on the Ti surface.
18. The device of claim 11, wherein the Ti surface is an internal surface of a container, and wherein the internal surface of the container has been coated with Ti.
19. The device of claim 11, wherein the Ti surface is a surface coated with Ti, and wherein the surface is metal, glass, silicon, plastic, or rubber.

Figure 1

PRIOR ART

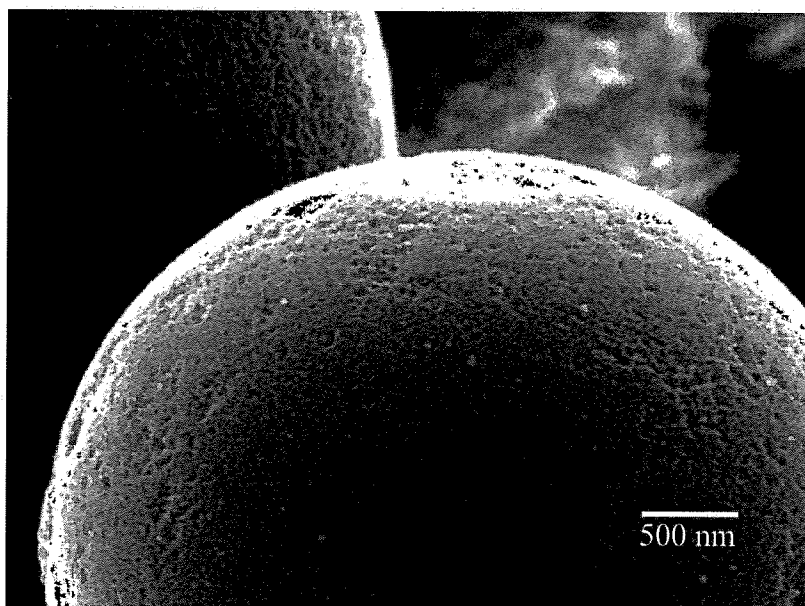


Figure 2

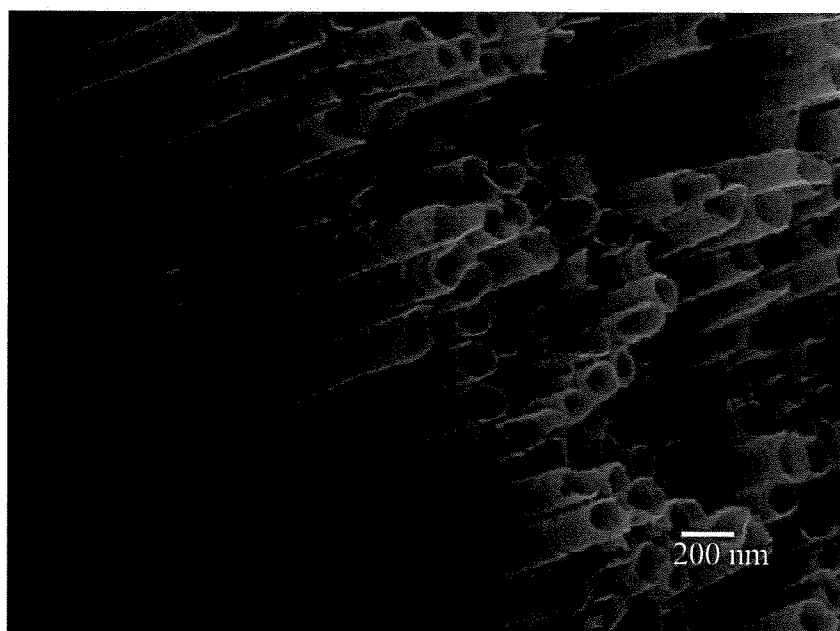


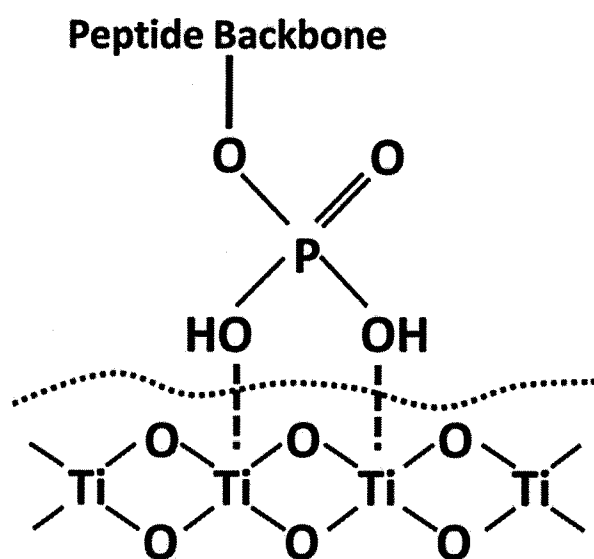
Figure 3

Figure 4

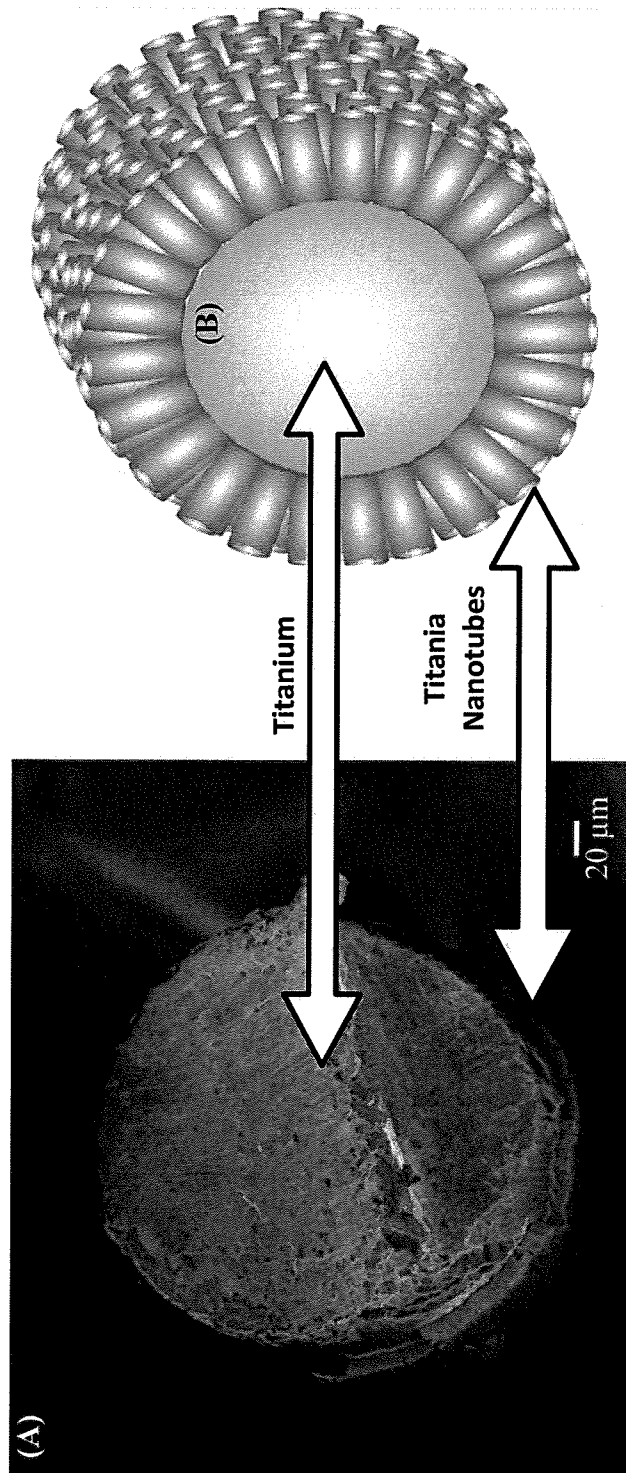


Figure 5

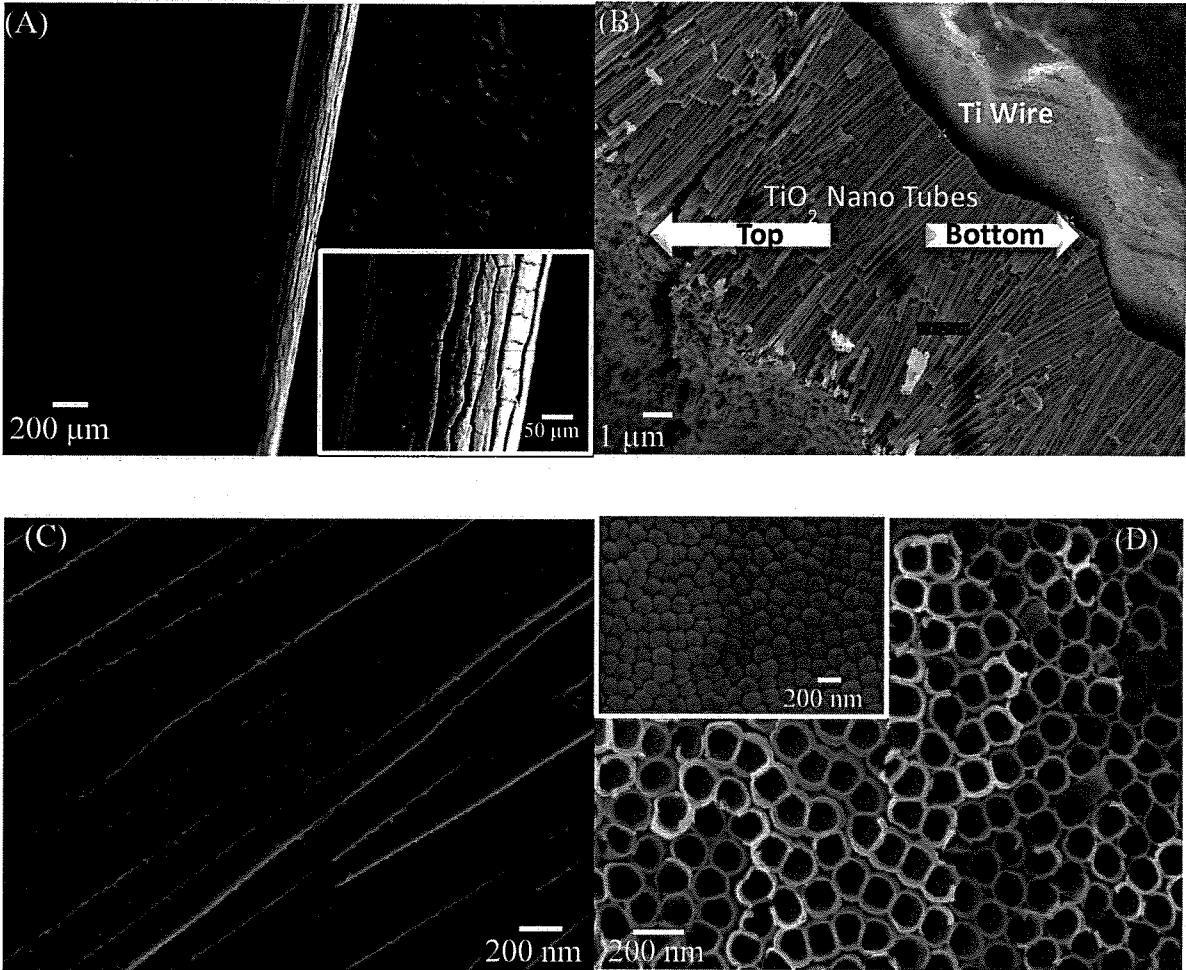


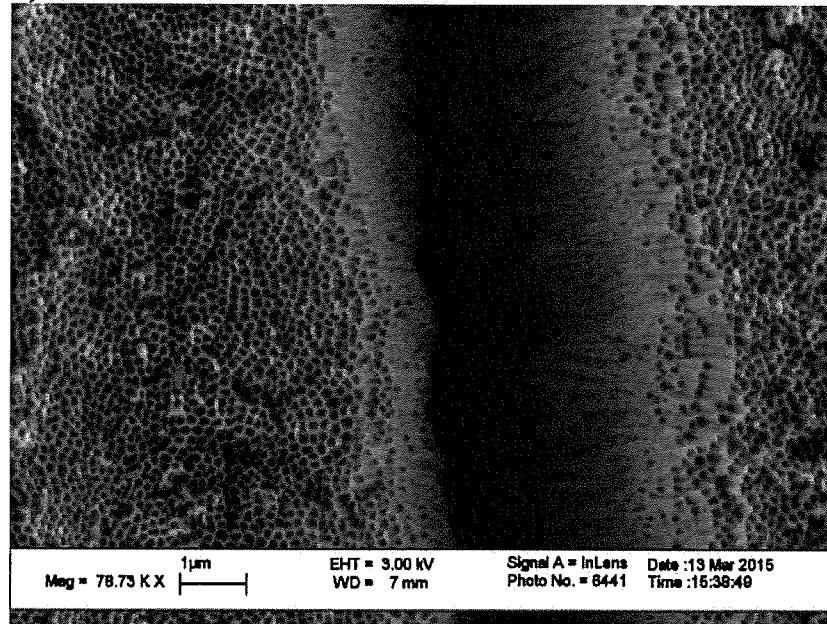
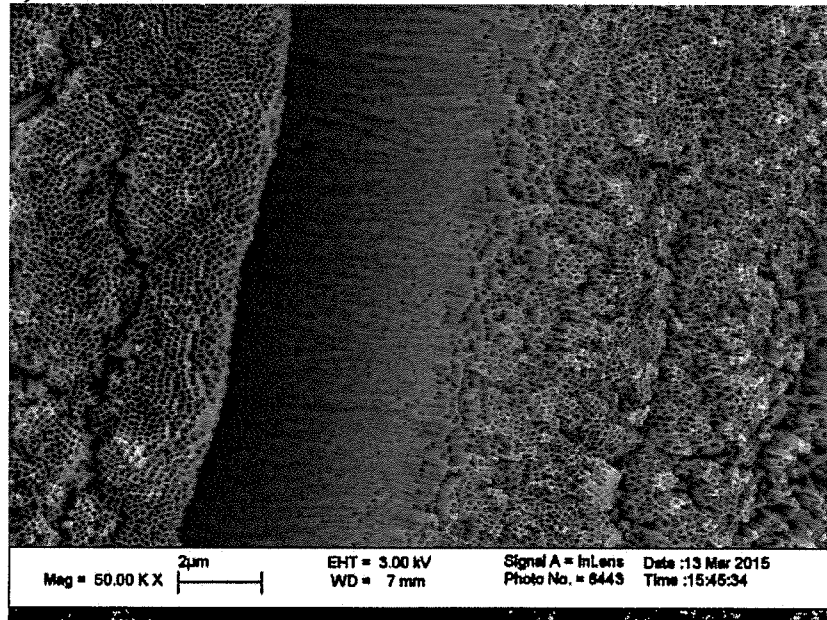
Figure 6**A)****B)**

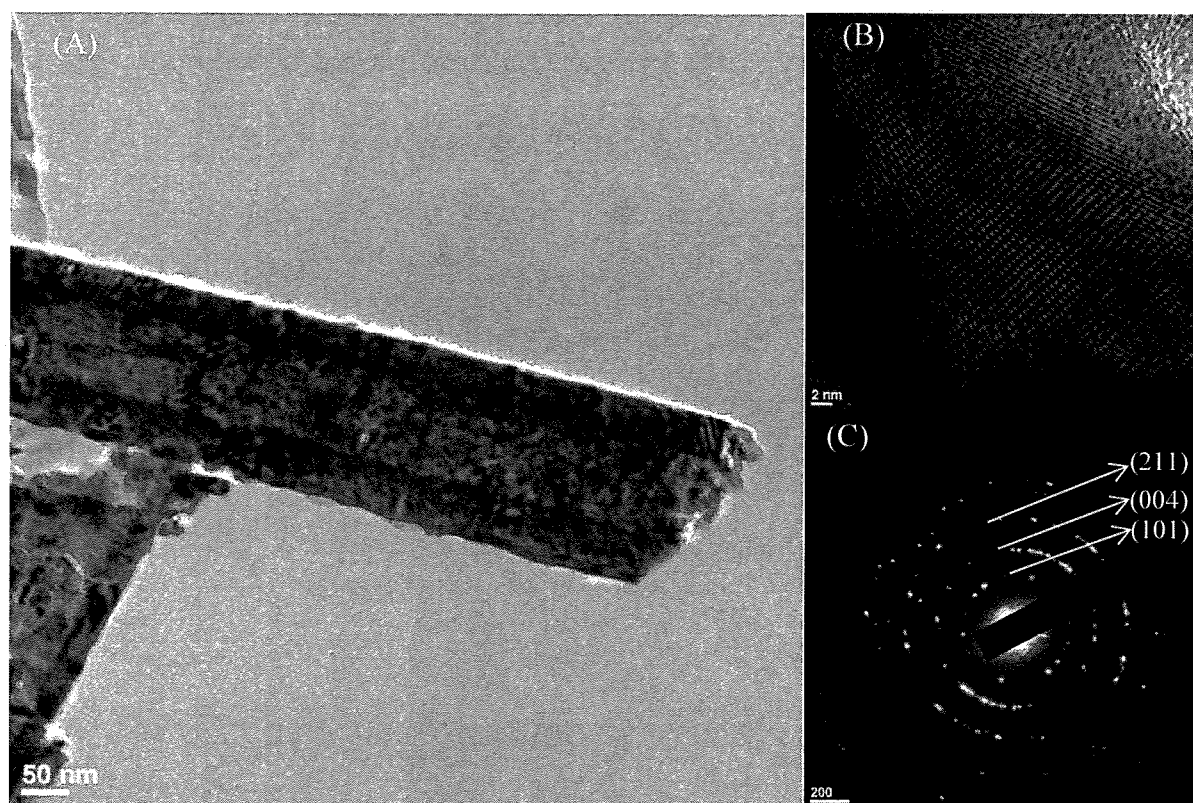
Figure 7

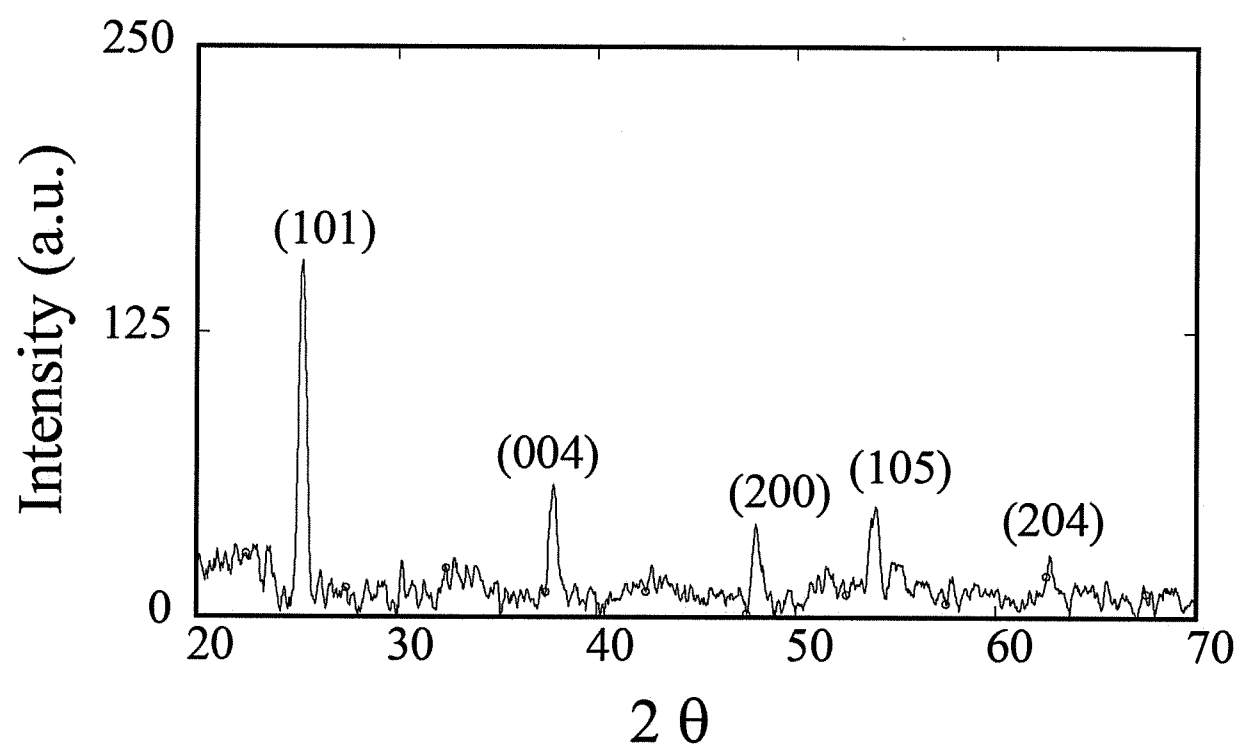
Figure 8

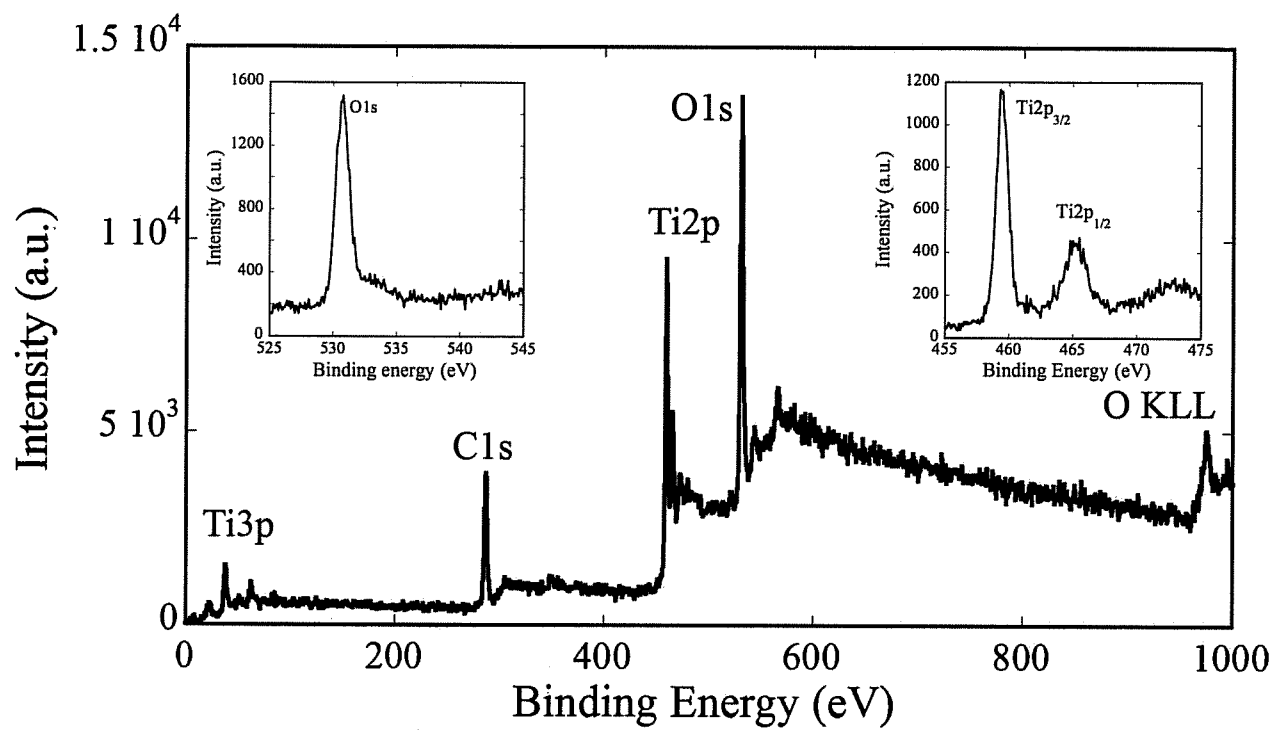
Figure 9

Figure 10

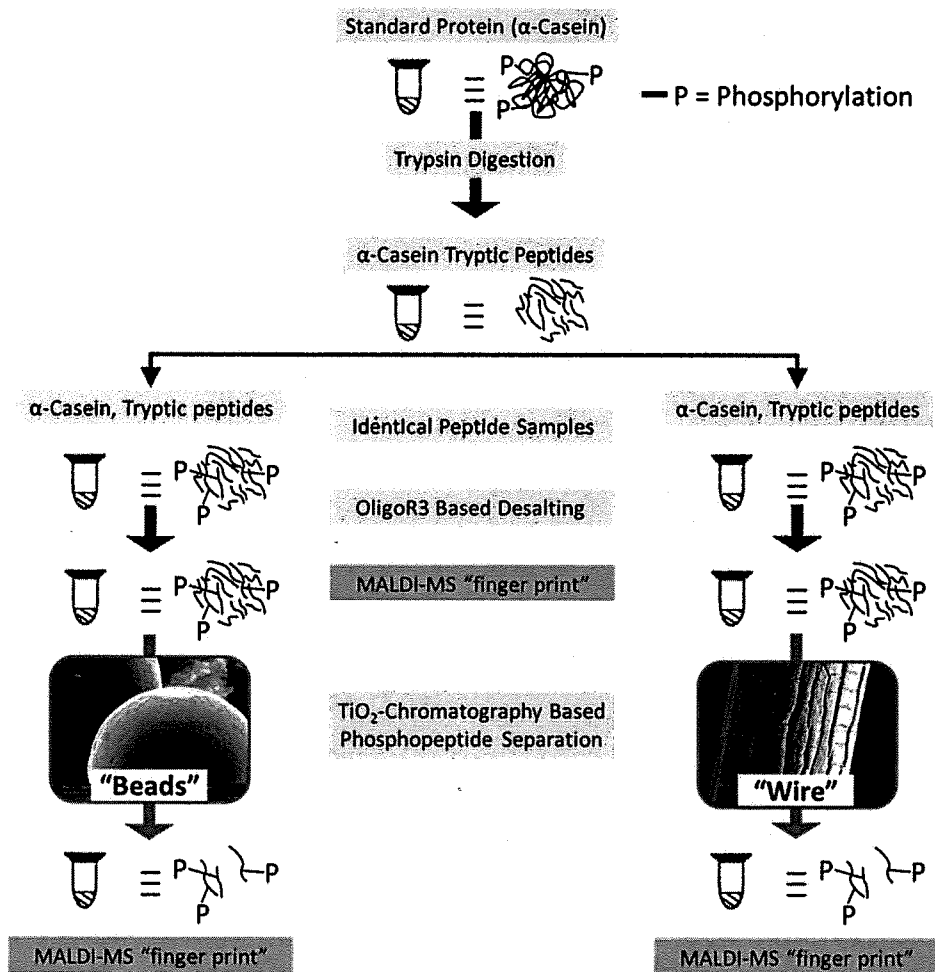


Figure 11

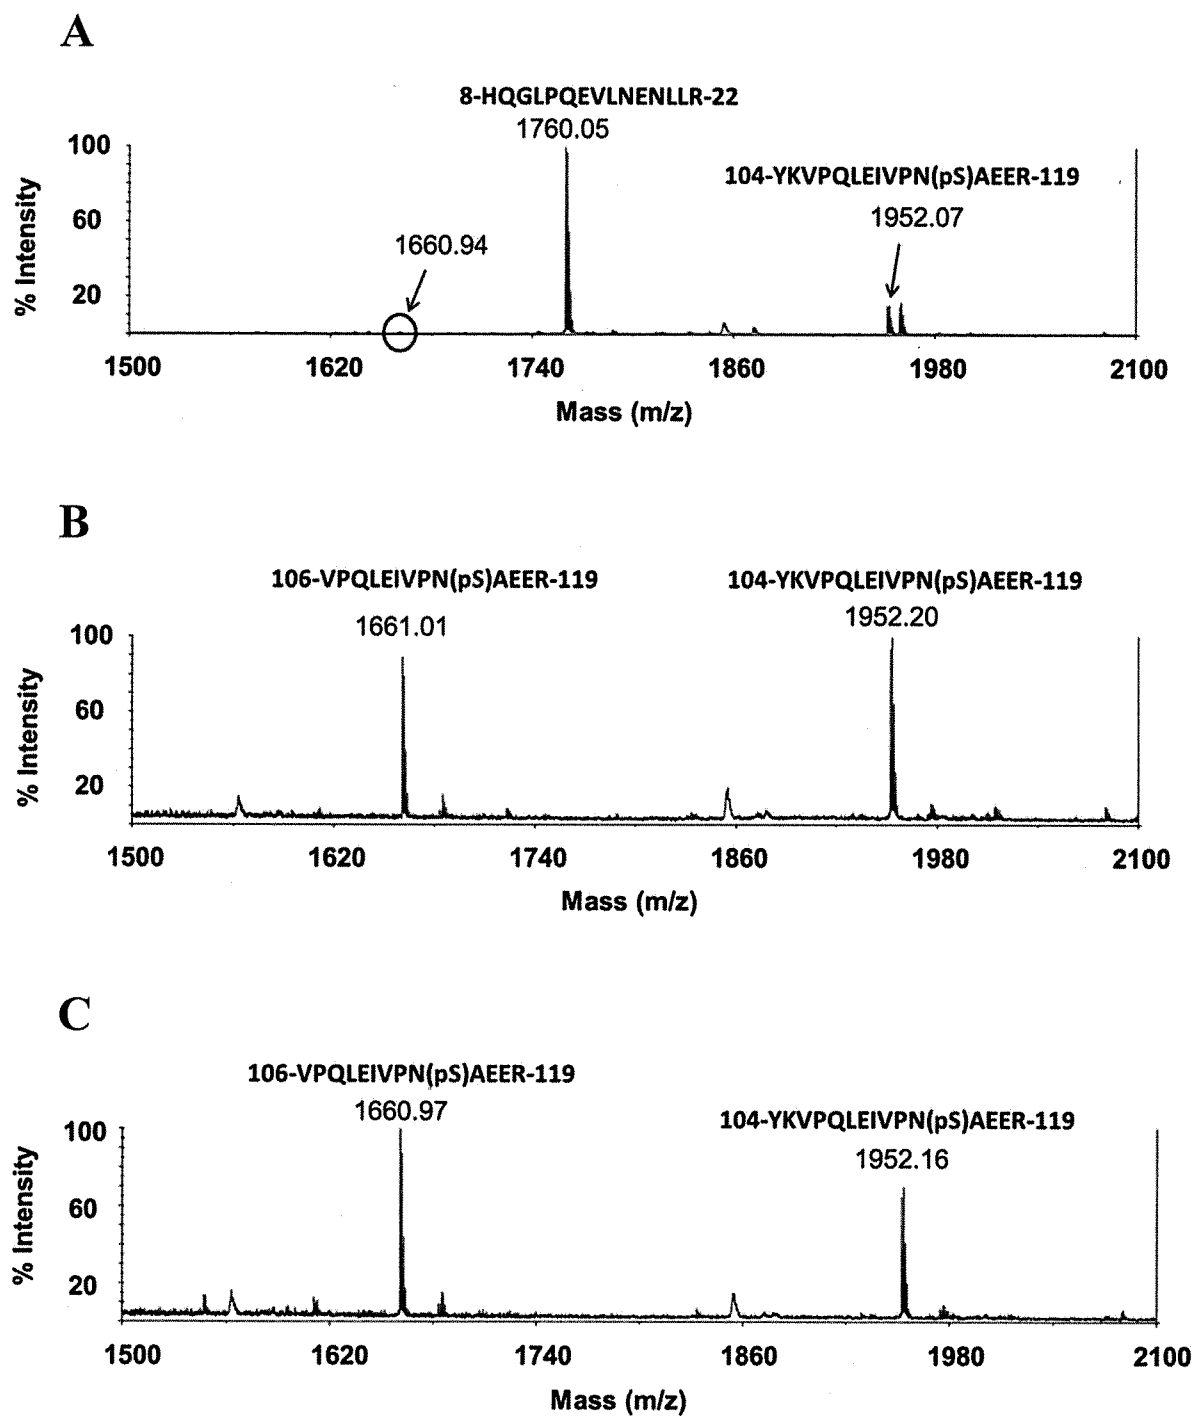
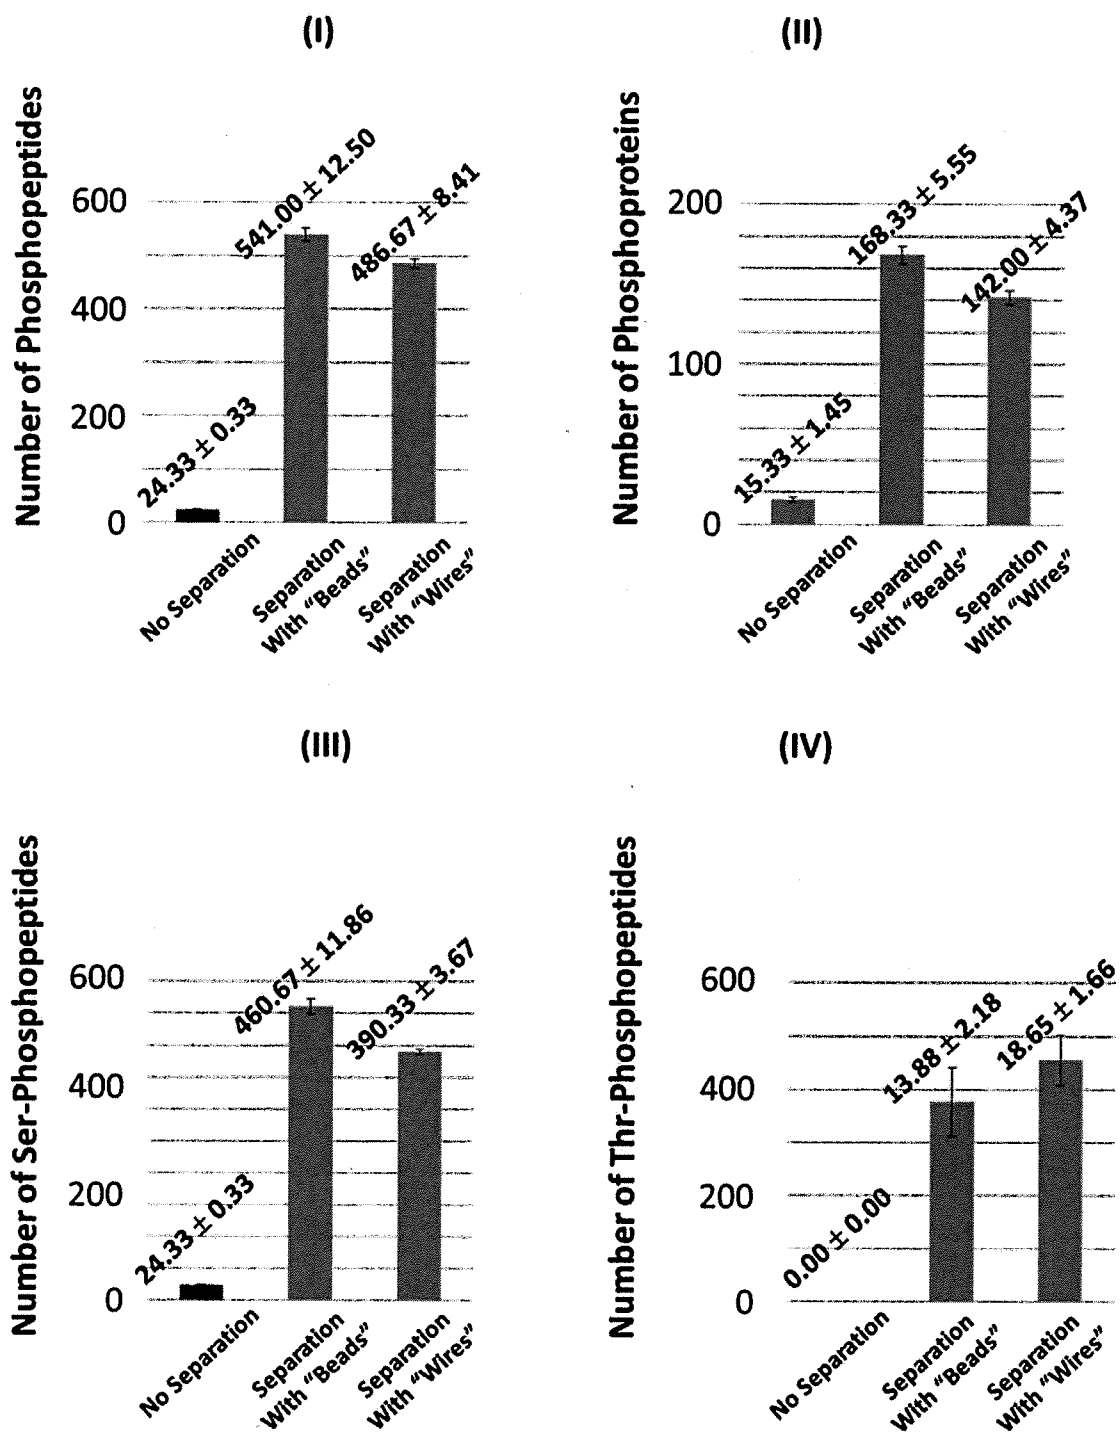


Figure 13



INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2015/065696**A. CLASSIFICATION OF SUBJECT MATTER****G01N 30/06(2006.01)i, G01N 30/72(2006.01)i, G01N 27/64(2006.01)i, G01N 33/68(2006.01)i, C01G 23/047(2006.01)i, B01J 20/02(2006.01)i, C07K 1/14(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

G01N 30/06; C12N 11/14; G01N 30/72; G01N 27/64; G01N 33/68; C01G 23/047; B01J 20/02; C07K 1/14

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: isolation, phosphopeptide, TiO₂ nanotube array, Ti surface, bind, anodic oxidation**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	MIN et al., Tailoring of a TiO ₂ nanotube array-integrated portable microdevice for efficient on-chip enrichment and isotope labeling of serum phosphopeptides, Lab on a Chip, 2013, Vol. 13, No. 19, pp. 3853-3860 See pages 3853-3860.	1-19
X	LO et al., Surface-assisted laser desorption/ionization mass spectrometry on titania nanotube arrays, Journal of the American Society for Mass Spectrometry, 2008, Vol. 19, No. 7, pp. 1014-1020 See pages 1014-1019.	1-19
A	US 2014-0308728 A1 (THE UNIV. OF N. CAROL. AT CHAPEL HILL) 16 October 2014 See paragraphs [0003], [0006], [0023]-[0197]; claims 1-36; and figures 1-13.	1-19
A	YAO et al., Enhanced osteoblast functions on anodized titanium with nanotube-like structures, Journal of Biomedical Materials Research Part A, 2008, Vol. 85, No. 1, pp. 157-166 See pages 157-165.	1-19



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

18 February 2016 (18.02.2016)

Date of mailing of the international search report

02 March 2016 (02.03.2016)

Name and mailing address of the ISA/KR

International Application Division

Korean Intellectual Property Office

189 Cheongsu-ro, Seo-gu, Daejeon, 35208, Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

CHANG, Bong Ho

Telephone No. +82-42-481-3353



INTERNATIONAL SEARCH REPORT

International application No.

PCT/US2015/065696

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	LI et al., Novel Fe ₃ O ₄ @TiO ₂ core-shell microspheres for elective enrichment of phosphopeptides in phosphoproteome analysis, J. of Proteome Research, 2008, Vol. 7, No. 6, pp. 2526-2538 See pages 2526-2537.	1-19
PX	WIJERATNE et al., Phosphopeptide separation using radially aligned titania nanotubes on titanium wire, ACS applied Materials & Interfaces, 2015, Vol. 7, No. 21, pp. 11155-11164 (Web Publication Date: 05 May 2015) See pages 11155-11163.	1-19

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2015/065696Patent document
cited in search reportPublication
datePatent family
member(s)Publication
date

US 2014-0308728 A1

16/10/2014

None