

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
21 April 2005 (21.04.2005)

PCT

(10) International Publication Number
WO 2005/035040 A1

(51) International Patent Classification⁷: **A61M 25/00**

(21) International Application Number:
PCT/US2004/027876

(22) International Filing Date: 27 August 2004 (27.08.2004)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
10/670,625 25 September 2003 (25.09.2003) US

(71) Applicant (for all designated States except US): **C. R. BARD, INC.** [US/US]; 730 Central Avenue, Murray Hill, NJ 07974 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **TRIPLETT, Daniel, J.** [US/US]; 583 South 225 East, Providence, UT 84332 (US). **WEINTRAUB, Robert** [US/US]; 12987 S. Brookhaven Cove, Draper, UT 84020 (US).

(74) Agents: **WIGHT, Todd, W.** et al.; Morrison & Foerster LLP, 555 W. Fifth Street, Suite 3500, Los Angeles, CA 90013 (US).


(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:
— with international search report

[Continued on next page]

(54) Title: PRE-MOLDED BIFURCATION INSERT

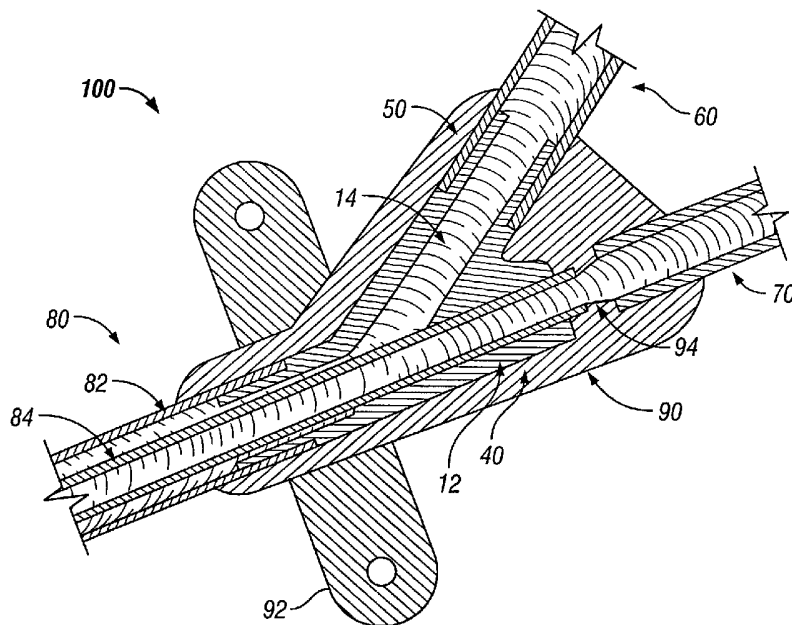

(57) Abstract: A bifurcation insert for a coaxial catheter and a assembly incorporation the bifurcation insert. The bifurcation insert contains an opening at a distal end and two openings in a proximal end, the distal end being configured for positioning within a proximal end of an outer lumen of the coaxial catheter. At the proximal end of the bifurcation insert, an arterial side is configured to receive a first extension tube, while a venous side is configured to receive a second extension tube. The catheter assembly incorporating the bifurcation insert includes a hub that is molded around the insert and properly positioned extension tubes and coaxial catheter such that each component is set into place with respect to one another.



For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

PRE-MOLDED BIFURCATION INSERT

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] Not applicable.

STATEMENT REGARDING FEDERALLY SPONSORED RESEARCH OR DEVELOPMENT

[0002] Not applicable.

REFERENCE TO A COMPACT DISK APPENDIX

[0003] Not applicable.

BACKGROUND OF THE INVENTION

[0004] Coaxial catheters are well-known in the art, being used for applications such as hemodialysis, where separate lumens are necessary to simultaneously remove blood from and return treated blood to a patient. Examples of coaxial catheters for use in hemodialysis treatments can be found in USPN 5,976,103 to Martin. Such coaxial catheters, generally comprised of one or more inner catheters disposed within an outer catheter, are conventionally connected to extension tubing for the purpose of attachment to a dialysis or other treatment device.

[0005] This is generally accomplished by molding a hub over the proximal end of the catheter, which transforms the coaxial configuration of the lumens to a side-by-side configuration so that the extension tubing will lay flat against a patient's skin. The extension tubing is then connected to the hub post-processing via a barbed fitting or the equivalent as shown in USPN 5,053,004 to Markel et al. The hub overmolding process is typically conducted after first inserting a cylindrical pin into an innermost catheter and C-shaped pins into the other catheter(s). Once the molding process is complete, the pins are removed and separate channels are created for the extension tubing.

[0006] There are drawbacks, however, to the above-described standard method. First, use of a post-processing connection system for the extension tubing as opposed to overmolding the hub with the extension tubing in place, provides a much

weaker connection and one that can become prone to detachment with higher flow rates. Second, use of C-shape rods in the overmolding process can result in flow disturbances and inefficiencies in a functioning catheter, as well as the formation of bubbles, which causes turbulent flow.

[0007] For these and other reasons, it would be advantageous to provide a single bifurcation insert for connection to both the catheter and extension tubing prior to a hub overmolding process to provide a complete product that avoids the common drawbacks associated with the standard manufacturing methods of a multi-lumen catheter with respect to a proximal hub for attachment thereto.

BRIEF SUMMARY OF THE INVENTION

[0008] Accordingly, a primary object of the present invention is to provide a single bifurcation insert for coaxial catheters, which itself becomes a component of the multi-lumen catheter system. It is another object of the present invention to provide a connection system for extension tubing, which does not detach from the hub under the presence of high flow rates. It is still another object of the present invention to provide a pre-defined fluid path for the lumens of a coaxial catheter that will enable seamless fluid flow between the extension tubing and the respective catheter lumens. It is yet another object of the present invention to provide an efficient and cost-effective method of attaching extension tubing to catheters. Various other objectives and advantages of the present invention will become apparent to those skilled in the art as more detailed description is set forth below.

[0009] In accordance with the present invention, several embodiments are described, which may be improvements to bifurcation assembly methods or may be novel hub embodiments heretofore undisclosed. As used herein, the term "venous" denotes the catheter, extension tubing or side of the insert/assembly through which cleansed blood is infused to a patient, while the term "arterial" denotes the catheter, extension tubing, or side of the insert/assembly through which blood to be cleaned is withdrawn from the patient.

[0010] The present invention is directed to a bifurcation insert for coaxial catheters as well as a catheter assembly including a bifurcation insert. The bifurcation

insert has a distal opening and two proximal openings, one each for the venous and arterial sides. Within the bifurcation insert is two passageways, a first extending from the distal opening to the venous side opening and the second extending from the first passageway to the arterial side opening. At the distal opening and arterial side opening, an outer wall is tapered, resulting in a shoulder so that placement within the outer lumen and first extension tube respectively is facilitated.

[0011] The catheter assembly is constructed by placing the bifurcation insert within a proximal end of an outer lumen of a coaxial catheter such that an outer wall of the outer lumen abuts the shoulder at the distal end of the insert. A first extension tube is positioned over the arterial side opening and an outer wall thereof abuts a shoulder adjacent the opening. A second extension tube is positioned in close proximity to an inner lumen, which itself is positioned through the outer lumen of the coaxial catheter and a first passageway of the bifurcation insert, exiting the venous side proximal opening. Pins are placed through the extension tubes and into the arterial side opening and inner lumen, respectively. A hub is overmolded around the assembled parts, locking in place the parts with respect to one another and creating a sealed assembly, after which the pins are removed.

[0012] A more complete understanding of the bifurcation insert of the present invention will be afforded to those skilled in the art, as well as a realization of additional advantages and objects thereof, by a consideration of the following detailed description of the preferred embodiments. Reference will be made to the appended sheets of drawings that will first be described briefly.

BRIEF DESCRIPTION OF THE DRAWINGS

[0013] FIG. 1 is a side perspective view of a bifurcation insert according to the present invention.

[0014] FIG. 2 is a cross-sectional view of the bifurcation insert of FIG. 1.

[0015] FIG. 3 is a cross-sectional view of an assembled catheter system with an integral bifurcation insert.

DETAILED DESCRIPTION OF THE INVENTION

[0016] The following detailed description should be read with reference to the drawings, in which like elements in different drawings are identically numbered. The drawings, which are not necessarily to scale, depict selected preferred embodiments and are not intended to limit the scope of the invention.

[0017] The detailed description illustrates by way of example, not by way of limitation, the principles of the invention. This description will clearly enable one skilled in the art to make and use the invention, and describes several embodiments, adaptations, variations, alternatives and uses of the invention, including what is presently believed to be the best mode of carrying out the invention.

[0018] The present invention satisfies the need for a bifurcation insert for coaxial catheters as an integral component of a multi-lumen catheter system, as well as the need for a reliable, efficient and uniform method of connecting a coaxial catheter to extension tubing. Although the bifurcation insert is described below in connection with a dual-lumen coaxial catheter, it is contemplated that the bifurcation insert could have other applications as well where there is a need to connect passageways together. Further, while a preferred material for the bifurcation insert according to the present invention is plastic, there are many other possible materials that could be utilized that would be within the scope of the present invention, such as stainless steel, titanium, nitinol and epoxy, to name a few. Moreover, while it is contemplated that the bifurcation insert would be formed by a molding process, other methods of fabricating the insert are also possible, such as traditional machining and sintering.

[0019] Referring now to FIG. 1, a bifurcation insert 10 is illustrated, having a distal end 20 and a proximal end 30. The distal end 20 has a tapered portion 22, containing a shoulder 26 and a distal opening 24, the shoulder 26 being configured for abutment with a wall of an outer lumen of a coaxial catheter arrangement as explained below in connection with FIG. 3. The proximal end 30 opens in two locations, having a venous side 40 and an arterial side 50. The venous side 40 of the bifurcation insert 10 extends directly from the distal end 20, forming a substantially straight passageway as shown in FIG. 2. The venous side 40 has an opening 44 that is

configured to accommodate an inner catheter of a coaxial catheter arrangement. The arterial side 50 extends at an angle with respect to the distal end 20 and similarly has a tapered portion 52 and a shoulder 56, along with an opening 54. The tapered portion 52 is configured for receiving an extension tube, wherein an outside wall of the tube abuts shoulder 56.

[0020] The cross-sectional view of FIG. 2 illustrates the passageways of the bifurcation insert of Fig. 1. From the distal opening 24, a first passageway 12 extends to the venous side opening 44. A second passageway 14 extends from the first passageway 12 at location 16 to the arterial side opening 54. Although location 16 is shown as being closer the distal end 20 than the proximal end 30, it is also possible that location 16 would be closer to the proximal end 30 or that location 16 would be midway between the two ends 20, 30.

[0021] Referring now to FIG. 3, a catheter assembly according to the present invention is illustrated in cross-section. The catheter assembly 100 includes the bifurcation insert 10, a coaxial catheter 80, extension tubes 60, 70 and a hub 90. The coaxial catheter 80 contains an inner lumen 84 within an outer lumen 82. The outer lumen 82 is in fluid communication, via the bifurcation insert 10, with a first extension tube 60, while the inner lumen 84 is in fluid communication with a second extension tube 70. The catheter assembly is constructed by inserting the distal end 20 of the bifurcation insert 10 into a proximal end of the outer lumen 82 so that the shoulder 26 abuts an outer wall thereof. The inner lumen 84, which in this example is longer in length than the outer lumen 82, is received within the first passageway 12, entering through the distal opening 24 and exiting the venous side opening 44. The first extension tube 60 is placed over the tapered portion 52 of the arterial side 50 so that a distal end thereof abuts the shoulder 56. The second extension tube is placed in close proximity to a proximal end of the inner lumen 84. Once the insert 10, coaxial catheter 80 and extension tubes 60, 70 have been properly aligned with respect to one another, a first pin (not shown) is placed through the first extension tube 60 and into the arterial side 50 of the bifurcation insert 10 and a second pin (not shown) is placed through the second extension tube 70 and into the inner lumen 84. The pins provide support to the respective lumens and tubes at the proximal end of the assembly during

the overmolding process (the distal taper 22 of the bifurcation insert 10 provides support for the outer lumen 82).

[0022] Following insertion of the pins, a hub 90 is molded over the assembled parts to lock into place their position with respect to one another. Specifically, the hub 90 extends over the entire bifurcation insert 10 and a portion of the outer lumen 82 and the extension tubes 60, 70. Of course, the distance the hub 90 extends over the outer lumen 82 and extension tubes 60, 70 is variable, the important aspect being that at least a portion thereof be covered so that each are secure and locked into position with respect to one another. Thus, many different possibilities exist with respect to the extent of reach distally and proximally of the hub 90, all of which would be within the scope of the present invention. After the molding process has been completed, the pins are removed from the extension tubes 60, 70. As shown in FIG. 3, a channel 94 is created between the inner lumen 84 and the second extension tube 70 enabling fluid communication therebetween, the channel formed by the second pin during the molding process. While this is one manner in which to establish fluid communication between the inner lumen 84 and the second extension tube 70, certainly other possibilities within the scope of the present invention exist, such as, for example, connecting the inner lumen 84 to the second extension tube 70 prior to molding, abutting the outer walls of the inner lumen 84 to the extension tube 70 prior to molding, inserting the inner lumen 84 within the extension tube 70, etc.

[0023] It should be appreciated that the first and second passageways 12, 14 can be constructed having large diameters or smaller diameters, depending on the patient and/or application. In addition, the passageways, 12, 14 can be varying in width along their length and can contain contoured regions to facilitate fluid flow therethrough. Moreover, it may be advantageous to configure the first passageway 12 more narrowly above the junction point 16 so that the inner lumen is tightly fit therein, preventing fluid flow in a direction towards the venous side opening 44, even though said opening would be closed following the molding process. Further, it may be advantageous to configure the arterial side opening 54 greater in diameter than that of the second passageway 14. It should also be appreciated that the angle formed between the first passageway 12 and second passageway 14 can be set at different values, depending on the goals to be attained. For example, a smaller angle may be

advantageous in providing optimal comfort for the patient as well as improved flow due to minimized flow redirection. Thus, while an angle of approximately 30° is shown, a preferred range is between approximately 15° and 60°. Of course, both angles smaller than 15° and larger than 60° are equally contemplated and would be within the scope of the present invention.

[0024] The present invention has been described above in terms of certain preferred embodiments so that an understanding of the present invention can be conveyed. However, there are many alternative arrangements for a bifurcation insert not specifically described herein but with which the present invention is applicable. Although specific features have been provided, the bifurcation insert of the present invention would equally be embodied by other configurations not specifically recited herein. The scope of the present invention should therefore not be limited by the embodiments illustrated, but rather it should be understood that the present invention has wide applicability with respect to catheter systems generally. All modifications, variations, or equivalent elements and implementations that are within the scope of the appended claims should therefore be considered within the scope of the invention.

CLAIMS

1. A proximal insert for a coaxial catheter, comprising:
a body, having a proximal end and distal end, comprising;
a first passageway extending from a first opening to a
second opening and configured to receive an
inner lumen of said coaxial catheter;
a shoulder on an outer surface of said distal end,
positioned proximate said first opening, wherein
said shoulder is configured to abut a wall of an
outer lumen of said coaxial catheter; and
a second passageway extending from said first
passageway to a third opening.
2. The proximal insert according to claim 1, wherein said
second passageway forms an angle with said first passageway in the range of
approximately 15° to 60°.
3. The proximal insert according to claim 1, wherein said
body is comprised of a material selected from the group consisting of plastic,
stainless steel, titanium, nitinol and epoxy.
4. The proximal insert according to claim 1, wherein an
outer surface distal of said shoulder is tapered.
5. The proximal insert according to claim 1, wherein said
first passageway has a smaller diameter proximal to the point at which said
second passageway connects thereto.

6. The proximal insert according to claim 1, wherein a diameter of said second passageway increases at a point adjacent said third opening.

7. The proximal insert according to claim 1, further comprising a second shoulder on an outer surface of said proximal end positioned proximate said third opening, wherein said second shoulder is configured to abut a wall of an extension tube.

8. A multi-lumen catheter, comprising:
a coaxial catheter comprising at least two lumens;
at least two extension tubes; and
an insert positioned between said catheter and said tubes,
comprising:

a body, having a proximal end and distal end,
comprising;

a first passageway extending from a first
opening to a second opening and
configured to receive an inner lumen of
said coaxial catheter;

a shoulder on an outer surface of said distal end,
positioned proximate said first opening,
wherein said shoulder is configured to
abut a wall of an outer lumen of said
coaxial catheter; and

a second passageway extending from said first
passageway to a third opening.

9. A multi-lumen catheter according to claim 8, wherein said inner lumen of said coaxial catheter is positioned within said first passageway of said body and said distal end of said body is positioned within said outer lumen of said coaxial catheter, said shoulder abutting a wall thereof.

10. A multi-lumen catheter according to claim 9, wherein a first of said extension leg tubes is connected to said inner lumen of said coaxial catheter and a second of said extension tubes is connected to said second opening of said body.

11. A multi-lumen catheter according to claim 10, further comprising a hub molded over a proximal end of said coaxial catheter and said body, wherein said body is completely encapsulated by said hub.

12. The process of attaching extension tubes to a coaxial catheter comprising the steps of:

providing an insert comprising:

a body, having a proximal end and distal end,
comprising;

a first passageway extending from a first
opening to a second opening and
configured to receive an inner lumen of
said coaxial catheter;

a shoulder on an outer surface of said distal end,
positioned proximate said first opening,
wherein said shoulder is configured to
abut a wall of an outer lumen of said
coaxial catheter; and

a second passageway extending from said first passageway to a third opening.

positioning said inner lumen of said coaxial catheter within said first passageway and positioning said distal end of said body within said outer lumen of said coaxial catheter, such that an outer wall of said outer lumen abuts said shoulder;

attaching a first of said extension tubes to said inner lumen of said coaxial catheter and attaching a second of said extension tubes to said third opening in said proximal end of said body; and

molding a hub over said body, a proximal end of said coaxial catheter and a distal end of said extension leg tubes, encapsulating each therein.

13. A multi-lumen catheter according to claim 12, wherein said attaching step further comprises the step of inserting a pin through said first of said extension tubes and into said inner lumen of said coaxial catheter prior to said molding step.

14. A multi-lumen catheter according to claim 12, wherein said attaching step further comprises the step of inserting a pin through said second of said extension tubes and into said third opening in said proximal end of said body prior to said molding step.

1/3

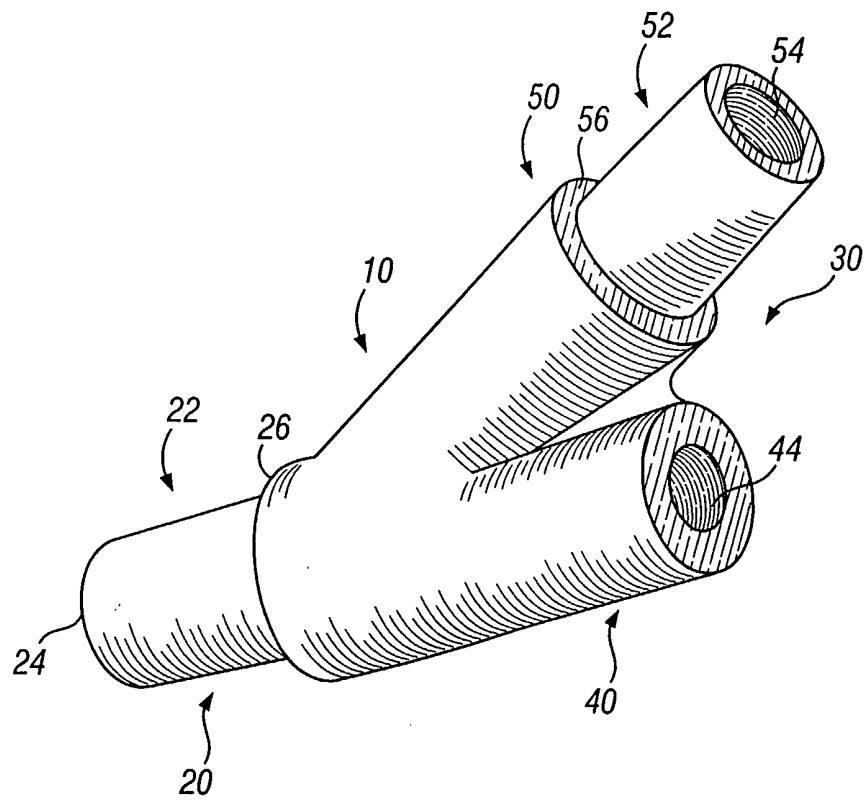


FIG. 1

2/3

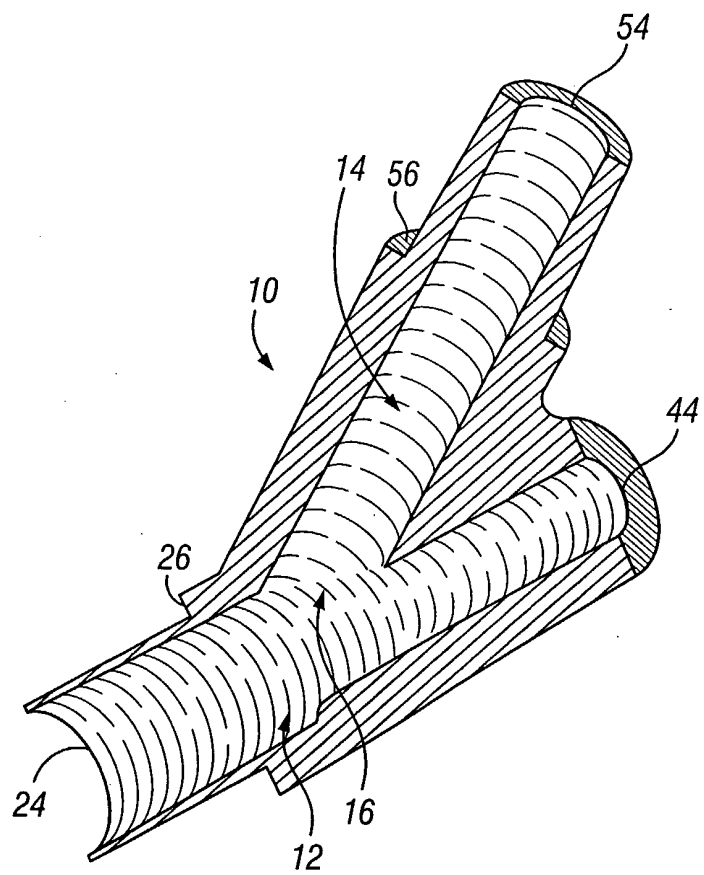


FIG. 2

3/3

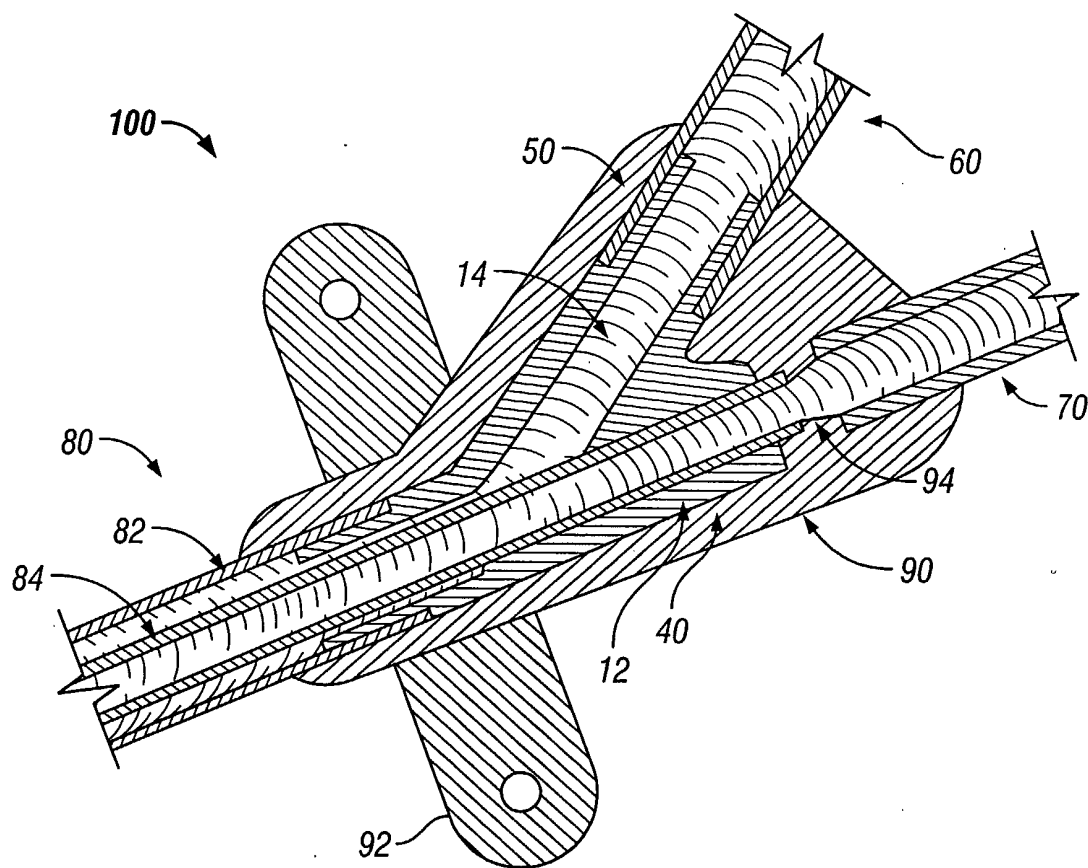


FIG. 3

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US2004/027876

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 A61M25/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
IPC 7 A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, PAJ, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 5 053 004 A (MARKEL DAVID F ET AL) 1 October 1991 (1991-10-01) cited in the application abstract; figure 1 -----	1-14
A	EP 0 616 817 A (BARD INC C R) 28 September 1994 (1994-09-28) abstract; figure 2 -----	1-14
A	US 4 931 049 A (KLIMAS DAVID R) 5 June 1990 (1990-06-05) abstract -----	1-14
A	US 5 820 612 A (BERG TODD A) 13 October 1998 (1998-10-13) abstract; figure 5 -----	1-14

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

° Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *G* document member of the same patent family

Date of the actual completion of the international search

14 January 2005

Date of mailing of the international search report

26/01/2005

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Mausser, T

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US2004/027876

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 5053004	A	01-10-1991	EP 0472105 A1 JP 4288167 A	26-02-1992 13-10-1992
EP 0616817	A	28-09-1994	CA 2106353 A1 EP 0616817 A1 JP 7100213 A	11-09-1994 28-09-1994 18-04-1995
US 4931049	A	05-06-1990	NONE	
US 5820612	A	13-10-1998	CA 2137116 A1 DE 4446127 A1 JP 7204280 A	08-07-1995 29-06-1995 08-08-1995