



- (51) **International Patent Classification:**
A61B 8/12 (2006.01)
- (21) **International Application Number:**
PCT/US2013/073081
- (22) **International Filing Date:**
4 December 2013 (04.12.2013)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (30) **Priority Data:**
61/734,286 6 December 2012 (06.12.2012) US
- (71) **Applicant:** VOLCANO CORPORATION [US/US];
3661 Valley Centre Drive, Suite 200, San Diego, California 92130 (US).
- (72) **Inventor:** VAN HOVEN, Dylan; 5388 Gooseberry Way,
Oceanside, California 92057 (US).
- (74) **Agents:** WEBB, Gregory P. et al.; Haynes and Boone,
LLP, 2323 Victory Ave., Ste 700, Dallas, Texas 75219
(US).
- (81) **Designated States** (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,


AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,
MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ,
OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA,
SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM,
TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM,
ZW.

- (84) **Designated States** (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV,
MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM,
TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW,
KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) **Title:** REINFORCED CATHETER TRANSITION WITH FLEXIBLE TIP PORTION

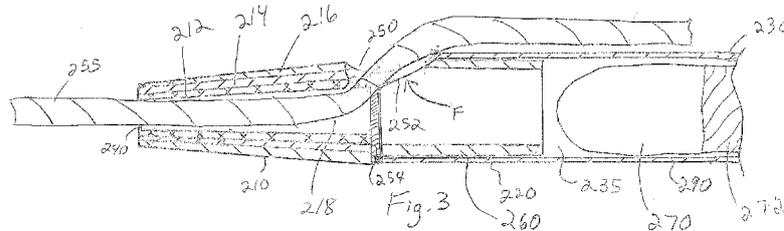

(57) **Abstract:** The present disclosure provides various embodiments of a sheath for a rotational intravascular probe for insertion into a vasculature. An exemplary sheath includes a flexible portion having a lumen for receiving an ultrasound probe, a distal portion that includes a flexible multi-layer tip, and a transition portion that couples the proximal portion and the distal portion. The multi-layer tip defines a guide wire lumen having a distal guide wire opening and a proximal guide wire opening through a sidewall. In some embodiments, an area between the proximal guide wire entry opening and the flexible proximal portion is supported to prevent kinking and prolapse.



REINFORCED CATHETER TRANSITION WITH FLEXIBLE TIP PORTION

TECHNICAL FIELD

The present disclosure relates generally to catheters for navigating through the
5 human vasculature, and in particular, to improved catheter tip designs and reinforced
sections of the catheter.

BACKGROUND

Intravascular ultrasound (IVUS) imaging is widely used in interventional cardiology
10 as a diagnostic tool for assessing a vessel, such as an artery, within the human body to
determine the need for treatment, to guide intervention, and/or to assess its effectiveness.
An IVUS imaging system uses ultrasound echoes to form a cross-sectional image of the
vessel of interest. Typically, IVUS imaging uses a transducer carried by an IVUS catheter
that both emits ultrasound signals (waves) and receives the reflected ultrasound signals.
15 The emitted ultrasound signals (often referred to as ultrasound pulses) pass easily through
most tissues and blood, but they are partially reflected by discontinuities arising from tissue
structures (such as the various layers of the vessel wall), red blood cells, and other features
of interest. The IVUS imaging system, which is connected to the IVUS catheter by way of
a patient interface module, processes the received ultrasound signals (often referred to as
20 ultrasound echoes) to produce a cross-sectional image of the vessel where the IVUS catheter
is located.

Short guide wire lumen rapid exchange (RX) catheter designs or “monorail” designs
generally employ a much shorter guide wire lumen at the distal end of the catheter, typically
in the range from about 1 cm to 4 cm. The transducer may then be disposed axially spaced
25 but close to the guide wire lumen, allowing a reduction in the total cross-sectional area of
the catheter. Among the difficulties sometimes encountered with short tipped guide wire
catheters is the possibility that the distal end or tip of the catheter may kink as it is advanced
through the patient’s vasculature. The unwanted bending may occur in the region of a guide
wire side port, irrigation port, or any unsupported region distal region of the imaging system
30 sheath. Kinking is the result of a deformation of the distal tip and usually is characterized
by a sharp deformation or point bend of the very distal section of the catheter. Such a

deformation may result from attempting to pass the distal tip through a very tortuous vascular section. Parts of the catheter may also kink or bend back upon itself in a condition referred to as prolapse. Thereafter, the catheter may return to its original shape, or it may remain permanently deformed if, during the bending, catheter material is bent beyond its
5 elastic limit.

Once the catheter has been kinked, the performance of the catheter is substantially degraded. Higher friction will be encountered at the location of the kink, adversely affecting torque transmission, as well as making it more difficult to advance the catheter over the guide wire.

10 The transition between the proximal section and the distal section of the catheter should also provide a good transition in flexibility from the relatively stiff proximal section to the relatively flexible distal section to facilitate tracking the catheter within the patient's tortuous vasculature. One difficulty has been that catheter junctions often result in a lump, step, or other surface irregularity in the bond junction.

15 Therefore, a need exists for catheters that are resistant to kinking or prolapse when introduced through tortuous regions of blood vessels.

SUMMARY

The present disclosure provides improved structural arrangements for the distal portion of intravascular devices, including intravascular imaging devices. In particular, the constructions of the present disclosure result in intravascular devices having improved handling characteristics due to the combination of flexibility and resistance to kinking or prolapse when introduced through tortuous regions of blood vessels.

The present disclosure provides various embodiments of a distal tip construction for use in intravascular ultrasound (IVUS) imaging. An exemplary tip construction includes three layers. The first layer is an inner layer adjacent to a guide wire lumen, the second layer is a middle layer adjacent the inner layer, and the third layer is an outer layer adjacent the middle layer. The first layer typically includes a lubricious polymer to promote low friction and ease of tracking over the guide wire. The second layer generally includes a polymer that adheres well to both the inner and outer layers. The third layer usually includes a polymer that is flexible and that can also be coated with a hydrophilic coating. This construction provides low friction and good guide wire movement, along with reduced friction between the catheter and blood vessel wall.

In other embodiments, the sheath includes a flexible portion having a lumen for receiving an ultrasound probe and a distal portion that includes a flexible tip. The tip defines a guide wire lumen having a distal guide wire opening and a proximal guide wire opening through a sidewall. An area between the proximal guide wire entry opening and the flexible proximal portion is supported to prevent prolapse. In some embodiments, the area is supported by a tube, which may comprise a polyimide and/or stainless steel. In alternative embodiments, the tube includes an inner lumen in communication with the ultrasound lumen and a flush hole through the tube. The sheath provides a flexible device that is locally reinforced between the proximal guide wire entry opening and ultrasound probe so that the monorail is flexible, tracks well, and does not prolapse. The additional support prevents localized kinking.

The present disclosure further provides methods for forming catheter body junctions. The methods include providing first and second elongated catheter shaft portions of different diameters to be bonded, placing a sleeve of material similar to the first or second shaft portions over a junction between the two shaft portions, placing a heat shrink thermoplastic sleeve around the junction of the first and second shaft portions, heating the assembly such that the heat shrink thermoplastic sleeve shrinks and constrains a flow of

sleeve material at the junction. The heat shrink thermoplastic sleeve is removed after cooling. The use of the thermoplastic sleeve helps to strengthen and improve the thermally bonded catheter junctions. The methods provide a smooth transition over the entire length of the bond junction.

5 Both the foregoing general description and the following detailed description are exemplary and explanatory in nature and are intended to provide an understanding of the present disclosure without limiting the scope of the present disclosure. In that regard, additional aspects, features, and advantages of the present disclosure will become apparent to one skilled in the art from the following detailed description.

10

BRIEF DESCRIPTIONS OF THE DRAWINGS

Aspects of the present disclosure are best understood from the following detailed description when read with the accompanying figures. It is emphasized that, in accordance with the standard practice in the industry, various features are not drawn to scale. In fact, the dimensions of the various features may be arbitrarily increased or reduced for clarity of discussion. In addition, the present disclosure may repeat reference numerals and/or letters in the various examples. This repetition is for the purpose of simplicity and clarity and does not in itself dictate a relationship between the various embodiments and/or configurations discussed.

10 FIG. 1 is an illustration of an intravascular ultrasound (IVUS) imaging catheter according to various aspects of the present disclosure.

 FIG. 2 is a stylized top view of a distal portion of a sheath for a rotational imaging system.

15 FIG. 3 is a diagrammatic cross-sectional side view of the sheath of FIG. 2 taken along line 3-3.

 FIG. 4 illustrates a subassembly of catheter shaft portions to be bonded according to various aspects of the present disclosure.

 FIG. 5 illustrates a transition junction between sheath sections of different diameters.

20

DETAILED DESCRIPTION

For the purposes of promoting an understanding of the principles of the present disclosure, reference will now be made to the embodiments illustrated in the drawings, and specific language will be used to describe the same. It is nevertheless understood that no
5 limitation to the scope of the disclosure is intended. Any alterations and further modifications to the described devices, systems, and methods, and any further application of the principles of the present disclosure are fully contemplated and included within the present disclosure as would normally occur to one skilled in the art to which the disclosure relates. In particular, it is fully contemplated that the features, components, and/or steps
10 described with respect to one embodiment may be combined with the features, components, and/or steps described with respect to other embodiments of the present disclosure. For the sake of brevity, however, the numerous iterations of these combinations will not be described separately.

Referring specifically to FIG. 1, a rotational intravascular probe or catheter 100 for
15 insertion into a patient for diagnostic imaging is shown. In some embodiments, the IVUS probe 100 is similar to a Revolution® Rotational IVUS Imaging Catheter available from Volcano Corporation and/or rotational IVUS catheters disclosed in U.S. Patent No. 5,243,988 and U.S. Patent No. 5,546,948, both of which are incorporated herein by reference in their entirety. The probe 100 includes an elongated, flexible catheter sheath
20 having a flexible proximal portion 130, a distal portion 110 shaped and configured for insertion into a lumen of a blood vessel, and a transition portion 120 that couples the proximal portion and the distal portion. The probe 100 is flexible such that it can adapt to the curvature of the blood vessel during use. Generally, the probe 100 may be configured to take on any desired straight or arcuate profile when in use.

25 The probe 100 comprises a sheath and a transducer shaft surrounded by the sheath. The transducer shaft is flushed with a sterile fluid, such as saline, within the catheter body. The fluid serves to eliminate the presence of air pockets or bubbles around the transducer shaft that adversely affect image quality. The fluid can also act as a lubricant.

The distal portion 110 of the sheath is inserted into a patient during the operation of
30 the probe 100. The distal portion 110 includes a short tip. With short tips, only the very distal end of the catheter follows the guide wire, while the remainder of the catheter is left to move as needed within a blood vessel. The short tip in illustrated embodiment is about

22-23 mm compared to about 22 cm for most other long tipped coronary RX catheters. In one embodiment, the tip is 23 mm.

The transition portion 120 of the sheath is typically only about 1-3 mm, but is typically not supported by a guide wire like the tip, or by the transducer shaft like the proximal portion 130. In one embodiment, the transition portion 120 is only about 3 mm in length and has a diameter of about 3.2 French (F) or about 1 mm. Thus, in prior designs this unsupported area is prone to kinking or prolapse.

The proximal portion 130 of the sheath and the proximal end portion of the transducer shaft are connected to an interface module. The rotation of the transducer shaft within the catheter body is controlled by the interface module, which provides a plurality of user interface controls that can be manipulated by a user. The interface module can receive, analyze, and/or display information received through the transducer shaft.

The usable length of the probe 100 (the portion that can be inserted into a patient) can be any suitable length and can be varied depending upon the application. The overall dimensions of the catheter will depend on use, with the length varying widely, typically being between about 40 cm and 150 cm, usually being between about 40 cm and 120 cm for peripheral catheters and being between about 110 cm and 150 cm for coronary catheters. The diameter of the catheter body may also vary widely, with the diameter of the distal portion 110 typically being between about 2F and 4F, and the diameter of the proximal portion 130 typically being about 3F and 6F. In an exemplary embodiment, the diameter of the proximal portion 130 is 3.5 F.

Turning now to FIGS. 2 and 3, illustrated is a portion of a sheath 200 showing a stylized portion of the distal tip 210 and the reinforced transition region 220 according to the present disclosure. FIG. 2 is a top view, while FIG. 3 is cross-sectional side view taken along line 3-3 of FIG. 2. For purposes of illustration, the sheath 200 is axially compressed. The sheath 200 employs a RX design, whereby a guide wire 255 enters the sheath 200 less than about 0.3 cm from the distal end or tip to allow an ultrasound probe 270 to be placed as close to the tip as possible. In use, the sheath 200 may be placed on guide wire 255 by threading the guide wire 255 through the distal guide wire opening 240, then the guide wire lumen 218, and finally the proximal guide wire opening 250. As shown in FIGS. 2 and 3, the proximal guide wire exit opening 250 extends through a sidewall of the sheath 200. The catheter body can then be then advanced along the guide wire 255 until the sheath 200 lies within the region of interest.

In one embodiment, proximal guide wire exit opening 250 includes a flush hole 252 to allow saline to flow out of the ultrasound probe lumen 235 in the direction of arrow F. In an alternative embodiment, a separate flush hole (not shown) is formed through support tube 280 and outer tube 290 opposite the guide wire exit opening.

5 The ultrasound probe lumen 235 may extend from the proximal end of the sheath 200 to the distal tip thereof, but will usually be terminated before reaching the distal tip. Thus, the guide wire lumen 218 may be disposed at least partially adjacent to the ultrasound probe lumen 235.

10 The distal tip portion 210 is coupled to the transition portion 220 and the proximal portion 230 by adhesive bonding 254. As illustrated, transition portion 220 and proximal portion 230 include the outer tube 290 that defines the ultrasound probe lumen 235. Within the transition portion 220 is support tube 260 to help support the transition portion 220 during use. The support tube 260 provides stiffness and controlled bending of the sheath 200 in the region proximal the proximal guide wire exit opening 250 and distal the
15 ultrasound probe 270. As shown in FIG. 3, the ultrasound probe 270 extends within the ultrasound probe lumen but does not extend into the support tube 260.

The ultrasound probe 270 is located at an end of a flexible transducer drive shaft that spins inside the sheath 200 inserted into the vessel of interest. The ultrasound probe 270 is usually oriented such that the ultrasound signals propagate generally perpendicular to an
20 axis of the catheter. In the typical rotational catheter, the fluid-filled (e.g., saline-filled) sheath 290 protects the vessel tissue from the spinning probe and shaft while permitting ultrasound signals to freely propagate from the probe into the tissue and back. As the shaft rotates (for example, at 30 revolutions per second), the probe is periodically excited with a high voltage pulse to emit a short burst of ultrasound. The ultrasound signals are emitted
25 from the probe, through the fluid-filled sheath and sheath wall, in a direction generally perpendicular to an axis of rotation of the shaft. The same probe then listens for returning ultrasound signals reflected from various tissue structures, and the imaging system assembles a two dimensional image of the vessel cross-section from a sequence of several hundred of these ultrasound pulse/echo acquisition sequences occurring during a single
30 revolution of the probe.

Turning back to FIG. 3, the distal portion 210 includes a flexible distal tip having a multi-layer construction. The distal tip includes three layers: an inner layer 212 adjacent the guide wire lumen 218, a middle layer 214 adjacent the inner layer 212, and an outer

layer 216 adjacent the middle layer 214. Flexibility is needed to make tortuous turns in the vasculature while following the guide wire 255, but rigidity is also needed to allow the tip to track along the guide wire.

In one embodiment, the length of the distal tip 210 is about 22 mm. In an alternative
5 embodiment, the length of the tip is less than about 3 cm.

The inner layer 212 includes a lubricious polymer that slides easily over guide wire 255. In an exemplary embodiment, the lubricious polymer includes a high-density polyethylene to promote low friction and ease of tracking over the guide wire 255.

The middle layer 214 includes a polymer that adheres to the inner layer 212 and the
10 outer layer 216. In an exemplary embodiment, the polymer includes a functionalized or maleic anhydride grafted polyethylene.

The outer layer 216 includes a flexible polymer. In an exemplary embodiment, the flexible polymer includes a polyether block amide and/or polyamide. The flexible polymer can make tight or tortuous bends in the anatomy. In a further aspect, the outer layer 216 can
15 be coated with a polymeric hydrophilic coating to reduce tracking friction against vessel walls in the anatomy.

The transition portion 220 includes support tube 260. The support tube 260 is located in an area between the proximal guide wire opening 250 and the flexible proximal portion 230. The support tube 260 may be positioned within a distal extremity of the lumen
20 235. The support tube 260 is formed of any material suitable to reinforce the transition portion 220 so that the transition portion 220 is supported and does not prolapse. In an exemplary embodiment, the support tube 260 includes polyimide and/or stainless steel. In an embodiment, the support tube 260 includes an inner lumen in communication with the ultrasound probe lumen 235 and a flush hole 252 through at least a portion of the support
25 tube 260. Without limitation to support members having alternative lengths, in the illustrated embodiment, the support member 260 has a length between 1-3 mm. In a further aspect, the support member 260 has a length of approximately 2 mm.

The sheath 200 of the present disclosure has excellent ability to track within the patient's tortuous vasculature due to the improved design of the distal tip portion 210 and
30 the reinforced transition portion 220.

The outer sheath 290 may be formed from a single tubular member that extends the entire distance from the proximal portion 130 to the distal portion 110 or may be formed from two or more tubular members that are joined together. The two tubular members may

be joined together so that they share a common inner lumen. As shown in FIG. 1 at detail 5, the outer sheath 290 transitions from a distal diameter of 3.2F to a proximal diameter of 3.5F.

Referring now to FIG. 4, shown is a subassembly of catheter shaft portions to be bonded. The subassembly is formed by positioning one end of a first catheter shaft portion 310 into an end of a second catheter shaft portion 320. The first catheter shaft portion 310 has an outer diameter D1 of approximately 3.2F that is different than the outer diameter D2 of approximately 3.5F of the second catheter shaft portion 320. A mandrel 350 is positioned in the inner lumen to keep the inner lumen open during the fusing of the first catheter shaft portion 310 and second catheter shaft portion 320. A sleeve 330 is placed over a junction 315 of the two shaft portions 310, 320. In an embodiment, the sleeve 330 includes the same material as one or both of the two shaft portions 310, 320. In an exemplary embodiment, the sleeve 430 includes a nylon and/or polyether block amide. The sleeve includes a shoulder 332 separating a first portion 334 having a first diameter substantially matching D1 and a second portion 336 having a diameter substantially matching D2. A heat shrink thermoplastic sleeve 340 is placed over the sleeve 330 and the junction 315 to create final subassembly.

Bonding of the subassembly is completed by applying heat to the subassembly melt the catheter portions and sleeve. During heating, the heat shrink thermoplastic sleeve 340 shrinks and constrains a flow of the sleeve material 330 and catheter materials at the junction 315. During the heating, the sleeve material 330 melts and fuses the two shaft portions 310, 320 together. The sleeve material 330 flows and fills in around the junction 315 to form a transition zone 360. After cooling, the heat shrink thermoplastic sleeve 340 is removed.

Referring now to FIG. 5, the heat shrink thermoplastic sleeve 340 created a smooth and long transition zone 360 from the first shaft portion 310 to the second shaft portion 320 over the junction 315. In addition, the heat shrink thermoplastic sleeve 440 results in a stronger junction 415 compared to a method that does not use sleeve 440. The use of a thermoplastic sleeve helps to strengthen and improve the thermally bonded catheter junctions by filling in surface irregularities and providing a smooth transition from one shaft to the next over the entire length of the bond junction. This smooth transition presents an atraumatic surface to tissue as the sheath is advanced within the body.

Persons skilled in the art will recognize that the devices and methods described above can be modified in various ways. Accordingly, persons of ordinary skill in the art will appreciate that the embodiments encompassed by the present disclosure are not limited to the particular exemplary embodiments described above. In that regard, although
5 illustrative embodiments have been shown and described, a wide range of modification, change, and substitution is contemplated in the foregoing disclosure. It is understood that such variations may be made to the foregoing without departing from the scope of the present disclosure. Accordingly, it is appropriate that the appended claims be construed broadly and in a manner consistent with the present disclosure.

10

THE CLAIMS

What is claimed is:

- 5 1. A distal tip for a guiding portion of a catheter, the tip comprising:
an inner layer adjacent a guide wire lumen;
a middle layer adjacent the inner layer; and
an outer layer adjacent the middle layer.
- 10 2. The distal tip construction of claim 1, wherein the inner layer comprises a lubricious polymer, the middle layer comprises a polymer that adheres to the inner and outer layers, and the outer layer comprises a flexible polymer.
- 15 3. The distal tip construction of claim 2, wherein the lubricious polymer comprises a high-density polyethylene, the polymer that adheres to the inner and outer layers comprises a functionalized or maleic anhydride grafted polyethylene, and the flexible polymer comprises a polyether block amide and/or polyamide.
- 20 4. The distal tip construction of claim 1, further comprising a hydrophilic coating adjacent the outer layer.
5. The distal tip construction of claim 1, wherein the length of the tip is about 22 mm.
- 25 6. The distal tip construction of claim 1, wherein the length of the tip is less than about 3 cm.

7. A sheath for an intravascular probe for insertion into a vasculature, the sheath comprising:
- a flexible sheath having a lumen for receiving a sensing probe; and
 - a distal tip attached to a distal extremity of the flexible sheath and defining a guide wire lumen, the tip having a distal guide wire opening and a proximal guide wire opening extending through a sidewall,
 - a support member positioned within at least the distal extremity of the flexible sheath adjacent the distal tip, wherein the support member prevents collapse of the distal extremity of the sheath during advancement along a guidewire.
- 10
8. The sheath of claim 7, wherein the support member is a tube.
9. The sheath of claim 8, wherein the tube comprises an inner lumen in communication with the ultrasound lumen and a flush hole through the tube.
- 15
10. The sheath of claim 8, wherein the tube comprises polyimide and/or stainless steel.
11. The sheath of claim 7, wherein the tip comprises an inner layer, a middle layer, and an outer layer.
- 20
12. The sheath of claim 11, wherein the inner layer comprises a polymer that promotes low friction and ease of tracking over a guide wire, the middle layer comprises a polymer that adheres to the inner and outer layers, and the outer layer comprises a flexible polymer that can be coated with a hydrophilic polymer.
- 25
13. The sheath of claim 12, wherein the polymer that promotes low friction and ease of tracking comprises a high-density polyethylene, the polymer that adheres to the inner and outer layers comprises a functionalized or maleic anhydride grafted polyethylene, and the flexible polymer that can be coated with a hydrophilic polymer comprises a polyether block amide and/or polyamide.
- 30
14. A method for forming catheter body junctions, the method comprising:

providing first and second elongated catheter shaft portions of different diameters to be bonded;

placing a sleeve of material similar to the first or second shaft portions over a junction between the two shaft portions;

5 placing a heat shrink thermoplastic sleeve around the junction of the first and second shaft portions to form an assembly;

heating the assembly such that the heat shrink thermoplastic sleeve shrinks and constrains a flow of sleeve material at the junction; and

removing the heat shrink thermoplastic sleeve.

10

15. The method of claim 14, further comprising placing the first shaft portion into the second shaft portion before placing the sleeve over the junction.

16. The method of claim 14, wherein heating the heat shrink thermoplastic sleeve results
15 in a smooth transition from the first shaft portion to the second shaft portion over the junction.

17. The method of claim 14, wherein heating the heat shrink thermoplastic sleeve results
20 in a stronger junction compared to a method where a heat shrink thermoplastic sleeve is not used.

18. The method of claim 14, wherein the sleeve includes a shoulder separating a first
portion having an internal diameter matching the outside diameter of the first catheter and a
second portion having internal diameter matching the outside diameter of the second
25 catheter.

19. The method of claim 14, wherein the sleeve material comprises a nylon and/or polyether block amide.

100 ↗

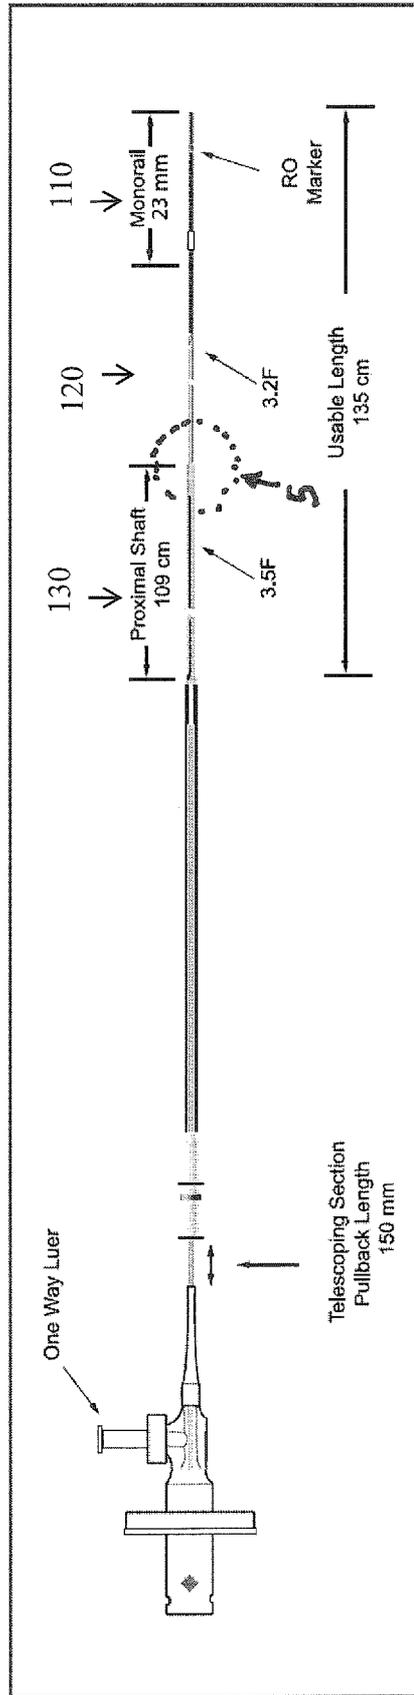


Fig. 1

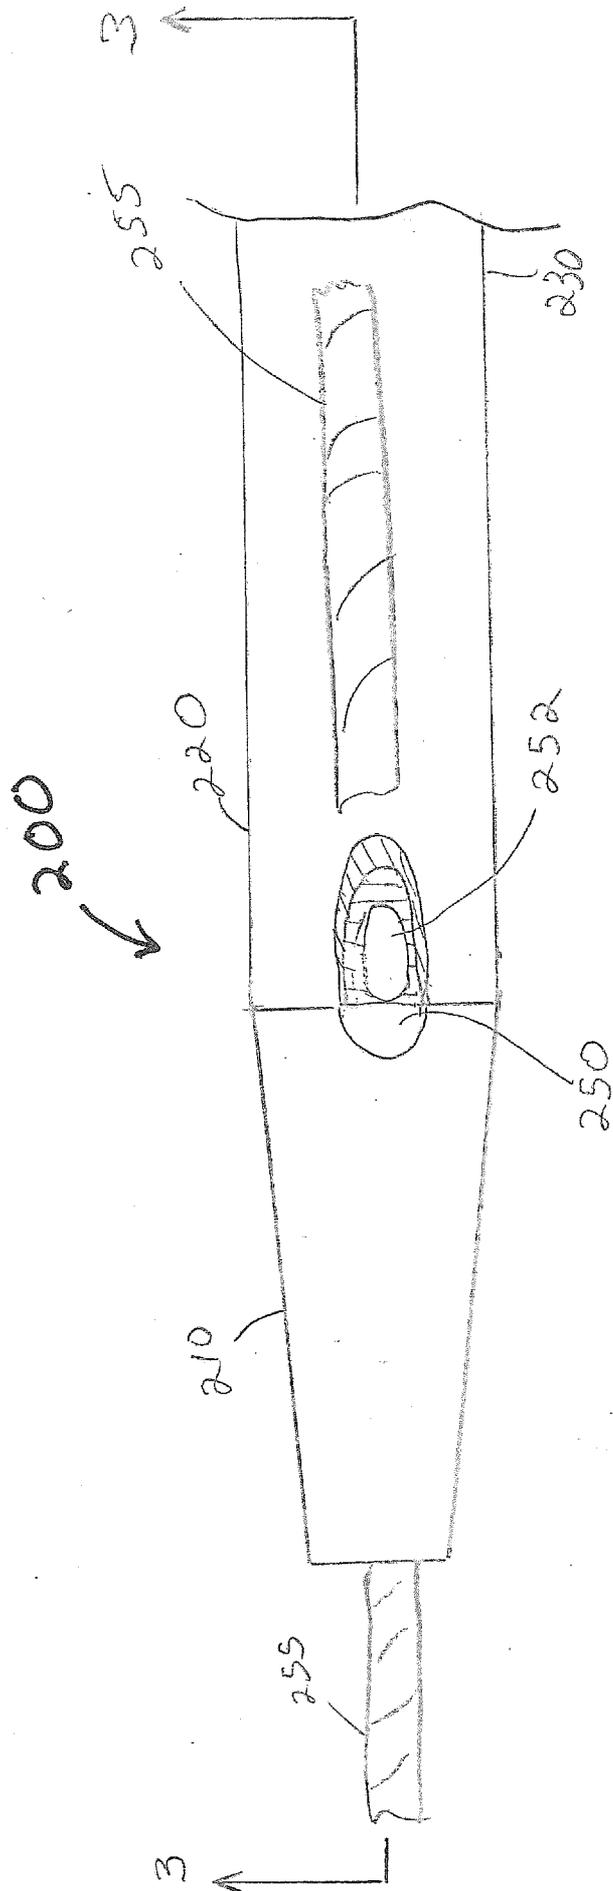
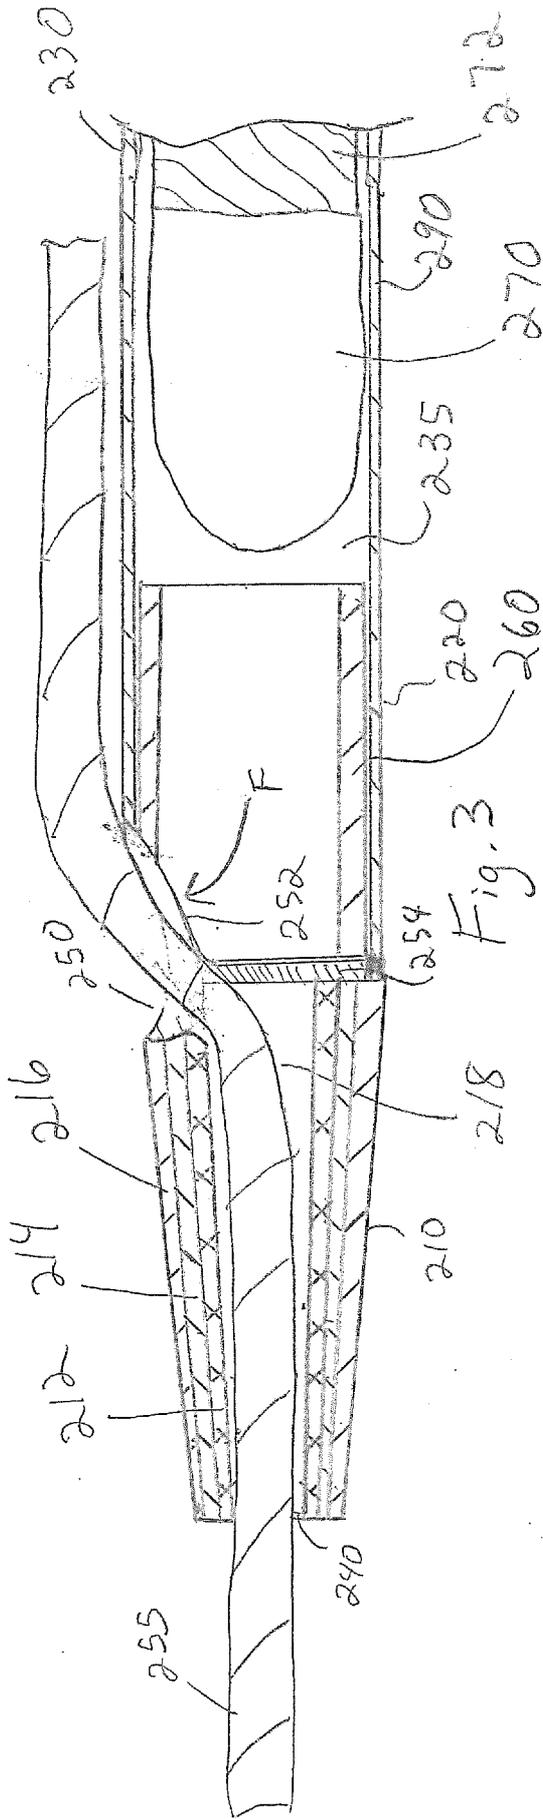


Fig. 2

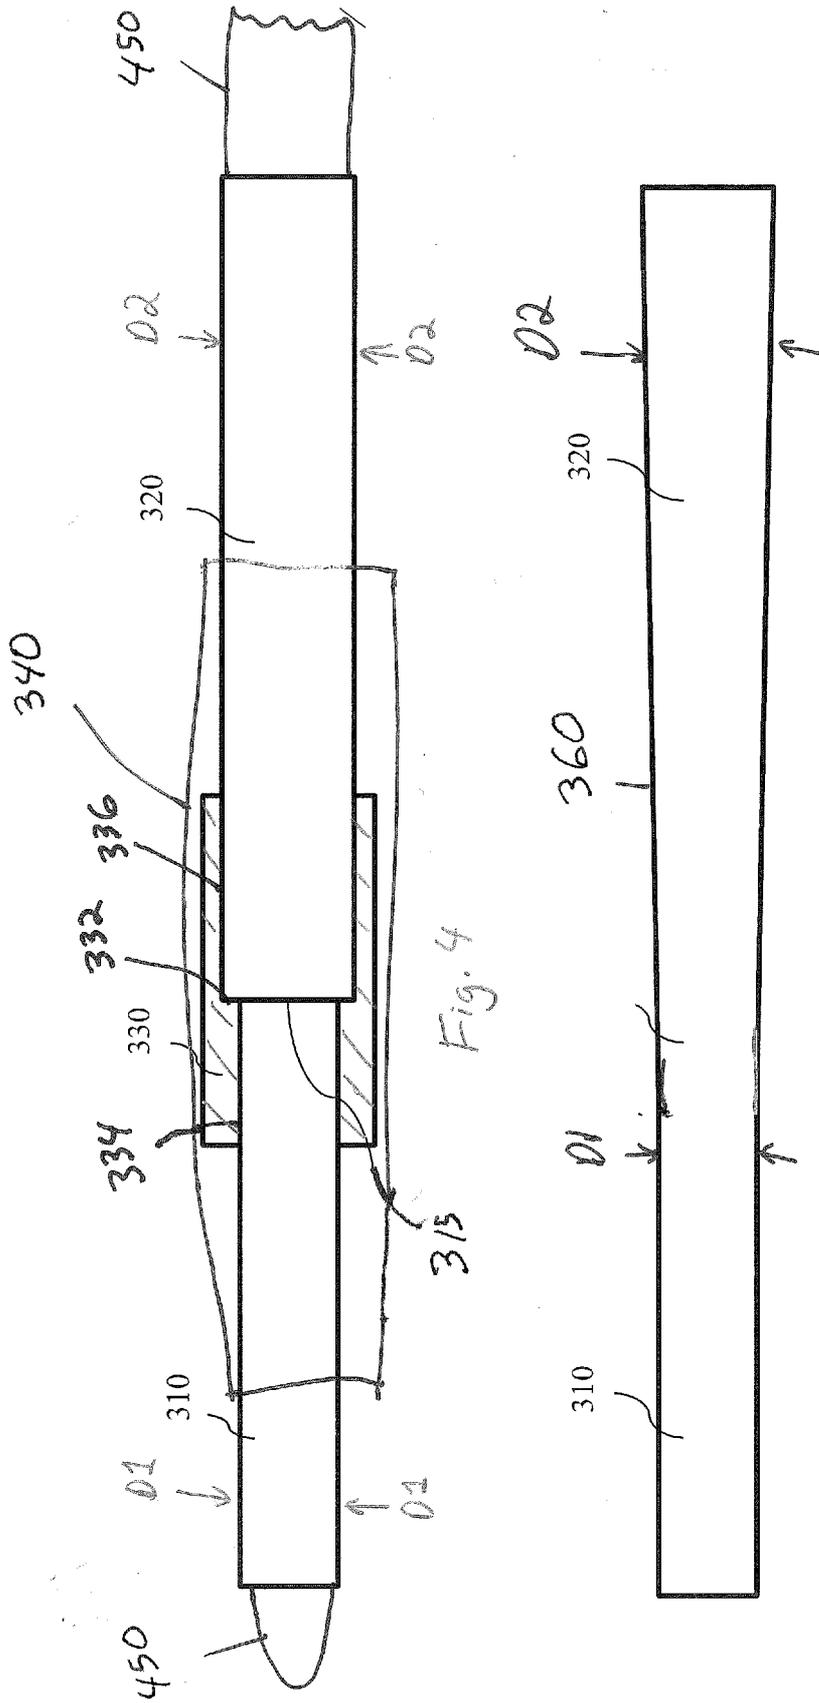


FIG. 5

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2013/073081**A. CLASSIFICATION OF SUBJECT MATTER****A61B 8/12(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHEDMinimum documentation searched (classification system followed by classification symbols)
A61B 8/12; A61M 5/32; A61M 31/00; A61M 25/09; A61M 29/00; A61M 25/00; A61B 17/22Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
Korean utility models and applications for utility models
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)
eKOMPASS(KIPO internal) & Keywords:distal, tip, sheath, intravascular, catheter, guide, flexible**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2008-0262470 A1 (JEONG S. LEE et al.) 23 October 2008 See abstract, paragraphs [0019]-[0038], claims 1-20 and figures 1-6.	1-6,14-19
Y		7-13
Y	US 2009-0264826 A1 (DUSTIN THOMPSON) 22 October 2009 See abstract, paragraphs [0023]-[0026], claims 1-12 and figures 1-2B.	7-13
A	US 2010-0094259 A1 (JOSHUA MAKOWER et al.) 15 April 2010 See abstract, paragraphs [0066]-[0075], claims 1-4 and figures 1a-1g.	1-19
A	US 2003-0036729 A1 (YUE-TEH JANG) 20 February 2003 See abstract, paragraphs [0045]-[0049], claims 1-10 and figures 3-4.	1-19
A	US 2006-0129178 A1 (NIKOLAUS REIFART et al.) 15 June 2006 See abstract, paragraphs [0032]-[0040], claim 29 and figures 1-3C.	1-19

 Further documents are listed in the continuation of Box C. See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

26 March 2014 (26.03.2014)

Date of mailing of the international search report

27 March 2014 (27.03.2014)

Name and mailing address of the ISA/KR

International Application Division
Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City, 302-701,
Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

KIM, Tae Hoon

Telephone No. +82-42-481-8407



INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/073081

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2008-0262470 A1	23/10/2008	EP 2148715 A1	03/02/2010
		JP 2010-524572 A	22/07/2010
		US 2009-0223624 A1	10/09/2009
		US 2013-138038 A1	30/05/2013
		US 7549975 B2	23/06/2009
		US 8444802 B2	21/05/2013
		WO 2008-130758 A1	30/10/2008
US 2009-0264826 A1	22/10/2009	US 8374680 B2	12/02/2013
US 2010-0094259 A1	15/04/2010	AT 370699 T	15/09/2007
		AT 489888 T	15/12/2010
		AU 1996-74316 B2	16/11/2000
		AU 1996-75953 B2	01/02/2001
		AU 1997-18471 B2	10/05/2001
		AU 1997-18472 B2	10/05/2001
		AU 1997-18473 B2	07/09/2000
		AU 1997-42340 B2	17/01/2002
		AU 1998-69686 B2	21/02/2002
		AU 1998-73581 B2	27/06/2002
		AU 1999-13928 A1	07/06/1999
		AU 1999-29054 A1	18/10/1999
		AU 1999-29054 B2	27/06/2002
		AU 1999-34594 A1	18/10/1999
		AU 1999-34594 B2	27/11/2003
		AU 1999-35477 A1	18/10/1999
		AU 1999-35477 B2	26/06/2003
		AU 1999-41875 A1	20/12/1999
		AU 1999-41875 B2	15/08/2002
		AU 1999-54672 A1	06/03/2000
		AU 2000-14489 A1	15/05/2000
		AU 7358198 A	11/11/1998
		AU 749373 B2	27/06/2002
		CA 2284720 A1	22/10/1998
		CA 2284720 C	12/09/2006
		CA 2285001 A1	22/10/1998
		CA 2308475 A1	27/05/1999
		CA 2324210 A1	07/10/1999
		CA 2324304 A1	07/10/1999
		CA 2325032 A1	30/09/1999
		CA 2333764 A1	09/12/1999
		CA 2657885 A1	17/01/2008
		CN 1204242 A0	06/01/1999
CN 1204244 A0	06/01/1999		
CN 1216929 A0	19/05/1999		
CN 1216930 A0	19/05/1999		
CN 1218414 A0	02/06/1999		
DE 69838287 D1	04/10/2007		
DE 69838287 T2	03/07/2008		

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/073081

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		DE 69842030 D1	13/01/2011
		EP 0879068 A1	02/01/2002
		EP 0910298 A1	22/01/2003
		EP 0910298 B1	20/08/2003
		EP 0932426 A1	02/03/2005
		EP 0954248 A1	17/10/2001
		EP 0954248 B1	15/09/2004
		EP 0955933 A1	16/04/2003
		EP 0955933 B1	26/08/2009
		EP 0964636 A1	22/12/1999
		EP 0964636 A1	03/11/2004
		EP 0964636 A4	21/07/2004
		EP 0964636 B1	22/08/2007
		EP 0981295 A2	01/03/2000
		EP 1006916 A1	14/06/2000
		EP 1037571 A1	27/09/2000
		EP 1066070 A1	10/01/2001
		EP 1067869 A2	17/01/2001
		EP 1067869 B1	02/11/2005
		EP 1067874 A1	17/01/2001
		EP 1067874 B1	23/04/2008
		EP 1082070 A1	14/03/2001
		EP 1166721 A2	02/01/2002
		EP 1166721 A3	03/12/2003
		EP 1317908 A2	11/06/2003
		EP 1317908 A3	11/06/2003
		EP 1317908 B1	06/07/2011
		EP 1600110 A1	30/11/2005
		EP 1600110 B1	22/04/2009
		EP 1707233 A2	04/10/2006
		EP 1707233 A3	20/12/2006
		EP 1820436 A2	22/08/2007
		EP 1820436 A3	14/11/2007
		EP 1820436 B1	01/12/2010
		ES 2293679 T3	16/03/2008
		IL 132197 D0	19/03/2001
		JP 11-513577 A	24/11/1999
		JP 11-514269 A	07/12/1999
		JP 2000-504594 A	18/04/2000
		JP 2000-505316 A	09/05/2000
		JP 2001-500401 A	16/01/2001
		JP 2001-508318 A	26/06/2001
		JP 2001-522692 A	20/11/2001
		JP 2001-527440 A	25/12/2001
		JP 2002-507458 A	12/03/2002
		JP 2002-509754 A	02/04/2002
		JP 2002-509768 A	02/04/2002
		JP 2002-514111 A	14/05/2002
		JP 2002-516704 A	11/06/2002
		JP 2006-181370A	13/07/2006

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/073081

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		JP 4019112 B2	12/12/2007
		JP 4184602 B2	19/11/2008
		JP 4348338 B2	21/10/2009
		JP 4448614 B2	14/04/2010
		JP 4498604 B2	07/07/2010
		KR 10-1999-0064208 A	26/07/1999
		KR 10-1999-0064209 A	26/07/1999
		US 2001-0047165 A1	29/11/2001
		US 2002-0002349 A1	03/01/2002
		US 2002-0029079 A1	07/03/2002
		US 2002-0062146 A1	23/05/2002
		US 2002-0111672 A1	15/08/2002
		US 2002-0123698 A1	05/09/2002
		US 2002-0179098 A1	05/12/2002
		US 2003-0018106 A1	23/01/2003
		US 2003-0229366 A1	11/12/2003
		US 2003-0236542 A1	25/12/2003
		US 2004-0059280 A1	25/03/2004
		US 2004-0073238 A1	15/04/2004
		US 2004-0088042 A1	06/05/2004
		US 2004-0098030 A1	20/05/2004
		US 2004-0122318 A1	24/06/2004
		US 2004-0133154 A1	08/07/2004
		US 2004-0133225 A1	08/07/2004
		US 2004-015225 A1	22/01/2004
		US 2004-0158143 A1	12/08/2004
		US 2004-0225036 A1	11/11/2004
		US 2005-0038141 A1	17/02/2005
		US 2005-0131113 A1	16/06/2005
		US 2006-0184089 A1	17/08/2006
		US 2007-0021730 A1	25/01/2007
		US 2007-0249762 A1	25/10/2007
		US 2008-0045996 A1	21/02/2008
		US 2009-0182360 A1	16/07/2009
		US 2010-0121357 A1	13/05/2010
		US 2010-0324471 A1	23/12/2010
		US 5830222 A	03/11/1998
		US 6068638 A	30/05/2000
		US 6159225 A	12/12/2000
		US 6190353 B1	20/02/2001
		US 6231587 B1	15/05/2001
		US 6283951 B1	04/09/2001
		US 6283983 B1	04/09/2001
		US 6302875 B1	16/10/2001
		US 6330884 B1	18/12/2001
		US 6375615 B1	23/04/2002
		US 6379319 B1	30/04/2002
		US 6432127 B1	13/08/2002
		US 6579311 B1	17/06/2003
		US 6613081 B2	02/09/2003

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/073081

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 6616675 B1	09/09/2003
		US 6638293 B1	28/10/2003
		US 6655386 B1	02/12/2003
		US 6660024 B1	09/12/2003
		US 6685648 B2	03/02/2004
		US 6709444 B1	23/03/2004
		US 6726677 B1	27/04/2004
		US 6746464 B1	08/06/2004
		US 6863684 B2	08/03/2005
		US 6894092 B2	17/05/2005
		US 6929009 B2	16/08/2005
		US 7059330 B1	13/06/2006
		US 7074846 B2	11/07/2006
		US 7087665 B2	08/08/2006
		US 7094230 B2	22/08/2006
		US 7134438 B2	14/11/2006
		US 7159592 B1	09/01/2007
		US 7179270 B2	20/02/2007
		US 7303571 B2	04/12/2007
		US 7316655 B2	08/01/2008
		US 7407506 B2	05/08/2008
		US 7637870 B2	29/12/2009
		US 7648517 B2	19/01/2010
		US 7670329 B2	02/03/2010
		US 7729738 B2	01/06/2010
		US 7846172 B2	07/12/2010
		US 7849860 B2	14/12/2010
		US 7955343 B2	07/06/2011
		US 8075580 B2	13/12/2011
		US 8083708 B2	27/12/2011
		WO 97-13463 A1	17/04/1997
		WO 97-13471 A1	17/04/1997
		WO 97-27893 A1	07/08/1997
		WO 97-27897 A1	07/08/1997
		WO 98-46119 A1	22/10/1998
US 2003-0036729 A1	20/02/2003	AT 157269 T	15/09/1997
		CA 2098570 A1	18/06/1992
		CA 2098570 C	01/04/2003
		DE 69127462 D1	02/10/1997
		DE 69127462 T2	02/04/1998
		EP 0563179 A1	06/10/1993
		EP 0563179 A4	01/12/1993
		EP 0563179 B1	27/08/1997
		JP 3367666 B2	14/01/2003
		US 5203338 A	20/04/1993
		US 5665533 A	09/09/1997
		US 5976093 A	02/11/1999
		US 5997523 A	07/12/1999
		US 6234971 B1	22/05/2001

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/073081

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2006-0129178 A1	15/06/2006	US 6730037 B2	04/05/2004
		WO 92-11055 A1	09/07/1992
		EP 578777 A1	19/01/1994
		EP 578777 B1	21/01/1998
		JP 3137646 B2	26/02/2001
		US 2005-0027249 A1	03/02/2005
		US 6702781 B1	09/03/2004
		US 6733473 B1	11/05/2004
		WO 92-17236 A1	15/10/1992