

(19)



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11)

EP 0 983 747 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
08.12.2004 Bulletin 2004/50

(51) Int Cl.7: **A61B 6/03**, A61B 6/00

(21) Application number: **99306966.5**

(22) Date of filing: **02.09.1999**

(54) **Cardiac CT system**

Kardiologische CT Vorrichtung

Système de tomographie cardiaque

(84) Designated Contracting States:
DE FR NL

(30) Priority: **04.09.1998 US 99234 P**
18.09.1998 US 157028

(43) Date of publication of application:
08.03.2000 Bulletin 2000/10

(73) Proprietor: **Koninklijke Philips Electronics N.V.**
5621 BA Eindhoven (NL)

(72) Inventors:
• **Heuscher, Dominic**
Aurora, Ohio 44202 (US)
• **Chandra, Shalabh**
Mayfield Heights, Ohio 44124 (US)

• **Shekhar, Raj**
Mayfield Heights, Ohio 44124 (US)
• **Hoffmeyer, Dave**
Concord, Ohio 44077 (US)

(74) Representative:
van der Veer, Johannes Leendert et al
Philips
Intellectual Property & Standards
P.O. Box 220
5600 AE Eindhoven (NL)

(56) References cited:
WO-A-98/32371 WO-A-99/07283
US-A- 5 383 231 US-A- 5 612 985

EP 0 983 747 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates to computed tomography (CT) imaging. It finds particular application in conjunction with cardiac gated spiral CT scanners, and will be described with particular reference thereto. However, it is to be appreciated that the present invention is also amenable to other like applications, especially diagnostic applications.

[0002] In typical spiral or helical CT scanning, an x-ray source or tube emits a fan beam of radiation as it rotates continuously around an examination region as a patient support table moves therethrough at a constant, linear velocity. Detectors positioned across the examination region from the x-ray tube convert x-rays which traverse the patient into corresponding electronic data. The collected data effectively represents a helical path of constant pitch through the patient. The helical data is reconstructed into a volumetric image representation, typically a series of consecutive thin slice images of a region of interest of the patient. See, for example, U.S. Patent Nos. 5,544,212; 5,485,493; 5,262,946; and, 5,396,418.

[0003] Furthermore, a number of methods are aimed at reconstructing cardiac images with reduced motion artifacts. For example: a prospective electrocardiogram (ECG) gated method with axial slice CT acquisition has been used to reconstruct cardiac images, as shown in U.S. Patent No. 5,751,782 to Yoshitome; a retrospective ECG-gated CT data acquisition and reconstruction technique using spiral CT is also known; a prospective ECG-gated technique with spiral CT data acquisition for imaging only the diastolic phase of the heart is known; and a prospective ECG-gated technique is known which employs a scan time of 100ms/slice in an electron beam CT (EBCT) scanner such as the one described in U.S. Patent No. 4,573,179 to Rutt. However, the above techniques have failed to provide a generalized scheme for cardiac reconstruction of any selected cardiac phase for various heart rates and/or different gantry speeds and configurations. In addition, the above techniques suffer from various drawbacks and are therefore less than ideal in certain aspects for diagnostic cardiac imaging.

[0004] For example, one drawback of the technique employed in U.S. Patent No. 5,751,782 and other such cardiac gated axial slice systems is that they use multiple rotations for reconstructing a single slice, and hence, have a longer scan time. A disadvantage of retrospective ECG-gated CT data reconstruction is that processor resources and time is consumed in the processing of too many images. The aforementioned prospective ECG-gated technique with spiral CT acquisition is less than ideal in that it is limited to a given phase of the heart and does not demonstrate the detector configuration, scanner speed, and imaging protocol best for removing motion artifacts.

[0005] Use of EBCT imaging in diagnostic cardiac applications also has certain drawbacks. First of all, it is primarily a research tool and it is not as widely available for clinical applications as conventional spiral CT scanners. In addition, EBCT scanners are generally much more expensive. Often, EBCT scanners have poor image quality and their z-axis resolution limits usefulness.

[0006] From document US 5,383,231 a helical scanning X-ray CT apparatus is known, with which a plurality of images are reconstructed in synchronism with cardiac beats of a patient. Temporal information from the electrocardiogram data is converted into positional information. The reconstruction step uses the positional information so that images having a specific relationship with the cardiac beats are generated.

[0007] International patent application WO 99/07283 A1 describes a cardiac CT scanner in which a measured average heart beat is used to enable asynchronous scanning between rotation time and average heart beat so that successive data segments from a given cardiac phase add to 180-degree data for reconstruction.

[0008] In accordance with one aspect of the present invention, a cardiac gated spiral CT scanner includes a source of penetrating radiation arranged for rotation about an examination region having a central axis extending in a z direction. The source emits a beam of radiation that passes through the examination region as the source rotates. A patient support holds a patient being examined at least partially within the examination region and translates the patient through the examination region in the z direction while the source is rotated such that the source follows a helical path relative to the patient. A control processor implements a patient-specific scan protocol in response to measured patient characteristics and scanner characteristics. Radiation detectors are arranged to receive radiation emitted from the source after it has traversed the examination region. An ECG monitor acquires ECG data from the patient. The ECG data is used to accurately correlate phases of the patient's heart with data collected by the radiation detectors. An image reconstruction processor reconstructs image representations of the patient based on data received from the radiation detectors and ECG monitor. Ultimately, a human viewable display selectively displays the image representations for assessing cardiac function.

[0009] In accordance with another aspect of the present invention, a method for cardiac gated spiral CT imaging is provided. The method includes assessing a breath hold time for a patient, measuring an average heart rate of the patient, and determining a range of scan coverage. Next, based on results from the initial steps, a patient-specific scan protocol is selected. In accordance with the selected scan protocol, a spiral CT scan of the patient is performed while collecting ECG data from the patient. The ECG data is used to correlate phases of the patient's heart with x-ray data collected via the spiral CT scan. Ultimately, an image representation of a region of interest of the patient at a point in

time corresponding to a selected phase of the patient's heart is reconstructed from the x-ray data collected.

[0010] Ways of carrying out the invention will now be described, by way of example, with reference to the accompanying drawings, in which:

FIGURE 1 is a diagrammatic illustration of a cardiac gated spiral CT scanner in accordance with aspects of the present invention; and

FIGURE 2 is a flow chart illustrating a cardiac gated spiral CT imaging technique in accordance with aspects of the present invention.

[0011] With reference to FIGURE 1, a cardiac gated spiral CT scanner **10** includes a stationary gantry portion **12** which defines an examination region **14** having a central axis extending in the z direction. A rotating gantry portion **16** is mounted on the stationary gantry portion **12** for rotation about the examination region **14**. A penetrating radiation source **20**, such as an x-ray tube, is arranged on the rotating gantry portion **16** such that a beam of radiation **22** passes through the examination region **14** as the rotating gantry portion **16** rotates. A collimator and shutter assembly **24** forms the beam of radiation **22** into a thin fan-shaped beam and selectively gates the beam **22** on and off. Alternately, the fan-shaped radiation beam **22** may also be gated on and off electronically at the source **20**.

[0012] A patient support **30**, such as a couch or the like, suspends or otherwise holds a patient being examined or imaged at least partially within the examination region **14**. Moreover, as the rotating gantry portion **16** rotates, the support **30**, and consequently the patient thereon, are translated in the z direction. In this manner, the source **20** follows a helical path relative to the patient.

[0013] In the illustrated fourth generation scanner, a ring of radiation detectors **40** are mounted peripherally around the examination region **14** on the stationary gantry portion **12**. Alternately, a third generation scanner is employed with the radiation detectors **40** mounted on the rotating gantry portion **16** on a side of the examination region **14** opposite the source **20** such that they span the arc defined by the fan-shaped beam **22**. Regardless of the configuration, the radiation detectors **40** are arranged to receive the radiation emitted from the source **20** after it has traversed the examination region **14**.

[0014] In an alternate preferred embodiment, there are multiple sets of radiation detectors **40** residing in separate corresponding parallel planes. The planes are displaced from one another in the z direction. In a fourth generation scanner, this configuration is achieved by having multiple rings (each ring displaced from one another in the z direction) of radiation detectors **40** mounted peripherally around the examination region **14** on the stationary gantry portion **12**. In a third generation scanner, similarly, multiple arcs of radiation detectors **40** are employed. When multi-ring or multi-arc configurations are employed, the beam **22** employed is a cone beam arranged to diverge in two dimensions.

[0015] In a source fan geometry, an arc of detectors which span the radiation emanating from the source **20** are sampled concurrently at short time intervals as the source **20** rotates behind the examination region **14** to generate a source fan view. In a detector fan geometry, the detectors are sampled a multiplicity of times as the source **20** rotates behind the examination region **14** to generate a detector fan view. The path between the source **20** and each of the radiation detectors **40** is denoted as a ray.

[0016] The radiation detectors **40** convert the detected radiation into electronic data. That is to say, each of the radiation detectors produces an output signal which is proportional to an intensity of received radiation. Optionally, a reference detector may detect radiation which has not traversed the examination region **14**. A difference between the magnitude of radiation received by the reference detector and each radiation detector **40** provides an indication of the amount of radiation attenuation along a corresponding ray of a sampled fan of radiation.

[0017] In detector fan geometry, each view or data line represents a fan of rays having its apex at one of the radiation detectors **40** collected over a short period of time as the source **20** rotates behind the examination region **14** from the detector. In source fan geometry, each view or data line represents a fan of rays having an apex at the source **20** collected by concurrent sampling of all detectors. Contiguous fan views which span 180° plus the angle of the fan constitute a complete set of data for reconstruction into an image slice.

[0018] A sampling processor **50** receives sampled data from the radiation detectors **40**. The sampling processor **50** optionally shuffles the data to transform it from a detector fan geometry to a source fan geometry or vice versa and performs a ripple filtering operation before passing the data on. The sampled fan views correspond to each angular position of the source **20** around the examination region **14** for each of a multiplicity of rotations. The apexes of the fan views are disposed along the helical path and are defined by an angular ϕ around the imaged volume and by a longitudinal position in the z direction along the imaged volume. Data or rays within each fan are further identified by their angle α within the fan.

[0019] A view processor **52** converts the spiral sampled views into planar data sets. The view processor includes a memory **54** which stores the spiral sampled views. An integrating interpolator **56** integrates corresponding rays of a preselected number of contiguous sets of spiral data with a filter or interpolation function retrieved from a memory **58**

to produce parallel axial slices. The memory **58** stores a plurality of filter or interpolation functions for integrating different numbers of spiral fan views. The more views that are combined, the thicker the corresponding image slice.

[0020] Thereafter, the combined set of data is conveyed to an image reconstruction processor **60**. The image reconstruction processor **60** processes the data from the view processor **52** and backprojects it into an image memory **66**. More specifically, the image reconstruction processor **60** performs mathematical manipulations which convolve each data set with an appropriate filter or convolution function for the view format. The image reconstruction processor **60** of the preferred embodiment includes a convolver **62** which convolves the thick slice interpolated data sets and a backprojector **64**. The backprojector **64** backprojects the convolved data sets into the image memory **66**. Ultimately, a video processor **68** selectively retrieves slices, projections, three-dimensional (3D) renderings, and other image information from the image memory **66** and appropriately formats an image representation for display on a human viewable display **70**, such as a video monitor or the like.

[0021] Via leads attached to the patient, an ECG monitor **80** (preferably digital) acquires ECG data from the patient. The ECG data is used to accurately correlate phases of the patient's heart with data collected by the radiation detectors **40**. More specifically, in a preferred embodiment, the sampling processor **50** tags sampled data views with the ECG data.

[0022] In operation, a control processor **90** implements a patient-specific scan protocol in response to measured patient characteristics and scanner characteristics. More specifically, in a preferred embodiment, the control processor accesses a look up table **92** which contains various scan protocols. The look up table **92** is accessed based on the following measured patient characteristics: the patient's assessed breath hold time (i.e. how long the patient can hold his breath, which, for a single breath hold scan, limits the total scan time); the patient's average or mean heart rate (obtained from the ECG monitor **80**); and the range of scan coverage in the z direction (the range of scan coverage in the z direction is chosen based on the particular patient's anatomy and the desired region of interest to be imaged, in a preferred embodiment the region of interest is the patient's heart and associated vasculature).

[0023] With reference to FIGURE 2 and continuing reference to FIGURE 1, a method of cardiac gated spiral CT imaging in accordance with a preferred embodiment of the present invention is set forth in the illustrated flow chart. The parameters used in the following description are as follows:

- the scan rate (sr) (e.g. 60, 90, 120, or 300 rpm) is the rate of rotation of the rotating gantry portion **16**;
- the pitch (p) (e.g. 0 to 8 mm) is the pitch of the helical path followed by the source **20** and it is determined by the rate at which the patient support **30** translates the patient through the examination region **14**;
- the detector ring width (d) (e.g. 1.3 or 4 mm) is the dimension of the radiation detectors **40** in the z direction;
- effective reconstructed slice thickness (est) is the effective image slice thickness in the z direction;
- rings reconstructed (rr) (e.g. 1, 2, or 3);
- the number of detector rings (nr) (e.g. 1, 2, 3, 5, or 9) takes into account multi-ring or multi-arc scanner configurations;
- the heart rate (hr) (e.g. 40-180 beats per minute (bpm)) is measured by the ECG monitor **80**;
- the total scan time (T) (e.g. 20-40 seconds) is limited by the assessed patient breath hold time in single breath hold scans;
- temporal resolution (Δt) (e.g. 250 ms);
- the total scan coverage (C) (e.g. 6-32 cm) in the z direction is determined by the patient's anatomy and the desired region of interest;
- a minimum applicable heart rate (hrmin) for a desired coverage; and,
- the maximum patient support travel in the z direction measured in millimeters per heart beat (mmpb).

[0024] The first step **100** is to select or determine the scan protocol based on patient parameters. The patient holds his breath and his breath-hold time is assessed. Via the ECG monitor **80**, the heart rate of the patient is measured over a period of time and the average or mean heart rate for the patient is calculated. In a preferred embodiment, the average or mean heart rate is measured while the patient is holding his breath to mimic upcoming imaging scan conditions. A pilot scan is performed to determine the scan range in the z direction. That is to say, the pilot scan roughly images the patient's anatomy so that the range of coverage in the z direction which contains the desired region of interest is readily discernable. Again, in a preferred embodiment, this takes place simultaneously with the breath hold. Based on these patient parameters and the particular scanner configuration employed, the control processor **90** selects a scan protocol from the look up table **92**. In this manner, the scan protocol is customized (i.e., the pitch, slice thickness, etc. are set to accommodate the patient parameters and scanner configuration) for each patient. In a preferred embodiment, the protocol selected operates to maximize resolution in the z direction by maintaining a continuous set of image slice data in the z direction. That is to say, the pitch and slice thickness are set such that neighbouring slices either overlap or are at least contiguous. Table 1 provided below illustrates exemplary protocols for various patient parameters and scanner configurations (see below for detailed derivation of table parameters).

Table 1

Sample Cardiac CT Configurations and Protocols for 20 seconds of Breath-hold							
Scanner Configuration nr x d	Reconstruction Mode rr (# rings)	Scan Rate sr (rpm)	Temporal Resolution Δt (msec)	Eff. Slice Thickness est (mm)	Coverage C (cm)	Heart Rate hrmin (bpm)	Pitch p (mm)
1 x 4 mm spiral	1	60	500-550	4	6	45+	3
3 x 4 mm spiral	1	90	333-360	4.2	16	40+	5.3
5 x 1.3 mm spiral	1	120	250-270	1.9	12	54+	3
100 x 1.3 mm 0-pitch	1	300	80-110	1.3	13	(all)	0

[0025] The next step **102** is to run the imaging spiral CT scan in accordance with the selected protocol. The ECG monitor **80** is used to acquire ECG data simultaneously with the spiral CT scan. In one embodiment, prior to the scan, a calibration is performed to account for any latency between delivery of the ECG data and the data collected from the radiation detectors **40**. As illustrated at step **104**, the sampling processor **50** tags each sampled fan view of data with the ECG amplitude and it is saved as part of every fan view such that various phases of the heart are accurately correlated to the view data. The source of penetrating radiation **20** stays on throughout the imaging scan to enable reconstruction of any selected phase of the heart.

[0026] At step **106**, image reconstruction of planar slices takes place in accordance with the ECG data to produce cardiac gated images **108**. The reconstructed image slices correspond to a point in time when the heart is in a selected phase. In a preferred embodiment, over-all image continuity is maintained by reconstructing contiguous image slices from contiguous heart beats. In any event, the interpolated axial slices that make up the volumetric image are centred on transverse axial planes located along the helical path where the phase of the heart is at the same position in its biological cycle as predicted from the ECG data. That is to say, the interpolator **56** centres the interpolation filter function retrieved from the memory **58** at that point on the helical path. In this manner, the technique is prospective in nature and the image reconstruction takes place while data continues to be collected from the radiation detectors **40**. In addition however, being that the source **20** remains on throughout the imaging scan and a complete helical set of data is collected, optionally different images (corresponding to different points in the cardiac cycle) are reconstructed retrospectively by selecting a set of centring points along the helical path where the heart is in a different phase.

[0027] At step **110**, the gated images from **108** are employed for 3D rendering and other clinical applications (discussed later herein) which measure and monitor cardiac structure and function three-dimensionally to reach a diagnosis or other result **112**.

[0028] The scan protocols associated with a particular scanner configuration are chosen in accordance with calculations using the parameters set forth in the list above. Moreover, the scan protocols are applicable to a number of variable scanner configurations.

[0029] In one preferred embodiment, the scanner configuration is not spiral. That is to say, the pitch of the helical path is zero such that axial slice data is collected. These 0-pitch scans are limited in z direction coverage by the number of detector rings used in the scan. With nr detector rings, nr axial images slices are reconstructed along the z direction, and the coverage is given by the following:

$$C = nr \cdot d \quad (1).$$

[0030] In operation, the ECG data is used to reconstruct and view the images slices simultaneously at one or more selected phase of the heart cycle. Optionally, these gated images are averaged over several heart cycles to improve contrast resolution, or compared over time, at the risk of patient movement, in which case it is desirable to have the patient hold his breath.

[0031] In another preferred embodiment, the scanner configuration is spiral. The objective in this case is to scan as much of the heart as possible (i.e., up to at least 20 cm), while maintaining good z direction resolution along the scanned volume for a selected phase of the heart cycle. Preferably, this scan is performed within a single breath hold (e.g., 20

to 40 seconds). Knowing the average heart rate is valuable in choosing the right scan protocol and method of reconstruction. To maintain adequate z direction resolution across the scanned volume, the following condition is met:

$$mmpb < (nr - rr + 1) \cdot d \quad (2).$$

[0032] In other words, the distance in mm of couch travel within one heart beat (mmpb) should be less than the distance between the first and last subset of rr out of nr rings (nr-rr+1) used to simultaneously reconstruct cardiac images at a selected phase of the heart cycle. For example, in a single-ring scan, nr=rr=1, or mmpb<d; and, in a five-ring scan using each ring separately to reconstruct image slices along the spiral, mmpb<(5-1+1)·d=5·d. Then, for a given pitch p and scan rate sr, this provides a minimum heart rate supported by the cardiac reconstruction as follows:

$$hrmin = sr \cdot p / (nr - rr + 1) \cdot d \quad (3).$$

[0033] For a given total scan time T, the corresponding coverage C in cm is given by the following:

$$C = sr \cdot T \cdot p / 600 \quad (4).$$

[0034] Using these relationships between heart rate, scan rate, and coverage, the following holds for a single-ring scan and a multi-ring scan. Consider for example, a single-ring scan with a 4 mm detector width (d). Coverage in this case ranges from 6 to 16 cm for heart rates from 45-120 bpm. For a multi-ring scan, with a 3 x 4 configuration and a scan speed of 60 rpm using a dual-ring (rr=2) reconstruction, the coverage is as much as 32 cm in 20 seconds, as long as the heart rate is greater than 60 bpm. As these numbers demonstrate, coverage and resolution is improved considerably by using a multi-ring scanner configuration.

[0035] Additionally, temporal resolution is maximized by using 180-plus-fan reconstruction weighting functions (i.e., those interpolation or filter functions stored in the memory 58) whose FWHM values are anywhere from .4 to .55 of one revolution while still maintaining unity-sum weighting over 180 degrees. In this case, the temporal resolution is given by the following:

$$\Delta t = (0.4 \text{ to } 0.55) \cdot 60 / sr \quad (5).$$

[0036] In one preferred embodiment, 0.4 revolution FWHM is achieved using a single-side-lobe higher order weighting function, which improves temporal resolution but also increases the noise in the reconstruction. Parallel beam reconstruction over 180 degrees with uniform weighting achieves a FWHM of 0.5 revolution. The standard spiral interpolator (smooth triangle with 0.9 peak value) achieves a FWHM of 0.55 revolution. Moreover, in response to the particular phase of the heart being imaged, different weighting functions are selected from the memory 58 which are most appropriate for bringing out or highlighting that phase. That is to say, different functions are used to produce higher quality cardiac images based on the phase of the heart being reconstructed.

[0037] Optionally, the weighting function is selected from the memory 58 such that it employs angular segments of spiral data corresponding to portions of neighbouring cardiac cycles to achieve higher temporal resolution. For this technique, the rotational gantry speed is selected based on the average heart rate to ensure that the aforementioned angular segments are minimally overlapping.

[0038] The cardiac gated spiral CT scanner and imaging techniques of the present invention, while not limited thereto, are particularly well suited to diagnostic 3D visualization and imaging of the heart and associated vasculature. In one preferred embodiment, the cardiac images are used to quantify calcifications. The calcification scoring is more accurate for gated images than ungated ones since the gated images have less motion artifacts. The selection of appropriate patient-specific scanning protocols also leads to uniform and continuous resolution in the z direction. Because of the uniform and continuous z direction resolution: (a) there is a very low probability that coronary calcification is missed; and, (b) the heart is reconstructed in 3D and, hence, a more accurate cardiac scoring algorithm based on 3D measurements is performed.

[0039] Another clinical application is the assessment of the coronary arteries from images reconstructed as proposed in this invention following intravenous injection of a radio-opaque dye. A CT-based coronary screening technique is virtually non-invasive and it may provide the same diagnostic information as provided by coronary angiography. Hence, the desired diagnostic information can be acquired non-invasively for initial screening purposes. Additionally, with volume images, the flexibility to view and assess the arteries from any angle in three dimensions is possible. Angiography,

on the other hand, permits only a limited number of two dimensional projection views.

[0040] Moreover, in another preferred embodiment, applying the principles of continuous CT, functional imaging of the heart is performed. A bolus of contrast is tracked over time for the same phase of the heart using 0-pitch scanning. This gives insight into various flow-related heart abnormalities. In yet another preferred embodiment, comparison of the heart anatomy at various phases of the heart is performed. A segmentation and measurement package accurately yields clinically significant quantities such as end-diastolic volume, stroke volume, ejection fraction, and the dynamics of ventricular wall motion.

[0041] One advantage of the above described cardiac gated spiral CT scanner is that it provides a versatile and selectable protocol for cardiac gated spiral CT imaging which is patient-specific. Another advantage is improved cardiac images with reduced motion artifacts. Yet another advantage is reduced scan times as compared to gated axial slice CT and prospective single cardiac phase spiral CT. One more advantage is that resolution along the longitudinal axis of the scan is maintained for improved three-dimensional imaging and diagnostic evaluations of the heart and associated vasculature. Another advantage is that any selected phase of the heart may be imaged.

Claims

1. A cardiac gated CT scanner comprising:

- a source (20) of penetrating radiation arranged for rotation about an examination region (14) having a central axis extending in a z direction, said source being arranged for (20) emitting a beam of radiation (22) that passes through the examination region (14) as the source (20) rotates;
- a patient support (30) for holding according a patient being examined at least partially within the examination region (14) and which is arranged to translate the patient through the examination region (14) in the z direction;
- radiation detectors (40) arranged to receive radiation emitted from the source (20) after it has traversed the examination region (14);
- an electrocardiogram monitor (80) for acquiring electrocardiogram data from the patient, said electrocardiogram data being used to accurately correlate phases of the patient's heart with data collected by the radiation detectors (40);
- an image reconstruction processor (60) for reconstructing image representations of the patient based on data received from the radiation detectors (40) and ECG monitor (80);
- a human viewable display (70) for selectively displaying the image representations; and
- a control processor (90) for implementing patient-specific scan protocol in response to measured patient characteristics and scanner characteristics,

characterized in that the patient characteristics include an average heart rate and a range of scan coverage in the z direction based on patient anatomy.

2. A cardiac gated CT scanner as claimed in claim 1, wherein the measured patient characteristics include patient breath hold time.

3. A cardiac gated CT scanner as claimed in claim 2, wherein the scan protocol selected sets a pitch for the helical path followed by the source (20) and sets an image slice thickness, such that (i) the patient's average heart rate, (ii) the patient's breath hold time, and (iii) a range of scan coverage in the z direction are accommodated while ensuring that neighboring image slices are at least contiguous in the z direction.

4. A cardiac gated CT scanner as claimed in claim 2 or claim 3, wherein the image representation is of the patient's heart and associated vasculature in a selected phase.

5. A cardiac gated CT scanner as claimed in claim 4, wherein the image representation is three-dimensional.

6. A cardiac gated CT scanner as claimed in any one of claims 1 to 5, wherein the patient support is arranged to translate the patient through the examination region in the z direction while the source (20) is rotated such that the source (20) follows a helical path relative to the patient.

7. A method of cardiac gated CT imaging comprising:

- (a) measuring patient characteristics that include an average heart rate of the patient and a range of scan

coverage in the z direction based on patient anatomy;
 (b) based on results from step (a), selecting a patient-specific scan protocol;
 (c) in accordance with the selected scan protocol, performing a CT scan of the patient while collecting electrocardiogram data from the patient;
 (d) using the electrocardiogram data to correlate phases of the patient's heart with x-ray data collected via the CT scan; and
 (e) reconstructing from the x-ray data collected an image representation of a region of interest of the patient at a point in time corresponding to a selected phase of the patient's heart.

8. A method as claimed in claim 7, wherein the patient characteristics include patient breath hold time.
9. A method as claimed in claim 7 or claim 8, wherein the image representation is three-dimensional.
10. A method as claimed in claim 9, wherein the region of interest includes the patient's heart and associated vasculature.
11. A method as claimed in any one of claims 7 to 10, in which the CT scan performed in step (e) is a spiral CT scan.
12. A method as claimed in claim 11, wherein the selected scan protocol determines (i) a pitch for a spiral path travelled by an x-ray source relative to the patient during the spiral CT scan and (ii) an image slice thickness, such that neighbouring image slices are at least contiguous along a direction of the pitch.

Patentansprüche

1. Cardiac-Gating-CT-Scanner, der Folgendes umfasst:

- eine Quelle (20) durchdringender Strahlung, die für eine Drehung um einen Untersuchungsbereich (14) mit einer sich in z-Richtung erstreckenden Zentralachse eingerichtet ist, wobei die genannte Quelle (20) dafür eingerichtet ist, ein Strahlenbündel (22) zu emittieren, der den Untersuchungsbereich (14) durchquert, während sich die Quelle (20) dreht;
- eine Patientenaufgabe (30), um einen zu untersuchenden Patienten zumindest teilweise innerhalb des Untersuchungsbereichs (14) zu halten, und die dafür eingerichtet ist, den Patienten in z-Richtung durch den Untersuchungsbereich (14) zu befördern;
- Strahlungsdetektoren (40), die dafür vorgesehen sind, von der Quelle (20) emittierte Strahlung aufzunehmen, nachdem sie den Untersuchungsbereich (14) durchquert hat;
- einen Elektrokardiogramm-Monitor (80) zum Erfassen von Elektrokardiogramm-Daten des Patienten, wobei die genannten EKG-Daten verwendet werden, um Phasen des Patientenherzens präzise mit von den Strahlungsdetektoren (40) erfassten Daten zu korrelieren;
- einen Bildrekonstruktionsprozessor (60), um die Bilddarstellungen des Patienten basierend auf den von den Strahlungsdetektoren (40) und dem EKG-Monitor (80) erhaltenen Daten zu rekonstruieren;
- eine von Menschen ablesbare Anzeigevorrichtung (70) zum selektiven Anzeigen der Bilddarstellungen; und
- einen Steuerungsprozessor (90), um ein patientenspezifisches Abtastprotokoll in Reaktion auf gemessene Patientenmerkmale und Scannermerkmale zu implementieren;

dadurch gekennzeichnet, dass die Patientenmerkmale eine mittlere Herzfrequenz und einen Abtastbereich in der z-Richtung basierend auf der Patientenanatomie beinhalten.

2. Cardiac-Gating-CT-Scanner nach Anspruch 1, wobei die gemessenen Patientenmerkmale eine Atemanhaltezeit des Patienten beinhalten.
3. Cardiac-Gating-CT-Scanner nach Anspruch 2, wobei das gewählte Abtastprotokoll eine Steigung für den helikalen Pfad, dem die Quelle (20) folgt, sowie eine Schichtbilddicke festlegt, so dass (i) die mittlere Herzfrequenz des Patienten, (ii) die Atemanhaltezeit des Patienten und (iii) ein Abtastbereich in der z-Richtung berücksichtigt werden, während sichergestellt wird, dass benachbarte Schichtbilder in der z-Richtung zumindest nahtlos aneinander grenzen.
4. Cardiac-Gating-CT-Scanner nach Anspruch 2 oder 3, wobei die Bilddarstellung das Herz des Patienten und das

zugehörige Gefäßsystem in einer gewählten Phase zeigt.

5. Cardiac-Gating-CT-Scanner nach Anspruch 4, wobei die Bilddarstellung dreidimensional ist.

6. Cardiac-Gating-CT-Scanner nach einem der Ansprüche 1 bis 5, wobei die Patientenaufgabe dafür eingerichtet ist, den Patienten in z-Richtung durch den Untersuchungsbereich zu befördern, während die Quelle (20) so gedreht wird, dass sie einem helikalen Pfad relativ zum Patienten folgt.

7. Verfahren zur CT-Bildgebung mittels Cardiac-Gating, das Folgendes umfasst:

- (a) Messen von Patientenmerkmalen, die eine mittlere Herzfrequenz des Patienten und einen Abtastbereich in der z-Richtung basierend auf der Patientenanatomie beinhalten;
- (b) Auswählen eines patientenspezifischen Abtastprotokolls basierend auf den Ergebnissen aus Schritt (a);
- (c) Durchführen einer CT-Abtastung des Patienten gemäß dem gewählten Abtastprotokoll, währenddessen EKG-Daten des Patienten erfasst werden;
- (d) Verwenden der EKG-Daten, um Phasen des Patientenherzens mit Röntgenstrahlendaten zu korrelieren, die über die CT-Abtastung erfasst wurden; und
- (e) Rekonstruieren einer Bilddarstellung einer interessierenden Region des Patienten anhand der erfassten Röntgenstrahlendaten zu einem Zeitpunkt, der einer ausgewählten Phase des Patientenherzens entspricht.

8. Verfahren nach Anspruch 7, wobei die Patientenmerkmale die Atemanhaltezeit des Patienten beinhalten.

9. Verfahren nach Anspruch 7 oder 8, wobei die Bilddarstellung dreidimensional ist.

10. Verfahren nach Anspruch 9, wobei die interessierende Region das Herz des Patienten und das zugehörige Gefäßsystem beinhaltet.

11. Verfahren nach einem der Ansprüche 7 bis 10, wobei die in Schritt (e) durchgeführte CT-Abtastung eine Spiral-CT-Abtastung ist.

12. Verfahren nach Anspruch 11, wobei das gewählte Abtastprotokoll (i) eine Steigung für einen spiralförmigen Pfad, auf dem sich eine Röntgenquelle während der Spiral-CT-Abtastung relativ zum Patienten bewegt, sowie (ii) eine Schichtbilddicke festlegt, so dass benachbarte Schichtbilder entlang einer Richtung der Steigung zumindest nahtlos aneinander grenzen.

Revendications

1. Scanner CT à synchronisation cardiaque, comprenant:

- une source (20) de rayonnement pénétrant prévue pour tourner autour d'une région d'examen (14) ayant un axe central qui s'étend dans une direction z, ladite source (20) étant agencée pour émettre un faisceau de rayonnement (22) qui passe à travers la région d'examen (14) à mesure que la source (20) tourne;
- un support de patient (30) pour maintenir un patient en cours d'examen au moins partiellement dans la région d'examen (14) et qui est agencé pour déplacer le patient à travers la région d'examen (14) dans la direction z;
- des détecteurs de rayonnement (40) agencés pour recevoir le rayonnement émis par la source (20) après qu'il a traversé la région d'examen (14);
- un moniteur d'électrocardiogramme (80) pour acquérir des données d'électrocardiogramme du patient, lesdites données d'électrocardiogramme étant utilisées pour corrélérer de manière précise des phases du coeur du patient avec des données collectées par les détecteurs de rayonnement (40);
- un processeur de reconstruction d'image (60) pour reconstruire des représentations d'images du patient basées sur des données reçues des détecteurs de rayonnement (40) et du moniteur d'électrocardiogramme (ECG) (80);
- un affichage observable par l'homme (70) pour afficher sélectivement les représentations d'images et,
- un processeur de contrôle (90) pour mettre en oeuvre un protocole de balayage spécifique au patient en réaction à des caractéristiques du patient et à des caractéristiques du scanner mesurées,

caractérisé en ce que les caractéristiques du patient comprennent une fréquence cardiaque moyenne et un

intervalle de couverture de balayage dans la direction z sur la base de l'anatomie du patient.

2. Scanner CT à synchronisation cardiaque suivant la revendication 1, dans lequel les caractéristiques mesurées du patient comprennent le temps d'apnée du patient.

3. Scanner CT à synchronisation cardiaque suivant la revendication 2, dans lequel le protocole de balayage sélectionné règle un pas pour le chemin hélicoïdal suivi par la source (20) et règle une épaisseur de coupe tomographique telle que (i) la fréquence cardiaque moyenne du patient, (ii) le temps d'apnée du patient et (iii) un intervalle de couverture de balayage dans la direction z soient adaptés tout en assurant que les coupes tomographiques voisines soient au moins contiguës dans la direction z.

4. Scanner CT à synchronisation cardiaque suivant la revendication 2 ou 3, dans lequel la représentation d'image est une représentation du coeur du patient et du système vasculaire associé dans une phase sélectionnée.

5. Scanner CT à synchronisation cardiaque suivant la revendication 4, dans lequel la représentation d'image est tridimensionnelle.

6. Scanner CT à synchronisation cardiaque suivant l'une quelconque des revendications 1 à 5, dans lequel le support de patient est agencé pour déplacer le patient à travers la région d'examen dans la direction z tandis que la source (20) est entraînée en rotation de sorte que la source (20) suit un trajet hélicoïdal par rapport au patient.

7. Procédé d'imagerie CT à synchronisation cardiaque comprenant:

la mesure de caractéristiques du patient qui comprennent une fréquence cardiaque moyenne du patient et un intervalle de couverture de balayage dans la direction z sur la base de l'anatomie du patient;
sur la base des résultats de l'étape (a), la sélection d'un protocole de balayage spécifique au patient;
suivant le protocole de balayage sélectionné, l'exécution d'un balayage CT du patient tout en collectant des données d'électrocardiogramme du patient;
l'utilisation des données de l'électrocardiogramme pour corréliser des phases du coeur du patient avec des données de rayons X collectées par le biais du balayage CT; et
la reconstruction à partir des données de rayons X collectées d'une représentation d'image d'une région d'intérêt du patient à un point dans le temps correspondant à une phase sélectionnée du coeur du patient.

8. Procédé suivant la revendication 7, dans lequel les caractéristiques du patient comprennent le temps d'apnée du patient.

9. Procédé suivant la revendication 7 ou 8, dans lequel la représentation d'image est tridimensionnelle.

10. Procédé suivant la revendication 9, dans lequel la région d'intérêt comprend le coeur du patient et son système vasculaire associé.

11. Procédé suivant l'une quelconque des revendications 7 à 10, dans lequel le balayage CT exécuté dans l'étape (e) est un balayage CT hélicoïdal.

12. Procédé suivant la revendication 11, dans lequel le protocole de balayage sélectionné détermine (i) un pas pour un trajet hélicoïdal parcouru par une source de rayons X par rapport au patient pendant le balayage CT hélicoïdal et (ii) une épaisseur de coupe tomographique, telle que des coupes tomographiques voisines soient au moins contiguës le long d'une direction du pas.

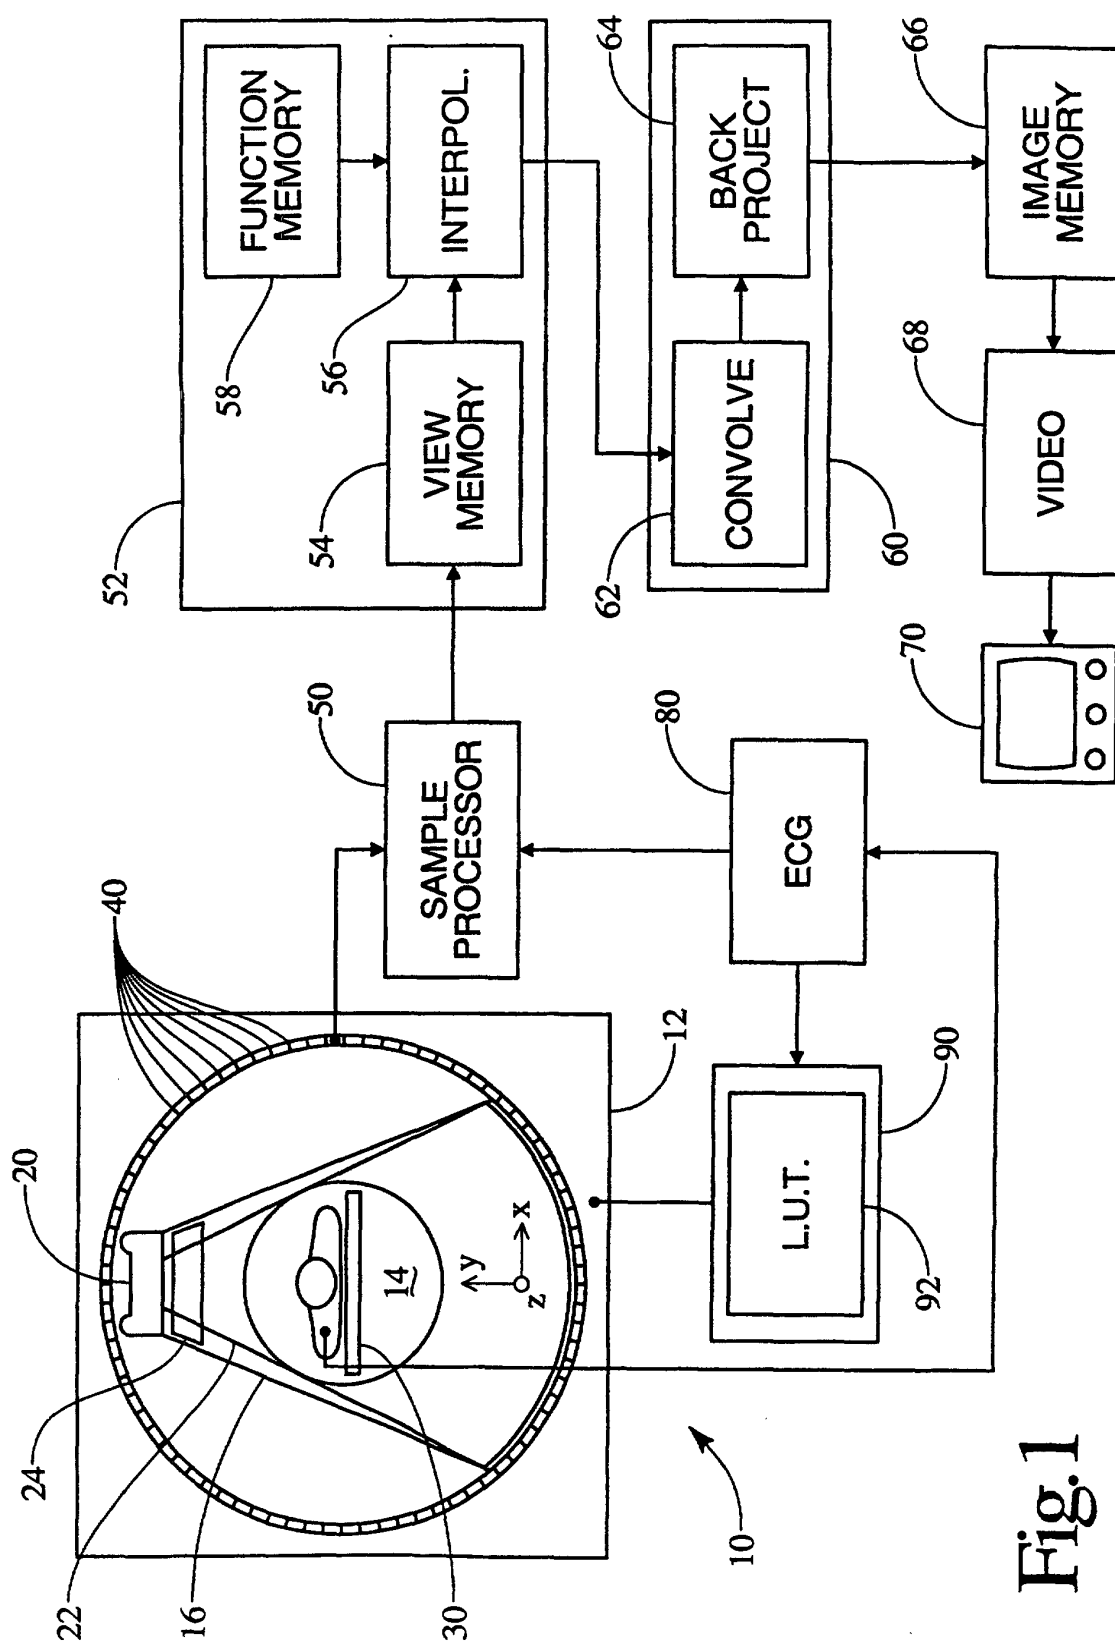


Fig. 1

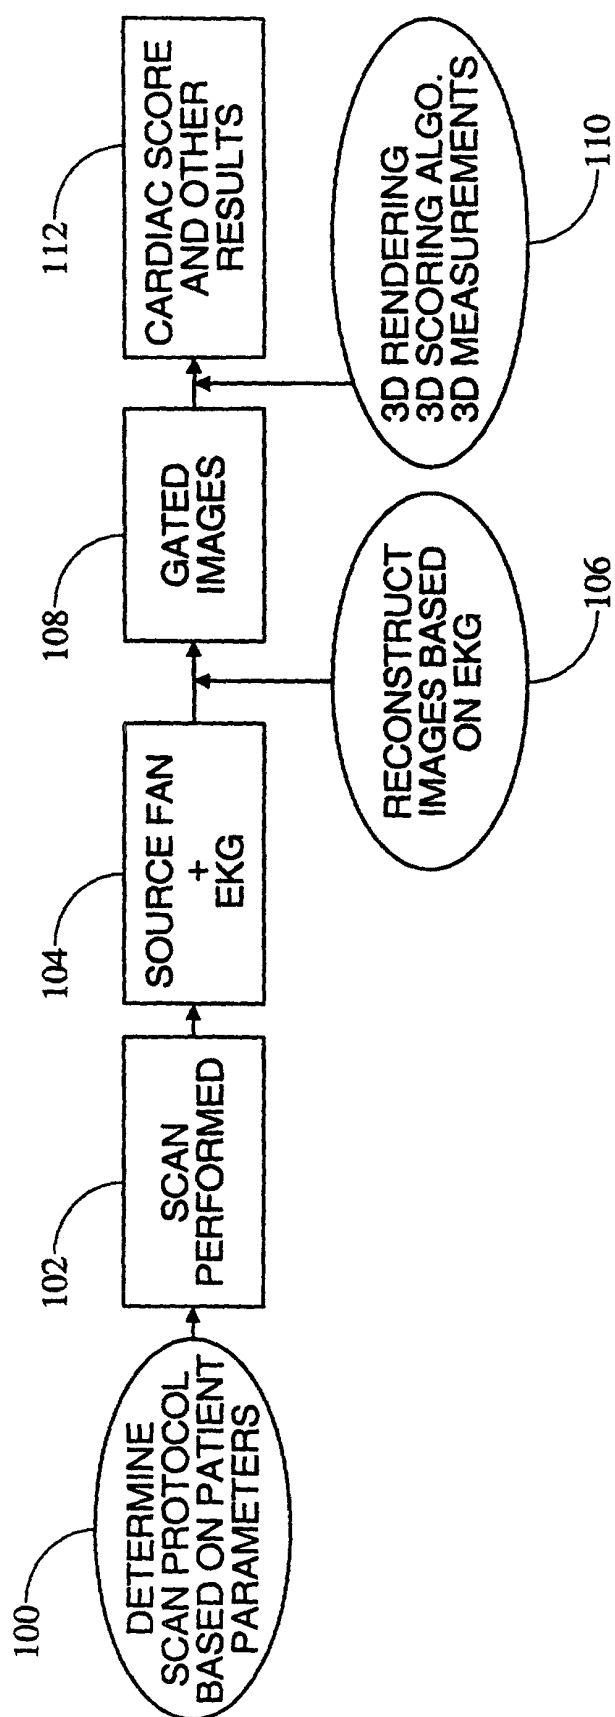


Fig. 2