



US0D1035907S

(12) **United States Design Patent**  
**Ling et al.**

(10) **Patent No.:** **US D1,035,907 S**

(45) **Date of Patent:** **\*\* Jul. 16, 2024**

(54) **DETECTION PEN FOR DETECTING MARKERS IN BIOLOGICAL FLUIDS**

(71) Applicant: **ASSURE TECH. (HANGZHOU) CO., LTD.**, Zhejiang (CN)

(72) Inventors: **Shisheng Ling**, Hangzhou (CN);  
**Yingchong Tong**, Hangzhou (CN)

(73) Assignee: **ASSURE TECH. (HANGZHOU) CO., LTD.**, Hangzhou (CN)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/865,300**

(22) Filed: **Jul. 18, 2022**

(30) **Foreign Application Priority Data**

Jan. 18, 2022 (CN) ..... 202230031895.0

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/223**

(58) **Field of Classification Search**

USPC ..... D24/107, 108, 112–114, 127, 130, 133,  
D24/169, 186, 216–217, 219, 222–226,  
D24/227, 231, 232; D10/81

CPC ..... G01N 33/76; G01N 33/558; G01N  
33/54386; G01N 33/689

See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

D499,812 S *	12/2004	Wu	.....	D24/223
D530,825 S *	10/2006	Lee	.....	D24/223
D531,735 S *	11/2006	Lee	.....	D24/223
D537,531 S *	2/2007	Sigel	.....	D24/223
D672,880 S *	12/2012	Laverack	.....	D24/223
D676,144 S *	2/2013	Laverack	.....	D24/223
D676,546 S *	2/2013	Lovell	.....	D24/113
D694,879 S *	12/2013	Julian	.....	D24/113

D694,903 S *	12/2013	Laverack	.....	D24/223
D698,457 S *	1/2014	Canova	.....	D24/223
D698,937 S *	2/2014	Laverack	.....	D24/223
D875,965 S *	2/2020	Gani	.....	D24/223
D922,608 S *	6/2021	Laverack	.....	D24/223
D935,049 S *	11/2021	Laverack	.....	D24/223
D954,981 S *	6/2022	Laverack	.....	D24/223
D981,003 S *	3/2023	Laverack	.....	D24/223

**OTHER PUBLICATIONS**

Fertility Tests. Online, published date unknown. Retrieved on Dec. 7, 2023 from URL: <https://www.diareagent.com/products-details-en.php?id=3>.\*

Find Out How Fertile You Are With the Best At-Home Fertility Tests. Online, published date May 11, 2023. Retrieved on Dec. 6, 2023 from URL: <https://www.verywellfamily.com/best-at-home-fertility-test-5080788>.\*

\* cited by examiner

*Primary Examiner* — Omeed Agilee

(74) *Attorney, Agent, or Firm* — METIS IP LLC

(57) **CLAIM**

The ornamental design for a detection pen for detecting markers in biological fluids, as shown and described.

**DESCRIPTION**

FIG. 1 is front view of a detection pen for detecting markers in biological fluids according to our new design;

FIG. 2 is a rear view thereof;

FIG. 3 is a left side view thereof;

FIG. 4 is a right side view thereof;

FIG. 5 is a top view thereof;


FIG. 6 is a bottom view thereof;


FIG. 7 is a front perspective view thereof; and,

FIG. 8 is a rear perspective view thereof.


The broken lines in the drawings depict portions of the detection pen for detecting markers in biological fluids that form no part of the claimed design.

**1 Claim, 8 Drawing Sheets**

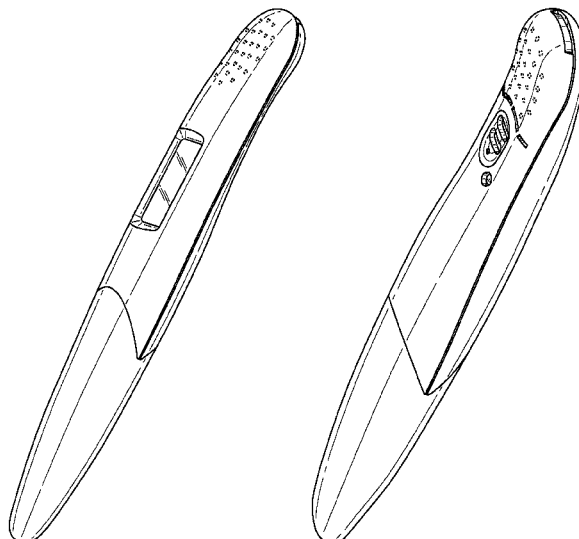


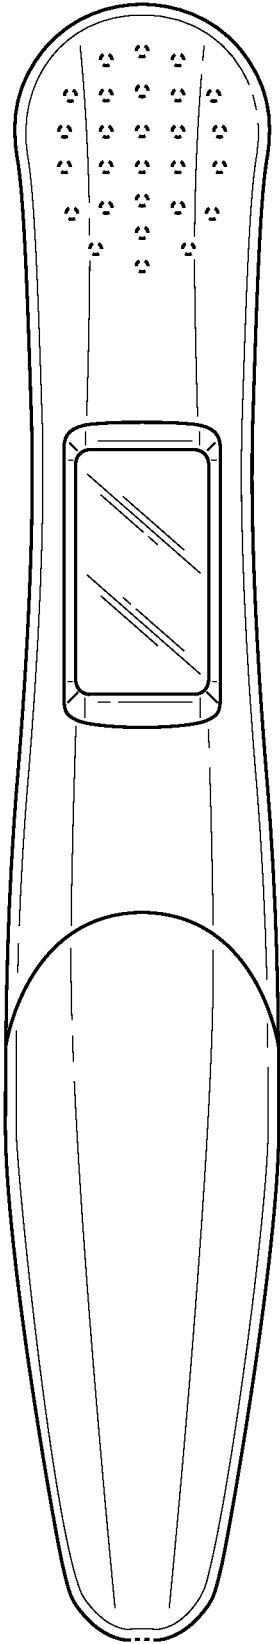


**FIG. 1**

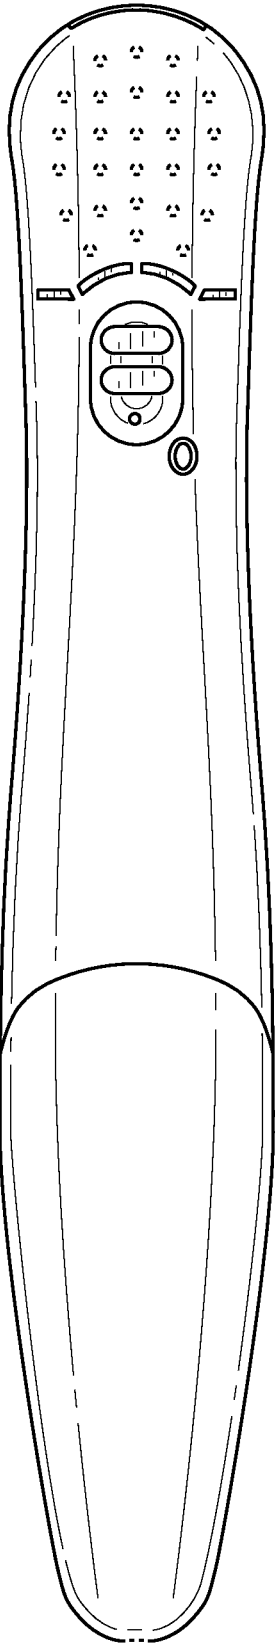


**FIG. 2**

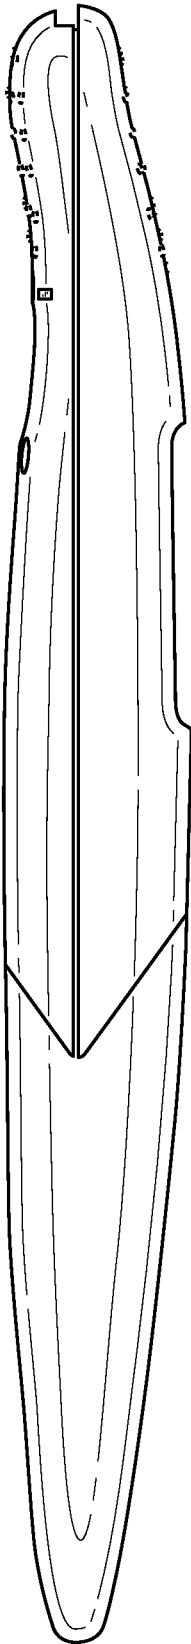


**FIG. 3**

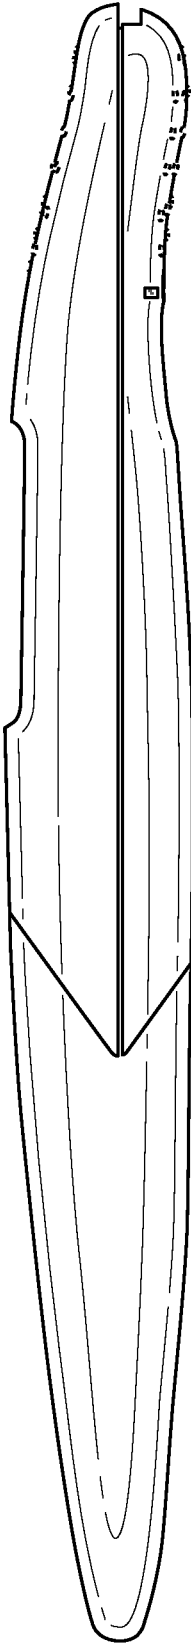


**FIG. 4**




**FIG. 5**



**FIG. 6**

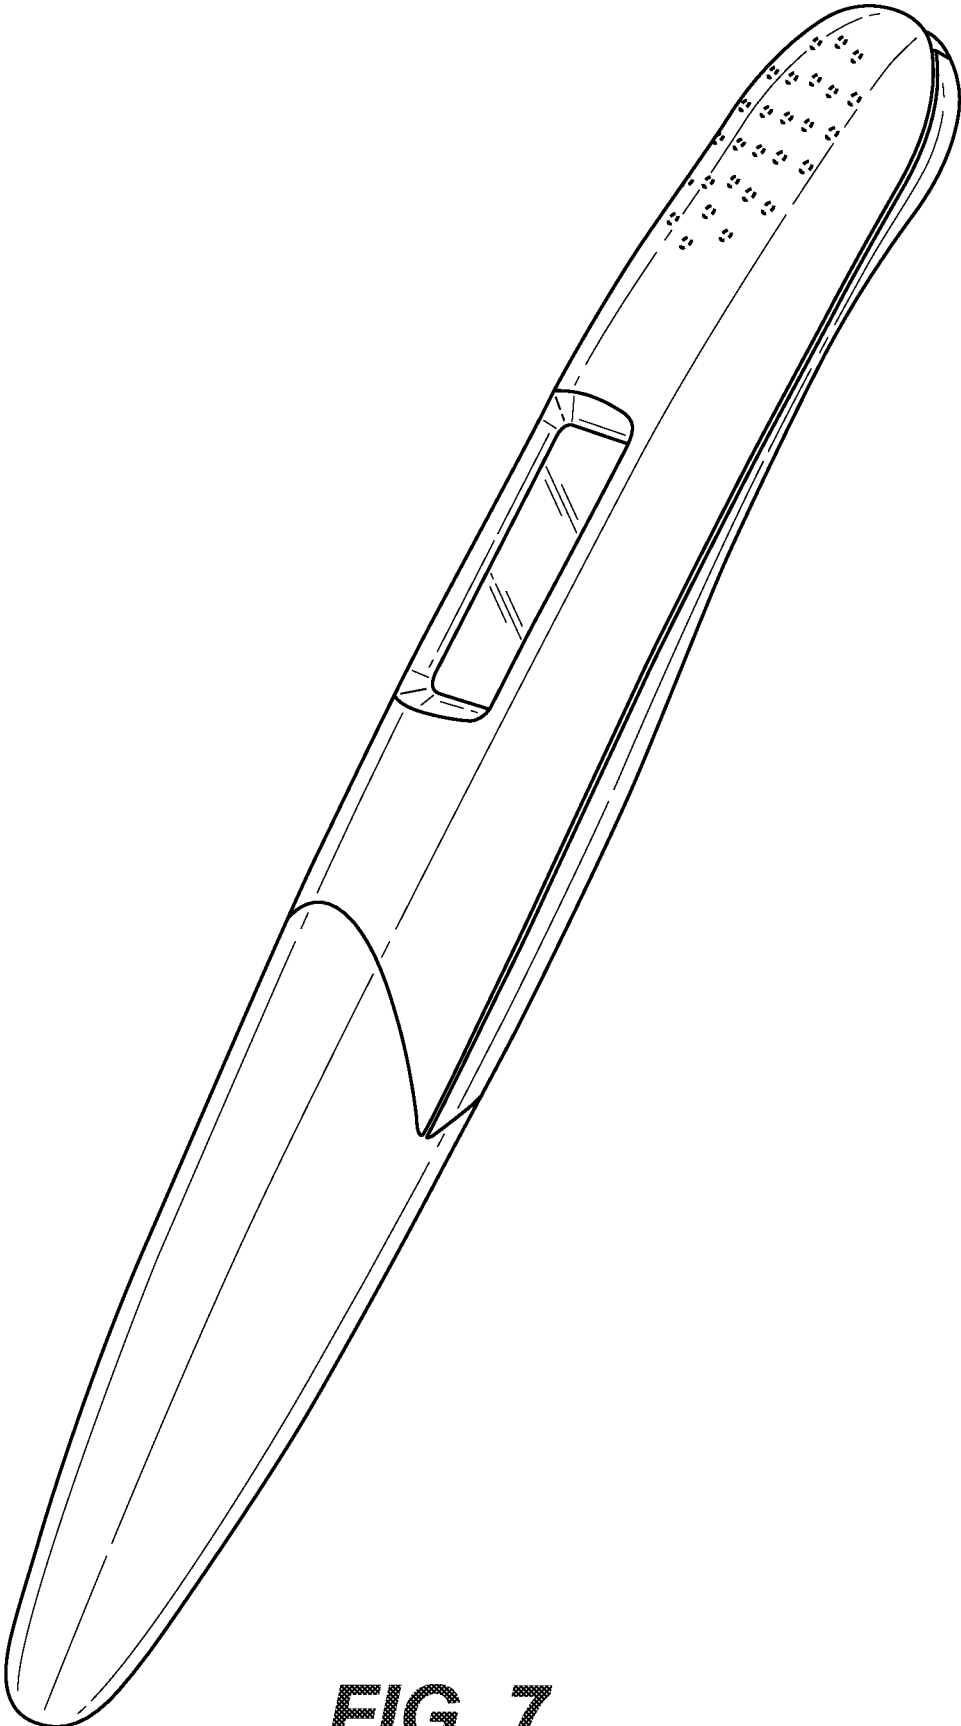

**FIG. 7**

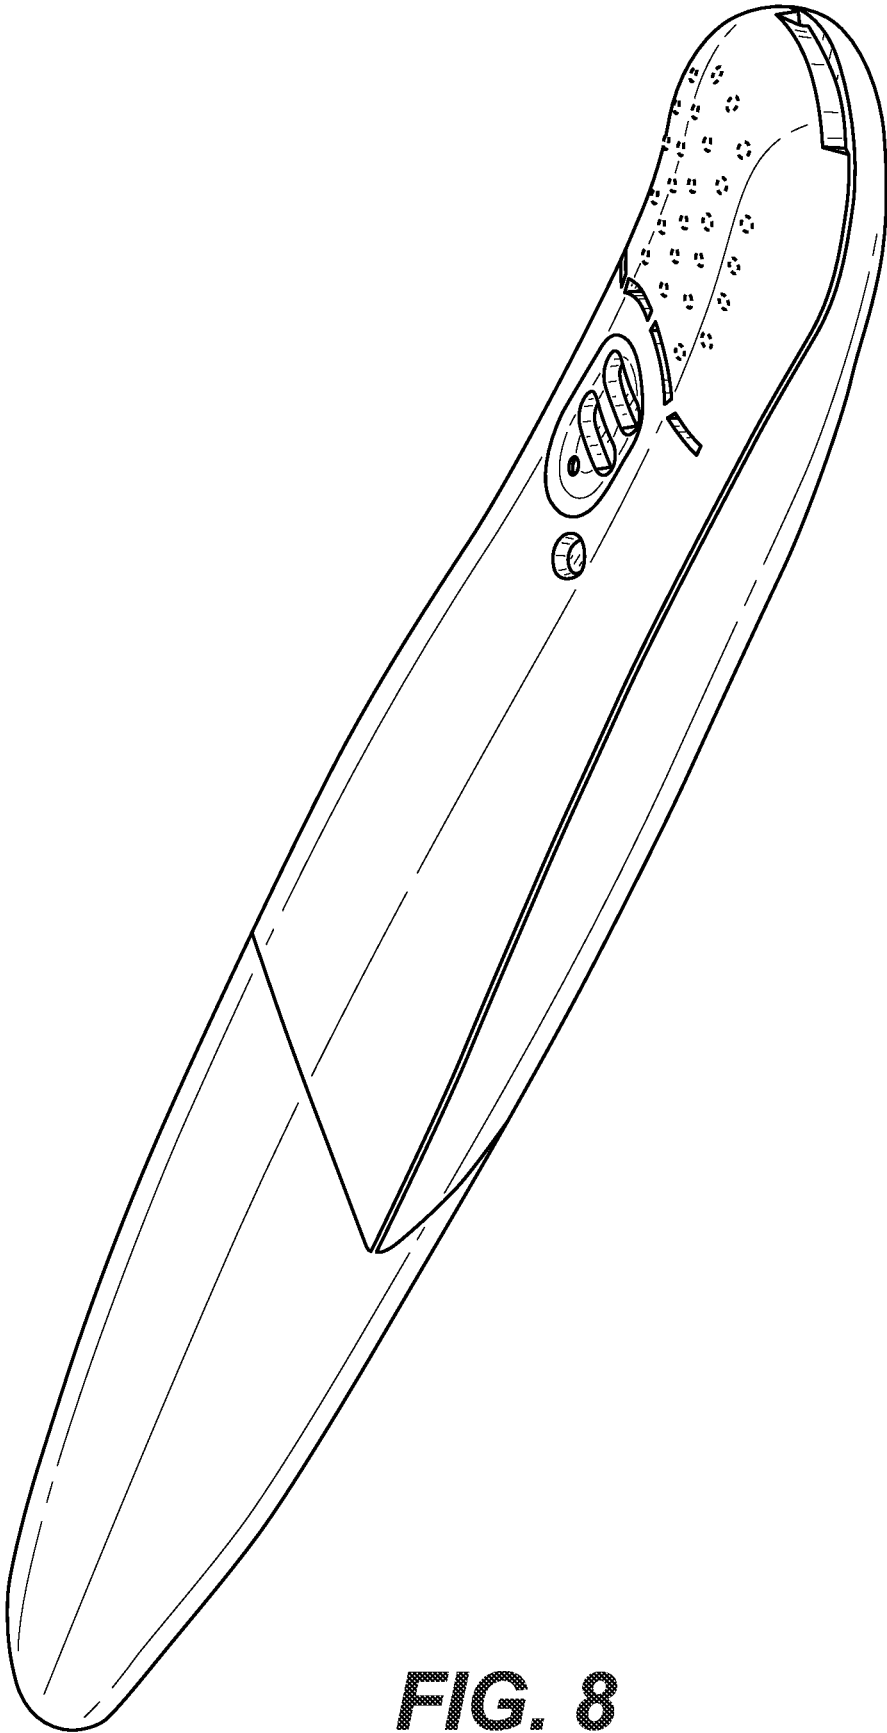

**FIG. 8**