



(51) International Patent Classification:
A61M 1/00 (2006.01)

(21) International Application Number:
PCT/US2012/038945

(22) International Filing Date:
22 May 2012 (22.05.2012)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/490,880 27 May 2011 (27.05.2011) US

(71) Applicant (for all designated States except US): **KCI LICENSING, INC.** [US/US]; P.O. Box 659508, San Antonio, TX 78265 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **LOCKE, Christopher, B.** [GB/GB]; c/o KCI Licensing, Inc., P.O. Box 659508, San Antonio, TX 78265 (US). **BENDELE, Kevin** [US/US]; c/o KCI Licensing, Inc., P.O. Box 659508, San Antonio, TX 78265 (US). **LUCKEMEYER, James** [US/US]; c/o KCI Licensing, Inc., P.O. Box 659508, San Antonio, TX 78265 (US).

(74) Agent: **SPENCE, Chris, W.**; Fulbright & Jaworski L.L.P., 98 San Jacinto Boulevard, Suite 1100, Austin, TX 78701 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: SYSTEMS AND METHODS FOR DELIVERING FLUID TO A WOUND THERAPY DRESSING

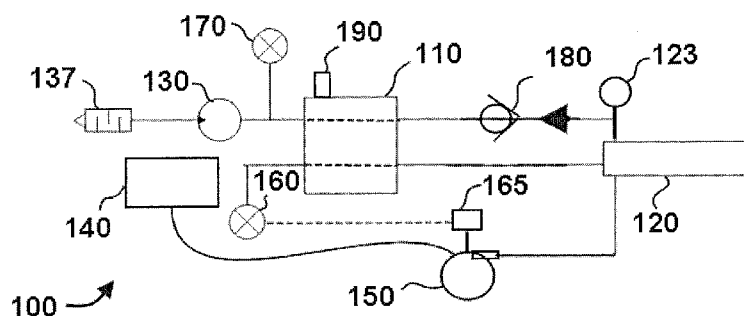


FIG. 1

(57) Abstract: Systems and methods for delivery of fluid to a wound therapy dressing. In exemplary embodiments, a pressure sensor measures the pressure at the wound therapy dressing and restricts fluid flow to the wound therapy dressing when a predetermined pressure is achieved.



DESCRIPTION

SYSTEMS AND METHODS FOR DELIVERING FLUID TO A WOUND THERAPY DRESSING

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims priority to U.S. Provisional Patent Application Serial No. 61/490,880, filed May 27, 2011, the entire contents of which are incorporated herein by reference.

BACKGROUND OF THE INVENTION

FIELD OF THE INVENTION

[0002] Embodiments of the invention relate to fluid (*e.g.*, liquid) delivery to a wound therapy dressing and more particularly relate to systems and methods for automated fluid delivery to a negative pressure wound therapy dressing.

DESCRIPTION OF THE RELATED ART

[0003] Existing fluid delivery systems for wound therapy dressings are typically based on infusion systems. It is worth noting that with drug delivery systems, the user is responsible for determining the dosage of the fluids and would not generally use an automated system to determine the desired volume of liquid that should be delivered.

[0004] However, if one considers the art with respect to fluid delivery for wound dressings, such an approach may not be appropriate. For example, wound dressing fluid delivery systems are not delivering intravenous drugs. Furthermore, wounds are not uniform and indeed will change volume as the therapy progresses. Consequently, using techniques employed in other areas to prescribe a dose volume may result in under- or over-delivery of fluids with the commensurate problems. In existing delivery systems, fluid pressure may be monitored to determine if there is a line blockage, but it is typically not monitored to determine the pressure of the fluid at the site of delivery.

[0005] The referenced shortcomings are not intended to be exhaustive, but rather are among many that tend to impair the effectiveness of previously known techniques in fluid delivery to wound dressings; however, those mentioned here are sufficient to demonstrate that the methodologies appearing in the art have not been satisfactory and that a significant need exists for the techniques described and claimed in this disclosure. Instillation of fluid as an adjunct to negative pressure wound therapy (NPWT) is currently accomplished by asking the user to specify an instillation time (gravity feed systems) or instillation volume (active pumping systems).

[0006] Because it is difficult to judge the volume of a dressed wound, either approach can be problematic and time-consuming to arrive at the desired fill volume. A “Fill Assist” approach has also been used, which requires the user to stop metered fluid flow based on visual observation of the wound filling; whereafter, the automated system dispenses the same volume in subsequent instillation cycles.

[0007] However, even this simplified approach requires that the user be attentive to stopping the flow, and can easily lead to over-filling the wound, waste of NPWT collection canister volume, and potentially instillation fluid leakage at the dressing. It is therefore desirable that automated systems and methods be developed to allow the user to determine when the wound dressing has received the proper volume of liquid for instillation.

SUMMARY OF THE INVENTION

[0008] From the foregoing discussion, it should be apparent that a need exists for a system and method for improved delivery of fluid to a wound therapy dressing.

[0009] The method in the disclosed embodiments substantially includes the steps necessary to carry out the functions presented above with respect to the operation of the described system.

[0010] Exemplary embodiments of the present disclosure can provide automated delivery of fluid to a wound therapy dressing. Such automation not only frees a caregiver from having to be attentive to the device rather than the patient, but addresses a perceived problem in that the caregiver may have difficulty making a judgment about when the dressing is appropriately filled.

[0011] Exemplary embodiments can provide for increased efficiency in both caregiver's time and reduced waste of instillation fluids. For example, exemplary embodiments can reduce the likelihood of accidental overfilling of the dressing caused by a distracted or non-attentive user or caregiver. Such overfilling can require a time-consuming cycling of the system in order to repeat the fluid delivery feature or cause other operational issues. Further, there is no requirement for the caregiver to estimate wound volume or provide other input to the automated fill system.

[0012] Exemplary embodiments of this disclosure provide an automated fluid delivery system, improving the caregiver's ability to determine the correct fill level which in turn ensures that the pneumatic performance is not compromised by an overfill condition.

[0013] Exemplary embodiments of the present disclosure are configured for delivering fluid to a volume space, which have (prior to instillation) been evacuated to a known pressure

and verified to not have leaks. Exemplary embodiments have the advantage of using the equalization of pressure which occurs as a fluid fills the dressing volume to provide an indicator of the correct fill level.

[0014] Certain embodiments include a system for delivering fluid to a negative pressure wound therapy dressing. In specific embodiments, the system comprises: a wound dressing; a negative pressure source coupled to the wound dressing; a fluid flow device in fluid communication with the wound dressing; a control device configured to control a fluid flow from the fluid flow device; and a pressure sensor coupled to the wound dressing and to the control device. In particular embodiments, the pressure sensor is configured to send a control signal to the control device and control fluid flow from the fluid flow device when pressure sensor detects a predetermined pressure at the wound dressing. Certain embodiments comprise a visual or audible indicator when the pressure sensor detects the predetermined pressure at the wound dressing. In particular embodiments, the fluid flow device can be a pump, including for example, a peristaltic pump or a centrifugal pump. In certain embodiments the fluid flow device can be a valve.

[0015] In specific embodiments, the control device is a control switch configured to turn the pump on or off. In particular embodiments, the control device is an actuator configured to change the position of the valve. In certain embodiments, the fluid flow device is a solenoid-actuated pinch valve. Particular embodiments may further comprise a reservoir coupled to the negative pressure source and in fluid communication with the fluid flow device. In specific embodiment, a fluid can flow from the reservoir to the wound dressing via a gravity feed system.

[0016] Particular embodiments may also comprise a check valve between the wound dressing and the reservoir, where the check valve is configured to restrict fluid flow to the reservoir when the reservoir is not at a negative pressure. In certain embodiments, the control device comprises a control switch configured to stop operation of the fluid flow device when the pressure sensor detects a predetermined pressure at the wound dressing. In specific embodiments, the control device comprises a solenoid valve configured to close when the pressure sensor detects a predetermined pressure at the wound dressing. In particular embodiments, the predetermined pressure is between approximately -1.0 mm Hg and 1.0 mm Hg, and in specific embodiments approximately 0.0 mm Hg.

[0017] Certain embodiments comprise a method for delivering fluid to a wound therapy dressing. In particular embodiments, the method comprises: creating a negative pressure on a wound therapy dressing; delivering fluid to the wound therapy dressing; monitoring pressure

at the wound therapy dressing via a pressure sensor; and restricting fluid delivery when the pressure reaches a predetermined value. In specific embodiments, restricting the fluid delivery comprises activating a control switch to cut off a supply of energy to a pump. In particular embodiments, restricting fluid delivery comprises closing a valve between a fluid flow device and the wound therapy dressing. In certain embodiments, the valve can be a solenoid valve.

[0018] Specific embodiments further comprise deactivating the negative pressure source prior to delivering fluid to the wound therapy dressing. Certain embodiments further comprise providing fluid flow to the wound therapy dressing via a gravity feed system. Particular embodiments further comprise providing a reservoir between the negative pressure source and the wound therapy dressing. Certain embodiments can also comprise providing a check valve between the negative pressure source and the wound therapy dressing, where the check valve is configured to restrict flow from the negative pressure source to the wound therapy dressing. Specific embodiments can also comprise venting the reservoir to atmosphere after de-activating the negative pressure source and prior to activating the pump to deliver fluid to the wound therapy dressing. In particular embodiments, the predetermined pressure is between approximately -1.0 mm Hg and 1.0 mm Hg, and in specific embodiments approximately 0.0 mm Hg.

[0019] Other features and associated advantages will become apparent with reference to the following detailed description of specific embodiments in connection with the accompanying drawings.

[0020] The term “coupled” is defined as connected, although not necessarily directly, and not necessarily mechanically.

[0021] The terms “a” and “an” are defined as one or more unless this disclosure explicitly requires otherwise.

[0022] The term “substantially” and its variations are defined as being largely but not necessarily wholly what is specified as understood by one of ordinary skill in the art, and in one non-limiting embodiment “substantially” refers to ranges within 10%, preferably within 5%, more preferably within 1%, and most preferably within 0.5% of what is specified.

[0023] The terms “comprise” (and any form of comprise, such as “comprises” and “comprising”), “have” (and any form of have, such as “has” and “having”), “include” (and any form of include, such as “includes” and “including”) and “contain” (and any form of contain, such as “contains” and “containing”) are open-ended linking verbs. As a result, a method or device that “comprises,” “has,” “includes” or “contains” one or more steps or

elements possesses those one or more steps or elements, but is not limited to possessing only those one or more elements. Likewise, a step of a method or an element of a device that “comprises,” “has,” “includes” or “contains” one or more features possesses those one or more features, but is not limited to possessing only those one or more features. Furthermore, a device or structure that is configured in a certain way is configured in at least that way, but may also be configured in ways that are not listed.

[0024] The term “negative pressure” refers to an absolute pressure that is lower than the absolute atmospheric pressure at the location of use of the device. A stated level of negative pressure in a region is therefore a relative measure between the absolute atmospheric pressure and the absolute pressure in the region. A statement that the negative pressure is increasing means the pressure in the region is moving towards atmospheric pressure (*i.e.* the absolute pressure is increasing). Where numeric values are used, a negative sign is placed in front of the numeric pressure value to indicate the value is a negative pressure relative to atmospheric pressure.

BRIEF DESCRIPTION OF THE DRAWINGS

[0025] The following drawings form part of the present specification and are included to further demonstrate certain aspects of exemplary embodiments of the present invention.

[0026] FIG. 1 is a schematic block diagram illustrating one embodiment of a system for delivering fluid to a wound therapy dressing in a first mode of operation.

[0027] FIG. 2 is a schematic block diagram of the embodiment of FIG. 1 in a second mode of operation.

[0028] FIG. 3 is a schematic block diagram of the embodiment of FIG. 1 in a third mode of operation.

[0029] FIG. 4 is an orthogonal view illustrating the embodiment of FIG. 1 for delivering fluid to a wound therapy dressing in a first mode of operation.

[0030] FIG. 5 is an orthogonal view illustrating the embodiment of FIG. 4 in a second mode of operation.

[0031] FIG. 6 is an orthogonal view illustrating the embodiment of FIG. 4 in a second mode of operation.

[0032] FIG. 7 is a flowchart illustrating a series of steps that can be performed in one embodiment of a method for delivering fluid to a wound therapy dressing.

DETAILED DESCRIPTION OF EXEMPLARY EMBODIMENTS

[0033] Various features and advantageous details are explained more fully with reference to the non-limiting embodiments that are illustrated in the accompanying drawings and detailed in the following description. Descriptions of well known starting materials, processing techniques, components, and equipment are omitted so as not to unnecessarily obscure the invention in detail. It should be understood, however, that the detailed description and the specific examples, while indicating embodiments of the invention, are given by way of illustration only, and not by way of limitation. Various substitutions, modifications, additions, and/or rearrangements within the spirit and/or scope of the underlying inventive concept will become apparent to those skilled in the art from this disclosure.

[0034] In the following description, numerous specific details are provided, such as examples of material selections, dimensions, etc., to provide a thorough understanding of the present embodiments. One skilled in the relevant art will recognize, however, that the invention may be practiced without one or more of the specific details, or with other methods, components, materials, and so forth. In other instances, well-known structures, materials, or operations are not shown or described in detail to avoid obscuring aspects of the invention.

[0035] FIGS. 1-3 illustrate one embodiment of a system 100 for providing fluid delivery to a negative pressure wound therapy system. In the exemplary embodiment shown, system 100 includes a reservoir 110, a wound dressing 120, and a negative pressure source 130 coupled to reservoir 110 and wound dressing 120. In this embodiment, system 100 further comprises a fluid flow device 150 (*e.g.* a pump or valve, as discussed below) in fluid communication with a fluid supply reservoir 140 and wound dressing 120.

[0036] Certain embodiments may utilize a gravity fluid flow from fluid supply reservoir 140 to wound dressing 120 without utilizing a pumping device for fluid flow device 150. In such embodiments, fluid flow device 150 may be a valve (*e.g.*, a solenoid-actuated pinch valve) configured to control the flow of fluid between fluid supply reservoir 140 and wound dressing 120. In still other embodiments, negative pressure source 130 may draw fluid into wound dressing 120 from fluid supply reservoir 140, without the aid of gravity feed or a pumping action from fluid flow device 150.

[0037] In particular exemplary embodiments, negative pressure source 130 may comprise a diaphragm vacuum pump. In certain embodiments, system 100 may also comprise a filter

or muffler 137 coupled to negative pressure source 130 to reduce the operating noise of negative pressure source 130 and/or filter air exiting negative pressure source 130.

[0038] In certain exemplary embodiments, fluid flow device 150 may comprise a pump, *e.g.*, a peristaltic, centrifugal or other suitable pump. In other exemplary embodiments, fluid flow device may comprise a gravity feed system instead of (or in conjunction with) a pump to deliver fluid to wound dressing 120. In such embodiments, a valve between the gravity feed system and wound dressing 120 can be used to restrict the fluid flow to wound dressing 120 when the predetermined pressure is reached, as explained more fully below.

[0039] In the disclosed embodiment, system 100 also comprises a vent 190 on reservoir 110, and a check valve 180 configured to allow flow in the direction from wound dressing 120 towards negative pressure source 130, and restrict fluid flow in the reverse direction. The exemplary embodiment shown in FIGS. 1-3 also comprises a pressure sensor 160 coupled to wound dressing 120, as well as a pressure sensor 170 coupled to negative pressure source 130 and wound dressing 120.

[0040] FIGS. 1-3 illustrate three modes of operation of system 100. In FIG. 1, negative pressure source 130 is activated to create a negative pressure on wound dressing 120, while fluid flow device 150 is not activated. In FIG. 2, negative pressure source 130 is not activated, but fluid flow device 150 is activated to provide a fluid flow to wound dressing 120. In FIG. 3, both negative pressure source 130 and fluid flow device 150 are not activated.

[0041] During initial operation of system 100 shown in FIG. 1, negative pressure source 130 is activated to create a negative pressure on reservoir 110 and wound dressing 120. The pressure at negative pressure source 130 and reservoir 110 and wound dressing 120 can be monitored via pressure sensor 170, as well as pressure sensor 160 (assuming normal operation without blockages in the conduit coupling the components). When the desired level of negative pressure (*e.g.*, -125 mm Hg) is achieved, negative pressure source 130 can be deactivated and vent 190 can be opened to vent reservoir 110 to atmosphere. In certain embodiments, check valve 180 maintains the negative pressure on wound dressing 120, which can be monitored via pressure sensor 160. In particular embodiments, check valve 180 may be a duckbill type or ball-check type or flap type valve.

[0042] Fluid flow device 150 can then be activated to begin fluid delivery to wound dressing 120. In particular embodiments, fluid flow device 150 may be configured to flow approximately 100 ml/minute. As fluid is pumped from fluid flow device 150 to wound dressing 120, the pressure at wound dressing 120 (which can be monitored via pressure sensor 160) will increase. When wound dressing 120 reaches a predetermined pressure, pressure

sensor 160 (which may be used to sense both positive and negative pressures) can send a control signal to control device 165 (*e.g.* a control switch or actuator) to restrict fluid flow from fluid flow device 150 to wound dressing 120. The increase in pressure of wound dressing 120 can be used as an indication that fluid from fluid flow device 150 has sufficiently filled wound dressing 120. By monitoring the pressure of wound dressing 120 with pressure sensor 160, system 100 can reduce the likelihood that wound dressing 120 will be overfilled. This can reduce waste of fluid and leakage of wound dressing associated with overfilling. It is understood that interface circuitry (not shown) may be utilized to generate a sufficiently strong control signal and to implement the control logic.

[0043] As previously mentioned, in certain embodiments, fluid flow device 150 may be a valve (*e.g.*, a solenoid-actuated pinch valve) that restricts fluid flow from fluid supply reservoir 140 or a pump that is activated to provide fluid flow. The operation of fluid flow device 150 (*e.g.*, the position of a valve or the activation/deactivation of a pump) may be automatically altered when a predetermined pressure is reached at wound dressing 120. In exemplary embodiments, the predetermined pressure of wound dressing 120 at which the operation of fluid flow device 150 is altered may be approximately 1.0 mm Hg (gauge pressure as measured by pressure indicator 160). In specific embodiments the predetermined pressure may be -10 and 10 mm Hg, including -10, -9, -8, -7, -6, -5, -4, -3, -2, -1, 0, 1, 2, 3, 4, 5, 6, 7, 8, 9 or 10 mm Hg, or any values between.

[0044] In other embodiments a user may monitor pressure sensor 160 and manually control operation of fluid flow device 150 when wound dressing 120 reaches the predetermined pressure. For example, a user may deactivate fluid flow device 150 by manipulating a control switch or restrict fluid flow from fluid flow device 150 by closing a valve.

[0045] When wound dressing 120 is sufficiently filled with fluid, the user may continue with the desired fluid instillation and vacuum therapy treatments. Exemplary embodiments can be used for each instillation cycle, which may offer advantages for wound dressings on articulated joints (*e.g.*, knee) where the wound or dressing volume could be influenced by the patient's body position. In certain embodiments utilizing a foam dressing, the dressing volume can change over time in part due to compression-set of the foam. For example, the volume of the foam may be reduced over time as the foam is subjected to pressure. This change in volume occupied by the foam can affect the volume of fluid needed to fill wound dressing 120. Such volume changes can be accommodated by exemplary embodiments,

which utilize pressure readings to indicate when the wound dressing has received a sufficient volume of liquid.

[0046] It is understood that the features shown FIGS. 1-3 and described in the accompanying discussion of the figures are merely one exemplary embodiment of the present disclosure. Other embodiments, for example, may utilize absorption layers in the wound dressing instead of, or in addition to, a reservoir.

[0047] Referring now to FIGS. 4-6, orthogonal views of previously-described system 100 are shown in the three modes of operation illustrated in FIGS. 1-3. In FIG. 4, negative pressure source 130 is activated to create a negative pressure on reservoir 110 and wound dressing 120 (via conduit 135). In this stage of operation, there is no fluid in wound dressing 120.

[0048] As shown in FIG. 5, negative pressure source 130 is deactivated, and fluid flow device 150 is activated to begin fluid flow to wound dressing 120. As shown in FIG. 5, fluid 125 from fluid flow device 150 has begun entering wound dressing 120, via conduit 155. As fluid 125 enters wound dressing 120, the pressure measured by pressure sensor 160 increases.

[0049] Referring now to FIG. 6, a sufficient volume of fluid 125 has entered wound dressing 120 to increase the pressure to the predetermined pressure, indicating that the desired volume of fluid 125 is located in wound dressing 120. At this stage of operation, pressure sensor 160 can provide information to a control circuit to restrict the flow of fluid 125 from fluid flow device 150. As explained above, pressure sensor 160 may send a control signal to control the operation of fluid flow device 150. For example, pressure sensor 160 may send a control signal to deactivate fluid flow device 150 if it is configured as a pump. Pressure sensor 160 may also send a control signal to close a valve if fluid flow device 150 is configured as a valve.

[0050] In certain embodiments, system 100 may comprise an audible or visual pressure indicator 123 at the dressing or elsewhere in the negative pressure path (e.g., a PrevenaTM dressing type available from Kinetic Concepts, Inc., San Antonio, Texas U.S.A. has a visual indicator that retracts when the dressing is below a pressure setpoint and extends when the dressing is above the pressure setpoint) that the predetermined pressure has been reached and that wound dressing 120 contains a sufficient volume of fluid 125. At this stage, the user may proceed with the desired fluid instillation and vacuum therapy treatments.

[0051] The schematic flow chart diagrams that follow are generally set forth as logical flow chart diagrams. As such, the depicted order and labeled steps are indicative of one embodiment of the presented method. Other steps and methods may be conceived that are

equivalent in function, logic, or effect to one or more steps, or portions thereof, of the illustrated method. Additionally, the format and symbols employed are provided to explain the logical steps of the method and are understood not to limit the scope of the method. Although various arrow types and line types may be employed in the flow chart diagrams, they are understood not to limit the scope of the corresponding method. Indeed, some arrows or other connectors may be used to indicate only the logical flow of the method. For instance, an arrow may indicate a waiting or monitoring period of unspecified duration between enumerated steps of the depicted method. Additionally, the order in which a particular method occurs may or may not strictly adhere to the order of the corresponding steps shown.

[0052] Referring now to FIG. 7, a method 200 is disclosed comprising a series of steps that may be executed for the operation of an exemplary system according to this disclosure. Certain embodiments may comprise a tangible computer readable medium comprising computer readable code that, when executed by a computer, causes the computer to perform operations comprising the steps disclosed in FIG. 7.

[0053] In this exemplary embodiment, step 210 comprises activating the negative pressure source to create negative pressure on the wound dressing. Step 220 comprises deactivating the negative pressure source and maintaining negative pressure on the wound dressing. Step 230 comprises activating the fluid flow device to begin fluid flow to the wound dressing, in this embodiment. Step 240 comprises monitoring the wound dressing pressure with the pressure sensor and determining when the predetermined wound dressing pressure is reached. In this embodiment, step 250 comprises sending a control signal from the pressure sensor to the control device to stop the fluid flow from the fluid flow device.

[0054] All of the methods disclosed and claimed herein can be made and executed without undue experimentation in light of the present disclosure. While the apparatus and methods of this invention have been described in terms of preferred embodiments, it will be apparent to those of skill in the art that variations may be applied to the methods and in the steps or in the sequence of steps of the method described herein without departing from the concept, spirit and scope of the invention. In addition, modifications may be made to the disclosed apparatus, and components may be eliminated or substituted for the components described herein, where the same or similar results would be achieved. All such similar substitutes and modifications apparent to those skilled in the art are deemed to be within the spirit, scope, and concept of the invention as defined by the appended claims.

CLAIMS

We claim:

1. A system for delivering fluid to a negative pressure wound therapy dressing, the system comprising:
 - a wound dressing;
 - a negative pressure source coupled to the wound dressing;
 - a fluid flow device in fluid communication with the wound dressing;
 - a control device configured to control a fluid flow from the fluid flow device; and
 - a pressure sensor coupled to the wound dressing and to the control device, wherein the pressure sensor is configured to send a control signal to the control device and control fluid flow from the fluid flow device when the pressure sensor detects a predetermined pressure at the wound dressing.
2. The system of claim 1, further comprising a visual or audible indicator when the pressure sensor detects the predetermined pressure at the wound dressing.
3. The system of claim 1 wherein the fluid flow device is a pump.
4. The system of claim 3 wherein the control device is a control switch configured to turn the pump on or off.
5. The system of claim 1 wherein the fluid flow device is a peristaltic pump.
6. The system of claim 1 wherein the fluid flow device is a centrifugal pump.
7. The system of claim 1 wherein the fluid flow device is a valve.
8. The system of claim 7 wherein the control device is an actuator configured to change the position of the valve.
9. The system of claim 1 wherein the fluid flow device is a solenoid-actuated pinch valve.

10. The system of claim 1 further comprising a reservoir coupled to the negative pressure source and in fluid communication with the fluid flow device.
11. The system of claim 10 wherein a fluid can flow from the reservoir to the wound dressing via a gravity feed system.
12. The system of claim 10 further comprising a check valve between the wound dressing and the reservoir, wherein the check valve is configured to restrict fluid flow to the reservoir when the reservoir is not at a negative pressure.
13. The system of claim 1 wherein the control device comprises a control switch configured to stop operation of the fluid flow device when the pressure sensor detects a predetermined pressure at the wound dressing.
14. The system of claim 1 wherein the control device comprises a solenoid valve configured to close when the pressure sensor detects a predetermined pressure at the wound dressing.
15. The system of claim 1 wherein the predetermined pressure is approximately 0.0 mm Hg.
16. The system of claim 1 wherein the predetermined pressure is between approximately -1.0 mm Hg and 1.0 mm Hg.
17. A method for delivering fluid to a wound therapy dressing, the method comprising:
 - creating a negative pressure on a wound therapy dressing;
 - delivering fluid to the wound therapy dressing;
 - monitoring pressure at the wound therapy dressing via a pressure sensor; and
 - restricting fluid delivery when the pressure reaches a predetermined value.
18. The method of claim 17 wherein restricting the fluid delivery comprises activating a control switch to cut off a supply of energy to a pump.
19. The method of claim 17 wherein restricting fluid delivery comprises closing a valve between a fluid flow device and the wound therapy dressing.

20. The method of claim 19 wherein the valve is a solenoid valve.
21. The method of claim 17 further comprising deactivating the negative pressure source prior to delivering fluid to the wound therapy dressing.
22. The method of claim 17 further comprising providing fluid flow to the wound therapy dressing via a gravity feed system.
23. The method of claim 21 further comprising:
 - providing reservoir between the negative pressure source and the wound therapy dressing;
 - providing a check valve between the negative pressure source and the wound therapy dressing, wherein the check valve is configured to restrict flow from the negative pressure source to the wound therapy dressing; and
 - venting the reservoir to atmosphere after de-activating the negative pressure source and prior to activating the pump to deliver fluid to the wound therapy dressing.
24. The method of claim 23 wherein the predetermined pressure is approximately 0.0 mm Hg.
25. The method of claim 23 wherein the predetermined pressure is between approximately -1.0 mm Hg and 1.0 mm Hg.

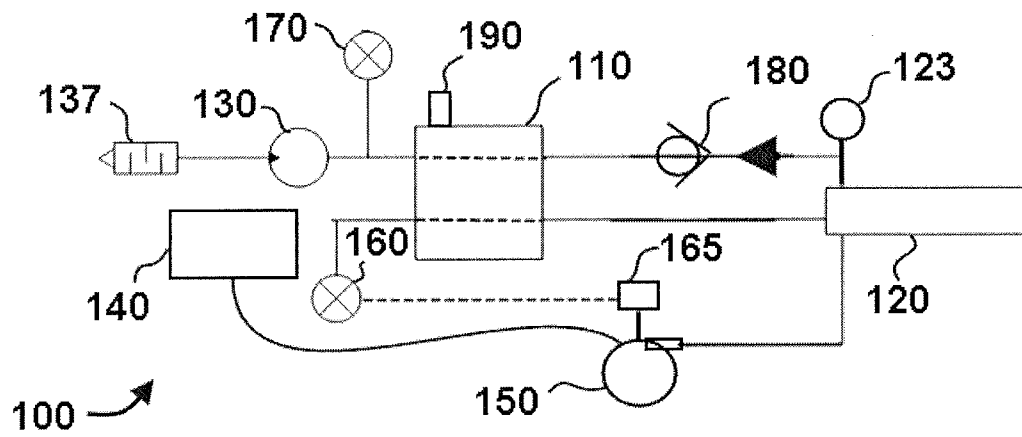


FIG. 1

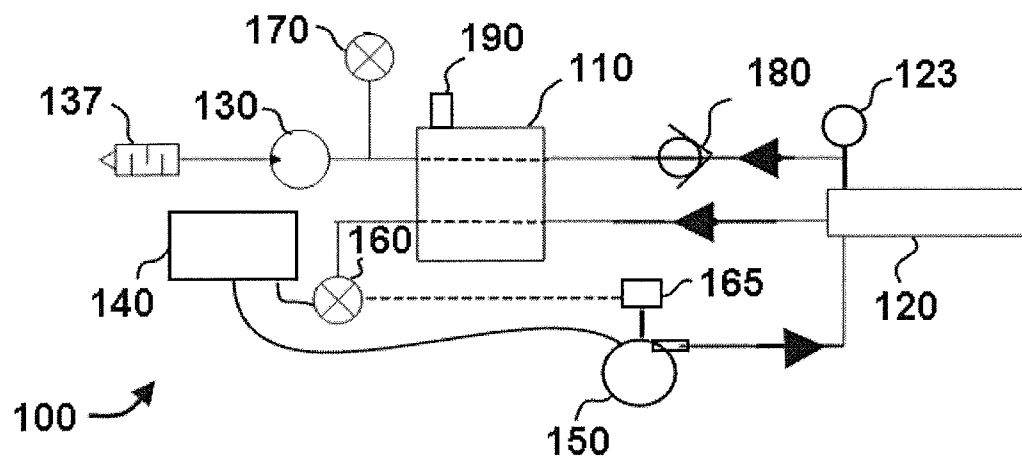
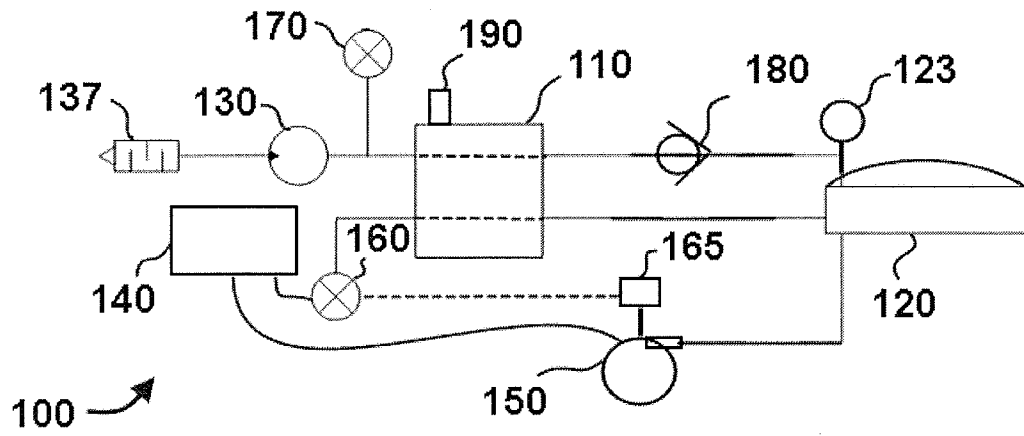


FIG. 2

**FIG. 3**

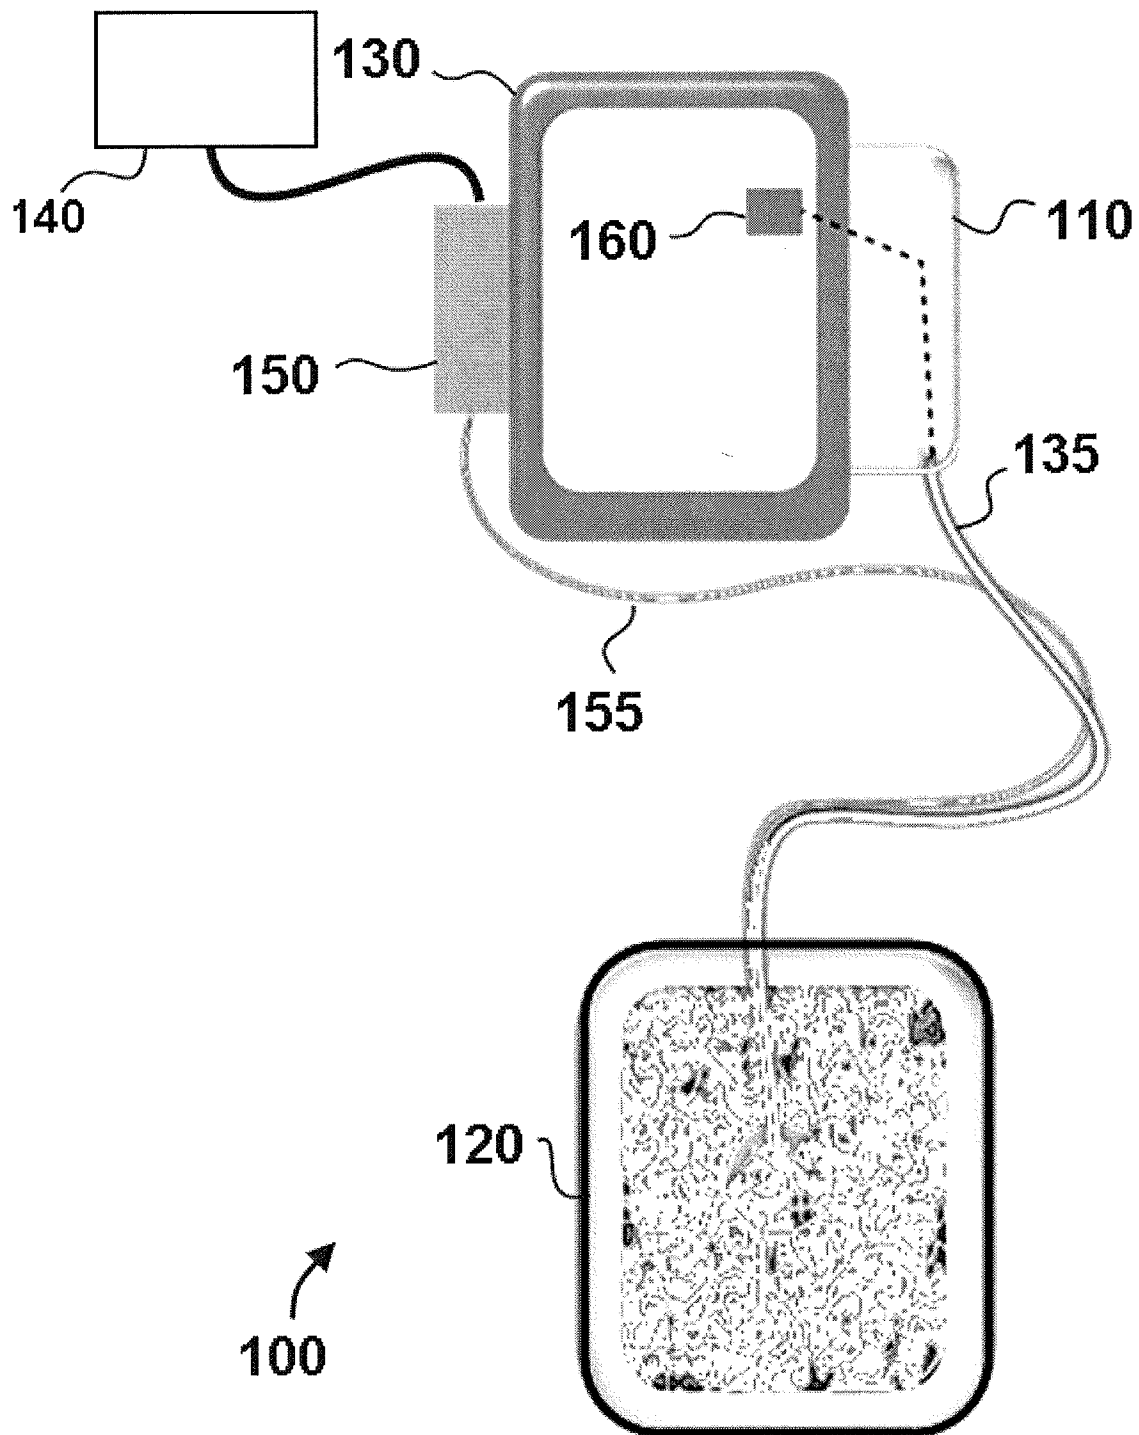


FIG. 4

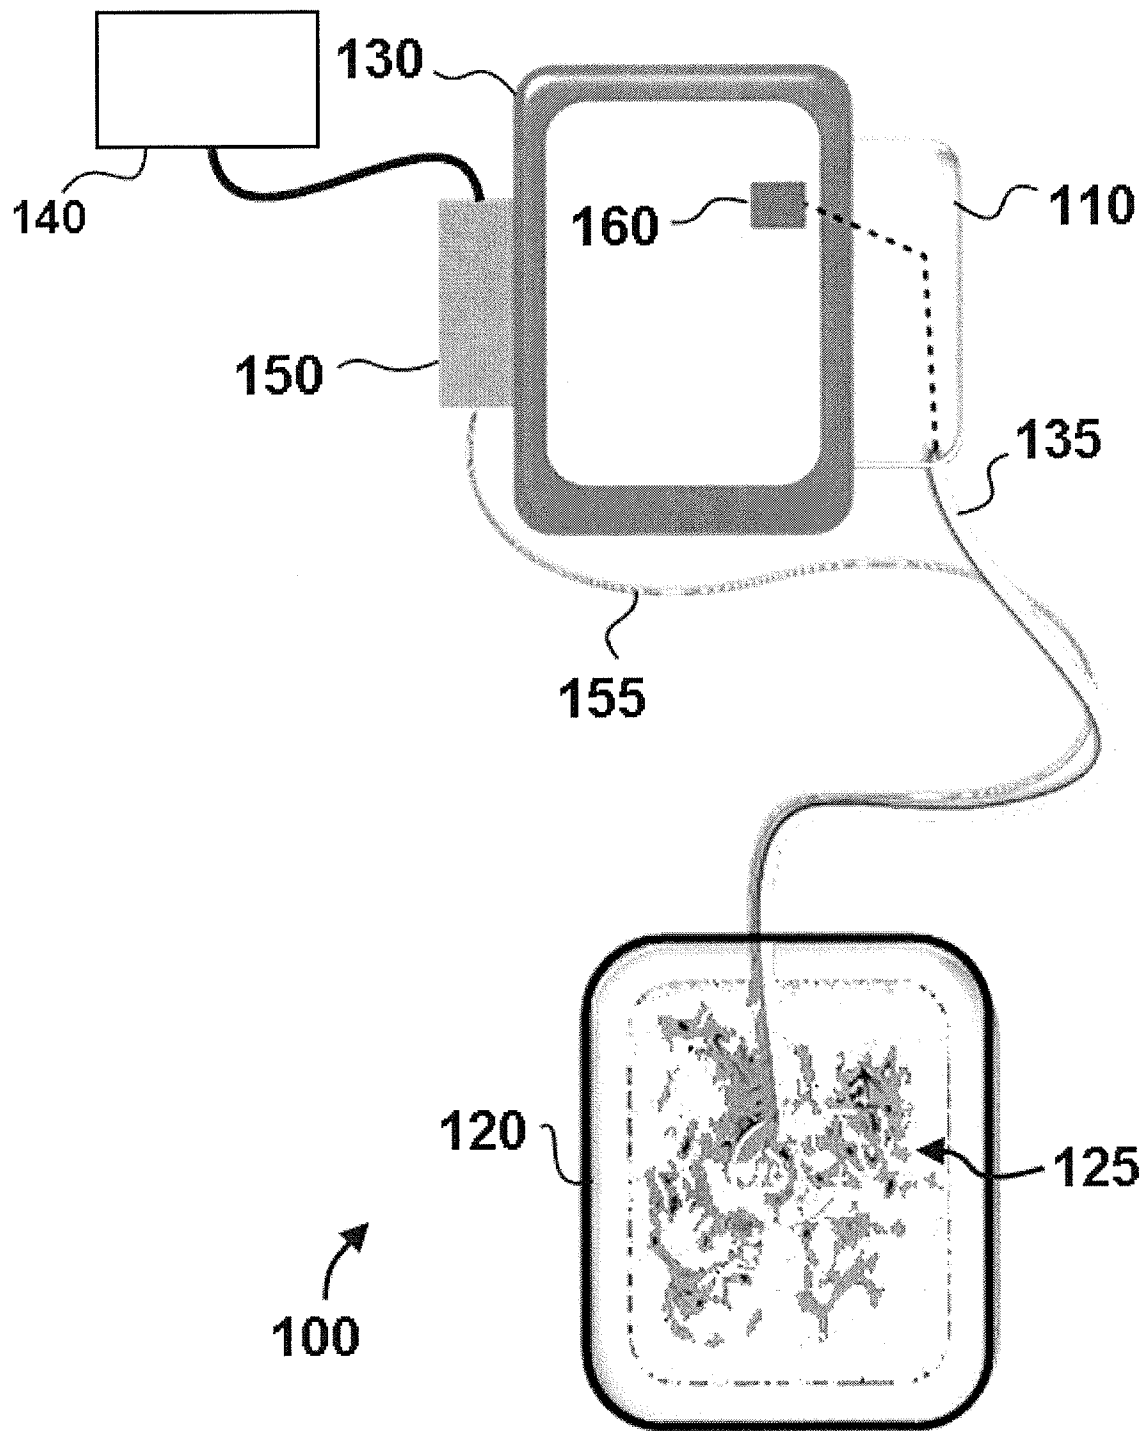


FIG. 5

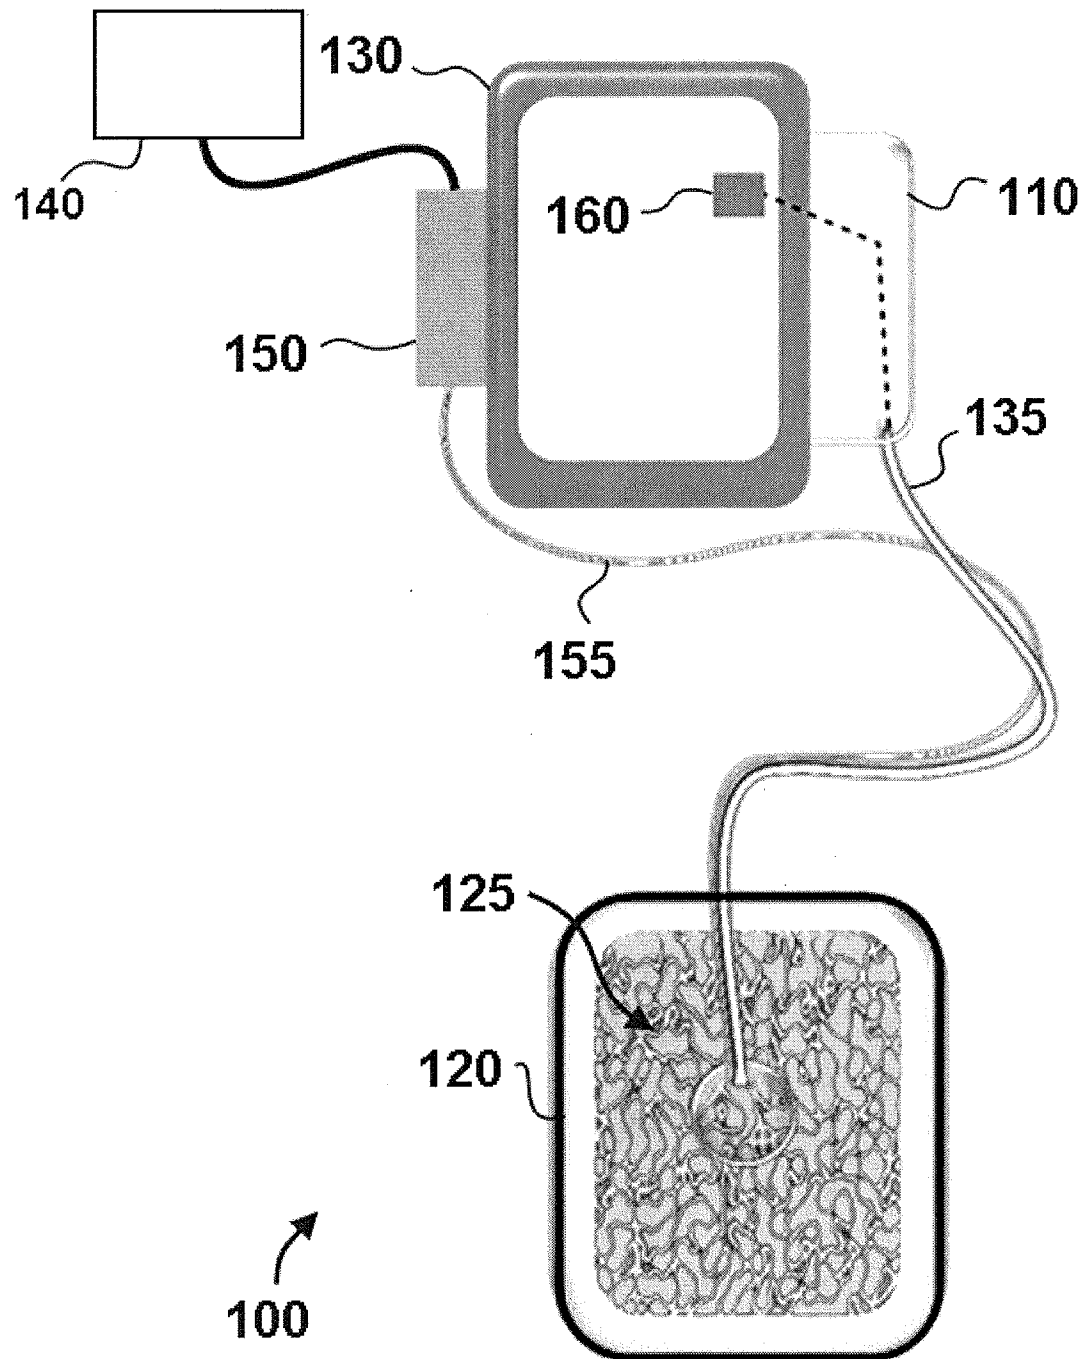
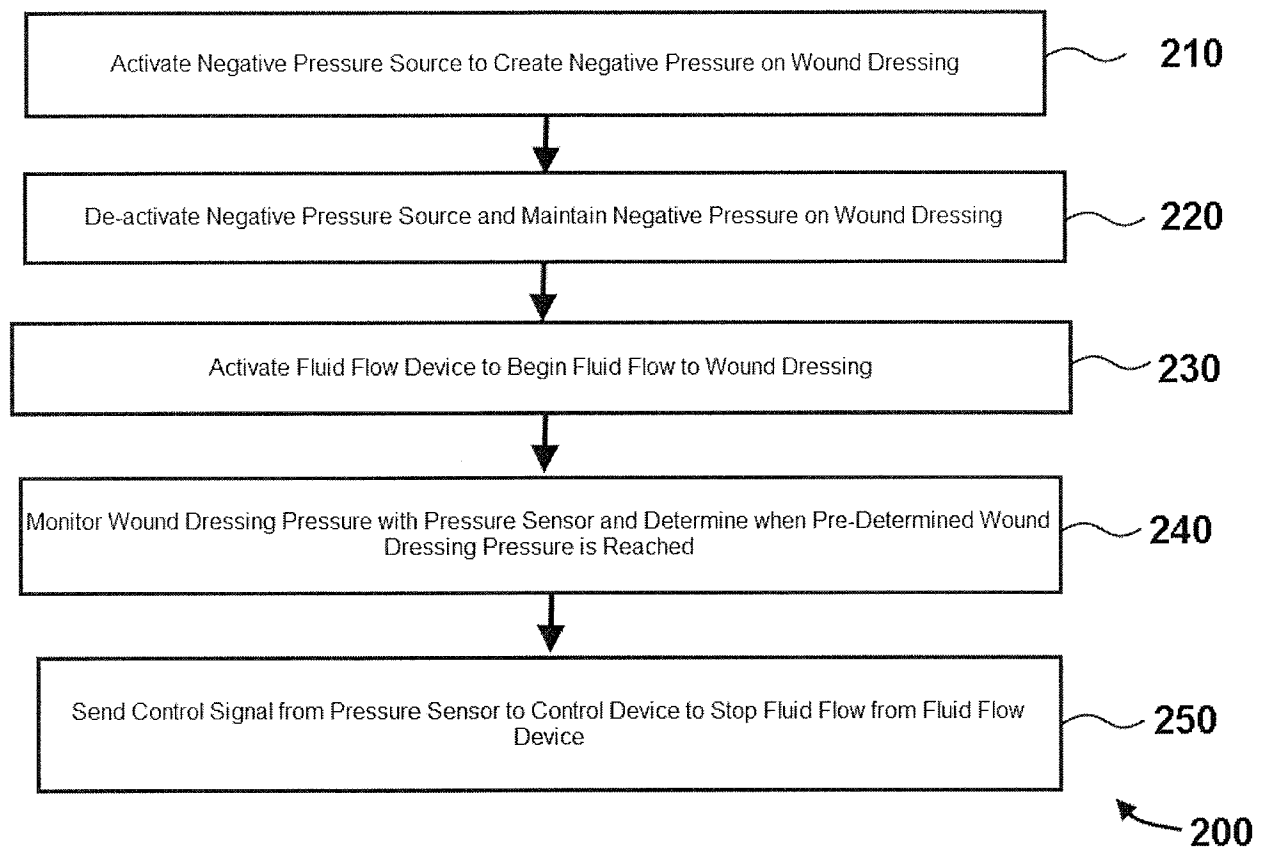


FIG. 6

**FIG. 7**

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2012/038945

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61M1/00
ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)
A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2007/118096 A1 (SMITH JOSHUA D [US] ET AL SMITH JOSHUA DAVID [US] ET AL) 24 May 2007 (2007-05-24) abstract; figures 1-5 paragraphs [0063], [0067] - [0070] -----	1-16
X	US 2009/275884 A1 (MCNULTY AMY [US] ET AL) 5 November 2009 (2009-11-05) abstract; figure 1 paragraphs [0058] - [0060] -----	1-16
X	US 2011/015587 A1 (TUMEY DAVID M [US] ET AL) 20 January 2011 (2011-01-20) abstract; figure 1 paragraphs [0039], [0042] - [0046] ----- -/-	1-16



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

18 July 2012

Date of mailing of the international search report

25/07/2012

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040,
Fax: (+31-70) 340-3016

Authorized officer

Kaden, Malte

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2012/038945

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 17-25
because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by therapy
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of Item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

International application No

PCT/US2012/038945

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 2008/130689 A1 (EILAT ERAN [IL]; DAGAN JACOB [IL]; TADIR YONA [IL]) 30 October 2008 (2008-10-30) abstract; figure 2 paragraphs [0038] - [0043] -----	1

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No

PCT/US2012/038945

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2007118096 A1	24-05-2007	EP 2010245 A1	07-01-2009
		US 2007118096 A1	24-05-2007
		US 2010121287 A1	13-05-2010
		WO 2007062024 A1	31-05-2007

US 2009275884 A1	05-11-2009	CA 2722671 A1	05-11-2009
		EP 2282759 A2	16-02-2011
		TW 200950824 A	16-12-2009
		US 2009275884 A1	05-11-2009
		WO 2009134967 A2	05-11-2009

US 2011015587 A1	20-01-2011	NONE	

WO 2008130689 A1	30-10-2008	NONE	
