



US 20060276974A1

(19) **United States**

(12) **Patent Application Publication**  
**Zeineh et al.**

(10) **Pub. No.: US 2006/0276974 A1**

(43) **Pub. Date: Dec. 7, 2006**

(54) **SYSTEM FOR REMOTE VIEWING AND  
DISPLAY OF A SLIDE**

**Publication Classification**

(75) Inventors: **Jack A. Zeineh**, Newport Beach, CA  
(US); **Usman Rashid**, Irvine, CA (US);  
**Rui-Tao Dong**, Mission Viejo, CA (US)

(51) **Int. Cl.**  
**G06F 19/00** (2006.01)  
**G06K 9/00** (2006.01)  
(52) **U.S. Cl.** ..... **702/19; 382/128**

Correspondence Address:  
**THE LAW OFFICE OF RICHARD W. JAMES**  
**25 CHURCHILL ROAD**  
**CHURCHILL, PA 15235 (US)**

(57) **ABSTRACT**

A method for creating a virtual slide is provided. A virtual slide is a digital representation of an area of interest of a microscope slide. One method is to use a motorized microscope that can move a specimen with respect to a microscope objective. With such a system, one can capture one or more images through a microscope objective, such that a region of interest is imaged. Each image is then joined together to form a composite or "virtual image." In one embodiment, after a virtual slide is created, a user may fully utilize the full capabilities of the remote microscope. Among these capabilities is a set of "optical objectives" and "virtual objectives." Optical objectives are images created by digitizing an image through a microscope objective in real time. Virtual objectives are digitally created magnifications created by utilizing the existing virtual slide data to digitally create a field of view.

(73) Assignee: **Trestle Acquisition Corp.**

(21) Appl. No.: **11/502,816**

(22) Filed: **Aug. 11, 2006**

**Related U.S. Application Data**

(62) Division of application No. 10/620,016, filed on Jul. 14, 2003.

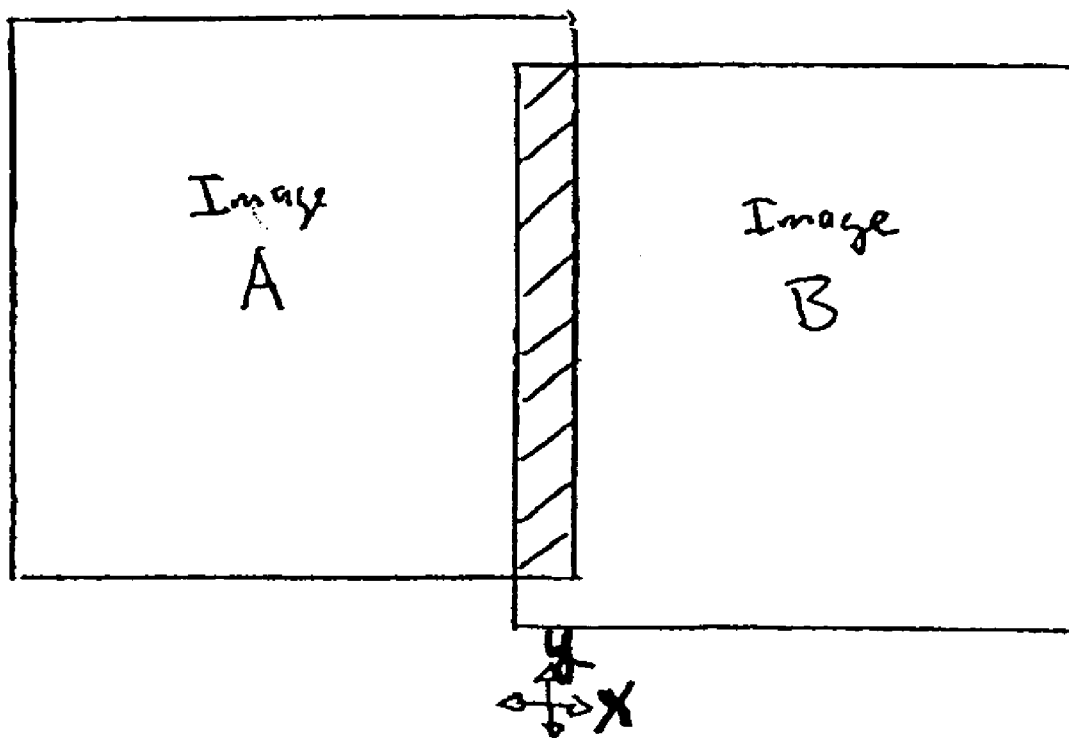


Figure 1

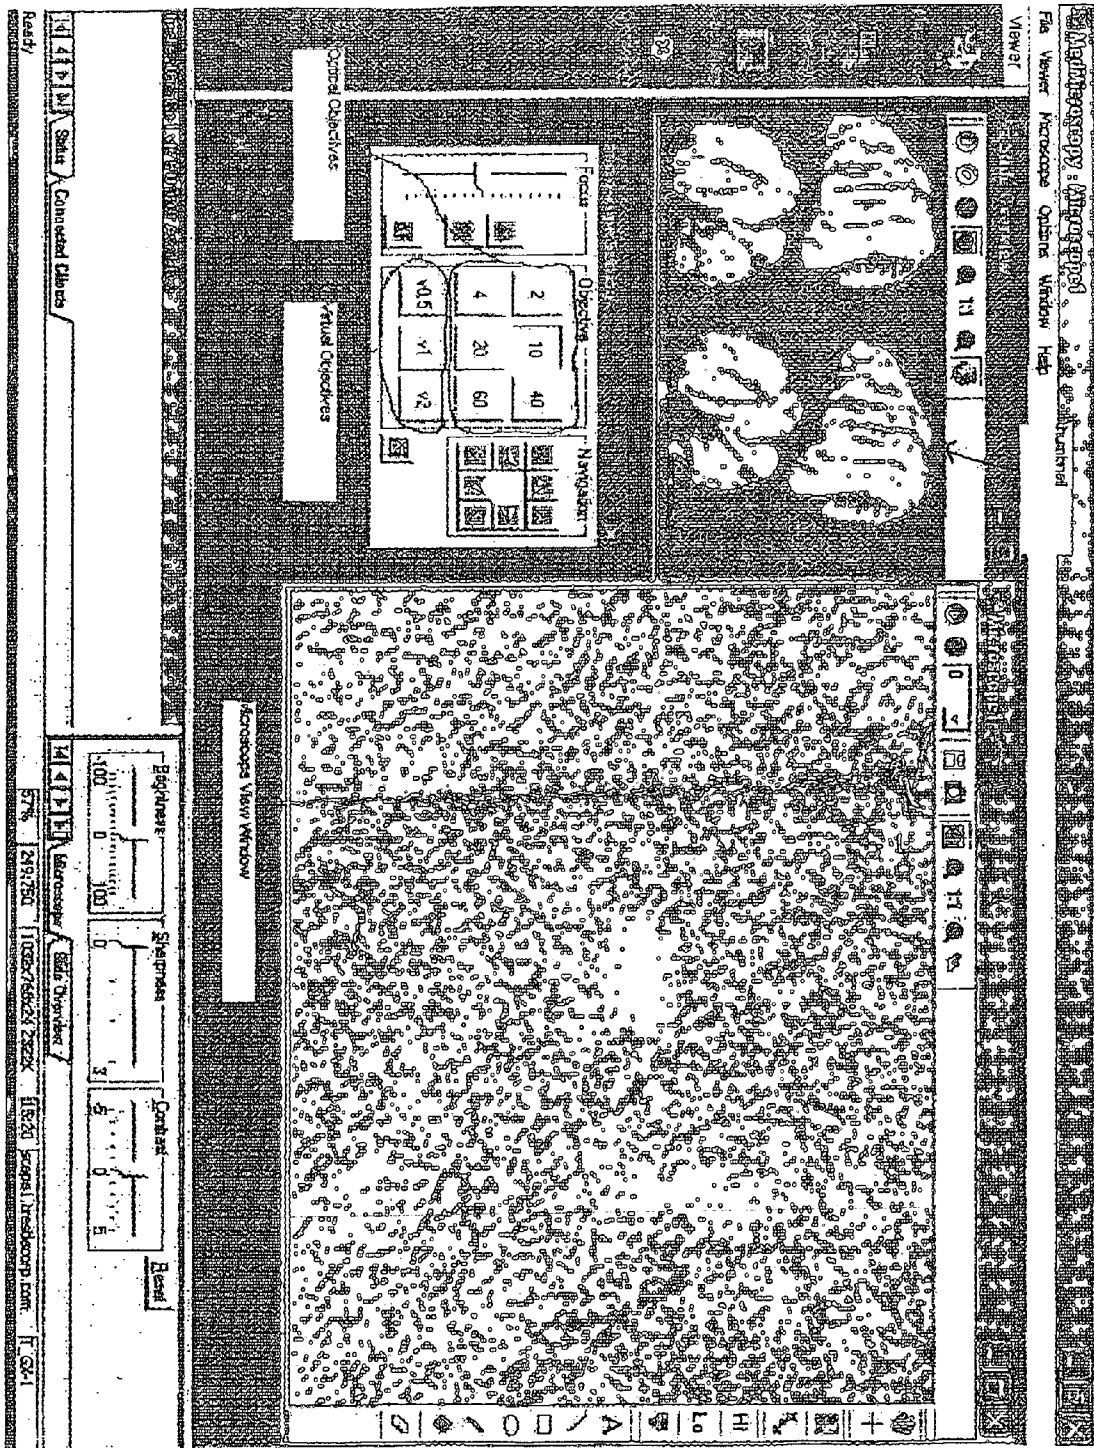


Figure 2

**SYSTEM FOR REMOTE VIEWING AND DISPLAY OF A SLIDE**

**CROSS REFERENCE TO RELATED APPLICATIONS**

[0001] This is a divisional application filed from application Ser. No. 10/620,016, filed Jul. 14, 2003, which claims benefit of U.S. Provisional Application No. 60/087,523, filed Jun. 1, 1998, U.S. application Ser. No. 09/323,371, filed Jun. 1, 1999, and U.S. application Ser. No. 10/488,913, filed May 30, 2003. U.S. patent application Ser. No. 10/620,016 is incorporated herein by reference.

**BACKGROUND OF THE INVENTION**

[0002] This invention relates to a method and apparatus for viewing remote microscope images.

[0003] Currently there is increasing demand for pathologist review of samples at remote locations. There exist multiple systems to address this need. They typically fall within one of two categories: live remote microscopy and virtual slide imaging.

[0004] In live remote control microscopy, a user receives images that are taken from a slide on a microscope. In virtual slide imaging, a user receives images previously captured. Virtual slide systems take one or more images of an area of interest and assemble them together (if there is more than one image) to form a virtual slide. Each of these techniques has its advantages. Live remote imaging provides users with the closest approximation to manual manipulation. Virtual slides allow faster image viewing, since images are already captured.

[0005] Virtual slide systems take one or more images and assemble them to form a "virtual slide."

[0006] However, users in the past were limited in their ability to integrate these technologies. One could only view and manipulate live and virtual images independently of one another. A user would have to clumsily go back and forth between these two modes of operation to separately look at the virtual slides and live microscope slides. We present a new method that integrates these ideas into one seamless operating environment.

**SUMMARY OF THE INVENTION**

[0007] In accordance with the present invention, a method and apparatus are provided for the analysis of remote slides in a hybrid live and virtual medium. Users obtain benefits of each technique in a unified environment.

**DETAILED DESCRIPTION OF THE PREFERRED EMBODIMENT**

[0008] A virtual slide is a digital representation of an area of interest of a microscopic slide. A virtual slide can be created multiple ways.

[0009] One method is to use a motorized microscope that can move a specimen with respect to a microscope objective (e.g., a microscope with a motorized stage). With such system, one can capture one or more images through a microscope objective, such that a region of interest (all or part of the microscopic slide) is imaged. Each image is then joined together to form a composite or "virtual image."

Multiple methods of joining images together are known in the art. One example is when images are simply abutted one next to another. However, this method does not generally produce virtual slides without seams, because errors such as camera rotation relative to the axis of motion are difficult to correct. Even with submicron accuracy stages it is, in practice, difficult to obtain consistent positioning. Another method is to utilize overlap between adjacent images to edge align images for maximum seamlessness. This can be done by sequentially shifting overlapping regions in the x and/or y axis, for example, by a stepping motor, and calculating a correlation value (or measure of goodness of overlap). The shift which results in the best correlation value is then used to join the images together (FIG. 1). While this method can be computationally expensive, it reduces reliance on difficult-to-attain mechanical positioning requirements and ultimately produces the best images in the sense of seamlessness.

[0010] In another method, the virtual slide is made simply by utilizing an imaging device with optics suitable to take an image of the area of interest on the slide in one snapshot. This method is embodied in the form of a conventional digital or analog camera with a macro lens.

[0011] This virtual slide can then be used to create a thumbnail view of the slide. To create the thumbnail view, the virtual slide is shrunk in resolution from its original, base resolution to a target resolution. If the target resolution is the same as the base resolution, then the image is unchanged. However, typically the resolution of the thumbnail desired is several times smaller than the base resolution.

[0012] With the virtual slide created, the user may fully utilize the full capabilities of the remote microscope. The user is presented with an image window and a set of control features (FIG. 2). Among these control features is a set of "optical objectives" and "virtual objectives."

[0013] Optical objectives are images that are created by a camera digitizing an image through a microscope objective (e.g., 10x, 20x, or 40x) in real time (i.e., an image is captured at the time the user requests the image). Virtual objectives are digitally created magnifications created not by digitizing in real time, but rather by utilizing the existing virtual slide data to digitally create a field of view.

[0014] When a user selects one of the optical objectives, a "change objective" command is sent to the microscope. This change objective command can also, specify additional qualifying information, such as microscope x, y, z positions, exposure setting, compression type and level, and image dimensions. If additional qualifying information is not sent, then the implicit qualifying information is the current state of the microscope or the last specified state. When the microscope receives the command, actions are taken to change the objective lens and to change the state of the microscope commensurate with the command (e.g., change the relative position of the objective lens relative to the microscopic slide, change exposure, etc.). An image is then digitized, compressed if so specified, and then transmitted to the user for display.

[0015] When a user selects a virtual objective, a virtual objective command is sent to the microscope. Similar to an optical objective command, this virtual objective command can also specify additional qualifying information, such as

microscope x, y, and/or z position. If additional qualifying information is not sent, then the implicit qualifying information is current microscope state or the last specified state. A region of interest is defined by the virtual request—it is the area on the microscope slide included in the field specified by the coordinates of the stage x, y and magnification of the command. This region of interest may optionally be trimmed such that image information already residing at the requesting user's view is not retransmitted to the user.

[0016] An image of the region of interest can be created from the virtual slide in multiple ways. If the virtual slide is not compressed, the retrieval of image information corresponding to the region of interest can be done by simply copying data from the virtual slide. If the virtual slide is compressed, a region corresponding to at least the region of interest can be decompressed to a raw bitmap from the main compressed image. If the virtual slide was stored as multiple compressed images rather than one large image, additional efficiencies are possible. For example, only those images that contain the desired region of interest need be accessed for decompression, rather than the entire area of the virtual slide. This enhances performance.

[0017] The decompression itself can also be performed in various ways. Strategies such as scaled decoding, as in the case of jpeg type compression, can be employed to improve the speed of the decompression by coupling a resolution reduction process with the decompression to speed up decompression when resolution reduction is required. Once the region of interest is decompressed, it can then be recompressed using a variety of strategies known to those skilled in the imaging field, which need not be the same as the method by which the virtual slide was compressed.

[0018] An alternative type of decompression/recompression step can also be used involving partial decompression. Partial decompression, such as decoding of Huffman-encoded data, as in the case of jpeg, can be performed to produce raw coefficients, rather than full decompression, which produces a raw bitmap. The raw coefficients corresponding to the area of the region of interest can then be selected. These coefficients which correspond to the region of interest are then re-encoded. In the case of jpeg compression, this would involve re Huffman encoding of the coefficients, rather than in normal full compression, where a dct must be performed followed by quantization and then Huffman coding.

[0019] Whichever the technique, the result is a compressed region of interest. The compressed region of interest is then transmitted to the user for viewing. The described method is more advantageous than sending the entire virtual slide, as one efficiently sends only that information required by the user.

[0020] However, direct transfer of the compressed image without decompression is feasible when the virtual slide is stored as multiple compressed images. The compressed images that include the area specified by the region of interest can be directly transferred to the user, rather than going through a decompression/recompression step. The disadvantage is that one may transfer more information than is needed if, for example, the compressed images are at a higher resolution than the requested resolution. This can be partially solved by creation of multiple resolution versions of the virtual slide. There are also compression strategies

available that allow only portions of the compressed images to be sent, such that a given resolution can be attained depending on which portions of the compressed image one chooses to send (e.g., progressive encoding). However, there is still the issue that the region of interest only partially covers the area of the compressed image. In this case, direct transfer of the image results in inefficiently sending data including both the region of interest and data outside the region of interest to the user.

[0021] With this invention, users are afforded a streamlined method of utilizing the features of virtual and live microscopy techniques.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0022] FIG. 1 is a drawing showing the overlap between adjacent images during optimization of overlap.

[0023] FIG. 2 is a photograph of a user's view of the remote microscope, showing a thumbnail view, microscope imaging window, and a set of microscope controls.

[0024] While the apparatus and methods of the present invention have been illustrated in terms of certain embodiments, the invention claimed herein is not limited to embodiments disclosed in this application. Rather, the scope of the invention is defined by the claims attached hereto.

[0025] While the invention has been illustrated and explained herein in terms of certain embodiments the invention is not limited to the specific embodiments disclosed. Rather, the invention is defined by the scope of the claims appended hereto.

[0026] A method for simultaneously viewing remote microscope images comprising virtual and live images and producing a seamless view of live and virtual images comprises: providing a virtual slide; providing a live microscope slide; and automatically and sequentially shifting overlapping regions of images from the slides to obtain the optimal image is disclosed.

What is claimed is:

1. A system for remote viewing of a slide, comprising:

a microscopy system comprising a microscope having a stage to receive the slide and a camera to couple with the microscope;

a single display to show an image of a portion of the slide and to show a plurality of control features, the plurality of control features comprising:

one or more first selections to command the microscopy system to capture a real time version of an other image of at least part of the slide and to transmit the captured image to the single display; and

one or more second selections to command a previously-captured version of the other image to be transmitted to the single display.

2. The system of claim 1, wherein the single display is further to show a thumbnail view of the slide.

3. The system of claim 2, wherein the thumbnail view of the slide comprises multiple images joined together.

4. The system of claim 1, wherein the one or more first selections are further to specify a microscope objective of the microscope through which the microscope system is to capture the real time version of the other image.

5. The system of claim 1, wherein the one or more second selections are further to specify a magnification of the previously-captured version of the other image to be transmitted.

6. The system of claim 1, wherein the one or more second selections are further to specify a region of interest of the slide, the region of interest to be shown by the previously-captured version of the other image.

7. The system of claim 6, wherein if the image of the portion of the slide to be shown on the display comprises part of the specified region of interest, then the previously-captured version of the other image to be transmitted to the single display is to not include the part of the specified region of interest.

8. The system of claim 1, wherein the plurality of control features further comprise one or more third selections to specify qualifying information for at least one of the real time version of the other image and the previously-captured version of the other image.

9. The system of claim 8, wherein the qualifying information comprises an x, y microscope position.

10. The system of claim 8, wherein the qualifying information comprises an x, y, z microscope position.

11. The system of claim 8, wherein the qualifying information comprises image dimensions.

12. The system of claim 8, wherein the qualifying information comprises an exposure setting.

13. The system of claim 8, wherein the qualifying information comprises a compression level.

14. The system of claim 8, wherein the qualifying information comprises a compression type.

15. A method for remote displaying of a slide, comprising: providing a single display showing an image of a portion of the slide and showing a plurality of control features; receiving, by receipt of a selection of one or more of the control features, a command to obtain an other image of at least part of the slide, the command specifying the other image as either previously-captured or for capture; and

in response to the command:

if the command specified the other image as previously-captured, retrieving a previously-captured of the other image and transmitting the previously-captured version to the single display; and

if the command specified the other image as for capture, capturing the other image and transmitting the captured other image to the single display.

16. The method of claim 15, wherein the single display further shows a thumbnail view of the slide.

17. The method of claim 15, wherein the command specifying the other image as for capture further specifies a

microscope objective, and wherein if the command specified the other image as for capture, the other image is captured through the microscope objective.

18. The method of claim 15, wherein the command specifying the other image as previously-captured further specifies a magnification of the other image, and wherein if the command specifies the other image as previously-captured, the previously-captured other image that is retrieved is at the specified magnification.

19. The method of claim 15, wherein the command further specifies the other image with qualifying information.

20. The method of claim 19, wherein the qualifying information comprises an x, y microscope position.

21. The method of claim 19, wherein the qualifying information comprises an x, y, z microscope position.

22. The method of claim 19, wherein the qualifying information comprises image dimensions.

23. The method of claim 19, wherein the qualifying information comprises an exposure setting.

24. The method of claim 19, wherein the qualifying information comprises a compression level.

25. The method of claim 19, wherein the qualifying information comprises a compression type.

26. A method for remote viewing of a slide, comprising: receiving an image of a portion of the slide and showing a plurality of control features and the image on a single display;

selecting certain of the image control features and thereby requesting an other image specified as either previously-captured or for capture, the other image of at least part of the slide; and

receiving the specified other image and showing the other image on the single display.

27. The method of claim 26, wherein the single display further shows a thumbnail view of the slide.

28. The method of claim 26, wherein the request further specifies the other image with qualifying information.

29. The method of claim 28, wherein the qualifying information comprises an x, y microscope position.

30. The method of claim 28, wherein the qualifying information comprises an x, y, z microscope position.

31. The method of claim 28, wherein the qualifying information comprises image dimensions.

32. The method of claim 28, wherein the qualifying information comprises an exposure setting.

33. The method of claim 28, wherein the qualifying information comprises a compression level.

34. The method of claim 28, wherein the qualifying information comprises a compression type.

\* \* \* \* \*