

(19) World Intellectual Property Organization
International Bureau




(43) International Publication Date
12 July 2001 (12.07.2001)

PCT

(10) International Publication Number
WO 01/50816 A1

- (51) International Patent Classification⁷: **H04R 25/00** (74) Agents: KAVOUNAS, Gregory, T. et al.; Marger Johnson & McCollom, P.C., 1030 S.W. Morrison Street, Portland, OR 97205 (US).
- (21) International Application Number: PCT/US00/35400
- (22) International Filing Date: 22 December 2000 (22.12.2000) (81) Designated States (*national*): JP, US.
- (25) Filing Language: English (84) Designated States (*regional*): European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR).
- (26) Publication Language: English
- (30) Priority Data: 09/478,136 5 January 2000 (05.01.2000) US
- (71) Applicant and (72) Inventor: HOUSE, David, William [US/US]; P.O. Box 330, Aurora, OR 97002 (US).
- Published:
— With international search report.
— Before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments.
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

(54) Title: COCHLEAR IMPLANTS WITH A STIMULUS IN THE HUMAN ULTRASONIC RANGE AND METHOD FOR STIMULATING A COCHLEA

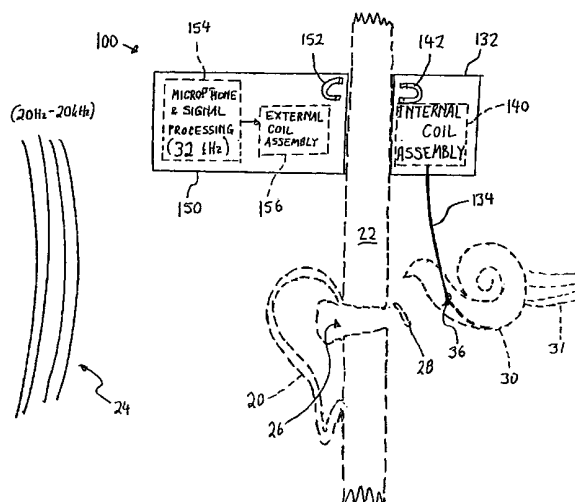

(57) Abstract: A cochlear implant system (100) for a patient's cochlea (30) includes an external unit (150) and an implanted internal unit (132). The internal unit (132) includes one electrode (134) for inserting in the patient's cochlea (30), and an internal coil assembly (140) for driving the electrode (134). The external unit (150) includes an oscillator for generating an electrical analog carrier signal, and an external coil to couple magnetically the modulated signal to the internal coil. The analog carrier signal has a frequency in the ultrasonic human range, i.e. greater than 20 kHz, such as 32 kHz or 80 kHz. In one embodiment, this can be heard as an alarm. In another embodiment, the external unit (150) also includes a microphone for outputting electrical sound signals in response to ambient or other sounds (24), and a modulator for modulating the carrier signal with the electrical sound signals to generate a modulated signal.

**COCHLEAR IMPLANTS WITH A STIMULUS IN THE HUMAN
ULTRASONIC RANGE
AND METHOD FOR STIMULATING A COCHLEA**

5

1. Technical field of the invention

The present invention is related to the field of hearing aids, and more specifically to the field of permanent cochlear implants for the hearing impaired.

10 **2. Description of the background art**

Hearing aids are often designed to amplify sound. These do not work, however, for patients with severe deafness because they cannot hear any sound, no matter how loud. For such patients, an implant technology is used, which stimulates directly the cochlea of the human ear.

15 The implant technology is now described in more detail with reference to FIG. 1. A human pinna (outer portion of the ear) 20 is supported on tissue 22 of the patient's head. When a sound 24 in the audible range of 20 Hz to 20,000 Hz reaches the pinna 20, the sound 24 reaches the eardrum 28 through an opening 26 in the tissue 22, known as the ear canal 26. In a healthy person, the eardrum 28 in turn excites the cochlea 30 mechanically, through
20 additional structures (bones of hearing; not shown). The cochlea 30 accordingly stimulates the hearing nerve 31. In a severely deaf person, however, the cochlea 30 does not produce nerve stimulations, and thus the hearing nerve 31 transmits nothing to the brain.

A cochlear implant has two main parts, an internal unit 32 and an external unit 50. The internal unit 32 is surgically implanted near the pinna 20 of the patient. The internal unit
25 32 has at least one electrode 34 that is coupled with the cochlea 30. The internal unit 32 includes an internal coil assembly 40 for electrically driving the electrode 34. The internal unit 32 also includes a magnet 42.

The external unit 50 also includes a magnet 52, for suspending the external unit 50 from the field of the magnet 42. The external unit 50 also includes a microphone and signal
30 processing component 54, and an external coil assembly 56. When the sound 24 reaches the microphone and signal processing component 54, the component 54 generates a signal which drives the external coil assembly 56. The signal is then inductively coupled ("injected") into the internal coil assembly 40.

Referring to FIG. 2, component 54 includes an oscillator 57, which generates a carrier
35 analog signal. A volume control unit 58 is preferably implemented by an adjustable gain

amplifier that amplifies the analog carrier signal. Adjusting the volume control unit 58 determines how much overall sound sensation, also known as percept, will reach the patient. In an older implementation of this cochlear implant, the amplified analog carrier signal is input into an amplitude modulator 60, to be amplitude modulated by the received sounds.

5 Component 54 also includes a microphone 62 with its associated circuitry, a preamplifier 64, and a band pass filter 66. The band pass filter 66 allows to pass only those frequencies of the preamplified electrical signal that correspond to sound in the range of 200 Hz - 4000 Hz. The band pass filter 66 discards the signal corresponding to sound 24 that corresponds to the rest of the frequencies, that is, anything outside the frequency range of the
10 band pass filter 66.

 The filtered signal from band pass filter (BPF) 66 is input in a modulation control unit 68. The modulation control unit 68 thus uses the filtered signal to modulate the pre-amplified analog carrier signal in modulator 60. The modulator 60 outputs the modulated signal to an output amplifier 70. Thus amplified, the modulated signal is input into external coil assembly
15 56 of FIG. 1.

 As described immediately above, the prior art limits how much sound percept can be delivered to the patient. This is now explained in more detail.

 Referring also to FIG. 3, the interrelationship of the chosen frequencies is placed in perspective. A healthy ear can hear sounds between 20 Hz and 20 kHz (thus these are called
20 the sonic, or hearable frequencies), which is denoted as a sonic range 78. The frequencies important to the understanding of speech belong within a speech range 80, reaching up to a frequency of 8 kHz. The carrier analog signal is denoted in FIG. 3 as an arrow 76, and is at a frequency of 16 kHz, which is within the sonic range 78.

 Experiments using the above system showed that sound frequencies higher than 4,000
25 Hz sounded unclear to the user. Accordingly, the prior art included the band pass filter 66 (seen in FIG. 2), which has a BPF range 86 (seen in FIG. 3).

 The result is that the prior art system only works for sounds within the BPF range 86 of the band pass filter 66. The prior art has rationalized this by concluding that the important portion of the sensitivity range of the human ear 78 is the portion where the speech range 80
30 belongs, and that further, the most important portion of the speech range 80 is found at 4,000 Hz and below.

 Patients desire to be able to hear speech at the frequency higher than 4,000 Hz, and other sounds at frequencies higher than 8,000 Hz, just like healthy people.

DISCLOSURE OF THE INVENTION

The present invention improves on the limitations of the prior art.

Generally, the present invention provides a cochlear implant system, and a method for stimulating a cochlea. The system includes an internal unit and an external unit. The internal unit includes at least one electrode for coupling with the patient's cochlea, and an internal (implanted) coil to inductively drive the electrode. The external unit includes an oscillator for generating an electrical analog carrier signal, which is coupled to the coil, and thus also to the electrode. The analog carrier signal has a frequency in the ultrasonic human range, i.e. greater than 20,000 Hz, such as 32,000 Hz or 80,000 Hz, and can serve at least as an alarm.

In one embodiment of the invention, the external unit also includes a microphone for producing electrical signals in response to external sounds, and a modulator for modulating the carrier signal with the sound signals to generate a modulated signal prior to coupling it to the internal coil.

This higher frequency results in clearer rendering of sounds, and a higher frequency range of rendered sounds.

The foregoing and other objects, features and advantages of the invention will become more readily apparent from the following detailed description of a preferred embodiment, which proceeds with reference to the drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a partial section view of a patient using a prior implant technology.

FIG. 2 is a block diagram of a microphone and signal processing component 54 of an external unit 50 of the prior implant technology of FIG. 1.

FIG. 3 is a graph showing the relative frequency ranges of the sensitivity of the human ear, speech, and a carrier frequency of an oscillator and a band pass filter in FIG. 2.

FIG. 4 is a partial section view of the patient using a cochlear implant system made according to an embodiment of the present invention.

FIG. 5 is a block diagram for a circuit of a driver for a cochlear implant system made according to an embodiment of the present invention.

FIG. 6 is diagram showing the frequency of a carrier according to an embodiment of the present invention relative to the ranges of the sensitivity of the human ear and of speech.

FIG. 7 is the flowchart for illustrating a method according to an embodiment of the present invention.

FIG. 8 is a partial section view of the patient using a cochlear implant system made according to another embodiment of the present invention.

FIG. 9 is a block diagram for a circuit of a driver for a cochlear implant system made according to an embodiment of the present invention.

5 FIG. 10 is the flowchart for illustrating a method according to an embodiment of the present invention.

BEST MODE OF CARRYING OUT THE INVENTION

As has been mentioned, the present invention provides a cochlear implant system, a
10 driver for cochlear implant system, and a method for stimulating a cochlea.

A cochlear implant system 100 according to a first embodiment of the invention is now described in detail with reference to FIGs. 4-7. The cochlear implant system 100 includes an internal unit 132 that is surgically implanted near the pinna 20 of the patient, and preferably close to the skin 22. The internal unit 132 has at least one active electrode 134
15 that is inserted into the cochlea 30 through hole 36. In addition, a second electrode (not shown) is optionally implanted in other nearby tissue, and used to provide a reference voltage to the active electrode 134.

The internal unit 132 includes an internal coil assembly 140 for electrically driving the electrode 134. In the preferred embodiment, the internal coil assembly 140 has two ends,
20 one coupled to the active electrode 134, and the other coupled with the reference electrode (not shown). An advantage of the implant technology is that the internal coil assembly 140 can be driven externally. As such, there is no need for a battery, which would require changing after sometime. This permits implanting permanently the internal unit 132, with its sensitive contact of the cochlea 30.

25 The internal unit 132 also includes a magnet 142, which can be a simple magnet, or a more sophisticated magnet arrangement. The magnet 142 is so oriented that its strongest field is located outside the head, in a preferential direction (e.g., north vs. south vertically).

The cochlear implant system 100 of the invention further includes a driver 150, which is also known as an external unit 150. The driver 150 is for driving the implanted internal
30 coil assembly 140, and therefore driving the electrode 134. The actual size of driver 150 can be as small in diameter as a U.S.A. penny (about 1.9 cm), or even smaller. In FIG. 4, the external unit 150 is shown larger only for clarity.

In another embodiment, the invention provides only the driver 150, which would be used for patients who have already been implanted with cochlear implant systems using the prior art, which will thus perform better.

The external unit 150 is suspended in a spatial relation to the internal unit 132 by any means known in the art. Preferably, the external unit 150 includes a magnet 152 that interacts with the field of the magnet 142. The magnets 152 and 142 are thus used to suspend the external unit 150 on the tissue 22 of the patient, without any further support. Preferably, the magnets are arranged such that their polarities permit the driver 150 to be attached to a single, well-defined place on the tissue 22. If, however, the external unit 150 is suspended in a different way, then there is no need for either the internal unit 132 to have a magnet 142, or for the driver to have a magnet 152.

The external unit 150 includes a microphone and signal processing component 154, and an external coil assembly 156. The external unit 150 preferably includes a battery (not shown), which can be replaced as needed. When the sound 24 reaches the microphone and signal processing component 154, the component 154 generates a signal for driving the external coil assembly 156. The generated signal is an analog signal that is also known as electrical sound signal. The generated signal is thus coupled into the internal coil assembly 140. In other words, the external coil assembly 156 forms a transformer with the internal coil assembly 140, and inductively drives it.

Referring to FIG. 5, the microphone and signal processing component 154 is described in detail. In one embodiment, component 154 includes an oscillator 157, which generates a carrier analog signal. The analog signal is continuous, and preferably sinusoidal. This is not limiting, however. The carrier analog signal of the invention can be triangular shaped, sawtooth shaped, etc. Such other shapes introduce additional, secondary carrier frequencies.

Importantly for the present invention, the carrier analog signal from oscillator 157 has a frequency greater than 20 kHz, i.e. it is outside the range of normal human hearing. One good operating value is 32 kHz. Higher values, such as 80kHz, also work very well. The significance of this choice will be appreciated in view of the description pertaining to FIG. 6, later in this document.

Continuing to refer to FIG. 5, a volume control unit 158 is preferably implemented by an adjustable gain amplifier that amplifies the analog carrier signal. Adjusting the volume control unit 158 determines how much total sound percept will reach the patient. The

amplified analog carrier signal is input into a modulator 160, to be amplitude modulated by the received sounds.

In one embodiment of the invention, modulator 160 is an amplitude modulator. In another embodiment of invention, modulator 160 is a frequency modulator. Stimulation by means of analog signals in the ultrasonic range can also be done directly, or in other ways, to provide the patient with a percept of sound.

Component 154 also includes a microphone 162 with its associated circuitry, and an optional preamplifier 164. The microphone 162 outputs an electrical signal responsive to the sounds 24 it receives. The preamplifier 164 amplifies the electrical signal of the microphone 162.

It should be noted that there is no need for a band pass filter, such as band pass filter 66 of FIG. 2. Even if one is included, its upper limit can be much higher than that of the prior art, thus permitting a wider range of frequencies to be presented or perceived.

The signal from the preamplifier 164 is input in a modulation control unit 168. The modulation control unit 168 thus uses the signal to modulate the preamplified analog carrier signal in modulator 160. The modulator 160 outputs the modulated signal to an output amplifier 170. Thus amplified, the modulated signal is input into the external coil assembly 156 of FIG. 4.

The superiority of the present invention is now explained by first analyzing further the weakness of the prior art system, as explained in FIG. 3. All the prior art globally adopted the carrier 76 to be at 16 kHz, within the sensitivity of human ear range 78. The prior art references universally treat the value of 16 kHz as an undisputed optimum.

The choice of the frequency of the carrier 76 imposes an upper limit as to the frequency that can be transmitted clearly. This results from the Nyquist limit. In other words, the carrier 76 samples the speech at its own frequency of 16 kHz. The higher the frequency of the sampled sound, the less clearly it will be rendered. For a frequency of 16 kHz, the Nyquist limit turns out to be 1/4 of that, in other words 4 kHz. Indeed, the users of the prior art system of FIG. 1 found sounds having a frequency of higher than 4 kHz confusing.

Referring now to FIG. 6, the invention proposes that there is no reason for the carrier 174 produced by the oscillator 157 to be within the sound sensitivity frequency range of the human ear, or in the sonic range 78. As such, the carrier 174 is chosen to have a frequency of greater than 20 kHz. As can be seen from observing the ordinary human range 78, these frequencies for the carrier 174 belong in the human ultrasonic range.

It will be appreciated how the Nyquist limit permits a much higher range for the system of the present invention. In the embodiment of FIG.s 4, 5 and 6, the carrier frequency is 32 kHz, with a Nyquist limit of 8 kHz. This includes the entire range of speech 80, without limiting it, as the prior art did. It will now also be clear that, to match the sensitivity of the healthy human ear, the system of the invention should have a carrier frequency of (4 x 20 kHz) 80 kHz.

There is no need to stop there, either. A higher carrier frequency will permit the user to hear frequencies higher than any human has ever heard before. This can be extended to people who have no hearing deficit in the first place.

Other technical details for implementing the invention can be gleaned from the following publications:

- U.S. Patent Re. 32,947;
- Design and Function: A Physical and Electrical Description of the 3M House Cochlear Implant System, Fretz & Fravel, Ear and Hearing, Vol. 6, No. 3 Supplement, pp. 14S - 19S, 1985; and
- U.S.A. Patent Application Serial Number 09/478,136, filed January 5, 2000.

Referring to FIG. 7, a method according to the first embodiment of the invention is now described for stimulating the cochlea in response to sound.

According to box 210, an electrical signal, also known as an electrical sound signal, is generated in response to the sound. This can be accomplished with a microphone, and associated circuitry.

According to box 220, an electrical analog carrier signal is generated having a frequency of greater than 20 kHz. This can be accomplished with an oscillator. The frequency can be 21 kHz, 32 kHz, 80 kHz, or whatever frequency is deemed suitable for the desired application.

According to box 230, the carrier signal is modulated with the sound signal to generate a modulated signal. Modulating can be by amplitude modulation or frequency modulation.

According to box 240, the modulated signal is applied to an electrode that is coupled with the cochlea.

A cochlear implant system 800 according to a second embodiment of the invention is now described in detail with reference to FIGs. 8-10. It will be recognized that many of the

components are similar to those of the first embodiment, which makes a further description unnecessary.

The cochlear implant system 800 includes an internal unit 132 similar to what was described with reference to FIG. 4.

5 The cochlear implant system 800 of the invention further includes a driver 850, which is also known as an external unit 850. The driver 850 is for driving the implanted internal coil assembly 140, of internal unit 132, and therefore driving the electrode 134.

10 In another embodiment, the invention provides only the driver 850, which would be used for patients who have already been implanted with cochlear implant systems using the prior art, which will thus perform better.

The external unit 850 is suspended in a spatial relation to the internal unit 132 by any means known in the art. Preferably, the external unit 850 includes a magnet 152 that works as per the above.

15 The external unit 850 includes a signal generator 852, and an external coil assembly 156. The external unit 850 preferably also includes a battery (not shown), which can be replaced as needed. The signal generator 854 generates a signal for driving the external coil assembly 156. The generated signal is an analog signal that is also known as electrical sound signal. The generated signal is thus coupled into the internal coil assembly 140.

20 Referring to FIG. 9, the signal generator 852 is described in detail. In one embodiment, the signal generator 852 includes an oscillator 857, which generates a carrier analog signal. Oscillator 857 can be made in the same way as oscillator 157.

The analog signal is continuous, and preferably sinusoidal. This is not limiting, however. The carrier analog signal of the invention can be triangular shaped, sawtooth shaped, etc. Such other shapes introduce additional, secondary carrier frequencies.

25 Importantly for the present invention, the carrier analog signal from oscillator 857 has a frequency greater than 20 kHz, i.e. it is outside the range of normal human hearing. One good operating value is 32 kHz. Higher values, such as 80kHz, also work very well. The advantage of this choice was explained above.

30 Continuing to refer to FIG. 9, a volume control unit 158 is preferably implemented as per the above, receiving the carrier analog signal from oscillator 857. The carrier analog signal is then input in an output amplifier 170, made as per the above.

It will be understood that the second embodiment does not transform an external sound into percept. Yet it provides a percept. The invention is based in part on the unexpected result that a percept is received even at these frequencies that are supersonic (also

known as ultrasonic), when considered as sound waves. The invention therefore provides a device and a method for bypassing the ear, which attenuates any sound frequencies above the supersonic range.

The percept provided by the second embodiment can be an alarm, or a coded
5 sequence of sound, that can be activated under a certain desired condition. A person skilled in the art will discern ways of activating signal generator 852, by implementing suitable sensors etc. (not shown) in conjunction with external unit 850.

Referring to FIG. 10, a method according to the second embodiment of the invention is now described for stimulating the cochlea.

10 According to box 920, an electrical analog carrier signal is generated having a frequency of greater than 20 kHz. This can be accomplished with an oscillator. The frequency can be 21 kHz, 32 kHz, 80 kHz, or whatever frequency is deemed suitable for the desired application. This can take place in response to an outside condition.

15 According to box 940, the modulated signal is applied to an electrode that is coupled with the cochlea.

In this description numerous details have been set forth in order to provide a more thorough understanding of the invention. A person skilled in the art will be able to practice the present invention in view of the present description and the incorporated references. In other instances, well-known features have not been described in detail in order not to obscure
20 unnecessarily the invention.

The inventor regards the subject matter of the invention to include all combinations and sub-combinations of the various elements, features, functions and/or properties disclosed herein. While the invention has been disclosed in its preferred form, the specific
25 embodiments thereof as disclosed and illustrated herein are not to be considered in a limiting sense. Indeed, it should be readily apparent to those skilled in the art in view of the present description that the invention can be modified in numerous ways.

The following claims define certain combinations and sub-combinations of these elements, which are regarded as novel and non-obvious. Additional claims for other combinations and sub-combinations of features, functions, elements and/or properties may be
30 presented in this or in a related document.

CLAIMS

The invention claimed is:

- 1 1. A cochlear implant system for a patient's cochlea comprising:
2 at least one electrode for coupling with the patient's cochlea;
3 an internal coil for implanting in the patient to drive the electrode;
4 an oscillator for generating an electrical analog carrier signal; and
5 an external coil for magnetically coupling the generated electrical analog carrier
6 signal to the internal coil,
7 wherein the improvement comprises in that the electrical analog carrier signal has a
8 frequency greater than 20 kHz.
- 1 2. The system of claim 1, wherein the electrical analog carrier signal has a
2 frequency of at least 32 kHz.
- 1 3. The system of claim 1, further comprising:
2 a microphone for outputting electrical sound signals in response to external sounds;
3 and
4 a modulator for modulating the carrier signal with the electrical sound signals prior to
5 coupling it to the internal coil.
- 1 4. The system of claim 3, wherein the modulator is an amplitude modulator.
- 1 5. The system of claim 3, wherein the modulator is a frequency modulator.
- 1 6. A method for stimulating a human cochlea, comprising:
2 generating an electrical analog carrier signal; and
3 applying the generated electrical analog carrier signal to an electrode that is coupled
4 with the cochlea,
5 wherein the improvement comprises that the electrical analog carrier signal has a
6 frequency greater than 20 kHz.

1 7. The method of claim 6, wherein the electrical analog carrier signal has a
2 frequency of at least 32 kHz.

1 8. The method of claim 6, further comprising:
2 generating an electrical sound signal in response to a sound; and
3 modulating the carrier signal with the electrical sound signal prior to applying it to the
4 electrode.

1 9. The method of claim 8, wherein modulating is by amplitude modulation.

1 10. The method of claim 8, wherein modulating is by frequency modulation.

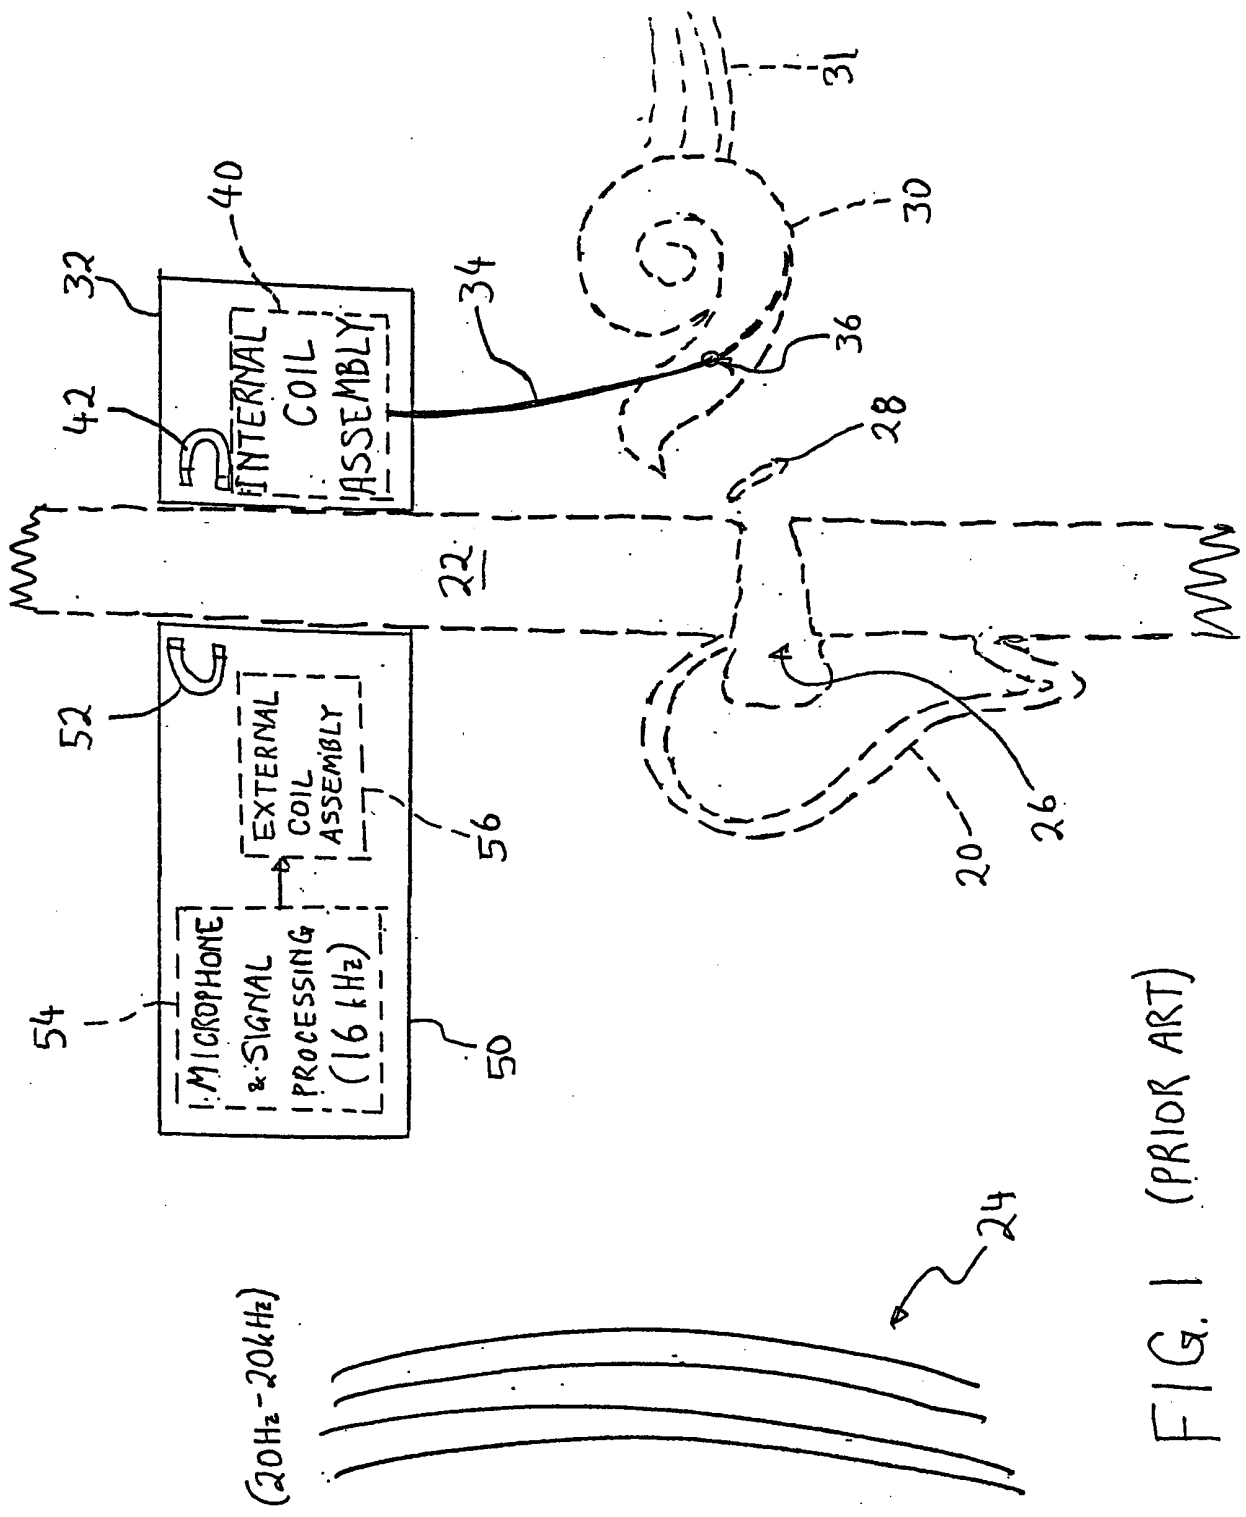


FIG. 1 (PRIOR ART)

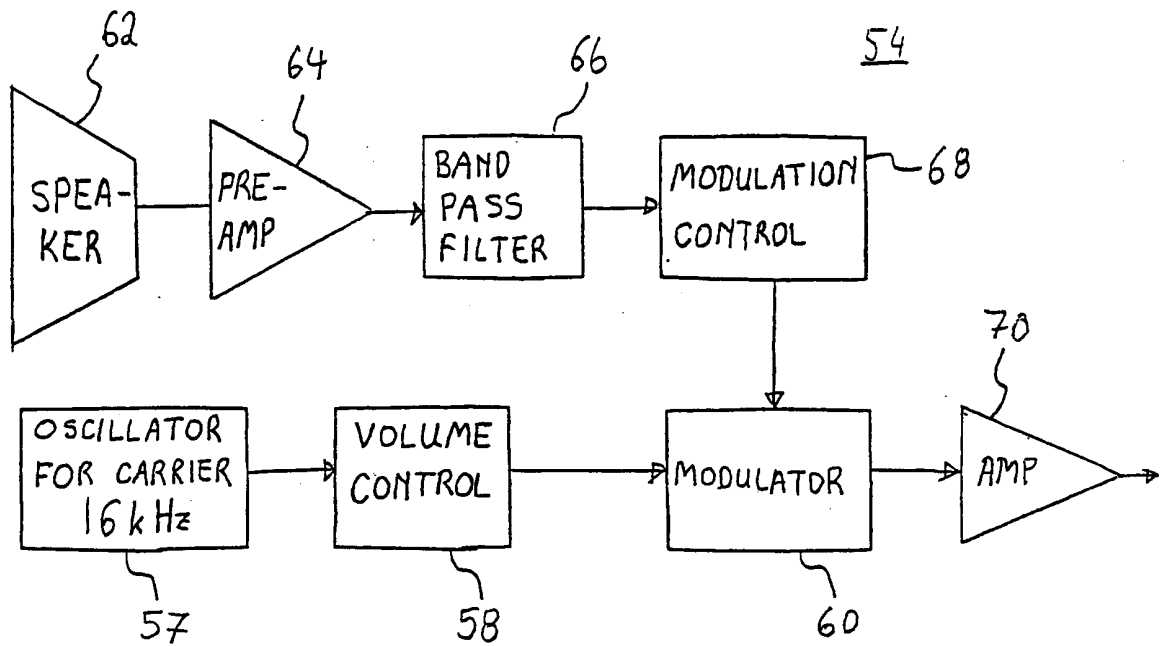


FIG. 2 (PRIOR ART)

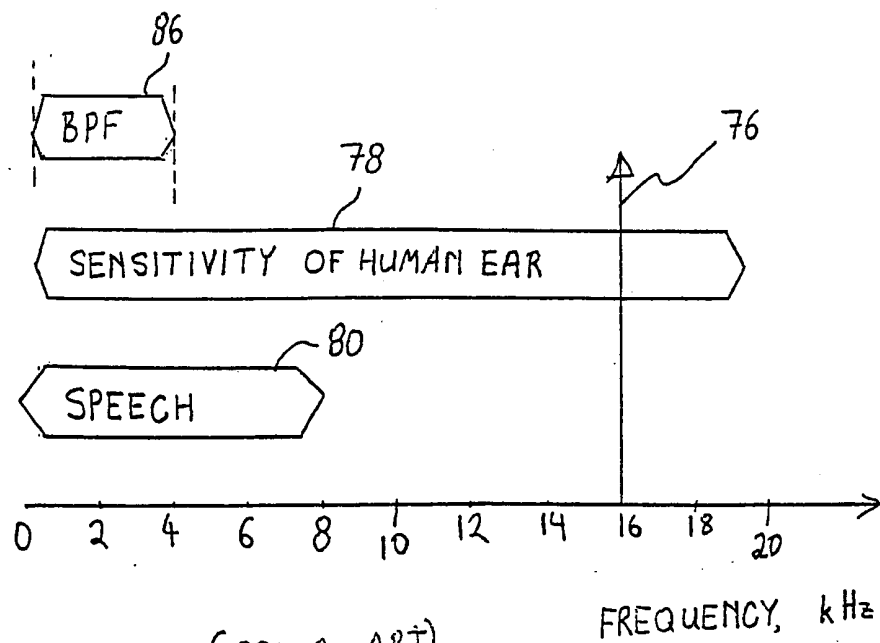


FIG. 3 (PRIOR ART)

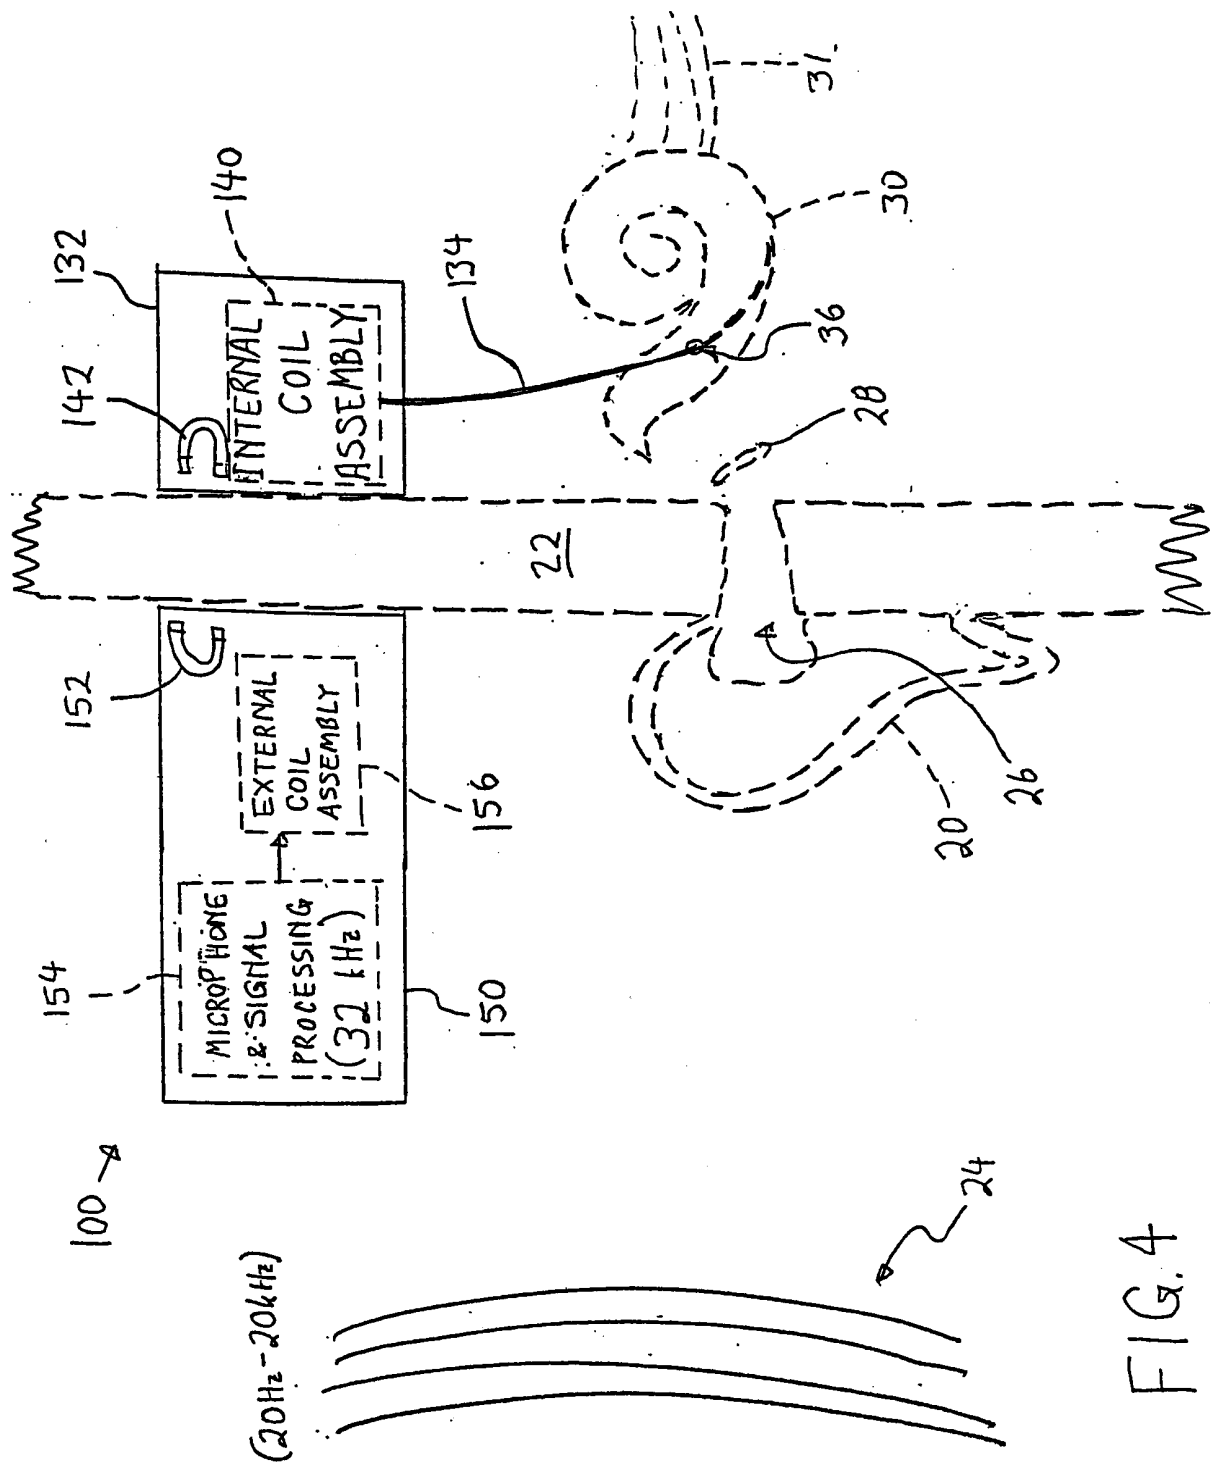


FIG. 4

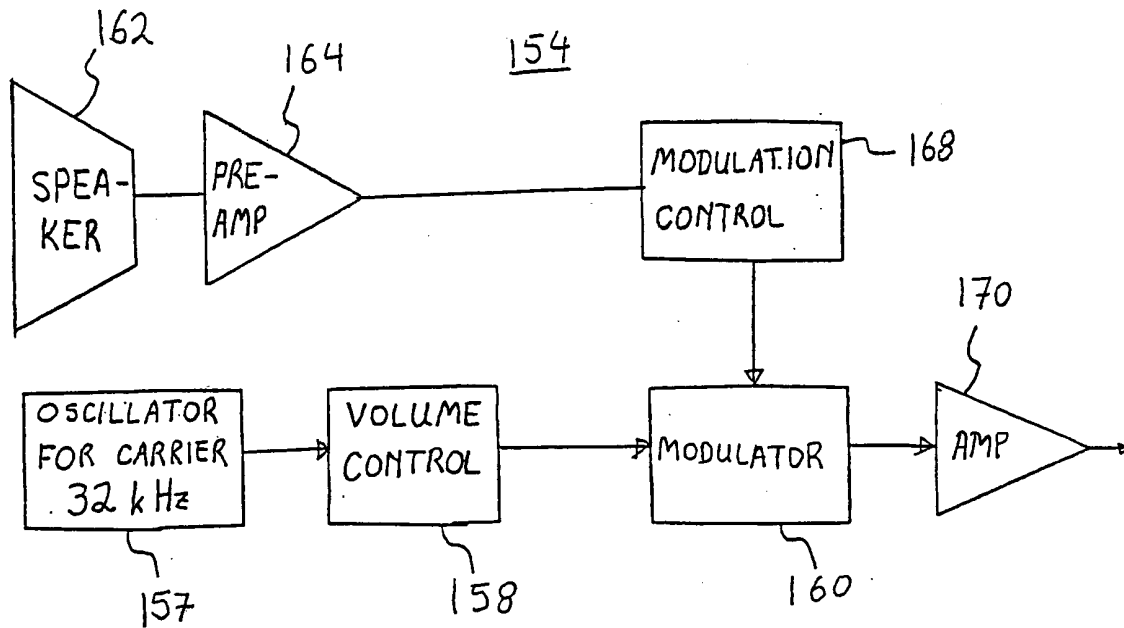


FIG. 5

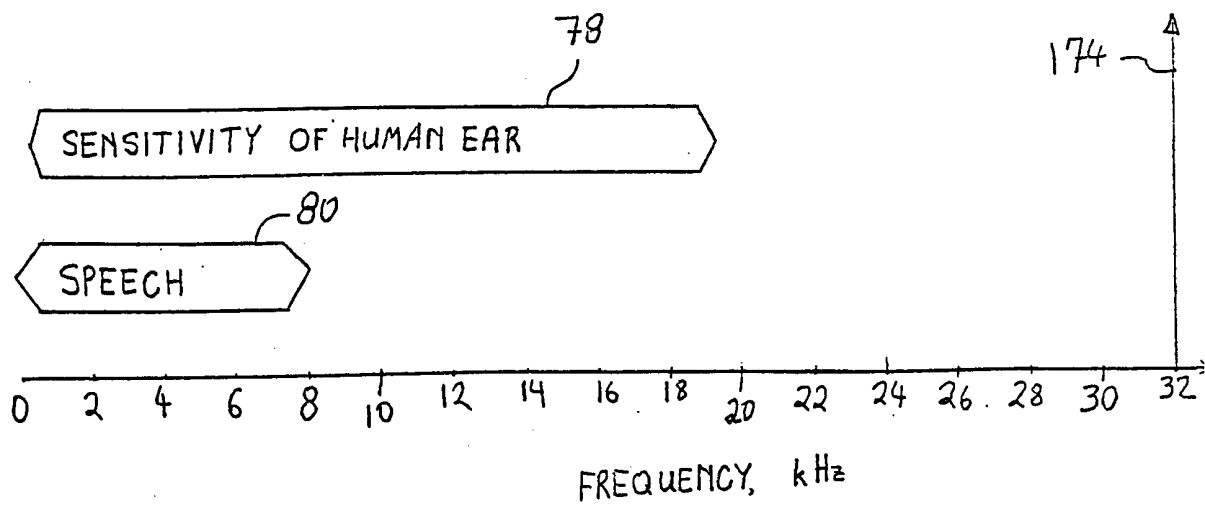


FIG. 6

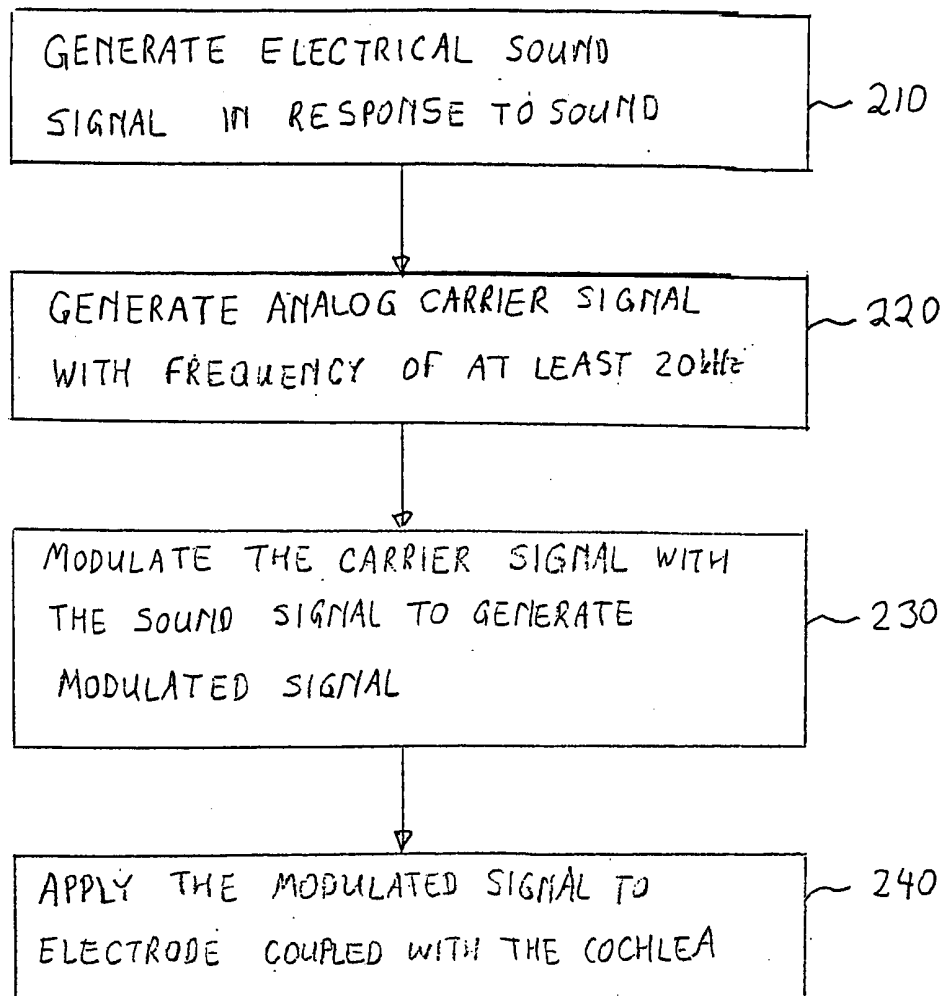


FIG. 7

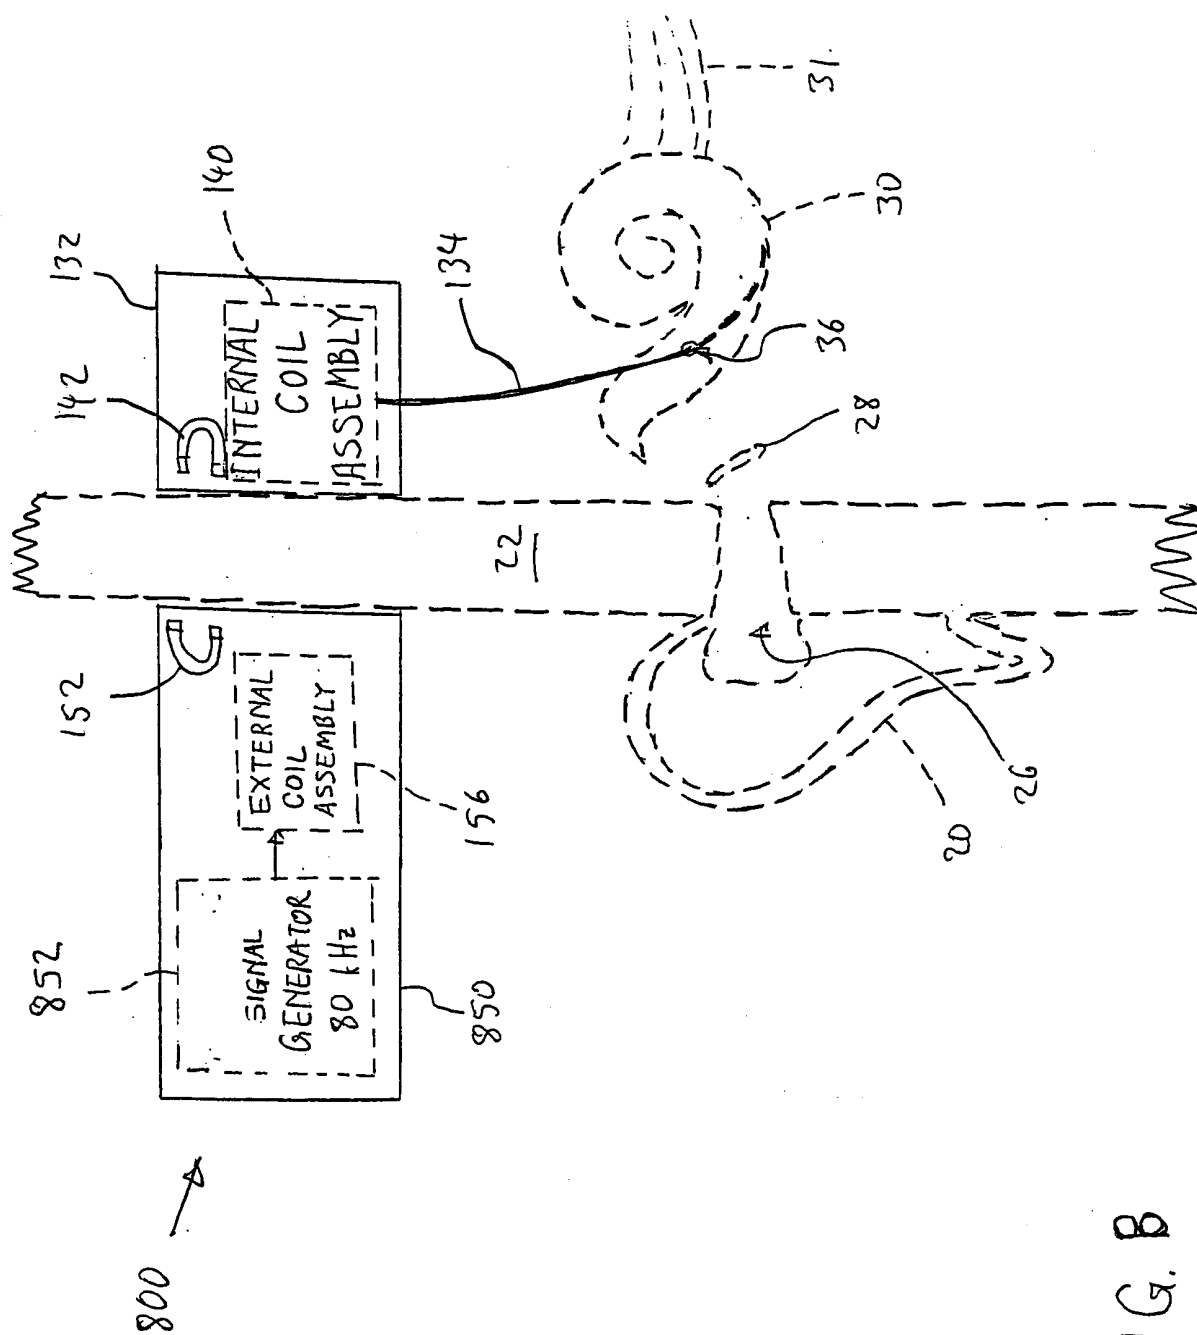


FIG. B

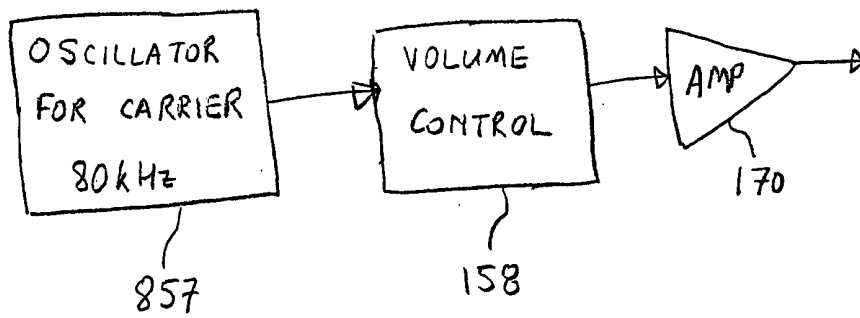


FIG. 9

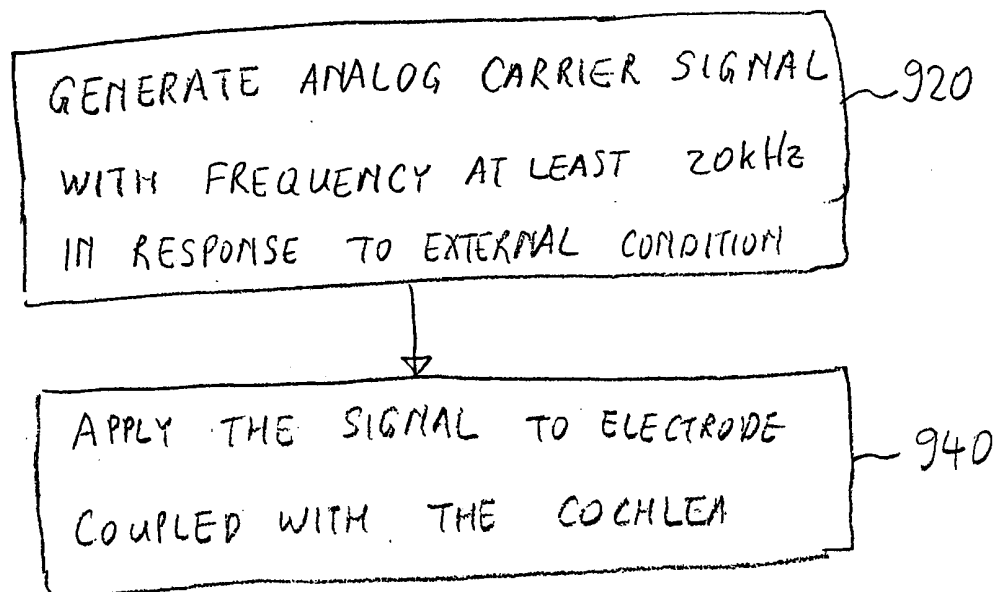


FIG. 10

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US00/35400**A. CLASSIFICATION OF SUBJECT MATTER**

IPC(7) :HO4R 25/00

US CL :381/326,331,151; 600/25; 607/56,57

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 381/326,331,151; 600/25; 607/56,57

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EAST IMAGE AND TEXT

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 4,352,960 A (DORMER) 05 October 1982, see entire doc.	1-10
Y	US 3,586,791 A (PUHARICH et al) 22 June 1971, see entire document	1-10
Y	US 5,571,148 A (LOEB) 05 November 1996, see entire document	1-10



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

21 FEBRUARY 2001

Date of mailing of the international search report

19 JUN 2001

Name and mailing address of the ISA/US
Commissioner of Patents and Trademarks
Box PCT
Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

DIONNE N. HARVEY

Telephone No. (703) 305-1111