



(51) International Patent Classification:

A61M 11/00 (2006.01) A61M 15/08 (2006.01)
A61M 15/00 (2006.01)

(21) International Application Number:

PCT/US2017/021599

(22) International Filing Date:

9 March 2017 (09.03.2017)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/306,045 9 March 2016 (09.03.2016)

US

(71) Applicant: **PROVERIS SCIENTIFIC CORPORATION**
[US/US]; 290 Donald Lynch Blvd., Suite 100, Marlborough,
Massachusetts 01752 (US).

(72) Inventors: **FARINA, Dino John**; 6 Old County Road #33,
Sudbury, Massachusetts 01776 (US). **PITLUK, Zachary**;
122 Canner Street, New Haven, Connecticut 06511 (US).

(74) Agent: **BARKER, Adrian**; Wilson Sonsini Goodrich &
Rosati, 650 Page Mill Road, Palo Alto, California 94304
(US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.


(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: METHODS FOR MEASURING DOSE CONTENT UNIFORMITY PERFORMANCE OF INHALER AND NASAL DEVICES

FIG. 1

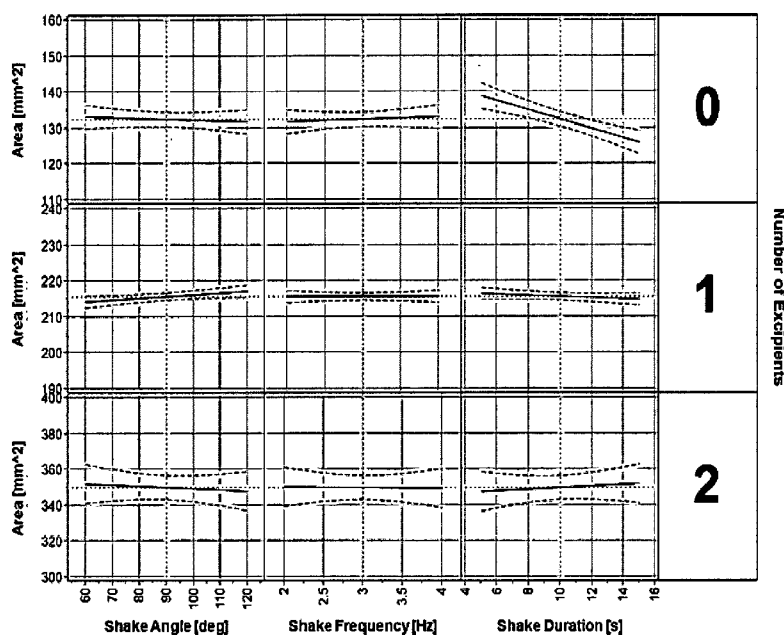

(57) Abstract: The methods described herein provide improvements to the measurement of dose content uniformity of inhaler and nasal devices. The methods involve analyzing and measuring a spray pattern of an emitted spray from an inhaler or nasal device. The spray pattern may be used to determine the dose content uniformity of an inhaler or nasal device.

METHODS FOR MEASURING DOSE CONTENT UNIFORMITY PERFORMANCE OF INHALER AND NASAL DEVICES

CROSS REREFERENCE

[0001] The present application claims priority to U.S. Provisional Application No. 62/306,045 filed on March 9, 2016, which is incorporated herein by reference in its entirety.

BACKGROUND OF THE INVENTION

[0002] The drive for an approved generic albuterol-based pMDI has significantly increased in recent years due to the cost barrier, patent expiration of reference products, and recently released draft FDA guidance documents. Product usage instructions for all of the current FDA approved albuterol pMDIs only include non-descript language for shaking the pMDI such as "... shake well before each use..." with no indication for the patient regarding shaking duration, frequency, orientation, shake-to-fire interval, or what the effects might be if the patient doesn't shake the product before use. From a formulation perspective, shaking is critical for suspension pMDIs because the active drug particles in the formulation tend to rapidly sink or rise to the liquid surface due to differences in density from the propellants.

[0003] The in-vitro spray test methods required to show bioequivalence of pMDI products from a regulatory perspective, particularly dose content uniformity (DCU) and aerodynamic particle size distribution (APSD) through-life testing, may in some instances be time intensive, complicated, and error-prone.

SUMMARY OF THE INVENTION

[0004] In one aspect, a method is provided for measuring performance of an inhaler or nasal device comprising a drug formulation, the method comprising: a) shaking the inhaler or nasal device, wherein the shaking comprises one or more shake parameters; b) actuating the inhaler or nasal device, thereby emitting a spray of the drug formulation; and c) measuring a spray pattern of the spray of the drug formulation, wherein the spray of the drug formulation comprises an emitted dose of a drug, and wherein dose content uniformity (DCU) performance of the inhaler or nasal device is determined based on the spray pattern. In some cases, the inhaler or nasal device is selected from the group consisting of: a pressurized metered dose inhaler (pMDI), a metered dose inhaler (MDI), and a nasal spray. In any of the preceding methods, the one or more shake parameters may comprise one or more of shake frequency, shake angle, shake duration, shake-to-fire interval and shake orientation. In some cases, the shake frequency comprises about 1.0 Hz to about 4.0 Hz. In any of the preceding methods, the shake angle may comprise about 30 degrees to about 180 degrees. In any of the preceding methods, the shake

duration may comprise about 2 seconds to about 15 seconds. In any of the preceding methods, the shake-to-fire interval may comprise about 0 seconds to about 10 seconds. In any of the preceding methods, the shake orientation may comprise about 0 degrees to about 359 degrees. In any of the preceding methods, the drug formulation may comprise a suspension formulation. In any of the preceding methods, the drug formulation comprises one or more excipients. In any of the preceding methods, the drug formulation may comprise no excipients. In any of the preceding methods, the method may further comprise, prior to b), monitoring the one or more shake parameters. In any of the preceding methods, b) may comprise actuating the inhaler or nasal device when the one or more shake parameters have reached or have exceeded a predetermined threshold. In some cases, the predetermined threshold is determined by a composition of the drug formulation. In any of the preceding methods, the method may be performed on the inhaler or nasal device during beginning-of-life administration, middle-of-life administration, end-of-life administration or any combination thereof. In any of the preceding methods, the spray pattern may be an optical spray pattern. In any of the preceding methods, c) may further comprise illuminating the spray with an illumination device and imaging the optical spray pattern with an imaging device. In any of the preceding methods, the spray pattern may be an impaction-based spray pattern. In any of the preceding methods, the spray pattern may be presented on a report. In some cases, the spray pattern may be represented on the report as a sensitivity plot. In some cases, the sensitivity plot may be plotted as a spray pattern area as a function of the one or more shake parameters. In any of the preceding methods, the actuating may comprise a length of time a valve of the inhaler or nasal device is left open by the actuating. In any of the preceding methods, the actuating may comprise compressing the inhaler or nasal device. In some cases, the compressing may comprise a stroke length. In some cases, the stroke length may comprise about 1 millimeter to about 200 millimeters.

[0005] In another aspect, a method is provided for testing for delivery of a drug formulation with an inhaler or nasal device, the method comprising: a) monitoring two or more shake parameters; and b) actuating the inhaler or nasal device when a predetermined threshold of the two or more shake parameters is reached or exceeded, thereby emitting a spray of the drug formulation, wherein the spray of the drug formulation comprises an emitted dose of a drug. In some cases, the emitted dose of a drug may be within about 15% of a target dose content uniformity (DCU) performance. In some cases, the target DCU performance may be defined by regulatory or industry guidelines. In any of the preceding methods, the method may further comprise repeating the monitoring and actuating one or more times, thereby emitting one or more additional sprays of the drug formulation, wherein each of the one or more additional sprays may comprise an emitted dose of the drug. In some cases, each of the one or more

additional sprays may comprise an emitted dose of the drug within about 15% of the target DCU performance. In any of the preceding methods, the two or more shake parameters may be selected from the group consisting of: shake duration, shake frequency, shake angle, shake-to-fire interval, and shake orientation. In any of the preceding methods, the method may further comprise, prior to a), shaking the inhaler or nasal device. In some cases, the shake duration may comprise about 2 seconds to about 15 seconds. In some cases, the shake angle may comprise about 30 degrees to about 180 degrees. In some cases, the shake frequency may comprise about 1.0 Hz to about 4.0 Hz. In some cases, the shake-to-fire interval may comprise about 0 seconds to about 10 seconds. In some cases, the shake orientation may comprise about 0 degrees to about 359 degrees. In any of the preceding cases, the monitoring may comprise measuring the two or more shake parameters. In any of the preceding cases, the drug formulation may comprise one or more excipients. In any of the preceding cases, the drug formulation may comprise no excipients. In some cases, the predetermined threshold may be determined based on (i) a number of the one or more excipients present in the drug formulation, (ii) a composition of the one or more excipients present in the drug formulation, or (iii) a combination of both. In some cases, each of the one or more additional sprays may comprise an emitted dose of the drug within about 15% of the target DCU performance at each of beginning-of-life administration, middle-of-life administration and end-of-life administration. In any of the preceding methods, the method may further comprise administering the emitted dose of a drug to a patient in need thereof. In any of the preceding methods, the method may further comprise, after the actuating, performing a spray pattern analysis on the spray. In some cases, the method may further comprise, determining an amount of the emitted dose of a drug from the spray pattern analysis. In some cases, performing the spray pattern analysis may comprise measuring an optical spray pattern of the spray. In some cases, measuring the optical spray pattern of the spray may comprise illuminating the spray with an illumination device and imaging the optical spray pattern with an imaging device. In some cases, performing the spray pattern analysis may comprise measuring an impaction-based spray pattern of the spray. In any of the preceding methods, the inhaler or nasal device may be selected from the group consisting of: a pressurized metered dose inhaler (pMDI), a metered dose inhaler (MDI), and a nasal spray. In any of the preceding claims, the drug formulation may comprise a suspension formulation. In some cases, the spray pattern analysis may be presented on a report. In some cases, the spray pattern analysis may be represented on the report as a sensitivity plot. In some cases, the sensitivity plot may be plotted as a spray pattern area as a function of at least one of the two or more shake parameters. In any of the preceding methods, the actuating may comprise a length of time a valve of the inhaler or nasal device is left open by the actuating. In any of the preceding

methods, the actuating may comprise compressing the inhaler or nasal device. In some cases, the compressing may comprise a stroke length. In some cases, the stroke length may comprise about 1 millimeter to about 200 millimeters.

[0006] In another aspect, a method is provided for testing for delivery of a drug formulation with an inhaler or nasal device, the method comprising: a) monitoring one or more shake parameters, wherein at least one of the one or more shake parameters comprises shake angle, shake frequency, shake-to-fire interval, or shake orientation; and b) actuating the inhaler or nasal device when a predetermined threshold of the one or more shake parameters is reached or exceeded, thereby emitting a spray of the drug formulation, wherein the spray of the drug formulation comprises an emitted dose of a drug. In some cases, the emitted dose of a drug may be within about 15% of a target dose content uniformity (DCU) performance. In some cases, the DCU performance may be defined by regulatory or industry guidelines. In any of the preceding methods, the method may further comprise repeating the monitoring and actuating one or more times, thereby emitting one or more additional sprays of the drug formulation, wherein each of the one or more additional sprays comprises an emitted dose of the drug. In some cases, each of the one or more additional sprays may comprise an emitted dose of the drug within about 15% of the target DCU performance. In any of the preceding methods, the one or more shake parameters may further comprise shake duration. In any of the preceding methods, the method may further comprise, prior to the monitoring, shaking the inhaler or nasal device. In some cases, the shake duration may comprise about 2 seconds to about 15 seconds. In any of the preceding methods, the shake angle may comprise about 30 degrees to about 180 degrees. In any of the preceding methods, the shake frequency may comprise about 1.0 Hz to about 4.0 Hz. In any of the preceding methods, the shake-to-fire interval may comprise about 0 seconds to about 10 seconds. In any of the preceding methods, the shake orientation may comprise about 0 degrees to about 359 degrees. In any of the preceding methods, the monitoring may comprise measuring the one or more shake parameters. In any of the preceding methods, the drug formulation may comprise one or more excipients. In any of the preceding methods, the drug formulation may comprise no excipients. In some cases, the predetermined threshold may be determined based on (i) a number of the one or more excipients present in the drug formulation, (ii) a composition of the one or more excipients present in the drug formulation, or (iii) a combination of both. In some cases, each of the one or more additional sprays may comprise an emitted dose of the drug within about 15% of the target DCU performance at each of beginning-of-life administration, middle-of-life administration and end-of-life administration. In any of the preceding methods, the method may further comprise administering the emitted dose of a drug to a patient in need thereof. In any of the preceding methods, the method may further comprise,

after the actuating, performing a spray pattern analysis on the spray. In any of the preceding methods, the method may further comprise, determining an amount of the emitted dose of a drug from the spray pattern analysis. In some cases, performing the spray pattern analysis may comprise measuring an optical spray pattern of the spray. In some cases, measuring the optical spray pattern of the spray comprises illuminating the spray with an illumination device and imaging the optical spray pattern with an imaging device. In some cases, performing the spray pattern analysis may comprise measuring an impaction-based spray pattern of the spray. In any of the preceding methods, the inhaler or nasal device may be selected from the group consisting of: a pressurized metered dose inhaler (pMDI), a metered dose inhaler (MDI), and a nasal spray. In any of the preceding methods, the drug formulation may comprise a suspension formulation. In any of the preceding methods, the spray pattern analysis may be presented on a report. In some cases, the spray pattern analysis may be represented on the report as a sensitivity plot. In some cases, the sensitivity plot may be plotted as a spray pattern area as a function of the one or more shake parameters. In any of the preceding methods, the actuating may comprise a length of time a valve of the inhaler or nasal device is left open by the actuating. In any of the preceding methods, the actuating may comprise compressing the inhaler or nasal device. In some cases, the compressing may comprise a stroke length. In some cases, the stroke length may comprise about 1 millimeter to about 200 millimeters.

INCORPORATION BY REFERENCE

[0007] All publications, patents, and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication, patent, or patent application was specifically and individually indicated to be incorporated by reference.

BRIEF DESCRIPTION OF THE DRAWINGS

[0008] The novel features of the invention are set forth with particularity in the appended claims. A better understanding of the features and advantages of the present invention will be obtained by reference to the following detailed description that sets forth illustrative embodiments, in which the principles of the invention are utilized, and the accompanying drawings of which:

[0009] **FIG. 1** depicts consolidated optical spray pattern sensitivity profiles for three tested pMDI products as a function of shaking. The tested pMDI products are identified by the number of excipients. Auto-scaled y-axes were used to accommodate the different spray pattern area ranges for the products.

[0010] **FIG. 2** depicts the effects of shaking versus not shaking on through-life DCU performance for a tested product with no excipients.

[0011] **FIG. 3** depicts a detailed view of end of life DCU performance for a tested product with no excipients, with and without shaking.

DETAILED DESCRIPTION OF THE INVENTION

[0012] The methods described herein generally relate to improving delivery of a formulation with oral inhaler or nasal devices. The methods also relate to the measurement of dose content uniformity (DCU) performance of oral inhaler or nasal devices. Oral inhaler or nasal products generally require “proper shaking” prior to actuation of the device to ensure that a target dose of drug is delivered. However, it is often unclear as to what parameters constitute “proper shaking.” The dose of drug delivered by the inhaler or nasal device can be adversely affected by improper shaking, for example, not shaking long enough or not shaking at the proper angle. Further, the drug formulation may affect the shaking parameters required to achieve “proper shaking”. For example, factors including the number of excipients present in the formulation, the composition of the excipients present in the formulation, as well as other physical factors may determine the shaking parameters required to achieve “proper shaking.”

[0013] In some instances, the devices (e.g. oral inhalers or nasal devices) referred to herein may be sprayed (e.g. via actuation, etc) after undergoing different parameters of shaking, and a spray pattern may be measured and/or recorded for the differing parameters of shaking. Optionally, the spray patterns may be analyzed and correlated with the DCU of the formulations being administered (e.g. sprayed), and desired shake parameters may be determined, e.g. based on the correlation. Accordingly, the present methods may provide an avenue for determining desired shake parameters, tailored to specific formulations, for delivery of the formulation via the devices.

[0014] In one aspect, the methods involve measuring the performance of an inhaler or nasal device comprising a drug formulation. The method may comprise: a) shaking the inhaler or nasal device; b) actuating the inhaler or nasal device, thereby emitting a spray of the drug formulation; and c) measuring a spray pattern of the spray of the drug formulation, wherein the spray of the drug formulation comprises an emitted dose of a drug. The dose content uniformity (DCU) performance of the inhaler or nasal device may be determined based on the spray pattern.

[0015] In another aspect, the methods may involve improving delivery of a drug formulation with an inhaler or nasal device. The method may comprise: a) monitoring two or more shake parameters; and b) actuating the inhaler or nasal device when a predetermined threshold of the

two or more shake parameters is reached or exceeded, thereby emitting a spray of the drug formulation, wherein the spray of the drug formulation comprises an emitted dose of a drug.

[0016] In yet another aspect, the methods may involve improving delivery of a drug formulation with an inhaler or nasal device. The method may comprise: a) monitoring one or more shake parameters, wherein at least one of the one or more shake parameters comprises shake angle, shake frequency, shake-to-fire interval, or shake orientation; and b) actuating the inhaler or nasal device when a predetermined threshold of the one or more shake parameters is reached or exceeded, thereby emitting a spray of the drug formulation, wherein the spray of the drug formulation comprises an emitted dose of a drug.

[0017] The methods disclosed herein may generally be used to measure the performance of inhaler or nasal devices. An inhaler device may be utilized for e.g., delivery of a drug or substance directly to the lungs of a subject. The methods described herein may be suitable for use with any inhaler device that requires shaking and/or actuation. In some cases, the inhaler device is a metered-dose inhaler (MDI), for example, a pressurized metered-dose inhaler (pMDI). Non-limiting examples of MDIs may include AeroChamber® and Autohaler®. In some cases, the MDI comprises a spacer or aerosol holding chamber. The inhaler device may be a dry powder inhaler, non-limiting examples including: Aerolizer®, Diskus®, Ellipta™, Flexhaler®, Handihaler®, Neohaler®, Pressair™, Twisthaler®, Rotahaler® and Turbuhaler®. In some cases, the methods may be used with a nasal device for, e.g., local delivery of a drug to the nose or the paranasal sinuses. Non-limiting examples of nasal devices may include: mechanical spray pumps (e.g., squeeze bottles, multi-dose metered-dose spray pumps, single/duo-dose spray pumps, bi-directional multi-dose spray pumps), gas-driven spray systems/atomizers, mechanical powder sprayers, breath actuated inhalers, and insufflators.

[0018] The inhaler or nasal device may be an Orally Inhaled or Nasal Drug Product (OINDP). Non-limiting examples of OINDPs which may be suitable for use with the methods described herein may include: aclidinium bromide inhalation powder (Tudorza® Pressair®), ipratropium inhalation aerosol (Atrovent® HFA), tiotropium inhalation powder Spiriva® Handihaler®), tiotropium inhalation solution (Spiriva® Respimat®), umeclidinium inhalation powder (Incruse® Ellipta®), albuterol/ipratropium inhalation solution (DuoNeb®), albuterol/ipratropium bromide inhalation spray (Combivent® Respimat®), budesonide/formoterol fumarate dihydrate inhalation aerosol (Symbicort®), fluticasone/salmeterol inhalation powder (Advair® Diskus®), fluticasone/salmeterol inhalation aerosol (Advair® HFA), fluticasone furoate/vilanterol inhalation powder (Breo® Ellipta®), mometasone furoate/formoterol fumarate inhalation aerosol (Dulera®), tiotropium bromide/olodaterol inhalation spray (Stiolto™ Respimat®), umeclidinium/ vilanterol inhalation

powder (Anoro® Ellipta®), beclomethasone dipropionate HFA inhalation aerosol (Qvar®), budesonide inhalation powder (Pulmicort® Flexhaler®), budesonide inhalation suspension (Pulmicort® Respules®), ciclesonide inhalation aerosol (Alvesco®), flunisolide inhalation aerosol (Aerospan®), fluticasone furoate inhalation powder (Arnuity™ Ellipta®), fluticasone propionate inhalation aerosol (Flovent® HFA), fluticasone propionate inhalation powder (Flovent® Diskus®), mometasone furoate inhalation powder (Asmanex® Twisthaler®), mometasone furoate inhalation aerosol (Asmanex® HFA), arformoterol tartrate inhalation solution (Brovana®), formoterol fumarate inhalation powder (Foradil®), formoterol fumarate inhalation solution (Perforomist®), indacaterol inhalation powder (Arcapta™ Neohaler™), olodaterol inhalation spray (Striverdi® Respimat®), salmeterol xinafoate inhalation powder (Serevent® Diskus®), albuterol sulfate inhalation powder (Proair® Respiclick®), albuterol sulfate inhalation aerosol (Proair® HFA), albuterol inhalation solution (AccuNeb®), albuterol sulfate inhalation aerosol (Proventil® HFA), albuterol sulfate inhalation aerosol (Ventolin® HFA), levalbuterol tartrate inhalation aerosol (Xopenex® HFA).

[0019] The inhaler or nasal device may include a formulation of, for example, a drug or an active ingredient. In some cases, the formulation includes one or more excipients. In some cases, the formulation does not include any excipients. In some cases, the formulation includes one or more propellants. The formulation may be a suspension, a solution, or a dry powder.

[0020] The methods may generally involve shaking the inhaler or nasal device. In some cases, shaking the inhaler or nasal device involves performing a shaking regimen with the inhaler or nasal device. A shaking regimen may include one or more shake parameters, including one or more of shake duration, shake angle, shake frequency, shake-to-fire interval, and shake orientation. The shaking regimen may be the specific combination of the one or more shake parameters required to be performed on the device in order to deliver, upon actuation of the device, an intended dosage range of a drug. The shaking regimen may be specific for a particular product and may be at least partly dependent on the formulation of the drug, one or more characteristics of the device, the volume of the metering valve, the relative mixing efficiency of the drug particles in the formulation with the excipient(s) and/or propellant(s), or any combination thereof. The shaking regimen may be affected by the composition of the formulation present in the canister (e.g., the number of excipients present with the drug in the formulation or the specific composition of the excipients present in the formulation). Therefore, different products each including the same drug may require very different shaking regimens to deliver an intended dosage range. In some embodiments, the methods provided herein may allow a user or tester of an inhaler or nasal device to identify the specific shake parameters (i.e.,

shake regimen) required to deliver an intended dosage range of drug from a specific inhaler or nasal device product.

[0021] The methods herein may involve monitoring one or more shake parameters of the inhaler or nasal device. The one or more shake parameters may include one or more of shake duration, shake angle, shake frequency, shake-to-fire interval and shake orientation.

[0022] The term “shake duration” as used herein may refer to the length of time the inhaler or nasal device is shaken. In some instances, the shake duration may refer to a desired length of time the device should be shaken, e.g. as determined during a shake study using the methods described herein. A desired shake duration may differ for different formulations of drugs (e.g. comprising different active ingredients and/or excipients). In some instances, a desired shake duration may differ for differing devices. A shake duration may be within a range of about 1 second to about 30 seconds. In some instances, a shake duration may be equal to about, or greater than about 1 second, 2 seconds, 3 seconds, 4 seconds, 5 seconds, 6, seconds, 7 seconds, 8 seconds, 9 seconds, 10 seconds, 11 seconds, 12 seconds, 13 seconds, 14 seconds, 15 seconds, 20 seconds, 25 seconds, 30 seconds, 35 second, 40 second, 45 seconds, 50 seconds, 55 second, 60 seconds.

[0023] The term “shake angle” as used herein may refer to the angle of the canister of the device during shaking as measured from its vertical axis. For example, a shake angle of 90 degrees would include shaking the canister horizontally. In some instances, the shake angle may refer to a desired angle the device or canister of the device should be shaken in, e.g. as determined during a shake study described in the present disclosure. A desired shake angle may differ for different formulations of drugs (e.g. comprising different active ingredients and/or excipients). In some instances, a desired shake angle may differ for differing devices. A shake angle may be within a range of about 30 degrees to about 180 degrees. In some instances, a shake angle may be equal to, or greater than about 0 degrees, 10 degrees, 20 degrees, 30 degrees, 40 degrees, 50 degrees, 60 degrees, 70 degrees, 80 degrees, 90 degrees, 100 degrees, 110 degrees, 120 degrees, 130 degrees, 140 degrees, 150 degrees, 160 degrees, 170 degrees, 180 degrees.

[0024] The term “shake frequency” as used herein may refer to the number of times (cycles) the device is shaken in a given time period. In some instances, the shake frequency may refer to a desired frequency the device should be shaken in a given time period, e.g. as determined during a shake study. A desired shake frequency may differ for different formulations of drugs (e.g. comprising different active ingredients and/or excipients). In some instances, a desired shake frequency may differ for differing devices. A shake frequency may be measured in Hertz (Hz) which is defined as the number of cycles in 1 second. A shake frequency may be within a range from about 1.0 Hz to about 5.0 Hz. In some instances, a shake frequency may be equal to about,

or greater than about 0.5 Hz, 1.0 Hz, 1.5 Hz, 2.0 Hz, 2.5 Hz, 3.0 Hz, 3.5 Hz, 4.0 Hz, 4.5 Hz, 5.0 Hz, 6.0 Hz, 7.0 Hz, 8.0 Hz, 9.0 Hz, or 10.0 Hz.

[0025] The term “shake-to-fire interval” as used herein may refer to the length of time that occurs between the end of a shaking regimen and the actuation of the device. In some instances, the shake-to-fire interval may refer to a desired length of time that occurs between the end of a shaking regimen and the actuation of the device, e.g. as determined during a shake study. A desired shake-to-fire interval may differ for different formulations of drugs (e.g. comprising different active ingredients and/or excipients). In some instances, a desired shake-to-fire interval may differ for differing devices. A shake-to-fire interval may be within a range from about 0 seconds to about 30 seconds. In some instances, a shake-to-fire interval may be equal to about, or greater than about 0 seconds (i.e., immediate actuation after shaking), 1 second, 2 seconds, 3 seconds, 4 seconds, 5 seconds, 6, seconds, 7 seconds, 8 seconds, 9 seconds, 10 seconds, 11 seconds, 12 seconds, 13 seconds, 14 seconds, 15 seconds, 20 seconds, 25 seconds, 30 seconds, 40 second, 50 seconds, or 60 seconds.

[0026] The term “shake orientation” as used herein may refer to an angular range that the device undergoes during shaking. For example, if the device, or canister, is shaken not in an up and down or side to side motion, but in an angular motion, a shake orientation for the device may be relevant. In some instances, the shake orientation may refer to a desired angular range that the device should undergo during shaking. In some instances, the shake orientation may refer to a desired shake orientation of the device, e.g., as determined during a shake study. A desired shake orientation may differ for different formulations of drugs (e.g., comprising different active ingredients and/or excipients). In some instances, a desired shake orientation may differ for differing devices. A shake orientation may be within a range from about 0 to about 359 degrees. In some instances, a shake orientation may be equal to about, or greater than about 0 degrees, 10 degrees, 20 degrees, 30 degrees, 40 degrees, 50 degrees, 60 degrees, 70 degrees, 80 degrees, 90 degrees, 100 degrees, 110 degrees, 120 degrees, 130 degrees, 140 degrees, 150 degrees, 160 degrees, 170 degrees, 180 degrees, 190 degrees, 200 degrees, 210 degrees, 220 degrees, 230 degrees, 240 degrees, 250 degrees, 260 degrees, 270 degrees, 280 degrees, 290 degrees, 300 degrees, 310 degrees, 320 degrees, 330 degrees, 340 degrees, 350 degrees, or 360 degrees.

[0027] In some examples, the appropriate shaking regimen for a particular inhaler or nasal device products may be unknown. The methods herein may involve testing a specific inhaler or nasal device product in order to determine the appropriate shaking regimen, for example, by monitoring or measuring one or more shake parameters of the inhaler or nasal device, and then measuring the emitted dose of drug after actuation of the device. Methods of measuring the

emitted dose of drug and determining the dose content uniformity performance of the device are described below.

[0028] In some embodiments, determining an appropriate shaking regimen may involve adjusting one or more shake parameters and measuring an emitted dose of drug from the device after actuation. In some cases, the effect of a single shake parameter on the performance of a device may be tested (e.g., shake angle). In such cases, the methods may involve shaking the inhaler or nasal device at a defined shake angle (e.g., 30 degrees), actuating the device, and recording the emitted dose, then subsequently shaking the device at a different shake angle (e.g., 40 degrees), actuating the device, and recording the emitted dose. This method may be repeated a plurality of times, each time varying the shake angle and recording the emitted dose. The method may then be used to determine the appropriate shake angle required to emit a target dosage range of drug. The method can be used to test the performance of an inhaler or nasal device with any number of shake parameters as described herein. In some cases, one, two, three, four, or five shake parameters are tested. In some cases, combinations of shake parameters may be tested (e.g., testing a specific combination of shake angle and shake frequency required to emit a target dosage range of drug).

[0029] The methods described herein may include actuating the device, after a shaking regimen has been performed, to release an amount of the formulation. In some cases, the formulation is released from the inhaler or nasal device in a spray. The spray may contain an emitted dose of a drug. The term “actuation” may refer to the act of compressing the canister of an inhaler or nasal device for a period of time to release a substance contained within the canister or the holder of the device. Actuation may be, for example, automated actuation or hand actuation.

[0030] Actuation of the device, for example, may release a single dose of a formulation contained therein. Proper actuation of the device may be required to release a target dosage of drug from the device. For example, an inhaler or nasal device that has been properly shaken according to a prescribed shaking regimen may deliver an unintended dosage of drug if the device is not properly actuated. As such, the methods provided herein may involve measuring or monitoring actuation of the inhaler or nasal device. Actuating an inhaler or nasal device may include one or more actuation parameters. The one or more actuation parameters may include, without limitation, compression velocity, compression acceleration, actuation hold time, decompression velocity, decompression acceleration, actuation stroke length, and any combination thereof. Thus, measuring or monitoring actuation of an inhaler or nasal device may involve measuring or monitoring one or more actuation parameters.

[0031] “Compression velocity” as used herein may refer to the speed with which the device is compressed (e.g., the speed with which a user pushes or compresses the canister or nasal

actuator during actuation). Compression velocity may be from about 10 mm/s to about 100 mm/s. For example, compression velocity may be about 10 mm/s, 15 mm/s, 20 mm/s, 25 mm/s, 30 mm/s, 35 mm/s, 40 mm/s, 45 mm/s, 50 mm/s, 55 mm/s, 60 mm/s, 65 mm/s, 70 mm/s, 75 mm/s, 80 mm/s, 85 mm/s, 90 mm/s, 95 mm/s, 100 mm/s or greater than 100 mm/s.

[0032] “Compression acceleration” as used herein may refer to the rate of change in velocity per unit time of the canister or nasal actuator during compression. Compression acceleration may be from about 500 mm/s² to about 4000 mm/s². For example, compression acceleration may be about 500 mm/s², 600 mm/s², 700 mm/s², 800 mm/s², 900 mm/s², 1000 mm/s², 1100 mm/s², 1200 mm/s², 1300 mm/s², 1400 mm/s², 1500 mm/s², 1600 mm/s², 1700 mm/s², 1800 mm/s², 1900 mm/s², 2000 mm/s², 2100 mm/s², 2200 mm/s², 2300 mm/s², 2400 mm/s², 2500 mm/s², 2600 mm/s², 2700 mm/s², 2800 mm/s², 2900 mm/s², 3000 mm/s², 3100 mm/s², 3200 mm/s², 3300 mm/s², 3400 mm/s², 3500 mm/s², 3600 mm/s², 3700 mm/s², 3800 mm/s², 3900 mm/s², 4000 mm/s² or greater than 4000 mm/s².

[0033] “Actuation hold time” as used herein may refer to the amount of time a device is held in its fully actuated state. “Fully actuated” may refer to maximal compression of the canister of an inhaler or nasal device. Actuation of a device may include compression of a device and may include an “actuation hold time window”, for example, a period of time in which a device is held in its fully actuated state. An actuation hold time window may be from about 0 seconds to about 30 seconds. For examples, an actuation hold time window may be about, for example, 0 seconds (immediate release), 1 second, 2 seconds, 3 seconds, 4 seconds, 5 seconds, 6 seconds, 7 seconds, 8 seconds, 9 seconds, 10 seconds, 11 seconds, 12 seconds, 13 seconds, 14 seconds, 15 seconds, 16 seconds, 17 seconds, 18 seconds, 19 seconds, 20 seconds, 21 seconds, 22 seconds, 23 seconds, 24 seconds, 25 seconds, 26 seconds, 27 seconds, 28 seconds, 29 seconds, 30 seconds or greater than 30 seconds.

[0034] “Decompression velocity” as used herein may refer to the speed with which the device is decompressed (e.g., speed with which a user releases or decompresses the canister or nasal actuator after actuation). Decompression velocity may be from about 10 mm/s to about 100 mm/s. For example, decompression velocity may be about 10 mm/s, 15 mm/s, 20 mm/s, 25 mm/s, 30 mm/s, 35 mm/s, 40 mm/s, 45 mm/s, 50 mm/s, 55 mm/s, 60 mm/s, 65 mm/s, 70 mm/s, 75 mm/s, 80 mm/s, 85 mm/s, 90 mm/s, 95 mm/s, 100 mm/s or greater than 100 mm/s.

[0035] “Decompression acceleration” as used herein may refer to the rate of change of velocity per unit time during decompression of the canister or nasal actuator during decompression. Decompression acceleration may be from about 500 mm/s² to about 4000 mm/s². For example, decompression acceleration may be about 500 mm/s², 600 mm/s², 700 mm/s², 800 mm/s², 900 mm/s², 1000 mm/s², 1100 mm/s², 1200 mm/s², 1300 mm/s², 1400 mm/s², 1500 mm/s², 1600

mm/s², 1700 mm/s², 1800 mm/s², 1900 mm/s², 2000 mm/s², 2100 mm/s², 2200 mm/s², 2300 mm/s², 2400 mm/s², 2500 mm/s², 2600 mm/s², 2700 mm/s², 2800 mm/s², 2900 mm/s², 3000 mm/s², 3100 mm/s², 3200 mm/s², 3300 mm/s², 3400 mm/s², 3500 mm/s², 3600 mm/s², 3700 mm/s², 3800 mm/s², 3900 mm/s², 4000 mm/s² or greater than 4000 mm/s².

[0036] “Actuation stroke length” as used herein may refer to the maximum amount the device is compressed during actuation. In some cases, the actuation stroke length is the mechanical compression limit for the device. Actuation stroke length may be from about 3 mm to about 20 mm. For example, actuation stroke length may be about 3 mm, 4 mm, 5 mm, 6 mm, 7 mm, 8 mm, 9 mm, 10 mm, 11 mm, 12 mm, 13 mm, 14 mm, 15 mm, 16 mm, 17 mm, 18 mm, 19 mm, 20 mm or greater than 20 mm.

[0037] In some examples, the appropriate actuation parameters for a particular inhaler or nasal device products may be unknown. The methods herein may involve testing a specific inhaler or nasal device product in order to determine the appropriate actuation parameters, for example, by monitoring or measuring one or more actuation parameters of the inhaler or nasal device, and then measuring the emitted dose of drug. Methods of measuring the emitted dose of drug and determining the dose content uniformity performance of the device are described below. In some embodiments, determining the appropriate actuation parameters may involve adjusting one or more actuation parameters and measuring an emitted dose of drug from the device. In some cases, the effect of a single actuation parameter on the performance of a device may be tested (e.g., actuation hold time). In such cases, the methods may involve actuating the inhaler or nasal device for a defined actuation hold time (e.g., 1 second), and recording the emitted dose, then subsequently actuating the device for a different actuation hold time (e.g., 2 seconds), and recording the emitted dose.

[0038] This method may be repeated a plurality of times, each time varying the actuation hold time and recording the emitted dose. The method may then be used to determine the appropriate actuation hold time required to emit a target dosage range of drug. The method can be used to test the performance of an inhaler or nasal device with any number of actuation parameters as described herein. In some cases, one, two, three, four, five, or six actuation parameters are tested. In some cases, combinations of actuation parameters may be tested (e.g., testing a specific combination of actuation hold time and compression velocity required to emit a target dosage range of drug). In other cases, one or more shake parameters may be combined with one or more actuation parameters to test the effect of specific combinations of shake parameters and actuation parameters on the performance of an inhaler or nasal device.

[0039] The methods may further include measuring or analyzing a spray pattern of a spray of drug formulation released from the device after actuation. Although specific embodiments of

measuring spray pattern are provided herein, it is envisioned that any method of measuring, or analyzing the spray characteristics of a spray released from an inhaler or nasal device may be utilized. Accordingly, it is to be understood that as used throughout, a spray pattern may refer to any characteristics of the spray, e.g. including the spray's divergence angle (e.g. plume geometry) as the spray exist the device, the spray's cross-sectional ellipticity, uniformity and particle/droplet distribution. In some cases, measuring the spray pattern of a spray involves measuring the time evolution of a spray plume (e.g., by taking multiple measurements of a spray plume over a period of time).

[0040] The spray pattern measurement may be further utilized as key identifiers for determining the appropriateness of shake parameters, e.g. for specific drug formulations and/or differing devices. In some instances, the spray pattern measurements may be utilized to verifying consistency and desired performance of the devices (e.g. oral inhalers, nasal devices, etc) having undergone the shake parameters. In some instances, the spray pattern measurements may be used to determine a dose content uniformity (DCU) performance of the devices. Optionally, the spray pattern measurements may be correlated with DCU. Further, based on the DCU performance and/or the correlation, desired shake parameters described throughout may be determined.

[0041] In some instances, an optical spray pattern may be measured or analyzed. Non-limiting examples of measuring an optical spray pattern of a spray may be as described in U.S. Patent Nos. 6,665,421 and 6,973,199, the disclosures of which are herein incorporated by reference in their entireties. For example, the methods herein may involve measuring an optical spray pattern of a spray by illuminating a spray plume with an illumination device (e.g., a laser), and then capturing an image of the spray plume with an imaging device (e.g., a camera).

[0042] Alternative methods of measuring or analyzing spray patterns as known in the art may be utilized. In some cases, impaction-based methods may be used. In one non-limiting example, the methods may involve firing the spray pump at a solid, thin-layer chromatography (TLC) plate having a coating that fluoresces in response to incident ultraviolet ("UV") radiation. The pattern of the spray deposited on the plate may then be analyzed.

[0043] In some aspects, the methods described herein involve performing a shaking regimen on the device, monitoring one or more spray parameters of the shaking regimen, and actuating the device when a predetermined threshold of the one or more spray parameters has been reached or exceeded. For example, if a shaking regimen included a shake duration of 5 seconds, a shake angle of 60 degrees, and a shake frequency of 2.0 Hz, the device would be actuated after all three shake parameters of the shaking regimen had been reached. In some cases, if one or more

of the shake parameters is not met before actuation of the device, the delivered dose of the drug may be different, in some cases substantially different, than the intended target dose.

[0044] In some aspects, the emitted dose of drug (e.g., after actuation of the device) is within about 15% of a target DCU performance of an inhaler or nasal device after performing the methods described herein. Dose content uniformity may refer to the uniformity of emitted drug per actuation, consistent with the label claim of the drug product. Thus, the methods herein provide for determining the DCU performance of an inhaler. The methods further provide for determining and/or selecting one or more shake parameters and/or one or more actuation parameters that are required to provide a DCU performance of an inhaler or nasal device product within about 15% of a target DCU performance. In some cases, the target DCU performance of an inhaler or nasal device is defined by regulatory or industry guidelines (e.g., by the U.S. Food and Drug Administration). In some cases, the emitted dose of drug is within about 25%, 24%, 23%, 22%, 21%, 20%, 19%, 18%, 17%, 16%, 15%, 14%, 13%, 12%, 11%, 10%, 9%, 8%, 7%, 6%, 5%, 4%, 3%, 2%, 1% or even identical to the target DCU performance of the inhaler.

[0045] In some embodiments, the methods include selecting one or more shake parameters and/or one or more actuation parameters for a specific inhaler or nasal device product such that the emitted dose of drug is within about 15% of a target DCU performance. In some aspects, the method is repeated one or more times (i.e., one or more of the shaking, monitoring, and actuating steps). In some cases, each emitted dose of drug is within about 15% of a target DCU performance of the inhaler. In some aspects, the method is performed in through-life testing of an inhaler or nasal device, for example, the device is tested at beginning-of-life (BoL), middle-of-life (MoL) and end-of-life (EoL). BoL administration may refer to actuating the device at the beginning of the labeled number of sprays (after any required priming sprays have been wasted, and usually within about the first 5% of the labeled number of sprays), MoL administration may refer to actuating the device at the middle of the labeled number of sprays (within about 45-55% of the labeled number of sprays), and EoL administration may refer to actuating the device at the end of the labeled number of sprays (within the last 95% of the labeled number of sprays). Generally, the shaking regimen, actuation parameters, or both are selected such that each emitted dose at BoL, MoL and EoL is within about 15% of a target DCU performance. Target DCU performance will be dependent on the target dose. The target dose is dependent on the product being tested.

[0046] In some cases, the spray pattern data may be used to determine the DCU performance of the inhaler. In some instances, the spray pattern data may be correlated with the DCU performance of the inhaler. In some examples, the spray pattern data may be performed in addition to, or as an alternative to, traditional DCU measurement techniques. In some

embodiments, the method herein involves alternating one or more rounds of spray pattern data analysis with one or more rounds of DUC performance measurement.

[0047] In one embodiment, the spray pattern area may be plotted relative to the shake parameters, actuation parameters, or both (for a non-limiting example, see **FIG. 1**). In some cases, dose content uniformity (DCU) performance of said inhaler or nasal device is determined based on said spray pattern by using a correlation, where such correlation may be derived from a suitably robust methodology involving experiment planning, data collection, data processing and statistical analysis of the data as may be described in the examples below, though other means of correlation could be implemented.

EXAMPLES

[0048] The following examples are given for the purpose of illustrating various embodiments of the invention and are not meant to limit the present invention in any fashion. The present examples, along with the methods described herein are presently representative of preferred embodiments, are exemplary, and are not intended as limitations on the scope of the invention. Changes therein and other uses which are encompassed within the spirit of the invention as defined by the scope of the claims will occur to those skilled in the art.

Example 1. Measuring the effects of shaking on pressurized metered dose inhaler (pMDI) performance

[0049] Introduction

[0050] The drive for an approved generic albuterol-based pMDI has significantly increased in recent years due to the cost barrier, patent expiration of reference products, and recently released draft FDA guidance documents. Product usage instructions for all of the current FDA approved albuterol pMDIs may only include non-descript language for shaking the pMDI such as "... shake well before each use..." with seldom indication for the patient regarding shaking duration, frequency, orientation, shake-to-fire interval, or what the effects might be if the patient doesn't shake the product before use. From a formulation perspective, shaking is critical for suspension pMDIs because the active drug particles in the formulation tend to rapidly sink or rise to the liquid surface due to differences in density or charge polarity from the propellants. Excipients, such as ethanol and oleic acid, are often added to suspension pMDI formulations to provide a more stable suspension of the active drug into the propellant.

[0051] Another factor that was used in selecting the particular albuterol pMDIs in this study is that patients are rarely prescribed just one inhaled medication. And since all of these products contain the same active ingredient, albuterol, a doctor/therapist could likely prescribe any of these products to a patient for the same indication thinking that the products are equivalent,

when they may not be due to their different excipients (among other physical differences) – and the effect of these differences may influence the performance of the product from a patient perspective. The implications of this type of patient confusion has been well documented in the respiratory literature.

[0052] Lastly, the in-vitro spray test methods required to show bioequivalence of pMDI products from a regulatory perspective, particularly dose content uniformity (DCU) and aerodynamic particle size distribution (APSD) through-life testing, are time intensive, complicated, and error-prone. Hence, a faster, more efficient, and less labor intensive performance indicating metric, such as optical spray pattern, would help relieve the testing/characterization burden for pMDI product development and help support the generation of more valuable DCU and APSD measurements.

[0053] Methods

[0054] Three different reference products containing albuterol sulfate were tested through life following a 3 variable, 3 level Box-Behnken Design of Experiments (“BB-DoE”) approach.

Table 1 below shows the derived control ranges employed to determine the effects of shaking (duration, angle, and frequency) on spray pattern in BB-DoE coded formats. Three canisters per product were tested using 13 variable shaking combinations that were inputted into Viota® software methods and executed using a SprayVIEW® measurement system SFpMDI (Proveris Scientific, Marlborough, MA U.S.A.).

[0055] Table 1. BB-DoE control variable ranges for tested shake parameters.

Control Variable	BB-DoE Value		
	-	0	+
Shake Frequency (Hz)	2.0	3.0	4.0
Shake Angle (deg)	60	90	120
Shake Duration (s)	5	10	15

[0056] Using the same shaking regime for each product, an experiment alternating actuations for spray pattern and DCU collection was designed to see if optical spray pattern and DCU are statistically correlated. This study involved collecting ten actuations each at the beginning, middle, and end of life on three (3) cans for each product. Additionally, a DCU through-life experiment was conducted for the product with no excipients using a “shake vs. no shake” comparison where the “shake” parameters were derived from the optical spray pattern DoE results. In these studies, each DCU sample was collected following the protocol outlined in the United States Pharmacopeia using an alternative dose uniformity sampling apparatus and

quantified using a spectrophotometric method (ThermoFisher GENESYS 10S UV-Vis Spectrophotometer). Alternatively, other appropriate measurement methodologies may be used (e.g., high performance liquid chromatography).

[0057] Results

[0058] The consolidated results from the multi-dimensional spray pattern DoE are shown in **FIG. 1**. Briefly, **FIG. 1** depicts a “sensitivity plot” of the spray pattern area plotted against the shaking parameters for each pMDI product (indicated by the number of excipients where Product A had no excipients, Product B had 1 excipient, and Product C had 2 excipients). **Table 2** below summarizes the sensitivity analysis in simple “yes” or “no” terms based on statistical p-value analysis.

[0059] **Table 2. Simplified optical spray pattern area sensitivity results.**

Number of excipients	Shake Angle	Shake Frequency	Shake Duration
0	No	No	Yes
1	Yes	No	No
2	No	No	No

[0060] The results clearly indicate that the products produce vastly different sized spray patterns under identical test conditions with Product A producing the smallest patterns (mean value of about 132 mm²) and Product C producing the largest (mean value of about 350 mm²). The results also indicate that Product A has acute sensitivity to shake duration (about a 20% change in spray pattern area when the device was shaken before each actuation for 5 seconds compared to 15 seconds), while Product B has some sensitivity to shake angle. This result is significant since shake duration is not indicated in any of the product’s respective patient usage instructions. Product C seems immune to shaking within the tested range. However, this product did exhibit substantially more shot-shot variation than the others and this variation may be masking the product’s true sensitivity.

[0061] Results from DCU through-life testing of Product A (no excipients) are shown in **FIG. 2** and **FIG. 3** where “no shake” indicates that the product samples were not shaken at any point during the experiments; and “shake” indicates that the product samples were shaken with set parameters (10 second duration, 60 degree angle, and 4 Hz frequency) prior to automated actuation. In all cases the product samples were allowed to rest for 3 minutes (180 seconds) between consecutive automated actuations.

[0062] The results show a startling effect of not shaking the product on DCU performance: the emitted dose during beginning of life is considerably variable and nearly three times the target

value (108 mcg) before it starts to taper off at the middle and end of life stages. However, since so much excess drug was emitted during BoL, the EoL performance shows only about 25% of the target dose is being delivered as shown in **FIG. 3**. In contrast, the “shake” data indicates very consistent and very near target DCU performance from the product at all life stages.

[0063] Conclusions

[0064] The DCU and optical spray pattern performance of three different commercially available albuterol pMDI products were shown to have markedly different sensitivities to shaking. The product with no added excipients produced the smallest optical spray patterns and was sensitive to shake duration – a parameter not included in any of the product’s patient usage instructions. Additionally, the effects of not shaking the product without excipients were profound – nearly 3 times the target DCU was measured at the beginning of life which resulted in only about 25% of the target dose being delivered at the end of life. Current patient instructions for the respective products do not include specified guidelines on shaking (particularly shake duration) or the effects of not shaking the product, which were shown here to be rather profound with respect to DCU on one product. However, by providing more defined instructions on how to shake and the importance of shaking, patient confusion could be reduced and more effective patient usage could occur.

[0065] While preferred embodiments of the present invention have been shown and described herein, it will be obvious to those skilled in the art that such embodiments are provided by way of example only. Numerous variations, changes, and substitutions will now occur to those skilled in the art without departing from the invention. It should be understood that various alternatives to the embodiments of the invention described herein may be employed in practicing the invention. It is intended that the following claims define the scope of the invention and that methods and structures within the scope of these claims and their equivalents be covered thereby.

CLAIMS

WHAT IS CLAIMED IS:

1. A method of measuring performance of an inhaler or nasal device comprising a drug formulation, the method comprising:
 - a) shaking said inhaler or nasal device, wherein said shaking comprises one or more shake parameters;
 - b) actuating said inhaler or nasal device, thereby emitting a spray of said drug formulation; and
 - c) measuring a spray pattern of said spray of said drug formulation,wherein said spray of said drug formulation comprises an emitted dose of a drug, and wherein dose content uniformity (DCU) performance of said inhaler or nasal device is determined based on said spray pattern.
2. The method of claim 1, wherein said inhaler or nasal device is selected from the group consisting of: a pressurized metered dose inhaler (pMDI), a metered dose inhaler (MDI), and a nasal spray.
3. The method of claim 1 or 2, wherein said one or more shake parameters comprises one or more of shake frequency, shake angle, shake duration, shake-to-fire interval and shake orientation.
4. The method of claim 3, wherein said shake frequency comprises about 1.0 Hz to about 4.0 Hz.
5. The method of claim 3 or 4, wherein said shake angle comprises about 30 degrees to about 180 degrees.
6. The method of any one of claims 3-5, wherein said shake duration comprises about 2 seconds to about 15 seconds.
7. The method of any one of claims 3-6, wherein said shake-to-fire interval comprises about 0 seconds to about 10 seconds.
8. The method of any one of claims 3-7, wherein said shake orientation comprises about 0 degrees to about 359 degrees.
9. The method of any one of claims 1-8, wherein said drug formulation comprises a suspension formulation.
10. The method of any one of claims 1-9, wherein said drug formulation comprises one or more excipients.
11. The method of any one of claims 1-10, wherein said drug formulation comprises no excipients.

12. The method of any one of claims 1-11, further comprising, prior to b), monitoring said one or more shake parameters.

13. The method of any one of claims 1-12, wherein b) comprises actuating said inhaler or nasal device when said one or more shake parameters have reached or have exceeded a predetermined threshold.

14. The method of claim 13, wherein said predetermined threshold is determined by a composition of said drug formulation.

15. The method of any one of claims 1-14, wherein said method is performed on said inhaler or nasal device during beginning-of-life administration, middle-of-life administration, end-of-life administration or any combination thereof.

16. The method of any one of claims 1-15, wherein said spray pattern is an optical spray pattern.

17. The method of any one of claims 1-16, wherein c) further comprises illuminating said spray with an illumination device and imaging said optical spray pattern with an imaging device.

18. The method of any one of claims 1-17, wherein said spray pattern is an impaction-based spray pattern.

19. The method of any one of claims 1-18, wherein said spray pattern is presented on a report.

20. The method of claim 19, wherein said spray pattern is represented on said report as a sensitivity plot.

21. The method of claim 20, wherein said sensitivity plot is plotted as a spray pattern area as a function of said one or more shake parameters.

22. The method of any one of claims 1-21, wherein said actuating comprises a length of time a valve of said inhaler or nasal device is left open by said actuating.

23. The method of any one of claims 1-22, wherein said actuating comprises compressing said inhaler or nasal device.

24. The method of claim 23, wherein said compressing comprises a stroke length.

25. The method of claim 24, wherein said stroke length comprises about 1 millimeter to about 200 millimeters.

26. A method of testing for delivery of a drug formulation with an inhaler or nasal device, the method comprising:

a) monitoring two or more shake parameters; and

b) actuating said inhaler or nasal device when a predetermined threshold of said two or more shake parameters is reached or exceeded, thereby emitting a spray of said drug formulation,

wherein said spray of said drug formulation comprises an emitted dose of a drug.

27. The method of claim 26, wherein said emitted dose of a drug is within about 15% of a target dose content uniformity (DCU) performance.

28. The method of claim 27, wherein said target DCU performance is defined by regulatory or industry guidelines.

29. The method of any one of claims 26-28, further comprising repeating said monitoring and actuating one or more times, thereby emitting one or more additional sprays of said drug formulation, wherein each of said one or more additional sprays comprises an emitted dose of said drug.

30. The method of claim 29, wherein each of said one or more additional sprays comprises an emitted dose of said drug within about 15% of said target DCU performance.

31. The method of any one of claims 26-30, wherein said two or more shake parameters are selected from the group consisting of: shake duration, shake frequency, shake angle, shake-to-fire interval, and shake orientation.

32. The method of any one of claims 26-31, further comprising, prior to a), shaking said inhaler or nasal device.

33. The method of claim 31 or 32, wherein said shake duration comprises about 2 seconds to about 15 seconds.

34. The method of any one of claims 31-33, wherein said shake angle comprises about 30 degrees to about 180 degrees.

35. The method of any one of claims 31-34, wherein said shake frequency comprises about 1.0 Hz to about 4.0 Hz.

36. The method of any one of claims 31-35, wherein said shake-to-fire interval comprises about 0 seconds to about 10 seconds.

37. The method of any one of claims 31-36, wherein said shake orientation comprises about 0 degrees to about 359 degrees.

38. The method of any one of claims 26-37, wherein said monitoring comprises measuring said two or more shake parameters.

39. The method of any one of claims 26-38, wherein said drug formulation comprises one or more excipients.

40. The method of any one of claims 26-39, wherein said drug formulation comprises no excipients.

41. The method of claim 39, wherein said predetermined threshold is determined based on (i) a number of said one or more excipients present in said drug formulation, (ii) a composition of said one or more excipients present in said drug formulation, or (iii) a combination of both.

42. The method of claim 29, wherein each of said one or more additional sprays comprises an emitted dose of said drug within about 15% of said target DCU performance at each of beginning-of-life administration, middle-of-life administration and end-of-life administration.

43. The method of any one of claims 26-42, further comprising administering said emitted dose of a drug to a patient in need thereof.

44. The method of any one of claims 26-43, further comprising, after said actuating, performing a spray pattern analysis on said spray.

45. The method of claim 44, further comprising, determining an amount of said emitted dose of a drug from said spray pattern analysis.

46. The method of claim 44, wherein performing said spray pattern analysis comprises measuring an optical spray pattern of said spray.

47. The method of claim 46, wherein measuring said optical spray pattern of said spray comprises illuminating said spray with an illumination device and imaging said optical spray pattern with an imaging device.

48. The method of claim 44, wherein performing said spray pattern analysis comprises measuring an impaction-based spray pattern of said spray.

49. The method of any one of claims 26-48, wherein said inhaler or nasal device is selected from the group consisting of: a pressurized metered dose inhaler (pMDI), a metered dose inhaler (MDI), and a nasal spray.

50. The method of any one of claims 26-49, wherein said drug formulation comprises a suspension formulation.

51. The method of any one of claims 44-50, wherein said spray pattern analysis is presented on a report.

52. The method of claim 51, wherein said spray pattern analysis is represented on said report as a sensitivity plot.

53. The method of claim 52, wherein said sensitivity plot is plotted as a spray pattern area as a function of at least one of said two or more shake parameters.

54. The method of any one of claims 26-53, wherein said actuating comprises a length of time a valve of said inhaler or nasal device is left open by said actuating.

55. The method of any one of claims 26-54, wherein said actuating comprises compressing said inhaler or nasal device.

56. The method of claim 55, wherein said compressing comprises a stroke length.

57. The method of claim 56, wherein said stroke length comprises about 1 millimeter to about 200 millimeters.

58. A method of testing for delivery of a drug formulation with an inhaler or nasal device, the method comprising:

a) monitoring one or more shake parameters, wherein at least one of said one or more shake parameters comprises shake angle, shake frequency, shake-to-fire interval, or shake orientation; and

b) actuating said inhaler or nasal device when a predetermined threshold of said one or more shake parameters is reached or exceeded, thereby emitting a spray of said drug formulation,

wherein said spray of said drug formulation comprises an emitted dose of a drug.

59. The method of claim 58, wherein said emitted dose of a drug is within about 15% of a target dose content uniformity (DCU) performance.

60. The method of claim 59, wherein said target DCU performance is defined by regulatory or industry guidelines.

61. The method of any one of claims 58-60, further comprising repeating said monitoring and actuating one or more times, thereby emitting one or more additional sprays of said drug formulation, wherein each of said one or more additional sprays comprises an emitted dose of said drug.

62. The method of claim 61, wherein each of said one or more additional sprays comprises an emitted dose of said drug within about 15% of said target DCU performance.

63. The method of any one of claims 58-62, wherein said one or more shake parameters further comprises shake duration.

64. The method of any one of claims 58-63, further comprising, prior to said monitoring, shaking said inhaler or nasal device.

65. The method of claim 63, wherein said shake duration comprises about 2 seconds to about 15 seconds.

66. The method of any one of claims 58-65, wherein said shake angle comprises about 30 degrees to about 180 degrees.

67. The method of any one of claims 58-66, wherein said shake frequency comprises about 1.0 Hz to about 4.0 Hz.

68. The method of any one of claims 58-67, wherein said shake-to-fire interval comprises about 0 seconds to about 10 seconds.

69. The method of any one of claims 58-68, wherein said shake orientation comprises about 0 degrees to about 359 degrees.

70. The method of any one of claims 58-69, wherein said monitoring comprises measuring said one or more shake parameters.

71. The method of any one of claims 58-70, wherein said drug formulation comprises one or more excipients.

72. The method of any one of claims 58-71, wherein said drug formulation comprises no excipients.

73. The method of claim 71, wherein said predetermined threshold is determined based on (i) a number of said one or more excipients present in said drug formulation, (ii) a composition of said one or more excipients present in said drug formulation, or (iii) a combination of both.

74. The method of claim 61, wherein each of said one or more additional sprays comprises an emitted dose of said drug within about 15% of said target DCU performance at each of beginning-of-life administration, middle-of-life administration and end-of-life administration.

75. The method of any one of claims 58-74, further comprising administering said emitted dose of a drug to a patient in need thereof.

76. The method of any one of claim 58-75, further comprising, after said actuating, performing a spray pattern analysis on said spray.

77. The method of claim 76, further comprising, determining an amount of said emitted dose of a drug from said spray pattern analysis.

78. The method of claim 76 or 77, wherein performing said spray pattern analysis comprises measuring an optical spray pattern of said spray.

79. The method of claim 78, wherein measuring said optical spray pattern of said spray comprises illuminating said spray with an illumination device and imaging said optical spray pattern with an imaging device.

80. The method of claim 76, wherein performing said spray pattern analysis comprises measuring an impaction-based spray pattern of said spray.

81. The method of any one of claims 58-80, wherein said inhaler or nasal device is selected from the group consisting of: a pressurized metered dose inhaler (pMDI), a metered dose inhaler (MDI), and a nasal spray.

82. The method of any one of claims 58-81, wherein said drug formulation comprises a suspension formulation.

83. The method of any one of claims 76-82, wherein said spray pattern analysis is presented on a report.

84. The method of claim 83, wherein said spray pattern analysis is represented on said report as a sensitivity plot.

85. The method of claim 84, wherein said sensitivity plot is plotted as a spray pattern area as a function of said one or more shake parameters.

86. The method of any one of claims 58-85, wherein said actuating comprises a length of time a valve of said inhaler or nasal device is left open by said actuating.

87. The method of any one of claims 58-86, wherein said actuating comprises compressing said inhaler or nasal device.

88. The method of claim 87, wherein said compressing comprises a stroke length.

89. The method of claim 88, wherein said stroke length comprises about 1 millimeter to about 200 millimeters.

1/3

FIG. 1

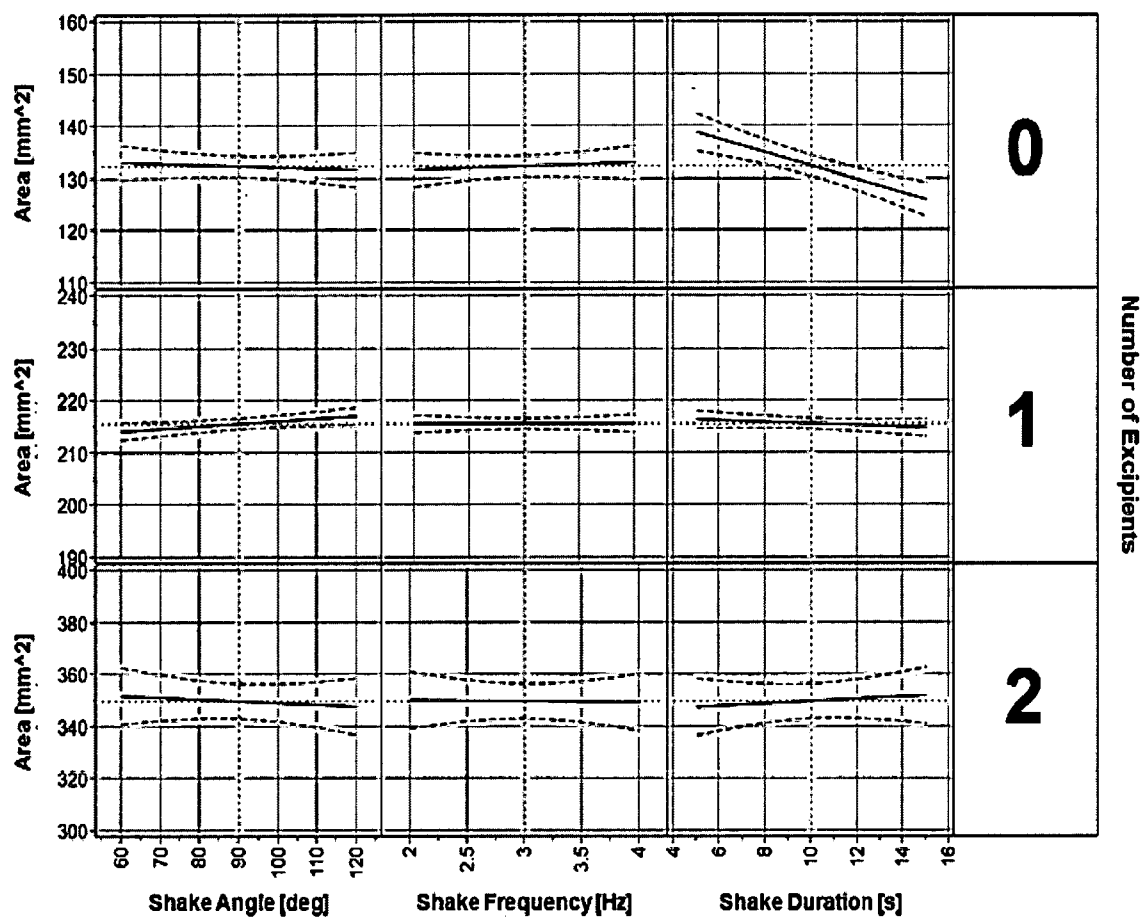


FIG. 2


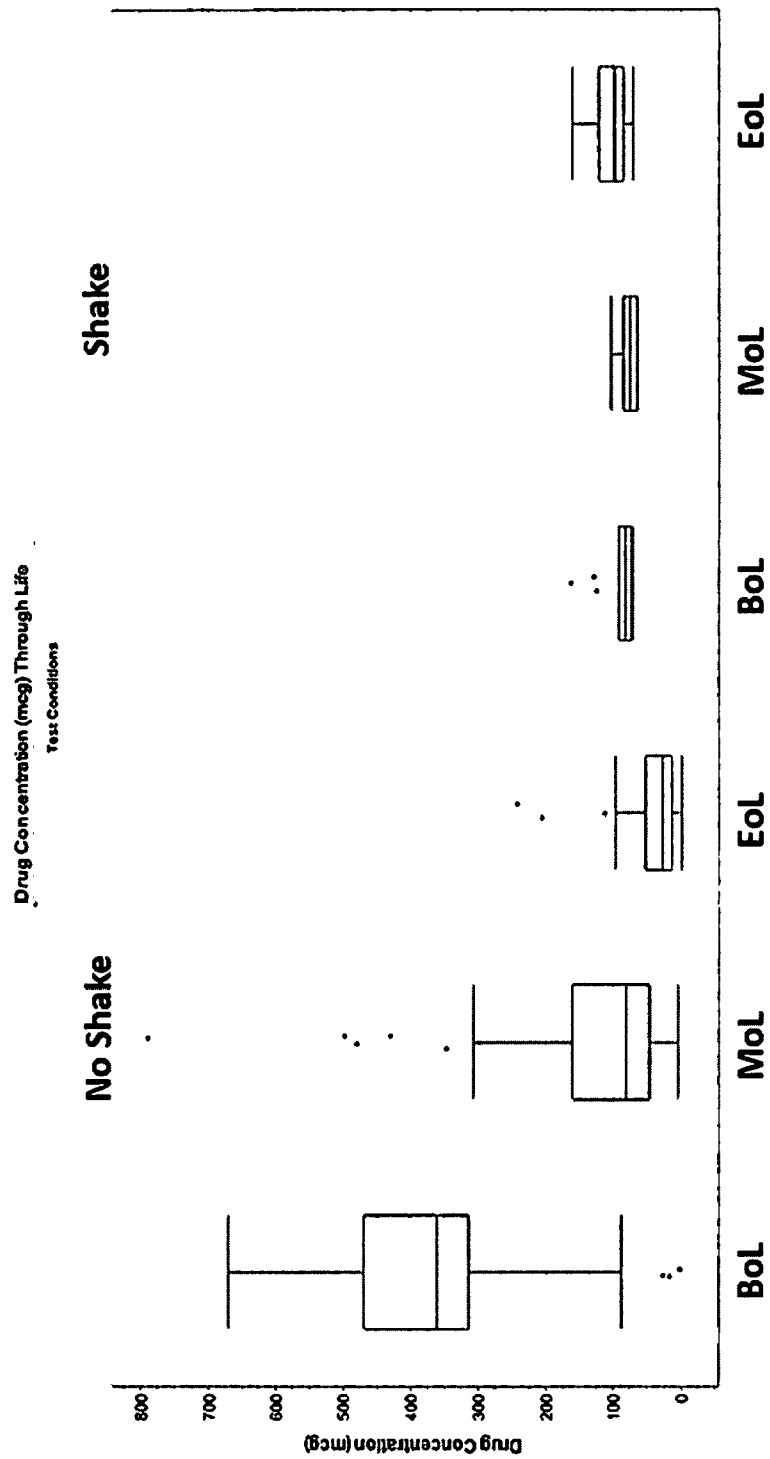


FIG. 3

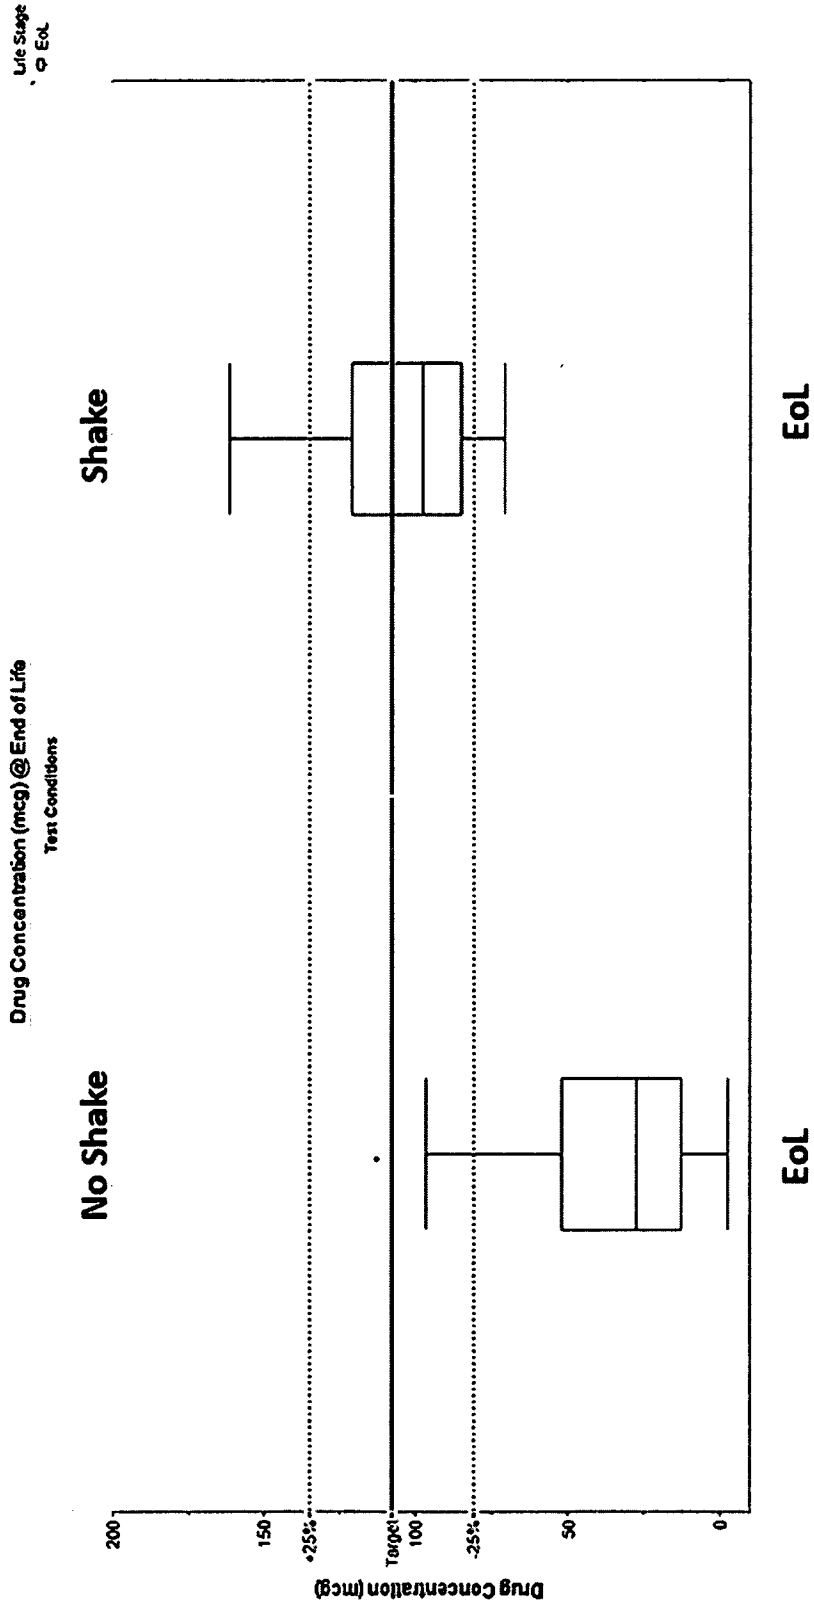

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US17/21599

A. CLASSIFICATION OF SUBJECT MATTER

IPC - A61M11/00, A61M15/00, A61M15/08 (2017.01)

CPC - A61M11/00, A61M15/00, A61M15/0005, A61M15/009, A61M15/0065, A61M15/08

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

See Search History document

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

See Search History document

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

See Search History document

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5,676,129 A (ROCCI, Jr., M et al.) 14 October 1997; column 1, lines 60-67; column 4, lines 51-67; column 8, lines 28-67	26, 29/26
Y		27, 28, 29/27, 29/28, 30
X	US 2008/0173067 A1 (FARINA, D et al.) 24 July 2008; paragraphs 42-43, 74, 77, 81-84, 113-115, 117	58, 61/58
Y		59, 60, 61/59, 61/60, 62
Y	US 2015/0157566 A1 (HANMI PHARM. CO., LTD.) 11 June 2015; paragraphs 19, 53, 69-70	27, 28, 29/27, 29/28, 30, 59, 60, 61/59, 61/60, 62
A	US 2006/0140873 A1 (CHANG, H) 29 June 2006; paragraphs 16, 22-23	1-4
A	US 2005/0147565 A1 (SEQUEIRA, J et al.) 7 July 2005; paragraphs 33, 56, 67-70	1-4



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T"

later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X"

document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y"

document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&"

document member of the same patent family

Date of the actual completion of the international search

15 May 2017 (15.05.2017)

Date of mailing of the international search report

01 JUN 2017

Name and mailing address of the ISA/

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-8300

Authorized officer

Shane Thomas

PCT Helpdesk: 571-272-4300
PCT OSP: 571-272-7774

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US17/21599

Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:

2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:

3. ☒ Claims Nos.: 5-25, 31-57, 63-89
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying additional fees, this Authority did not invite payment of additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:

4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.