



US00D947918S

(12) **United States Design Patent**
Matuschek et al.

(10) **Patent No.:** **US D947,918 S**

(45) **Date of Patent:** **** Apr. 5, 2022**

(54) **SURGICAL MICROSCOPE WITH STAND**

(71) Applicant: **Carl Zeiss Meditec AG**, Jena (DE)

(72) Inventors: **Walter Matuschek**, Aalen (DE);
Christian Siegel, Aalen (DE)

(73) Assignee: **Carl Zeiss Meditec AG**, Jena (DE)

(**) Term: **15 Years**

(21) Appl. No.: **29/684,037**

(22) Filed: **Mar. 18, 2019**

(30) **Foreign Application Priority Data**

Sep. 18, 2018 (EM) 005647054

(51) **LOC (13) Cl.** **16-06**

(52) **U.S. Cl.**
USPC **D16/131**

(58) **Field of Classification Search**
USPC D16/130–136; D24/107, 128, 137, 138,
D24/185, 186, 232, 234
CPC G02B 21/00; G02B 21/002; G02B 21/06;
G02B 21/082
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

6,471,165	B2 *	10/2002	Twisselmann		F16M 11/18 248/123.11
D482,708	S *	11/2003	Matuschek		D16/131
D623,210	S *	9/2010	Matuschek		D16/131
D626,236	S *	10/2010	Ninomiya		D24/185
D634,344	S *	3/2011	Nusser		D16/131
D649,992	S *	12/2011	Nusser		D16/131
D650,405	S *	12/2011	Nusser		D16/131
D666,653	S *	9/2012	Nusser		D16/131
D707,359	S *	6/2014	Kim		D24/185
D707,360	S *	6/2014	Kim		D24/185
D716,448	S *	10/2014	Kim		D24/158

D751,209	S *	3/2016	DiMino		D24/186
D758,465	S *	6/2016	Matuschek		D16/131
D836,692	S *	12/2018	Matuschek		D16/131
D836,693	S *	12/2018	Matuschek		D16/131
D837,856	S *	1/2019	Matuschek		D16/131
D841,070	S *	2/2019	Matuschek		D16/131
D874,657	S *	2/2020	Bailey		D24/185

(Continued)

OTHER PUBLICATIONS

Dari Zeiss Meditec AG brochure “OPMI Lumera 700 from ZEISS”,
2014, 14 pages.

(Continued)

Primary Examiner — Holly E Thurman

(74) *Attorney, Agent, or Firm* — Walter Ottesen, P.A.

(57) **CLAIM**

The ornamental design for a surgical microscope with stand,
as shown and described.

DESCRIPTION

FIG. 1 is a first perspective view of the surgical microscope
with stand of our new design;

FIG. 2 is a second perspective view of the surgical micro-
scope with stand of FIG. 1;

FIG. 3 is a rear elevation view of the surgical microscope
with stand of FIG. 1;

FIG. 4 is a front elevation view of the surgical microscope
with stand of FIG. 1;

FIG. 5 is a top plan view of the surgical microscope with
stand of FIG. 1;


FIG. 6 is a bottom plan view of the surgical microscope with
stand of FIG. 1;

FIG. 7 is a right side elevation view of the surgical micro-
scope with stand of FIG. 1; and,

FIG. 8 is a left side elevation view of the surgical micro-
scope with stand of FIG. 1.

The broken lines form no part of the claimed design.

1 Claim, 8 Drawing Sheets

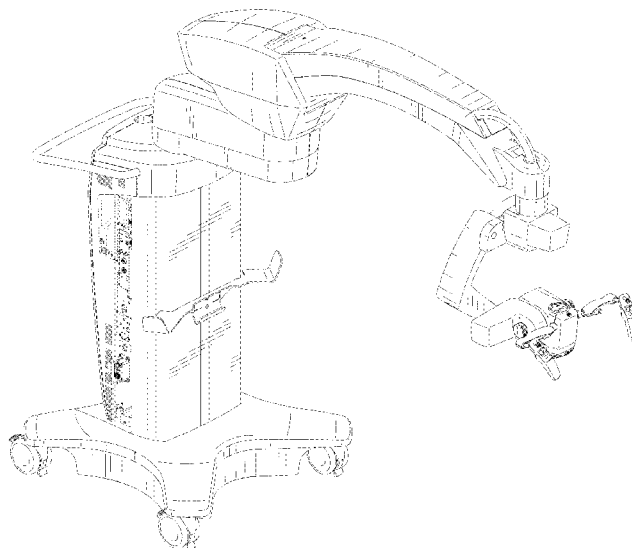

(56)

References Cited

U.S. PATENT DOCUMENTS

D881,963	S	*	4/2020	Liu		D16/131
D881,964	S	*	4/2020	Liu		D16/131
D881,965	S	*	4/2020	Liu		D16/131
2003/0230698	A1	*	12/2003	Strauss		F21V 21/06 248/648
2005/0041282	A1	*	2/2005	Rudolph		G02B 7/001 359/368

OTHER PUBLICATIONS

Dari Zeiss Meditec AG brochure “OPMI Vario from ZEISS”, 2014, 12 pages.
 Dari Zeiss Meditec AG brochure “OPMI Pentero 800 from ZEISS”, 2015, 7 pages.
 Dari Zeiss Meditec AG brochure “KINEVO 900 von ZEISS”, 2017, 22 pages.
 U.S. Appl. No. 29/684,005, filed Mar. 18, 2019, Carl Zeiss Meditec AG, Walter Matuschek Christian Siegel.
 U.S. Appl. No. 29/684,045, filed Mar. 18, 2019, Carl Zeiss Meditec AG, Walter Matuschek Christian Siegel.
 U.S. Appl. No. 29/684,052, filed Mar. 18, 2019, Carl Zeiss Meditec AG, Walter Matuschek Christian Siegel.

* cited by examiner

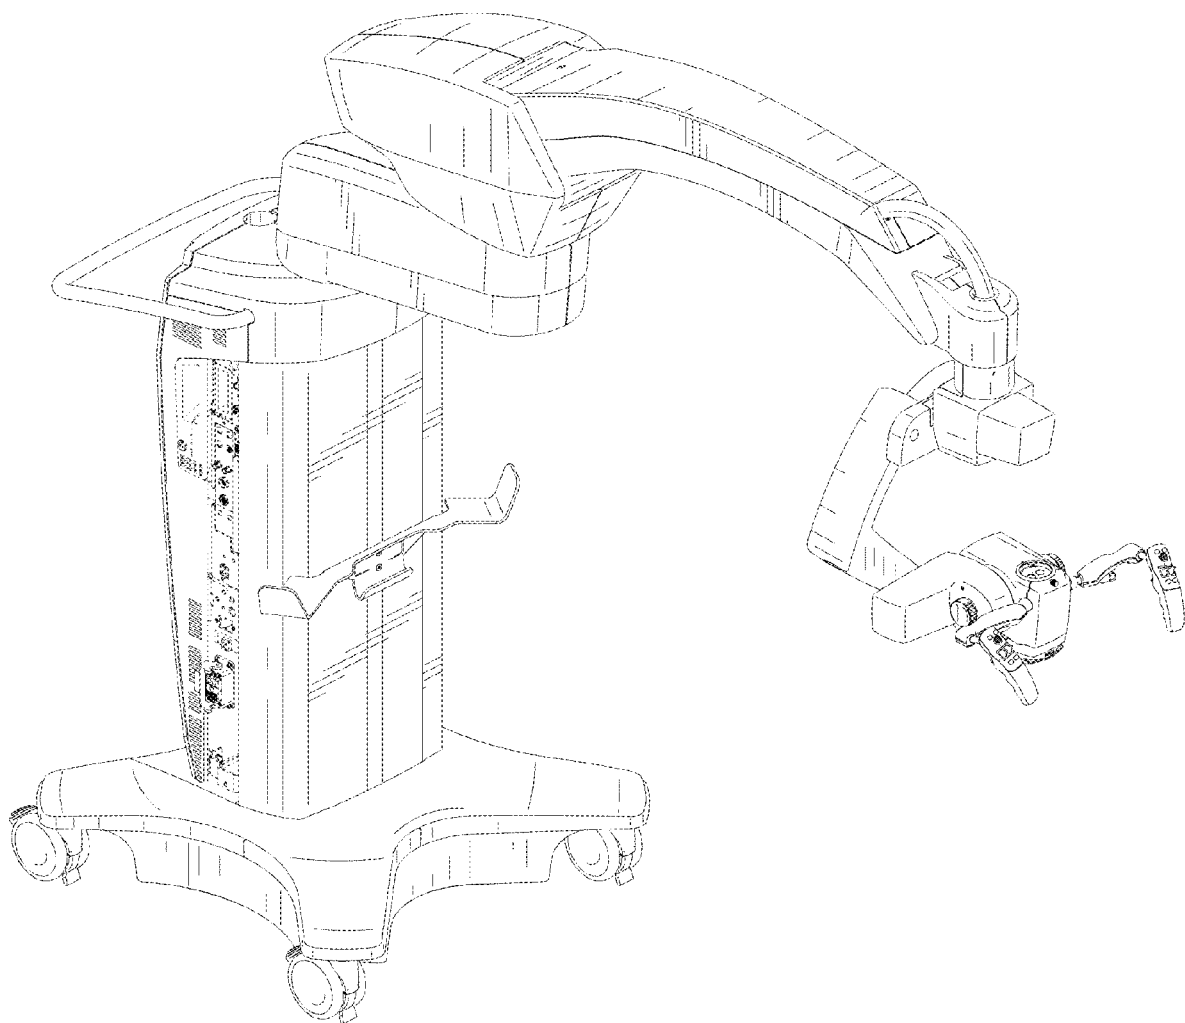


FIG. 1

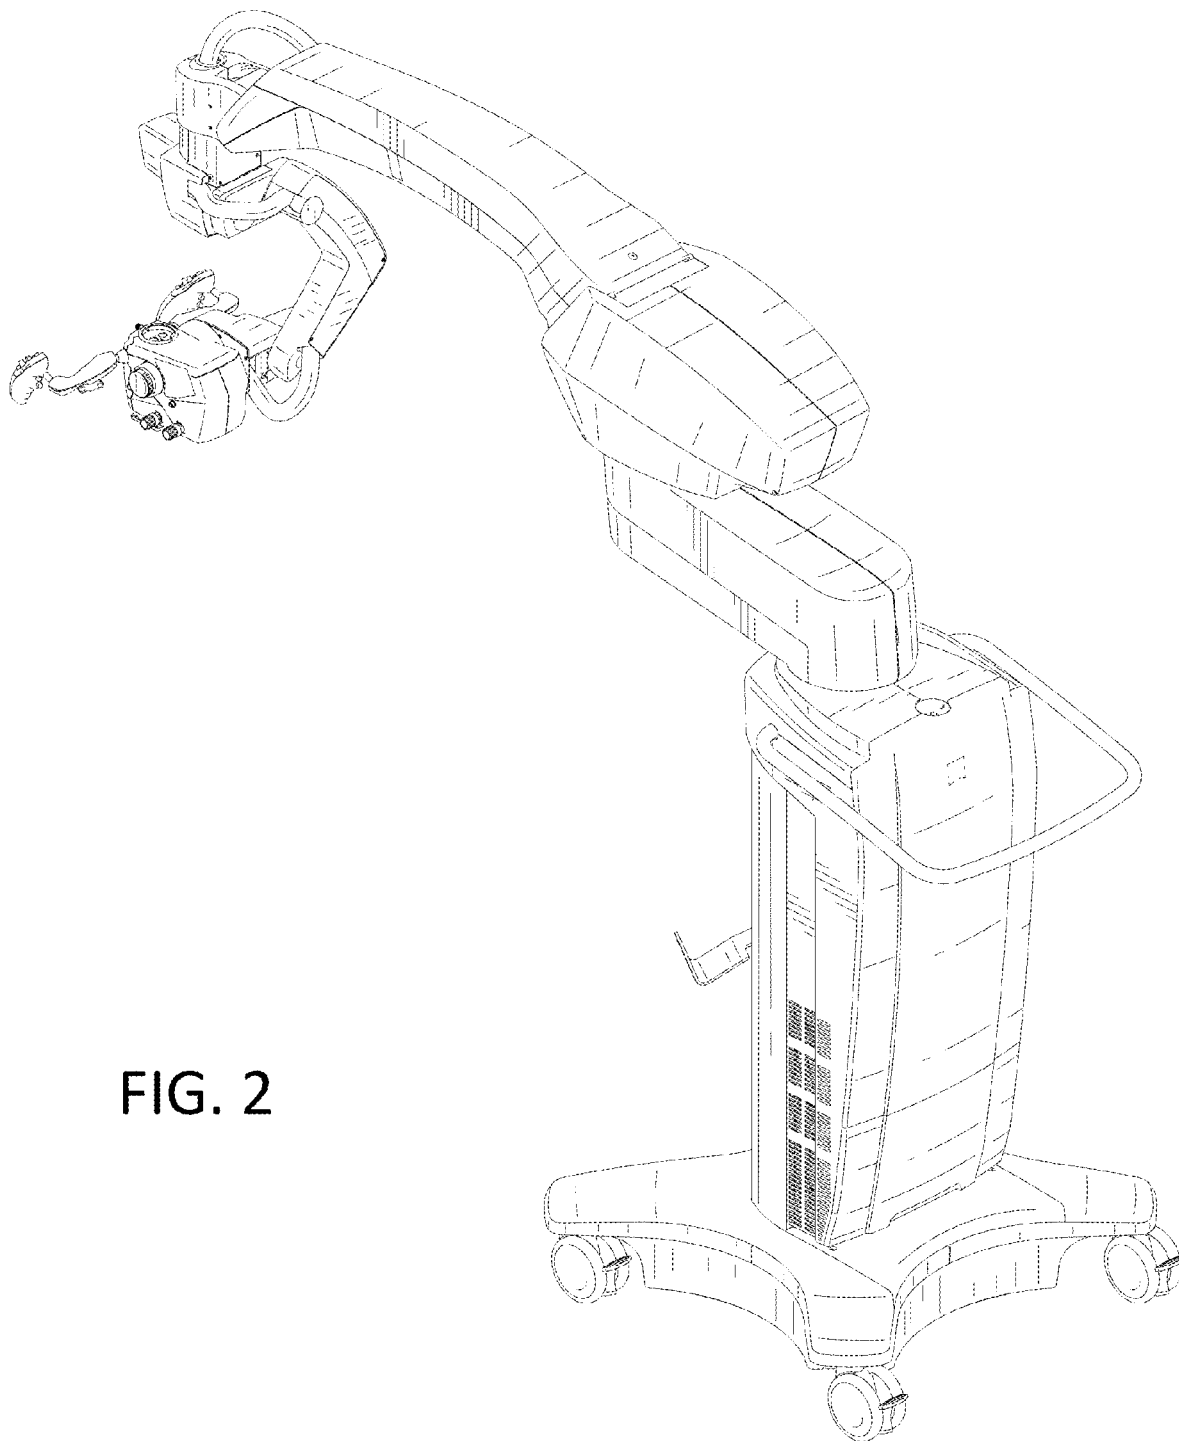


FIG. 2

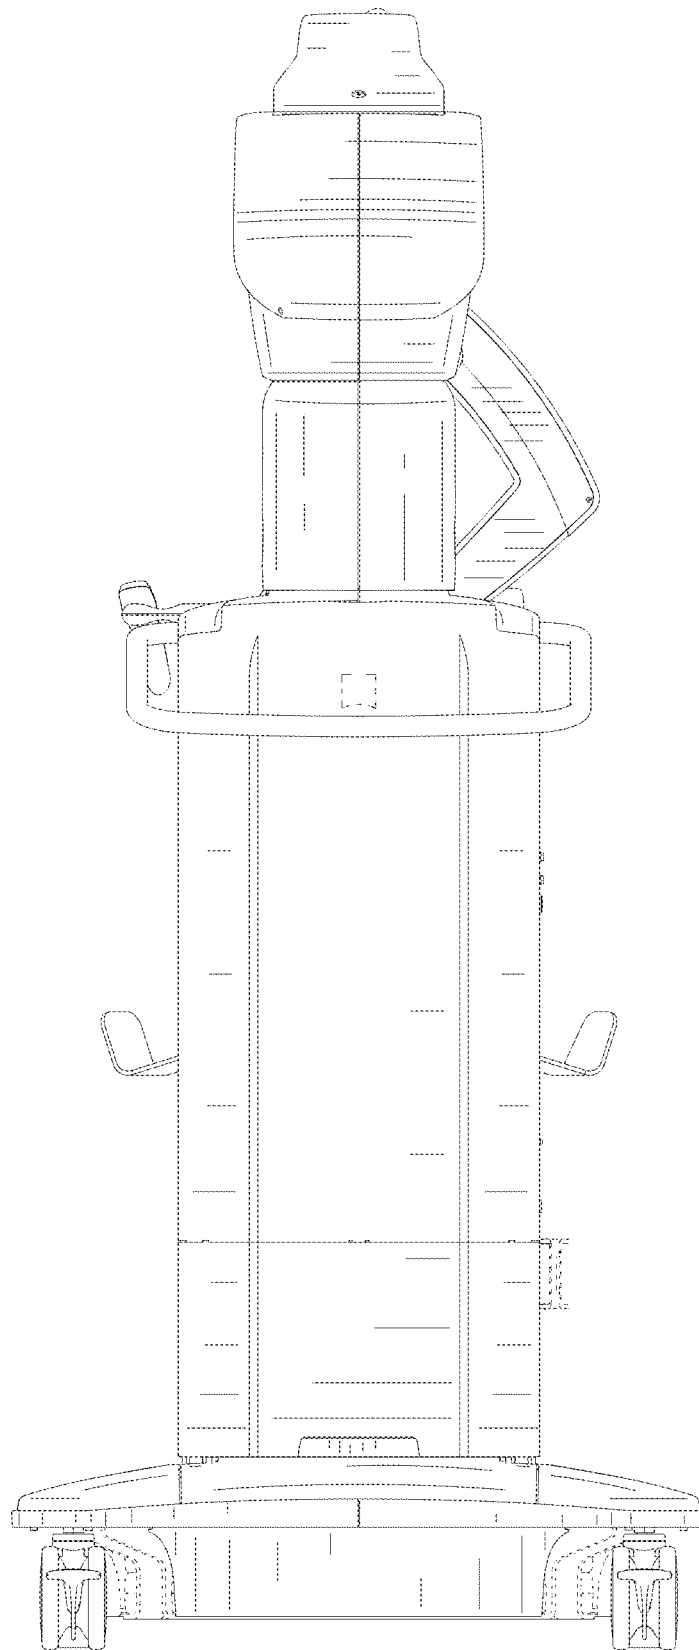


FIG. 3

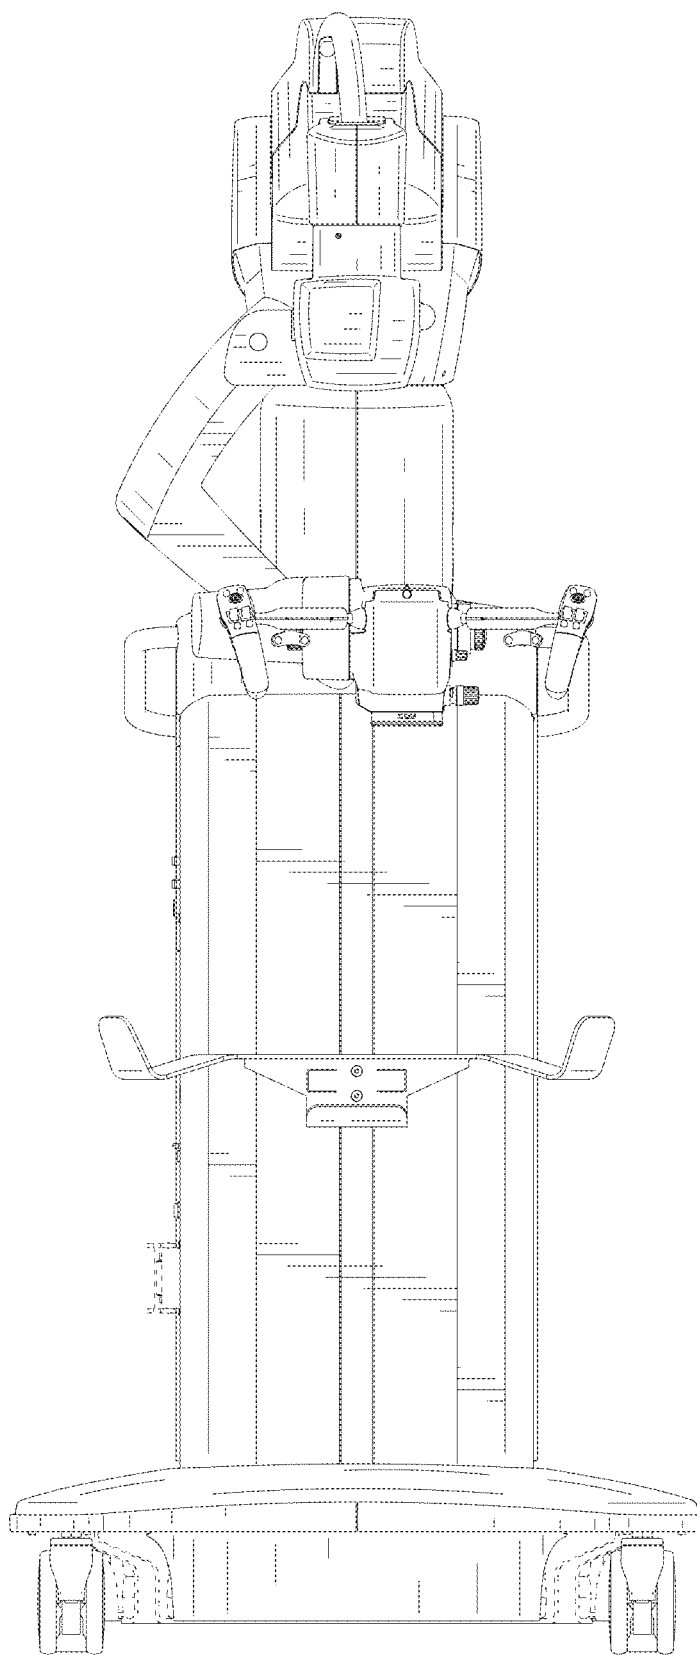


FIG. 4

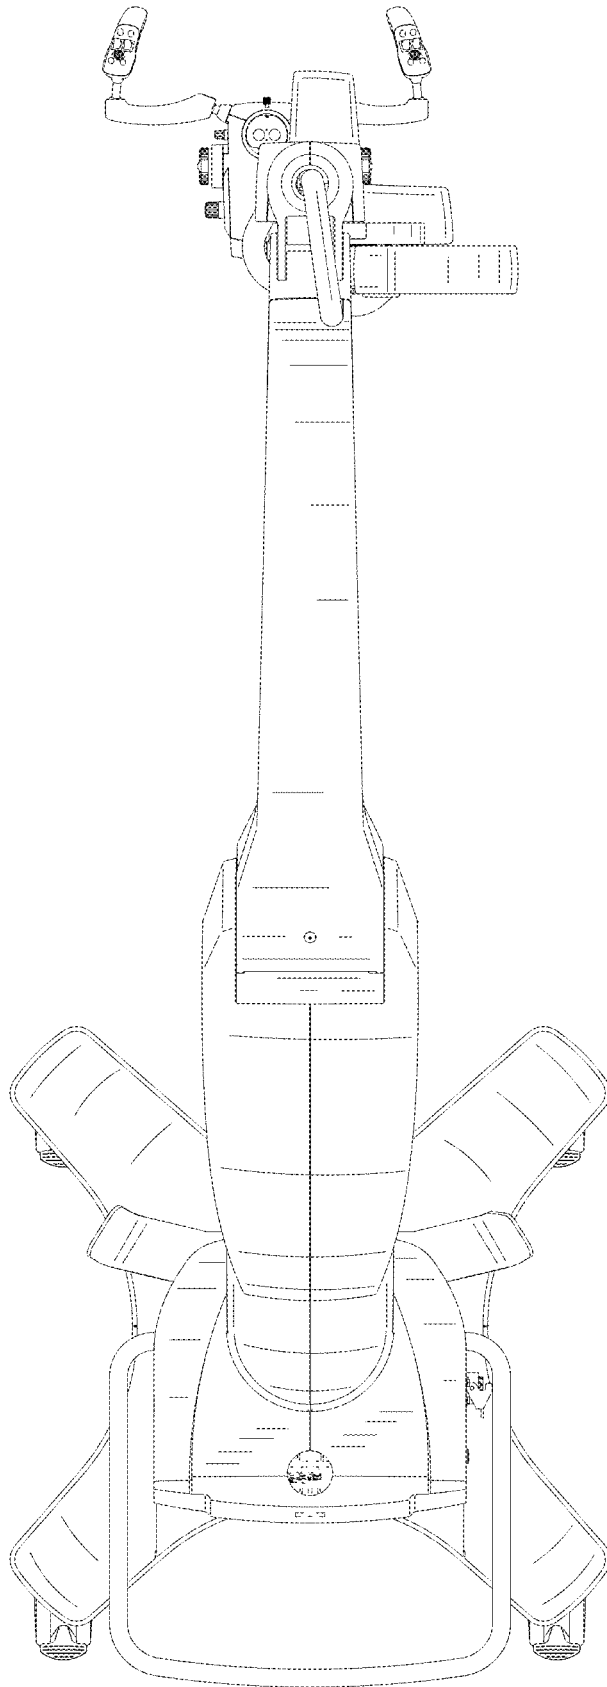


FIG. 5

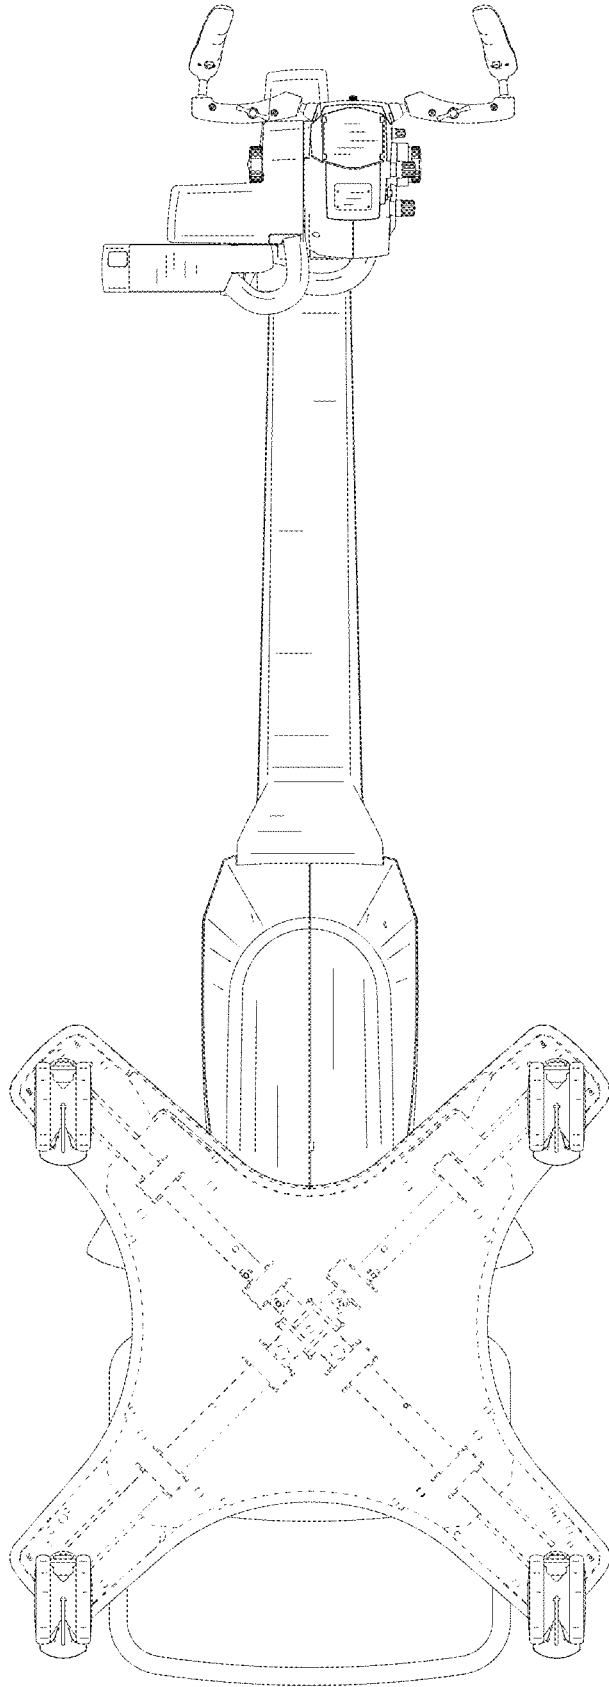


FIG. 6

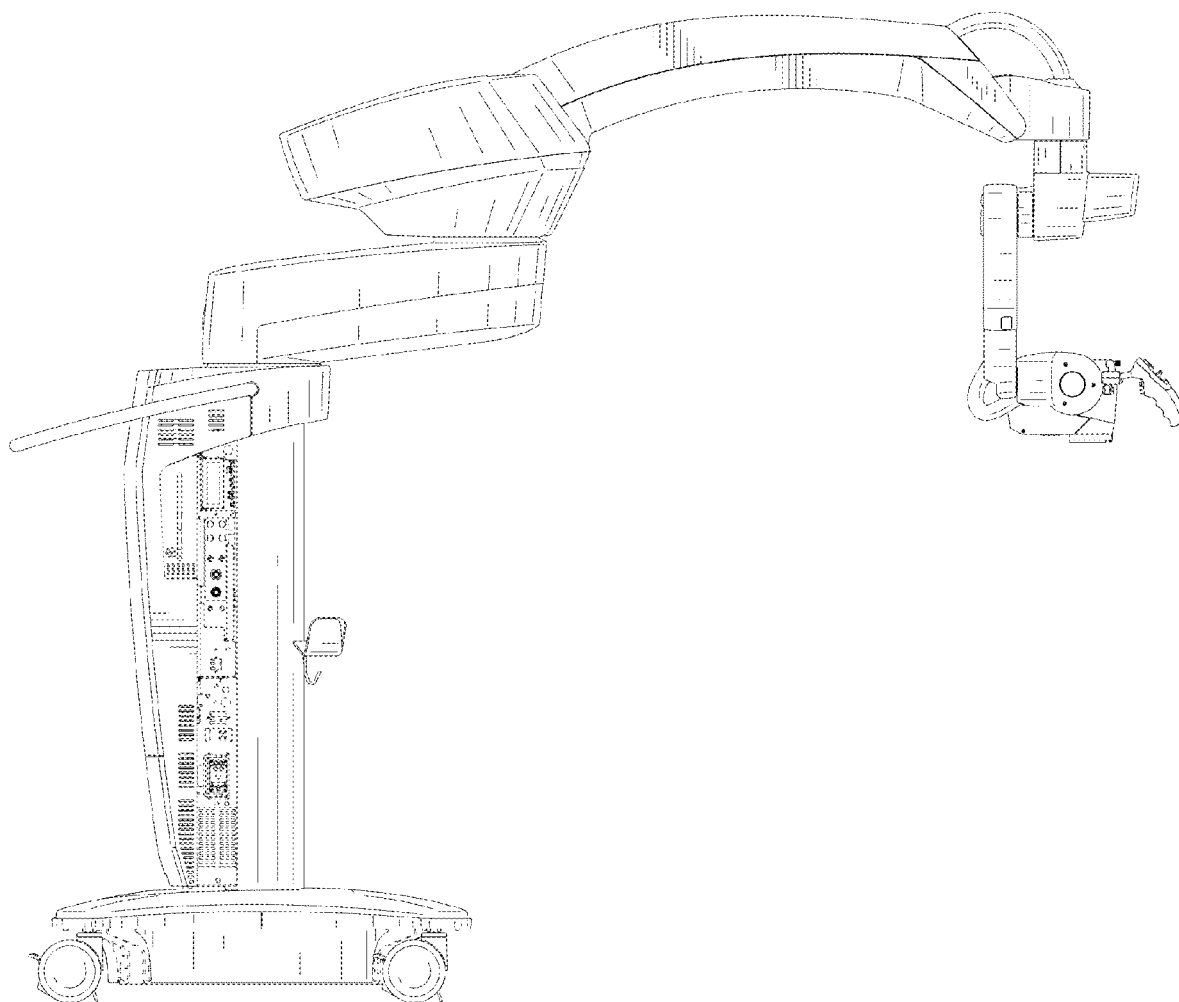


FIG. 7

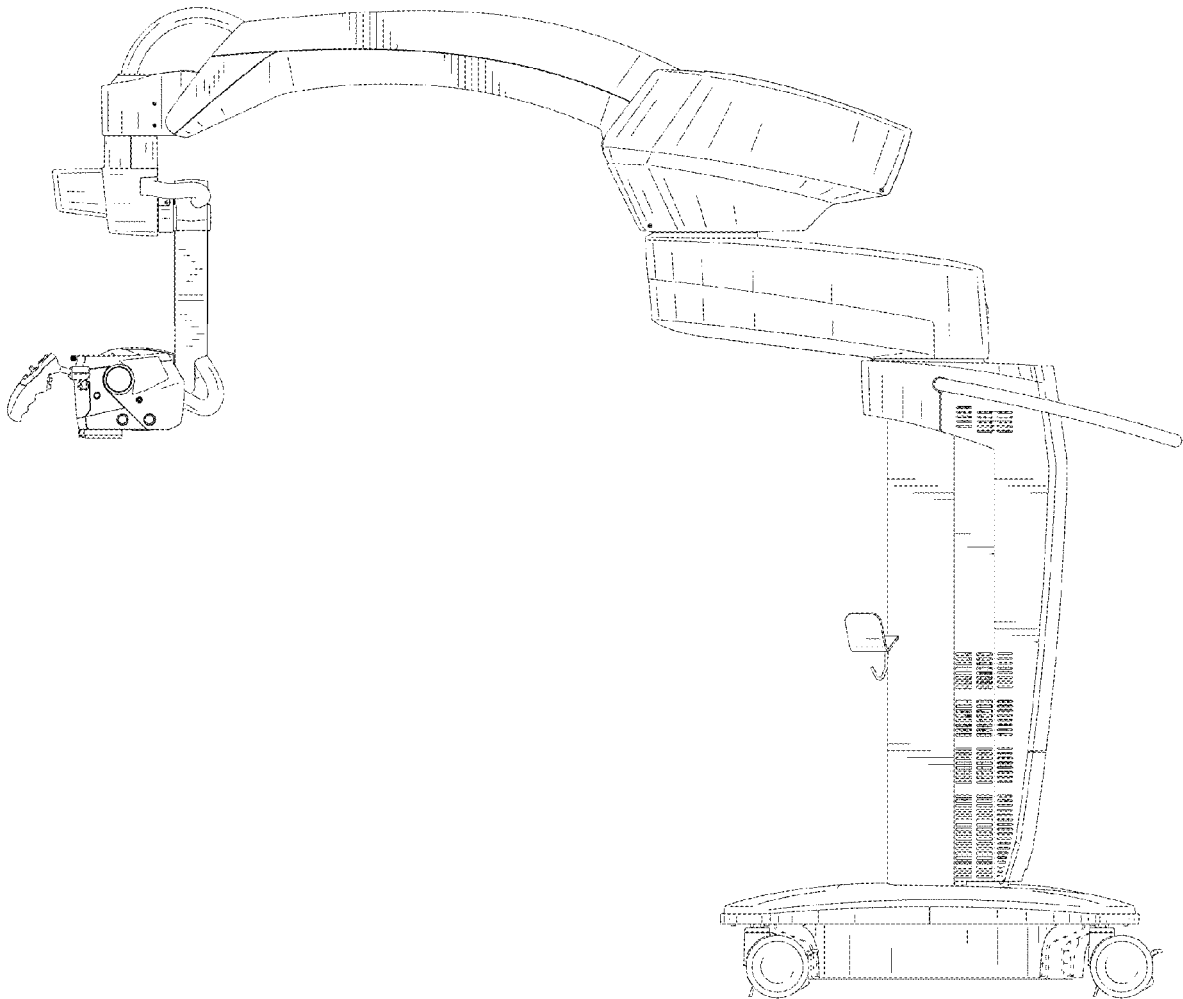


FIG. 8