



(12) **United States Design Patent** (10) **Patent No.:** **US D960,356 S**
Balkovec (45) **Date of Patent:** **** Aug. 9, 2022**

(54) **PIERCING STYLET WITH
NON-CONTACTING DISTAL TIP**

(71) Applicant: **Baylis Medical Company Inc.,**
Montreal (CA)

(72) Inventor: **Christian Balkovec**, Burlington (CA)

(73) Assignee: **Baylis Medical Company Inc.,**
Mississauga (CA)

(**) Term: **15 Years**

(21) Appl. No.: **29/740,455**

(22) Filed: **Jul. 3, 2020**

(51) **LOC (13) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/112**

(58) **Field of Classification Search**
USPC D24/108, 112, 127, 130, 133, 138, 140,
D24/144, 146, 147; 128/200.26, 207.14;
600/585; 604/170.02, 170.03, 264, 540;
606/129
CPC A61M 25/0102; A61M 25/06; A61M
25/0067; A61M 16/0488; A61B 17/3478
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

2,154,968 A * 4/1939 Alkio A61M 25/0041
604/540
5,221,253 A * 6/1993 Coll A61F 2/04
604/170.03
6,036,682 A * 3/2000 Lange A61M 25/0108
604/264
6,210,408 B1 * 4/2001 Chandrasekaran
A61B 18/1492
600/585
D753,302 S * 4/2016 Alley D24/144
9,968,761 B2 * 5/2018 Brecker A61M 25/09025
11,083,875 B2 * 8/2021 McDonald A61M 25/0102
2001/0037065 A1 * 11/2001 Graf A61M 25/0108
600/452

(Continued)

OTHER PUBLICATIONS

[Versa Cross RF Transseptal Solution], available on baylismedical.com, Published [2019] [online], [site visited Jan. 20, 2022], Internet URL: <https://www.baylismedical.com/system/resource_files/PRM-00556%20EN%20VersaCross%20Order%20Guide%20DIGITAL%20J-1,2%20V-5.pdf>. (Year: 2019).*

Primary Examiner — Jonathan J Han

Assistant Examiner — Amanda J Berlinski

(74) *Attorney, Agent, or Firm* — Samuel Tekie; Vincent Man; Glenn Arnold

(57) **CLAIM**


The ornamental design for a piercing stylet with non-contacting distal tip, as shown and described.

DESCRIPTION

FIG. 1 is a right side view of the piercing stylet with non-contacting distal tip;
FIG. 2 is a left side view of the piercing stylet with non-contacting distal tip;
FIG. 3 is a front view of the piercing stylet with non-contacting distal tip;
FIG. 4 is a right side view of the piercing stylet with non-contacting distal tip;
FIG. 5 is a left side 45 degrees from the front view of the piercing stylet with non-contacting distal tip;
FIG. 6 is a right side 45 degrees from the rear view of the piercing stylet with non-contacting distal tip;
FIG. 7 is a left side 45 degrees from the rear view of the piercing stylet with non-contacting distal tip; and,
FIG. 8 is a rear view of the piercing stylet with non-contacting distal tip.

The piercing stylet with non-contacting distal tip is shown with a symbolic break in its length. Any portions not shown after the break line form no part of the claimed design.

1 Claim, 6 Drawing Sheets

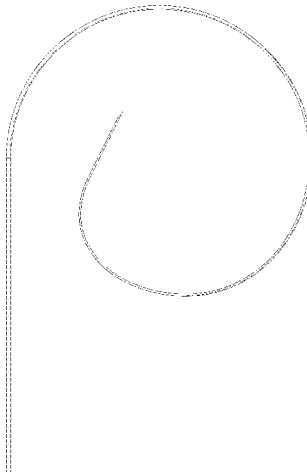

(56)

References Cited

U.S. PATENT DOCUMENTS

2006/0266366	A1 *	11/2006	Tsukashima	A61B 5/065 128/207.14
2007/0078385	A1 *	4/2007	Accisano	A61M 25/0097 604/95.04
2010/0042108	A1 *	2/2010	Hibino	A61B 1/0051 606/129
2011/0190734	A1 *	8/2011	Graffam	A61M 25/04 604/540
2013/0150808	A1 *	6/2013	Ogle	A61M 25/0012 604/264
2016/0357007	A1 *	12/2016	Swanson	G02B 6/3548
2017/0245990	A1 *	8/2017	McDonald	A61F 2/2427
2019/0015644	A1 *	1/2019	Thomspen Smith	A61B 17/3478
2019/0167305	A1 *	6/2019	Pedersen	A61B 17/3468
2020/0086086	A1 *	3/2020	Barone	A61B 8/12
2020/0353208	A1 *	11/2020	Merhi	A61B 17/00234
2021/0205562	A1 *	7/2021	Toth	A61M 16/0434
2021/0322730	A1 *	10/2021	Hayzelden	A61M 25/0138

* cited by examiner

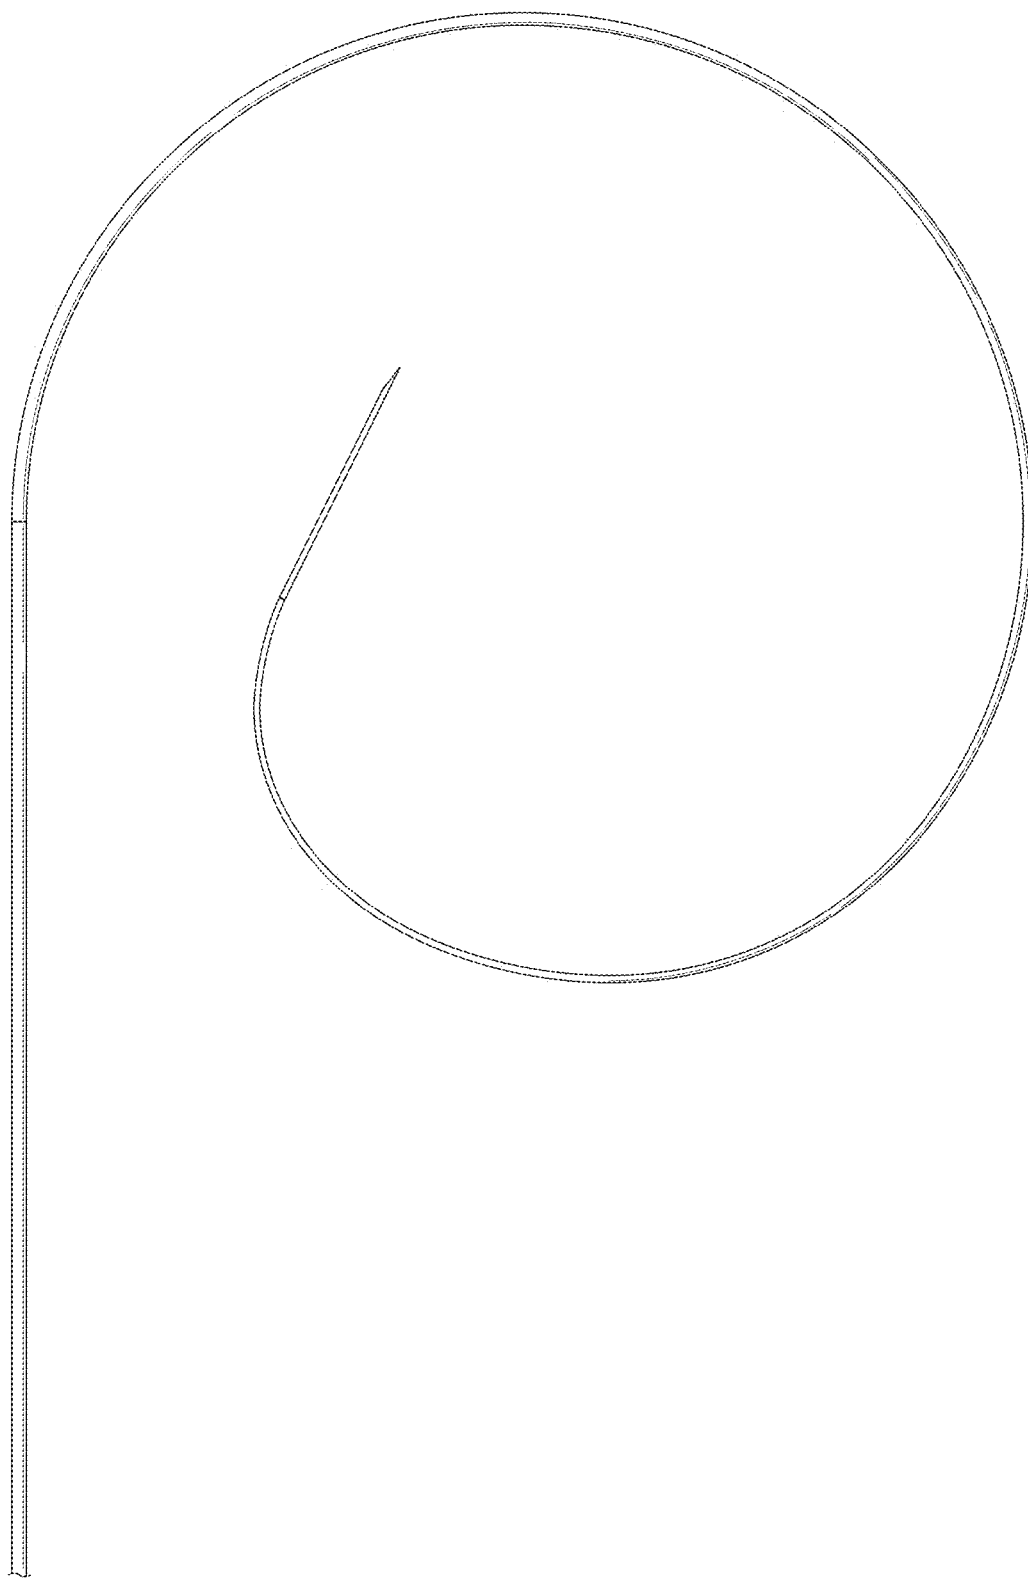


FIG. 1

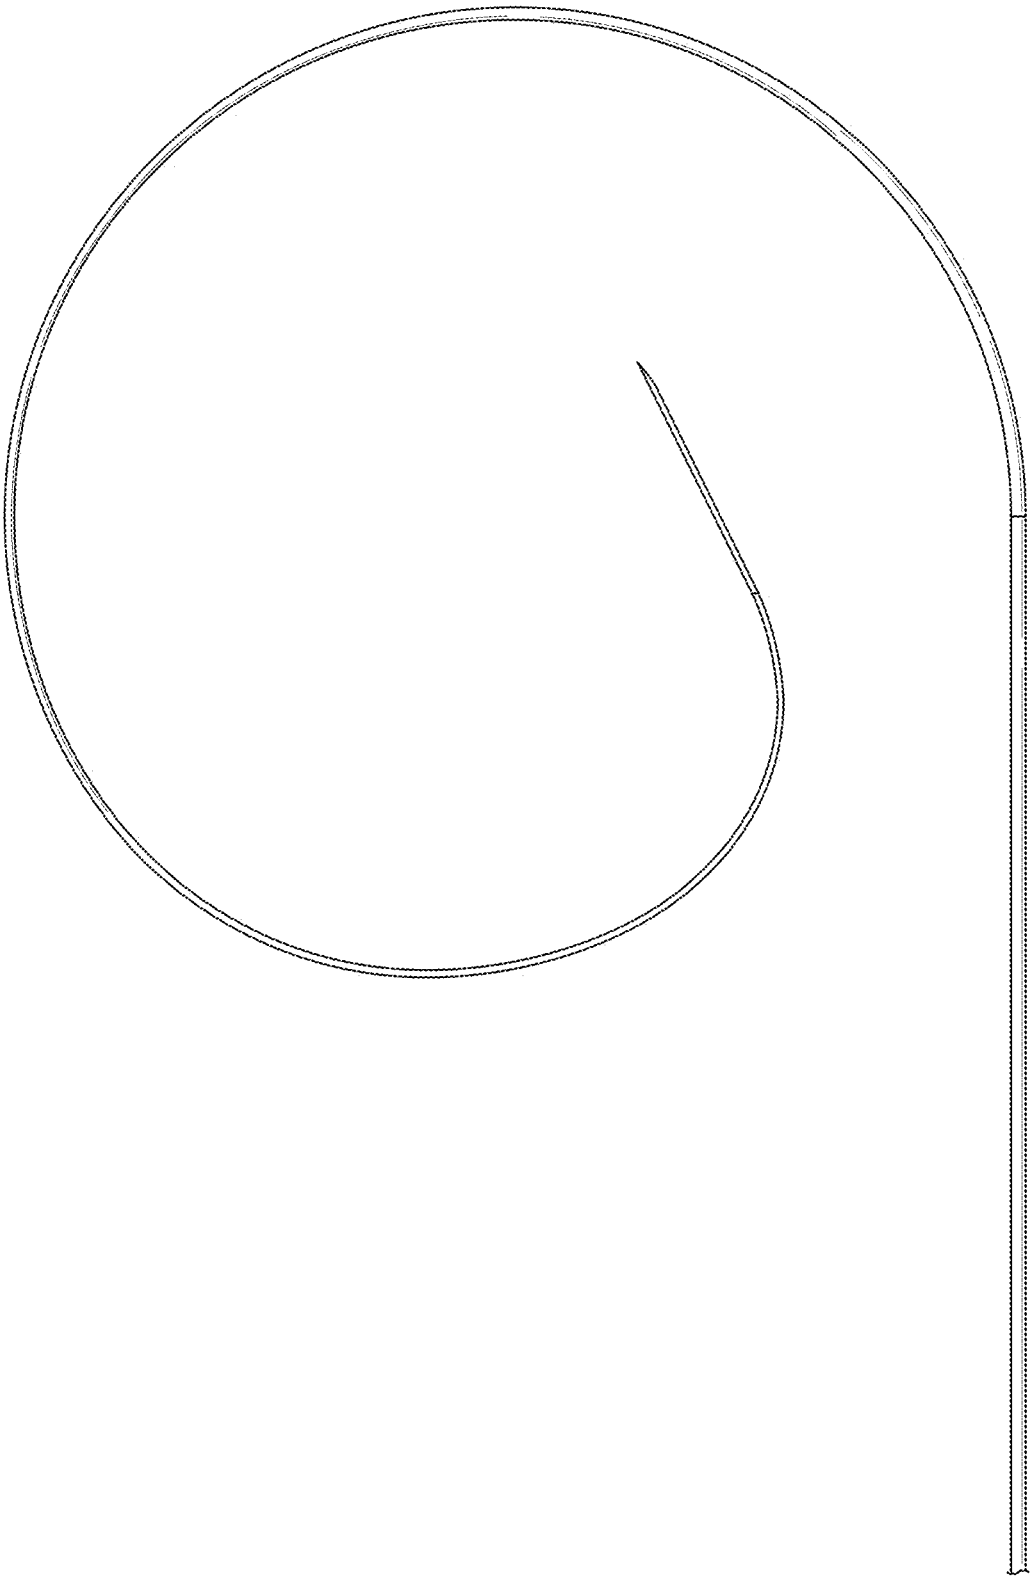


FIG. 2




FIG. 3

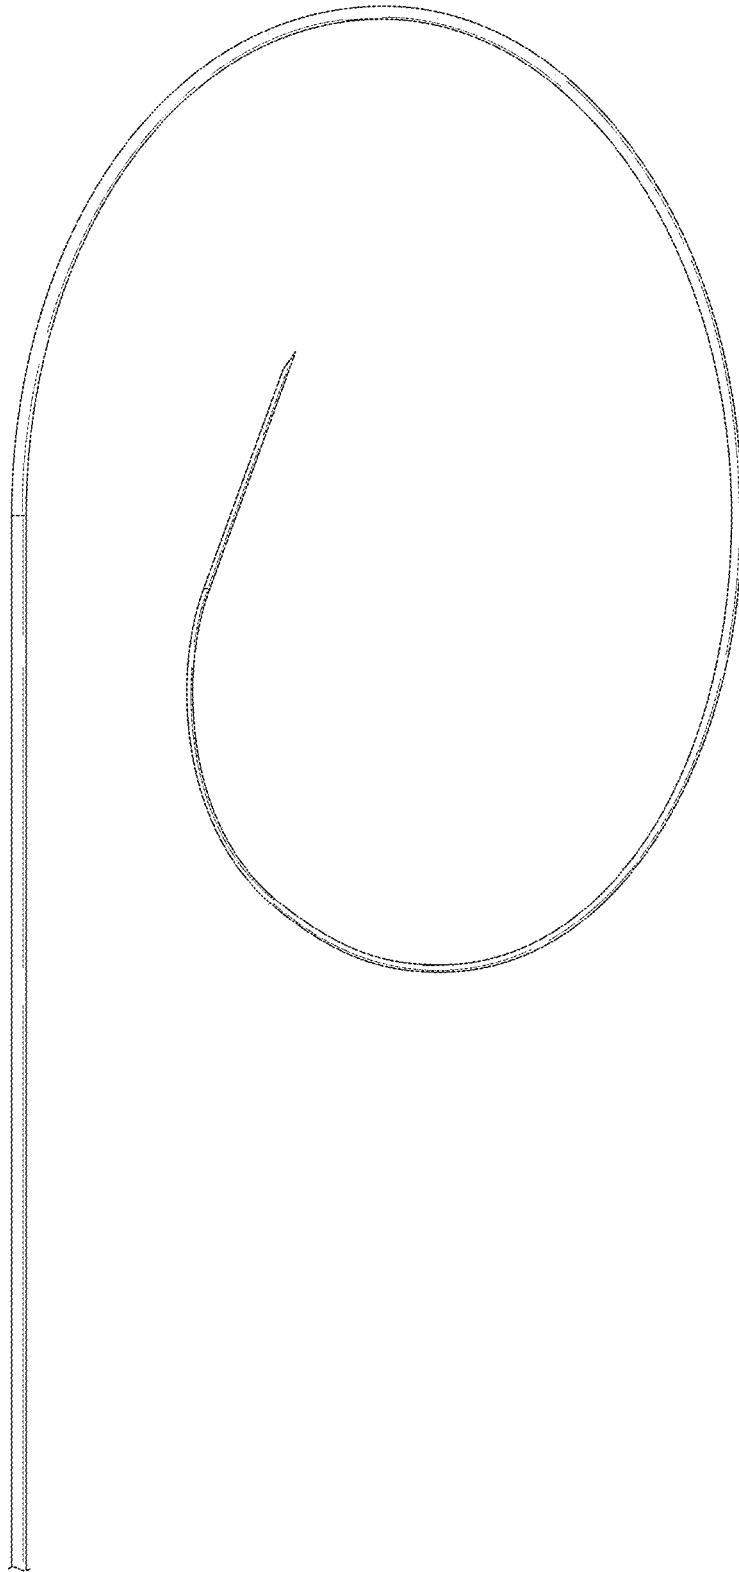


FIG. 4

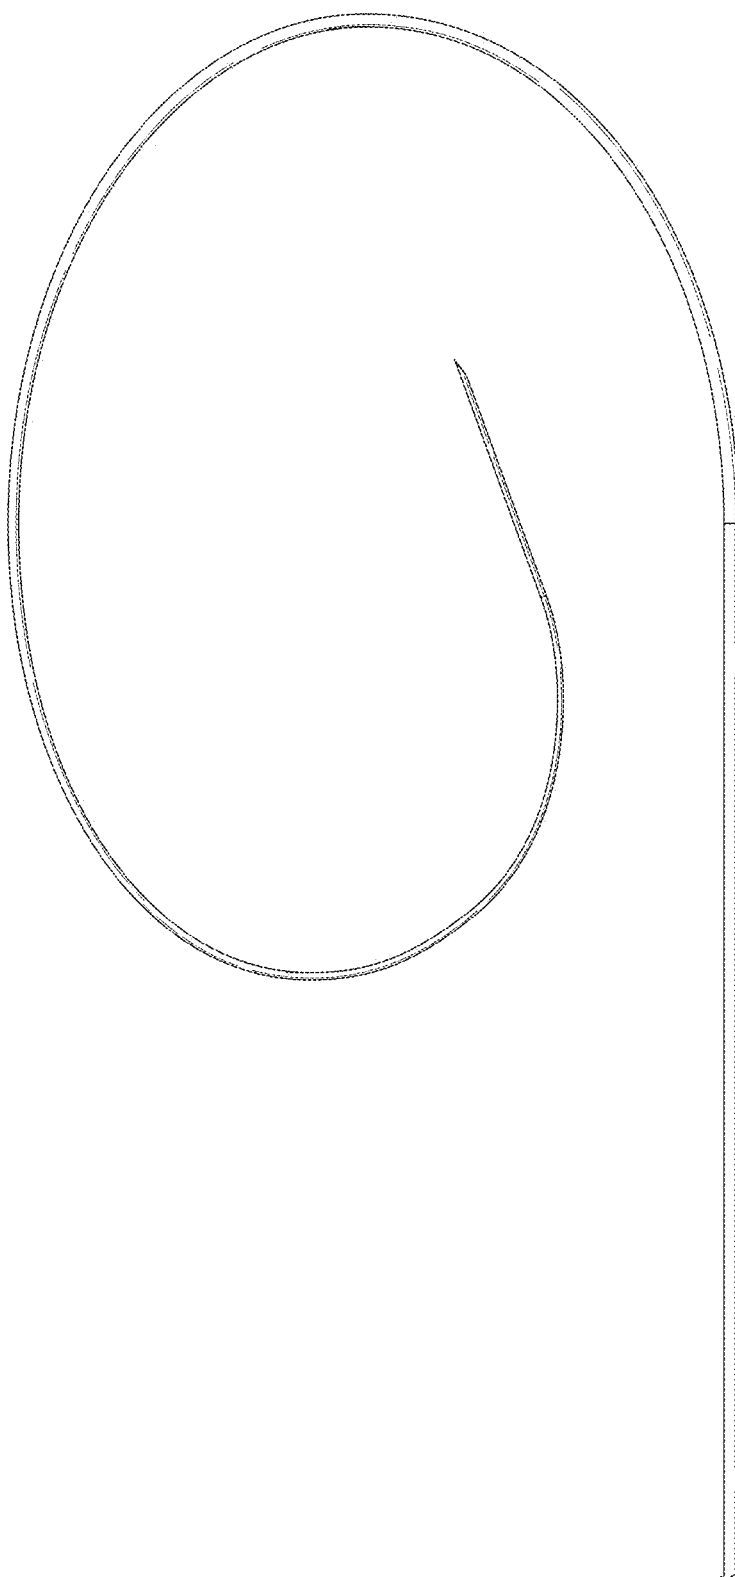


FIG. 5

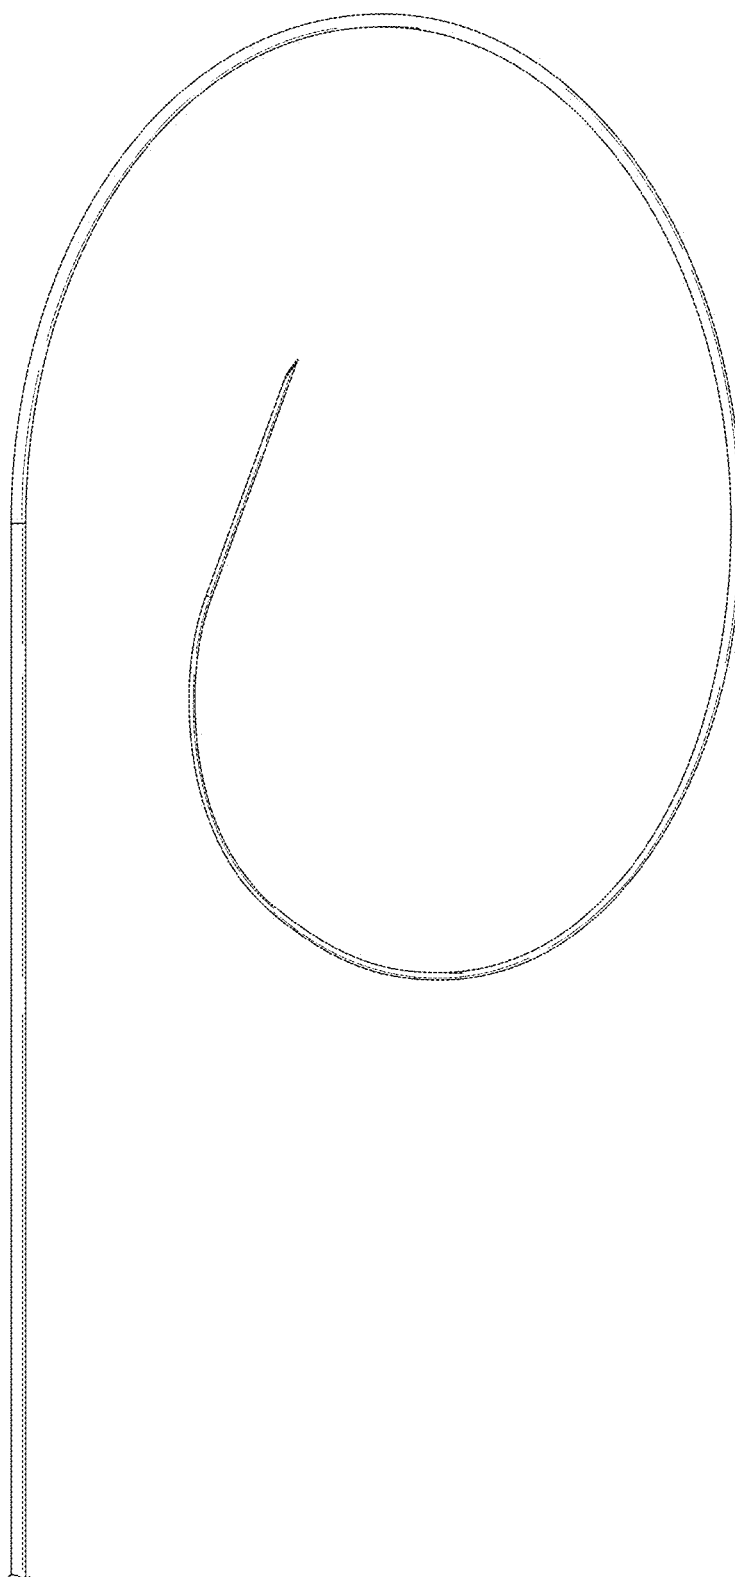


FIG. 6

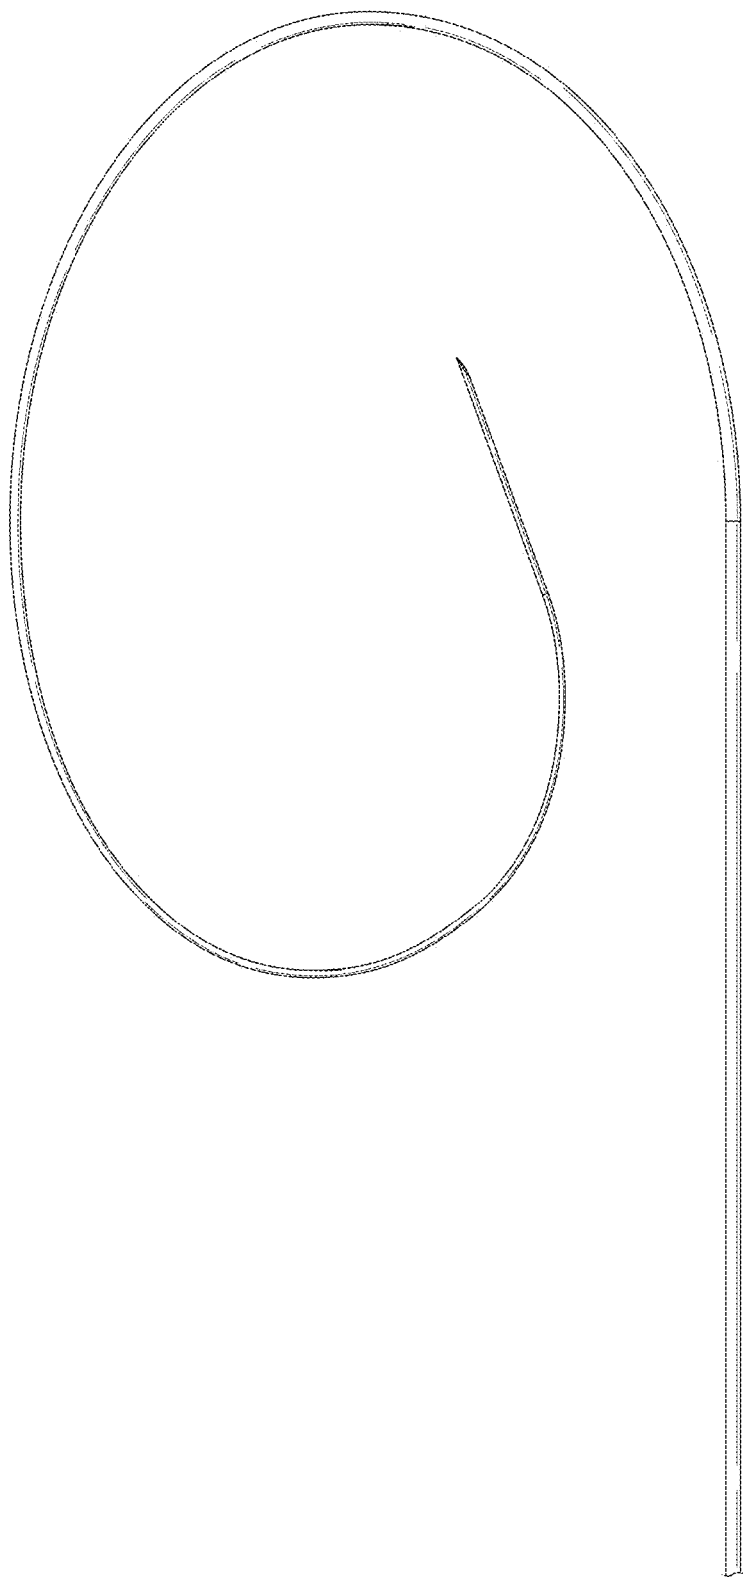


FIG. 7



FIG. 8