



US009044239B2

(12) **United States Patent**
Griego

(10) **Patent No.:** **US 9,044,239 B2**
(45) **Date of Patent:** ***Jun. 2, 2015**

(54) **MULTIPLE CLIP DEPLOYMENT MAGAZINE**

(75) Inventor: **John A. Griego**, Blackstone, MA (US)

(73) Assignee: **BOSTON SCIENTIFIC SCIMED, INC.**, Maple Grove, MN (US)

(*) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 1620 days.

This patent is subject to a terminal disclaimer.

(21) Appl. No.: **12/543,928**

(22) Filed: **Aug. 19, 2009**

(65) **Prior Publication Data**

US 2009/0306682 A1 Dec. 10, 2009

Related U.S. Application Data

(63) Continuation of application No. 11/032,973, filed on Jan. 11, 2005, now Pat. No. 8,080,021.

(51) **Int. Cl.**

A61B 17/10 (2006.01)
A61B 17/128 (2006.01)
A61B 17/068 (2006.01)
A61B 17/122 (2006.01)
A61B 17/08 (2006.01)
A61B 17/04 (2006.01)

(52) **U.S. Cl.**

CPC **A61B 17/1285** (2013.01); **Y10T 29/53491** (2013.01); **A61B 17/068** (2013.01); **A61B 17/083** (2013.01); **A61B 17/122** (2013.01); **A61B 17/1227** (2013.01); **A61B 2017/0488** (2013.01)

(58) **Field of Classification Search**

USPC 606/143, 157, 139, 142; 227/176.1, 227/179.1; 29/809, 811.2

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,512,345 A 4/1985 Green
5,366,459 A 11/1994 Yoon

(Continued)

FOREIGN PATENT DOCUMENTS

AU 2004289214 5/2005
WO 2005/046489 5/2005

Primary Examiner — Thomas McEvoy



Assistant Examiner — Julie A Szpir

(74) *Attorney, Agent, or Firm* — Fay Kaplun & Marcin, LLP

(57) **ABSTRACT**

An apparatus for deployment of multiple hemostatic clips, comprises a shaft connected to a handle and a control linkage operatively connected to the handle in combination with a magazine disposed at a distal end of the shaft, the magazine containing a plurality of clips arranged in a chain rotatable within the magazine, wherein a proximal-most one of the clips is coupled to the control linkage, a distal portion of the magazine being contoured to permit opening of a distal-most one of the clips during a distal stroke of the control linkage, and to assist closing and locking of the distal-most clip during a proximal stroke of the control linkage, the magazine including an expanded chamber sized to allow opening in any rotational orientation of a next clip located immediately proximal to the distal-most clip to a degree sufficient to disengage the distal-most clip. A method for deploying multiple hemostatic clips, comprises positioning a distal end of a magazine containing a clip chain over selected target tissue and actuating a control link of the magazine in a distal stroke to open and distally translate a distal-most clip of the clip chain in combination with orienting the open distal-most clip in a desired orientation to grasp the target tissue and actuating the control link in a proximal stroke to close and lock the distal-most clip over the target tissue. The control link is further actuated in the proximal stroke to move a next clip immediately proximal to the distal-most clip into an expanded portion of the magazine sized to allow the next clip to open to a degree sufficient to release the distal-most clip regardless of a circumferential orientation of the next clip.

13 Claims, 30 Drawing Sheets

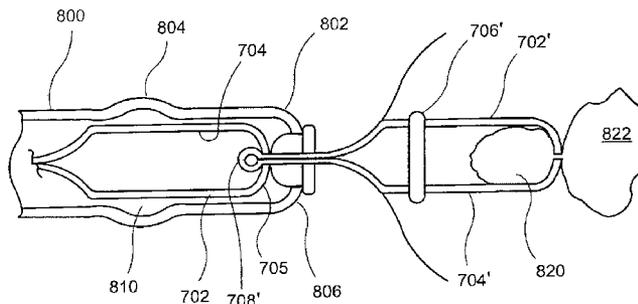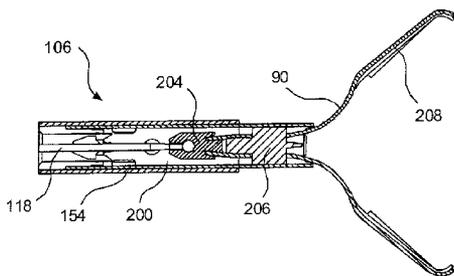

(56)

References Cited

U.S. PATENT DOCUMENTS

6,599,298	B1 *	7/2003	Forster et al.	606/139	2002/0198538	A1	12/2002	Kortenbach et al.	
2002/0045909	A1	4/2002	Kimura et al.		2002/0198539	A1	12/2002	Sixto, Jr. et al.	
2002/0151916	A1 *	10/2002	Muramatsu et al.	606/158	2003/0069592	A1	4/2003	Adams et al.	
					2005/0107809	A1 *	5/2005	Litscher et al.	606/142

* cited by examiner

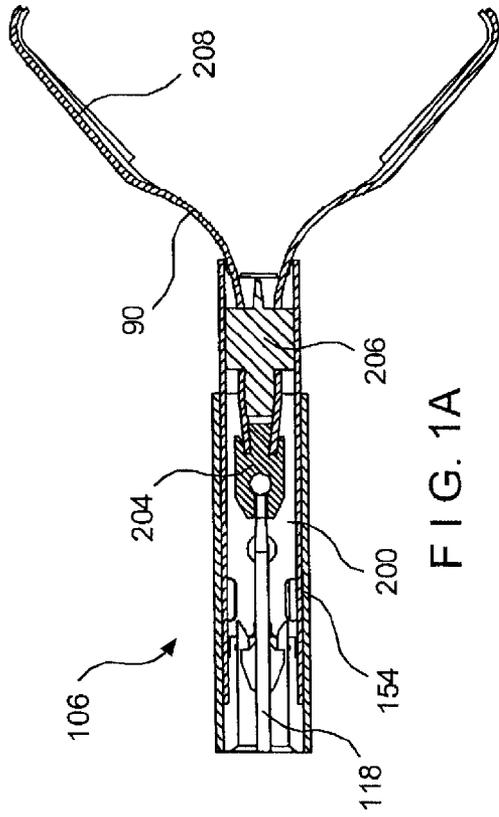


FIG. 1A

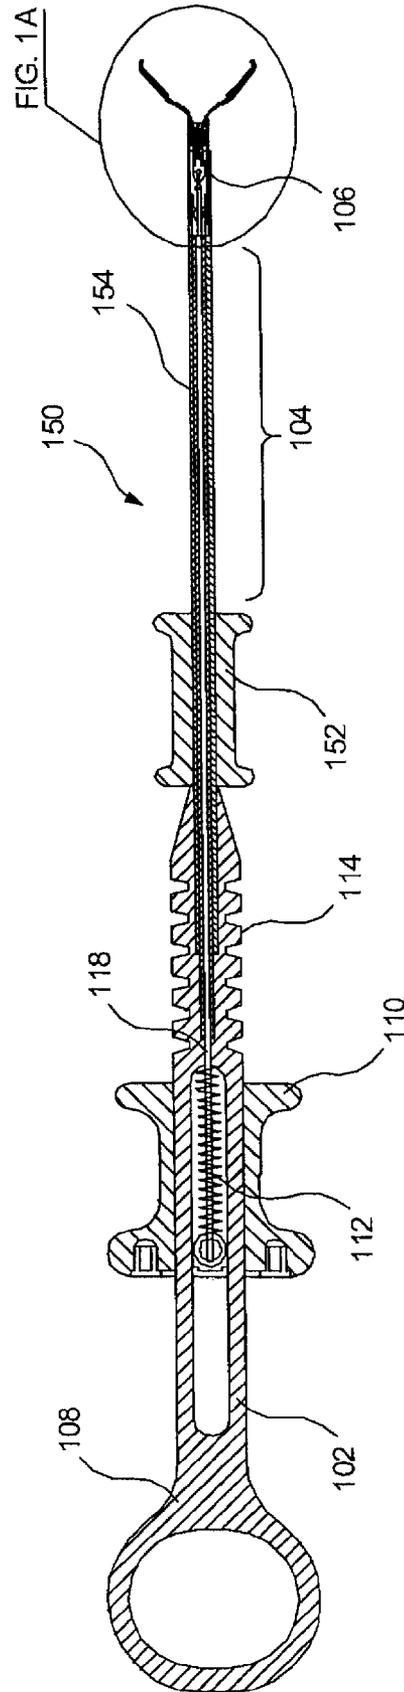



FIG. 1

FIG. 1A

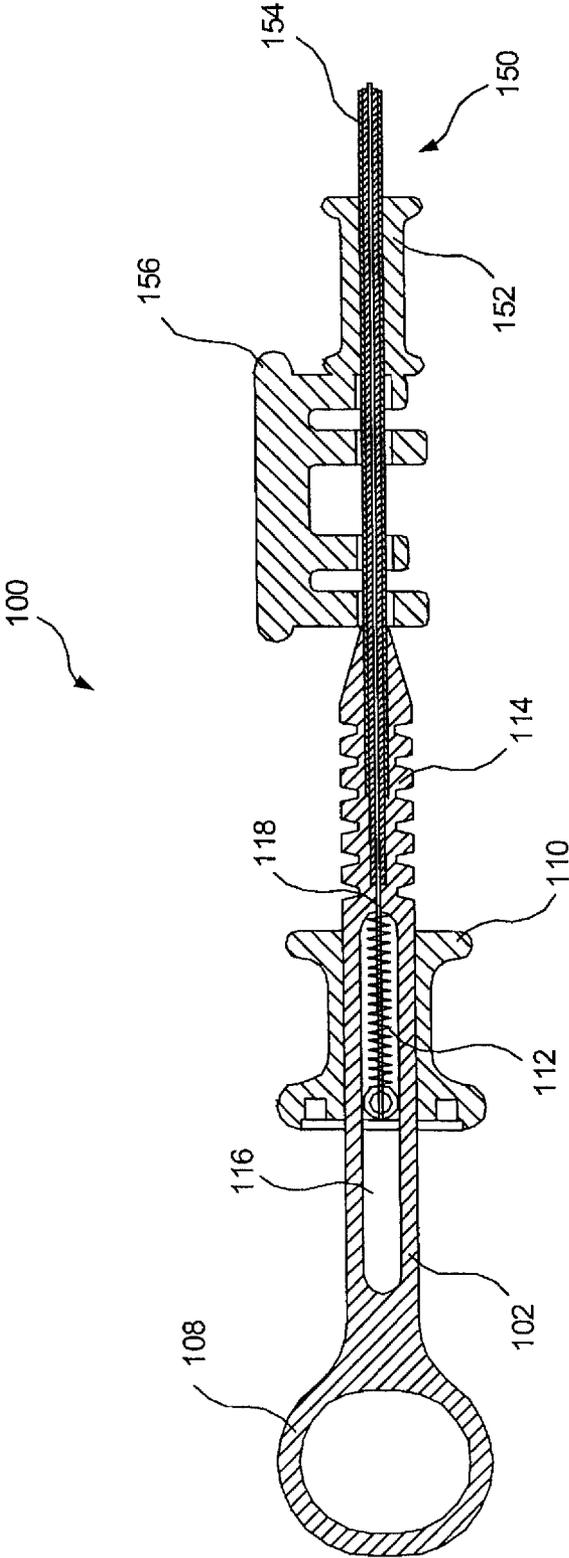


FIG. 2

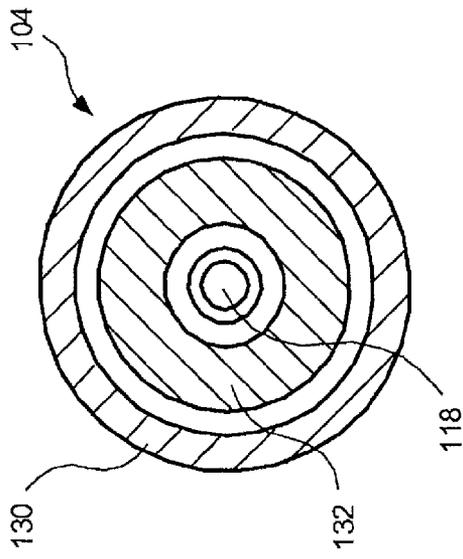


FIG. 4

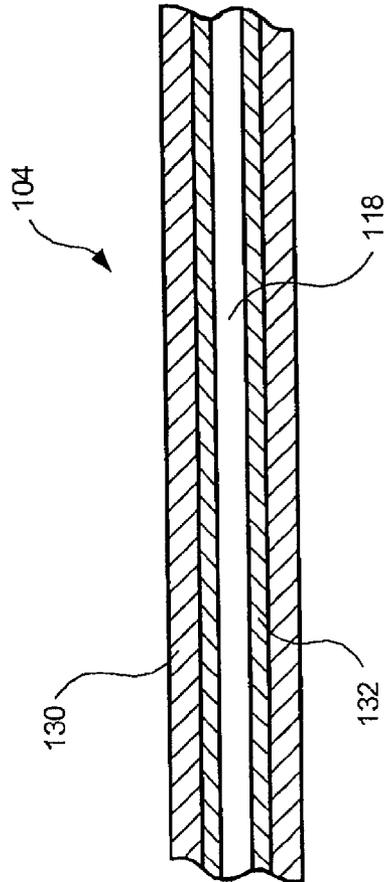


FIG. 3

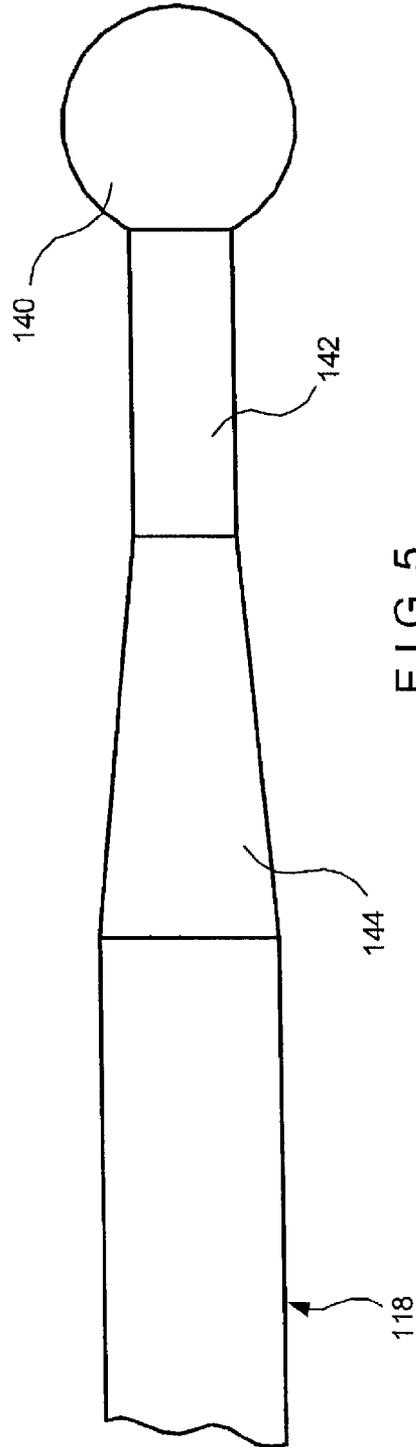
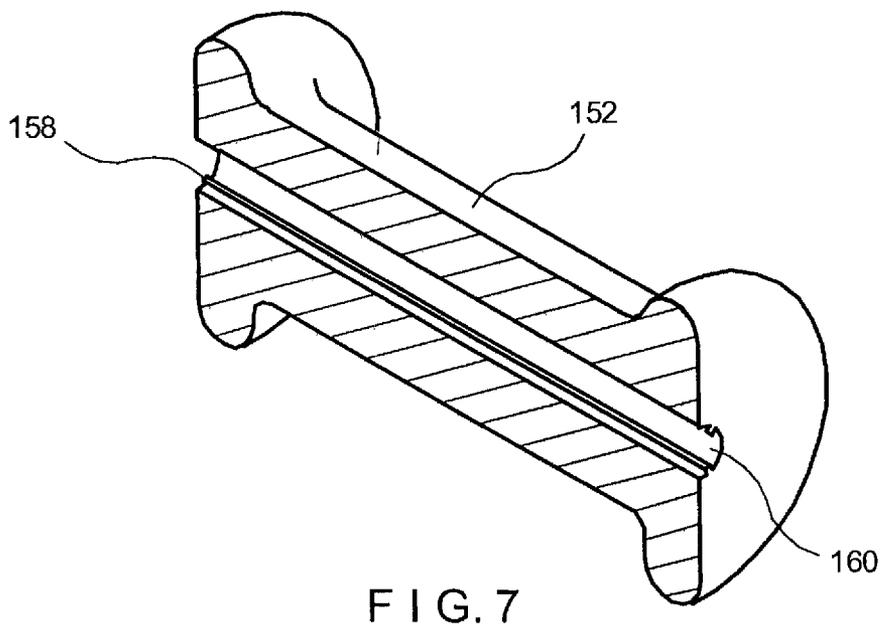
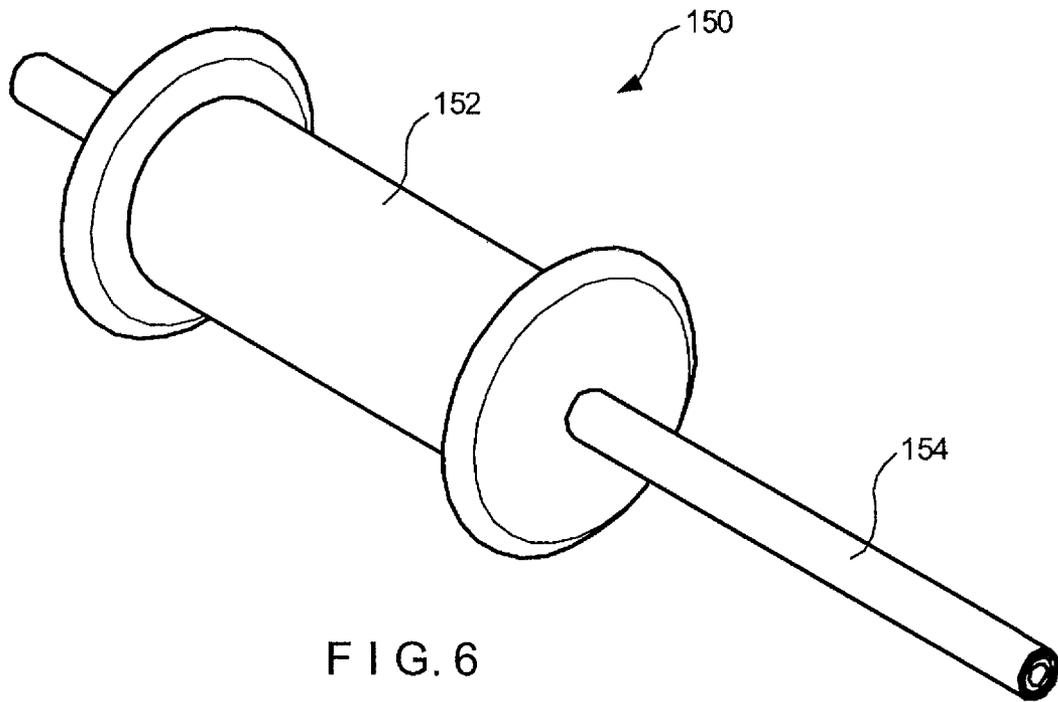


FIG. 5



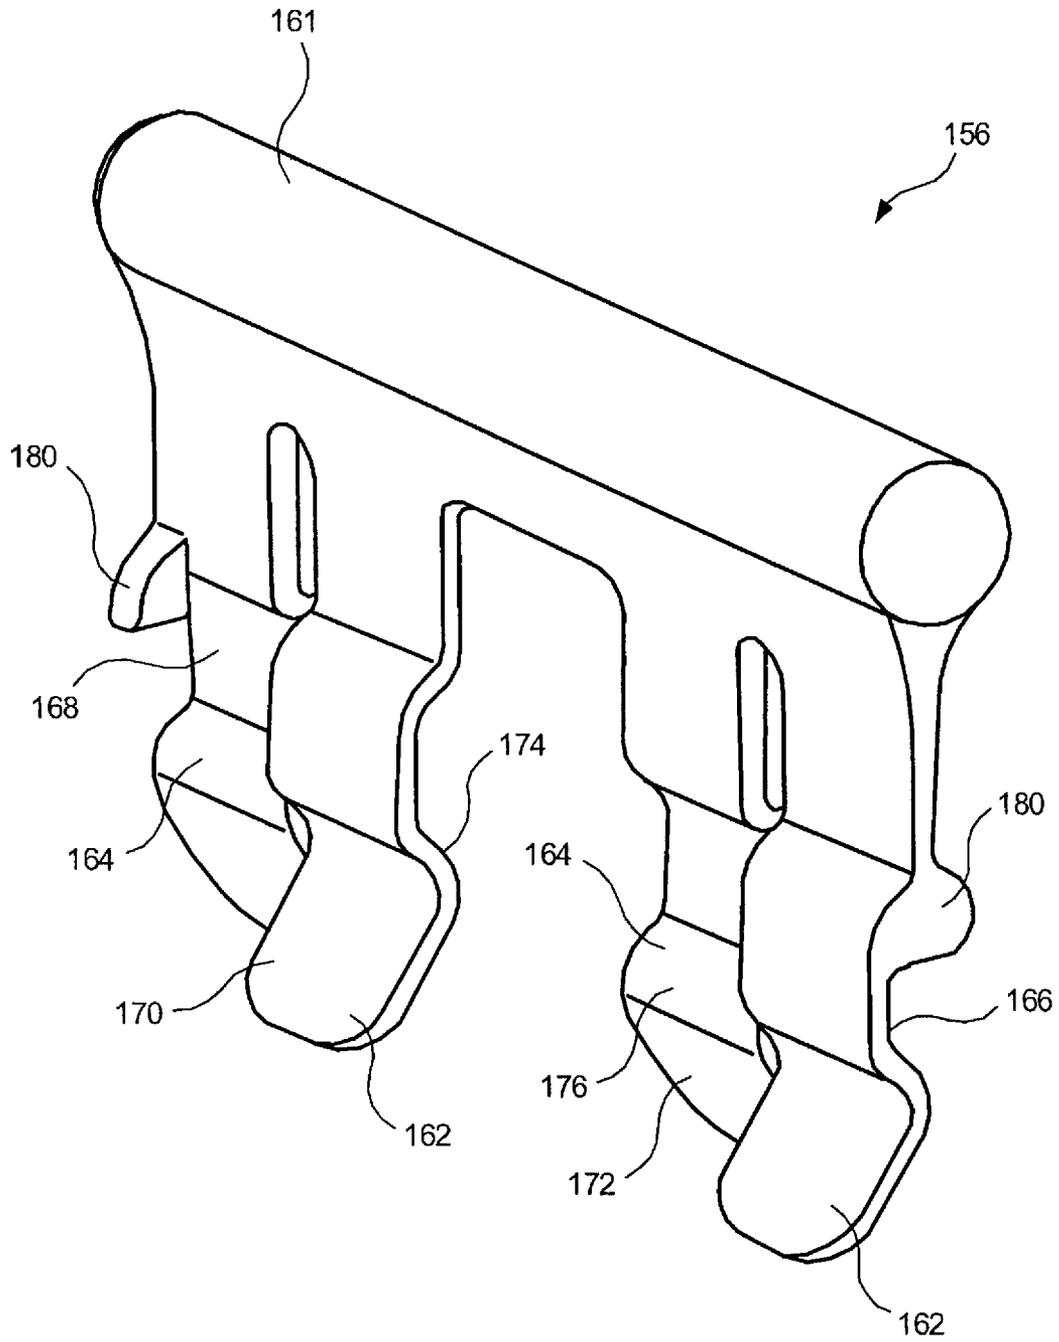


FIG. 8

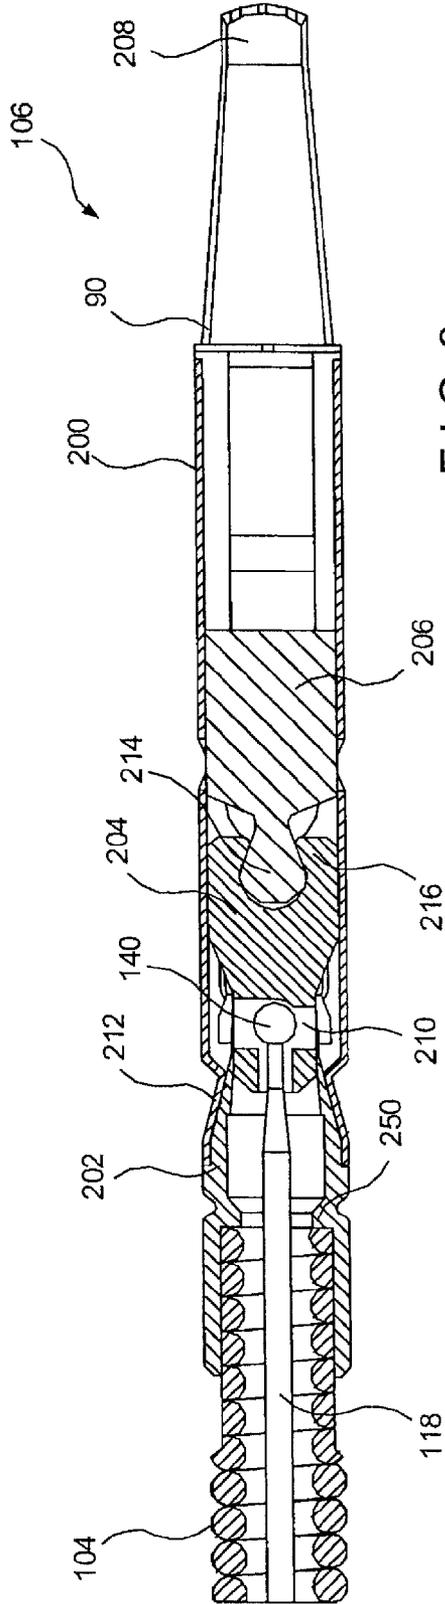


FIG. 9

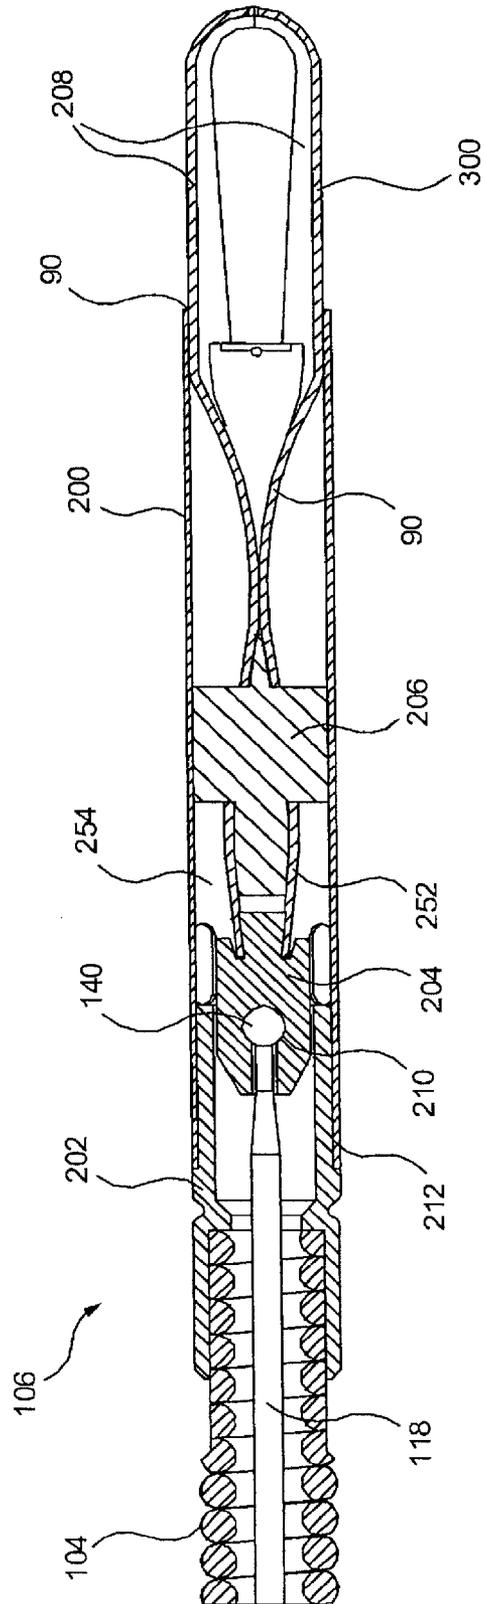


FIG. 10

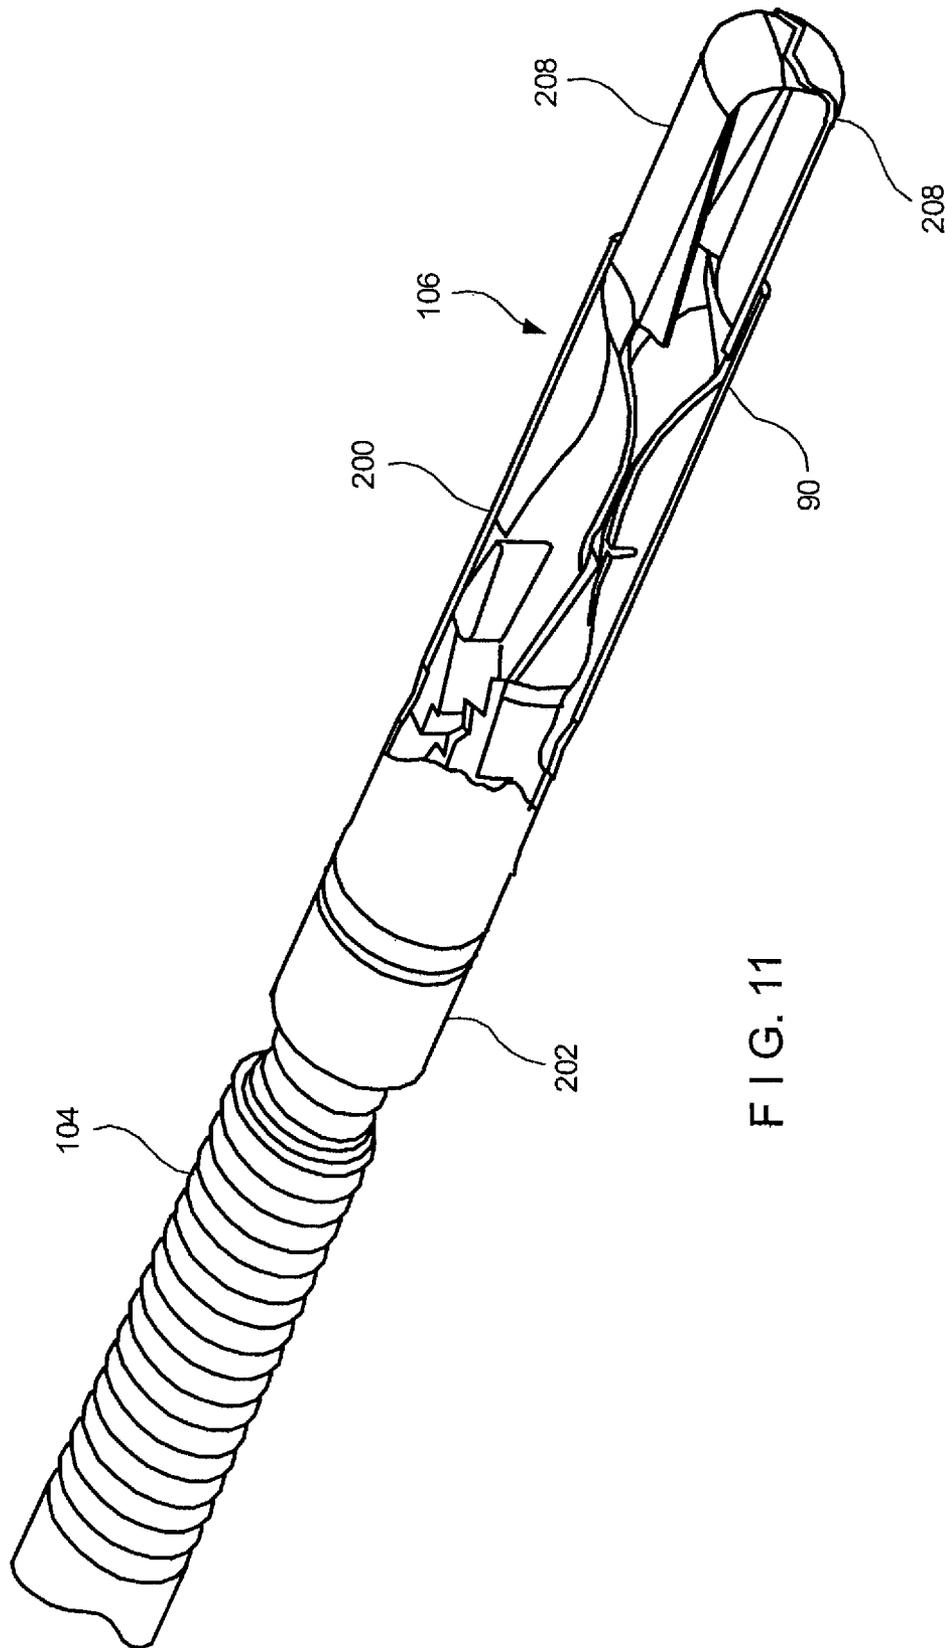


FIG. 11

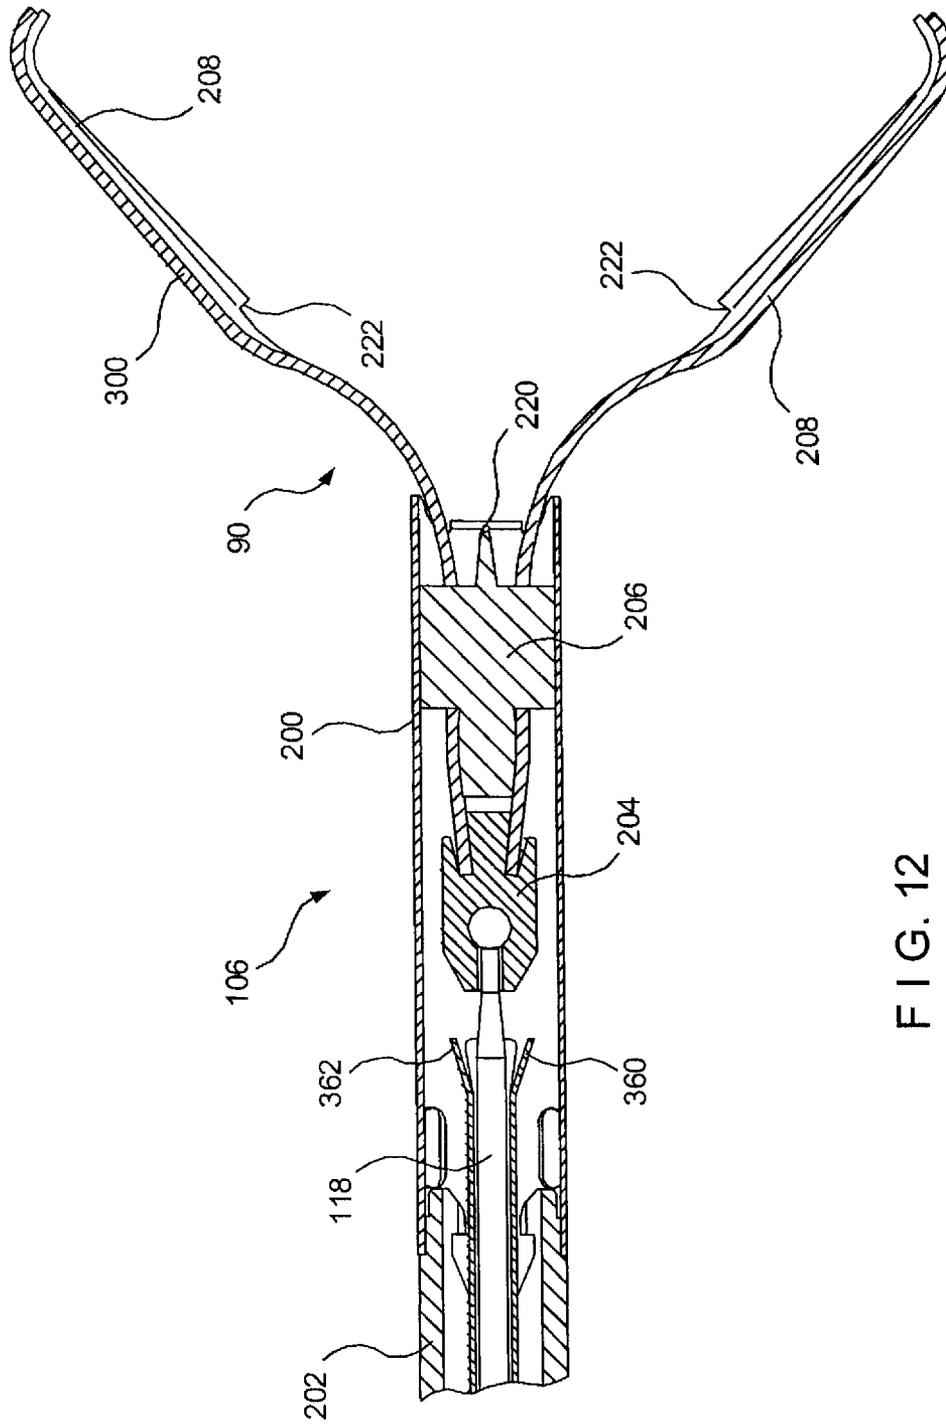


FIG. 12

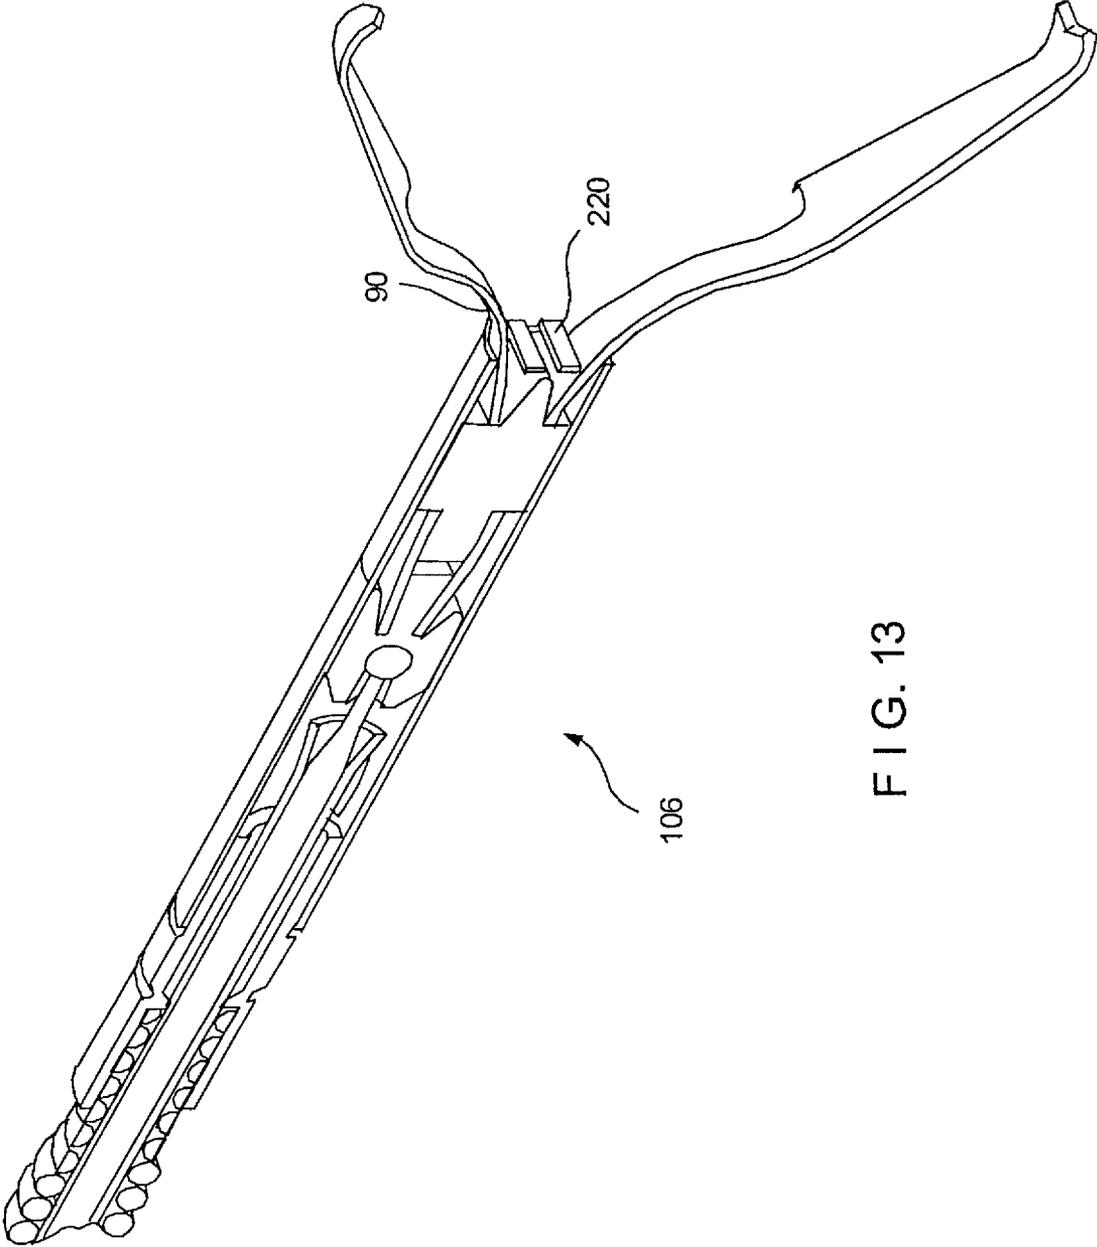


FIG. 13

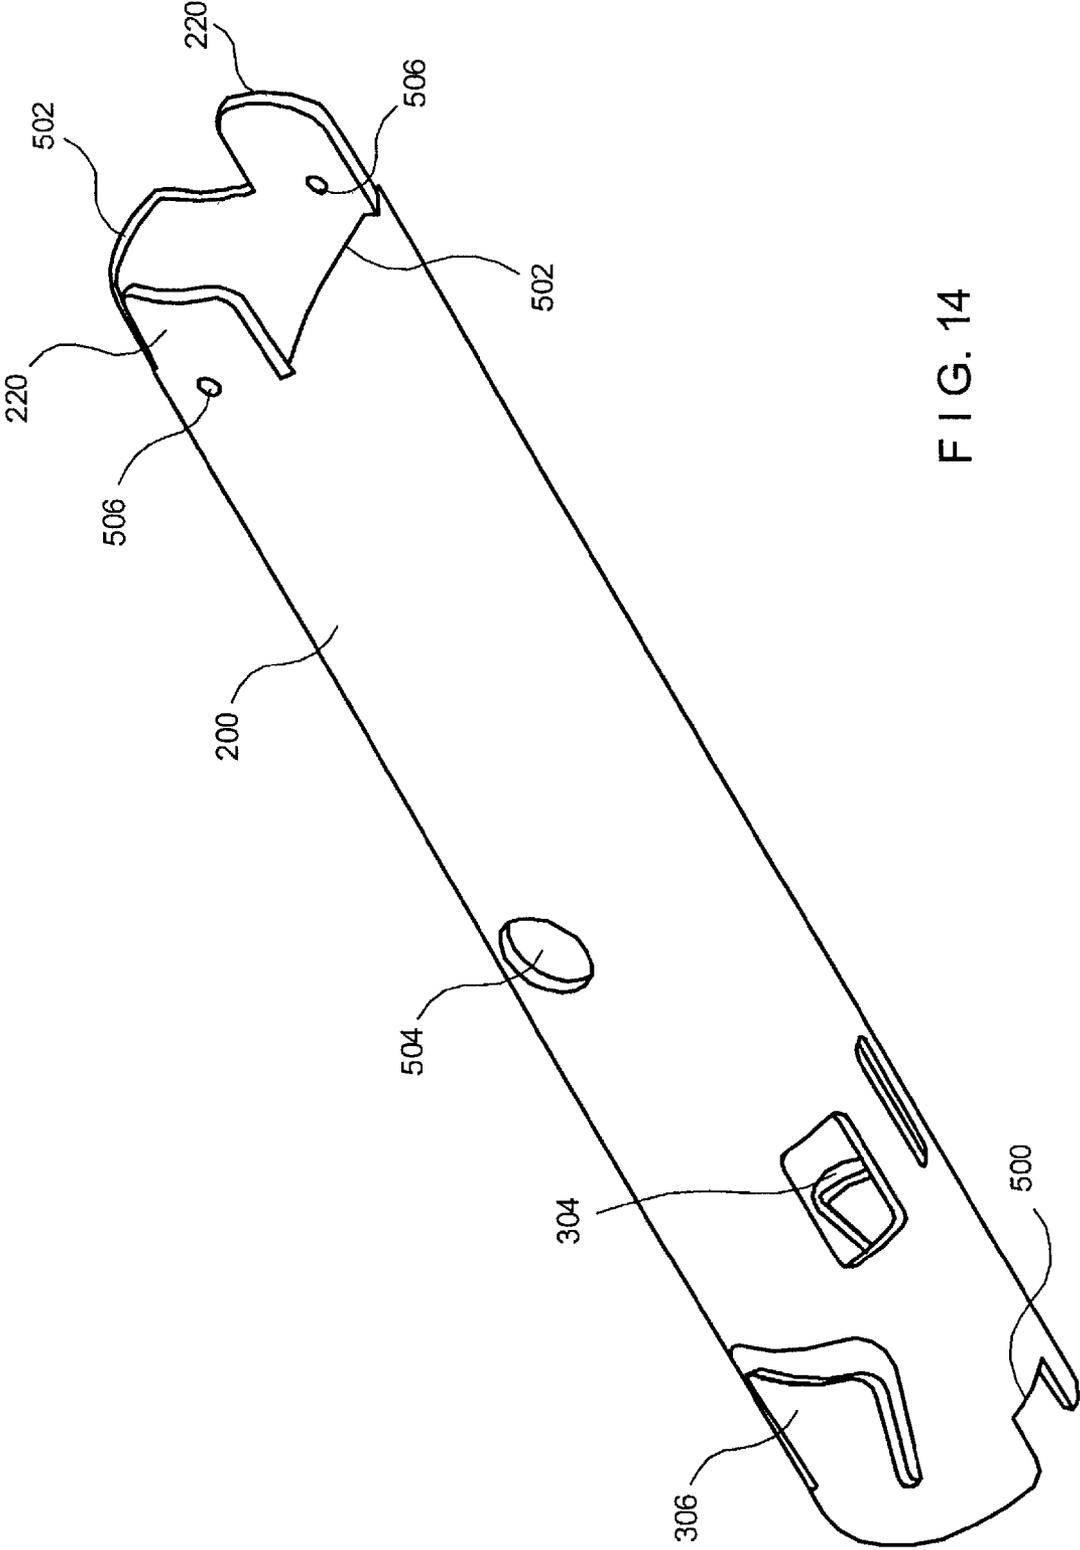
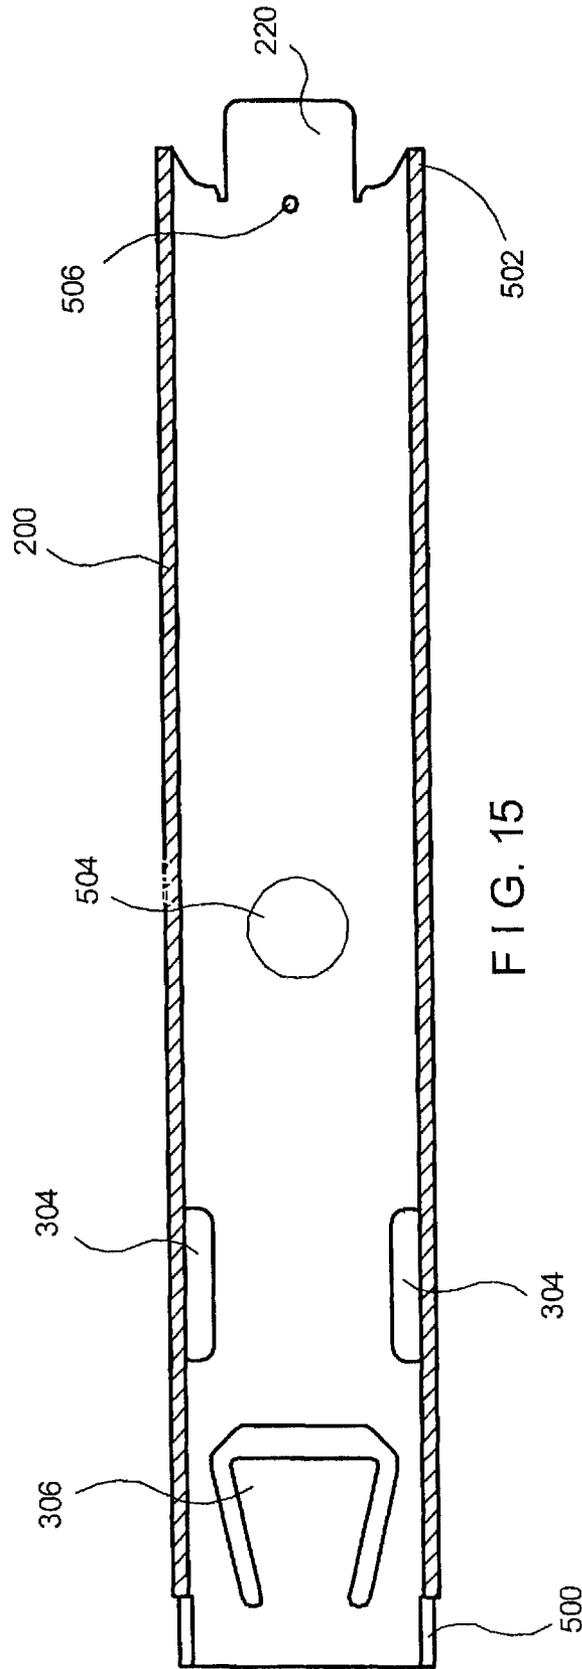


FIG. 14



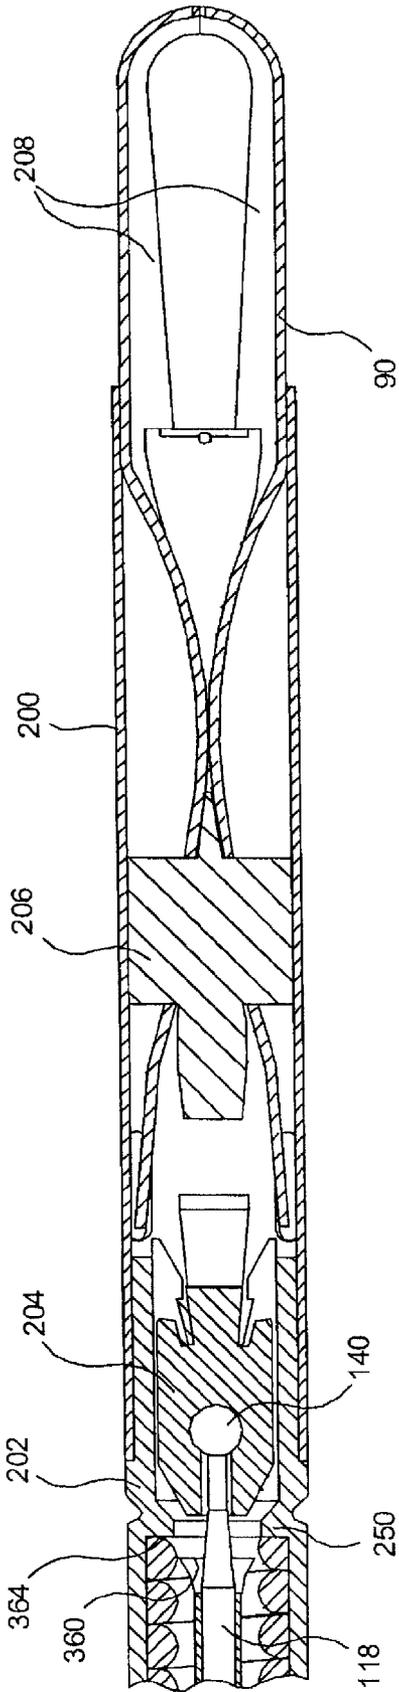


FIG. 16

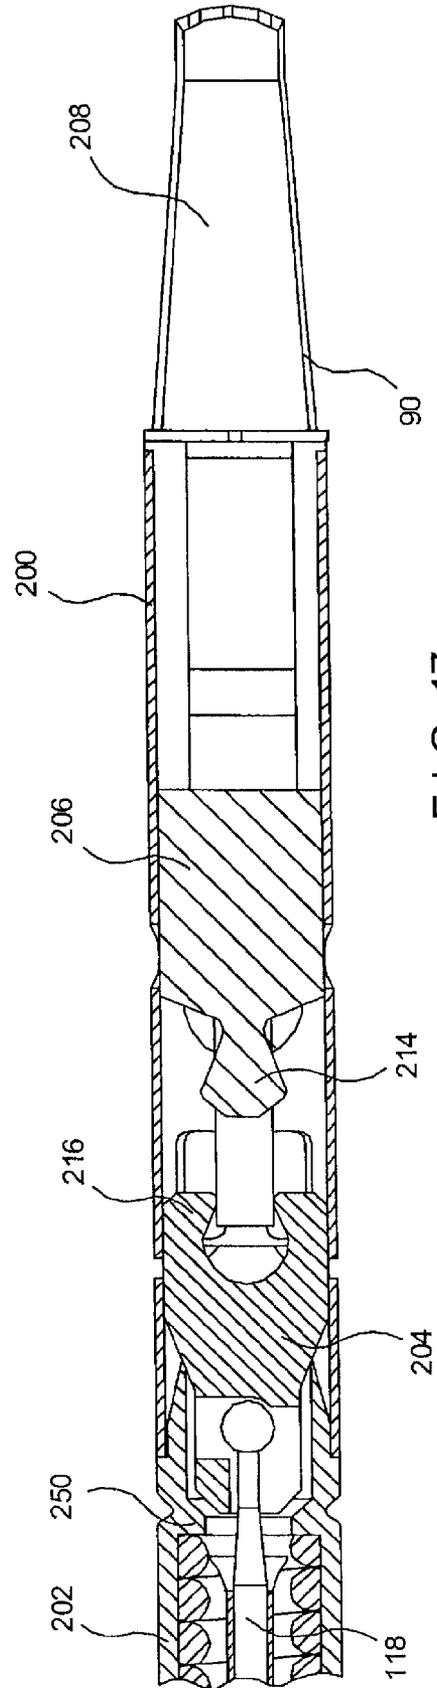


FIG. 17

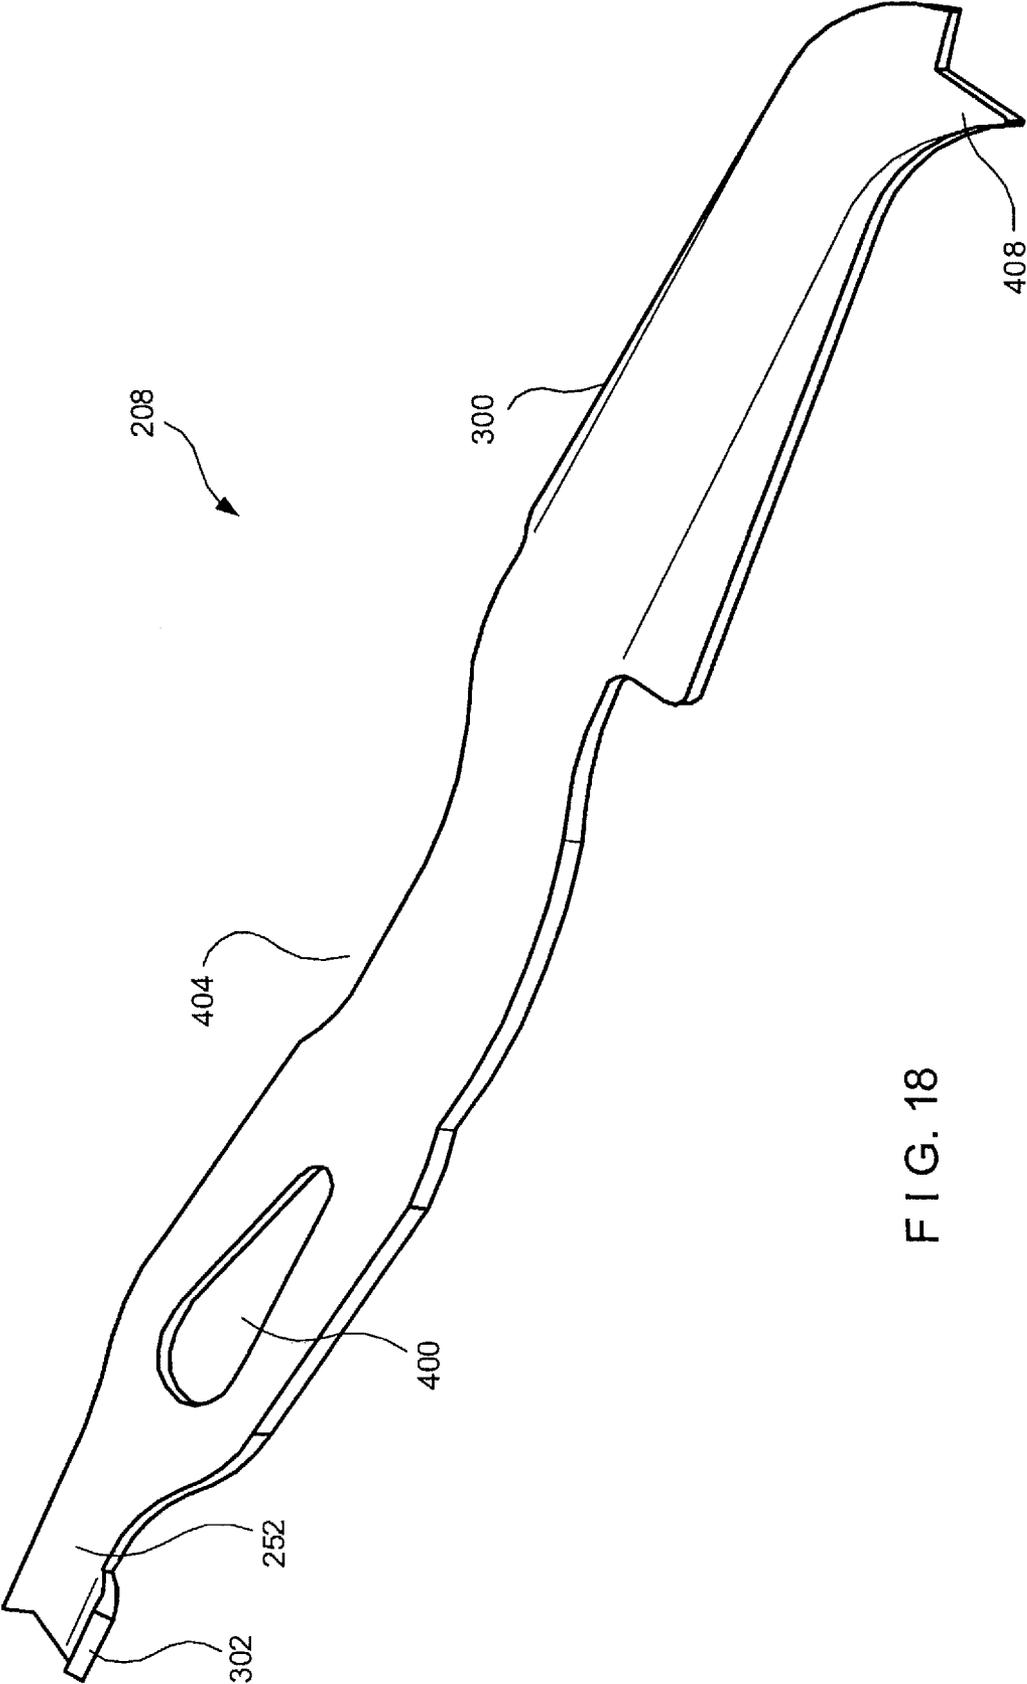
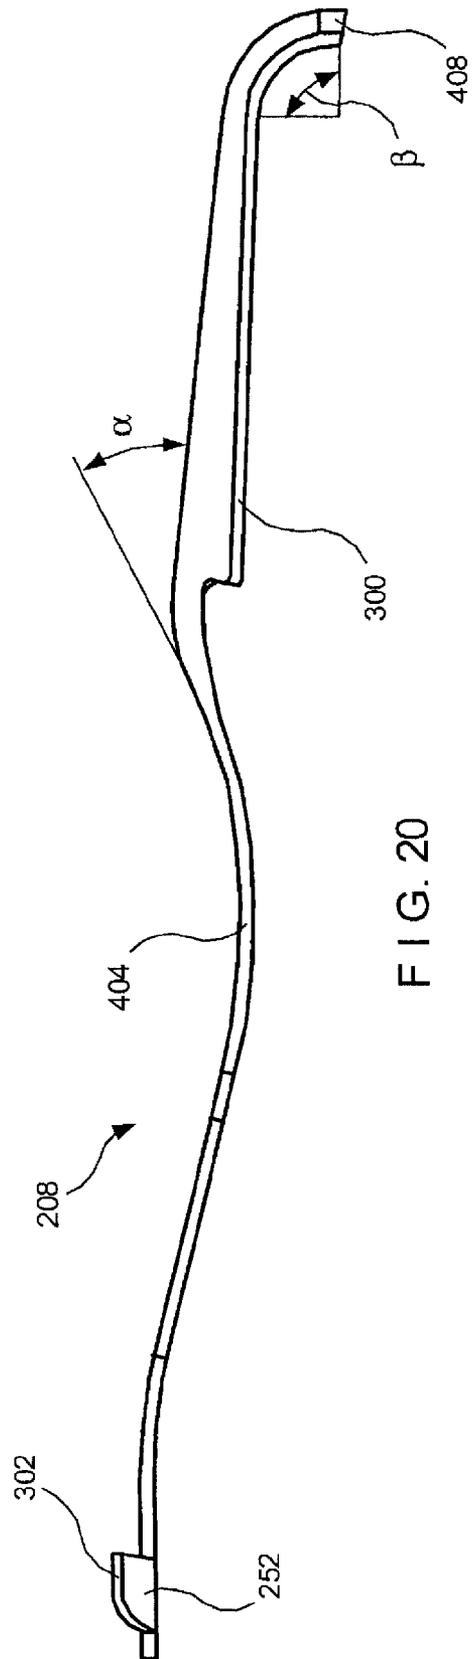
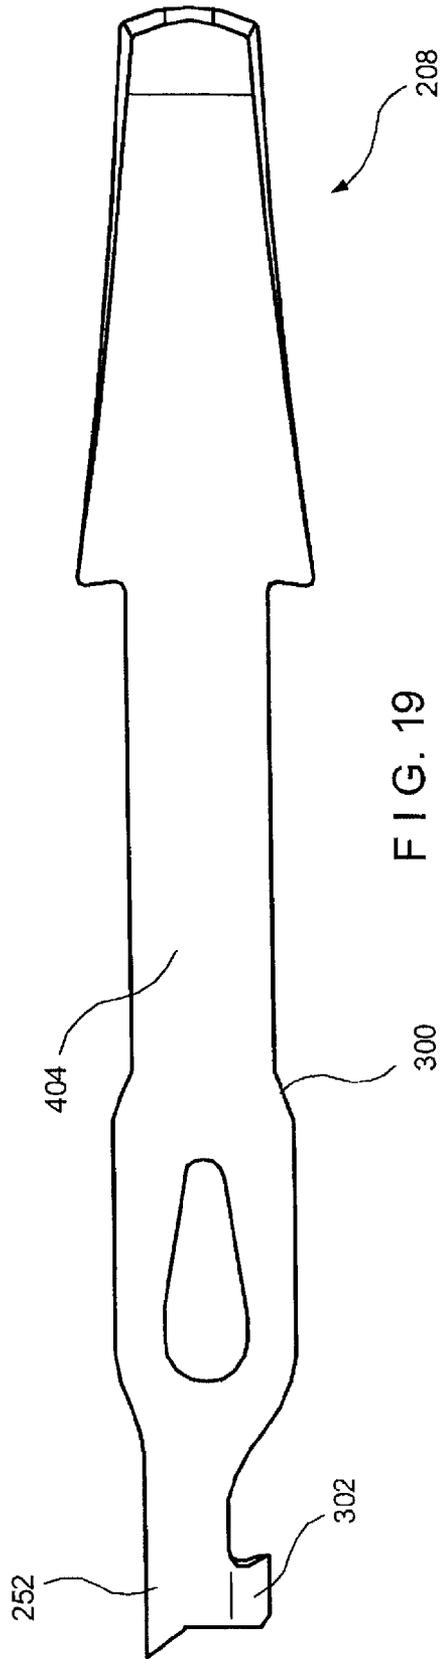


FIG. 18



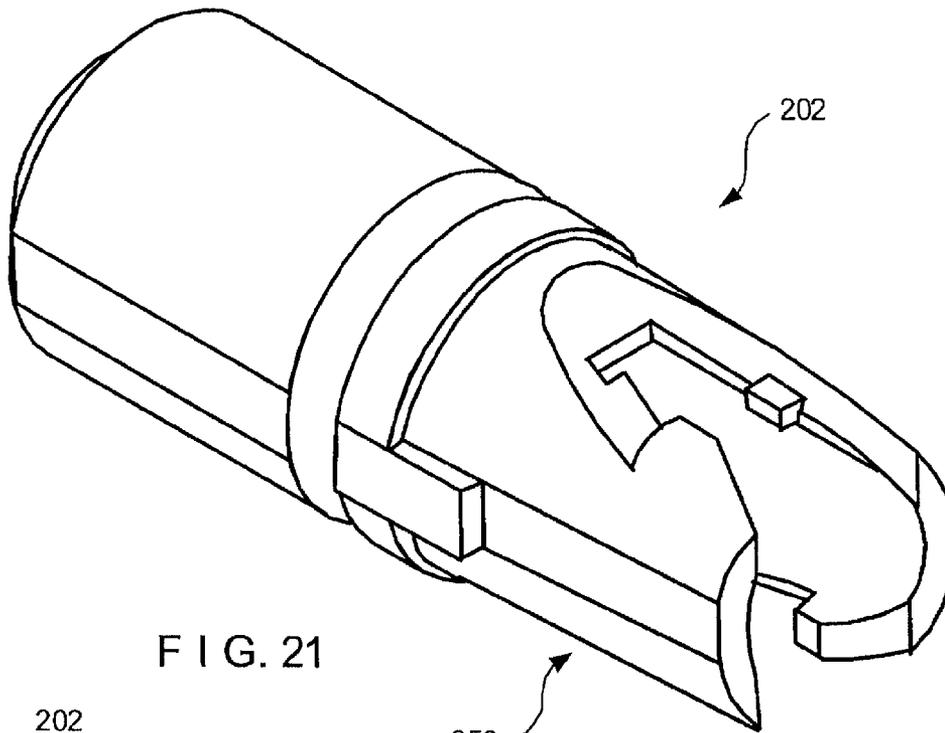


FIG. 21

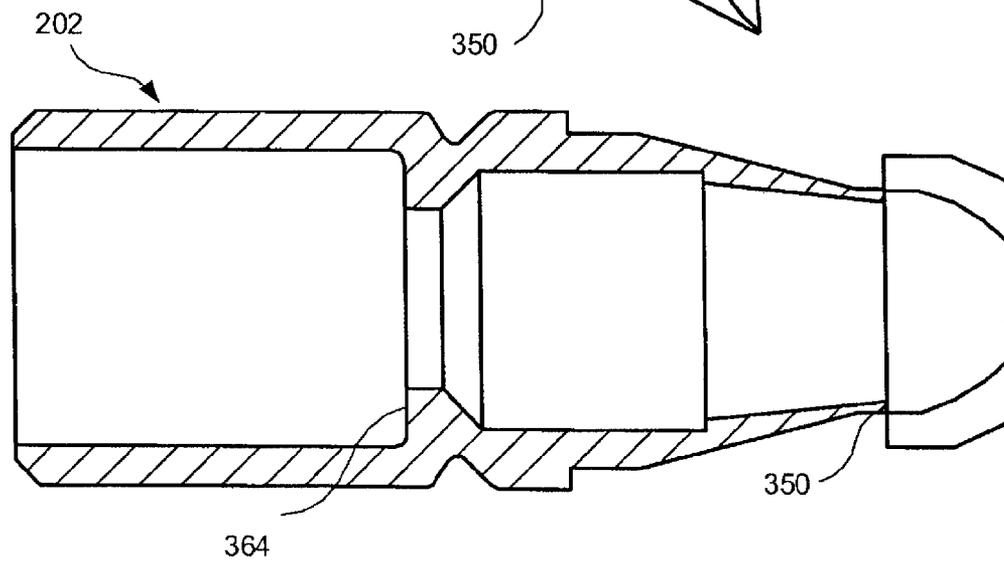


FIG. 22

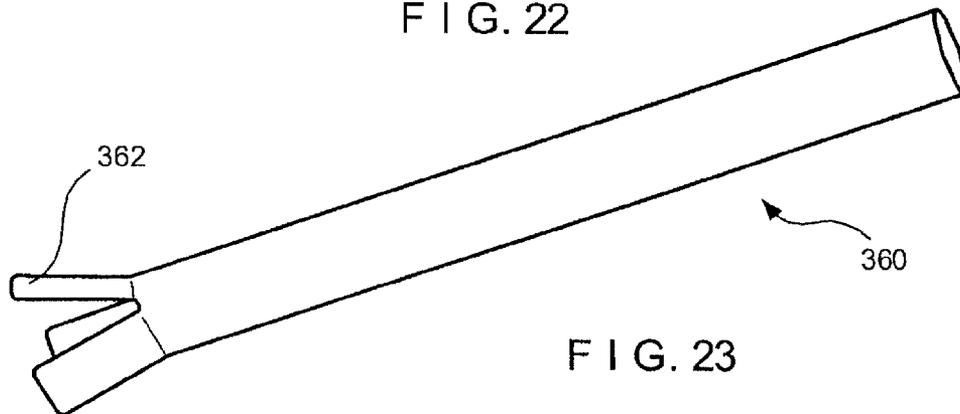


FIG. 23

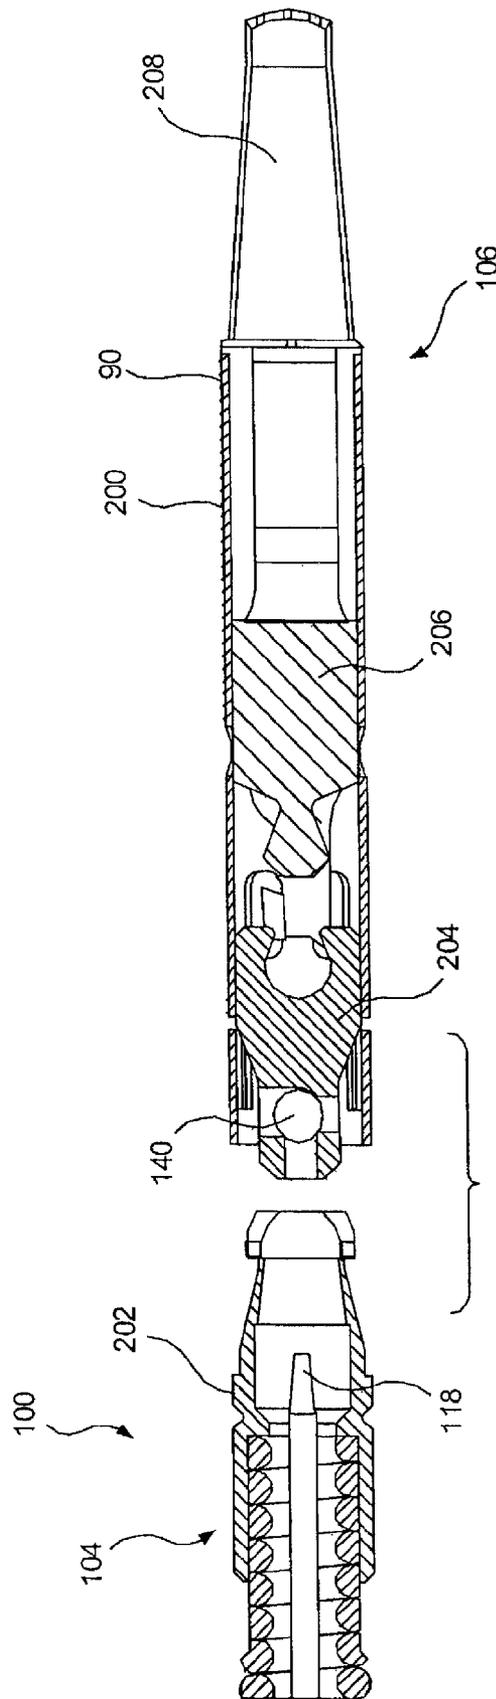


FIG. 24

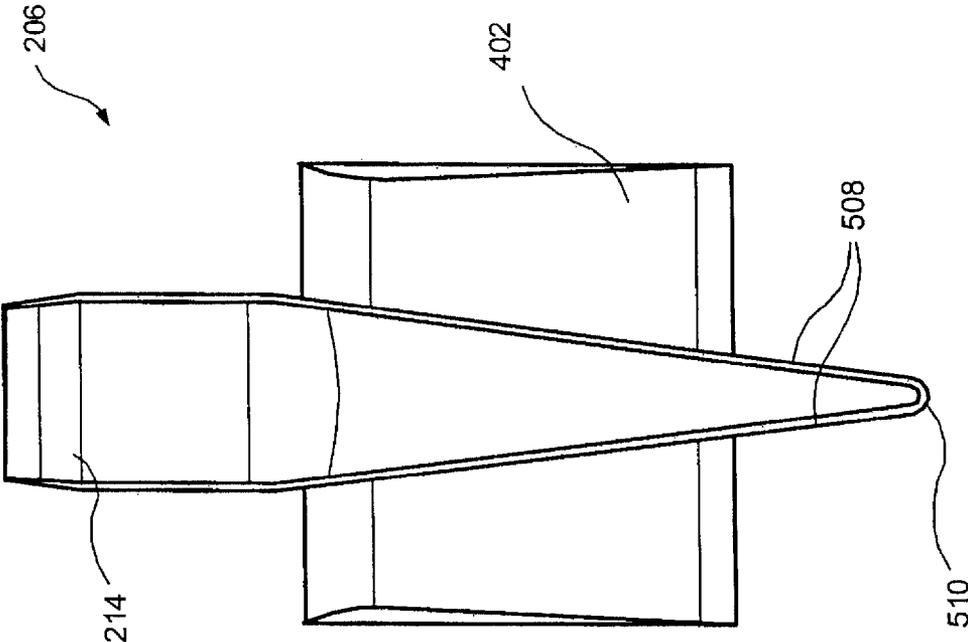


FIG. 26

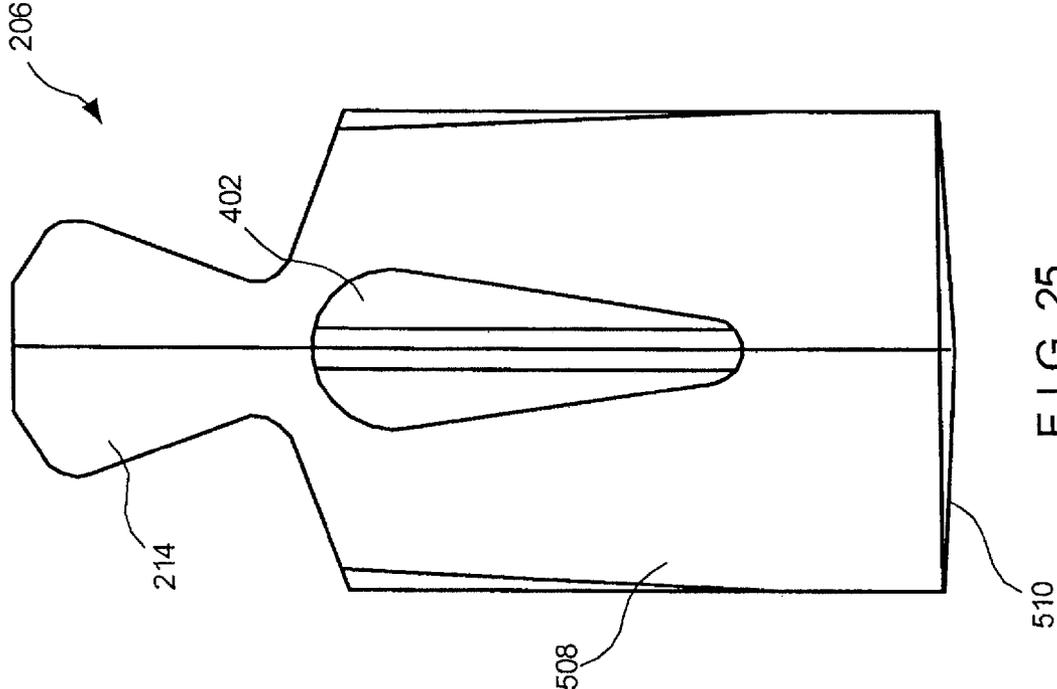


FIG. 25

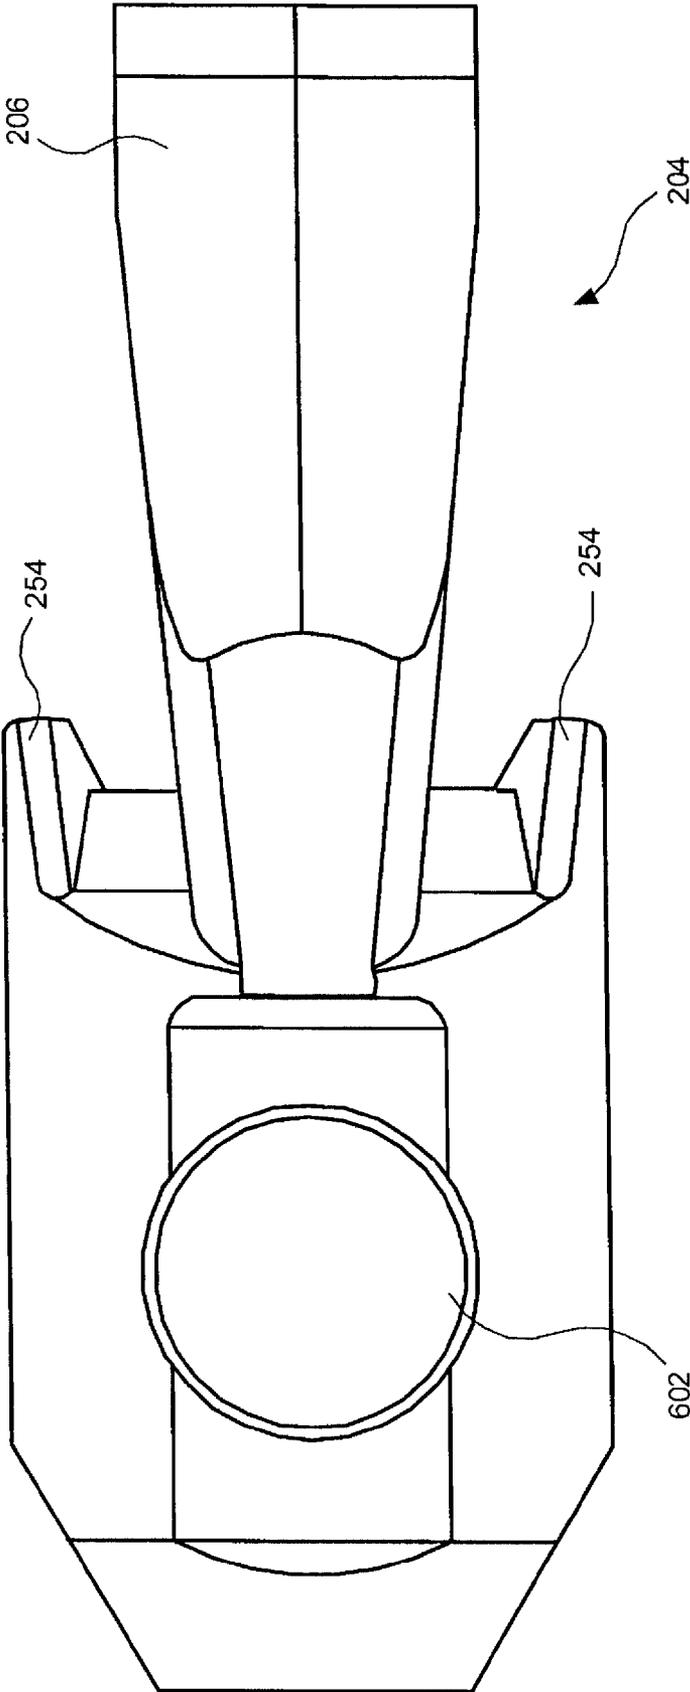


FIG. 27

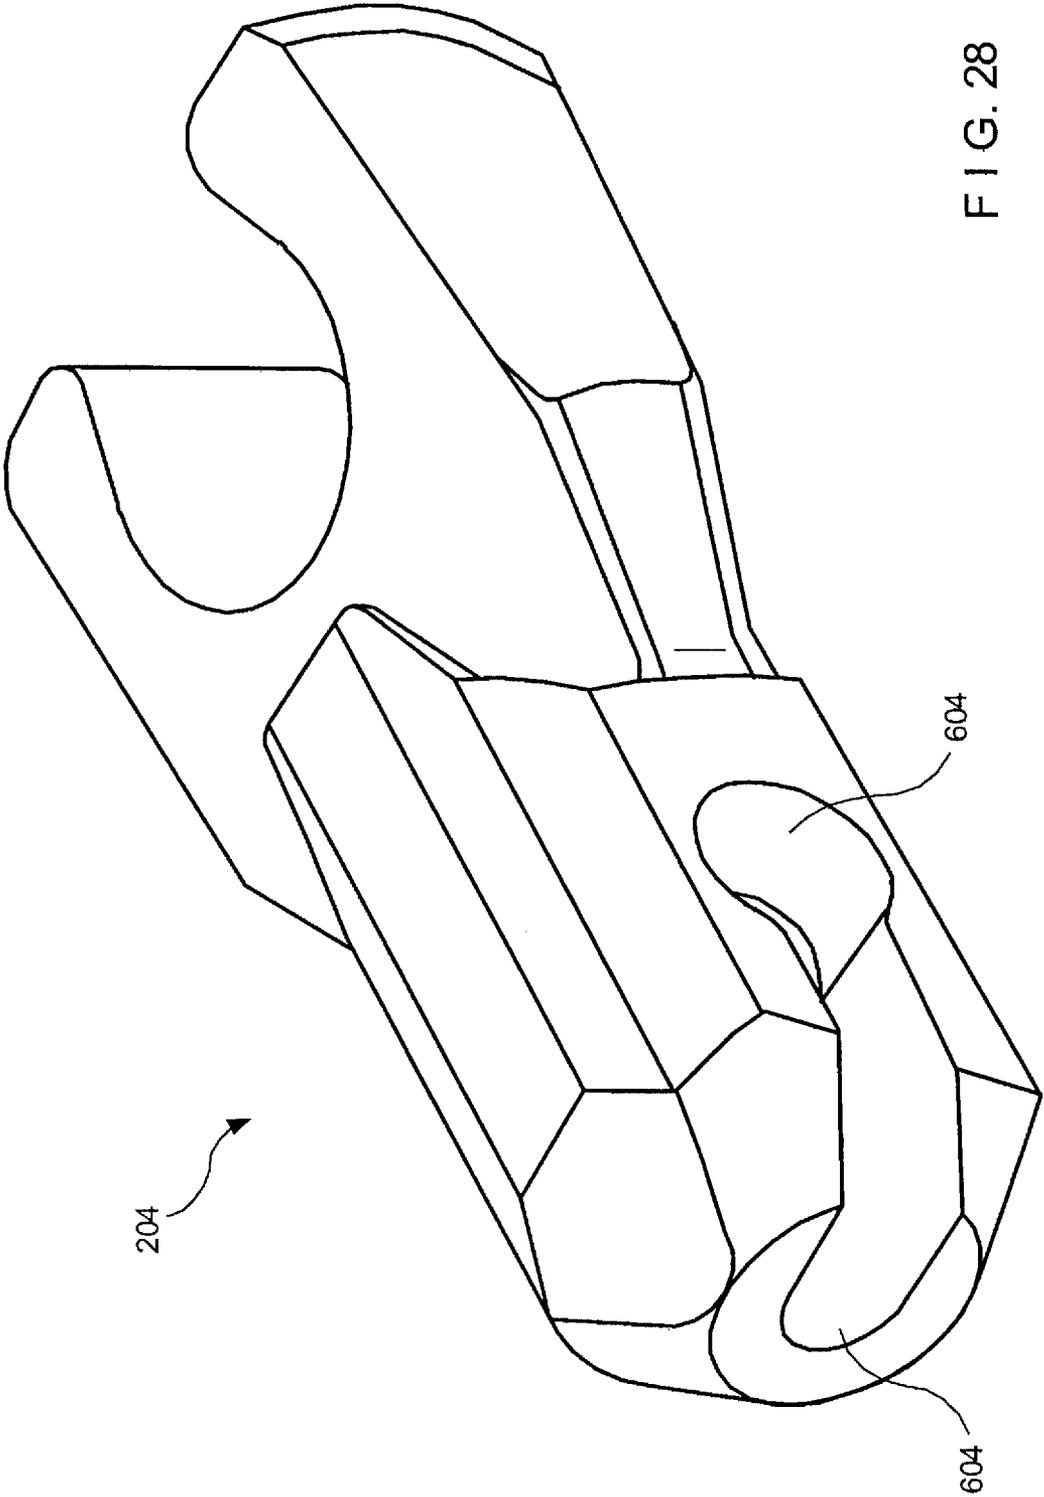


FIG. 28

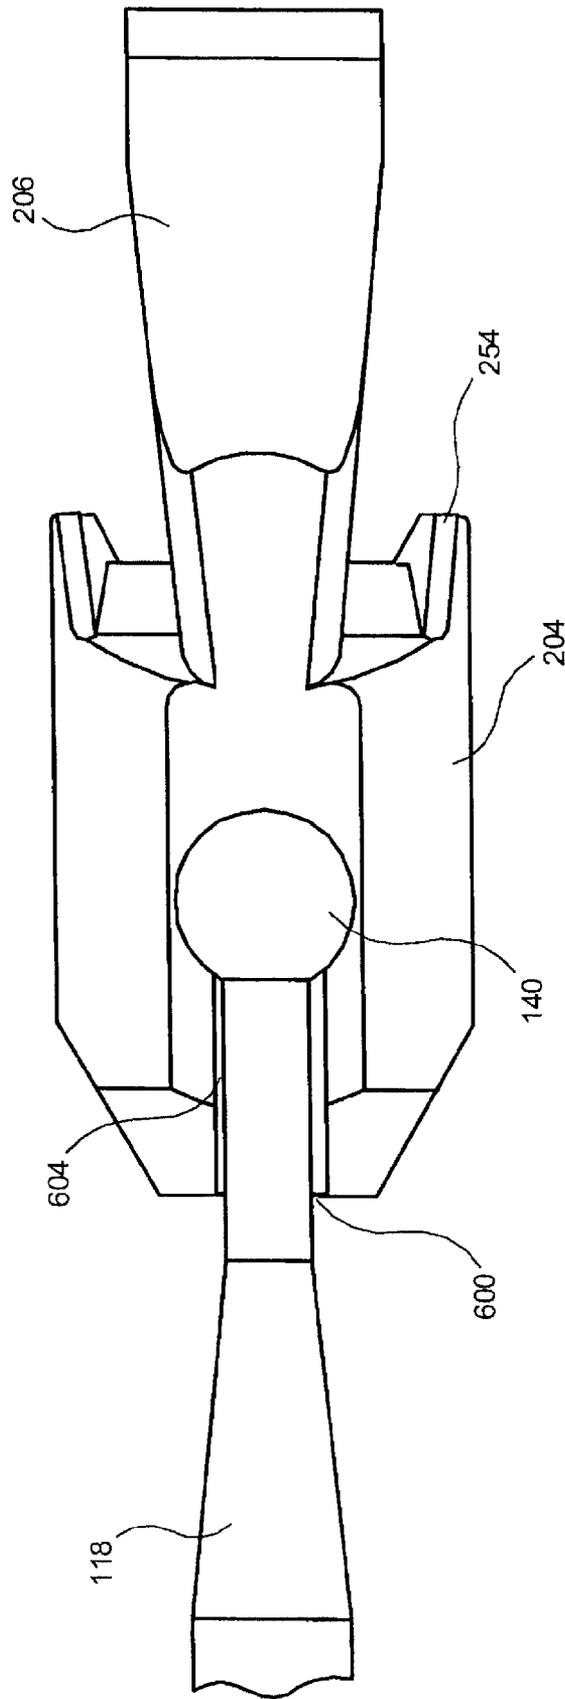


FIG. 29

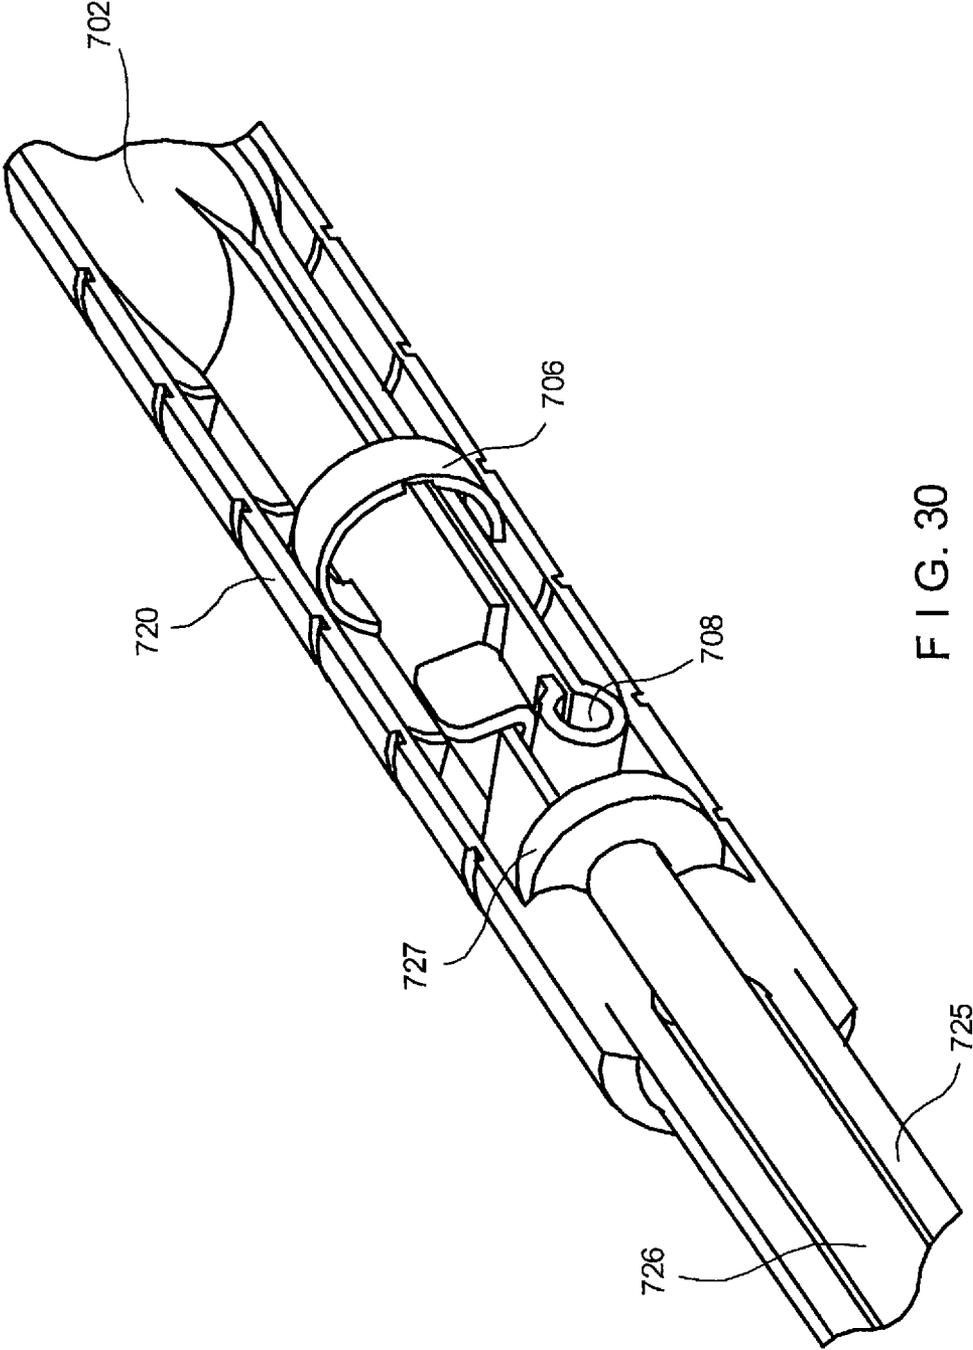


FIG. 30

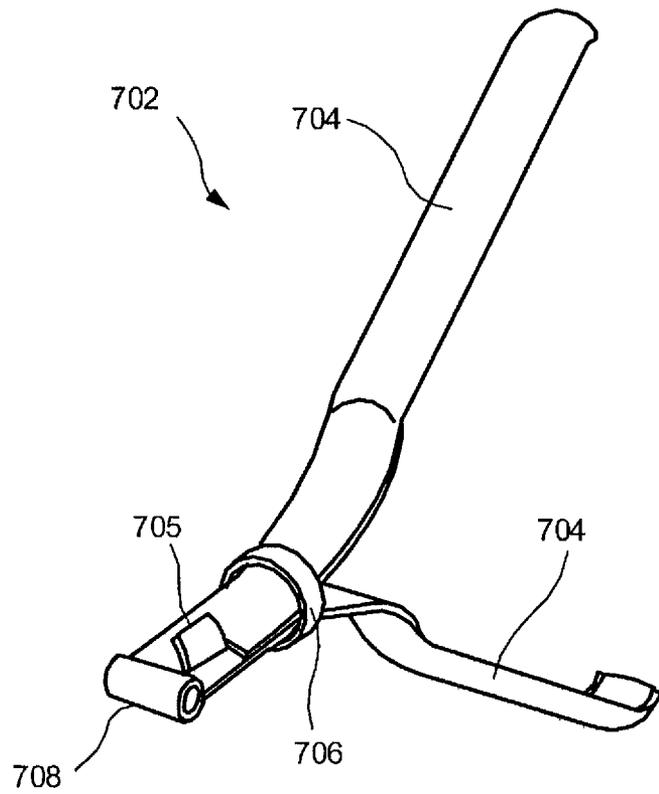
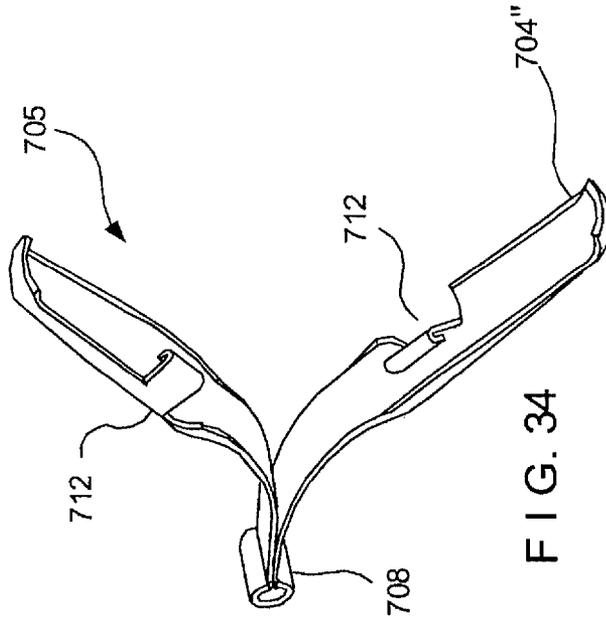
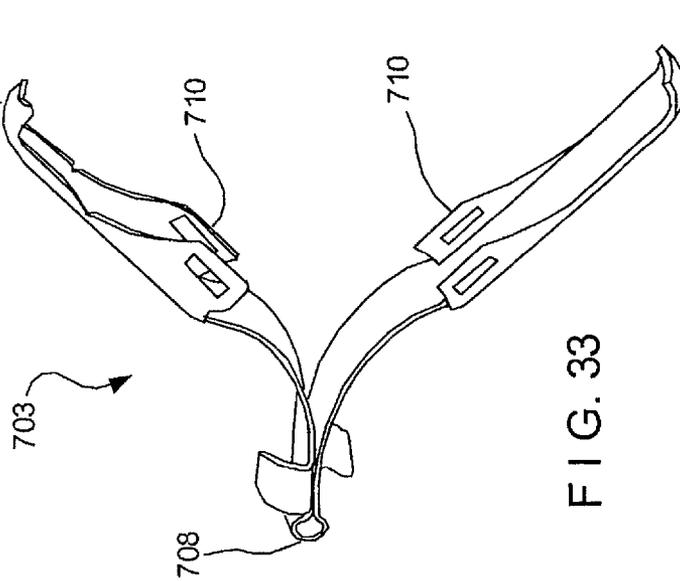
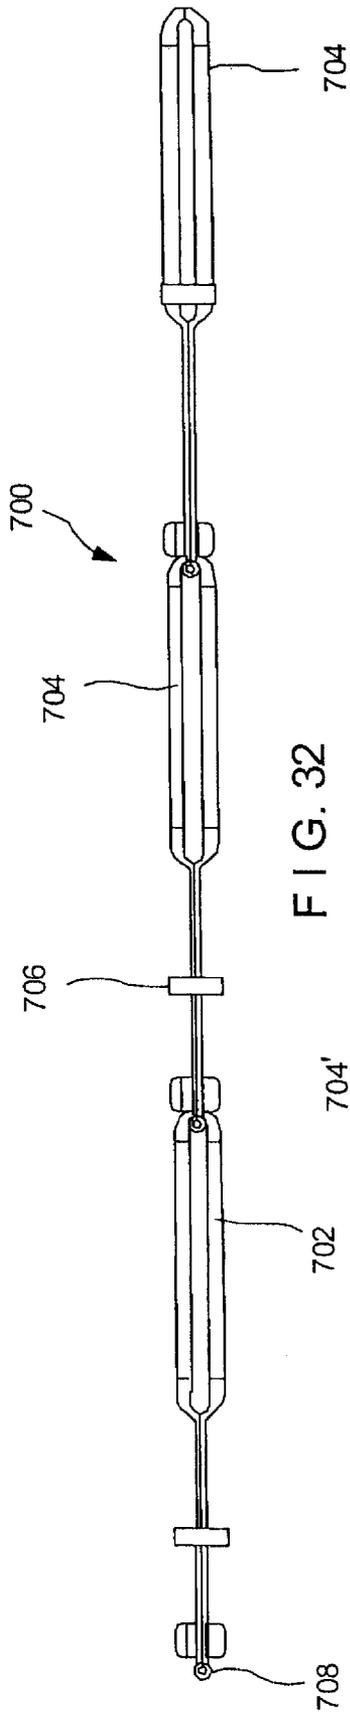


FIG. 31



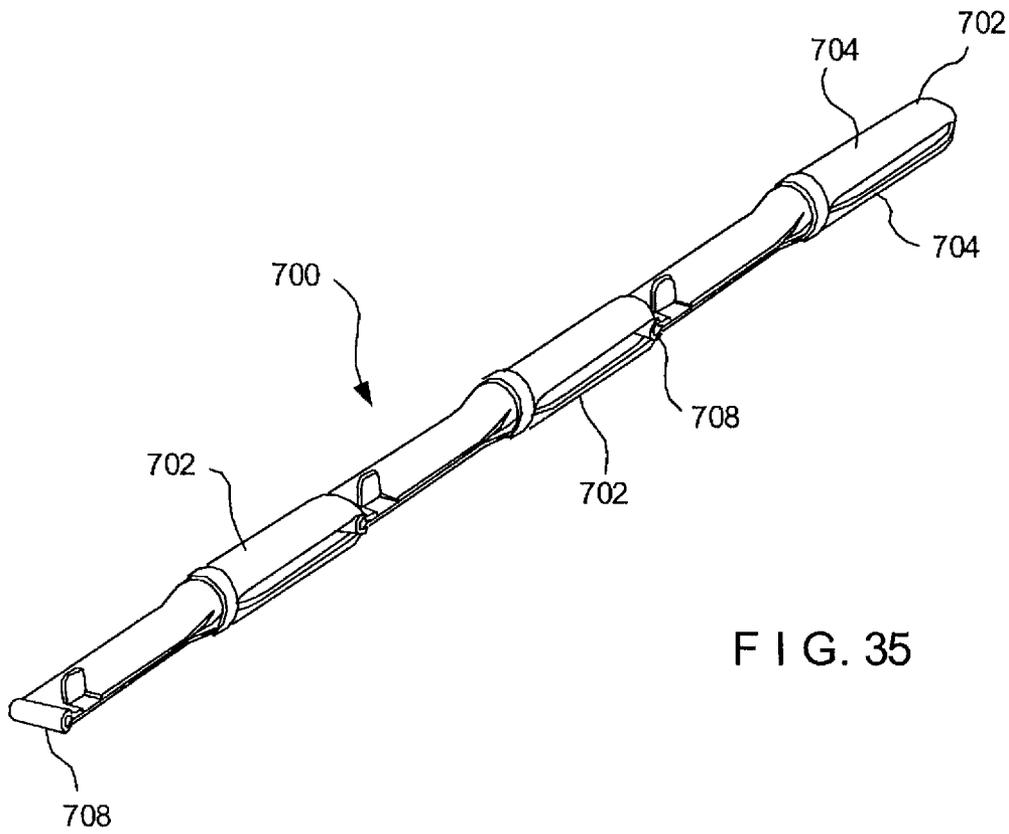


FIG. 35

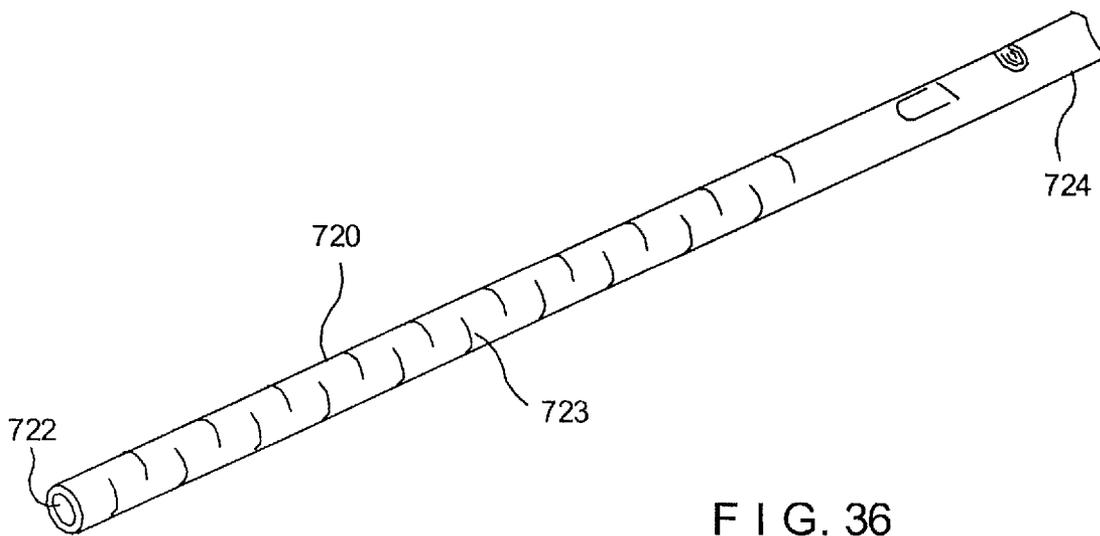


FIG. 36

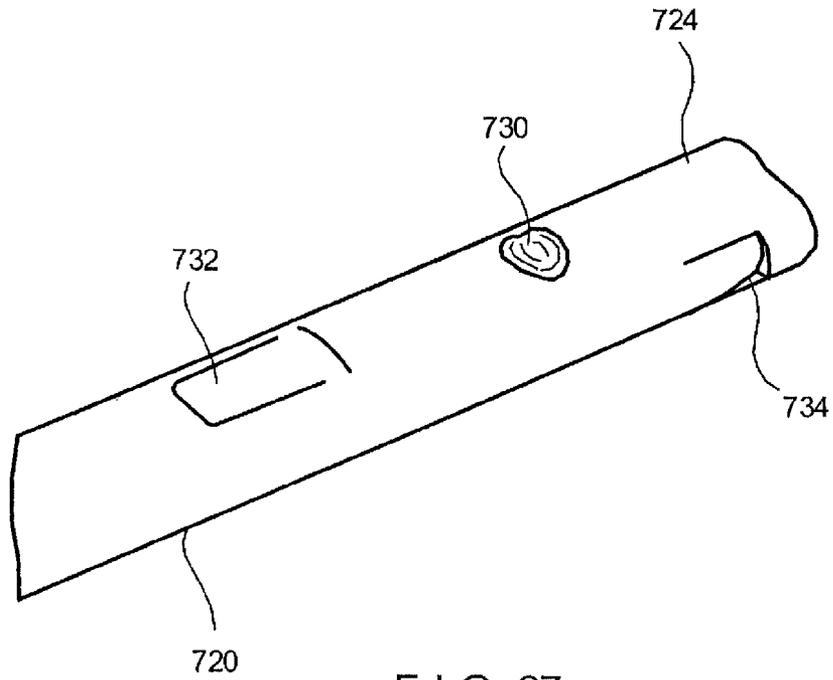


FIG. 37

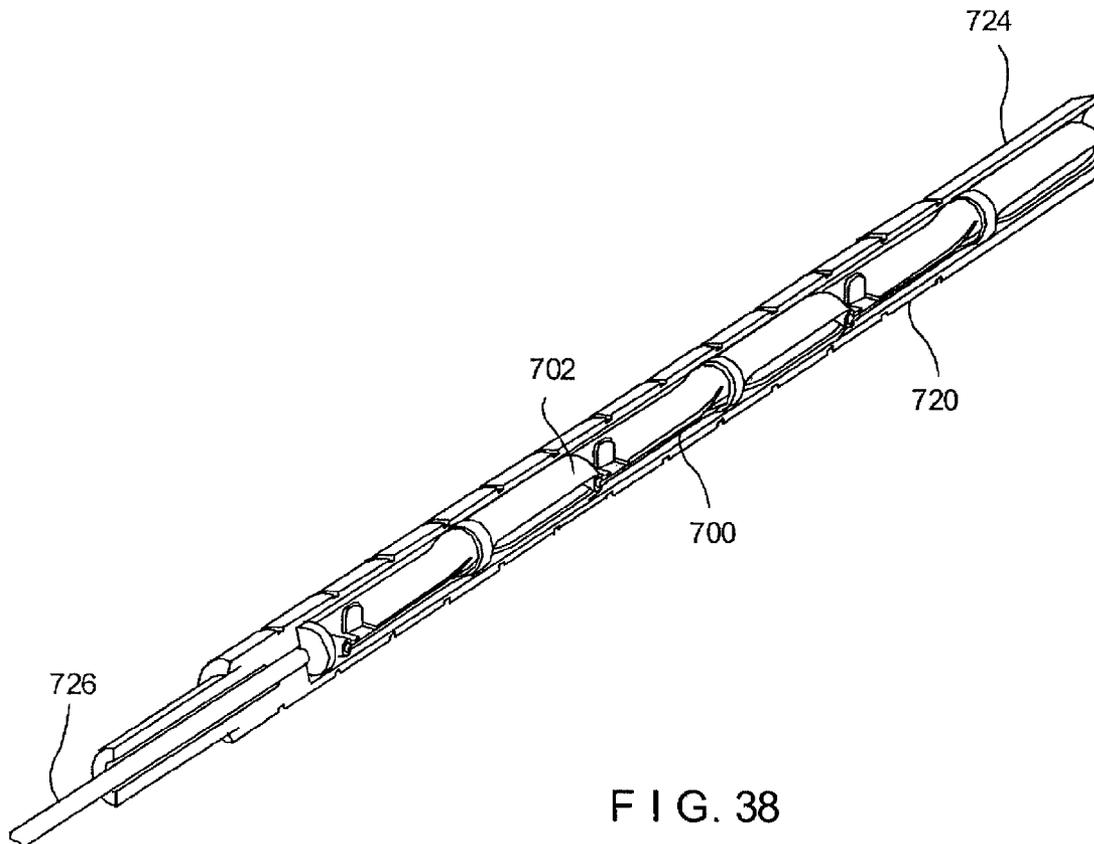


FIG. 38

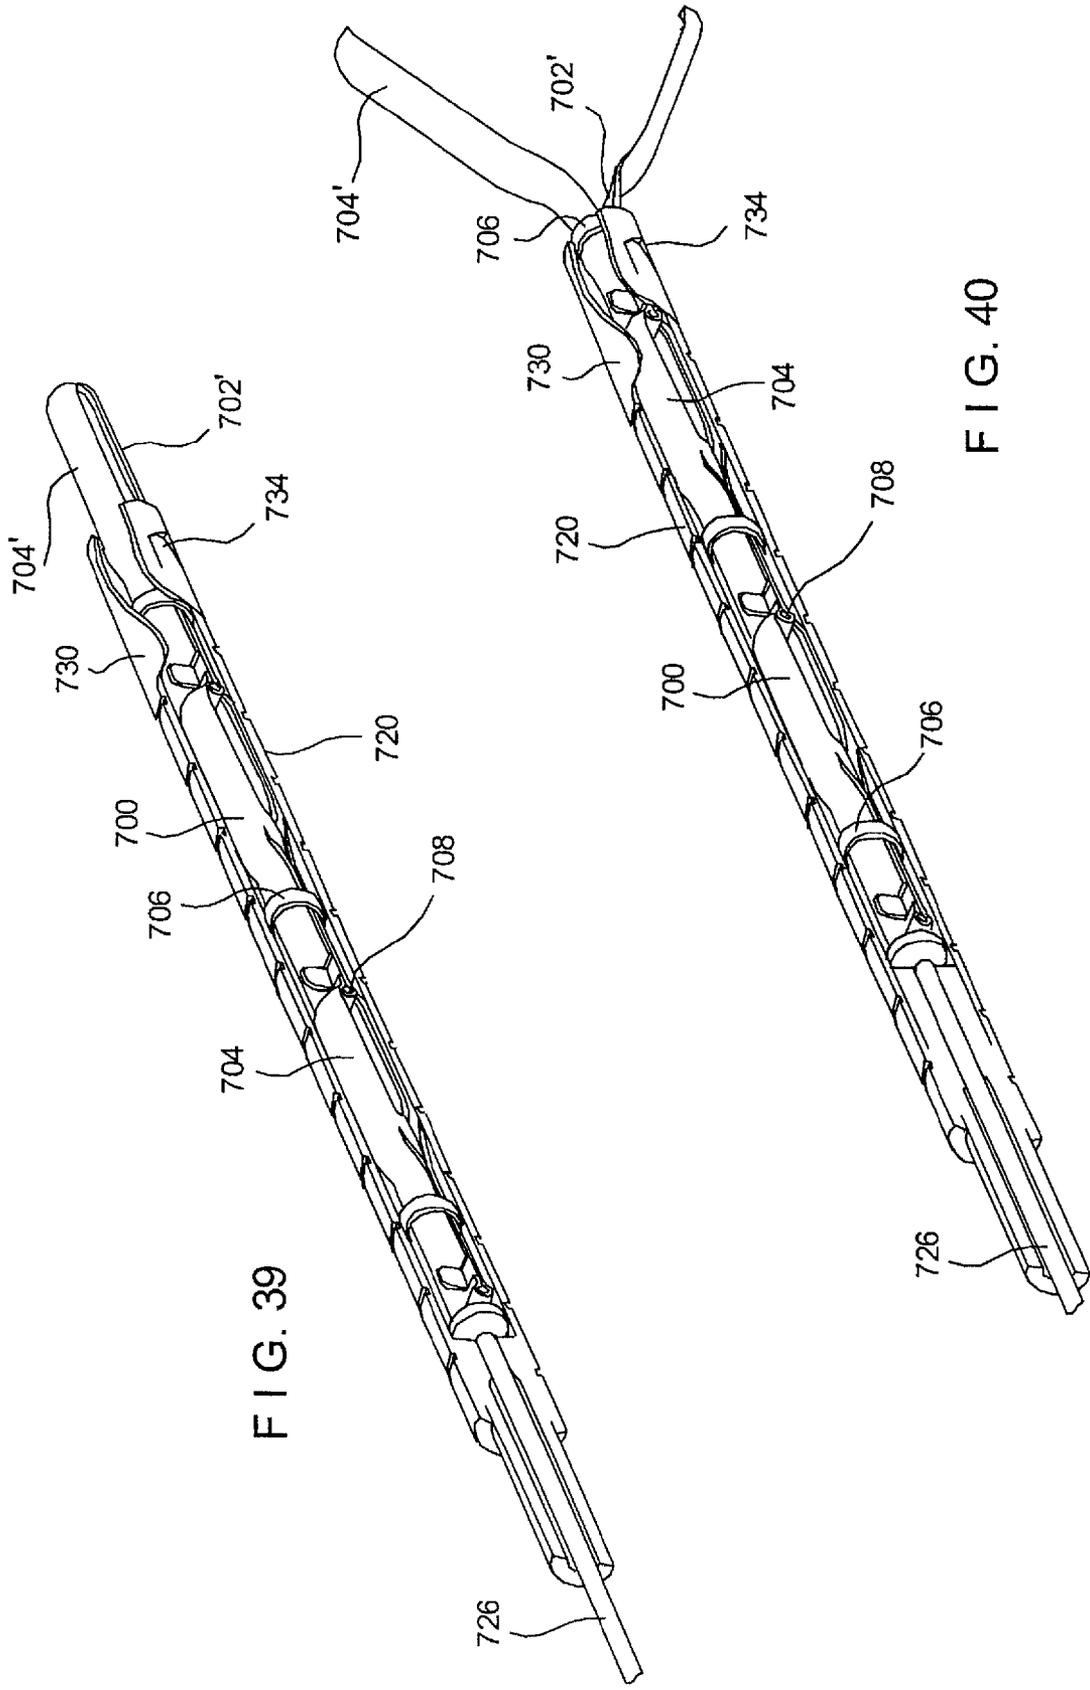


FIG. 39

FIG. 40

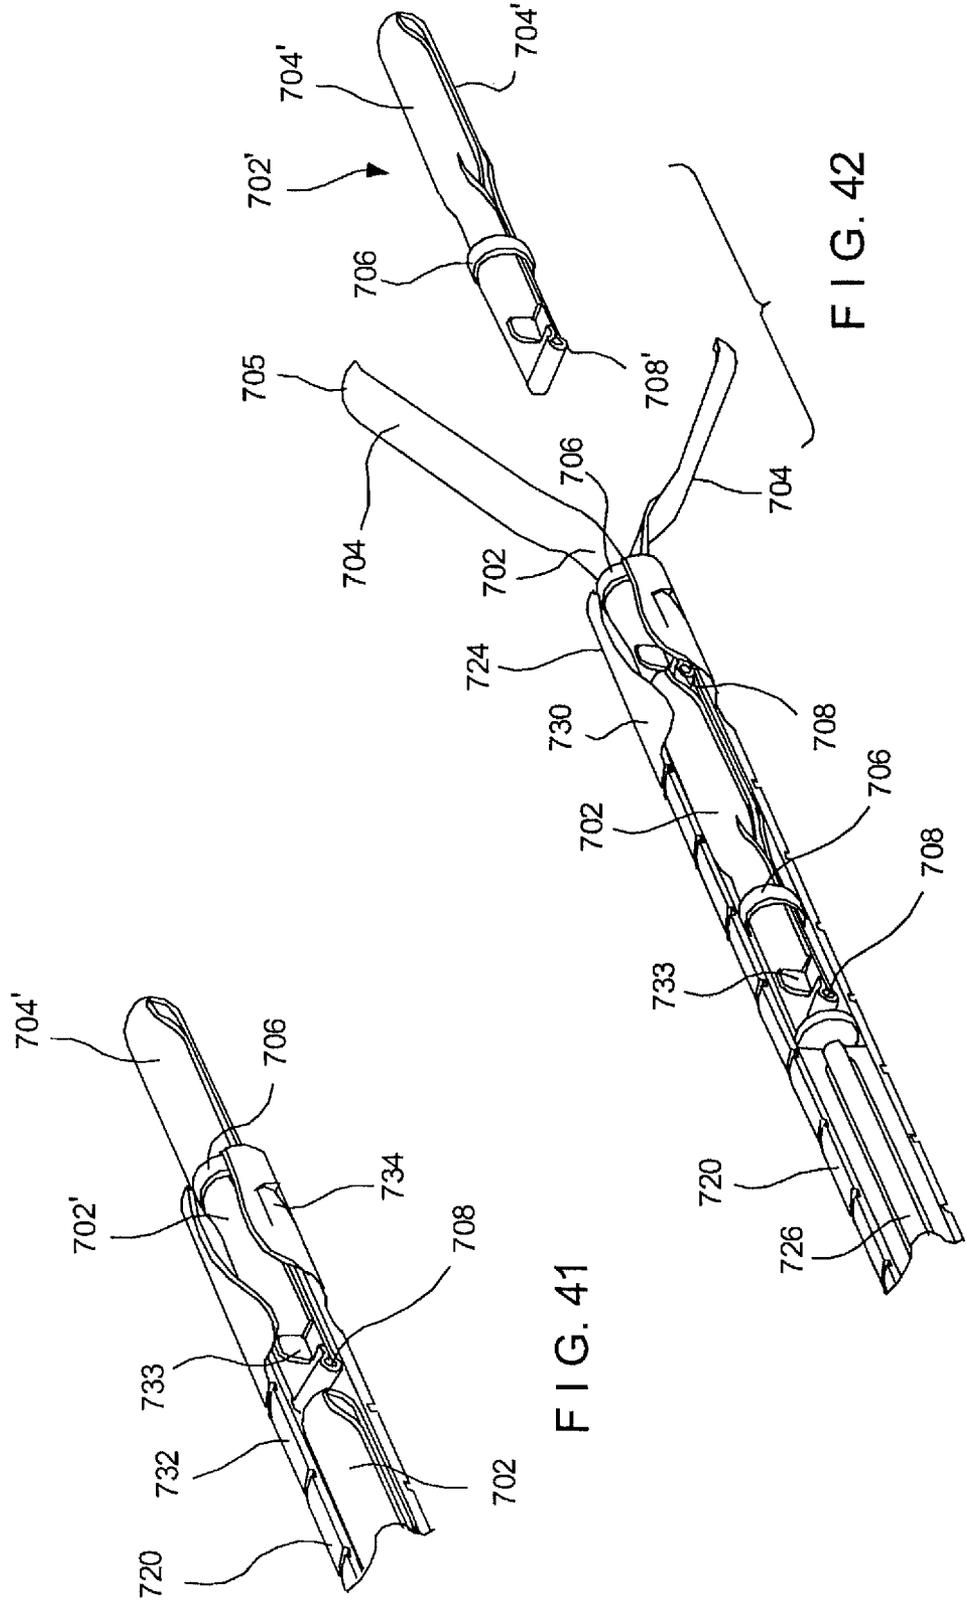


FIG. 41

FIG. 42

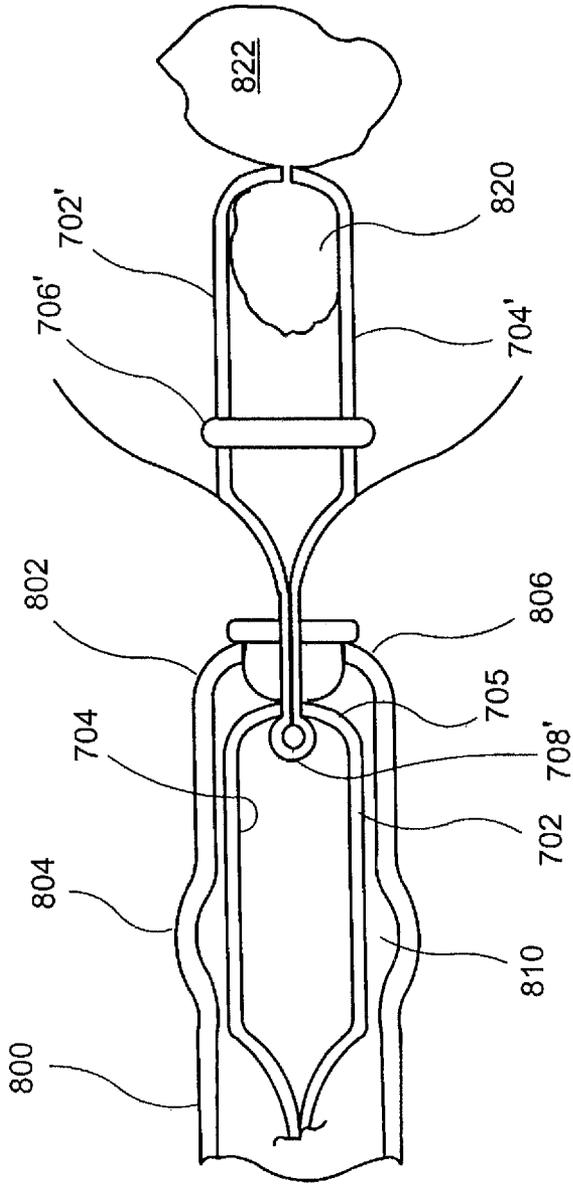


FIG. 43

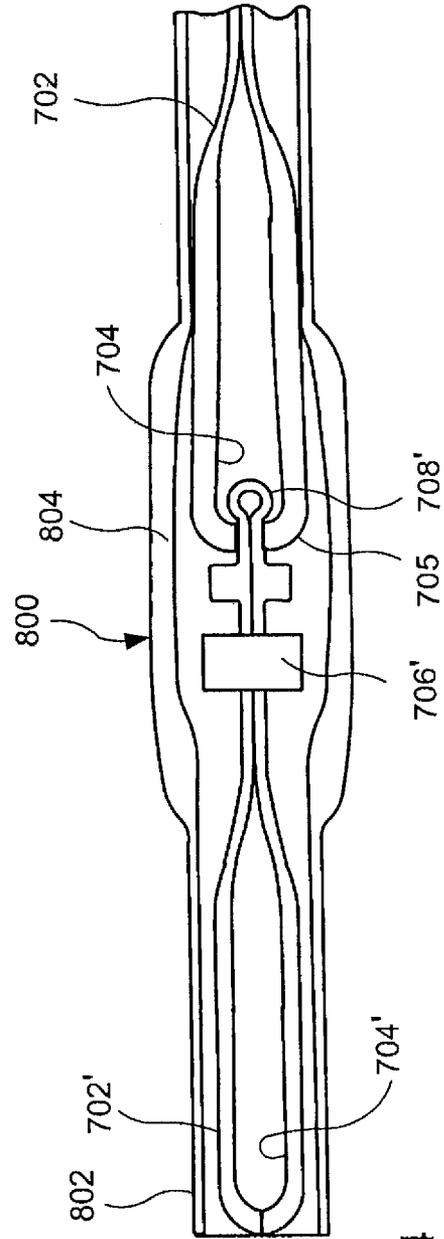


FIG. 44

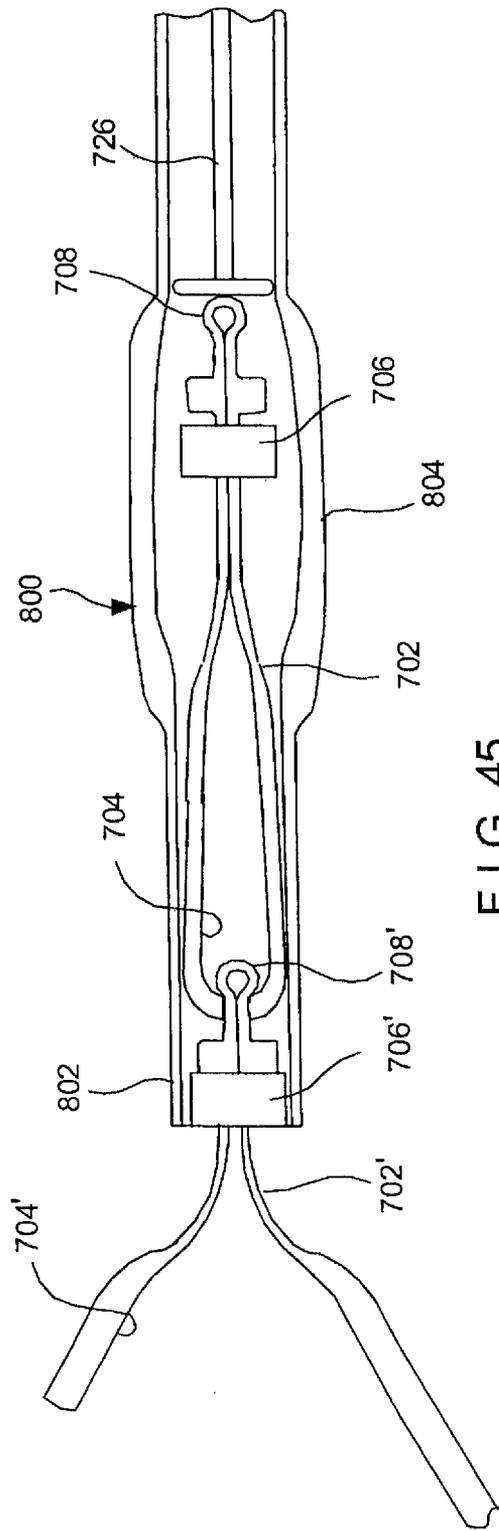


FIG. 45

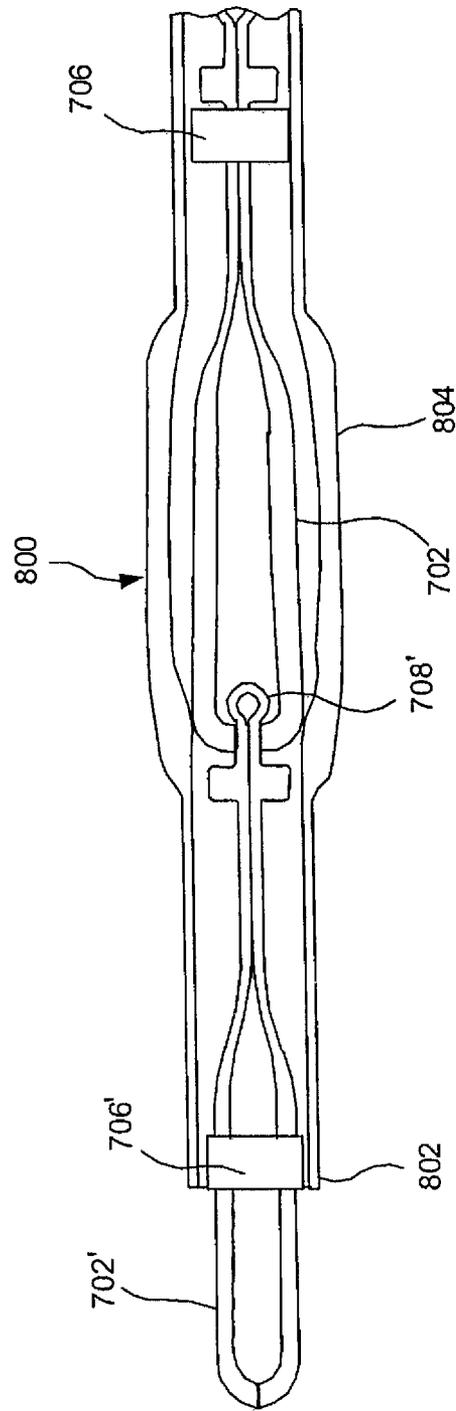


FIG. 46

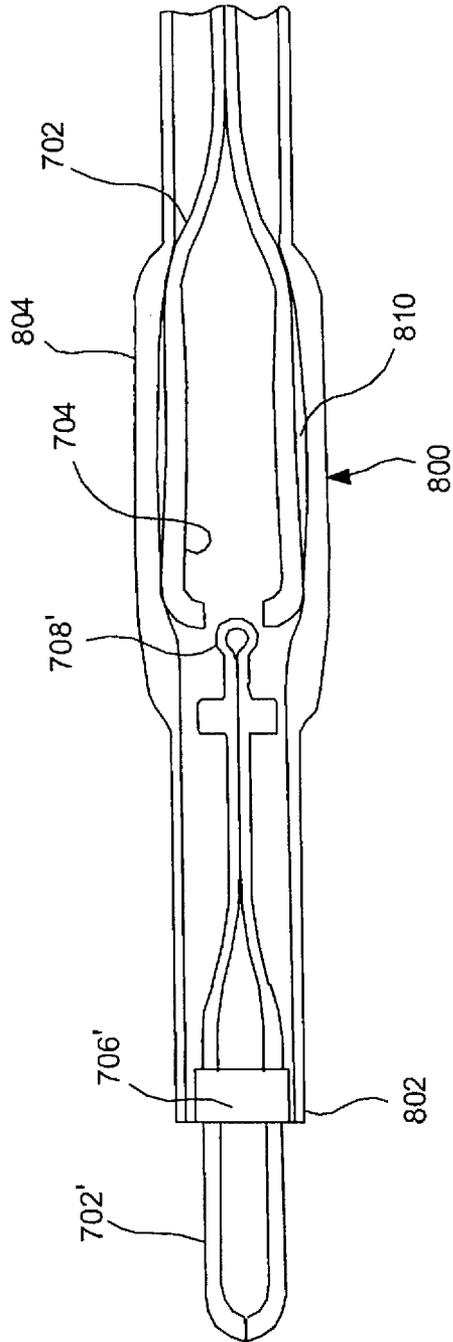


FIG. 47

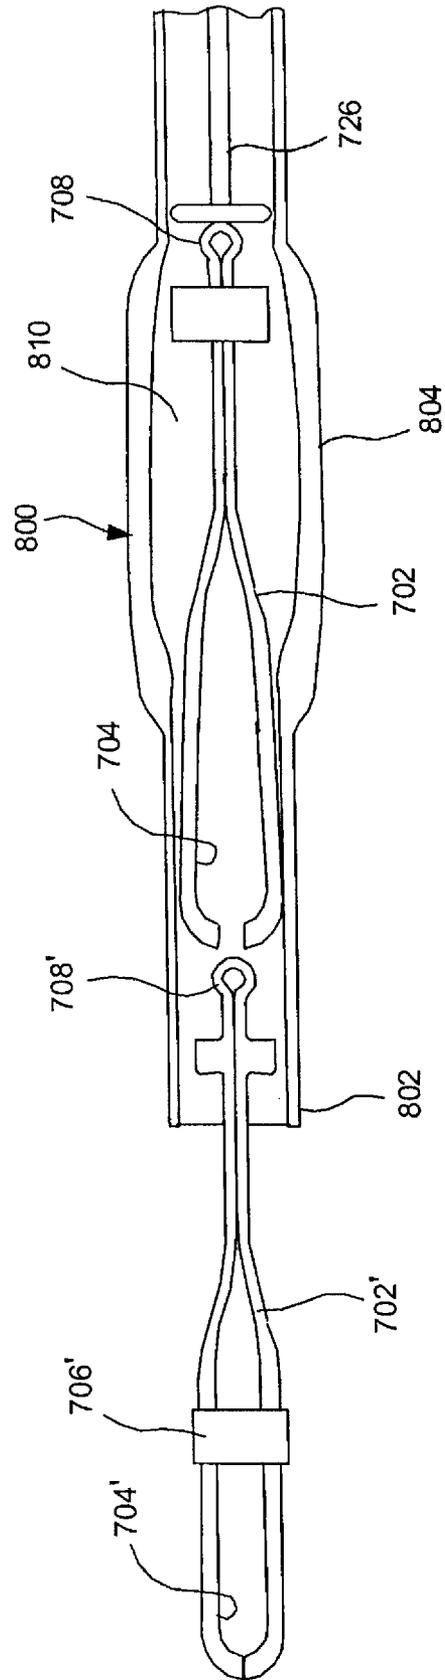


FIG. 48

MULTIPLE CLIP DEPLOYMENT MAGAZINE**PRIORITY CLAIM**

This application is a Continuation application of U.S. patent application Ser. No. 11/032,973 filed on Jan. 11, 2005 entitled "Multiple Clip Deployment Magazine". The application is expressly incorporated herein, in its entirety, by reference.

BACKGROUND

Endoscopic procedures to treat abnormal pathologies of the gastrointestinal ("GI") canal, of the biliary tree, of the vascular system and of various other body lumens are becoming increasingly common. An endoscope is basically a hollow tube placed at a desired location within the body to facilitate access to the relevant body ducts and lumens, etc. The endoscope itself cannot carry out many of the required procedures. To that end, the endoscope is fitted with a lumen, or internal channel, which permits the user to insert various medical devices therethrough to the location that requires treatment. Once the distal end of the inserted device has reached the tissue to be treated, it can be manipulated using controls which remain outside the body.

An hemostatic clipping tool is one of the devices which may be inserted through an endoscope so that treatment may be carried out. Hemostatic clips are deployed from the clipping tool and are used to stop internal bleeding by clamping together the edges of a wound. The clipping tool complete with clips attached to its distal end is inserted through the endoscope to the location of the bleeding. A clip is then remotely manipulated into position over the site of bleeding, clamped over the wound and detached from the tool. After a number of clips sufficient to stop the bleeding has been deployed, the tool is withdrawn from the patient's body through the endoscope. The size and shape of the clips and of the clipping tool are limited by the inner diameter of the endoscope's lumen, thus placing constraints on the design of the clip positioning and release mechanisms.

One challenge facing the endoscope operator is to properly position the hemostatic clips over the wound, so that closing the clips over the tissue will be effective in stopping the bleeding. If a clip is deployed improperly, additional clips may be required to stop the bleeding extending the time required for and the complexity of the procedure and leaving additional medical devices within the patient. It is thus beneficial if the clipping tool allows the user to orient the clips as required during deployment. It is also important for the device operator to be certain of the status of the clip during the deployment operation. For example, before withdrawing the tool from the endoscope, the operator should have positive indication that a clip has fully deployed, and has been released from the tool. At the same time the design of the tool should ensure that clips are fully released after they have been closed over the tissue.

SUMMARY OF THE INVENTION

In one aspect, the present invention is directed to an apparatus for deployment of multiple hemostatic clips, comprising a shaft connected to a handle and a control linkage operatively connected to the handle in combination with a magazine disposed at a distal end of the shaft, the magazine containing a plurality of clips arranged in a chain rotatable within the magazine, wherein a proximal-most one of the clips is coupled to the control linkage. A distal portion of the

magazine is contoured to permit opening of a distal-most one of the clips during a distal stroke of the control linkage and to assist closing and locking of the distal-most clip during a proximal stroke of the control linkage. The magazine includes an expanded chamber sized to allow opening in any rotational orientation of a next clip located immediately proximal to the distal-most clip to a degree sufficient to disengage the distal-most clip from the clip chain.

The present invention is further directed to a method for deploying multiple hemostatic clips, comprising positioning a distal end of a magazine containing a clip chain over selected target tissue and actuating a control link of the magazine in a distal stroke to open and distally translate a distal-most clip of the clip chain in combination with orienting the open distal-most clip in a desired orientation to grasp the target tissue and actuating the control link in a proximal stroke to close and lock the distal-most clip over the target tissue. The control link is further actuated in the proximal stroke to move a next clip immediately proximal to the distal-most clip into an expanded portion of the magazine sized to allow the next clip to open to a degree sufficient to release the distal-most clip from the clip chain regardless of a circumferential orientation of the next clip and the distal-most clip is released by partially opening the next clip.

BRIEF DESCRIPTION OF THE DRAWINGS

FIG. 1 is a schematic side view of a clipping device according to an embodiment of the present invention, with FIG. 1A showing a detail view of an exemplary clip assembly;

FIG. 2 is a schematic side view of the embodiment shown in FIG. 1, with an outer sheath;

FIG. 3 is a cut away side view of the shaft section according to an embodiment of the present invention;

FIG. 4 is a cross sectional view of the shaft section shown in FIG. 3;

FIG. 5 is a detail view of the distal end of the control wire according to an embodiment of the present invention;

FIG. 6 is a perspective view of an outer sheath according to an embodiment of the present invention;

FIG. 7 is an cross sectional exploded view of the handle of the outer sheath shown in FIG. 6;

FIG. 8 is a perspective view of an outer sheath lock according to an embodiment of the present invention;

FIG. 9 is a cross sectional side view of a distal end of a clipping device according to an embodiment of the present invention;

FIG. 10 is a cross sectional top view of a distal end of the clipping device shown in FIG. 9;

FIG. 11 is a perspective view of the distal end of the clipping device shown in FIG. 9;

FIG. 12 is a top view of the clip arms according to an embodiment of the present invention;

FIG. 13 is a perspective view of the clip arms shown in FIG. 12, according to an embodiment of the present invention;

FIG. 14 is a perspective view of a capsule according to an embodiment of the present invention;

FIG. 15 is a cross sectional side view of the of the capsule shown in FIG. 14;

FIG. 16 is a top view of the distal end of a clipping device according to an embodiment of the present invention;

FIG. 17 is a side view of the distal end shown in FIG. 16;

FIG. 18 is a perspective view of a clip arm according to an embodiment of the present invention;

FIG. 19 is a side view of the clip arm shown in FIG. 18;

FIG. 20 is a top view of the clip arm shown in FIG. 18;

FIG. 21 is a perspective view of a bushing according to an embodiment of the present invention;

FIG. 22 is a cross sectional side view of the bushing shown in FIG. 21;

FIG. 23 is a perspective view of a wire stop according to an embodiment of the present invention;

FIG. 24 is a schematic side view of a clip assembly detached from a bushing, according to an embodiment of the present invention;

FIG. 25 is a side view of a tension member according to an embodiment of the present invention;

FIG. 26 is a top view of the tension member shown in FIG. 25;

FIG. 27 is a top view of a yoke according to an embodiment of the present invention;

FIG. 28 is a perspective view of the yoke shown in FIG. 27;

FIG. 29 is a top view of a yoke with a control wire according to an embodiment of the present invention;

FIG. 30 shows a detail of a connection between a control link and a clip chain according to an embodiment of the invention;

FIG. 31 shows a perspective view of an individual hemostatic clip of a clip chain according to an embodiment of the invention;

FIG. 32 shows a side elevation view of a clip chain according to an embodiment of the invention;

FIG. 33 shows a perspective view of a second embodiment of a clip for a clip chain according to the invention;

FIG. 34 shows a perspective view of a third embodiment of a clip for a clip chain according to the invention;

FIG. 35 shows a perspective view of the clip chain shown in FIG. 32;

FIG. 36 shows a perspective view of a clip magazine according to an embodiment of the invention;

FIG. 37 shows a distal end detail of the clip magazine shown in FIG. 36;

FIG. 38 shows a cut away perspective view of a clip chain loaded in a clip magazine according to an embodiment of the invention;

FIG. 39 shows the clip chain of FIG. 38 being pushed out of the clip magazine;

FIG. 40 shows the clip chain of FIG. 38 yet further out of the clip magazine with one clip deployed;

FIG. 41 shows a distal end detail of the clip magazine shown in FIG. 39;

FIG. 42 shows the clip chain of FIG. 38 with a clip deployed and released from the clip chain;

FIG. 43 is a schematic diagram showing a detail of the magazine as clips according to an embodiment of the present invention;

FIG. 44 is a cut-away diagram showing two clips in the magazine in a pre-deployment configuration;

FIG. 45 is a cut-away diagram showing one of the clips shown in FIG. 44 with open clip arms;

FIG. 46 is a cut-away diagram showing one of the clips of FIG. 44 being locked in the closed configuration;

FIG. 47 is a cut-away diagram showing one of the clips of FIG. 44 being disconnected from the other clip; and

FIG. 48 is a cut-away diagram showing one of the clips of FIG. 44 deployed from the magazine.

DETAILED DESCRIPTION

Hemostatic clips are used routinely to stop bleeding from openings created during surgery as well as wounds resulting from other trauma to tissues. In the simplest form, these clips grasp the tissue surrounding a wound and bring the wound's

edges together, to allow the natural scarring process to heal the wound. Endoscopic hemostatic clips are used to stop internal bleeding due resulting from surgical procedures and/or tissue damage from disease, etc. Specialized endoscopic hemostatic clipping devices are used to bring the clips to the desired location within a patient's body and to position and deploy the clip at the appropriate place on the tissue. The clipping device is then withdrawn, leaving the clip within the patient. Such hemostatic clipping devices are described in U.S. patent application Ser. No. 10/647,512, filed on Sep. 30, 2003, and Provisional U.S. Patent Application Ser. No. 60/518,167 which are hereby incorporated herein by reference in their entirety.

Endoscopic hemostatic clipping devices are designed to reach affected tissues deep within a patient's body, such as within the GI tract, the pulmonary system, the vascular system or within other lumens and ducts. During the procedures to treat those areas, an endoscope is generally used to provide access to and visualization of the tissue which is to be treated. The clipping device may, for example, be introduced through a working lumen of the endoscope. The design and construction of such a "through the scope" endoscopic hemostatic clipping device presents several challenges. The endoscopic clipping device has to be sufficiently small to fit in the lumen of an endoscope and, at the same time, must be designed to provide for the positive placement and actuation of the hemostatic clip. Feedback to the operator is preferably also provided so that the operator will not be confused as to whether the hemostatic clip has been properly locked in place on the tissue and released from the device before the device itself is withdrawn through the endoscope.

FIG. 1 shows a side elevation view of a through the scope hemostatic clipping device according to an exemplary embodiment of the present invention. This device is a hand operated tool that is used to insert a hemostatic clip through an endoscope lumen, position the clip over a wound, clamp it and deploy it over the affected tissue. The tool is further designed to release the hemostatic clip once it has been clamped in place, and to be withdrawn through the endoscope. To more clearly explain the operation and construction of the exemplary device, it may be divided into three principal components. As shown, the hemostatic clipping device 100 comprises a handle assembly 102, a shaft section 104, and a clip assembly 106. The clip assembly 106 is shown more clearly in FIG. 1A.

Handle assembly 102 forms the component that supplies a mechanical actuation force to deploy and clamp the clip. In this embodiment, the device is hand operated (i.e., the user's hands provide the force required to carry out all the functions related to the hemostatic clip). The handle assembly 102 may be constructed in a manner similar to conventional handle assemblies of the type generally employed in endoscopic biopsy devices or in similar applications. The handle assembly 102 allows the user to move a control wire 118 or other force transmission member, which extends through the shaft section 104 to the clip assembly 106 at a distal end of the device 100. The handle assembly 102 comprises a handle body 108 which can be grasped by the user to stabilize the device and apply a force to it. A sliding spool 110 is connected to control wire 118, so that the user can easily pull or push said wire 106 as desired.

As shown in FIGS. 1 and 2, a sliding spool 110 is mounted on the handle body 108 so that it can slide along a slot 116, which maintains its position within the handle assembly 102. Because the sliding spool 110 is connected to the control wire 118, the user may manipulate the control wire 118 by grasping the handle body 108 and moving the sliding spool 110

5

along the slot 116. A return spring 112 may be provided within the handle body 108 to bias the sliding spool 110, and thus the control wire 118 toward a desired position. In the present embodiment, the sliding spool 110 is biased to the proximal position. The handle assembly 102 may also include a connection portion 114, which receives the control wire 118 and attaches the shaft section 104 to the handle assembly 102.

The shaft section 104 mechanically connects the handle assembly 102 to the clip assembly 106 and, together with the clip assembly 106, is designed to be inserted into a lumen of an endoscope. As shown in FIGS. 3 and 4, the shaft section 104 comprises an outer flexible coil 130 which is designed to transmit a torque from the proximal end to the distal end of the device 100 and to provide structural strength to the shaft section 104. The coil 130 may be a conventional coil used in biopsy devices and may, for example, comprise a single, coiled wire. The coiled wire may have a round, square or a rectangular cross section, and may be made of a biocompatible material such as, for example, stainless steel. Additional protective and low friction outer layers may be included on the shaft section 104, according to known methods of construction.

The control wire 118 transmits mechanical force applied to the handle 102 to the clip assembly 106. The control wire 118 has a proximal end which is attached to a movable part of the handle 102, such as the sliding spool 110, using known methods. Stainless steel or other high yield biocompatible materials may be used to manufacture the control wire 118, so that the structural integrity of the assembly is maintained. It is also important to prevent stretching of the control wire 118 when under tension since, if the wire stretches, the handle 102 will have to travel a greater distance to carry out a desired operation. As shown in FIG. 5, the distal end of the control wire 118 ends in a ball 140 which is used to connect the control wire 118 to the appropriate elements of the clip assembly 106, as will be described below. In this embodiment, the diameter of the control wire 118 is substantially constant from a proximal end thereof to a proximal end of a distal tapered section 144. The ball 140 may have a diameter which is greater than the diameter of the control wire 118, to facilitate attachment to a yoke 204. The control wire 118 may extend the length of the device 100, from the yoke 204 to the sliding spool 110, and may be designed to slide longitudinally along the device 100. It may be made, for example, of stainless steel or other biocompatible metal.

The control wire 118 may also include a reduced diameter section 142 designed to fail when a predetermined tension is applied thereto through the handle assembly 102. The tapered section 144 may be used to transition between the main body of the control wire 118 and the reduced diameter section 142, without steps or other discontinuities which may concentrate stress and make the fracture point more unpredictable. As will be described in greater detail below, one purpose of the reduced diameter section 142 is to facilitate the release of a hemostatic clip from the hemostatic clipping device 100 once the clip has been properly deployed. It will be apparent to those of skill in the art that the location of the reduced diameter section 142 along control wire 118 may be varied to take into account specific requirements of the device 100.

An inner sheath 132 may be used in the construction of the shaft section 104, as shown in FIGS. 3 and 4. The inner sheath 132 provides a low friction bearing surface disposed between the outer diameter of the control wire 118, and the inner diameter of the shaft section 104. The inner sheath 132 may be formed of a low friction material such as, for example, Teflon™, HDPE or Polypropylene. In one exemplary embodiment, the inner sheath 132 is slidable within the shaft

6

section 104, and the control wire 118 is slidable within the inner sheath 132 forming a low friction system of multiple bearing surfaces. To further reduce friction, a bio-compatible lubricant may be applied to the inner and outer surfaces of the inner sheath 132, along the length of the shaft section 104. For example, silicone lubricants may be used for this purpose.

A slidable over-sheath 150 may be included in the design of the shaft section 104, as shown in FIGS. 1 and 2. The over-sheath 150 is designed to protect the inner lumen of the endoscope from the metal clip assembly 106 and from the metal coil 130 while the hemostatic clipping device 100 passes through the endoscope's lumen. After the clipping device 100 and, more specifically, after the clip assembly 106 has passed through the endoscope, the over-sheath 150 may be withdrawn to expose the distal portion of the clipping device 100. The over-sheath 150 may be formed, for example, as a single lumen plastic extrusion element slidable over the distal portions of the clipping device 100 to selectively cover and uncover the clip assembly 106. In one embodiment, the over-sheath 150 is formed of a low friction polymer such as, for example, Teflon™, HDPE, Polypropylene, or similar materials.

The over-sheath 150 may include a grip portion 152 and an elongated body 154. The grip portion 152 is designed as a handle making it easier for the user to slide the over-sheath 150 over the shaft of the clipping device 100. In one exemplary embodiment, the grip portion 152 is made of a rubber-like material to provide a good gripping surface for the user. For example, an injection moldable polymer such as TPE may be used to construct the grip portion 152. The elongated body 154 may be formed as a substantially cylindrical shell surrounding the shaft of the clipping device 100. The elongated body 154 may be attached to the grip portion 152 using conventional methods as would be understood by those skilled in the art.

As shown in FIGS. 6 and 7, an exemplary grip portion 152 comprises a central hollow channel 160 that may be used to receive the shaft of the clipping device 100. The central hollow channel 160 is aligned with the elongated body 154 to provide a continuous channel containing the shaft of the clipping device 100. The material of the grip portion 152 may have a high coefficient of friction, so that an interference fit is possible between the central hollow channel 160 and the shaft of the clipping device 100 without the use of adhesives or mechanical fastening devices. In one embodiment, friction bosses 158 may be provided on an inner diameter of the hollow channel 160 to provide additional friction between the shaft of the clipping device 100 and the over-sheath 150 assembly. The friction bosses 158 may be formed, for example, as protrusions extending from the inner diameter of the over-sheath 150 and may have a variety of stubby or elongated shapes. The amount of friction between these two components may be balanced so that no unwanted relative movement takes place while, at the same time, making it relatively easy for the user to slide the over-sheath 150 proximally and distally when necessary.

A sheath stop 156 may be provided for the clipping device 100 to prevent the over-sheath 150 from sliding away from the distal end while the clipping device 100 is inserted in the endoscope. As shown in the exemplary embodiment of FIGS. 2 and 8, the sheath stop 156 physically blocks the grip portion 152 from sliding proximally to prevent the over-sheath 150 from being withdrawn and exposing the clip assembly 106. The sheath stop 156 is designed to easily snap in place near the proximal end of the shaft section 104 where it can be reached and manipulated by the operator during the surgical procedure. Once the clip assembly 106 has been inserted in

the endoscope and has reached the desired location in the patient's body, the sheath stop **156** may be removed from the shaft section **104** so that the user can move the grip portion **152** proximally to uncover the clip assembly **106**.

The connection between the sheath stop **156** and the shaft section **104** may include, for example, pairs of opposing fingers **162**, **164** that are designed to snap over the shaft section **104**. The fingers **162**, **164** cooperate to securely and releasably hold the body of the shaft section **104** therebetween. The fingers **162**, **164** respectively comprise guide portions **170**, **172**; shaft channel portions **166**, **168**; and blocking portions **174**, **176**. Insertion of the sheath stop **156** on the elongated body **154** is accomplished by pressing the body of the shaft section **104** between the guide portions **170**, **172**, to spread the fingers **162**, **164** and allow further insertion of the shaft **104** between the fingers **162**, **164**. The guide portions **170**, **172** and the blocking portions **174**, **176** are shaped so that insertion of the shaft section **104** towards the channel portions **166**, **168** requires less effort than moving the shaft section **104** in the opposite direction.

Once shaft section **104** has been placed within the channel portions **166**, **168**, the fingers **162**, **164** snap back to their non-spread position and retain the shaft section **104** in place therebetween. The shaft section **104** is removed by pulling the sheath stop **156** away from the shaft section **104**. Due to the shape of the blocking portions **174**, **176**, removing the shaft section **104** requires the application of more force than does insertion thereinto. Stops **180** may also be provided on the sheath stop **156** to limit the movement of the shaft section **104** towards the grasping portion **161** to prevent damage to the device that may be caused by excessive spreading of the fingers **162**, **164**. The sheath stop **156** may be formed of a resilient material, such as a polymer, and may be manufactured by injection molding.

The clip assembly **106** is disposed at the distal end of the clipping device **100**, and contains the mechanism that converts the proximal and distal movement of the control wire **118** into the actions necessary to deploy and release a hemostatic clip **90**. FIGS. **9**, **10** and **11** show, respectively, side, top and perspective views of the distal end of the clipping device **100**, including the clip assembly **106** having clips in the folded configuration. This configuration is used, for example, to ship the clipping device **100** and to insert the clipping device **100** through the lumen of an endoscope. Some of the components of the clip assembly **106** include a capsule **200** which provides a structural shell for the clip assembly **106**, the clip arms **208** which move between open and closed positions, a bushing **202** attached to the distal end of the control wire **118**, and a yoke **204** adapted to connect the capsule **200** to the control wire **118**.

As depicted, the proximal end of the capsule **200** slides over the distal end of the bushing **202**. A locking arrangement between these two components is provided by capsule tabs **212**, which are designed to lock into the bushing **202** so that mechanical integrity is temporarily maintained between the capsule **200** and the bushing **202**. Within the capsule **200** are contained a yoke **204** and a tension member **206** which transmit forces applied by the control wire **118** to the clip arms **208**. The ball **140** formed at the distal end of the control wire **118** is mated to a receiving socket **210** formed at the proximal end of the yoke **204**. A male C-section **214** extending from the tension member **206** is received in a corresponding female C-section **216** formed in the yoke **204**, so that the two components are releasably connected to one another, as will be described below. The clip arms **208** in the closed configuration have a radius section **300** which is partially contained within the capsule **200** to prevent opening of the arms. Each of

the clip arms **208** goes over the tension member **206** and has a proximal end **222** which slips under a yoke overhang **254**, to further control movement of the arms **208**.

FIGS. **12** and **13** show a top and a perspective view of one exemplary embodiment of the clip assembly **106** in an open configuration with the clip arms **208** in a fully open position. The open configuration is obtained when the sliding spool **110** shown in FIG. **1** is moved distally so that the ball **140** of the control wire **118** pushes the assembly containing the yoke **204** and the tension member **206** forward, sliding within the capsule **200**. As will be described below, the distal ends of the clip arms **208** are biased toward the open position and revert to this position whenever they are not constrained by the capsule **200**. In the exemplary embodiment, a maximum opening of the clip arms **208** occurs when the clip arms **208** ride over the folded distal folding tabs **220** which extend from the distal end of the capsule **200**, as shown in FIGS. **14** and **15**. In this embodiment, the tabs **220** provide a cam surface, and the clip arms **208** act as cam followers, being deflected by the tabs **220**. In addition, the folding tabs **220** may also provide a distal stop for the tension member **206**, to retain it within the capsule **200**. Thus, by moving the sliding spool **110** distally, the user opens the clip arms **208** to prepare to grasp tissue therebetween.

When the sliding spool **110** is moved proximally by the user, the assembly within the capsule **200** also moves proximally and the clip arms **208** are withdrawn within the capsule **200**. As the clip arms **208** move proximally within the capsule **200**, clip stop shoulders (CSS) **222** contact a distal portion of the capsule **200**, for example, the folded tabs **220**. This interaction of the CSS **222** with the capsule **200** provides to the user a first tactile feedback in the form of increased resistance to movement of the sliding spool **110**. This feedback gives to the operator a positive indication that further movement of the handle control will cause the hemostatic clip **90** to be deployed from the clip assembly **106**. The operator may then decide whether the current position of the clip **90** is acceptable or not. If the position is acceptable, the operator can deploy the clip **90** by continuing to move the sliding spool **110** with increased proximal pressure to cause the clip arms **208** to close on the tissue. If not, the operator can move the sliding spool **110** distally to re-open the clip arms **208** and extend them out of the capsule **200**, reposition the clip **90**, and repeat the above steps to close the clip **90** at a more appropriate location.

When the user determines that the clipping device **100** is positioned correctly, the proximal pressure on the sliding spool **110** may be increased to continue deployment of the hemostatic clip **90** from the clip assembly **106**. FIGS. **16** and **17** show respectively a top and side view of the clipping device **100** in this condition. As the proximal tension on sliding spool **110** is increased, the control cable **118** pulls the yoke **204** proximally, away from the tension member **206**. The tension member **206** is firmly attached to the clip arms **208** which are prevented from moving proximally by the interaction of the CSS **222** with the folded tabs **220**. If sufficient pulling force is applied to the yoke **204**, the male C section **214** of the tension member **206** yields and loses integrity with the female C section **216** of the yoke **204**. This can occur because, in the exemplary embodiment, the tension member **206** is formed of a material with a lower yield strength than the material of the yoke **204**.

The force required to break the tension member **206** away from the yoke **204** may be tailored to achieve a desired feedback that can be perceived by the user. The minimum force required to break the tension member **206** free of the yoke **204** may be selected so that a tactile feedback is felt by the user, to

prevent premature deployment of the hemostatic clip **90** while a maximum force may be selected so that other components of the linkage between the sliding spool **110** and the clip arms **208** do not fail before the male C section **214** and the female C section **216** disconnect from one another. In one exemplary embodiment, the tension force necessary to disconnect the two components may be in the range of approximately 4 lbf to about 12 lbf. This range may vary depending on the size of the device and the specific application. To obtain this force at the interface of the male and female C sections **214**, **216** a larger force will be applied by the user at the sliding spool **110**, since friction within the device may cause losses along the long flexible shaft.

When the male C section **214** of tension member **206** yields, several events take place within the exemplary device **100** nearly simultaneously. More specifically, the yoke **204** is no longer constrained from moving proximally by the CSS **222** abutting the capsule **200**. Thus the yoke **204** travels proximally until coming to rest against a distal bushing shoulder **250**. The tension member **206** is not affected by this movement since it is no longer connected to the yoke **204**. The proximal ends **252** of the clip arms **208** are normally biased away from a center line of the device **100** and are no longer constrained by the yoke overhangs **254**. Accordingly, the clip latches **302** are free to engage the latch windows **304** of the capsule **200**, thus maintaining the integrity of the capsule-clip arms combination after deployment. Details of one exemplary embodiment of the capsule **200** are shown in FIGS. **14**, **15** and details of the clip arms **208** are shown in FIGS. **18**, **19** and **20**.

As the yoke **204** moves proximally to abut against the bushing **202**, the capsule tabs **306** are bent away from the centerline of the capsule **200** by the cam surfaces of the yoke **204**. As a result, the capsule tabs **306** are no longer engaged to the corresponding bushing undercuts **350**, shown in the side and perspective views of the bushing **202** depicted in FIGS. **21**, **22**. Since the capsule **200** and the bushing **202** (which is securely connected to shaft section **104**) are no longer connected, the clip assembly **106** is prevented from being released from the shaft section **104** only by its connection to the ball **140** of the control wire **118**.

A further result of moving the yoke **204** against the distal bushing shoulder **250** of the bushing **202** is that the distal end of the wire stop **360** (shown in FIGS. **12**, **16**) is placed near the proximal bushing shoulder **364** (shown in FIG. **22**). The flared fingers **362** located at the distal end of the wire stop **360**, better shown in FIG. **23**, are compressed as they pass through the central ID of the bushing **202**, but return to their normally biased open position (shown in FIG. **23**) after passing past the proximal bushing shoulder **364**. Further distal movement of the sliding spool **110** is thus prevented since that movement would engage the fingers **362** of the wire stop **360** with the proximal bushing shoulder **364**. This feature prevents the clip assembly **106** from being pushed away from the bushing **202** before the ball **140** is separated from the control wire **118**, as will be described below.

The wire stop **360** comprises a tube with a first slotted and flared end attached to the control wire **118** by conventional means. As shown in FIG. **23**, the slots impart flexibility to the device so it can easily pass through the central lumen of the bushing **202**. Flared fingers **362** are formed by the slots, and engage the proximal bushing shoulder **364**. The wire stop **360** is made of a material that is biocompatible and that has enough resilience so that the fingers **362** re-open after passage through the bushing **202**. For example, stainless steel may be used for this application.

One feature of the exemplary embodiment of the invention described above is that the user receives both tactile and auditory feedback as the clip assembly **106** is deployed and released. The separation of the tension member **206** from the yoke **204** produces a small clicking noise and a tactile feel that is perceptible while holding the handle assembly **102**. The change in axial position of the sliding spool **110** is thus augmented by the changes in resistance to its movement and by the clicking sound and feel through the start and stop of the movement. As a result the user is always aware of the status of the clip assembly **106**, and the inadvertent deployment of a hemostatic clip **90** in an incorrect location is less likely. It will be apparent to those of skill in the art that the order of male and female connectors in the device may be reversed or changed without affecting the operation of the device.

It may be beneficial for the user to be certain that the clip assembly **106** has been deployed before the rest of the clipping device **100** is removed from the endoscope. Injury to the tissue being treated could result if the clipping device **100** is removed from the operative site when the hemostatic clip **90** is only partially deployed. Accordingly, a large tactile feedback may be incorporated, to augment the auditory and tactile feedback stemming from the separation of the yoke **204** from the tension member **206**. FIG. **24** depicts the condition where the clip assembly **106** separates from the rest of the clipping device **100**. According to the described embodiment, this second user feedback is obtained by designing the control wire **118** so that it will separate from the end ball **140** when a predetermined tension is applied to it. In other words, the ball **140** of the control wire **118** is mechanically programmed to yield and separate from the body of the control wire **118** when a pre-set tension is applied thereto. The size of the reduced diameter section **142** can be selected so that, when the user continues to move the sliding spool **110** proximally as the programmed yield tension is reached, the ball **140** detaches from the tapered section **144** and provides a large tactile feedback to the operator.

When the ball **140** detaches, the sliding spool **110** bottoms out at the proximal end of the handle **108**, such that a full stroke of the handle assembly **102** is reached. The tension required to cause the reduced diameter section **142** to yield and release the ball **140** may vary over a range of values. However, for best results the force should be greater than the tension force required for the male C section member **214** to separate from the yoke **204**. If this condition is not satisfied, a situation may occur where the clip assembly **106** is locked in place on the patient's tissue, but cannot be released from the clipping device **100**. It will be apparent that this situation should be avoided. In one exemplary embodiment, the tension force required to separate the ball **140** from the body of the control wire **118** is in the range of between about 10 lbf and 20 lbf at the distal end of the control wire **118**. As discussed above, losses along the elongated flexible shaft may require the user to apply a force substantially greater than this to the handle body **102**.

Once the ball **140** has separated from the rest of the control wire **118**, the user can pull the rest of the clipping device **100** from the endoscope. As this is done, the yoke **204** is retained within the capsule **200** by the spring and frictional forces of various features of the capsule **200**, such as the capsule tabs **306**. Prior to withdrawing the clipping device **100**, the oversheath **150** may be moved distally by the user over the entire remaining portions of the shaft section **104** to prevent damage to the endoscope as the clipping device **100** is withdrawn therethrough. The sheath stop **156** may also be placed on the

shaft section **104** proximally of the over-sheath grip **152** to prevent inadvertent sliding of the over-sheath **150** from the distal end of the device **100**.

A more detailed description of several components of the clipping device **100** follows. The clip arms **208** are shown in detail in FIGS. **18**, **19** and **20**; the tension member **206** is shown in side and top views in FIGS. **25**, **26**; while top and side views of the yoke **204** are shown respectively in FIGS. **27** and **28**. The clip arms **208** may be formed of a biocompatible material such as Nitinol, Titanium or stainless steel. Maximum spring properties may be obtained by using materials such as 400 series stainless or 17-7 PH. As shown, a tear drop keyway **400** is formed in the clip arm **208** to mate with a corresponding tear drop key **402** formed on the tension member **206**. This feature maintains the relative positions of these two components and of the yoke **204** substantially constant. The shape of the keyways **400** may be varied. For example, the keyway **400** may be oval or elliptical. Central portions of the clip arms **208** define a spring section **404**. When the proximal ends **252** of the clip arms **208** are under the yoke overhangs **254**, the clip arms **208** are allowed to pivot over the tension member **206**, which in turn biases the distal ends **252** towards the open configuration when no longer restrained by the capsule **200**. As a result, the proximal end **252** of each clip arm **208** springs upward and engages the latch windows **304** in the capsule **200**.

The clip arms **208** also comprise a radius section **300** that adds strength to the clip and reduces system friction. The radius of the radius section **300** approximately matches the inner diameter of the capsule **200** and has a smooth profile to avoid scratching the inner surface of the capsule **200**. A pre-load angle α is defined between the radius section **300** and the spring section **404**. The pre-load angle α determines how much interference (pre-load) exists between the two opposing clip arms **208** at their distal ends when closed. The greater the pre-load angle α , the greater the engaging force that is applied by the clip arms **208**. However, this condition also causes the greatest system friction when the hemostatic clip **90** is closed. The clip arms **208** also comprise interlocking teeth **408** disposed at their distal ends. In the exemplary embodiment, the teeth **408** are identical so that the arms may be interchangeable and will mesh smoothly with the set facing them. The teeth **408** are disposed at a nose angle β which may be between approximately 90 and 135 degrees, but in other applications may be greater or lesser than the described range.

One exemplary embodiment of the capsule **200** is shown in detail in FIGS. **14** and **15** and comprises alignment keyways **500** that are designed to mate with corresponding features on the bushing **202** to rotationally align the two components. In this embodiment, the capsule tabs **306** may be bent towards the centerline of the capsule **200** to engage the bushing undercuts **350**. The engagement maintains the integrity between the capsule assembly **200** and the rest of the clipping device **100** until the yoke is pulled into the distal bushing shoulder. The capsule overhangs **502** provide added clamping strength to the deployed clip arms **208**. This is achieved by reducing the length of the portion of each clip arm **208** that is not supported by a portion of the capsule **200**. This feature does not affect the amount of tissue that may be captured by the clip arms **208** since the capsule overhangs **502** extend on a plane substantially parallel to the plane of the clip arms **208**.

Additional features of the capsule **200** include an assembly aid port which may be used to assist in aligning the components of the clip assembly **106**. Bending aids **506** facilitate a smooth bend when the distal folding tabs **220** are bent inward, as described above. The bending aids **506**, as shown, are holes

aligned with the folding line of the tabs **220**, but may also include a crease, a linear indentation, or other type of stress concentrator. The capsule **200** may be formed from any of a variety of biocompatible materials. For example, stainless steel, Titanium or Nitinol or any combination thereof may be used. High strength polymers like PEEK™ or Ultem™ may also be used to form the capsule **200**, with a heat set treatment being used to adjust positionable elements.

FIGS. **25** and **26** depict additional details of the tension member **206**. As shown, tear drop keys **402** are designed to engage the tear drop keyways **400** of the clip arms **208**, as described above. Clip follower planes **508** are shaped to form a fulcrum which allows the clip arms **208** to rock between the open and closed configurations. The tension member **206** comprises a distal stop face **510** which abuts the distal folding tabs **220** of the capsule **200** to stop the distal motion of the capsule assembly **106**. In general, all surfaces and edges of the tension member **206** that are in contact with the inner surfaces of the capsule **200** preferably have a radius substantially similar to an inner radius of the capsule **200** to provide a sliding fit therein. The tension member **206** may be formed of a biocompatible polymer, monomer or thermoset. The type of mechanism selected to release the tension member **206** from the yoke **204** may determine the type of material used since a release due to fracture of the male C section **214** requires a relatively brittle material while release due to yielding without fracture calls for a softer material.

Additional details of the yoke **204** are shown in FIGS. **27-29**. When the control wire **118** is seated in the yoke **204**, it is desirable to ensure that it cannot inadvertently be removed from the control wire slot **600**. Accordingly, in the present embodiment the ball cavity **602** has a diameter sufficiently large to allow the ball **140** to pass therethrough while the wire cavity **604** is large enough to allow the control wire **118** to pass therethrough, but not large enough to allow the ball **140** pass therethrough. To assemble the control wire **118** with the yoke **204** according to the exemplary embodiment, the proximal end of wire **140** is inserted into the ball cavity **602** until the ball bottoms out, and then the control wire **118** is rotated until it is seated in the control wire cavity **604**, thus constraining further movement of the ball **140**. According to the present embodiment, the yoke **204** may be made of a biocompatible metal such as stainless steel or a high strength polymer such as Ultem™.

According to embodiments of the present invention, the clipping device **100** may be scaled to fit the requirements of different surgical procedures. In one exemplary embodiment, the clipping device **100** may be sized to fit through an endoscope having a working channel diameter of approximately 0.110 inches. The exemplary bushing may have a length of about 0.22 inches and an OD of approximately 0.085 inches. The capsule may have a length of about 0.5 inches, an OD of about 0.085 inches, and a wall thickness of about 0.003 inches. When assembled, the rigid length of the capsule **200** and the bushing **202** is approximately 0.625 inches. This length is important because if it is too great, the assembly will not pass through the bends of the flexible endoscope. In the exemplary clipping device, the outer sheath may have an ID of approximately 0.088 inches and an OD of about 0.102 inches. The overall length of the clipping device may be approximately 160 inches, while the tissue grasping portion of the clip arms **208** may be approximately 0.4 inches long.

In treating internal bleeding, and in particular to apply an hemostatic treatment to gastrointestinal bleeding, it is often necessary to apply more than one hemostatic clip to the injured tissue. Using conventional methods, the treatment involves repeatedly utilizing a single deployment clip appa-

13

ratus, with the disadvantage of having to remove the old clipping device from the endoscope, prepare additional clipping devices, and re-inserting the additional clipping devices in the endoscope for each clip. After insertion in the endoscope, each additional device has to be re-positioned over the wounded tissue before the new clip may be deployed. Multi deployment clipping devices are also in use, but generally require the device to be removed from the endoscope so that a new clip may be loaded manually in the device.

In a further embodiment of the present invention, a multiclip endoscopic hemostatic device may be used to discharge multiple hemostatic clips without the necessity to remove the device from the endoscope after each clip is deployed. The multiclip device achieves equal or better results than conventional single deployment clipping devices, while greatly facilitating the placement of multiple hemostatic clips in cases where a single hemostatic clip is insufficient. In one embodiment, the clips used by the multiclip device according to the present invention are substantially similar in size to conventional hemostatic clips, and thus can be used with conventional endoscopes. According to the invention, the cost of manufacturing the multiclip apparatus is sufficiently low to permit the units to be disposable, and be discarded after use with only one patient.

According to the invention, the multiclip hemostatic clipping apparatus is used in a minimally invasive environment, such that it is applied to the surgical site through an endoscope. The distal end of the hemostatic multiclip device is inserted through the working lumen of the endoscope, and is brought in the vicinity of the surgical site where the bleeding occurs. For example, an endoscope having a working channel of at least about 1.8 mm inner diameter may be used to reach the surgical site. The proximal ends of the endoscope and of the hemostatic multiclip device are provided with hand controls used by the user/physician to operate the devices.

The hemostatic multiclip device according to an exemplary embodiment of the present invention uses a magazine containing a plurality of hemostatic clips that is advanced through the endoscope's working lumen, to a location near the surgical site. The magazine may be attached to a sheath designed to protect the inner surfaces of the endoscope from damage caused by sharp edges of the magazine and clip assembly, and which extends beyond the magazine through the length of the endoscope. The hemostatic clips are joined in a clip chain which is inserted in the magazine, and is free to translate in the magazine within certain limits that will be described below. Each of the clips may be formed, for example, of sheet metal or of another material having appropriate mechanical and bio-compatibility properties. The material of the clips is selected to resist plastic deformation while constrained in the closed configuration, so that the hemostatic clips will return to the open configuration when not otherwise restrained.

A modified version of the clipping device 100, shown in FIGS. 1 and 2, may be used with the clip magazine and clip chain described above. A clip magazine containing multiple hemostatic clips may be inserted in the proximal end of the shaft section 104, such that the clips are deployed from the distal end thereof. A handle 108 and sliding spool 110, or similar implements, may be used in conjunction with a control linkage to operate the multiclip dispensing apparatus, as will be described in detail below.

FIG. 31 shows an exemplary embodiment of a hemostatic clip according to the present invention. Exemplary clip 702 comprises two clip arms 704 which have inner facing surfaces adapted to grasp and retain tissue therebetween when placed in a closed configuration. In FIG. 31, the clip arms 704 are in

14

the open configuration which is assumed by the clip 702 in the early phase of deployment, before the tissue is clamped. Clip 702 may be formed of two parts joined at the common portion 705, or may be of a single piece construction. In the exemplary embodiment, clip 702 is biased in the open configuration (shown in FIG. 31) prior to being loaded in the clip magazine. A sliding lock ring 706 may be used to lock clip arms 704 in the closed configuration, which is assumed by the clip 702 when it is clamped to the tissue. In different exemplary embodiments, the sliding locking ring 706 may be replaced by different devices adapted to lock clip arms 704 in the closed configuration.

As indicated above, a plurality of clips may be loaded in the magazine for use with the hemostatic multiclip device according to the present invention. FIG. 32 shows an exemplary embodiment of a clip chain according to the invention. Clip chain 700 is formed by joining hemostatic clips 702 to one another using, for example, a linking feature 708. Linking feature 708 may comprise an attachment which retains the two joined clips 702 together as long as there is no movement of the joined clip ends in a direction perpendicular to the longitudinal axis of the clips. In this manner, the clip chain 700 remains intact as long as the clips are translated in a direction generally along the longitudinal axis of the clips. One clip may be released, however, by moving the appropriate clip end along a diameter of the device, that is in a direction perpendicular to the longitudinal axis. For example, linking feature 708 may be clamped between the distal ends of clip arms 704 which are held in the closed configuration. Linking feature 708 may be formed integrally with the body of hemostatic clip 702, or may be an optional addition that may be attached to more conventional clips.

An exemplary clip magazine 720 is shown in perspective view in FIG. 36. Clip chain 700 (shown in perspective view in FIG. 35) may be inserted longitudinally in the hollow channel 722 of magazine 720, as shown in FIG. 38. Magazine 720 may be a generally cylindrical structure located at the distal end of the hemostatic multiclip device, which contains a portion or all of the clips 702 within the clip chain 700. Magazine 720, together with clip chain 700, forms a capsule having dimensions and sufficient flexibility to comply with the curvature of the endoscope's working channel. Compliance features 723 may be used to impart flexibility to the body of magazine 720, and for example may comprise circumferential slits. A control link 726 may enter a proximal opening 722 of the clip magazine 720, opposite from the distal end 724.

The most proximal of the clips 702 may be connected to control link 726 in a releasable manner. Control link 726 may be designed to carry compression and tension loads, so that clip chain 700 may be translated in both directions through forces transmitted by control link 726. Control link 726 may be formed by a rigid tube, a semi rigid wire, or by any other structural element capable of transmitting tension and compression loads along the length of the hemostatic multiclip device. Control link 726 may be connected to a control handle at the proximal end, to give to the surgeon control of the clip's deployment.

FIG. 30 shows a detail of the connection between the control link 726 and the most proximal hemostatic clip 702. In this embodiment, control link 726 is a rod or tube which terminates in a connector portion 727 adapted to push against linking element 708. Connector portion 727 may also be designed to apply a tension force to the linking element 708, in a known manner. A sheath 725 may be used to encapsulate control link 726, to protect the working channel of an endo-

scope from damage, and to reduce friction between the moving control link 726 and the clip magazine 720.

A control handle portion of the hemostatic multclip device (not shown) is provided at the proximal end of the device, extending outside of the proximal end of the endoscope. The control portion may be similar to that shown in FIG. 1, and may comprise hand controls which operate the control link 726 to cause the deployment and the release of the successive clips 702. For example, hand movements of the surgeon may be transformed within the control portion into longitudinal movements of the control link 726 along the working channel of the endoscope. In an exemplary embodiment, clip chain 700 is rigid in compression and supports tensile loads, at least while contained within the clip magazine 720. Clip chain 700 can therefore be translated along magazine 720 via movement of the control link 726.

As shown in FIG. 38, the clip chain 700 is formed of hemostatic clips 702 which remain attached to one another while they are within the cylindrical containment of the clip magazine 720. Clip magazine 720 supports and constrains the clips 702 of the clip chain 700 in the radial direction through a large portion of its length. This prevents pairs of adjacent clips 702 from disconnecting, by not allowing relative radial movement between two clips. In particular, the radial movement of the substantially closed clip arms 704 of a first hemostatic clip is prevented, so that the linking feature 708 of a second clip, adjacent to the first clip, is not released. The exemplary design of clip chain 700 helps to minimize the width of the device, since it is only as wide as the width of the clips themselves.

The diameter of clip chain 700 works in conjunction with the shape of the distal end 724 of clip magazine 720 to control the position of the distal portion of clip chain 700 through the distal end 724. As shown in FIG. 37, magazine 720 has a reduced cross section portion 730 designed to limit the diameter of what passes therethrough. Specifically, reduced cross section 730 allows the passage of a single clip unattached to another clip at its distal end. However, reduced cross section 730 does not allow passage of a pair of connected clips. This is because the diameter of two connected clips is greater than the diameter of a single clip. In the exemplary embodiment that is due to the clip arms 704 not closing fully when they lock onto the linking feature 708 of another clip 702, resulting in a greater distal tip diameter of the clip.

The function of the clip chain 700 is better shown in FIGS. 39, 40, where a clip 702' is placed to lead the clip chain 700 through the distal end 724 and through cross section reduction 730. As the control element 726 is pushed distally, clip chain 700 is pushed distally until its second most distal clip 702 is stopped by reduced cross section 730, at a position where the most distal clip 702' is outside of magazine 720, and is biased in the open configuration ready to grasp the tissue. In FIG. 39, the most distal hemostatic clip 702' is being pushed outside of clip magazine 720, past the distal end 724. As the control link 726 continues to push distally, clip arms 704 of the second most distal clip 702 of chain 700 about the reduced cross section 730 (FIG. 40). At this point the single distal clip 702' is largely outside of magazine 720, and its clip arms 704' take the open configuration since they are no longer constrained by magazine 720.

Once the user has placed the open clip 702' over the desired location on the tissue, control link 726 is pulled proximally, so that clip chain 700 (including the most distal clip 702') is pulled back into magazine 720, as shown in FIG. 41. Clip sliding lock ring 706 is held distally by lock ring anti-pull back tabs 734, as distal clip 702' is pulled proximally. This causes lock ring 706 to move partially over clip arms 704' and

lock them in the closed configuration, to firmly grasp the tissue held within clips arms 704'. At this point the most distal hemostatic clip 702' is clamped securely over the tissue, but is still attached via linking feature 708 to the clip chain 700.

After deployment and clamping of the most distal hemostatic clip 702' is achieved, further proximal movement of the control linkage 726 causes separation of clip 702' from clip chain 700. Additional features may be formed on the clip 702' or on the lock ring 706 to cooperate with distal end 724 and prevent further proximal movement of the distal clip 702' relative to magazine 720. The pull back distance of distal clip 702' may be controlled, for example by properly positioning the additional feature 733, so that the link between the most distal clip 702' and the next to most distal clip 702 is located in a relief portion 732 of the distal end 724. Relief portion 732 may be a movable tab or opening which allows local diametrical expansion of the clips within that portion of magazine 720.

As continued proximal tension force is applied by control link 726, clip arms 704 of the second most distal clip 702 are pushed diametrically outward over the interlock feature 708 of the most distal hemostatic clip 702', which now acts as a cam surface. Relief portion 732 of the clip magazine 720 allows the outward expansion due to the outward movement of clip arms 704 over linking feature 708, thereby permitting clip arms 704 to continue moving proximally and separate from distal-most clip 702'. In other words, the separation of the two adjacent clips is caused by the force in the diametrical direction resulting from clip arms 704 being forced over clip lock feature 708 of distal clip 702', and this force overcoming the bias of relief portion 732. Distal most clip 702' is still prevented to further move proximally by the additional feature 733 described above, but is now free to move distally and exit magazine 720.

FIG. 42 depicts the situation where the "former" most distal hemostatic clip 702' has been ejected from clip magazine 720, and is clamped securely to the target tissue. A "new" most distal hemostatic clip 702 has been pushed partially out of magazine 720, and its clip arms 704 are in the open configuration, outside of distal portion 724. The new most distal clip 702 is still connected to another clip 702 which is fully inside of clip magazine 720, and is part of clip chain 700. The user may at this point position open clip arms 704 over the desired tissue, and repeat the process described above to clamp clip arms 704 over the tissue, lock them closed, and release the new distal-most clip 702 from the clip chain 700 and from clip magazine 720.

To release the most distal clip 702' from the clip chain 700, the clip arms 704 belonging to the clip 702, adjacent to the clip 702', have to disengage from the linking feature 708'. To do so, the distal tip of clip arms 704 has to open at least sufficiently to clear the linking feature 708' of the most distal clip 702'. The clip 702 is contained within the magazine 720, which because of its radially rigid construction, for the most part prevents the clip arms 704 from opening. The only time that the clip arms 704 can open and release the linking feature 708' is when the distal tips 705 of the clip arms 704 are substantially aligned with a section of the magazine 720 which either is radially wider, or is designed to yield when pressed by the clip arms 704. For example, the relief portion 732 may comprise a cut out opening or a non-rigid portion of the magazine's wall, dimensioned to accommodate the tips 705 of the clip arms 704.

The utility of the multi clip deployment device according to the invention may be increased by configuring the multi-clip magazine so that the release of the linking feature 708' from clip arms 704 can be performed more easily. In an additional exemplary embodiment shown in FIG. 43, the magazine 800

is formed with an expanded section **804** which extends 360 degrees around the circumference of the magazine **800**. The expanded section **804** formed by the wall of the magazine **800** defines an expanded chamber **810** within the lumen of magazine **800**. The expanded chamber **810** provides for sufficient room within the magazine **800** to allow distal tips **705** of the clip arms **704** to move radially outwards, as the clip arms **704** open to pass over the linking feature **708'**.

The deployment of the most distal clip **702'** from the exemplary magazine **800** is in many respects similar to the deployment from the magazine **720**, described above. A control link **726** may be used to transfer commands from the surgeon to the clip deployment mechanism in the form of proximal and distal translation of the link **726**. The most distal clip **702'** is initially connected to a clip chain **700**, and may be translated forward and backwards while still connected to the adjacent clip **702**. After the surgeon places the distal end of clip **702'** in position over the target tissue **822**, the most distal clip **702'** is pulled back inside the magazine **800**, so that clip arms **704'** close over a portion **820** of the target tissue **822**. The lock ring **706'** may be pushed distally by distal lip **806** of the magazine **800**, to lock the clip arms **704'** in the closed position around the target tissue portion **820**.

After the most distal clip **702'** is clamped and locked in the closed position around the portion of target tissue **820**, further proximal movement of the clip **702** causes the distal clip **702'** and its adjacent clip **702** to detach. For the purposes of this discussion, clip **702** is referred to as the next-to-most distal clip. More specifically, the distal ends **705** of the adjacent clip's arms **704** partially open to pass over the linking feature **708'** of the most distal clip **702'**, under the traction applied by the control linkage **726** which pulls clip **702** proximally. As described above, the most distal clip **702'** is prevented from moving proximally by the shape of the distal end **806** of the magazine **800**, so that a tension exists between the most distal clip **702'** and the next-to-most distal clip **702**. As the clip **702** moves proximally, linking feature **708'** acts as a cam forcing the clip arms **704** to open. The expanded chamber **810** allows the radial opening of the clip arms **704**, which releases the linking feature **708'**.

The magazine **800** provides several benefits to the multi-clip deployment device according to the present invention. Since the expanded section **804** is a radial bulge which spans 360 degrees around the circumference of the magazine **800**, the rotational orientation of the clip chain **700**, which includes clips **702** and **702'**, within the magazine **800** is not important. The surgeon therefore has greater liberty to orient the distal clip **702'** as necessary to best perform the procedure. The rotational orientation of the clip chain **700** may be changed relative to the orientation of the magazine **800** and of the entire multi-clip delivery device to which the magazine **800** is attached, to better align the clip with the target tissue. This configuration simplifies the clip deployment procedure and makes the entire procedure simpler and less time consuming. In addition, manufacturing of the magazine **800** can be simpler, since there is no need to process the magazine to form radial relief regions such as relief portions **732**, or to cut openings in the wall of the magazine **800**.

An exemplary clip deployment sequence from a magazine **800** according to the present invention is described below. FIGS. **44-48** are used to depict the deployment of a most distal clip **702'** from the magazine **800**. FIG. **44** depicts a pre-deployment configuration of the most distal clip **702'** from the magazine **800**, such that the clip arms **704'** are completely within the distal portion **802** of the magazine **800**. In this configuration, the linking feature **708'** is being grasped by the clip arms **704** of the clip **702**, such that the two clips **702**, **702'**

are connected in the clip chain **700**. The lock ring **706'** is away from the clip arms **704'**, and does not yet constrain them in the closed configuration. In this step of the deployment, the surgeon may position the distal tip **802** of the magazine **800** in proximity of the target tissue, while preparing to clamp the clip **702'** to that tissue.

As the control link **726** is pushed distally during a distal stroke of the deployment sequence, clip **702'** is pushed outside of the magazine **800**, as shown in FIG. **45**. In this configuration, the arms **704'** of clip **702'** are no longer constrained by the walls of the magazine **800**. The lock ring **706'** is still near the clip's proximal end, held by the tip **802** within the magazine **800**, so that the clip arms **704'** are free to move to the open configuration. At this point, the clips **702**, **702'** are connected by means of the linking feature **708'**, and are free to rotate 360 degrees in any rotational orientation within the magazine **800** to facilitate proper orientation relative to the tissue to be clamped. Using the ability to place the clip **702'** in any desired rotational orientation, the surgeon can orient the clip arms **704'** in any desired position over the target tissue **820**, so that closing the clip arms causes the tissue to be clamped as effectively as possible.

When the clip arms **704'** are correctly placed in the proper orientation over the target tissue **820**, the surgeon may continue the deployment by carrying out a proximal stroke of the deployment sequence. This causes the control link **726** to move proximally, thus entraining clip **704** and clip **704'**. As described in the context of other embodiments, the proximal stroke of control link **726** causes the clip arms **704'** to close, and clamp on the portion **820** of the target tissue **822**. Distal end **802** of the magazine **800** forces the clip arms **704'** to close as clip **702'** moves proximally inside of the magazine **800**, such that the target tissue is clamped, as shown in FIG. **46**. The lock ring **706'** is held near distal tip **802** by protrusions within magazine **800**, and slides distally over the clip arms **704'** as they are pulled proximally within the magazine **800**. In this manner, the clip arms **704'** are securely locked in the closed configuration by ring **706'**, and are clamped on the target tissue. After the clip arms **704'** are locked in the closed configuration on the target tissue, the magazine **800** and the rest of the device can be rotated relative to the clips **702**, **702'**, since these are free to turn 360 degrees within the magazine **800**.

Continued proximal tension on the control link **726** causes the clip **702** to further move proximally within the magazine **800**. FIG. **47** depicts this step of the clip deployment process. However, the most distal clip **702'** is prevented from further proximal movement by the lock ring **706'** interacting with the protrusions formed at the distal end **802** of the magazine **800**. Lock ring **706'** is also prevented from moving too far distally over the closed clip arms **704'** by ring stops **705**. Accordingly, clip arms **704** are pushed apart by the linking feature **708**, which acts as a cam as the tip of clip arms **704** pass over it. The expanded chamber **810** defined by the expanded section **804** of magazine **800** gives sufficient room to the clip legs **704** to open and pass over the linking element **708'**, so that the clip **702** can disengage from the clip **702'**. Expanded section **804** extends 360 degrees around the circumference of the magazine **800**, so that the orientation of clips **702**, **702'** within the magazine **800** is not important. This makes it possible for the surgeon to change the rotational orientation of the clip **702'** relative to the magazine **800** throughout the deployment steps, to maintain the desired orientation between the clip **702'** and the target tissue **822**.

FIG. **48** depicts the final step of the clip deployment sequence, in which the clip **702'** is released from the magazine **800** and is left clamped to the target tissue. In this step, control

19

link 726 may be again moved distally, to push clips 702 and 702', which are now disconnected. As shown, clip 702' is pushed outside of the magazine 800 by the distal portion of clip 702, until it is ejected from the magazine 800. Clip 702 now becomes the most distal clip present in the magazine 800, and the same steps described relative to carry out the deployment of clip 702' may be repeated to deploy the new clip 702. Although the drawings depict a magazine 800 containing only two clips 702 and 702', it will be apparent to those of skill in the art that additional clips may be connected in the same manner within magazine 800, to form a longer clip chain 700.

As described, the distal most clip 702' after release from the clip chain 700, or more simply from clip 702, may exit clip magazine 800 due to the tension applied to it by the clamped tissue. Alternatively, clip 702' may be pushed out by the distal movement of clip 702, as it is pushed towards the distal end 802. The surgeon may ensure a complete release of clip 702' by causing the control link 726 to move distally, for example by manipulating the hand control of the device. Conventional methods may be used to transform the hand movements of the surgeon into translation of the control link 726, and to carry out the initial distal stroke and the subsequent proximal stroke.

The present invention has been described with reference to specific exemplary embodiments. Those skilled in the art will understand that changes may be made in details, particularly in matters of shape, size, material and arrangement of parts without departing from the teaching of the invention. Accordingly, various modifications and changes may be made to the embodiments without departing from the broadest scope of the invention as set forth in the claims that follow. The specifications and drawings are, therefore, to be regarded in an illustrative rather than a restrictive sense.

What is claimed is:

1. A multi clip magazine for surgical procedures, comprising:

- a substantially cylindrical shell;
- a proximal end of the shell adapted for connection with a clip deployment apparatus;
- a central lumen for containing a clip chain rotatable therein; a distal end of the shell having a clip deployment opening and surface features adapted to facilitate opening and to cause closing and locking of a distal-most clip of the clip chain; and
- an expanded portion of the shell providing a region for the next clip immediately proximal to the distal-most clip to open and release the distal-most clip while the next clip is in any rotational orientation, wherein the expanded portion extends 360 degrees around a circumference of the shell, wherein the expanded portion comprises a circumferential bulge of the shell having a radius increased with respect to proximal and distal portions of the shell.

20

2. The multi clip magazine according to claim 1, wherein the proximal end is adapted to receive a control link operatively connectable to the clip chain.

3. The multi clip magazine according to claim 1, wherein the circumferential bulge has a radius substantially corresponding to a dimension of the next clip when opened sufficiently to release the distal-most clip.

4. The multi clip magazine according to claim 1, wherein the expanded portion is symmetrical with respect to a longitudinal axis of the multi clip magazine.

5. The multi clip magazine according to claim 1, wherein the clip chain comprises hemostatic clips.

6. The multi clip magazine according to claim 1, wherein the shell is adapted for insertion into a patient through an endoscopic instrument.

7. The multi clip magazine according to claim 1, further comprising distal surface features adapted to move a locking ring of the distal-most clip to a clip locking position.

8. The multi clip magazine according to claim 1, wherein the shell outside of the expanded portion has a diameter corresponding to a dimension of closed clips of the clip chain.

9. The multi-clip magazine of claim according to claim 1, wherein the circumferential bulge defines an increased diameter of central lumen.

10. A multi clip magazine for surgical procedures, comprising:

- a substantially cylindrical shell;
- a proximal end of the shell adapted for connection with a clip deployment apparatus;
- a central lumen for containing a clip chain rotatable therein; and
- an expanded portion of the shell providing a region for the next clip immediately proximal to the distal-most clip to open and release the distal-most clip while the next clip is in any rotational orientation, wherein the expanded portion comprises a circumferential bulge of the shell having a radius increased with respect to proximal and distal portions of the shell and wherein:
 - a distal end of the shell includes a clip-deployment opening bounded by a distal lip against which a locking element may be pushed into a locking configuration over arms of the distal-most clip.

11. The multi clip magazine of claim 10, wherein the circumferential bulge has a radius substantially corresponding to a dimension of the next clip when opened sufficiently to release the distal-most clip.

12. The multi clip magazine according to claim 10, wherein the expanded portion is symmetrical with respect to a longitudinal axis of the multi clip magazine.

13. The multi-clip magazine of claim 10, wherein the circumferential bulge defines an increased diameter of central lumen.

* * * * *