

(19)



(11)

EP 1 705 950 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
06.08.2014 Bulletin 2014/32

(51) Int Cl.:
H04R 25/00 (2006.01)

(21) Application number: **06006023.3**

(22) Date of filing: **23.03.2006**

(54) Method for individually fitting a hearing instrument

Verfahren zur individuellen Anpassung eines Hörgeräts

Procedé pour l'adaptation individuelle d'un appareil auditif

(84) Designated Contracting States:
**AT BE BG CH CY CZ DE DK EE ES FI FR GB GR
HU IE IS IT LI LT LU LV MC NL PL PT RO SE SI
SK TR**

(43) Date of publication of application:
27.09.2006 Bulletin 2006/39

(60) Divisional application:
10177370.3 / 2 278 827

(73) Proprietor: **Phonak AG
8712 Stäfa (CH)**

(72) Inventors:
• **Boretzki, Michael, Dr.
8630 Rüti (CH)**

- **Kühnel, Volker
8708 Männerdorf (CH)**
- **von Buol, Andreas
8044 Zürich (CH)**
- **Zbindne, Paul, Dr.
8634 Hombrechtikon (CH)**

(74) Representative: **Schwan Schorer & Partner mbB
Patentanwälte
Bauerstrasse 22
80796 München (DE)**

(56) References cited:
**WO-A-00/65872 WO-A-2004/054318
US-A- 4 099 035**

EP 1 705 950 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

[0001] The present invention relates to a method for individually fitting a hearing instrument.

[0002] A hearing instrument usually comprises a microphone for generating an input audio signal from ambient sound, an audio signal processing unit (which nowadays often is digital) for processing the input audio signal into a processed output audio signal and an output transducer for stimulation of the user's hearing according to the processed output audio signals. Audio signal processing in the audio signal processing unit involves applying a gain function to the input audio signal, which depends on level and frequency of the input audio signal. Hearing instruments usually are used by persons suffering from a hearing loss compared to normal-hearing persons, which depends on level and frequency of the ambient sound. Usually the hearing instrument undergoes a fitting procedure in order to individually set the gain provided by the hearing instrument such that the hearing loss of the user is compensated as far as possible.

[0003] In the prior art various attempts have been made for the fitting of hearing aids to the needs of an individual patient.

[0004] US 4,577,641 relates to a fitting process for a cochlear implant wherein equal loudness contour (ELC) measurements are conducted after the device has been implanted in order to determine the individual optimized gain function of the hearing instrument. The ELC measurements are carried out at the most comfortable loudness level.

[0005] DE 32 05 685 A1 relates to a hearing instrument with an electroacoustic output transducer, wherein a sound generator is integrated within the hearing instrument for performing hearing threshold measurements as a function of frequency.

[0006] DE 199 14 992 A1 relates to the integration of a sound generator for audiometric measurement within a partially or fully implantable hearing instrument for e.g. direct mechanical stimulation of the inner ear.

[0007] According to EP 0 535 425 B1 loudness curves as a function of the sound input level are measured for various frequencies. From these loudness curves contours of equal loudness as a function of frequency are plotted for various loudness values. However, the loudness curves are obtained without the hearing aid being used.

[0008] DE 100 41 726 C1 relates to an implanted hearing instrument with an electromechanical transducer, wherein the quality of the coupling between the transducer and the user's ear is evaluated by measuring the mechanical impedance after implantation of the transducer.

[0009] EP 0 661 905 B1 relates to a fitting model for hearing aids in order to take into account various psychoacoustic effects, i.e. in order to take into account the fact that loudness curves are measured with sinus tones or low-band noise while practical ambient sound, in partic-

ular speech, is perceived by the user in a much more complex manner than sinus tones or narrow-band noise.

[0010] Fitting procedures for hearing instruments with electroacoustic output transducers are suggested in US 6,574,342 B1 and US 6,201,875 B1 which propose to perform measurements of the contours of equal loudness with the hearing instrument worn by the user and with the stimuli created by the hearing instrument itself. In these measurements, for a plurality of frequencies f or frequency bands, the input level of the hearing instrument is varied such that the loudness perceived by the user is kept constant. This procedure is repeated for different values/categories of loudness ranging from very soft to extremely loud. The thus measured contours of equal loudness are used to determine the individual gain function which is finally implemented in the hearing instrument to compensate for the user's individual hearing loss.

[0011] While using the fitting procedures suggested in US 6,574,342 B1 and US 6,201,875 B1 the hearing device can be well fitted to the individual hearing loss experienced by the patient, these procedures are disadvantageous in that a large number of measurements has to be taken. In particular, in the fitting procedures described in US 6,574,342 B1 and US 6,201,875 B1 measurements are taken at 12 different frequencies for 7 different loudness levels. That means that 84 individual reading points are investigated, which necessitates a lengthy and troublesome procedure both for the patient and the physician or audiologist.

[0012] WO 2004/054318 relate to a method for fitting the gain of a hearing aid to the individual hearing loss of the person, wherein the measurements are carried-out with the person using a hearing aid similar to that the person will use in practice after the fitting process, wherein the measurements are carried-out at three different volume/loudness levels, namely at the most comfortable level (MCL), at a loud level and at a soft level, and wherein at each volume level the measurement is repeated at four different frequency bands. With regard to frequency/frequency resolution, each of the volume levels is treated the same, i.e. the measurements are carried-out at the same number of frequency bands and with the same frequency resolution.

[0013] It is an object of the invention to provide for a simple and nevertheless accurate method for individually fitting a hearing instrument comprising an output transducer for stimulation of the human auditory system.

[0014] This object is achieved by a method as defined in claims 1 and 21, respectively.

[0015] The solution according to claim 1 is beneficial in that, by measuring the perceived loudness at the intermediate loudness level for a larger number of frequencies or frequency bands and with a finer frequency resolution than at said low and high loudness levels and calculating the individual gain function to be implemented in the audio signal processing unit in order to achieve the pre-defined target loudness function using the transducer input audio signal levels taken during such measure-

ments, the number of measurement points to be investigated can be substantially reduced.

[0016] The present invention takes advantage of the finding that the fine frequency dependency of the overall transfer function, i.e. that part of the frequency dependency which varies strongly/steeply within short frequency intervals (in other words, the short scale variations), is relatively similar for even significantly different perceived loudness levels of the signal. It has been found that thus, instead of individually determining the transfer functions for every single loudness category by taking measurements at a high frequency resolution for each loudness category of interest, it is usually sufficient to determine the transfer function only for a single intermediate loudness level at a higher frequency resolution, whereas for the low and high loudness levels measurement with low frequency resolution at only a few frequencies/frequency bands, i.e. at only a few measurement points is sufficient, since the actual short scale variations with frequency for those low and high loudness levels usually will be similar to that having been measured for the intermediate loudness level, which thus can be estimated by transferring that having been measured for the intermediate loudness level to the low and high loudness levels. Thus, having determined the frequency dependency of the overall transfer function by conducting measurements with a high frequency resolution at one loudness level, such as the most comfortable level (MCL), it is thus possible to quite precisely interpolate, preferably by linear interpolation, the frequency dependency also for loudness levels in which measurements were taken only for a few frequencies

[0017] It is noted that the finding that the coupling transfer function from the output transducer to the user's hearing usually depends strongly on frequency but less on loudness level, while the hearing loss of the patient usually depends strongly on loudness level but less on frequency, enables separation of these two components by calculations so that common fitting software tools, which usually need these two components as separate input, can be used.

[0018] Preferably, in such measurements the intermediate loudness level is the most comfortable level, which may be from 60 to 70 phon and which is the input sound pressure level at which intelligibility of the stimulus by the user is best and to which the user could comfortably listen over an extended period of time. The low loudness level preferably is the hearing threshold, which is the input sound pressure level at which the stimulus becomes detectable by the user, and the high loudness level preferably is the uncomfortable level (UCL), which is the input sound pressure level at which loudness becomes uncomfortable to the user and the sensation could not be tolerated for an extended period of time.

[0019] Whereas for the intermediate loudness level the transducer input audio signal level should preferably be measured at at least 5 different frequencies or frequency bands, respectively, for the low and/or high loudness lev-

el measurements at 3 to 5 frequencies or frequency bands can be sufficient in the practice of the invention. In the range of 0.75 to 3 kHz which is the range into which usually the resonance of an electromechanical output transducer falls so that the variation of the overall transfer function due to individual spread of the output transducer resonance can be eliminated, each contour of equal loudness preferably is measured at at least 5 different frequencies or frequency bands, respectively.

[0020] Preferably, in order to obtain a good frequency resolution, the transducer input audio signal level for the intermediate loudness level is measured for at least 8 frequencies or frequency bands. An even finer frequency resolution can be obtained by increasing the number of frequencies at which the loudness perception is measured, such as by measuring the transducer input audio signal level for the intermediate loudness level for at least 15 frequencies or frequency bands.

[0021] In a preferred embodiment of the invention the transducer input audio signal level is measured for each loudness level for frequencies or frequency bands in a range of from 100 to 10,000 Hz. Preferably, the frequencies or frequency bands are spaced in equal distances in the range of from 100 to 10,000 Hz.

[0022] In a particularly preferred embodiment of the invention the frequency dependence of the values of the transducer input audio signal level as measured for the intermediate loudness level is used to interpolate between the values of the transducer input audio signal level to be applied to the transducer input as measured for the low and the high loudness level. In this manner the present method enables to obtain functions representing the frequency dependency of the loudness perception at a high frequency resolution also for loudness categories in which readings are taken at a substantially lower frequency resolution, i.e. by taking measurements only for a few frequencies.

[0023] Preferably, the measurements for the intermediate loudness level are conducted as an equal loudness contour measurement, that is as a measurement wherein subsequently for each frequency or frequency band a transducer input audio signal level is selected which causes a constant level of loudness perception for the user.

[0024] Whereas for taking the measurements for the intermediate loudness level preferably narrow band noise is used, the measurements for the low and high loudness levels preferably are conducted with pure sinus tones. Instead of measuring — according to the solution defined in claim 1 - the transducer input audio signal level which has to be applied to the transducer input in order to achieve a certain intermediate perceived loudness level, according to the solution defined in claim 21 a predetermined level of the processed output audio signal at a number of frequencies or frequency bands is present to the user and then the loudness level perceived by the user at the respective frequency or frequency band is measured. Using the thus obtained relationship between

the level of the processed output audio signal, which is used as input signal for the transducer, and the perceived loudness level the overall transfer function can be determined.

[0025] In a preferred embodiment of the present invention transducer input audio signal levels are measured for the low and high loudness levels as an equal loudness contour measurement, wherein subsequently for each frequency or frequency band the transducer input audio signal level is selected such that the same loudness level is perceived by the user. Then a preliminary individual gain function is calculated by taking into account the measured transducer input audio signal levels for the low and high loudness levels, so as to achieve a pre-defined target loudness function which at least in a range of medium input sound pressure levels corresponds to the standard loudness function of a normal hearing person. In a further step, the contour of equal loudness is estimated for the intermediate loudness level from the preliminary individual gain function, and the individual gain function is calculated by correcting the preliminary individual gain function by taking into account the difference between the contour of equal loudness measured for the intermediate loudness and the estimated contour of equal loudness.

[0026] In this embodiment of the invention thus a two-stage fitting procedure is employed, wherein in-situ ELC measurements are made in the second stage, whereby a particularly simple but nevertheless accurate fitting procedure is provided which does not require knowledge of the transfer function of the components of the hearing instrument; in particular, it does not require knowledge the transfer function of the electromechanical or electroacoustical output transducer and the coupling to the user's anatomy. In particular, with the help of the ELC measurements in the second stage of the fitting procedure the hearing instrument can be compensated for the usually unknown and significantly spreading resonance of the electromechanical output transducer in the range of 0.75 to 3 kHz.

[0027] The reason for performing in this embodiment initial coarse audiogram measurements is to determine preliminary fitting parameters in order to enable accurate measurements of the contour of equal loudness in the second step, with the hearing instrument already being operated in a manner taking into account those preliminary fitting parameters (e.g. hearing threshold, MCL, UCL). Thereby it becomes possible to perform the contour of equal loudness measurements with the hearing instrument already being operated in a manner more or less close to the finally fitted hearing instrument.

[0028] Generally, the measurement of the contour of equal loudness should have a finer frequency resolution than the initial audiogram measurements, thereby serving as a correction of the initial, relatively coarse audiogram measurement. To this end, the number of frequencies or frequency bands at which the contour of equal loudness is measured preferably is larger than the

number of frequencies or frequency bands at which the initial audiogram measurement is performed.

[0029] When estimating the contour of equal loudness from the initial loudness measurements, this can be done by linear interpolation between the measured frequencies or frequency bands, respectively.

[0030] Preferably, the initial audiogram measurements are performed with pure sinus tones, while the measurement of the contour of equal loudness is performed with narrow-band noise.

[0031] The target loudness function at least in the range of medium input sound pressure levels preferably corresponds to the standard loudness function of a normal hearing person. For medium input sound pressure levels an individual gain function thus can be determined by adding the difference between the standard loudness function of a normal hearing person and the initially determined individual loudness function being derived from the audiogram data to the preset standard gain function.

[0032] For low and high input sound pressure levels the gain in the target loudness function may be progressively reduced compared to the gain for medium input sound pressure levels, i.e. for low and high sound input pressure levels the gain may be smaller than the sum of the difference between the standard loudness function of a normal hearing person and the determined individual loudness function and the preset standard gain function. For low input sound pressure levels, the gain in the target loudness function may be progressively reduced towards low input sound pressure levels, while for high input sound pressure levels the gain in the target loudness function may be progressively reduced towards high input sound pressure levels. Above a given high input sound pressure level the gain may be reduced below zero in order to provide for a maximum power output limitation, so that the hearing instrument saturates at very high input sound pressure levels.

[0033] While the transducer input audio signal used in the measurements can be generated by providing corresponding sound to the microphone, preferably the stimulus is generated by the audio signal processing unit itself. To this end, the audio signal processing unit can be provided with a sound generator. Such measurements, which are more accurate and reproducible than earphone measurements, are made possible by the fact that usually the transfer function of ambient sound to the audio signal processing unit via the microphone is known.

[0034] According to a preferred embodiment, an electromechanical output transducer is used which is directly connected, via an artificial incus, with the stapes or the footplate of the stapes or with the round window or an artificial window of the cochlear wall. Such hearing instruments also are known as DACS (Direct Acoustic Cochlear Stimulator).

[0035] However, the fitting method according to the invention also can be used for hearing instruments with electroacoustic output transducer or for cochlea implants.

[0036] In the following, examples of the invention will be described in more detail by reference to the attached drawings.

- Fig. 1 is a schematic view of a hearing instrument according to the invention;
- Fig. 2 is an example of the spread of the electro-mechanical output transducer transfer function;
- Fig. 3 shows an example of the loudness curve of a normal-hearing person and an measured individual loudness curve of a hearing impaired person using a hearing instrument operated at a preset standard gain function;
- Fig. 4 shows an example of a preliminary individual gain function of the hearing instrument derived from the measured individual loudness curves;
- Fig. 5 shows an example of hearing instrument output curves estimated from the measurements of the individual loudness curves as a function of frequency for several input levels;
- Fig. 6 shows an example of an equal loudness contour of a normal hearing person at 65 phon, wherein the input level necessary to achieve this loudness is given as a function of frequency, together with arrows indicating the difference between a measured equal loudness contour of the person using the hearing instrument operated at the preliminary individual gain function to an equal loudness contour estimated by frequency interpolation from the initial loudness measurements;
- Fig. 7 shows how the obtained differences of the individually measured equal loudness contour curve and the estimated equal loudness contour curve, i.e. the arrows of Fig. 6, are used to correct the 75 dB input level curve;
- Fig. 8 shows the hearing instrument output curves of Fig. 5 after having been corrected according to the equal loudness contour measurements;
- Fig. 9 is a diagram illustrating a signal conversion as performed in a hearing instrument;
- Fig. 10 is a graphical representation of the points of measurement;
- Fig. 11A shows a measuring curve obtained at the

most comfortable level (MCL);

Fig. 11B shows the results obtained by the measurements taken at the most uncomfortable level (UCL), wherein the data curve is obtained by interpolation between the measuring data using the curve shown in Fig. 11A; and

Fig. 11B shows the results obtained by the measurements taken at the hearing threshold (THR), wherein the data curve is obtained by interpolation between the measuring data using the curve shown in Fig. 11A.

[0037] To facilitate understanding of the fitting procedure, signal conversion as performed in a hearing instrument will be explained below by reference to Fig. 9. As it is schematically shown in Fig. 9 a sound level L_0 is applied to a microphone M which is arranged in an environment U. Microphone M converts the sound signal into an electric signal level L_1 , which by means of an audio signal processing unit E is converted into an electric signal level L_2 to be applied as input signal to an output transducer TD. Output transducer TD, which can be an electroacoustic transducer (i.e. a speaker/receiver), an electrode for direct electric stimulation of the cochlea or an electromechanical output transducer for direct mechanical stimulation of the middle ear or the inner ear, and which in case that the output transducer TD is an electrode or an electromechanical output transducer has to be implanted, is coupled to the hearing apparatus EAR of the patient. In dependency of the type of output transducer used, the coupling, for example, may be acoustically via the tympanic membrane, or mechanically via the stapes or the oval window, so as to generate within the hearing apparatus EAR a stimulus which is perceived by the patient as loudness sensation L_3 .

[0038] Conversion of the original sound level L_0 into the loudness sensation L_3 perceived by the patient involves a number of transfer functions which also are indicated in Fig. 9. In particular, conversion of the original sound level L_0 into the electric signal level L_1 is governed by a transfer function T_{01} which basically is dependent on the frequency of the signal presented to the microphone and thus can be assumed to be known. The transfer function T_{12} which describes conversion of electric signal level L_1 to processed electric signal level L_2 to be applied as input signal to output transducer TD can be adjusted by means of audio signal processing unit E. For audio signal measurements, instead of using an airborne sound signal to be picked up by microphone M, there can be provided a signal processor SG which feeds a known sound level L_2 to output transducer TD. The transfer function T_{23} which associates a certain loudness perception to a certain input signal level L_2 of the transducer TD generally is not known and depends on the individual circumstances of the patient. In particular, transfer function T_{23} combines a coupling portion T_C which accounts

for the transducer resonance and the coupling of the transducer to the anatomic structures of the patient as well as a hearing loss portion T_{HL} which represents the individual hearing loss experienced by the patient. In order to be able to determine the overall transfer function T_{03} by which conversion of a sound event into a hearing impression can be described and which is composed of the above partial transfer function T_{01} , T_{12} and T_{23} , transfer function T_{23} has to be determined in the course of the fitting procedure.

[0039] In view of the above the fitting procedure aims at adjusting the audio signal processing unit E (and hence transfer function T_{12}) such that the overall transfer function T_{03} (and hence association of a certain loudness perception L_3 to a certain input signal level L_2) assumes a certain shape, which often, at least for intermediate loudness levels, approximates the overall transfer function T_{03} that is realized in normal healthy hearing. For low and high loudness levels often an overall transfer function T_{03} is preferred which differs from that achieved in normal hearing. Thus, whereas for low loudness levels often a so-called "Soft Squelch" function is implemented by which the gain function is progressively reduced towards low input sound levels, for high loudness levels many patients prefer a limitation of the loudness level, i.e. a compression of the gain function.

[0040] In the course of the fitting procedure first the initially unknown transfer function T_{23} is determined with the aid of audiologic measurements. In a second step, using the known microphone transfer function T_{01} and the required transfer function T_{12} of the audio signal processing unit E as a function of loudness level and frequency, a desired overall transfer function T_{03} can be calculated and implemented in the audio signal processing unit E.

[0041] Fig. 1 is a schematic view of an example of a hearing instrument according to the invention comprising an external part 10 and an implantable part 12 which are connected via a percutaneous plug 14. The external part 10 comprises a housing 16 to be worn somewhere at the user's body, for example, behind the ear. The housing 16 forms a control unit 18 which comprises at least one microphone 20 for converting ambient sound into an input audio signal, a battery 22, a data memory 24 and a digital audio signal processing unit 26. The digital audio signal processing unit 26 is for processing the audio input signal provided by the microphone 20 into a processed output audio signal by applying a gain function, which depends on frequency and audio signal input level, to the input audio signal provided by the microphone 20. The gain function, together with other operating parameters and the operating program for the digital audio signal processing unit 26, may be stored in the memory 24. The digital audio signal processing unit also may comprise a sound generator 28. In an alternative embodiment the sound generator 28 may be provided separate from the digital audio signal processing unit 26.

[0042] The control unit 18 is connected to the percu-

taneous plug 14 via a tube 30 which houses wires for providing the output audio signal from the digital audio signal processing unit 26 to an electromechanical output transducer 32 and for supplying the electromechanical output transducer 32 with power from the battery 22. To this end, the output transducer 32 is electrically connected to the percutaneous plug 14 via a tube 34. The implantable part 12 consists of the output transducer 32, the tube 34 and the implantable part of the plug 14. The implantable part 12 is implanted into the skull of the user, with the output transducer 32 comprising a bone plate 36 which is fixed at the user's skull.

[0043] The output transducer comprises a housing 38 comprising a drive 40 for driving a rod 42 for reciprocating movement. The free end of the rod 42 is provided with an artificial incus 44 which is to be mechanically connected to the cochlea of the user. The fixation of the artificial incus 44 at the user's cochlea can be achieved by surgical techniques which are known as stapedotomy or stapedectomy. Conventionally, these techniques are used for connecting the artificial incus of a middle ear prosthesis to the patient's stapes (stapedotomy) or footplate of the stapes (stapedectomy) when treating otosclerosis.

[0044] The drive 40 may be an electromagnetic drive (an example of which is described in US 6,315,710 B1) or a piezoelectric drive (an example of which is described in US 6,554,762 B2).

[0045] The hearing instrument of Fig. 1 is particularly suited for patients who cannot be effectively treated with electroacoustic hearing aids alone and therefore would require surgery anyhow. The hearing instrument used in the present invention completely bypasses the middle ear and thus does not require a functional middle ear.

[0046] Fitting of such hearing instrument to the individual user, i.e. determination of the most appropriate gain function, is critical for several reasons. First, the transducer resonance may spread significantly from device to device (this is shown by two examples in Fig. 2). Second, the coupling of the output transducer to the cochlea is not known and may spread significantly from case to case. Third, the output of the output transducer is not available in acoustic form.

[0047] Therefore it is necessary to perform a fitting procedure in which the gain function which the hearing instrument applies to the sound signal is adapted to the individual circumstances and requirements of the user of the hearing instrument.

[0048] In such fitting procedure audiogram measurements are made wherein loudness perception of a stimulus by the user is tested when using the hearing instrument. In particular, upon having pre-defined a desired target loudness function, measurements are taken of the transducer input audio signal level which has to be applied to the transducer input in order to achieve a certain intermediate perceived loudness level, which preferably is the most comfortable level (MCL). These measurements are repeated for a number of frequencies or frequency bands. Most preferably the measurements for

the intermediate loudness level are conducted with a frequency resolution which corresponds to the frequency resolution of the hearing instrument.

[0049] As it is indicated in Fig. 10, which illustrates the points where measurements are taken in terms of stimulus frequency f and perceived loudness L_3 , the measurements of the perceived loudness level preferably are conducted as an equal loudness contour measurement, wherein a transducer input audio signal level L_2 is selected such that the same loudness level L_3 is perceived by the user.

[0050] Fig. 11A illustrates an exemplary chart of results obtained by the measurements taken at the most comfortable level (MCL) and indicates for each frequency tested the respective transducer input audio signal level L_2 that is required to obtain that the constant loudness level L_3 . As can be seen from Fig. 11A, the transfer function T_{23} which describes the relationship between the transducer input audio signal level L_2 and the perceived loudness level L_3 is not a linear function but usually shows large variations over the tested frequency range.

[0051] Since, however, such variation of the perceived loudness level L_3 in the course of the frequency range was found to be largely independent from the loudness level being tested, in the method suggested herein the measurements for low and high loudness levels such as the hearing threshold (THR) and the uncomfortable level (UCL), respectively are restricted to only a few measurement points, for example to only three frequencies, as it is indicated in Fig. 10.

[0052] As it is shown in Figs. 11B and Fig. 11C, using the frequency dependency obtained at high frequency resolution for the intermediate perceived loudness level shown in Fig. 11, curves for the low and high loudness levels are obtained by interpolation between the measurement values taken for the low and high loudness levels at the lower frequency resolution.

[0053] In a practical example, the present fitting procedure further may be designed as a two-stage fitting procedure, wherein at the first stage the hearing instrument is used in order to perform audiogram measurements at a few frequencies, whereby some points of the individual loudness curve versus sound input level are obtained between which the individual loudness curve is interpolated. From the individual loudness curve a preliminary individual gain function is calculated which may be used for operating the hearing instrument at the second stage (in particular if the stimulus is provided by an earphone to the microphone 20) wherein at least one contour of equal loudness is measured with a finer frequency resolution than that of the loudness curve of the first stage. The measured contour of equal loudness then is used for correcting the individual preliminary gain function, in particular in between the frequencies already measured in the first stage, in order to consider, for example, the relatively sharp resonance of the output transducer. Thereby from the individual preliminary gain function obtained in the first stage a corrected individual gain

function is determined in the second stage, which then is finally used for operating the hearing instrument.

[0054] The audiogram measurements may be performed such that for each frequency at least two points of the loudness curve are determined, usually the hearing threshold (denoted by A in Fig. 3) and at least one of MCL (denoted by B) and UCL (denoted by C). Such loudness curve as shown in Fig. 3 should be determined at least for four different frequencies spread over the most relevant part of the audible frequencies. The loudness measurements of the first stage are performed with pure sinus tones. While in principle it would be possible to provide the stimulus by an earphone to the microphone 20 (in that case a standard gain function would be used for operating the hearing instrument in the first stage, which preferably is linear with respect to sound input level), it is preferred to generate the stimulus by the sound generator 28 within the control unit 18.

[0055] For determining the preliminary individual gain function, at each test frequency the difference between the measured individual loudness curve and the standard loudness curve of the normal hearing person, i.e. the difference in input level necessary for obtaining the same loudness perception, is considered. This is indicated by arrows D1 and D2 in Fig. 3. To this end, the individual loudness curve is interpolated linearly between the measured test input levels. Each input level difference D1 and D2 corresponds to the necessary additional gain at the respective input level of the standard loudness curve (which is labeled S in Fig. 3). The result is shown in Fig. 4 wherein the additional gain relative to the standard gain function necessary for approaching the loudness curve of a normal-hearing person is shown for a given frequency as a function of the input level.

[0056] For low input levels the gain may be progressively reduced towards low input levels regarding the values obtained from Fig. 3 in order to implement a function which is known as "soft squelch" and which serves to reduce or eliminate microphone noise otherwise occurring at very low input levels. At high input levels the gain may be progressively reduced towards high input levels relative to the gain determined from Fig. 3 in order to implement a "maximum power output" (MPO) function which serves to avoid uncomfortably high loudness values so that the UCL should not be exceeded.

[0057] From this first stage measurements for each test frequency an individual preliminary gain function is obtained by adding the standard gain function used during the audiogram measurements to the gain curve shown in Fig. 4.

[0058] The obtained data could be represented in an alternative manner as shown in Fig. 5, wherein the transducer output level is plotted as function of frequency for various input levels. Between the test frequencies f_0 to f_3 the values have been interpolated linearly. The transducer output level shown in Fig. 5 corresponds to the preliminary individual gain of the hearing instrument plus the input level.

[0059] At the second stage of the fitting procedure, the hearing instrument is operated with the preliminary individual gain function determined at the first stage in order to measure at least one contour of equal loudness (however, use of preliminary individual gain function for operating the hearing instrument is not necessary if the stimulus is generated by the sound generator 28). Preferably, the contour of equal loudness is measured at the MCL, for example, at 65 phon. In contrast to the audiogram measurements of the first stage, narrow-band noise other than pure sinus tones is used as the stimulus. Analogously to the first stage measurements, the stimulus preferably is provided by the internal sound generator 28 of the control unit 18. In order to determine the contour of equal loudness, for a number of test frequencies the input level of the stimulus is varied until the desired loudness is perceived by the user.

[0060] The test frequencies for the ELC measurements are selected such that the frequency resolution is improved regarding the audiogram measurements of the first stage. In particular, between two of the test frequencies of the first stage at least one test frequency of ELC measurement should be located. In the example shown in Fig. 6, two additional test frequencies of the second stage are located between each pair of adjacent test frequencies of the first stage. Generally, the number of test frequencies of the ELC measurements is higher than the number of test frequencies of the first stage loudness measurements. In the example shown in Fig. 6, twenty test frequencies are used between 0.125 and 8 kHz. The solid line in Fig. 6 shows an example of an ELC of a normal hearing person. The arrows in Fig. 6 represent the difference between the measured ELC and the ELC for the same loudness as estimated from the loudness measurements of the first stage by linear interpolation between the test frequencies of the first stage loudness measurements. In other words, the arrows of Fig. 6 essentially show the deviation of the actually measured ELC from the linear interpolation. However, even if the test frequencies of the first and second stage measurements coincide, there may be some deviation, since the first stage loudness measurements were performed with pure sinus tones, while the second stage ELC measurements were performed with narrow-band noise, which different stimuli may cause different loudness perception even for the same input level.

[0061] It is obvious from Fig. 6 that in the region around 2 kHz the most pronounced deviation from the linear interpolation is observed, which is due to the relatively sharp resonance of the output transducer 32 in that frequency range. Preferably, the ELC measurements include at least five test frequencies between 0.75 and 3 kHz in order to be able to compensate the resonance of the output transducer 32 accurately.

[0062] Fig. 7 is similar to Fig. 5, with the arrows of Fig. 6 having been added to the 75 dB input level curve (the transducer output level is input level times gain provided by the hearing instrument).

[0063] Fig. 8 is a representation similar to Fig. 7, wherein the transducer output level curves have been corrected according to the ELC measurement arrows, with the regions between the test frequencies having been interpolated. Since the output transducer resonance is expected to be linear regarding input level, the corrections obtained from this single ELC measurement can be extrapolated linearly to ELC at other loudness values, so that measurement of ELC for one single loudness is sufficient. This is how the corrected curves at input levels other than 75 dB of Fig. 8 are obtained.

[0064] From the transducer output level curves of Fig. 8 the corrected individual gain function can be determined, since the gain function is the ratio of the transducer output level to the input level.

[0065] Finally, the hearing instrument is operated with the corrected individual gain function obtained by the above-described fitting procedure.

Claims

1. A method for individually fitting a hearing instrument (10, 12) to a user, comprising at least one microphone (20) for generating an input audio signal from ambient sound, an audio signal processing unit (26) for processing the input audio signal into a processed output audio signal, and a transducer for stimulation of the human auditory system according to the processed output audio signal as input to said transducer, the method comprising:

- (a) providing the user with the hearing instrument and starting operation of the hearing instrument;
- (b) pre-defining a desired target loudness function, wherein loudness perception of a stimulus by the user when using the hearing instrument is defined as function of frequency and input sound pressure level at the microphone;
- (c) measuring for a given measurement parameter set of perceived loudness levels and frequencies or frequency bands the respective transducer input audio signal level to be applied to the transducer input in order to achieve the respective perceived loudness level at the respective frequency or frequency band, said measurement parameter set comprising at least a low loudness level, an intermediate loudness level and a high loudness level, and said intermediate loudness level being measured for a larger number of frequencies or frequency bands and with a finer frequency resolution than said low and high loudness levels;
- (d) calculating an individual gain function to be implemented in the audio signal processing unit in order to achieve the pre-defined target loudness function of step (b) by taking into account

- the measured transducer input audio signal levels of step (c);
(e) operating the hearing instrument with the individual gain function of step (d).
2. The method of claim 1, wherein in step (c) the intermediate loudness level is the most comfortable level, which is the input sound pressure level at which intelligibility of the stimulus by the user is best and to which the user could comfortably listen over an extended period of time,
 3. The method of claim 1 or 2, wherein in step (c) the low loudness level is the hearing threshold, which is the input sound pressure level at which the stimulus becomes detectable by the user.
 4. The method of one of the preceding claims, wherein in step (c) the high loudness level is the uncomfortable level, which is the input sound pressure level at which loudness becomes uncomfortable to the user and the sensation could not be tolerated for an extended period of time.
 5. The method of one of the preceding claims, wherein the transducer input audio signal level is measured in step (c) for the intermediate loudness level for at least 8 frequencies or frequency bands.
 6. The method of claim 5, wherein the transducer input audio signal level is measured in step (c) for the intermediate loudness level for at least 15 frequencies or frequency bands.
 7. The method of one of the preceding claims, wherein the transducer input audio signal level is measured in step (c) for the intermediate loudness level at at least 5 different frequencies or frequency bands, respectively, in the range from 0.75 to 3 kHz.
 8. The method of one of the preceding claims, wherein the transducer input audio signal level is measured in step (c) for the low and/or high loudness level for 3 to 5 frequencies or frequency bands.
 9. The method of claim 8, wherein the transducer input audio signal level is measured in step (c) for each loudness level except for said intermediate loudness level for 3 to 5 frequencies or frequency bands.
 10. The method of one of the preceding claims, wherein the transducer input audio signal level is measured in step (c) for each loudness level for frequencies or frequency bands in a range from 100 to 10,000 Hz.
 11. The method of claim 10, wherein the transducer input audio signal level is measured in step (c) for each loudness level for frequencies or frequency bands which are spaced in equal distances in a range from 100 to 10,000 Hz.
 12. The method of one of the preceding claims, wherein the frequency dependence of the values of the transducer input audio signal level as measured in step (c) for the intermediate loudness level is used to interpolate between the values of the transducer input audio signal level to be applied to the transducer input as measured in step (c) for the low and the high loudness level.
 13. The method of one of the preceding claims, wherein the measurements of step (c) for the intermediate loudness level are conducted as an equal loudness contour measurement, wherein subsequently for each frequency or frequency band the transducer input audio signal level is selected such that the same loudness level is perceived by the user.
 14. The method of one of the preceding claims, wherein the measurements of step (c) for the low and high loudness levels are conducted as a series of constant frequency measurements wherein for each frequency or frequency band the transducer input audio signal level is selected such that first the low and then the high loudness level or first the high and then the low loudness level is perceived by the user.
 15. The method of one of the preceding claims, wherein the measurements of step (c) for the intermediate loudness level are conducted with narrow band noise.
 16. The method of one of the preceding claims, wherein the measurements of step (c) for the low and high loudness levels are conducted with pure sinus tones.
 17. The method of one of the preceding claims, wherein the values of the transducer input audio signal measured in step (c) for each frequency or frequency band for the intermediate loudness level are interpolated linearly.
 18. The method of one of the preceding claims, wherein in step (c) said measurement parameter set comprises only said low, intermediate and high loudness levels.
 19. The method of one of the preceding claims, wherein the frequency resolution of the measurements in step (c) for the intermediate loudness level corresponds to the frequency resolution of the hearing instrument.
 20. The method of one of the preceding claims, wherein in step (c) transducer input audio signal levels are measured for the low and high loudness levels as

an equal loudness contour measurement, wherein subsequently for each frequency or frequency band the transducer input audio signal level is selected such that the same loudness level is perceived by the user

a preliminary individual gain function is calculated by taking into account the measured transducer input audio signal levels for the low and high loudness levels, so as to achieve a pre-defined target loudness function which at least in a range of medium input sound pressure levels corresponds to the standard loudness function of a normal hearing person; the contour of equal loudness is estimated for the intermediate loudness level from the preliminary individual gain function; and the individual gain function is calculated by correcting the preliminary individual gain function by taking into account the difference between the contour of equal loudness measured in step (c) for the intermediate loudness and the estimated contour of equal loudness.

- 21.** A method for individually fitting a hearing instrument (10, 12) to a user, comprising at least one microphone (20) for generating an input audio signal from ambient sound, an audio signal processing unit (26) for processing the input audio signal into a processed output audio signal, and a transducer for stimulation of the human auditory system according to the processed output audio signal as input to said transducer, the method comprising:

- (a) providing the user with the hearing instrument and starting operation of the hearing instrument;
- (b) pre-defining a desired target loudness function, wherein loudness perception of a stimulus by the user when using the hearing instrument is defined as function of frequency and input sound pressure level at the microphone;
- (c) measuring for a given measurement parameter set of levels of the processed output audio signal and frequencies or frequency bands the loudness level perceived by the user at the respective frequency or frequency band, said measurement parameter set comprising at least a low audio signal level, an intermediate audio signal level and a high audio signal level, and said intermediate audio signal level being measured for a larger number of frequencies or frequency bands and with a finer frequency resolution than said low and high audio signal levels;
- (d) calculating an individual gain function to be implemented in the audio signal processing unit in order to achieve the pre-defined target loudness function of step (b) by taking into account the perceived loudness levels measured in step (c);

- (e) operating the hearing instrument with the individual gain function of step (d).

- 22.** The method of claim 21, wherein the perceived loudness level is measured in step (c) for the intermediate audio signal level for at least 8 frequencies or frequency bands.
- 23.** The method of claim 22, wherein the perceived loudness level is measured in step (c) for the intermediate audio signal level for at least 15 frequencies or frequency bands.
- 24.** The method of one of claims 21 to 23, wherein the perceived loudness level is measured in step (c) for the intermediate audio signal level at at least 5 different frequencies or frequency bands, respectively, in the range from 0.75 to 3 kHz
- 25.** The method of one of claims 21 to 24, wherein the perceived loudness level is measured in step (c) for the low and/or high audio signal level for 3 to 5 frequencies or frequency bands.
- 26.** The method of claim 24, wherein the perceived loudness level is measured in step (c) for each loudness level except for said intermediate audio signal level for 3 to 5 frequencies or frequency bands.
- 27.** The method of one of claims 21 to 26, wherein the perceived loudness level is measured in step (c) for each audio signal level for frequencies or frequency bands in a range from 100 to 10,000 Hz.
- 28.** The method of claim 27, wherein the perceived loudness level is measured in step (c) for each audio signal level for frequencies or frequency bands which are spaced in equal distances in a range from 100 to 10,000 Hz.
- 29.** The method of one of claims 21 to 28, wherein the frequency dependence of the values of the perceived audio signal level as measured in step (c) for the intermediate audio signal level is used to interpolate between the values of the perceived loudness level measured in step (c) for the low and the high audio signal level.
- 30.** The method of one of claims 21 to 29, wherein the measurements of step (c) for the intermediate audio signal level are conducted with pure sinus tones.
- 31.** The method of one of claims 21 to 30, wherein the measurements of step (c) for the low and high audio signal levels are conducted with narrow band noise.
- 32.** The method of one of claims 21 to 31, wherein the values of the perceived loudness level measured in

step (c) for each frequency or frequency band for the intermediate audio signal level are interpolated linearly.

33. The method of one of the preceding claims, wherein the target loudness function at least in a range of medium input sound pressure levels corresponds to the standard loudness function of a normal hearing person. 5
34. The method of claim 33, wherein for low input sound pressure levels the target loudness function is progressively reduced towards low input sound pressure levels with respect to the standard loudness function of a normal hearing person. 10
35. The method of one of claims 33 and 34, wherein for high input sound pressure levels the target loudness function is progressively reduced towards high input sound pressure levels with respect to the standard loudness function of a normal hearing person. 15
36. The method of one of the preceding claims, wherein the transducer input audio signal used in the measurements of step (c) is generated by the audio signal processing unit (26). 20
37. The method of one of claims 1 to 35, wherein the transducer input audio signal used in the measurements of step (c) is generated by providing corresponding sound to the microphone (20). 25
38. The method of one of the preceding claims, wherein the output transducer is an electromechanical output transducer (32) for direct mechanical stimulation of the middle ear or the inner ear. 30
39. The method of claim 38, wherein the electromechanical output transducer (32) is directly connected in step (a) with the stapes, footplate of stapes or the cochlea wall. 35
40. The method of one of claims 1 to 36, wherein the output transducer is an electroacoustic output transducer. 40

Patentansprüche

1. Verfahren zum individuellen Anpassen einer Hörvorrichtung (10, 12) an einen Nutzer, mit mindestens einem Mikrofon (20) zum Erzeugen eines Eingangsaudiosignals aus Umgebungsschall, einer Audiosignalverarbeitungseinheit (26) zum Verarbeiten des Eingangsaudiosignals in ein verarbeitetes Ausgangsaudiosignal, und einem Wandler zum Stimulieren des menschlichen Gehörs gemäß dem verarbeiteten Ausgangsaudiosignal als Eingangssignal 50

für den Wandler, wobei im Zuge des Verfahrens:

- (a) der Nutzer mit der Hörvorrichtung versorgt wird und der Betrieb der Hörvorrichtung gestartet wird;
- (b) eine gewünschte Ziellautheitsfunktion vordefiniert wird, wobei die Lautheitswahrnehmung eines Stimulus durch den Nutzer bei Benutzung der Hörvorrichtung als Funktion der Frequenz und des Eingangsschalldruckpegels an dem Mikrofon festgelegt wird;
- (c) für einen vorgegebenen Messparametersatz von wahrgenommenen Lautheitspegeln und Frequenzen oder Frequenzbändern der entsprechende Wandleringangsaudiosignalpegel gemessen wird, mit welchem der Wandleringang beaufschlagt werden muss, um den entsprechenden wahrgenommenen Lautheitspegel bei der entsprechenden Frequenz oder dem entsprechenden Frequenzband zu erzielen, wobei der Messparametersatz mindestens einen niedrigen Lautheitspegel, einen mittleren Lautheitspegel und einen hohen Lautheitspegel aufweist, und wobei der mittlere Lautheitspegel für eine größere Anzahl von Frequenzen oder Frequenzbändern und mit einer höheren Auflösung als der niedrige Lautheitspegel und der hohe Lautheitspegel gemessen wird;
- (d) eine individuelle Verstärkungsfunktion berechnet wird, die in der Audiosignalverarbeitungseinheit zu implementieren ist, um die vordefinierte Ziellautheitsfunktion von Schritt (b) unter Berücksichtigung der gemessenen Wandleringangsaudiosignalpegel von Schritt (c) zu erzielen;
- (e) die Hörvorrichtung mit der individuellen Verstärkungsfunktion von Schritt (d) betrieben wird.

2. Verfahren gemäß Anspruch 1, wobei im Schritt (c) es sich bei dem mittleren Lautheitspegel um den angenehmsten Pegel handelt, welcher der Eingangsschalldruckpegel ist, bei welchem die Verständlichkeit des Stimulus durch den Nutzer am höchsten ist und bei welchem der Nutzer in angenehmer Weise über einen längeren Zeitraum zuhören kann.
3. Verfahren gemäß Anspruch 1 oder 2, wobei im Schritt (c) es sich bei dem niedrigen Lautheitspegel um die Hörschwelle handelt, die der Eingangsschalldruckpegel ist, bei welchem der Stimulus durch den Nutzer wahrnehmbar wird.
4. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei im Schritt (c) es sich bei dem hohen Lautheitspegel um den unangenehmen Pegel handelt, welcher der Eingangsschalldruckpegel ist, bei welchem die Lautheit für den Nutzer unangenehm wird und die Hörempfindung nicht über einen längeren 55

ren Zeitraum ertragen werden kann.

5. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für den mittleren Lautheitspegel für mindestens acht Frequenzen oder Frequenzbänder gemessen wird. 5
6. Verfahren gemäß Anspruch 5, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für den mittleren Lautheitspegel für mindestens 15 Frequenzen oder Frequenzbänder gemessen wird. 10
7. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für den mittleren Lautheitspegel bei mindestens 5 verschiedenen Frequenzen bzw. Frequenzbändern im Bereich von 0,75 bis 3 kHz gemessen wird. 15
8. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für den niedrigen und/oder hohen Lautheitspegel für 3 bis 5 Frequenzen oder Frequenzbänder gemessen wird. 20
9. Verfahren gemäß Anspruch 8, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für jeden Lautheitspegel mit Ausnahme des mittleren Lautheitspegels für 3 bis 5 Frequenzen oder Frequenzbänder gemessen wird. 25
10. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für jeden Lautheitspegel für Frequenzen oder Frequenzbänder im Bereich von 100 bis 10.000 Hz gemessen wird. 30
11. Verfahren gemäß Anspruch 10, wobei der Wandlereingangsaudiosignalpegel im Schritt (c) für jeden Lautheitspegel für Frequenzen oder Frequenzbänder gemessen wird, die im gleichen Abstand im Bereich von 100 bis 10.000 Hz angeordnet sind. 35
12. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Frequenzabhängigkeit der Werte des Wandlereingangsaudiosignalpegels, die im Schritt (c) für den mittleren Lautheitspegel gemessen wurden, verwendet werden, um zwischen den im Schritt (c) für den niedrigen Lautheitspegel und den hohen Lautheitspegel gemessenen Werten des dem Wandlereingang zuzuführenden Wandlereingangsaudiosignalpegels zu interpolieren. 40
13. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Messungen von Schritt (c) für den mittleren Lautheitspegel als eine Messung von Linien gleicher Lautheit durchgeführt werden, wobei 45

für jede Frequenz oder jedes Frequenzband der Wandlereingangsaudiosignalpegel nacheinander so ausgewählt wird, dass der gleiche Lautheitspegel vom Nutzer wahrgenommen wird.

14. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Messungen von Schritt (c) für den niedrigen Lautheitspegel und den hohen Lautheitspegel als eine Reihe von Messungen mit konstanter Frequenz durchgeführt werden, wobei für jede Frequenz oder jedes Frequenzband der Wandlereingangsaudiosignalpegel so ausgewählt wird, dass zuerst der niedrige und dann der hohe Lautheitspegel oder zuerst der hohe und dann der niedrige Lautheitspegel vom Nutzer wahrgenommen wird. 50
15. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Messungen von Schritt (c) für den mittleren Lautheitspegel mit schmalbandigem Rauschen durchgeführt werden. 55
16. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Messungen von Schritt (c) für den niedrigen Lautheitspegel und den hohen Lautheitspegel mit reinen Sinustönen durchgeführt werden.
17. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die im Schritt (c) für jede Frequenz oder jedes Frequenzband für den mittleren Lautheitspegel gemessenen Werte des Wandlereingangsaudiosignalpegels linear interpoliert werden.
18. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei im Schritt (c) der Messparametersatz nur den niedrigen, den mittleren und den hohen Lautheitspegel umfasst.
19. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Frequenzauflösung der Messungen im Schritt (c) für den mittleren Lautheitspegel der Frequenzauflösung der Hörvorrichtung entspricht.
20. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei in Schritt (c) Wandlereingangsaudiosignalpegel für den niedrigen Lautheitspegel und den hohen Lautheitspegel als Messungen mit Linien gleicher Lautheit gemessen werden, wobei der Wandlereingangsaudiosignalpegel für jede Frequenz oder jedes Frequenzband so ausgewählt wird, dass der gleiche Lautheitspegel vom Nutzer wahrgenommen wird; eine vorläufige individuelle Verstärkungsfunktion berechnet wird, indem die gemessenen Wandlereingangsaudiosignalpegel für den niedrigen Lautheitspegel und den hohen Lautheitspegel berücksichtigt

werden, um eine vordefinierte Ziellautheitsfunktion zu erzielen, welche mindestens in einem Bereich mittlerer Eingangsschalldruckpegel der Standardlautheitsfunktion einer normal hörenden Person entspricht;
 die Linie gleicher Lautheit für den mittleren Lautheitspegel aus der vorläufigen individuellen Verstärkungsfunktion abgeschätzt wird; und
 die individuelle Verstärkungsfunktion berechnet wird, indem die vorläufige individuelle Verstärkungsfunktion korrigiert wird, indem der Unterschied zwischen der Linie gleicher Lautheit gemäß der Messung in Schritt (c) für die mittlere Lautheit und die abgeschätzte Linie gleicher Lautheit herangezogen werden.

- 21.** Verfahren zum individuellen Anpassen einer Hörvorrichtung (10, 12) an einem Nutzer, mit mindestens einem Mikrofon (20) zum Erzeugen eines Eingangsaudiosignals aus Umgebungsschall, einer Audiosignalverarbeitungseinheit (26) zum Verarbeiten des Eingangsaudiosignals zu einem verarbeiteten Ausgangsaudiosignal, und einem Wandler zum Stimulieren des menschlichen Gehörs gemäß dem verarbeiteten Ausgangsaudiosignal als Eingangssignal des Wandlers, wobei im Zuge des Verfahrens:

(a) der Nutzer mit der Hörvorrichtung versorgt wird und der Betrieb der Hörvorrichtung gestartet wird;

(b) eine gewünschte Ziellautheitsfunktion vordefiniert wird, wobei die Lautheitswahrnehmung eines Stimulus durch den Nutzer bei Verwendung der Hörvorrichtung als Funktion der Frequenz und des Eingangsschalldruckpegels an dem Mikrofon definiert ist;

(c) für einen vorgegebenen Messparametersatz von Pegeln des verarbeiteten Ausgangsaudiosignals und Frequenzen oder Frequenzbändern der von dem Nutzer bei der entsprechenden Frequenz oder dem entsprechenden Frequenzband wahrgenommene Lautheitspegel gemessen wird, wobei der Messparametersatz mindestens einen niedrigen Audiosignalpegel, einen mittleren Audiosignalpegel und einen hohen Audiosignalpegel aufweist, und wobei der mittlere Audiosignalpegel für eine größere Zahl von Frequenzen oder Frequenzbändern und mit einer höheren Frequenzauflösung als der niedrige Audiosignalpegel und der hohe Audiosignalpegel gemessen wird;

(d) eine individuelle Verstärkungsfunktion berechnet wird, die in der Audiosignalverarbeitungseinheit zu implementieren ist, um die vordefinierte Ziellautheitsfunktion von Schritt (b) unter Berücksichtigung der wahrgenommenen Lautheitspegel, die in Schritt (c) gemessen wurden, zu erreichen;

(e) die Hörvorrichtung mit der individuellen Verstärkungsfunktion von Schritt (d) betrieben wird.

- 22.** Verfahren gemäß Anspruch 21, wobei der wahrgenommene Lautheitspegel in Schritt (c) für den mittleren Audiosignalpegel für mindestens 8 Frequenzen oder Frequenzbänder gemessen wird.
- 23.** Verfahren gemäß Anspruch 22, wobei der wahrgenommene Lautheitspegel im Schritt (c) für den mittleren Audiosignalpegel für mindestens 15 Frequenzen oder Frequenzbänder gemessen wird.
- 24.** Verfahren gemäß einem der Ansprüche 21 bis 23, wobei der wahrgenommene Lautheitspegel im Schritt (c) für den mittleren Audiosignalpegel bei mindestens 5 unterschiedlichen Frequenzen bzw. Frequenzbändern im Bereich von 0,75 bis 3 kHz gemessen wird.
- 25.** Verfahren gemäß einem der Ansprüche 21 bis 24, wobei der wahrgenommene Lautheitspegel im Schritt (c) für den niedrigen und/oder hohen Audiosignalpegel für 3 bis 5 Frequenzen oder Frequenzbänder gemessen wird.
- 26.** Verfahren gemäß Anspruch 24, wobei der wahrgenommene Lautheitspegel in Schritt (c) für jeden Lautheitspegel mit Ausnahme des mittleren Audiosignalpegels für 3 bis 5 Frequenzen oder Frequenzbänder gemessen wird.
- 27.** Verfahren gemäß einem der Ansprüche 21 bis 26, wobei der wahrgenommene Lautheitspegel im Schritt (c) für jeden Audiosignalpegel für Frequenzen oder Frequenzbänder im Bereich von 100 bis 10.000 Hz gemessen wird.
- 28.** Verfahren gemäß Anspruch 27, wobei der wahrgenommene Lautheitspegel im Schritt (c) für jeden Audiosignalpegel für Frequenzen oder Frequenzbänder gemessen wird, die in gleichem Abstand im Bereich von 100 bis 10.000 Hz angeordnet sind.
- 29.** Verfahren gemäß einem der Ansprüche 21 bis 28, wobei die Frequenzabhängigkeit der Werte der wahrgenommenen Audiosignalpegel gemäß Messung im Schritt (c) für den mittleren Audiosignalpegel verwendet wird, um zwischen den im Schritt (c) für den niedrigen Audiosignalpegel und den hohen Audiosignalpegel gemessenen Werten des wahrgenommenen Lautheitspegels zu interpolieren.
- 30.** Verfahren gemäß einem der Ansprüche 21 bis 29, wobei die Messungen von Schritt (c) für den mittleren Audiosignalpegel mit reinen Sinustönen durchgeführt werden.

31. Verfahren gemäß einem der Ansprüche 21 bis 30, wobei die Messungen von Schritt (c) für den niedrigen Audiosignalpegel und den hohen Audiosignalpegel mit schmalbandigem Rauschen durchgeführt werden. 5
32. Verfahren gemäß einem der Ansprüche 21 bis 31, wobei die im Schritt (c) für jede Frequenz oder jedes Frequenzband für den mittleren Audiosignalpegel gemessenen Werte des wahrgenommenen Lautheitspegels linear interpoliert werden. 10
33. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei die Ziellautheitsfunktion mindestens in einem Bereich von mittleren Eingangsschalldruckpegeln der Standardlautheitsfunktion einer normal hörenden Funktion entspricht. 15
34. Verfahren gemäß Anspruch 33, wobei für niedrige Eingangsschalldruckpegel die Ziellautheitsfunktion bezüglich der Standardlautheitsfunktion einer normal hörenden Person zu niedrigen Eingangsschalldruckpegeln hin progressiv verringert wird, 20
35. Verfahren gemäß einem der Ansprüche 33 bis 34, wobei die Ziellautheitsfunktion für hohe Eingangsschalldruckpegel hinsichtlich der Standardlautheitsfunktion einer normal hörenden Person zu hohen Eingangsschalldruckpegeln hin progressiv verringert wird. 25 30
36. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei das Wandlereingangsaudiosignal, welches in den Messungen von Schritt (c) verwendet wird, mittels der Audiosignalverarbeitungseinheit (26) erzeugt wird. 35
37. Verfahren gemäß einem der Ansprüche 1 bis 35, wobei das in den Messungen von Schritt (c) verwendete Wandlereingangsaudiosignal erzeugt wird, indem dem Mikrofon (20) entsprechender Schall zugeführt wird. 40
38. Verfahren gemäß einem der vorhergehenden Ansprüche, wobei es sich bei dem Ausgangswandler um einen elektromechanischen Ausgangswandler (32) zum direkten mechanischen Stimulieren des Mittelohrs oder Innenohrs handelt. 45
39. Verfahren gemäß Anspruch 38, wobei der elektromechanische Ausgangswandler (32) im Schritt (a) direkt mit dem Steigbügel, der Steigbügelplatte oder der Cochleawand verbunden wird. 50
40. Verfahren gemäß einem der Ansprüche 1 bis 36, wobei es sich bei dem Ausgangswandler um einen elektroakustischen Ausgangswandler handelt. 55

Revendications

1. Procédé pour adapter individuellement un instrument d'audition (10, 12) à un utilisateur, comprenant au moins un microphone (20) pour générer un signal audio d'entrée à partir d'un son ambiant, une unité de traitement de signal audio (26) pour traiter le signal audio d'entrée en un signal audio de sortie traité, et un transducteur pour la stimulation du système auditif humain en fonction du signal audio de sortie traité tel qu'il est entré sur ledit transducteur, le procédé comprenant :
 - (a) la fourniture à l'utilisateur de l'instrument d'audition et le démarrage du fonctionnement de l'instrument d'audition ;
 - (b) la prédéfinition d'une fonction de volume cible désirée, dans laquelle une perception de volume d'un stimulus par l'utilisateur lors de l'utilisation de l'instrument d'audition est définie en fonction d'une fréquence et d'un niveau de pression sonore d'entrée au niveau du microphone ;
 - (c) la mesure, pour un jeu de paramètres de mesure donné de niveaux de volume perçus et de fréquences ou de bandes de fréquence, du niveau de signal audio d'entrée de transducteur respectif devant être appliqué à l'entrée du transducteur afin d'obtenir le niveau de volume perçu respectif à la fréquence ou à la bande de fréquence respective, ledit jeu de paramètres de mesure comprenant au moins un niveau de faible volume, un niveau de volume intermédiaire et un niveau de fort volume, et ledit niveau de volume intermédiaire étant mesuré pour un plus grand nombre de fréquences ou de bandes de fréquence et avec une définition de fréquence plus fine que lesdits niveaux de volume faible et fort ;
 - (d) le calcul d'une fonction de gain individuelle destinée à être mise en oeuvre dans l'unité de traitement de signal audio de façon à obtenir la fonction de volume cible prédéfinie de l'étape (b) par le fait de tenir compte des niveaux de signal audio d'entrée de transducteur mesurés de l'étape (c) ;
 - (e) le fonctionnement de l'instrument d'audition avec la fonction de gain individuelle de l'étape (d).
2. Procédé selon la revendication 1, dans lequel, dans l'étape (c), le niveau de volume intermédiaire est le niveau le plus confortable, à savoir le niveau de pression sonore d'entrée auquel l'intelligibilité du stimulus pour l'utilisateur est la meilleure et auquel l'utilisateur pourra écouter confortablement pendant une période de temps prolongée.
3. Procédé selon la revendication 1 ou 2, dans lequel,

dans l'étape (c), le niveau de faible volume est le seuil d'audition, à savoir le niveau de pression sonore d'entrée auquel le stimulus devient décelable par l'utilisateur.

4. Procédé selon l'une des revendications précédentes, dans lequel, dans l'étape (c), le niveau de fort volume est le niveau inconfortable, à savoir le niveau de pression sonore d'entrée auquel le volume devient inconfortable pour l'utilisateur et la sensation ne pourrait pas être tolérée pendant une période de temps prolongée. 5
5. Procédé selon l'une des revendications précédentes, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré dans l'étape (c), pour le niveau de volume intermédiaire, pour au moins 8 fréquences ou bandes de fréquence. 10
6. Procédé selon la revendication 5, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré dans l'étape (c), pour le niveau de volume intermédiaire, pour au moins 15 fréquences ou bandes de fréquence. 20
7. Procédé selon l'une des revendications précédentes, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré dans l'étape (c), pour le niveau de volume intermédiaire, à au moins 5 fréquences ou bandes de fréquence différentes, respectivement, dans la plage de 0,75 à 3 kHz. 25
8. Procédé selon l'une des revendications précédentes, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré dans l'étape (c), pour le niveau de volume faible et/ou fort, pour 3 à 5 fréquences ou bandes de fréquence. 30
9. Procédé selon la revendication 8, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré, dans l'étape (c), pour chaque niveau de volume à l'exception dudit niveau de volume intermédiaire, pour 3 à 5 fréquences ou bandes de fréquence. 35
10. Procédé selon l'une des revendications précédentes, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré dans l'étape (c), pour chaque niveau de volume, pour des fréquences ou des bandes de fréquence dans une plage de 100 à 10.000 Hz. 40
11. Procédé selon la revendication 10, dans lequel le niveau de signal audio d'entrée de transducteur est mesuré dans l'étape (c), pour chaque niveau de volume, pour des fréquences ou des bandes de fréquence qui sont espacées de distances égales dans une plage de 100 à 10.000 Hz. 45

12. Procédé selon l'une des revendications précédentes, dans lequel la dépendance vis-à-vis de la fréquence des valeurs du niveau de signal audio d'entrée de transducteur tel qu'il est mesuré dans l'étape (c) pour le niveau de volume intermédiaire est utilisée pour effectuer une interpolation entre les valeurs du niveau de signal audio d'entrée de transducteur devant être appliqué à l'entrée du transducteur tel qu'il est mesuré dans l'étape (c) pour le niveau de faible volume et le niveau de fort volume. 50
13. Procédé selon l'une des revendications précédentes, dans lequel les mesures de l'étape (c) pour le niveau de volume intermédiaire sont effectuées sous la forme d'une mesure de contour de volume égal, dans laquelle, ensuite, pour chaque fréquence ou bande de fréquence, le niveau de signal audio d'entrée de transducteur est sélectionné de telle sorte que le même niveau de volume soit perçu par l'utilisateur. 55
14. Procédé selon l'une des revendications précédentes, dans lequel les mesures de l'étape (c) pour les niveaux de volume faible et fort sont effectuées sous la forme d'une série de mesures à fréquence constante, dans lesquelles, pour chaque fréquence ou bande de fréquence, le niveau de signal audio d'entrée de transducteur est sélectionné de telle sorte que d'abord le niveau de faible volume puis le niveau de fort volume, ou d'abord le niveau de fort volume puis le niveau de faible volume, soit perçu par l'utilisateur.
15. Procédé selon l'une des revendications précédentes, dans lequel les mesures de l'étape (c) pour le niveau de volume intermédiaire sont effectuées avec un bruit à bande étroite.
16. Procédé selon l'une des revendications précédentes, dans lequel les mesures de l'étape (c) pour les niveaux de volume faible et fort sont effectuées avec des tonalités sinusoïdales pures.
17. Procédé selon l'une des revendications précédentes, dans lequel les valeurs du signal audio d'entrée de transducteur mesuré dans l'étape (c) pour chaque fréquence ou bande de fréquence pour le niveau de volume intermédiaire sont interpolées de façon linéaire.
18. Procédé selon l'une des revendications précédentes, dans lequel, dans l'étape (c), ledit jeu de paramètres de mesure comprend uniquement lesdits niveaux de volume faible, intermédiaire et fort.
19. Procédé selon l'une des revendications précédentes, dans lequel la définition de fréquence des mesures dans l'étape (c) pour le niveau de volume in-

termédiaire correspond à la définition de fréquence de l'instrument d'audition.

- 20.** Procédé selon l'une des revendications précédentes, dans lequel :

dans l'étape (c), des niveaux de signal audio d'entrée de transducteur sont mesurés pour les niveaux de volume faible et fort sous la forme d'une mesure de contour de volume égal, dans laquelle, ensuite, pour chaque fréquence ou bande de fréquence, le niveau de signal audio d'entrée de transducteur est sélectionné de telle sorte que le même niveau de volume soit perçu par l'utilisateur ;

une fonction de gain individuelle préliminaire est calculée en tenant compte des niveaux de signal audio d'entrée de transducteur mesurés pour les niveaux de volume faible et fort, de façon à obtenir une fonction de volume cible prédéfinie, qui, au moins dans une plage de niveaux de pression sonore d'entrée moyenne, correspond à la fonction de volume standard d'une personne à audition normale ;

le contour de volume égal est estimé pour le niveau de volume intermédiaire à partir de la fonction de gain individuelle préliminaire ; et la fonction de gain individuelle est calculée par la correction de la fonction de gain individuelle préliminaire en tenant compte de la différence entre le contour de volume égal mesuré dans l'étape (c) pour le volume intermédiaire et du contour estimé de volume égal.

- 21.** Procédé pour adapter individuellement un instrument d'audition (10, 12) à un utilisateur, comprenant au moins un microphone (20) pour générer un signal audio d'entrée à partir d'un son ambiant, une unité de traitement de signal audio (26) pour traiter le signal audio d'entrée en un signal audio de sortie traité, et un transducteur pour la stimulation du système auditif humain en fonction du signal audio de sortie traité tel qu'il est entré sur ledit transducteur, le procédé comprenant :

(a) la fourniture à l'utilisateur de l'instrument d'audition et le démarrage du fonctionnement de l'instrument d'audition ;

(b) la prédéfinition d'une fonction de volume cible désirée, dans laquelle une perception de volume d'un stimulus par l'utilisateur lors de l'utilisation de l'instrument d'audition est définie en fonction d'une fréquence et d'un niveau de pression sonore d'entrée au niveau du microphone ;

(c) la mesure, pour un jeu de paramètres de mesure donné de niveaux du signal audio de sortie traité et de fréquences ou de bandes de fréquence, du niveau de volume perçu par l'utilisateur

à la fréquence ou à la bande de fréquence respective, ledit jeu de paramètres de mesure comprenant au moins un niveau de faible signal audio, un niveau de signal audio intermédiaire et un niveau de fort signal audio, et ledit niveau de signal audio intermédiaire étant mesuré pour un plus grand nombre de fréquences ou de bandes de fréquence et avec une définition de fréquence plus fine que lesdits niveaux de signal audio faible et fort ;

(d) le calcul d'une fonction de gain individuelle destinée à être mise en oeuvre dans l'unité de traitement de signal audio de façon à obtenir la fonction de volume cible prédéfinie de l'étape (b) par le fait de tenir compte des niveaux de volume perçus mesurés dans l'étape (c) ;

(e) le fonctionnement de l'instrument d'audition avec la fonction de gain individuelle de l'étape (d).

- 22.** Procédé selon la revendication 21, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour le niveau de signal audio intermédiaire, pour au moins 8 fréquences ou bandes de fréquence.

- 23.** Procédé selon la revendication 22, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour le niveau de signal audio intermédiaire, pour au moins 15 fréquences ou bandes de fréquence.

- 24.** Procédé selon l'une des revendications 21 à 23, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour le niveau de signal audio intermédiaire, à au moins 5 fréquences ou bandes de fréquence différentes, respectivement, dans la plage de 0,75 à 3 kHz.

- 25.** Procédé selon l'une des revendications 21 à 24, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour le niveau de signal audio faible et/ou fort, pour 3 à 5 fréquences ou bandes de fréquence.

- 26.** Procédé selon la revendication 24, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour chaque niveau de volume à l'exception dudit niveau de signal audio intermédiaire, pour 3 à 5 fréquences ou bandes de fréquence.

- 27.** Procédé selon l'une des revendications 21 à 26, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour chaque niveau de signal audio, pour des fréquences ou des bandes de fréquence dans une plage de 100 à 10.000 Hz.

- 28.** Procédé selon la revendication 27, dans lequel le niveau de volume perçu est mesuré dans l'étape (c), pour chaque niveau de signal audio, pour des fré-

quences ou des bandes de fréquence qui sont espacées de distances égales dans une plage de 100 à 10.000 Hz.

29. Procédé selon l'une des revendications 21 à 28, dans lequel la dépendance vis-à-vis de la fréquence des valeurs du niveau de signal audio perçu tel qu'il est mesuré dans l'étape (c) pour le niveau de signal audio intermédiaire est utilisée pour effectuer une interpolation entre les valeurs du niveau de volume perçu mesuré dans l'étape (c) pour le niveau de faible signal audio et le niveau de fort signal audio. 5
30. Procédé selon l'une des revendications 21 à 29, dans lequel les mesures de l'étape (c) pour le niveau de signal audio intermédiaire sont effectuées avec des tonalités sinusoïdales pures. 10
31. Procédé selon l'une des revendications 21 à 30, dans lequel les mesures de l'étape (c) pour les niveaux de signal audio faible et fort sont effectuées avec un bruit à bande étroite. 20
32. Procédé selon l'une des revendications 21 à 31, dans lequel les valeurs du niveau de volume perçu mesuré dans l'étape (c) pour chaque fréquence ou bande de fréquence pour le niveau de signal audio intermédiaire sont interpolées de façon linéaire. 25
33. Procédé selon l'une des revendications précédentes, dans lequel la fonction de volume cible, au moins dans une plage de niveaux de pression sonore d'entrée moyenne, correspond à la fonction de volume standard d'une personne à audition normale. 30
34. Procédé selon la revendication 33, dans lequel, pour de faibles niveaux de pression sonore d'entrée, la fonction de volume cible est progressivement réduite vers de faibles niveaux de pression sonore d'entrée par rapport à la fonction de volume standard d'une personne à audition normale. 35
35. Procédé selon l'une des revendications 33 et 34, dans lequel, pour de forts niveaux de pression sonore d'entrée, la fonction de volume cible est progressivement réduite vers de forts niveaux de pression sonore d'entrée par rapport à la fonction de volume standard d'une personne à audition normale. 40
36. Procédé selon l'une des revendications précédentes, dans lequel le signal audio d'entrée de transducteur utilisé dans les mesures de l'étape (c) est généré par l'unité de traitement de signal audio (26). 45
37. Procédé selon l'une des revendications 1 à 35, dans lequel le signal audio d'entrée de transducteur utilisé dans les mesures de l'étape (c) est généré par la délivrance d'un son correspondant au microphone 50

(20).

38. Procédé selon l'une des revendications précédentes, dans lequel le transducteur de sortie est un transducteur de sortie électromécanique (32) pour une stimulation mécanique directe de l'oreille moyenne ou de l'oreille interne.
39. Procédé selon la revendication 38, dans lequel le transducteur de sortie électromécanique (32) est directement relié, dans l'étape (a), à l'étrier, à la base de l'étrier ou à la paroi du limaçon osseux.
40. Procédé selon l'une des revendications 1 à 36, dans lequel le transducteur de sortie est un transducteur de sortie électroacoustique.

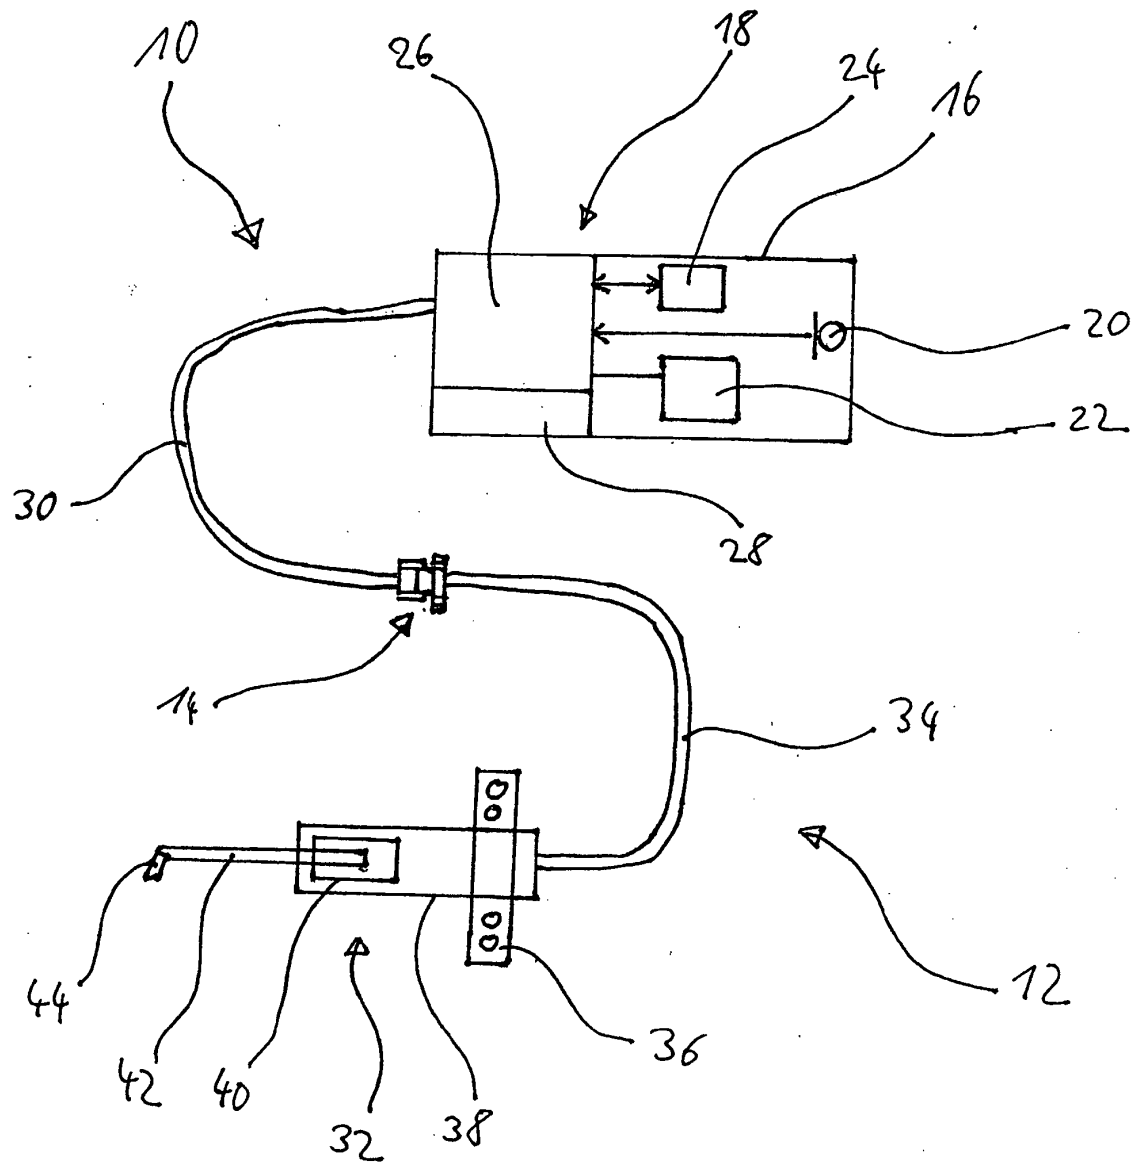


Fig. 1

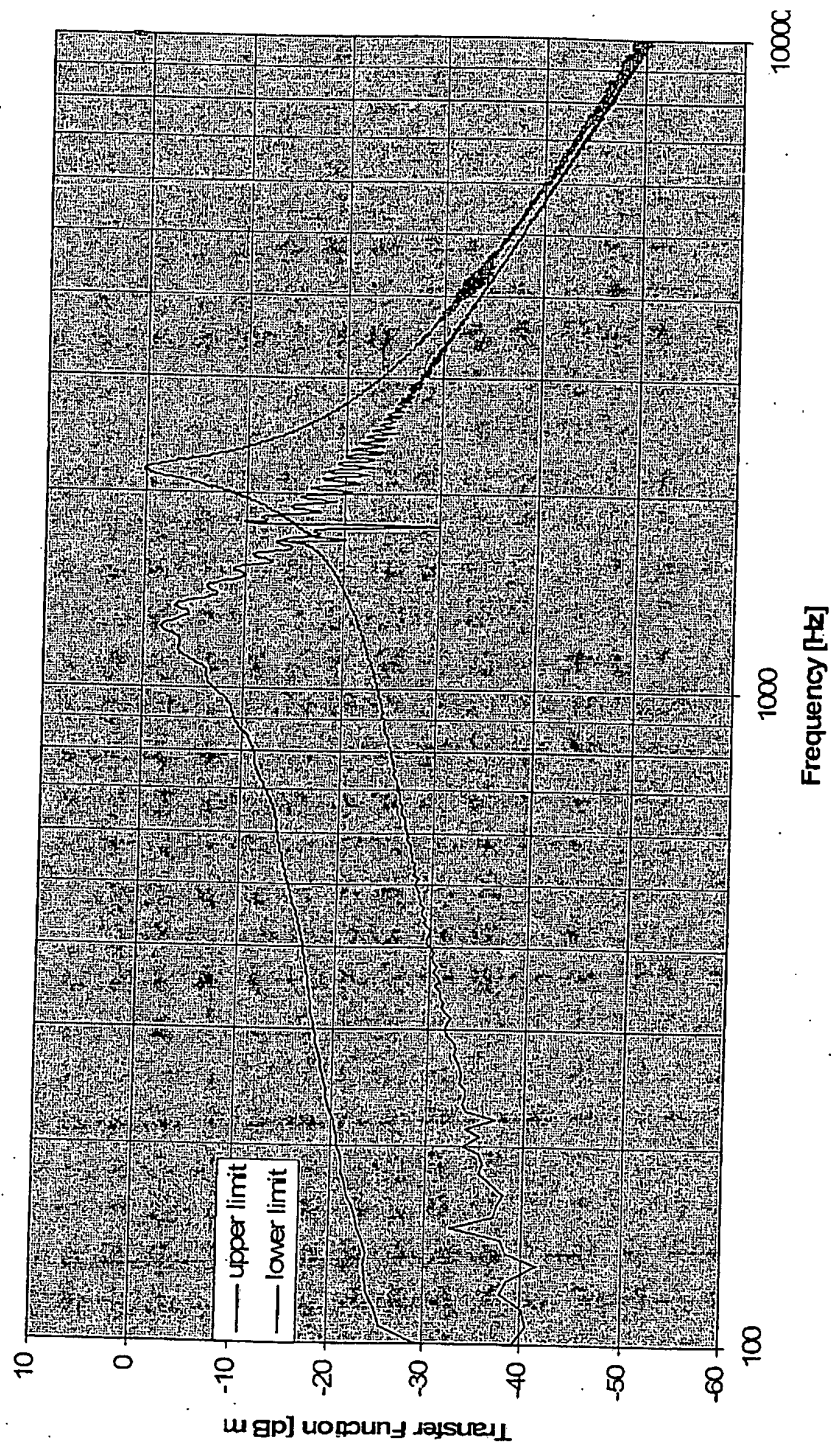


Fig. 2

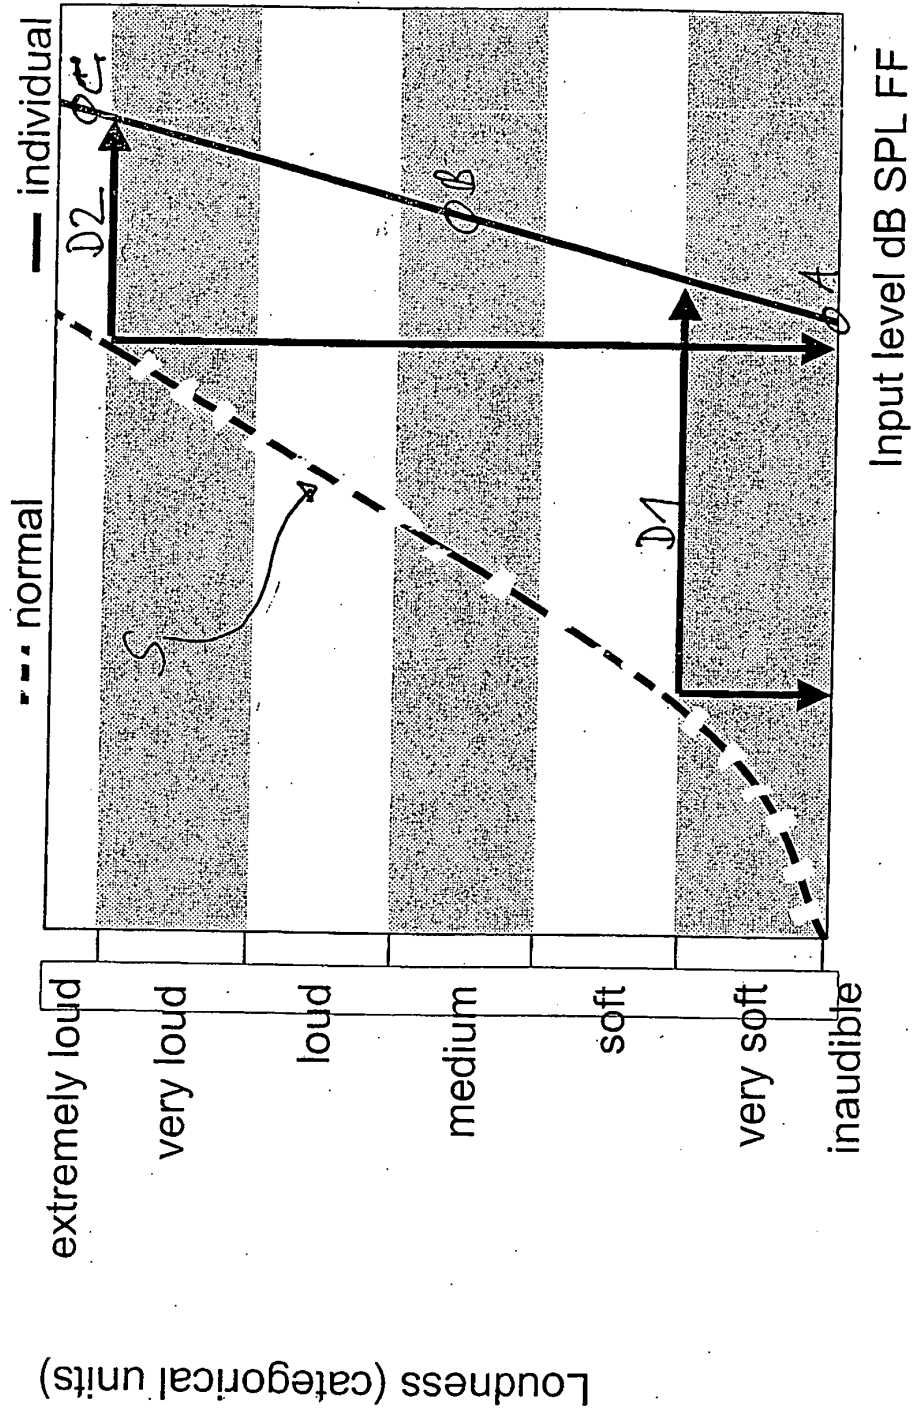


Fig. 3

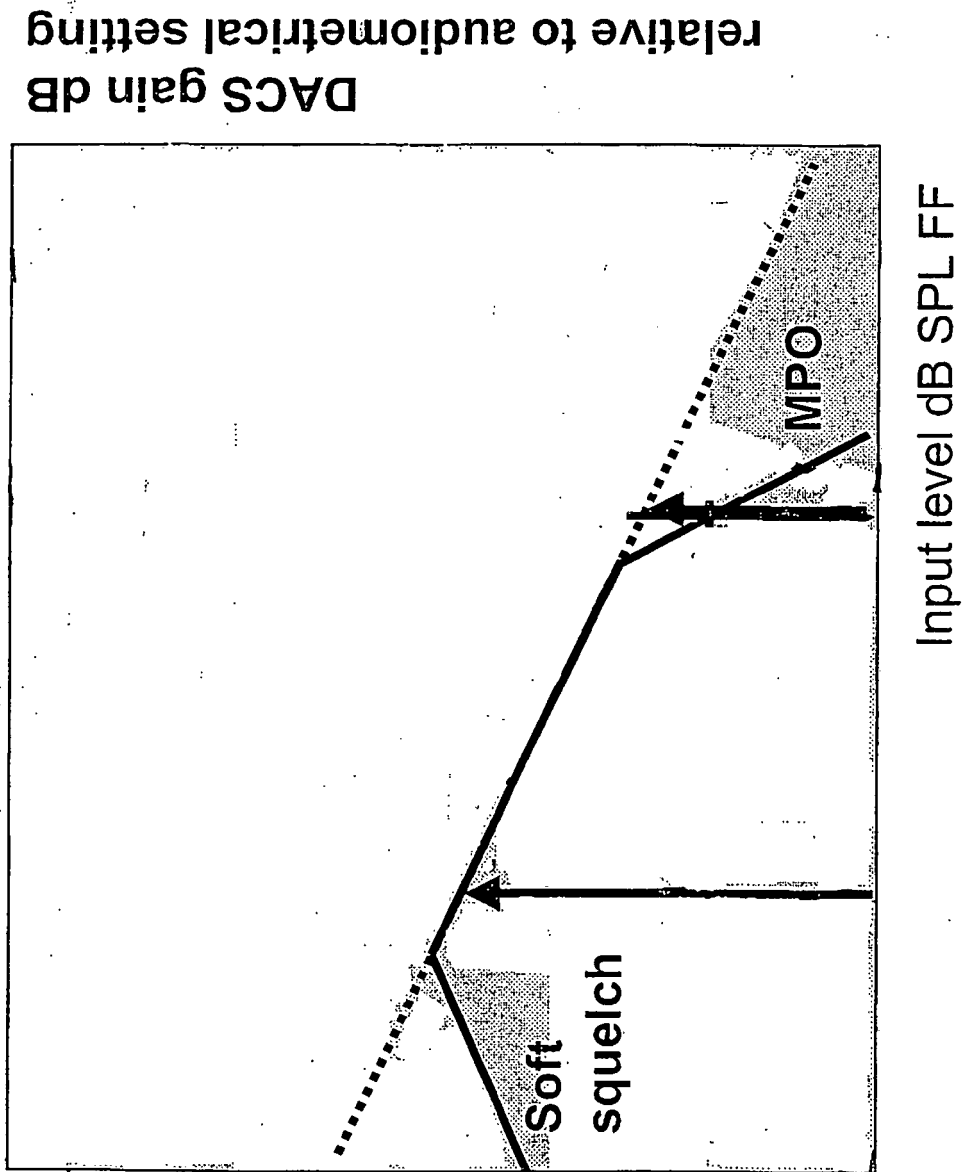


Fig. 4

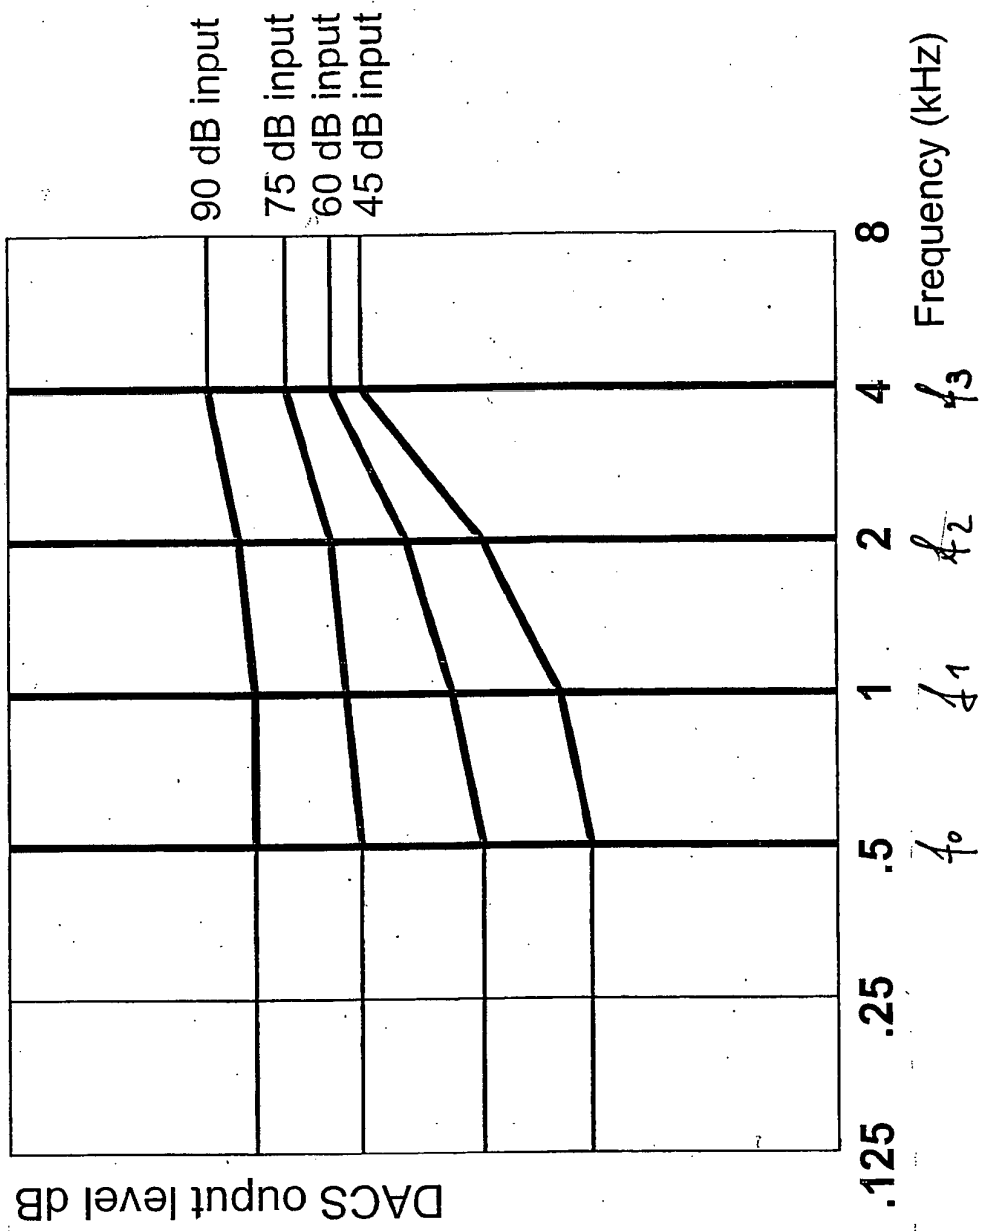


Fig. 5

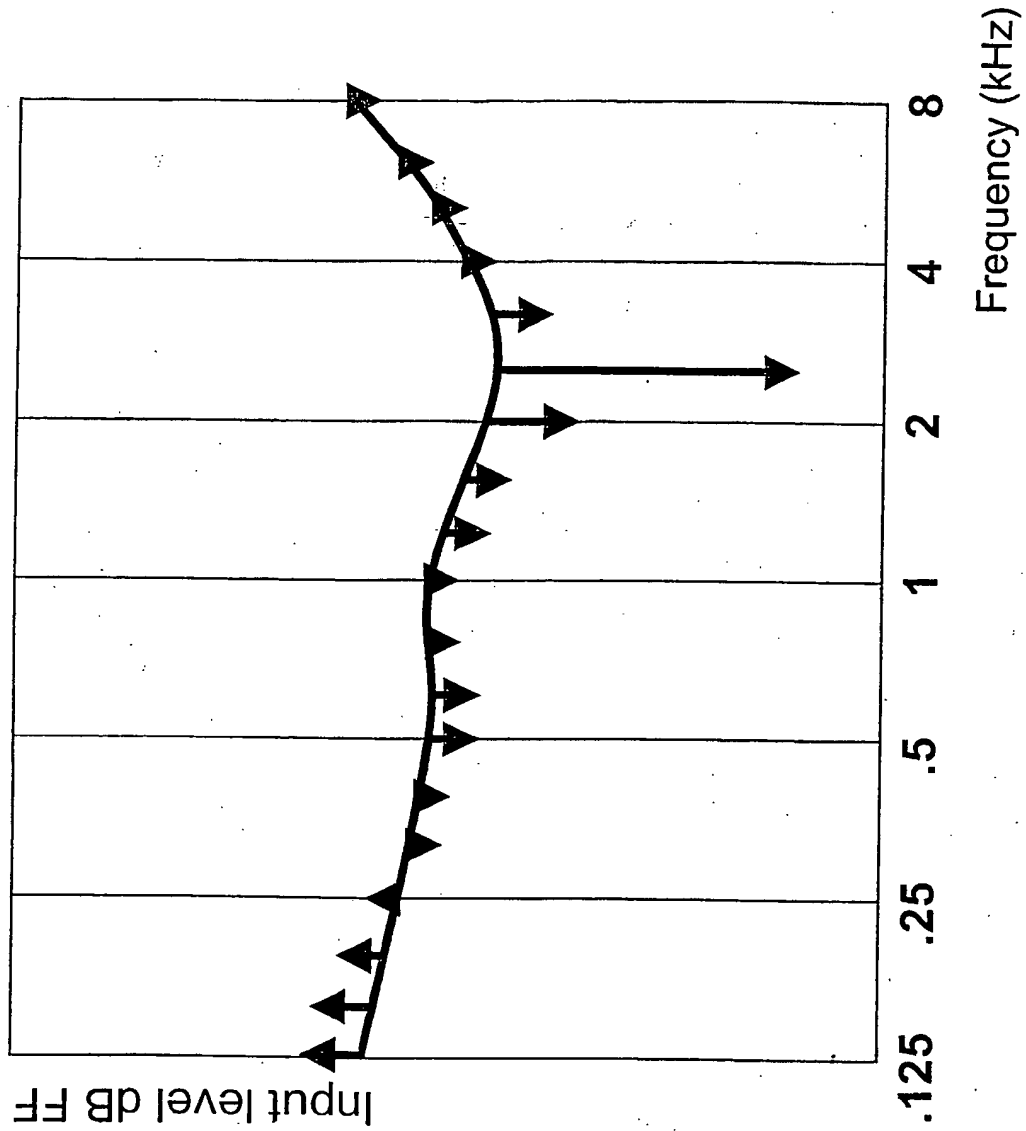


Fig. 6

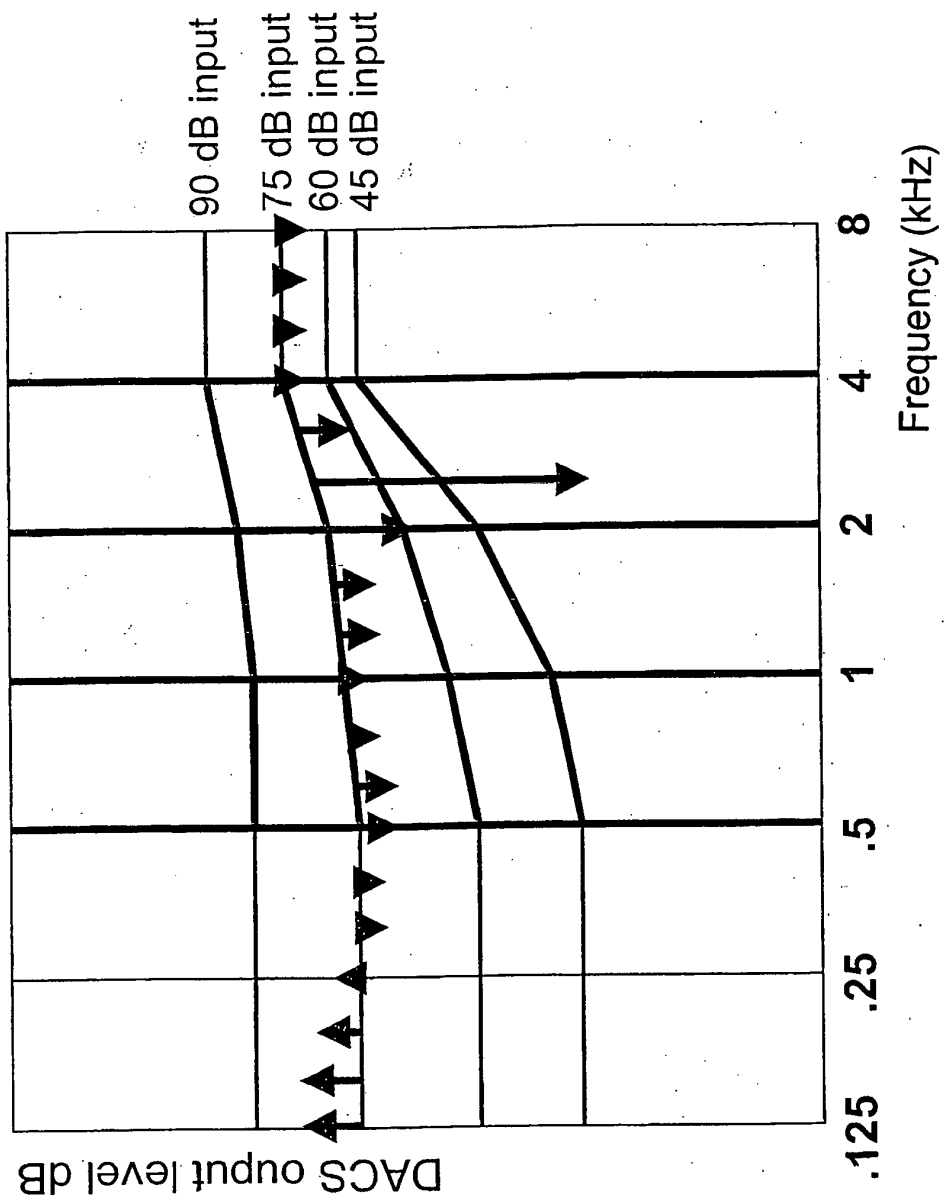


Fig. 7

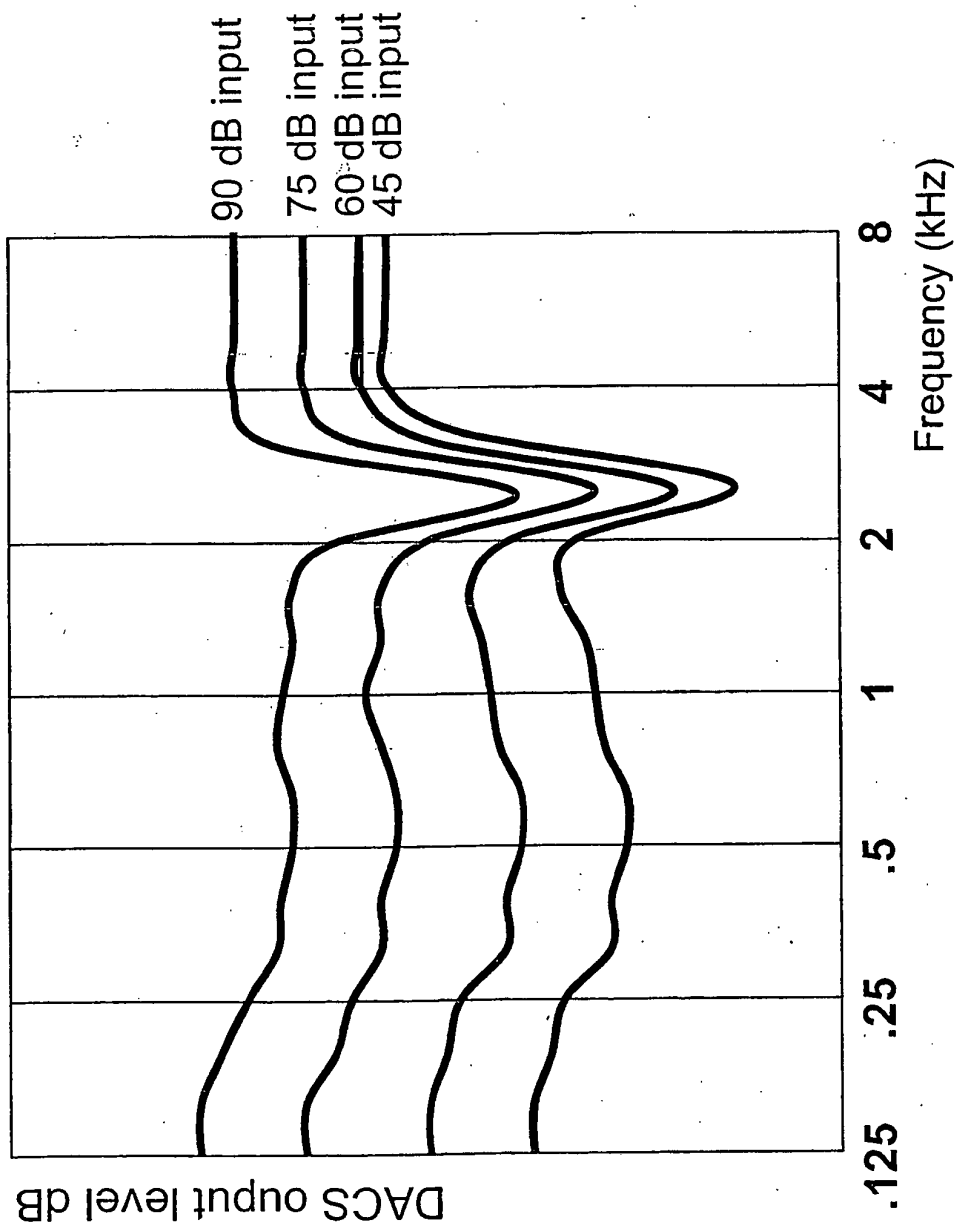


Fig. 8





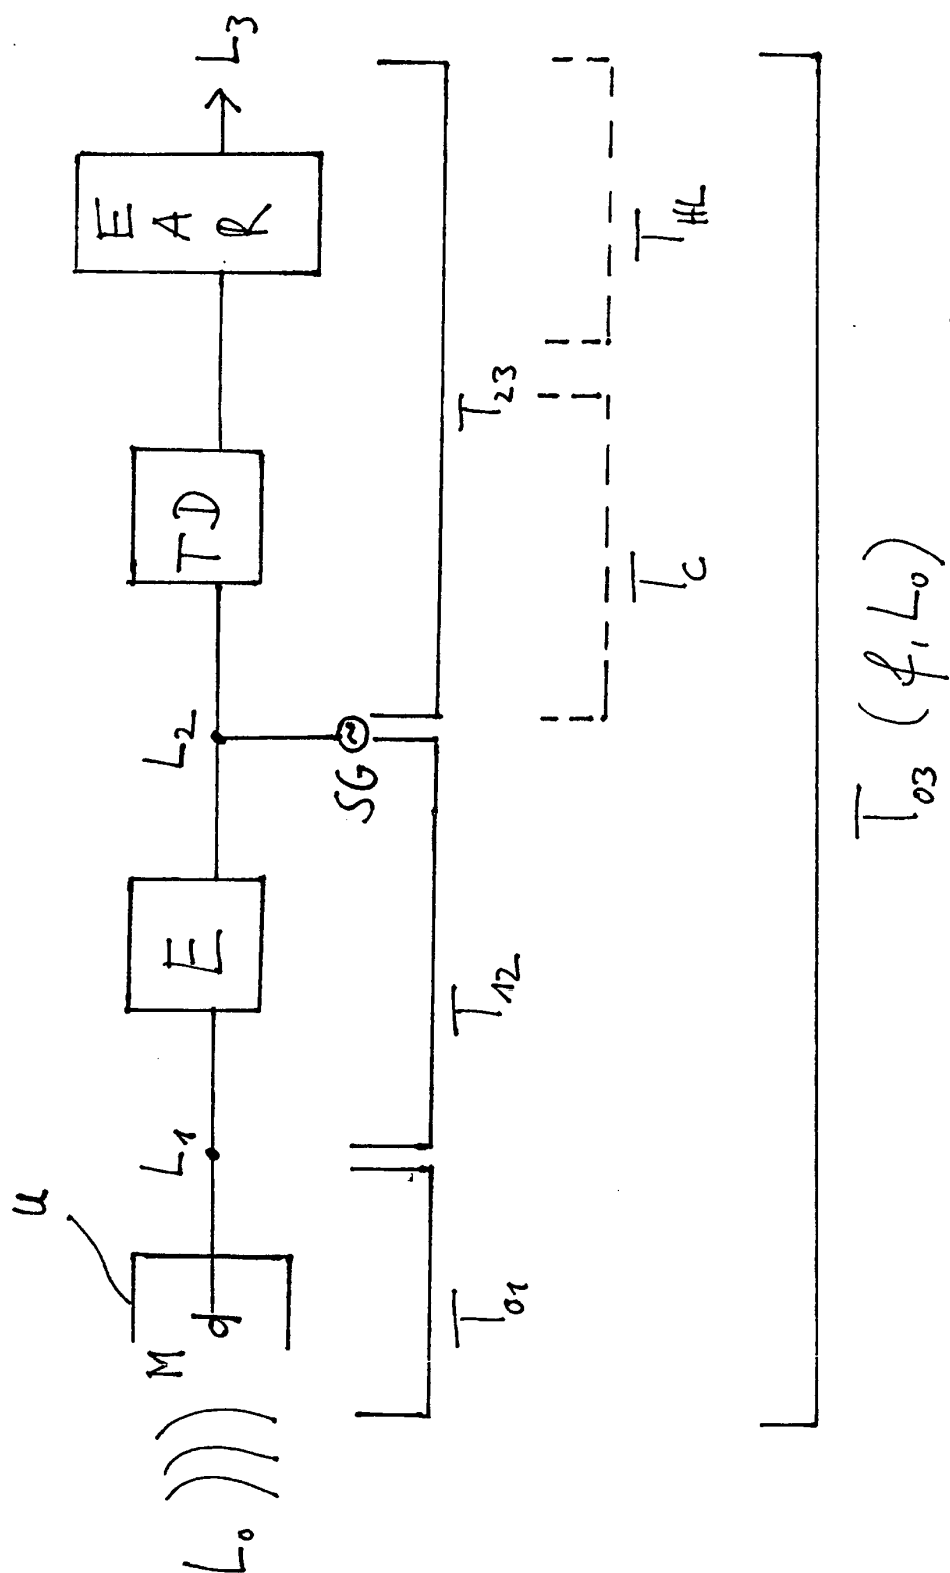


Fig. 9

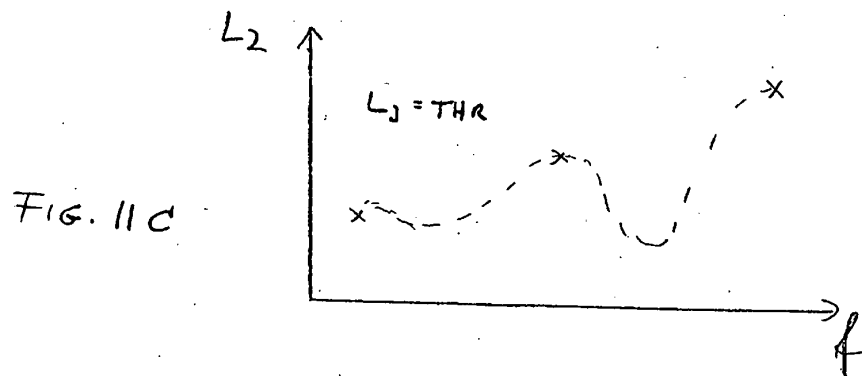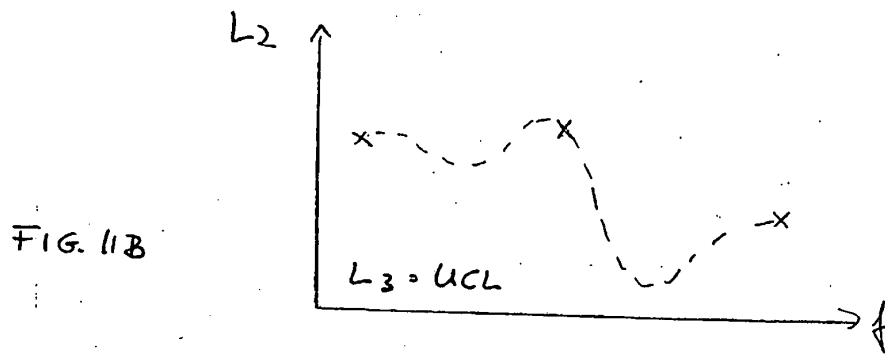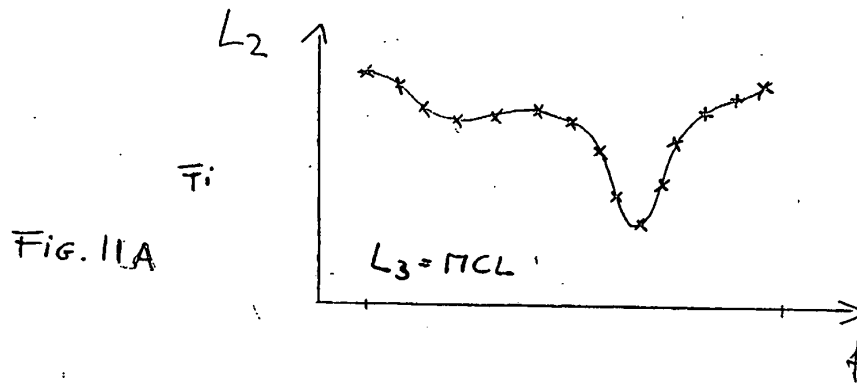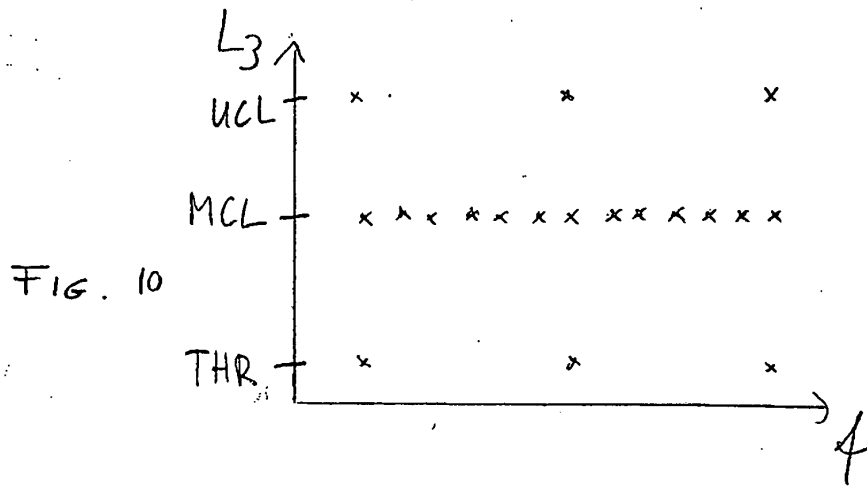

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 4577641 A [0004]
- DE 3205685 A1 [0005]
- DE 19914992 A1 [0006]
- EP 0535425 B1 [0007]
- DE 10041726 C1 [0008]
- EP 0661905 B1 [0009]
- US 6574342 B1 [0010] [0011]
- US 6201875 B1 [0010] [0011]
- WO 2004054318 A [0012]
- US 6315710 B1 [0044]
- US 6554762 B2 [0044]