

(51) International Patent Classification:
A61B 17/15 (2006.01) *A61B 17/17* (2006.01)(21) International Application Number:
PCT/GB2011/050780(22) International Filing Date:
20 April 2011 (20.04.2011)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
1006590.2 20 April 2010 (20.04.2010) GB(71) Applicant (for all designated States except US):
BIOMET LTD. [GB/GB]; Waterton Industrial Estate,
Bridgend, Mid Glamorgan CF31 3XA (GB).

(72) Inventors; and


(71) Applicants : **GOODFELLOW, John** [GB/GB]; 4 Up-
land Park Road, Summertown, Oxford, Oxfordshire
OX27 RU (GB). **O'CONNOR, John** [GB/GB]; Quarry
Mannor, 9 Beaumont Road, Headlington, Oxford, Ox-
fordshire OX27 JN (GB). **DODD, Chris** [GB/GB]; 1
Tackley Place, Oxford, Oxfordshire OX26 6RR (GB).
MURRAY, David [GB/GB]; Cuddeson House, Wheatley
Road, Oxford, Oxfordshire OX44 9HB (GB).(74) Agent: **BARKER BRETTELL LLP**; 100 Hagley Road,
Edgbaston, Birmingham, West Midlands B16 8QQ (GB).(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ,
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,
NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD,
SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR,
TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG,
ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ,
TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK,
EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU,
LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,
SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ,
GW, ML, MR, NE, SN, TD, TG).

Published:

— without international search report and to be republished
upon receipt of that report (Rule 48.2(g))

(54) Title: UNICONDYLAR KNEE REPLACEMENT

Fig. 1

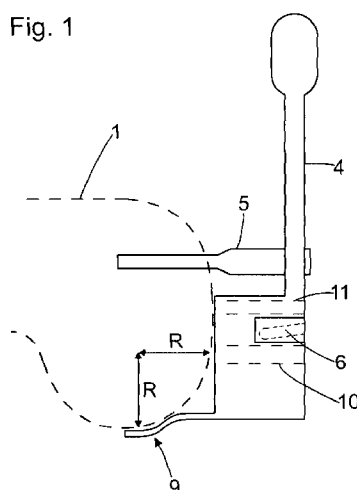(57) Abstract: A kit of parts for use in unicondylar knee replacement of a patient having a femur and a tibia comprises a drill
guide (4) and an intramedullary rod (5), the intramedullary rod being sized to fit within the intramedullary canal of the femur of
the patient. The drill guide is arranged so as to engage a distal end of the intramedullary rod to that which engages the patient's in-
tramedullary canal, and is formed with a foot portion (9) sized to fit between the patient's femur and tibia before any bone is re-
moved from the femur or tibia. The drill guide provides a guide for drilling of at least one hole in the femur. A further kit of parts
for use in unicondylar knee replacement of a patient having a femur and a tibia comprises a femoral component (3) for implanta-
tion in the femur, the femoral component having a bearing surface having a radius of curvature, and a guide spoon (13). The guide
spoon has a bowl-shaped portion (14) with an internal radius of curvature the same as that of the bearing surface, and a handle
portion (16) extending from the bowl- shaped portion. Methods of performing unicondylar knee replacement are also described.

UNICONDYLAR KNEE REPLACEMENT

FIELD OF THE INVENTION

- 5 The present invention relates to kits of parts for, and methods of, performing unicondylar knee replacement.

BACKGROUND OF THE INVENTION

- 10 The knee comprises three inter-dependent joints in three separate compartments, all surrounded by a fibrous capsule covered by the skin. The medial tibio-femoral joint involves contact between the thigh bone (the femur) and the leg bone (the tibia) on the inside of the lower limb. The lateral tibio-femoral joint involves contact between the femur and the
15 tibia on the outside of the lower limb. The patello-femoral joint involves contact between the femur and the knee cap (the patella) on the front of the lower limb.

- The front of the lower (distal) end of the femur comprises a flanged
20 concave groove providing a track for the patella. The back of the distal femur divides into two separate near-spherical concave condyles making contact with the tibia. The upper surface of the tibia is like a plateau which is slightly dished on the medial side for contact with the medial femoral condyle forming the medial tibio-femoral joint and slightly
25 convex on the lateral side for contact with the lateral femoral condyle forming the lateral tibio-femoral joint with a protrusion (the tibial eminence) running from front to back between the joints.

- The articulating surfaces in each joint are covered with thin layers of a
30 tough protective layer called cartilage, and are lubricated by synovial fluid secreted from a membrane on the inner surface of the fibrous

capsule surrounding the knee. The surfaces of the tibio-femoral joints are further separated by the menisci, semi-circular semi-lunar collagen bundles oriented circumferentially. Each bundle is securely attached at each end to the tibia. The menisci form closely-fitting sockets for the femoral condyles bringing the dissimilar surfaces of the femur and tibia into closer conformity.

The bones are held together actively by muscles with their tendons which span the joints and passively by ligaments and the joint capsule. The ligaments comprise bundles of collagen fibres running mainly longitudinally. The collateral ligaments arise on the external surfaces of the medial and lateral condyles. The medial collateral ligament inserts into the external medial surface of the proximal tibia. The lateral collateral ligament inserts into the proximal surface of the fibula. The medial collateral ligament is a much larger and stiffer structure than the lateral collateral ligament. The cruciate ligaments arise from the internal surfaces of the femoral condyles and insert into the tibial eminence.

The ligaments and the bones together form a mechanism which controls a complex pattern of movement of the bones on each other. In the unloaded state, flexion of the knee to 130° about a transverse axis is accompanied by approximately 25° rotation about the axis of the tibia (axial rotation) and approximately 5° about an anteroposterior axis (abduction-adduction). These movements are accommodated by mainly antero-posterior translations of the tibio-femoral contact areas so that the bones roll as well as slide on each other and the patella slides over the anterior femur.

Under load, the ligaments stretch and the articular surfaces indent, significantly modifying the relationship between flexion, axial rotation and abduction-adduction and between flexion and contact area

translations. Movements at the knee are therefore load and activity dependent.

Damage to the articular surfaces or to the ligaments changes the patterns
5 of movement of the bones on each other and response of the joint to load. Osteoarthritis follows from failure of the cartilage in one or other of the three joints, leading to bone-on-bone contact and the onset of pain. Frequently, osteoarthritis first manifests itself in the medial compartment, while the ligaments remain intact. The disease can remain confined to the
10 medial compartment until the anterior cruciate ligament fails and the disease then spreads to the other two compartments. No drug treatment has been found which reverses these processes.

Total knee replacement is the most common surgical treatment for
15 osteoarthritis, involving replacement of the articular surfaces of all three compartments and sacrifice of some of the ligaments. Partial knee replacement involves replacement of the articular surfaces in only one compartment, leaving intact the surfaces of the other two compartments and all of the ligaments. Partial knee replacement can act
20 prophylactically, reducing the rate of development of the disease in the other compartments. Partial knee replacement is surgically more demanding and is not always used when it is indicated.

To implant the prosthetic components of a knee replacement, sufficient
25 sections of bone first have to be removed from the surfaces of the tibia and the femur. The tibial surface is sawn first, using a saw guide that is applied with its shaft parallel to the long axis of the tibia and its upper end nailed to the exposed bone. The level of the guide is estimated, usually conservatively so that more bone can be resected if required.

Once the initial resection of the tibia has taken place, the femur is prepared for the implantation of the femoral component of the knee replacement. Holes are drilled for insertion of the femoral saw block, the spigots for milling and the trial femoral component. The positions and angles of these holes are referenced by inspection off features of the femur, and the position of the resected tibial plateau is checked and revised if necessary. Once the initial cutting, milling and trimming of the femur has taken place, a trial femoral component and a tibial template are inserted. The new gap between the femoral and tibial components is measured at the extremes of knee flexion, and the femur is further milled to equalise these flexion gaps. Final trimmings of the femur and tibia take place before the appropriate bearing is fitted and the final components are cemented in place.

BRIEF SUMMARY OF THE INVENTION

According to a first aspect of the invention, there is provided a kit of parts for use in unicondylar knee replacement of a patient having a femur and a tibia, comprising a drill guide and an intramedullary rod, the intramedullary rod being sized to fit within the intramedullary canal of the femur of the patient, the drill guide being arranged so as to engage a distal end of the intramedullary rod to that which engages the patient's intramedullary canal, the drill guide being formed with a foot portion sized to fit between the patient's femur and tibia before any bone is removed from the femur or tibia, the drill guide providing a guide for drilling of at least one hole in the femur.

Thus, the drill guide has two points of reference on the patient's femur; firstly, the intramedullary rod, and, secondly, the foot portion being fitted between the unresected tibia and femur. Thus, the drill guide can

be held securely and accurately in place, to ensure accurate and consistent drilling.

In order to fit between the unresected tibial and femoral components, the
5 foot portion may have a maximum thickness of 2 mm.

Typically, the guide will comprise at least one hole, through which a drill bit can be passed in order to drill the or each hole in the femur. Typically, there will be a main hole, such as may be used to drill a hole
10 for a main peg on the femoral component to be implanted. The distance between the centre of the main hole and the foot portion may be equal to a radius of the femoral condyle. The distance between the centre of the main hole and the foot portion may also be equal to a radius of the femoral component.

15

The guide may comprise a further hole for drilling a further hole in the femur; the distance between the main hole and the further hole in the drill guide may be equal to a distance between the main peg and a further peg in the femoral component to be implanted. The distance between the
20 main hole and the further hole in the drill guide may also be equal to a distance between two holes in a saw guide used in a resection of the femur.

The drill guide may connect to the intramedullary rod by means of a
25 linkage. The linkage may comprise at least one rod which engages the end of the intramedullary rod. The linkage may also comprise at least one rod which engages at least one hole in the drill guide. The holes in the drill guide may be positioned such that, for a left knee the linkage engages a first hole and not a second hole, and for a right knee the
30 linkage engages a second hole and not the first hole. Thus, the same apparatus can be used for right or left knees.

The kit of parts may further comprise at least one femoral component. At least one femoral component may be a trial femoral component which is temporarily implanted in the femur. At least one femoral component may
5 be a prosthetic femoral component which is permanently implanted in the femur. At least one prosthetic femoral component may have a radius equal to that of at least one trial femoral component.

According to a second aspect of the invention, there is provided a kit of
10 parts for use in unicondylar knee replacement of a patient having a femur and a tibia, comprising a femoral component for implantation in the femur, the femoral component having a bearing surface having a radius of curvature, and a guide spoon, the guide spoon having a bowl-shaped
15 portion with an internal radius of curvature the same as that of the bearing surface, and a handle portion extending from the bowl-shaped portion.

This spoon guide can therefore provide an accurate reference point for further resection of the patient's knee, typically the tibia. Typically, the
20 femoral component will be a trial femoral component, which is only temporarily implanted in the femur.

The bowl-shaped portion will typically have a rim; the rim and the handle portion may be co-planar in a common plane. The kit of parts may
25 further comprise a clamp and a horizontal saw guide, the clamp being arranged to clamp to the hand portion and to space the saw guide from the handle portion by a pre-determined distance, typically in the direction perpendicular to the common plane. Thus, the "horizontal" cut in the tibia can be correctly placed.

The kit of parts may further comprise a vertical saw guide, which comprises a first arm which engages a hole in the femoral component, the hole being keyed such that the first arm will not rotate in the hole, and a second arm which extends at an angle from the mechanical axis of the femur. Typically, the angle will be approximately 7 degrees, such that the second arm runs parallel to the diaphyseal femoral axis.

The hole may have rotational symmetry (typically of even order) such that the first arm can be placed in at least two positions therein to work with left and right knees. Typically, the hole will be square or rectangular in cross section.

In order to enable the correct cut to be made by placing a saw against the vertical saw guide and the rim of the spoon, the rim of the spoon may be circular with a radius sized so that, when a wall of the tibial component is installed in the cut that is to be made, there is a gap of predetermined size – typically approximately 1 mm – between the wall and a bearing, typically a meniscal bearing, to be inserted between the tibial and femoral components. Typically, the radius will be the sum of half the width of the bearing, the width of the wall and the distance between the bearing and the wall, less the width of the saw blade to be used. The kit of parts may further comprise at least one of the tibial component and the saw blade.

The first and second arms of the vertical saw guide may be offset by the radius of the rim also.

The kit of parts may further comprise a U-shaped channel for connecting to the second arm of the vertical saw guide and arranged to constrain a saw blade placed therein to cut parallel to the second arm.

The dimensions of the vertical saw guide may be made so that the slot mechanism points both at the correct angle and in the correct position for the cut. The length x of the crank portion may be calculated as:

5
$$x = r/\cos\theta - y\tan\theta$$

where

θ is the angle at which the guide portion is axially bent away from the axis of the first end,

10 y is the radial distance of the crank portion away from the centre of the spoon, and

r is the radius of the rim of the spoon

According to a third aspect of the invention, there is provided a method
15 of performing unicondylar knee replacement of knee of a patient, comprising using the kit of parts of the first aspect of the invention by placing the intramedullary rod in the intramedullary canal of the femur of the knee, connecting the drill guide to the intramedullary rod, placing the foot portion between the femur and the tibia of the knee, aligning the drill
20 guide laterally to the central prominence of the femoral condyle and then drilling a hole in the femur guided by the guide.

Thus, the drill guide has two points of reference on the patient's femur; firstly, the intramedullary rod, and, secondly, the central prominence of
25 the femoral condyle. This ensures accurate and consistent drilling. A rotational degree of freedom may allow the foot portion to move around the spherical surface of the condylar cartilage. Typically, it will be the main hole of the drill guide that is aligned laterally with the central prominence of the femoral condyle.

The method may comprise drilling a first hole in the femur by passing a drill bit through the main hole and then drilling with the bit. The method may comprise leaving the drill bit in place after the first hole has been drilled, and then rotating the drill guide about the main hole (typically
5 having disconnected the drill guide from the intramedullary rod after the first hole has been drilled) to correctly position the further hole, then drilling a second hole in the femur through the further hole in the drill guide.

10 The method may comprise the implantation of a femoral component, typically a trial femoral component that is only implanted temporarily. Typically, once the first hole and any second hole have been drilled, the femoral condyle to be replaced can be milled and cut, typically using prior art techniques, and the femoral component implanted using the first
15 and/or second holes as positional guides.

According to a fourth aspect of the invention, there is provided a method of performing unicondylar knee replacement of a knee of a patient using the kit of parts of the second aspect of the invention, comprising
20 implanting the femoral component in the femur of the knee, inserting the spoon with its bowl against the bearing surface.

This spoon guide can therefore provide an accurate reference point for further resection of the patient's knee, typically the tibia. The femoral
25 component may be a trial femoral component that is only implanted temporarily.

The method may further comprise the step of clamping the clamp and the horizontal saw guide to the handle portion; typically this will space the
30 saw guide from the handle portion by a pre-determined distance, typically in the direction perpendicular to the common plane. The method may

then comprise cutting the tibia along a plane indicated by the horizontal saw guide. Thus, the “horizontal” cut in the tibia can be correctly placed.

5 The method may further comprise the step of inserting the vertical saw guide into the femoral component, then sawing into the tibia guided by the vertical saw guide. Thus, the “vertical” cut can be achieved. Typically, the vertical cut will be extended to meet the horizontal cut.

10 According to a fifth aspect of the invention, there is provided a method of performing unicondylar knee replacement of a patient, comprising implanting a femoral component in the femur of a knee of the patient before a tibial component is implanted in the tibia of the knee. In the preferred embodiment, the femoral component once implanted is used to
15 determine the correct position for resectioning of the tibia in advance of the implantation of the tibial component.

The femoral component may be a trial femoral component that is only implanted temporarily.

20

Typically, the method will comprise the steps of a method according to the third aspect of the invention, followed by a method according to the fourth aspect of the invention.

25 **BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWINGS**

There now follows, by way of example only, an embodiment of the invention, described with reference to, and as illustrated in, the
30 accompanying drawings, in which:

Figure 1 shows a side elevation of a kit of parts according to a first embodiment of the invention being used to implant a femoral component;

5 **Figure 2** shows a further side elevation of the drill guide of the kit of parts of Figure 1;

Figure 3 shows an underside plan view of the drill guide of Figure 2;

10

Figure 4 shows the linkage used to connect the intramedullary rod and drill guide of the kit of parts of Figure 1;

15 **Figure 5** shows further elements of the kit of parts of Figure 1, used to implant a tibial component;

Figure 6 shows a plan view of a spoon being part of the kit of parts of Figure 5;

20 **Figure 7** shows a “horizontal” cut being made in the tibia, using the kit of parts of Figure 5;

Figure 8 shows a side elevation of the vertical saw guide of the kit of parts of Figure 5 fitted to the femoral component;

25

Figure 9 shows a plan view of the vertical saw guide of Figure 8 being used to make a “vertical” cut in the tibia;

30 **Figure 10** shows an optional saw guide that can be used with the vertical saw guide of Figure 8;

Figure 11 shows the horizontal positioning of the meniscal bearing in relation to the tibial component; and

Figure 12 shows the dimensions of the vertical saw guide.

5

DETAILED DESCRIPTION OF THE INVENTION

Figures 1 to 4 show a kit of parts according to a first embodiment of the invention being used to effect the initial stages of a unicondylar knee replacement. In this first stage, a femoral component 3 (Figure 5) is to be fitted into the femur 1 of a patient, and so the femur must be resected to allow for the implantation.

In order to do so, a drill guide 4 is used to determine the position of the two holes that are required in the femur to support the locating peg or pegs of the femoral component 1. This is used in conjunction with an intramedullary rod 5, which is inserted into the intramedullary canal of the femur 1 in order to provide a fixed location. A narrow foot portion 9, having a thickness of about 2 mm is provided at a lower end of the drill guide 4; the foot portion 9 can fit between the patient's femur and tibia before any resection takes place.

In order to provide the location of the first hole to be drilled, two holes 6 are provided in the drill guide to accept one of two rods 8 comprised in a linkage 7. The holes 6 extend into the drill guide at an angle of 10 degrees to the horizontal towards the foot portion 9 and at an angle of 7 degrees horizontally towards either side of a vertical drill hole 10, which will be discussed in more detail below. Only one hole 6 will be used for a given knee, as the combination allows the use of this kit of parts for both left and right knees. The intramedullary rod 5 is adapted to accept the other one of the two rods 8 which is not inserted into a hole 6, thus

linking the drill guide with the intramedullary rod and maintaining a predefined spacing and alignment between them. Linking the drill guide to the intramedullary rod in this way ensures that the drill hole is directed at an angle of 10 degrees to the horizontal away from the foot portion 9 and at an angle of 7
5 degrees horizontally, parallel to the horizontal component of the diaphyseal femoral axis.

The drill hole 10 provides the surgeon with a guide as to where to drill the main drill hole for the main peg of the femoral component. The
10 distance between the drill hole 10 and the foot portion 9 is the same as the radius of curvature R of the femoral component 1.

A further drill hole 11 is provided, which will provide the surgeon with the location for a further, smaller, peg hole as described below.

15

Once the drill guide 4 and the intramedullary rod 5 are linked, the position of the drill guide 4 is adjusted so that the drill hole 10 is aligned with the centre of the correct condyle. A drill is then used to drill the main peg hole. The drill bit is left in place in the hole, whilst the
20 linkage 7 is removed. The drill guide 4 is then rotated about the drill hole 10, until the further drill hole 11 is aligned centrally along the prominence of the femoral condyle, below the first hole, thus ensuring that the distance between the two holes is correct. The smaller hole can then be drilled through the further drill hole 11. Once that is done, the
25 drill guide 4 and drills are removed, and the primary milling and cutting of the condyle 1a carried out using existing methods. The trial, temporary, femoral component 3 is then inserted.

As will be explained below, now that the trial femoral component 3 has
30 been implanted, this can be used to provide a reference for the correct position in which the cuts to the patient's tibia should be made. This

makes for an overall more accurate set of cuts, and may reduce the need for repeated cuts and corrections mid-surgery.

In the next stage, shown in Figures 5 to 7 of the accompanying drawings, the first, horizontal cut is made to the patient's tibia 12. A guide spoon 13 is used, which has a bowl portion 14 having an inner radius of curvature the same as the radius of curvature R of the femoral component 3. The bowl portion 14 has a rim 15 and a handle portion 16 extending from and co-planar with the rim 15. It has a thickness of 1 mm.

The guide spoon 13 is inserted with the bowl portion 14 under the trial femoral component 3 and clamped using the handle portion and a clamp 17 to a horizontal saw guide 18, which guides the surgeon to the correct location for the horizontal cut. The clamp ensures that the spoon handle 16 is parallel to the horizontal saw guide 18 and that the cut 19 is the desired distance – 7.5 mm – below the femoral component, allowing for the thickness of the platform of the tibial template and the meniscal bearing insert (3.5 mm and 4.5 mm respectively).

20

Once the horizontal cut is made, the procedure can proceed to the situation shown in Figures 8 to 10 of the accompanying drawings. A vertical saw guide 20 is used, which comprises a generally elongate body of square cross section, a first end 22 of which is received in a square hole 21 in the femoral component 3. Being square, the vertical saw guide 20 can be received in the hole 21 in two orientations to allow for left or right knees to be operated upon (of course, there will be two further orientations in which such insertion is possible, but these are not in practice used).

30

The hole 21 in the femoral component is vertically in line with the peg of the trial femoral component. The axis of this peg is parallel with the plane of the flat portion of the component (i.e. horizontal) so the axis of the hole is on the same line as that of the peg. The hole will be central in the femoral component 3, given that it will be used in both left and right knees.

The vertical saw guide 20 then comprises a crank portion 23 connected to a guide portion 24 at the end distal from the first end 22. The crank portion 23 axially separates the first end 22 from the guide portion 24. The guide portion is also axially bent away from the axis of the first end and of the mechanical axis of the femur by an angle θ of 7 horizontal degrees, so as to be aligned with the diaphyseal femoral axis.

The saw for the vertical tibial cut 25 is positioned parallel to the guide portion 24 and against the rim 15 of the spoon 13. As shown in Figure 11, the dimensions of the rim 15 ensure that, when the wall 27 of the tibial component 28 is flush against the vertical tibial cut 25, there is a 1 mm gap 29 between the wall 27 and the bearing 30.

20

Accordingly, the rim 15 of the spoon 13 is circular with a radius equal to: $\frac{1}{2}(\text{bearing insert width}) + \text{width of wall} + \text{distance between bearing and wall} - \text{width of saw blade}$. Apart from the bearing insert width, these values are respectively 1.5 mm, 1 mm and 1 mm. The crank portion 23 is also of this length.

25

A slot mechanism 26 (shown in Figure 10) may be fitted on the guide portion 24. It is of the form of a U-shaped slot, and will correctly orient the saw blade. The dimensions of the vertical saw guide 20 can be made so that the slot mechanism 26 points both at the correct angle and in the

30

correct position for the cut. The length x of the crank portion 23 can be given as:

$$x = r/\cos\theta - y\tan\theta$$

5

where

θ is the angle at which the guide portion 24 is axially bent away from the axis of the first end 22,

10 y is the radial distance of the crank portion 23 away from the centre of the spoon 13, and

r is the radius of the rim 15 of the spoon 13; these dimensions are shown in more detail in Figure 12 of the accompanying drawings.

15 Once these cuts have been made, the tibial plate is fitted using existing methods which may be with cement or cementless. With the tibial platform in place, the surgeon finishes the operation by fitting the implantable femur and selecting the appropriate bearing to balance the ligaments in extension and flexion using existing practices.

CLAIMS

1. A kit of parts for use in unicondylar knee replacement of a patient having a femur and a tibia, comprising a drill guide and an intramedullary rod, the intramedullary rod being sized to fit within the intramedullary canal of the femur of the patient, the drill guide being arranged so as to engage a distal end of the intramedullary rod to that which engages the patient's intramedullary canal, the drill guide being formed with a foot portion sized to fit between the patient's femur and tibia before any bone is removed from the femur or tibia, the drill guide providing a guide for drilling of at least one hole in the femur.
2. The kit of claim 1, in which the guide comprises at least one hole, through which a drill bit can be passed in order to drill the or each hole in the femur the holes including a main hole, the distance between the main hole and the foot portion being equal to a radius of the femoral component to be implanted.
3. The kit of claim 2, in which the guide comprises a further hole for drilling a further hole in the femur; the distance between the main hole and the further hole in the drill guide may be equal to a distance between the main peg and a further peg in the femoral component to be implanted.
4. The kit of any preceding claim, in which the drill guide connects to the intramedullary rod by means of a linkage comprising at least one rod which engages an end of the intramedullary rod, and a rod which engages at least two holes in the drill guide, in which the holes in the drill guide are positioned such that, for a left knee the linkage engages a first hole and not a second hole, and for a right knee the linkage engages a second hole and not the first hole.

5. The kit of any preceding claim, comprising at least one femoral component, which is to be implanted in the femur, typically including a trial femoral component which is to be temporarily implanted in the femur and a prosthetic femoral component which is to be permanently implanted
5 in the femur.

6. A kit of parts for use in unicondylar knee replacement of a patient having a femur and a tibia, comprising a femoral component for implantation in the femur, the femoral component having a bearing
10 surface having a radius of curvature, and a guide spoon, the guide spoon having a bowl-shaped portion with an internal radius of curvature the same as that of the bearing surface, and a handle portion extending from the bowl-shaped portion.

7. The kit of claim 6, in which the bowl-shaped portion has a rim; the rim and the handle portion being co-planar in a common plane, the kit of parts further comprise a clamp and a horizontal saw guide, the clamp being arranged to clamp to the hand portion and to space the saw guide from the handle portion by a pre-determined distance, typically in the
20 direction perpendicular to the common plane.

8. The kit of claim 6 or claim 7, further comprising a vertical saw guide, which comprises a first arm which engages a hole in the femoral component, the hole being keyed such that the first arm will not rotate in
25 the hole, and a second arm which extends at an angle from the mechanical axis of the femur, the angle being such that the second arm runs parallel to the diaphyseal femoral axis.

9. The kit of claim 8, in which the vertical saw guide further
30 comprises a U-shaped channel connected to the second arm and arranged to constrain a saw blade placed therein to cut parallel to the second arm.

10. The kit of any of claims 6 to 9, in which the rim of the spoon is circular with a radius sized so that, when a wall of the tibial component is installed in the cut that is to be made, there is a gap of predetermined size
5 between the wall and a bearing to be inserted between the tibial and femoral components.

11. The kit of claim 10, in which the radius of the rim is the sum of half the width of the bearing, the width of the wall and the distance
10 between the bearing and the wall, less the width of the saw blade to be used.

12. The kit of any of claims 6 to 11, further comprising at least one of the tibial component to be implanted and the saw blade to be used in
15 cutting the patient's tibia.

13. A method of performing unicondylar knee replacement of knee of a patient, comprising using the kit of parts of any of claims 1 to 5 by placing the intramedullary rod in the intramedullary canal of the femur of
20 the knee, connecting the drill guide to the intramedullary rod, placing the foot portion between the femur and the tibia of the knee, aligning the drill guide laterally to the central prominence of the femoral condyle and then drilling a hole in the femur guided by the guide.

25 14. The method of claim 13, comprising drilling a first hole in the femur by passing a drill bit through the main hole and then drilling with the bit, leaving the drill bit in place after the first hole has been drilled, and then rotating the drill guide about the main hole to correctly position the further hole, then drilling a second hole in the femur through the
30 further hole in the drill guide.

15. The method of claim 13 or claim 14, comprising the implantation of a femoral component in the patient's femur, typically a trial femoral component that is only implanted temporarily.

5 16. A method of performing unicondylar knee replacement of a knee of a patient using the kit of parts of any of claims 6 to 12, comprising implanting the femoral component in the femur of the knee, typically only temporarily, and inserting the spoon with its bowl against the bearing surface.

10

17. The method of claim 16, further comprising the step of clamping the clamp and the horizontal saw guide to the handle portion so as to position the saw guide from the handle portion by a pre-determined distance and cutting the tibia along a plane indicated by the horizontal
15 saw guide.

18. The method of claim 17, further comprise the step of inserting the vertical saw guide into the femoral component, then sawing into the tibia guided by the vertical saw guide.

20

19. A method of performing unicondylar knee replacement of a patient, comprising implanting a femoral component in the femur of a knee of the patient before a tibial component is implanted in the tibia of the knee.

25 20. The method of claim 19, comprising carrying out a method according to any of claims 13 to 15, followed by carrying out a method according any of claims 16 to 18.

21. A kit of parts comprising the kit of parts of any of claims 1 to 6
30 and the kit of parts of any of claims 7 to 12.

22. A kit of parts for use in unicondylar knee replacement substantially as described herein with reference to and as illustrated in the accompanying drawings.

1/5

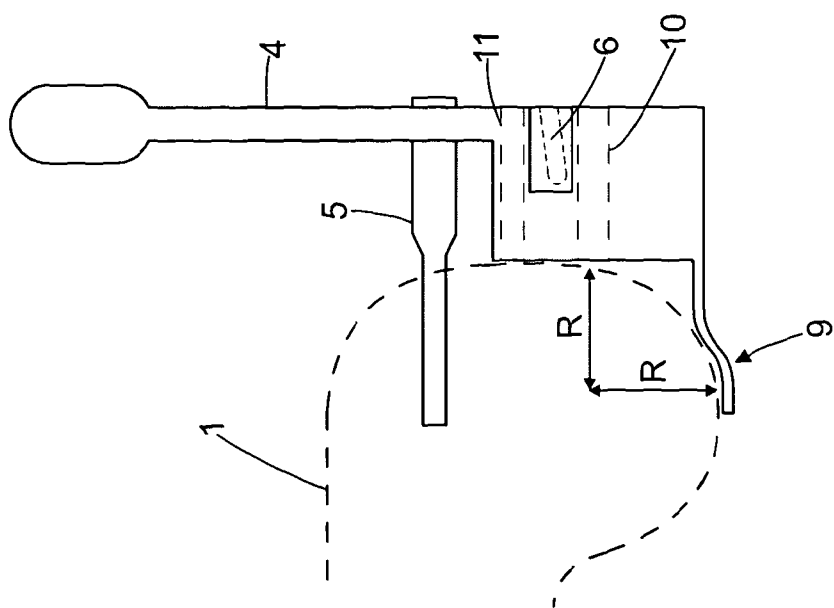


Fig. 1

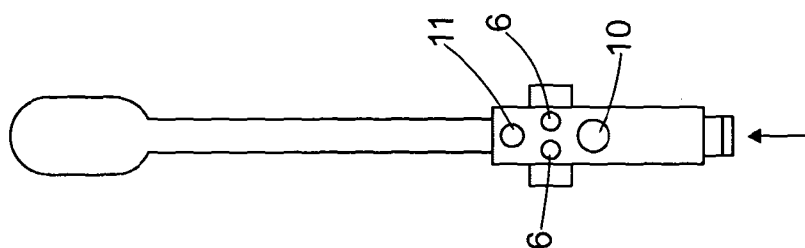


Fig. 2

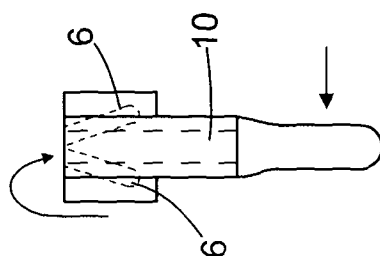


Fig. 3

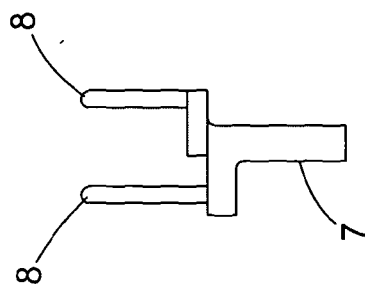


Fig. 4

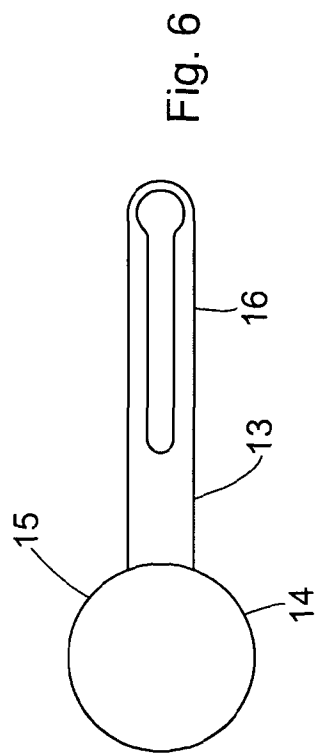


Fig. 6

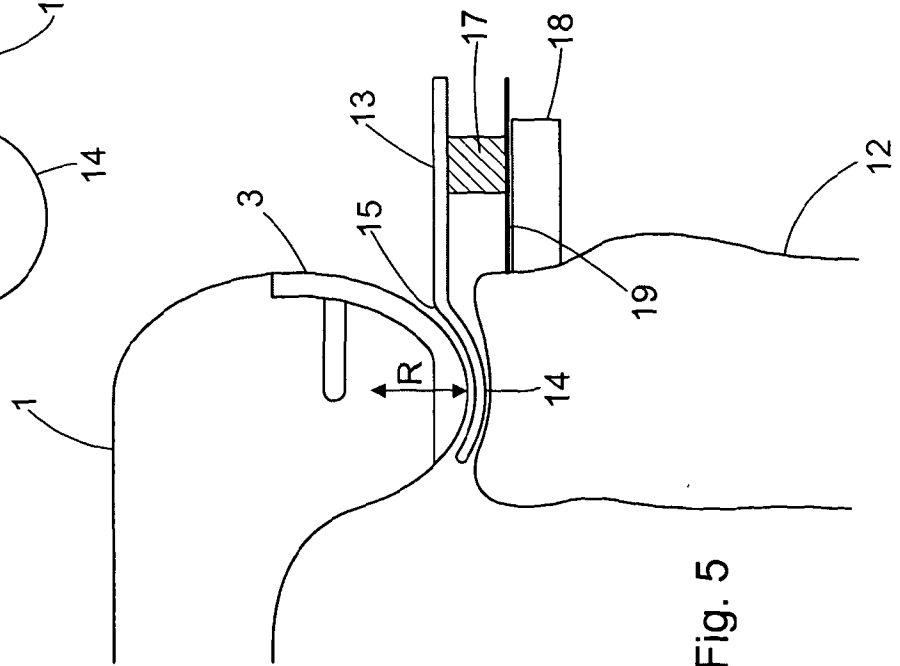


Fig. 5




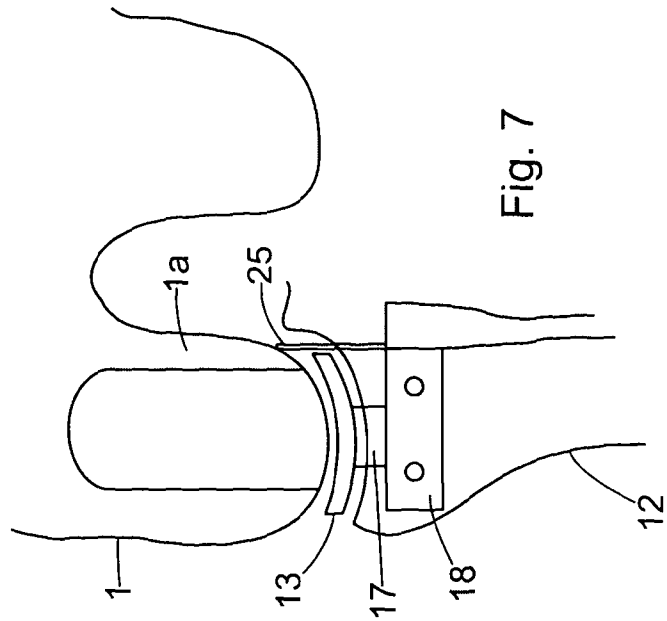


Fig. 7

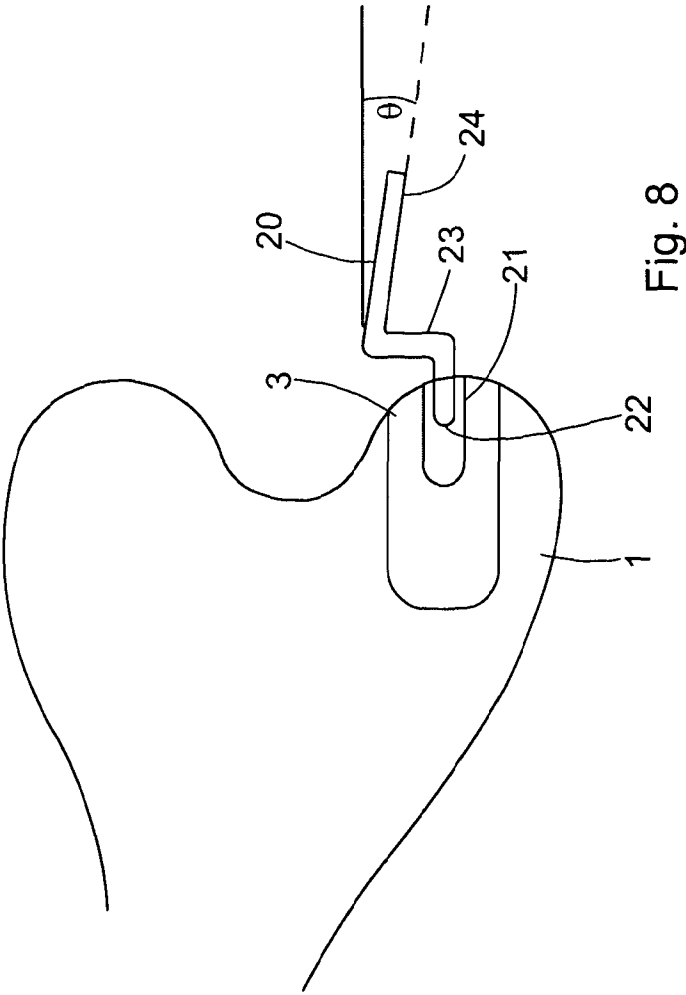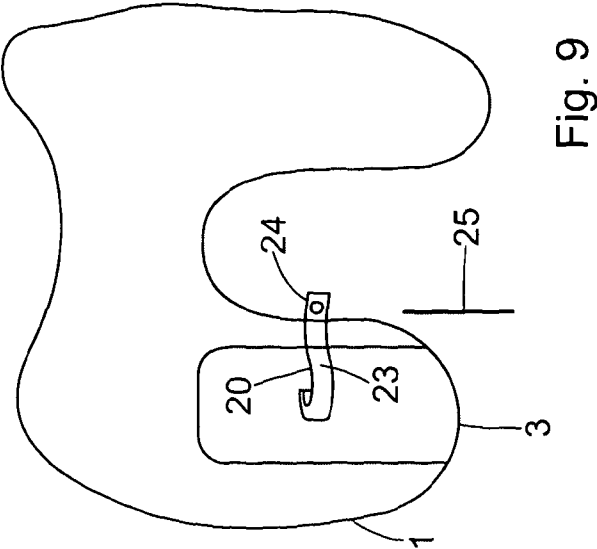

4/5

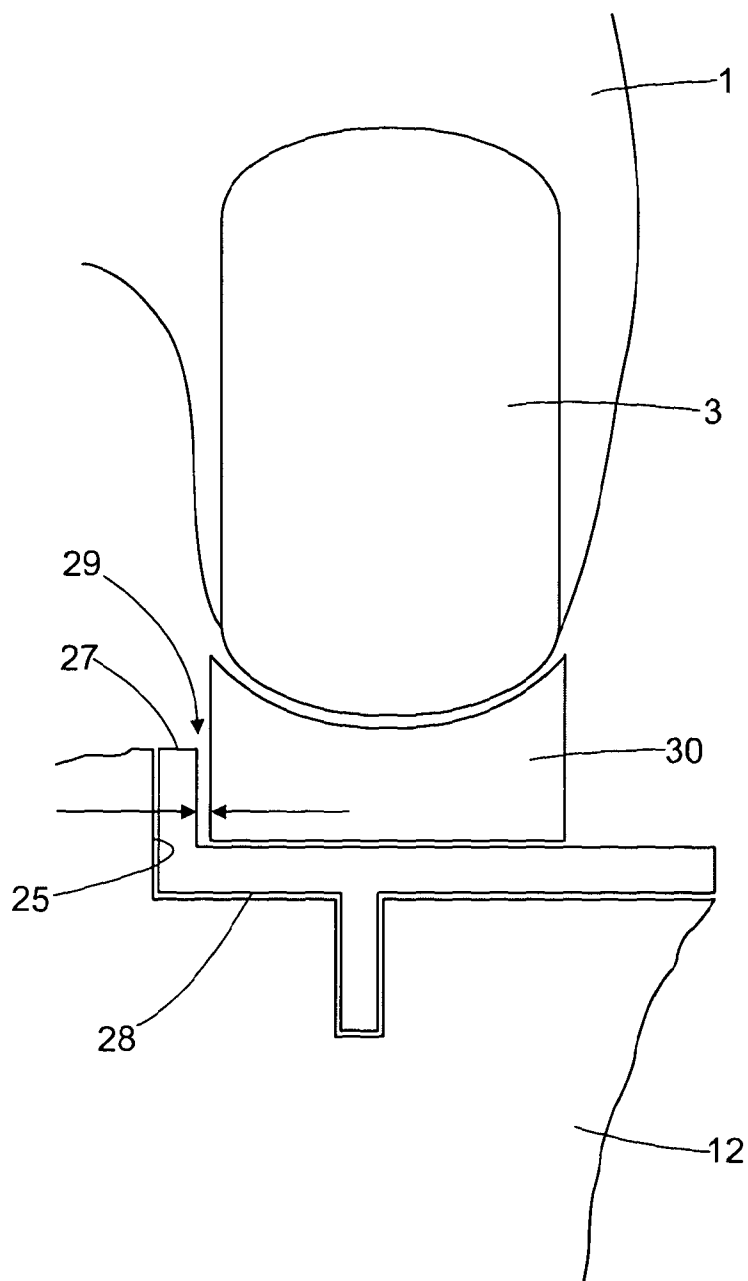


Fig. 11

5/5

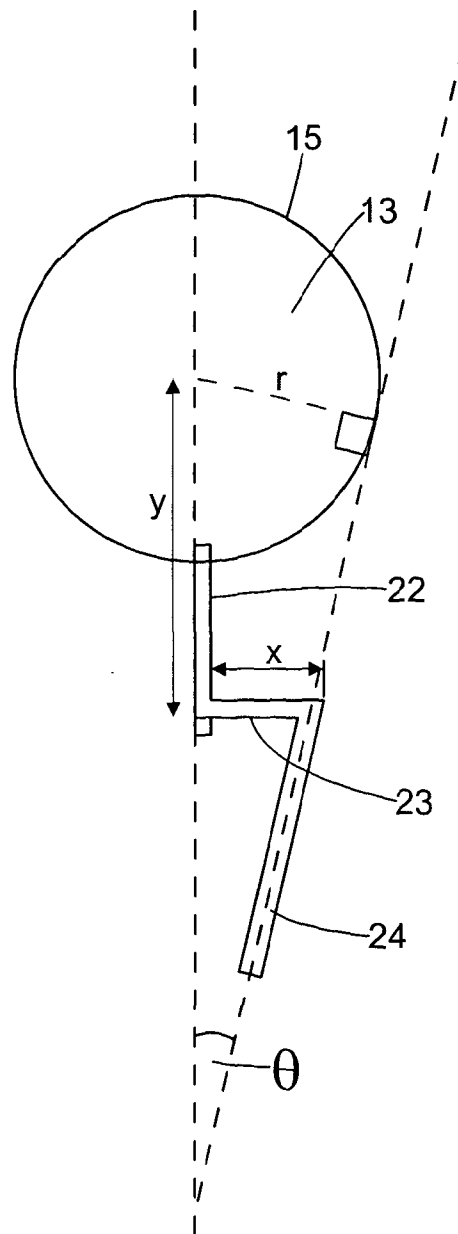


Fig. 12