

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



(10) International Publication Number

WO 2016/181404 A1

(43) International Publication Date
17 November 2016 (17.11.2016)

(51) International Patent Classification:

A61B 1/005 (2006.01)

(21) International Application Number:

PCT/IL2016/050515

(22) International Filing Date:

15 May 2016 (15.05.2016)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

62/160,253 12 May 2015 (12.05.2015) US

(72) Inventor; and

(71) Applicant : LEVY, Avraham [IL/IL]; Derech Ha Aviv 8b, Kfar Shmaryahu (IL).

(74) Agent: EREZ, Jonathan; Jonathan Erez & Co., 23 Begin Road, Tel Aviv (IL).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,

DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(54) Title: A DYNAMIC FIELD OF VIEW ENDOSCOPE

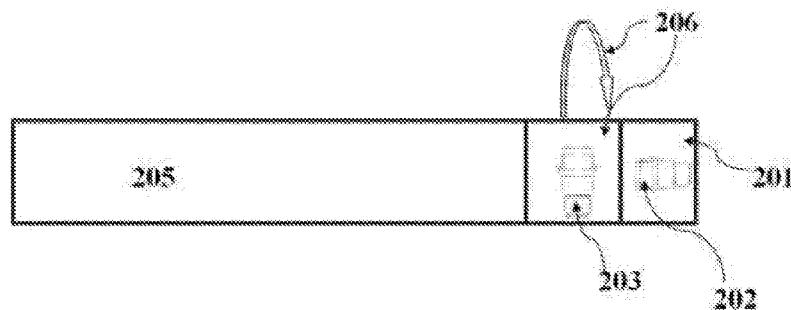


FIG. 2A

(57) Abstract: The subject matter discloses a multi-sensor endoscope having a dynamic field of view comprising an elongated shaft terminating with a tip section; a maneuvering section connected to the elongated shaft; at least two sensors, wherein at least one sensor is placed behind the tip section, on the maneuvering section; and one or more illuminators located on external surface of the shaft. In some cases, the sensors include a camera. The subject matter also discloses a multi-sensor endoscopy system comprising an endoscope comprising a handle and a controller, such that the maneuvering section is controlled by the controller.

A DYNAMIC FIELD OF VIEW ENDOSCOPE

CROSS-REFERENCE TO RELATED APPLICATION

The present application relies on, for priority, United States Provisional Patent Application number 62/160253 entitled "A Dynamic Field of View Endoscope", which is also herein incorporated by reference in its entirety.

FIELD OF THE INVENTION

The present specification relates generally to a multi sensor endoscope having a dynamic field of view.

BACKGROUND OF THE INVENTION

Endoscopes have attained great acceptance within the medical community, since they provide a means for performing procedures with minimal patient trauma, while enabling the physician to view the internal anatomy of the patient. Over the years, numerous endoscopes have been developed and categorized according to specific applications, such as laparoscopy, hysteroscopy, cystoscopy, colonoscopy, upper GI endoscopy and others. Endoscopes may be inserted into the body's natural orifices or through an incision in the skin.

An endoscope is usually an elongated tubular shaft, rigid or flexible, having a video camera or a fiber optic lens assembly at its distal end or at the back behind the tubular shaft. The shaft is connected to a handle, which sometimes includes an ocular for direct viewing. Viewing is usually possible via an external screen.

The foregoing examples of the related art and limitations related therewith are intended to be illustrative and not exclusive. Other limitations of the related art will become apparent to those of skill in the art upon a reading of the specification and a study of the figures.

SUMMARY OF THE INVENTION

The following embodiments and aspects thereof are described and illustrated in conjunction with systems, tools and methods which are meant to be exemplary and illustrative, not limiting in scope.

In one embodiment the present invention provides a multi-sensor endoscope having a dynamic field of view comprising:

- a. an elongated shaft terminating with a tip section;
- b. at least one maneuvering section;
- c. at least two sensors, wherein at least one sensor is placed behind the tip section; and
- d. one or more illuminators.

The term “behind” is defined as an area in the endoscope located towards the person holding the endoscope. That is, in case the tip section is the first section inserted into a specific tissue, the sensors located behind the tip section will be able to enter the tissue after the tip section.

In some embodiments, said maneuvering section comprises bending, rotating and or angulating section.

In another embodiment, when the endoscope comprises more than one maneuvering section, said maneuvering sections may operate separately or simultaneously.

In some embodiments each one of said maneuvering section (such as bending, rotating or angulating section) is operated manually or electrically.

In some embodiments, at least some of said sensors are placed up to 135 degrees, or 120 degrees, or 90 degrees, or 60 degrees, or 45 degrees, or 30 degrees, or 0 degrees from the elongated shaft axis at the proximal section.

In some embodiments, said sensors are pointing at different directions to one another. For example, in a three-sensor system, two sensors may be placed in opposite directions to each other, while the third sensor may be pointing to any direction.

In some embodiments, each sensor can change its viewing direction separately by using the maneuvering (e.g., rotating or bending or angulating) mechanism.

In some embodiments, one or more of said sensors is a camera.

In another embodiment, each of said cameras comprises a Charge Coupled Device (CCD) or a Complementary Metal Oxide Semiconductor (CMOS) image sensor.

In some embodiments, said multi sensor endoscope include thermal sensor or infra red (IR) light sensor, ultra violet (UV) sensor, an ultrasound sensor or a x-ray sensor.

In another embodiment one or more of said sensors that are located behind the tip section, may be located in one or more of the sections behind the tip section.

In some embodiments, at least one of said cameras comprises a lens assembly providing a field of view of 45 degrees or more.

In some embodiments, at least one of said cameras comprises a lens assembly providing a field of view of 60 degrees or more.

In some embodiments, at least one of said cameras comprises a lens assembly providing a field of view of 80 degrees or more.

In some embodiments, at least one of said cameras comprises a lens assembly providing a field of view of 100 degrees or more.

In some embodiments, at least one of said cameras comprises a lens assembly providing a field of view of 120 degrees or more.

In some embodiments, at least one of said cameras comprises a lens assembly providing a field of view of 140 degrees or more.

In some embodiments, at least one of said cameras comprises a lens assembly providing a focal length of approximately 2-20 centimeters.

In some embodiments, at least one of said cameras comprises a lens assembly providing a focal length of approximately 2-18 centimeters.

In some embodiments, at least one of said cameras comprises a lens assembly providing a focal length of approximately 2-15 centimeters.

In some embodiments, at least one of said cameras comprises a lens assembly providing a focal length of approximately 2-13 centimeters.

In some embodiments, at least one of said cameras comprises a lens assembly providing a focal length of approximately 2-10 centimeters.

In some embodiments, fields of view of said cameras are at least partially overlapping from a specific distance and specific direction of the viewing direction camera lenses, such that an object from a the specific distance of the interest viewed via said one camera remains in the field of view of said second camera while said tip section or other section behind the tip section is being turned or fixed towards the object, and at least until the object becomes visible through one of said cameras.

In some embodiments, said sensors and said illuminators are configured to operate separately or simultaneously in various combinations.

In some embodiments, each of said illuminators comprises a light-emitting diode (LED).

In some embodiments, at least one of said illuminators is configured to emit white light.

In some embodiments, at least one of said illuminators is configured to emit ultraviolet light.

In some embodiments, at least one of said illuminators is configured to emit infrared light.

In some embodiments, at least one of said illuminators is configured to emit near-infrared light.

In some embodiments, at least one of said illuminators is configured to emit light in different wavelengths.

In some embodiments, at least one of said illuminators is an ultrasound transducer to emit ultrasound signals.

In some embodiments, at least one of said illuminators is an X-ray configured to emit different X-ray wavelengths.

In some embodiments, said endoscope is a laparoscope.

In another embodiment, the present invention provides a method of achieving a dynamic field of view in an endoscope that can alternate its field of view parameters by using at least two sensors, wherein at least one sensor can move in respect to other sensor.

In another embodiment the present invention provides a multi-sensor endoscopy system comprising: an endoscope comprising a handle; an elongated shaft terminating with a tip section; a maneuvering section; at least two sensors, wherein at least one sensor is placed behind the tip section; one or more illuminators; a controller connected to said handle of said endoscope by way of a utility cable; a display connected to said controller and configured to display signals streams received from said sensors.

In addition to the exemplary aspects and embodiments described above, further aspects and embodiments will become apparent by reference to the figures and by study of the following detailed description.

BRIEF DESCRIPTION OF THE FIGURES

Exemplary embodiments are illustrated in referenced figures. Dimensions of components and features shown in the figures are generally chosen for convenience and clarity of presentation and are not necessarily shown to scale. It is intended that the embodiments and figures disclosed herein are to be considered illustrative rather than restrictive. The figures are listed below:

FIG. 1 shows a cross sectional view of a prior art endoscope.

FIGS. 2A-B show cross sectional views of a multi-sensor endoscope having a rotating section, according to exemplary embodiments of the present invention.

FIG. 3 shows a cross sectional view of a multi-sensor endoscope having a bending section, according to exemplary embodiments of the present invention.

FIG. 4 shows cross-sectional view of a multi sensor endoscope having an angulating section, according to exemplary embodiments of the present invention.

FIG. 5 shows a semi-pictorial view of a multi-sensor endoscopy system, according to exemplary embodiments of the present invention.

FIGS. 6A-B show cross-sectional views of a multi sensor endoscope having more than one maneuvering section, according to exemplary embodiments of the present invention.

DETAILED DESCRIPTION OF THE INVENTION

An aspect of embodiments related to an endoscope having an elongated shaft terminating with a tip section, a maneuvering section and two or more sensors, wherein at least one sensor is placed behind the tip section. Preferably, the sensor is a camera. For simplicity of discussion the sensors are represented by cameras, which are meant to be exemplary and illustrative, not limiting in scope.

Reference is now made to FIG. 1, which shows across sectional view of a prior art endoscope, in this example three cameras (102, 103 and 106) (as well as other elements such as a light source or a working channel, not shown) are located at the tip section (101). In this case when the shaft (105) is moving or bended, using bending section (104), the entire tip is moving and as a result the whole sensor's image is moving as well without the option of changing the directions of the cameras relatively to each other. The present invention provides an endoscope having one or more maneuvering section such as bending, rotating or angulating sections. In this configuration each sensor may be operated independently and as a result a dynamic field of view may be obtained. As used herein, the term "rotating section" refers to a section of the endoscope, which can be rotated around the shaft axis for up to 360 degrees or less.

As used herein, the term "bending section" refers to a section of the endoscope which has a plurality of links, which enable the turning of a tip section and or other section placed in front of the bending section in different directions.

As used herein, the term "angulating section" refers to a section of the endoscope, which enables the turning of the tip section and or other section placed in front of the angulating section in different directions.

During endoscopic procedures many times there is a need to extend the field of view to see more organs, and even the entire abdominal cavity, while another camera may still view another location. In order to achieve that, the present invention enables to change the direction of one camera relative to a direction of another camera during the operation. FIG. 2A shows an example of an endoscope, having a rotating section (206), a front pointing camera (202) located at the tip section (201) and another camera positioned at 90 degrees along the shaft axis (203) located at the rotating section 206.

Advantageously, this configuration allows obtaining a dynamic field of view. Here, one

sensor, e.g. the front pointing camera remains still, while the additional sensor, located at the rotating section 206 may be rotated separately, with no need to rotate the shaft 205.

FIG. 2B shows another example of a similar endoscope having a rotating section (260), a tilted front pointing camera (220) located at the tip section (210) and another camera positioned at 90 degrees along the shaft axis (230) located at the rotating section 260. Since the front camera 220 is tilted, when only the shaft (250) is (mechanically) rotated, the whole sensor image will move. Using a rotating section as described herein enables to obtain a dynamic field of view.

Another way to obtain a dynamic field of view is by using a bending section behind the tip section. FIG. 3 shows an example of an endoscope having a bending section (305) behind the tip section (301), a front pointing camera (302) located at the tip and a side pointing camera (306) located behind the bending section. The side pointing camera 306 is positioned on an external surface 307 of a tube 308 of the endoscope. The tube 308 comprises a hollow volume in which electronic wires carry information from the sensors to a remote system, as described in figure 5. This configuration allows obtaining a dynamic field of view with a wide angle of view. A similar sensor image may be obtained if an angulating section is present instead of a bending section (not shown).

However, if an angulating section is used, the control of movement is preferred. Also, when an angulating section is used instead of a rotating section, it is possible to include more sensors, e.g. cameras of the same quality, at the same proximal length. FIG. 4 shows an endoscope having an angulating section (405), a tilted front pointing camera (402) located at the frontal tip section (401), which is a portion of tip section (409). Another camera is positioned at 90 degrees along the shaft axis (403) located behind the tip section (409) and a third camera (406) located behind the angulating section (405), on an external surface 407 of the tube 408, similar to tube 308 disclosed above. This configuration allows having a dynamic field of view with a wide viewing angle.

As mentioned above the multi sensor endoscope of the present invention is not limited only to one maneuvering section, but may include two or more identical or different maneuvering sections. Reference is now made to FIGS. 6A-B, in which configurations of multi sensor endoscopes having more than one maneuvering section are

shown. Advantageously, in these configurations the field of view during maneuvering is highly controlled. Configuration A describes an endoscope comprising a bending section (604) and a rotating section (606), a front pointing camera (602) located at the tip section (601) and another camera at 90 degrees along the shaft axis (603) located behind the tip section may be rotated by rotating section (606). Configuration B describes an endoscope comprising an angulating section (670) and a rotating section (660), a tilted front pointing camera (620) located on an external surface 630 at the tip section (610), another camera at 90 degrees along the shaft axis (680) located behind the tip section may be rotated by rotating section (660) and a third camera at 90 degrees along the shaft axis (690) located behind the angulating section (670). Similarly, in other configurations (not shown), two or more maneuvering sections are present and two or more cameras may be positioned in each of these sections at different degrees along the shaft axis.

Reference is now made to FIG. 5, which shows a semi-pictorial view of a multi-sensor endoscopy system. The system may include a multi-sensor endoscope, such as the endoscope of FIGS. 2, 3, 4 and/or 6. The Multi-sensor endoscope may include a handle (510), from which an elongated shaft (520) emerges. Elongated shaft (520) terminates with a tip section (530). Handle (510) may be used for maneuvering elongated shaft (520) within a body cavity; the handle may include one or more knobs (515) and/or switches which control bending, rotating and or angulating sections (525). A utility cable (580) may connect between handle (510) and a controller (540). Utility cable (580) may include therein one or more electrical channels. The electrical channel(s) may include at least one data cable for receiving signals, e.g., video signals, from the front and side-pointing sensors, e.g. cameras as well. In addition the light source cable (590) may connect between the handle and (550) light source unit.

Controller (540) may govern power transmission to the endoscope's tip section (530), such as for the tip section's sensors. Controller (540) may further control the maneuvering by signals from the handle of one or more bending, rotating or angulating sections. One or more input devices, such as a keyboard (545), may be connected to controller (540) for the purpose of human interaction with the controller 540. A display (560) may be connected to controller (540), and configured to display signals such as images and/or

video streams received from the sensors, e.g. cameras of the multi-sensor endoscope. Display (560) may further be operative to display a user interface for allowing a human operator to set various features of system.

Optionally, when the sensors are cameras, the video streams received from the different cameras of multi-sensor endoscope may be displayed separately on display (560), either side-by-side or interchangeably (namely, the operator may switch between views from the different cameras manually).

Alternatively, these video streams may be processed by controller (540) to combine them into a single, panoramic video frame, based on an overlap between fields of view of the cameras. In another configuration (not shown), two or more displays may be connected to controller (540), each for displaying a video stream from a different camera of the multi-sensor endoscope.

Claims:

1. A multi-sensor endoscope having a dynamic field of view comprising:
 - a. an elongated shaft terminating with a tip section;
 - b. at least one maneuvering section connected to the elongated shaft;
 - c. at least two sensors, wherein at least one sensor is placed behind the tip section, on an external surface of the elongated shaft; and
 - d. one or more illuminators located on external surface of the elongated shaft.
2. The multi-sensor endoscope according to claim 1, wherein one or more of said sensors is a camera.
3. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed up to 135 degrees from the elongated shaft axis at the proximal section.
4. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed up to 120 degrees from the elongated shaft axis at the proximal section.
5. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed up to 90 degrees from the elongated shaft axis at the proximal section.
6. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed up to 60 degrees from the elongated shaft axis at the proximal section.
7. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed up to 45 degrees from the elongated shaft axis at the proximal section.
8. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed up to 30 degrees from the elongated shaft axis at the proximal section.
9. The multi sensor endoscope according to claim 1, wherein each one of said sensor is placed at 0 degrees from the elongated shaft axis at the proximal section.
10. The multi sensor endoscope according to claim 1, wherein said sensors are pointing at different directions to one another.
11. The multi-sensor endoscope according to claim 2, wherein each of said cameras comprises a Charge Coupled Device (CCD) or a Complementary Metal Oxide Semiconductor (CMOS) image sensor.

12. The multi sensor endoscope according to claim 1, wherein one or more of said sensors is a thermal sensor or infra red (IR) light sensor, ultra violet (UV) sensor, an ultrasound sensor or an X-ray sensor.
13. The multi sensor endoscope according to claim 1, wherein said maneuvering section comprises a bending section..
14. The multi sensor endoscope according to claim 1, wherein said maneuvering section comprises a rotating section.
15. The multi sensor endoscope according to claim 1, wherein said maneuvering section comprises an angulating section
16. The multi sensor endoscope according to claim 1, wherein said maneuvering sections operate separately or simultaneously.
17. The multi sensor endoscope according to claim 1, wherein each one of said maneuvering section is operated manually or electrically.
18. The multi sensor endoscope according to claim 1, wherein one or more of said sensors that are located behind the tip section, is located in one or more of the sections behind the tip.
19. The multi sensor endoscope according to claim 1, wherein said sensors and said illuminators are configured to operate separately or simultaneously in various combinations.
20. The multi sensor endoscope according to claim 1, wherein said endoscope is a laparoscope.
21. The multi sensor endoscope according to claim 1, wherein each of said illuminators comprises a light-emitting diode (LED).
22. The multi sensor endoscope according to claim 1, wherein at least one of said illuminators is configured to emit white light.
23. The multi sensor endoscope according to claim 1, wherein at least one of said illuminators is configured to emit ultraviolet light.
24. The multi sensor endoscope according to claim 1, wherein at least one of said illuminators is configured to emit infrared light.

25. The multi sensor endoscope according to claim 1, wherein at least one of said illuminators is configured to emit near-infrared light.
26. The multi sensor endoscope according to claim 1, wherein said illuminators are configured to emit light in different wavelengths.
27. The multi sensor endoscope according to claim 1, wherein at least one of said illuminators is an ultrasound transducer to emit ultrasound signals.
28. The multi sensor endoscope according to claim 1, wherein said illuminators is an X-ray configured to emit different X-ray wavelengths.
29. The multi sensor endoscope according to claim 1, wherein each sensor can change its viewing direction separately by using the maneuvering mechanism.
30. The multi sensor endoscope according to claim 2, wherein at least one of said cameras comprises a lens assembly providing a field of view of 45 degrees or more.
31. The multi sensor endoscope according to claim 2, wherein at least one of said cameras comprises a lens assembly providing a field of view of 60 degrees or more.
32. The multi sensor endoscope according to claim 2, wherein at least one of said cameras comprises a lens assembly providing a field of view of 80 degrees or more.
33. The multi sensor endoscope according to claim 2, wherein at least one of said cameras comprises a lens assembly providing a field of view of 100 degrees or more.
34. The multi sensor endoscope according to claim 2, wherein at least one of said cameras comprises a lens assembly providing a field of view of 120 degrees or more.
35. The multi sensor endoscope according to claim 2, wherein at least one of said cameras comprises a lens assembly providing a field of view of 140 degrees or more.
36. The multi sensor endoscope according to claim 2, wherein said cameras comprises a lens assembly providing a focal length of approximately 2-20 centimeters.
37. The multi sensor endoscope according to claim 2, wherein said cameras comprises a lens assembly providing a focal length of approximately 2-18 centimeters.
38. The multi sensor endoscope according to claim 2, wherein said cameras comprises a lens assembly providing a focal length of approximately 2-15 centimeters.
39. The multi sensor endoscope according to claim 2, wherein said cameras comprises a lens assembly providing a focal length of approximately 2-13 centimeters.

40. The multi sensor endoscope according to claim 2, wherein said cameras comprises a lens assembly providing a focal length of approximately 2-10 centimeters.
41. The multi sensor endoscope according to claim 2, wherein fields of view of said cameras are at least partially overlapping from a specific distance and specific direction of the viewing direction camera lenses, such that an object from a the specific distance of the interest viewed via said one camera remains in the field of view of said second camera while said tip section or other section behind the tip section is being turned or fixed towards the object, and at least until the object becomes visible through one of said cameras.
42. A method of achieving a dynamic field of view in an endoscope, comprising maneuvering at least one maneuvering section connected to an elongated shaft, wherein the maneuvering section comprises a first camera that changes a viewing direction relative to another camera of the endoscope.
43. A multi-sensor endoscopy system comprising:
 - an endoscope comprising a handle;
 - an elongated shaft terminating with a tip section, said shaft is controlled by the handle;
 - a maneuvering section connected to the elongated shaft;
 - at least two sensors, wherein at least one sensor is placed behind the tip section, on the maneuvering section;
 - one or more illuminators;
 - a controller connected to said handle of said endoscope by way of a utility cable;
 - a display connected to said controller and configured to display signals streams received from said sensors.

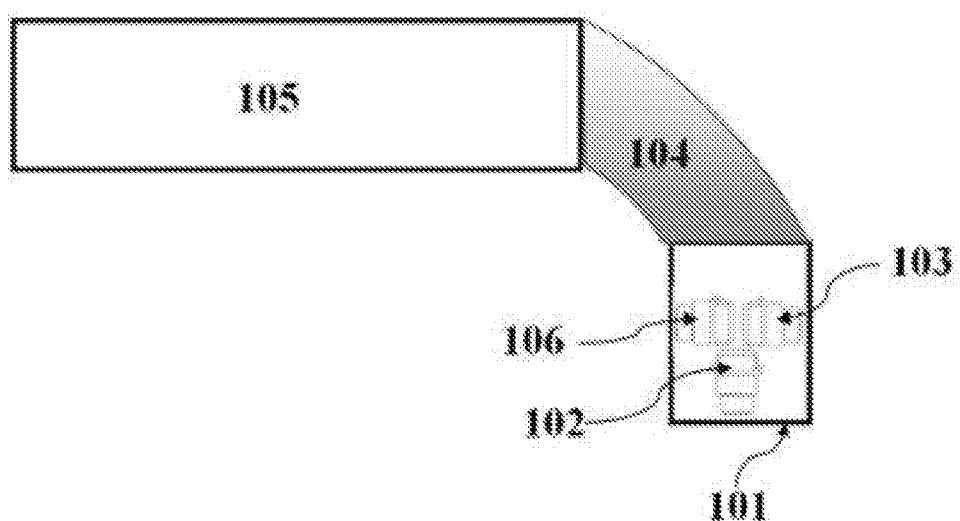


FIG. 1

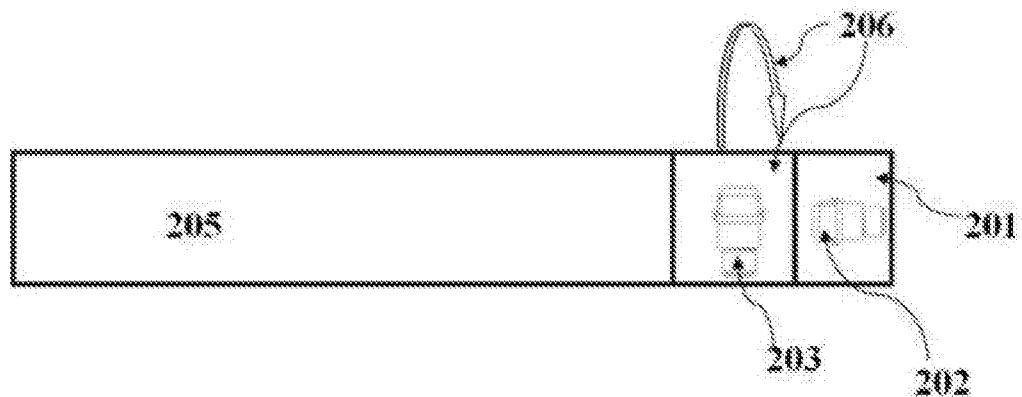


FIG. 2A

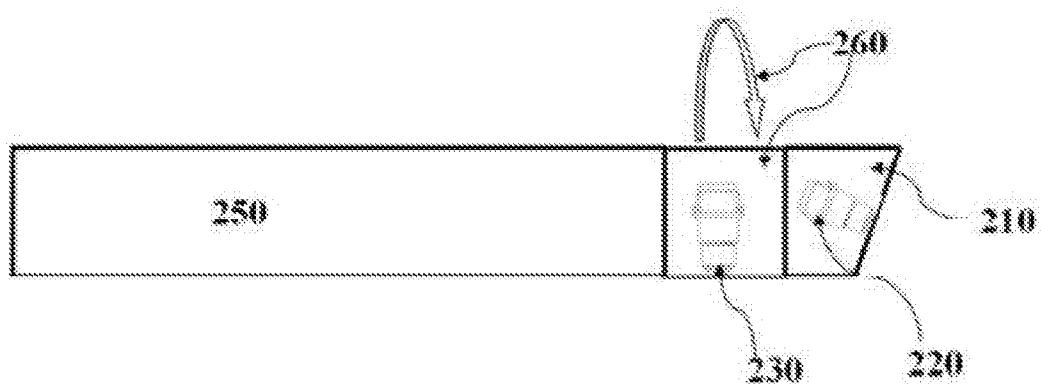


FIG. 2B

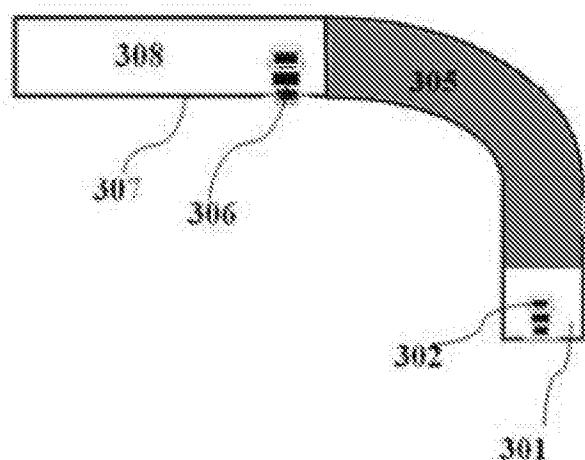


FIG. 3

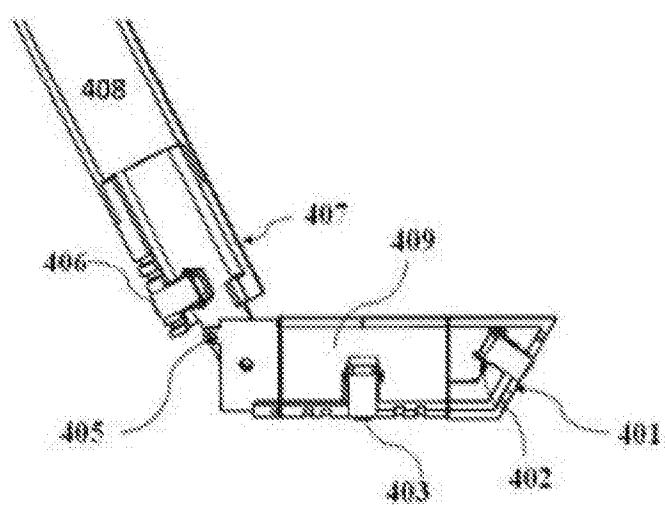


FIG. 4

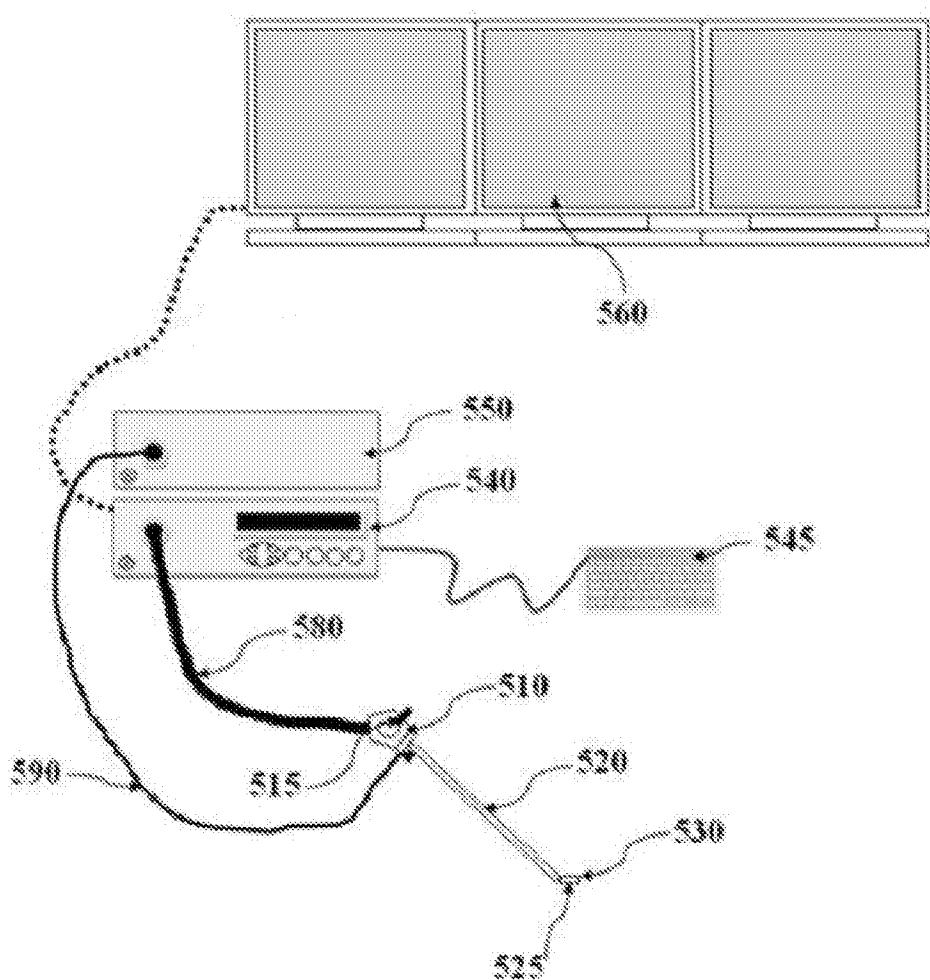


FIG. 5

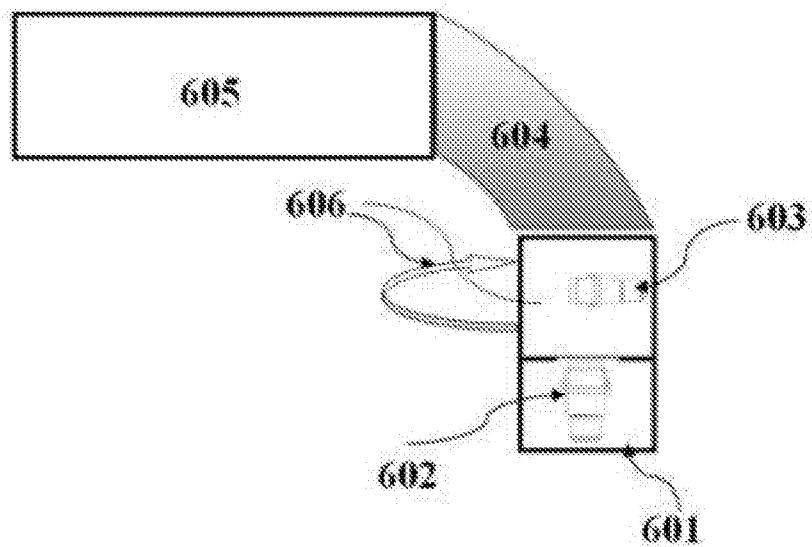


FIG. 6A

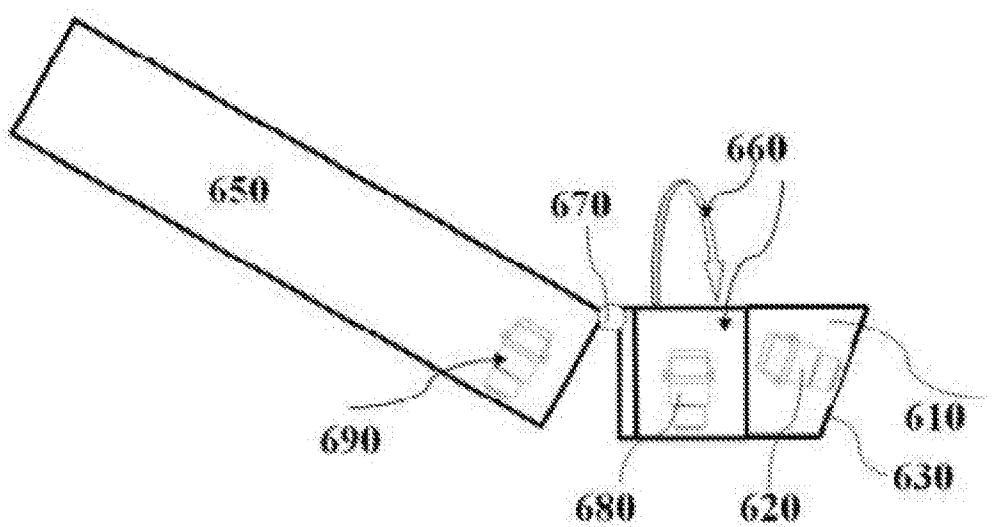


FIG. 6B

INTERNATIONAL SEARCH REPORT

International application No.

PCT/IL2016/050515

A. CLASSIFICATION OF SUBJECT MATTER

IPC (2016.01) A61B 1/005

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC (2016.01) A61B 1/005

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

Databases consulted: THOMSON INNOVATION, Esp@cenet, Google Patents

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 6846286 B2 Suzuki et al 25 Jan 2005 (2005/01/25) Abstract, Col. 14 lines 7-10, Cylinder 150 senors 212,250, Fig 25	1,43

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents:

“A” document defining the general state of the art which is not considered to be of particular relevance

“E” earlier application or patent but published on or after the international filing date

“L” document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

“O” document referring to an oral disclosure, use, exhibition or other means

“P” document published prior to the international filing date but later than the priority date claimed

“T” later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

“X” document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

“Y” document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

“&” document member of the same patent family

Date of the actual completion of the international search

05 Sep 2016

Date of mailing of the international search report

11 Sep 2016

Name and mailing address of the ISA:

Israel Patent Office

Technology Park, Bldg.5, Malcha, Jerusalem, 9695101, Israel

Facsimile No. 972-2-5651616

Authorized officer

BRODET Eyal

Telephone No. 972-5651778

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/IL2016/050515

Patent document cited search report	Publication date	Patent family member(s)		Publication Date
US 6846286 B2	25 Jan 2005	US 2002183592	A1	05 Dec 2002
		US 6846286	B2	25 Jan 2005
		JP 2002355245	A	10 Dec 2002
		JP 3845270	B2	15 Nov 2006
		JP 2002345729	A	03 Dec 2002
		JP 3881525	B2	14 Feb 2007
		JP 2002345730	A	03 Dec 2002
		JP 3881526	B2	14 Feb 2007
		JP 2002355215	A	10 Dec 2002
		JP 3898910	B2	28 Mar 2007
		JP 2003052613	A	25 Feb 2003
		JP 3911139	B2	09 May 2007
		JP 2003052614	A	25 Feb 2003
		JP 3917391	B2	23 May 2007
		JP 2003065735	A	05 Mar 2003
		JP 3920603	B2	30 May 2007
		JP 2003038493	A	12 Feb 2003
		JP 3943353	B2	11 Jul 2007
		JP 2003052612	A	25 Feb 2003
		JP 3943355	B2	11 Jul 2007
		JP 2003038492	A	12 Feb 2003
		JP 2003070718	A	11 Mar 2003
		JP 2003102677	A	08 Apr 2003