



- (51) International Patent Classification:
A61B 18/18 (2006.01)
- (21) International Application Number:
PCT/US2012/023390
- (22) International Filing Date:
31 January 2012 (31.01.2012)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
61/439,531 4 February 2011 (04.02.2011) US
61/454,901 21 March 2011 (21.03.2011) US
61/491,541 31 May 2011 (31.05.2011) US
61/537,483 21 September 2011 (21.09.2011) US
- (63) Related by continuation (CON) or continuation-in-part (CIP) to earlier application:
US 13/387,315 (CIP)
Filed on 2 November 2011 (02.11.2011)
- (71) Applicant (for all designated States except US): **ARQOS SURGICAL, INC.** [US/US]; 20195 Stevens Creek Blvd, Suite 120, Cupertino, CA 95014-2380 (US).
- (72) Inventors; and
(75) Inventors/Applicants (for US only): **GERMAIN, Aaron** [US/US]; 3563 S. Bascom Avenue, Apt. #2, Campbell, CA 95008 (US). **LESKO, Balazs** [HU/HU]; Pokmaniczky Utc 77. Iii/5., H-1064 Budapest (HU). **ORCZY-TIMKO, Benedek** [HU/HU]; Ruszti Street 10, H-1022 Budapest (HU). **TRUCKAI, Csaba** [US/US]; 19566 Arden Court, Saratoga, CA 95070 (US).
- (74) Agents: **PORTNOW, Douglas** et al.; Wilson Sonsini Goodrich & Rosati, 650 Page Mill Road, Palo Alto, CA 94304-1050 (US).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME,

[Continued on next page]

(54) Title: MEDICAL ABLATION SYSTEM AND METHOD OF USE

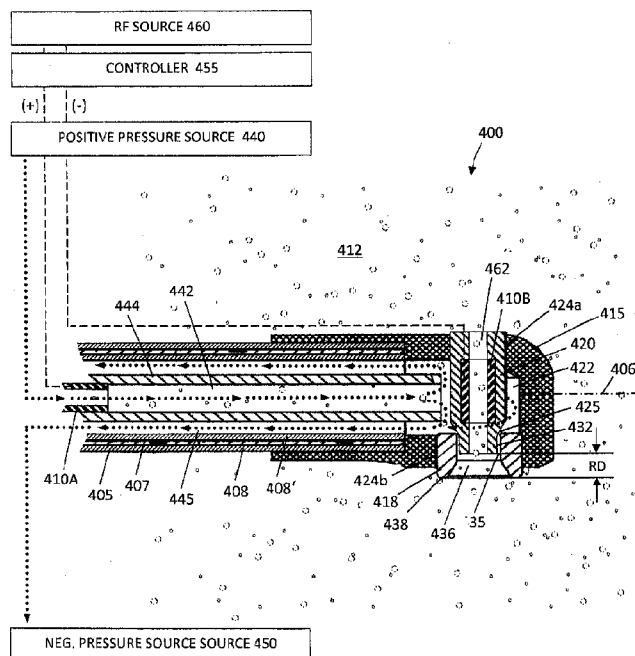


FIG. 12A

(57) Abstract: Cartilage and other tissues are treated by generating a plasma in an interior space of a probe and exposing the tissue to the plasma. The plasma is released through a gap in a working end of the probe.



MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD,

Published:

— *with international search report (Art. 21(3))*

MEDICAL ABLATION SYSTEM AND METHOD OF USE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Provisional Application Nos. 61/439,531 (Attorney Docket No. 33291-708.101), filed on February 4, 2011; 61/454,901 (Attorney Docket No. 33291-709.101), filed on March 21, 2011; 61/491,541 (Attorney Docket No. 33291-718.101), filed on May 31, 2011; and 61/537,483 (Attorney Docket No. 33291-722.101), filed on September 21, 2011; this application is also a continuation-in-part of U.S. Application No. 13/387,315 (Attorney Docket No. 33291-722.201), filed November 2, 2011, the full disclosures of which are incorporated herein by reference.

BACKGROUND OF THE INVENTION

[0002] 1. Field of the Invention. This invention relates to medical instruments and systems for applying energy to tissue, and more particularly relates to a system for ablating and treating damaged cartilage tissue.

[0003] Various types of medical instruments utilizing radiofrequency (RF) energy, laser energy and the like have been developed for delivering thermal energy to tissue, for example to ablate tissue. While such prior art forms of energy delivery work well for some applications, prior art RF and laser devices are not capable of ablating surfaces of cartilage to provide smooth surfaces. Further, such prior art devices cause unacceptable thermal damage to cartilage tissue.

[0004] What is needed are systems and methods that can controllably apply energy to fibrillated or damaged cartilage to smooth the cartilage without any thermal damage to the cartilage surface layers.

SUMMARY OF THE INVENTION

[0005] A probe for ablating tissue comprises an electrosurgical working end comprising first and second dielectric bodies and defining an interior chamber, wherein an interface between the first and second bodies is sufficiently fluid-tight to prevent liquid flow therethrough but permit plasma propagation therethrough, first and second opposing polarity electrodes configured for creating a current path within the interface. A probe for cutting and extracting tissue, comprises an elongated introducer with a first channel for tissue-extraction having a termination in a working end surface, a second channel for plasma generation having a

termination in the working surface, first and second polarity electrodes configured for igniting a plasma in a region of the second channel, and a negative pressure source in communication with the first and second channels. A method of ablating tissue, comprises providing an electrosurgical working end with an interior chamber communicating with a working surface through a space that is sufficiently fluid-tight to prevent liquid flow therethrough but permit plasma propagation therethrough, igniting a plasma in or adjacent to the gap utilizing first and second opposing polarity electrodes positioned on either side of the gap, and controlling propagation of the plasma through the gap to interface with tissue.

[0006] Methods for treating a target tissue utilize a probe having an interior space and a working end with a working surface. A plasma is ignited within the interior space and propagates outwardly from the working surface. The target tissue is exposed to the plasma for treatment, typically ablation, cutting, coagulation, resurfacing, tissue smoothing or the like.

[0007] In a first aspect of the present invention, the plasma is released from the interior space through a gap in the working end of the probe. Typically, a flow of saline or other conductive media is provided adjacent to or through the gap and ignited either before entering the gap or as it passes through the gap to generate the plasma. The gap typically has an interior periphery and an exterior periphery with a spacing therebetween which is sufficiently fluid tight (resistive to fluid flow) to inhibit fluid flow but permit plasma propagation there through. The plasma is typically ignited by applying electrical energy to the conductive medium from opposite polarity electrodes positioned on either side of the gap within one electrode within the interior space. For example, a first polarity electrode maybe disposed in proximity to the inner-periphery of the gap or may be disposed in a fluid channel in communication with said inner-periphery. The second polarity electrode may be in or on the working end in potential fluid communication with the exterior periphery of the gap. The gap typically has a mean dimension (spacing) between said interior and exterior peripheries in the range from 0.005 inches to 0.25 inches. The total area of the gap surfaces may be in the range from 0.01 mm² to 10 mm². The gap may have any one of a variety of configurations, including annular, linear, oval, elongated, star shaped, and the like.

[0008] Methods of the present invention may further comprise controlling a rate of propagation of the plasma through the gap. The plasma propagation rate may be controlled by controlling a dimension of the gap, typically a width of the gap. Alternatively or additionally, the propagation rate may be controlled by controlling a dimension of the gap between a plasma initiation region within the interior space and the working surface. Still further alternatively or additionally, the propagation rate may be controlled by varying a pressure of the conductive

media in the interior space, either by controlling the inlet pressure and/or an outlet pressure of the conductive media as it flows through the interior space.

[0009] In still other embodiments, igniting the plasma may comprise establishing a continuous “loop” flow of the conductive media throughout the interior space. In such embodiments, a portion of the conductive media is then ignited within the interior space and a remainder of the conductive medium exits the interior space. Typically, the conductive media enters the interior space through an inlet flow channel in the probe while the remainder of the conductive media exits through an outlet flow channel in the probe. The plasma which is generated within the interior space then exits or emerges through one or more gaps in the working end of the probe. In such embodiments, a propagation rate may be controlled by varying the inlet pressure, the outlet negative pressure, or a combination of both. The flows may also be controlled by varying a dimension of the gap. Plasmas are typically generated by passing current through opposite polarity electrodes in or near the interior space, and the interior space may comprise a channel transition zone between the inlet and outlet channels. Typically, the channel transition zone comprises a flow restriction, and the plasma is ignited at the flow restriction.

[0010] In all embodiments, the plasma typically propagates from the working surface by a distance of less than 2 mm, usually less than 1mm, and often less than 0.5 mm. The temperature of the plasma will usually be less than 80° C, often less than 70° C, and frequently less than 60° C. Typically, the target tissue may be submerged in a conductive medium when it is being treated by the methods disclosed herein.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] FIG. 1 is perspective view of the ablation device corresponding to the invention that includes an elongated shaft extending along an axis with an articulating working end.

[0012] FIG. 2 is a sectional view of a handle portion of the device of FIG. 1.

[0013] FIG. 3 is a perspective view of the distal ablation body portion of the device of FIG. 1.

[0014] FIG. 4 is a plan view of the distal ablation body portion of the device of FIG. 1.

[0015] FIG. 5A is a sectional longitudinal view of the working end of the device of FIG. 1 showing the slotted sleeves configured for articulation.

[0016] FIG. 5B is a cut-away view of the working end similar to FIG. 5A showing an electrode arrangement.

[0017] FIG. 6 is a cut-away view of the distal ablation body portion of the device of FIG. 1 further showing fluid flow pathways.

[0018] FIG. 7 is a schematic illustration of the device of FIG. 1 introduced into a knee joint to treat abnormal cartilage.

[0019] FIG. 8A is a longitudinal sectional view of the ablation body portion of the device of FIG. 1 showing fluid flows, plasma formation and the use of a low pressure chamber to provide a selected dimension of plasma propagating from a working surface.

[0020] FIG. 8B is another longitudinal sectional view of the ablation body portion as in FIG. 8A with the fluid flow parameters altered to provide an alternative dimension of plasma propagating from the working surface.

[0021] FIG. 9A is an illustration of a method of the invention in ablating fibrillation in cartilage tissue.

[0022] FIG. 9B is another illustration of the method of FIG. 8A which results in a smooth cartilage surface without thermal damage to the cartilage tissue.

[0023] FIG. 10A is an illustration of an alternative embodiment of a working end that is articulatable with an independently rotatable ablation body portion.

[0024] FIG. 10B is a schematic view of the working end embodiment of FIG. 10A being positioned in a hip joint to treat abnormal cartilage.

[0025] FIG. 11 is a schematic view of a RF generator, controller housing and peristaltic pumps corresponding to certain embodiments of the invention.

[0026] FIG. 12A is a sectional view of an alternative working end similar to that of FIGS. 3-6, but configured with first and second polarity electrodes disposed in the interior of the working end, wherein FIG. 12A illustrates fluid flows within the device.

[0027] FIG. 12B is a schematic cut-away view of the working end of FIG. 12A showing the RF current paths which can be substantially confined to the interior of the working end.

[0028] FIG. 13 is a schematic sectional view of another alternative working end with a different passageway configuration that carries an interior electrode.

[0029] FIG. 14A is a sectional view of a ceramic core component of an alternative working end with a different passageway including a valve.

[0030] FIG. 14B is a sectional view of another ceramic core component of a working end with a different passageway including exposure to a passive conductive or capacitive material.

[0031] FIG. 15A is a sectional view of a working end variation configured with first and second polarity electrodes disposed in the interior of the working end, wherein one electrode is within an aspiration channel, with FIG. 15A illustrating fluid flows within the device.

[0032] FIG. 15B is a schematic cut-away view of the working end of FIG. 15A showing the RF current paths which can be substantially confined to the interior of the working end.

[0033] FIG. 16A is a perspective view of an alternative working end configured with first and second polarity electrodes disposed in interior channels and a tissue extraction lumen.

[0034] FIG. 16B is a perspective view of the working end of FIG. 16A de-mated from its shaft showing the flow channels in the working end.

[0035] FIG. 17A is a sectional view of the working end of FIGS. 16A-16B showing a looped inflow-outflow channels and a first polarity electrode disposed in an interior channel, and illustrating fluid flows within the working end.

[0036] FIG. 17B is another sectional view of the working end of FIGS. 16A-16B showing a tissue extraction channel and a second polarity electrode disposed in this channel, and further illustrating a fluid flow path through the working end.

[0037] FIG. 18A is another sectional view of the working end of FIGS. 16A-16B showing fluid flows within and through the working end and first and second polarity electrodes disposed in the interior of the working end.

[0038] FIG. 18B is a sectional view as in FIG. 18A showing the RF current paths between the first and second polarity electrodes which are substantially confined to the interior of the working end.

[0039] FIG. 19 is a cut-away view of an alternative working end similar to that of FIGS. 16A-18B configured with an additional inflow channel for delivering a saline distension fluid to a working space and an alternative electrode arrangement.

[0040] FIG. 20 is a sectional view of another working end variation similar to that of FIGS. 16A-18B with a different annular interface between dielectric bodies configured for plasma formation therein and plasma propagation therethrough together with an alternative electrode arrangement.

[0041] FIG. 21 is a cut-away view of another working end variation of an ablation probe that focuses plasma formation about the end of a restrictive flow channel.

[0042] FIG. 22 is a cut-away view of another working end that is configured to form plasma in an interior chamber of the working end to heat a secondary flow of fluid through the working end.

[0043] FIG. 23 is a cut-away view of another variation that is configured with first and second restrictive flow channel portions to insure that plasma formation is directed distally from the probe's distal surface.

DETAILED DESCRIPTION OF THE INVENTION

[0044] Referring now to the drawings and the reference numbers marked thereon, FIGS. 1 and 2 illustrate one embodiment of chondroplasty plasma ablation device 100 that includes handle portion 104 and elongated shaft 105 that extends along longitudinal axis 108. The working end 110 comprises an articulating shaft portion 112 that allows the distal ablation body portion 115 to be articulated to 90° or more to thus allow the physician to orient the distal ablation body portion 115 as needed in a joint to ablate and smooth damaged regions of an articular surface, such as in a knee, hip, shoulder, ankle or other joint. In one embodiment, the shaft 105 comprises an assembly of concentric thin-wall inner and outer stainless steel sleeves 120a and 120b with an outermost assembly diameter of approximately 3.0 mm (FIGS. 2-3). An insulative polymer outer layer 118 is provided around the shaft 105, which can comprise a flexible temperature resistant material such as PEEK. It should be appreciated that the shaft 105 can be fabricated of a metal, polymer or combination thereof with a diameter ranging from about 1.0 mm to 6.0 mm. Referring to FIGS. 1, 3, 4 and 5A-5B, the articulating shaft portion 112 comprises inner and outer slotted sleeve portions, 122a and 122b, that are coupled at distal weld 124 to thus allow axial forces to be applied to one sleeve relative to the other sleeve to thus articulate the working end 110 as is known in the art. In the embodiment of FIGS. 1 and 2, the inner and outer slotted sleeve portions, 122a and 122b, can have any configuration of slot depth, orientation and shape to provide a desired range of articulated shapes, torque resistance and the like.

[0045] In FIG. 2, it can be seen that handle grip portion 128a can be moved toward handle portion 128b (from an 'open' position indicated at A toward a 'closed' position indicated at B) to articulate the working end 110. More in particular, the movement of handle portion 128a about pivot 130 causes the upper handle end block 132 to engage and move flanges 133a, 133b of the inner sleeve 120b distally to thus articulate the working end 110 between a linear shape and an articulated shape. FIGS. 1 and 2 illustrate that the shaft 105 is rotatable relative to handle 104 by manipulation of rotation collar 135 that is rotatably coupled to projecting portion 136 of the handle. The moveable handle portion 128a is further configured with a ratchet-detent member 137a that engages detents 137b in handle portion 128b which is adapted to releasably maintain the handle portions and working end 110 in a selected articulated shape. By moving the moveable handle portion 128a toward an 'open' position A, the working end 110 will return to a linear configuration as shown in FIG. 1. Actuator buttons 138a and 138b are provided in the grip portion 128a for changing the RF power level, but also can be configured for ON-OFF actuation of the system and RF power.

[0046] Now turning to FIGS. 3-6, the plasma generating system within the working end 110 is shown. FIGS. 3-4 depict one example of distal plasma ablation body portion 115 in a perspective view and in a plan view. In FIGS. 3 and 4, it can be seen that the distal body portion 115 has an expanded width relative to shaft 105 and in one embodiment can extend to a width W ranging from about 4.0 mm to 8.0 mm. FIG. 3 illustrates that the thickness T of the distal body portion is similar to the diameter of shaft 105, for example about 3.0 mm.

[0047] Of particular interest, referring to FIGS. 3-6, the entirety of the distal body portion 115 consists of electrically non-conductive materials which can comprise ceramics or a combination of ceramic and polymeric materials. In one embodiment shown in FIGS. 5A, 5B and 6, the body portion 115 comprises a PEEK housing 140, annular or donut-shaped ceramic element 142 that surrounds a core ceramic member indicated at 144. The ceramic annular element 142 and the ceramic core 144 are press-fit and bonded to bores in housing 140 to provide a very slight annular gap 145 having dimension G between the ceramic element 142 and ceramic core 144. Of particular interest, the fluid flow restriction caused by the gap 145, as will be described below, is designed to focus electrical energy density to generate plasma in gap 145. In one embodiment, the dimension G of gap 145 is 0.02 mm, and can range from about 0.005 mm to 0.06 mm. In FIG. 6, it can be seen the annular gap 145 transitions to slightly larger annular channel 146 having width dimension G' of about 0.08 mm to 0.10 mm which opens to the substantially planar surface 148 of body portion 115.

[0048] As will be described in detail below, the plasma ablation region 150 is adjacent and radially inward of the annular channel 146 in the planar surface 148. The finely controlled plasma can be generated to have different geometries dependent upon the operating parameters of power, fluid inflows and fluid outflows.

[0049] As described above, since the entire distal body portion 115 comprises electrically non-conductive materials, the working end 110 in FIGS. 5A-6 has its opposing polarity conductive electrodes 155A and 155B positioned remote from a plasma ablation region 150 that extends outward from gap 145 and annular channel 146 of distal body portion 115. As depicted in FIGS. 3 and 5A, the plasma ablation region 150 is indicated as a 'hatched' circular region in the center of the substantially planar surface 148 of the distal body portion 115.

[0050] Referring now to FIGS. 5A-5B, the first polarity electrode 155A comprises the distal portion of an interior tubular sleeve 160 of the shaft assembly. The second polarity electrode indicated at 155B comprises an exposed portion of outer slotted sleeve 120a wherein a portion of the flexible outer sleeve 118 is removed. The exposed portion of sleeve 120a that comprises

the electrode can have an area ranging from about 1 mm² to 20 mm² and can have any shape, such as an axial, circumferential, helical or another shape.

[0051] In one embodiment depicted schematically in FIGS. 5A-5B, the first polarity electrode 155A is spaced proximally a distance D from the center or centerline 156 of the plasma ablation region 150 by at least 20 mm, 30 mm, 40 mm or 50 mm. Similarly, the distal edge 158 of second polarity electrode 155B can be spaced proximally a distance D' from the centerline 156 of plasma ablation region 152 by at least 10 mm, 20 mm, 30 mm, 40 mm or 50 mm (FIG. 5A).

[0052] Referring to FIGS. 5A-5B and 6, the electrical components and the means of operation of system can be understood. In FIG. 5A, it can be seen that a pressurized fluid source 170 is in fluid communication with lumen 172 in conductive central tubular sleeve 160 which transitions into a non-conductive sleeve 175, which can be a polymeric material or a ceramic. In one embodiment, the non-conductive sleeve 175 is a flexible, non-kinkable PEEK that can flex and bend as the working end is articulated. The distal end 158 of conductive sleeve 160 is coupled to the proximal end 176 of non-conductive sleeve 175 by any suitable means such as adhesives (FIG. 6). It be seen in FIGS. 5A- 5B and FIG. 6 that lumen 172' in sleeve 175 has an open termination 176 in chamber 177 in the housing 140.

[0053] FIGS. 5A and 6 illustrate another electrically insulative component of the working end 110 that comprises flexible sleeve 180 that in one embodiment comprises a thin-wall FEP. As can be understood, FIGS. 5A and 6, the insulative FEP sleeve is adapted to provide an insulative fluid-tight layer between the first polarity electrode 150A and the slotted tubes 120a and 120b that are in the current carrying path to the exposed second polarity electrode 155B. In FIG. 6, it can be seen that the distal end 182 of the insulative sleeve 180 is bonded to sealably bonded the interior bore 184 in the housing 140.

[0054] In another aspect of the invention, still referring to FIGS. 5A-6, a circulating flow path is provided through the interior of the device (see arrows in FIG. 6) wherein positive pressure fluid source 170 supplies a saline solution that flows through lumens 172 and 172' to flow into chamber 177 of the housing 140. Thereafter, the fluid inflow reversed course and flows in the proximal direction in annular passageway 185 within the distal body portion 115 is coupled to negative pressure source 190 and a collection reservoir 192. A controller 195 is provided to control the positive and negative pressures applied within the system to provide a selected rate of liquid flow from the fluid source 170 through the device. The system further includes RF source 200 coupled by electrical leads to the first and second polarity electrodes 155A and 155B.

[0055] FIG. 7 is a schematic illustration of a method of use of the plasma ablation device of FIGS. 1-6 in treating cartilage, which is shown in a knee joint 202. It should be appreciated that the device can be used to treat cartilage in any joint, such as knees, hips, shoulders, ankles and elbows.

[0056] FIGS. 8A-8B are cut-away schematic views of the ablation body portion 115 of working end 110 and further illustrate the dimensions of 'projection' of the plasma ablation region 150 relative to planar surface 148 of distal body portion 115 when operated under different parameters. In one embodiment shown in FIG. 8A, an inflow of fluid through lumen 172' from source 170 is provided at a flow rate 10 ml/minute. The outflow of fluid through annular lumen 185 provided by negative pressure source 195 is provided at a flow rate greater than the inflow rate, and in this example is greater than 13 ml/minute. Thus, if the working end is immersed in fluid, such as in an arthroscopic procedure, and the pressurized fluid source 170 and the negative pressure source 195 are actuated without activating the RF source 200, the device will suction fluid from the arthroscopic working space into the interior chamber 177 of the device through annular gap 146—and then outwardly through lumen 185 into the collection reservoir 192. In other words, the inflows and outflows will not be in equilibrium when the RF is not actuated, resulting in suctioning of fluid from the working space. Thus, one aspect of the invention is to provide a system controller 195 that operates the inflow and outflow subsystems to thereby create a substantially low pressure in chamber 177 before the actuation of RF wherein the low pressure allows for generation of a plasma ablation region 150 with unique characteristics.

[0057] FIG. 8A depicts the ablation body portion 115 operating under first operating parameters which results in plasma ablation region 150 extending a distance P from the planar surface 148. In FIG. 8A, the operating parameters include creating very low pressures in chamber 177, for example with outflow pressure exceeding inflow pressure by greater than 10%. In operation, when the plasma is generated or ignited by actuation of RF source 200, an equilibrium is created between the inflowing media through lumen 172, the outflowing media through lumen 185, and the plasma projection through annular gap 146. Such an equilibrium is created after the plasma is generated, which initially greatly increases pressure in chamber 177. Thus, the objective of the negative pressure source 195 is demonstrated in FIG. 8A, as the applied suction from negative pressure source 195 causes the plasma to form in a low (below ambient) pressure chamber with suction forces applied to ionized gas (plasma) and flow media that is in a liquid or vapor state. Thus, it can be understood that such negative pressures applied to chamber 177 functions (i) to control the dimension P of the plasma

projected from surface 148 and (ii) to cool the plasma projected from surface 148. FIG. 8B illustrates the plasma region 150 being projected from surface 148 a certain dimension P' which is provided by reducing the net negative pressure applied to interior chamber 177 by inflow and outflow subsystems. In FIG. 8B, the operating parameters include creating a low pressure in chamber 177 wherein outflow pressure exceeds inflow pressure up to 50%.

[0058] In general, the method of the invention includes generating an equilibrium plasma in flow media within an interior of a medical device and controlling plasma projection outward of a working end surface a selected dimension ranging from 0.1 mm to 10 mm, or 0.5 mm to 5 mm.

[0059] In general, the invention is based on an appreciation of the fact that an RF-generated plasma can be controllably contained in an interior chamber 177 by providing less than ambient pressures in the interior chamber wherein the treatment plasma can be controllably emitted from at least one aperture that is in communication with the interior chamber.

[0060] Another aspect of the invention relating to tissue treatment is based on the observation that a plasma can be generated by RF energy in an interior chamber which interfaces with a negative pressure source that has the effect of cooling the plasma. In one embodiment, the temperature (i.e., average mass temperature) of the plasma is less than 80° C., less than 70° C., less than 60° C, or less than 50° C.

[0061] Another aspect of the invention is based on an appreciation of the fact that the above-described device can ablate, smooth and volumetrically remove tissue from cartilage surface without causing any thermal damage to non-targeted tissue. The energetic plasma can be generated by RF energy in an interior chamber and then projected from the device surface to ablate tissue, and the lack of collateral damage results in part from the fact that the plasma is cooled by the low pressure chamber, with the plasma temperature being selected to be less than 80° C., less than 70° C., less than 60° C or less than 50° C.

[0062] FIGS. 9A-9B illustrate a method of the invention in treating damaged region 205 of articular cartilage, such as in a patient's knee as shown in FIG. 7. In FIG. 9A, a sectional view of a small a portion of a patients joint shows the cortical or subcondral bone 212, and cartilage layer which consists of radial zone 214, transitional zone 216, and tangential zone 220. The zones 214, 216 and 220 each are characterized by differing collagen fiber orientations with the surface zone having collagen fibers and fibril oriented mostly parallel to the cartilage surface. A common form of chondromalacia or damaged cartilage is shown in FIG. 9A which consists of a fibrillated cartilage surface, wherein collagen fibril bundles 222 of the tangential zone 220 are disrupted and fibril ends 224 float outward from the cartilage surface. Such articular

cartilage damage is typically only identified after an MRI scan or when the physician view the joint with an arthroscope. The grading of cartilage damage uses the following nomenclature: Grade 0, the cartilage is normal and intact; Grade 1 cartilage has some softening and blistering; Grade 2 has partial thickness (less than 50%) defects or minor tears in the cartilage surface; Grade 3 has deeper defects (more than 50%) and Grade 4 has full thickness cartilage loss with exposure of the subchondral bone 212.

[0063] The device of the present invention is adapted for smoothing a fibrillated cartilage surface as depicted in FIGS. 9A and 9B. FIG. 9A schematically illustrates the ablation body portion 115 introduced into saline 126 that fills the joint space. FIG. 9A further depicts the plasma ablation region 150, which can have a temperature of less than 50° C, extending outward from the device to ablate and remove the fibril ends 224 that are floating into the joint space. FIG. 9B illustrates that cartilage surface after ablation and removal of the fibril ends 224 resulting in a smooth cartilage surface. Tests have been performed with the device of FIGS. 5A-9B on human cartilage tissue immediately after such tissue was removed from a patient in a 'total knee' replacement operation. It was found that the treated cartilage surface was very smooth when compared to prior art bi-polar electrode devices with exposed electrodes. In another important aspect of the invention, tests have shown that the plasma region 150 as depicted in FIGS. 9A-9B produce no thermal effects or cell death in the cartilage surface. Tests were performed using confocal laser microscopy as described in Edwards, R, "Thermal Chondroplasty of Chondromalacic Human Cartilage An Ex Vivo Comparison of Bipolar and Monopolar Radiofrequency Devices," The American Journal of Sports Medicine (2002) Vol. 30, No. 1, p 90. In tests of the present invention, no significant chondrocyte death was found as determined by cell viability staining in conjunction with confocal laser microscopy methods. In contrast, in the Edwards article above, all prior art RF devices that were tested caused substantial cell death in cartilage tissue.

[0064] FIG. 10A illustrates another embodiment of working end 110' wherein the ablation body portion 115 is rotatable relative to shaft 105 no matter how the shaft is articulated. This is accomplished by providing an additional rotatable, torque-able sleeve 230 that carries the ablation body portion 115 and is rotatable within outer articulating sleeve assembly 232. FIG. 11 is a schematic illustration of the working end of FIG. 10A being used in a hip joint 240, wherein the device is introduced through an access cannula 245. After being deployed in the joint space with the introducer shaft 105 being articulated, the ablation end 115 can be rotated (see arrow) to orient the plasma to treat targeted cartilage tissue.

[0065] FIG. 11 illustrates a controller box or housing 300 that combines an RF generator source 310, computer controller 315 and positive and negative pressure subsystems configured for operating the ablation devices described above and below. The RF source 310 can be a conventional generator as is known in the art operates at within the range of 100 kHz to 550 kHz, and in one embodiment operates at 150 kHz. The front panel of controller housing 300 carries the exposed roller pump portions of first and second peristaltic pumps 316 and 318 as are known in the art that can be configured as the positive and negative pressure subsystems. The controller and ablation system can be operated from the touch screen display 320. FIG. 11 further shows single-channel or multi-channel tubes 322 and 324 that are detachably coupled to each peristaltic pump 316 and 318 to deliver positive pressure and negative pressure to the ablation device (see FIG. 1). The system further includes a fluid or saline source 330 connected to a positive pressure source to provide fluid inflows to the ablation device and a collection reservoir 335 associated with at least one negative pressure source to collect aspirated fluid and ablation by products. A footswitch 340 is provided for ON-OFF operation of the system and the RF source, although operating controls also can be provided in the handle of the device.

[0066] FIGS. 12A-12B illustrate another variation of a plasma ablation working end 400 that configured for chondroplasty procedures. The working end 400 of FIG. 12A is carried at the distal end of shaft 405 and is based on the same operational principles described above in the embodiment of FIGS. 3-6. The shaft 405 extends about axis 406 and can comprise a thin-wall stainless steel tube 407 with insulative inner and outer coatings or layers 408 and 408'. The variation of FIGS. 12A-12B differs in that both first and second polarity electrodes, 410A and 410B, are disposed in interior passageways or regions of the device remote from articular tissue targeted for treatment. This configuration of the opposing polarity electrodes 410A and 410B provides for increased control over RF current paths in the immersed working space which consists of saline 412. More particularly, the electrode configuration can confine RF current paths substantially to the interior channels of the working end 400 and thus limit RF energy density in articular tissue to prevent active Joule heating of such tissue. In other words, the working end variation of FIGS. 12A-12B insures that targeted tissue can be treated with a low temperature plasma alone, which can best be described as "plasma etching" of such articular tissue. Such plasma etching can smooth the cartilage surface without causing thermal damage to cartilage below the articular surface.

[0067] The embodiment of FIGS. 12A-12B has a distal body portion or housing 415 that consists of electrically non-conductive materials such as a ceramic or polymer. In the

embodiment shown in FIG. 12A, the housing portion 415 is a ceramic mated with an annular, donut-shaped ceramic element 418 that partly surrounds a core ceramic member 420. The annular element 418 and ceramic core 420 extend transversely through interior chamber 422 and are bonded in bores 424a and 424b in housing 415 to provide the small annular gap 425 as described previously in which plasma formation is initiated. The annular gap 425 has a dimension as described above to function as a flow restriction wherein plasma 430 (FIG. 12B) can be controllably ignited as described in the previous embodiment. In FIG. 12A, it can be seen that the annular gap 425 transitions into annular channel 432 which has an open termination indicated at 435 from which plasma is projected outwardly. In this embodiment, the open termination 435 is within a recess or concavity 436 in the surface or perimeter 438 of body portion 415. More in particular, the open termination 435 is spaced inwardly from surface 438 a recessed dimension RD that can range from 0.5 mm to 5.0 mm. In operation, the system parameters can be modulated to cause the plasma to be projected outwardly a selected dimension from the open termination 435 of annular channel 432 into the concavity 436.

[0068] Still referring to FIG. 12A, the circulating saline flow paths are provided through the interior of the device (see dotted lines and arrows in FIG. 12A) wherein positive pressure fluid source 440 supplies a saline solution that flows through lumen or first channel 442 in insulative sleeve 444 into chamber 422 of the housing 415. Thereafter, the fluid inflow reverses course in the interior chamber 422 which may also be described as a flow transition zone herein. The fluid then can flow in the proximal direction in the concentric passageway or second channel 445 that extends through the distal body portion 415 and shaft 405 and is coupled to negative pressure source 450 and collection reservoir 335 (see FIG. 11). As can be seen in FIGS. 12A, the interior chamber 432 or transition zone also communicates with annular gap 425 and annular channel 432 which also is called a third channel herein. A controller 455 is provided to control the positive and negative pressures applied within the system to provide a selected rate of liquid flow from the fluid source 440 through the device. The system further includes RF source 460 that is operatively connected to the first and second polarity electrodes, 410A and 410B. As can be seen in FIGS. 12A and 12B, the second polarity electrode 410B is positioned in the interior of a passageway 462 that extends transverse to the axis of the shaft 405 with open ends on both sides of the working end. Thus, the passageway 462 has a dimension and configuration that permits saline 412 to flow into the passageway 462 as soon as the working end is immersed and thus electrode 410B will be in contact with the conductive saline 412 in the working space while the electrodes is maintained spaced apart from targeted tissue.

[0069] In another aspect of the invention, referring to FIG. 12B, it can be seen that RF current paths CP can extend from first polarity electrode 410A through interior chamber 422 and annular channel 432 to the second polarity electrode 410B in passageway 462 without extending substantially outward from the exterior surface 438 of the working end. This aspect of the invention allows for control of plasma as it projects outward from exits annular channel 432 and can confine plasma with the recess 436 in the surface which in turn can control any potential RF energy density is tissue. The plasma's geometry further can be controlled by modulating the operating parameters of applied RF power, fluid inflows and fluid outflows which control operating pressure in interior chamber 422.

[0070] Referring to FIGS. 12A-12B, the looped inflow and outflow subsystems provide operating parameters as described previously wherein very low pressures can be created in interior chamber 422 during plasma generation, for example with outflow pressures exceeding inflow pressures by greater than 10%. In one aspect of the invention, the negative pressure source 450 functions to modify the plasma (initiated in gap 425 and then extended outwardly through channel 432) from a volatile plasma to a non-volatile plasma. The term 'volatile' plasma, as used herein, is meant to describe the gaseous plasma media in its dynamic phase-transitioning stage, as saline is phase-transitioned instantly from liquid to water vapor and then to an ionized gas. In such a phase-transitioning or 'volatile' plasma, there is substantial popping, bubble formation and bubble collapse. Such a volatile plasma with bubble formation and collapse is undesirable in the volume of saline 412 that fills and comprises the working space (FIGS. 12A-12B). Thus, it can be understood the negative pressures applied to chamber 422 can function to suction the bubbles and liquid media from the volatile plasma in the interior chamber 422 to thereby create a non-volatile, non-bubbling plasma that can be extended through annular channel 232 to interface with targeted tissue. As described above, the negative pressures applied to interior chamber 422 additionally function (i) to control the dimension or geometry of the plasma projected outward from open termination 435 of the annular channel 432 and (ii) to cool the plasma projected from channel 432. In FIGS. 12-12B, the operating parameters include creating a low pressure in chamber 422 wherein outflow pressure from negative pressure source 450 exceeds inflow pressure of saline by at least 10%, 20%, 30%, 40% and 50%.

[0071] In general, a method corresponding to invention comprises creating a non-volatile plasma in an immersed conductive fluid workspace and interfacing the non-volatile plasma with targeted tissue. The method comprises ablating a targeted body structure with a non-volatile, non-bubbling plasma in a fluid environment which permits endoscopic viewing in the

non-bubbling environment. More in particular, the method includes positioning a probe working end in proximity to a targeted structure of a patient's body, wherein the working end includes an interior space, and creating a volatile plasma in the interior space and extending a non-volatile plasma outwardly from the interior space to interface with the targeted structure. The method includes modifying a plasma from volatile to non-volatile. The method further includes modifying the plasma by applying negative pressure to the volatile plasma to remove bubbles and liquid from the volatile plasma. The method includes igniting the plasma in flow media flowing in a looped flow through the interior space 422 in a device working end (FIGS. 12A-12B).

[0072] FIG. 13 is a cut-away view of another embodiment of working end 400' that is similar to the embodiment depicted in FIGS. 12A-12B, in which like reference numbers indicate like features. The variation in FIG. 13 differs only in the configuration of the transverse passageway in ceramic core 420 that extends transverse to the axis 406 of shaft 405 and that carries electrode 410B. In FIG. 13, it can be seen that the transverse passageway has a non-uniform cross-section with larger diameter portion 472 transitioning to smaller diameter portion 474. This variation is adapted to substantially prevent saline flows through the transverse passageway during a treatment interval which might be induced by saline or plasma flows in annular channel 432. The variation of FIG. 13 also shows the open termination 435 of the annular channel 432 is within a smooth contour concavity 475 in the working end.

[0073] FIGS. 14A-14B illustrate alternative ceramic cores 420' and 420'' that can be used in the working end embodiments of FIG. 12A or FIG. 13. The variations of FIGS. 14A-14B are again adapted to control saline flow in the transverse passageway in the ceramic core while still insuring that a conductive path is provided interior electrode 410B which is exposed to the passageway. In FIG. 14A, it can be seen that the transverse passageway 482 has a flap-valve 485 or any type of one-way valve in transverse passageway portion 486 to limit, but permit, saline flows into and/or through the passageway. FIG. 14B depicts a closed-end passageway 492 that carries electrode 410B. In FIG. 14B, the closed end 494 of the passageway interfaces with a conductive or capacitive material 496 that is not coupled to electrode 410B but can potentially carry current to saline in the passageway 492. It should be appreciated that the open end of the passageways 482 and 492 in FIGS. 14-14B can be oriented in either direction relative to opening 435 of annular channel 432.

[0074] FIGS. 15A-15B are cut-away views of another embodiment of working end 500 that is similar to the embodiment depicted in FIGS. 12A-12B and again in which like reference numbers indicate like features. The embodiment of variation in FIGS. 15A-15B includes

opposing polarity electrodes 510A and 510B disposed within active fluid flow passageways in the interior of the working end 500. In this embodiment, a second negative pressure source 515 is provided which is configured to suction flow media and fibrillated cartilage into an interface with plasma projecting outward from the opening 435 of annular channel 432. Further, the second negative pressure source 515 can extract ablation debris and bubbles from saline 412 during operation. More in particular, the second negative pressure source 515 is coupled to aspiration lumen or fourth channel 520 in insulative sleeve 522 that extends to opening 524 in transverse passageway 532 within the ceramic cores 420. As can be seen in FIG. 15A, the saline inflow from source 440 is similar to previous embodiments wherein circulating saline inflows and outflows are provided through inflow channel 536 in insulative sleeve 538 and thereafter through interior chamber 422 and outflow channel 540. In this embodiment, the first polarity electrode 510A is carried in inflow channel 536 and the second polarity electrode 510B is carried in aspiration channel 520. FIG. 15A shows the various flow channels as being concentric for convenience, and it should be appreciated that any configuration of the multiple channels can be used.

[0075] In operation, FIG. 15A indicates the various fluid flows by dotted lines and arrows. In FIG. 15B, the RF current paths CP are shown during operation in the same manner as shown in FIG. 12B to illustrate the formation of plasma 445 in the flow restriction. As can be seen in FIG. 15B, the RF current path extends from first electrode 510A exposed to saline in flow channel 536 through the flow restriction 425 (see FIG. 15A) and then through transverse passageway 532 and lumen 520 to second electrode 510B. As in the embodiment of FIGS. 12A-12B, the RF current paths are substantially confined to the interior of the working end which lowers or eliminates RF current density in tissue. In all other respects, the working end 500 functions as described previously.

[0076] FIGS. 16A-18B illustrate another electrosurgical system 600 and working end 605 that is adapted for chondroplasty procedures. In FIG. 16, it can be seen that a round or oval probe shaft 610 carries a dielectric working end 605 that can comprises ceramic bodies as generally described above. The shaft 610 can comprise a stainless steel tube covered with a thin wall dielectric material 611. In one embodiment, the distal working end 605 comprises an assembly of first and second ceramic bodies 612A and 612B (e.g., zirconium) that define an interface 615 therebetween. Both ceramic bodies 612A and 612B are carried in ceramic housing 614. The interface 615 between the ceramic bodies 612A and 612B (see FIG. 18A), terminating in gap G in the surface 618, can be extremely tight and in one embodiment the interface is sufficiently fluid-tight to prevent liquid flow therethrough but still permit electrons

and plasma to propagate through the interface 615. In working end 605 of FIGS. 16A-18B, the first and second polarity electrodes, 620A and 620B are disposed entirely within the interior of ceramic bodies 612A and 612B with no exposure in the working surface 618 or shaft 610.

[0077] Now turning to FIG. 16B, the ceramic working end 605 is shown de-mated from the shaft 610. In FIG. 16B, it can be seen that there is a looped or circulating first inflow channel 622A and second outflow channel 622B wherein a positive pressure source 625 delivers saline solution through first channel 622A and around the interior channel portion 630 (see FIG. 17A) adjacent the interface 615 between ceramic bodies 612A and 612B (see FIG. 18A). A negative pressure source 635 is configured to draw or suction the saline through channel 622B to a remote collection reservoir. In addition, the negative pressure source 635 communicates with a tissue extraction lumen 640 in the probe shaft and working end 605 which has an open termination 644 in working surface 622. In one embodiment, a single negative pressure source 635 is used to communicate with both (i) the saline outflow through second channel 622B and (ii) saline outflow through the tissue extraction channel 640. As will be described below, one embodiment provides pressure and/or a flow control mechanism positioned intermediate the negative pressure source 635 and the tissue extraction channel 640. In one such embodiment, the pressure control mechanism comprises a check valve 648 shown schematically in FIG. 16B. Such a check valve or pressure relief valve 648 can be disposed in the working end 605 or in the shaft 610 or in a handle of the device (not shown). The check valve can function to maintain negative pressure parameters in the second channel 622B and channel portion 630 (see FIGS. 17A and 18A) to maintain predetermined plasma ignition parameters in the event the tissue debris clogs the tissue extraction lumen 640.

[0078] Now turning to FIG. 17A, a sectional view is provided through a portion of the working end 605 of FIG. 16B and more particularly through the inflow and outflow channels 622A and 622B. It can be seen how the positive pressure source 625 introduces saline through first channel 622A and then around the looped channel portion 630 adjacent the interface 615 between the ceramic bodies 612A and 612B to finally flow into the outflow channel 622b assisted by the negative pressure source 635. The plasma can be controlled to project through the interface 615 to the working surface 618. FIG. 17A further shows a first polarity electrode 650A disposed in the inflow channel 622A from which RF current can flow through the interface 615 as will be described below. The electrode 650A is operatively coupled to RF source 655 and controller 660.

[0079] FIG. 17B is another section through working end 605 and more particularly through the tissue extraction channel 640 in the working end of FIG. 16B. It can be seen that the single

negative pressure source 635 is in fluid communication with the proximal end of the tissue extraction lumen 640 as well as the second channel 622B described above. Further, a second polarity electrode 650B is disposed within the tissue extraction channel 640 so that both polarity electrodes are entirely internal to the working end 605.

[0080] FIGS. 18A-18b are cut-away views of working end 605 that show fluid flows and RF current paths within the working end in using the probe to treat damaged cartilage or similar tissue. Referring to FIG. 18A, the working end 605 is shown disposed in a distending fluid, such as a saline solution, in a working space 662. The dotted lines in FIG. 18A indicate potential and actual fluid flows within the working end and through the working end 604 from the working space. FIG. 18A shows that the negative pressure source 635 is coupled to both the tissue extraction lumen 640 and the outflow lumen 622B. The purpose of the pressure control mechanism or pressure relief valve 648 can be better understood from FIG. 18A. The probe and working end 605 are designed to smooth cartilage in a working space 662 and in some instances the plasma may ablate and extract fibrillations that will clog the tissue extraction lumen 640. In such an instance, there will be an imbalance in the negative pressure source 635 applying suction pressures to both channels 622B and 640. Thus, one embodiment uses as pressure relief valve 648 which can prevent excessive negative pressure from being directed to the second channel 622B when the extraction channel 640 is clogged in which case the excessive negative pressure would alter or diminish plasma formation. In another embodiment, at least one optional pressure sensor 670 (FIG. 18B) can be provided to sense pressure in either or both channels 622B and 640 wherein the sensor can be configured to signal the controller to modulate a valve (not shown) to maintain a predetermined pressure in the second channel 622B to thereby maintain plasma formation in the interface 615. In another embodiment, referring to FIG. 19, the probe can have first and second independently controlled negative pressure sources 635 and 635' coupled to respective outflow channel 622B and tissue extraction channel 640. In another embodiment, the tissue extraction channel can carry a pressure sensor 670 as described previously (see FIG. 18B) wherein the sensor can sense tissue clogging the channel in which case the controller 660 would modulate pressure in the channel between greater negatives pressures, pulsed negative pressures, positive inflow pressures, pulsed inflow pressures, or a combination of such pressure modulations designed to remove the tissue debris clogging the channel 640.

[0081] FIG. 18B illustrates the current paths CP within and about the working end 605 during operation in which plasma is generated and translated across a tissue surface. As can be seen in FIG. 18B, both the sleeve like electrodes 650A and 650B are disposed in channels

622A and 640, respectively, in the working end 605 and the RF current paths CP communicates through channel 622A, interface 615 and extraction channel 640 to provide for plasma-tissue contact while both electrodes 650A and 650B are disposed in the interior of the working end 605. Thus, the working end 605 and system creates RF current paths CP that are confined within the working end and extend only slightly into or around a portion of the working surface 618 of the probe. In one aspect of the invention, the fact that both electrodes 650A and 650B are completely internal within the working end means the no high energy densities are created about an electrode adjacent to or in contact with tissue. This in turn means that tissue cannot be heated to high temperatures or carbonized which is undesirable and can lead to elevated immune responses and delay healing of treated tissue.

[0082] FIG. 19 illustrates another system and working end embodiment 680 which is similar to that of FIGS. 16A-16B except that this embodiment includes a further inflow channel 682 for delivering a saline distention fluid through probe and outwardly from the working end. In this embodiment, another internal saline flow is provided in the paths as previously described circulating through inflow channel 622A, loop channel portion 630 and outflow channel 622B. The tissue extraction channel 640 is again as described previously. The variation in FIG. 19 has first and second negative pressure sources 635 and 635' independently coupled to channel 622B and 640. The distention fluid channels 682 in FIG. 19 is operatively coupled to a second positive pressure source 625' which provides the saline distention fluid. In the working end 680 of FIG. 19, the opposing polarity electrodes 650A and 685 are disposed entirely within the interior of the device. In one embodiment, the first polarity electrode 650A again is carried in inflow channel 622A and the second polarity electrode 685 is carried in the distention fluid inflow channel 682. In operation, it can be understood that current paths CP (not shown) will extend from first polarity internal electrode 650A through interface 615 and inflow channel 682 to the second polarity internal electrode 685.

[0083] FIG. 20 illustrates another working end 700 embodiment that is similar to that of FIGS. 16A-18B except that the opposing polarity first and second electrodes 705A and 705B have a different configuration—still positioned within the interior channels of the working end 700. As can be seen in FIG. 20, the inflow and outflow channels 622A and 622B are similar to previous embodiments. The working end 700 further has a fluid extraction channel 640 as described previously. In one variation, the working end 700 has a looped wire first polarity electrode 705A extending through the working end through first inflow channel 622B, around looped channel portion 630 adjacent interface 615 and extending partly through second outflow channel 622B. In the working end 700 of FIG. 20, both the first and second electrodes

705A and 705B are round wires with large surface areas which enhances RF current flow in the fluid environment. This electrode configuration provides an increased surface area to the electrode and extends such an electrode surface around the region of plasma ignition which together with the absence of sharp edges can enhance the uniformity of the plasma generation in the interface 615. The electrode 705A can have any suitable diameter ranging from about 0.005" to 0.10". Similarly, the second polarity electrode 705B is configured to have a substantial exposed surface with a length, for example, ranging from 2 mm to 20 mm (and diameter of about 0.005" to 0.10") in the tissue-extraction channel 640. The distal end 708 of the electrode 705A is embedded and sealed into ceramic housing 614 to prevent any sharp electrode edges exposed to the channel 640.

[0084] As can be understood from FIG. 20, the RF current paths CP between the first and second polarity electrodes 705A and 705B extends through the interface 615 between the ceramic bodies 612A and 612Bt as described previously. In another aspect of the invention, still referring to FIG. 20, the interface 615 has a greatly increased surface area compared to previous embodiments. It can be seen in FIG. 20 that a tapered annular interface 615 is provided between the dielectric bodies 612A and 612B which after assembly comprises an extremely small gap. In one embodiment, the interface is dimensioned to be sufficiently fluid-tight to prevent liquid flow therethrough and will only permit current flows and plasma propagation therethrough. In this embodiment, the tapered interface or taper lock between the first and second dielectric bodies 612A and 612B is provided by a predetermined surface roughness that is fabricated on either or both dielectric bodies 612A and 612B at either side of the interface 615. In other words, the first and second dielectric bodies 612A and 612B are wedged together tightly with a micron or sub-micron dimensioned gap between the surface finishes of the mating dielectric bodies.

[0085] In one embodiment, the interface 615 is annular as shown in FIG. 20 and extends between a first interior periphery 710 of the interface 615 and a second exterior periphery 715 of the interface wherein the mean dimension between the inner and outer peripheries ranges from 0.005" to 0.25". Although the variation of FIG. 20 illustrates an annular interface 615, the scope of the invention includes any interface configuration such as a linear configuration, an oval configuration, any elongated configuration, or a polygonal or star-shaped configuration. The total area of such an interface 615 can be from 0.01 mm² to 10 mm².

[0086] In general, a method of ablating tissue corresponding to the invention comprises providing an electrosurgical working end with an interior chamber communicating with a working surface through a space that is sufficiently fluid-tight to prevent liquid flow

therethrough but permit plasma propagation therethrough, igniting a plasma in the gap utilizing first and second opposing polarity electrodes positioned on either side of the gap, and controlling propagation of the plasma through the gap to interface with tissue. In one aspect of the invention, the plasma propagation is controlled by controlling pressure interior of the gap. In another aspect of the invention, the plasma propagation is controlled by controlling the dimensions of said gap which can comprised the width or cross section of the gap and/or the dimension between the inner and outer peripheries of the gap.

[0087] In another variation, an ablation probe 840 is shown in FIG. 21 that has a working end 850A configured to expose plasma to tissue in a focused manner. The probe 840 includes a handle 852 and extension member 855 that terminates in working end 850A. The working end 850A comprises a body portion 856 of an insulator such as a ceramic carried in a metal sleeve 860. The working end 850A can be carried at the end of a rigid shaft or a flexible catheter, and can have a diameter ranging from 1 mm to 6 mm. The ceramic body portion 856 has a small diameter or cross-section flow channel 865 that extends through the working end and is coupled to a pressurized flow source 870 of a conductive fluid such as saline. In the embodiment of FIG. 21, the system includes an RF source 875A and controller 875B that couples energy to opposing polarity electrodes, which comprise a tungsten or similar wire 877 disposed in channel 865 and a wherein the second electrode comprises the exposed portion of metal sleeve 860. The pressurized flow of conductive liquid thus functions as a liquid electrode as the flow extends through flow channel 865 until its distal termination or outlet 880 (Fig. 22) in a distal surface of the ceramic body 856. When the probe is operated in a submerged environment such as in saline 882, the flow channel 865 has a selected cross section or diameter that provides high resistance to flow which in turn causes high impedance to electrical current flow therein. As a result of coupling electrical energy to the fluid flow, the flow restriction causes the highest energy density to occur about the outlet 880 and thus a highly localized plasma 885 (Fig. 21) ignites about the outlet 880. In one embodiment, the diameter of the channel 865 is 230 microns and such diameter can range from about 10 to 500 microns. The length of channel 865 extending from outlet 880 can range from about 5 mm to several cm or can extend substantially through the extension member 855. The distal end 887 of electrode wire 877 can be axially spaced from the outlet 880 by a distance A ranging from about 10 mm to 100 mm. The distal end of electrode sleeve 860 can also be axially spaced from outlet 880 by a distance ranging from about 10 mm to 100 mm. As can be seen in FIG. 21, an insulative sleeve 888 is provided about extension member 855. In use, the working end 850A and plasma 885 can be moved into contact with tissue (not shown) to thereby cause localized ablation of tissue, for example in an orthopedic or other procedure.

[0088] FIG. 22 illustrates another variation of ablation probe 840 with a different working end 850B that operates in a similar manner to the embodiment shown in FIG. 21. In FIG. 22, the working end 850B again comprises a ceramic body comprising concentric ceramic sleeves 856A and 856B carried in metal sleeve 860. The small diameter flow channel 865 coupled to saline flow source 870 again extends through the center of the working end. In the embodiment of FIG. 22, the system further provides a second pressurized flow of conductive liquid through channel 890 between sleeves 856A and 856B into a larger open bore 892. In operation in a submerged saline environment 882, the flow channel 865 again provides high resistance to flow causing high impedance to RF current flow therein. The coupling of electrical energy to the flow again ignites the localized plasma 885 about outlet 880. In this variation of FIG. 22, the plasma 885 can heat the liquid flowing into bore or chamber 892 to create a heated fluid media 895 which can be used to contact tissue to thereby heat tissue. This embodiment can operate in pulses of electrical delivery to develop pulses of heated fluid that can be expelled from the working end to treat tissue. An outer insulative sleeve on the extension member 855 is not shown for convenience in FIG. 22 and subsequent figures.

[0089] FIG. 23 illustrates another variation of ablation probe 900 with an elongate probe shaft 902 extending to a working end 905 that functions in a similar manner as the embodiment of FIG. 21. The shaft 902 can be rigid or a flexible member and can have a diameter ranging from 2 mm to 5 mm with any square, rounded, blunt or concave distal surface 906. In FIG. 23, the working end 905 comprises an insulative body 908 that can comprise a ceramic material and extends distally from metal sleeve 910. A flow channel 915 in the ceramic body extends to an outlet 916 in the distal surface 906 of the probe. The channel 915 has a first or proximal channel region 918A that extends proximally through the shaft 900 and communicates with saline flow source 870. The diameter of proximal channel region 918A can range from about 0.5 mm to 5 mm. In this variation, the working end 905 includes a first polarity electrode 920 (+) in a second or distal flow channel portion 918B that can have a diameter in the range of the proximal channel portion 918A. The second polarity electrode indicated at 925 (-) comprises the metal sleeve 910. As can be seen in FIG. 23, saline that flows from source 870 through channel 915 moves through a first flow restriction channel 926A proximal to channel region 918B and thereafter moves through a second flow restriction channel 926B to outlet 916. In one variation, the distal or second flow restriction channel 926B has a smaller diameter or cross-section than the proximal restriction channel 926A. It has been found that the providing the smaller restriction channel 926A can prevent any plasma formation or migration into the restriction channel 926A or the proximal channel portion 918A. The proximal restriction

channel 926A can have a diameter or cross-section that is less than 95%, 90%, 80%, 70%, 60 or 50% of the diameter cross-section of the distal flow restriction channel 926B. As can be understood from FIG. 23, the plasma 885 will form about the outlet 916 and the physician can move the probe surface 906 into an interface with tissue to precisely ablate a targeted tissue region.

[0090] Although particular embodiments of the present invention have been described above in detail, it will be understood that this description is merely for purposes of illustration and the above description of the invention is not exhaustive. Specific features of the invention are shown in some drawings and not in others, and this is for convenience only and any feature may be combined with another in accordance with the invention. A number of variations and alternatives will be apparent to one having ordinary skills in the art. Such alternatives and variations are intended to be included within the scope of the claims. Particular features that are presented in dependent claims can be combined and fall within the scope of the invention. The invention also encompasses embodiments as if dependent claims were alternatively written in a multiple dependent claim format with reference to other independent claims.

What is claimed is:

1. A device for applying energy to tissue, comprising:
an elongate probe carrying an energy applicator body;
first and second channels in the probe communicating an interior chamber in the applicator body;
a positive pressure source coupled to the first channel configured to provide a fluid inflow toward the interior chamber;
a negative pressure source coupled to the second channel configured to provide a fluid out flow away from the interior chamber; and
an electrode arrangement carried by the probe capable of applying energy to the fluid sufficient to create a plasma in proximity to the interior chamber.
2. The device of claim 1, further comprising a third channel extending between the interior chamber and a surface of the applicator body.
3. The device of claim 2, wherein the third channel has an annular configuration.
4. The device of claim 3, including a flow restrictor intermediate the interior chamber and an open termination of the third channel in said surface.
5. The device of claim 4, wherein the flow restrictor has an annular configuration.
6. The device of claim 4, wherein the flow restrictor comprises a plurality of apertures.
7. The device of claim 2, wherein the first polarity electrode is in the first channel.
8. The device of claim 7, wherein the second polarity electrode is in the second channel.

9. The device of claim 7, wherein the second polarity electrode is in a fourth channel having an open termination in the surface of the applicator body.

10. The device of claim 1, wherein the fluid flow comprises a conductive liquid.

11. The device of claim 10, wherein the conductive liquid is a saline solution.

12. A probe for ablating tissue, comprising:
an electrosurgical working end comprising first and second dielectric bodies and defining an interior chamber;

wherein an interface between the first and second bodies is sufficiently fluid-tight to prevent liquid flow therethrough but permit plasma propagation therethrough;

first and second opposing polarity electrodes configured for creating a current path within the interface.

13. The probe of claim 12, wherein the interface has an interior periphery exposed to the interior chamber and an exterior periphery exposed to an exterior surface of the working end.

14. The probe of claim 12, wherein the first polarity electrode had a surface exposed to the interior chamber.

15. The probe of claim 12, wherein the first polarity electrode had a surface exposed to lumen communicating with the interior chamber.

16. The probe of claim 12, wherein the second polarity electrode at least partly comprises an exterior probe surface.

17. The probe of claim 12, wherein the second polarity electrode is within an interior lumen communicating with an opening in the working end.

18. The probe of claim 12, wherein the second polarity electrode is within an aspiration lumen in the probe.

19. The probe of claim 12, further comprising a liquid source coupled to an inflow lumen communicating with the interior chamber.

20. The probe of claim 12, further comprising a negative pressure source coupled to an outflow lumen communicating with the interior chamber.

21. A probe for ablating tissue, comprising:
an electrosurgical working end comprising first and second dielectric bodies defining an interface therebetween that is sufficiently fluid-tight to prevent liquid flow therethrough but permit plasma propagation therethrough; and
first and second opposing polarity electrodes carried by the working end.

22. The probe of claim 21, wherein the interface has an interior periphery and exterior periphery and further comprising a first polarity electrode in proximity to said inner periphery.

23. The probe of claim 21, wherein the first polarity electrode is in a fluid channel in communication with said inner periphery.

24. The probe of claim 23, further comprising a second polarity electrode in the working end in potential fluid communication with said exterior periphery.

25. The probe of claim 21, wherein a mean dimension between said interior and exterior peripheries of the interface is from 0.005" to 0.25".

26. The probe of claim 21, wherein the total area of the interface is from 0.01 mm² to 10 mm².

27. The probe of claim 21, wherein the interface has an annular configuration.

28. The probe of claim 21, wherein the interface has a linear configuration.
29. The probe of claim 21, wherein the interface has an oval configuration.
30. The probe of claim 21, wherein the interface has an elongated configuration.
31. The probe of claim 21, wherein the interface has a star-shaped configuration.
32. A probe for cutting and extracting tissue, comprising:
 - an elongated introducer with a first channel for tissue-extraction having a termination in a working end surface;
 - a second channel for plasma generation having a termination in the working surface;
 - first and second polarity electrodes configured for igniting a plasma in a region of the second channel; and
 - a negative pressure source in communication with the first and second channels.
33. The probe of claim 32, wherein further comprising a pressure control mechanism intermediate the negative pressure source and the first channel.
34. The probe of claim 33, wherein the pressure control mechanism comprises a relief valve.
35. The probe of claim 33, wherein the pressure control mechanism comprises a pressure balancing mechanism for balancing pressure between the first and second channels.
36. The probe of claim 32, wherein further comprising a pressure control mechanism intermediate the negative pressure source and the second channel.
37. The probe of claim 32, wherein further comprising a first negative pressure source in communication with the first channel.

38. The probe of claim 32, wherein further comprising a second negative pressure source in communication with the second channel.

39. A probe for cutting and extracting tissue, comprising:
an elongated introducer with a first channel for tissue-extraction having a termination in a working end surface;
a second channel for plasma generation having a termination in the working surface;
a first polarity electrode carried in the first channel; and
a second polarity electrodes carried in the second channel.

40. The probe of claim 39, further comprising a negative pressure source in communication with at least one of the first and second channels.

41. The probe of claim 39, further comprising a negative pressure source in communication with both the first and second channels.

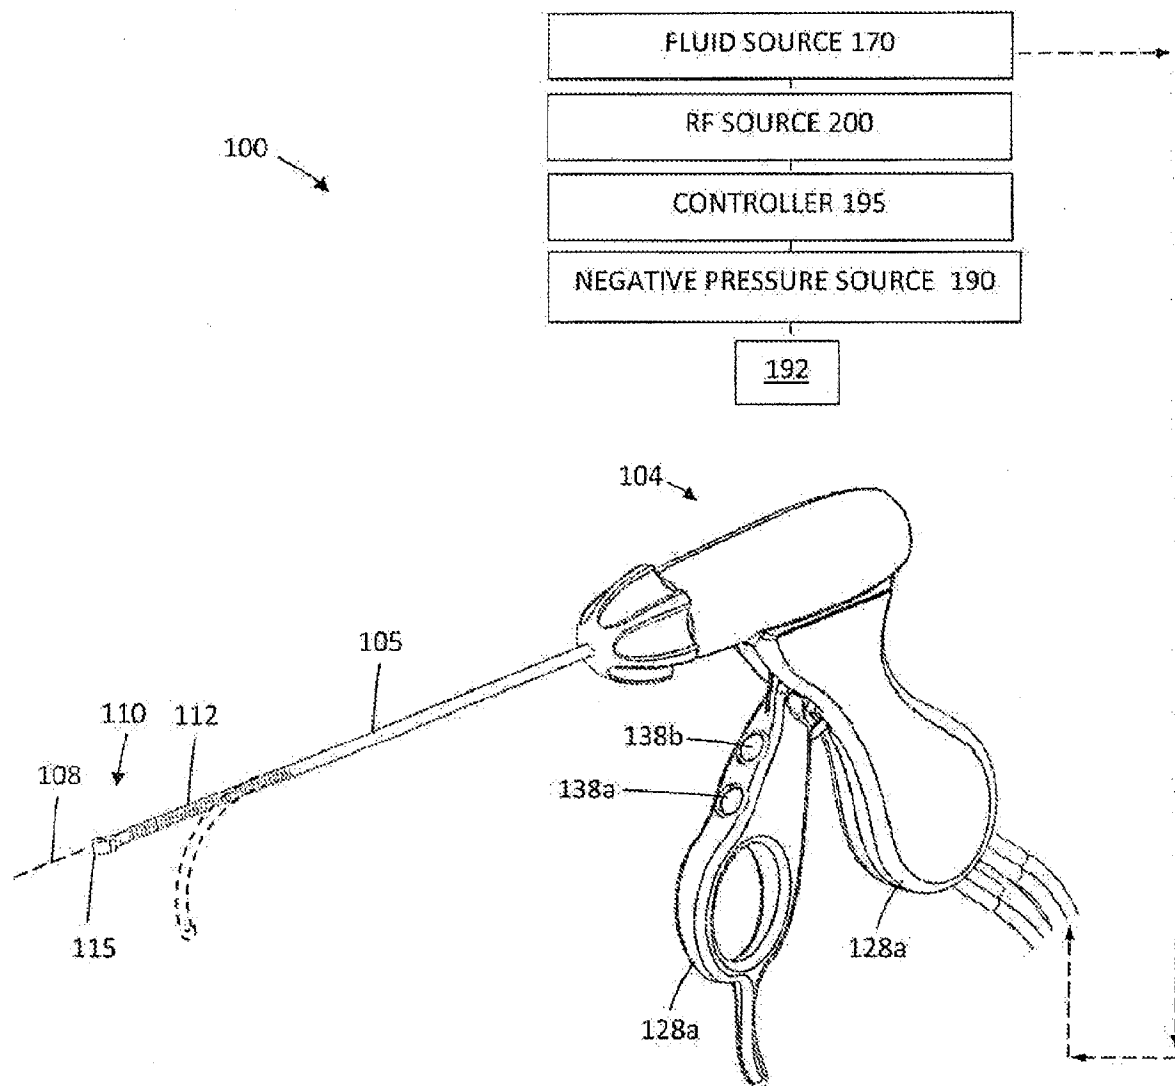


FIG. 1

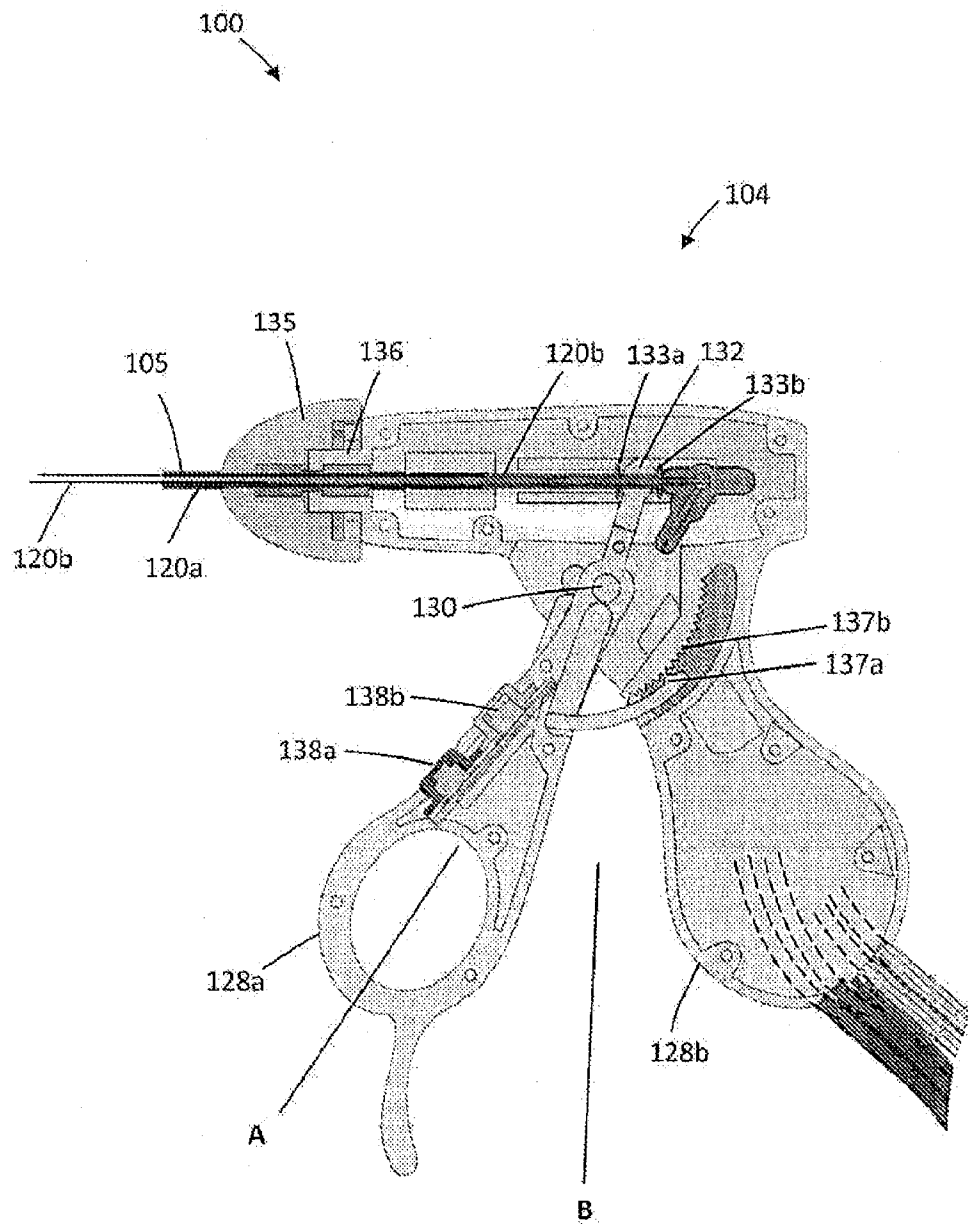


FIG. 2

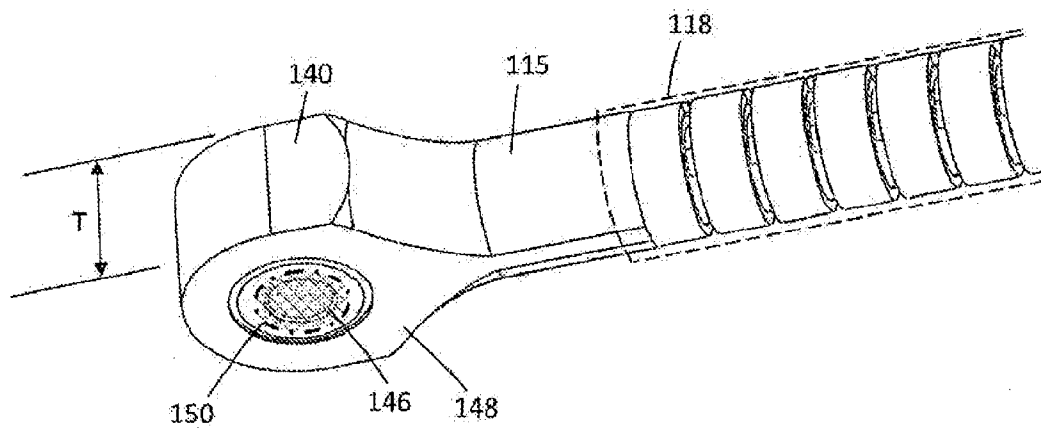


FIG. 3

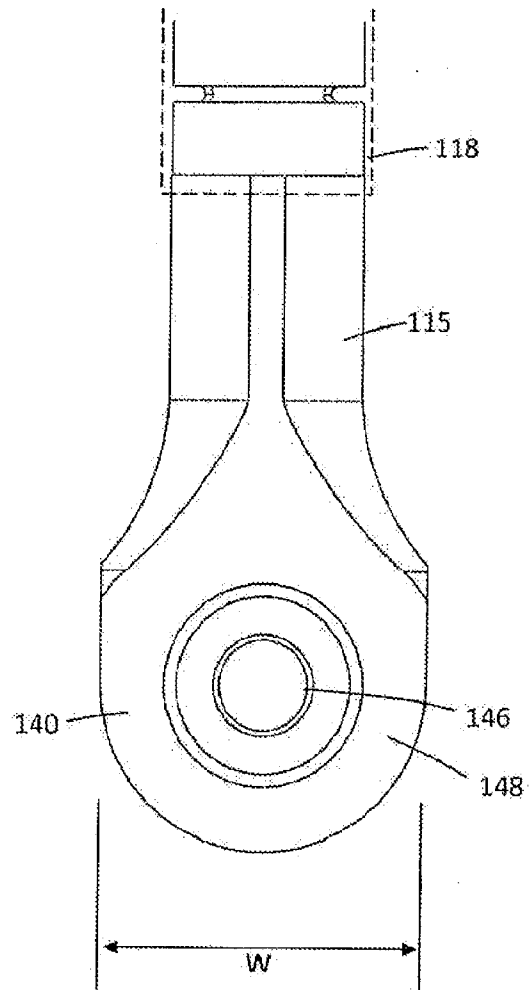


FIG. 4

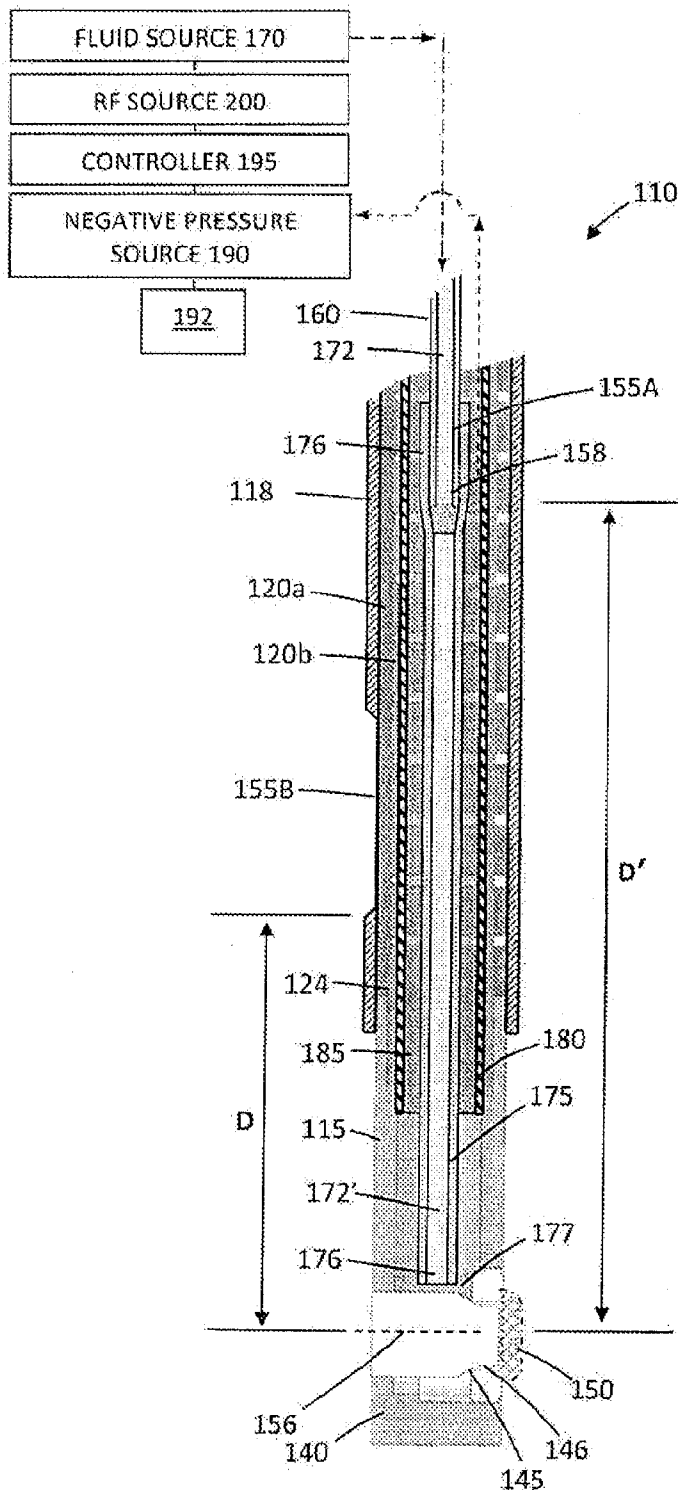


FIG. 5A

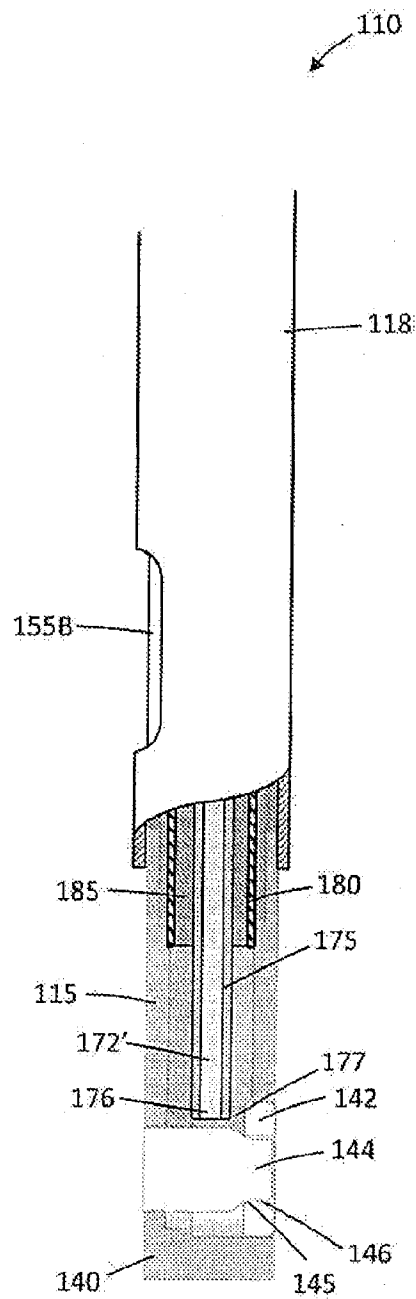


FIG. 5B

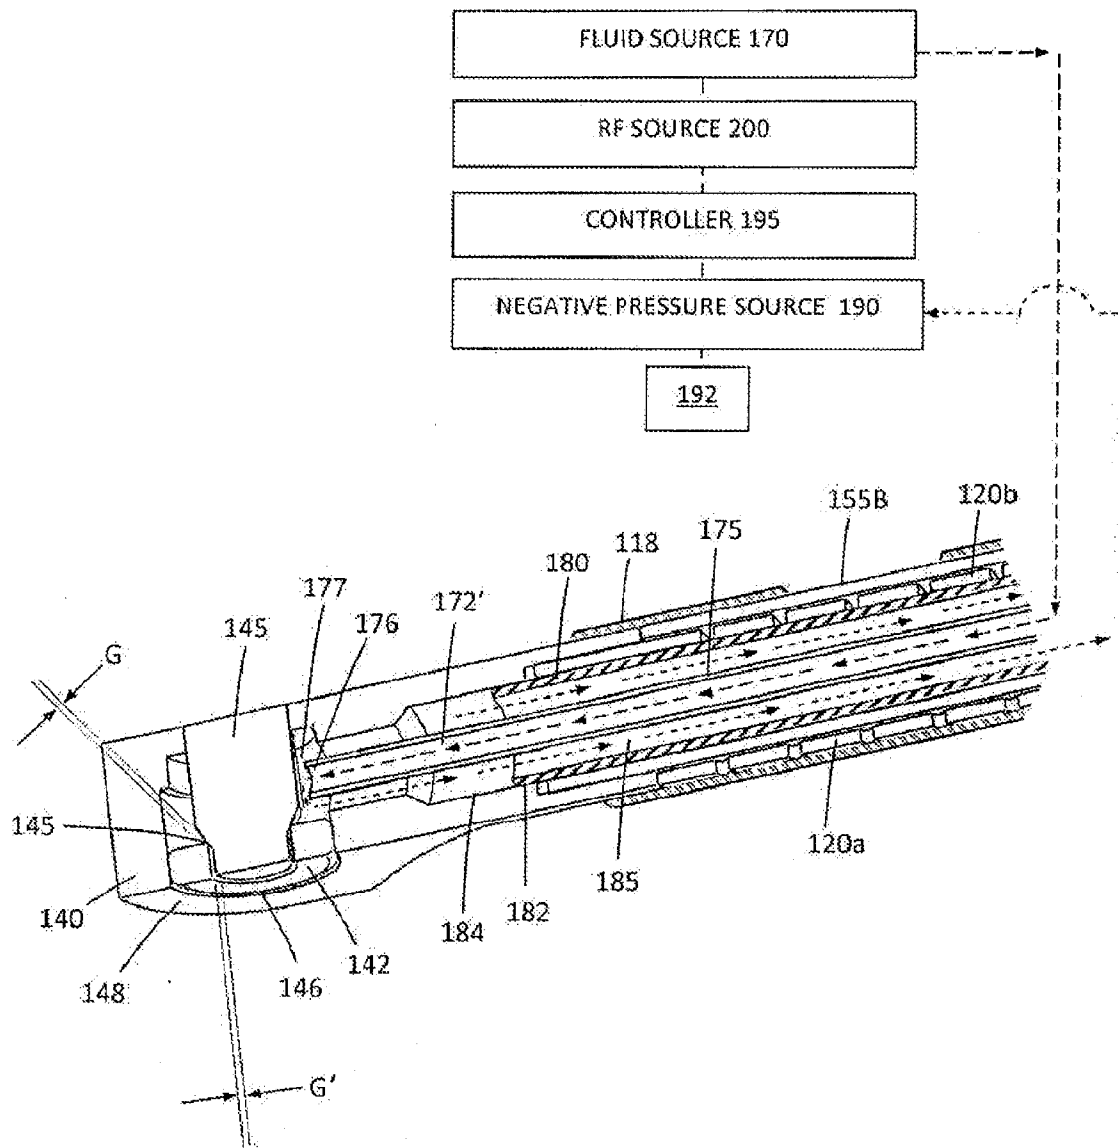


FIG. 6

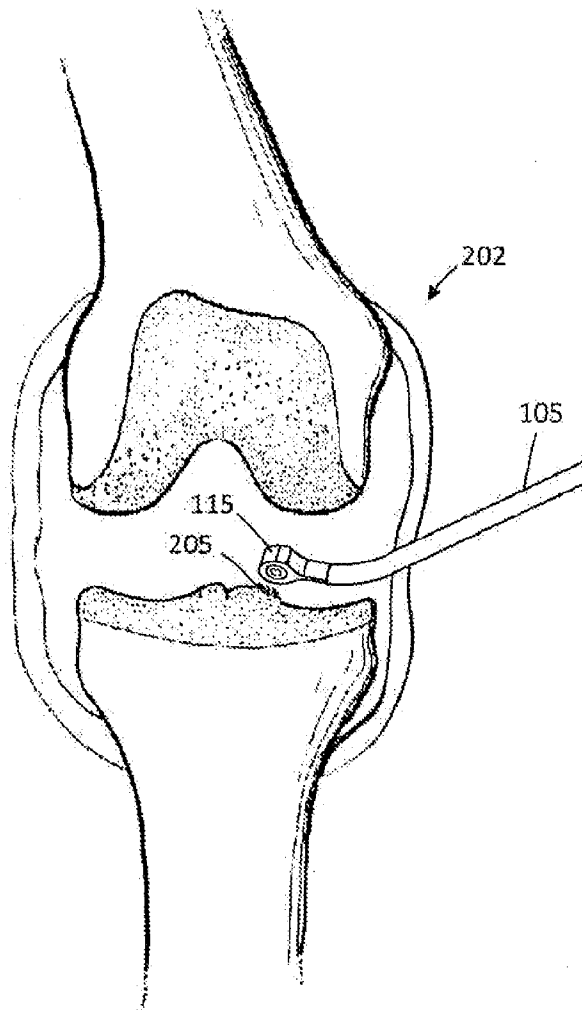


FIG. 7

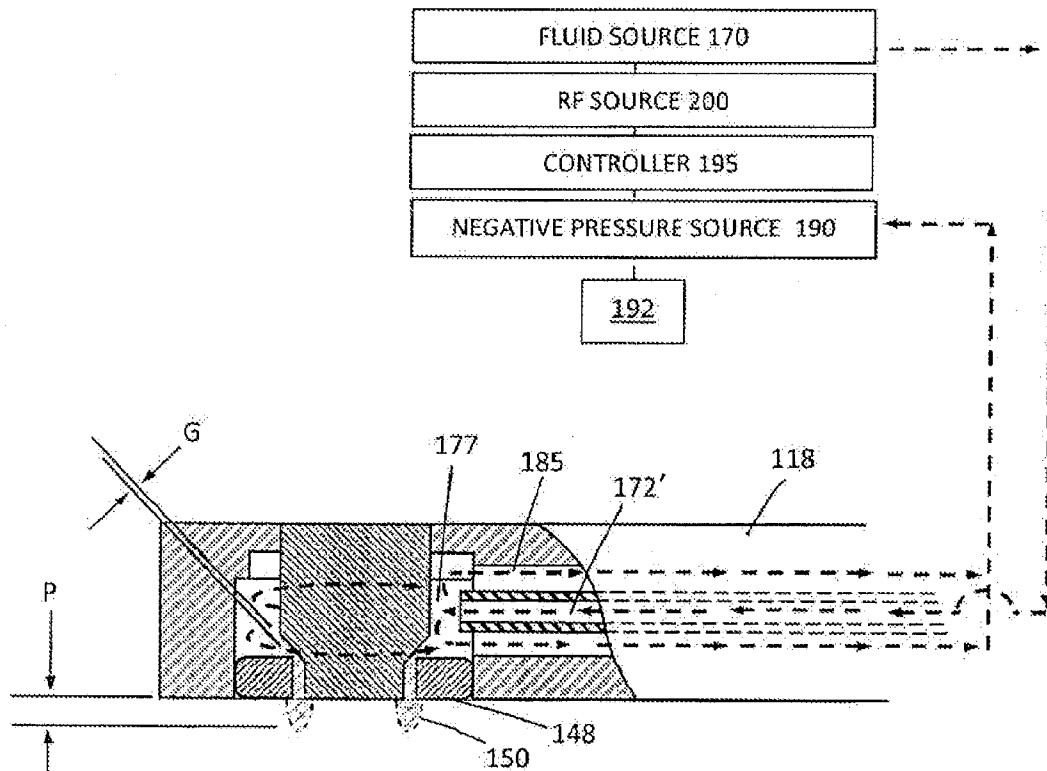


FIG. 8A

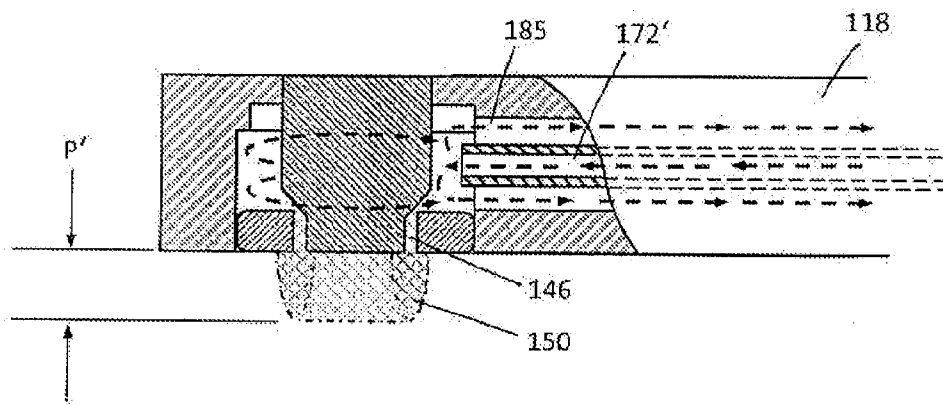


FIG. 8B

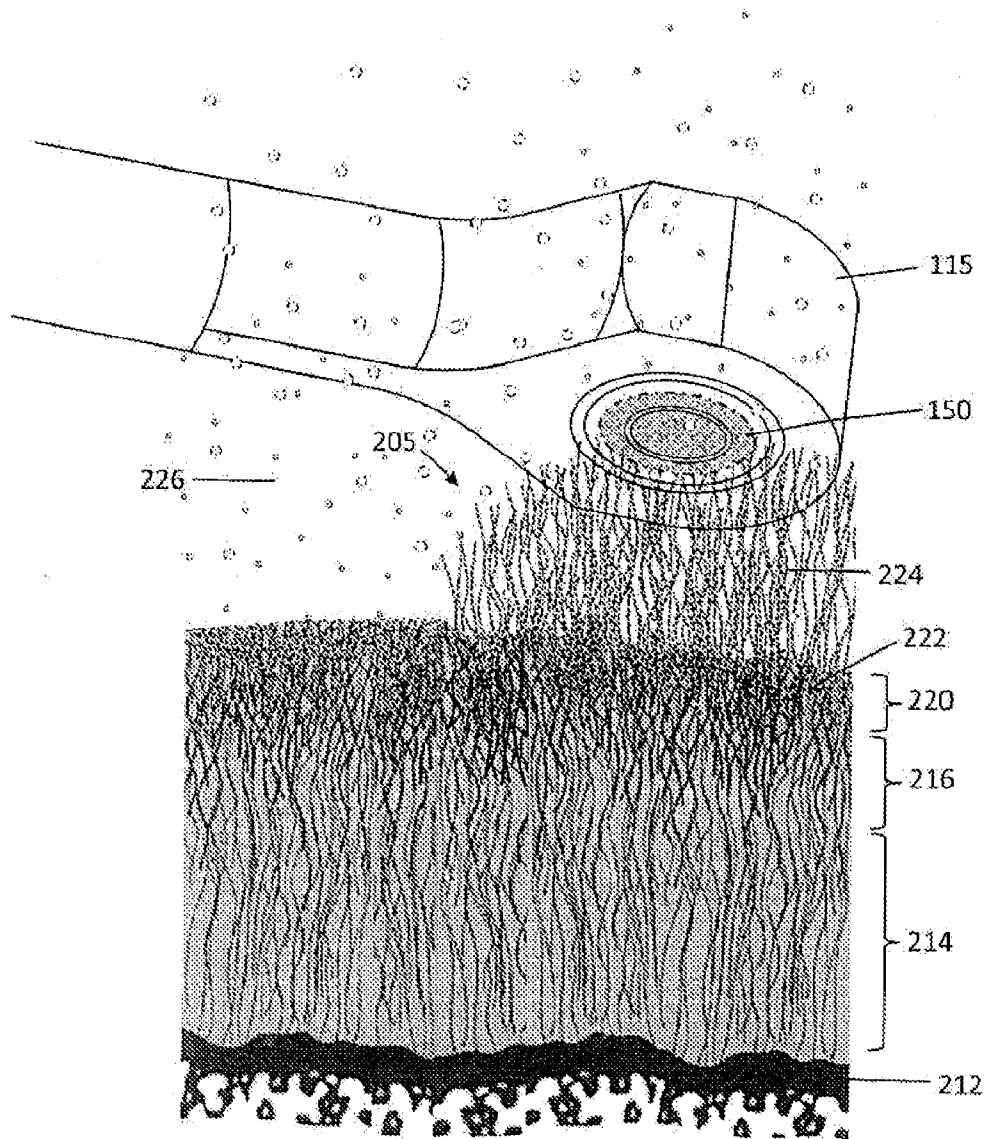


FIG. 9A

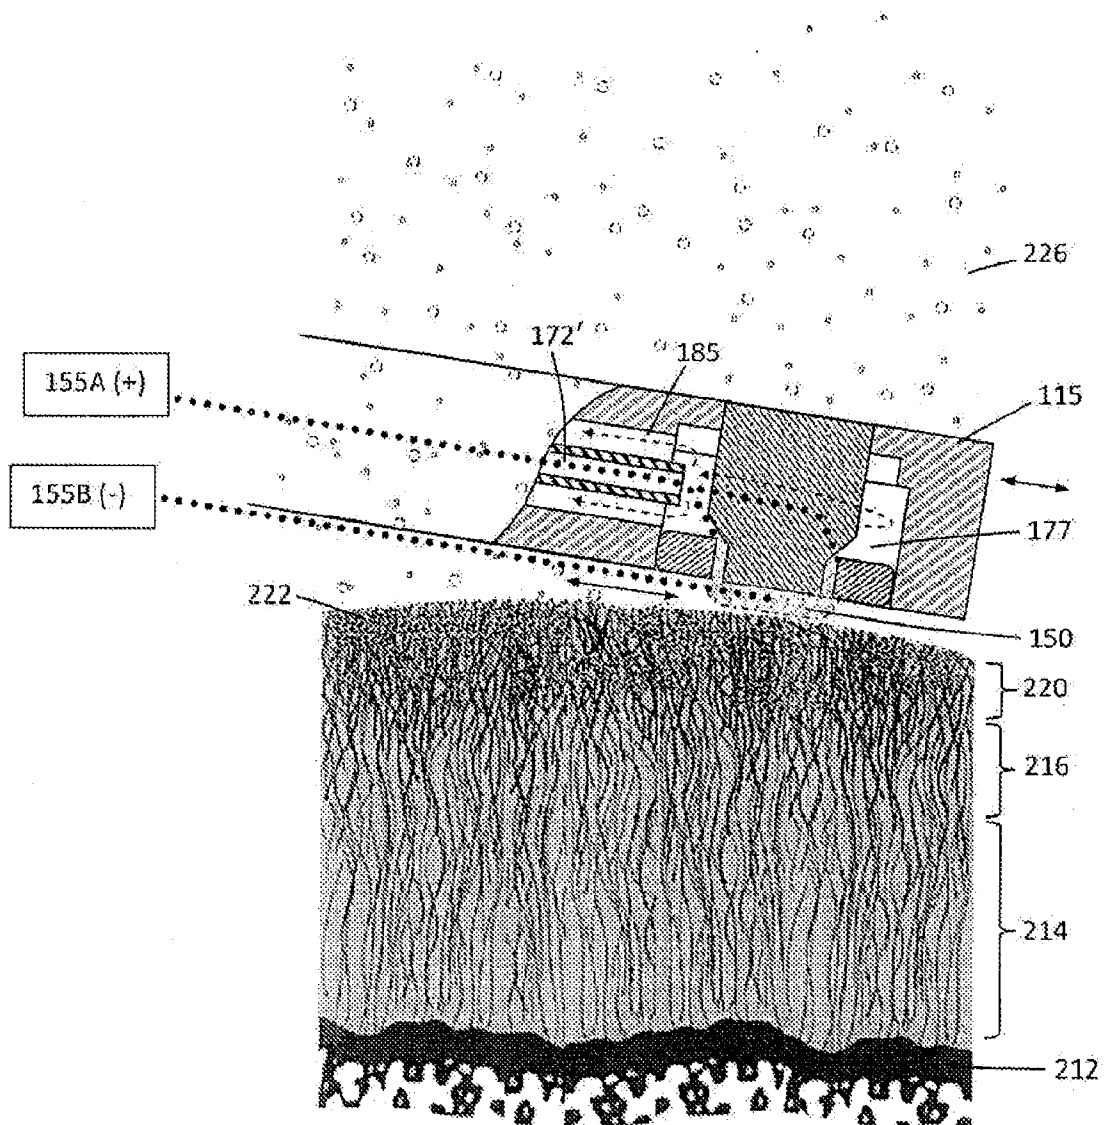


FIG. 9B

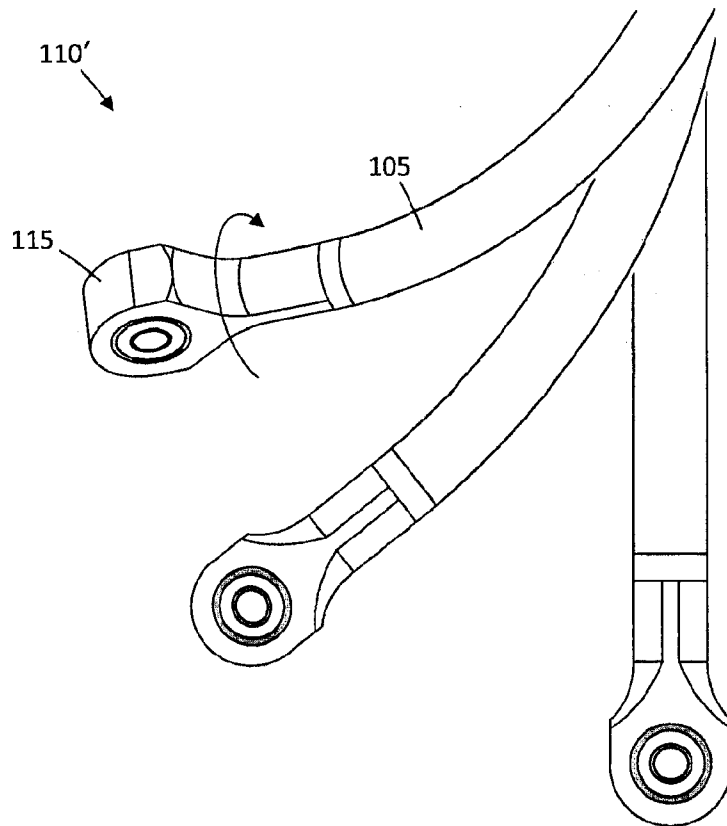


FIG. 10A

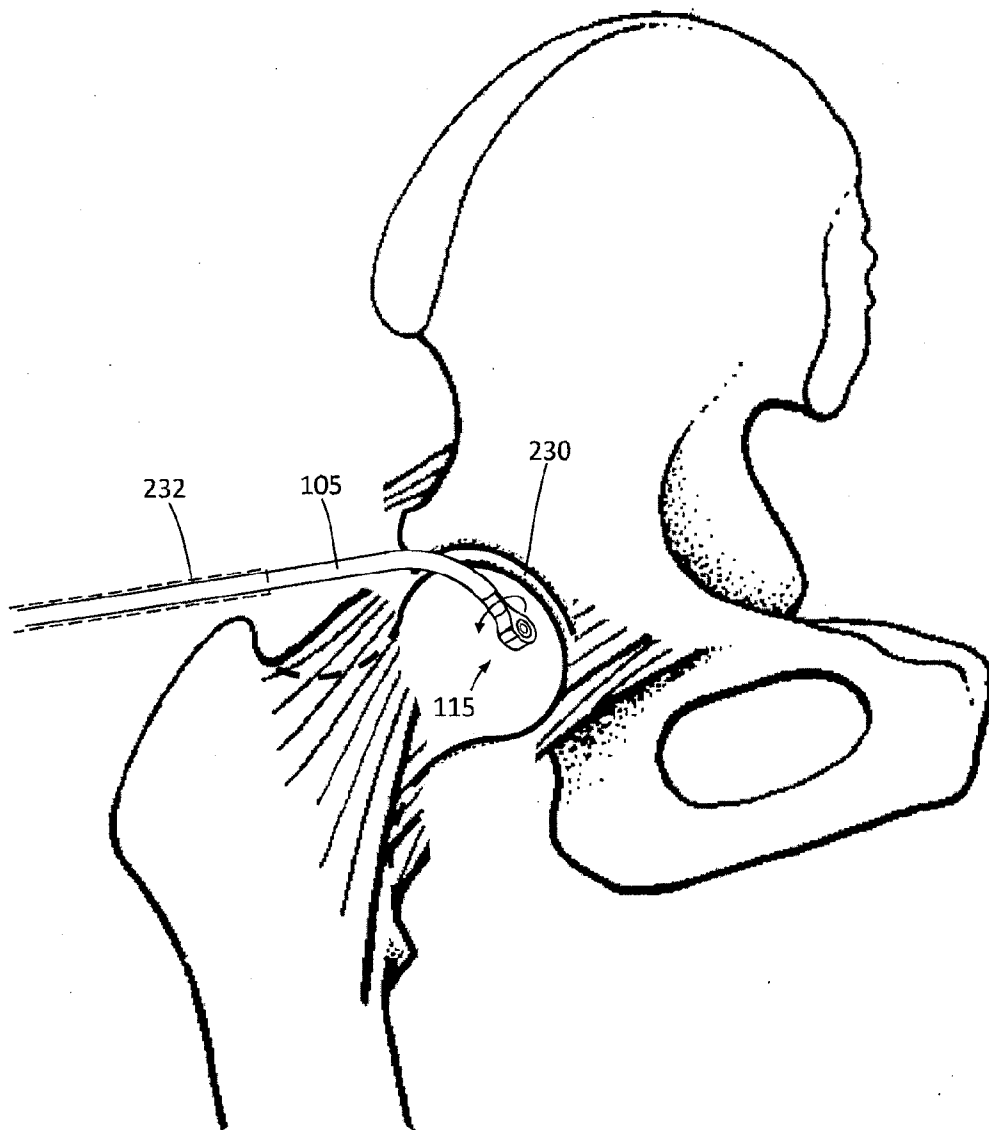


FIG. 10B

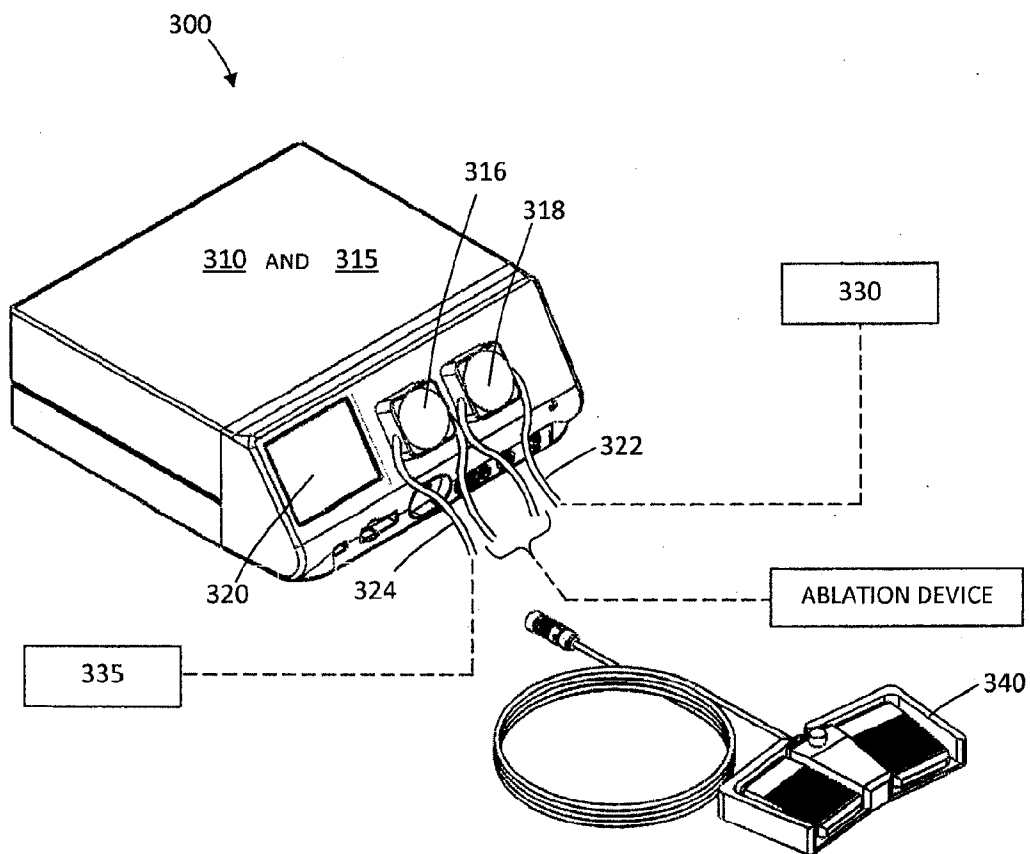


FIG. 11

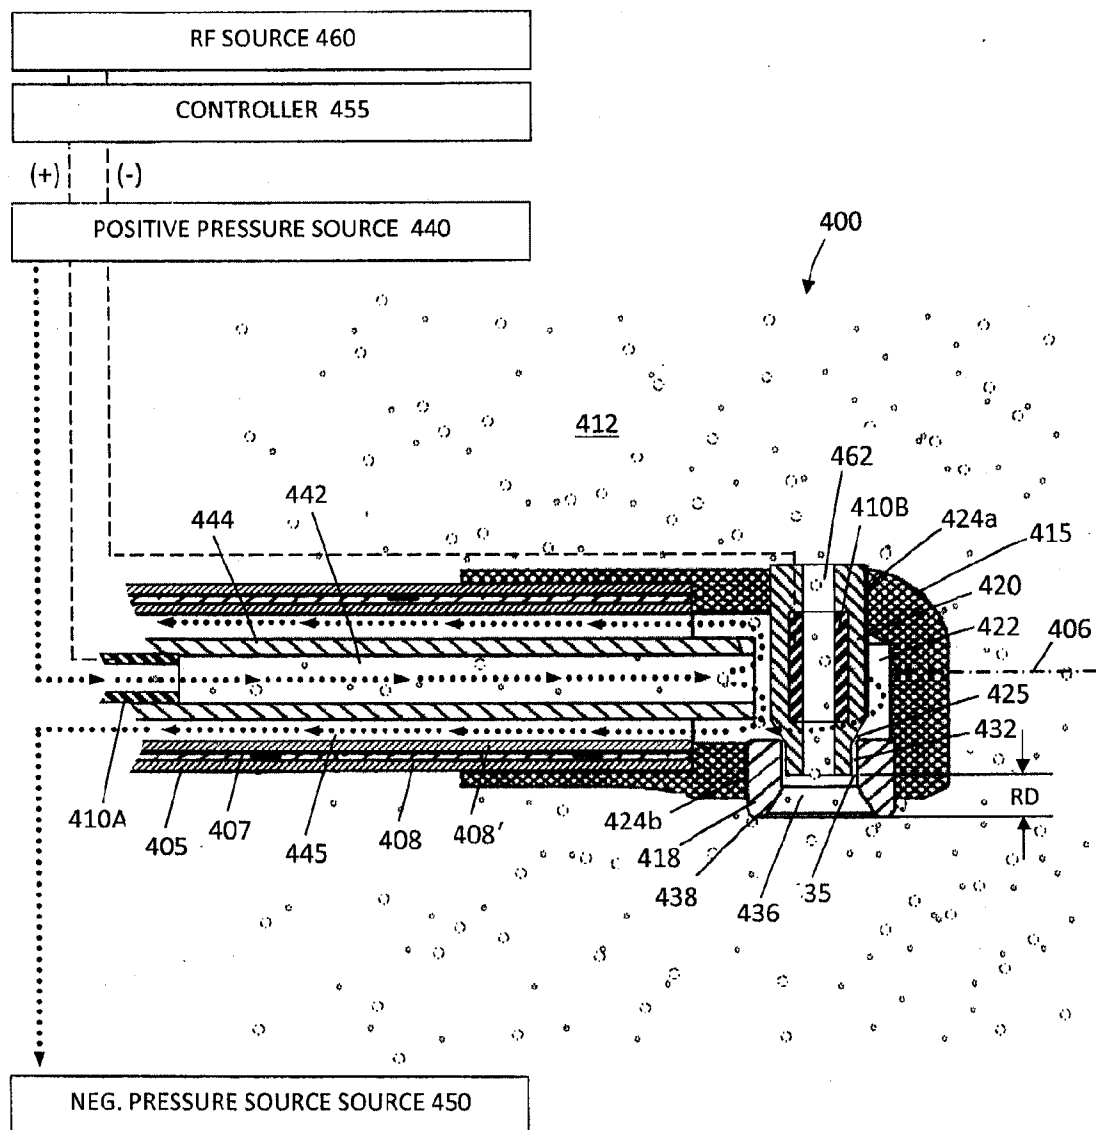


FIG. 12A

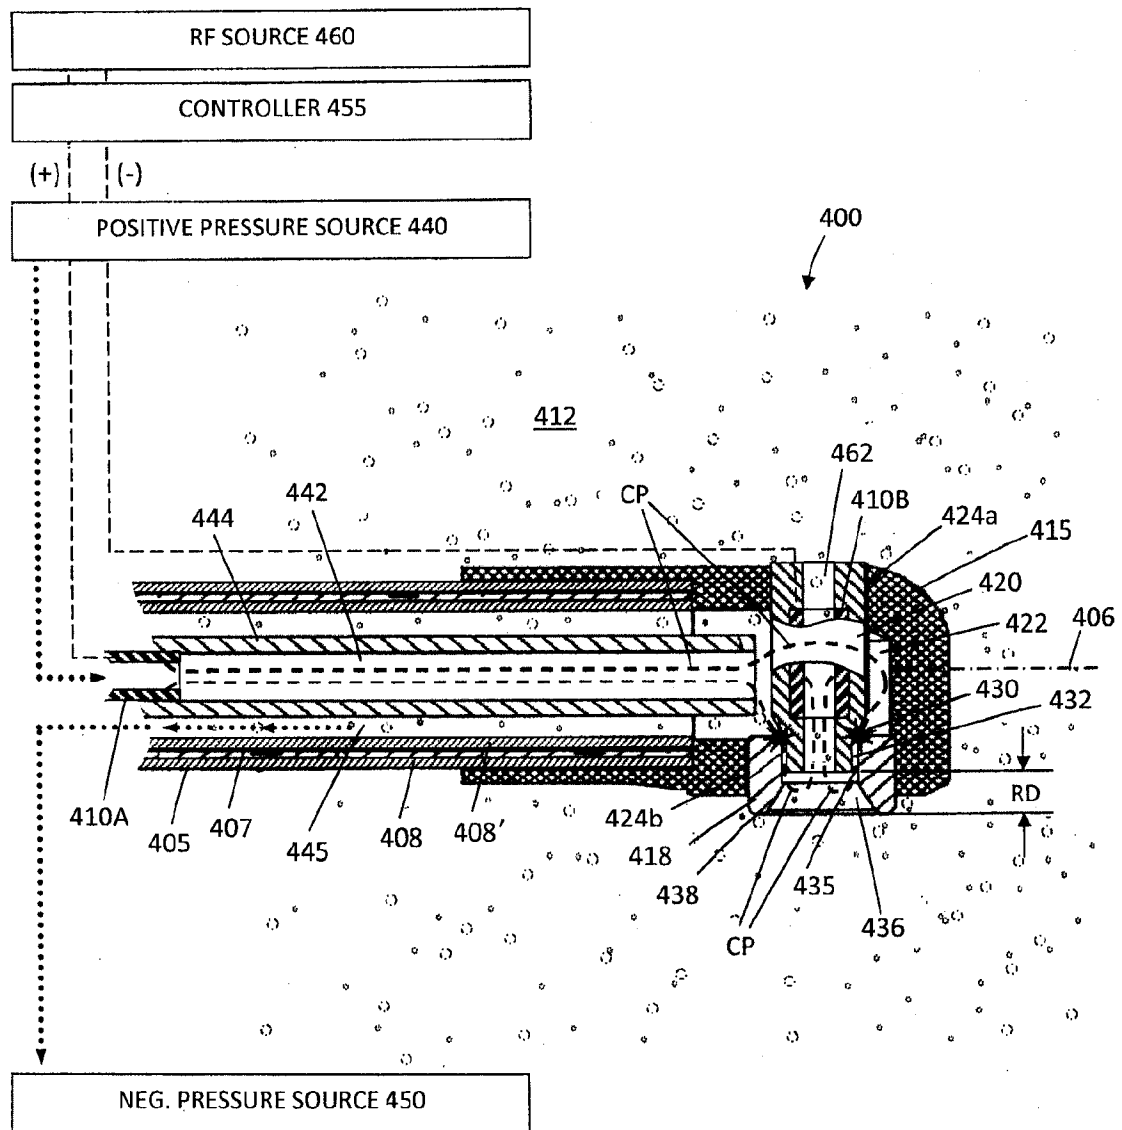


FIG. 12B

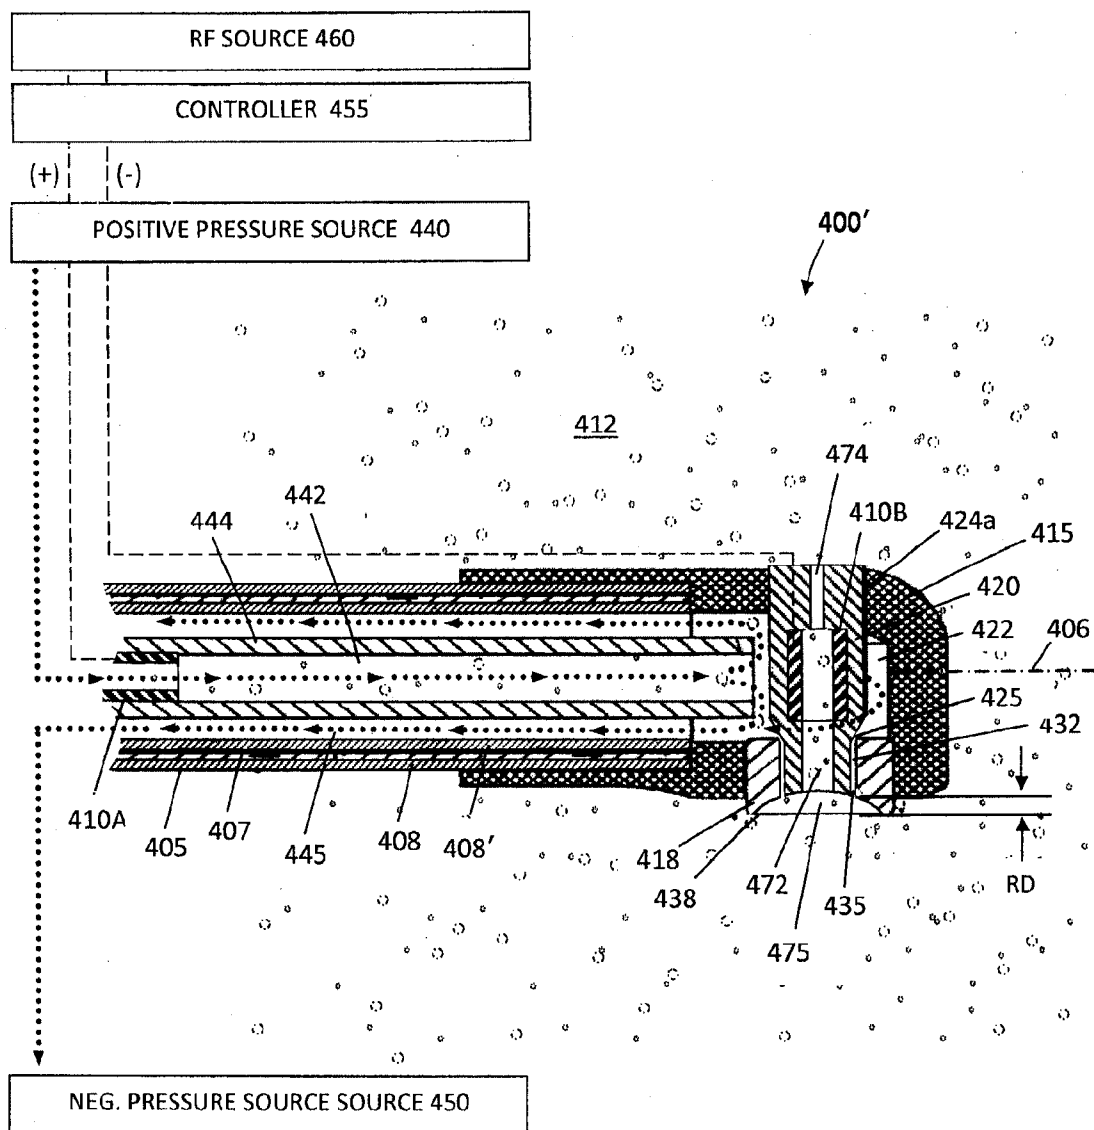


FIG. 13

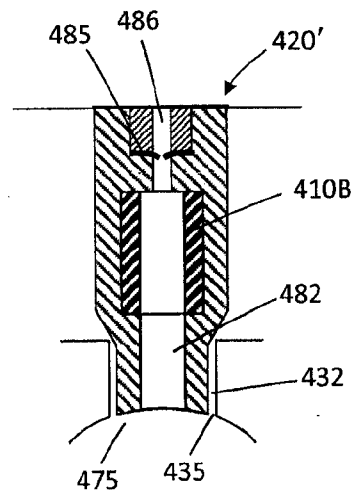


FIG. 14A

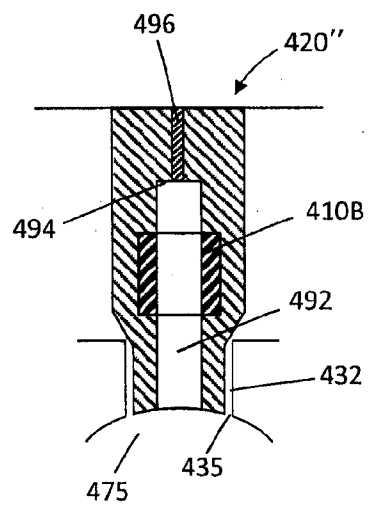
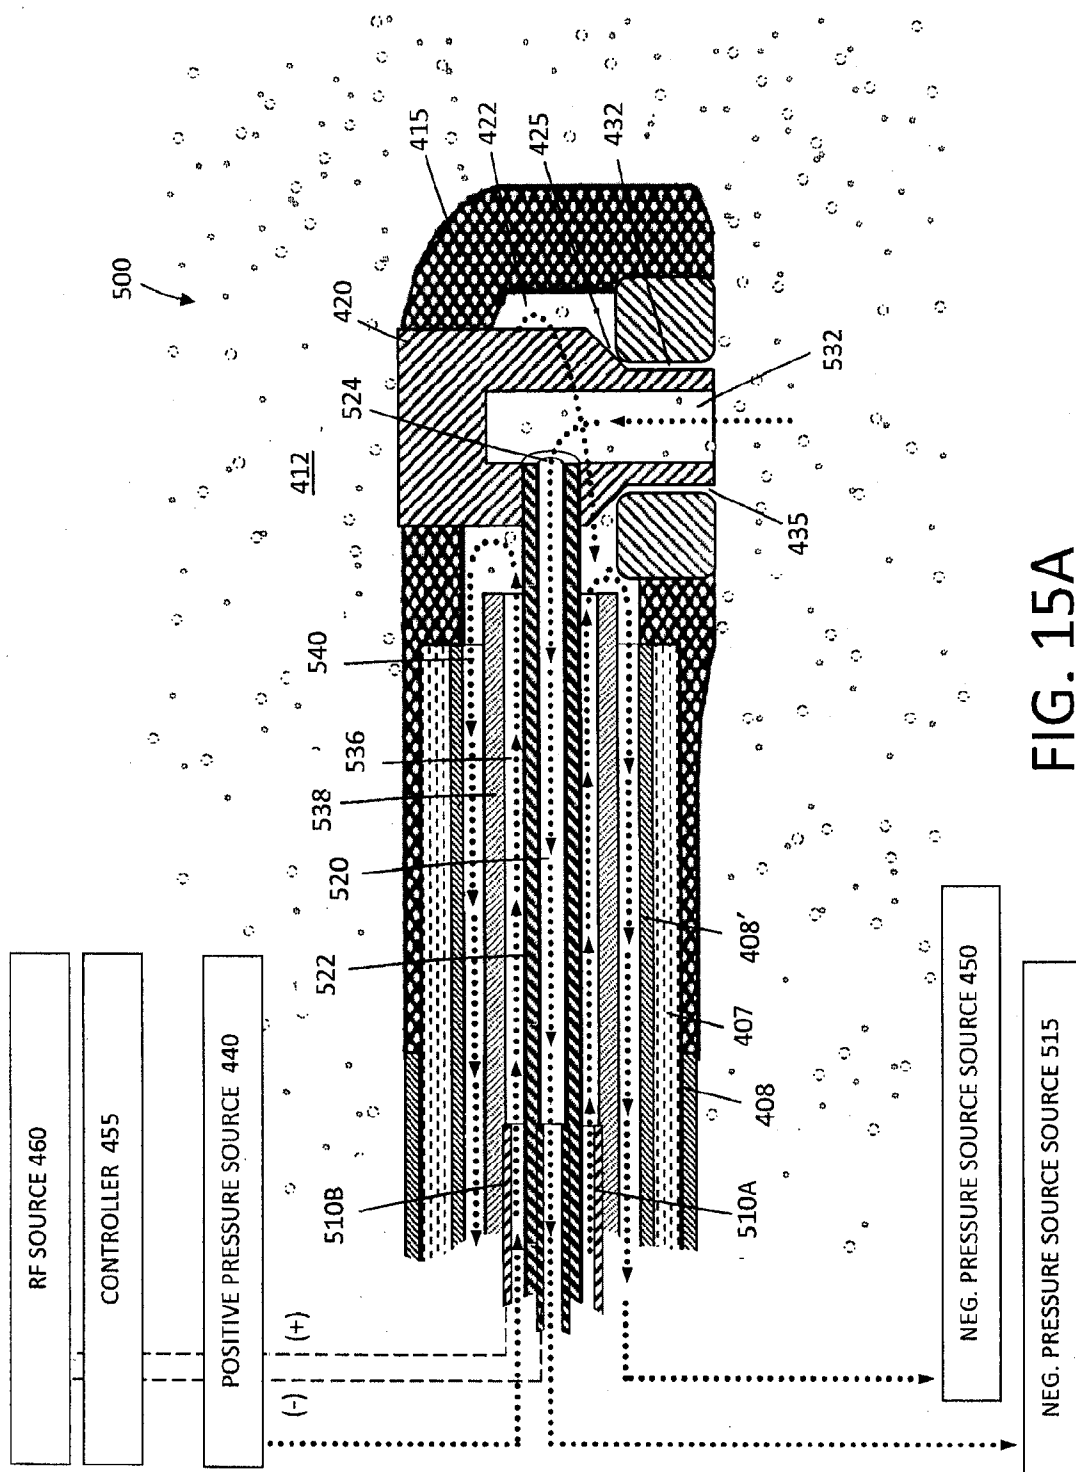


FIG. 14B



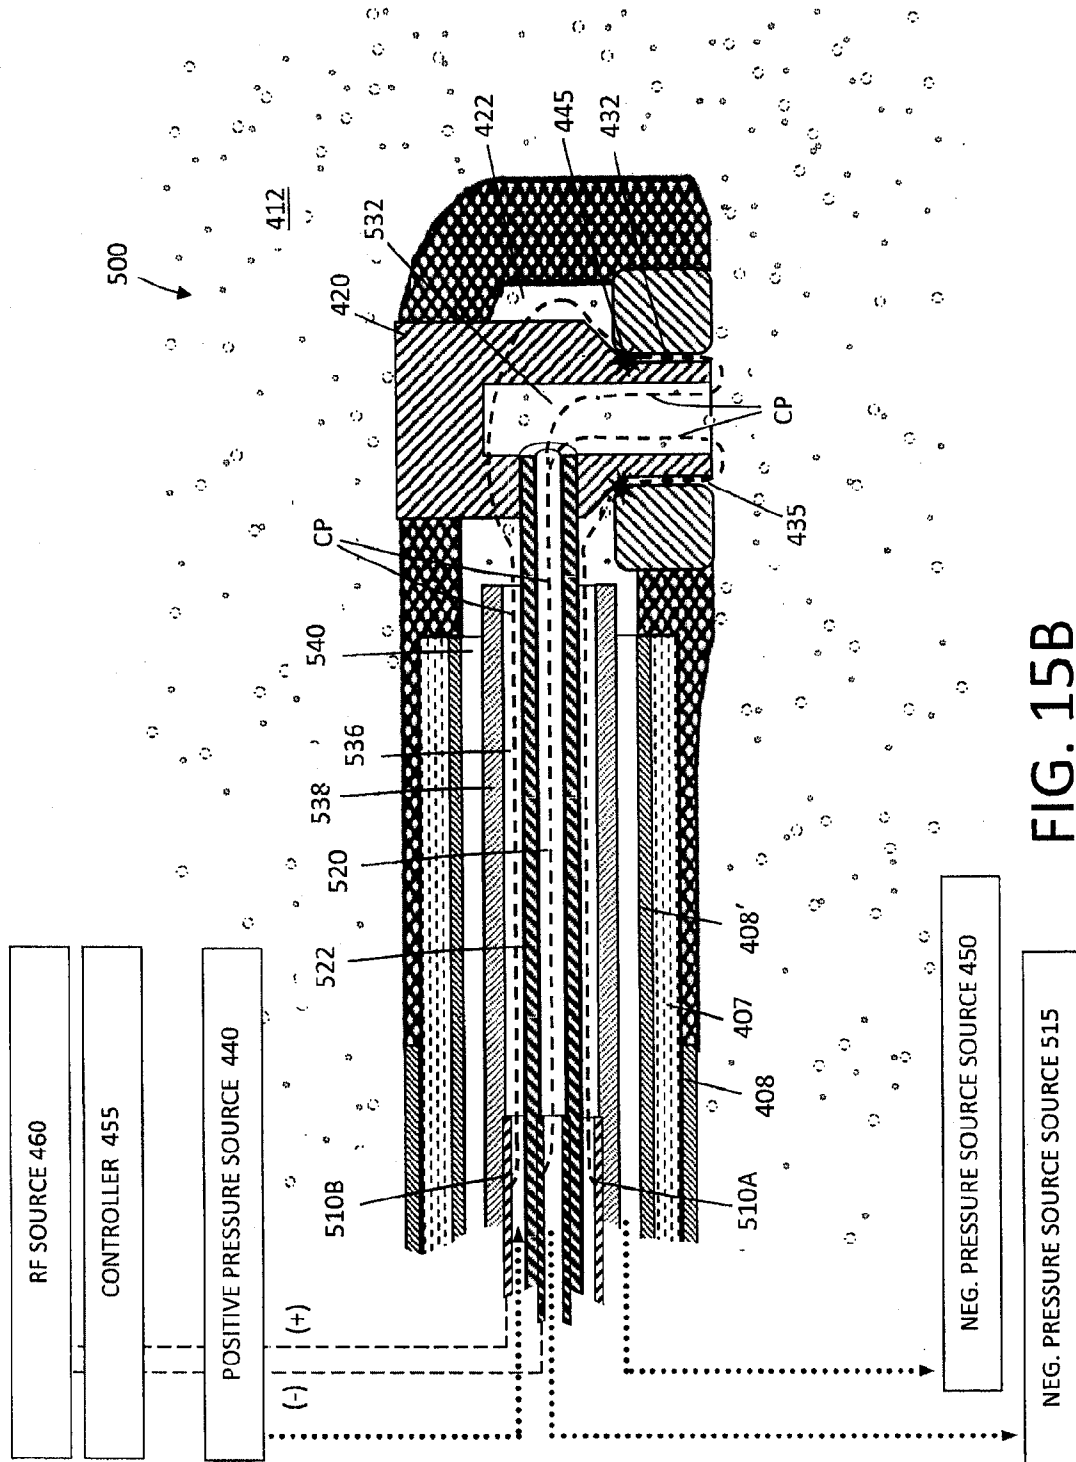


FIG. 15B

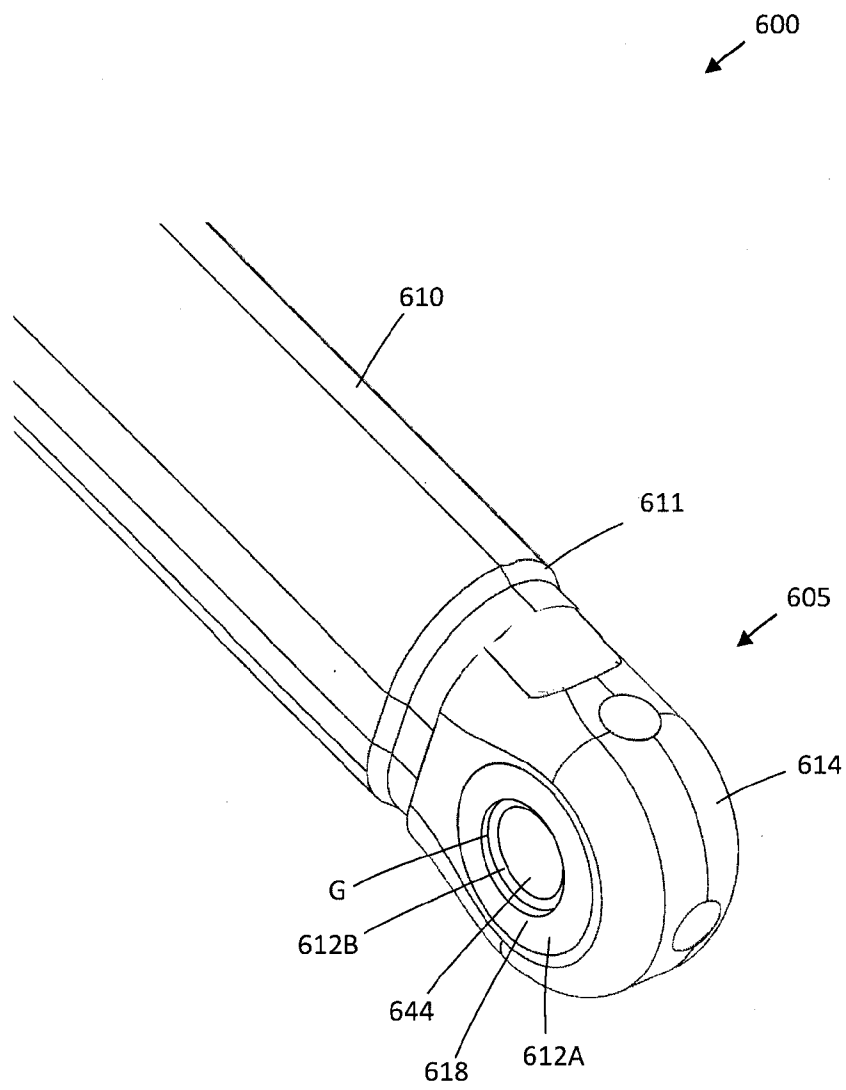


FIG. 16A

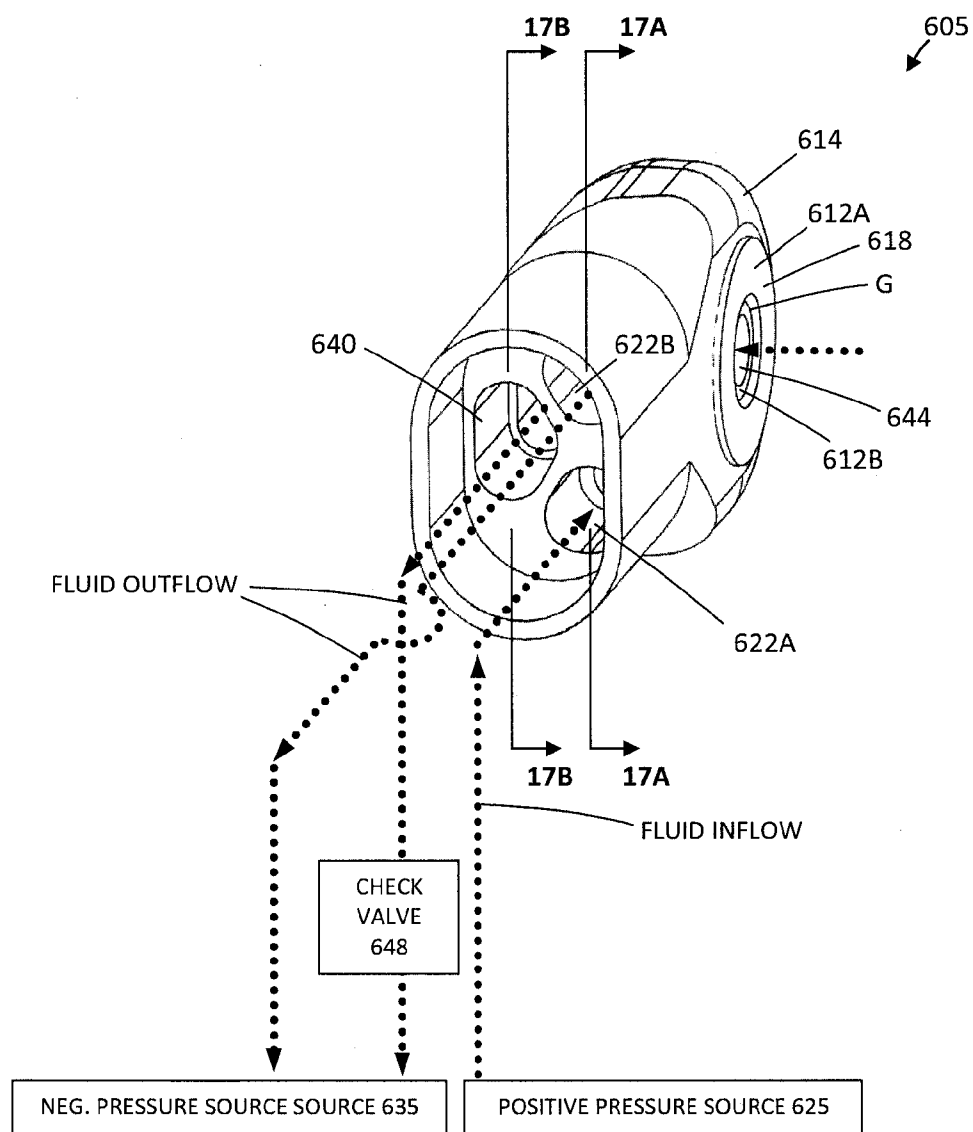


FIG. 16B

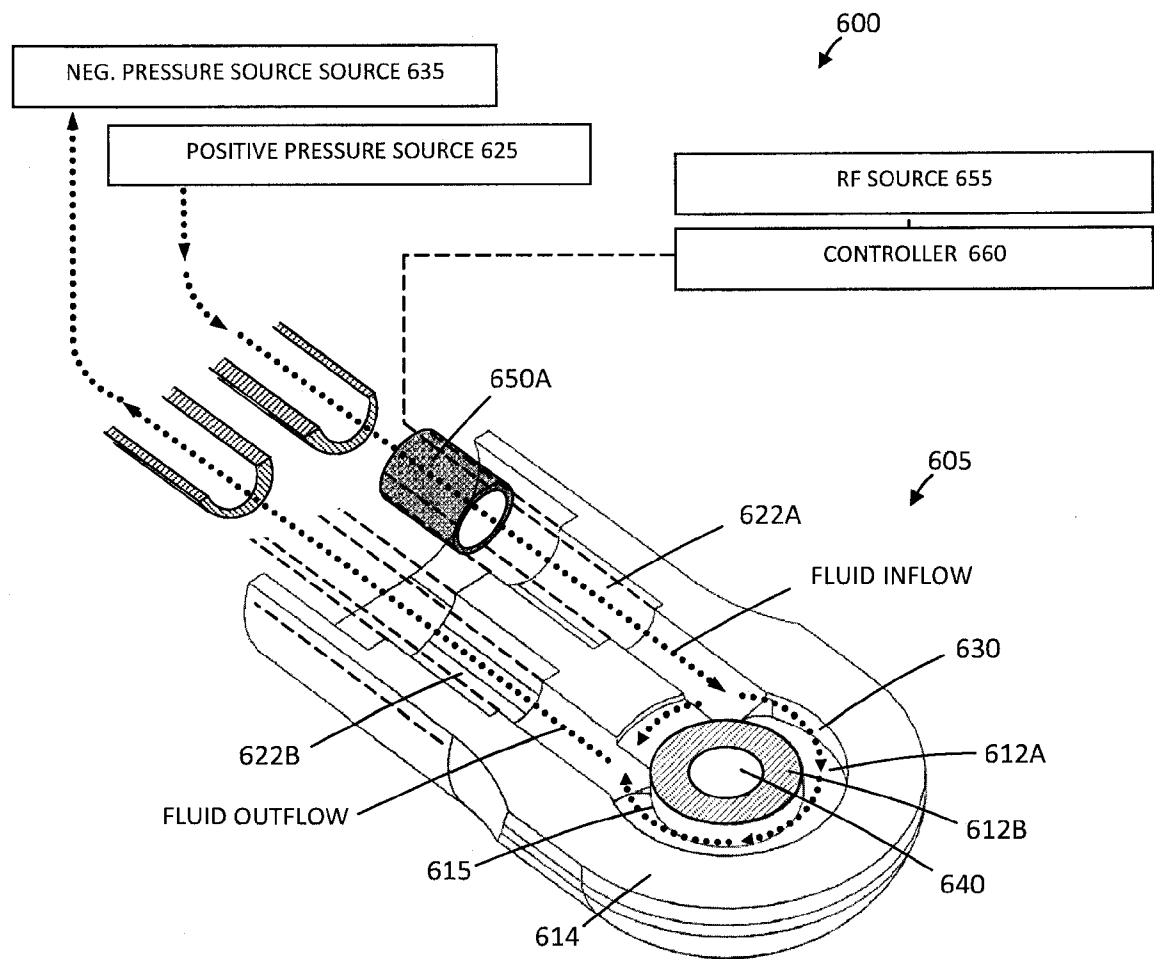


FIG. 17A

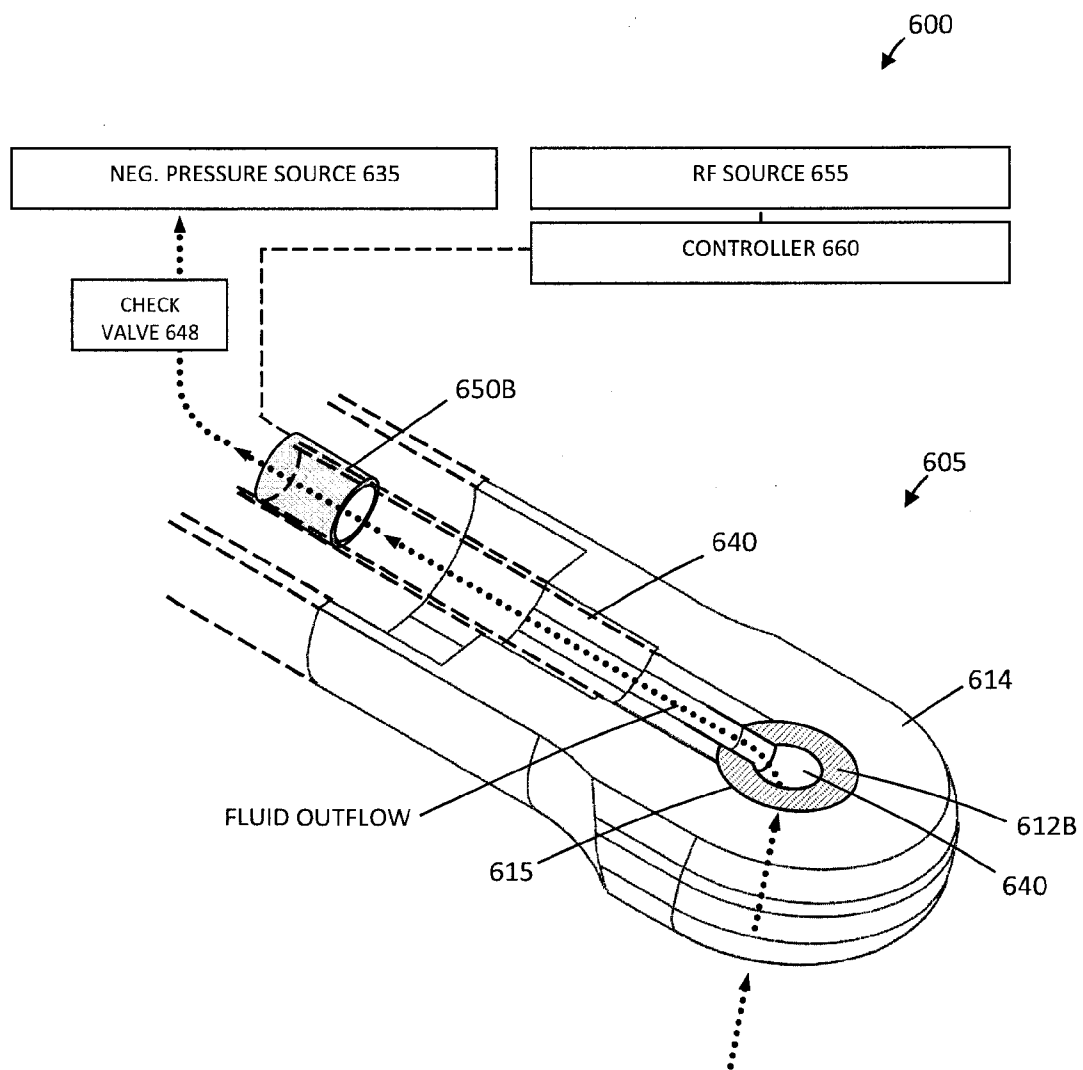


FIG. 17B

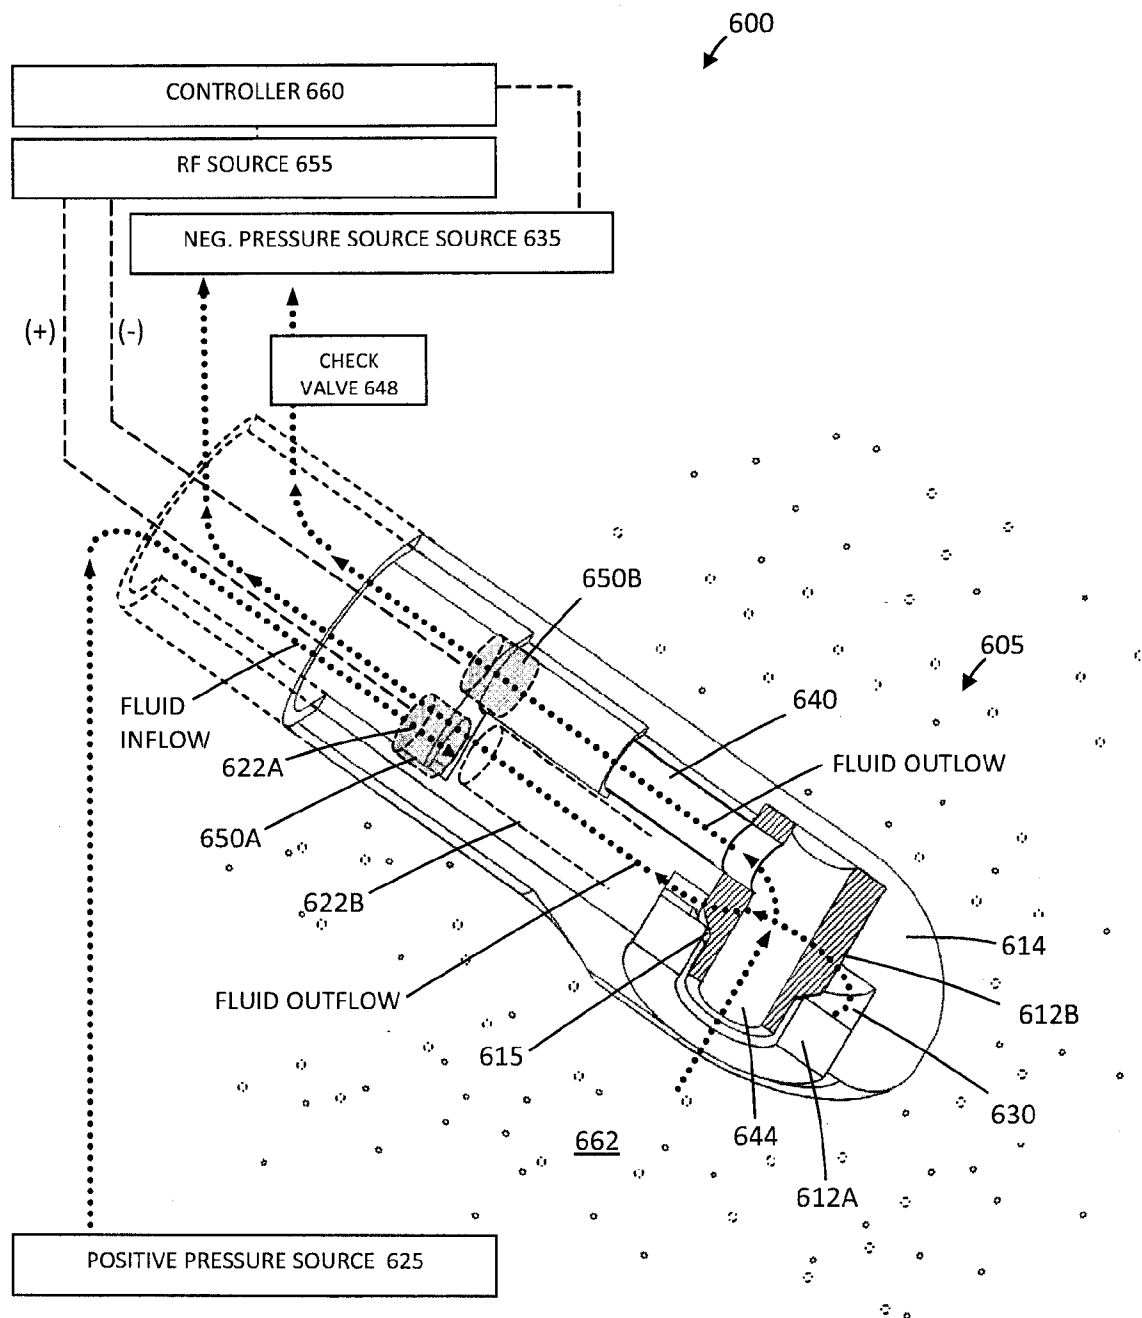


FIG. 18A

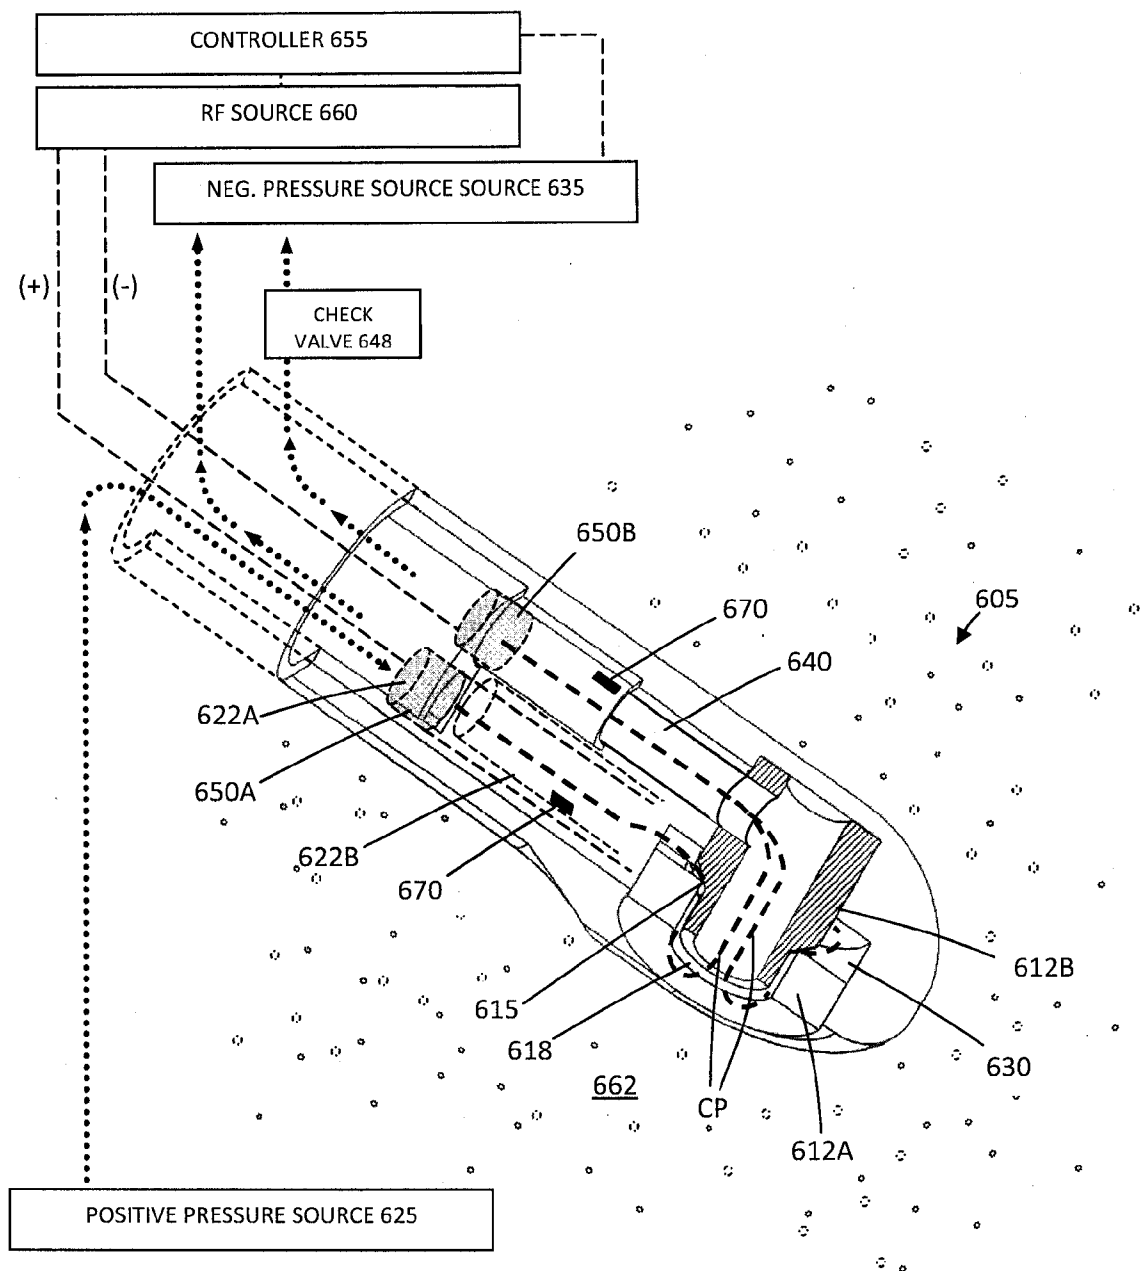


FIG. 18B

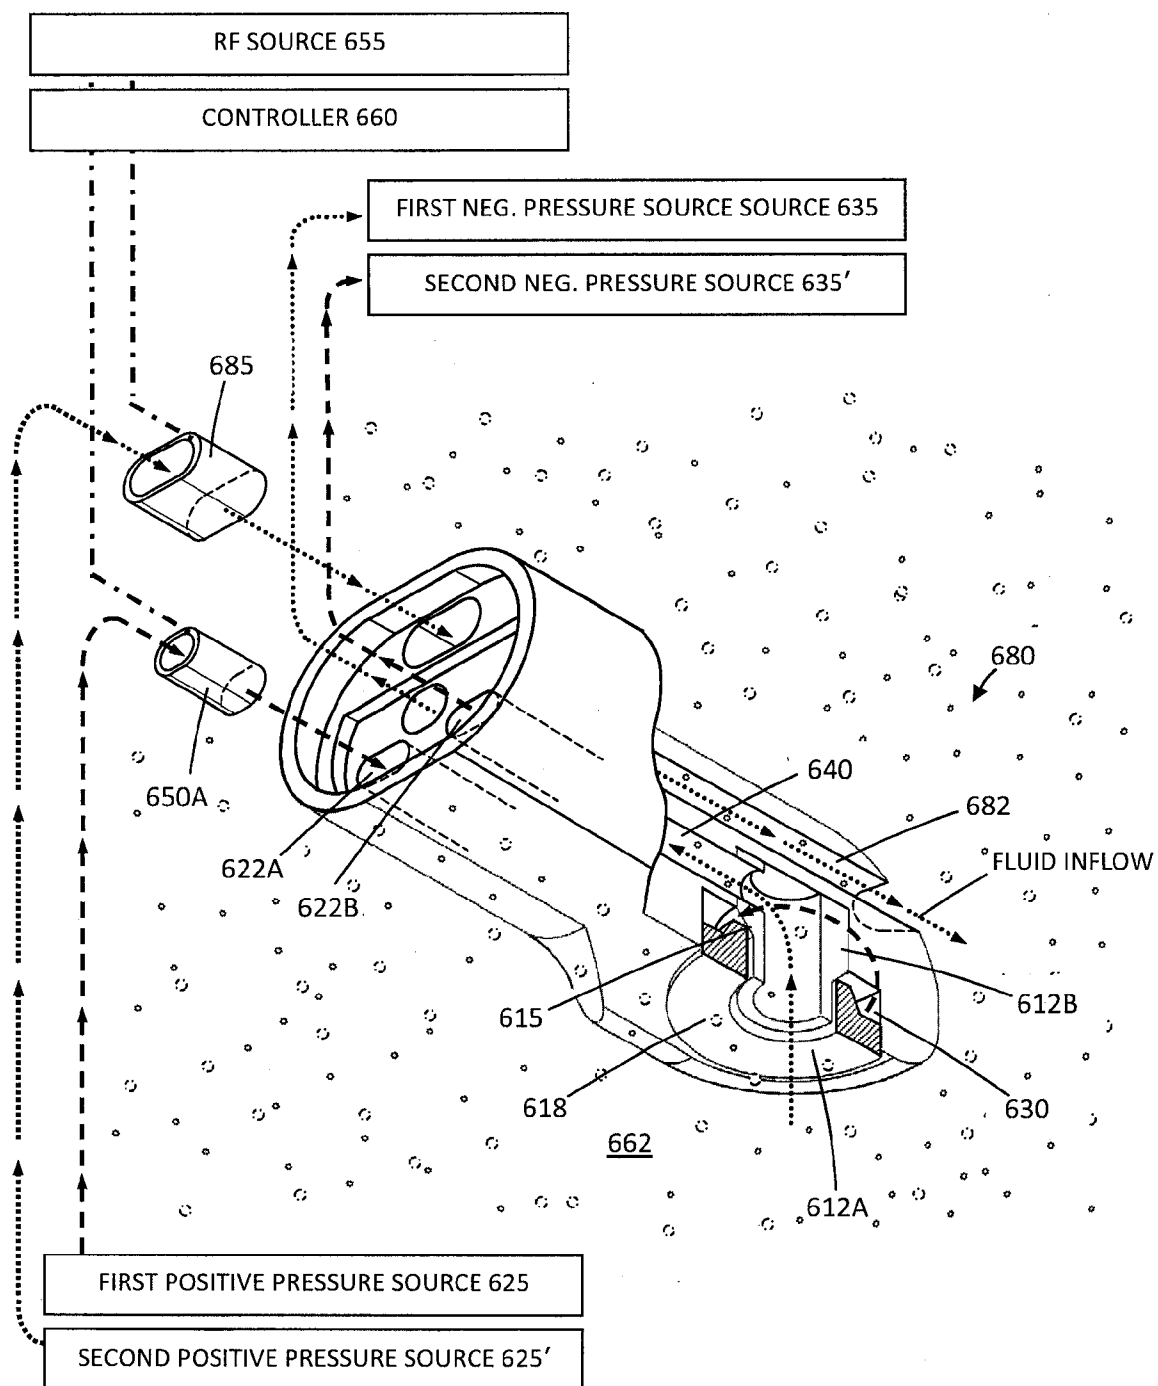


FIG. 19

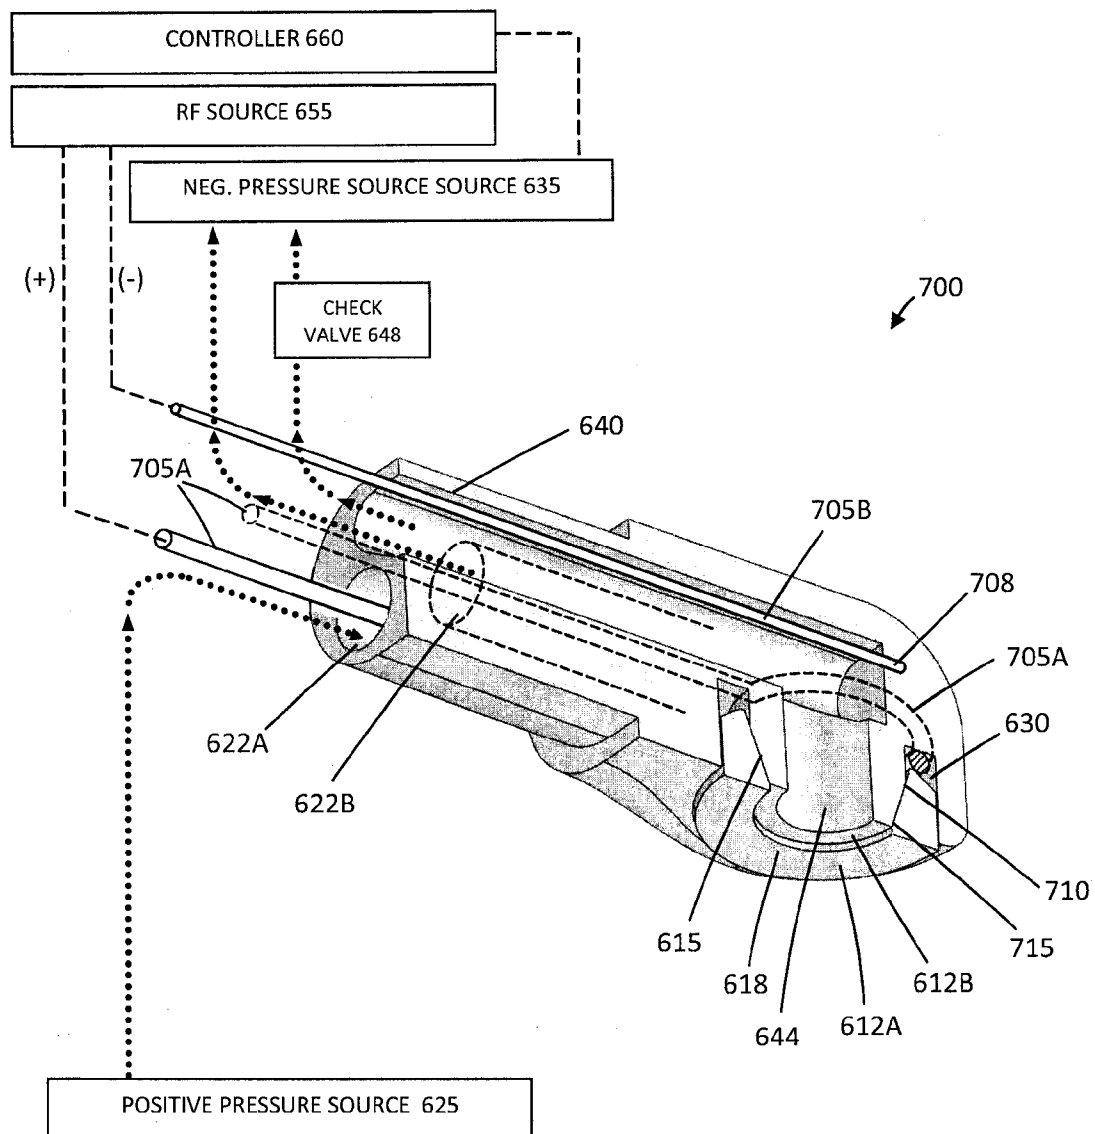
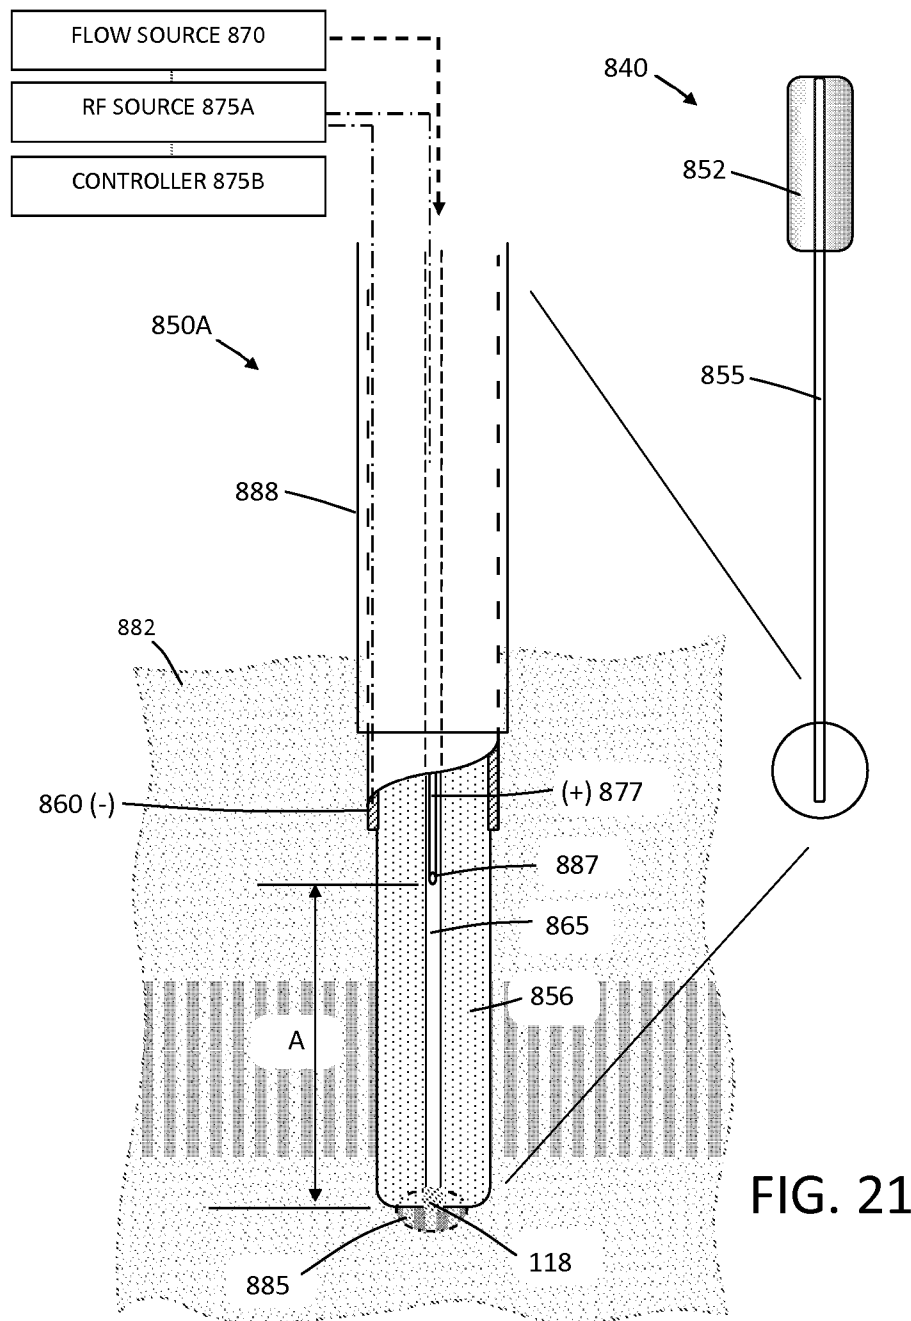
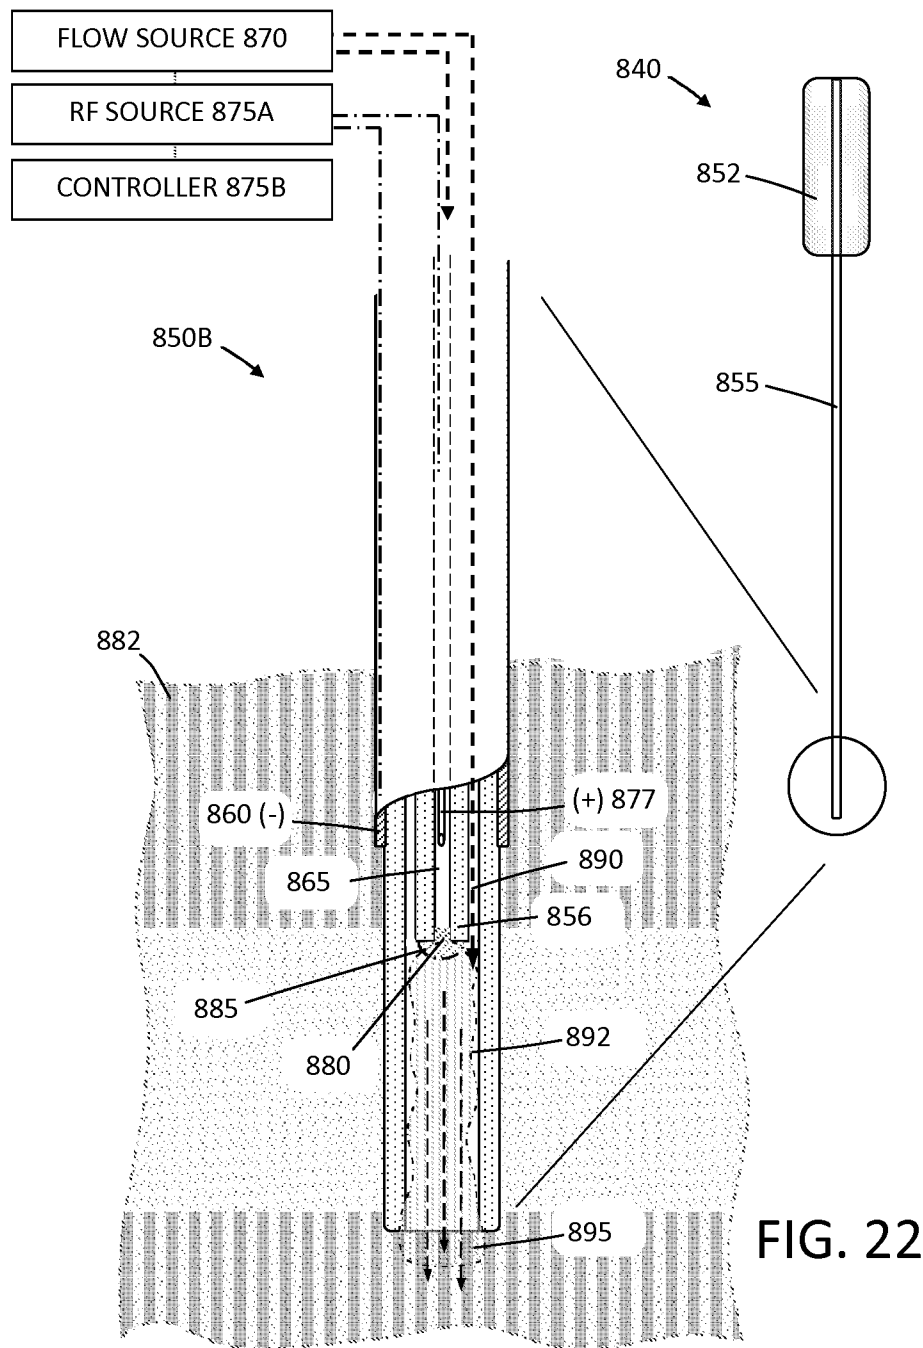


FIG. 20





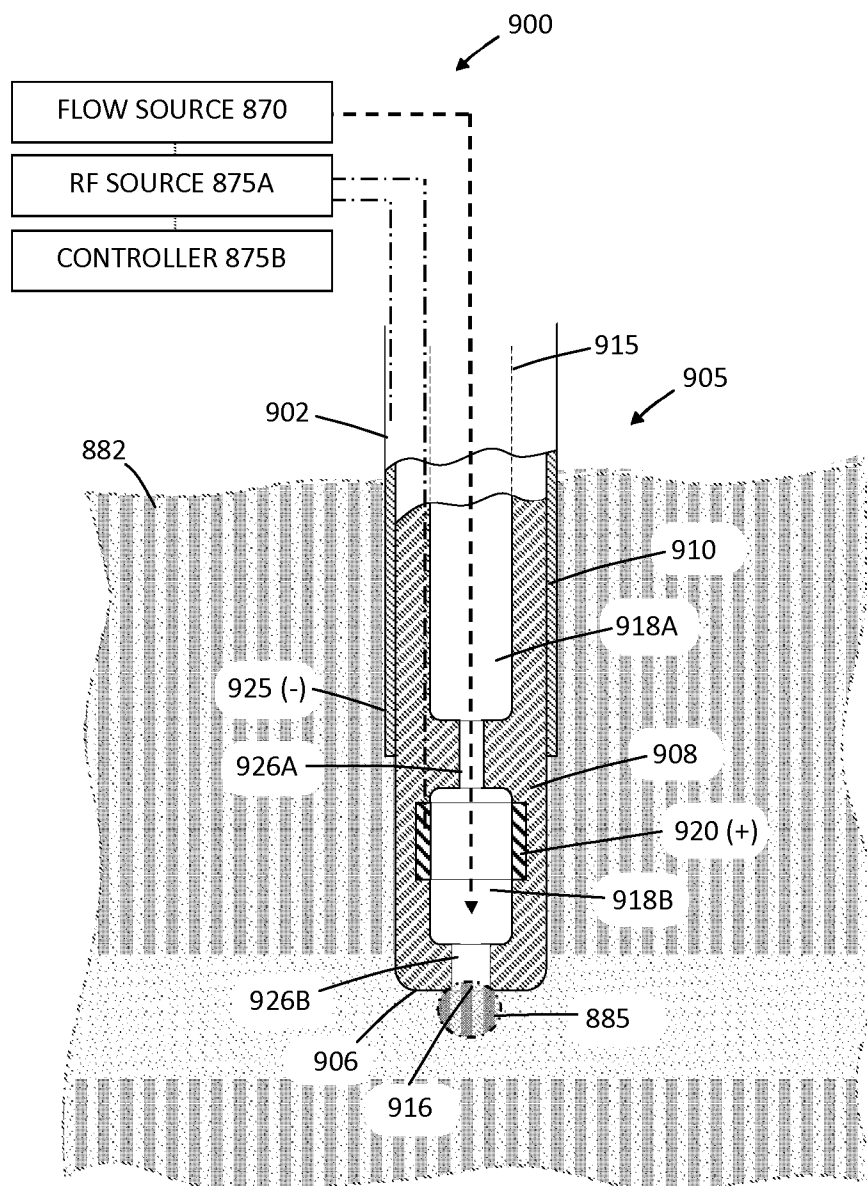


FIG. 23

A. CLASSIFICATION OF SUBJECT MATTER

IPC(8) - A61B 18/18 (2012.01)

USPC - 606/41

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC: A61B 18/18 (2012.01)

USPC: 606/41

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

USPC: 606/41,34,40,32,48

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

PubWest(US PreGrant Pubs; US Patents Fulltext; EPO Abstracts; JPO Abstracts); Google Scholar; Google Patents (Search Terms: Ablation, probe, energy, applicator, channel, positive, pressure, negative, pressure, flow, restrict, restrictor, polarity, electrode, plasma, outflow, fluid)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X - Y	US 2010/0100091 A1 (TRUCKAI) 22 April 2010 (22.04.2010) Fig. 3,12,19; clm 1,4,13,14; para[0078];[0083]-[0090];[0096];[0110]	1-3,7-10,12-31 4-6, 11
X	US 2006/0224154 A1 (SHADDUCK et al) 05 October 2006 (05.10.2006) Fig. 22-23,26; para[0065];[0068];[0082]-[0083];[0085]	32-41
Y	US 2009/0076498 A1 (SAADAT et al) 19 March 2009 (19.03.2009) para[0089];[0097]; Fig. 4A;	4-6,11

☐ Further documents are listed in the continuation of Box C.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

10 May 2012 (10.05.2012)

Date of mailing of the international search report

23 MAY 2012

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US, Commissioner for Patents
P.O. Box 1450, Alexandria, Virginia 22313-1450

Facsimile No. 571-273-3201

Authorized officer:

Lee W. Young

PCT Helpdesk: 571-272-4300

PCT OSP: 571-272-7774