



- (51) International Patent Classification:
A61B 8/08 (2006.01)
- (21) International Application Number:
PCT/US2012/035685
- (22) International Filing Date:
27 April 2012 (27.04.2012)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:

61/479,806	27 April 2011 (27.04.2011)	US
61/500,858	24 June 2011 (24.06.2011)	US
61/504,687	5 July 2011 (05.07.2011)	US
61/532,266	8 September 2011 (08.09.2011)	US

- (72) Inventors; and
- (75) Inventors/Applicants (*for US only*): **PROVOST, Jean** [CA/US]; 223 Avenue B, Apt.3, New York, NY 10009 (US). **LUO, Jianwen** [CN/US]; 344 Fort Washington Avenue, Apt. 5c, New York, NY 10033 (US). **OKRASINSKI, Stanley, J.** [US/US]; 526 W. 112th Street, Apt. 22a, New York, NY 10025 (US). **KONOFAGOU, Elisa, E.** [GR/US]; 101 West End Avenue, Apt. 25g., New York, NY 10023 (US). **THIEBAUT, Stephane** [FR/FR]; 34 Rue Racine, F-92160 Antony (FR). **NGUYEN, Vu, Thanh-hieu** [CH/CH]; Route De Chaffeiru 43, CH-1745 Lentigny (CH).


- (71) Applicant (*for all designated States except US*): **THE TRUSTEES OF COLUMBIA UNIVERSITY IN THE CITY OF NEW YORK** [US/US]; 412 Low Memorial Library, 535 West 116th Street, Mail Code 4308, New York, NY 10027 (US).

- (74) Agents: **CATAN, Mark, A.** et al.; Miles & Stockbridge P.C., 1751 Pinnacle Drive, Suite 500, Mclean, VA 22102-3833 (US).

- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN,

[Continued on next page]

(54) Title: ULTRASOUND IMAGING METHODS, DEVICES, AND SYSTEMS

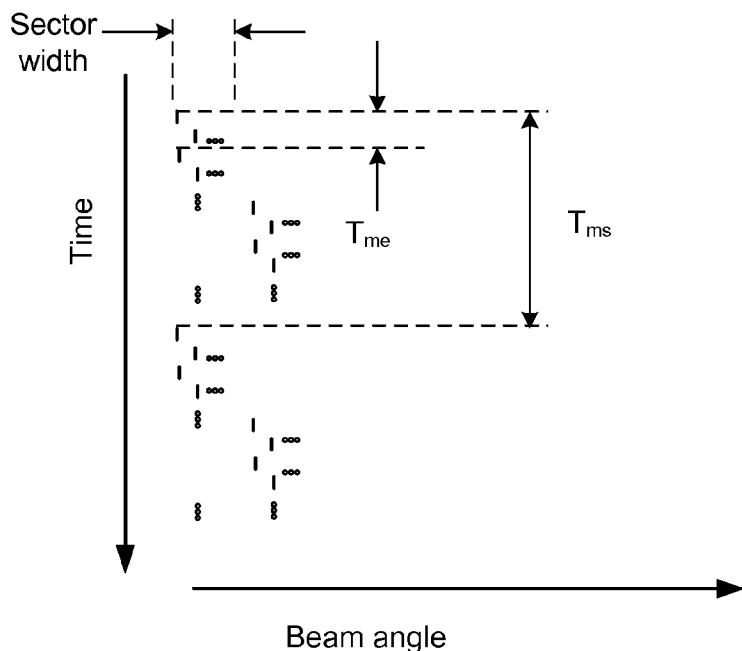

(57) Abstract: Ultrasound methods devices and systems are described which support a useful compromise in terms of spatial resolution and temporal resolution for capturing motion in tissue structures. A particular application is electromechanical wave imaging (EWI).

Fig. 3





HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,

Published:

— without international search report and to be republished upon receipt of that report (Rule 48.2(g))

Ultrasound Imaging Methods, Devices, and Systems

Cross Reference to Related Applications

This application claims the benefit of United States Provisional Applications 61/500,858 filed 24 June 2011; 61/504,687 filed 5 July 2011; 61/532,266 filed 8 September 2011; and 61/479,806 filed 27 April 2011, each of which is hereby incorporated by reference in its entirety herein.

Statement Regarding Federally Sponsored Research

This invention was made with government support under Grant/Contract Nos. R01EB006042 and R21HL096094 awarded by the National Institute of Health (NIH). The government has certain rights in the invention.

Background

Electromechanical Wave Imaging (EWI) is an entirely non-invasive, ultrasound-based imaging method capable of mapping the electromechanical wave (EW) in vivo, i.e., the transient deformations occurring in response to the electrical activation of the heart. Achieving the optimal imaging frame rates necessary to capture the EW in a full-view of the heart poses a technical challenge due to the limitations of conventional imaging sequences, in which the frame rate is low and tied to the imaging parameters. To achieve higher frame rates, EWI is typically performed in multiple small regions of interest acquired over separate heartbeats which are then combined into one view. Yet, the frame rates achieved remain sub-optimal, because they are tied to the imaging parameters rather than being optimized to image the EW. More importantly, the reliance on multiple heartbeats precluded the study from application in non-periodic arrhythmias such as fibrillation.

Summary

The disclosed subject matter relates to the use of ultrasound for extracting spatio-temporal data from living tissue or other moving and/or deforming targets that can be imaged using ultrasound. This includes solid and liquid materials, for example, muscle tissue and blood. In embodiments, the disclosed subject matter, outgoing ultrasound energy is directed according to non-sequential patterns that permit different tradeoffs between temporal and spatial resolution of a target material. For example, an overall frame rate of a scan of an angular region can be reduced in order to generate brief delays between multiple (e.g., 2) scan

lines in a particular, or each, region of a scan which are delayed by a selected interval that is less than the overall frame rate and then using cross correlation of the regions to extract high frequency motion information while obtaining lower rate motion and spatial information from the aggregate of the region scans. Other embodiments produce different tradeoffs.

A temporally-unequispaced acquisition sequence (TUAS) is described for which a wide range of frame rates are achievable independently of the imaging parameters, while maintaining a full view of the heart at high beam density. TUAS is first used to determine the optimal frame rate for EWI in a paced canine heart *in vivo*. The feasibility of performing single-heartbeat EWI during ventricular fibrillation is then demonstrated. These results indicate that EWI can be performed optimally, within a single heartbeat, and implemented in real time for periodic and non-periodic cardiac events. Other applications for high speed imaging, motion estimation, high frame rate imaging, and property determination exist with different emphases on the combination of a need for speed and spatial resolution exist. Spatially unequispaced embodiments are also described.

Objects and advantages of embodiments of the disclosed subject matter will become apparent from the following description when considered in conjunction with the accompanying drawings. The Summary is not intended to summarize all the disclosed or claimed subject matter.

Brief Description of the Drawings

Embodiments will hereinafter be described in detail below with reference to the accompanying drawings, wherein like reference numerals represent like elements. The accompanying drawings have not necessarily been drawn to scale. Where applicable, some features may not be illustrated to assist in the description of underlying features.

Fig. 1A shows a conventional imaging sequence according to the prior art.

Fig. 1B shows a temporally unequispaced sequence according to an embodiment of the disclosed subject matter in which a displacement estimation is done between two RF lines separated by a first time interval and displacement estimations by a second interval that is greater than, and independent of, the first interval.

Fig. 2 shows a comparison of a high strain, high rate interval of an EWI scan for comparing motion estimate at different frame and motion estimation parameters.

Fig. 3 shows a class of TUAS schemes in which a scan is performed sector by sector at intervals chosen responsively to the predicted motion (e.g. strain) rate of change in a target tissue.

Fig. 4 shows a graph of strain distribution as a function of the motion-estimation rate during activation.

Figs. 5A is a plot of expected value of the SNR_e as a function of the motion-estimation rate for five cardiac cycles and during activation.

Fig. 5B is a plot of variance of the SNR_e as a function of the motion-estimation rate for five cardiac cycles and during activation.

Fig. 5C is a plot of probability of obtaining a SNR_e value higher than 3, 5 and 10 as a function of the motion-estimation rate for five cardiac cycles and during activation.

Figs. 6A, 6B, and 6C illustrate embodiments employing, flash or plane wave imaging, which may increase the temporal resolution of displacement estimates in ultrasound scans.

Figs. 7A, 7B, and 7C illustrate embodiments, employing broad transmit beams, which may increase the temporal resolution of displacement estimates in ultrasound scans.

Fig. 8 illustrates embodiments in which multiple focused beams are simultaneously transmitted.

Figs. 9A, 9B, and 9C are for describing apodization function features.

Fig. 10 illustrates axis conventions for describing experiments.

Figs. 11A and 11B describe embodiments for imaging and motion estimation in 1D, 2D, and 3D with features for non-axial motion estimation.

Figs. 12A and 12B describe further embodiments for imaging and motion estimation in 1D, 2D, and 3D with features for non-axial motion estimation.

Fig. 13 illustrates processes for setting up and generating output for TUAS systems.

Fig. 14 figuratively illustrates a TUAS system.

Figs. 15A through 15C illustrate features of output display embodiments where signals received for motion estimation of body structures and fluid flows are combined as enabled by the time resolution of TUAS.

Figs. 16A and 16B illustrate spatially unequipped and temporally unequipped beam embodiments.

Figs. 17A, 17B, and 17C shows alternative variations of the beam layouts of Figs. 11A, 11B, and 12A, 12B for lateral strain estimation in 3D.

Figs. 17D and 17E illustrate a 2D arrangement for lateral strain estimation that was validated by experiment.

Detailed Description of the Embodiments

Electromechanical Wave Imaging (EWI) is a non-invasive ultrasound-based imaging method that can map the transient deformations of the myocardium resulting from local electrical activation, i.e., the electromechanical wave (EW). The EW and electrical activation maps have been shown to be closely correlated, therefore indicating that EWI could become a low-cost, non-invasive, and real-time modality for the characterization of arrhythmias. EWI is a target application for the disclosed technology, but it can be used for other purposes as well. For purposes of describing the technology, EWI will be emphasized, however.

In EWI, inter-frame motion (or, displacement) may be estimated via cross-correlation of consecutive RF frames. From the displacements, the inter-frame strains (or, strains) depicting the EW may be generated by applying gradient operators on the displacement field. However, the heart is an organ that undergoes significant three-dimensional motion and large deformations, which both may lead to decorrelation of the RF signals and thus to the degradation of the motion and deformation estimation accuracy. To overcome this difficulty, the present embodiments adapt the time resolution of the motion estimation. For example the time lapse between frames may be optimized against the need for spatial resolution to prevent decorrelation from compromising the motion estimation. Short intervals covering a short interval may lie below the sensitivity of the motion estimator.

The present application describes validated methods, devices, and systems for capturing high speed motion over a large field of view. In embodiments, accurate motion estimation and anatomy are captured without reliance on cyclical repetition, such as cardiac cycles. Further, in embodiments, the capture is effective for evaluation of electromechanical wave propagation and distinguishing anomalies therein, particularly for the purpose of diagnosis and responsive medical treatment. The non-reliance on cyclical repetition allows the characterization of anomalies like arrhythmia and/or avoiding the need for patients to hold their breath during multiple cardiac cycles.

EWI maps the transient inter-frame strains (referred to here as 'strains' for brevity) occurring in the vicinity of the electrical activation of the heart. At the tissue level, the depolarization of myocardial regions triggers the electromechanical activation, i.e., the first time, at which the muscle transitions from a relaxation to a contraction state. Spatially, this electromechanical activation forms the EW front that follows the propagation pattern of the electrical activation sequence.

In embodiments, temporally-unequispaced acquisition sequence (TUAS) is used to acquire images of muscle deformation such as EW. In embodiments, TUAS employs sector-based sequence adapted to optimally estimate cardiac deformations. The TUAS was verified

by an embodiment implemented on a conventional clinical ultrasound scanner. The embodiments of TUAS cover the simultaneous provision of a wide range of frame rates for motion estimation, high beam density for high resolution, and a large field of view in a single motion cycle, e.g., heartbeat. For a given set of imaging parameters, motion can be estimated at frame rates varying from a few Hz to kHz. To achieve this, the sampling rate of the motion estimation is reduced, as shown, such that there is little effect on the accuracy of EW maps. This is accomplished, in embodiments, by maintaining the sampling rate above a threshold selected for the target motion information.

In the TUAS embodiments, a wide range of frame rates can be achieved, including very high frame rates, independently of other imaging parameters. By maintaining a set of imaging parameters (e.g., field of view, imaging depth), the frame rate is selected responsively to the elastographic signal-to-noise ratio (SNR_e) and the EW. A probabilistic framework based on experimental data, acquired in a paced canine *in vivo*, was used to establish the technique for selecting an optimal frame rate. The single- heartbeat EWI at the optimal frame rate was used to study the electromechanical activity of fibrillation, a non-periodic arrhythmia.

In the study, which was approved by the Institutional Animal Care and Use Committee of Columbia University, a male mongrel dog, 18 kg in weight, was anesthetized with an intravenous injection of Diazepam 0.5- 1.0mg/kg IV as premedication, and Methohexital 4-11mg/kg IV as induction anesthetic. It was mechanically ventilated with a rate- and volume-regulated ventilator on a mixture of oxygen and titrated isoflurane (0.5%–5.0%). Morphine (0.15 mg/kg, epidural) was administered before surgery, and lidocaine (50 micrograms/kg/h, intravenous) was used during the entire procedure.

To maintain blood volume, 0.9% saline solution was administered intravenously at 5 mL/kg/h. Standard limb leads were placed for surface electrocardiogram (ECG) monitoring. Oxygen saturation of the blood and peripheral blood pressure were monitored throughout the experiment. The chest was opened by lateral thoracotomy using electrocautery. Three pacing electrodes were sutured at the basal region of the lateral wall, at the left ventricular apex and at the right ventricular apex. Only one pacing electrode, located at the basal region of the lateral wall, was used to pace the heart in certain evaluation experiments. RF ablation of the left bundle branch was performed under fluoroscopy and a basket catheter (Boston Scientific, Natick, MA) was introduced in the left ventricle for the purpose of another study.

The motion-estimation rate r_{me} is defined as the inverse of the time, i.e., T_{me} , lapsing between the two RF frames used to estimate motion. The motion-sampling rate r_{ms} is defined

as the inverse of the time, i.e., T_{ms} , lapsing between two consecutive displacement maps. In conventional imaging sequences, these two rates are equal, because a given frame is typically used for two motion estimations. Commonly an ultrasound image is constructed using a phased array to acquire a number of beams, typically 64 or 128, over a 90° angle. Fig. 1A illustrates the conventional scheme showing a simplified scheme with only a few beams repeated over two cycles for purpose of discussion. In Fig. 1A, the beams are acquired sequentially, and the process is repeated for each frame with each frame separated by an interval $T_{me} = T_{ms}$. The motion estimation interval (T_{me}) is defined as the inverse of the inter frame rate used to estimate motion, whereas the motion sampling interval (T_{ms}) is defined as the inverse of the displacement frame rate. That is, full frames are obtained and the motion estimated by cross-correlation of the images using known techniques. For example, a given beam angle will be repeated at a fixed interval $T_{me} = T_{ms}$.

In some TUAS embodiments, the motion-estimation rate and the motion-sampling rate are different so that $T_{me} \neq T_{ms}$. In TUAS, the motion-estimation rate is selected independently of the sampling rate. As shown in Fig. 1B, only a fraction of the entire frame is scanned before the fraction is scanned again so that a fractional sector of the full 90 degree frame is scanned twice before the next sector (in the illustration there are only two beams at respective angles per a sector). A frame in the TUAS case provides motion estimation, thus drastically reducing the motion-sampling interval relative to the conventional method and thereby increasing the temporal resolution used for motion estimation. In the TUAS embodiments similar to that of Fig. 1B, the number of angles per sector can be varied to generate different ratios of T_{me} to T_{ms} .

An acquisition performed at a 12-cm-depth with 64 beams with a conventional sequence may correspond to a frame rate of 100 Hz. However, while 100 Hz may suffice to satisfy the Nyquist sampling criterion of cardiac motion, it is, as described below, insufficient for accurate motion tracking using RF cross-correlation. Therefore, to reach a higher frame rate of, e.g., 400 Hz typically used for EWI, the conventional approach would be to divide the number of beams by four, and thereby reduce either the lateral resolution, the field of view, or both. At the same depth and beam density, TUAS provides a motion-sampling rate of 50 Hz and a motion-estimation rate that can be varied, as shown in the following section, within the following group: {6416, 3208, 1604, 802, 401, 201, 100} Hz. This has numerous advantages. For example, both the lateral resolution and the field of view can be maintained while estimating the cardiac motion with an optimal frame rate, which could be, for example, 401 or 802 Hz, depending on the amplitude of the cardiac motion. This results in a halving of

the motion-sampling rate. However, the motion-sampling rate has little effect on the motion estimation accuracy. If this rate remains above the Nyquist rate of the estimated cardiac motion, this will have no effect.

To estimate the effects of the motion-sampling rate on the accuracy of the motion estimation, RF data acquired over multiple heartbeats at 480 Hz from a previous study was decimated to vary the motion-estimation and motion-sampling rates. At the scale of the full cardiac cycle, both rates have little influence on the general trend of the displacements but as shown in Fig. 2, during fast transients deformations, e.g., during the electrical activation, larger differences were observed. These larger differences also correspond to higher strain values than e.g., during end-systole. For a fixed motion-sampling rate, dividing the motion-estimation rate by four leads to an error of approximately 100% in the displacements. However, when dividing the motion-sampling rate by four while maintaining a high motion-estimation rate, only a small variations are observed in the incremental displacements. From experiments, it is estimated that at a motion-sampling rate above 120 Hz, the significance of the motion-sampling rate became negligible compared to the effect of the motion-estimation rate.

In a conventional imaging sequence, two consecutive frames with N beams per frame are acquired beam by beam in sequence resulting in a time between two frames of $2dN/c$, where d is the imaging depth, N is the number of beams in the image, and c is the speed of sound. Motion is then estimated between the two consecutive acquisitions of beams at the same location. For example, motion is estimated through the cross-correlation of beam 1 acquired at time 1 and beam 1 acquired at time $N+1$. Therefore, identical motion estimation and motion sampling rates are obtained, equal to $c(2dN)^{-1}$.

TUAS was implemented in an open-architecture Ultrasonix MDP system (Ultrasonix Corp, Burnaby, BC, Canada) using the Texo Software Development Kit. In TUAS, the beams constituting two frames are acquired in a different order. Beams are acquired consecutively within sectors containing k beams, and then repeated. In Fig. 3 the k beams may be repeated twice for two sector-sized mini-frames for motion estimation. Alternatively, there may be more than two sector-sized mini-frames to obtain two inter-mini frame motion estimates which may be stored separately with respective times or averaged to form a single motion estimate for the sector. The number of beams comprising a sector is labeled “sector width” (angular spacing of adjacent beams multiplied by the number of beams per sector k) assuming a regular spacing of the beams in a sector. The time interval between mini-frames of a single sector is indicated as T_{me} . The time interval between frames of the entire regular frame is

indicated as T_{ms} . Note that the beams per sector can be varied between sectors or the spacing between beams in a sector or among different sectors can be different. Note that k can be equal to one up to a fraction of the total beams per global frame.

Axial motion is estimated between two beams acquired consecutively at the same location, which results in a motion estimation rate of $c(2dk)^{-1}$. Since k needs to be a divisor of N , i.e., $\text{div}(N)$, the group of available motion-estimation rates for a given number of beams is given by $c(2d)^{-1}\{(\text{div}(N))^{-1}\}$. The highest motion estimation rate occurs at $k = 1$, i.e., $c(2d)^{-1}$, and the lowest motion estimation rate occurs at $k = N$, and is equal to that of a conventional imaging sequence, i.e., $c(2dN)^{-1}$. If motion is estimated only between the two closest acquisitions of the same beam in time, the motion-sampling rate is $c(4dN)^{-1}$. Note that in addition to motion being estimated between beams separated by T_{me} , lower motion-estimation rates can also be achieved by estimating motion between beams separated by $T_{ms} - T_{me}$ (See Figs. 1A, 1B, and Fig. 3 and attending discussion), corresponding to a motion-estimation rate of $c(2d(N-k))^{-1}$, in which case the motion-sampling rate would be $c(2dN)^{-1}$.

A 3.3-MHz phased array was used to image the myocardium *in vivo*. Axial displacements were estimated using a 1D cross correlation algorithm using RF signals sampled at 20 MHz. The window size used was 4.60 mm and the overlap 90%. The heart was segmented using an automated contour tracking technique. The incremental axial strains were estimated with a least-squares method and a kernel size of 10.7 mm. Images were acquired at different motion-estimation rates, i.e., {41, 82, 163, 350, 452, 855, 1100, 1283, 1540} Hz and their corresponding motion-sampling rates {163, 163, 163, 163, 211, 132, 128, 119, 119} at a 10-cm depth.

To assess the accuracy of a strain measurement, the SNR_e was used, which is defined as:

$$SNR_e = \frac{\mu}{\sigma}, \quad (1)$$

where μ is the local average of strains ε at a given time, and σ the corresponding standard deviation. In experiments, the SNR_e at different motion-estimation rates was computed by averaging and calculating the standard deviation of the incremental strains within an axial window of 4.85 mm for individual pixels over multiple frames, corresponding to up to 5 heart cycles, after segmenting the heart. This provides the SNR_e as a function of space and time, $SNR_e(x,y,t)$ where x and y are the lateral and axial directions, respectively and t is the time. Previous literature on the strain-filter indicates that the SNR_e will depend mostly on the value of the strains to be measured, when the imaging parameters are fixed. This theoretical

framework allows the construction of an upper limit on the SNR_e as a function of the strain amplitude (a.k.a., the strain-filter). The strain filter corresponds, in this case, to the Ziv-Zakai Lower Bound (ZZLB) on the variance. The ZZLB is a combination of the Cramér-Rao Lower Bound (CRLB) and the Barankin bound (BB). The ZZLB transitions from the CRLB to the BB when decorrelation becomes important to the point that only the envelope of the signal contains information on the motion. In the correlation model used here, this transition occurs only at very large strains. The strain filter was adapted to the imaging parameters used in this study as a reference. For that purpose, the RF data SNR of 1500 (60 dB) was assumed, similar to what was previously considered in prior literature. Such a high value is justified since acquisition was performed in an open-chest setting.

The motion-estimation rate is directly linked to the strain distribution in the heart. Consider the cumulative strain function at a given point (x_o, y_o) , $e(x_o, y_o, t) = e(t)$. Then, the strain at a time t_0 can be defined as

$$\varepsilon(t_0) = e(t_0 + T_{me}) - e(t_0) \quad (2)$$

When expanding $e(t)$ in Taylor series around t_0 , the result is

$$\begin{aligned} \varepsilon(t_0) &= e(t_0) + e'(t_0)(T_{me} + t_0 - t_0) - [e(t_0) + e'(t_0)(t_0 - t_0)] + O(T_{me}^2) \\ &= e'(t_0)T_{me} + O(T_{me}^2) \\ &\approx \frac{e'(t_0)}{r_{me}}, \quad (3) \end{aligned}$$

where $e'(t_0)$ is the strain rate, and is independent of the motion-estimation rate r_{me} . Let consider the same heart with two strain distributions acquired at a rate r_{me1} and r_{me2} comprised in $\varepsilon_1 \pm \Delta\varepsilon_1$ and $\varepsilon_2 \pm \Delta\varepsilon_2$. Then,

$$\varepsilon_2 \pm \Delta\varepsilon_2 \approx \frac{r_{me1}}{r_{me2}} (\varepsilon_1 \pm \Delta\varepsilon_1) = \left(\frac{r_{me1}}{r_{me2}} \varepsilon_1 \pm \frac{r_{me1}}{r_{me2}} \Delta\varepsilon_1 \right) \quad (4)$$

Therefore, if $r_{me2} = 2r_{me1}$, $\varepsilon_2 \pm \Delta\varepsilon_2 = \varepsilon_1/2 \pm \Delta\varepsilon_1/2$. In other words, when doubling the motion-estimation rate, both the center and width of the strain distribution are halved. Finding the optimal motion-estimation rate is thus equivalent to finding the optimal strain distribution.

To perform this optimization, the probability of obtaining a SNR_e value is determined within a given interval, e.g., $[s_1, s_2]$, for a given strain ε_0 , i.e., in a probabilistic framework, $P(s_1 < SNR_e < s_2 \mid \varepsilon = \varepsilon_0)$. SNR_e and ε are simultaneously measured. As a result, their two-dimensional histogram can be constructed and used to determine their joint probability density function (pdf), i.e., $f(SNR_e, \varepsilon)$. The individual pdf of SNR_e and ε can also be obtained from 1-D histograms. Finally, the conditional pdf $f(SNR_e \mid \varepsilon)$ can be obtained through the following relationship:

$$f(SNR_e \mid \varepsilon) = \frac{f(SNR_e, \varepsilon)}{f(\varepsilon)}, \quad (5)$$

Note that $f(SNR_e)$, $f(SNR_e, \varepsilon)$ and $f(SNR_e \mid \varepsilon)$ also depend on the motion-estimation rate, r_{me} , and on the temporal portion of the heart cycle of interest, Δt_c , i.e.,

$$f(SNR_e \mid \varepsilon; r_{me}, \Delta t_c) = \frac{f(SNR_e, \varepsilon; r_{me}, \Delta t_c)}{f(\varepsilon; r_{me}, \Delta t_c)} \quad (6)$$

The analysis below is based on assumptions a and b:

a) $f(SNR_e \mid \varepsilon; r_{ME}, \Delta t_c) = f(SNR_e \mid \varepsilon; r_{ME})$, i.e., the relationship linking SNR_e and ε does not explicitly depend on the cardiac phase. For example, a 1% strain occurring during systole will lead to the same SNR_e distribution as a 1% strain occurring during diastole.

b) $f(SNR_e \mid \varepsilon; r_{ME}) = f(SNR_e \mid \varepsilon)$, i.e., the relationship linking SNR_e and ε does not explicitly depend on the motion-estimation rate. For example, a 1% strain measured with a motion-estimation rate of 1500 Hz will lead to the same SNR_e distribution than a 1% strain measured at 400 Hz. This assumption is stronger than **a**). Effectively, theoretical models of the correlation coefficient typically rely, for fixed imaging parameters, only on the strain value, which would support assumption **b**). However, in the heart, the decorrelation effect of out-of-beam motion might be important. In such a case, a high motion-estimation rate would reduce decorrelation caused by out-of-beam motion in comparison with a lower motion-estimation rate and thus modify the relationship between SNR_e and ε .

Finally, the expected value of the SNR_e was obtained as follows:

$$E\{SNR_e; r_{me}, \Delta t_c\} = \int_0^{+\infty} E\{SNR_e \mid \varepsilon; r_{me}\} f(\varepsilon; r_{me}, \Delta t_c) d\varepsilon, \quad (7)$$

where the conditional expected value is given by

$$E\{SNR_e \mid \varepsilon; r_{me}\} = \int_0^{+\infty} SNR_e f(SNR_e \mid \varepsilon; r_{me}) dSNR_e, \quad (8)$$

under assumption **(a)**.

This expected value of SNR_e varies during the cardiac cycle, i.e. as a function of Δt_e , as indicated in eq. (7). Two strain distributions were constructed: $f(\epsilon; r_{ME}, \Delta t_t)$ and $f(\epsilon; r_{ME}, \Delta t_a)$ where Δt_t and Δt_a correspond to five cardiac cycles (approx. 3000 ms) and the 20 frames following the R-wave (approx. 100-170 ms), respectively. $f(\epsilon; r_{ME}, \Delta t_t)$ was used to construct a robust conditional pdf, i.e., $f(SNR_e | \epsilon; r_{ME})$, based on a large enough number of samples (approx. 300,000) under assumption **a**). By averaging $f(SNR_e | \epsilon; r_{ME})$ over all the motion-estimation rates, $f(SNR_e | \epsilon)$ was obtained under assumption **b**).

The strain distribution was found to have varied both during the cardiac cycle and at different motion-estimation rates. Analysis of the variation of the strain distribution as a function of the motion-estimation rate during activation indicates that at high motion-estimation rates, a bimodal distribution is obtained. A local minimum consistently occurs at an approximately 4% strain. This is in contradiction with eq. 4, which predicts a shift of that minimum. However, as the motion-estimation rate increases, the distribution translates towards lower strain values, narrows and becomes unimodal. As predicted by eq. 3, the center and width of the strain distribution decreases in $(r_{me})^{-1}$. These observations may be seen in Fig. 4.

Highly variable strain distributions as a function of time were observed, during the cardiac cycle both during pacing and during sinus rhythm (for the sinus rhythm case only, data was acquired in a different canine using the automatic composite technique). For example, high strain values were observed during the electrical activation (0-100 ms) and following repolarization (350-450 ms). During diastole, strain amplitudes vary greatly, i.e., from very high values (500-600 ms) to very low values (600-700 ms).

The probability of measuring a SNR_e value simultaneously with a given strain value of (i.e., the joint pdf) was plotted. For low motion-estimation rates (41 Hz), the joint pdf spreads towards larger strain values and is associated with small values of SNR_e . At 452 Hz, the probability of higher SNR_e values is higher, and located between 0.01% and 1% strains. At large motion-estimation rates (1540 Hz), the pdf is concentrated in lower strain values and lower SNR_e values are more probable. These joint pdfs directly depend on the probability of measuring strain. As a result, if, for a given motion-estimation rate, the probability of measuring a given strain was low, the probability of measuring the SNR_e associated with that strain value was also low. To normalize this effect, the conditional pdf was analyzed. In that case, the probability is normalized for each individual strain value. The different conditional pdf's obtained for different motion-estimation rates were very similar in overlapping domains at different motion-estimation rates, therefore indicating that assumption b) can be used. To

obtain a complete representation of the conditional pdf, it was averaged over nine different motion-estimation rates. The SNR_e remained below the CRLB, with the conditional expected SNR_e value being approximately one order of magnitude lower. An experimental transition zone corresponding to a minimum observed at 4% strain was also added and corresponded to a sharp transition in the conditional pdf. For strains higher than 4%, the conditional pdf remained limited by the BB. The motion-estimation rates corresponding to the center of the strain distribution over 5 cardiac cycles and during activation only are also shown, by computing $e'(t_0)$ in eq. (3). The average value of $e'(t_0)$ over five cardiac cycles, i.e., $e'(\Delta t_c)$, and during activation only, i.e., $e'(\Delta t_a)$, was 155.5 s^{-1} and 389.1 s^{-1} , respectively. The same conditional pdf with the conditional expected value of the SNR_e showed the peak conditional expected value of the SNR_e is located between approximately 0.1% and 1% strain, which corresponds to 1555 and 155 Hz over 5 cardiac cycles, and to 3891 and 389 Hz during activation only, respectively.

The expected value of the SNR_e as a function of the motion-estimation rate was then obtained following eq. (7) for five cardiac cycles and during activation only (Fig. 5A). Note that unlike the *conditional expected value* shown in figure 4, the expected value encompasses an entire strain distribution. A sharp increase in the expected value of the SNR_e is observed as the motion-estimation rate transitions from low values up to a maximum at 163 Hz and 350 Hz over five cardiac cycles and during activation only, respectively. The expected value of the SNR_e then slowly decays with the motion-estimation rate. A similar behavior is observed in the variance of the SNR_e (Fig. 5B): a maximum is achieved at 350 Hz that decays at higher motion-estimation rates. Finally, the probability of obtaining a SNR_e value higher than 3, 5 and 10 was also explored (Fig. 5C). A maximum value also occurred at 350 Hz. For example, it is approximately twice as likely to obtain a SNR_e higher than 3 at 350 Hz than at 41 Hz during activation.

The EW was imaged during a single heartbeat using TUAS in a full four-chamber view of a canine heart in an open-chest canine *in vivo*. Image frames were overlaid with color maps indicating the axial incremental strains. For example, the axial incremental strains may be shown for a sequence showing the EW imaged with a 1100 Hz motion estimation rate and a 137 Hz motion sampling rate. Such images showed features of the EW that are expected during pacing from the basal region of the lateral wall. In the parasternal four-chamber view, electrical activation results mostly in thickening of the myocardium; therefore, activation appears as a transition from thinning to thickening. The EW first appears in the basal region of the lateral wall, approximately 30 ms after pacing. The EW was

initiated at the epicardium and traveled towards the endocardium of the lateral wall. Its average velocity over a region of 5 cm can be estimated to be approximately 1.0 m/s, which corresponds to the expected velocity of the electrical activation in the cardiac muscle. The image sequence indicated that the EW then propagated to the septum and then the right ventricle.

In embodiments, the time interval for estimating motion is selected responsively to the error sources captured by the foregoing analysis. In embodiments, the motion capture frequency is optimized to ensure a low random signal component and a low risk of distortion of the motion estimation resulting from strain (motion other than pure displacement).

Using TUAS, it is possible to image cardiac abnormalities that are not periodic, such as fibrillation and this was demonstrated. This was proved experimentally. After prolonged pacing, a heart underwent ventricular fibrillation. The heart was imaged with a motion-estimation rate of 2000 Hz. An acquisition was performed during 8 seconds. No, or very little, wall motion was observed on a B-mode image sequence. However, the incremental strains mapped depicted small, local and oscillating deformations. While pacing from the basal region of the lateral wall was maintained during fibrillation, no clear propagation was observed from the pacing origin.

In the experiments, a TUAS-based imaging sequence was developed and implemented *in vivo*. Such a method increases the motion-estimation rate at the cost of a lower motion-sampling rate, thus allowing very high frame rate motion estimation while maintaining a high lateral resolution and a full view of the heart. Using this technique, the optimal motion-estimation rate for EWI was obtained within a probabilistic framework. Finally, the feasibility of imaging non-periodic arrhythmias in a full field of view with a high motion-estimation rate is demonstrated.

To show the importance of optimally selecting the motion-estimation rate to perform accurate strain estimation, the SNR_e was estimated *in vivo* in a paced canine, with a wide range of motion-estimation rates available with TUAS. Since the motion-estimation rate can be used as a means to translate and narrow the strain distribution, one can find the optimal value by studying the link between the strains and the SNR_e . By constructing first the joint pdf of the SNR_e and the strains, the conditional pdf was obtained for every motion-estimation rate. By averaging these conditional pdf's, a combined conditional pdf spanning a large range of strains values was obtained. This combined pdf was in agreement with the strain-filter theory, which provides a higher bound on the SNR_e . Electronic noise at low strains values and decorrelation at high strain values prevented high SNR_e 's in these ranges. The ZZLB

predicts a sharp transition between the CRLB and BB when decorrelation becomes important to the point that the phase of the signal does not contain information about motion. Using a model of correlation that takes into account only strains, this transition was expected to occur at 40% strains. However, the findings suggest that this transition occurs in the vicinity of 4% strains instead, indicating that other causes resulting in decorrelation such as out-of-beam motion have large consequences on the value of the SNR_e . It was confirmed that the combined conditional pdf is comprised within the CRLB up to approximately 4% before it becomes comprised within the BB. A sharp decrease in the expected value of the SNR_e is also observed at 4% strain, underlying the importance of using the phase information of the RF signal for accurate strain measurements. It was also observed that the strain distribution lacked values around this transition. A distortion in the strain distribution may indicate that while a high SNR_e can be maintained, the accuracy of the strain estimator is impaired at low motion-estimation rates, i.e., less than 350 Hz in this case. Four measures were used to determine the optimal motion-estimation rate: the expected value of the SNR_e and the probability of obtaining a SNR_e value larger than 3, 5 and 10. For all these measures, the optimal motion-estimation rate was found to be 350 Hz. However, 350 Hz also corresponded to the highest variance in the SNR_e . In other words, a motion-estimation rate of 350 Hz provides the highest SNR_e but is also riskier, in the sense that the SNR_e will not be homogeneous within one image. By increasing the motion-estimation rate further, the expected value of the SNR_e decreases but so does the variance. Therefore, there is a trade-off between the expected value of the SNR_e and the likelihood of obtaining this value.

These results are, however, tied to the context of this study. This validation was performed in an open-chest setting, which provides very good image quality with the ultrasound system used. In a more clinically-relevant transthoracic imaging, the signal-to-noise ratio of the RF signals themselves are expected to be lower, shifting the ZZLB towards higher strain values and thus modifying the optimal motion-estimation rate value. Inversely, in a context of higher RF signal-to-noise ratio such as in trans-esophageal echocardiography, the ZZLB may be expanded towards lower strains, thus improving the SNR_e associated with higher motion-estimation rates. Because of the wide range of motion-estimation range available when using TUAS, an optimization process similar to the one developed here could be adjusted on an individual basis.

The effect of reducing the motion-sampling rate was also investigated. At motion-sampling rates of 120Hz, it was found possible to depict the EW. This indicates that the motion-sampling rate can be reduced at very little cost in terms of motion estimation

performance. The location of the activation was detected because of the high precision achieved for the motion estimation. This shows that the trade-off of TUAS, i.e., halving the sampling rate compared to a conventional sequence with the same beam density, does not jeopardize the EW depiction. Decoupling the two frame rates may thus be a solution to improving the precision of the axial estimation without sacrificing the lateral resolution.

It was shown that TUAS is capable of accurately depicting non-periodic events at high temporal resolution. Effectively, the ability to image the displacements and strains in a fibrillating canine heart, in a full-view and with high beam density, was demonstrated. Strain patterns expected during such a phenomenon were depicted, such as a disorganized contraction, leading to little-to-no large scale motion of the heart. Regions of the myocardium were oscillating rapidly from thinning to thickening and thickening to thinning over time. Studying the frequencies of these oscillations could be useful in understanding the mechanisms of fibrillation.

Various focusing patterns designed may be used to improve the motion estimation/spatial resolution trade-off. The following discusses embodiments which may be implemented in combination with composite imaging (combining samples from multiple repeating cycles) or TUAS.

A focused beam may be used as in a standard acquisition sequence in which the frame rate is increased by sending only a limited number of transmits and creating multiple lines per transmit as has been described with reference to Figs. 1B and 3.

Flash or plane wave mode (Fig. 6A), consists of sending non focused transmit waves 201. In this case, all the elements of the probe fire at the same time resulting in a wavefront parallel to the probe. An image is created from a single transmit event so that

$$FR=c/2d$$

The flash (could also be plane wave – will use “flash” hereon for convenience) sequence may produce lower image quality since no focus is present. Also, the energy emitted is distributed over the field of view making this technique more sensitive to reflections from high-impedance tissues such as bones. A single flash pulse 201 may be emitted and receive beam forming used to generate receive beams 200. As is understood in the art, the receive beams may be used to create an image. The process is repeated to create an image sequence from which motion can be estimated.

Fig. 6B illustrates a combination of flash mode image acquisition and conventional frame scanning (B-mode) image acquisition. The flash mode produces less resolution but fast motion estimation. So flash mode acquisition pairs 240A, 240B and 242A, 242B are

used for high frequency motion estimation and further image frames are generated on a longer time base by conventional focused beams 241, 243. The pattern repeats for the duration of the scan. Fig. 6C shows that the temporal separation between the flash acquisitions and the conventional focused beam acquisitions is flexible in that the flash acquisitions 250A, 250B, 250C, 250D, 250E etc. can be temporally interspersed among the lines of the focused beams 251A, 251B, 251C 251D etc. The time gap T_g between pairs of flash acquisitions may be varied independently. The focused beams 251A, 251B, 251C form a single image frame. The image frames provided by the focused beam image frames provide the detailed anatomical information and gross motion while the flash modes can provide motion estimation and these can be overlaid on an output display. It will be evident that a user may select the temporal spacing of the flash and focused beam acquisitions to permit the T_{mc} and T_{ms} intervals to be substantially independently selected. The additional flash acquisitions may be combined with focused frame acquisitions to generate or improve the quality of interpolation frames as well as provide more frequent displacement estimations.

Partial defocusing or “Explososcan” lies between the standard and flash sequences. The size of the focus is increased making the formation of more than one line per transmit more efficient as illustrated in Fig. 7A. This may be done by appropriate beam forming or by using a Hanning window. Receive beam forming is used as indicated by the multiple return arrows 202 for each transmit event 204. , i.e. less transmits are necessary to illuminate a given area. The size of the focus and the number of lines consequently formed can be varied as much as wanted. The size of the focus can be easily chosen by varying the size of the aperture. In this case, the drawback is also a reduced image quality since resolution becomes smaller as focus size increases. In the partial defocusing imaging sequence the beam is focused at the desired focal length and steered across the field of view. The partial defocusing sequence is similar to the standard sequence, but the size of the focus is bigger, thus decreasing the number of transmits required to illuminate a given area.

In another embodiment, an imaging technique consists of creating multiple foci for each transmit as shown in Fig. 8. The beam is focused at multiple angles, thus creating multiple beam lines in parallel to permit simultaneous acquisition of multiple beams 206A and 206B. It can be implemented different ways and is easily understood with an example; assuming three foci are desired. Firstly, it is possible to create three foci by sending three pulses on each element. The pulses have to be delayed by the amount of time needed to reach the different foci spots. This may be implemented on a scanner configured to transmit multiple pulses per element. In addition, equation 9, the well-known Fraunhofer

approximation, shows that the pressure field is the Fourier transform of the pressure at the aperture.

$$\boxed{P_{\text{focal}} \cong \mathcal{F}\{P_{\text{aperture}}\}} \quad (9)$$

Another embodiment creates multiple foci through the application of an appropriate apodization function. Fig. 7B illustrates a variation of the embodiment of Fig. 8 in which multiple partially defocused transmit beams 208, 210 are emitted in parallel.

Fig. 7C shows another embodiment in which pairs of broad (defocused) transmit beams are used to acquire motion data as pairs 270A, 270B; 270C, 270D; 270E, 270F; 270G, 270H; 270I, 270J; and 270K, 270K. The pairs are interspersed among focused beam trains 271A, 271B, 271C, 271D, and 271E which in combination form a single image frame.

In evaluation experiments, four transmit patterns (focused, flash, partial defocusing and multi-foci) were implemented in combination with TUAS on an ultrasound scanner as follows for purposes of experimental evaluation: the embodiment of Fig. 7C may, as described with reference to Fig. 6C be used to provide arbitrary number of motion estimates per image frame using partially defocused transmit beams. The motion estimates may be used to increase the time resolution of motion estimation changes as well as to improve interpolation of image data acquired using the focused beams.

For the focused pattern, a conventional focusing method was used using suitable delays as in conventional beamforming. For the flash pattern, the delays in transmit were not set to zero. For the experiment, using a phased array, the field of view would have been too small if the wavefront was parallel to the probe. A diverging beam was used instead of the conventional approach with a larger probe. In the present approach, the focus was located behind the probe at a distance $z = (d/2)/\tan(\pi/4)$, where d is the size of the aperture.

For the partial defocusing example, the beam was focused following the conventional method, but an apodization window narrowing the aperture was used to increase the size of the focus. Several windows were implemented (rect, Hanning, Tukey, Blackman).

For the multiple focus example, in the same way as for the partial defocusing method, the beam was focused while applying an apodization window. The duality property of the Fourier transform shows that taking two Fourier transforms in a row results in inverting the input function and scaling it by a factor 2π .

$$f(t) = F(\omega) \quad (10)$$

$$F(t) = 2\pi f(\omega) \quad (11)$$

To obtain three foci, a function whose Fourier transform has three distinct peaks was used, a *Battle* wavelet (Figs. 9A to 9B). The Battle wavelet is shown in Fig. 9A, its Fourier transform which serves as the apodization function in Fig. 9B, and the Fourier transform of the apodization function predicts the pressure field at the focal distance in Fig. 9C.

The example embodiments were tested using an ultrasound system that could store signals for each transducer in the array separately. For a 64 element phased array, this is 64 times the data compared to a conventional ultrasound system. Image depth for sampling was set to 12 cm. A tissue mimicking phantom was used which produced strain and motion using a pulsatile flow of water. The phantom was placed in a water tank which was filled to provide coupling. A 2.5 MHz phased array was used.

The image reconstruction is completely independent of the apodization function, so the same method was applied for each sequence. A pixel-based method was used instead of a conventional reconstruction where a line is computed by summing the data of each element over time. The pixel-based reconstruction computes the value of each pixel by summing only the RF data contributing to image the specific location. Contrarily to a conventional method where each line is computed by applying one set of delays to the RF, the pixel-based reconstruction applies different sets of delays for each pixel. Assuming the axis convention shown in Fig. 10 (A set of time delays is computed for each pixel based on the time needed for a wave to travel back and forth) and a constant speed of sound through the medium, the value of the pixels are given by

$$s(x, z) = \int_{array} RF(k, t(k, x, z)) dk$$

where (x, z) are the coordinates of the pixel wanted and $t(k, x, z)$ is the time needed for a sound wave to travel back and forth from the point (x, z) to the element k on the probe. This reconstruction technique has been described for a flash sequence and adapted for our specific cases. A reconstruction was done for each transmit resulting in one sub-frame per transmit.

Displacements were estimated using a fast cross-correlation technique. 2D motion (axial and lateral) was estimated using a 1D kernel (5.0 mm) in each direction. There was a 80% overlap in the axial direction. In the lateral direction, the RF signals are interpolated along the lateral direction of the ultrasound beam to perform sub-beam lateral displacement estimation. Displacement maps were obtained after a two-steps process: firstly, displacements were estimated between sub-frames i and $i + N$, for $[i = 1, 2, 3, \dots, N - 1]$, where N is the number of transmits used to image the complete field of view. The indexes i and $N + i$ correspond to the sub-frames reconstructed with the same transmit angle. Secondly, the

displacement maps between two frames were computed as the sum of the $N - 1$ maps previously obtained. Strains were computed as the spatial derivative of the displacements.

Laboratory tests showed that the partial defocusing and multi-foci methods could be used to estimate displacements. Both techniques created artifacts on the B-mode, but did not lead to any significant consequences on the displacements. The focused, partial defocusing, multi-foci and flash methods were implemented on the ultrasound scanner. Raster scans were performed in order to characterize the beam profiles and to assess a safety limit specific for each method. All the imaging techniques were tested in a phantom study and have shown to be capable of providing promising and coherent strain maps of a moving phantom.

In experiments with a canine heart, imaging sequences used a global frame rate of 131 Hz, a local frame rate of 418 Hz and 12 transmits per frames. The flash sequence was as described above. RF data were acquired as described above. The partial defocusing method was co-registered with cardiac mapping for comparison.

A pixel-based reconstruction was performed followed by displacement and strain estimation. The latter allowed the computation of isochronal maps of the electromechanical wave. On both isochrones, a wave propagating from the earliest activation point to the base and to the apex is clearly visible. Also, the last segment to be activated was the basal septum. The electrical activation times were compared with the onset of the EW at the approximate location of the electrodes.

A strong correlation was found between the isochrones of both techniques. This result demonstrates that the imaging technique implemented was suitable for EWI allowing an isochronal map to be obtained that was highly correlated with the measurements made with the cardiac mapping. The experiment was performed over a single heart cycle showing that the new imaging technique could replace composite imaging which requires multiple cycles and repeating motion.

In further experiments, axial displacements were estimated at a 500-Hz motion-estimation rate in both cases and at a 2000-Hz and 137-Hz motion-sampling rates in flash and wide beams sequences, respectively. A 1D cross-correlation algorithm of RF signals reconstructed at 20 MHz in a phased array configuration was used. The window size was 4.60 mm and the overlap 90%. The heart was segmented using an automated contour tracking technique. The incremental axial strains were estimated with a least-squares method and a kernel size of 10.7 mm. The strains were then overlaid onto the B-mode image acquired immediately following the flash sequence. Finally, isochrones were constructed as in previous studies.

The wide beam sequence was used in an open-chest animal and correlated with the electrical activation sequence during pacing from the apical region of the lateral wall. The heart was imaged in the four-chamber view, but with the ultrasound probe positioned parasternally. In that view, activation results mostly in thickening of the tissue (since the ultrasound beam is aligned with the radial direction of the heart). EWI shows activation originating from the apical region of the lateral wall, followed by the activation of the right-ventricular wall and finally by the septum. Corresponding EWI isochrones reflected this behavior. The EW and the electrical activation mapped using the basket catheter were highly correlated. A slope of 1.31 ($R^2 = 0.99$) was obtained between the electrical activation and the EW onset.

EWI at 2000 fps was then performed in a standard apical four-chamber view in a normal, conscious canine during sinus rhythm using the flash sequence. In that view, the EW is expected to mostly result in shortening (negative strains) of the tissue, since the ultrasound beam is aligned with the longitudinal direction of the heart. During sinus rhythm, the natural pacemaker is the sinus node, located in the right atrium. Signals are generated spontaneously at the node, travel through the atrium (during the P-wave), to the atrio-ventricular node, the bundle of His and finally the Purkinje fiber network and the ventricular myocardium (during the QRS complex). Complex activation patterns are expected when imaging the ventricles, since activation will originate from multiple locations following the Purkinje fiber network. It was confirmed that the EW follows such a pattern. The EW originated from the right atrium and propagated towards the left atrium. Between the P- and the Q-wave on the ECG, little or no propagation is observed. During the QRS complex, activation originating from multiple sources, located for example at the mid-level of the septum, high on the lateral wall and near the right apex are observed. These results are in accordance with previous studies of the normal electrical activation of the heart and with previous studies using EWI with ACT.

The same animal was then imaged during pacing from the right ventricle after the ablation of the atrio-ventricular node. In that case, the electrical activation of the atria and the ventricles are dissociated, i.e., the activation of the sinus node do not necessarily results in the activation of the ventricles. This phenomenon was observed on an ECG trace, where multiple P-waves without a following QRS complex were observed. During the P-wave, the EW was initiated from the right atrium and propagated in the left atrium. This was expected, since the atria are still driven by the sino-atrial node as during sinus rhythm. During the QRS complex however, activation was triggered by the pacemaker located near the apex of the right ventricle. Therefore, the EW was expected to propagate from the right ventricle near

the apex towards the other regions of the heart. EWI displayed such a pattern: the EW originated near the right ventricular apex and propagated towards the septum and the lateral wall.

The feasibility of flash- and wide-beam acquisition types for EWI in a full view of the heart were experimentally evaluated and confirmed. Experiments were first conducted in open-chest canines to allow for simultaneous cardiac electrical mapping using a basket catheter and confirming that a high correlation between EWI and cardiac mapping is maintained when using new transmit sequences. Then, experiments were conducted in a closed-chest setting. In these canines, EWI was performed both during sinus rhythm and during right-ventricular pacing following atrioventricular dissociation, i.e., a non-periodic rhythm. EWI performed in a closed-chest setting while respecting the Food and Drug Administration standards is more prone to artifacts originating from reflections, e.g., from the rib cage, and thus similar to the clinical setting. Therefore, this study indicates that flash- and wide-beam EWI can be applied in humans and permits the study of irregular arrhythmias in patients.

Fig. 11A shows an example of a temporally unequipped acquisition in 3D. The principles are applicable to estimation of motion in 1D and 2D along any axis of set of axes. A reference region 401 is first illuminated, in this case, by four beams 402 and echoes acquired to form a reference frame. Subsequently, a short time later, a comparison region 403 in the same plane is illuminated by, in this case, nine beams and the echoes acquired to form a comparison frame. The projection of beams 402 and 404 are shown at 406 and 408 respectively. The beams in the reference and comparison regions are recorded at the same axial depth, though are separated in the axial direction in figure for the sake of clarity. The time of transmit and acquisition of echoes of each beam is shown in Fig. 11B with each line numbered 1-4 and 1-9 indicating a corresponding beam as in Fig. 11A. This technique can be applied in either 1-D, 2-D, or 3-D estimations. The comparison beams 404 are arrayed around a respective one of reference beams 402 a spacing (s_r) and number such that an expected magnitude of displacement in the lateral and azimuthal directions may be detected. If only axial displacement is to be detected the reference and comparison beams can be arranged collinearly. In addition there may be different numbers of reference and comparison beams.

Referring to Fig. 12A, a larger region may be scanned by illuminating and acquiring multiple sets of reference 420 and comparison 422 regions rather than illuminating the entire global region 430 at once using the same TUAS technique as described above with reference

to axial displacement estimation. The example TUAS sequence is depicted for three regions. Note that the reference and comparison regions are at the same axial depth, though are separated in this figure for clarity. The amount of time between the acquisition of a reference region and its corresponding comparison region may remain constant. A time graph of the sequence is shown in Fig. 12B. The bars 430, 431, and 432 bracket complementary pairs of regions 420 and 422. It is evident that a region may be scanned in interleaving steps. Fig. 12B shows the time is constant between the three separate regions. This technique can be applied in 1-D, 2-D, or 3-D estimations.

With regard to the scanning of reference and comparison regions, it may be desirable for motion estimation interval T_{me} to be constant and as close as possible to an optimum (See Figs. 5A-5C and discussion) because a small T_{me} will generate a noisy motion estimation and a large T_{me} will result in poor inter-frame correlation as a result of the deformation of structures. Assuming this and also the requirement that any group of beams must be acquired sequentially, which is the case for most ultrasound scanning systems in which the ultrasound signals are not multiplexed, though this is not an absolute requirement and the following may be adjusted for systems where beams can be transmitted simultaneously.

In the 1D, 2D, and 3D embodiments and embodiments where lateral (or non-axial) motion estimation is to be done, each reference beam (which will be called a principal line or PL) uses a group of beams (which will be called blocks) that are transmitted after an interval of T_{ms} . It is assumed that the members of the blocks will be transmitted consecutively so that the time between them is minimal and therefore they can best approximate transmission at a single instant of time. Using an index, a single principal line and a block of three lines could be designated i_1 , i_2 , i_3 , and i_4 .

In the case of 12 lines (i_1 to i_{12}) consisting of three blocks and three PLs, the lines can be arranged in $12!$ possible sequences. The possible arrangement will be reduced to satisfy two constraints mentioned above and restated here:

- Constraint 1 : i_4 , i_5 , i_6 must be consecutive, as well as i_7 , i_8 and i_9 together and i_{10} , i_{11} and i_{12} together.
- Constraint 2 : The second constraint is that the time between i_1 and i_4 , i_2 and i_7 and i_3 and i_{10} must be equal to ensure same motion estimation rate in each sector.


The sequencing problem can be described as one of placing 3 PLs into 12 possible spaces each corresponding to a beam transmit time. Below, each underscore represents a possible space where there can be a PL. Between two blocks there can be 0, 1, 2 PLs, because

constraint 2 eliminates 3 PLs being together so the problem is locating the PLs into the spaces indicated by numbered spaces below.


		block					block					block				
1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17

The potential positions for the PLs are: 1, 2, 6, 7, 11, 12, 16 and 17 since the blocks occupy {3,4 and 5}, {8, 9 and 10} and {13, 14 and 15}. The first index of each block is: 3, 8, and 13.

The method now described is a constructive method that provides at least one sequence of the given number of sectors. The method may not be the only solution. For an odd number of PLs the PLs are placed every 4 positions starting from 1 (example : 1 5 9 and 13, which leaves {2,3,4},{6,7,8},{10,11,12},{14,15,16} for the blocks). To maximize the distance between one PL and the block of its sector while fulfilling the requirement of constraint 2, the process is as follows.

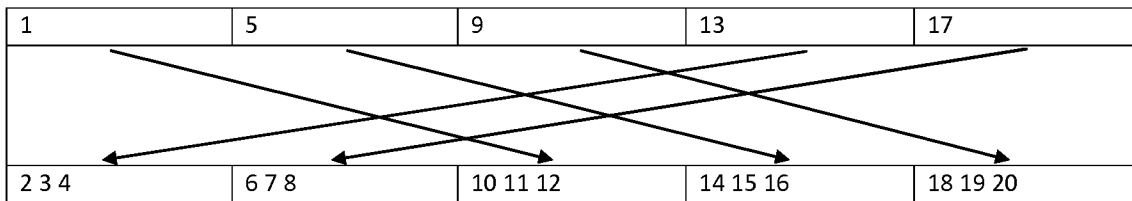

Divide the motion estimation rate by $10-1 = 9$. For an even number of PLs place the PLs every 4 positions starting from 1 until half of the total number of positions are reached and then place PLs every 4 positions starting from the last possible index until half of the total number of positions is reached. For example : 1, 5, 9, 24, 20, and 16, leaves {2,3,4}, {6,7,8}, {10,11,12}, {13,14,15}, {17,18,19}, and {21,22, 23} for the blocks. Then maximize the distance between one PL and the block of its sector while fulfilling the requirement of constraint 2. Here the motion estimation rate is divided by $13-1 = 1$.

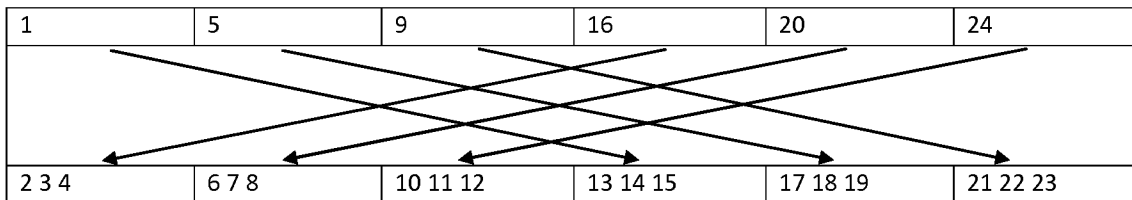

So in a class of embodiments, a single temporal sequence of spatially separated ultrasound transmission beams is ordered in time in the following manner. A fraction of the beams are principal beams and the remaining are divided among the principal beams, two, three, four or more to each principal beam, each of these being called a “block.” Each principal beam is separated in time from its respective block by a fixed time interval. All the beams of a given block are temporally adjacent one another. Each principal beam is

separated from the members of its corresponding block by a predefined distance (or the distance may vary by region of the target structure or time depending on an expected rate of motion). Since the beams in a block are not temporally coincident, the time difference between a principal beam and its corresponding block is the time difference between one of its members and the principal beam. The predefined distance is selected responsively to the rate of movement of the target structure and the fixed time interval such that an axial pattern imaged by the reference beam will be identifiable the fixed time interval later (or prior) in an image from at least one of the members of the corresponding block.

In other embodiments, at a first time, the system transmits a reference beam and subsequently transmits corresponding comparison beams where each comparison beam is spatially separated from the reference beam within a range of displacements around the reference beam, the range of displacement being responsive to a predicted rate of displacement and the time interval T_{ms} (a predefined interval) between the reference and one of the comparison beams. At a second time, multiple reference beams are transmitted which are spatially separated from another reference beam (the another reference beam not yet being transmitted at the second time) within a range displacements which are also responsive to the predicted rate of displacement and the time interval T_{ms} between one of the comparison beams and the reference beam. After the second time, the corresponding reference beam is transmitted, which is located spatially in the middle of, or at least adjacent, the comparison beams. In embodiments, the comparison beams corresponding to the reference beam are temporally adjacent (i.e., they are transmitted together without any other beams being transmitted temporally between them). So essentially what this is saying is that sometimes the reference beam of a reference beam-comparison beam block pair will be transmitted in that order and sometimes they will be transmitted in reverse order.

Fig. 14 shows an ultrasound system 301 including one or more ultrasound probes 310, a driver/data acquisition element 312, a processor 314, and a user interface and display element 316. The driver/data acquisition element 312 and a processor 314 communicate with a data store 318 for raw ultrasound signal data, reduced data such as images, image sequences, and motion estimation data, and software. The ultrasound probe 310 may include multiple probes that are used simultaneously (frequency encoded, for example) or a kit of probes that are used at different times. Also the ultrasound probe 310 may be a combined probe with multiple heads that are automatically driven at different times such as flash sequence probe and a phased array probe combined as a unit that can generate both flash pulses and focused beams for combined scans, for example as discussed above with reference

to Figs. 6B and 6C. The system 301 is figurative and it should be clear based on the state of the art in digital data acquisition and control systems that any of the elements of the system 301 may include one or more components for each function or the functions combined into combined elements.

Fig. 13 shows a process 280 for generating a display which runs in parallel with a process 282 for acquiring sample data which is passed by a data store or transfer channel to the process 280. At S10, parameters of the scan are displayed on the user interface and selected. For example, the parameters may be displayed on a touch screen and selected by touch. Alternatively names profiles may be stored and provide grouped selections. The parameters that may independently on a per session or per profile basis may include the following or equivalents.

- Type of scan (TUAS narrow beam, TUAS broad beam, Flash with B-mode, etc.)
- T_{ms} - the temporal spacing of ultrasound image frames.
- T_{me} - the temporal spacing of motion/strain estimation frames.
- s_r - the spacing of comparison region lines from corresponding reference region lines.
- Number of beams.
- Virtual origin of diffuse beam approximation of flash (if phased array used to generate).

In addition, conventional parameters of ultrasound may also be chosen as well as any other parameters of the embodiments described herein.

At S12, a first subframe or flash acquisition is made and at S14 a second subframe or flash acquisition is made. One or more focused beam acquisition may occur between the flash acquisitions if flash mode embodiments are being performed. The steps are repeated as indicated by the ellipses S19 and S22, S24 while in the contemporaneous process 280, the acquired data is processed into images and motion data in S16, S18 and displayed S20. The processing of process 280 may take advantage of delays in process 282 or may employ hardware and I/O and data storage subsystems and techniques to permit completely independent execution of S280 and 282. As a result, real time or near real time display of anatomy and motion data may be provided.

In all of the disclosed embodiments where transmit focused or partially focused beams are used, the ultrasound images can be generated from stored data received at all

transducers in an array (2D or 3D) of the ultrasound probe from a wide or flash beam transmit using known signal processing techniques under the general category of receive beam forming. Thus additional embodiments can be generated from the above disclosure by making this change in the structures and methods.

Figs. 17A, 17B, and 17C shows alternative variations of the beam layouts of Figs. 11A, 11B, and 12A, 12B for lateral strain estimation in 3D. In Fig. 17A, the principal beam 502 has a block 504 of 9 beams with one beam collinear with it. The plan view is shown at 492. In Fig. 17B, the principal beam 502 has a block 506 of 5 beams with one beam collinear with it. The plan view is shown at 494. In Fig. 17B, the principal beam 502 has a block 508 of 5 beams with one beam collinear with it. The plan view is shown at 494. These three layouts can be modified by the removal of the collinear beam to form new embodiments. These figures are included to highlight that various beam layouts are possible.

Figs. 17D and 17E illustrate a 2D arrangement for lateral strain estimation that was validated by experiment. The acquisition was of a canine heart using flash 528 sequences with the receive beams 630 indicated for illustration. The beamforming can be done using stored data and was done that way in the validation experiment. The frequency of flash transmits was 2000Hz. Four flash transmits are shown but 4000 were generated over the 2 sec. cycle of the data acquisition. Each flash is used to generate a principal beam which is compared to block of beam formed from a flash 1/500 sec. removed and this is repeated for the nearly 4000 flash pulses for which it is possible.

In the experiment, images were acquired using a phased array probe with 64 elements. Images were acquired at 2000 fps during 2 sec. interval followed immediately by the acquisition of a 128 line, 30 fps, B-mode image over 1.5 s. An electrocardiogram (ECG) was acquired simultaneously. RF signals were reconstructed from the element data in a pixel-wise fashion. As mentioned, lateral displacements were estimated at a 500 Hz motion-estimation rate and at a 2000 motion-sampling rate.

The incremental lateral displacements that occurred from end-diastole to end-systole were integrated to obtain the cumulative lateral displacement. For each pixel, appropriate registration between consecutive displacement images was performed in order to ensure that the cumulative displacement depicted the motion in the same myocardium region. The cumulative lateral strains were estimated from the cumulative lateral displacements with a least-squares method and a kernel size of 10.7 mm. The strains were then overlaid onto the B-mode image acquired immediately following the flash sequence to generate a display sequence which was reviewed with the following observations.

The cumulative lateral strain showed that during systole, the left and right segments of the myocardium exhibit lateral lengthening, while the top and bottom segments show slight lateral shortening. These results show the feasibility of lateral tracking in a canine myocardium.

In all of the foregoing embodiments, the motion capture and estimation is not limited to tissue structures such as muscle. The velocity of fluid such as blood can be captured using the higher rate data. The flow of blood in the ventricles may be simultaneously captured along with motion such as the electromechanical wave. The user interface may allow a selective display of the fluid (e.g. Blood) data and other tissue as illustrated in Figs. 15A through 15C. In Fig. 15A, displacement contour or color maps (regions indicated by 330, 332, 334) for non-fluid tissue structure (such as myocardium) are shown in an image sequence. One or more controls may be actuated to switch to motion data display of fluid near or within the tissue structure 354 in a further display of Fig. 15B (showing, for example, velocity contour map regions 340, 342) or combined in Fig. 15C.

Fig. 16A illustrates a spatially unequidistant transmit beams, which may be focused or unfocused. The embodiment increases the local beam density. This may be used to spend the line density budget where it can provide the most benefit. For example, it may be known *a priori* or through a prior registration imaging cycle, that the motion to be imaged occurs at particular regions. These regions can be imaged with high beam density and surrounding regions may be imaged with lower line density. For example, the progress of EW in myocardium may be known or determined from prior imaging and used to change the beam density during a cardiac cycle so as to improve the relevant image. Also this may permit high temporal resolution by permitting a smaller line count to be used. An another alternative, the beams are expanded and focused variably over a single scan in a manner similar to Fig. 7C embodiments, but responsively to the locations where spatial resolution is needed. For example, low resolution requirement regions are scanned with broad transmit beams and high resolution requirement regions with narrow beams. In Figs. 16A and 16B, the beams are indicated by number indicating the timing of the beam in a sequence. Fig. 16B shows a special case of the embodiment of Fig. 3 in which the beams are scanned twice in a row to be used for motion estimation.

In all of the foregoing embodiments, various methods devices and systems are described at least for addressing the problems of EW. In EW, inter-frame motion (or, displacement) is estimated axially via cross-correlation of consecutive RF frames. From the displacements, one can then obtain the inter-frame strains (or, strains) depicting the EW by

applying gradient operators on the displacement field. However, the heart is an organ that undergoes significant three-dimensional motion and large deformations, which both lead to the decorrelation of the RF signals and thus to the degradation of the motion and deformation estimation accuracy. Increasing the imaging frame rate reduces these effects. However, imaging at high frame rates over a large field of view and at high resolution constitutes a technical challenge which is addressed by the present technology.

In any of the foregoing embodiments, the data handling burden may be limited by scanning at a specific point in a cyclical event, such as a cardiac cycle. This may be done by scanning for a few cycles and then predicting the next cycle start and end times and controlling the ultrasound acquisition to begin and end within those times.

In many of the foregoing embodiments, the sequence of the transmit beams is such that spatially adjacent beams are transmitted consecutively.

In many of the foregoing embodiments, the sequence of the transmit beams is such that scanned beams (beams other than flash) are repeated for each frame. However, it will be clear that this is not a requirement in that beams that are close to, but not coincident with, prior beams, can still be used to generate images that can be compared to generate motion estimates and image sequences. Thus, all of the foregoing embodiments may be modified such that beams making up mini-frames and partly defocused beams may be aimed differently even for those forming a pair to be compared for motion estimation. For example, transmit beam 270A and 270B in Fig. 7C may be shifted spatially (angle-wise) relative to each other, within limits.

According to embodiments, the disclosed subject matter includes an ultrasound system for imaging a target structure that moves or deforms with time. The system includes an ultrasound imaging device configured to image at a spatial resolution and sample a predefined field of view no faster than a frequency $1/T_{ms}$. The target structure is one which moves or deforms such that relative displacement of portions of the target structure of a size equal to the inverse of the spatial resolution are substantially uncorrelated at time intervals greater than a time interval T_{me} . The target structure is also one where relative displacements propagate over time scales many times greater than T_{me} where T_{me} is much smaller than T_{ms} . The system has a controller configured to control the ultrasound imaging device to image the target structure at a frequency of $1/T_{me}$ and to capture relative displacement data responsive thereto. The controller is further configured to generate an image sequence representing the field of view in which the relative displacement data is shown on the image sequence.

The controller may be configured to acquire multiple first image frames consecutively in time which first image frames are smaller than the field of view. The controller may further be configured to assemble first image frames to form second image frames spanning the field of view.

According to embodiments, the disclosed subject matter includes method for estimating properties of motion of a body structure. The method includes directing at least a first ultrasonic beam into a first angular sector of the body structure. The method further includes directing at least a second ultrasonic beam into a second angular sector of the body structure. The method further includes directing at least a third ultrasonic beam into the first angular sector of the body structure prior to the directing at least a second ultrasonic beam into the second angular sector of the body structure. The method further includes detecting motion of the body structure in the first angular sector by detecting a magnitude of a displacement of a portion of the body structure occurring between return echoes from the at least a first ultrasonic beam and the at least a third ultrasonic beam.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure. The method includes directing a first at least three ultrasonic beams into respective angular sectors of the body structure, the angular sectors combining to span a field of view of an ultrasonic transducer, wherein the beams are separated by at least first and second angular intervals so that the angular beam density varies over the field of view. The method further includes repeating said directing for a second at least three ultrasonic beams and receiving return echoes from the first and second at least three ultrasonic beams. The method further includes detecting motion of the body structure by detecting a magnitude of a displacement of a portion of the body structure occurring between the return echoes from the at least three ultrasonic beams.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure. The method includes generating a reference ultrasound scan of region of the body structure at a selected axial depth using a pattern of first beams distributed over a first angular range and directed at respective first angles. The method further includes generating a comparison ultrasound scan of the region of the body structure at the selected axial depth using a second pattern of beams distributed over substantially the first angular range and directed at respective second angles. The first angles and the second angles are non-collinear. The first angles may be distributed over a solid angular ranges. The first and second angles may be distributed over solid angular ranges. The first angles may lie between respective ones of the second angles.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure. The method includes generating a first reference ultrasound scan of a region of the body structure at a selected axial depth using a pattern of first beams distributed over a first angular range and directed at respective first angles. The method further includes generating a first comparison ultrasound scan of the region of the body structure at the selected axial depth using a second pattern of beams distributed over substantially the first angular range and directed at respective second angles. The method further includes generating a second

reference ultrasound scan of region of the body structure at a selected axial depth using a pattern of first beams distributed over a second angular range and directed at respective third angles. The method further includes generating a second comparison ultrasound scan of the region of the body structure at the selected axial depth using a second pattern of beams distributed over substantially the second angular range and directed at respective fourth angles. The first, second, third, and fourth angles are non-collinear.

The first angular range may be a solid angular range. The first and second angular range may be a solid angular range. The first angles may lie between respective ones of the second angles.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure including directing, into the body structure, first and second broad ultrasound beams in respective first and second transmit events. For each of the transmit events, the multiple receive beams may be formed to form first images of said body structure at first and second times. The method further includes generating motion information by comparing the first images. The method further includes generating first and second ultrasound image scans using focused beams generated by first and second sets of transmit events. The first and second transmit events and the first and second sets of transmit events all occur during a single motion event of said body structure.

The single motion event may be induced by an electromechanical wave in a heart muscle. The first set of transmit events may occur at a time between the first and second transmit events. The first and second transmit events and the first and second sets of transmit events may have substantially the same spatial scope. The method may also include generating a B-mode image responsively to the first and second ultrasound scans and overlaying motion data resulting from the step of generating motion information. The method may further include generating a B-mode image sequence responsively to the first and second ultrasound scans and overlaying motion data resulting from the step of generating motion information.

According to embodiments, the disclosed subject matter includes a high frame rate ultrasound image acquisition method. The method includes generating waveforms with respective time delays and respective apodization weightings determined to cause selected transducer elements of a transducer array to transmit respective transmit beams along corresponding transmit beam paths toward a body structure to be imaged during a first transmit event such that the first transmit event is distributed over a first portion of a field of view. This is followed by transmission of respective transmit beams along corresponding transmit beam paths during a second transmit event distributed over a second portion of the field of view. The method includes acquiring a first plurality of spatially separated beam lines at selected transducer elements during a first receive event subsequent to said first transmit event along corresponding receive beam paths, and acquiring a second plurality of spatially separated beam lines at selected transducer elements during a second receive event subsequent to said second transmit event along corresponding receive beam paths. The first plurality

of spatially separated beam lines are acquired multiple times in succession before acquiring the second plurality of spatially separated beam lines.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound. The method includes directing a first beam into the body structure. directing multiple second beams into the body structure. where a and b are repeated in the sequence: at least two a) events followed by at least one b) event which sub-sequence is repeated multiple times with each sequence is the same or different from other sequences. from multiple a) events, estimating the displacement of anatomical portions of said body structure to generate at least first motion estimates from echoes of the first beams. from multiple b) events. The method further includes estimating at least the relative positions of anatomical portions of said body structure from echoes of said second beams over time to generate images of said body structure. and combining the images and first motion estimates to form a display indicating motion within the body structure.

The first beams may be wider than the second beams. The first beams may be parallel beams. The first beams may be single pulses spanning a field of view of the body structure.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound, comprising: generating a first beam aimed a first fraction of a field of view of the body structure. The method includes receiving multiple beams from a received echo to generate a first image frame. The method further includes generating a second beam aimed the first fraction of the field of view of the body structure. The method further includes receiving multiple beams from a received echo to generate a second image frame. The method further includes comparing the first and second frames and generating motion estimates from a result of the comparing. The method further includes repeating the foregoing generating and receiving while aiming the first and second beams at a second fraction of the field of view to generate successive image frames covering the entire field of view. The method further includes combining the motion estimates and successive image frames to generate an output signal indicating tissue deformation in said body structure as well as the movement of anatomical features of said body structure.

The output signal may represents a video sequence. The combining may include compensating gross motion information represented in the successive image frames.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound, comprising: generating a first beam aimed at the body structure. The method includes receiving multiple beams from a received echo to generate an image frame. The method includes repeating the foregoing generating and receiving to generate successive image frames covering the entire field of view. The method further includes cross-correlating the image frames to generate motion estimates. The method further includes combining the motion estimates and the successive image frames to generate an output signal indicating tissue

deformation in said body structure as well as the movement of anatomical features of said body structure.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound. The method includes generating a first and second beams simultaneously from a first ultrasound transmission and focused at first respective regions of the body structure. The method further includes generating a third and fourth beams simultaneously from a second ultrasound transmission and focused at second respective regions of the body structure. The method includes receiving echos to generate an image frame from the foregoing generating. The method further includes repeating the foregoing generating and receiving to generate successive image frames covering the entire field of view and cross-correlating the image frames to generate motion estimates. The method further includes combining the motion estimates and the successive image frames to generate an output signal indicating tissue deformation in said body structure as well as the movement of anatomical features of said body structure.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound. The method includes imaging a field of view in multiple sectors, the images for each sector being taken sequentially at first frame rate. The method further includes reconstructing a composite image of the entire field of view by appending the images for each sector together. estimating motion corresponding to the first frame rate from the images for respective sectors and combining with the composite image.

The method may further include repeating the imaging and reconstructing to form a composite image sequence.

In any of the disclosed methods, the motion estimates may include axial displacement magnitude. Also, in any of the disclosed methods, the image frames may include phase information and the motion estimation may be generated by comparing phase information of the reflected ultrasound.

According to embodiments, the disclosed subject matter includes an ultrasound method for acquiring sequential images of a target sample that moves in a unique pattern over an interval of a single movement cycle, the method being for constructing an image sequence of fractional image frames from a plurality of beam lines. The beam lines are spatially separated from each other. The method includes varying an acquisition order of multiple beam lines, a beam line size, and/or a shape of a beam focus over the interval of the single movement cycle to acquire successive fractions of the movement cycle during the single movement cycle.

The varying the acquisition order may include: dividing an image frame into a plurality of image frame sectors, sequentially imaging the image frame sectors over multiple frames, and combining the acquired image frame sectors to obtain a complete image of the target sample.

The varying the acquisition order may include acquiring a plurality of lines in a first region of the target sample before acquiring lines from an adjacent region thereby increasing locally the line

density (i.e., temporally-unequispaced acquisition sequences (TUAS)). The varying the acquisition order may include acquiring the same line in a target region before the end of a frame acquisition, thereby reducing the time between consecutive lines (i.e., temporally-unequispaced acquisition sequences (TUAS)). The varying the acquisition order may include acquiring a plurality of lines in a first region of the target sample before acquiring lines from an adjacent region thereby increasing locally the line density and acquiring the same line in a target region before the end of a frame acquisition, thereby reducing the time between consecutive lines (i.e., temporally-unequispaced acquisition sequences (TUAS)). The varying the size and/or shape of the beam focus may include transmitting a limited number of the available beam lines over the target sample, each transmission including multiple beam lines, thereby generating multiple focused transmit events scanned across a field of view (i.e., focused sequences). The varying the size and/or shape of the beam focus may include transmitting all available beam lines at the same time across the target sample thereby generating a single transmit event distributed over a field of view (i.e., plane-wave or flash sequences). The varying the size and/or shape of the beam focus may include sequentially scanning spatially separated beam lines across the target sample while varying the size of the focus thereby controlling the size of the focus and the number of lines per transmit (i.e., partially-defocused sequences). The varying the size and/or shape of the beam focus may include generating multiple focus points for each beam line transmit (i.e., multi-foci sequences).

According to embodiments, the disclosed subject matter includes a method of identifying an optimal sequence acquisition method for electromechanical wave imaging (EWI) of a target sample. The method includes (a) performing an image sequence acquisition on a target sample to reconstruct an image of the target sample according to any of the describe methods. The method further includes (b) estimating axial, lateral, and/or elevational displacements based on the image obtained from (a). and comparing the results in (b) with previously generated axial, lateral, and/or elevational displacements. The previously generated axial, lateral, and/or elevational displacements may be generated at an optimal frame rate.

According to embodiments, the disclosed subject matter includes a system to generate a cardiac activity map of a target sample. The system has a plurality of electrodes positioned along a portion of the target sample to detect electrical activity at respective locations and a measuring device connected to the plurality of electrodes and configured to measure potential differences between adjacent electrodes and generate corresponding data signals. The system further includes a processing device adapted to process the data signals received from the measuring device and to generate a 3D electrical activation map based on the processed signals and a display device to display the generated electrical activation map.

The system may further include a device for filtering and amplifying the data signals prior to generating the electrical activation map. The device may include a printed circuit board. The system may further include a controlling device to control the pacing of the target sample.

According to embodiments, the disclosed subject matter includes a method of imaging a biological tissue. The method includes capturing at least two successive frames of a first subsection of the biological tissue. The method further includes subsequently capturing at least two successive frames of a second subsection of the biological tissue. The method further includes generating a still or moving image of the combined first and second subsections from both the at least two successive frames and generating motion estimation data respective to each of the first and second subsections from the respective at least two successive frames corresponding to the each of the first and second subsections from a comparison of the each of the at least two successive frames.

The capturing may include imaging with ultrasound.

According to embodiments, the disclosed subject matter includes a method of imaging biological tissue including using ultrasound to acquire image sequence data representing motion of the biological tissue at a first frame rate and also motion information at a second frame rate that is faster than the second frame rate by scanning each of the respective subsections of the biological tissue at the second frame rate at least enough times to produce motion estimation data for the respective subsection, and scanning multiple subsections in the aggregate at least enough times for form the image sequence.

The method may further include superposing the motion estimation or data derived therefrom onto an image sequence captured at the first frame rate. The method may further include scanning a first subsection twice and scanning a second subsection twice, then returning to the first subsection and repeating. The biological tissue may be a myocardium.

According to embodiments, the disclosed subject matter includes a method of imaging a electromechanical wave by using ultrasound to capture a moving image of a myocardium at a first frame rate over a single cardiac cycle, the capturing including scanning to permit the acquisition of motion estimates from motion estimation frames representing images of a fraction of the myocardium where a time difference between the motion estimation frames is shorter than the inverse of the first frame rate.

According to embodiments, the disclosed subject matter includes a method of generating ultrasound motion information. The method includes scanning multiple A or RF beam lines to obtain spatial information of a target medium. The scanning includes scanning beam lines separated by a first spatial separation over a first spatial scanning range and separated by a second spatial separation over a second spatial scanning range to capture a first frame and repeating for multiple frames to obtain locally higher line density in a first region of the target medium and lower line density in a second region of the target medium to capture a first frame and repeating for multiple frames to obtain locally higher line density in a first region of the target medium and lower line density in a second region of the target medium.

According to embodiments, the disclosed subject matter includes a method of generating ultrasound motion information including scanning multiple A or RF beam lines to obtain spatial

information of a target medium, the scanning including scanning a first beam line a selected number of times, at least twice in succession, to obtain a higher motion estimation rate along the first beam line than a frame rate, and repeating for multiple frames.

According to embodiments, the disclosed subject matter includes a method of generating ultrasound motion information that includes the two foregoing methods in combination.

According to embodiments, the disclosed subject matter includes an ultrasound method for acquiring sequential images of a target sample for reconstructing an image frame from a plurality of beam lines, the lines is spatially separated from each other. The method includes acquiring a plurality of lines in a first region of the target sample before acquiring lines from an adjacent region thereby increasing locally the line density.

According to embodiments, the disclosed subject matter includes an ultrasound method for acquiring sequential images of a target sample for reconstructing an image frame from a plurality of beam lines, the lines being spatially separated from each other. The method includes acquiring the same line in a target region before the end of the frame acquisition, thereby reducing the time between two consecutive lines.

According to embodiments, the disclosed subject matter includes a system for mapping transient deformations of a myocardium resulting from electrical activation (i.e., electromechanical wave imaging) within a single heartbeat using an ultrasound method as in any of the described method.

According to embodiments, the disclosed subject matter includes a system for detecting and characterizing periodic and non-periodic cardiac events using electromechanical wave imaging within a single heartbeat using any of the methods described herein.

Note that the mentioned non-periodic events may include arrhythmias, such as fibrillation.

According to embodiments, the disclosed subject matter includes a method for mapping transient deformations of the myocardium within a single heartbeat at an optimal frame rate, wherein the optimal frame rate includes a frame rate which is adapted to accurately estimate cardiac deformations.

According to embodiments, the disclosed subject matter includes a method for identifying an optimal frame rate for electromechanical imaging of the target sample. The method includes varying a frame rate while maintaining a set of imaging parameters constant and determining the optimal frame rate based on an elastographic signal-to-noise ratio.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound. The method includes scanning the body structure using multiple focused beams from a phased ultrasound array of transducer elements according to a predefined sequence. The beams form spatially adjacent groups. The sequence defines the temporal order in which the beams are transmitted. The sequence is such that each spatially

adjacent group is transmitted twice a predetermined interval apart before another spatially adjacent group is transmitted.

The scanning may be performed using a phased array of transducer elements. The body structure may be a myocardium. The method may be applied for body structures that are myocardium and with no external source of motion other than the natural motion of the myocardium and the ultrasound used for scanning is present. The time difference between the successive transmits used to capture motion estimation data may be selected responsively to an estimate of image cross-correlation or noise.

In any of the disclosed methods, the time difference between the successive transmits used to capture motion estimation data may be selected responsively to a probabilistic estimate of signal to noise ratio.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound. The method includes generating single temporal sequence of spatially separated ultrasound transmission beams ordered in time. A fraction of the beams are principal beams and the remaining are divided among the principal beams, with multiple beams corresponding to each principal beam forming a corresponding block. Each principal beam is separated in time from its respective block by a predetermined motion estimation time interval, wherein the time difference between a principal beam and its corresponding block is taken as the time difference between one of its members and the principal beam. The beams of each block are mutually temporally adjacent (i.e., generated one right after the other without any other intervening beams). Each principal beam is separated from the members of its corresponding block by a predefined distance.

The predefined distance may be selected responsively to the rate and variability of the movement of the target structure and the fixed time interval such that an axial pattern imaged by the reference beam is identifiable the fixed time interval later (or prior) in an image from at least one of the members of the corresponding block. The at least one of the blocks may be transmitted before its corresponding principal beam. The at least one of the principal beams may be transmitted before its corresponding block. The predefined distance may vary by region of the target structure or time depending on a predicted rate of motion of the region of the target structure. The predefined distance may vary by region of the target structure or time responsively to a predicted rate of motion of the region of the target structure. The members of each block may be arrayed in two dimensions around its corresponding principal beam. The members of each block may be three in number. The members of each block may vary in number and average between 2 and four in number.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound, comprising: at a first time, transmitting a reference beam and subsequently transmitting corresponding comparison beams where each comparison beam is spatially separated from the reference beam within a range of displacements

around the reference beam, the range of displacement being selected responsively to a predicted rate of displacement and a time interval T_{ms} between the reference and one of the comparison beams. The method including, at a second time, transmitting multiple comparison beams, the comparison beams is spatially separated from another reference beam, the another reference beam not yet being transmitted at the second time, located within a range displacements which are also responsive to the predicted rate of displacement and the time interval T_{ms} , after the second time. The method including transmitting the another reference beam the time interval T_{ms} later, the reference beam being located spatially adjacent, the corresponding comparison beams. The comparison beams may correspond to a given reference beam are mutually temporally adjacent, i.e., they are transmitted together without any other beams is transmitted temporally between them. The the another reference beam may be spatially between the corresponding reference beams.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound, comprising: scanning the body structure using ultrasound to generate a series of image frames at an sampling rate, each image representing the configuration of the body structure at a point in time and spanning a field of view of an ultrasound scanner. the scanning including capturing displacements of portions of the body structure at intervals less than an inverse of the sampling rate.

According to embodiments, the disclosed subject matter includes a method for estimating properties of motion of a body structure using ultrasound, comprising: receiving a first input signal from a user interface representing data indicating a sampling rate. The method includes receiving a second input signal from a user interface data indicating a motion estimation frequency. The method includes scanning the body structure using ultrasound to generate a series of image frames at the sampling rate, each image representing the configuration of the body structure at a point in time and spanning a field of view of an ultrasound scanner. The scanning may include capturing displacements of portions of the body structure at the motion estimation frequency. outputting a result of said scanning in the form of an image sequence showing representations of the image frames as a video sequence with motion data responsive to the displacements superposed thereon. The time difference between the successive transmits used to capture motion estimation data may be selected responsively to a predicted quality of the motion estimates based on strain in the body structure. The time difference between the successive transmits used to capture motion estimation data may be selected responsively to a predicted quality of the motion estimates based on strain in the body structure and random error. The method of any of the foregoing claims wherein the time difference between the successive transmits used to capture motion estimation data is selected responsively to a predicted quality of the motion estimates based on an optimum responsive to a random signal component and a competing distortion of the motion estimation resulting from strain, i.e., motion other than pure displacement.

According to embodiments, the disclosed subject matter includes a system for estimating properties of motion of a body structure using ultrasound, comprising: an ultrasound probe connected to a driver and data acquisition element and a programmable processor with a user interface having a display and a data storage element. The system includes software instructions recorded on the data storage element, the software instructions defining a procedure for operating at least the ultrasound probe, driver and data acquisition element in order to execute the method of any of the foregoing claims.

According to embodiments, the disclosed subject matter includes a system for estimating properties of motion of a structure using ultrasound, comprising: at least one ultrasound probe configured to scan a structure using ultrasound. a controller configured to control the at least one ultrasound probe to transmit ultrasonic beams into the structure and receive echoes thereof. The controller is further configured to transmit multiple beams repeatedly over an inspection interval such that the echoes may be used to form a representation of the structure over the entire spatial scope of detection of the ultrasound probe which can be updated no more frequently than a sample frequency. The controller is further configured such that the echoes may be used to determine displacements of portions of the structure occurring within fractions of the spatial scope of detection and within fractions of the sample frequency.

The controller may be configured to accept data representing a magnitude T_{me} of said fractions of the sample frequency. T_{me} may represent the time separation between image samples of said portions of the structure generated by said controller responsively to said echoes. T_{me} may be selected responsively to a predicted or measured maximum of a cross-correlation time scale between said image samples.

The controller may transmit beams in pairs at a frequency that is greater than the sample frequency, where each pair covers less than the spatial scope of detection.

It will be appreciated that the modules, processes, systems, and sections described above can be implemented in hardware, hardware programmed by software, software instruction stored on a non-transitory computer readable medium or a combination of the above. For example, a method for imaging can be implemented using a processor configured to execute a sequence of programmed instructions stored on a non-transitory computer readable medium. For example, the processor can include, but not be limited to, a personal computer or workstation or other such computing system that includes a processor, microprocessor, microcontroller device, or is comprised of control logic including integrated circuits such as, for example, an Application Specific Integrated Circuit (ASIC). The instructions can be compiled from source code instructions provided in accordance with a programming language such as Java, C++, C#.net or the like. The instructions can also

comprise code and data objects provided in accordance with, for example, the Visual Basic™ language, LabVIEW, or another structured or object-oriented programming language. The sequence of programmed instructions and data associated therewith can be stored in a non-transitory computer-readable medium such as a computer memory or storage device which may be any suitable memory apparatus, such as, but not limited to read-only memory (ROM), programmable read-only memory (PROM), electrically erasable programmable read-only memory (EEPROM), random-access memory (RAM), flash memory, disk drive and the like.

Furthermore, the modules, processes, systems, and sections can be implemented as a single processor or as a distributed processor. Further, it should be appreciated that the steps mentioned above may be performed on a single or distributed processor (single and/or multi-core). Also, the processes, modules, and sub-modules described in the various figures of and for embodiments above may be distributed across multiple computers or systems or may be co-located in a single processor or system. Exemplary structural embodiment alternatives suitable for implementing the modules, sections, systems, means, or processes described herein are provided below.

The modules, processors or systems described above can be implemented as a programmed general purpose computer, an electronic device programmed with microcode, a hard-wired analog logic circuit, software stored on a computer-readable medium or signal, an optical computing device, a networked system of electronic and/or optical devices, a special purpose computing device, an integrated circuit device, a semiconductor chip, and a software module or object stored on a computer-readable medium or signal, for example.

Embodiments of the method and system (or their sub-components or modules), may be implemented on a general-purpose computer, a special-purpose computer, a programmed microprocessor or microcontroller and peripheral integrated circuit element, an ASIC or other integrated circuit, a digital signal processor, a hardwired electronic or logic circuit such as a discrete element circuit, a programmed logic circuit such as a programmable logic device (PLD), programmable logic array (PLA), field-programmable gate array (FPGA), programmable array logic (PAL) device, or the like. In general, any process capable of implementing the functions or steps described herein can be used to implement embodiments of the method, system, or a computer program product (software program stored on a non-transitory computer readable medium).

Furthermore, embodiments of the disclosed method, system, and computer program product may be readily implemented, fully or partially, in software using, for example, object or object-oriented software development environments that provide portable source code that

can be used on a variety of computer platforms. Alternatively, embodiments of the disclosed method, system, and computer program product can be implemented partially or fully in hardware using, for example, standard logic circuits or a very-large-scale integration (VLSI) design. Other hardware or software can be used to implement embodiments depending on the speed and/or efficiency requirements of the systems, the particular function, and/or particular software or hardware system, microprocessor, or microcomputer being utilized.

Embodiments of the method, system, and computer program product can be implemented in hardware and/or software using any known or later developed systems or structures, devices and/or software by those of ordinary skill in the applicable art from the function description provided herein and with a general basic knowledge of ultrasonography and/or computer programming arts.

Moreover, embodiments of the disclosed method, system, and computer program product can be implemented in software executed on a programmed general purpose computer, a special purpose computer, a microprocessor, or the like.

It is, thus, apparent that there is provided, in accordance with the present disclosure, imaging methods devices and systems. Many alternatives, modifications, and variations are enabled by the present disclosure. Features of the disclosed embodiments can be combined, rearranged, omitted, etc., within the scope of the invention to produce additional embodiments. Furthermore, certain features may sometimes be used to advantage without a corresponding use of other features. Accordingly, Applicants intend to embrace all such alternatives, modifications, equivalents, and variations that are within the spirit and scope of the present invention.

Claims

What is claimed is:

1. An ultrasound system for imaging a target structure that moves or deforms with time, comprising:
 - an ultrasound imaging device configured to image at a spatial resolution and sample a predefined field of view no faster than a frequency $1/T_{ms}$;
 - the target structure being one which moves or deforms such that relative displacement of portions of the target structure of a size equal to the inverse of the spatial resolution are substantially uncorrelated at time intervals greater than a time interval T_{me} ;
 - the target structure being one where relative displacements propagate over time scales many times greater than T_{me} where T_{me} is much smaller than T_{ms} ;
 - a controller configured to control the ultrasound imaging device to image the target structure at a frequency of $1/T_{me}$ and to capture relative displacement data responsive thereto;
 - the controller being further configured to generate an image sequence representing the field of view in which the relative displacement data is shown on the image sequence.
2. The system of claim 1, wherein the controller is configured to acquire multiple first image frames consecutively in time which first image frames are smaller than the field of view.
3. The system of claim 2, wherein the controller is configured to assemble first image frames to form second image frames spanning the field of view.
4. A method for estimating properties of motion of a body structure, comprising:
 - directing at least a first ultrasonic beam into a first angular sector of the body structure;
 - directing at least a second ultrasonic beam into a second angular sector of the body structure;
 - directing at least a third ultrasonic beam into the first angular sector of the body structure prior to the directing at least a second ultrasonic beam into the second angular sector of the body structure;
 - detecting motion of the body structure in the first angular sector by detecting a magnitude of a displacement of a portion of the body structure occurring between return echoes from the at least a first ultrasonic beam and the at least a third ultrasonic beam.
5. A method for estimating properties of motion of a body structure, comprising:

directing a first at least three ultrasonic beams into respective angular sectors of the body structure, the angular sectors combining to span a field of view of an ultrasonic transducer, wherein the beams are separated by at least first and second angular intervals so that the angular beam density varies over the field of view;

repeating said directing for a second at least three ultrasonic beams;

receiving return echoes from the first and second at least three ultrasonic beams;

detecting motion of the body structure by detecting a magnitude of a displacement of a portion of the body structure occurring between the return echoes from the at least three ultrasonic beams.

6. A method for estimating properties of motion of a body structure, comprising:
generating a reference ultrasound scan of region of the body structure at a selected axial depth using a pattern of first beams distributed over a first angular range and directed at respective first angles; and

generating a comparison ultrasound scan of the region of the body structure at the selected axial depth using a second pattern of beams distributed over substantially the first angular range and directed at respective second angles;

the first angles and the second angles being non-collinear.

7. The method of claim 6, wherein the first angles are distributed over a solid angular ranges.

8. The method of claim 6, wherein the first and second angles are distributed over solid angular ranges.

9. The method of claim 6 or 8, wherein the first angles lie between respective ones of the second angles.

10. A method for estimating properties of motion of a body structure, comprising:
generating a first reference ultrasound scan of a region of the body structure at a selected axial depth using a pattern of first beams distributed over a first angular range and directed at respective first angles; and

generating a first comparison ultrasound scan of the region of the body structure at the selected axial depth using a second pattern of beams distributed over substantially the first angular range and directed at respective second angles;

generating a second reference ultrasound scan of region of the body structure at a selected axial depth using a pattern of first beams distributed over a second angular range and directed at respective third angles; and

generating a second comparison ultrasound scan of the region of the body structure at the selected axial depth using a second pattern of beams distributed over substantially the second angular range and directed at respective fourth angles;

the first, second, third, and fourth angles being non-collinear.

11. The method of claim 6, wherein the first angular range is a solid angular range.

12. The method of claim 6, wherein the first and second angular range is a solid angular range.

13. The method of claim 6 or 8, wherein the first angles lie between respective ones of the second angles.

14. A method for estimating properties of motion of a body structure, comprising: directing, into the body structure, first and second broad ultrasound beams in respective first and second transmit events;

for each of the transmit events, forming multiple receive beams to form first images of said body structure at first and second times;

generating motion information by comparing the first images;

generating first and second ultrasound image scans using focused beams generated by first and second sets of transmit events;

the first and second transmit events and the first and second sets of transmit events all occurring during a single motion event of said body structure.

15. The method of claim 14, wherein the single motion event is induced by an electromechanical wave in a heart muscle.

16. The method of claim 14, wherein the first set of transmit events occurs at a time between the first and second transmit events.

17. The method of claim 14 or 16, wherein the first and second transmit events and the first and second sets of transmit events have substantially the same spatial scope.

18. The method of claim 14 or 16, further comprising generating a B-mode image responsively to the first and second ultrasound scans and overlaying motion data resulting from the step of generating motion information.

19. The method of claim 14 or 16, further comprising generating a B-mode image sequence responsively to the first and second ultrasound scans and overlaying motion data resulting from the step of generating motion information.

20. A high frame rate ultrasound image acquisition method, comprising:

generating waveforms with respective time delays and respective apodization weightings determined to cause selected transducer elements of a transducer array to transmit respective transmit beams along corresponding transmit beam paths toward a body structure to be imaged during a first transmit event such that the first transmit event is distributed over a first portion of a field of view, followed by transmission of respective transmit beams along corresponding transmit beam paths during a second transmit event distributed over a second portion of the field of view;

acquiring a first plurality of spatially separated beam lines at selected transducer elements during a first receive event subsequent to said first transmit event along corresponding receive beam paths, and acquiring a second plurality of spatially separated beam lines at selected transducer elements during a second receive event subsequent to said second transmit event along corresponding receive beam paths,

wherein the first plurality of spatially separated beam lines are acquired multiple times in succession before acquiring the second plurality of spatially separated beam lines.

21. A method for estimating properties of motion of a body structure using ultrasound, comprising:

- a) directing a first beam into the body structure;
- b) directing multiple second beams into the body structure;

where a and b are repeated in the sequence: at least two a) events followed by at least one b) event which sub-sequence is repeated multiple times with each sequence being the same or different from other sequences;

from multiple a) events, estimating the displacement of anatomical portions of said body structure to generate at least first motion estimates from echoes of the first beams;

from multiple b) events, estimating at least the relative positions of anatomical portions of said body structure from echoes of said second beams over time to generate images of said body structure; and

combining the images and first motion estimates to form a display indicating motion within the body structure.

22. The method of claim 21, wherein the first beams are wider than the second beams.

23. The method of claim 21, wherein the first beams are parallel beams.

24. The method of claim 21, wherein the first beams single pulses spanning a field of view of the body structure.

25. A method for estimating properties of motion of a body structure using ultrasound, comprising:

- generating a first beam aimed a first fraction of a field of view of the body structure;
- receiving multiple beams from a received echo to generate a first image frame;
- generating a second beam aimed the first fraction of the field of view of the body structure;
- receiving multiple beams from a received echo to generate a second image frame;
- comparing the first and second frames and generating motion estimates from a result of the comparing;
- repeating the foregoing generating and receiving while aiming the first and second beams at a second fraction of the field of view to generate successive image frames covering the entire field of view;
- combining the motion estimates and successive image frames to generate an output signal indicating tissue deformation in said body structure as well as the movement of anatomical features of said body structure.

26. The method of claim 25, wherein the output signal represents a video sequence.

27. The method of claim 25, wherein the combining includes compensating gross motion information represented in the successive image frames.

28. A method for estimating properties of motion of a body structure using ultrasound, comprising:

- generating a first beam aimed at the body structure;
- receiving multiple beams from a received echo to generate an image frame;
- repeating the foregoing generating and receiving to generate successive image frames covering the entire field of view;
- cross-correlating the image frames to generate motion estimates;
- combining the motion estimates and the successive image frames to generate an output signal indicating tissue deformation in said body structure as well as the movement of anatomical features of said body structure.

29. A method for estimating properties of motion of a body structure using ultrasound, comprising:

- generating a first and second beams simultaneously from a first ultrasound transmission and focused at first respective regions of the body structure;

generating a third and fourth beams simultaneously from a second ultrasound transmission and focused at second respective regions of the body structure;
receiving echos to generate an image frame from the foregoing generating;
repeating the foregoing generating and receiving to generate successive image frames covering the entire field of view;
cross-correlating the image frames to generate motion estimates;
combining the motion estimates and the successive image frames to generate an output signal indicating tissue deformation in said body structure as well as the movement of anatomical features of said body structure.

30. A method for estimating properties of motion of a body structure using ultrasound, comprising:

imaging a field of view in multiple sectors, the images for each sector being taken sequentially at first frame rate;

reconstructing a composite image of the entire field of view by appending the images for each sector together;

estimating motion corresponding to the first frame rate from the images for respective sectors and combining with the composite image.

31. The method of claim 30, further comprising repeating the imaging and reconstructing to form a composite image sequence.

32. The method of any of the above claims, wherein the motion estimates include axial displacement magnitude.

33. The method of any of the above claims, wherein image frames include phase information and the motion estimation is generated by comparing phase information of the reflected ultrasound.

34. An ultrasound method for acquiring sequential images of a target sample that moves in a unique pattern over an interval of a single movement cycle, the method being for constructing an image sequence of fractional image frames from a plurality of beam lines, the beam lines being spatially separated from each other, the method comprising: varying an acquisition order of multiple beam lines, a beam line size, and/or a shape of a beam focus over the interval of the single movement cycle to acquire successive fractions of the movement cycle during the single movement cycle.

35. The method as claimed in claim 34, wherein the varying the acquisition order includes: dividing an image frame into a plurality of image frame sectors; sequentially

imaging the image frame sectors over multiple frames; and combining the acquired image frame sectors to obtain a complete image of the target sample (i.e., composite imaging).

36. The method as claimed in claim 34, wherein the varying the acquisition order includes acquiring a plurality of lines in a first region of the target sample before acquiring lines from an adjacent region thereby increasing locally the line density (i.e., temporally-unequispaced acquisition sequences (TUAS)).

37. The method of claim 34, wherein the varying the acquisition order includes acquiring the same line in a target region before the end of a frame acquisition, thereby reducing the time between consecutive lines (i.e., temporally-unequispaced acquisition sequences (TUAS)).

38. The method of claim 34, wherein the varying the acquisition order includes acquiring a plurality of lines in a first region of the target sample before acquiring lines from an adjacent region thereby increasing locally the line density and acquiring the same line in a target region before the end of a frame acquisition, thereby reducing the time between consecutive lines (i.e., temporally-unequispaced acquisition sequences (TUAS)).

39. The method of claim 34, wherein varying the size and/or shape of the beam focus includes transmitting a limited number of the available beam lines over the target sample, each transmission including multiple beam lines, thereby generating multiple focused transmit events scanned across a field of view (i.e., focused sequences).

40. The method of claim 34, wherein varying the size and/or shape of the beam focus includes transmitting all available beam lines at the same time across the target sample thereby generating a single transmit event distributed over a field of view (i.e., plane-wave or flash sequences).

41. The method of claim 34, wherein varying the size and/or shape of the beam focus includes sequentially scanning spatially separated beam lines across the target sample while varying the size of the focus thereby controlling the size of the focus and the number of lines per transmit (i.e., partially-defocused sequences).

42. The method of claim 34, wherein varying the size and/or shape of the beam focus includes generating multiple focus points for each beam line transmit (i.e., multi-foci sequences).

43. A method of identifying an optimal sequence acquisition method for electromechanical wave imaging (EWI) of a target sample, the method comprising:

(a) performing an image sequence acquisition method as claimed in any of the foregoing method claims on a target sample to reconstruct an image of the target sample;

(b) estimating axial and lateral and/or elevational displacements based on the image obtained from (a); and

(c) comparing the results in (b) with a previously generated axial, lateral and/or elevational displacements.

44. The method as claimed in claim 20, wherein the previously generated axial, lateral, and/or elevational displacements were generated at an optimal frame rate.

45. A system to generate a cardiac activity map of a target sample, the system comprising:

a plurality of electrodes positioned along a portion of the target sample to detect electrical activity at respective locations;

a measuring device connected to the plurality of electrodes and configured to measure potential differences between adjacent electrodes and generate corresponding data signals;

a processing device adapted to process the data signals received from the measuring device and to generate a 3D electrical activation map based on the processed signals; and

a display device to display the generated electrical activation map.

46. The system as claimed in claim 22, further comprising a device for filtering and amplifying the data signals prior to generating the electrical activation map.

47. The system as claimed in claim 23, wherein the device is a printed circuit board.

48. The system as claimed in claim 22, further comprising a controlling device to control the pacing of the target sample.

49. A method of imaging a biological tissue, comprising:
capturing at least two successive frames of a first subsection of the biological tissue;
subsequently capturing at least two successive frames of a second subsection of the biological tissue;

generating a still or moving image of the combined first and second subsections from both the at least two successive frames and generating motion estimation data respective to each of the first and second subsections from the respective at least two successive frames corresponding to the each of the first and second subsections from a comparison of the each of the at least two successive frames.

50. The method of claim 49, wherein the capturing includes imaging with ultrasound.

51. A method of imaging biological tissue, comprising: using ultrasound to acquire image sequence data representing motion of the biological tissue at a first frame rate

and also motion information at a second frame rate that is faster than the second frame rate by scanning each of the respective subsections of the biological tissue at the second frame rate at least enough times to produce motion estimation data for the respective subsection, and scanning multiple subsections in the aggregate at least enough times for form the image sequence.

52. The method of claim 51, further comprising superposing the motion estimation or data derived therefrom onto an image sequence captured at the first frame rate.

53. The method of claim 51, further comprising scanning a first subsection twice and scanning a second subsection twice, then returning to the first subsection and repeating.

54. The method of claim 51 or 53, wherein the biological tissue is a myocardium.

55. A method of imaging an electromechanical wave, comprising: using ultrasound to capture a moving image of a myocardium at a first frame rate over a single cardiac cycle, the capturing including scanning to permit the acquisition of motion estimates from motion estimation frames representing images of a fraction of the myocardium where a time difference between the motion estimation frames is shorter than the inverse of the first frame rate.

56. A method of generating ultrasound motion information, comprising: scanning multiple A or RF beam lines to obtain spatial information of a target medium, the scanning including scanning beam lines separated by a first spatial separation over a first spatial scanning range and separated by a second spatial separation over a second spatial scanning range to capture a first frame and repeating for multiple frames to obtain locally higher line density in a first region of the target medium and lower line density in a second region of the target medium to capture a first frame and repeating for multiple frames to obtain locally higher line density in a first region of the target medium and lower line density in a second region of the target medium.

57. A method of generating ultrasound motion information, comprising: scanning multiple A or RF beam lines to obtain spatial information of a target medium, the scanning including scanning a first beam line a selected number of times, at least twice in succession, to obtain a higher motion estimation rate along the first beam line than a frame rate, and repeating for multiple frames.

58. A method of generating ultrasound motion information, comprising combining the method as claimed in claim 1 with the method as claimed in claim 57.

59. An ultrasound method for acquiring sequential images of a target sample for reconstructing an image frame from a plurality of beam lines, the lines being spatially

separated from each other, the method comprising acquiring a plurality of lines in a first region of the target sample before acquiring lines from an adjacent region thereby increasing locally the line density.

60. An ultrasound method for acquiring sequential images of a target sample for reconstructing an image frame from a plurality of beam lines, the lines being spatially separated from each other, the method comprising acquiring the same line in a target region before the end of the frame acquisition, thereby reducing the time between two consecutive lines.

61. A system for mapping transient deformations of a myocardium resulting from electrical activation (i.e., electromechanical wave imaging) within a single heartbeat using an ultrasound method as claimed in any one of claims 56-60.

62. A system for detecting and characterizing periodic and non-periodic cardiac events using electromechanical wave imaging within a single heartbeat using the method as claimed in any one of claims 56-60.

63. The system of claim 61 or 62 wherein the non-periodic events may include arrhythmias, such as fibrillation.

64. A method for mapping transient deformations of the myocardium within a single heartbeat at an optimal frame rate, wherein the optimal frame rate includes a frame rate which is adapted to accurately estimate cardiac deformations.

65. A method for identifying an optimal frame rate for electromechanical imaging of the target sample, comprising:

- varying a frame rate while maintaining a set of imaging parameters constant; and
- determining the optimal frame rate based on an elastographic signal-to-noise ratio.

66. A method for estimating properties of motion of a body structure using ultrasound, comprising:

- scanning the body structure using multiple focused beams from a phased ultrasound array of transducer elements according to a predefined sequence, the beams forming spatially adjacent groups;

- the sequence defining the temporal order in which the beams are transmitted;

- the sequence being such that each of the spatially adjacent groups are transmitted twice a predetermined interval apart before another spatially adjacent group is transmitted.

67. The method of claim 66, wherein the scanning is performed using a phased array of transducer elements.

68. The method of claim 66 or 67 wherein the body structure is a myocardium.

69. The method of claim 66 or 67 wherein the body structure is a myocardium and no external source of motion other than the natural motion of the myocardium and the ultrasound used for scanning is present.

70. The method of any of the foregoing claims wherein the time difference between the successive transmits used to capture motion estimation data is selected responsively to an estimate of image cross-correlation or noise.

71. The method of any of the foregoing claims wherein the time difference between the successive transmits used to capture motion estimation data is selected responsively to a probabilistic estimate of signal to noise ratio.

72. A method for estimating properties of motion of a body structure using ultrasound, comprising:

- generating single temporal sequence of spatially separated ultrasound transmission beams ordered in time;

- a fraction of the beams being principal beams and the remaining being divided among the principal beams, with multiple beams corresponding to each principal beam forming a corresponding block;

- each principal beam is separated in time from its respective block by a predetermined motion estimation time interval, wherein the time difference between a principal beam and its corresponding block being taken as the time difference between one of its members and the principal beam;

- the beams of each block being mutually temporally adjacent (i.e., generated one right after the other without any other intervening beams);

- each principal beam being separated from the members of its corresponding block by a predefined distance.

73. The method of claim 72, wherein the predefined distance is selected responsively to the rate and variability of movement of the target structure and the fixed time interval such that an axial pattern imaged by the reference beam is identifiable the fixed time interval later (or prior) in an image from at least one of the members of the corresponding block.

74. The method of claim 72 or 73, wherein at least one of the blocks is transmitted before its corresponding principal beam.

75. The method of claim 71 or 74, wherein at least one of the principal beams is transmitted before its corresponding block.

76. The method of any of claims 71 to 75, wherein the predefined distance may vary by region of the target structure or time depending on a predicted rate of motion of the region of the target structure.

77. The method of any of claims 71 to 75, wherein the predefined distance varies by region of the target structure or time responsively to a predicted rate of motion of the region of the target structure.

78. The method of any of claims 71 to 77, wherein the members of each block are arrayed in two dimensions around its corresponding principal beam.

79. The method of any of claims 71 to 77, wherein the members of each block are three in number.

80. The method of any of claims 71 to 77, wherein the members of each block vary in number and average between 2 and four in number.

81. A method for estimating properties of motion of a body structure using ultrasound, comprising:

at a first time, transmitting a reference beam and subsequently transmitting corresponding comparison beams where each comparison beam is spatially separated from the reference beam within a range of displacements around the reference beam, the range of displacement being selected responsively to a predicted rate of displacement and a time interval T_{ms} between the reference and one of the comparison beams;

at a second time, transmitting multiple comparison beams, the comparison beams being spatially separated from another reference beam, the another reference beam not yet being transmitted at the second time, located within a range displacements which are also responsive to the predicted rate of displacement and the time interval T_{ms} ;

after the second time, transmitting the another reference beam the time interval T_{ms} later, the reference beam is located spatially adjacent, the corresponding comparison beams;

82. The method of claim 81, wherein the comparison beams corresponding to a given reference beam are mutually temporally adjacent, i.e., they are transmitted together without any other beams being transmitted temporally between them.

83. The method of claim 81 or 82, wherein the another reference beam is spatially between the corresponding reference beams.

84. A method for estimating properties of motion of a body structure using ultrasound, comprising:

scanning the body structure using ultrasound to generate a series of image frames at an sampling rate, each image representing the configuration of the body structure at a point in time and spanning a field of view of an ultrasound scanner;

the scanning including capturing displacements of portions of the body structure at intervals less than an inverse of the sampling rate.

85. A method for estimating properties of motion of a body structure using ultrasound, comprising:

receiving a first input signal from a user interface representing data indicating a sampling rate;

receiving a second input signal from a user interface data indicating a motion estimation frequency;

scanning the body structure using ultrasound to generate a series of image frames at the sampling rate, each image representing the configuration of the body structure at a point in time and spanning a field of view of an ultrasound scanner;

the scanning including capturing displacements of portions of the body structure at the motion estimation frequency;

outputting a result of said scanning in the form of an image sequence showing representations of the image frames as a video sequence with motion data responsive to the displacements superposed thereon.

86. The method of any of the foregoing claims wherein the time difference between the successive transmits used to capture motion estimation data is selected responsively to a predicted quality of the motion estimates based on strain in the body structure.

87. The method of any of the foregoing claims wherein the time difference between the successive transmits used to capture motion estimation data is selected responsively to a predicted quality of the motion estimates based on strain in the body structure and random error.

88. The method of any of the foregoing claims wherein the time difference between the successive transmits used to capture motion estimation data is selected responsively to a predicted quality of the motion estimates based on an optimum responsive to a random signal component and a competing distortion of the motion estimation resulting from strain, i.e., motion other than pure displacement.

89. A system for estimating properties of motion of a body structure using ultrasound, comprising:

an ultrasound probe connected to a driver and data acquisition element and a programmable processor with a user interface having a display and a data storage element; software instructions recorded on the data storage element, the software instructions defining a procedure for operating at least the ultrasound probe, driver and data acquisition element in order to execute the method of any of the foregoing claims.

90. A system for estimating properties of motion of a structure using ultrasound, comprising:

at least one ultrasound probe configured to scan a structure using ultrasound;
a controller configured to control the at least one ultrasound probe to transmit ultrasonic beams into the structure and receive echoes thereof;

the controller being further configured to transmit multiple beams repeatedly over an inspection interval such that the echoes may be used to form a representation of the structure over the entire spatial scope of detection of the ultrasound probe which can be updated no more frequently than a sample frequency;

the controller being further configured such that the echoes may be used to determine displacements of portions of the structure occurring within fractions of the spatial scope of detection and within fractions of the sample frequency.

91. The system of claim 90, wherein the controller is configured to accept data representing a magnitude T_{me} of said fractions of the sample frequency.

92. The system of claim 92 wherein T_{me} represents the time separation between image samples of said portions of the structure generated by said controller responsively to said echoes.

93. The system of claim 92 wherein T_{me} is selected responsively to a predicted or measured maximum of a cross-correlation time scale between said image samples.

94. The system of any of claims 91 through 94, wherein the controller transmits beams in pairs at a frequency that is greater than the sample frequency, where each pair covers less than the spatial scope of detection.

95. A method of identifying an optimal sequence acquisition method for electromechanical wave imaging (EWI) of a target sample, the method comprising:

- (a) performing an image volume sequence acquisition method as claimed in any one of claims 1-14 on a target sample to reconstruct an image volume of the target sample;
- (b) estimating axial, lateral and elevational displacements based on the image obtained from (a); and

(c) comparing the results in (b) with a previously generated axial, lateral and elevational displacements.

96. A method as in any of the above method claims wherein the body structure is a heart muscle and the motion is a result of a deformation of the heart muscle.

97. The method of claim 96 wherein the single motion is induced by a deformation in a heart muscle.

98. In any of the above claims, wherein motion is detected in all three or any two of axial, lateral and elevational directions.

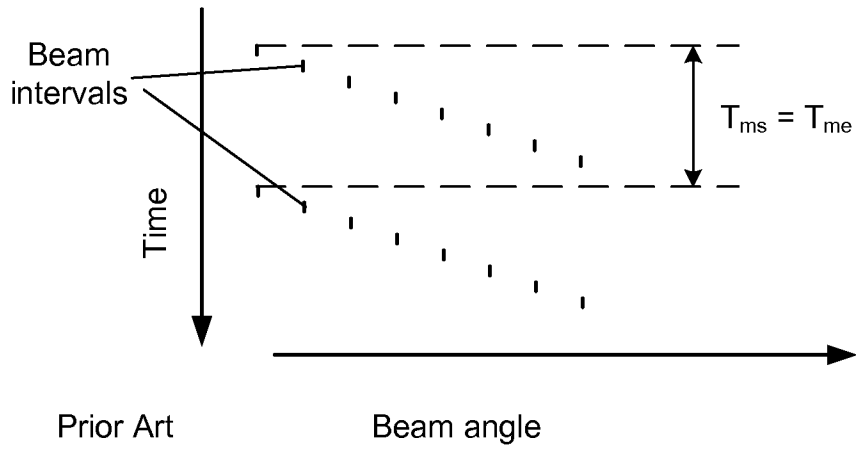


Fig. 1A

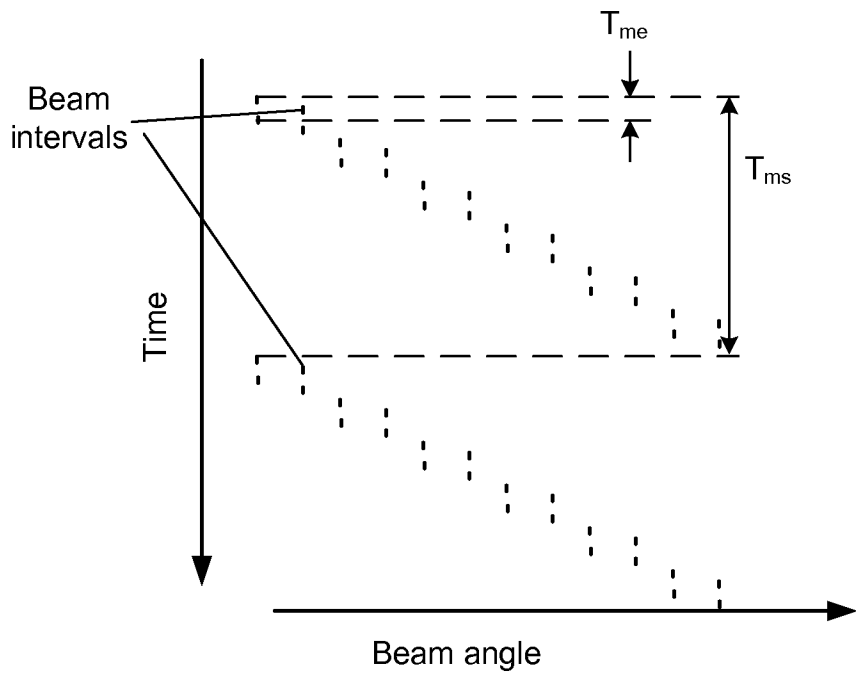


Fig. 1B

2/11

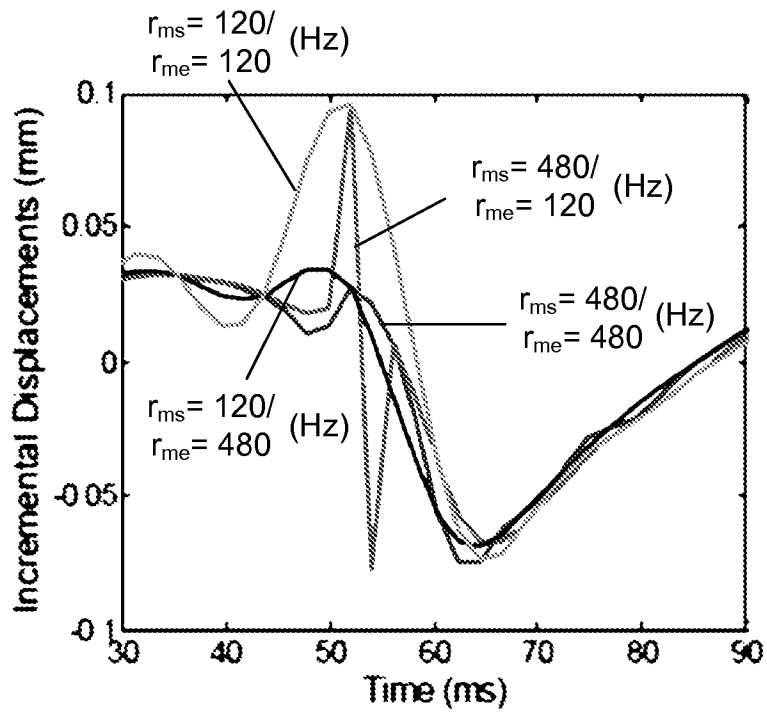


Fig. 2

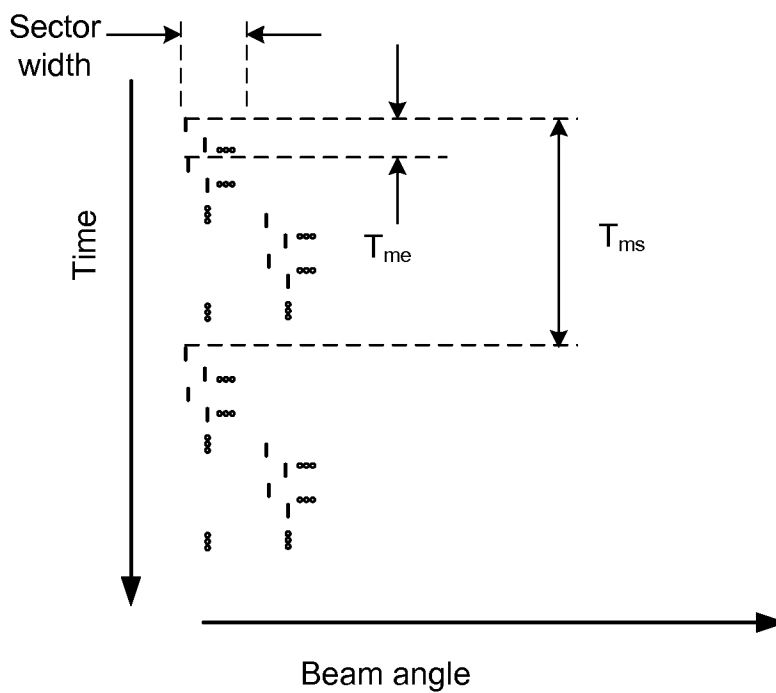


Fig. 3

3/11

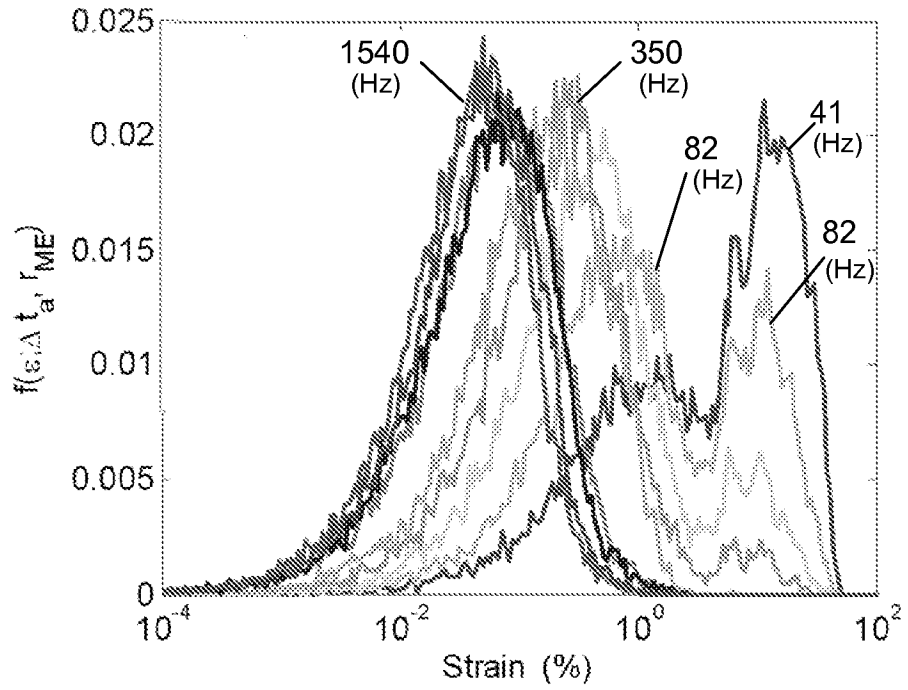


Fig. 4

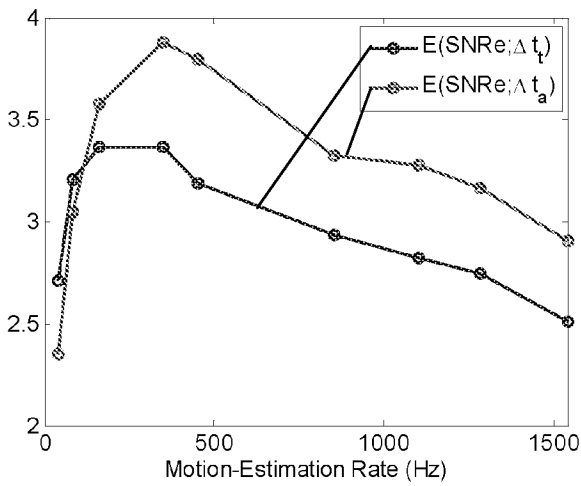


Fig. 5A

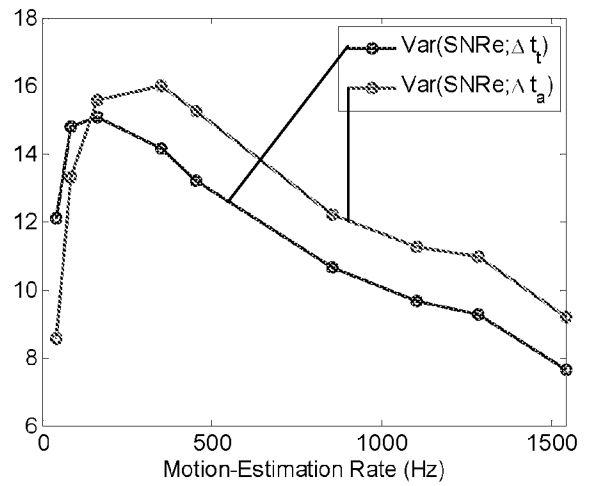


Fig. 5B

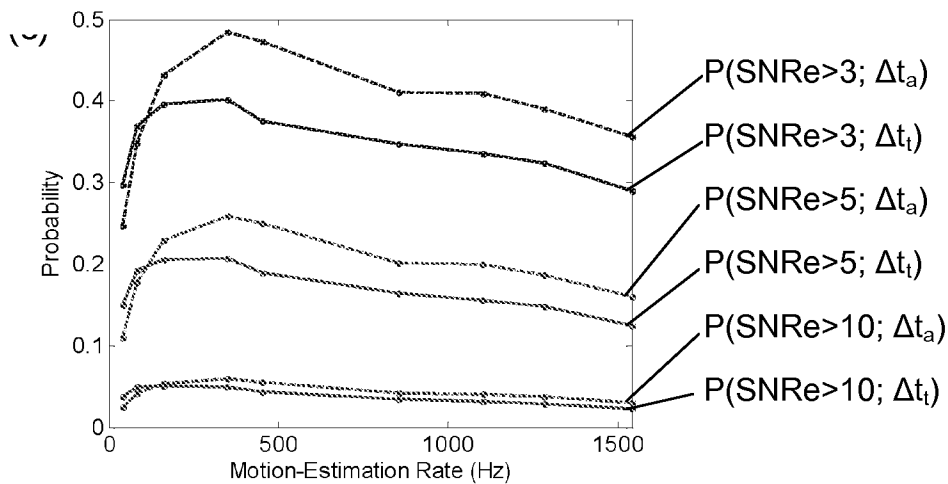


Fig. 5C

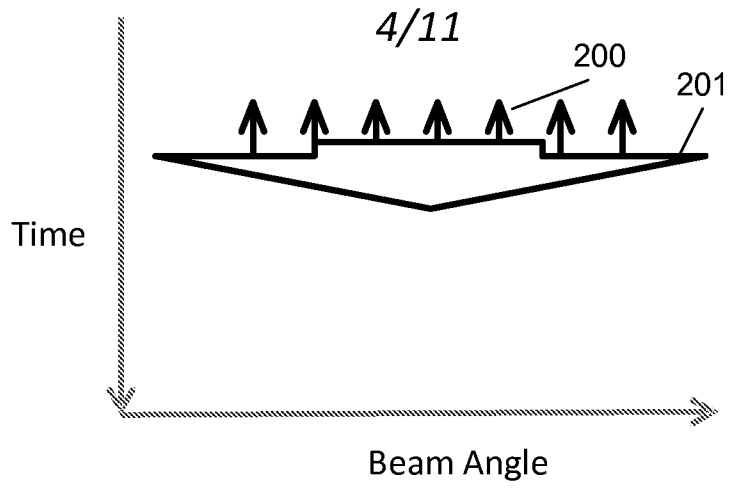


Fig. 6A

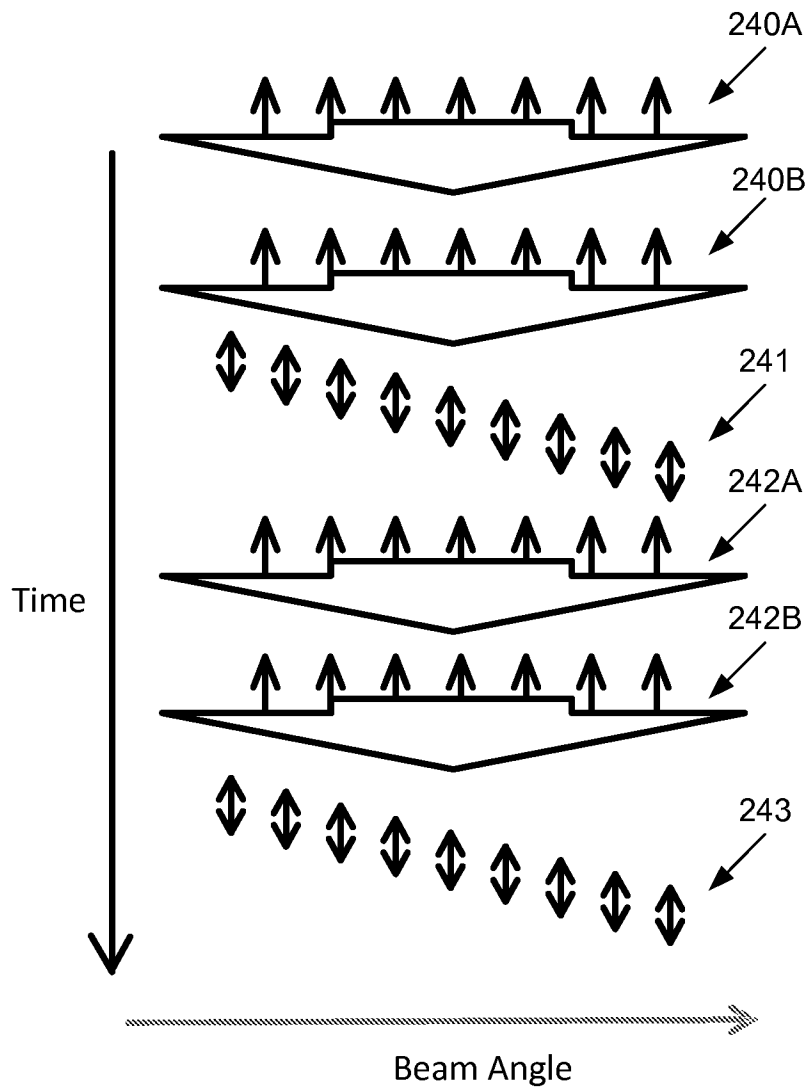


Fig. 6B

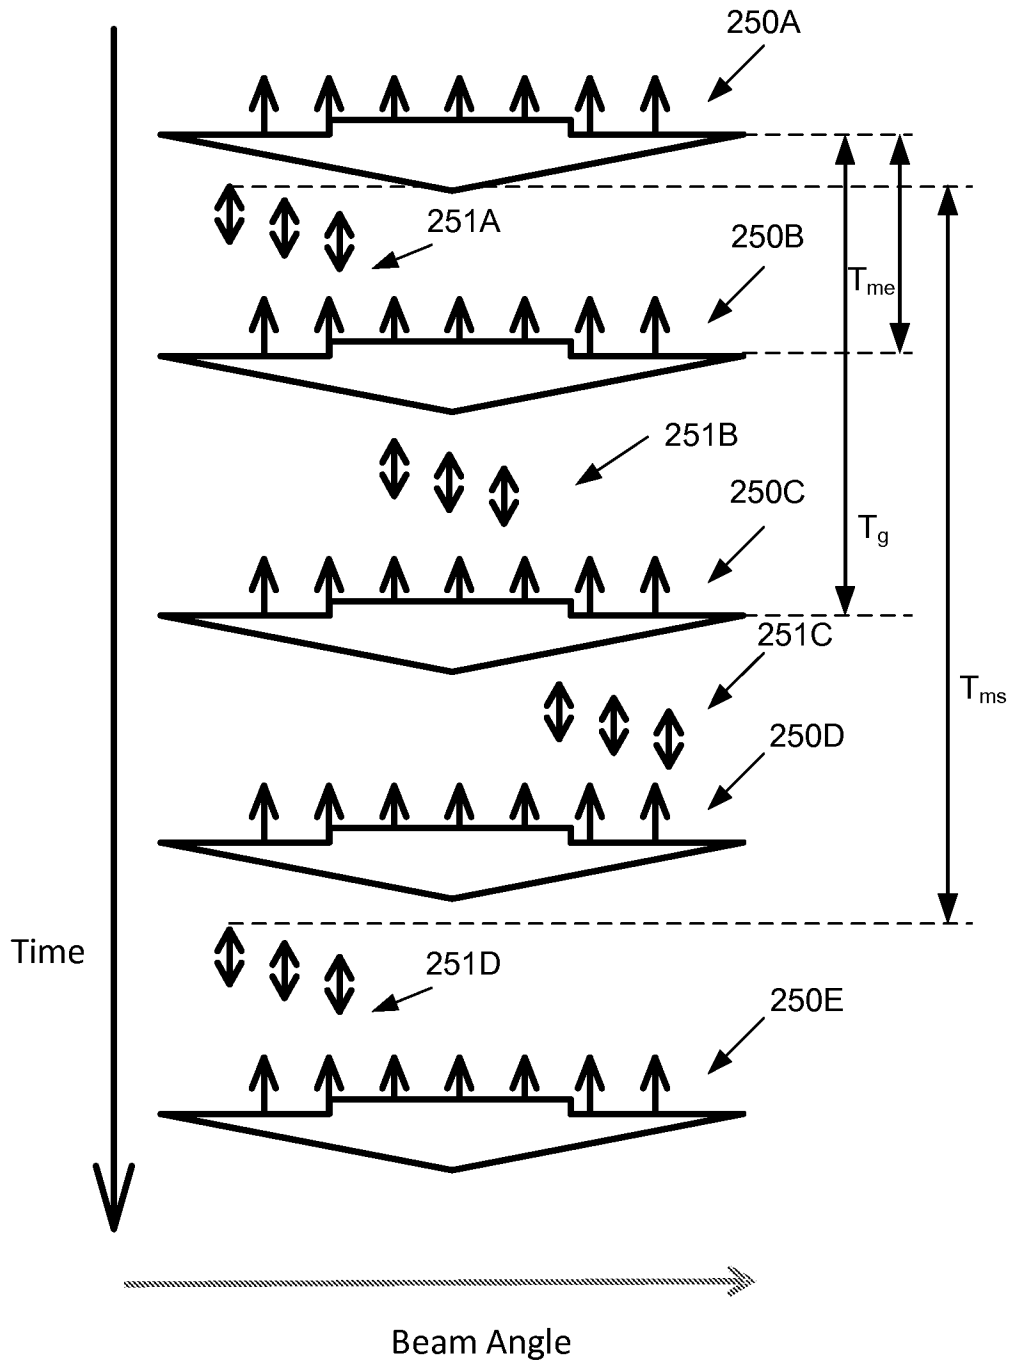


Fig. 6C

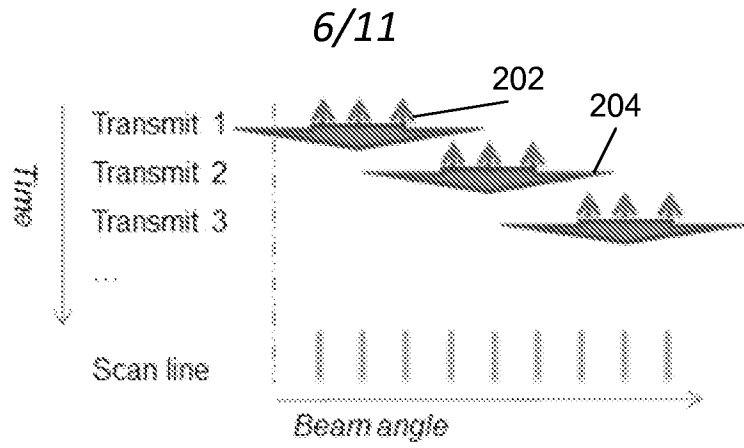


Fig. 7A

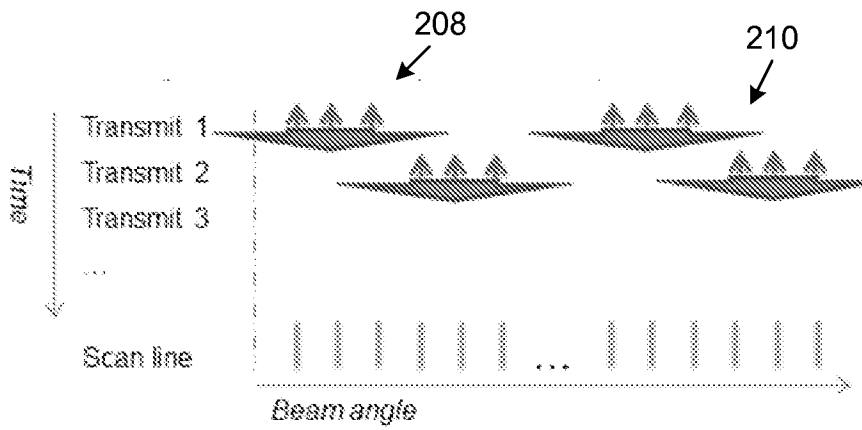


Fig. 7B

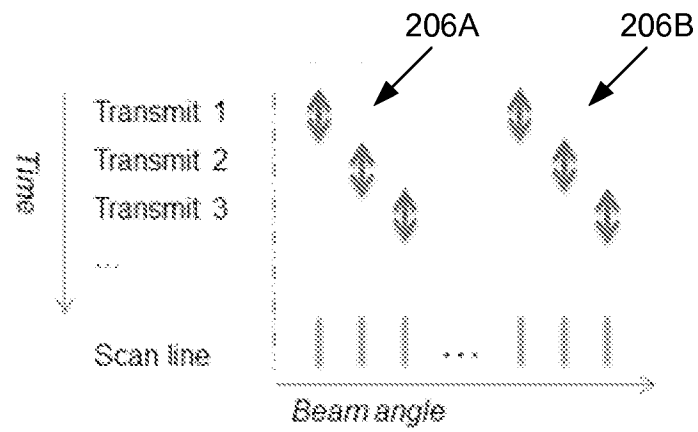


Fig. 8

7/11

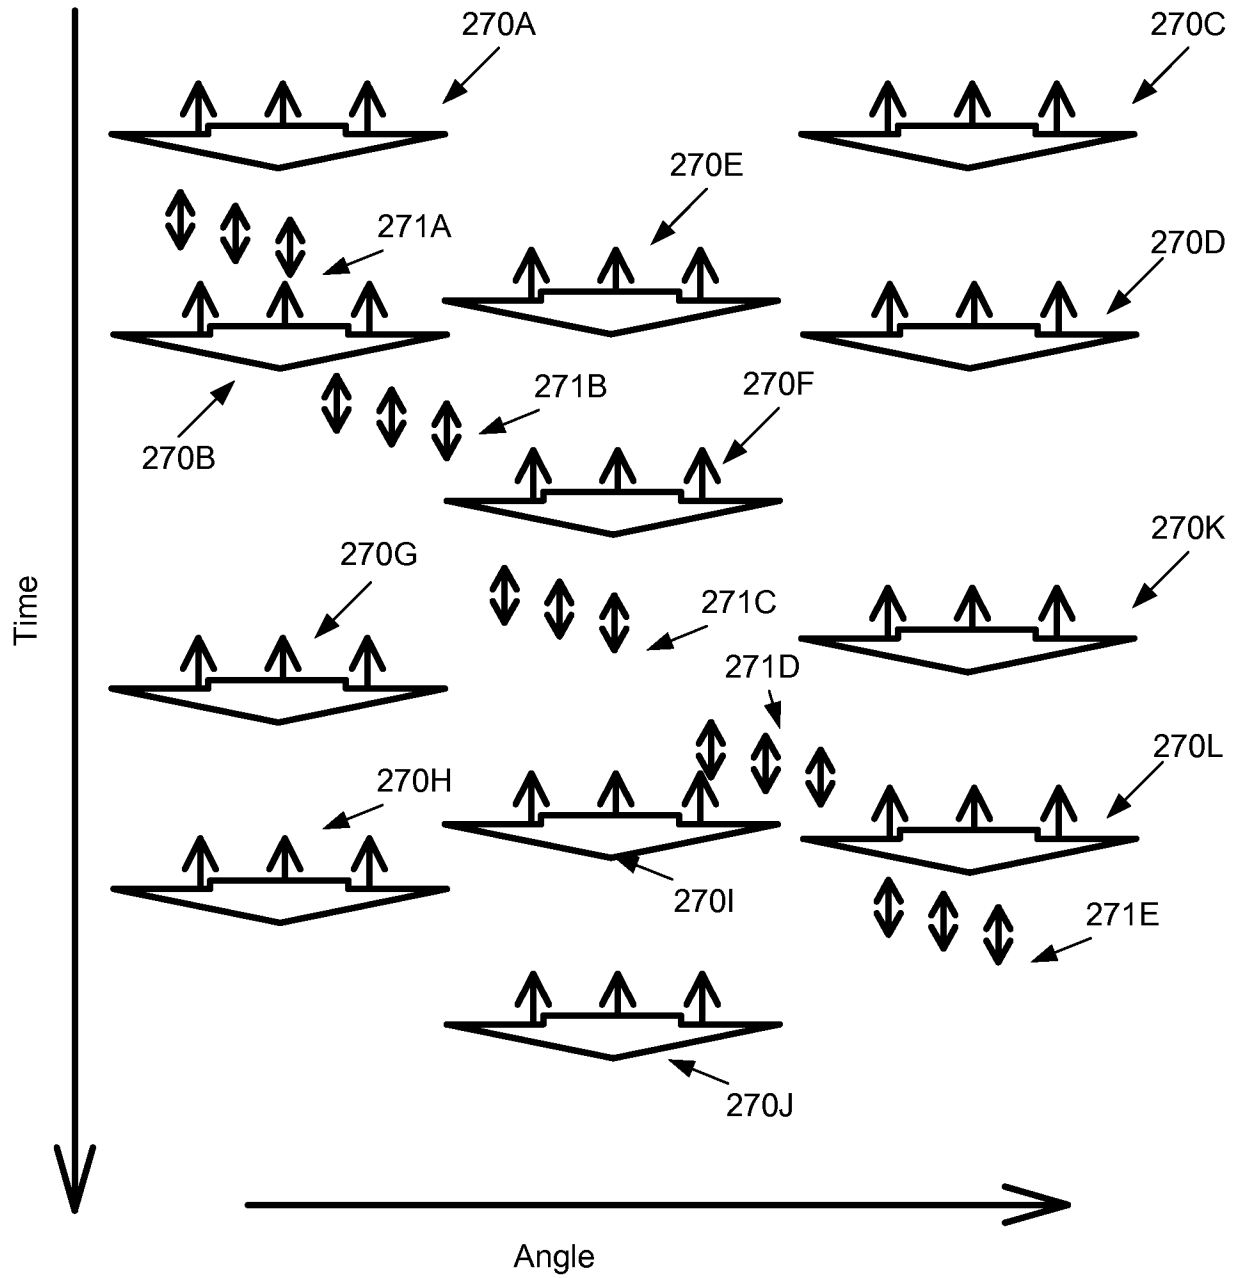


Fig. 7C

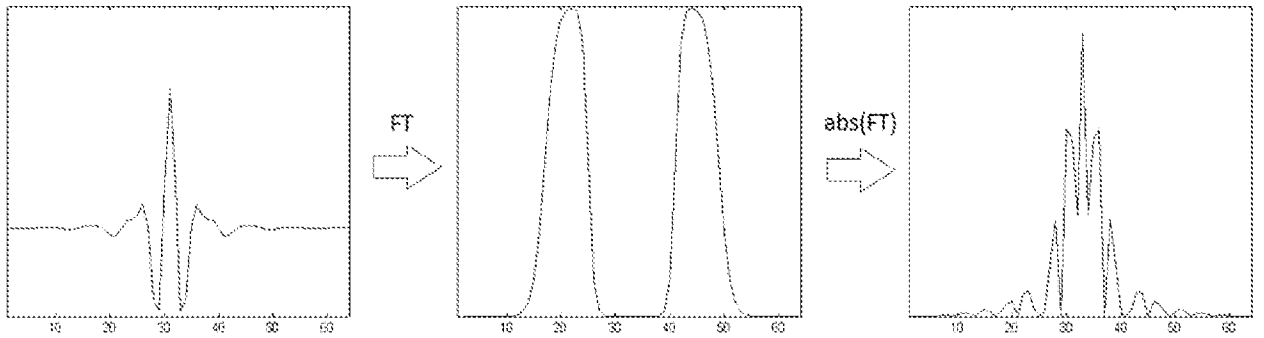


Fig. 9A

Fig. 9B

Fig. 9C

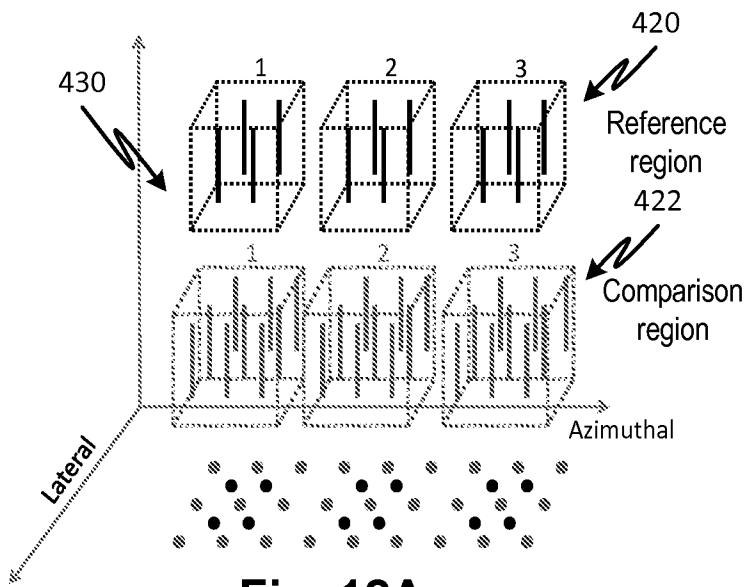


Fig. 12A

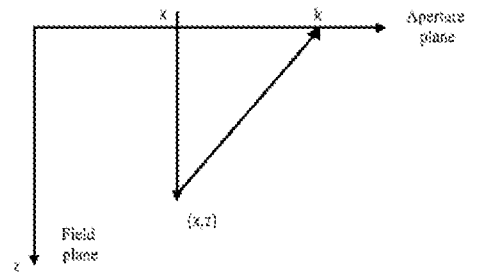


Fig. 10

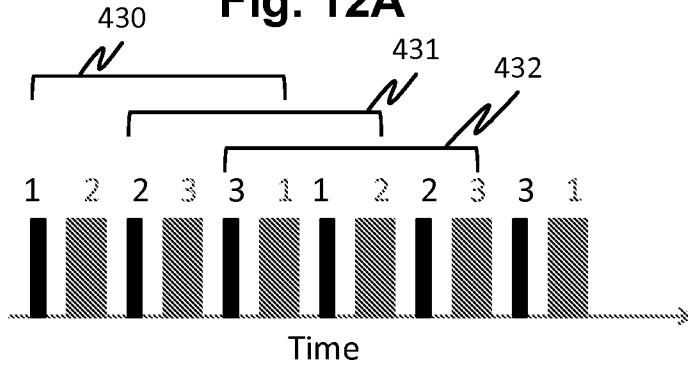


Fig. 12B

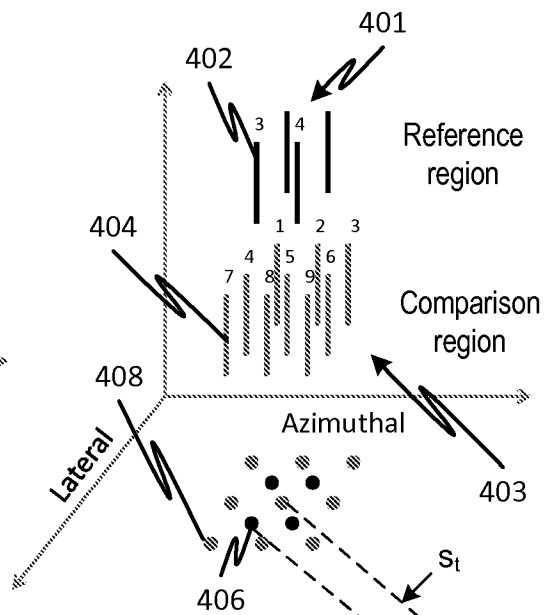


Fig. 11A

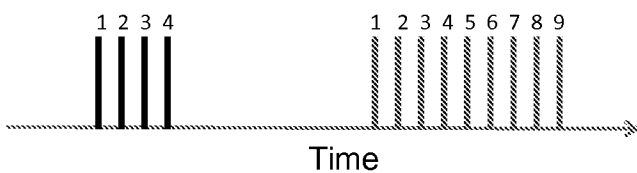


Fig. 11B

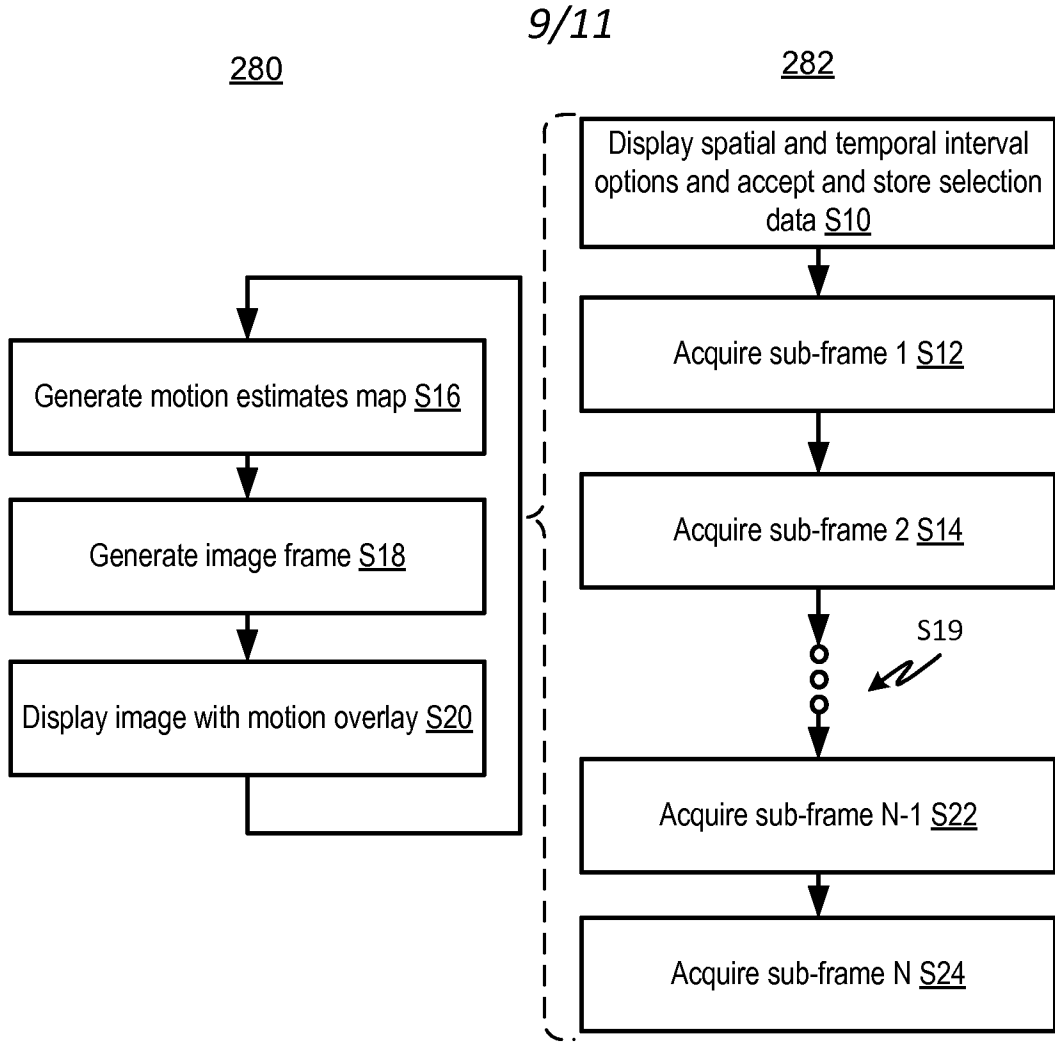


Fig. 13

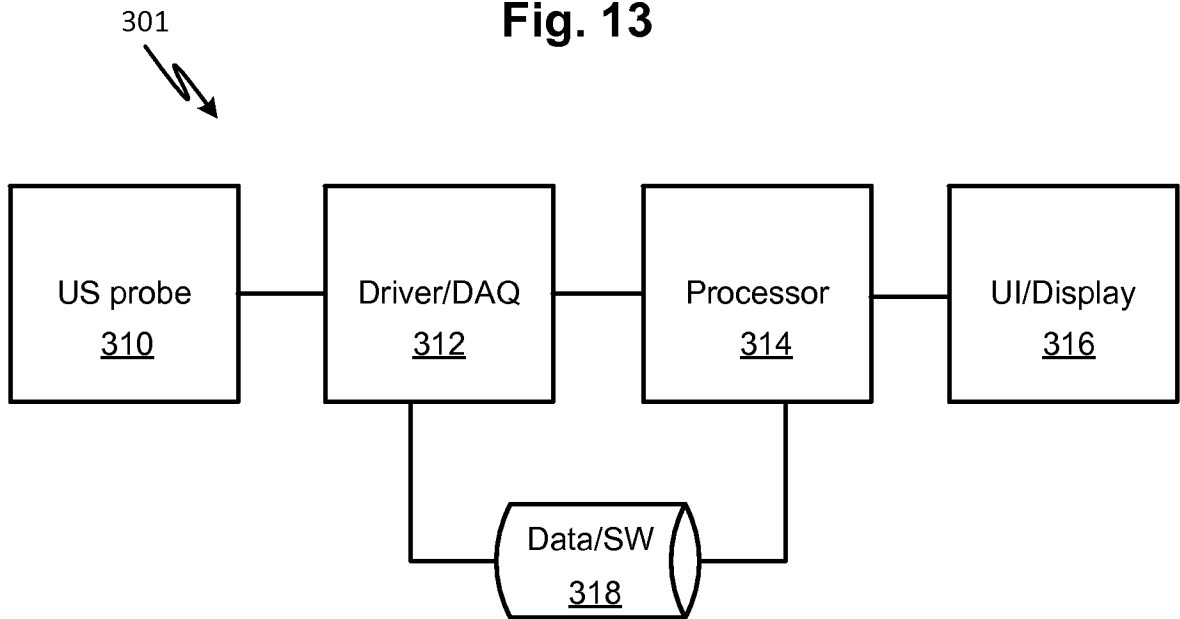


Fig. 14

10/11

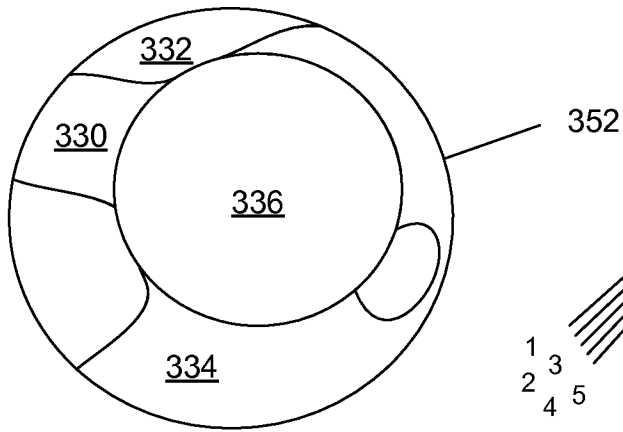


Fig. 15A

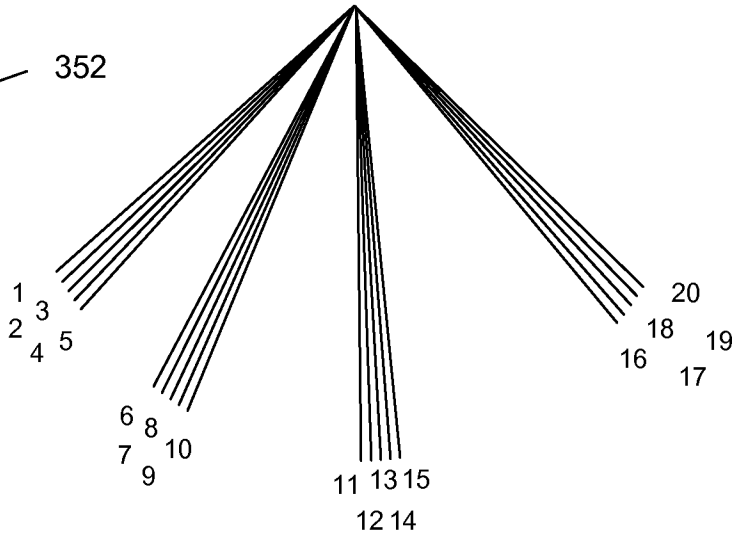


Fig. 16A

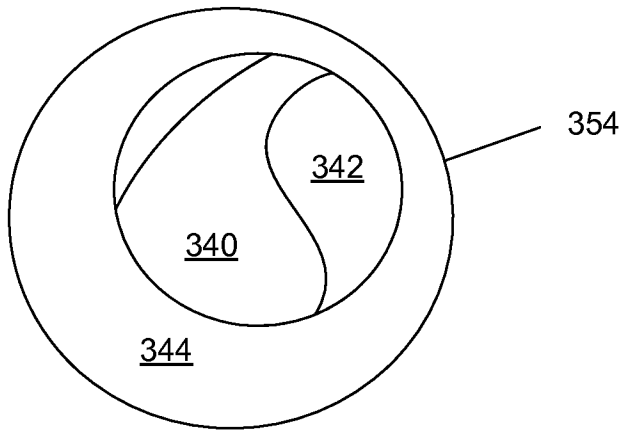


Fig. 15B

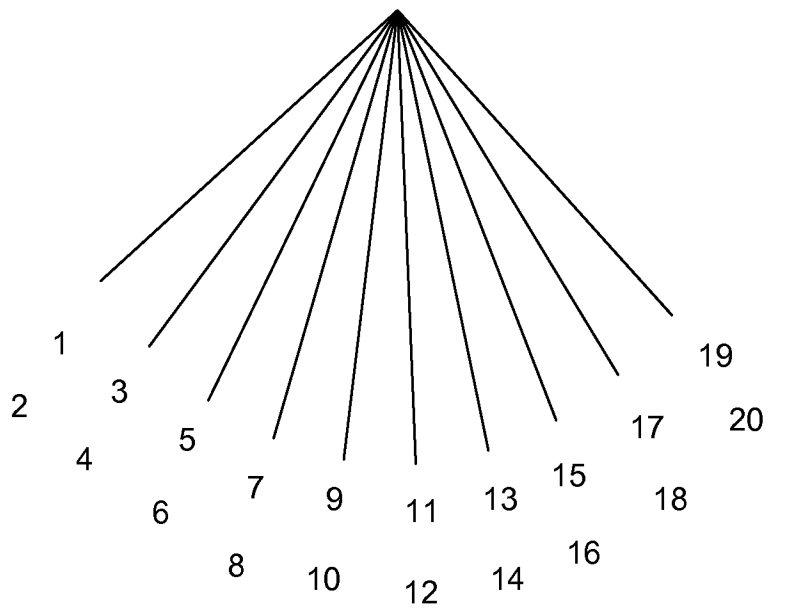


Fig. 16B

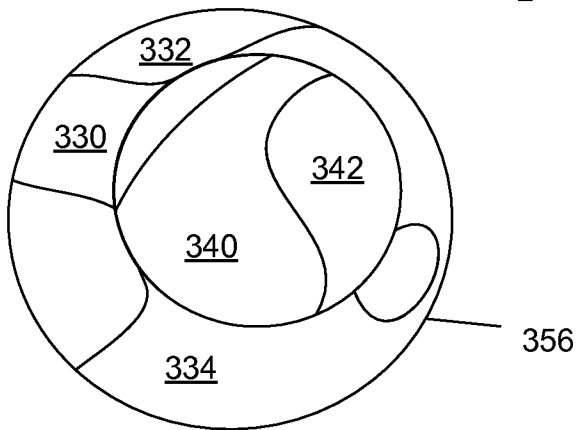


Fig. 15C

11/11

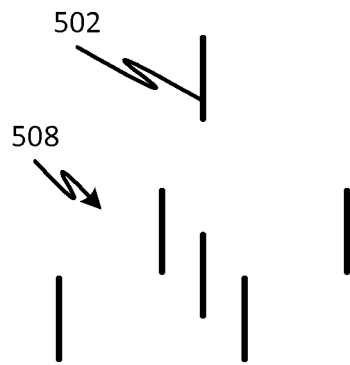
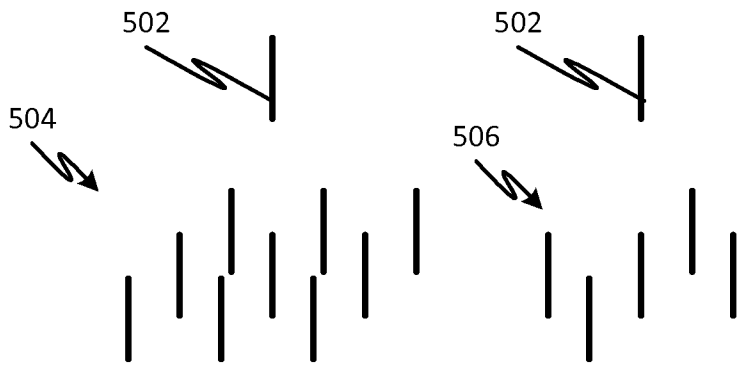
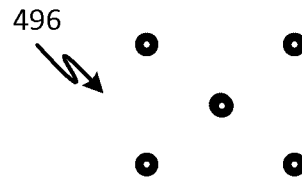

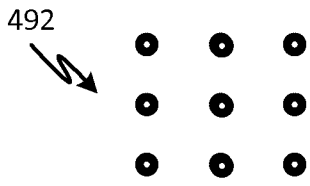


Fig. 17A

Fig. 17B

Fig. 17C

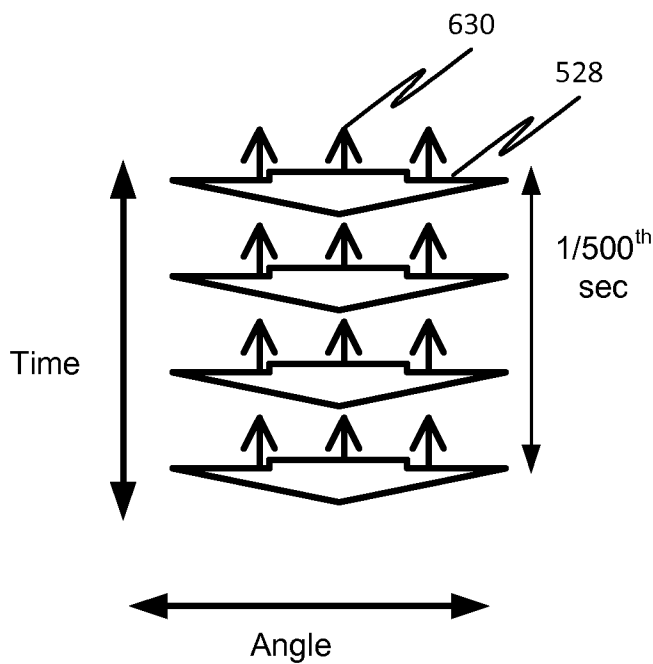


Fig. 17D

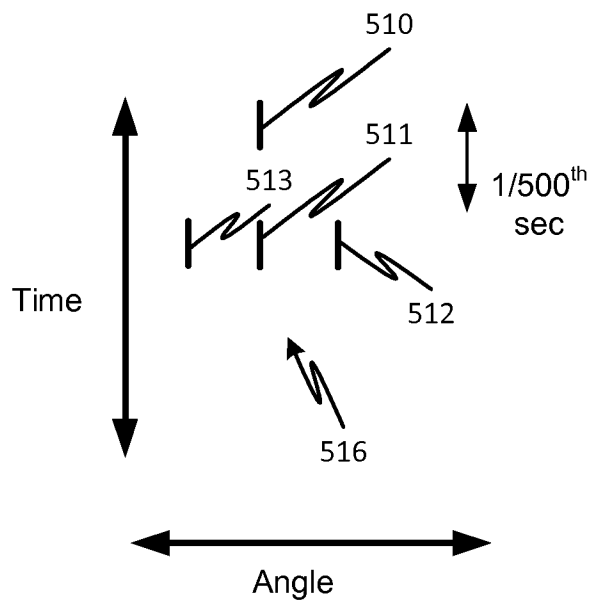


Fig. 17E