



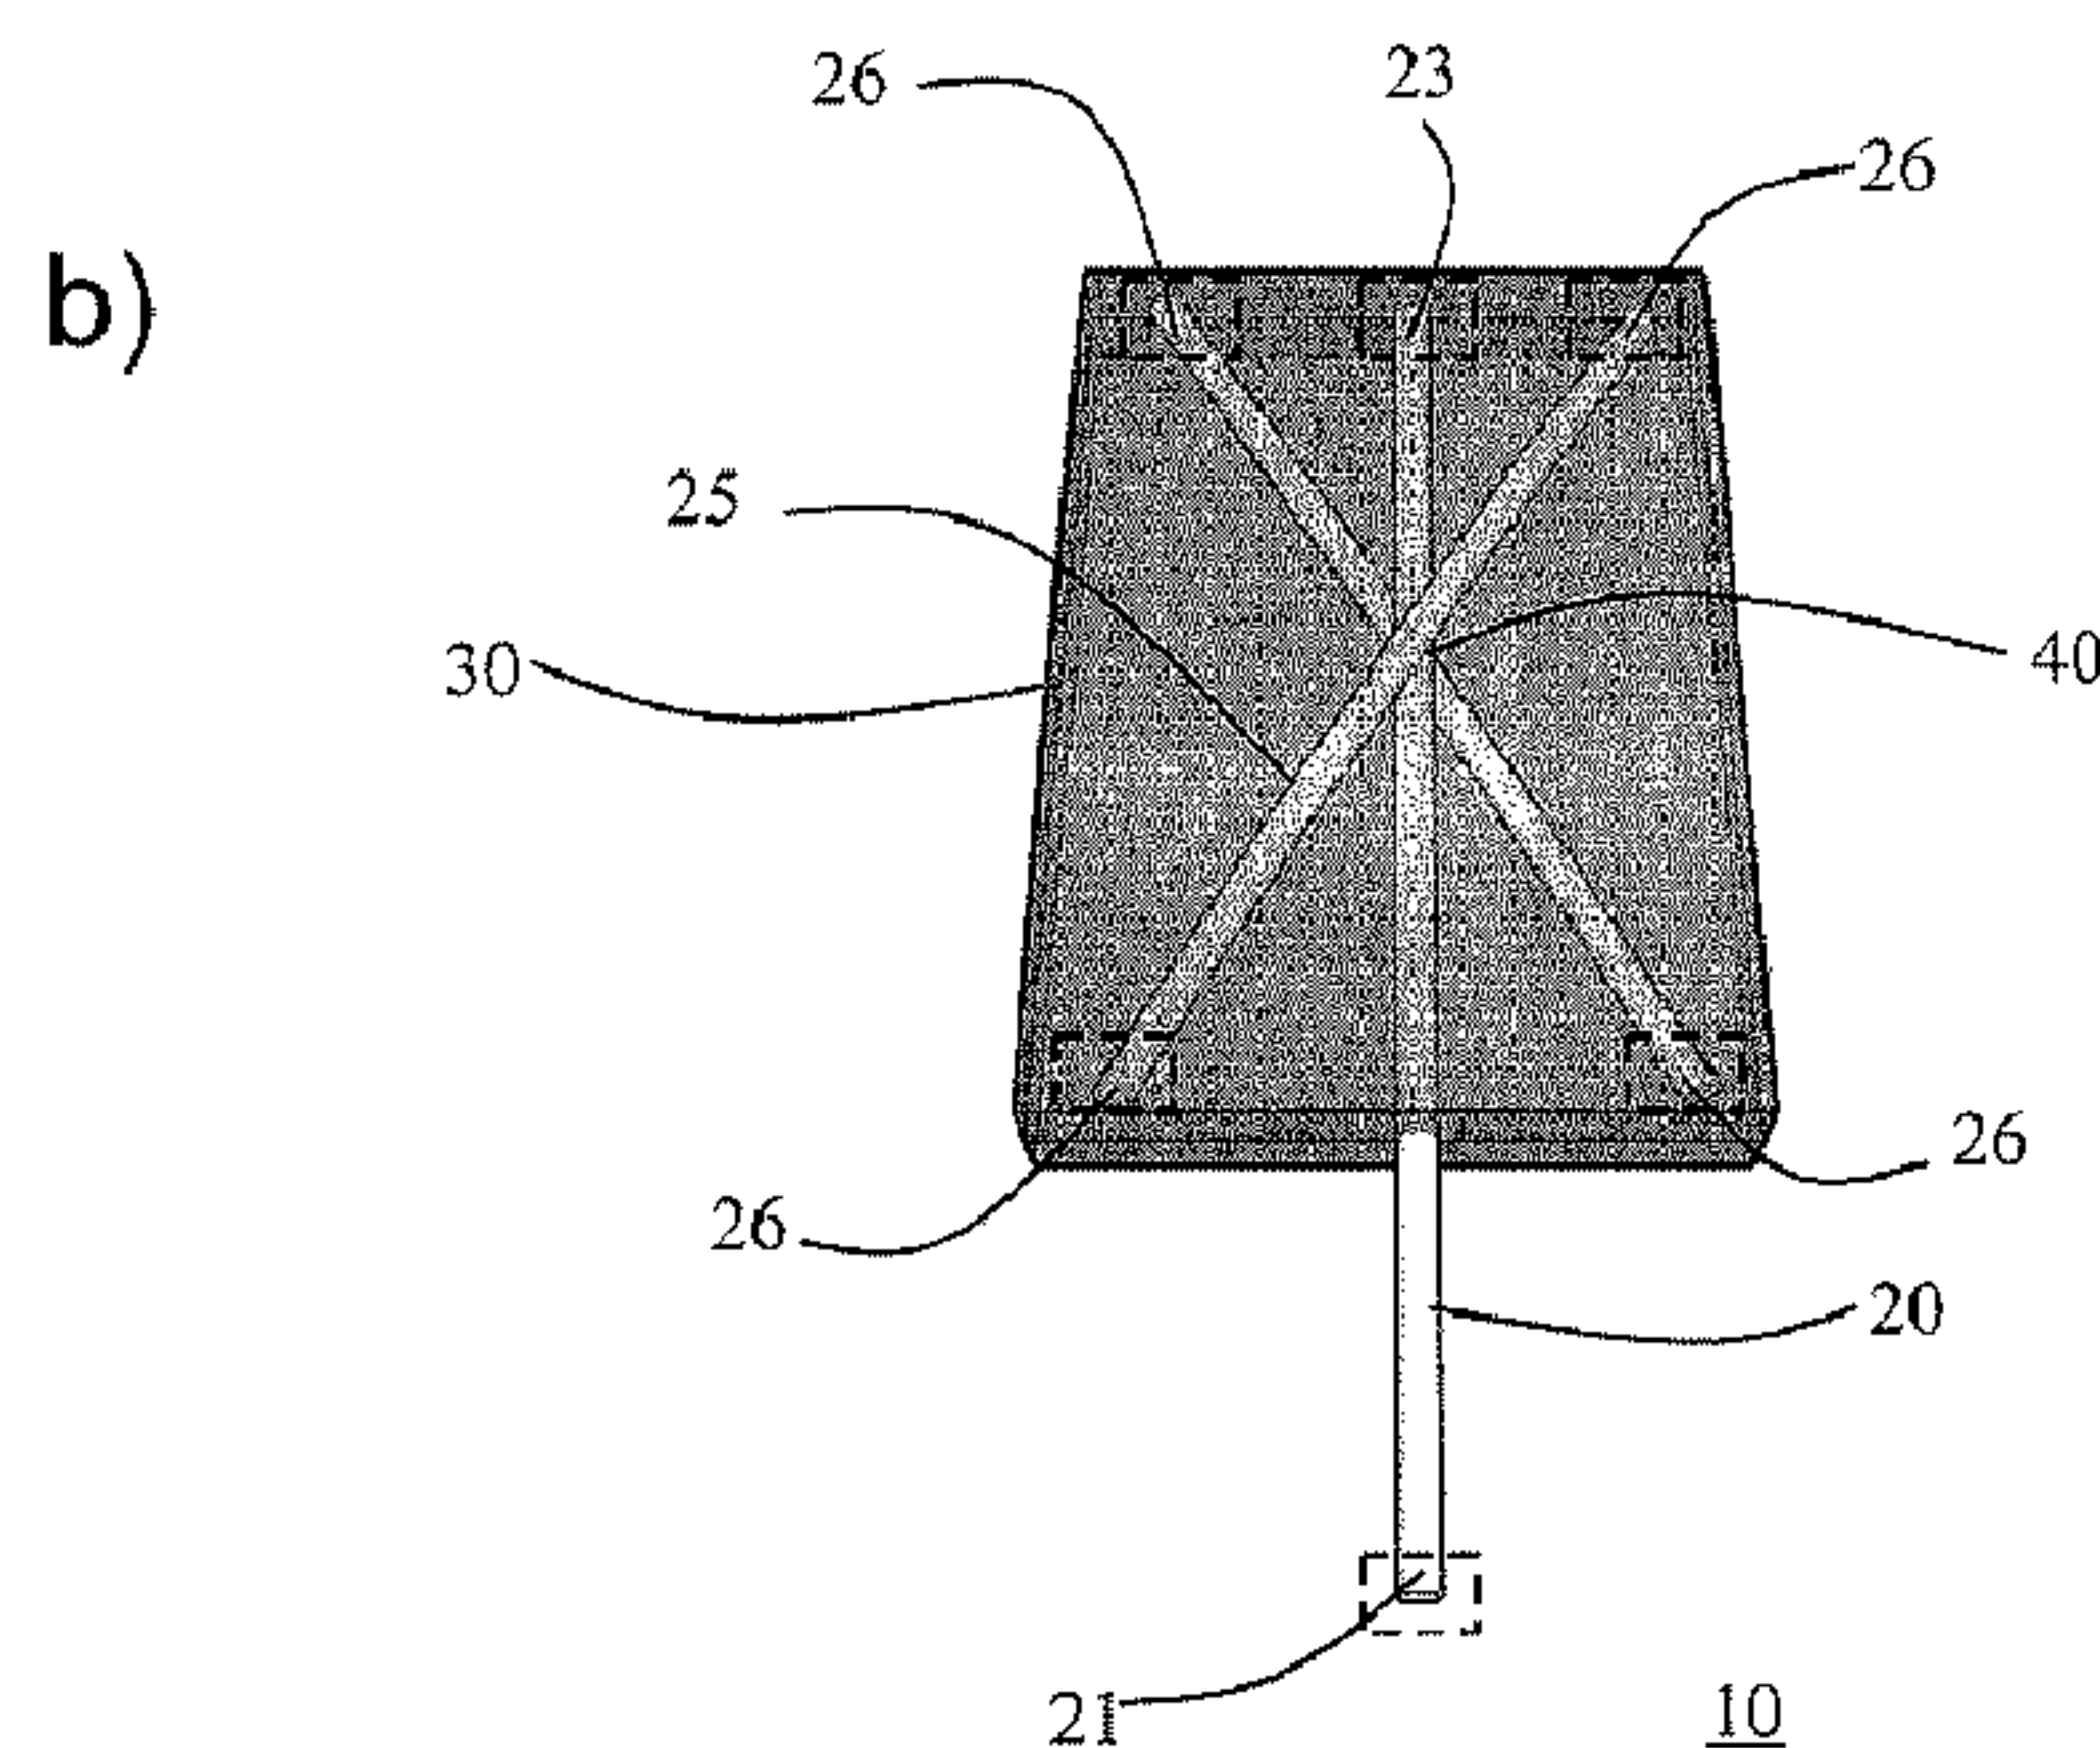

(86) **Date de dépôt PCT/PCT Filing Date:** 2009/03/27
(87) **Date publication PCT/PCT Publication Date:** 2009/10/01
(45) **Date de délivrance/Issue Date:** 2018/11/27
(85) **Entrée phase nationale/National Entry:** 2010/09/22
(86) **N° demande PCT/PCT Application No.:** US 2009/038702
(87) **N° publication PCT/PCT Publication No.:** 2009/121043
(30) **Priorité/Priority:** 2008/03/27 (US61/039,862)

(51) **Cl.Int./Int.Cl.** *G01N 35/00* (2006.01),
G01N 33/48 (2006.01), *G01N 33/49* (2006.01),
G01N 33/493 (2006.01), *G01N 33/50* (2006.01)
(72) **Inventeurs/Inventors:**
RECHES, MEITAL, US;
DICKY, MICHAEL D., US;
BUTTE, MANISH J., US;
WHITESIDES, GEORGE M., US
(73) **Propriétaire/Owner:**
PRESIDENT AND FELLOWS OF HARVARD COLLEGE,
US
(74) **Agent:** MBM INTELLECTUAL PROPERTY LAW LLP

(54) **Titre : FIL DE COTON SERVANT DE PLATE-FORME DIAGNOSTIQUE POUR ANALYSES MULTIPLES A BAS COUTS**
(54) **Title: COTTON THREAD AS A LOW-COST MULTI-ASSAY DIAGNOSTIC PLATFORM**

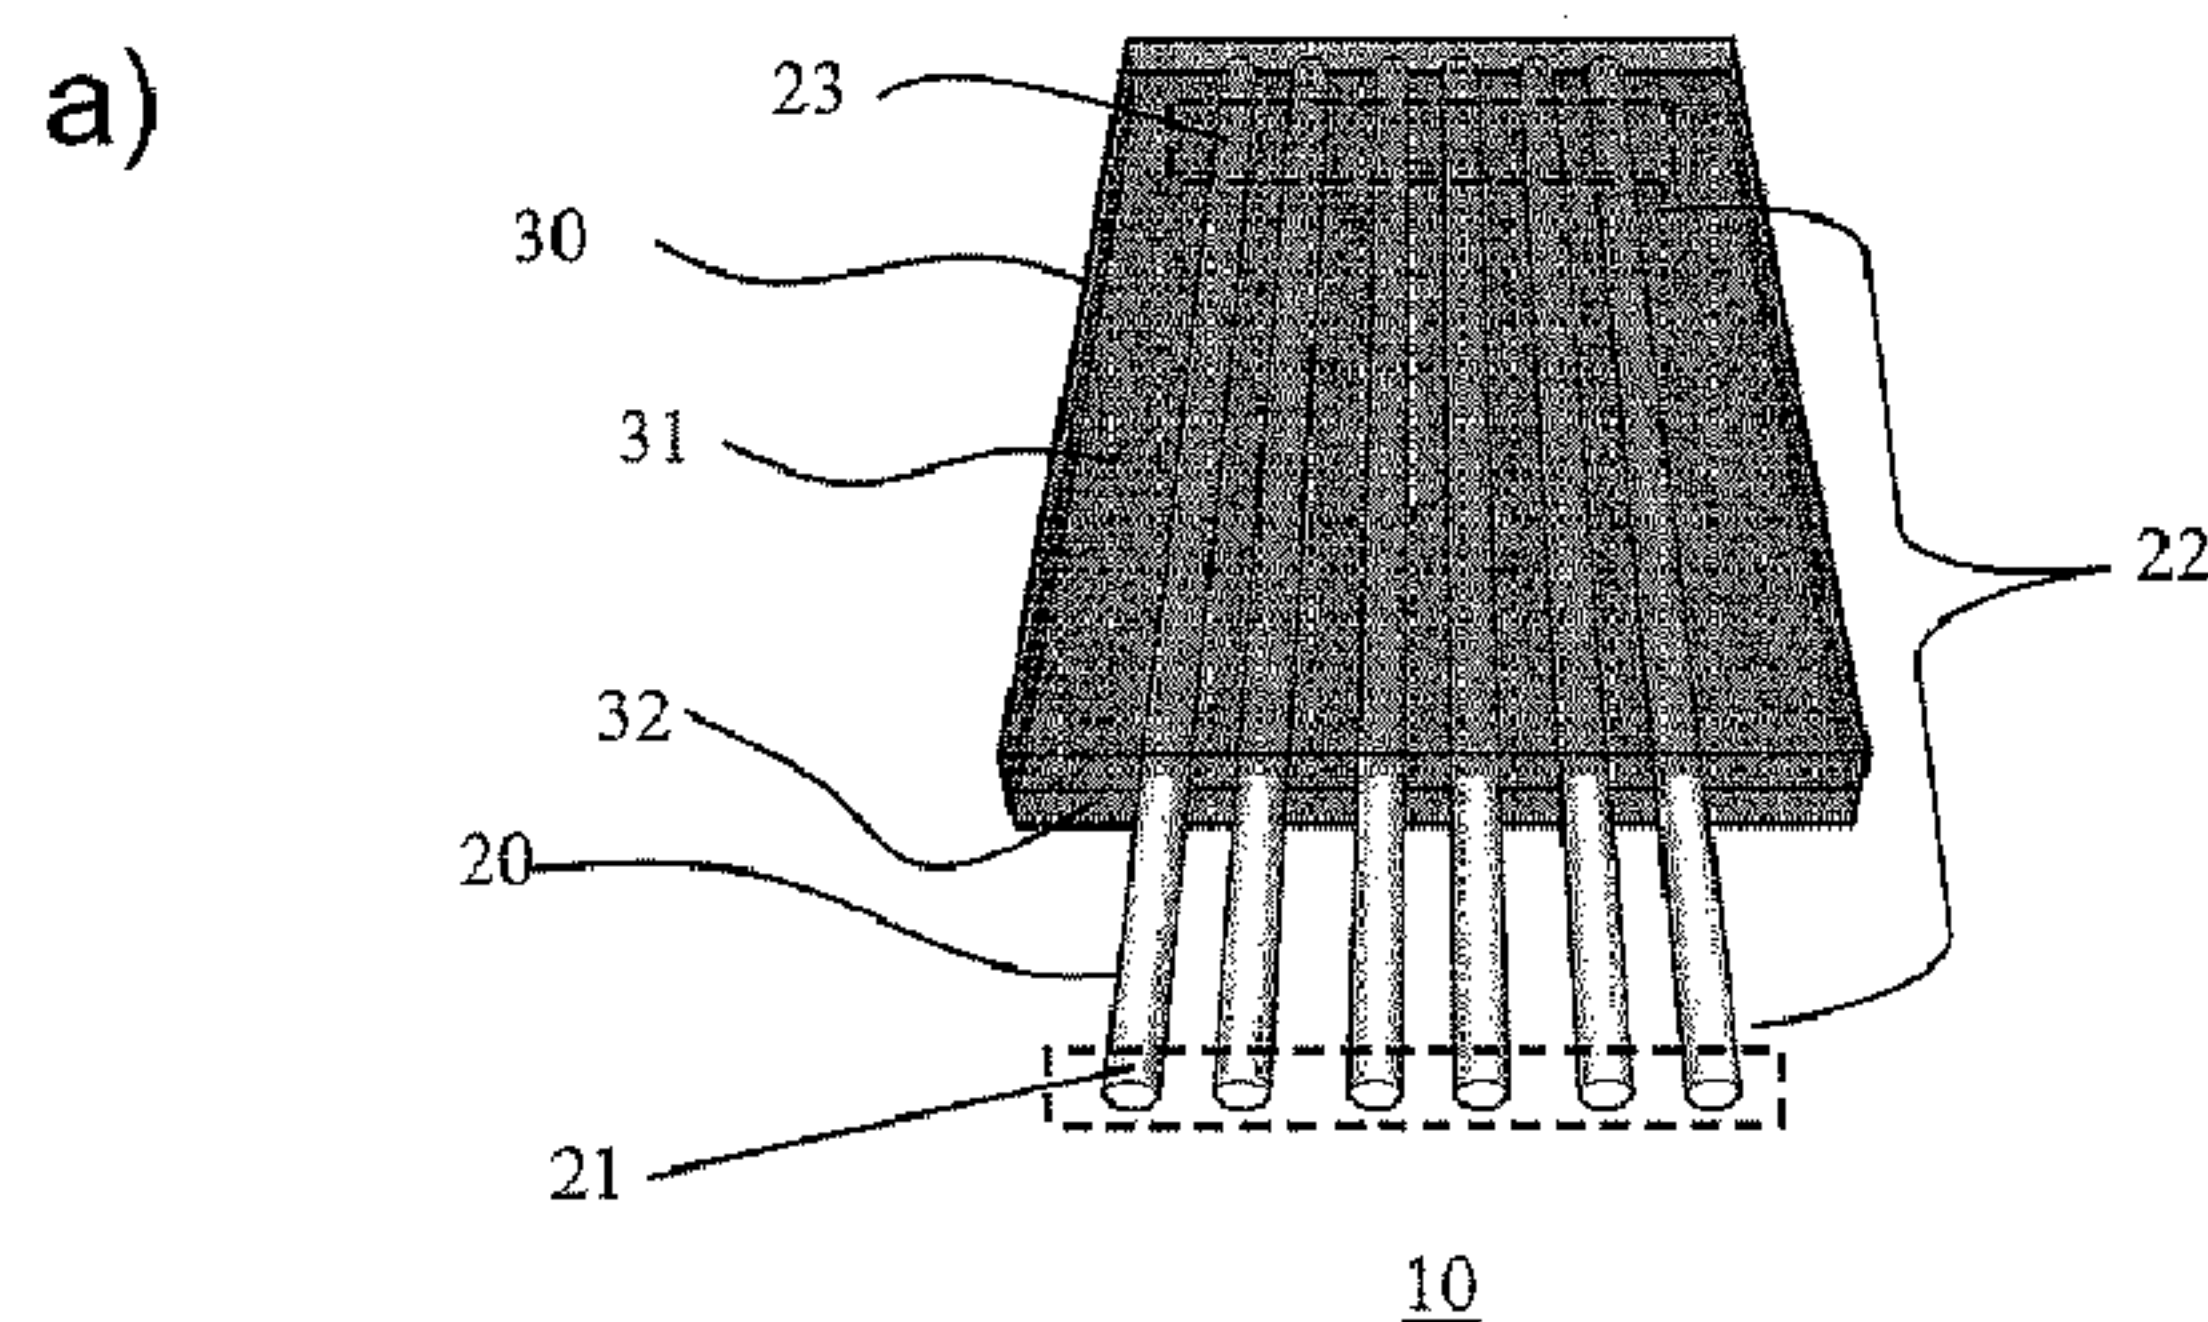

(57) **Abrégé/Abstract:**

Hydrophilic threads as platforms for inexpensive, low volume, portable diagnostic systems, and methods of making the same are described. A diagnostic system includes a hydrophilic loading thread having an inlet zone at a proximal end; a testing zone at a

(57) Abrégé(suite)/Abstract(continued):

distal end; and an intermediate zone located between the inlet zone and the testing zone, wherein the testing zone does not directly contact the inlet zone. In another aspect, a diagnostic system includes (i) a hydrophilic loading thread that includes an inlet zone at a proximal end and an intermediate zone at a distal end; and (ii) one or more additional hydrophilic threads that contact the intermediate zone of the loading thread. A method of detecting the presence or absence of an analyte in a fluid sample includes applying the sample to an inlet zone of a diagnostic system that includes a hydrophilic loading thread with an inlet zone at a proximal end; an intermediate zone; and a testing zone at a distal end; wherein the testing zone does not directly contact the inlet zone.

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
1 October 2009 (01.10.2009)

PCT

(10) International Publication Number
WO 2009/121043 A3

(51) International Patent Classification:

G01N 35/00 (2006.01) *G01N 33/49* (2006.01)
G01N 33/48 (2006.01) *G01N 33/50* (2006.01)
G01N 33/493 (2006.01)

(21) International Application Number:

PCT/US2009/038702

(22) International Filing Date:

27 March 2009 (27.03.2009)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/039,862 27 March 2008 (27.03.2008) US

(71) Applicant (for all designated States except US): **PRESIDENT AND FELLOWS OF HARVARD COLLEGE** [US/US]; 17 Quincy Street, Cambridge, MA 02138 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **RECHES, Meital** [IL/US]; 44 Cherry Street, Somerville, MA 02144 (US). **DICKEY, Michael, D.** [US/US]; 97 Hancock Street, #7, Cambridge, MA 02139 (US). **BUTTE, Manish, J.** [US/US]; 11-D Parley Avenue, Boston, MA 02130 (US). **WHITESIDES, George, M.** [US/US]; 124 Grasmere Street, Newton, MA 02458 (US).

(74) Agents: **SCOZZAFAVA, Mary, Rose et al.**; Wilmer Cutler Pickering Hale And Dorr LLP, 60 State Street, Boston, MA 02109 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report (Art. 21(3))
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

(88) Date of publication of the international search report:

7 January 2010

(54) Title: COTTON THREAD AS A LOW-COST MULTI-ASSAY DIAGNOSTIC PLATFORM

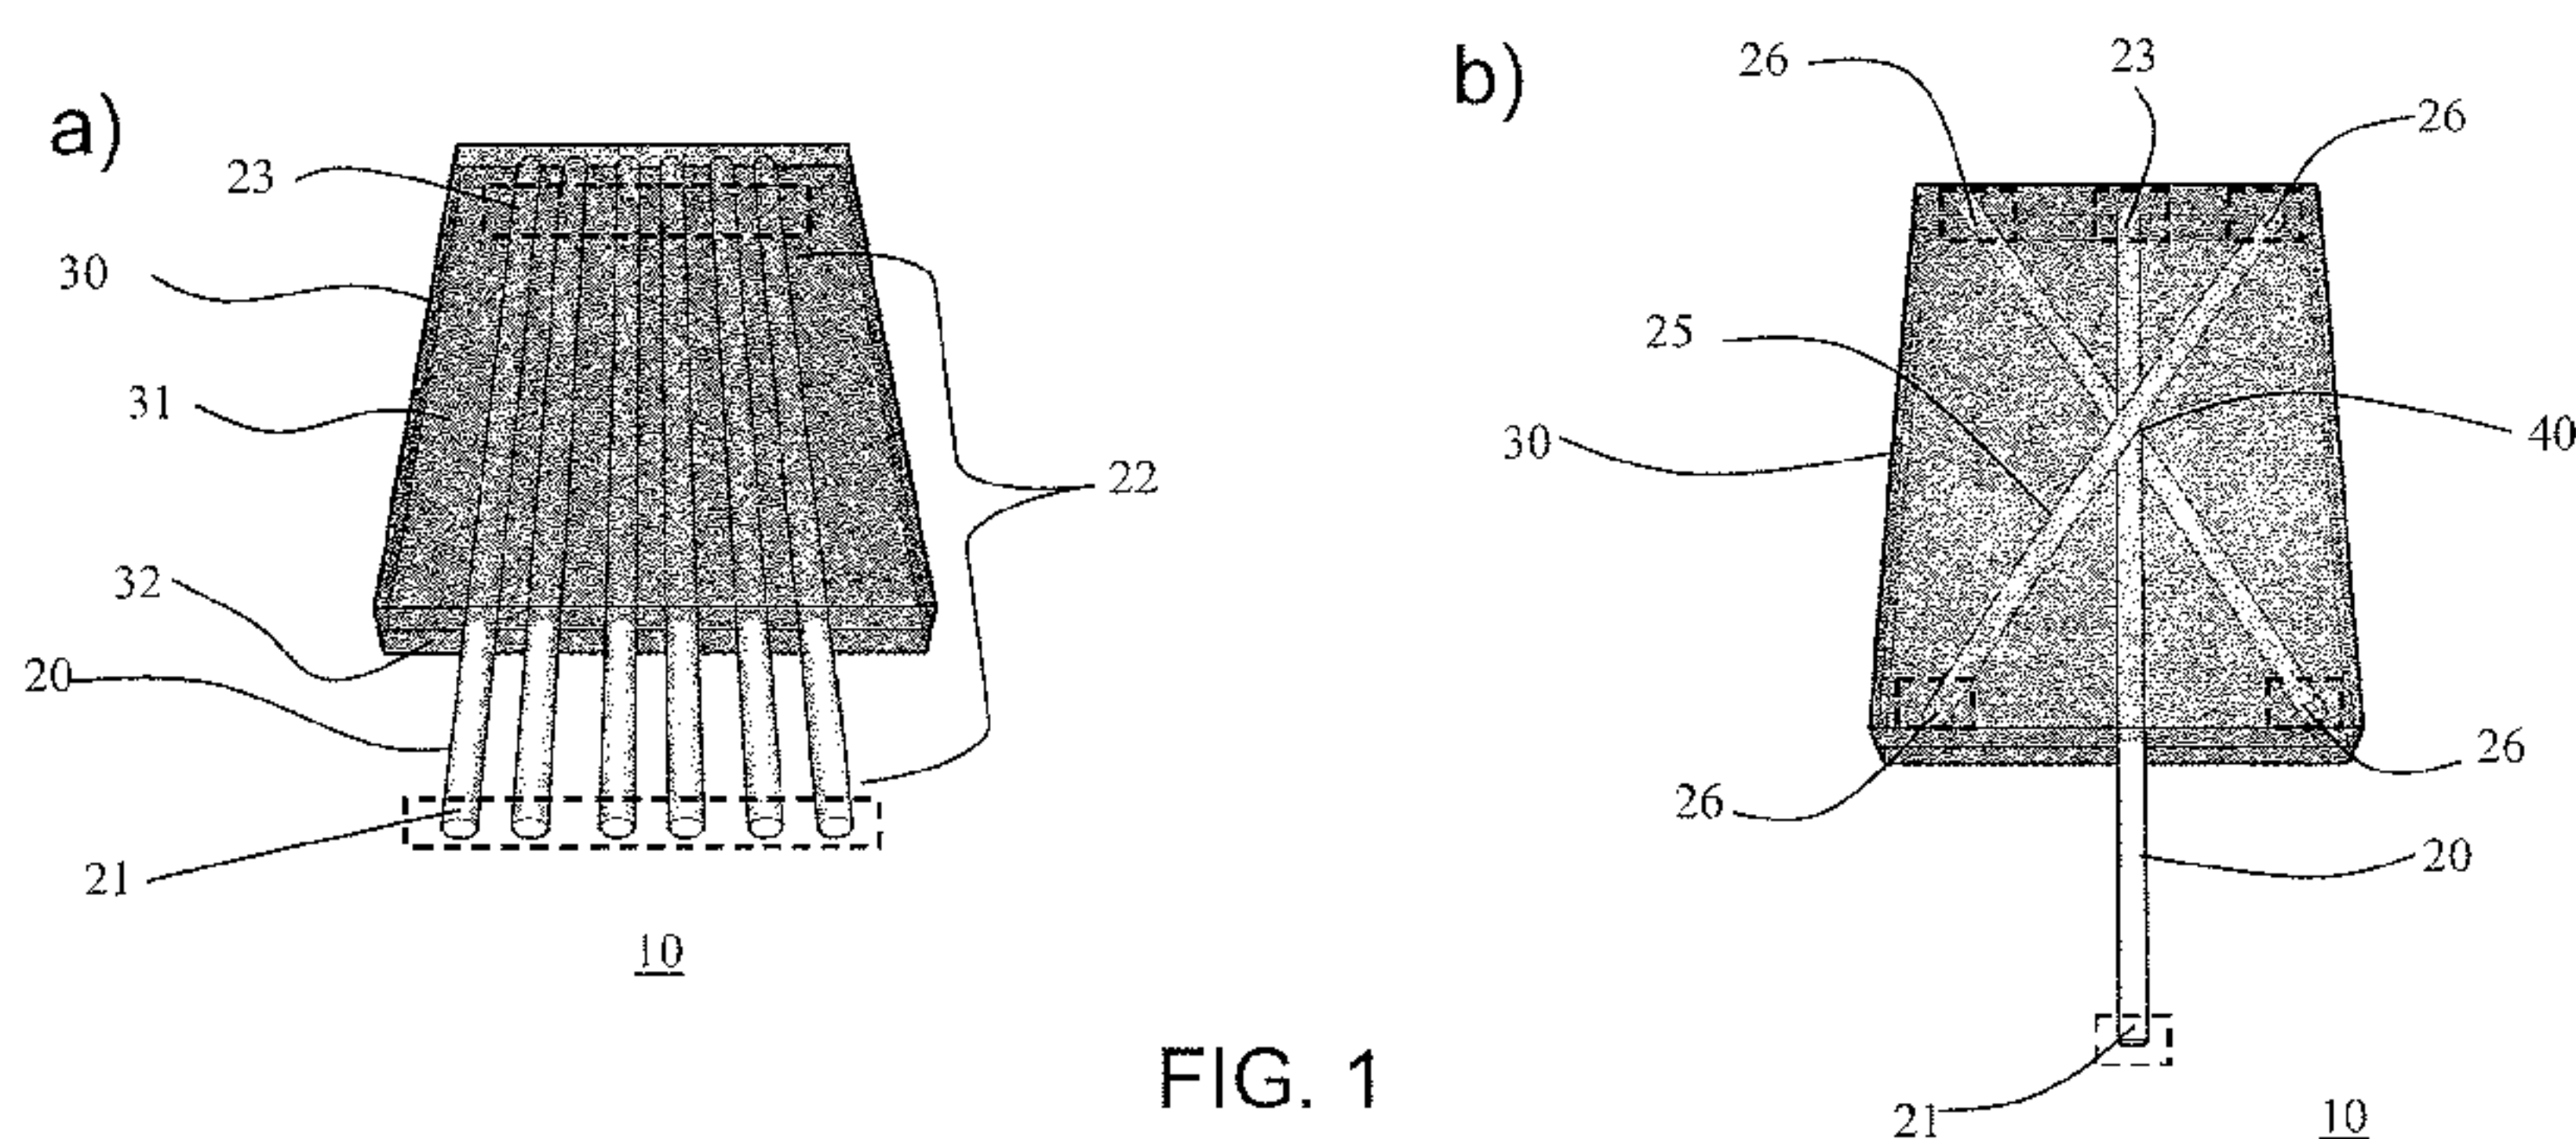


FIG. 1

(57) Abstract: Hydrophilic threads as platforms for inexpensive, low volume, portable diagnostic systems, and methods of making the same are described. A diagnostic system includes a hydrophilic loading thread having an inlet zone at a proximal end; a testing zone at a distal end; and an intermediate zone located between the inlet zone and the testing zone, wherein the testing zone does not directly contact the inlet zone. In another aspect, a diagnostic system includes (i) a hydrophilic loading thread that includes an inlet zone at a proximal end and an intermediate zone at a distal end; and (ii) one or more additional hydrophilic threads that contact the intermediate zone of the loading thread. A method of detecting the presence or absence of an analyte in a fluid sample includes applying the sample to an inlet zone of a diagnostic system that includes a hydrophilic loading thread with an inlet zone at a proximal end; an intermediate zone; and a testing zone at a distal end; wherein the testing zone does not directly contact the inlet zone.

COTTON THREAD AS A LOW-COST MULTI-ASSAY DIAGNOSTIC PLATFORM

[0001] DELETED

BACKGROUND

[0002] Most current bioanalytical assays are inaccessible to developing economies. Current diagnostic assays typically require large and expensive laboratory instruments that are operated by trained personnel. Although “dipstick” technologies have increased the accessibility of many assays, many of the assays are too expensive for low-cost settings and often require relatively large sample volumes. Thus, there remains a need for low-cost diagnostic assays that are not cumbersome and that can be performed on small sample volumes.

SUMMARY

[0003] Hydrophilic threads as platforms for inexpensive, low volume, portable diagnostic systems, and methods of making the same are described. Under certain aspects, the diagnostic systems are constructed by positioning hydrophilic threads within a laminated structure. This type of thread diagnostic is convenient for running low-cost, portable, and technically simple multiplexed bioassays. An illustrative embodiment is described in which the thread diagnostic is used for the simultaneous detection of glucose and protein in 20 μ L of artificial urine. Under many aspects, the diagnostic system is small, disposable, easy to use (and carry), and requires no external equipment, reagents, or power sources. This kind of diagnostic system is attractive for uses in developing countries, in the field, and/or as an inexpensive alternative to more advanced technologies already used in clinical settings.

[0004] Accordingly, in one aspect, a diagnostic system includes a hydrophilic loading thread having an inlet zone at a proximal end; a testing zone at a distal end;

and an intermediate zone located between the inlet zone and the testing zone, wherein the testing zone does not directly contact the inlet zone. In some embodiments, the system includes one or more additional hydrophilic threads that contact the intermediate zone of the loading thread, where the additional threads include testing zones. In one or more embodiments, the testing zone is treated with a detection reagent to provide a visible indication of an analyte present in a fluid sample.

[0005] In another aspect, a diagnostic system includes (i) a hydrophilic loading thread that includes an inlet zone at a proximal end and an intermediate zone at a distal end; and (ii) one or more additional hydrophilic threads that contact the intermediate zone of the loading thread. In some embodiments, one or more of the additional hydrophilic threads include a testing zone.

[0006] In another aspect, a method of detecting the presence or absence of an analyte in a fluid sample includes applying the sample to an inlet zone of a diagnostic system that includes a hydrophilic loading thread with an inlet zone at a proximal end; an intermediate zone; and a testing zone at a distal end; wherein the testing zone does not directly contact the inlet zone.

[0007] As used herein, an “inlet zone” is an area of a hydrophilic thread where a biological sample is applied or loaded onto a diagnostic system.

[0008] As used herein, a “loading thread” is a hydrophilic thread that includes at least an inlet zone and an intermediate zone. After the sample is applied to the inlet zone, the sample is carried through the loading thread from the inlet zone through the intermediate zone by capillary action. In some embodiments, the loading thread further includes a testing zone, which is physically separated from the inlet zone by the intermediate zone.

[0009] As used herein, an “intermediate zone” is an area of a hydrophilic thread distal to an inlet zone. In some embodiments, an intermediate zone is oriented between an inlet zone and a testing zone on a hydrophilic thread. In other embodiments, a hydrophilic thread includes an inlet zone at a proximal end and terminates in an intermediate zone at a distal end.

[0010] As used herein, a “testing zone” or “detection zone” is an area of a hydrophilic thread that is treated with a detection reagent.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] The foregoing and other objects of the present invention, the various features thereof, as well as the invention itself, may be more fully understood from the following description, when read together with the accompanying drawings, in which:

[0012] FIG. 1A is a schematic illustration of a “woven array” diagnostic system. FIG. 1B is a schematic illustration of a “branching array” diagnostic system. FIG. 1C is a schematic illustration of a “sewn array” diagnostic system.

[0013] FIG. 2 is a schematic illustration of an additional embodiment of a thread-based diagnostic system.

[0014] FIG. 3 is a schematic illustration of an additional embodiment of a thread-based diagnostic system.

[0015] FIG. 4A is a schematic illustration of a “woven array” diagnostic system with a wider gap between the threads. FIG. 4B is a schematic illustration of a “woven array” diagnostic system with a narrower gap between the threads.

[0016] FIG. 5 is a schematic illustration of a method of making a “woven array” diagnostic system.

[0017] FIG. 6A is an image of a rolled “woven array” diagnostic system. FIG. 6B is an image of an unrolled “woven array” diagnostic system after loading. FIG. 6C is an image of a “woven array” diagnostic system used to assay for glucose and protein.

[0018] FIG. 7 is an image of a “woven array” diagnostic system of two threads coated with petroleum jelly.

[0019] FIG. 8A is an image of a “woven array” diagnostic system of threads within a housing of two pieces of vinyl tape. FIG. 8B is an image of a “woven array” diagnostic system of threads within a housing of two pieces of Scotch tape. FIG. 8C is an image of a “woven array” diagnostic system of threads within a housing of one piece of Scotch tape and one piece of vinyl tape. FIG. 8D is an image of a “woven array” diagnostic system of threads coated with petroleum jelly within a housing of two pieces of Scotch tape.

[0020] FIG. 9 is an image of a “branching array” diagnostic system loaded with a fluid sample and assayed for glucose and protein.

[0021] FIG. 10A is an image of a “sewn array” diagnostic system that includes a thread sewn through a Mylar sheet. FIG. 10B is an image of the bottom side of a “sewn array” diagnostic system that includes two threads sewn through an adhesive bandage. FIG. 10C is an image of the top side of a “sewn array” diagnostic system that includes two threads sewn through an adhesive bandage.

[0022] FIG. 11A is an image of a “woven array” diagnostic system used to detect various analytes. FIG. 11B is an image of a “branching array” diagnostic system used to detect various analytes. FIG. 11C is an image of a “sewn array” diagnostic system used to detect various analytes.

DETAILED DESCRIPTION

[0023]

The materials, methods, and examples are illustrative only and not intended to be limiting. Unless otherwise defined, all technical and scientific terms used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. Although methods and materials similar or equivalent to those described herein can be used in the practice or testing of the present invention, suitable methods and materials are described below.

I. Diagnostic Systems

[0024] The methods and compositions described herein relate to diagnostic systems that utilize hydrophilic threads to assay fluid samples. No external power source is necessary to perform the assays, as capillary action rapidly draws the sample along the thread and into testing zones used in the assays. Further, the assays can be conducted rapidly, on the order of minutes.

[0025] With reference to Figures 1A, 1B, and 1C, a few nonlimiting configurations of a diagnostic system 10 are illustrated therein. In the illustrated configurations, the system 10 generally includes loading threads 20 and a housing 30.

[0026] Figure 1A illustrates a “woven array” configuration. With reference to Figure 1A, a diagnostic system 10 includes loading threads 20 and a housing 30. The loading threads 20 and housing 30 are configured such that a proximal end of

each loading thread **20** is exposed and a distal end of each loading thread **20** is enclosed within housing **30**.

[0027] Loading thread **20** comprises an inlet zone **21**, intermediate zone **22**, and testing zone **23**. Inlet zone **21** is at the proximal end of loading thread **20** and is not disposed within housing **30**. Intermediate zone **22** encompasses the entire region of loading thread **20** between inlet zone **21** and testing zone **23**. In Figure 1A, a proximal end of intermediate zone **22** is not disposed within housing **30**, and a distal end of intermediate zone **22** is disposed within housing **30**. Testing zones **23** include one or more detection reagents described herein.

[0028] Figure 1B illustrates a “branching array” configuration. With reference to Figure 1B, a diagnostic system **10** includes loading thread **20**, testing threads **25**, and a housing **30**. Loading thread **20** and housing **30** are configured such that a proximal end of loading thread **20** is exposed and a distal end of loading thread **20** is disposed within housing **30**. Testing threads **25** are disposed within housing **30** and intersect loading thread **20** at branching point **40**.

[0029] Loading thread **20** comprises an inlet zone **21**, intermediate zone **22**, and testing zone **23**. Inlet zone **21** is at the proximal end of loading thread **20** and is not disposed within housing **30**. Intermediate zone **22** encompasses the entire region of loading thread **20** between inlet zone **21** and testing zone **23**. In Figure 1B, a proximal end of intermediate zone **22** is not disposed within housing **30**, and a distal end of intermediate zone **22** is disposed within housing **30**. Intermediate zone **22** intersects testing threads **25** at branching point **40**. Testing threads **25** comprise intermediate zones that intersect with intermediate zone **22** at branching point **40**, and the ends of testing threads **25** comprise testing zones **26**. Testing zones **23** and **26** include one or more detection reagents described herein.

[0030] Figure 1C illustrates a “sewn array” configuration. With reference to Figure 1C, a diagnostic system **10** includes loading thread **20** and a housing **30**. Housing **30** comprises a top face **31** and a bottom face **32**. Loading thread **20** is disposed onto housing **30** such that testing zones **23** of loading thread **20** are disposed on and exposed at the top face **31** of housing **30** and inlet zones **21** of loading thread **20** are disposed on and exposed at the bottom face **32** of housing **30**. Loading thread **20** includes intermediate zones **22** located between inlet zones **21**

and testing zones **23**. A proximal end of intermediate zone **22** is exposed on the bottom face **32** of housing **30** and a distal end of intermediate zone **22** is exposed on the top face **31** of housing **30**. The distal end of testing zone **23** contacts linker region **50** of thread **20**. Linker region **50** contacts the top face **31** of housing **30**, passes through housing **30**, and contacts the bottom face **32** of housing **30**. The distal end of linker region **50** contacts the next inlet zone **21** of thread **20**. Testing zones **23** include one or more detection reagents described herein.

[0031] The diagnostic systems described herein include a housing **30**. The housing can be made of plastic or any other inert material that does not interfere with the assay procedure. For example, the housing can be any known flexible sheet or molded plastic. Preferably, the housing is made of tape. The housing can be used as a support to maintain the hydrophilic threads in the appropriate configurations. The housing can also protect the hydrophilic threads from contamination and mechanical damage during handling and storage. Further, as described herein, the housing can be used to seal and separate one or more hydrophilic threads from each other to prevent cross-contamination.

[0032] In some embodiments, e.g., “woven array” or “branching array” configurations, at least one face of the housing is made of a transparent material. In some embodiments, e.g., “sewn array” configurations, the housing can be a substrate, such as an adhesive bandage, paper, cloth, or clothing.

[0033] The diagnostic systems described herein can include various additional configurations. For example, the proximal ends of hydrophilic threads can be braided to perform multiple assays on a fluid sample. As depicted in Figure 2, diagnostic system **10** can include three hydrophilic loading threads **20**, each of which contacts testing threads **25** at branching points **40**. Loading threads **20** and testing threads **25** include testing zones **23**, resulting in 9 separate testing zones. Although Figure 2 depicts the loading threads **20** in a linear orientation, in other embodiments, the inlet zones of loading threads **20** or the inlet zones and at least a portion of intermediate zones of loading threads **20** can be braided or can be brought together to facilitate simultaneous loading of a sample.

[0034] In other embodiments, the diagnostic system has a configuration depicted in Figure 3. In this configuration, the diagnostic system includes loading thread **20**

with inlet zone **21** and intermediate zone **22** that contacts testing threads **25**, each of which includes a testing zone **23** having the same detection reagent. The distal ends of testing threads **25** combined. In some embodiments, the distal ends of testing threads **25** are braided. Such a configuration can be used, e.g., to provide a combined detectable signal can be used to assay fluid samples containing small concentrations of analytes.

Hydrophilic Threads

[0035] Threads **20** and **25** described herein can be of any hydrophilic material that wicks fluid by capillary action. For example, cotton, nylon, polyester, polyolefins (such as polypropylene), fluoropolymers (such as polyvinylidene fluoride), nitrocellulose, cellulose, cellulose acetate, and glass microfiber structures can be used in the diagnostic systems described herein.

[0036] Preferably, the threads are made of cotton, which is inexpensive, available worldwide, and is an established material (e.g., in the form of gauze) in hospitals because of its biocompatibility. Thread is durable under many environmental conditions, yet flexible and light weight; these properties correspond with the potential for ubiquitous use, as well as easy transport and storage (e.g., as light weight reels). Cotton thread wicks most non-viscous, water-based biological fluids while simultaneously filtering particulates.

[0037] The threads have dimensions that exhibit a high-aspect ratio (length:diameter). Such a high-aspect ratio reduces lateral flow within the thread. The lack of lateral transport reduces the required volume of sample (e.g., the volume of blood from a finger prick is likely to be sufficient) and focuses the assay signal (i.e., the analyte wicks to the end of the thread, increasing the local concentration and therefore the signal).

[0038] In some embodiments, the hydrophilic thread is functionalized to enhance the absorptive and/or wicking properties using any of a number of known substances and methods. For example, the hydrophilic threads can be exposed to oxygen plasma (SPI Plasma-Prep II, Structure Probe, Inc.) or to a mercerization process (exposure of the thread to NaOH while under tension).

Detection Reagents

[0039] The diagnostic systems described herein can contain hydrophilic threads that include diagnostic reagents capable of reacting with a predetermined analyte whose presence is suspected in a sample to be assayed. In some embodiments, the hydrophilic threads (e.g., testing zones) can be treated with one or more detection reagents before the diagnostic system is assembled. For example, a detection reagent can be spotted onto one end of a thread and allowed to be incorporated into the thread by capillary action. The thread can subsequently be dried, and the area of the thread contacted by the detection reagent results in a testing zone.

[0040] The interaction or complex of a detection reagent and a predetermined analyte within a fluid sample can generate a detectable effect, for example one that is apparent to the naked eye (e.g., detected as a color change). Alternatively, such an interaction can be detected using a spectrometer or other technical means (e.g., to detect a change in ultraviolet absorption).

[0041] Typically, the detection reagent has a greater affinity for the predetermined analyte than for other components of the fluid sample to be assayed. The detection reagent can be a chemical, which undergoes a color change when contacted with a particular analyte, or an enzyme that can convert an analyte into a detectable compound or can convert a second agent into a detectable compound in the presence of an analyte.

[0042] In some embodiments, the detection reagent is an immunoglobulin, e.g., an antibody, e.g., a primary antibody, that specifically binds to a particular analyte. In some embodiments, a detection antibody, e.g., a secondary antibody, can be loaded onto the diagnostic system after the fluid sample is loaded. When the detection reagent, e.g., primary antibody, specifically binds to an analyte in the fluid and a detection antibody is subsequently loaded onto the diagnostic system, the detection antibody can specifically bind to an analyte bound to the primary antibody and can provide a detectable signal.

[0043] In some embodiments, a diagnostic system includes many detection reagents, each of which can react with a different analyte to produce a detectable effect. Alternatively, each detection reagent can be sensitive only to a predetermined concentration of a single analyte.

[0044] In some embodiments, the detection reagent is disposed along the testing zone of a hydrophilic thread and is freely mobile when contacted by the fluid sample. In such embodiments, the detection reagent is carried through the hydrophilic thread to the end of the thread, e.g., by capillary action, allowing detection of an analyte to occur at the end of the thread (e.g., testing zone). In other embodiments, the detection reagent is disposed at the end of a thread and the fluid sample is carried through the hydrophilic thread to the detection reagent at the end of the thread. In certain embodiments, detection can occur as the concentration of analyte that reaches the end of the testing zone increases due to capillary action, resulting in an increase in detectable effect produced by the detection reagent. In some embodiments, the biological sample evaporates at the end of the testing zone, resulting in a continued amount of biological sample being wicked through the hydrophilic thread to the end of the testing zone. This can result in increasing amounts of analyte being carried to the detection reagent at the end of the testing zone and an increase in the detectable effect.

II. Methods of using Diagnostic Systems

[0045] The diagnostic systems described herein can be used to test for the presence of analytes in fluid samples. With reference to Figure 1A, the diagnostic system **10** can be loaded with a fluid sample by contacting the fluid sample with the inlet zone **21** on thread **20**. The fluid sample is then transported through thread **20** by wicking action from the inlet zone **21** to intermediate zone **22**. The fluid is transported through intermediate zone **22** to testing zone **23** by wicking action. Testing zone **23** includes a detection reagent described herein, e.g., a detection reagent for a specific analyte. The interaction of a predetermined analyte within the fluid sample with the detection reagent results in a detectable signal at testing zone **23**.

[0046] In certain embodiments, testing zones **23** include the same detection reagent. In other embodiments, at least one testing zone **23** includes a detection reagent that is different from the detection reagent on a second testing zone **23**.

[0047] With reference to Figure 1B, a fluid sample is loaded by contacting the fluid sample with the inlet zone **21** on thread **20**. The fluid sample is then transported through thread **20** by wicking action from the inlet zone **21** to

intermediate zone **22**. When the fluid sample reaches branching point **40**, the fluid sample contacts testing threads **25**, and a portion of the fluid sample is transported through testing threads **25** by wicking action to testing zones **26**. A portion of the fluid sample is also wicked through intermediate zone **22** of thread **20** to testing zone **23**.

[0048] In certain embodiments, testing zones **23** and **26** include the same detection reagent. In other embodiments, at least one of testing zone **23** and testing zones **26** includes a detection reagent that is different from the detection reagent on another testing zone. Preferably, testing zone **23** and testing zones **26** each include a unique detection reagent.

[0049] With reference to Figure 1C, a fluid sample is loaded by contacting the fluid sample with the inlet zone **21** on thread **20**. The fluid sample is transported through thread **20** from inlet zone **21** to intermediate zone **22** to testing zone **23** by wicking action. In certain embodiments, testing zones **23** include the same detection reagent. In other embodiments, at least one testing zone **23** includes a detection reagent that is different from the detection reagent on a second testing zone **23**. In certain embodiments, inlet zones **21** are loaded simultaneously.

[0050] The “sewn array” configuration has several characteristics that are well-suited for assays. First, every pair of stitches (i.e., a portion of the thread that spans both sides of the substrate) can serve as a different assay. Second, the fluid sample travels a short distance and therefore the response of the device can be fast. Third, the “sewn array” can be incorporated into clothing, bandages, or diapers. The stitches close to the skin can serve as the inlet zones, while the stitches on the exterior side of the device can serve as the testing zones, where they can be easily observed in a non-intrusive manner.

Biological Samples

[0051] The diagnostic systems described herein can be used for assaying small volumes of biological samples, e.g., fluid samples. Biological samples that can be assayed using the diagnostic systems described herein include, e.g., urine, whole blood, blood plasma, blood serum, cerebrospinal fluid, ascites, tears, sweat, saliva, excrement, gingival cervicular fluid, or tissue extract.

[0052] In some embodiments, the volume of fluid sample to be assayed can be a drop of blood, e.g., from a finger prick, or a small sample of urine, e.g., from a newborn or a small animal.

Applications

[0053] The hydrophilic diagnostic threads described herein have many applications in modern medicine (e.g., in sports medicine, infant/child diagnostics, diabetes monitoring, military, underwater/diving monitoring, diagnostic dental floss, etc.). Additionally, the diagnostic systems described herein can be utilized in applications in which low cost is a concern, e.g., healthcare in the less-industrialized world, military and homeland security operations, environmental, on-site testing.

[0054] For example, hydrophilic diagnostic threads can be woven or knitted into clothing using existing technology, such as high-speed shuttleless weaving machines (e.g., at 2000 meters per minute). Such embodiments can provide, e.g., ubiquitous and continuous monitoring of subjects, such as soldiers in the field. In other embodiments, hydrophilic diagnostic threads can be woven into bandages.

[0055] In another embodiment, the diagnostic systems described herein can be used in diapers, e.g., to monitor premature babies. In one embodiment, a thread is located at the proper place inside the diaper, which leads to the external surface of the diaper. Urine is loaded into the inlet zone of the thread, which is then used to load diagnostic threads located on the external surface of the diaper, where colorimetric indicators can be read by a nurse/technician/doctor.

[0056] In other embodiments, diagnostic hydrophilic threads can be incorporated into paper or other assay mediums. For example, a thin sheet of paper can be placed between the protective laminates as the assay medium and the thread could be used to deliver the analyte to a precise location on the paper. For example, hydrophilic paper, patterned into channels with hydrophobic lines of polymer (as described in PCT/US07/081848), can be used in combination with the threads described herein. In these devices, the flow of fluid is driven by capillarity.

[0057] The invention is further illustrated by the following examples. The examples are provided for illustrative purposes only. They are not to be construed as limiting the scope or content of the invention in any way.

EXAMPLES

Example 1 – Preparation and Use of a “Woven Array” Diagnostic System

Thread

[0058] In some diagnostic systems, 100% cotton thread with a diameter of 0.3mm was used (Cebelia Crochet Cotton Art G167, DMC, NJ, USA). This thread was of sufficient width to be enable analyte detection by the naked eye and reducing the loss of detection due to the presence of the analyte within the interior of the thread. The thread was manufactured by a process that included mercerization (exposure of a thread under tension to a NaOH bath, followed by neutralization with acid). This process increased the strength of the thread and its absorbency of water. The ability of Nylon thread (unwaxed dental floss, CVS Pharmacy Inc., RI, USA) and 100% polyester thread (McMaster-Carr, NJ, USA) to wick fluids was also tested. These artificial fibers may be well-suited for applications where transparency of the thread is needed to index-match with biological fluids.

Housings

[0059] In some of the diagnostic systems, the thread was encapsulated between two pieces of transparent, water-impermeable, polymer tape. The tape (i) acted as a substrate onto which the thread could be arranged and supported, (ii) served as a “handle” by which the device could be manipulated, labeled, stored, dispensed, and used, (iii) protected the assays from the environment; and, (iv) minimized evaporation, which could alter the concentration or rate of wicking of the analyte.

[0060] Two types of tape were tested: (i) multipurpose tape (Scotch®MultiTask Tape) and, (ii) vinyl tape with rubber adhesive backing (3M™ Vinyl Tape #471). The vinyl tape is able to make complete conformal contact with its substrate (in this case, the thread). The Scotch tape combines crystal clarity, strength and moisture resistance for performance over a wide range of taping tasks, but does not adhere conformally to the entire surface of the thread.

[0061] To ensure good contact between the tape and the thread, laminator (Pro-Etch laminator, Micro-Mark) was used. The laminator sandwiched the thread

between two pieces of tape using heat and pressure. The laminator was used in its “hot mode” and used to laminate the tape and thread within seconds.

Device Preparation

[0062] For the fabrication of the “woven array” device (depicted in Figure 1A), a loom was used to arrange several threads in parallel to each other. The loom was made by installing steel pins (McMaster-Carr, NJ, USA) into a 1.5 cm thick Derlin block (two parallel rows of pins, 6 cm apart, with the pins in each row spaced by 0.5 cm). A piece of tape was inserted underneath the threads, the threads were pressed against the tape to make intimate contact between the tape and the thread, and a second piece of tape was pressed on top of the threads to encapsulate them between the two pieces of tape (Figure 5). To disconnect the thread from the loom, the thread was cut where it contacted the pins of the loom and a laminator was used to make a better contact between the thread and the tape (Figure 5). The threads of the device were cut such that one end of each piece of thread (i.e., “branch”) protruded from the tape portion of the device and served as the inlet zone. To facilitate the application of the sample, the device was rolled such that the ends of the threads converged to a single point (Figure 6A). The length of each thread that protruded from the device was long enough to allow their convergence.

Assays

[0063] The colorimetric assay for protein was based on the binding of tetrabromophenol blue (TBPB) to protein; TBPB changes from yellow to blue through the dissociation of phenolic hydroxyl groups at a pH of about 3 when a protein is present. For protein detection, a solution of 0.5 μ L of 250 mM citric acid (pH 1.8) and 0.5 μ L 3.3 mM tetrabromophenol blue (TBPB) in 95% ethanol was spotted onto the testing zone of the thread using a pipetman.

[0064] To detect glucose, the enzymatic oxidation of iodide to iodine was used; this reaction induces a color change from colorless to yellowish-brown in the presence of glucose. For this assay, 0.5 μ L of 0.6 M solution of potassium iodide and 0.5 μ L of a 1:5 horseradish peroxidase/glucose oxidase solution (15 units of protein per 1 ml of solution) was spotted onto the testing zone of the thread using a pipetman.

[0065] After spotting the reagents at the desired locations, the thread was laminated between two pieces of tape using a laminator (Pro-Etch laminator, Micro-Mark, USA).

[0066] To test the wicking properties of the woven array configuration, the tape portion of the device was rolled and the protruding ends of the threads (i.e., the inlet zones) were dipped in different volumes of red ink. To load a device composed of nine threads, about 30 μ l of ink was used. The solution wicked along the threads rapidly, at a rate of about 2.5 cm/min (see Figure 6B).

[0067] To test the ability to perform diagnostic colorimetric assays with the device, a pipette was used to spot the tip of each piece of thread (prior to encapsulating the thread with tape) with the reagents for colorimetric assays that detect the level of glucose and protein in urine. The reagents were dried in ambient conditions for about 1 hour. After spotting the reagents onto the thread, the device was sealed with another piece of tape, the device was disconnected from the loom, it was laminated it.

[0068] Figure 6C, depicts a device 2 minutes after adding a 30 μ l sample of artificial urine that contained 75 μ M BSA and 500mM glucose. Both assays were performed in duplicate and in parallel. When the sample was applied, the fluid wicked along the thread. The enzymatic reaction of the glucose assay required oxygen for its activity, and therefore color appeared at the end of the thread where it was exposed to air. TBPB reacted with the sample as soon as the sample reached the detection zone, and therefore a change in color was observed closer to the inlet zone.

[0069] The minimum detection levels were 2.5 mM for glucose and 0.5 μ M for BSA (defined as the minimum concentration that generated a color response observable by the unaided eye). Color changes in the thread were apparent about 10 seconds after spotting the sample, and the colors reached their maximum intensity after 2 min. These response times are similar to those of conventional dipsticks.

Modifications to Threads

[0070] To improve the wicking properties (i.e., the speed in which the thread wicks fluids) of the thread, the thread was plasma oxidized for 5 minutes. This procedure improved the wicking properties of the thread from 1.25 cm/min to 2.5

cm/min. The wicking properties of Nylon threads and polyester threads were also examined. Both the Nylon thread and the polyester threads wicked at a rate of 5 cm/min. Although these threads wicked faster than cotton thread, their adherence to the tape was weaker than the cotton thread. Thus, these threads could be useful in devices that require faster wicking and do not entail the encapsulation of a thread within tape.

[0071] In another method to modify the wicking properties of the thread, a hydrophobic coating (petroleum jelly or wax) was placed on the outer side of the hydrophilic thread. When the thread was subsequently laminated between two pieces of Scotch tape, wicking was observed only within the thread (Figure 7). The use of petroleum jelly also facilitated removal of the thread from the encapsulating tape (Figure 7). This method can be used to separate the thread from the tape for further analysis of the analytes on the thread.

Modifications to Housing

[0072] Different tapes were tested for their effects on the wicking properties of threads encapsulated within the tape. Both vinyl tape and clear Scotch tape were used to fabricate the woven device. When vinyl tape was used to fabricate the device, the tape softened upon lamination and formed a conformal seal around the threads. The Scotch tape, however, did not form a conformal seal and thus created a small gap between the tape adjacent to the thread.

[0073] This difference between the tapes affected the wicking properties of the device. The difference was observed upon dipping the thread protruding from the tape, along with a small portion of the tape, into a solution of red ink (Figure 8). The vinyl tape formed a tight seal with the thread. The seal ensured that the solution only wicked through the thread (which was observed under an optical microscope). The Scotch tape did not form a conformal seal around the threads, and the solution wicked both through the threads and through a small gap between the tape and the thread (see Figure 8B and Figure 4). This gap effectively formed a fluidic channel. The wicking through the gap was faster (6 cm/min) than the wicking through the thread (1.25 cm/min).

[0074] When the threads were laminated between one piece of Scotch tape and one piece of vinyl tape and the bottom of the device was submerged into the ink

solution, the ink wicked through a gap between the tape and the thread. This gap was significantly smaller than the gap formed with the threads laminated between two pieces of Scotch tape (Figure 8C).

[0075] No difference was seen between the wicking behavior of the two tapes when only the tips of the threads (and not the edge of the two pieces of tape) were dipped into a solution of red ink. For both devices, the threads wicked the ink solution.

[0076] Both types of contacts made by the tapes are useful. The conformal seal formed by the Vinyl tape ensures that wicking occurs only within the thread such that individual diagnostic assays remain separated and individually encapsulated. The small gap created by the Scotch tape is useful as a capillary to allow rapid wicking through an open-channel.

Example 2 – Preparation and Use of a “Branching Array” Diagnostic System

[0077] A loom as described in Example 1 was used to weave thread into a “branching array” configuration (as illustrated in Figure 1B). The “branching array” illustrated in Figure 1B contains only one inlet zone, which may result in smaller error rate compared to the “woven array” design. However, the “woven array” configuration may have a faster response than that of the “branching array”, because the distance from the inlet zone to the testing zone is shorter.

[0078] A branching array was used to run the colorimetric assays described in Example 1 (Figure 9). Two factors were taken into consideration when determining the lengths of the threads for this device. First, the threads had to be long enough to prevent cross-contamination between the assays through the branching point. Second, the threads had to be longer than the distance that the diagnostic reagents traveled along the thread when preparing the testing zones.

[0079] When the detection reagents were spotted onto each thread, the detection reagents spread by capillary action a distance of about 0.5 cm towards the branching point. Based on this distance, the thread was made at least 2-3 times this length to ensure that no cross contamination would occur and that an intermediate zone existed between the inlet zone and the testing zone.

Example 3 – Preparation of a “Sewn Array” Diagnostic System

[0080] A “sewn array” diagnostic system (as illustrated in Figure 1C) was fabricated by sewing a thread with a needle into a 0.127 mm thick Mylar strip (about 2” x 6”). The assays on two adjacent stitches were physically isolated by blocking every other hole (formed by the needle) in the Mylar with 3 μ L droplets of clear nail polish. Another “sewn array” was fabricated by sewing threads into an all-purpose latex free plastic bandage (CVS Pharmacy, Inc., RI), using the small holes in the bandage as guidelines for sewing the threads.

[0081] One stitch on the bottom side of the substrate and one stitch on the upper side of the substrate constitute one assay (see Figure 1C). The lower stitch (i.e., on the bottom face of the substrate) serves as the inlet zone and the upper stitch (i.e., on the top face of the substrate) serves as the testing zone (Figure 1C). These two stitches were defined as one unit and isolated from the other stitches by applying a 3 μ L drop of clear nail polish to block the holes (formed by sewing) in the substrate, and onto the thread located at these holes.

[0082] To test the wicking properties of the sewn array device, different volumes of red ink were introduced to the inlets. A volume of 0.5 μ L was found to be sufficient to fill a segment of the thread.

[0083] Figure 10A depicts a Mylar strip with four stitches of thread. In Figure 10A, the left two stitches formed one “assay unit”, having an inlet zone on the bottom face of the strip and a testing zone on the top face of the strip. The second set of stitches on the right side of the strip formed a second “assay unit”, with an inlet zone on the bottom face of the strip and a testing zone on the top face of the strip. The first and second assay units were separated by the application of clear nail polish at the hole formed by the thread passing through the strip at this point. Subsequently, 0.5 μ L of a red dye was applied to the inlet zone of the first assay unit on the left, and 0.5 μ L of a blue dye was applied to the inlet zone of the second assay unit on the right. As demonstrated in Figure 10A, the individual assay units did not “bleed” together by capillary action.

[0084] The sewn array design is well-suited for assays embedded in bandages because one side of the device can absorb and wick fluid samples and transport them to a testing zone on the other side of the device. This concept was demonstrated by

sewing thread into a bandage, isolating the “assay units” with clear nail polish, and applying dye to the inlet zones. Figure 10B shows the bottom side of a device that made with a thread sewn into a latex free bandage while Figure 10C shows the top side of the device.

Example 4 – Using Diagnostic Systems to Assay Artificial Urine

[0085] Artificial urine was tested for the presence of four analytes: nitrite, glucose, ketone, and protein. A “woven array”, a “branching array”, and a “sewn array” were prepared as described herein. To detect nitrite, the thread was spotted with 0.5 uL-solution of 2 mg/mL sulfanilamide, 1.7 mg/ml 3-hydroxy-1,2,3,4-tetrahydrobenzo(h)quinoline and 25 mg/mL tartaric acid in methanol. To detect ketone, the thread was spotted with 0.5 uL solution of 20 mg/mL sodium phosphate, 20 mg/mL sodium borate, 10 mg/mL glycine, 0.5 uL solution of 20 mg/mL nitroprusside, 30 mg/mL polyethylenglycol (PEG, Mw = 2000), and 2 mg/ml polyacrylic acid (PAA, Mw = 2000). To detect glucose and protein, the threads were spotted as described in Example 1. Artificial urine was prepared that contained 1mM BSA, 200 mg/ml lithium acetate, 0.5 mM sodium nitrate, and 500 mM glucose.

[0086] The diagnostic colorimetric assay was performed using the “woven array” device by rolling the device and contacting the joined inlet zones with 30 μ L of artificial urine. As shown in Figure 11A, all four analytes were detected.

[0087] The diagnostic colorimetric assay was performed using the “branching array” and “sewn array” devices by contacting the inlet zones with 15 μ L and 0.5 μ L of the artificial urine sample, respectively. As shown in Figures 11B and 11C, the analytes were detected using these two devices.

EQUIVALENTS

[0088] It is to be understood that while the invention has been described in conjunction with the detailed description thereof, the foregoing description is intended to illustrate and not limit the scope of the invention, which is defined by the scope of the appended claims. Other aspects, advantages, and modifications are within the scope of the following claims.

THE EMBODIMENTS OF THE INVENTION FOR WHICH AN EXCLUSIVE PROPERTY OR PRIVILEGE IS CLAIMED ARE DEFINED AS FOLLOWS:

1. A system for performing an assay on a sample comprising one or more hydrophilic testing threads having a high length-to-diameter ratio that avoids lateral transport of fluid within the thread, each thread comprising a sample inlet zone at a proximal end, an intermediate zone distal to the inlet zone through which fluid sample is carried by capillary action, and a testing zone distal to the intermediate zone and comprising a detection reagent which reacts with a predetermined analyte to produce a detectable signal.
2. The system of claim 1 further comprising a housing for support of the hydrophilic testing thread.
3. The system of claim 1, wherein the signal is detectable by a naked eye or a spectrometer.
4. The system of claim 2, wherein at least a portion of the hydrophilic testing thread is enclosed within the housing to protect the hydrophilic testing thread from contamination and mechanical damage.
5. The system of claim 2, wherein the housing comprises two faces, and the hydrophilic testing thread is sewn into the housing and exposed on each face.
6. The system of claim 2, wherein the testing zone is enclosed within and visible from outside the housing.
7. The system of claim 1, wherein the detection reagent is a colorimetric detection reagent.
8. The system of claim 1, wherein the one or more hydrophilic testing threads are part of an array of hydrophilic testing threads for performing multiple assays on the sample.
9. The system of claim 1 comprising a portion of a bandage or cloth.

10. The system of claim 1, wherein the one or more hydrophilic testing threads are part of a woven array of hydrophilic testing threads.
11. The system of claim 2, wherein the one or more hydrophilic testing threads are part of a woven array of hydrophilic testing threads.
12. The system of claim 1, wherein a said hydrophilic testing thread comprises multiple testing zones or multiple inlet zones.
13. The system of claim 2, wherein a said hydrophilic testing thread comprises multiple testing zones or multiple inlet zones.
14. The system of claim 1 for performing multiple assays on the sample further comprising a housing, a hydrophilic loading thread comprising an inlet zone outside the housing, where one or more of said hydrophilic testing threads communicate with said loading thread and at least a portion of the testing threads is enclosed within the housing.
15. The system of claim 14, wherein the signal produced by the detection reagent is apparent to the naked eye.
16. The system of claim 14, wherein at least two testing zones comprise different detection reagents.
17. The system of claim 1, wherein the detection reagent is freely mobile within the testing zone.
18. A method of detecting an analyte in a fluid sample, the method comprising contacting the inlet zone of the system of claim 1 with a sample to induce sample flow by capillary action to the testing zone and visually observing the signal at said testing zone.

19. The method of claim 18 comprising visually observing a plurality of signals at multiple detection zones.

20. The method according to claim 18, wherein the fluid sample is a biological sample that evaporates at the end of the testing zone, resulting in a continued amount of biological sample being wicked through the hydrophilic testing thread to the end of the testing zone.

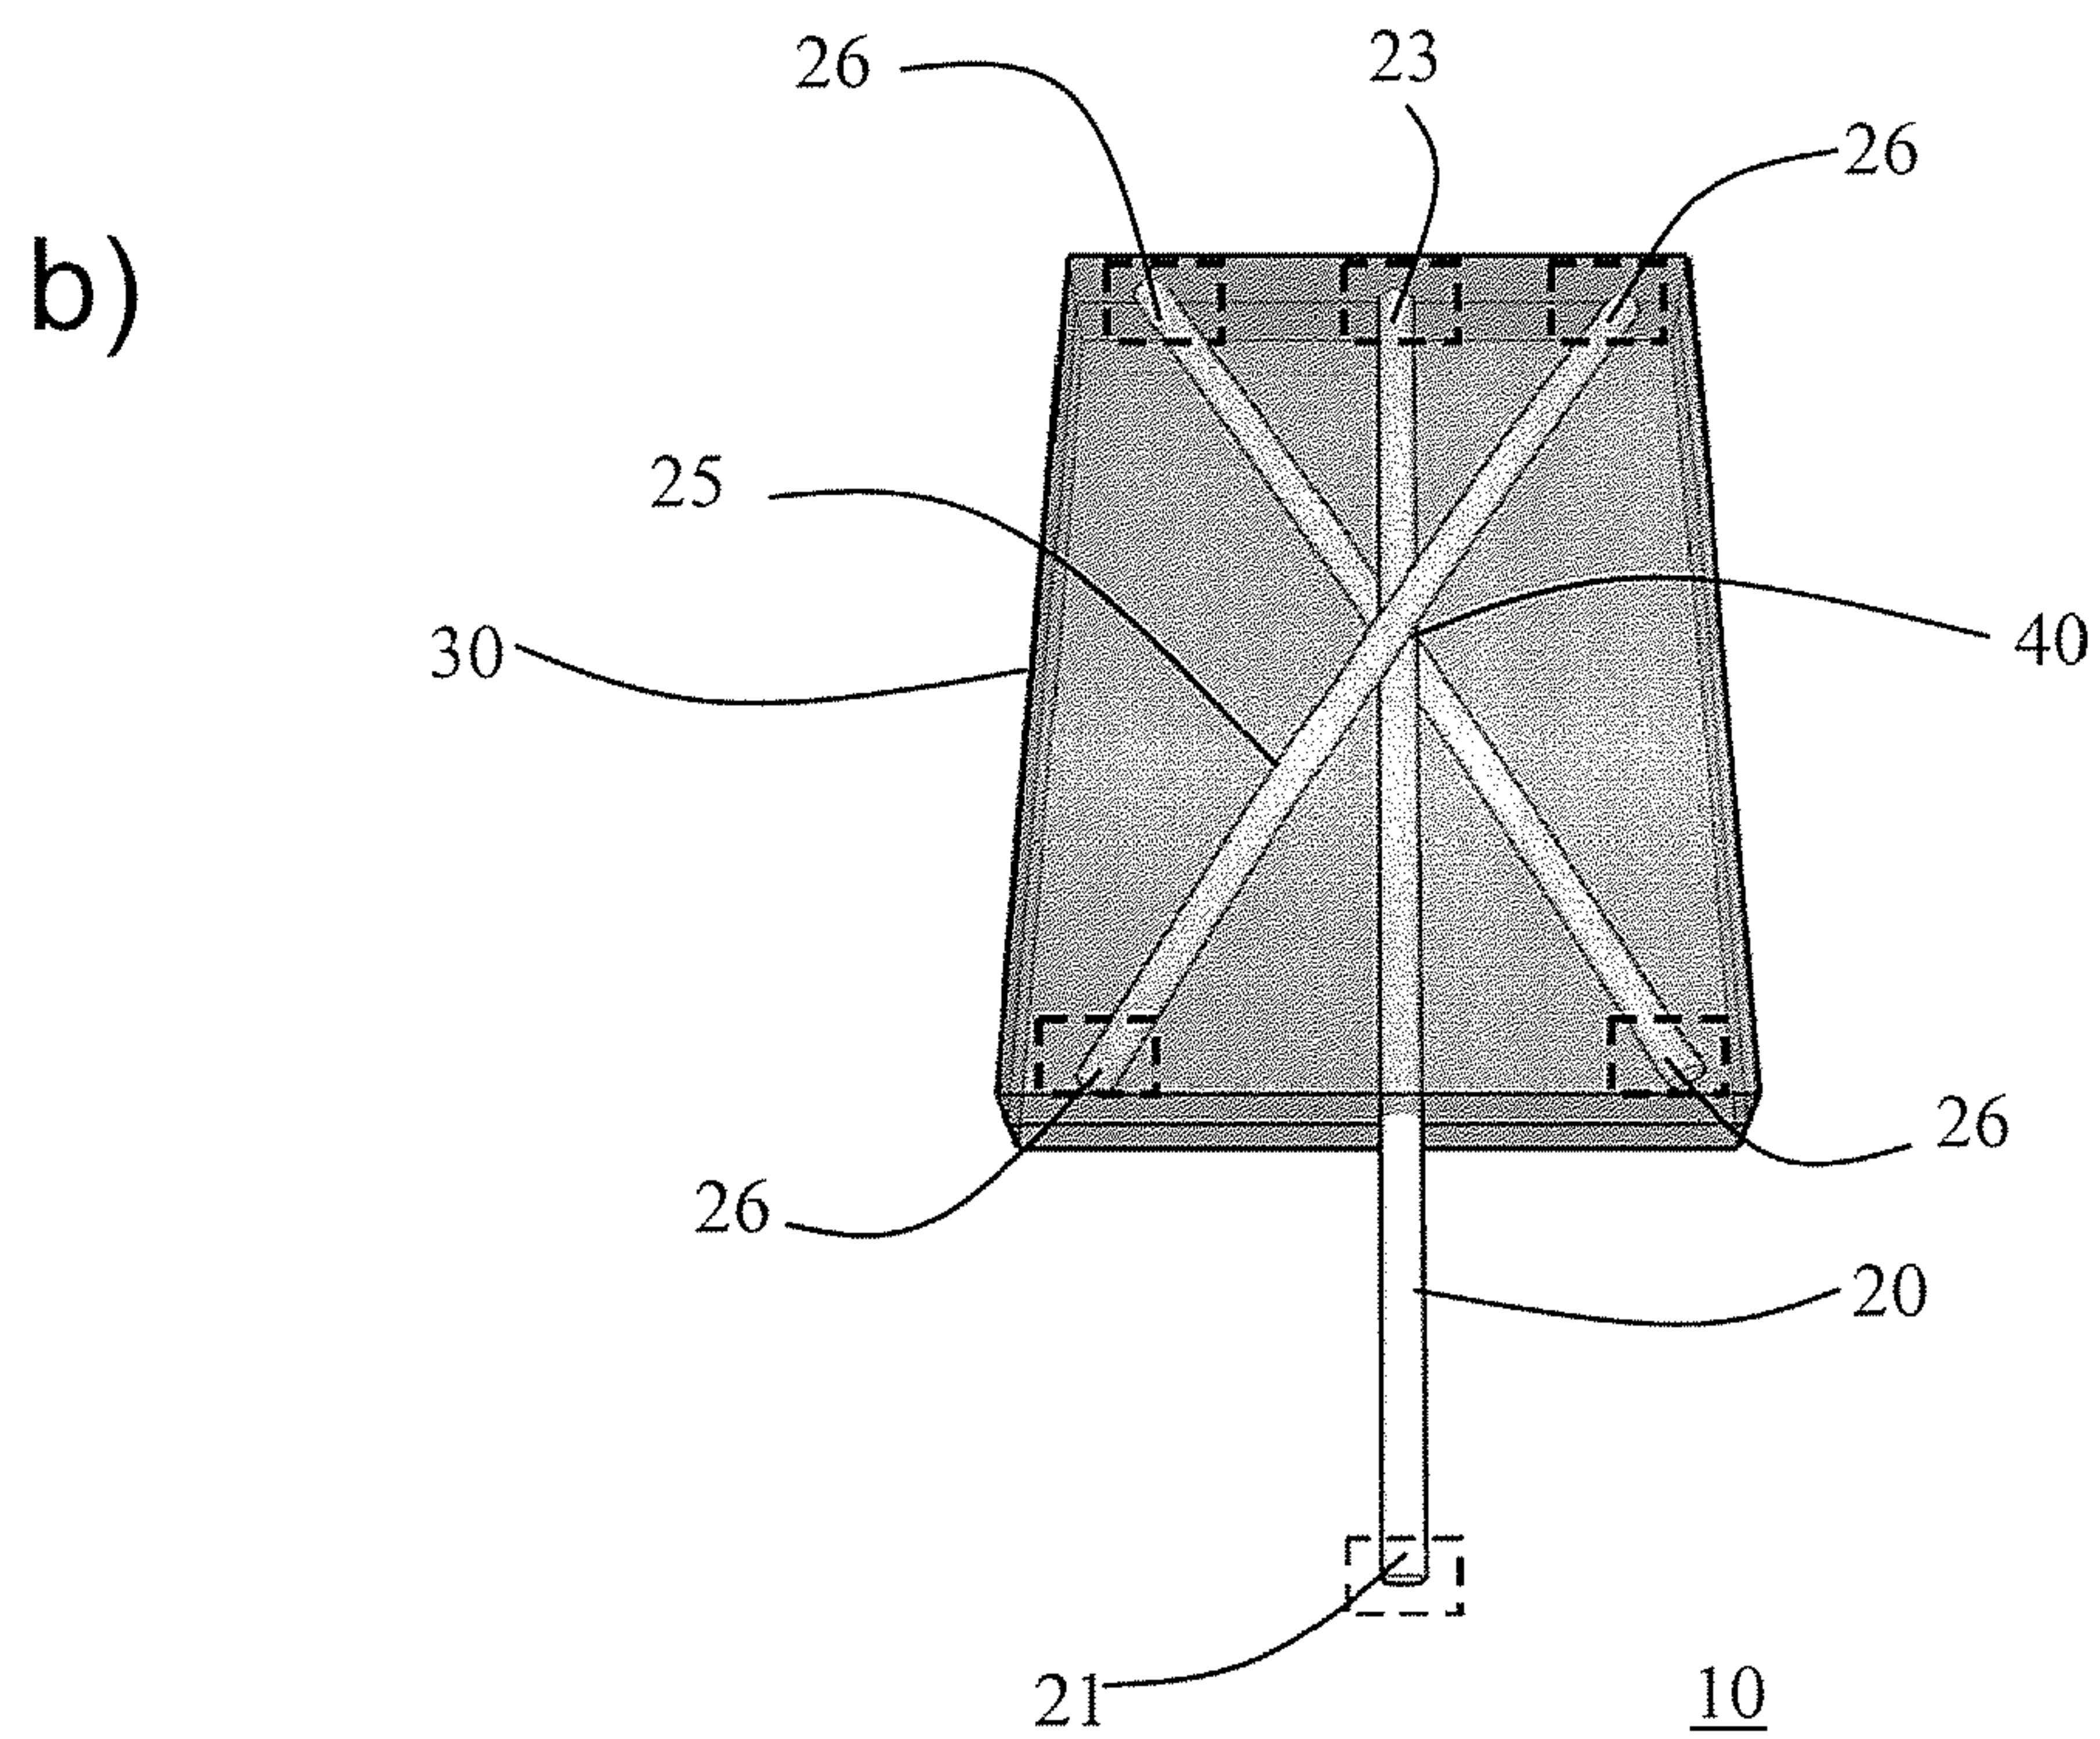
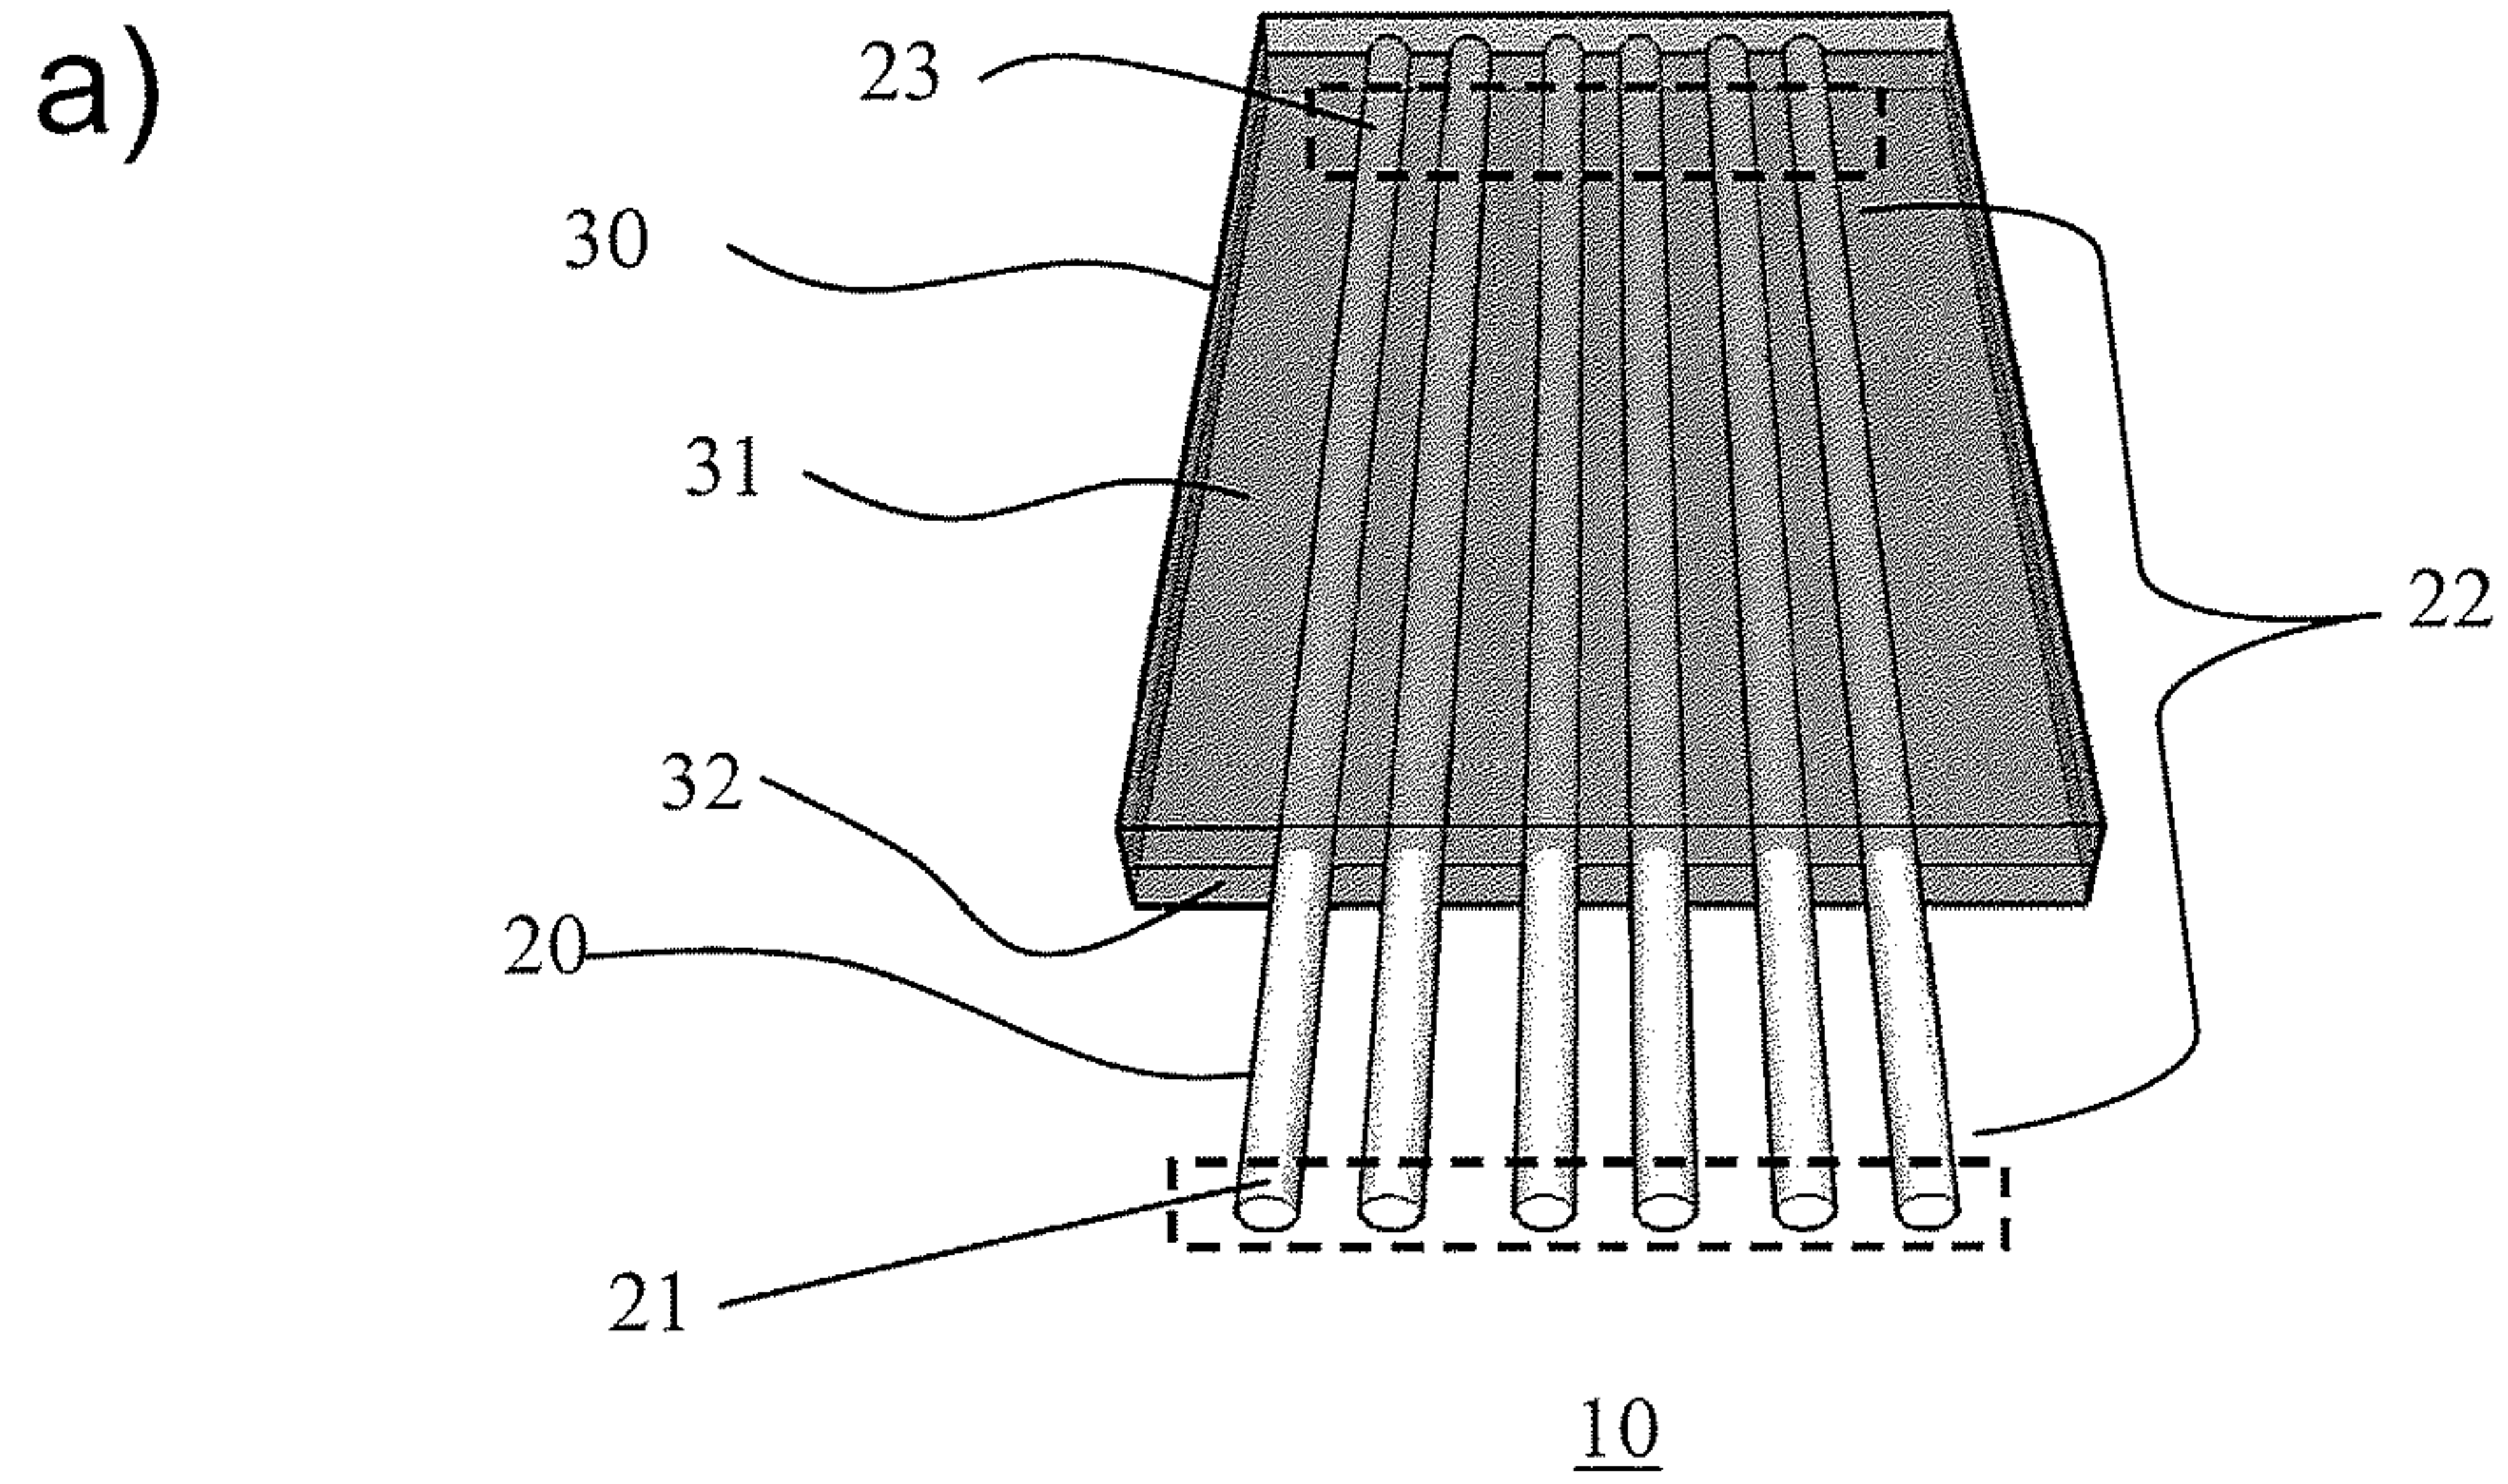


FIG. 1

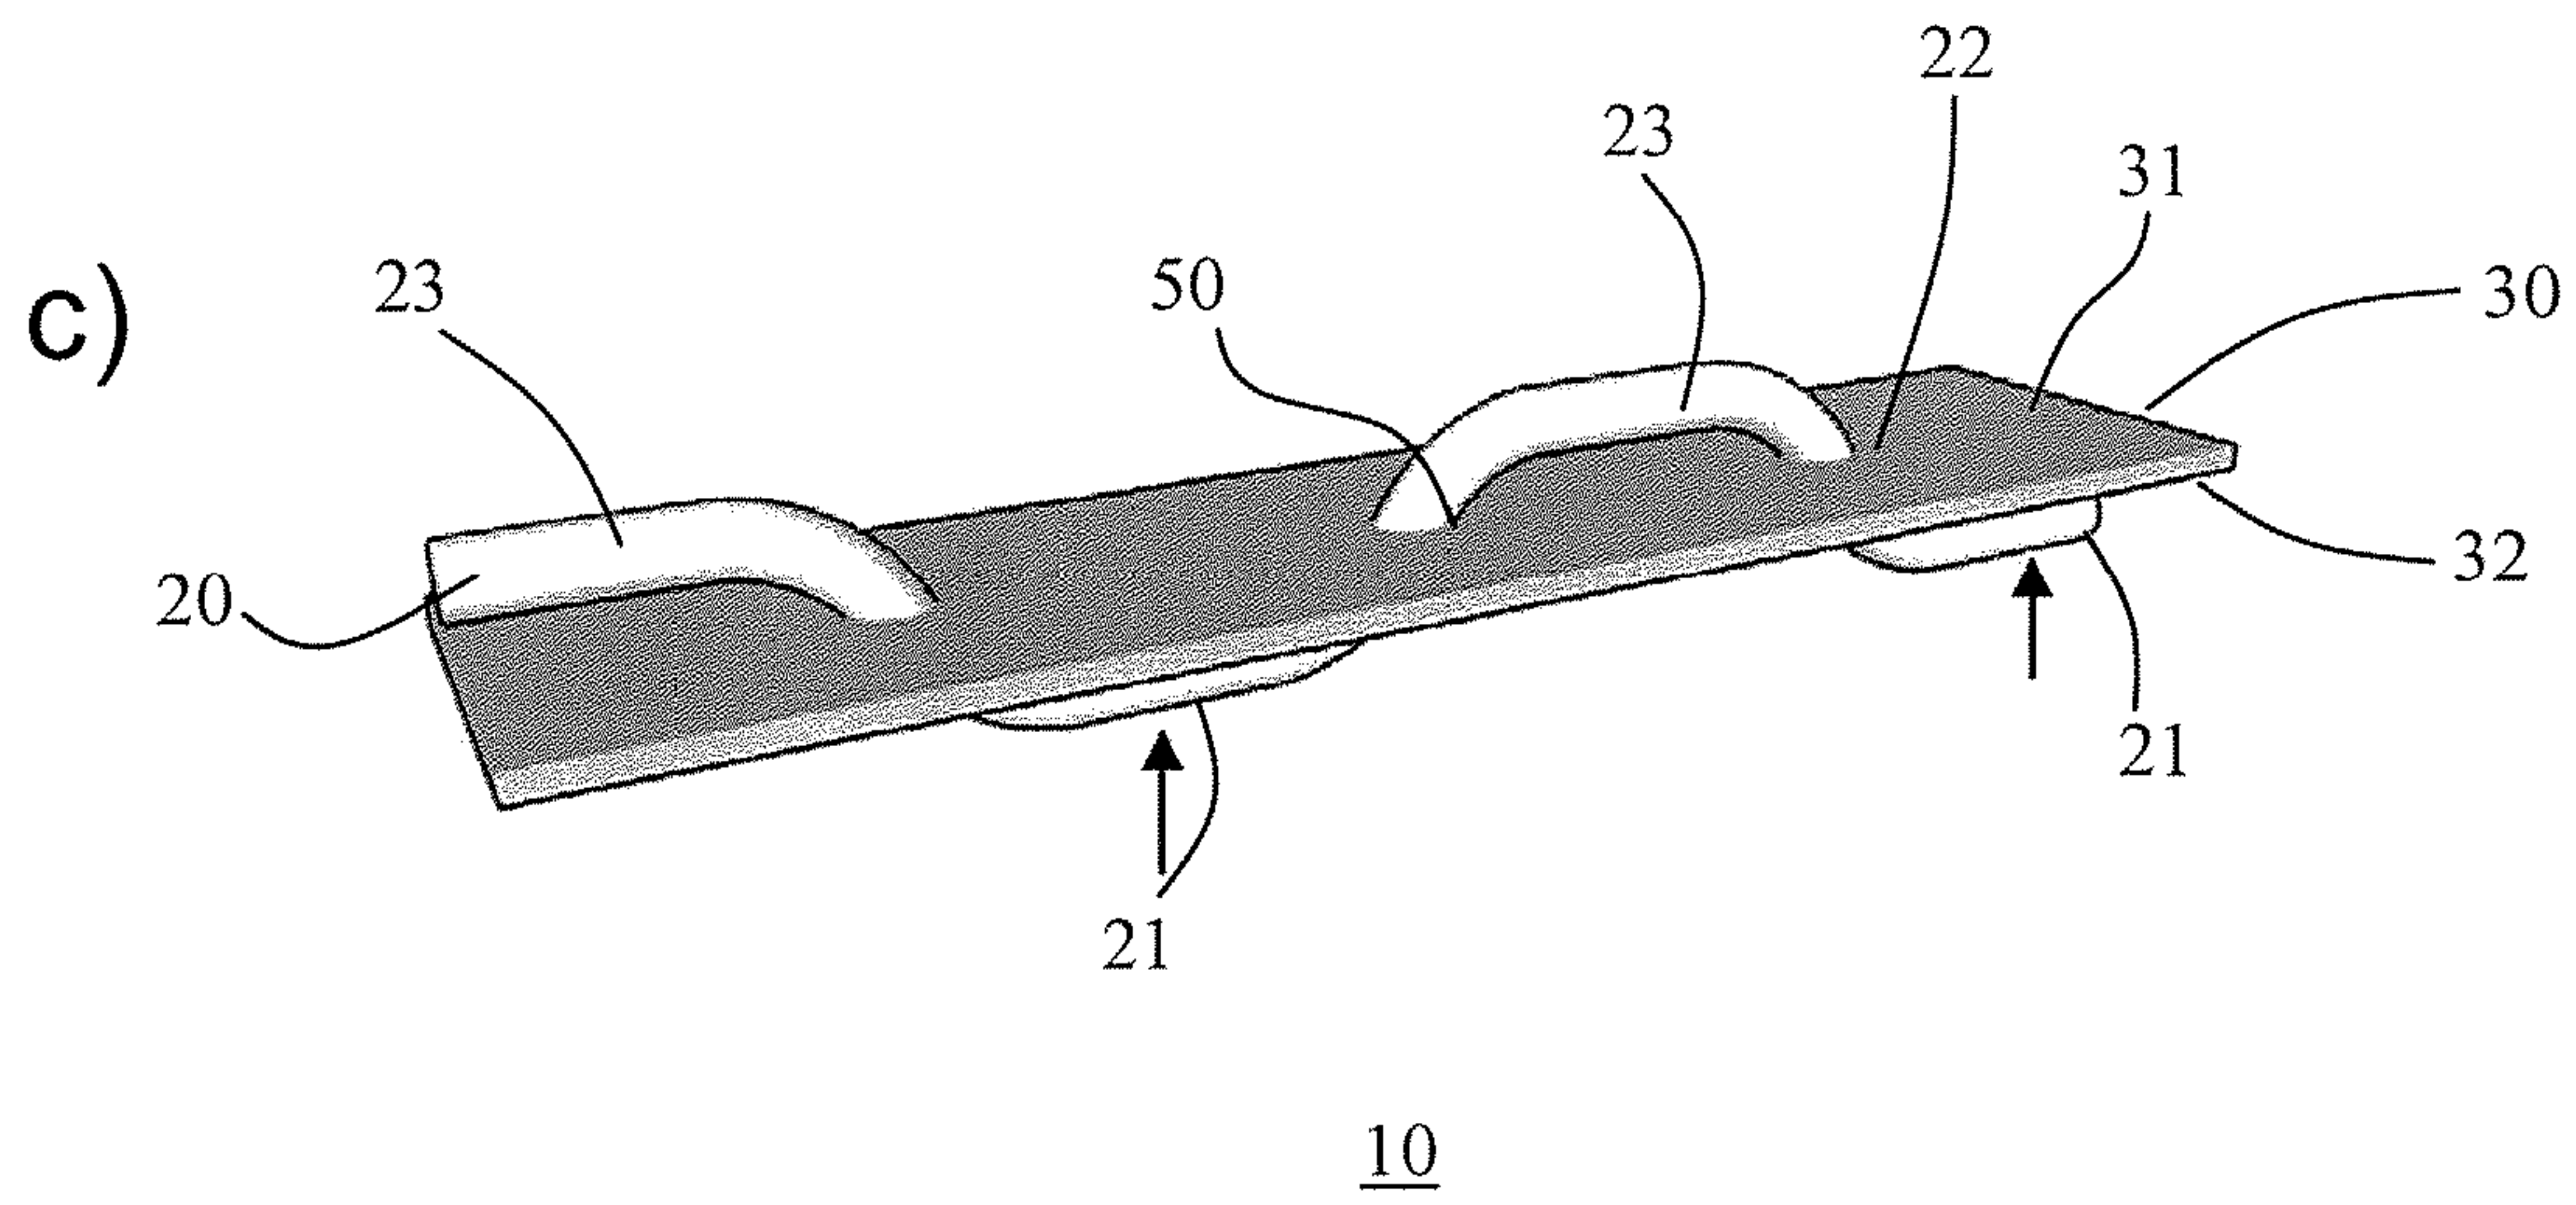


FIG. 1

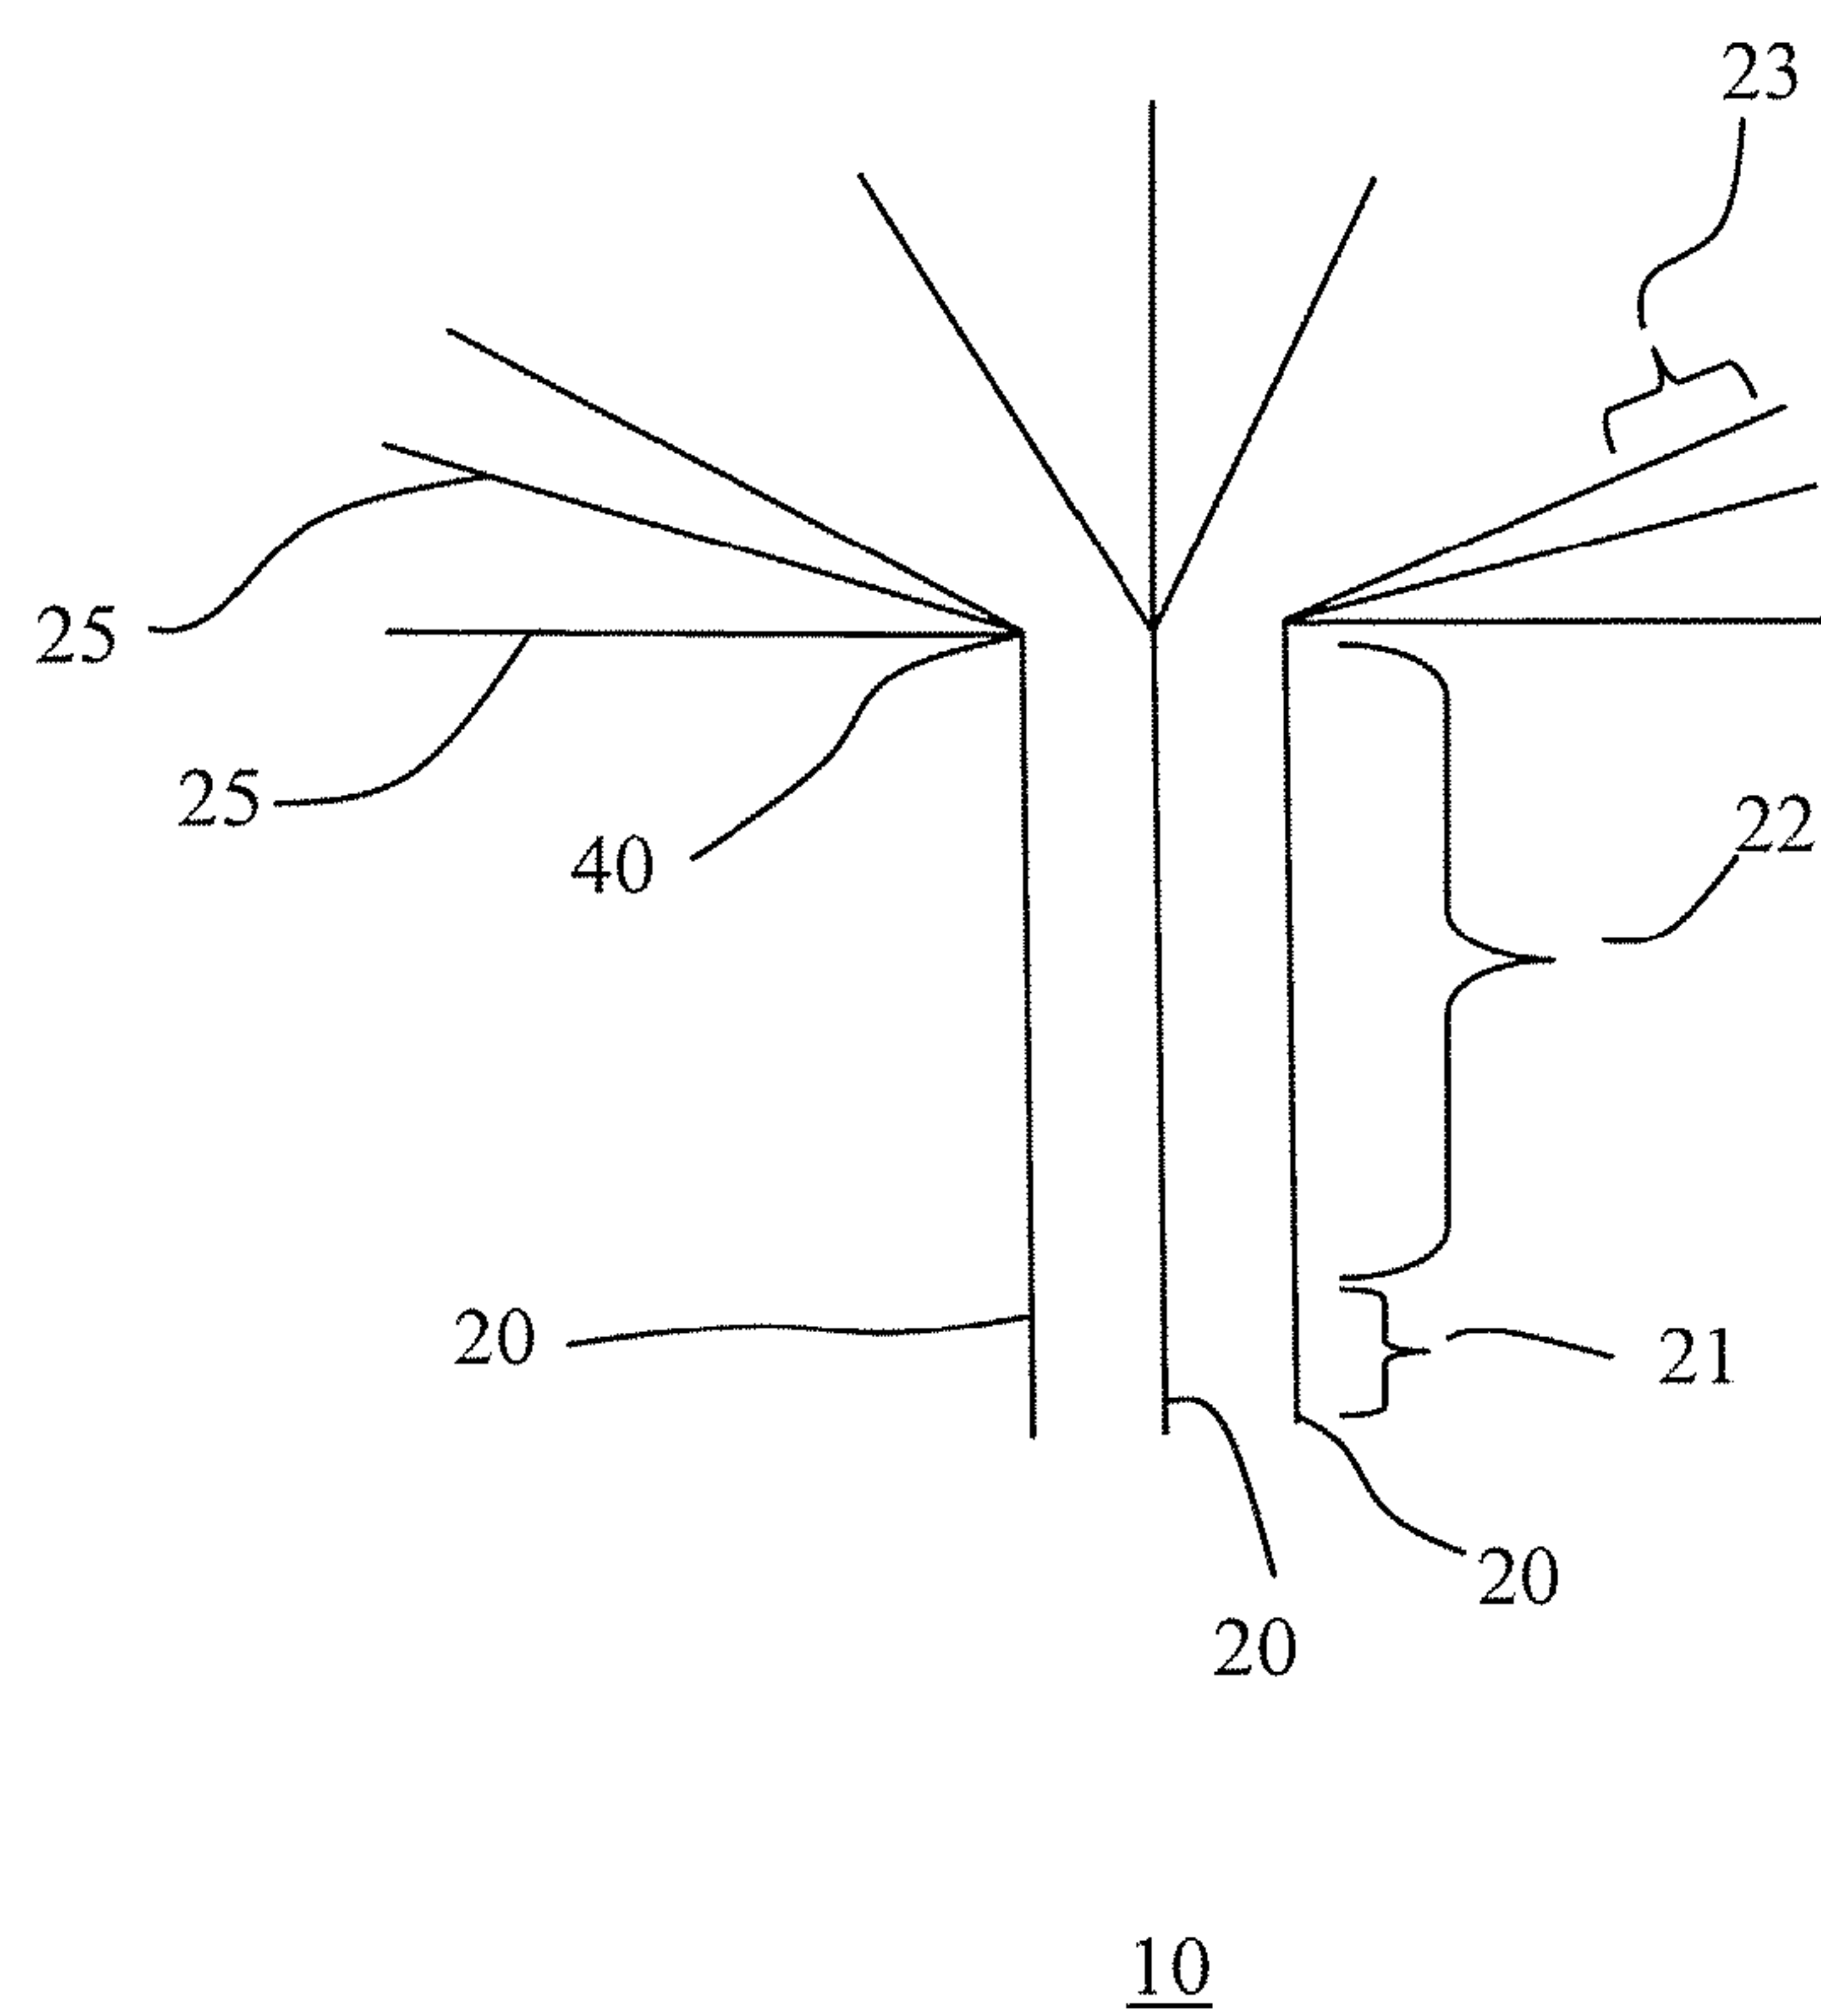


FIG. 2

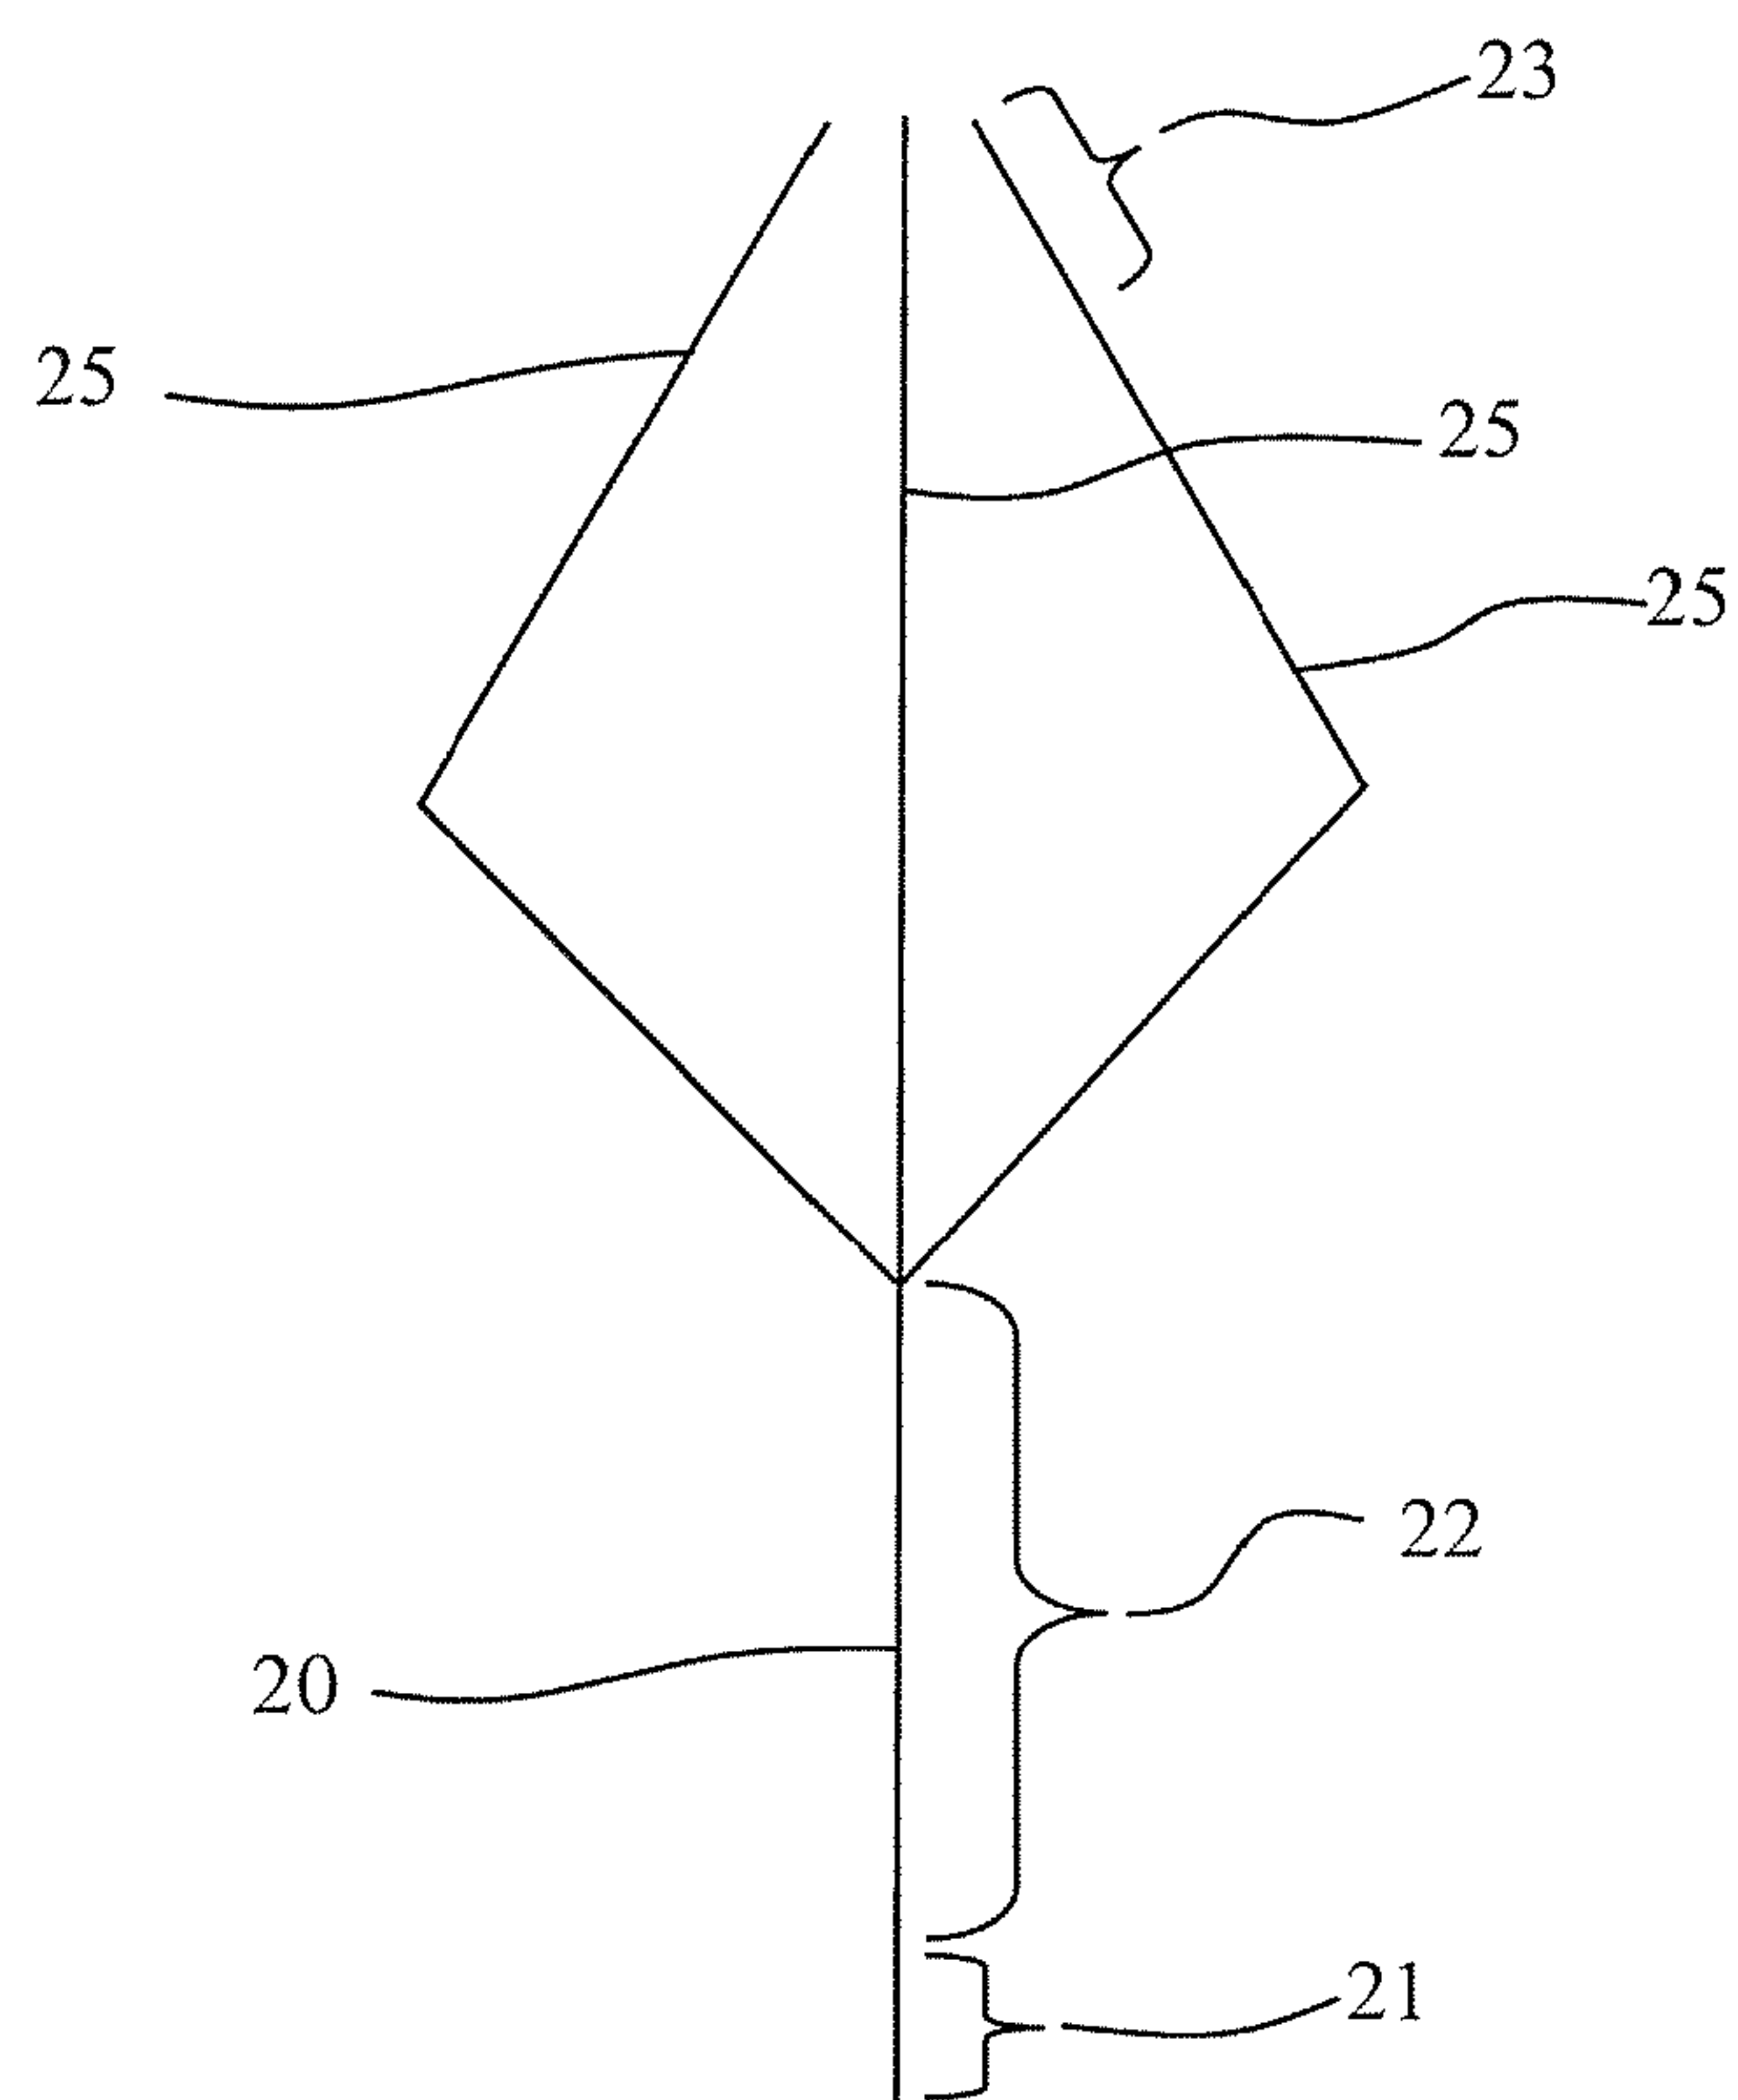


FIG. 3

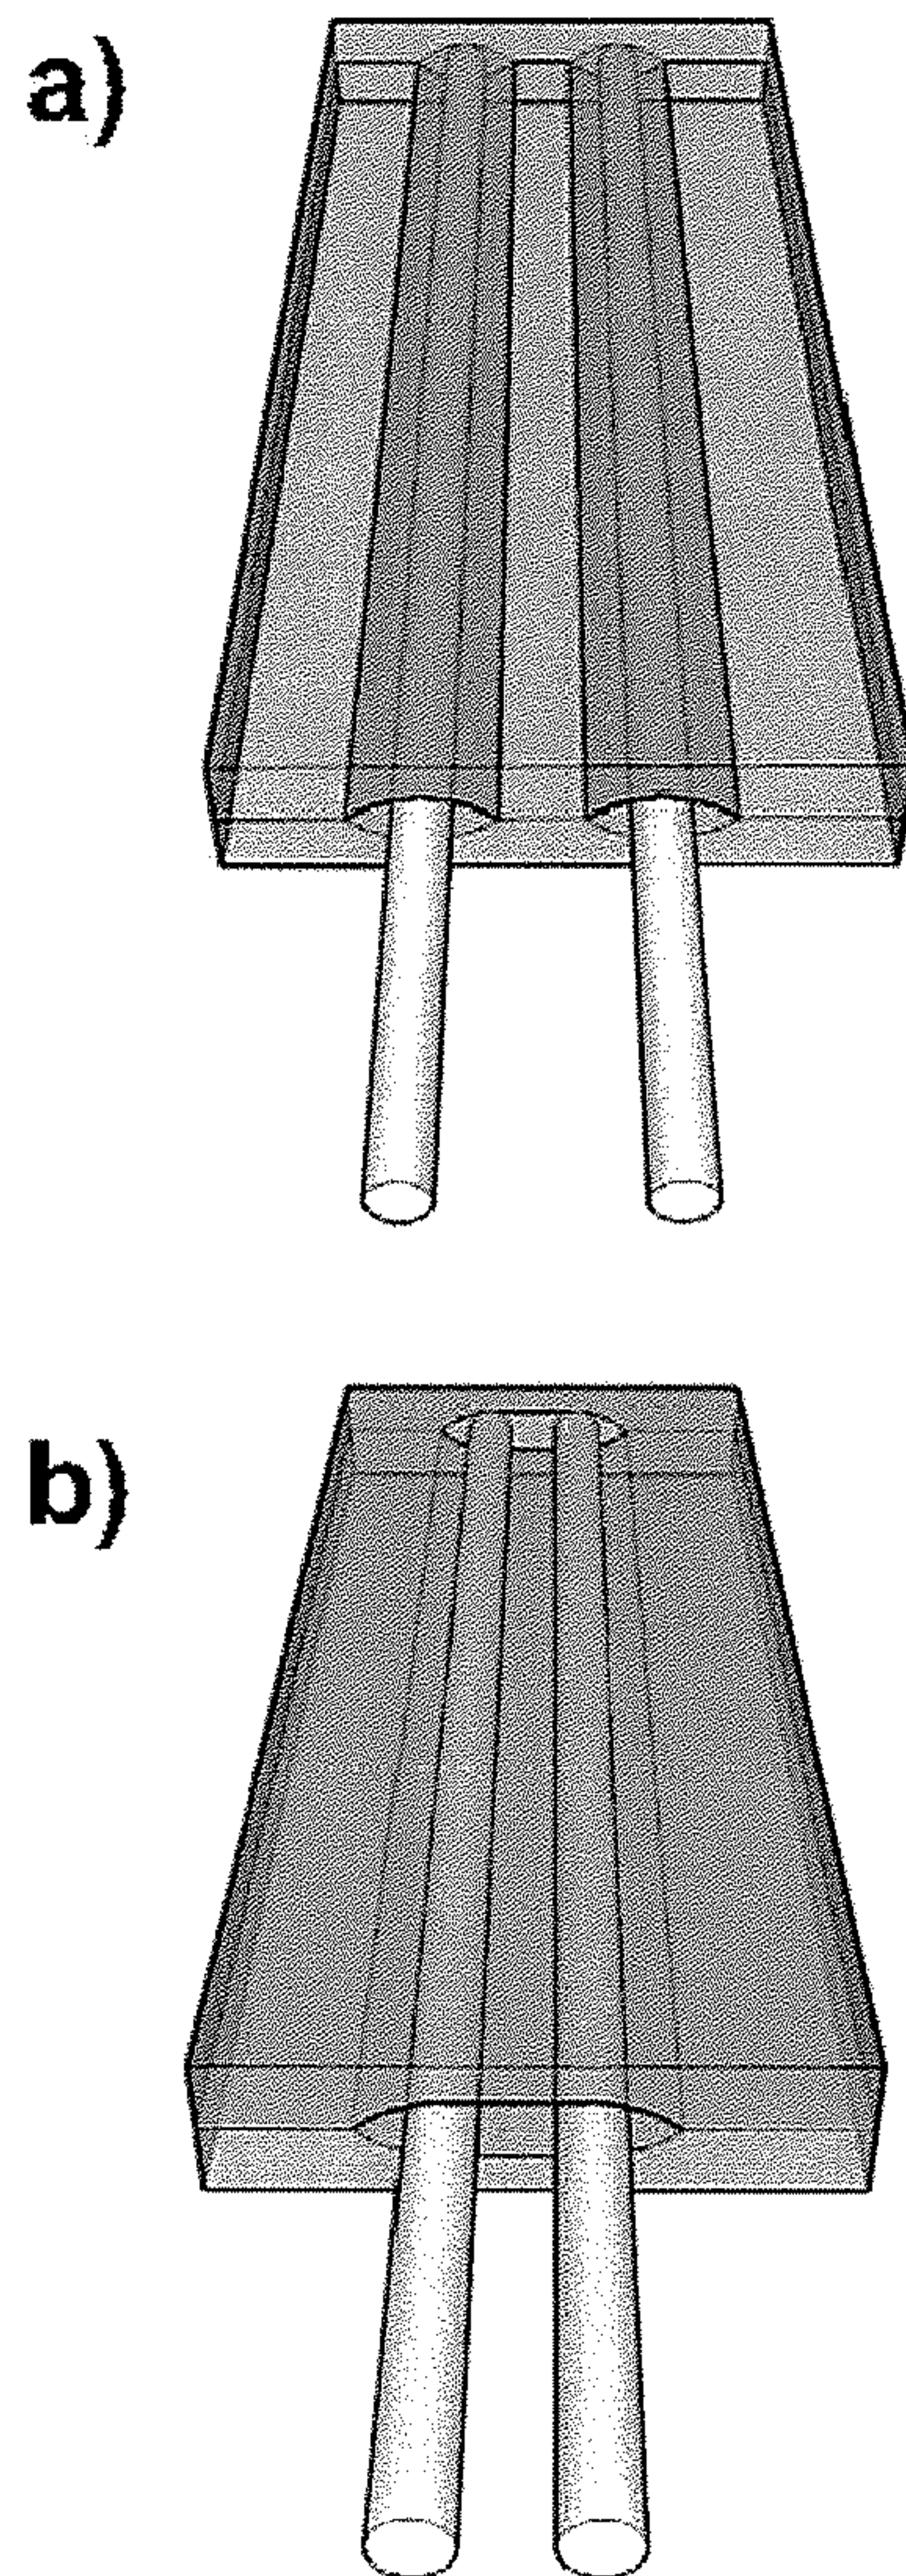


FIG. 4

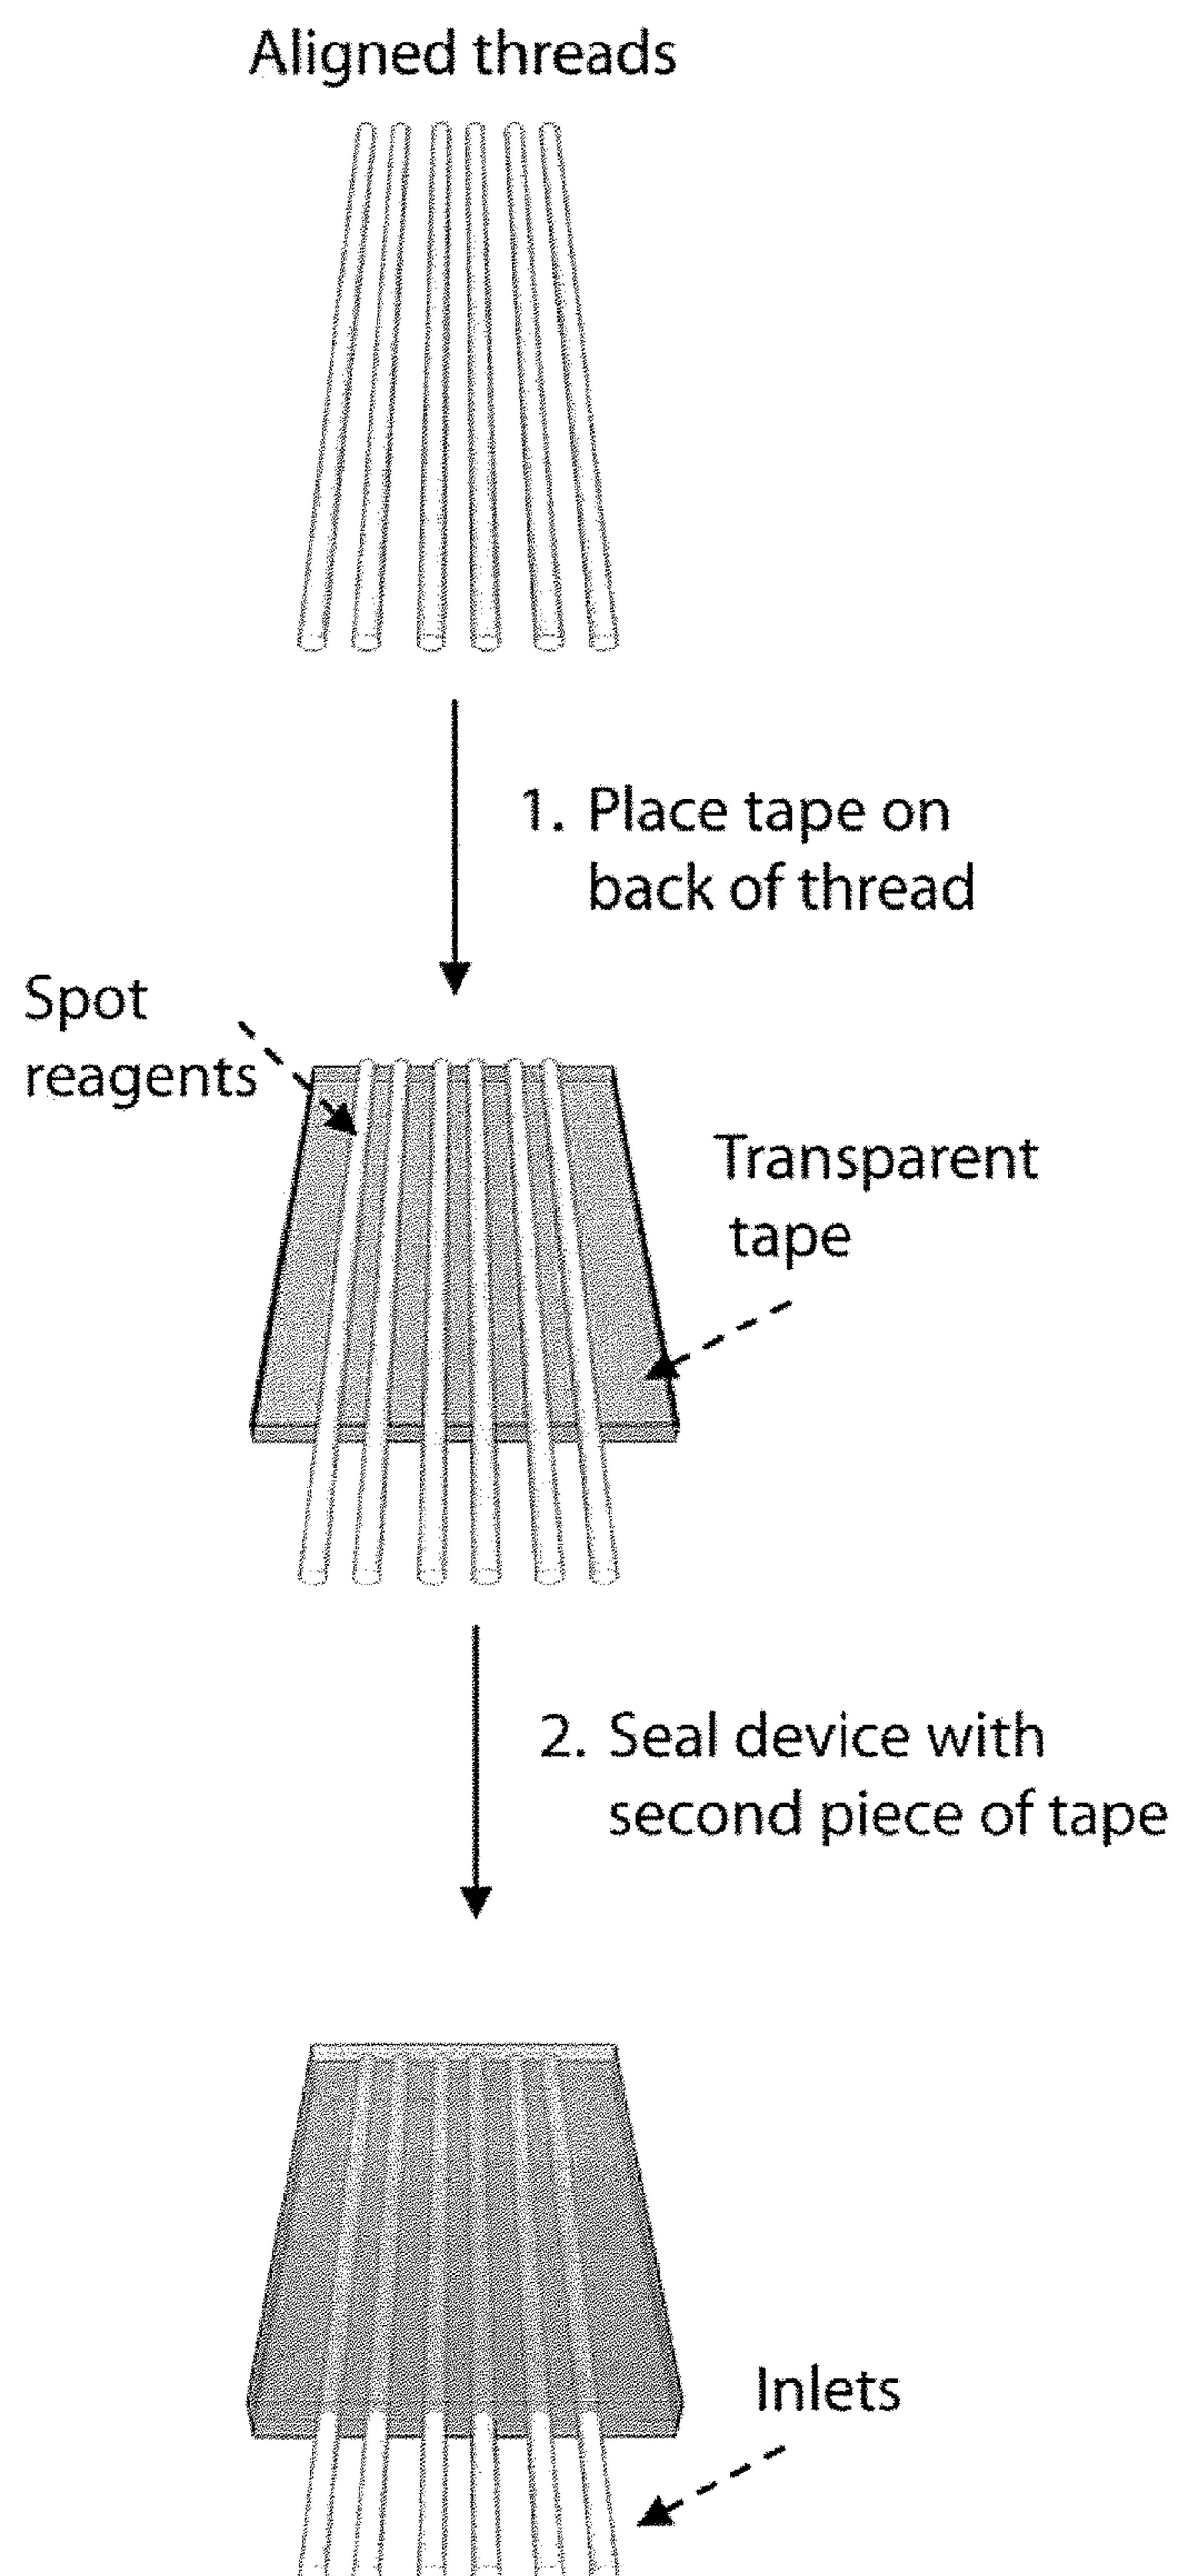


FIG. 5

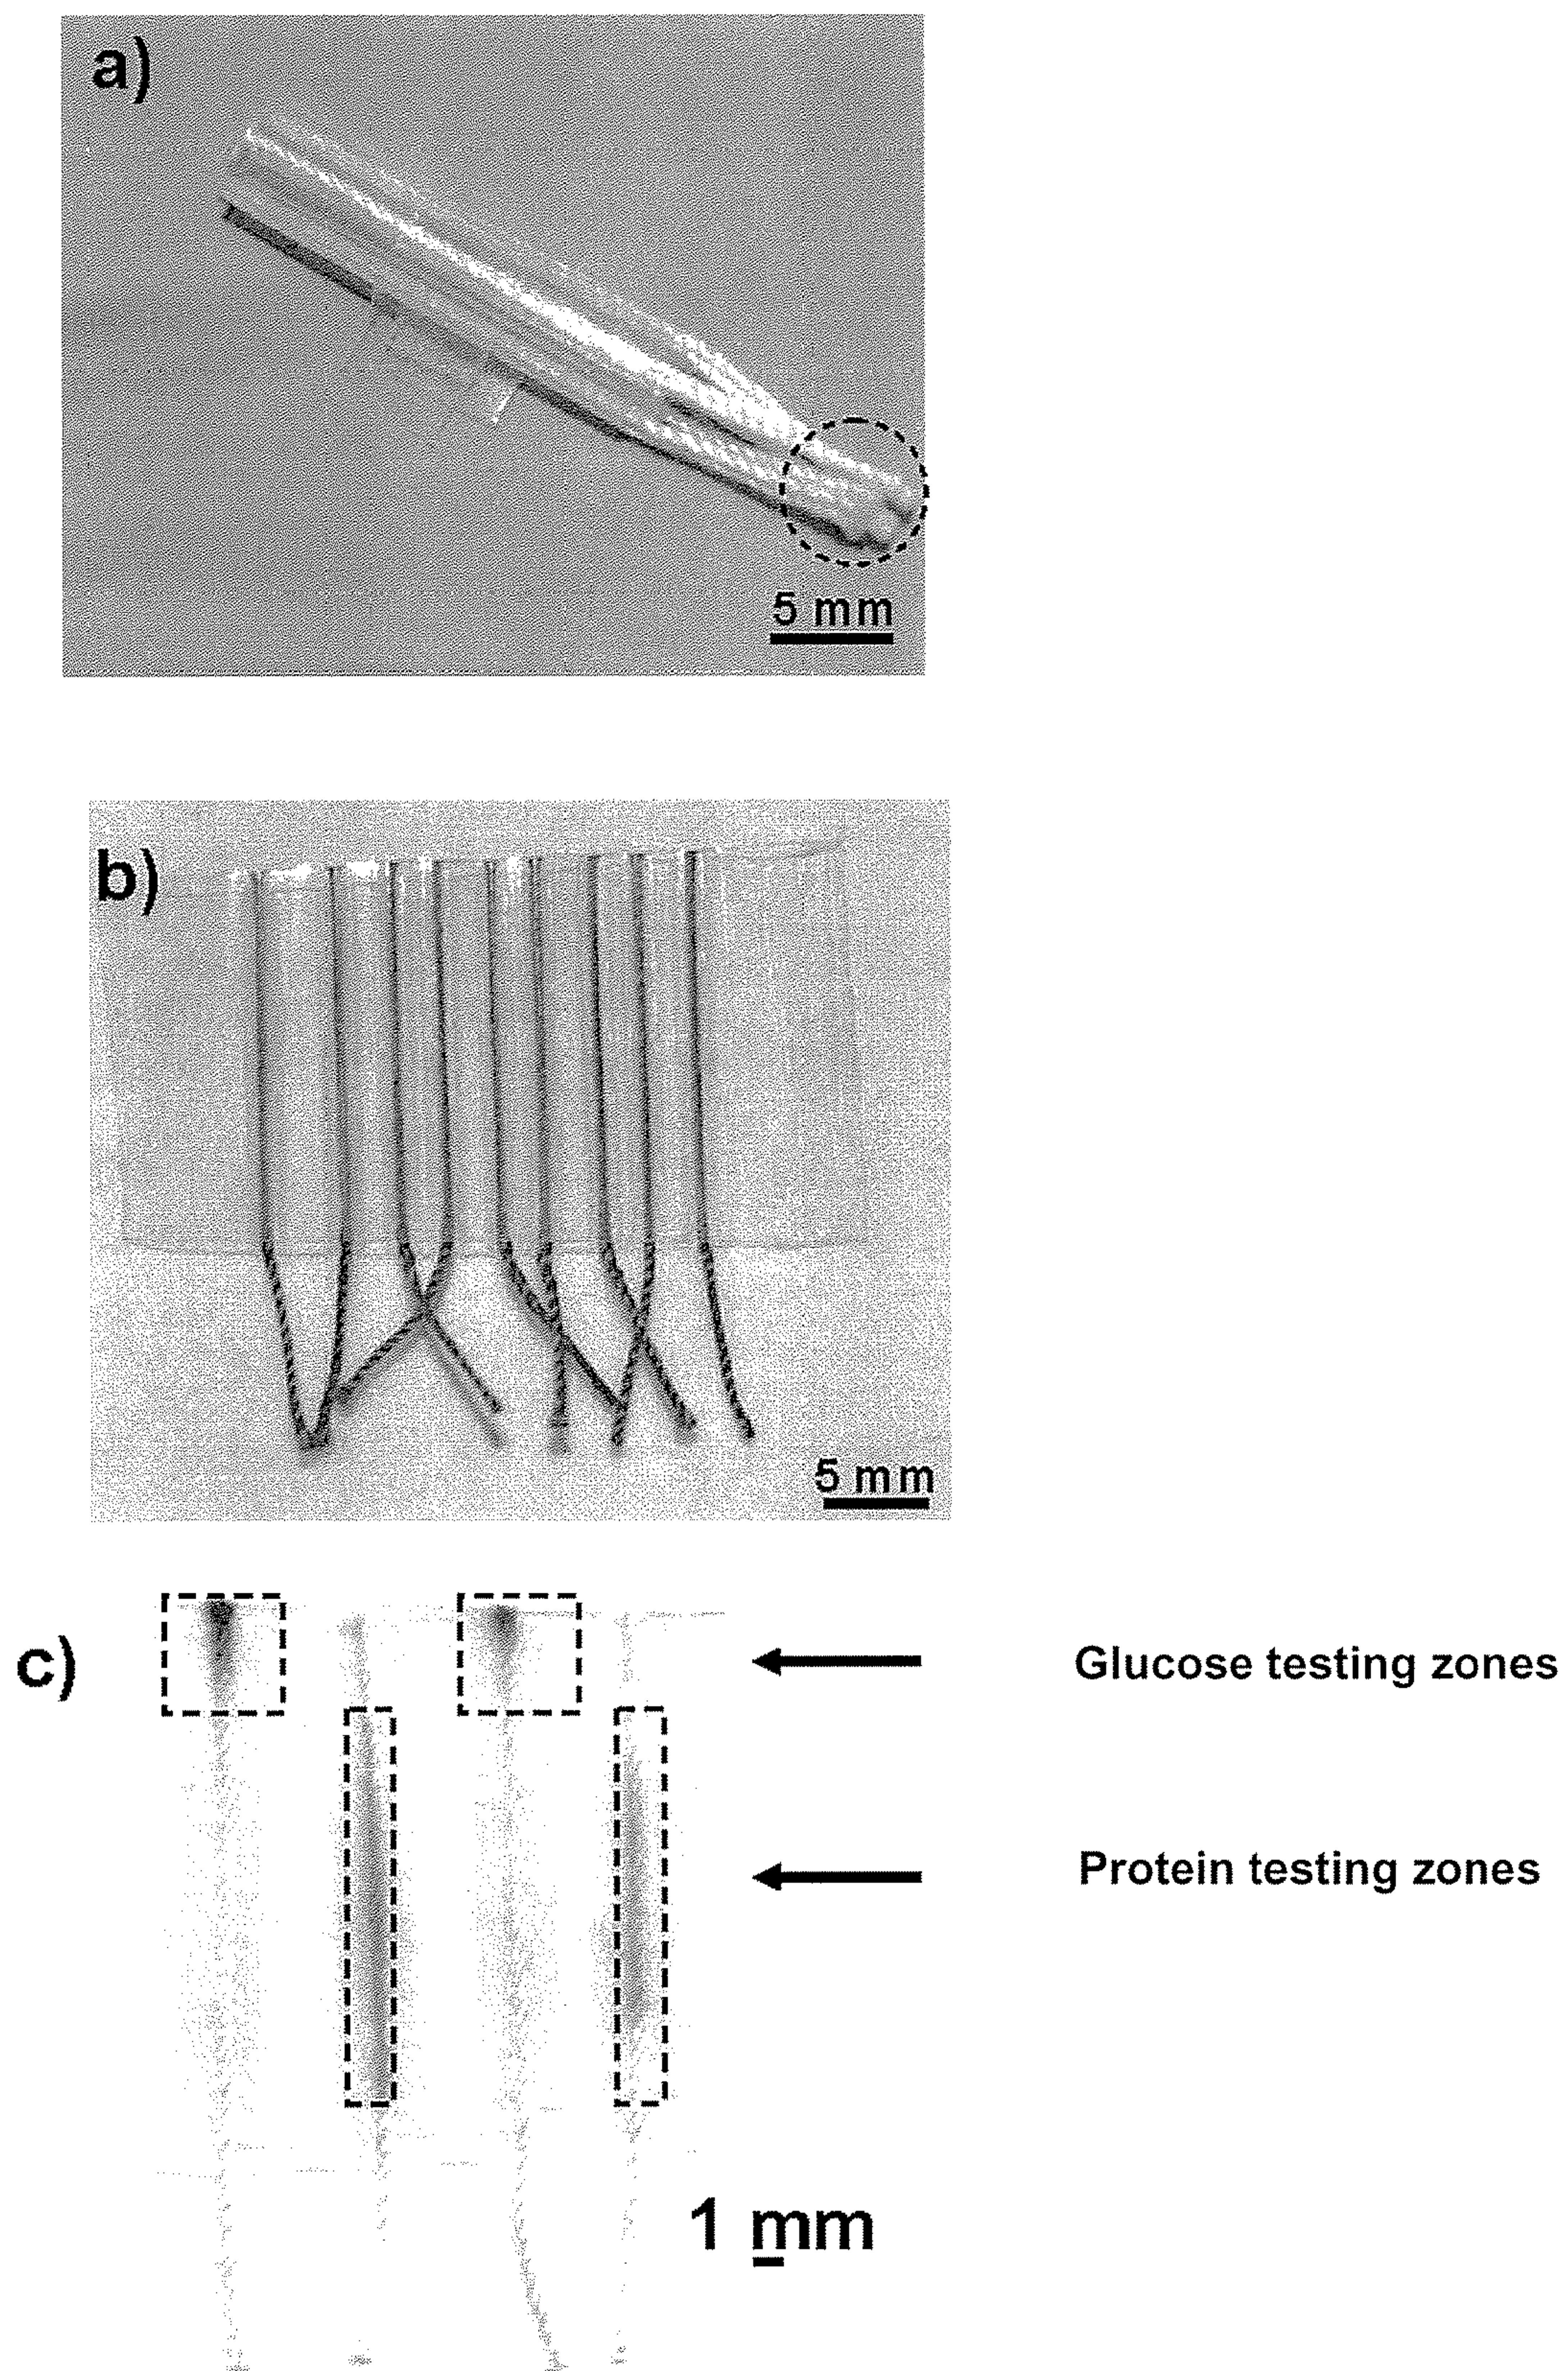


FIG. 6

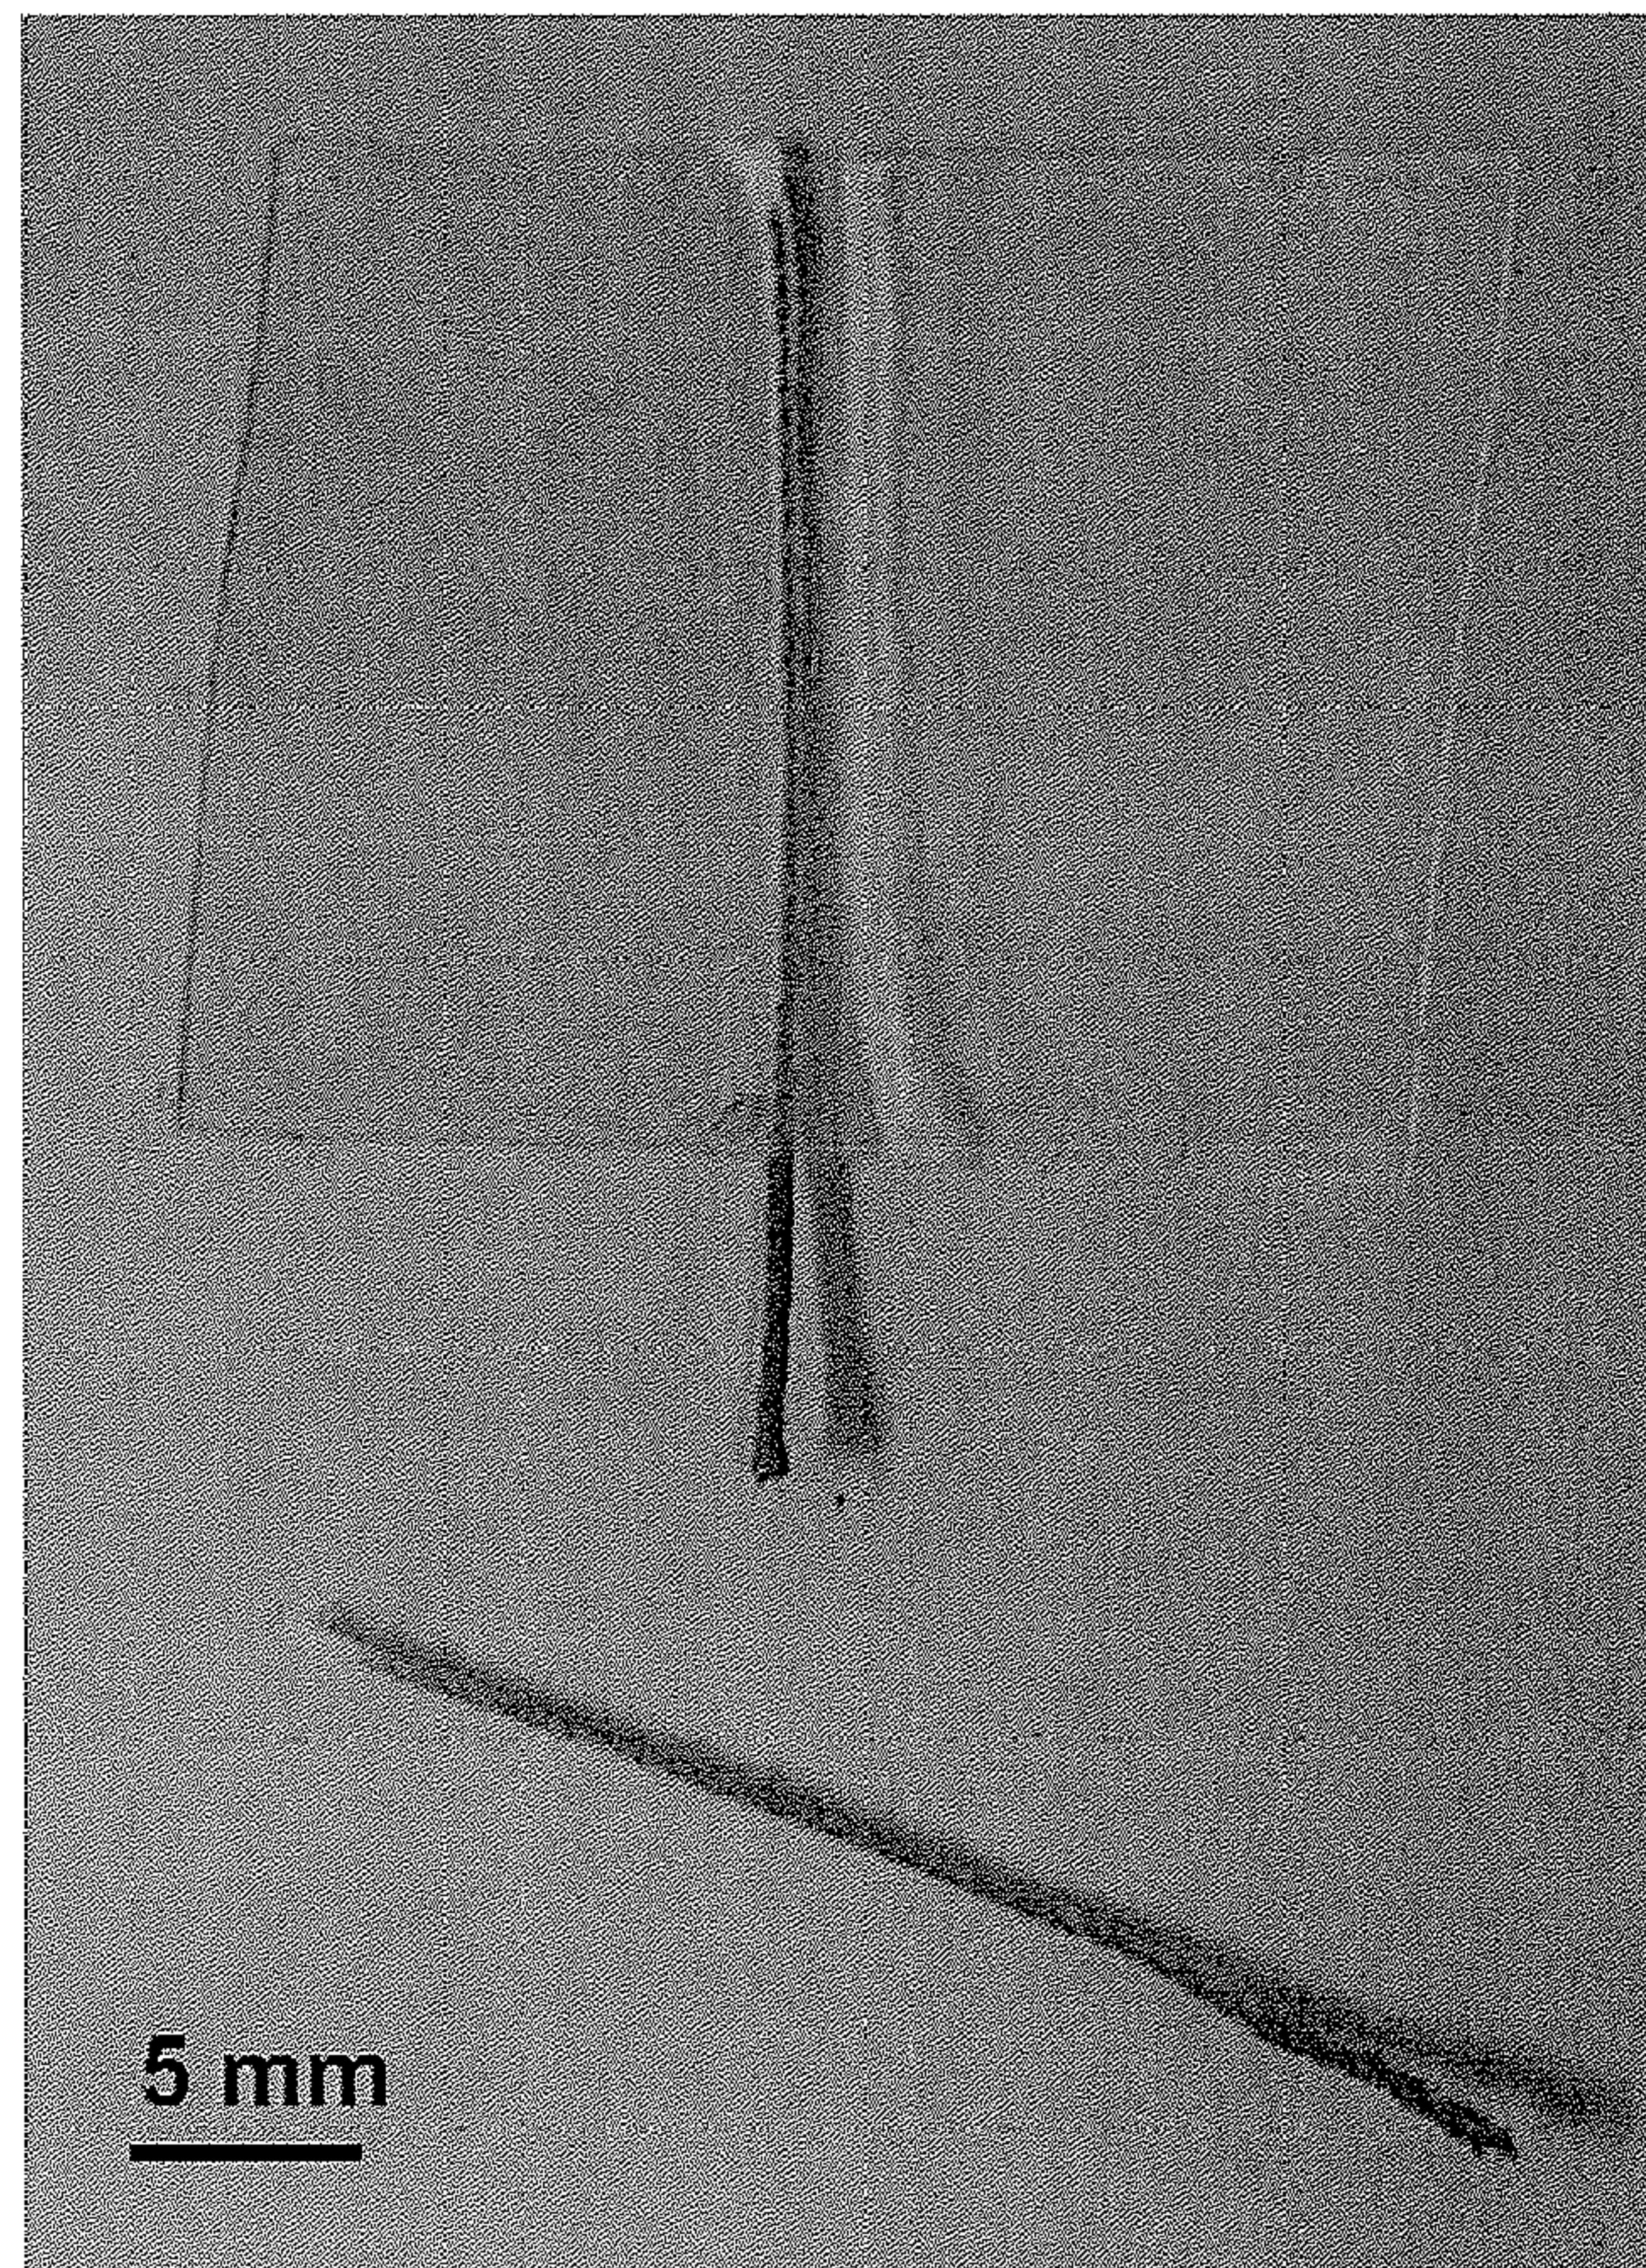


FIG. 7

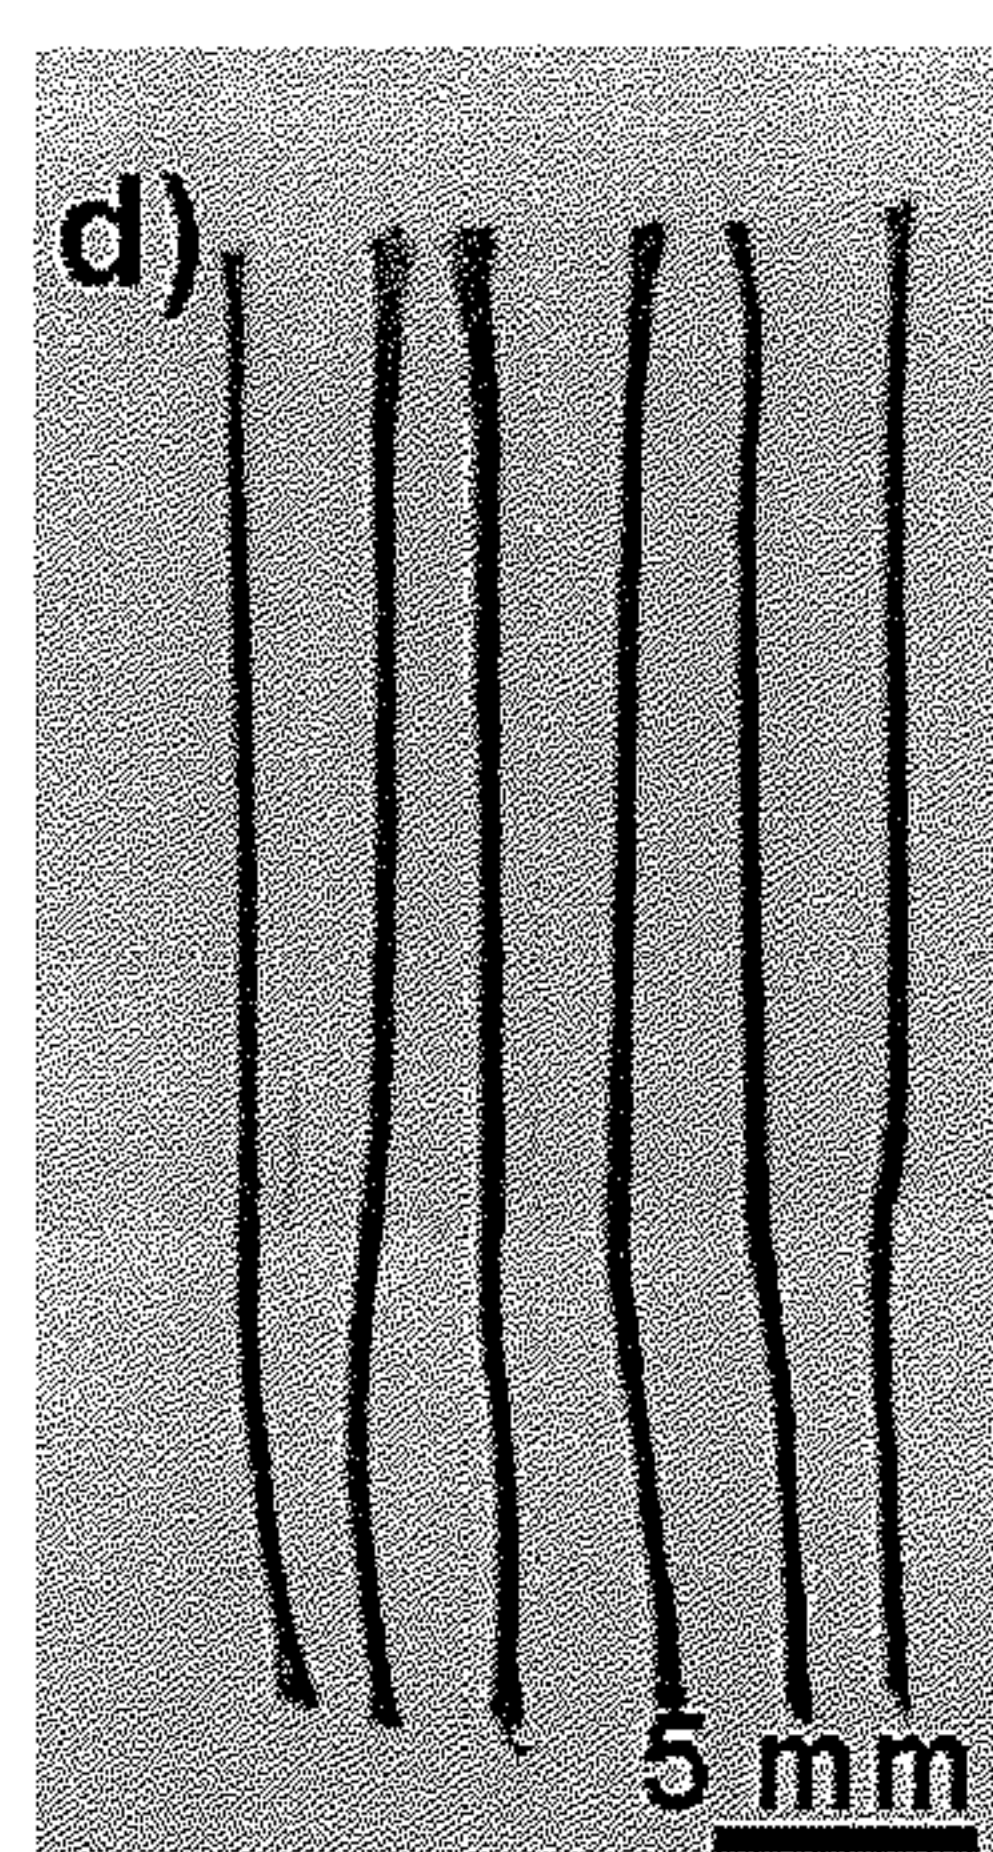
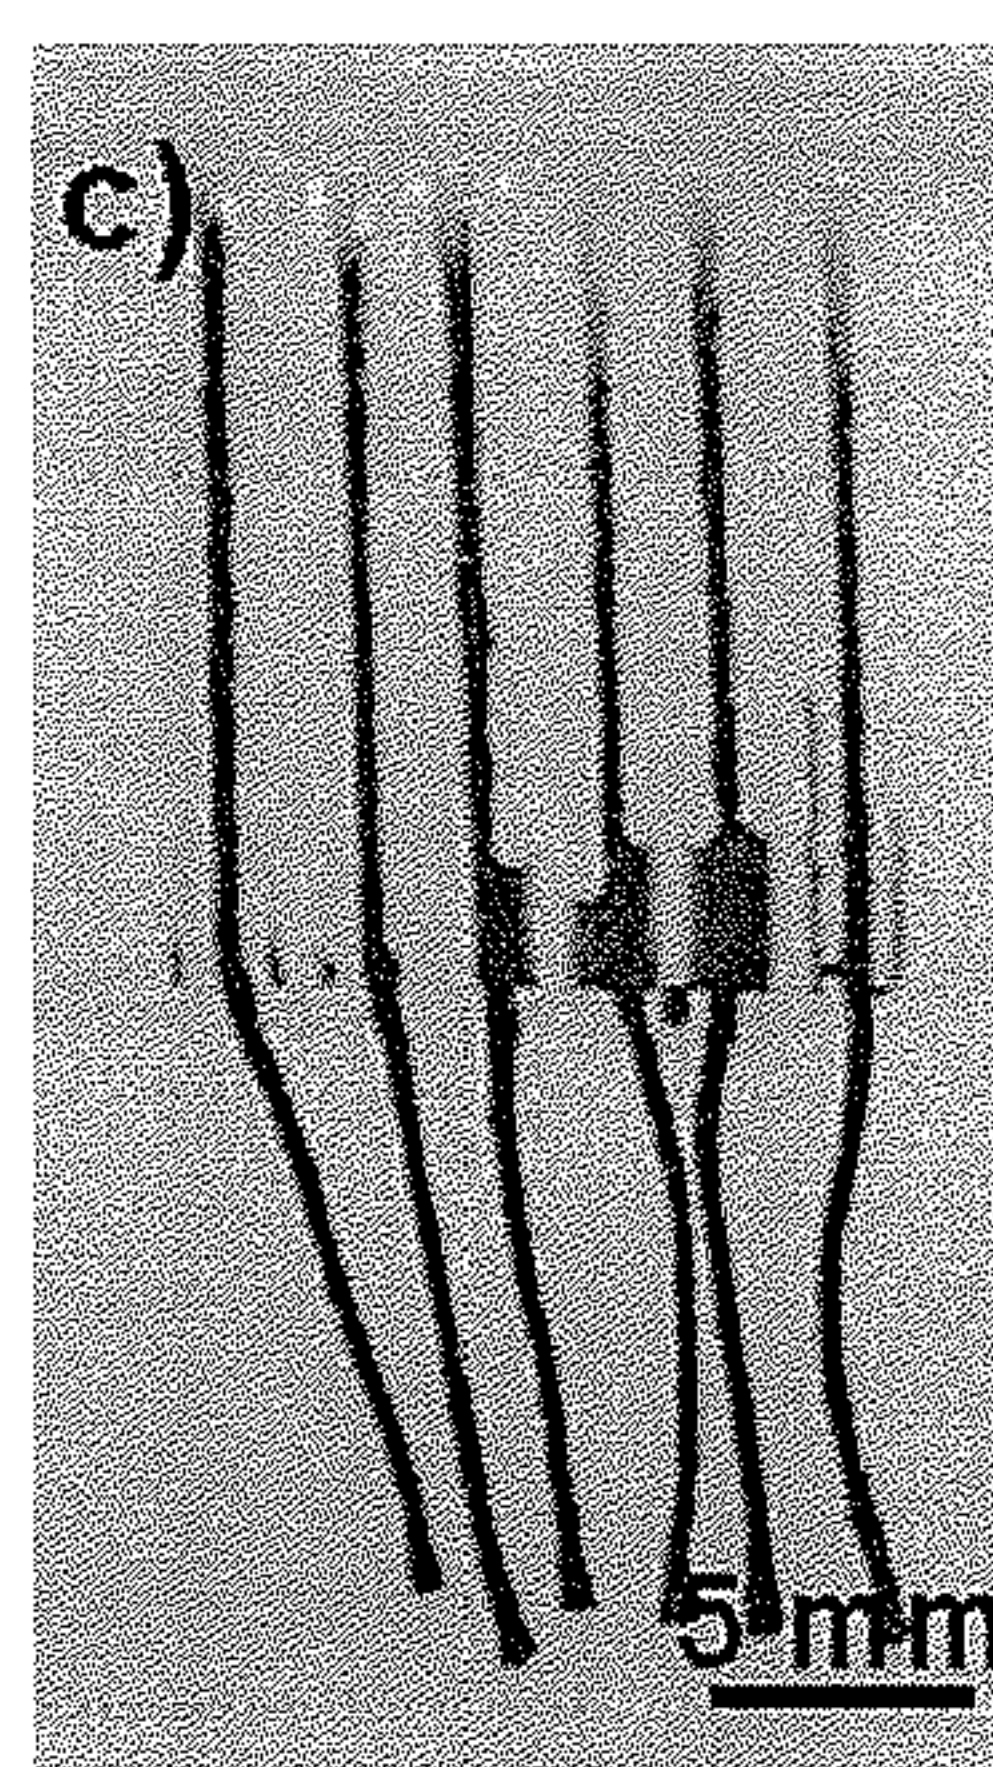
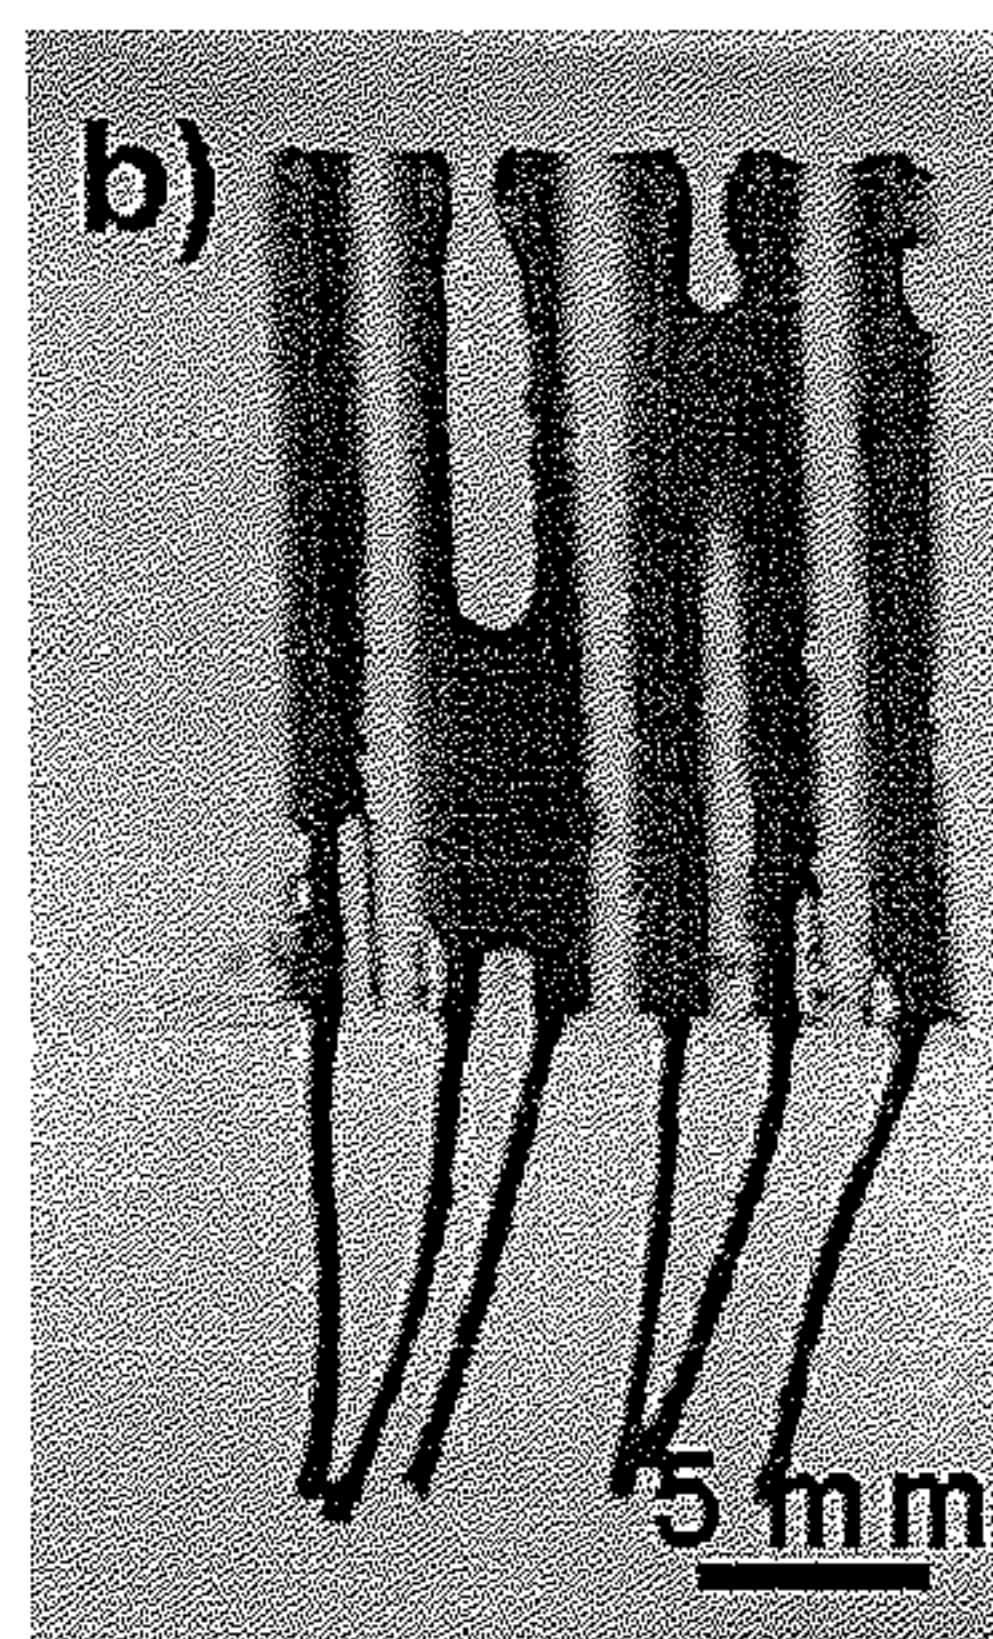
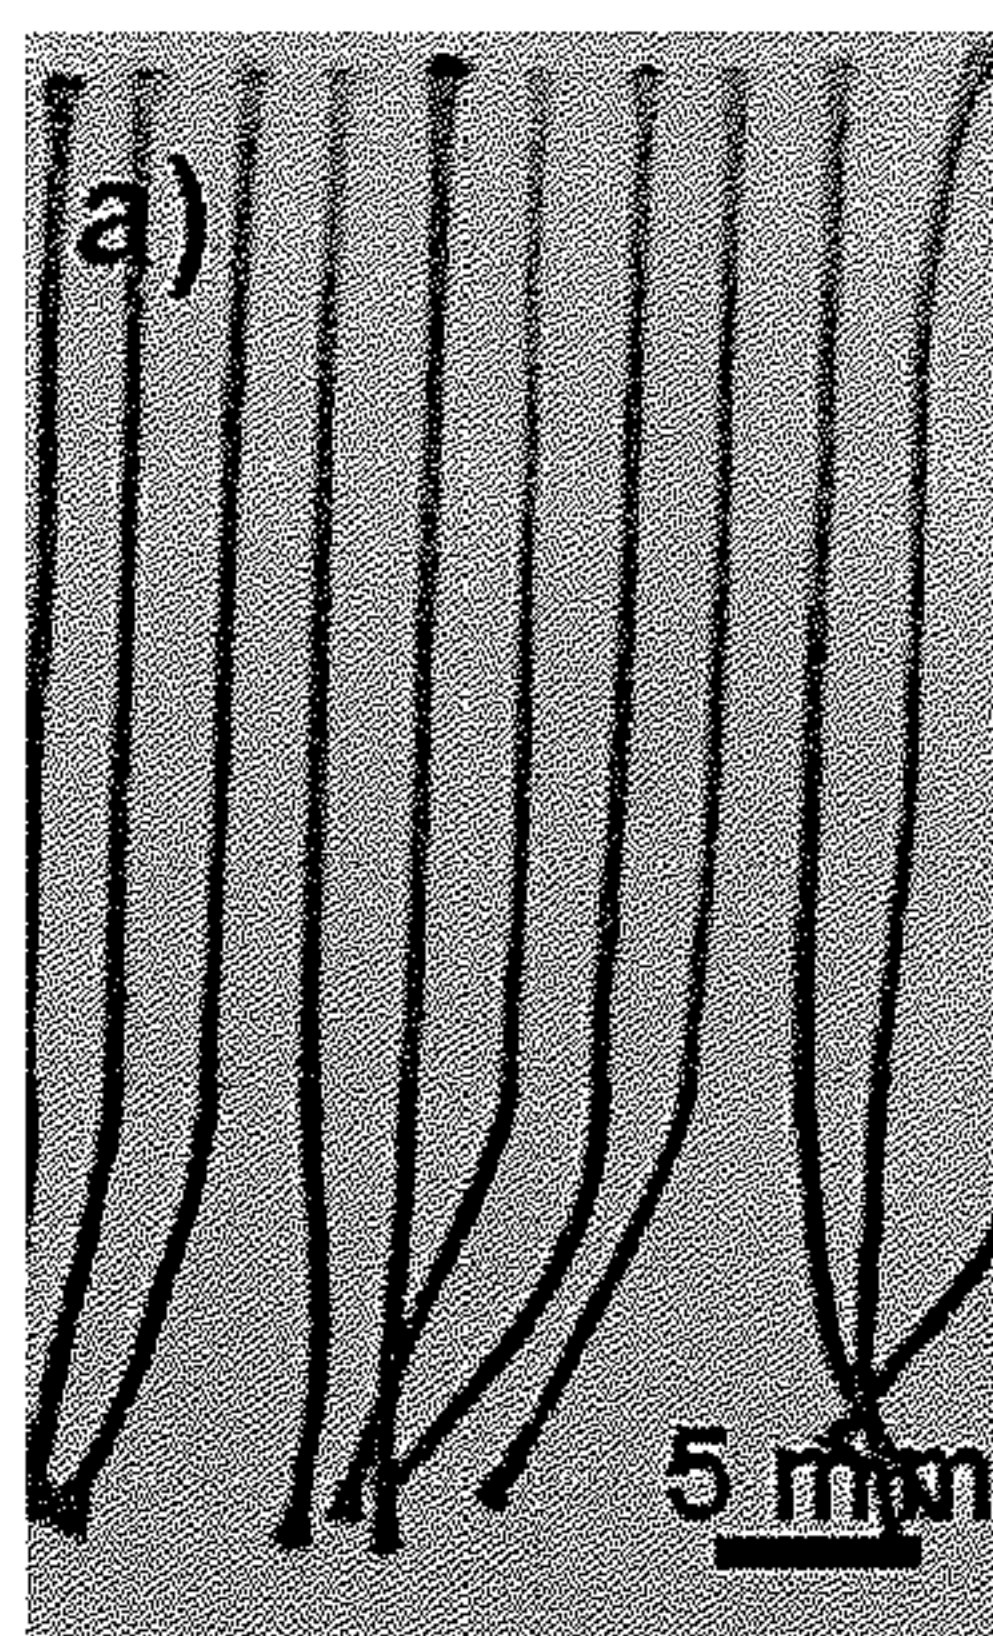


FIG. 8

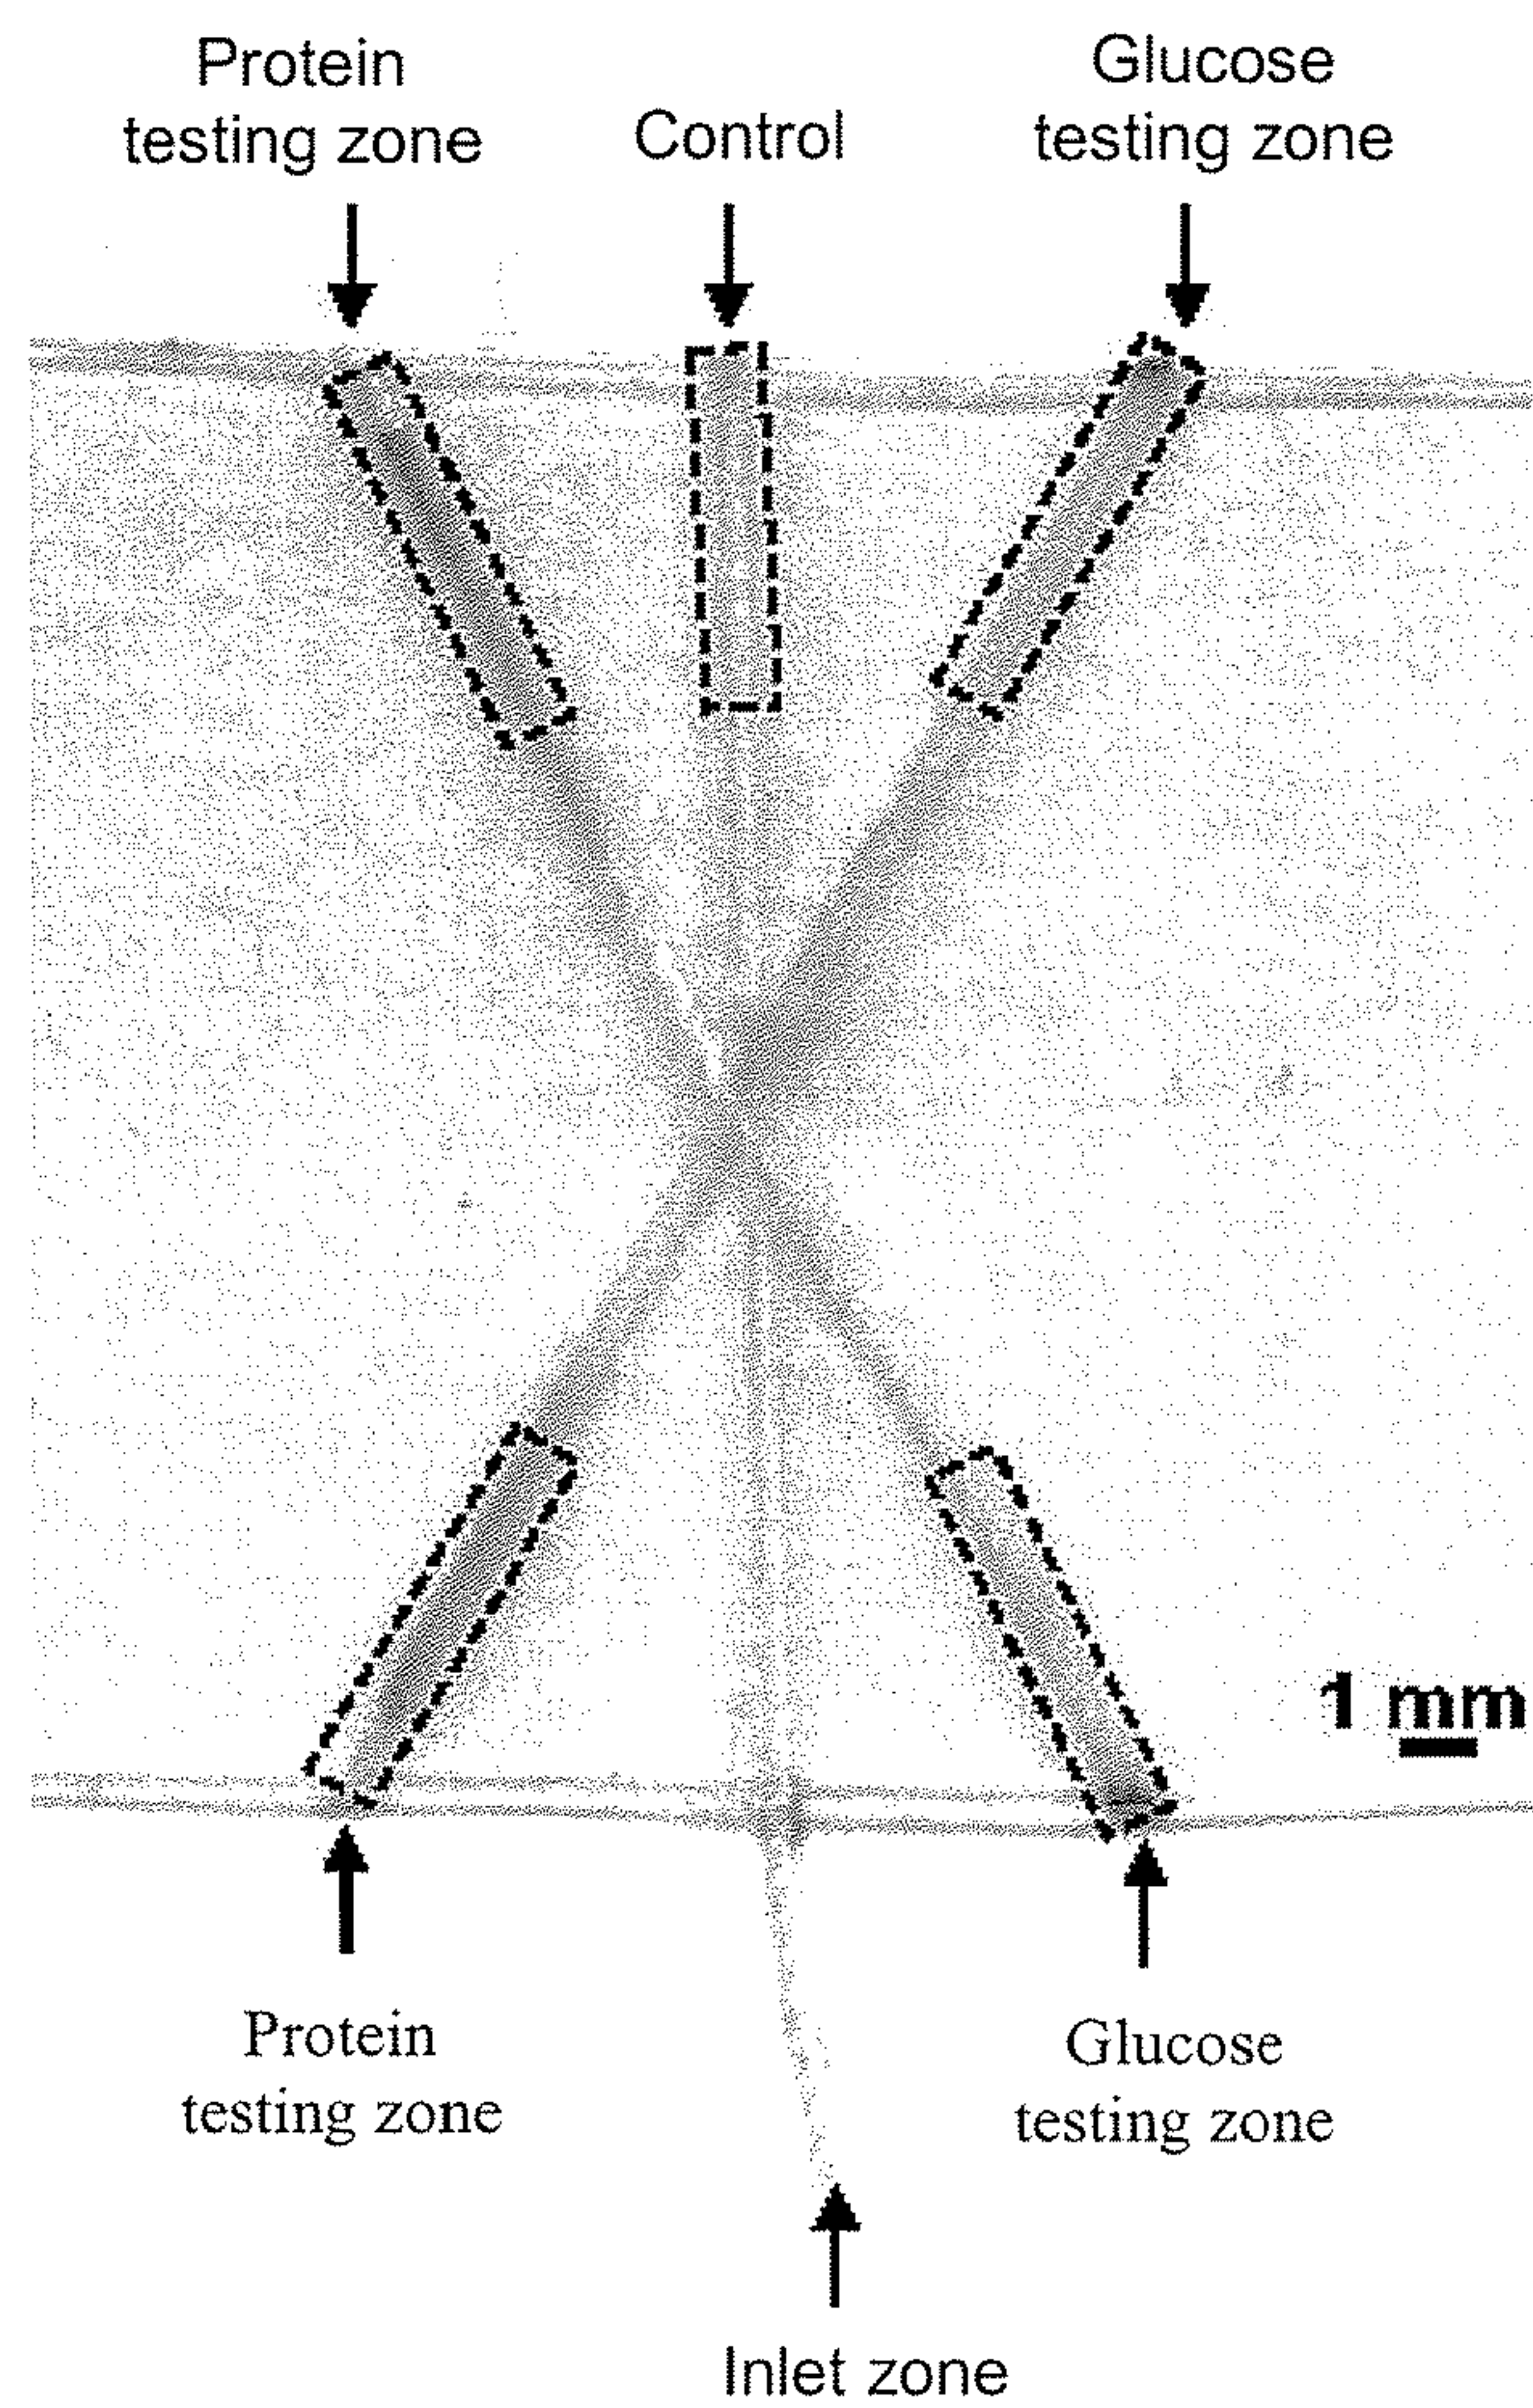


FIG. 9

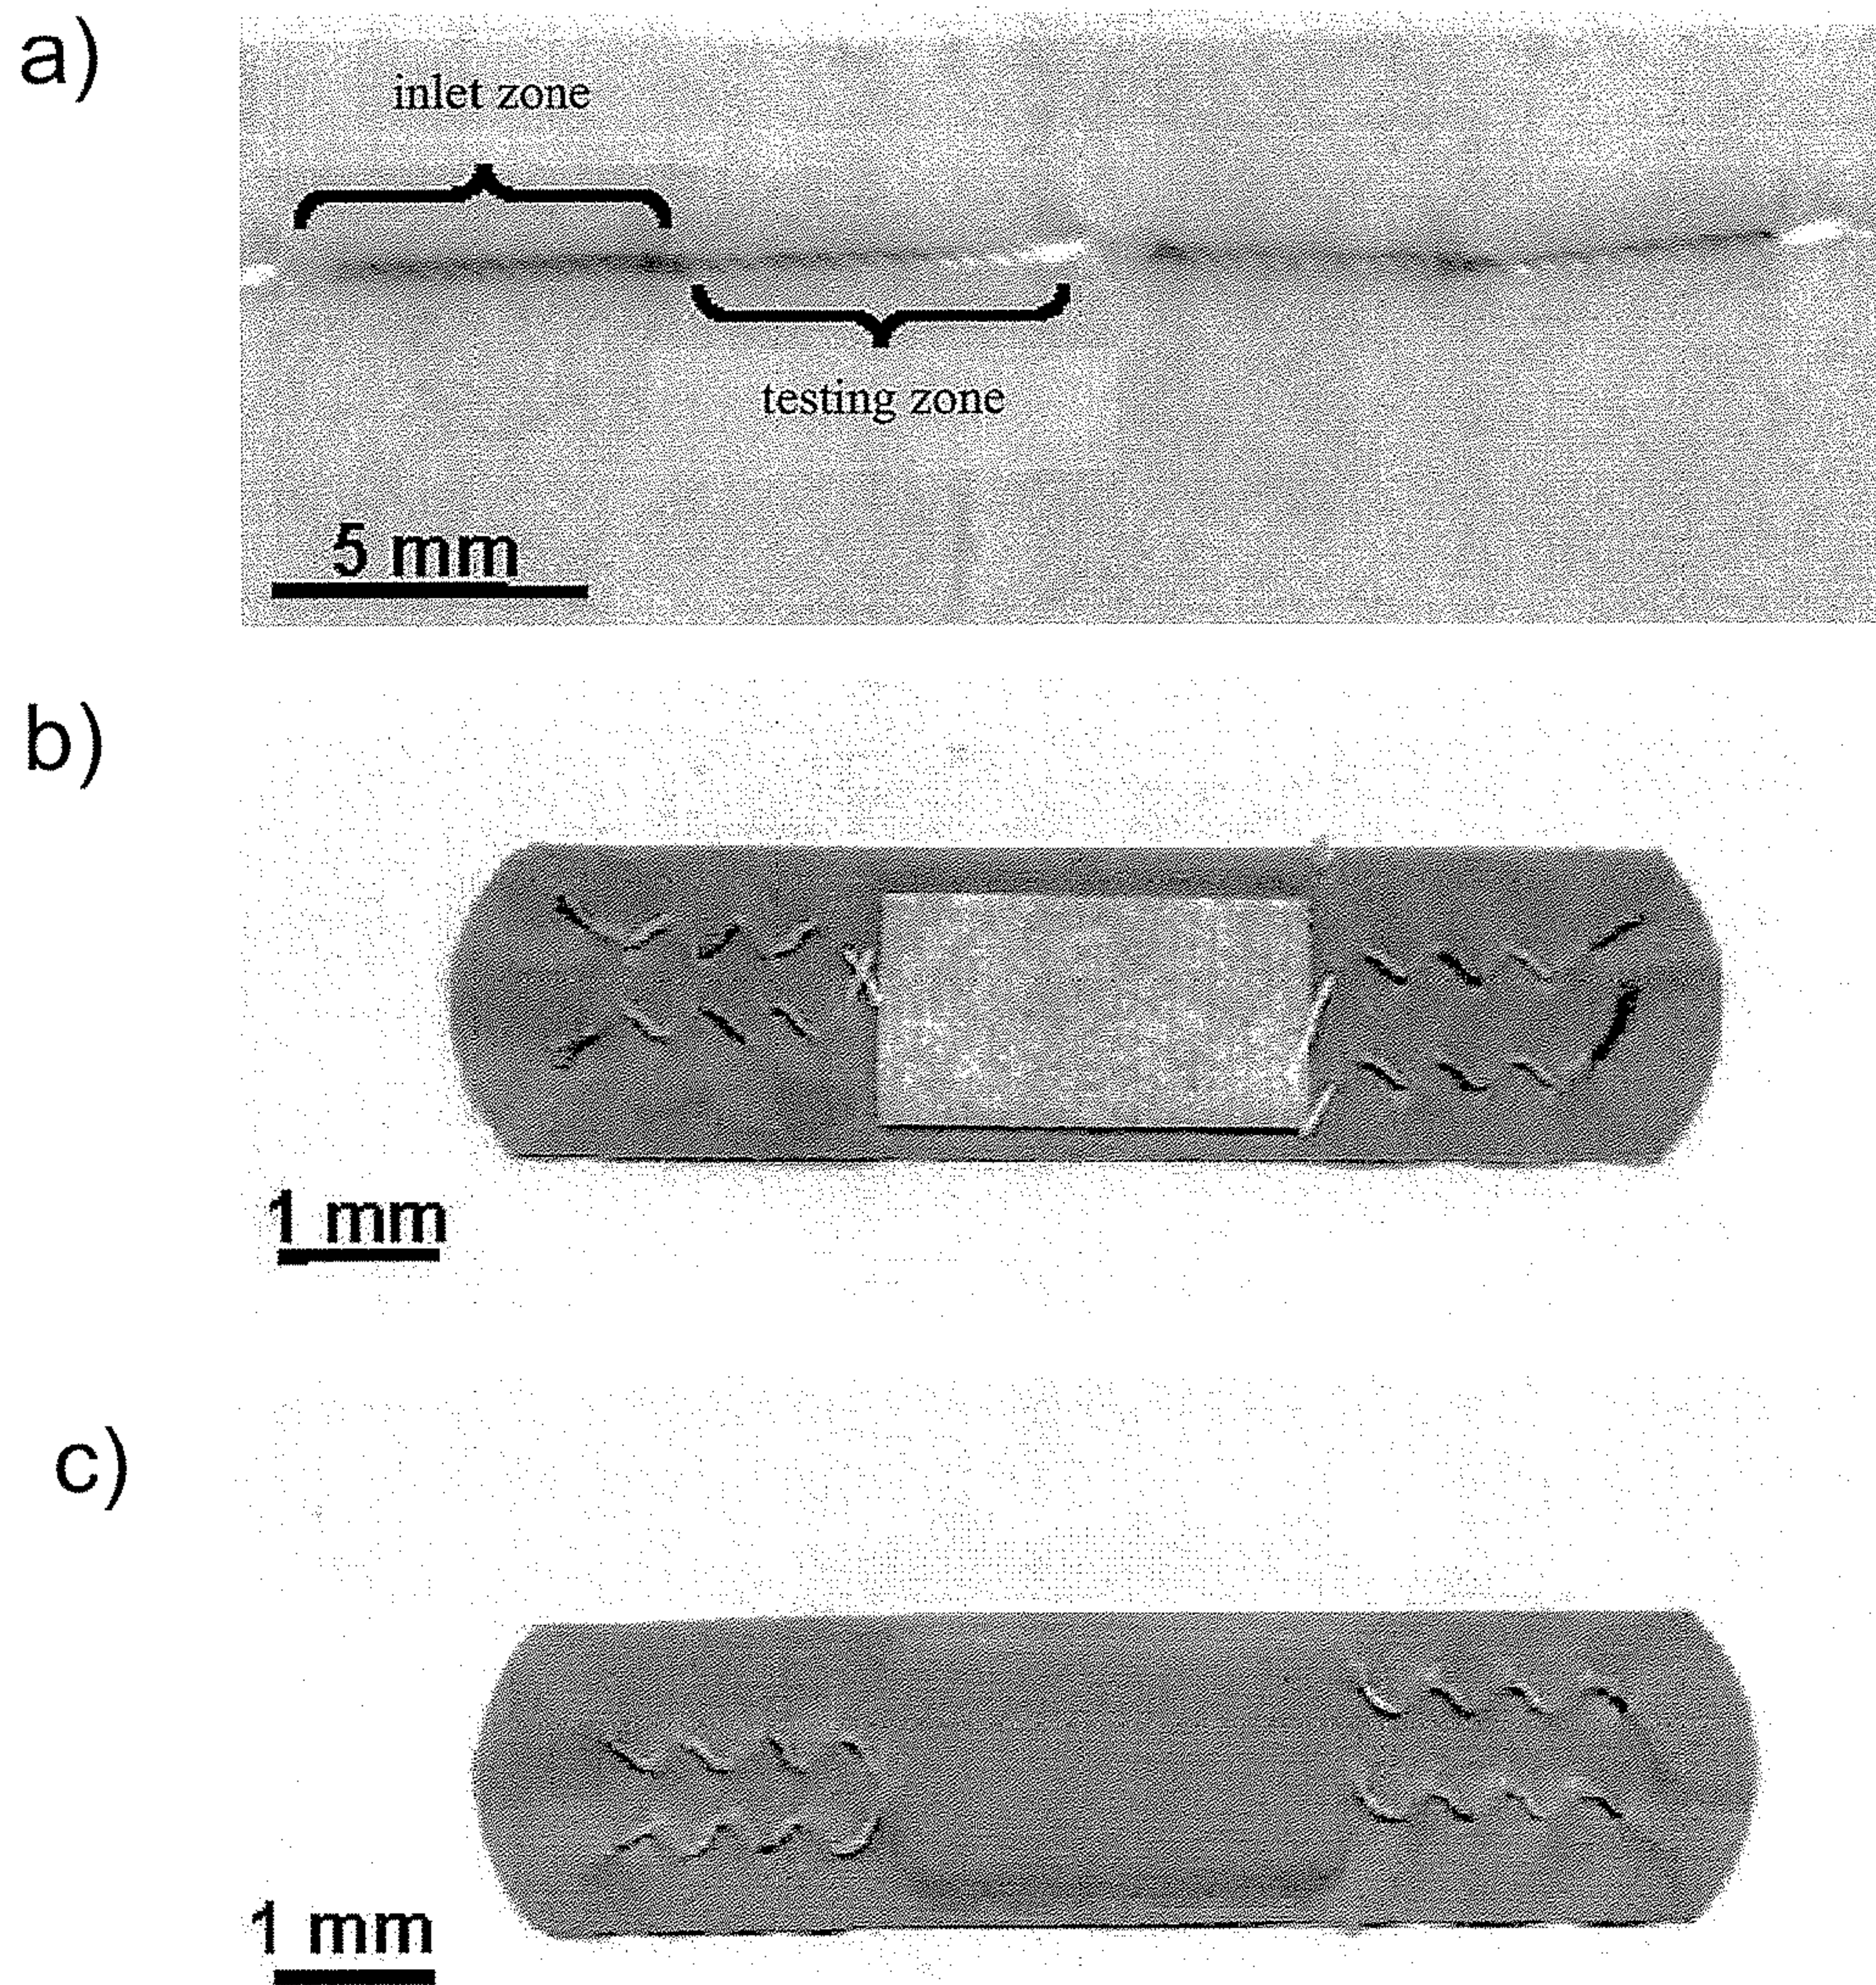


FIG. 10

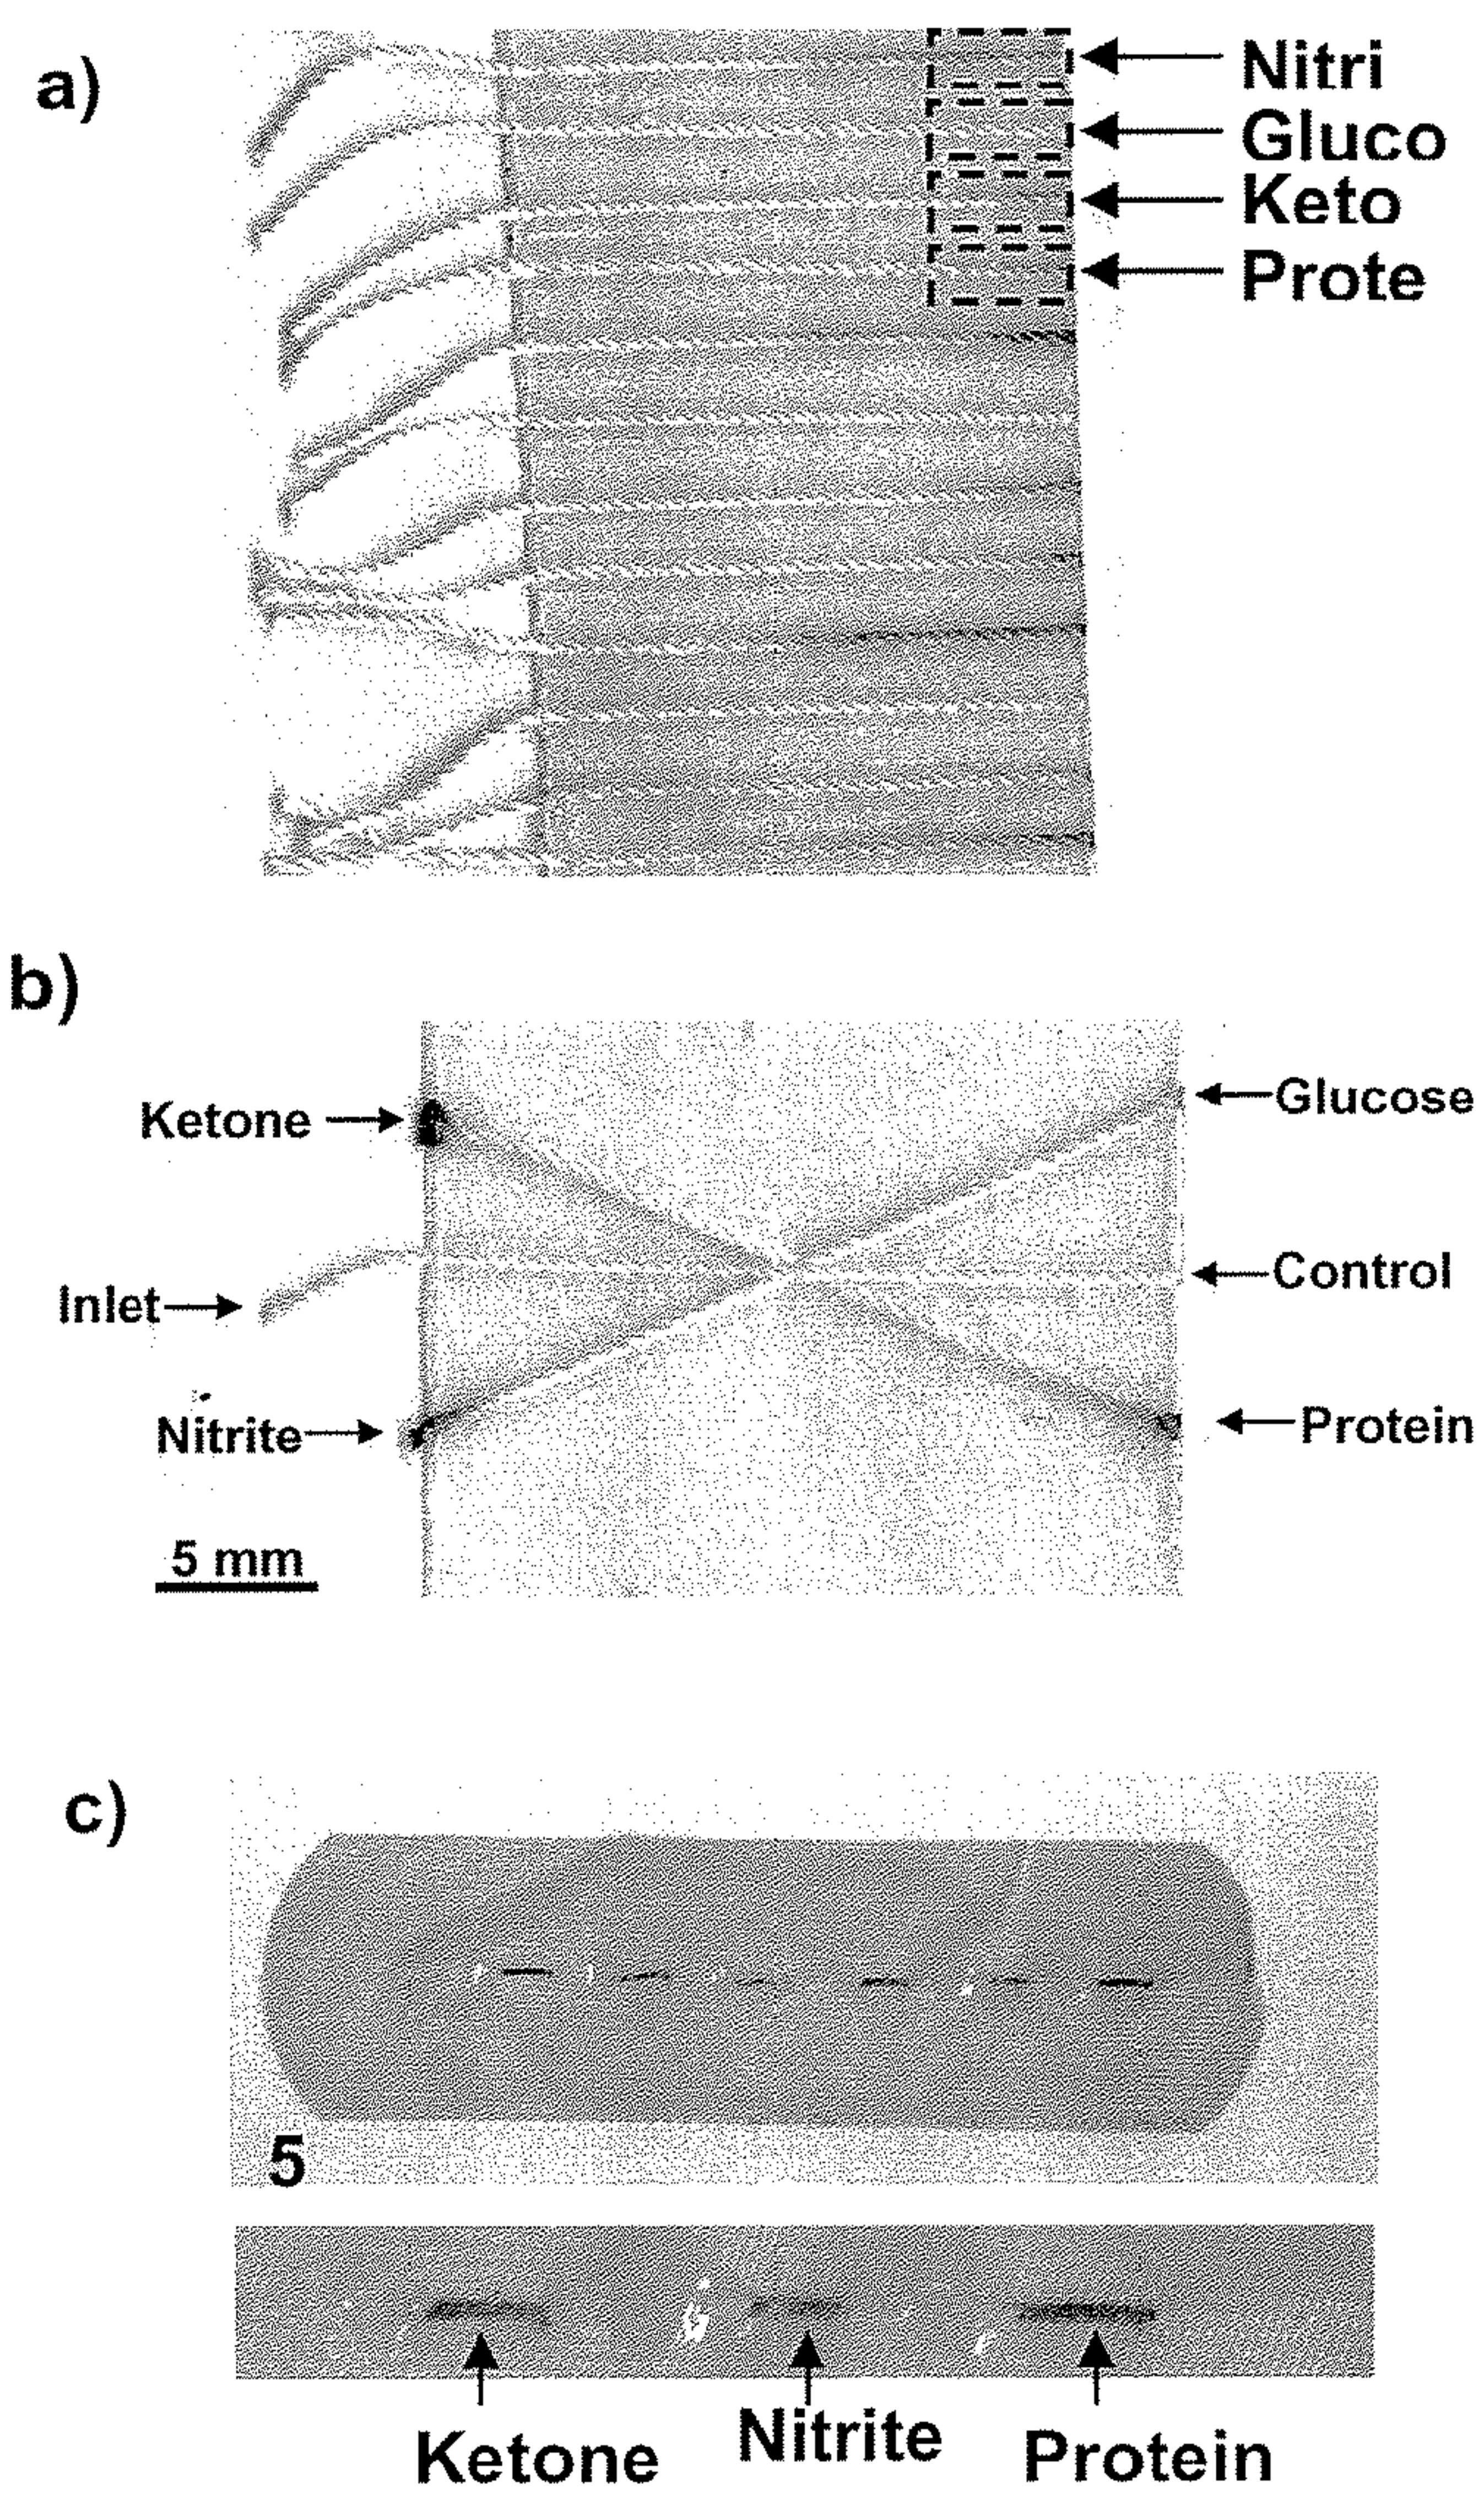


FIG. 11

