



US00D701965S

(12) **United States Design Patent**
Matsumura et al.

(10) **Patent No.:** **US D701,965 S**

(45) **Date of Patent:** **** Apr. 1, 2014**

(54) **ULTRASOUND PROBE**

(71) Applicant: **GE Medical Systems Global Technology Company, LLC**, Waukesha, WI (US)

(72) Inventors: **Kiyoshi Matsumura**, Tokyo (JP); **Koji Yanagihara**, Tokyo (JP)

(73) Assignee: **GE Medical Systems Global Technology Company, LLC**, Waukesha, WI (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/459,728**

(22) Filed: **Jul. 2, 2013**

(30) **Foreign Application Priority Data**

Jan. 4, 2013 (JP) 2013-000007

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/187**

(58) **Field of Classification Search**
USPC D24/107, 141, 158, 164, 165, 167, 170,
D24/186-187, 231; D10/57, 60, 78, 80;
600/407, 461, 459; 378/98.7, 98.8, 189
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

- D316,376 S * 4/1991 Dubut D10/60
- D387,867 S * 12/1997 Henderson et al. D24/187
- D389,918 S * 1/1998 Ninomiya et al. D24/186
- D389,919 S * 1/1998 Ninomiya et al. D24/186
- D390,959 S * 2/1998 Mesaros et al. D24/186
- D392,044 S * 3/1998 Mesaros et al. D24/186
- D545,433 S 6/2007 Messerly et al.
- D547,871 S 7/2007 Watson et al.
- D554,264 S 10/2007 Watson et al.
- D555,252 S * 11/2007 Kitayama et al. D24/186

- D609,352 S * 2/2010 Kitayama D24/186
- D619,266 S * 7/2010 Sakai D24/186
- D622,401 S * 8/2010 Suzuki D24/187
- D634,849 S 3/2011 Kanokogi et al.
- D667,557 S * 9/2012 Boudier D24/186

(Continued)

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(74) *Attorney, Agent, or Firm* — Armstrong Teasdale LLP

(57) **CLAIM**

We claim the ornamental design for an ultrasound probe, as shown and described.

DESCRIPTION

FIG. 1 is a front view of an ultrasound probe showing our new design;

FIG. 2 is a back view of the ultrasound probe design shown in FIG. 1;

FIG. 3 is a left view of the ultrasound probe design shown in FIG. 1;

FIG. 4 is a right view of the ultrasound probe design shown in FIG. 1;

FIG. 5 is a top view of the ultrasound probe design shown in FIG. 1;

FIG. 6 is a bottom view of the ultrasound probe design shown in FIG. 1;

FIG. 7 is a front perspective view of the ultrasound probe design shown in FIG. 1;


FIG. 8 is a back perspective view of the ultrasound probe design shown in FIG. 1;

FIG. 9 is a front perspective view of the ultrasound probe design shown in FIG. 1; and,

FIG. 10 is a front perspective view of the ultrasound probe design shown in FIG. 1.

In these drawings, the solid lines illustrate the claimed ornamental design, whereas the broken lines illustrate unclaimed environmental features and form no part of the claimed design.

1 Claim, 10 Drawing Sheets

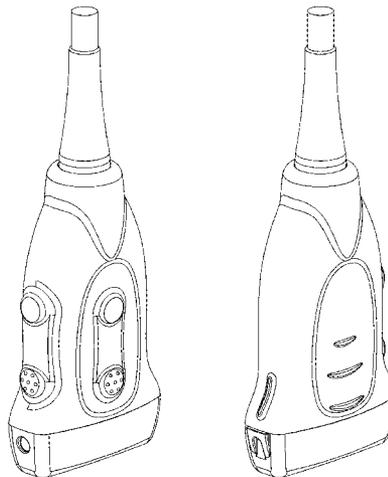

(56)

References Cited

U.S. PATENT DOCUMENTS

D671,644 S	11/2012	Dodd et al.	
D678,500 S	3/2013	Osepaishvili	
D679,021 S *	3/2013	Tani et al.	D24/187
D681,820 S *	5/2013	Shinohara et al.	D24/186
D681,823 S *	5/2013	Shinohara et al.	D24/186
D681,824 S *	5/2013	Shinohara et al.	D24/186
D681,825 S *	5/2013	Shinohara et al.	D24/186
D681,827 S *	5/2013	Shinohara et al.	D24/186
D681,828 S *	5/2013	Shinohara et al.	D24/186
D682,433 S *	5/2013	Shinohara et al.	D24/186
D685,100 S *	6/2013	Shinohara et al.	D24/186
D688,376 S *	8/2013	Bartlett	D24/187
2013/0085391 A1	4/2013	Matsumura et al.	

* cited by examiner

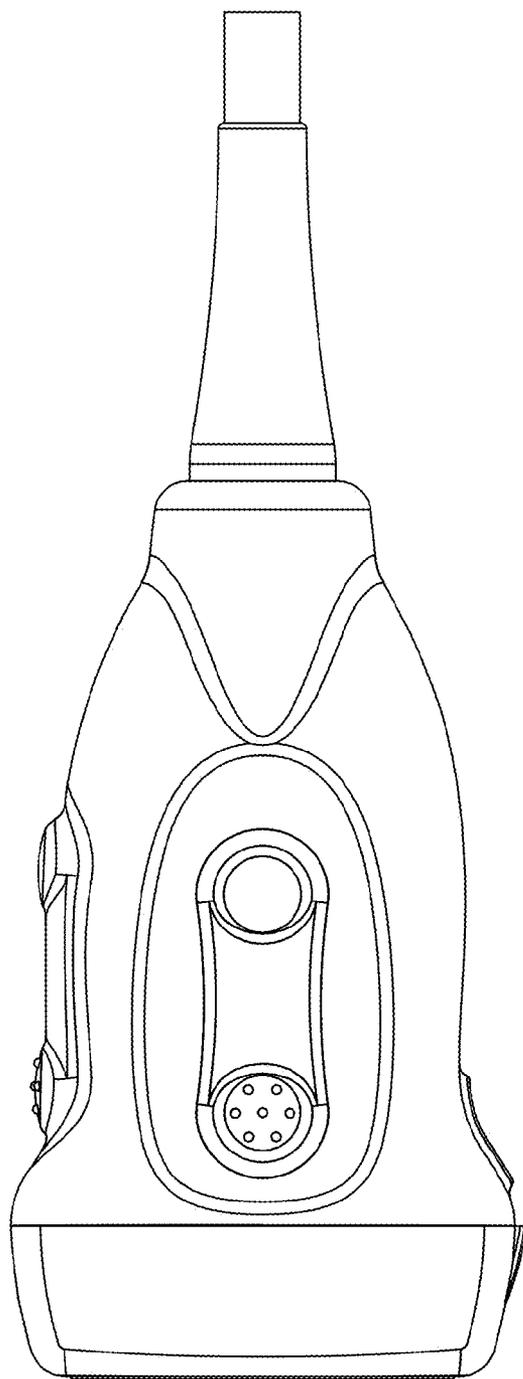


FIG. 1

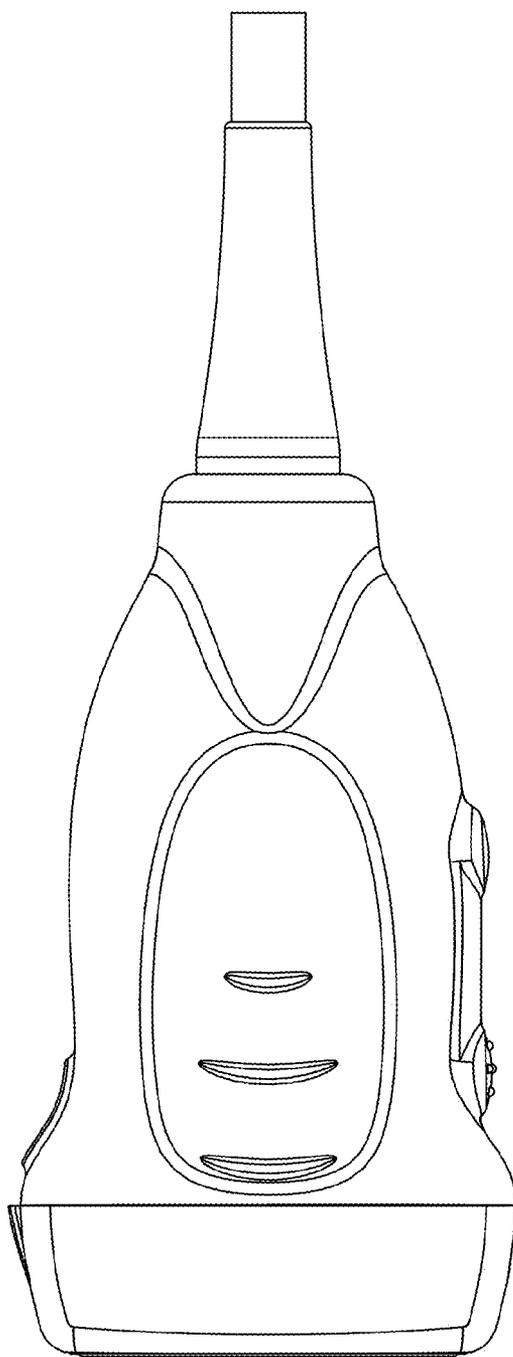


FIG. 2

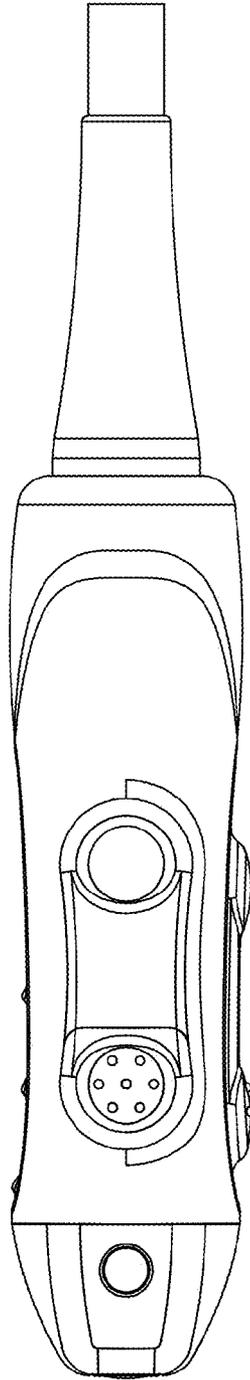


FIG. 3

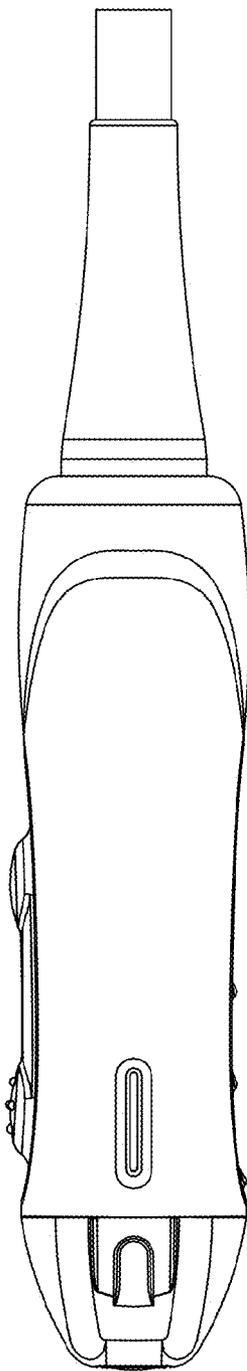


FIG. 4

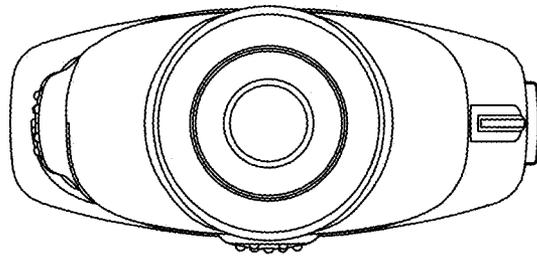


FIG. 5

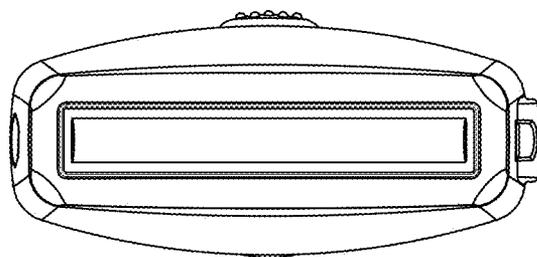


FIG. 6

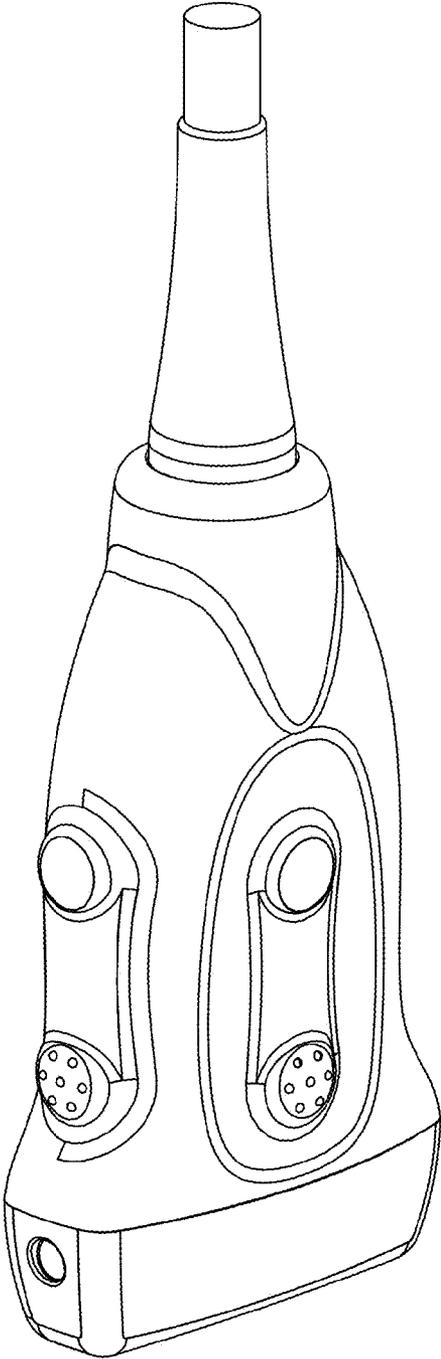


FIG. 7

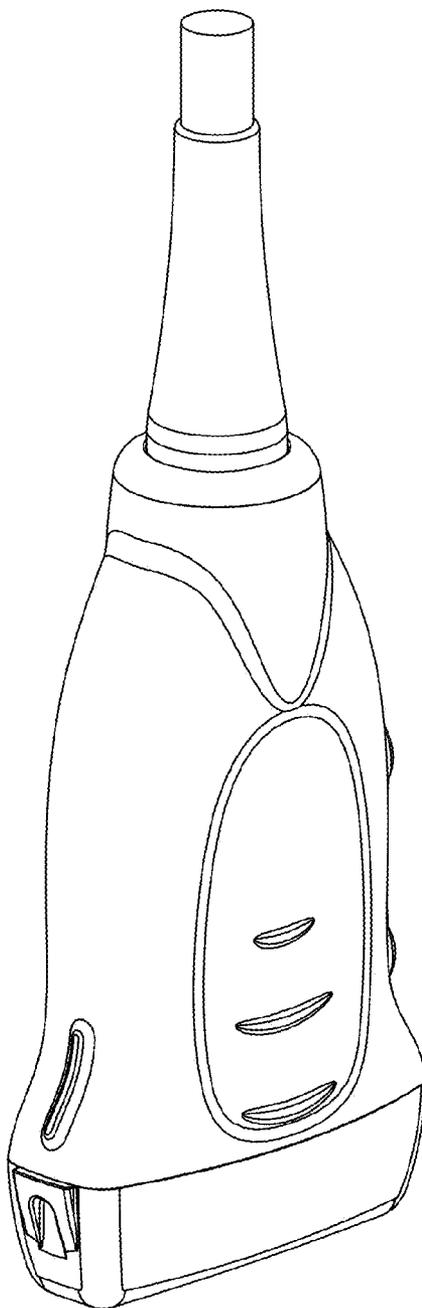


FIG. 8

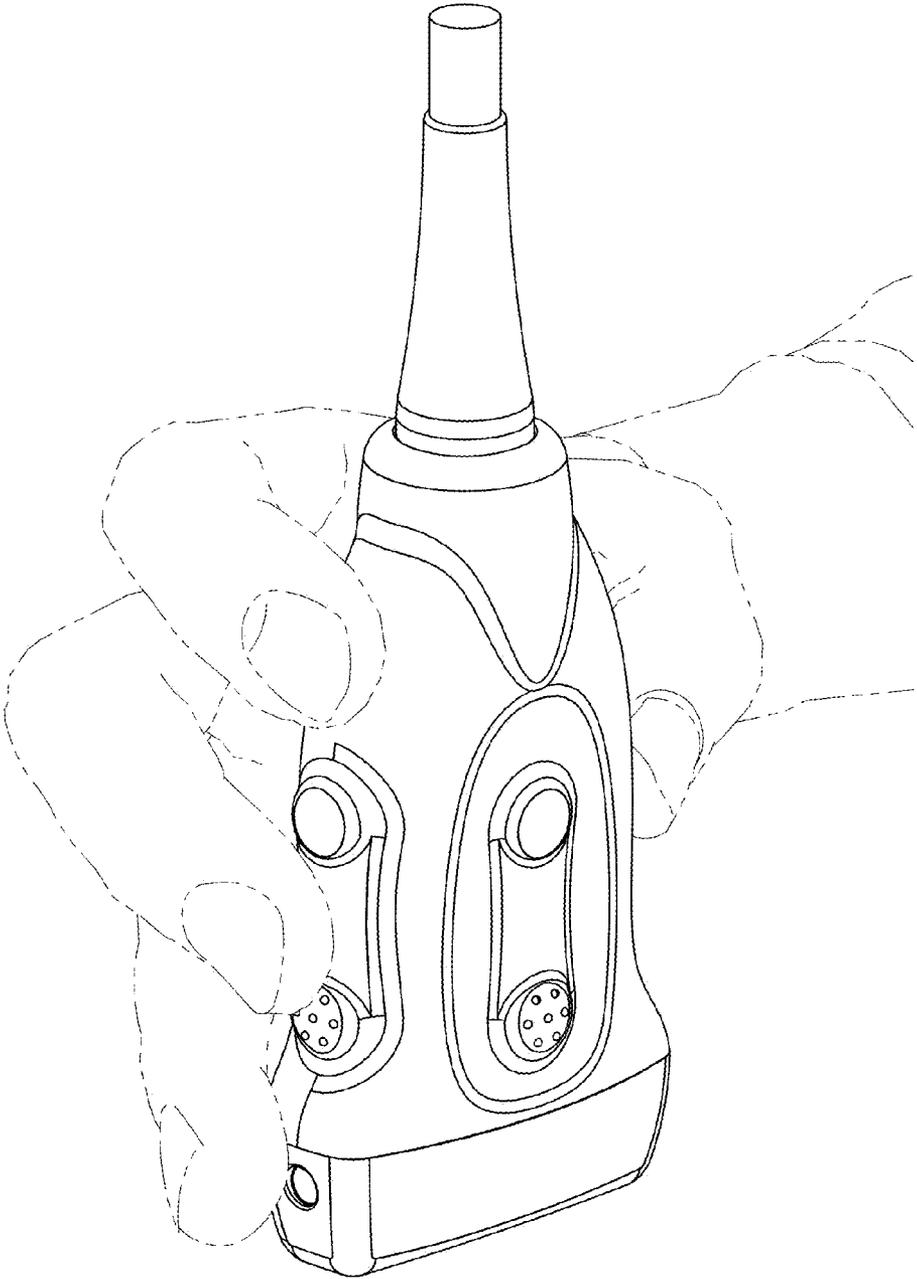


FIG. 9

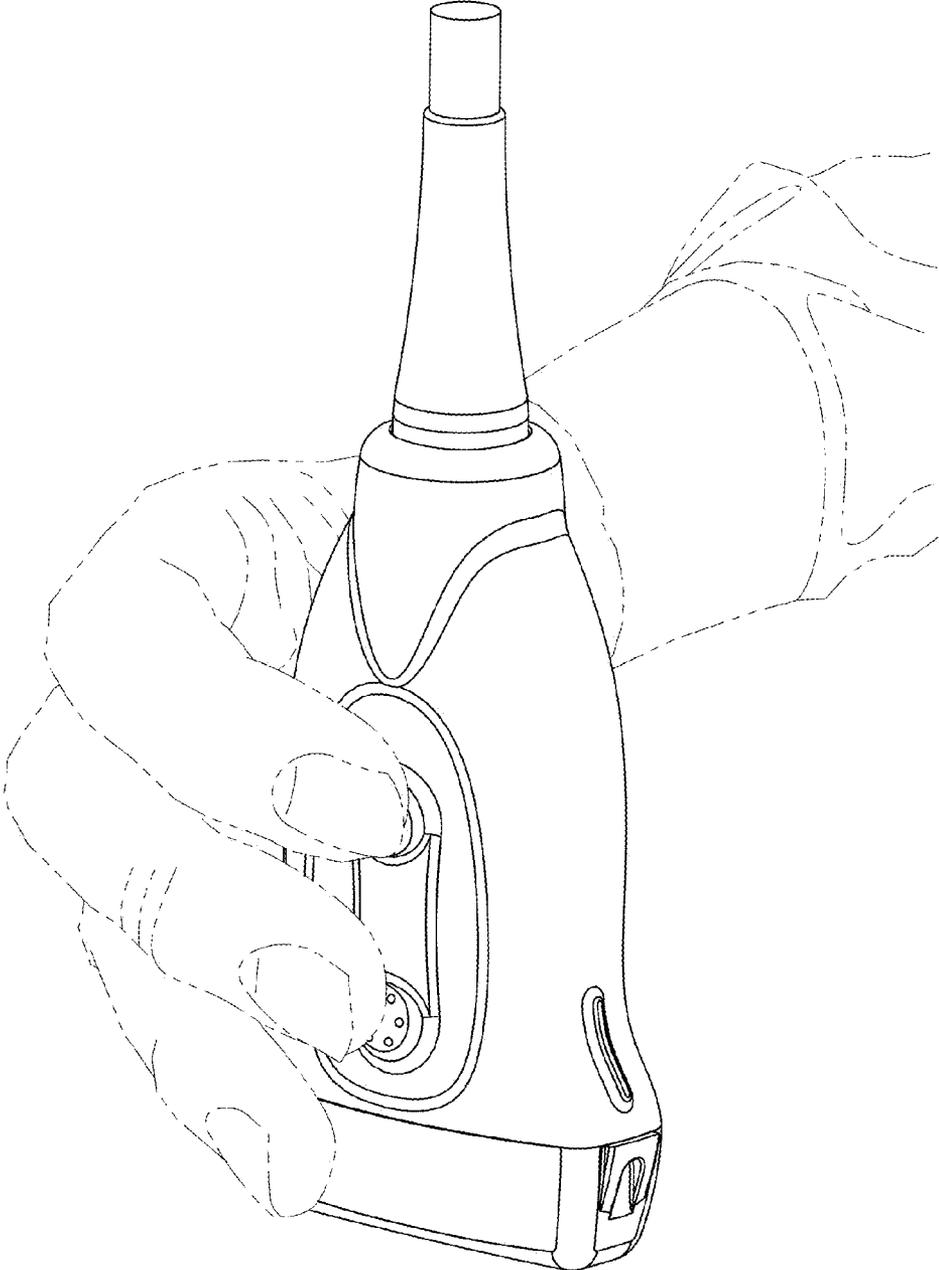


FIG. 10