

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
23 November 2006 (23.11.2006)

PCT

(10) International Publication Number
WO 2006/124896 A2

- (51) International Patent Classification:
A61B 17/32 (2006.01)
- (21) International Application Number:
PCT/US2006/018915
- (22) International Filing Date: 12 May 2006 (12.05.2006)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
60/680,388 12 May 2005 (12.05.2005) US
- (71) Applicant and
(72) Inventor: **MODESITT, D. Bruce** [US/US]; 120 Wingate Avenue, San Carlos, CA 94070 (US).
- (74) Agent: **LEVINE, David, A.**; Levine Bagade LLP, 2483 East Bayshore Road, Suite 100, Palo Alto, CA 94050 (US).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM,

AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, LY, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NG, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, LV, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *without international search report and to be republished upon receipt of that report*

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.



WO 2006/124896 A2

(54) Title: ACCESS AND CLOSURE DEVICE AND METHOD

(57) Abstract: Devices and methods for accessing and closing vascular sites are disclosed. Self-sealing closure devices and methods are disclosed. A device that can make both steeply sloping and flat access paths into a vascular lumen is disclosed. The device can also form arteriotomies with sections cleaved between a vessel's intima and adventitia. Methods for using the device are also disclosed.

ACCESS AND CLOSURE DEVICE AND METHOD

D. Bruce Modesitt

CROSS-REFERENCE TO RELATED APPLICATION

[0001] This application claims the benefit under 35 U.S.C. §119(e) of U.S. Provisional Application 60/680,388 filed May 12, 2005, the content of which is incorporated herein by reference in its entirety.

BACKGROUND OF THE INVENTION

1. Field of the Invention

[0002] The present invention relates to the field of accessing a biological lumen and closing the access port thereby created.

2. Description of the Related Art

[0003] A number of diagnostic and interventional vascular procedures are now performed transluminally, where a catheter is introduced to the vascular system at a convenient access location - such as the femoral, brachial, or subclavian arteries - and guided through the vascular system to a target location to perform therapy or diagnosis. When vascular access is no longer required, the catheter and other vascular access devices must be removed from the vascular entrance and bleeding at the puncture site must be stopped.

[0004] One common approach for providing hemostasis is to apply external force near and upstream from the puncture site, typically by manual compression. This method is time-consuming, frequently requiring one-half hour or more of

1 compression before hemostasis. This procedure is uncomfortable for the patient and
2 frequently requires administering analgesics. Excessive pressure can also present the
3 risk of total occlusion of the blood vessel, resulting in ischemia and/or thrombosis.

4 **[0005]** After hemostasis is achieved by manual compression, the patient is
5 required to remain recumbent for six to eighteen hours under observation to assure
6 continued hemostasis. During this time bleeding from the vascular access wound can
7 restart, potentially resulting in major complications. These complications may require
8 blood transfusion and/or surgical intervention.

9 **[0006]** Bioabsorbable fasteners have also been used to stop bleeding. Generally,
10 these approaches rely on the placement of a thrombogenic and bioabsorbable material,
11 such as collagen, at the superficial arterial wall over the puncture site. This method
12 generally presents difficulty locating the interface of the overlying tissue and the
13 adventitial surface of the blood vessel. Implanting the fastener too far from the
14 desired location can result in failure to provide hemostasis. If, however, the fastener
15 intrudes into the vascular lumen, thrombus can form on the fastener. Thrombus can
16 embolize downstream and/or block normal blood flow at the thrombus site.

17 Implanted fasteners can also cause infection and auto-immune reactions/rejections of
18 the implant.

19 **[0007]** Suturing methods are also used to provide hemostasis after vascular
20 access. The suture-applying device is introduced through the tissue tract with a distal
21 end of the device located at the vascular puncture. Needles in the device draw suture
22 through the blood vessel wall on opposite sides of the punctures, and the suture is
23 secured directly over the adventitial surface of the blood vessel wall to close the
24 vascular access wound.

1 [0008] To be successful, suturing methods need to be performed with a precise
2 control. The needles need to be properly directed through the blood vessel wall so
3 that the suture is well anchored in tissue to provide for tight closure. Suturing
4 methods also require additional steps for the surgeon.

5 [0009] Due to the deficiencies of the above methods and devices, a need exists for
6 a more reliable vascular closure method and device. There also exists a need for a
7 vascular closure device and method that is self-sealing and secure. There also exists a
8 need for a vascular closure device and method requiring no or few extra steps to close
9 the vascular site.

10

11

BRIEF SUMMARY OF THE INVENTION

12 [0010] A method for accessing a biological lumen having a lumen wall and
13 surrounding tissue is disclosed. The method includes forming a path between the
14 lumen wall and the surrounding tissue. The method further includes extending the
15 path through the lumen wall. The method also includes opening the path to the
16 lumen.

17 [0011] The method of forming the path can include inserting a device between the
18 lumen wall and the surrounding tissue. Extending the path can include inserting the
19 device through the lumen wall. Opening the path can include inserting the device into
20 the lumen. The method can include delivering a filler into the path.

21 [0012] The method can include filling the path. Filling the path can include
22 delivering a filler into the path. The filler can have a solid-setting liquid. The filler
23 can have an epoxy.

24 [0013] The method can include applying pressure to the path. Applying pressure
25 to the path can include delivering filler adjacent to the path. Delivering filler adjacent

1 to the path can include delivering filler between the lumen wall and the surrounding
2 tissue. Delivering filler can include delivering filler in the lumen wall. Delivering
3 filler can include delivering filler in the surrounding tissue.

4 [0014] Also disclosed is a method for forming an arteriotomy in a lumen having a
5 lumen wall and surrounding tissue. The method includes translating a device
6 substantially between the lumen wall and the surrounding tissue. The method further
7 includes turning the device toward the lumen. The method also includes translating
8 the device through the lumen wall. The method also includes removing the device
9 from the lumen wall.

10 [0015] The surrounding tissue can have adventitia. Turning can include
11 relaxation of a pre-formed configuration in the device.

12 [0016] The method can also include translating a guide through the device.
13 Translating a guide can include translating the guide into the lumen. The method can
14 also include translating a guide into the lumen. Translating a guide can include
15 translating the guide through the device.

16 [0017] An access device for accessing a biological lumen is disclosed. The
17 device has an introduction device having a relaxed configuration. The relaxed
18 configuration has a first flat section, a first bend at an end of the first flat section, and
19 a first slope extending at a first end from the first bend. The introduction device is
20 configured to be translated with respect to the access device.

21 [0018] The relaxed configuration of the introduction device can have a second
22 bend at a second end of the first slope, a second flat section extending at a first end
23 from the second bend, a third bend at a second end of the second flat section, and a
24 second slope extending from the third bend. The access device can have a delivery
25 guide. The delivery guide can be configured to deliver the introduction device.

1 [0019] The access device can have an anchor. The anchor can extend from the
2 delivery guide. The anchor can be configured to stabilize the access device with
3 respect to the lumen.

4 [0020] A device for accessing a biological lumen is disclosed. The biological
5 lumen has a lumen wall having a longitudinal lumen wall axis. The device has an
6 elongated member that has a longitudinal member axis. The member is configured to
7 access the lumen at a first angle.

8

9 BRIEF DESCRIPTION OF THE DRAWINGS

10 [0021] Figure 1 is an embodiment of a method of using the arteriotomy device in
11 a cross-section of a lumen.

12 [0022] Figures 2 through 5 illustrate a method of using the arteriotomy device in a
13 cross-section of a lumen.

14 [0023] Figure 6 illustrates a portion of an arteriotomized lumen.

15 [0024] Figures 7 through 11 illustrate various embodiments of section A-A of
16 Figure 6.

17 [0025] Figure 12 illustrates an embodiment of the arteriotomy device in a first
18 configuration.

19 [0026] Figure 13 is a close-up view of an embodiment of section B of Figure 12.

20 [0027] Figure 14 illustrates an embodiment of the arteriotomy device of Figure 12
21 in a second configuration.

22 [0028] Figure 15 is a close-up view of an embodiment of section C of Figure 14.

23 [0029] Figure 16 illustrates an embodiment of the arteriotomy device of Figure 12
24 in a third configuration.

25 [0030] Figure 17 is a close-up view of an embodiment of section D of Figure 16.

- 1 [0031] Figure 18 illustrates an embodiment of the arteriotomy device of Figure 12
2 in a fourth configuration.
- 3 [0032] Figure 19 is a close-up view of an embodiment of section E of Figure 18.
- 4 [0033] Figure 20 illustrates an embodiment of the arteriotomy device of Figure 12
5 in a fourth configuration.
- 6 [0034] Figures 21 and 22 are close-up views of various embodiments of section F
7 of Figure 20.
- 8 [0035] Figure 23 illustrates an embodiment of the arteriotomy device.
- 9 [0036] Figure 24 illustrates an embodiment of the arteriotomy device of Figure 12
10 in a fifth configuration.
- 11 [0037] Figure 25 is a close-up view of an embodiment of section G of Figure 24.
- 12 [0038] Figure 26 illustrates an embodiment of the arteriotomy device.
- 13 [0039] Figure 27 is a close-up view of an embodiment of section H of Figure 26.
- 14 [0040] Figures 28 through 32 illustrate various embodiments of cross-section I-I
15 of Figure 27.
- 16 [0041] Figures 33 and 34 are a perspective and side view, respectively, of an
17 embodiment of section H of Figure 26.
- 18 [0042] Figure 35 illustrates an embodiment of a method of using the arteriotomy
19 device in a cross-section of a lumen.
- 20 [0043] Figure 36 is a close-up view of an embodiment of section J of Figure 35.
- 21 [0044] Figure 37 illustrates an embodiment of a method of using an embodiment
22 of the arteriotomy device of Figure 35 in a cross-section of a lumen.
- 23 [0045] Figure 38 is a close-up view of an embodiment of section K of Figure 37.
- 24 [0046] Figures 39 and 40 illustrate various methods of using the arteriotomy
25 device.

1 [0047] Figures 41 and 42 illustrate sectional views of an embodiment of the
2 delivery guide.

3 [0048] Figures 43 through 48 illustrate various embodiments of the introduction
4 device.

5 [0049] Figures 49 and 50 are various embodiments of cross-section K-K of Figure
6 48.

7 [0050] Figures 51 through 53 illustrate various embodiments of the introduction
8 device.

9 [0051] Figures 54 and 55 illustrate various embodiments of the introduction
10 device in relaxed configurations.

11 DETAILED DESCRIPTION

12 [0052] U.S. Patent Application No. 10/844,247, filed 12 May 2004, is
13 incorporated by reference herein in its entirety. Aspects, characteristics, components
14 or complete embodiments of devices and methods disclosed therein can be used with
15 anything disclosed herein.

16 [0053] Figures 1 through 6 illustrate embodiments of an arteriotomy device 2, and
17 methods for accessing (e.g., percutaneously) a biological lumen 4 and deploying an
18 introduction device 6 that can have one or more pre-formed bends. The biological
19 lumen 4 can be surrounded by a lumen wall 8 (e.g., intima and/or media). The lumen
20 wall 8 can be surrounded by surrounding tissue 10 (e.g., media and/or adventitia).

21 [0054] The arteriotomy device 2 can have a delivery guide 12. The delivery guide
22 12 can be slidably attached to an anchor 14. The anchor 14 can be rigid, flexible or
23 combinations thereof. The anchor 14 can be resilient, deformable or combinations
24 thereof. The anchor 14 can be retractable and extendable from the delivery guide 12.
25 The anchor 14 can have a guide eye sheath or an attachable guidewire. The anchor 14

1 can have an integral, or multiple separate and fixedly attached, wound wire. The
2 anchor 14 can have a wire coating, for example a lubricious coating and/or a coating
3 made from urethane

4 [0055] The anchor 14 can have an anchor longitudinal axis 16. The introduction
5 device can have an introduction longitudinal axis 18. The intersection of the anchor
6 longitudinal axis 16 and the introduction longitudinal axis 18 can be an introduction
7 angle 20. The anchor 14 can be inserted into the biological lumen 4 using a Seldinger
8 technique, modified Seldinger technique, or other method known to one having
9 ordinary skill in the art.

10 [0056] The arteriotomy device 2 can be configured to deliver the introduction
11 device at the introduction angle 20. The introduction device 6 can have an
12 introduction longitudinal axis. The introduction angle 20 can be the intersection of
13 the introduction longitudinal axis 18 and the anchor longitudinal axis 16. The
14 introduction angle 20 can have an absolute value from about 0° to about 30°, more
15 narrowly from about 0° to about 19°, yet more narrowly from about 0° to about 15°,
16 yet more narrowly from about 5° to about 10°, for example about 10°.

17 [0057] Any or all elements of the arteriotomy device 2 or other devices or
18 apparatuses described herein can be made from, for example, a single or multiple
19 stainless steel alloys, nickel titanium alloys (e.g., Nitinol), cobalt-chrome alloys (e.g.,
20 ELGILOY® from Elgin Specialty Metals, Elgin, IL; CONICHROME® from
21 Carpenter Metals Corp., Wyomissing, PA), molybdenum alloys (e.g., molybdenum
22 TZM alloy, for example as disclosed in International Pub. No. WO 03/082363 A2,
23 published 9 October 2003, which is herein incorporated by reference in its entirety),
24 tungsten-rhenium alloys, for example, as disclosed in International Pub. No. WO
25 03/082363, polymers such as polyester (e.g., DACRON® from E. I. Du Pont de

1 Nemours and Company, Wilmington, DE), carbon fiber composites (e.g., carbon fiber
2 nylon composite, such as carbon fiber reinforced nylon 66), polypropylene,
3 polytetrafluoroethylene (PTFE), expanded PTFE (ePTFE), polyether ether ketone
4 (PEEK), nylon, polyether-block co-polyamide polymers (e.g., PEBAX® from
5 ATOFINA, Paris, France), aliphatic polyether polyurethanes (e.g., TECOFLEX®
6 from Thermedics Polymer Products, Wilmington, MA), polyvinyl chloride (PVC),
7 polyurethane, thermoplastic, fluorinated ethylene propylene (FEP), absorbable or
8 resorbable polymers such as polyglycolic acid (PGA), polylactic acid (PLA),
9 polydioxanone, and pseudo-polyamino tyrosine-based acids, extruded collagen,
10 silicone, zinc, echogenic, radioactive, radiopaque materials or combinations thereof.
11 Examples of radiopaque materials are barium sulfate, zinc oxide, titanium, stainless
12 steel, nickel-titanium alloys, tantalum and gold.

13 **[0058]** Any or all elements of the arteriotomy device 2, including supplemental
14 closure devices, such as filler, or other devices or apparatuses described herein can be
15 or have a matrix for cell ingrowth or used with a fabric, for example a covering (not
16 shown) that acts as a matrix for cell ingrowth. The matrix and/or fabric can be, for
17 example, polyester (e.g., DACRON® from E. I. du Pont de Nemours and Company,
18 Wilmington, DE), polypropylene, PTFE, ePTFE, nylon, extruded collagen, silicone or
19 combinations thereof.

20 **[0059]** The elements of the arteriotomy device 2 and/or the filler and/or the fabric
21 can be filled and/or coated with an agent delivery matrix known to one having
22 ordinary skill in the art and/or a therapeutic and/or diagnostic agent. The agents
23 within these matrices can include radioactive materials; radiopaque materials;
24 cytogenic agents; cytotoxic agents; cytostatic agents; thrombogenic agents, for
25 example polyurethane, cellulose acetate polymer mixed with bismuth trioxide, and

1 ethylene vinyl alcohol; lubricious, hydrophilic materials; phosphor cholene; anti-
2 inflammatory agents, for example non-steroidal anti-inflammatories (NSAIDs) such
3 as cyclooxygenase-1 (COX-1) inhibitors (e.g., acetylsalicylic acid, for example
4 ASPIRIN® from Bayer AG, Leverkusen, Germany; ibuprofen, for example ADVIL®
5 from Wyeth, Collegeville, PA; indomethacin; mefenamic acid), COX-2 inhibitors
6 (e.g., VIOXX® from Merck & Co., Inc., Whitehouse Station, NJ; CELEBREX®
7 from Pharmacia Corp., Peapack, NJ; COX-1 inhibitors); immunosuppressive agents,
8 for example Sirolimus (RAPAMUNE®, from Wyeth, , Collegeville, PA), or matrix
9 metalloproteinase (MMP) inhibitors (e.g., tetracycline and tetracycline derivatives)
10 that act early within the pathways of an inflammatory response. Examples of other
11 agents are provided in Walton et al, Inhibition of Prostaglandin E₂ Synthesis in
12 Abdominal Aortic Aneurysms, *Circulation*, July 6, 1999, 48-54; Tambiah et al,
13 Provocation of Experimental Aortic Inflammation Mediators and Chlamydia
14 Pneumoniae, *Brit. J. Surgery* 88 (7), 935-940; Franklin et al, Uptake of Tetracycline
15 by Aortic Aneurysm Wall and Its Effect on Inflammation and Proteolysis, *Brit. J.*
16 *Surgery* 86 (6), 771-775; Xu et al, Sp1 Increases Expression of Cyclooxygenase-2 in
17 Hypoxic Vascular Endothelium, *J. Biological Chemistry* 275 (32) 24583-24589; and
18 Pyo et al, Targeted Gene Disruption of Matrix Metalloproteinase-9 (Gelatinase B)
19 Suppresses Development of Experimental Abdominal Aortic Aneurysms, *J. Clinical*
20 *Investigation* 105 (11), 1641-1649 which are all incorporated by reference in their
21 entireties.

22 [0060] The delivery guide 12 can be deployed through the surrounding tissue 10
23 and into the lumen wall 8 and/or the lumen 4. As illustrated in Figures 45 and 46 of
24 U.S. Patent Application No. 10/844,247 for a toggle deployment device, the
25 arteriotomy device 2 can have a pressure check port. The pressure check port can be

1 in fluid communication with a sensor or port on or near the handle of the arteriotomy
2 device 2, such as an external lumen where blood flow can be observed, for example
3 from flow from the end of an external tube or port and/or through a transparent or
4 translucent window. The pressure check port can facilitate deployment of the
5 arteriotomy device 2 to a location where the pressure check port is introduced to
6 pressure, for example when the pressure check port enters the biological lumen 4.
7 The sensor or port on or near the handle of the arteriotomy device 2 will signal that
8 the pressure check port has been placed into the biological lumen 4 (e.g., by
9 displaying a small amount of blood flow). The pressure check port can be deployed
10 into the biological lumen 4 and then withdrawn from the biological lumen 4 to the
11 point where the lumen wall 8 just stops the pressure in the pressure check port. An
12 entry wall retainer port can additionally perform the function as described herein for
13 the pressure check port.

14 **[0061]** The delivery guide 12 can form a first arteriotomy 22. When the anchor
15 14 is properly located in the lumen 4, a luminal retainer 24 and/or an entry wall
16 retainer 26 can be deployed from the anchor 14 and/or the delivery guide 12. The
17 anchor 14, and/or luminal retainer 24, and/or entry wall retainer 26 can be wires, rods,
18 inflatable balloons, or combinations thereof. The anchor 14, and/or luminal retainer
19 24, and/or entry wall retainer 26 can be separate, integral or a single component.

20 **[0062]** When the anchor 14 is properly located in the lumen 4, the introduction
21 device 6 can be translated, as shown by arrow. The introduction device can form a
22 second arteriotomy 28. The introduction device 6 can create a cleavage 30 between
23 the lumen wall 8 and the surrounding tissue 10. The introduction device 6 can cleave
24 a plane in the lumen wall 8, as shown in Figure 2. The cleavage 30 and/or cleavage
25 plane can be substantially parallel with a lumen wall surface 32. The introduction

1 device 6 can be adjacent to the adventitia in a blood vessel. The introduction device 6
2 can be advanced along the subintimal or submedial cleavage plane in a blood vessel.

3 [0063] Once the lumen wall 8, and/or the surrounding tissue 10, and/or the
4 cleavage 30 has been cleaved, a subintimal angioplasty can be performed as known to
5 one having ordinary skill in the art. Once the lumen wall 8, and/or the surrounding
6 tissue 10, and/or the cleavage 30 has been cleaved, a remote endarterectomy can be
7 performed as known to one having ordinary skill in the art.

8 [0064] The introduction device 6 can have one or more straights and/or bends.
9 Various bent introduction devices 34 and straight introduction devices 36 can be
10 swapped during use to selectively cleave the lumen wall 8 and/or the surrounding
11 tissue 10 and/or the cleavage 30. Tools, such as guides (e.g., guidewires), can be
12 inserted through hollow introduction devices 6 to selectively cleave.

13 [0065] As shown in Figure 3, when a bend 34 in the introduction device 6 moves
14 into the lumen wall 8, the introduction device 6 can rotate and slope, as shown by
15 arrow, toward the biological lumen 4. The bend 34 in the introduction device 6 can
16 continue to rotate the introduction device 6 toward the biological lumen 4. When the
17 introduction device 6 is sloping, the introduction angle 20 can be from about 0° to
18 about 120°, more narrowly from about 5° to about 45°, yet more narrowly from about
19 10° to about 30°, for example about 15°.

20 [0066] Figure 4 illustrates that the introduction device 6 can be further translated,
21 as shown by arrow. The introduction device 6 can enter the lumen 4.

22 [0067] The introduction device 6 can pass through an introduction run 38 and an
23 introduction rise 40. The introduction run 38 can be the component of the length of
24 the introduction device 6 in the lumen wall 8 that is parallel to the lumen wall 8. The
25 introduction run 38 can be the component of the length parallel to the lumen wall 8

1 between the opening of the second arteriotomy 28 on the outside of the lumen wall 8
2 and the opening of the second arteriotomy 28 on the inside lumen wall surface 32.
3 The introduction run 38 can be from about 0.10 cm (0.010 in.) to about 3.810 cm
4 (1.500 in.), for example about 0.64 cm (0.25 in.).

5 **[0068]** The introduction rise 40 can be the component of the length of the
6 introduction device 6 in the lumen wall 8 that is perpendicular to the lumen wall 8.
7 The introduction rise 40 can be the component of the length perpendicular to the
8 lumen wall 8 between the opening of the second arteriotomy 28 on the outside of the
9 lumen wall 8 and the opening of the second arteriotomy 28 on the inside lumen wall
10 surface 32. The introduction rise 40 can be from about 0.51 mm (0.020 in.) to about
11 5.08 mm (0.200 in.), for example about 1.0 mm (0.040 in.).

12 **[0069]** An introduction slope can be the ratio of the introduction rise 40 to the
13 introduction run 38. The introduction slope can be from about $\frac{1}{2}$ to about $\frac{1}{40}$ or less,
14 for example about $\frac{1}{6}$, also for example about $\frac{1}{3}$. The introduction slope can be, for
15 examples, equal to or less than about $\frac{1}{2}$ or $\frac{1}{3}$, more narrowly equal to or less than
16 about $\frac{1}{3}$ or $\frac{1}{4}$, yet more narrowly equal to or less than about $\frac{1}{5}$ or $\frac{1}{6}$, even still more
17 narrowly than about equal to or less than about $\frac{1}{10}$.

18 **[0070]** The introduction rise 40 and the introduction run 38 can be components of
19 an introduction vector. The introduction run 38 can be the component of the
20 introduction vector parallel to the lumen wall 8. The introduction rise 40 can be the
21 component of the introduction vector perpendicular to the lumen wall 8. The
22 introduction vector can be a vector from an outer opening 42 to an inner opening 44.
23 The outer opening 42 can be a temporary or permanent opening in the lumen wall 8 or
24 in the surrounding tissue 10 formed by the initial translation of the introduction device

1 6 out of the delivery guide 12. The inner opening 44 can be a temporary or permanent
2 opening on the lumen wall surface 32.

3 [0071] Figure 5 illustrates that the introduction device 6 can act as a pathway for
4 a luminal tool, for example a guidewire 46.

5 [0072] An introducer sheath (not shown) can be inserted over the guidewire 46
6 and/or over or through the introduction device 6. The introducer sheath can be less
7 than about 22 French (7.3 mm, 0.29 in. diameter) or less than the diameter of the
8 lumen to which the introducer sheath is introduced. The introducer sheath can be, for
9 examples, about 6 French (2.3 mm, 0.092 in. diameter), and about 8 French (2.67 mm,
10 0.105 in. diameter). The introducer sheath can be known to one having ordinary skill
11 in the art, for example the introducer sheath described in U.S. Patent No. 5,183,464 to
12 Dubrul, et al.

13 [0073] The introducer sheath can be inserted into the second arteriotomy 28. The
14 introducer sheath can expand the second arteriotomy 28 to a desired or workable size.
15 The introducer sheath can be inserted into the second arteriotomy 28 before and/or
16 after and/or concurrently with when the filler, described infra, is deployed and/or
17 other closure methods or devices are used.

18 [0074] Figures 6 and 7 illustrate an exemplary biological lumen 4 after the
19 arteriotomy device 2 has been deployed to, and removed from, the biological lumen 4.
20 The biological lumen 4 can have the second arteriotomy 28. The biological lumen 4
21 can have a first web 48 on one side of the second arteriotomy 28, and a second web
22 50 on the opposite side of the second arteriotomy 28. The blood pressure 52, shown
23 by arrows, on the first and second webs 48 and 50 can self-seal the second
24 arteriotomy 28.

1 [0075] The second arteriotomy 28 can have an arteriotomy cross-section that can
2 have an arteriotomy diameter 54. The arteriotomy diameter 54 can be from about 0.5
3 mm (0.020 in.) to about 400 mm (15 in.), yet a narrower range from about 1.0 mm
4 (0.040 in.) to about 10.2 mm (0.400 in.), for example about 2.54 mm (0.100 in.). The
5 arteriotomy diameter 54 can be about the diameter of the introduction device 6.

6 [0076] The arteriotomy cross-section can be non-circular. The arteriotomy can
7 have an arteriotomy width and an arteriotomy height. The arteriotomy width can be
8 about half the circumference of the arteriotomy. The arteriotomy width can be from
9 about 1.0 mm (0.040 in.) to about 10.2 mm (0.400 in.), for example about 4.06 mm
10 (0.160 in.).

11 [0077] The arteriotomy height 152 can be less than about 0.51 mm (0.020 in.),
12 more narrowly, less than about 0.38 mm (0.015 in.). The arteriotomy height can be
13 from about 0.25 mm (0.010 in.) to about 1.3 mm (0.050 in.), for example about 0.38
14 mm (0.015 in.). The arteriotomy diameter, and/or height, and/or width can be small
15 enough to enable cell growth, blood clotting, acoustic sealing, heat sealing, gluing,
16 enhanced self-sealing and combinations thereof across the second arteriotomy 28.

17 [0078] The delivery guide 12 and/or other components of the arteriotomy device 2
18 can form a delivery path 56 during use. During percutaneous use, the delivery path
19 can extend to the skin 138.

20 [0079] The second arteriotomy 28 can have a flat 58 and a slope 60. The flat 58
21 can be the cleavage 30 between the lumen wall 8 and the surrounding tissue.

22 [0080] Figure 8 illustrates that the second arteriotomy 28 can have a first flat 58, a
23 first slope 64, a second flat 66, and a second slope 68. The second arteriotomy 28
24 having multiple flats and slopes can be made from one or more introduction devices 6
25 that can have various geometries.

1 [0081] Figure 9 illustrates that the second arteriotomy 28, for example in the flat
2 58 and/or the slope 60, can be filled with a filler 70. The filler 70 can be a solid single
3 component, multiple solid components (e.g., beads), a biocompatible epoxy, or
4 combinations thereof. The filler 70 can be completely or partially bioabsorbable,
5 bioresorbable, bioadsorbable or combinations thereof. The filler 70 can be made from
6 homografts, heterografts or combinations thereof. The filler 70 can be made from
7 autografts, allografts or combinations thereof.

8 [0082] The filler 70 can be delivered (e.g., injected and/or implanted) into the
9 second arteriotomy 28 through the surrounding tissue 10, for example by
10 percutaneous injection. The filler 70 can be delivered (e.g., injected and/or
11 implanted) into the second arteriotomy 28 through the second arteriotomy 28, for
12 example via the introduction device 6 during introduction and/or removal of the
13 introduction device 6.

14 [0083] The filler 70 can be permanently or temporarily deployed. The filler 70
15 can biodissolve after hemostasis is achieved and/or after the arteriotomy is
16 substantially or completely healed. The filler 70 can be maintained from about 15
17 minutes to about 24 hours or more, for example about 120 minutes.

18 [0084] Figure 10 illustrates that the filler can be in the cleavage 30, not in the
19 second arteriotomy 28. The filler 70 can exert a filler pressure 72 on the second
20 arteriotomy 28, for example on the flat 58 and/or slope 60. The second arteriotomy
21 28 can be compressed by the blood pressure 52 and the filler pressure 72.

22 [0085] Figure 11 illustrates that the filler can be in the in the cleavage 30, not in
23 the second arteriotomy 28. The filler 70 can exert filler pressure 72 against the
24 second flat 66 and/or first slope 64 and/or other sections of the second arteriotomy 28.

1 [0086] The filler 70 can be between the second arteriotomy 28 and the lumen 4
2 (not shown). The filler 70 can be in the surrounding tissue 10.

3 [0087] Figures 12 and 13 illustrate the arteriotomy device 2. The arteriotomy
4 device 2 can have a handle 74 that can be integral with or fixedly attached to a
5 delivery guide extension 76. The delivery guide extension 76 can be integral with or
6 fixedly attached to the delivery guide 12. The anchor 14 can extend from, and be
7 slidably and/or fixedly attached to or integral with, the delivery guide 12.

8 [0088] The anchor 14 can have an anchor first length 78 extending from the
9 delivery guide 12. The anchor 14 can have an anchor first bend 80 at the end of the
10 first anchor length 78 distal to the delivery guide 12. An anchor second length 82 can
11 extend at a first end from the anchor first bend 80. A second end of the anchor second
12 length 82 can have an anchor second bend 84. An anchor third length 86 can extend
13 from the anchor second bend 84. The anchor third length 86 can terminate. The
14 anchor 14 can have any combination of lengths and bends.

15 [0089] The radius of curvature for the anchor bends 80 and 84 can be from about
16 0.1 mm (0.004 in.) to about 2.0 mm (0.079 in.). The anchor lengths on both sides of
17 any anchor bend can form an anchoring angle. The anchoring angles can be from
18 about 90° to about 160°, more narrowly from about 120° to about 150°, for example
19 about 135°. The anchor 14 can have a cross-section having an anchor diameter from
20 about 0.38 mm (0.015 in.) to about 1.0 mm (0.039 in.), for example about 0.71 mm
21 (0.028 in.).

22 [0090] The anchor third length 86 can have an anchor tip 88. The anchor tip 88
23 can be narrowed, widened, sharpened, dulled, or otherwise configured to promote
24 sharp or blunt dissection. The anchor tip 88 can have an anchor end port 90. The
25 anchor end port 90 can be in communication with an anchor guidewire lumen (not

1 shown). The anchor guidewire lumen can be in communication with a guide lumen
2 92 in the delivery guide extension 76, and/or the handle 74, and/or a third control 94.

3 The guide lumen 92 can have open access along the delivery guide extension 76,
4 and/or along the handle 74, and/or along the third control 94 (as shown).

5 [0091] The handle 74 can have a first control 96. The first control 96 can be
6 slidably attached to a control slide 98. The first control 96 can be configured to be
7 ergonomically receptive to be activated a digit and/or a palm.

8 [0092] The handle 74 can have a second control 100. The second control 100 can
9 be rotatably attached to the handle 74, for example at a control pivot 102. The second
10 control 100 can have a tab 104. The tab 104 can be configured to be ergonomically
11 receptive to be activated by a digit and/or a palm.

12 [0093] The handle 74 can have a third control 94. The third control can be
13 slidably attached to the handle 74. The third control 94 can have or be a plunger. The
14 third control 94 can have a press 106. The press 106 can be configured to be
15 ergonomically receptive to be activated by a digit and/or a palm. The handle 74 can
16 have one or more grips 108. The grips 108 can be configured to be ergonomically
17 receptive to be held by a digit and/or a palm.

18 [0094] The configuration of any of the first, second or third controls 96, 100 and
19 94 can be any configuration (e.g., the first control can have the rotatable lever of the
20 second control 100).

21 [0095] A guidewire 46 can be in proximity to the anchor tip 88.

22 [0096] Figures 14 and 15 illustrate that the guidewire 46 can be inserted into the
23 anchor end port 90, as shown by arrows. The guidewire 46 can be fed through the
24 anchor guidewire lumen and the guide lumen 92. The guidewire 46 can exit through
25 the open section of the guide lumen 92.

1 [0097] The guidewire 46 can be used to deploy the arteriotomy device to a desired
2 location in a lumen. The arteriotomy device 2 can be translated, for example
3 percutaneously, over and along the guidewire 46. If the guidewire 46 is in a lumen,
4 the arteriotomy device 2 can be translated along the guidewire 46, for example, until
5 blood appears at the pressure check port.

6 [0098] Figure 16 illustrates that the first control 96 can be activated, as shown by
7 arrow. The first control 96 can be translated along the control slide 98. Activating
8 the first control 96 can translatably and/or rotatably deploy the luminal retainer 24, as
9 shown by arrow in Figure 17.

10 [0099] The luminal retainer 24 can be a wire, scaffold or stent - for example made
11 from a deformable or resilient material, such as a shape memory alloy - an inflatable
12 balloon, or combinations thereof. Intraluminal inflatable balloons, such as those
13 inflated with saline solution or carbon dioxide, are known to those having ordinary
14 skill in the art. The luminal retainer 24 can extend into the delivery guide 12.

15 [0100] Figure 17 illustrates that the luminal retainer 24 can be deployed, as shown by
16 arrow, for example due to the activation of the first control 96. The luminal retainer
17 24 can have a first stressed configuration. The luminal retainer 24 can have a second
18 relaxed configuration. The luminal retainer 24 can be in a relaxed or a stressed
19 configuration prior to deployment. The luminal retainer 24 can be in a relaxed or a
20 stressed configuration after deployment. The relaxed configuration of the luminal
21 retainer 24 can be the deployed configuration of the luminal retainer 24.

22 [0101] The luminal retainer 24 can be configured to press against the lumen 4 during
23 use. The luminal retainer can be deployed by translating, rotating or a combination
24 thereof, with respect to the anchor 14.

1 [0102] The luminal retainer 24 can deploy from the anchor 14. The luminal retainer
2 24 can deploy from a luminal retainer port (not shown). The luminal retainer 24 can
3 have a luminal retainer deployed diameter. The luminal retainer deployed diameter
4 can be from about 2.54 mm (0.100 in.) to about 10.2 mm (0.400 in.), for example
5 about 6.35 mm (0.250 in.).

6 [0103] Figures 18 illustrates that the second control 100 can be activated, as shown by
7 arrow. The second control 100 can be rotated around the control pivot 102.
8 Activating the second control can translatably and/or rotatably retract the anchor 14,
9 as shown by arrows in Figure 19.

10 [0104] Figure 19 illustrates that the anchor 14 can translate both parallel and/or
11 perpendicular to the delivery guide 12.

12 [0105] The anchor first length 78 can have an anchor shift 110 or small inflection.
13 The anchor shift 110 can be configured wherein the anchor first length 78 shifts
14 perpendicular to the longitudinal axis of the delivery guide 12, as seen in Figure 19.
15 An introduction lumen exit port 112 can be covered by the anchor first length 78, for
16 example, before the anchor is retracted into the delivery guide 12.

17 [0106] When the anchor is retracted into the delivery guide 12, an introduction lumen
18 exit port 112 can be exposed. When the anchor is retracted into the delivery guide 12,
19 the anchor shift 110, laterally positioned compared to the rest of the anchor first
20 length 78, can expose the introduction lumen exit port 112. When the anchor is
21 retracted into the delivery guide 12, the anchor shift 110, laterally positioned
22 compared to the rest of the anchor first length 78, can force the entire anchor 14 to
23 move laterally, thereby exposing the introduction lumen exit port 112.

24 [0107] Figure 20 illustrates that the third control 94 can be activated, as shown by
25 arrow. The third control 94 can be translated with respect to the handle 74.

1 Activating the third control can translatably deploy the introduction device 6, as
2 shown by arrow in Figure 21.

3 **[0108]** The introduction device 6 can have an introduction device diameter. The
4 introduction device diameter can be from about 0.25 mm (0.010 in.) to about 1.0 mm
5 (0.039 in.), for example about 0.56 mm (0.022 in.).

6 **[0109]** The arteriotomy device 2 can be configured to deploy the introduction device
7 6 from the anchor 14 and/or the delivery guide 12 (as shown). The anchor 14 and/or
8 delivery guide 12 can have the introduction lumen exit port 112. The introduction
9 device 6 can deploy through the introduction lumen exit port 112. The introduction
10 device 6 can be a solid or hollow needle, or combinations thereof.

11 **[0110]** Figure 22 illustrates that the distance perpendicular to the introduction device
12 6 between the introduction lumen exit port 112 to the anchor first length 78 can be
13 substantially and/or completely equal to the introduction rise 40. The anchor 14 can
14 have one or more radiopaque marks. For example, the anchor first length 78 can have
15 a first radiopaque mark 114. The first radiopaque mark 114 can be significantly
16 longer along the anchor first length 78 than the first radiopaque mark 114 is tall or
17 wide. The delivery guide 12 can have a second radiopaque mark 116. The second
18 radiopaque mark 116 can be parallel and aligned with the path of the introduction
19 device 6 where the introduction device 6 exits the introduction lumen exit port 112.
20 The user can view a radiograph or to assist in the placement of the arteriotomy device
21 2.

22 **[0111]** Figure 23 illustrates that the arteriotomy device can have a first, second and
23 third radiopaque marks 114, 116 and 118. The first radiopaque mark 114 can be on
24 the handle. The second radiopaque mark 116 can be on the delivery guide extension
25 76. The third radiopaque mark 118 can be on the anchor 14. A straight alignment

1 axis 120 can pass through the first, second and third radiopaque marks 114, 116 and
2 118. The user can utilize the alignment axis 120 to assist in the placement of the
3 arteriotomy device 2, for example while viewing a radiograph.

4 **[0112]** The radiopaque marks can be marks for any type of medical imagining. For
5 example, the marks could be sono-opaque and/or sono-reflective for use with
6 sonographs.

7 **[0113]** Figure 24 illustrates that the third control 94 can be activated further, for
8 example, by continuing to translate the third control 94 toward the handle 74, as
9 shown by arrow. Activating or re-activating the third control can translatably deploy
10 the introduction device 6, as shown by arrow in Figure 25.

11 **[0114]** The introduction device 6 can have a bend 34. The bend 34 can be in a
12 relaxed configuration of the introduction device 6. If the introduction device 6 is
13 deployed far enough, the bend 34 can rotate the introduction device 6 toward the
14 lumen 4.

15 **[0115]** The first, second and third controls 96, 100 and 94 can have lockouts to
16 prevent the controls 96, 100 and 94 from being activated incorrectly (e.g., to prevent
17 use in the wrong order).

18 **[0116]** Figure 26 illustrates that the luminal retainer 24 can form a circular, oval, or
19 spiral configuration. Figure 27 illustrates that the anchor 14 can have a luminal
20 retainer exit port 122.

21 **[0117]** Figures 28 through 32 illustrate various configurations of the luminal retainer
22 24 in the anchor 14 prior to deployment. Figure 28 illustrates that one end of the
23 luminal retainer can be fixedly or rotatably attached to the anchor 14. The luminal
24 retainer 24 can have a ball 124 and the anchor 14 can have a socket 126. The ball 124
25 can have an interference fit in the socket 126. When the deployment force is applied,

1 shown by arrow, the luminal retainer 24 can relax, if pre-stressed (e.g., heat-treated to
2 a specific shape), and/or be forced into buckling out through the luminal retainer exit
3 port 122.

4 **[0118]** Figure 29 illustrates that the luminal retainer 24 can be loaded in a loop or
5 spiral configuration in the anchor 14. When the deployment force is applied, as
6 shown by arrow, the loop 128 will naturally expand and exit the luminal retainer port
7 122.

8 **[0119]** Figure 30 illustrates that the luminal retainer can be pre-formed with a
9 curvature 130. When the deployment force is applied, shown by arrow, the luminal
10 retainer 24 can relax, if pre-stressed (e.g., heat-treated to a specific shape), and/or be
11 forced into buckling into the anchor 14 across from the luminal retainer exit port 122.
12 The luminal retainer 24 can then buckle and/or twist at the weakest point along the
13 length, for example the curvature 130. The luminal retainer 24 can then exit through
14 the luminal retainer exit port 122.

15 **[0120]** Figure 31 illustrates that the luminal retainer 24 can be fixed to the anchor 14,
16 for example at a fixation area 132 (e.g., via welding, gluing, snap fitting, etc.). Figure
17 32 illustrates that the embodiments of the luminal retainer can be reversed in direction
18 with respect to the remainder of the arteriotomy device 2.

19 **[0121]** Figures 33 and 34 illustrate that the luminal retainer 24 can deploy as the loop
20 or spiral. The luminal retainer 24 can deploy out of the luminal retainer exit port 122
21 on the anchor (as shown) and/or the delivery guide 12.

22 **[0122]** Figures 35 and 36 illustrate that arteriotomy device 2 can be translated deep
23 enough into the lumen 4 to contact the deployed luminal retainer 24 against the lumen
24 wall 8 opposite from the arteriotomy 134. Figures 37 and 38 illustrate that the handle
25 74 can be translated, as shown by arrow in Figure 37, away from the lumen 4. The

1 luminal retainer 24 can be translated, as shown by arrow in Figure 38, into the lumen
2 wall 8 closest to the arteriotomy 134. The luminal retainer 24 can abut the lumen wall
3 8, for example, acting as the entry wall retainer 26. The delivery guide extension 76
4 can be rotatably attached to the delivery guide 12, for example by a hinge 136.

5 **[0123]** Figure 39 illustrates that the handle 74 and the delivery guide extension 76 can
6 rotate around the hinge, as shown by arrows, with respect to the delivery guide 12, the
7 anchor 14 and the luminal retainer 24. Rotated configurations of the handle 74 and
8 the delivery guide extension are shown in phantom lines. The handle 74 and delivery
9 guide extension 76 can be manipulated during use with a minimal impact on the
10 delivery guide 12, the anchor 14 and the luminal retainer 24.

11 **[0124]** Figure 40 illustrates that the delivery guide extension can be flexible. The
12 handle 74 and the delivery guide extension 76 can rotate around the flexible delivery
13 guide extension 76, as shown by arrows, with respect to the delivery guide 12, the
14 anchor 14 and the luminal retainer 24. Rotated configurations of the handle 74 and the
15 delivery guide extension are shown in phantom lines.

16 **[0125]** Figure 41 illustrates a first longitudinal section 140 of the delivery guide 12.
17 Figure 42 illustrates a second longitudinal section 142 of the delivery guide 12. The
18 first longitudinal section 140 can be a complete or substantial mirror image of the
19 second longitudinal section 142.

20 **[0126]** An extension attachment 144 can be configured to fixedly attach to the
21 delivery guide extension 76. The extension abutment 146 can be configured to abut
22 against and/or fixedly attach to the delivery guide extension 76. The extension
23 attachment 144 and/or extension abutment 146 can form fluid-tight and/or air-tight
24 seals with the delivery guide extension 76.

1 [0127] The anchor lumen 148 can be configured to receive and deploy the anchor 14
2 out the anchor exit port 150. The introducer lumen 152 can be configured to receive
3 and deploy the introduction device 6 out the introduction lumen exit port 112. The
4 relative geometries of the anchor lumen 148, the introducer lumen 152, the anchor
5 exit port 150, and the introduction lumen exit port 112 can be changed to alter the
6 introduction angle 20, introduction run 38, introduction rise 40, and the geometry of
7 the arteriotomy 134 including the geometries of the slopes 60 and flats 58 of the
8 arteriotomy 134.

9 [0128] The delivery guide half attachments 154 can attach the first longitudinal
10 section 140 to the second longitudinal section 142, for example by rotatably attaching
11 to a screw. The seam surfaces 156 of the first longitudinal section 140 can form fluid-
12 tight and/or air-tight seals with the seam surfaces 156 of the second longitudinal
13 section 142. The delivery guide tip 158 can be sharpened, dulled, or otherwise
14 configured to aid sharp or blunt dissection.

15 [0129] Figures 43 through 46 illustrate solid introduction devices 6 that can each have
16 an introduction device shaft 160 that can terminate in an introduction device tip 162.
17 As shown in Figure 43, the introduction device tip 162 can have a centered needle
18 point. The introduction device tip 162 can have an introduction device tip cross-
19 section 164. The introduction device tip cross-section 164 can be circular or square or
20 combinations thereof. The introduction device tip can be curved (not shown).

21 [0130] Figure 44 illustrates that the introduction device tip 162 can have an off-center
22 needle point. The introduction device tip cross-section 164 can be circular or square
23 or combinations thereof. The introduction device 6 can be configured to have a flat
24 side along the introduction device shaft 160 and along the introduction device tip 162.

1 [0131] Figure 45 illustrates that the introduction device tip 162 can have a centered
2 chisel point. The introduction device tip cross-section 164 can be oval, rectangular,
3 elliptical, or a combination thereof.

4 [0132] Figure 46 illustrates that the introduction device tip 162 can have a off-
5 centered chisel point. The introduction device tip cross-section 164 can be oval,
6 rectangular, elliptical, or a combination thereof. The introduction device 6 can be
7 configured to have a flat side along the introduction device shaft 160 and along the
8 introduction device tip 162.

9 [0133] Figures 47 through 53 illustrate hollow introduction devices 6 that can each
10 have an introduction device shaft 160 that can terminate in an introduction device tip
11 162. The introduction device shaft 160 can have a hollow guide lumen 92 than can
12 extend to the introduction device tip 162 or to the side of the introduction device shaft
13 160. The guide lumen 92 can terminate at a guide port 166. A guide (e.g., a
14 guidewire or other tool) can be slidably attached to the introduction device 6 in the
15 guide lumen 92. The guide lumen can have a guide shaft 168 that can terminate in a
16 guide tip 170. The guide 172 can exit the introduction device at the guide port 166.

17 [0134] As shown in Figure 47, the introduction device tip 162 can be a centered
18 hollow needle point. The guide tip 170 can be a centered needle point. The guide tip
19 170 can be aligned with the introduction device tip to form a substantially smooth
20 combined tip.

21 [0135] As shown in Figure 48, the introduction device tip 162 can be an off-center
22 hollow needle point. The guide tip 170 can be a centered needle point.

23 [0136] Figure 49 illustrates that the guide shaft 168 can have a key 174 and/or a slot
24 176 (not shown). The introduction device shaft 160 can have a slot 176 and/or a key
25 174 (not shown). The key 174 on the guide shaft 168 can slidably attach to the slot

1 176 in the introduction device shaft 160. The slidable attachment of the key 174 and
2 slot 176 can prevent the guide shaft 168 from rotating about a longitudinal axis with
3 respect to the introduction device shaft 160.

4 [0137] Figure 50 illustrates that the guide lumen 92 and the guide shaft 168 can be
5 oval. The oval configurations of the guide lumen 92 and the guide shaft 168 can
6 prevent the guide shaft 168 from rotating about a longitudinal axis with respect to the
7 introduction device shaft 160.

8 [0138] Figure 51 illustrates that the introduction device tip 162 can have a curved end
9 178. The curved end 178 can be configured to fit into a recess 180 in the guide 172.
10 The recess 180 can have a hook 182. The curved end 178 can have a notch 184. The
11 hook 182 can interference fit and/or snap fit the notch 184.

12 [0139] Figure 52 illustrates that the guide lumen 92 can be curved. The guide lumen
13 92 can terminate at a guide port 166 in the side of the introduction device shaft 160.

14 [0140] Figure 53 illustrates that the introduction device tip 162 and/or the
15 introduction device shaft (not shown) can be curved. The guide 172 or lengths of the
16 guide 172 can be curved in a relaxed configuration. The guide 172 or lengths of the
17 guide 172 can be curved in a stressed configuration due to the curvature of the
18 introduction device 6.

19 [0141] Any of the introduction devices 6 shown in Figure 43 through Figure 46 can
20 be hollowed and configured identically or similar to the introduction devices
21 illustrated in Figures 47 through Figure 53. Any of the introduction devices 6 shown
22 in Figure 47 through Figure 53 can have no guide lumen and be configured identically
23 or similar to the introduction devices illustrated in Figures 43 through Figure 46.

24 [0142] The guides 172 and/or guide lumens 92 and/or introduction devices 6 can have
25 a lubricious coating or be impregnated to elute a lubricious material.

1 [0143] Figure 54 illustrates that the introduction device 6 can have a relaxed
2 configuration having a flat 58 that can have a bend 34 at one end. A slope can extend
3 from the bend 34. The relaxed configuration of the introduction device 6 can form the
4 arteriotomy configuration, for example, as shown in Figures 7 and 9, during
5 deployment of the introduction device 6 from the delivery guide 12.

6 [0144] Figure 55 illustrates that the introduction device 6 can have a relaxed
7 configuration having a first flat 62 that can have a first bend 186 at one end. A first
8 slope 64 can extend at a first end from the first bend 186. The first slope 64 can have
9 at a second end a second bend 188. A second flat 66 can extend at a first end from the
10 second bend 188. The second flat 66 can have at a second end a third bend 190. A
11 second slope 68 can extend from the third bend 190. The relaxed configuration of the
12 introduction device 6 can form the arteriotomy configuration, for example, as shown
13 in Figures 8, 10 and 11, during deployment of the introduction device 6 from the
14 delivery guide 12.

15 [0145] The introduction device 6, for example a hollow introduction device 6, can act
16 as a pathway for a luminal tool, for example tools such as a guidewire 46, to be
17 deployed into the lumen 4. The introduction device 6, for example a solid
18 introduction device 6, can be removed from the second arteriotomy 28 and the
19 luminal tool can be deployed through, for example, the introduction lumen exit port
20 112, and the second arteriotomy 28. The introduction device 6, or part thereof, can be
21 the luminal tool, for example the guide 172. The introduction device 6 can be further
22 deployed and used as a luminal tool after passing through the lumen wall 8.

23 [0146] The guide 172 can remain substantially in place after the arteriotomy device 2
24 is removed. A portion of the guide 172 can be outside the lumen 4 and another
25 portion of the guide 172 can be inside the lumen 4. The guide proximal end can then

1 be attached to additional devices and implants to guide the devices and implants into
2 the lumen. The filler 70 can be added after additional procedures are completed and
3 the guide 172 is removed, or before the guide 172 is removed, using the guide 172 to
4 redeploy the arteriotomy device 2 back to the arteriotomy 134 to deliver the filler 70.
5

6 METHOD OF MANUFACTURE

7 [0147] The elements of the arteriotomy device 2, and those of any other devices and
8 components disclosed herein, can be directly attached by, for example, melting,
9 screwing, gluing, welding or use of an interference fit or pressure fit such as crimping,
10 snapping, or combining methods thereof. The elements can be integrated, for
11 example, molding, die cutting, laser cutting, electrical discharge machining (EDM) or
12 stamping from a single piece or material. Any other methods can be used as known to
13 those having ordinary skill in the art.

14 [0148] Integrated parts can be made from pre-formed resilient materials, for example
15 resilient alloys (e.g., Nitinol, ELGILOY®) that are preformed and biased into the
16 post-deployment shape and then compressed into the deployment shape as known to
17 those having ordinary skill in the art.

18 [0149] Any elements of the arteriotomy device 2, and those of any other devices and
19 components disclosed herein, including the supplemental closure devices, as a whole
20 after assembly, can be coated by dip-coating, brush-coating or spray-coating methods
21 known to one having ordinary skill in the art.

22 [0150] One example of a method used to coat a medical device for vascular use is
23 provided in U.S. Patent No. 6,358,556 by Ding et al. and hereby incorporated by
24 reference in its entirety. Time release coating methods known to one having ordinary

1 skill in the art can also be used to delay the release of an agent in the coating, for
2 example the coatings on the supplemental closure devices.

3 **[0151]** Any elements herein can be covered with a fabric, for example polyester (e.g.,
4 DACRON® from E. I. du Pont de Nemours and Company, Wilmington, DE),
5 polypropylene, PTFE, ePTFE, nylon, extruded collagen, silicone or combinations
6 thereof. Methods of covering an implantable device with fabric are known to those
7 having ordinary skill in the art.

8 **[0152]** As shown in Figures 13, 41 and 42, the delivery guide 12 can be fixedly
9 composited, for example with a weld, unitary construction (e.g., by casting), snap
10 fitting components, a screw 192, or combinations thereof. The screw 192 can attach
11 the delivery guide 12 to the delivery guide extension 76, for example by screwing
12 through the delivery guide and/or by squeezing the delivery guide onto the delivery
13 guide extension.

14 **[0153]** The radiopaque marks can be attached to the elements and/or coated on the
15 surface of the elements and/or manufactured integrally in the elements.

16 **[0154]** The introduction device 6, guide 172, anchor 14, luminal retainer 24, entry
17 wall retainer 26, any other elements, or combinations thereof can be heat set in a
18 relaxed configuration using methods know to those having ordinary skill in the art.

19 **[0155]** It is apparent to one skilled in the art that various changes and modifications
20 can be made to this disclosure, and equivalents employed, without departing from the
21 spirit and scope of the invention. Elements shown with any embodiment are
22 exemplary for the specific embodiment and can be used on other embodiments within
23 this disclosure.

CLAIMS

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25

I claim:

1. A method for accessing a biological lumen having a lumen wall and surrounding tissue, the method comprising:

forming a path between the lumen wall and the surrounding tissue;

extending the path through the lumen wall; and

opening the path to the lumen.

2. The method of Claim 1, wherein forming the path comprises inserting a device between the lumen wall and the surrounding tissue.

3. The method of Claim 2, wherein extending the path comprises inserting the device through the lumen wall.

4. The method of Claim 3, wherein opening the path comprises inserting the device into the lumen.

5. The method of Claim 4, further comprising delivering a filler into the path.

6. The method of Claim 1, further comprising filling the path.

7. The method of Claim 6, wherein filling the path comprises delivering a filler into the path.

8. The method of Claim 7, wherein the filler comprises a solid-setting liquid.

1

2 9. The method of Claim 8, wherein the filler comprises an epoxy.

3

4 10. The method of Claim 1, further comprising applying pressure to the path

5

6 11. The method of Claim 10, wherein applying the pressure comprises delivering
7 filler adjacent to the path.

8

9 12. The method of Claim 11, wherein delivering filler comprises delivering filler
10 between the lumen wall and the surrounding tissue.

11

12 13. The method of Claim 11, wherein delivering filler comprises delivering filler in
13 the lumen wall.

14

15 14. The method of Claim 11, wherein delivering filler comprises delivering filler in
16 the surrounding tissue.

17

18 15. A method for forming an arteriotomy in a lumen having a lumen wall and
19 surrounding tissue, the method comprising:

20 translating a device substantially between the lumen wall and the surrounding
21 tissue;

22 turning the device toward the lumen;

23 translating the device through the lumen wall; and

24 removing the device from the lumen wall.

25

- 1 16. The method of Claim 15, wherein the surrounding tissue comprises adventitia.
2
- 3 17. The method of Claim 15, wherein turning comprises relaxation of a pre-formed
4 configuration in the device.
5
- 6 18. The method of Claim 15, further comprising translating a guide through the
7 device.
8
- 9 19. The method of Claim 18, wherein translating a guide comprises translating the
10 guide into the lumen.
11
- 12 20. The method of Claim 15, further comprising translating a guide into the lumen.
13
- 14 21. The method of Claim 20, wherein translating a guide comprises translating the
15 guide through the device.
16
- 17 22. An access device for accessing a biological lumen comprising:
18 an introduction device having a relaxed configuration comprising a first flat
19 section, a first bend at an end of the first flat section, and a first slope extending at a
20 first end from the first bend, the wherein the introduction device is configured to be
21 translated with respect to the access device.
22
- 23 23. The device of Claim 22, wherein the relaxed configuration of the introduction
24 device further comprises a second bend at a second end of the first slope, a second flat

1 section extending at a first end from the second bend, a third bend at a second end of
2 the second flat section, and a second slope extending from the third bend.

3

4 24. The device of Claim 23, further comprising a delivery guide, wherein the delivery
5 guide is configured to deliver the introduction device.

6

7 25. The device of Claim 24, further comprising an anchor, wherein the anchor
8 extends from the delivery guide, and wherein the anchor is configured to stabilize the
9 access device with respect to the lumen.

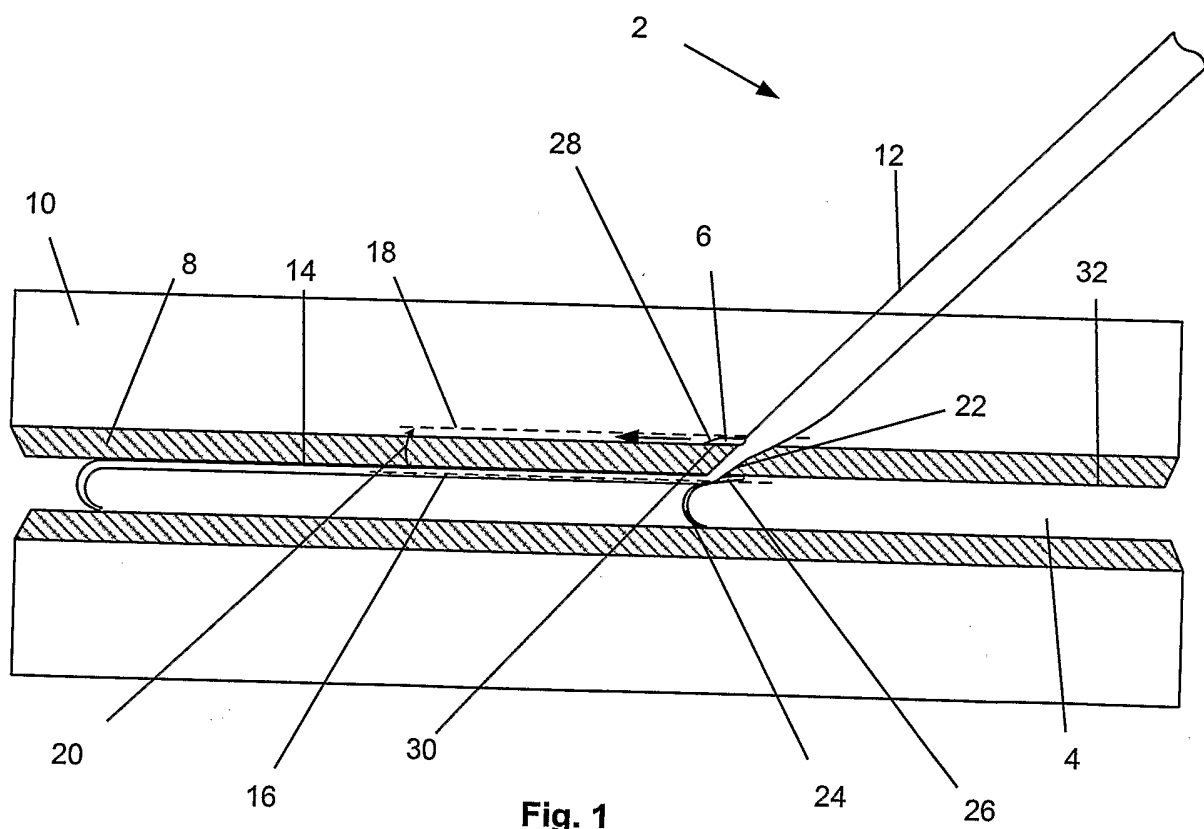


Fig. 1

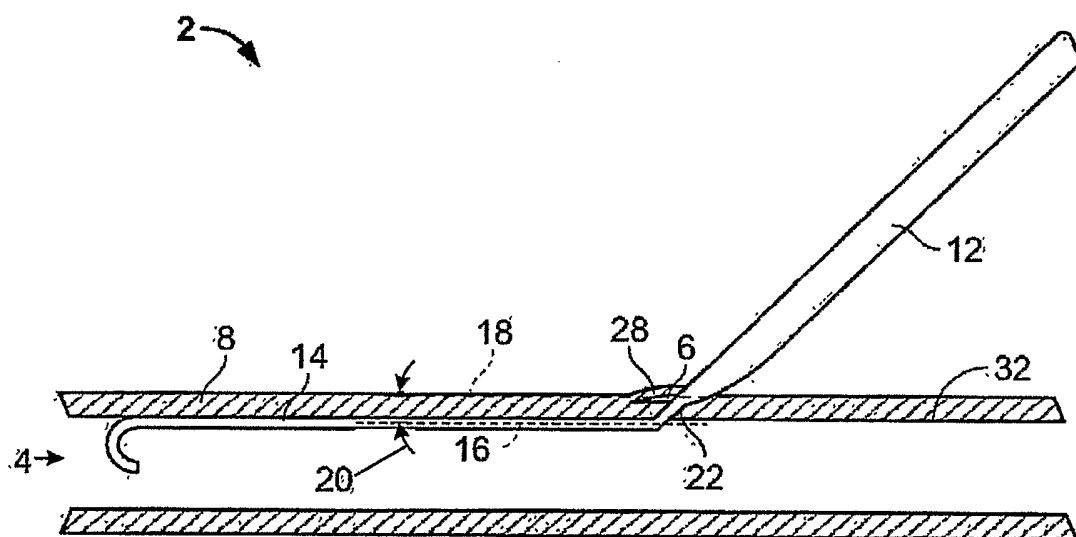


FIG. 2

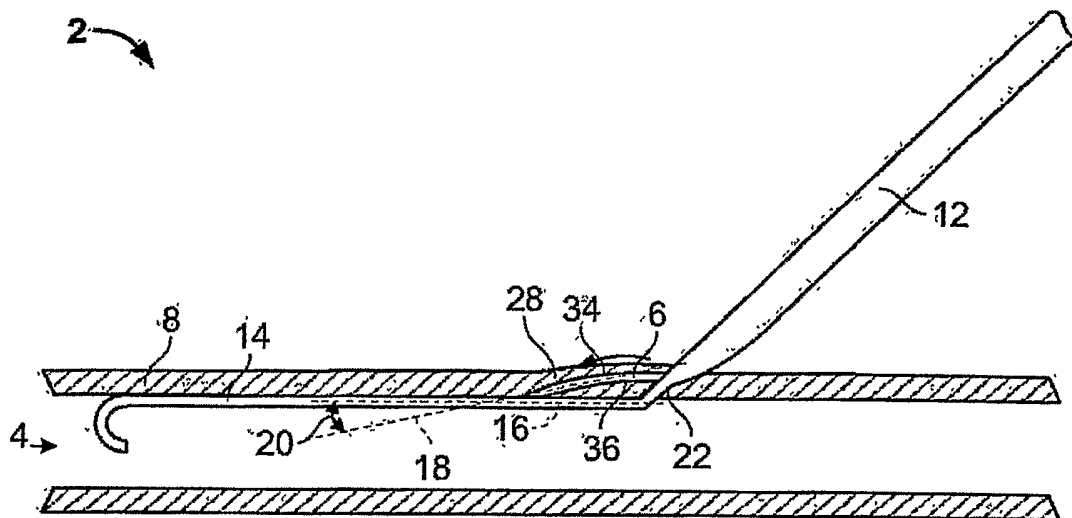


FIG. 3

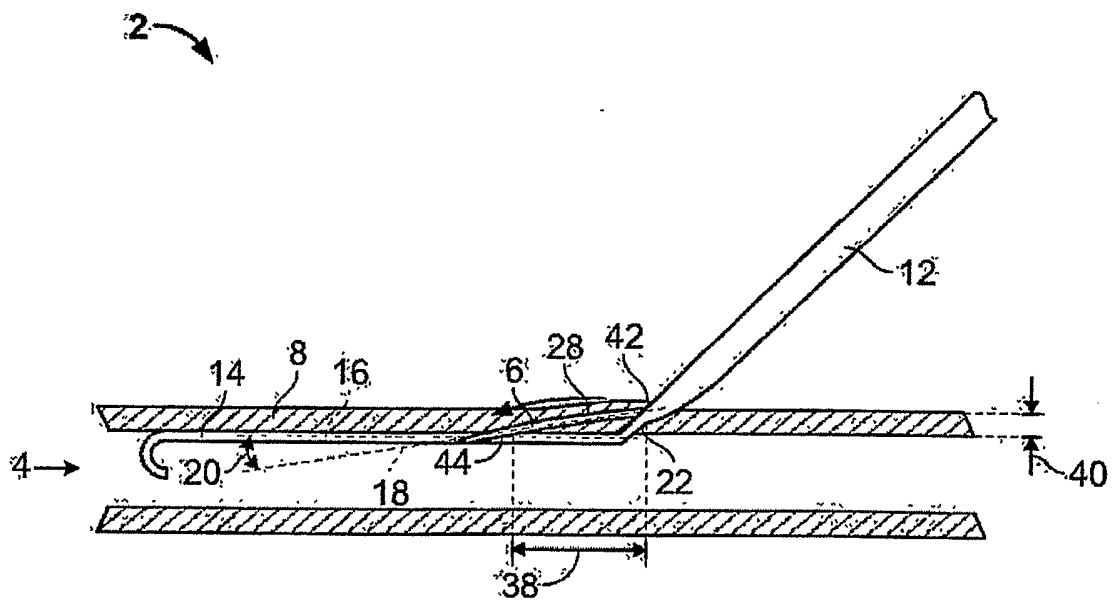


FIG. 4

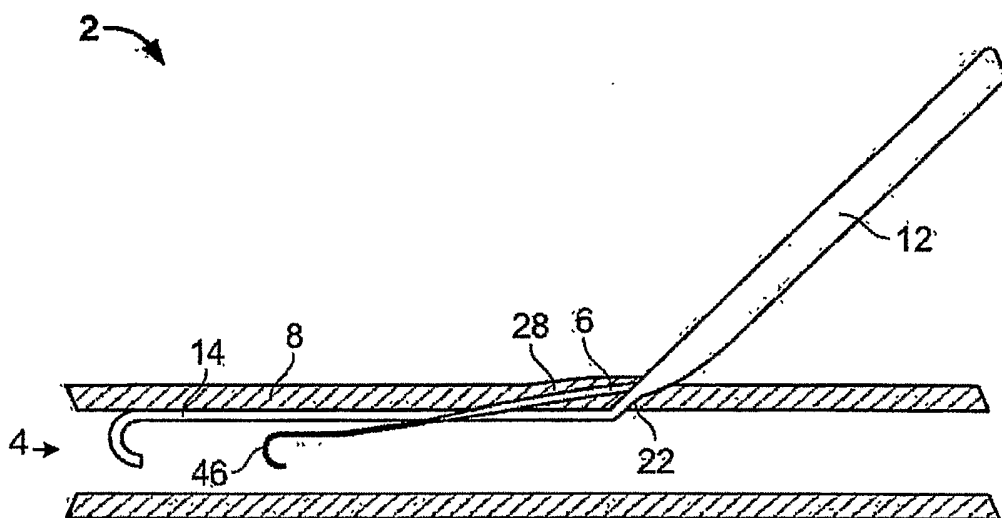


FIG. 5

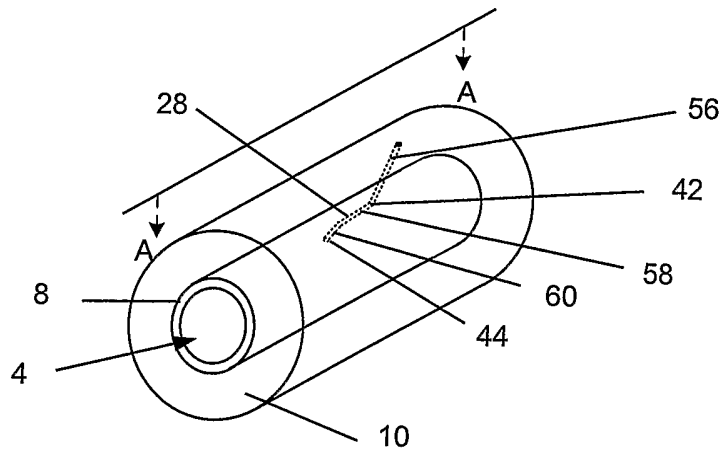


Fig. 6

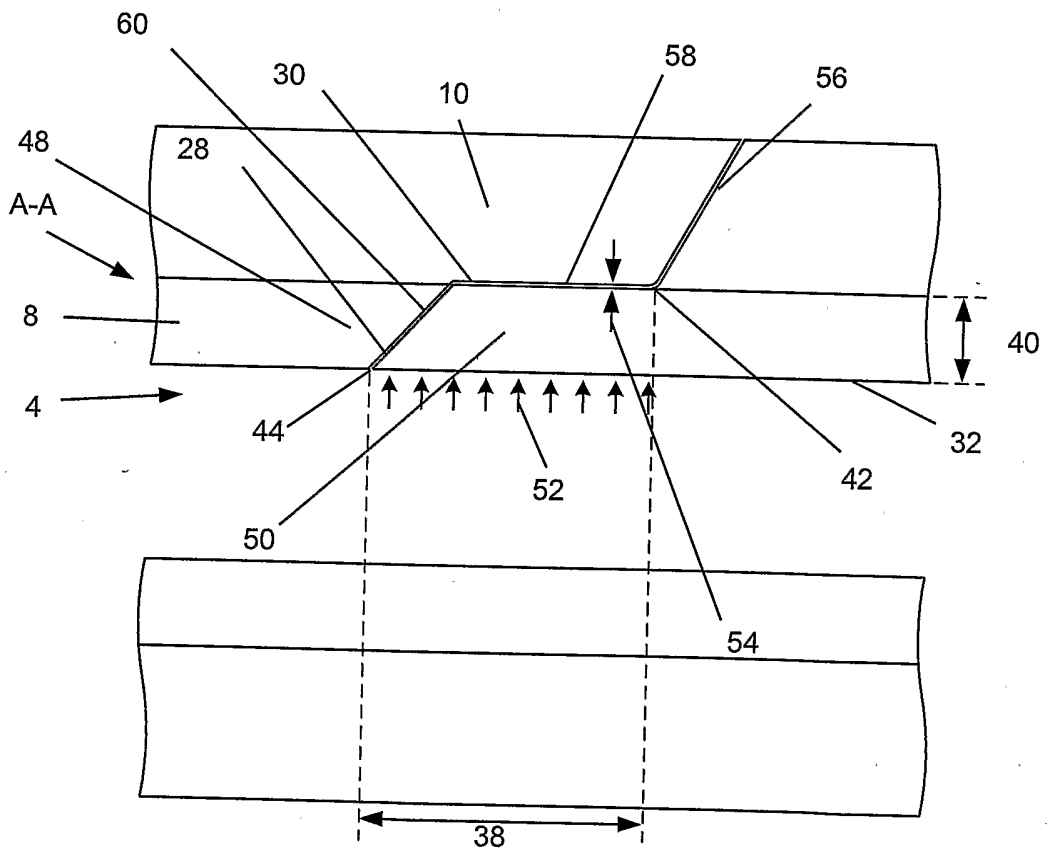


Fig. 7

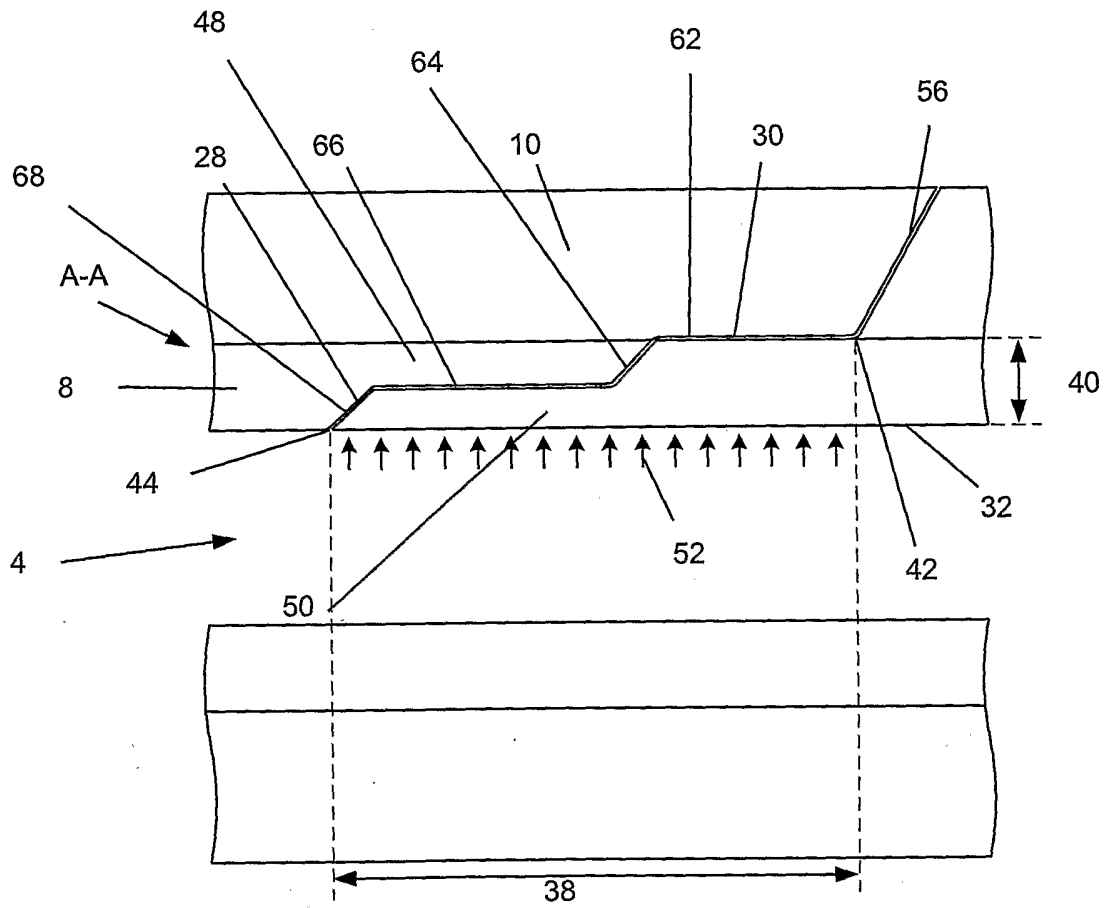


Fig. 8

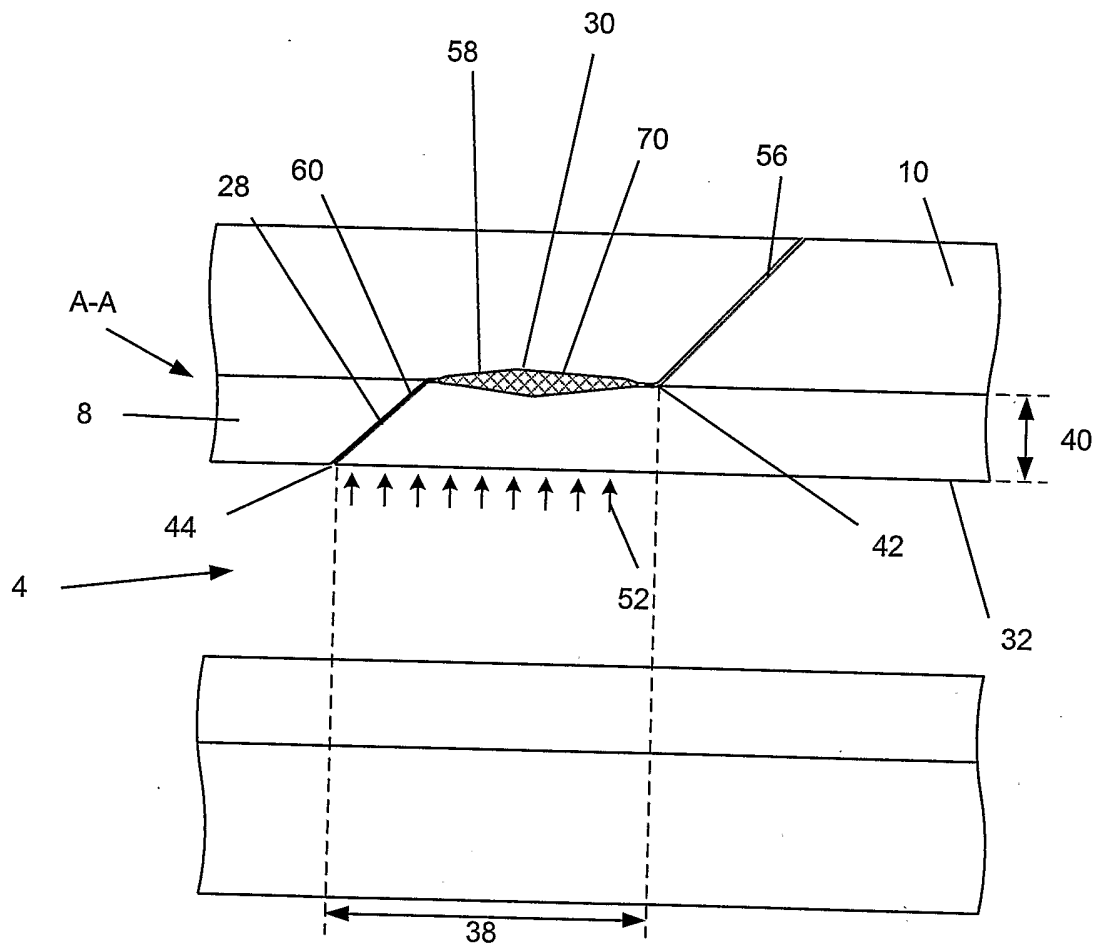


Fig. 9

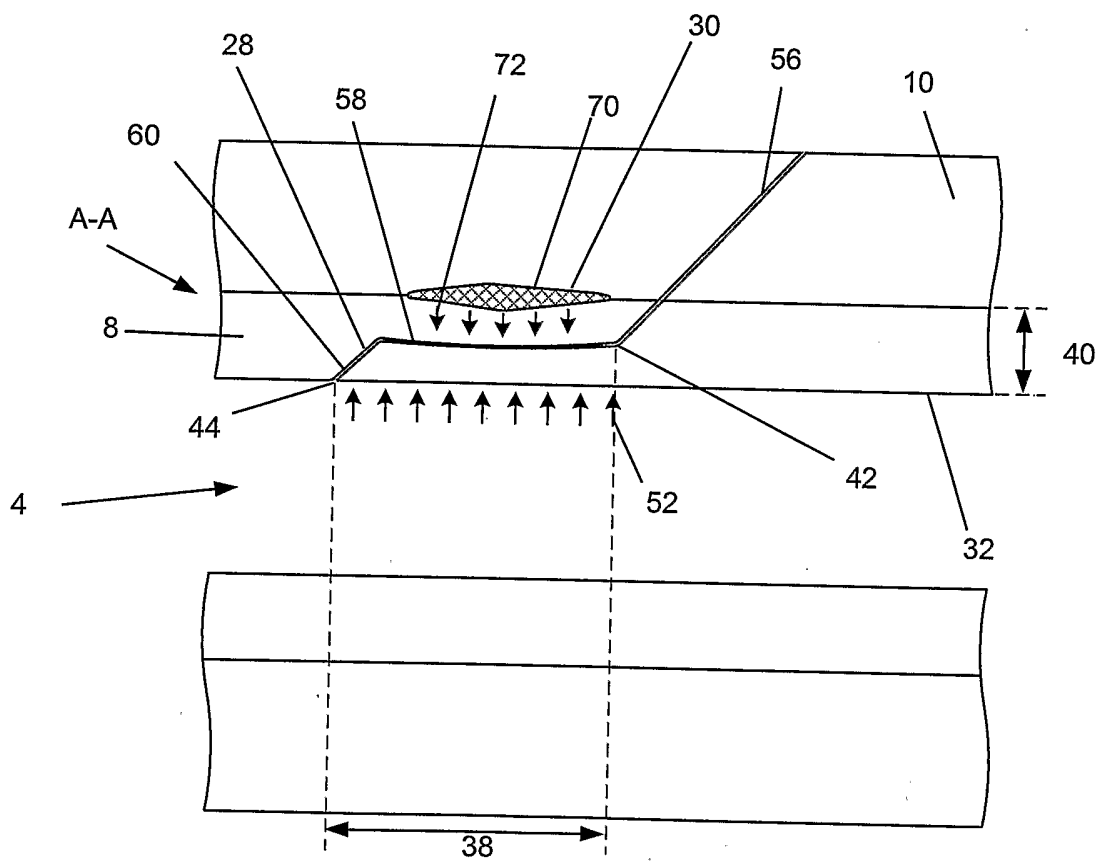


Fig. 10

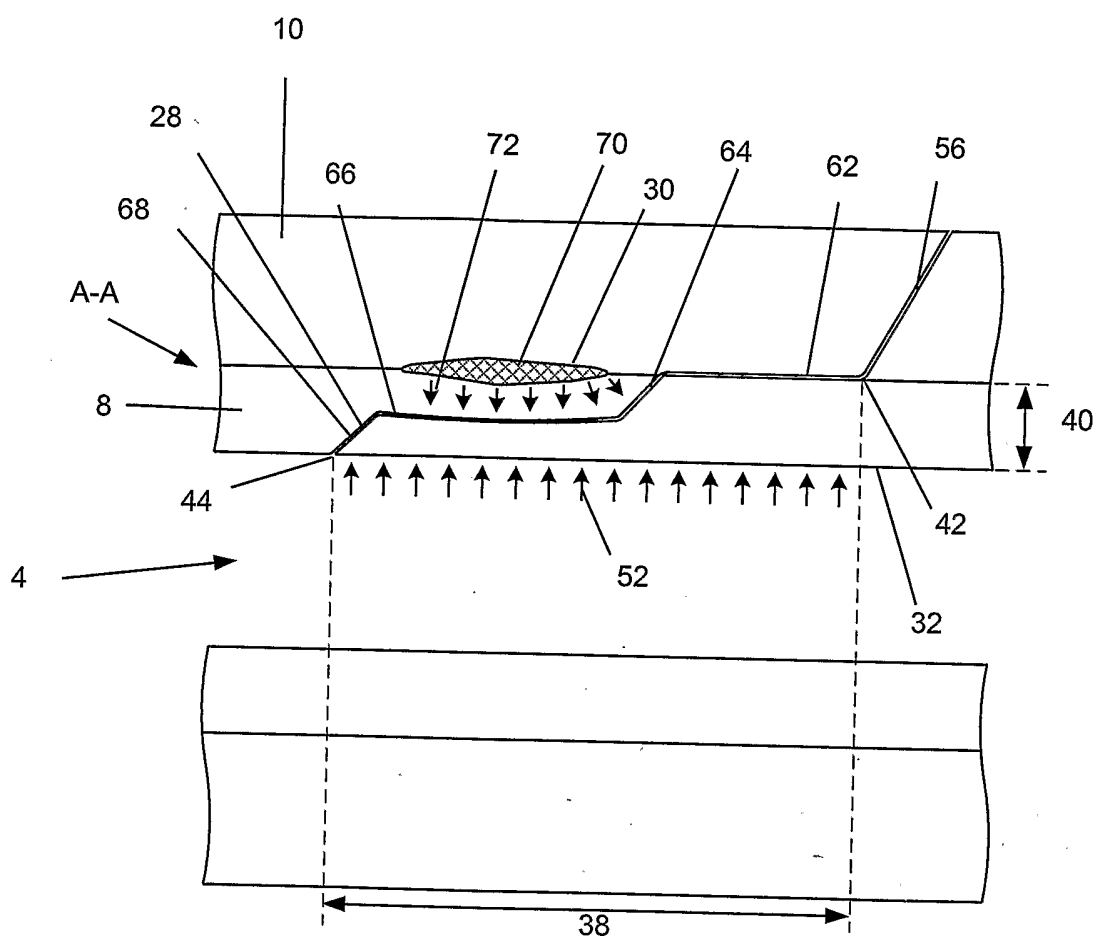


Fig. 11

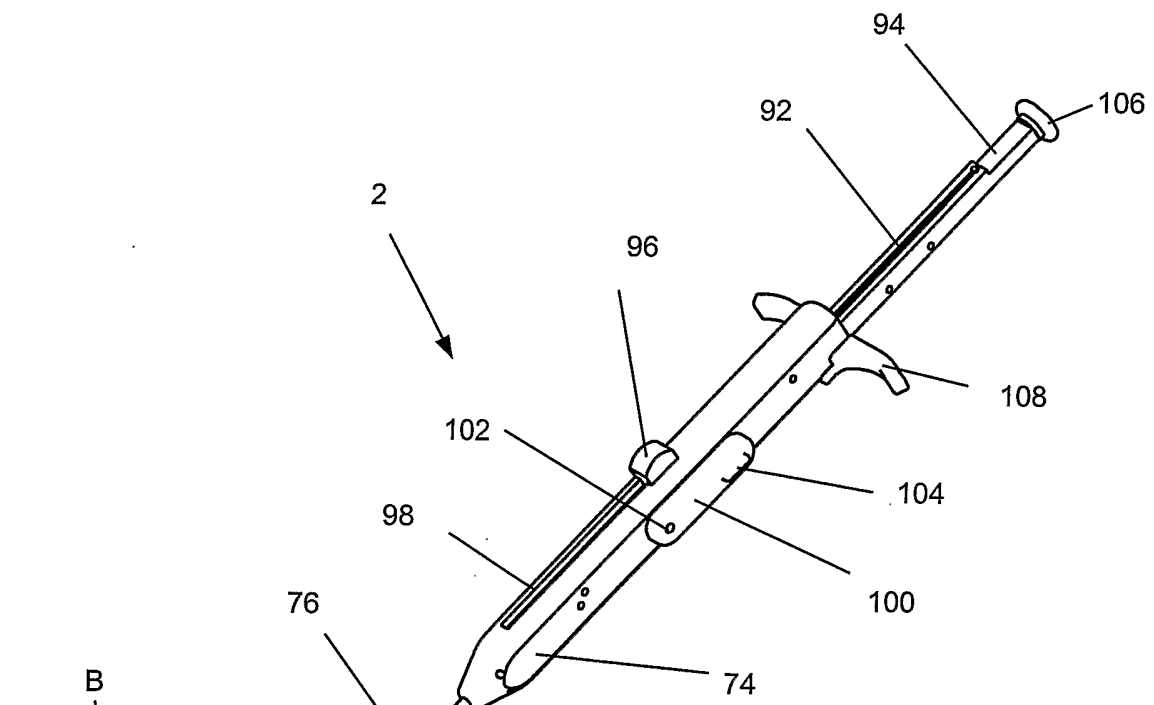


Fig. 12

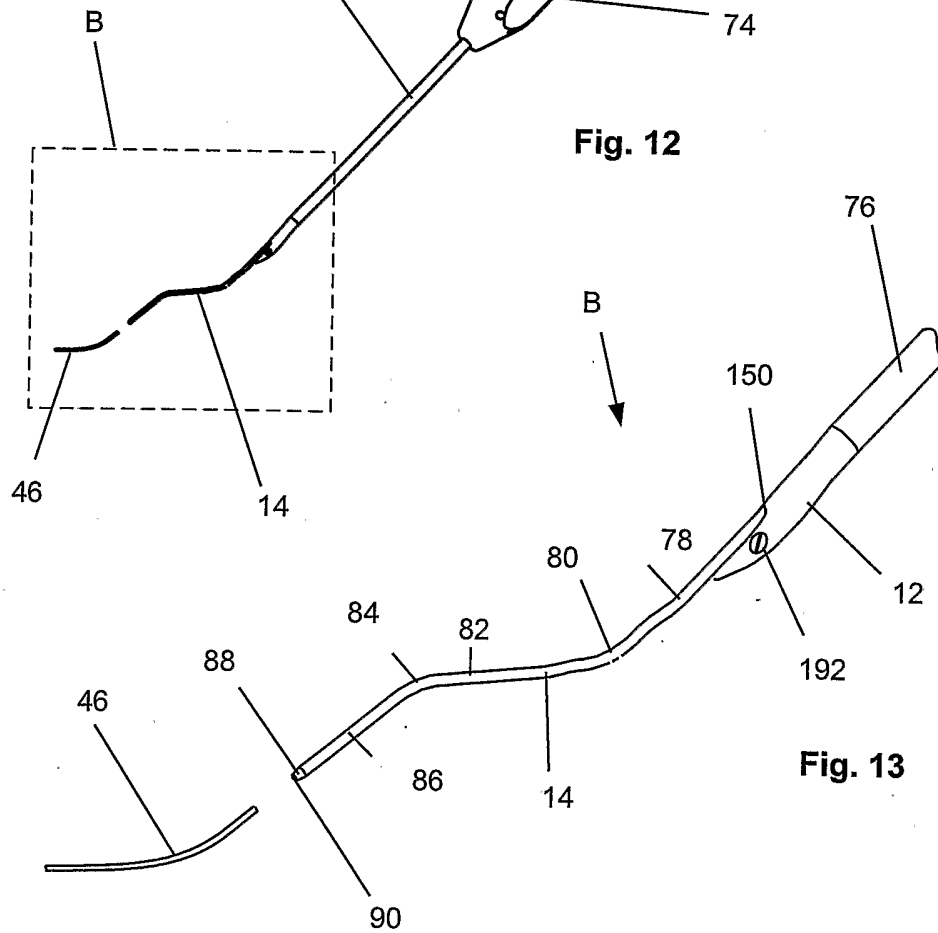
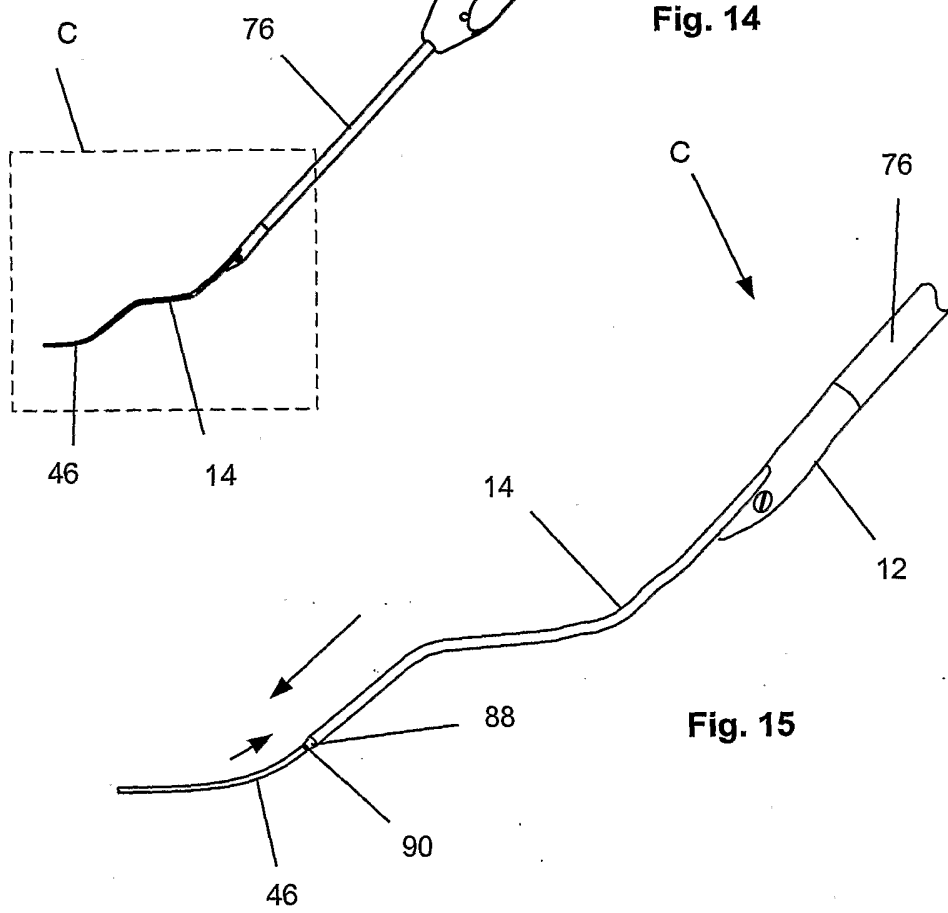
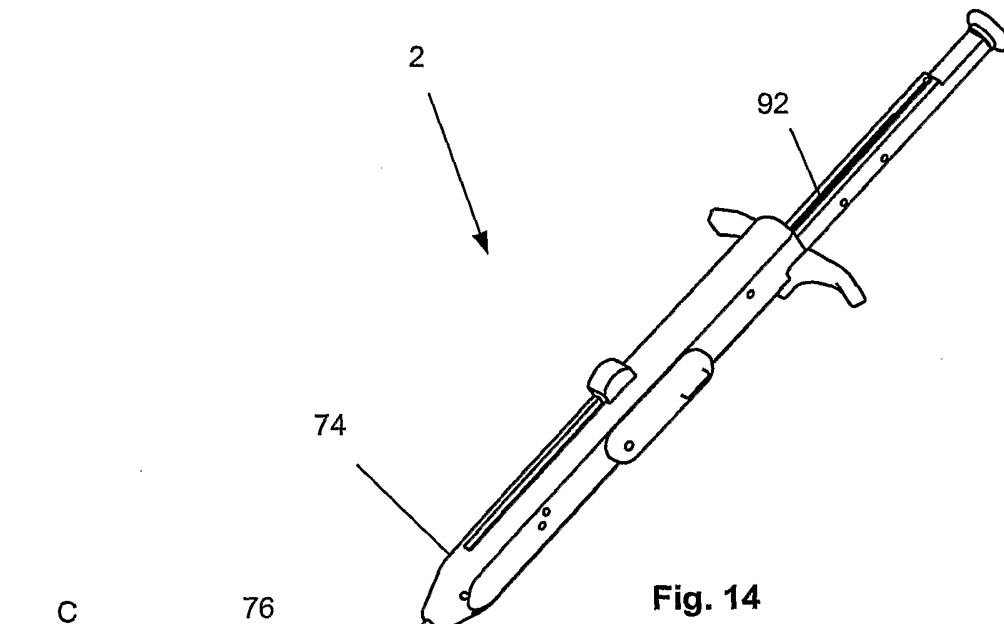


Fig. 13



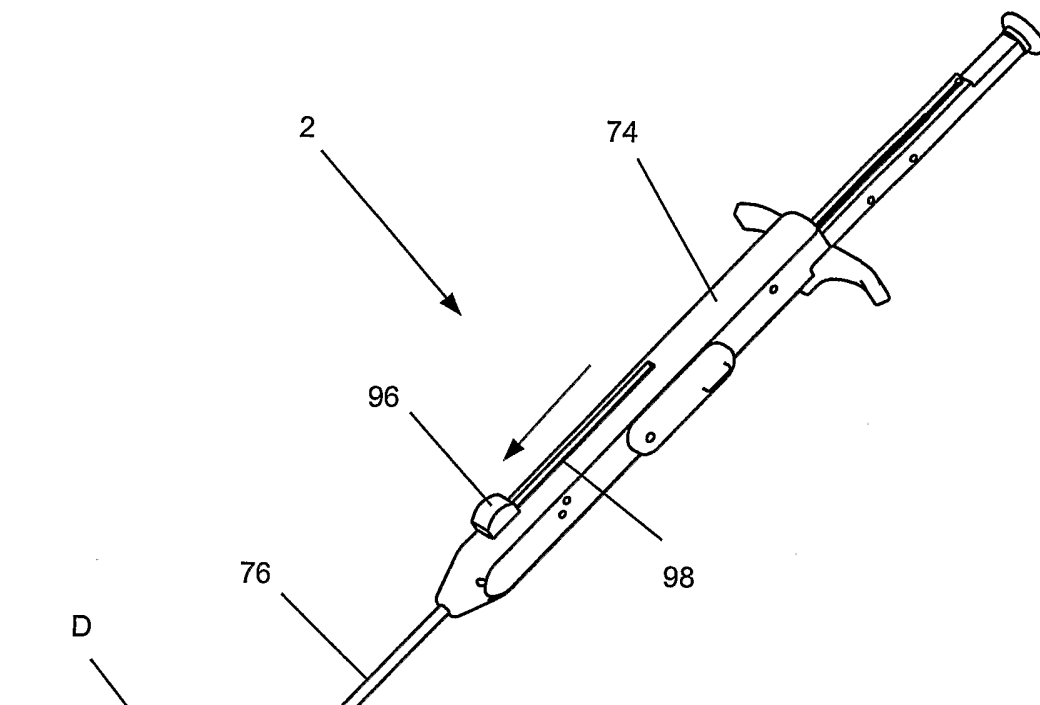


Fig. 16

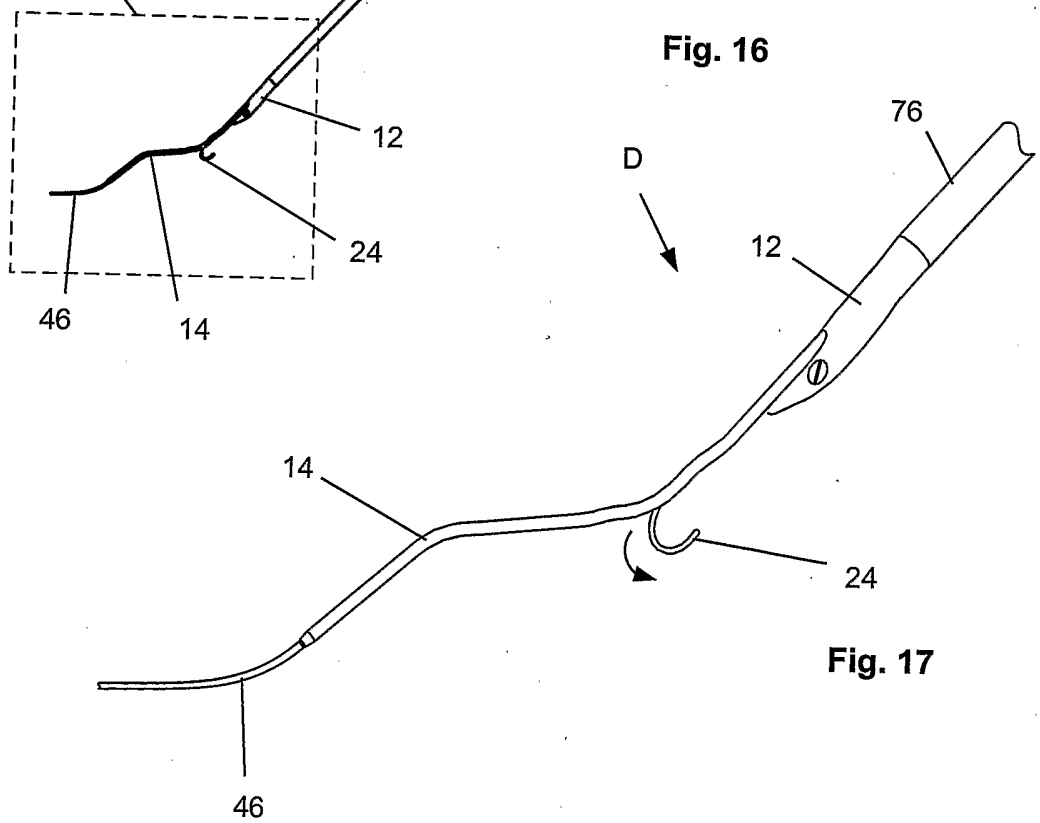


Fig. 17

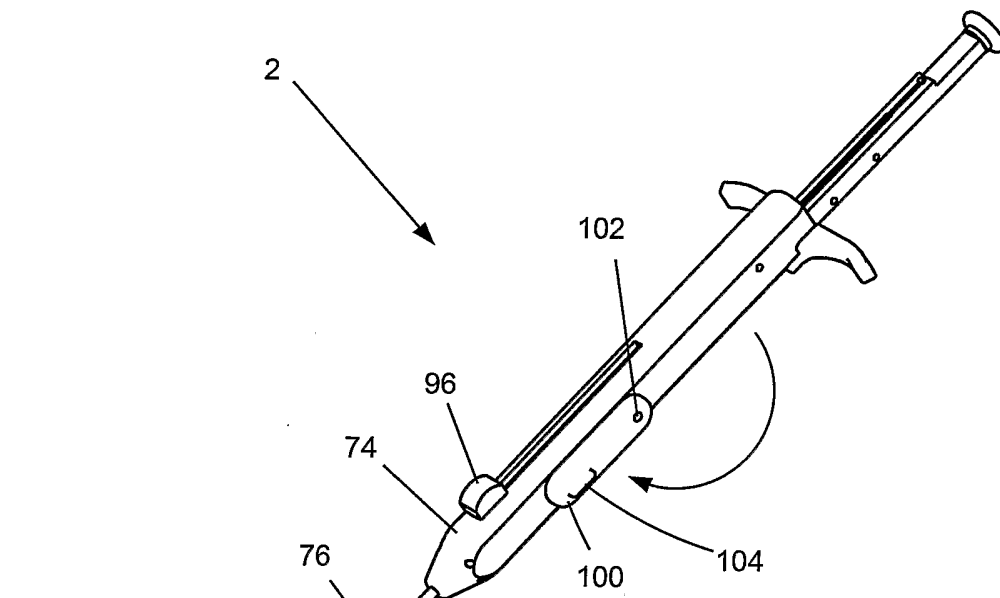


Fig. 18

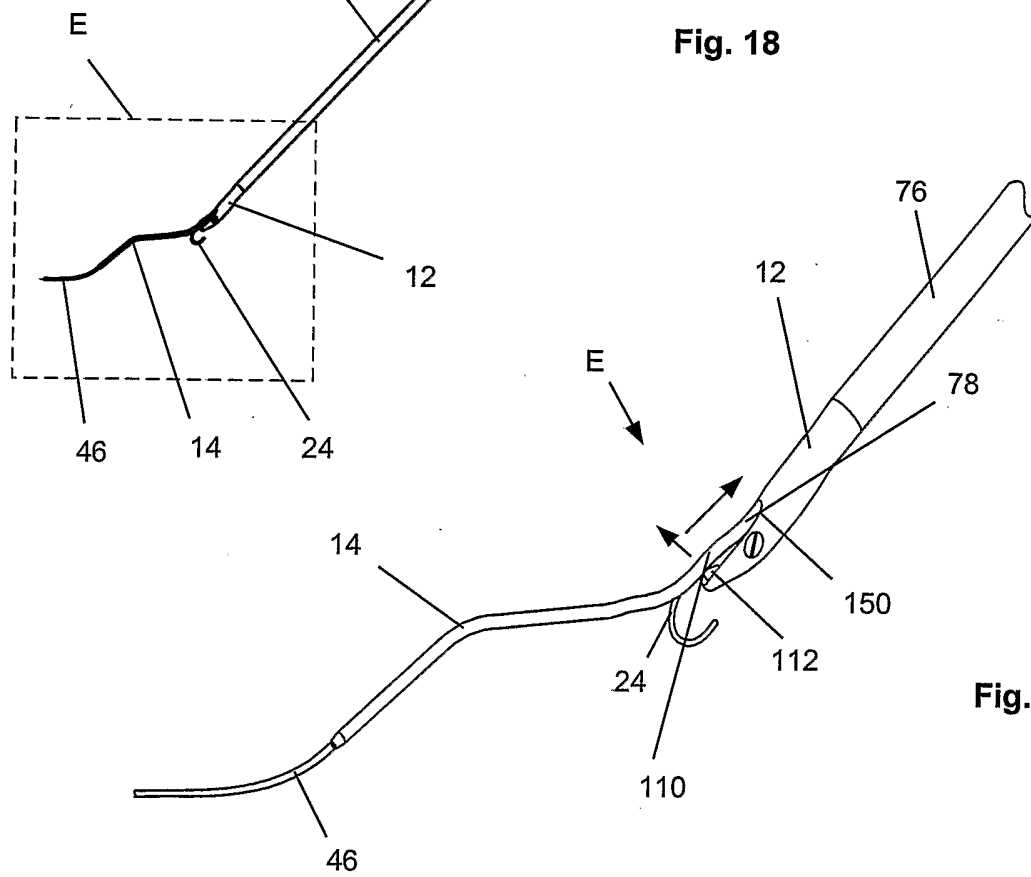
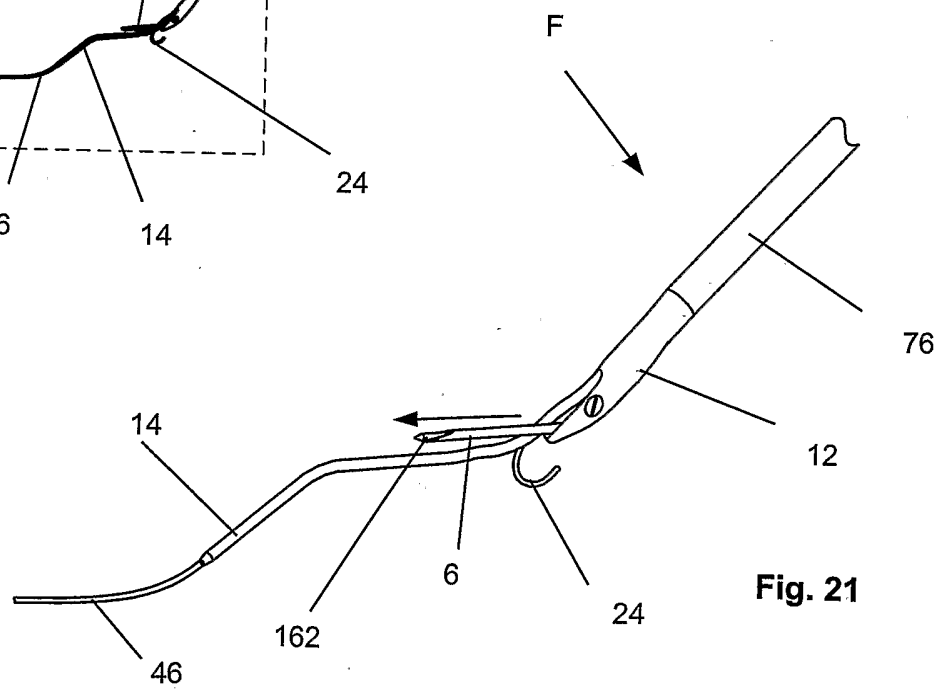
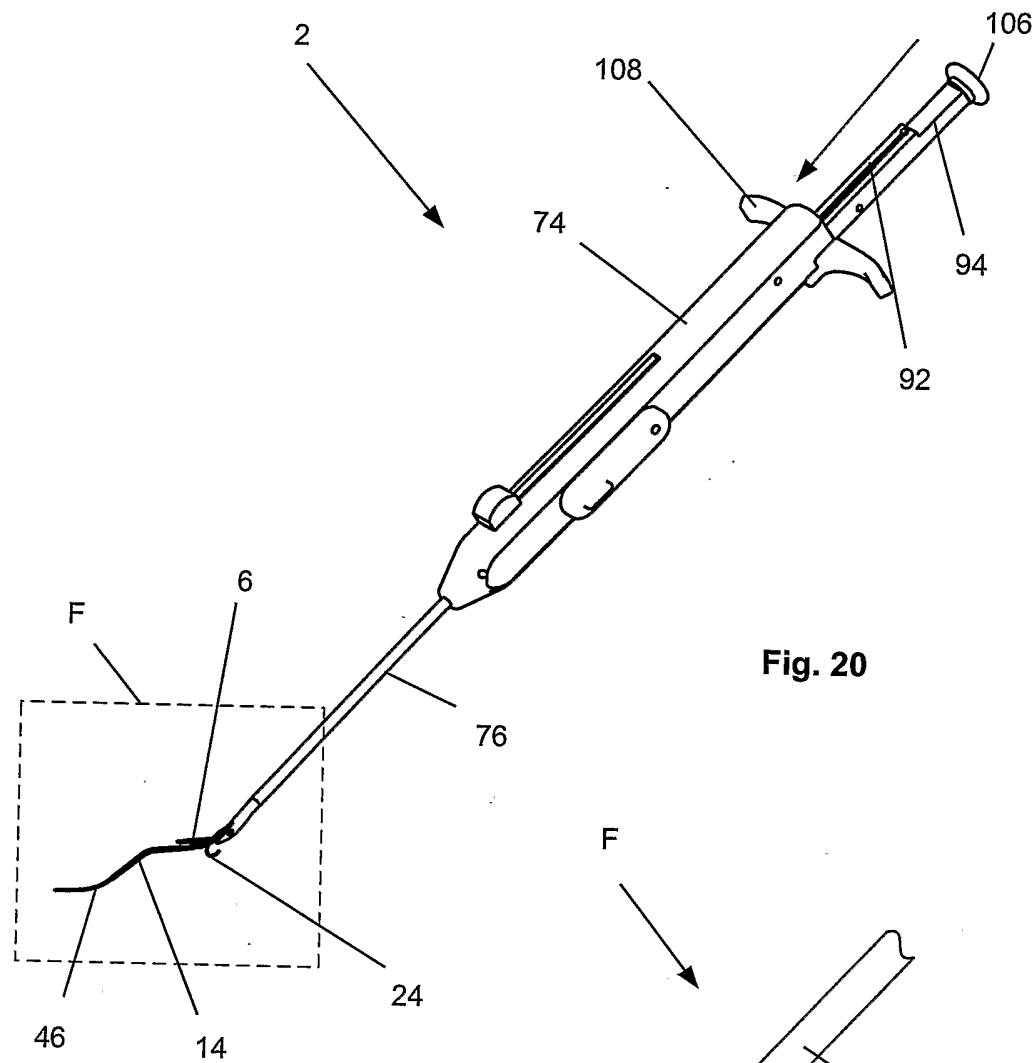


Fig. 19



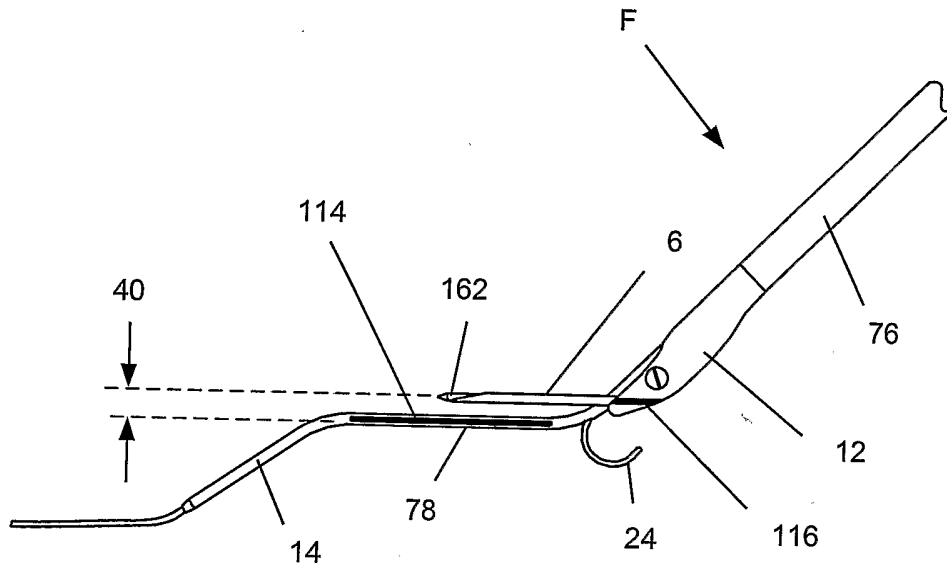


Fig. 22

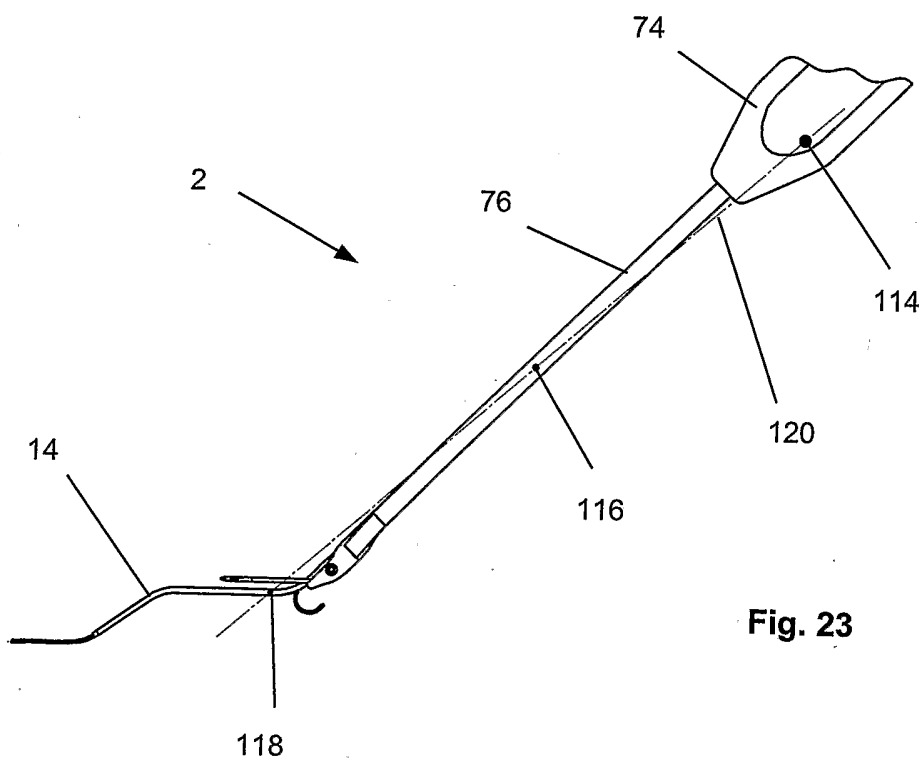
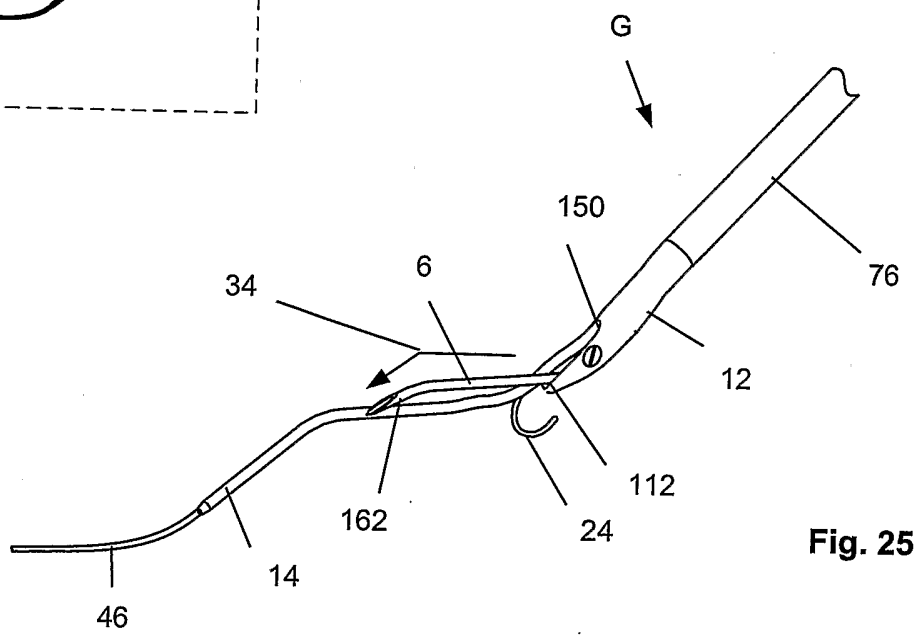
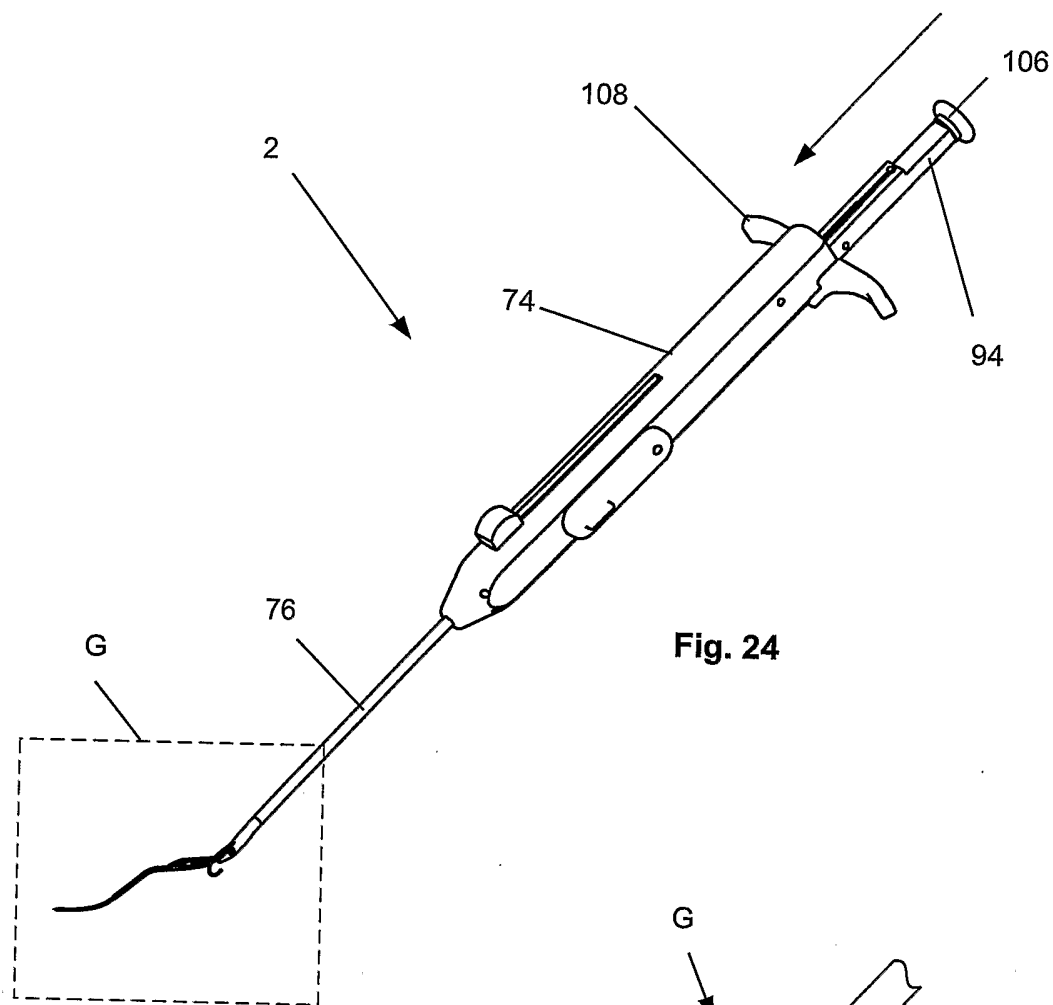
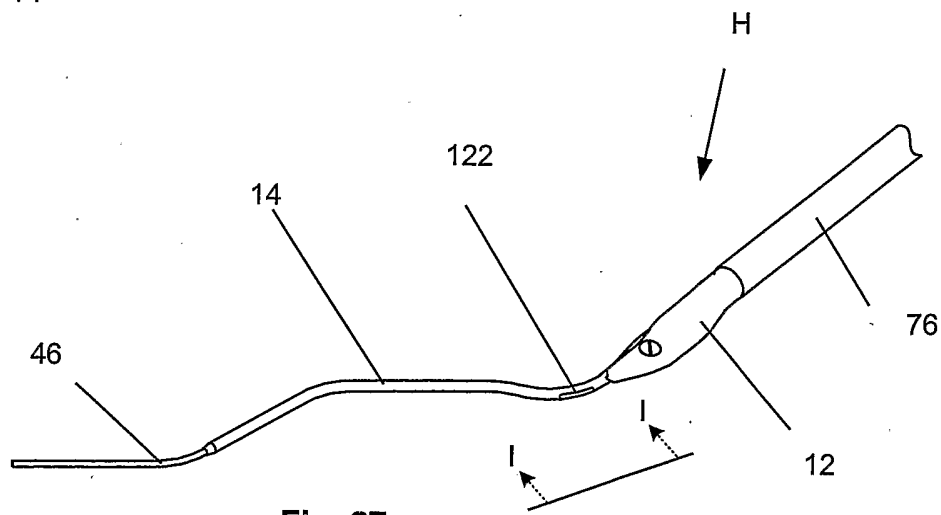
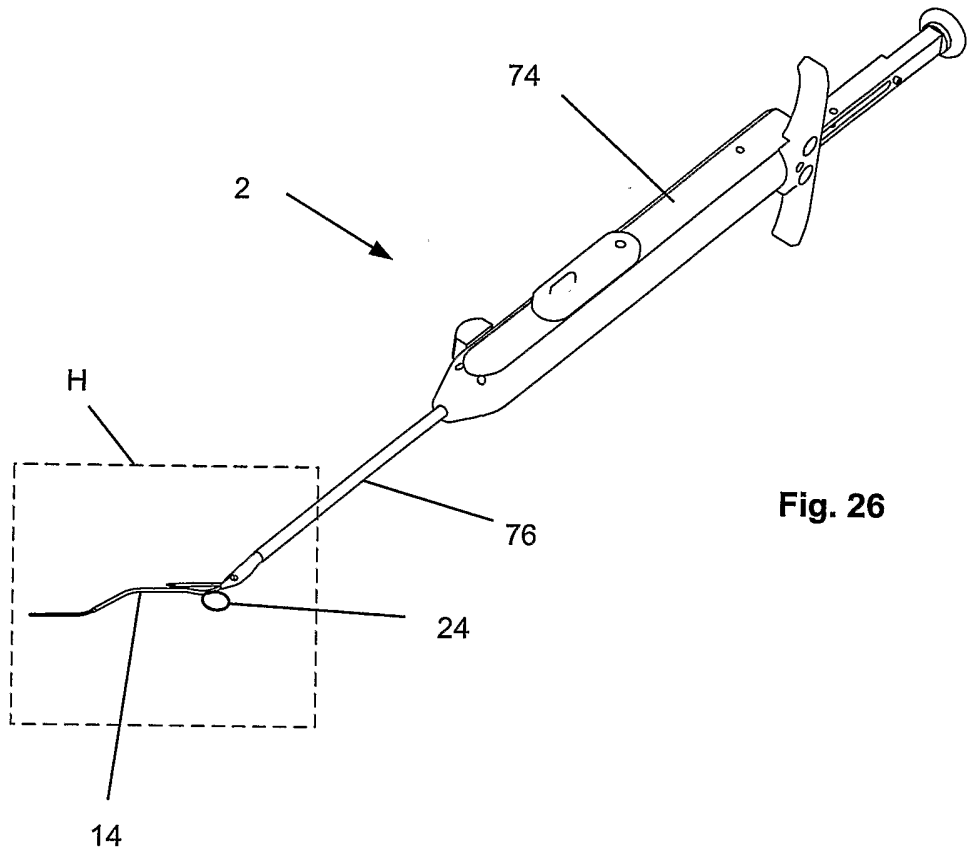


Fig. 23





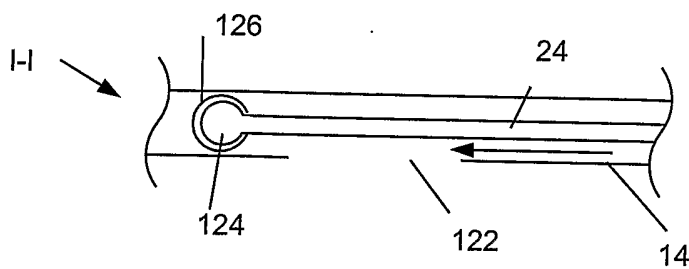


Fig. 28

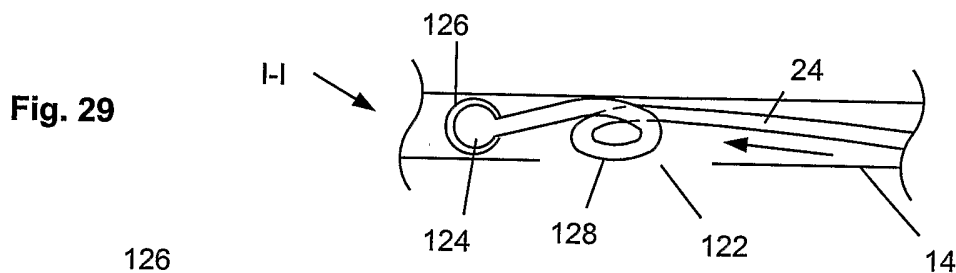


Fig. 29

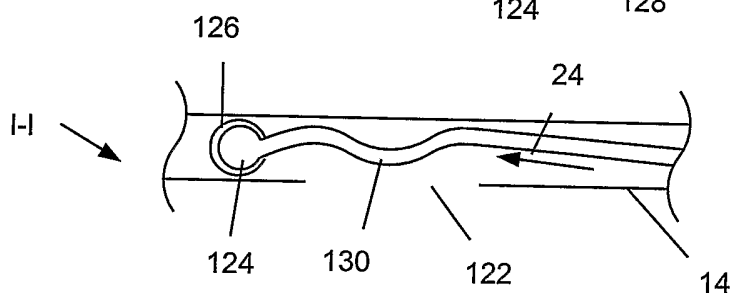


Fig. 30

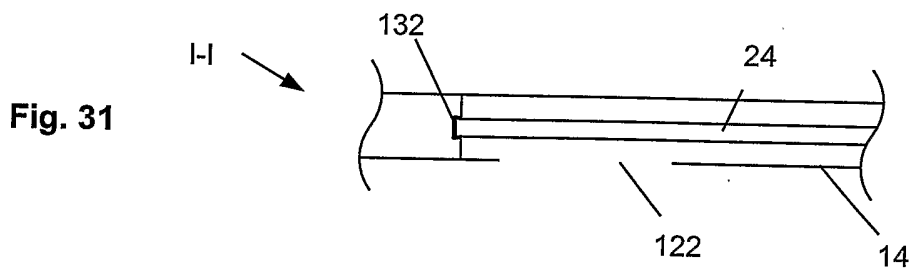


Fig. 31

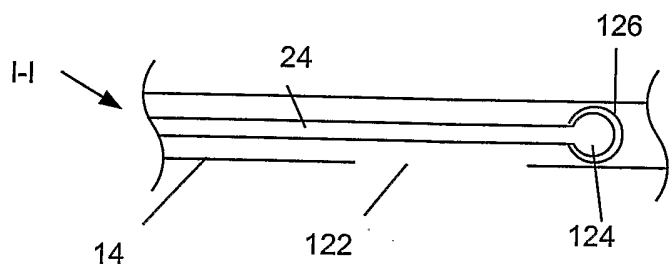


Fig. 32

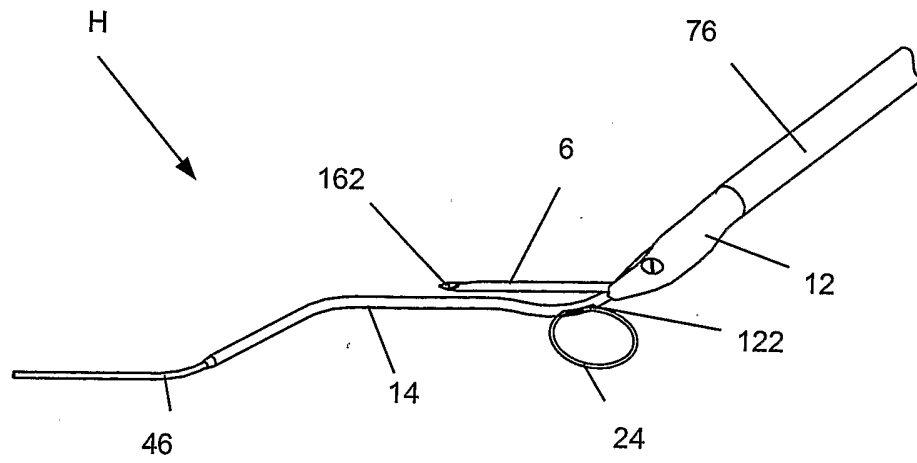


Fig. 33

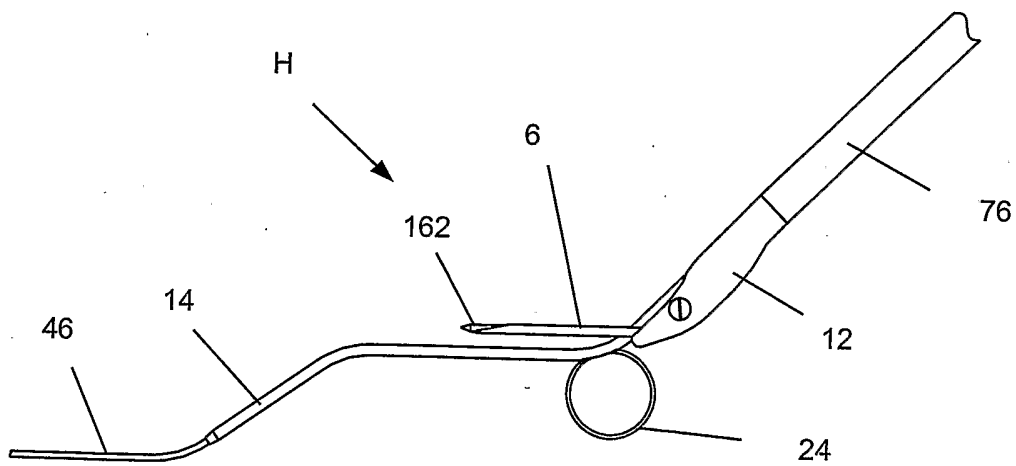
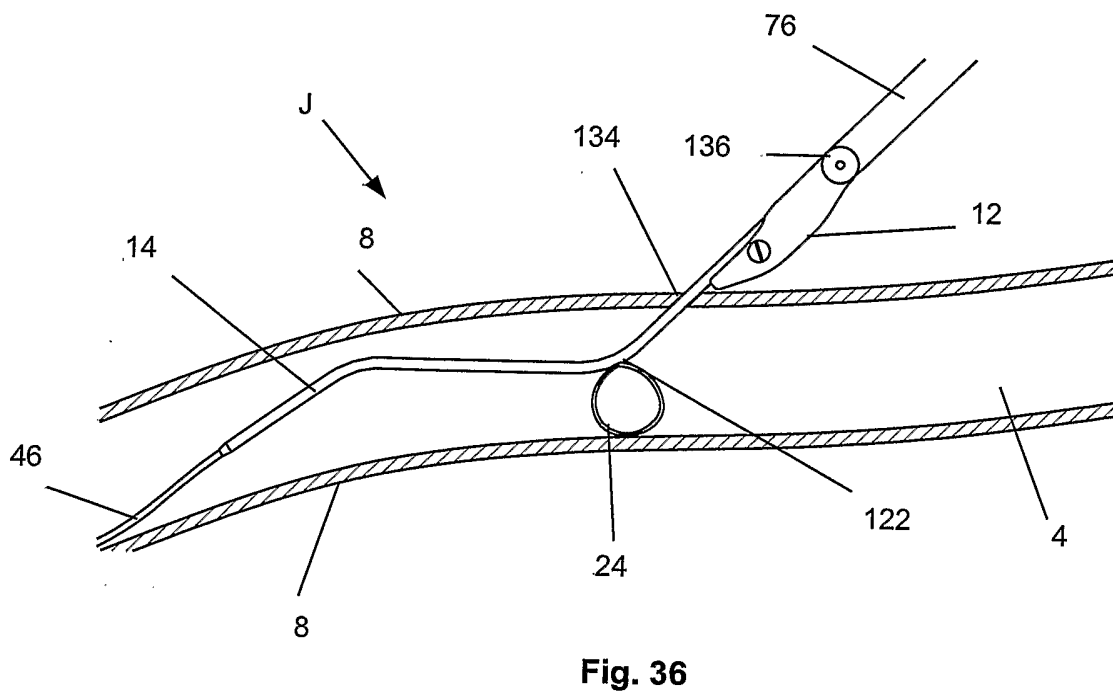
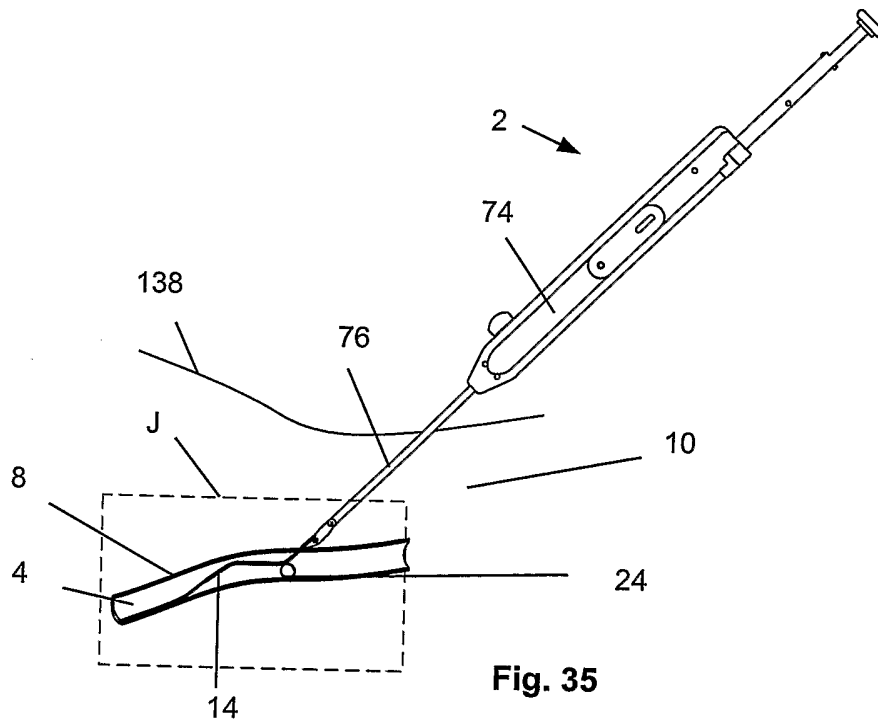


Fig. 34



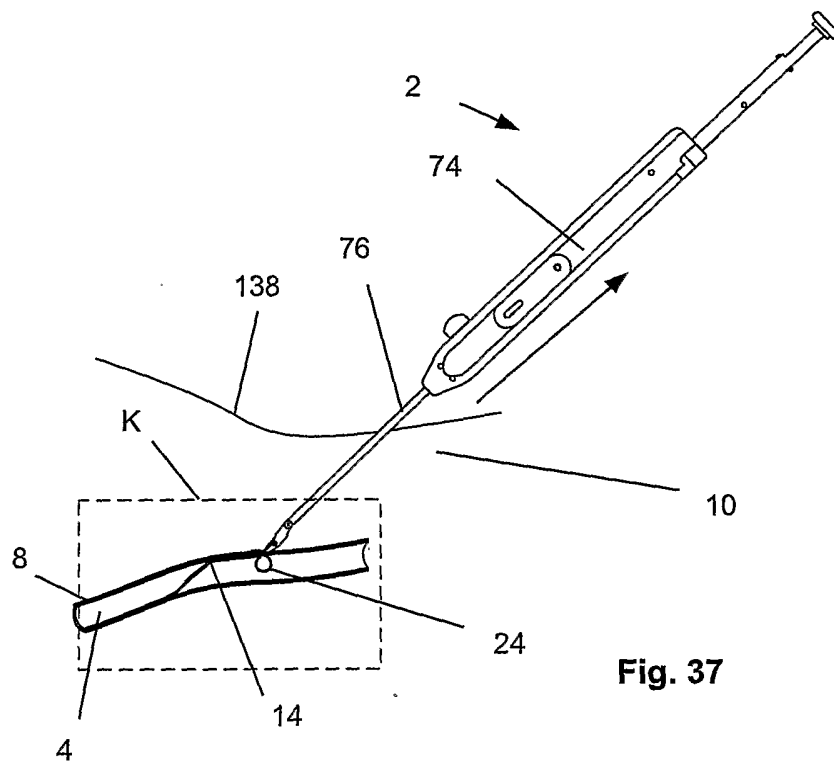


Fig. 37

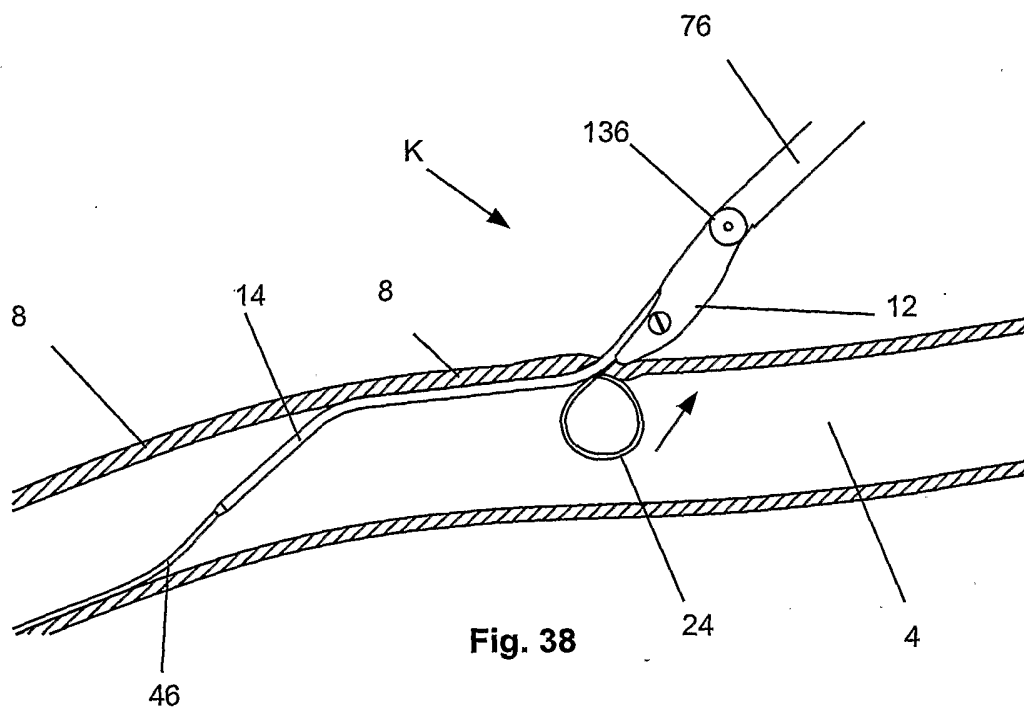


Fig. 38

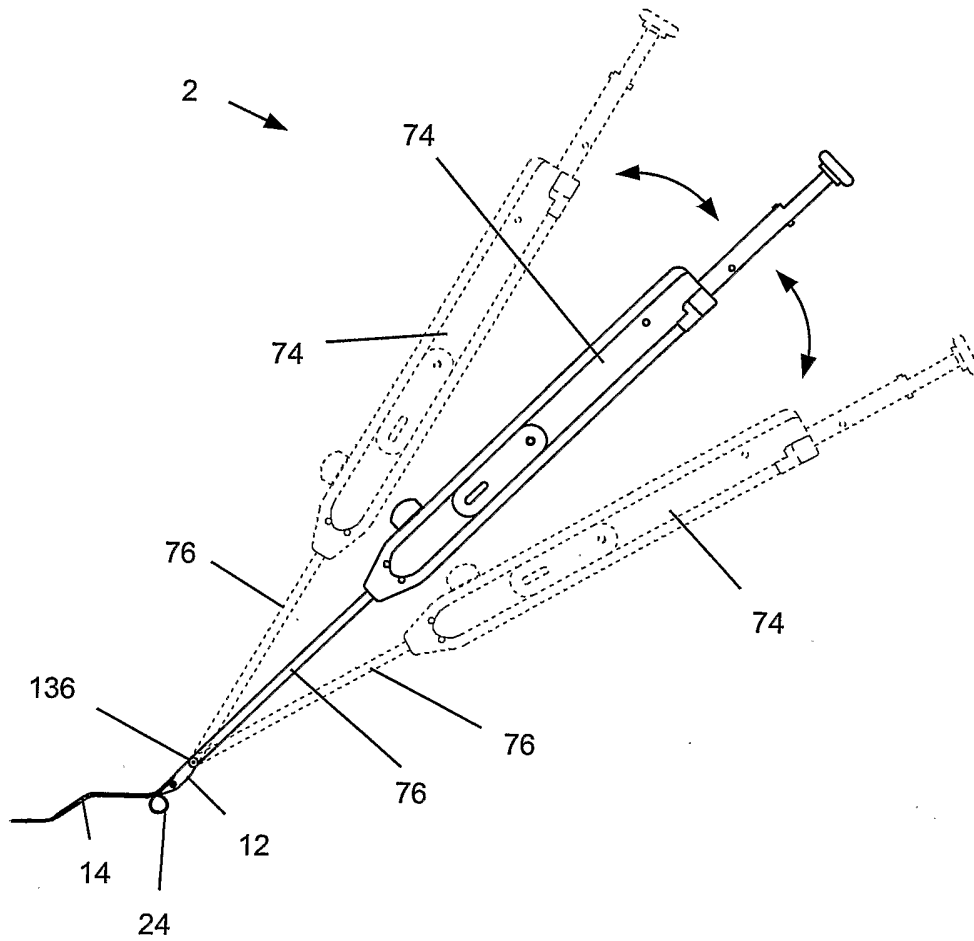


Fig. 39

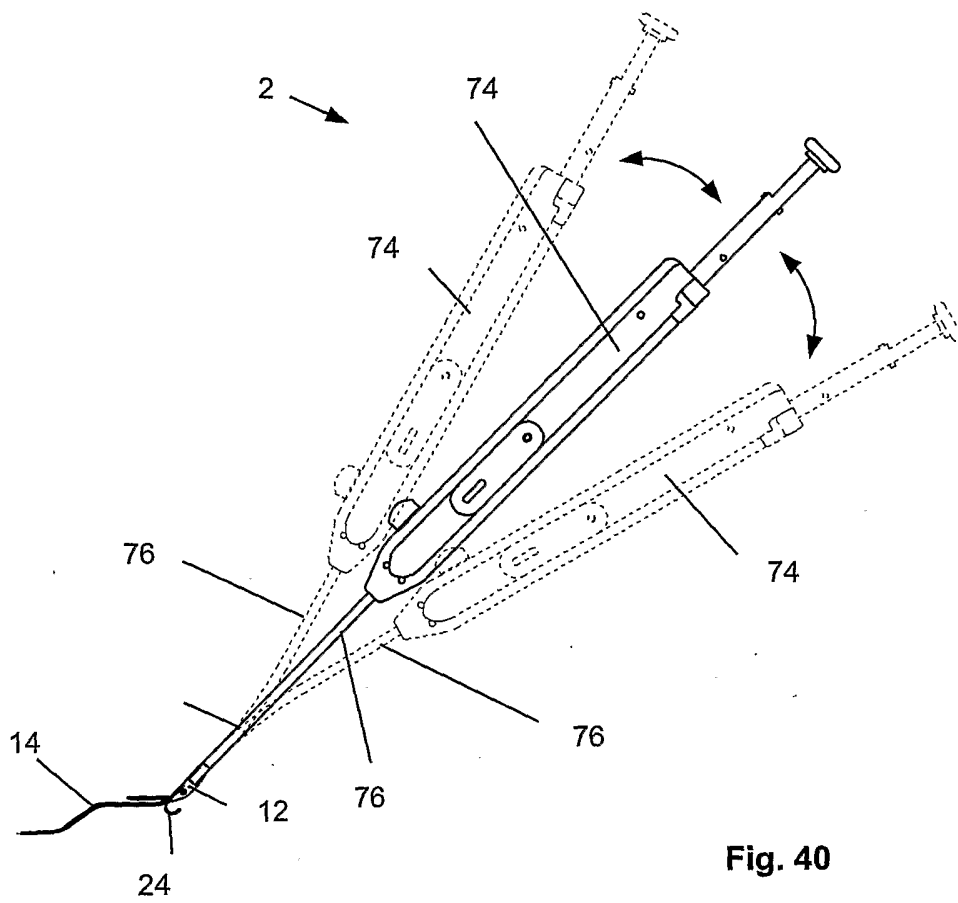


Fig. 40

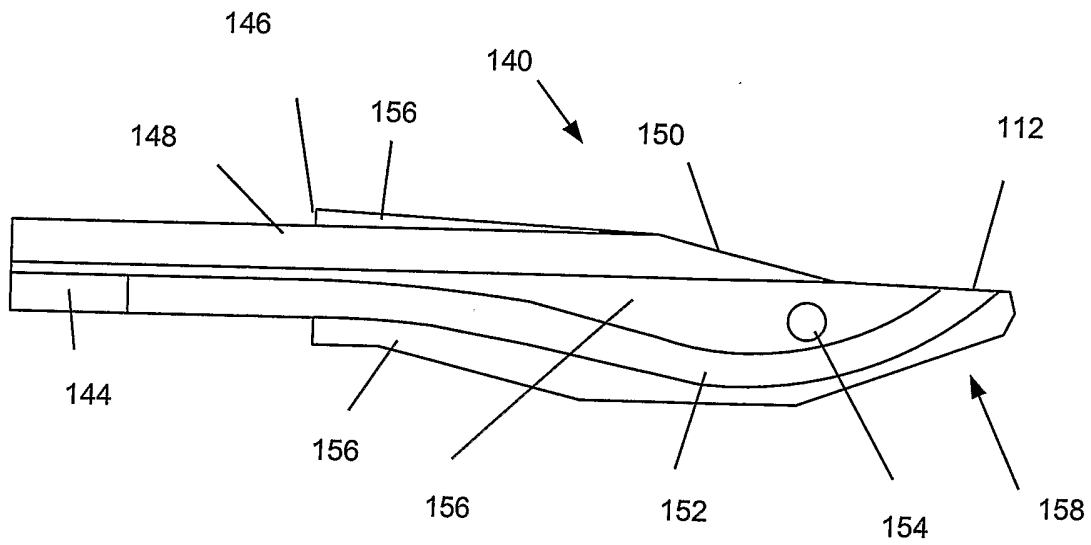


Fig. 41

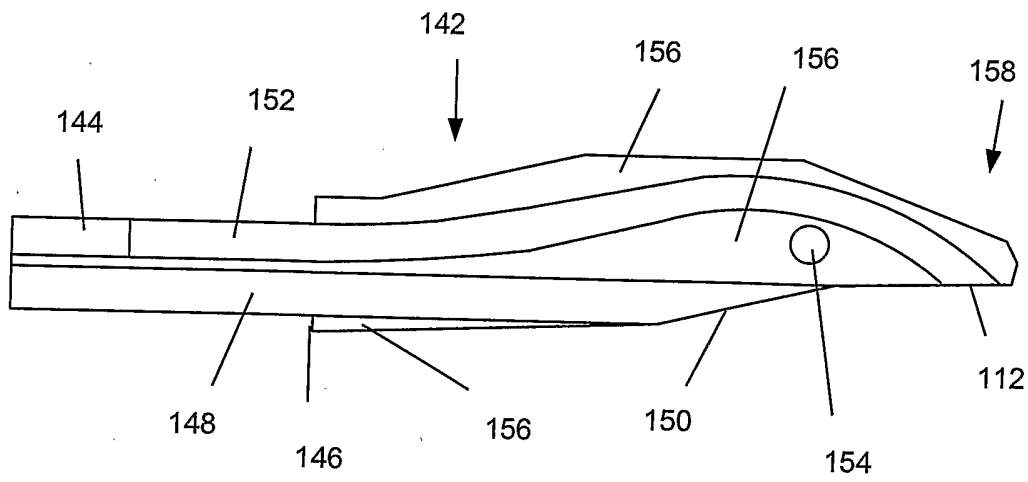
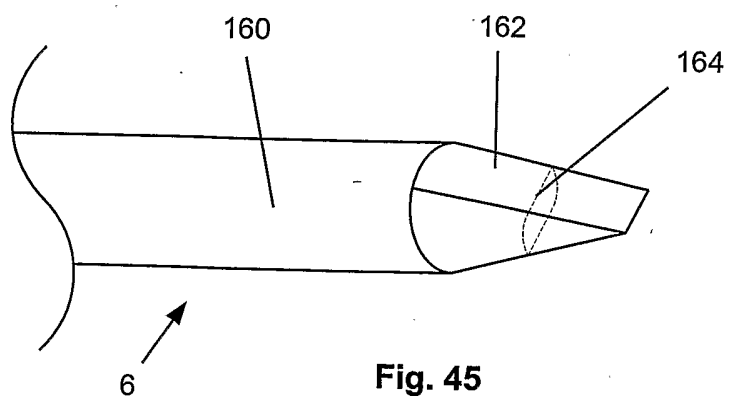
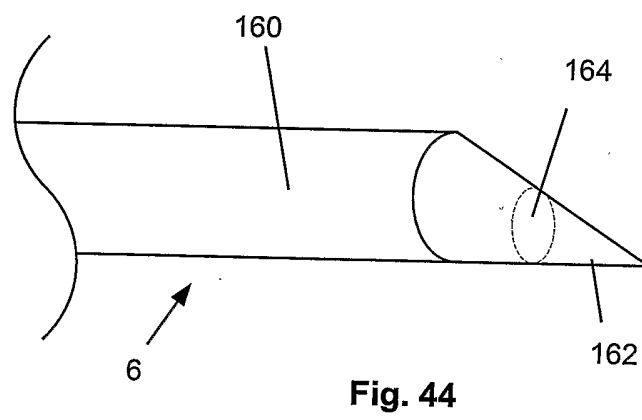
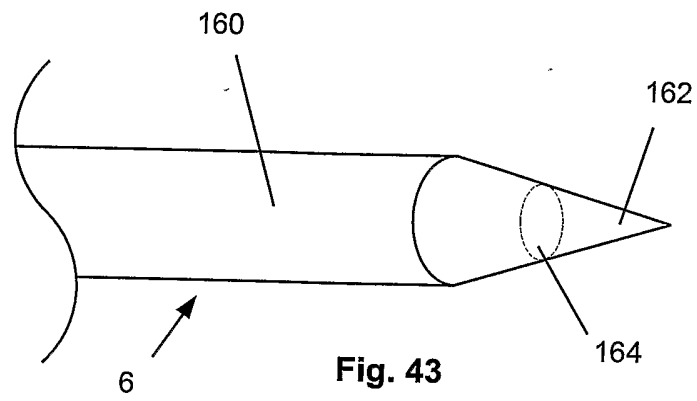
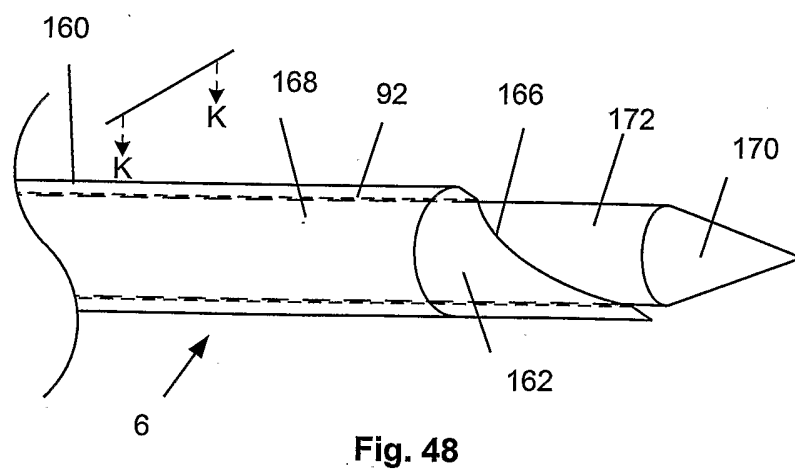
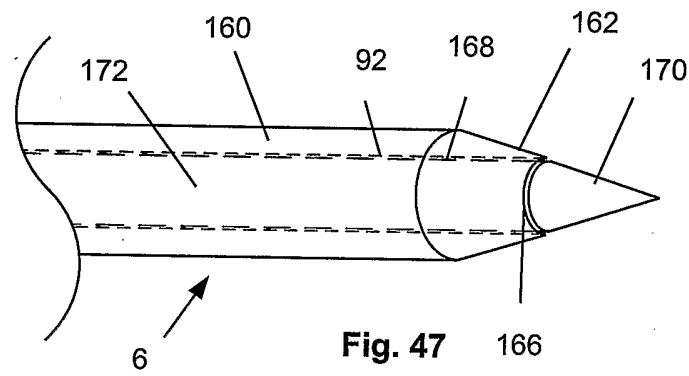
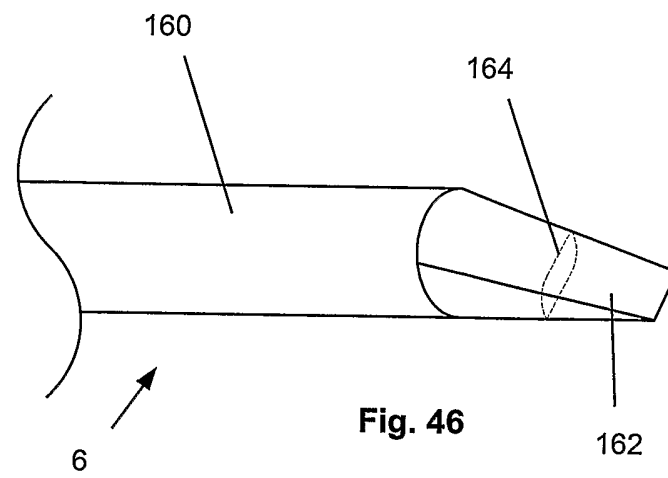


Fig. 42





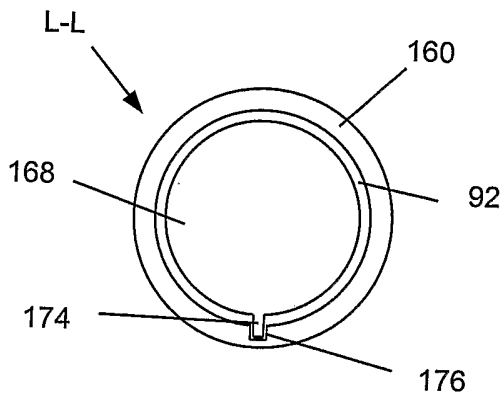


Fig. 49

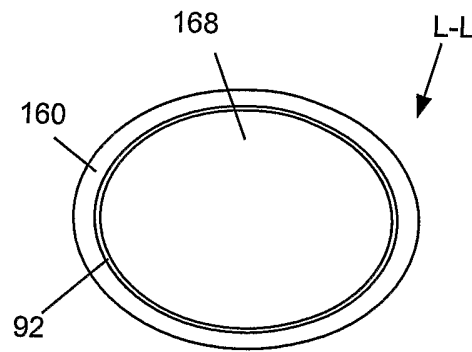


Fig. 50

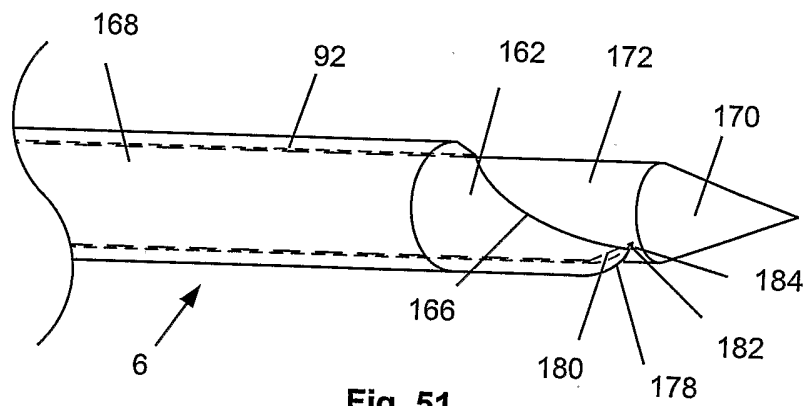


Fig. 51

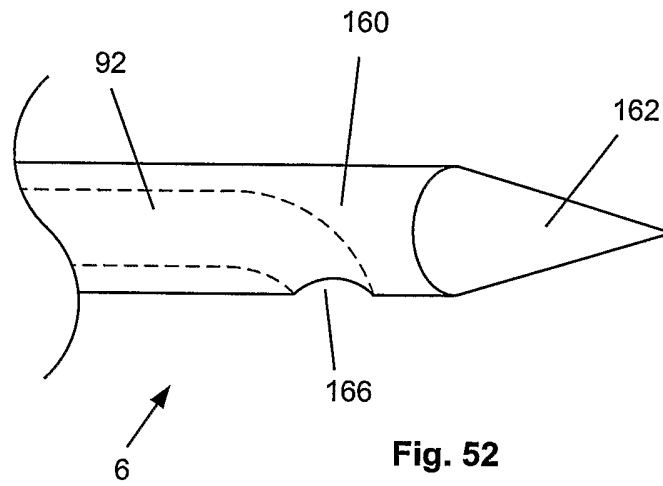


Fig. 52

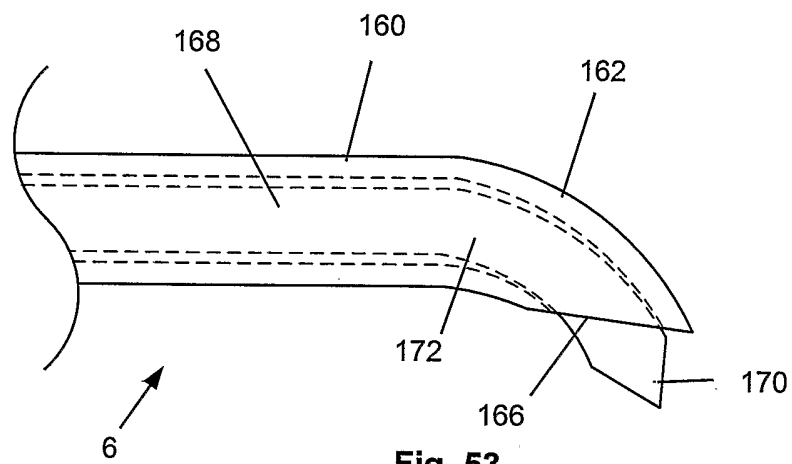


Fig. 53

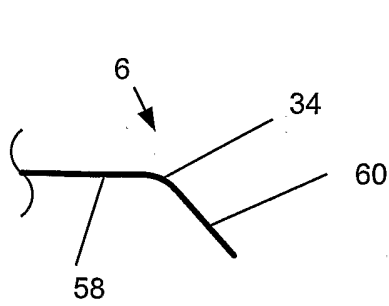


Fig. 54

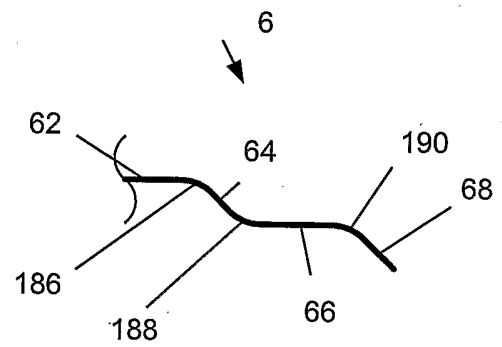


Fig. 55