




(86) Date de dépôt PCT/PCT Filing Date: 2015/03/03
(87) Date publication PCT/PCT Publication Date: 2015/09/11
(45) Date de délivrance/Issue Date: 2019/10/01
(85) Entrée phase nationale/National Entry: 2016/08/31
(86) N° demande PCT/PCT Application No.: CA 2015/050158
(87) N° publication PCT/PCT Publication No.: 2015/131278
(30) Priorités/Priorities: 2014/03/04 (US61/947,776);
2014/11/25 (US62/084,292)

(51) Cl.Int./Int.Cl. *G02B 27/00* (2006.01),
A61B 1/06 (2006.01), *G02B 1/00* (2006.01),
H04N 7/015 (2006.01)
(72) Inventeur/Inventor:
MOORE, FREDERICK ALLEN, CA
(73) Propriétaire/Owner:
NOVADAQ TECHNOLOGIES ULC, CA
(74) Agent: GOWLING WLG (CANADA) LLP

(54) Titre : SYSTEME DE LENTILLE DE RELAIS POUR IMAGERIE A LARGE BANDE
(54) Title: RELAY LENS SYSTEM FOR BROADBAND IMAGING

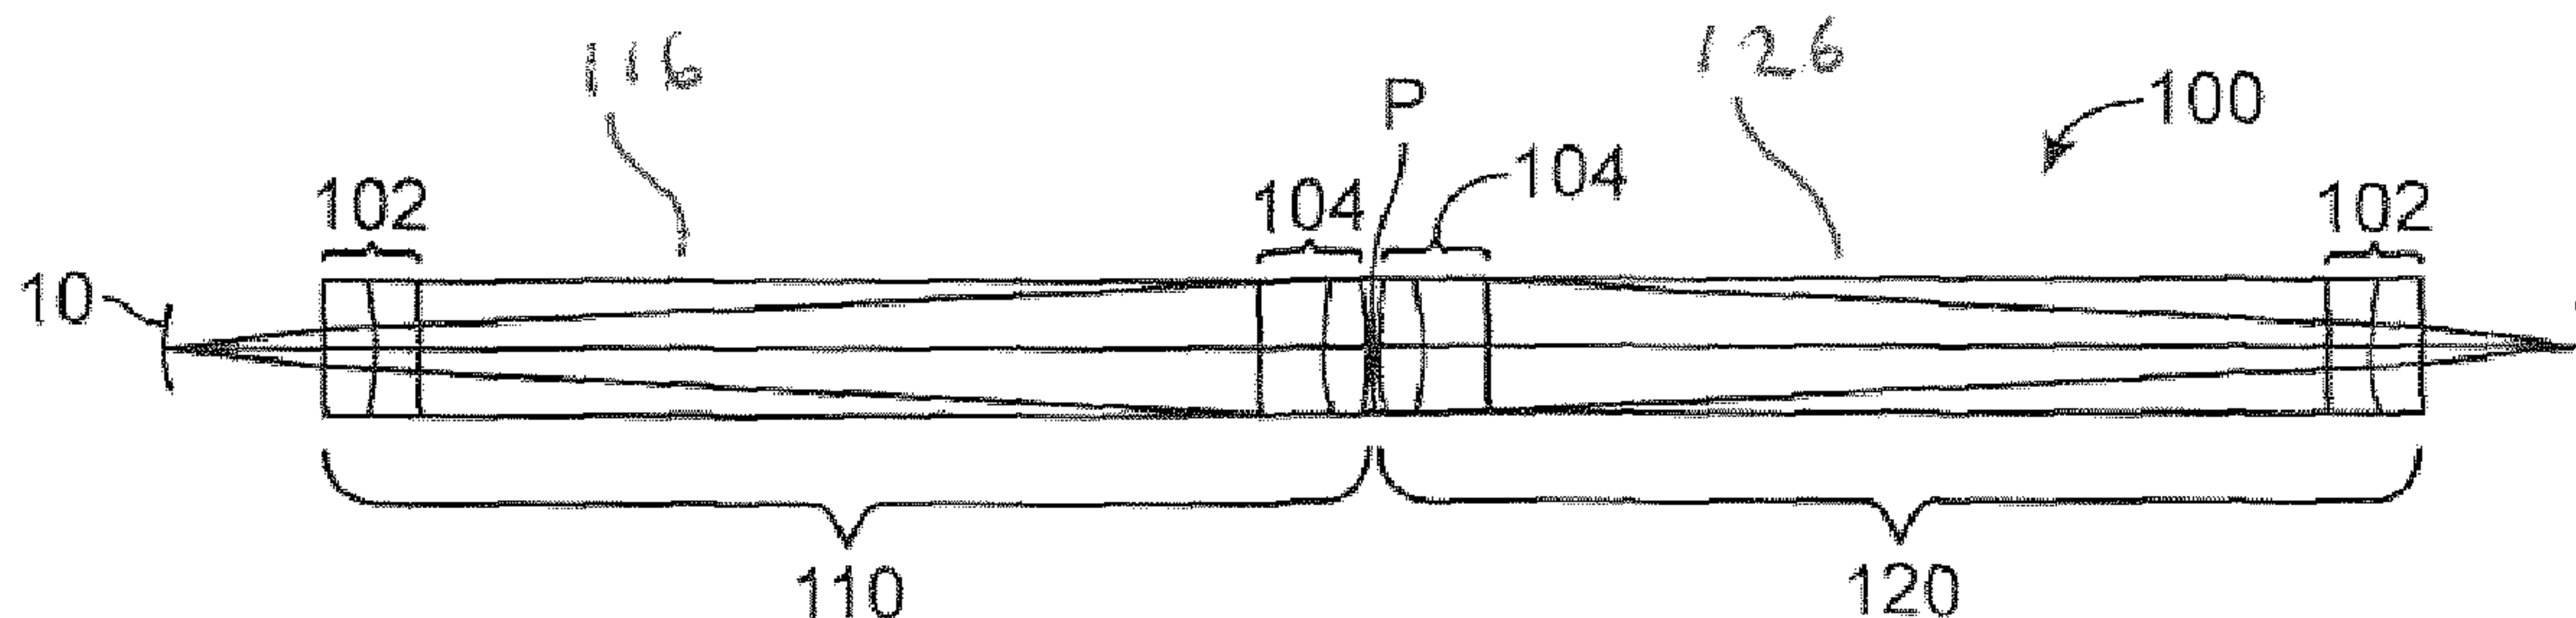

(57) **Abrégé/Abstract:**

An optical system is provided including a first relay rod of a first material, a second relay rod of a second material, different from the first material, and a lens between the first and second relay rods.

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
11 September 2015 (11.09.2015)

WIPO | PCT

(10) International Publication Number
WO 2015/131278 A1

(51) International Patent Classification:

G02B 27/00 (2006.01) *G02B 1/00* (2006.01)
A61B 1/06 (2006.01) *H04N 7/015* (2006.01)

(21) International Application Number:

PCT/CA2015/050158

(22) International Filing Date:

3 March 2015 (03.03.2015)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

61/947,776 4 March 2014 (04.03.2014) US
62/084,292 25 November 2014 (25.11.2014) US

(71) Applicant: **NOVADAQ TECHNOLOGIES INC.**

[CA/CA]; 5090 Explorer Drive, Suite 202, Mississauga,
Ontario L4W 4T9 (CA).

(72) Inventor: **MOORE, Allen;** 2277 West Second Avenue,
Suite 303, Vancouver, British Columbia V6K 1H8 (CA).(74) Agents: **SIM, Lisa** et al.; Gowling Lafleur Henderson
LLP, Suite 2300, 550 Burrard Street, Vancouver, British
Columbia V6C 2B5 (CA).

(81) Designated States (unless otherwise indicated, for every
kind of national protection available): AE, AG, AL, AM,
AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY,
BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM,
DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,
HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR,
KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, ME, MG,
MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM,
PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC,
SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every
kind of regional protection available): ARIPO (BW, GH,
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, ST, SZ,
TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU,
TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE,
DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU,
LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK,
SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ,
GW, KM, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))

(54) Title: RELAY LENS SYSTEM FOR BROADBAND IMAGING

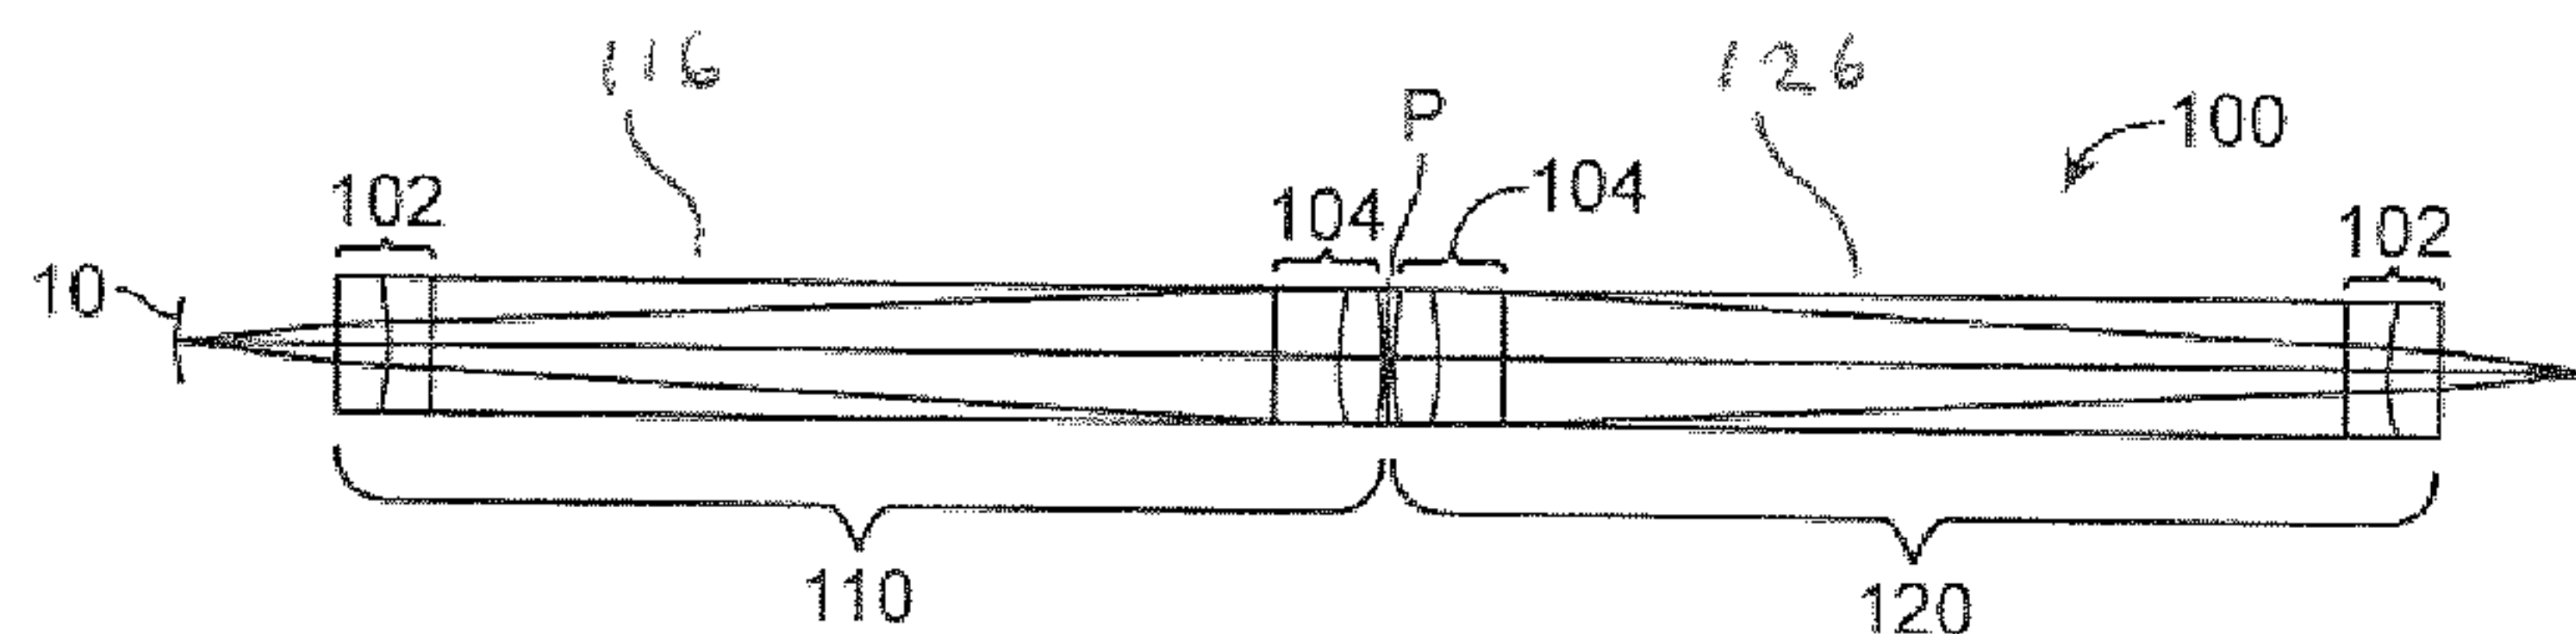


FIG. 1A

(57) Abstract: An optical system is provided including a first relay rod of a first material, a second relay rod of a second material, different from the first material, and a lens between the first and second relay rods.

RELAY LENS SYSTEM FOR BROADBAND IMAGING

5

TECHNICAL FIELD

The present disclosure relates generally to the field of optical lens systems. More
10 specifically, the disclosure relates to rod-type relay lens systems for use in
broadband imaging.

BACKGROUND

Medical endoscopes are used to view internal body organs and tissue through small
15 openings created in and through the body wall or skin or by way of existing openings
or orifices. For example, fluorescence endoscopy is an endoscopic examination
method in which fluorescent dye is administered to patients and excited with light
having a specific excitation wavelength. The excited fluorescent dye emits light of a
specific emission wavelength, which is longer than the excitation wavelength, so that
20 visualization of tissue and/or vessels containing the dye can be enhanced relative to
conventional white-light endoscopy.

SUMMARY

One or more embodiments are directed to an optical system, including a first relay
25 rod of a first material, a second relay rod of a second material, different from the first
material, and a lens between the first and second relay rods.

- 2 -

The first and second materials may be selected to reduce the wavefront error across the field of view of the optical system as compared with using a same material for both the first and second relay rods. The first and second relay rods may have no optical power. The first and second relay rods may have no optically powered surfaces.

The first and second relay rods may be geometrically symmetric to one another relative to a pupil or conjugate pupil of the optical system. The lens may include a first relay objective and a second relay objective. The first and second relay objectives may have a same design and material. A pupil region of the system may be in air.

The optical system may include a third relay rod of a third material, a fourth relay rod of a fourth material, the fourth material being different from the third material; and a lens between the third and fourth relay rods. The first and third materials are the same and the second and fourth materials may be the same.

The optical system may include a detector to detect light from 460 nm to 850 nm.

The optical system may be in an endoscope.

One or more embodiments are directed to a kit including a first relay rod of a first material, a second relay rod of a second material, different from the first material, and a lens to be inserted between the first and second relay rods.

The lens may include a first relay objective and a second relay objective. The first and second relay objectives have a same design and material.

One or more embodiments are directed to a method of compensating for dispersion in a relay lens system, the method including providing a first relay rod of a first material, providing a second relay rod of a second material, different from the first material, and providing a lens between the first and second relay rods.

5

One or more embodiments are directed to use of an imaging agent and the optical system according to the various embodiments in medical imaging of a tissue of a subject. One or more embodiments are directed to use of the endoscope according to the various embodiments in medical imaging of a tissue of a subject. One or more embodiments are directed to use of method of compensating for dispersion in a relay lens system according to the various embodiments in medical imaging of a tissue of a subject.

In one or more embodiments, the imaging agent may be or comprises a fluorescence imaging agent such as, for example, indocyanine green (ICG). ICG in combination with the optical system, endoscope and methods according to the various embodiments may be used in a diagnosis of tissue of a subject. The diagnosis may be based on medical imaging including fluorescence imaging.

One or more embodiments are directed to a kit comprising an imaging agent, a first relay rod of a first material, a second relay rod of a second material, different from the first material; and a lens to be inserted between the first and second relay rods. The imaging agent in the kit may be or comprises a fluorescence imaging agent such as, for example, ICG.

In one or more embodiments, the medical imaging of the tissue of the subject may comprise assessment of the tissue, diagnosis of the tissue, or a combination thereof. The tissue may form a body structure or a portion thereof. The medical imaging may be performed in the visible region, near infrared region, or a combination thereof.

5

BRIEF DESCRIPTION OF THE DRAWINGS

Features will become apparent to those of skill in the art by describing in detail exemplary embodiments with reference to the attached drawings in which:

- 10 FIGS. 1A and 1B illustrate a relay pair according to an embodiment;
FIG. 1C illustrates a plurality of relay pairs according to an embodiment;
FIG. 2 illustrates how index and Abbe values interplay through a relay set;
FIG. 3 is a graph of refractive index versus wavelength for exemplary glass types;
FIG. 4 is a graph illustrating partial dispersion versus inverse dispersion for various
15 glass types;
FIG. 5 is a graph illustrating refractive index versus Abbe number for exemplary
glasses; and
FIGS. 6A to 6C illustrate plots of MTF versus spatial frequency for comparative
examples and an example according to an embodiment.

20

DETAILED DESCRIPTION

Example embodiments will now be described more fully hereinafter with reference to the accompanying drawings; however, they may be embodied in different forms and should not be construed as limited to the embodiments set forth herein. Rather,
25 these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey exemplary implementations to those skilled in the

- 4 -

art. Generally, corresponding or similar reference numbers will be used, when possible, throughout the drawings to refer to the same or corresponding parts.

Optical design requirements for endoscopes have changed with the introduction of
5 new technologies, such as image sensors and solid state illumination. An endoscope
designed for visual use only may be optimized for F,d,C light, which spans the
region of 486 nm through to 656 nm. An endoscope designed for machine vision,
where a camera will display an image on a monitor, may operate with illumination
wavelengths extending further into the blue, for example to 460 nm. Additionally,
10 there is demand to visualize tissue and body structures in other waveband regimes
beyond that of visible bands, e.g., near infrared regions (700 nm to 900 nm) where
tissue is maximally transparent to light and where dyes such as Indocyanine Green
(ICG) fluoresce and are used as markers. Additionally, the resolution required of
endoscopes has increased with the introduction of high definition (HD) video image
15 sensors having smaller and more numerous pixels than earlier NTSC or PAL
formats. In both diagnostic and therapeutic procedures where endoscopes are used,
it is advantageous to provide guiding imagery and fluorescent markers. Accordingly,
high resolution imaging is desired in the visible bands as well as in longer
wavelength regions beyond that of human vision.

20

Imaging optical systems, including endoscopes, must be designed with the
operational wavelengths in mind. The refractive properties of materials are such that
light of different wavelengths will propagate along slightly different paths through
an optical system, and arrive at slightly different image planes. In order to ensure
25 that the image planes for different wavelengths are sufficiently close so as not to
degrade image quality, the design of the system must take into consideration these
refractive properties.

- 5 -

A system designed for use across a broadband of wavelengths, e.g., between 460 nm to 850 nm, may have one or more image sensors. If the system has two sensors, e.g., one for the visible region and one for the near infrared region, then the design of the system may consider separately the problems of image quality for the visible and image quality for the near infrared region, since each region will have its own corresponding sensor. If however, the system operates with a single image sensor, then the system must focus all light throughout its operational waveband onto one image plane. This latter condition is more difficult, but also offers more utility to the remainder of the design, as a single sensor may be used.

A system designed for broadband use, for example visible and near infrared, and designed for single sensor operation, requires tight control over chromatic aberrations, such as axial color. Light of different wavelengths focus at different distances from the optics. Axial color arises from dispersion, i.e., the variation of refractive index versus wavelength in refractive materials. Sensitivity to dispersion increases as the $f/\#$ is faster.

Therefore, one or more embodiments are directed to providing a relay lens system that offsets the effect of dispersion as light propagates through the system, as discussed in detail below.

According to an embodiment, there is provided an optical system comprising a first relay rod of a first material, a second relay rod of a second material, different from the first material, and a lens between the first and second relay rods. In an embodiment, the first and second materials are selected to reduce the wavefront error across the field of view of the optical system as compared with using a same material

- 6 -

for both the first and second relay rods. In other embodiments, the first and second relay rods have no optical power, or have no optically powered surfaces. In an embodiment, the first and second relay rods are geometrically symmetric to one another relative to a pupil or conjugate pupil of the optical system.

5

In yet another embodiment, the optical system may further comprise a third relay rod of a third material, a fourth relay rod of a fourth material, the fourth material being different from the third material, and a lens between the third and fourth relay rods.

In an embodiment, the first and third materials are the same and the second and
10 fourth materials are the same.

FIGS. **1A** and **1B** illustrate an exemplary relay pair **100** for a broadband system using a single detector. FIG. **1A** illustrates the on-axis beam and FIG. **1B** illustrates the off-axis beam. FIG. **1C** illustrates an odd number of relay pairs to produce an
15 upright image at a detector **200**. In particular, the image after an objective lens **10** is inverted, so any odd number of relay pairs, e.g., 1, 3, 5, 7, and so forth, will produce an upright image.

The relay pair includes a first relay rod lens assembly **110** and a second relay rod
20 lens assembly **120**. Each of the first and second relay rod lens assemblies **110**, **120** includes a rod **116**, **126**, respectively, and a plurality of bonded lenses selected to provide color correction from a lower limit, e.g., 460 nm, to an upper limit, e.g., 850 nm. In particular, the bonded lenses may include a relay field lens **102** and a relay objective **104**, here both shown as doublets.

25

The rods **116**, **126** are made of different materials that compensate for residual wavefront error in the relay pair **100** as illustrated in FIG. **2**. The diffraction-limited

- 7 -

relay pair in FIG. 2 illustrates refractive index symmetry about the pupil region P, and Abbe number asymmetry about the pupil region P.

The relay pair **100** operates with unit magnification. The bonded lenses of the relay
5 rod lens assemblies **110** and **120** are symmetric or mirrored about a pupil (or aperture
stop) **130** between the first and second relay rod assemblies **110**, **120**. In other
words, the relay field lenses **102** and the relay objectives **104** are the same, i.e., the
same material, the same prescription, and so forth, throughout the relay pair **100**.

10 Although a design is optimized based on wavefront error and MTF performance, and
although this process will offset some aberrations through constructive introduction
of other aberrations, it may be helpful to explore the problem in traditional terms,
such as may be found by considering the system in terms of Seidel errors. While
typical, symmetrical design of the relay pair will correct for odd Seidel aberrations,
15 e.g., coma, distortion, lateral chromatic aberration, and so forth, even Seidel
aberrations, e.g., spherical, astigmatism, field curvature, axial chromatic, and so
forth, are not corrected by such symmetry. Axial chromatic aberration is of
particular concern as the wavelength bandwidth increases, while the image plane
remains constrained to a single detector. Additional lenses or different lenses on
20 different sides of the relay pupil may be used to correct for the dispersion, but this
increases cost and complexity.

However, by using different materials for the relay rod in the first and second relay
rod lens assemblies **110**, **120** in accordance with an embodiment, the basic form of
25 the relay pair **100** may be maintained. In other words, since the material of the relay
rods introduce dispersion themselves, by selecting appropriate materials for the relay
rods **116**, **126** in the first and second relay rod lens assemblies **110**, **120**, the

- 8 -

dispersion over the relay pair **100** may be compensated, while otherwise using the same elements throughout the relay pair **100**. The relay rod carries no optical power, but instead is used to make the space between powered elements appear to have a shorter optical path distance, without using total internal reflection.

5

Thus, by treating the material of the relay rod as another degree of freedom, dispersion in the relay pair **100** may be altered, i.e., corrected, without modifying the basic form. The relay rod lens assemblies **110** and **120** will have nearly identical focal lengths in order to meet the required unit magnification. The first rod **116** and
10 the second rod **126** are symmetrical to one another relative to the pupil. However, as noted above, the first rod **116** is made of a first glass type and the second rod **126** is made of a second glass type. The second glass type is different from the first glass type. In design, the first glass type and the second glass type are selected to reduce residual wavefront error within the optical system. Otherwise, the pair of relay and
15 rod lens assembly is identically configured, e.g., identical lengths, identical lens elements, identical geometric form, and so forth, while using different rod materials.

Referring to FIG. **3**, it can be seen that for any wavelength, different materials have different local tangents (derivatives). Thus, glass materials not only exhibit different
20 aggregate dispersion (different inverse Abbe numbers) but also exhibit different partial dispersion, which is a measure of dispersion over a subset of the bandwidth. FIG. **4** illustrates how partial dispersion ($P_{g,F}$) varies with inverse dispersion (Abbe number or V_d) for SCHOTT®'s optical glass assortment.

25 Relay rod glass material is selected first for its transmission properties; a designer may build a design-specific list of materials ranked according to transmission, then draw upon the top candidates for their remainder attributes (such as index,

- 9 -

dispersion, thermal coefficient, etc). In general, optical glasses that are reasonably well suited for use in relay rods tend to occur at abbe numbers between 35 and 65, and indices of refraction between 1.5 and 1.65 (refer to the plot of refractive index versus Abbe number of FIG. 5, in which some suitable glasses made by SCHOTT® with Abbe numbers between 50 and 65 include, e.g., N-PSK3, N-BALF5, N-SK2, N-BAK2, N-K5 and N-KF9). Glasses that will form the outer elements may be then selected based on other design requirements, such as their thermal coefficients relative to their neighbor glass on the other side of a lens bond. Optimization for minimum wavefront error across all field positions will drive the form to be symmetric about the pupil in regard to index of refraction, and asymmetric about the pupil in regard to Abbe number (or inverse dispersion). An example of a diffraction-limited solution is illustrated in FIG. 2. The outer elements, i.e., the relay objectives and field lenses will be the same on both sides of the relay pupil. The focal lengths for each relay rod lens assembly are nearly identical, but the partial dispersions of the relay rod lens assemblies due to the different rod materials have compensatory effects on residual wavefront error.

FIGS. 6A to 6C illustrate dispersion in a comparative example and an example according to an embodiment. FIG. 6A shows a plot of the modulus of the optical transfer function (OTF) (MTF) versus spatial frequency in cycles per mm for an F/4.5 relay in which the same material, here N-PSK3, is used for both relay rods in a relay system for a 30 cm visible-near infrared endoscope having three relay pairs. FIG. 6B shows a plot of MTF versus spatial frequency in which elements of the same relay system as used for FIG. 6A are used, except the same material for the relay rods is N-BALF5. FIG. 6C shows a plot of MTF versus spatial frequency in which elements of the same relay system as used for FIG. 6A are used, except different materials are used for the relay rods on opposite sides of the relay pupil. For

- 10 -

example, a first material, here N-PSK3, is used for the first relay rod, and a second material, here N-BALF5, is used for the second material. The comparing FIGS. 6A to 6C, the MTF for the transverse off-axis ray is significantly improved by use two different materials for the relay rods.

5

By way of summation and review, endoscopes typically include a long, thin, rigid or semi-rigid optical cylinder that is mounted on or to a viewing mechanism or imager. When the endoscope is inserted and positioned for use, an image of the object being viewed is formed by an objective lens at the inserted or distal end of the endoscope.

10 The image passes through a relay lens system, comprising of one or more sets of relay lenses, along the cylinder to a viewer comprising an eyepiece or viewing lens or a video camera or imager at the viewing or proximal end of the endoscope.

A relay lens system will reconstruct the image formed at the objective lens one or
15 more times, depending on the number of relays used. A single relay will form one image. Additional relays may be used to form additional images. The purpose of these elements is not to produce many images, but rather to carry the image field to another position. Endoscopes are narrow in order to reduce the size of an incision. Endoscopes are long because the object under study may be deep within the body.
20 The image formed by the objective lens at the distal end is relayed along the length of the endoscope to the proximal end by the relay lens system.

When used in endoscopes, the relay lenses may be very narrow, e.g., less than 6.5 mm in diameter and approximately 20 mm to 50 mm long. Most endoscopes require
25 three or more sets of relay lenses for proper operation. The number of lenses generally depends on the length and specific requirements of the particular endoscope and/or the application for which it is intended. Because the objective and

- 11 -

each relay set is producing an image with unit magnification which is turned upside down, and because a standard endoscope should produce an upright image, usually an odd number of relay lenses are used so that the image produced by the optical system at the ocular or at the detector, is upright.

5

For good image quality, the optical system of an endoscope should be well corrected for the major lens aberrations. A relay lens typically operates with unit magnification with lenses configured to be symmetric about the relay's internal stop plane, i.e., the pupil within the relay. This set of conditions will result in the odd Seidel aberrations
10 formed by the lenses before the relay's pupil to be cancelled out by the lenses after the relay's pupil. However, the even Seidel aberrations are not corrected. As noted above, these even Seidel aberrations may become more problematic as an operational waveband over which the optical system is to perform increases.

15 According to an embodiment discussed above, using different materials for relay rods on opposite sides of the relay pupil may allow dispersion to be compensated without changing the basic form of the relay. In other words, by using different rod materials on opposite sides of the relay pupil, other elements, e.g., objectives and field lenses, on opposite sides of the relay pupil may be identical, such that the pair
20 of relay rod lens assemblies are otherwise identically configured, e.g., identical lengths, identical lens elements, identical geometric form, and so forth, while using different rod materials.

According to another embodiment, there is further provided a method of
25 compensating for dispersion in a relay lens system. The method comprises providing a first relay rod of a first material, providing a second relay rod of a second material,

- 12 -

different from the first material, and providing a lens between the first and second relay rods.

According to yet further embodiment, there is provided a kit comprising a first relay
5 rod of a first material, a second relay rod of a second material, different from the first material, and a lens to be inserted between the first and second relay rods. In an embodiment the lens includes a first relay objective and a second relay objective. In an embodiment, the first and second relay objectives have a same design and material.

10

Example embodiments have been disclosed herein, and although specific terms are employed, they are used and are to be interpreted in a generic and descriptive sense only and not for purpose of limitation. In some instances, as would be apparent to one of ordinary skill in the art as of the filing of the present application, features,
15 characteristics, and/or elements described in connection with a particular embodiment may be used singly or in combination with features, characteristics, and/or elements described in connection with other embodiments unless otherwise specifically indicated. Accordingly, it will be understood by those of skill in the art that various changes in form and details may be made without departing from the
20 spirit and scope of the present invention as set forth in the following claims. For example, while specific examples have been directed to endoscopes, embodiments may be used with other imaging system with similar waveband and single detector requirements, e.g., borescopes.

25

**THE EMBODIMENTS OF THE INVENTION IN WHICH AN EXCLUSIVE
PROPERTY OR PRIVILEGE IS CLAIMED ARE DEFINED AS FOLLOWS:**

1. An optical system, comprising:
5 a first relay rod of a first material;
a second relay rod of a second material, different from the first
material; and
a lens between the first and second relay rods;
wherein the first and second relay rods are geometrically symmetric to one
10 another relative to a pupil or conjugate pupil of the optical system.
2. The optical system as claimed in claim 1, further comprising a field of view,
wherein the optical system produces a wavefront error across the field of view and
wherein the first and second materials are selected to reduce the wavefront error within
15 the field of view as compared with using a same material for both the first and second
relay rods.
3. The optical system as claimed in claim 1 or 2, wherein the first and second relay
rods have no optical power.
20
4. The optical system as claimed in any one of claims 1 to 3, wherein the first and
second relay rods have no optically powered surfaces.
5. The optical system as claimed in any one of claims 1 to 4, wherein the
25 lens includes a first relay objective and a second relay objective.
6. The optical system as claimed in claim 5, wherein the first and second
relay objectives have a same design and material.
- 30 7. The optical system as claimed in any one of claims 1 to 6, wherein a

pupil region of the system is in air.

8. The optical system as claimed in any one of claims 1 to 7, further comprising:

- 5 a third relay rod of a third material;
 a fourth relay rod of a fourth material, the fourth material being
 different from the third material; and
 a lens between the third and fourth relay rods.

10 9. The optical system as claimed in claim 8, wherein the first and third
materials are the same and the second and fourth materials are the same.

10. The optical system as claimed in any one of claims 1 to 9, further comprising a detector to detect light from 460 nm to 850 nm.

15 11. An endoscope including the optical system as claimed in any one of
claims 1 to 10.

12. A kit, comprising:

- 20 a first relay rod of a first material;
 a second relay rod of a second material, different from the first
material; and
 a lens to be inserted between the first and second relay rods;
 wherein the first and second relay rods are geometrically symmetric to one
25 another relative to a pupil or conjugate pupil of the optical system.

13. The kit as claimed in claim 12, wherein the lens includes a first relay objective and a second relay objective.

30 14. The kit as claimed in claim 13, wherein the first and second relay objectives have a same design and material.

15. A method of compensating for dispersion in a relay lens system, the method comprising:
- 5 providing a first relay rod of a first material;
- providing a second relay rod of a second material, different from the first material; and
- providing a lens between the first and second relay rods;
- wherein the first and second relay rods are geometrically symmetric to one another relative to a pupil or conjugate pupil of the optical system.
- 10
16. Use of an imaging agent and the optical system of any one of claims 1 to 10 in medical imaging of tissue of a subject.
17. Use of an imaging agent and the endoscope of claim 11 in medical imaging of tissue
- 15 of a subject.
18. Use of an imaging agent and the method of claim 15 in medical imaging of tissue of a subject.
- 20
19. Use of the optical system of any one of claims 1 to 10 in medical imaging of tissue of a subject.
20. Use of the endoscope of claim 11 in medical imaging of tissue of a subject.
- 25
21. Use of the method of claim 15 in medical imaging of tissue of a subject.
22. The use of any one of claims 19 to 21 wherein the medical imaging comprises use of an imaging agent.
- 30
23. The use of any one of claims 16 to 18 or claim 22 wherein the imaging agent is or comprises a fluorescence imaging agent.

24. The use of claim 23 wherein the fluorescence imaging agent is or comprises indocyanine green (ICG).

5 25. The kit of claim 12 further comprising an imaging agent.

26. The kit of claim 25 wherein the imaging agent is or comprises a fluorescence imaging agent.

10 27. The kit of claim 26 wherein the fluorescence imaging agent is or comprises ICG.

28. Use of the kit of any one of claims 12 to 14, or claims 25 to 27 for medical imaging of tissue of a subject.

15 29. The use of any one of claims 16 to 24 or claim 28 wherein the medical imaging of tissue of the subject comprises assessment of the tissue, diagnosis of the tissue, or a combination thereof.

20 30. The use of any one of claims 16 to 24, 28, or 29 wherein the tissue forms a body structure or a portion thereof.

31. The use of any one of claims 16 to 24, or claims 28 to 30 wherein the medical imaging is performed in the visible region, near infrared region, or a combination thereof.

25

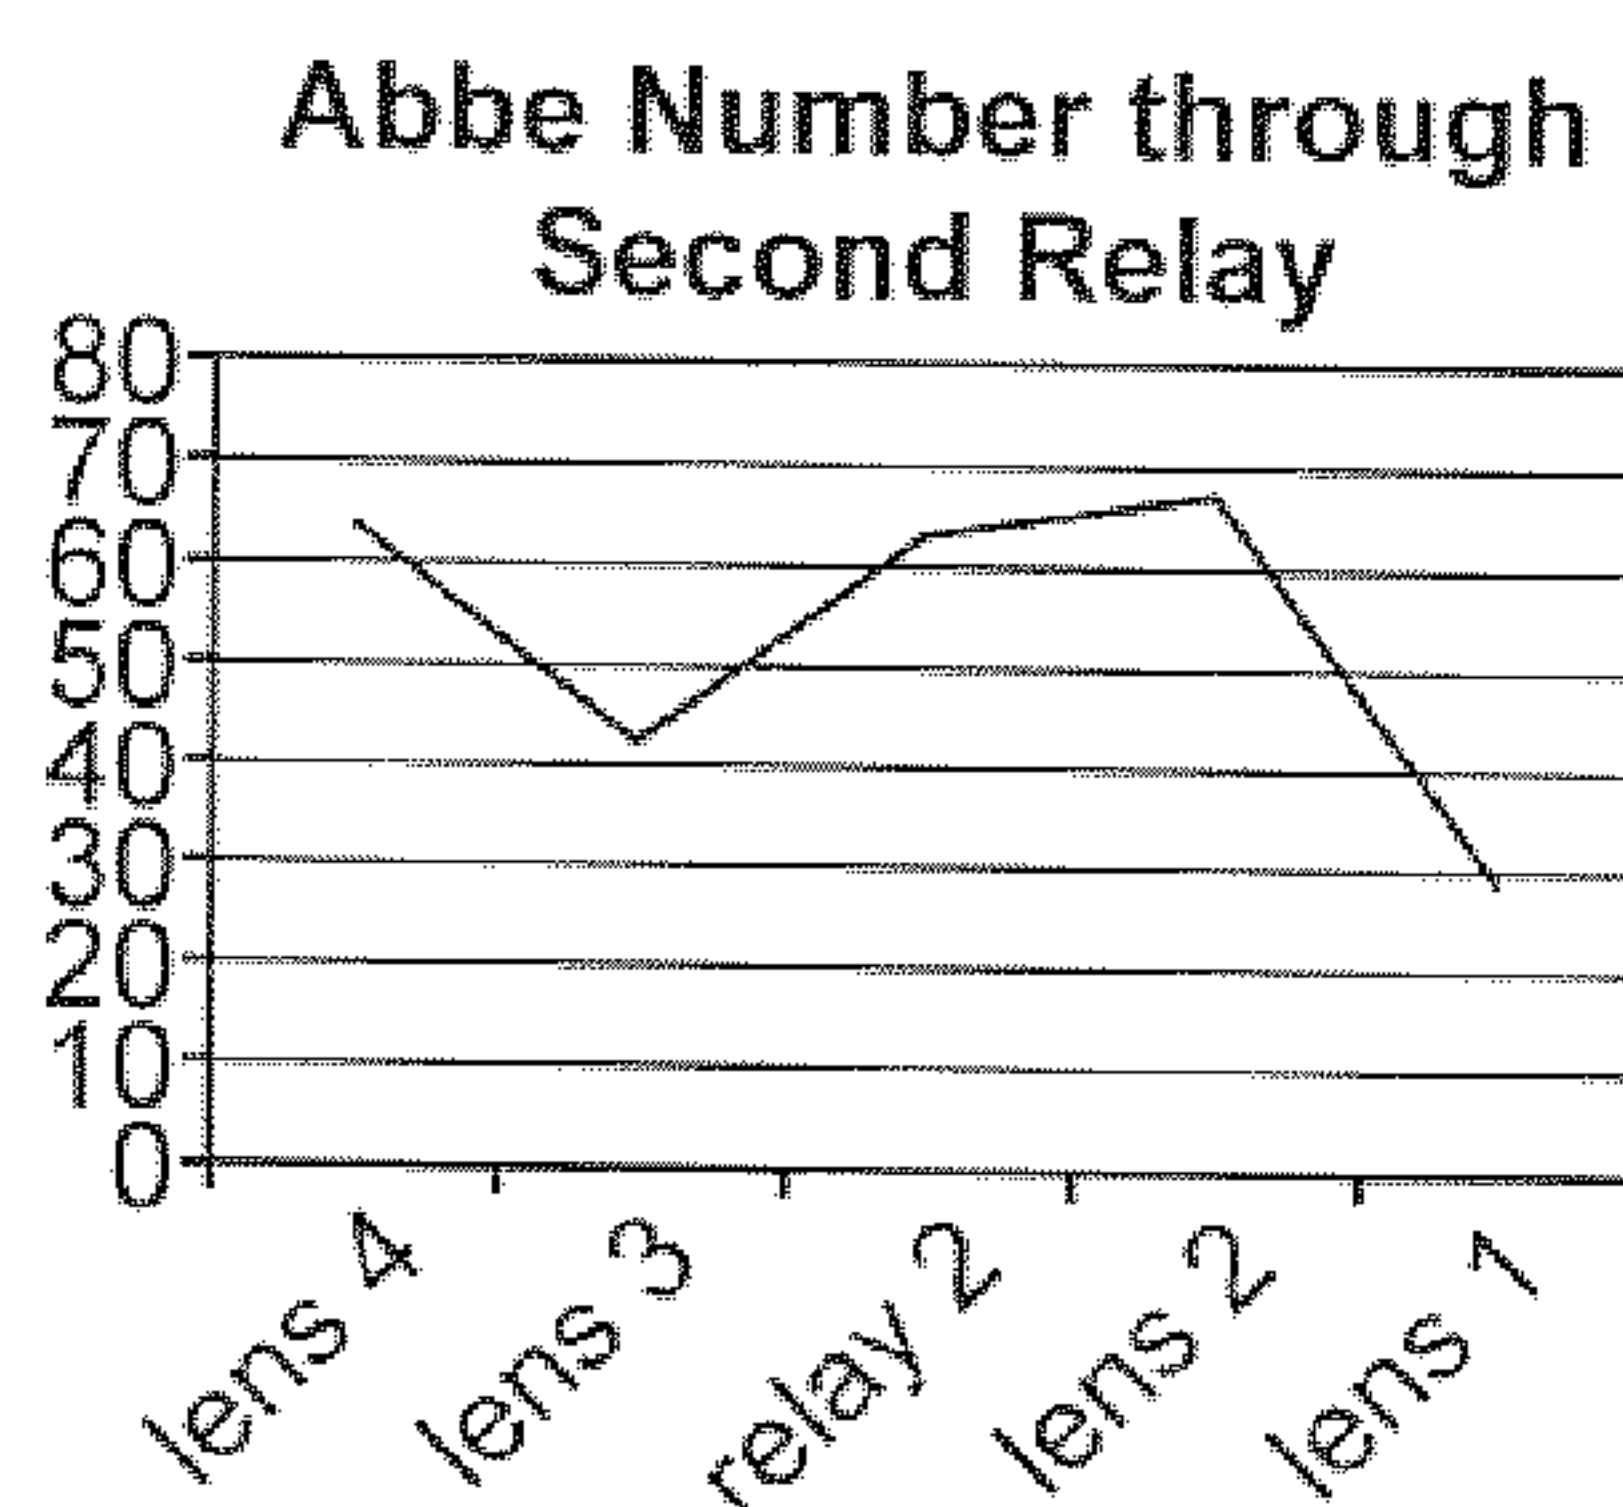
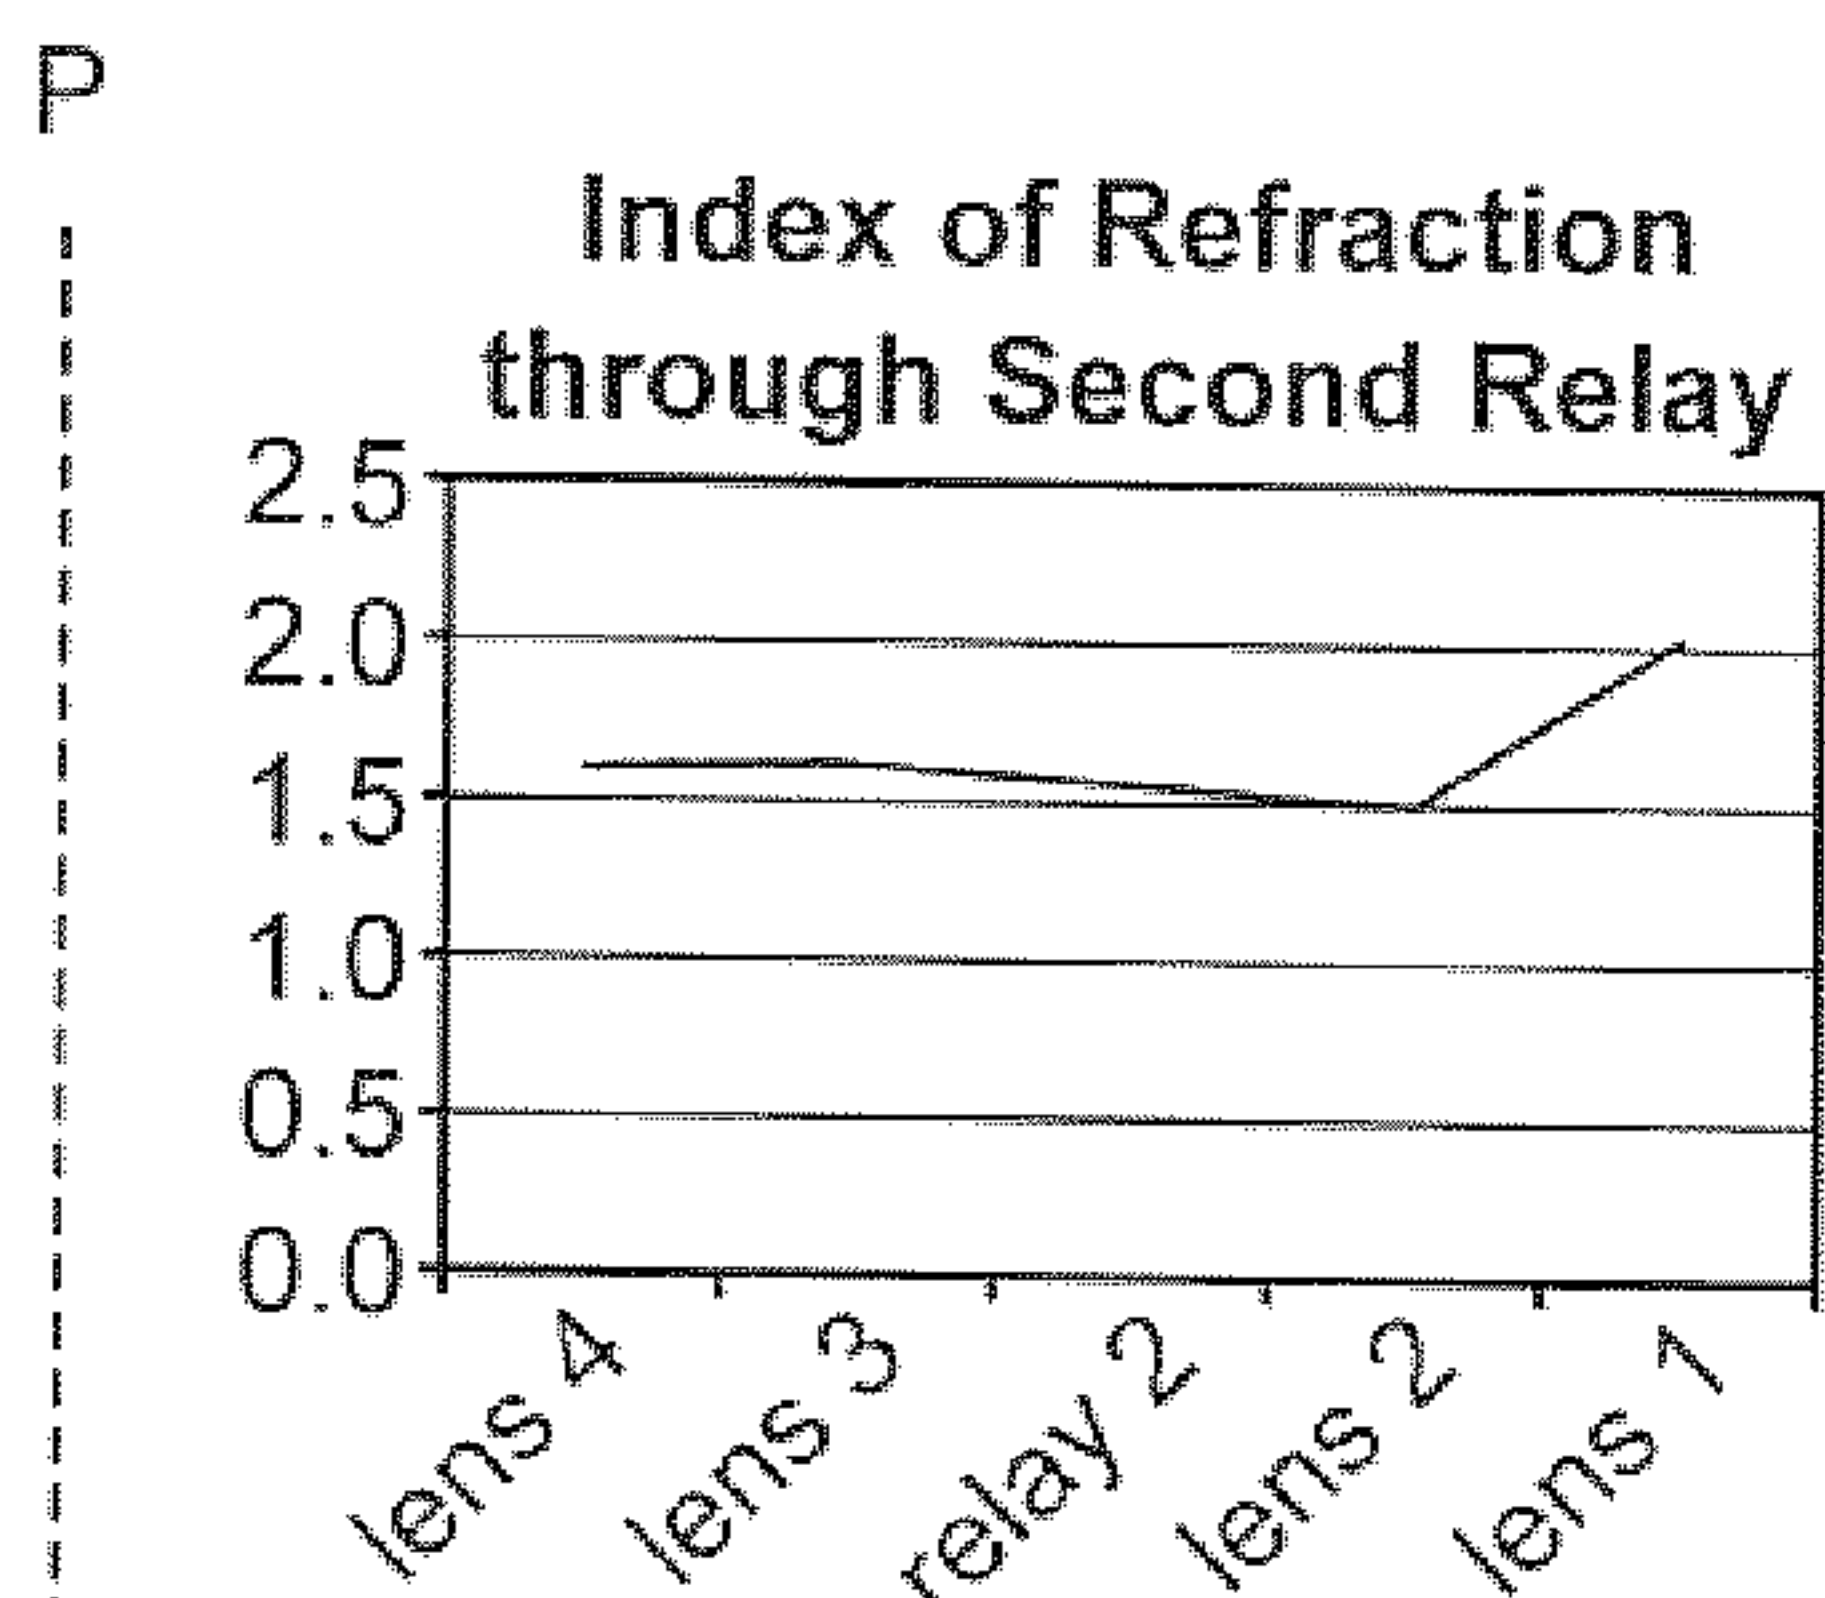
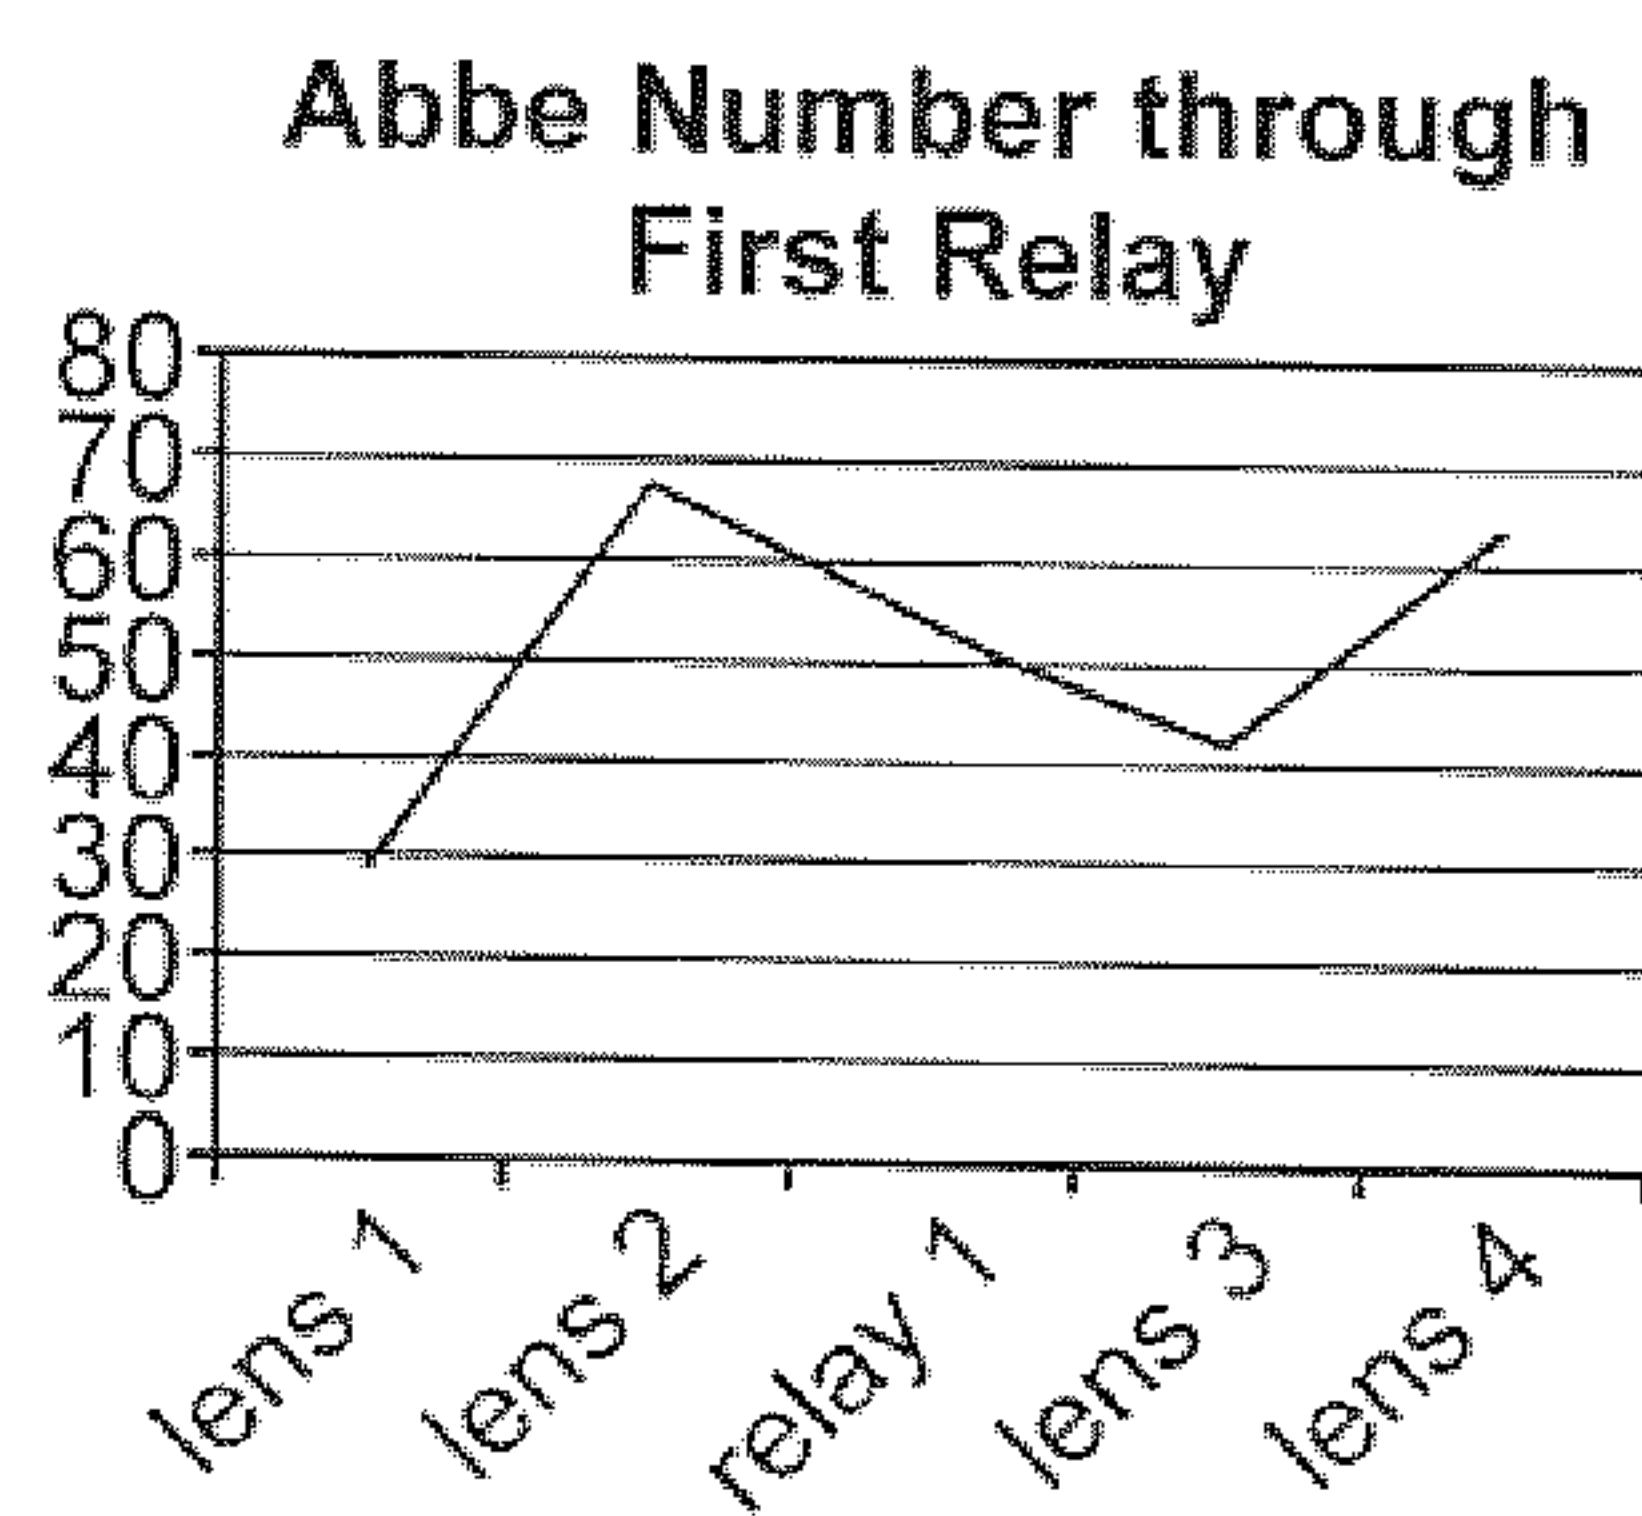
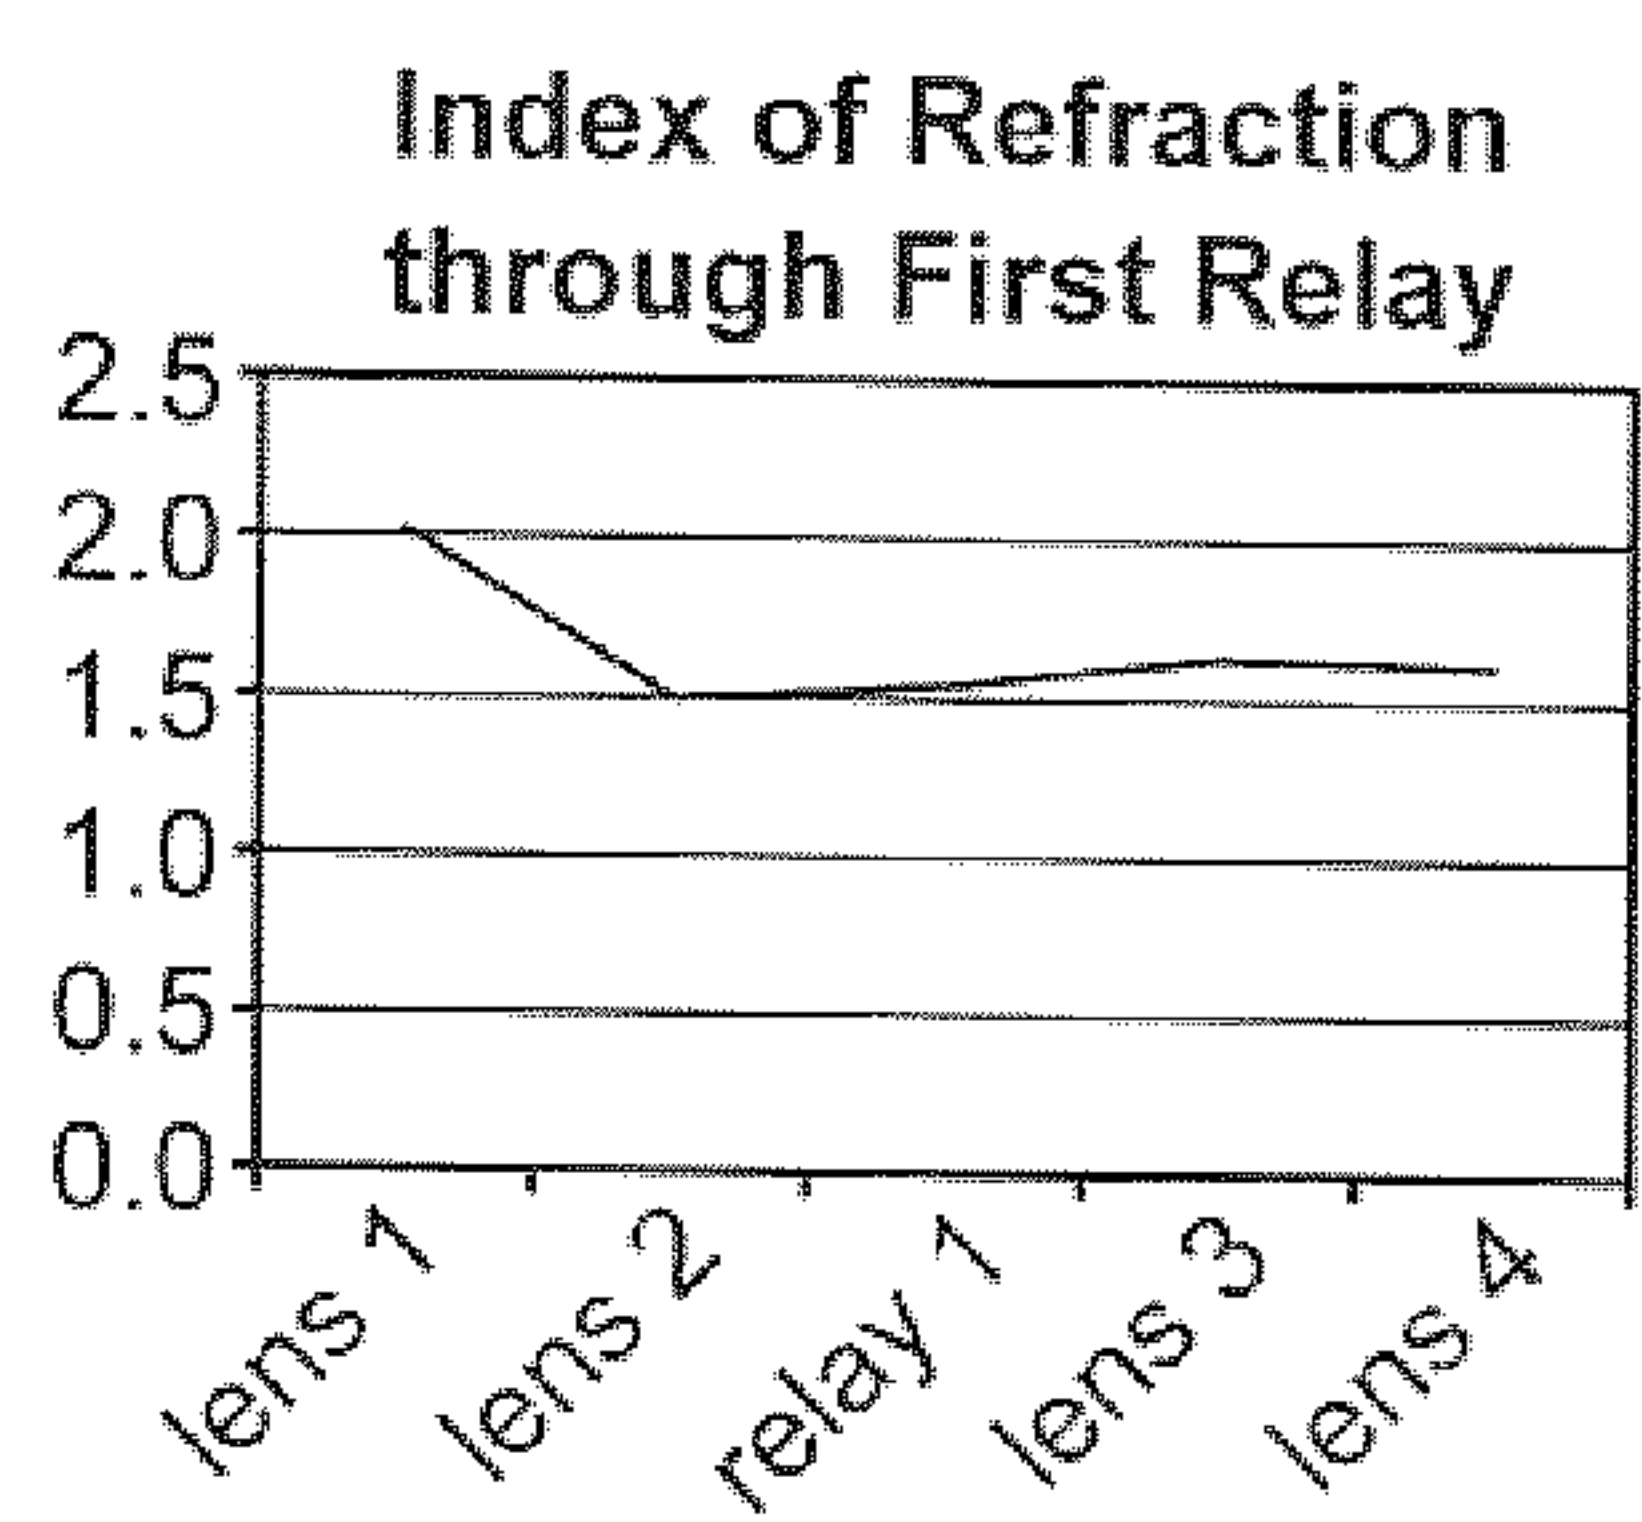
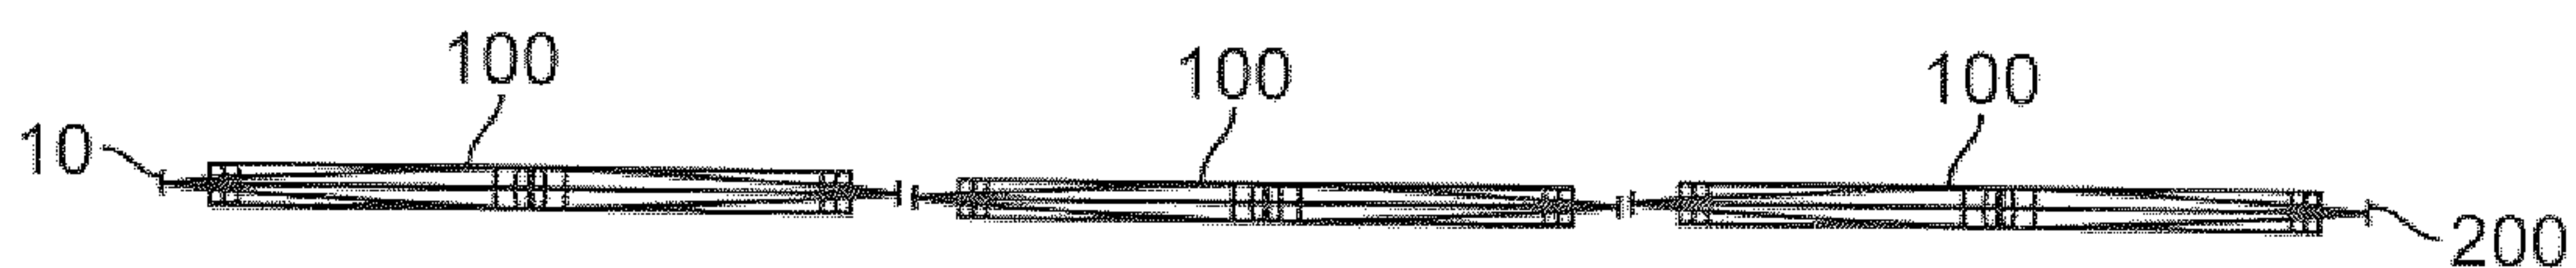
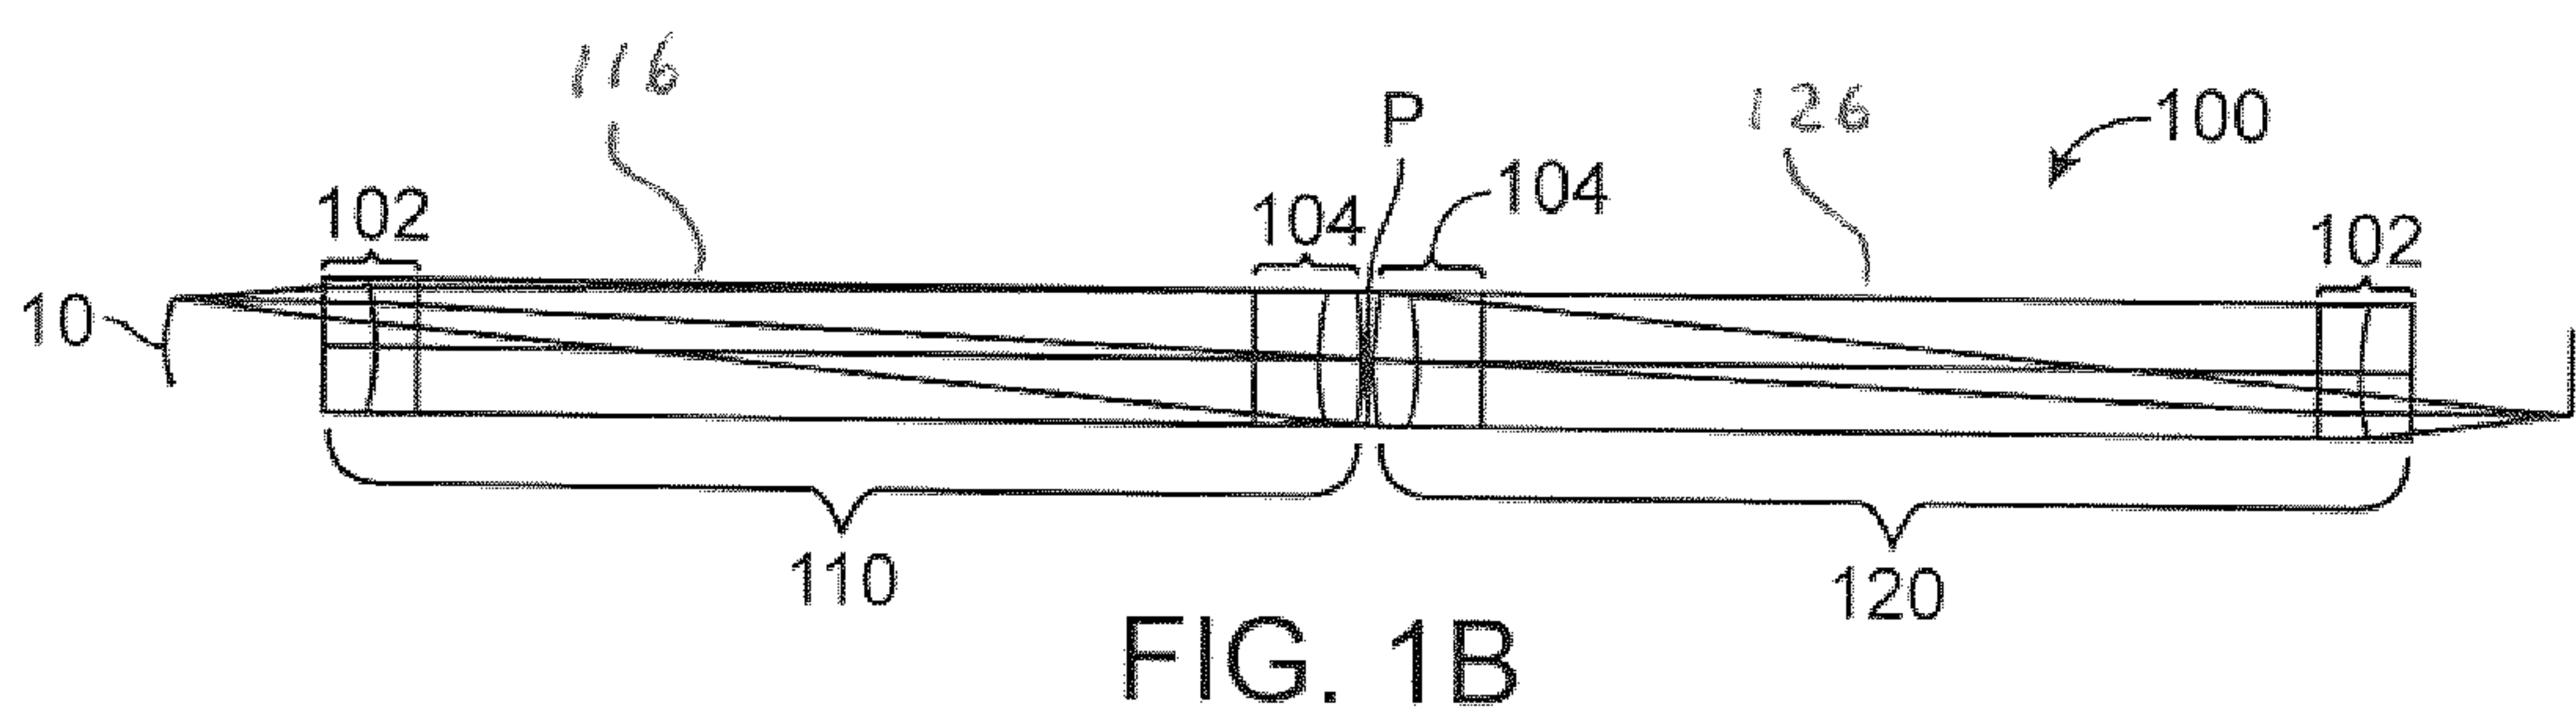
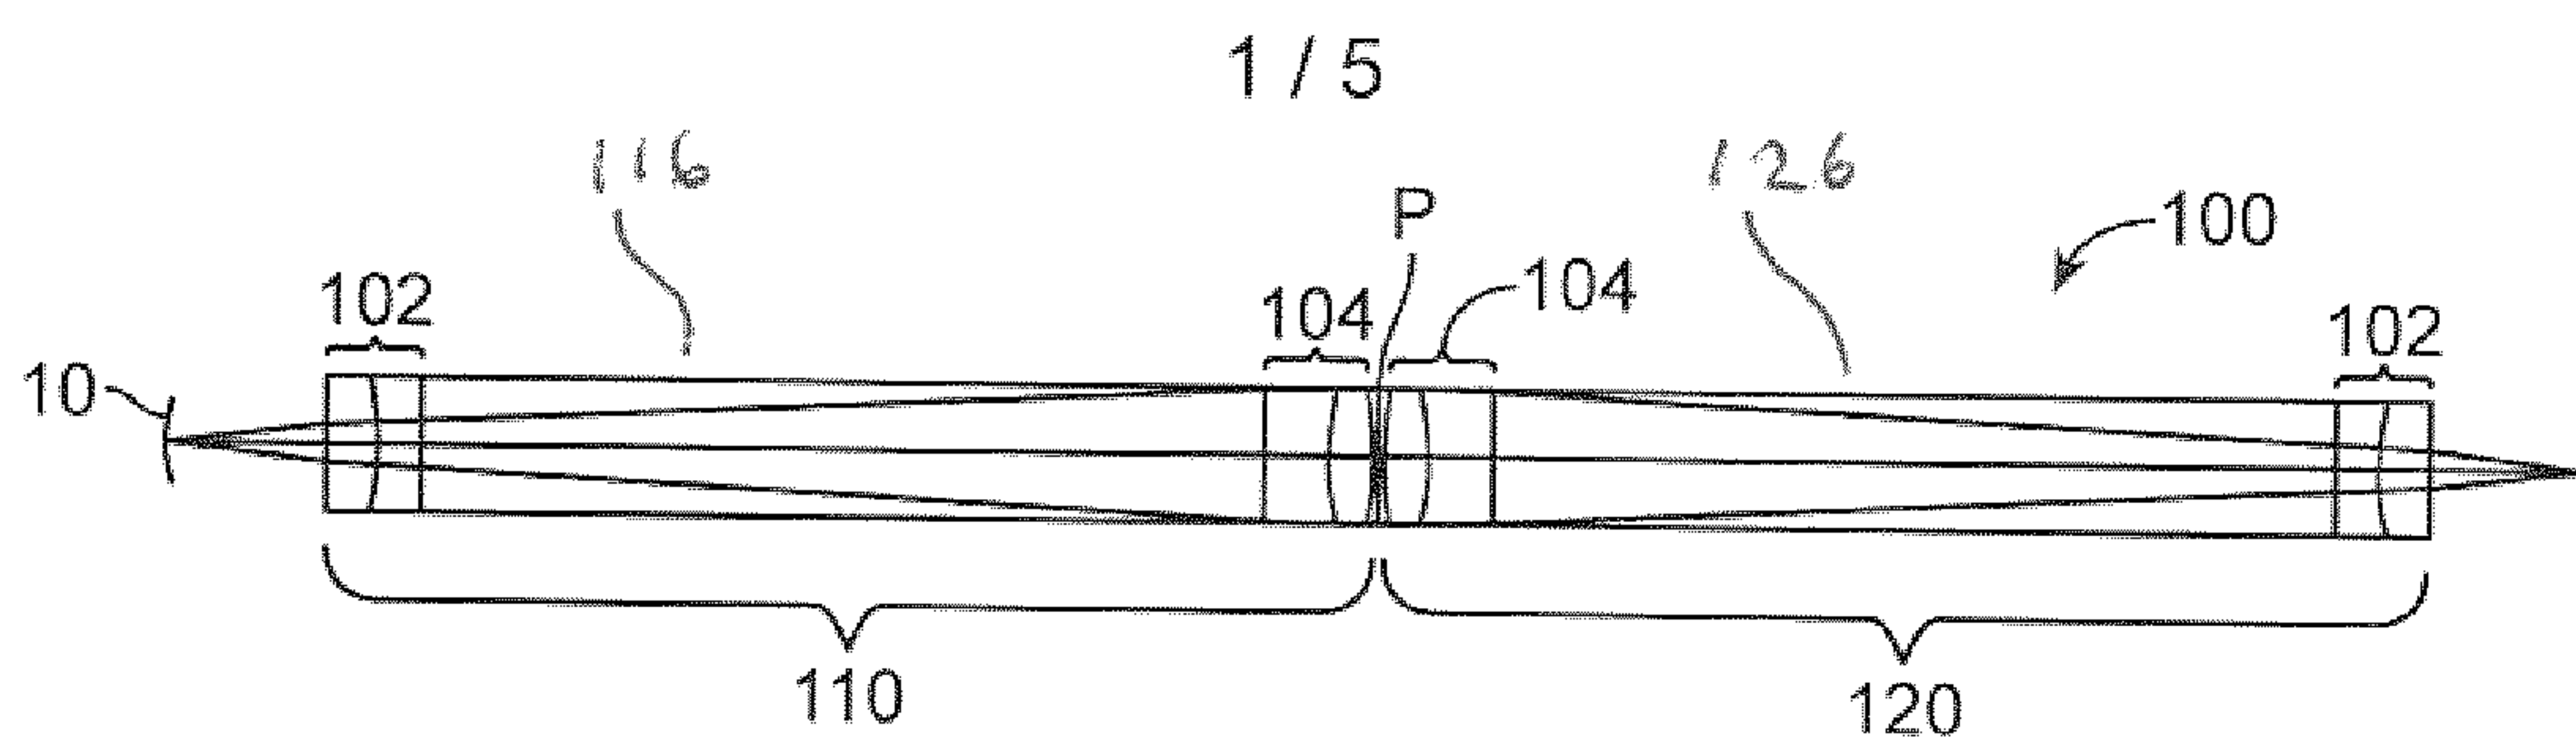


FIG. 2

2 / 5



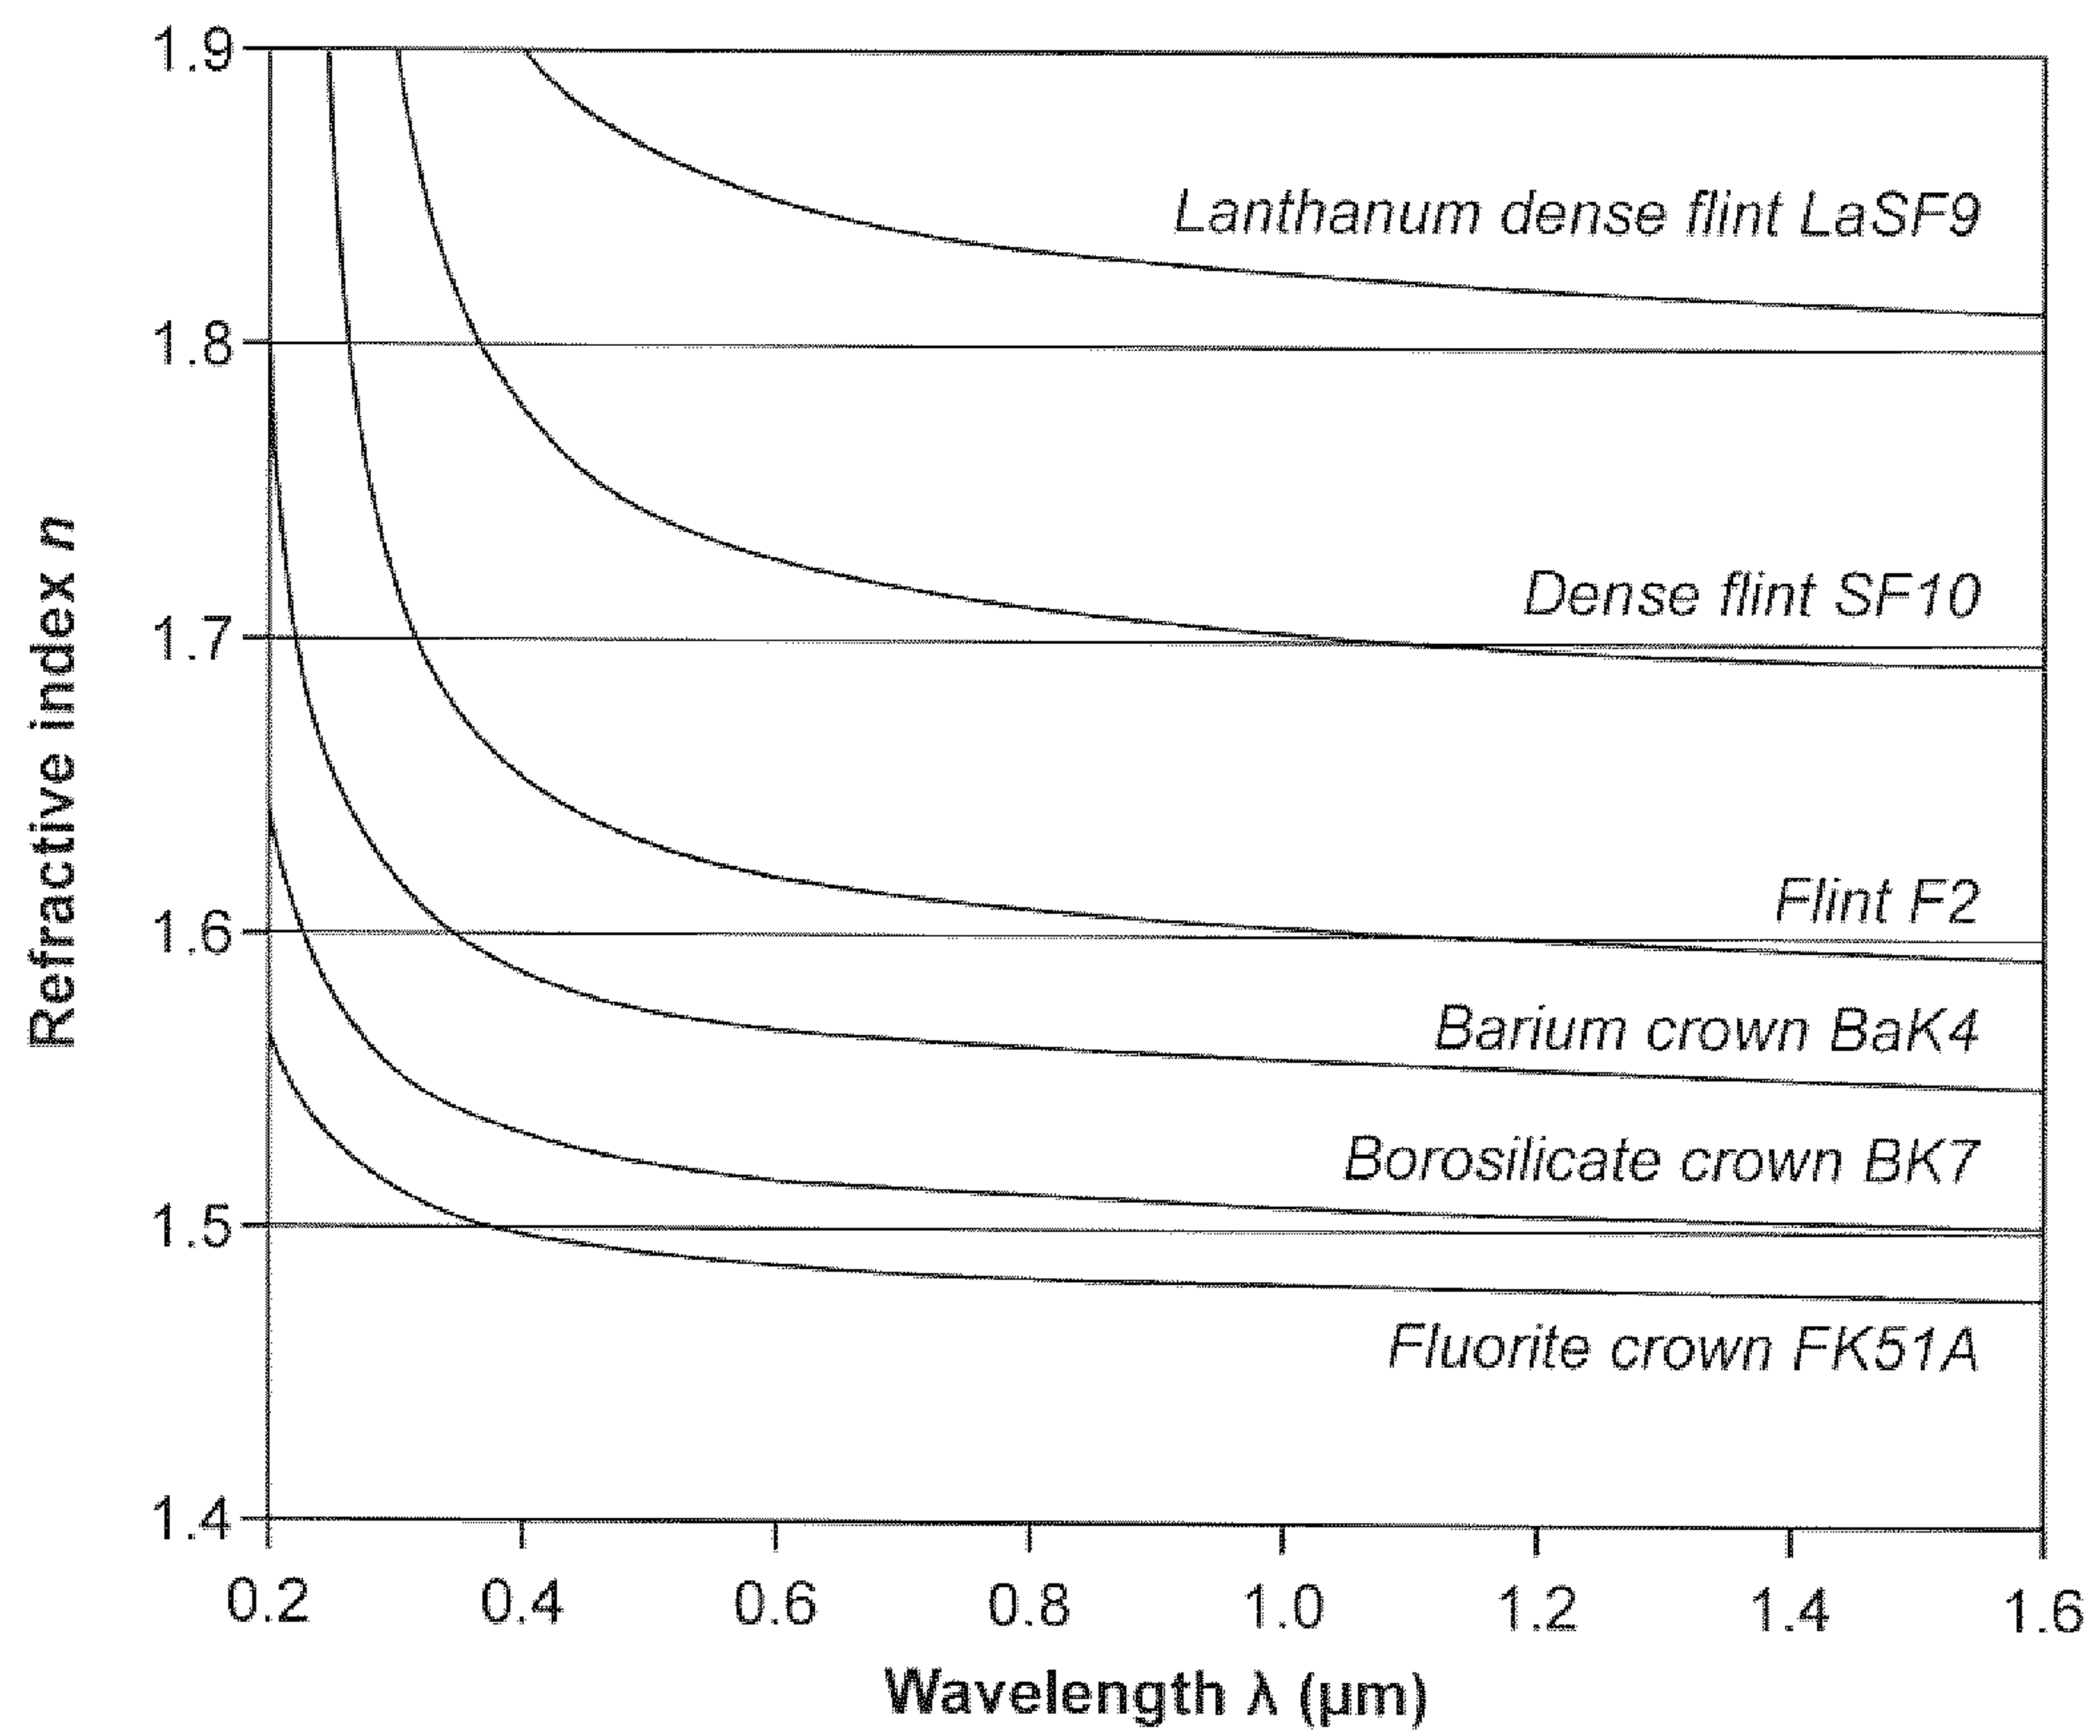


FIG. 3

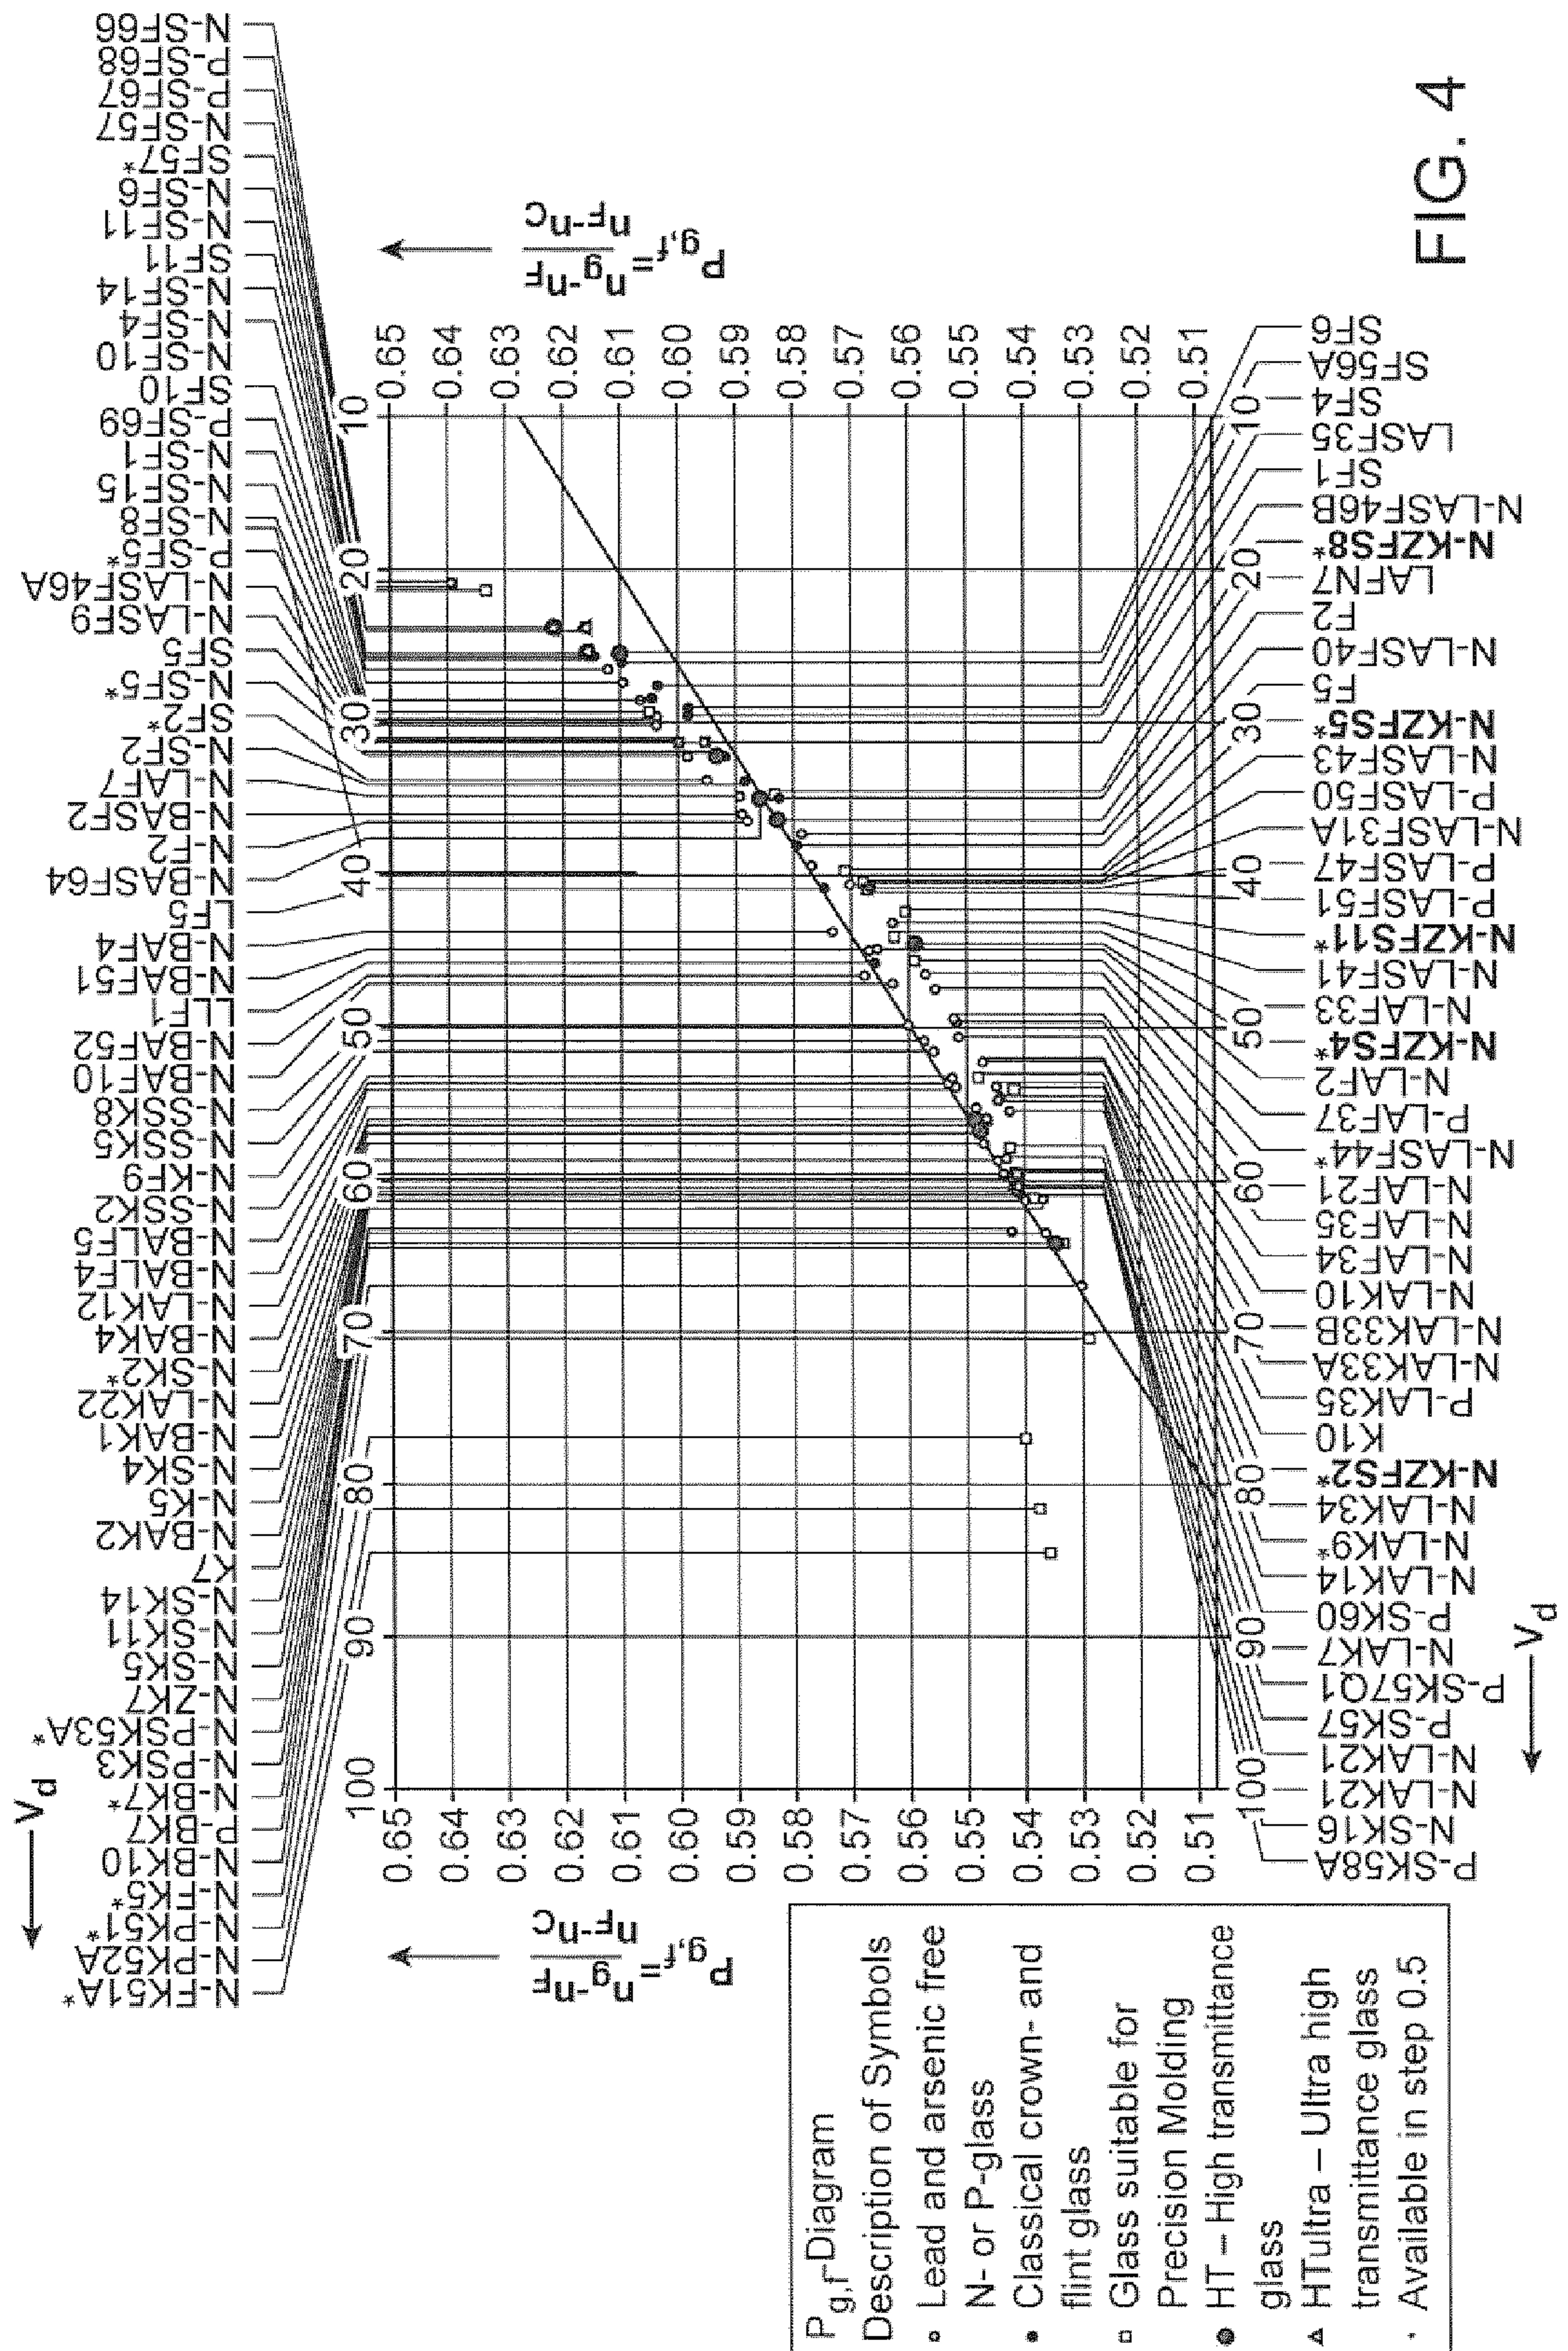

८५

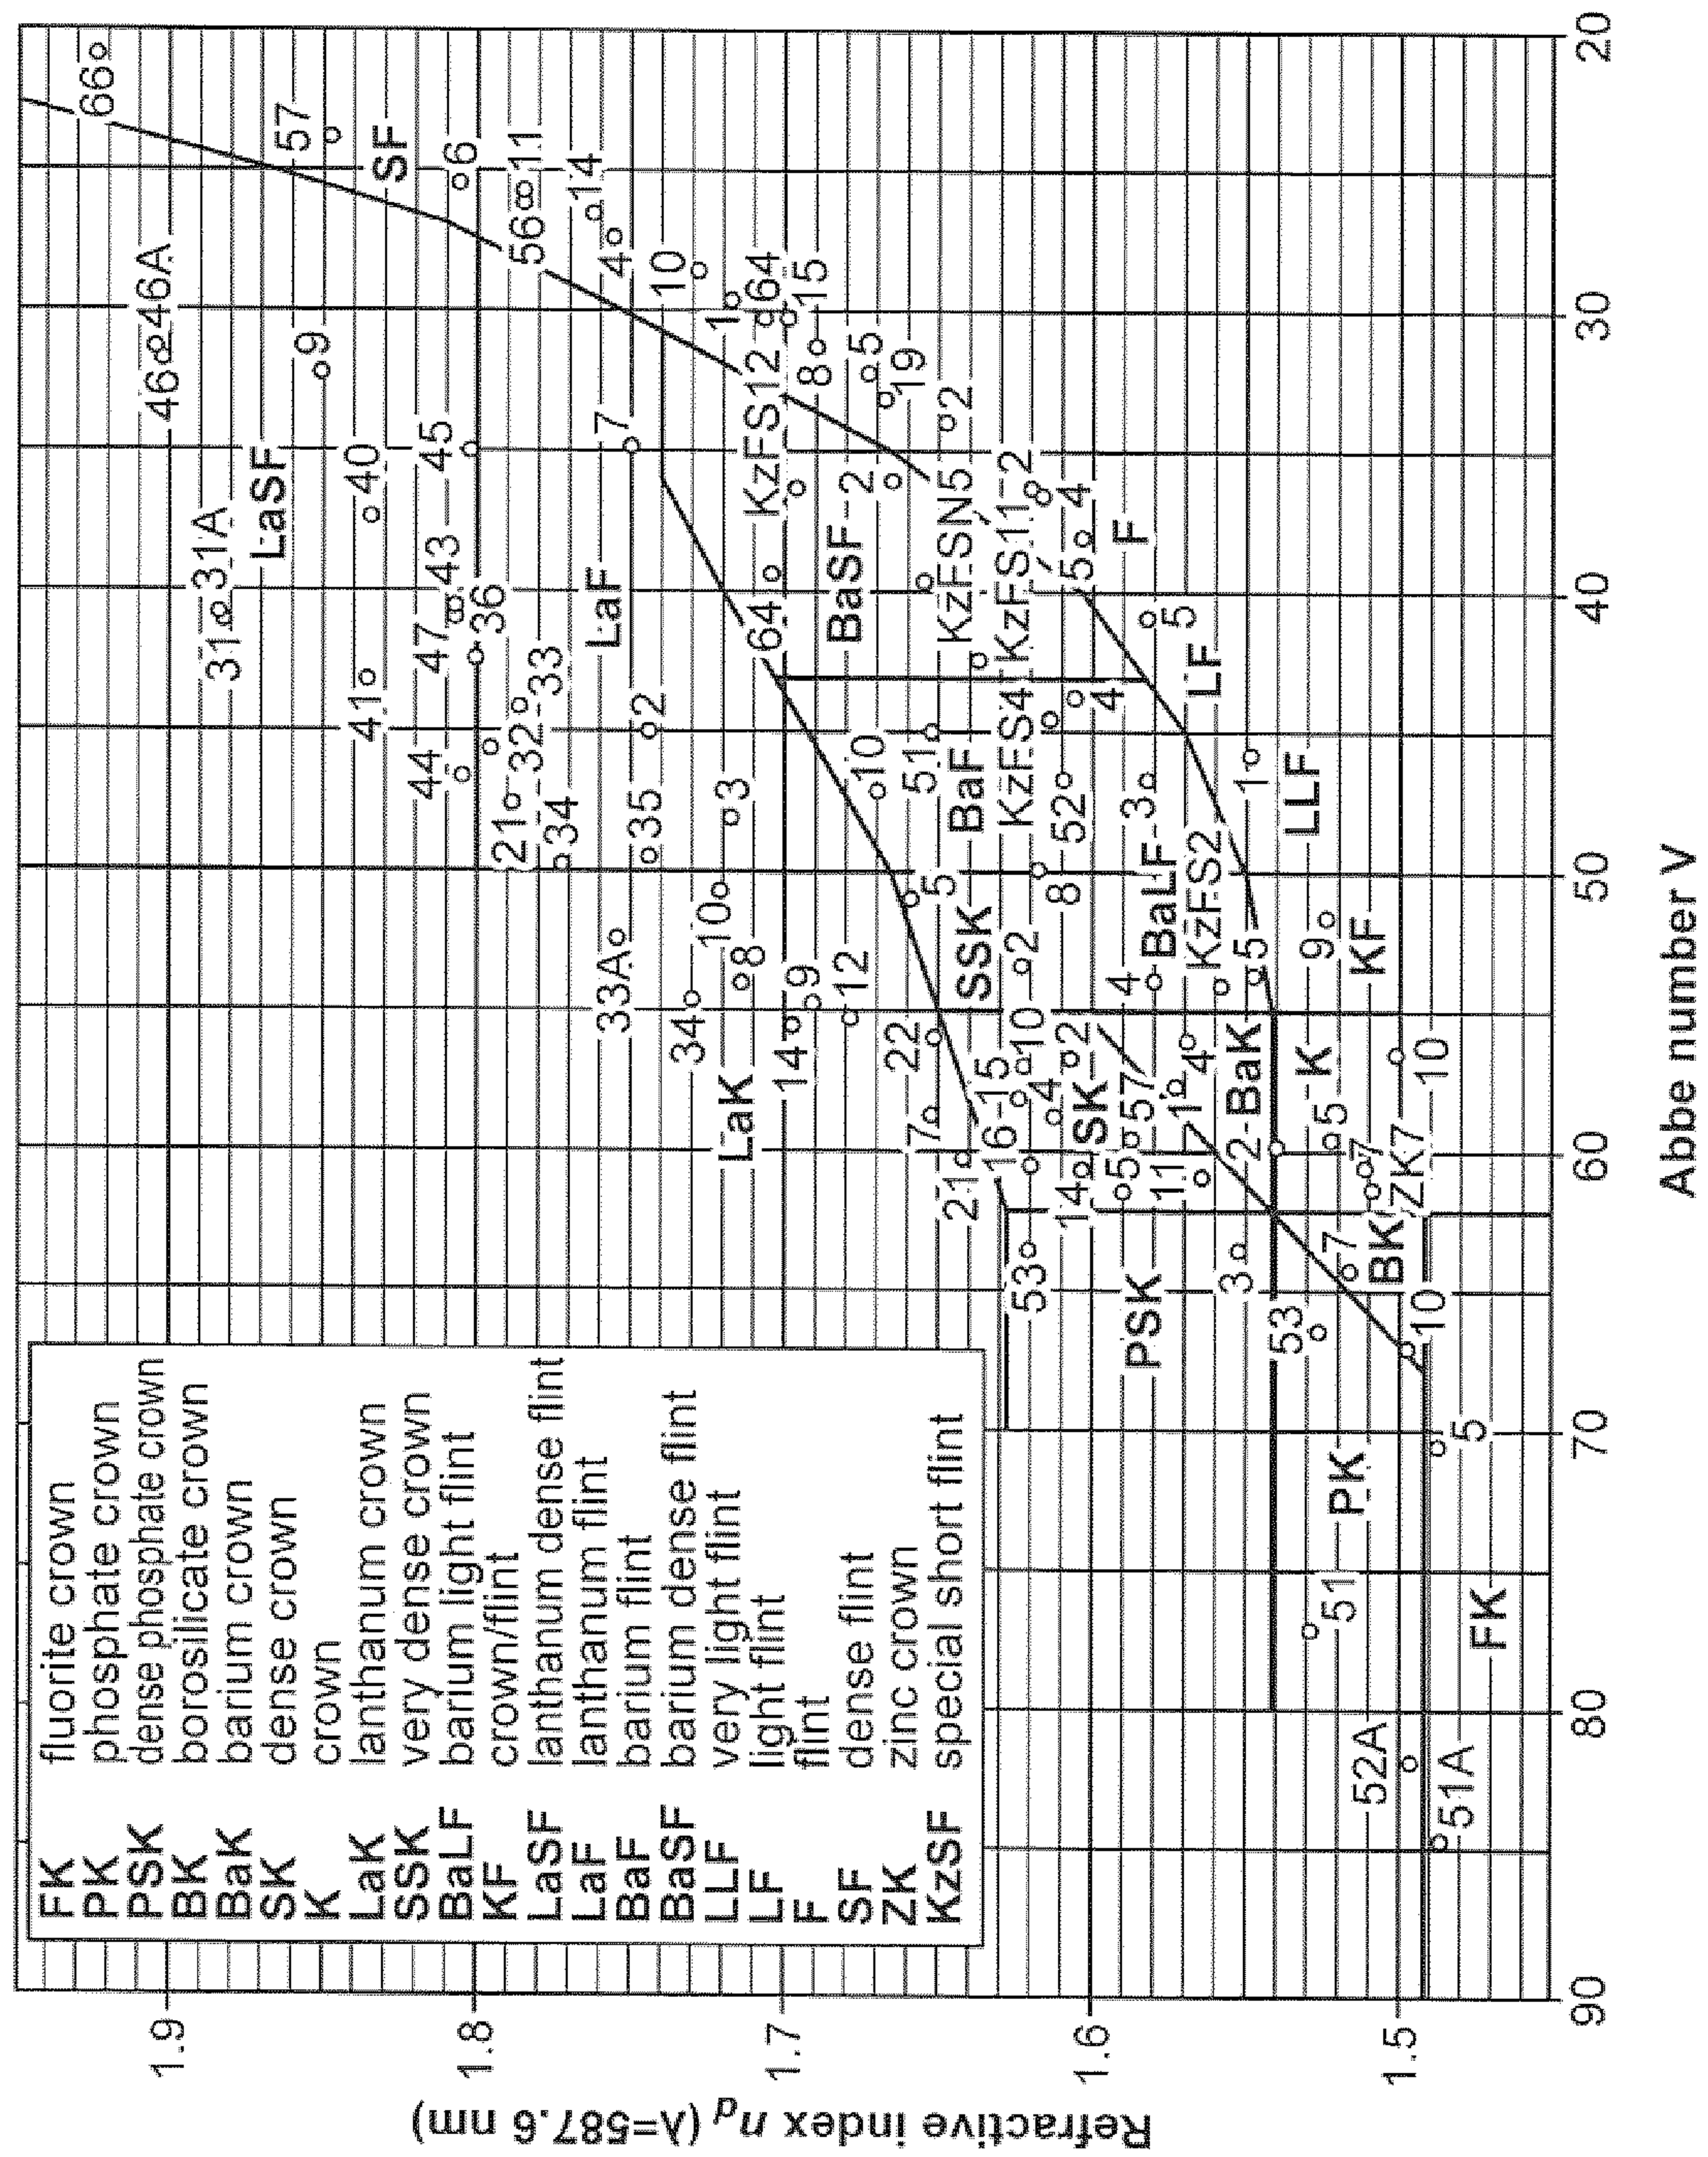

5 / 5

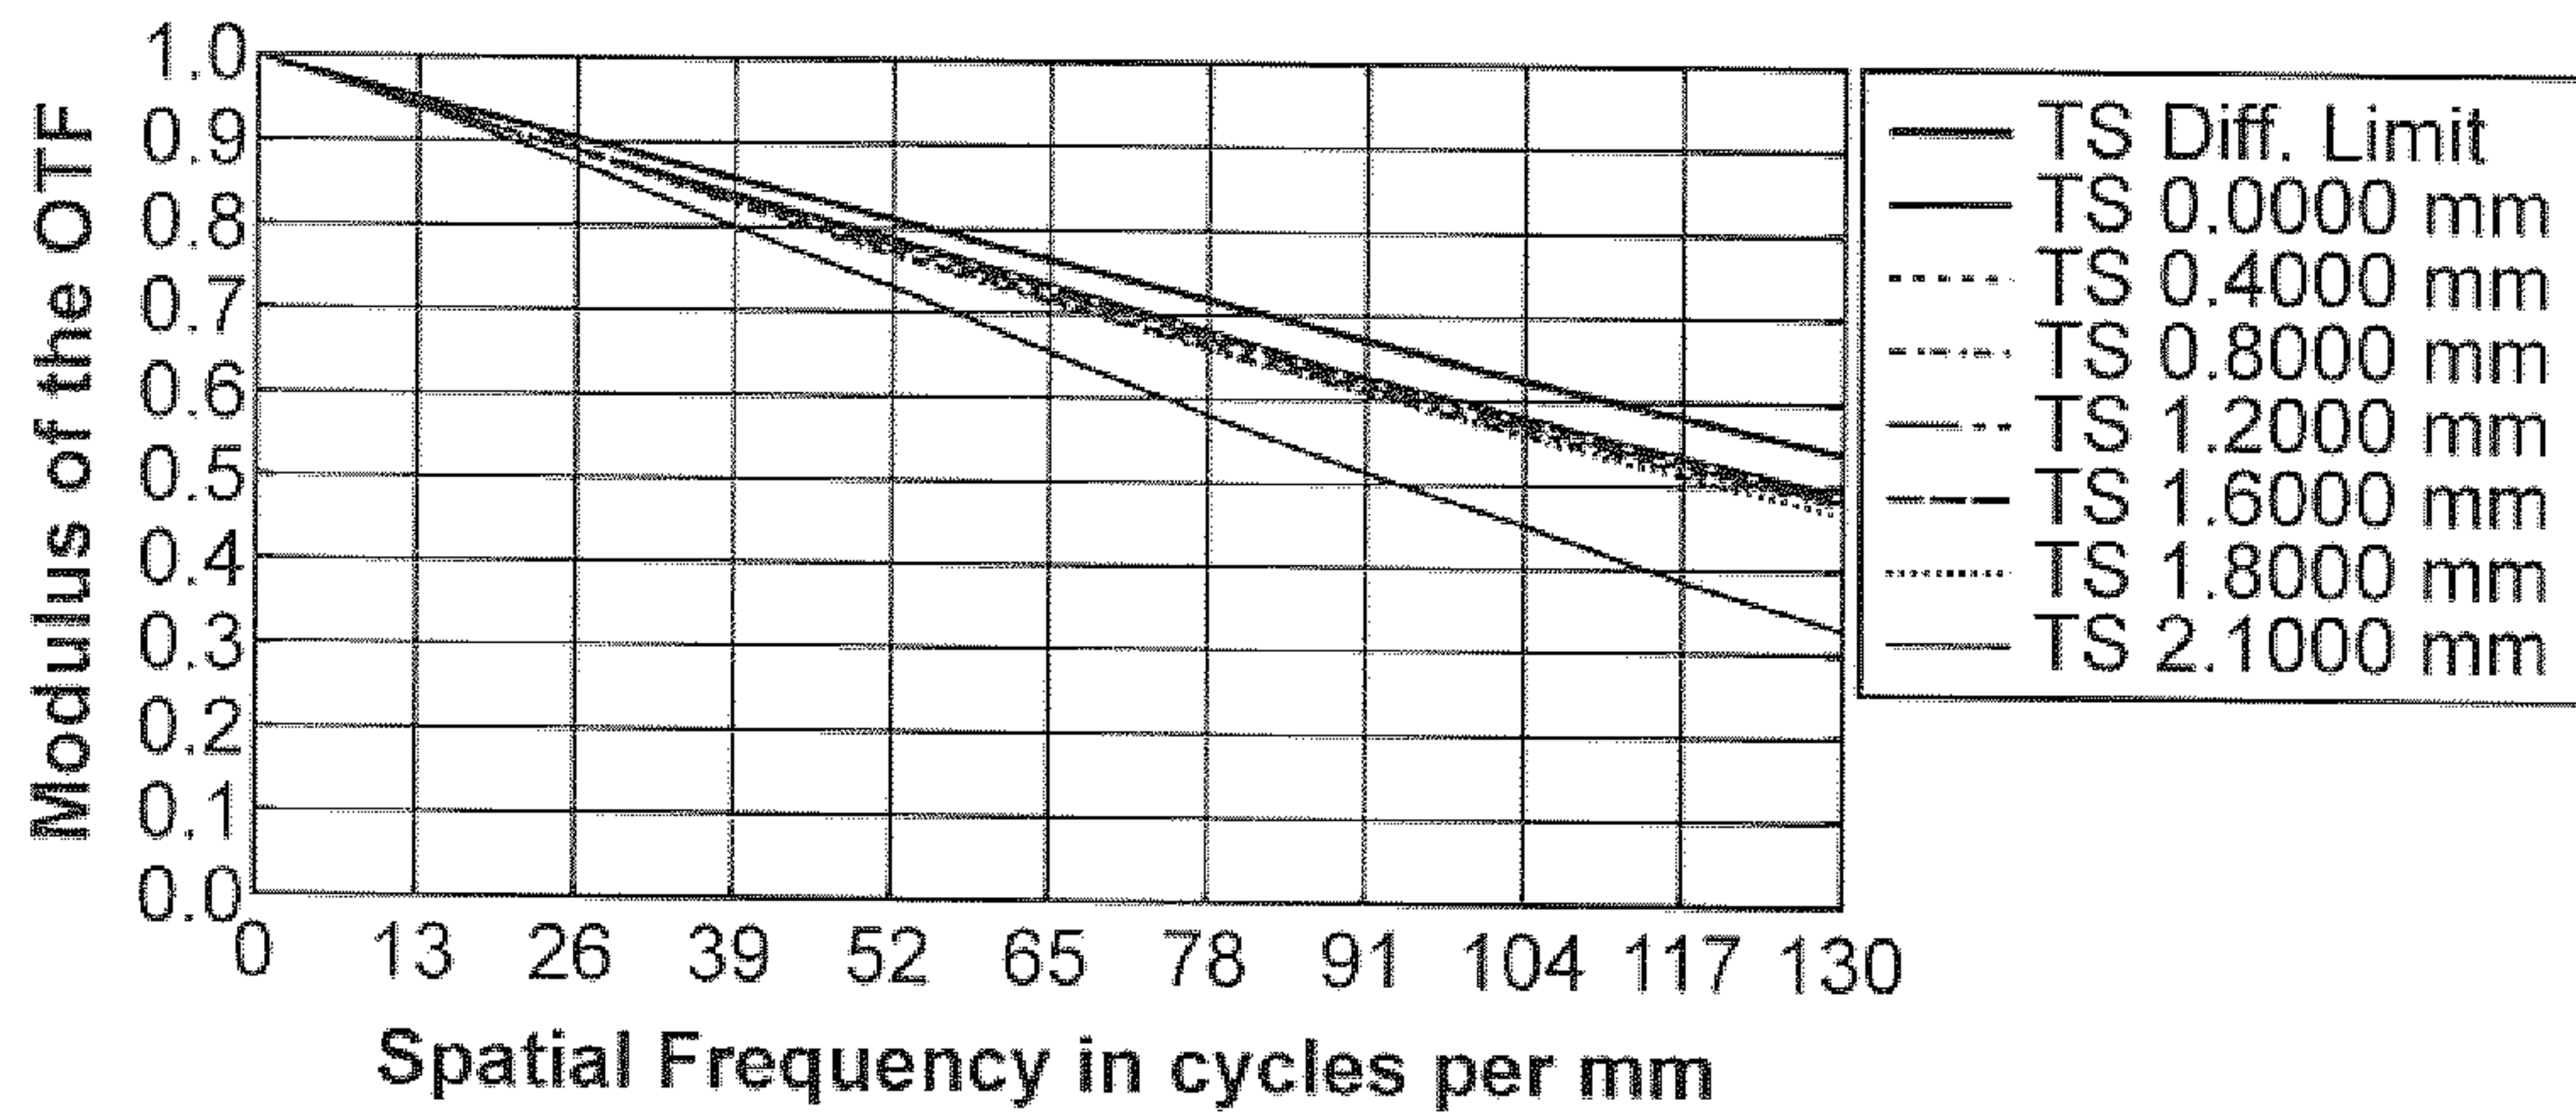


FIG. 6A

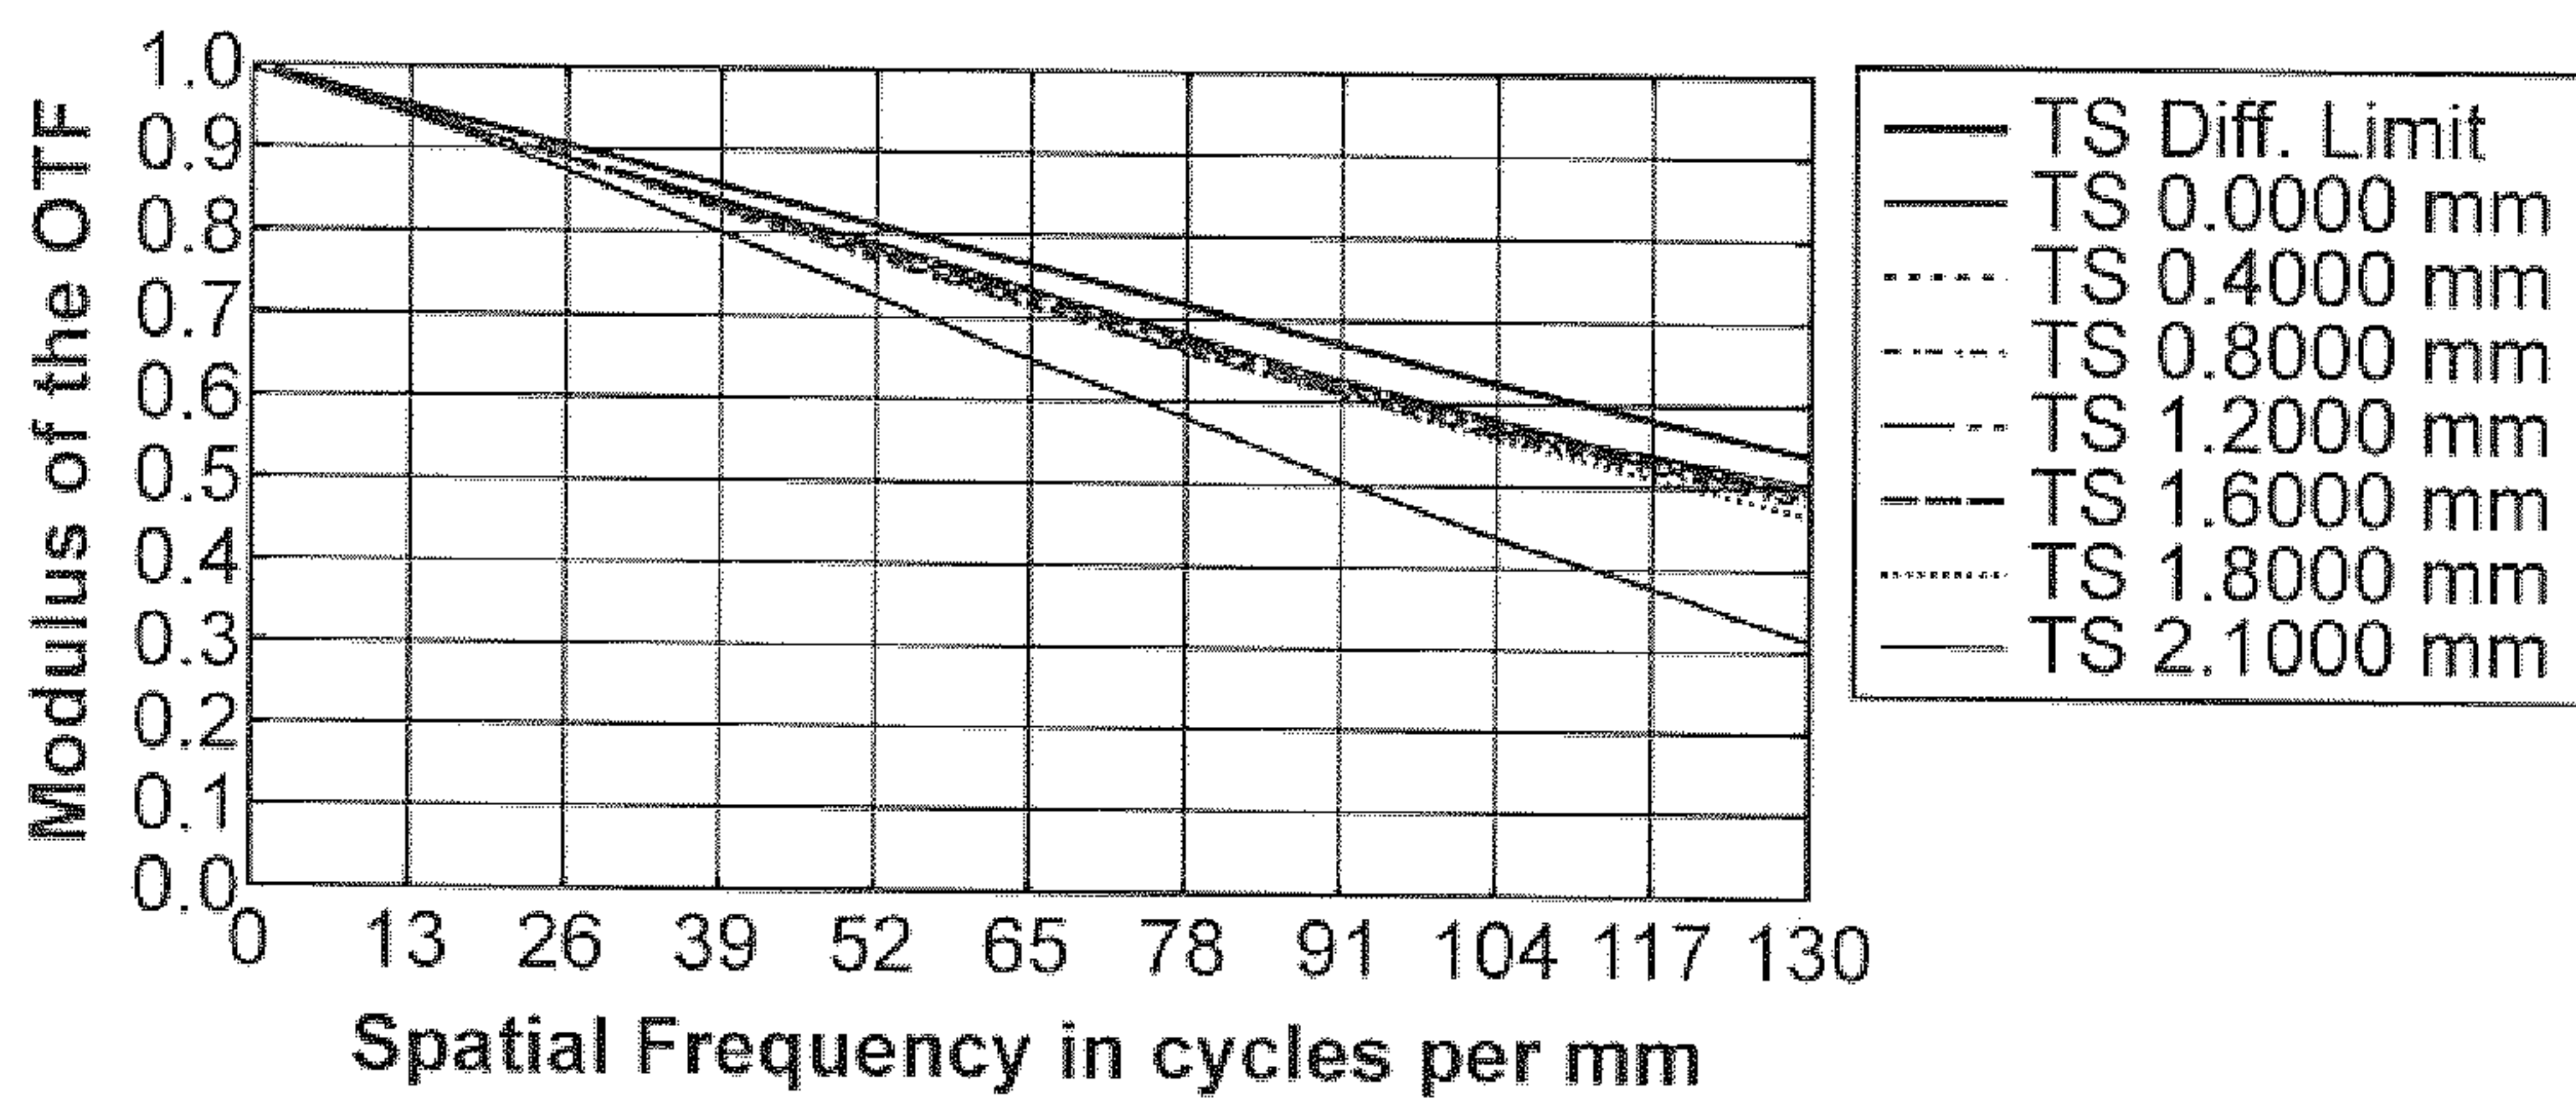


FIG. 6B

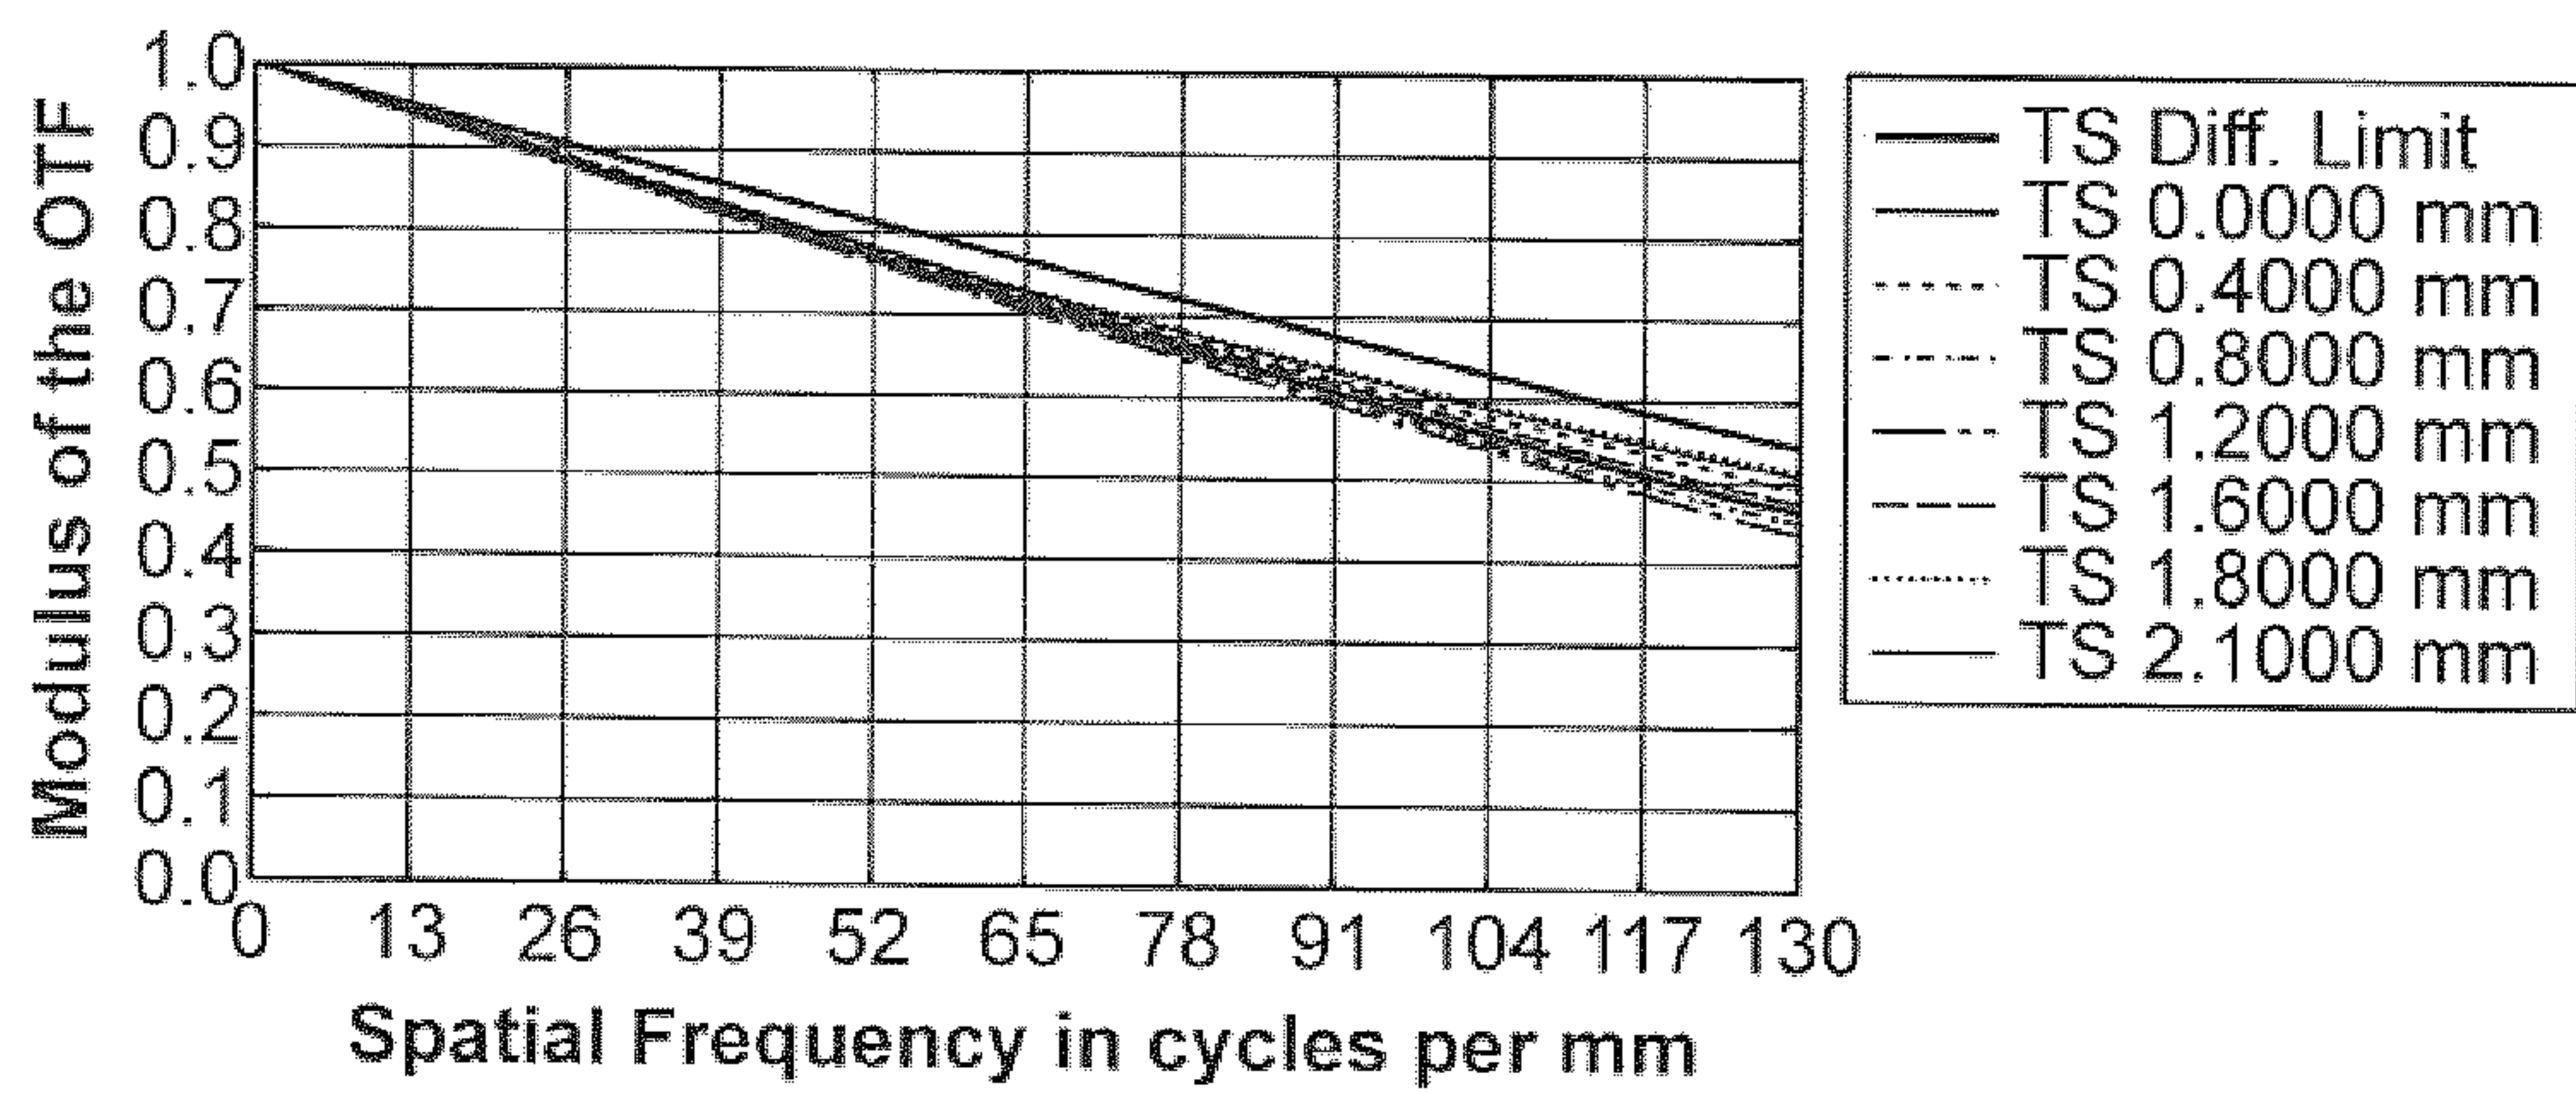


FIG. 6C

