


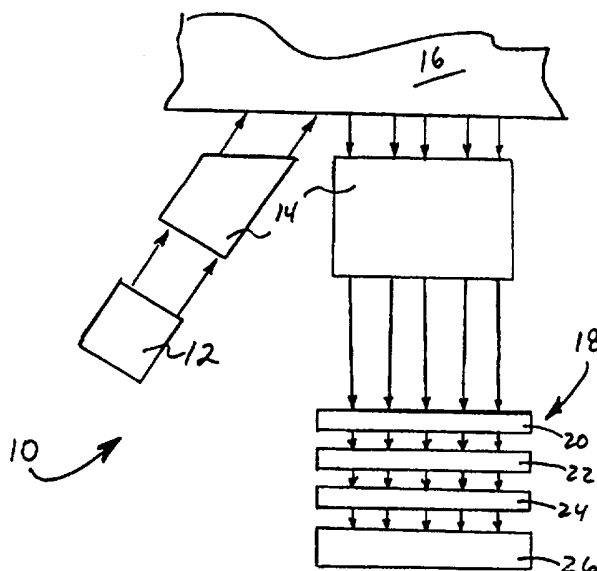

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : G01N 21/35, 21/31, A61B 5/00	A1	(11) International Publication Number: WO 97/28437 (43) International Publication Date: 7 August 1997 (07.08.97)
(21) International Application Number: PCT/US97/01369 (22) International Filing Date: 31 January 1997 (31.01.97) (30) Priority Data: 08/597,480 2 February 1996 (02.02.96) US (71) Applicant: INSTRUMENTATION METRICS, INC. [US/US]; Suite 102, 2085 Technology Circle, Tempe, AZ 85284 (US). (72) Inventors: MALIN, Stephen, F.; 16228 S. Fourth Street, Phoenix, AZ 85048 (US). KHALIL, Gamal; 17717 N.E. 24th Street, Redmond, WA 98008 (US). (74) Agents: REED, Dianne, E. et al.; Reed & Robins L.L.P., Suite 200, 285 Hamilton Avenue, Palo Alto, CA 94301 (US).		(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, HU, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, TJ, TM, TR, TT, UA, UG, UZ, VN, ARIPO patent (KE, LS, MW, SD, SZ, UG), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the</i> <i>claims and to be republished in the event of the receipt of</i> <i>amendments.</i>

(54) Title: METHOD AND APPARATUS FOR MULTI-SPECTRAL ANALYSIS IN NONINVASIVE INFRARED SPECTROSCOPY

**(57) Abstract**

A method and apparatus are described for determining the concentration of an analyte present in a sample using multi-spectral analysis in the near infrared and mid-infrared ranges. Incident radiation containing a plurality of distinct, nonoverlapping regions of wavelengths in the range of approximately 1100 to 5000 nm is used to scan a sample. Diffusively reflected radiation emerging from the sample is detected, and a value indicative of the concentration of the analyte is obtained using an application of chemometrics techniques. Information obtained from each nonoverlapping region of wavelengths can be cross-correlated in order to remove background interferences.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AM	Armenia	GB	United Kingdom	MW	Malawi
AT	Austria	GE	Georgia	MX	Mexico
AU	Australia	GN	Guinea	NE	Niger
BB	Barbados	GR	Greece	NL	Netherlands
BE	Belgium	HU	Hungary	NO	Norway
BF	Burkina Faso	IE	Ireland	NZ	New Zealand
BG	Bulgaria	IT	Italy	PL	Poland
BJ	Benin	JP	Japan	PT	Portugal
BR	Brazil	KE	Kenya	RO	Romania
BY	Belarus	KG	Kyrgyzstan	RU	Russian Federation
CA	Canada	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	KZ	Kazakhstan	SG	Singapore
CH	Switzerland	LI	Liechtenstein	SI	Slovenia
CI	Côte d'Ivoire	LK	Sri Lanka	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LT	Lithuania	SZ	Swaziland
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	LV	Latvia	TG	Togo
DE	Germany	MC	Monaco	TJ	Tajikistan
DK	Denmark	MD	Republic of Moldova	TT	Trinidad and Tobago
EE	Estonia	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	UG	Uganda
FI	Finland	MN	Mongolia	US	United States of America
FR	France	MR	Mauritania	UZ	Uzbekistan
GA	Gabon			VN	Viet Nam

5 METHOD AND APPARATUS FOR MULTI-SPECTRAL
ANALYSIS IN NONINVASIVE INFRARED SPECTROSCOPY

Technical Field:

10 The present invention relates to a method
and apparatus for determining the concentration of a
target analyte in a sample using multi-spectral
analysis. The invention finds application in a wide
range of chemical analyses, and particularly in
15 noninvasive spectrophotometric analysis of blood
analytes.

Background of the Invention:

 The measurement of the concentration of
20 various blood constituents finds application in a wide
variety of procedures for the diagnosis and treatment
of conditions and disease in human subjects. One
important application is in the measurement of blood
glucose. Specifically, the concentration of blood
25 glucose should be monitored on a periodic basis in
persons suffering from diabetes, and with respect to
insulin-dependent or Type I diabetes, it is often
necessary or desirable to monitor blood glucose
several times a day. Further, the measurement of
30 blood cholesterol concentrations provides important
information in the treatment or prevention of persons
suffering from coronary artery disease, and the
measurement of other organic blood analytes, such as
bilirubin and alcohol, is important in various
35 diagnostic contexts.

 The most accurate and widely practiced
method of obtaining blood analyte concentrations

involves the extraction of blood from a patient, which blood is then analyzed, either in a laboratory using highly accurate and sensitive assay techniques, or by the use less accurate self-testing methods. In particular, traditional blood glucose monitoring methods require the diabetic to draw a blood sample (e.g., by a finger-tip lance) for each test and to read the glucose level using a glucometer (a spectrophotometer that reads glucose concentrations) or a colorimetric calibration method. Such invasive blood extractions create a painful and tedious burden to the diabetic and expose the diabetic to the possibility of infection, particularly in light of the frequency of testing which is necessary. These considerations can lead to an abatement of the monitoring process by the diabetic.

Accordingly, there is a recognized need in the art for a simple and accurate method and device for noninvasively measuring blood analyte concentration, particularly in the context of blood glucose monitoring by diabetics. One approach to the problem entails the use of traditional methods of near infrared (near-IR or "NIR") analysis, wherein the measurement of absorbance at one or more specific wavelengths is used to extract analyte-specific information from a given sample.

Near-IR absorbance spectra of liquid samples contain a large amount of information about the various organic constituents of the sample. Specifically, the vibrational, rotational and stretching energy associated with organic molecular structures (e.g., carbon-carbon, carbon-hydrogen, carbon-nitrogen and nitrogen-hydrogen chemical bonds) produces perturbations in the near-IR region which can be detected and related to the concentration of various organic constituents present in the sample. However, in complex sample matrices, near-IR spectra

also contain an appreciable amount of interferences, due in part to similarities of structure amongst analytes, relative levels of analyte concentration, interfering relationships between analytes and the
5 magnitude of electronic and chemical "noise" inherent in a particular system. Such interferences reduce the efficiency and precision of measurements obtained using near-IR spectrometry to determine the concentration of liquid sample analytes. However, a
10 number of near-IR devices and methods have been described to provide noninvasive blood analyte determinations.

U.S. Patent No. 5,360,004 to Purdy et al. describes a method and apparatus for the determination
15 of blood analyte concentrations, wherein a body portion is irradiated with radiation containing two or more distinct bands of continuous-wavelength incident radiation. Purdy et al. emphasize filtration techniques to specifically block radiation at the two
20 peaks in the NIR absorption spectrum for water, occurring at about 1440 and 1935 nm. Such selective blocking is carried out in order to avoid a heating effect that may be due to the absorption of radiation by water in the body part being irradiated.

25 By contrast, U.S. Patent No. 5,267,152 to Yang et al. describes noninvasive devices and techniques for measuring blood glucose concentration using only the portion of the IR spectrum which contains the NIR water absorption peaks (e.g., the
30 "water transmission window," which includes those wavelengths between 1300 and 1900 nm). Optically controlled light is directed to a tissue source and then collected by an integrating sphere. The collected light is analyzed and blood glucose
35 concentration calculated using a stored reference calibration curve.

Devices have also been described for use in determination of analyte concentrations in complex samples.

For example, U.S. Patent No. 5,242,602 to
5 Richardson et al. describes methods for analyzing aqueous systems to detect multiple active or inactive water treating components. The methods involve determination of the absorbance or emission spectrum of the components over the range of 200 to 2500 nm,
10 and application of chemometrics algorithms to extract segments of the spectral data obtained to quantify multiple performance indicators.

U.S. Patent No. 5,252,829 to Nygaard et al. describes a method and apparatus for measuring the
15 concentration of urea in a milk sample using an infrared attenuation measuring technique. Multivariate techniques are carried out to determine spectral contributions of known components using partial least squares algorithms, principal component
20 regression, multiple linear regression or artificial neural network learning. Calibration is carried out by accounting for the component contributions that block the analyte signal of interest. Thus, Nygaard et al. describe a technique of measuring multiple
25 analyte infrared attenuations and compensating for the influence of background analytes to obtain a more accurate measurement.

U.S. Patent No. 4,306,152 to Ross et al. describes an optical fluid analyzer designed to
30 minimize the effect of background absorption (i.e., the overall or base level optical absorption of the fluid sample) on the accuracy of measurement in a turbid sample or in a liquid sample which is otherwise difficult to analyze. The apparatus measures an
35 optical signal at the characteristic optical absorption of a sample component of interest and another signal at a wavelength selected to approximate

background absorption, and then subtracts to reduce the background component of the analyte-dependent signal.

5 The accuracy of information obtained using the above-described methods and devices is limited by the spectral interference caused by background, i.e., non-analyte, sample constituents that also have absorption spectra in the near-IR range. Appreciable levels of background noise represent an inherent
10 system limitation, particularly when very little analyte is present. In light of this limitation, attempts have been made to improve signal-to-noise ratios, e.g., by avoiding water absorption peaks to enable the use of increased radiation intensity, by
15 reducing the amount of spectral information to be analyzed, or by using subtraction or compensation techniques based on an approximation of background absorption. Although such techniques have provided some improvement, there remains a need to provide a
20 method and apparatus capable of rendering a more precise determination of the concentration of analytes in a liquid matrix, particularly in the context of blood glucose monitoring.

25 Disclosure of the Invention

Accordingly, it is a primary object of the invention to address the above-described needs in the art, by providing a method of determining the concentration of an analyte present in a sample having
30 a varying background matrix and possibly having substantial component interferences as well. The method accounts for the similarity of structures among various components present in the sample, the relative magnitude of the analyte concentration and spectral
35 interferences provided by various sample components and instrumentation variances.

The method generally involves: (1) identifying several distinct, nonoverlapping regions of wavelengths in the near-IR, which have high correlation to the concentration of the analyte; (2) irradiating a sample with incident radiation containing those regions in order to obtain radiation that has been spectrally attenuated as a result of interaction with sample constituents; (3) detecting the spectrally attenuated radiation; (4) measuring the intensity of the spectrally attenuated radiation at a wavelength in nonoverlapping regions of wavelengths; and (5) correlating the measurements to obtain a value indicative of the concentration of the analyte.

In one aspect of the invention, a method is provided wherein spectral data from both the near infrared and the mid-infrared regions are analyzed to obtain analyte-specific information. Thus, the method involves the identification of several distinct, nonoverlapping regions of wavelengths in the near-IR and mid-IR regions, generally in the range of approximately 1100 to 5000 nm, which are substantially correlated with the concentration of the selected analyte or provide information about measurement and instrumentation parameters.

In another aspect of the invention, a method is provided which generally involves: (1) selecting several distinct, nonoverlapping regions of wavelengths in the near infrared range which have high correlation to the concentration of the analyte; (2) irradiating a sample using infrared light containing the selected spectral ranges to obtain spectrally modified radiation; (3) optically filtering the spectrally modified radiation to isolate or emphasize a portion of the radiation from each nonoverlapping region; (4) collecting and measuring the intensity of the optically filtered radiation using a detector; and (5) obtaining a value indicative of the analyte

concentration by applying a defined mathematical model to the optically filtered radiation.

It is also an object of the invention to provide a spectrophotometric apparatus for determining the concentration of an analyte present in a sample having a varying background matrix and substantial component interferences. The apparatus is configured to include an arrangement of detectors capable of collecting and measuring attenuated radiation reflected from a sample. The apparatus is used in a multi-spectral analysis to obtain spectral information containing analyte-specific signals as well as signals related to instrument background noise and interfering spectral information. Chemometrics techniques are used to configure filter elements capable of enhancing the correlation of analyte-specific information with the concentration of the analyte and to derive system algorithms capable of determining analyte concentration values. In one aspect of the invention, a diffraction grating system is used to obtain analyte-specific spectral information which is detected by a linear detector array capable of analyzing up to several hundred data points or wavelengths simultaneously.

25

Brief Description of the Figures

Figure 1 is a diagrammatic representation of an apparatus constructed according to the invention having a linear array of detectors capable of analyzing wavelengths in both the near infrared and mid infrared regions.

Figure 2 is a diagrammatic representation of an alternative apparatus constructed according to the invention.

Figure 3 is a graph illustrating time-dependent scans taken during an *in vivo* glucose tolerance study.

Figure 4 depicts in graph form the results obtained from a noninvasive determination of blood glucose concentration conducted using the method of the invention.

5

Modes for Carrying Out the Invention

Before the invention is described in detail, it is to be understood that this invention is not limited to the particular component parts of the devices or methods described, as such may vary. It is also to be understood that the terminology used herein is for purposes of describing particular embodiments only, and is not intended to be limiting. It must be noted that, as used in the specification and the appended claims, the singular forms "a," "an" and "the" include plural referents unless the context clearly dictates otherwise. Thus, for example, reference to "an analyte" includes mixtures of analytes, reference to "an optical transfer cell" includes two or more optical transfer cells, "a means for reflectively transmitting radiation" includes two or more such means, "a wavelength" includes two or more wavelengths, "a chemometrics algorithm" includes two or more algorithms, and the like.

In this specification and in the claims which follow, reference will be made to a number of terms which shall be defined to have the following meanings:

"Chemometrics" relates to the application of mathematical, statistical and pattern recognition techniques in chemical analysis applications. See, e.g., Brown et al. (1990) *Anal. Chem.* 62:84-101. Chemometrics is practiced herein in the context of developing and using noninvasive diagnostic instrumentation that employs advanced signal processing and calibration techniques. Signal processing is used to improve the accessibility of

physically significant information in analytical signals. Examples of signal processing techniques include Fourier transformation, first and second derivatives, and digital or adaptive filtering.

5 In the context of chemometrics, "calibration" refers to the process of relating data measurements to a chemical concentration for the purpose of quantification. Particularly, statistical calibrations using chemometric methods can be used to
10 extract specific information from a complex set of data. Such methods of calibration include linear regression, multiple-linear regression, partial linear regression, and principal components analysis. In other applications, calibrations can be carried out
15 using artificial neural networks, genetic algorithms and rotated principal components analysis.

Instrumentation that detects information for one or more constituents in a complex chemical matrix must rely upon analysis algorithms (such as those
20 derived using chemometrics) in order to reveal information that is specific for one or more chemical constituent. Chemometrics techniques can be used to compare unknowns with calibrated standards and data bases to provide advanced forms of cluster analysis,
25 and to extract features from an unknown sample that can be used as information in statistical and mathematical models.

"Principal components analysis" (PCA) is one method of data reduction which can be performed in the
30 application of chemometric techniques to spectroscopic measurement of chemical analytes in a complex matrix. PCA is used to reduce the dimensionality of a large number of interrelated variables while retaining the information that distinguishes one component from
35 another. This reduction is effected using an eigenvector transformation of an original set of interrelated variables (e.g., an absorption spectrum)

into a substantially smaller set of uncorrelated principal component (PC) variables that represents most of the information in the original set. The new set of variables is ordered such that the first few
5 retain most of the variation present in all of the original variables. See, e.g., Jolliffe, L.T., *Principal Component Analysis*, Springer-Verlag, New York (1986). More particularly, each PC is a linear combination of all the original measurement variables.
10 The first is a vector in the direction of the greatest variance of the observed variables. The succeeding PCs are chosen to represent the greatest variation of the measurement data and to be orthogonal to the previously calculated PC. Therefore, the PCs are
15 arranged in descending order of importance.

The term "weighting constant" includes the wavelength coefficients of partial least squares regression and/or principal components regression, or any constant obtained from any statistical calibration
20 that can be used to calculate values (such as analyte concentration) for unknown samples. A "wavelength weighting factor" is an embodiment of a weighting constant which is used in the construction of an optical filter means capable of emphasizing
25 wavelength-specific information from spectral data. The wavelength-specific information can be used to determine desired values relating to the sample undergoing analysis (e.g., analyte concentration). A wavelength weighting factor can be embodied as a
30 particular filter density (e.g., neutral or wavelength-specific), filter thickness, or the like, such parameters having been determined using the above-described statistical calibration techniques.

An optical filter means that embodies a
35 wavelength weighting factor can be used to selectively emphasize wavelengths having high correlation with a selected analyte concentration. "High correlation" or

"close correlation" refers to the quantitative association between the absorption spectrum at a particular wavelength and a particular analyte concentration, wherein the two variables have a correlation coefficient (r) of 0.9 or higher.

A "neutral density filter" refers to a standard optical filter means having a flat absorption spectrum. A neutral density filter can be used in concert with correlation filters in a filter system to provide a weighting factor to attenuate absorbance due to the analyte at selected wavelengths and further improve the accuracy of the correlation provided by the system. A neutral density filter can have an absorption spectrum sufficient to attenuate radiation equally at all wavelengths in the range of interest.

As used herein, an "aqueous medium" encompasses any composition containing water. Generally, an aqueous medium herein contains water as the major component, i.e., water is present in an amount of at least about 50 vol.%. Such aqueous media include, for example mammalian tissue.

The term "blood analyte" refers to a blood constituent that is absorbing in the near-IR range, the measurement of which is useful in patient monitoring or in the provision of health care.

As used herein, the term "near infrared" or "near-IR" encompasses radiation in a spectrum ranging from approximately 660 nm to 3500 nm, but typically in the range of approximately 1050 to 2850 nm, and more typically in the range of approximately 1100 to about 2500 nm.

The term "mid-infrared" or "mid-IR" encompasses radiation in a spectrum ranging from about 3501 nm to about 6000 nm.

The term "background absorption" relates to the overall or base level of optical absorption of an aqueous sample which is to be analyzed, from which the

absorption of a selected constituent departs at one or more characteristic wavelengths to an extent indicative of the concentration of the selected constituent. When the level of background absorption is high in relation to the characteristic absorption of the selected constituent, such as in complex aqueous media where numerous interfering constituents are found, accurate measurement of the magnitude of a slight change in the absorption at the characteristic wavelength of a constituent of interest requires application of the chemometrics techniques described herein. This is particularly so in applications wherein the overall concentration of the constituent of interest is low relative to the aqueous medium, e.g., in the measurement of blood analytes.

General Methods

A spectrophotometric method is provided for determining the concentration of an analyte in a liquid sample using near- and mid-IR radiation. In contrast to prior techniques, the present method uses all of the spectral information contained in the near-IR region in order to obtain a set of measurements that can be used to determine an analyte concentration with a heightened degree of accuracy.

The method includes the steps of (1) selecting several distinct, nonoverlapping regions of wavelengths in the near-IR range, generally spanning 1100-3000 nm, or from the near-IR range and the mid-IR range, generally spanning 3501-5000 nm, wherein each region defines a spectral range, (2) irradiating a sample using infrared light containing the selected spectral ranges to obtain spectrally modified radiation which has been attenuated, (3) collecting and measuring the intensity of the spectrally attenuated radiation at one or more wavelengths contained within each of the selected spectral ranges,

and (4) correlating those measurements to obtain a value indicative of the analyte concentration.

Spectral information obtained using this method can be subjected to a combination of
5 mathematical transformations to arrive at a precise analyte concentration value. For example, standard statistical techniques, such as partial least squares (PLS) analysis, or principal components regression (PCR) analysis, can be used to correlate the
10 absorbance of radiation at specific wavelengths to analyte structure and concentration. PLS techniques are described, for example, in, Geladi et al. (1986) *Analytica Chimica Acta* 185:1-17. For a description of PCR techniques, reference may be had to Jolliffe,
15 L.T., *Principal Component Analysis*, Springer-Verlag, New York (1986).

Accordingly, in determining blood analyte concentration from a body tissue sample, one method involves the selection of three nonoverlapping regions
20 of wavelengths in the near infrared, generally in the range of approximately 1100 to 3500 nm. Preferably, although not necessarily, the first region is within the range of 1100 to 1350 nm, the second region is in the range of 1430 to 1450 nm or 1930 to 1959 nm, and
25 the third region is in the range of 2000 to 2500 nm, wherein each region defines a "spectral range." The first region contains wavelengths in which proteins and other cellular components exhibit dominant spectral activity, the second region is dominated by
30 the absorption spectrum of water, and the third region contains wavelengths in which organic analyte molecules exhibit significant spectral activity. These constituents also contribute to the absorption spectra in those regions where they are not the
35 dominant species. Accordingly, the spectrally attenuated radiation obtained from each region contains a large amount of interrelated information

that must be reduced using statistical methods to obtain analyte-specific information.

The invention also involves the use of signal processing to improve the accessibility of physically significant information in the analytical signals. The intensity values of signals obtained at particular wavelengths can thus be processed to reduce the effect of instrumentation noise. The processed signals are then subjected to multivariate analysis using known statistical techniques.

The PCA method of data reduction is one preferred method used in the practice of the invention to reduce the dimensionality of a large number of interrelated variables while retaining information that distinguishes one component from another. Data reduction is carried out using an eigenvector transformation of an original set of interrelated variables (e.g., the absorption spectrum) into a substantially smaller set of uncorrelated principal component (PC) variables that represents most of the information in the original set. The new set of variables is ordered such that the first few retain most of the variation present in the original set.

The principal component vectors can be transformed by orthogonal rotation against an average value for the absorbance to obtain both a known wavelength and the relative value of the absorbance at that wavelength which is attributable to the analyte. By performing this analysis on information obtained from each of the three spectral regions, cross-correlating the principal component vectors via a linear algorithm, and using subtractive methods to remove the effect of interfering analytes, values are obtained which can be used in a system algorithm to determine the concentration of the analyte.

Multivariate techniques are used to provide a model that relates the intensity of radiation at

specific wavelengths in each spectral region to
analyte concentrations in a particular sample matrix,
e.g., body tissue. The model is constructed using two
sets of exemplary measurements that are obtained
5 simultaneously, the first set of measurements, the
"prediction set," comprising spectral data, e.g.,
radiation intensity at selected wavelengths, and the
second set of measurements, the "calibration set,"
comprising highly accurate analyte concentrations that
10 have been determined using invasive sampling
techniques. The procedure is carried out over a range
of analyte concentrations to provide calibration and
prediction data sets.

Measurements obtained in both the
15 calibration set and the prediction set are subjected
to multivariate analysis, such as by the use of
commercially available multivariate model developing
software programs, to provide an initial model. The
initial model is applied to the prediction data to
20 derive analyte concentration values that can be
compared to the values obtained by the invasive
techniques. By iteratively performing the above
steps, a refined mathematical model is developed which
can be used to establish a system algorithm for use in
25 analyzing data obtained by the methods of the
invention.

In the practice of the invention, non-
analyte specific information from the various
nonoverlapping spectral regions can be used, for
30 example, to normalize each spectral scan, to subtract
background and base line interferences, or to provide
signal values used to detect an inaccurate
measurement.

When determining a blood analyte
35 concentration in a body tissue sample, measurements
taken in the spectral range spanning approximately
1320 - 1340 nm provide a highly reflected,

unattenuated, signal, as there are no major absorption bands present in the region. By collecting and measuring the intensity of radiation in that range, a value is obtained which can be used to estimate the actual intensity of the near-IR light used to irradiate the sample. The value can be used to normalize each individual scan and to correct for fluctuations in the intensity of the light source which could effect the accuracy of analyte concentration values obtained using the method of the invention.

Additionally, measurements taken in the spectral ranges spanning approximately 1430 - 1450 nm and approximately 1930 - 1950 nm provide substantially non-reflected, highly attenuated, signals, as a result of the two dominant absorption peaks occurring at about 1440 and 1935 nm in the near-IR absorption spectrum for water. By collecting and measuring the intensity of radiation in one or both of those ranges, a value is obtained which can be used to estimate the intensity of near-IR light that is not totally absorbed by the irradiated sample. The value can be used to subtract background or base-line information from the analyte-specific signals obtained in other regions and/or to provide an internal reference to detect inaccurate measurements. The value can be subtracted from each spectral measurement obtained using the present method in order to correct for the pedestal effect caused by specular reflection which varies with skin texture and age.

Measurements of substantially unattenuated signals obtained from a first region (e.g., the spectral range spanning approximately 1320 - 1340 nm) and measurements of highly attenuated signals obtained from a second region (e.g., the spectral ranges spanning approximately 1430 - 1450 nm and approximately 1930 - 1950 nm) can also be used to

compare diffusely reflected radiation with specular radiation. If the signals in the two regions have relatively comparable values, it is likely that most of the radiation used to irradiate the tissue sample
5 was reflected from the skin surface, and thus failed to penetrate the skin to interact with the blood analytes. This information can be used to identify ineffective measurements arising from a failure to obtain a proper instrumentation scan of the tissue
10 sample.

In one aspect of the invention, a method of determining the concentration of an analyte in a sample is provided using non-invasive measurements obtained in several distinct, nonoverlapping regions
15 of wavelengths in the infrared region and an optical processing system that is particularly suited for field or home applications. The method generally involves the steps of (1) selecting several distinct, nonoverlapping regions of wavelengths from the near-IR range, preferably spanning 1100-3000 nm, or from the
20 near-IR range spanning 1100-3500 nm and the mid-IR range spanning 3501-5000 nm, wherein each region defines a spectral range, (2) irradiating a sample using infrared light containing the selected spectral ranges to obtain spectrally modified radiation, i.e.,
25 reflected radiation, (3) optically filtering the spectrally modified radiation to isolate or emphasize a portion of the radiation from each nonoverlapping region, (4) collecting and measuring the intensity of the optically filtered radiation using a detector, and
30 (5) obtaining a value indicative of the analyte concentration by applying a defined mathematical model to the optically filtered radiation. The mathematical model can comprise a correlation algorithm obtained
35 using the above-described chemometrics techniques.

The method of the invention can be carried out using a number of spectrophotometer

configurations. Referring now to Figure 1, one particular apparatus for determining the concentration of an analyte in a liquid sample is generally indicated at 10. The apparatus includes a radiation source 12 which provides a plurality of distinct, nonoverlapping regions of wavelengths in the range of approximately of 1100 to 5000 nm. A number of suitable radiation sources are known in the art and can be used herein, e.g., incandescent light sources directed across interference filters, halogen light sources modulated by an associated chopper wheel, laser light sources, laser diode arrays, or high speed light-emitting diode (LED) arrays. In one particular apparatus, the radiation source 12 provides radiation at three distinct regions of wavelengths, specifically a first region of wavelengths in the approximate range of 1100 to 1350 nm, a second region in the approximate range of 1930 to 1950 nm and a third region in the approximate range of 2000 to 3500 nm.

The apparatus 10 also includes sample interface optic means 14 which launches incident radiation from the radiation source into contact with a sample medium 16 containing an analyte. After contacting the sample medium, spectrally modified radiation emerging from the sample as diffusively reflected light is collected and delivered to a multi-stage filter means, generally indicated at 18.

In various configurations, the sample interface optic means 14 can be designed to enable the close interface of the apparatus 10 with the medium 16, such as where the launch is carried out by placing the apparatus in direct contact with the sample medium, thereby bringing the radiation source into close proximity with the sample to be analyzed. After the launch, the reflected radiation is collected using optically active means, such as light converging means or beam deflection optics. Alternatively, the sample

interface optic means 14 can comprise fiber optic waveguides coupled to the apparatus in order to enable remote apparatus placement and operation. Other configurations are provided wherein a single fiber optic bundle is employed to transmit the radiation to and from the medium. An optrode disposed at the end of the single bundle transmits the near-IR radiation to the sample medium 16 and receives spectrally modified radiation therefrom which is directed back through the bundle to the apparatus 10. Sapphire or high-grade quartz can be used as optical elements in the above fiber optic waveguides, as those materials have very good transmission characteristics in the near-IR spectral range.

Referring still to Figure 1, the reflected light emerging from the sample 16 passes to the multi-stage filter means 18. Specifically, the light passes to a first stage comprising an adjustable filter means 20 which is capable of having its absorption characteristics adjusted in response to a signal that is either externally generated, or that has been generated by the apparatus 10. The adjustable filter means generally comprises a screen filter, such as a neutral density filter, having absorption characteristics that are adjusted to variably attenuate the intensity of radiation as dictated by an external signal or system command. The degree of attenuation provided by the adjustable filter means 20 is based upon a predetermined factor selected to ensure that radiation emitted from the adjustable filter will be at a constant value regardless of the intensity of the pre-filtered radiation.

Attenuated radiation emerging from the adjustable filter means 20 is communicated to a principal analyte filter 22 which has optical characteristics capable of selectively passing one or more wavelengths from each of the distinct

nonoverlapping regions of wavelengths launched by the radiation source 12. The wavelengths passed by the principal analyte filter are selected to have a correlation with the concentration of the analyte.

5 A second filter means 24 is arranged in the apparatus 10 relative to the principal analyte filter 22 such that selectively passed wavelengths emerging from the principal analyte filter interact with the second filter means. The second filter means has
10 absorption characteristics selected such that the intensity of each passed wavelength is attenuated by the second filter means. The attenuations provided by the second filter means can be determined, for example, by an independent set of weighting factors
15 derived using chemometrics techniques.

 In one particular configuration, the weighting factors are determined using a partial least squares or principal component regression of an original spectrum obtained from a sample containing
20 the analyte. The second filter means 24 can be constructed using a suitable substrate layer that is capable of transmitting radiation at least in the 1100 to 5000 nm range. The substrate layer is generally coated with one or more layers of metals and/or oxides
25 that are conventional in the art to provide a plurality of second filter densities. Such coatings can be applied to the substrate using emulsion or chemical vapor deposition (CVD) techniques well known in the art. In an alternative apparatus, the second
30 filter means is a photographic mask having spectral lines of optical density that are proportional to weighting functions determined using a rotated principal components or least squares analysis technique.

35 After attenuation by the second filter means, the independent wavelengths are communicated with a detection means 26, such as one or more Lead

Sulfide (PbS) detectors, Gallium Arsenide detectors, or the like. In one particular apparatus configuration wherein it is desired to obtain measurements over the entire range of from about 1100 to 5000 nm, one or more Lead Selenide (PbSe) detectors can be used.

The detection means 26 detects and converts the attenuated wavelengths emitted from the second filter means into a signal which can then be applied toward an analyte specific algorithm to determine analyte concentration. Specifically, signals obtained from the second detection means can be readily converted into digital signals using an analog/digital converter. The digitized information is readily available for input into a microprocessor, or other electronic memory means, where it is used to provide an analyte concentration which can be visualized on a display device and/or recorded on an output recorder.

In an alternative configuration, the apparatus 10 can include a diffraction grating system and a linear detector array in place of the multi-stage filter means 18. Reflected light emerging from the sample 16 can be passed to a diffraction grating system configured to selectively pass discrete wavelengths therefrom, wherein the passed wavelengths are specifically correlated with the concentration of the analyte. The passed wavelengths are then communicated to a linear detector array, such as a PbS-based linear detector array or the like. In particular applications for obtaining measurements over the entire range of from about 1100 to 5000 nm, a PbSe-based linear detector array can be used. PbSe linear arrays can be obtained, for example, under the tradename MULTIPLEXIR™ (available from Graseby Infrared, Orlando, Fla.).

As described above, the linear detector array collects and measures the wavelengths passed by

the diffraction grating system to provide signals which can be applied toward an analyte specific algorithm to determine analyte concentration.

The apparatus 10 can be used to obtain
5 measurements of analyte concentration in a variety of complex media, such as in aqueous media having complex spectral backgrounds. In one application, the apparatus can be used in the determination of blood analyte concentrations, particularly organic blood
10 analytes such as, but not limited to, glucose, urea (BUN), lipids, bilirubin and alcohol. The blood analyte can be present in an *in vitro* sample medium (e.g., a blood sample), or the apparatus can be used to measure blood analytes in tissue. However, the
15 apparatus 10 is particularly adapted for use in field applications, e.g., in the measurement of blood alcohol, or in home health monitoring, e.g., in blood glucose determination.

Referring now to Figure 2, an alternative
20 apparatus for determining the concentration of an analyte in a sample is indicated at 50. The apparatus includes a radiation source 52 which provides a plurality of distinct, nonoverlapping regions of wavelengths in the approximate range of 1100 to
25 approximately 5000 nm. The apparatus 50 also includes sample interface optic means 54 which launches incident radiation from the radiation source into contact with a sample medium 56 containing an analyte. After contacting the sample medium, spectrally
30 modified radiation emerging from the sample as diffusively reflected light is collected and delivered to a filter means 58 which is configured to pass light of specific wavelengths.

In operation, incident radiation is launched
35 from the source 52 to the sample medium via sample interface optic means which, in one configuration, can be designed to enable the close interface of the

apparatus with the particular sample medium being analyzed. After the launch, reflected radiation is collected using optically active means, such as a light converging means (i.e., a lens) or beam deflection optics. The sample interface optic means 54 can comprise fiber optic waveguides coupled to the apparatus 50 which enable remote apparatus placement and operation. As described above, one alternative system uses a single fiber optic bundle to transmit radiation to and from the medium.

The reflected radiation is directed to a filter means 58 which includes a plurality of discrete filter elements, indicated at $\lambda_1, \lambda_2, \lambda_3, \dots \lambda_n$. The filter means 58 passes a population of selected wavelength ranges which provide analyte-specific information, information about the measurement background and information that can be used to correct for instrument changes or interference effects. The selected wavelengths emerging from the filter means are detected by an arrangement of detectors 60, having a plurality of discrete detector units generally indicated at $D_1, D_2, D_3, \dots D_n$. The detectors are arranged such that each selected wavelength range emerging from the filter means is detected by a single, discrete detector. Suitable detector configurations are known in the art and can include, for example, an arrangement of PbS or PbSe detectors. Each detector converts the detected radiation into an electrical signal which can be used to obtain a value indicative of analyte concentration.

Signals obtained from the detectors can be readily converted into digital signals, e.g., digital signals indicative of the intensity of the detected wavelengths, using an analog/digital converter. The digitized information is then available for input into a microprocessor for further processing (e.g., applied to a system algorithm), or the information can be

visualized via an electronic display means. Analog signals obtained from each discrete detector are communicated to an analog/digital (A/D) converter for conversion to digital form. The analog signals may be pre-amplified prior to conversion using techniques known in the art. Digital information from the A/D converter is then readily input into a microprocessor to calculate the analyte concentration using a system algorithm that is specific for the analyte. The microprocessor calculates analyte concentration by application of a chemometrics algorithm to the detected signals. Analyte-specific algorithms can be determined using iterative calibration and statistical modeling techniques, such as the above-described chemometrics methods.

In the practice of the invention, the filter means 58 can be constructed to include at least one discrete filter element having an absorption characteristic capable of providing enhanced correlation of the passed wavelength with the concentration of the analyte. Specifically, the filter means can include one or more filter elements which attenuate the intensity of a passed wavelength as determined, for example, by an independent set of weighting factors derived using chemometrics techniques. Such weighting factors can be derived using a partial least squares or principal component regression of an original spectrum obtained from a sample containing the analyte.

In another alternative configuration, the filter means 58 comprises a two-stage filter, the first stage includes a plurality of sections configured to selectively pass a population of selected wavelength ranges from the attenuated radiation reflected from the sample. The selectively passed wavelengths include analyte-specific information, information about the measurement

background and information that can be used to correct for instrument changes or interference effects. The second stage of the filter is arranged directly adjacent to the first stage, and serves to attenuate the intensity of each of the passed wavelengths emerging from the first stage. The second stage of the two-stage filter means can be a neutral density filter having a flat absorption spectrum that is sufficient to equally attenuate the intensity of each of the passed wavelengths emerging from the first stage of the filter.

The apparatus 50 can be used to ascertain the concentration of one or more analytes of interest present in a variety of complex mediums, such as in an aqueous medium having a complex spectral background. Specifically, the apparatus can be used in the determination of blood analyte concentrations, particularly organic blood analytes such as, but not limited to, glucose, urea (BUN), lipids, bilirubin and alcohol. As described above, analysis of blood analyte concentrations can be conducted using *in vitro* samples, or an analysis can be carried out using a near-IR scan of tissue, such as reflective measurements obtained from a forearm tissue scan.

When the apparatus 50 is used to obtain blood analyte measurements from a tissue source, incident radiation launched from the source 52 via sample interface optic means 54 is caused to impinge upon the skin surface of tissue, such as upon a subject's forearm. The sample interface optic means directs the radiation at an angle toward the tissue such that it is absorbed by the tissue material near the surface and reflected as diffuse radiation. The incident radiation is spectrally modified as a result of infrared absorptions by the blood and tissue constituents. Portions of the incident near-IR radiation are absorbed, dispersed, diffused and

reflected from the blood constituents present within the tissue source. This spectrally modified radiation contains information specific for each optically active blood constituent.

5 In determining blood glucose levels using the apparatus 50, vibrational motions of blood glucose molecules can be detected and measured using diffuse-reflective near-IR radiation. The vibrational motion includes both rotational and translational motion of
10 the glucose molecules, including overtone vibrations and combined vibrations. Of these motions, the overtone vibrations are dominant and occur in the range of approximately 1670 to 1690 nm. The glucose combination vibration bands occur in the range of
15 approximately 2120 to 2280 nm. Glucose does not have significant optical activity in the near-IR range of approximately 1320 to 1340 nm.

Accordingly, the apparatus 50 can include a filter means 58 having four distinct sections, where
20 the first section is configured to pass reflected radiation from the region of wavelengths in the range of approximately 1300 to 1360 nm, the second section is configured to pass reflected radiation from the region of wavelengths, either in the range of
25 approximately 1430 to 1450 nm, or approximately 1930 to 1950, the third section is configured to pass reflected radiation from the region of wavelengths in the range of approximately 1670 to 1690, and the fourth section is configured to pass reflected
30 radiation from the region of wavelengths in the range of approximately 2120 to 2280 nm.

The intensity of wavelengths passed by the third and fourth sections of the filter means contains analyte-specific information. As described above, the
35 third and fourth filter sections can be configured to include weighting factors which enhance the correlation of the passed radiation with the

concentration of glucose present in the tissue sample. Information obtained from the first section of the filter can be used to estimate the background spectral contributions in each measurement, and can thus be
5 used to correct or normalize the measurements obtained from the third and fourth filter sections. The signals obtained from the second filter section (the water absorption information) can be used as an internal check to identify ineffective measurements,
10 e.g., those arising from a failure to obtain a proper instrumentation scan of the tissue sample, or the information can be used to correct for temperature changes in the measurements obtained from the third and fourth filter sections.

15

It is to be understood that while the invention has been described in conjunction with
20 preferred specific embodiments thereof, the foregoing description, as well as the examples which follow, are intended to illustrate and not limit the scope of the invention. Other aspects, advantages and modifications within the scope of the invention will
25 be apparent to those skilled in the art to which the invention pertains.

Example

A noninvasive glucose measurement was
30 obtained using the method of the invention. Particularly, reflective optical measurements in the near-IR region of approximately 1100 nm to 3500 nm were carried out. Spectral scans were collected from volunteer forearm subjects, using an instrument having
35 a Tungsten-Mercury (W-Hg) radiation source, a Lead Sulfide (PbS) detector and a scan speed of nm / 0.4 second.

A number of specific spectral ranges were identified as containing information which can be used to determine glucose concentration from a forearm tissue scan. The specified regions were determined from an *in vivo* glucose tolerance study conducted in tandem with invasively obtained *in vitro* blood glucose concentration determinations. In particular, time-dependent scans taken during the *in vivo* tolerance study are depicted in Figure 3. As can be seen, significant changes in the reflective intensity differences over the range of about 2120 to 2180 nm were recorded during the time course of the study. These changes increased in direct relation to increases in blood glucose level during the tolerance test, signifying that the range of 2120 to 2180 nm contains glucose-specific spectral information.

Once the specific spectral ranges were identified, noninvasive glucose measurements were obtained using information from the four distinct spectral ranges. The first spectral range included radiation occurring at about 1320 to 1340 nm. This range provides a very highly reflected signal, and there is no major glucose absorption band in this range. Information obtained from the first spectral range can be used to normalize each individual scan in order to correct for fluctuations in the radiation source, and changes due to mechanical perturbations.

The second spectral range included radiation occurring at either about 1440 to 1460 nm, or about 1940 to 1960 nm. These ranges provide a substantially non-reflected signal due to the highly absorptive water bands which attenuate diffusively reflected radiation. Information obtained from these ranges can be used for background and base line subtraction from other measurements. These measurements allow for a pedestal adjustment to account for fluctuations induced by

specular reflection signal values, and can be used to detect improper measurements.

The third range included radiation occurring at about 1670 to 1690 nm. This range provides
5 analyte-specific information due to the presence of glucose vibrational overtone bands.

The fourth range included radiation occurring at about 2120 to 2280 nm. This range provides analyte-specific information due to glucose
10 combination vibrational bands.

Signals obtained from the first range were used to normalize signals of other regions. This process, when repeated with each spectral scan, eliminates the problem associated with light source
15 changes and serves to provide an internal reference. Measurement variations induced by differences in optical interface, e.g., patient placements, were accordingly substantially reduced.

Background information was eliminated by
20 subtracting the signals obtained in the second range, from the signals obtained in the third and fourth analyte-specific ranges. In this manner, the pedestal effect created by specular reflection, which varies with skin texture and age, was corrected for.

25 The normalized and base line corrected signals from the third and fourth ranges were applied in an analytical chemometric analysis. Figure 4 depicts the normalized differences between signals in the second and third ranges.

30 As can be seen by the results depicted in Figure 4, increase in blood glucose level results in an increase in the signal differences between the two ranges.

35

Claims:

1. A method of determining the
5 concentration of an analyte in a sample, comprising:
 - (a) determining a plurality of distinct,
nonoverlapping regions of wavelengths within the near-
and mid-IR spectral ranges and having high correlation
to the concentration of the analyte, each of said
10 regions corresponding to a spectral analysis range;
 - (b) irradiating the sample using infrared
light containing the selected spectral ranges to
obtain spectrally modified radiation in each spectral
analysis range;
 - 15 (c) optically filtering the spectrally
modified radiation to isolate or emphasize a portion
of the radiation from each range;
 - (d) collecting and measuring the intensity
of the optically filtered radiation using a detector
20 means; and
 - (e) obtaining a value indicative of the
analyte concentration by applying a mathematical model
to the optically filtered radiation.
- 25 2. The method of claim 1, wherein the step
of optically filtering the spectrally modified
radiation comprises passing said radiation through
optical filter means having absorption characteristics
capable of selectively passing discrete wavelengths
30 from each spectral range, wherein said discrete
wavelengths are specifically correlated with the
concentration of the analyte.
3. The method of claim 2, wherein the
35 absorption characteristics of the optical filter means
are derived using chemometrics techniques.

4. The method of claim 1, wherein the detector means comprises a plurality of detectors.

5. The method of claim 4, wherein the detectors are comprised of lead selenide.

6. The method of claim 1, wherein the sample is comprised of body tissue and the analyte is an organic blood analyte.

10

7. The method of claim 6, wherein the blood analyte is selected from the group consisting of glucose, urea (BUN), lipids, bilirubin and ethyl alcohol.

15

8. The method of claim 7, wherein the blood analyte is glucose.

9. A method of determining the concentration of an analyte in a sample, comprising:

20 (a) determining a plurality of distinct, nonoverlapping regions of wavelengths within the near- and mid-IR spectral ranges and having high correlation to the concentration of the analyte, each of said regions corresponding to a spectral analysis range;

25 (b) irradiating the sample with near infrared light containing the spectral analysis ranges determined in step (a), wherein the irradiating gives rise to both spectrally attenuated radiation and spectrally unattenuated radiation emerging from the sample, said spectrally attenuated radiation having wavelengths in each of the spectral analysis ranges;

30 (c) collecting the spectrally attenuated radiation;

35 (d) measuring the intensity of the collected spectrally attenuated radiation at a predetermined

wavelength in each of the spectral analysis ranges;
and

(e) correlating the measurements obtained in
step (d) to obtain a value indicative of the
5 concentration of the analyte.

10. The method of claim 9, wherein the near
infrared light contains a first spectral analysis
region of wavelengths in the range of approximately
10 1100 to 1350 nm, a second spectral analysis region of
wavelengths in the range of approximately 1550 to 1850
nm, and a third spectral analysis region of
wavelengths in the range of approximately 2000 to 3500
nm.

15

11. The method of claim 10, further
comprising the steps of collecting and measuring the
intensity of the spectrally unattenuated radiation
emerging from the sample, wherein said unattenuated
20 radiation is from the first spectral analysis region
and contains wavelengths in the range of approximately
1320 to 1340 nm.

12. The method of claim 11, wherein the
25 value obtained in the measurement of the unattenuated
radiation is used to estimate the intensity of the
near infrared light used in step (b).

13. The method of claim 10, wherein the
30 spectrally attenuated radiation includes highly
attenuated radiation.

14. The method of claim 10, further
comprising the steps of collecting and measuring the
35 intensity of highly attenuated radiation emerging from
the sample, wherein said highly attenuated radiation
is selected from a band of wavelengths corresponding

to a peak in the spectrum of radiation absorption by water.

15. The method of claim 14, wherein the
5 value obtained in the measurement of the highly attenuated radiation is used to estimate the intensity of the near infrared light not absorbed by the irradiated sample.

10 16. The method of claim 15, wherein the selected band of wavelengths is in the range of approximately 1430 to 1450 nm.

15 17. The method of claim 15, wherein the selected band of wavelengths is in the range of approximately 1930 to 1950 nm.

18. An apparatus for determining the concentration of an analyte in a sample, comprising:
20 (a) means for irradiating the sample with incident radiation containing a plurality of distinct, nonoverlapping regions of wavelengths in the near- and mid-IR spectral ranges;
(b) means for collecting reflected
25 radiation emerging from the sample and directing said reflected radiation into a beam path;
(c) adjustable filter means disposed in the beam path, wherein said adjustable filter means attenuates the intensity of radiation in the beam
30 path;
(d) principal analyte filter means capable of receiving attenuated radiation emerging from the adjustable filter means, and selectively passing discrete wavelengths therefrom, wherein said discrete
35 wavelengths are specifically correlated with the concentration of the analyte;

(e) second filter means capable of receiving the discrete wavelengths emerging from the principal analyte filter means and attenuating the intensity of said wavelengths;

5 (f) detection means for receiving the attenuated wavelengths emerging from the second filter means; and

(g) means for converting the detected wavelengths into a signal representative of the
10 intensity of said wavelengths.

19. The apparatus of claim 18, wherein the adjustable filter means comprises a neutral density filter.

15

20. The apparatus of claim 18, wherein the second filter means comprises a neutral density filter.

20 21. The apparatus of claim 20, wherein the attenuation provided by the second filter means is established using weighting factors.

22. The apparatus of claim 21, wherein the
25 weighting factors are derived using chemometrics techniques.

23. The apparatus of claim 22, wherein the weighting factors are derived using rotated principal components analysis of an absorption spectrum of the
30 analyte.

24. The apparatus of claim 18, wherein the detector means comprises a lead selenide detector.

35

25. The apparatus of claim 18, wherein the incident radiation is in the range of approximately 1100 to 5000 nm.

5 26. An apparatus for determining the concentration of an analyte in a sample, comprising:

 (a) means for irradiating the sample with incident radiation containing a plurality of distinct, nonoverlapping regions of wavelengths in the near- and
10 mid-IR spectral ranges;

 (b) means for collecting reflected radiation emerging from the sample and directing said reflected radiation into a beam path;

 (c) filter means disposed in the beam path,
15 said filter means comprising a plurality of sections configured to selectively pass at least one wavelength from the reflected radiation emerging from the sample;

 (d) a plurality of detectors arranged such that each wavelength emerging from the filter means is
20 detected by a discrete detector; and

 (e) means for converting the detected wavelengths into a signal representative of the intensity of said wavelengths.

25 27. The apparatus of claim 26, wherein the filter means comprises a two-stage filter having a first stage comprising a plurality of sections configured to selectively pass at least one wavelength from the reflected radiation emerging from the sample,
30 a second stage arranged adjacent to the first stage and capable of attenuating the intensity of each selectively passed wavelength emerging from the first stage of the filter means.

35 28. The apparatus of claim 27, wherein the second stage of the two-stage filter means is a neutral density filter.

29. The apparatus of claim 26, wherein the filter means comprises a plurality of discrete filter elements.

5 30. The apparatus of claim 29, wherein at least one discrete filter element comprises an absorption characteristic selected to provide enhanced correlation of a passed wavelength with the concentration of the analyte.

10 31. The apparatus of claim 30, wherein the absorption characteristic is provided by a weighting factor derived using chemometrics techniques.

15 32. The apparatus of claim 31, wherein the weighting factor is derived using rotated principal components analysis of an absorption spectrum of the analyte.

20 33. The apparatus of claim 28, wherein the detectors are comprised of lead selenide.

 34. The apparatus of claim 26, wherein the incident radiation is in the range of approximately
25 1100 to 5000 nm.

 35. The apparatus of claim 34, wherein the filter means comprises a first section configured to pass at least one wavelength from a first spectral
30 analysis region of wavelengths in the range of approximately 1300 to 1360 nm, a second section configured to pass at least one wavelength from a second spectral analysis region of wavelengths in the range of approximately 1670 to 1690 nm, a third
35 section configured to pass at least one wavelength from a third spectral analysis region of wavelengths in the range of approximately 1930 to 1950 nm, and a

fourth section configured to pass at least one wavelength from a third spectral analysis region of wavelengths in the range of approximately 2120 to 2280 nm.

5

36. An apparatus for determining the concentration of an analyte in a sample, comprising:

(a) means for irradiating the sample with incident radiation containing a plurality of distinct, nonoverlapping regions in the near- and mid-IR spectral ranges;

(b) means for collecting reflected radiation emerging from the sample and directing said reflected radiation into a beam path;


(c) diffraction grating means disposed in the beam path, wherein said diffraction grating means is capable of reflected radiation emerging from the sample and selectively passing discrete wavelengths therefrom, wherein said discrete wavelengths are specifically correlated with the concentration of the analyte;


(d) a linear detector array for receiving the passed wavelengths emerging from the diffraction grating means; and

(g) means for converting the detected wavelengths into a signal representative of the intensity of said wavelengths.

37. The apparatus of claim 36, wherein the linear detector array is comprised of lead selenide detectors.

35

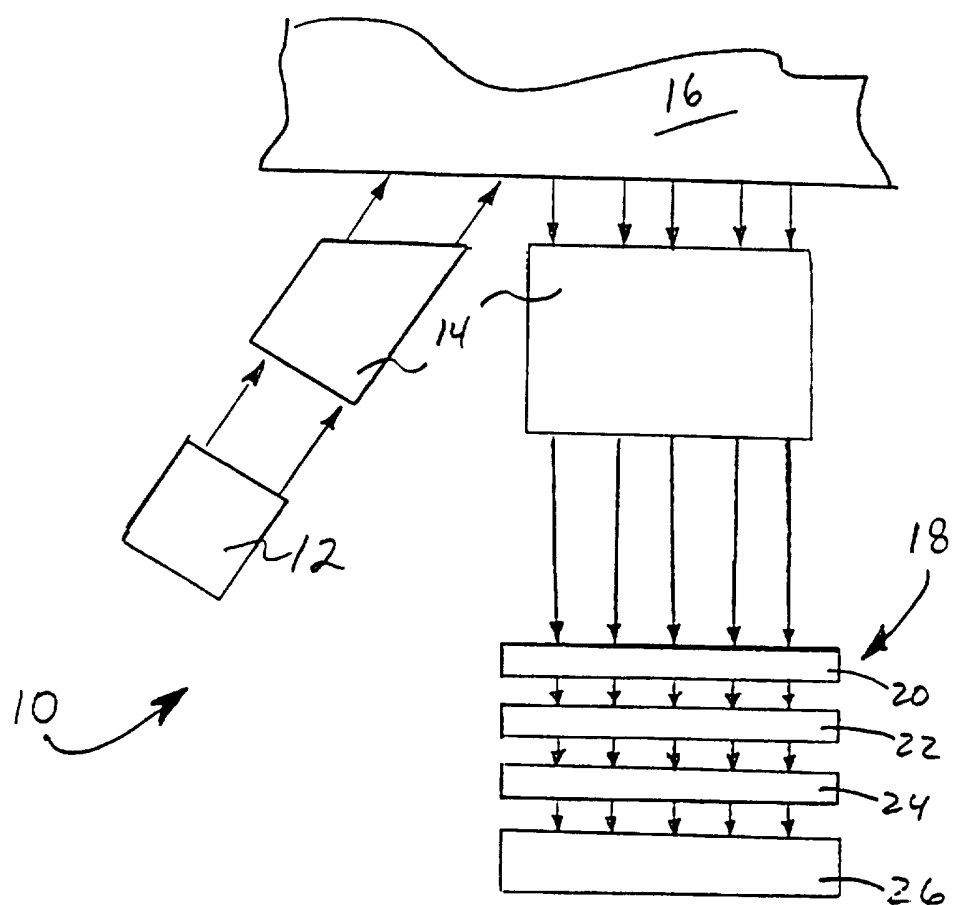**FIGURE 1**

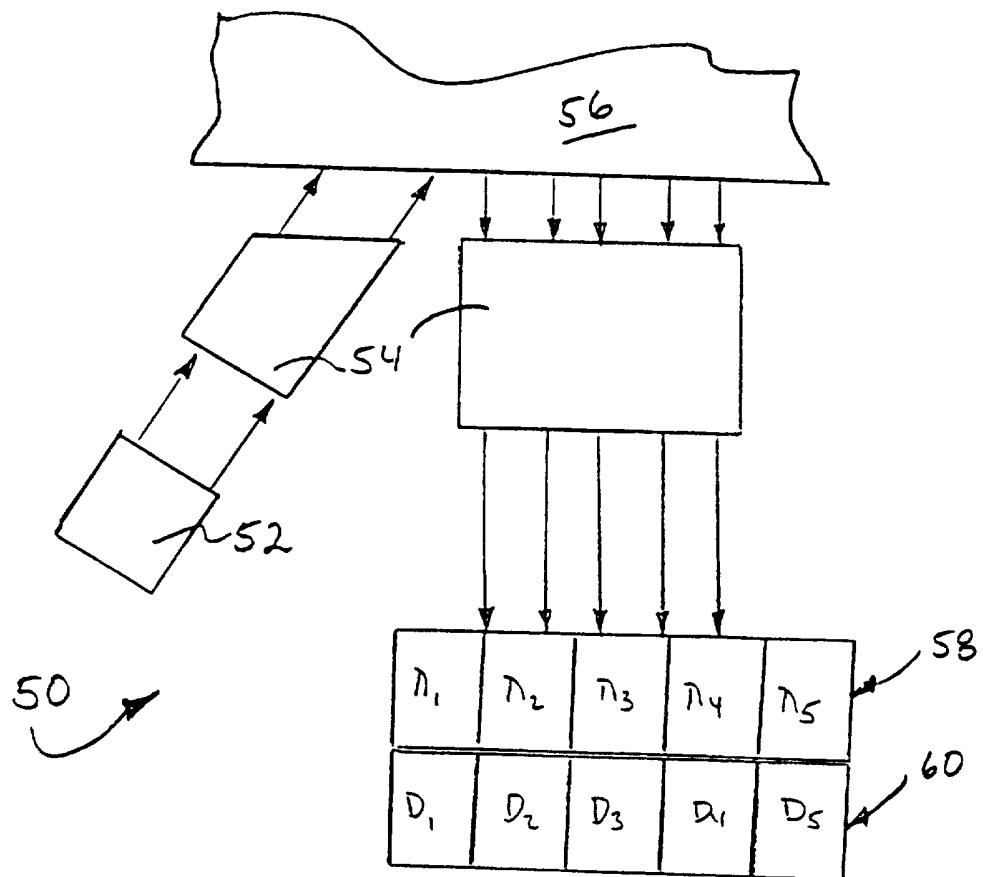**FIGURE 2**

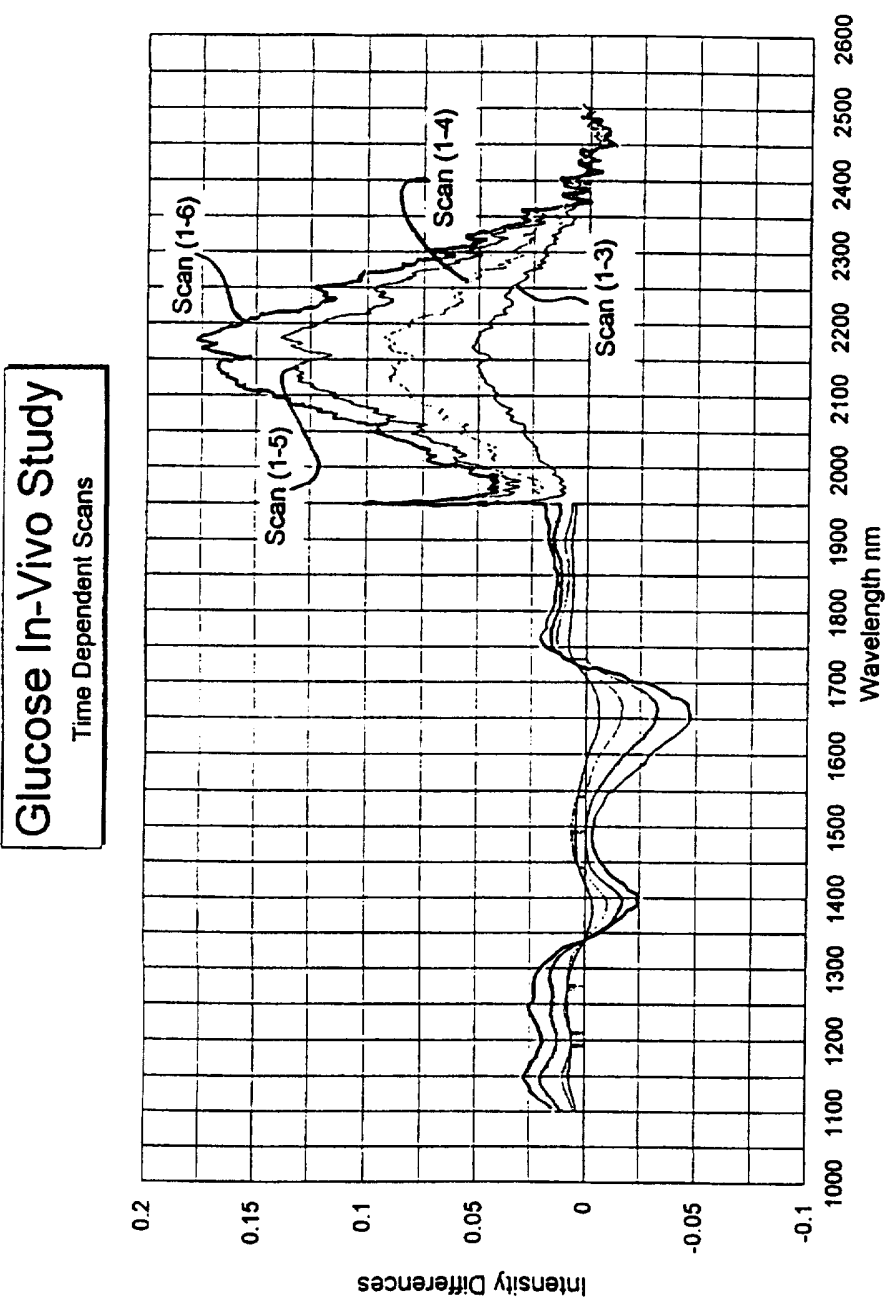
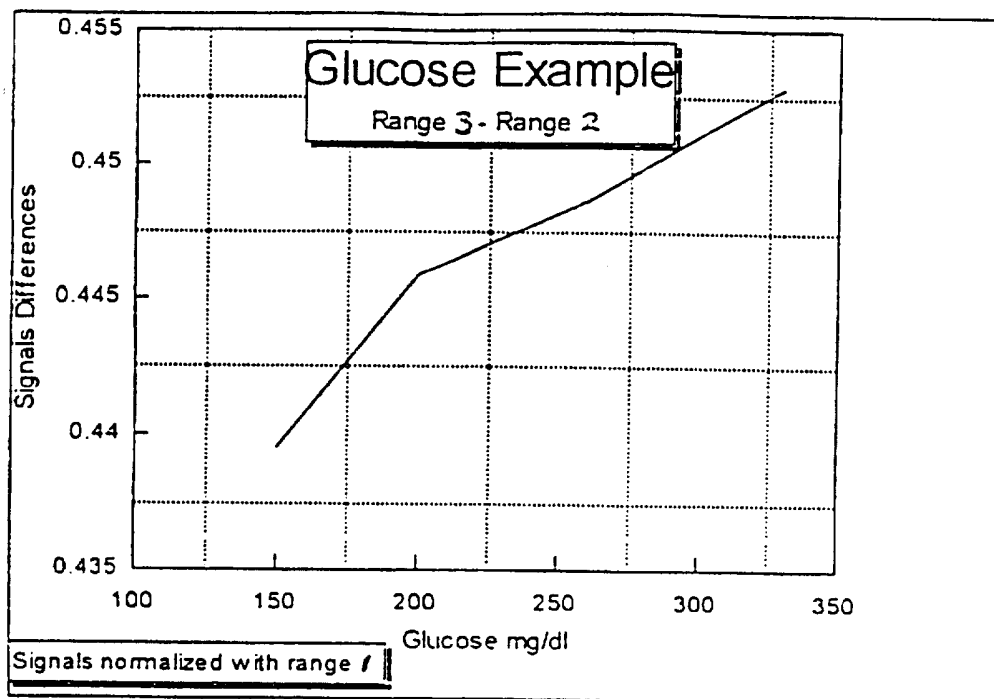


FIGURE 3

**FIGURE 4**

INTERNATIONAL SEARCH REPORT

Int. onal Application No

PCT/US 97/01369

A. CLASSIFICATION OF SUBJECT MATTER
IPC 6 G01N21/35 G01N21/31 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 242 602 A (RICHARDSON JOHN ET AL) 7 September 1993 cited in the application see column 4, line 47 - column 6, line 62	9
Y A	---	1-4,6 18,22, 23,26,32
Y	DE 22 55 300 A (SIEMENS AG) 22 May 1974 see page 6, paragraph 2 - page 8, paragraph 2 see figure 1	1-4,6
X	DE 43 39 067 A (JENOPTIK JENA GMBH) 18 May 1995 see claims 1,3,10,11,15-18; figures	36
Y A	---	37 1,4,6-8
	-/--	

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
- "&" document member of the same patent family

Date of the actual completion of the international search

3 June 1997

Date of mailing of the international search report

11. 06. 97

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+ 31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+ 31-70) 340-3016

Authorized officer

Krametz, E

INTERNATIONAL SEARCH REPORT

International Application No
PCT/US 97/01369

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 5 360 004 A (PURDY DAVID L ET AL) 1 November 1994 cited in the application see column 2, line 55 - column 3, line 32 see column 5, line 34 - column 6, line 68	37
A	---	1-8,18, 24,26,33
A	US 4 882 492 A (SCHLAGER KENNETH J) 21 November 1989 see column 2, line 59 - column 3, line 36 see column 3, line 46 - column 5, line 19 see figure 1	1,2,5-9, 18,24, 33,37
A	---	1,3,6-9, 22,23
A	EP 0 631 137 A (STARK EDWARD W) 28 December 1994 see page 3, line 24 - page 5, line 17 ---	1-3,6-9, 18,26
A	EP 0 226 822 A (HELLIGE GMBH) 1 July 1987 see page 4, line 21 - page 8, line 7 see figure 1 -----	

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PC1/US 97/01369

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5242602 A	07-09-93	AU 3319793 A BR 9300730 A CA 2090820 A CN 1079301 A EP 0559305 A JP 6066718 A NZ 245904 A ZA 9301218 A	09-09-93 08-09-93 05-09-93 08-12-93 08-09-93 11-03-94 28-03-95 17-09-93
DE 2255300 A	22-05-74	NONE	
DE 4339067 A	18-05-95	WO 9513739 A EP 0679064 A	26-05-95 02-11-95
US 5360004 A	01-11-94	US 5379764 A WO 9613202 A AU 6186494 A CA 2123152 A EP 0623307 A JP 7132120 A WO 9613204 A AU 8094894 A	10-01-95 09-05-96 10-11-94 08-11-94 09-11-94 23-05-95 09-05-96 23-05-96
US 4882492 A	21-11-89	NONE	
EP 0631137 A	28-12-94	NONE	
EP 0226822 A	01-07-87	DE 3541165 A	27-05-87