



- (51) International Patent Classification:  
A61B 17/29 (2006.01) A61B 17/072 (2006.01)
- (21) International Application Number:  
PCT/US2012/028894
- (22) International Filing Date:  
13 March 2012 (13.03.2012)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
13/048,566 15 March 2011 (15.03.2011) US
- (71) Applicant (for all designated States except US):  
ETHICON ENDO-SURGERY, INC. [US/US]; 4545  
Creek Road, Cincinnati, OH 45242 (US).
- (72) Inventors; and
- (75) Inventors/Applicants (for US only): SCHUCKMANN,  
John, C. [US/US]; 7348 Timberknoll Drive, Cincinnati,  
OH 45242 (US). SWAYZE, Jeffrey, S. [US/US]; 7047  
Birchley Drive, Hamilton, OH 45011 (US). SCHEIB,  
Charles, J. [US/US]; 11329 Donwiddle Drive, Loveland,  
OH 45140 (US).
- (74) Agents: JOHNSON, Philip, S. et al.; Johnson & Johnson,  
One Johnson & Johnson Plaza, New Brunswick, NJ 08933  
(US).

- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Declarations under Rule 4.17:**

- as to the identity of the inventor (Rule 4.17(i))
- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))

[Continued on next page]

(54) Title: SURGICAL INSTRUMENTS WITH LOCKABLE ARTICULATING END EFFECTOR

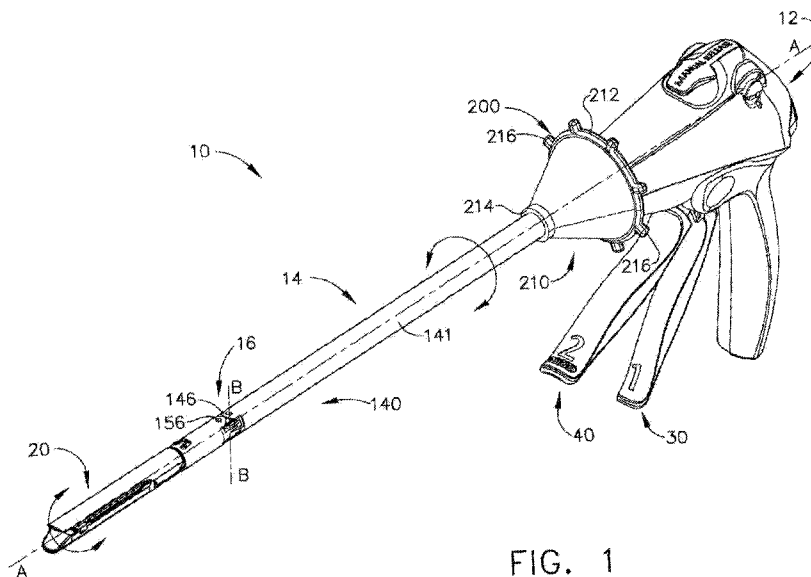


FIG. 1

(57) Abstract: Hand-held surgical instruments that have an end effector attached to an elongate shaft are disclosed. The end effector has at least a portion that is movable in response to opening and closing motions applied thereto by a closure member. An articulation control system is provided to articulate the end effector relative to the shaft. An articulation locking system is provided to lock the end effector in a desired articulated position. The locking system interfaces with the closure member and is activated upon application of a closure motion to the end effector.

WO 2012/125618 A1

- *as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))*
- Published:**
- *with international search report (Art. 21(3))*

## TITLE

SURGICAL INSTRUMENTS WITH LOCKABLE  
ARTICULATING END EFFECTOR

## BACKGROUND

## Technical Field

[0001] The present invention relates to surgical instruments and, in various embodiments, to minimally invasive surgical instruments having an articulating end effector.

## Background

[0002] Endoscopic and other minimally invasive surgical instruments typically include an end effector positioned at the distal end of an elongate shaft and a handle at the proximal end of the elongate shaft allowing a clinician to manipulate the end effector. In use, the end effector is provided to a surgical site through a cannula of a trocar. At the surgical site, the end effector engages tissue in any number of ways to achieve a diagnostic or therapeutic effect. Endoscopic surgical instruments are often preferred over traditional open surgical instruments because they require smaller incisions that generally heal with less post-operative recovery time than traditional open surgery incisions. Because of this and other benefits of endoscopic surgery, significant development has gone into a range of endoscopic surgical instruments having end effectors that engage tissue to accomplish a number of surgical tasks. For example, end effectors have been developed to act as endocutters, graspers, cutters, staplers, clip applicators, access devices, drug/gene therapy delivery devices, ultrasound, RF, or laser energy devices, and other surgical instruments.

[0003] In use, the positioning of the end effector at the surgical site may be constrained by the trocar cannula. Generally, the elongate shaft of the device enables the clinician to insert the end effector to a desired depth and rotate the end effector about the longitudinal axis of the shaft. This allows the end effector to be positioned at the surgical site, to a degree. With judicious placement of the trocar and use of graspers, for instance, through another trocar, this amount of positioning is often sufficient. Depending upon the nature of the operation, however, it may be desirable to adjust the positioning of the end effector of an endoscopic surgical instrument. In particular, it is often desirable to orient the end effector at any one of multiple angles relative to the longitudinal axis of the elongate shaft of the instrument.

[0004] Movement of the end effector through multiple angles relative to the instrument shaft is conventionally referred to as "articulation." Articulation is typically accomplished by a pivot (or articulation) joint being placed in the elongate shaft just proximal to the end effector. This allows the clinician to articulate the end effector remotely to either side for better surgical placement of the tissue fasteners and easier tissue manipulation and orientation. An articulating end effector permits the clinician to more easily engage tissue in some instances, such as behind an organ. In addition, articulated positioning advantageously allows an endoscope to be positioned behind the end effector without being blocked by the elongate shaft.

[0005] Approaches to articulating end effectors tend to be complicated because mechanisms for controlling the articulation must be integrated with mechanisms for operating the end effector. For example, for end effectors that have open and closable jaw features, the closure sleeve, drive member and mechanisms for articulation must be implemented within the small diameter constraints of the instrument's shaft. One common prior design involves an accordion-like articulation mechanism ("flex-neck") that is articulated by selectively drawing back one of two connecting rods through the implement shaft wherein each rod is offset respectively on opposite sides of the shaft centerline. The connecting rods ratchet through a series of discrete positions.

[0006] Over the years, other forms of articulating end effector arrangements have been developed. For example, U.S. Patent No. 7,670,334, entitled "Surgical Instrument Having an Articulating End Effector", and U.S. Patent No. 7,819,298, entitled "Surgical Stapling Apparatus With Control Features Operable With One Hand", the disclosures of which are each herein incorporated by reference in their respective entireties, disclose various surgical instruments that employ articulating end effector arrangements that effectively address many of the shortcomings of prior instruments with articulating effectors.

[0007] Many prior surgical instrument arrangements also employ a component commonly referred to as a "nozzle" that is rotatably supported on the instrument handle and is attached to the elongated shaft. When the clinician desires to rotate the end effector about the shaft axis, he or she simply rotates the nozzle relative to the handle. When the clinician also desires to articulate the end effector, the clinician must actuate a slide bar or other form of articulation control member to accomplish the desired articulation. Such control devices (e.g., the nozzle and articulation bar/control arrangement) typically must be actuated by using both hands.

**[0008]** In performing many surgical procedures, it is desirable to effect a desired amount of end effector articulation and rotation by using only one hand. For example, many vascular operations require precise control of the end effector. In such applications, it would be desirable to be able to have a surgical instrument that employs a single control mechanism for selectively articulating and rotating the end effector that can be easily actuated by using the same hand that is supporting the handle portion of the instrument.

**[0009]** The foregoing discussion is intended only to illustrate some of the shortcomings present in the field of the invention at the time, and should not be taken as a disavowal of claim scope.

### SUMMARY

**[0010]** In accordance with general aspects of at least one form, there is provided a surgical instrument that has an elongate shaft that defines a longitudinal axis. An end effector is coupled to the elongate shaft for selective pivotal travel relative thereto. The end effector has at least one movable portion that is responsive to opening and closing motions. A closure member interfaces with the movable portion of the end effector to selectively apply the closing motion thereto. An articulation control system operably interfaces with the end effector to apply articulation motions thereto. An articulation lock system interfaces with the articulation control system and said closure member. The articulation lock system is configured to move from an unlocked position wherein the articulation control system applies the articulation motions to the end effector and a locked position wherein the articulation lock system prevents the articulation control system from applying the articulation motions to the end effector upon application of the closure motion by the closure member.

**[0011]** In accordance with other general aspects of at least one form, there is provided a surgical instrument that has an elongate shaft that defines a longitudinal axis. An end effector is coupled to the elongate shaft for selective pivotal travel relative thereto to various articulated positions. The end effector has at least one portion that is movably responsive to opening and closing motions. A closure member interfaces with the movable portion of the end effector to apply the closure motion thereto when the closure member is moved in a closure direction. The closure member further applies the opening motion to the end effector movable portion when the closure member is moved in an opening direction. A first elongated articulation member is movably supported relative to the closure member and is configured to apply a first articulation

motion to the end effector when the first elongated articulation member is moved in a first actuation direction and a second articulation motion to the end effector when the first articulation member is moved in a second actuation direction. A locking member operably interfaces with the closure member and the first elongated articulation member such that when the closure member is moved in the closing direction, the locking member lockingly engages the first elongated articulation member to prevent movement thereof in the first and second actuation directions and when the closure member is moved in the opening direction, the locking member disengages the first articulation member to enable the first articulation member to move in the first and second actuation directions.

**[0012]** In accordance with still other general aspects of at least one form, there is provided a method of operating a surgical instrument. In various forms, the method comprises providing a surgical instrument that has an end effector that has at least a portion that is movably responsive to opening and closing motions applied thereto. The end effector is also articulatable about a longitudinal axis to a plurality of articulated positions in response to articulation motions applied thereto. The method further comprises applying an articulation motion to the end effector to articulate the end effector to one of the articulated positions and applying a closing motion to the end effector such that upon application of the closing motion, the end effector is retained in the articulated position.

#### BRIEF DESCRIPTION OF DRAWINGS

**[0013]** The above-mentioned and other features and advantages of this invention, and the manner of attaining them, will become more apparent and the invention itself will be better understood by reference to the following description of embodiments of the invention taken in conjunction with the accompanying drawings, wherein:

**[0014]** FIG. 1 is a perspective view of a surgical instrument with a non-limiting articulating end effector embodiment of one form of the present invention;

**[0015]** FIG. 2 is an exploded assembly view of a non-limiting end effector embodiment of at least one form of the present invention;

**[0016]** FIG. 3 is an assembly view of a non-limiting articulation control system embodiment of at least one form of the present invention;

**[0017]** FIG. 4 is a perspective view of the non-limiting articulation control system of FIG. 3;

[0018] FIG. 5 is a perspective view of a portion of the non-limiting articulation control system of FIGS. 3 and 4;

[0019] FIG. 6 is a perspective view of the non-limiting articulation control system of FIGS. 3-5 with a portion thereof shown in cross-section;

[0020] FIG. 7 is a cross-sectional plan view of the non-limiting articulation control system of FIGS. 3-6 with the end effector articulated in a first articulation direction;

[0021] FIG. 8 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 3-7 with the end effector in an unarticulated orientation;

[0022] FIG. 9 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 3-8 with the end effector articulated in a second articulation direction;

[0023] FIG. 10 is a perspective view of a non-limiting articulation control system embodiment of at least one other form of the present invention;

[0024] FIG. 11 is a perspective view of the non-limiting articulation control system of FIG. 10 with the rotation nozzle omitted for clarity;

[0025] FIG. 12 is a perspective view of the non-limiting articulation control system of FIGS. 10 and 11 with some components thereof shown in cross-section;

[0026] FIG. 13 is an exploded assembly view of the non-limiting articulation control system of FIGS. 10-12;

[0027] FIG. 14 is a cross-sectional plan view of the non-limiting articulation control system of FIGS. 10-13 with the end effector articulated in a first articulation direction;

[0028] FIG. 15 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 10-14 with the end effector in an unarticulated orientation;

[0029] FIG. 16 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 10-15 with the end effector articulated in a second articulation direction;

[0030] FIG. 17 is a perspective view of a non-limiting articulation control system embodiment of at least one other form of the present invention;

[0031] FIG. 18 is another perspective view of the non-limiting articulation control system of FIG. 17 with some components thereof shown in cross-section;

[0032] FIG. 19 is an exploded assembly view of the non-limiting articulation control system of FIGS. 17 and 18 with some components thereof shown in cross-section;

[0033] FIG. 20 is another exploded assembly view of the non-limiting articulation control system of FIGS. 17-19 with some components thereof shown in cross-section;

[0034] FIG. 21 is a perspective view of the non-limiting articulation control system of FIGS. 17-20 with the right nozzle portion thereof moved in the first actuation direction;

[0035] FIG. 22 is a cross-sectional plan view of the non-limiting articulation control system of FIGS. 17-21 with the end effector articulated in a first articulation direction;

[0036] FIG. 23 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 17-22 with the end effector articulated in a second articulation direction;

[0037] FIG. 24 is a perspective view of a non-limiting nozzle assembly embodiment of another form of the present invention;

[0038] FIG. 25 is a cross-sectional view of the nozzle assembly of FIG. 24 taken along line 25-25 in FIG. 24;

[0039] FIG. 26 is a perspective view of a non-limiting articulation control system embodiment of at least one other form of the present invention;

[0040] FIG. 27 is a perspective view of a portion of the non-limiting articulation control system embodiment of FIG. 26;

[0041] FIG. 28 is another perspective view of the portion of the non-limiting articulation control system embodiment of FIG. 27 with a portion shown in cross-section;

[0042] FIG. 29 is an exploded assembly view of the non-limiting articulation control system of FIGS. 26-28;

[0043] FIG. 30 is a side elevation view of a portion of the non-limiting articulation control system of FIGS. 26-29;

[0044] FIG. 31 is a cross-sectional plan view of the non-limiting articulation control system of FIGS. 26-30 with the end effector articulated in a first articulation direction;

[0045] FIG. 32 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 26-31 with the end effector in an unarticulated orientation;

[0046] FIG. 33 is another cross-sectional plan view of the non-limiting articulation control system of FIGS. 26-32 with the end effector articulated in a second articulation direction;

[0047] FIG. 34 is a perspective view of a non-limiting articulation control system embodiment of at least one other form of the present invention;



- [0048] FIG. 35 is a perspective view of a portion of the non-limiting articulation control system embodiment of FIG. 34;
- [0049] FIG. 36 is a rear perspective view of the non-limiting articulation control system embodiment of FIGS. 34 and 35;
- [0050] FIG. 37 is a cross-sectional perspective view of the non-limiting articulation control system embodiment of FIGS. 34-36;
- [0051] FIG. 38 is an exploded assembly view of the non-limiting articulation control system embodiment of FIGS. 34-37;
- [0052] FIG. 39 is a cross-sectional view of the non-limiting articulation control system embodiment of FIGS. 34-38;
- [0053] FIG. 40 is another cross-sectional view of the non-limiting articulation control system embodiment of FIGS. 34-39 with the end effector articulated in a first articulation direction;
- [0054] FIG. 41 is another cross-sectional view of the non-limiting articulation control system embodiment of FIGS. 34-40;
- [0055] FIG. 42 is a cross-sectional view of the non-limiting articulation control system embodiment of FIGS. 34-41 with the end effector articulated in a second articulation direction;
- [0056] FIG. 43 is a perspective view of another non-limiting articulation control system embodiment of the present invention;
- [0057] FIG. 44 is an exploded assembly view of the non-limiting articulation control system embodiment of FIG. 43;
- [0058] FIG. 45 is another exploded assembly view of the non-limiting articulation control system embodiment of FIGS. 43 and 44;
- [0059] FIG. 46 is another exploded assembly view of the non-limiting articulation control system embodiment of FIGS. 43-45;
- [0060] FIG. 47 is a cross-sectional view of the non-limiting articulation control system embodiment of FIGS. 43-46 in an unlocked position;
- [0061] FIG. 48 is an enlarged cross-sectional view of a portion of the non-limiting articulation control system embodiment of FIGS. 43-47 in an unlocked position;
- [0062] FIG. 49 is a cross-sectional view of the non-limiting articulation control system embodiment of FIGS. 43-48 in a locked position; and

[0063] FIG. 50 is an enlarged cross-sectional view of a portion of the non-limiting articulation control system embodiment of FIGS. 43-49 in a locked position.

#### DETAILED DESCRIPTION

[0064] Applicant of the present application also owns U.S. Patent Application Serial No. \_\_\_\_\_, entitled “SURGICAL INSTRUMENTS WITH ARTICULATABLE AND ROTATABLE END EFFECTOR”, Docket No. END6846USNP/100531, which was filed on even date herewith and which is hereby incorporated by reference in its entirety.

[0065] Certain exemplary embodiments will now be described to provide an overall understanding of the principles of the structure, function, manufacture, and use of the instruments and methods disclosed herein. One or more examples of these embodiments are illustrated in the accompanying drawings. Those of ordinary skill in the art will understand that the devices and methods specifically described herein and illustrated in the accompanying drawings are non-limiting exemplary embodiments and that the scope of the various embodiments of the present invention is defined solely by the claims. Reference throughout the specification to “various embodiments,” “some embodiments,” “one embodiment,” or “an embodiment”, or the like, means that a particular feature, structure, or characteristic described in connection with the embodiment is included in at least one embodiment. Thus, appearances of the phrases “in various embodiments,” “in some embodiments,” “in one embodiment”, or “in an embodiment”, or the like, in places throughout the specification are not necessarily all referring to the same embodiment. Furthermore, the particular features, structures, or characteristics may be combined in any suitable manner in one or more embodiments. Thus, the particular features, structures, or characteristics illustrated or described in connection with one embodiment may be combined, in whole or in part, with the features structures, or characteristics of one or more other embodiments without limitation. Such modifications and variations are intended to be included within the scope of the various invention embodiments disclosed herein and their respective equivalents.

[0066] The terms “proximal” and “distal” are used herein with reference to a clinician manipulating the handle portion of the surgical instrument. The term “proximal” referring to the portion closest to the clinician and the term “distal” referring to the portion located away from the clinician. It will be further appreciated that, for convenience and clarity, spatial terms such

as “vertical”, “horizontal”, “up”, “down”, “right” and “left” may be used herein with respect to the drawings. However, surgical instruments are used in many orientations and positions, and these terms are not intended to be limiting and/or absolute.

[0067] Various exemplary instruments and methods are provided for performing laparoscopic and minimally invasive surgical procedures. However, the person of ordinary skill in the art will readily appreciate that the various methods and instruments disclosed herein can be used in numerous surgical procedures and applications including, for example, in connection with “open” surgical procedures. As the present Detailed Description proceeds, those of ordinary skill in the art will further appreciate that the various instruments disclosed herein can be inserted into a body in any way, such as through a natural orifice, through an incision or puncture hole formed in tissue, etc. The working portions or end effector portions of the instruments can be inserted directly into a patient’s body or can be inserted through an access device such as a trocar that has a working channel through which the end effector and elongated shaft of a surgical instrument can be advanced.

[0068] Turning to the Drawings wherein like numerals denote like components throughout the several views, FIG. 1 depicts one embodiment of a surgical stapling and severing instrument 10 that is capable of practicing various unique benefits of at least one form of the present invention. Various portions of the instrument 10 may be identical to portions of the devices disclosed in U.S. Patent No. 7,670,334, which has been herein incorporated by reference and/or U.S. Patent No. 7,000,818, entitled “Surgical Stapling Instrument Having Separate Distinct Closing and Firing Systems”, the disclosure of which is herein incorporated by reference in its entirety.

[0069] As shown in FIG. 1, in one non-limiting form, the surgical instrument 10 generally includes a handle 12, a shaft 14 and an articulating end effector 20 that is pivotally connected to the shaft 14 at articulation pivot 16. An articulation control 200 is provided to effect rotation of the end effector 20 about the articulation pivot 16. The end effector 20 is shown configured to act as an endocutter for clamping, severing and stapling tissue. However, those of ordinary skill in the art will understand that various embodiments of the present invention may include end effectors (not shown) that are configured to act as other surgical devices including, for example, graspers, cutters, staplers, clip applicators, access devices, drug/gene therapy delivery devices, ultrasound, RF, or laser energy devices, etc.

[0070] The handle 12 of the instrument 10 may include a closure trigger 30 and a firing trigger

40 for actuating the end effector 20. It will be appreciated that instruments having end effectors directed to different surgical tasks may have different numbers or types of triggers or other suitable controls for operating an end effector. The end effector 20 is shown separated from a handle 12 by the elongate shaft 14 that defines a longitudinal axis A-A. A clinician may articulate the end effector 20 relative to the shaft 14 about an articulation axis B-B that is substantially transverse to the longitudinal axis A-A (articulation pivot 16) utilizing the articulation control 200 as will be discussed in further detail below. As used herein, the phrase, "substantially transverse to the longitudinal axis" where the "longitudinal axis" is the axis of the shaft 14, refers to a direction that is nearly perpendicular to the longitudinal axis. It will be appreciated, however, that directions that deviate some from perpendicular to the longitudinal axis are also substantially transverse to the longitudinal axis.

[0071] FIG. 2 shows an exploded view of the end effector 20 and elongate shaft 14 including various internal components. An end effector frame 90 and shaft frame 100 are configured to be joined at articulation pivot 50 which defines an articulation axis B-B (FIG. 1). The shaft frame 100 is supported by the handle 12 in a known manner. As such, the construction of shaft frame 100 will not be discussed in great detail herein beyond that which is necessary to understand the various embodiments of the present invention. In various embodiments, for example, the end effector frame 90 has a boss 96 integrally formed or otherwise attached thereto that is coupled to a distally directed tang 102 on the shaft frame 100 defining an aperture 104. The aperture 104 may be positioned to interface with an articulation pin (not shown) included in end effector frame 90 allowing the end effector frame 90 to pivot relative to the shaft frame 100, and accordingly, the end effector 20 to pivot relative to the shaft 14. When assembled, the various components may pivot about articulation pivot 50 at articulation axis B-B as shown in FIG. 1.

[0072] As can be further seen in FIG. 2, in one non-limiting form, the end effector 20 includes an elongate channel 110 that is sized and configured to removably support a staple cartridge 120 therein. The elongate channel 110 is attached to the end effector frame 90 by a pair of frame tabs 93 that extend into corresponding slots 115 in the elongate channel 110. The staple cartridge 120 may comprise a molded cartridge body 122 that operably supports a plurality of staples 124 resting upon corresponding staple drivers 126 within respective upwardly open staple apertures 128. In this non-limiting embodiment, the end effector 20 also includes an anvil 130 that is coupled to the elongate channel 110. A pair of apertures 112 may be provided in elongate

channel 110 to movably receive trunnions or pins 132 on the anvil 130, allowing the anvil 120 to pivot from an open position to a closed position relative to the elongate channel 110 and staple cartridge 120 in response to opening and closing motions received from a closure tube assembly 140. Such closing motions may also be used to effectively actuate the jaws of other types of end effectors as is known.

[0073] As can also be seen in FIG. 2, the closure tube assembly 140 employs a “double pivot” closure sleeve assembly 142. It will be appreciated that the invention is not limited to a double pivot closure sleeve design and may include any suitable closure sleeve arrangement. In various non-limiting embodiments, for example, the double pivot closure sleeve assembly 142 includes a proximal closure tube segment 141 that has upper and lower distally projecting tangs 146, 148. An end effector closure tube section 150 includes a horseshoe aperture 152 and tab 154 for engaging an opening tab 134 on the anvil 130. As is known, when the end effector closure tube section 150 is advanced distally on the end effector frame 90, the horseshoe aperture applies a closing motion to the tab 134 to move the anvil 130 toward the staple cartridge 120. When the end effector closure tube 150 is withdrawn in the proximal direction, the tab 154 engages the tab 134 to move the anvil 130 away from the staple cartridge 120 to an open position. The closure tube section 150 is shown having upper 156 and lower (not visible) proximally projecting tangs.

[0074] The end effector closure tube section 150 is pivotally attached to the proximal closure tube segment section 141 by an upper double pivot link 160 and a lower double pivot link 170. The upper double pivot link 160 includes upwardly projecting distal and proximal pivot pins 162, 164 that engage respectively an upper pin hole 157 in the upper proximally projecting tang 156 and an upper proximal pin hole 147 in the upper distally projecting tang 146. A lower double pivot link 170 includes downwardly projecting distal and proximal pivot pins (not shown) that engage respectively a lower distal pin hole in the lower proximally projecting tang and a lower proximal pin hole 149 in the lower distally projecting tang 148. In use, the closure sleeve assembly 140 is translated distally to close the anvil 130, for example, in response to the actuation of the closure trigger 30.

[0075] The device 10 further includes a firing bar 180 that is configured to longitudinally translate through the shaft 14, through the flexible closure and pivoting frame articulation joint 50, and through a firing slot 91 in the end effector frame 90 into the end effector 20. The firing bar 180 may be constructed from one solid section, or in various embodiments, may include a

laminate material comprising, for example, a stack of steel plates 182. It will be appreciated that a firing bar 180 made from a laminate material may lower the force required to articulate the end effector 20. A distally projecting end of the firing bar 180 is attached to an E-beam 184 that assists in spacing the anvil 130 from the staple cartridge 120 when the anvil 130 is in a closed position. A sharpened cutting edge 186 of the E-beam 184 may also be used to sever tissue.

[0076] In operation, the E-beam 184 actuates the staple cartridge 120. A wedge sled 190 is driven distally by the E-beam 184, sliding upon a cartridge tray 192 that holds together the various components of the replaceable staple cartridge 120. The wedge sled 192 upwardly cams the staple drivers 126 to force out the staples 124 into deforming contact with the anvil 130 while a cutting surface 186 of the E-beam 184 severs clamped tissue. The firing bar 180 is movably supported within the shaft 14 such that it passes through the cartridge 120 when the instrument 10 is fired (e.g., actuated). In at least one non-limiting embodiment, the firing bar 180 is instead positioned within the shaft 14 such that all or a portion of the body of the firing bar element 180 is supported by a slot (not shown) in the anvil 130 during firing. Because the anvil 130 may be stronger than the cartridge 120, support from the slot may prevent the firing bar 180 from buckling, even when high loads are applied to the distal end of the firing bar 180. This may be useful in embodiments where the firing bar element 182 includes laminate plates 182.

[0077] Various E-beam configurations also include upper pins 188 that are configured to engage the anvil 130 during firing while middle pins 185 and a bottom foot 187 engage various portions of the cartridge body 122, cartridge tray 192 and elongate channel 110. In use, a centrally disposed slot 123 in the cartridge body 122 aligns with a slot 193 in the cartridge tray 190 and with a slot 113 in the elongate channel 110. The leading edge of E-beam 184 slides through the aligned slots 123, 193, and 113. As the firing bar 180 is advanced distally, the foot 187 is braced against the bottom of channel 110 and the upper pins 180 are braced in a groove 131 in the bottom surface of the anvil 130 to prevent the anvil 130 and channel 110 from being forced apart from resistance of tissue. Thereafter, the firing bar 180 is retracted proximally, retracting as well the E-beam 184, allowing the anvil 130 to be opened to release the two stapled and severed tissue portions (not shown).

[0078] In various non-limiting embodiments, a spring clip 195 is mounted in the end effector frame 90 as a lockout for firing bar 180. Distal and proximal square apertures 192, 193 formed on top of the end effector frame 90 may define a clip bar 196 therebetween that receives a top

arm 197 of a clip spring 195 whose lower, distally extended arm 198 asserts a downward force on a raised portion 183 of the firing bar 180 as is known. It will be appreciated that various embodiments may include other types of lockouts or no lockouts at all.

[0079] In the various embodiments depicted in FIGS. 1 and 3-9, the end effector 20 is selectively rotatable about the longitudinal axis A-A and selectively articulatable about articulation axis B-B relative to the proximal shaft segment 141 by the articulation control system 200. In various non-limiting embodiments, the articulation control system 200 includes a nozzle 210 that is rotatably supported relative to the handle 12. In the embodiments depicted in FIGS. 3-9, the nozzle 210 has proximal end portion 212 that tapers to a distal end portion 214. To facilitate easy rotation of the nozzle 210 about the longitudinal axis A-A by a portion of the same hand in which the clinician is gripping the handle 12, a plurality of radially protruding actuation buttons 216 are formed around the proximal end 212 of the nozzle 210 as shown. The clinician may then rotate the nozzle 210 relative to the handle with his or her index finger or other finger or portion of their hand that is supporting the handle 12.

[0080] Turning to FIGS. 3 and 4, it can be seen that the nozzle 210 may be provided in multiple pieces for assembly purposes. In the illustrated embodiment, for example, the nozzle 210 is formed from a lower nozzle portion 211 and an upper nozzle portion 213. Lower and upper nozzle portions 211, 213 may be fabricated from, for example, glass-filled polycarbonate or other suitable material and be interconnected together by appropriate adhesive, welding, snap features, screws, frictional posts/holes, etc. In various non-limiting embodiments, the nozzle 210 is pivotally pinned to the proximal closure tube segment 141 by upper and lower pins 220, 222, respectively. The proximal closure tube segment 141 may be fabricated in multiple segments for assembly purposes. Those of ordinary skill in the art will appreciate that the proximal portion of the proximal closure tube segment 141 will interface with known components for attaching or communicating with the closure trigger of the device. For example, such arrangements are disclosed in U.S. Patent No. 7,000,818, which has been herein incorporated by reference. However, the actuation of the closure tube assembly may be controlled by a myriad of other known trigger and handle arrangements without departing from the spirit and scope of the present invention. In the embodiment depicted in FIGS. 3-6, the proximal closure tube segment 141 is fabricated from a lower shaft segment 143 and an upper shaft segment 145. In various embodiments, the lower and upper shaft segments 143, 145 may be fabricated from stainless

steel or other suitable material and be connected together by an appropriate adhesive or other suitable fastener arrangement to form a substantially hollow tubular structure to accommodate various components of the articulation control system 200 such as an articulation assembly 230 as well as the firing bar 182, shaft frame 100, etc.

**[0081]** As can be seen in FIGS. 3 and 6, in various non-limiting embodiments, the upper pin 220 is rotatably received within a hole 149 in the upper shaft segment 145 and the lower pin 222 is rotatably received in a lower hole 147 in the lower shaft segment 143. The upper and lower pins 220, 222 are coaxially aligned and define a nozzle axis C-C about which the nozzle 210 may pivot relative to the proximal closure tube segment 141. As can be most particularly seen in FIG. 6, a hole 219 is provided through the proximal end 214 of the nozzle 210. The hole 219 is sized relative to the proximal closure tube segment 141 to permit the nozzle 210 to be pivoted about the nozzle axis C-C as will be discussed in further detail below.

**[0082]** In the non-limiting embodiment of FIG. 2, the articulation control system 200 includes an articulation assembly 230. In at least one embodiment, the articulation assembly 230 may comprise a right articulation rod 232 and a left articulation rod 234. The right and left articulation rods 232, 234 may be configured as shown in FIGS. 2 and 3 and be fabricated from stainless steel or other suitable material. The articulation assembly 230 comprises a right articulation rod 232 and a left articulation rod 234 that, when received within the proximal closure tube segment 141, may be axially moved therein relative to each other as will be discussed in further detail below. As can be seen in FIG. 2, the right and left articulation rods 232, 234 define a centrally disposed elongate slot 236 that is configured to accommodate the axial movement of the firing bar 180 therebetween. A right articulation band 238 protrudes distally from a distal end 233 of the right articulation rod 232 and a left articulation band 240 protrudes distally from the distal end 239 of the left articulation rod 234. See FIG. 2. In various non-limiting embodiments, the articulation bands 238, 240 are attached to the boss 96. For example, the bands 238, 240 may be pivotally pinned to the boss 96.

**[0083]** The articulation assembly 230 is configured to interface with the nozzle 210 such that pivotal travel of the nozzle 210 about the nozzle axis C-C results in the axial actuation of the right and left articulation rods 232, 234 which ultimately causes the end effector 20 to articulate about articulation axis B-B. More specifically and with reference to FIGS. 3, 5, and 6-9, the right articulation rod 232 has a right pivot pin 250 that is attached thereto and protrudes laterally



therefrom through a right slot 251 in the proximal closure tube segment 141. The end of the right pivot pin 250 extends into a right socket or aperture 252 in the nozzle 210. Similarly, the left articulation rod 234 has a left pivot pin 254 that is attached thereto and protrudes laterally therefrom through a left slot 255 in the proximal closure tube segment 141. The end of the left pivot pin 254 extends into a socket or aperture 256 in the nozzle 210.

**[0084]** The operation of the articulation control system 200 can be understood from reference to FIGS. 7-9. FIG. 7 illustrates articulation of the end effector 20 to the left of the articulation pivot 50 (about articulation axis B-B – shown in FIG. 1). To accomplish this range of articulation, the clinician pivots the nozzle 210 in the first actuation direction represented by arrow “E” in FIG. 7. When the nozzle 210 is pivoted in the “E” direction, the right articulation rod 232 is moved in the distal direction “DD” and the left articulation rod 234 is moved in the proximal direction “PD”. Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the right articulation band 238 and a pulling motion to the boss 96 by the left articulation band 240 which results in the articulation of the end effector 20 as shown. FIG. 8 illustrates the end effector 20 in coaxial alignment with the shaft 14 (e.g., in an unarticulated position). Such end effector orientation may be employed, for example, during insertion of the end effector 20 through a trocar cannula (not shown) or other opening in the patient. FIG. 9 illustrates articulation of the end effector 20 to the right of the articulation pivot 50 (about articulation axis B-B – shown in FIG. 1). To accomplish this range of articulation, the clinician pivots the nozzle 210 in a second actuation direction represented by arrow “F” in FIG. 9. When the nozzle 210 is pivoted in the “F” direction, the right articulation rod 232 is moved in the proximal direction “PD” and the left articulation rod 234 is moved in the distal direction “DD”. Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the left articulation band 240 and a pulling motion to the boss 96 by the right articulation band 238 which results in the articulation of the end effector 20 as shown. The end effector 20 may be rotated about the longitudinal axis simply by rotating the nozzle 210 about the longitudinal axis A-A. This action may be accomplished by a portion of the hand that is supporting the handle portion of the device, thereby avoiding the need for both hands to rotate the end effector about the longitudinal axis. Although the articulation assembly 230 as described above employs two elongated articulation rods or members, in alternative embodiments, only one elongated articulation member is employed.

[0085] FIGS. 10-17 illustrate another non-limiting articulation control system embodiment of the present invention generally designed as 300 that is similar to the articulation control system 200 described above, except for the differences noted below. Those components that are the same as the components employed in the above-described embodiments will be labeled with the same element numbers and those of ordinary skill in the art can refer to the disclosure set forth hereinabove that explains their construction and operation. As can be seen in FIG. 10, articulation control system 300 employs a separate rotation nozzle 302 for controlling the rotation (arrow "G" in FIG. 10) of the closure tube assembly 140 and ultimately, the end effector 12. As can be seen in FIG. 13, in at least one embodiment, the rotation nozzle 302 is fabricated from an upper rotation nozzle portion 303 and a lower rotation nozzle portion 304 that is attached to the upper rotation nozzle portion 303 by, for example frictional posts and sockets 341, 343. However, the nozzle portions 303, 304 may be attached together by other suitable means such as adhesive, welding, snap features, screws, etc. The upper rotational nozzle portion 303 and the lower rotational nozzle portion 304 are attached to the proximal closure tube segment 141. In at least one embodiment, for example, the upper rotational nozzle section 303 is keyed to the upper shaft segment 145 by a key 305 that extends through an opening 306 in the upper shaft segment 145 and the lower rotational nozzle section 304 is keyed to the lower shaft segment 143 by a key 307 that extends through an opening 308 in the lower shaft segment 143. However, the rotational nozzle 302 may be non-rotatably attached to the proximal closure tube segment 141 by other suitable means such that rotation of the rotational nozzle 302 results in the rotation of the end effector 20 about the longitudinal axis A-A.

[0086] As shown in FIG. 13, the articulation nozzle 310 may be provided in multiple pieces for assembly purposes. In the illustrated embodiment, for example, the articulation nozzle 310 is formed from a right nozzle portion 311 and a left nozzle portion 313. Right and left nozzle portions 311, 313 may be fabricated from, for example, glass-filled polycarbonate and be interconnected together by frictional posts/holes, 345, 347. However, the right and left nozzle portions 311, 313 may be attached together by appropriate adhesive, welding, snap features, screws, etc. In various non-limiting embodiments, the articulation nozzle 310 is pivotally mounted on upper and lower pins 220, 222, respectively. The upper pin 220 is attached to the upper shaft segment 145 and the lower pin 222 is attached to the lower shaft segment 143. The upper and lower pins 220, 222 are coaxially aligned and define a nozzle axis C-C about which

the articulation nozzle 310 may pivot relative to the proximal closure tube segment 141. As can be most particularly seen in FIG. 11, a hole 319 is provided through the proximal end 314 of the articulation nozzle 310. The hole 319 is sized relative to the closure tube section 141 to permit the articulation nozzle 310 to be pivoted about the nozzle axis C-C as will be discussed in further detail below.

**[0087]** In the non-limiting embodiment of FIG. 13, the articulation control system 300 includes an articulation assembly 230. In at least one embodiment, the articulation assembly 230 may comprise a right articulation rod 232 and a left articulation rod 234. The right and left articulation rods 232, 234 may be configured as shown in FIG. 14 and be fabricated from stainless steel or other suitable material. As was discussed above, when the right and left articulation rods are received within the proximal closure tube segment 141, they may be axially moved therein relative to each other. When received within the proximal closure tube segment 141, the right and left articulation rods 232, 234 define a centrally disposed elongate slot 236 that is configured to accommodate the axial movement of the firing bar 180. A right articulation band 238 protrudes distally from a distal end 233 of the right articulation rod 232 and a left articulation band 240 protrudes distally from the distal end 239 of the left articulation rod 234. In various non-limiting embodiments, the articulation bands 238, 240 are attached to the boss 96. For example, the bands 238, 240 may be pivotally pinned to the boss 96.

**[0088]** The articulation assembly 230 is configured to interface with the articulation nozzle 310 such that pivotal travel of the articulation nozzle 310 about the nozzle axis C-C results in the actuation of the articulation assembly 230 which ultimately causes the end effector 20 to articulate about articulation axis B-B at articulation pivot 50. More specifically and with reference to FIGS. 14-17, the right articulation rod 232 has a right pivot pin 320 that is attached thereto and protrudes laterally therefrom through a right slot 251 in the shaft closure tube section 141. In various non-limiting embodiments, a ball 321 may be provided on the end of the right pivot pin 320 and be rotatably received within an aperture 323 in the articulation nozzle 310. Similarly, the left articulation rod 234 has a left pivot pin 330 that is attached thereto and protrudes laterally therefrom through a left slot 255 in the proximal closure tube segment 141. A ball 332 may be provided on the end of the left pivot pin 330 and be rotatably received within an aperture 334 in the articulation nozzle 310.

**[0089]** The operation of the articulation control system 300 can be understood from reference to FIGS. 14-16. FIG. 14 illustrates articulation of the end effector 20 to the left of the articulation pivot 50. To accomplish this range of articulation, the clinician pivots the articulation nozzle 310 in the actuation direction represented by arrow “E” in FIG. 14. When the articulation nozzle 310 is pivoted in the “E” direction, the right articulation rod 232 is moved in the distal direction “DD” and the left articulation rod 234 is moved in the proximal direction “PD”. Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the right articulation band 238 and a pulling motion to the boss 96 by the left articulation band 240 which results in the articulation of the end effector 20 as shown. FIG. 15 illustrates the end effector 20 in coaxial alignment with the shaft 14 (e.g., in an unarticulated position). Such end effector orientation may be employed, for example, during insertion of the end effector 20 through a trocar cannula (not shown) or other opening in the patient. FIG. 16 illustrates articulation of the end effector 20 to the right of the articulation pivot 50. To accomplish this range of articulation, the clinician pivots the articulation nozzle 310 in the actuation direction represented by arrow “F” in FIG. 15. When the articulation nozzle 310 is pivoted in the “F” direction, the right articulation rod 232 is moved in the proximal direction “PD” and the left articulation rod 234 is moved in the distal direction “DD”. Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the left articulation band 240 and a pulling motion to the boss 96 by the right articulation band 238 which results in the articulation of the end effector 20 as shown. Although the articulation assembly 230 as described above employs two elongated articulation rods or members, in alternative embodiments, only one elongated articulation member is employed.

**[0090]** FIGS. 17-23 illustrate another non-limiting articulation control system embodiment of the present invention generally designated as 400. Those components that are the same as the components employed in the above-described embodiments will be labeled with the same element numbers and those of ordinary skill in the art can refer to the disclosure set forth hereinabove that explains their construction and operation. In various non-limiting embodiments, the articulation control system 400 includes an articulation nozzle 410 that is fabricated in multiple pieces. For example, the articulation nozzle 410 has a right nozzle portion 412 that is axially movable relative to a left nozzle portion 430. See FIG. 21. In at least one non-limiting embodiment, the right nozzle portion 412 consists of an upper right portion 414 and

a lower right portion 420. See FIG. 19. The upper and lower right nozzle portions 412, 414 may be fabricated from, for example, glass-filled polycarbonate or other suitable material.

Similarly, the left nozzle portion 430 consists of an upper left nozzle portion 432 and a lower left nozzle portion 440. The upper and lower left nozzle portions 432, 440 may be fabricated from, for example, glass-filled polycarbonate or other suitable material.

[0091] As can be seen in FIG. 20, the upper right nozzle portion 414 is provided with a pair of spaced retention band segments 416 and the lower right nozzle portion 420 is provided with a pair of spaced retention band segments 422. When the upper and lower right nozzle portions 414, 420 are joined together, the retention band segments 416 in the upper portion 414 cooperate with the retention band segments 422 in the lower portion 420 to form continuous annular right retention bands, generally designed as 424, the purpose of which will be discussed in further detail below. Similarly, the upper left nozzle portion 432 is provided with a pair of spaced retention band segments 434 and the lower left nozzle portion 440 is provided with a pair of spaced retention band segments 442. When the upper and lower left nozzle portions 432, 440 are joined together, the retention band segments 434 in the upper portion 432 cooperate with the retention band segments 442 in the lower portion 440 to form continuous annular left retention bands, generally designed as 444.

[0092] In at least one non-limiting embodiment, the articulation control system 400 includes an articulation assembly 230. In at least one embodiment, the articulation assembly 230 may comprise a right articulation rod 232 and a left articulation rod 234. The right and left articulation rods 232, 234 may be configured as shown in FIG. 19 and be fabricated from stainless steel or other suitable material. The right and left articulation rods 232, 234 when movably supported within the proximal closure tube segment 141 as illustrated, serve to define a centrally disposed elongate slot 236 that is configured to accommodate the axial movement of the firing bar 180. A right articulation band 238 protrudes distally from a distal end 233 of the right articulation rod 232 and a left articulation band 240 protrudes distally from the distal end 239 of the left articulation rod 234. In various non-limiting embodiments, the articulation bands 238, 240 are attached to the boss 96. For example, the bands 238, 240 may be pivotally pinned to the boss 96. The right and left articulation rods 232, 234 are slidably inserted into the hollow proximal closure tube segment 141. The right articulation rod 232 has a right pivot pin 450 that is attached thereto and protrudes laterally therefrom through a right slot 251 in the shaft closure

tube section 141. Similarly, the left articulation rod 234 has a left pivot pin 460 that is attached thereto and protrudes laterally therefrom through a left slot 255 in the shaft closure tube section 141. Such arrangement enables the right articulation rod 232 and the second articulation rod to be independently axially movable within the proximal closure tube segment 141. The end of the right pivot pin 450 is configured to be received within an aperture 452 formed by the joined upper and lower right nozzle portions 414, 420. Likewise, the end of the left pivot pin 460 is configured to be received within an aperture 462 formed by the upper and lower left nozzle portions 432, 440.

**[0093]** To assemble at least one embodiment, the upper nozzle portions 414, 432 are brought together to form a temporary upper nozzle assembly 433, but remain unattached to each other as illustrated in FIG. 19. As is also illustrated in FIG. 19, the lower nozzle portions 420, 440 are brought together to form a temporary lower nozzle assembly 443, but remain unattached to each other. Then, the temporary upper nozzle assembly 433 is joined to the temporary lower nozzle assembly 443 over the proximal closure tube segment 141 while capturing the right pivot pin 450 in the right aperture 452 and the left pivot pin 460 in the left aperture 462. In at least one non-limiting embodiment, the right upper nozzle portion 414 is provided with attachment posts 415 (FIG. 20) that are sized to be frictionally fitted into attachment holes 425 in the lower right nozzle portion to retain those two portions 414, 420 together to form the right nozzle section 412. Likewise, the lower left nozzle portion 440 is provided with attachment posts 445 that are sized to be frictionally fitted into attachment holes 435 in the upper left nozzle portion 432 to retain those two portions 440, 432 together to form the left nozzle portion 430. However, other fastener arrangements and/or adhesive may be employed to attach the upper right nozzle portion 414 to the lower right nozzle portion 420 and the upper left nozzle portion 432 and the lower left nozzle portion 440.

**[0094]** The operation of the articulation control system 400 can be understood from reference to FIGS. 22 and 23. FIG. 22 illustrates articulation of the end effector 20 to the left of the articulation pivot 50. To accomplish this range of articulation, the clinician axially moves the right nozzle portion 412 in the distal direction “D-D” and the left nozzle portion 430 in the proximal direction “PD” which causes the right articulation rod 232 and left articulation rod 234 to move the end effector to the left about the articulation point 50. Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by

the right articulation band 238 and a pulling motion to the boss 96 by the left articulation band 240 which results in the articulation of the end effector 20 as shown. FIG. 23 illustrates articulation of the end effector 20 to the right of the articulation pivot 50. To accomplish this range of articulation, the clinician axially moves the right nozzle portion 412 in the proximal direction "PD" and the left nozzle portion 430 in the distal direction "DD" which causes the right articulation rod 232 and left articulation rod 234 to move the end effector 20 to the right about the articulation point 50. Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the left articulation band 240 and a pulling motion to the boss 96 by the right articulation band 238 which results in the articulation of the end effector 20 as shown. Although the articulation assembly 230 as described above employs two elongated articulation rods or members, in alternative embodiments, only one elongated articulation member is employed.

**[0095]** FIGS. 24 and 25 illustrate an alternative nozzle embodiment 410' that may be employed instead of the nozzle embodiment 410 described above. In this embodiment, the nozzle 410' is fabricated from a right nozzle portion 412' that is axially movable relative to a left nozzle portion 430'. As can be seen in those Figures, the left nozzle portion 430' has a left axial opening 460 therein that defines a left axial ledge 462 that is adapted to be slidably engaged by a right latch portion 470. Likewise the right nozzle portion 412' has a right axial opening 472 that has a right axial ledge 474 that is adapted to be slidably engaged by a left latch portion 464. Such arrangement serves to join the right nozzle portion 412' to the left nozzle portion 430' to each other about the proximal closure shaft 141 while enabling those portions to move axially relative to each other. The right nozzle portion 412' has a right aperture 452' therein for receiving the right pivot pin 450 therein and the left nozzle portion 430' has a left aperture 462' therein for receiving the left pivot pin 460 therein. The alternative nozzle 410' is otherwise operated in the manner described above to articulate the end effector 20 about the articulation pivot 50 and articulation axis B-B.

**[0096]** FIGS. 26-33 illustrate another non-limiting articulation control system embodiment of the present invention generally designated as 500. Those components that are the same as the components employed in the above-described embodiments will be labeled with the same element numbers and those of ordinary skill in the art can refer to the disclosure set forth hereinabove that explains their construction and operation. In at least one embodiment, the

articulation control system 500 includes an articulation nozzle 510 that is fabricated in multiple pieces. For example, the articulation nozzle 510 has a right nozzle portion 512 that is configured to be attached to a left nozzle portion 530. See FIG. 29. In at least one non-limiting embodiment, the right nozzle portion 512 may be provided with attachment posts 513 formed thereon that are sized to be frictionally received in corresponding attachment apertures (not shown) in the left nozzle portion 530. The right nozzle portion 512 may likewise have attachment apertures 515 therein that are sized to frictionally engage corresponding attachment posts 531 on the left nozzle portion 530 to couple the right and left nozzle portions 512, 530 together. See FIG. 29. Other fastening arrangements such as adhesive, welding, mechanical fasteners, snap features, etc. may be used to attach the right and left nozzle portions together. In various non-limiting embodiments, the right nozzle portion 512 has a proximal end 514 with actuation buttons or protrusions 516 formed thereon. The right nozzle portion 512 further has a distal end 517 that has a key 518 formed thereon for receipt within a key opening 519 in the proximal closure tube segment 141 to non-rotatably affix the right nozzle portion 512 to the proximal closure tube segment 141. Similarly, the left nozzle portion 530 has a proximal end 534 with actuation buttons or protrusions 516 formed thereon. The left nozzle portion 530 further has a distal end 537 that has a key 538 formed thereon for receipt in a key opening 539 in the proximal closure tube segment 141 to non-rotatably affix the left nozzle portion 530 to the proximal closure tube segment 141. See FIGS. 31-33.

**[0097]** In at least one non-limiting embodiment, the articulation control system 500 includes an articulation assembly 230. In at least one embodiment, the articulation assembly 230 may comprise a right articulation rod 232 and a left articulation rod 234. The right and left articulation rods 232, 234 may be configured as shown in FIG. 29 and be fabricated from stainless steel or other suitable material. The right and left articulation rods 232, 234 when movably supported within the proximal closure tube segment 141 as illustrated, serve to define a centrally disposed elongate slot 236 that is configured to accommodate the axial movement of the firing bar 180. A right articulation band 238 protrudes distally from a distal end 233 of the right articulation rod 232 and a left articulation band 240 protrudes distally from the distal end 239 of the left articulation rod 234. In various embodiments, the articulation bands 238, 240 are attached to the boss 96. For example, the bands 238, 240 may be pivotally pinned to the boss 96. The right and left articulation rods 232, 234 are slidably inserted into the hollow proximal



closure tube segment 141. The right articulation rod 232 has a right pivot pin 550 that is attached thereto and protrudes laterally therefrom through a right slot 251 in the proximal closure tube segment 141. Similarly, the left articulation rod 234 has a left pivot pin 560 that is attached thereto and protrudes laterally therefrom through a left slot 255 in the proximal closure tube segment 141.

**[0098]** In at least one non-limiting embodiment, the articulation control 500 includes an actuator assembly 562 that protrudes through openings 564, 566 in the nozzle 510 and is selectively pivotable about an actuator axis H-H that is substantially transverse to the longitudinal axis A-A. In various forms, the actuator assembly 562 comprises a first actuator portion 570 that is coupled to a second actuator portion 580. The first actuator portion 570 has a pivot hole 571 therethrough that is adapted to pivotally receive a first actuator pin 590 that is coupled to the proximal closure tube segment 141. See FIGS. 28 and 19. Similarly, the second actuator portion 580 has a pivot hole 581 therethrough that is adapted to pivotally receive a second actuator pin 592 that is coupled to the proximal closure tube segment 141. The first and second actuator pins 590, 592 serve to define the actuator axis H-H that is substantially transverse to the longitudinal axis A-A and about which the actuator assembly 562 may pivot. The first actuator portion 570 may be attached to the second actuator portion 580 by a variety of methods. In the illustrated version, for example, the first actuator portion 570 has a pair of attachment posts 572 that are sized to be frictionally received within corresponding attachment holes (not shown) in the second actuator portion 580. Likewise, the second actuator portion 580 may have attachment posts 580 that are sized to be frictionally received within attachment holes 574 in the first actuator portion, such that when the first and second actuator portions 570, 580 are joined together, they form the actuator assembly 562. However, the first and second actuator portions 570, 580 may be coupled together using any suitable means such as by adhesive, snap features, fasteners, etc.

**[0099]** As can be seen in FIGS. 28 and 29, the first actuator portion 570 operably interfaces with the first articulation rod 232 to effectuate axial movement thereof within the proximal closure tube segment 141 by means of a first cam slot 576 that is configured to receive a portion of the right pivot pin 550 therein. Thus, by pivoting the first actuator portion 570 about the actuator axis H-H, the interaction between the first cam slot 576 and the right pivot pin 550 will cause the first articulation rod 232 to axially move within the proximal closure tube segment 141.

Similarly, the second actuator portion 580 operably interfaces with the second articulation rod 234 to effectuate axial movement thereof within the proximal closure tube segment 141 by means of a second cam slot 586 that is configured to receive a portion of the left pivot pin 560 therein. Thus, when the second actuator portion 580 pivots about the actuator axis H-H, the interaction between the second cam slot 586 and the left pivot pin 560 will cause the second articulation rod 234 to axially move within the proximal closure tube segment 141.

**[0100]** The operation of the articulation control system 500 can be understood from reference to FIGS. 26 and 31-33. Turning first to FIG. 26, to rotate the proximal closure tube segment 141 and ultimately end effector 20 (shown in FIGS. 31-33) about the longitudinal axis AA, the clinician simply rotates the nozzle 510 about the longitudinal axis A-A as represented by arrow "I" in FIG. 26. FIG. 31 illustrates articulation of the end effector 20 to the left of the articulation pivot 50. To accomplish this range of articulation, the clinician simply pivots the actuator assembly 562 in the "J" direction (illustrated in FIG. 30) about the actuator axis H-H. Such movement of the actuator assembly 562 results in interaction between the right pivot pin 550 and the right cam slot 576 which results in the axial movement of the right articulation rod 232 in the distal direction "DD". Such movement of the actuator assembly 562 also results in interaction between the left pivot pin 560 and the left cam slot 586 which simultaneously results in the axial movement of the left articulation rod 234 in the proximal direction "PD". Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the right articulation band 238 and a pulling motion to the boss 96 by the left articulation band 240 which results in the articulation of the end effector 20 as shown. FIG. 33 illustrates articulation of the end effector 20 to the right of the articulation pivot 50. To accomplish this range of articulation, the clinician pivots the actuator assembly 562 in the "K" direction (shown in FIG. 30) about the actuator axis H-H. Such movement of the actuator assembly 562 results in interaction between the right pivot pin 550 and the right cam slot 576 which results in the axial movement of the right articulation rod 232 in the proximal direction "PD". Such movement of the actuator assembly 562 also results in interaction between the left pivot pin 560 and the left cam slot 586 which simultaneously results in the axial movement of the left articulation rod 234 in the distal direction "DD". Such movement of the right and left articulation rods 232, 234 result in the application of a pushing motion to the boss 96 by the left articulation band 240 and a pulling motion to the boss 96 by the right articulation band 238 which results in the articulation of the

end effector 20 as shown. Although the articulation assembly 230 as described above employs two elongated articulation rods or members, in alternative embodiments, only one elongated articulation member is employed.

[0101] FIGS. 34-42 illustrate another non-limiting articulation control system embodiment of the present invention, generally designated as 600. Those components that are the same as the components employed in the above-described embodiments will be labeled with the same element numbers and those of ordinary skill in the art can refer to the disclosure set forth hereinabove that explains their construction and operation. In this embodiment, the articulation control system 600 includes an articulation nozzle 610 that is fabricated in multiple pieces. For example, the articulation nozzle 610 has an upper nozzle portion 612 that is configured to be attached to a lower nozzle portion 630. See FIG. 38. In at least one non-limiting embodiment, the upper nozzle portion 612 may be provided with attachment posts (not shown) formed thereon that are sized to be frictionally received in corresponding attachment apertures 631 in the lower nozzle portion 630. Other fastening arrangements such as adhesive, mechanical fasteners, snap features, etc. may be used to attach the upper and lower nozzle portions 612, 630 together. In various non-limiting embodiments, the upper nozzle portion 612 has a proximal end 614 with actuation buttons or protrusions 616 formed thereon. Similarly, the lower nozzle portion 630 has a proximal end 634 with actuation buttons or protrusions 616 formed thereon.

[0102] In at least one non-limiting embodiment, the articulation control system 600 includes an articulation assembly 700. In at least one embodiment, the articulation assembly 700 may comprise a right articulation band 710 and a left articulation band 730 that are received with a proximal closure tube segment 750. The right articulation band 710 has an elongated right band portion 712 and a proximal actuation portion 714. Similarly the left articulation band 730 has a left elongated band portion 732 and a proximal actuation portion 734. The right and left articulation bands 710, 730 may be fabricated from stainless steel or other suitable material. The proximal closure tube segment 750 comprises a hollow tube that may be fabricated from, for example, stainless steel or other suitable material. In at least one non-limiting embodiment, the hollow proximal closure shaft segment 750 has a right band passage 752 and a left band passage 754 formed in its wall. The center of the proximal closure tube segment 750 provides a passage to accommodate the device's proximal frame or spine portion (not shown) as well as the firing bar (not shown) in the various manners described above. As illustrated in FIG. 38, the elongated

right articulation band portion 712 is slidably supported within the right band passage 752 and the elongated left articulation band portion 732 is slidably supported in the left band passage 754. In various non-limiting embodiments, the articulation bands 712, 732 are attached to the boss 96. See FIGS. 40 and 42. For example, the bands 238, 240 may be pivotally pinned to the boss 96. The right and left articulation rods 232, 234 are slidably inserted into the hollow proximal closure tube segment 141. The right articulation rod 232 has a right pivot pin 550 that is attached thereto and protrudes laterally therefrom through a right slot 251 in the proximal closure tube segment 141. Similarly, the left articulation rod 234 has a left pivot pin 560 that is attached thereto and protrudes laterally therefrom through a left slot 255 in the proximal closure tube segment 141.

**[0103]** The nozzle 610 is non-rotatably affixed to the proximal closure shaft segment 700 such that rotation of the nozzle 610 about the longitudinal axis A-A will result in the rotation of the end effector 20 about the longitudinal axis A-A. In at least one non-limiting embodiment, the nozzle 610 has a key 613 that extends into a slot 751 in the proximal closure tube segment 750. See FIG. 38. Such arrangement serves to non-rotatably affix the nozzle 610 to the proximal closure tube segment 750 while facilitating the axial movement of the nozzle 610 relative thereto. As can also be seen in FIGS. 37 and 38, the upper nozzle portion 612 further has an actuation notch 640 formed therein that is configured to operably engage an actuation pivot member or pivot plate 650. In at least one non-limiting embodiment, the pivot plate 650 comprises a right pivot plate portion 652 and a left pivot plate portion 670. The right pivot portion has a pivot pin 654 formed therein that is adapted to be pivotally received within a pivot hole 780 in the proximal closure tube segment 750. See FIG. 42. Similarly, the left pivot plate portion 670 has a right pivot pin 672 formed therein that is adapted to be pivotally received within a pivot hole 682 in the proximal closure tube segment 750. The right and left pivot pins 654, 672 are coaxially aligned with each other to define an actuation axis L-L about which the pivot plate 650 may pivot and which is substantially transverse to the longitudinal axis "L-L". The right and left pivot plate portions 650, 670 are attached together by posts (not shown) and holes 655 that are designed for frictional engagement. The right and left pivot plate portions 650, 670 may also be attached together by adhesive or other suitable fastener arrangement. As can be seen in FIGS. 36, 37, and 39 the proximal closure tube segment 750 has upper and lower

clearance slots 753, 755 therein to facilitate pivotal travel of the pivot plate 650 about the actuation axis L-L (FIG. 36).

**[0104]** As can be further seen in FIGS. 37-40 and 41, the right pivot plate portion 650 has a lower right actuation slot 656 that is configured to align with a corresponding lower left actuation slot 674 in the left pivot plate portion 670 to form a lower actuation slot 676 in the pivot plate 650 for receiving and operably engaging an actuator tab 716 formed on the actuator portion 714 of the actuator band assembly 710. The right pivot plate portion 650 has an upper right articulation slot 658 that is configured to align with a corresponding upper left articulation slot (not shown) in the left pivot plate portion 670 to form an upper articulation slot 678 in the pivot plate 650 for receiving and operably engaging an actuator tab 736 formed on the actuator portion 734 of the actuator band assembly 730.

**[0105]** The operation of the articulation control system 600 can be understood from reference to FIGS. 39-42. Turning first to FIGS. 39 and 40, to pivot the end effector 20 in the right direction about the pivot point 50, the clinician axially pushes the nozzle 610 axially in the distal direction "DD". Such movement of the nozzle 610 in the distal direction "DD" causes the pivot plate 650 to pivot about the actuation axis L-L in the "M" direction (FIG. 39) thereby pushing the left articulation band assembly 730 in the distal direction "DD" and pulling the right articulation band assembly 750 in the proximal direction "PD". Such axial movement of the nozzle 610 and the right and left articulation band assemblies 710, 730 result in the application of a pushing motion to the boss 96 by the left articulation band assembly 730 and a pulling motion to the boss 96 by the right articulation band assembly 710 which results in the articulation of the end effector 20 as shown in FIG. 40. Likewise, to pivot the end effector 20 about the pivot point 50 in the left direction (FIG. 42), the clinician pulls the nozzle 610 in the proximal direction "PD". Such movement of the nozzle 610 in the proximal direction "PD" causes the pivot plate 650 to pivot about the actuation axis L-L in the "N" direction (FIG. 41) thereby pushing the right articulation band assembly 710 in the distal direction "DD" and pulling the left articulation band assembly 750 in the proximal direction "PD". Such axial movement of the nozzle 610 and the right and left articulation band assemblies 710, 730 result in the application of a pushing motion to the boss 96 by the right articulation band assembly 710 and a pulling motion to the boss 96 by the left articulation band assembly 730 which results in the articulation of the end effector 20 as shown in FIG. 42. To rotate the end effector 20 about the

longitudinal axis A-A, the clinician simply rotates the nozzle 610 about the longitudinal axis A-A. Such action may be accomplished by a portion of the same hand that is supporting the handle of the instrument. Although the articulation assembly 230 as described above employs two elongated articulation rods or members, in alternative embodiments, only one elongated articulation member is employed.

**[0106]** FIGS. 43-50 illustrate another articulation control system embodiment of the present invention, generally designated as 800. Those components that are the same as the components employed in the above-described embodiments will be labeled with the same element numbers and those of ordinary skill in the art can refer to the disclosure set forth hereinabove that explains their construction and operation. In at least one non-limiting embodiment, the articulation control system 800 includes an articulation nozzle 810 that is fabricated in multiple pieces. For example, the articulation nozzle 810 has a first nozzle portion 812 that is configured to be attached to a second nozzle portion 830. See FIGS. 44-46. In at least one non-limiting embodiment, the right nozzle portion 812 and left nozzle portion 830 are attached together by a collection of posts 813 that are frictionally received in corresponding apertures 815. Other fastening arrangements such as adhesive, mechanical fasteners, snap features, etc. may be used to attach the first and second nozzle portions 812, 830 together. In various non-limiting embodiments, the first nozzle portion 812 has a proximal end 814 with actuation buttons or protrusions 816 formed thereon. Similarly, the second nozzle portion 830 has a proximal end 834 with actuation buttons or protrusions 816 formed thereon.

**[0107]** In at least one non-limiting embodiment, the articulation control system 800 includes a selectively lockable articulation assembly 900. In at least one non-limiting embodiment, the articulation assembly 900 may comprise a right articulation band 910 and a left articulation band 930 that are received with a spine segment 850 that is affixed to the instrument handle (not shown). The right articulation band 910 has an elongated right band portion 912 and a proximal actuation portion 914 that has a right actuation tab 916 formed thereon. Similarly the left articulation band 930 has a left elongated band portion 932 and a proximal actuation portion 934 that has a left actuation tab 936 formed thereon. The right and left articulation bands 910, 930 may be fabricated from stainless steel or other suitable material.

**[0108]** In various non-limiting embodiments, the spine segment 850 comprises a hollow tube that may be fabricated from, for example, stainless steel or other suitable material. In at least

one non-limiting embodiment, the hollow spine segment 850 has a right band passage 852 and a left band passage 854 formed in its wall. The center of the spine segment 850 provides a passage 851 sized and configured to accommodate the device's proximal frame or spine portion 100 (shown in FIG. 2) as well as the firing bar 180 (shown in FIG. 2) in the various manners described above. As illustrated in FIG. 47, the elongated right articulation band portion 912 is slidably supported within the right band passage 852 and the elongated left articulation band portion 932 is slidably supported in the left band passage 854. In various non-limiting embodiments, the articulation bands 912, 932 are attached to the boss 96 of the end effector frame 90 as was discussed above.

**[0109]** As can be seen in FIGS. 44-47 and 49, in at least one non-limiting embodiment, the right and left actuation tabs 916, 936 are configured for operable engagement with an actuation or pivot plate 980. In various embodiments, the pivot plate 980 comprises a first pivot plate portion 982 and a second pivot plate portion 990. The first pivot plate portion 982 has a first pivot pin 984 formed thereon that is adapted to be pivotally received within a first pivot hole 853 in the spine segment 850. See FIGS. 44 and 46. Similarly, the second pivot plate portion 990 has a second pivot pin 992 formed thereon that is adapted to be pivotally received within a second pivot hole 852 in the spine segment 850. The first pivot pin 984 also extends through an elongated first slot 954 in a proximal closure tube segment 950. Similarly the second pivot pin 992 extends through an elongated second slot 956 in the proximal closure tube segment 950. Such arrangement enables the proximal closure tube segment 950 to move axially on the spine segment 850 while facilitating pivotal travel of the pivot plate 980 relative thereto. The first and second pivot pins 984, 992 are coaxially aligned with each other to define an actuation axis N-N about which the pivot plate 980 may pivot and which is substantially transverse to the longitudinal axis "A-A". See FIG. 45. The first and second pivot plate portions 982, 990 are attached together by posts 983 and holes 993 that are designed for frictional engagement. The first and second pivot plate portions 982, 990 may also be attached together by adhesive, welding, snap features or other suitable fastener arrangements.

**[0110]** As can be seen in FIG. 49, the spine segment 850 has a right tab slot 860 through which right actuator tab 916 extends. The spine segment 850 further has a left tab slot 862 through which the left articulation tab 936 extends. In addition, the right actuator tab 916 extends through a right slot 960 in the proximal closure tube segment 950 and the left actuator tab 936

extends through a left slot 962 in the proximal closure tube segment 950. As can be further seen in FIGS. 44-47, the first pivot plate portion 982 has a right actuation slot 987 that is configured to align with a corresponding right actuation slot (not shown) in the second pivot plate portion 990 to form a right articulation slot 995 in the pivot plate 980 for receiving and operably engaging the right actuator tab 916 therein. Similarly, the right pivot plate portion 982 has a left actuation slot 988 that is configured to align with a corresponding left actuation slot 996 in the second pivot plate portion 990 to form a left articulation slot 997 in the pivot plate 980 for receiving and operably engaging the left actuator tab 936 therein.

**[0111]** In various non-limiting embodiments, the articulation nozzle 810 is non-rotatably affixed to a proximal closure shaft segment 950 such that rotation of the articulation nozzle 610 about the longitudinal axis A-A will result in the rotation of the end effector 20 about the longitudinal axis A-A. In at least one non-limiting embodiment, the articulation nozzle 810 has a key 818 that extends into a corresponding elongated slot 951 in the proximal closure tube segment 950 and corresponding slot 859 in the spine segment 850 as shown in FIG. 49. Such arrangement facilitates the axial movement of the articulation nozzle 810 relative to the proximal closure tube segment 950 and spine segment 950 while also facilitating the rotation of the proximal closure tube segment 950 as a unit by rotating the nozzle 810 about the longitudinal axis A-A. As can also be seen in FIGS. 44 and 49, an actuator notch 817 is provided in the articulation nozzle 810 to engage the pivot plate 980. Thus, axial movement of the nozzle 810 will cause the pivot plate 980 to pivot about the actuation axis N-N.

**[0112]** To pivot the end effector in the left direction about the pivot point or articulation axis, the clinician moves the articulation nozzle 810 axially in the distal direction "DD". Such movement of the articulation nozzle 810 in the distal direction "DD" causes the pivot plate 980 to pivot about the actuation axis N-N in thereby moving the right articulation band 910 in the distal direction "DD" and pulling the left articulation band 930 in the proximal direction "PD". Such axial movement of the articulation nozzle 810 and the right and left articulation bands 910, 930 result in the application of a pushing motion to the boss 96 by the right articulation band 910 and a pulling motion to the boss 96 by the left articulation band assembly 930 which results in the articulation of the end effector. See FIG. 49. Likewise, to pivot the end effector about the pivot point or the articulation axis in the right direction, the clinician pulls the articulation nozzle 810 in the proximal direction "PD". Such movement of the nozzle 810 in the proximal direction



“PD” causes the pivot plate 980 to pivot about the actuation axis N-N thereby pushing the left articulation band 930 in the distal direction “DD” and pulling the right articulation band 910 in the proximal direction “PD”. Such axial movement of the articulation nozzle 810 and the right and left articulation bands 910, 930 result in the application of a pushing motion to the boss 96 by the left articulation band 930 and a pulling motion to the boss 96 by the right articulation band 910 which results in the articulation of the end effector to the right of the longitudinal axis A-A. To rotate the end effector about the longitudinal axis A-A, the clinician simply rotates the articulation nozzle 810 about the longitudinal axis A-A.

**[0113]** As was discussed above, the proximal closure tube segment 950 interfaces with the closure trigger, such that when the clinician actuates the closure trigger, the proximal closure tube segment 950 moves in the distal direction. In various non-limiting embodiments, the distal end portion of the proximal closure tube segment may be configured as shown, for example, in FIG. 2, to be pivotally coupled to the distal closure tube segment 150 to apply opening and closing motions to the anvil 130. In various non-limiting embodiments, the articulation locking system 1000 is configured to be locked when the proximal closure tube segment 950 is axially moved in the distal direction “DD” and be unlocked when the proximal closure tube segment 950 is axially moved in the proximal direction “PD”.

**[0114]** More specifically, as can be seen in FIG. 45, the right articulation band 910 has a plurality of right locking detents 1010 formed therein. Each detent 1010 corresponds to a particular angular or articulated orientation of the end effector about the articulation axis. The right locking detents 1010 are configured to be engaged by a right locking ball 1012 that is movably supported in a right locking hole 1014 in the spine segment 850. Similarly, the left articulation band 930 has a plurality of left locking detents 1020 formed therein that are configured to be engaged by a left locking ball 1022 that is movably supported in a left locking hole 1024 in the spine segment 850. See FIG. 49. The right locking ball 1012 is received in an elongated right locking cavity 1016 formed in the proximal closure tube segment 950. Such elongated locking cavity 1016 provides sufficient clearance for the right locking ball 1012 to move radially as the right articulation band 912 is moved axially within the spine segment 850. As can be most particularly seen in FIGS. 48 and 50, the proximal end 1017 of the elongated right locking cavity 1016 has a locking ramp 1018 formed thereon. Similarly, the left locking ball 1022 is received in an elongated left locking cavity 1026 formed in the proximal closure

tube segment 950. Such elongated locking cavity 1026 provides sufficient clearance for the left locking ball 1022 to move radially as the left articulation band 932 is moved axially within the spine segment 850. As can be most particularly seen in FIG. 49, the proximal end of the elongated left locking cavity 1026 has a left locking ramp 1028 formed thereon.

**[0115]** The operation of the articulation control system 800 and articulation locking system 1000 will now be described with reference to FIGS. 47-50. In various non-limiting embodiments, when the clinician desires to articulate the end effector about the articulation axis, the nozzle 810 is axially moved in a desired direction in the manner described above. The clinician may accomplish this action with the same hand that he or she is using to grasp and support the handle of the instrument. During the articulation process, the closure trigger has not been actuated and the proximal closure tube 950 is in the “open” position as shown in FIGS. 47 and 48. As the right articulation band 912 is moved axially, the right locking ball 1012 is permitted to move sufficiently radially away from the right articulation band 912 to permit it to move axially thereby and as the left articulation band 932 is moved axially, the left locking ball 1022 is permitted to move sufficiently radially away from the left articulation band 932 to permit it to move axially thereby. As the clinician advances the nozzle 810 in the appropriate axial direction and the right and left articulation bands 912, 932 move past the right and left locking balls 1012, 1022, respectively, the clinician receives tactile feedback as the locking detents 1010, 1020 movably engage the locking balls 1012, 1022, respectively. Once the clinician has attained the desired amount of articulation which corresponds to a position wherein the right locking ball 1012 engages a right locking detent 1010 that corresponds with that articulated position and the left locking ball 1022 likewise engages the left locking detent 1020 that corresponds with that articulated position, the clinician can then activate the closure trigger.

**[0116]** As discussed above, when the clinician activates the closure trigger, the proximal closure tube segment 950 is axially advanced in the distal direction “DD”. As the proximal closure tube segment 950 is distally advanced, the right locking ramp 1018 engages the right locking ball 1012 and presses it radially inward into locking engagement with the corresponding right locking detent 1010. Likewise, the left locking ramp 1028 engages the left locking ball 1022 and presses it radially inward into locking engagement with the corresponding left locking detent 1020. Further axial advancement of the proximal closure tube segment 950 in the distal direction “DD” will continue to press the right and left locking balls 1012, 1022 into locking

engagement to retain the end effector in the desired articulated position while the anvil is closed and the instrument is further used. After the end effector has been used “fired” and the closure trigger is unlocked and returned to the open position, the proximal closure tube segment 950 is moved in the proximal direction “PD” to the starting position wherein the articulation bands 912, 932 may be axially moved if desired to orient the end effector in the desired position for removal from the surgical site. Thus, such articulation locking system is essentially activated by the application of closing motions to the end effector. Although the articulation assembly as described above employs two elongated articulation rods or members, in alternative embodiments, only one elongated articulation member is employed. Likewise, in alternative embodiments, the articulation locking system may only employ one locking ball arrangement configured to engage locking detents in the corresponding elongated articulation member. Also, in embodiments that employ two elongated articulation members, only one locking ball may be employed to lock one of the articulation members upon application of a closure force to the end effector.

**[0117]** The devices disclosed herein can be designed to be disposed of after a single use, or they can be designed to be used multiple times. In either case, however, the device can be reconditioned for reuse after at least one use. Reconditioning can include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, the device can be disassembled, and any number of the particular pieces or parts of the device can be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, the device can be reassembled for subsequent use either at a reconditioning facility, or by a surgical team immediately prior to a surgical procedure. Those skilled in the art will appreciate that reconditioning of a device can utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

**[0118]** Preferably, the inventions described herein will be processed before surgery. First, a new or used instrument is obtained and if necessary cleaned. The instrument can then be sterilized. In one sterilization technique, the instrument is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and instrument are then placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-

energy electrons. The radiation kills bacteria on the instrument and in the container. The sterilized instrument can then be stored in the sterile container. The sealed container keeps the instrument sterile until it is opened in the medical facility.

**[0119]** Any patent, publication, or other disclosure material, in whole or in part, that is said to be incorporated by reference herein is incorporated herein only to the extent that the incorporated materials does not conflict with existing definitions, statements, or other disclosure material set forth in this disclosure. As such, and to the extent necessary, the disclosure as explicitly set forth herein supersedes any conflicting material incorporated herein by reference. Any material, or portion thereof, that is said to be incorporated by reference herein, but which conflicts with existing definitions, statements, or other disclosure material set forth herein will only be incorporated to the extent that no conflict arises between that incorporated material and the existing disclosure material.

**[0120]** While this invention has been described as having exemplary designs, the present invention may be further modified within the spirit and scope of the disclosure. This application is therefore intended to cover any variations, uses, or adaptations of the invention using its general principles. Further, this application is intended to cover such departures from the present disclosure as come within known or customary practice in the art to which this invention pertains.

What is claimed is:

1. A surgical instrument comprising:
  - an elongate shaft defining a longitudinal axis;
  - an end effector coupled to said elongate shaft for selective pivotal travel relative to said elongate shaft, said end effector having at least one movable portion responsive to opening and closing motions;
  - a closure member interfacing with said at least one movable portion of said end effector to selectively apply said closing motion thereto;
  - an articulation control system operably interfacing with said end effector to apply articulation motions thereto; and
  - an articulation lock system interfacing with said articulation control system and said closure member, said articulation lock system configured to move from an unlocked position wherein said articulation control system applies said articulation motions to said end effector and a locked position wherein said articulation lock system prevents said articulation control system from applying said articulation motions to said end effector upon application of said closure motion by said closure member.
  
2. The surgical instrument of claim 1 wherein said articulation control system comprises a nozzle supported relative to said elongate shaft such that said nozzle may be axially moved in first and second axial directions relative to said elongate shaft and rotation of said nozzle about said longitudinal axis causes said end effector to rotate about said longitudinal axis and wherein said articulation control system comprises an articulation assembly operably interfacing with said end effector and said nozzle such that movement of said nozzle in said first axial direction causes said articulation assembly to apply a first articulation motion to said end effector and movement of said nozzle in said second axial direction causes said articulation assembly to apply a second articulation motion to said end effector.
  
3. The surgical instrument of claim 2 wherein said articulation assembly comprises:

a first elongated articulation member having a first proximal end and a first distal end wherein the first distal end operably interfaces with said end effector and said first proximal end operably interfaces with said nozzle; and

a second elongated articulation member having a second proximal end and a second distal end wherein the second distal end operably interfaces with said end effector and wherein said second proximal end operably interfaces with said nozzle.

4. The surgical instrument of claim 3 wherein said articulation lock system comprises a first locking member movably interfacing with said closure member and said first elongated articulation member such that, upon application of said closure motion to said end effector by said closure member, said first locking member is moved into locking engagement with said first elongated articulation member.

5. The surgical instrument of claim 4 wherein said end effector is articulatable to various articulated positions and wherein said first elongated articulation member comprises a plurality of first locking positions corresponding to said various articulated positions.

6. The surgical instrument of claim 5 wherein said first locking member comprises a first locking ball movably supported for travel between an unlocked position and said plurality of locked positions.

7. The surgical instrument of claim 4 wherein said articulation lock system further comprises a second locking member movably interfacing with said closure member and said second elongated articulation member such that upon application of said closure motion to said end effector by said closure member, said second locking member is moved into locking engagement with said second elongated articulation member.

8. The surgical instrument of claim 7 wherein said second elongated articulation member defines a plurality of second locking positions corresponding to said plurality of said first locking positions.

9. The surgical instrument of claim 8 wherein said second locking member comprises a second locking ball movably supported for movable travel between said closure member and said second elongated articulation member and wherein said plurality of said second locking positions comprise a plurality of second locking detents in said second elongated articulation member for selective locking engagement with said second locking ball.

10. The surgical instrument of claim 1 wherein said end effector comprises a surgical cutting and fastening instrument.

11. A surgical instrument comprising:  
an elongate shaft defining a longitudinal axis;  
an end effector coupled to said elongate shaft for selective pivotal travel relative to said elongate shaft to various articulated positions, said end effector having at least one portion movably responsive to opening and closing motions;  
a closure member interfacing with said at least one portion of said end effector to apply said closure motion thereto when said closure member is moved in a closure direction and to apply said opening motion thereto when said closure member is moved in an opening direction;  
a first elongated articulation member movably supported relative to said closure member and configured to apply a first articulation motion to said end effector when said first elongated articulation member is moved in a first actuation direction and a second articulation motion to said end effector when said first articulation member is moved in a second actuation direction;  
and  
a locking member operably interfacing with said closure member and said first elongated articulation member such that when said closure member is moved in said closing direction, said locking member lockingly engages said first elongated articulation member to prevent movement thereof in said first and second actuation directions and when said closure member is moved in said opening direction, said locking member disengages said first articulation member to enable said first articulation member to move in said first and second actuation directions.

12. The surgical instrument of claim 11 wherein said first elongated articulation member defines a plurality of first locking positions corresponding to said various articulated positions.

13. The surgical instrument of claim 12 wherein said locking member comprises a first locking ball movably supported for radial travel between said closure member and said first elongated articulation member and wherein said plurality of locking positions comprise a plurality of first locking detents in said first elongated articulation member for selective locking engagement with said first locking ball.

14. The surgical instrument of claim 11 further comprising:  
a second elongated articulation member movably supported relative to said closure member; and  
a second locking member operably interfacing with said closure member and said second elongated articulation member such that when said closure member is moved in said closing direction, said second locking member lockingly engages said second elongated articulation member to prevent movement thereof and when said closure member is moved in said opening direction, said second locking member disengages said second elongated articulation member to enable said second articulation member to move.

15. The surgical instrument of claim 14 wherein said first elongated articulation member comprises a plurality of first locking positions corresponding to said various articulated positions and wherein said second elongated articulation member comprises a plurality of second locking positions corresponding to said plurality of said first locking positions.

16. The surgical instrument of claim 15 wherein said locking member comprises a first locking ball movably supported for radial travel between said closure member and said first elongated articulation member and wherein said plurality of locking positions comprise a plurality of first locking detents in said first elongated articulation member for selective locking engagement with said first locking ball and wherein said second locking member comprises a second locking ball movably supported for radial travel between said closure member and said



second elongated articulation member and wherein said plurality of said second locking positions comprise a plurality of second locking detents in said second elongated articulation member for selective locking engagement with said second locking ball.

17. The surgical instrument of claim 11 wherein said end effector comprises a surgical cutting and fastening instrument.

18. A method of operating a surgical instrument, said method comprising:  
providing a surgical instrument having an end effector having at least a portion responsive to opening and closing motions and being articulatable about a longitudinal axis to a plurality of articulated positions in response to articulation motions;  
applying an articulation motion to the end effector to articulate the end effector to one of the articulated positions; and  
applying a closing motion to the end effector such that upon application of said closing motion, the end effector is retained in the articulated position.

19. The method of claim 18 further comprising:  
applying an opening motion to the end effector;  
applying another articulation motion to the end effector to articulate the end effector into another one of the articulated position;  
applying the closing motion to the end effector such that upon application of said closing motion, the end effector is retained in the another articulated position.

20. The method of claim 18 wherein the surgical instrument has a handle that operably supports a closure trigger for applying the closing motions and an articulation system for applying the articulation motions and wherein said method further comprises:  
grasping the handle in a single hand;  
activating the articulation system with the hand that is grasping the handle; and  
activating the closure trigger with the hand that is grasping the handle.

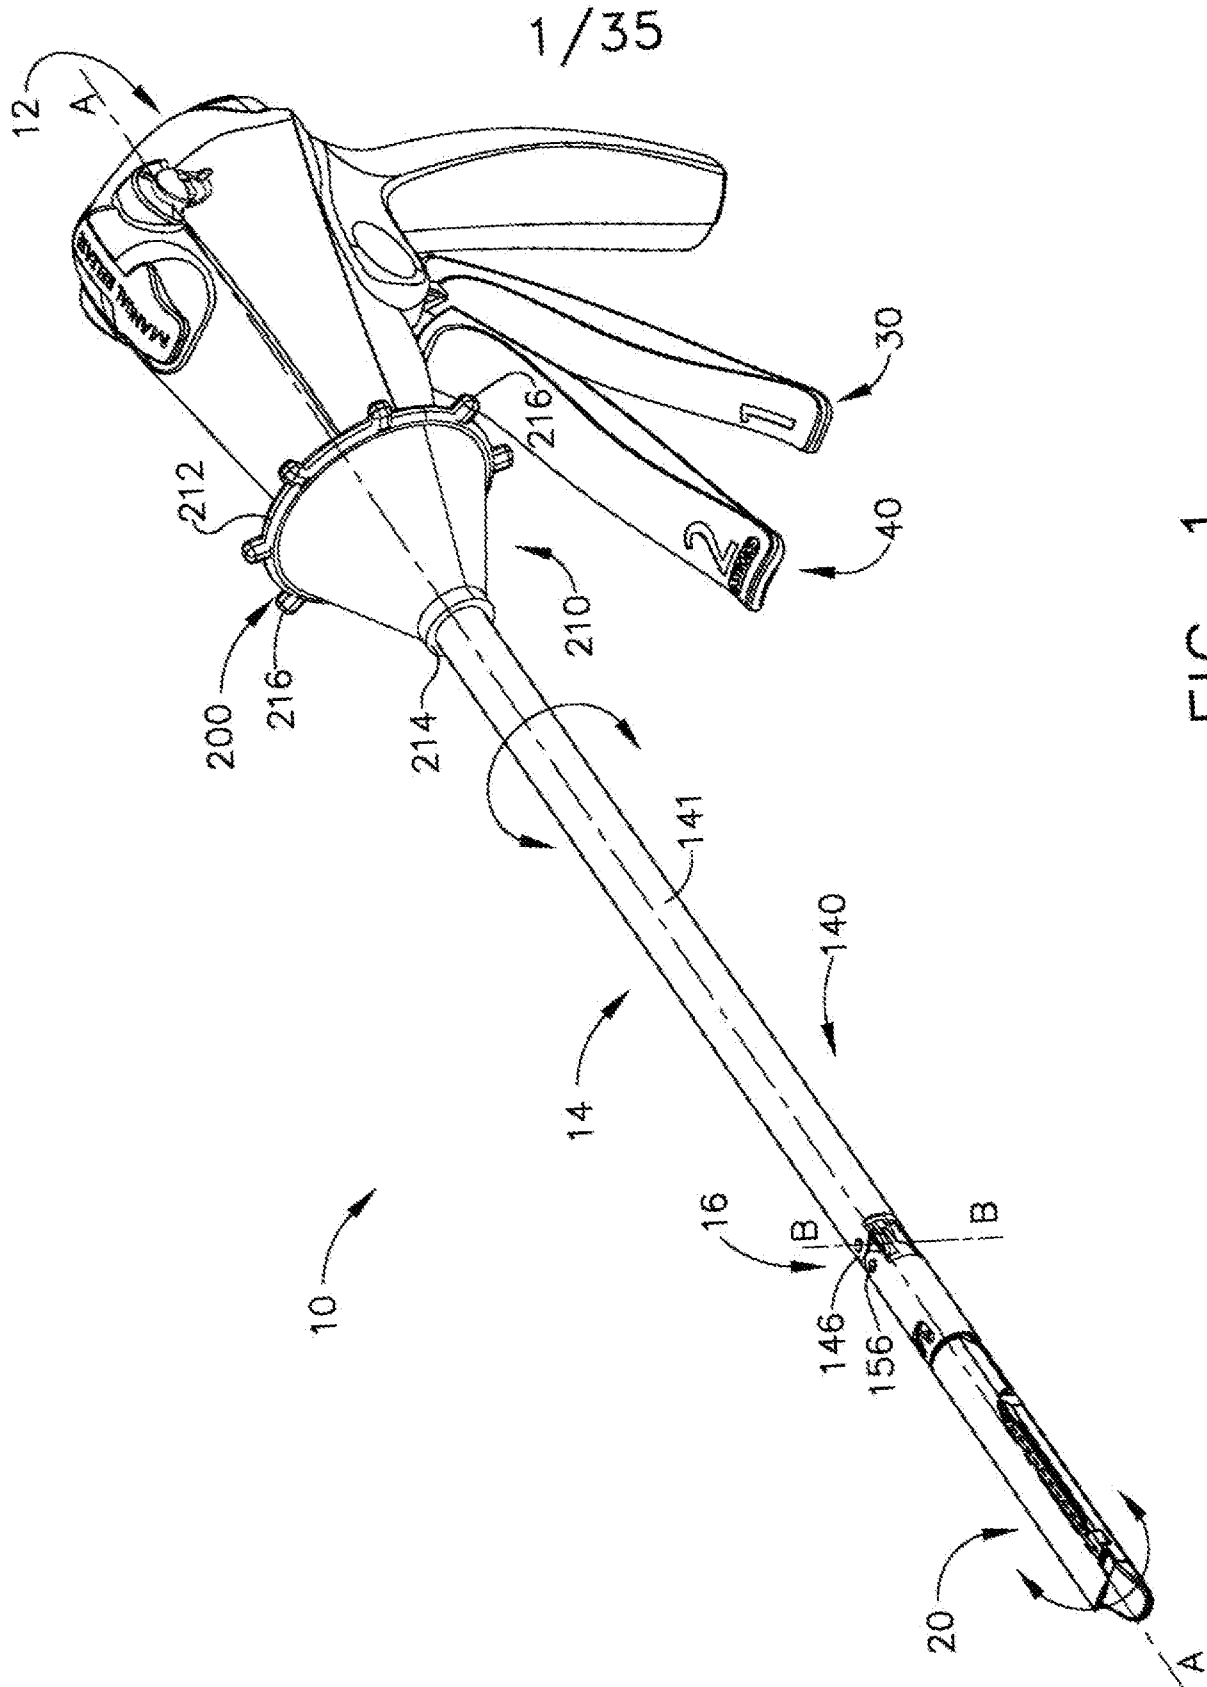


FIG. 1

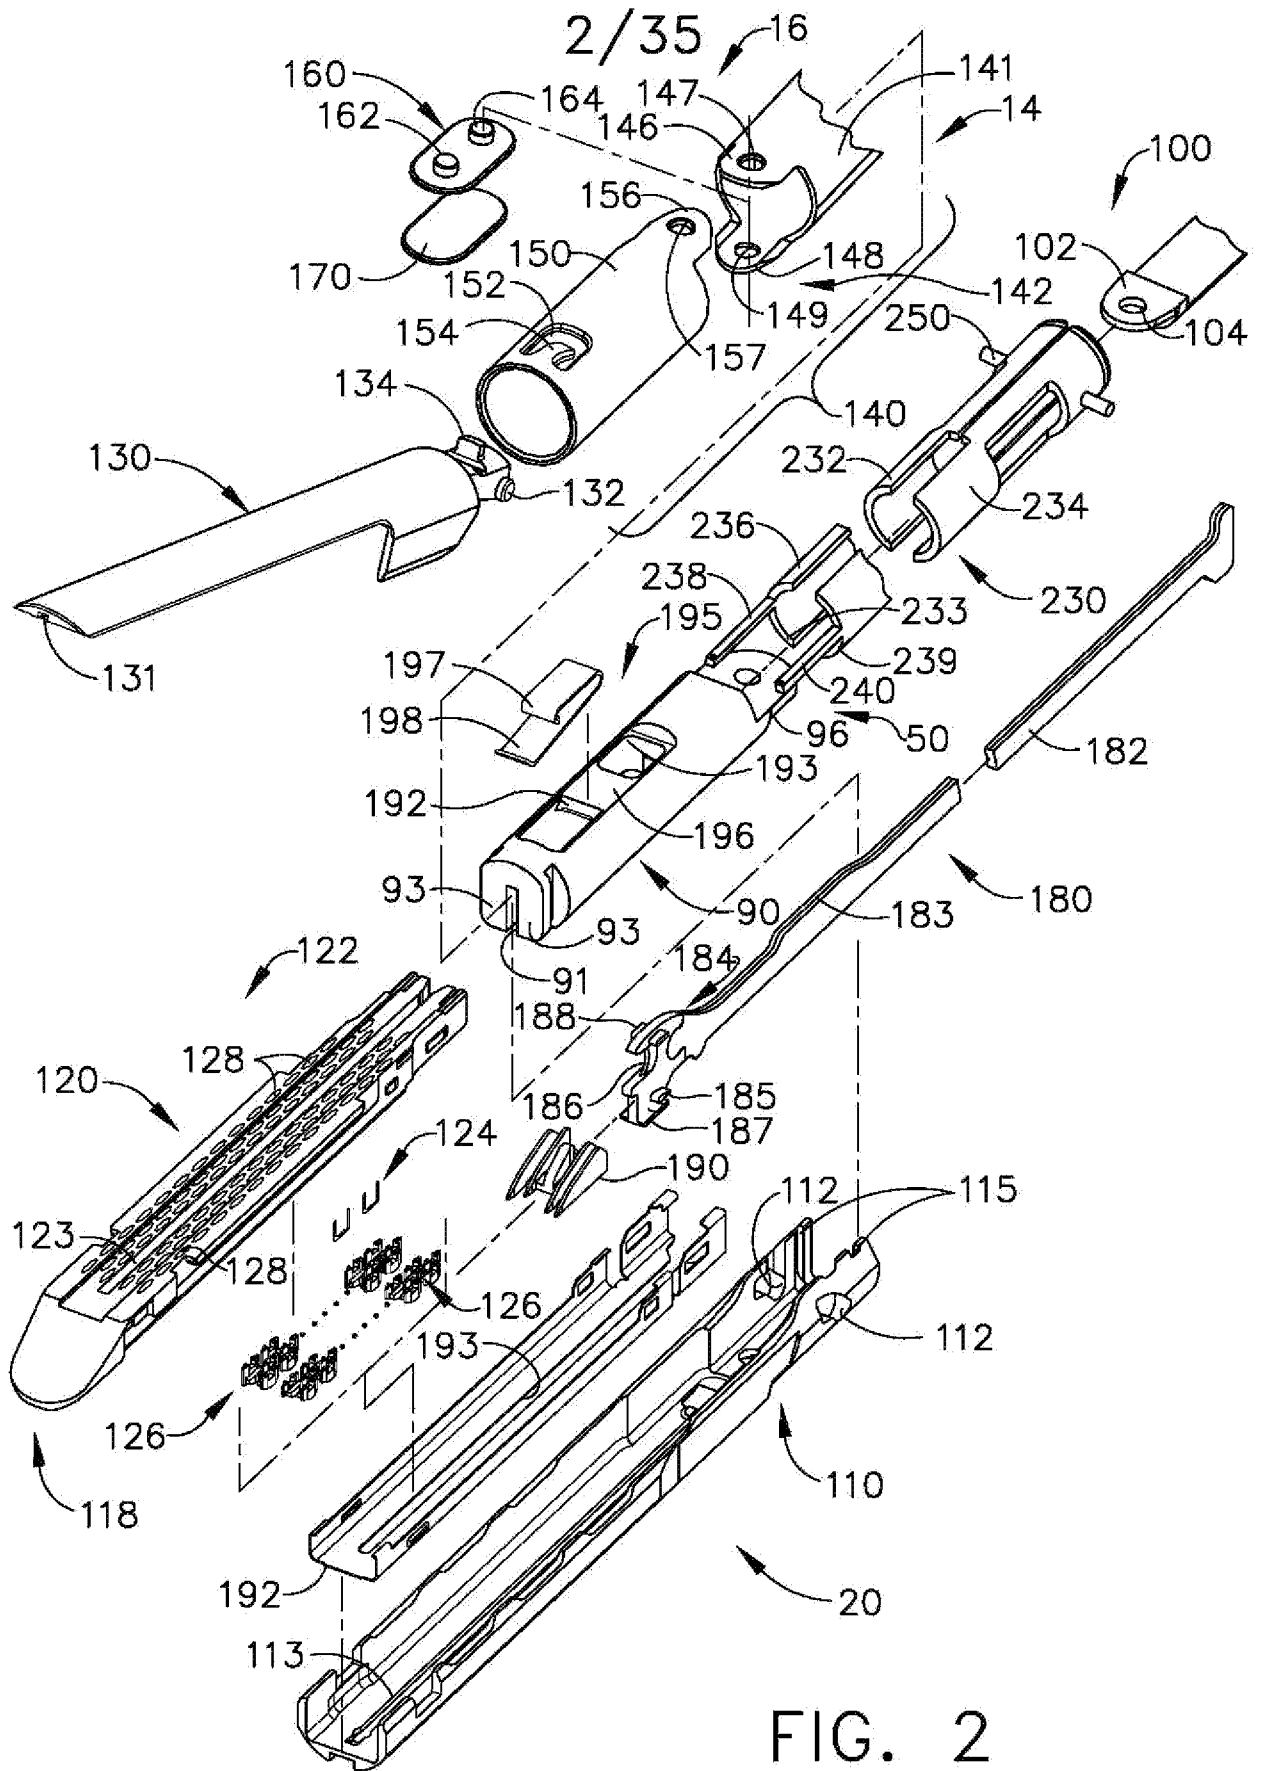


FIG. 2

3/35

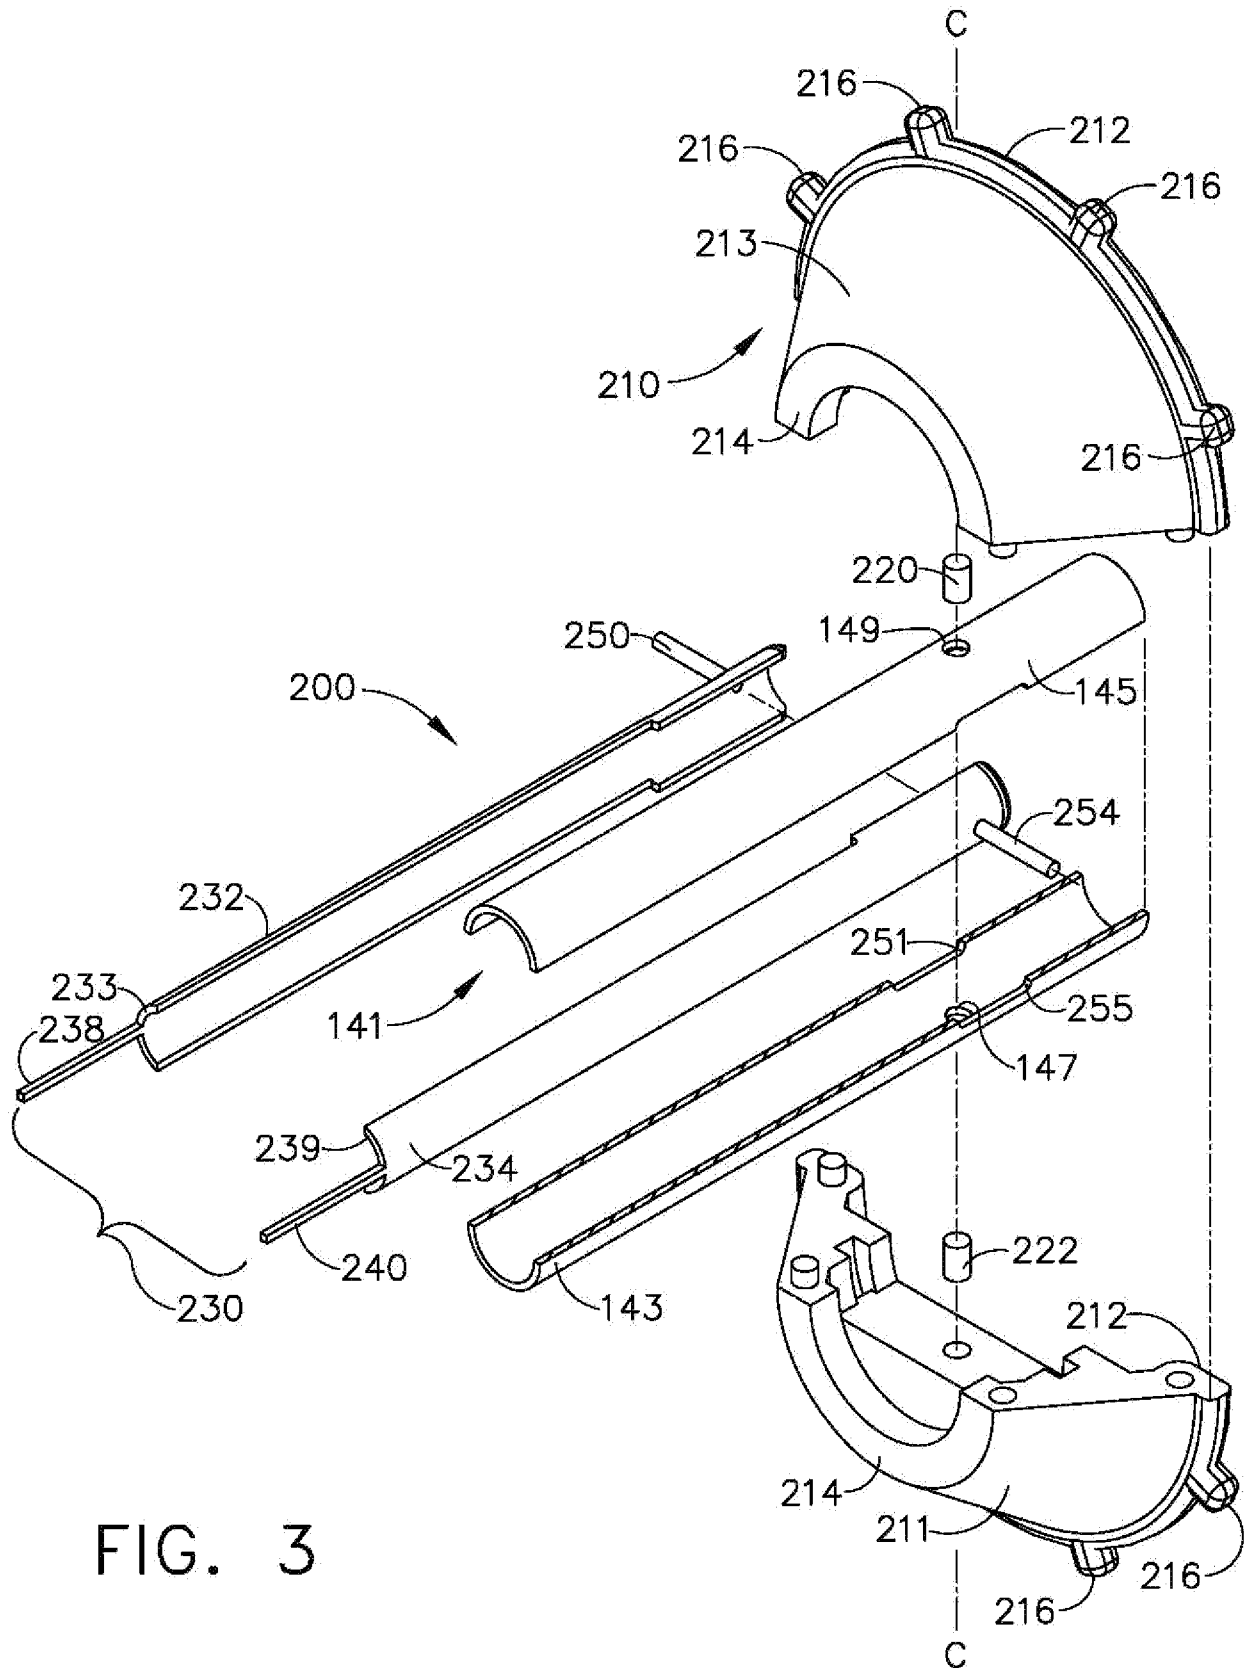


FIG. 3

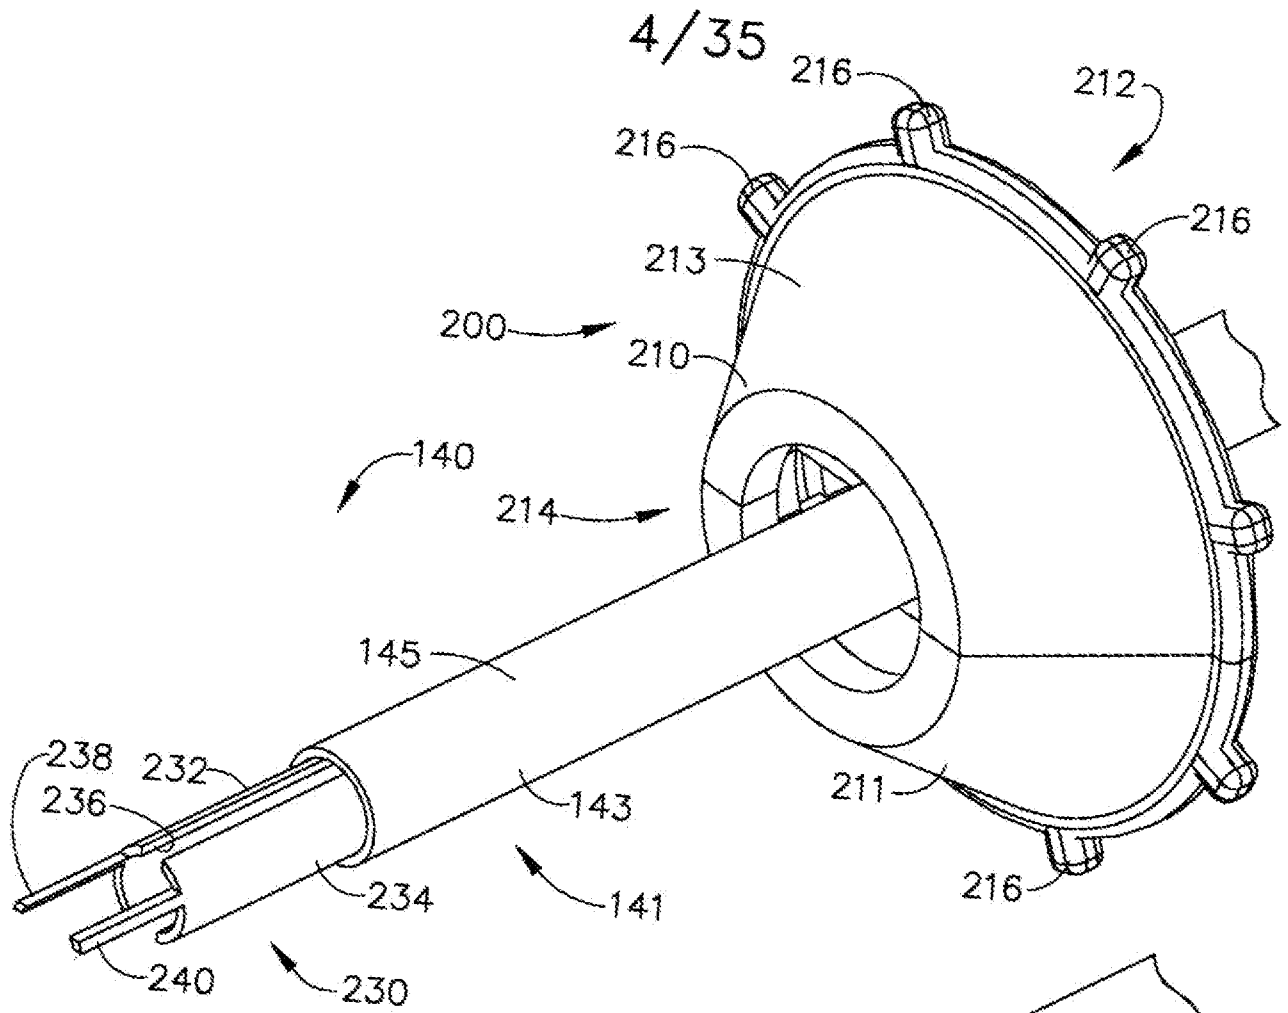


FIG. 4

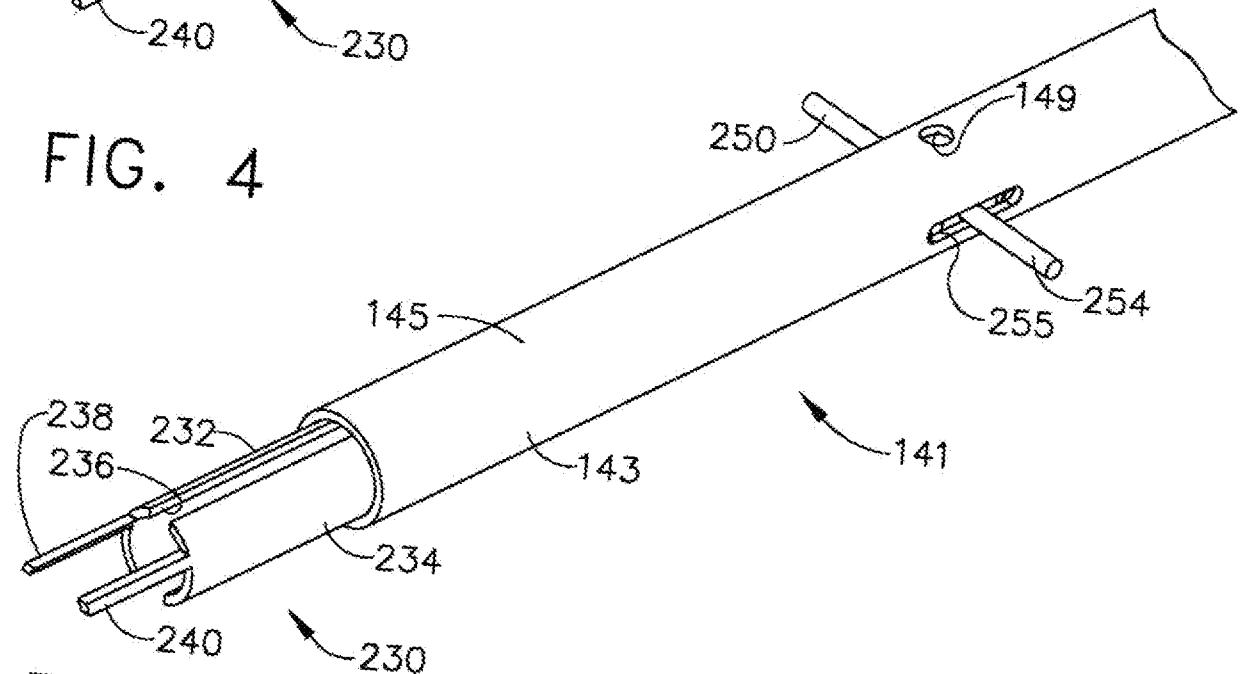


FIG. 5

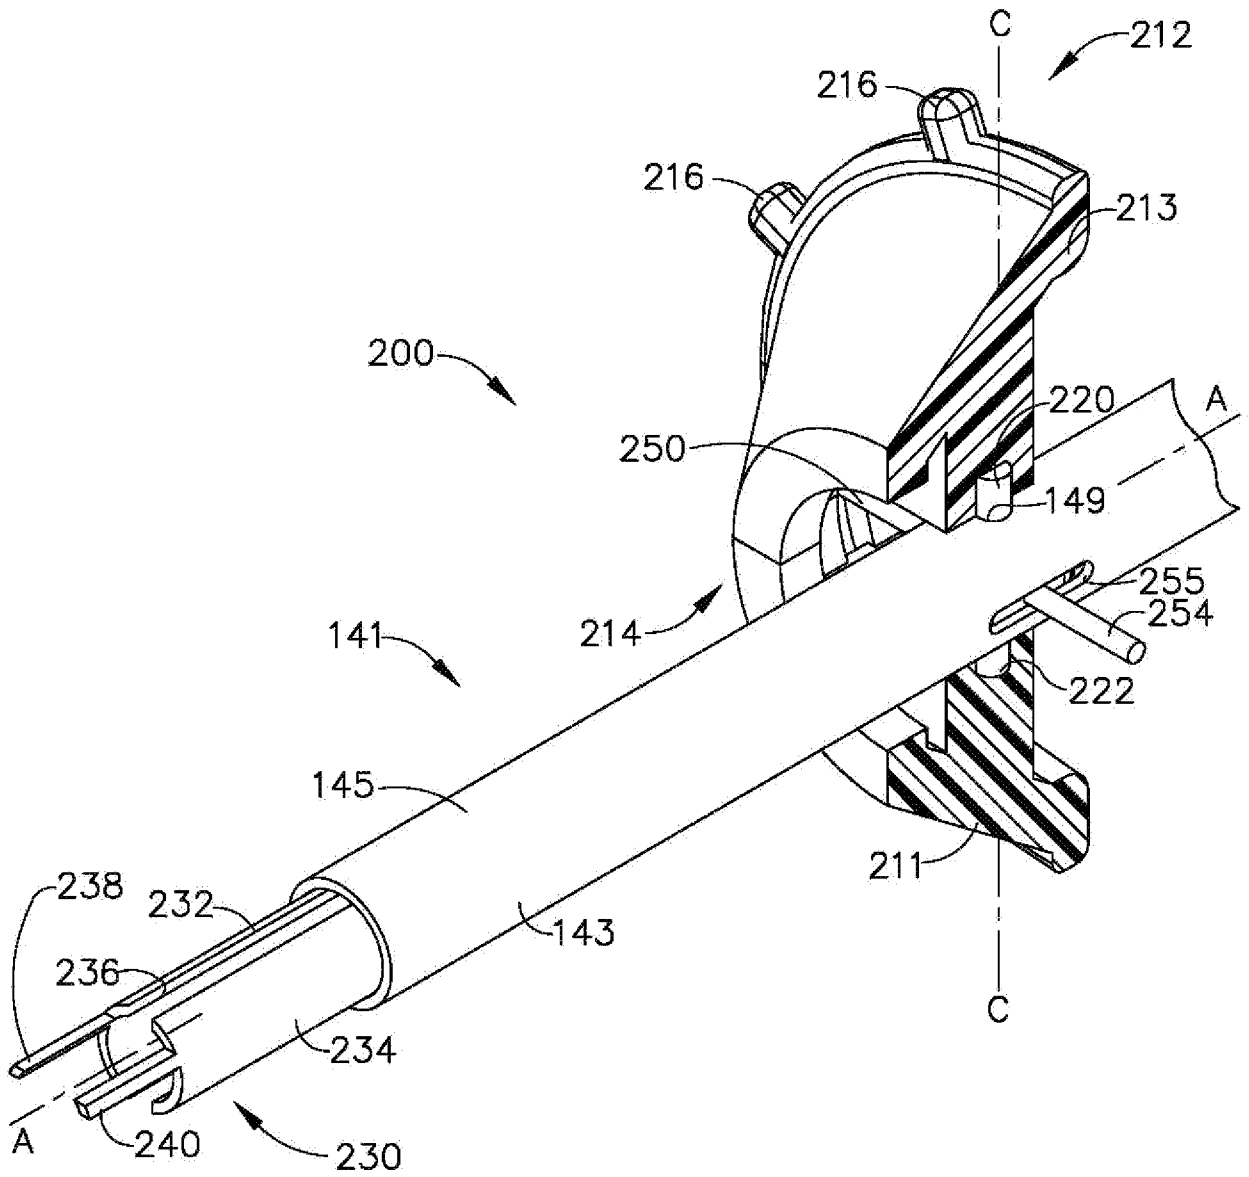


FIG. 6

6/35

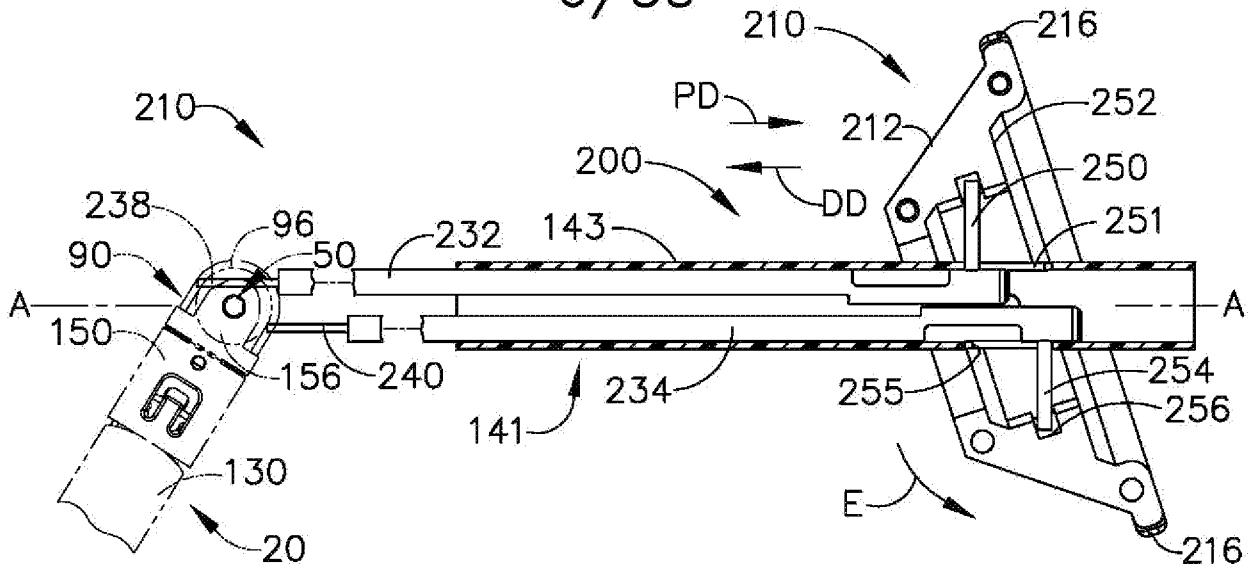


FIG. 7

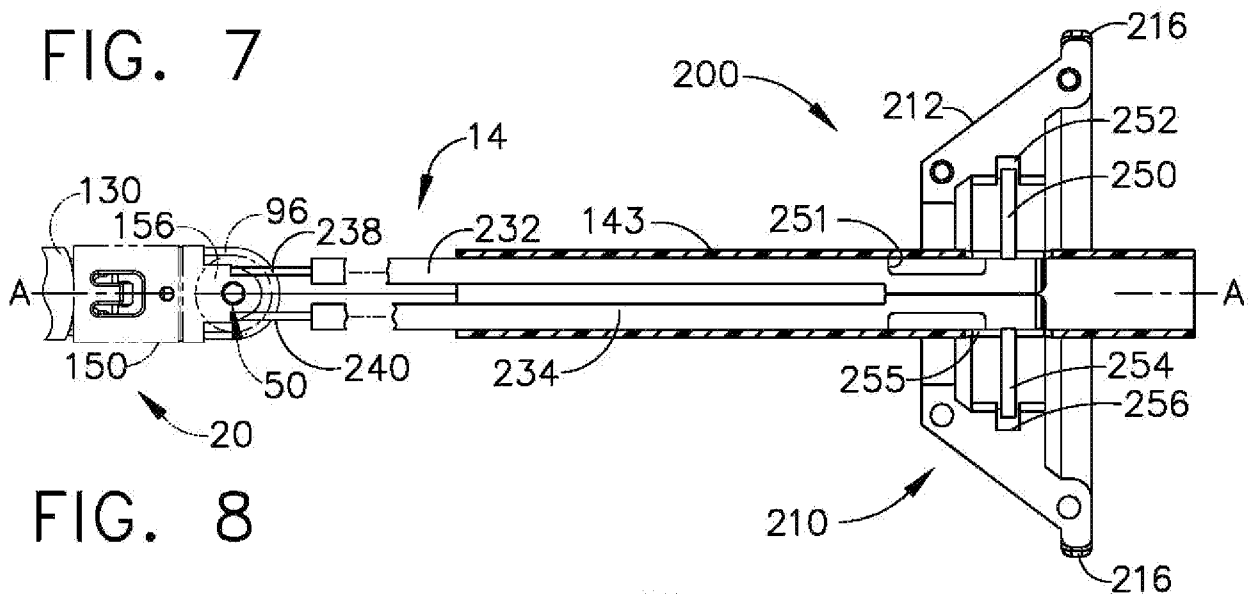


FIG. 8

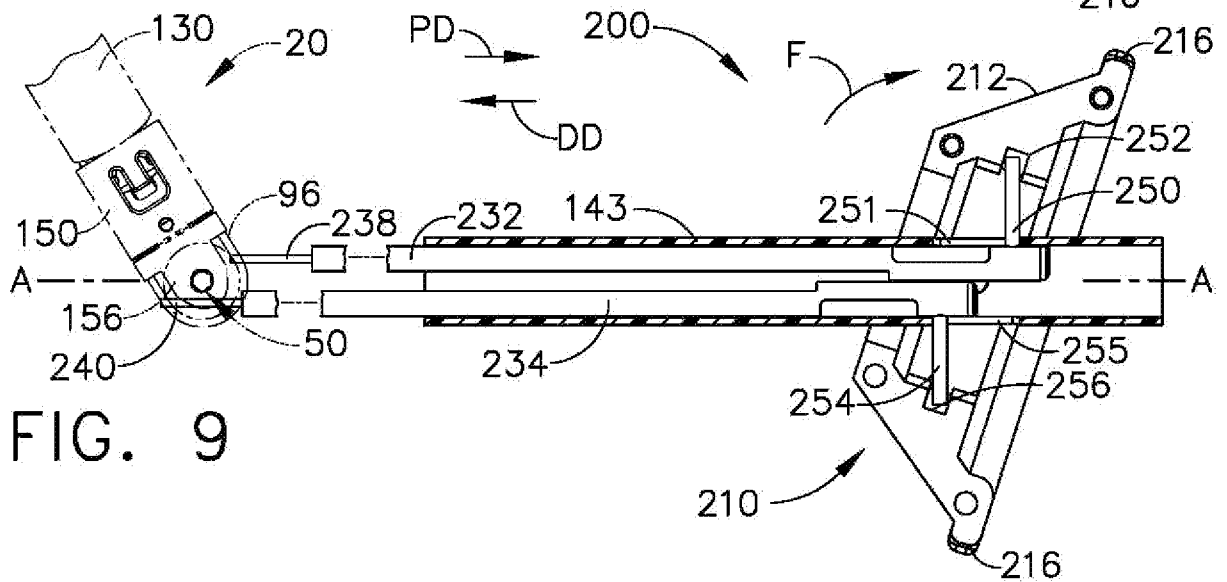
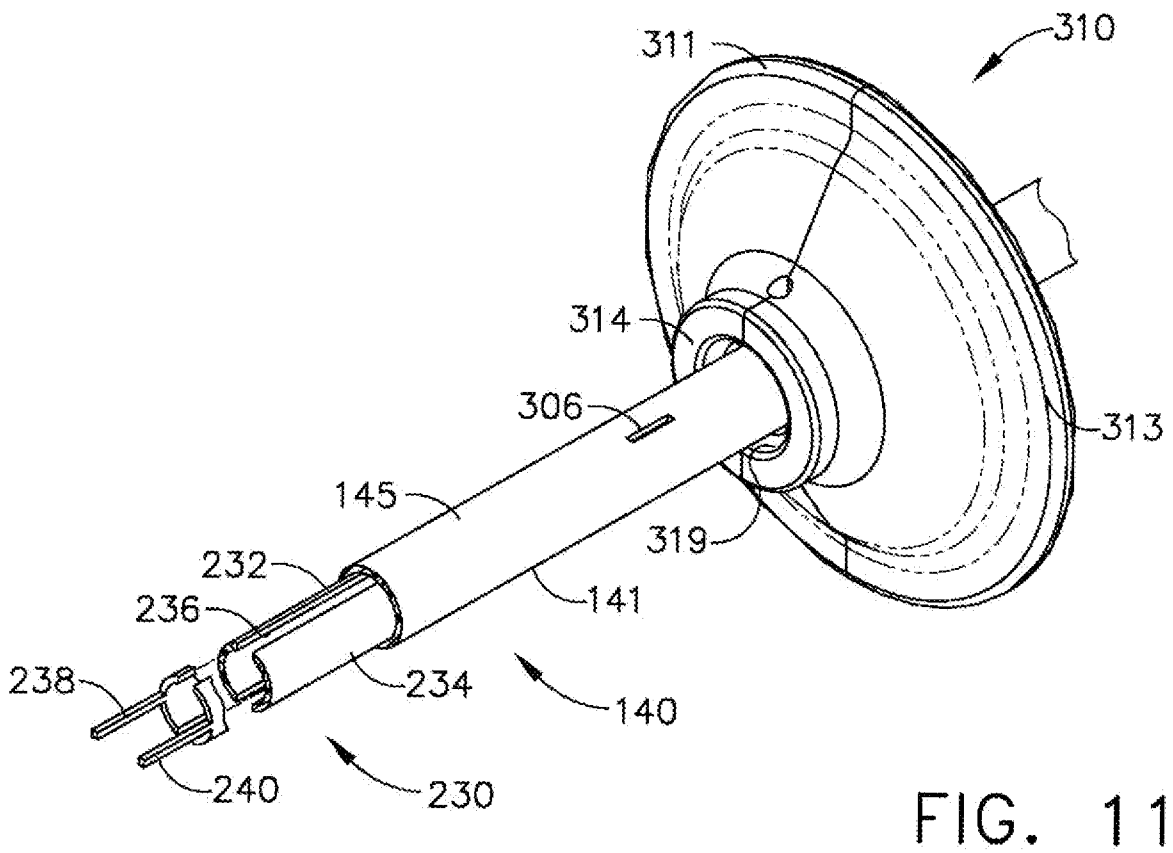
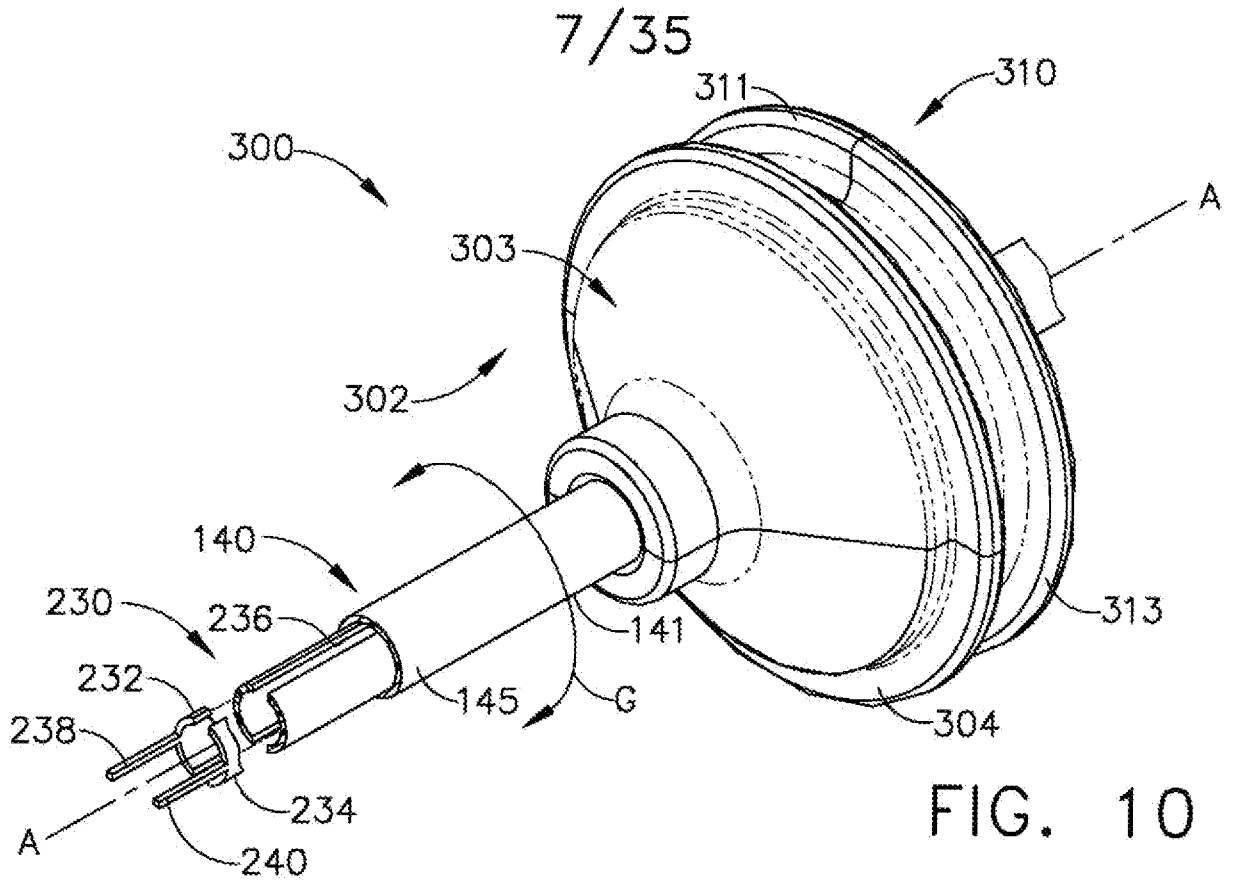


FIG. 9





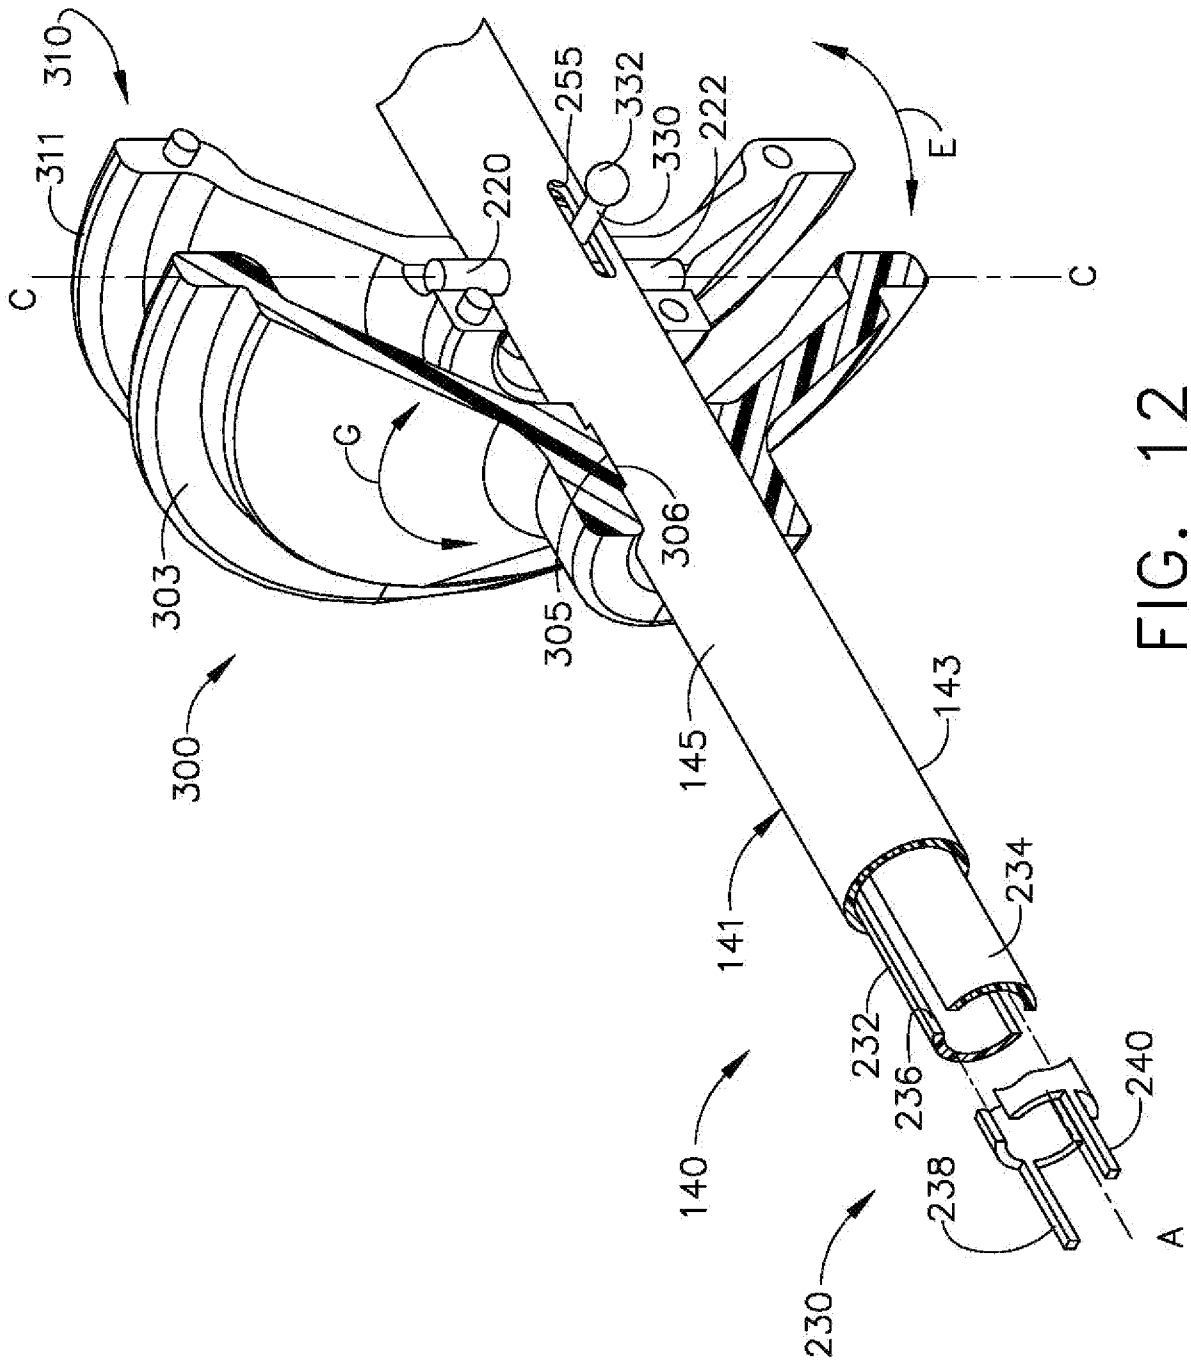


FIG. 12

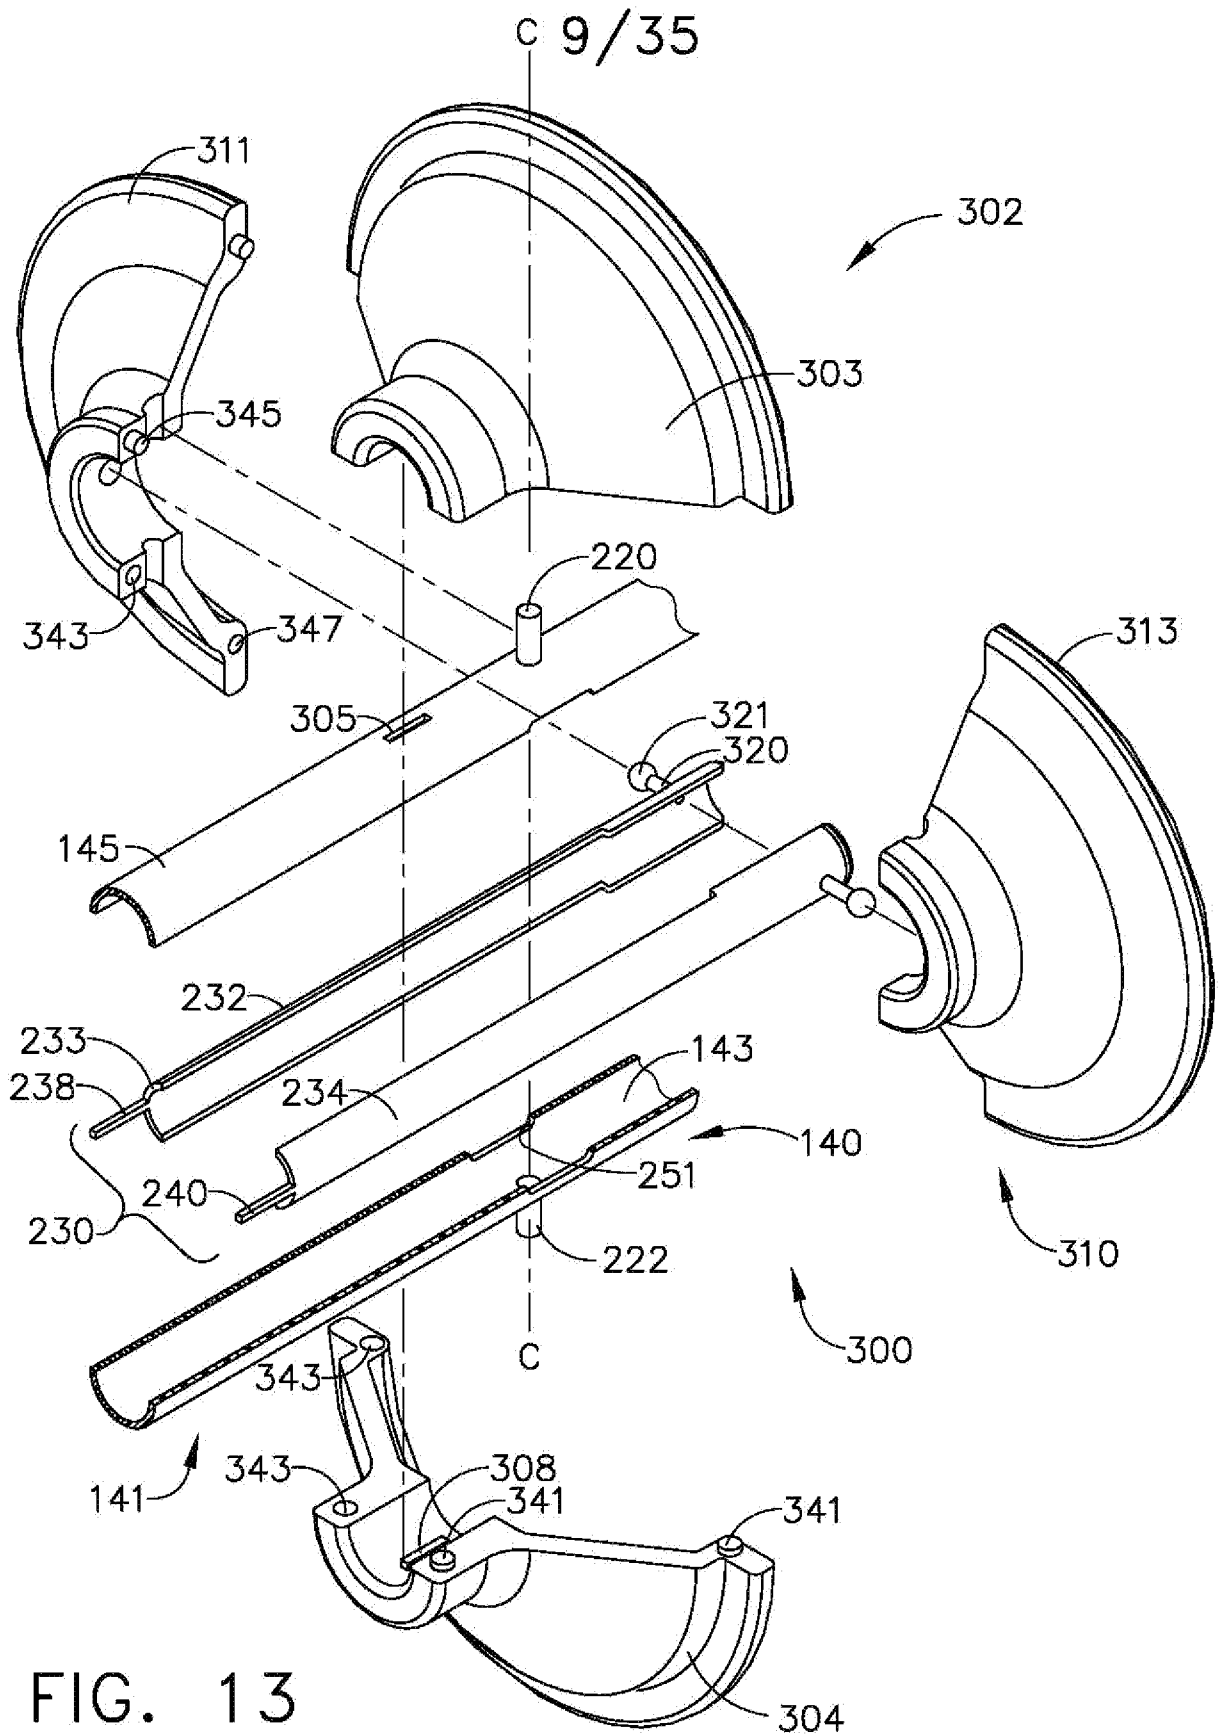


FIG. 13

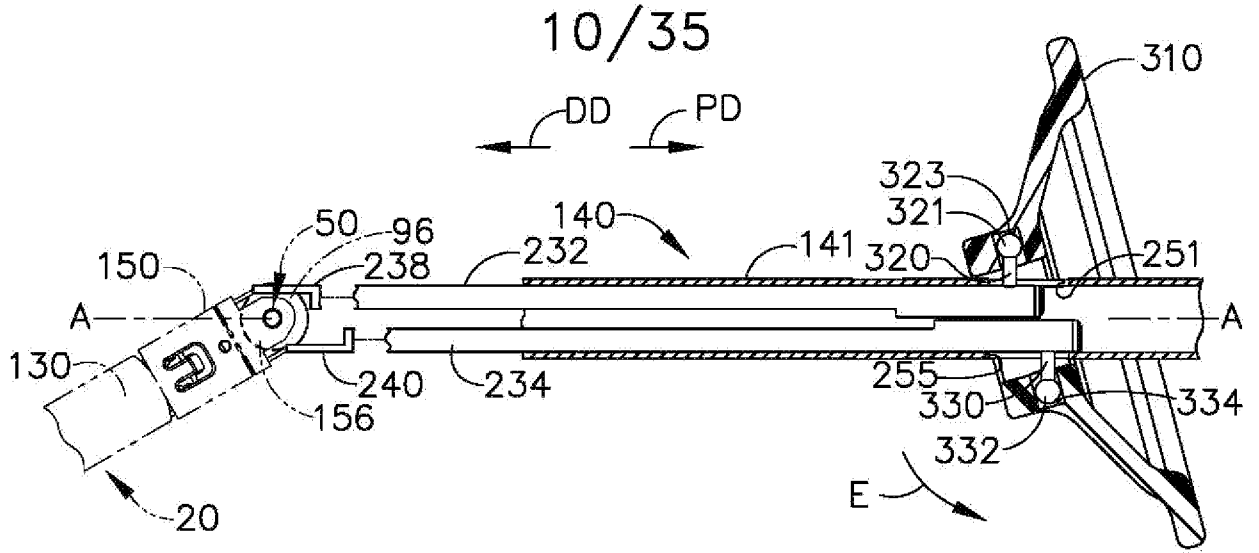


FIG. 14

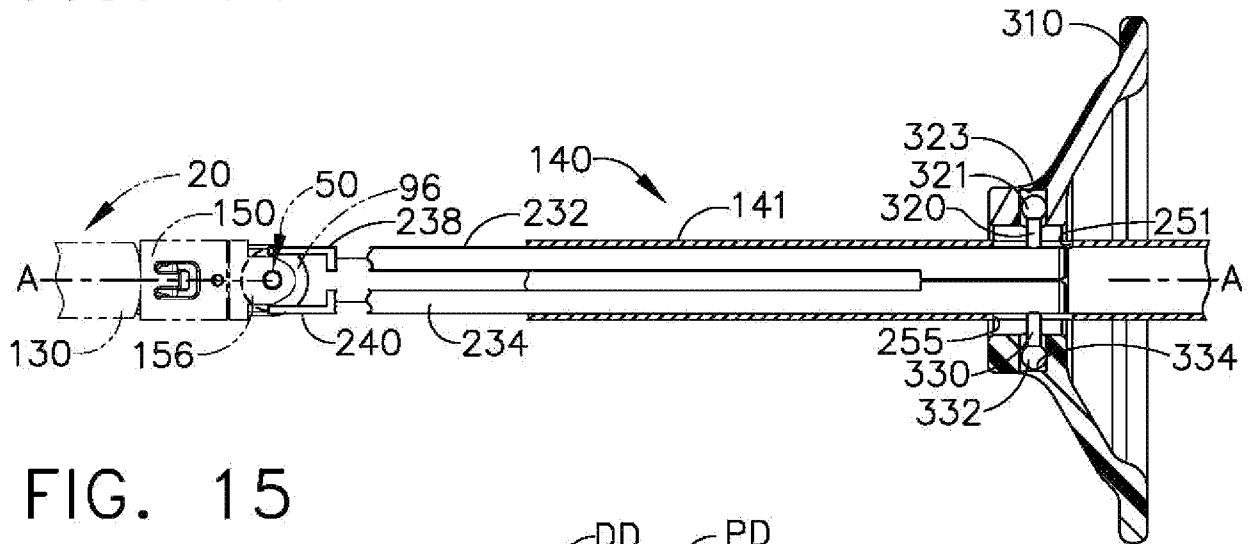


FIG. 15

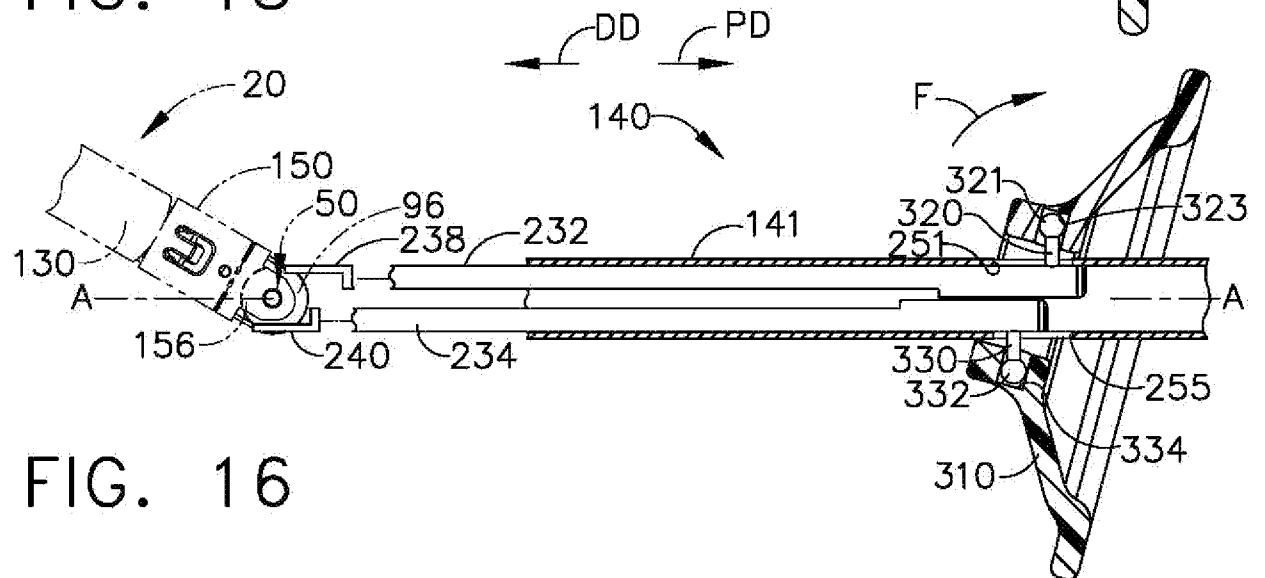


FIG. 16

11/35

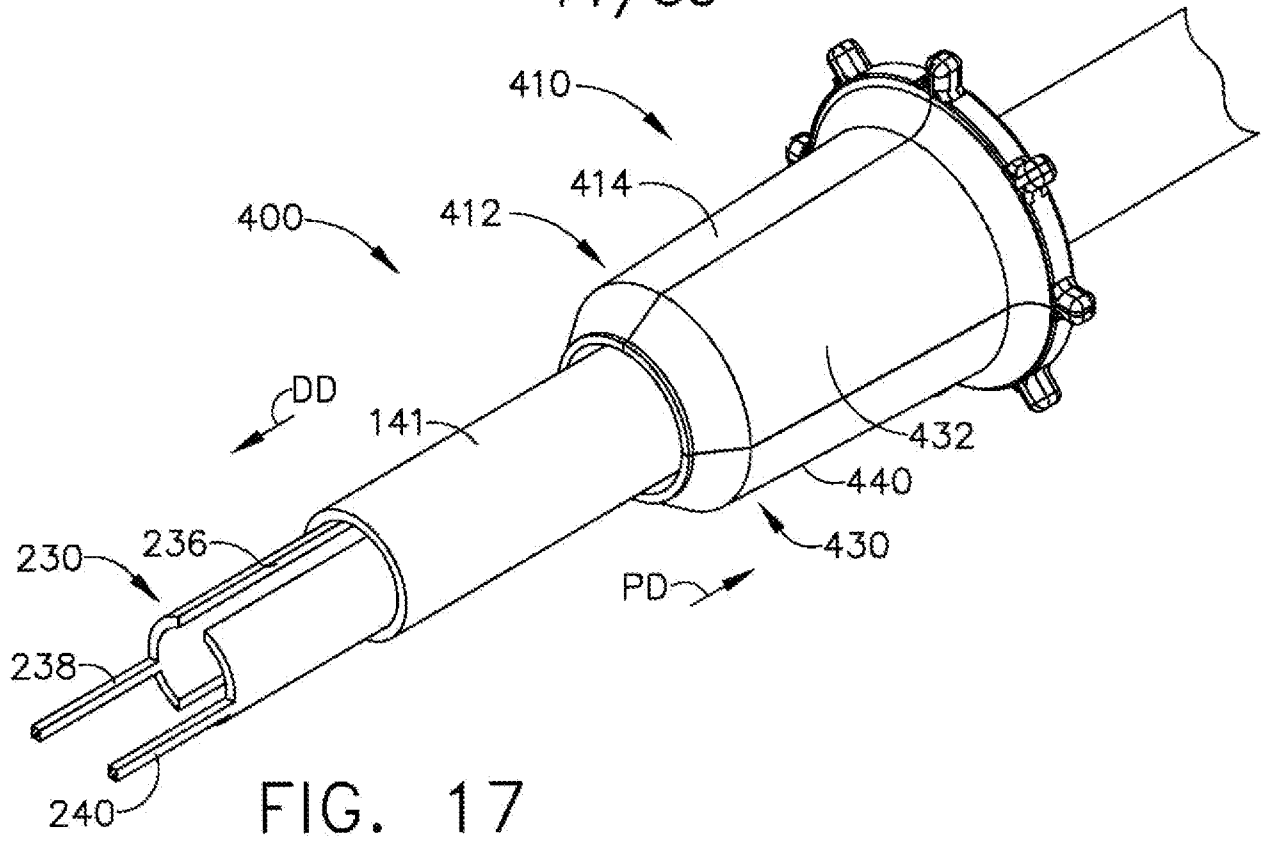


FIG. 17

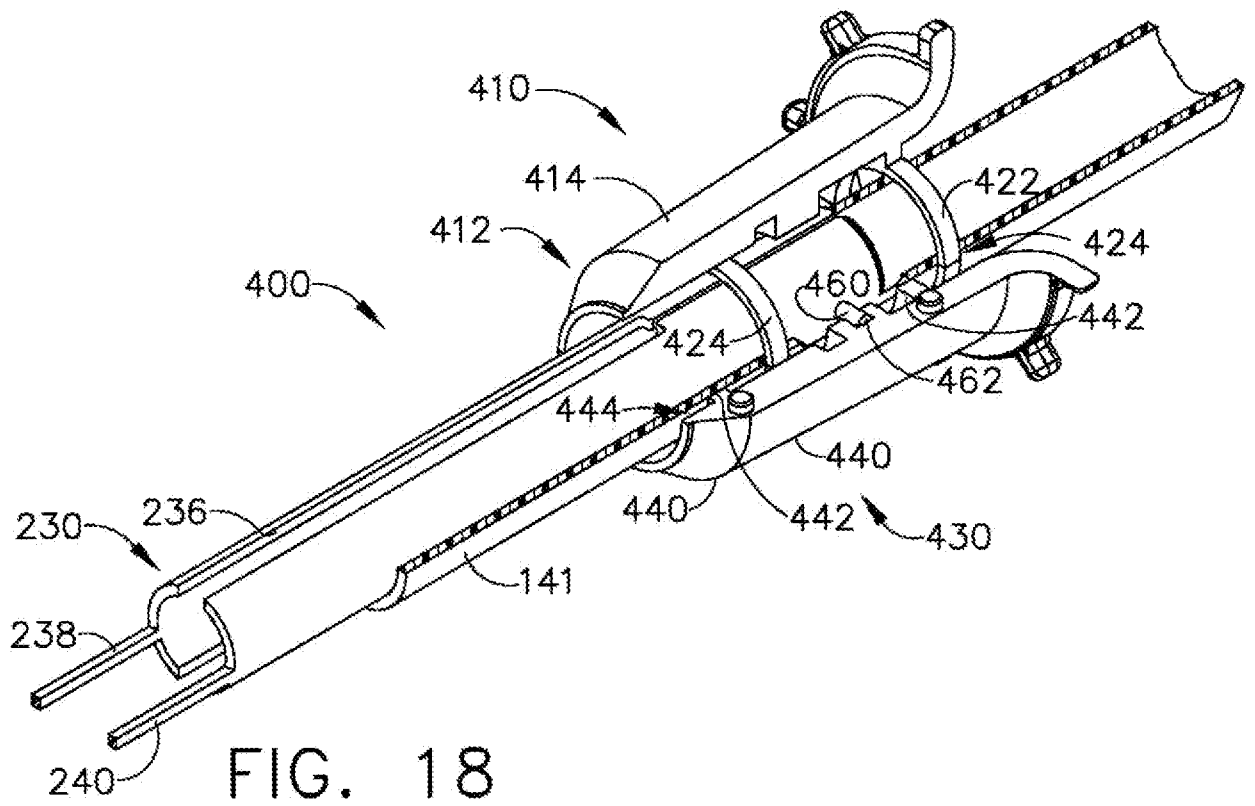


FIG. 18

12/35

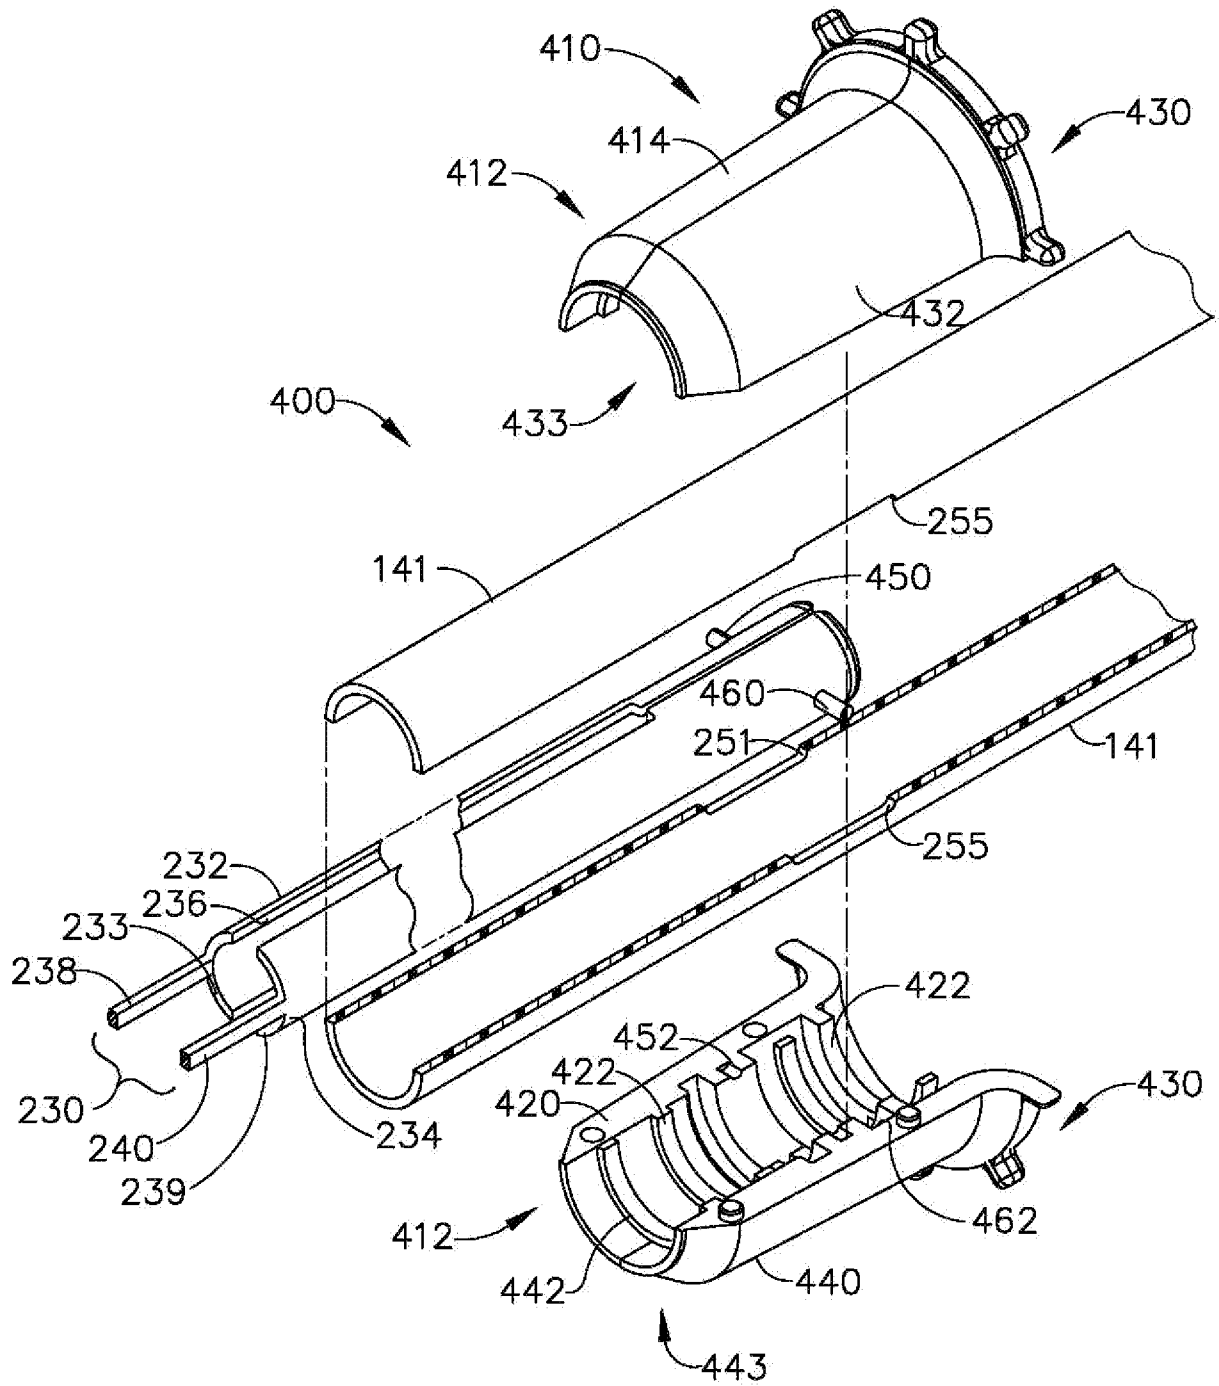


FIG. 19

13/35

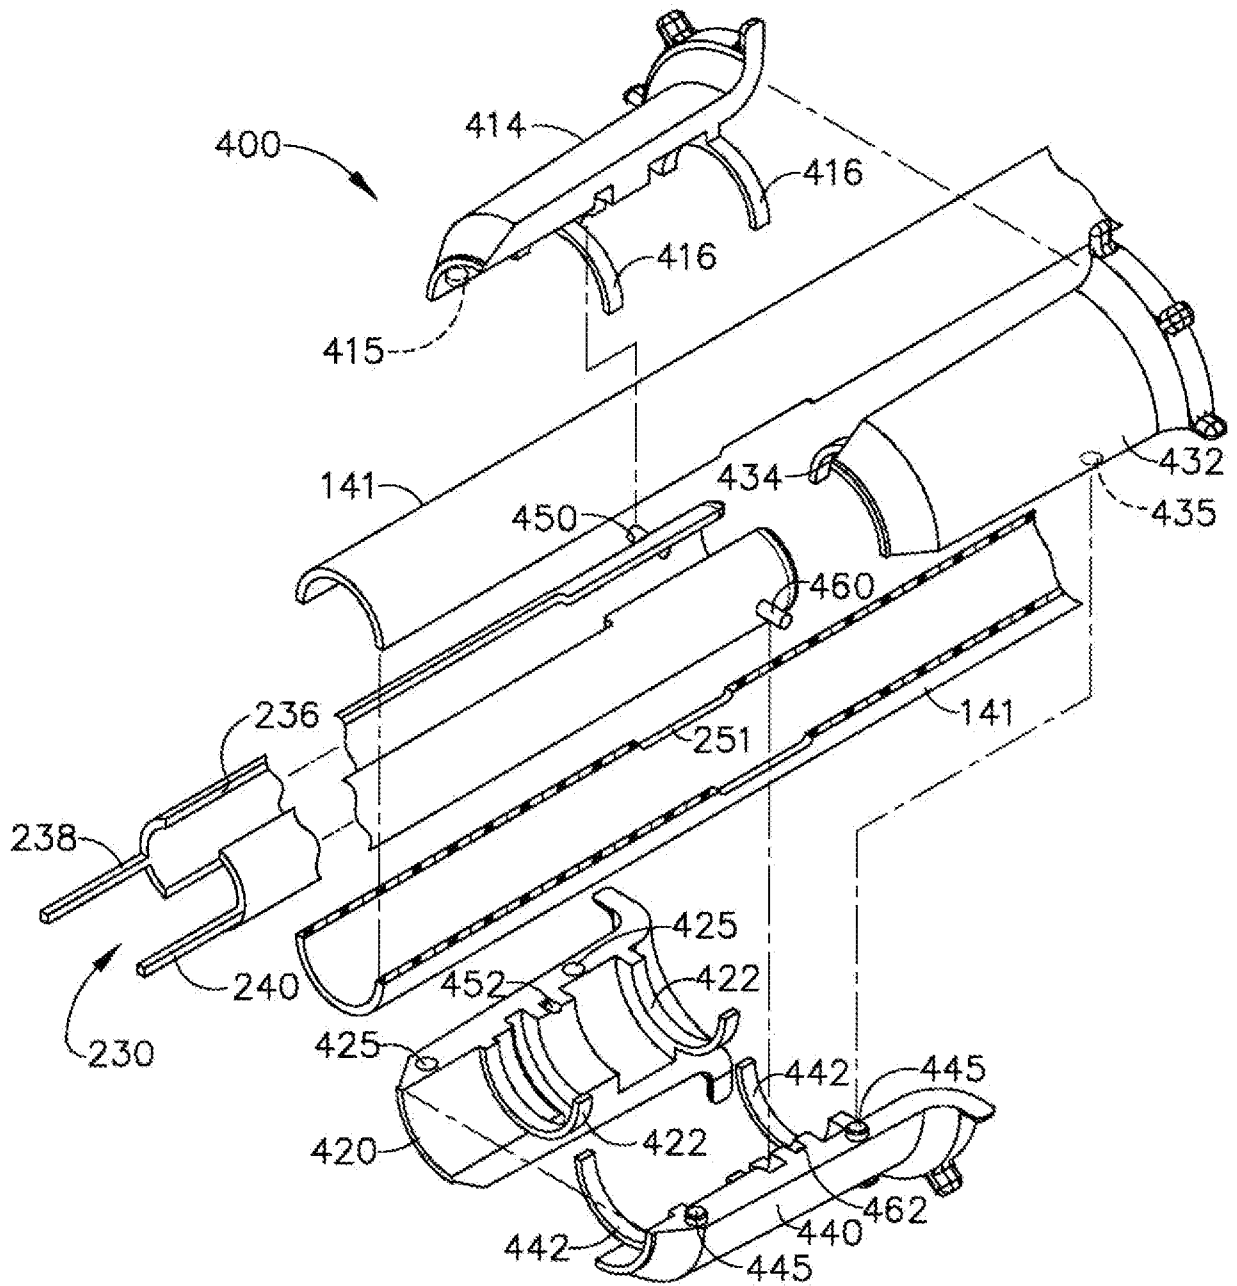


FIG. 20

14/35

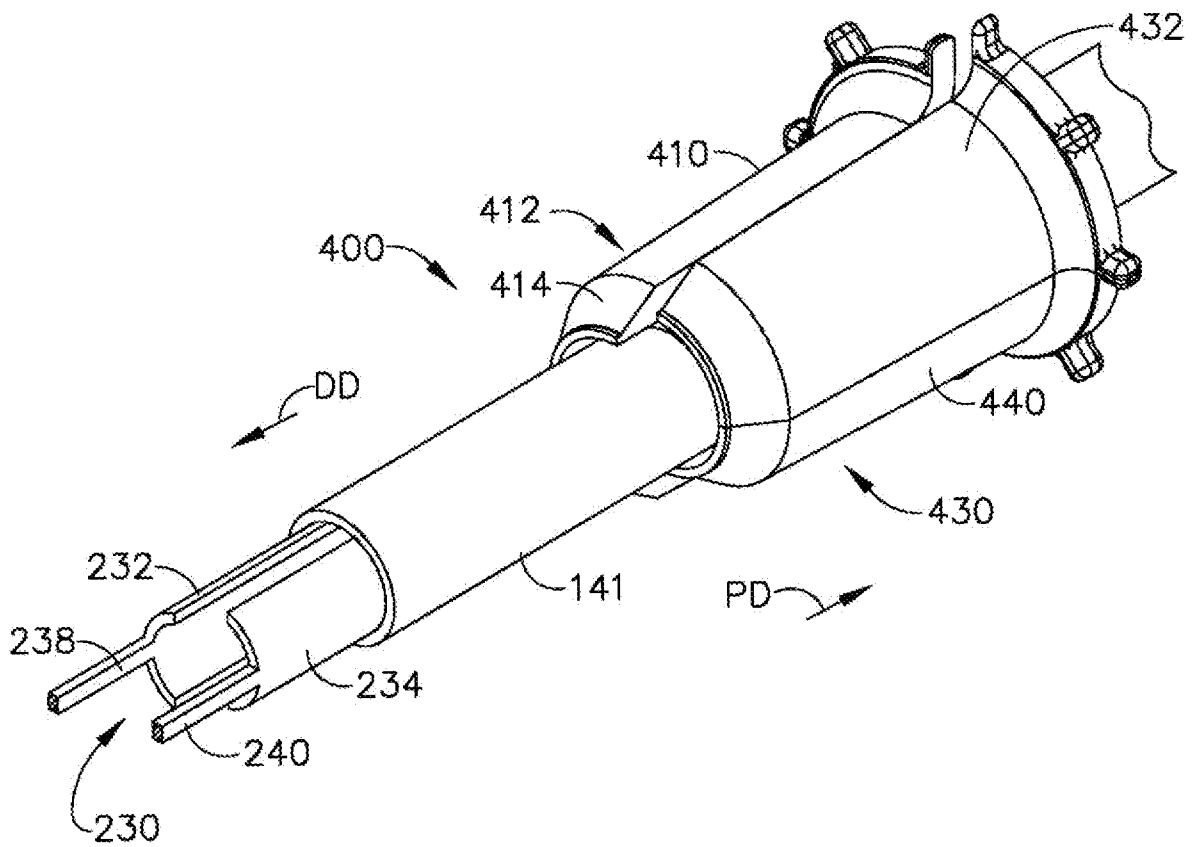


FIG. 21

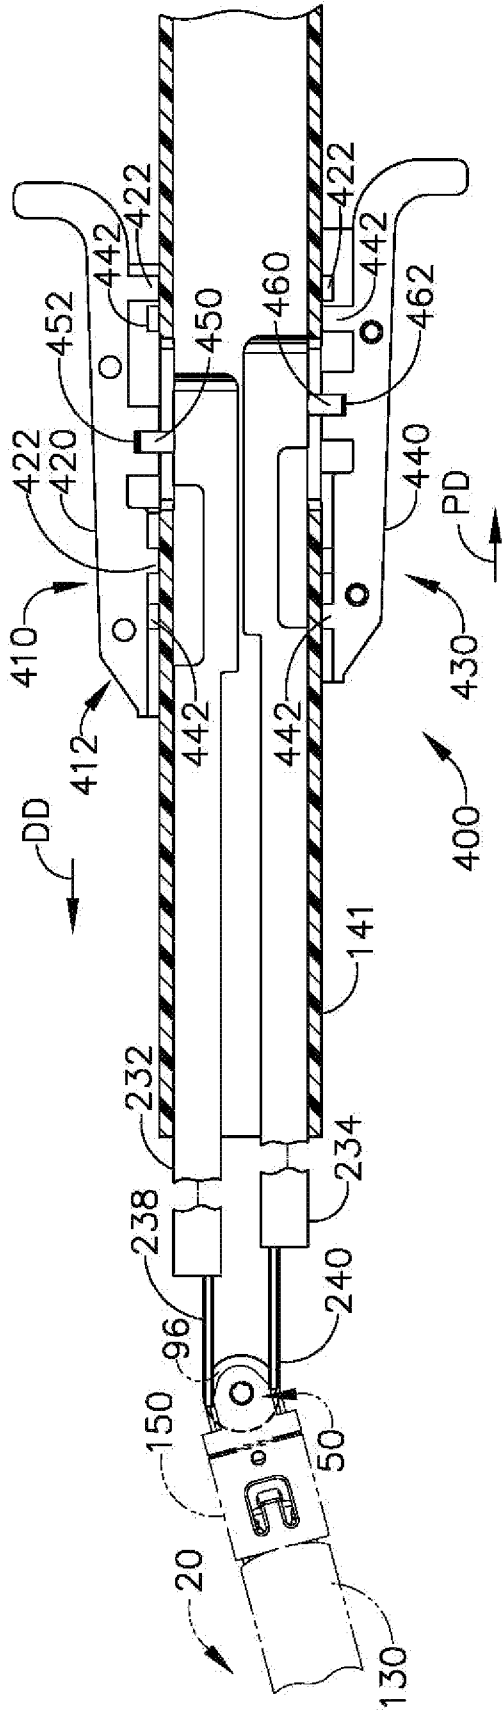


FIG. 22

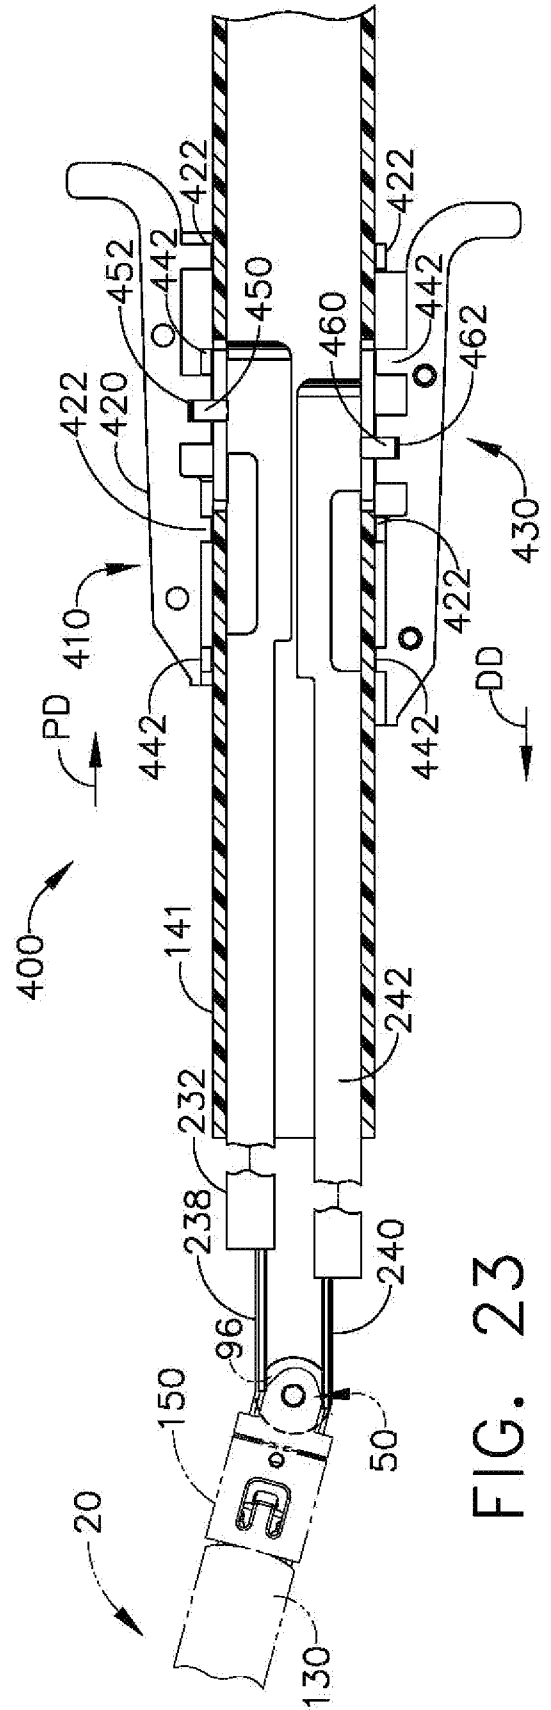


FIG. 23



16/35

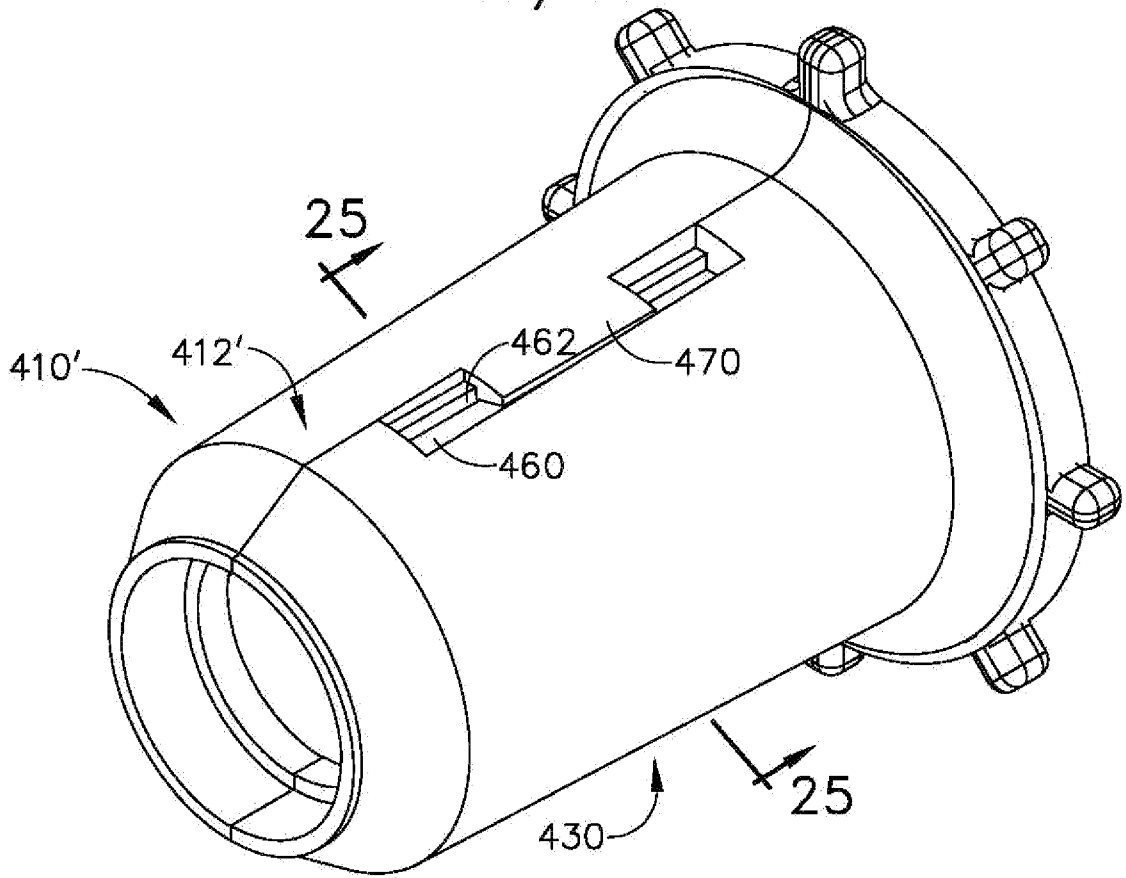


FIG. 24

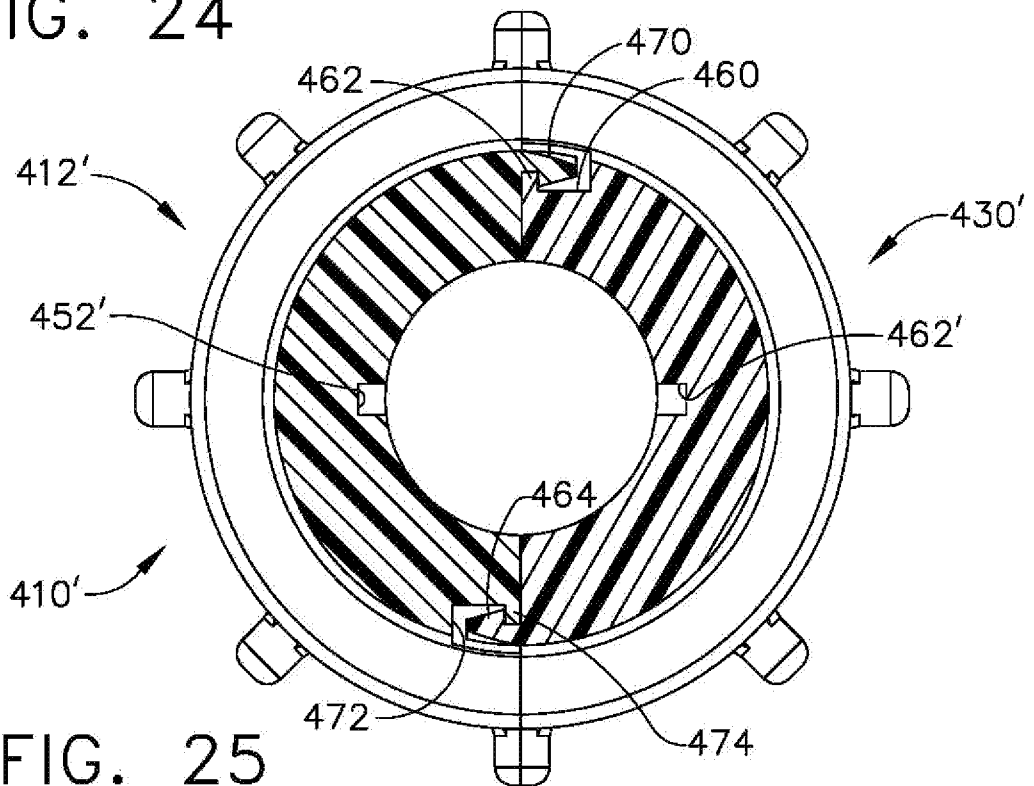


FIG. 25


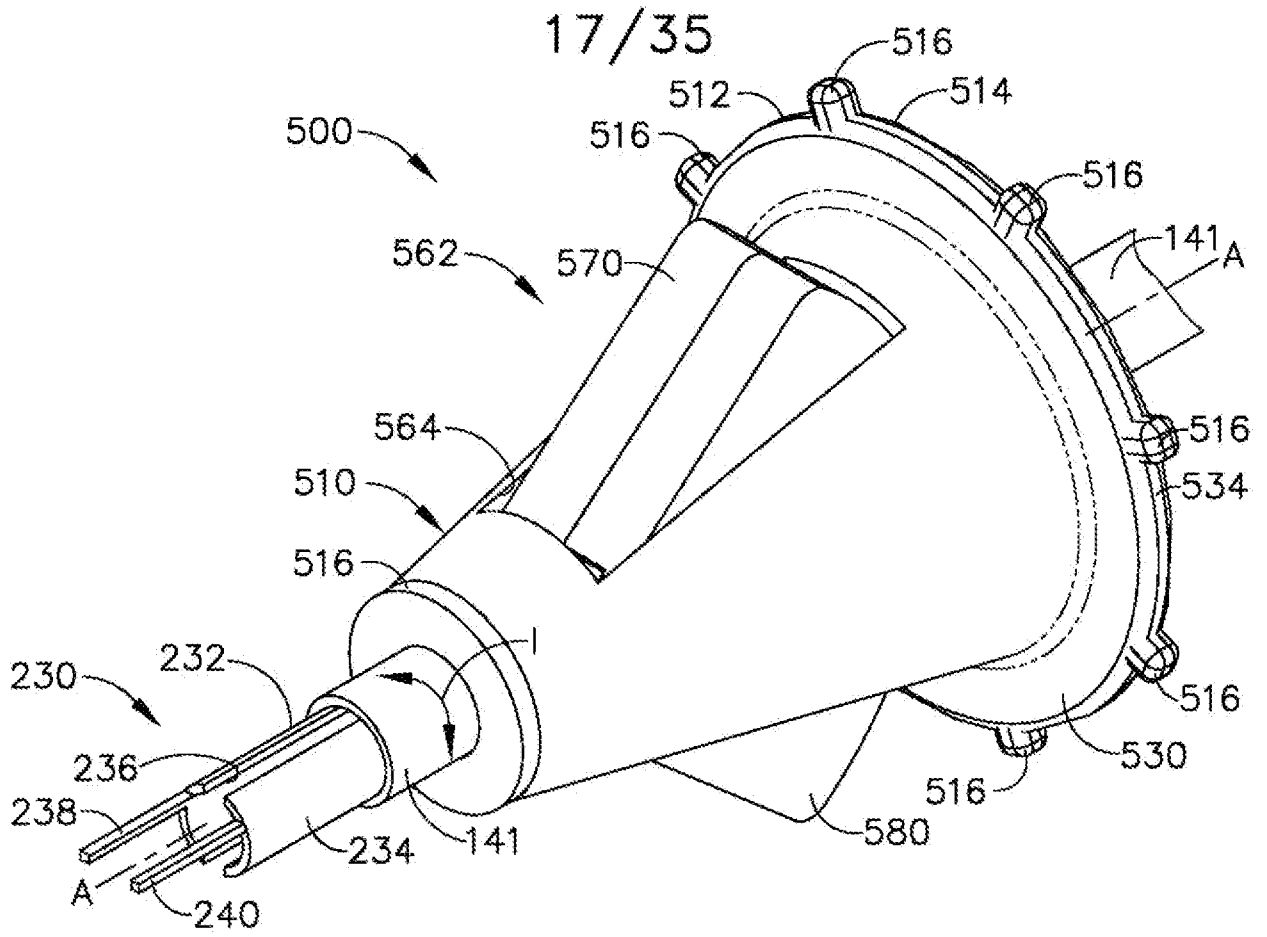


FIG. 26

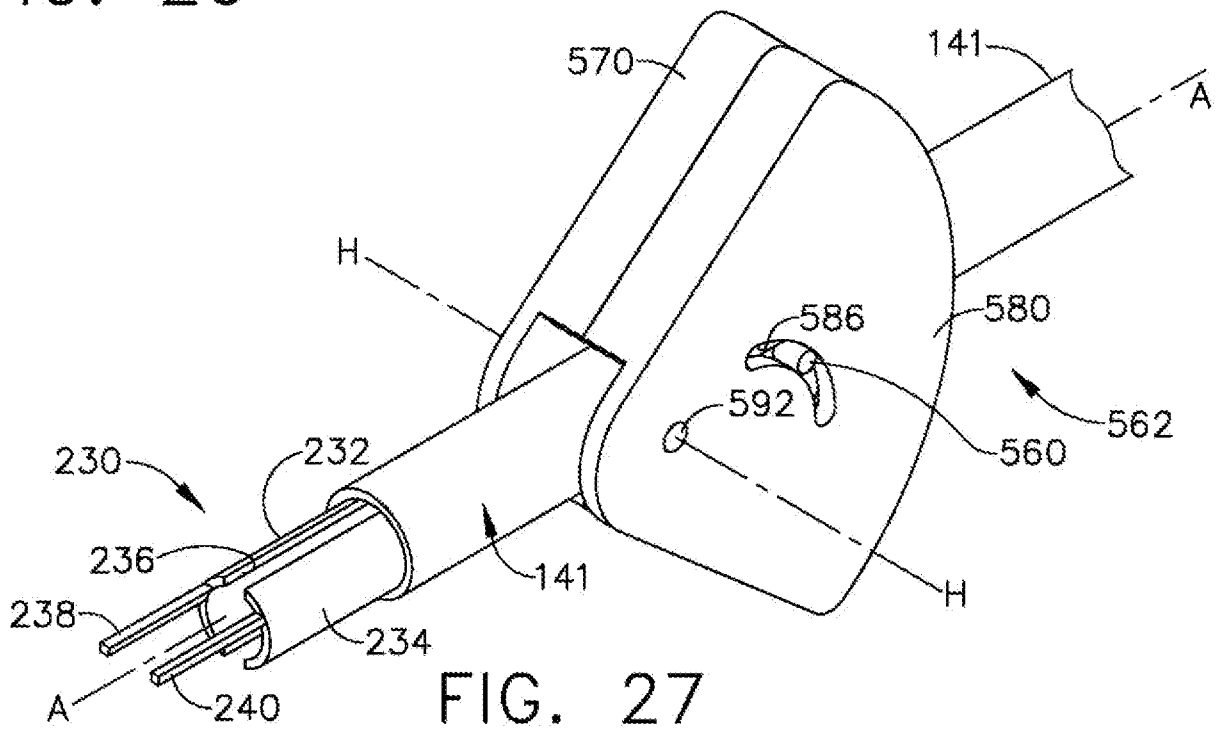

18/35


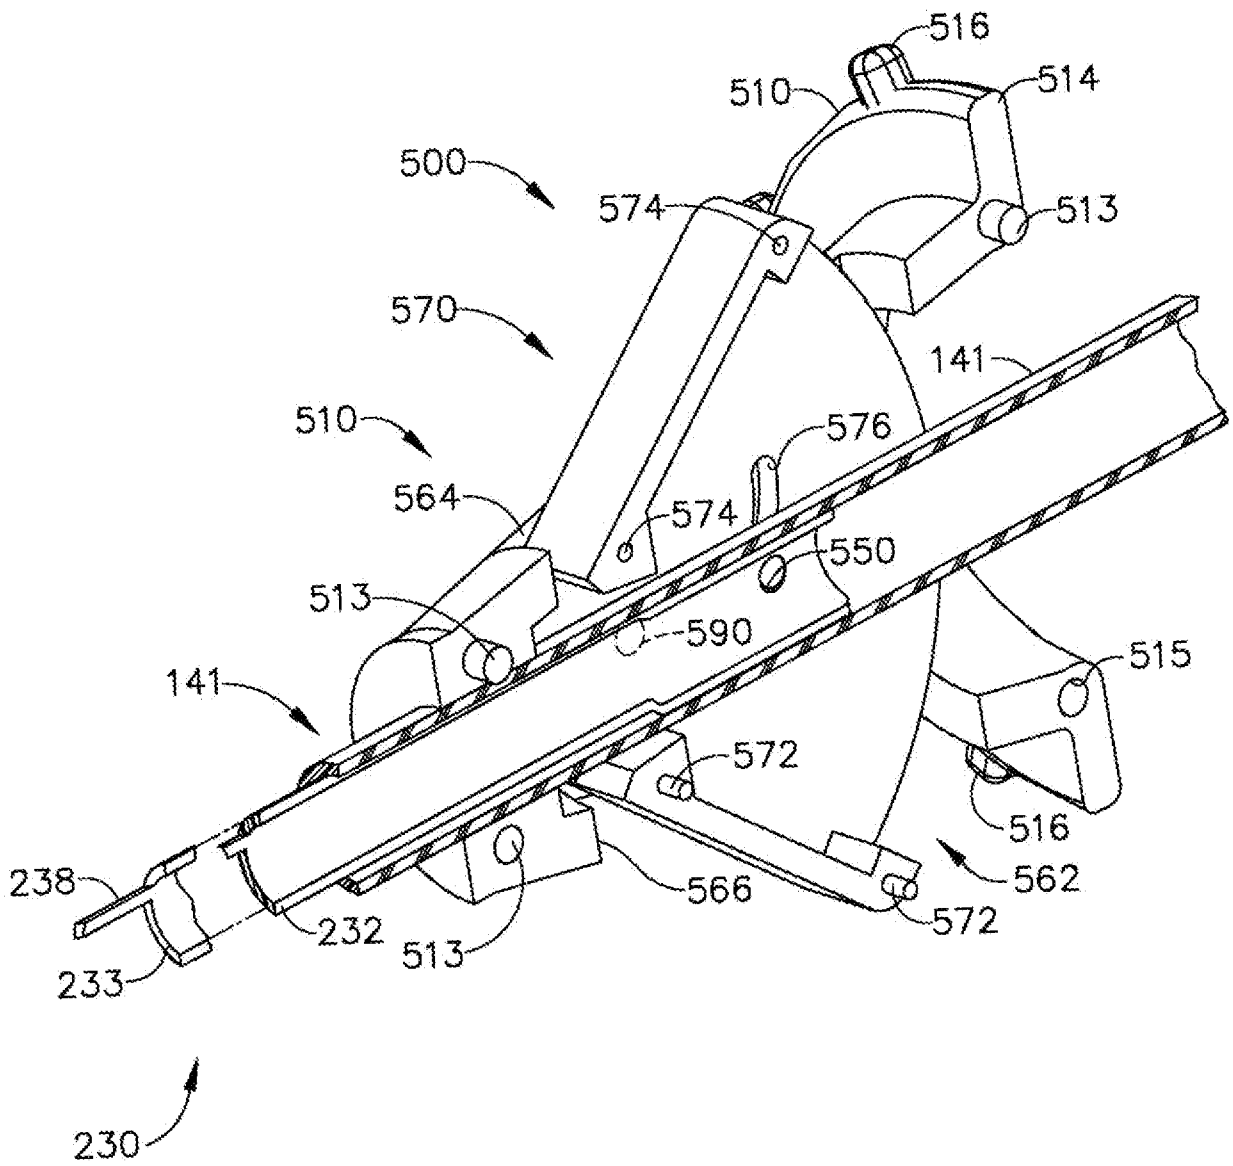


FIG. 28

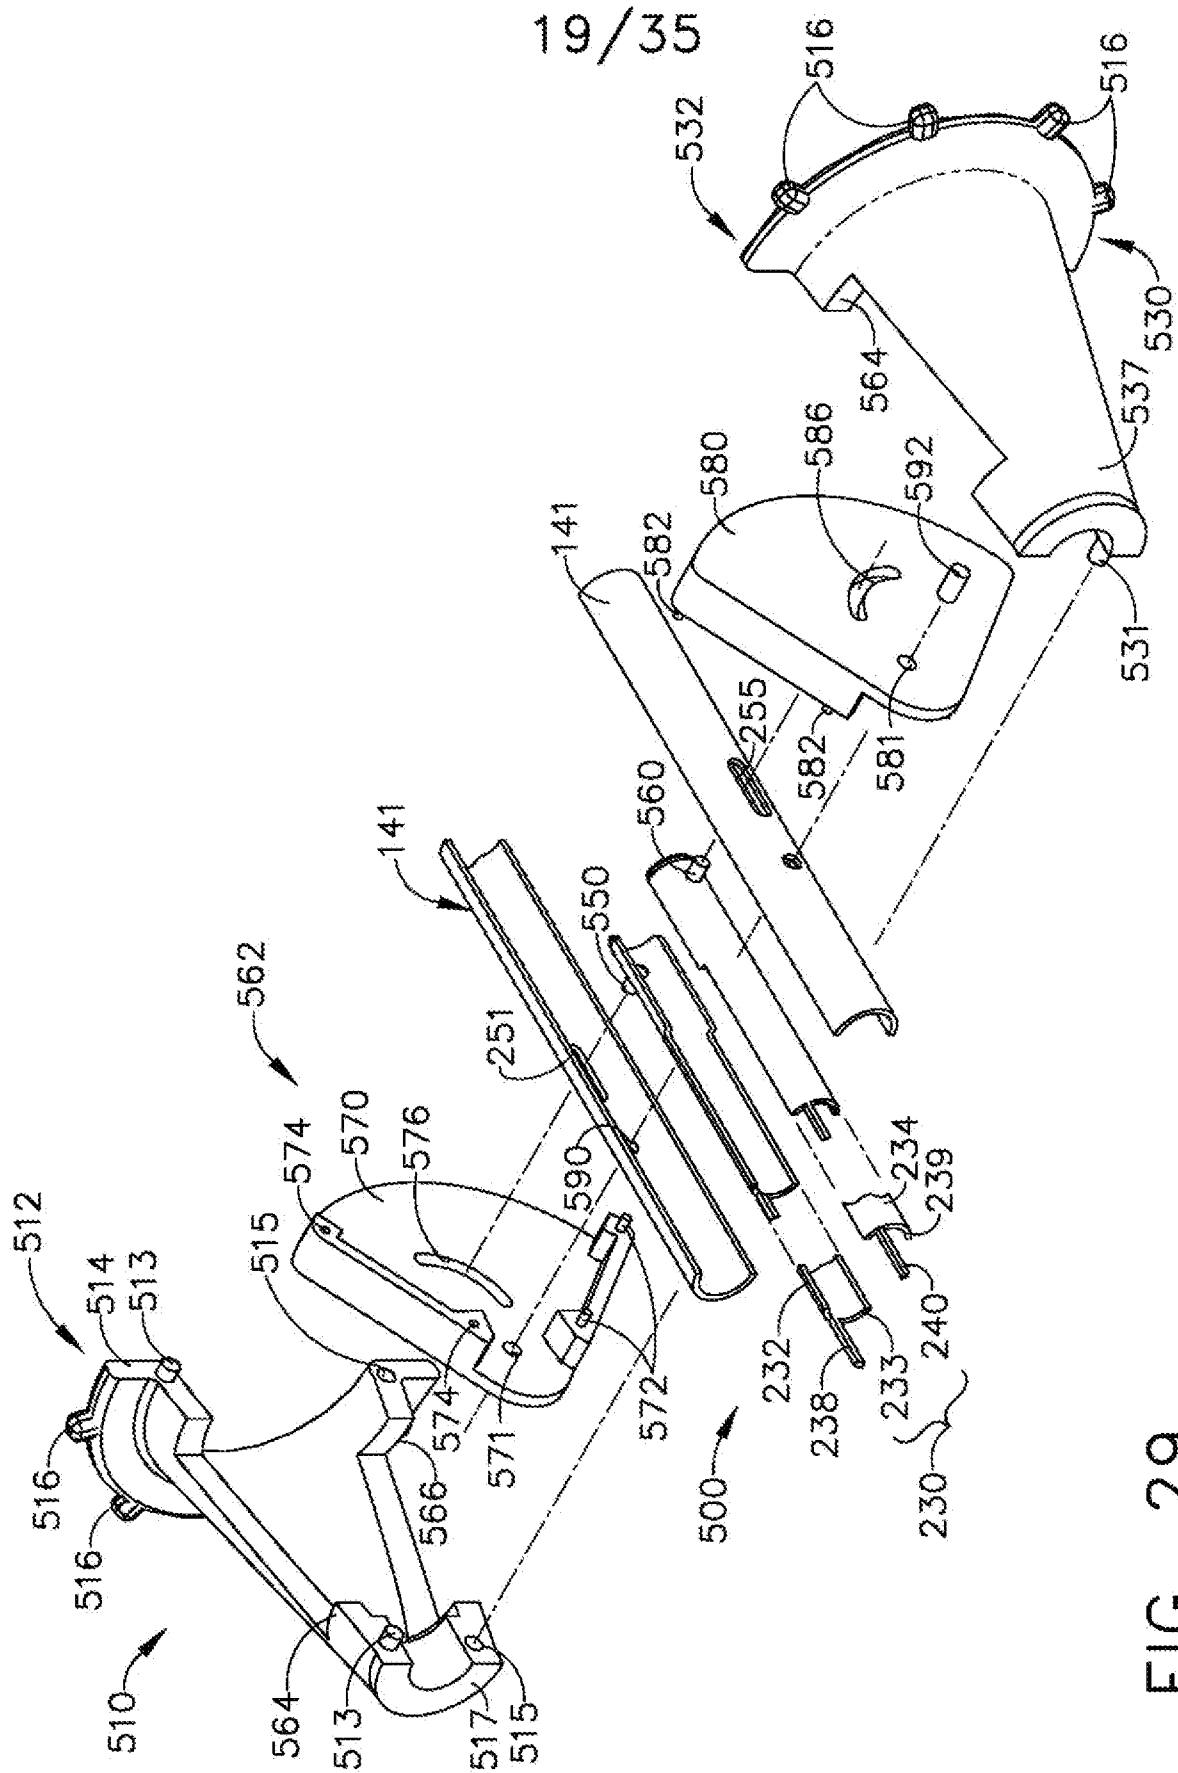

20/35

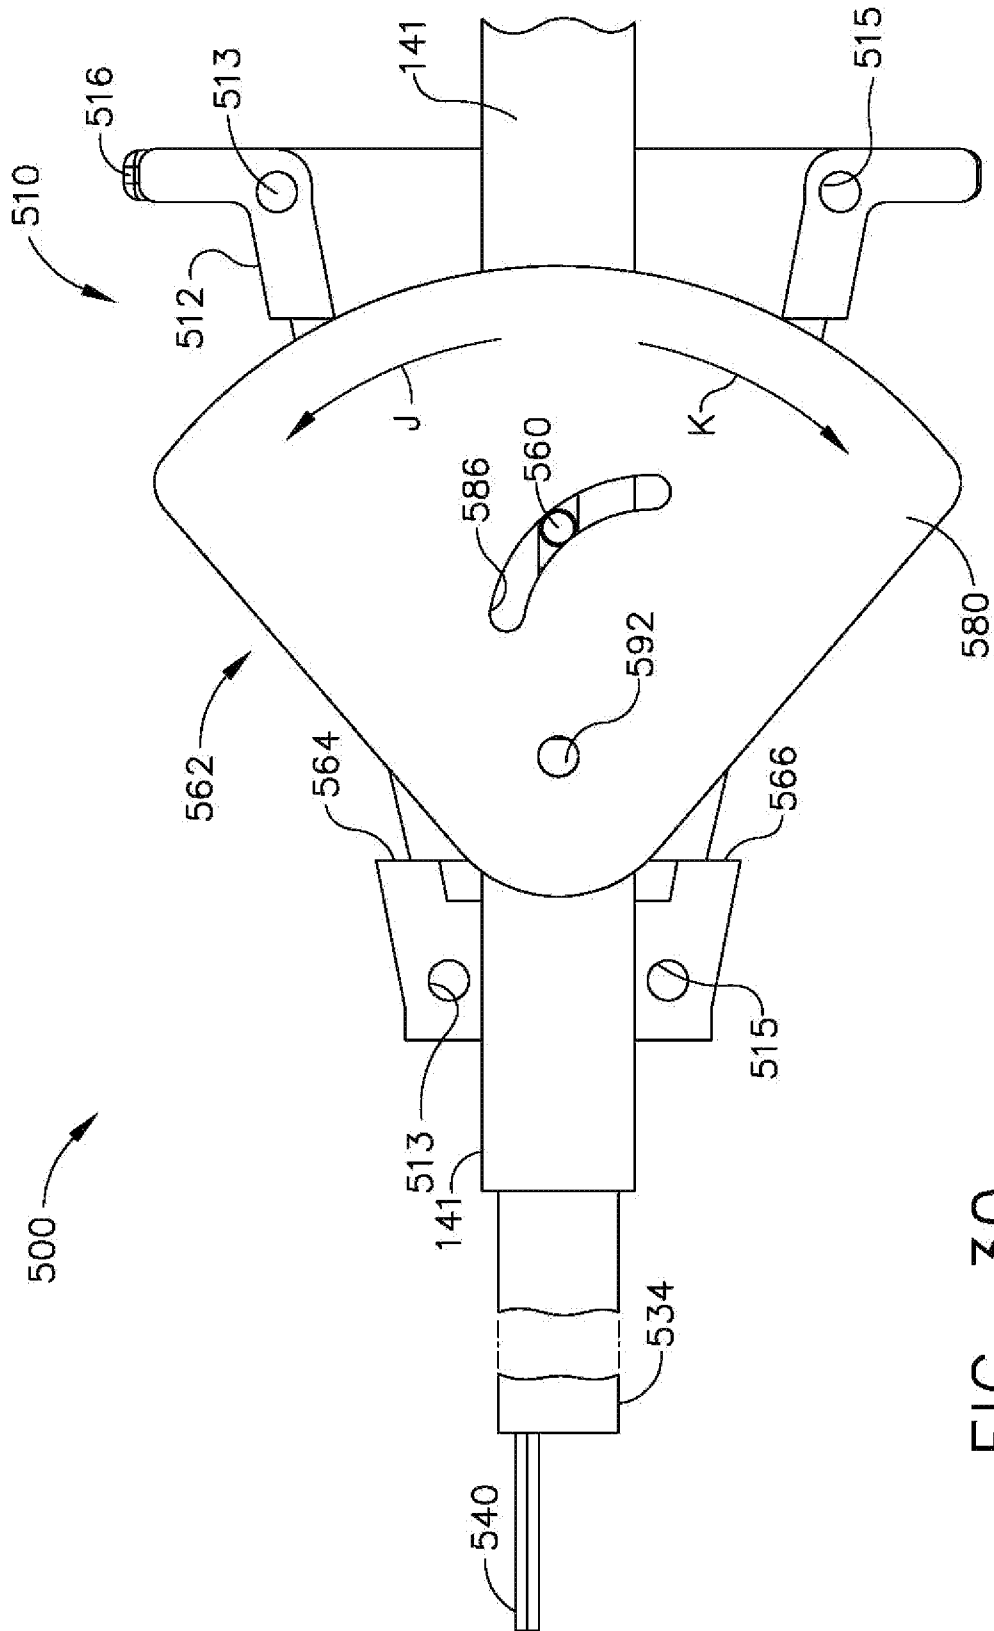


FIG. 30

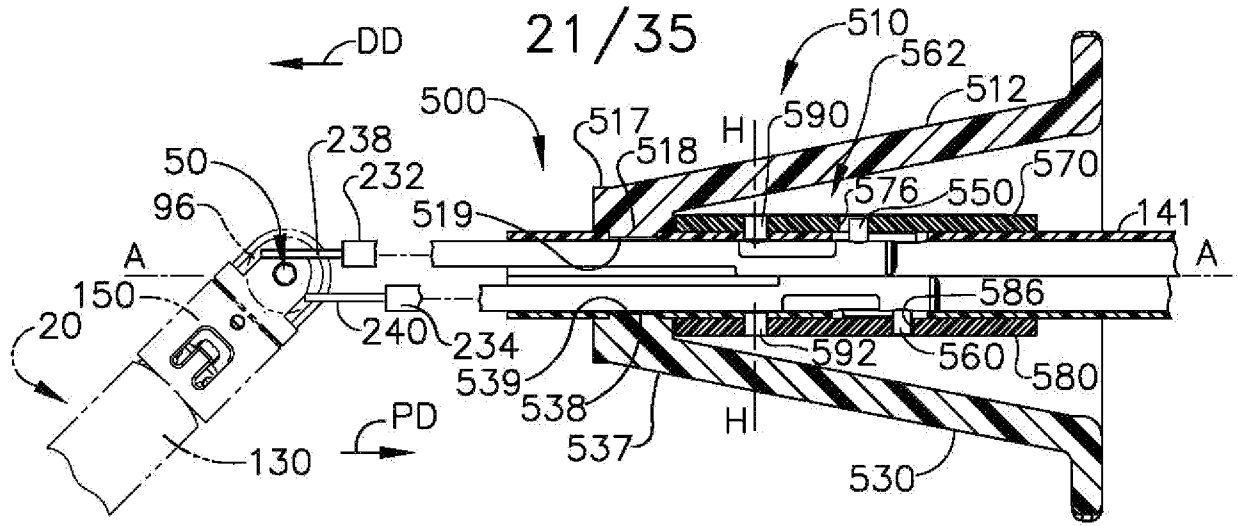


FIG. 31

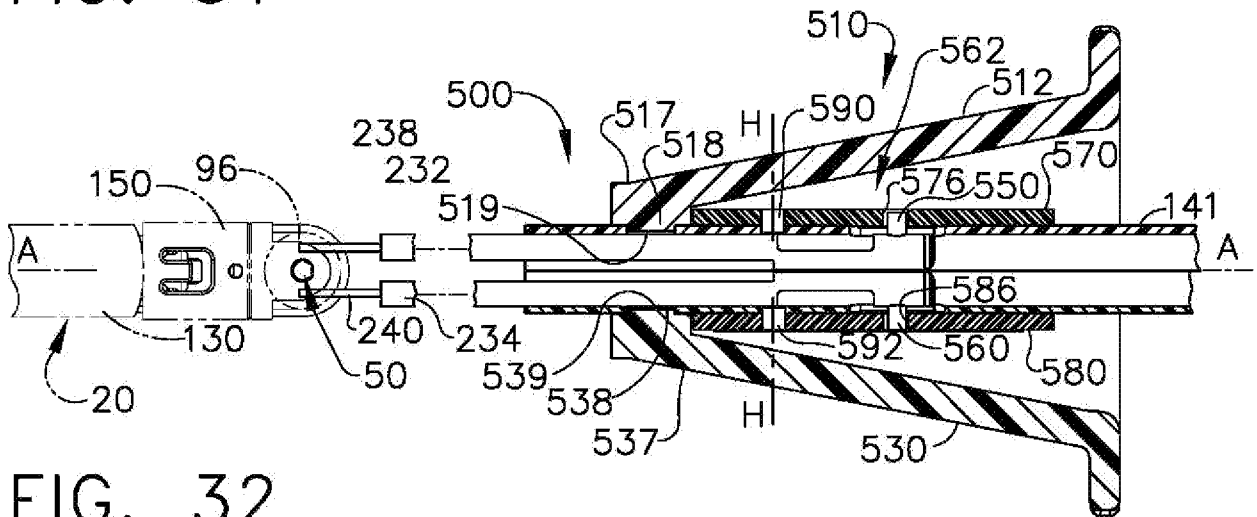


FIG. 32

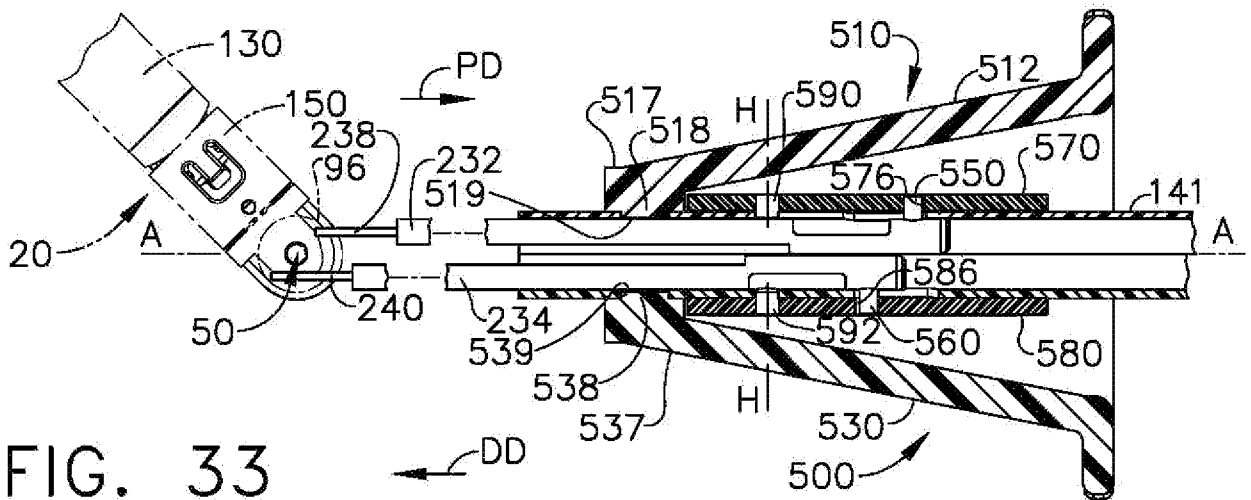


FIG. 33

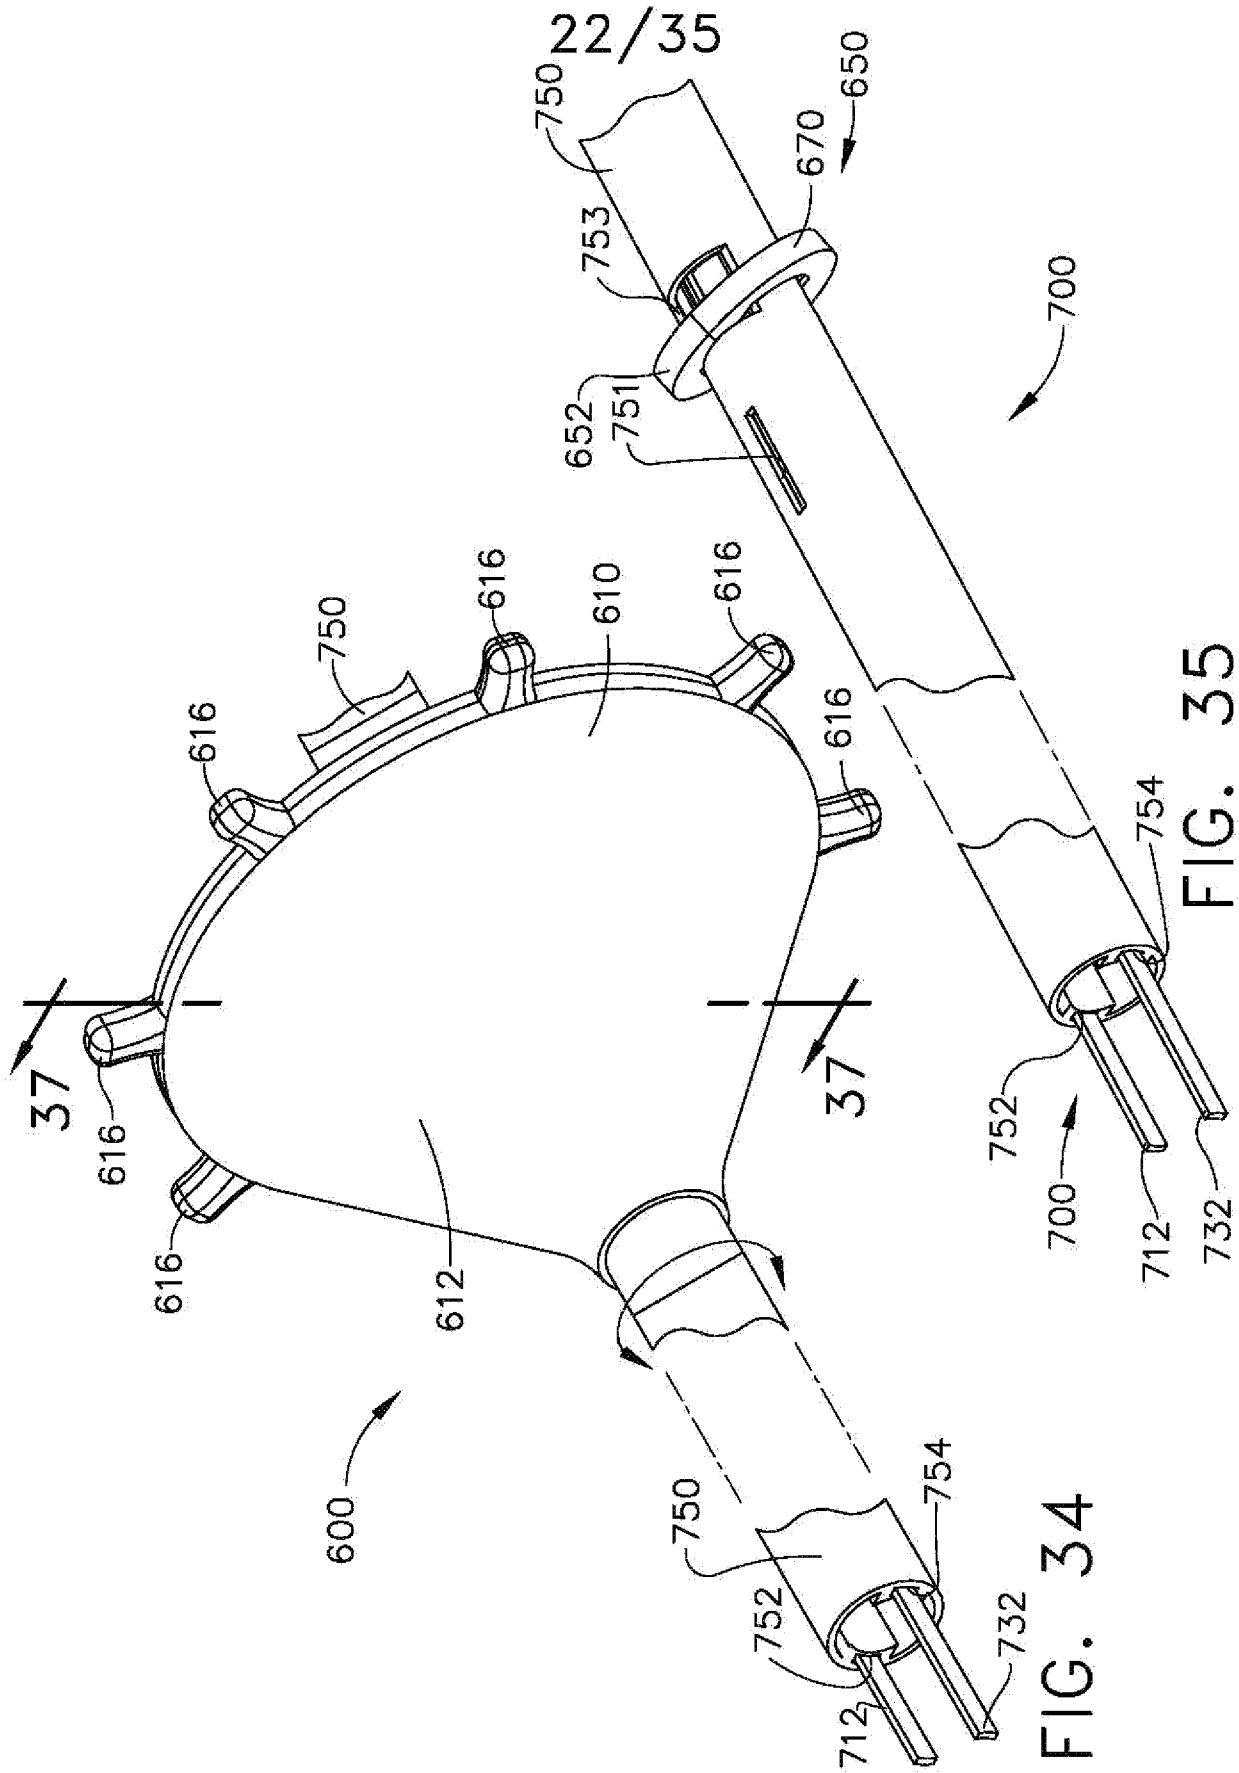


FIG. 34

FIG. 35

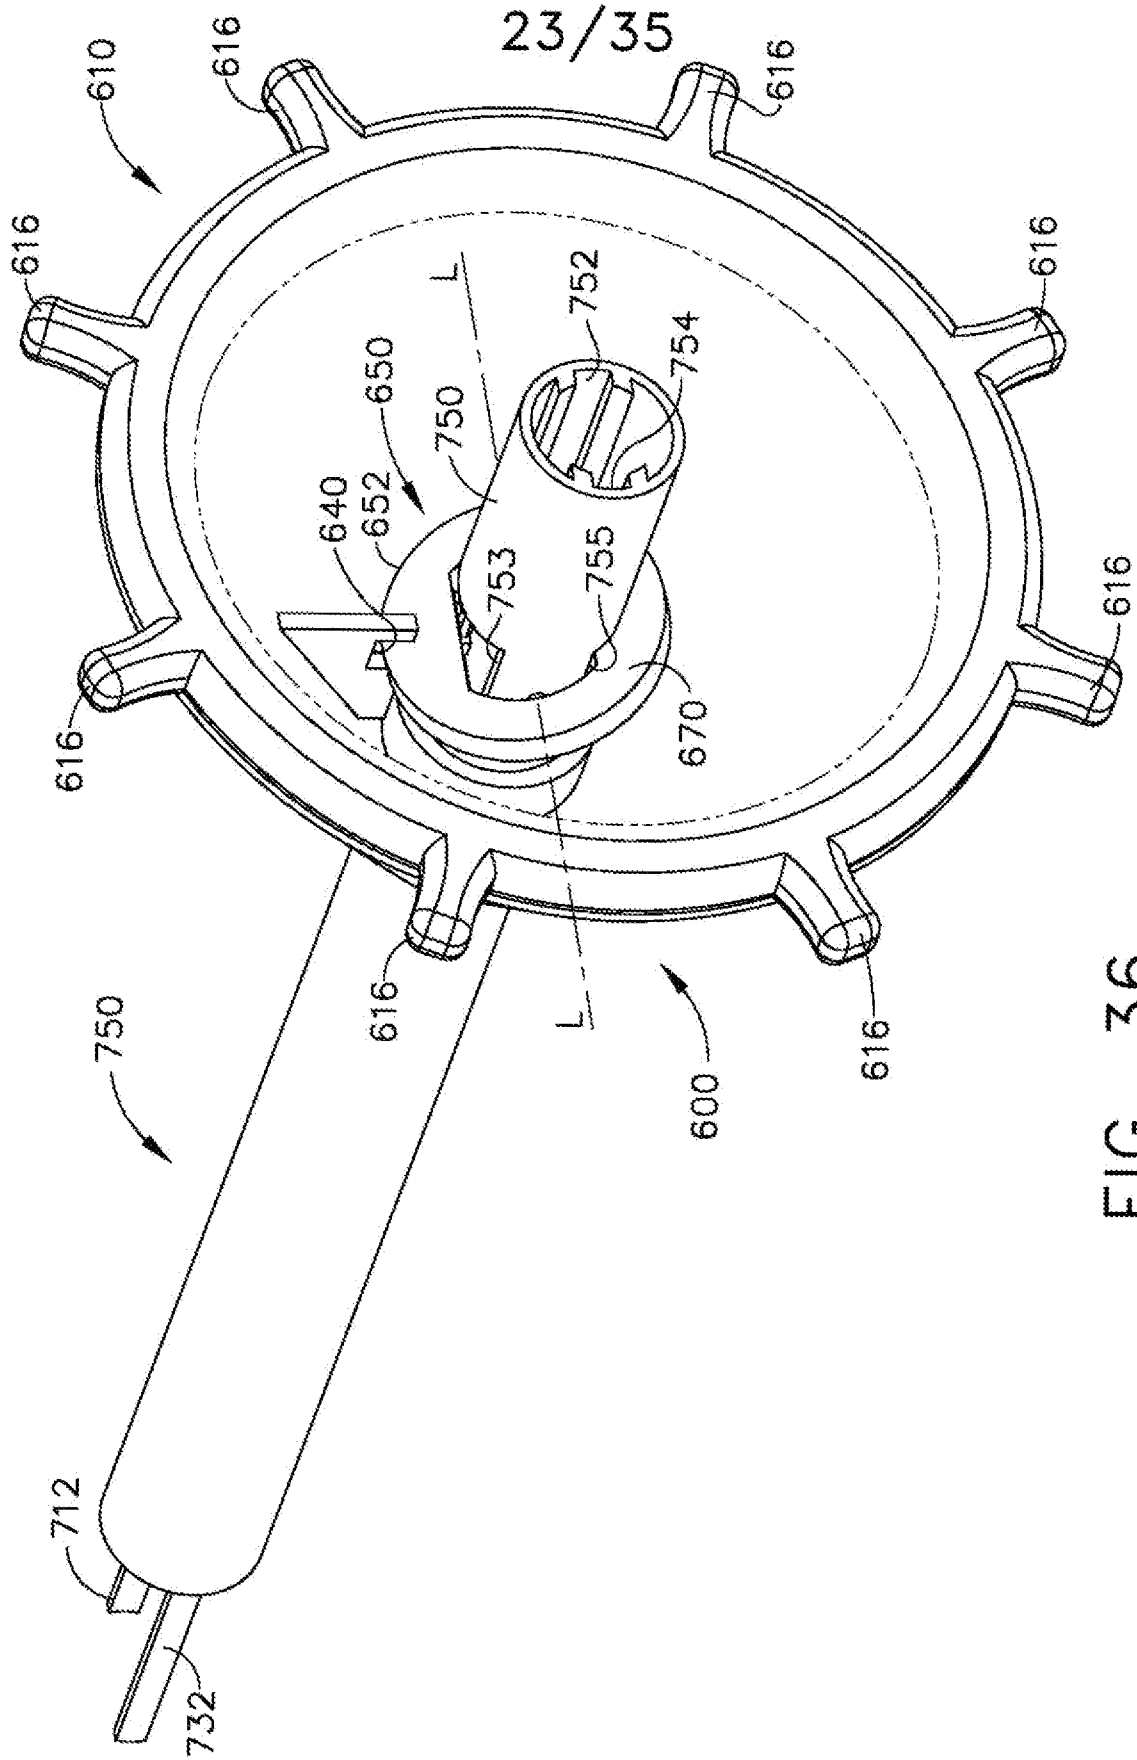


FIG. 36



24/35

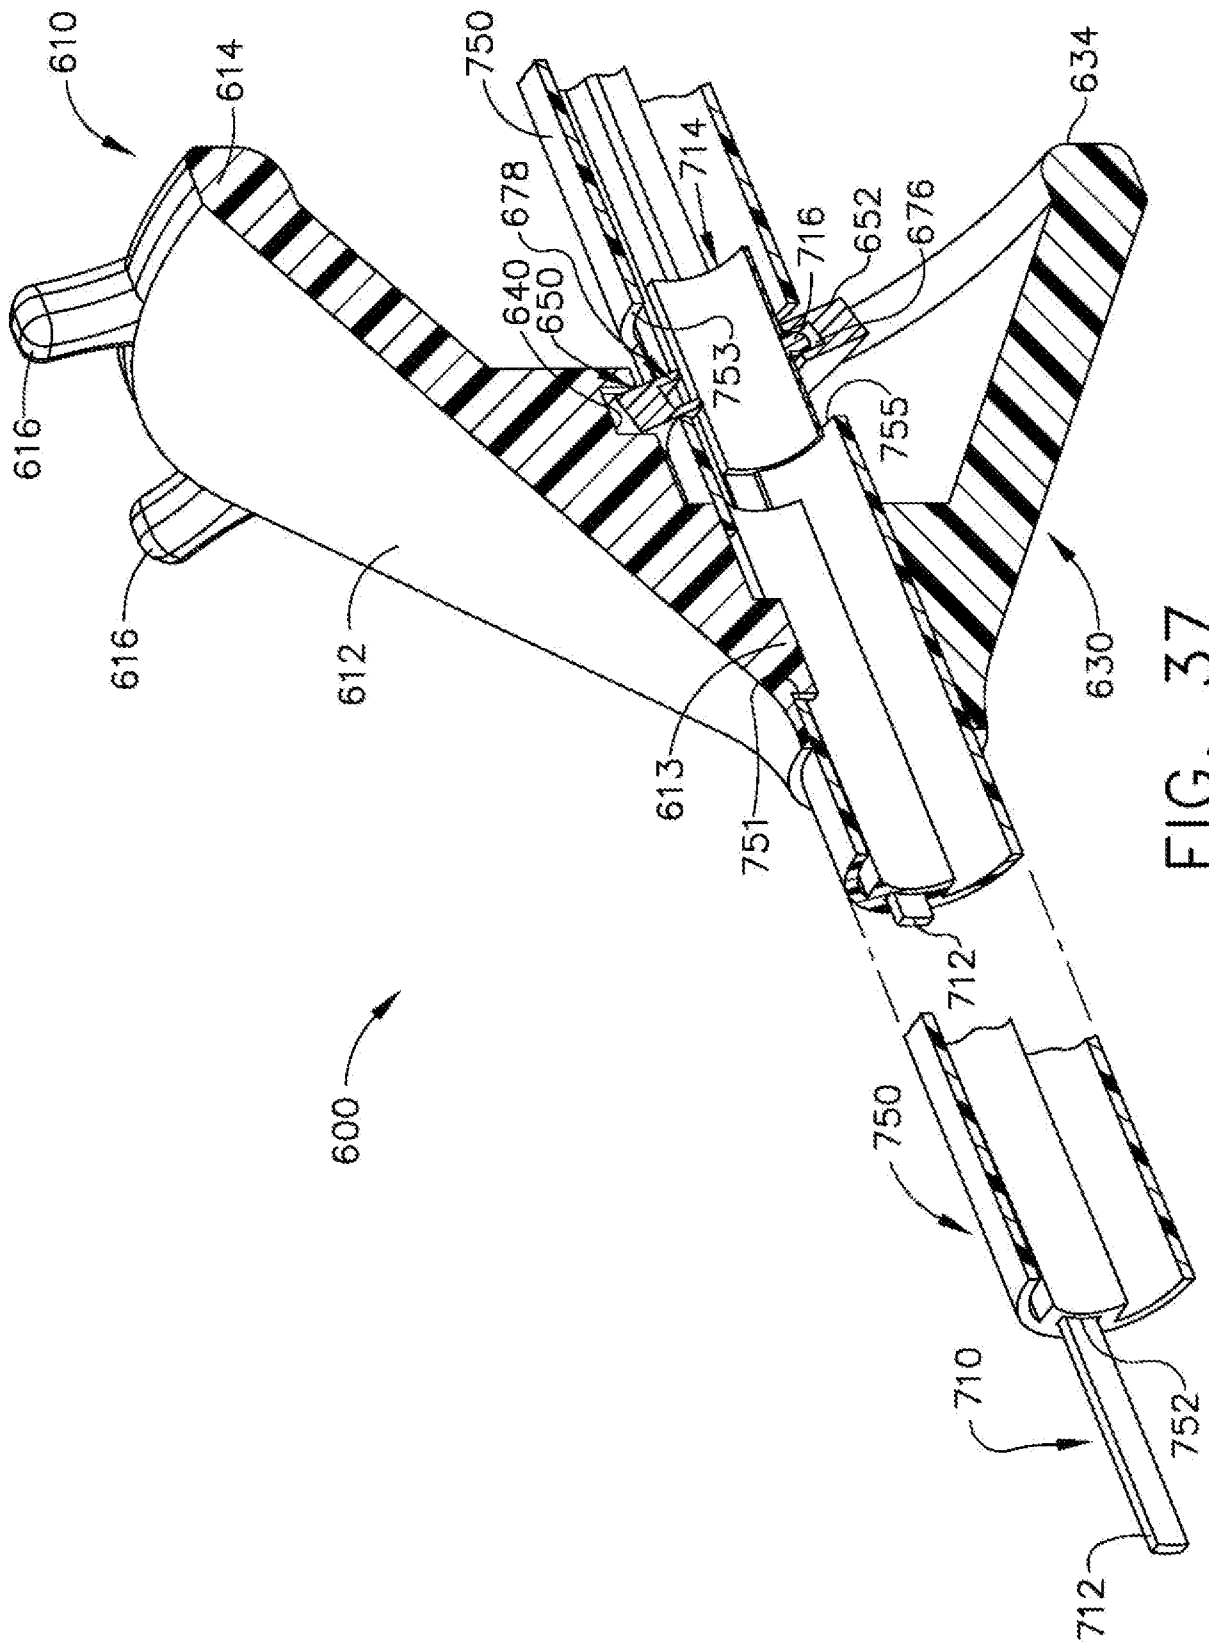


FIG. 37

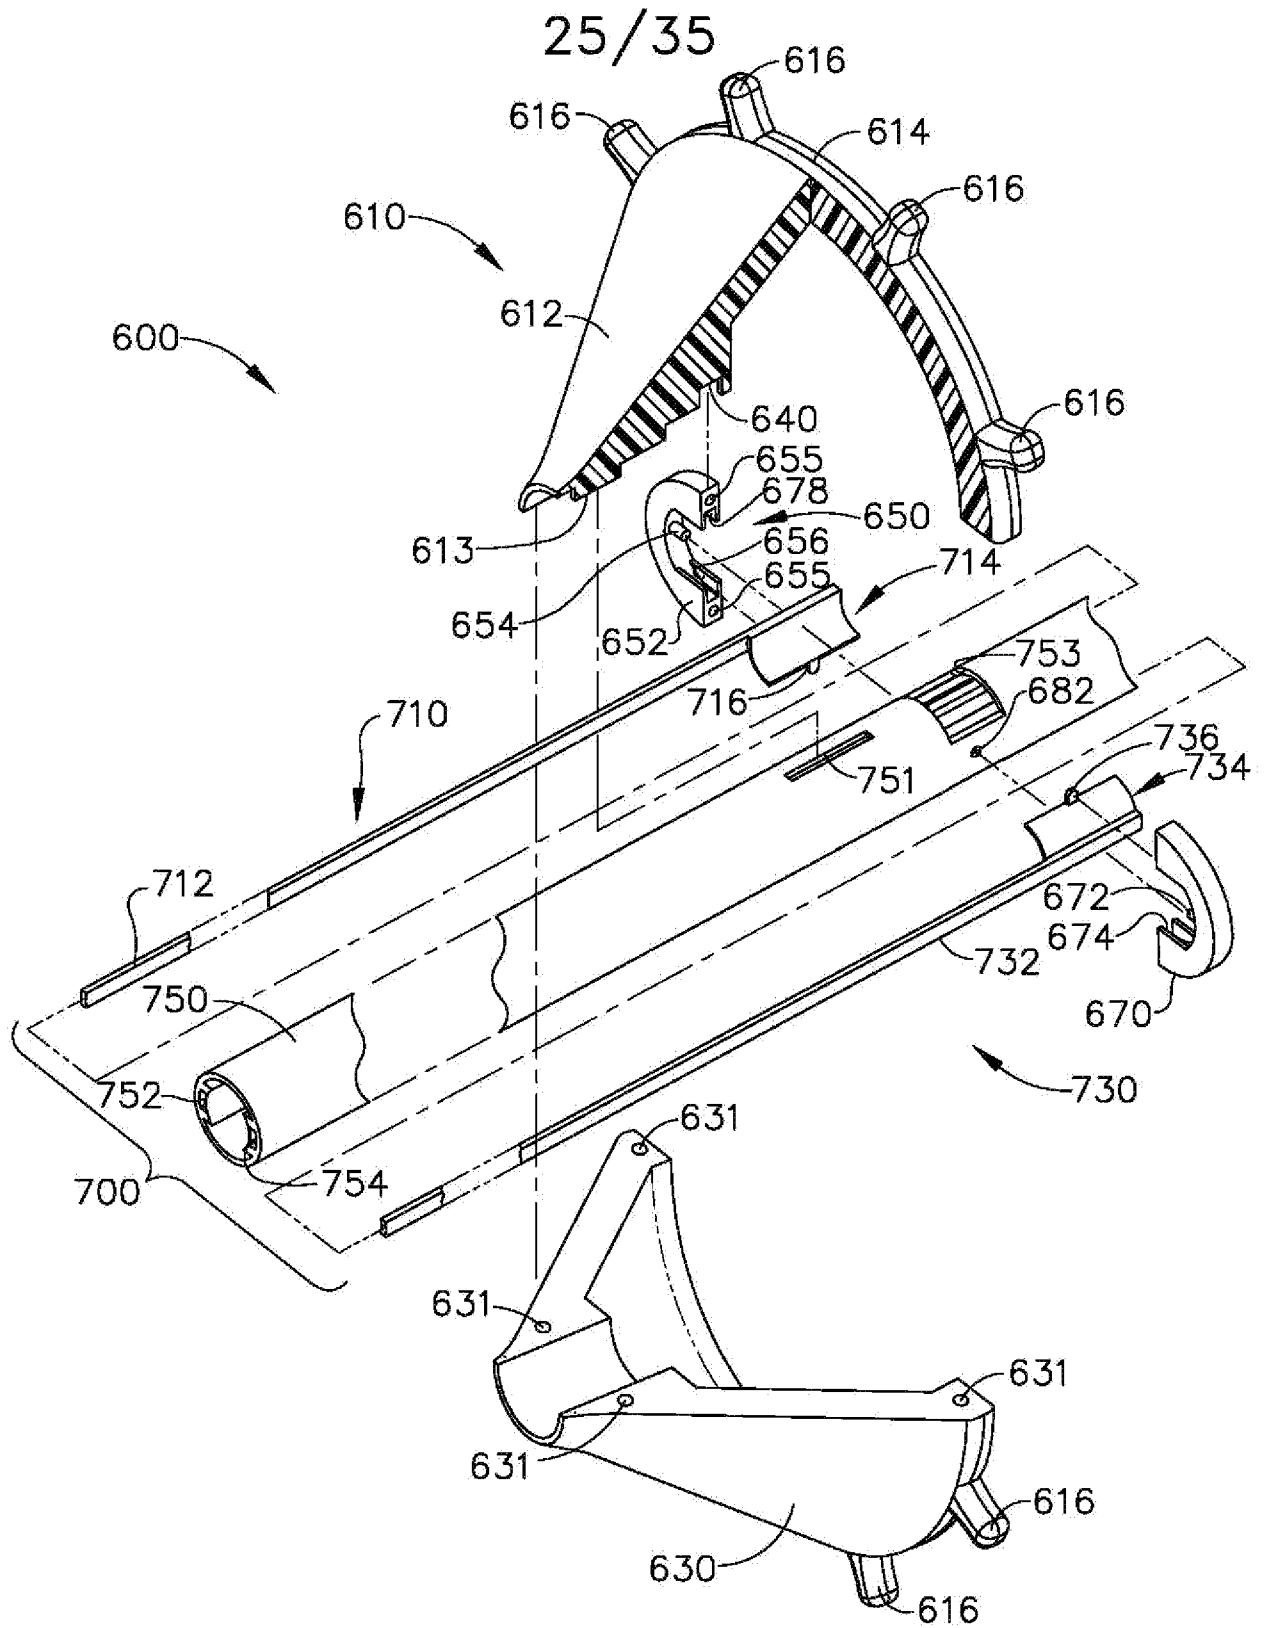


FIG. 38

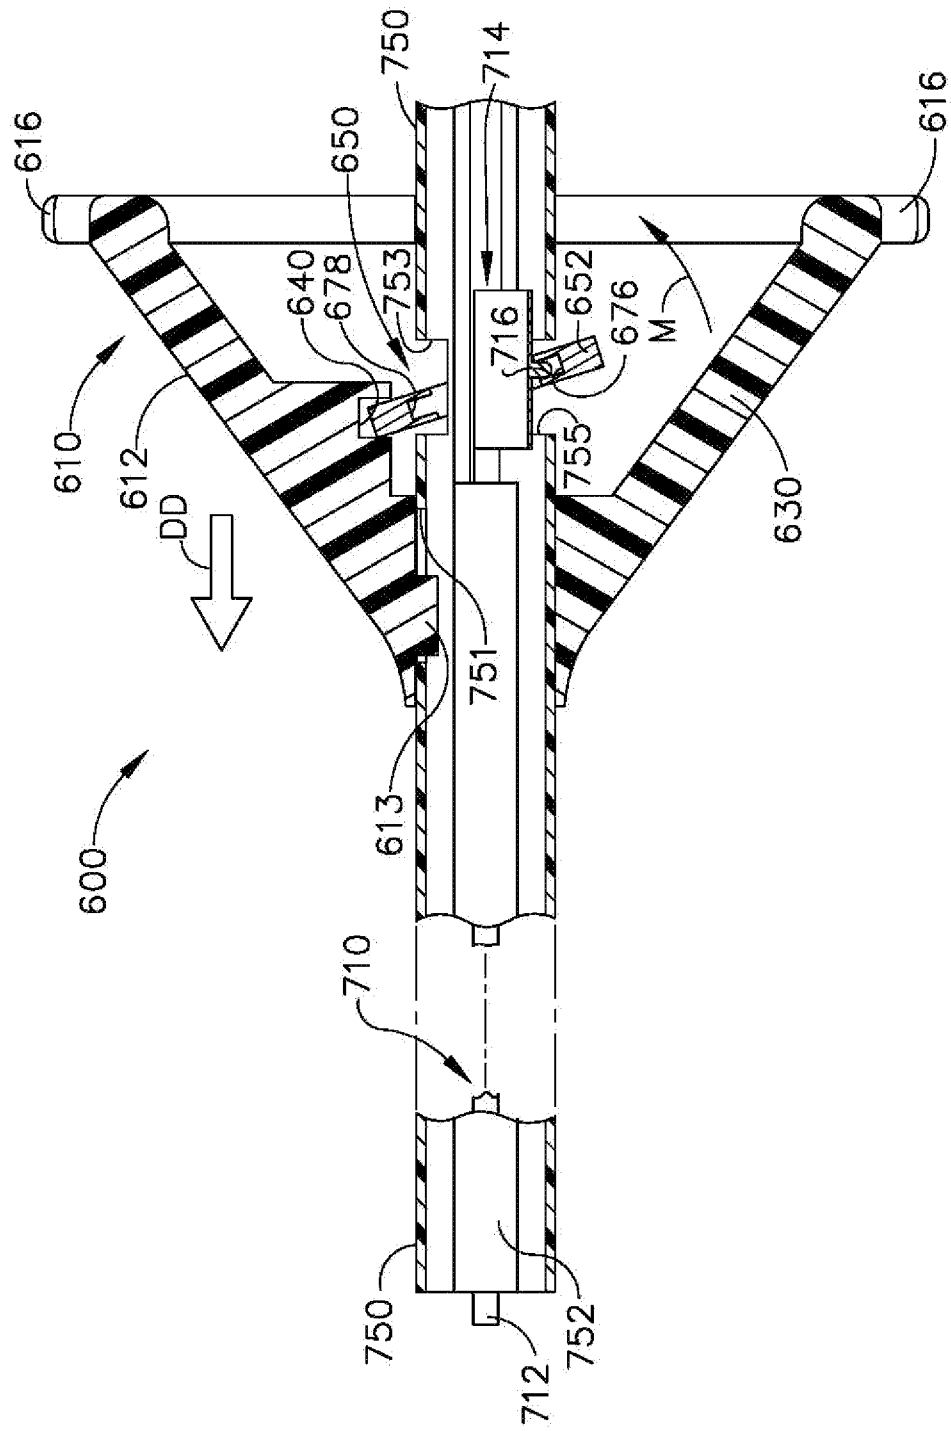


FIG. 39

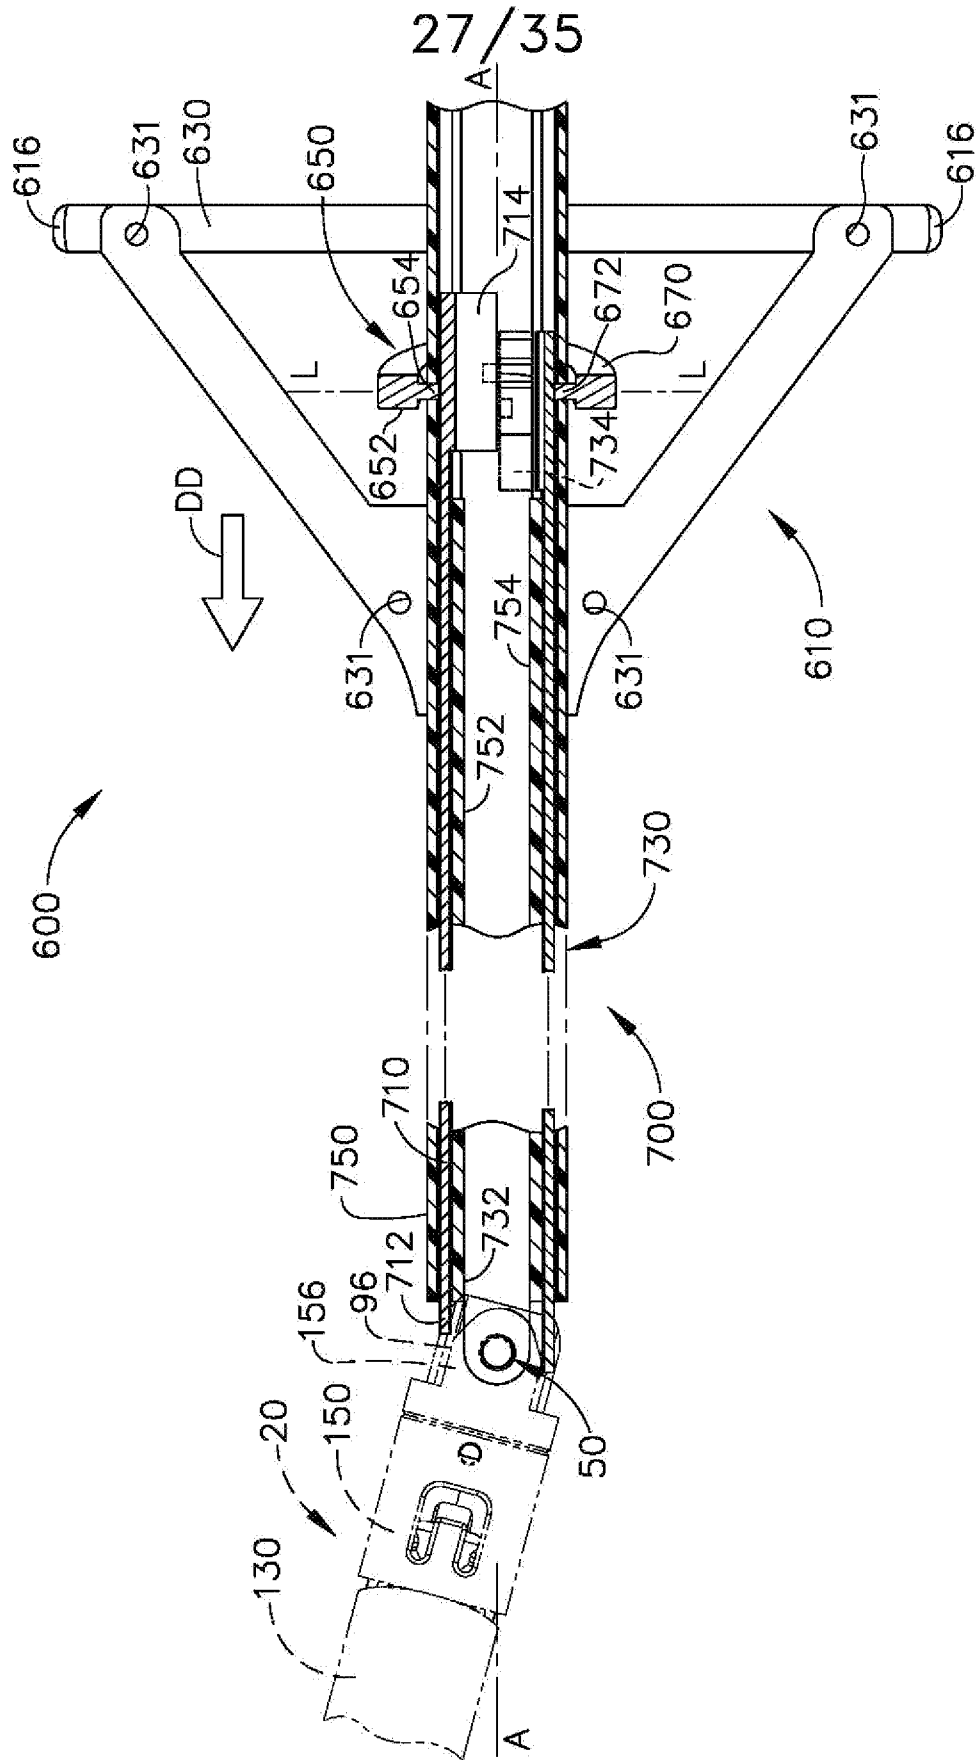


FIG. 40

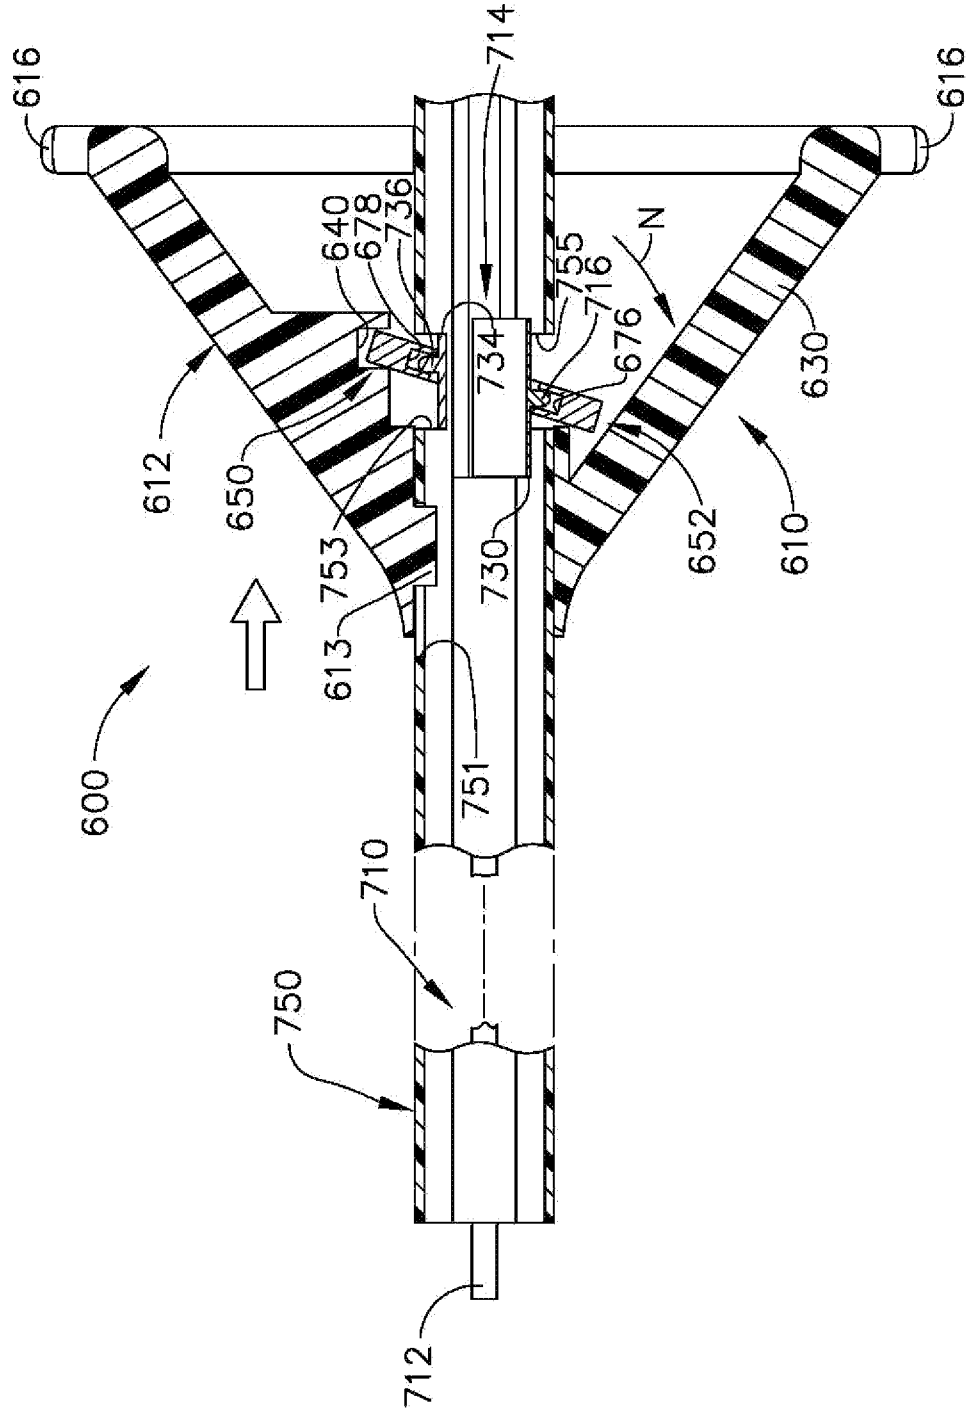


FIG. 41

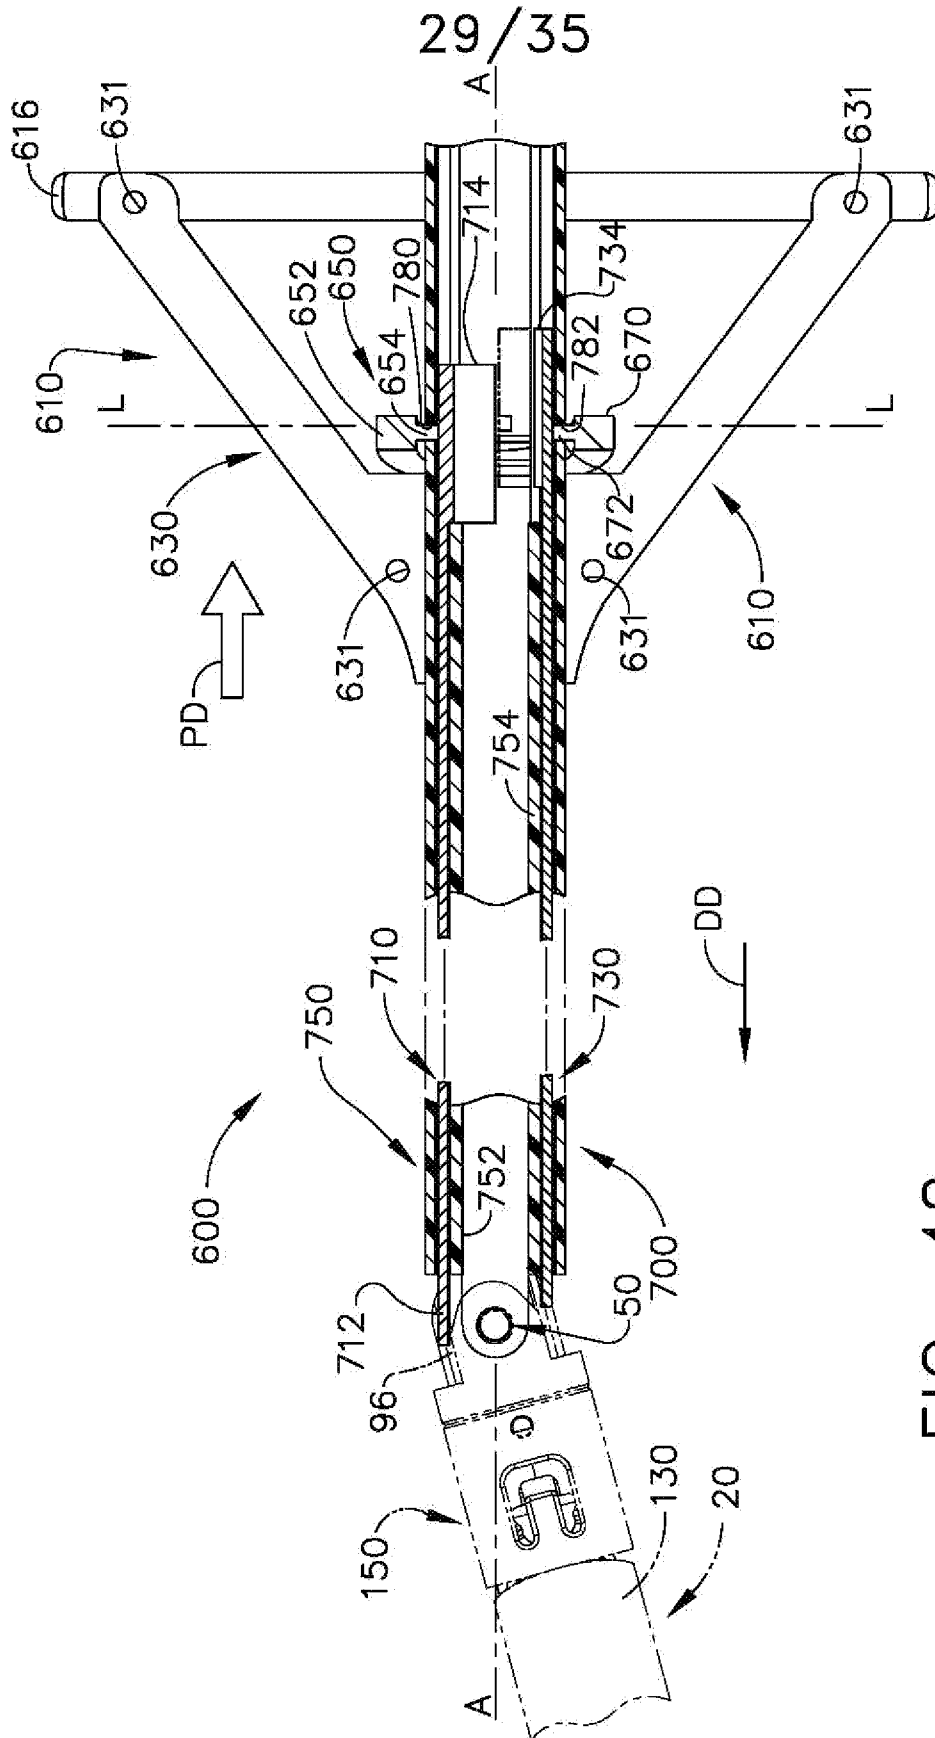


FIG. 42

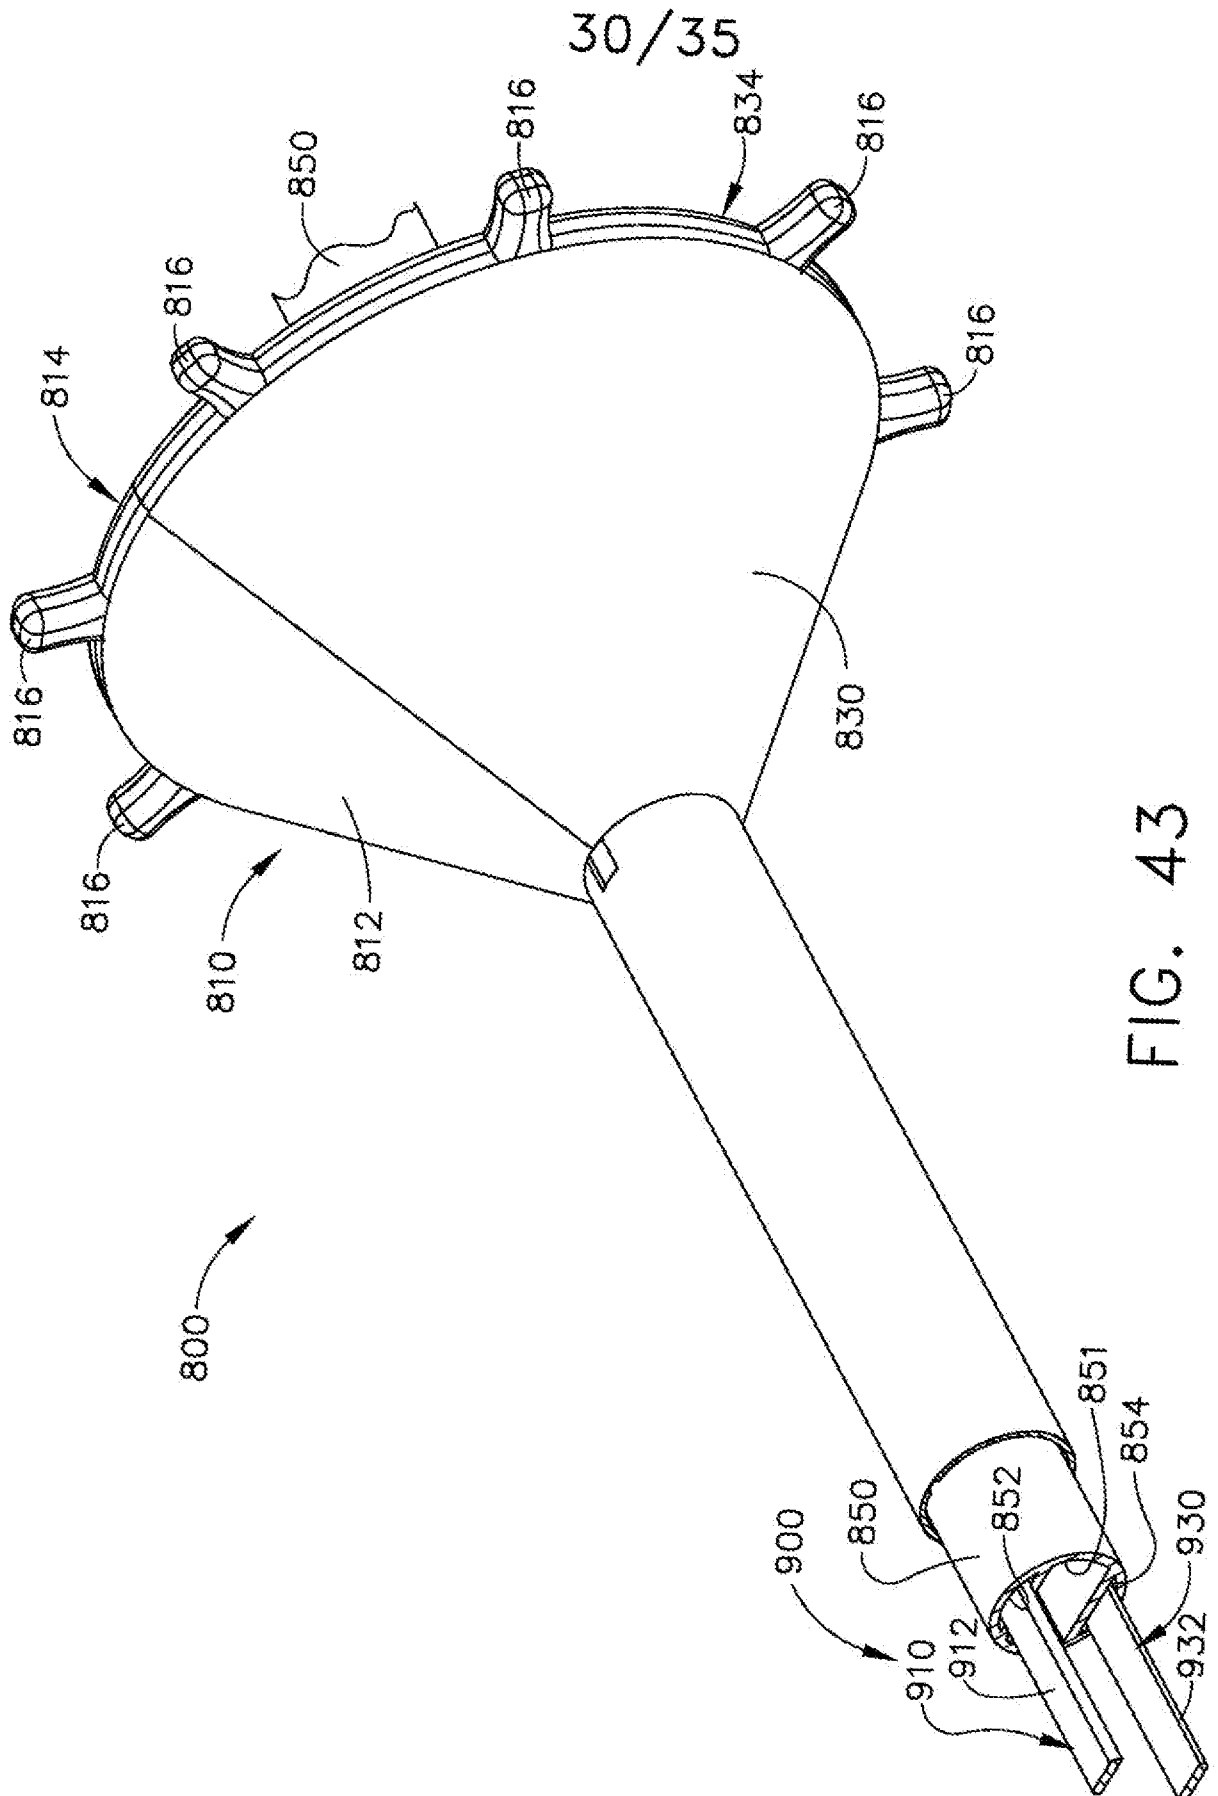


FIG. 43

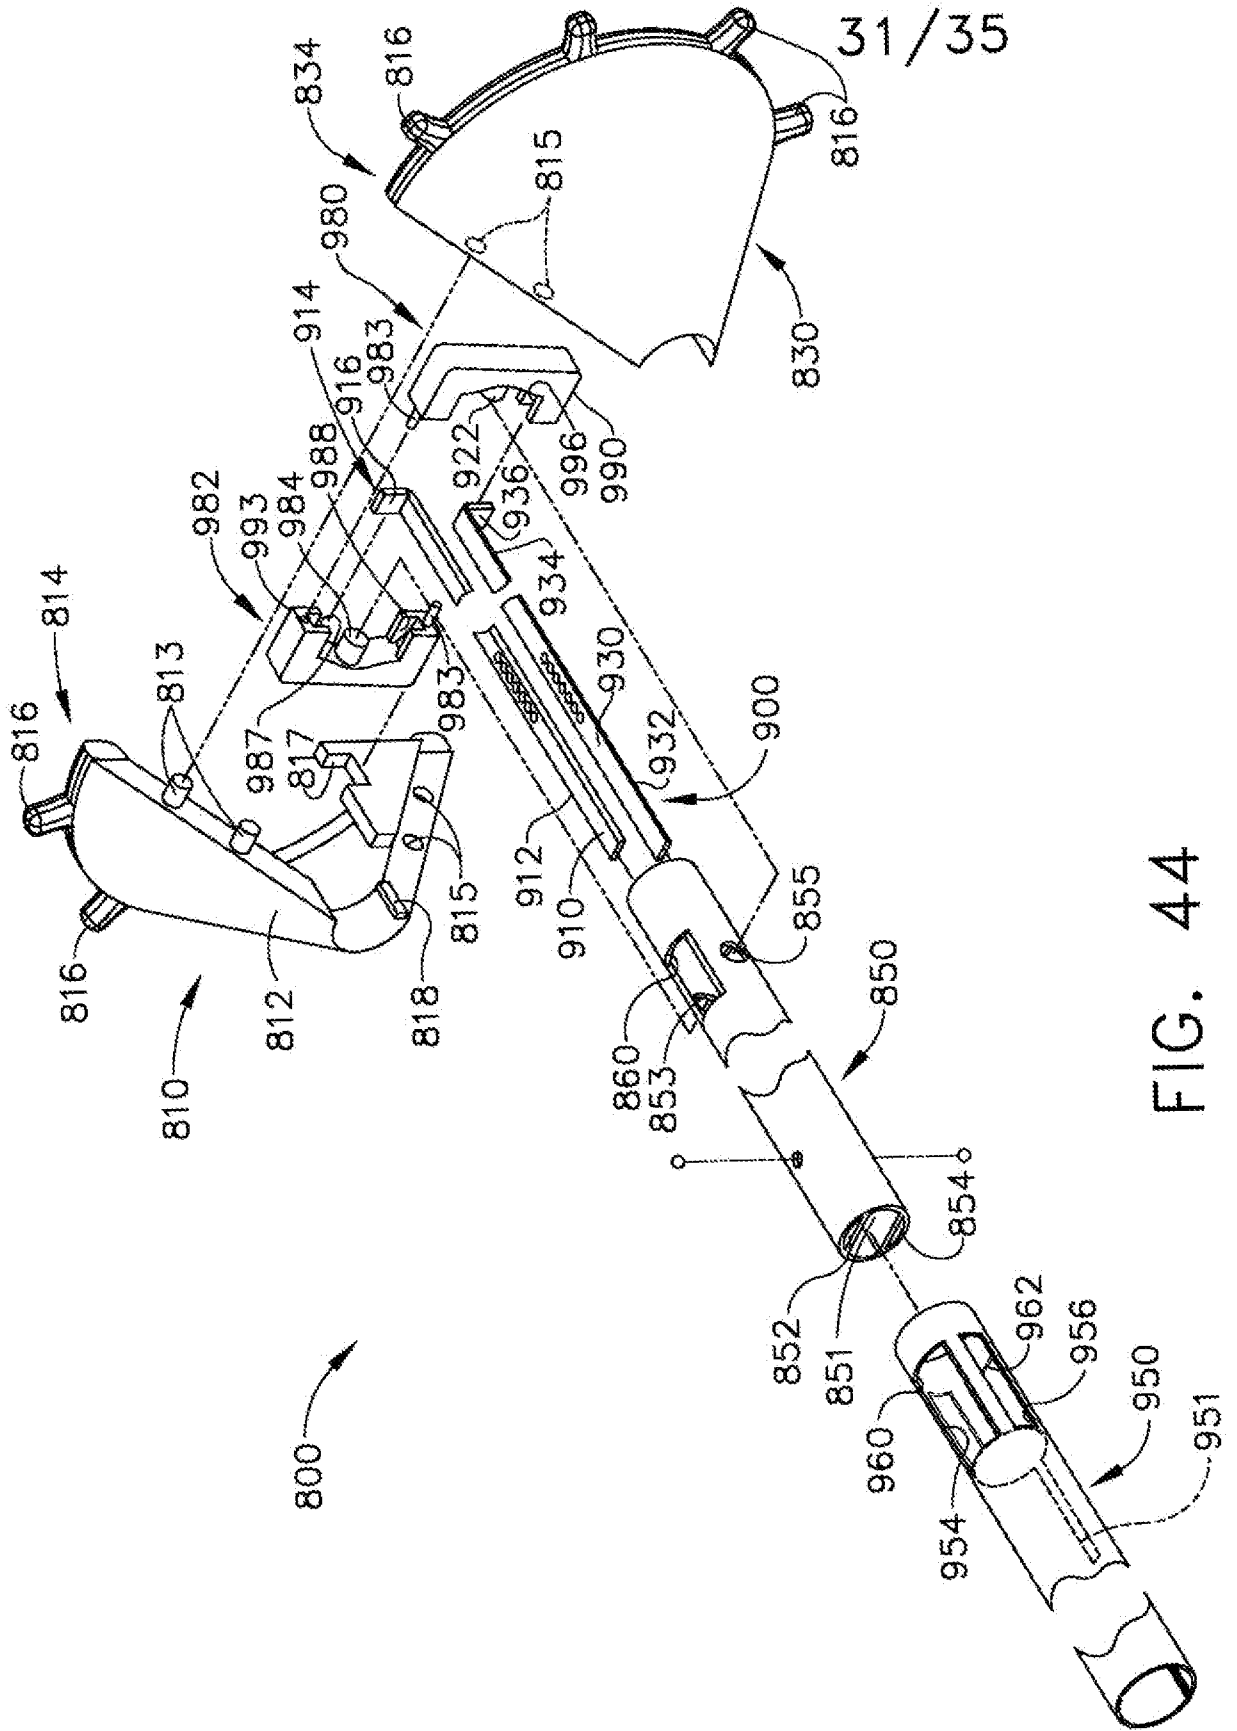


FIG. 44



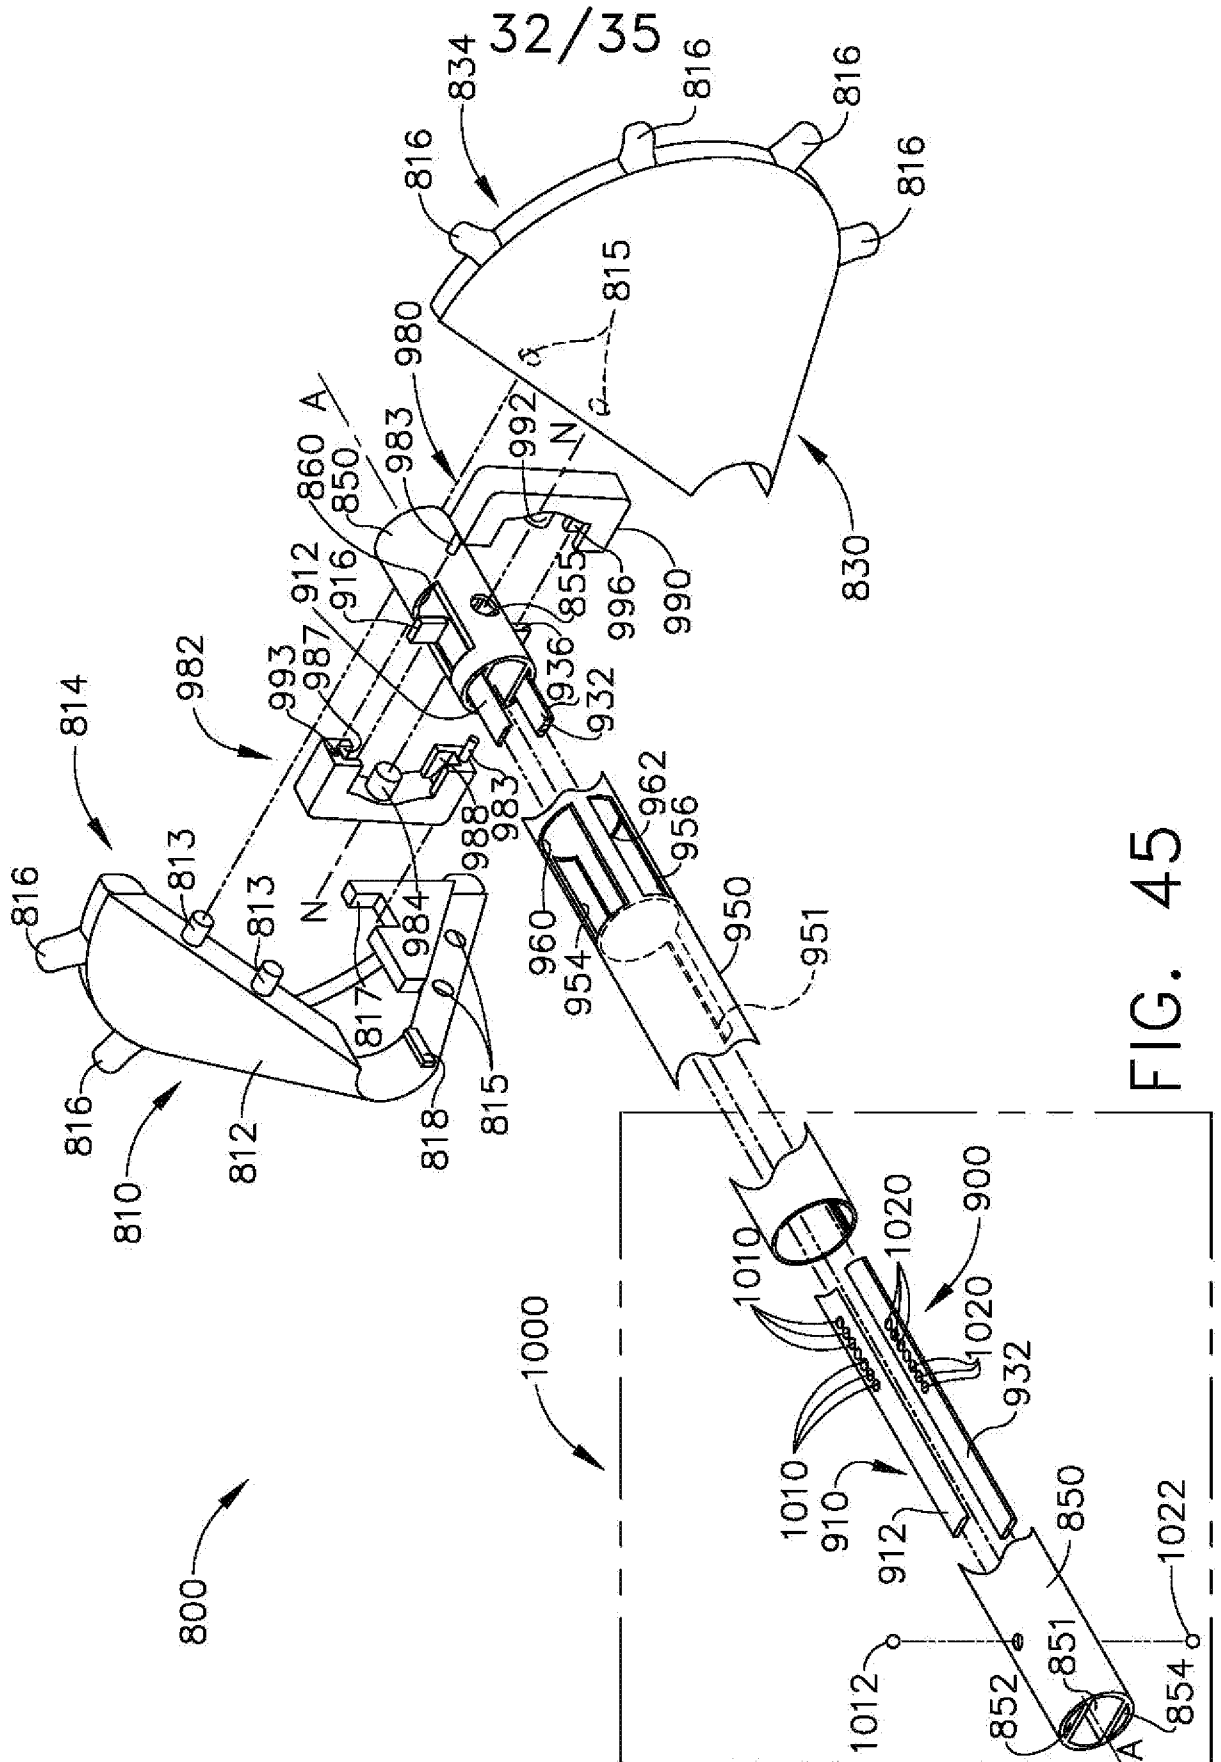


FIG. 45

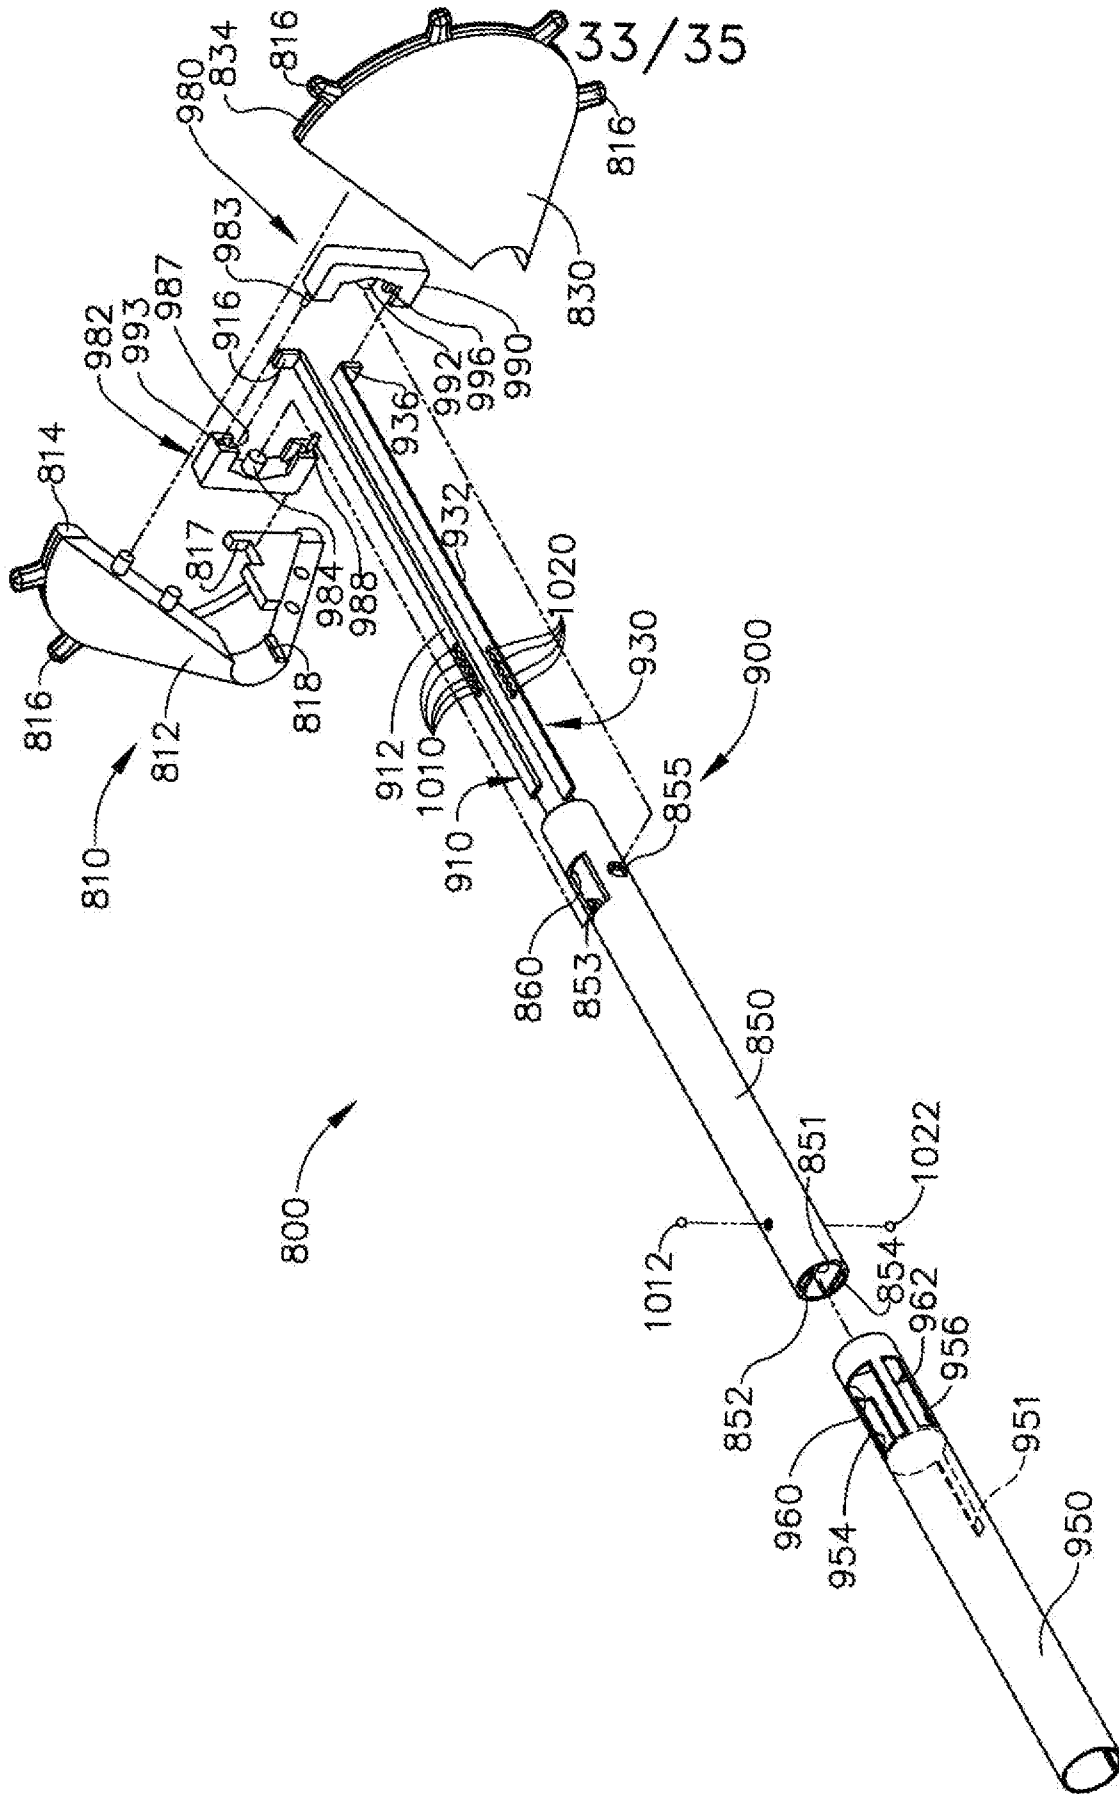
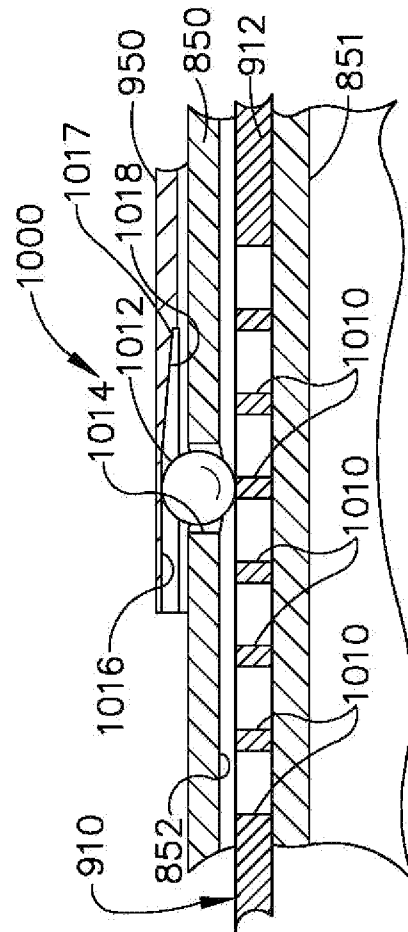
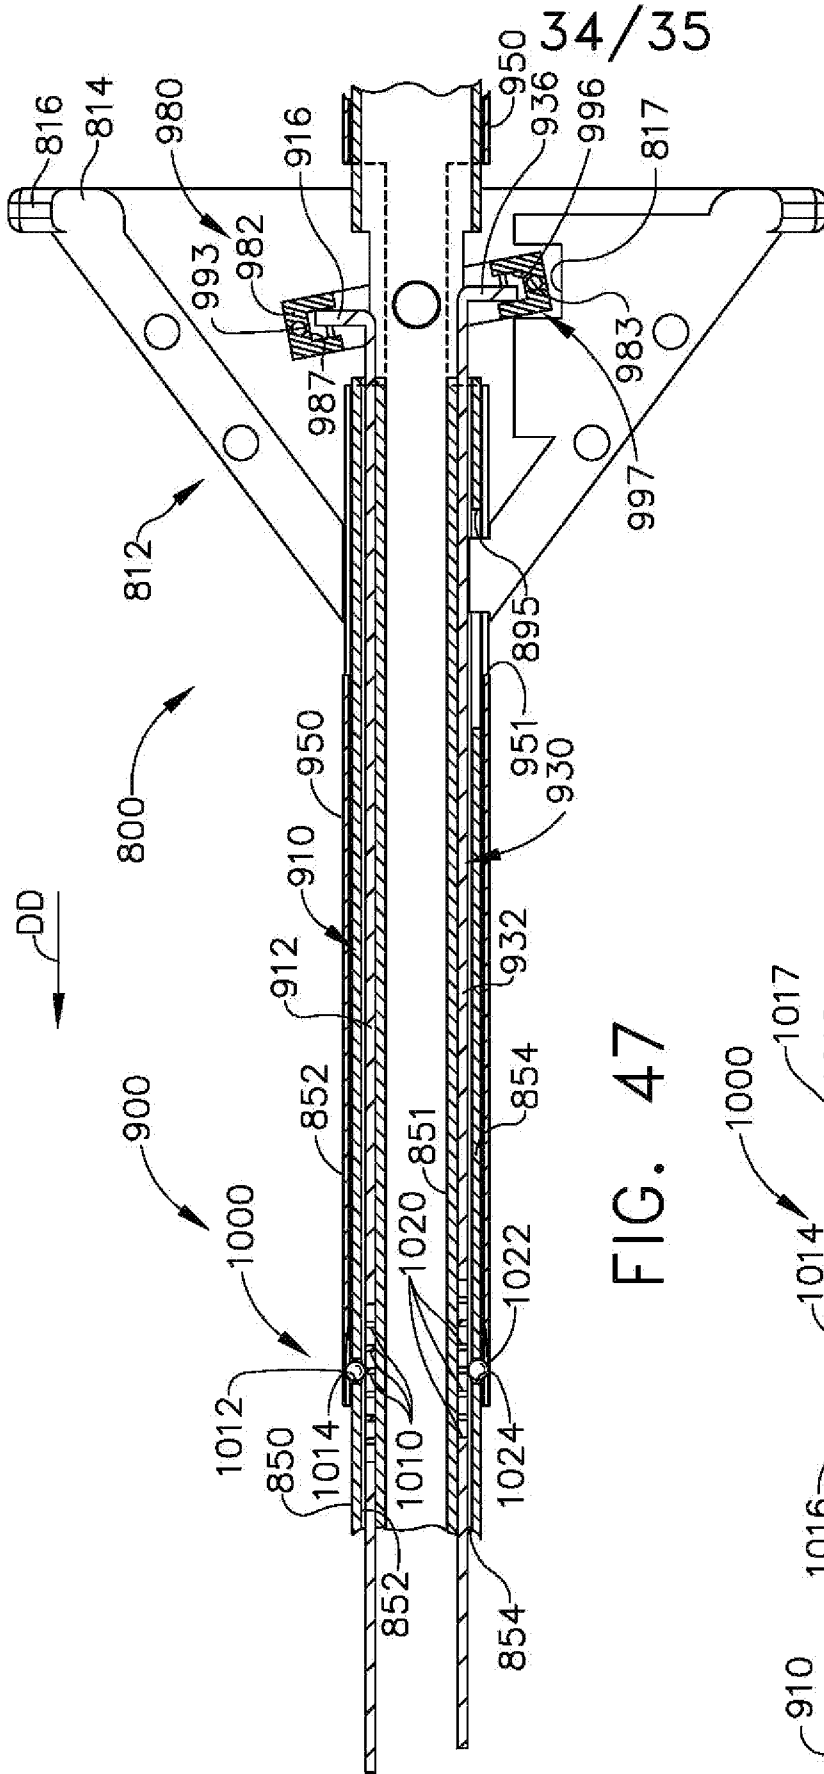


FIG. 46



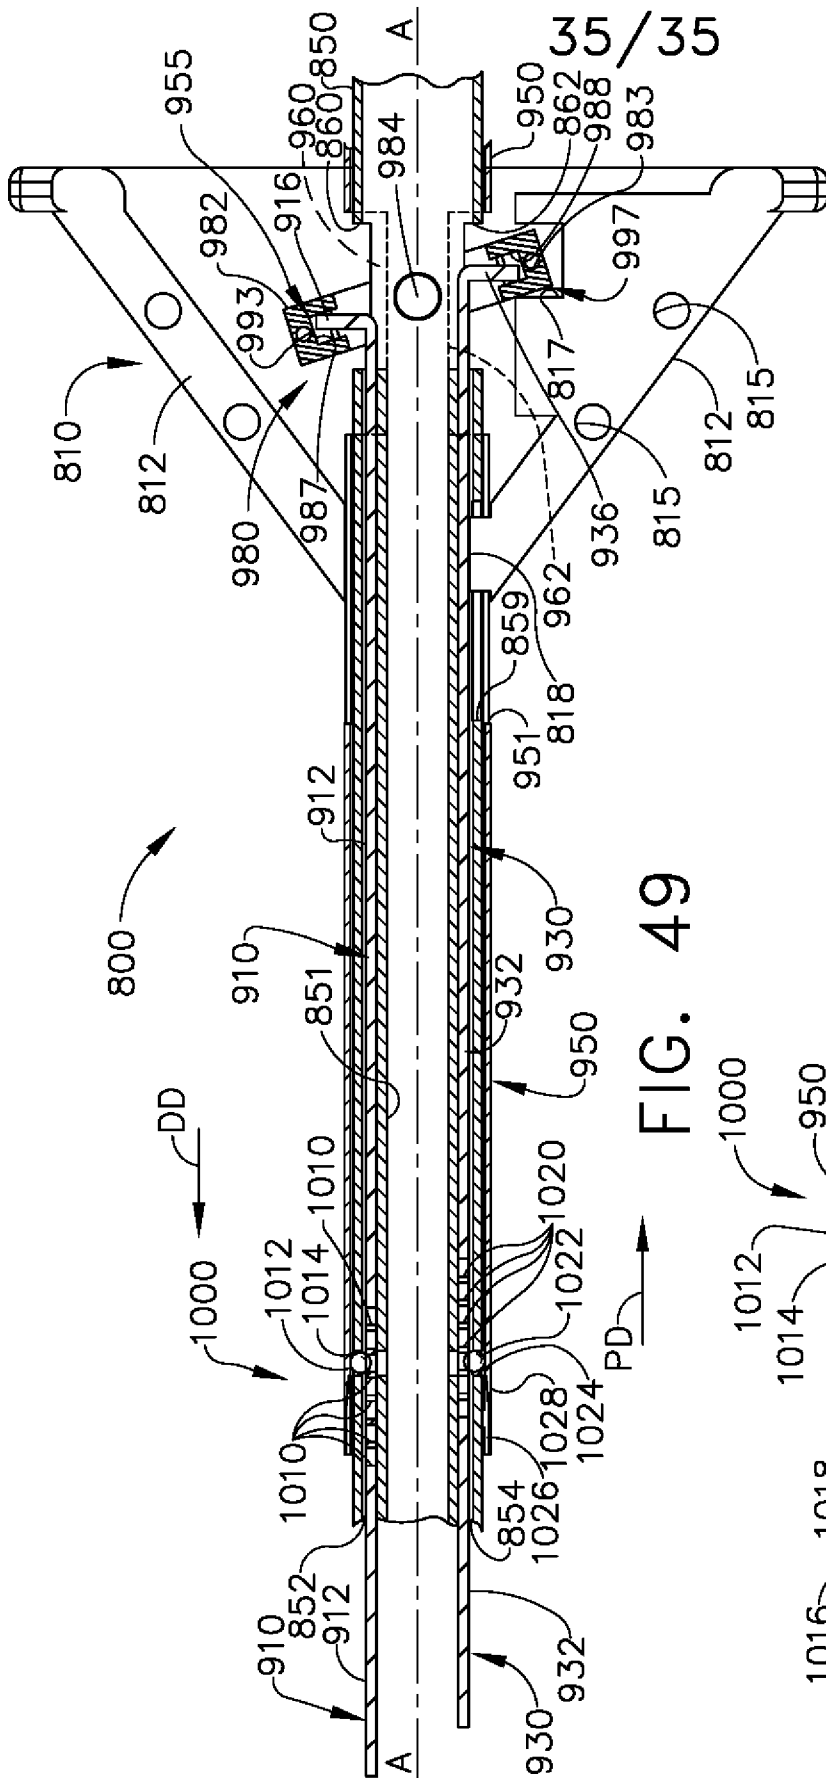


FIG. 49

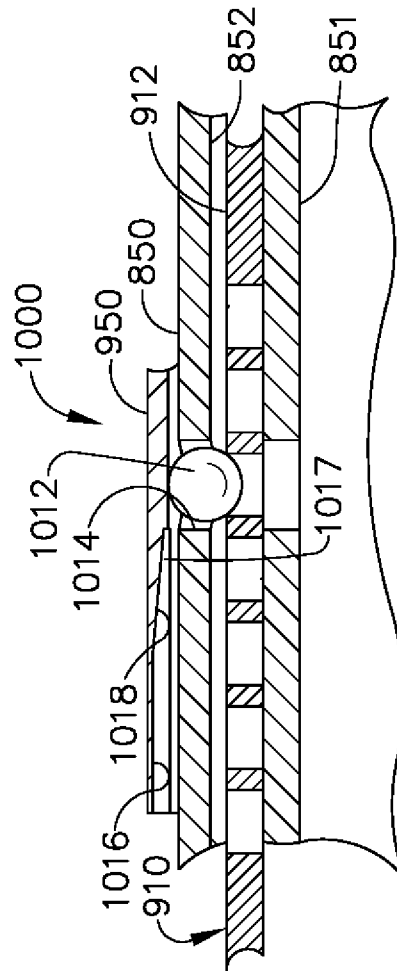


FIG. 50

# INTERNATIONAL SEARCH REPORT

International application No <b>PCT/US2012/028894</b>
--

**A. CLASSIFICATION OF SUBJECT MATTER**  
 INV. A61B17/29      A61B17/072  
 ADD.

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
**A61B**

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

**EPO-Internal**

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2009/084826 A1 (SHAH ET AL.) 2 April 2009 (2009-04-02)  the whole document -----	1, 11, 12, 14, 15, 17-20
A	US 6 666 854 B1 (LANGE) 23 December 2003 (2003-12-23) abstract; figures column 3, line 55 - column 4, line 18 column 7, lines 37-52 -----	1, 11, 18-20
A	WO 2007/145825 A2 (CAMBRIDGE ENDOSCOPIC DEVICES, INC.) 21 December 2007 (2007-12-21) abstract; figures -----	1, 11, 18-20
A	US 2009/198272 A1 (KERVER ET AL.) 6 August 2009 (2009-08-06) paragraph [0045]; figures -----	1, 11, 18-20

Further documents are listed in the continuation of Box C.
  See patent family annex.

\* Special categories of cited documents :

- |   |   |
|---|---|
| <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier application or patent but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> | <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"&amp;" document member of the same patent family</p> |
|---|---|

Date of the actual completion of the international search

1 June 2012

Date of mailing of the international search report

12/06/2012

Name and mailing address of the ISA/

European Patent Office, P.B. 5818 Patentlaan 2  
 NL - 2280 HV Rijswijk  
 Tel. (+31-70) 340-2040,  
 Fax: (+31-70) 340-3016

Authorized officer

Giménez Burgos, R

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/US2012/028894
---

Patent document cited in search report	Publication date	Patent family member(s)	Publication date	
US 2009084826	A1	02-04-2009	AU 2008207366 A1	23-04-2009
			CA 2639439 A1	28-03-2009
			CN 101396294 A	01-04-2009
			EP 2042107 A1	01-04-2009
			ES 2366493 T3	20-10-2011
			JP 2009082704 A	23-04-2009
			US 2009084826 A1	02-04-2009
			US 2010163597 A1	01-07-2010
-----				
US 6666854	B1	23-12-2003	AT 249173 T	15-09-2003
			DE 60005187 D1	16-10-2003
			DE 60005187 T2	27-05-2004
			EP 1189539 A1	27-03-2002
			FR 2795301 A1	29-12-2000
			JP 2003520623 A	08-07-2003
			US 6666854 B1	23-12-2003
			WO 0100095 A1	04-01-2001
-----				
WO 2007145825	A2	21-12-2007	NONE	
-----				
US 2009198272	A1	06-08-2009	AU 2009212240 A1	13-08-2009
			CA 2713983 A1	13-08-2009
			CN 101938946 A	05-01-2011
			EP 2240095 A2	20-10-2010
			JP 2011510800 A	07-04-2011
			KR 20100118573 A	05-11-2010
			US 2009198272 A1	06-08-2009
			WO 2009100366 A2	13-08-2009
-----				