



US0D1027215S

(12) **United States Design Patent**  
**Webb**

(10) **Patent No.:** **US D1,027,215 S**

(45) **Date of Patent:** **\*\* May 14, 2024**

(54) **MEDICAL DEVICE TRAY SEALER HAVING  
A TRAY BURST TESTING SYSTEM**

(71) Applicant: **Charles Webb**, Solvange, CA (US)

(72) Inventor: **Charles Webb**, Solvange, CA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/859,987**

(22) Filed: **Nov. 15, 2022**

(51) **LOC (14) Cl.** ..... **24-02**

(52) **U.S. Cl.**  
USPC ..... **D24/216**

(58) **Field of Classification Search**  
USPC ..... D24/107, 169, 186, 209, 210, 216, 217,  
D24/218, 219, 231-234; D10/81;  
D9/414, 430

CPC ..... G01N 2035/00158; G01N 35/1002; G01N  
35/10029; G01N 35/00732; G01N  
35/1079; B01L 7/52; C12Q 1/6844  
See application file for complete search history.

(56) **References Cited**

**U.S. PATENT DOCUMENTS**

2,822,476	A *	2/1958	Osgood	.....	A61L 2/10 250/455.11
D289,081	S *	3/1987	Ludwig	.....	D24/185
D297,361	S *	8/1988	Yamamoto	.....	D24/232
D297,564	S *	9/1988	Yamamoto	.....	D24/232
D301,611	S *	6/1989	Peterson	.....	D24/217
D347,396	S *	5/1994	Ohnuma	.....	D24/232
D378,782	S *	4/1997	LaBarbera	.....	D24/231
D380,273	S *	6/1997	Emerson	.....	D24/186
D384,446	S *	9/1997	Linton	.....	D32/1
D394,613	S *	5/1998	Kamimura	.....	D10/81
D406,416	S *	3/1999	Chan	.....	D32/1
D413,539	S *	9/1999	Ditterline	.....	D24/186
D414,304	S *	9/1999	Schumaier	.....	D32/1
D430,304	S *	8/2000	Oonuma	.....	D24/232

D445,224	S *	7/2001	Costello	.....	D32/1
D456,523	S *	4/2002	Waluszko	.....	D24/216
D527,464	S *	8/2006	Ina	.....	D24/232
D533,669	S *	12/2006	Haunschild	.....	D24/217
D546,473	S *	7/2007	Xu	.....	D24/217
D560,131	S *	1/2008	Hu	.....	D24/186
D581,823	S *	12/2008	Mori	.....	D24/186
D588,276	S *	3/2009	Isozaki	.....	D24/232
D591,864	S *	5/2009	Schmidt	.....	D24/216

(Continued)

*Primary Examiner* — T Chase Nelson

*Assistant Examiner* — Kelly L Gross

(74) *Attorney, Agent, or Firm* — Michael J. Foycik, Jr.

(57) **CLAIM**

The ornamental design for a medical device tray sealer having a tray burst testing system, as shown and described.

**DESCRIPTION**

FIG. 1 is a Front Perspective left view of a medical device tray sealer having a tray burst testing system, showing my new design;

FIG. 2 is a Front Perspective right view of the medical device tray sealer having a tray burst testing system of FIG. 1.

FIG. 3 is a Rear Perspective view of the medical device tray sealer having a tray burst testing system of FIG. 1, the right view being a mirror image of this view.

FIG. 4 is a front view of the medical device tray sealer having a tray burst testing system of FIGS. 1-3.

FIG. 5 is a back view thereof.

FIG. 6 is a left view thereof.

FIG. 7 is a right view thereof.


FIG. 8 is a top view thereof.

FIG. 9 is a bottom view thereof.

FIG. 10 is a front perspective left open tray view thereof; and,

FIG. 11 is a front perspective right open tray view thereof.

**1 Claim, 8 Drawing Sheets**

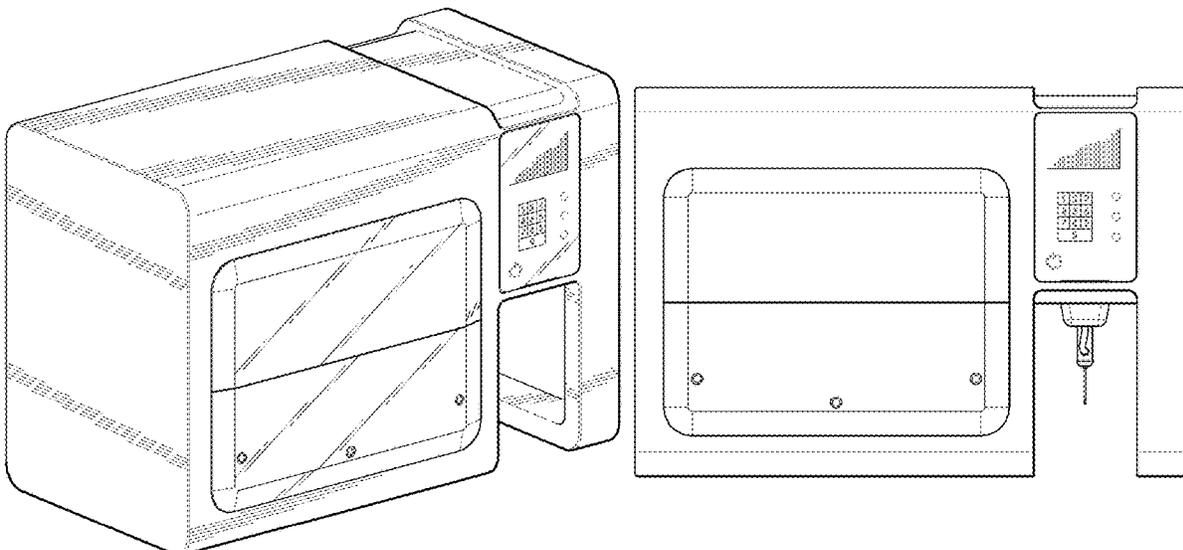


(56)

References Cited


U.S. PATENT DOCUMENTS

D598,129	S *	8/2009	Tsukuda	.....	D24/234	D777,048	S *	1/2017	Barton	.....	D24/216
D599,234	S *	9/2009	Ito	.....	D10/81	D796,056	S *	8/2017	Saito	.....	D24/232
D621,523	S *	8/2010	Onuma	.....	D24/234	D799,999	S *	10/2017	Barton	.....	D24/216
D624,197	S *	9/2010	Rindoks	.....	D24/234	D811,251	S *	2/2018	Barton	.....	D24/216
D631,976	S *	2/2011	Oonuma	.....	D24/216	D822,222	S *	7/2018	Smith	.....	D24/216
D637,931	S *	5/2011	Kimura	.....	D10/81	D830,210	S *	10/2018	Ihara	.....	D24/216
D638,952	S *	5/2011	Oonuma	.....	D24/216	D838,865	S *	1/2019	Potty	.....	D24/234
D648,844	S *	11/2011	Nelson	.....	D24/185	D843,251	S *	3/2019	Barton	.....	D24/216
D662,431	S *	6/2012	Kimura	.....	D10/81	D846,146	S *	4/2019	Amos	.....	D24/231
D663,856	S *	7/2012	Lieblein	.....	D24/216	D848,635	S *	5/2019	Davis	.....	D24/217
D670,401	S *	11/2012	Tsuda	.....	D24/216	D870,910	S *	12/2019	Livingston	.....	D24/216
D676,976	S *	2/2013	Walsh	.....	D24/216	D887,545	S *	6/2020	Heintze	.....	D24/107
D681,233	S *	4/2013	Thomas	.....	D24/232	D888,281	S *	6/2020	Hu	.....	D24/232
D681,844	S *	5/2013	Matsuguma	.....	D24/232	D895,462	S *	9/2020	Kimura	.....	D24/216
D681,845	S *	5/2013	Matsuguma	.....	D24/232	D917,063	S *	4/2021	Ong	.....	D24/216
D682,440	S *	5/2013	Degn	.....	D24/216	D918,396	S *	5/2021	Gray	.....	D24/185
D690,023	S *	9/2013	Chang	.....	D24/216	D923,197	S *	6/2021	Allegoren	.....	D24/232
D692,156	S *	10/2013	Matoba	.....	D24/232	D923,198	S *	6/2021	Allegoren	.....	D24/232
D692,157	S *	10/2013	Matoba	.....	D24/232	D944,472	S *	2/2022	Schmitt	.....	D32/1
D693,714	S *	11/2013	Noda	.....	D24/232	D954,002	S *	6/2022	Thompson	.....	D13/162
D703,343	S *	4/2014	Biswas	.....	D24/217	D954,288	S *	6/2022	Wade	.....	D24/216
D705,432	S *	5/2014	Lura	.....	D24/185	D956,261	S *	6/2022	Segawa	.....	D24/232
D705,441	S *	5/2014	Chang	.....	D24/216	D959,014	S *	7/2022	Kim	.....	D12/416
D714,944	S *	10/2014	Gerber	.....	D24/185	D962,473	S *	8/2022	Wu	.....	D24/232
D716,966	S *	11/2014	Lizari Illarramendi	.....	D24/232	D967,456	S *	10/2022	Allegoren	.....	D24/232
D719,666	S *	12/2014	Manian	.....	D24/216	D968,645	S *	11/2022	Allegoren	.....	D24/232
D719,667	S *	12/2014	Manian	.....	D24/216	D977,139	S *	1/2023	Lai	.....	D24/217
D721,815	S *	1/2015	Lura	.....	D24/185	D981,881	S *	3/2023	Henderson	.....	D24/216
D755,405	S *	5/2016	Zhu	.....	D24/216	D984,293	S *	4/2023	Tam	.....	D10/75
						D992,081	S *	7/2023	McKelvie	.....	D24/217
						D992,140	S *	7/2023	Clottu	.....	D24/217
						2019/0092506	A1 *	3/2019	Webb	.....	B29C 66/43121


\* cited by examiner

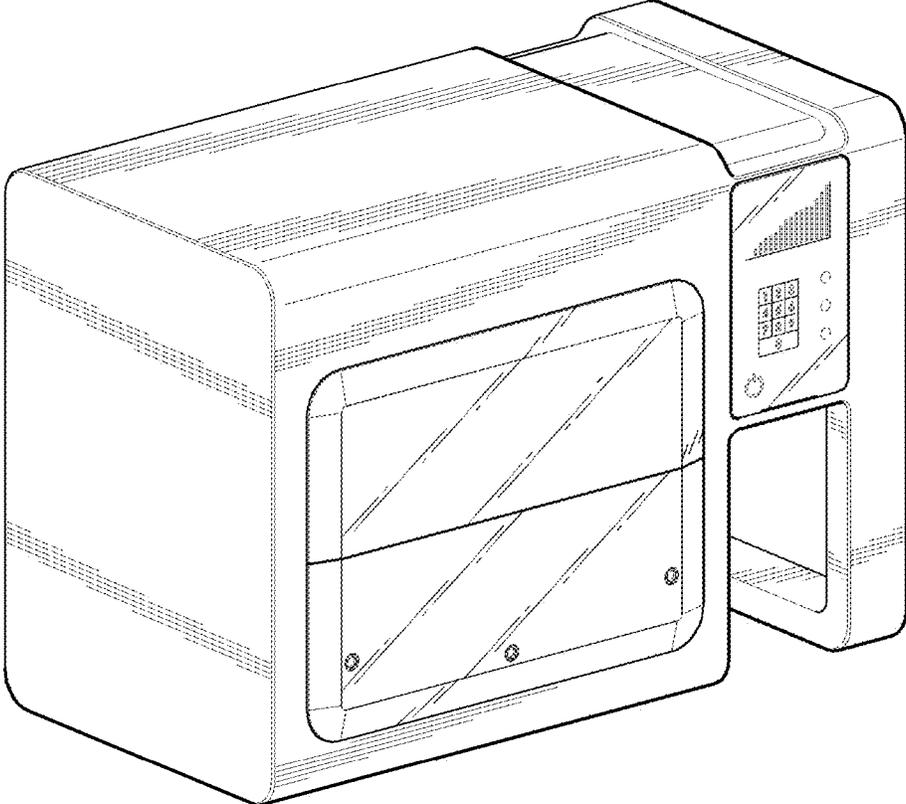


**FIG. 1**

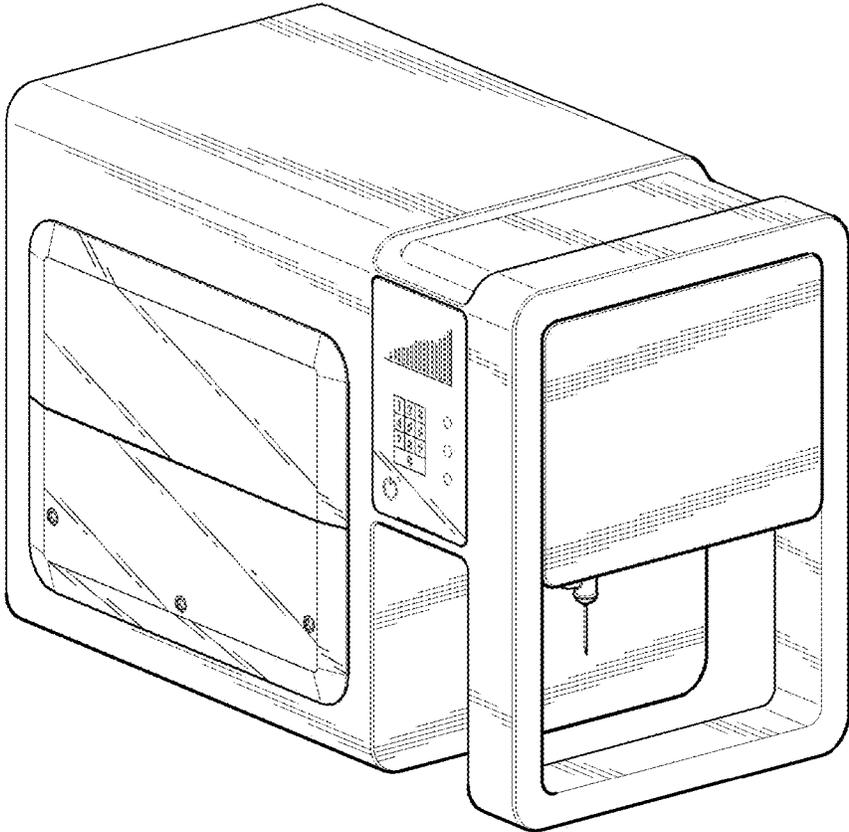


**FIG. 2**

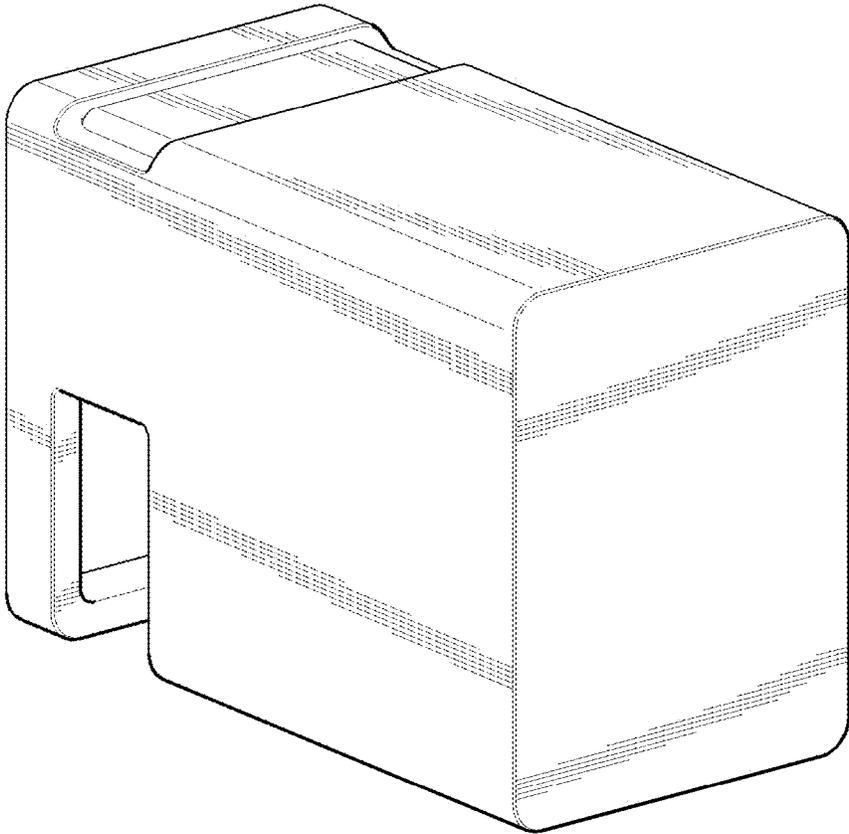


***FIG. 3***

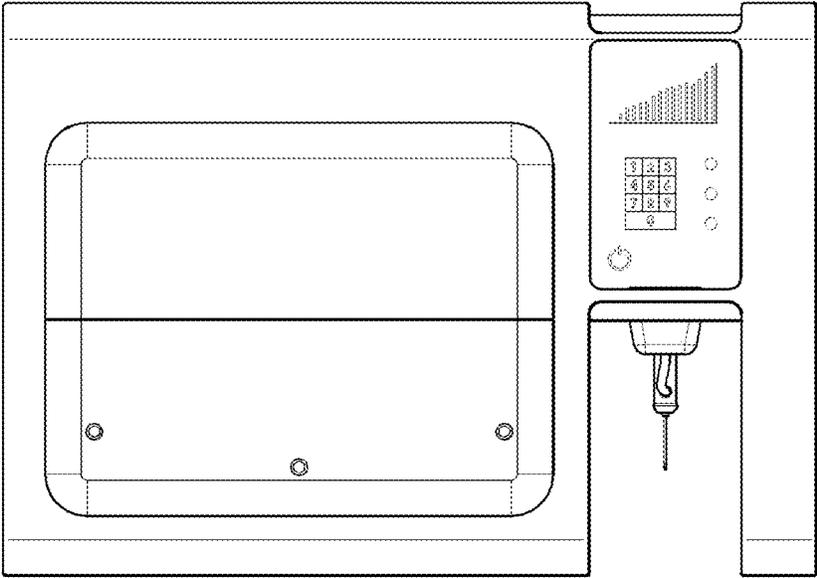


**FIG. 4**

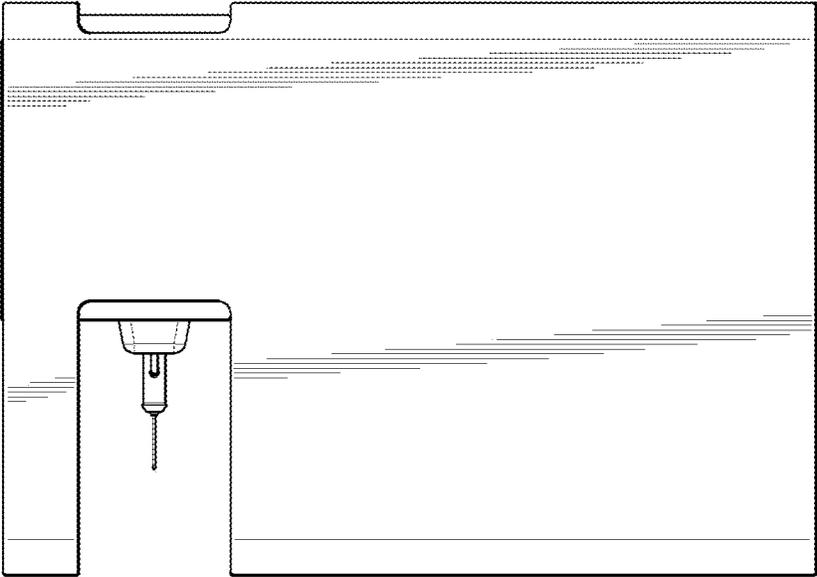


**FIG. 5**

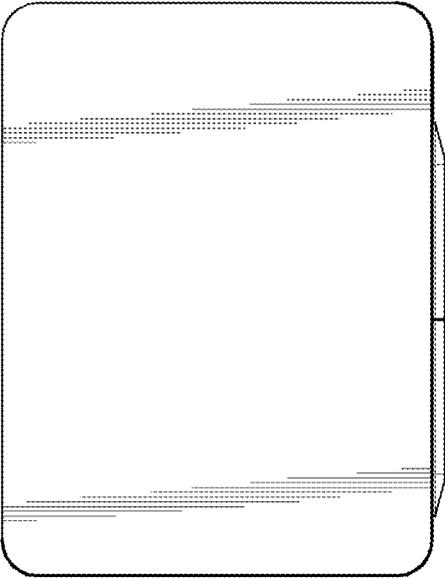


**FIG. 6**

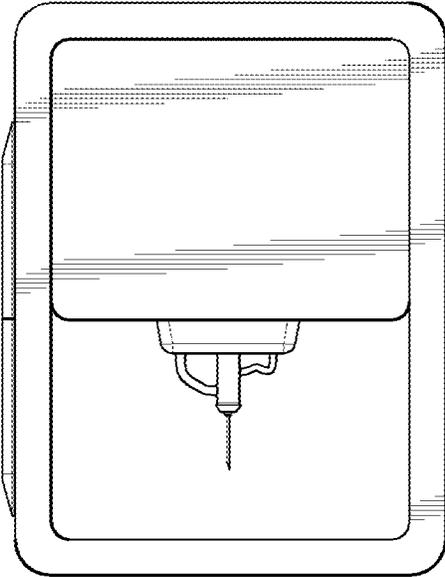


**FIG. 7**

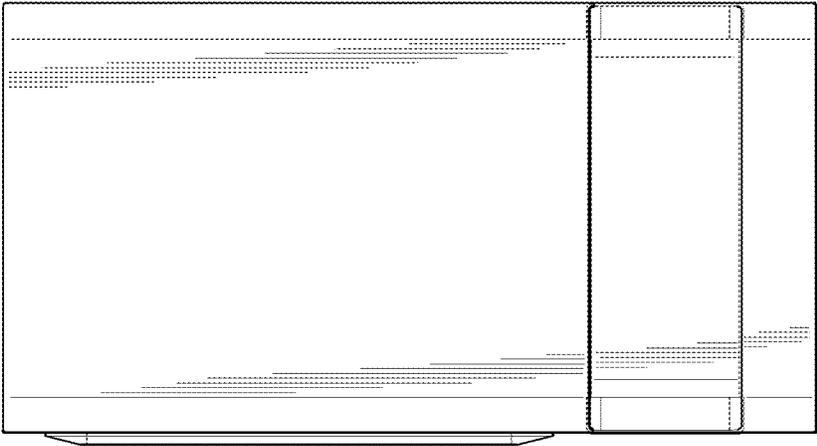


**FIG. 8**

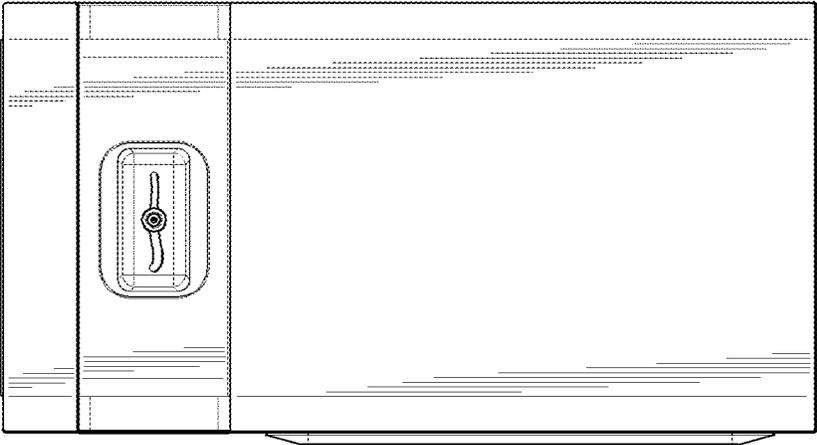

**FIG. 9**

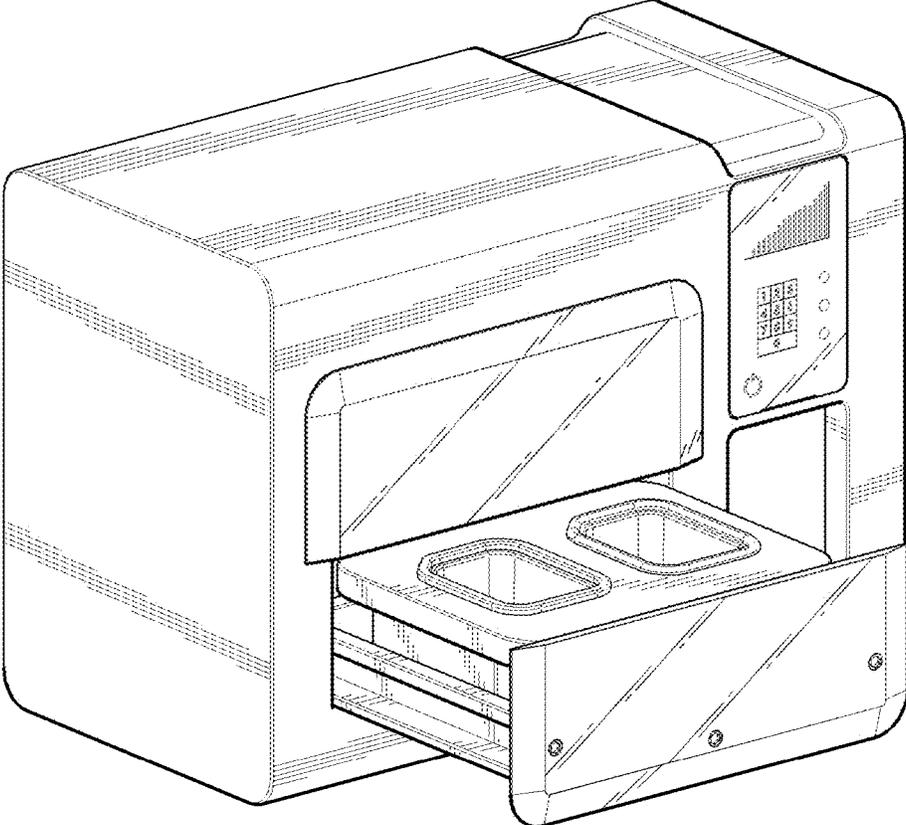

**FIG. 10**

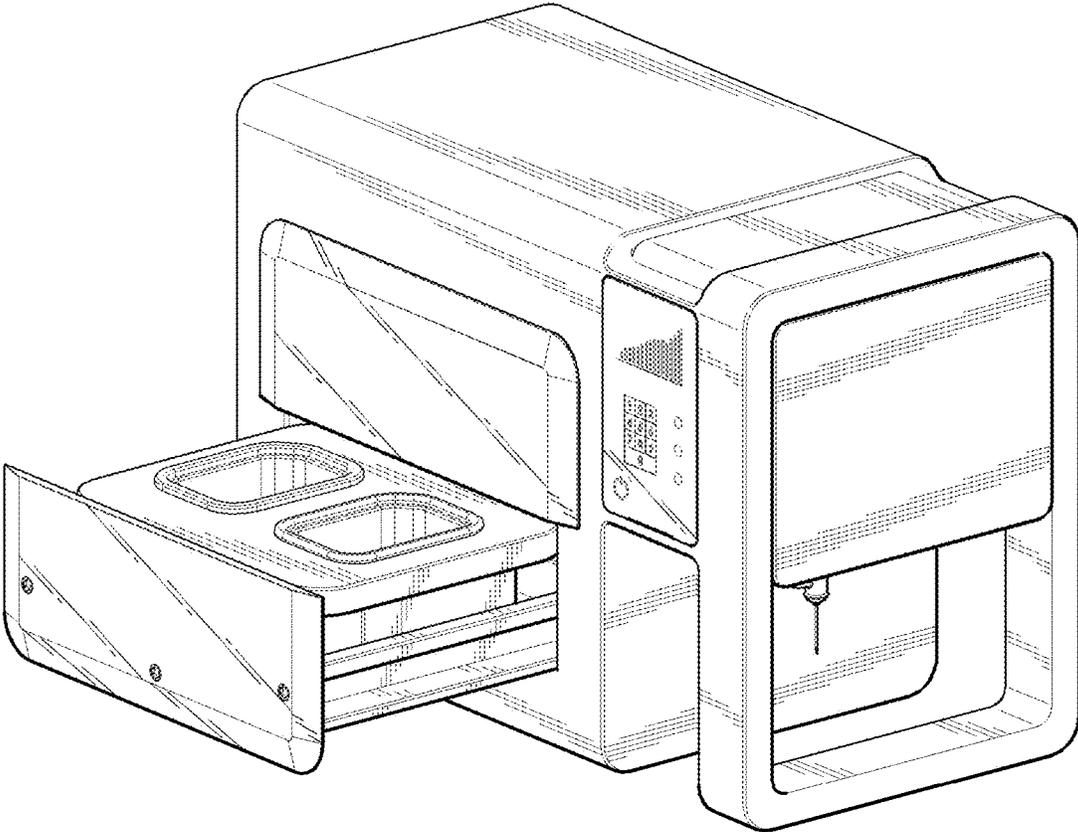

**FIG. 11**