



US0D1038401S

(12) **United States Design Patent**
Kim

(10) **Patent No.:** **US D1,038,401 S**

(45) **Date of Patent:** **** *Aug. 6, 2024**

(54) **MEDICAL DEVICE FOR TRICUSPID VALVE
REGURGITATION**

FOREIGN PATENT DOCUMENTS

(71) Applicant: **TAU-PNU MEDICAL CO., LTD.**,
Busan (KR)

GB 9004722916-0007 * 2/2018
JP D1731370 * 7/2022

(Continued)

(72) Inventor: **June Hong Kim**, Busan (KR)

OTHER PUBLICATIONS

(73) Assignee: **TAU-PNU MEDICAL CO., LTD.**,
Busan (KR)

Cleveland Clinic, New Sutureless Aortic Valve: Perspectives from Its Earliest U.S. Adopter (Video), Published on: May 3, 2016, consultqd.clevelandclinic.org, Retrieved from Internet: https://consultqd.clevelandclinic.org/new-sutureless-aortic-valve-perspectives-earliest-u-sadopter-video/ (Year: 2016).*

(Continued)

(*) Notice: This patent is subject to a terminal disclaimer.

(**) Term: **15 Years**

Primary Examiner — Jennifer L Rempfer

Assistant Examiner — Edward P Jones

(21) Appl. No.: **29/810,083**

(74) *Attorney, Agent, or Firm* — Justin H. Kim

(22) Filed: **Sep. 30, 2021**

(30) **Foreign Application Priority Data**

Apr. 1, 2021 (JP) 2021-006968

(51) **LOC (14) Cl.** **24-02**

(52) **U.S. Cl.**

USPC **D24/167**

(58) **Field of Classification Search**

USPC D24/167, 155, 112, 231

CPC A61F 2/06; A61F 2/24; A61F 2/82; A61F 2/243; A61F 2/246; A61F 2/915; A61F 2/848; A61F 2/2409; A61F 2/2412; A61F 2/2418; A61F 2/2427; A61F 2/2433; A61F 2/2436; A61F 2/2442; A61F 2/2445; A61F

(Continued)

(56) **References Cited**

U.S. PATENT DOCUMENTS

8,216,302 B2 * 7/2012 Wilson A61F 2/246
623/2.11

9,259,317 B2 * 2/2016 Wilson A61F 2/2466

(Continued)

(57) **CLAIM**

The ornamental design for a medical device for tricuspid valve regurgitation, as shown as described.

DESCRIPTION

FIG. 1 is a front view of a medical device for tricuspid valve regurgitation;

FIG. 2 is an enlarged detail front view of FIG. 1;

FIG. 3 is an enlarged detail rear view FIG. 1;

FIG. 4 is an enlarged detail top view of FIG. 1;

FIG. 5 is an enlarged detail bottom view of FIG. 1;


FIG. 6 is an enlarged detail right view of FIG. 1;

FIG. 7 is an enlarged detail left view of FIG. 1; and,

FIG. 8 is an enlarged detail perspective view of FIG. 1.

The dashed broken lines in the drawings depict portions of the medical device for tricuspid regurgitation that form no part of the claimed design. The dashed broken lines define the bounds of the claimed design and form no part thereof. The dashed break-line in the enlarged views FIGS. 2-8 indicates the boundary of the detail view and forms no part of the claimed design.

1 Claim, 8 Drawing Sheets

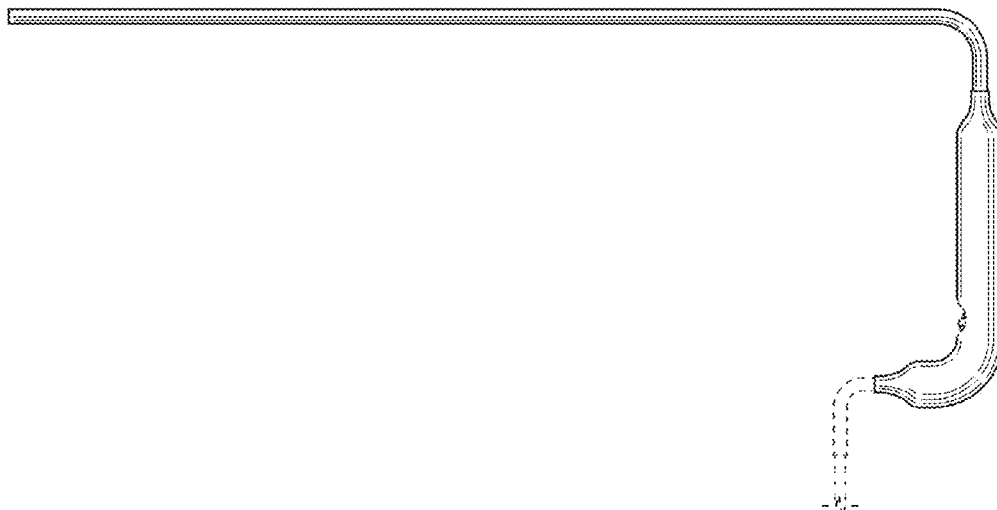

(58) **Field of Classification Search**

CPC 2/2454; A61F 2/2457; A61F 2/2463; A61F 2/2466

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D1,019,952	S *	3/2024	Kim	D24/167
D1,019,953	S *	3/2024	Kim	D24/167
2009/0137968	A1 *	5/2009	Rottenberg	A61M 29/02 604/509
2013/0190798	A1 *	7/2013	Kapadia	A61F 2/246 606/195
2013/0338763	A1 *	12/2013	Rowe	A61F 2/246 623/2.11
2020/0000592	A1 *	1/2020	Lee	A61F 2/2427
2020/0229824	A1 *	7/2020	Kim	A61B 17/12122
2022/0160500	A1 *	5/2022	Kim	A61F 2/2466
2023/0099085	A1 *	3/2023	Kim	A61F 2/2487 623/2.11
2023/0397991	A1 *	12/2023	Kim	A61F 2/2466

FOREIGN PATENT DOCUMENTS

KR	301175425	*	10/2021
KR	301175427	*	10/2021
KR	301175431	*	10/2021
KR	301175432	*	10/2021
KR	301175435	*	10/2021
KR	301175438	*	10/2021

OTHER PUBLICATIONS

Daily Mail Reporter, Artificial valve could replace open heart surgery for frail patients in the U.S., Published on: Jul. 18, 2011, dailymail.co.uk, Retrieved from Internet: <https://www.dailymail.co.uk/health/article-2016093/Artificial-valve-replace-open-heart-surgery-frail-patients-U-S.html> (Year: 2011).*

Dicardiology News, First U.S. Transcatheter Tricuspid NaviGate Valve Successfully Implanted, Published on: Dec. 31, 2016, dicardiology.com, <https://www.dicardiology.com/content/first-us-transcatheter-tricuspid-navigate-valve-successfully-implanted> (Year: 2016).*

FDA, Summary of Safety and Effectiveness Data (SSED) of Perceval Sutureless Heart Valve, Jan. 8, 2016, accessdata.fda.gov, Retrieved from Internet: https://www.accessdata.fda.gov/cdrh_docs/pdf15/p150011b.pdf (Year: 2016).*

Tau-PNU Medical & Tau Cardio, Pivot-TR (Tricuspid Valve Regurgitation), Uploaded on: Sep. 16, 2021, YouTube, Retrieved from Internet: <https://www.youtube.com/watch?v=TCNJLNPvRJY> (Year: 2023).*

Edwards Lifesciences Corp., Building on the benefits of the Sapien 3 platform, Downloaded from Internet: Jul. 2023, Retrieved from Internet: <https://www.edwards.com/healthcare-professionals/products-services/transcatheter-heart/transcatheter-sapien-3-ultra-resilia> (Year: 2023).*

Min-Ku Chon, A Novel Device for Tricuspid Regurgitation Reduction Featuring 3-Dimensional Leaflet and Atraumatic Anchor, Published on: Dec. 1, 2022, Elsevier, Retrieved from Internet: <https://www.sciencedirect.com/science/article/pii/S2452302X22002686> (Year: 2022).*

* cited by examiner

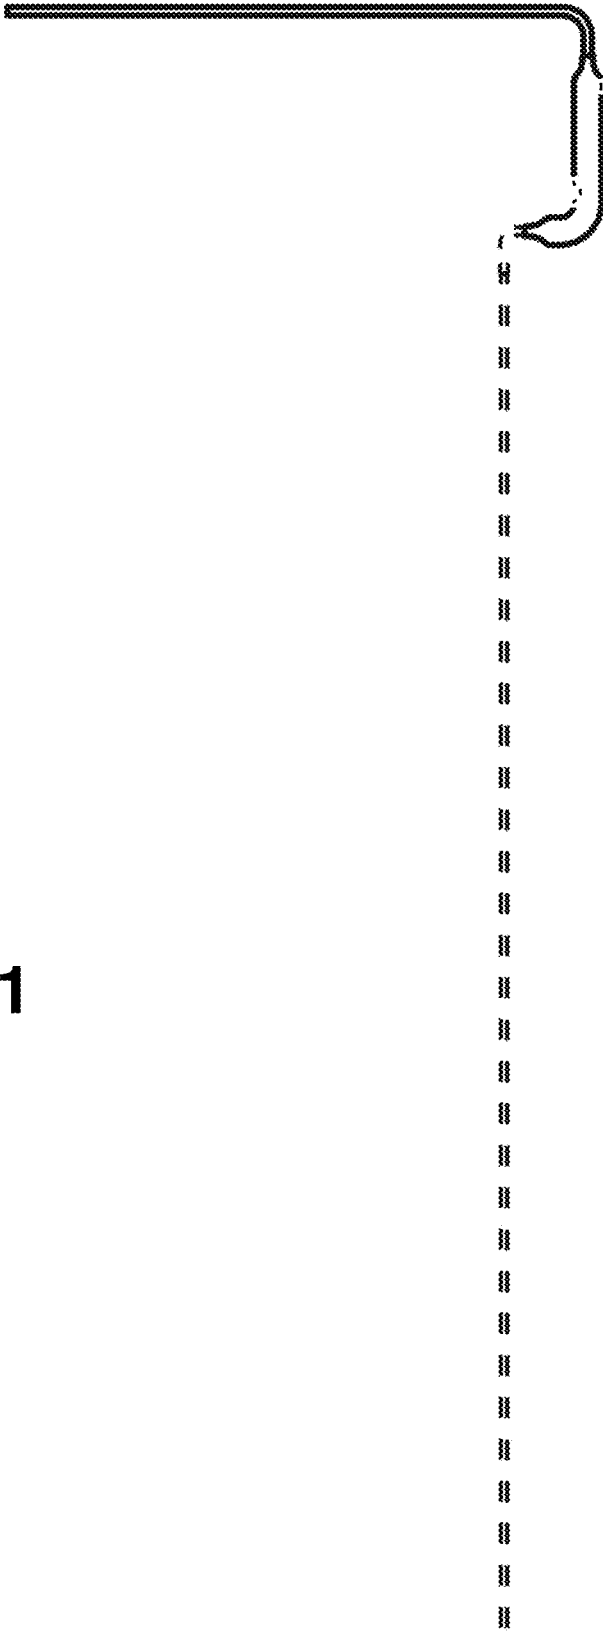


FIG. 1

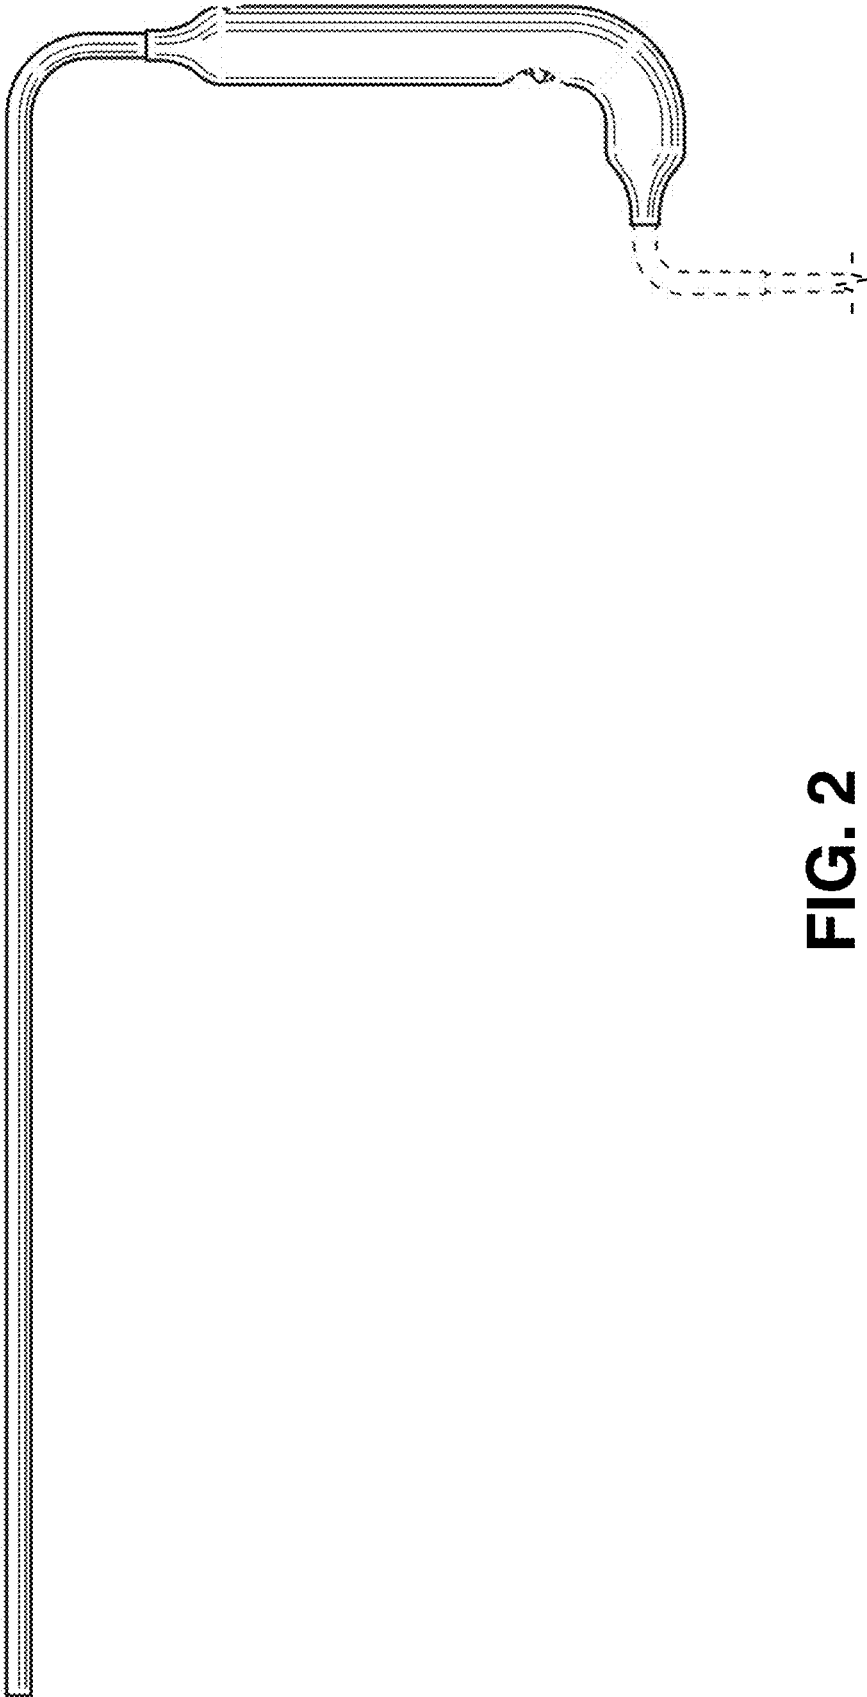


FIG. 2

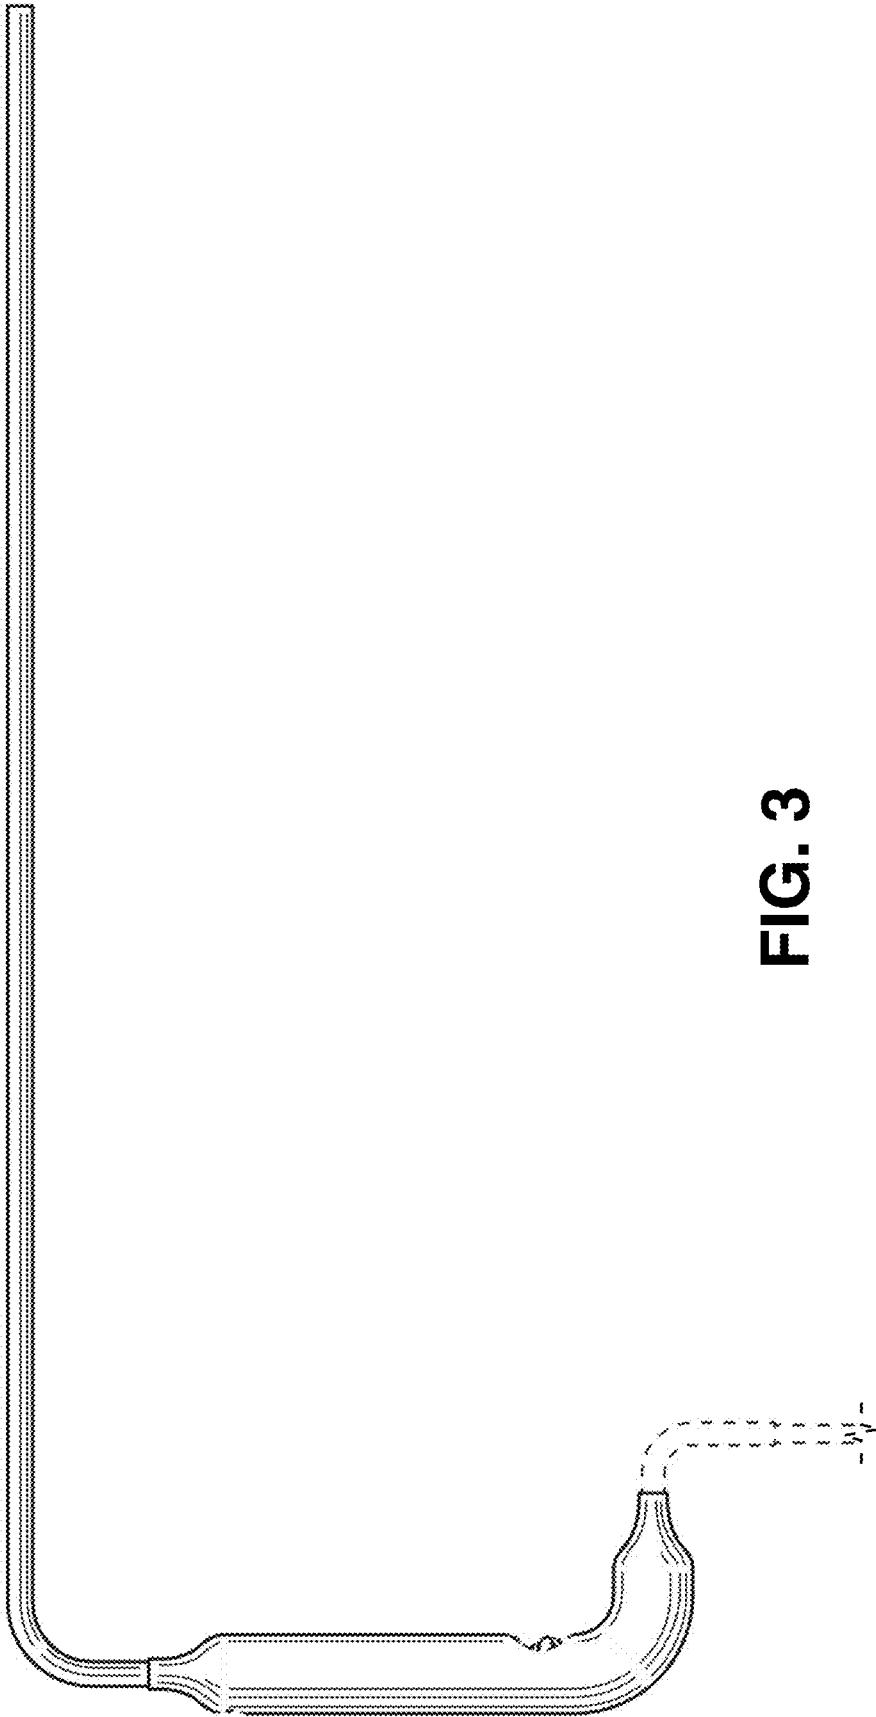


FIG. 3




FIG. 4




FIG. 5

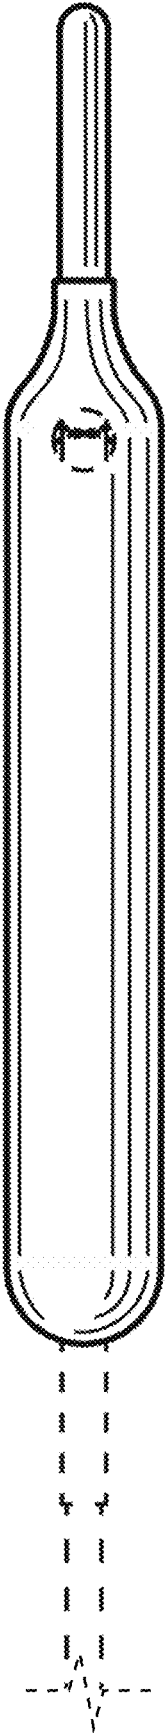


FIG. 6

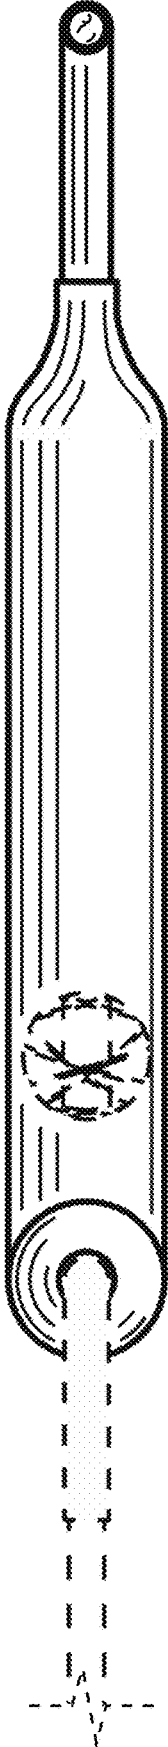


FIG. 7

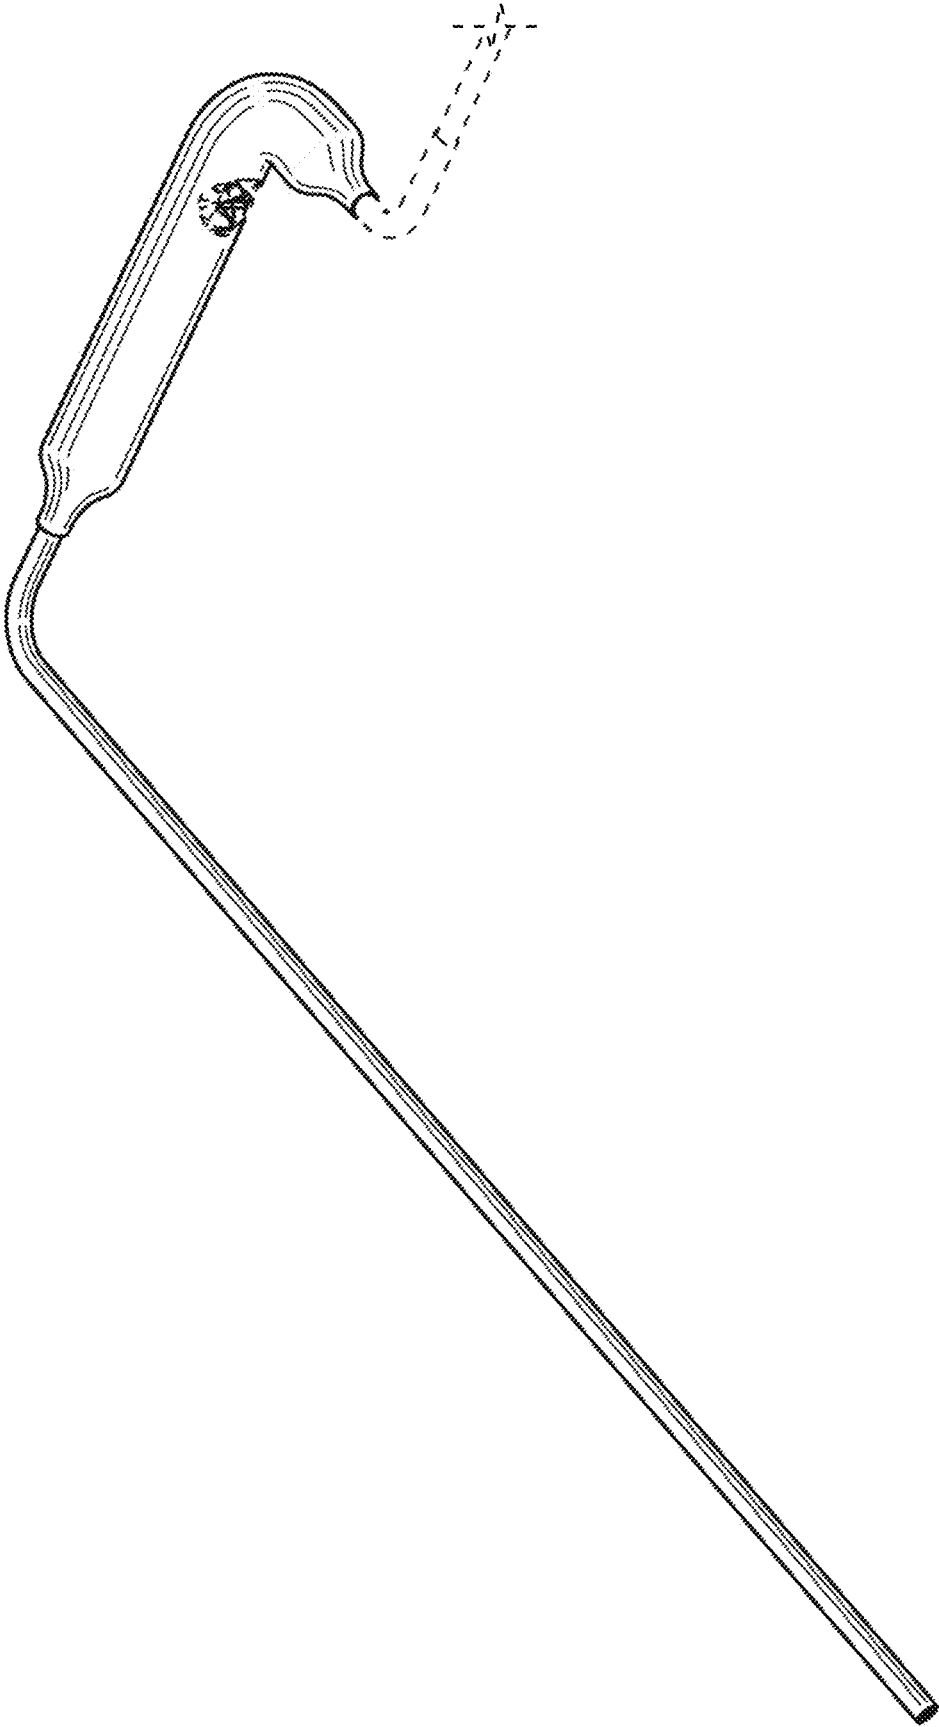


FIG. 8