




US 20170136158A1

(19) **United States**(12) **Patent Application Publication**
Culhane et al.(10) **Pub. No.: US 2017/0136158 A1**(43) **Pub. Date: May 18, 2017**(54) **SYSTEMS AND METHODS FOR REMOVING
UNDESIRABLE MATERIAL WITHIN A
CIRCULATORY SYSTEM**(71) Applicant: **ANGIODYNAMICS, INC.**, Latham,
NY (US)(72) Inventors: **Jim Culhane**, Westborough, MA (US);
Kevin Swift, Brighton, MA (US);
Rebecca Gagnon, Uxbridge, MA (US)(73) Assignee: **ANGIODYNAMICS, INC.**, Latham,
NY (US)(21) Appl. No.: **15/295,529**(22) Filed: **Oct. 17, 2016****Related U.S. Application Data**(60) Provisional application No. 62/242,493, filed on Oct.
16, 2015.**Publication Classification**(51) **Int. Cl.****A61M 1/00** (2006.01)**A61M 25/10** (2006.01)**A61M 1/36** (2006.01)(52) **U.S. Cl.**CPC **A61M 1/0056** (2013.01); **A61M 1/0066**
(2013.01); **A61M 1/008** (2013.01); **A61M**
1/3638 (2014.02); **A61M 1/3643** (2013.01);
A61M 1/3659 (2014.02); **A61M 25/10**
(2013.01); **A61M 2205/0266** (2013.01); **A61M**
2205/32 (2013.01)

(57)

ABSTRACT

The present invention relates generally to improved systems and methods for removing undesirable material residing in vessels. More specifically, the present invention relates to systems and methods for using at least one cannula to remove to remove substantially en bloc, from a site of obstruction or interest, undesirable material without fragmentation and without excessive fluid loss.

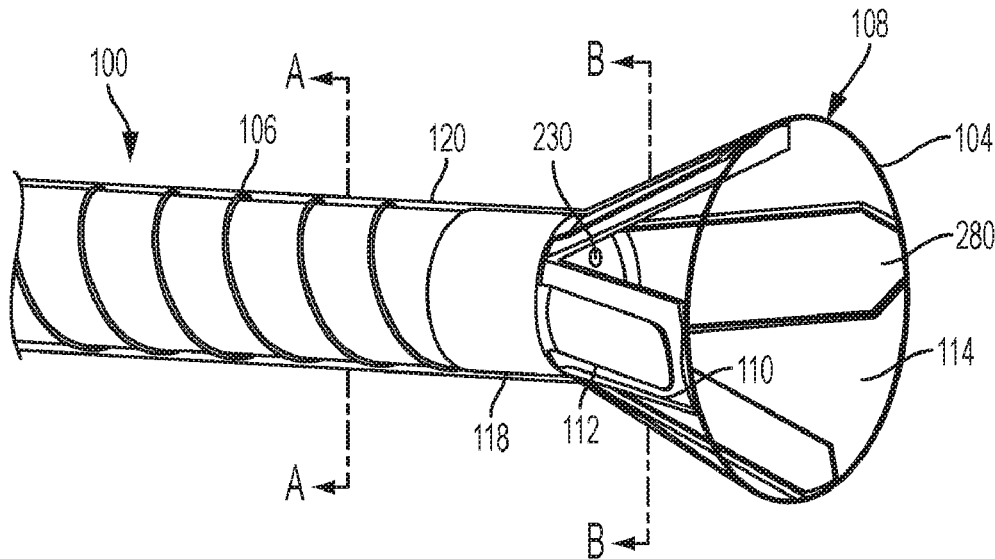

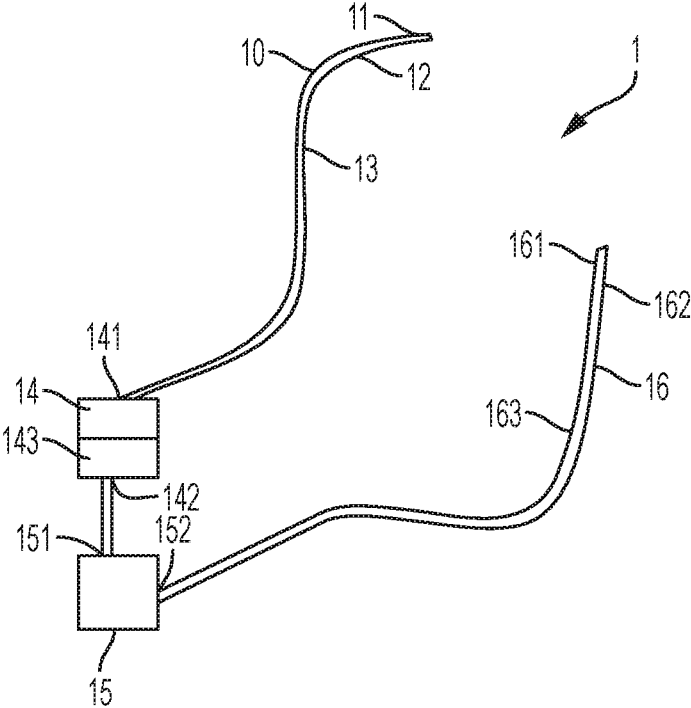


FIG. 1

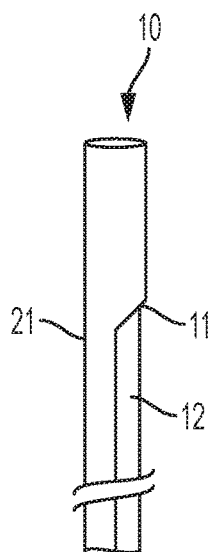


FIG. 2A

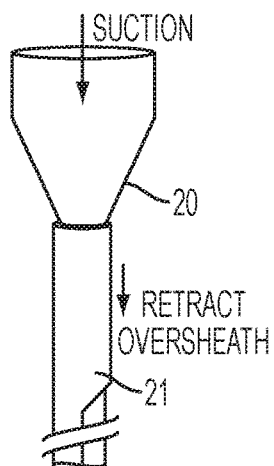


FIG. 2B

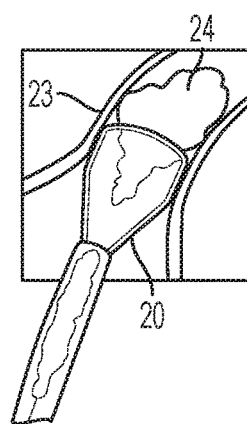


FIG. 2C

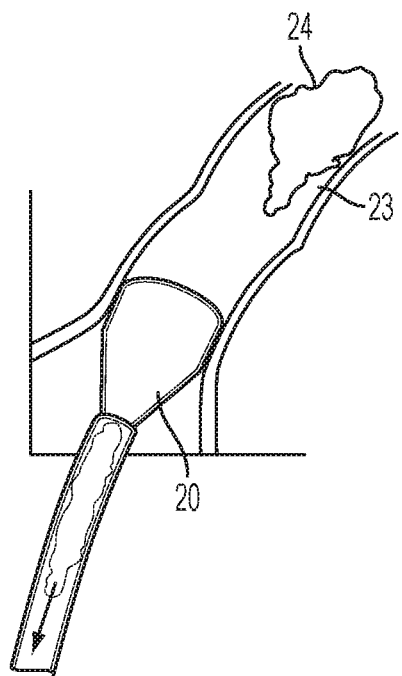


FIG. 2D

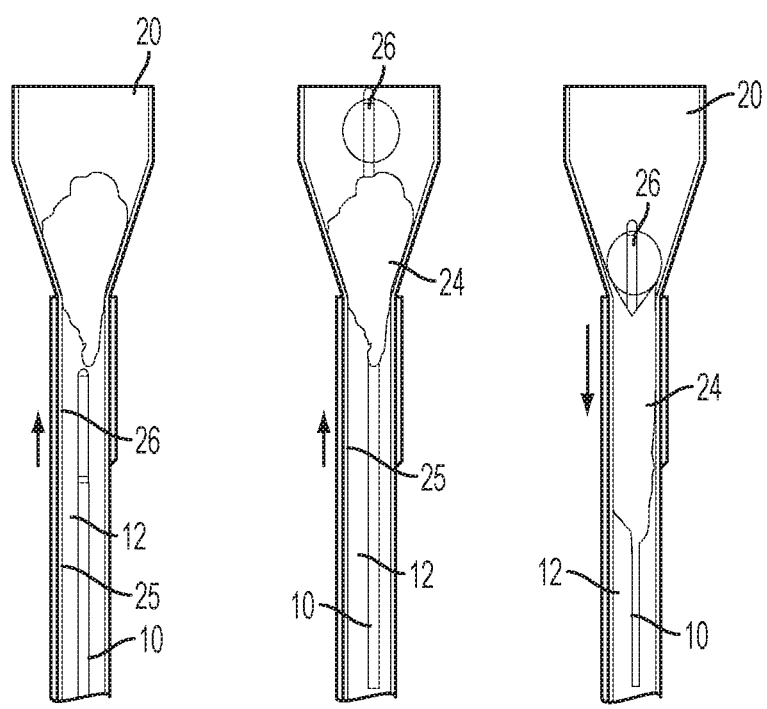


FIG. 2E FIG. 2F FIG. 2G

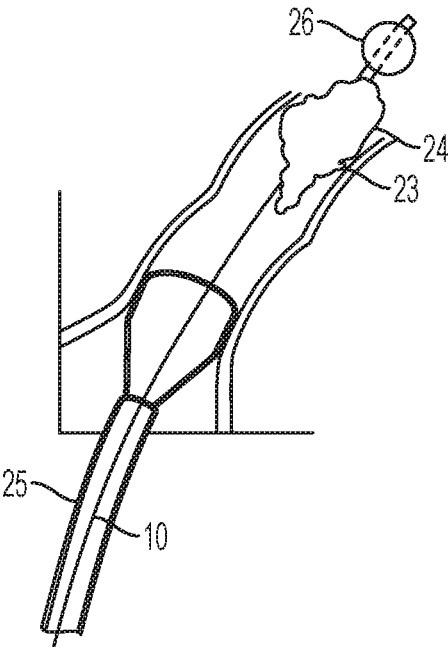


FIG. 2H

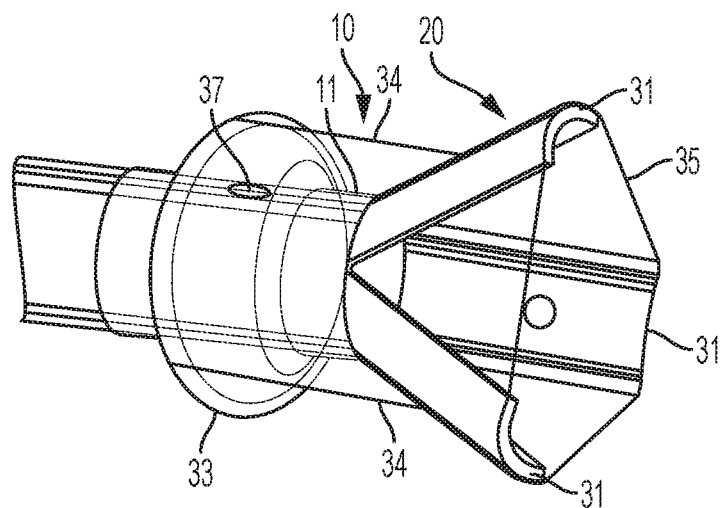


FIG. 3A

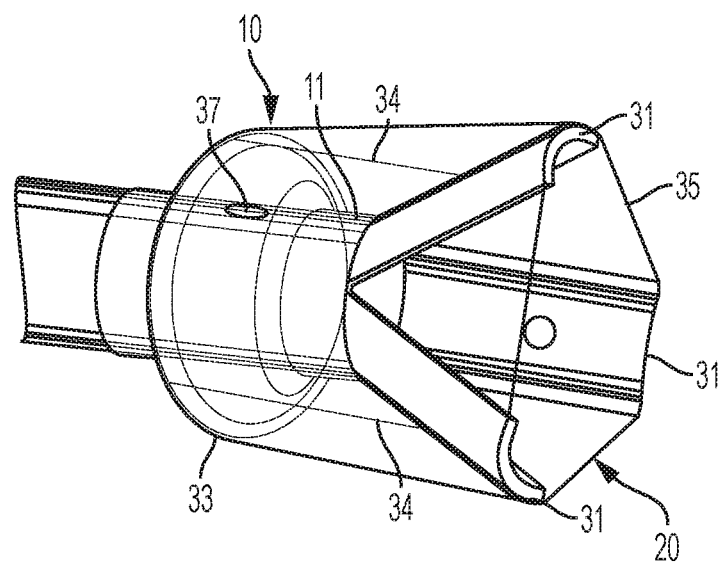


FIG. 3B

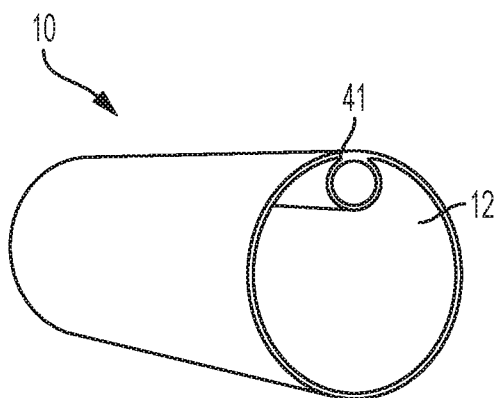


FIG. 4A

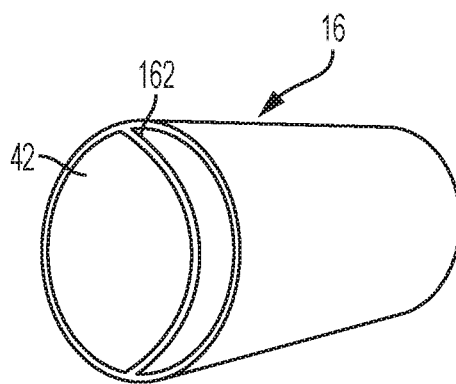


FIG. 4B

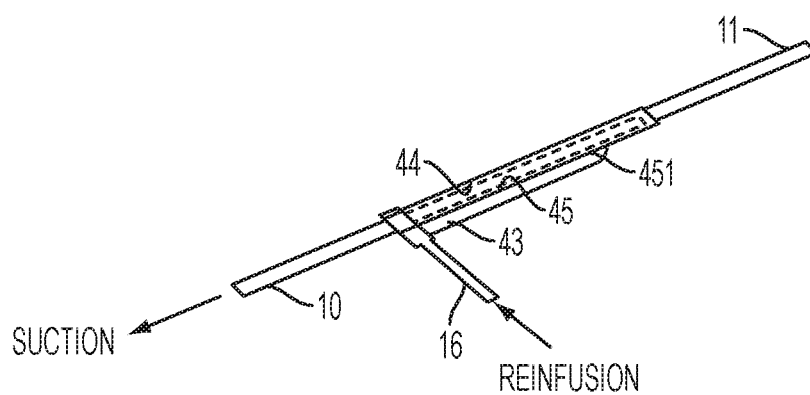


FIG. 4C

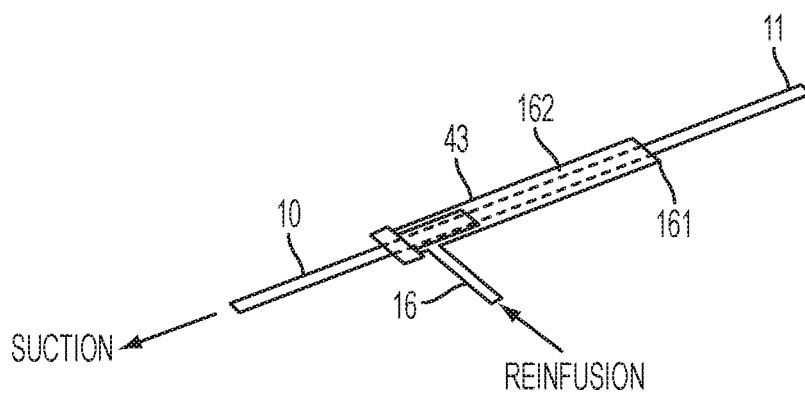


FIG. 4D

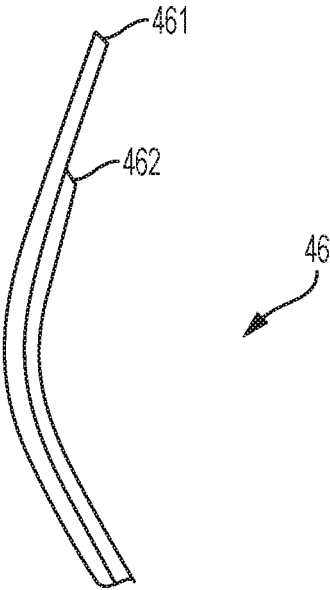


FIG. 4E

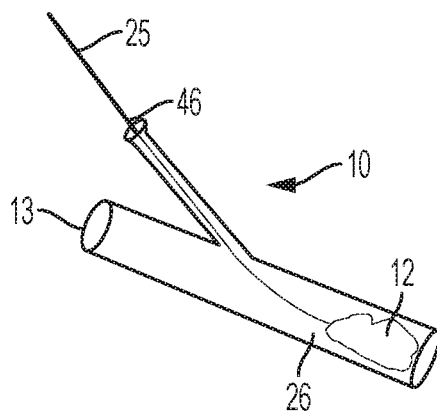


FIG. 5

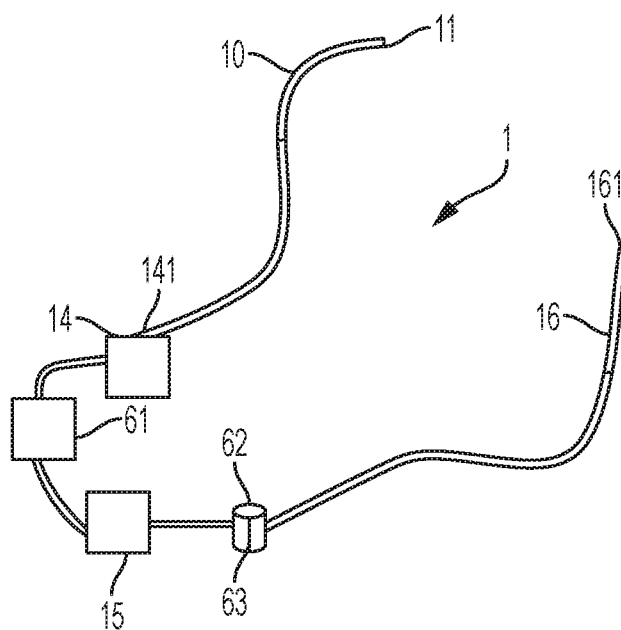


FIG. 6

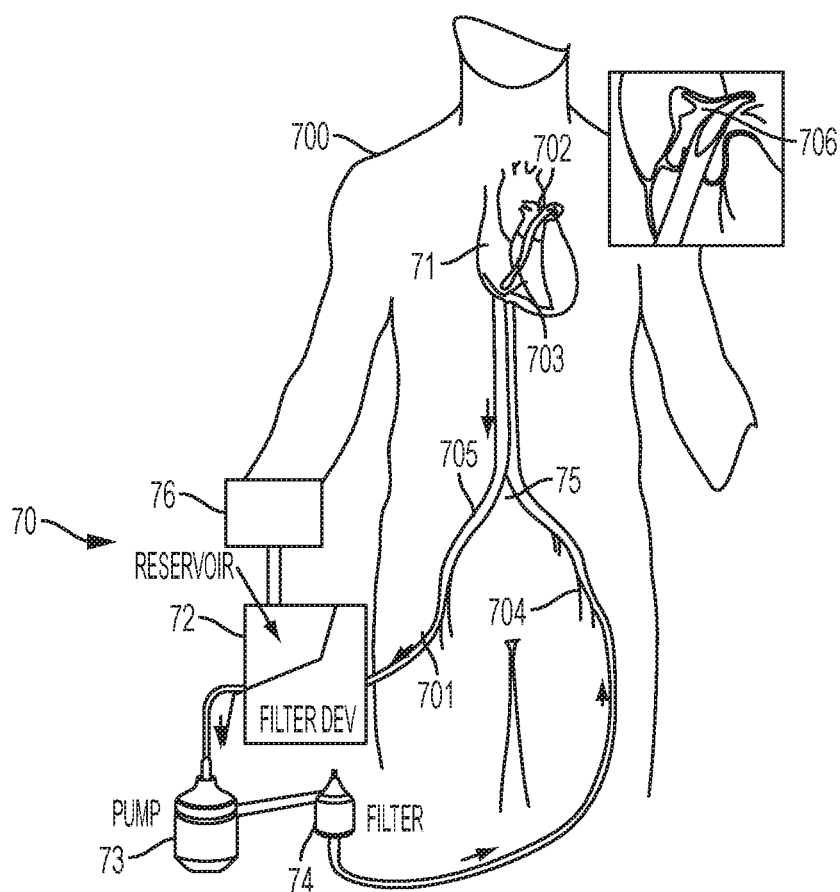


FIG. 7

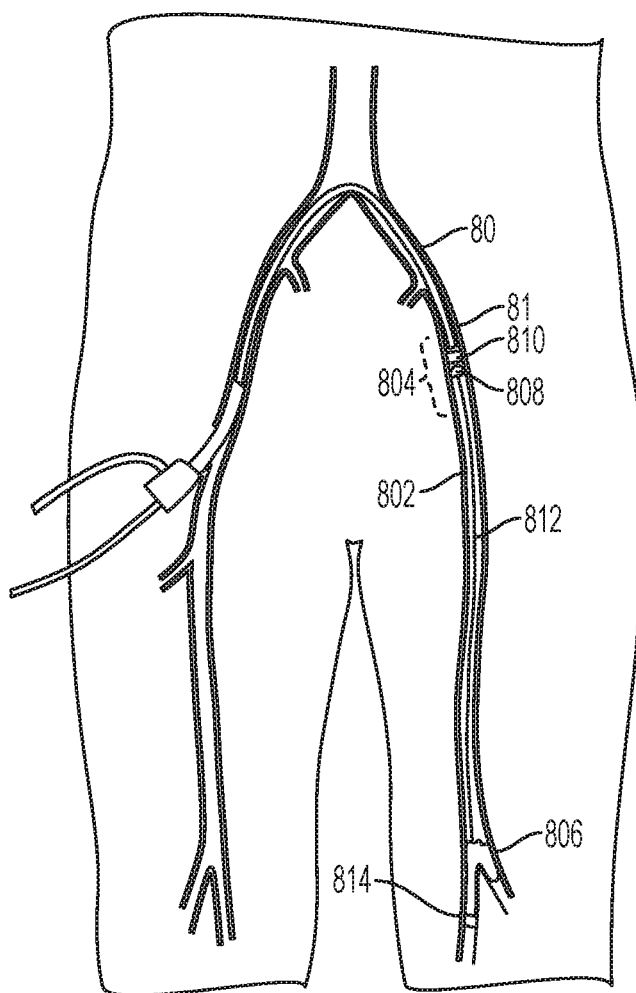


FIG. 8

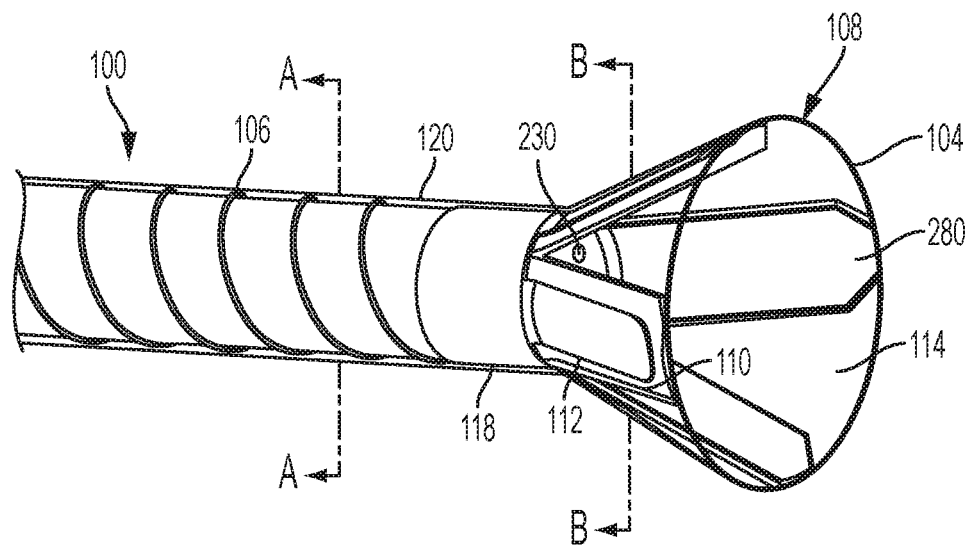


FIG. 9A

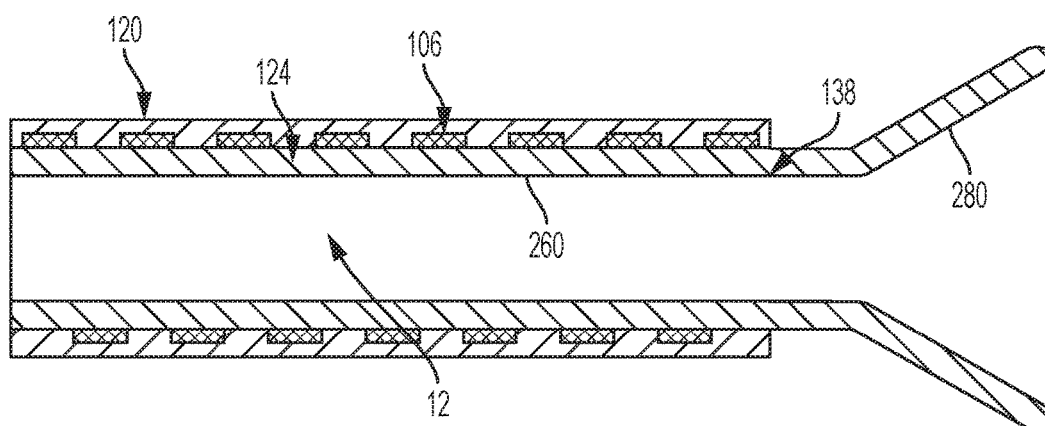


FIG. 9B

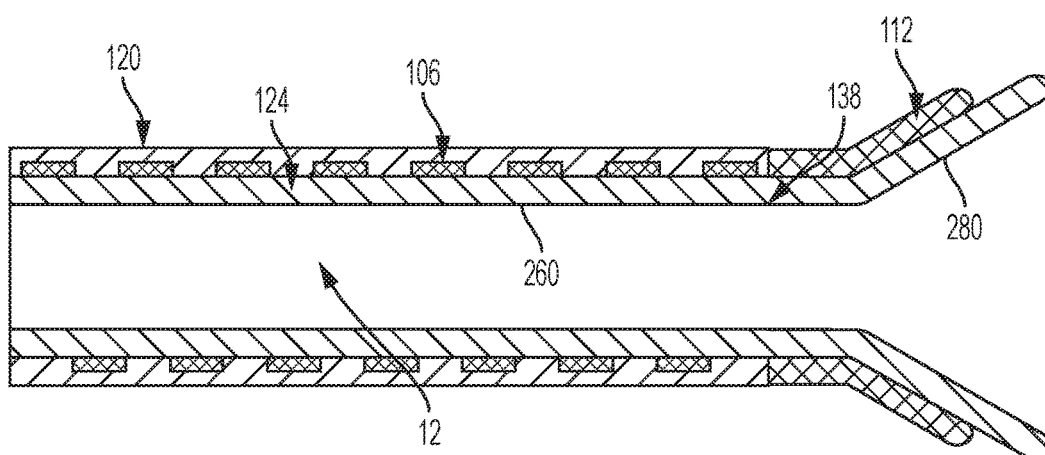


FIG. 9C

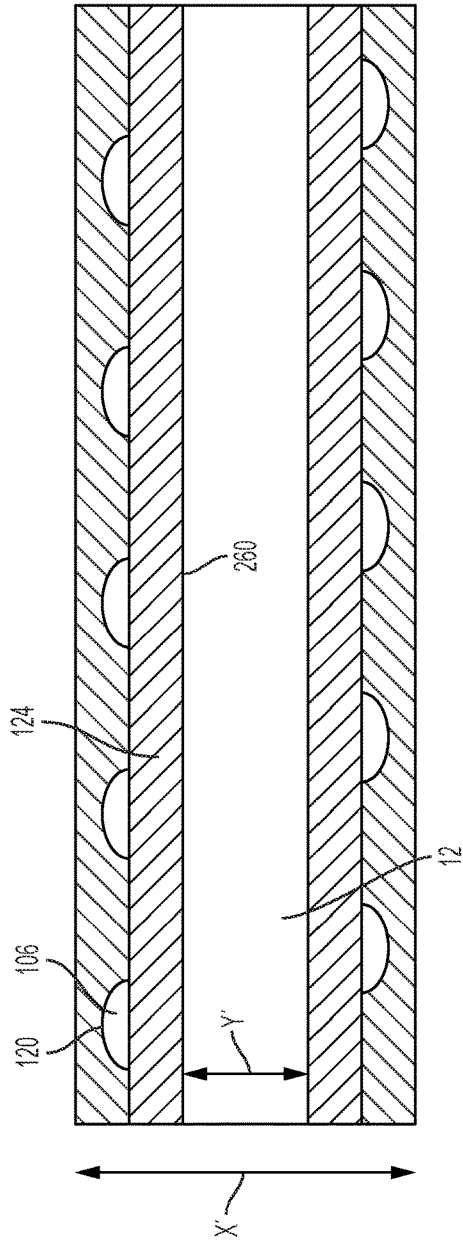


FIG. 9D

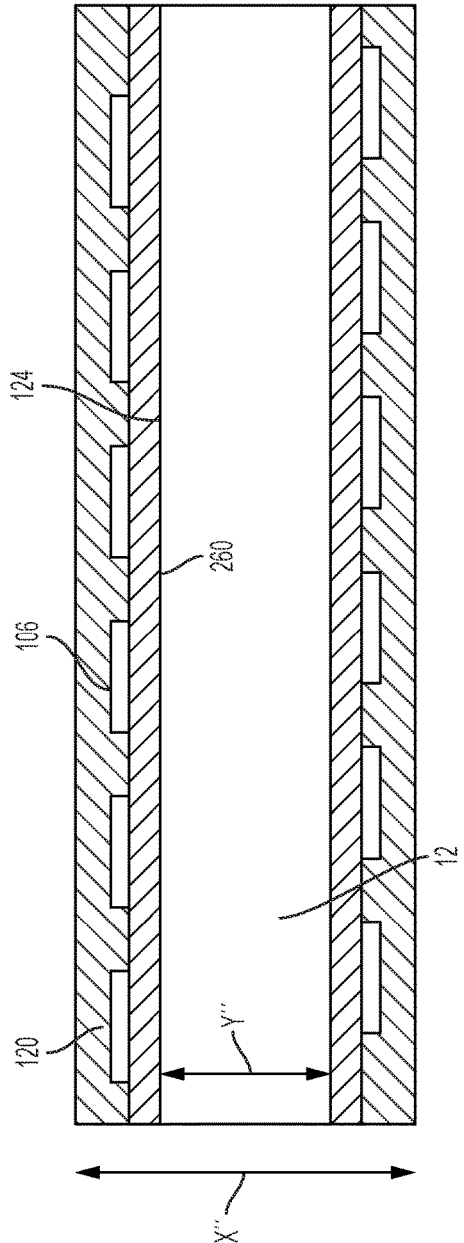


FIG. 9E

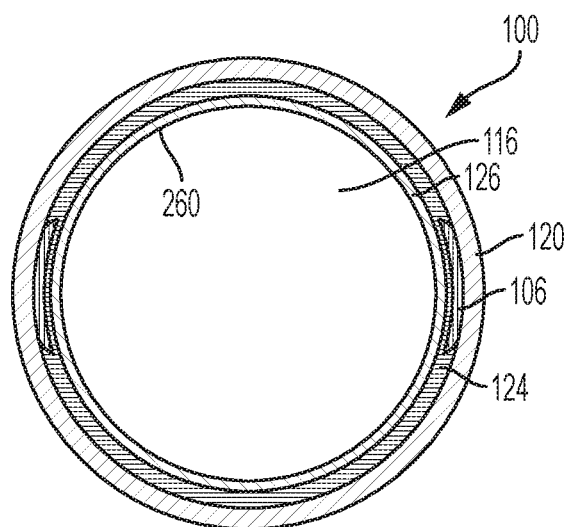


FIG. 9A-A

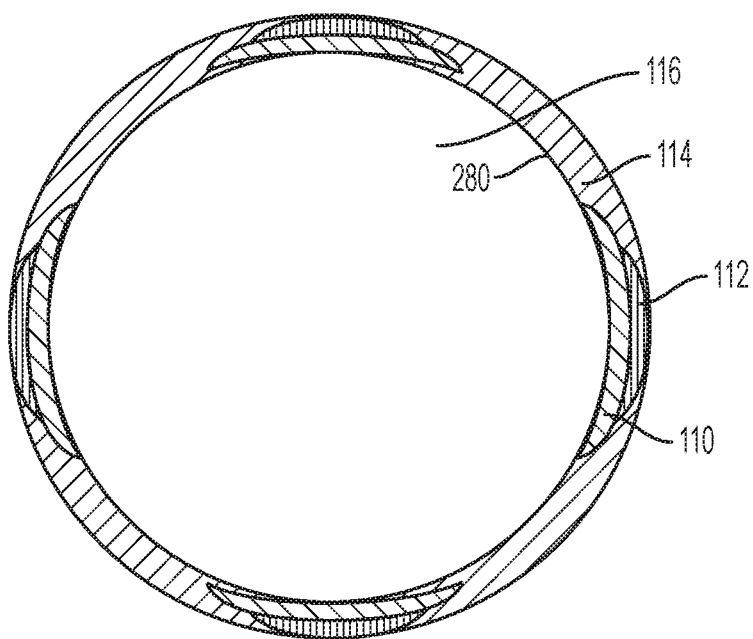


FIG. 9B-B

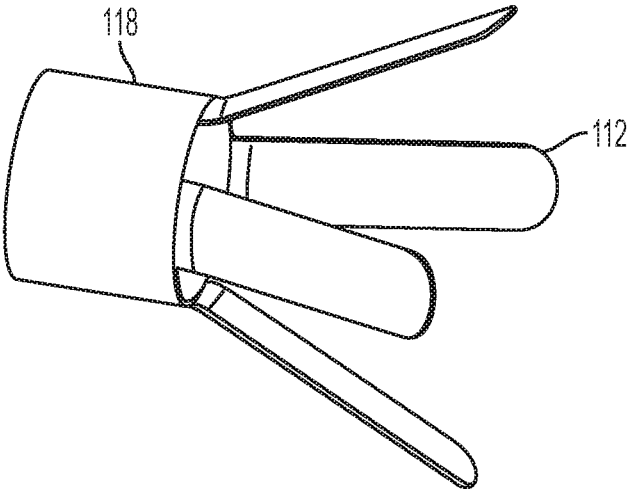


FIG. 10

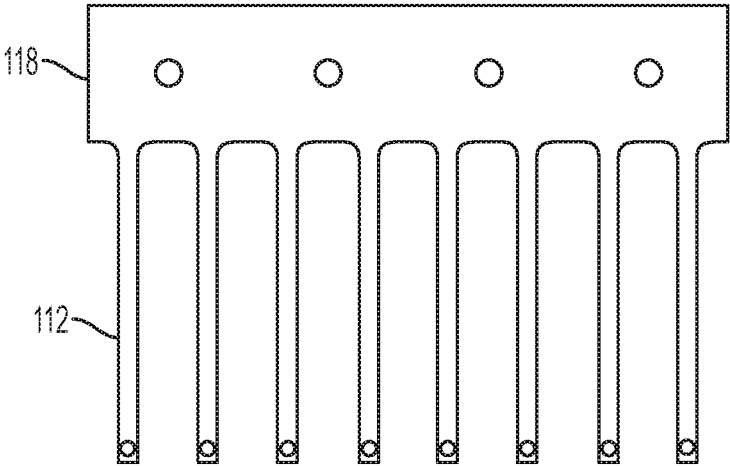


FIG. 10A

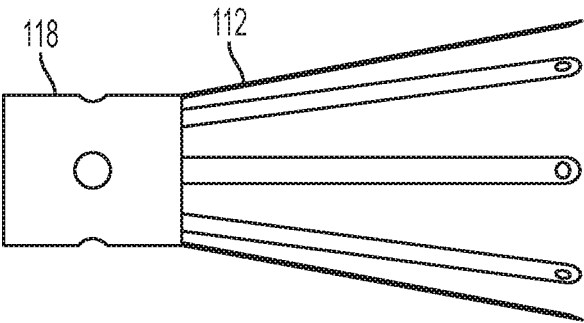


FIG. 10B

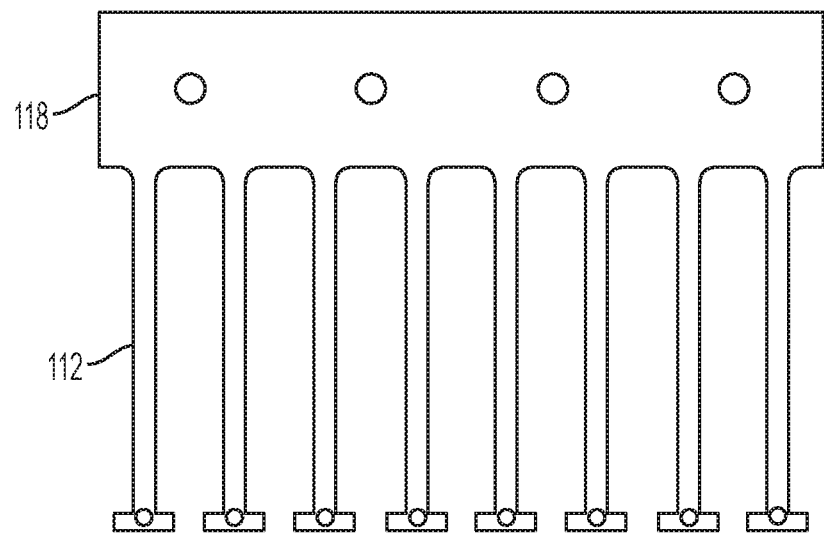


FIG. 10C

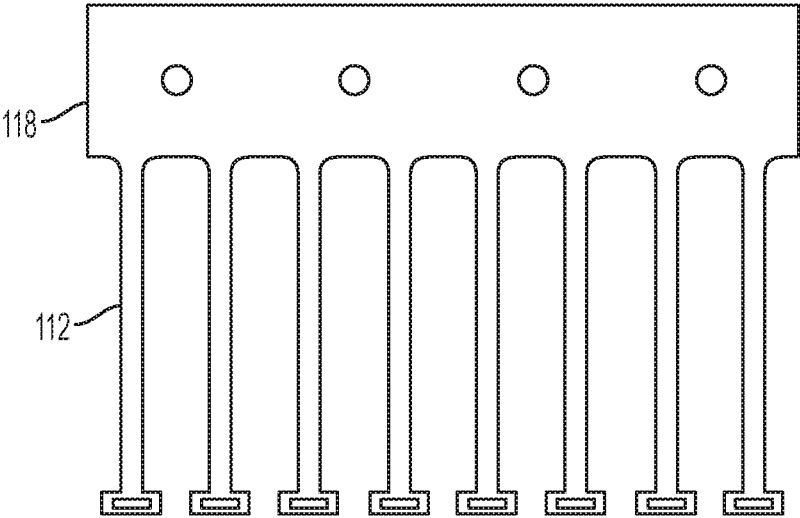


FIG. 10D

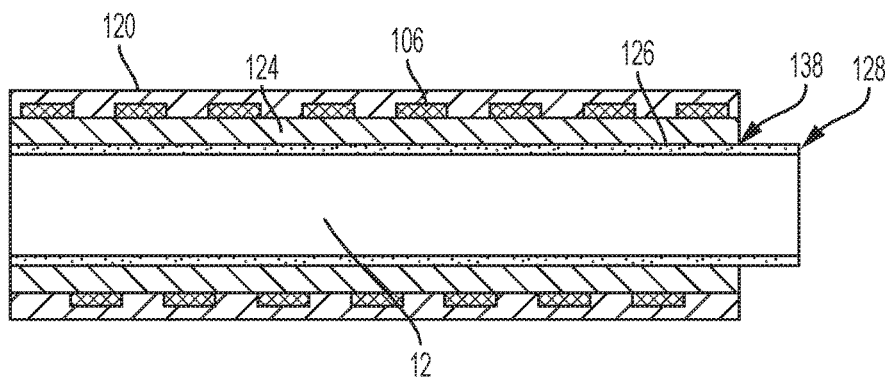


FIG. 11A

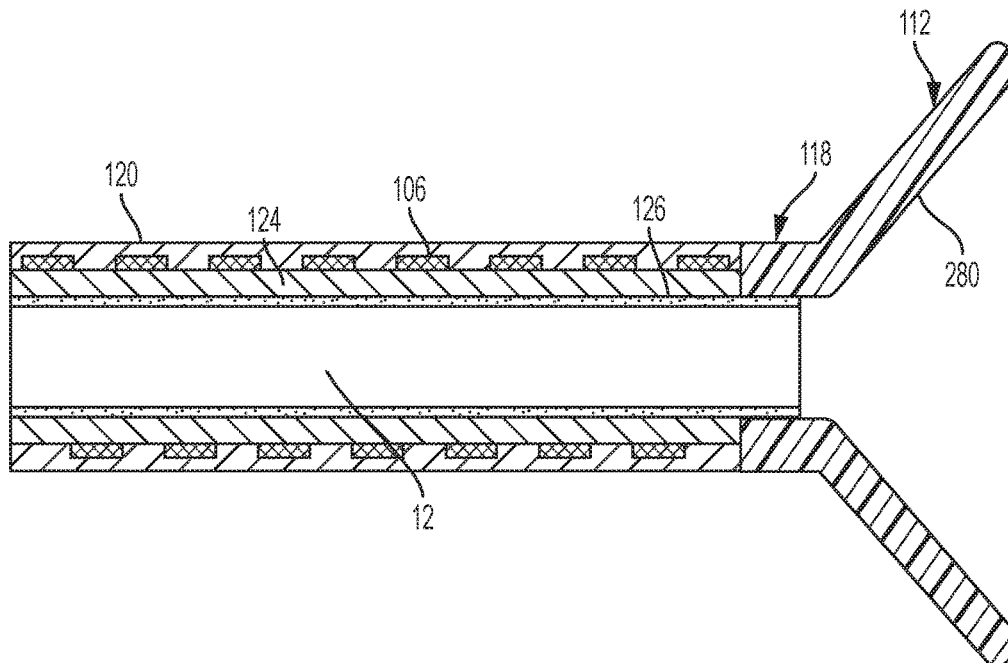


FIG. 11B

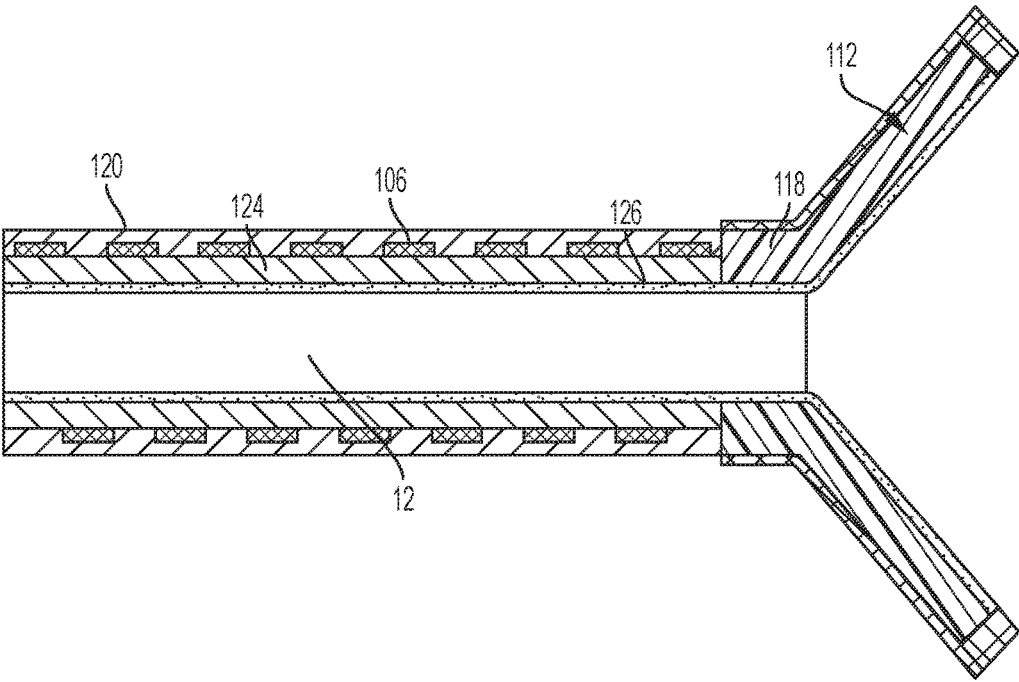


FIG. 11C

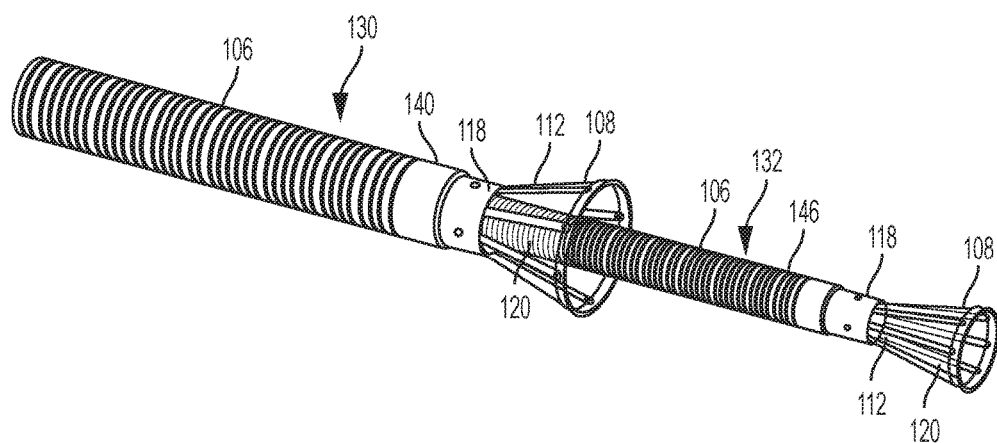


FIG. 12

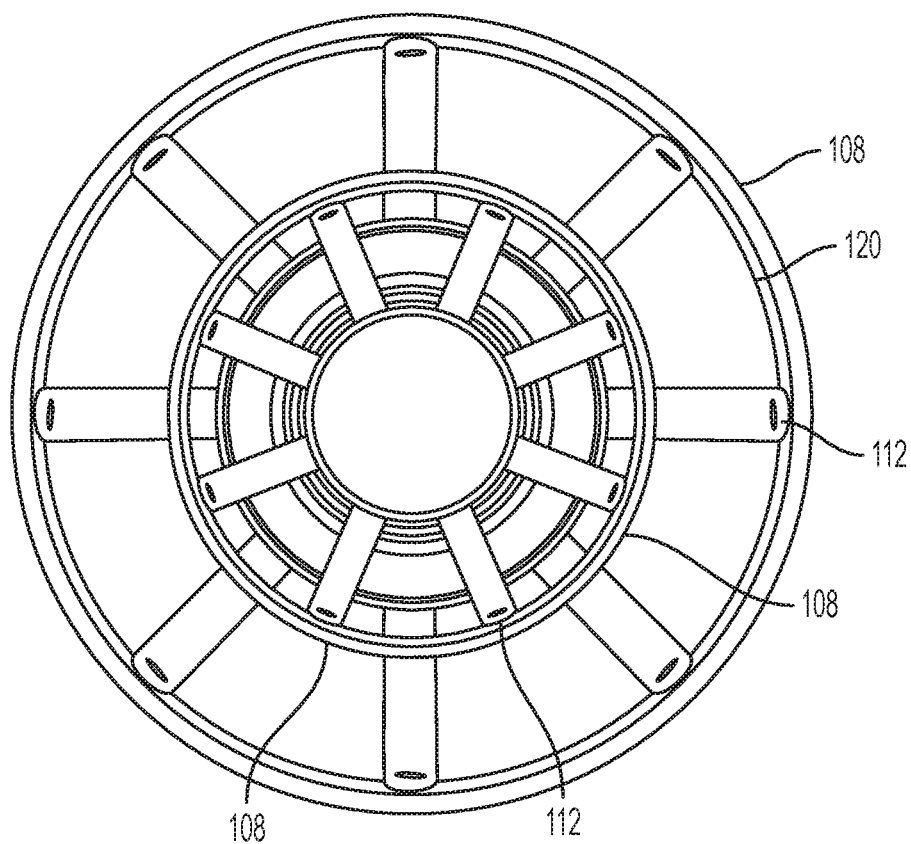


FIG. 13

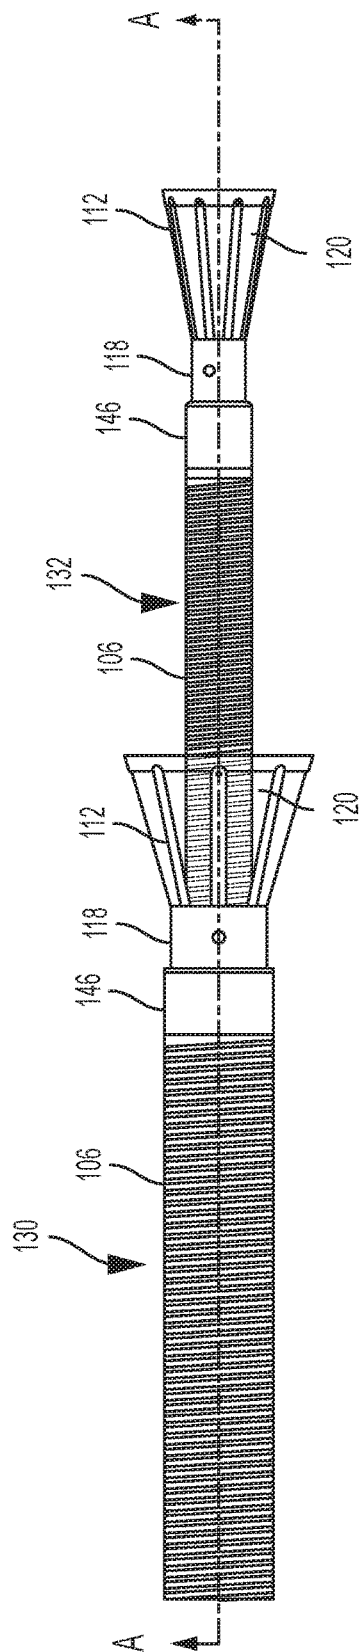


FIG. 14

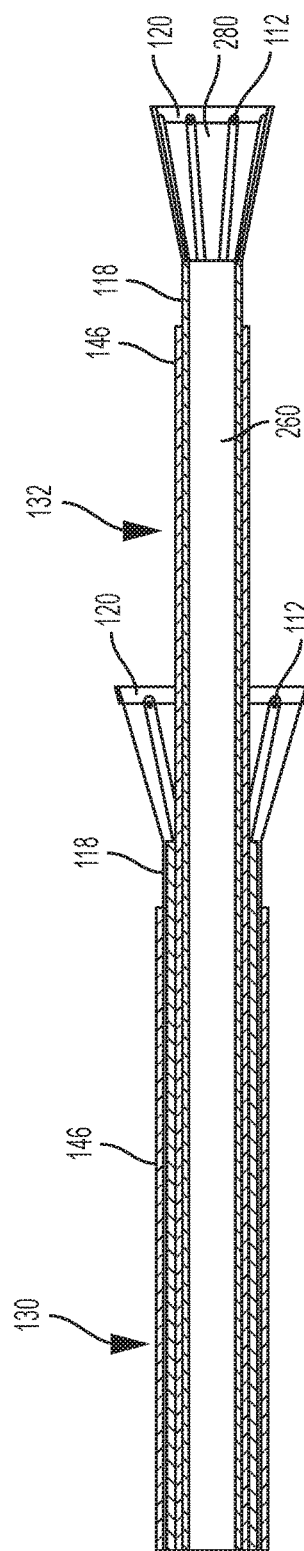


FIG. 14A-A

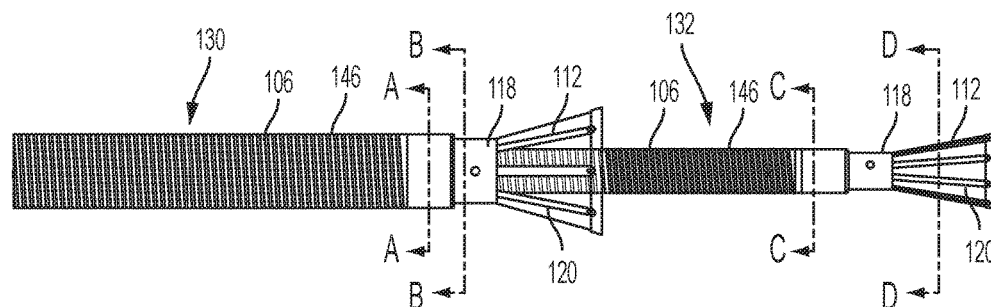


FIG. 15

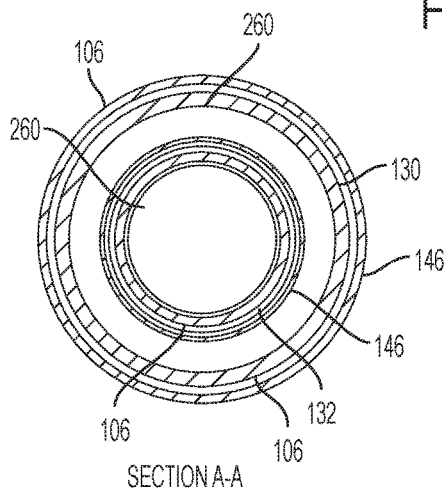


FIG. 15A-A

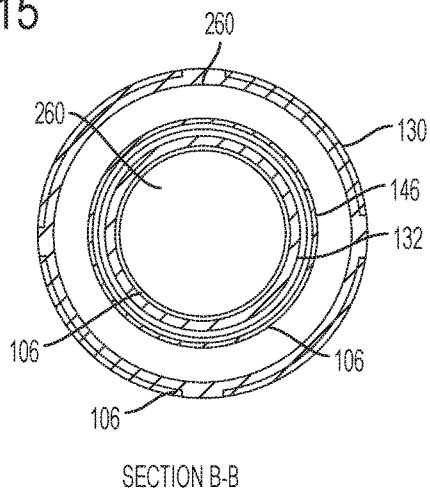


FIG. 15B-B

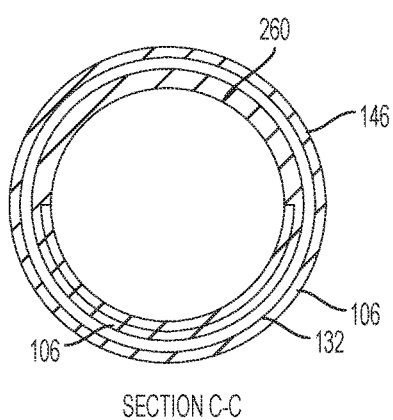


FIG. 15C-C

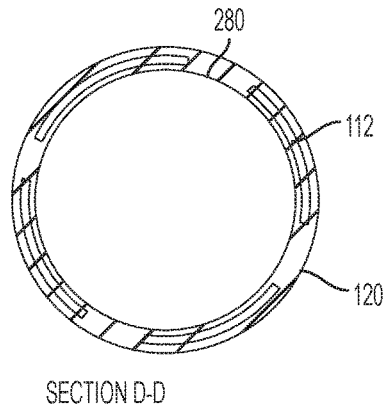


FIG. 15D-D

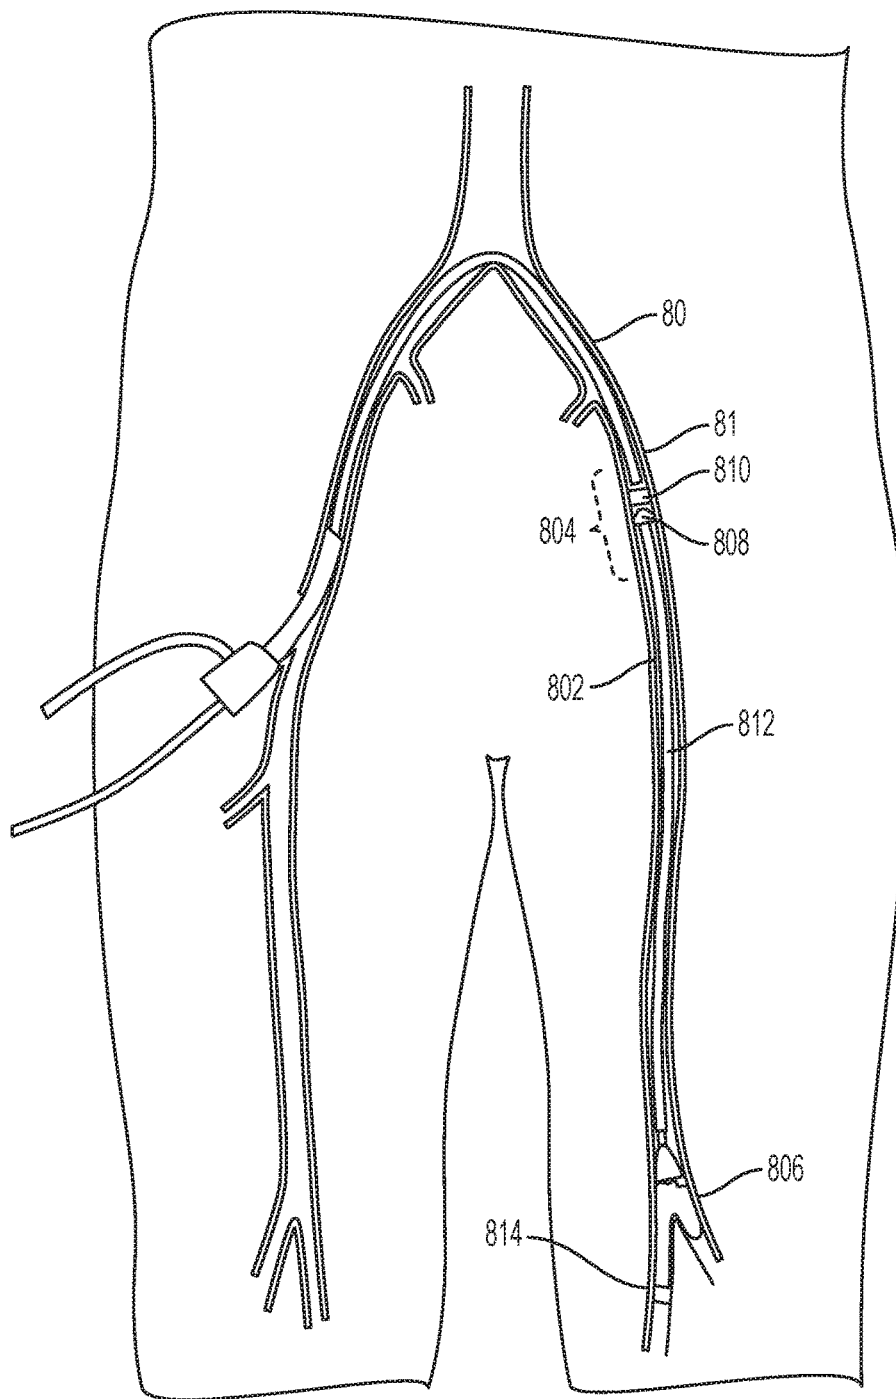


FIG. 16

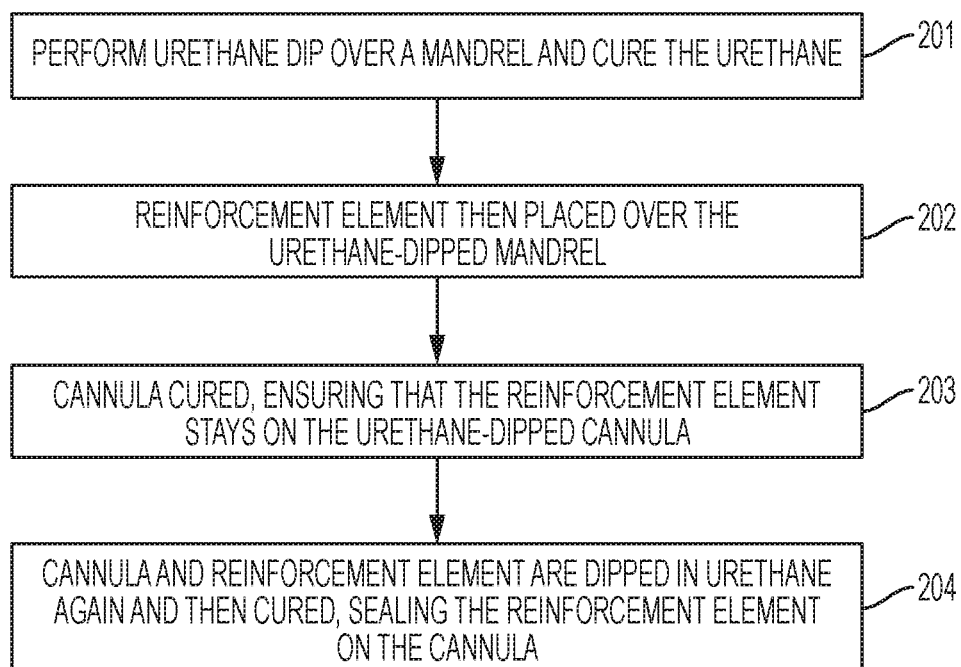


FIG. 17

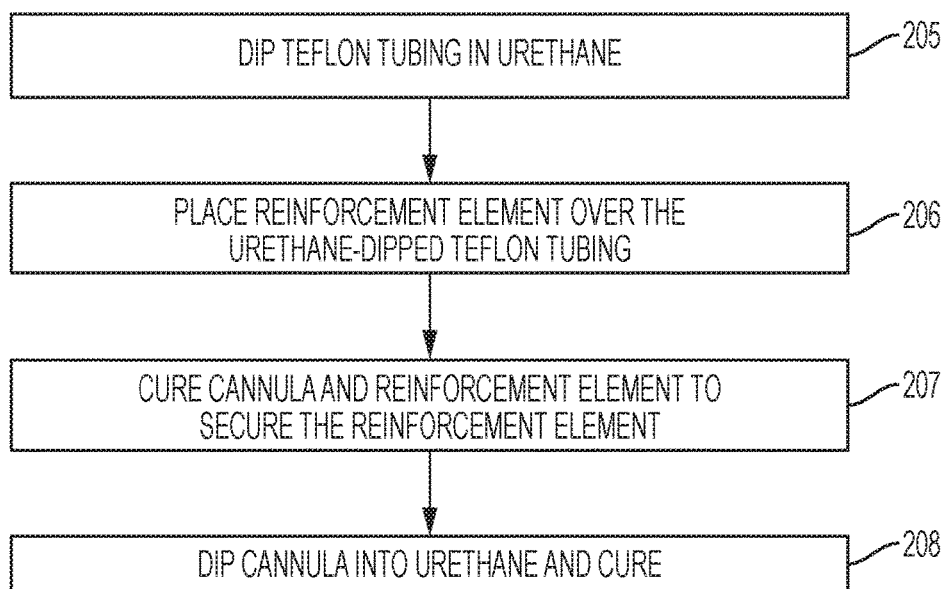


FIG. 18

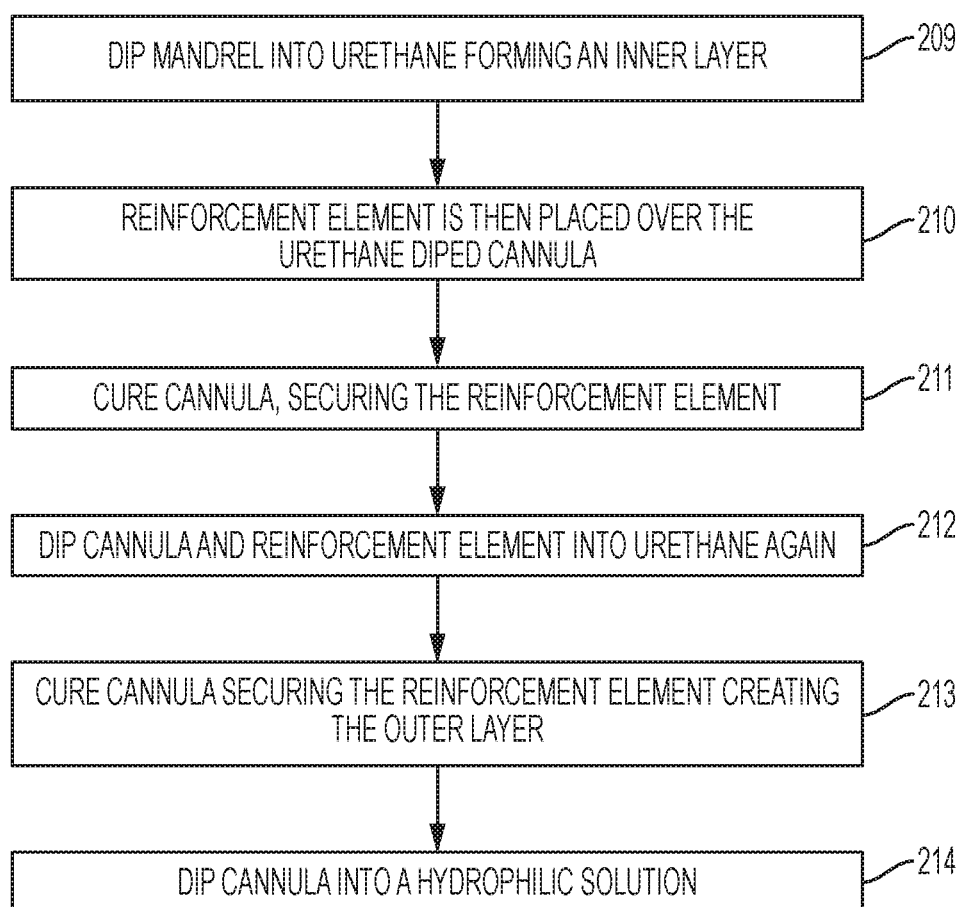


FIG. 19

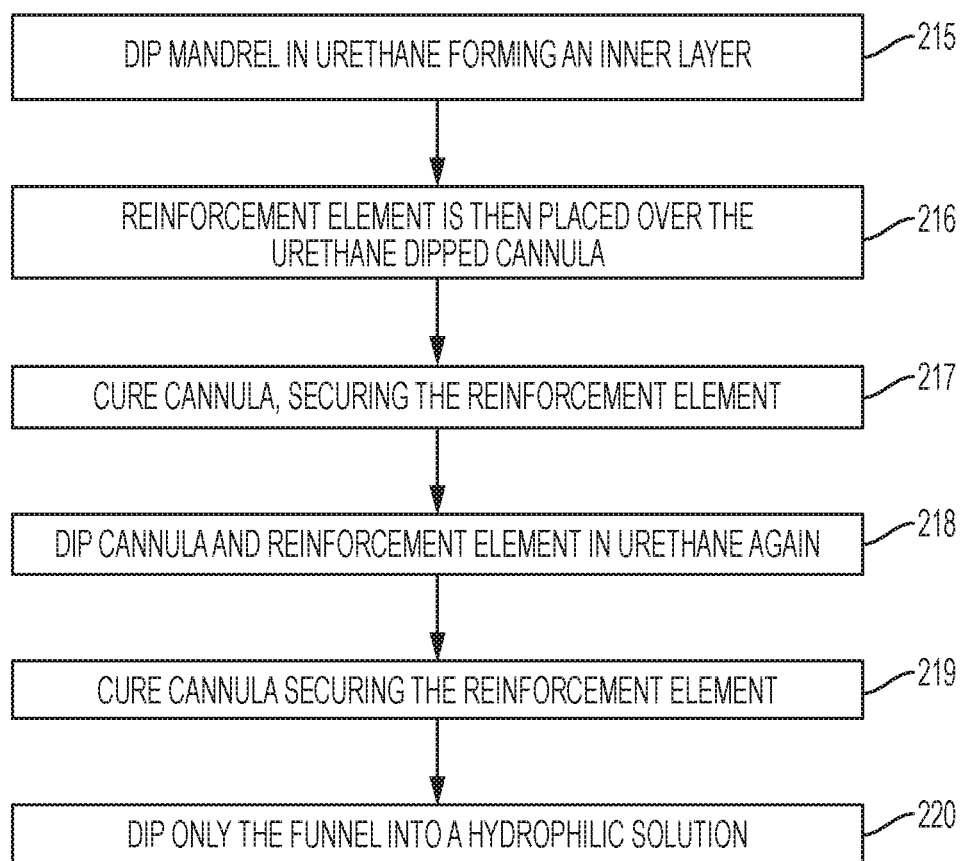


FIG. 20

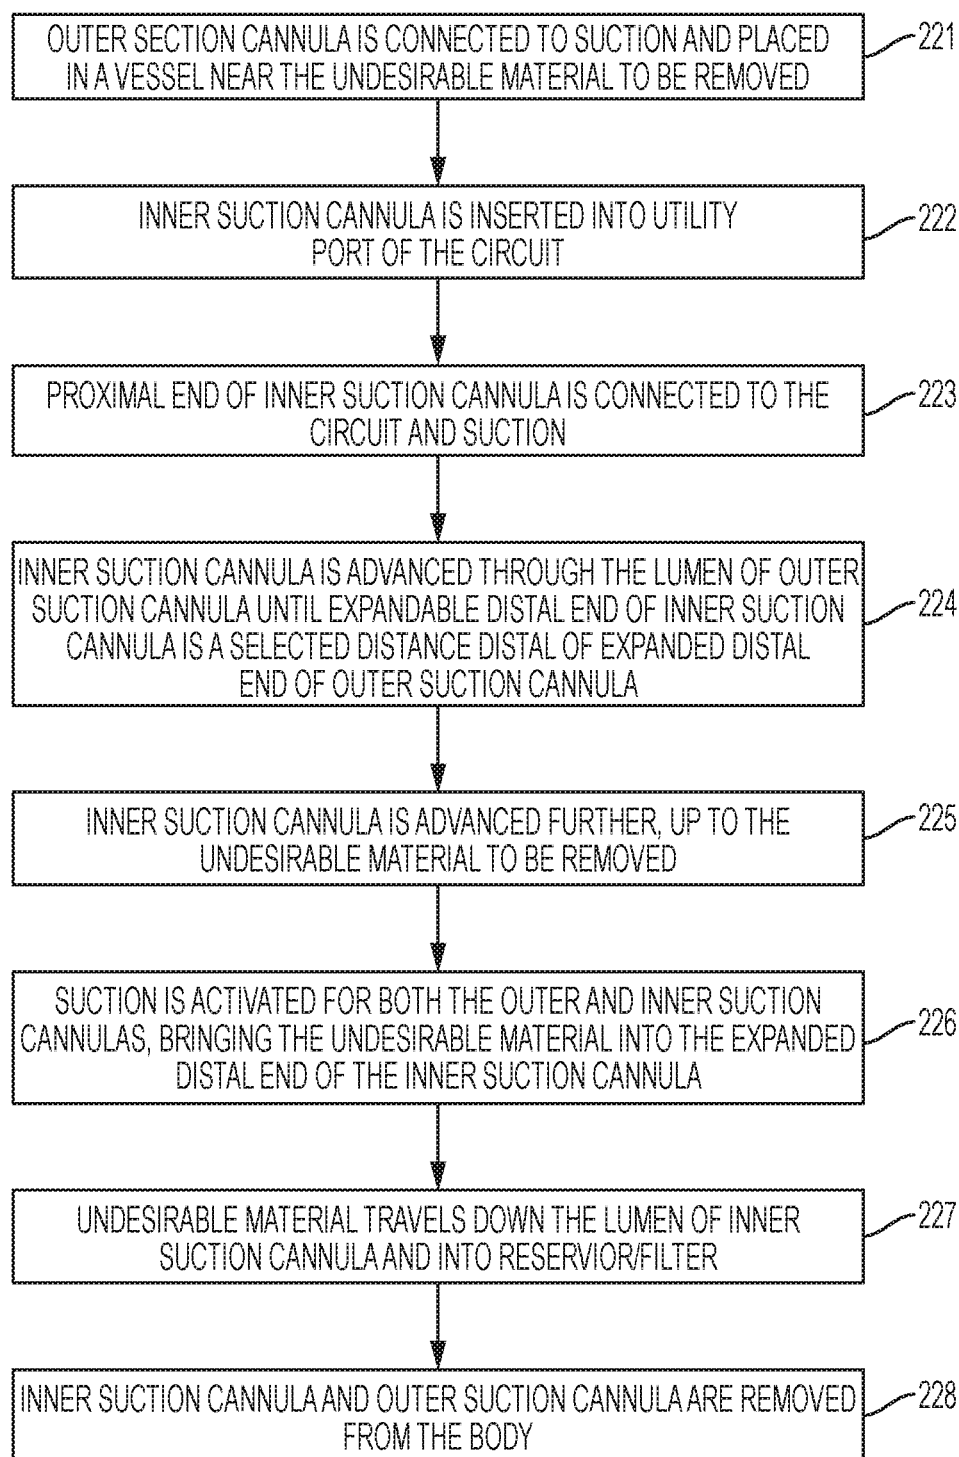


FIG. 21

SYSTEMS AND METHODS FOR REMOVING UNDESIRABLE MATERIAL WITHIN A CIRCULATORY SYSTEM

RELATED U.S. APPLICATION(S)

[0001] This application claims the benefit of U.S. Provisional Application 62/242,493, filed Oct. 16, 2015, which is hereby incorporated herein by reference.

TECHNICAL FIELD

[0002] The present invention relates to systems and methods for removing undesirable materials from a site of interest within the circulatory system. More particularly, the present invention relates to systems and methods for removing substantially en bloc clots, thrombi, and emboli, among others, from within heart chambers, as well as medium to large vessels, while reinfusing fluid removed from the site of interest back into the patient to minimize fluid loss.

BACKGROUND ART

[0003] Many of the most common and deadly diseases afflicting mankind result from or in the presence of undesirable material, most notably blood clots, in the blood vessels and heart chambers. Examples of such diseases include myocardial infarction, stroke, pulmonary embolism, deep venous thrombosis, atrial fibrillation, infective endocarditis, etc. The treatment of some of these conditions, which involve smaller blood vessels, such as myocardial infarction and stroke, has been dramatically improved in recent years by targeted mechanical efforts to remove blood clots from the circulatory system. Other deadly conditions, which involve medium to large blood vessels or heart chambers, such as pulmonary embolism (½ million deaths per year) or deep venous thrombosis (2-3 million cases per year) have not benefited significantly from such an approach. Present treatment for such conditions with drugs or other interventions is not sufficiently effective. As a result, additional measures are needed to help save lives of patients suffering from these conditions.

[0004] The circulatory system can be disrupted by the presence of undesirable material, most commonly blood clots, but also tumor, infective vegetations, and foreign bodies, etc. Blood clots can arise spontaneously within the blood vessel or heart chamber (thrombosis) or be carried through the circulation from a remote site and lodge in a blood vessel (thromboemboli).

[0005] In the systemic circulation, this undesirable material can cause harm by obstructing a systemic artery or vein. Obstructing a systemic artery interferes with the delivery of oxygen-rich blood to organs and tissues (arterial ischemia) and can ultimately lead to tissue death or infarction. Obstructing a systemic vein interferes with the drainage of oxygen-poor blood and fluid from organs and tissues (venous congestion) resulting in swelling (edema) and can occasionally lead to tissue infarction.

[0006] Many of the most common and deadly human diseases are caused by systemic arterial obstruction. The most common form of heart disease, such as myocardial infarction, results from thrombosis of a coronary artery following disruption of a cholesterol plaque. The most common causes of stroke include obstruction of a cerebral artery either from local thrombosis or thromboemboli, typically from the heart. Obstruction of the arteries to abdominal

organs by thrombosis or thromboemboli can result in catastrophic organ injury, most commonly infarction of the small and large intestine. Obstruction of the arteries to the extremities by thrombosis or thromboemboli can result in gangrene.

[0007] In the systemic venous circulation, undesirable material can also cause serious harm. Blood clots can develop in the large veins of the legs and pelvis, a common condition known as deep venous thrombosis (DVT). DVT arises most commonly when there is a propensity for stagnated blood (long-haul air travel, immobility) and clotting (cancer, recent surgery, especially orthopedic surgery). DVT causes harm by (1) obstructing drainage of venous blood from the legs leading to swelling, ulcers, pain and infection and (2) serving as a reservoir for blood clot to travel to other parts of the body including the heart, lungs (pulmonary embolism) and across a opening between the chambers of the heart (patent foramen ovale) to the brain (stroke), abdominal organs or extremities.

[0008] In the pulmonary circulation, the undesirable material can cause harm by obstructing pulmonary arteries, a condition known as pulmonary embolism. If the obstruction is upstream, in the main or large branch pulmonary arteries, it can severely compromise total blood flow within the lungs and therefore the entire body, resulting in low blood pressure and shock. If the obstruction is downstream, in large to medium pulmonary artery branches, it can prevent a significant portion of the lung from participating in the exchange of gases to the blood resulting low blood oxygen and build up of blood carbon dioxide. If the obstruction is further downstream, it can cut off the blood flow to a smaller portion of the lung, resulting in death of lung tissue or pulmonary infarction.

[0009] The presence of the undesirable material within the heart chambers can cause harm by obstructing flow or by serving as a reservoir for emboli to other organs in the body. The most common site for obstruction within the heart is in the heart valves. Infective vegetations, a condition known as endocarditis, can cause partial obstruction to flow across a valve before destroying the valve. Patients with prosthetic valves, especially mechanical valves, are particularly prone to valve thrombosis and obstruction. The heart chambers are the most common source of emboli (cardioemboli) to the systemic circulation, including stroke. Emboli tend to arise from areas that are prone to stagnation of blood flow under pathologic conditions. The left atrial appendage in patients with atrial fibrillation is prone to thrombosis, as well as the left ventricular apex in patients with acute myocardial infarction or dilated cardiomyopathy. Infected vegetations or thrombi on the heart valves are also common sources of emboli. Undesirable material such as blood clots and infected vegetations can reside in the chambers of the right heart (atrium and ventricle), often associated with prosthetic material such as pacemaker leads or long-term indwelling catheters.

[0010] The most effective treatment for conditions resulting from the presence of blood clots or other undesirable materials within the circulation is, of course, to stabilize or eliminate the material before it has embolized. Alternatively, if obstruction to flow has already occurred but before the obstruction has caused permanent harm (infarction, shock, death), the material can be eliminated by utilizing biologic or mechanical means.

[0011] Biologic treatments involve the delivery of agents to the material, which either dissolve the material or, at a

minimum, stabilize it until the body can eliminate it. In the case of infective vegetations, antimicrobial agents can, over time, decrease the chances of embolization. In the case of blood clots, the agents include 1) anticoagulant agents (heparin, warfarin, etc.) which prevent propagation of blood clots; and 2) more potent thrombolytic agents (streptokinase, urokinase, tPA, etc) which actively dissolve clots. The agents are usually delivered systemically, i.e., into a peripheral or central vein and allowed to circulate throughout the body. Thrombolytic agents can also be delivered through a catheter directly to the blood clot which can increase its effectiveness by increasing local concentrations but this does not completely eliminate the absorption into systemic circulation throughout the body.

[0012] Thrombolytic agents have been shown to increase survival in patients with hemodynamically significant pulmonary embolism as documented by echocardiographic evidence of right ventricular strain. The use of thrombolytic agents is the standard of care in this subgroup of patients with a high 20-25% early mortality. They are commonly used in to dissolve clots in other blood vessels including arteries to heart, abdominal organs and extremities.

[0013] There are two primary disadvantages to thrombolytic agents. First, every cell in the body is exposed to the agent which can lead to serious and often life threatening bleeding complications in remote areas such as the brain and stomach. The risk of major bleeding complications can be as high as 25% and the risk of often fatal bleeding into the brain can go up to 3%. Second, blood clots undergo a process called organization where the soft gel-like red/purple clot is transformed into a firmer, whitish clot by the cross-linking of proteins such as fibrin. Organized clots are much less amenable to treatment with thrombolytic agents. Thromboemboli, such as pulmonary emboli, can contain a significant amount of organized clot since the thrombus frequently developed at its original site (e.g., the deep veins of the legs) over a long period of time prior to embolizing to the remote site (e.g., the lungs).

[0014] Mechanical treatments involve the direct manipulation of the material to eliminate the obstruction. This can involve aspiration, maceration, and compression against the vessel wall, or other types of manipulation. The distinct advantage of mechanical treatment is that it directly attacks the offending material and eliminates the vascular obstruction independent of the specific content of the offending material. Mechanical treatments, if feasible, can usually prove to be superior to biologic treatments for vascular obstruction. Procedural success rates tend to be higher. The best example of this advantage is in the treatment of acute myocardial infarction. Although thrombolytic therapy has had a major impact on the management of patient with myocardial infarction, this option is now relegated to a distant second choice. The clear standard of care today for an acute myocardial infarction is an emergency percutaneous coronary intervention during which the coronary artery obstruction is relieved by aspiration, maceration or balloon compression of the offending thrombus. This mechanical approach has been shown to decrease the amount of damaged heart tissue and improve survival relative to the thrombolytic biological approach.

[0015] Mechanical treatment, however, has played a limited role in the removal of blood clots found in larger blood vessels such as pulmonary arteries and heart chambers. Surgical pulmonary embolectomy involves opening the pul-

monary artery and removing the offending clot under direct vision. This operation has been performed for nearly 100 years, but did not become practical until the introduction of the heart lung machine. Even then, it was generally relegated to a salvage procedure in moribund patients in whom all other options had been exhausted because of the inherent danger in the surgery and the recovery period. While surgical pulmonary embolectomy is very effective in completely evacuating pulmonary emboli whether soft-fresh and firm-organized clot, it is an invasive procedure. Recent data has shown that the early outcomes with surgical pulmonary embolectomy are excellent, at least as good as thrombolytic treatment, as long as the procedure is performed in a timely fashion before the patient become very ill or suffers a cardiac arrest. The long term outcomes of patients surviving surgical pulmonary embolectomy have always been very good. Although these data have generated a renewed interest in performing surgical pulmonary embolectomy, its use remains limited because of the invasiveness of the procedure. Although minimally invasive approaches have been described, the standard procedure requires a 20-25 cm incision through the sternal bone and placing the patient on cardiopulmonary bypass (the heart-lung machine).

[0016] Catheter-based removal of blood clots from larger blood vessels (e.g., pulmonary arteries) and heart chambers has had limited success, at least compared to smaller blood vessels (e.g., coronary arteries). Catheter pulmonary embolectomy, where the pulmonary emboli are removed percutaneously using one of several techniques, has been around for nearly 30 years but few patients currently receive these therapies. These techniques can be subdivided into three categories. With fragmentation thrombectomy, the clot is broken into smaller pieces, most of which migrate further downstream, decreasing the central obstruction but resulting in a "no-reflow" phenomenon. It is sometimes used in combination with thrombolytics which preclude their use as an alternative to thrombolytics. With the rheolytic thrombectomy, high velocity saline jets create a Venturi effect and draw the fragments of the clot into the catheter. Finally the aspiration techniques draw the clot into a catheter via suction. With a Greenfield embolectomy, the catheter with the attached clot is repeatedly drawn out of the vein. All of these techniques rely on catheters which are small compared to the size of the clots and blood vessels. Their limited success is likely related to their inability to achieve a complete en-bloc removal of the material without fragmentation.

[0017] The experience with catheter-based treatment of deep venous thrombus has also had limited success. The operator must use relatively small catheters to remove or break up large amounts of well embedded clot. This procedure is therefore time-consuming, inefficient and ultimately not very effective in removal of the whole clot.

[0018] It is clear that all of the therapeutic options available to patients with clot or other undesirable material in medium or large blood vessels, such as those with pulmonary embolism, have serious limitations. Anticoagulation only limits propagation of clot, it does not remove it. Thrombolytic therapy is not targeted, carries a real risk of major bleeding, and is not very effective in firm/organized clots. Catheter embolectomy uses technology developed for small blood vessels, does not scale well to material residing in medium and large vessels or heart chambers, and thus is not very effective. Surgical embolectomy is highly effective

but highly invasive. There is a real need for a direct mechanical treatment that is as effective as surgical embolectomy but can be performed using endovascular techniques.

[0019] Current efforts to apply existing catheter embolectomy technologies to medium to large blood vessels and heart chambers encounter at least two obstacles: fragmentation and excessive blood loss. Techniques which depend on fragmentation of the material tend to be inefficient and ineffective in medium to large blood vessels and heart chambers because the flow of blood will carry a significant portion of the fragmented material away before it can be captured in the catheter. On the other hand, techniques which depend on aspiration of undesirable material will result in excessive blood loss as the size of the catheter increases.

[0020] A need therefore exists for a system and method to endovascularly remove undesirable material residing in medium to large blood vessels and heart chambers with minimal fragmentation and without excessive blood loss.

SUMMARY OF THE INVENTION

[0021] The present invention relates generally to systems and methods for removing undesirable material residing in vessels, such as blood vessels, or within chambers of the heart. More specifically, the subject invention relates to systems and methods for using a cannula to remove substantially en bloc, from a site of obstruction or interest, an undesirable material, such as blood clots, embolisms and thromboembolisms, without significant fragmentation and without excessive fluid loss. In addition, the systems and methods of the present invention may simultaneously reinfuse aspirated (i.e., removed) and filtered fluid, such as blood, back into the patient on a substantially continuous basis to minimize any occurrences of fluid loss and/or shock. The subject invention may be particularly useful, but may not be limited to, the removal of blood clots, tumors, infective vegetations and foreign bodies from medium to large blood vessels and heart chambers.

[0022] In one embodiment, a system for removing an undesirable material from within a vessel is provided. The system includes a first cannula having a distal end and an opposing proximal end. The distal end of the first cannula, in an embodiment, may include or may be deployable to a diameter relatively larger than that of the proximal end. The first cannula may be designed for maneuvering within the vessel to a site of interest, such that an undesirable material can be captured substantially en bloc through the distal end and removed along the first cannula away from the site. The system may also include a pump, in fluid communication with the proximal end of the first cannula, so as to provide a sufficient suction force for removing the undesirable material from the site of interest. The system may further include a second cannula in fluid communication with the pump, so that fluid removed from the site of interest by the first cannula can be directed along the second cannula and reinfused through a distal end of the second cannula. In one embodiment, the distal end of the second cannula may be situated in spaced relation to the distal end of the first cannula. The system may also be provided with a filter device positioned in fluid communication with the first cannula. The filter device, in an embodiment, may act to entrap or capture the undesirable material and remove it from the fluid flow. The system may further be provided with

a reservoir in fluid communication with the filter device. The reservoir may act to transiently collect fluid being directed from the filter device and to provide a source of fluid for reinfusion by the second cannula. A second filter may also be included in fluid communication between the pump and the second cannula, so as to remove, prior to reinfusion, any debris that may have escaped from the filter device from the fluid flow.

[0023] In another embodiment, there is provided a method for removing an undesirable material from within a vessel. The method includes initially maneuvering a first cannula having a distal end and an opposing proximal end to a site of interest within the vessel, such that the distal end of the first cannula is positioned adjacent the undesirable material. Next, a second cannula, in fluid communication with the first cannula, may be positioned such that its distal end can be situated in spaced relation to the distal end of the first cannula. Thereafter, a suction force may be provided through the distal end of the first cannula to the site of interest, so as to remove, through the distal end of the first cannula, the undesirable material substantially en bloc from the site of interest. Subsequently, any fluid removed along with the undesirable material may be reinfused, through the distal end of the second cannula, to a location in spaced relation from the distal end of the first cannula. The suction and reinfusion of blood can occur, in an embodiment, continuously for a desired duration to minimize fluid loss in the patient. Alternatively, the step of suctioning an undesirable material can occur at an intermittent pulse for a desired duration following reinfusion of the removed fluid.

[0024] In a further embodiment, an apparatus for removing an undesirable material from within a vessel is provided. The apparatus includes an elongated tube having a distal end through which an undesirable material can be captured, a pathway extending along the tube to provide a passage for transporting the undesirable material from the distal end, and a proximal end in opposing relations to the distal end through which the undesirable material can exit. The apparatus also includes a funnel situated at the distal end of the tube, and designed for deployment between an flared open position and a collapsed closed position, so as to better engage and capture the undesirable material. The apparatus further includes a mechanism positioned about a distal portion of the tube, which mechanism, upon actuation, can deploy the funnel between the closed closed position and the open position. In one embodiment, the funnel includes a plurality of strips, with each strip being pivotally coupled at one end to the distal end of the tube. The funnel may also include a substantially impermeable membrane extending across a space between adjacent strips, such that the membrane, in connection with the strips define the shape of the funnel. The mechanism, in an embodiment, includes a balloon positioned circumferentially about the tube at a location proximal to the funnel, and an attachment mechanism provided with one end attached to the funnel and an opposite end attached to the balloon. By design, upon expansion of the balloon, the attachment mechanism can pull on the funnel to deploy it into a flared open position. The apparatus may also include a jacket positioned circumferentially about the distal end of the tube, and extending from the funnel to the balloon to protect the vessel from potential irritation that may be caused by the balloon and the strips defining the funnel. As the jacket may be attached to the funnel and the balloon, in one embodiment, the jacket

may act as the mechanism for deploying the funnel into a flared open position upon expansion of the balloon. In another embodiment, a proximal collar having fingers may be fit to the distal end of the first cannula. The fingers may be made of a shape memory alloy and may be in a flared position in its resting state. An outer sheath may be placed circumferentially around the first cannula, thereby keeping the fingers in a collapsed position until the distal end of the first cannula is near the undesirable material to be removed.

[0025] In a further embodiment, a method of removing undesirable material is disclosed. The method includes an outer suction cannula and an inner suction cannula, the outer suction cannula having an outer suction cannula lumen and the inner suction cannula having an inner suction cannula lumen, wherein the inner suction cannula is situated within the outer suction cannula lumen.

[0026] A method of manufacture of a suction cannula is also provided. In one embodiment, the method of manufacture of a suction cannula with an outer sheath is provided. In one embodiment, the method of manufacture of a Teflon lined suction cannula is provided. In another embodiment, the method of manufacture of a hydrophilically coated cannula is provided. In another embodiment, a method of manufacture of a suction cannula with a urethane shaft and a hydrophilically coated funnel is provided.

BRIEF DESCRIPTION OF THE DRAWINGS

[0027] These and other features and advantages of the present invention will become more apparent from the following detailed descriptions taken in conjunction with the accompanying drawings wherein like reference characters denote corresponding parts throughout the several views.

[0028] FIG. 1 illustrates a plan view of a system for removing an undesirable material from within a vessel in accordance with one embodiment of the present invention.

[0029] FIGS. 2A-H illustrate partial isometric views of a distal end of a suction cannula in operation in connection with the system shown in FIG. 1.

[0030] FIGS. 3A-B illustrate partial isometric views of an alternate distal end of a suction cannula used in connection with the system shown in FIG. 1.

[0031] FIGS. 4A-B illustrate partial isometric views of a variety of cannulas for use in connection with the system shown in FIG. 1.

[0032] FIGS. 4C-E illustrate plan views of a variety of cannulas for use in connection with the system shown in FIG. 1.

[0033] FIG. 5 illustrates a partial isometric view of a port through which another device may be introduced within a suction cannula used in connection with the system shown in FIG. 1.

[0034] FIG. 6 illustrates a plan view of a system for removing an undesirable material from within a vessel in accordance with another embodiment of the present invention.

[0035] FIG. 7 illustrates an isometric view of a system of the present invention being deployed within a patient for removing an undesirable material from a site of interest.

[0036] FIG. 8 illustrates a plan view of an improved suction cannula in connection with FIG. 1. FIG. 9A illustrates a partial isometric view of the distal section of another embodiment of the suction cannula.

[0037] FIGS. 9A-A-9B-B illustrate cross-sectional views of the suction cannula of FIG. 9A taken along lines A-A and B-B.

[0038] FIGS. 9B-9E illustrate longitudinal partial cross-sectional views of the distal section of the suction cannula depicting the manufacturing process.

[0039] FIG. 10 illustrates an isometric view of the reinforcement arms with proximal collar.

[0040] FIG. 10A-10D illustrate plan views of the various embodiments of the reinforcement arms with proximal collar.

[0041] FIGS. 11A-11C illustrate longitudinal partial cross-sectional partial views of the distal section of suction cannula depicting the manufacturing process.

[0042] FIG. 12 illustrates a partial isometric view of a multiple suction cannula device.

[0043] FIG. 13 illustrates a front-end plan view of the multiple suction cannula device of FIG. 12.

[0044] FIG. 14 illustrates a partial plan side view of the multiple suction cannula device of FIG. 12.

[0045] FIG. 14A-A illustrates a longitudinal cross-sectional view of the multiple suction cannula device of FIG. 14 taken along lines A-A.

[0046] FIG. 15 illustrates a partial plan side view of the multiple suction cannula device of FIG. 14.

[0047] FIG. 15A-A-15 D-D illustrates cross-sectional views of the multiple suction cannula device of FIG. 14 taken along lines A-A, B-B, C-C and D-D.

[0048] FIG. 16 depicts a plan view of the suction cannula device of the current invention inserted through groin of a patient.

[0049] FIG. 17-20 illustrate flow charts depicting methods of manufacturing the device.

[0050] FIG. 21 illustrates a flow chart depicting one method of using the device of the current invention.

DETAILED DESCRIPTION OF SPECIFIC EMBODIMENTS

[0051] As noted above, existing catheter techniques may not be effective in removing undesirable material, such as clots, from medium and large size blood vessels or from heart chambers, because these catheters tend to be small relative to the material to be removed. As a result, the material often needs to be fragmented in order to fit within the catheter. However, with fragmentation, the chances of the fragments being carried away in the bloodstream increases, resulting in downstream obstruction. If the catheter is enlarged to accommodate the larger structure and material, such a catheter may aspirate an unacceptable volume of blood, resulting in excessive fluid loss and/or shock in the patient.

[0052] The present invention overcomes the deficiencies of existing devices and techniques and can act to remove substantially en bloc (i.e., wholly or entirely) undesirable material, such as thrombi and emboli, from the vasculature, including medium to large size blood vessels, and from heart chambers. Vessels from which the undesirable material may be removed, in accordance with an embodiment of the present invention, include, for example, those within the pulmonary circulation (e.g., pulmonary arteries), systemic venous circulation (e.g., vena cavae, pelvic veins, leg veins, neck and arm veins) or arterial circulation (e.g., aorta or its large and medium branches). The heart chambers may be, for example, in the left heart (e.g., the left ventricular apex

and left atrial appendage), right heart (e.g., right atrium and right ventricle), or on its valves. The present invention can also act to remove tumors, infective vegetations and other foreign.

[0053] Although reference is made to medium and large vessels, it should be appreciated that the systems and methods, hereinafter disclosed, can be scaled and adapted for use within smaller vessels within the body, if desired.

[0054] Referring now to FIG. 1, there is illustrated a system 1 for removing an undesirable material, substantially en bloc, from an obstruction site or site of interest within the vasculature, and for reinfusion of fluid removed (i.e., suctioned or aspirated) from the site of interest back into a patient, in order to minimize fluid loss within the patient. System 1, in an embodiment, may be provided with a first or suction cannula 10 for capturing and removing en bloc the undesirable material from the site of interest, such as that within a blood vessel or a heart chamber. Cannula 10, in an embodiment, may be an elongated tube and may include a distal end 11 through which the undesirable material can be captured and removed. Cannula 10 may also include a lumen or pathway 12 extending along a body portion of cannula 10. Pathway 12, in one embodiment, provides a passage along which the captured material and aspirated circulatory fluid, such as blood, that may be captured therewith may be transported and directed away from the site of interest. Cannula 10 may further include a proximal end 13 in opposing relations to the distal end 11, and through which the captured material may exit from the cannula 10.

[0055] Since cannula 10 may be designed for introduction into the vasculature, for instance, through a peripheral blood vessel, and may need to subsequently be maneuvered therealong to the site of interest, cannula 10, in an embodiment, may be made from a pliable material. In addition, as cannula 10 may be used to introduce a suction force to the site of interest for capturing the undesirable material, cannula 10 may be made from a sufficiently stiff material or may be reinforced with a sufficiently stiff material, so as not to collapse under a suction force. In one embodiment, cannula 10 may be constructed from a biocompatible material, such as polyvinyl chloride, polyethylene, polypropylene, polyurethane, Pebax®, silicone, or a combination thereof.

[0056] In certain instances, it may be desirable to maneuver cannula 10 to the site of interest using image guidance, for example, using fluoroscopy or echocardiography. In order to permit cannula 10 to be visualized, cannula 10, in an embodiment, may also include a radioopaque material or any material capable of being visualized.

[0057] To better engage and capture the undesirable material substantially en bloc and without significant fragmentation, the distal end 11 of cannula 10 may be designed to have a diameter that can be relatively larger than that of the proximal end 13. In one embodiment, as illustrated in FIGS. 2A-D, distal end 11 of cannula 10 may be in the shape of a funnel 20, and may be provided with a diameter, for example, approximately at least three times that of pathway 12.

[0058] Of course, depending on the surgical procedure being implemented, the ratio between the diameter of funnel 20 and pathway 12 can be varied, if so desired. Funnel 20, with its design, may be placed directly at a site of interest 23 to engage undesirable material 24 (FIG. 2C), or spatially away from the site of interest 23 to capture the undesirable material 24 (FIG. 2D). In a situation where the distal end 11

may be situated spatially away from the site of interest, by providing distal end 11 with funnel 20, a vortex effect may be generated during suctioning to better direct the undesirable material into the funnel 20. It is believed that fluid flowing into funnel 20 can often exhibit a laminar flow circumferentially along the interior surface of the funnel 20 to generate a vortex flow into the distal end 11 of suction cannula 10. Thus, in the presence of a vortex flow, such a flow can act to direct the undesirable material toward the distal end 11 to allow the material to subsequently be pulled into the distal end by suctioning.

[0059] To provide a funnel shaped distal end, cannula 10 may include, in an embodiment, a sheath 21 circumferentially situated about distal end 11 of cannula 10. Sheath 21, as illustrated, may be designed to slide toward as well as away from the distal end 11 of cannula 10. In that way, when the distal end 11 is positioned at the site of interest 23, and sheath 21 is retracted (i.e., slid away from the distal end 11), funnel 20 may be exposed and expanded into the desired shape in order to engage undesirable material 24. To collapse funnel 20, sheath 21 may be advanced toward the distal end 11 and over the funnel 20. Thereafter, cannula 10 may be maneuvered from the site of interest 23.

[0060] In order to enhance capture and removal of the undesirable material 24, looking now at FIGS. 2E-G, cannula 10 may be designed to allow introduction of a catheter 25 with balloon 26 to the site of interest. In an example where the undesirable material 24 may be entrapped within funnel 20, catheter 25 with balloon 26 may be directed along the lumen or pathway 12 of cannula 10 and into funnel 20. Once catheter 25 has been advanced past the undesirable material 24 within funnel 20, balloon 26 may be inflated to a size sufficient to pull on the undesirable material entrapped within funnel 20. As balloon 26 is pulled down the funnel 20 towards pathway 12, balloon 26 can dislodge the entrapped material and can eventually partially or substantially occlude a pathway 12, distal to the undesirable material 24, which in essence occludes the fluid communication between cannula 10 and the vessel. The suction force within pathway 12, as a result, can be enhanced to better remove the undesirable material. Similarly, as shown in FIG. 2H, in a situation where undesirable material 24 may be firmly lodged in the vessel at the site of interest 23 and the suction applied by cannula 10, spatially situated away from the site of interest 23, may be insufficient to dislodge the undesirable material 24, catheter 25 and balloon 26 may be advanced past the distal end of cannula 10 and past the undesirable material 24 at the site of interest 23. Once past the undesirable material 24 the balloon 26 may be inflated and as balloon is withdrawn back towards the distal end 11 of cannula 10, it can dislodge the undesirable material and allow the suction to draw it into the distal end of cannula 10. Of course, this approach can also be applied when cannula 10 is situated directly at the site of interest 23 and the suction force may be insufficient to dislodge the undesirable material 24.

[0061] In another embodiment, looking now at FIGS. 3A-B, funnel 20 located at distal end 11 of cannula 10 may be created by providing a plurality of independent strips 31, each coupled at one end to distal end 11 of cannula 10.

[0062] In the embodiment shown in FIG. 3A, three strips 31 are illustrated. However, it should be appreciated that two or more strips 31 may be used, if so desired. Strips 31, in an embodiment, may be designed to pivot between a closed position, where strips 31 may be substantially adjacent one

another, and an open position, where strips may be flared into a funnel 20, shown in FIG. 3A. To deploy strips 31, and thus funnel 20, between an open and closed position, cannula 10 may include a balloon 33 positioned circumferentially about cannula 10 and proximal to strips 31. In addition, an attachment mechanism, such as a string 34 or any similar mechanisms (e.g., rod, chain etc.), may be provided for each of the strips 31, with one end attached to one strip 31 and an opposite end attached to balloon 33. In this way, when balloon 33 is inflated and expands radially, balloon 33 may pull on each attachment mechanism 34, so as to deploy strips 31 into a flared open position. Balloon 33, in one embodiment, may be inflated through opening 37 through the use of any fluid, including water, air, or radioopaque contrast material. It should be noted that securing of the attachment mechanism to the strips 31 and balloon 33 can be accomplished using any methods or mechanisms known in the art. For instance, adhesives, knots, or soldering etc. may be used. Moreover, to the extent desired, strips 33 and balloon 31 may be designed to expand to a diameter larger than that of the vessel within which cannula 10 is being deployed. In that way, cannula 10 may be securely positioned at the site of interest for removal of the undesirable material substantially en bloc.

[0063] To better capture the undesirable material and direct it into the cannula 10, a membrane 35 may be placed across a space between adjacent strips 31 when the strips 31 are in the open position. In one embodiment, a continuous membrane 35 may be used to circumferentially stretch across each of the space between adjacent strips 31. Membrane 35 may also act to enhance suction at the site of interest, as it can cover up any open space between the strips 31. To that end, membrane 35, in an embodiment, may be made from a non-permeable material. It should be appreciated that membrane 35 and strips 31, as illustrated, together define funnel 20 at distal end 11 of cannula 10.

[0064] Furthermore, to protect the vessel from irritation or damage that may be caused by the presence of balloon 33 and/or strips 31, jacket 36, as shown in FIG. 3B, may be provided circumferentially about the distal 11 of cannula 10. In an embodiment, jacket 36 may extend substantially from a tip of each strip 31 to balloon 33. Jacket 36, however, can be affixed anywhere along each strip 31, if necessary. Since jacket 36 attaches at one end to strips 31 and at an opposite end to balloon 33, jacket 36, in an embodiment, may be used instead of attachment mechanism 34 to deploy strips 31 into an open position when balloon 33 is expanded. Of course, jacket 36 may also be used in conjunction with attachment mechanism 34 to deploy strips 31 into an open position. Furthermore, in one embodiment, jacket 36 may be lengthened, so that the end connected to strips 31 may instead be pulled over strips 31, into funnel 20, and attached substantially to a base of each strips 31 (i.e., base of funnel 20). With such a design, membrane 35 may not be necessary, as jacket 36 may serve the purpose of membrane 35 to cover the space between each of strips 31. In such an embodiment, at least that portion of jacket 36 extending over strips 31 and into the base funnel 20 can be impermeable.

[0065] In certain instances, balloon 33 may act to enhance the suction force being applied at the site of interest when removing the undesirable material. For instance, when cannula 10 is deployed downstream of the undesirable material, rather than substantially adjacent to the undesirable material, within a vessel having a venous circulation (i.e., flow toward

the heart), balloon 33, when expanded radially, can substantially occlude the vessel, such that collateral fluid flow within the vessel can be minimized, thereby increasing the suction force that can be applied to the undesirable material. Additionally, the occlusion of such a vessel by balloon 33 can better direct the material being removed into the funnel 20 and prevent the material from being carried by the flow of blood past the funnel.

[0066] Alternatively, when cannula 10 is deployed upstream of the undesirable material within a vessel having an arterial circulation (i.e., flow away from the heart), rather than substantially adjacent to the undesirable material, balloon 33, when expanded radially, can substantially occlude the vessel, such that pressure being exerted on the downstream material by the fluid flow can be lessened. By lessening the pressure on the material to be removed, the suction force being applied at the site of interest can act to remove the material more easily.

[0067] As suction cannula 10 may be made from a pliable material, in order to efficiently direct it along a vessel to the site of interest, cannula 10 may be reinforced with wire or other material to optimize maneuverability within the vessel without kinking. Referring now to FIG. 4A, suction cannula 10 may, in addition to pathway 12, be provided with one or more additional pathway or lumen 41. In this multi-lumen design, pathway 12 may act, as noted above, to provide a passage along which the captured material may be transported and directed away from the site of interest. Lumen 41, on the other hand, can provide a passage along which a fluid can be directed to inflate balloon 33 through opening 37 (FIGS. 3A-B). In certain embodiments, lumen 41 may also be used to accommodate other devices, such as other catheters or surgical instruments, for use in connection with a variety of purposes. For example, a device may be inserted and advanced along lumen 41 through the distal end 11 of suction cannula 10 to dislodge the undesirable material. An angiography catheter can be inserted and advanced along lumen 41 through the distal end 11 of suction cannula 10 to perform an angiogram to confirm the location of the undesirable material or confirm that it has been successfully removed. A balloon embolectomy catheter can be inserted along lumen 41 toward the distal end 11 of suction cannula 10 to remove any material which may have clogged the cannula or past the any undesirable material firmly lodged in the vessel to draw it into the cannula. Although illustrated with such a multi-lumen design, any other multi-lumen design may be possible.

[0068] To introduce other devices, such as catheter 25 with balloon 26, into lumen 41 or pathway 12, cannula 10 may be provided with a port 51, as shown in FIG. 5, located at the proximal end 13 of cannula 10. It should be appreciated that in the embodiment where cannula 10 has only pathway 12 (i.e., single lumen cannula), port 51 may similarly be provided at the proximal end 13 of cannula 10 to allow the introduction of other devices into pathway 12.

[0069] Cannula 10 of the present invention may be of any sufficient size, so long as it can be accommodated within a predetermined vessel, such as a medium to large size blood vessel. The size of cannula 10 may also be determined by the size of the undesirable material to be removed, so long as the undesirable material can be removed substantially en bloc without significant fragmentation. In one embodiment, suction cannula 10 may be designed to remove at least 10 cm³ of undesirable material substantially en bloc. Of course,

cannula **10** can be scaled and adapted for use within smaller vessels in the body and for removing a relatively smaller volume or amount undesirable material, if so desired.

[0070] Looking again at FIG. 1, system **1** can also include filter device **14** in fluid communication with the proximal end **13** of cannula **10**. Filter device **14**, in one embodiment, may include an inlet **141** through which fluid removed from the site of interest along with the captured undesirable material can be directed from cannula **10**. Filter device **14** may also include an outlet **142** through which filtered fluid from within device **14** may be directed downstream of system **1**. To prevent the undesirable material captured from the site of interest from moving downstream of system **1**, filter device **14** may further include a permeable sheet **143** positioned within the fluid flow between the inlet **141** and the outlet **142**.

[0071] Permeable sheet **143**, in an embodiment, may include a plurality of pores sufficiently sized, so as to permit fluid from the site of interest to flow therethrough, while preventing any undesirable material captured from the site of interest from moving downstream of system **1**. Examples of permeable sheet **143** includes coarse netting, fine netting, a screen, a porous filter, a combination thereof, or any other suitable filter material capable of permitting fluid to flow through while impeding movement of the captured undesirable material. It should be noted that, rather than just one, a plurality of permeable sheets **143** may be used. Alternatively, one permeable sheet **143** may be folded to provide multiple surfaces, similar to an accordion, for use in connection with filter device **14**. By using a plurality of permeable sheets **143** or by folding sheet **143**, the number of filtration surfaces through which the fluid must flow increases to enhance filtration and further minimize any occurrence of any undesirable material from moving downstream of system **1**.

[0072] Although a permeable sheet **143** is described, it should be appreciated that filter device **14** may be of provided with any design capable of entrapping the undesirable material, while allowing fluid to move therethrough. To that end, filter device **14** may include a mechanical trap to remove the undesirable material from the fluid flow. Such a mechanical trap may be any trap known in the art and may be used with or without permeable sheet **143**.

[0073] Still looking at FIG. 1, system **1** may also be provided with a pump **15** designed to generate negative pressure, so as to create a necessary suction force through cannula **10** to pull any undesirable material from the site of interest. In one embodiment, pump **15** may include an intake port **151** in fluid communication with outlet **142** of filter device **14**. Intake port **151**, as illustrated, may be designed to receive filtered fluid from filter device **14**. Pump **15** may also be designed to generate the positive pressure, so as to create a necessary driving force to direct fluid through exit port **152** and downstream of system **1** for reinfusion of fluid removed from the site of interest back into the body. In an embodiment, the suction force and the drive force may be generated by pump **15** simultaneously and may take place continuously or intermittently for a set duration. Pump **15**, as it should be appreciated, may be any commercially available pump, including those for medical applications and those capable of pumping fluids, such as blood. Examples of such a pump includes a kinetic pump, such as a centrifugal pump, and an active displacement pump, such as a rollerhead pump.

[0074] In an alternate embodiment, an independent vacuum device (not shown), may be provided for generating the necessary suction force at the site of interest, while a pump **15** may act to generate the necessary driving force for reinfusion purposes. In such an embodiment, pump **15** may be in fluid communication with the filter device **14**, while the vacuum device may be in fluid communication with suction cannula **10** upstream to the filter device **14**. The independent pump **15** and vacuum device may operate intermittently for a set duration, and if desired, either the vacuum device or pump **15** may operate continuously, while the other operates intermittently.

[0075] Downstream of pump **15**, system **1** may further include a second or reinfusion cannula **16** in fluid communication with the exit port **152** of pump **15**. Reinfusion cannula **16**, in an embodiment, may be designed to permit filtered fluid, directed from filter device **14** by way of pump **15**, to be reinfused back into a patient at a desired site. To that end, reinfusion cannula **16** may be designed for placement within the same or different vessel within which suction cannula **10** may be located.

[0076] Reinfusion cannula **16**, in one embodiment, may be an elongated tube and includes a distal end **161** through which cleansed or filtered fluid can be reinfused back into the body. In an embodiment, distal end **161** of reinfusion cannula **16** may be designed so that it can be situated in spaced relation to the distal end **11** of the suction cannula **10** when system **1** is in operation. Reinfusion cannula **16** may also include a lumen or pathway **162** extending along its body portion to provide a passage along which the filtered fluid, such as blood, may be transported to a reinfusion site. Reinfusion cannula **16** may further include a proximal end **163** in opposing relations to the distal end **161**, and through which the filtered fluid from pump **15** may enter into the cannula **16**.

[0077] Furthermore, similar to suction cannula **10**, since reinfusion cannula **16** may be designed for introduction into the vasculature, and may need to be maneuvered therealong, reinfusion cannula **16**, in one embodiment, may be made from a pliable material. In one embodiment, reinfusion cannula **16** may be constructed from a biocompatible material, such as polyvinyl chloride, polyethylene, polypropylene, polyurethane, Pebax®, silicone, or a combination thereof. In certain instances, it may be desirable to maneuver reinfusion cannula **16** to the reinfusion site using image guidance, for example, using fluoroscopy or echocardiography. To permit reinfusion cannula **16** to be visualized, reinfusion cannula **16**, in an embodiment, may also be made to include a radioopaque material.

[0078] Since reinfusion cannula **16** may be made from a pliable material, in order to efficiently direct it along a vessel to the reinfusion site, reinfusion cannula **16** may be reinforced to optimize maneuverability within the vessel without kinking. Moreover as shown in FIG. 4B, reinfusion cannula **16** may be provided with one or more additional lumens. With a multi-lumen design, lumen **162**, as noted above, may act to provide a passage along which the filtered fluid may be transported and directed to the reinfusion site. Lumen **42**, on the other hand, can provide a passage through which a guide wire can be inserted to assist in the guiding the reinfusion cannula **16** to the reinfusion site, or through which other instruments and devices may be inserted for various surgical procedures. With such a multi-lumen design, reinfusion cannula **16** can serve as an introducer

sheath by providing lumen 42 through which these instruments can pass, while filtered blood can be reinfused through lumen 162. Although illustrated with such a multi-lumen design, any other multi-lumen design may be possible.

[0079] Although illustrated as a separate component from suction cannula 10, in certain embodiments, the reinfusion cannula 16 may be designed to be substantially integral with suction cannula 10. In one embodiment, as illustrated in FIG. 4C, reinfusion cannula 16 may be incorporated as part of a double or multi-lumen introducer sheath 43 for insertion into the same vessel within which the suction cannula 10 may be situated. In particular, suction cannula 10 may be inserted and maneuvered through one lumen 44 of sheath 43, while reinfusion cannula 16 may be in fluid communication with lumen 45 of sheath 43. In such an embodiment, lumen 45 may include a distal end 451 in spaced relations to the distal end 11 of cannula 10, so that cleansed or filtered fluid may be introduced to the reinfusion site away from the site of interest where the distal end 11 of cannula 10 may be positioned.

[0080] Alternatively, as illustrated in FIG. 4D, reinfusion cannula 16 may be incorporated as part of a double or multi-lumen introducer sheath 43 where the reinfusion cannula 16 and the suction cannula 10 may be concentrically aligned along a shared axis A. In the embodiment shown in FIG. 4D, reinfusion cannula 16 may have a diameter that can be relatively larger than that of suction cannula 10. To that end, reinfusion cannula 16 can accommodate suction cannula 10 within pathway 162 of the reinfusion cannula 16, and allow suction cannula 10 to extend from within pathway 162, such that the distal end 11 of suction cannula 10 may be positioned in spaced relations relative to the distal end 161 of reinfusion cannula 16. The spaced relations between distal end 161 and distal end 11 allows filtered fluid to be introduced to the reinfusion site away from the site of interest, where the removal of the undesirable material may be occurring.

[0081] In another embodiment, reinfusion cannula 16 and suction cannula 10 can be integrated into a single multi-lumen suction-reinfusion cannula 46, as shown in FIG. 4E. In the embodiment shown in FIG. 4E, multi-lumen cannula 46 may include a distal suction port 461 through which undesirable material from the site of interest can be removed, and a proximal reinfusion port 462 through which cleansed or filtered fluid may be reinfused back into the body. The spaced relations between the suction port 461 and reinfusion port 462 allows filtered fluid to be introduced to the reinfusion site away from the site of interest where the removal of the undesirable material may be occurring.

[0082] In an embodiment, the size of the reinfusion cannula, whether independent from the suction cannula, part of a multi-lumen introducer sheath, part of a multi-lumen combined suction-reinfusion cannula, or in concentric alignment with the suction cannula, may be designed so that it can handle a relatively rapid reinfusion of large volumes of fluid by pump 15. With reference now to FIG. 6, system 1 may also include a reservoir 61. Reservoir 61, in one embodiment, may be situated in fluid communication between filter device 14 and pump 15, and may act to transiently collect fluid filtered from the site of interest, prior to the filtered fluid being directed into reinfusion cannula 16. By providing a place to transiently collect fluid, reservoir 61 can allow the rate of suctioning (i.e., draining, aspirating) to be separated

from rate of reinfusing. Typically, the rate of reinfusion occurs at substantially the same rate of suctioning, as the volume of fluid suctioned from the site of interest gets immediately directed along the system 1 and introduced right back to the reinfusion site in a patient. However, the availability of a volume of transiently collected fluid in reservoir 61 now provides a source from which the amount or volume of fluid being reinfused back into the patient can be adjusted, for example, to be less than that being suctioned from the site of interest, as well as the rate at which fluid can be reinfused back into the patient, for example, at a relatively slower rate in comparison to the rate of suctioning. Of course, if so desired or necessary, the reinfusion rate and volume can be adjusted to be higher, relative to the rate and volume of suction.

[0083] In accordance with one embodiment of the present invention, reservoir 61 may be a closed or an open container, and may be made from a biocompatible material. In an embodiment where reservoir 61 may be a closed container, system 1, likewise, will be a closed system. As a result, pump 15 may be used as both a suction source and a driving force to move fluid from the site of interest to the reinfusion site. In such an embodiment, pump 15 can generate a suction force independently of or alternately with a driving force to allow reservoir 61 collect filtered fluid from filter device 14. In one embodiment, pump 15 may be provided with a gauge in order to measure a rate of flow of the fluid being reinfused. Alternatively, where reservoir 61 may be an open container, reservoir 61, in such an embodiment, may be designed to accommodate both a volume of fluid, typically at the bottom of reservoir 61, and a volume of air, typically at the top of reservoir 61, to provide an air-fluid interface within reservoir 61. As a result, using pump 15 in fluid communication with reservoir 61 may not provide the needed driving force and/or suction force to adequately remove the undesirable material and to subsequently reinfuse fluid back into a patient.

[0084] To address this, system 1, in an embodiment, may include a separate and independent vacuum source, in fluid communication with the volume of air at the top of reservoir 61, for providing the necessary suction force from the top area of reservoir 61 where air exists, through filter device 14, through the distal end 11 of cannula 10, and to the site of interest. A port provided above the fluid level within reservoir 61 may be provided to allow the independent vacuum source to be in fluid communication with the volume of air within reservoir 61. Pump 15, on the other hand, may be in fluid communication with the volume of fluid within reservoir 61, and may act to generate the necessary driving force for reinfusion purposes. It should be appreciated that although shown as separate components, to the extent desired, reservoir 61 and filter device 14 may be combined as a single unit.

[0085] Still referring to FIG. 6, system 1 may further include a second filter device 62 positioned in fluid communication between pump 15 and reinfusion cannula 16. Second filter device 62 may act to remove any debris or material (e.g., ranging from smaller than microscopic in size to relatively larger) that may have escaped and moved downstream from filter device 14, so that the fluid may be substantially cleansed prior to reinfusion. In an embodiment, second filter device 62 may include a porous membrane 63 whose pores may be measurably smaller than that in filter device 14, but still capable of allowing fluid to flow there-

through. Since fluid such as blood needs to be filtered through system **1**, it should be noted that system **1** and its components may be made from a biocompatible material to minimize any adverse reaction when fluid removed from the site of interest gets reinfused back into the body.

[0086] In operation, system **1** of the present invention may be introduced into the vasculature, preferably through a peripheral blood vessel, to remove undesirable material, such as a clot, emboli, or thrombi, substantially en bloc and without significant fragmentation, and subsequently reinfusing fluid removed from the site of interest back into a patient. In particular, system **1** and its components disclosed above can collectively form a substantially closed circuit through which fluid and an undesirable material from a site of interest can be removed by suction, cleared of the undesirable material, filtered to remove any additional debris, and actively introduced back into a patient at a reinfusion site.

[0087] With reference now to FIG. **7**, there is shown one embodiment of the system of the present invention being utilized for removal of an undesirable material within a patient **700**. System **70**, as illustrated, includes a suction cannula **71**, filter device **72**, pump **73**, second filter device **74** and reinfusion cannula **75**. It should be appreciated that depending on the procedure and to the extent desired, system **70** may not need all of the components shown, or may need other components in addition to those shown.

[0088] In general, the method of the present invention, in one embodiment, includes, initially accessing a first blood vessel **701** either by surgical dissection or percutaneously with, for instance, a needle and guide wire. The first blood vessel through which suction cannula **71** may be inserted into patient **700** can be, in an embodiment, any blood vessel that can be accessed percutaneously or by surgical dissection such as femoral vein, femoral artery or jugular vein. Next, suction cannula **71** may be inserted into the first blood vessel **701** over the guide wire, and advanced toward a site of interest **702**, for instance, in a second vessel or a heart chamber **703** where an undesirable material **706** may be residing. The second blood vessel or heart chamber, in an embodiment, can be the main pulmonary artery, branch pulmonary arteries, inferior vena cavae, superior vena cavae, deep veins of the pelvic, legs, arms or neck, aorta, or any other medium to large blood vessel for which the use of a cannula is suitable for removing undesirable material without causing undesirable damage to the blood vessel. In addition, the advancement of suction cannula **71** may be gauged or documented by fluoroscopic angiography, echocardiography or other suitable imaging modality.

[0089] In the case of pulmonary embolism, the suction cannula **71** may normally be introduced through the femoral, jugular or subclavian vein. Alternatively, the suction cannula **71** may be introduced, if desired, directly into the cardiac chambers using a minimally invasive surgical or endoscopic, thoracoscopic, or pericardioscopic approach.

[0090] Thereafter, a third blood vessel **704** may be accessed either by surgical dissection or percutaneously with, for example, a needle and guide wire. Subsequently, reinfusion cannula **75** may be inserted into the third blood vessel **703** using an open or over the guide wire technique. The third blood vessel through which the reinfusion cannula **75** may be inserted, in one embodiment, can be any large vein, such as the femoral vein or jugular vein. Reinfusion cannula **75** may then be advanced toward a reinfusion site, for example, within a fourth blood vessel **705**. The fourth

blood vessel, in one embodiment, can be the femoral vein, iliac vein, inferior vena cava, superior vena cava or right atrium.

[0091] Once reinfusion cannula **75** is in place and components of system **70** have connected, pump **73** may be activated, and suction cannula **71** may then be placed against and in substantial engagement with the undesirable material **706** at the site of interest **702** for removal by suctioning through the suction cannula **71**. The undesirable material **706** and circulatory fluid removed from the site of interest **702** may thereafter be directed along suction cannula **71** into filter device **72** where the undesirable material **706** can be entrapped and removed from the fluid flow. The resulting filtered fluid may next be directed downstream by way of pump **73** into the second filter device **74**, where any debris or material (e.g., ranging from smaller than microscopic in size to relatively larger) that may have escaped and moved downstream from filter device **74** can be further captured and removed from the fluid flow prior to reinfusion. The resulting cleansed fluid may then be directed into the reinfusion cannula **75** and introduced back into the patient **700**.

[0092] It should be appreciated that in certain instances, prior to connecting the suction cannula **71** and the reinfusion cannula **75**, system **70** may need to be primed with fluid to minimize or eliminate any air and/or air bubbles from the system prior to the initiation of suction and reinfusion. To that end, the suction cannula **71** and reinfusion cannula **75** can be primed separately with fluid or by allowing blood to backfill the cannulae after insertion. The remaining components of the system **70** including all tubing, the filter device **72**, the pump **73** and any other components of system **70** may also need to be primed with fluid prior to connecting them to the cannulae. In one embodiment, this can be achieved by temporarily connecting these components in fluid communication with other as a closed circuit and infusing fluid through a port, similar to port **51** in FIG. **5**, while providing another port through which air can be displaced. Once these components have been fully primed with fluid, the circuit can be detached and connected to the primed suction cannula **71** and reinfusion cannula **75** in the appropriate configuration. Examples of a priming fluid include crystalloid, colloid, autologous or heterologous blood, among others.

[0093] During operation, pump **73**, in one embodiment, may remain activated so that suction and continuous reinfusion of blood can occur continuously for a desired duration or until the removal of the undesirable material has been confirmed, for instance, by visualizing the captured undesirable material in the filter device **72**. Alternatively pump **73** can be activated intermittently in short pulses, either automatically or manually by an operator (e.g., surgeon, nurse or any operating room attendant), for a desired duration or until the removal of the undesirable material has been confirmed by visualization of the material within filter device **72**.

[0094] It should be appreciated that since suction cannula **71** may be deployed within any vessel within patient **700**, depending on the procedure, in addition to being placed substantially directly against the undesirable material at the site of interest, suction cannula **71** may be deployed at a location distant from the site of interest where direct engagement with the undesirable material may not be possible or desired.

[0095] In a situation where the suction cannula **71** is positioned within a vessel exhibiting a venous flow and at a

distant location from the undesirable material, it may be desirable to place the distal end of suction cannula **71** downstream of the undesirable material, so that the fluid flow can push the undesirable material from the site of interest into suction cannula **71** during suction. To the extent there may be some difficulties with suctioning the undesirable material from its location, if necessary, a catheter may be deployed through suction cannula **71** and to the site of interest, where the undesirable material may be dislodged location for subsequent removal.

[0096] On the other hand, when suction cannula **71** is positioned within a vessel exhibiting arterial flow and at a distant location from the undesirable material, it may be necessary to place the distal end of suction cannula **71** upstream of the undesirable material for the purposes of removal, even though the undesirable material must move against the fluid flow in order to enter into the suction cannula **71**. In such a situation, since the fluid flow in the vessel tends to exert a pressure against the undesirable material at the site of interest, and thus may make the undesirable material difficult to remove, suction cannula **71** may include a flow occlusion mechanism, similar to balloon **33** shown in FIG. 3. When expanded radially, the mechanism can substantially occlude the vessel, such that pressure being exerted on the downstream material by the fluid flow can be lessened. By lessening the pressure on the undesirable material to be removed, the suction force being applied at the site of interest can act to remove the material more easily. Again, if necessary, a catheter may be deployed through suction cannula **71** and to the site of interest, where the undesirable material may be dislodged or drawn back into the cannula to facilitate its removal.

[0097] The method of the present invention may also utilize a fluid reservoir, similar to reservoir **61** shown in FIG. 6, in connection with system **70**. Such a reservoir may be placed in fluid communication between filter device **72** and pump **73**. The reservoir, in an embodiment, may be an independent reservoir or may be integrated with filter device **72** as a single unit, similar to that shown in FIG. 7. By utilizing a reservoir, a volume of transiently collected fluid may be used to independently control the rate or volume of suctioning (i.e., draining, aspirating) and/or the rate or volume of reinfusion.

[0098] In an embodiment where the reservoir may be an open container, it should be appreciated that system **70** may not be a substantially closed system. As a result, rather than utilizing a pump that can generate both a suction and a driving force for a closed system, an independent vacuum device **76** may be employed to generate the necessary suction force, from the top of the reservoir where a volume of air exists, for removal of the undesirable material, while independent pump **73** may be employed to generate the necessary driving force, from the bottom of the reservoir where a volume of aspirated fluid exists, for reinfusion.

[0099] The method of the present invention may also utilize a suction cannula **71** with a deployable funnel tip, similar to funnel **20** in FIG. 2 or in FIG. 3. In such an embodiment, the funnel may be deployed after suction cannula **71** has been positioned adjacent the site of interest. Thereafter, once the suction force has been activated, the funnel may be advanced to engage the undesirable material for removal. The funnel may remain deployed while the suction force is activated, and through multiple cycles, if necessary, until the undesirable material can be removed.

Subsequently, the funnel may be retracted in order to reposition or remove suction cannula **71**.

[0100] The method of the present invention may further utilize reinfusion cannula **75** that has been incorporated into an introducer sheath, such as sheath **43** as a multi-lumen cannula (FIG. 4C) or as one which concentrically aligns the suction cannula and reinfusion cannula (FIG. 4D). In this embodiment, the sheath/reinfusion cannula **75** may initially be inserted into a first blood vessel. Suction cannula **71** may then be inserted into the introducer lumen of the sheath/reinfusion cannula **75**, and the assembly advanced together to a site of interest in a second blood vessel or heart chamber.

[0101] The method of the present invention may also further utilize a combined multi-lumen suction/reinfusion cannula, similar to cannula **46** shown in FIG. 4E. In such an embodiment, the combined suction/reinfusion cannula may initially be inserted into a first blood vessel to a location where its distal suction lumen can be placed adjacent the site of interest within a second blood vessel, while its proximal located reinfusion lumen can be positioned at an appropriately spaced location from the suction lumen.

[0102] The method of the present invention may, in an embodiment, be employed to remove a plurality of undesirable materials, for instance, within the same vessel or its branches, from multiple vessels within the same vascular bed (e.g. left and right pulmonary arteries), from different vascular beds (e.g. pulmonary artery and iliofemoral veins), or a combination thereof. In such an embodiment, after the first undesirable material has been removed, the suction force may be deactivated. The next undesirable material to be removed may then be located, for example, using an appropriate imaging modality. Suction cannula **71** may thereafter be advanced to the location of this second undesirable material, and the suction force reactivated as above until this second undesirable material may be removed. The cycle may be repeated until each undesirable material at the various identified locations has been removed. Once all undesirable material has been removed, an appropriate procedure to prevent the development of or migration of new material, such as placement of an inferior vena cava filter, may be performed.

[0103] The method of the present invention may also be employed in combination with a balloon embolectomy catheter or other devices suitable for dislodging clots or other undesirable material from a cannula or a vessel. For example, should an undesirable material be lodged within suction cannula **71**, a balloon catheter can be inserted through, for instance, a side port, similar to port **51** in FIG. 5, of suction cannula **71** and advanced past the lodged undesirable material. The balloon catheter may subsequently be inflated distal to the undesirable material. Once inflated, the suction force may be activated and the inflated catheter withdrawn along the suction cannula **71** to dislodge the undesirable material its location of obstruction. In a situation where the undesirable material may be adherent to a vessel wall, or for some other reason cannot be dislodged by simply applying suction to the site of interest, the balloon catheter can be inserted through the side port of suction cannula **71**, advanced past a distal end of cannula **71**, and past the adherent undesirable material. The balloon catheter may then be inflated distal to the undesirable material. Once inflated, the suction force may be activated and the inflated catheter withdrawn along the suction cannula **71**. As it is

withdrawn, the balloon catheter can act to drag the undesirable material into suction cannula 71.

[0104] The method of the present invention may further be employed in combination with a distal protection device (not shown), such as a netting device, designed to be positioned downstream of the undesirable material, when removal may be performed within a vessel having arterial flow. In particular, with suction cannula 71 positioned upstream of the undesirable material, the netting device may be inserted through a side port in suction cannula 71, advanced past the undesirable material to a downstream location. The netting device may then be deployed to an open position approximating the diameter of the vessel. The deployed netting device may then act to entrap any material that may be dislodged from the site of interest and pushed downstream by the fluid flow. In the absence of the netting device, a dislodged material may be pushed downstream and may be lodged in a more life threatening location.

[0105] It is evident from the above description that the systems, including the various components, and methods of the present invention can act to remove clots and other types of undesirable material from the circulation, particularly from medium to larger vessels and heart chambers. Important to achieving this includes the ability of the operator to perform substantially en bloc removal of the undesirable material without significant fragmentation from the site of interest. Such a protocol may only be achieved previously with invasive, open surgery. In addition, by providing a system with components to permit aspirated fluid from the site of interest to be reinfused back to the patient, the system of the present invention allows a sufficiently and relatively large suction cannula to be employed for the removal of a relatively large undesirable material 15 in substantially one piece, without fragmentation. Furthermore, by providing a definitive mechanical treatment to the problem, the systems and methods of the present invention provide an attractive alternative to treatments, such as thrombolysis, which may not be an option or may be ineffective for many patients, and which may carry a significant risk of major complications. As such, the systems and methods of the present invention now provide a significant contribution to the field of cardiovascular medicine and surgery, particularly thromboembolic disease.

[0106] Although references have been made in connection with surgical protocols, it should be appreciated that the systems and methods of the present invention may be adapted for use in connection with non-surgical protocols, and in connection with any vessel capable of permitting fluid flow therethrough and capable of being obstructed. For instance, the system of the present invention may be adapted for use in connection with clearing obstructed oil pipelines, water pipes, and air ducts, among others.

[0107] Another embodiment of the system is shown in FIGS. 9-11A. FIG. 9 depicts an improvement on the suction cannula 10 described above. The improved suction cannula 100 of this embodiment is designed to be used together with the previously described circuit in the various embodiments above. The cannula 100 includes a proximal end 102 and a distal end 104. The cannula 100 may also have a reinforcement element 106 along the shaft extending from the proximal end 102 to a selected distance distal to the distal most end 104. The distal end 104 of the cannula 100 may transition from a collapsed state (not shown) into an expandable funnel shape 108. The expandable funnel 108 of the

cannula 100 may include independent strips 110, reinforcement arms 112, and a jacket 114. The cannula 100 may have a low friction lining along the lumen 116. The low friction lining may include a material such as PTFE, ETFE, and may also include the use of a lubricated or hydrophilic coating. The size of the cannula 100 for this embodiment is conceived to range from 12 F up to 24 F. The cannula 100 may be comprised of a urethane material.

[0108] The cannula 100 may also be pre-shaped to provide a predetermined bend in the cannula. An advantage of pre-bending the cannula 100 is to enhance the usability and more easily track the cannula 100 around tortuous vasculature and target a clot that is difficult to reach with a straight cannula or a clot that is attached to a vessel wall. For example, if the cannula 100 is intended to be used in or around the heart, such as when the user wants to access the Right Ventricle and must pass through the tricuspid valve, the user may have to guide the cannula 100 from the insertion site, such as in the groin area, around the tortuous vasculature leading from the insertion site to the treatment site. A pre-determined shape to the cannula 100 will provide the user with easier maneuverability when placing the cannula 100 for treatment, when combined with an outer sheath 146. The outer sheath 146 in this type of situation is designed to keep the cannula 100 straight until the user is at the area where the shaped cannula 100 is required. The user will then retract the outer sheath 146, allowing for the cannula 100 to assume its shaped configuration and access the intended area. The outer sheath 146 will be described in greater detail below.

[0109] The reinforcement element 106 may be in the shape of a coil and comprise a stiff material, such as stainless steel, nitinol, or other metal, that provides rigidity and trackability. The pitch of the reinforcement element 106 can also have an effect on the stiffness of the cannula 100. The tighter the pitch of the reinforcement element 106, the stiffer the cannula 100 is going to be. The more loose the pitch of the reinforcement element 106 is, the less stiff the cannula 100 is going to be. The advantage to having a stiffer cannula is increased durability and a cannula 100 that is easier to advance in the vasculature. The advantage of a less stiff cannula 100 is that the cannula 100 is more flexible, thereby making the cannula more easily maneuverable. There are multiple embodiments of the reinforcement element 106 that can be used with the cannula 100. In one embodiment, the reinforcement element 106 can be circular. In a preferred embodiment, the reinforcement element 106 is flat, instead of circular. There are several advantages to using a flat reinforcement element 106 instead of a circular reinforcement element 106, but most importantly, the flat reinforcement element lessens the high-point of the cannula 100. With a lessened high-point, the cannula 100 can have a larger inner diameter while still keeping the same French size.

[0110] The expandable funnel 108 may include independent strips 110, reinforcement arms 112, and a jacket 114 that together provide a structure that allows for en bloc removal of undesirable material. The plurality of independent strips 110 are created by removing material from the distal end of the cannula 100. The independent strips 110 and low friction layer 126 therefore combine to create a continuous inner pathway from the distal most end of the cannula 100 to the proximal most end of the cannula 100. In FIG. 9A, four strips 110 are depicted; however it is con-

ceivable that a minimum of two strips **110** or more than four strips **110** may be used. The strips **110** may be designed to pivot between a closed position, where the strips **110** are substantially next to one another, and an open position, where the strips **110** are flared in a funnel shape as shown in FIG. 9A. The strips **110** may include radiopaque markers to aid in the visualization of the funnel **108** under medical imaging. However, the reinforcement arms **112** may be radiopaque depending on their material, such as nitinol, in which case additional radiopaque markers may not be necessary.

[0111] Referring now to FIG. 9A-A, a cross-sectional view along the shaft of the cannula **100** is shown. The cannula **100** is comprised of an outer shaft layer **120**, a reinforcement layer comprising a reinforcement element **106**, an inner shaft layer **124**, and a low friction layer **126** lining the lumen **116**. There are several embodiments of the cannula **100** disclosed in this invention, each having a unique method of manufacturing.

[0112] In one embodiment (as shown in FIG. 17), the cannula **100** is created using urethane. First, a mandrel is dipped into a urethane solution **201**. Next, a reinforcement element **106** is placed **202** over the urethane dipped cannula **100**. After the reinforcement element **106** is placed over the urethane-dipped cannula, the cannula **100** is cured **203**, thereby securing the reinforcement element **106** to the cannula shaft **116**. Next, the cannula **100** and reinforcement element **106** are dipped into urethane once again and cured **204**, sealing the reinforcement element **106** to the shaft of the cannula **100**. In another embodiment, an outer sheath **146** is created using the same steps above. The outer sheath **146** is used in an embodiment to expand a funnel **108** at the distal end of the cannula **100**, and is described in greater detail below.

[0113] In yet another embodiment (as shown in FIG. 18), a PTFE (Teflon) lined cannula is disclosed. The cannula **100** may be manufactured by a dipping process (as commonly known in the art) in which each layer is independently dipped into a specific material, allowed to cure, and then dipped again into either the same material or another material to create the next layer. Teflon tubing, which comprises the inner shaft layer **124**, will create an inner surface of the cannula **100** that has less friction than a traditional urethane inner surface. Next, the Teflon tubing is dipped into urethane **205** or some other pliable material. Next, the reinforcement element **106** is placed over the urethane-dipped Teflon tubing **206**. As described above, the reinforcement element **106** may extend from the proximal most end of the cannula, thereby providing additional support and strength of the connection point between the cannula **100** and circuit, to a selected distance proximal to the expandable funnel **108**. After the reinforcement element **106** has been placed on the urethane-dipped Teflon tubing, the cannula is cured **207**, thereby securing the reinforcement element **106**. Lastly, the cannula **100** is dipped into urethane again and cured **208** to create the outer shaft layer **120**.

[0114] In yet another embodiment (as shown in FIG. 19), a hydrophilically coated cannula is provided. First, a urethane dip is performed over a mandrel **209**. Next, a reinforcement element **106** is placed over the urethane dip **210** and is cured **211** in order to keep the reinforcement element **106** in place on the cannula shaft **116**. The cannula **100** and reinforcement element **106** are then once again dipped into urethane **212** and cured **213**. Finally, the cured cannula **100** is dipped into

a hydrophilic solution **214**, thereby coating both the inside and the outside of the cannula **100**. Hydrophilically coating both the inner luminal wall and outer wall of the cannula **100** has several advantages. For example, the hydrophilic coating allows for a lumen that has less friction than a cannula **100** with a urethane dip, thereby allowing the clot to move more easily through the cannula shaft. The hydrophilic coating creates an outer surface of the cannula that has less friction as a cannula with a urethane outer shaft, thereby allowing for easier use of an outer sheath **146** to collapse and expand the funnel **108** at the distal end of the cannula, which is described in greater detail below.

[0115] In yet another embodiment (as shown in FIG. 20), a urethane cannula **100** with a hydrophilically coated expandable funnel **108** is disclosed. First, a urethane dip is performed over a mandrel **215**. Next, a reinforcement element **106** is placed **216** over the Urethane-dipped cannula **100**. After the reinforcement element is placed on the Urethane-dipped cannula **100**, the cannula **100** is cured **217** in order to keep the reinforcement element in place. After the cannula **100** is cured, the cannula **100** and reinforcement element **106** are again dipped in urethane **218** and cured **219**. Next, only the expandable funnel **108** of the cannula **100** is dipped in a hydrophilic coating **220**, leaving the shaft of the cannula with a Urethane lining. The advantage of this embodiment is the varying coefficient of friction between the expandable funnel **108**, which has a first coefficient of friction and the lumen of the cannula **100**, which has a second coefficient of friction. The inner surface **260** of the expandable funnel **108** may have a lower coefficient of friction than the lumen, thereby allowing the undesirable material to more easily move, travel, or exit the expandable funnel **108**. An advantage of the lumen having a higher coefficient of friction than the expandable funnel **108** is that the undesirable material may move, travel, or exit along the lumen while remaining en bloc, thereby reducing breakage of the undesirable material into smaller pieces.

[0116] Referring now to FIG. 9B-B, a cross-sectional view of the expanded funnel **108** is shown. The funnel **108** is comprised of a jacket **114**, reinforcement arms **112**, strips **110**, and the low friction layer **126**. The funnel **108** is manufactured by altering the materials used during the dipping process of the cannula **100**. For example, the low friction layer **126** of the shaft extends all the way to the distal most end of the funnel **108**—thereby creating a continuous pathway along the entire cannula **100**. The strip **110** layer is comprised of the same urethane material used to create the inner shaft layer **124**, except material is removed between each strip **110** so that they may move independently of one another. Next, the reinforcement arms **112**, as described in more detail below, are placed on top of the strips **110**. Lastly, the funnel is dipped into the urethane material again to create the jacket **114**.

[0117] To aid in the deployment of the strips **110** into a flared position the cannula **110** may include reinforcement arms **112**. As shown in FIGS. 10-10D, the reinforcement arms **112** may be comprised of a shape memory material, such as nitinol. The reinforcement arms **112** can be placed on top of each strip **110**, but can act to expand the expandable funnel **108** without the use of the strips **110** as mentioned above. The reinforcement arms **112** are able to pivot between a closed position (not shown) and an open position. The reinforcement arms **112**, as depicted in FIG. 10, may have a distal end and a proximal end. The proximal end of

the reinforcement arms **112** may be connected by a proximal collar **118**. The proximal collar **118** provides support and a connection point for each of the reinforcement arms **112**. The proximal collar **118** may be placed a selected distance proximal of the expandable funnel **108**. The distal end of the reinforcement arms **112** are designed to end a selected distance proximal to the distal most end of the strips **110**. To expand the funnel **108** shaped distal end, the system may include, in this embodiment, an outer sheath **146** is circumferentially situated about distal end of cannula **100**, similar to sheath **21** of the above described embodiment in FIGS. 2A-2C. The outer sheath **146** may be designed to slide toward, as well as away, from the funnel **108**. In that way, when the distal end **104** of cannula **100** is positioned at the site of interest (not shown), and sheath may be either retracted (i.e., slid back from the distal end **104**) or the cannula **100** may be advanced (i.e., slid past the distal end of the sheath) so funnel **108** may be exposed and expanded into the desired shape in order to engage undesirable material. The funnel **108** may expand due to the expansion of the reinforcement arms **112**. The reinforcement arms **112** are comprised of shape memory material being pre-shaped in an expanded configuration. The degree of expansion of funnel **108** may relate to the degree the reinforcement arms **112** have been pre-shaped. To collapse funnel **108**, sheath may be advanced toward the distal end **104** and over the funnel **108** forcing the reinforcement arms **112** to collapse. Thereafter, cannula **100** may be maneuvered from the site of interest.

[0118] The proximal collar **118** and reinforcement arms **112** may have several different embodiments, as seen in FIGS. 10-10D. In one embodiment, the reinforcement arms **112** are made with rounded tips at the distal end of the reinforcement arms **112** (as shown in FIGS. 10 and 10B). In addition to helping with the collapse of the funnel **108**, the rounded tips in this embodiment make the reinforcement arms **112** less traumatic, resulting in less injury to the vessel wall. In another embodiment, the reinforcement arms **112** can be made with an oval tip at the distal end. The oval tip serves multiple purposes, including being less traumatic to the vessel wall and helping to collapse the funnel **108** since the oval tips are more easily stackable. In another embodiment, the reinforcement arms **112** are made having a lesser radius than the other embodiments (as shown in FIG. 10A). The smaller radius of the reinforcement arms **112** in this embodiment would make collapse of the funnel **108** easier. In another embodiment, the reinforcement arms **112** are made in a "T-Tip" formation, with the tip of the reinforcement arms **112** being substantially perpendicular to the shaft of the reinforcement arms **112** (as shown in FIG. 10C). The configuration of the reinforcement arms **112** in this embodiment would help in the reinforcement arms **112** being able to lay flat, and thus, helping to collapse the funnel **108**. In another embodiment, the "T-Tip" configuration of the previous embodiment is modified, with the shaft of the reinforcement arms **112** being thinner than the previous embodiment and the "T-Tip" of the distal end of the reinforcement arms **112** being larger than the previous embodiment (as shown in FIG. 10D). This configuration would allow for easier stacking of the reinforcement arms **112** and thus, easier collapse of the expandable funnel **108**.

[0119] The jacket **114** of the expandable funnel **108** may extend along the space between the strips **110** when the funnel **108** is in the expanded position. When the funnel **108**

is in a compressed state the jacket **114** material will no longer be taut between each strip **110** but instead have some slack and be compressed towards (not shown) the lumen **116**. The jacket **114** may be comprised of the same material as the cannula **100**, such as urethane. Unlike the lumen **116** of the cannula **100**, the jacket **114** may not be comprised of a low friction lining along the inner surface. The inner surface of the expandable funnel **108** may be comprised of different materials having varying degrees of friction. For example, the inner surface of the strips **110** may be lined with a material, such as Teflon, with a low degree of friction, whereas the inner surface of the jacket **114** may be comprised of a urethane material that has a relatively higher degree of friction. When the funnel is in the expanded state the jacket **114**, comprised of a higher friction material, will be between each strip **110**, comprised of a material with a lower degree of friction. The varying degree of friction along the inner surface of the expandable funnel **108** enhances the creation of a vortex flow. As fluid flows into and along the inner surface of the funnel **108** the interface between varying degrees of friction increases the laminar flow circumferentially along the interior surface of the funnel **20** to generate and enhance a vortex flow into the distal end of suction cannula **100**.

[0120] As shown in FIG. 11A-11C, another embodiment of the suction cannula **10** is shown. In this embodiment, the suction cannula is comprised of a piece of Teflon tubing **126**, an inner shaft layer **124**, and an outer shaft layer **120** with a reinforcement element **106**. The distal most end of the inner shaft layer **124** extends a selected distance beyond the distal most end of the outer shaft layer **120**, thereby creating a stepped distal end **138** of the suction cannula.

[0121] As seen in FIG. 11B, this embodiment of the suction cannula may also comprise an expandable member **108**. The expandable member **108** may be comprised of a funnel shape or any other shape that enhances removal of unwanted material through the suction cannula. The expandable member **108** may further be comprised of a plurality of reinforcement arms **112** attached to a proximal collar **118**. The reinforcement arms **112** may be comprised of shape memory metal, a polymer material or any other materials known in the art. The reinforcement arms **112** may be hinged or otherwise movably connected to the proximate collar **118** such that the reinforcement arms **112** have an expanded state and a compressed state. The proximate collar **118** and reinforcement arms **112** are secured to the suction cannula by coaxially aligning the proximate collar **118** on top of or over the stepped distal end **138** of the suction cannula.

[0122] FIG. 11-11C depicts the suction cannula **10**, stepped distal end **138** of the cannula and the attachment of the expandable member **108** to the stepped distal end **138**. The method of manufacturing the cannula **10** begins by first by taking a tube **126**, such as a Teflon tube commonly known in the art and priming it in order to make it capable of having urethane adhere to it. Next, the tubing **126** is dipped in urethane in order to make the inner shaft layer **124** of the cannula. Next, a reinforcement coil **106** is wrapped around the inner shaft layer **124**. The reinforcement coil **106** is meant to provide rigidity and stiffness to the cannula **10**, so insertion and navigation within the lumen is easier. After the reinforcement coil **106** is wrapped around the inner shaft layer **124**, the suction cannula **10** is dipped into urethane once again in order to fix the reinforcement coil **126** to the suction cannula **10** and also creates the outer shaft layer **120**.

This second dip in urethane creates the outer shaft layer **120**. Next, the stepped distal end **138** is formed by using a flared mandrel that matches the geometry of the distal most end of the inner shaft layer (roughly at 0.5" distance), the cone at the end of the flared mandrel having a diameter of about 14 mm to create the inner diameter of the expandable member **108**. The shaft of the suction cannula is created with enough space left at the distal most end to slide the proximate collar **118** onto the space left at the distal most end of the inner shaft layer in order to be affixed to the distal most end of the inner shaft layer. The tubing **126** may or may not extend to the distal most end of the inner shaft layer.

[0123] The thickness of the walls of the expandable member **108** can vary based on the desired flexibility and/or stiffness of the expandable member. If the operator desires a thicker wall for the expandable member **108**, the distal most end of the cannula will be dipped into urethane to create additional layers on the expandable member **108**. This will be done until the walls of the expandable member are to the stiffness that the operator desires. The preferred thickness of the wall of the expandable member **108** is one that allows the expandable member **108** to be flexible enough to collapse, without being so thin that the walls become susceptible to damage during procedures.

[0124] FIGS. **11B-11C** depict the affixing of the proximate collar **118** and reinforcement arms **112** to the suction cannula **10**. The reinforcement arms **112** are dipped into urethane in order to affix the reinforcement arms **112** and proximate collar **118** to the cannula **10**. The urethane layer **136** forms around and in between the reinforcement arms **112** of the proximate collar **118** in order to form the funnel **20** at the distal end of the cannula. The urethane layer **136** also covers a portion of the distal end of the cannula **100**, thus fixing the proximate collar **118** and reinforcement arms **112** to the cannula. In addition, a fenestration hole **130** may be provided on the expandable funnel **108**. An advantage of having a fenestration hole **230** (as shown in FIG. **9A**) on the expandable funnel is to reduce the pressure associated with using suction through the cannula **100**.

[0125] FIGS. **12-16** depict yet another embodiment of the device in which multiple suction cannulas may be used together to create a system for removing undesirable material. The outer suction cannula **130** may be sized up to 24 F and consist of any of the above described suction cannula embodiments. The inner suction cannula **132** will be smaller, such as 12 F, and may also consist of any of the above described suction cannula embodiments. The inner suction cannula **132** is sized such that it can independently coaxially move within the outer suction cannula **130**. The circuit may comprise a utility port (not shown) along the proximal end of the outer suction **130** sized to allow the inner suction cannula **132** to be inserted into the lumen of the outer cannula **130**. The inner suction cannula **132** may be connected to either a secondary vacuum/suction force, or alternatively may be connected to the same circuit pump that is described above. The advantage of using a smaller inner suction cannula **132** is to provide a system that allows the user to easily maneuver the inner suction cannula **132** into smaller vasculature that the outer suction cannula **130** could not fit. It is common for undesirable material to be located along large sections of vasculature. Often time the undesirable material extends into smaller diameter vessels that do not easily permit a 24 F sized device, such as the outer suction cannula **130**. The smaller inner suction cannula **132**

is sized such as it can more easily fit into these smaller diameter vessels and capture the undesirable material.

[0126] It is conceived that during a method of using the system of this embodiment (as shown in FIGS. **16** and **21**), the outer suction cannula **130** will be first placed a selected distance proximal of the treatment site. The treatment site may include vessels of varying degree of diameter, ranging from a large diameter sufficient to place a 24 F device to a smaller diameter in which a smaller device, such as a 12 F (or smaller) cannula, can fit. The user may use this system to remove undesirable material substantially en bloc through the outer suction cannula **130** and/or inner cannula **132**. The user may then determine, using commonly known medical imaging techniques, such as CT or X-Ray if any undesirable material is located in a vessel that is too small for the outer section cannula **130** to be placed **221**. If it is determined that additional treatment of smaller diameter vessels is required, the user may then insert the inner suction cannula **132** into the utility port of the circuit (not shown) **222**. The inner suction cannula **132** may be connected to a suction force, either independent from the circuit or the same pump as the outer suction cannula **130**. As shown in step **223**, the proximal end of the inner suction cannula **132** (not shown) may be connected to the circuit so that the blood removed through the inner suction cannula **132** will be recirculated back into the body through the return cannula of the circuit. After the inner suction cannula **132** is connected, the user may coaxially advance **224** the inner suction cannula **132** along the lumen of the outer suction cannula **130** until the expandable funnel of the inner cannula **132** is a selected distance distal of the expanded funnel of the outer cannula **130**. The user may then advance **225** the inner suction cannula **132** beyond the outer cannula **130** into the smaller diameter vasculature without expanding the expandable funnel **108** by keeping the outer sheath **146** advanced to the distal end of the inner cannula **132**. When the inner cannula **132** is at the target site, the outer sheath **146** can be retracted in a proximal direction, expanding the expandable funnel **108**. The user may then activate suction **226** for both the outer cannula **130** and the inner cannula **132** simultaneously, thereby creating a sufficient suction force to draw the undesirable material in the smaller diameter vessels en bloc into the inner suction cannula **132**. Alternatively, one of either the inner or outer cannula may be activated to apply suction in a specific vessel area. Sequential activation of suction to one of the cannulas may be beneficial in targeting specific clot masses. Both the inner suction cannula **132** and the outer suction cannula **130** have an expandable funnel **108** at the distal end of each respective cannula. When suction is applied, the undesirable material moves into the selected cannula or both cannulas substantially en bloc. The clot mass is drawn through the cannulas by the force of the suction and into the reservoir/filter **227** before the filtered blood is returned to the body. After clot removal is accomplished and blood is returned to the patient, the cannulas may be removed from the patient **228**.

[0127] In an alternative embodiment of the method of using the suction cannula described above, an optional mechanical thrombectomy and/or chemical fluid delivery assembly may be used in conjunction with the procedure. As an example, an expandable compliant or non-compliant balloon catheter may be inserted through either in the inner or outer cannula and advanced through the funnel and clot mass. Once distal of the clot mass, the balloon may be

inflated and used to drag the clot from the vessel wall and toward the funnel for removal. Clot segments not captured within the smaller funnel may be captured by the larger more proximal funnel. Alternatively or in addition, a fluid delivery catheter may be advanced into the clot for the delivery of a thrombolytic agent to facilitate the removal of more mature or difficult to remove clots. By utilizing the inner cannula as a conduit for mechanical/chemical thrombectomy devices, more distal clot can be targeted for removal through a combination therapy of suction removal augmented by clot dissolution, dislodgement and/or maceration treatment.

[0128] FIGS. 13-14A-A show a head-on view, a partial plan view and a cross-sectional view of the multiple suction cannula embodiment, respectively, showing the inner suction cannula 132 within the lumen of the outer suction cannula 130. In one embodiment, the inner suction cannula 132, as well as the outer suction cannula 130 have an outer sheath 146 circumferentially disposed along the shaft of each respective suction cannula. The outer sheath 146, much like in the earlier cannula embodiments, is used in order to facilitate the collapse and expansion of the expandable funnel 108 of the outer cannula 130 and inner cannula 132. The outer sheath 146 is advanced distally over the expandable funnel 108 in order to collapse the funnel 108 and is retracted proximally in order to expand the expandable funnel 108. The collapse of the expandable funnel 108 by the outer sheath 146 aids in the advancement of not only the outer cannula to the site of the undesirable material, but will also aid in the advancement of the inner suction cannula 132 through the lumen of the outer suction cannula 130 and to the site of the undesirable material to be removed.

[0129] FIGS. 15-15D-D show a plan view and cross-sectional views at points A-A, B-B, C-C, and D-D, respectively. FIG. 15A-A shows a cross-sectional view taken at point A-A, a point before the outer sheath 146 146 reaches the distal end of the outer suction cannula 130. This view shows the outer sheath 146 146 over the outer suction cannula 130, the outer suction cannula 130, the outer sheath 146 146 over the inner suction cannula, and the inner suction cannula. FIG. 15B-B shows a cross-sectional view taken at point B-B, a point after the outer sheath 146 146 of the outer suction cannula 130, but before the expandable funnel 108 of the outer suction cannula 130. This view shows the outer suction cannula 130, the reinforcement element 106 of the outer suction cannula 130, the outer sheath 146 146 of the inner suction cannula 132, the reinforcement element 106 of the inner suction cannula 132, as well as the inner suction cannula 132. FIG. 15C-C shows a cross-sectional view taken at point C-C, a point after the outer suction cannula 130, but before the end of the outer sheath 146 146 of the inner suction cannula 132. This view depicts the outer sheath 146 146 of the inner suction cannula 132, the reinforcement element 106 of the inner suction cannula 132, and the inner suction cannula 132. FIG. 15D-D is a cross-sectional view taken at point D-D, a point at the expandable funnel 108 of the inner suction cannula. This view depicts the reinforcement arms 112 of the expandable funnel 108 of the inner suction cannula 132, as well as the urethane jacket 114 that is composed between the reinforcement arms 112 of the expandable funnel 108.

1. A system for removing undesirable material from within a vessel, the system comprising:

- a first cannula, the first cannula comprising:
 - a proximal end;

- a distal end;

- a shaft comprising an inner layer, a reinforcement element, and an outer layer, and

- an expandable distal end formed in part by extensions of the outer layer of the shaft, the expandable distal end further comprising reinforcement arms on top of the outer layer extensions, the expandable distal end further comprising a jacket between the outer layer extensions, and the expandable distal end capable of expanding to a diameter greater than the proximal end and capturing the undesirable material from the vessel;

- a second cannula, the second cannula having a proximal end and a distal end, the distal end of the second cannula is placed in a spaced relation to the distal end of the first cannula;

- a pump, the pump being in fluid communication with the proximal of the first cannula and the proximal end of the second cannula; and

- a filter, the filter placed in fluid communication with the proximal end of the first cannula.

2. The system of claim 1, further comprising an outer sheath, the outer sheath capable of being advanced towards the distal end of the first cannula or retracted towards the proximal end of the second cannula.

3. The system of claim 1, wherein the reinforcement element comprises a flat coil allowing for a greater increased luminal diameter, as compared to a round wire.

4. The system of claim 1, wherein the expandable distal end of the first cannula further comprises a proximal collar connected to the reinforcement arms.

5. The system of claim 1, wherein the inner surface of the inner layer of the first cannula shaft has a higher friction coefficient than the inner surface of the expandable distal end.

6. The system of claim 1, wherein the inner surface of the inner layer of the first cannula shaft has a lower friction coefficient than the inner surface of the expandable distal end.

7. The system of claim 1, wherein the expandable distal end further comprises a fenestration hole.

8. The system of claim 1, further comprising a third cannula capable of being advanced through a lumen of the first suction cannula.

9. A system for removing undesirable material from within a vessel, the system comprising:

- a first cannula, the first cannula comprising:

- a proximal end;

- a distal end;

- a shaft comprising an inner layer, a reinforcement element, and an outer layer;

- an expandable distal end comprising a collar connected to at least two pre-shaped reinforcement arms extending away from the first cannula in an expanded position, a jacket extending between the at least two pre-shaped reinforcement arms, and the expandable distal end capable of expanding to a diameter greater than the proximal end and capturing the undesirable material from the vessel;

- a second cannula comprising a proximal end and a distal end, the distal end of the second cannula is placed in a spaced relation to the distal end of the first cannula;

- a pump, the pump capable of simultaneously performing both a suction force and a driving force, the pump being

in fluid communication with the proximal of the first cannula and the proximal end of the second cannula;
 a filter, the filter placed in fluid communication with the proximal end of the first cannula; and
 a reservoir for collection of the undesirable material and residual fluid that is captured during collection of the undesirable material.

10. The system of claim **9**, further comprising an outer sheath, the outer sheath capable of being advanced towards the distal end of the first cannula or retracted towards the proximal end of the second cannula.

11. The system of claim **9**, wherein the inner surface of the inner layer of the first cannula shaft has a higher friction coefficient than the inner surface of the expandable distal end.

12. The system of claim **9**, wherein the inner surface of the inner layer of the first cannula shaft has a lower friction coefficient than the inner surface of the expandable distal end.

13. The system of claim **9**, wherein the outer layer of the first cannula shaft has a lower friction coefficient than the expandable distal end.

14. The system of claim **9**, wherein the expandable distal end further comprises a fenestration hole.

15. The system of claim **9**, further comprising a third cannula capable of being advanced through a lumen of the first suction cannula.

16. A method for removing undesirable material from a treatment site within a vessel, the method comprising:

placing a first cannula for removing undesirable material from within a vessel, the first cannula comprising:

a proximal end;

a distal end;

a shaft comprising an inner layer, a reinforcement element, and an outer layer;

an expandable distal end comprising a collar connected to at least two pre-shaped reinforcement arms extending away from the first cannula in an expanded position, the expandable distal end capable of expanding to a diameter greater than the proximal end and capturing the undesirable material from the vessel; and

placing a distal end of a second cannula in a spaced relation to the distal end of the first cannula;

activating a pump, the pump being in fluid communication with the proximal of the first cannula and the proximal end of the second cannula; and

filtering the undesirable material through a filter.

17. The method of claim **16**, further comprising the step of:

advancing a third cannula through a lumen of the first cannula, the third cannula comprising a collar connected to at least two pre-shaped reinforcement arms extending away from the third cannula in an expanded position.

* * * * *