

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization

International Bureau



WIPO | PCT



(10) International Publication Number

WO 2013/142323 A1

(43) International Publication Date  
26 September 2013 (26.09.2013)

(51) International Patent Classification:  
*A61F 2/16* (2006.01)      *A61F 2/76* (2006.01)  
*A61F 2/14* (2006.01)

(21) International Application Number:  
PCT/US2013/032054

(22) International Filing Date:  
15 March 2013 (15.03.2013)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:  
61/613,929      21 March 2012 (21.03.2012)      US

(71) Applicant: POWERVISION, INC. [US/US]; 260 Harbor Boulevard, Belmont, CA 94002 (US).

(72) Inventor: MATTHEWS, Gregory, Vinton; 260 Harbor Boulevard, Belmont, CA 94002 (US).

(74) Agents: ZLOGAR, Thomas, M. et al.; Shay Glenn LLP, 2755 Campus Drive, Suite 210, San Mateo, CA 94403 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM,

AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report (Art. 21(3))



WO 2013/142323 A1

(54) Title: INTRAOCULAR LENS DELIVERY SYSTEMS AND METHODS OF USE

(57) Abstract: Intraocular lens delivery devices and methods of use.

## INTRAOCULAR LENS DELIVERY SYSTEMS AND METHODS OF USE

### CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of U.S. Prov. App. No. 61/613,929, filed March 5 21, 2012, the disclosure of which is incorporated by reference herein.

[0002] This application is related to and incorporates by reference herein the disclosures of the following U.S. patent applications: U.S. App. No. 13/180,427, filed July 11, 2011, and U.S. App. No. 13/427,617, filed March 22, 2012.

### 10 INCORPORATION BY REFERENCE

[0003] All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

### 15 BACKGROUND

[0004] Intraocular lenses are positioned within a patient's eye, such as in the anterior chamber or posterior chamber. After making a small incision in the eye, a physician typically positions a distal opening of a delivery device within or adjacent to the opening. The physician then delivers the intraocular lens out of the delivery device, through the opening, and into the 20 target location within the eye. In some procedures, but not all, an intraocular lens is delivered into a native capsule after the native lens has been removed.

[0005] Some intraocular lenses, because of their size and/or their configuration, and possibly the desired incision size, need to be reconfigured and/or have at least a first portion reoriented with respect to a second portion to be delivered into an eye. When some intraocular lenses are 25 advanced through a delivery device and/or delivered out of the delivery device, forces on the intraocular lens can damage the intraocular lens.

[0006] What are needed are delivery systems and methods of use that can deliver an intraocular lens without damaging the intraocular lens.

### SUMMARY OF THE DISCLOSURE

30 [0007] One aspect of the disclosure is a method of deploying an intraocular lens into an eye, comprising providing an intraocular lens within a delivery device; at least partially plugging a gap between the intraocular lens and an inner surface of the delivery device; and delivering a fluid into the delivery device to deploy the intraocular lens from the delivery device and into an eye. In some embodiments at least partially plugging a gap reduces the amount of fluid that

flows passed the intraocular lens in the delivery device. In some embodiments at least partially plugging a gap allow for an increase in fluid pressure in the delivery device proximal to an optic portion of the intraocular lens. In some embodiments at least partially plugging a gap increase a pressure differential in the delivery device between a location proximal to an optic portion of the 5 intraocular lens and a location distal to the intraocular lens. In some embodiments at least partially plugging a gap comprises at least partially plugging a gap that is disposed radially between the intraocular lens and an inner surface of the delivery device. In some embodiments at least partially plugging a gap between the intraocular lens and an inner surface of the delivery device comprises at least plugging a gap that exists between a trailing haptic and an inner surface 10 of the delivery device. In some embodiments the method further comprises reconfiguring a plugging element while delivering the fluid into the delivery device. Reconfiguring the plugging element can act to form a seal between the plugging element and an inner surface of the delivery device. Reconfiguring the plugging element can include unrolling the plugging element.

**[0008]** In some embodiments delivering a fluid into the delivery device to deploy the 15 intraocular lens from the delivery device comprises delivering a fluid through a porous material.

**[0009]** One aspect of the disclosure is a method of deploying an intraocular lens into an eye, comprising providing an intraocular lens within a delivery device; at least partially plugging a gap disposed radially between the intraocular lens and an inner surface of the delivery device; and delivering a fluid into the delivery device to deploy the intraocular lens from the delivery 20 device. In some embodiments at least partially plugging a gap disposed radially between the intraocular lens and an inner surface of the delivery device comprises at least partially plugging a gap disposed radially between a haptic extending generally longitudinally through the delivery device and an inner surface of the delivery device.

**[00010]** One aspect of the disclosure is a method of deploying an intraocular lens into an eye, 25 comprising providing an intraocular lens within a delivery device; delivering a fluid into the delivery device to deploy the intraocular lens from the delivery device; and increasing fluid pressure proximal to at least an optic portion of the IOL, wherein increasing the fluid pressure is a step different than delivering the fluid into the delivery device. In some embodiments increasing fluid pressure proximal to at least an optic portion of the IOL comprises plugging a 30 gap between the IOL and an inner surface of the delivery device.

**[00011]** One aspect of the disclosure is an apparatus for deploying an intraocular lens into an eye, comprising: an intraocular lens delivery device with an intraocular lens disposed therein; a support device adapted to be disposed within the delivery device, the support device having a lumen therein adapted to allow fluid to flow therethrough; and a plug element disposed

relative to the support device such that it is adapted to at least partially plug a gap between an intraocular lens positioned in the delivery device and an inner surface of the delivery device.

[00012] In some embodiments the support device is secured to the plug element. The plug element can have a proximal portion secured to the support device. In some embodiments the 5 plug element is a tubular element. In some embodiments the plug element is open at a distal end after deployment. In some embodiments the plug element has a fluid flow restriction proximal to a distal end of the plug element. In some embodiments the plug element is everted at a distal end. In some embodiments the plug element is flexible. In some embodiments the plug element is porous. In some embodiments the plug element is adapted to be reconfigured in response to 10 fluid flow through the lumen. Only a distal portion of the plug element can be adapted to be reconfigured. In some embodiments the plug element has a flow restriction proximal to a distal end of the plug element. The plug element can have a portion distal to the flow restriction that is adapted to be reconfigured.

[00013] In some embodiments the plug element is open at a distal end. In some embodiments 15 the plug element is an ePTFE tube. In some embodiments a distal portion of the support element is oriented towards an inner wall of the delivery device. In some embodiments a distal portion of the support element is oriented away from a longitudinal axis of a proximal portion of the support element. In some embodiments a trailing haptic extends proximal relative to an optic portion of the intraocular lens. The plug element can be disposed radially between the 20 intraocular lens and an inner surface of the delivery device. In some embodiments the apparatus further comprises a vent adapted to vent air from inside the apparatus.

[00014] One aspect of the disclosure is an apparatus for deploying an intraocular lens into an eye, comprising: an intraocular lens delivery device and an intraocular lens disposed therein; a support device adapted to be disposed within the delivery device, the support device having a 25 lumen therein adapted to allow to fluid to flow therethrough; and a flexible plug element secured to the support device, the plug element adapted to at least partially plug a gap between an intraocular lens positioned in the delivery device and an inner surface of the delivery device when fluid is flowed into the lumen.

[00015] One aspect of the disclosure is an apparatus for deploying an intraocular lens into an 30 eye, comprising: an intraocular lens delivery device with an intraocular lens disposed therein; a support device adapted to be disposed within the delivery device, the support device having a lumen therein adapted to allow to fluid to flow therethrough; and a vent that is not an intraocular lens delivery port, the vent adapted to vent air from inside the delivery device when fluid flows therethrough.

[00016] One aspect of the disclosure is a method of deploying an intraocular lens into an eye, comprising providing an intraocular lens within a delivery device; delivering a fluid into the delivery device to deploy the intraocular lens from the delivery device; and venting air from within the delivery device through a vent, wherein the vent is not an intraocular lens delivery port.

5

#### BRIEF DESCRIPTION OF THE DRAWINGS

[00017] Figure 1 illustrates an exemplary accommodating intraocular lens that can be delivered into an eye using any of the delivery devices herein.

10 [00018] Figure 2 illustrates an exemplary intraocular lens delivery device.

[00019] Figures 3A and 3B illustrate a portion of an exemplary intraocular lens delivery device.

[00020] Figure 4 illustrates an exemplary intraocular lens delivery device with an intraocular lens therein.

15 [00021] Figure 5 illustrates an exemplary intraocular lens delivery device with a sealing element.

[00022] Figures 6A and 6B illustrate an exemplary sealing element.

[00023] Figures 7A and 7B illustrate an exemplary intraocular lens delivery device with a sealing element deployed and loaded.

20 [00024] Figures 8A-8C illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element delivering an intraocular lens from a distal delivery port.

[00025] Figures 9A-9C illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element delivering an intraocular lens from a distal delivery port.

[00026] Figures 10A-10C illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element delivering an intraocular lens from a distal delivery port.

25 [00027] Figures 11A-11C illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element.

[00028] Figures 12A and 12B illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element.

30 [00029] Figures 13A and 13B illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element.

[00030] Figures 14A-14B illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element in a loaded configuration.

[00031] Figure 15 illustrates an exemplary plugging element in a fully deployed configuration.

[00032] Figures 16A-16B illustrate an exemplary intraocular lens delivery device with a sealing, or plugging, element in a deployed configuration.

[00033] Figures 17A-E illustrate an exemplary delivery process of an intraocular lens with a delivery device with a plugging element.

5 [00034] Figure 18 illustrates venting of air out of a vent that is not a delivery port in an intraocular lens delivery device.

[00035] Figures 19A-19C illustrate an exemplary screw drive for advancing fluid through a an intraocular lens delivery device.

10

## DETAILED DESCRIPTION

[00036] The disclosure is related to methods and devices for delivering an intraocular lens (“IOL”) into an eye. The systems and methods herein can, however, be used to advance any type of IOL within a delivery or loading device. The intraocular lens can be accommodating or non-accommodating. The methods and devices herein may be beneficial when the IOL body does not occupy the entire volume of a section of the delivery device in which the IOL is positioned.

[00037] An IOL is typically implanted within a patient’s eye to replace or supplement the function of an eye’s native lens. The native lens can become diseased (e.g., cataract), or the lens can lose the ability to accommodate over time (i.e., presbyopia). In either case, the native lens can be removed and replaced with an IOL. To deliver the IOL through as small an incision as reasonable (e.g., about 2.8 mm to about 4.5 mm), the IOL typically undergoes some type of deformation or reconfiguration during the loading and/or delivery process to reduce the profile of the IOL. Additionally, some IOLs include components that can be reoriented and/or reconfigured relative to another component, such as a peripheral portion relative to an optic portion, and the controlled positioning or deformation of these components during the loading and/or delivery steps can enhance the loading and/or delivery and reduce the likelihood of damage to the IOL.

[00038] In some embodiments the delivery systems can be used to deliver an IOL that have one or more flowable media therein. For example, the delivery systems can be used to deliver fluid-filled accommodating IOLs, while in some embodiments the IOL may comprise a low viscosity polymeric material. The disclosure is not limited by the exemplary IOLs provided herein. Any suitable IOL that can benefit from the use of the systems and methods of herein can be delivered as described herein.

[00039] Figure 1 illustrates an exemplary intraocular lens that is delivered in any of the method herein. Accommodating intraocular lens 100 includes optic body 120 with a fluid chamber therein that is in fluid communication with fluid chambers in haptic 130 and haptic 140.

Haptics 130 and 140, part of the peripheral portion of the IOL, are responsive to capsular reshaping, and the IOL is adapted such that flowable media, such as a fluid, is moved between the haptics and optic in response to capsular reshaping. Additional exemplary details of accommodating IOL 100 can be found in U.S. App. No. 13/672,608, filed November 8, 2012, 5 which is incorporated by reference herein.

[00040] One first aspect of the disclosure is a delivery device adapted to deliver an accommodating intraocular lens, such as the intraocular lens shown in Figure 1, into the eye. While the delivery device is described as delivering the lens shown in Figure 1, it is understood that any other suitable lens can be delivered using the devices, systems, and methods described 10 herein. Figures 2A and 2B illustrate an exploded view and assembly view, respectively, of an exemplary delivery device (“device” may be used interchangeably with “system” herein unless there is a specific indication to the contrary). Figures 3A and 3B illustrate top sectional views of the assembly, with Figure 3B showing a partial sectional view of a distal portion of the assembly (only a portion of tray 14 and plunger 12 are shown). Delivery device 10 includes plunger 12, 15 tray 14, and cartridge 16. Tray 14 is adapted to interact with plunger 12 and cartridge 16, allowing an intraocular lens to be delivered from within cartridge 16 into an eye. Tray 14 includes plunger guide 22 extending through a proximal portion that is adapted to receive plunger 12 therein (see Figure 3A). Plunger 12 includes stop 20 that is configured to engage a complimentary stop feature on the tray to prevent further distal movement of plunger 12 within 20 tray 14. Plunger 12 includes lumen 32 extending from its proximal end to its distal end, allowing material, such as viscoelastic fluid, to be advanced from the proximal end of plunger into the cartridge. Plunger 12 also includes sealing members 18 in the form of O-rings that engage with an inner surface of cartridge 16 and provide a fluid seal between the distal end of plunger 12, cartridge 16, and tray 14. Cartridge 16 includes stabilizing elements 23 that are adapted to 25 secure the cartridge with respect to tray 14 by engaging corresponding stabilizing elements 24 on tray 14. As seen in Figures 3A and 3B, when plunger 12 is fully advanced within tray 14, and when cartridge 16 is interfacing tray 14, the distal end of plunger 12 is within the proximal end of channel extending through cartridge 16. This allows a material such as a viscoelastic fluid, or other material, to be delivered from the proximal end of the plunger into the cartridge, pushing 30 the loaded intraocular lens (not shown) from within the cartridge out the distal tip 28 (shown with a bevel) and into the patient’s eye. The tapering cartridge will previously have been placed through an incision in the eye allowing the lens to be delivered into the eye.

[00041] Figures 4A and 4B illustrate the exemplary intraocular lens from Figure 1 already loaded into the cartridge lumen 30. The intraocular lens can be advanced from a staging area in 35 the tray (referred to generally as 34 in Figure 2A) into the cartridge by any suitable loading

technique. In one approach, the intraocular lens is positioned within staging area 34 in a configuration such that leading haptic 36 is positioned generally distal to optic 38, while trailing haptic 40 is positioned generally proximal to optic 38. From this staged configuration, the lens can be advanced into cartridge. For example, the lens can be loaded into the cartridge with any 5 suitable plunger by being pushed into the cartridge. The lens could also be hydraulically loaded into the cartridge using a fluid. The loading device and approach can vary and is not limited herein. In some embodiments the system includes a plunger that is both adapted to load the lens from the tray into the cartridge, and is also adapted to deliver the lens from the cartridge into the eye as described below. Additional exemplary loading devices can be found in U.S. Provisional 10 Application No. 61/467,352, filed March 24, 2011, the disclosure of which is incorporated by reference herein.

[00042] After the lens is loaded into the cartridge as shown in Figure 4A, a viscoelastic fluid, or other type of fluid, is delivered from a syringe and into lumen 32 of plunger 12 (see Figure 4B). The viscoelastic fluid is delivered from the distal port of plunger 12 and into contact with 15 the intraocular lens, forcing the lens distally within cartridge and out the distal end 28 of the cartridge. In general, the delivery of the intraocular lens from the cartridge relies on development of pressure differential in the viscoelastic over the lens to move it down the reducing section of the cartridge (shown as surface 42 in Figure 4B) and into the eye. The configuration of the lens in general and/or the configuration that the intraocular lens assumes 20 when loaded into the proximal region of the cartridge, however, creates some gaps, which provide a path for some of the viscoelastic to leak past the optic portion, as shown by the flow arrows in Figure 4B. Ideally, none (or substantially none) of the viscoelastic fluid flows past the optic body portion. Ideally, all or substantially all of the viscoelastic remains proximal to at least the optic body portion, building up pressure and forcing the lens to be deployed from the distal 25 end of the cartridge. When the viscoelastic does flow past the lens body it can create drag on the leading haptic that is efficiently filling the tip of the cartridge (Figure 4B). The advancing leading haptic can create a high strain at the connection between the haptic and the optic body, possibly causing damage at the connection point. Any intraocular lens that may be susceptible to damage while being delivered may benefit from the systems and methods described herein.

30 [00043] One approach to preventing the fluid from flowing past the optic body and reducing the risk of damage to the lens is to create an efficient seal behind the lens body to reduce the flow of viscoelastic around the lens body. In one specific embodiment the device includes a plunger that includes at least one component that creates a seal behind the lens body. The component preferably does not restrict the deployment of the trailing haptic from the cartridge during the 35 last portion of the delivery process. Additionally, the component(s) preferably do not exit the

distal end of the cartridge into the eye at the end of the delivery process. While the sealing component is described as part of the plunger herein, it is understood that the sealing component could be a part of the tray, the cartridge, or other part of the delivery device.

**[00044]** Figures 5A-5C (side views of the device shown in Figures 2A-4B) show a portion of a delivery sequence of the lens in which the delivery device includes a sealing component, or plug, in the form of a compliant filament of material that is introduced into the viscoelastic stream. The filament is adapted to flow toward and into the location at which the viscoelastic fluid is flowing past the lens body. Once impeded by a restriction, the filament collapses and further obstructs the fluid flow path. This develops a soft sealing mechanism behind the lens body that also follows the lens while moving for delivery. Figure 5A illustrates the device including sealing component 52 in the form of a filament attached to the distal end of plunger 12 at attachment point 50. As shown in Figure 5A, filament 52 is initially disposed within lumen 32 of plunger 12, with the filament distal end extending in the proximal direction within the lumen. As the viscoelastic fluid is advanced through lumen 32 from the proximal end of the plunger, as shown by the arrow in Figures 5A-C, filament 52 is carried by the fluid in the distal direction, as shown in Figure 5B. The filament flows toward the location at which the viscoelastic fluid is flowing past the lens body and creates a seal, as shown in Figure 5B. In Figure 5B the filament is shown plugging up a space adjacent the trailing haptic 130, creating at least a substantial seal. Once the seal is formed, the force of the viscoelastic fluid on the lens body will properly cause both the leading haptic and the optic portion to be advanced distally within the cartridge. Figure 5C shows the leading haptic partially deployed from the cartridge while the optic body has been properly advanced through the cartridge. As the fluid continues to be advanced through the plunger and into the cartridge, the lens is advanced further through the cartridge until the leading haptic 140, optic body 120, and trailing haptic 140 are delivered, in that order, from the cartridge and into the eye. Once delivered the lens will inherently revert toward its original configuration, which is generally shown in the sectional view of Figure 1. The deployment occurs without damage to the lens, particularly at the attachment point between the leading haptic and the optic body.

**[00045]** Figures 6A and 6B illustrate an exemplary embodiment of filament 56 with slit 58 formed therein extending along substantially the entire length of filament 56. The slit forms two filament segments 60 extending along the length of filament 56. The length of the segments 60 is substantially greater than the width of the segments. Filament 56 from Figure 6A is then folded to bring two ends 62 together, as shown in Figure 6B. Figures 7A and 7B illustrate the folded filament attached to plunger 12. The filament is secured to the distal region of the plunger by compressing the two filament end regions under the two o-rings 18 that are a seal to

the cartridge, as discussed above. To prepare the device for use, the segments 60, in the form of loops, are tucked within the plunger lumen and ready for deployment during the delivery, as shown in Figure 7B. In use, the filament loops extend and roll out of the lumen in the viscoelastic stream and flow into an open volume behind the lens buttress and adjacent the trailing haptic as discussed above in the embodiment in Figures 5A-5C. The filament bunches into that area until sufficiently plugging the flow at which time the lens body moves forward. When the lens moves sufficiently forward to plug the tip completely and there is substantially no viscoelastic flow by the lens body, the filament will be left behind.

5 [00046] If, during the delivery, the optic body stops moving in the cartridge and the viscoelastic is leaking past the optic body again, the filaments are adapted to again move to the area of leakage to act as a plug to the viscoelastic and move the lens out of the cartridge. The filaments as described herein as therefore adapted to repeatedly, as may be necessary, find or seek out the region where fluid is flowing past the optic body, move to that location, and plug the leak.

10 [00047] The embodiment in Figures 5A-7B illustrate embodiments in which the proximal end of the filament is attached to the distal region and the exterior of the plunger, and the filament is considered to roll out of the plunger during delivery of the lens. This allows the filament to slide out of the plunger past the attachment location and the first contact with the lens will be with a region of the filament that is near the proximal end of the filament. The filament repositions into 15 a suitable plugging orientation. There are, however, a number of variations in attachment points of the filament to the plunger (or other portions of the delivery device) yielding variations in deployment of the filament.

20 [00048] Figures 8A-8C illustrate an alternative embodiment in which the proximal end of the filament is attached to the distal region of the plunger, but is attached at a location on the interior 25 of the plunger (i.e., within the plunger lumen). As indicated in Figure 8A, the plunger has a proximal lumen section with a larger diameter bore than a distal tip section. Filament 70 is attached to stopper 72 at its proximal end. Filament 70 extends from stopper 70 towards the distal end of the plunger. The reduced diameter distal section acts as a lumen restriction and prevents stopper 72 from advancing further distally, as shown in Figure 8C. This prevents the 30 filament from flowing out of the distal tip of the cartridge. As the viscoelastic is delivered through the lumen, stopper 72 is advanced distally within the lumen, and filament 70 flows straight out of the lumen and does not double back (or fold) back on itself as in the previously described embodiments above. The filament is adapted to flow towards the flow leakage as described elsewhere herein.

[00049] Figures 9A-9C illustrate sectional views of an alternative embodiment in which the proximal end of the filament 80 is secured to the proximal region of the plunger interior using press-ring filament capture 78, which is shown in greater detail in Figure 15. Filament 74 includes a coiled or stretchable section 76 that is adapted to uncoil or stretch as the viscoelastic is delivered. The uncoiling or stretching of the filament effectively lengthens the filament, allowing the filament to be advanced into the cartridge to plug up any leaks, but is prevented from flowing out of the distal end of the cartridge. Figure 9B shows the filament finding the leaking area and plugging it.

[00050] The embodiment shown in Figures 9A-9C includes a plunger with a distal tip region that has a reduced diameter relative to the proximal region. This feature can be incorporated into any the embodiments herein. The reduced diameter can create a relatively higher flow rate of fluid from the plunger distal tip, which helps pull the filament out of the distal end of the plunger. The increased flow rate minimizes tangles and compaction of the filament in the proximal end of the plunger as the viscoelastic is delivered.

[00051] Figures 10A-10C illustrate an alternative embodiment similar to that in Figures 9A-9C in that the proximal end of the filament 82 is attached to an internal proximal region of the plunger 84. In this embodiment the filament 82 is a material that has a stretching property to it, such as a material that is perforated in such a way that it compresses efficiently in the plunger lumen (see Figure 10A) and yet stretches to a static length when deployed (see Figure 10C). In this embodiment the filament is an axially compressed perforated tubing. The filament is secured at its proximal end 845, and the plunger has a fluid channel radially outward from the attachment point. This is shown in Figure 10B, in which the fluid flow is indicated the arrows. The fluid causes the perforated tubing to stretch as shown in Figure 10B. This plunger design, with the distal reduced diameter, provides for a low velocity flow region and a high velocity flow region in the distal region. Figure 10B illustrates the plunger sealing the leak, and Figure 10C illustrates the leading haptic being deployed from the cartridge.

[00052] The filament material and design should be selected to enable the filament to seal the fluid flow as described above. An optimization of material structure and properties will generally provide a filament that is best suited to seal the fluid flow and allow for the intraocular lens to be delivered undamaged. It is envisioned, however, that in some instances it may be desirable to have some amount of fluid that does pass the optic body, after which the sealing should occur. The filament material can theoretically be selected that will provide that functionality to the system.

[00053] The properties of the filament will influence how it responds during the delivery process. Properties that can be modified to accomplish the specific goal include without

limitation, compliance, coefficient of friction, and elasticity. In embodiments described above, properties that have been shown to influence performance include compliance, a low coefficient of friction, and in some cases elasticity. It is understood that not all of these need to be optimized, and there may be other properties that can be controlled to achieve a desired result.

5 [00054] In some embodiments the filament has a degree of deformability and elasticity that allows it to be pulled from the plunger and seal the leak. In some particular embodiments expanded PTFE, an expanded Teflon material, is used. In some embodiments the filament comprises an open cell foam. For example, a low durometer open cell silicone foam with a single strand form can be used in both the straight out method (e.g., Figures 8A-8C) and roll out 10 methods (e.g., Figures 5A-5C). In some embodiments PVA bio-absorbable type foams that provide good open cell performance can also be used. In some embodiments light wall (e.g., 0.004in) low durometer (e.g., 20-35shoreA) silicone tubing can be used, particularly with the roll-out method. In some embodiment electro-spun or non-woven materials are used, and materials that allow for compaction of the mat under low pressures can be used in a straight out 15 method with a relatively large cross section. It is understood that other suitable materials can be used to accomplish the intended goal.

20 [00055] The filaments can be further manipulated to control the performance characteristics. For example, one or more slits formed in the filament can provide desired functionality. Radial and axial slits have been shown to increase compliance and bending of the filament to optimize sealing performance to the lens. One or more slits can be formed in the filaments. The one or 25 more slits can take on any configuration within the material.

[00056] In some embodiments the filament is a monofilament ePTFE material. The material can be formed with one or more loops (see Figures 6A-7B), and in some embodiments between one and three loops to optimize cross section in the plunger lumen relative to the tip plunger 30 lumen size.

[00057] While specific embodiments have been described herein that focus on the use of a filament, other material can be incorporated into the delivery device to accomplish the goal. For example, any suitable material that can be used to seal off the gaps can be used. Other deformable or flexible materials, for example, that are not described herein could theoretically be 35 suitable or adapted to function as a sealing element as described herein.

[00058] In alternative embodiments, the sealing element is a sealed porous tube of PTFE that is filled with viscoelastic or other fluid. The porous tube is adapted to allow viscoelastic to pass through the tube, or "weep" through the pores. In this alternative all of the viscoelastic fluid delivered into the system is pushed through the porous tube. The tube is adapted to seal off the 35 fluid leaks as described above. The pore size can be varied to control the flow rate.

Additionally, different viscoelastic fluids have different viscosities and flow properties, and thus the fluid can be varied to modify the flow rate as well.

**[00059]** Figures 11A-11C and 12A and 12B illustrate an embodiment that includes a plug component that is a flexible porous tube 200 sealed on its distal end. The tube is sheathed over a 5 hypo-tube support 202 that is sealed to the interior lumen of the proximal end of the plunger 204. The porous tube 200 is long relative to the length of the support tube 202 to be able to extend to the tip of the cartridge when deployed. In a packaged state, the porous tube 200 is packed onto the support 202 to decrease the length. The support tube 202 communicates with the proximal end 206 of the plunger to allow for the passage of viscoelastic (not shown) to be delivered 10 directly to the tip 208 of the sealed porous tube 200. With flow of viscoelastic through support tube 202 and into the porous tube 200, the porous tube 200 will pressurize slightly and extend off of the support tubing 202 to move into a region behind the lens that both seals, as described above, and is able to transmit axial force mechanically to the lens. When the lens moves forward in the tapering cartridge and creates an efficient seal, the sealing and mechanical action of the 15 porous tube will lend less influence to its functionality and it will transition in performance to simply pass viscoelastic therethrough (via the pores), which will move the lens forward with pressure differential. The functionality of the porous tubing can be modified as needed by modifying the properties of the tubing. For example, with a low porosity (i.e., small pore size) material, the tube will generally develop a higher internal pressure while the viscoelastic tubing 20 is flowing, which will allow it to function more as a mechanical hydraulic piston applying force to the lens when contacted. With a relatively higher porosity construction (i.e., larger pore size), the tube will behave more similarly to the filament structures described above, acting more prominently as a sealing element to seal off any leaking fluid. The porosity (or other property of the tube) can therefore be modified as needed to achieve the desired functionality of the porous 25 tubing.

**[00060]** Figures 13A and 13B illustrate an alternative exemplary embodiment of an IOL delivery system adapted to deliver an IOL into an eye of a patient. The system includes cartridge 301, tray 302, and plunger 303. Figure 13B shows the assembled system, which figure 13A shows the disassembled system components. In other embodiments one or more of the three 30 components may be integrally formed rather than separate parts.

**[00061]** In the assembly of Figure 13B, cartridge 301 is positioned with respect to tray 302 such that cartridge 301 and tray 302 are in secured engagement. In some embodiments cartridge 301 and tray 302 are integrally formed such that cartridge 301 is not adapted to be disassociated from tray 302. Tray 302 is adapted to receive a distal portion of plunger 303 therein. The distal 35 end 306 of plunger 303 is sized and configured to be disposed within proximal opening 305 in

cartridge 301 when assembled. Plunger 303 includes seals 307 in the form of O-rings. Seals 307 are adapted to create a seal between an inner surface of cartridge 301 when distal portion 306 of plunger is advanced into opening 305 of cartridge 301. Tray 302 facilitates the interaction between the cartridge and the plunger.

5 [00062] Plunger 303 has a proximal portion that is adapted to interact with a fluid delivery device, such as a syringe, so that fluid can be advanced from the fluid delivery device and into an inner lumen within plunger 303. Distal end 306 of plunger 303 is disposed within the cartridge, and thus the fluid is delivered to a location that is radially and axially within the lumen, even if it does not exit the plunger.

10 [00063] Cartridge 301 and tray 302 are in secure engagement as described in U.S. App. No. 13/427,617, filed March 22, 2012, which is incorporated by reference herein. Tray 302 includes two clips 361 with locking elements 365, wherein the clip are adapted to interface with camming surfaces 363 on plunger. Clips will splay outward as plunger 303 is advanced in tray 302, and locks 367 on plunger will lock with locks 365 on tray 302.

15 [00064] Figures 14A and 14B illustrate top section views of the assembled system from Figure 13B (IOL not shown for clarity). As can be seen, the distal portion 306 of plunger 303 is disposed within a proximal portion of lumen 310 of cartridge. While not shown, an IOL will also be disposed within lumen 310 and positioned to be deployed out of the distal end 311 of cartridge 301.

20 [00065] Plunger 303 includes outer shell 313, on which seals 307 are disposed. As can be seen, seals 307 create a seal between outer shell 313 and an inner surface of lumen 310. Plunger 303 also includes plug subassembly 321 within a lumen of plunger 303. The plug subassembly is also shown in greater detail in Figure 15. Plug subassembly 321 includes support tube base 316, in which support tube 314 is disposed and secured thereto, and plug element 317. Plug element 317 is sheathed over and secured to the outer surface of support tube 314 at location 308 (see Figure 15). In one embodiment a heat shrunk collar secures plug element 317 to support tube 314 at location 308. The distal end of support tube 314 extends from the distal end of base 316, and is configured with an orientation to one side. That is, the distal portion of tube 314 does not extend along the longitudinal axis of plunger 303. This helps direct support tube 314 and plug 317 away from the trailing haptic. Plug element 317 is long relative to the length of the support tube 314 such that the distal end of plug element 317 is disposed at the tip of the cartridge when the plug is fully deployed. In a packaged, or loaded, state (see Figures 14A and 14B), plug element 317 is packed onto support tube 314 to decrease its relative length. Support tube 314 communicates with the proximal end of plunger 303 to allow for the passage of a fluid such as viscoelastic (not shown) into plug element 317. Plug subassembly 321 also include seal

25

30

35

315 adapted to create a seal between plug subassembly 321 and an inner surface of outer shell 313 of plunger 313.

[00066] In this embodiment, plug element 317 is a tubular structure secured to the distal end of support tube 314 as shown in Figure 15. In this embodiment plug element is a flexible and porous material but need not necessary be porous. In one exemplary embodiment plug element is tubular ePTFE. In this embodiment the tubing is open-ended at both ends and is tied in a knot 327 along its length, with distal section 309 of plug 317 extending distally from knot 327. Knot 327 acts as a flow restrictor, and also helps stabilize the plug on the support tube. In this embodiment plug element 317 includes one or more optional perforations 325 just proximal to knot 327. The flow restrictor can be, for example, tied, glued, crimped, or swaged.

[00067] To load the plug subassembly into outer shell 313, distal section 39 of plug element 317 is rolled back, or folded back, towards the proximal end of the subassembly, in the direction of arrows shown in Figure 15. It is everted until flow restrictor 307 is substantially at the distal end of the plug element 317. The distal portion of plug element 317, in a loaded configuration, 15 thus has an everted section of material at its distal end. Plug assembly 321 is then advanced distally through open end 312 of outer shell 313 of plunger 303 until it is in the loaded position shown in Figures 14A and 14B. The open distal end of plug element 317, in its everted configuration, is retained within the lumen of outer shell 313, maintaining the eversion. Figure 14A illustrates the biased configuration of the distal end of support tube 314. Figure 14B is a 20 side section view of the plug subassembly in a loaded configuration and position within outer shell 313 of plunger 303.

[00068] Figures 16A and 16B illustrate a fully deployed configuration of plug element 317 within cartridge 301, as is also shown in Figure 15 outside of a cartridge. For clarity, this is illustrated without showing the IOL. A method of use with an IOL is shown below. As 25 described in more detail below, after the plug is loaded (as shown in Figures 14A and 14B), a fluid is delivered through support tube 314 to initiate the deployment of plug element 317. As plug element 317 continues to be deployed, the everted section 309 remains everted until the full extension of the proximal portion of the plug element 317, at which time everted section 309 begins to unroll, and ultimately plug element 317 assumes the general elongate configuration 30 shown in Figures 16A and 16B. The distal end of plug element 317 is substantially at the tip of cartridge 301 when fully deployed.

[00069] Figure 17A illustrates an IOL comprising optic 120 and haptics 130 and 140 positioned (e.g., such as the IOL shown in Figure 1) within cartridge 301. The IOL has been loaded into cartridge 301, and exemplary methods of loading the IOL into cartridge are described 35 below. The disclosure herein is not intended to be limited to the manner in which IOL becomes

positioned into cartridge 301. In the IOL's loaded configuration shown in Figure 17A, leading haptic 130 has been reoriented from an at-rest orientation (see Figure 1) and extends distally from optic 120. Trailing haptic 140 has also been reoriented from an at-rest orientation (see Figure 1) and extends relatively proximally from optic 120 within cartridge.

5 [00070] In general, the delivery of the IOL out of the cartridge relies on development of a pressure differential in the cartridge to move the IOL distally through the cartridge and into the eye. The configuration of the IOL in general and/or the configuration that the IOL assumes when loaded into the cartridge, however, creates some gaps between the IOL and the inner surface(s) of the cartridge. That is, the IOL does not occupy the entire volume defined by the  
10 inner surfaces of the cartridge. The gaps, or voids, provide a path for some of the fluid to leak past the optic portion as fluid is advanced during the delivery. Ideally, none (or substantially none) of the fluid flows past the optic body portion. Ideally, all, or substantially all, of the fluid remains proximal to at least the optic body portion, building up pressure and forcing the IOL to be deployed out of the distal end of the cartridge. When fluid does flow past the lens body it can  
15 create drag on leading haptic 130 that is efficiently filling the tip of the cartridge. The advancing leading haptic can create a high strain at the connection between the leading haptic and the optic body, possibly causing damage at the connection point. Any IOL that may be susceptible to damage while being delivered may benefit from the systems and methods described herein.

20 [00071] An exemplary method of assembling the system includes placing cartridge 301 in tray 302, loading the IOL into cartridge 301, and then positioning plunger 303 relative to tray 302 such that it extends into cartridge 301, as shown in Figure 17A. In Figure 17A, plug subassembly 321 is in the same loaded position and configuration within cartridge 301 as shown in Figures 14A and 14B. In this configuration the plug element 317, and specifically everted portion 309, is positioned adjacent trailing haptic 140. Plug element 317 is disposed in a gap  
25 that exists between trailing haptic 140 and the inner surface of cartridge 301. As described above, this distal end of support tube 314 is oriented away from trailing haptic 140, which disposes the plug element 317 in the position shown in Figure 17A, which is radially adjacent to trailing haptic 140. The support tube distal end is therefore adapted to avoid damaging the IOL when positioned in the cartridge. In this configuration plug element 317 acts like a plug to fill in  
30 the gap, or a substantial portion of the gap, to obstruct the flow of fluid, thereby minimize the amount of fluid that flows past the trailing haptic 140 during the delivery. Plug element 317 may or may not be in contact with the IOL at this time. As described below, plug element 317 reduces the volume of fluid that flows past the optic during delivery, increasing the pressure differential, and thus reducing the risk of damage to the lens. Plug element 317 can also be  
35 thought of as creating a seal, or a substantial seal, behind the IOL body to reduce the flow of

viscoelastic around the IOL. "Plug" or "seal" are not limited to mean a completely fluid tight seal is created. These terms are used herein to mean that fluid flow around the IOL is reduced from what it would be without the plug or seal element. The plug element can also be any of the components described above as creating a seal behind the optic.

5 [00072] After the plug subassembly is positioned as shown in Figure 17A, a fluid, such as a viscoelastic, is advanced through support tube 314 using a fluid delivery device such as a syringe (not shown). With the flow of viscoelastic through support tube 314 and into plug element 317, plug element 317 will pressurize slightly and reconfigure off of the support tube 314 to move more fully into a region behind the lens that plugs the gap and is able to transmit force

10 mechanically to the lens. As the IOL moves forward in the tapering cartridge inner lumen and creates an efficient, or substantial, seal, the sealing and mechanical action of the porous tube will lend less influence to its functionality and it will transition in performance to pass viscoelastic therethrough (via the pores, or other perforation constructs), which will move the lens forward with pressure differential. The functionality of the porous tubing can be modified as needed by

15 modifying the properties of the tubing. For example, with a low porosity (i.e., small pore size) material, the tube will generally develop a higher internal pressure while the viscoelastic is flowing, which will allow it to function more as a mechanical hydraulic piston applying force to the lens when contacted. With a relatively higher porosity construction (i.e., larger pore size), the tube will behave more similarly to the filament structures above, acting more prominently as

20 a plug element to seal off leaking fluid. The porosity (or other property of the tube) can therefore be modified as needed to achieve the desired functionality of the plug element.

[00073] As the fluid exists the distal end of support tube 314, the fluid pressure within the everted portion 309 of plug element 317 causes the distal end of plug element 317 to be released from the distal end of outer shell 313 of plunger 303. As the free distal end of the plug is

25 released from the inner lumen of the plunger, it begins to at least partially seal against the inner walls of the cartridge, further reducing the volume of fluid that flows past the IOL. The plug element also at least partially plugs the gap that exists radially between adjacent trailing haptic 140 and the inner wall of the cartridge. This plugging action minimizes the volume of fluid that can flow passed trailing haptic and therefore passed optic portion, increasing the pressure

30 differential in the cartridge.

[00074] As fluid continues to be advanced through support element 314, as shown in Figure 17C, the everted plug element continues to follow the IOL, still plugging the gap between trailing haptic 140 and the cartridge. As the optic is advanced closer to the distal port, as shown in Figure 17D, the size of the port and the volume that the optic occupies cause the optic to begin

35 to self-seal, or substantially create a seal in the distal port. In Figure 17D the IOL begins to

move distally relative to plug element 317, or outrun the plug element 317. In Figure 17E the optic has been delivered out of the cartridge and trailing haptic 140 is rolling off of everted portion 309. This causes the everted portion of the plug element to unroll, as shown in Figure 17E. The everted portion 309 of the plug element reduces drag on trailing haptic 140 between at least Figures 17D and 17E, when it is unfurling, or unrolling. A static plug element, unlike everted portion 309, can cause the trailing haptic to get stuck against the wall of the cartridge due to the radial expansion of the plug and static friction between the plug and the haptic. When the plug element includes a feature that can contact and unfurl with the trailing haptic, drag on the trailing haptic is reduced, preventing it from sticking against the cartridge wall and not deploying properly. This also reduces the likelihood of damage at the junction between the optic and the trailing haptic.

[00075] In the embodiment in Figures 17A-17E, plug 317 is a porous ePTFE material. The porous material is adapted to allow viscoelastic to pass through the tube, or “weep” through the pores. In embodiments herein plug 317 also includes optional perforations 325 (two shown in the embodiment in Figures 17A-17E) in the plug material just proximal to the knot location 327. In one particular embodiment the perforations are created with a 32G surgical needle about 1mm proximal to the knot. The perforations act as an over-pressure relief for the viscoelastic material (or other fluid). The porosity of the ePTFE (or other porous material) can be variable, and in some cases, which may depend on the viscoelastic material used, the material may fully contain the viscoelastic without allowing for effective weeping. If this occurs the plug element may disengage from the support tube 314 due to pressure at the end of extension. The perforations can thus serve as an over-pressure relief to prevent this possibility. In a secondary roll, the perforation can also direct fluid into the everted section of the plug to facilitate its release from the plunger and thus sealing against the inner surface of the cartridge.

[00076] The porosity of the plug allows viscoelastic to lubricate the interfaces between the moving plug and other system components. The porosity also allows the continued flow of the fluid when the plug is at full deployment and the IOL is moving due to a hydraulic seal at the tip.

[00077] The pore size can be varied to control the flow rate. Additionally, different viscoelastic fluids have different viscosities and flow properties, and thus the fluid can be varied to modify the flow rate as well. In an exemplary embodiment the plug element is ePTFE and the intermodal distance (i.e., the distance between the nodes), which determines the porosity, is 100  $\mu\text{m}$ . ePTFE with other internodal distances can also be used.

[00078] The embodiment shown in Figures 13A, 13B, 14A, 14B, 16A, 16B, and 17A-17E are also adapted to purge trapped air in the system that, if not purged, can interfere with the delivery process. Figure 18 illustrates a side section view of the assembled device shown in Figure 14B

(IOL not shown for clarity), illustrating the purging of air from the plunger. As described herein, fluid travels from a syringe (not shown) through support tube 314 and exits in proximity of the trailing haptic of the IOL within the plug element (everted section 309 labeled). A fluid front travels both distally in the “D” direction shown, filling the plug element, and rearward in the “P” direction, which evacuates dead volume air through vent 330 in the direction of arrow “A.” The vent will not pass viscoelastic so is able to maintain pressure when fully evacuated. This effect purges the air from the back of the system to reduce spring effects of trapped air during the release of the IOL during delivery. In some instances if the air is not purged the air can forcefully push the IOL forward during delivery, without operator action/input, possibly damaging the IOL or the capsule in the eye, and can even cause the IOL to be delivered outside of the capsule. The purging of air is important for a smooth, controlled delivery of the IOL. Some IOLs may not require as much control in the delivery, and thus venting of air may not be required.

**[00079]** In some embodiments the delivery system includes a vent and does not include a plug, or sealing element. In these embodiments fluid such as viscoelastic is delivered towards the lens as part of the delivery process. Air venting to increase control during delivery while decreasing the volume of air bubbles that are moved forward through the tip into the eye provides a significant advantage even in the absence of a plug element. In an alternative embodiment, the device is similar to the delivery device in Figures 14A and 14B but does not include a plug element 317.

**[00080]** Figures 19A-19C illustrate an exemplary way of driving fluid such as viscoelastic from within a delivery device into the support tube 314. In this embodiment the delivery assembly, including cartridge 301, tray 302, and plunger 303, with syringe 360 secured thereto, are mounted into screwdrive assembly 370. Screwdrive assembly 370 includes base 390 with end posts 372 over which slots in tray 302 are aligned. The delivery assembly self-aligns with screw 380. Screw 380 is advanced until it touches the plunger of the syringe, as shown in Figure 19C. Screw 380 is then turned to cause the syringe plunger to be advanced, which drives the fluid from the syringe and into support tube 314. The screwdrive assembly can be modified to more finely control the force applied to the syringe, and can include a pressure gauge.

**[00081]** As set forth herein, an IOL can be positioned, or loaded, into the cartridge using any suitable technique. For the specific IOL described herein, the loading process includes changing the orientation of the haptics with respect to the optic, such that the haptics generally extend away from the optic. In general this process of reorienting the haptics is referred to herein as splaying the haptics. The loading process, for the IOL herein, also includes reconfiguring at least one portion of the IOL, such as the optic. Exemplary loading techniques include without

limitation, hydraulically loading the IOL, as is set forth in U.S. App. No. 12/178,565, filed July 23, 2008. Alternatively, the IOL can be mechanically loaded, such as is described in U.S. App. No. 13/427,617, filed March 22, 2012. Another example of mechanical loading includes using forceps to pick up the IOL, reorient one or more haptics, and advance the IOL into the cartridge.

5 [00082] The IOL can be loaded into the cartridge and stored, such as for packaging, or loading can occur just prior to implantation.

10 [00083] The devices and methods herein are able to deliver an IOL through an incision that is between about 2.8 mm to about 4.5 mm. In some embodiments the incision is about 4 mm. The devices and methods can be modified if needed to deliver an IOL through a bigger or smaller incision.

[00084] While the disclosure focused on a tubular member for the plug, other sealing mechanisms can also be inserted into the cartridge to help create at least a partial seal between the IOL and cartridge to aid in the delivery of the IOL.

15 [00085] The IOL to be delivered need not have one or more dedicated "haptics" as described herein. The IOL can more generally include a peripheral portion.

## CLAIMS

## WHAT IS CLAIMED IS:

1. A method of deploying an intraocular lens into an eye, comprising  
5 providing an intraocular lens within a delivery device;  
at least partially plugging a gap disposed radially between the intraocular lens and an inner surface of the delivery device; and  
delivering a fluid into the delivery device to deploy the intraocular lens from the delivery device and into an eye.  
10
2. The method of claim 1 wherein at least partially plugging a gap reduces the amount of fluid that flows passed the intraocular lens in the delivery device.
3. The method of claim 1 wherein at least partially plugging a gap allow for an increase in  
15 fluid pressure in the delivery device proximal to an optic portion of the intraocular lens.
4. The method of claim 1 wherein at least partially plugging a gap between the intraocular lens and an inner surface of the delivery device comprises at least plugging a gap that exists between a trailing haptic and an inner surface of the delivery device.  
20
5. The method of claim 1 further comprising reconfiguring a plugging element while delivering the fluid into the delivery device.
6. The method of claim 5 wherein reconfiguring the plugging element acts to form a seal  
25 between the plugging element and an inner surface of the delivery device.
7. The method of claim 5 wherein reconfiguring the plugging element unrolls the plugging element.
- 30 8. The method of claim 1 wherein delivering a fluid into the delivery device to deploy the intraocular lens from the delivery device comprises delivering a fluid through a porous material.
- 35 9. An apparatus for deploying an intraocular lens into an eye, comprising:  
an intraocular lens delivery device with an intraocular lens disposed therein;

a support device adapted to be disposed within the delivery device, the support device having a lumen therein adapted to allow fluid to flow therethrough; and  
a plug element secured to the support device such that it is adapted to at least partially plug a gap between an intraocular lens positioned in the delivery device and an inner surface of  
5 the delivery device.

10. The apparatus of claim 9 wherein the plug element is a tubular element.
11. The apparatus of claim 10 wherein the plug element is open at a distal end after  
10 deployment.
12. The apparatus of claim 10 wherein the plug element has a fluid flow restriction proximal to a distal end of the plug element.
- 15 13. The apparatus of claim 9 wherein the plug element is everted at a distal end.
14. The apparatus of claim 9 wherein the plug element is porous.
15. The apparatus of claim 9 wherein the plug element is adapted to be reconfigured in  
20 response to fluid flow through the lumen.
16. The apparatus of claim 9 wherein only a distal portion of the plug element is adapted to be reconfigured.
- 25 17. The apparatus of claim 9 wherein the plug element has a flow restriction proximal to a distal end of the plug element.
18. The apparatus of claim 17 wherein the plug element has portion distal to the flow restriction that is adapted to be reconfigured.
- 30 19. The apparatus of claim 9 wherein the plug element is open at a distal end.
20. The apparatus of claim 9 wherein the plug element is an ePTFE tube.

21. The apparatus of claim 9 wherein a distal portion of the support element is oriented towards an inner wall of the delivery device.
22. The apparatus of claim 9 wherein a distal portion of the support element is oriented away from a longitudinal axis of a proximal portion of the support element.  
5
23. The apparatus of claim 9 wherein a trailing haptic extends proximal relative to an optic portion of the intraocular lens.
- 10 24. The apparatus of claim 23 wherein the plug element is disposed radially between the intraocular lens and an inner surface of the delivery device.
25. The apparatus of claim 9 further comprising a vent adapted to vent air from inside the apparatus.  
15
26. An apparatus for deploying an intraocular lens into an eye, comprising:  
an intraocular lens delivery device with an intraocular lens disposed therein;  
a support device adapted to be disposed within the delivery device, the support device having a lumen therein adapted to allow fluid to flow therethrough; and  
20 a vent that is not an intraocular lens delivery port, the vent adapted to vent air from inside the delivery device when fluid flows therethrough.
27. A method of deploying an intraocular lens into an eye, comprising  
providing an intraocular lens within a delivery device;  
25 delivering a fluid into the delivery device to deploy the intraocular lens from the delivery device; and  
venting air from within the delivery device through a vent, wherein the vent is not an intraocular lens delivery port.

30

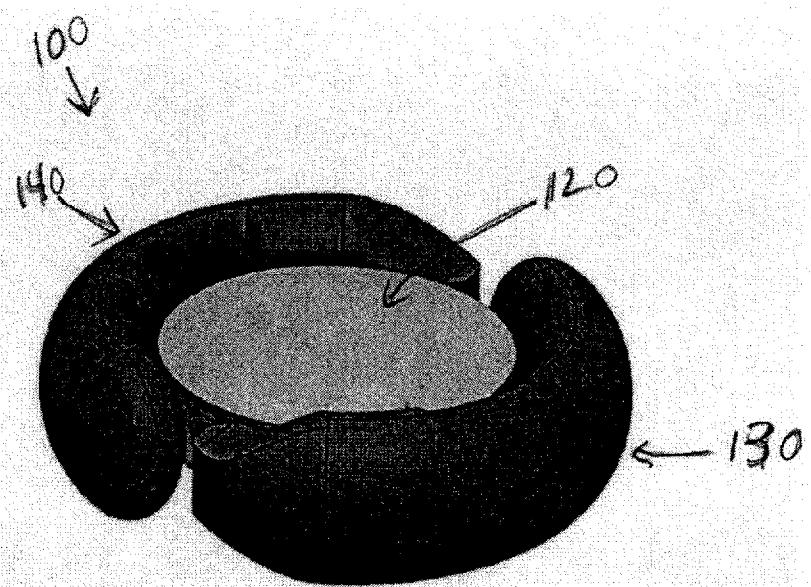


FIG. 1

2 / 17

FIG. 2A



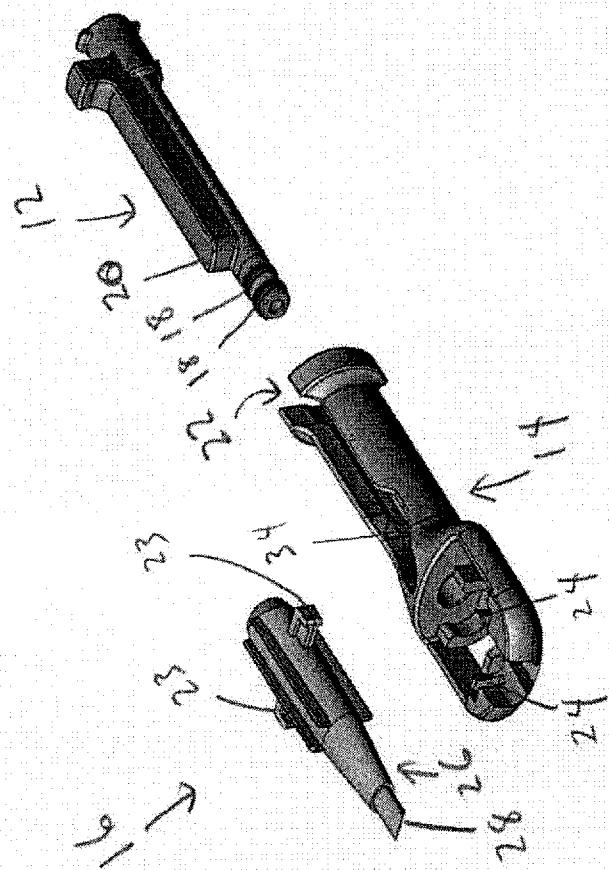


FIG. 2B

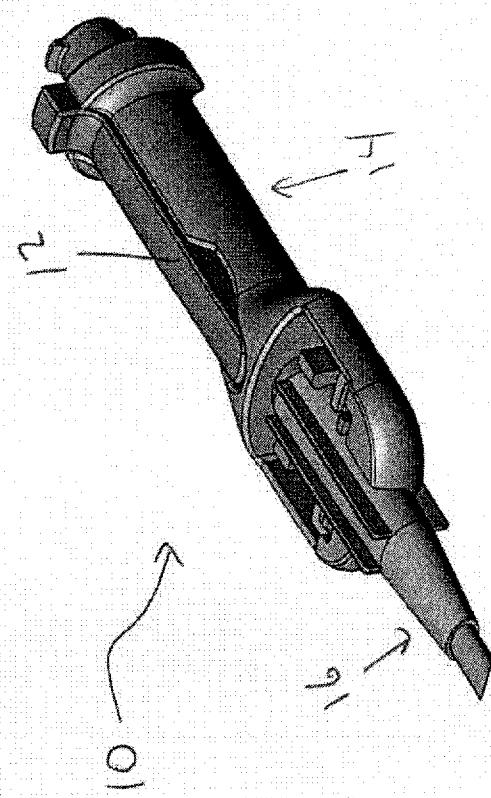

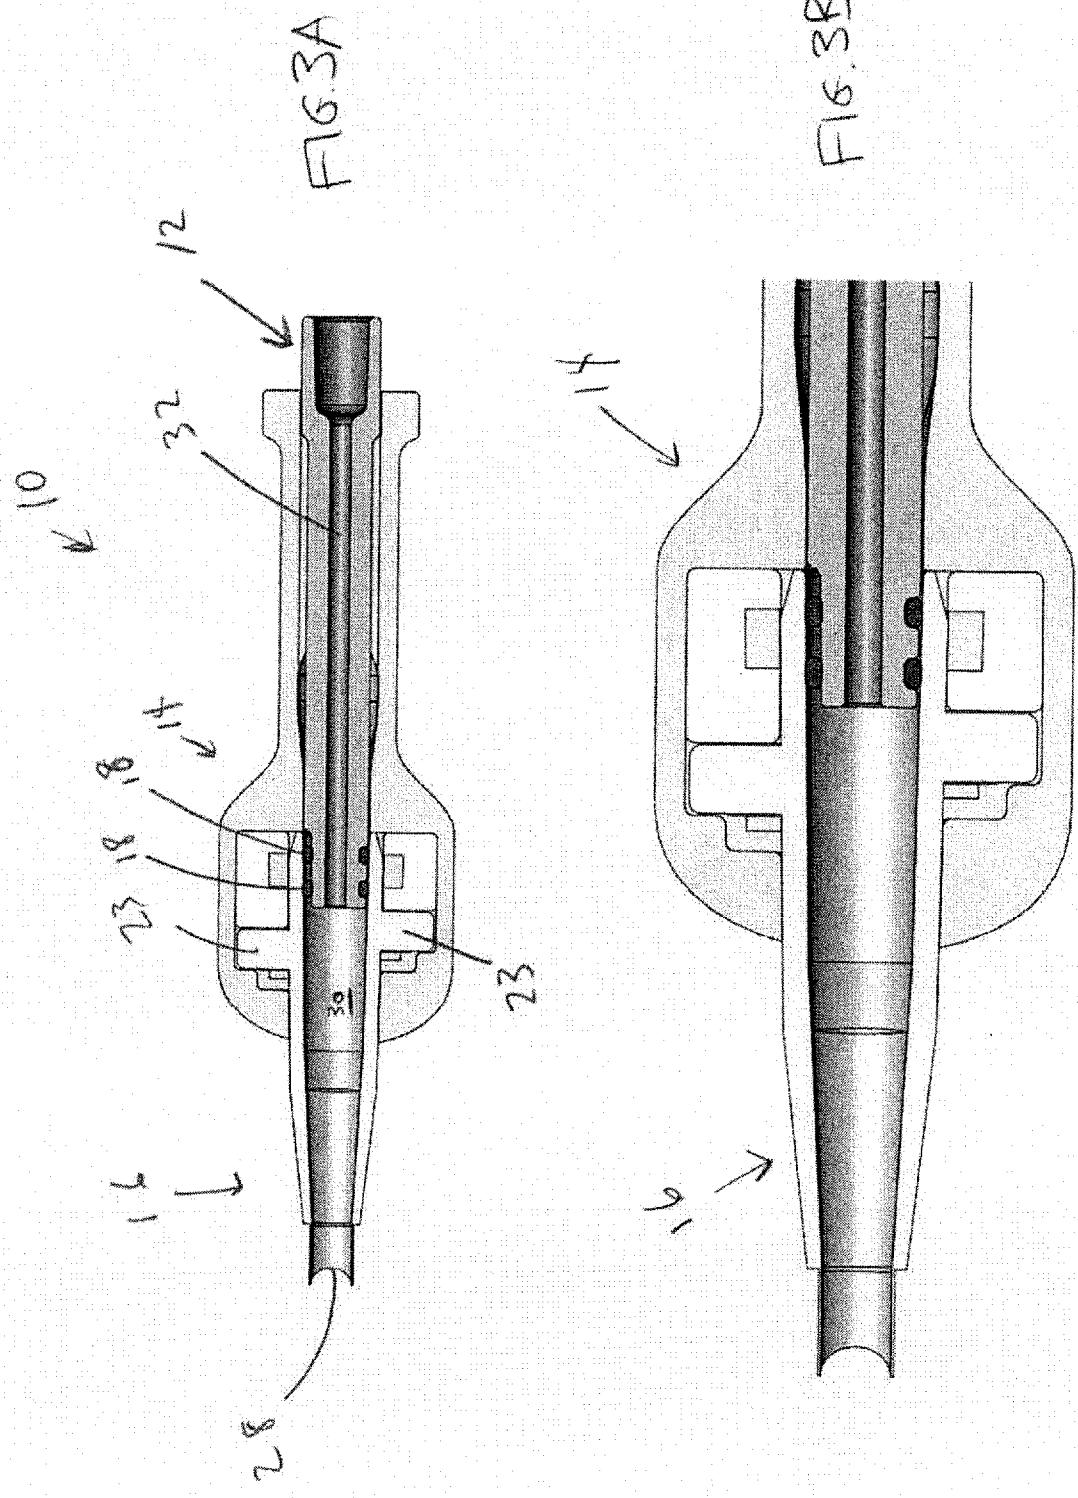

4 / 17

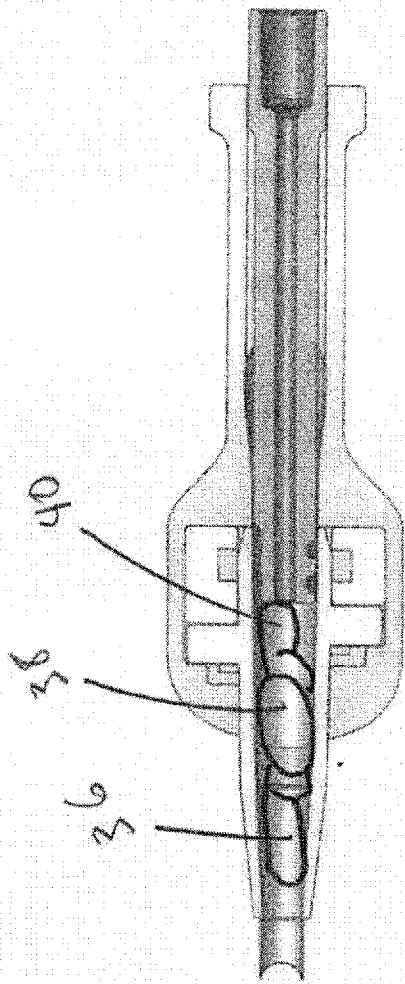


FIG. 4A



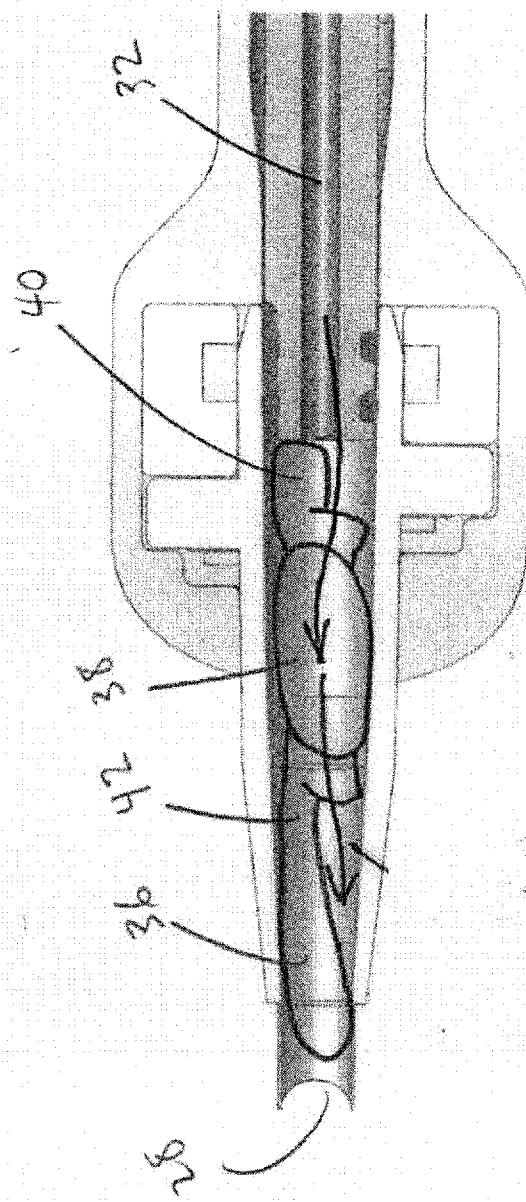


FIG. 4B


5 / 17

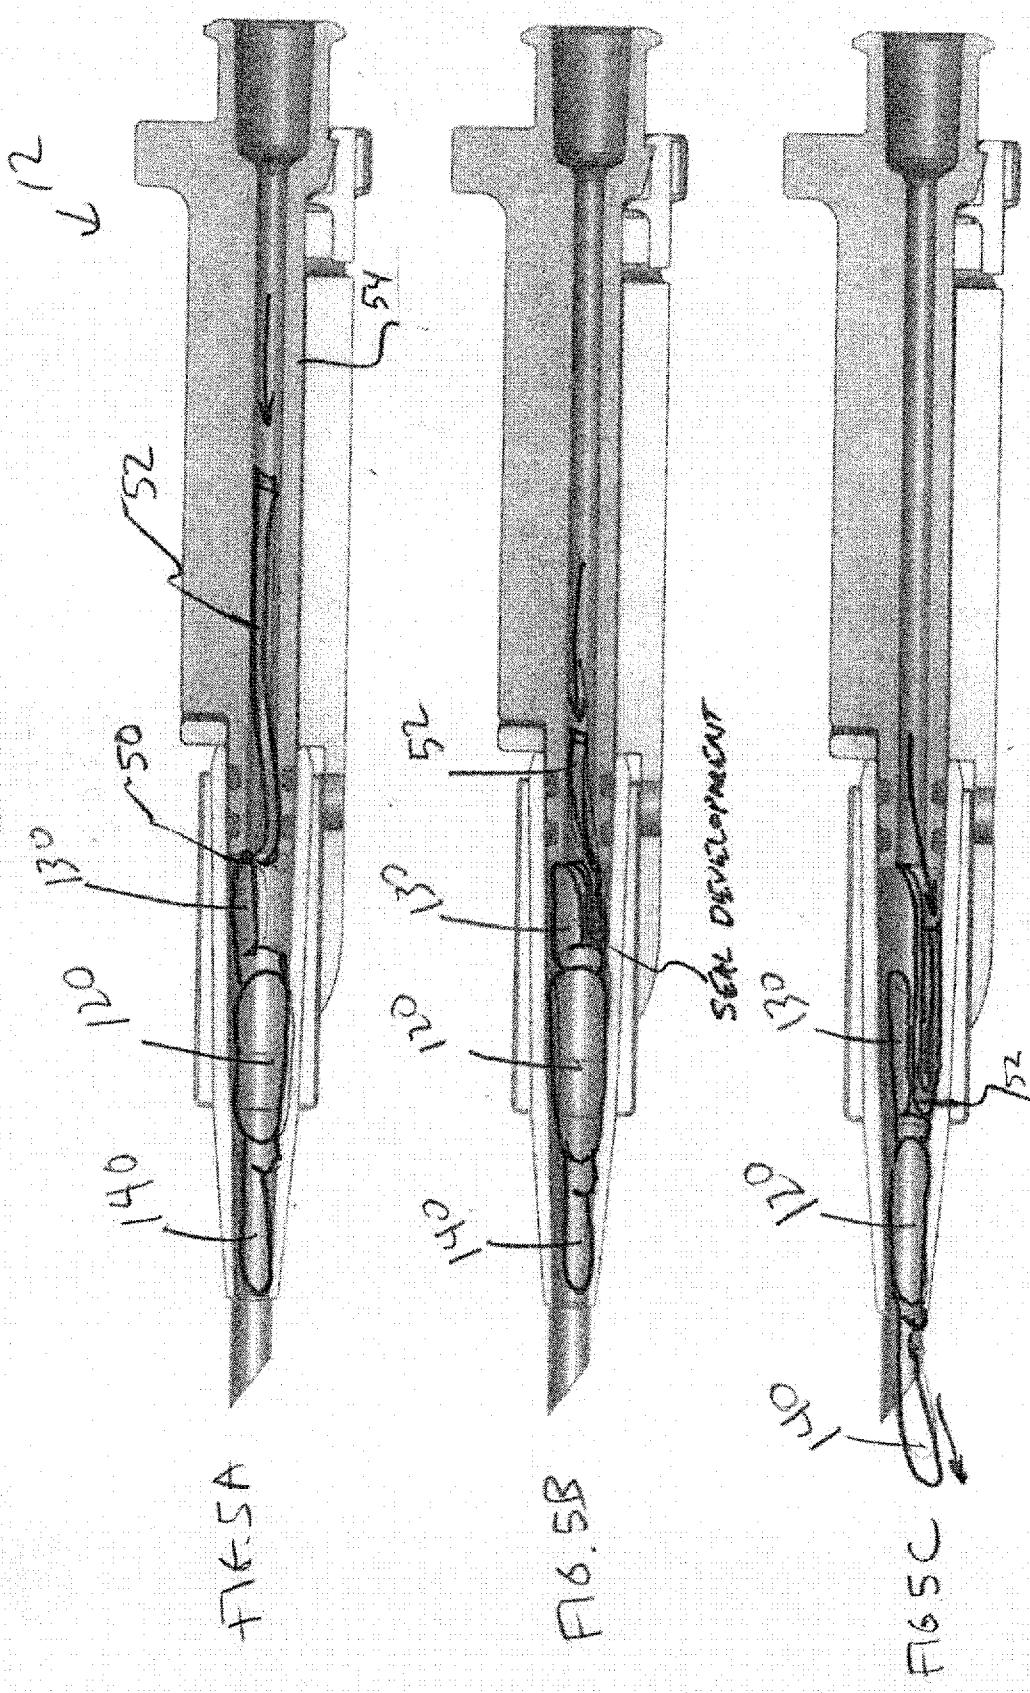


6/17

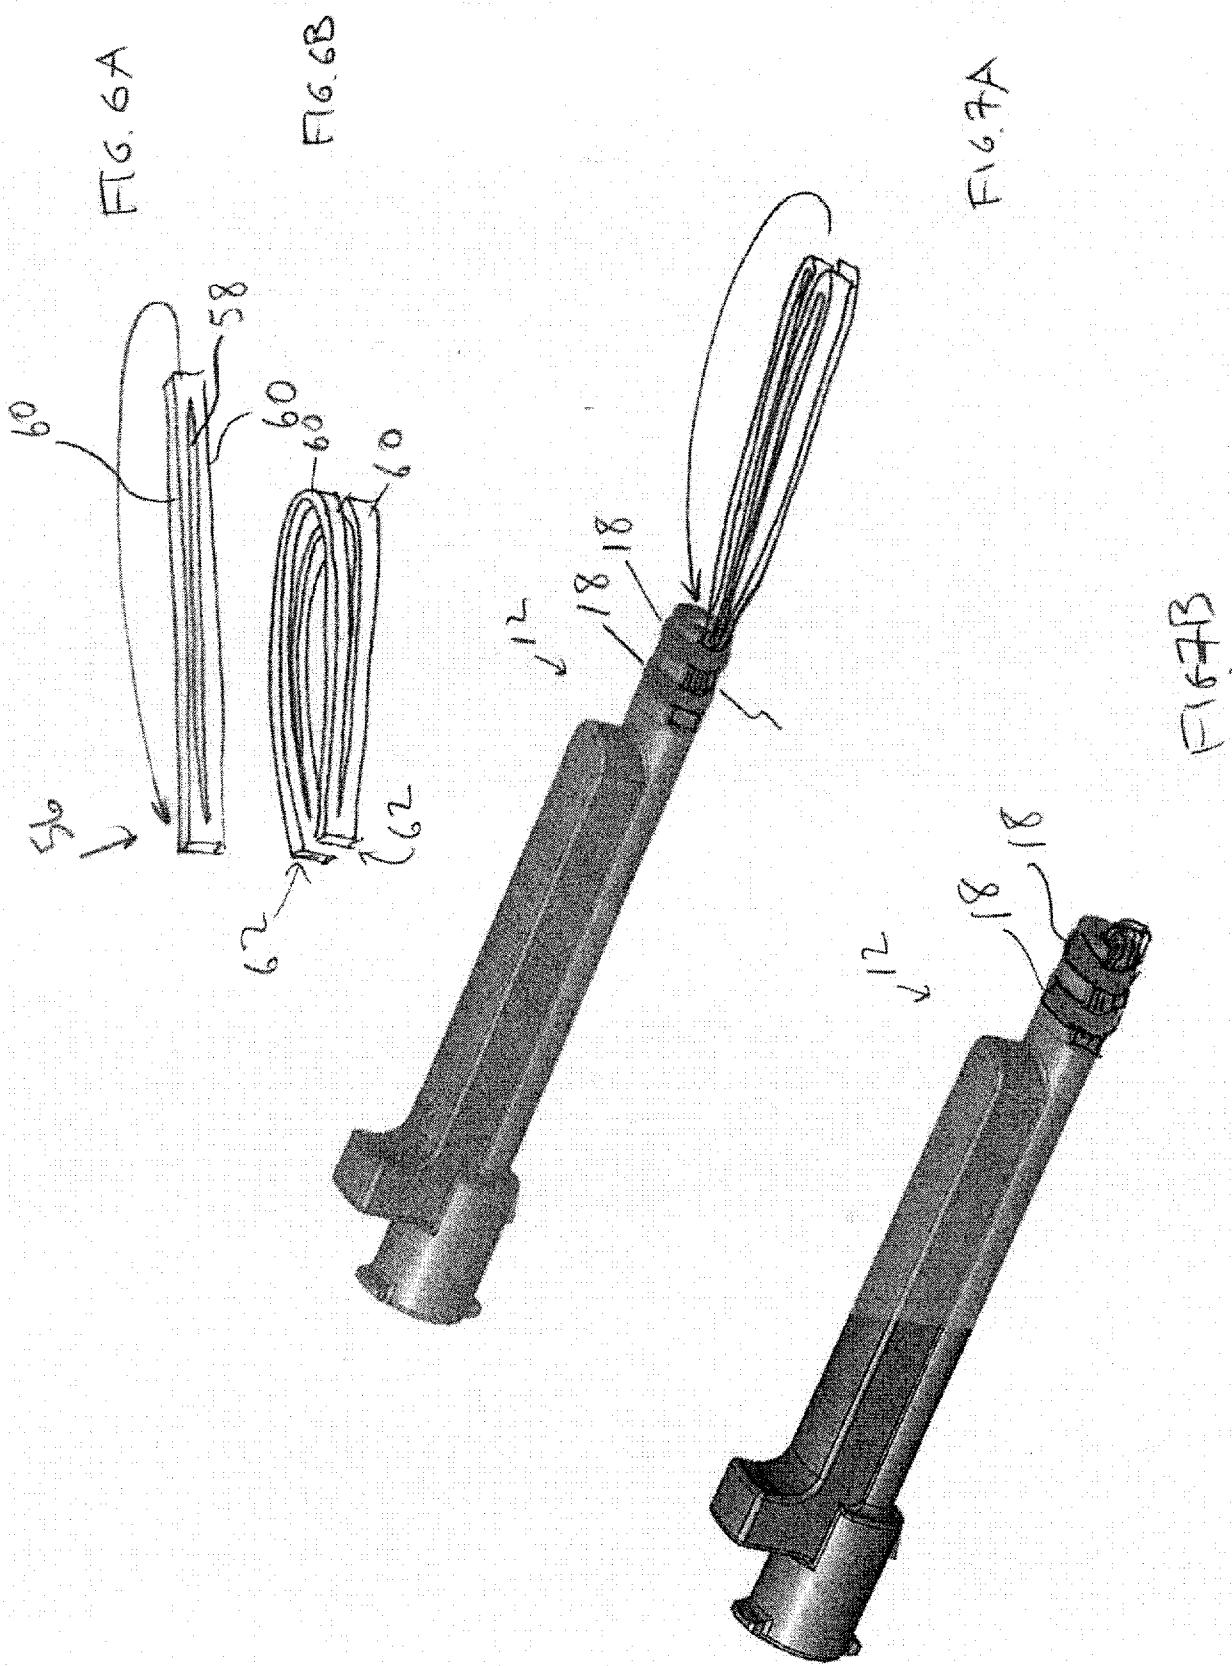


7/17

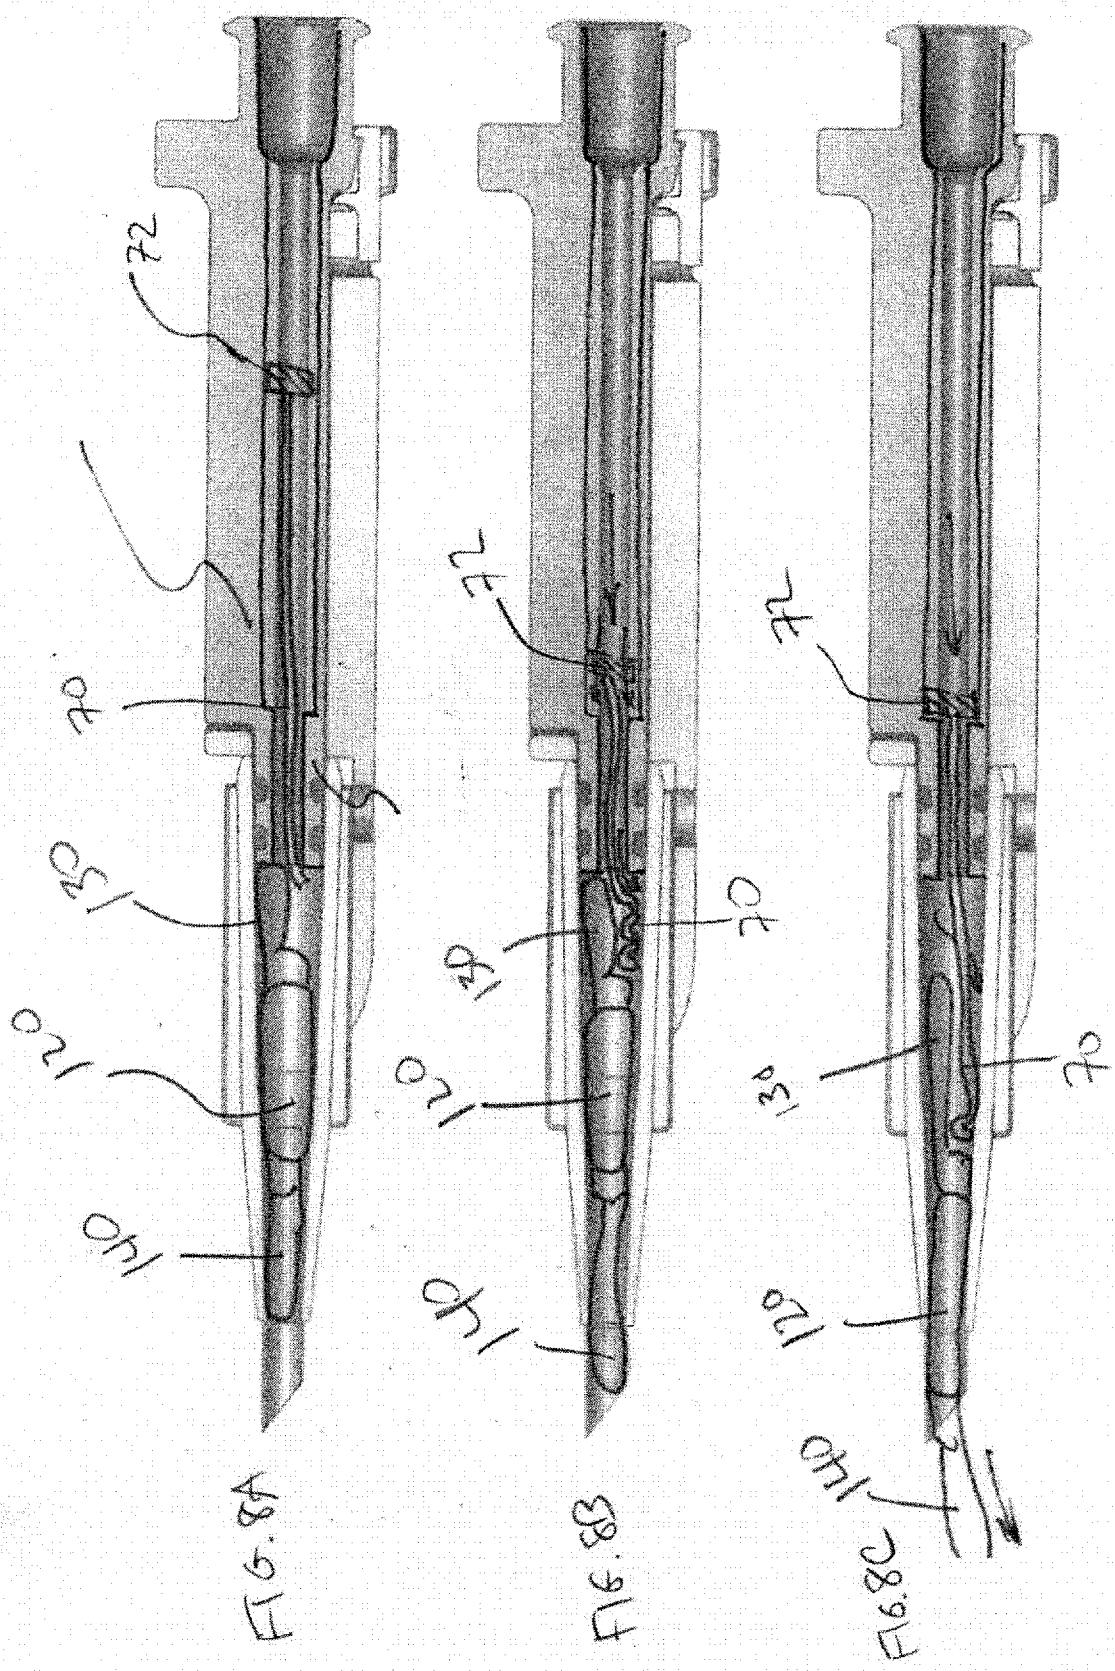


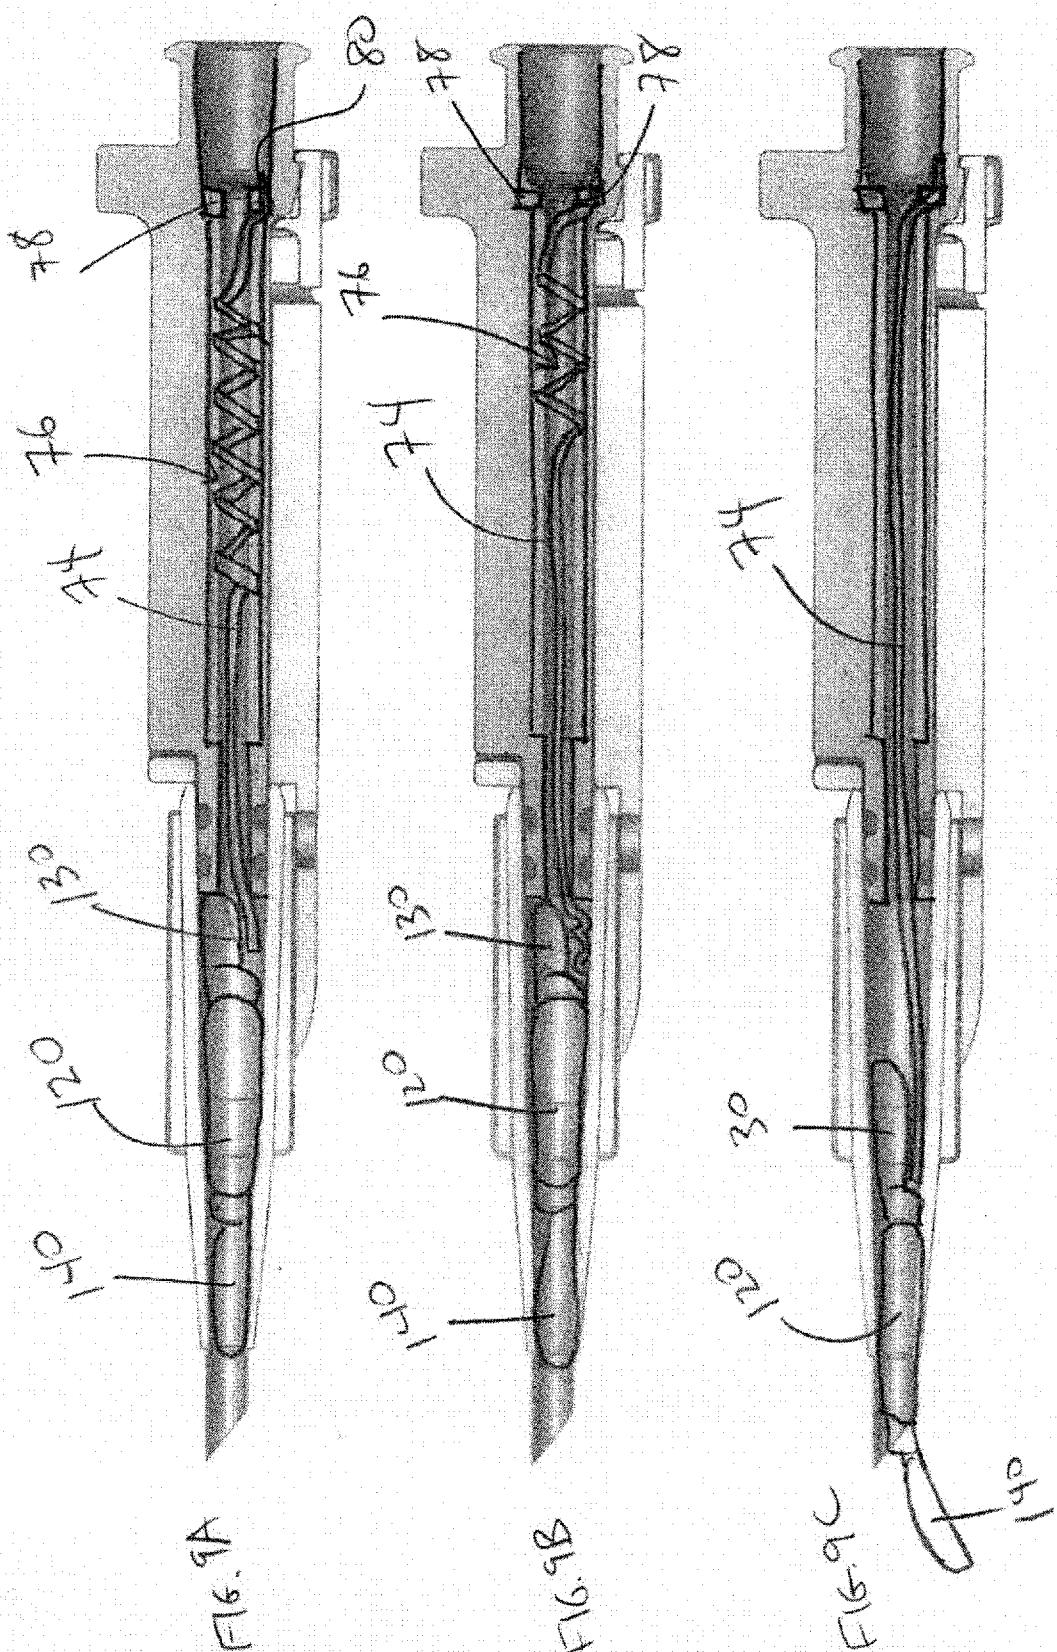

9/17

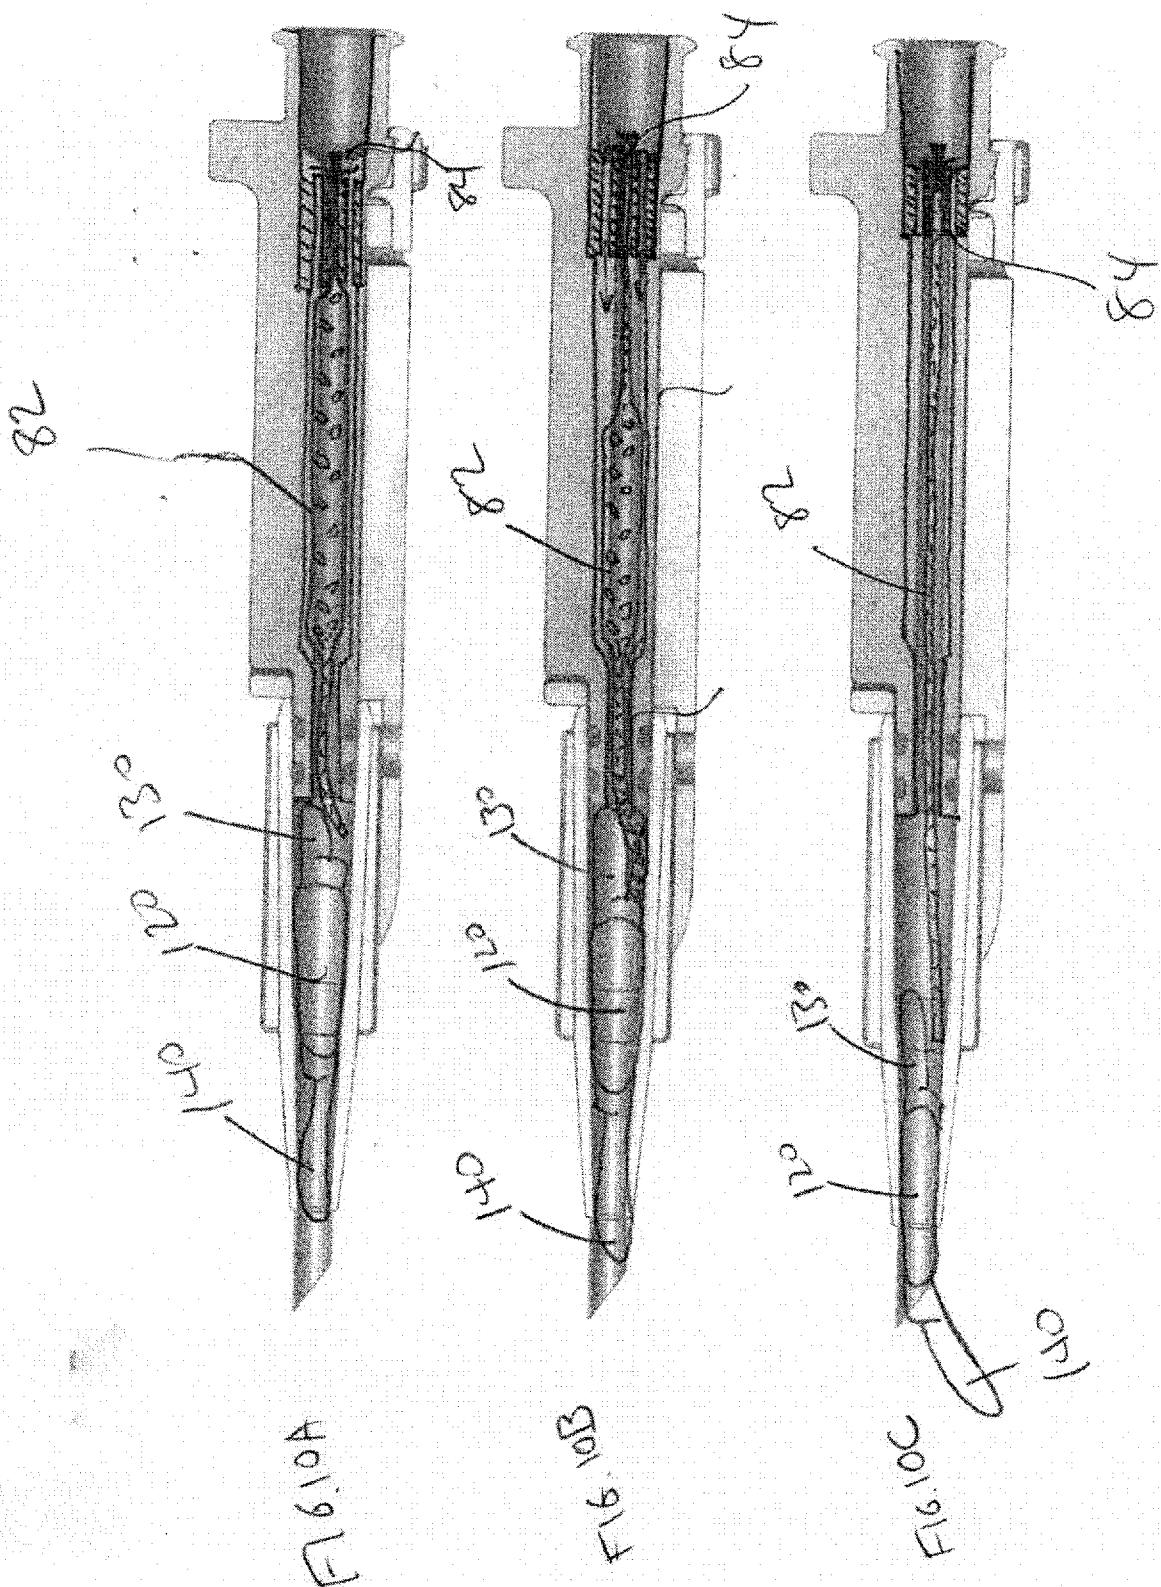

10 / 17

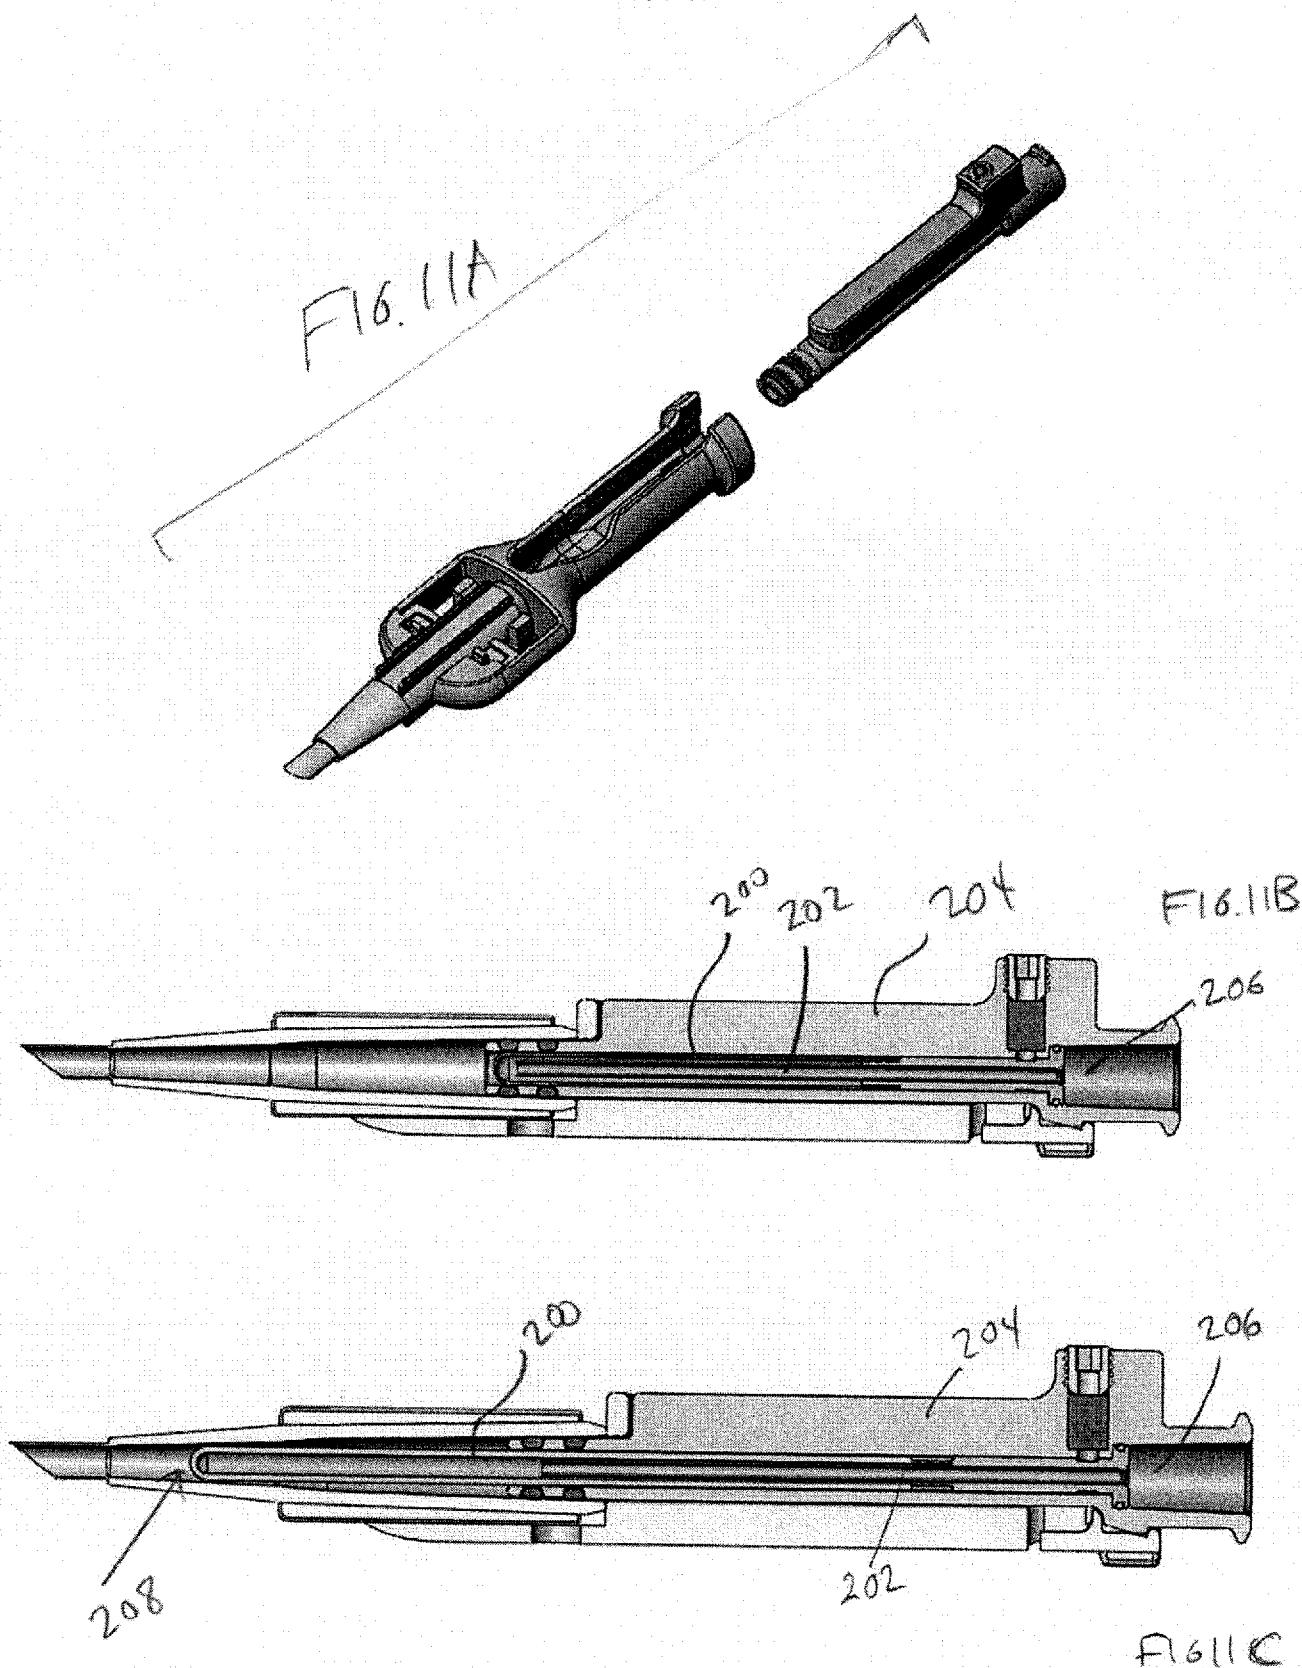

11 / 17

FIG. 12A






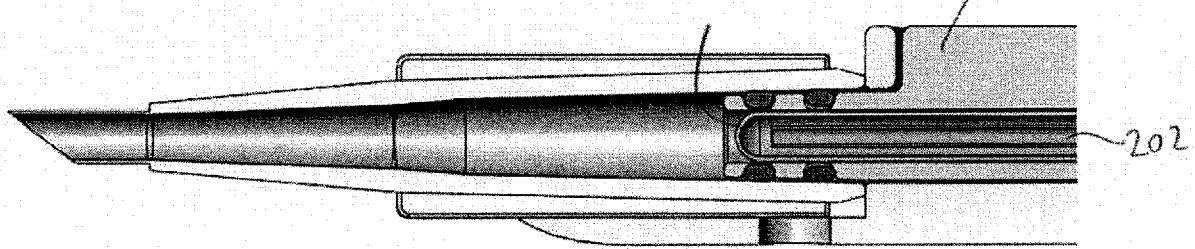



FIG. 12B

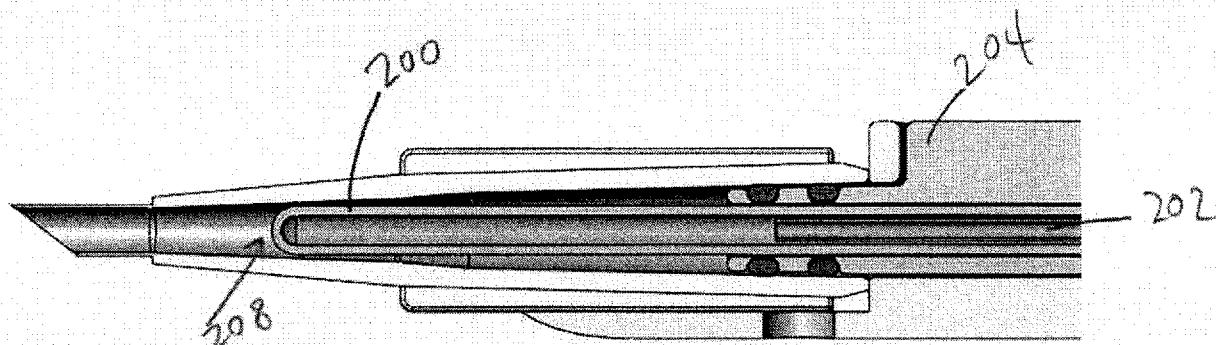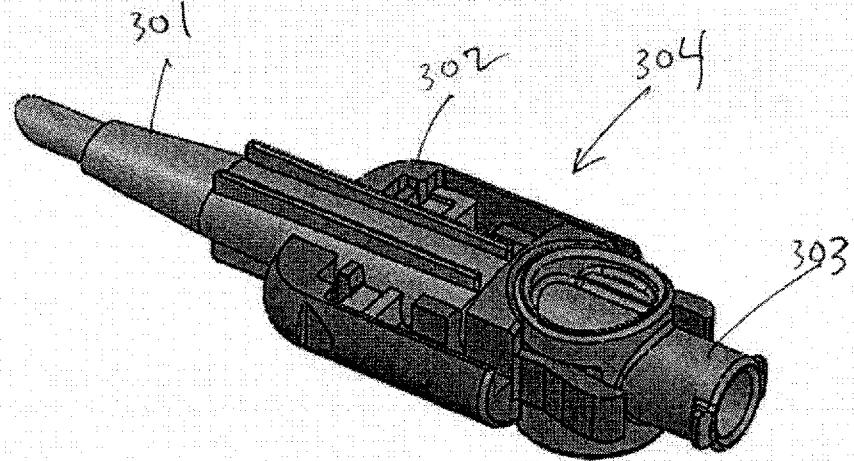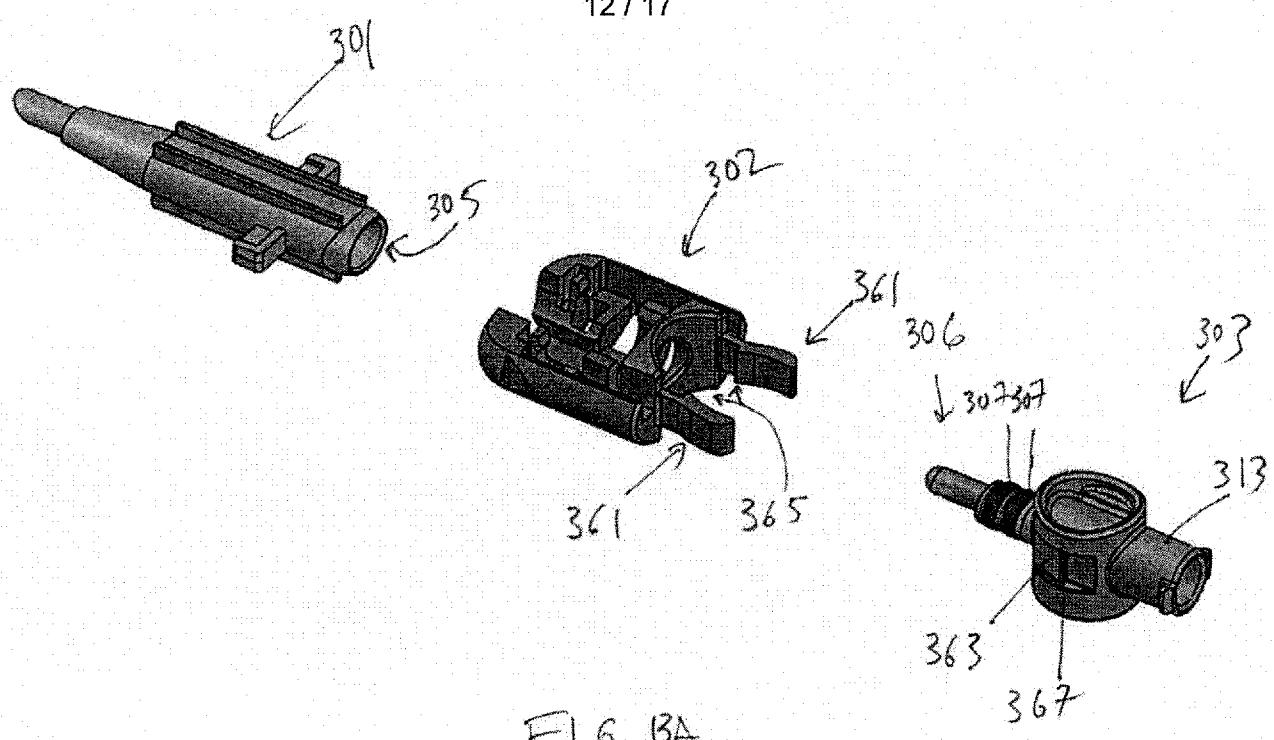





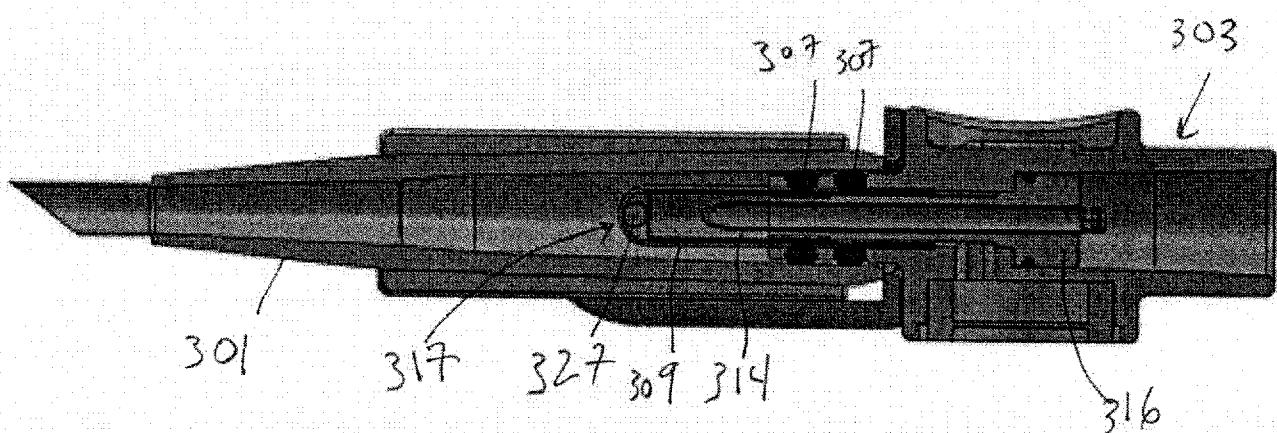


13/17

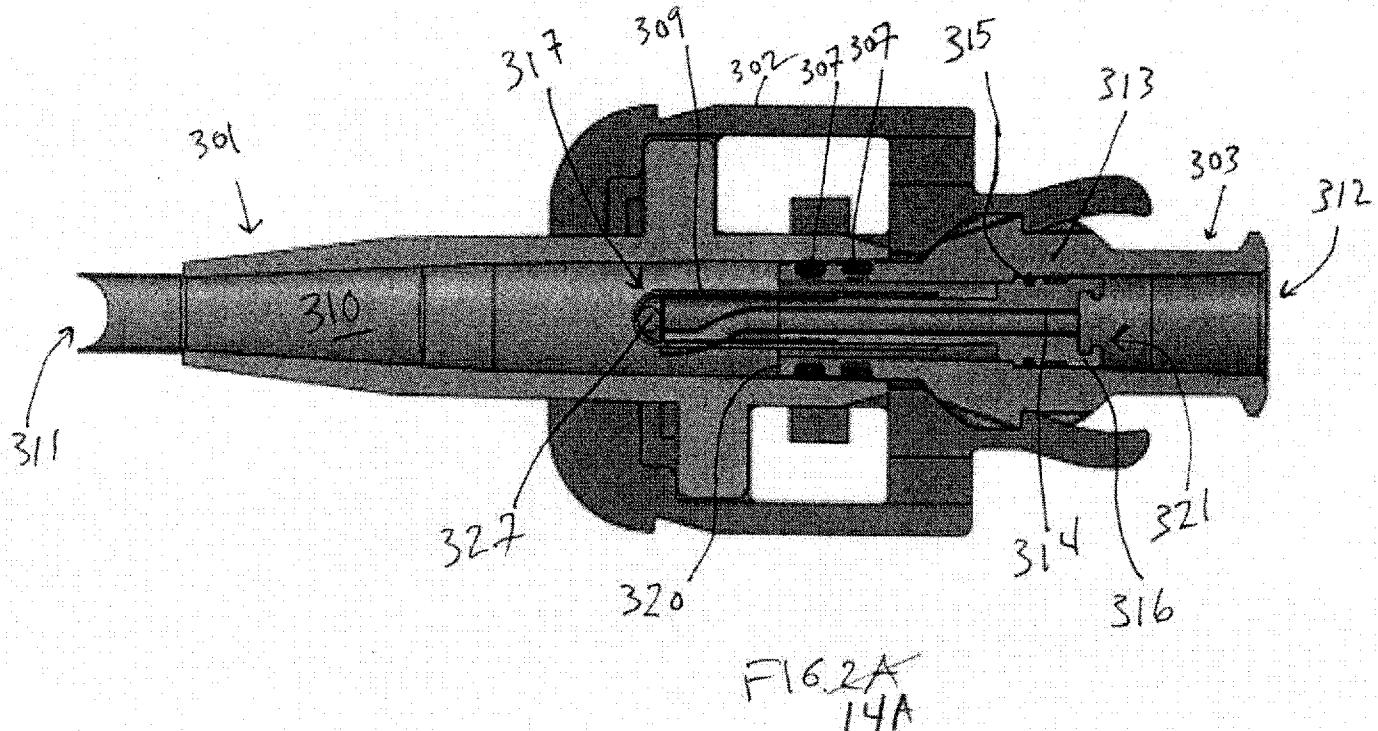


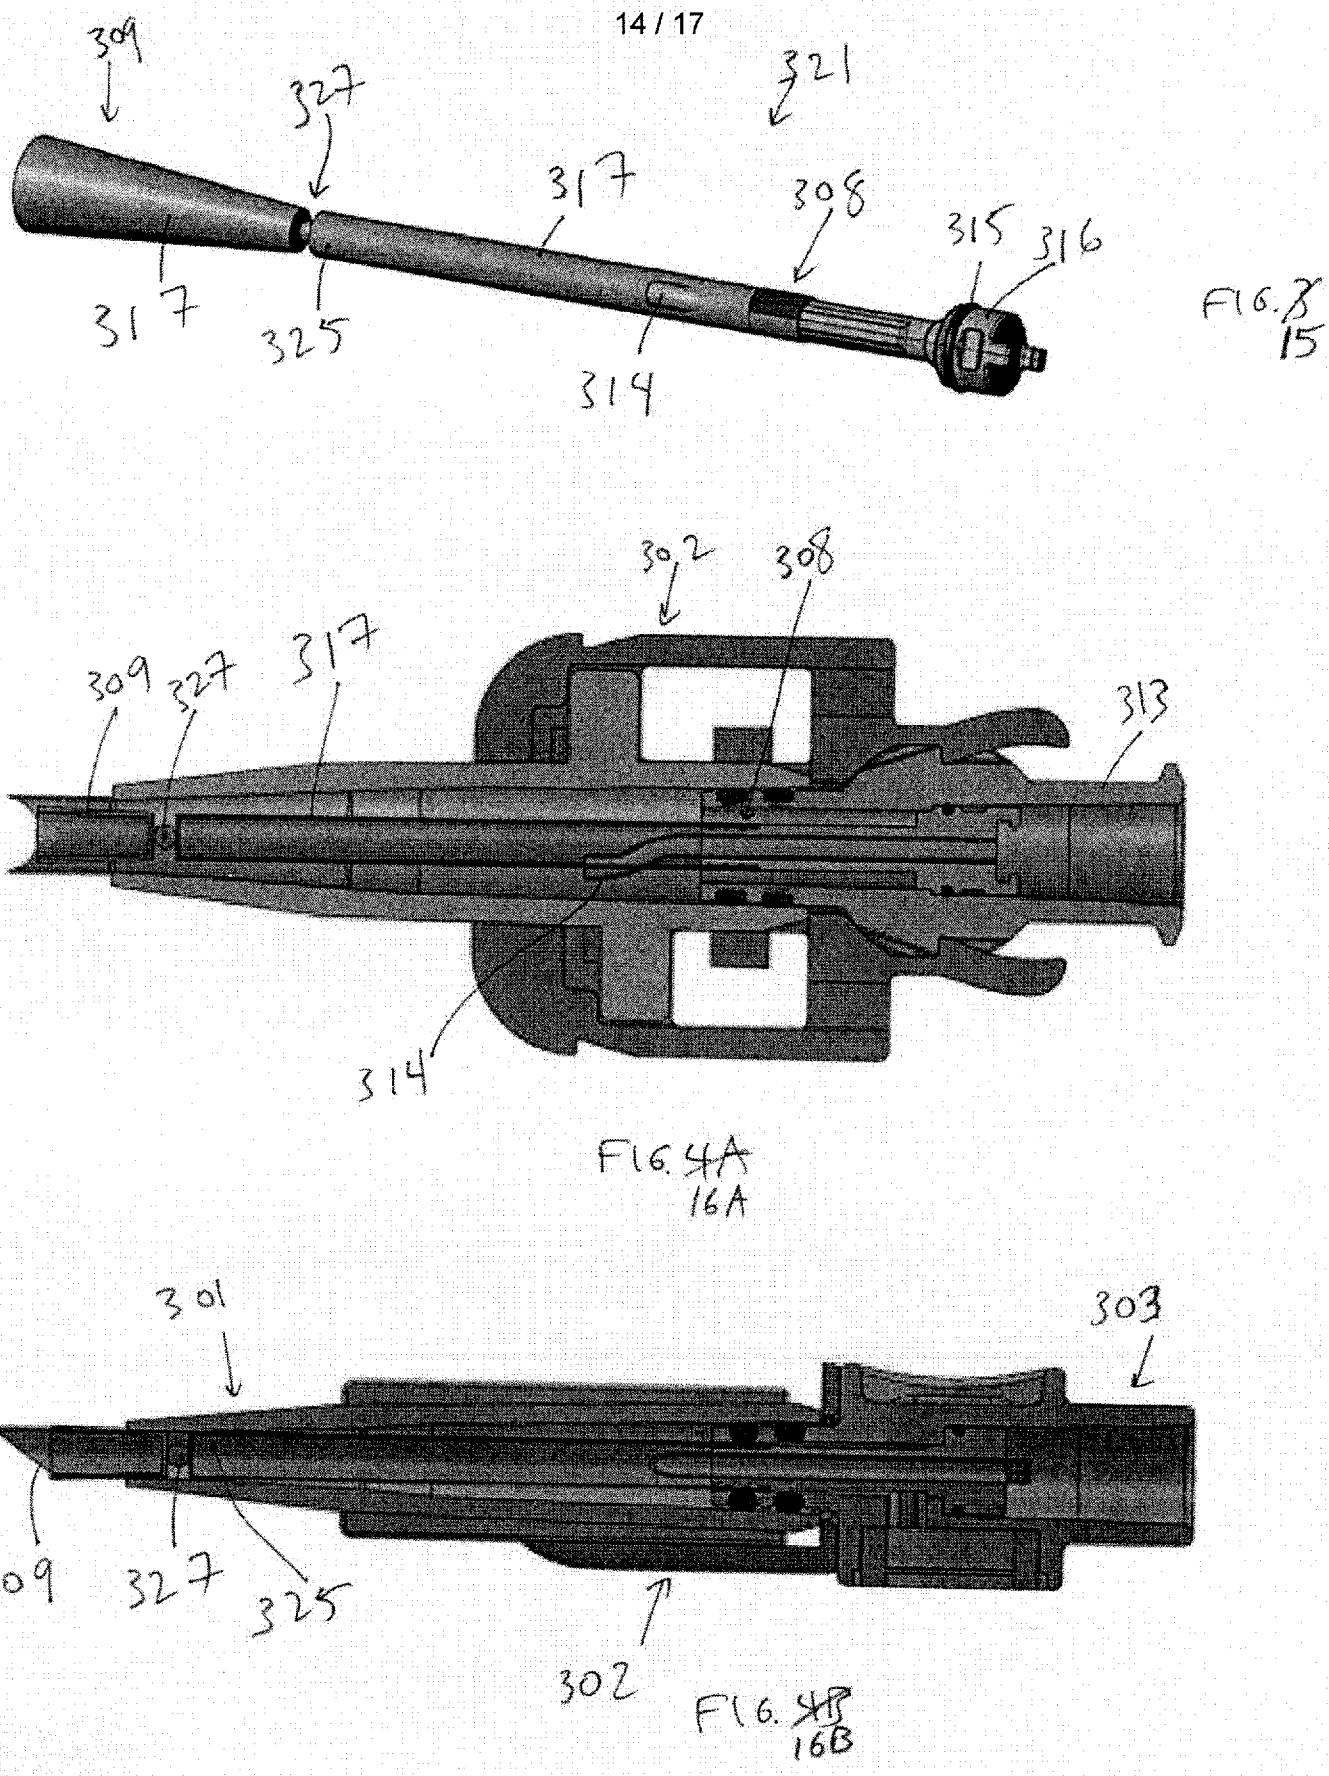

15 / 17

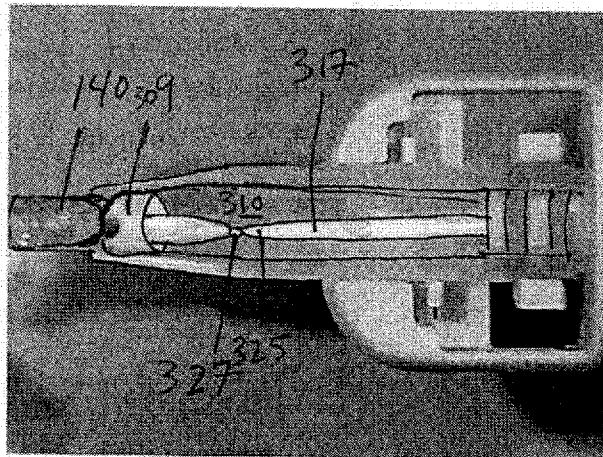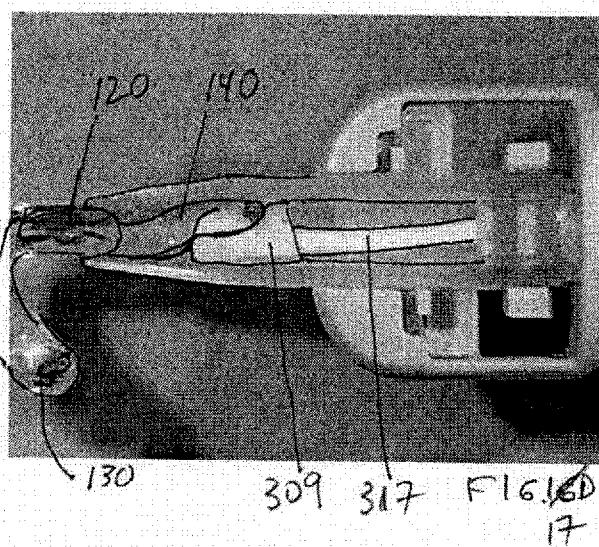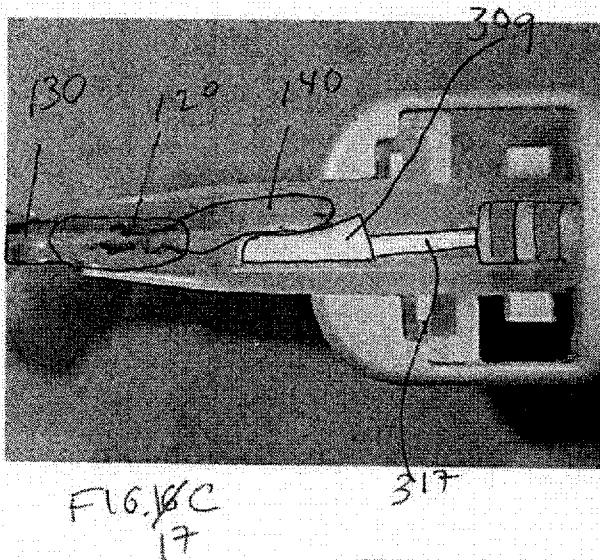
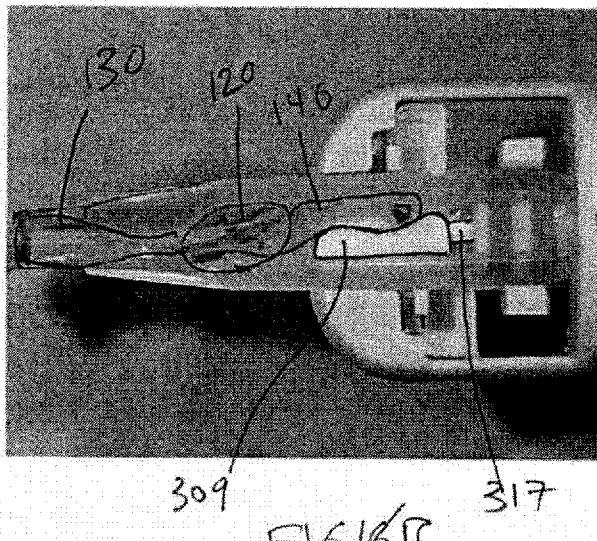
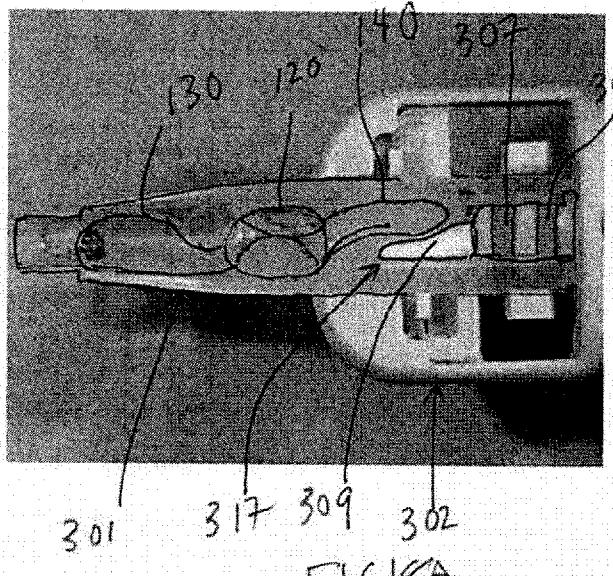


16 / 17

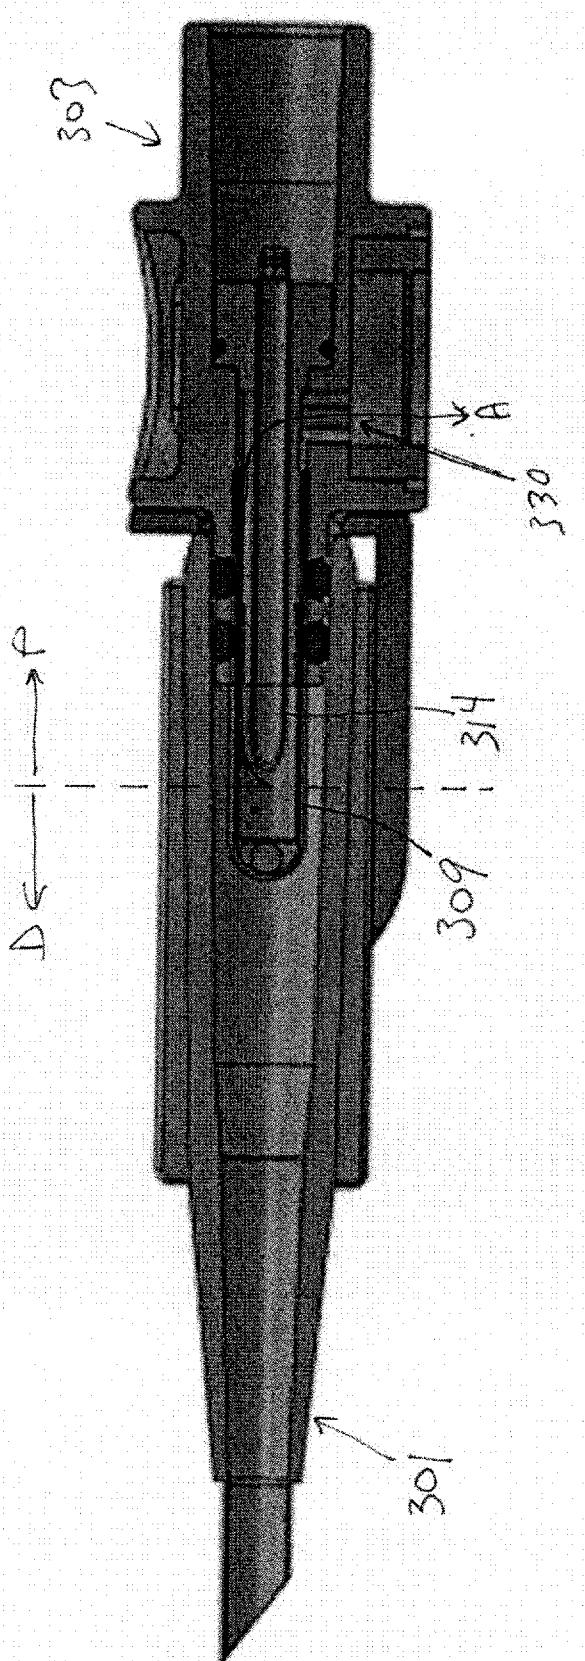

16. 7/8

17/17

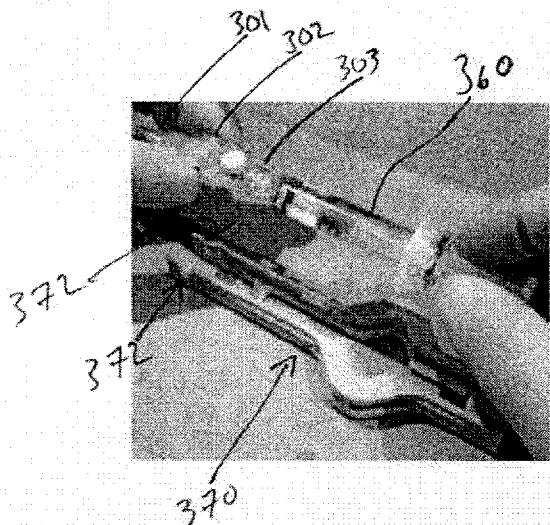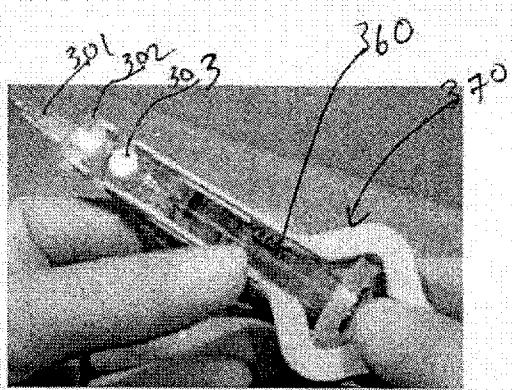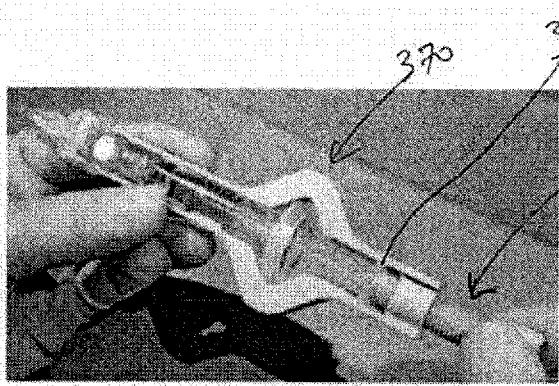F16.8A  
19AF16.8B  
19F16.8C  
19

## INTERNATIONAL SEARCH REPORT

International application No.  
**PCT/US2013/032054****A. CLASSIFICATION OF SUBJECT MATTER****A61F 2/16(2006.01)i, A61F 2/14(2006.01)i, A61F 2/76(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**Minimum documentation searched (classification system followed by classification symbols)  
A61F 2/16; A61F 9/007; A61B 17/00; A61M 5/315; A61F 2/14; A61F 2/76Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched  
Korean utility models and applications for utility models  
Japanese utility models and applications for utility modelsElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)  
eKOMPASS(KIPO internal) & Keywords: intraocular lens, delivery, fluid, plug, vent**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 2060243 A1 (STAAR JAPAN INC.) 20 May 2009 See abstract; paragraphs [0021],[0022]; figure 1.	9-26
X	EP 2074962 A1 (MENICON CO., LTD.) 1 July 2009 See abstract; paragraphs [0025],[0076],[0082]; figure 1.	26
A		9-25
A	WO 2007-005692 A1 (ADVANCED MEDICAL OPTICS, INC.) 11 January 2007 See abstract; paragraphs [0052],[0062],[0043]; figures 4, 6.	9-26
A	JP 2008-307394 A (STAAR JAPAN INC.) 25 December 2008 See abstract; paragraph [0038]; figures 2, 3.	9-26
A	US 2010-0161049 A1 (INOUE, M.) 24 June 2010 See abstract; paragraph [0042]; figure 1.	9-26

 Further documents are listed in the continuation of Box C. See patent family annex.

\* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance  
 "E" earlier application or patent but published on or after the international filing date  
 "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of citation or other special reason (as specified)  
 "O" document referring to an oral disclosure, use, exhibition or other means  
 "P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search  
25 June 2013 (25.06.2013)

Date of mailing of the international search report

**28 June 2013 (28.06.2013)**Name and mailing address of the ISA/KR  
  
 Korean Intellectual Property Office  
 189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City,  
 302-701, Republic of Korea  
 Facsimile No. 82-42-472-7140

Authorized officer

KIM, Sung Gon

Telephone No. 82-42-481-8746



**INTERNATIONAL SEARCH REPORT**

International application No.

**PCT/US2013/032054****Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1.  Claims Nos.: 1-8,27  
because they relate to subject matter not required to be searched by this Authority, namely:  
Claims 1-8, 27 pertain to methods for treatment of the human body and thus relate to a subject-matter which this International Searching Authority is not required, under Article 17(2)(a)(i) of the PCT and Rule 39.1(iv) of the Regulations under the PCT, to search.
2.  Claims Nos.:  
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3.  Claims Nos.:  
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

**Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)**

This International Searching Authority found multiple inventions in this international application, as follows:

1.  As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2.  As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3.  As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4.  No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

**Remark on Protest**

- The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- No protest accompanied the payment of additional search fees.

**INTERNATIONAL SEARCH REPORT**

Information on patent family members

International application No.

**PCT/US2013/032054**

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP 2060243 A1	20.05.2009	AT 526907 T EP 2060243 B1	15.10.2011 05.10.2011
EP 2074962 A1	01.07.2009	AT 551018 T CN 101467925 A CN 101467925 B EP 2074962 B1 ES 2384355 T3 HK 1133812 A1 JP 2009-160151 A US 2009-0171366 A1 US 8080017 B2	15.04.2012 01.07.2009 27.06.2012 28.03.2012 04.07.2012 09.11.2012 23.07.2009 02.07.2009 20.12.2011
WO 2007-005692 A1	11.01.2007	AU 2006-265859 A1 BR PI0612615A 2 CA 2613448 A1 EP 1909698 A1 JP 2008-544816 A US 2007-0005135 A1	11.01.2007 20.03.2012 11.01.2007 16.04.2008 11.12.2008 04.01.2007
JP 2008-307394 A	25.12.2008	CN 1985781 A CN 1985781 B EP 1800623 A1 JP 04234156 B2 JP 2007-190360 A US 2008-0027460 A1	27.06.2007 13.10.2010 27.06.2007 04.03.2009 02.08.2007 31.01.2008
US 2010-0161049 A1	24.06.2010	EP 2177178 A1 JP 05086713 B2 JP 2009-018009 A SG 183003 A1 WO 2009-008441 A1	21.04.2010 28.11.2012 29.01.2009 30.08.2012 15.01.2009