



(12) **United States Design Patent**  
**Terry et al.**

(10) **Patent No.:** **US D888,252 S**  
(45) **Date of Patent:** **\*\* Jun. 23, 2020**

(54) **TRANSCUTANEOUS ANALYTE SENSOR APPLICATOR**

(56) **References Cited**

(71) Applicant: **DexCom, Inc.**, San Diego, CA (US)  
(72) Inventors: **Warren Terry**, Poway, CA (US);  
**Patrick John Castagna**, San Diego, CA (US); **David A. Keller**, Encinitas, CA (US); **Young Woo Lee**, San Diego, CA (US); **Joseph J. Baker**, Vista, CA (US); **Randall Scott Koplín**, Middleton, WI (US); **Andrew Joncich**, Madison, WI (US)

U.S. PATENT DOCUMENTS

3,759,375 A	9/1973	Nappi
4,511,035 A	4/1985	Alpem
5,390,671 A	2/1995	Lord et al.
5,575,403 A	11/1996	Charlton
5,586,553 A	12/1996	Halili et al.
5,868,253 A	2/1999	Krueger et al.
7,494,465 B2	2/2009	Brister et al.
7,497,827 B2	3/2009	Brister et al.

(Continued)

(73) Assignee: **DexCom, Inc.**, San Diego, CA (US)

(\*\*) Term: **15 Years**

(21) Appl. No.: **29/653,761**

(22) Filed: **Jun. 18, 2018**

OTHER PUBLICATIONS

International Search Report and Written Opinion for Application No. PCT/US2018/038117 dated Nov. 28, 2018, 15 pages.

*Primary Examiner* — Anhdao Doan

(74) *Attorney, Agent, or Firm* — Knobbe, Martens, Olson & Bear, LLP

**Related U.S. Application Data**

(63) Continuation-in-part of application No. 16/011,527, filed on Jun. 18, 2018.

(51) **LOC (12) Cl.** ..... **24-01**

(52) **U.S. Cl.**  
USPC ..... **D24/186; D24/169**

(58) **Field of Classification Search**  
USPC ..... D24/107, 167, 186, 187, 112, 169;  
D10/70, 75, 98, 97, 81; D14/344  
CPC ..... A61B 5/6801; A61B 5/681; A61B 5/6819;  
A61B 5/6823; A61B 5/6824; A61B  
5/02405; A61B 5/02427; A61B 5/02438;  
A61B 5/0245; A61B 5/0402; A61B  
5/0404; A61B 5/0004; A61B 5/14503;  
A61B 5/14532; A61B 5/14865; A61B  
5/6832; A61B 5/6833; A61B 5/6849;  
A61B 2560/0412; A61B 2560/0443;  
A61B 2560/0462; A61B 25/0206; A61M  
25/0206

See application file for complete search history.

(57) **CLAIM**

The ornamental design for a transcutaneous analyte sensor applicator, as shown and described.

**DESCRIPTION**

FIG. 1 is a top, front, and right-side perspective view of a transcutaneous analyte sensor applicator showing our design;

FIG. 2 is a front view thereof;

FIG. 3 is a rear view thereof;

FIG. 4 is a right-side view thereof;


FIG. 5 is a left-side view thereof;

FIG. 6 is a top view thereof; and,

FIG. 7 is a bottom view thereof.

The broken lines illustrate portions of the transcutaneous analyte sensor applicator that form no part of the claimed design.

**1 Claim, 4 Drawing Sheets**

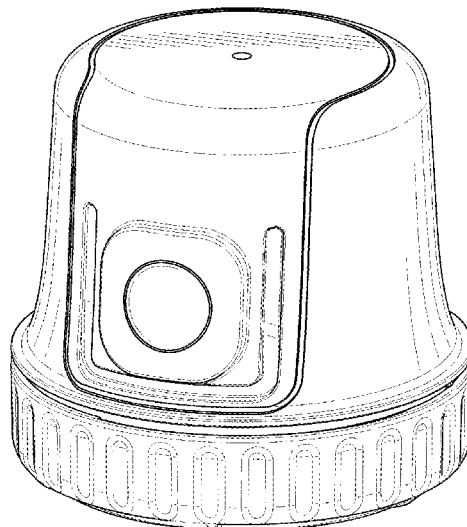

(56)

References Cited

U.S. PATENT DOCUMENTS

D603,050 S *	10/2009	Chen .....	D24/187	9,402,544 B2	8/2016	Yee et al.	
7,774,145 B2	8/2010	Brauker et al.		9,402,570 B2	8/2016	Pace et al.	
8,252,229 B2	8/2012	Thomas et al.		9,636,068 B2	5/2017	Yee et al.	
8,275,437 B2	9/2012	Brauker et al.		D794,800 S *	8/2017	Gobrecht .....	D24/169
8,396,528 B2	3/2013	Kamath et al.		9,717,843 B2	8/2017	Grucela et al.	
8,478,377 B2	7/2013	Shariati et al.		10,029,043 B2	7/2018	Grucela et al.	
D691,710 S *	10/2013	White .....	D24/107	2002/0119711 A1	8/2002	VanAntwerp et al.	
D693,927 S *	11/2013	Wilson .....	D24/167	2008/0114280 A1	5/2008	Stafford	
8,684,172 B2	4/2014	Yao		2011/0319729 A1 *	12/2011	Donnay .....	A61B 5/15194 600/309
D705,422 S *	5/2014	Burton .....	D24/112	2012/0227358 A1	9/2012	Larson et al.	
8,783,102 B2	6/2014	Heck et al.		2016/0106349 A1	4/2016	Pryor et al.	
8,764,657 B2	7/2014	Curry et al.		2016/0128615 A1	5/2016	Curry et al.	
8,802,006 B2	8/2014	Thomas et al.		2017/0112531 A1	4/2017	Schoonmaker et al.	
9,101,305 B2	8/2015	Larson et al.		2017/0112534 A1 *	4/2017	Schoonmaker .....	A61B 5/0004
9,239,252 B2	1/2016	Koga et al.		2017/0188910 A1	7/2017	Halac et al.	
9,265,453 B2	2/2016	Curry et al.		2018/0296749 A1	10/2018	Grucela et al.	
9,357,951 B2	6/2016	Simpson et al.		2018/0360357 A1	12/2018	Baker et al.	
				2018/0360358 A1	12/2018	Baker et al.	
				2018/0360493 A1	12/2018	Baker et al.	

\* cited by examiner

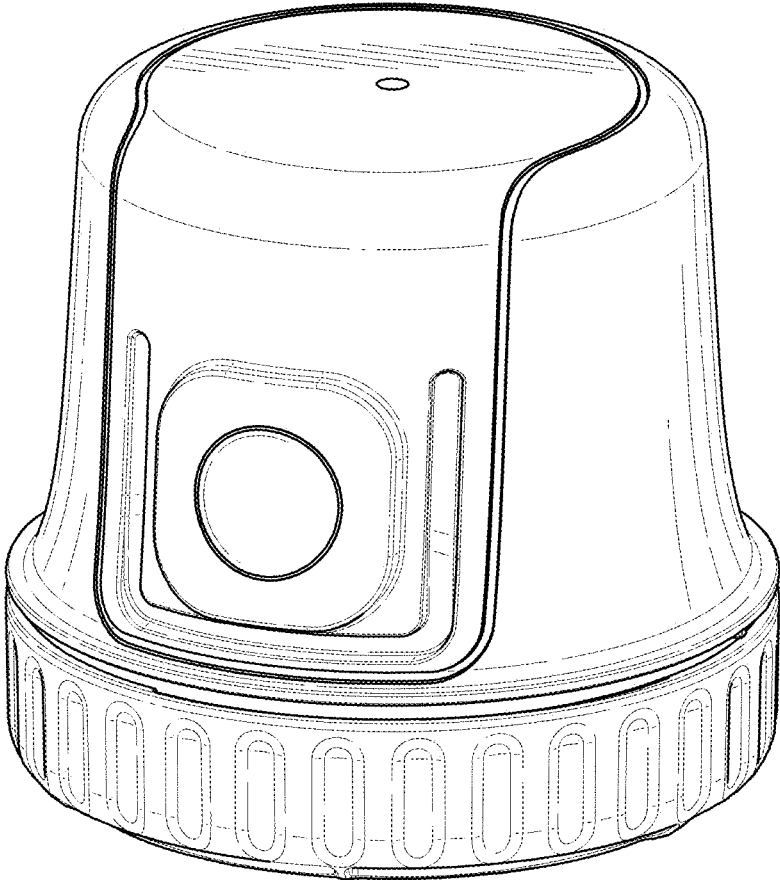


FIG. 1

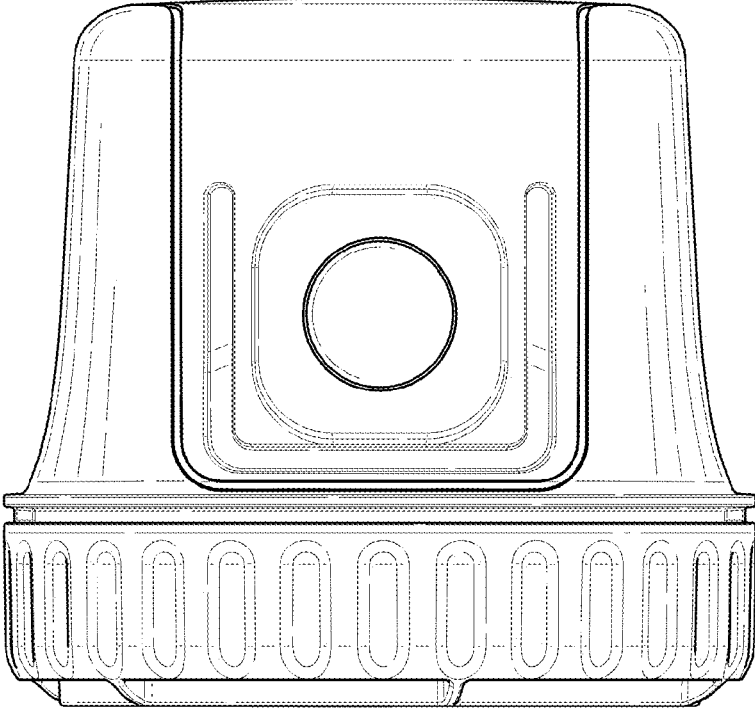


FIG. 2

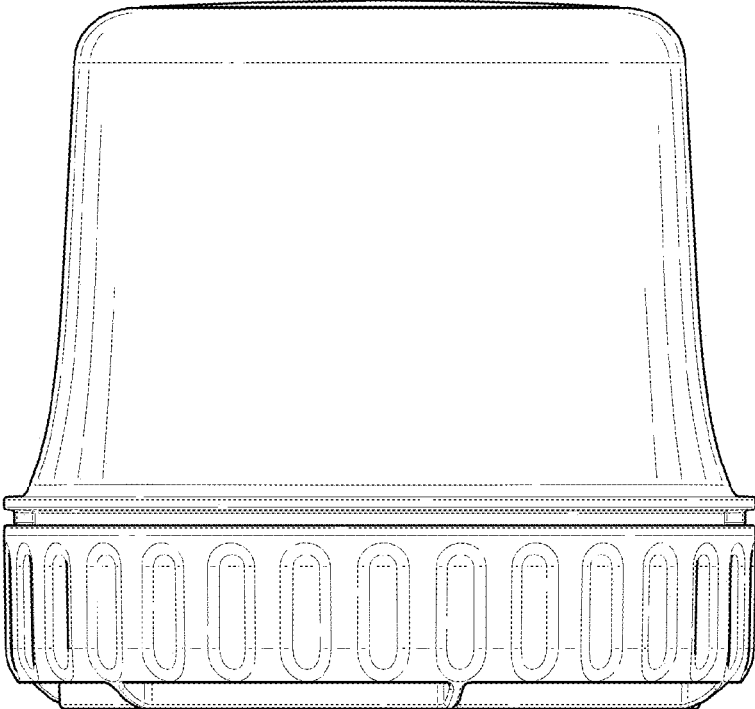


FIG. 3

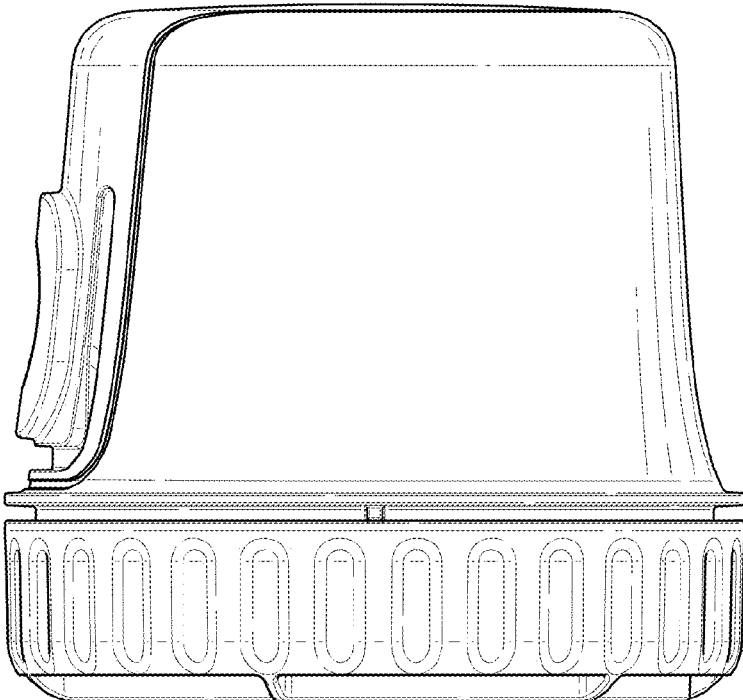


FIG. 4

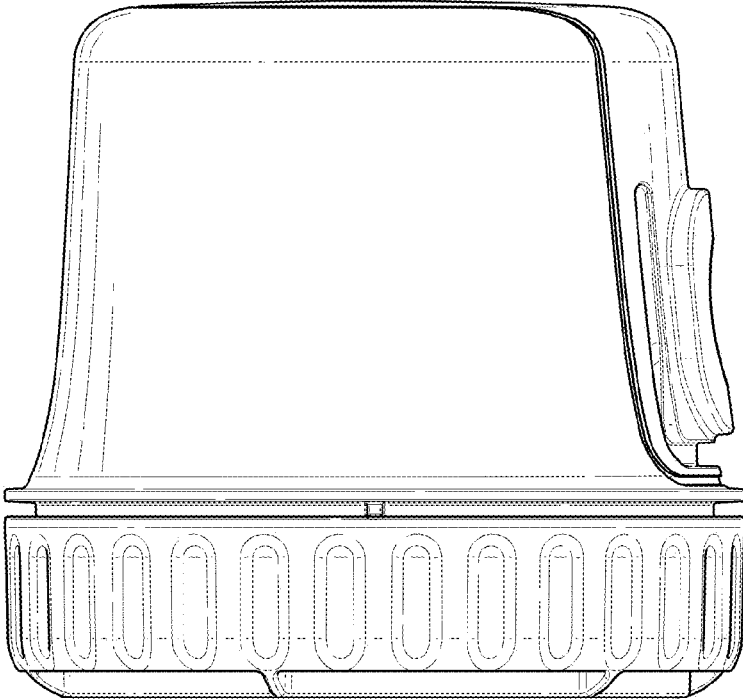


FIG. 5

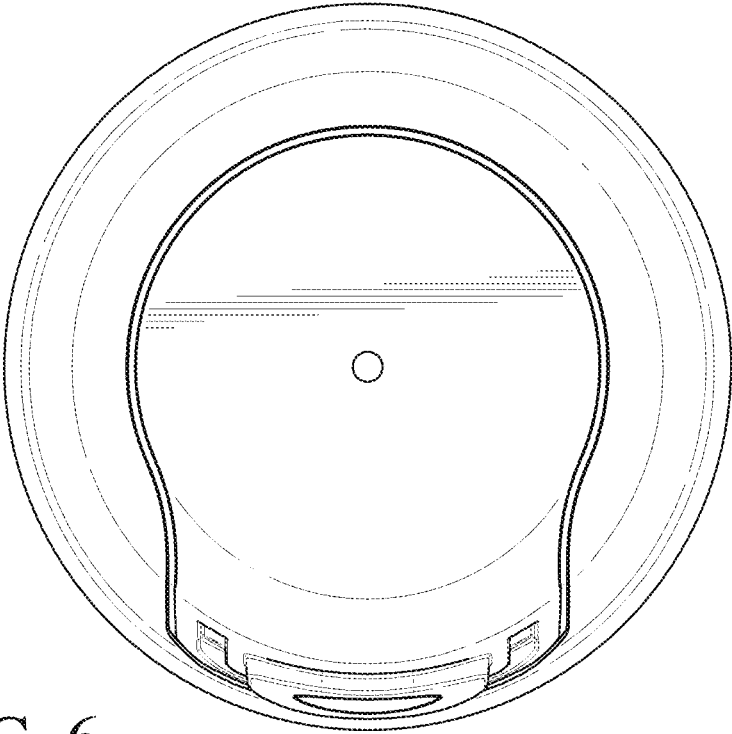


FIG. 6

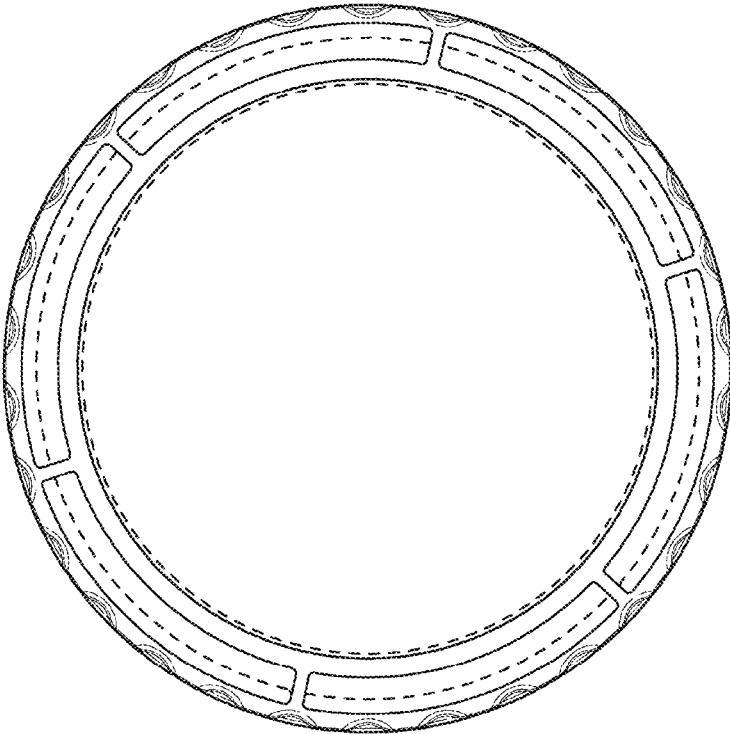


FIG. 7