



## (51) International Patent Classification:

A61B 18/04 (2006.01) A61B 19/00 (2006.01)  
A61B 17/32 (2006.01)

## (21) International Application Number:

PCT/US2011/059358

## (22) International Filing Date:

4 November 2011 (04.11.2011)

## (25) Filing Language:

English

## (26) Publication Language:

English

## (30) Priority Data:

61/410,603	5 November 2010 (05.11.2010)	US
61/487,846	19 May 2011 (19.05.2011)	US
13/276,660	19 October 2011 (19.10.2011)	US

## (71) Applicant (for all designated States except US):

**ETHICON ENDO-SURGERY, INC.** [US/US]; 4545  
Creek Road, Cincinnati, OH 45242 (US).

## (72) Inventors; and

(75) Inventors/Applicants (for US only): **HOUSER, Kevin,**

**L.** [US/US]; 570 Foliage Lane, Springboro, OH 45066  
(US). **DANNAHER, William, D.** [US/US]; 8907 Eldora  
Drive, Cincinnati, OH 45236 (US). **DIETZ, Timothy, G.**  
[US/US]; 9 Elm Ledge, Terrace Park, OH 45174 (US).  
**STULEN, Foster, B.** [US/US]; 6245 Bridgewater Court,  
Mason, OH 45040 (US). **SHELTON, Frederick, E., IV**  
[US/US]; 245 East Main Street, Hillsboro, OH 45133  
(US). **YATES, David, C.** [US/US]; 7534 Galway Court,  
West Chester, OH 45069 (US). **WORRELL, Barry, C.**  
[US/US]; 1647 Lago Mar Drive, Centerville, OH 45458  
(US).

(74) Agents: **JOHNSON, Philip, S.** et al.; Johnson & John-  
son, One Johnson & Johnson Plaza, New Brunswick, NJ  
08933 (US).

## (81) Designated States (unless otherwise indicated, for every

kind of national protection available): AE, AG, AL, AM,  
AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ,  
CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO,  
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT,  
HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP,  
KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD,  
ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI,  
NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU,  
RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ,  
TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA,  
ZM, ZW.

## (84) Designated States (unless otherwise indicated, for every

kind of regional protection available): ARIPO (BW, GH,  
GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ,  
UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD,  
RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ,  
DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT,  
LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS,  
SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM,  
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

## Declarations under Rule 4.17:

- as to the identity of the inventor (Rule 4.17(i))
- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

[Continued on next page]

## (54) Title: USER FEEDBACK THROUGH HANDPIECE OF SURGICAL INSTRUMENT

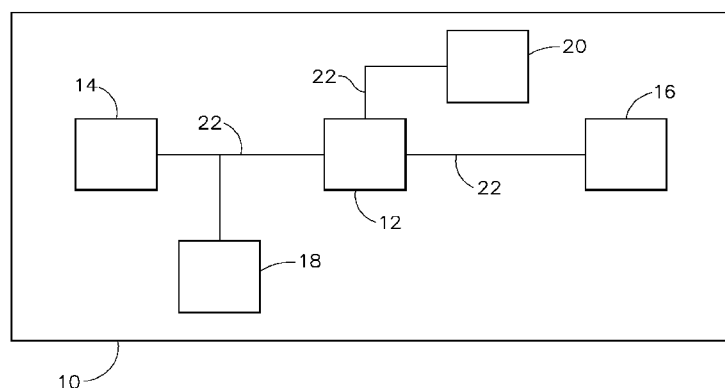


Fig.1

(57) **Abstract:** A surgical instrument includes a handpiece having a user input feature and a user feedback feature. A shaft assembly extends distally from the handpiece. An end effector is disposed at a distal end of the shaft assembly. The end effector includes an active feature responsive to actuation of the user input feature. The active feature is operable to operate on tissue in response to actuation of the user input feature. The user feedback feature is operable to provide feedback to the user that indicates information relating to operation of the end effector. The feedback may include haptic, visual, and/or auditory feedback.



---

**Published:**

- *without international search report and to be republished  
upon receipt of that report (Rule 48.2(g))*

## USER FEEDBACK THROUGH HANDPIECE OF SURGICAL INSTRUMENT

## PRIORITY

- [0001] This application claims priority to U.S. Provisional Application Serial No. 61/410,603, filed November 5, 2010, entitled “Energy-Based Surgical Instruments,” the disclosure of which is incorporated by reference herein.
- [0002] This application also claims priority to U.S. Provisional Application Serial No. 61/487,846, filed May 19, 2011, entitled “Energy-Based Surgical Instruments,” the disclosure of which is incorporated by reference herein.
- [0003] This application also claims priority to U.S. Nonprovisional Application Serial No. 13/276,660, filed October 19, 2011, entitled “USER FEEDBACK THROUGH HANDPIECE OF SURGICAL INSTRUMENT,” the disclosure of which is incorporated by reference herein.

## BACKGROUND

- [0004] In some settings, endoscopic surgical instruments may be preferred over traditional open surgical devices since a smaller incision may reduce the post-operative recovery time and complications. Consequently, some endoscopic surgical instruments may be suitable for placement of a distal end effector at a desired surgical site through a cannula of a trocar. These distal end effectors may engage tissue in a number of ways to achieve a diagnostic or therapeutic effect (e.g., endocutter, grasper, cutter, stapler, clip applier, access device, drug/gene therapy delivery device, and energy delivery device

using ultrasound, RF, laser, etc.). Endoscopic surgical instruments may include a shaft between the end effector and a handle portion, which is manipulated by the clinician. Such a shaft may enable insertion to a desired depth and rotation about the longitudinal axis of the shaft, thereby facilitating positioning of the end effector within the patient.

[0005] Examples of endoscopic surgical instruments include those disclosed in U.S. Pat. Pub. No. 2006/0079874, entitled "Tissue Pad Use with an Ultrasonic Surgical Instrument," published April 13, 2006, the disclosure of which is incorporated by reference herein; U.S. Pat. Pub. No. 2007/0191713, entitled "Ultrasonic Device for Cutting and Coagulating," published August 16, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. Pub. No. 2007/0282333, entitled "Ultrasonic Waveguide and Blade," published December 6, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. Pub. No. 2008/0200940, entitled "Ultrasonic Device for Cutting and Coagulating," published August 21, 2008, the disclosure of which is incorporated by reference herein; U.S. Pat. Pub. No. 2009/0209990 entitled "Motorized Surgical Cutting and Fastening Instrument Having Handle Based Power Source," published August 20, 2009, the disclosure of which is incorporated by reference herein; and U.S. Pat. Pub. No. 2010/0069940 entitled "Ultrasonic Device for Fingertip Control," published March 18, 2010, the disclosure of which is incorporated by reference herein; U.S. Pat. Pub. No. 2011/0015660, entitled "Rotating Transducer Mount for Ultrasonic Surgical Instruments," published January 20, 2011, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,500,176, entitled "Electrosurgical Systems and Techniques for Sealing Tissue," issued December 31, 2002, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,416,101 entitled "Motor-Driven Surgical Cutting and Fastening Instrument with Loading Force Feedback," issued August 26, 2008, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,738,971 entitled "Post-Sterilization Programming of Surgical Instruments," issued June 15, 2010, the disclosure of which is incorporated by reference herein; and U.S. Pat. Pub. No. 2011/0087218, entitled "Surgical Instrument Comprising First and Second Drive Systems Actuable by a Common Trigger Mechanism," published April 14, 2011, the disclosure of which is incorporated by reference herein. Additionally, such surgical tools may include a cordless transducer such as that disclosed in U.S. Pat. Pub. No.

2009/0143797, entitled “Cordless Hand-held Ultrasonic Cautery Cutting Device,” published June 4, 2009, the disclosure of which is incorporated by reference herein. In addition, the surgical instruments may be used, or adapted for use, in robotic-assisted surgery settings such as that disclosed in U.S. Pat. No. 6,783,524, entitled “Robotic Surgical Tool with Ultrasound Cauterizing and Cutting Instrument,” issued August 31, 2004.

[0006] While several systems and methods have been made and used for surgical instruments, it is believed that no one prior to the inventors has made or used the invention described in the appended claims.

#### BRIEF DESCRIPTION OF THE DRAWINGS

[0007] While the specification concludes with claims which particularly point out and distinctly claim this technology, it is believed this technology will be better understood from the following description of certain examples taken in conjunction with the accompanying drawings, in which like reference numerals identify the same elements and in which:

[0008] FIG. 1 depicts a schematic view of an exemplary medical device having an internal power source;

[0009] FIG. 2 depicts a perspective view of an exemplary medical device having an internal power source;

[0010] FIG. 3 depicts a side elevational view of an exemplary battery powered surgical instrument having a circuit board and a haptic indicator;

[0011] FIG. 4 depicts a side elevational view of an exemplary surgical instrument having a feedback pad;

[0012] FIG. 5 depicts a side elevational view of an exemplary surgical instrument including a display screen;

- [0013] FIG. 6 depicts a spring loaded gauge in communication with a trigger of the instrument of FIG. 5;
- [0014] FIG. 7 depicts a pressure sensor in communication with a trigger of the instrument of FIG. 5;
- [0015] FIG. 8 depicts a side elevational view of an exemplary surgical instrument including a display screen as a visual indicator and speaker holes as an auditory indicator;
- [0016] FIG. 9 depicts a plan view of a top surface of the exemplary surgical instrument of FIG. 8;
- [0017] FIG. 10 depicts a top plan view of an exemplary surgical instrument including a visual indicator screen;
- [0018] FIG. 11 depicts a cross-sectional view of the instrument of FIG. 10, showing a path for transmission of emitted light from lighting devices to the visual indicator screen;
- [0019] FIG. 12 depicts a cross-sectional view of the instrument of FIG. 10, showing an alternate path for transmission of emitted light from lighting devices to the visual indicator screen;
- [0020] FIG. 13 depicts a cross-sectional view of the instrument of FIG. 10, showing yet another path for transmission of emitted light from lighting devices to the visual indicator screen; and
- [0021] FIG. 14 depicts a cross-sectional view of an alternate version of the exemplary surgical instrument of FIG. 13, in which the flexible display is replaced with a projecting lens.
- [0022] The drawings are not intended to be limiting in any way, and it is contemplated that various embodiments of the technology may be carried out in a variety of other ways, including those not necessarily depicted in the drawings. The accompanying drawings incorporated in and forming a part of the specification illustrate several aspects of the present technology, and together with the description serve to explain the principles of

the technology; it being understood, however, that this technology is not limited to the precise arrangements shown.

#### DETAILED DESCRIPTION

[0023] The following description of certain examples of the technology should not be used to limit its scope. Other examples, features, aspects, embodiments, and advantages of the technology will become apparent to those skilled in the art from the following description, which is by way of illustration, one of the best modes contemplated for carrying out the technology. As will be realized, the technology described herein is capable of other different and obvious aspects, all without departing from the technology. Accordingly, the drawings and descriptions should be regarded as illustrative in nature and not restrictive.

[0024] I. Medical Devices for Use With Insertable or Reclaimable Components

[0025] FIG. 1 shows components of an exemplary medical device (10) in diagrammatic block form. As shown, medical device (10) comprises a control module (12), a power source (14), and an end effector (16). Merely exemplary power sources (14) may include NiMH batteries, Li-ion batteries (e.g., prismatic cell type lithium ion batteries, etc.), Ni-Cad batteries, or any other type of power source as may be apparent to one of ordinary skill in the art in light of the teachings herein. Control module (12) may comprise a microprocessor, an application specific integrated circuit (ASIC), memory, a printed circuit board (PCB), a storage device (such as a solid state drive or hard disk), firmware, software, or any other suitable control module components as will be apparent to one of ordinary skill in the art in light of the teachings herein. Control module (12) and power source (14) are coupled by an electrical connection (22), such as a cable and/or traces in a circuit board, etc., to transfer power from power source (14) to control module (12). Alternatively, power source (14) may be selectively coupled to control module (12). This allows power source (14) to be detached and removed from medical device (10), which may further allow power source (14) to be readily recharged or reclaimed for resterilization and reuse, such as in accordance with the various teachings herein. In addition or in the alternative, control module (12) may be removed for servicing, testing,

replacement, or any other purpose as will be apparent to one of ordinary skill in the art in view of the teachings herein.

**[0026]** End effector (16) is coupled to control module (12) by another electrical connection (22). End effector (16) is configured to perform a desired function of medical device (10). By way of example only, such function may include cauterizing tissue, ablating tissue, severing tissue, ultrasonically vibrating, stapling tissue, or any other desired task for medical device (10). End effector (16) may thus include an active feature such as an ultrasonic blade, a pair of clamping jaws, a sharp knife, a staple driving assembly, a monopolar RF electrode, a pair of bipolar RF electrodes, a thermal heating element, and/or various other components. End effector (16) may also be removable from medical device (10) for servicing, testing, replacement, or any other purpose as will be apparent to one of ordinary skill in the art in view of the teachings herein. In some versions, end effector (16) is modular such that medical device (10) may be used with different kinds of end effectors (e.g., as taught in U.S. Provisional Application Serial No. 61/410,603, etc.). Various other configurations of end effector (16) may be provided for a variety of different functions depending upon the purpose of medical device (10) as will be apparent to those of ordinary skill in the art in view of the teachings herein. Similarly, other types of components of a medical device (10) that may receive power from power source (14) will be apparent to those of ordinary skill in the art in view of the teachings herein.

**[0027]** Medical device (10) of the present example includes a trigger (18) and a sensor (20), though it should be understood that such components are merely optional. Trigger (18) is coupled to control module (12) and power source (14) by electrical connection (22). Trigger (18) may be configured to selectively provide power from power source (14) to end effector (16) (and/or to some other component of medical device (10)) to activate medical device (10) when performing a procedure. Sensor (20) is also coupled to control module (12) by an electrical connection (22) and may be configured to provide a variety of information to control module (12) during a procedure. By way of example only, such configurations may include sensing a temperature at end effector (16) or determining the oscillation rate of end effector (16). Data from sensor (20) may be



processed by control module (12) to effect the delivery of power to end effector (16) (e.g., in a feedback loop, etc.). Various other configurations of sensor (20) may be provided depending upon the purpose of medical device (10) as will be apparent to those of ordinary skill in the art in view of the teachings herein. Of course, as with other components described herein, medical device (10) may have more than one sensor (20), or sensor (20) may simply be omitted if desired.

[0028] FIG. 2 depicts a merely exemplary form that medical device (10) may take. In particular, FIG. 2 shows a medical device (100) comprising a power source (110), a control module (120), a housing (130), end effector (140), and an electrical connection (150). In the present example, power source (110) is located internally within housing (130) of medical device (100). Alternatively, power source (110) may only partially extend into housing (130) and may be selectively attachable to a portion of housing (130). In yet a further exemplary configuration, a portion of housing (130) may extend into power source (110) and power source (110) may be selectively attachable to the portion of housing (130). Power source (110) may also be configured to detach from medical device (100) and decouple from control module (120) or electrical connection (150). As a result, power source (110) may be completely separated from medical device (100) in some versions. As is readily apparent, this may allow the power source (110) to be removed to be recharged or reclaimed for resterilization and reuse, such as in accordance with various teachings herein. After recharging, or after an initial charge, power source (110) may be inserted or reinserted into medical device (100) and secured to housing (130) or internally within housing (130). Of course, medical device (100) may also allow power source (110) to be charged and/or recharged while power source (110) is still in or otherwise coupled relative to housing (130).

[0029] It should also be understood that control module (120) may be removed for servicing, testing, replacement, or any other purpose as will be apparent to one of ordinary skill in the art in view of the teachings herein. Further, end effector (140) may also be removable from medical device (100) for servicing, testing, replacement, or any other purpose as will be apparent to one of ordinary skill in the art in view of the teachings herein. In some versions, power source (110) is external to medical device

(100). For instance, power source (110) may be constructed in accordance with at least some of the teachings of U.S. Pat. Pub. No. 2011/0087212, entitled “Surgical Generator for Ultrasonic and Electrosurgical Devices,” published April 14, 2011, the disclosure of which is incorporated by reference herein.

[0030] While certain configurations of an exemplary medical device (100) have been described, various other ways in which medical device (100) may be configured will be apparent to those of ordinary skill in the art in view of the teachings herein. By way of example only, medical devices (10, 100) and/or any other medical device referred to herein may be constructed in accordance with at least some of the teachings of U.S. Pat. No. 5,322,055 entitled “Clamp Coagulator/Cutting System for Ultrasonic Surgical Instruments,” issued June 21, 1994, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 5,873,873 entitled “Ultrasonic Clamp Coagulator Apparatus Having Improved Clamp Mechanism,” issued February 23, 1999, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 5,980,510, entitled “Ultrasonic Clamp Coagulator Apparatus Having Improved Clamp Arm Pivot Mount,” filed October 10, 1997, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 6,325,811 entitled “Blades with Functional Balance Asymmetries for use with Ultrasonic Surgical Instruments,” issued December 4, 2001, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2006/0079874 entitled “Tissue Pad for Use with an Ultrasonic Surgical Instrument,” published April 13, 2006, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2007/0191713 entitled “Ultrasonic Device for Cutting and Coagulating,” published August 16, 2007, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2007/0282333 entitled “Ultrasonic Waveguide and Blade,” published December 6, 2007, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2008/0200940 entitled “Ultrasonic Device for Cutting and Coagulating,” published August 21, 2008, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2009/0143797, entitled “Cordless Hand-held Ultrasonic Cautery Cutting Device,” published June 4, 2009, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2010/0069940 entitled “Ultrasonic Device for Fingertip Control,” published March 18, 2010, the disclosure of which is incorporated by reference herein; U.S. Pub. No. 2011/0015660, entitled

“Rotating Transducer Mount for Ultrasonic Surgical Instruments,” published January 20, 2011, the disclosure of which is incorporated by reference herein; and/or U.S. Provisional Application Serial No. 61/410,603, filed November 5, 2010, entitled “Energy-Based Surgical Instruments,” the disclosure of which is incorporated by reference herein.

[0031] Of course, housing (130) and medical device (100) may include other configurations. For instance, housing (130) and/or medical device (100) may include a tissue cutting element and one or more elements that transmit bipolar RF energy to tissue (e.g., to coagulate or seal the tissue). An example of such a device is the ENSEAL® Tissue Sealing Device by Ethicon Endo-Surgery, Inc., of Cincinnati, Ohio. Further examples of such devices and related concepts are disclosed in U.S. Pat. No. 6,500,176 entitled “Electrosurgical Systems and Techniques for Sealing Tissue,” issued December 31, 2002, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,112,201, entitled “Electrosurgical Instrument and Method of Use,” issued September 26, 2006, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,125,409, entitled “Electrosurgical Working End for Controlled Energy Delivery,” issued October 24, 2006, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,169,146 entitled “Electrosurgical Probe and Method of Use,” issued January 30, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,186,253, entitled “Electrosurgical Jaw Structure for Controlled Energy Delivery,” issued March 6, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,189,233, entitled “Electrosurgical Instrument,” issued March 13, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,220,951, entitled “Surgical Sealing Surfaces and Methods of Use,” issued May 22, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,309,849, entitled “Polymer Compositions Exhibiting a PTC Property and Methods of Fabrication,” issued December 18, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,311,709, entitled “Electrosurgical Instrument and Method of Use,” issued December 25, 2007, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,354,440, entitled “Electrosurgical Instrument and Method of Use,” issued April 8, 2008, the disclosure of which is incorporated by reference herein; U.S. Pat. No. 7,381,209, entitled “Electrosurgical Instrument,” issued June 3, 2008, the disclosure of

which is incorporated by reference herein; U.S. Pub. No. 2011/0087218, entitled “Surgical Instrument Comprising First and Second Drive Systems Actuable by a Common Trigger Mechanism,” published April 14, 2011, the disclosure of which is incorporated by reference herein; and U.S. Pat. App. No. 13/151,181, entitled “Motor Driven Electrosurgical Device with Mechanical and Electrical Feedback,” filed June 2, 2011, the disclosure of which is incorporated by reference herein.

[0032] It is further understood that any one or more of the teachings, expressions, embodiments, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, embodiments, examples, etc. that are described herein. The following-described teachings, expressions, embodiments, examples, etc. should therefore not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

[0033] II. Exemplary Haptic or Visual Indicators on Ultrasonic Surgical Instrument

[0034] Examples described below relate to uses of haptic and/or visual information indicating devices with surgical instruments. It should be understood that the teachings below may be readily incorporated into any of the devices (10, 100) described above and/or any of the devices described in the various references cited herein. Throughout this disclosure, reference numbers utilized with different alphanumeric extensions indicate similar components in different versions of a described reference (i.e., waveguide (210) and waveguide (210F)).

[0035] A. Exemplary Haptic Indicators

[0036] FIG. 3 shows an exemplary surgical instrument (50A), similar to medical device (10, 100) described above, that additionally includes a haptic user feedback system (400). Haptic indicators are currently used in application for cell phones, gaming devices, and other similar applications known to those of ordinary skill in the art. Such devices with haptic indicators provide a tactile sensation to provide a user with feedback. For

example, such devices may cause a perceptible continuation or sporadic vibration to a user (to indicate, for example, an incoming call on a cell phone); other devices may provide another type of impulse in reaction to a triggering event or change in status of certain received data or information.

[0037] Instrument (50A) includes end effector (80A), multi-piece handle assembly (60A), and elongated transmission assembly (70A). Transmission assembly (70A) may be removably received in the direction of arrow (A) within a distal aperture (not shown) formed in a distal end of multi-piece handle assembly (60A). Instrument (50A) may additionally be a battery-powered device. Battery (402), haptic indicator (404), and circuit board (406) are housed in multi-piece handle assembly (60A).

[0038] Haptic indicator (404) may take the form of a vibration generator, for example, that may be constructed and operable in accordance with the teachings of U.S. Patent App. Publ. No. 2011/0152901, entitled "Implantable Port with Vibratory Feedback", published June 23, 2011, the disclosure of which is incorporated by reference herein. The vibration generator may comprise a reciprocating or oscillating weight that may be provided by a permanent magnet suspended by a resilient member. Vibration occurs as a selectively energized ring or coil causes the permanent magnet weight to reciprocate or oscillate. Other merely illustrative components and configurations of such a reciprocating weight type of a vibration generator are disclosed in U.S. Pat. No. 7,292,227, entitled "Electronic Device, Vibration Generator, Vibration-Type Reporting Method, and Report Control Method," issued Nov. 6, 2007, the disclosure of which is incorporated by reference herein. Additional exemplary components and configurations that a vibration generator may incorporate are disclosed in U.S. Pat. No. 6,982,696, entitled "Moving Magnet Actuator for Providing Haptic Feedback," issued Jan. 3, 2006, the disclosure of which is incorporated by reference herein; and U.S. Pat. No. 5,800,336, entitled "Advanced Designs of Floating Mass Transducers," issued Sep. 1, 1998, the disclosure of which is incorporated by reference herein. In some versions, the vibration generator may comprise a rotatable weight located eccentric to an axis of rotation and a rotatable by a motor. The rotation of the eccentric weight may cause a vibration. Merely illustrative components and configurations that such a rotating eccentric weight type of a

vibration generator may incorporate are also disclosed in U.S. Pat. No. 7,292,227. As another merely illustrative example, a rotating eccentric weight type of a vibration generator may be configured in accordance with the teachings of U.S. Pat. No. 5,107,155, entitled "Vibrator Motor for Wireless Silent Alerting Device," issued Apr. 21, 1992, the disclosure of which is incorporated by reference herein. By way of example only, the motor may rotate the weight at speeds up to approximately 10,000 rpm or at any other suitable speed.

[0039] As another merely illustrative example, a vibration generator may comprise a piezoelectric element. By way of example only, the vibration generator may be configured in accordance with the teachings of U.S. Pat. No. 5,277,694, entitled "Electromechanical Transducer for Implantable Hearing Aids," issued Jan. 11, 1994, the disclosure of which is incorporated by reference herein. As another example, the vibration generator may be configured in accordance with the teachings of U.S. Pat. No. 7,583,564, entitled "Piezoelectric Actuator and Electronic Equipment with Piezoelectric Actuator," issued Sep. 1, 2009, the disclosure of which is incorporated by reference herein. In some other versions, the vibration generator may comprise a piezoelectric element that is contained within a clamshell housing. When the piezoelectric element is excited (e.g., by a transcutaneously applied field, by a signal from a wire that is coupled with the piezoelectric element, etc.), the outward motion of the piezoelectric element pushes outwardly on each half of the surrounding clamshell housing. A vibratory mass may be coupled with one of the clamshell halves, while the other clamshell half may be "grounded" or secured directly to a medical device such as instrument (50A). Thus, if the piezoelectric element pushes upwardly a distance "x" and downwardly a distance "x," the displacement of the vibratory mass relative to the "ground" of instrument (50A) would be "2x."

[0040] As yet another merely illustrative example, the vibration generator may comprise a magnetostrictive material. For instance, a magnetostrictive material may be provided as a coil that is wrapped around an inner shaft. The inner shaft may contain the exciting element that acts on the magnetostrictive material. For instance, the inner shaft may be formed by an electromagnet that is selectively activated at a frequency selected to

provide a rapid expansion and contraction of the magnetorestrictive material. In particular, when the magnetostrictive material is selectively excited by the inner shaft, the magnetorestrictive material expands and contracts at a rapid rate, producing vibration as it hits upper and lower bounding diaphragms.

[0041] As another merely illustrative example, the vibration generator may comprise a lever arm that has a mass at one end and a piezoelectric element under the other end. The piezoelectric element and the fulcrum support of the lever arm may be "grounded" or secured directly to a medical device such as instrument (50A). Other forms of the vibration generator may include one or more solenoids, rotational motors, steppers, etc. In some versions, a vibratory actuator within a vibration generator acts as a corporeal vibration/motion energy harvester. For instance, such an energy harvesting actuator may act as an actuator "run in reverse" while it is not actively vibrating instrument (50A), to passively collect energy that can be stored in a battery or capacitor within instrument (50A) for later use when the vibration generator needs to be activated to vibrate. Various ways in which a vibratory actuator (or other component) within the vibration generator or elsewhere can be configured to act as such an energy harvester will be apparent to those of ordinary skill in the art in view of the teachings herein. It should therefore be understood that the vibration generator may be powered by an implanted power source, by an external coil, and/or by an implanted energy harvester, including combinations thereof. Similarly, and regardless of whether an energy harvester is included, other suitable variations, components, features, and configurations of a vibration generator will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0042] It should be understood that the choice of the mass of instrument (50A) and the choice of the mass of a moving member in a vibration generator may determine a resonant frequency of the vibration generator. For instance, such masses and resultant resonant frequencies may be selected in accordance with the teachings of Dietz, et al.; "Partially Implantable Vibrating Ossicular Prosthesis"; Transducers '97; International Conference on Solid State Sensors and Actuators; Chicago, Jun. 16-19, 1997; Vol. 1., pp. 433-436, the disclosure of which is incorporated by reference herein. Suitable resonant frequencies for the vibration generator, as well as methods/equations for determining a

resonant frequency of a vibration generator, will thus be apparent to those of ordinary skill in the art. In addition, it should be understood that the vibration generator may generate vibrations having any suitable amplitude and frequency. By way of example only, the vibration generated by a vibration generator may have an amplitude of approximately 100 micrometers within a frequency range of approximately 1 Hz and approximately 100 Hz. As another merely illustrative example, the vibration generated by a vibration generator may have an amplitude between approximately 100 micrometers and approximately 10 micrometers within a frequency range of approximately 5 Hz and approximately 100 Hz. As yet another merely illustrative example, the vibration generated by a vibration generator may have an amplitude between approximately 1000 micrometers and approximately 1 micrometer within a frequency range of approximately 10 Hz and approximately 800 Hz. Still other various suitable vibratory frequencies and amplitudes that may be generated by a vibration generator will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0043] Circuit board (406) may be a wireless communications board to transmit wireless information about instrument (50A) in a manner apparent to those of ordinary skill in the art in view of the teachings herein. Circuit board (406) may electrically communicate with end effector (80A) via one or more electrical connections and additionally communicates with haptic indicator (404) via one or more electrical connections such as wires (407). In the present example, haptic indicator (404) is attached to pistol grip portion (412) of multi-piece handle assembly (60A). Pistol grip portion (412) encompasses an area where a user's palm will directly contact instrument (50A), such that information may be indicated to the user's palm via haptic contact with pistol grip portion (412) and closely positioned haptic indicator (404). Haptic indicator (404) may be vibrate multi-piece handle assembly (60A) while mechanical and/or electrical energy is applied to instrument (50A). Some forms of information that may be communicated through haptic indicator (404) include, but are not limited to, confirmation of an activation of the end effector, a confirmation of reaching a set threshold amount of resistance measured in ohms applied across operated upon tissue that may additionally serve as a confirmation of the ending stage of severing and sealing tissue via instrument (50A) (or for a surgical instrument receiving RF energy, an indication of tissue state



sensed by electrodes positioned in a respective end effector energizing such tissue), confirmation of an attachment of a removable end effector (not shown) within reusable multi-piece handle assembly (60A), an indication of lower battery power within instrument (50A), or other fault indication with respect to instrument (50A), etc. Thus, the user may be informed of important events during the surgical procedure without looking at instrument (50A) to retrieve the information, which might otherwise require the user to look away from the surgical site being operated upon.

[0044] As shown in FIG. 4, exemplary surgical instrument (50B) may additionally include user feedback pad (408) on an exterior, proximal upper surface (410) for a user to activate and/or operate via the user's fingers, for example. In some such versions, user feedback pad (408) and haptic indicator (404) may form a single unit. FIG. 4 also shows transmission assembly (70B) permanently attached to multi-piece handle assembly (60B), though it should be understood that transmission assembly (70B) may be removable from handle assembly (60B) in some versions. During use of instrument (50B), a user interacts with user feedback pad (408) to obtain information and to input settings for instrument (50B). To ensure that a user has feedback indicating that instrument (50B) has accepted user entered new settings, for example, haptic indicator (404) may provide a tactile feedback such as a vibration. Haptic feedback may provide direct feedback for button pushes and may also provide an indication that instrument (50B) is active while providing an indication of an error codes when device (50B) encounters an error. Additionally or alternatively, feedback to a user indicating that instrument (50B) has accepted new user entered settings or other information may be provided in visual and/or auditory form.

[0045] Feedback systems utilized by haptic user feedback system (400) may be, for example, TouchSense® Tactile Feedback Systems and/or TouchSense® Force Feedback Systems provided by Immersion Corporation of San Jose, CA (where TouchSense® is a registered trademark of Immersion Corporation). Through use of such haptic technology, it may be possible to provide a haptic click upon completion of an insertion of transmission assembly (70A) into instrument (50A) and/or upon achieving a desirable rotation angle of end effector (80A) to signal to a user that instrument (50A) is properly

assembled. For example, a torque sensor may determine when an ultrasonic blade of end effector (80A) and transmission assembly (70A) is properly attached to multi-piece handle assembly (60A) and provide a tactile “click” to a user to indicate such attachment. Also, for surgical instruments requiring one or more electrical connections, a feedback tactile “click” may be sent to a user once a required electrical connection is made.

[0046] FIG. 5 shows another exemplary version of ultrasonic surgical instrument (50D), which is similar to medical device (10, 100) described above and includes a force sensor. The force sensor may comprise, for example, pressure sensor (426) of FIG. 6 or spring loaded gauge (414) of FIG. 7, both described further below. The force sensor assists with determining an amount of force a user is applying to trigger (68D) of surgical instrument (50D) in the direction arrow (B). Additionally, instrument (50D) includes a clamping end effector (e.g., like end effector (140) described above, etc.) that clamps upon application of a pressing force on trigger (68D), as described below. Further, instrument (50D) includes a visual and/or haptic indicator to indicate when a clamping force is being applied to tissue via the end effector’s response to an actuation of trigger (68D). Visual user feedback panel (416) on surgical instrument (50D) may give a user a graphical representation of such an applied force via utilization of bars or other graphical indications. Additionally or alternatively, a haptic indicator, similar to haptic indicator (404) of surgical instrument (50A), may increase a frequency or level of vibration that is supplied to multi-piece handle assembly (60D). In an alternative version, a circuit board, similar to circuit board (406) of surgical instrument (50A) described above, may communicate information to visual user feedback panel (416) and/or the haptic indicator to respectively allow feedback panel (416) and/or the haptic indicator to indicate to a user the amount of power being supplied to the tissue (such power may be supplied to instrument (50D) via an electrical source, such as cable (418) connected to a generator (not shown)).

[0047] In use, a force applied by a user on trigger (68D) that effects clamping on tissue via an end effector of instrument (50D) may have beneficial or detrimental effects on the welding of the clamped tissue. A visual supporting data set, such as via feedback panel (416) described above, may be beneficial to a user, particularly in addition to an optional

tonal feedback given to the user. A user may then understand what information instrument (50D) is conveying to the user within minimal disruption from the surgical procedure. Such visual representation of a user load upon instrument (50D) shown via feedback panel (416) compared to a depicted “ideal operation range” or threshold shown on feedback panel (416) via phantom lines (420) would assist a user with understanding what the status of the operated upon tissue might be. Feedback panel (416) may utilize an electrical liquid crystal display (“LCD”) type of display or even light-emitted diodes (“LEDs”) that light up in discrete steps areas of feedback panel (416). Types of LED displays described herein may also be used in combination with LCD types of displays as will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0048] FIG. 6 shows an example of how the clamping force of the end effector of instrument (50D) may be sensed. In particular, FIG. 6 shows pressure sensor (426) built into clamp mechanism (428) of multi-piece handle assembly (60D). Pressure sensor (426) may comprise an electronic pressure sensor, or pressure transducer, converting pressure into an analog electrical signal. Such pressure transducers may utilize force collectors such as a diaphragm to measure strain or deflection due to an applied force over a space. Force collector types may include but not be limited to a piezoresistive strain gauge, capacitive strain gauge, electromagnetic strain gauge, piezoelectric strain gauge, and/or optical strain gauge. Various suitable forms that such gauges may take will be apparent to those of ordinary skill in the art in view of the teachings herein. Similarly, various suitable ways in which such strain gauges may be incorporated into clamp mechanism (428) will be apparent to those of ordinary skill in the art in view of the teachings herein.

[0049] It should be understood that sensor (426) may take a variety of additional or alternative forms. For instance, sensor (426) may be operable to measure the acoustic impedance of instrument (50D) (e.g., by comparing current to voltage). In addition or in the alternative, sensor (426) may be operable to measure electrical impedance of tissue. Furthermore, sensor (426) may comprise a displacement measuring device giving feedback on a position of a clamp arm of the end effector (not shown) (e.g., indicating whether the clamp arm is in an open position, closed position, or somewhere between).

Sensor (426) may also comprise one or more thermal sensors disposed within the clamp arm of the end effector to register a clamp arm temperature and/or a tissue temperature. Sensor (426) may also comprise a pressure sensor disposed in the clamp arm of the end effector to measure the pressure applied to tissue by the clamp arm and an opposing blade of the end effector. Sensor (426) may additionally be a combination of two or more of the above-described sensors. For example, one or more sensors (426) may be operable to provide information regarding both clamp force as well as clamp arm position. Other suitable forms that sensor (426) may take will be apparent to those of ordinary skill in the art in view of the teachings herein.

**[0050]** Clamp mechanism (428) is coupled with the end effector (not shown) of instrument (50D) such that clamp mechanism (428), along with other components, converts pivotal movement of actuation trigger (68D) into clamping action at the end effector. In particular, clamp mechanism (428) is configured to receive a portion of actuation trigger (68D), which pivots about pin (430). As a user applies force to actuation trigger (68D) in the direction of arrow (D), actuation trigger (68D) rotates about pin (430) in the direction of arrow (E) to apply a force in the direction of arrow (F) against pressure sensor (426). Feedback from pressure sensor (426) may be sent to feedback panel (416) of surgical instrument (50D) to display the feedback information to a user via the LCD display of feedback panel (416). Feedback from pressure sensor (426) may additionally or alternatively be sent through surgical instrument (50D) as a haptic indication, as described above, and/or an audible indication, as described in greater detail below.

**[0051]** FIG. 7 shows another example of how the clamping force of the end effector of instrument (50D) may be sensed. A mechanical indication may occur via spring loaded gauge (414) shown in FIG. 7. Spring loaded gauge (414) of this example includes a gauge (421) positioned between a pair of opposing resilient members such as springs (423), which are connected at a fixed end to fixed point (417) in instrument (50D) and at another end to pin (419) of trigger (68D). Gauge (421) may have any of the configurations noted above for sensor (426) and/or any other suitable configuration. Spring loaded gauge (414) may measure a displacement caused by trigger (68D) and act

as a transducer to convert the mechanical displacement into an electrical signal in a manner as apparent to those of ordinary skill in the art in view the teachings herein. Spring loaded gauge (414) may be placed in series with actuation trigger (68D) of surgical instrument (50D) to measure an applied force, shown via solid line (422) in FIG. 7, and transmit the measurement, as shown via arrow (C), to a panel such as feedback panel (416A) for display. For example, a user may press actuation trigger (68D) in the direction of arrow (D) such that trigger (68D) rotates about pin (415). Actuation of trigger (68D) may thus cause an expansion of spring loaded gauge (414), from which a measured of applied force may be retrieved; and release of trigger (68D) may cause spring loaded gauge (414) to return to an original, compressed position. The applied force may then be measured and compared against a preset ideal force, which is indicated as phantom line (424). A “too little force” or a “too much force” condition may thus be indicated to a user. Gauge (414) may additionally or alternatively be a solenoid type gauge. With such a gauge, an increasing force causes an increasing displacement of a core of the solenoid that can be measured in the electrical inputs to the solenoid. Gauge (414) may additionally or alternatively comprise linear variable differential transformers (“LVDTs”). Additionally or alternatively, outputs of instrument (50D) such as blade amplitude and power may be augmented by the information received from feedback features, as described above, as well as other types of indicators such as visual, haptic, and/or auditory indicators.

**[0052]** FIGS. 8-9 show another version of exemplary ultrasonic surgical instrument (50E), which is similar to medical device (10, 100) described above. Surgical instrument (50E) includes hand activation buttons (431) and both auditory and visual feedback features. For example, as shown in FIG. 9, upper surface (432) of multi-piece handle assembly (60E) includes LED indicators (434, 436). LED indicator (434) may provide a visual display bar for indication of an amount of power left in surgical instrument (50E) by, for example, displaying an amount of power left in batteries power surgical instrument (50E). LED indicator (436) may provide a visual display bar for indication of measurements of impedance during use of instrument (50E). For instance, instrument (50E) of this example has an end effector (e.g., similar to end effector (140) described above) with jaws that include sensors. The sensors are used to measure the impedance of

tissue being clamped by the jaws. This measured impedance may be monitored to determine the degree to which the tissue is sealed by ultrasonic energy or RF energy, etc. In addition or in the alternative, the measured impedance may be used as a feedback input through a control algorithm to control the delivery of ultrasonic energy or RF energy to the tissue via the jaws. Various suitable ways in which tissue impedance may be measured are described in various references cited herein.

[0053] LED indicator (436) as an impedance indicator may change by, for example, lighting up more LED bars or changing a color display as tissue impedance increases. Such a change allows a user to understand that instrument (50E) is approaching a back side of a power curve, or rather, that impedance or resistance to applied voltage has increased, indicating that portions of the operated upon tissue has been sufficiently sealed. Different patterns, such as pattern (438) shown in FIG. 8, may reflect codes relaying a message to a user. For example, if an error occurred when using instrument (50E), a beep pattern from a generator could change from a pre-defined normal pattern reflected by a pattern and number of lit LED bars to a different illuminated non-normal pattern to indicate the error. The normal and non-normal patterns may be set forth in a user guide, for example, to allow a user to interpret the appropriate error message and whether an error is occurring.

[0054] With respect to auditory feedback mechanisms, surgical instrument (50E) includes speaker holes (440) on distal end (442) of upper surface (432) of multi-piece handle assembly (60E). A speaker (not shown) disposed below speaker holes (440) will emit sounds to provide audible feedback during activation of instrument (50E). For example, a pattern of audible “beeps” may change upon selection of a minimum or maximum amount of activation power. Or, a pattern or tone may change relative to a measured amount of impedance or power left in the batteries powering surgical instrument (50E), such as projecting a lower pitch or tone as the batteries lose power.

[0055] B. Exemplary Visual Indicators

[0056] FIGS. 10-13 show an exemplary ultrasonic surgical instrument (50F), similar to medical device (10, 100) described above, that additionally includes a visual indicator to

provide visual feedback. FIG. 10 shows proximal end portion (444) of surgical instrument (50F) with a phantom view of projecting trigger (68F). Surgical instrument (50F) includes information display location (446), which may include, for example, a LCD screen including LED lighting imaging to reflect such information from instrument (50F) as described above for other instrument versions.

[0057] FIG. 11 shows a cross-section of multi-piece handle assembly (60F) of surgical instrument (50F) including acoustic waveguide (210F). Clear lens (448) is positioned on upper surface (450) of an exterior proximal end portion (444) either as part of information display location (446) or separate from information display location (446). Clear lens (448) may comprise plastic or any other suitable material. Cartridge (452) housed in multi-piece handle assembly (60F) includes electronic module(s) to transmit information and/or batteries to power surgical instrument (50F). One or more projecting light sources (454), which may comprise LEDs, are mounted on an upper surface of cartridge (452). In use, projecting light sources (454) project light through instrument (50F) in the respective directions of arrows (G, H) around acoustic assembly shown by acoustic waveguide (210F) through to clear lens (448), which collects the projected light and transmits the light to enable a user to see the light. Cartridge (452) is removable from multi-piece handle assembly (60F) of surgical instrument (50F) and includes one or more electronics modules. The electronics module(s) of cartridge (452) may control the display functions. Thus, cartridge (452) controls visual feedback to a user as cartridge (452) causes at least one projecting light source (454) to project a light that is seen by the user. The at least one projecting light source (454) is positioned on cartridge (452) such that it is visible to a user through at least one clear plastic lens (448) during use of instrument (50F).

[0058] It should be understood that the positioning of cartridge (452) and the use of lens (448) may permit assembly (60F) to be sterilized using gamma sterilization and/or other techniques without harming cartridge (452). In addition or in the alternative, cartridge (452) may be removed to undergo some other form of reprocessing while assembly (60F) is sterilized using gamma sterilization and/or other techniques. In other words, all of the electronic components of instrument (50F) may be contained on cartridge (452), such that

the removability of cartridge (452) enables sterilization of assembly (60F) using techniques that might otherwise damage such electronic components.

**[0059]** It should also be understood that transparent bezels, light pipes, and light collectors may be used to assist with projecting light from light sources (454) through lens (448) on upper surface (450) of instrument (50F). For example, FIG. 12 shows an alternate version of exemplary ultrasonic surgical instrument (50G), similar to instrument (50F) described above. However, projecting light sources (454) on cartridge (452) project light in the directions of arrows (I, J) through light tunnels (456A, 456B), which may comprise light pipes or light fibers, for example.

**[0060]** FIG. 13 shows an exemplary ultrasonic surgical instrument (50H), similar to medical device (10, 100) described above, with an exemplary alternative feature to provide visual feedback. Surgical instrument (50H) includes clear bezel (458) positioned on an exterior of upper surface (450) of instrument (50H). Flexible display (460) is disposed within multi-piece handle assembly (60H) or on upper surface (450) below clear bezel (458). Flexible display (460) conforms to the shape of upper surface (450) to better display information such as a display light, text, graphics, etc. through clear bezel (458). While flexible display (460) is shown as disposed beneath clear protective bezel (458), flexible display (460) may alternatively be disposed on the surface of instrument (50H) with a fluid tight electrical connection disposed within multi-piece handle assembly (60H) of instrument (50H). Flexible display (460) is connected to cartridge (452) via a feed-through contact shown as connector (462), discussed below, embedded in the shroud housing of multi-piece handle assembly (60H). Flexible display (460) is operable to display information such as light from light source (470), described below, may be driven by electronic connections from cartridge (452). Flexible display (460) may be a LED, organic LED (“OLED”), electro-chromic, active-matrix OLED (“AMOLED”), or backlight LCD type of display. Information from cartridge (452) is displayed on flexible display (460) for a user to see and use. A touch screen version may be used to enable control of settings such as generator settings through the display.



[0061] Connector (462) is in communication with cartridge (452). For example, wires (464) connect connector (462) to electrical connection (466). Electrical connection (466) is mated to a mating electrical connection (468) disposed on top surface (469) of cartridge (452) and electronically communicates with cartridge (452). While electrical connection (466) is shown to be a female connection mated to male mating electrical connection (468), the reverse mating orientation is possible. Light source (470) is disposed on top surface (469) of cartridge (452). Light source (470) may be a light for a back lit LCD or electro-chromic display.

[0062] FIG. 14 shows exemplary surgical instrument (50I), similar to instrument (50H) described above but showing an alternative version. For example, surgical instrument (50I) includes display surface or display screen (472) with projector lens (474) disposed below display screen (472). Projector lens (474) projects information, such as light, for example, onto display screen (472) in the direction of arrows (K). Thus, flexible display (460) is replaced by display screen (472), which provides a surface for projector lens (474) to project information to a user. Projector lens (474) is attached to cartridge (452) by a data cable (not shown) to allow projector lens (474) to project information to a user about instrument (50I).

[0063] III. Miscellaneous

[0064] It should be understood that any one or more of the teachings, expressions, embodiments, examples, etc. described herein may be combined with any one or more of the other teachings, expressions, embodiments, examples, etc. that are described herein. The following-described teachings, expressions, embodiments, examples, etc. should therefore not be viewed in isolation relative to each other. Various suitable ways in which the teachings herein may be combined will be readily apparent to those of ordinary skill in the art in view of the teachings herein. Such modifications and variations are intended to be included within the scope of the claims.

[0065] Versions of the devices described above may have application in conventional medical treatments and procedures conducted by a medical professional, as well as application in robotic-assisted medical treatments and procedures. For instance, those of

ordinary skill in the art will recognize that various teaching herein may be readily combined with various teachings of U.S. Pat. No. 6,783,524, entitled "Robotic Surgical Tool with Ultrasound Cauterizing and Cutting Instrument," published August 31, 2004, the disclosure of which is incorporated by reference herein.

[0066] Versions of described above may be designed to be disposed of after a single use, or they can be designed to be used multiple times. Versions may, in either or both cases, be reconditioned for reuse after at least one use. Reconditioning may include any combination of the steps of disassembly of the device, followed by cleaning or replacement of particular pieces, and subsequent reassembly. In particular, some versions of the device may be disassembled, and any number of the particular pieces or parts of the device may be selectively replaced or removed in any combination. Upon cleaning and/or replacement of particular parts, some versions of the device may be reassembled for subsequent use either at a reconditioning facility, or by a user immediately prior to a procedure. Those skilled in the art will appreciate that reconditioning of a device may utilize a variety of techniques for disassembly, cleaning/replacement, and reassembly. Use of such techniques, and the resulting reconditioned device, are all within the scope of the present application.

[0067] By way of example only, versions described herein may be sterilized before and/or after a procedure. In one sterilization technique, the device is placed in a closed and sealed container, such as a plastic or TYVEK bag. The container and device may then be placed in a field of radiation that can penetrate the container, such as gamma radiation, x-rays, or high-energy electrons. The radiation may kill bacteria on the device and in the container. The sterilized device may then be stored in the sterile container for later use. A device may also be sterilized using any other technique known in the art, including but not limited to beta or gamma radiation, ethylene oxide, or steam.

[0068] Having shown and described various versions in the present disclosure, further adaptations of the methods and systems described herein may be accomplished by appropriate modifications by one of ordinary skill in the art without departing from the scope of the present invention. Several of such potential modifications have been

mentioned, and others will be apparent to those skilled in the art. For instance, the examples, versions, geometrics, materials, dimensions, ratios, steps, and the like discussed above are illustrative and are not required. Accordingly, the scope of the present invention should be considered in terms of the following claims and is understood not to be limited to the details of structure and operation shown and described in the specification and drawings.

I/We claim:

1. A surgical instrument comprising:
  - (a) a handpiece, wherein the handpiece comprises a user feedback feature;
  - (b) a shaft assembly extending distally from the handpiece; and
  - (c) an end effector disposed at a distal end of the shaft assembly, wherein the end effector is operable to delivery energy from the shaft assembly to a surgical site;wherein the user feedback feature is operable to provide feedback to the user, indicating information relating to operation of the end effector.
2. The surgical instrument of claim 1, wherein the user feedback feature is operable to provide at least one of a visual, an auditory, or a haptic feedback and is operable to provide information relating to at least one of amplitude of a blade of the end effector or a power level associated with the surgical instrument.
3. The surgical instrument of claim 1, wherein the handpiece further comprises a user input feature, wherein the end effector includes an active feature responsive to actuation of the user input feature, and wherein the active feature is operable to operate on tissue in response to actuation of the user input feature.
4. The surgical instrument of claim 3, wherein the user feedback feature is operable to provide haptic feedback to a user.
5. The surgical instrument of claim 4, wherein the user feedback feature comprises a haptic motor configured to vibrate in response to a signal of a change in a status of the surgical instrument.
6. The surgical instrument of claim 4, wherein the user input feature comprises a feedback pad configured to receive one or more user inputted setting commands, and wherein the feedback pad and the user feedback feature form one of a single

unit or separate units.

7. The surgical instrument of claim 3, wherein the user feedback feature comprises a visual indicator operable to provide visual feedback to a user.
8. The surgical instrument of claim 7, wherein the visual indicator is configured to display information upon a screen disposed on the surgical instrument in response to a signal of a change in a status of the surgical instrument.
9. The surgical instrument of claim 8, wherein the user input feature comprises a trigger, wherein the change in status is associated with a force applied to the trigger.
10. The surgical instrument of claim 8, further comprising a force sensor, wherein the user input feature comprises a trigger, wherein the force sensor is operable to measure force applied through the trigger.
11. The surgical instrument of claim 10, wherein the force sensor comprises a spring loaded gauge in communication with the trigger.
12. The surgical instrument of claim 10, wherein the force sensor is selected from the group consisting of a pressure sensor in communication with the trigger, a pressure sensor in communication with the end effector, an acoustic impedance sensor, a tissue impedance sensor, and a displacement measuring device.
13. The surgical instrument of claim 8, wherein the displayed information comprises at least one of a pattern display or a bar display.
14. The surgical instrument of claim 8, further comprising a removable cartridge disposed in the handpiece, wherein the screen comprises clear plastic and is disposed on a proximal, upper surface of the handpiece, wherein the user

feedback feature comprises one or more lighting devices in communication with the cartridge, wherein the lighting devices are operable to emit light through the clear plastic screen.

15. The surgical instrument of claim 8, wherein the user feedback feature further comprises a flexible display, wherein the cartridge is in electrical communication with the flexible display, wherein the flexible display is disposed below the clear plastic lens.
16. A surgical instrument comprising:
  - (a) a handpiece, wherein the handpiece comprises:
    - i. a user input feature,
    - ii. a user feedback feature;
  - (b) a shaft assembly extending distally from the handpiece; and
  - (c) an end effector disposed at a distal end of the shaft assembly, wherein the end effector includes an active feature responsive to actuation of the user input feature, wherein the active feature is operable to operate on tissue in response to actuation of the user input feature;wherein the user feedback feature is operable to provide haptic feedback to the user, indicating information relating to operation of the end effector.
17. The instrument of claim 16, wherein the user feedback feature is configured to vibrate in response to a level of impedance sensed in tissue engaged by the end effector.
18. The instrument of claim 16, wherein the user feedback feature is further operable to provide an auditory feedback to the user, indicating information relating to operation of the end effector.
19. The instrument of claim 16, wherein the handpiece comprises a pistol grip, wherein at least part of the user feedback feature is positioned within the pistol

grip to transmit haptic feedback to a user through the pistol grip.

20. A surgical instrument comprising:

- (a) a handpiece, wherein the handpiece comprises:
  - i. a user input feature,
  - ii. a user feedback feature;
- (b) a shaft assembly extending distally from the handpiece; and
- (c) an end effector disposed at a distal end of the shaft assembly, wherein the end effector includes an active feature responsive to actuation of the user input feature, wherein the active feature is operable to operate on tissue in response to actuation of the user input feature;

wherein the user feedback feature is operable to provide visual feedback to the user, indicating information relating to operation of the end effector and displaying the information on a display screen on the surgical instrument.

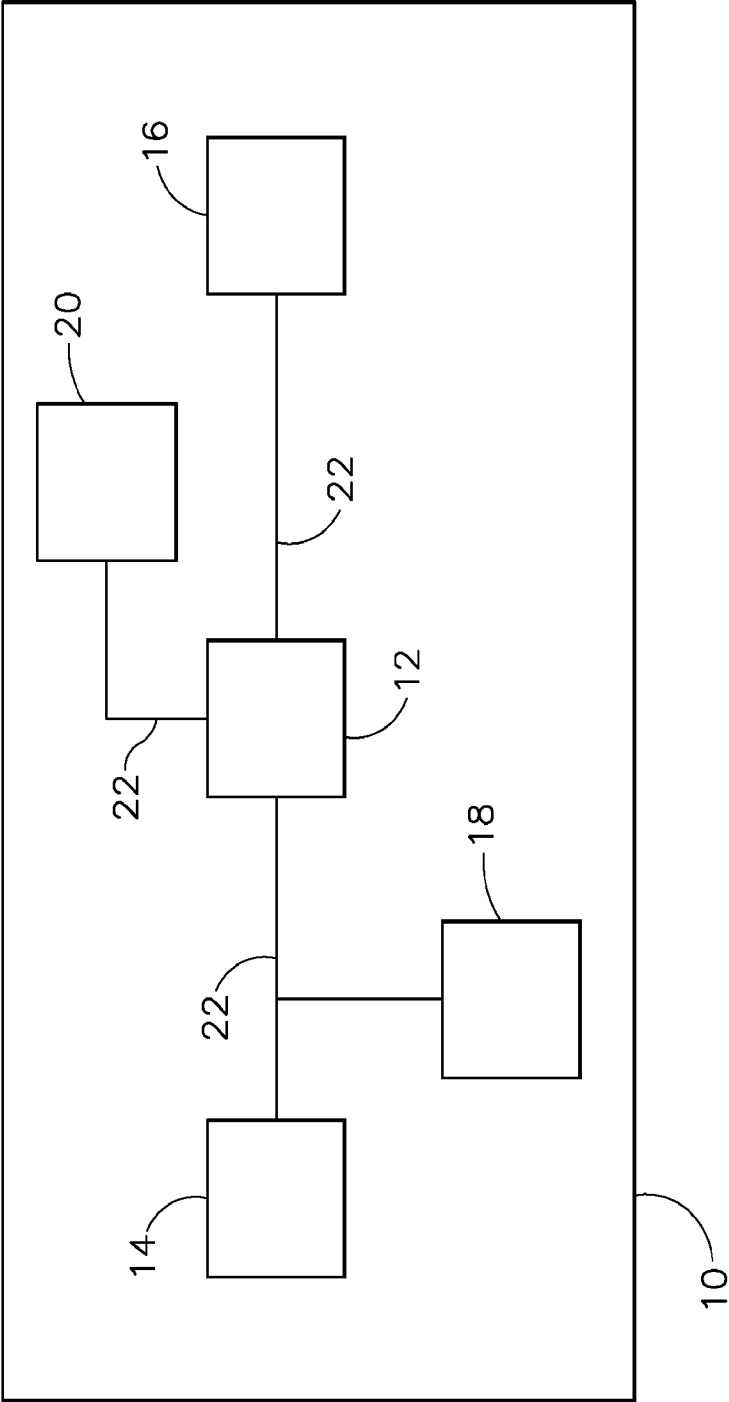


Fig. 1



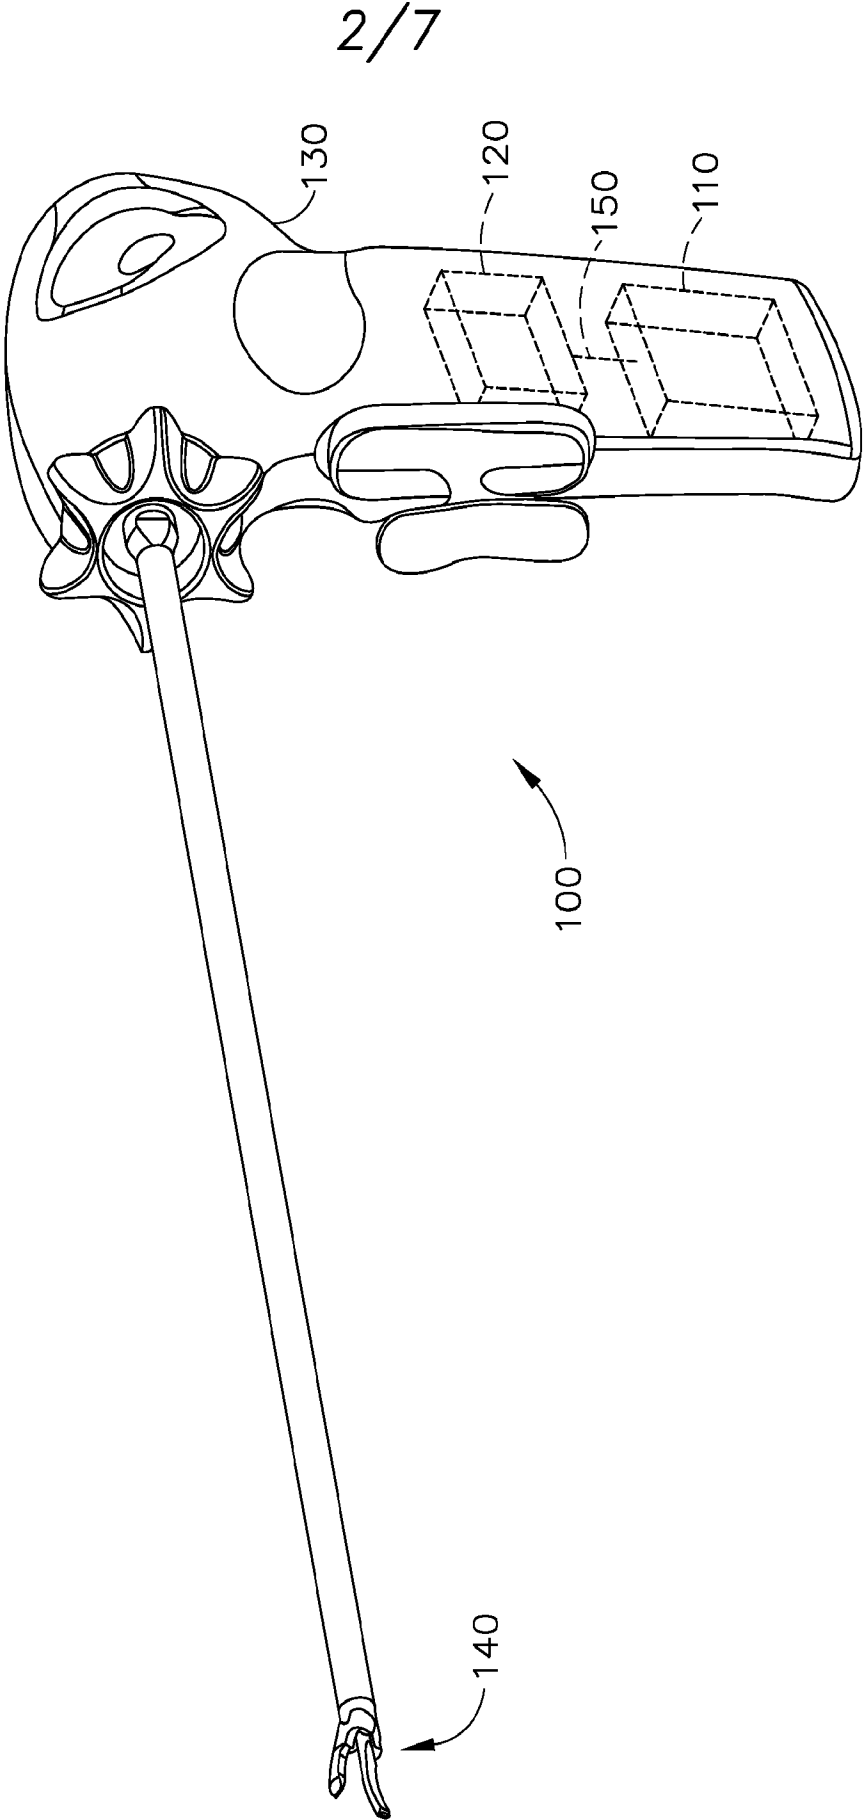


Fig.2

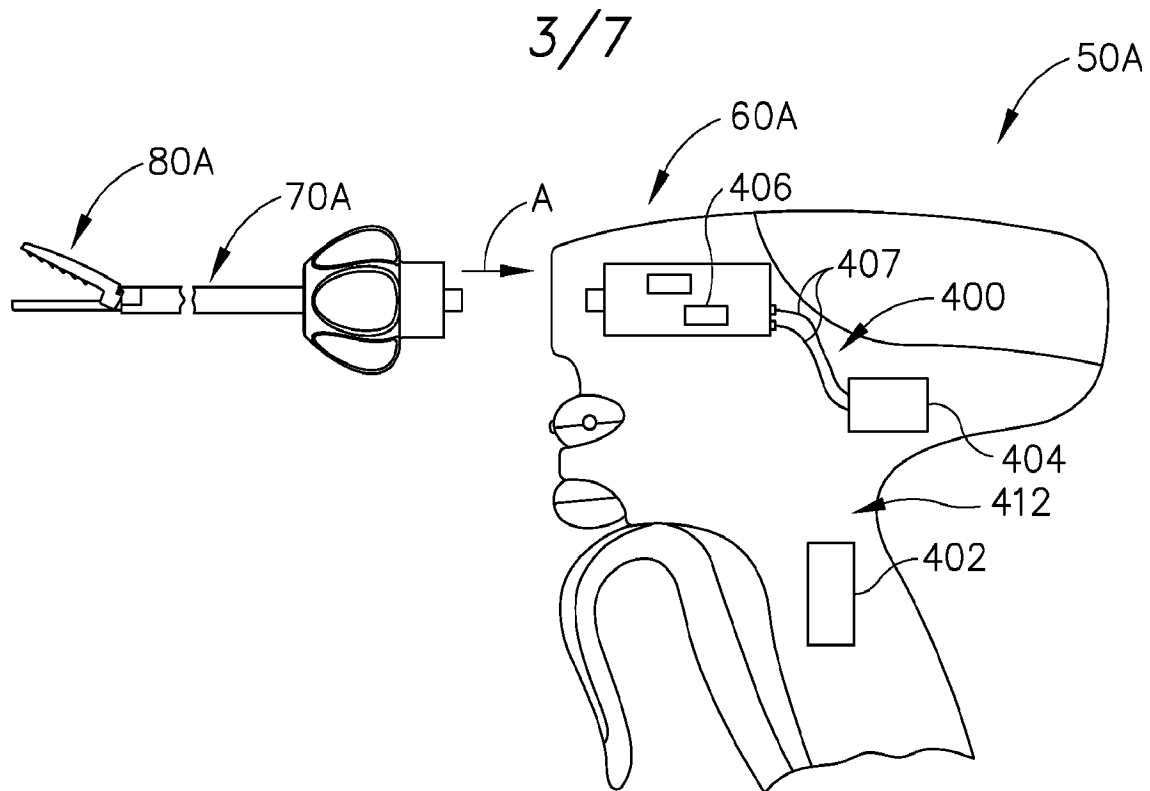


Fig.3

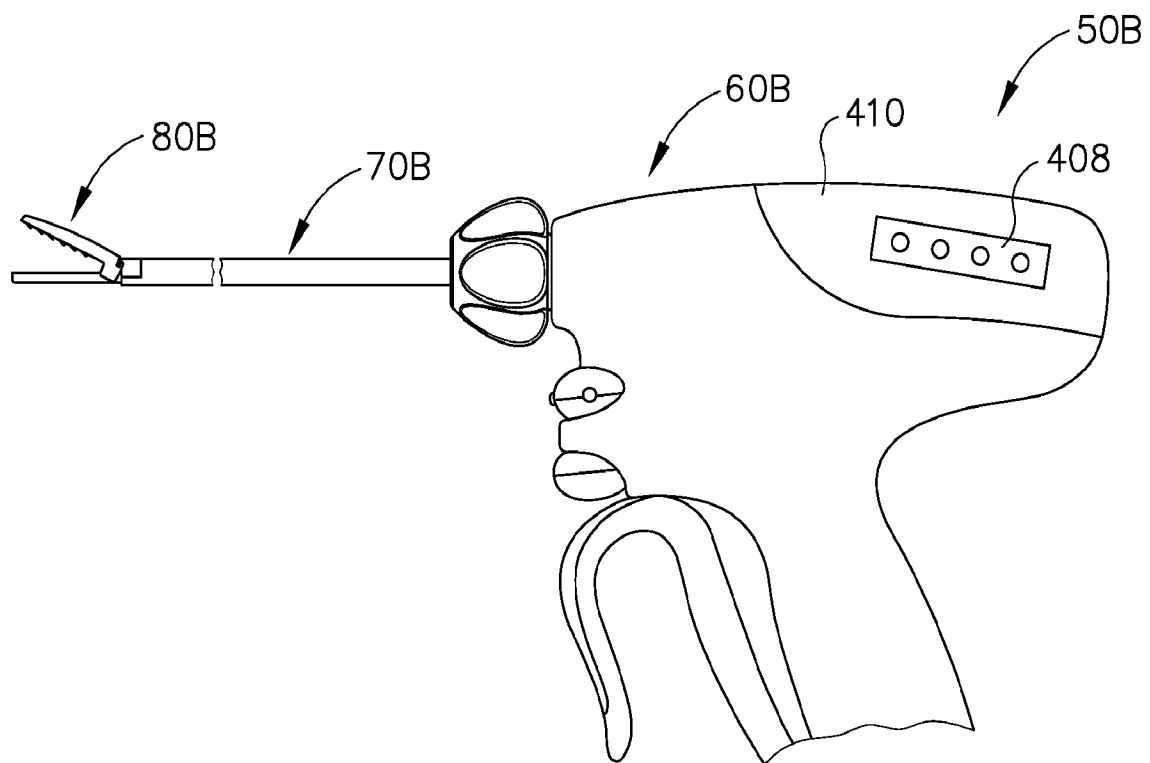


Fig.4

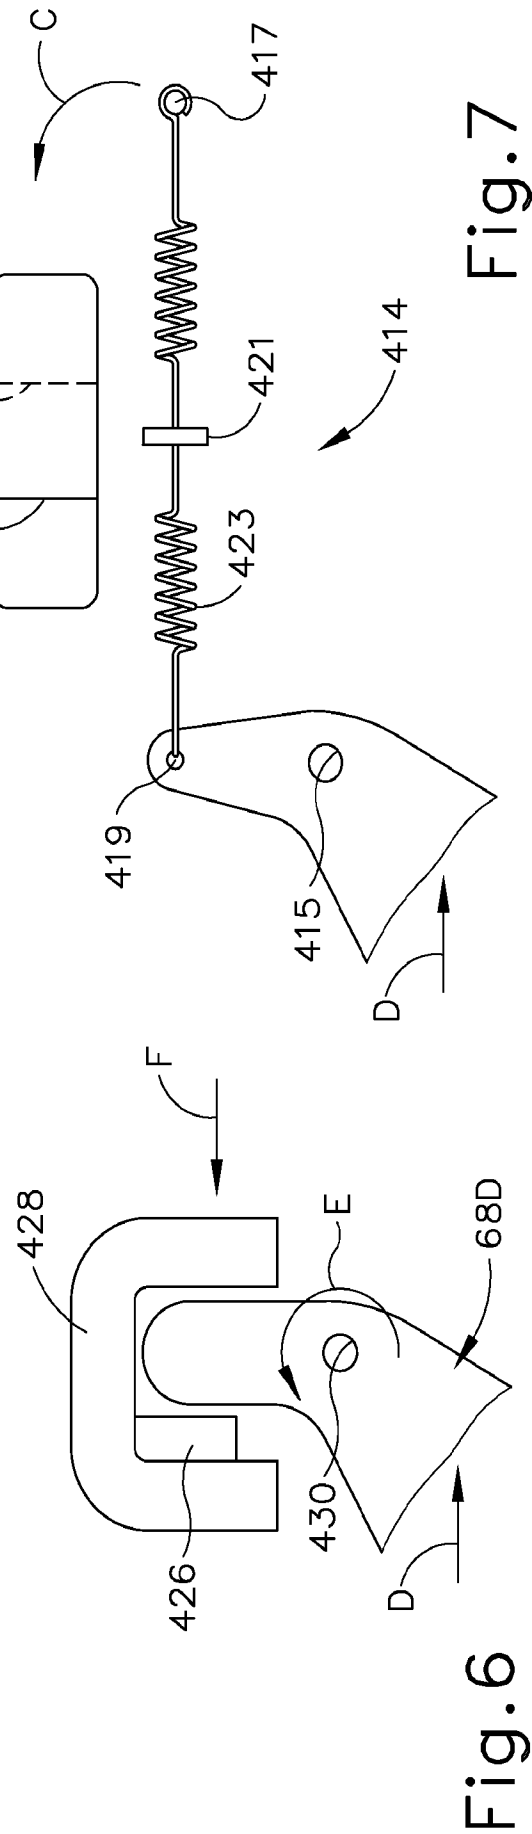
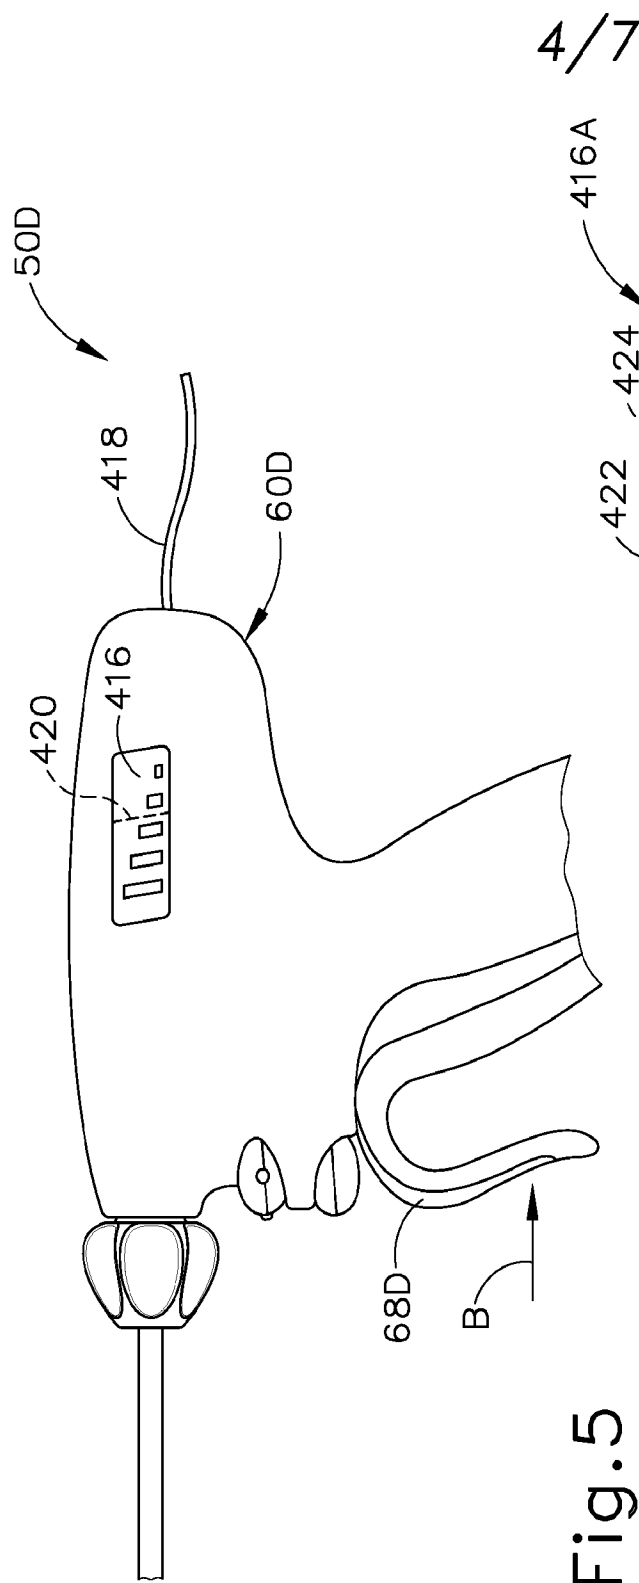


Fig. 7

5/7

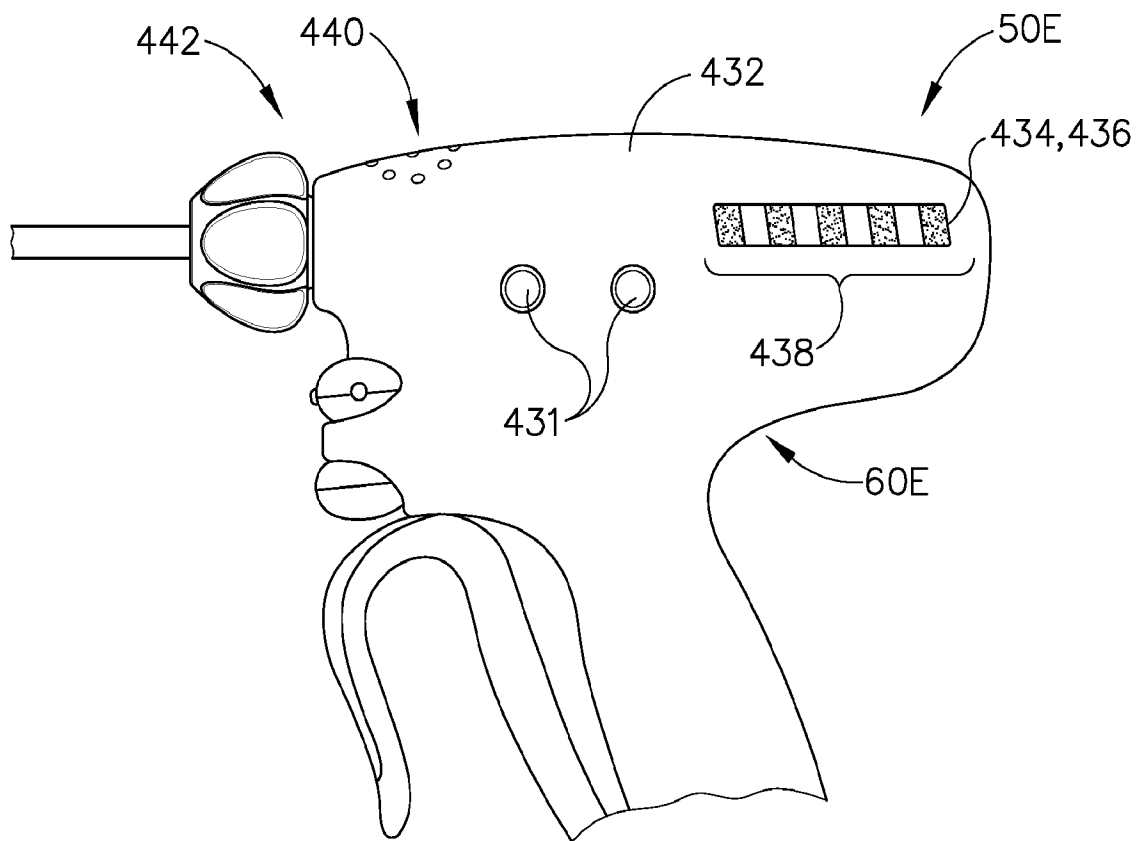


Fig.8

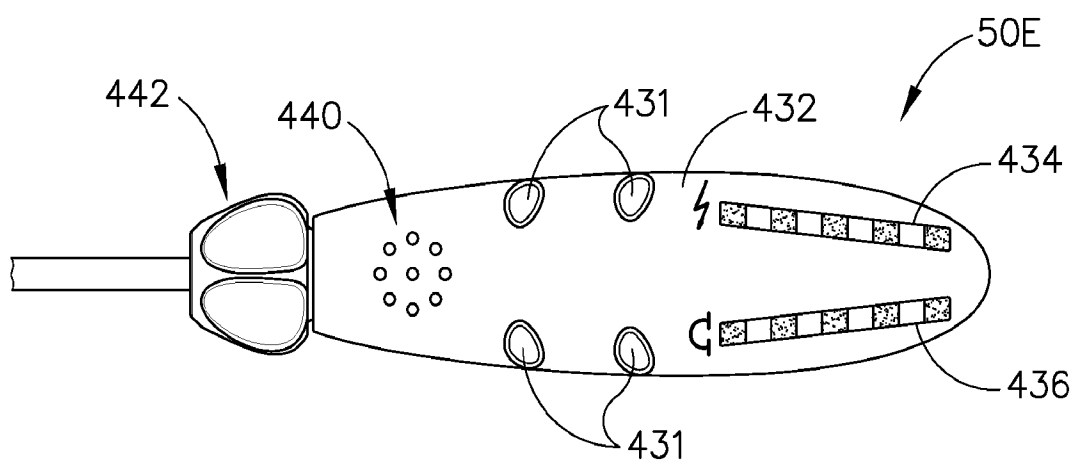


Fig.9

6/7

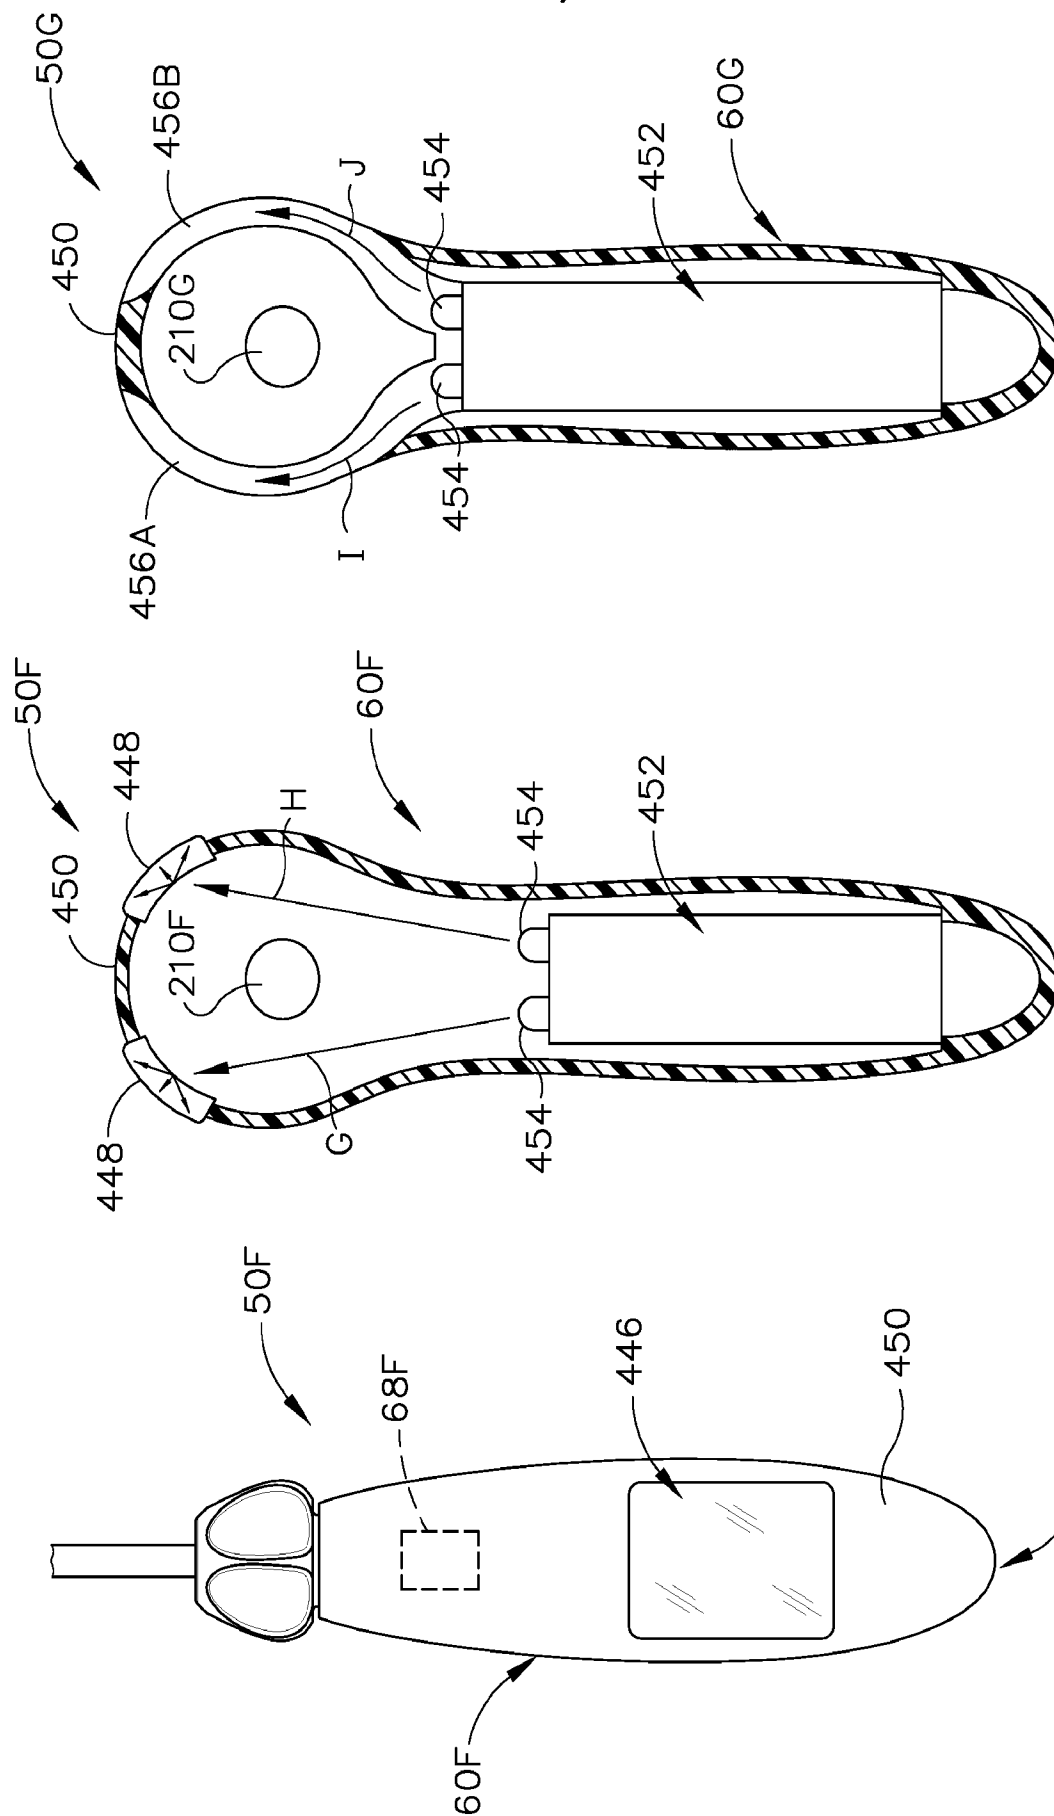


Fig.12

Fig.11

Fig.10

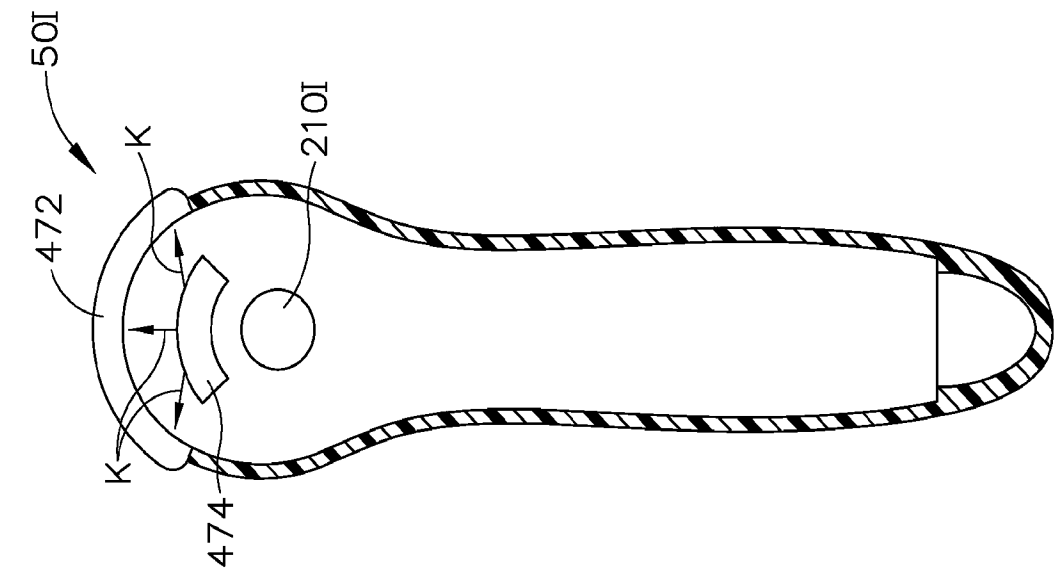


Fig. 13

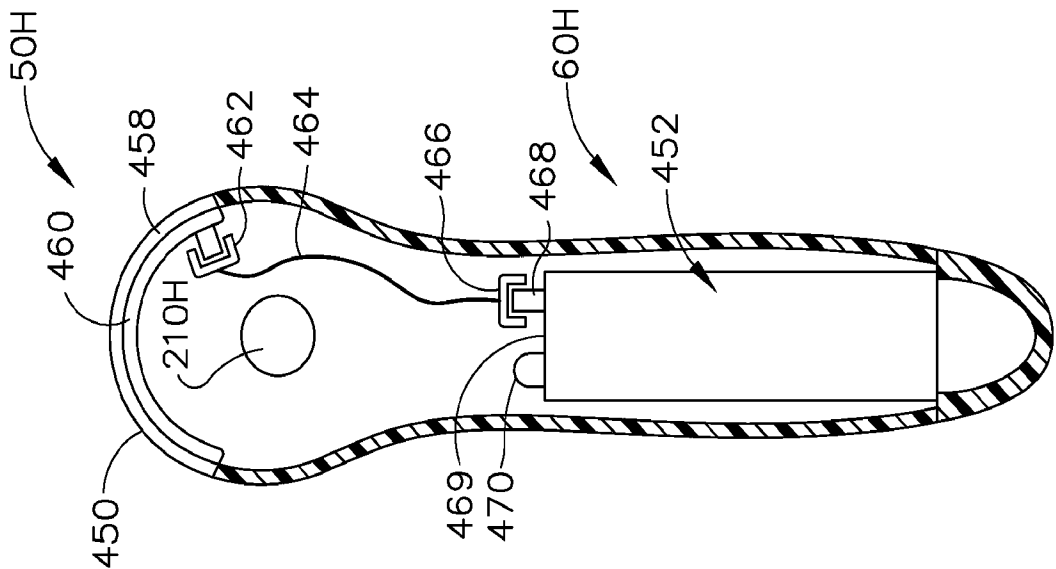


Fig. 14