



(51) International Patent Classification:

A61F 5/00 (2006.01) A41H 1/02 (2006.01)
A41D 19/015 (2006.01) F41H 5/04 (2006.01)

(21) International Application Number:

PCT/US2012/037305

(22) International Filing Date:

10 May 2012 (10.05.2012)

(25) Filing Language:

English

(26) Publication Language:

English

(30) Priority Data:

13/105,715 11 May 2011 (11.05.2011) US
13/178,392 7 July 2011 (07.07.2011) US

(71) Applicant (for all designated States except US): **ALLERGAN, INC.** [US/US]; 2525 Dupont Drive, Irvine, California 92612 (US).

(72) Inventors; and

(75) Inventors/Applicants (for US only): **CHITRE, Kaustubh S.** [IN/US]; 235 Pacific Oaks Road #210, Goletta, California 93117 (US). **HONARYAR, Babak** [US/US]; 14 Beaconsfield Court, Orinda, California 94563 (US). **TEZEL, Ahmet** [US/US]; 3946 Stacy Lane, Santa Barbara, California 93110 (US). **MANESIS, Nicholas J.** [US/US]; 2280 Varley Street, Summerland, California 93067 (US).

(74) Agents: **DONOVAN, Stephen** et al.; Allergan, INC., 2525 Dupont Drive, Irvine, CA 92612 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).


Declarations under Rule 4.17:

- as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii))
- as to the applicant's entitlement to claim the priority of the earlier application (Rule 4.17(iii))

Published:

- with international search report (Art. 21(3))

(54) Title: NEEDLE GUARD TO PROTECT ACCESS PORT TUBING

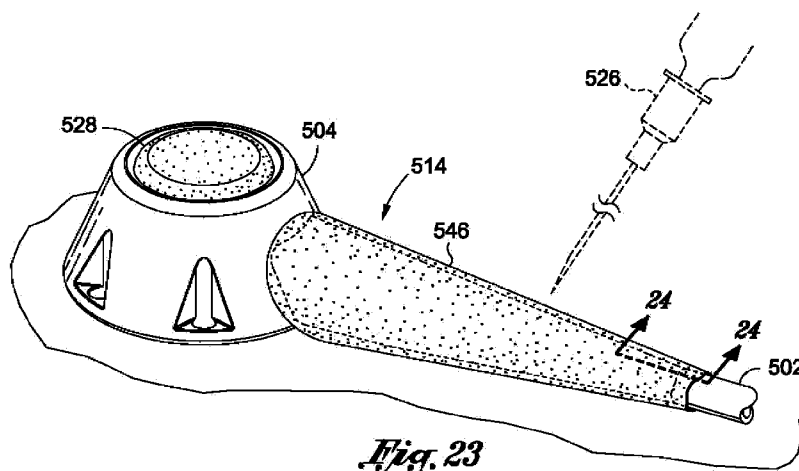

(57) Abstract: A device for the treatment of the obesity (406) comprising an access part (404) a tube (402) and a needle guard assembly, suitable to protect the tube leading from the implantable access port. The needle guard assembly may include a first composite guard and a second composite guard, each composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members are positioned. The needle guard assembly may comprise a sleeve extending over an end of the tube.



NEEDLE GUARD TO PROTECT ACCESS PORT TUBING

BY

KAUSTUBH S. CHITRE, BABAK HONARYAR, AHMET TEZEL, AND NICHOLAS J. MANESIS

RELATED APPLICATIONS

[0001] This application is a continuation-in-part of U.S. Patent Application No. 13/105,715, entitled "INFLATABLE PROSTHESES AND METHODS OF MAKING SAME," filed on May 11, 2011, which is a continuation-in-part of U.S. Patent Application No. 13/021,523, entitled "INFLATABLE PROSTHESIS AND METHODS OF MAKING SAME," filed on February 4, 2011, which claims the benefit and priority of U.S. Provisional Patent Application No. 61/301,910, filed on February 5, 2010, and the benefit and priority of U.S. Provisional Patent Application No. 61/409,440, filed on November 2, 2010, the entire disclosure of each of these applications are hereby incorporated by reference herein.

FIELD

[0002] The present invention generally relates to medical implants and more specifically relates to inflatable prostheses, such as tissue expanders, suitable for implantation in a mammal, and also relates to tube protectors for use with implantable access ports.

BACKGROUND

[0003] Prostheses or implants for reconstruction and/or augmentation of the human body are well known.

[0004] Fluid filled prostheses, for example, mammary prostheses or breast implants, are widely used to replace excised tissue, for example after a radical mastectomy, or to augment the body to improve surface configurations. Although there are many applications where these are used, the most common is the mammary prosthesis, used to augment or otherwise change the size or shape of the female breast.

[0005] A conventional saline-filled breast implant includes an outer shell of several layers of silicone elastomer having a valve or fill port. The prosthesis is typically implanted into the breast cavity in an empty or only partially filled state. The implant is then inflated to its final size by means of the valve or the fill port. This helps reduce the size of the needed incision, and enables a surgeon to adjust and even micro-adjust the volume of the implant. Unfortunately, the valve or the fill port is sometimes noticeable to the touch.

[0006] Many or even most implants are manufactured to a given size and shape, and are implanted without means or expectation of changing their size after implantation or initial filling when first inserted into the breast. However, in many situations it is desirable to be able to adjust the size of the implant over a substantial period of time. If the volume can later be adjusted, an implant of lesser initial volume can be implanted, and as the post-surgical swelling goes down, the implant used as a prosthesis can be enlarged. Also, because often the procedure is for cosmetic purposes, it is useful to be able to make a later adjustment of size without having to replace the prosthesis with one of a different size, which would require a subsequent surgical procedure.

[0007] One problem with many conventional adjustable implants is that they require a valve to be part of the implant.

[0008] It would be advantageous to provide an adjustable volume implant which does not require a valve or other access port for receiving fluid for adjustment.

[0009] Prior to implantation of a more permanent prosthesis, it is common practice to utilize a more temporary implant, for example, what is known as a "tissue expander" in order to gradually create the space necessary for the more permanent prosthesis. Keeping living tissues under tension by means of a tissue expander causes new cells to form and the amount of

tissue to increase. Conventionally, a tissue expander comprises an inflatable body, having an inflation valve connected thereto. The valve may be formed into the inflatable body itself or may be remotely located and connected to the inflatable body by means of an elongated conduit.

[0010] The inflatable body of the tissue expander is placed subcutaneously in the patient, at the location of where tissue is to be expanded. The inflation valve, whether on the implant or remote thereto, is also subcutaneously positioned or implanted, and is configured to allow gradual introduction of fluid, typically saline, into the inflation body, by injection with a syringe. After gradual inflation at pre-determined intervals, the skin and subcutaneous tissues overlying the expander are consequently caused to expand in response to the pressure exerted upon such tissues by the inflatable body as solution is gradually introduced therein.

[0011] After gradual inflation at pre-determined intervals, which may extend over weeks or months, the skin and subcutaneous tissue will expand to the point where further medical procedures can be performed, such as the permanent implantation of a prosthesis, plastic and reconstructive surgery, or for use of the skin and subcutaneous tissue for use in some other part of the body.

[0012] During a mastectomy, a surgeon often removes skin as well as breast tissue, leaving the remaining chest tissues flat and tight. To create a breast-shaped space for a reconstructive implant, a tissue expander is sometimes used as described above.

[0013] In any event, it should be appreciated that locating the fill valve on a prosthesis such as a tissue expander or adjustable implant requires considerable practitioner skill. Attempts to make products which facilitate this include the development of various products having structure, for example,

embedded magnets or a raised ring, for assisting physicians in locating the valve.

[0014] It has also proven difficult to develop a flexible protective material that is effective as a puncture resistant material while also being safe for implantation in the body. A puncture resistant material used as a component of a breast implant or tissue expander would ideally be sufficiently flexible such that the implant could still be folded or rolled and inserted through a small incision while also providing resistance to needle punctures aimed at inflating the implant/expander to its final size.

[0015] Bark et al., U.S. Patent No. 5,066,303, discloses a self-sealing tissue expander with a shell having a flowable sealing material. According to Bark et al., fluid infusion into the shell can be done directly through the shell, without the need for a fluid entry port.

[0016] Schuessler, U.S. Patent Application No. 12/543,795, filed on August 19, 2009, the entire disclosure of which is incorporated herein by this specific reference, discloses a fluid filled implant including a self-sealing shell.

[0017] It has also proven difficult to develop a flexible protective material that is effective to protect the tubing leading from an implantable access port. Such an access port may be used as part of an implantable gastric banding system, for example, a system using the LAP-BAND® (Allergan, Inc., Irvine, CA) gastric band or the LAP-BAND AP® (Allergan, Inc., Irvine, CA) gastric band.

[0018] There is a need for improved temporary tissue expanders, more permanent adjustable implants, and other inflatable prostheses. In addition, there is a need for a flexible protective material that is effective to protect the tubing

leading from an implantable access port. The present invention addresses these needs.

SUMMARY

[0019] The invention relates, in part, to expandable prostheses, for example, implants and tissue expanders, and in particular to implantable temporary tissue expanders as well as more permanent mammary prostheses. The invention additionally relates to protective materials that may be used to protect access port tubing from puncture.

[0020] Accordingly, the present invention provides, in part, implants, for example, but not limited to tissue expanders and more permanent prostheses, for example, those implantable in a breast, and methods of making the same. The present invention provides inflatable prosthetic implants, components thereof and methods of making the same. In one embodiment of the invention, inflatable prosthetic implants are provided which include, as a component of such implants, flexible, puncture resistant materials.

[0021] In another embodiment of the invention, inflatable implants or prostheses, for example, tissue expanders and adjustable implants are provided which generally comprise a puncturable, self-sealing anterior portion, or shell, a puncture resistant posterior portion substantially opposing the anterior portion, and a fillable cavity defined between the anterior portion and the posterior portion.

[0022] It is to be appreciated that the terms "implant" "prosthesis" and "tissue expander" as used herein are intended to encompass permanent implants, including adjustable implants, as well as relatively temporary tissue expanders, and components, for example, shells, of such implantable devices.

[0023] In one embodiment of the invention, a method of making an inflatable device or prosthesis, suitable for implantation in a

mammal, is provided wherein the method generally comprises the steps of providing a plurality of mesh segments, positioning the plurality of segments on a curved molding surface, applying a fluid elastomeric material to the molding surface with the segments positioned thereon, and allowing the elastomeric material to set to form a flexible shell having an open end, the shell including the fabric segments embedded within the set elastomer, and the shell being useful as a component of an inflatable prosthesis. The step of positioning may include substantially entirely covering the molding surface with the mesh segments, for example, in a manner such that the mesh segments overlap one another. The method further comprises the step of sealing the open end of the elastomeric shell, for example, by providing a puncture resistant member and sealing the puncture resistant member to the open end of the elastomeric shell.

[0024] In one embodiment, the mesh segments comprise a non-stretchable mesh fabric, for example, a substantially non-expanding polyester fabric mesh. In another embodiment, the mesh segments comprise a stretchable mesh fabric.

[0025] The method may further comprise the step of applying a tacky material to the curved molding surface prior to the step of positioning the mesh. The tacky material may be a fluid elastomeric material, for example, a silicone dispersion.

[0026] In another embodiment, the method comprises pre-shaping, for example, thermoforming, a mesh element, from a two-dimensional sheet into a three dimensional "sock" having the general shape of the molding surface. The method includes positioning the pre-shaped mesh element onto the molding surface, applying a fluid elastomeric material to the molding surface with the pre-formed mesh positioned thereon, and allowing the elastomeric material to set to form a flexible shell having an open end, the shell including the preformed mesh

embedded within the set elastomer, and the shell being useful as a component of an inflatable prosthesis.

[0027] In another embodiment of the invention, an inflatable prosthesis made by the methods described herein is provided.

[0028] Further, in another embodiment, an inflatable prosthesis generally comprises an interior shell defining an inflatable chamber, an exterior shell comprising a silicone-based elastomer material having a mesh embedded therein, a gel separating the interior shell and the exterior shell, and a puncture resistant member forming a base of the prosthesis.

[0029] In yet another embodiment of the invention, a method of making a needle guard for an inflatable prosthesis suitable for implantation in a mammal is provided. The method generally comprises the steps of providing a first layer of puncture resistant members, for example, elongated slats, providing a second layer of puncture resistant members such that the second layer of members overlies and is offset from the first layer of members, molding or otherwise applying a flexible material to the first layer of members and the second layer of slats to form a device useful as a needle guard for an inflatable prosthesis. The step of applying or molding includes coupling the members to, for example, encasing the members within the flexible material.

[0030] In one embodiment, the members are elongated slats, and the slats of the first layer are substantially parallel to the slats of the second layer. The slats may be made of any suitable puncture resistant material, for example, a material selected from a group of materials comprising acetal, nylon, and polycarbonate. In some embodiments, the slats are made of a metal, for example, stainless steel, aluminum or titanium. The slats may be individual, separate elements that are cut from a sheet of material using any suitable means such as laser cutting. In other embodiments, at least one of the first layer

of slats and the second layer of slats comprises a single, undivided sheet of material having grooves defining the adjacent slats.

[0031] In some embodiments, the step of applying a flexible material comprises applying an elastomeric sheet between the first layer of slats and the second layer of slats, for example, applying an uncured elastomeric sheet between the first layer of slats and the second layer of slats, and subsequently curing the sheets.

[0032] Alternative to the first and second layers of slats, a puncture-resistant fabric may be used, for example, in conjunction with an elastomeric layer, to form a suitable needle guard.

[0033] In one embodiment of the invention, a method for making an inflatable prosthesis suitable for implantation in a mammal is provided, wherein the method comprises providing a needle guard made by a method of the invention as described elsewhere herein and securing a flexible, inflatable shell to the needle guard.

[0034] In another embodiment of the invention, an inflatable prosthesis is provided generally comprising a flexible shell forming an anterior surface of the prosthesis, wherein the needle guard forms at least a portion of a posterior surface of the prosthesis, and comprises an elastomer portion and a first layer of puncture resistant slats embedded in the elastomer portion.

[0035] The needle guard may further comprise a second layer of puncture resistant slats. In some embodiments, the second layer of slats is offset from the first layer of slats.

[0036] In yet another embodiment of the invention, flexible, resilient puncture resistant assemblies are provided, the assemblies being, useful as components of surgical implants, for

example, but not limited to, needle guards as components of inflatable implants that are accessed with a needle and a syringe. Such implants for which the present materials are useful include inflatable tissue expanders. Other implants that can benefit from the present invention include fluid access ports which include a fluid reservoir and a needle penetratable septum. In these and other implantable devices, puncture resistant or puncture proof assemblies of the invention can be highly beneficial, for example, as a means for preventing a needle tip from penetrating other areas of the device that are not intended to be punctured. For example, a needle guard assembly may serve to protect a tube leading from an implantable access port from being punctured by a syringe needle. Other beneficial uses for the present assemblies will become more apparent upon reading the present specification, and are considered to be included within the scope of the invention.

[0037] For example, puncture resistant assemblies are provided which are flexible and/or formable into desired configurations.

[0038] In some embodiments, puncture resistant assemblies are provided which are both flexible and resilient. Some of the present assemblies have the characteristic of shape memory, such that after being rolled or folded, they can resume an original shape or configuration. This embodiment of the invention is particularly, but certainly not exclusively, useful for application in a surgical environment, in which the assembly may be in the form of a puncture proof material is rolled or folded into a narrow configuration, thereby enabling insertion thereof through a relatively small incision. Advantageously, some of the assemblies of the invention are structured to be able to automatically resume an original, pre-deformed shape, for example, automatically, once the material is at the desired implantation site.

[0039] In one embodiment of the invention, a puncture resistant assembly is provided which generally comprises a first composite guard, a second composite guard, and an intermediate layer securing the first and second composite guards together and/or containing the first and second composite guards.

[0040] Each of the first and second composite guards generally comprises an arrangement of puncture resistant elements or members and a flexible substrate on which the members are secured and positioned, generally in a spaced-apart relationship.

[0041] The members may be in the form of domes or plates. The members have a hardness effective to resist penetration, puncture or breakage upon forceful contact with a sharp surface, for example, a tip of a needle, an edge of a cutting implement such as a scalpel or knife, or the like. The members may be made of any suitable material, such as a hard moldable substance, for example, a high durometer elastomer, polymer or rubber. Other suitable materials include metals, ceramics, and alloys thereof.

[0042] The flexible substrate on which the members are disposed may comprise a fabric, mesh, film, elastomer, or other material.

[0043] Notably, the first composite guard and the second composite guard are disposed with respect to one another such that the arrangement of members of the first composite guard is offset or misaligned with respect to the arrangement of members of the second composite guard. In some embodiments, a third composite guard is provided. The third composite guard may be positioned with respect to the first and second composite guards such that the members of the third composite guard are misaligned with the members of at least one of the first and second composite guards.

[0044] Advantageously, the misaligned or overlapping members of the adjacent composite guards provide a puncture resistant, or puncture proof, area while not significantly sacrificing flexibility of the assembly as a whole. That is, the composite guards may be arranged such that there are no significant gaps between individual puncture resistant members. It can be appreciated that depending upon the use of the final assembly, there may be some gaps between members so long as the gaps are sufficiently narrow to resist or prevent penetration by the type of instrument that the assembly is intended to be protected against puncture from.

[0045] In any event, in some embodiments of the invention, the puncture resistant members of the composite guards may provide an area of protection that substantially entirely covers a first side of the needle guard assembly.

[0046] The assembly may further comprise an intermediate layer, for example, an elastomer, securing together the first and second composite guards such that the members maintain their offset relationship. The intermediate layer may be located between adjacent composite guards and may be bonded thereto. In one embodiment, the intermediate layer seals the flexible composite members together and encapsulates the composite guards. For example, the intermediate layer may be a fluid tight barrier containing the two or more layered composite guards. In some embodiments, the intermediate layer exhibits a springiness and resiliency or provides a shape memory characteristic to the assembly.

[0047] In another aspect of the invention, a method of making a needle guard assembly is provided wherein the method generally comprises the steps of providing first and second composite guards where each composite guard includes a layer of puncture resistant members secured to a flexible substrate and bonding the first composite guard with the second composite guard in

such that the members of the first composite guard are misaligned with the members of the second composite guard. In some embodiments, the method includes the step of bonding a third composite guard to the second composite guard such that the members of the third composite guard are misaligned with the members of at least one of the first composite guard and/or the second composite guard.

[0048] In some embodiments, the method may comprise the step of providing an intermediate layer between the composite guards. In some embodiments, the method may comprise the step of encasing or encapsulating the composite guards in a fluid tight seal.

[0049] In one embodiment, an inflatable prosthesis is provided which comprises an inflatable portion including an interior shell, an exterior shell comprising a silicone-based elastomer material having a mesh embedded therein and a gel separating the interior shell and the exterior shell. The prosthesis further comprises a needle guard assembly comprising a first composite guard and a second composite guard, each composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members are disposed in a spaced apart fashion. The first composite guard and the second composite guard are positioned such that the arrangement of puncture resistant members of the second composite guard are misaligned with the arrangement of puncture resistant members of the first composite guard. The needle guard assembly further comprises an intermediate layer disposed between and connecting the first composite guard with the second composite guard.

[0050] In one embodiment, a needle guard assembly to protect a tube leading from an access port is provided. The needle guard assembly protects the tube from puncture by an incoming syringe needle. The needle guard assembly may comprise a first

composite guard and a second composite guard, each composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members are positioned. The first composite guard and the second composite guard are positioned such that the arrangement of puncture resistant members of the second composite guard is misaligned with the arrangement of puncture resistant members of the first composite guard. The needle guard assembly further comprises an intermediate layer positioned between and connecting the first composite guard with the second composite guard. The needle guard assembly may further comprise a top layer and a bottom layer forming outer surfaces of the needle guard assembly.

[0051] Each and every feature described herein, and each and every combination of two or more of such features, is included within the scope of the present invention provided that the features included in such a combination are not mutually inconsistent.

BRIEF DESCRIPTION OF THE DRAWINGS

[0052] The present invention may be more clearly understood and certain aspects and advantages thereof better appreciated with reference to the following Detailed Description when considered with the accompanying Drawings of which:

[0053] Figure 1 is cross-sectional view of a tissue expander in accordance with an embodiment of the invention, the tissue expander shown as implanted in a breast of a human being;

[0054] Figure 2 is magnified view of a portion of the expander shown in Figure 1;

[0055] Figure 3 is a cross-sectional view of another tissue expander in accordance with an embodiment of the invention;

[0056] Figure 4 is a cross-sectional view taken along line 4-4 of Figure 3;

[0057] Figures 4A and 4B are a simplified top view and cross sectional view, respectively, of a needle guard feature of the tissue expanders in accordance with an embodiment of the invention;

[0058] Figure 5 is a cross-sectional view of another tissue expander in accordance with an embodiment of the invention;

[0059] Figure 6 is a cross-sectional view of yet another tissue expander in accordance with an embodiment of the invention;

[0060] Figure 7 is a cross-sectional view taken along line 7-7 of Figure 6;

[0061] Figures 8-10 show steps useful in making some of the tissue expanders in accordance with an embodiment of the invention;

[0062] Figure 11 is cross-sectional view of another inflatable prosthesis including a puncture resistant assembly in accordance with an embodiment of the invention;

[0063] Figure 12 is an exploded view of the prosthesis shown in Figure 11 in order to illustrate certain components of the puncture resistant assembly;

[0064] Figure 13 is a top view of a composite guard which is a component of the puncture resistant assembly shown in Figure 11;

[0065] Figure 14 is a magnified view of a portion of the composite encompassed by line 14 of Figure 13;

[0066] Figure 15 is a cross-sectional view of the composite guard taken along line 15-15 of Figure 14;

[0067] Figure 16 is a cross-sectional view, similar to the view shown in Figure 15, of an alternative composite guard in accordance with an embodiment of the invention;

[0068] Figure 16a is a cross-sectional view, similar to the view shown in Figure 15, of yet another composite guard in accordance with an embodiment of the invention;

[0069] Figures 17-19 illustrate steps useful in making some of the puncture resistant assemblies in accordance with an embodiment of the invention;

[0070] Figure 20 illustrates a perspective view of a gastric banding system including a needle guard assembly, in accordance with an embodiment of the invention;

[0071] Figure 21 illustrates a perspective view of an access port, tube, and needle guard assembly in accordance with an embodiment of the invention;

[0072] Figure 22 illustrates a cross-sectional view of the needle guard assembly and tube shown in Figure 21, taken along line 22-22 of Figure 21;

[0073] Figure 23 illustrates a perspective view of an access port, tube, and needle guard assembly in accordance with an embodiment of the invention;

[0074] Figure 24 illustrates a cross-sectional view of the needle guard assembly and tube shown in Figure 23, taken along line 24-24 of Figure 23;

[0075] Figure 25 illustrates a magnified view of a portion of the needle guard assembly encompassed by line 25 of Figure 24;

[0076] Figure 26 illustrates a perspective view of a clip engaged with an access port in accordance with an embodiment of the invention;

[0077] Figure 27 illustrates a perspective view of the clip shown in Figure 26, in accordance with an embodiment of the invention;

[0078] Figure 28 illustrates a bottom view of the clip shown in Figure 26, and a bottom view of the access port shown in Figure 26, in accordance with an embodiment of the invention;

[0079] Figure 29 illustrates a perspective view of a needle guard assembly having a flanged portion, in accordance with an embodiment of the invention;

[0080] Figure 30 illustrates a perspective view of the needle guard assembly shown in Figure 29, separated from an access port, in accordance with an embodiment of the invention;

[0081] Figures 31 and 32 illustrate sheets of material for use as composite guards in accordance with an embodiment of the invention;

[0082] Figure 33 illustrates a top view of a composite guard in accordance with an embodiment of the invention;

[0083] Figure 34 illustrates a perspective view of three composite guards and a frame in accordance with an embodiment of the invention;

[0084] Figure 35 illustrates a top perspective view of three composite guards with a frame passing therethrough in accordance with an embodiment of the invention;

[0085] Figure 36 illustrates a bottom perspective view of the three composite guards with a frame passing therethrough, as shown in Figure 35;

[0086] Figure 37 illustrates a perspective view of a needle guard assembly in accordance with an embodiment of the invention; and

[0087] Figure 38 illustrates a magnified view of a portion of the needle guard assembly shown in Figure 37.

DETAILED DESCRIPTION

[0088] The present invention generally pertains to implantable inflatable devices and methods for making same, for example, devices such as soft fluid-filled implants, for example, but not limited to, permanent or temporary implants useful in breast reconstruction or breast augmentation procedures.

[0089] Turning now to Figure 1, an inflatable device, in accordance with an embodiment of the invention, is shown generally at **10**, as implanted in a human breast **2**. The device **10** is being inflated with a suitable fluid, such as a saline solution **14**, by means of a typical syringe **18**.

[0090] The device **10** generally comprises an inflatable portion **12** comprising an outer shell **22**, an inner shell **24** and an intermediate layer **26** therebetween. The inner shell **24** defines an inflatable cavity **28** (shown here as being filled with saline solution **14**).

[0091] Inflation of the cavity **28** causes expansion of the device as shown by arrows **30**. The device **10** further includes a posterior portion **34** that is generally resistant to expansion upon inflation of the cavity **28**. The total volume of the device **10** is adjustable by introduction and removal of fluid into and from the fillable cavity **28**.

[0092] The outer shell **22** of the device **10** may comprise at least one layer of elastomeric material, for example, a first layer **36** of elastomeric material and a second layer **38** of elastomeric material, and an additional layer of a different material, for example, a reinforcement layer **40** located between the first and second layers **36**, **38** of the elastomeric material.

[0093] The elastomeric material may be a silicone elastomer such as a dimethyl silicone elastomer, for example, a substantially homogeneous dimethyl-diphenyl silicone elastomer. One composition useful in the present invention is described in Schuessler, et al., U.S. Application Serial No. 12/179,340, filed on July 24, 2008, the disclosure of which is incorporated herein in its entirety by this specific reference. The elastomeric material may comprise a room temperature vulcanizing (RTV) or a high temperature vulcanizing (HTV) silicone from about 0.1-95 wt %, for example, about 1-40 wt %, for example, about 30 wt %. In an exemplary embodiment, the silicone-based

fluid material is a high temperature vulcanizing (HTV) platinum-cured silicone dispersion in xylene.

[0094] The reinforcement layer **40** may comprise a mesh or fabric, for example, a synthetic polymer mesh or fabric, for example, a mesh or fabric made from poly (ethylene terephthalate) (PET), polypropylene (PP), polyurethane (PU), polyamide (Nylon), polyethylene (PE), any other suitable material, or combinations thereof.

[0095] In an exemplary embodiment, the outer shell **22** is made by dipping two or more layers of silicone-based elastomer over a conventional breast implant mandrel, followed by placement of a pre-fabricated 2 or 4-way stretchable "sock" of the reinforcing material layer **40**, followed by two or more dips of the silicone-based elastomer. The reinforcing "sock" is able to take the shape of the mandrel and the fabric is trapped on both sides between the elastomer layers **36**, **38**. In this embodiment, the stretchable pre-shaped "sock" (which may form the reinforcing layer **40** of the outer shell **22**) can be relatively easily mounted on the mandrel because of its flexibility and elasticity, making it easier to manufacture a reinforced shell with the intended shape and dimensions of the mandrel. The entire assembly forming the outer shell **22** is heated in an oven at a temperature and time suitable to cure the silicone.

[0096] In one embodiment of the invention, the reinforcement layer **40** is provided by forming a "sock" by using a cinch **40a** as illustrated in Figures 8 and 9. Alternatively, the reinforcement layer **40** is thermoformed into "sock" by placing a single sheet of suitable material, for example, a non-stretchable mesh, over a curved molding surface, for example, a mandrel, and gathering the mesh material at **40b**, as shown in Figure 10. The gathered mesh material is shaped, for example, thermoformed, to take on the 3-D shape of the mandrel.

[0097] Alternatively, rather than mesh sock, the reinforcement layer may comprise a plurality of fabric or mesh segments which are positioned on a mandrel or other curved molding surface. The segments may substantially entirely cover the molding surface. The segments may be positioned such that they overlap one another. The molding surface may first be contacted with a tacky material, for example, contacted with or coated with a silicone elastomer dispersion, to facilitate adherence of the segments thereto. An elastomeric material, such as an uncured silicone sheet or a silicone dispersion, is applied to the molding surface with the segments positioned thereon. The elastomeric material is allowed to set to form a flexible shell having an open end, the shell including the fabric or mesh segments embedded within the set elastomer, and the shell being useful as a component of an inflatable prosthesis.

[0098] Post-curing, the reinforced shell is removed from the mandrel, and another elastomeric shell (which forms the inner shell **24**) is placed inside the first shell (which forms the outer shell **22**). The inner shell **24** may be a typical unreinforced elastomeric shell, or alternatively may be made similarly to that described above with respect to the outer shell **22**. The inner shell **24** may have the same or smaller size relative to the outer shell **22**. The two shells **22**, **24** are vulcanized close to their open base using, for example, a ring-shaped patch **44**, thus forming an inter-shell compartment. The dual-shell assembly is mounted back on a mandrel. The size of the mandrel can be the same as the one used for the inner shell fabrication or slightly larger. The latter would result in a laterally stressed inner shell with potentially enhanced sealing properties.

[0099] In some embodiments of the invention, at least one of the inner shell **24** and the outer shell **22** comprises an elastomeric material comprising a substantially homogenous layer of a

silicone elastomer comprising a polysiloxane backbone and having a minimum mole percent of at least 10% of a substituted or pendant chemical group that sterically retards permeation of said silicone gel through the layer. More specifically, in this embodiment, the silicone elastomer is a polydimethyl siloxane and the pendant chemical group is one of a phenyl group, for example, a diphenyl group or a methyl-phenyl group, a trifluoropropyl group, and mixtures thereof. Such materials are described in detail in Schuessler, et al., U.S. Patent Application No. 12/179,340, filed on July 24, 2008, the entire disclosure of which is incorporated herein by this specific reference. This material may make up one or more layers of the shell(s) **22**, **24**.

[0100] After the inner shell **24** and the outer shell **22** are bonded together, a cavity formed therebetween is then filled with a material, for example, a flowable material, for example, a silicone gel. This may be accomplished using any suitable means known to those of skill in the art. In one embodiment, the gel is introduced through a reinforced silicone plug on the outer shell **22**. The silicone gel between the outer and inner shells **22**, **24**, forms the intermediate layer **26**. After filling, the assembly made up of the inner shell **24**, the outer shell **22** and the intermediate layer **26**, is cured, for example, by exposing the assembly to heat in an oven for a suitable length of time. The mandrel that defines the desired shape of the implant can be round or oval, with a lower or upper pole for optimal projection. Before sealing the implant with a patch, a needle guard element, such as that described and shown elsewhere herein, may be inserted and bonded to the inner shell **24** and/or the outer shell **22**, to form the posterior portion **34** of the device.

[0101] It can be appreciated that the device **10**, in the form of a tissue expander, once implanted in a patient, should be

repeatedly accessed during the expansion process with percutaneous needle punctures, such as shown in Figure 1. In some embodiments, the tissue expander devices are able to survive repeated puncturing and over-expansion to 200% by saline without leakage.

[0102] The device **10** can also be in the form of a more permanent mammary prosthesis, for example, an adjustable breast implant. The volume of the implant can be adjusted in situ by accessing the cavity **28** with a needle through the self-sealing anterior portion of the device **10**. In some embodiments, the cavity **28** has a small volume relative to the gel portion **26**, to provide a comfortable implant having the desirable qualities of a gel-filled implant with the advantages of being size-adjustable with saline.

[0103] The anterior surface of the device **10** is self-sealing and can be accessed for fluid communication. The mechanism of self-sealing is facilitated by a combination of the gel layer **26** and shell **22**. After a void is created by a needle used to introduce filler (saline) into the implant **10**, the gel layer **26** prevents the saline **14** from having a direct path to the exterior and the reinforcing mesh **40** enhances this property by physically constraining the gel from expansion under pressure exerted by the saline **14**. The reinforcing materials **40** include, but are not limited to, meshes and fabrics made from PET, PP, PU, Nylon, etc. and combinations thereof. This invention features a novel manufacturing method for shaping the implant shell into 2-D and 3-D structures making it more convenient to manufacture and convert these reinforced structures into mammary prostheses.

[0104] In order to limit the depth of penetration of the needle, and also to give the medical professional feedback as to when the needle has reached the correct location for filling, conventional tissue expander devices sometimes include a rigid backing or needle stop behind the filling port in the posterior

side of the device. Typically these needle stops are made of metals or very hard or thick plastics to prevent needle penetration through the injection site. By nature then, these needle stops are quite rigid and inflexible, can be uncomfortable, and can limit the collapsibility of the device which affects ease of insertion of the expander through the initial incision.

[0105] The posterior portion **34** of device **10** may comprise an improved needle guard **50**. The needle guard **50** may comprise any suitable biocompatible polymer (e.g. PE, PP, PU, PET, PI, TPU, high durometer silicones, ABS etc.) that is strong enough to resist needle puncture. The needle guard **50** may comprise one or more layers **56** of puncture resistant material with or without an intermediate layer **58**. In some embodiments, the needle guard **50** is structured so as to prevent, or substantially prevent, the device **10** from expanding toward the chest wall during inflation of the cavity **28**.

[0106] For filling an implant of the present invention, a syringe coupled to a 21g or smaller needle may be used. The needle may be introduced anywhere in the anterior portion of the implant, such that it reaches the needle guard **50**, where it is prevented from penetrating further. The implant is then filled with saline or other liquids for tissue expansion. After removal of the needle, the assembly (e.g., the outer shell **22**, the inner shell **24** and the intermediate layer **26**) self-seals and prevents the implant from leaking.

[0107] In Figures 3 and 4, the needle guard **50** may comprise an elastomer portion **62**, and one or more layers of puncture resistant members coupled thereto. In the shown embodiment, members comprise elongated members, for example, slats **68** coupled to the elastomer portion **62**.

[0108] In this case, the needle guard **50** comprises one or more layers of slats **68**, for example, a first layer **64** of slats **68**

and a second layer **66** of slats **68** coupled to the elastomer portion **62**. As shown, the slats **68** of the first layer **64** overlap, or are offset from, the slats **68** of the second layer **66**. For example, spacing between the slats **68** of the first layer **64** are aligned with slats of the second layer **66** and vice versa. The elastomer portion **62** may include grooves **69** or slots. The grooves may be aligned with the slats **68** to facilitate rolling or folding of the device **10**.

[0109] The slats **68** extend across substantially the entire posterior portion **34** and are aligned substantially parallel to one another. This arrangement allows the device **10** to be rolled or folded in alignment with the slats **68** while the offset or overlapping positioning of the first and second layers **64**, **66** provides protection in the event a needle enters the spacing **70** between adjacent slats **68**.

[0110] Alternative to this arrangement, adjacent slats in each layer may overlap one another (not shown). The needle guard comprises overlapping but independent small pieces of rigid puncture-resistant material, and like the offset layers of slats **68** described and shown elsewhere herein, the overlapping configuration provide that there are no "line-of-sight" openings through which a needle can pass.

[0111] The slats **68** may be a polymer material. The slats **68** may be, for example, nylon, acetal, polycarbonate, or other suitable, biocompatible, puncture resistant or puncture-proof polymeric material. The slats **68** may be metal, for example, stainless steel, aluminum or titanium.

[0112] In various exemplary embodiments, the slats **68** may be between about 10 mm to about 100 mm or more in length, about 2 mm to about 30 mm in width, and about 0.2 mm to about 4 mm in thickness. The slats of other configurations and dimensions suitable for achieving the desired flexibility of the needle guard **50** may also be used. Such variations of materials and

dimensions are considered to fall within the scope of the present invention. In one embodiment, the slats **68** have a thickness of about 2 mm and the needle guard **50**, including first and second layers **64**, **66** of the slats **68** and elastomer material therebetween, has a total thickness of about 5.0 mm or less.

[0113] The slats **68** may be formed by laser cutting same from a sheet of material. Alternatively, the slats **68** may be defined by grooves in a single sheet of material. In this specific example, the 2 layers of parallel slats of puncture-resistant plastic about .25" wide and with about .05" open space between each slat. The layers are offset from each other so that the open space of one slat layer is centered on the middle of a slat in the layer below. All the slats are encapsulated in a soft flexible material like silicone. The open space between the slats gives the whole assembly flexibility to be readily folded or rolled up even though the plastic itself is rigid and resistant to extensive bending. Other shapes and layering designs of independent pieces of puncture resistant materials would provide the needle stop with more and different degrees of bending and folding capability.

[0114] The rigid or semi-rigid material forming the slats can be thermoplastics such as acetal, nylon, polycarbonate, and others; or thin metals such as stainless steels, aluminum, or titanium. The use of plastics can be advantageous in that the entire device **10** can be made to be MRI compatible.

[0115] In a similar embodiment of the invention, thin elastomeric films (0.25-1mm) made of materials resistant to needle puncture may be used as a component of the needle guard portion of the implant. In some embodiments, such films can be provided with grooves in their design to allow folding/unfolding during insertion. The films may be attached to the shell using adhesives or alternatively may be are encapsulated in silicone.

[0116] In another embodiment, rather than independent slats **68**, one or more layers of flexible "slat sheets" are provided. In this embodiment, adjoining slats can be made by starting with readily available sheets of the desired plastic of the appropriate thickness. Parallel, adjacent slats are created by laser cutting through the plastic to create the desired spacing between the slats but not all the way to the edges of the plastic sheet, thereby leaving a material, for example, a border that holds all the slats together. In this way, the pre-cut slats can still be handled as one piece and therefore maintain the desired spacing and orientation. In one embodiment, two of these pre-cut plastic "slat sheets" are alternately layered between 3 sheets of silicone. After curing the silicone, a die cutter of the desired shape of the needle stop can cut within the borders of the pre-cut slats to stamp out the finished needle stop that now has many unconnected slats each independently encased in silicone.

[0117] Alternatively still, the pre-cut slat sheets can be held in the desired orientation in a mold and silicone can be injected and cured around them. Additional assembly steps can include creating a silicone border around the needle stop that would assemble to the expander envelope, texturing or adding features to the needle stop surface, or shaping the needle stop assembly so that it has a concave exterior to better fit the chest wall anatomy in the case of a breast tissue expander.

[0118] Turning to Figures 4A and 4B, yet another variation of a needle guard **150** is provided, similar to the needle guard **50**, except that rather than the slats **68**, one or more layers of a puncture resistant mesh **152** are provided. The needle guard **150** may be substantially identical to the needle guard **50** described above, with one or more differences being as follows.

[0119] In the shown exemplary embodiment, the needle guard **150** comprises one or more layers of mesh **152**, for example, a single

layer of mesh **152** coupled to, for example, embedded in, the elastomer portion **162**. In other embodiments, not shown, two or more layers of mesh are provided, wherein fibers or cords making up the mesh, in adjacent layers of mesh, overlap one another. For example, interstices or a spacing between a mesh fiber of a first layer of mesh aligns with the mesh fiber of a second layer of mesh, and vice versa. Alternatively, a single layer of mesh is provided with interstices between fibers being sized to prevent needle penetration therethrough.

[0120] Flexibility of the mesh **152** and the elastomer portion **162** allow the entire implant device to be rolled or folded upon insertion into a breast cavity through a small incision.

[0121] The mesh **152** may be a polymer or a metallic material. The mesh may be, for example, a polymer such as nylon, acetal, polycarbonate, or other suitable, biocompatible, puncture resistant or puncture-proof material. The mesh **152** may be metal, for example, stainless steel, aluminum or titanium.

[0122] It should be appreciated that in many of the embodiments of the present invention, the needle guard making up the posterior portion of the implant comprises puncture resistant members arranged in an overlapping configuration to provide no "line-of-sight" openings through which a needle can pass. These puncture resistant members can be variously configured and arranged to achieve this goal.

[0123] In a preferred embodiment, it is desirable for the needle stop to be flexible for insertion yet rigid to resist needle puncture. To prevent movement of the needle guard inside the device, the needle stop material may be adhered, fused or vulcanized to the posterior of the implant or the patch. For this purpose, the needle guard may be dipped in silicone that is then heat cured, such that the needle guard is covered by a silicone sheath. This silicone sheath is vulcanized to the

silicone patch or posterior of the implant, to prevent movement of the guard inside the implant.

[0124] Another device **110** in accordance with the invention is shown in Figures 5-7. The device **110** may be substantially identical to the device **10** except that the device **110** does not include an inner shell **24** or an intermediate layer **26**. The device **110** comprises a self-sealing outer layer **122**. The self-sealing outer layer **122** may be identical to the layer **22** of the device **10**. Further, rather than the needle guard **50**, the device **110** comprises the needle guard **128** which comprises a puncture resistant elastomeric member **130** having grooves **132** for facilitating rolling or folding of the device **110** during insertion.

[0125] Turning now to Figures 11-16a, another device, for example, an inflatable implant, in accordance with the invention is shown generally at **310**. The implant **310** may be identical to the implant **10** shown in Figure 3, with the primary difference being that instead of the needle guard **50** made up of layers of slats as described elsewhere herein, the implant **310** includes a puncture resistant material **314** as shown and now described.

[0126] The device **310** includes an inflatable portion **312**, and a puncture resistant assembly **314**.

[0127] The device **310** is expanded or inflated (or deflated) by insertion of a needle **313** (Figure 11) through the inflatable portion **312** (which may be identical to the inflatable portion **12** of the device **10**) and introduction of fluid into a cavity **312a**. Instead of the inflatable portion **12**, it can be appreciated that the inflatable portion **312** can include any suitable structure, including an elastomeric bladder having an access port with a needle penetratable septum, or may be made partially or entirely of a puncturable, but self sealing material. Some suitable self sealing materials are described, for example, in U.S. Patent Application No. 12/543,795, filed on August 19, 2009, the entire

specifications of which are incorporated herein by this reference.

[0128] In order to prevent the needle **313** from undesirably penetrating through the device **310**, the device is equipped with an assembly **314**.

[0129] Referring now to Figure 12, the assembly **314** generally comprises a first composite guard **316** and a second composite guard **318**. In the shown embodiment, the assembly **314** further includes a third composite guard **320**. In other embodiments, only two composite guards or more than three composite guards are provided. An intermediate layer **324** is provided between adjacent guards, for example, between the guard **316** and the guard **318**, and likewise, between the guard **318** and the guard **320**.

[0130] Turning now as well to Figures 13 and 14, each of the composite guards **316**, **318**, **320** includes a plurality of, for example, an arrangement, array, or pattern of, puncture resistant members **330**, and a flexible substrate **332** having a first side on which the puncture resistant members **330** are disposed in a generally spaced apart fashion.

[0131] As can be perhaps best appreciated from Figure 11 (and Figure 19), the first composite guard **316** and the second composite guard **318** are positioned such that the arrangement of puncture resistant members **330** of the second composite guard **318** are misaligned with the arrangement of puncture resistant members **330** of the first composite guard **316**. Similarly, the second composite guard **318** and the third composite guard **320** may be positioned such that the arrangement of the puncture resistant members of the third composite guard **320** are misaligned with the arrangement of puncture resistant members of at least one of the first composite guard **316** and the second composite guard **318**. Thus, accordingly, the composite guards **316**, **318**, **320** are arranged relative to one another such that

there are no straight line open spaces, or substantial gaps, between the members **330** to allow a needle or sharp implement to penetrate entirely through the assembly **314**. Yet, advantageously, the assembly **314** as a whole may be quite flexible in that the substrate **332** on which the spaced apart **330** members are disposed is supple, flexible and/or bendable.

[0132] Turning specifically to Figure 12, the intermediate layer **324** may comprise a flexible, connecting material which is effective to couple or bond the first composite guard **316** with the second composite guard **318**, and the second composite guard **318** with the third composite guard **320**. As shown in Figure 12, the intermediate layer **324** is positioned between the arrangement of the puncture resistant members **330** of the first layer **316** and the flexible substrate **332** of the second layer **318**, and another intermediate layer **324** is positioned between the arrangement of the puncture resistant members **330** of the second layer **318** and the flexible substrate **332** of the third layer **320**.

[0133] The composite guards **316**, **318**, **320** may be identical to one another, and for the sake of simplicity, only the first composite guard **316** will now be described, with the understanding that, in the shown embodiment, what is described for the first composite guard **316** is also applicable to the second composite guard **318** and the third composite guard **320**.

[0134] The members **330** may be any suitable shape. In Figure 15, the members **330** are somewhat dome shaped with rounded surfaces. In other embodiments, the members **330a** may be planar as illustrated in Figure 16. Alternatively still, the members **330b** may include both rounded surfaces and planar or flat surfaces, such as the members **330b** which are dome shaped with a flat upper surface, as illustrated in Figure 16a.

[0135] The members **330** have a thickness of between about 0.1 mm and about 1.0 mm, for example, a thickness of between about 0.2 mm and about 0.5 mm. The members **330** have a spacing D of

between about 0.2 mm and about 0.5 mm. The members **330** have a diameter of between about 0.5 mm and about 2.0 mm, for example, a diameter of about 1.5 mm.

[0136] In some embodiments, the guard **316** includes between about 50 and about 1000 members per square inch (psi), for example, about 400 psi.

[0137] In a specific embodiment, the guard **316** include about 400 members psi, each having a diameter of about 1.5 mm and each being spaced apart about 0.2 mm.

[0138] The members **330** (and **330a** and **330b**) are made of a suitable puncture resistant material, such as an epoxy, polymer, rubber, ceramic or metal, or suitable combination or alloy thereof. For some applications, suitable materials include polyethylene (PE), polypropylene (PP), polyurethane (PU), polyethylene terephthalate (PET), polycarbonate (PC), polyisoprene (PI), thermoplastic urethanes and thermoplastic polyurethanes (TPU), high durometer silicones, acrylonitrile butadiene styrene (ABS), etc. In some embodiments, the members **330** are made of material such as acetal, nylon, and polycarbonate. In some embodiments, the members **330** are made of a metal, for example, stainless steel, aluminum, titanium, or other metal. The members **330** may be made of any other material specifically indicated to comprise the puncture resistant members **330** in this application, including any materials discussed in relation to the members **430**, **436**, **530**, **536**, **550** shown in Figures 22 and 24-25, and the members **1030**, **1036**, **1050** shown in Figure 38.

[0139] The flexible substrate **332** may comprise a mesh, film, fabric, elastomer, or other suitable material. The flexible substrate **332** may be made of any other material specifically indicated to comprise the flexible substrate **332** in this application, including any materials discussed in relation to the flexible substrates **432**, **434**, **532**, **534**, **552** shown in Figures

22 and 24-25, and the substrates **1032**, **1034**, **1052** shown in Figure 38.

[0140] The intermediate layer **324** may be a polymer, for example, an elastomeric polymer, for example, a silicone elastomer, for example, a low durometer silicone rubber. The intermediate layer **324** may be made of any other material specifically indicated to comprise the intermediate layer **324** in this application, including any materials discussed in relation to the intermediate layers **424**, **524**, **525** shown in Figures 22 and 24-25, and the intermediate layers **1024**, **1025** shown in Figure 38.

[0141] In some embodiments, the assembly **314** has a resiliency or a shape memory such that it will restore from a folded or rolled configuration to an original, different configuration. The original configuration may be a generally flat or planar configuration. This may be provided by using a suitable intermediate layer material, such as a silicone elastomer, that has a shape memory characteristic.

[0142] Assembly of the guard assembly **314** may be accomplished as follows and as shown in Figures 17-19.

[0143] Turning now to Figure 17, the guard **316**, generally comprising the members **330** and the substrate **332**, is made by any suitable method, including stencil printing, for example, using equipment and processes used in surface mount technology/PCB fabrication. Other processes that can be used to make the guard **316** include micro-dot dispensing and printing, and laser etching. Other suitable methods will be known to those skilled in the art. Other suitable methods include those discussed in relation to the formation of the composite guards **416**, **418**, **516**, **518**, **520** shown in Figures 22 and 24-25.

[0144] Turning to Figure 18, the intermediate layer **324** may be formed as follows. A suitable material, for example, a sheet of

uncured silicone, is placed on one side of the guard **316**, for example, on the side having the members **330** and the substrate **332**. The sheet is then subjected to curing conditions to cause the sheet to adhere to the members **330**, forming the intermediate layer **324** thereon. In the presently described example embodiment, this step is done three times, with three separate guards **316**, **318**, **320**, to form the components **316'**, **318'** and **320'** of assembly **314**. (See Figure 18a).

[0145] The assembly **314** is then placed in an oven or otherwise subjected to further curing conditions to seal the assembly **15** components together such as shown in Figure 19.

[0146] Figure 20 illustrates an embodiment of the present invention, in which a needle guard assembly **414**, having a similar construction as the needle guard assembly **314** discussed in relation to Figures 11-19, is utilized to protect a tube **402** used in conjunction with an implantable access port **404**. In the embodiment shown in Figure 20, the tube **402**, the access port **404**, and the needle guard assembly **414**, are used in an implantable gastric banding system **406**, including a gastric band **408** configured to form a loop around a portion of a patient's **410** stomach **412** to form a stoma. The gastric band **408** may have a composition as described in Birk, U.S. Patent No. 7,811,298, the entire disclosure of which is incorporated herein by this specific reference.

[0147] The gastric banding system **406** is used for the treatment of obesity. The gastric band **408** is preferably wrapped around the cardia, or esophageal junction of the stomach **412**, to restrict the flow of food passing from the upper portions of the patient's **410** stomach **412** to the lower portions of the patient's **410** stomach **412**. The restricted flow of food enhances the satiety signals sensed by the patient **410**, which desirably reduces food consumption of the patient **410**, which hopefully causes the patient **410** to lose weight.

[0148] Over time, a physician may need to adjust the degree to which the gastric band **408** constricts the patient's **410** stomach **412**. As such, the gastric band **408** may include an inflatable portion **422**, which comprises an inflatable cuff that wraps around the patient's **410** stomach **412**. The inflatable portion **422** may be filled with fluid. The amount of fluid in the inflatable portion **422** defines the degree to which the gastric band **408** constricts the patient's **410** stomach **412** (e.g., a greater amount of fluid in the inflatable portion **422** will increase the constriction of the patient's stomach). A physician may adjust the amount of fluid in the inflatable portion **422** via the access port **404**.

[0149] The access port **404** is preferably fixed subcutaneously within the patient's body, and is preferably fixed to body tissue including the patient's **410** interior muscle wall. The tube **402** conveys fluid to and from the inflatable portion **422**, from the access port **404**. One end of the tube **402** couples to the access port **404**, and the other end of the tube **402** couples to the inflatable portion **422** of the gastric band **408**.

[0150] A physician inserts a syringe **426** needle into the patient's body to access the access port **404**, and vary the amount of fluid in the inflatable portion **422** of the gastric band **408**. Generally, the physician must attempt to locate a septum **428** of the access port **404** to pass the syringe **426** needle through the septum **428**. The septum **428** must be penetrated by the syringe **426** needle to allow fluid to enter, or be removed from the access port **404**. The physician will typically palpate the area around the access port **404** to locate the septum **428**.

[0151] However, it may be difficult for the physician to properly locate the septum **428**, because the access port **404** may be covered by many layers of the patient's **410** fat. Accordingly, it is possible the physician may not properly locate the septum **428**, and may errantly insert the syringe **426**

needle. The physician may contact a portion of the tube **402** leading from the access port **428** to the gastric band **408**. The syringe **426** needle may puncture the tube **402**, specifically the end of the tube **402** connected to the access port **404**, and may cause fluid to leak from the gastric banding system **406**. A surgical procedure may be necessary to repair the punctured tube **402**, or replace the entire gastric banding system **406**. The needle guard assembly **414** is intended to prevent this undesirable result, by shielding the end of the tube **402** connected to the access port **404**, and protecting the tube **402** from puncture.

[0152] Figure 21 illustrates a perspective view of the access port **404**, the needle guard assembly **414**, and the tube **402** shown in Figure 20. The needle guard assembly **414** forms a sleeve that entirely encircles an outer surface of the end of the tube **402** that connects the access port **404**. Thus, the end of the tube **402** connected to the access port **404** is protected in all directions from a syringe **426** needle that has missed the septum **428**, and is headed towards the end of the tube **402**.

[0153] The needle guard assembly **414** has a similar construction as the needle guard assembly **314** discussed in relation to Figures 11-19. Namely, the needle guard assembly **414** similarly includes a layered construction of composite guards, connected with an intermediate layer of flexible, connecting material, which bonds the composite guards together. Each composite guard includes a plurality of, for example, an arrangement, array, or pattern of, puncture resistant members, and a flexible substrate having a first side on which the puncture resistant members are positioned. The puncture resistant members are made of a material resistant to puncture by a syringe needle. The flexible substrates are made of a flexible material that provides a degree of compliance for the needle guard assembly **414**. In Figure 21, the puncture resistant members **436** and the

flexible substrate **434** of an outer layer of the needle guard assembly **414** are visible.

[0154] Figure 22 illustrates a cross-sectional view of a portion of the tube **402** and the needle guard assembly **414** shown in Figure 21. The needle guard assembly **414** is shown to comprise a first composite guard **416** covered by a second composite guard **418**. The construction of the first composite guard **416** and the second composite guard **418** is similar to the respective constructions of the first composite guard **316** and the second composite guard **318**, as described in relation to Figures 11-19. Namely, the puncture resistant members **430** of the first composite guard **416** are positioned on one side of a flexible substrate **432**. The puncture resistant members **436** of the second composite guard **418** are positioned on one side of a flexible substrate **434**. Each puncture resistant member **430**, **436** is coupled to the respective flexible substrate **432**, **434**. An intermediate layer **424** is positioned between, and connects the first composite guard **416** to the second composite guard **418**. The first composite guard **416** is positioned between the second composite guard **418** and the tube **402**. The second composite guard **418** covers the first composite guard **416**.

[0155] In the embodiment shown in Figure 22, the first composite guard **416**, the second composite guard **418**, and the intermediate layer **424**, are shaped to wrap around the entirety of the outer surface of the tube **402**. The composite guards **416**, **418** each are wrapped to have a substantially cylindrical shape, or conical shape, that allows them to extend entirely around the outer surface of the tube **402**.

[0156] Similar to the positioning of the composite guards **316**, **318**, **320**, discussed in relation to Figures 11-19, the first composite guard **416** and the second composite guard **418** are positioned such that the arrangement of the puncture resistant members **436** of the second composite guard **418** is misaligned with

the arrangement of the puncture resistant members **430** of the first composite guard **416**. Thus, the composite guards **416**, **418** are arranged relative to one another such that there are no straight line open spaces, or substantial gaps, between members **430**, **436** to allow a needle or sharp implement to penetrate entirely through the needle guard assembly **414**. The puncture resistant members **436** of the second composite guard **418** cover each space between the puncture resistant members **430** of the first composite guard **416**. For example, Figure 22 illustrates a syringe needle **427a** impacting a puncture resistant member **436** of the second composite guard **418**. However, the composite guards **416**, **418** are misaligned such that if an incident syringe needle misses the puncture resistant members **436** of the second composite guard **418**, then the syringe needle will contact the puncture resistant members **430** of the first composite guard **416**. For example, Figure 22 illustrates a syringe needle **427b** passing through a space between the members **436** of the second composite guard **418**, and passing through the flexible substrate **434** of the second composite guard **418**, and through the intermediate layer **424**. Yet, the syringe needle **427b** contacts the puncture resistant member **430** of the first composite guard **416**, and does not penetrate the tube **402**.

[0157] In addition, similar to the embodiments of the needle guard assembly **314** discussed in relation to Figures 11-19, the members **436**, **430** may each have a thickness **442** of between about 0.1 millimeter (mm) and about 1.0 mm. The members **436**, **430** may each have a diameter **438** of between about 0.5 mm and about 2.0 mm, for example, a diameter of about 1.5 mm.

[0158] A space may be positioned between adjacent puncture resistant members **436**, **430**. The space may have a width **440** of between about 0.2 mm and about 0.5 mm.

[0159] The puncture resistant members **430**, **436**, similar to the members **330** discussed in relation to Figures 11-19, may be any

suitable shape. In Figure 22, the members **430**, **436** are shown to have a round shape, with a flattened, or planar shaped top, similar to the embodiment of the puncture resistant members **330a**, shown in Figure 16. In other embodiments, the members **430**, **436** may have any shape shown in Figures 15-16a, or as discussed elsewhere in this disclosure. In particular, the members **430**, **436** may have a dome shape as shown in Figure 15, or a dome shape with a flattened, or planar, upper surface, as illustrated in Figure 16a. In addition, similar to the needle guard assembly **316** discussed in relation to Figures 11-19, the needle guard assembly **414** may include between about 50 members and about 1000 members **430**, **436** per square inch (psi), for example, about 400 psi.

[0160] In one specific embodiment, each composite guard **416**, **418** may include about 400 members psi, each having a diameter of about 1.5 mm and each being spaced apart about 0.2 mm.

[0161] The needle guard assembly **414** may comprise a pre-formed sleeve that is slid over the end of the tube **402** connected to the access port **404**. The needle guard assembly **414** may then be glued to the end of the tube **402**, through an appropriate adhesive, for example, a silicone-based glue, or the like. In one embodiment, the leading end of the needle guard assembly **414** may be glued directly to the access port **404**. In one embodiment, the needle guard assembly **414** may be formed directly on the tube **402**. For example, the first composite guard **416** may be cut to the appropriate shape out of a sheet of material, shown for example, in Figure 31 or 32. The first composite guard **416** may be wrapped around the outer surface of the tube **402** and glued in place. Then, the intermediate layer **424** may be placed over the first composite guard **416**. The second composite guard **418** may be cut to size out of a similar sheet of material as the first composite guard, and then fixed to the intermediate layer **424**.

[0162] The needle guard assembly **414** may be shaped to contour to the shape of the underlying tube **402**. For example, Figure 21 illustrates the needle guard assembly **414** having a conical shape, as it conforms to the underlying conical shape of the tube **402**. In other embodiments, the needle guard assembly **414** may have any shape that produces equivalent operation, including a cylindrical shape, or a pyramidal shape, or the like.

[0163] The needle guard assembly **414** is positioned on the tube **402** such that no gap exists between the access port housing and the assembly **414**, such that a needle could not penetrate the portion of the tube **402** that is directly connected to the access port **404**. The needle guard assembly **414** thus completely protects the end of the tube **402** connected to the access port **404**. In other embodiments, the needle guard assembly **414** may only cover a portion of the tube **402**, or may not wrap entirely around the outer surface of the tube **402**. For example, the needle guard assembly **414** may be configured to only cover the uppermost portion of the tube **402**, or the portion facing the nearest surface of the patient's skin. The amount of protection offered by the needle guard assembly **414** may be varied as desired.

[0164] In the embodiment of the needle guard assembly **414** shown in Figures 21 and 22, the outer surface of the needle guard assembly **414** has a bumpy surface, caused by the spacing between the puncture resistant members **436** of the second composite guard **418**. In other embodiments, the needle guard assembly **414** may be covered by a material, for example, an elastomeric material, to smooth the surface of the needle guard assembly **414**.

[0165] The layered composition of the needle guard assembly **414** may be varied as desired. For example, the number of composite guards utilized with the needle guard assembly **414** may be varied, from two guards to four guards. In other embodiments, additional guards may be utilized, if equivalent operation

results. In one embodiment, only one composite guard may be utilized, with puncture resistant members spaced closely to each other, or close enough to block an incoming syringe needle. In addition, in other embodiments, the orientation of the composite guards may additionally be varied. For example, in one embodiment, the second composite guard **418** may be flipped such that the puncture resistant members **436** of the second composite guard **418** face the puncture resistant members **430** of the first composite guard **416**. In other words, the puncture resistant members **436** of the second composite guard **418** may be positioned on the other side of the flexible substrate **434**, than shown in Figure 22.

[0166] Figure 23 illustrates an embodiment of a needle guard assembly **514**, similar to the needle guard assembly **414** discussed in relation to Figures 20-22, which is configured to protect an end of a tube **502** connected to an access port **504**. The needle guard assembly **514** similarly blocks the passage of a syringe **526** needle that has missed contacting the septum **528** of the access port **504**. However, the layered composition of the needle guard assembly **514** differs from the composition of the needle guard assembly **414** discussed in relation to Figures 20-22. The needle guard assembly **514** shown in Figure 23 includes three composite guards, two intermediate layers, a bottom layer, and a top layer **546** that is visible in Figure 23.

[0167] Figure 24 illustrates a cross sectional view of the needle guard assembly **514**, and the tube **502** shown in Figure 23. Figure 25 shows a close up view of a portion of the needle guard assembly **514** as shown in Figure 24. Referring to both Figures 24 and 25, the needle guard assembly **514** includes a first composite guard **516**, a second composite guard **518**, and a third composite guard **520**. A first intermediate layer **524** is positioned between the first composite guard **516**, and the second composite guard **518**. A second intermediate layer **525** is

positioned between the second composite guard **518** and the third composite guard **520**. Each composite guard **516**, **518**, **520** has a similar composition as the guards forming the needle guard assemblies **314**, **414**, discussed in relation to Figures 11-22. Namely, each composite guard **516**, **518**, **520** includes an arrangement, array, or pattern of, respective puncture resistant members **530**, **536**, **550**, and a respective flexible substrate **532**, **534**, **552** having a first side on which the respective puncture resistant members **530**, **536**, **550**, are positioned, or coupled thereto. The first and second intermediate layers **524**, **525** have similar compositions as the intermediate layers **324**, **424** discussed in relations to Figures 11-22.

[0168] The composite guards **516**, **518**, **520**, each include respective puncture resistant members **530**, **536**, **550**, that do not have a space positioned between adjacent puncture resistant members. As shown in Figure 25, each of the puncture resistant members **530**, **536**, **550**, directly contacts an adjacent puncture resistant member. Yet, each composite guard **516**, **518**, **520**, is still misaligned with at least one other composite guard (e.g., the third composite guard **520** is misaligned with at least one of the first composite guard **516**, or the second composite guard **518**), to assure that no straight line open spaces, or substantial gaps, between members **530**, **536**, **550**, may exist to allow a needle or sharp implement to penetrate entirely through the assembly **514**, and contact the tube **502**. The lack of space between adjacent puncture resistant members **530**, **536**, **550**, further enhances the ability of the needle guard assembly **514** to prevent needle penetration. For example, Figure 24 illustrates syringe needles **527a**, **527b**, unable to penetrate even the outermost composite guard **520**.

[0169] The needle guard assembly **514** includes an inner or bottom layer **544** that is positioned below the first composite guard **516**. The needle guard assembly **514** includes an outer or top

layer **546** that is positioned above the third composite guard **520**. The top layer **546** and bottom layer **544** each comprise a soft elastomeric material, such as silicone. The top layer **546** and the bottom layer **544** may connect at an end **548** of the layers **546**, **544**, to enclose the composite guards **516**, **518**, **520**, and the intermediate layers **524**, **525**, and to provide a fluid tight barrier for the interior of the needle guard assembly **514**.

[0170] Aside from the additional top layer **546**, the bottom layer **544**, the second intermediate layer **525**, the third composite guard **520** and the spacing of the puncture resistant members **530**, **536**, **550**, the needle guard assembly **514** includes similar construction as the needle guard assembly **414** discussed in relation to Figures 20-22. Namely, the thickness and the diameter of the puncture resistant members **530**, **536**, **550**, may be the same as the members of the needle guard assembly **414** discussed in relation to Figures 20-22. In addition, the shape and the amount of the puncture resistant members **530**, **536**, **550** on the needle guard assembly **514**, may be the same as for the members of the needle guard assembly **414** discussed in relation to Figures 20-22. In addition, the sleeve shape of the needle guard assembly **514**, and the position of the needle guard assembly **514** along the tube **502**, may be the same as for the needle guard assembly **414** discussed in relation to Figures 20-22.

[0171] Although the needle guard assembly **514** is shown without any space between adjacent puncture resistant members **530**, **536**, **550**, in one embodiment, the puncture resistant members **530**, **536**, **550**, may include spaces, and the spaces may be sized the same as for the members of the needle guard assembly **414** discussed in relation to Figures 20-22. In addition, the construction of the needle guard assembly **514** as a pre-formed sleeve, or as a series of layers formed directly on the tube **502**, may be identical to the construction of the needle guard assembly **414** discussed in

relation to Figures 20-22. The three-composite layers preferably enhance the protection offered by the needle guard assembly **514**. The three composite guard layers provide increased protection for the tube **502** from needle puncture compare to the two composite guards and/or the needle guard assembly **414** discussed in relation to Figures 20-22.

[0172] The needle guard assemblies **414**, **514**, discussed in relation to Figures 20-25, beneficially provide a flexible protective material over an end of the respective tubes **402**, **502**. The needle guard assemblies **414**, **514** may each also have a resiliency or a shape memory such that it will restore it to a particular shape after being manipulated by a physician. This may be provided by using a suitable intermediate layer material, such as a silicone elastomer that has a shape memory characteristic. The flexibility of each of the needle guard assemblies **414**, **514** may reduce discomfort for the patient upon insertion of the respective access ports **404**, **504**. In addition, the flexibility of each of the needle guard assemblies **414**, **514**, may allow a physician to more easily position the respective access port **404**, **504**, and the tube **402**, **502**, within a patient's body during implantation.

[0173] The needle guard assemblies **414**, **514**, discussed in relation to Figures 20-25, may be utilized with access ports that are not part of the gastric banding systems. Although a gastric banding system is one intended embodiment of the present invention, the needle guard assemblies **414**, **514** may be used to protect tubing attached to any implantable access port, including, but not limited to, a drug eluting access port, an access port used to control the pressure of a urinary restriction device, or anal incontinence device, or the like. The needle guard assemblies **414**, **514** may be used in any implantable medical device utilizing an access port, and having a component that requires protection from puncture.

[0174] The puncture resistant members **430, 436, 530, 536, 550** shown in Figures 20-25 may be made of a similar puncture resistant material as the puncture resistant members **330** (and **330a** and **330b**) discussed in relation to Figures 11-19. Namely, the members **430, 436, 530, 536, 550** are made of a suitable puncture resistant material, such as an epoxy, acrylic materials, hot-melt adhesives, thermoplastics, polymer, rubber, ceramic or metal, or suitable combination or alloy thereof. For some applications, suitable materials include polyethylene (PE), polypropylene (PP), polyurethane (PU), polyethylene terephthalate (PET), polycarbonate (PC), polyisoprene (PI), thermoplastic urethanes and thermoplastic polyurethanes (TPU), high durometer silicones, acrylonitrile butadiene styrene (ABS) etc. In some embodiments, the members **430, 436, 530, 536, 550** may be made from a UV-curable epoxy. In some embodiments, the members **430, 436, 530, 536, 550** are made of a material such as acetal, nylon, polycarbonate, and combinations thereof. In some embodiments, the members **430, 436, 530, 536, 550** are made of a metal, for example, stainless steel, aluminum, titanium, or other metal.

[0175] The flexible substrates **432, 434, 532, 534, 552** shown in Figures 20-25 may be made of a similar flexible material as the flexible substrate **332** discussed in relation to Figures 11-19. Namely, the flexible substrates **432, 434, 532, 534, 552** may comprise a mesh, film, fabric, elastomer, or other suitable material. The flexible substrates **432, 434, 532, 534, 552** may be made from thin polyimide, polyester, or other biocompatible film with appropriate thickness. The flexible substrates **432, 434, 532, 534, 552** may be made from silicone, polyurethane, or other foam materials. The flexible substrates **432, 434, 532, 534, 552** may be made from woven or non-woven mesh materials such as Nylon or Polyester. In one embodiment, the flexible substrates **432, 434, 532, 534, 552** may be made from Kapton film.

In one embodiment, the flexible substrates **432**, **434**, **532**, **534**, **552** may be made from a polymer foam or plastic film.

[0176] The intermediate layers **424**, **524**, **525** shown in Figures 20-25 may be made of a similar material as the intermediate layers **324** discussed in relation to Figures 11-19. Namely, the intermediate layers **424**, **524**, **525** may be a polymer, for example, an elastomeric material, such as an elastomeric polymer, for example, a silicone elastomer, for example, a low durometer silicone rubber. The intermediate layers **424**, **524**, **525** may comprise a soft, tacky layer of elastomeric material, generally comprised of silicone. The top layer **546** and the bottom layer **544** shown in Figures 24 and 25 may be made of similar materials discussed above for the intermediate layers **424**, **524**, **525**.

[0177] All materials used to form the needle guard assemblies **414**, **514** may be biocompatibility rated at USP Class VI. In addition, an encapsulating layer of an elastomeric material, forming a top layer **546** and a bottom layer **544** may be a grade of silicone designed for long term implantation (e.g., 5 or more years of implantation).

[0178] Figure 26 illustrates a needle guard assembly **614** utilized in conjunction with a clip **652**. The needle guard assembly **614** may be configured similarly as the needle guard assembly **514** shown and discussed in relation to Figures 23-25. In particular, the needle guard assembly **614** may comprise a layered assembly of composite guards and intermediate layers. The needle guard assembly **614** may include a first composite guard, a second composite guard, and a third composite guard that each have similar compositions as the respective first composite guard **516**, the second composite guard **518**, and the third composite guard **520** shown in Figures 24 and 25. Namely, the first composite guard, the second composite guard, and the third composite guard of the needle guard assembly **614** may include an arrangement, array, or pattern of, respective

puncture resistant members, and a respective flexible substrate having a first side on which the respective puncture resistant members are positioned, or coupled thereto.

[0179] The needle guard assembly **614**, similarly as the needle guard assembly **514** discussed in relation to Figures 23-25, may also include a top layer **646**, a bottom layer, an intermediate layer between a first composite guard and a second composite guard, and an intermediate layer between a second composite guard and a third composite guard. The layers of the needle guard assembly **614** may have similar compositions as the respective top layer **546**, bottom layer **544**, and intermediate layers **524**, **525** shown and described in relation to Figures 23-25. The outer surface of the top layer **646** is visible in Figure 26.

[0180] The needle guard assembly **614** shown in Figure 26 forms a sleeve that extends partially around the outer surface of the tube **602**. The needle guard assembly **614** covers the upper, or top surface of the tube **602**, and the sides of the tube **602**.

[0181] The clip **652** includes a sleeve portion **654** and a mounting portion **656**. The sleeve portion **654** is a portion of the clip **652** that extends over, and overlays, the needle guard assembly **614**. The sleeve portion **654** secures the needle guard assembly **614** to the end of the tube **602** connected to the access port **604**. In the embodiment shown in Figure 26, the sleeve portion includes a plurality of ribs **662** separated by slots **664**. Each rib **662** and each slot **664** extends transverse to the length of the tube **602**. The ribs **662** of the sleeve portion **654** overlay the needle guard assembly **614**. The slots **664** separate the ribs **662** and provide flexibility for the sleeve portion **654**.

[0182] The mounting portion **656** of the clip **652** couples the sleeve portion **654** to the access port **604**. In the embodiment shown in Figure 26, the mounting portion **656** comprises a substantially flattened, or planar portion, of the clip **652** that

extends beneath the access port **604**, to mount to suture holes **666** (shown in Figure 28) in the access port **604**. The mounting portion **656** includes a plurality of posts **660** that extend vertically from an upper surface of the mounting portion **656**, to pass through the access port **604** suture holes. The posts **660** secure the clip **652** to the access port **604** via a friction fit between the posts **660** and the access port **604** suture holes. The clip **652** may additionally include suture holes **658** that extend outward or radially from the mounting portion **656** of the clip **652**. The suture holes **658** are configured to allow a user to secure the access port **604** to a portion of a patient's body, in lieu of the suture holes extending through the access port **604** itself.

[0183] Figure 27 illustrates a perspective view of the clip **652** separated from the access port **604**. The mounting portion **656** of the clip **652** is shown to comprise a substantially flattened surface **668** configured to abut a bottom surface of the access port **604**. In addition, the posts **660** are shown to extend from the surface **668** of the clip **652**, and being positioned on the surface **668** to mate with corresponding suture holes **666** of the access port **604**, shown in Figure 28. Figure 27 additionally illustrates an aperture **670** positioned in the center of the mounting portion **656**. The mounting portion **656** forms a flattened ring around the aperture **670**.

[0184] Figure 28 illustrates a bottom view of the clip **652** separated from the access port **604**. The access port **604** includes a substantially flat bottom surface **672** that abuts the substantially flattened surface **668** of the clip **652**, shown in Figure 27.

[0185] Referring to Figures 26-28, the clip **652** may be removably secured to the access port **604**. The posts **660** of the clip **652** may be slidably removable from the suture holes **666** of the access port **604**, such that the entire clip **652** may be removed

from the access port **604**. To install the clip **652** onto the access port **604** from an initially separated configuration, the tube **602** may be initially passed through the aperture **670** of the clip **652**. Then, once the clip **652** nears the access port **604**, the clip **652** may be rotated such that the posts **660** pass through the suture holes **666** of the access port **604**. As the posts **660** enter the suture holes **666**, the tube **602** will enter the cavity formed by the sleeve portion **654** of the clip **652**. The posts **660** secure the clip **652** against the access port **604**. The clip **652** secures the needle guard assembly **614** to the tube **602**. To remove the clip **652** from the access port **604**, the installation process is reversed.

[0186] The clip **652** beneficially serves to secure the needle guard assembly **614** against the end of the tube **602** that is coupled to the access port **604**. The clip **652** presses the needle guard assembly **614** against the outer surface of the tube **602** to secure the assembly **614** in position on the tube **602**. Thus, the needle guard assembly **614** does not need to be directly adhered to the tube **602**, or form a sleeve extending entirely around the outer surface of the tube **602**. The clip **652** may press-fit the needle guard assembly **614** in place against the tube **602**.

[0187] The sleeve portion **654** of the clip **652** is preferably made flexible to accommodate movement of the needle guard assembly **614**. The slots **664** separating the ribs **662** of the sleeve portion **654** provide flexibility for the sleeve portion **654** by removing material between the ribs **662**. In addition, the slots **664** reduce the total weight of the clip **652**.

[0188] The clip **652** additionally serves as an additional protective layer over the needle guard assembly **614**. The clip **652** may be made of a needle-impenetrable material such as plastic. If an incident needle misses the septum **628** of the access port **604** and contacts the clip **652**, then the clip **652** may

block movement of the incident needle, and prevent the needle from puncturing the tube **602**.

[0189] The clip **652** may be configured in a variety of shapes designed to equivalently secure the needle guard assembly **614** in position on the tube **602**. In one embodiment, the sleeve portion **654** of the clip **652** may be a substantially solid sleeve that does not include ribs **662** or slots **664**. In one embodiment, the sleeve portion **654** may include slots **664** that extend lengthwise along the tube **602**. In one embodiment, the mounting portion **656** of the clip **652** may extend over a top surface of the access port **604** or wrap around an outer surface of the access port **604**. In one embodiment, the clip **652** may be configured as any device capable of securing a needle guard assembly in position on tubing.

[0190] The clip **652** is preferably made of a needle-impenetrable, yet flexible material such as plastic. Other equivalent materials, capable of securing the needle guard assembly **614** in position to the tube **602** may also be utilized.

[0191] In one embodiment, the clip **652** is adhered to the access port **604**. In this embodiment, the posts **660** may be adhered to the suture holes **666** of the access port **604** with a suitable biocompatible adhesive. In addition, in one embodiment, a suitable biocompatible adhesive may be positioned on the upper surface **668** of the clip **652**, to adhere the clip **652** to a bottom surface **672** of the access port **604**.

[0192] In one embodiment, the needle guard assembly **614** may be directly adhered to the clip **652**.

[0193] Figure 29 illustrates a needle guard assembly **714** having a flanged portion **770** extending from a sleeve portion **772** of the needle guard assembly **714**. The needle guard assembly **714** may be configured similarly as the needle guard assembly **514** shown and discussed in relation to Figures 23-25. In particular, the

needle guard assembly **714** may comprise a layered assembly of composite guards and intermediate layers. The needle guard assembly **714** may include a first composite guard, a second composite guard, and a third composite guard that each have similar compositions as the respective first composite guard **516**, the second composite guard **518**, and the third composite guard **520** shown in Figures 24 and 25. Namely, the first composite guard, the second composite guard, and the third composite guard of the needle guard assembly **714** may include an arrangement, array, or pattern of, respective puncture resistant members, and a respective flexible substrate having a first side on which the respective puncture resistant members are positioned, or coupled thereto.

[0194] The needle guard assembly **714**, similarly as the needle guard assembly **514** discussed in relation to Figures 23-25, may also include a top layer **746**, a bottom layer, an intermediate layer between a first composite guard and a second composite guard, and an intermediate layer between a second composite guard and a third composite guard. The layers of the needle guard assembly **714** may have similar compositions as the respective top layer **546**, bottom layer **544**, and intermediate layers **524**, **525** shown and described in relation to Figures 23-25. The outer surface of the top layer **746** is visible in Figure 29.

[0195] The sleeve portion **772** of the needle guard assembly **714** is shaped to substantially contour to the shape of the tube **702**. In the embodiment shown in Figure 29, the sleeve portion **772** does not extend entirely around the outer surface of the tube **702**, but only extends over the top of the tube **702** and the sides of the tube **702**. A flanged portion **770** of the needle guard assembly **714** extends outward from the sleeve portion **772**. A part of the flanged portion **770** may extend beneath the access port **704**, to adhere to the bottom of the access port **704**.

[0196] The access port **704** may be fixed to a portion of the patient's body by use of the suture holes **760** on the access port **704**. The needle guard assembly **714** may include suture holes (shown in Figure 30) that correspond to the location of the access port's **704** suture holes **760**.

[0197] Figure 30 illustrates the needle guard assembly **714** separated from the access port **704**. The upper surface **774** of the needle guard assembly **714**, which fixes to the access port **704**, is visible. In addition, an aperture **776** in the needle guard assembly **714** is visible. The suture holes **761** in the flanged portion **770** of the needle guard assembly **714**, which correspond to the suture holes **760** of the access port **704**, are visible.

[0198] To secure the needle guard assembly **714** to the access port **704** from an initially separated configuration, as shown in Figure 30, the tube **702** may be initially passed through the aperture **776** of the needle guard assembly **714**. Then, once the needle guard assembly **714** nears the access port **704**, the upper surface **774** of the needle guard assembly **714** may be adhered to the access port **704**. The adhesive may be a soft, biocompatible silicone rubber material, such as Nusil MED-4805, or 4810, or the like. The adhesive may be applied to the entire surface of the needle guard assembly **714** and may act as a bonding agent to the access port **704** while curing.

[0199] The sleeve portion **772** of the needle guard assembly **714** is positioned above the tube **702**, to prevent incident needles from puncturing the tube **702**. The flanged portion **770** of the needle guard assembly **714** is positioned above a portion of the patient's body tissue, to prevent incident needle from penetrating the patient's body tissue. As discussed above, the access port **704** is preferably fixed to tissue such as a patient's muscle wall. If an incident needle missed the septum **728** and penetrated the patient's muscle wall, the patient would

likely experience great pain. The flanged portion **770** of the needle guard assembly **714** protects the patient's muscle wall from incident needle penetration. The flanged portion **770** additionally serves to strengthen the needle guard assembly **714**, and to serve as an attachment structure for the needle guard assembly **714** to the access port **704**.

[0200] The needle guard assembly **714** may be configured in a variety of shapes designed to equivalently protect the tube **702** from puncture. In one embodiment, the flanged portion **770** may have a curved shape, or any variety of equivalent shapes extending from a sleeve portion **772** of the needle guard assembly **714**. In one embodiment, the flanged portion **770** may extend over a top surface of the access port **704** or wrap around an outer surface of the access port **704**. In one embodiment, the needle guard assembly **714** may have any equivalent shape capable of protecting the tube **702** from puncture.

[0201] The composite guards **416, 418, 516, 518, 520** shown in Figures 20-25, or discussed in relation to Figures 26-30, may be formed in a similar manner as the guards **316** discussed in relation to Figures 11-19. For example, the composite guards **416, 418, 516, 518, 520** may be formed by a suitable method, including stencil printing, for example, using equipment and processes used in surface mount technology/PCB fabrication. Other processes that can be used to make the composite guards **416, 418, 516, 518, 520** include micro-dot dispensing and printing, laser etching, and stencil printing. For example, a uniform film of a hard encapsulant may be applied on the flexible substrate and etched with laser etching/engraving equipment to achieve a desired pattern. Other suitable methods will be known to those of skill in the art. Referring to Figures 31 and 32, the composite guards **816, 916** are initially formed in the shape of generally flat sheets. The formation methods result in composite guards **816, 916** with puncture

resistant members bonded to the flexible substrates. A composite guard **416**, shown in Figure 22, for example, will then be cut from the sheets to the appropriate shape, as desired.

[0202] In addition, the intermediate layers **424**, **524**, **525** shown in Figures 20-25, or discussed in relation to Figures 26-30 may be formed in a similar manner as the intermediate layers **324** discussed in relation to Figures 11-19, and as specifically shown in Figures 17-19. For example, a suitable material for the intermediate layer **424**, **524**, **525**, for example, a sheet of uncured silicone, is placed on one side of the respective composite guard **416**, **418**, **516**, **518**, **520**, for example, on the side having the respective puncture resistant members **430**, **436**, **530**, **536**, **550**. The sheet is then subjected to curing conditions to cause the sheet to adhere to the respective puncture resistant members **430**, **436**, **530**, **536**, **550**, forming respective intermediate layer **424**, **524**, **525** thereon. Such curing conditions may include placement of the sheet in an oven. In an embodiment in which the needle guard assemblies **414**, **514** are formed directly on the respective tubes **402**, **502**, the composite guards **416**, **418**, **516**, **518**, **520** and the intermediate layers **424**, **524**, **525** may be placed on the respective tubes **402**, **502** prior to the curing step. In an embodiment including a bottom layer **544** and/or a top layer **546**, the bottom layer **544** and/or the top layer **546** may be appropriately positioned on the tube **502** prior to curing. The methods of forming composite guards **816**, **916** may additionally be used to form the composite guards discussed in relation to Figures 33-38.

[0203] Figure 33 illustrates an embodiment of a composite guard **1016** including registration holes **1072** extending through the surface of the composite guard **1016**. The composite guard **1016** may have a similar composition as the respective first composite guard **516** shown in Figures 24 and 25. Namely, the composite guard **1016** may include an arrangement, array, or pattern of,

respective puncture resistant members **1030**, and a respective flexible substrate **1032** having a first side on which the respective puncture resistant members **1030** are positioned, or coupled thereto.

[0204] The registration holes **1072** are positioned on the composite guard **1016** in a manner such that the arrangement of puncture resistant members **1030** on the flexible substrate **1032** is misaligned with the arrangement of puncture resistant members of at least one other composite guard. Figure 34 illustrates an embodiment in which three composite guards are utilized to form a needle guard assembly. The first composite guard **1016** is utilized in combination with a second composite guard **1018**, and a third composite guard **1020**. The second composite guard **1018** and the third composite guard **1020** may have a similar composition as the respective second composite guard **518**, and the third composite guard **520** shown in Figures 24 and 25. Namely, the composite guards **1018**, **1020** may each include an arrangement, array, or pattern of, respective puncture resistant members, and a respective flexible substrate having a first side on which the respective puncture resistant members are positioned, or coupled thereto.

[0205] The second composite guard **1018** and the third composite guard **1020** include respective registration holes **1074**, **1076**. The position of the registration holes **1072** of the first composite guard **1016** corresponds to the position of the registration holes **1076** of the third composite guard **1020**, such that the arrangement of puncture resistant members of the first composite guard **1016** is aligned with the arrangement of puncture resistant members of the third composite guard **1020**. The position of the registration holes **1072** of the first composite guard **1016** corresponds to the position of the registration holes **1074** of the second composite guard **1018**, such that the arrangement of puncture resistant members of the first composite

guard **1016** is misaligned, or offset, with the arrangement of puncture resistant members of the second composite guard **1018**. The puncture resistant members of the first composite guard **1016** are misaligned, or offset, with the arrangement of puncture resistant members of the second composite guard **1018** by half the distance between two adjacent puncture resistant members.

[0206] A frame **1078** is passed through the registration holes **1072, 1074, 1076** of the respective first composite guard **1016**, the second composite guard **1018**, and the third composite guard **1020** to maintain the puncture resistant members in position relative to each other during construction of the needle guard assembly. The frame **1078** includes pins **1082** and arms **1080** connecting the pins **1082**. The pins **1082** extend through the registration holes **1072, 1074, 1076** to maintain the misalignment between the first composite guard **1016** and the second composite guard **1018**. The frame **1078** may be thin, and flexible, and made out of a biocompatible grade plastic, such as PEEK or PolySulfone, or PolyPhenylSulfide, or the like. The frame **1078** may additionally be made of a thin metal such as titanium, or stainless steel, or the like.

[0207] Figures 35 and 36 illustrates perspective views of the first composite guard **1016**, the second composite guard **1018**, and the third composite guard **1020** after the pins **1082** have passed through the respective registration holes **1072, 1074, 1076** (shown in Figure 34). Figure 36 illustrates a bottom perspective view of the composite guards **1016, 1018, 1020** with the frame **1078** abutting a bottom surface, or side, of the third composite guard **1016**.

[0208] Once the composite guards **1016, 1018, 1020** are in position relative to each other, with the frame **1078** extending through the registration holes **1072, 1074, 1076** (shown in Figure 34), then an overmolding of an elastomeric material may be formed over the composite guards **1016, 1018, 1020** and the frame

1078. Figure 37 illustrates a needle guard assembly **1014** formed after the overmolding of an elastomeric material. The overmolding entirely encapsulates the composite guards **1016**, **1018**, **1020** and the frame **1078**, visible in Figure 38. The overmolding forms a top layer **1046**, a bottom layer **1044** and an enclosing side end **1048** of elastomeric material.

[0209] Figure 38 illustrates a detail view of the needle guard assembly **1014** shown in Figure 37. The puncture resistant members **1030** and the flexible substrate **1032** of the first composite guard **1016** are shown in a layered configuration below the puncture resistant members **1036** and the flexible substrate **1034** of the second composite guard **1018**, and the puncture resistant members **1050** and the flexible substrate **1052** of the third composite guard **1020**. The frame **1078** extending through the composite guards **1016**, **1018**, **1020** maintains the misalignment between the first composite guard **1016** and the second composite guard **1018**. The frame **1078** additionally maintains the alignment between the first composite guard **1016** and the third composite guard **1020**.

[0210] The top layer **1046** and the bottom layer **1044** of the overmolding of the elastomeric material each form an outer surface of the needle guard assembly **1014**. The overmolding of elastomeric material additionally forms a first intermediate layer **1024** between the first composite guard **1016** and the second composite guard **1018**, and forms a second intermediate layer **1025** between the second composite guard **1018** and the third composite guard **1020**.

[0211] The overmolding of elastomeric material may encapsulate the frame **1078**. The frame **1078** may remain bonded to the composite guards **1016**, **1018**, **1020**, such that when the needle guard assembly **1014** is implanted for use within a patient's body, the frame **1078** retains the relative positions of the composite guards **1016**, **1018**, **1020**. In an embodiment in which

the needle guard assembly **1014** is shaped to contour to the shape of a tube, for example a tube **502** shown in Figure 23, the frame **1078** may be made sufficiently flexible to allow the needle guard assembly **1014** to wrap around the tube **502**. In one embodiment, the frame **1078** may be removed from the assembly **1014** before the encapsulating layer is formed around the composite guards **1016**, **1018**, **1020**. In this embodiment, the bonding of the encapsulating layer retains the relative positions of the composite guards **1016**, **1018**, **1020**. The elastomeric material may comprise silicone, or the equivalent.

[0212] The needle guard assembly **1014** may be utilized as a needle guard, to protect a tubing from puncture, in the manner discussed in relation to Figures 20-25. The needle guard assembly **1014** may be utilized in combination with a clip **652**, as shown in relation to Figures 26-28, or may be shaped to include a flanged portion, for example the flanged portion **770**, shown in Figures 29-30. In one embodiment, the needle guard assembly **1014** may be utilized to protect an implantable device **310**, for example the implantable device **310** shown and discussed in relation to Figures 11-12.

[0213] The puncture resistant members **1030**, **1036**, **1050** shown in Figures 33-38 may be made of a similar puncture resistant material as the puncture resistant members **430**, **436**, **530**, **536**, **550** discussed in relation to Figures 20-25. Namely, the members **1030**, **1036**, **1050** are made of a suitable puncture resistant material, such as an epoxy, acrylic materials, hot-melt adhesives, thermoplastics, polymer, rubber, ceramic or metal, or suitable combination or alloy thereof. For some applications, suitable materials include polyethylene (PE), polypropylene (PP), polyurethane (PU), polyethylene terephthalate (PET), polycarbonate (PC), polyisoprene (PI), thermoplastic urethanes and thermoplastic polyurethanes (TPU), high durometer silicones, acrylonitrile butadiene styrene (ABS) etc. In some embodiments,

the members **1030, 1036, 1050** may be made from a UV-curable epoxy. In some embodiments, the members **1030, 1036, 1050** are made of material such as acetal, nylon, polycarbonate, and combinations thereof. In some embodiments, the members **1030, 1036, 1050** are made of a metal, for example, stainless steel, aluminum, titanium, or other metal.

[0214] The flexible substrates **1032, 1034, 1052** shown in Figures 33-38 may be made of a similar flexible material as the flexible substrates **432, 434, 532, 534, 552** discussed in relation to Figures 20-25. Namely, the flexible substrates **1032, 1034, 1052** may comprise a mesh, film, fabric, elastomer, or other suitable material. The flexible substrates **1032, 1034, 1052** may be made from thin polyimide, polyester, or other biocompatible film with appropriate thickness. The flexible substrates **1032, 1034, 1052** may be made from silicone, polyurethane, or other foam materials. The flexible substrates **1032, 1034, 1052** may be made from woven or non-woven mesh materials such as Nylon or Polyester. In one embodiment, the flexible substrates **1032, 1034, 1052** may be made from Kapton film. In one embodiment, the flexible substrates **1032, 1034, 1052** may be made from a polymer foam or plastic film.

[0215] The intermediate layers **1024, 1025** shown in Figures 37-38 may be made of a similar material as the intermediate layers **424, 524, 525** discussed in relation to Figures 20-25. Namely, the intermediate layers **1024, 1025** may be a polymer, for example, an elastomeric material, such as an elastomeric polymer, for example, a silicone elastomer, for example, a low durometer silicone rubber. The intermediate layers **1024, 1025** may comprise a soft, tacky layer of elastomeric material, generally comprised of silicone. The top layer **1046** and the bottom layer **1044** shown in Figures 37 and 38 may be made of similar materials discussed above for the intermediate layers **1024, 1025**.

[0216] All materials used to form the needle guard assembly **1014** may be biocompatibility rated at USP Class VI. In addition, the encapsulating layer of an elastomeric material, forming a top layer **1046** and a bottom layer **1044** may be a grade of silicone designed for long term implantation (e.g., 5 or more years of implantation).

[0217] Unless otherwise indicated, all numbers expressing quantities of ingredients, volumes of fluids, and so forth used in the specification and claims are to be understood as being modified in all instances by the term "about." Accordingly, unless indicated to the contrary, the numerical parameters set forth in the specification and attached claims are approximations that may vary depending upon the desired properties sought to be obtained by the present invention. At the very least, and not as an attempt to limit the application of the doctrine of equivalents to the scope of the claims, each numerical parameter should at least be construed in light of the number of reported significant digits and by applying ordinary rounding techniques. Notwithstanding that the numerical ranges and parameters setting forth the broad scope of the invention are approximations, the numerical values set forth in the specific examples are reported as precisely as possible. Any numerical value, however, inherently contains certain errors necessarily resulting from the standard deviation found in their respective testing measurements.

[0218] The terms "a," "an," "the" and similar referents used in the context of describing the invention (especially in the context of the following claims) are to be construed to cover both the singular and the plural, unless otherwise indicated herein or clearly contradicted by context. Recitation of ranges of values herein is merely intended to serve as a shorthand method of referring individually to each separate value falling within the range. Unless otherwise indicated herein, each

individual value is incorporated into the specification as if it were individually recited herein. All methods described herein can be performed in any suitable order unless otherwise indicated herein or otherwise clearly contradicted by context. The use of any and all examples, or exemplary language (e.g., "such as") provided herein is intended merely to better illuminate the invention and does not pose a limitation on the scope of the invention otherwise claimed. No language in the specification should be construed as indicating any non-claimed element essential to the practice of the invention.

[0219] Groupings of alternative elements or embodiments of the invention disclosed herein are not to be construed as limitations. Each group member may be referred to and claimed individually or in any combination with other members of the group or other elements found herein. It is anticipated that one or more members of a group may be included in, or deleted from, a group for reasons of convenience and/or patentability. When any such inclusion or deletion occurs, the specification is deemed to contain the group as modified thus fulfilling the written description of all Markush groups used in the appended claims.

[0220] Certain embodiments of this invention are described herein, including the best mode known to the inventors for carrying out the invention. Of course, variations on these described embodiments will become apparent to those of ordinary skill in the art upon reading the foregoing description. The inventor expects skilled artisans to employ such variations as appropriate, and the inventors intend for the invention to be practiced otherwise than specifically described herein. Accordingly, this invention includes all modifications and equivalents of the subject matter recited in the claims appended hereto as permitted by applicable law. Moreover, any combination of the above-described elements in all possible

variations thereof is encompassed by the invention unless otherwise indicated herein or otherwise clearly contradicted by context.

[0221] Furthermore, certain references have been made to patents and printed publications throughout this specification. Each of the above-cited references and printed publications are individually incorporated herein by reference in their entirety.

[0222] Specific embodiments disclosed herein may be further limited in the claims using consisting of or and consisting essentially of language. When used in the claims, whether as filed or added per amendment, the transition term "consisting of" excludes any element, step, or ingredient not specified in the claims. The transition term "consisting essentially of" limits the scope of a claim to the specified materials or steps and those that do not materially affect the basic and novel characteristic(s). Embodiments of the invention so claimed are inherently or expressly described and enabled herein.

[0223] In closing, it is to be understood that the embodiments of the invention disclosed herein are illustrative of the principles of the present invention. Other modifications that may be employed are within the scope of the invention. Thus, by way of example, but not of limitation, alternative configurations of the present invention may be utilized in accordance with the teachings herein. Accordingly, the present invention is not limited to that precisely as shown and described.

CLAIMS**WHAT IS CLAIMED IS:**

1. An implantable medical device for the treatment of obesity comprising:

an access port configured to attach to body tissue;

a tube having a first end and a second end, the first end coupled to the access port; and

a needle guard assembly covering the first end of the tube, the needle guard assembly including:

a first composite guard and a second composite guard, each composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members are positioned,

the second composite guard covering the first composite guard, and

the first composite guard and the second composite guard being positioned such that the arrangement of puncture resistant members of the second composite guard is misaligned with the arrangement of puncture resistant members of the first composite guard.

2. The implantable device of claim 1 wherein the needle guard assembly is a sleeve that entirely encircles an outer surface of the first end of the tube.

3. The implantable device of claim 1 further comprising:

a first intermediate layer made of an elastomeric material, and positioned between and connecting the first composite guard with the second composite guard;

a bottom layer made of an elastomeric material, the first composite guard being positioned between the bottom layer and the first intermediate layer;

a third composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members of the third composite guard are positioned, the arrangement of puncture resistant members of the third composite guard being misaligned with the arrangement of puncture resistant members of at least one of the second composite guard or the first composite guard;

a second intermediate layer made of an elastomeric material, and positioned between and connecting the second composite guard and the third composite guard; and

a top layer made of an elastomeric material, the top layer forming an outer surface of the needle guard assembly and being positioned such that the third composite guard is between the top layer and the second intermediate layer.

4. The implantable device of claim 3 wherein the bottom layer, the first intermediate layer, the second intermediate layer, and the top layer, are each made of implantable grade silicone.

5. The implantable device of claim 1 wherein each puncture resistant member of the first composite guard directly contacts an adjacent puncture resistant member of the first composite guard.

6. The implantable device of claim 1 wherein a space is positioned between each puncture resistant member of the first composite guard and an adjacent puncture resistant member of the first composite guard, and

a space is positioned between each puncture resistant member of the second composite guard and an adjacent puncture resistant member of the second composite guard.

7. The implantable device of claim 6 wherein the arrangement of puncture resistant members of the second composite guard is misaligned with the arrangement of puncture resistant members of the first composite guard, such that the puncture resistant members of the second composite guard cover each space positioned between each puncture resistant member of the first composite guard and the adjacent puncture resistant member of the first composite guard.

8. The implantable device of claim 6 wherein each space positioned between each puncture resistant member of the first composite guard and the adjacent puncture resistant member of the first composite guard, and each space positioned between each puncture resistant member of the second composite guard and the adjacent puncture resistant member of the second composite guard, has a size of between about 0.1 millimeter and about 1.0 millimeter.

9. The implantable device of claim 1 wherein each of the puncture resistant members of the first composite guard, and each of the puncture resistant members of the second composite guard, are made from a material selected from a group consisting of epoxy, acrylic, hot-melt adhesive, thermoplastic, polymer, rubber, ceramic, metal, and combinations thereof.

10. The implantable device of claim 1 wherein the flexible substrate of the first composite guard, and the flexible substrate of the second composite guard, are each made from a material selected from a group consisting of a mesh, a film, a fabric, an elastomer, and combinations thereof.

11. The implantable device of claim 1 wherein the puncture resistant members of the first composite guard, and the puncture resistant members of the second composite guard, each have a

shape selected from a group consisting of a dome shape, a planar shape, and combinations thereof.

12. The implantable device of claim 1 wherein each of the puncture resistant members of the first composite guard, and each of the puncture resistant members of the second composite guard, has a thickness of between about 0.1 millimeter and about 1.0 millimeter.

13. The implantable device of claim 1 wherein each of the puncture resistant members of the first composite guard, and each of the puncture resistant members of the second composite guard, has a diameter of between about 0.5 millimeter and about 2.0 millimeters.

14. The implantable device of claim 1 further comprising a clip covering the needle guard assembly and securing the needle guard assembly to the first end of the tube.

15. The implantable device of claim 14 wherein the clip is secured to the access port.

16. The implantable device of claim 1 wherein the needle guard assembly is secured to an outer surface of the access port.

17. The implantable device of claim 1 wherein the first composite guard and the second composite guard each include registration holes, and

the needle guard assembly further comprises a frame extending through the registration holes of the first composite guard and the second composite guard to retain the arrangement of puncture resistant members of the second composite guard in a

misaligned position relative to the arrangement of puncture resistant members of the first composite guard.

18. A needle guard assembly for protecting an implantable tube coupled to an implantable access port, the needle guard assembly comprising:

a first composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members of the first composite guard are positioned;

a second composite guard including an arrangement of puncture resistant members and a flexible substrate having a first side on which the puncture resistant members of the second composite guard are positioned; and

a layer of elastomeric material forming an outer surface of the needle guard assembly,

the first composite guard, the second composite guard, and the layer of elastomeric material being layered relative to each other, and the first composite guard and the second composite guard being layered such that the arrangement of puncture resistant members of the second composite guard is misaligned with the arrangement of puncture resistant members of the first composite guard.

19. The needle guard assembly of claim 18 wherein the first composite guard and the second composite guard each include registration holes, and

the needle guard assembly further comprises a frame extending through the registration holes of the first composite guard and the second composite guard to retain the arrangement of puncture resistant members of the second composite guard in a misaligned position relative to the arrangement of puncture resistant members of the first composite guard.

20. The needle guard assembly of claim 18 wherein the layer of elastomeric material is part of an overmolding of the elastomeric material that encompasses the first composite guard and the second composite guard.

21. The needle guard assembly of claim 18 wherein the elastomeric material is implantable grade silicone.

22. The implantable device of claim 18 wherein each of the puncture resistant members of the first composite guard, and each of the puncture resistant members of the second composite guard, are made from a material selected from a group consisting of epoxy, acrylic, hot-melt adhesive, thermoplastic, polymer, rubber, ceramic, metal, and combinations thereof.

23. The implantable device of claim 18 wherein the flexible substrate of the first composite guard, and the flexible substrate of the second composite guard, are each made from a material selected from a group consisting of a mesh, a film, a fabric, an elastomer, and combinations thereof.

24. A gastric banding system for the treatment of obesity comprising:

- a gastric band configured to form a loop around a portion of a patient's stomach to form a stoma;

- an access port configured to attach to body tissue;

- a tube having a first end and a second end, the first end coupled to the access port, and the second end coupled to the gastric band; and


- a needle guard assembly covering the first end of the tube, the needle guard assembly including:

- a first composite guard and a second composite guard, each composite guard including an arrangement of puncture resistant members and a flexible substrate having a first

side on which the puncture resistant members are positioned,

the second composite guard covering the first composite guard, and

the first composite guard and the second composite guard being positioned such that the arrangement of puncture resistant members of the second composite guard is misaligned with the arrangement of puncture resistant members of the first composite guard.

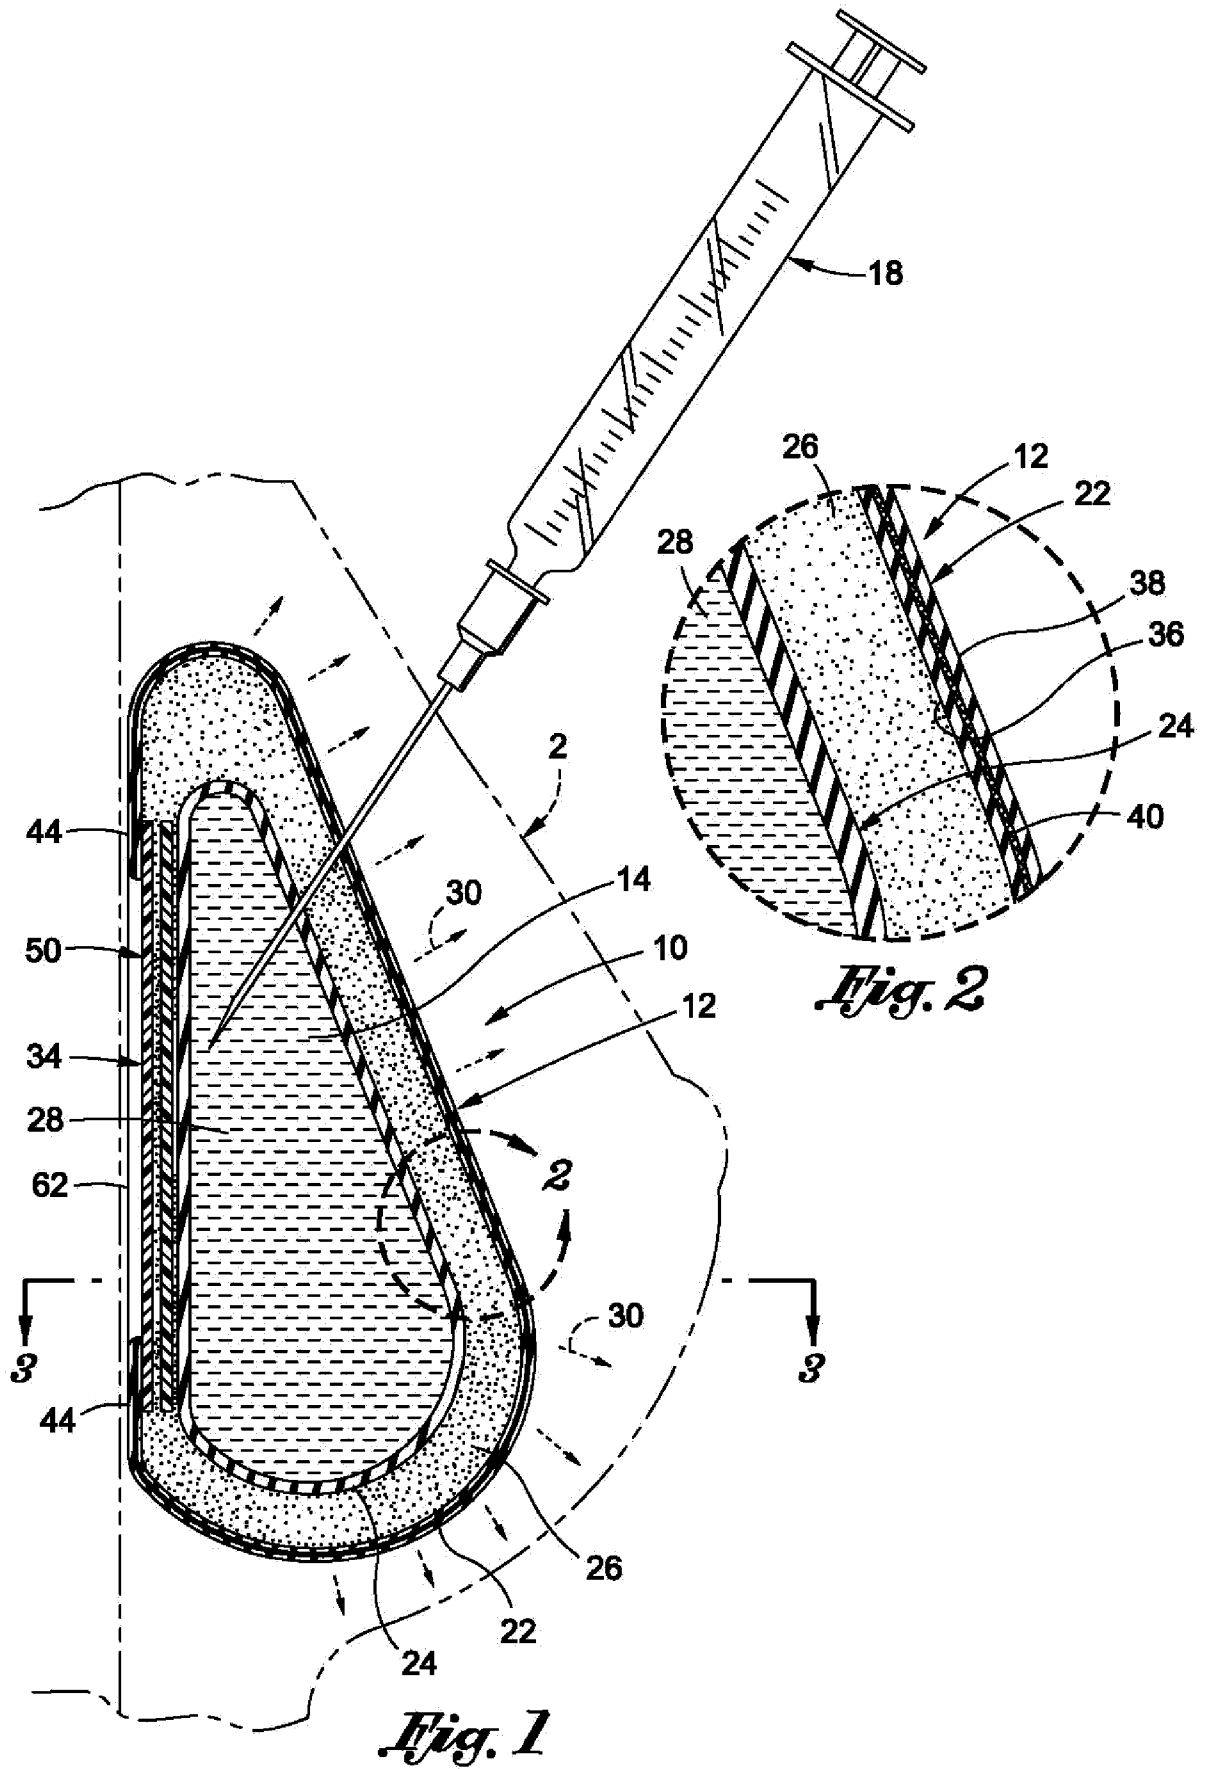

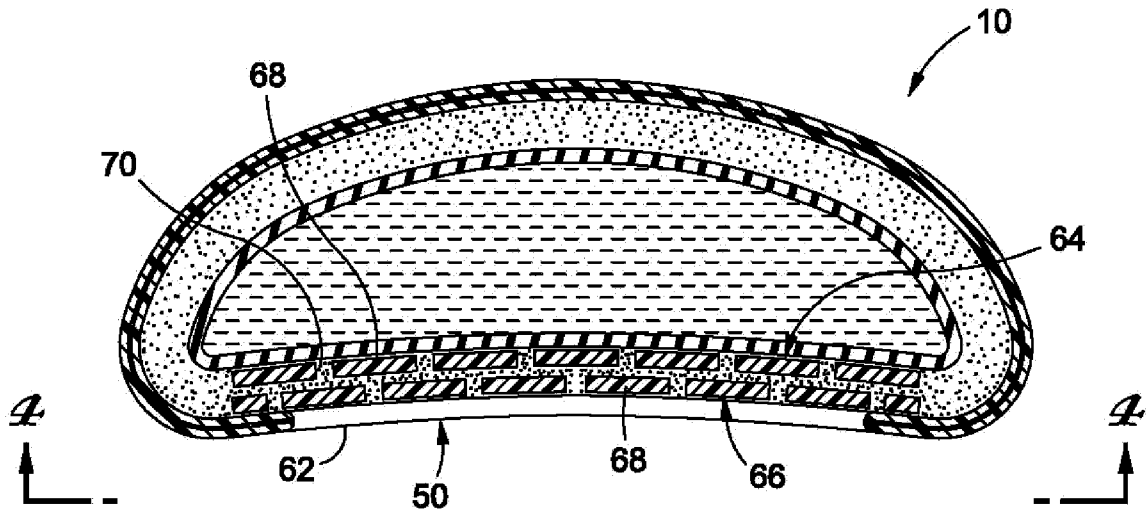


Fig. 3

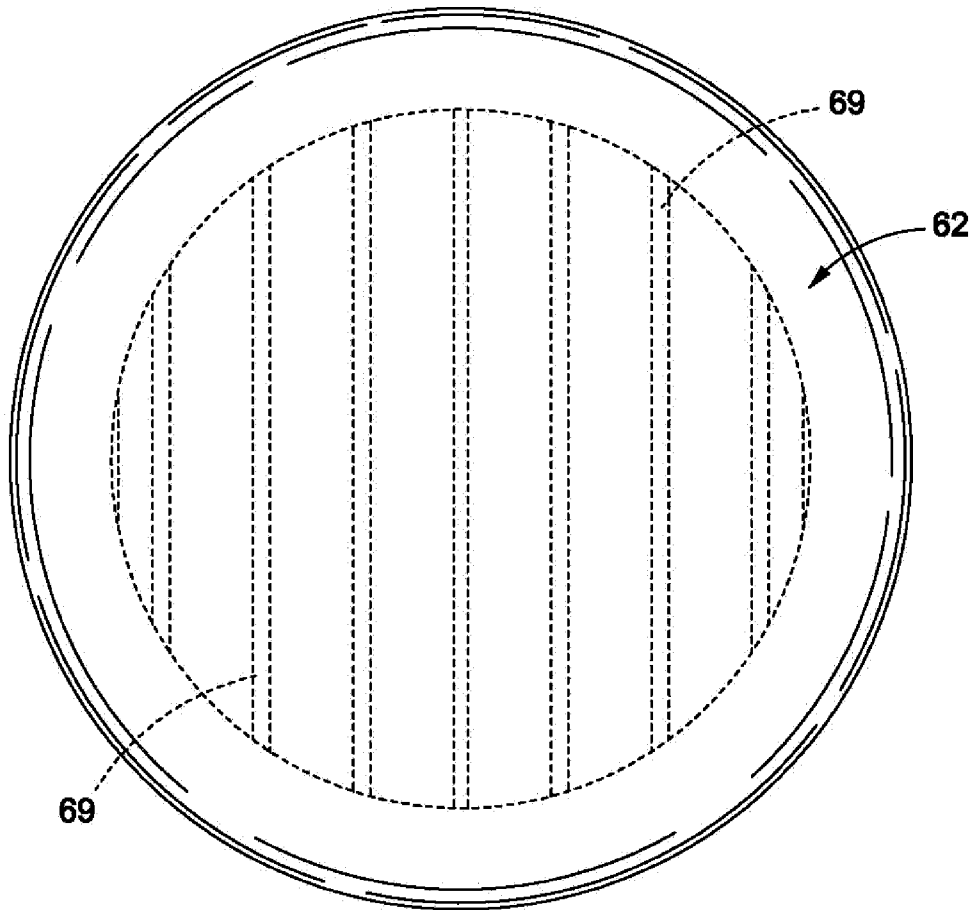


Fig. 4

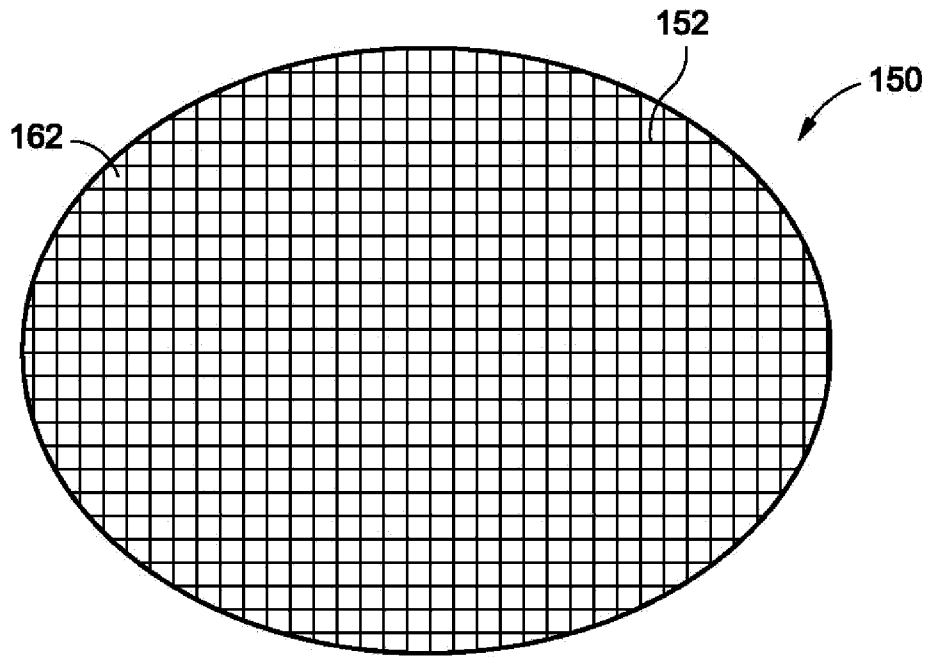


Fig. 4A

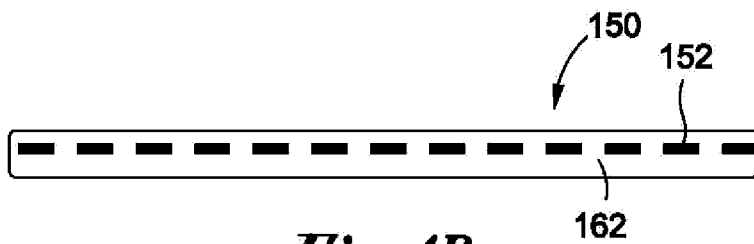


Fig. 4B

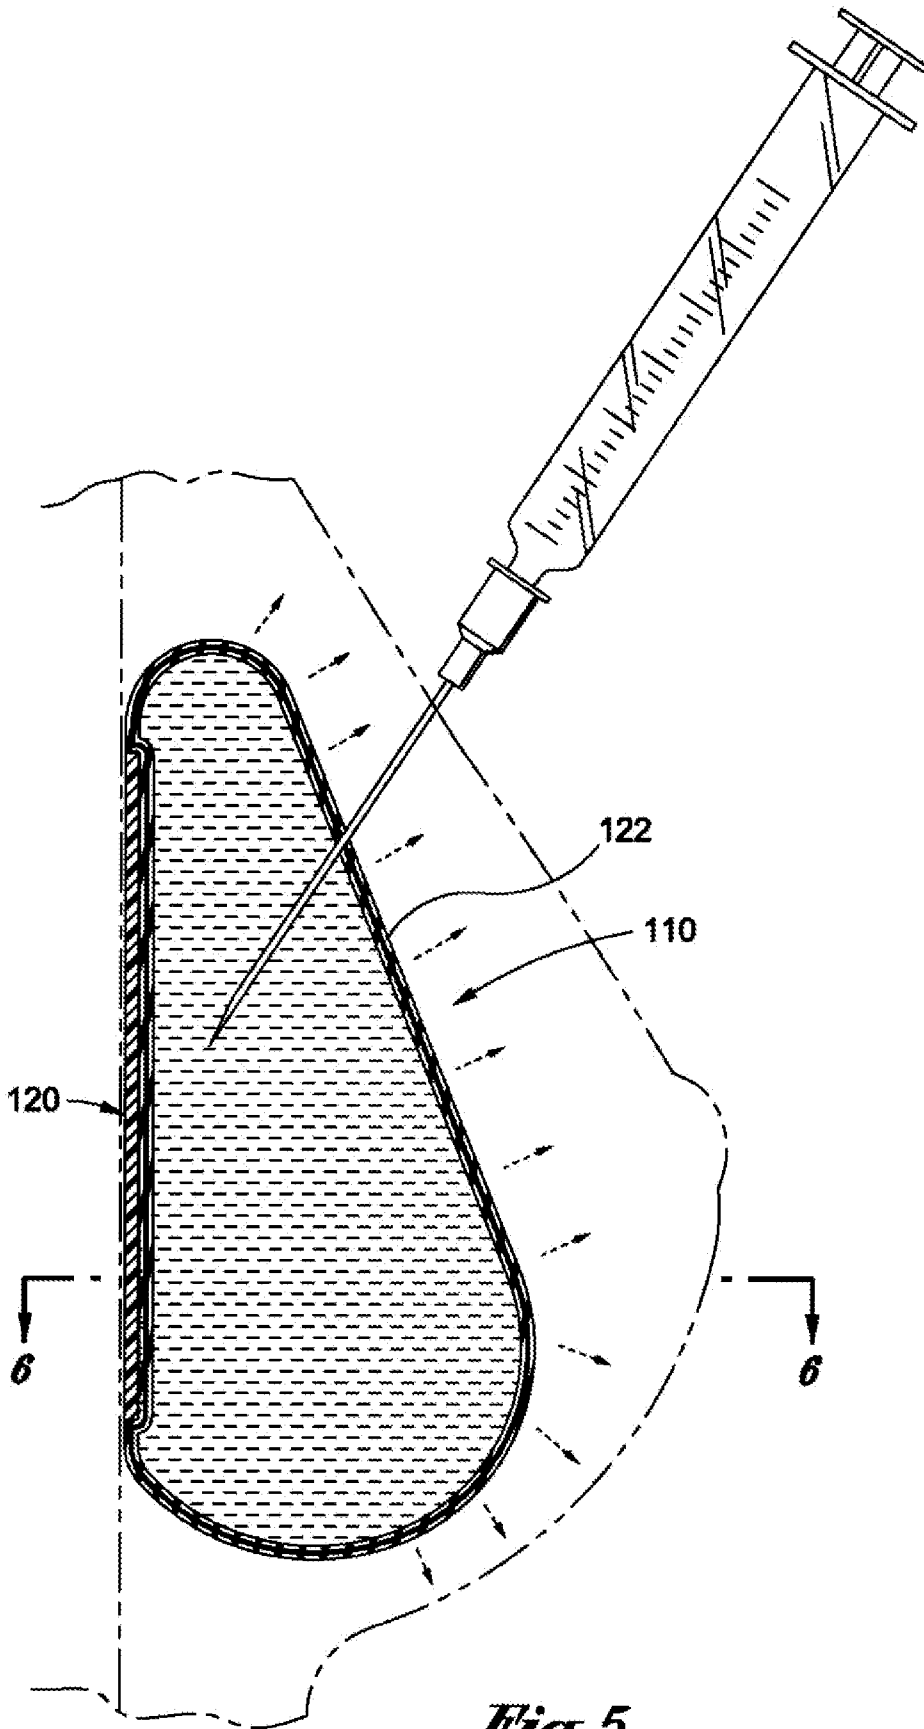


Fig. 5

5/22

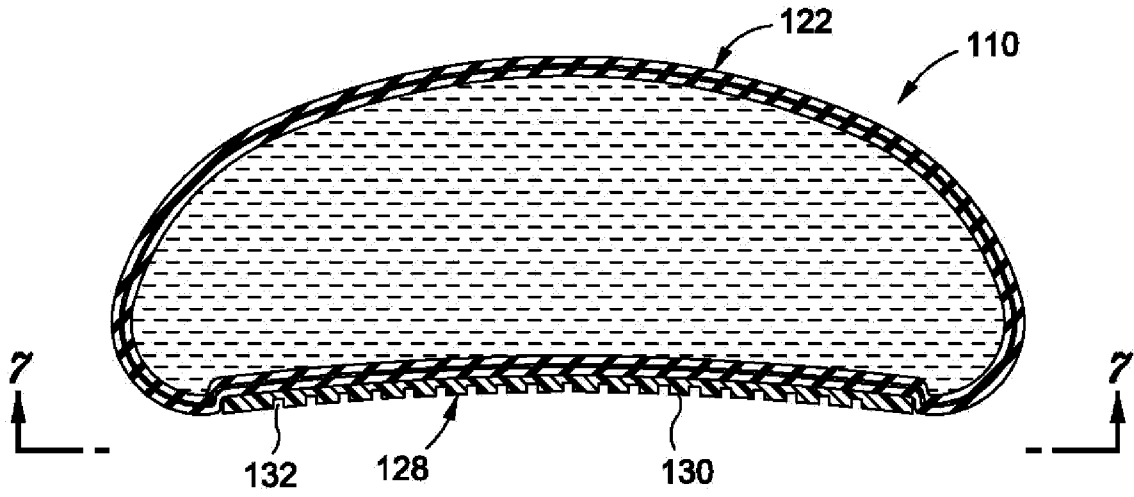


Fig. 6

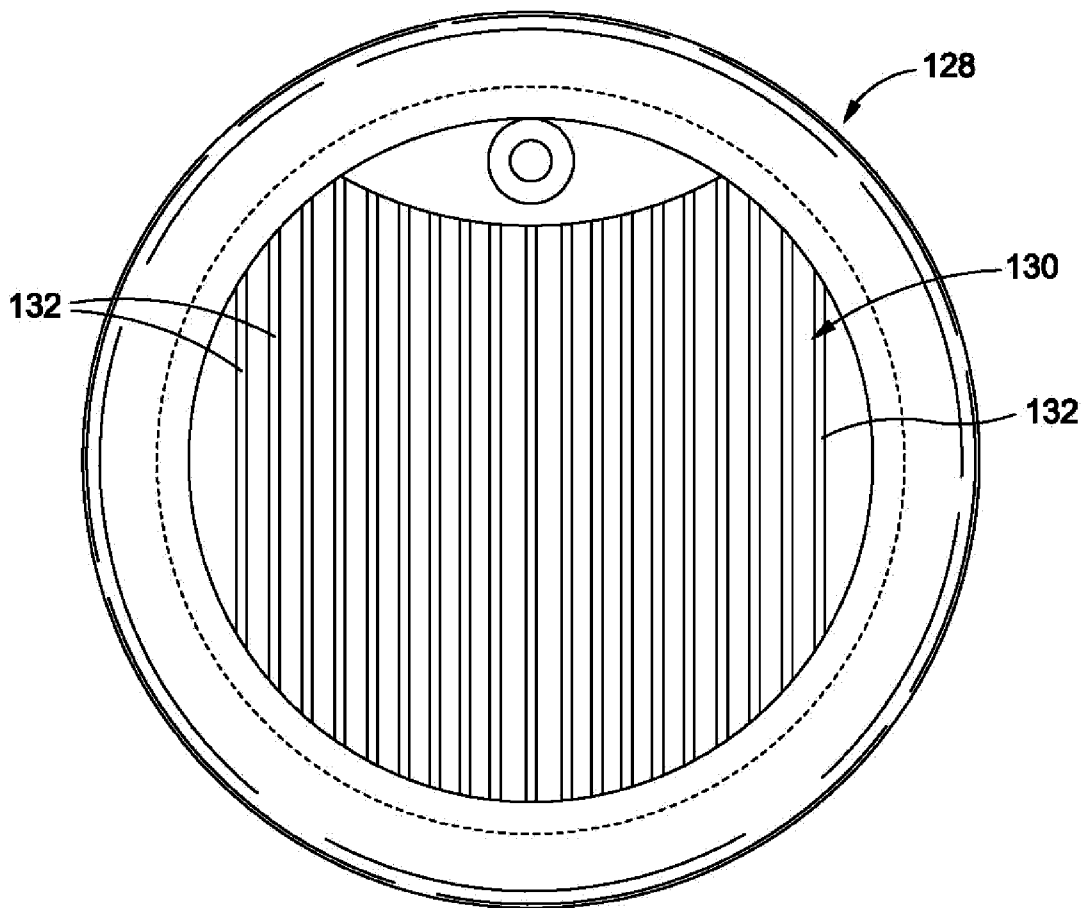
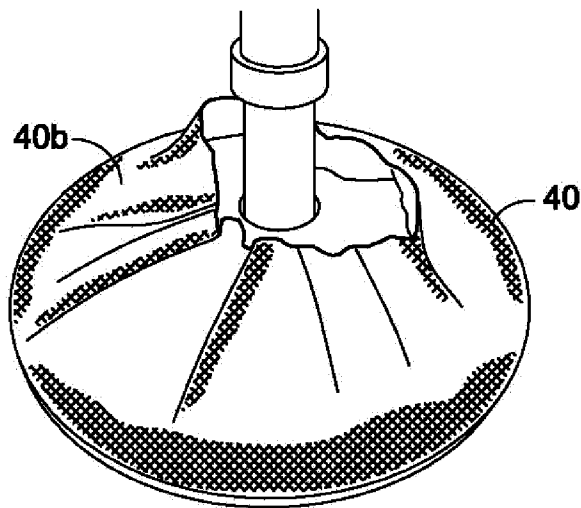
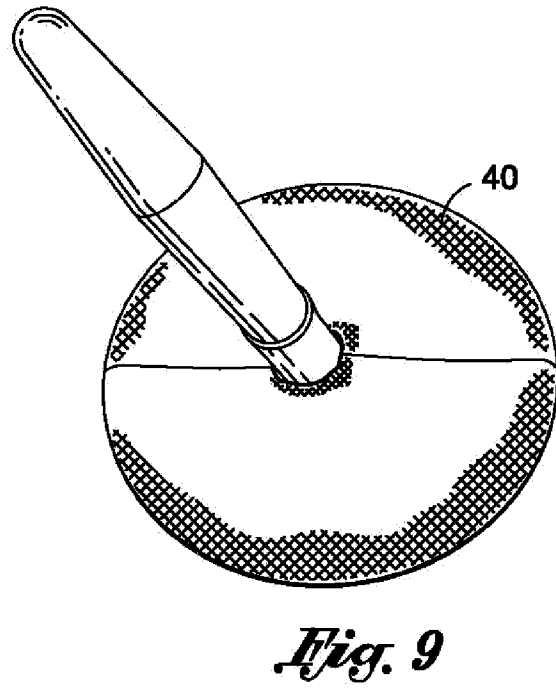
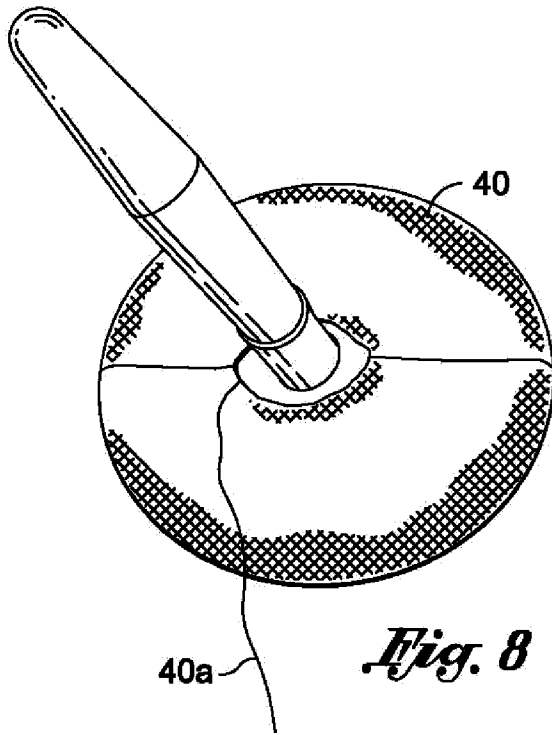


Fig. 7

6/22



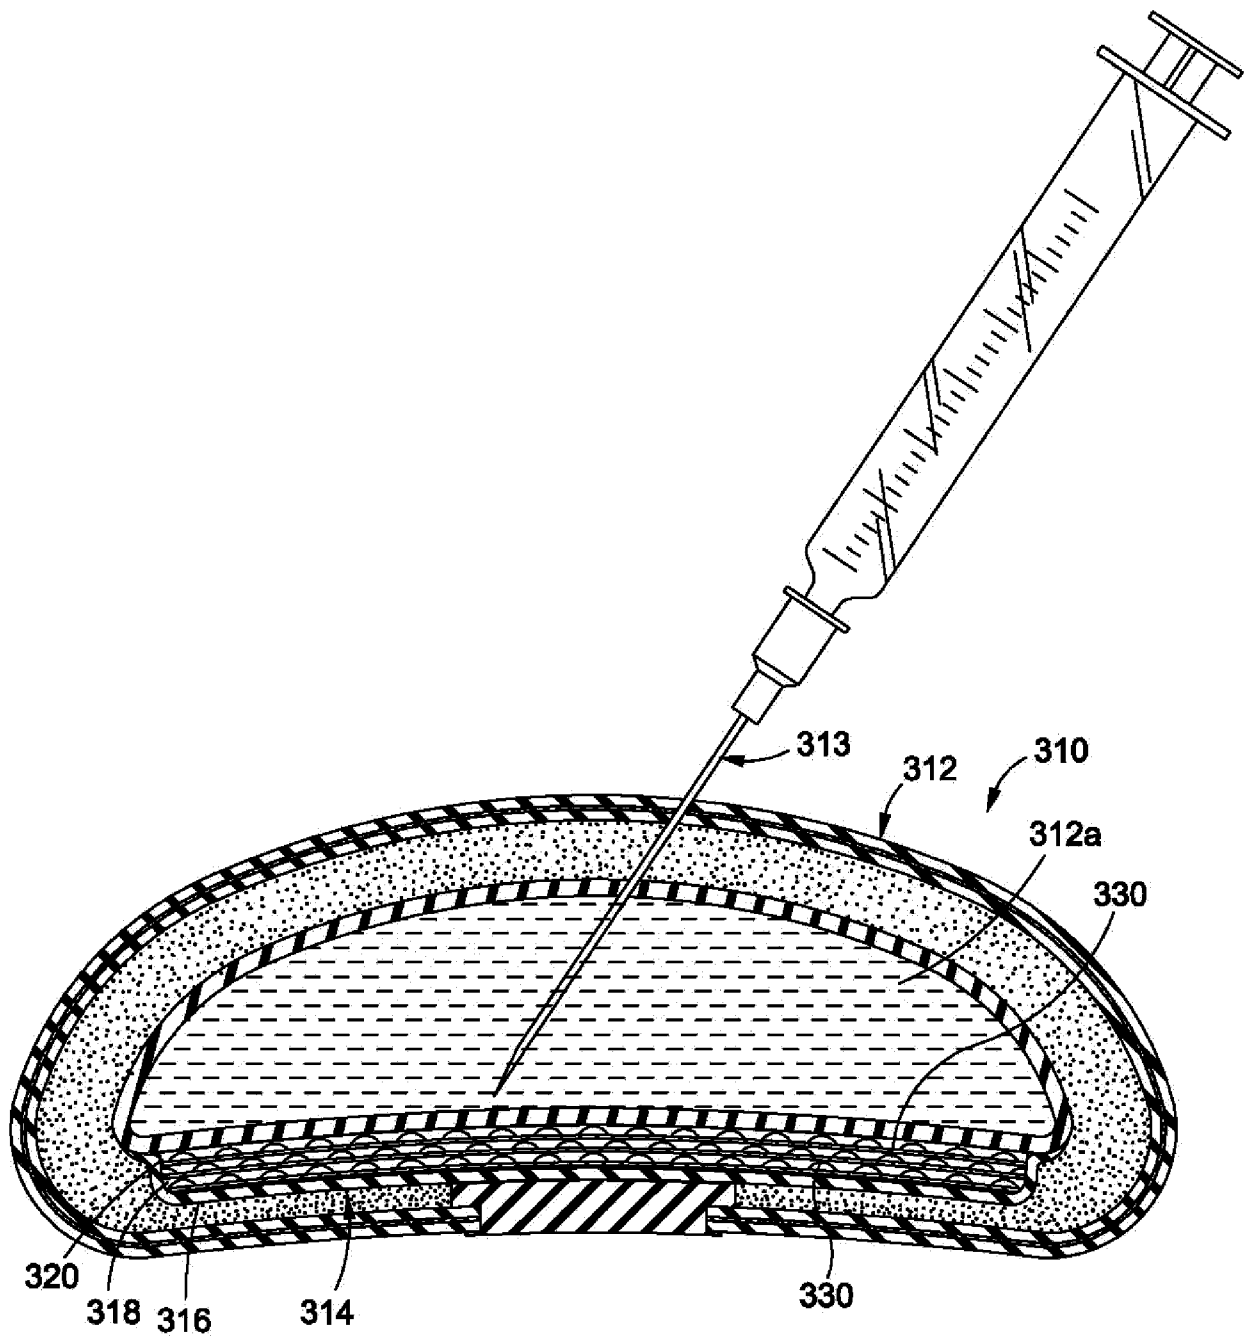


Fig. 11

8/22

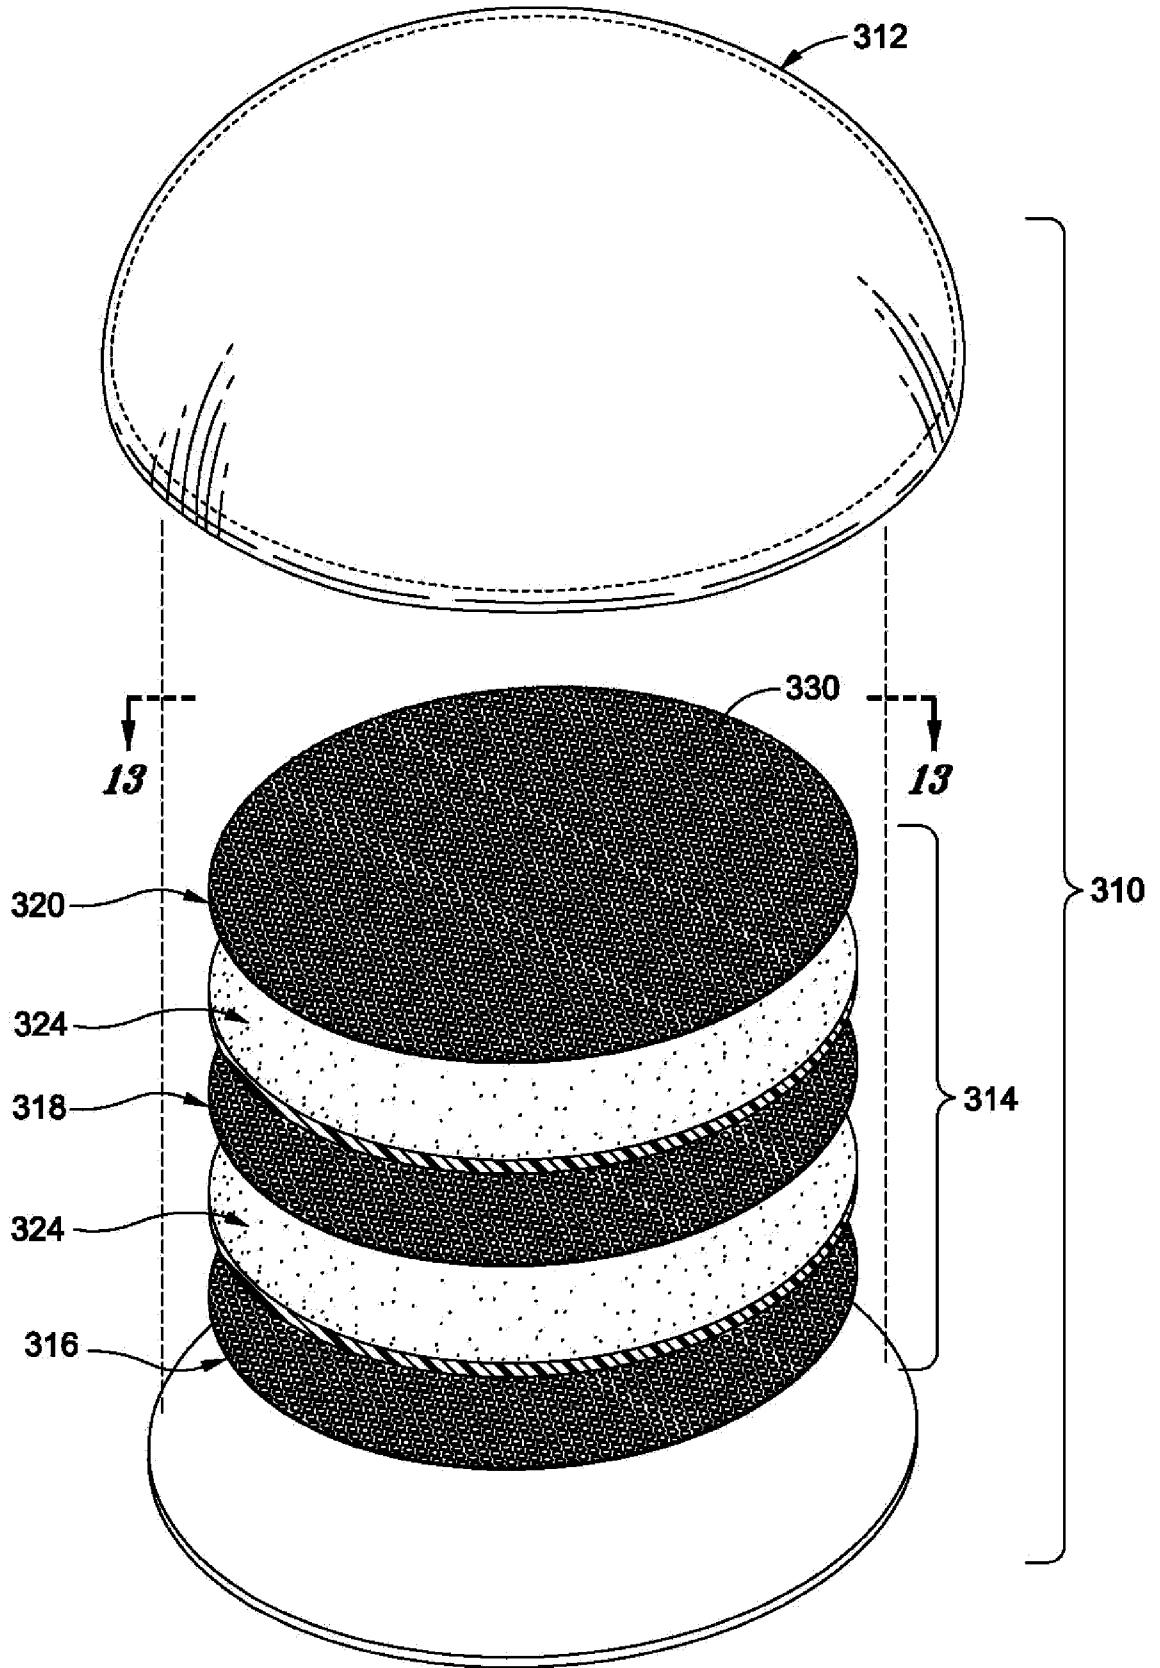


Fig. 12

9/22

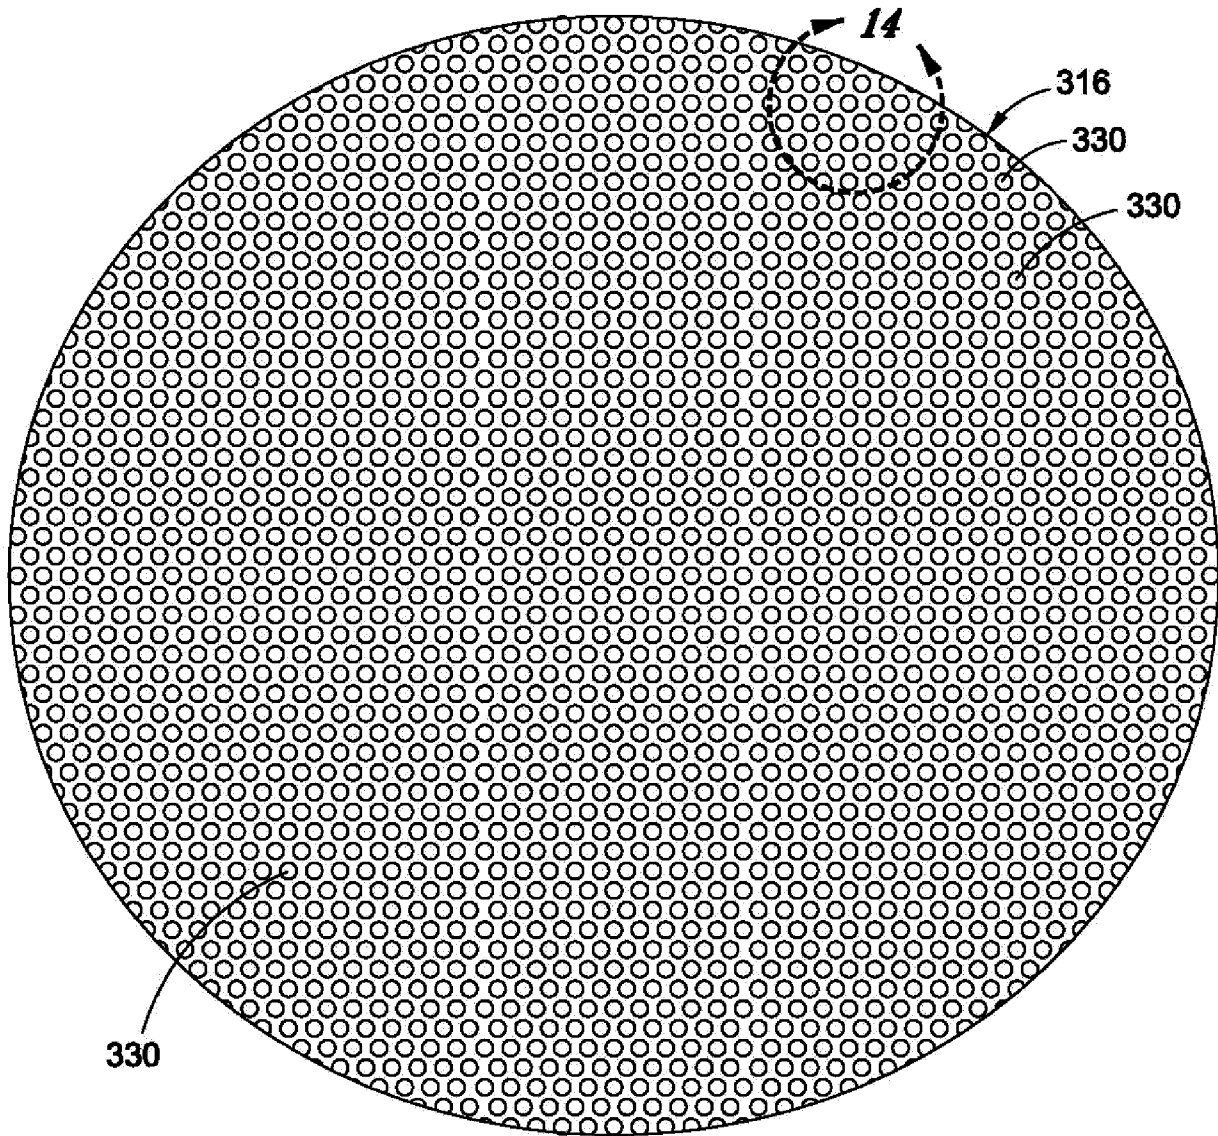


Fig. 13

10/22

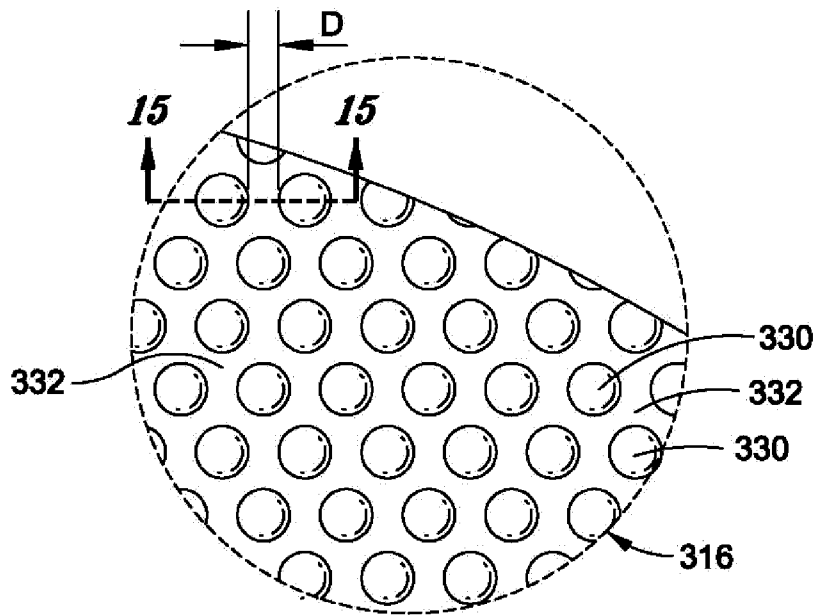


Fig. 14

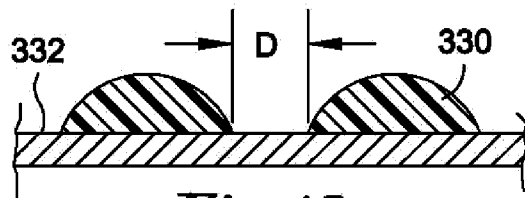


Fig. 15

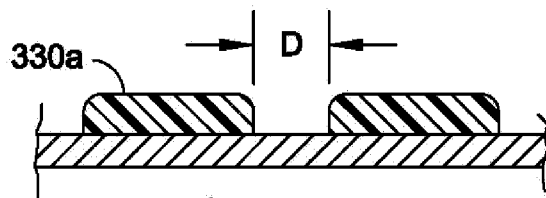


Fig. 16

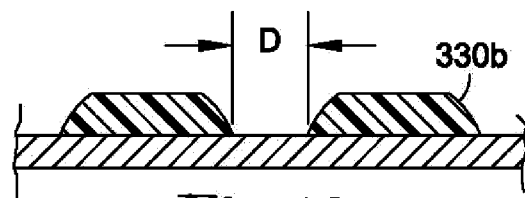


Fig. 16a

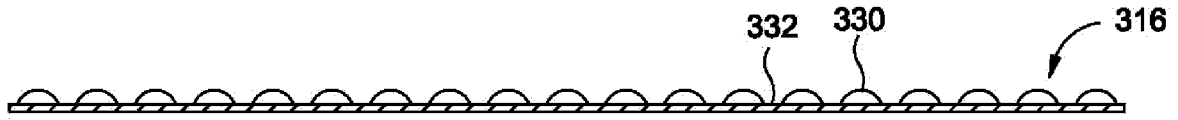


Fig. 17

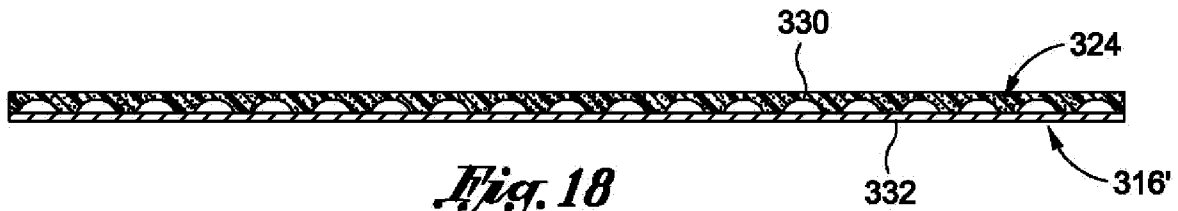


Fig. 18

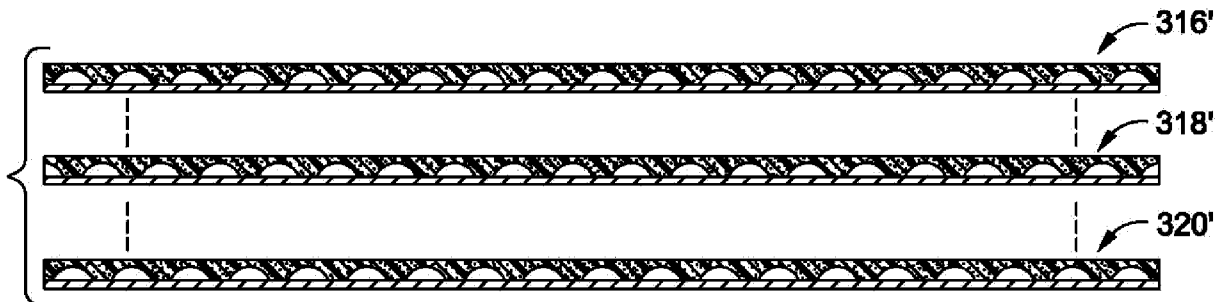


Fig. 18a

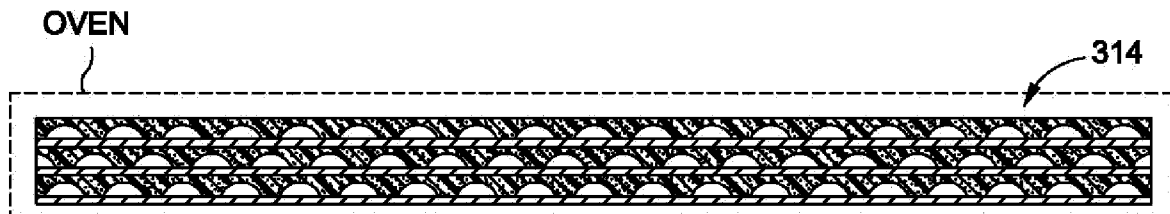


Fig. 19

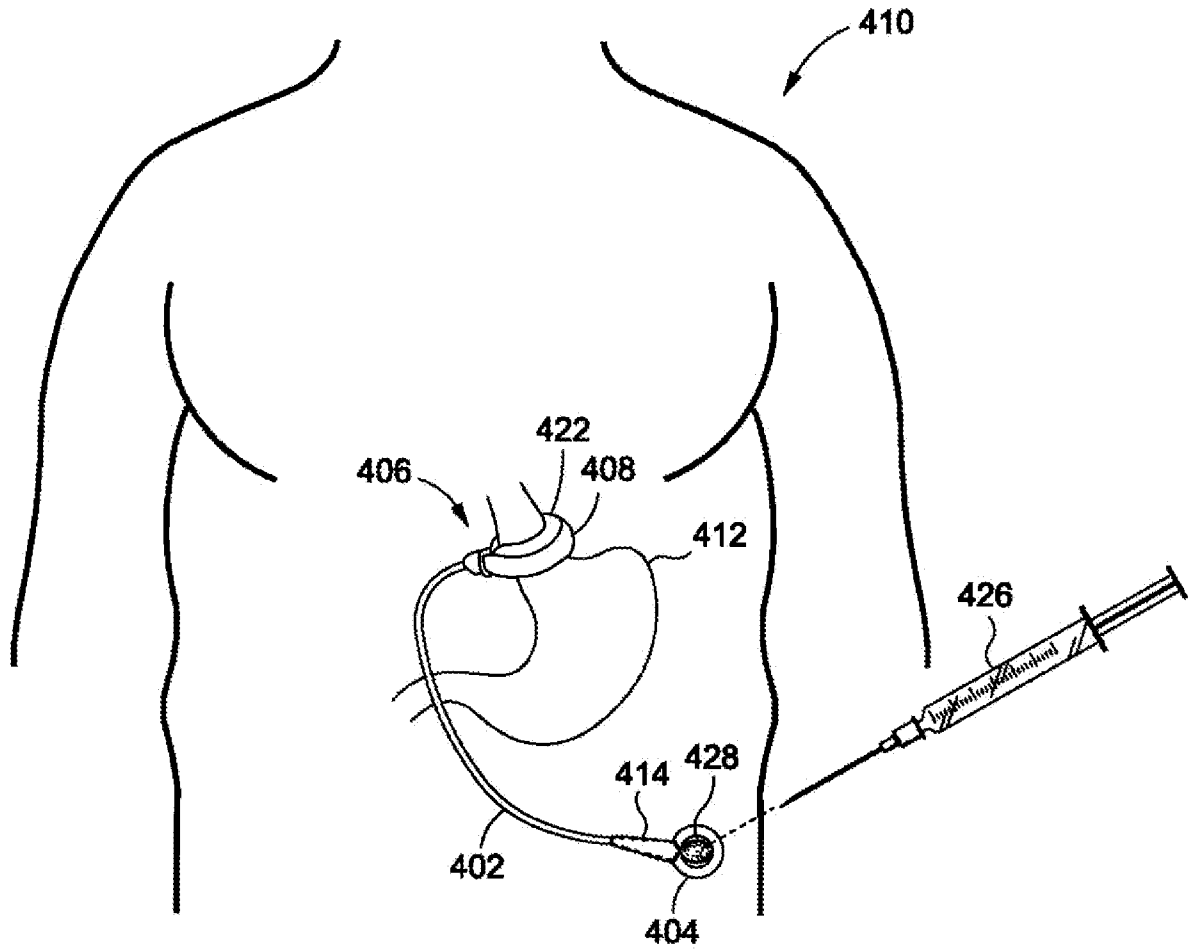


Fig. 20

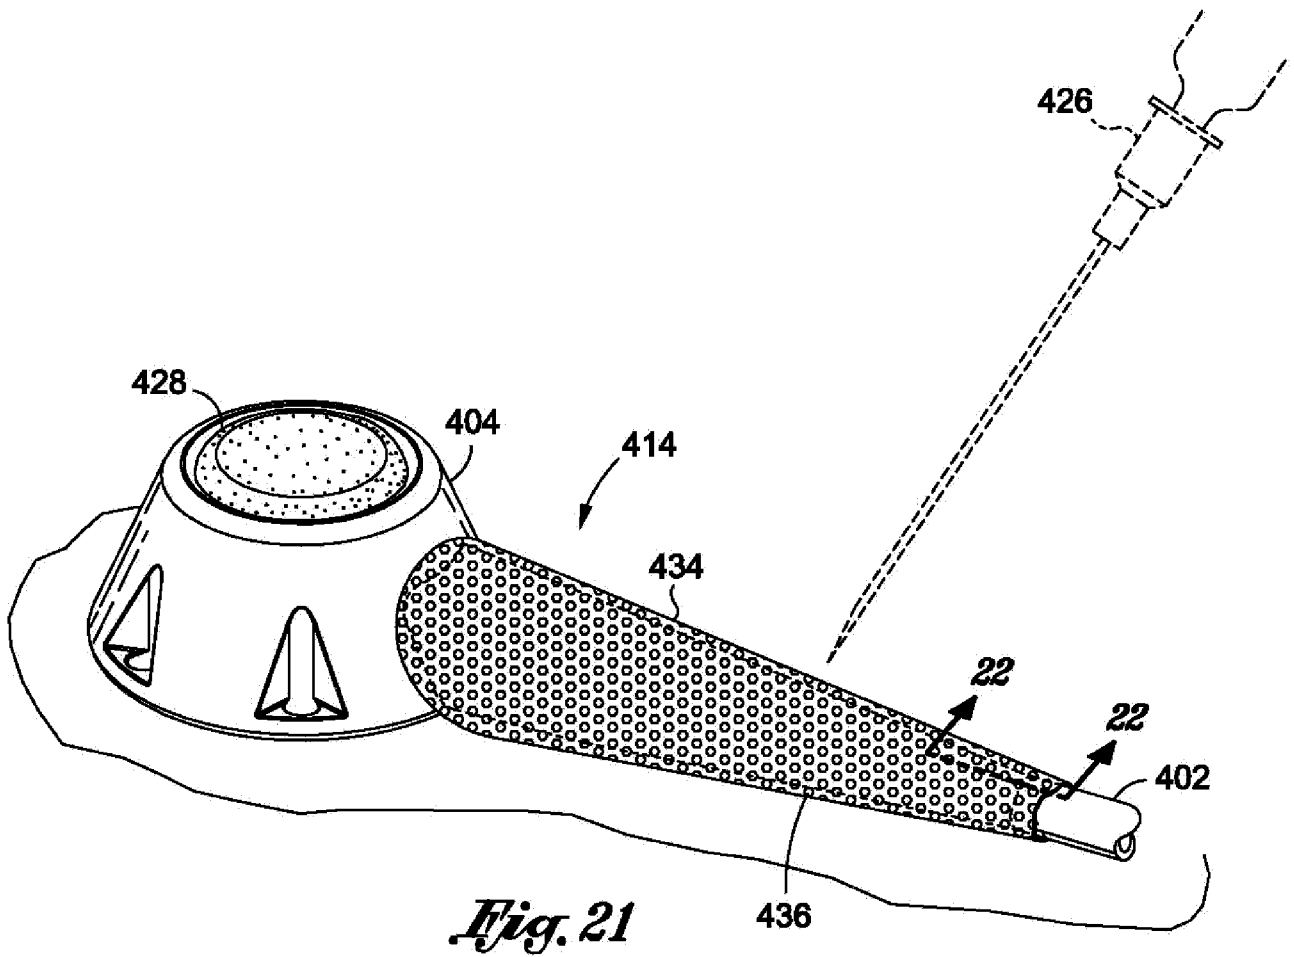


Fig. 21

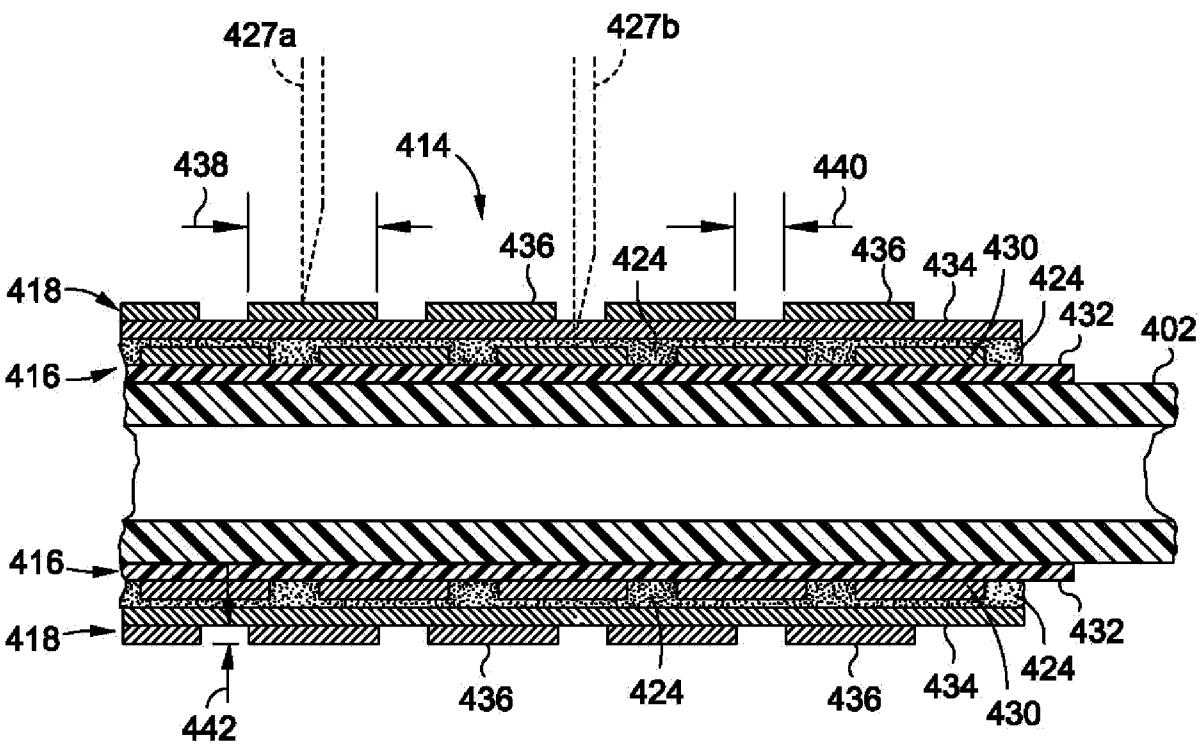
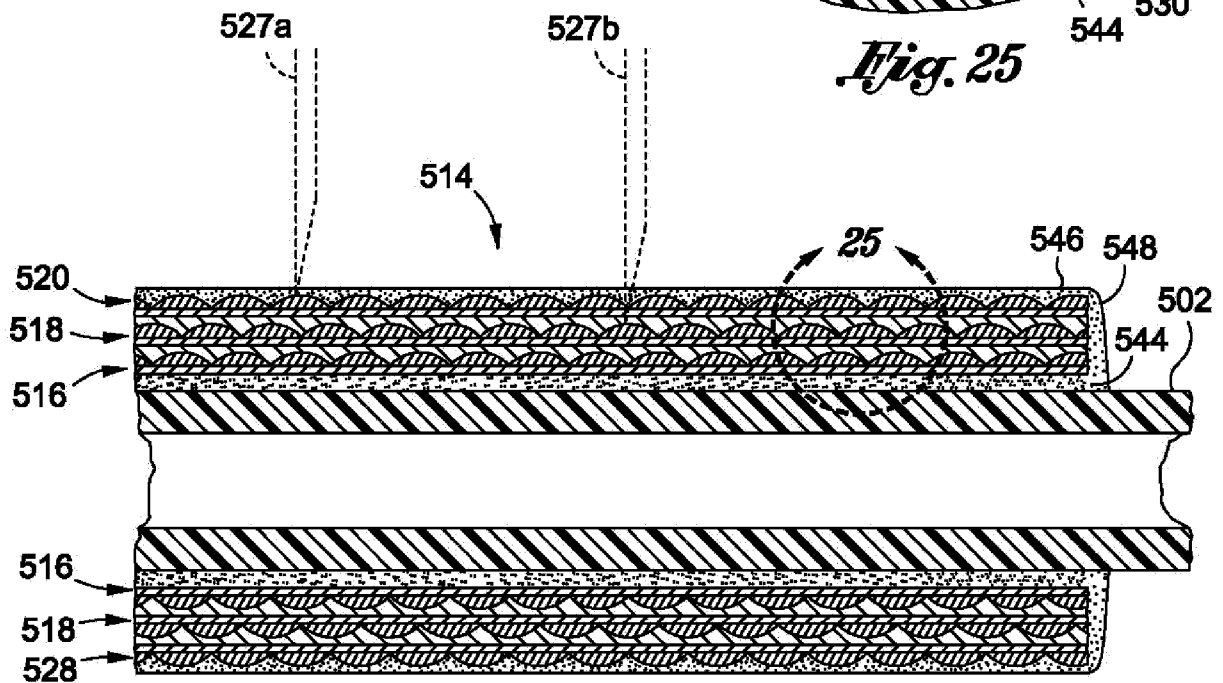
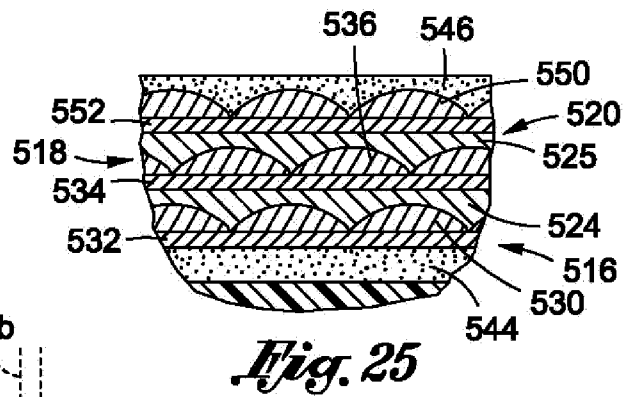
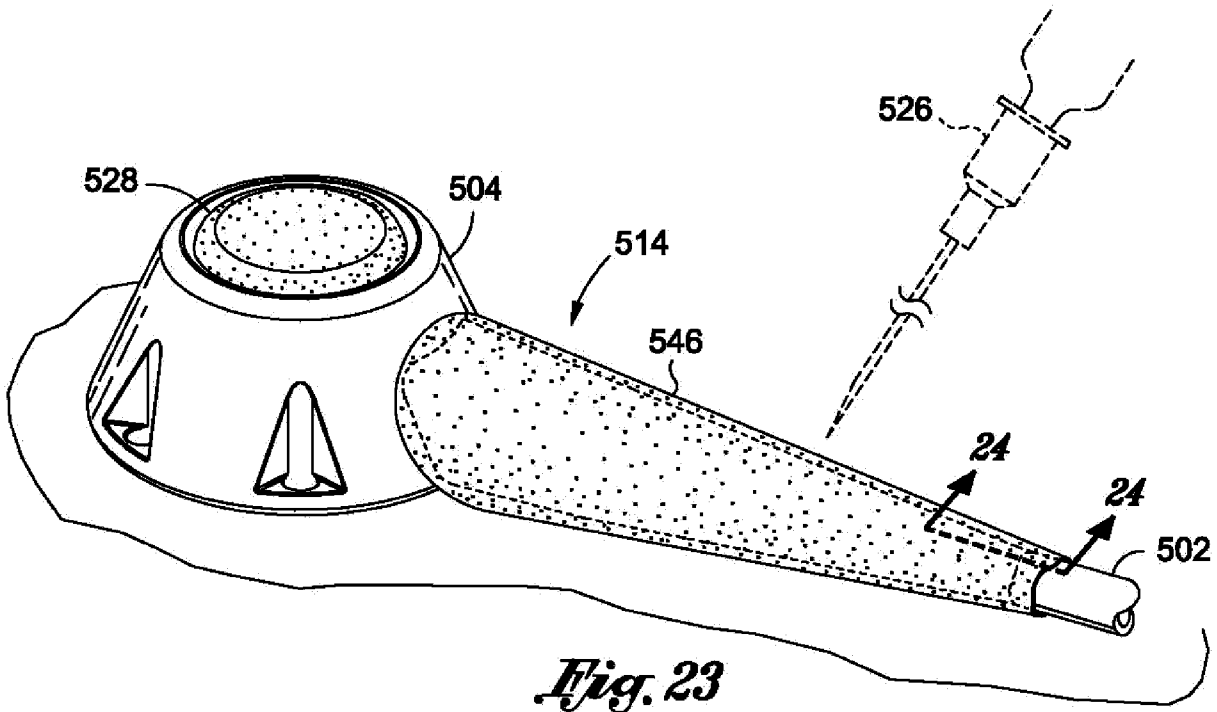


Fig. 22

14/22



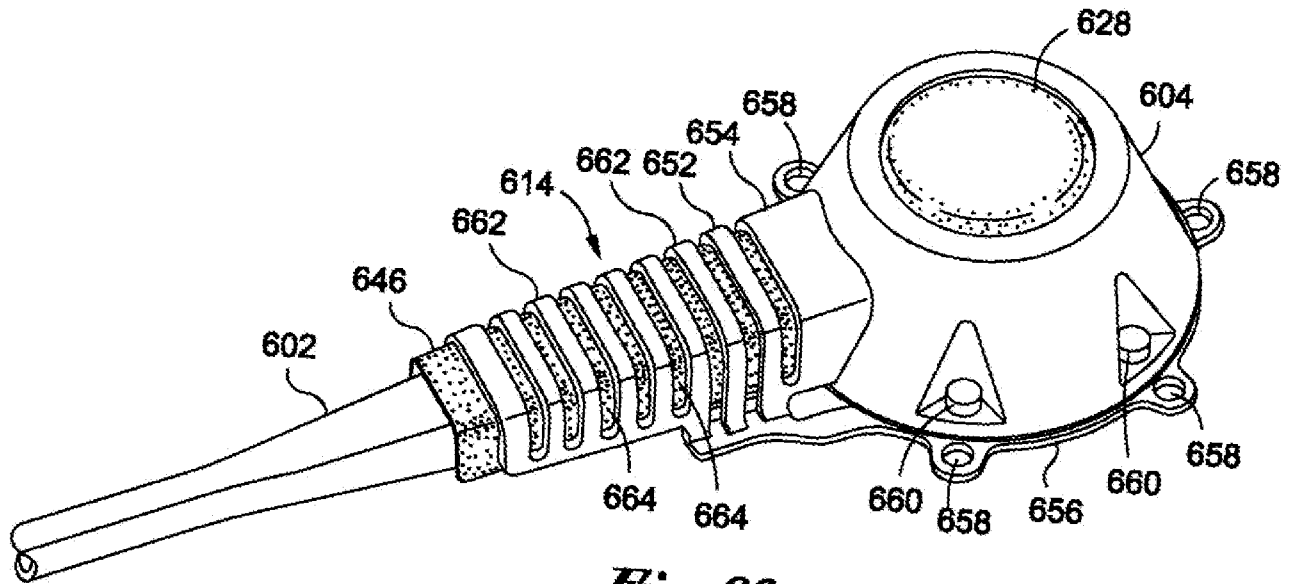


Fig. 26

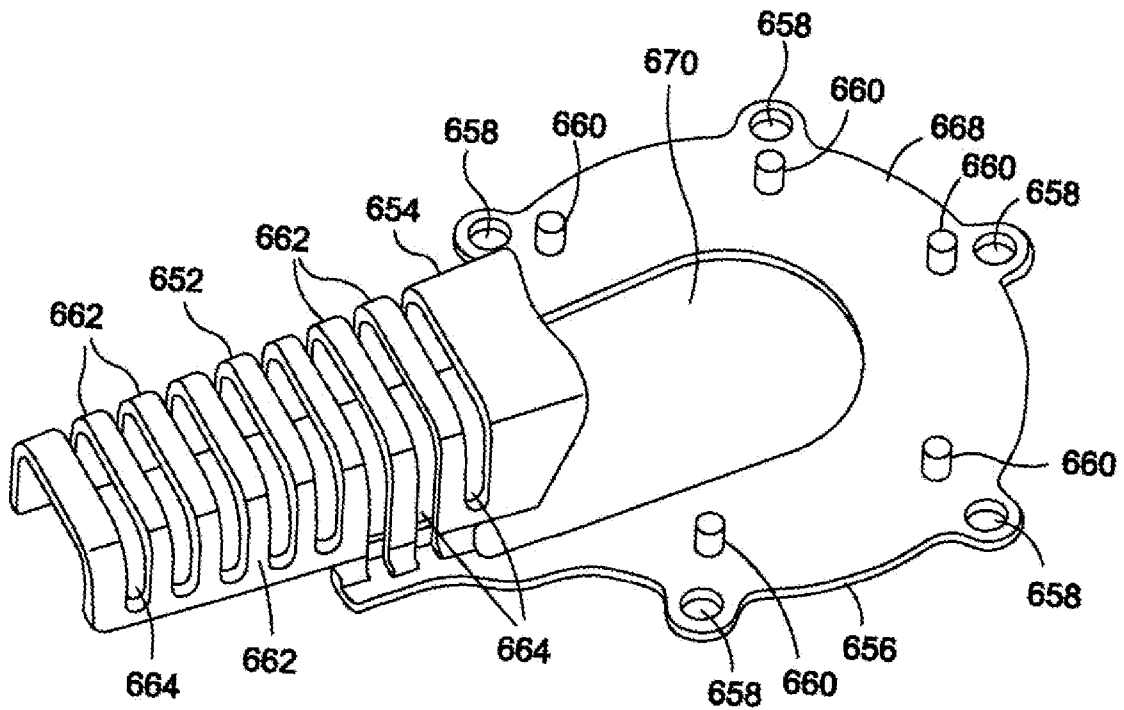


Fig. 27

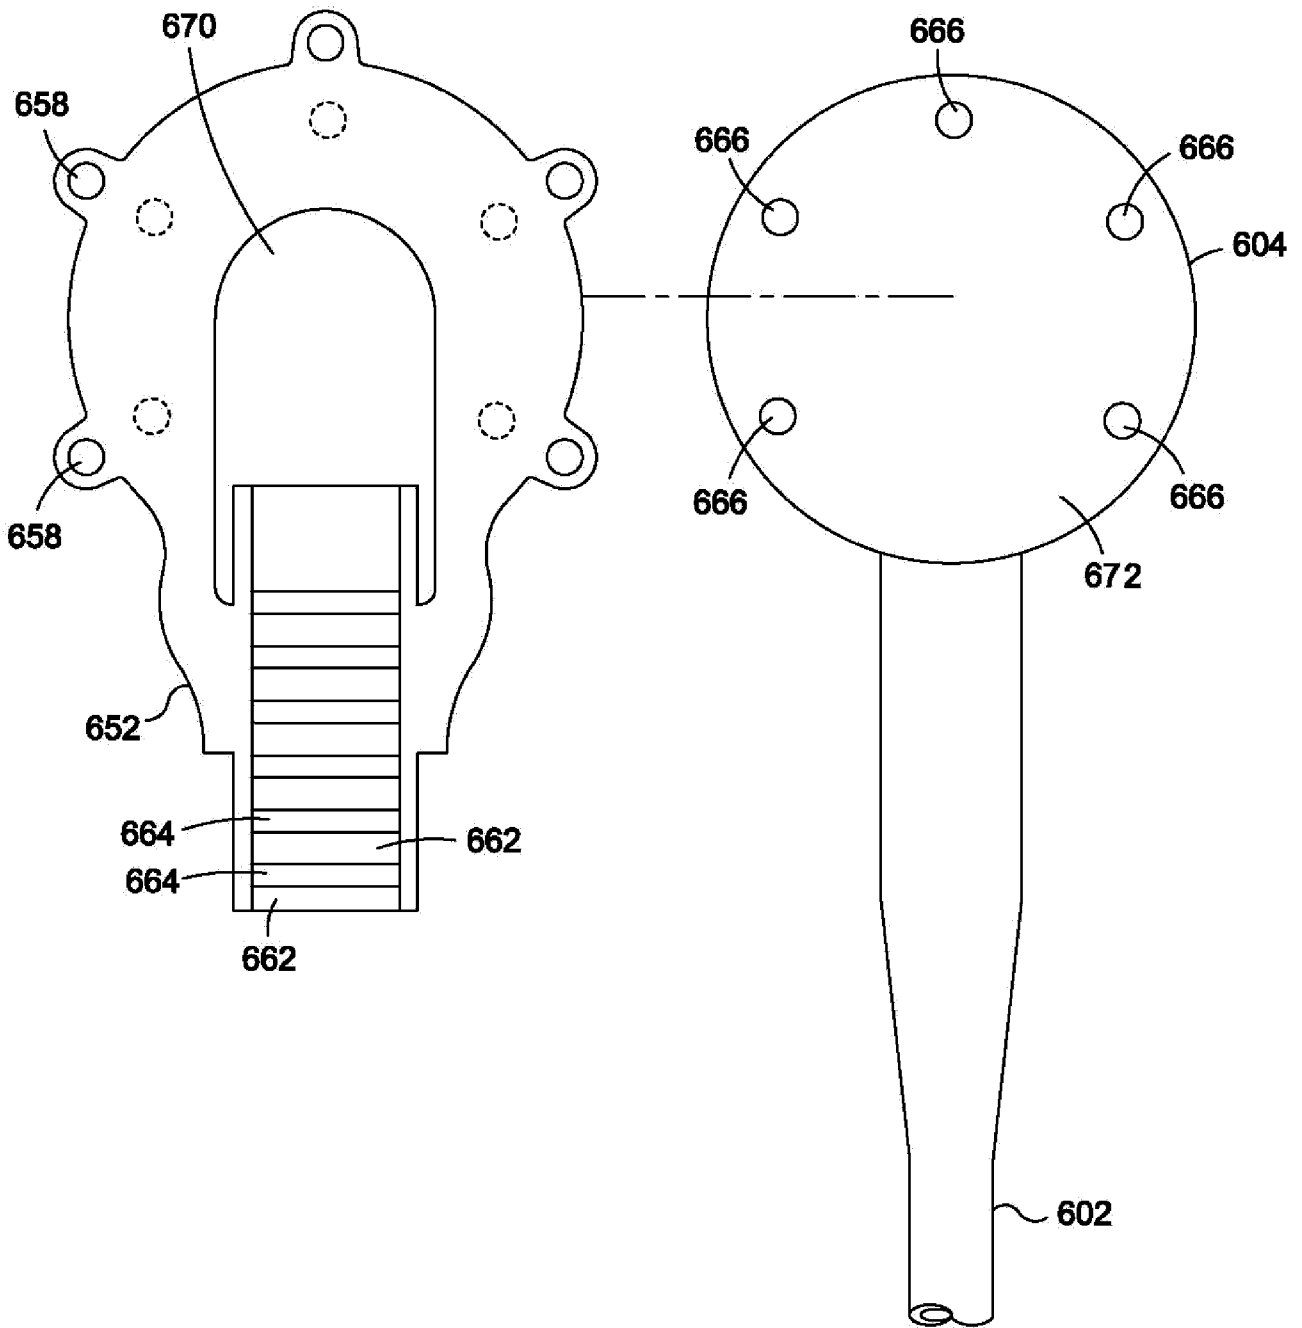


Fig. 28

17/22

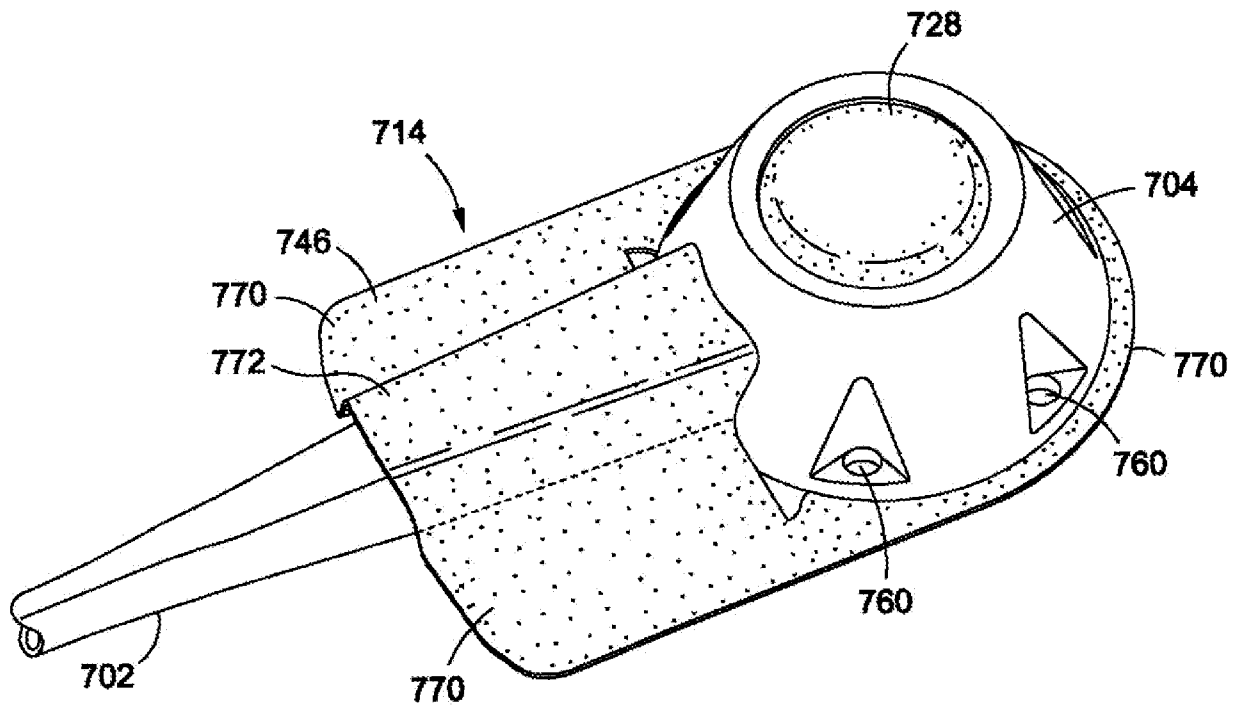


Fig. 29

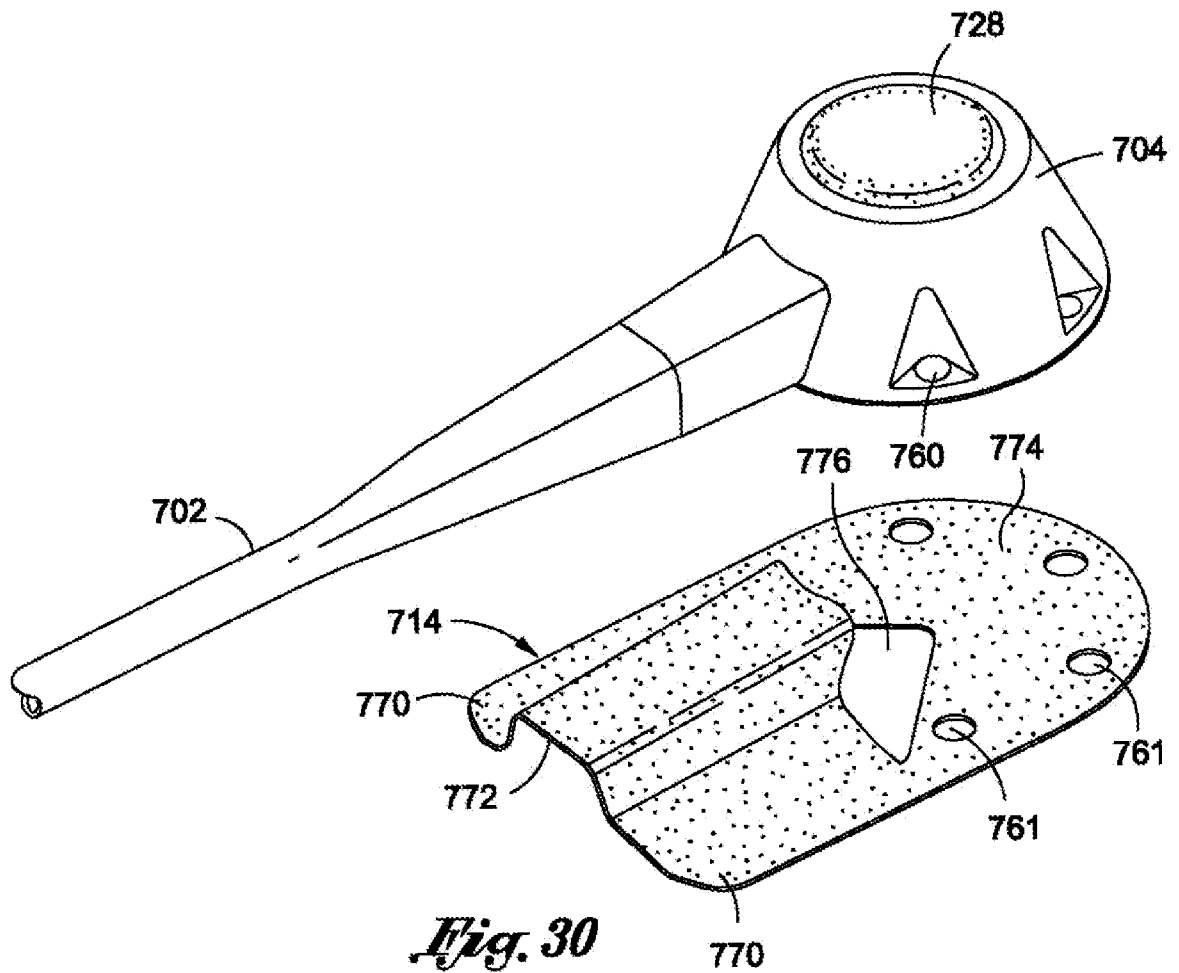


Fig. 30

18/22

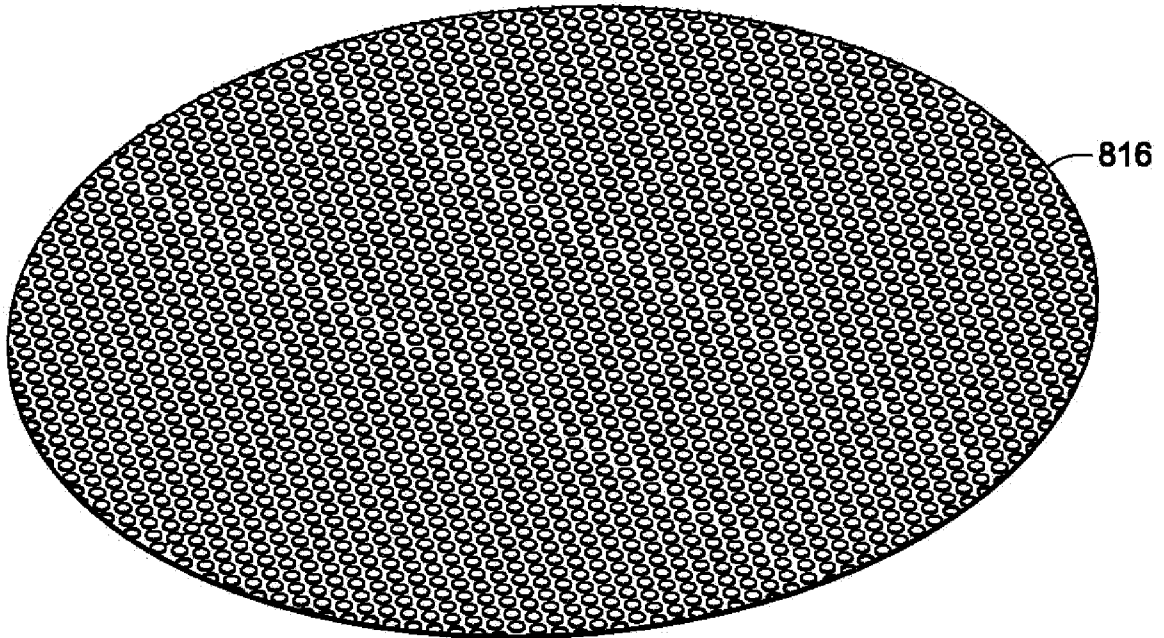


Fig. 31

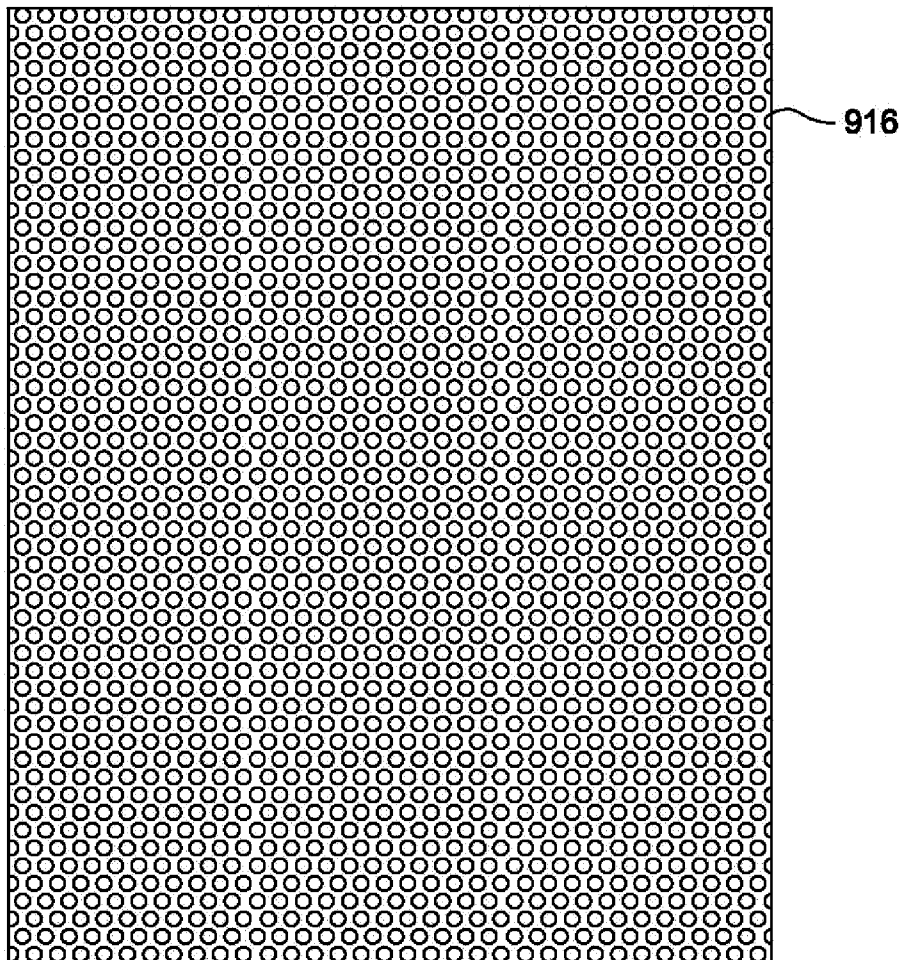


Fig. 32

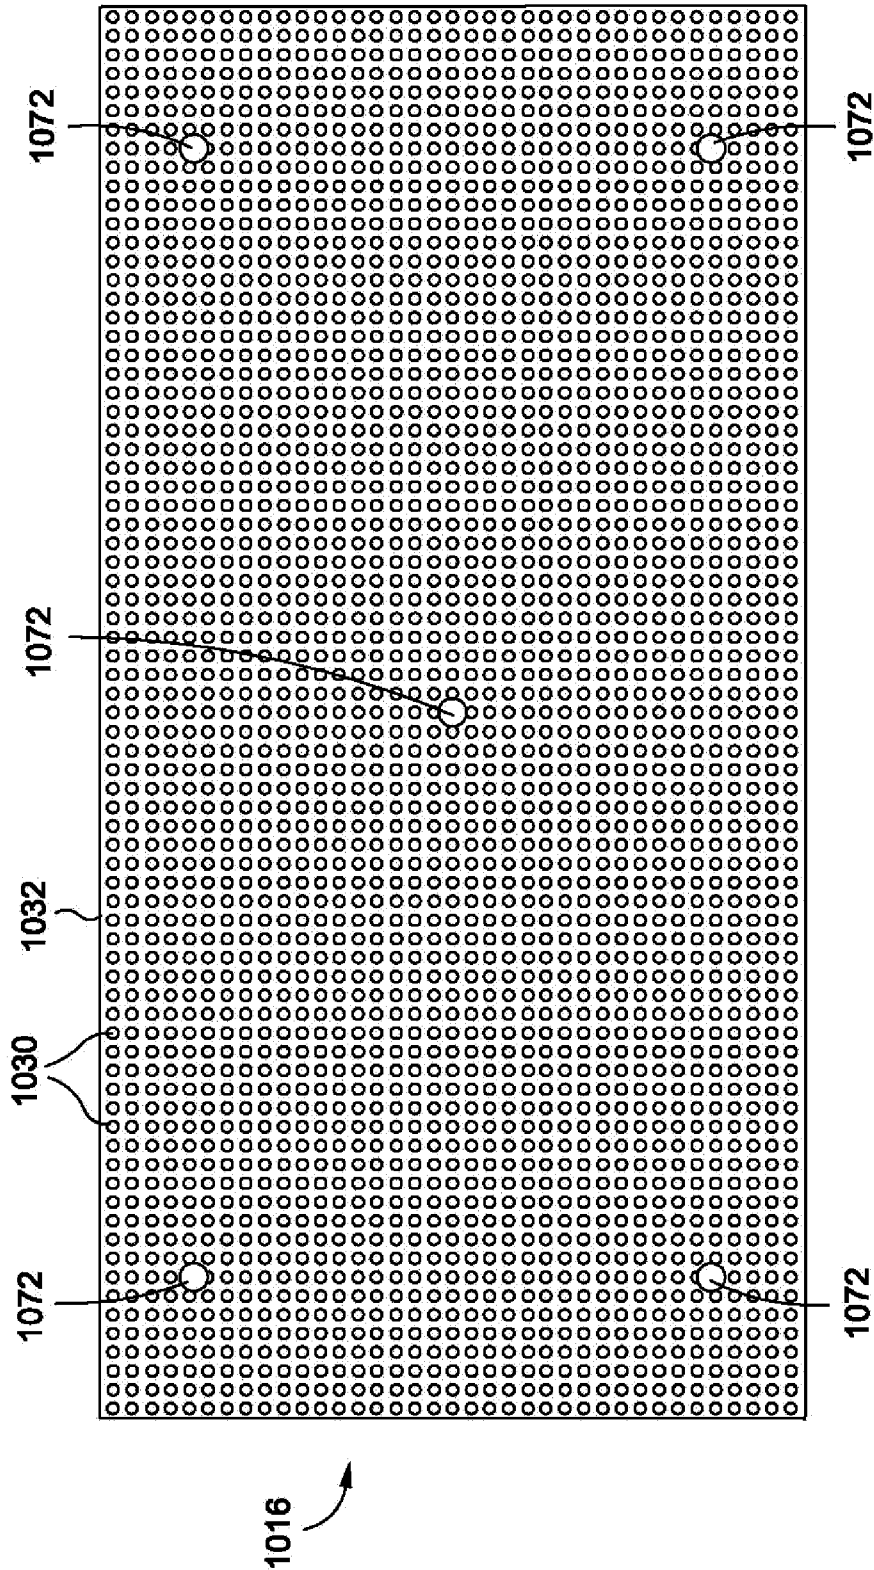


Fig. 33

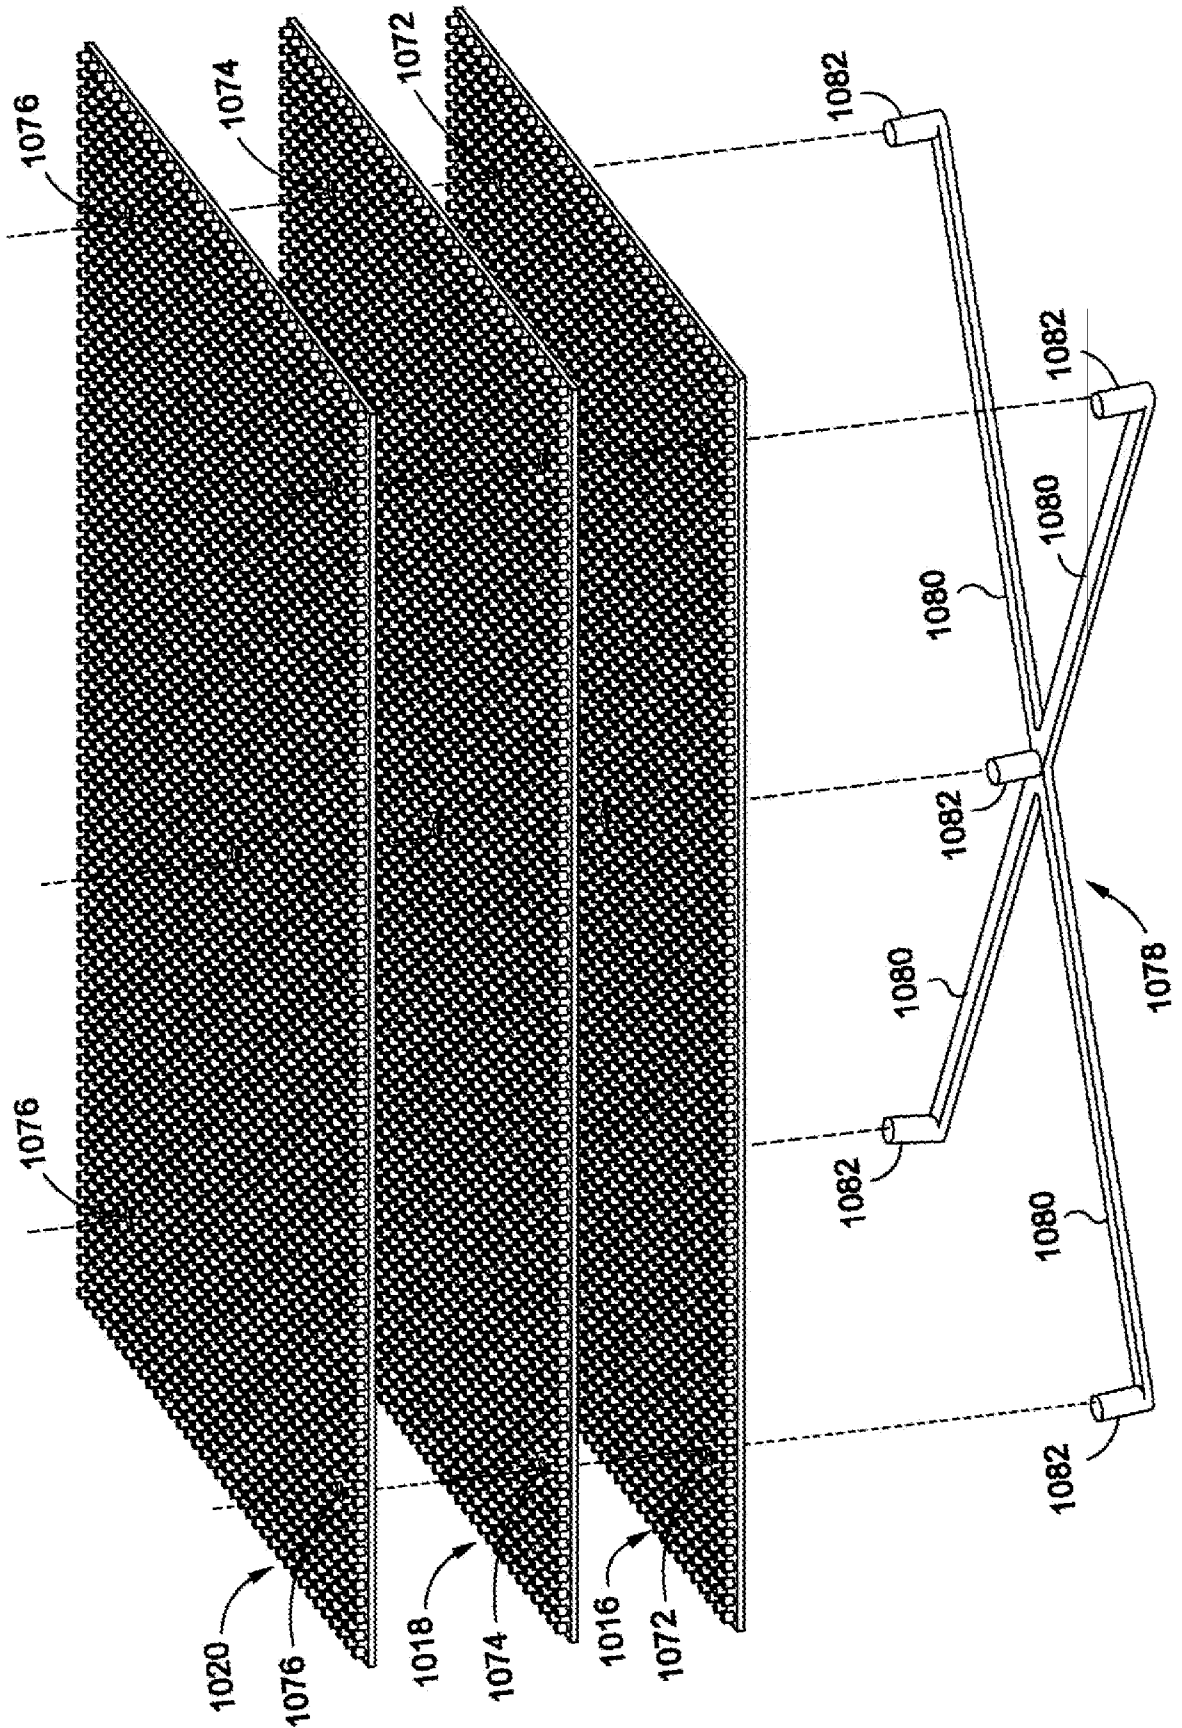


Fig. 34

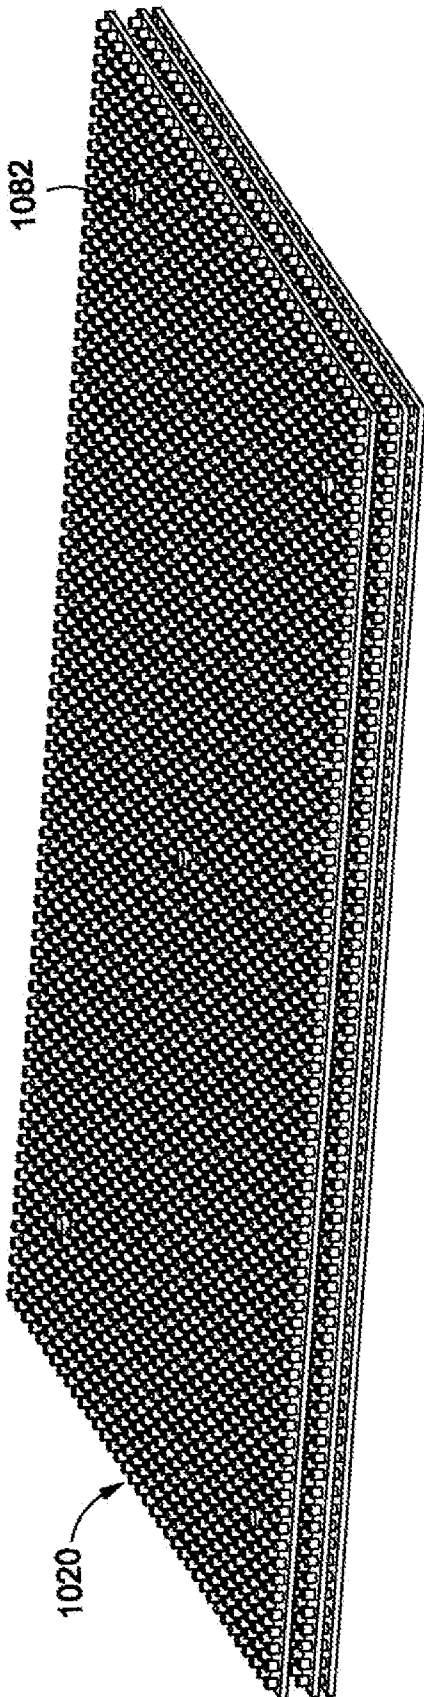


Fig. 35

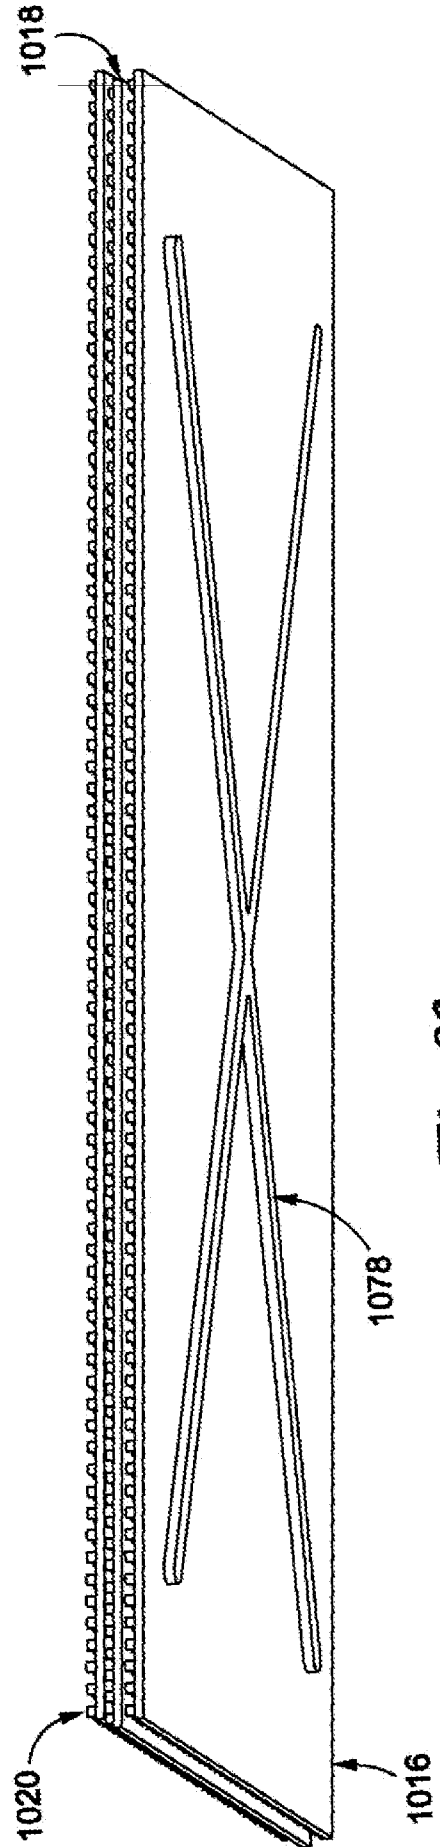


Fig. 36

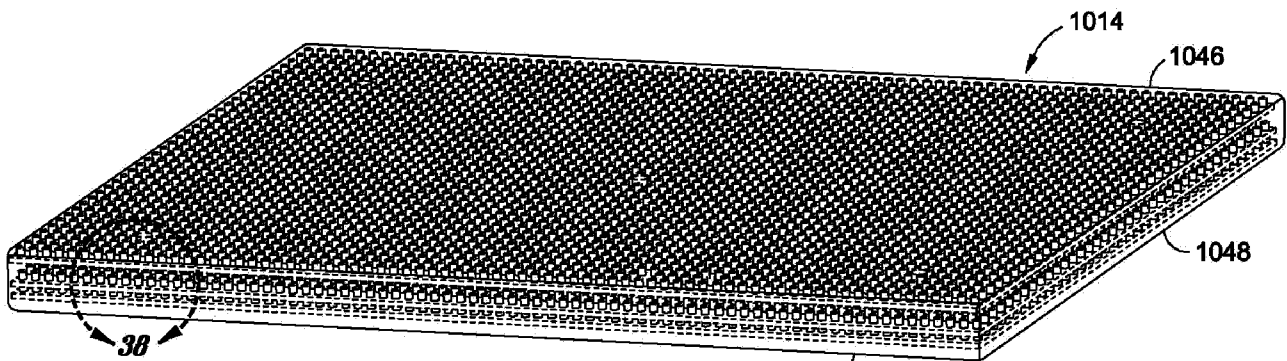


Fig. 37

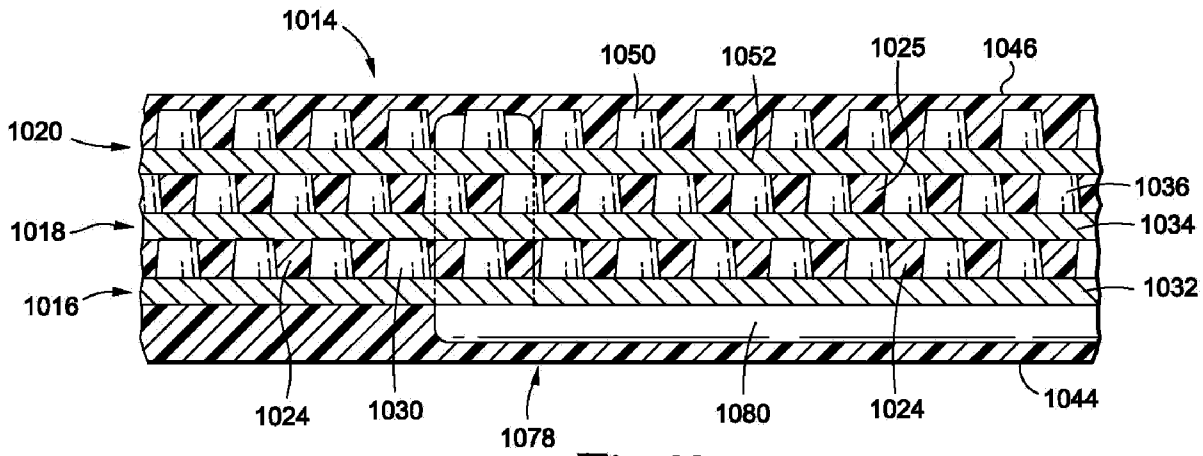


Fig. 38

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2012/037305

A. CLASSIFICATION OF SUBJECT MATTER
INV. A61F5/00 A41D19/015 A41H1/02 F41H5/04
ADD.
According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED
Minimum documentation searched (classification system followed by classification symbols)
A61F A41D A41H F41H

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
EPO-Internal, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 2009/270904 A1 (BIRK JANEL A [US] ET AL) 29 October 2009 (2009-10-29) paragraph [0046]; claims; figures -----	1-24
Y	US 2011/054407 A1 (OLROYD CRAIG [US] ET AL) 3 March 2011 (2011-03-03) paragraph [0110]; claims; figures -----	1-24
Y	WO 02/10667 A2 (HIGHER DIMENSION MEDICAL INC [US]; YOUNG HWA KIM PH D [US]; HONG JI [U]) 7 February 2002 (2002-02-07) page 47, line 16 - page 48, line 10; figures 9, 10 -----	1-24
Y	US 2001/052141 A1 (ANDERSEN LARS P [NO]) 20 December 2001 (2001-12-20) the whole document -----	1-24
	-/--	

Further documents are listed in the continuation of Box C.

See patent family annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search 11 July 2012	Date of mailing of the international search report 20/07/2012
---	--

Name and mailing address of the ISA/ European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel. (+31-70) 340-2040, Fax: (+31-70) 340-3016	Authorized officer Serra i Verdaguer, J
--	--

INTERNATIONAL SEARCH REPORT

International application No
PCT/US2012/037305

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 92/20519 A1 (ALLIED SIGNAL INC [US]) 26 November 1992 (1992-11-26) page 27, line 14 - line 19 -----	1-24

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No PCT/US2012/037305

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2009270904	A1	29-10-2009	AU 2009240634 A1
			CA 2722516 A1
			EP 2303200 A1
			JP 2011518617 A
			KR 20110014158 A
			US 2009270904 A1
			WO 2009132127 A1

US 2011054407	A1	03-03-2011	AU 2010289968 A1
			CA 2772543 A1
			EP 2470128 A1
			US 2011054407 A1
			WO 2011028370 A1

WO 0210667	A2	07-02-2002	AU 785345 B2
			AU 7587601 A
			BR 0106945 A
			CA 2384335 A1
			CN 1398342 A
			EP 1299684 A2
			IL 148552 A
			JP 2004504966 A
			MX PA02002456 A
			US 6962739 B1
			US 2005170221 A1
			US 2009142535 A1
			WO 0210667 A2

US 2001052141	A1	20-12-2001	AU 4487601 A
			US 2001052141 A1
			WO 0167902 A2

WO 9220519	A1	26-11-1992	US 5316820 A
			WO 9220519 A1
