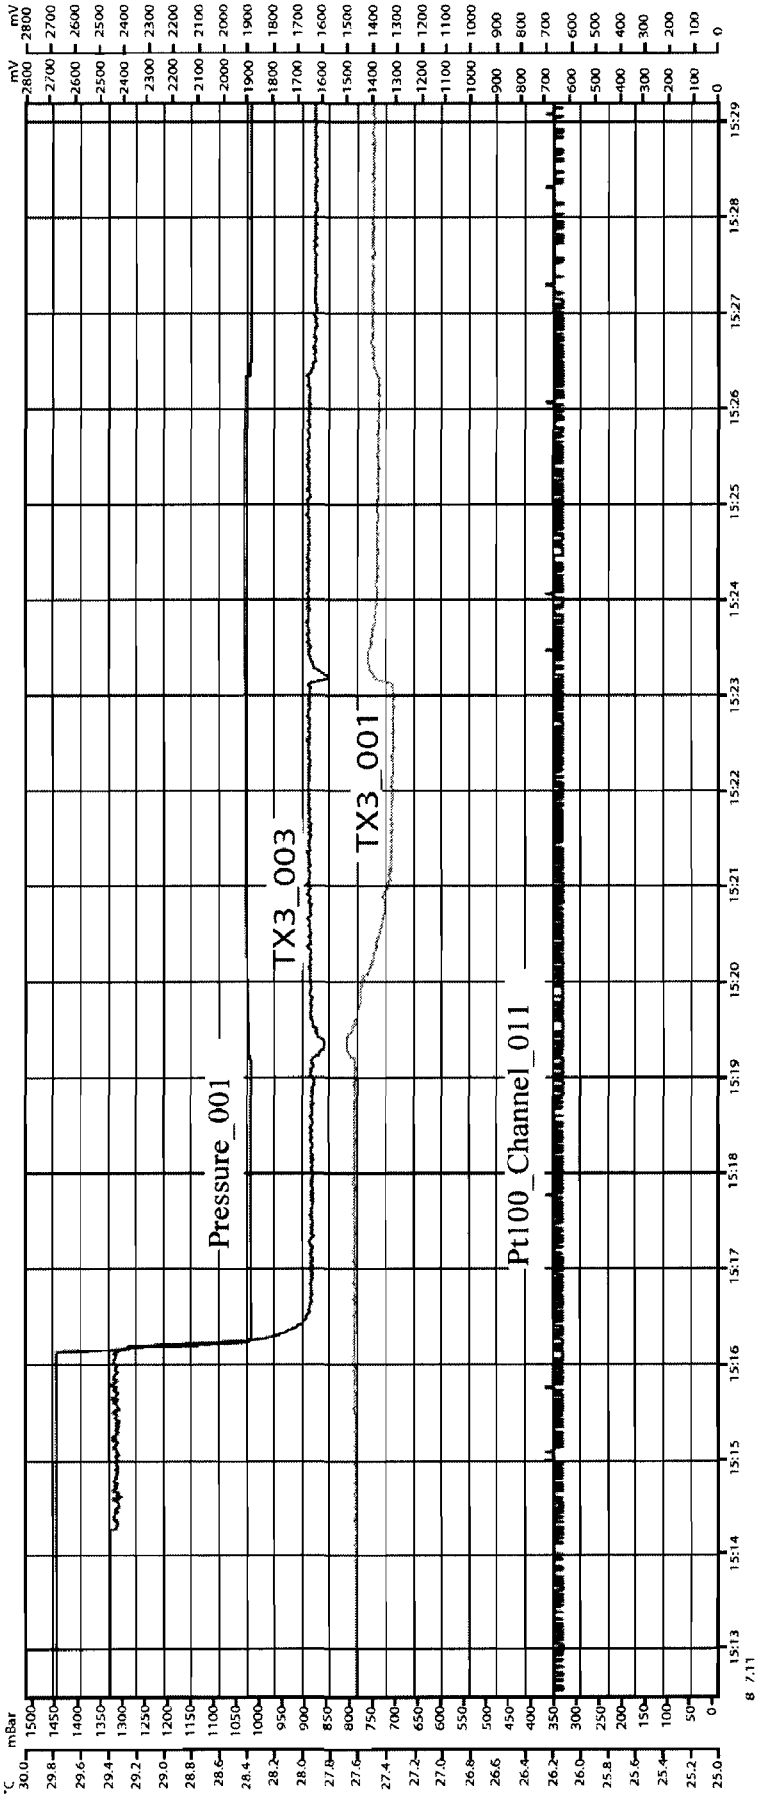


Figure 2

Environment	25.6 °C	1017 mbar 762.9407352 Torr	38.1 % rel. Humidity
Measuring devices:	Cronos PL3	Pressure_001 abs. Reactor	Pressure_002 abs. Environment O2-004
	Microx TX 3 001		Pressure_003 abs.
	Microx TX 3 002		
	Microx TX 3 003	O2-003	



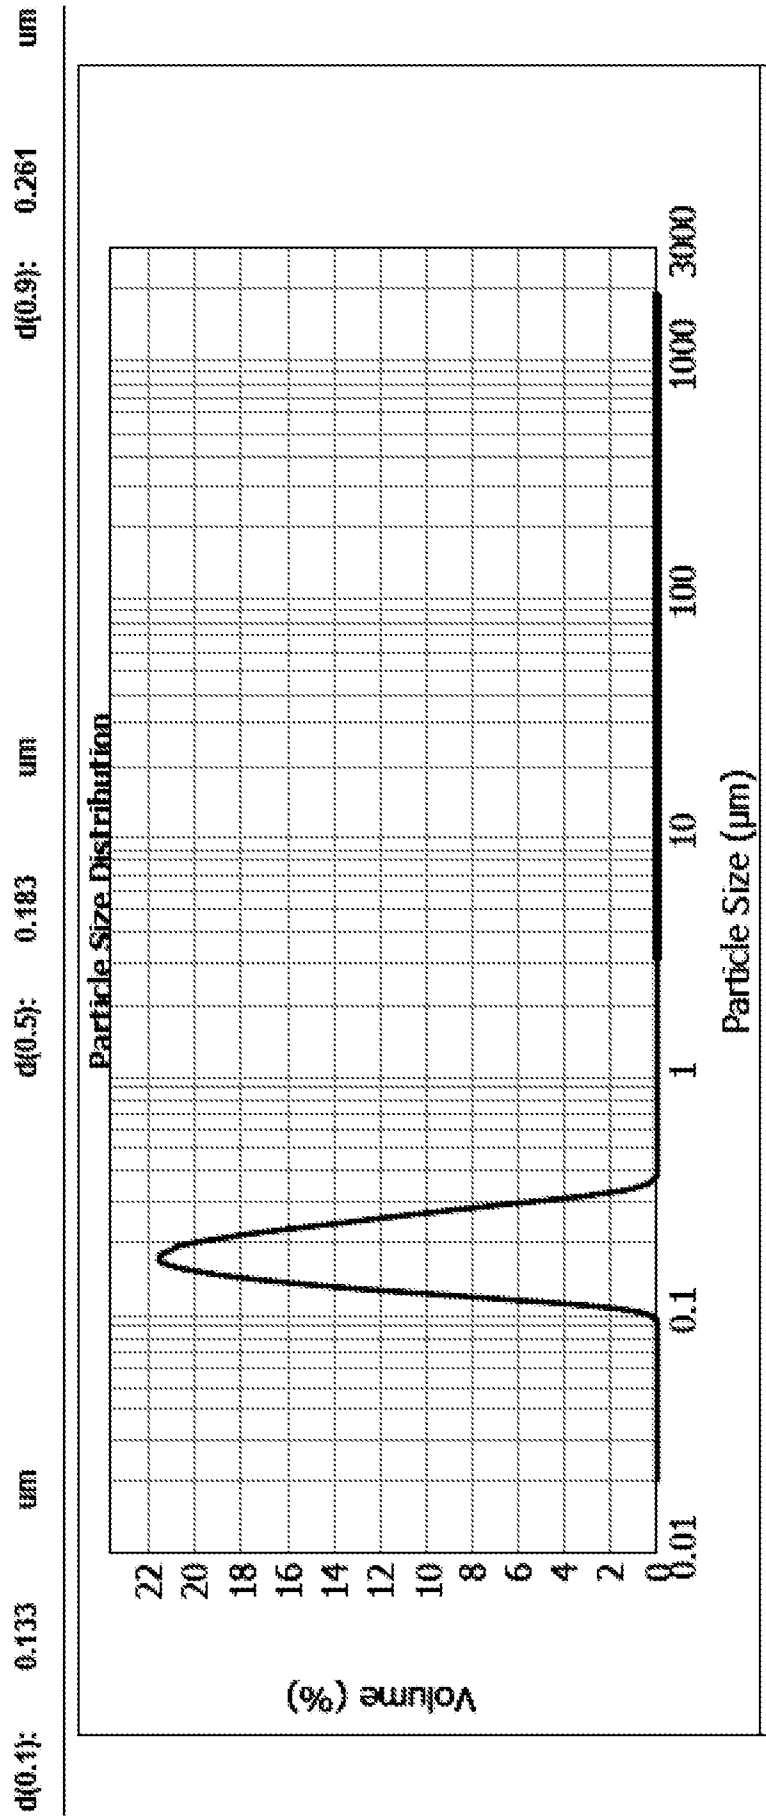


FIGURE 3

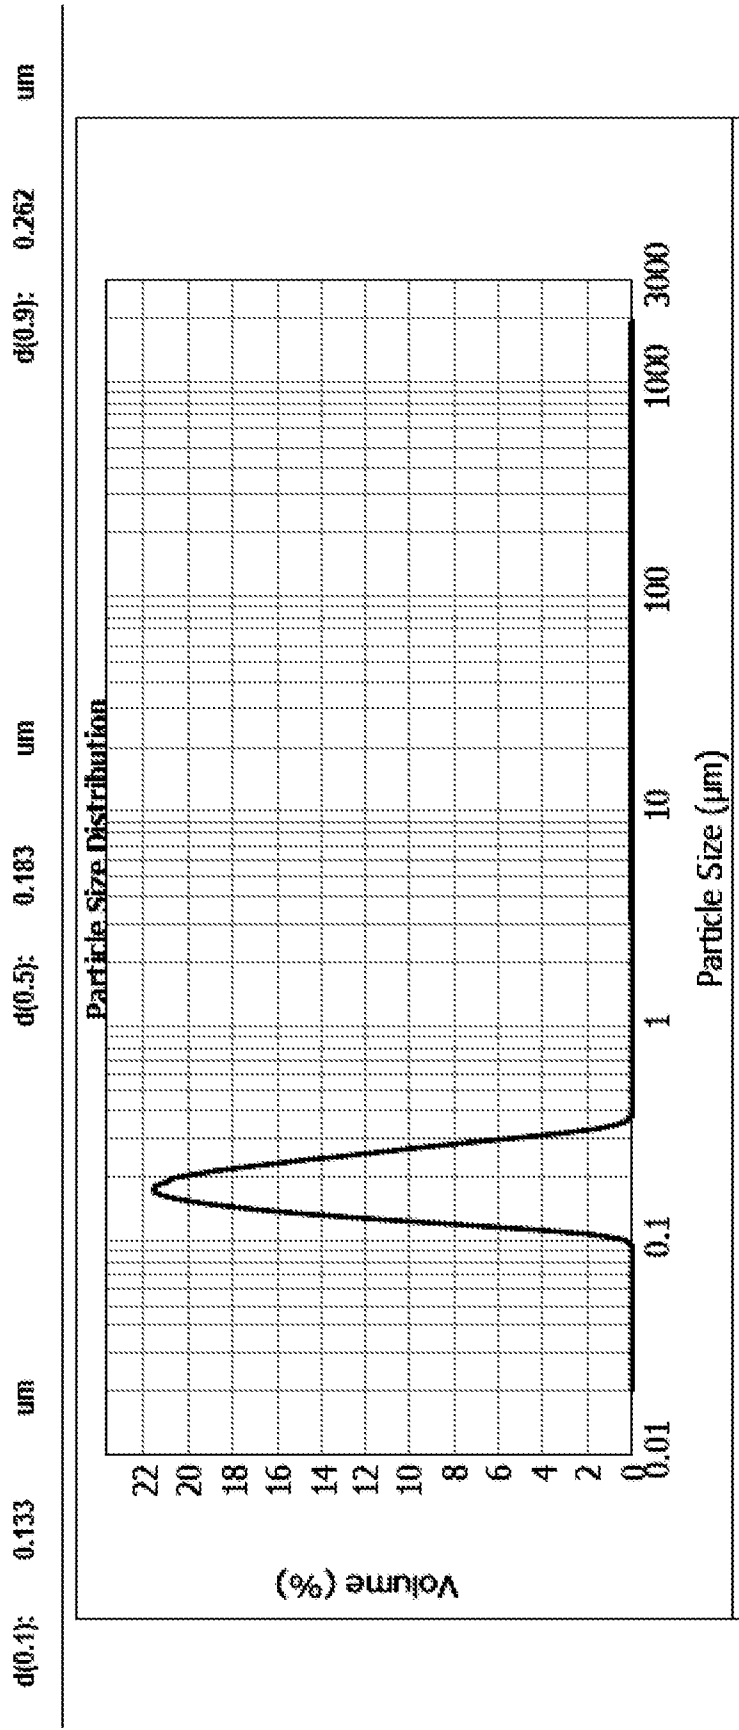


FIGURE 4

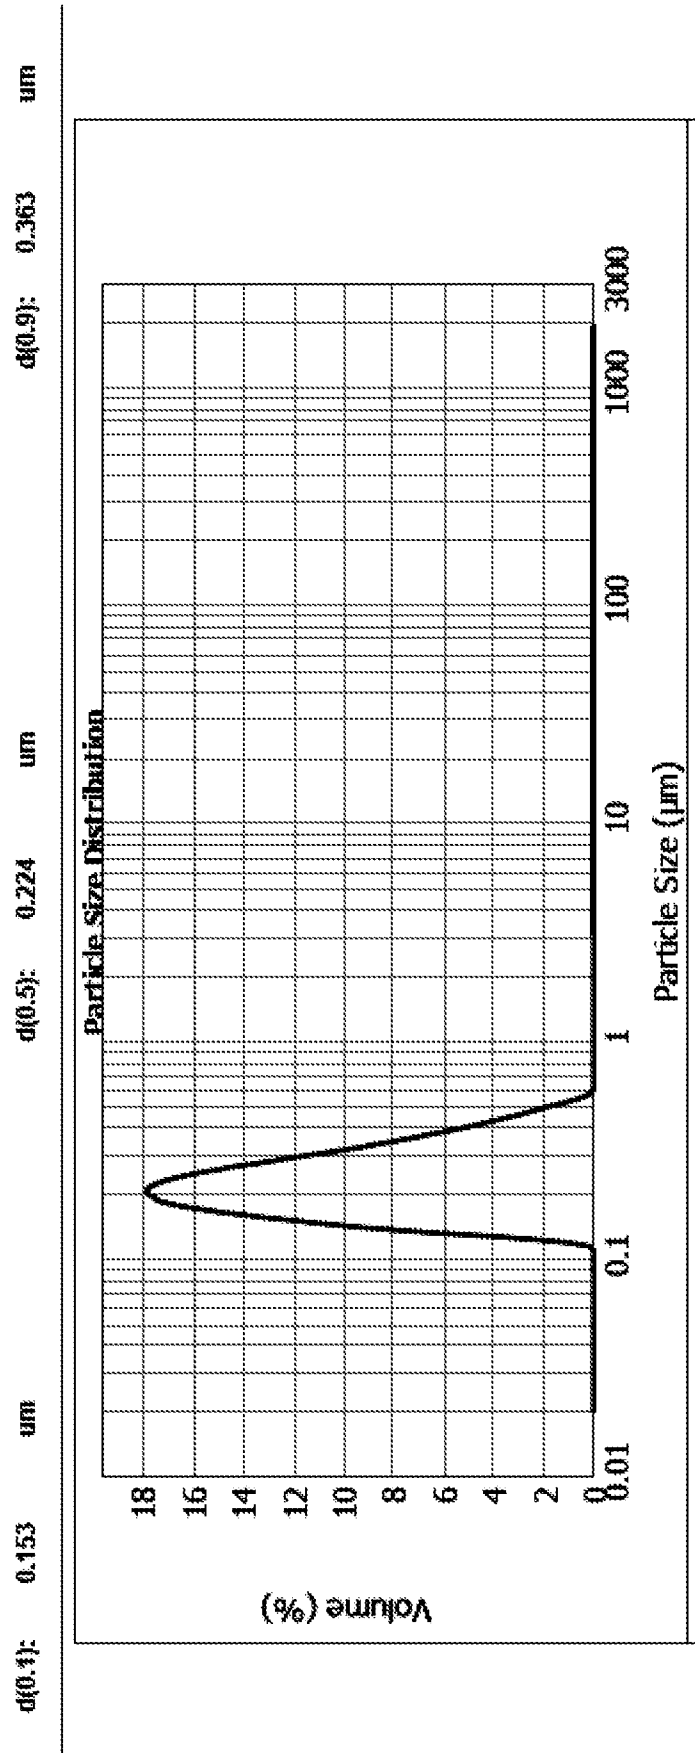


FIGURE 5

d(0.1): 0.158 μm d(0.5): 0.236 μm d(0.9): 0.401 μm

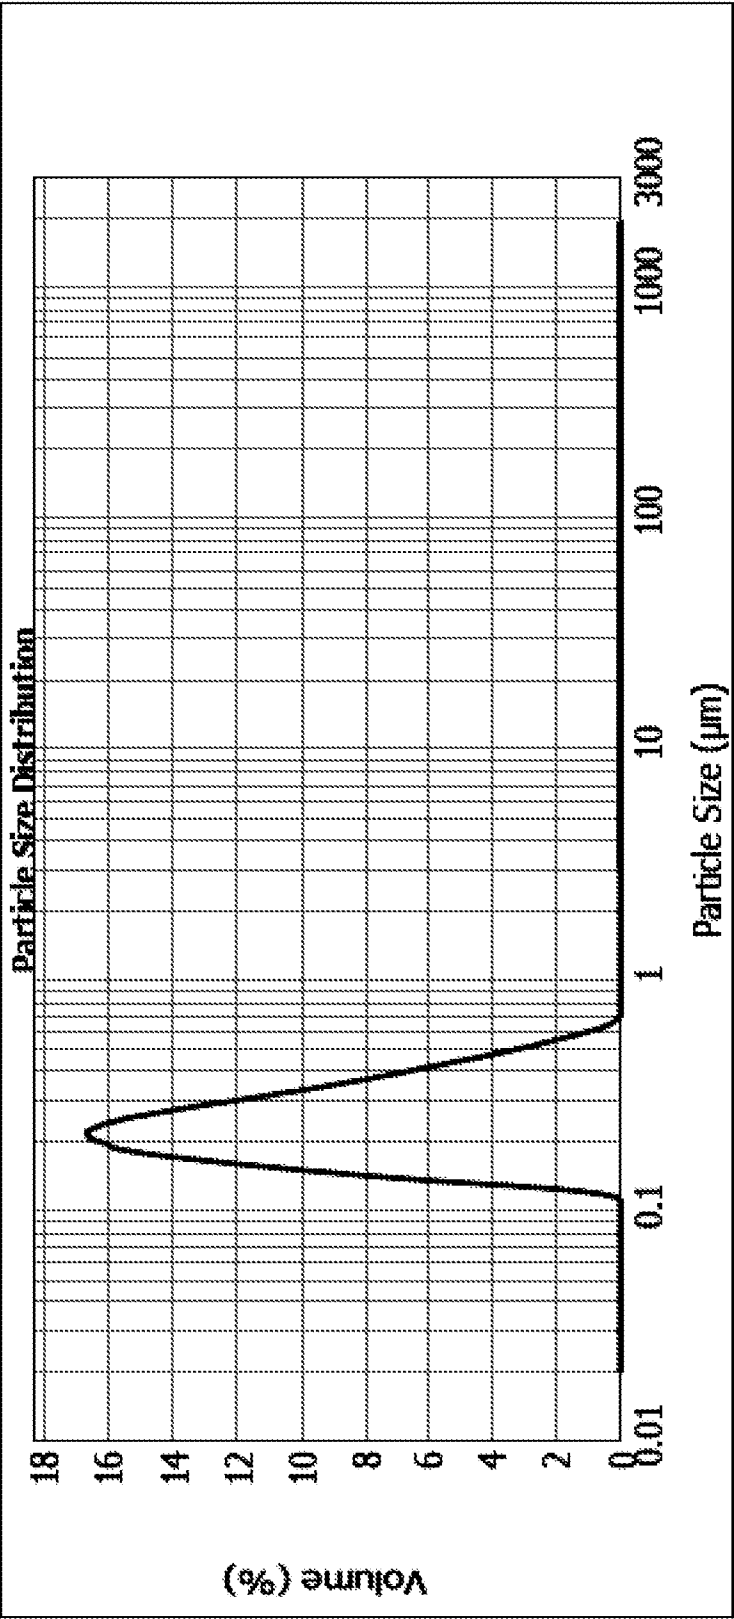


FIGURE 6