

(19) World Intellectual Property Organization  
International Bureau




(43) International Publication Date  
5 April 2001 (05.04.2001)

PCT

(10) International Publication Number  
**WO 01/23039 A1**

- (51) International Patent Classification<sup>7</sup>: **A61N 1/36**
- (21) International Application Number: PCT/US00/26616
- (22) International Filing Date:  
28 September 2000 (28.09.2000)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:  
09/409,018 29 September 1999 (29.09.1999) US
- (71) Applicant: **PI MEDICAL, INC.** [US/US]; 2800 Patton Road, St. Paul, MN 55113 (US).
- (74) Agent: **BRUESS, Steven, C.**; Merchant & Gould P.C., P.O. Box 2903, Minneapolis, MN 55402-0903 (US).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).
- Published:**  
— With international search report.
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.
- (72) Inventors: **KNUDSON, Mark, B.**; 1309 West Royal Oaks Drive, Shoreview, MN 55126 (US). **NICKOLOFF, Robert, S.**; 1525 Summit Avenue, St. Paul, MN 55105 (US). **CONRAD, Timothy, R.**; 6903 Ros Emily Lane, Eden Prairie, MN 55344 (US).

(54) Title: **IMPLANTABLE STIMULATION DEVICE FOR SNORING TREATMENT**

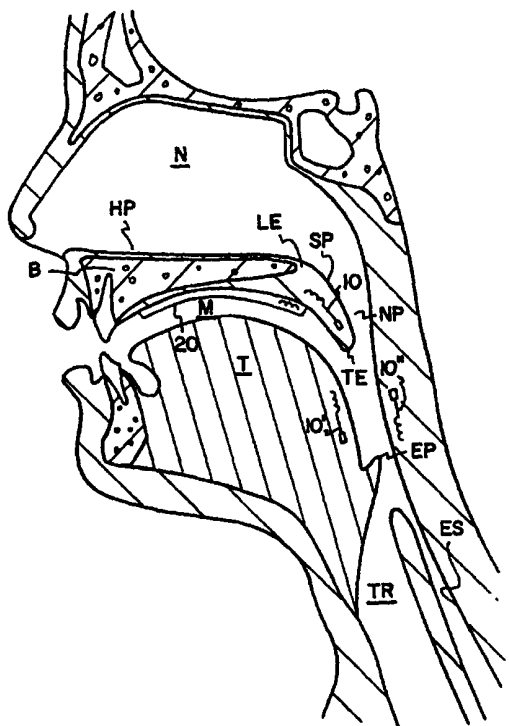

(57) Abstract: The present disclosure relates to methods and apparatuses for treating snoring by implanting a stimulating electrode into a patient. The electrode is placed in stimulating contact with an airway passage-controlling muscle of the patient. The electrode is energized to contract the muscle and alter the airway passage.



WO 01/23039 A1

## IMPLANTABLE STIMULATION DEVICE FOR SNORING TREATMENT

### BACKGROUND

#### 1. Field of the Invention

5                   This invention is directed to method and apparatus for treating snoring.

#### 2. Description of the Prior Art

                  Snoring has received increased scientific and academic attention. One publication estimates that up to 20% of the adult population snores habitually. Huang, et al., "Biomechanics of Snoring", Endeavour, Vol. 19, No. 3, pp. 96 – 100 (1995). Snoring can be a serious cause of marital discord. In addition, snoring can present a serious health risk to the snorer. In 10% of habitual snorers, collapse of the airway during sleep can lead to obstructive sleep apnea syndrome. Id.

15                   Notwithstanding numerous efforts to address snoring, effective treatment of snoring has been elusive. Such treatment may include mouth guards or other appliances worn by the snorer during sleep. However, patients find such appliances uncomfortable and frequently discontinue use (presumably adding to marital stress).

20                   Surgical treatments have been employed. One such treatment is uvulopalatopharyngoplasty. In this procedure, so-called laser ablation is used to remove about 2 cm of the trailing edge of the soft palate thereby reducing the soft palate's ability to flutter between the tongue and the pharyngeal wall of the throat. The procedure is frequently effective to abate snoring but is painful and frequently results in undesirable side effects. Namely, removal of the soft palate trailing edge comprises the soft palate's ability to seal off nasal passages during swallowing and speech. In an estimated 25% of uvulopalatopharyngoplasty patients, fluid escapes from the mouth into the nose while drinking. Huang, et al., supra at 99. Uvulopalatopharyngoplasty (UPPP) is also described in Harries, et al., "The Surgical treatment of snoring", Journal of Laryngology and Otology, pp. 1105 – 1106 (1996) which describes removal of up to 1.5 cm of the soft palate. Assessment of snoring treatment is discussed in Cole, et al., "Snoring: A review and a Reassessment", Journal of Otolaryngology, pp. 303 – 306 (1995).

30                   Huang, et al., supra, describe the soft palate and palatal snoring as an oscillating system which responds to airflow over the soft palate. Resulting flutter of the soft palate (rapidly opening and closing air passages) is a dynamic response generating sounds associated with snoring. Huang, et al., propose an alternative to uvulopalatopharyngoplasty. The proposal includes using a surgical laser to create

scar tissue on the surface of the soft palate. The scar is to reduce flexibility of the soft palate to reduce palatal flutter. Huang, et al., report initial results of complete or near-complete reduction in snoring and reduced side effects.

5 Surgical procedures such as uvulopalatopharyngoplasty and those proposed by Huang, et al., continue to have problems. The area of surgical treatment (i.e., removal of palatal tissue or scarring of palatal tissue) may be more than is necessary to treat the patient's condition. Surgical lasers are expensive. The proposed procedures are painful with drawn out and uncomfortable healing periods. The procedures have complications and side effects and variable efficacy (e.g.,  
10 Huang, et al., report promising results in 75% of patients suggesting a full quarter of patients are not effectively treated after painful surgery). The procedures may involve lasting discomfort. For example, scar tissue on the soft palate may present a continuing irritant to the patient. Importantly, the procedures are not reversible in the event they happen to induce adverse side effects not justified by the benefits of  
15 the surgery.

Electrical stimulation of the soft palate has been suggested to treat snoring and obstructive sleep apnea. See, e.g., Schwartz, et al., "Effects of electrical stimulation to the soft palate on snoring and obstructive sleep apnea", J. Prosthetic Dentistry, pp. 273 – 281 (1996). Devices to apply such stimulation are described in  
20 U.S. Pat. Nos. 5,284,161 and 5,792,067. Such devices are appliances requiring patient adherence to a regimen of use as well as subjecting the patient to discomfort during sleep. Alternatively, these devices must be used during the day for a period of time causing disruption of daily activity, interference with daily life. This may generally be assumed to cause them to be prone to a significant risk of non-  
25 compliance by the wearer. Such devices, though have met with some success in treating disorders such as snoring and Obstructive Sleep Apnea.

### SUMMARY OF THE INVENTION

30 According to a preferred embodiment of the present invention, a method and apparatus are disclosed for treating snoring of a patient. The invention includes implanting a stimulating electrode into a patient. The electrode is placed in stimulating contact with an airway passage-controlling muscle of the patient. The electrode is energized to contract the muscle and alter the airway passage.

### BRIEF DESCRIPTION OF THE DRAWINGS

35 Fig. 1 is a side sectional view of a portion of a human head showing a soft palate in a relaxed state and in relation in adjacent anatomical features;

Fig. 2 is a portion of the view of Fig. 1 showing the soft palate in a flexed state;

Fig. 3 is a front view of an interior of the mouth shown in Fig. 1 and showing an area to be ablated according to a first prior art surgical procedure;

5 Fig. 4 is the view of Fig. 3 and showing an area to be scarred according to a second prior art surgical procedure;

Fig. 5 is a schematic representation of a spring-mass system model of the soft palate;

10 Fig. 6 is the view of Fig. 1 showing electrodes placed in the muscles of the soft palate, tongue and throat; and

Fig. 7 is a schematic representation of a pacing electrode inductively coupled to a control device.

#### DESCRIPTION OF THE PREFERRED EMBODIMENT

15 For ease of understanding the present invention, the dynamics of snoring are explained with reference to Figs. 1 – 5. The hard palate HP overlies the tongue T and forms the roof of the mouth M. The hard palate HP includes a bone support B and does not materially deform during breathing. The soft palate SP is soft and is made up of mucous membrane, fibrous and muscle tissue extending  
20 rearward from the hard palate HP. A leading end LE of the soft palate SP is anchored to the trailing end of the hard palate HP. A trailing end TE of the soft palate SP is unattached. Since the soft palate SP is not structurally supported by bone or hard cartilage, the soft palate SP droops down from the plane of the hard palate HP in an arcuate geometry of repose.

25 The pharyngeal airway passes air from the mouth M and the nasal passages N into the trachea TR. The portion of the pharyngeal airway defined between opposing surfaces of the upper surface of the soft palate SP and the wall of the throat is the nasopharynx NP.

30 During normal breathing, the soft palate SP is in the relaxed state shown in Fig. 1 with the nasopharynx NP unobstructed and with air free to flow into the trachea TR from both the mouth M and the nostrils N.

35 During swallowing, the soft palate SP flexes and extends (as shown in Fig. 2) to close the nasopharynx NP thereby preventing fluid flow from the mouth M to the nasal passages N. Simultaneously, the epiglottis EP closes the trachea TR so that food and drink pass only into the esophagus ES and not the trachea TR. The soft palate SP is a valve to prevent regurgitation of food into the nose N. The soft palate SP also regulates airflow through the nose N while talking. Since the soft

palate SP performs such important functions, prior art techniques for surgically altering the soft palate SP can compromise these functions.

The majority of snoring is caused by the soft palate SP flapping back and forth. If breathing is solely through the nose N with the mouth closed, the trailing edge TE of the soft palate SP is sucked into the nasopharyngeal space NP obstructing the airway and subsequently falls opening the airway in a repeating cycle. When the mouth is open, air flows over the upper and lower surfaces of the soft palate SP causing the soft palate SP to flap up and down alternating in obstructing the oral and nasal passageways M, N. The snoring sound is generated by impulses caused by rapid obstruction and opening of airways. Huang, et al., state the airway passage opening and closing occurs 50 times per second during a snore. Huang, et al., utilizing a spring-mass model (Fig. 5) to illustrate oscillation of the soft palate in response to airflow (where the soft palate is the ball B of mass depending by a spring S from a fixed anchor A).

Huang, et al., analogize the shortening of the soft palate SP in uvulopalatopharyngoplasty as effectively raising the critical air flow speed at which soft palate flutter will occur. The shaded area SA in Fig. 3 shows the area of the trailing end TE of the soft palate SP to be removed during this procedure. The alternative procedure proposed by Huang, et al., reduces the flexibility of the soft palate SP through surface scarring which is asserted as effecting the critical flow speed. The shaded area SA' in Fig. 4 shows the area to be scarred by this alternate procedure. In Fig. 4, dashed line L shows the demarcation between the soft and hard palates.

The present invention is directed to a method and apparatus for altering the dynamic response of the soft palate by altering airflow past the soft palate. With reference to the spring-mass model (Fig. 5), the soft palate is moved by airflow. Airflow through an orifice varies in response to the orifice size. The present invention alters the size of the air passage through a minimally invasive surgical implant to allow stimulation of airway defining muscles of the oro-pharynx (i.e., mouth and throat).

The present invention stimulates muscles of one or more of the soft palate SP, tongue T and back of the throat. In the soft palate SP, these muscles include, but are not limited to, the Levator veli palatini, the dextera, the Palatopharyngeous and the Palatoglossus muscles. At the back of the throat, these muscles include, but are not limited to, the Superior, Middle and Inferior pharyngeal constrictor, the Salpingopharyngeous and the Stylopharyngeous muscles. In the tongue T, these muscles include, but are not limited to, the Genioglossus and Geniohyoid muscles.

Stimulating the muscles of the soft palate, tongue and throat is intended to alter the dynamic response of the soft palate to airflow. Namely, stimulation of the soft palate SP causes the soft palate to move away from the tongue T, stimulation of the tongue T causes the tongue T to move away from the soft  
5 palate SP, and stimulation of the back of the throat causes the throat to move rearwardly. Alone or in combination, these actions increase the size of the airway thereby decreasing air velocity and the disrupting force which would otherwise cause oscillation of the soft palate SP.

Stimulation of the muscles is accomplished by implanted electrodes  
10 10, 10' and 10'' placed in the airway passage-defining muscles (identified above) of the soft palate SP, tongue T and back of throat (as illustrated in Fig. 6). Implantable muscle stimulating electrodes are well known and may be such as those used in cardiac pacing.

The implant 10, 10', 10'' can be positioned and stimulated in a  
15 plurality of ways to alter the shape of the airway, to change the dynamic response of the airway tissues or a combination of both. Unlike the prior art surgical techniques, the electrodes 10, 10', 10'' that will be described are easy to insert in a small incision resulting in reduced patient discomfort and are not exposed to the interior of the mouth (such as the surface scarring of Huang, et al.) as a patient irritant. Also, as  
20 will be described, the degree of dynamic remodeling and stimulation pattern can be fine tuned avoiding the need for excessive anatomical modification and are reversible in the event of adverse consequences.

The present invention permits the surgeon to apply stimulation to various muscles until the desired alteration in airway area and tone is achieved so  
25 that snoring inducing oscillation is abated at normal airflow. The individual electrodes 10, 10', 10'' may be placed into the soft palate, tongue or throat muscles through small individual incisions closed by sutures which is much less traumatic than the gross anatomical destruction of uvulopalatopharyngoplasty or the large surface area scarring proposed by Huang, et al.

30 A control device 20 is provided for controlling the electrodes 10, 10', 10''. The control device 20 is shown as a removable appliance (schematically shown in Fig. 6 with it being appreciated that appliances for placement in the mouth are well known) which fits the form of the hard palate or sub-lingual spaces.

The control device 20 is electrically coupled to the electrodes 10, 10',  
35 10'' through electromagnetic coupling which avoids the need for electrode leads being exposed from the implants 10, 10', 10''. Specifically, the electrode 10 (shown in Fig. 7 and it being appreciated that electrodes 10', 10'' are of similar construction) includes a pacing electrode 12 for stimulating muscle in response to a

signal through the electrode 10. Leads 14 connect the pacing electrode 12 to an inductive winding 16. In use, the entire electrode 10 (i.e., each of the components of the pacing electrode 12, leads 14 and winding 16) are imbedded in the patient and not exposed.

5           The control device 20 is shown schematically and includes an inductive winding 22 connected to a control circuit 24. Control circuit 24 is only shown schematically. Control circuits for pacing electrodes are well known and widely used in cardiac pacing. In the present invention, preferably none of the components of the control device 20 (i.e., the winding 22 and circuit 24) are  
10           implanted. Instead, preferably such components are contained in the removable oral appliance control device 20 although some elements (e.g., a battery may be worn externally by the patient).

          The control winding 22 is positioned on the control device 20 to be inductively coupled to the electrode winding 16 when the control device 20 is in  
15           place. In the event multiple electrodes 10, 10', 10'' are placed in multiple muscles, the control device 20 may contain a plurality of windings 22 each uniquely tuned to the windings of the electrodes 10, 10', 10'' such that each electrode 10, 10', 10'' may be uniquely paced. Also, each of the electrodes 10, 10', 10'' can be provided with filter circuits to pass only desired signals to the pacing electrodes.

20           The control device 20 sends a pulsatile signal to the electrode 10 through the inductive coupling of windings 16 and 22. In response, the electrode 10 causes pacing contraction of the muscle. Preferably, the pacing is selected to contract the muscle up to and including tetanic contraction.

          With the present invention, the muscle is contracted to increase the  
25           size of the airway and reduce palatal flutter. The amount of pacing can be tuned to the unique physiology of the patient. The control device need only be used during sleep. It is anticipated that regular use of the control device 20 results in improved tone of the paced muscles reducing or eliminating future need to use the control device 20. Unlike the appliances of U.S. Pat. Nos. 5,284,161 and 5,792,067, the  
30           present device has more effective pacing since muscles are being paced directly by implanted electrodes rather than through less efficient surface stimulation. Further, the present invention contemplates pacing of all muscles defining the airway passage and not just the soft palate.

          Having described the invention, alternatives and embodiments may  
35           occur to one of skill in the art. It is intended that such modifications and equivalents shall be included within the scope of the following claims.

What is claimed is:

1. A method for treating snoring comprising:  
implanting a stimulating electrode into a patient with said electrode in  
stimulating contact with an airway passage-controlling muscle of said patient;  
and  
energizing said electrode to contract said muscle and alter said airway  
passage.
2. A method according to claim 1 wherein said electrode is energized by  
electrically coupling said electrode through an electromagnetic field to a  
controller not implanted in said patient.
3. A method according to claim 2 wherein said controller is contained with an  
appliance sized to be removably placed within a mouth cavity of said patient  
and with said controller electrically coupled to said electrode when said  
appliance is placed within said mouth cavity.
4. A method according to claim 1 wherein said muscle is a muscle of the soft  
palate.
5. A method according to claim 1 wherein said muscle is a muscle of the tongue.
6. A method according to claim 1 wherein said muscle is a muscle of the  
pharynx.
7. A method according to claim 4 wherein said muscle is selected from at least  
one of the Levator veli palatini, the Palatopharyngeous and the Palatoglossus  
muscles.
8. A method according to claim 5 wherein said muscle is selected from at least  
one of the Genioglossus and Geniohyoid muscles.
9. A method according to claim 6 wherein said muscle is selected from at least  
one of the Superior, Middle and Inferior pharyngeal constrictor, the  
Salpingopharyngeous and the Stylopharyngeous muscles.



10. An apparatus for treating snoring of a patient, said apparatus comprising:  
a stimulating electrode adapted to be implanted into a patient with  
said electrode in stimulating contact with an airway passage-controlling muscle  
5 of said patient; and  
a control member for energizing said electrode to contract said  
muscle and alter said airway passage
11. An apparatus according to claim 10 wherein said electrode and control member  
10 include cooperating components for inductively coupling said control member  
and said electrode.
12. An apparatus according to claim 11 wherein said control member is carried on  
an appliance adapted to be removably placed, non-invasively in mouth of said  
15 patient.

FIG. 1

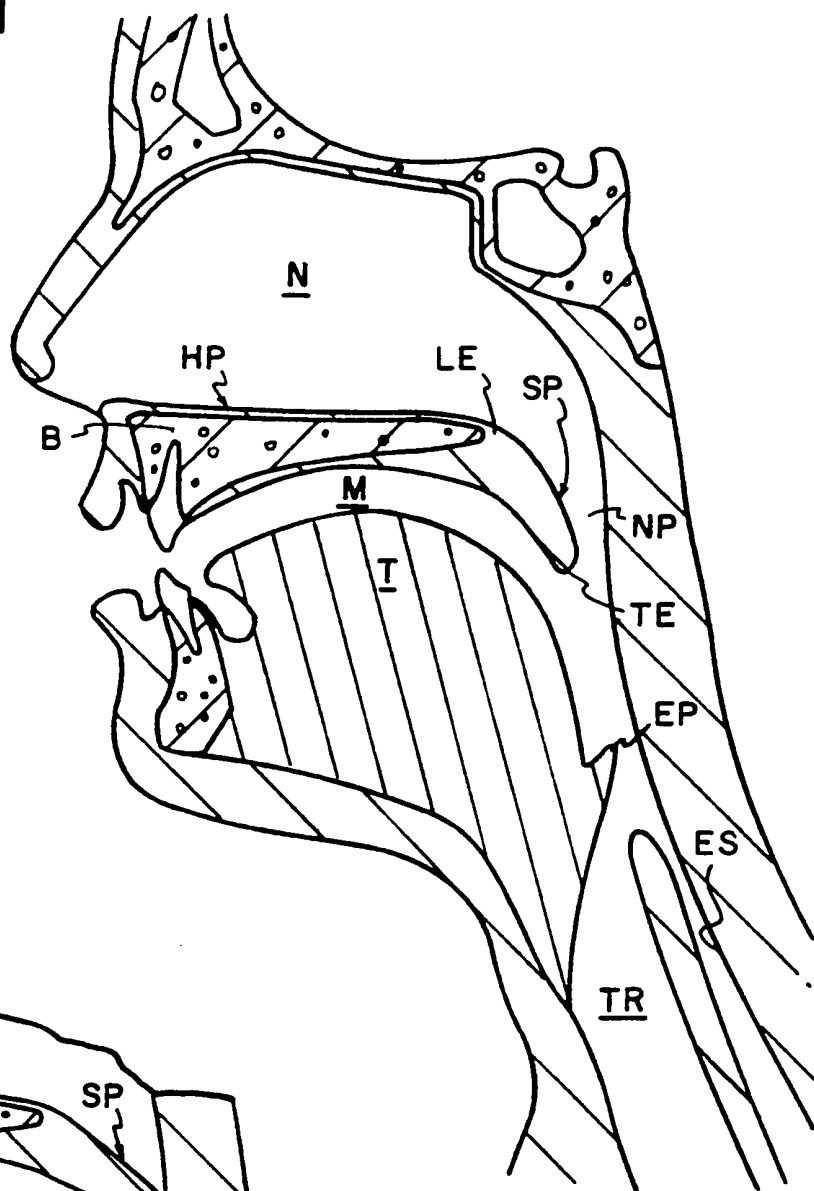


FIG. 2

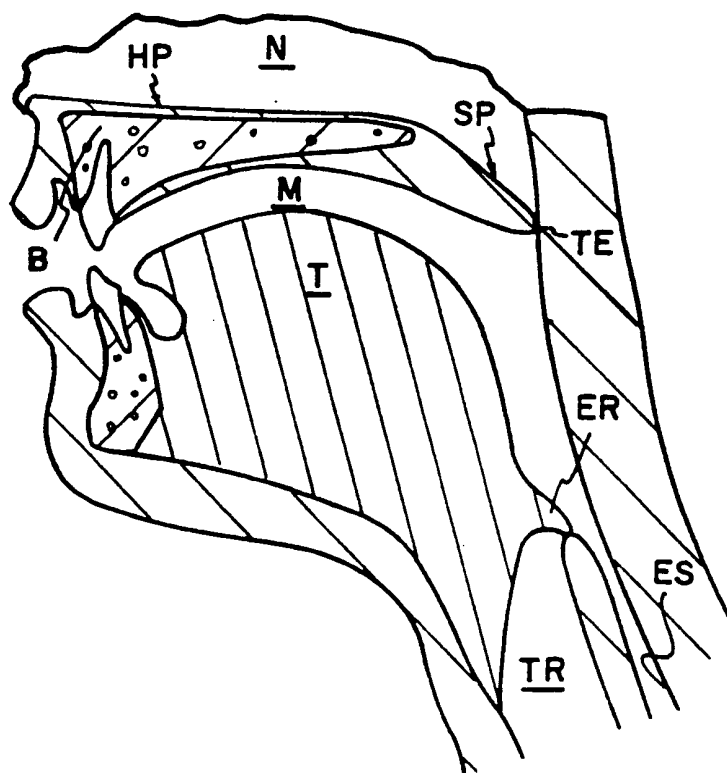


FIG. 3

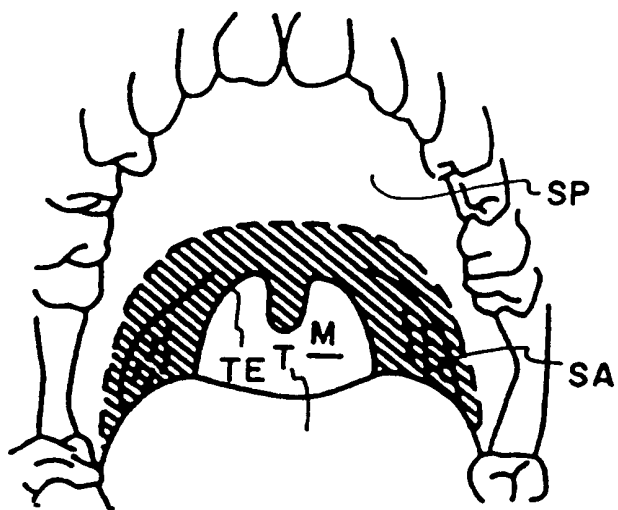


FIG. 4

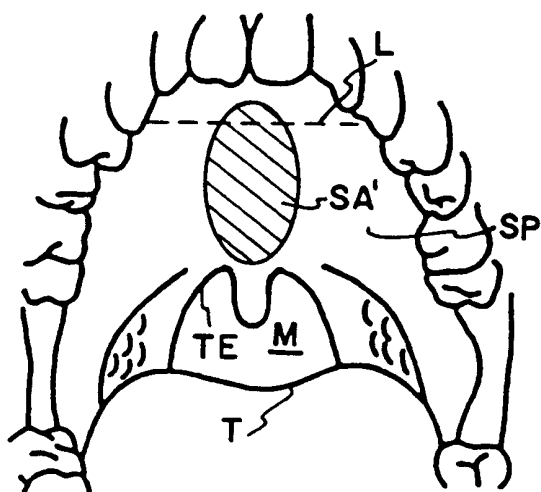


FIG. 5

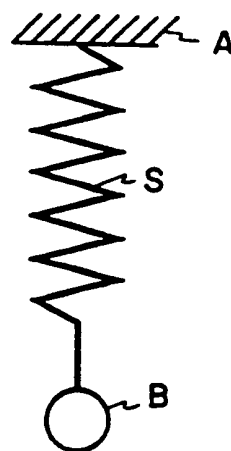


FIG. 7


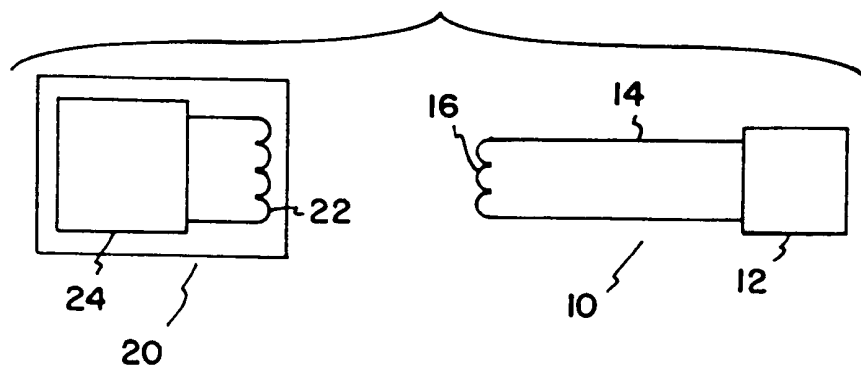


FIG. 6

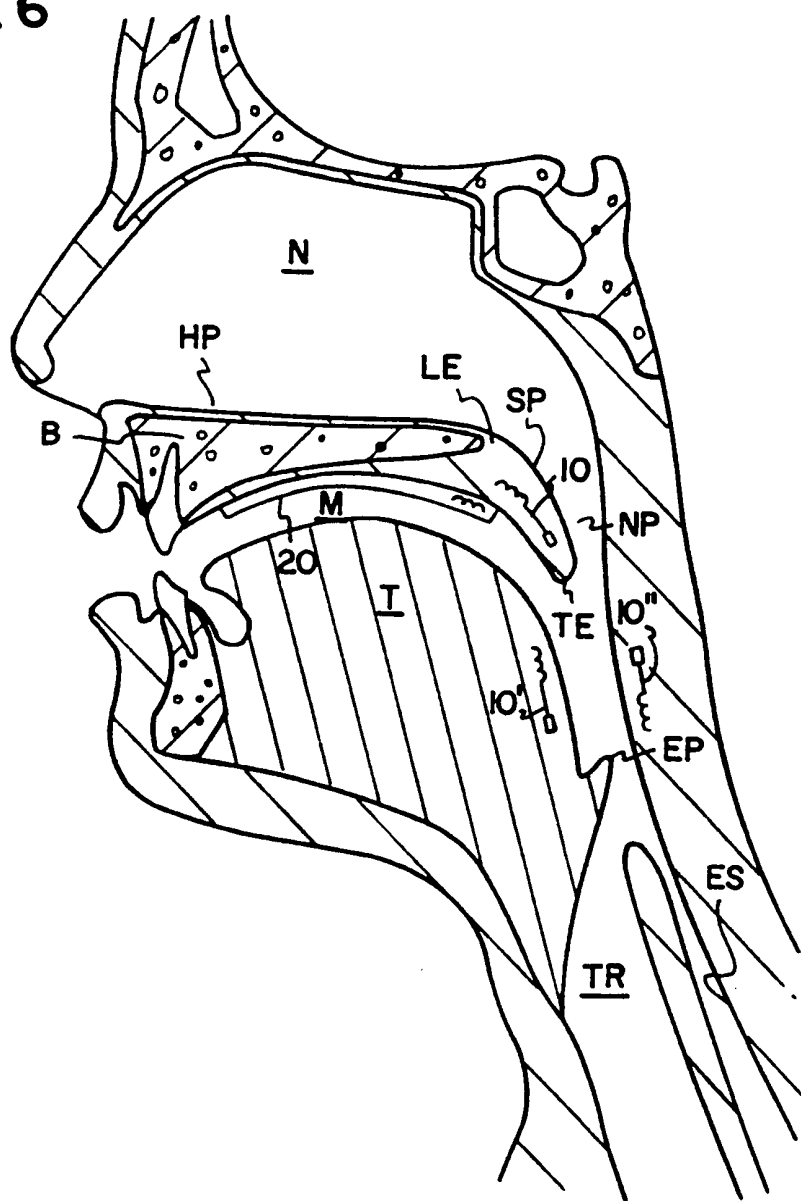

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 00/26616

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61N1/36

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category °	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 830 008 A (MEER JEFFREY A) 16 May 1989 (1989-05-16) the whole document	10
Y	---	11,12
Y	EP 0 706 808 A (MEDTRONIC INC) 17 April 1996 (1996-04-17) column 12, line 45 - line 53; figure 5	11,12
A	US 5 792 067 A (KARELL MANUEL L) 11 August 1998 (1998-08-11) cited in the application the whole document	10-12
A	US 5 284 161 A (KARELL MANUEL L) 8 February 1994 (1994-02-08) cited in the application the whole document	10-12



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

° Special categories of cited documents :

\*A\* document defining the general state of the art which is not considered to be of particular relevance

\*E\* earlier document but published on or after the international filing date

\*L\* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

\*O\* document referring to an oral disclosure, use, exhibition or other means

\*P\* document published prior to the international filing date but later than the priority date claimed

\*T\* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

\*X\* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

\*Y\* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

\*G\* document member of the same patent family

Date of the actual completion of the international search

6 December 2000

Date of mailing of the international search report

14/12/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Ferrigno, A

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 00/26616

Patent document cited in search report		Publication date	Patent family member(s)		Publication date
US 4830008	A	16-05-1989	CA 1323069	A	12-10-1993
EP 0706808	A	17-04-1996	US 5549655	A	27-08-1996
			JP 9187521	A	22-07-1997
US 5792067	A	11-08-1998	AU 1120297	A	11-06-1997
			EP 0874662	A	04-11-1998
			WO 9718854	A	29-05-1997
US 5284161	A	08-02-1994	US RE36120	E	02-03-1999