

(51) International Patent Classification:
A61B 3/10 (2006.01) *G01B 9/02* (2006.01)(21) International Application Number:
PCT/US2013/059047(22) International Filing Date:
10 September 2013 (10.09.2013)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
61/699,257 10 September 2012 (10.09.2012) US
61/799,502 15 March 2013 (15.03.2013) US

(71) Applicant: OREGON HEALTH & SCIENCE UNIVERSITY [US/US]; Office of Technology Transfer and Business Development, 690 SW Bancroft Street, Mail Code L106TT, Portland, OR 97239 (US).

(72) Inventors: HUANG, David; 0841 SW Gaines Street, Unit 1712, Portland, OR 97239-3104 (US). JIA, Yali; 4498 NW Oakpoint Way, Portland, OR 97229 (US). TOKAY-ER, Jason; 2729 East Pershing Court, Visalia, CA 93292 (US). TAN, Ou; 4685 NW Moretti Terrace, Portland, OR 97229 (US).

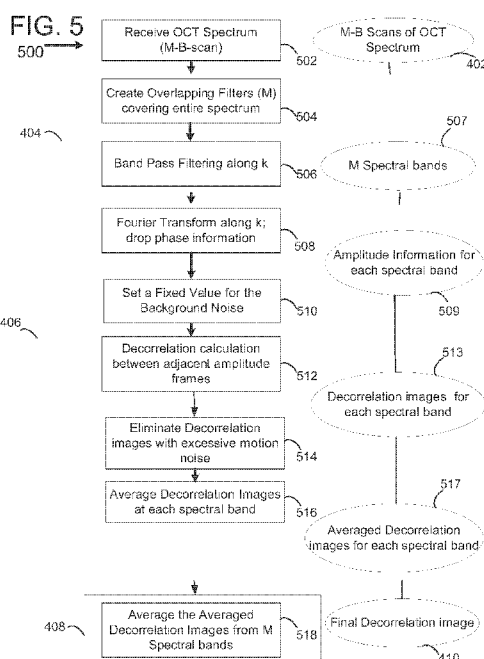
(74) Agents: PREWITT, Steven, J. et al.; Schwabe, Williamson & Wyatt, P.C., Pacwest Center, Suite 1900, 1211 SW 5th Avenue, Suite 1900, Portland, OR 97204 (US).

(81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

(84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: QUANTIFICATION OF LOCAL CIRCULATION WITH OCT ANGIOGRAPHY



(57) Abstract: Impaired intraocular blood flow within vascular beds in the human eye are associated with certain ocular diseases including, for example, glaucoma, diabetic retinopathy and age-related macular degeneration. A reliable method to quantify blood flow in one or more of the various intraocular vascular beds could provide insight into the vascular component of ocular disease pathophysiology. Using ultrahigh-speed optical coherence tomography (OCT), a new 3D angiography algorithm called split-spectrum amplitude-decorrelation angiography (SSADA) was developed for imaging microcirculation within different intraocular regions including, for example, the ocular disc, the temporal ellipse, the peripapillary retina, the peripapillary choroid, the macular retina, the macular choroid, the fovea avascular zone, and the area of non-perfusion. As described herein, a method to quantify SSADA results was developed and used to detect perfusion changes in early stage ocular disease. Associated embodiments relating to methods for quantitatively measuring blood flow at various intraocular vasculature sites, systems for practicing such methods, and use of such methods and systems for diagnosing certain ocular diseases are herein described.



Published:

— with international search report (Art. 21(3))

— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

QUANTIFICATION OF LOCAL CIRCULATION WITH OCT ANGIOGRAPHY

CROSS-REFERENCE TO RELATED APPLICATIONS

5 The present application claims benefit of U.S. Provisional Patent Application No. 61/699,257 filed September 10, 2012, entitled "QUANTIFICATION OF LOCAL CIRCULATION WITH OCT ANGIOGRAPHY", and to U.S. Provisional Patent Application No. 61/799,502 filed March 15, 2013, entitled "IN VIVO QUANTITATIVE OPTICAL FLOW IMAGING". Priority to these provisional applications is expressly
10 claimed, and the disclosures of these provisional applications are herein incorporated by reference in their entirety.

TECHNICAL FIELD

 This disclosure relates generally to the field of biomedical imaging, and more
15 specifically to methods, apparatuses, and systems associated with optical coherence tomography and angiography.

ACKNOWLEDGMENT OF GOVERNMENT SUPPORT

 This invention was made with government support under grant numbers
20 R01-EY013516 awarded by the National Institutes of Health. The government has certain rights in the technology.

BACKGROUND

 Diabetic retinopathy, age-related macular degeneration and glaucoma are
25 the typical ocular diseases in which vascular disorders and impaired circulation have been observed. For example, an increasing body of evidence suggests that dysfunction of ocular microcirculation in the optic nerve influences the progression of glaucoma. Quantification of ocular circulation is therefore important for the diagnosis of ophthalmic diseases.

30 Currently, a number of methods have been used for measuring ocular perfusion. Fluorescein angiography (FA) provides useful qualitative information in health and disease; however, it only shows the superficial retinal vessels and does not assess deep perfusion, such as the microcirculation in optic nerve head (ONH), choroidal blood flow. Additionally, injection of dye can cause nausea and

anaphylaxis, making it unsuitable as a tool for routine glaucoma assessment. Both laser Doppler flowmetry [e.g. Heidelberg Retinal Flowmeter (HRF)], which samples capillary flow over a small retinal area, and laser speckle flowgraphy, which provides a spot sample of blood velocity, can show differences between diseases and normal groups. However the measurements provided by these methods are too variable for diagnostic application due to dependence on the signal strength and the location of the small sampled area. Magnetic resonance imaging (MRI) has been proposed to quantitatively image ONH perfusion; however, the major limiting factor with this method is the small size of the ONH and limited resolution to detect focal or mild circulatory insufficiency.

Optical coherence tomography (OCT) is an imaging technique that has been widely used for diagnosis and management of ocular diseases. As a coherence detection technique, OCT can detect the Doppler frequency shift of the backscattered light that provides information on blood flow. Doppler OCT has been used for measuring total human retinal blood flow (TRBF) in patients with glaucoma, optic neuropathy, and diabetic retinopathy. With this method, global blood flow from central retinal vessels can be quantified, but local microcirculation cannot be resolved because the velocity range is too low for accurate Doppler measurement. To measure local microcirculation, we recently developed the split-spectrum amplitude-decorrelation angiography (SSADA) algorithm that provides high quality three-dimensional (3D) angiography using ultrahigh speed OCT. Because SSADA is based on the variation of reflectance in resolution cells of isotropic dimensions, it is equally sensitive to transverse and axial movements. Thus it may be able to provide more impartial estimates of local microvascular perfusion that are independent of beam incidence angle. In contrast, both Doppler and phase-variance OCT angiography are more sensitive to axial flow than to transverse flow. Therefore SSADA may be a good basis for quantitative angiography of the microcirculation within different vascular beds.

In vivo three-dimensional mapping of biologic tissue and vasculature is difficult due to the highly-scattering and absorptive nature of biologic tissue. Some current methods have slow scanning speeds making in vivo three-dimensional imaging difficult. Some other techniques having faster scanning speeds are still lacking due to their inability to scan deeply into biologic tissue without producing overlapped images, requiring the use of invasive procedures to scan the tissue of

interest. Many techniques aimed at deeper imaging generally cannot provide deep imaging of tissue having moving material (e.g., blood flow). Therefore, methods to effectively image structure and/or tissue movement, such as blood flow, are of substantial clinical importance.

5 Optical coherence tomography (OCT) is an imaging modality for high-resolution, depth-resolved cross-sectional, and 3-dimensional (3D) imaging of biological tissue. Among its many applications, ocular imaging in particular has found widespread clinical use. In the last decade, due to the development of light source and detection techniques, Fourier-domain OCT, including spectral
10 (spectrometer-based) OCT and swept-source OCT, have demonstrated superior performance in terms of sensitivity and imaging speed over those of time-domain OCT systems. The high-speed of Fourier-domain OCT has made it easier to image not only structure, but also blood flow. This functional extension was first demonstrated by Doppler OCT which images blood flow by evaluating phase
15 differences between adjacent A-line scans. Although Doppler OCT is able to image and measure blood flow in larger blood vessels, it has difficulty distinguishing the slow flow in small blood vessels from biological motion in extravascular tissue. In the imaging of retinal blood vessels, Doppler OCT faces the additional constraint that most vessels are nearly perpendicular to the OCT beam, and therefore the
20 detectability of the Doppler shift signal depends critically on the beam incident angle. Thus, other techniques that do not depend on beam incidence angle are particularly attractive for retinal and choroidal angiography.

 Several OCT-based techniques have been successfully developed to image microvascular networks in human eyes *in vivo*. One example is optical
25 microangiography (OMAG), which can resolve the fine vasculature in both retinal and choroid layers. OMAG works by using a modified Hilbert transform to separate the scattering signals from static and moving scatters. By applying the OMAG algorithm along the slow scanning axis, high sensitivity imaging of capillary flow can be achieved. However, the high-sensitivity of OMAG requires precise removal of
30 bulk-motion by resolving the Doppler phase shift. Thus, it is susceptible to artifacts from system or biological phase instability. Other related methods such as phase variance and Doppler variance have been developed to detect small phase variations from microvascular flow. These methods do not require non-perpendicular beam incidence and can detect both transverse and axial flow. They

have also been successful in visualizing retinal and choroidal microvascular networks. However, these phase-based methods also require very precise removal of background Doppler phase shifts due to the axial movement of bulk tissue. Artifacts can also be introduced by phase noise in the OCT system and transverse
5 tissue motion, and these also need to be removed.

To date, most of the aforementioned approaches have been based on spectral OCT, which provides high phase stability to evaluate phase shifts or differentiates the phase contrast resulting from blood flow. Compared with spectral OCT, swept-source OCT introduces another source of phase variation from the
10 cycle-to-cycle tuning and timing variabilities. This makes phase-based angiography noisier. To use phase-based angiography methods on swept-source OCT, more complex approaches to reduce system phase noise are required. On the other hand, swept-source OCT offers several advantages over spectral OCT, such as longer imaging range, less depth-dependent signal roll-off, and less motion-induced
15 signal loss due to fringe washout. Thus an angiography method that does not depend on phase stability may be the best choice to fully exploit the advantages of swept-source OCT. In this context, amplitude-based OCT signal analysis may be advantageous for ophthalmic microvascular imaging.

One difficulty associated with OCT's application in microvascular imaging
20 comes from the prevalent existence of speckle in OCT images obtained from *in vivo* or *in situ* biological samples. Speckle is the result of the coherent summation of light waves with random path lengths and it is often considered as a noise source which degrades the quality of OCT images. Various methods have been developed to reduce speckle in spatial domain, such as angle compounding,
25 spectral compounding, and strain compounding. Speckle adds to "salt-and-pepper-like" noise to OCT images and induces random modulation to interferometric spectra which can significantly reduce contrast.

In spite of being a noise source, speckle also carries information. Speckle patterns form due to the coherent superposition of random phasors. As a result of
30 speckle, the OCT signal becomes random in an area that is macroscopically uniform. If a sample under imaging is static, the speckle pattern is temporally stationary. However, when photons are backscattered by moving particles, such as red blood cells in flowing blood, the formed speckle pattern will change rapidly over time. Speckle decorrelation has long been used in ultrasound imaging and in laser

speckle technique to detect optical scattering from moving particles such as red blood cells. This phenomenon is also clearly exhibited by real-time OCT reflectance images. The scattering pattern of blood flow varies rapidly over time. This is caused by the fact that the flow stream drives randomly distributed blood cells through the imaging volume (voxel), resulting in decorrelation of the received backscattered signals that are a function of scatterer displacement over time. The contrast between the decorrelation of blood flow and static tissue may be used to extract flow signals for angiography.

The speckle phenomenon has been used in speckle variance OCT for the visualization of microvasculature. Speckle patterns at areas with flowing blood have a large temporal variation, which can be quantified by inter-frame speckle variance. This technique termed "speckle variance" has been used with swept-source OCT demonstrating a significant improvement in capillary detection in tumors by calculation of the variance of the OCT signal intensity. A key advantage of the speckle variance method is that it does not suffer from phase noise artifacts and does not require complex phase correction methods. Correlation mapping is another amplitude-based method that has also recently demonstrated swept-source OCT mapping of animal cerebral and human cutaneous microcirculation *in vivo*. These amplitude-based angiography methods are well suited to swept-source OCT and offer valuable alternatives to the phase-based methods. However, such methods still suffer from bulk-motion noise in the axial dimension where OCT resolution is very high. Therefore, an amplitude-based swept-source angiography method that is able to reduce bulk-motion noise without significant sacrifice in the flow signal would be optimal. For example, imaging of retinal and choroidal flow could be particularly improved with such noise reduction, as in the ocular fundus the flow signal is predominantly in the transverse rather than axial dimension.

While improving qualitative blood flow measurement through noise reduction methods has immense value, determining quantitative blood flow measurement in regions of interest is highly desirable clinically. To date, while several methods exist to measure global retinal blood flow, they have significant limitations and are not used clinically. For example, ultrasound color Doppler imaging does not have sufficient spatial resolution to measure retinal vessels. It measures velocity and resistive indices in large retrobulbar vessels. Although studies have shown differences between normal and glaucoma groups using ultrasound color Doppler

imaging, variability in measurements has limited its potential for clinical diagnosis. Bidirectional laser Doppler velocimetry can measure velocity and flow in individual retinal vessels, but measurement of total retinal blood flow is too time consuming to be practical. Dicon's pulsatile ocular blood flow analyzer can analyze intraocular
5 pressure, but has been shown to be a poor correlate of ocular circulation. Finally, dual-angle Doppler OCT has the limitation of requiring special hardware that is not compatible with existing commercial OCT designs.

As noted above, Doppler OCT, on its own, has difficulty distinguishing the slow flow in small blood vessels from biological motion in extravascular tissue, as
10 well as has difficulty detecting and defining vessel anatomy due to most vessels being nearly perpendicular to the OCT beam. However, Doppler shift can provide valuable quantitative velocity information. Thus, an optimal bulk-noise reduction amplitude-based swept-source angiography method used in combination with Doppler OCT (e.g., via dual scanning, done simultaneously or near simultaneously)
15 could allow for measurement of total retinal blood flow (TRBF), including both vein and artery measurement around the optic disc.

SUMMARY

As described below, a new quantitative system has been established for making quantitative ocular blood flow measurements. Specifically, the methods
20 described herein are able to measure circulation in ONH (e.g. whole disc/temporal ellipse, peripapillary retina, peripapillary choroid) and macula (e.g. macular retina, macular choroid, fovea avascular zone and the area of non-perfusion). Quantification of different circulation obtained from patients having an ocular disease compared with the result from normal subjects are herein described.

25 One embodiment is directed to methods for quantitatively measuring blood flow in an ocular vascular bed. In certain embodiments, the method for quantitatively measuring blood flow in an ocular vascular bed may comprise the steps of selecting an ocular vascular bed from which to quantitatively measure blood flow, scanning the ocular vascular bed to obtain M-B scans of OCT spectrum
30 therefrom, splitting the M-B scans of OCT spectrum into M spectral bands and determining a quantitative measurement of blood flow from the M spectral bands. In additional embodiments, the step of splitting the M-B scans of the OCT spectrum into M spectral bands may comprise creating overlapping filters covering the OCT spectrum, and filtering the OCT spectrum with the overlapping filters. In yet further

embodiments, the step of determining a quantitative measurement of blood flow from the M spectral bands may comprise creating decorrelation images for the M spectral bands and combining the decorrelation images for the M spectral bands to create a flow image and/or the step of creating decorrelation images for the M spectral bands may comprise determining amplitude information for each spectral band and calculating decorrelation between adjacent amplitude frames for each spectral band.

Yet other embodiments are directed to methods for quantitatively measuring blood flow in an ocular vascular bed as described above that further comprise the step of removing background noise. The methods described herein may optionally also comprise combining the decorrelation images for the M spectral bands to create a flow image that comprises averaging the decorrelation images for each spectral band to create an average decorrelation image for each spectral band and averaging the averaged decorrelation images from the M spectral bands. The ocular vascular bed from which quantitative blood flow measurements are obtained may include the ocular nerve head, the macula, the ocular disc, the temporal ellipse, the peripapillary retina, the peripapillary choroid, the macular retina, the macular choroid, the fovea avascular zone, or the area of non-perfusion.

Other embodiments are directed to use of the herein described methods for quantitatively measuring blood flow in an ocular vascular bed for the purpose of diagnosing an ocular disease. In this regard, it is noted that ocular diseases such as glaucoma, diabetic retinopathy and age-related macular degeneration are associated with impaired intraocular blood flow and circulation.

Yet further embodiments are directed to specific systems useful for quantitatively measuring blood flow in an intraocular vascular bed. In certain embodiments, such systems may comprise an optical coherence tomography apparatus and one or more processors coupled to the OCT apparatus and adapted to cause that apparatus to obtain M-B scans of OCT spectrum from the ocular vascular bed, split the M-B scans of OCT spectrum into M spectral bands, and determine a quantitative measurement of blood flow from the M spectral bands.

Additional embodiments will be readily apparent to one skilled in the art upon reading the present specification.

BRIEF DESCRIPTION OF THE DRAWINGS

Embodiments described herein will be readily understood by the following detailed description in conjunction with the accompanying drawings. Embodiments are illustrated by way of example and not by way of limitation in the figures of the accompanying drawings.

Figure 1 is a chart comparing prior art techniques with those described herein with regard to vascular connectivity and decorrelation signal/noise (DSNR).

Figure 2 schematically illustrates modification of an OCT imaging resolution cell to create an isotropic resolution cell utilizing a band-pass filter.

Figure 3 schematically illustrates M-B-scan mode for acquiring OCT spectrum.

Figure 4 is a flowchart showing an exemplary method for creating a decorrelation (flow) image that uses split-spectrum techniques and the full information in the entire OCT spectral range.

Figure 5 is a flowchart showing additional exemplary methods of the exemplary method of Figure 4.

Figure 6 schematically illustrates a 2D spectral interferogram split into different frequency bands.

Figure 7 schematically illustrates the methods of Figure 4 and Figure 5 for creating a decorrelation (flow) image that uses split-spectrum techniques and the full information in the entire OCT spectral range.

Figure 8 is a flowchart showing an exemplary method for eliminating decorrelation images with excessive motion noise.

Figure 9 schematically illustrates an *in vivo* imaging system for collecting image information.

Figure 10 illustrates an embodiment of an *in vivo* imaging system in accordance with various embodiments described herein.

Figure 11 illustrates an embodiment of an article of manufacture for *in vivo* imaging in accordance with various embodiments described herein.

Figure 12 illustrates *in vivo* 3-D volumetric structure images of the optic nerve head using imaging methods in accordance with various embodiments described herein.

Figure 13 illustrates *in vivo* 3-D volumetric structure images of the macula using methods in accordance with various embodiments described herein.

Figure 14 illustrates *in vivo* images of macular retinal circulation using methods in accordance with prior art methods and in accordance with various
5 embodiments described herein.

Figure 15 illustrates *in vivo* images depicting vascular connectivity and signal to noise ratio (SNR) using methods in accordance with prior art methods and in accordance with various embodiments described herein.

Figure 16 illustrates *in vivo* images using methods in accordance with
10 various embodiments described herein, including multiple rings circular scan pattern and Doppler angle estimation for a single vessel.

Figures 17A-D illustrates *in vivo* images using methods in accordance with various embodiments described herein, including multiple rings circular scan Doppler OCT in combination with SSADA to provide total retinal blood flow (TRBF)
15 measurement.

Figure 18 schematically illustrates an OCT angiography scan pattern for blood flow quantification.

Figure 19 schematically shows the creation of an isotropic resolution cell.

Figure 20 is a flowchart showing an exemplary method for conducting
20 quantitative blood flow measurements.

Figure 21 illustrates the specific segmentation of various ocular vascular beds.

Figure 22 illustrates an exemplary alternative segmentation method for the ocular nerve head (ONH).

25 Figure 23 illustrates an exemplary method for detecting disc margin.

Figure 24 illustrates an exemplary method for quantifying ONH blood flow.

Figure 25 illustrates detection of the fovea avascular zone and other areas of non-perfusion.

Figure 26 illustrates OCT angiography showing reduced ONH blood flow in
30 glaucoma.

DETAILED DESCRIPTION

In the following detailed description, reference is made to the accompanying drawings which form a part hereof. It is to be understood that other embodiments may be utilized and structural or logical changes may be made.

5 Various operations may be described as multiple discrete operations in turn, in a manner that may be helpful in understanding embodiments described herein; however, the order of description should not be construed to imply that these operations are order dependent.

10 The description may use perspective-based descriptions such as up/down, back/front, and top/bottom. Such descriptions are merely used to facilitate the discussion and are not intended to restrict the application of embodiments described herein.

The description may use the phrases "in an embodiment," or "in embodiments," which may each refer to one or more of the same or different 15 embodiments. Furthermore, the terms "comprising," "including," "having," and the like, as used with respect to embodiments described herein, are synonymous.

A phrase in the form of "A/B" means "A or B." A phrase in the form "A and/or B" means "(A), (B), or (A and B)." A phrase in the form "at least one of A, B and C" means "(A), (B), (C), (A and B), (A and C), (B and C) or (A, B and C)." A phrase in 20 the form "(A) B" means "(B) or (A B)," that is, A is optional.

In various embodiments described herein, methods, apparatuses, and systems for biomedical imaging are provided. In exemplary embodiments described herein, a computing system may be endowed with one or more components of the disclosed articles of manufacture and/or systems and may be 25 employed to perform one or more methods as disclosed herein.

In various embodiments, structure and/or flow information of a sample may be obtained using optical coherence tomography (OCT) (structure) and OCT angiography (structure and flow) imaging based on the detection of spectral interference. Such imaging may be two-dimensional (2-D) or three-dimensional (3-D), depending on the application. Structural imaging may be of an extended depth 30 range relative to prior art methods, and flow imaging may be performed in real time. One or both of structural imaging and flow imaging as disclosed herein may be enlisted for producing 2-D or 3-D images.

Unless otherwise noted or explained, all technical and scientific terms used herein are used according to conventional usage and have the same meaning as commonly understood by one of ordinary skill in the art which the disclosure belongs. Although methods, systems, and apparatuses/materials similar or
5 equivalent to those described herein can be used in the practice or testing of the present disclosure, suitable methods, systems, and apparatuses/materials are described below.

All publications, patent applications, patents, and other references mentioned herein are incorporated by reference in their entirety. In case of
10 conflict, the present specification, including explanation of terms, will control. In addition, the methods, systems, apparatuses, materials, and examples are illustrative only and not intended to be limiting.

In order to facilitate review of the various embodiments of the disclosure, the following explanation of specific terms is provided:

15 **A-scan:** A reflectivity profile that contains information about spatial dimensions and location of structures with an item of interest (e.g., an axial depth scan).

Autocorrelation: A cross-correlation of a signal with itself; the similarity between observations as a function of the time separation between them. For
20 example, autocorrelation can be used to find repeating patterns, such as the presence of a periodic signal which has been buried under noise, or used to identify the missing fundamental frequency in a signal implied by its harmonic frequencies.

B-scan: A cross-sectional tomograph that may be achieved by laterally combining a series of axial depth scans (e.g., A-scans).

25 **Cross-correlation:** A measure of similarity of two waveforms as a function of a time-lag applied to one of the waveforms.

Decorrelation: A process that is used to reduce autocorrelation within a signal, or cross-correlation within a set of signals, while preserving other aspects of the signal. For example, decorrelation can be used to enhance differences found in
30 each pixel of an image. A measure of a lack of correlation or similarity between corresponding pixels in two images can also describe decorrelation. The end result of a decorrelation process is that faint information within a signal may be enhanced to bring out (e.g., present) subtle differences that may be meaningful. For example, one can calculate decorrelation to find a difference between images.

Illustrated in Figure 1 is a comparison chart 100 of prior art amplitude-based OCT signal analysis methods and the embodiments described herein based on vascular connectivity and decorrelation signal/noise (DSNR). Full-spectrum decorrelation method 100, for example, can be utilized as the baseline value for comparison purposes, however, as described previously, it is sensitive to axial bulk motion causing significant noise in the resulting images produced. In pixel averaging method 112 the signal in several adjacent pixels is combined resulting in an improvement of decorrelation signal-to-noise ratio (DSNR). The improved DSNR of pixel averaging method 112 in turn leads to higher quality images of microcirculation (compared to full-spectrum decorrelation method 100), which can be assessed by measuring the vasculature of the microvascular network revealed in the OCT angiograms. As described herein, split-spectrum decorrelation 122 further improves DSNR (compared to the improvement offered by pixel averaging method 112) by reducing the noise due to axial bulk motion. This can be accomplished by the methods described herein below (e.g., reducing the axial dimension of the effective resolution cell).

The improved DSNR of split-spectrum decorrelation method 122 in turn leads to even higher quality images of microcirculation (compared to full-spectrum decorrelation method 100 and pixel averaging method 112), which can be assessed by measuring the vasculature of the microvascular network revealed in the OCT angiograms. Such an improvement, can allow for images and information useful in for diagnostic and management of diseases in the eye, as well as investigations and analysis of circulation, angiogenesis and the other blood flow imaging analysis. Additionally, the split-spectrum decorrelation 122 could be used to obtain angiography images that could be used to replace fluorescein and indocyanine green angiographies, with the additional advantage of being intrinsically 3-dimensional rather than 2-dimensional. Additional uses can include, but not be limited to, imaging of blood flow in other biological tissue and the imaging of flow in any system, living or nonliving.

In more detail, prior art full-spectrum decorrelation 102 achieves decorrelation purely through process the amplitude signal and does not require phase information. To evaluate the flow signals coming from the scattering tissue, an average decorrelation image $\overline{D}(x, z)$ at each position is obtained by averaging

N-1 decorrelation image frames computed from N reflectance amplitude images frames from M-B mode scanning. Each decorrelation frame is computed from 2 adjacent amplitude frames: $A_n(x, z)$ and $A_{n+1}(x, z)$. Using the full spectrum decorrelation method 102, the decorrelation image it is given by the following equation:

$$(1)$$

$$\overline{D}(x, z) = 1 - \frac{1}{N-1} \sum_{n=1}^{N-1} \frac{A_n(x, z)A_{n+1}(x, z)}{\left[\frac{1}{2}A_n(x, z)^2 + \frac{1}{2}A_{n+1}(x, z)^2\right]} \quad (N = 8)$$

where x and z are lateral and depth indices of the B-scan images and n denotes the B-scan slice index. In this full spectrum equation, the decorrelation signal-to-noise ratio acquired from full spectrum can only be increased by increasing the number N of B-scans taken at the same position. However, more scans require more imaging time which may not be practical.

In more detail, prior art pixel averaging method 112 can produce decorrelation images given by the following equation:

$$(2)$$

$$\overline{D}(x, z) = 1 - \frac{1}{N-1} \frac{1}{PQ} \sum_{n=1}^{N-1} \sum_{p=1}^P \sum_{q=1}^Q \frac{A_n(x+p, z+q)A_{n+1}(x+p, z+q)}{\left[\frac{1}{2}A_n(x+p, z+q)^2 + \frac{1}{2}A_{n+1}(x+p, z+q)^2\right]}$$

($P=1, Q=4, N=8$)

where P and Q are the averaging window widths in the X and Z directions, as described in .J. Enfield, E. Jonathan, and M. Leahy, "In vivo imaging of the microcirculation of the volar forearm using correlation mapping optical coherence tomography (cmoct)," Biomed. Opt. Express 2(5), 1184-1193 (2011). To suppress the spurious noise and discontinuities in the vasculature, P by Q window moving average can be implemented over the X - Z 2D map. To fairly compare the prior art pixel averaging method 112 with the split-spectrum decorrelation 122 described herein, a 1 by 4 window can be created, which means pixel-averaging is only

applied along the Z direction, the same direction used for splitting the spectrum in split-spectrum decorrelation 122

In more detail, split-spectrum decorrelation 122 can produce decorrelation images given by the following equation:

5 (3)

$$\bar{D}(x, z) = 1 - \frac{1}{N-1} \frac{1}{M} \sum_{n=1}^{N-1} \sum_{m=1}^M \frac{A_n(x, z) A_{n+1}(x, z)}{\left[\frac{1}{2} A_n(x, z)^2 + \frac{1}{2} A_{n+1}(x, z)^2 \right]}$$

(M = 4, N = 8)

After splitting the spectrum by applying M (for example, M can = 4 as described in an exemplary example below) equally spaced bandpass filters, M individual decorrelation images can be obtained between each pair of B-scans, which can then be averaged along both the lateral (X) and axial (Z) directions to increase DSNR. In split-spectrum decorrelation 122, the average decorrelation image $\bar{D}(x, z)$ can be described as the average of decorrelation images from M spectral bands. By increasing the number M (up to a point), the decorrelation signal-to-noise ratio can be improved without increasing the scan acquisition time.

15 Whichever decorrelation method is used (full-spectrum 102, pixel- averaging 112, and split-spectrum 122) the resulting average decorrelation image frame $\bar{D}(x, z)$ should be a value between zero and one, indicating weak and strong decorrelation, respectively. By describing the decorrelation methods in such detail above, it is possible to compare the methods to one another based on the resulting decorrelation images obtained as illustrated in chart 100 of Figure 1. The split-spectrum method 122 suppresses noise from axial bulk motion and, in addition, makes use of information in the full k spectrum resulting in superior decorrelation signal-to-noise ratio for flow detection. Utilizing the split-spectrum method 122, axial bulk motion can be suppressed by the use of spectral (k) bandpass filters that increase the axial dimension of the resolution cell so that it can be equal (or substantially equal) to the transverse dimension of the resolution cell.

Illustrated in Figure 2 is diagram 200 visually depicting modification of an OCT imaging resolution cell 202 via two distinct and separate techniques (band-pass filtering 204 and split-spectrum 206) to create an isotropic resolution cell 208. Each pixel in a B-scan OCT image is formed from backscattered signals of a 3D volume in space, referred to as a resolution cell (e.g., imaging resolution cell 202 in Figure 2). The statistical changes in the envelope intensity are related to the motion of scatterers through the OCT resolution cell. For a typical swept-source OCT setup, the axial (Z direction) resolution, determined by the source central wavelength and its spectral bandwidth, is much higher than the lateral resolution determined by the laser beam profile in both X and Y directions. For example, in common swept source OCT systems, using the full-width-half-maximum (FWHM) amplitude profile definition, the axial resolution ($\sim 5\ \mu\text{m}$) is four times higher than the lateral resolution ($\sim 18\ \mu\text{m}$) if both are defined as full-width-half-maximum amplitude profiles (e.g., imaging resolution cell 202 depicts $x=y=4z$). This anisotropic resolution cell, with higher axial than transverse resolution, will result in higher decorrelation sensitivity for axial motion. In the fundus, ocular pulsation related to heart beat, driven by the retrobulbar orbital tissue, mainly occurs along the axial direction. The anisotropic resolution cell of retinal OCT imaging is very sensitive to this axial motion noise. On the other hand, retinal and choroidal blood flow vectors are primarily transverse to the OCT beam, along the wider (less sensitive) dimensions of the OCT resolution cell. Therefore, to improve the signal-to-noise ratio (SNR) of flow detection, it is desirable to lower the axial resolution and dampen the axial decorrelation sensitivity. This reduces the axial motion noise without sacrificing the transverse flow signal.

One straightforward way to achieve this resolution modification is band-pass filtering of the spectral interferogram (e.g., band-pass filtering 204). Unfortunately, this also sacrifices most of the speckle information in the spectral interferogram and decreases the flow signal. Thus, this is not an effective way to increase the SNR of flow (decorrelation) detection. A better way to decrease axial resolution without losing any speckle information is to split the spectrum into different frequency bands (e.g., split-spectrum 206) and calculate decorrelation in each band separately. The decorrelation (flow) images from the multiple spectral bands can then be averaged together to make full use of the speckle information in the entire

OCT spectrum. The details of the split-spectrum procedure are explained herein and below (e.g., split-spectrum decorrelation 122 of Figure 1 can be utilized).

Illustrated in Figure 3 is a visual 300 of one 3D volumetric data 302 comprising data obtained via an exemplary embodiment M-B-scan mode from an OCT system. N consecutive B-scans at a single Y position comprise M-B-scan 306 (e.g., in some exemplary embodiments described herein, N= eight (8), but is not limited to any specific N). Therefore, for each 3D volumetric data 302, in the fast scan (x) axis, a single B-scan comprises a plurality of A-scans 304, and in the slow scan (y) axis, there are a number of M-B-scans 306 comprising N consecutive B-scans.

Figure 4 shows an exemplary method 400 for creating a decorrelation (flow) image that uses split-spectrum techniques and the full information in the entire OCT spectral range. The method 400 can be performed, for example, by *in vivo* imaging systems described herein below. Portions of method 400 and any of the other methods (or portion of methods) described herein can be performed by computer-executable instructions stored on computer-readable media and articles of manufacture for *in vivo* imaging.

At 402, M-B scans of OCT spectrum are received. For example, M-B scans as depicted in visual 300 of Figure 3 can be received from an OCT *in vivo* imaging system.

At 404, M spectral bands can be created from the M-B scans of OCT spectrum 402. For example, split spectrum 206 of Figure 2 can be utilized to create the M spectral bands.

At 406, averaged decorrelation images for each spectral band of the M spectral bands can be created. For example, split spectrum decorrelation 122 described in Figure 1 can be utilized to create decorrelation images for the M spectral bands and then for each spectral band those decorrelation images can be averaged.

At 408, the averaged decorrelation images for each spectral band created at 406 can be averaged to create a single final image (e.g., final decorrelation image) 410.

Figure 5 shows additional exemplary methods 500, including reference to similar methods within method 400 of Figure 4, for creating a decorrelation (flow) image that uses split-spectrum techniques and the full information in the entire OCT

spectral range. The method 500 can be performed, for example, by *in vivo* imaging systems described herein below. Portions of method 500 and any of the other methods (or portion of methods) described herein can be performed by computer-executable instructions stored on computer-readable media and articles of manufacture for *in vivo* imaging.

Figure 6 schematically illustrates via visual 600 a 2D spectral interferogram split into different frequency bands as described in methods 400 of Figure 4 and 500 of Figure 5.

Figure 7 schematically illustrates via visual 700 the methods 400 of Figure 4 and 500 of Figure 5 for creating a decorrelation (flow) image that uses split-spectrum techniques and the full information in the entire OCT spectral range.

Figure 8 is a flowchart 800 showing an exemplary method for eliminating decorrelation images with excessive motion noise (e.g., as described in method 500 of Figure 5).

Continuing with the method 500 of Figure 5, at 502, M-B scans of OCT spectrum are received. For example, M-B scans of OCT spectrum 402 can be received from an OCT *in vivo* imaging system, as depicted in Figure 7. In more detail, for example, spectral interference signal recorded by a high speed digitizer in swept-source OCT, after subtracting background and autocorrelation terms, can be received and simply given by the following equation

(4)

$$I(x, k) = \int_{-\infty}^{\infty} R(k)A(x, k, z)\cos(2kz)dz$$

where x is the transverse position of focus beam spot on the sample along the fast scan axis, k is the wavenumber, $I(x, k)$ is the light intensity, $R(k)$ is the amplitude of light reflected from the reference arm, $A(x, k, z)$ is the amplitude of the light backscattered from the sample, and z is the optical delay mismatch between the sample reflections and the reference reflection in the free space equivalent.

At 504, overlapping filters (M) covering the entire spectrum can be created. Additionally, at 506, band pass filtering along k can be conducted. Collectively, creating overlapping filters 504 and band pass filtering 506 can result in creating M spectral bands 507 as depicted in Figure 7 (e.g., as described in creating M

spectral bands 404 in method 400 of Figure 4). Following along with the example provided above of the spectral interference signal represented by equation (4), the Gaussian shape above the 2D interferogram $I(x, k)$ (e.g., 2D interferogram 605 of Figure 6) can be used to express the received interferometric fringe at one position.

5 The bandwidth of this full-spectrum fringe can first be defined, and then a filter bank created to divide this full-spectrum fringe into different bands (e.g., creating overlapping filters (M) 504 of method 500). The specifications of this filter bank can depend on several factors, including, but not limited to, 1) filter type, 2) bandwidth of each filter, 3) overlap between different bands, and 4) number of bands. In one
10 exemplary embodiment, a Gaussian filter can be introduced whose function was defined by the following equation:

(5)

$$G(n) = \exp\left[-\frac{(n-m)^2}{2\sigma^2}\right]$$

15

where n is the spectral element number that varies from 1 to 1400 and is linearly mapped to wavenumber k . The range of sampled k can be 10000 to 9091 cm^{-1} , corresponding to a wavelength range of 1000 to 1100 nm. The bandwidth, referred to as “BW,” (e.g., as depicted in 604 of Figure 6) of the full spectrum can be 69 nm,
20 which can provide a FWHM axial spatial resolution of 5.3 μm . m is the position of the spectral peak. In an exemplary embodiment, the peaks of the spectral Gaussian filters can be placed at 9784, 9625, 9466, and 9307 cm^{-1} . σ^2 is the variance of the Gaussian filter in terms of the number of spectral elements. In an exemplary embodiment, the FWHM amplitude bandwidth, referred to as “bw,” of the
25 bandpass filters can equal to $2\sqrt{2\ln 2}\sigma$, covering 378 spectral elements, corresponding to a wavelength range of 27nm or a wavenumber range of 245 cm^{-1} . The four (4) bandpass filters (e.g., as depicted in 608, 610, 612, and 614 of Figure 6), described in such an exemplary embodiment, can overlap so that none of the frequency components of the original signal are lost in the processing. Figure 6
30 visually displays a 2D spectral interferogram 605 split at 606 (e.g., via 404 of method 400 of Figure 4) into four new spectra with smaller k bandwidth, with “BW” 604 indicating the bandwidth of a full-spectrum filter and multiple “bw”s 608, 610, 612, and 614 being the bandwidth of multiple Gaussian filters, respectively, and

regions of non-zero values in the data block are indicated by the dark shaded patterns 616, 618, 620, and 622 (similarly visually depicted, for example in Figure 7).

At 508, the M spectral bands 507 from each individual frequency band can be passed into conventional Fourier-domain OCT algorithms to Fourier transform along k . Additionally, phase information can be dropped to result in amplitude information for each spectral band 509 (e.g., as depicted in Figure 7).

For example, the OCT signals therefore can be directly calculated from the decomposed interferograms $I'(x, k)$ by applying Fourier transform upon wavenumber k . The computed OCT signal can be a complex function, $\tilde{I}(x, z)$, which can be written as the following equation:

(6)

$$\tilde{I}(x, z) = FFT\{I'(x, k)\} = A(x, z)exp[i\varphi(x, z)]$$

where $\varphi(x, z)$ is the phase of the analytic signal $\tilde{I}(x, z)$. The amplitudes of the OCT signals, $A(x, z)$, can be used while the phase information can be selectively disregarded.

At 510, a fixed value can be set for removal of high decorrelation generated by background noise. Decorrelation of OCT signal amplitude between B-scans taken at the same nominal position can be caused by several sources: (1) flow, (2) bulk tissue motion or scanner position error, and (3) background noise. To help accentuate true flow measurement in the images created and improve the signal-to-noise ratio for flow detection, removal of high decorrelation generated by background noise is desirable. Background noise is random and therefore has high decorrelation between B-scan frames. Noise predominates in pixels with low OCT signal amplitude and therefore flow cannot be assessed in these pixels with any accuracy. A fixed decorrelation value of zero (0) can be assigned to these pixels with low OCT signal amplitude. For example, this can be achieved by setting the low signal pixels a constant amplitude value. The threshold value, for example, can then be chosen to be two standard deviations above the mean background value measured when the sample beam was blocked.

At 512, decorrelation calculation can be obtained between adjacent amplitude frames. For example, split-spectrum decorrelation 122 as described in Figure 1 can be utilized to produce decorrelation images for each spectral band 513 (e.g., as depicted in Figure 7 visually).

5 At 514, decorrelation images for each spectral band 513 having excessive motion noise can be eliminated. To help accentuate true flow measurement in the images created and improve the signal-to-noise ratio for flow detection, removal of decorrelation generated by bulk tissue motion or scanner position is desirable. Saccadic and micro-saccadic eye movements are rapid and cause a high degree of
10 decorrelation between B-scans, as depicted, for example, in flowchart 800 of Figure 8. Such movements can be seen in visual 802 which displays three frames of a set of seven (7) decorrelation images 804 (D_n) of the region around the optic nerve head (ONH), computed from eight (8) OCT B-scans at the same Y location. Each decorrelation image frame depicted can be calculated from a pair of adjacent B-
15 scan amplitude frames, for example as described using the methods described above. In six (6) of the seven (7) decorrelation frames, flow pixels could be distinguished from non-flow pixels by their higher decorrelation values. However, in frame D4 806, both flow (vessel) and non-flow (bulk tissue) pixels had high decorrelation values possibly due to rapid eye movement (e.g., saccadic). To
20 detect bulk motion, the median decorrelation value in the highly reflective portion of the imaged tissue structures (between the region noted as 808) can be determined. High bulk motion in frame D4 806 can be detected by high median decorrelation value in pixel histogram analysis 810. Histogram analysis can be performed within
25 a high reflectivity band starting at the retinal inner limiting membrane and spanning 30 pixels below (within region 808 of 802. By comparing the median decorrelation value 814 to a preset threshold 812 (e.g., in one exemplary embodiment the threshold was set at 0.15, two standard deviations above the median decorrelation value), it can be determined that a frame (e.g. frame D4) is a statistical outlier and should be eliminated. Visual 816 depicts the result after the removal of the outlier
30 frame D4.

At 516, the decorrelation images at each spectral band that remain after images with excessive motion noise have been removed can be averaged to create an average decorrelation image for each spectral band, therefore resulting in

multiple averaged decorrelation images (i.e., one average decorrelation for each spectral band as visualized in Figure 7).

At 518, the averaged decorrelation images from M spectral bands are averaged to create one final decorrelation image 410 (e.g., as visualized in Figure 7 and also described in method 400, step 408 of Figure 4).

Returning back to flowchart 800 of Figure 8, after removing frame D4 806 as an outlier, the remaining six (6) decorrelation images can be averaged to produce a cleaned decorrelation image 818 which displays high contrast between flow pixels (e.g., bright area in retinal vessels and choroid) and non-flow dark regions. An uncleaned decorrelation image 820 depicts a final decorrelation image had outlier frame D4 806 remained showing less contrast between flow (vessels) and non-flow (static tissue) pixels compared to the cleaned decorrelation image 818, as evident by the lack of completely dark space between retinal vessels in the peripapillary areas circled at 822 and 824.

Utilizing method 500, a 3D dataset comprising a stack of two hundred (200) corrected average decorrelation cross-sectional images, along with the associated average reflectance images, that together spans 3 mm in the slow transverse scan (Y) direction can be obtained. In some embodiments it may be desirable to separate the 3D data into retinal and choroidal regions with the dividing boundary set at the retina pigment epithelium (RPE). The depth (Z position) of the highly reflective RPE can be identified through the analysis of the reflectance and reflectance gradient profiles in depth. The region above the RPE is the retinal layer and the region below is the choroidal layer. The *en face* X-Y projection angiograms can then be produced by selecting the maximum decorrelation value along the axial (Z) direction in each layer. In ONH scans, the RPE depth just outside the disc boundary can be used to set an interpolated RPE plane inside the disc.

Figure 9 schematically illustrates an *in vivo* imaging system 900 for collecting OCT image information. For example, a high-speed swept-source OCT system 900 (e.g., as described in B. Potsaid, B. Baumann, D. Huang, S. Barry, A. E. Cable, J. S. Schuman, J. S. Duker, and J. G. Fujimoto, "Ultrahigh speed 1050nm swept source / fourier domain oct retinal and anterior segment imaging at 100,000 to 400,000 axial scans per second," Opt. Express 18(19), 20029-20048 (2010)) can be used to demonstrate the methods described above for imaging of microcirculation in the human ocular fundus. High speed swept-source OCT system 900 comprises

a tunable laser 901. For example, tunable laser 901 (e.g., a tunable laser from Axsun Technologies, Inc, Billerica, MA, USA) may have a wavelength of 1050 nm with 100 nm tuning range, a tuning cycle with a repetition rate of 100 kHz and a duty cycle of 50%. Such OCT system 900 can produce a measured axial
5 resolution of 5.3 μm (full-width-half-maximum amplitude profile) and an imaging range of 2.9 mm in tissue. Light from swept source 901 can be coupled into a two by two fiber coupler 902 through single mode optical fiber. One portion of the light (e.g., 70%) can proceed to the sample arm (i.e., the patient interface), and the other portion of the light (e.g., 30%) can proceed to the reference arm.

10 In the sample arm, a sample arm polarization control unit 903 can be used to adjust light polarization state. The exit light from the fiber coupler 902 can then be coupled with a retinal scanner whereby the light is collimated by sample arm collimating lens 904 and reflected by mirror 905 and two dimensional galvo scanner 909 (e.g., an XY galvonanometer scanner). Two lenses, first lense 906 (e.g., an
15 objective lense) and second lense 907 (e.g., an ocular lense) can relay probe beam reflected by galvo scanner 909 into a human eye 908. For example, a focused spot diameter of 18 μm (full-width-half-maximum amplitude profile) can be calculated on the retinal plane based on an eye model. The average light power (i.e., output power of the laser) onto a human eye can be 1.9 mW, which is consistent with safe
20 ocular exposure limit set by the American National Standard Institute (ANSI).

The reference arm can comprise a first reference arm collimating lens 913, a water cell 912, a retro-reflector 911, a glass plate 914 and a second reference arm collimating lens 915. Glass plate 914 can be used to balance the dispersion between the OCT sample arm and reference arm. Water cell 912 can be used to
25 compensate the influence of dispersion in the human eye 908. Retro-reflector 911 can be mounted on a translation stage 910 which can be moved to adjust the path length in the reference arm.

Light from the sample and reference arm can interfere at beam splitter 917. A reference arm polarization control unit 916 can be used to adjust the beam
30 polarization state in the reference arm to maximum interference signal. The optical interference signal from beam splitter 917 (e.g., a 50/50 coupler) can be detected by a balanced detector 918 (e.g., a balanced receiver manufactured by Thorlabs, Inc, Newton, NJ, USA), sampled by an analog digital conversion unit 919 (e.g., a high speed digitizer manufactured by Innovative Integration, Inc.) and transferred

into computer 920 for processing. For example, computer 920 can be used for storing instructions for, and implementing, the methods described herein. Interference fringes, for example, can be recorded by analog digital conversion unit 919 at 400 MHz with 14-bit resolution, with the acquisition driven by the optical clock output of tunable laser 901. In such an exemplary setup, imaging system 900, sensitivity can be measured with a mirror and neutral density filter at 95 dB, with a sensitivity roll-off of 4.2 dB/mm.

While a swept-source OCT system has been described above, the technology disclosed herein can be applied to any Fourier-domain OCT system. In Fourier-domain OCT systems the reference mirror is kept stationary and the interference between the sample and reference reflections are captured as spectral interferograms, which are processed by Fourier-transform to obtain cross-sectional images. In the spectral OCT implementation of Fourier-domain OCT, a broad band light source is used and the spectral interferogram is captured by a grating or prism-based spectrometer. The spectrometer uses a line camera to detect the spectral interferogram in a simultaneous manner. In the swept-source OCT implementation of Fourier-domain OCT, the light source is a laser that is very rapidly and repetitively tuned across a wide spectrum and the spectral interferogram is captured sequentially. Swept-source OCT can achieve higher speed and the beam can be scanned transversely more rapidly (with less spot overlap between axial scans) without suffering as much signal loss due to fringe washout compared to other Fourier-domain OCT systems. However, a very high speed spectral OCT system could also be utilized with the technology disclosed herein.

Any one of the various embodiments as discussed may be incorporated in combination with multiple rings circular scan Doppler OCT to provide total retinal blood flow (TRBF) measurement for both veins and arteries around the optic disc. Utilizing faster OCT systems, higher velocities of flow in arteries (and veins) can be within detectable range and more circles (e.g., rings) can be scanned within a fraction of the cardiac cycle time. By utilizing a scan pattern of multiple rings (e.g., four (4) or more circular scans) the calculation of vessel curvature and slope relative to the OCT beam axis can be obtained. These calculations can allow for more accurate calculation of Doppler angles in the highly curved segments of retinal vessels as they emerge from the optic head nerve (OHN.) The circles can

be closer to the ONH, where the Doppler angles are usually larger, obviating the need for a dual-angle scanning protocol. The OCT beam can then approach at a single angle through the center of an undilated pupil. Each scan can therefore yield a valid TRBD measurement, so fewer scans will be needed. As a vessel can be
5 transected by four (4) or more circular scans, the crossing and branching points can be disregarded (in full or part) in favor of straight sections where flow measurements can be more reliable. With faster scan times per circular scan, motion errors can be reduced as well. In lieu of color disc photography commonly utilized in combination with Doppler OCT, 3D angiography utilizing the techniques
10 discussed (e.g. SSADA) can be used to resolve 3D vessel anatomy.

Any one or more of various embodiments as discussed may be incorporated, in part or in whole, into a system. Figure 10 illustrates an exemplary embodiment of an *in vivo* imaging system (e.g. an OCT system) 1000 in accordance with various embodiments described herein. In the embodiments, OCT
15 system 1000 may comprise an OCT apparatus 1002 and one or more processors 1012 coupled thereto. One or more of the processors 1012 may be adapted to perform methods in accordance with various methods as disclosed herein. In various embodiments, OCT system 1000 may comprise a computing apparatus including, for example, a personal computer in any form, and in various ones of
20 these embodiments, one or more of the processors may be disposed in the computing apparatus. OCT systems in accordance with various embodiments may be adapted to store various information. For instance, an OCT system may be adapted to store parameters and/or instructions for performing one or more methods as disclosed herein.

25 In various embodiments, an OCT system may be adapted to allow an operator to perform various tasks. For example, an OCT system may be adapted to allow an operator to configure and/or launch various ones of the above-described methods. In some embodiments, an OCT system may be adapted to generate, or cause to be generated, reports of various information including, for
30 example, reports of the results of scans run on a sample.

In embodiments of OCT systems comprising a display device, data and/or other information may be displayed for an operator. In embodiments, a display device may be adapted to receive an input (e.g., by a touch screen, actuation of an icon, manipulation of an input device such as a joystick or knob, etc.) and the input

may, in some cases, be communicated (actively and/or passively) to one or more processors. In various embodiments, data and/or information may be displayed, and an operator may input information in response thereto.

Any one or more of various embodiments as discussed may be
5 incorporated, in part or in whole, into an article of manufacture. In various
embodiments and as shown in Figure 11, an article of manufacture 1100 in
accordance with various embodiments described herein may comprise a storage
medium 1112 and a plurality of programming instructions 1102 stored in storage
medium 1112. In various ones of these embodiments, programming instructions
10 1102 may be adapted to program an apparatus to enable the apparatus to perform
one or more of the previously-discussed methods.

In various embodiments, an OCT image may provide data from which a
diagnosis and/or evaluation may be made. In embodiments, such determinations
may relate to biologic tissue structure, vasculature, and/or microcirculation. For
15 example, in some embodiments, 3-D *in vivo* imaging of a biologic tissue and
quantifying flow of blood through individual vessels therein may be useful in
understanding mechanisms behind a number of disease developments and
treatments including, for example, ischemia, degeneration, trauma, seizures, and
various other neurological diseases. In still other embodiments, an OCT image and
20 techniques herein disclosed may be used to identify cancer, tumors, dementia, and
ophthalmologic diseases/conditions (including, e.g., glaucoma, diabetic retinopathy,
age-related macular degeneration). Still further, in various embodiments, OCT
techniques as herein disclosed may be used for endoscopic imaging or other
internal medicine applications. The foregoing illustrative embodiments of diagnosis
25 and/or evaluation are exemplary and thus embodiments described herein are not
limited to the embodiments discussed.

Although certain embodiments have been illustrated and described herein
for purposes of description, it will be appreciated by those of ordinary skill in the art
that a wide variety of alternate and/or equivalent embodiments or implementations
30 calculated to achieve the same purposes may be substituted for the embodiments
shown and described. Those with skill in the art will readily appreciate that
embodiments described herein may be implemented in a very wide variety of ways.

EXEMPLARY EMBODIMENTS

A. Certain Embodiments

Macular and ONH imaging were performed on three normal volunteers using a swept-source OCT system 900 described herein, as approved by an Institutional Review Board (IRB). For each imaging, the subject's head was stabilized by chin and forehead rests. A flashing internal fixation target was projected by an attenuated pico projector using digital light processing (DLP) technology (Texas Instruments, Dallas, TX, USA). The imaging area on the fundus was visualized by the operator using real-time *en face* view of a 3 mm×3 mm OCT preview scan.

The swept-source OCT system was operated at 100-kHz axial scan repetition rate. In the fast transverse scan (X) direction, the B-scan consisted of 200 A-scans over 3 mm. In the slow transverse scan (Y) direction, there were 200 discrete sampling planes over 3 mm. Eight consecutive B-scans were acquired at each Y position. This is referred to as the "M-B-scan mode" (e.g., as illustrated in Figure 3) because it enables detection of motion between consecutive B-scans at the same position. Thus, it took 3.2 sec to obtain a 3D volumetric data cube comprised of 1600 B-scans and 32,0000 A-scans. Under this scanning protocol, methods described herein were applied to the repeated frame sequences at each step. Finally, the 200 calculated B-scan frames were combined to form 3D blood perfusion images of posterior part of the human eye.

Figure 12 illustrates *in vivo* 3-D volumetric structure images (3.0 (x) X 3.0 (y) X 2.9 (z) mm) of the optic nerve head (ONH) in the right eye of a myopic individual using imaging methods in accordance with various embodiments described herein. From one 3D volumetric dataset, both reflectance intensity images and decorrelation (angiography) images were obtained. For the optical nerve head (ONH) scan, the *en face* maximum projection of reflectance intensity 1202 showed the major retinal blood vessels and the second order branches 1204, but finer branches and the microcirculation of the retina, choroid, and optic disc were not visible. In the vertical cross-sectional intensity image 1208 taken from plane 1206 of projection 1202, the connective tissue struts (bright) and pores (dark) of the lamina cribosa could be visualized deep within the optic disc. Around the disc, the retina, choroid, and sclera can be delineated. The ONH angiogram obtained by the methods described herein showed both many orders of vascular branching as well as the microcirculatory network. The *en face* maximum decorrelation projection

angiogram 1210 showed many orders of branching from the central retinal artery and vein, a dense capillary network in the disc, a cilioretinal artery (reference by an arrow in angiogram 1210 at the nasal disc margin), and a near continuous sheet of choroidal vessels around the disc, much of which could not be visualized well on the *en face* intensity image 1202. The vertical SSADA cross-section decorrelation image 1212 (in the same plane 1206 as 1208 displayed) created showed blood flow in blood vessels in the disc (represented by arrows), retinal vessels, and choroid that form columns from the surface to a depth of ~1.0 mm. It may be unclear if this represents deep penetrating vessels or if this is represents decorrelation projection artifact. Projection artifact refers to the fact that light reflected from deeper static structures may show decorrelation due to passing through a more superficial blood vessel. This type of artifact is evident where the peripapillary retinal vessels seem thicker than they should be, for example in fly-through movie still frame image 1216 and in decorrelation image 1212. Due to this artifact, these vessels extended down the full depth of the nerve fiber layer (NFL), and the decorrelation signal appeared in the subjacent pigment epithelium (RPE), which should be avascular.

To separately view the retinal vessels and superficial disc vessels, pixels were removed below the level of the peripapillary RPE to remove the choroid. The resulting *en face* angiogram 1214 showed that the superficial vascular network nourishes the disc ends at the disc boundary. By comparison, the choroidal circulation formed an almost continuous sheet of blood flow under the retina as shown in 1210. The *en face* images 1202, 1210, and 1214 show RPE atrophy in a temporal crescent just outside the disc margin. Inside the crescent there was also a small region of choriocapillaris atrophy (see the arrow region within 1210). Overlaying the cross-sectional gray scale reflectance intensity image with the color scale flow (decorrelation) image showed that the major retinal branches vessels were at the level of the peripapillary NFL, as shown in fly-through movie still frame image 1216 (i.e., how the disc, retina, and choroid are perfused in a 3D volumetric fashion). It also showed the blood flow within the full thickness of the choroid. The combined image 1216 also showed that the deeper disc circulation resides primarily in the pores of the lamina cribosa and not in the connective tissue struts. This may be the first time that the disc microcirculation has been visualized noninvasively in such a comprehensive manner. The horizontal line across the

image was a result of a fixed pattern artifact that originated from the swept laser source.

Another exemplary embodiment disclosed herein was demonstrated in macular angiography. The macular region of the fundus is responsible for central vision. Capillary dropout in the macular region due to diabetic retinopathy is a major cause of vision loss. Focal loss of the choriocapillaris is a possible causative factor in the pathogenesis of both dry and wet age-related macular degeneration, the leading cause of blindness in industrialized nations. Thus macular angiography is important. The technology described herein was used to demonstrate macular angiography of both the retinal and choroidal circulations in a normal eye as shown in the *in vivo* 3-D volumetric structure images (3.0 (x) X 3.0 (y) X 2.9 (z) mm) of the macula in Figure 13.

The vascular pattern and capillary networks visualized using the technology disclosed herein were similar to those previously reported using phase-based OCT angiography techniques. The flow pixels formed a continuous microcirculatory network in the retina. There was an absence of vascular network in the foveal avascular zone (as shown in *en face* maximum decorrelation projection angiogram 1302) of approximately 600µm diameter, in agreement with known anatomy. There were some disconnected apparent flow pixels within the foveal avascular zone due to noise. Horizontal OCT cross section through the foveal center (upper dashed line in 1302) with merged flow information (decorrelation represented in bright/color scale) and structure information (reflectance intensity represented in gray/darker scale) is represented with foveal center image 1304. Inspection of foveal center image 1304 shows these false flow pixels to be decorrelation noise in the high reflectance layers of the RPE and photoreceptors. The choriocapillaris layer forms a confluent overlapping plexus, so it is to be expected that the projection image of the choroid circulation (see *en face* maximum decorrelation projection angiogram of the choroidal circulation 1306) shows confluent flow. Similar to 1304, a merged horizontal OCT cross section of the inferior macula (lower dashed line in 1302) is represented with inferior macula image 1308. The cross section images 1304 and 1308 showed retinal vessels from the NFL to the outer plexiform layer, in agreement with known anatomy. The flow in the inner choroid had higher velocity as based on decorrelation seen in the bright/color scale. The volume was also greater than the retinal circulation (as shown in the cross section images 1304 and

1308), again consistent with known physiology that the choroidal circulation has much higher flow than the retinal circulation. There were signal voids in the outer choroid which may be due to fringe washout from high flow velocity and the shadowing effect of overlying tissue. The cross section images 1304 and 1308 also
5 showed a few spots of decorrelation in the RPE layer. These are likely artifacts because the RPE is known to be avascular. As mentioned previously, this is likely due to the projection of decorrelation of flow in a proximal layer (i.e., inner retinal layers) onto distal layers with a strong reflected signal (i.e., RPE). There was also a tendency for vessels to form vertical arrays in the inner retina, which may in some
10 instances be due to the projection artifact as well.

Another embodiment disclosed herein was demonstrated to appreciate the differences between full-spectrum, pixel-averaging, and split-spectrum techniques (as described in Figure 1) for decorrelation-based angiography. To obtain angiograms, the methods described above were used, in particular with reference
15 to Figure 1 and as described by equations (1)-(3), respectively. For fair comparison, identical motion error reduction, noise threshold, and *en face* projection methods were used.

Figure 14 illustrates *en face* angiograms of macular retinal circulation using methods in accordance with prior art methods full-spectrum (1402) and pixel-averaging (1404) and in accordance with various embodiments described herein (1408). While the prior art methods and those described herein provided good visualization of major macular vessels, the capillary network looked the cleanest and most continuous in split-spectrum angiogram 108 generated with the split-spectrum embodiment. The pixel-averaging method producing pixel-averaging
20 angiogram 1404 displays the second cleanest and continuous capillary network. The full-spectrum method producing full-spectrum angiogram 1402 showed significantly more disconnected flow pixels that were likely to be noise. The noise can be most easily appreciated in the foveal avascular zone (inside the yellow circles of 1402A, 1402B, and 1408C images of 600-um diameter), which should not
25 have any retinal vessels, including capillaries. In the split-spectrum angiogram 1408, there was a near continuous visualization of the capillary network just outside the avascular zone, while this loop appeared broken up using the other two prior art techniques. The cross-sectional angiograms for each method as displayed in 1402D, 1404E, and 1408F (all scanned across a horizontal dashed line as shown
30

in 1402A showed that the split-spectrum method provided the cleanest contrast between distinct retinal vessels and dark background. Again, the pixel-averaging method was second best, and the full-spectrum method showed visible snow-like background noise.

5 To obtain quantitative figures of merit to compare the three decorrelation-based angiography techniques, two pieces of anatomic knowledge were used. One is that the retinal vessels form a continuous network, and the other is that there are no retinal vessels within the foveal avascular zone. Figure 15 illustrates *in vivo* images depicting vascular connectivity and signal to noise ratio (SNR) using
10 methods in accordance with prior art methods and in accordance with various embodiments described herein. In Figure 15, images 1502A1- 1502A4 were obtained using the full-spectrum method (all in row 1502), images 1504B1-1504B4 were obtained using the pixel-averaging method (all in row 1504), and images 1506C1-C4 were obtained using the split-spectrum technology described herein.
15 To assess vessel connectivity, the projection images (1402A, 1404B, and 1408C of Figure 14) obtained by the three different methods were converted to binary images (e.g., binarized) (as shown in the images in first column 1508 of Figure 15, images 1502A1, 1504B1, and 1506C1) based on a fixed threshold. Then a skeletonizing morphological operation (e.g., skeletonized) was applied to obtain a vascular
20 network made of 1-pixel wide lines and dots (as shown in the images in second column 1510 of Figure 15, images 1502A2, 1504B2, and 1506C2). Next the unconnected flow pixels were separated from the connected flow skeleton (e.g., filtered to remove unconnected flow pixels) (as shown in the images in third column 1512 of Figure 15, images 1502A3, 1504B3, and 1506C3). The vascular
25 connectivity was defined as the ratio of the number of connected flow pixels to the total number of flow pixels on the skeleton map. Connectivity was analyzed on the OCT macular angiograms of six eyes of the three participants (see Table 1 below). A comparison of the three techniques based on paired *t*-tests showed that the split-spectrum technology had significantly better connectivity relative to the pixel-
30 averaging ($p = 0.037$) and full-spectrum ($p = 0.014$) techniques. The split-spectrum technology disclosed herein reduced the number of unconnected flow pixels (18%) by more than a factor of 2 when compared with the full-spectrum prior art technique (39%).

To compute a signal to noise (SNR) for the decorrelation signal, it was necessary to define relevant signal and noise regions. For the macula, fortuitously, the central foveal avascular zone (FAZ) is devoid of blood vessels, including capillaries. The parafoveal capillary network nourishes the fovea and the loss of
 5 these capillaries in diabetic retinopathy is an important mechanism in the loss of vision. Thus the ratio of decorrelation value in the parafoveal region relative to the FAZ can be a clean and clinically relevant way to compute SNR.

In the fourth column 1512 of Figure 15, images 1502A4, 1504B4, and 1506C4, show decorrelation SNR, where the noise region was inside the foveal avascular
 10 zone (displayed as inner dotted circles with radius R1) and the signal region was the parafoveal annulus (as displayed the grayed region between radius R2 and radius R3). The radius of the FAZ (R1) is approximately 0.3 mm. Therefore, it was chosen that the central FAZ with a radius of 0.3 mm was the noise region and the annular parafoveal region between 0.65 (R2) and 1.00 mm (R3) radii was the signal
 15 region. Therefore, the decorrelation signal-to-noise ratio *DSNR* can be represent using the following formula:

(7)

$$DSNR = \frac{\overline{D}_{Parafovea} - \overline{D}_{FAZ}}{\sqrt{\sigma_{FAZ}^2}}$$

20 where $\overline{D}_{Parafovea}$ and $\overline{D}_{FAZ}$ are the average decorrelation values within the parafoveal annulus and FAZ, respectively; and σ_{FAZ}^2 is the variance of decorrelation values within the FAZ. These computations were performed over the *en face* maximum projection images.

The *DSNR* was analyzed on the OCT macular angiograms performed on six
 25 eyes of the three participants (see Table 1 below). The paired *t*-test showed that the *DSNR* of the split-spectrum technology was significantly higher than the pixel-averaging technique ($p = 0.034$) and the full-spectrum technique ($p = 0.012$). The split-spectrum technology improved the *DSNR* by more than a factor of 2 compared to the full-spectrum technique.

30

Table 1. Vascular Connectivity and Signal-to-Noise Ratio of Three Angiography Algorithms

Amplitude decorrelation	Connectivity (mean$\pm$sd)	Improvement of connectivity	<i>DSNR</i> (mean$\pm$sd)	Improvement of <i>DSNR</i>
full-spectrum	0.61 $\pm$ 0.08	N/A	3.30 $\pm$ 0.81	N/A
pixel-averaging	0.70 $\pm$ 0.06	14.8%	4.57 $\pm$ 1.08	38.5%
split-spectrum	0.82 $\pm$ 0.07	34.4%	6.78 $\pm$ 0.82	105%

DSNR = decorrelation signal-to-noise ratio. Statistical analysis is based on 6 eyes of 3 normal human subjects.

5

Utilizing the technology disclosed, visualization of both larger blood vessels and the capillary network in the retinal and choroidal circulations has been demonstrated. This visualization can also been achieved using Doppler and other phase-based flow detection techniques, however the SSADA (i.e., the split-spectrum) techniques disclosed have several potential advantages over phase-based techniques. Insensitivity to phase noise is one advantage. Another advantage includes the ability to quantify microvascular flow. Because the effective resolution cell is made isotropic (having the same size in X, Y, and Z dimensions, as described in Figure 2), it is equally sensitive to transverse (X, Y) and axial (Z) flow. This contrasts with all phase-based techniques, which are intrinsically more sensitive to flow in the axial direction over which Doppler shift occurs. Thus utilizing the technology disclosed results in the decorrelation value as a function of the flow velocity regardless of direction. The faster blood particles move across the laser beam, the higher the decorrelation index of the received signals within a velocity range set by the scan parameters. In theory the saturation velocity should be approximately the size of the resolution cell (0.018 mm) divided by the interframe time delay (0.002 sec), or 9 mm/sec. The minimum detectable flow velocity can be determined by the decorrelation noise floor, which can be based on the decorrelation distribution statistics of the non-flow tissue voxels. In this example, the projection view of split-spectrum technology showed the vascular pattern within the macular capillary zone (parafoveal region). This describes that the split-spectrum technology disclosed is able to detect retinal capillary flow, which is within

25

the range of 0.5-2 mm/sec. Calibration of velocity to decorrelation values using *in vitro* flow phantom experiments can be done to further determine the minimum detectable flow velocity.

5 The projection of flow from proximal (shallower) layers to distal (deeper) layers can be challenging. Flow in the major peripapillary retinal arteries and veins (as shown in Figure 12) and larger macular vessels in the inner retina (as shown in Figure 13) projects onto the highly reflective RPE, which should not contain any blood vessels. There were also probable projection of flow from the more superficial inner retinal layers (i.e. nerve fiber layer and ganglion cell layer) to the
10 deeper inner retinal layers (i.e. inner and outer plexiform layers). This does not affect the accuracy of *en face* projection of the retinal circulation, but it could affect the accuracy of cross-sectional angiograms and *en face* projection of the choroidal circulation. One can raise the threshold decorrelation value for flow identification in deeper voxels if a more superficial voxel has a suprathreshold decorrelation value;
15 however, this can inevitably introduce a potential shadow artifact in place of a flow projection artifact. Thus, images of deeper vessels can be interpreted with this artifact in mind.

Noise from bulk tissue motion, while dramatically reduced using the technology disclosed herein, may not be entirely eliminated. As described in the
20 examples disclosed, no attempt was made to compensate for X-Z motion between consecutive B-scan frames by the use of frame-shift registration. This registration can likely reduce the effect of bulk motion in the X-Z dimensions (though not in the Y direction) and improve the accuracy of flow detection further. It is also apparent from the *en face* angiograms that there are saccadic motion artifacts in the 3D
25 dataset. This can likely be reduced by the use of 3D registration algorithms.

Figure 16 illustrates *in vivo* images using methods in accordance with various embodiments described herein, including a multiple rings circular scan pattern (e.g. a ring number of 4 and a diameter of 1.6-2.2mm) and Doppler angle estimation for a single vessel. A vessel center line can be constructed based on
30 vessel center position with spline curve fitting. The flow vector at each circle can be estimated using the tangential vector of vessel center line.

The multiple ring circular scan can be done with an ultrahigh-speed OCT. The scan pattern can include multiple concentric circular scans with 4 or more diameters. At each location (e.g., diameter), the circular scan can be repeated to

cover the cardiac cycle and reduce the effect of eye movement. The total scan time can cover at least one cardiac cycle. The axial scan density can be high for precise Doppler shift signal calculation.

After the scan is obtained, the vessel location can be detected on each frame for each vessel. For a particular vessel, the center positions on the scans can be used to reconstruct a vessel center line curve. The curve can be used to estimate the Doppler angle between OCT beam and vessel normal vector (as shown figure 16). The angle θ can be calculated between the OCT beam and the flow vector, which is the tangential vector of the vessel center line at vessel center. Then, the Doppler angle can be estimated as $90 - \theta$.

With the angle and Doppler shift signal, the blood flow can be estimated by the following equation,

(8)

$$Flow = \frac{1}{n} \sum_{i=1}^n \iint_{\text{vessel area}} \frac{\lambda \Delta f_i dx dz}{2n \sin(\alpha_i)}$$

where, λ : is center wavelength of the OCT laser source, Δf_i is Doppler shift signal in i th circular scan, n is refractive index, α is Doppler angle on i th circular scan, which is equal to $90 - \theta$, θ is the angle between vessel vector and OCT beam on i th circular scan. When the Doppler angle is close to 0, it can be difficult to detect the vessel position automatically. To solve this problem, an OCT angiography scan can be added into the multiple ring circular scan. For each position (diameter), except the single circular scan which creates Doppler OCT image, multiple circular scans with less axial-scan density can be done just before or after the Doppler scan and the angiography techniques described herein (e.g., SSADA) can be applied to get the OCT angiograph. The Doppler scan and angiography scan can be registered, as they are done at the same location, and eye movement should be small in such short period (< 0.1 seconds). Then, vessel positions and regions detected on the angiograph scan can be mapped to the Doppler scan.

In order to get precise flow vector estimation, the interval of circle diameter can be reduced. This can involve increasing the number of circles and therefore the total scan time would increase. In clinical practice, the total scan time is

desired to be about 2 seconds. Therefore there is a compromise between scan time and the accuracy of angle estimation in multiple ring circular scanning. To solve this problem, flow vector from a 3D OCT angiograph can be obtained. The 3D angiograph scan can cover the Doppler scan area. The vessel position can be manually or automatically detected on the 3D angiograph and the 3D vessel structure around the optic disc can be reconstructed. The circular Doppler scan and/or circular angiograph scan can be registered to the 3D angiograph scan. An automatic rigid registration based on the vessel pattern and inner limited membrane can be utilized. After the registration, the 3D vessel structure can be mapped to the Doppler scan for vessel detection and angle estimation.

For example, on a swept-source OCT with 100,000 ascan/second scan rate, a four ring circular scan pattern was implemented. The scan diameter utilized was 2.2mm, 2.0mm, 1.8mm and 1.6mm. 8 fast circular scans (500 A scans) followed by 1 slow circular scan (4000 A scans) were scanned on each diameter. Then the scans on 4 diameters were repeated 6 times. Together, the scans took about 2 seconds, within the desired clinical timeframe. The faster scans were used to calculate the OCT angiograph and the slow scan was used to calculate the Doppler shift signal. A 3X3mm 3D OCT angiography was also obtained. Figures 17 A-D illustrates *in vivo* images using methods in accordance with various embodiments described herein, including multiple rings circular scan Doppler OCT in combination with SSADA to provide total retinal blood flow (TRBF) measurement as mentioned above. The multiple ring circular scan was used to calculate the total retinal blood flow around the optic disc using information from both arteries and veins. Figure 17A shows an *en face* OCT angiogram computed with the SSADA technology disclosed herein. The vascular pattern, including branching and crossing, can be extracted using a graph search technique. Figure 17B shows a cross-section SSADA angiogram providing precise positions of the top boundary of retinal vessels (depicted with arrow heads.) Figure 17C shows a color Doppler display of a section of a circular scan showing the blue and red Doppler shifts in lumen cross-section that can be used for velocity calculations. One vessel (as noted with a green arrowhead) is visible on decorrelation-based angiography image shown in Figure 17B, but is not on the color Doppler image shown in Figure 17C. This visualizes decorrelation angiography reliably defining vessel anatomy, while Doppler shift can provide more quantitative velocity information. Figure 17D shows

a composite image showing Doppler measurements (blue & red vessel segments) from the circular scans overlaid on the *en face* summation view of the 3D OCT scan. This visualization shows that the vessel trajectory (e.g, position, slope, and curvature fit by second order spline function,) branching, and crossing can be characterized by the combination of multi-circular and 3D scans, thereby allowing for accurate measurement of TRBF (e.g., by summing flow measurements in arteries and veins in a region and dividing by half.)

B. Additional Embodiments

Certain embodiments are directed to novel quantitative systems for measuring ocular blood flow as described below. Specifically, these systems are able to measure circulation in ONH (e.g. whole disc/temporal ellipse, peripapillary retina, peripapillary choroid) and macula (e.g. macular retina, macular choroid, fovea avascular zone and the area of non-perfusion). Quantification of different circulation obtained from glaucoma patients compared with that from normal subjects is herein described.

Acquisition of 3D Decorrelation Image

Design of 3D scan pattern

The 3D scan pattern 100 to scan macula and disc of the eye is optimized to implement split-spectrum amplitude decorrelation algorithm (SSADA) [Jia et al., *Opt. Express* 20:4710-4725 (2012)]. It is illustrated in Figure 18. For each 3D volumetric data 102 comprising data obtained via an M-B-scan mode from an OCT system. M-B-scan 104 is composed by N consecutive B-scans at a single Y position (e.g. N=8). Therefore, for each 3D volumetric data 102, in the fast scan axis, a single B-scan comprises a number of A-scans 106, and in the slow scan axis, there are a number of M-B-scans 104 comprising N consecutive B-scans. For example, the scan pattern used for an OCT system with a scan speed of 100K axial scan/second can contain 200 A-lines covering 3mm along fast scan direction, and contain 200 M-B-scans (N=8) along slow scan direction. One 3D data set 102 can be acquired in 3.4 seconds. The repeated B-frames 104 are used for the SSADA calculation to obtain both the structure and blood flow images.

Application of SSADA

As described previously [Jia et al., *Opt. Express* 20:4710-4725 (2012)], SSADA can split the spectrum into different frequency bands and calculate decorrelation in each band separately (Figure 19). The decorrelation (flow) images from the multiple spectral bands can then be averaged together to make full use of the speckle information in the entire OCT spectrum. By splitting the full OCT spectral interferograms into several wavenumber bands, the OCT resolution cell in each band is modified intentionally and less susceptible to axial motion noise.

For visualization purposes, the modified resolution cell is unnecessary to be exactly isotropic; however, for quantification purposes, the isotropic resolution cell is the key point because it can be sensitive to axial and transverse flow equally. In other words, decorrelation value derived from isotropic resolution cell is proportional to velocity regardless of direction. Figure 19 is an example to explain how to split raw interference spectrum 202 and create an isotropic resolution cell 212. For a swept source OCT setup, the axial (Z) resolution in the resolution cell 206 is determined by the source central wavelength (1050nm) and its spectral bandwidth 204 (69nm); and the lateral (X and Y) resolution is determined by the laser beam profile. Using the full-width-half maximum (FWHM) amplitude profile definition, the axial resolution (5.3 μ m) is 3.3 times higher than the lateral resolution (17.7 μ m) in the resolution cell 206 where $X=Y=3.3Z$. In order to create an isotropic resolution cell 212 where $X=Y=Z$, spectrum should be split into different frequency bands with the new bandwidth 210 of 21 μ m (e.g. split-spectrum 208). Please note the overlap between different spectral bands can be increased to further enhance image quality, which might also increase computing time.

Quantitative Blood Flow Assessment

A flowchart of quantitative blood flow measurements is provided in Figure 20. It begins with the detection of measurement flow volumes using reliable anatomical landmarks on reflectance images and ends up with the calculation of two blood flow parameters: flow index and vessel density. Additionally, the measurement of non-perfusion area is also demonstrated for the quantification purpose.

Detection of measurement volumes

Based on the 3D volumetric data set 102 from the above scanning protocol 100, SSADA algorithm 303 is performed on raw interference spectrum 302 and both reflectance intensity images 304 and decorrelation (flow) images 306 can be obtained simultaneously. If necessary, the image distortion due to the saccadic motion artifacts can be reduced by performing 3D registration 307 [Kraus et al., *Biomed. Opt. Express* 3:1182-1199 (2012)]. When registered B-scan reflectance 308 and registered B-scan flow 310 are processed, at 311, the anatomical landmarks are identified on B-scan reflectance 308 and used for the segmentation of B-scan flow 310. At 313, maximum projection algorithm [Jia et al., *Opt. Express* 20:4710-4725 (2012)] is applied on both reflectance 308 and segmented flow 312 image. The projection algorithm finds the maximum reflectance and decorrelation value for each transverse position, representing the highest reflectance and fastest flowing vessel lumen respectively. Next, at 317, the landmarks on *en face* reflectance 314 are identified and used to mask *en face* segmented flow image 316. Then segmented *en face* flow image 318 is obtained and used for calculation of flow index 320 and vessel density 322.

Figure 21 shows the specific segmentation within various ocular vascular beds, which is also summarized in Table 2 below. At ONH region, segmentation at B-scan for whole disc 410 and temporal ellipse 420 is supplementary data and of lesser value, so all signals between internal limiting membrane (ILM) 411 and bottom can remain. The ellipse bounding neural canal opening (NCO) 412 can be selected for whole disc angiography 413 and ellipse at temporal area (tilted along disc-fovea axis) 422 for temporal ellipse angiography 423. For peripapillary retina 430, the region between ILM 411 and the inner-segment/outer-segment (IS/OS) junction plane 431 is for retina and 0.5 mm wide region surrounding the disc ellipse 432 can be demarcated for peripapillary region. For peripapillary choroid 440, the

- region between retinal pigment epithelium (RPE) 441 and 50 μ m below it is for choroid and peripapillary region is same as defined above. At macula region, macula retina 450 can be separated by segmenting the region between ILM 411 and IS/OS 431 at B-scan and 1mm wide region 452 surrounding fovea avascular zone (FAZ) 451 at en face flow image to obtain perifovea macular angiography 453; macula choroid 460 can also be extracted by choosing the region between RPE 441 and 50 μ m below it at B-scan and a round region 462 centered at FAZ 451.

Table 2. Summary of segmentation of various vascular beds

Vascular beds	Segmentation at B-scan	Segmentation at En face
ONH – Whole Disc (410)	Between ILM (411) and bottom	Ellipse bounding NCO (412)
ONH – Temporal Ellipse (420)	Between ILM (411) and bottom	Ellipse at temporal area (tilted along disc-fovea axis) (422)
Peripapillary Retina (430)	Between ILM (411) and IS/OS (431)	0.5 mm wide region (432) surrounding the disc ellipse (412)
Peripapillary Choroid (440)	Between RPE (441) and 50 μ m below it	0.5 mm wide region (432) surrounding the disc ellipse (412)
Macular Retina (450)	Between ILM (411) and IS/OS (431)	1 mm wide region (452) surrounding FAZ (451) (D=0.6 mm)
Macular Choroid (460)	Between RPE (441) and 50 μ m below it	Round region (462) (D=2.6 mm) centered at FAZ (451)

- Dividing boundaries at B-scans can be identified through the analysis of the reflectance gradient profiles in depth. The disc boundary can be identified by detecting the boundary of NCO and the FAZ 451 boundary can be identified by the retina thickness map on the macula on which the thinnest point is the center of FAZ 451 and the circle region with diameter of 600 μ m is the size of FAZ 451 [Roh and

Weiter, "Retinal and Choroidal Circulation" in *Ophthalmology*, M. Yanoff and J.S. Duker eds. (Mo: Mosby Elsevier, St. Louis, 2008)]. Other boundary detection skills can also be applied for the identification of landmarks.

It should be noted that in ONH scans, the IS/OS 431 and the RPE 441 plane
5 can be set by interpolating their depth just outside the disc boundary for segmentation at B-scans. Other alternative segmentation methods for ONH scans can also be used. For example, as shown by Figure 22, both retina 504 and ONH 506 can be segmented away from choroid 508 through the entire 3D volume 502 and then segment the *en face* retina and ONH angiography 510 and *en face*
10 choroid angiography 512 to obtain whole disc 410, temporal ellipse 420 and peripapillary retina 430 and choroid 440. In addition, the choroid of 50 μ m can be chosen to better represent the inner choroidal part, choriocapillaris layer [Roh and Weiter, "Retinal and Choroidal Circulation" in *Ophthalmology*, M. Yanoff and J.S. Duker eds. (Mo: Mosby Elsevier, St. Louis, 2008)] and to avoid the effects from the
15 signal voids in the outer choroid [Jia et al., *Opt. Express* 20:47190-4725 (2012)]. Alternatively, choroid thickness can also be slightly changed.

An example demonstrating how to detect optic disc boundary 412 and temporal ellipse of disc 422 is described herein below and in Figure 23. The NCO 604, which is the termination of the retinal pigment epithelium (RPE)/Bruch's
20 membrane (BM) complex [Strouthidis et al., *Invest. Ophthalmol. Vis. Sci.* 50:214-223 (2009) and Hu et al., *Invest. Ophthalmol. Vis. Sci.* 51:5708-5717 (2010)], can be used to define the ONH margin 412 [Strouthidis et al., *Invest. Ophthalmol. Vis. Sci.* 50:4709-4718 (2009)]. In OCT cross-sectional B-scans, the boundary of the NCO 604, indicated by two green dashed lines 606 is determined by the
25 termination of the RPE/BM complex (two green arrows) 604. It corresponds to the two margin points 608 at the disc region. These representative margin points are transferred on the corresponding flow cross-sectional image 610 and *en face* projection maps 612. The boundary produced by the surrounding peripapillary choroidal blood flow 614 in the flow data 502 is not optimally used as the detection
30 method for disc margin 412.

Because the NCO 604 is detectable, it can be manually delineated on the reflectance projection image 314. Shown by Figure 24, the major 702 and minor axes 704 of the ellipse are calculated along the vertical and horizontal directions. The approximate center of disc is the centroid of the selected ellipse 706.

After the position and dimensions of a disc are determined, the whole disc 412 and temporal ellipse areas 422 can be segmented for quantitative analysis. The optic disc mask 708 is idealized as an ellipse with vertical diameter (VD) 702 and horizontal diameter (HD) 704. The mask value is 1 inside the ellipse and 0 outside. An elliptical mask 710 is also defined for the disc region temporal to the major superior and inferior branch arteries and veins. The temporal ellipse 422 has a major axis diameter of 0.75 VD and a minor axis diameter of 0.50 HD. The temporal ellipse is tilted inferiorly to fit the tilt of the disc vessel pattern associated with the tilt of the disc-fovea axis 712. According to the literature measurements on the normal population [J. M. McDonnell, "Ocular embryology and anatomy," in *Retina*, S. J. Ryan, ed. (CV Mosby, St Louis, 1989), pp. 5–16], the average value of this angle is 7.1°. The temporal ellipse angiography 423 does not contain any major branch retinal blood vessels and therefore may be a better measure of local disc microcirculation.

15 Definition and Calculation of flow index and vessel density

By multiplying different masks 317 with original blood flow projection map 316, respectively, the segmented flow maps 318 can be acquired for further quantification.

The flow index 320 is defined as the average decorrelation values in the segmented area, which can be given by,

$$\frac{\int_A D \cdot V dA}{\int_A dA} \quad (V=1, \text{ if vessel; } V=0, \text{ if not}) \quad (1)$$

The vessel density is defined as the percentage area occupied by vessels in the segmented area, using the following formula,

$$\frac{\int_A V dA}{\int_A dA} \quad (V=1, \text{ if vessel; } V=0, \text{ if not}) \quad (2)$$

Where A can be segmented *en face* flow area 318, D is the decorrelation value acquired by SSADA 303. The threshold used to judge V is 1 or 0 and was set at 0.125, two standard deviations above the mean decorrelation value in noise region. As described by previous report [Jia et al., *Opt. Express* 20:4710-4725 (2012)], the central FAZ 451 in the normal eyes can be chosen as a noise region after the same scanning pattern 100 was applied on the macular region, and then calculated decorrelation values by SSADA 303.

Detection fovea avascular zone and other areas of non-perfusion

First, a macular retinal angiography 802 of 200 X 200 pixels, as shown in Figure 25, is obtained by projecting 3D retinal vasculature 502 segmented between ILM 411 and IS/OS 431. Then this angiography 802 can be smoothed through a Gaussian filter 803. A Gaussian filter 803 is an effective smoothing filter for random noise reduction. In practice, the standard deviation and the window size of a Gaussian filter 803 should be chosen with care to smooth the capillary bed around FAZ 451. Their values are usually chosen based on the diameters of main retinal vessel branches 804. Typically, a σ value of 75 μ m is chosen with a window size of 150 μ m $\times$ 150 μ m because visually they generate smoothed 2D angiogram 806 for the subsequent analyses. The non-perfusion information 808 can be computed by identifying the pixels whose values are lower than the noise floor 807. In this part, the parameters chosen for Gaussian filter 803 can be varied according to the pixel size.

C. Further Embodiments

Preliminary studies were carried out utilizing the technology described herein. The swept-source OCT system was operated at the center wavelength of 1050 nm, speed of 100,000 axial scans per second, axial resolution of 5 μ m and spot diameter of 18 μ m (FWHM amplitude). With this configuration and the scan pattern described previously, the B-scan frame rate of the system was 500 frames per second; therefore, 1600 B-scans were acquired to form a 3D data cube, corresponding to an acquisition time of 3.4 seconds.

Both normal and glaucoma groups were studied. Within glaucoma group, two perimetric glaucoma subjects, three pre-perimetric glaucoma subjects and one suspect subjects with ocular hypertension were enrolled for study. In normal subjects, a dense microvascular network was visible on the OCT angiography of

the disc 902, in addition to large retinal vessels. This network was visibly attenuated in all PPG subjects, as shown in the disc 904 of Figure 26. This difference cannot be visualized and quantified by disc photographs normal 906 & PPG 908 respectively. Within the whole disc region, the flow index was reduced by 32% in the glaucoma group. These reductions were statistically significant (see Table 3 below). Regional disc perfusion measurements on the temporal ellipse showed differences between two groups were statistically significant. Thus the estimated reductions were higher than those based on the whole disc region. For this small region quantification, the repeatabilities of the measurements of flow index at whole disc and temporal ellipse were 6.6% and 7.9% respectively. Quantification on peripapillary retina, peripapillary choroid and central macula didn't show any statistical difference between two groups (Table 3).

Table 3 – Quantification of different vascular beds in glaucoma

Flow index (dimensionless)	Normal	Glaucoma + Suspect	P-value (Wilcoxon)
ONH – Whole Disc	0.159 ± 0.020	0.108 ± 0.013	0.008
ONH – Temporal Ellipse	0.151 ± 0.014	0.072 ± 0.022	0.005
Peripapillary Retina	0.141 ± 0.023	0.122 ± 0.024	0.191
Peripapillary Choroid	0.226 ± 0.016	0.168 ± 0.071	0.105
Macular Retina	0.120 ± 0.017	0.112 ± 0.039	0.819

15

In the techniques described herein, the major superior and inferior branches of the retinal vessels on the temporal side were excluded, and quantifications focused mainly on ONH microvascular beds. Preliminary results suggest that in early glaucoma the reduction of ONH microvascular flow is much more dramatic than that of whole ONH circulation. This suggests that quantification performed on microvascular perfusion may be more sensitive for detecting ONH circulatory changes in early glaucoma patients.

20

For ONH angiography, ONH flow index and peripapillary choroidal flow index are important for the diagnosis and evaluation of glaucoma. Differences between normal and glaucoma in a pilot clinical study were shown. Macular angiography is useful for macular diseases. Perifoveal retinal flow index and macular retinal flow map (size of foveal avascular zone, and identification of any other nonperfusion area) are important for the evaluation of macular ischemia in diabetic retinopathy. Macular choroidal flow index and macular choroidal flow map are important in the evaluation of AMD.

In one embodiment, for the diagnosis of age-related macular degeneration, measuring the flow index of and detecting an impairment in blood flow in either/both of the choroidal neovascular membrane and/or macular choroid is of primary importance. In another embodiment, for the diagnosis of glaucoma, measuring the flow index of and detecting an impairment in blood flow in the ocular nerve head is of primary importance. Finally, in yet an additional embodiment, for the diagnosis of diabetic retinopathy, measuring the flow index of and detecting an impairment in blood flow in the perifoveal avascular region is of primary importance. Data confirming the above described correlations not shown (manuscripts in preparation).

The disclosure set forth above encompasses multiple distinct embodiments. While each of these embodiments have been disclosed in its preferred form, the specific embodiments as disclosed and illustrated herein are not to be considered in a limiting sense as numerous variations are possible. The subject matter of the present disclosure includes all novel and non-obvious combinations and subcombinations of the various elements, features, functions and/or properties disclosed herein. Similarly, where any claim recites "a" or "a first" element or the equivalent thereof, such claim should be understood to include incorporation of one or more such elements, neither requiring nor excluding two or more such elements.

Claims

What is claimed is:

- 5 1. A method for quantitatively measuring blood flow in an ocular vascular bed, said method comprising:
- selecting an ocular vascular bed from which to quantitatively measure blood flow;
- scanning said ocular vascular bed to obtain M-B scans of OCT spectrum
- 10 therefrom;
- splitting the M-B scans of OCT spectrum into M spectral bands; and
- determining a quantitative measurement of blood flow from the M spectral bands.
- 15 2. The method of Claim 1, wherein the step of splitting the M-B scans of the OCT spectrum into M spectral bands comprises:
- creating overlapping filters covering the OCT spectrum; and
- filtering the OCT spectrum with the overlapping filters.
- 20 3. The method of Claim 1, wherein the step of determining a quantitative measurement of blood flow from the M spectral bands comprises:
- creating decorrelation images for the M spectral bands; and
- combining the decorrelation images for the M spectral bands to create a flow image.
- 25 4. The method of Claim 3, wherein the step of creating decorrelation images for the M spectral bands comprises:
- determining amplitude information for each spectral band; and
- calculating decorrelation between adjacent amplitude frames for each
- 30 spectral band.
5. The method of Claim 4 further comprising the step of removing background noise.

6. The method of Claim 3, wherein the step of combining the decorrelation images for the M spectral bands to create a flow image comprises:
- averaging the decorrelation images for each spectral band to create an average decorrelation image for each spectral band; and
- 5 averaging the averaged decorrelation images from the M spectral bands.
7. The method of Claim 6, further comprising the step of eliminating decorrelation images for each spectral band having excessive motion noise.
- 10 8. The method of Claim 1, wherein the ocular vascular bed is selected from the group consisting of the ocular nerve head and the macula.
9. The method of Claim 1, wherein the ocular vascular bed is selected from the group consisting of the ocular disc, the temporal ellipse, the peripapillary retina, the peripapillary choroid, the macular retina, the macular choroid, the fovea avascular zone, and the area of non-perfusion.
- 15 10. A method of diagnosing the presence of an ocular disease in a subject suspected of having said ocular disease, said method comprising:
- 20 selecting a specific ocular vascular bed in said subject from which to quantitatively measure blood flow;
- scanning said ocular vascular bed to obtain M-B scans of OCT spectrum therefrom;
- splitting the M-B scans of OCT spectrum into M spectral bands;
- 25 determining a quantitative measurement of blood flow from the M spectral bands; and
- comparing said quantitative measurement of blood flow to that obtained from a normal subject, wherein a decrease in blood flow in the patient suspected of having said ocular disease as compared to that obtained from said normal subject
- 30 is indicative of the presence of said disease.
11. The method of Claim 10, wherein said ocular disease is glaucoma.

12. The method of Claim 11, wherein the specific ocular vascular bed is the optic nerve head.
13. The method of Claim 10, wherein said ocular disease is diabetic retinopathy.
- 5 14. The method of Claim 13, wherein the specific ocular vascular bed is the perifoveal avascular zone
- 10 15. The method of Claim 10, wherein said ocular disease is age-related macular degeneration.
16. The methods of Claim 15, wherein the specific ocular vascular bed is the choroidal neovascular membrane or the macular choroid.
- 15 17. The method of Claim 10, wherein the ocular vascular bed is selected from the group consisting of the ocular nerve head and the macula.
18. The method of Claim 10, wherein the ocular vascular bed is selected from the group consisting of the ocular disc, the temporal ellipse, the peripapillary retina, the peripapillary choroid, the macular retina, the macular choroid, the fovea avascular zone, and the area of non-perfusion.
- 20 19. A system for quantitatively measuring blood flow in an ocular vascular bed, said system comprising:
- 25 an optical coherence tomography apparatus; and
- one or more processors coupled to said apparatus and adapted to cause said apparatus to obtain M-B scans of OCT spectrum from said ocular vascular bed, split the M-B scans of OCT spectrum into M spectral bands, and determine a quantitative measurement of blood flow from the M spectral bands.
- 30 20. The system of Claim 19, wherein the one or more processors adapted to cause the apparatus to split the M-B scans of OCT spectrum into M spectral bands further comprises being adapted to cause the apparatus to create overlapping

filters covering the OCT spectrum and filter said OCT spectrum with the overlapping filters.

21. The system of Claim 19, wherein the one or more processors adapted to
5 cause the apparatus to determine a quantitative measurement of blood flow from the M spectral bands further comprises being adapted to cause the apparatus to create decorrelation images for the M spectral bands and combine the decorrelation images for the M spectral bands to determine a quantitative measurement of blood flow.

10

22. The system of Claim 21, wherein the one or more processors adapted to cause the apparatus to create decorrelation images for M spectral bands further comprises being adapted to cause the apparatus to determine amplitude information for each spectral band and calculate decorrelation between adjacent
15 amplitude frames for each spectral band.

23. The system of Claim 21, wherein the one or more processors adapted to cause the apparatus to combine the decorrelation images for the M spectral bands to determine a quantitative measurement of blood flow further comprises being
20 adapted to cause the apparatus to average the decorrelation images for each spectral band to create and average decorrelation image for each spectral band and average the averaged decorrelation images from the M spectral bands.

FIG. 1

100

	Amplitude Decorrelation	Vascular Connectivity	Decorrelation Signal/Noise (DSNR)
102 Full Spectrum (Prior Art)	-----	-----	-----
112 Pixel Averaging (Prior Art)	↑	↑	↑
122 Split-Spectrum	↑↑	↑↑↑	↑↑↑

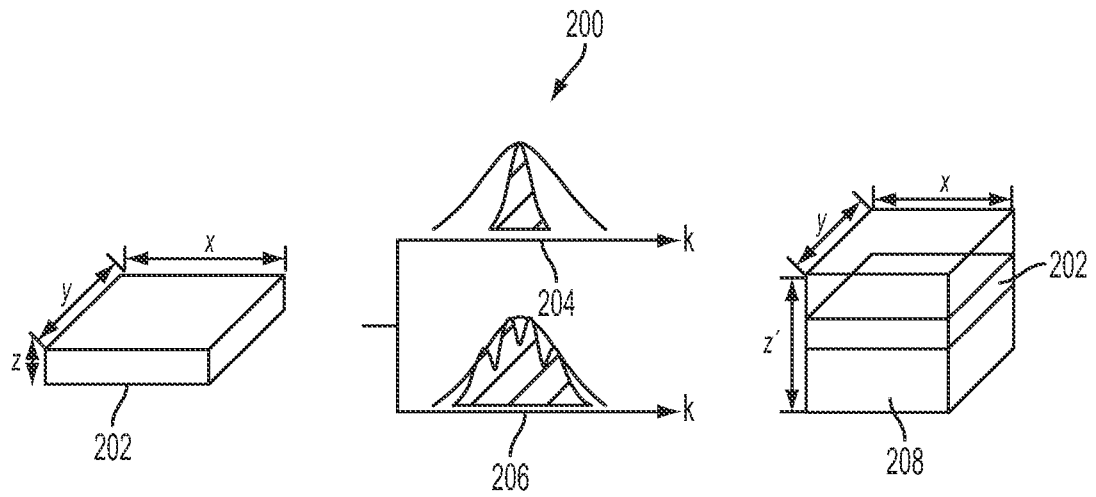


FIG. 2

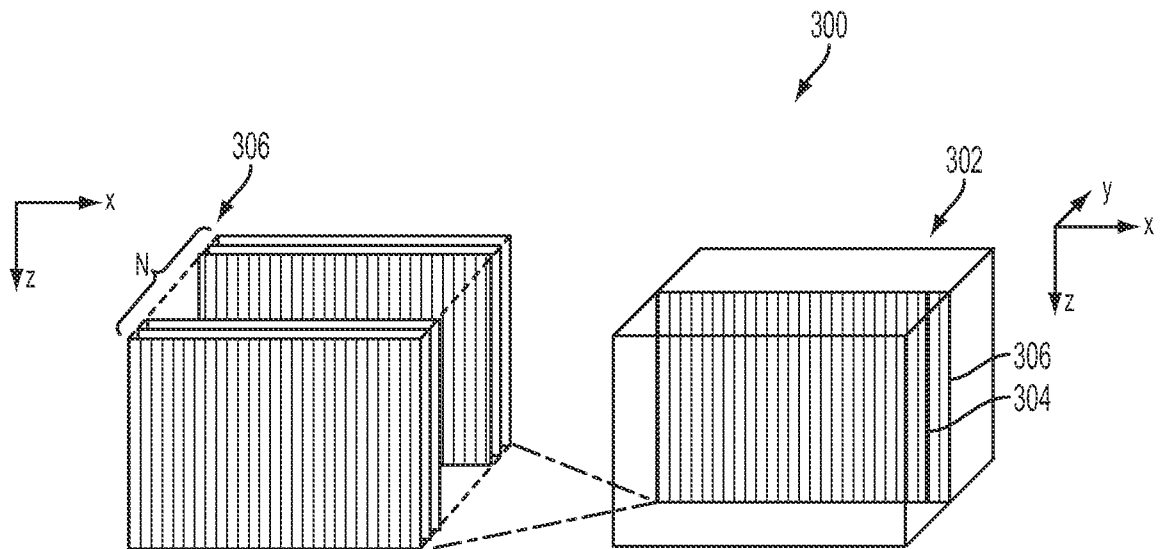


FIG. 3

FIG. 4


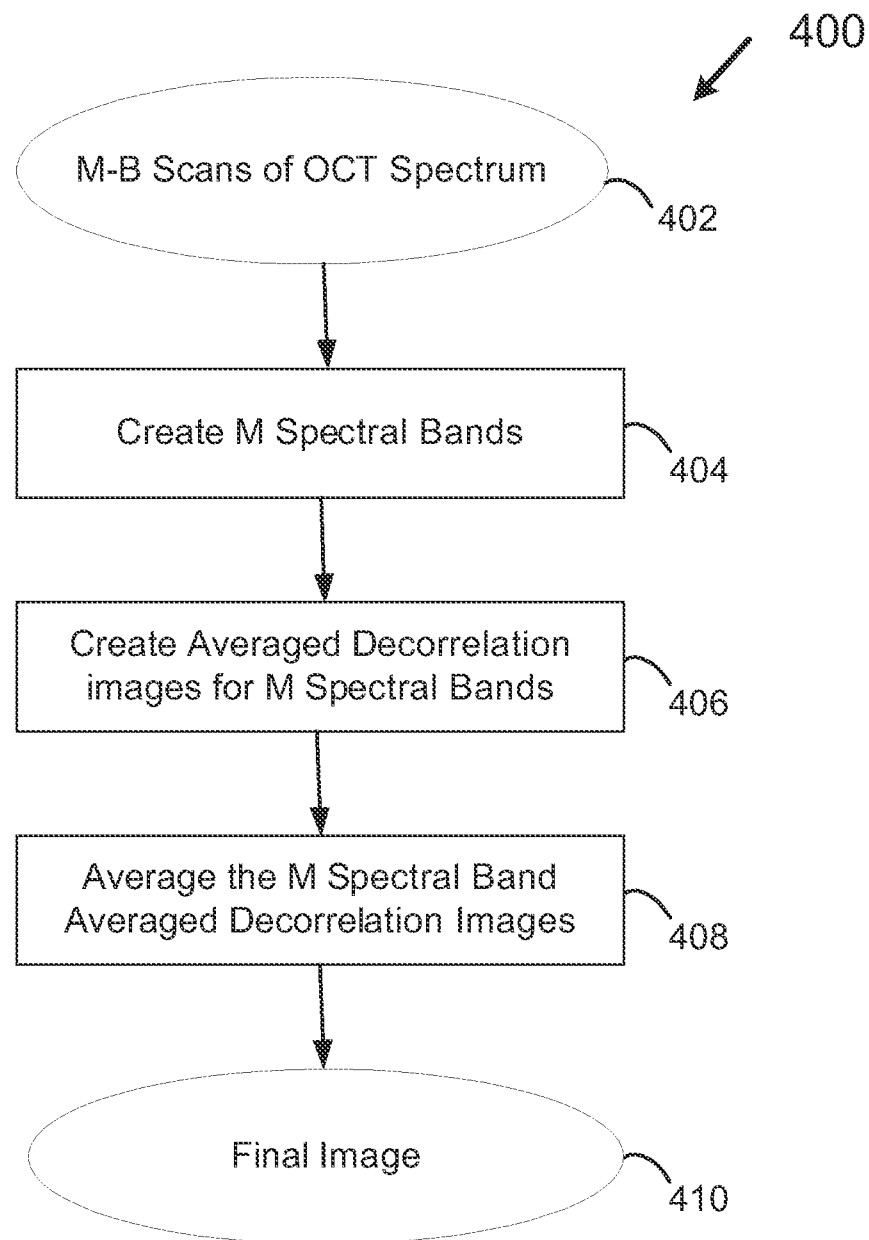


FIG. 5

500

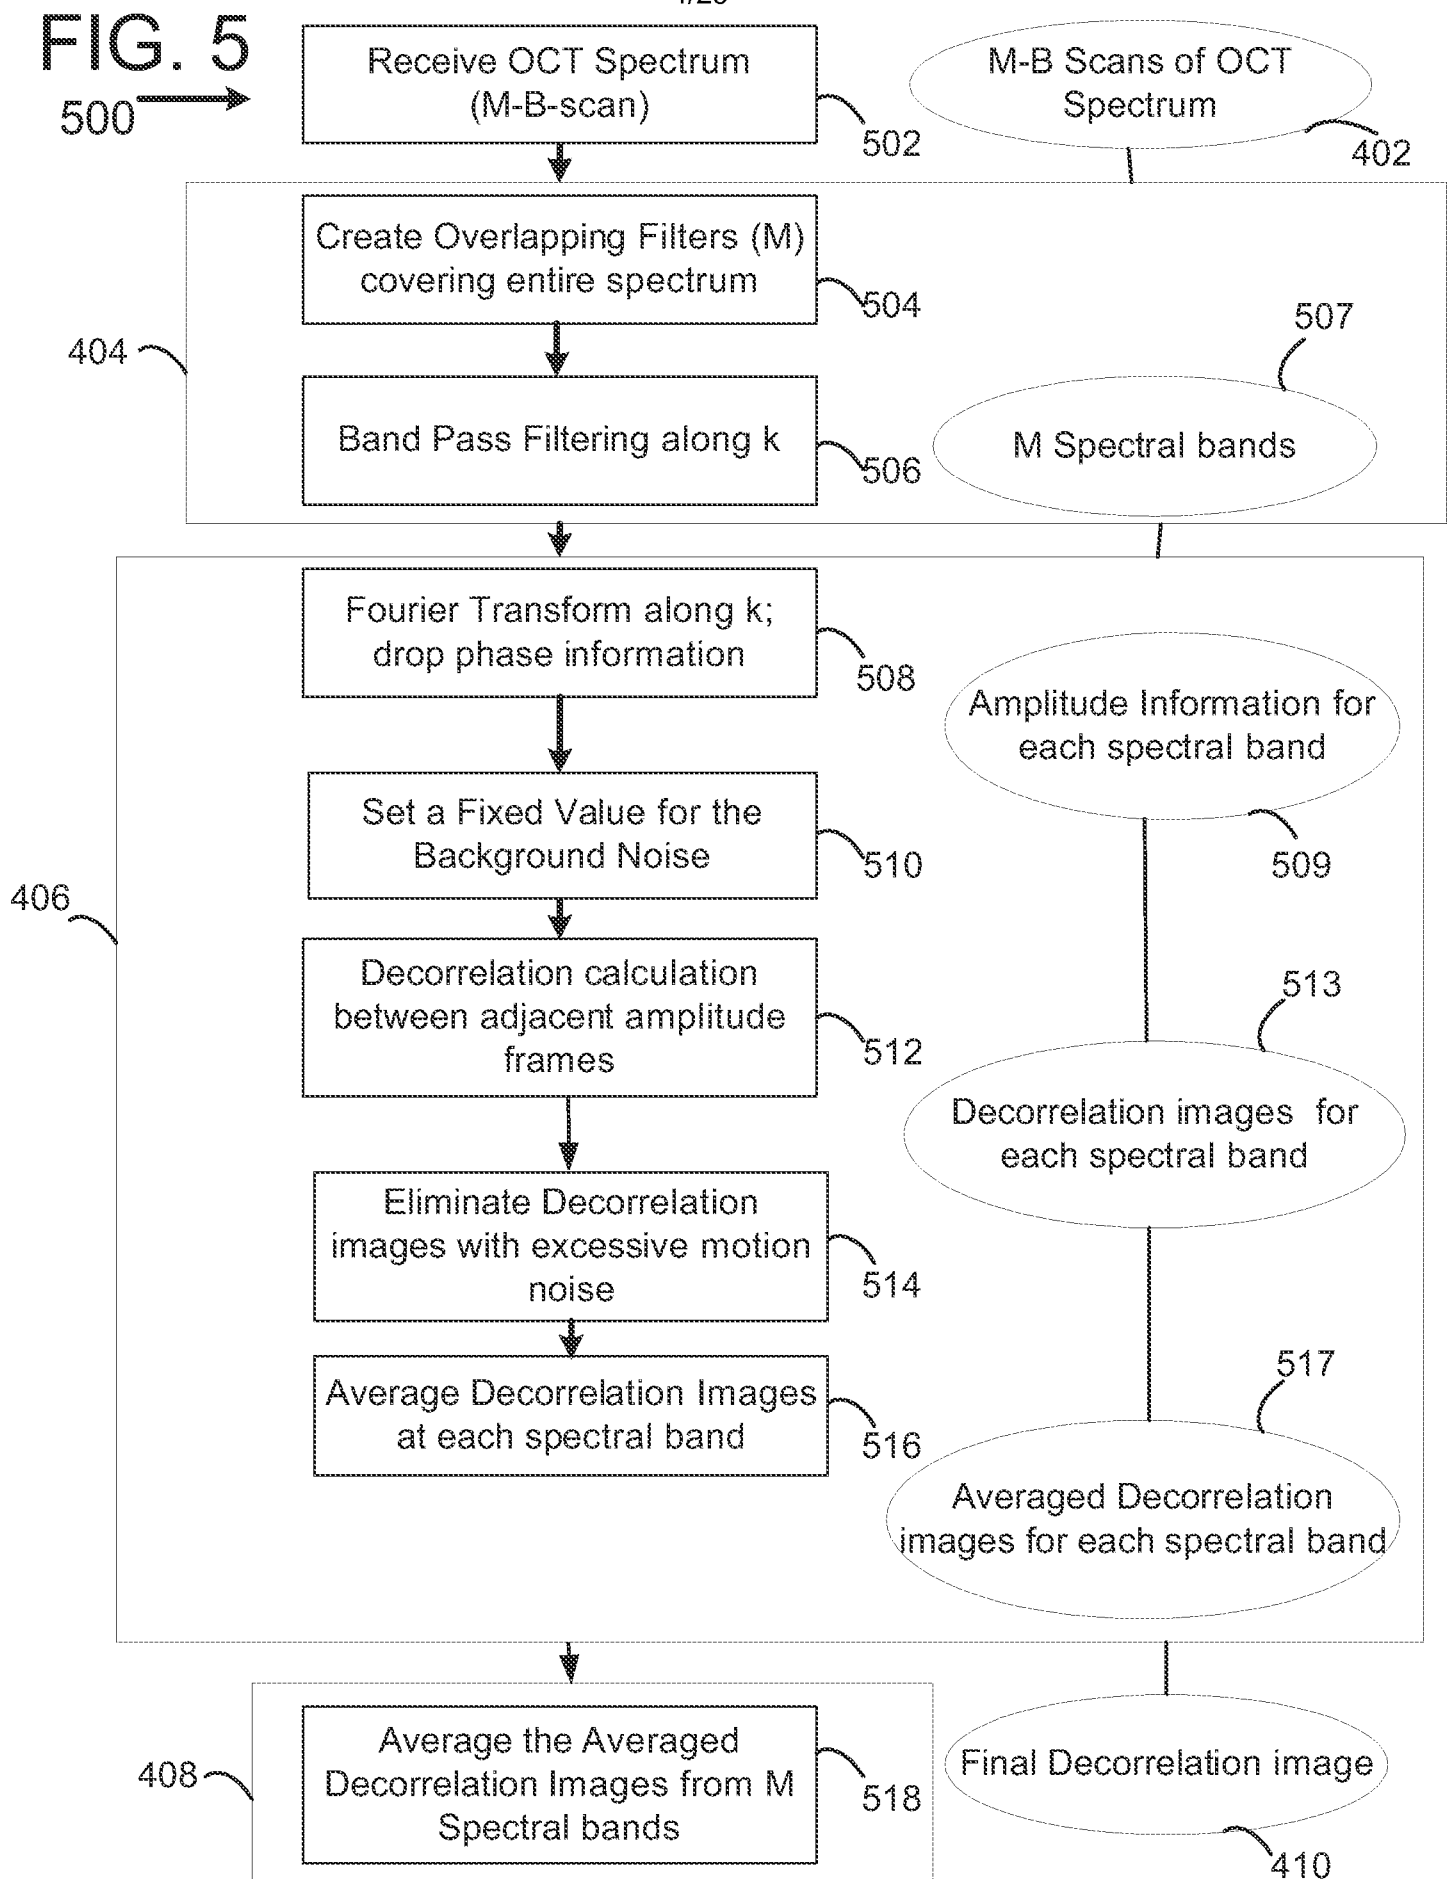

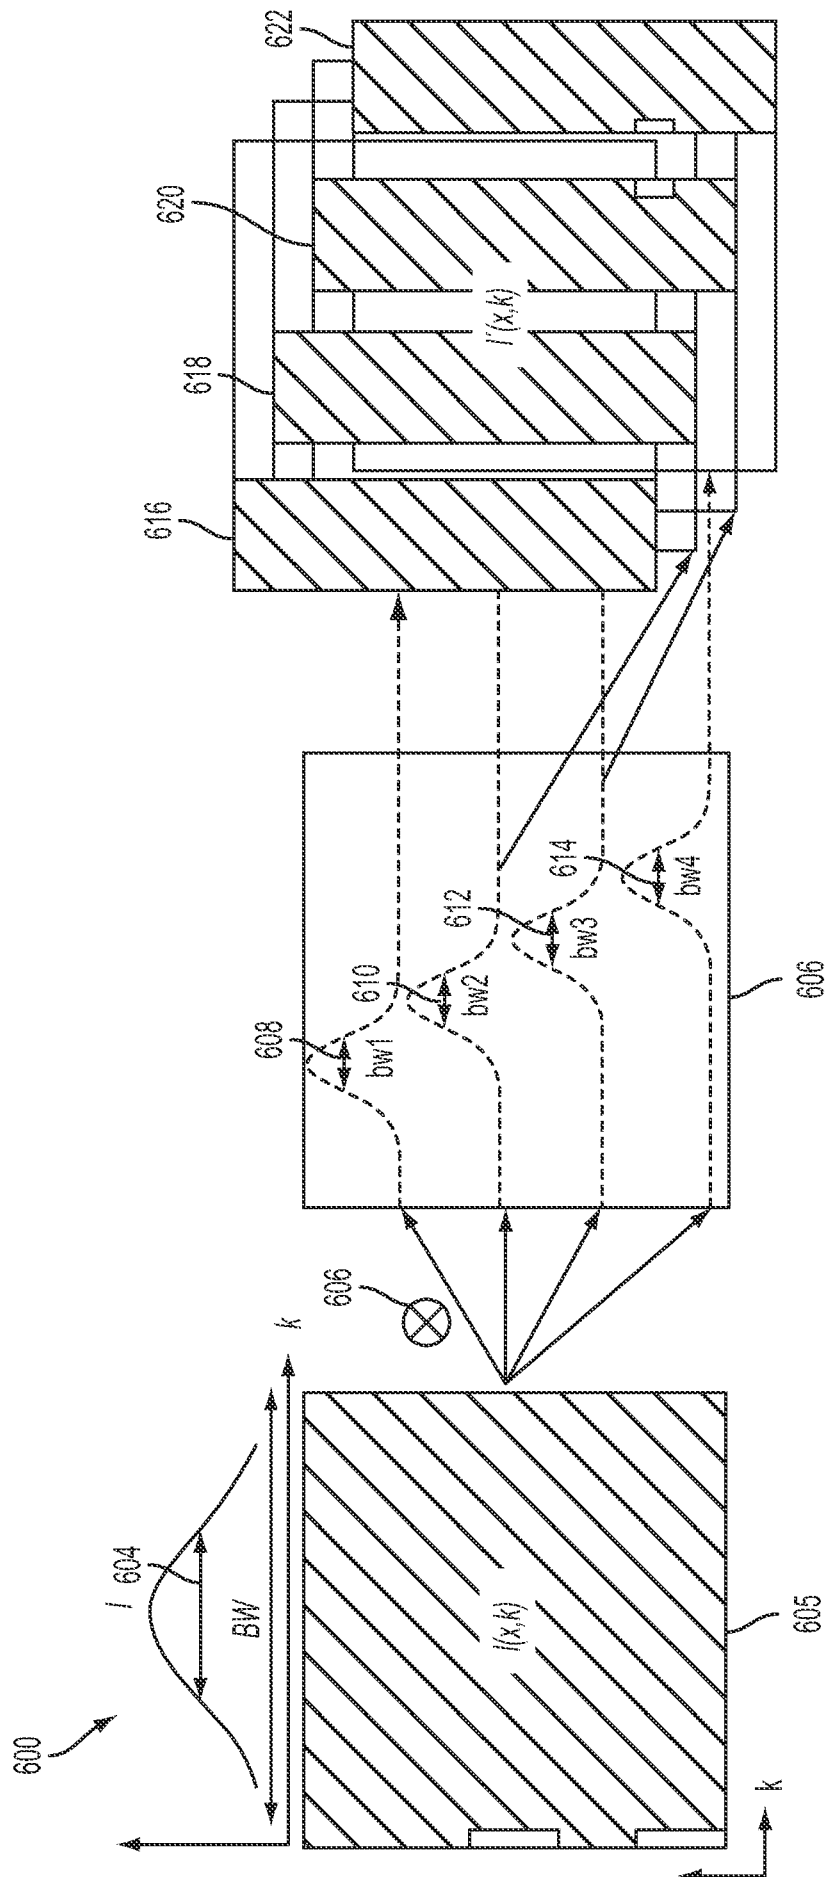


FIG. 6

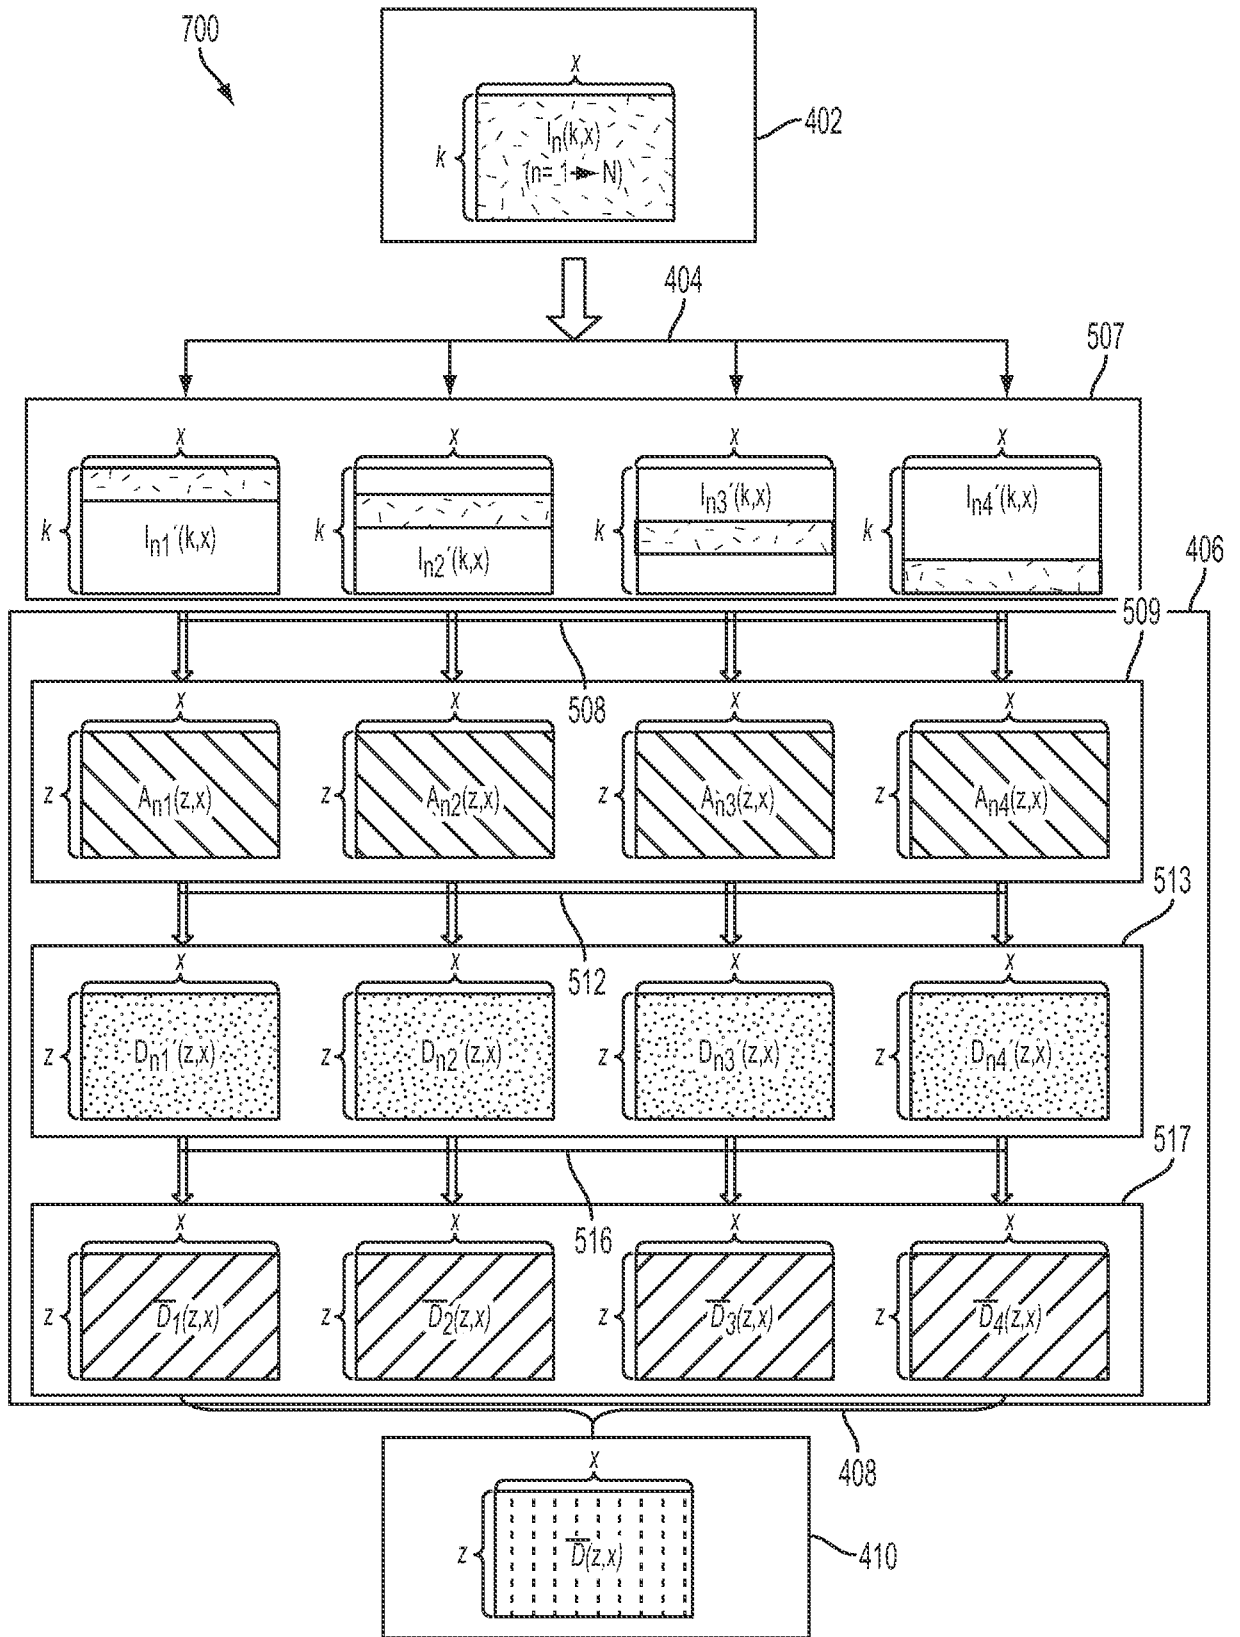


FIG. 7

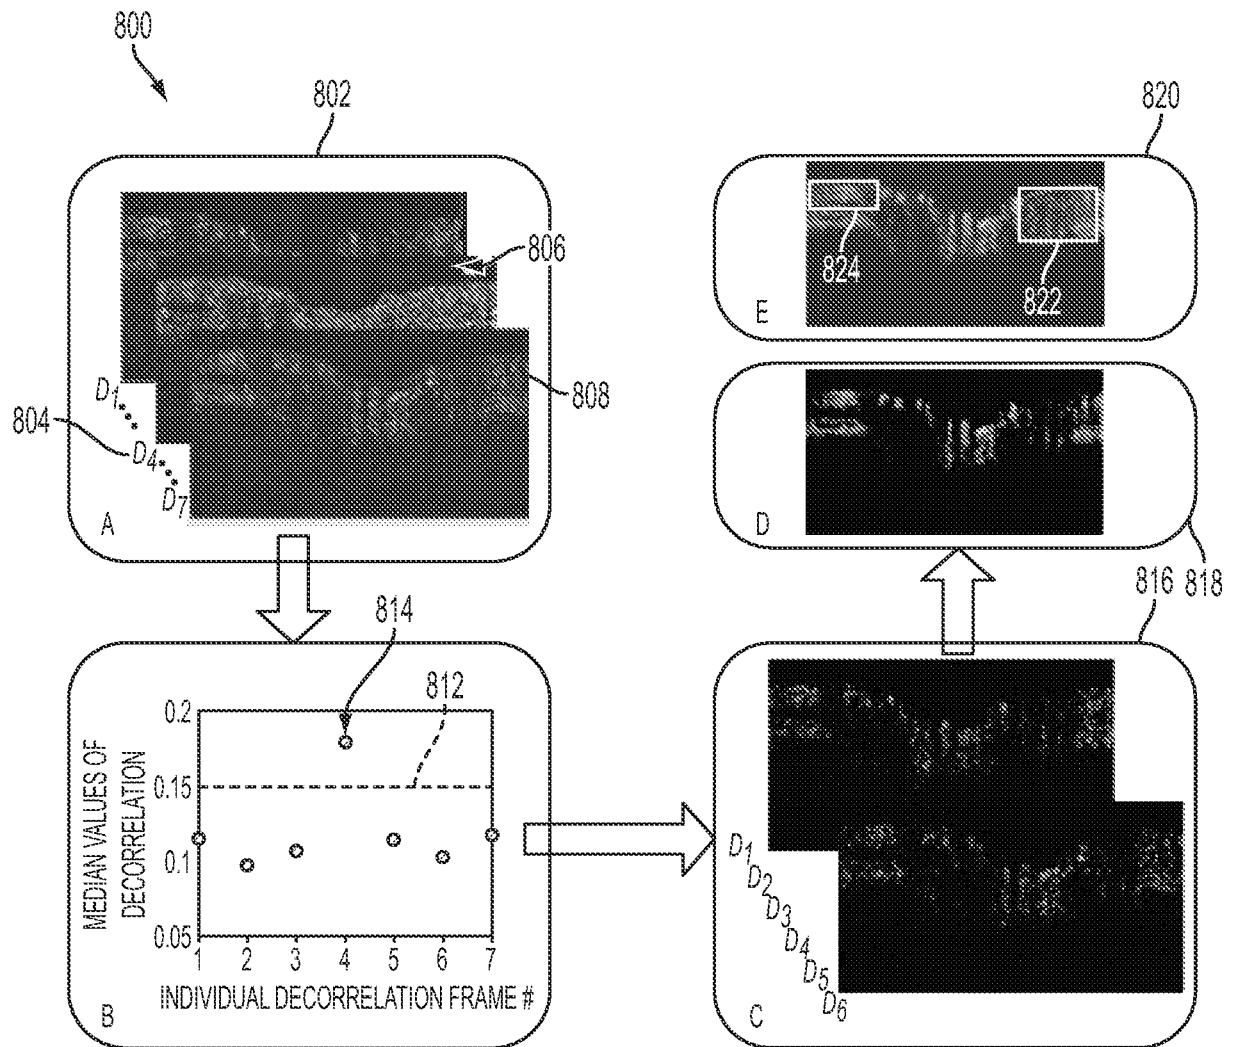


FIG. 8

FIG. 9

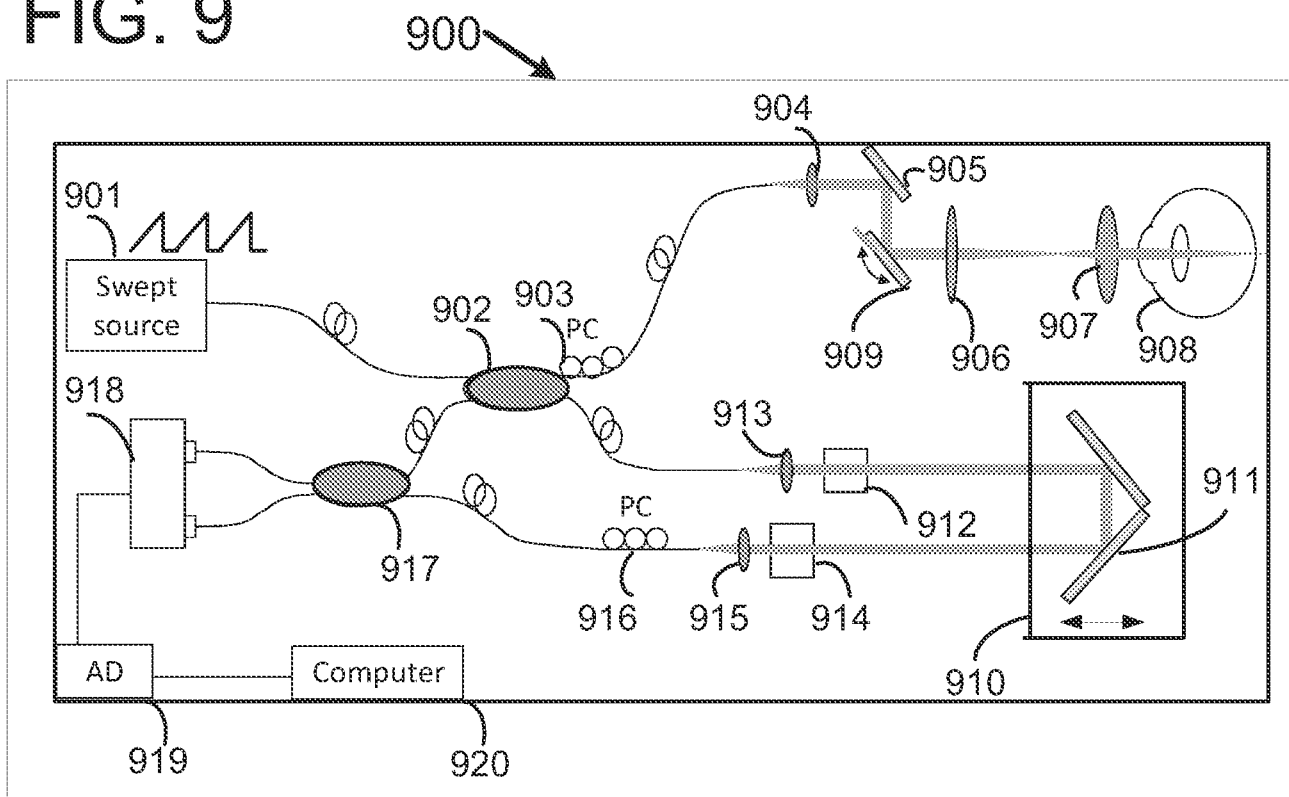


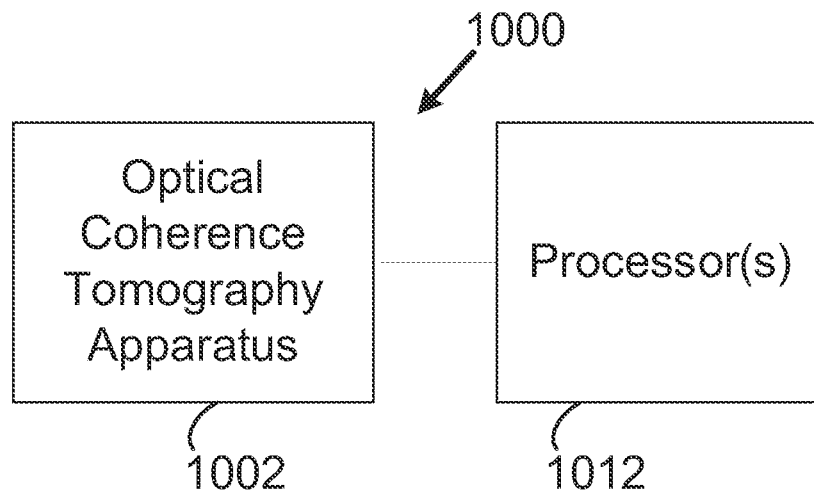
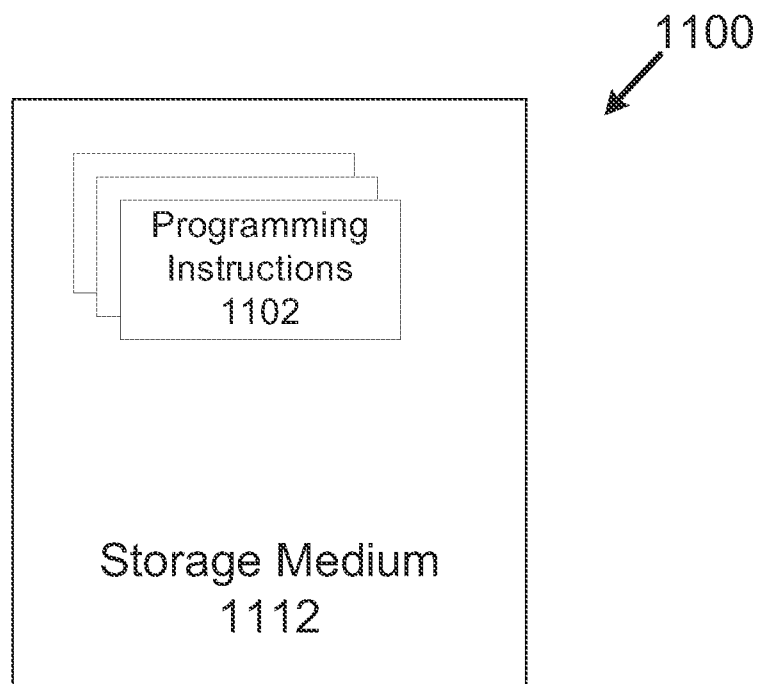
**FIG.
10****FIG.
11**

FIG. 12

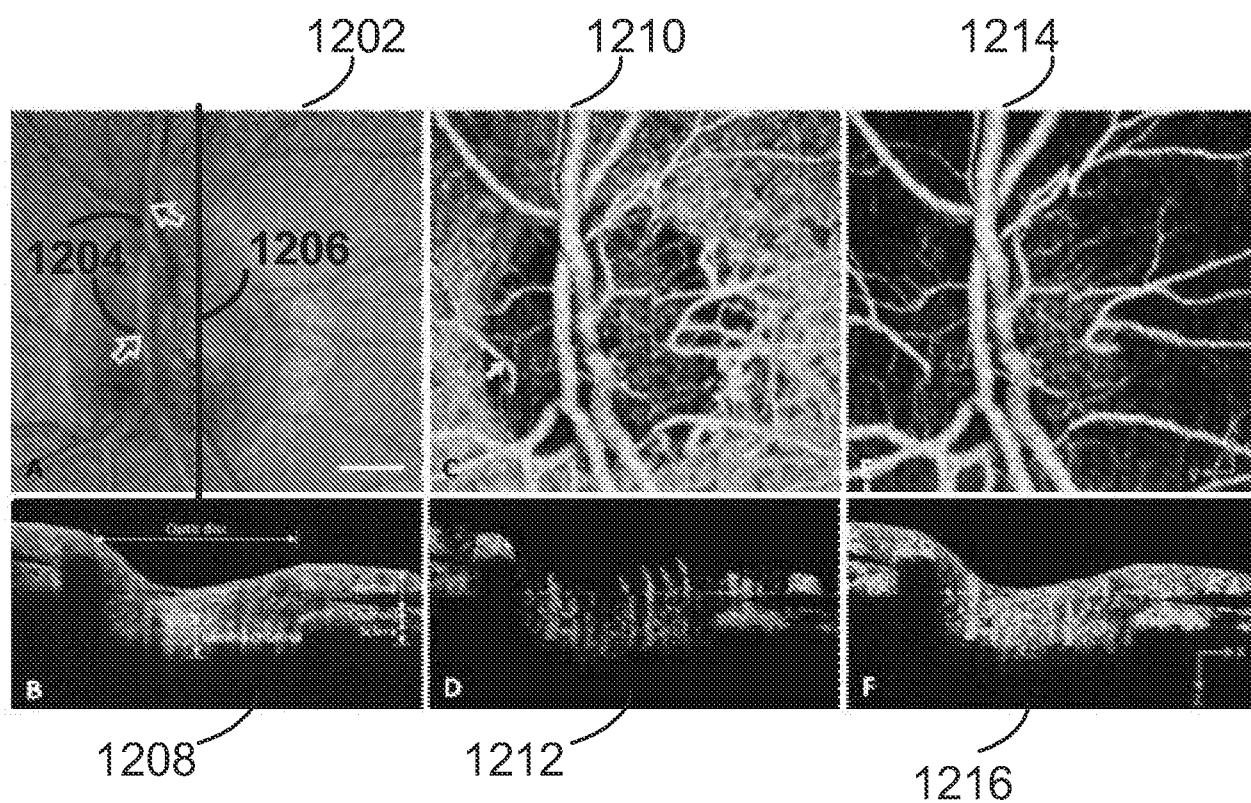


FIG. 13

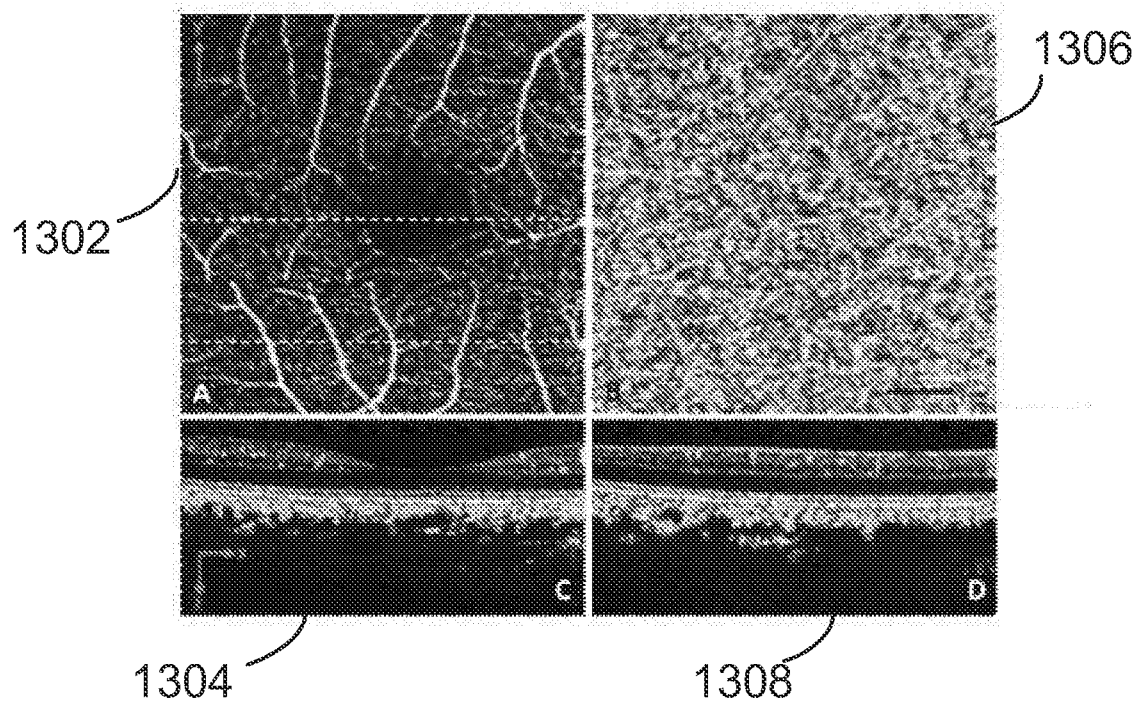


FIG. 14

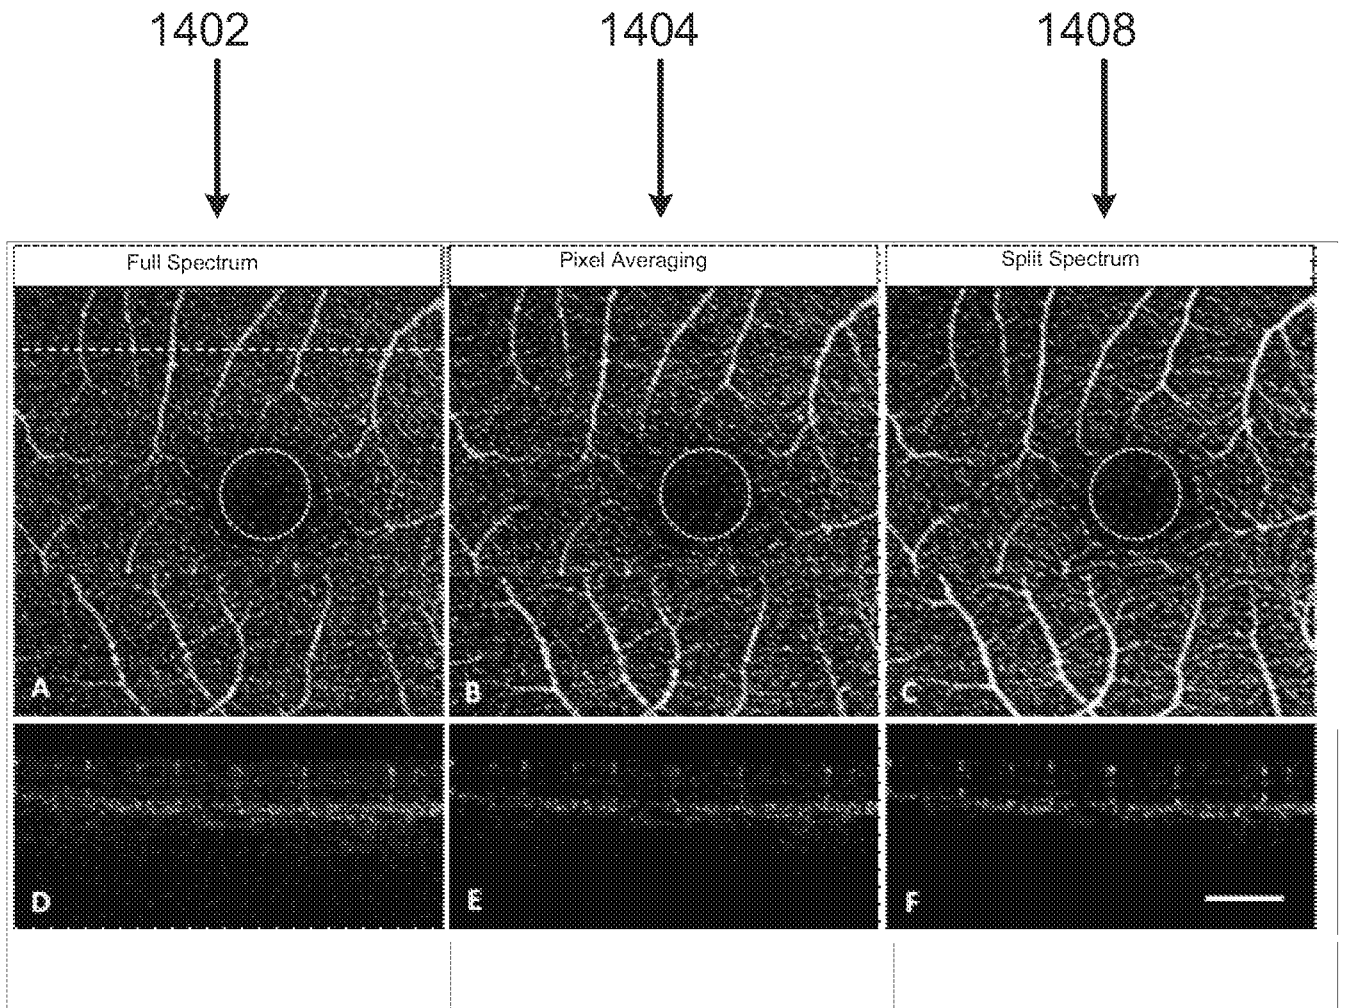


FIG. 15


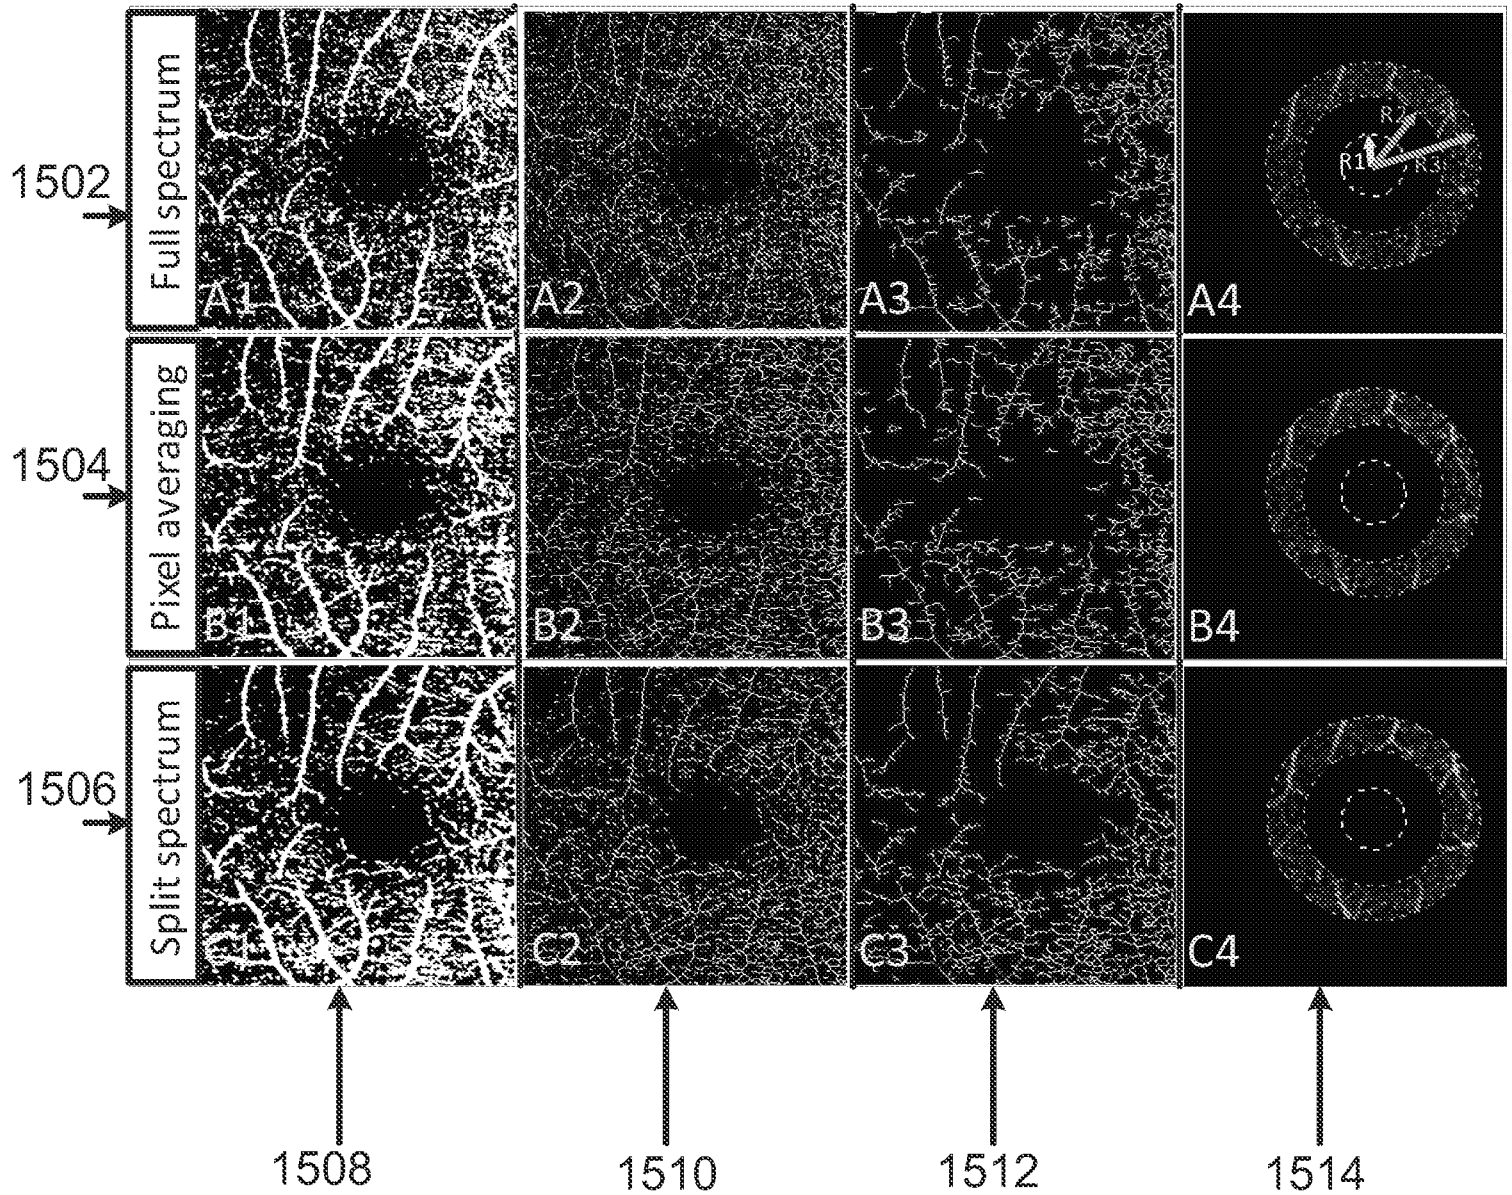


Figure 16

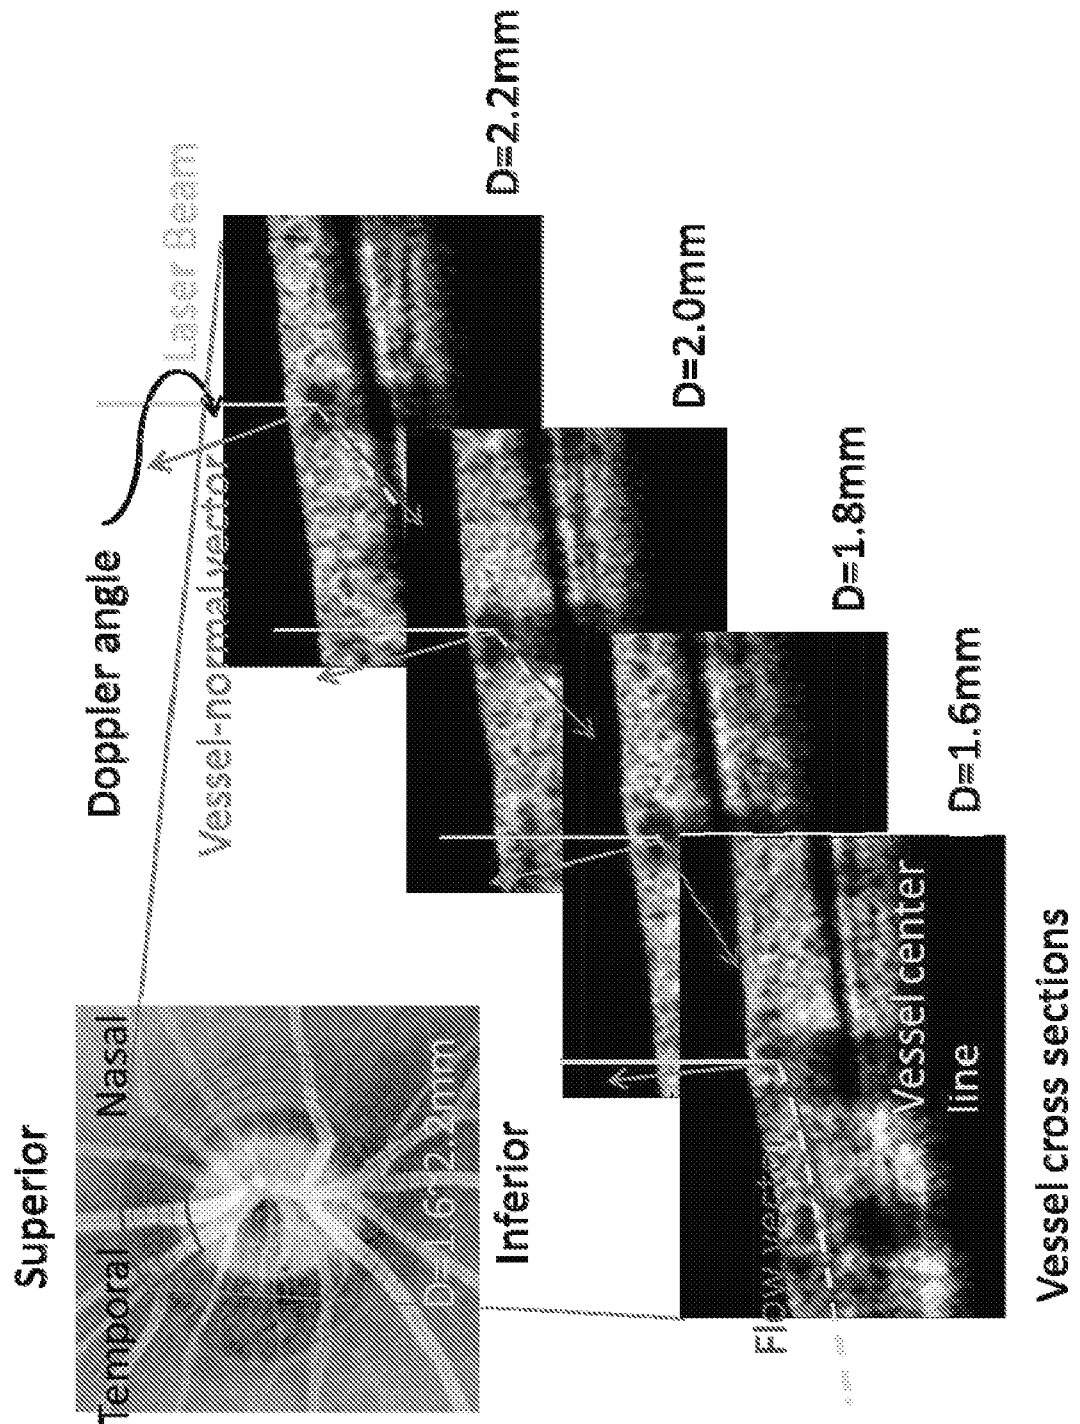

Figures 17 A-D

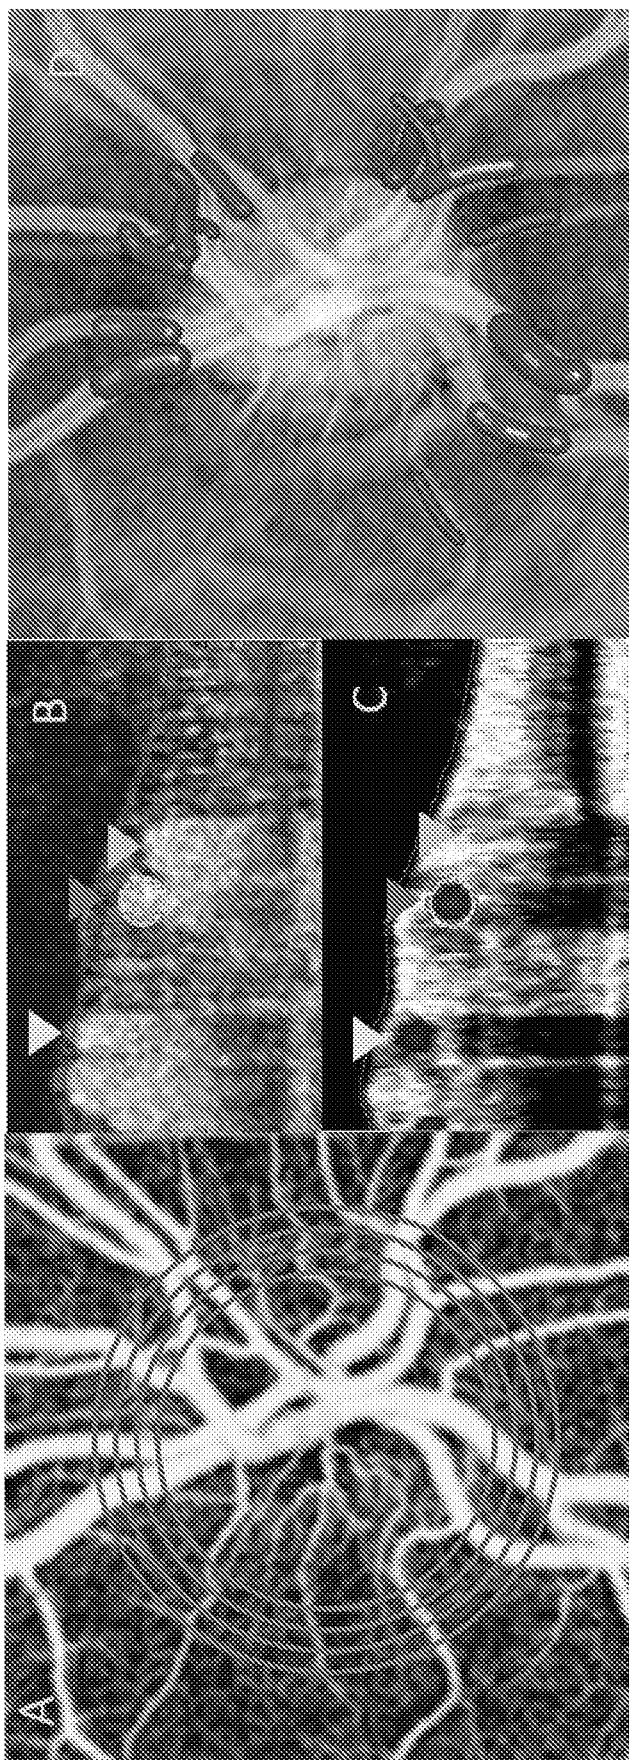


FIG. 18

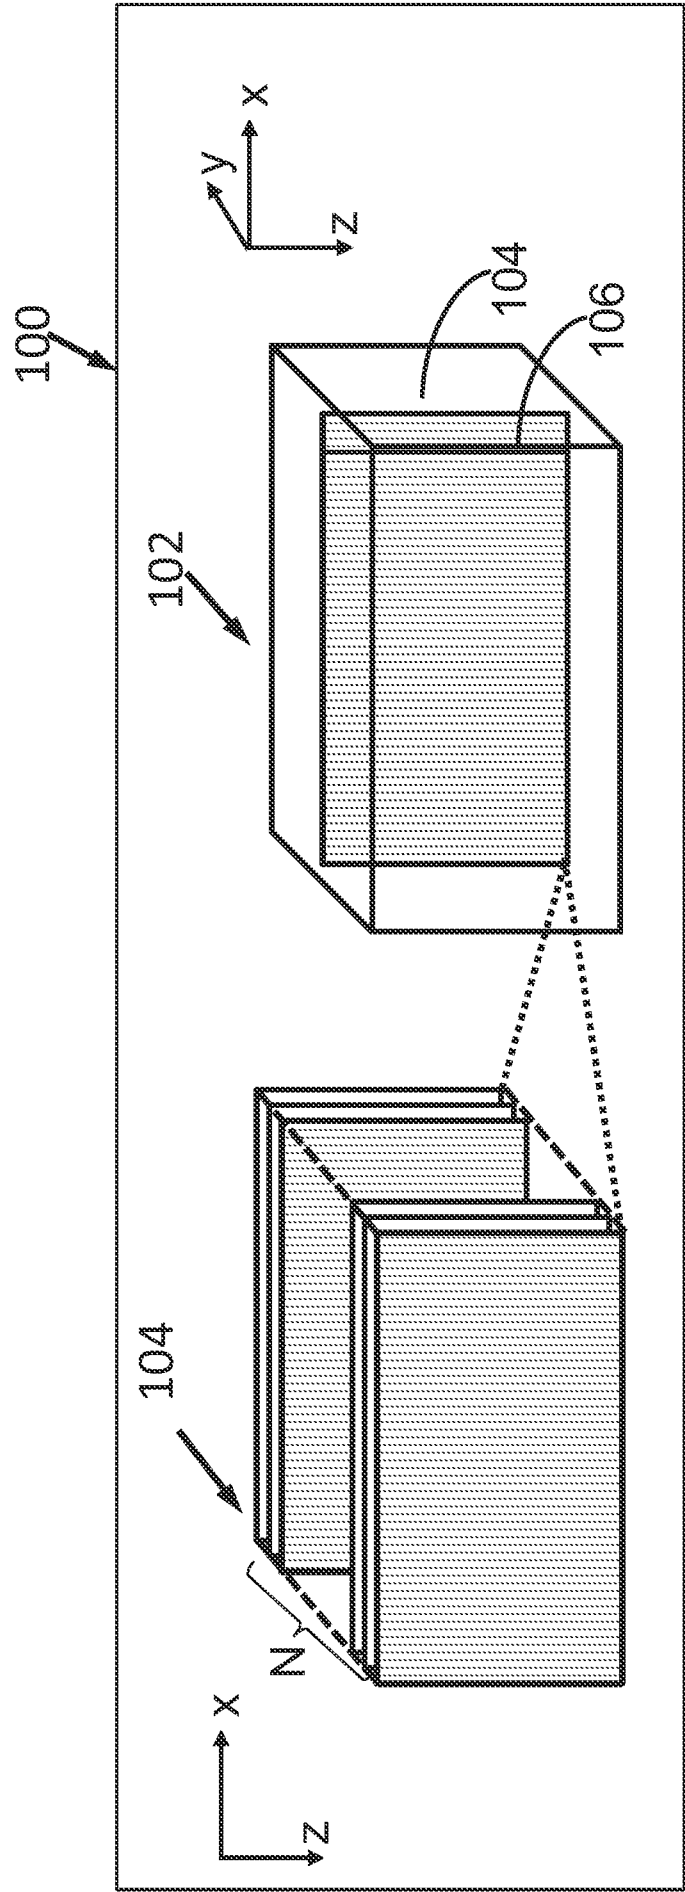


FIG. 19

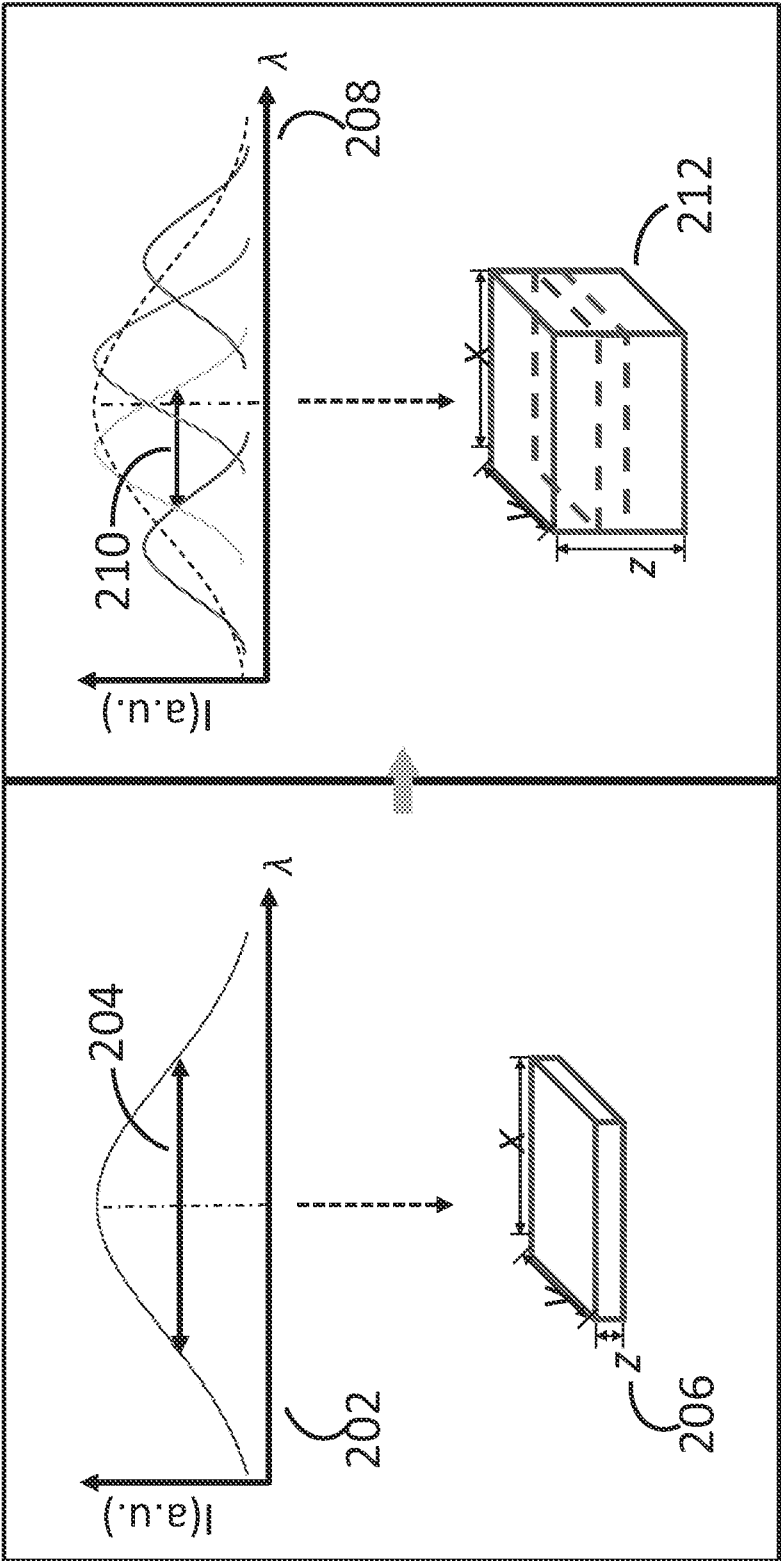


FIG. 20

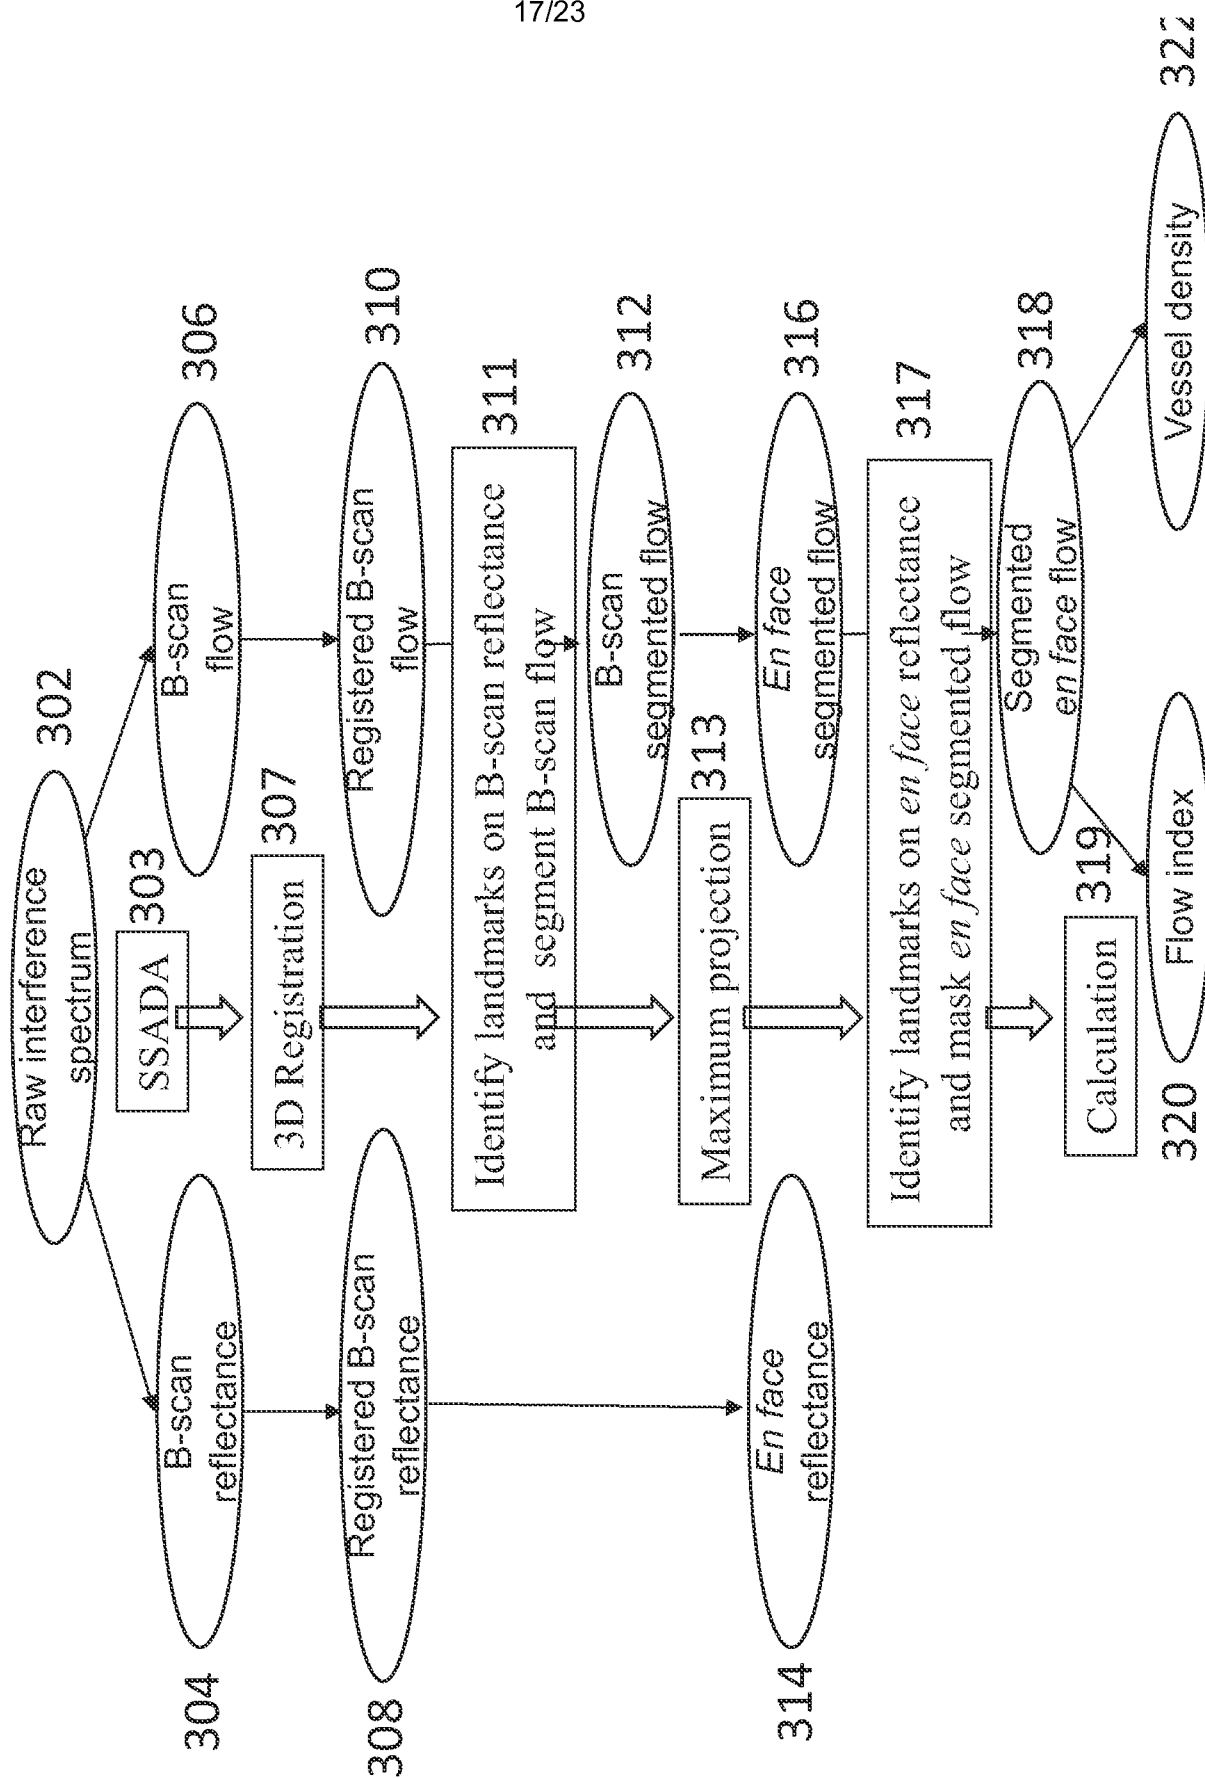


FIG. 21

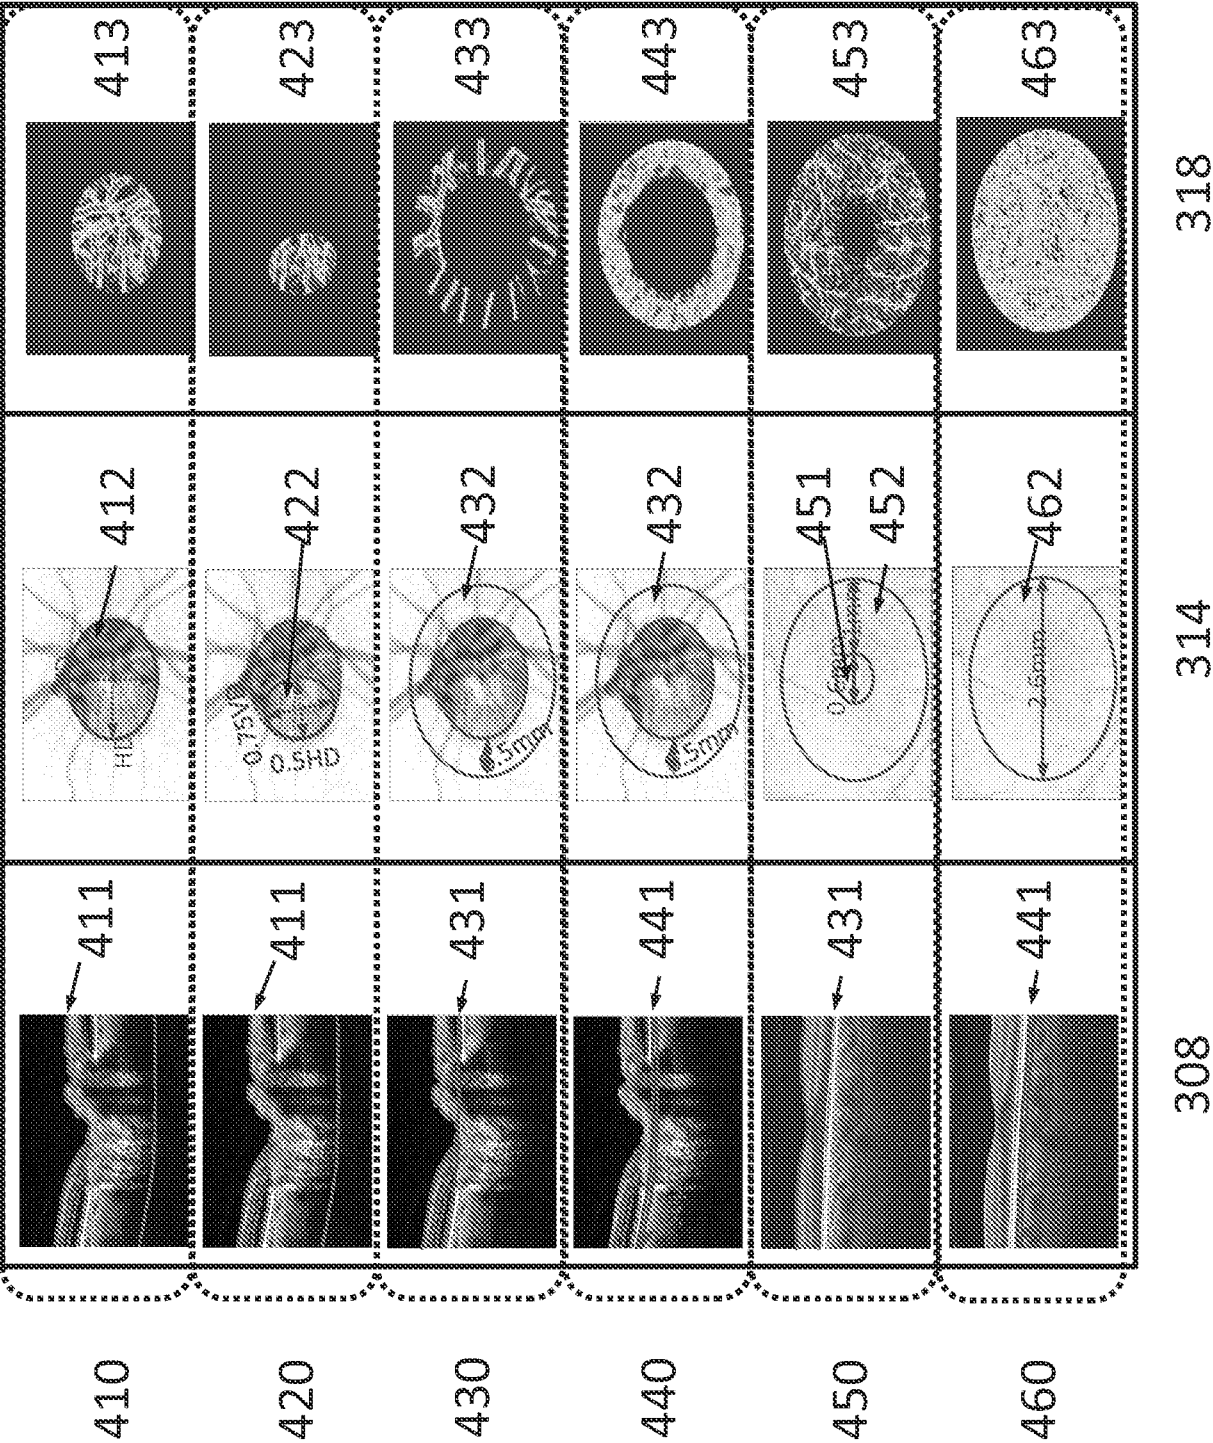


FIG. 22

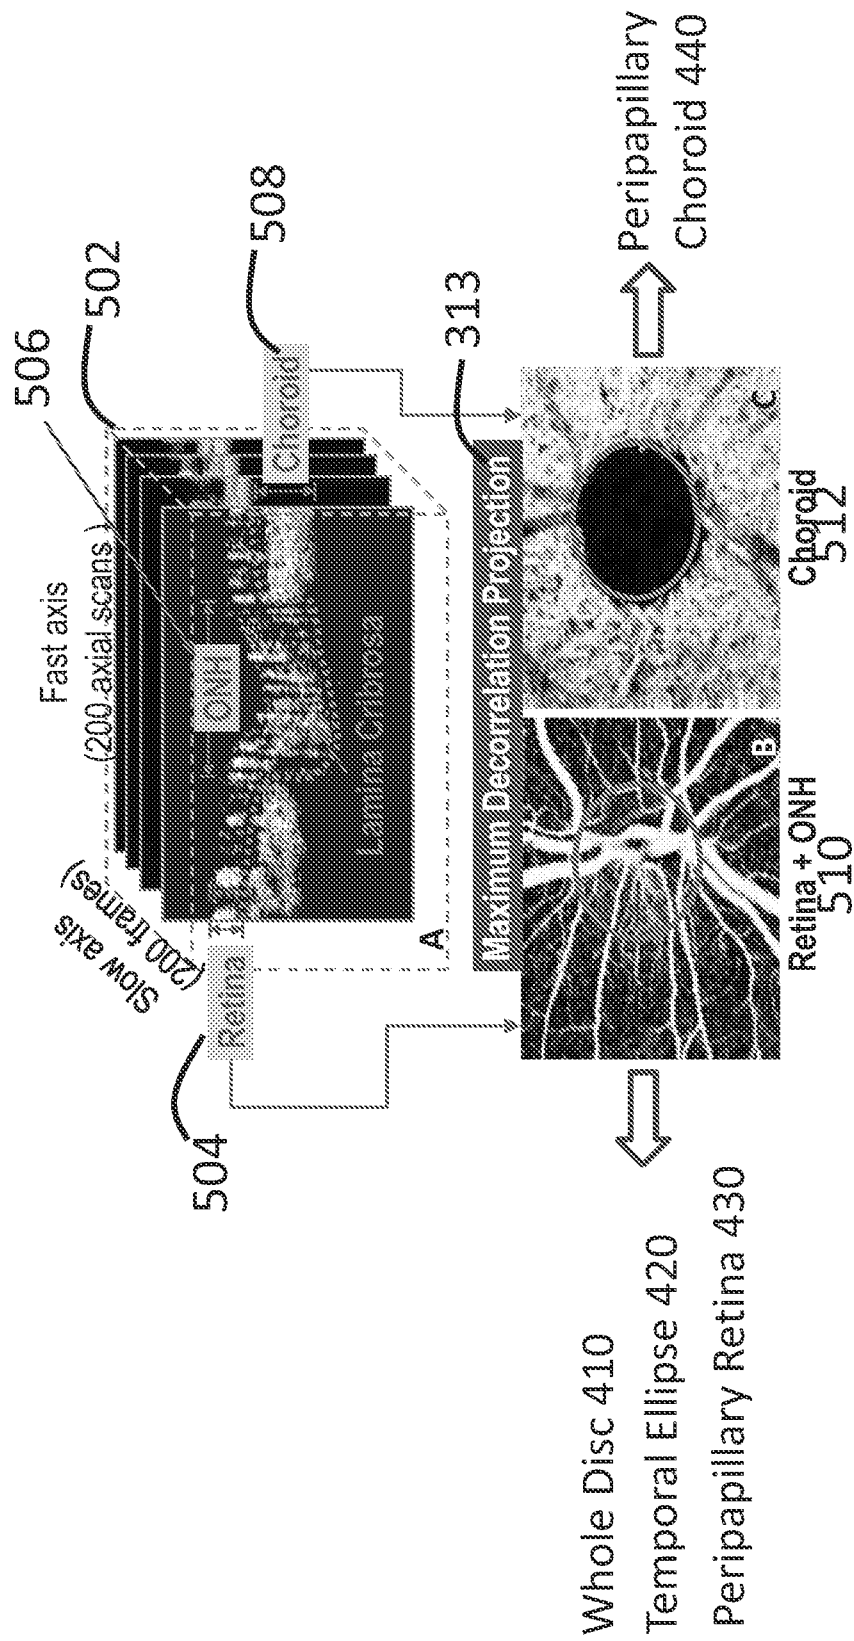


FIG. 23

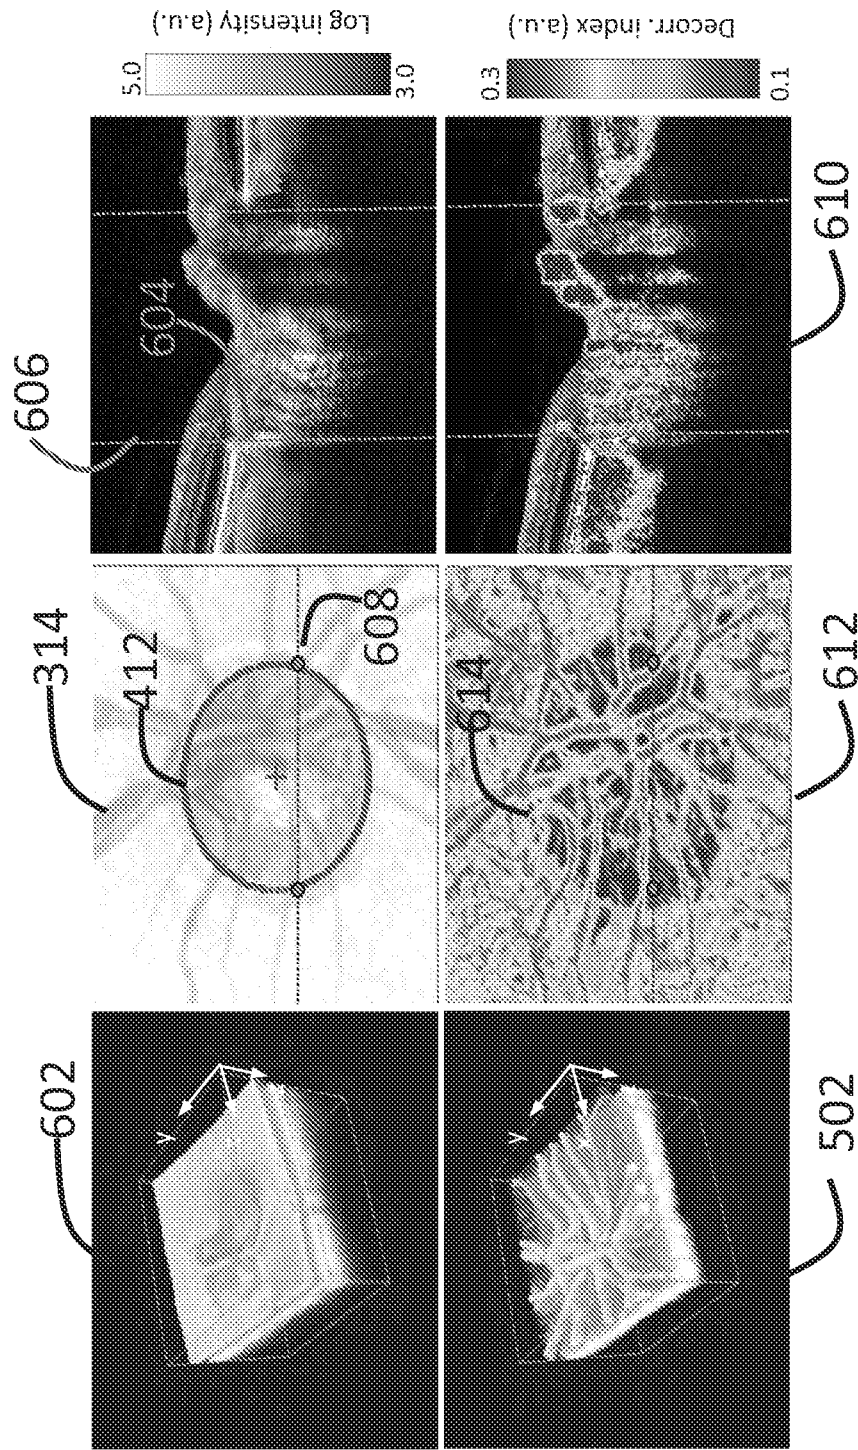


FIG. 24

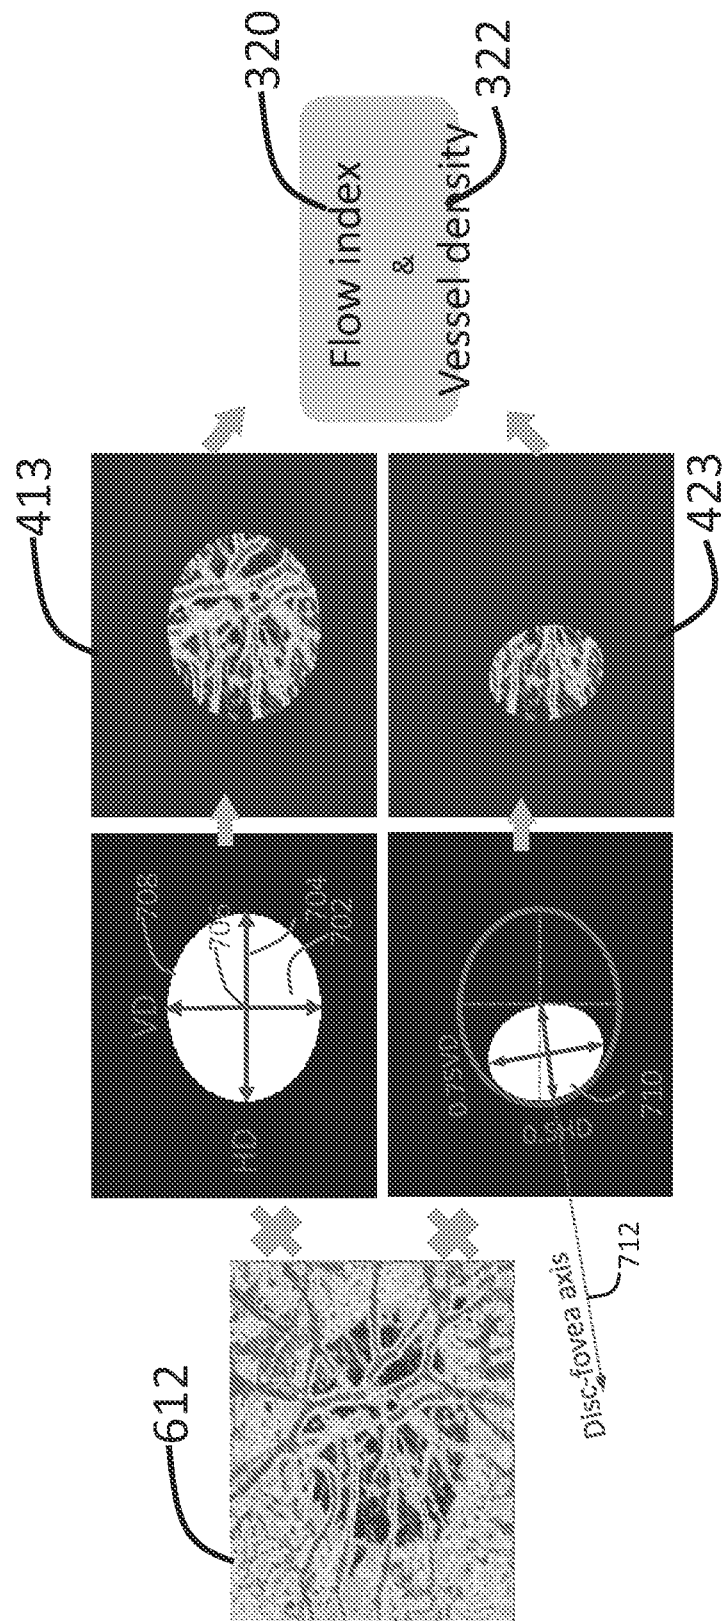


FIG. 25


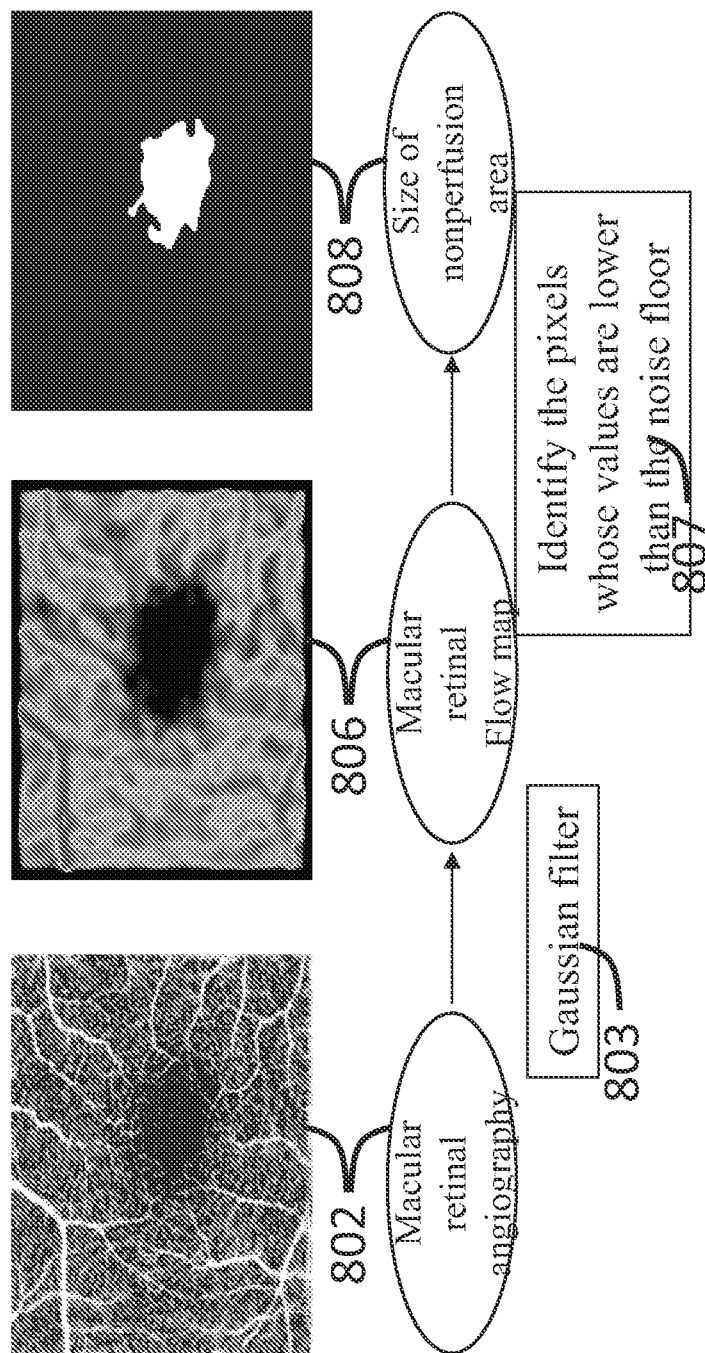


FIG. 26

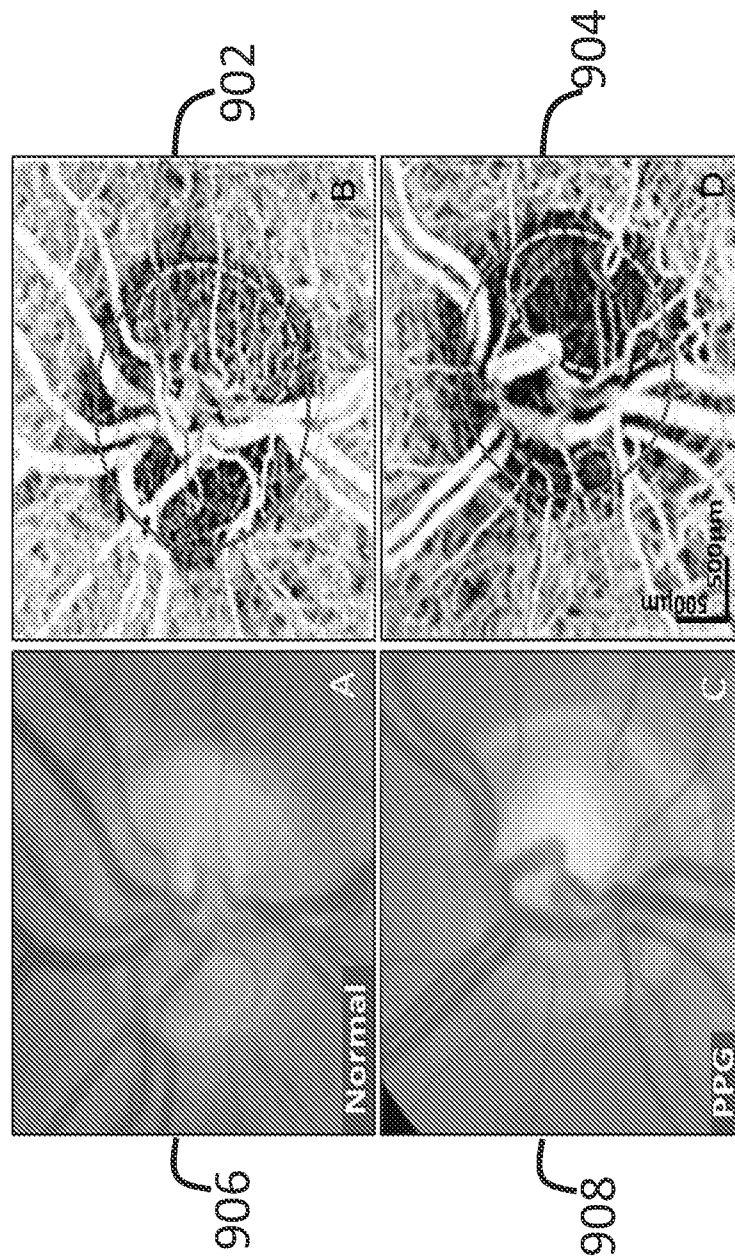

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US2013/059047**A. CLASSIFICATION OF SUBJECT MATTER****A61B 3/10(2006.01)i, G01B 9/02(2006.01)i**

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

A61B 3/10; A61B 5/05; A61B 3/12; G01B 11/02; G01N 21/00; G01B 9/02

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Korean utility models and applications for utility models

Japanese utility models and applications for utility models

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

eKOMPASS(KIPO internal) & Keywords: blood flow, ocular vascular bed, scan, OCT, spectrum, M-B scan, spectral band

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	US 2009-0149726 A1 (RODERICK A. HYDE et al.) 11 June 2009 See abstract, paragraphs [0012]-[0037],[0077] and figures 1,2.	1-9, 19-23
A	US 2008-0094613 A1 (JOHANNES F. DE BOER et al.) 08 November 2011 See abstract, paragraphs [0046]-[0065] and figures 1-6.	1-9, 19-23
A	US 2007-0291277 A1 (MATTHEW J. EVERETT et al.) 20 December 2007 See abstract, paragraphs [0047]-[0073] and figures 1-5.	1-9, 19-23
A	JP 2009-535164 A (PHYSICAL SCIENCES, INC.) 01 October 2009 See abstract, paragraphs [0030]-[0052] and figures 1-4.	1-9, 19-23
A	US 2007-0019208 A1 (MASAHIRO TOIDA et al.) 25 January 2007 See abstract, paragraphs [0029]-[0081],[0136]-[0173] and figures 1-12, 18-21.	1-9, 19-23



Further documents are listed in the continuation of Box C.



See patent family annex.

* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier application or patent but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&" document member of the same patent family

Date of the actual completion of the international search

07 January 2014 (07.01.2014)

Date of mailing of the international search report

08 January 2014 (08.01.2014)

Name and mailing address of the ISA/KR

Korean Intellectual Property Office
189 Cheongsa-ro, Seo-gu, Daejeon Metropolitan City,
302-701, Republic of Korea

Facsimile No. +82-42-472-7140

Authorized officer

KIM, Tae Hoon

Telephone No. +82-42-481-8407



INTERNATIONAL SEARCH REPORTInternational application No.
PCT/US2013/059047**Box No. II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)**

This international search report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☒ Claims Nos.: 10-18
because they relate to subject matter not required to be searched by this Authority, namely:
Claims 10-18 pertain to methods for treatment of the human body by therapy or surgery, as well as diagnostic methods, and thus relate to a subject matter which this International Searching Authority is not required to search under Article 17(2)(a)(i) of the PCT and Rule 39.1(iv) of the Regulations under the PCT.
2. ☐ Claims Nos.:
because they relate to parts of the international application that do not comply with the prescribed requirements to such an extent that no meaningful international search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box No. III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

1. ☐ As all required additional search fees were timely paid by the applicant, this international search report covers all searchable claims.
2. ☐ As all searchable claims could be searched without effort justifying an additional fees, this Authority did not invite payment of any additional fees.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this international search report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this international search report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest and, where applicable, the payment of a protest fee.
- ☐ The additional search fees were accompanied by the applicant's protest but the applicable protest fee was not paid within the time limit specified in the invitation.
- ☐ No protest accompanied the payment of additional search fees.

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/059047

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2009-0149726 A1	11/06/2009	CN 102753096 A	24/10/2012
		CN 102753887 A	24/10/2012
		CN 103167840 A	19/06/2013
		EP 2533695 A1	19/12/2012
		EP 2534415 A2	19/12/2012
		EP 2632380 A1	04/09/2013
		US 2010-0222662 A1	02/09/2010
		US 2010-0222774 A1	02/09/2010
		US 2010-0222775 A1	02/09/2010
		US 2010-0256437 A1	07/10/2010
		US 2010-0256467 A1	07/10/2010
		US 2011-0194176 A1	11/08/2011
		US 2011-0196221 A1	11/08/2011
		US 2011-0196222 A1	11/08/2011
		US 2011-0196239 A1	11/08/2011
		US 2011-0222059 A1	15/09/2011
		US 2012-296180 A1	22/11/2012
		US 8385997 B2	26/02/2013
		US 8388509 B2	05/03/2013
		US 8467842 B2	18/06/2013
		US 8504129 B2	06/08/2013
		US 8585567 B2	19/11/2013
		WO 2011-100065 A2	18/08/2011
		WO 2011-100065 A3	03/11/2011
		WO 2011-100066 A1	18/08/2011
		WO 2012-060862 A1	10/05/2012
US 2008-0094613 A1	24/04/2008	AU 2003-210669 A1	02/09/2003
		AU 2003-210669 A2	02/09/2003
		AU 2003-210669 B2	29/10/2009
		AU 2004-225188 A1	14/10/2004
		AU 2004-225188 B2	15/04/2010
		AU 2004-252482 A1	06/01/2005
		AU 2004-252482 B2	26/05/2011
		CA 2474331 A1	31/07/2003
		CA 2519937 A1	14/10/2004
		CA 2519937 C	20/11/2012
		CA 2527930 A1	06/01/2005
		CN 101793823 A	04/08/2010
		CN 103082996 A	08/05/2013
		CN 103181753 A	03/07/2013
		CN 103181754 A	03/07/2013
		CN 1623085 C0	01/06/2005
		CN 1875242 A	06/12/2006
		CN 1875242 C0	06/12/2006
		EP 1470410 A2	27/10/2004
		EP 1470410 B1	11/01/2012
		EP 1611470 A2	04/01/2006
		EP 1639330 A2	29/03/2006

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/059047

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		EP 1639330 B1	08/10/2008
		EP 1685366 A1	02/08/2006
		EP 1685366 B1	15/06/2011
		EP 2008579 A2	31/12/2008
		EP 2008579 A3	25/03/2009
		EP 2011434 A2	07/01/2009
		EP 2011434 A3	25/03/2009
		EP 2030562 A2	04/03/2009
		EP 2030562 A3	25/03/2009
		EP 2030563 A2	04/03/2009
		EP 2030563 A3	25/03/2009
		EP 2270447 A1	05/01/2011
		EP 2270448 A1	05/01/2011
		EP 2278287 A1	26/01/2011
		EP 2280256 A1	02/02/2011
		EP 2280257 A1	02/02/2011
		EP 2280258 A2	02/02/2011
		EP 2280259 A1	02/02/2011
		EP 2280260 A2	02/02/2011
		EP 2280260 A3	28/11/2012
		EP 2290336 A2	02/03/2011
		EP 2290336 A3	09/10/2013
		EP 2290337 A2	02/03/2011
		EP 2290338 A2	02/03/2011
		EP 2290338 A3	28/11/2012
		EP 2290339 A2	02/03/2011
		EP 2290339 A3	28/11/2012
		EP 2293031 A2	09/03/2011
		EP 2436307 A1	04/04/2012
		JP 2005-516187 A	02/06/2005
		JP 2006-522341 A	28/09/2006
		JP 2007-510143 A	19/04/2007
		JP 2007-526620 A	13/09/2007
		JP 2011-209293 A	20/10/2011
		JP 2011-215162 A	27/10/2011
		JP 2011-215163 A	27/10/2011
		JP 2011-215164 A	27/10/2011
		JP 2011-215165 A	27/10/2011
		JP 2011-221043 A	04/11/2011
		JP 2012-015532 A	19/01/2012
		JP 4805142 B2	02/11/2011
		KR 10-1130739 B1	29/03/2012
		KR 10-1204370 B1	23/11/2012
		KR 10-1321413 B1	22/10/2013
		KR 10-2006-0028684 A	31/03/2006
		KR 10-2012-0106905 A	26/09/2012
		KR 10-2013-0029816 A	25/03/2013
		TW 201237457 A	16/09/2012
		TW I346428 I	01/08/2011
		US 2002-0198457 A1	26/12/2002

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/059047

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
		US 2005-0018201 A1	27/01/2005
		US 2005-0035295 A1	17/02/2005
		US 2006-0227333 A1	12/10/2006
		US 2006-0244973 A1	02/11/2006
		US 2008-0094637 A1	24/04/2008
		US 2008-0097709 A1	24/04/2008
		US 2008-0100837 A1	01/05/2008
		US 2008-0152353 A1	26/06/2008
		US 2008-0170225 A1	17/07/2008
		US 2008-0181263 A1	31/07/2008
		US 2009-0027689 A1	29/01/2009
		US 2009-0257461 A1	15/10/2009
		US 2010-0094576 A1	15/04/2010
		US 2010-0157309 A1	24/06/2010
		US 2010-0254414 A1	07/10/2010
		US 2012-0281237 A1	08/11/2012
		US 7355716 B2	08/04/2008
		US 7519096 B2	14/04/2009
		US 7567349 B2	28/07/2009
		US 7630083 B2	08/12/2009
		US 7643152 B2	05/01/2010
		US 7643153 B2	05/01/2010
		US 7724786 B2	25/05/2010
		US 7733497 B2	08/06/2010
		US 7797119 B2	14/09/2010
		US 7864822 B2	04/01/2011
		US 7872757 B2	18/01/2011
		US 7903257 B2	08/03/2011
		US 7969578 B2	28/06/2011
		US 7995627 B2	09/08/2011
		US 8054468 B2	08/11/2011
		US 8174702 B2	08/05/2012
		US 8559012 B2	15/10/2013
		WO 03-062802 A2	31/07/2003
		WO 03-062802 A3	04/12/2003
		WO 2004-088361 A2	14/10/2004
		WO 2004-088361 A3	07/04/2005
		WO 2005-001401 A2	06/01/2005
		WO 2005-001401 A3	28/04/2005
		WO 2005-047813 A1	26/05/2005
US 2007-0291277 A1	20/12/2007	US 2007-0216909 A1	20/09/2007
		US 2010-0278402 A1	04/11/2010
		US 2011-0007321 A1	13/01/2011
		US 2012-140238 A1	07/06/2012
		US 7768652 B2	03/08/2010
		US 8045176 B2	25/10/2011
		US 8085408 B2	27/12/2011
		US 8427654 B2	23/04/2013

INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No.

PCT/US2013/059047

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
JP 2009-535164 A	01/10/2009	CA 2649065 A1	15/11/2007
		EP 2012653 A2	14/01/2009
		EP 2012653 B1	12/12/2012
		EP 2345363 A1	20/07/2011
		JP 5128583 B2	23/01/2013
		US 2007-0263171 A1	15/11/2007
		US 2010-0073634 A1	25/03/2010
		US 2011-0085136 A1	14/04/2011
		US 2012-062843 A1	15/03/2012
		US 7648242 B2	19/01/2010
		US 7866821 B2	11/01/2011
		US 8033665 B2	11/10/2011
		WO 2007-130411 A2	15/11/2007
		WO 2007-130411 A3	10/07/2008
US 2007-0019208 A1	25/01/2007	EP 1669739 A1	14/06/2006
		EP 1669739 B1	11/02/2009
		EP 1704814 A2	27/09/2006
		EP 1704814 A3	13/12/2006
		EP 1704814 B1	29/10/2008
		EP 1705476 A1	27/09/2006
		JP 2006-189424 A	20/07/2006
		JP 2007-327909 A	20/12/2007
		JP 4818823 B2	16/11/2011
		US 2006-0132791 A1	22/06/2006
		US 2006-0215170 A1	28/09/2006
		US 2006-0256348 A1	16/11/2006
		US 2007-0238527 A1	11/10/2007
		US 7450242 B2	11/11/2008

摘要

於人眼內血管床中的眼內血流量受損與某些眼部疾病有關，包括例如，青光眼，糖尿病視網膜病變和老年黃斑退化。一個可靠的方法來量化在各眼內血管床中的血流可以提供眼部疾病病理生理學血管成分的洞察。使用超高速光學相干斷層掃描（OCT），一個全新的 3D 血管造影的算法稱為分譜振幅解相關血管造影（SSADA）被開發以對不同的眼內區域內的微循環。一個量化 SSADA 結果的方法被開發和用於檢測早期眼部疾病血流灌注的變化。在本文中描述的相關實施方案與定量測定不同眼血管位置血流量的方法，用於實施這樣的方法的系統以及使用這樣的方法和系統以用於診斷某些眼病有關。