US 20150250417A1

(19) **United States**

(12) **Patent Application Publication**

CHENG et al.

(10) **Pub. No.: US 2015/0250417 A1**

(43) **Pub. Date: Sep. 10, 2015**

(54) **STAMINA MONITORING METHOD AND DEVICE**

(71) Applicant: **bOMDIC INC.**, Taipei (TW)

(72) Inventors: **SHIH-HENG CHENG**, Taipei (TW); **HSIN-FU KUO**, Taipei (TW)

(21) Appl. No.: **14/718,104**

(22) Filed: **May 21, 2015**

Related U.S. Application Data

(63) Continuation-in-part of application No. 14/460,339, filed on Aug. 14, 2014.

(60) Provisional application No. 61/867,229, filed on Aug. 19, 2013.

Publication Classification

(51) **Int. Cl.**

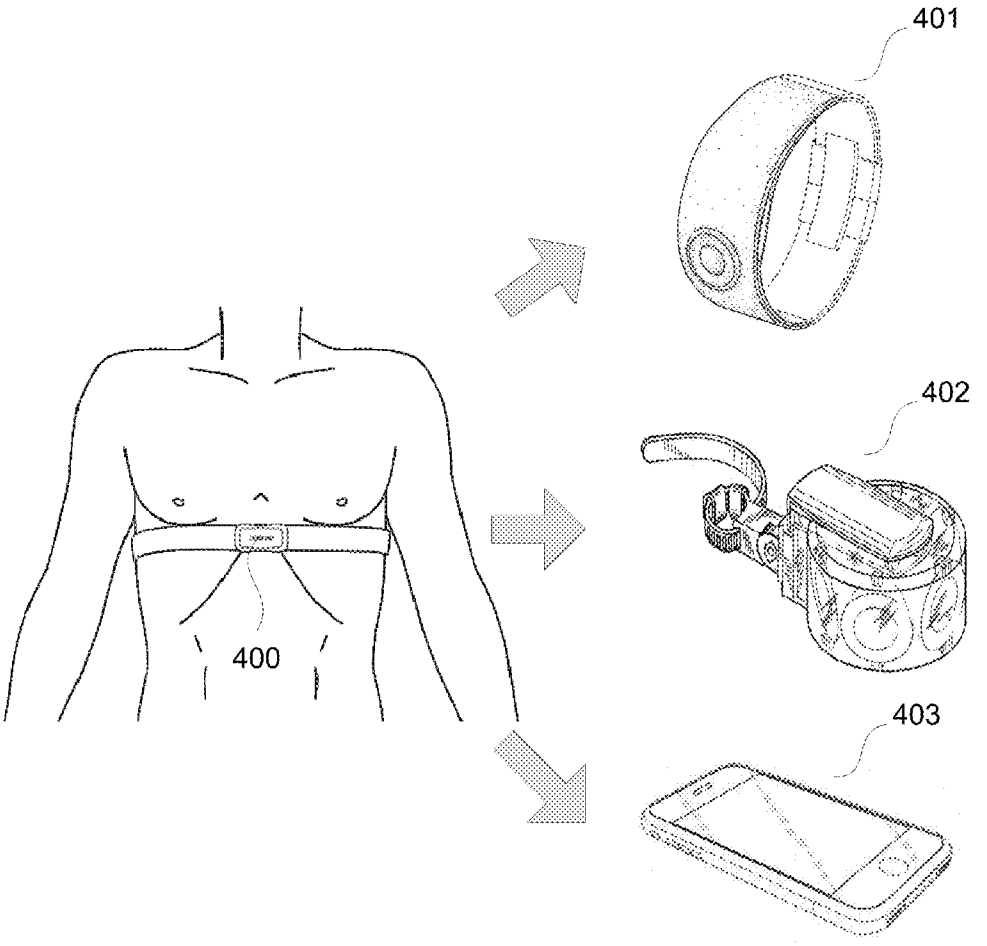
A61B 5/00	(2006.01)
A61B 5/11	(2006.01)
A61B 5/145	(2006.01)
A61B 5/0205	(2006.01)
A61B 5/0402	(2006.01)

(52) **U.S. Cl.**

CPC ***A61B 5/4866*** (2013.01); ***A61B 5/02055*** (2013.01); ***A61B 5/0402*** (2013.01); ***A61B 5/14542*** (2013.01); ***A61B 5/14546*** (2013.01); ***A61B 5/1118*** (2013.01); ***A61B 5/7278*** (2013.01); ***A61B 5/742*** (2013.01); ***A61B 5/7455*** (2013.01); ***A61B 5/7405*** (2013.01); *A61B 5/021* (2013.01)

(57) **ABSTRACT**

The present disclosure provides an exercise assistive device. The present disclosure also provides a method for estimating stamina level and a method for adjusting the method according to a user's anaerobic energy level and aerobic energy level. The present disclosure further provides the several types and applications of the exercise assistive device.



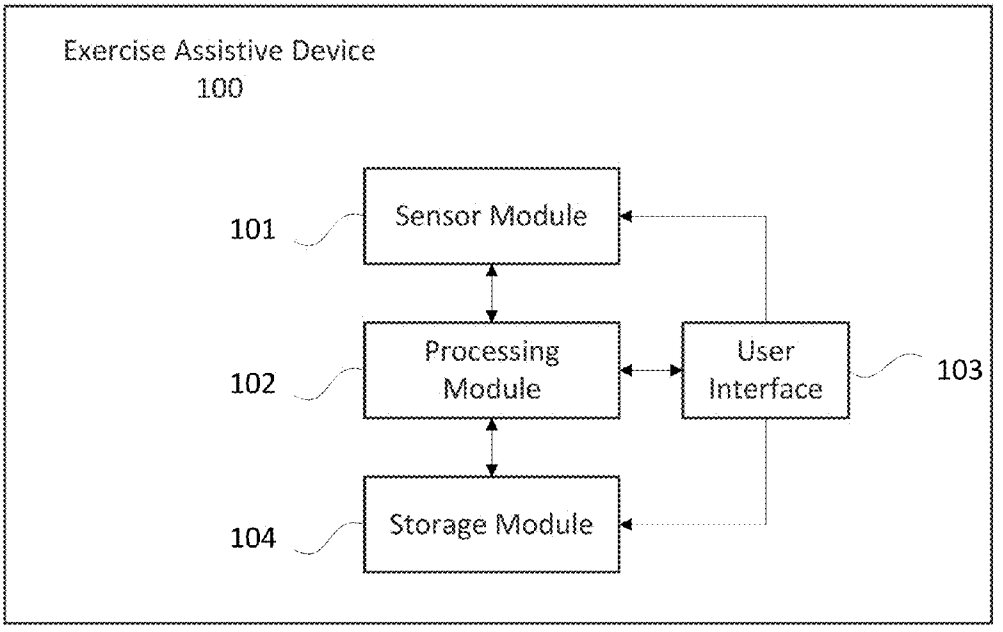

Exercise Assistive Device
100
101
Sensor Module
102
Processing Module
User Interface
103
104
Storage Module

FIG. 1

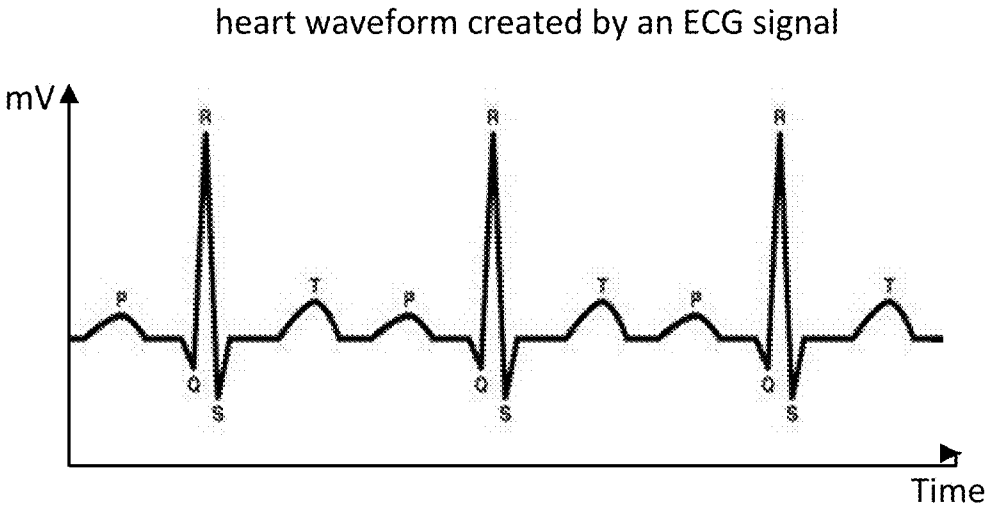

heart waveform created by an ECG signal
mV
R
T
P
Q
S
Time

FIG. 2A

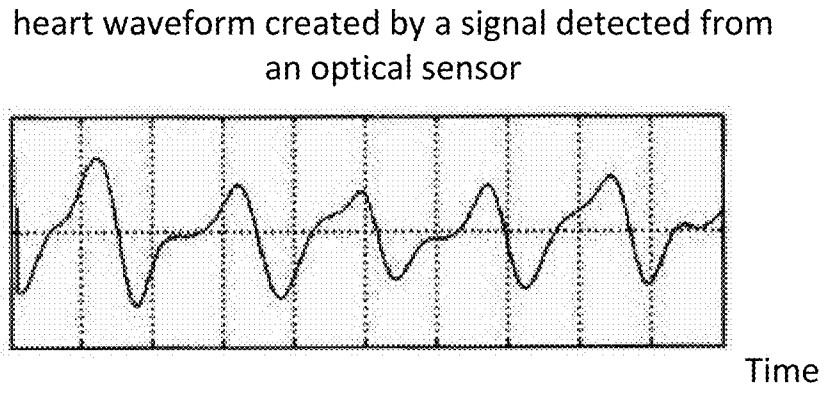

heart waveform created by a signal detected from an optical sensor
Time

FIG. 2B

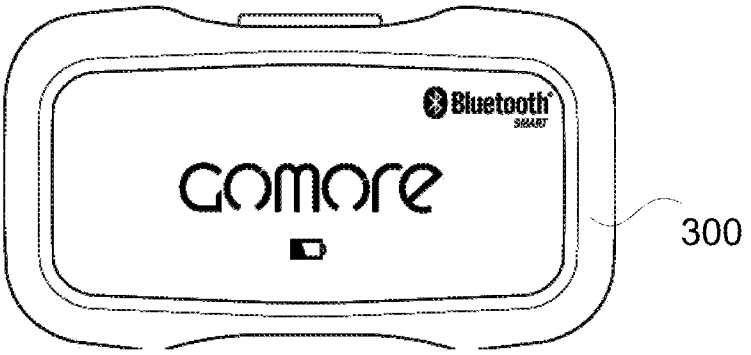


FIG. 3A

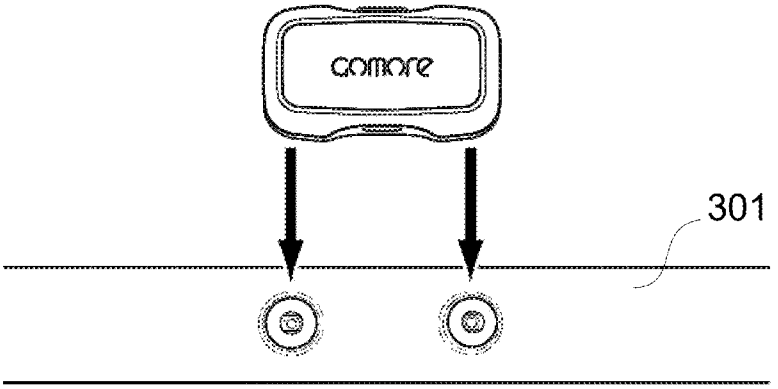


FIG. 3B

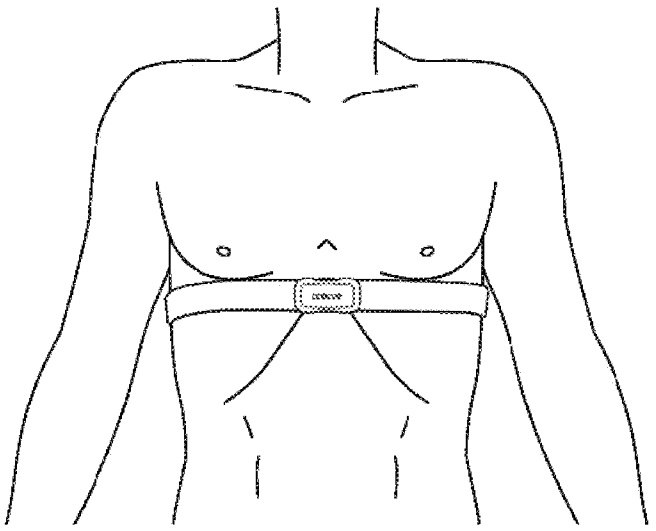


FIG. 3C

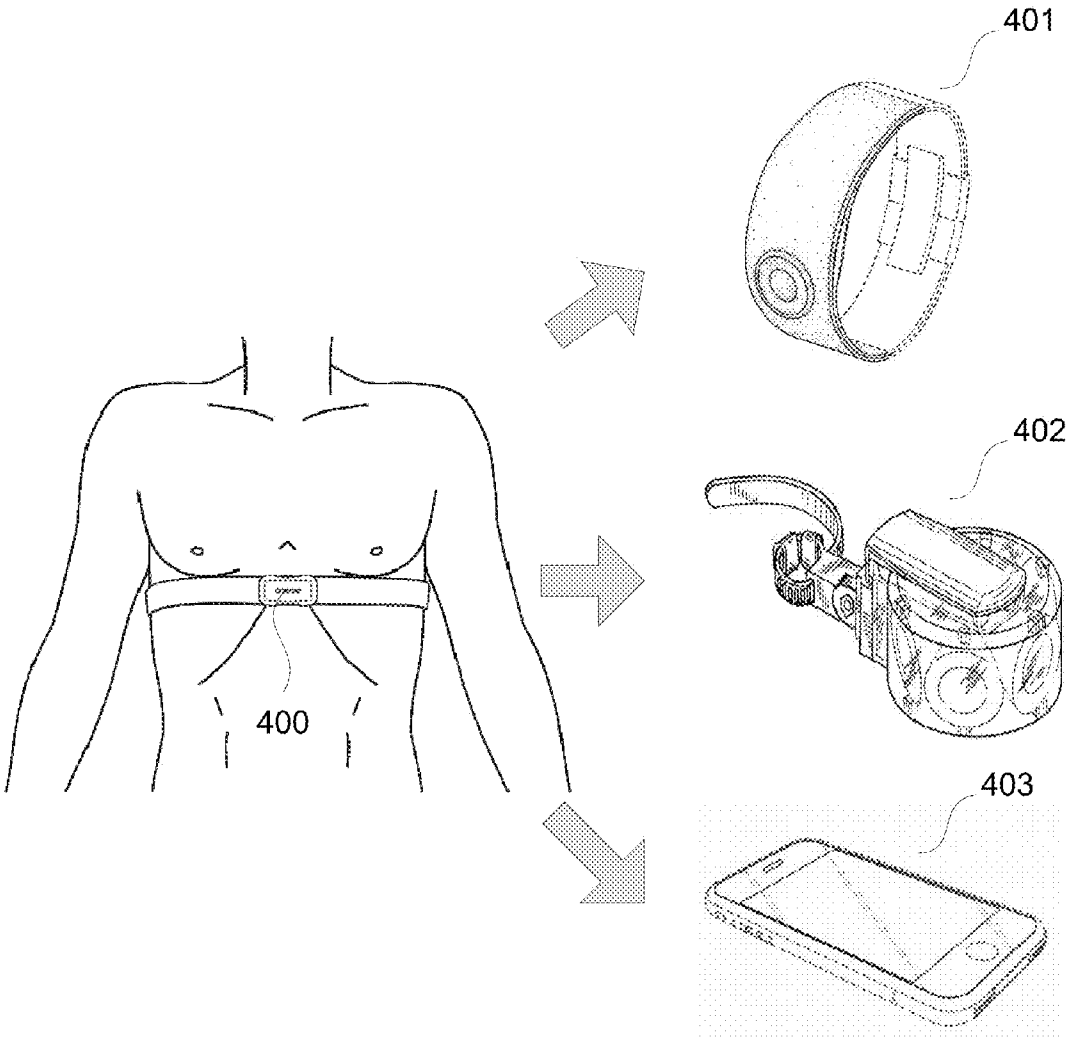


FIG. 4

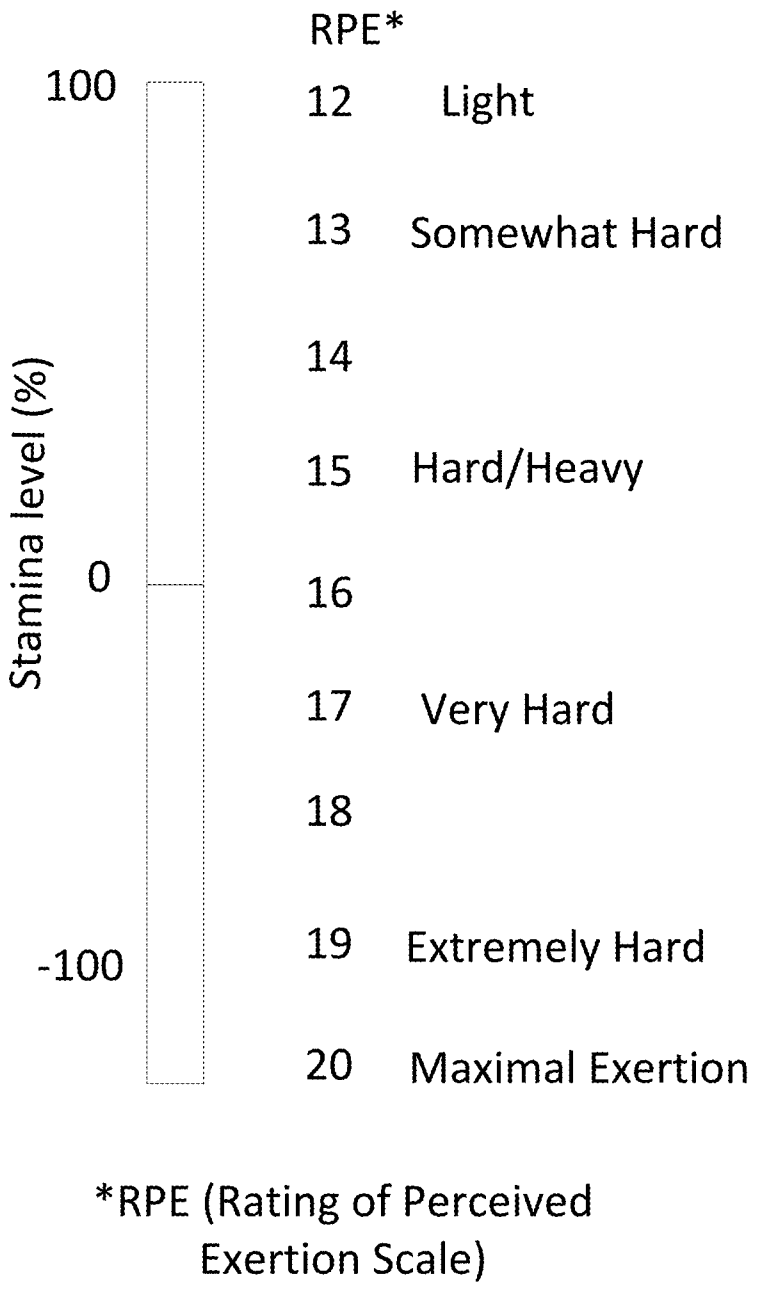

Stamina Level and RPE Mapping
RPE*
100
0
-100
Stamina level (%)
12 Light
13 Somewhat Hard
14
15 Hard/Heavy
16
17 Very Hard
18
19 Extremely Hard
20 Maximal Exertion
*RPE (Rating of Perceived Exertion Scale)

FIG. 5

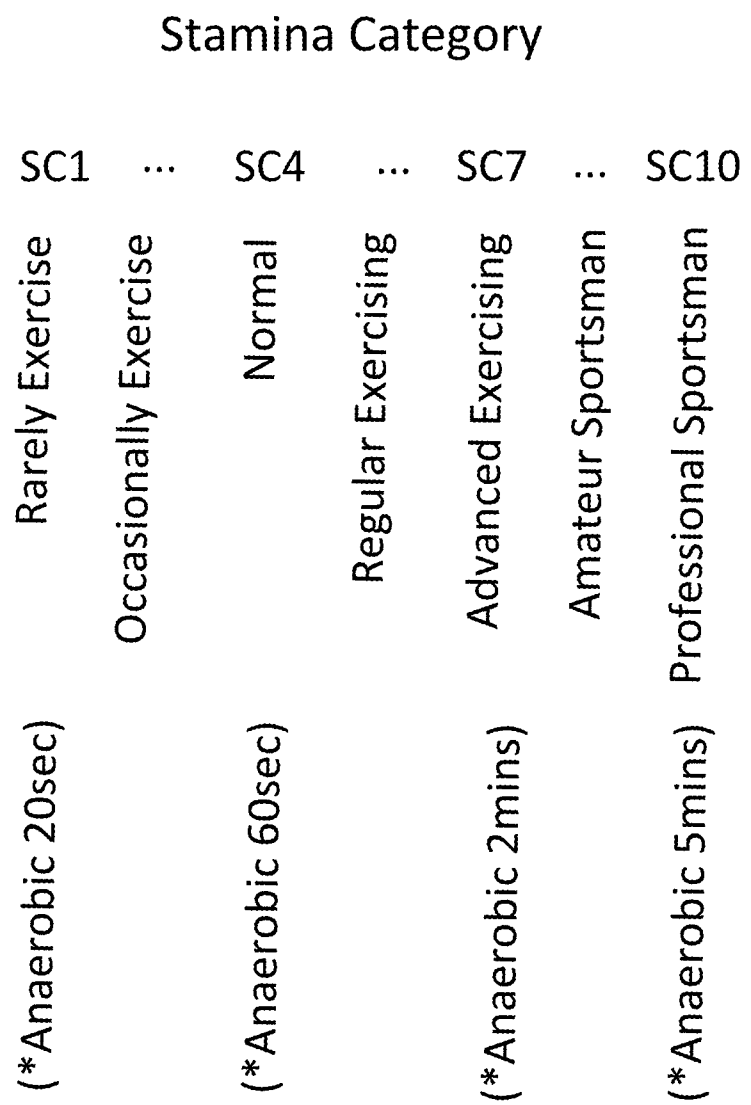

Stamina Category
SC1
...
SC4
...
SC7
...
SC10
Rarely Exercise
Occasionally Exercise
Normal
Regular Exercising
Advanced Exercising
Amateur Sportsman
Professional Sportsman
(*Anaerobic 20sec)
(*Anaerobic 60sec)
(*Anaerobic 2mins)
(*Anaerobic 5mins)

FIG. 6

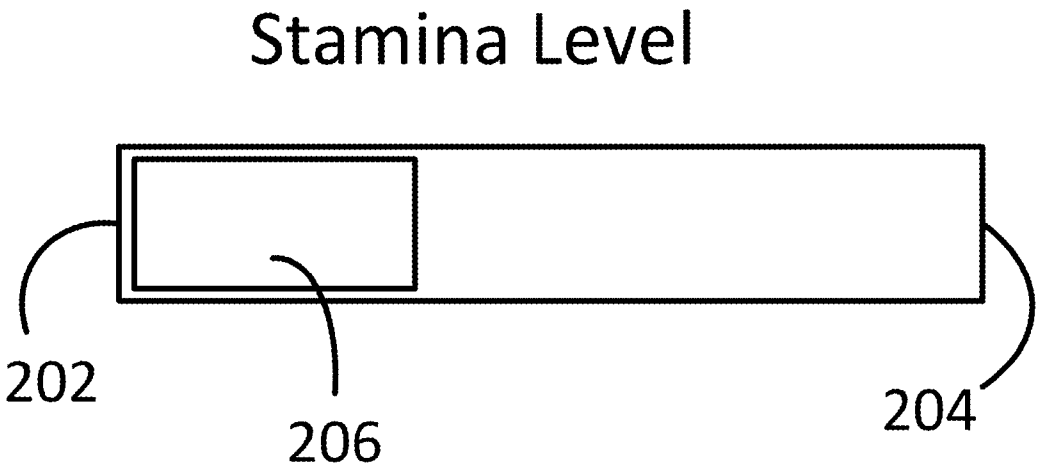


FIG. 7

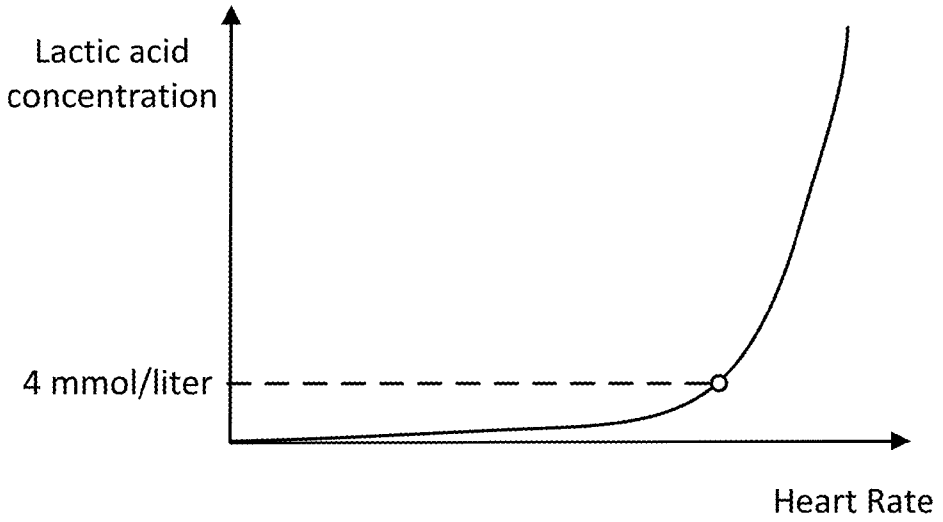


FIG. 8

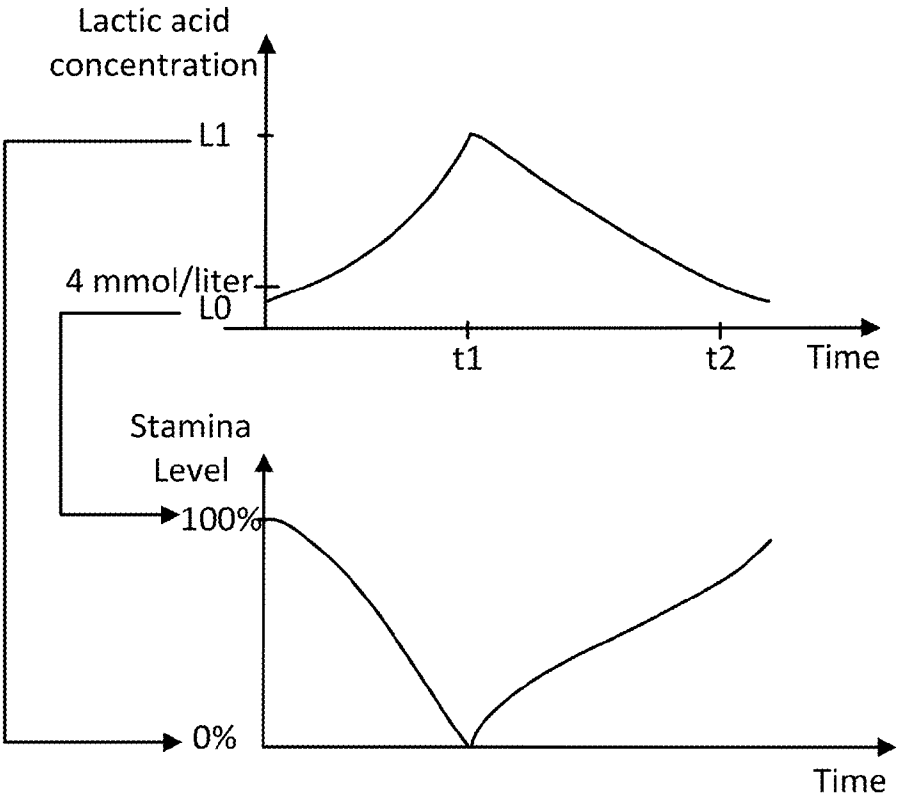

Lactic acid concentration
L1
4 mmol/liter
L0
t1
t2
Time
Stamina Level
100%
0%
Time

FIG. 9

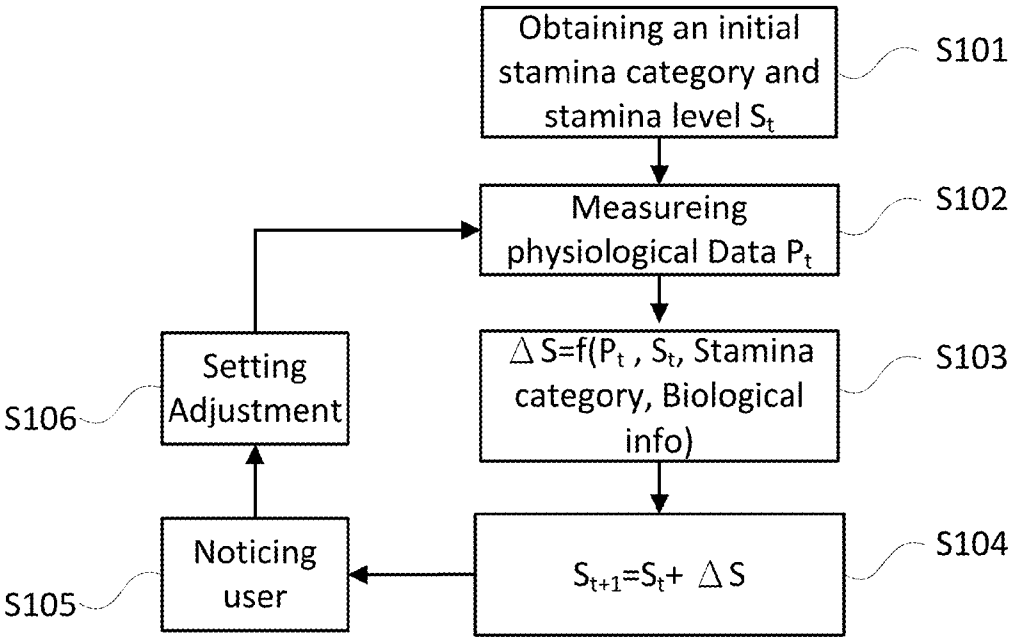

Obtaining an initial stamina category and stamina level S_t
S101
Measureing physiological Data P_t
S102
$\Delta S=f(P_t, S_t,$ Stamina category, Biological info)
S103
$S_{t+1}=S_t+\Delta S$
S104
Noticing user
S105
Setting Adjustment
S106

FIG. 10

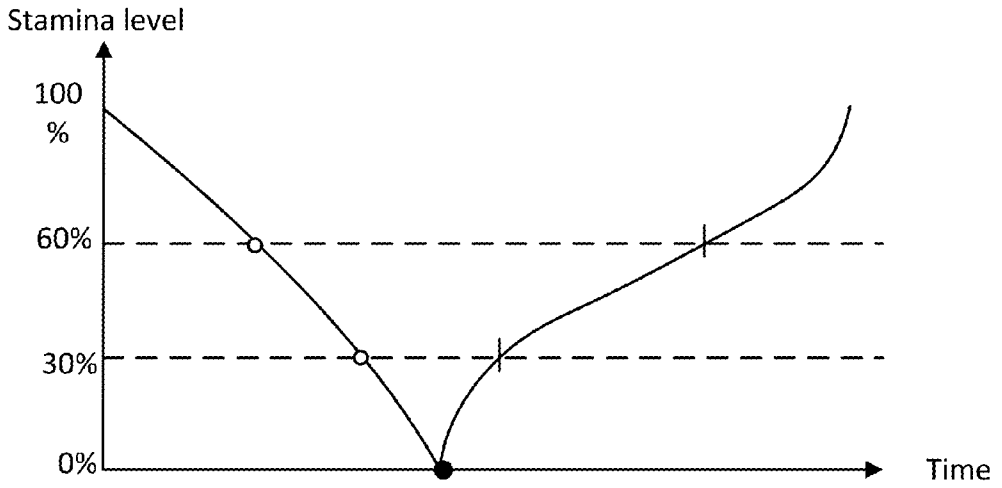


FIG. 11

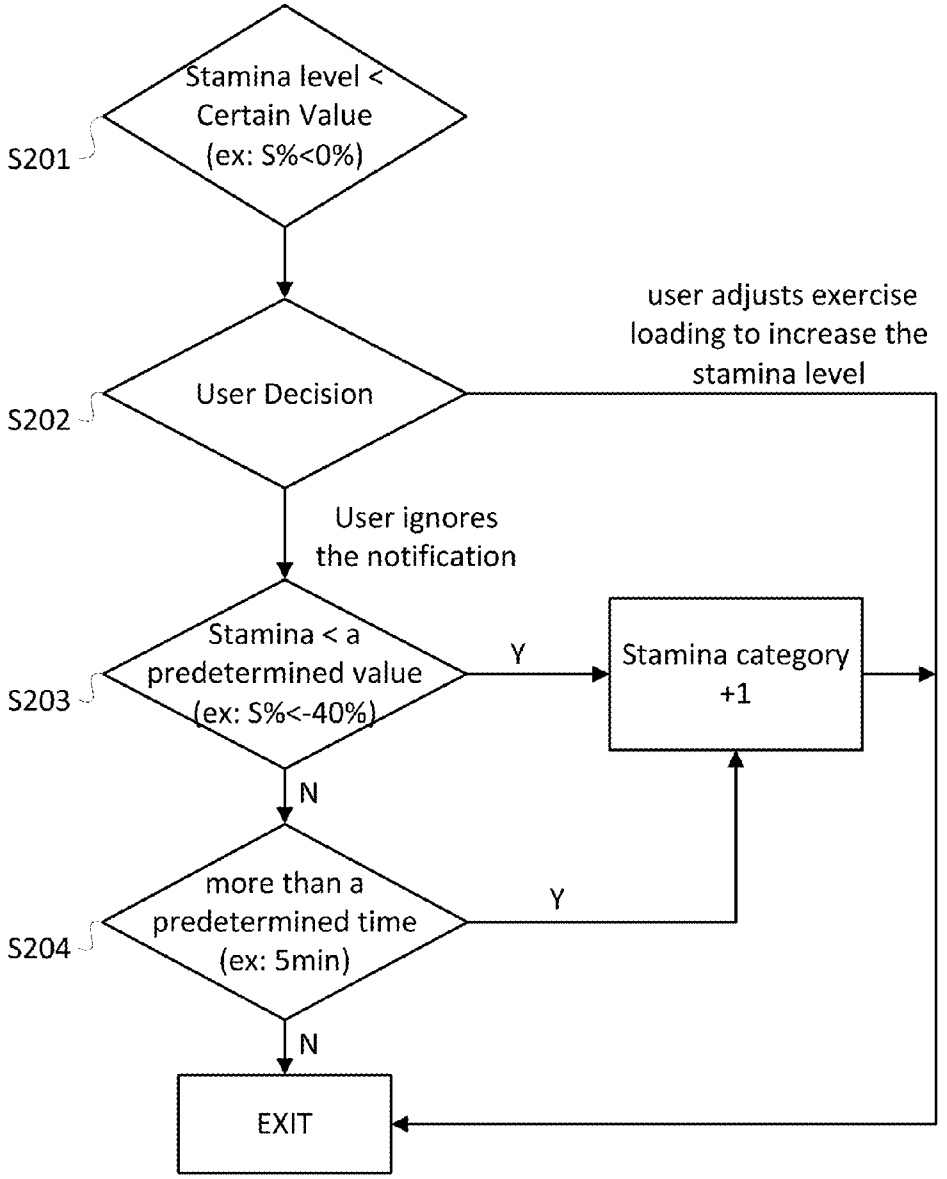

Stamina level < Certain Value (ex: S%<0%)
S201
User Decision
S202
user adjusts exercise loading to increase the stamina level
User ignores the notification
Stamina < a predetermined value (ex: S%<-40%)
S203
Y
Stamina category +1
N
more than a predetermined time (ex: 5min)
S204
Y
N
EXIT

FIG. 12

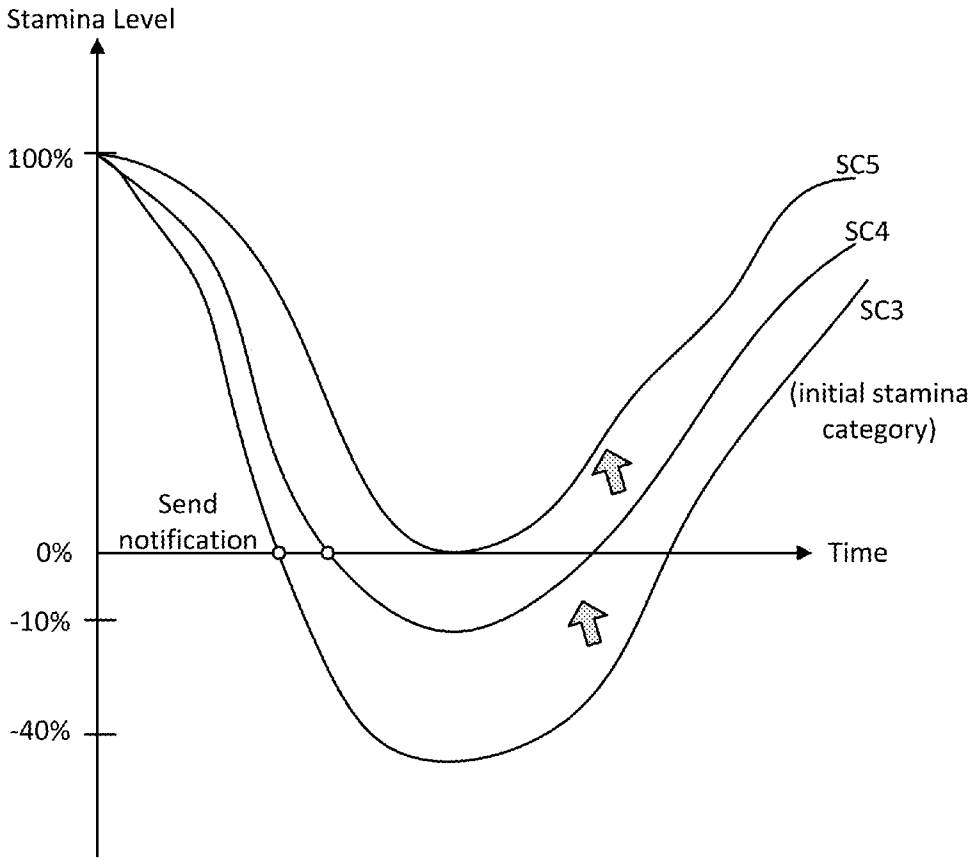

Stamina Level
100%
0%
-10%
-40%
Send
notification
Time
SC5
SC4
SC3
(initial stamina
category)

FIG. 13

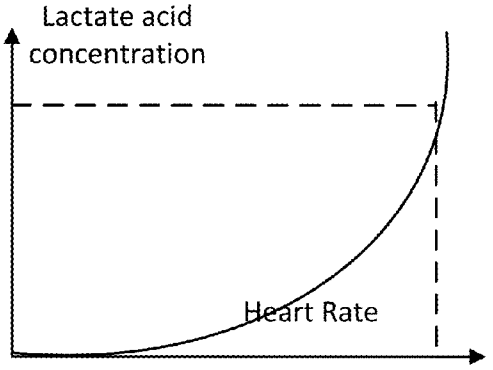


FIG. 14A

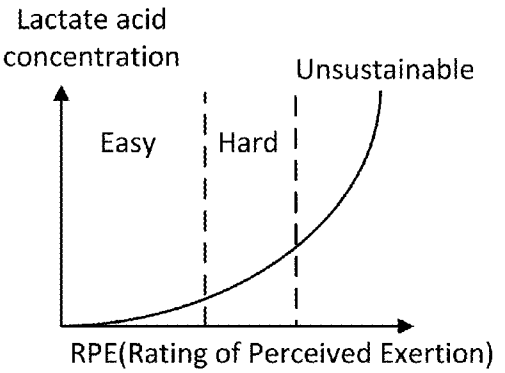


FIG. 14B

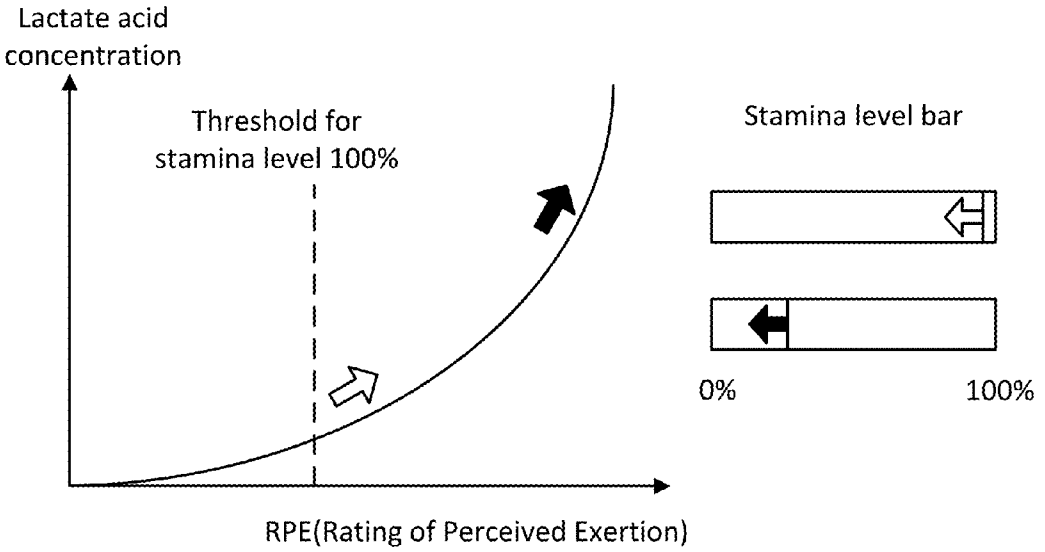


FIG. 14C

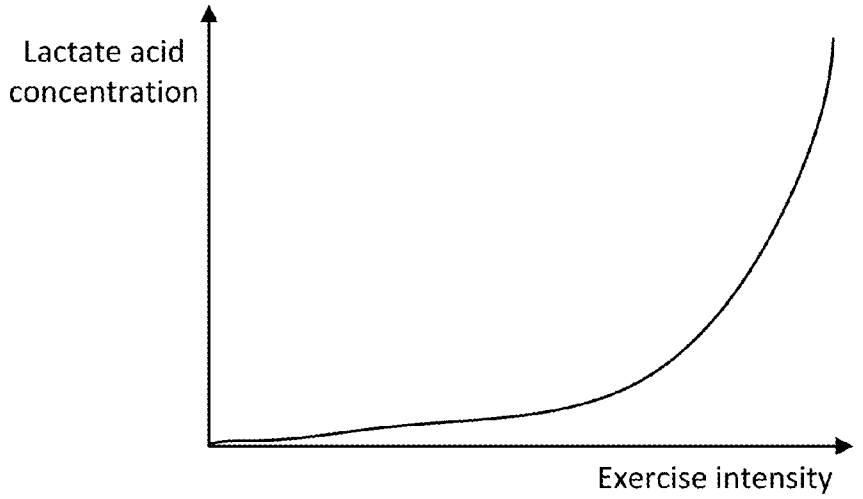


FIG. 15A

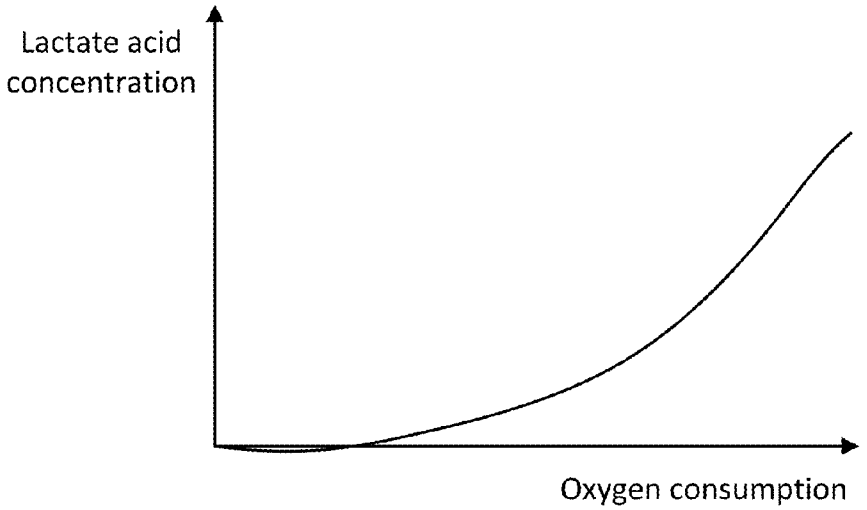


FIG. 15B

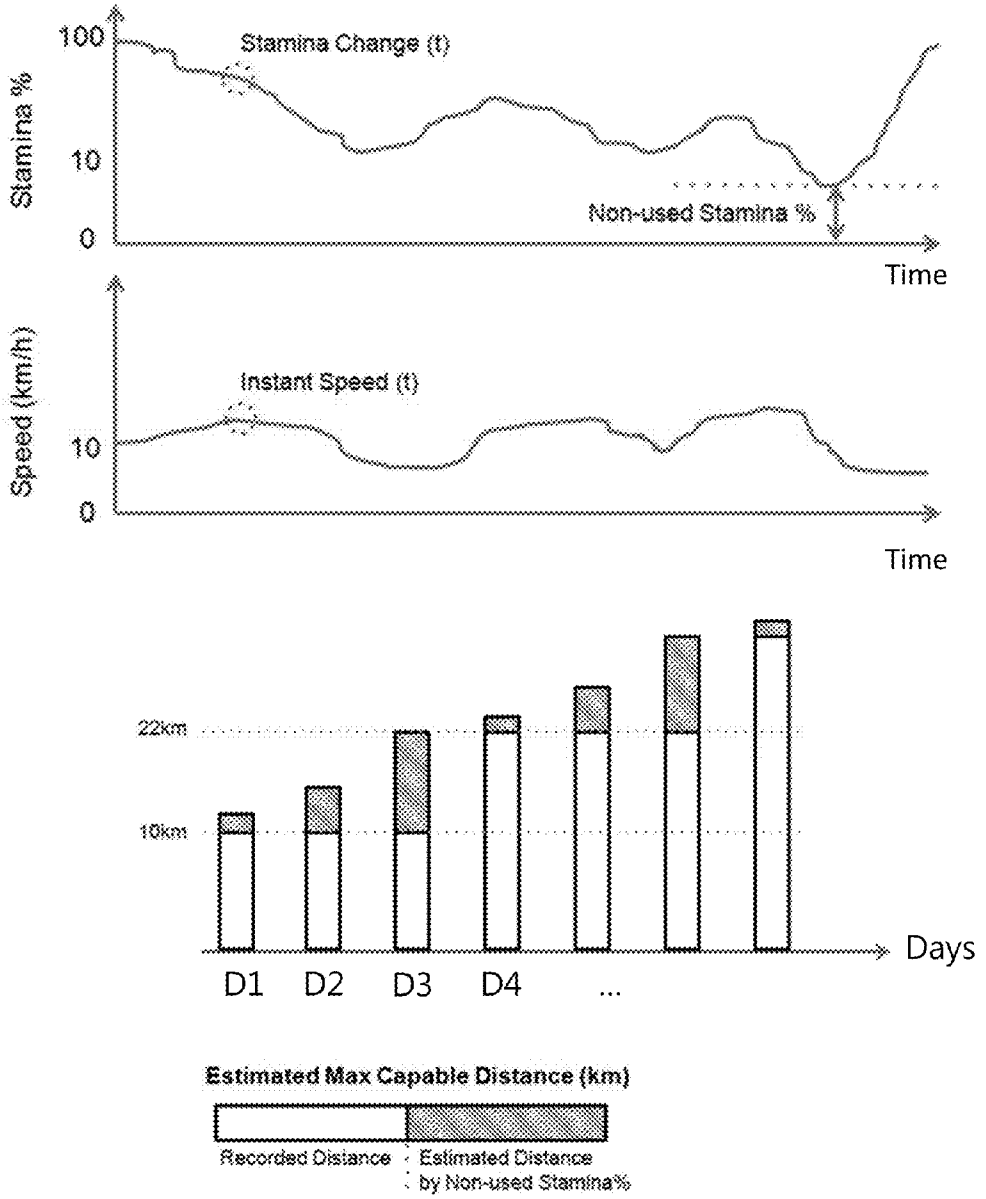

Stamina %
100
10
0
Stamina Change (t)
Non-used Stamina %
Time
Speed (km/h)
10
0
Instant Speed (t)
Time
22km
10km
D1
D2
D3
D4
...
Days
Estimated Max Capable Distance (km)
Recorded Distance
Estimated Distance by Non-used Stamina%

FIG. 16

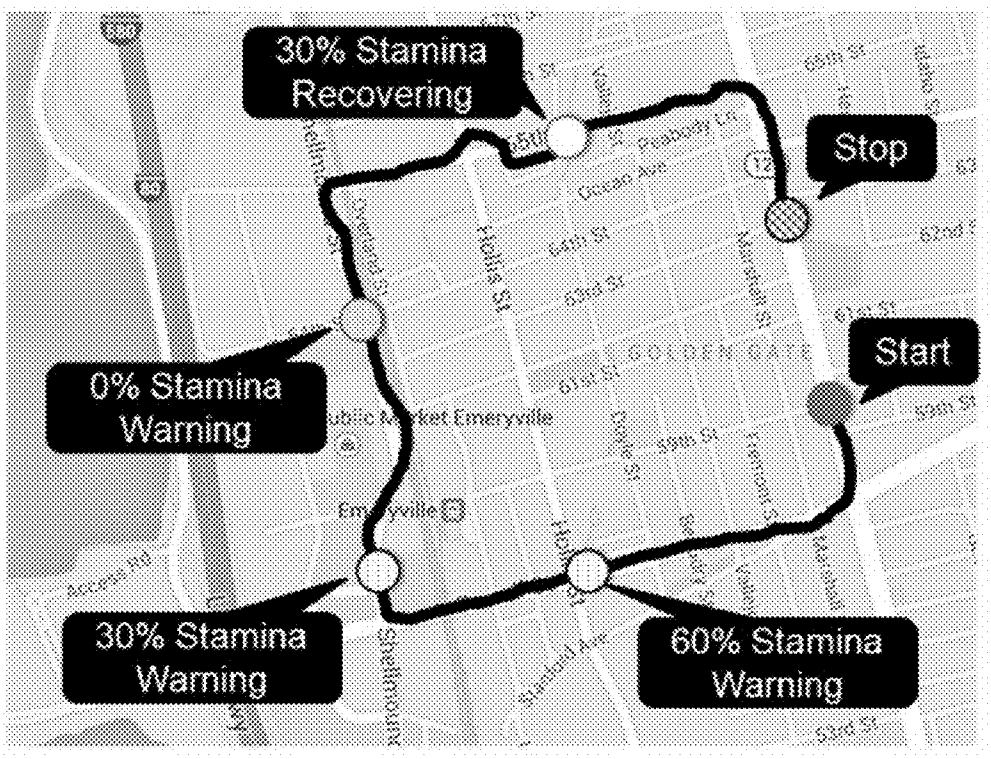

30% Stamina Recovering
Stop
Start
0% Stamina Warning
30% Stamina Warning
60% Stamina Warning

FIG. 17

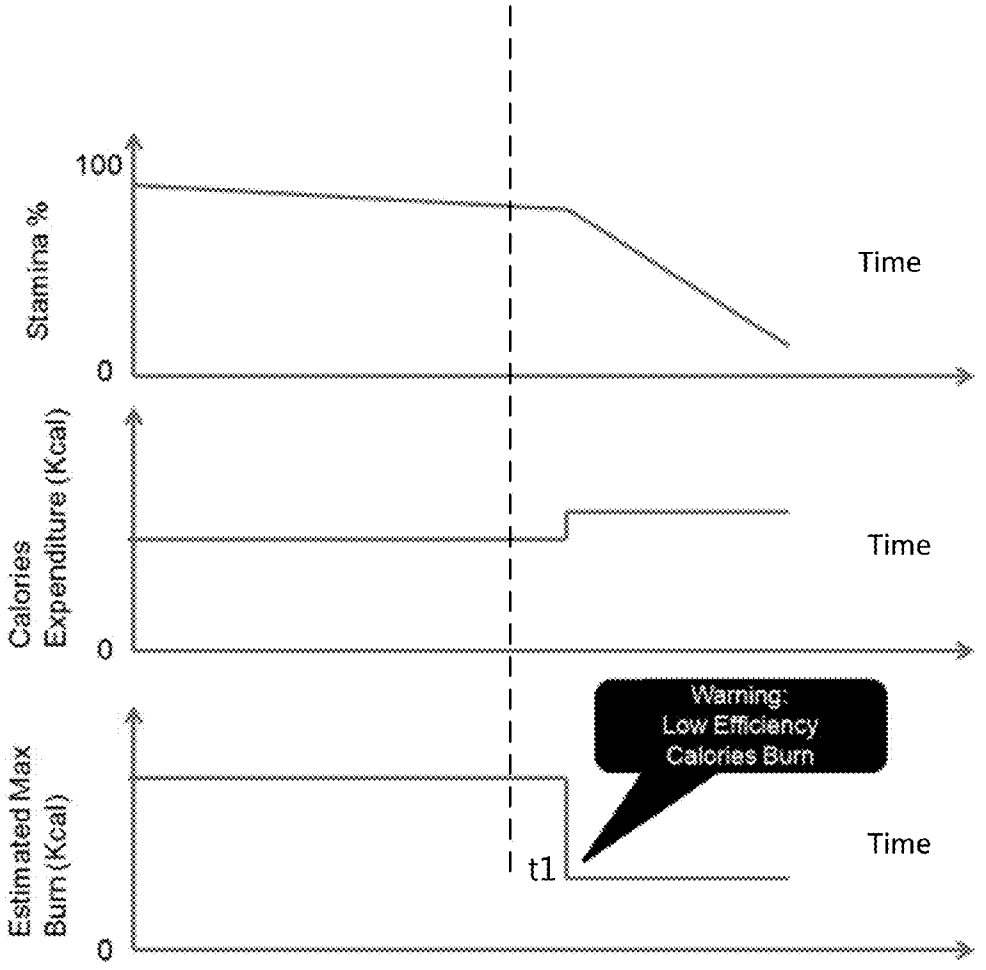

100
Stamina %
0
Time
Calories Expenditure (Kcal)
0
Time
Warning:
Low Efficiency
Calories Burn
Estimated Max Burn (Kcal)
0
t1
Time

FIG. 18

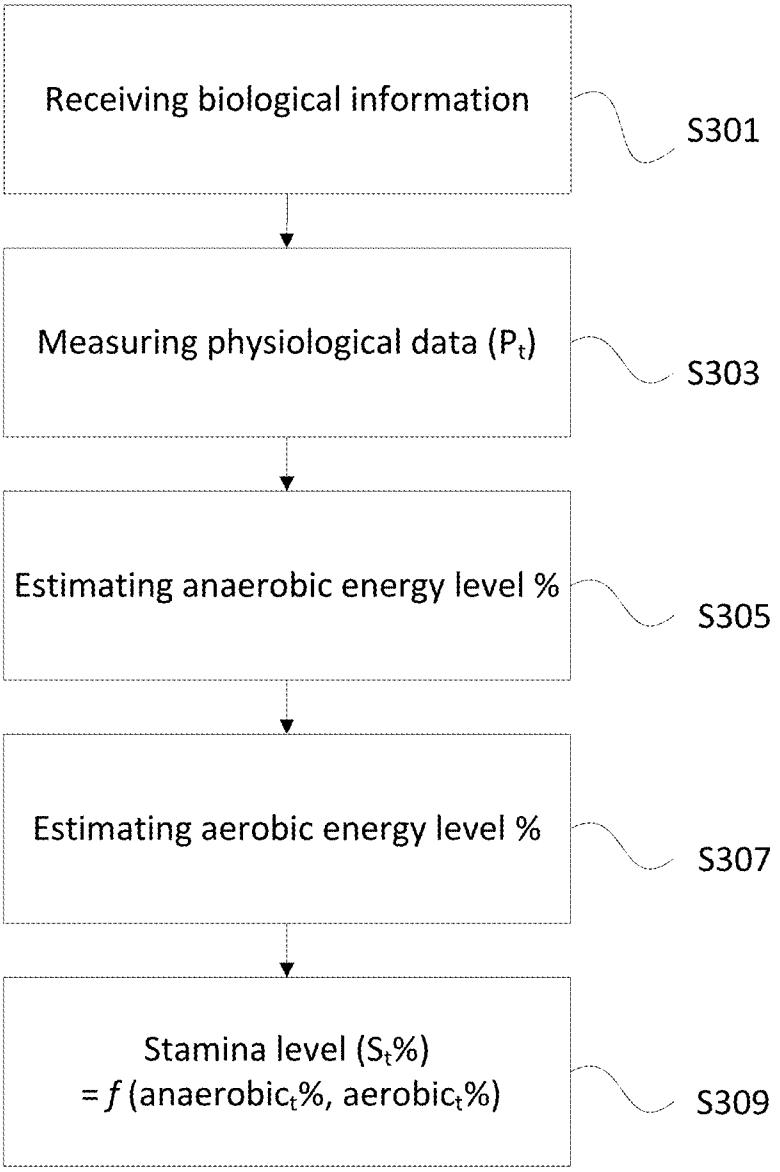

Receiving biological information
S301
Measuring physiological data (P_t)
S303
Estimating anaerobic energy level %
S305
Estimating aerobic energy level %
S307
Stamina level (S_t%)
= f (anaerobic$_t$%, aerobic$_t$%)
S309

FIG. 19

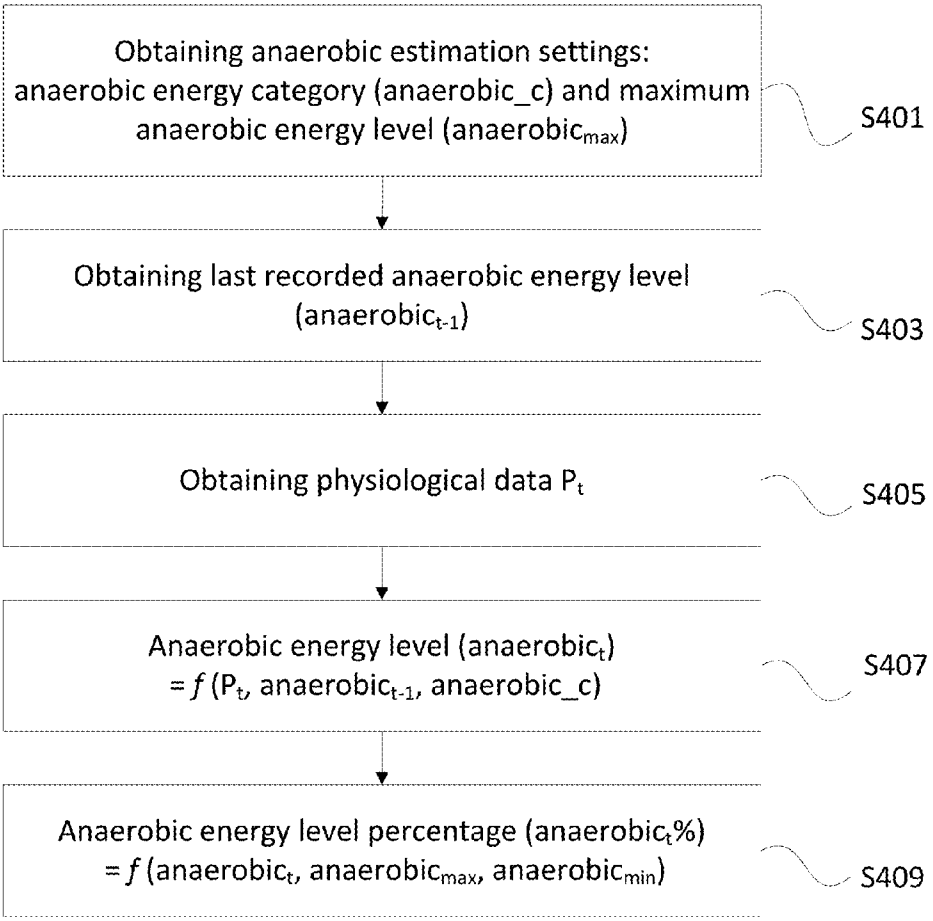

Obtaining anaerobic estimation settings: anaerobic energy category (anaerobic_c) and maximum anaerobic energy level ($anaerobic_{max}$)
S401
Obtaining last recorded anaerobic energy level ($anaerobic_{t-1}$)
S403
Obtaining physiological data P_t
S405
Anaerobic energy level ($anaerobic_t$) = f (P_t, $anaerobic_{t-1}$, anaerobic_c)
S407
Anaerobic energy level percentage ($anaerobic_t$%) = f ($anaerobic_t$, $anaerobic_{max}$, $anaerobic_{min}$)
S409

FIG. 20

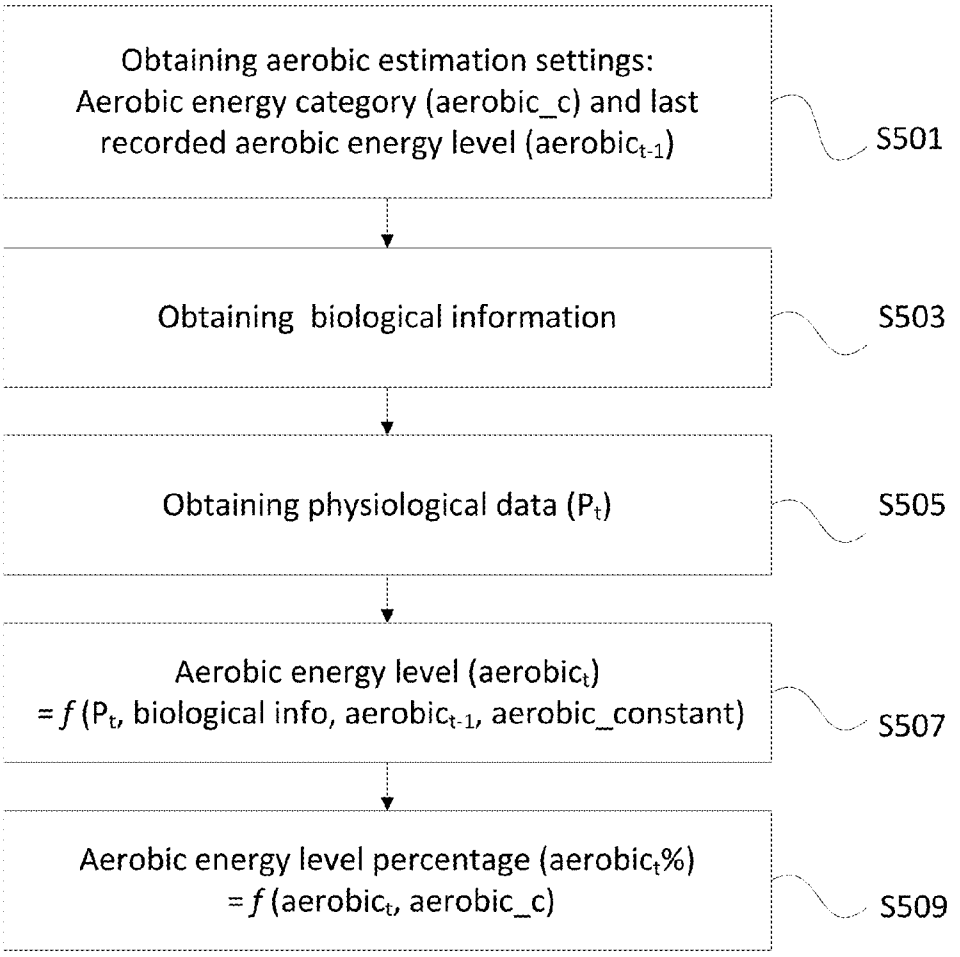

Obtaining aerobic estimation settings: Aerobic energy category (aerobic_c) and last recorded aerobic energy level (aerobic$_{t-1}$)
S501
Obtaining biological information
S503
Obtaining physiological data (P_t)
S505
Aerobic energy level (aerobic$_t$) = f (P_t, biological info, aerobic$_{t-1}$, aerobic_constant)
S507
Aerobic energy level percentage (aerobic$_t$%) = f (aerobic$_t$, aerobic_c)
S509

FIG. 21

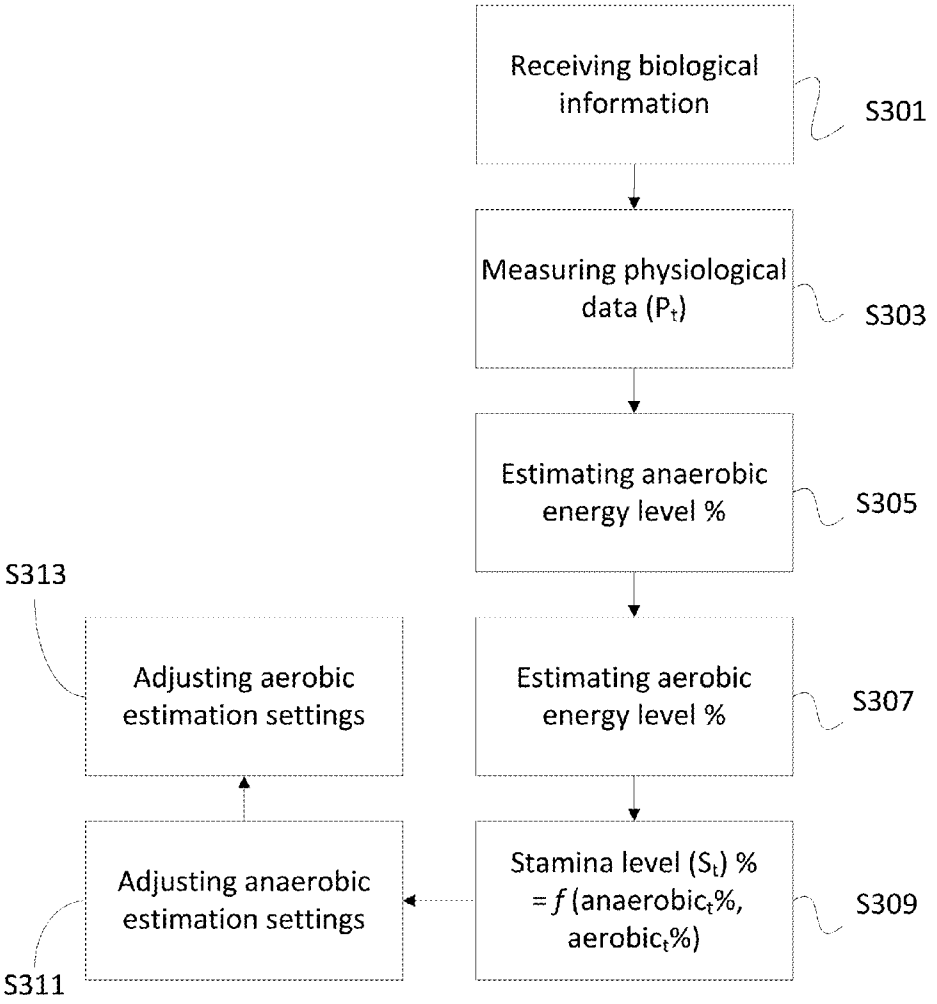

Receiving biological information
S301
Measuring physiological data (P_t)
S303
Estimating anaerobic energy level %
S305
Estimating aerobic energy level %
S307
Stamina level (S_t) % = f (anaerobic$_t$%, aerobic$_t$%)
S309
Adjusting anaerobic estimation settings
S311
Adjusting aerobic estimation settings
S313

FIG. 22

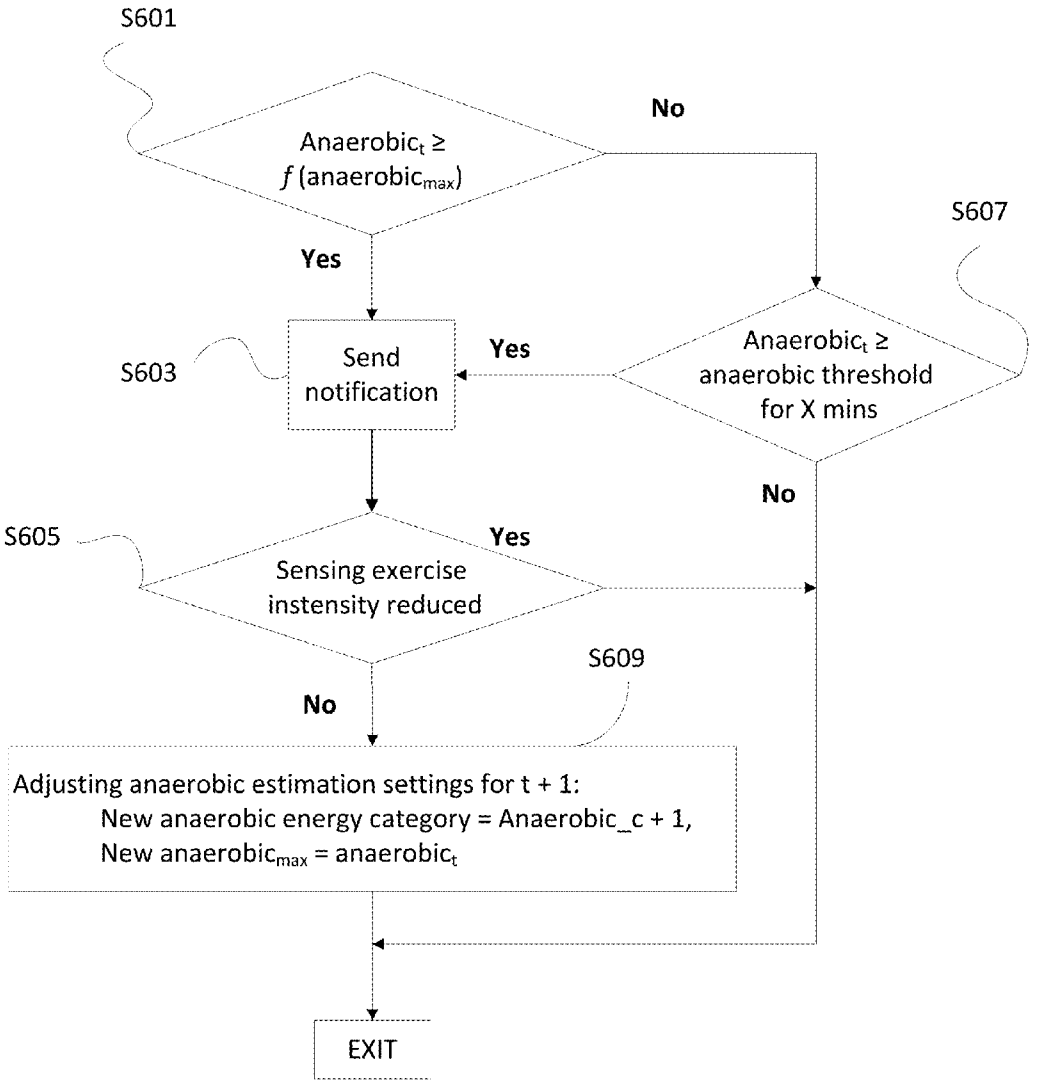

S601
Anaerobic$_t$ ≥ f (anaerobic$_{max}$)
No
Yes
S607
S603
Send notification
Yes
Anaerobic$_t$ ≥ anaerobic threshold for X mins
No
S605
Yes
Sensing exercise instensity reduced
S609
No
Adjusting anaerobic estimation settings for t + 1:
New anaerobic energy category = Anaerobic_c + 1,
New anaerobic$_{max}$ = anaerobic$_t$
EXIT

FIG. 23

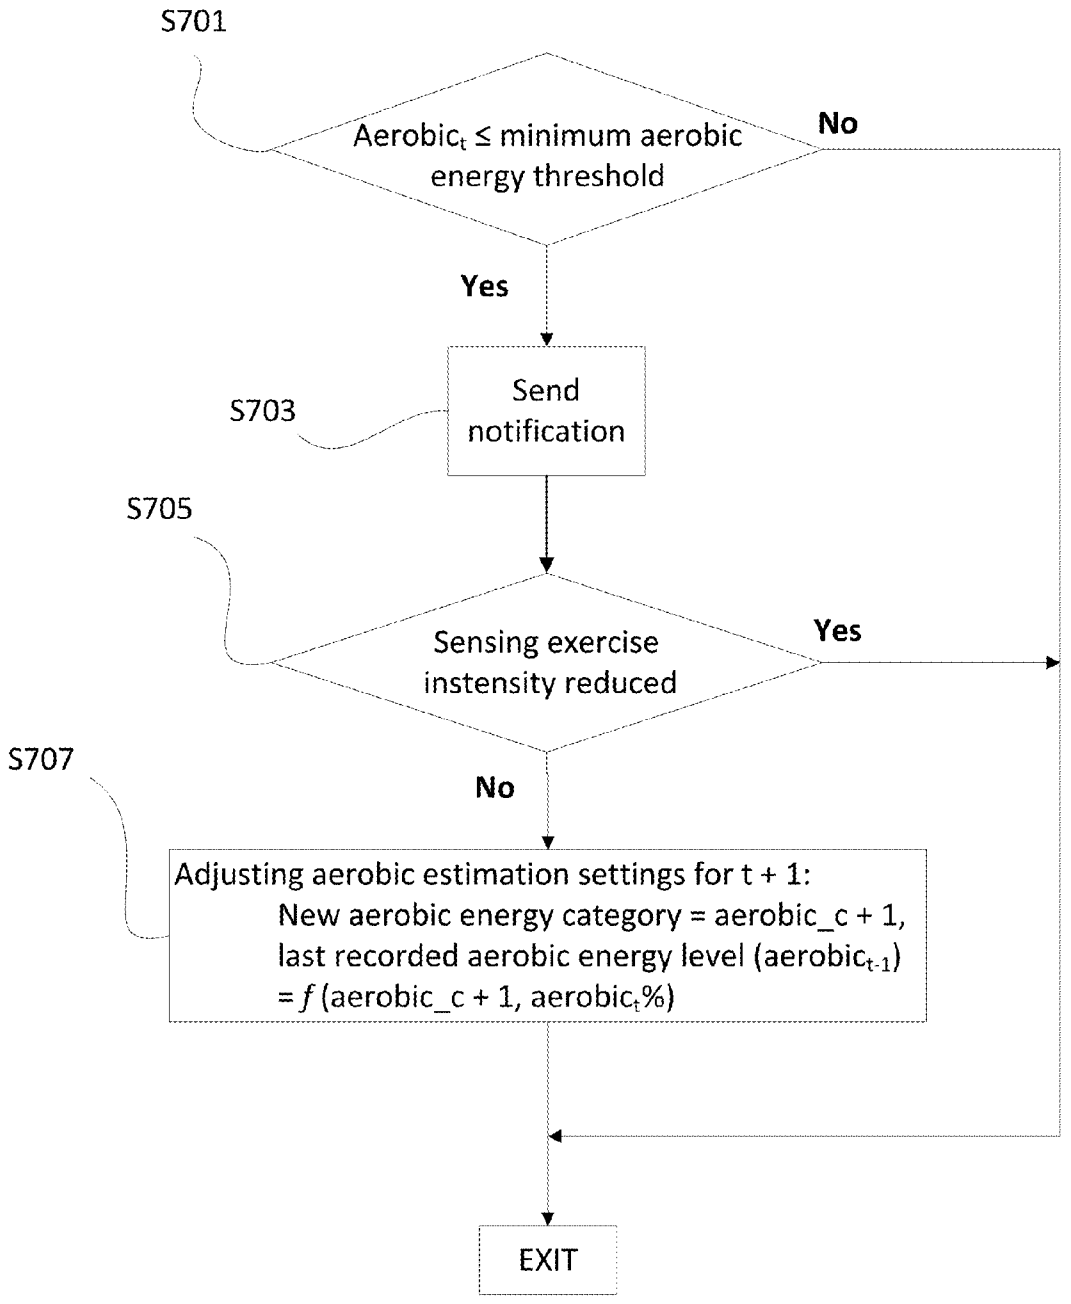

S701
Aerobic$_t$ ≤ minimum aerobic energy threshold
No
Yes
S703
Send notification
S705
Sensing exercise instensity reduced
Yes
S707
No
Adjusting aerobic estimation settings for t + 1:
New aerobic energy category = aerobic_c + 1,
last recorded aerobic energy level (aerobic$_{t-1}$)
= f (aerobic_c + 1, aerobic$_t$%)
EXIT

FIG. 24

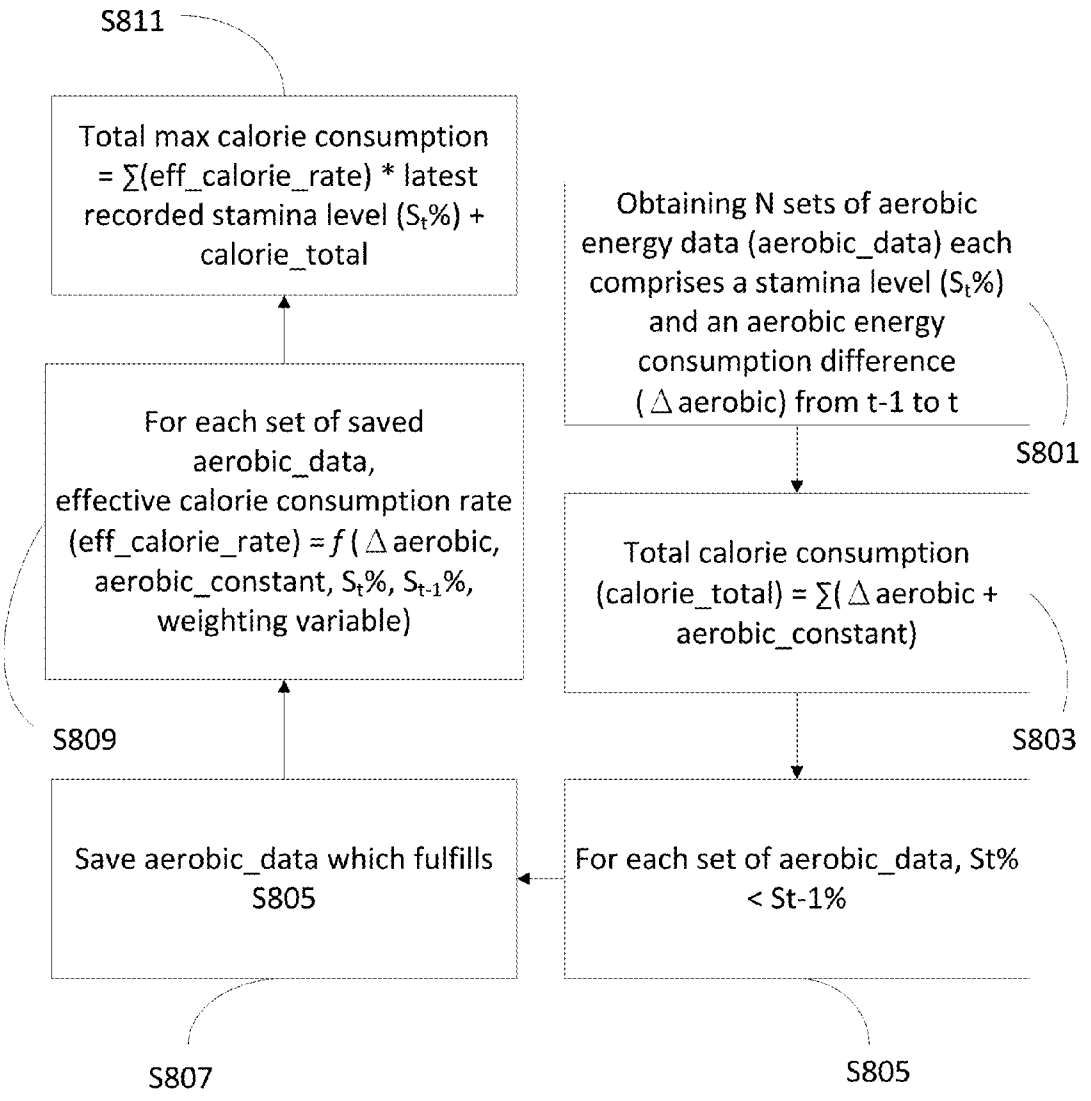

S811
Total max calorie consumption = ∑(eff_calorie_rate) * latest recorded stamina level (S_t%) + calorie_total
For each set of saved aerobic_data, effective calorie consumption rate (eff_calorie_rate) = f (Δ aerobic, aerobic_constant, S_t%, S_{t-1}%, weighting variable)
S809
Save aerobic_data which fulfills S805
S807
Obtaining N sets of aerobic energy data (aerobic_data) each comprises a stamina level (S_t%) and an aerobic energy consumption difference (Δ aerobic) from t-1 to t
S801
Total calorie consumption (calorie_total) = ∑(Δ aerobic + aerobic_constant)
S803
For each set of aerobic_data, St% < St-1%
S805

FIG. 25

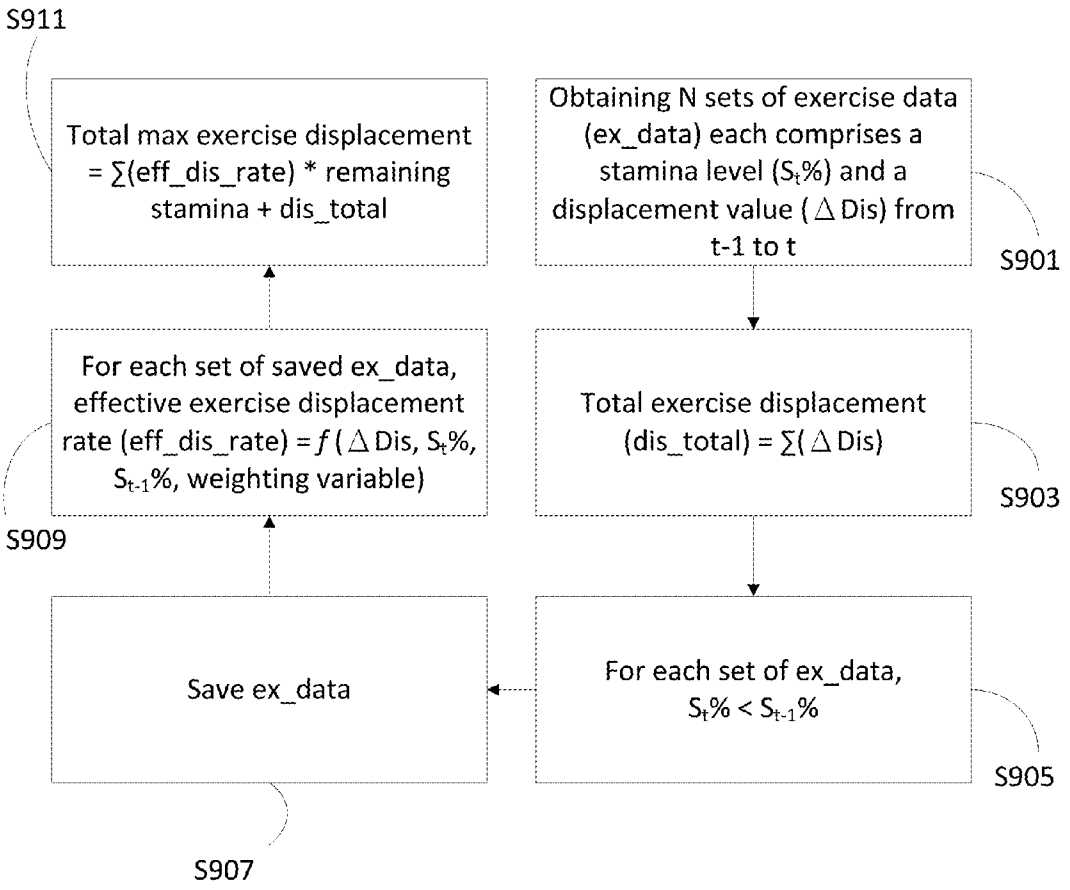

S911
Total max exercise displacement = ∑(eff_dis_rate) * remaining stamina + dis_total
Obtaining N sets of exercise data (ex_data) each comprises a stamina level (S_t%) and a displacement value (Δ Dis) from t-1 to t
S901
For each set of saved ex_data, effective exercise displacement rate (eff_dis_rate) = f (Δ Dis, S_t%, S_{t-1}%, weighting variable)
S909
Total exercise displacement (dis_total) = ∑(Δ Dis)
S903
Save ex_data
S907
For each set of ex_data, S_t% < S_{t-1}%
S905

FIG. 26

STAMINA MONITORING METHOD AND DEVICE

FIELD OF THE INVENTION

[0001] The present invention relates generally to an exercise assistive device. More specifically, the present invention relates to an exercise assistive device and method for indicating stamina of a user and providing notification based on certain conditions.

BACKGROUND OF THE INVENTION

[0002] Professional athletes, sports enthusiasts or people who like exercise often evaluate their own physical conditions during exercises, and thus configure their own physical strengths in order to complete an exercise or a competition. Typically, people evaluate their own physical conditions and environmental factors before or during an exercise to adjust their workouts. In addition, after an exercise, people record and analyze their physical strengths and endurances as references for the next exercise.

[0003] Recently, various types of exercise assistive devices have been developed to assess a user's physical strength in real-time. These devices are capable of providing users with their own physiological signals during exercise, and providing the user with exercise history records for browsing after exercise, and sharing the records with social networks. However, the indication of physiological signal, such as heart rate, often cannot be reliably and accurately correlated to the user's physical strength and endurance. Namely, the provision of only the physiological signal is of no or little effect for the user to decide when the used needs to decrease or increase the intensity during the exercise (i.e. when to slow down or speed up during marathon).

[0004] In view of the above, what is needed is an exercise assistive device and method which reliably indicates a stamina level of each of the users regardless of the differences of the physical condition among each of the users.

BRIEF DESCRIPTION OF THE DRAWINGS

[0005] The accompanying drawings illustrate one or more embodiments of the invention and together with the written description, serve to explain the principles of the invention. Wherever possible, the same reference numbers are used throughout the drawings to refer to the same or like elements of an embodiment, and wherein:

[0006] FIG. **1** is a schematic block diagram of an exercise assistive device according to at least one embodiment of the present invention.

[0007] FIGS. **2**A and **2**B are schematic illustrations of heart waveform created by an EKG signal or by a signal detected from an optical sensor, respectively, according to at least one embodiment of the present invention.

[0008] FIGS. **3**A to **3**C are schematic illustrations of an exemplary exercise assistive device according to one embodiment of the present invention.

[0009] FIG. **4** is a schematic illustration of types of exemplary exercise assistive devices according to another embodiment of the present invention.

[0010] FIG. **5** is a schematic illustration of the mapping concept between stamina level and RPE.

[0011] FIG. **6** a schematic illustration of the relationship between exemplary stamina categories and the fitness condition of a user.

[0012] FIG. **7** is a schematic illustration of an exemplary stamina level indicator according to at least one embodiment of the present invention.

[0013] FIG. **8** is a schematic illustration of the correlation between lactic acid concentration and heart rate.

[0014] FIG. **9** is a schematic illustration of the changes in lactic acid concentration with respect to the exercise time period of a user and the mapping between lactic acid concentration and stamina level.

[0015] FIG. **10** is a flowchart of a method for estimating stamina level according to at least one embodiment of the present invention.

[0016] FIG. **11** is a schematic illustration of the examplary conditions for sending notifications to a user according to at least one embodiment of the present invention.

[0017] FIG. **12** is a flowchart of a method for adjusting stamina category according to at least one embodiment of the present invention.

[0018] FIG. **13** is a schematic illustration of the exemplary conditions where stamina category can be automatically adjusted in FIG. **12**.

[0019] FIGS. **14**A and **14**B are schematic illustrations of relationship among heart rate, lactate acid concentration and RPE, and FIG. **14**C is the mapping between stamina level and RPE related to lactate acid concentration according to at least one embodiment of the present invention.

[0020] FIGS. **15**A and **15**B are schematic illustrations of relationship between the lactate acid concentration and exercise intensity or that between the lactate acid concentration and oxygen consumption.

[0021] FIG. **16** is a schematic illustration of an exemplary application of estimating a user's maximum exercise distance using the user's stamina level and exercise speed.

[0022] FIG. **17** is a schematic illustration of an exemplary application of outputting the user's stamina level in conjunction with a map.

[0023] FIG. **18** is a schematic illustration of an exemplary application of estimating a user's calorie consumption by utilizing the user's stamina level.

[0024] FIG. **19** is a method to estimate stamina level based on physiological data according to one embodiment of the present invention;

[0025] FIG. **20** is a method to estimate anaerobic energy based on physiological data according to one embodiment of the present invention;

[0026] FIG. **21** is a method to estimate aerobic energy based on physiological data according to one embodiment of the present invention;

[0027] FIG. **22** is a method to estimate stamina level based on physiological data with setting adjustments according to one embodiment of the present invention;

[0028] FIG. **23** is a method to adjust anaerobic estimation settings for the method to estimate stamina level according to one embodiment of the present invention;

[0029] FIG. **24** is a method to adjust aerobic estimation settings for the method to estimate stamina level according to one embodiment of the present invention;

[0030] FIG. **25** is a method to estimate total maximum calorie consumption according to one embodiment of the present invention;

[0031] FIG. **26** is a method to estimate total maximum exercise displacement according to one embodiment of the present invention.

[0032] In accordance with common practice, the various described features are not drawn to scale and are drawn to emphasize features relevant to the present disclosure. Like reference characters denote like elements throughout the figures and text.

DETAILED DESCRIPTION OF THE INVENTION

[0033] The present invention will now be described more fully hereinafter with reference to the accompanying drawings, in which exemplary embodiments of the invention are shown. This invention may, however, be embodied in many different forms and should not be construed as limited to the embodiments set forth herein. Rather, these embodiments are provided so that this disclosure will be thorough and complete, and will fully convey the scope of the invention to those skilled in the art. Like reference numerals refer to like elements throughout.

[0034] The terminology used herein is for the purpose of describing particular embodiments only and is not intended to be limiting of the invention. As used herein, the singular forms "a", "an" and "the" are intended to include the plural forms as well, unless the context clearly indicates otherwise. It will be further understood that the terms "comprises" and/or "comprising," or "includes" and/or "including" or "has" and/or "having" when used herein, specify the presence of stated features, regions, integers, steps, operations, elements, and/or components, but do not preclude the presence or addition of one or more other features, regions, integers, steps, operations, elements, components, and/or groups thereof.

[0035] It will be understood that the term "and/or" includes any and all combinations of one or more of the associated listed items. It will also be understood that, although the terms first, second, third etc. may be used herein to describe various elements, components, regions, parts and/or sections, these elements, components, regions, parts and/or sections should not be limited by these terms. These terms are only used to distinguish one element, component, region, part or section from another element, component, region, layer or section. Thus, a first element, component, region, part or section discussed below could be termed a second element, component, region, layer or section without departing from the teachings of the present invention.

[0036] Unless otherwise defined, all terms (including technical and scientific terms) used herein have the same meaning as commonly understood by one of ordinary skill in the art to which this invention belongs. It will be further understood that terms, such as those defined in commonly used dictionaries, should be interpreted as having a meaning that is consistent with their meaning in the context of the relevant art and the present disclosure, and will not be interpreted in an idealized or overly formal sense unless expressly so defined herein.

[0037] The description will be made as to the embodiments of the present invention in conjunction with the accompanying drawings in FIGS. **1**~**18**. Reference will be made to the drawing figures to describe the present invention in detail, wherein depicted elements are not necessarily shown to scale and wherein like or similar elements are designated by same or similar reference numeral through the several views and same or similar terminology.

[0038] FIG. **1** is a schematic block diagram of an exercise assistive device (also known as stamina monitoring device) according to at least one embodiment of the present invention.

[0039] Referring to FIG. **1**, the exercise assistive device **100** includes a sensor module **101**, a processing module **102**, a user interface **103** and a storage module **104**.

[0040] The sensor module **101** includes at least one sensor for sensing and measuring physiological signals of the user. For example, the physiological signal comprises at least one of the following: EKG signal, heart rate variability, pulse, heart rate, breathing pattern, body temperature, body composition, blood glucose, blood pressure, glycogen concentration, and oxygen concentration. The body composition may comprise percentages of fat, bone, water and muscle in human bodies.

[0041] The processing module **102** is hardware such as a microcontroller or a microprocessor with auxiliary circuits that carries out the instructions of a computer program by performing the basic arithmetical, logical, and input/output operations of the exercise assistive device.

[0042] The user interface **103** comprises at least one output unit and/or at least one input unit, or any combination thereof. The output can be a display, a vibrating component or a speaker, or any combination thereof for stating the user's stamina level during or after the exercise of a user. The input can be any human-machine interface such as a touch-panel, a voice receiver or a button that is capable of receiving biological information from the user, such as height, weight, age, gender and so forth. In addition, the user interface **103** can be adapted to send information directly to the sensor module **101**, the processing module **102** or the storage module **104**. The inputted information may be processed by the processing module **102** and send to the output for the user to know the user's current body condition. For example, BMI value, etc.

[0043] The storage module **104** can be any type of disk or memory for storing information from the sensor module **101**, the processing module **102** or the user interface **103**. For example, the stored information can be activity history or biological information of the user, and the aforementioned information can be used to calculate the user's stamina level and can be used to calculate the user's initial stamina category, since the activity history or the biological information can be used to calculate a base blood lactate acid concentration, a base heart rate, a base oxygen intake rate, or any combination thereof that associates with a rest state of the user.

[0044] It should be noticed that the term, stamina, refers to the ability of an organism to exert itself and remain active for a period of time. Furthermore, the concept of the stamina level and the stamina category will be brought out in the following paragraphs.

[0045] Referring back to FIG. **1**, the processing module **102** receives the physiological signal from the sensor module **101** and processes based on the physiological signal and the instructions stored in the storage module **104**, and provides processed information as results to the user interface **103**. In addition, the processing module **102** can also receive instructions from the user interface **103** as input and carries out the instructions with or without the information stored in the storage module **104**, and provides commands to operate the sensor module **101**.

[0046] The sensor module **101**, the processing module **102**, the user interface **103** and the storage module **104** can be configured with wired or wireless connection. The wired connection can be any type of physical contact, for example, an electric cable or conduct lines on printed circuit board. The

wireless connection can be any type of wireless transmission, such as WiFi, Bluetooth, or radio frequency assisted transmission.

[0047] FIGS. **2**A and **2**B are schematic illustrations of heart waveform created by an EKG signal or by a signal detected from an optical sensor, respectively, according to at least one embodiment of the present invention.

[0048] Referring to FIG. **2**A, in the sensor module **101** of the exercise assistive device **100**, the sensor for monitoring heart rate can be an electrocardiography (EKG) sensor. Referring to FIG. **2**B, in the sensor module **101** of the exercise assistive device **100**, the sensor for monitoring heart rate can be an optical sensor. Since the optical sensor is sensitive to artifacts such as other heart related signals and body movements, which interfere with the actual heart rate signal and reduce the accuracy of the heart rate reading, the EKG sensor is preferred over the optical sensor as the EKG sensor senses P, Q, R, S and T waves from different operational stages of the heart. The artifacts in an EKG signal can be distinguished from the PQRST waves, thus removing the artifacts to provide an accurate heart rate reading. Namely, the heart rate of a user is determined based on the time intervals between specific EKG waves. For example, the time interval between each consequent T wave or R wave corresponds to the time between each heartbeat. In addition, the EKG signal is used to filter noises through the identification of its specific characteristics of waveform, such as T wave, thus preventing taking irrelevant artifacts in to consideration of heart rate calculation.

[0049] FIGS. **3**A to **3**C are schematic illustrations of an exemplary exercise assistive device according to one embodiment of the present invention.

[0050] Referring to FIGS. **3**A to **3**C, the exercise assistive device **300** may be a single device having casing that houses at least one of the sensor module **101**, the processing module **102**, the user interface **103** and the storage module **104**. Also, the exercise assistive device **300** may be a single device having casing that houses all of the sensor module **101**, the processing module **102**, the user interface **103** and the storage module **104**. The exercise assistive device **300** may be part of a wearable device to be worn around a human's body part, for example, chest, a wrist, an arm, waist, or a leg, to sense and measure the physiological signals from the body part of the user.

[0051] Referring to FIG. **3**A, the exercise assistive device **300** comprises an casing that houses a sensor module **101**, a processing module **102**, a user interface **103** and a storage module **104**. Referring to FIG. **3**B, the exercise assistive device **300** also comprises a strap **301** (i.e. an elastic band) for strapping the exercise assistive device **300** around a user's chest and positioning the exercise assistive device **100** at the vicinity of the user's heart. In addition, the sensor module **101** of the exercise assistive device **300** may has at least one electrode (i.e. two electrodes connected with the strap) to sense an EKG signal of the user. Referring to FIG. **3**C, the exercise assistive device **300** having the strap **301** is worn around a user's chest and thus the EKG signal of the user's heartbeat can be sensed. Furthermore, the exercise assistive device **300** also comprises a vibrating component within the casing for sending vibrating notifications to the user according to the change in the stamina level during the exercise of the user. Again, it should be noticed that the concept of the stamina level will be brought out in the following paragraphs.

[0052] FIG. **4** is a schematic illustration of types of exemplary exercise assistive devices according to another embodiment of the present invention.

[0053] Referring to FIG. **4**, the exercise assistive device **100** may be separate into a first device and a second device. The first device can be configured to wirelessly communicate with the second device. The first device can be a combination of at least one of the sensor module **101**, the processing module **102**, the user interface **103** or the storage module **104**. The second device can be a combination of at least one of the sensor module **101**, the processing module **102**, the user interface **103** or the storage module **104**. Based on the collaboration of the first device and the second device, the function of the original exercise assistive device **100** can be completely operated as well.

[0054] The first device can be part of a wearable device **400** to be worn around a human's body part, for example, a chest, a wrist, an arm, waist, or a leg, to sense and measure the physiological signals from the body part. The second device can be a part of an extended device such as a bracelet, a cycling meter, a smart phone, running watches, fitness equipment, or any combination thereof.

[0055] To clearly illustrate, the aforementioned extended device may be a bracelet **401** that comprises a user interface that visually illustrates the stamina level of a user in a range, for example from 100% to 0%. The aforementioned extended device may also be an indicator light **402** equipped at the rear of a cycle that illuminates different colors or gleams according to the stamina level of a cyclist. The aforementioned extended device may also be a smart phone **403** that may receive the information, process the information, visually illustrate the stamina level of a user in a range from 100% to 0% (optionally), and even upload the information to the Internet (optionally), such as social network or many types of applications.

[0056] FIG. **5** is a schematic illustration of the mapping concept between stamina level and RPE.

[0057] Referring to FIG. **5**, a mapping between the stamina level and rating of perceived exertion (RPE) is disclosed. In addition, the type of RPE may be Borg Rating of Perceived Exertion Scale. The stamina level is a measurement resulting from real-time exercise intensity. The stamina level recovers when fatigue level, blood lactate acid concentration (the lactate acid concentration in the blood stream) or real-time exercise loading decreases. On the other hand, the stamina level decreases when fatigue level, blood lactate acid concentration (the lactate acid concentration in the blood stream) or real-time exercise loading increases.

[0058] The stamina level can be presented within a certain range, such as 100% to 0%. In addition, the stamina level is at least partially related to the RPE scale linearly or non-linearly. For example, a RPE between 11 and 13 suggests that exercise intensity is being performed at a moderate level by the user of the exercise assistive device **100**. That is to say, the user may experience "light" muscle fatigue or breathing, and thus a RPE between 11 and 13 may correspond to a 100% stamina level.

[0059] On the other hand, a RPE between **15** and **17** suggests that exercise intensity is being performed at a much higher level by the user of the exercise assistive device **100**. That is to say, the user may experience "hard/heavy" muscle fatigue or breathing, and thus a RPE between 15 and 17 may correspond to a 0% stamina level.

[0060] To clearly illustrate in an example, the stamina level at 100% maps to a RPE at **12**, and the stamina level at 0% maps to a RPE at **16**, where the user can recovers from 0% back to 100% stamina level in a time period, such as 8 to 12 minutes preferably.

[0061] Moreover, in a perspective that takes heart signal as input of the exercise assistive device **100** as an example, the RPE scale is linearly or nonlinearly proportional to the heart rate, and thus the stamina level is also linearly or nonlinearly proportional to the heart rate. In another example, the stamina level of each user is normalized to a fixed range according to the maximum and minimum heart rate.

[0062] It should be noticed that although the aforementioned heart rate is disclosed for mapping and normalizing with the RPE scale and the stamina level, other physiological signal can also be implemented. Also, it should be noticed that the stamina level can be a negative value, and the negative value can be used for the automatic stamina category adjustment calculations, which will be further explained in the following paragraphs.

[0063] FIG. **6** a schematic illustration of the relationship between exemplary stamina categories and the fitness condition of a user.

[0064] Referring to FIG. **6**, the stamina category is classified into 10 levels, SC**1** to SC **10**. Different stamina category corresponds to different person's physical strength and endurance. For the user that rarely exercises, the stamina category may be initially set to category **1** (SC **1**), in the case of a professional athlete, the stamina category may be initially set to category **10** (SC**10**).

[0065] To further elaborate, the stamina category can be determined by the biological information input by the user, and can be modified according to the user's responses during an exercise, more specifically the stamina level change. For example, the exercise assistive device **100** can comprises a default database stored in the storage module **104** that determines the user's stamina category according to the user's biological information such as age, gender, weight, height and the user's exercise routine data (i.e. the information of the stamina category stored in the storage module after the last exercise of the user). The user's biological information or exercise routine data (i.e. the stored stamina category associated with the last exercise of the user) can be inputted by the user through the user interface **103**, or can be retrieved from other devices.

[0066] No matter what the stamina category is initially set to (i.e. based on biological information of the user or information of a stored stamina category in the exercise assistive device **100**), the stamina category for the user is automatically adjusted to a higher stamina category when the stamina level reaches certain thresholds while the user continues with the exercise without severe fatigue, and thus the stamina category adjustment automatically adapts to the user's progression in fitness level. Namely, as the user's physical condition improves, the stamina level maps to the appropriate RPE scale based on the current stamina category of the user, thus reflecting an accurate stamina level. The aforementioned stamina category adjustment can be regarded as an auto-RPE mechanism.

[0067] FIG. **7** is a schematic illustration of an exemplary stamina level indicator according to at least one embodiment of the present invention.

[0068] Referring to FIG. **7**, the stamina level is illustrated as a bar, with an upper boundary **204** indicating a 100% stamina level, and a lower boundary **202** indicating a 0% stamina level. Another graphical illustration, for example, a block **206** that is distinguishable from the bar by color, shape or style, represents the current stamina level of the user. The block **206** changes shape, color or style as the current stamina level of the user increases or decreases.

[0069] The upper boundary **204** may correspond to an anaerobic threshold, where lactate, more specifically, lactic acid, starts to accumulate in the blood stream due to exercise. The lower boundary **202** may correspond to a certain threshold level for lactic acid concentration, where the user feels exhausted. The threshold level of the lower boundary **202** can be different for each stamina category as each user's endurance to exercise intensity is different. Although the illustration of stamina level is implemented in the form of a bar shape, it is not limited to a bar, and can be implemented with various visual illustrations.

[0070] FIG. **8** is a schematic illustration of the correlation between lactic acid concentration and heart rate.

[0071] Referring to FIG. **8**, the anaerobic threshold for the abovementioned upper boundary **204** is defined as the exercise intensity at which the lactic acid concentration reaches a concentration of 2-6 mmol per liter (at rest it is around 1 mmol per liter).

[0072] For example, a 4 mmol per liter of lactate acid concentration is defined as 100% stamina level, and any concentration below 4 mmol per liter is considered as the user's operating at 100% stamina level.

[0073] The definition of the aforementioned anaerobic threshold may correlate with approximately 65% to 85% of the maximum heart rate. In addition, the maximum and minimum heart rate of the user is evaluated by age, gender, the rest state of the user, height and weight.

[0074] To replace the aforementioned definition of the anaerobic threshold, a certain gradient of the lactic acid concentration and heart rate correlation curve can be defined as 100% stamina level. For example, the 100% stamina level is a point with a gradient value on the curve just before steep incline, which also corresponds approximately to the lactic acid concentration between 2~6 mmol per liter.

[0075] It is well known in the art that a lactic acid concentration of 4 mmol per liter is considered as a threshold between aerobic exercise and anaerobic exercise. With aerobic exercise, oxygen is carried through the user's breath to the muscles giving them the energy needed to sustain the effort. With anaerobic exercise, the exercise intensity is high enough to trigger lactic acid formation, which causes discomfort and fatigue at sustained levels.

[0076] FIG. **9** is a schematic illustration of the changes in lactic acid concentration with respect to the exercise time period of a user and the mapping between lactic acid concentration and stamina level.

[0077] Referring to FIG. **9**, the stamina level of a user with particular stamina category is set to 100% when the lactate acid concentration is at a range of 2~6 mmol per liter. As the user continues with the exercise, the lactate acid concentration increases while the stamina level decreases. Once the lactate acid concentration reaches a threshold, i.e. at L1 lactic acid at t1 time, the user's stamina level reaches substantially 0%. Namely, the user's rate of perceived exertion scale is at approximately 15 to 17, the user may be suggested to choose to decrease the exercise intensity to remove the accumulated lactic acid and thus the stamina level recovers from 0% to 100% during t1 to t2 time frame. It should be noticed that the

recovery from 0% to 100% is not necessary, but a recovery from 0% to a certain percentage is better for a user to improve his/her performance during the exercise or competition.

[0078] Referring back to FIG. **7**, the value for the lower boundary **202** is determined based on the abovementioned t1 to t2 time for the lactate acid concentration to decreases to a predetermined value, for example less than 4 mmol per liter. Regardless of stamina category, the time for different user to fully recovered, for example from 0% to 100% stamina level, is similar, for example, approximately 8 to 12 minutes.

[0079] FIG. **10** is a flowchart of a method for estimating stamina level according to at least one embodiment of the present invention.

[0080] Referring to FIG. **10**, in step S**101**, the exercise assistive device **100** first sets the user's initial stamina category and stamina level based on the user's biological information or information of a stored stamina category in the exercise assistive device. The information of the stored stamina category mainly relates to the condition of the user during the last exercise.

[0081] In step S**102**, the physiological information of the user is obtained through the sensor module **101**. The physiological information P_t can be current heart rate, activity intensity, oxygen consumption, or any combination thereof.

[0082] In step S**103**, the stamina difference (ΔS) is calculated based on physiological information (P_t), the current stamina level (S_t), the initial stamina category and biological information.

[0083] Then, In step S**104**, the subsequent stamina level S_{t+1} is calculated by adding S_t and ΔS. In step S**105**, the user is notified when the stamina level decreases or increases to some specific thresholds. In step **106**, the initial stamina category can remains at the current level or adjusts to a higher level according to the S_{t+1} (i.e. from SC **3** to SC**4**).

[0084] It should be noticed that the exercise assistive device **100** updates information of the stored stamina category based on the adjustment of the initial stamina category. Also, It should be noticed that the steps S**102** to S**106** operates iteratively in the exercise assistive device **100**, and thus the auto-RPE mechanism remains active during the exercise or competition of the user.

[0085] FIG. **11** is a schematic illustration of the exemplary conditions for sending notifications to a user according to at least one embodiment of the present invention.

[0086] Referring to FIG. **11**, a notification can be triggered at a stamina level equal to or substantially equal to 0% or other predetermined values no more than 50% or no less than 50%. For example, a notification may be triggered when the stamina level drops to 60%, 30% or 0%. In addition, the notification may also be triggered when the stamina level recovers to 30% or 60%.

[0087] The notification may be any form that allows the users to become aware of the notifications, and examples of the notification can be voice, visual or vibrating notifications send out by the user interface **103** notifying the users that exercise intensity should be lower to reduce fatigue or other health related issues. In addition, different types of notifications can be configured for different stamina level. For example, 3 short vibration notifications can be used when the stamina level drops from 60% and then reaches 30% stamina level; a long vibration notification can be used when the stamina level drops from 30% and then reaches 0% stamina level; and 1 short vibration notification can be used when the stamina level rises from 0% and then reaches 30% stamina level or when the stamina level rises from 30% and then reaches 60% stamina level.

[0088] FIG. **12** is a flowchart of a method for adjusting stamina category according to at least one embodiment of the present invention.

[0089] Referring to FIG. **12**, in step S**201**, when the stamina level drops to a first threshold (or a predetermined value), for example, 0% stamina level, a notification is sent to the user. In step S**202**, if the user lowers the exercise intensity accordingly and the stamina level starts to recover to above the first threshold, the adjustment ends without modifying the current stamina category.

[0090] Then, in step S**203**, if the user ignores the notification in step S**202** and continues with the exercise until the stamina level reaches below a second threshold (or predetermined value), for example, minus 40% stamina level, the stamina category is adjusted to one higher level (i.e., from SC **3** to SC **4**).

[0091] In step S**204**, if the user ignores the notification in step S**202** and continues with exercise while the stamina level remains between the first and second predetermined value, for example, between 0% and minus 40% stamina level, for more than a first time period (a predetermined time), for example, 4 to 6 minutes, the stamina category is adjust to one higher level (i.e., from SC **3** to SC **4**). On the other hand, if the stamina level continuously remains between the first and second predetermined value for less than a first time period (a predetermined time), the adjustment ends without modifying the stamina category.

[0092] The stamina level increases or decreases according to each user's exercise intensity during a period of time. Different users with different stamina categories consume different amount of stamina levels during the same period of time. For example, the user with stamina category **3** (SC**3**) consumes stamina to 0% stamina level faster than the user with stamina category **5** (SC**5**) assumed the conditions are the same, because the user with SC **5** has more stamina than the user with SC **3**.

[0093] Thus, if the user's initial stamina category is not appropriate selected, the user may continue with the exercise without feeling severe fatigue after the stamina level reaches 0%, thereby causing sudden situations that fail the exercise or competition. So, the accuracy and effectiveness of the stamina level is based on the appropriate stamina category assigned to the user according to the user's fitness condition. The stamina category can be automatically adjusted to a higher level according to the disclosed adjustment method in FIG. **12**.

[0094] FIG. **13** is a schematic illustration of the exemplary conditions where stamina category can be automatically adjusted in FIG. **12**.

[0095] Referring to FIG. **13**, there are two examples of conditions where stamina category can be automatically adjusted. For the user with an initial stamina category of SC**3**, in a first condition, if the user's stamina level reaches below 0% and the user ignores the notification and continues with the exercise until the stamina level reaches below minus 40%, the user's stamina category is automatically adjusted to SC**4**.

[0096] Then, for the user with an initial stamina category of SC**4**, in a second condition, if the user's stamina level reaches below 0% and the user ignores the notification and continues with the exercise while the stamina level continuously

remains between 0% and minus 10% for more than a first time period (i.e. 5 minutes), the user's stamina category is automatically adjusted to SC**5**.

[0097] FIGS. **14**A and **14**B are schematic illustrations of relationship among heart rate, lactate acid concentration and RPE, and FIG. **14**C is the mapping between stamina level and RPE related to lactate acid concentration according to at least one embodiment of the present invention.

[0098] Referring to FIG. **14**A, the average heart rate of the user is positively correlated to the lactate acid concentration, which can be approximated with a linear regression model, a non-linear regression model, a piecewise function, other mathematical models or any combination thereof. Thus, the lactate acid concentration associated with the lactate acid accumulated in the blood stream is able to be estimated based on the heart rate of the user.

[0099] Referring to FIG. **14**B, since the heart rate is positively correlated to or is nearly proportional to the RPE scale, thus the lactate acid concentration is also positively correlated to the RPE scale. When the lactate acid concentration is low, the user experiences "light/easy" in sustaining the exercise effort, and when the lactate acid concentration is high, the user experiences "heavy/hard" or even "unsustainable" in sustaining the exercise effort.

[0100] Referring to FIG. **14**C, the stamina level is directly correlated to the lactate acid concentration and thus the RPE based on the understanding of FIGS. **14**A and **14**B. In addition, the stamina level can be represented as a bar-type stamina level indicator as shown in FIG. **7**. For example, when the lactate acid concentration reaches above a predetermined threshold in the left side of FIG. **14**C, where the stamina level is designated to be 100%, the stamina level indicator starts to decrease as the lactate acid concentration increases following the aforementioned linear or non-linear mathematical models, as illustrated by the white and black arrows in the right side of FIG. **14**C.

[0101] FIGS. **15**A and **15**B are schematic illustrations of relationship between the lactate acid concentration and exercise intensity or that between the lactate acid concentration and oxygen consumption.

[0102] Referring to FIGS. **15**A and **15**B, the lactate acid concentration associated with the lactate acid accumulated in the blood stream can be estimated based on other physiological signal other than heart rate. For example, the user's exercise intensity or oxygen consumption may be monitored with the sensor module **101**, and the aforementioned signals are positively correlated to the lactate acid concentration, which can be approximated with a linear regression model, a non-linear regression model, a piecewise function, other mathematical models, or any combination thereof.

[0103] The stamina level can be recorded over a period of time, for example, during an exercise, a race/competition, a challenge and so forth. In addition, the stamina level records can be uploaded to the Internet for further application such as some expressions or interactions in social network. To further elaborate, the stamina level records can be combined with various parameters to fulfill the user's demands for different applications, for example, the stamina level may be combined with at least one of heart rate, velocity, time, map, temperature, humidity, altitude, calorie consumption, exercising efficiency, estimated maximum exercise displacement, or any combination thereof. It should be noticed that the stamina level records may be expressed or exported in real-time or after a period of time.

[0104] FIG. **16** is schematic illustration of an exemplary application of estimating a user's maximum exercise distance using the user's stamina level and exercise speed.

[0105] To begin with, the users may refer back to the stamina level record histories to evaluate their stamina level changes over certain distance, speed, terrains, temperature or weather condition, and adjust their speed or route for the next exercise session. The users may also monitor their stamina level changes over the same course for several days or weeks to evaluate their progress in fitness levels.

[0106] Referring to FIG. **16**, the user's stamina level is correlated to the user's exercising speed over a certain period of time. For example, if a user has completed a 5 kilometer running exercise with 10% stamina level remaining, the exercise assistive device **100** can estimate the total running distance if the user is to used up all 100% stamina level for this exercise.

[0107] The additional distance associated with the remaining 10% stamina level may be estimated by multiplying the instant speed of the user with the stamina consumption time, and the aforementioned additional distance refers to an estimated distance by non-used stamina percentage, For example, if the additional distance associated with the remaining 10% stamina level is estimated to be 1 kilometer, the exercise assistive device **100** may notifies the user that a 100% stamina corresponds to a total of 6 kilometer running exercise.

[0108] Therefore, the estimated maximum exercise displacement can be used in designing training plans. For example, the user may have a training plan that has different distance targets in the first day and the consequent days. For example, the exercise assistive device **100** shows that the recorded distance exercised by the user is 10 kilometer in Day 1, but the estimated maximum exercise displacement is 11 kilometer since the estimated distance by non-used stamina percentage is 1 kilometer. In Day 3, the estimated maximum exercise displacement reaches to 22 km, and thus the user with the exercise assistive device **100** is ready to practice running at a distance of 22 kilometers in Day 4 under proper evaluation.

[0109] It should be noticed that different users with different stamina categories may compare their stamina level records with each other to adjust their exercise loading distribution since the stamina level of each user is normalized to a range of 0% to 100%. In another example, a gym coach can monitor the stamina level of all the members in a class and inform each individual to adjust his/her exercise loading accordingly.

[0110] FIG. **17** is schematic illustration of an exemplary application of outputting the user's stamina level in conjunction with a map.

[0111] Referring to FIG. **17**, the stamina level records can be utilized with GPS data and correlated with a map to evaluate the locations where most users have dramatic decrease in stamina level, for example, at the top of a steep hill.

[0112] The aforementioned information may be beneficial to water or food store owners to evaluate the locations to set up their stores. In addition, the aforementioned information may be combined with the information captured by some specific devices, such as a video recorder or a camera, and thus the user's video feeds along with the user's stamina level can be watched through the Internet.

[0113] FIG. **18** is schematic illustration of an exemplary application of estimating a user's calorie consumption by utilizing the user's stamina level.

[0114] Referring to FIG. **18**, the user's stamina level can be mapped to the user's calorie consumption with mathematical models. For example, if a user is exercising with a steady pace, the steady decrease in the stamina level corresponds to a constant calorie consumption. The total calorie consumption during the exercise may be estimated by multiplying this constant calorie consumption with the total time of this exercise. If the user is to increase the exercise loading at time t**1**, the calorie consumption becomes higher. However, the user may not be able to sustain with the exercise loading for a long time, and therefore the total calorie consumption may be lower after time t**1**. If the main goal for the user is to lose weight by maximizing caloric burns, the exercise assistive device is able to illustrate the correlation between the exercise loadings (i.e. the rate of decreasing in the stamina level) with the total calorie consumption, and sends notifications to the user suggesting the appropriate exercise loading.

[0115] FIG. **19** is a method to estimate stamina level based on physiological data according to one embodiment of the present invention.

[0116] In one embodiment of the present invention, stamina level is a combination of anaerobic energy level and aerobic energy level, wherein the stamina level is positively correlated to the anaerobic energy level and aerobic energy level that can be estimated by a linear regression model, a non-linear regression model, a piecewise function, other mathematical models or any combination thereof.

[0117] Referring to FIG. **19**, the following steps may be carried out to estimate stamina level based on physiological data:

[0118] S**301**: Receiving biological information from the user interface **103**;

[0119] S**303**: Measuring physiological data (P_t) by the sensor module **101**;

[0120] S**305**: Estimating anaerobic energy level in percentage by the processing module **102** based on the physiological data (P_t);

[0121] S**307**: Estimating aerobic energy level in percentage by the processing module **102** based on the physiological data (P_t) and the biological information;

[0122] S**309**: Estimating the stamina level in percentage (S_t%) based on the anaerobic energy level and the aerobic energy level in percentage by the processing module **102**.

[0123] In one embodiment of the present invention, the order of the step S**301**, S**303**, S**305** and S**307** are interchangeable as long as S**301** is before S**307** and S**303** is before both S**305** and S**307**.

[0124] In one embodiment of the present invention, the biological information may comprise at least one of the following: height, weight, age, and gender, etc.

[0125] In one embodiment of the present invention, the physiological data (P_t) may comprise at least one of the following: EKG signal, heart rate variability, pulse, heart rate, breathing pattern, body temperature, blood glucose, blood pressure, glycogen concentration, and oxygen concentration, etc. Each time the physiological data (P_t) is measured, the physiological data (P_t) may be either saved in the storage module **104** for later use or be sent to the processing module **102** for estimation of the anaerobic energy and the aerobic energy.

[0126] In one embodiment of the present invention, the stamina level (S_t%) may be mapped to RPE scale by the processing module **102** and outputted to the user by the user interface **103**.

[0127] In one embodiment of the present invention, the anaerobic energy level may be correlated to accumulation of lactate acid concentration, and the aerobic energy level may be correlated to extra calorie consumption. In this case, the stamina level (S_t%) may be estimated based on the accumulation of lactate acid concentration and the extra calorie consumption using a linear regression model, a non-linear regression model, a piecewise function, other mathematical models or any combination thereof.

[0128] FIG. **20** is a method to estimate anaerobic energy based on physiological data according to one embodiment of the present invention, wherein the method is an elaboration of the step S**305** in FIG. **19**.

[0129] Referring to FIG. **20**, the following steps may be carried out to estimate the anaerobic energy based on physiological data:

[0130] S**401**: Obtaining anaerobic estimation settings such as anaerobic energy category (anaerobic_c) and maximum anaerobic energy level (anaerobic_{max}) from the storage module **104**;

[0131] S**403**: Obtaining last recorded anaerobic energy level (anaerobic_{t-1}) from the storage module **104**;

[0132] S**405**: Obtaining physiological data (P_t) from the storage module **104**;

[0133] S**407**: Estimating anaerobic energy level (anaerobic) by the processing module **102** based on the physiological data (P_t), the anaerobic estimation settings and the last recorded anaerobic energy level (anaerobic_{t-1});

[0134] S**409**: Calculating anaerobic energy level in percentage (anaerobic_t%) by the processing module **102** using the anaerobic energy level (anaerobic_t), maximum anaerobic energy level (anaerobic_{max}) and a minimum anaerobic energy level (anaerobic_{min}).

[0135] In one embodiment of the present invention, the order of the step S**401**, S**403** and S**405** are interchangeable.

[0136] In one embodiment of the present invention, in step S**405**, the physiological data (P_t) may be measured by the sensor module **101** instead of obtained from the storage module **104**. Therefore, the method to estimate anaerobic energy may be carried out without relating to the method in FIG. **19**.

[0137] In one embodiment of the present invention, the anaerobic energy category (anaerobic_c) may be a lactate acid dilution rate or a lactate acid production rate.

[0138] In one embodiment of the present invention, the anaerobic energy level may be the accumulation of lactate acid concentration of the user, and the maximum anaerobic energy level (anaerobic_{max}) may be a maximum lactate acid concentration that a person can withstand theoretically, wherein the maximum lactate acid concentration may be varied by adjustment to anaerobic estimation settings. For example, a professional athlete may withstand higher lactate acid concentration than a casual runner. In addition, even the same person may withstand different lactate acid concentration. For example, a person stop exercising for a period of time, the person might be only able to withstand lower lactate acid concentration than before. Another example is that a person exercise regularly might be able to withstand higher lactate acid concentration than before. Therefore, the maximum anaerobic energy level (anaerobic_{max}) may be pre-configured with a certain value, and be adjusted each time the

exercise assistive device **100** estimates the stamina level (S_t%). Alternatively, the adjustment may also be carried out after the exercise assistive device **100** is turned off or on by the user. The method of adjustment to anaerobic estimation settings will be introduced later on.

[0139] In one embodiment of the present invention, the minimum anaerobic energy level ($anaerobic_{min}$) may be a lactate acid concentration that a user can sustain without increasing the user's lactate acid concentration dramatically while doing exercise. In this case, the minimum anaerobic energy level ($anaerobic_{min}$) may be set to 4 mmol/liter as shown in FIG. **8**. The minimum anaerobic energy level ($anaerobic_{min}$) may either be a constant pre-configured in the exercise assistive device **100** as a constant or be inputted by the user using the user interface **103**.

[0140] In one embodiment of the present invention, the last recorded anaerobic energy level ($anaerobic_{t-1}$) may be a value stored in the storage module **104** from the last estimation of anaerobic energy level, wherein $anaerobic_{t-1}$ may be equal to $anaerobic_{min}$ in the case of first time using the exercise assistive device **100** assuming no exercise has been done by the user.

[0141] FIG. **21** is a method to estimate aerobic energy based on physiological data according to one embodiment of the present invention, wherein the method is an elaboration of the step S**307** in FIG. **19**.

[0142] Referring to FIG. **21**, the following steps may be carried out to estimate the aerobic energy based on physiological data:

[0143] S**501**: Obtaining aerobic estimation settings such as aerobic energy category (aerobic_c) and last recorded aerobic energy level ($aerobic_{t-1}$) from the storage module **104**;

[0144] S**503**: Obtaining biological information from the storage module **104**;

[0145] S**505**: Obtaining physiological data (P_t) from the storage module **104**;

[0146] S**507**: Estimating aerobic energy level ($aerobic_t$) by the processing module **102** based on the physiological data (P_t), the biological information, the last recorded aerobic energy level ($aerobic_{t-1}$), and an aerobic energy constant (aerobic constant);

[0147] S**509**: Calculating aerobic energy level in percentage ($aerobic_t$%) of the aerobic energy category (aerobic_c) by the processing module **102** using the aerobic energy level ($aerobic_t$) and the aerobic energy category (aerobic_c).

[0148] In one embodiment of the present invention, the order of the step S**501**, S**503** and S**505** are interchangeable.

[0149] In one embodiment of the present invention, in step S**505**, the physiological data (P_t) may be measured by the sensor module **101** instead of obtained from the storage module **104**. Therefore, the method to estimate aerobic energy may be carried out without relating to the method in FIG. **19**.

[0150] In one embodiment of the present invention, the aerobic energy category (aerobic_c) may be an aerobic energy capacity of the user, wherein the aerobic_c may be a pre-configured value stored in the storage module **104**. The higher the aerobic_c, the higher the aerobic energy capacity which means the better the user's physical endurance. Thus, the aerobic energy level in percentage estimated in step S**509** may show the aerobic energy level left in percentage in comparison to the aerobic energy capacity.

[0151] In one embodiment of the present invention, the last recorded aerobic energy level ($aerobic_{t-1}$) may be stored in the storage module **104** from the last estimation of aerobic energy level, wherein $aerobic_{t-1}$ may be equal to aerobic_c in the case of first time using the exercise assistive device **100** assuming no exercise has been done by the user.

[0152] In one embodiment of the present invention, the aerobic energy constant (aerobic_constant) may be a rate of the aerobic energy consumed by an ordinary person while not exercising, wherein the rate may be a constant value pre-configured in the exercise assistive device **100**. It should be noticed that, the user may consume aerobic energy all the time even when the user is asleep. Therefore, the user's aerobic energy consumption is higher than the aerobic_constant when the user is exercising, and the change of the user's aerobic energy consumption is lower than the aerobic constant when the user is recovering. In the other word, the extra aerobic energy consumption is positive when the user is exercising and negative when the user is recovering. As mentioned before in FIG. **19**, the aerobic energy may be correlated to the extra calorie consumption, wherein the extra calorie consumption is the difference between the user's aerobic energy consumption and the aerobic_constant. Thus, aerobic_c minus the extra calorie consumption would be the estimated aerobic energy level (aerobic) in step S**507**.

[0153] FIG. **22** is the method to estimate stamina level (S_t%) based on physiological data as shown in FIG. **19** plus setting adjustments according to one embodiment of the present invention.

[0154] In one embodiment of the present invention, the method to estimate stamina level (S_t%) may be improved by comprising setting adjustments for anaerobic energy estimation and aerobic energy estimation, wherein the anaerobic estimation settings and aerobic estimation settings may be updated to improve the accuracy of estimating the stamina level (S_t%). Due to the fact that the anaerobic estimation settings and the aerobic estimation settings may not represent the actual physical condition of the user accurately each time the methods in FIG. **20**~**21** are carried out, the anaerobic estimation settings and the aerobic estimation settings may be updated after the estimation of anaerobic energy level and the estimation of aerobic energy level.

[0155] Referring to FIG. **22**, the following steps may be carried out after the method described in FIG. **19**:

[0156] S**311**: Adjusting the anaerobic estimation settings by the processing module **102** based on the anaerobic energy level ($anaerobic_t$);

[0157] S**313**: Adjusting the aerobic estimation settings by the processing module **102** based on the aerobic energy level ($aerobic_t$).

[0158] In one embodiment of the present invention, the step S**311** may be carried out any time after the step S**305**, and the step S**313** may be carried out any time after the step S**307**.

[0159] FIG. **23** is a method to adjust anaerobic estimation settings for the method to estimate stamina level (S_t%) according to one embodiment of the present invention, wherein the method is an elaboration of the step S**311** in FIG. **22**.

[0160] Referring to FIG. **23**, the following steps may be carried out to adjust anaerobic estimation settings for the method in FIG. **22**:

[0161] S**601**: Comparing whether the anaerobic energy level ($anaerobic_t$) is larger than or equal to a function of maximum anaerobic energy f ($anaerobic_{max}$) by the processing module **102**, if yes go to step S**603**, else go to step S**607**;

[0162] S**603**: Sending a notification to the user by the user interface **103**;

[0163] S**605**: Sensing whether the user reduces exercise intensity by the sensor module **101**, if yes go to step S**609**, else EXIT;

[0164] S**607**: Comparing whether the anaerobic energy level ($anaerobic_t$) is larger than or equal to an anaerobic threshold for X minutes by the processing module **102**, if yes go to step S**603**, else go to EXIT;

[0165] S**609**: Updating anaerobic estimation settings for t+1 by increasing the anaerobic energy category such as anaerobic_c+1, and the anaerobic energy level (anaerobic) will be used as new maximum anaerobic energy for next round estimation of anaerobic energy level.

[0166] In one embodiment of the present invention, the function of maximum anaerobic energy f ($anaerobic_{max}$) such as f ($anaerobic_{max}$)=2.5*$anaerobic_{max}$ may be pre-configured and saved in the storage module **104**. Alternatively, the function of maximum anaerobic energy f ($anaerobic_{max}$) may be replaced by a value configured by the user. For example the function may be replaced with a value such as 10 mmol/liter in the case when anaerobic energy level is lactate acid concentration. If the anaerobic energy level ($anaerobic_t$) estimated is 12 mmol/liter, then the exercise assistive device **100** will send a notification to the user.

[0167] In one embodiment of the present invention, the anaerobic threshold and the X minutes may be pre-configured and saved in the storage module **104**. Alternatively, the anaerobic threshold and the X minutes may be configured by the user. For example, the anaerobic threshold may be 6 mmol/liter in the case when anaerobic energy level is lactate acid concentration, and the X minutes may be 5 minutes. If the anaerobic energy level ($anaerobic_t$) estimated is 7 mmol/liter for 5 minutes, then a notification will be sent to the user.

[0168] In step S**609**, the anaerobic_c+1 means increasing the anaerobic_c by a pre-configure amount such as a fixed value or a percentage. For example, the anaerobic_c+1 may be increasing the lactate acid dilution rate or decreasing the lactate acid production rate by 1 mmol/liter or simply by 5%. And the new maximum anaerobic energy for next round estimation of anaerobic energy level may either be the anaerobic energy level (anaerobic) or a pre-configure increment from the maximum anaerobic energy (anaerobic.).

[0169] In one embodiment of the present invention, the notification in S**603** may be sent to the user in various forms such as visual, audio and vibration, etc.

[0170] In one embodiment of the present invention, in step S**605**, the sensor module **101** may sense whether the user reduces exercise intensity by the change of the physiological data (P_t). For example, the physiological data (P_t) sensed by the sensor module **101** is heart rate. The exercise assistive device **100** may determine the user reduces exercise intensity if the heart rate sensed at time t is lower than the previous recorded heart rate such as $P_t<P_{t-1}$.

[0171] The method to adjust anaerobic estimation settings may be applied as if the exercise assistive device **100** underestimates the user's physical strength and endurance. When the user fulfill the conditions in S**601** or S**607** and the exercise assistive device **100** does not sense any change in physiological data (P_t) which indicates reduction in exercise intensity, the exercise assistive device **100** adjusts the anaerobic estimation settings as shown in S**609**. In the case of anaerobic energy level being lactate acid concentration, the adjustments in S**609** not only increases the maximum anaerobic energy but also increases the lactate acid dilution rate or decreases the lactate acid production rate for using in the next round anaerobic energy estimation as anaerobic estimation settings.

[0172] FIG. **24** is a method to adjust aerobic estimation settings for the method to estimate stamina level (S_t%) according to one embodiment of the present invention, wherein the method is an elaboration of the step S**313** in FIG. **22**.

[0173] Referring to FIG. **24**, the following steps may be carried out to adjust aerobic estimation settings for the method in FIG. **24**:

[0174] S**701**: Comparing whether the aerobic energy level ($aerobic_t$) is less than or equal to a minimum aerobic energy threshold by the processing module **102**, if yes go to step S**703**, else EXIT;

[0175] S**703**: Sending a notification to the user by the user interface **103**;

[0176] S**705**: Sensing whether the user reduces exercise intensity by the sensor module **101**, if yes go to step S**707**, else EXIT;

[0177] S**707**: Adjusting aerobic estimation settings for t+1 by increasing the aerobic energy category such as aerobic_c+1, and the last recorded aerobic energy level ($aerobic_{t-1}$) will be updated as ($aerobic_{t-1}$)=f (aerobic_c+1, $aerobic_t$%).

[0178] In one embodiment of the present invention, the minimum aerobic energy threshold may be pre-configured and stored in the storage module **104**. For example, the minimum aerobic energy threshold may be 5% of the aerobic_c.

[0179] In one embodiment of the present invention, the notification in S**703** may be sent to the user in various forms such as visual, audio and vibration, etc.

[0180] In one embodiment of the present invention, in step S**705**, the sensor module **101** may sense whether the user reduces exercise intensity by the change of the physiological data (P_t). For example, the physiological data (P_t) sensed by the sensor module **101** is heart rate. The exercise assistive device **100** may determine the user reduces exercise intensity if the heart rate sensed at time t is lower than the previous recorded heart rate such as $P_t<P_{t-1}$.

[0181] In step S**707**, the aerobic_c+1 means increasing the aerobic_c by a pre-configure amount such as a fixed value or a percentage. For example, the aerobic_c+1 may be increasing the aerobic energy capacity by 1 or simply by 5% of aerobic_c as new aerobic energy capacity to be used in next round of aerobic energy estimation. And the last recorded aerobic energy level ($aerobic_{t-1}$) for next round estimation of aerobic energy level may be adjusted accordingly such as $aerobic_{t-1}$=the new aerobic energy capacity*$aerobic_t$%.

[0182] The method to adjust aerobic estimation settings may be applied as if the exercise assistive device **100** underestimates the user's physical strength and endurance. When the user fulfill the conditions in S**701** and the exercise assistive device **100** does not sense any change in physiological data (P_t) which indicates reduction in exercise intensity, the exercise assistive device **100** adjusts the aerobic estimation settings as shown in S**707**. In the case of aerobic energy level being correlated to extra calorie consumption, the adjustments in S**707** not only increases the aerobic energy capacity, which is aerobic_c, but also increases the estimated aerobic energy level accordingly, which is $aerobic_{t-1}$ for using in the next round aerobic energy estimation as aerobic estimation settings.

[0183] FIG. **25** is a method to estimate total maximum calorie consumption according to one embodiment of the present invention. As mentioned before, the aerobic energy is

consumed by the user all the time, therefore the aerobic energy consumption may only increase but never decrease. As the user using the exercise assistive device **100** to monitor stamina level (S_t%), each of the estimation of aerobic energy level ($aerobic_t$) may be recorded together with the stamina level (S_t%) and saved in the storage module **104**. Therefore $aerobic_{t-1}$ minus $aerobic_t$ will be an aerobic energy consumption difference (Δ aerobic). Each aerobic energy consumption difference (Δ aerobic) may be combined with the stamina level (S_t%) as a set of aerobic energy data (aerobic_data). As mentioned before, the aerobic energy level may be correlated to the extra calorie consumption, so the aerobic energy consumption difference (Δ aerobic) may be the difference of calorie consumption from t−1 to t. Thus, the actual calorie consumption at time t will be Δ aerobic+aerobic constant.

[0184] Referring to FIG. **25**, the following steps may be carried out by the processing module **102** and the storage module **104** to estimate the total maximum calorie consumption which the user may achieve:

[0185] S**801**: Obtaining N sets of aerobic energy data (aerobic_data) from the storage module **104**, wherein each set of aerobic energy data (aerobic_data) comprises the stamina level (St %) and the aerobic energy consumption difference (Δaerobic) from t−1 to t;

[0186] S**803**: Calculating total calorie consumption (calorie_total) as a sum of all the aerobic energy consumption difference (Δaerobic) each with an aerobic_constant;

[0187] S**805**: For each set of aerobic_data, comparing whether the stamina level (S_t%) is less than the stamina level (S_{t-1}%) from previous set of aerobic_data;

[0188] S**807**: Saving all the aerobic_data which fulfills the condition in S**805** in the storage module **104**;

[0189] S**809**: For each set of saved aerobic_data, calculating effective calorie consumption rate (eff_calorie_rate) by a function of aerobic energy consumption difference (Δaerobic), aerobic_constant, stamina level (S_t%), previous set of stamina level (S_{t-1}%) and a weighting variable;

[0190] S**811**: Estimating the total maximum calorie consumption by Σ(eff_calorie_rate)*latest recorded stamina level (S_t%)+calorie total, wherein the sum of the effective calorie consumption rate (eff_calorie_rate) for each set of saved aerobic_data from S**809** is multiplied to the latest recorded stamina level (S_t%) of N set of aerobic_data, and adding the total calorie consumption (calorie_total) to the result of multiplication.

[0191] In one embodiment of the present invention, the step S**803** may be carried out any time in between S**801** and S**811**.

[0192] The method to estimate total maximum calorie consumption may be applied as the user would like to know how much calorie in total can be burned before the stamina level (S_t%) reaches zero.

[0193] In one embodiment of the present invention, in step S**803**, the total calorie consumption (calorie_total) may be outputted by the user interface **103**, so the user may be able to keep track of the calorie consumed so far. In addition, the calorie_total may be subtracted from the total maximum calorie consumption and outputted to the user, so the user may know how much more calorie may be consumed for the usage of remaining stamina which is the latest recorded stamina level.

[0194] In one embodiment of the present invention, the calorie_total and/or the total maximum calorie consumption may be outputted to the user in various forms such as visual, audio and vibration, etc.

[0195] In one embodiment of the present invention, the weighting variable is a specific to each set of saved aerobic_data. Assuming each percent of stamina level (S_t%) consumption requires equal amount of time, the weighting variable may represent the contribution of aerobic energy consumption in terms of each percent of stamina level (S_t%) consumed by the user. For a particular set of saved aerobic_data, the contribution of calorie burning may be a ratio between an aerobic energy consumption difference (Δaerobic) from the particular set of saved aerobic_data to the sum of aerobic energy consumption difference (Δaerobic) from all the saved aerobic_data.

[0196] In one embodiment of the present invention, the effective calorie consumption rate (eff_calorie_rate) is the rate of calorie consumption when stamina is actually consumed. In the other word, eff_calorie_rate is how much calorie could be burned by the user when each percent of stamina is consumed by the user.

[0197] FIG. **26** is a method to estimate total maximum exercise displacement according to one embodiment of the present invention. As the user using the exercise assistive device **100** to monitor stamina level (S_t%), each of the stamina level (S_t%) may be recorded together with a displacement value (Δ Dis) sensed by an exercise sensor (not shown) in the sensor module **101** from t−1 to t and saved in the storage module **104**. The exercise sensor may be comprised by the sensor module **101**, and the exercise sensor may be one of the following: gyroscope, an accelerometer, a step counter, a cadence monitor, a speedometer, a GPS receiver, or a power meter, wherein the exercise sensor may also directly or indirectly provide real-time displacement information such as speed, elevation, inclination, etc. Each displacement value (Δ Dis) may be combined with the stamina level (S_t%) as a set of exercise data (ex_data). The exercise sensor may measure the user's exercising power, cadence (ex: paddling frequency, step frequency, etc), displacement information, etc.

[0198] Referring to FIG. **26**, the following steps may be carried out by the processing module **102** and the storage module **104** to estimate the total maximum exercise displacement which the user may achieve:

[0199] S**901**: Obtaining N sets of exercise data (ex_data) from the storage module **104**, wherein each set of exercise data (ex_data) comprises the stamina level (St %) and the displacement value (Δ Dis) from t−1 to t;

[0200] S**903**: Calculating total total exercise displacement (dis_total) as a sum of all the displacement value (Δ Dis);

[0201] S**905**: For each set of ex_data, comparing whether the stamina level (S_t%) is less than the stamina level (S_{t-1}%) from previous set of ex_data;

[0202] S**907**: Saving all the ex_data which fulfills the condition in S**905** in the storage module **104**;

[0203] S**909**: For each set of saved ex_data, calculating effective exercise displacement rate (eff_dis_rate) by a function of displacement value (ΔDis), stamina level (S_t%), previous set of stamina level (S_{t-1}%) and a weighting variable;

[0204] S**911**: Estimating the total maximum exercise displacement by Σ(eff_dis_rate)*latest recorded stamina level (S_t%)+dis_total, wherein the sum of the effective exercise displacement rate (eff_dis_rate) for each set of saved ex_data from S**909** is multiplied to the latest recorded stamina level (S_t%) of N set of ex_data, and adding the total exercise displacement (dis_total) to the result of multiplication.

[0205] In one embodiment of the present invention, the step S**903** may be carried out any time between S**901** and S**911**.

[0206] In one embodiment of the present invention, in step S**903**, the total exercise displacement (dis_total) may be outputted by the user interface **103**, so the user may be able to keep track of the displacement made so far. For example, distance of running, height of climbing, etc. In addition, the dis_total may be subtracted from the total maximum exercise displacement and outputted to the user, so the user may know how much more displacement may be made for the usage of remaining stamina which is the latest recorded stamina level. This is particularly useful to the user as the user may adjust exercise intensity to achieve a desire exercise displacement. For example, the user would like to cycle for 10 km. When the total maximum exercise displacement is estimated by the exercise assistive device **100** as 8 km, a notification may be sent to the user by the user interface **103**. Therefore, the user may slow down to lower the rate of stamina consumption, and the user may be able to cycle more than 8 km with the remaining stamina. If the total maximum exercise displacement is estimated by the exercise assistive device **100** as 12 km, the user may increase cycling speed and still be able to achieve 10 km. In addition, the exercise assistive device **100** may calculate the rate of stamina level consumed by the user against the cycling speed of the user to suggest how fast the user may cycle and still achieve the 10 km goal. Furthermore, the exercise assistive device **100** may even calculate how many times of attack (To quickly accelerate while riding in a pack, or in smaller numbers, with a view to create a gap between the user and other cyclers) the user may make and still achieve the 10 km goal. This could be done by pre-configuring an amount of maximum exercise displacement the user needs to sacrifice to make an attack. For example, the user may use 3 km of maximum exercise displacement for each attack. When the maximum exercise displacement estimated for the user is 17 km, the user may make two more attacks and still achieve the 10 km goal without completely consuming all the stamina the user has. Alternatively, the exercise assistive device **100** may be configured to estimate the rate of stamina consumption or decrease of maximum exercise displacement while the user making an attack by tracking user's heart rate, motion, or any other exercising factors which varies with the user's exercising intensity. After calculation by the processing module **102**, the available attacks may be outputted to the user by the user interface **103**. Thus the user may manage his/her exercising activities with ease especially when the user does not intend to remain a constant exercising intensity.

[0207] In one embodiment of the present invention, the dis_total and/or the total maximum exercise displacement may be outputted to the user in various forms such as visual, audio and vibration, etc.

[0208] In one embodiment of the present invention, the weighting variable is a specific to each set of saved ex_data. Assuming each percent of stamina level (S_t%) consumption requires equal amount of time, the weighting variable may represent the contribution of displacement in terms of each percent of stamina level (S_t%) consumed by the user. For a particular set of saved ex_data, the contribution of displacement may be a ratio between a displacement value (ΔDis) from the particular set of saved ex_data to the sum of displacement value (ΔDis) from all the saved ex_data.

[0209] In one embodiment of the present invention, effective exercise displacement rate (eff_dis_rate) is the rate of displacement made by the user when stamina is actually consumed. In the other word, eff_dis_rate is how much displacement could be made by the user when each percent of stamina is consumed by the user.

[0210] In one embodiment of the present invention, the sensor module **101** may measure the user's exercising information such as power, cadence, speed, elevation, inclination, body composition, etc. The measurement from the sensor module **101** may be correlated with the stamina level obtained using method in FIG. **10** and FIG. **19**. For example, the measurement of exercising power may be used to estimate the user's maximum power the user exerted during/after exercise via the output unit. The measurement of cadence may be used to determine whether the user is exercising efficiently or simply to provide a most efficient exercising cadence to the user via the output unit (ex: 60 steps/min for a running exercising, 60 pedals/min for a cycler, etc). The displacement information may be used to estimate how the user's body react with change of different speed, elevation, inclination, etc. Therefore, the processing module **102** may use the measurement of the exercise information to estimate the user's body endurance and/or power exertion. Furthermore, the body endurance and/or power exertion of the user may be taken into account to further adjusting the anaerobic estimation settings in FIG. **23** and/or aerobic estimation settings in FIG. **24**. The body composition may be used to estimate the user's body energy density. For example, correlating the user's muscle density to anaerobic energy level, and/or aerobic energy level, and/or stamina, etc.

[0211] Previous descriptions are only embodiments of the present invention and are not intended to limit the scope of the present invention. Many variations and modifications according to the claims and specification of the disclosure are still within the scope of the claimed invention. In addition, each of the embodiments and claims does not have to achieve all the advantages or characteristics disclosed. Moreover, the abstract and the title only serve to facilitate searching patent documents and are not intended in any way to limit the scope of the claimed invention.

What is claimed is:

1. A stamina monitoring device, comprising:

a sensor module to sense a physiological signal;

an user interface to receive a biological information;

a storage to store the biological information and at least one mathematical model;

a processing module to execute the at least one mathematical model to do the following:

estimating an anaerobic energy and an aerobic energy based on the physiological signal and the biological information;

combining the anaerobic energy and the aerobic energy into a stamina level.

2. The device of claim **1**, wherein the anaerobic energy is correlated to accumulation of lactate acid concentration.

3. The device of claim **1**, wherein the aerobic energy is correlated to calorie consumption.

4. The device of claim **1**, wherein the biological information comprises at least one of body dimension information such as height, weight, age, gender.

5. The device of claim **1**, wherein the sensor module senses at least one of the following: EKG signal, heart rate variability, pulse, heart rate, breathing pattern, body temperature, blood glucose, blood pressure, glycogen concentration, oxygen concentration, body composition, power, cadence, speed, elevation, and inclination.

6. The device of claim **1**, wherein the sensor module comprises an EKG sensor that senses heart rate.

7. The device of claim **1**, wherein the user interface comprises at least one output such as a display, a vibrating component, or a speaker.

8. The device of claim **1** further comprising:

a strap, wherein the stamina monitoring device is fixed directly or indirectly on a user's skin by the strap.

9. The device of claim **8**, wherein the stamina monitoring device is fixed at the user's forehead, wrist, leg or arm by the strap.

10. The device of claim **1**, wherein the stamina level is outputted to be in conjunction with at least one parameter such as heart rate, velocity, time, map, temperature, humidity, altitude, calorie consumption, exercising efficiency, body composition, power, cadence, speed, elevation, inclination, BMI or estimated maximum exercise displacement.

11. The device of claim **1**, wherein the user interface outputs a notification when the anaerobic energy and/or the aerobic energy reaches a threshold.

12. The device of claim **11**, wherein the notification is vibrating notification, voice notification, or visual notification.

13. The device of claim **1**, wherein the stamina level is further mapped to a RPE scale and outputted by the user interface.

14. The device of claim **1**, wherein the processing module is further configured to estimate a maximum calorie consumption based on the stamina level and the aerobic energy.

15. The device of claim **1**, further comprising:

an exercise sensor to directly or indirectly provide real-time displacement information.

16. The device of claim **15**, wherein the processing module is further configured to estimate a maximum exercising displacement based on the stamina level and the displacement information.

17. The device of claim **16**, wherein the user interface outputs available attacks which is calculated by the processing module based on the stamina level or maximum exercising displacement.

18. A stamina monitoring method, comprising:

sensing a physiological signal by a sensor module;

receiving a biological information from a user interface;

estimating an anaerobic energy and an aerobic energy based on the physiological signal and the biological information by a processing module using at least one mathematical model stored in a storage module;

estimating a stamina level based on the anaerobic energy and the aerobic energy;

outputting the stamina level by at least one output unit.

19. The method of claim **18**, wherein the anaerobic energy is correlated to accumulation of lactate acid concentration.

20. The method of claim **18**, wherein the aerobic energy is correlated to calorie consumption.

21. The method of claim **18**, wherein the biological information comprises at least one of body dimension information such as height, weight, age, gender.

22. The method of claim **18**, wherein the sensor module senses at least one of the following: EKG signal, heart rate variability, pulse, heart rate, breathing pattern, body temperature, blood glucose, blood pressure, glycogen concentration, oxygen concentration, body composition, power, cadence, speed, elevation, and inclination.

23. The method of claim **18**, wherein the sensor module comprises an EKG sensor that senses heart rate.

24. The method of claim **18**, wherein the at least one output is a display, a vibrating component, or a speaker.

25. The method of claim **18**, wherein the stamina level is outputted to be in conjunction with at least one parameter such as heart rate, velocity, time, map, temperature, humidity, altitude, calorie consumption, exercising efficiency, body composition, power, cadence, speed, elevation, inclination, BMI or estimated maximum exercise displacement.

26. The method of claim **18**, wherein the at least one output unit outputs a notification when the anaerobic energy and/or the aerobic energy reaches a threshold.

27. The method of claim **26**, wherein the notification is vibrating notification, voice notification, or visual notification.

28. The method of claim **18**, further comprising:

mapping the stamina level to a RPE scale by the processing module;

outputting the RPE scale by the at least one output unit.

29. The method of claim **18**, further comprising:

estimating a maximum calorie consumption by the processing module based on the stamina level and the aerobic energy.

30. The method of claim **18**, further comprising:

obtaining a real-time displacement information directly or indirectly from an exercise sensor.

31. The method of claim **30**, further comprising:

estimating a maximum exercising displacement by the processing module based on the stamina level and the displacement information.

32. The method of claim **31**, further comprising:

Outputting available attacks by the user interface, wherein the available attacks is calculated by the processing module based on the stamina level or maximum exercising displacement.

33. A stamina monitoring device, comprising:

a sensor module to sense a physiological signal;

an user interface to receive a biological information;

a storage to store the biological information and at least one mathematical model;

a processing module to execute the at least one mathematical model to do the following:

estimating a stamina level based on the physiological signal and the biological information;

estimating a exercise assistive information based on the stamina level;

sending the stamina level to the user interface which comprises an output unit. outputting the stamina level by the user interface.

34. The device of claim **33**, wherein the processing module is further configured to estimate a maximum calorie consumption based on the stamina level and an aerobic energy, and the aerobic energy is estimated based on the physiological signal and the biological information.

35. The device of claim **33**, further comprising an exercise sensor which directly or indirectly provides a real-time displacement information, and the processing module is further configured to estimate a maximum exercise displacement based on the stamina level and the displacement information.

36. The device of claim **35**, wherein the user interface outputs available attacks which is calculated by the processing module based on the stamina level or maximum exercising displacement.

37. The device of claim **35**, wherein the storage further storing a displacement target, and a notification is output to the user when the maximum exercise displacement is lower than the displacement target.

38. The device of claim **33**, wherein the user interface comprises at least one output such as a display, a vibrating component, or a speaker.

39. The device of claim **33**, wherein the biological information comprises at least one of body dimension information such as height, weight, age, gender.

40. The device of claim **33**, wherein the sensor module comprises an EKG sensor that senses heart rate.

41. The device of claim **33**, wherein the stamina level is outputted to be in conjunction with at least one parameter such as heart rate, velocity, time, map, temperature, humidity, altitude, calorie consumption, exercising efficiency, body composition, power, cadence, speed, elevation, inclination, BMI or estimated maximum exercise displacement.

42. The device of claim **33**, wherein the sensor module senses at least one of the following: EKG signal, heart rate variability, pulse, heart rate, breathing pattern, body temperature, blood glucose, blood pressure, glycogen concentration, oxygen concentration, body composition, power, cadence, speed, elevation, and inclination.

* * * * *