

(19)



Europäisches Patentamt
European Patent Office
Office européen des brevets



(11) Publication number:

0 230 996 B1

(12)

EUROPEAN PATENT SPECIFICATION(45) Date of publication of patent specification: **07.01.93** (51) Int. Cl.⁵: **A61M 25/00, A61M 29/00**(21) Application number: **87100942.9**(22) Date of filing: **26.01.87**

Divisional application 90115824.6 filed on
26/01/87.

(54) **Pressure-Controlled Intermittent Coronary Sinus Occlusion.**(30) Priority: **31.01.86 US 824721**(43) Date of publication of application:
05.08.87 Bulletin 87/32(45) Publication of the grant of the patent:
07.01.93 Bulletin 93/01(84) Designated Contracting States:
AT DE FR GB IT

(56) References cited:

EP-A- 0 079 086	FR-A- 2 502 499
US-A- 4 069 815	US-A- 4 299 226
US-A- 4 456 000	US-A- 4 601 706

(73) Proprietor: **Mohl, Werner, M.D.**
Endemangasse 6-18/2/35 Flat 235
A-1238 Vienna(AT)

Proprietor: **MANSFIELD SCIENTIFIC, INC.**
135 Forbes Boulevard
Mansfield Massachusetts 02048(US)

(72) Inventor: **Mohl, Werner**
Endemangasse 6-18/2/35, App.235
A-1238 Wien(AT)
Inventor: **Tolkoff, Marc Joshua**
39 Jordan Road
Brookline, Massachusetts 02146(US)

(74) Representative: **Heidrich, Udo, Dr. jur.,**
Dipl.-Phys.
Rechtsanwalt & Patentanwalt Dipl.-Phys. Dr.
jur. U. HEIDRICH Franziskanerstrasse 30
W-8000 München 80(DE)

EP 0 230 996 B1

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid (Art. 99(1) European patent convention).

Description

Background of the Invention

5 This invention relates to intermittent periodic occlusion of the coronary sinus in order to accomplish retroperfusion, i.e., repeatedly temporarily blocking the major vein which collects blood from the heart muscle in order to cause venous blood to flow back from the normal contracting myocardium to reach ischemic portions of the heart muscle.

Arterial blood which feeds the heart muscle is able to pass through and nourish healthy heart tissue, but
10 has difficulty in reaching the ischemic tissue. This reduces the delivery of nutrients to, and the carrying away of the waste products of metabolism (metabolites) from, the ischemic tissue.

It has been proposed to reach the ischemic tissue by causing blood to flow in a reverse direction from the coronary sinus back through the coronary venous system. Such retroperfusion has been attempted by feeding blood into the coronary sinus from another source, either by permanently connecting an artery to
15 the coronary sinus or by temporarily inserting into the sinus a catheter supplied with blood which has been taken from a remote artery and passed through a blood pump outside the patient's body.

Another proposed technique for retroperfusion uses an inflatable balloon held on the end of a catheter to intermittently occlude the coronary sinus. Blood pressure in the sinus then rises as the heart beats so that blood received in the sinus through the healthy tissue of the heart muscle is forced back into the
20 ischemic tissue. In such intermittent coronary sinus occlusion, the balloon end of the catheter is inserted percutaneously or intraoperatively. The other end of the catheter is supplied with gas or liquid by a pump which can be controlled to cause the balloon to inflate and deflate cyclically, for example at a rate synchronized with the heart pulse rate, or on the basis of pressure.

Summary of the Invention

In general, the invention concerns an improvement that leads to making intermittent occlusion of a coronary sinus a successful and useful technique. The invention employs means for occluding the sinus, a pressure transducer for sensing the fluid pressure within the sinus and providing corresponding fluid
30 pressure signals, and a controller responsive to the transducer and arranged to provide trigger signals to the occluding means to trigger an occlusion and to interrupt the occlusion. The controller is also arranged to calculate the optimum deflation time between occlusions utilizing data obtained from coronary sinus blood pressure and/or flow.

The invention is found to provide sufficient retroperfusion flow to effectively wash toxic metabolites and edema from the ischemic tissue while minimizing damage to healthy tissue. Heart contractability can be
35 improved. The invention may be used in bolstering heart function during heart surgery and catheterization, especially in combination with conventional pharmacological agents.

It is realized, for instance, that the rate of rise of the curve of maxima usually indicates the contractility of the heart, the steeper the rate of rise, the more contractile.

40 The invention features triggering the initiation of the next occlusion at a time based on fluid pressure signals taken from the sinus during occlusion. As a result, the start of the next occlusion can be delayed until the time when peak reactive hyperemia has occurred.

In preferred embodiments, the timing of the initiation of the next occlusion is based on a combination of parameters derived from successive pressure maxima and pressure minima. The pressure maxima and
45 minima are fitted to exponential curves. The parameters include heart rate, the asymptotic plateaus of the exponential curves, and the time constants of the exponential curves.

In preferred embodiments, the estimation is based on local maxima and local minima of the fluid pressure signals.

Other advantages and features of the invention will be apparent from the following description of the
50 preferred embodiment and from the claims.

Description of the Preferred Embodiment

We first briefly describe the drawings.

Drawings

Fig. 1 is a diagrammatic view of a heart with intermittent coronary sinus occlusion apparatus.

Fig. 1A is a flowchart associated with the operation of the intermittent coronary sinus occlusion apparatus of Fig. 1.

Fig. 2A is an isometric view, broken away, of the distal end of the catheter of Fig. 1.

Fig. 2B is an isometric view of an alternative embodiment of Fig. 2A.

5 Fig. 3 is a block diagram of the controller of Fig. 1.

Figs. 4, 7 is a representational graph of changes of coronary sinus pressure with time.

Fig. 5 is a representational graph of changes of coronary sinus pressure with time showing the interrupt period.

Fig. 6 is a representational graph of changes of coronary blood flow rate with time.

10 Figs. 8 through 16 are graphs of normalized data points of various parameters versus the time of peak reactive hyperemia (Tp).

Fig. 17 is a graph of data points of predicted Tp versus measured Tp.

Fig. 18 is a flow chart of a procedure for triggering start of occlusion.

Fig. 19 is a block diagram of apparatus for performing the procedure of Fig. 18.

15 Figs. 20, 21 show additional steps and apparatus for analyzing the area of heart tissue at risk (AR) and the size of infarcted tissue (IS).

Structure

20 Referring to Fig. 1, intermittent coronary sinus occlusion apparatus 10 includes multi-lumen catheter 12 having its distal end 14 inserted into the coronary sinus of heart 16 via the right atrium. The proximal end 18 of catheter 12 has a balloon inflation lumen 20 connected to pump 22. A second lumen 24, coaxial with lumen 20, and wires 42 are connected to controller 28 which contains circuitry for delivering control signals over line 30 to trigger the starting and stopping of pump 22.

25 Referring to Fig. 2A, at distal end 14 of catheter 12, lumen 20 communicates with inflatable balloon 34 via proximal aperture 32. Lumen 24 passes through the balloon and exits distally via aperture 36. Lumen 20 and balloon 34 contain gas delivered from pump 22.

The distal end of lumen 24 is open to the coronary sinus and holds a stationary column of isotonic heparinized saline solution with or without pharmacological agents. Changes in blood pressure in the sinus are transmitted to the proximal end of lumen 24, and are sensed at controller 28. (Pressure may also be sensed by fiberoptic elements residing in lumen 24.)

30 The distal end of lumen 24 is surrounded by an ultrasonic transducer 40 for sensing the flow of fluid in the sinus and delivering corresponding flow signals. Transducer 40 is connected to wires 42.

Referring to Fig. 2B, the catheter may include a third lumen 65 for carrying cardioplegic and thrombolytic (or other pharmacological) agents into the sinus for retroperfusion to the ischemic tissue. The delivery of the agents through lumen 65 may begin as soon as the balloon is inflated or may be triggered based on the trend of the local maxima during infusion.

Referring to Fig. 3, controller 28 has a pressure transducer (or other pressure sensor) 50 attached to the proximal end of lumen 24 (for sensing the blood pressure in the coronary sinus and providing corresponding fluid pressure signals). Transducer 50 is connected through amplifier 52 and interface 54 (which includes an A-to-D converter) to processor 56. Processor 56 has microprocessor 58, RAM 60, and ROM 62 (which holds the program for processor 56). Processor 56 also has an input connected to flow analyzer 63, which includes Doppler circuitry for driving transducer 40 to vibrate ultrasonically and for detecting the Doppler shift of the resulting vibrations bouncing back to transducer 40 from blood flowing in the coronary sinus, thus to give an indication of flow velocity.

45 The output of processor 56 is connected through interface 64 (including a D-to-A converter) to line 30 which carries trigger signals to turn on and shut off pump 22.

Processor 56 is also connected to real time display 83 for displaying the sinus pressure over time for observation of the successive local pressure maxima as an indication of the state of health of the heart tissue, e.g., its contractility.

Operation

55 The distal end of catheter 12 is inserted, percutaneously or intraoperatively, into the coronary sinus. In operation, controller 56 issues a trigger signal through interface 64 and over line 30 to turn on pump 22. Gas is pumped into lumen 20 causing balloon 34 to inflate within the coronary sinus, blocking blood flow out of the sinus. Blood continues to flow into the sinus and retroperfuses back into the ischemic tissue.

Referring to Fig. 4, with the sinus blocked, systolic pressure 67 varies cyclically with the heart pulse

rate. For each heartbeat, pressure rises to a local maximum (e.g., 68), and then falls near to a base level, after which the cycle is repeated. The successive local maxima lie on a curve 70 which rises toward asymptotic plateau 72, e.g., 80 mm of Hg. With higher pressures, the retroperfused blood reaches more ischemic tissue, but the peak pressure for successive heartbeats rises approximately exponentially and we realize, accordingly, that the amount of additional tissue being reached in each successive heartbeat is not as great as in prior heartbeats. We also realize that a benefit of retroperfusion, the washout of metabolites, is dependent upon attainment of pressure, but not prolongation of pressure, at the ischemic site, while continuing to occlude the sinus once plateau 72 is reached could damage healthy heart tissue. According to the invention, controller 28 is arranged to terminate the occlusion on the basis of the predicted plateau, more specifically when the sinus pressure reaches a predetermined level (e.g., 94% of the predicted plateau, or a calculated value thereof (i.e., X% (70-98%) of predicted plateau and n heart cycles or X% and n seconds)).

Referring to Fig. 1A, processor 56 samples (80) the output of interface 54 many times in each heart pulse cycle (e.g., at a rate of at least 2500 Hz) and stores the pressure samples in RAM 60. It then compares successive samples to determine the local maximum pressure for each heartbeat. Each local maximum is sorted (84) in RAM 60. Processor 56 then performs a curve fitting route (86), e.g., by regression analysis, in which the available local maxima are fitted to an exponential function of the form $P = A - Be^{-ct}$, where P is the pressure as a function of time, A is the plateau pressure, t is time and B the difference between the plateau and the base-line pressures, and c is the slope constant. From the resulting function, processor 56 estimates (88) the level that plateau 72 would have and calculates 94% of that plateau (89). Finally, processor 56 compares (90) each newly calculated local maximum with the 94% value and when a local maximum first reaches at least that 94% value (e.g., at time 92 in Fig. 4), processor 56 triggers the pump to evacuate, or provide negative pressure to, lumen 20, thus interrupting the inflation of balloon 34 before the plateau is reached.

The local maxima can also be displayed in real time 85 in order to permit analysis of the condition of the heart tissue, and can be used as the basis for triggering an infusion of pharmacological agents 87.

Referring to Fig. 5, after pump cutoff, the curve of the local pressure maxima falls off to its baseline level until, at time 100, the pump is turned on again and the cycle repeats.

During occlusion, the heart muscle vascular system is subjected to back pressure and accordingly is resiliently expanded. When pump 22 is shut off and the back pressure is relieved, the heart muscle resiliently relaxes by contracting, thus forcing blood, toxic metabolites, and water from the ischemic tissue into the coronary sinus and other drainage systems, i.e., thebesian vessels and lymph vessels.

How long the pump operation should be interrupted before initiating a subsequent occlusion depends on balancing the effect of maximum outwashing obtained by a longer interruption period with the effects of additional retroperfusion obtained by a shorter interruption period.

The time to begin occlusion (i.e., the time T, of peak reactive hyperemia corresponding to point 102 on Fig. 6) can be determined by measuring certain characteristics of the coronary sinus pressure curve, CSP-(t), during the previous period of occlusion. Referring to Fig. 7, a typical plot of coronary sinus pressure against time, beginning at the onset of occlusion (T_o), exhibits a series of systolic pressure peaks interleaved with a series of diastolic valleys 112. The pulse period 114 of the heartbeat is represented by the time between successive peaks or between successive valleys. The systolic pressure peaks can be fitted to an exponential curve 116 of the form

$$P_s(t) = (A_s(1 - 3^{-t/T_s}))$$

where A_s is the asymptotic plateau of pressure maxima and T_s is the time to reach the plateau. Similarly the diastolic pressure valleys can be fitted to an exponential curve 118 of the form

$$P_d(t) = A_d(1 - 3^{-t/T_d})$$

where A_d is the asymptotic plateau of diastolic pressure valleys, and T_d is the time to reach the plateau. T_p represents the period between the termination of occlusion and the peak reactive hyperemia. T_p can be estimated as

$$\begin{aligned}
T_p = & - 1.60 T_s + 0.82 T_d + 3.70 T_s/T_d \\
& - 3.50 T_d/T_s - 0.260 A_s + 1.60 A_d \\
& - 0.510 A_s/A_d - 53.0 A_d/A_s \\
& - 0.0081 HR + 18.0 RRI + 0.65 A_s/RRI \\
& - 0.38 A_d/RRI - 0.10 T_s/RRI + 0.15 T_d/RRI + 7.7
\end{aligned}$$

where HR is the heart rate, i.e., the reciprocal of the pulse period, and RRI is the recipitrol of the heart rate.

Figs. 8-16 show the experimentally determined relationships between normalized T_p and normalized values of HR, T_s , T_s/T_d , T_d , T_d/T_s , A_s , A_d/A_s , A_d , and A_s/A_d in experiments with 12 dogs. The correlations represented by this data are

T_s	$= -.21$	$T_p + .49;$	$r = .11$
T_d	$= -.39$	$T_p + 5.0;$	$r = .21$
T_s/T_d	$= 0.63$	$T_p + .98;$	$r = .14$
T_d/T_s	$= -.060$	$T_p + 1.1;$	$r = .18$
A_s	$= 0.46$	$T_p + .62;$	$r = .003$
A_d	$= -.041$	$T_p + .14;$	$r = .008$
A_s/A_d	$= -.074$	$T_p + 5.1;$	$r = .046$
A_d/A_s	$= .0002$	$T_p + .22;$	$r = .002$
HR	$= -.419$	$T_p + 127;$	$r = .21$

Fig. 17 shows the correlation between predicted $\hat{T}_p$ and measured T_p in seconds. A linear regression between $\hat{T}_p$ and T_p yields

$$\hat{T}_p = 0.92 T_p + 0.00; r = 0.634 (P 0.001)$$

Measured T_p had a mean of 3.4 seconds (SD = 0.9, n = 128).

Referring to Fig. 18, the steps for triggering the start of occlusion include sensing sinus pressure 150, determining local systolic peaks (maxima) and diastolic valleys (minima) 152, storing the maxima and minima 154, determining heart rate 156, fitting the stored data to exponential curves 158, predicting T_p 160, and deciding pump turn-on time 162 accordingly.

Referring to Fig. 19, the procedure of Fig. 1 is performed in the apparatus 170. Line 24 is connected to a pressure transducer 171 which detects the electrical signals representing coronary sinus pressure and delivers them to an amplifier 172 which in turn sends them to an A-to-D converter 174 which provides them to sample storage 176. A local max and min calculator 178 uses the stored samples to determine the local systolic maxima and diastolic minima and provides them to max and min storage 180. A heart rate calculator 181 uses the successive maximum to determine the heart rate HR which is delivered to parameter storage 182. A curve fitting calculator 184 simultaneously fits the stored max and min values to exponential curves and generates the values A_s , A_d , T_s , T_d and delivers them to parameter storage 182. $\hat{T}_p$ calculator 186 then calculates $\hat{T}_p$ from the stored parameters and delivers its value to a pump turn-on trigger 188. Trigger 188 triggers pump turn-on at a time corresponding to the value $\hat{T}_p$.

Other parameters may also be used as the basis for timing the start of occlusion. For example, the frequency spectrum of the coronary sinus pressure curve during occlusion is also useful in determining $\hat{T}_p$. For this purpose the $\hat{T}_p$ calculator 186 in Fig. 19 can be arranged to perform the appropriate Fourier analysis of the CSP data to derive a frequency spectrum, and to use the spectral information as one factor in calculating $\hat{T}_p$.

In addition to predicting $\hat{T}_p$, the information available from the CSP curve is useful in predicting, at the beginning of intermittent occlusion, the area of the heart tissue that is at risk of dying, and at later stages of intermittent occlusion, the size of the infarcted tissue.

The area at risk is correlated to (a) the maximum local diastolic valley on the CSP curve (e.g., valley 202, Fig. 7) measured at the early stages of a period of intermittent occlusion, (b) the maximum local systolic peak on the CSP curve (e.g., peak 204, Fig. 7) measured after occlusion is interrupted (at time t_i).

during the early stages of a period of intermittent occlusion, (c) the same as (a) but measured at the later stages of the intermittent occlusion period, and (d) the maximum local systolic peak on the CSP curve (e.g., peak, 206, Fig. 7) measured during occlusion at the later stages of the intermittent occlusion period.

The infarct size is correlated to (a) the same as (c) above but taken during the later stages of the period of intermittent occlusion, (b) the maximum local systolic peak during occlusion in the middle stages of a period of intermittent occlusion, (c) the maximum local systolic valley while occlusion is interrupted during the middle stages of a period of intermittent occlusion.

In one example of these correlations, 3 groups of dogs (28 in total) with myocardial infarction were investigated: Group I, 5 dogs with 6 hours of coronary artery occlusion (CAO); Group II, 11 dogs with 3 hours of CAO and 3 hours of reperfusion; Group III, 12 dogs with 3 hours of reperfusion. In all groups, intermittent sinus occlusion was performed, beginning at 15 minutes after CAO in Group I, 30 minutes after CAO in Group II, and 2.5 hours after CAO in Group III; and continuing in all groups during reperfusion. The maximum valley systolic and maximum peak diastolic pressures during occlusion and during the interruption of occlusion were measured shortly after the onset of intermittent occlusion (early stages), and 3 hours (middle stages) and 6 hours (later stages) thereafter. The actual area at risk (AR) and infarct size (IS) were measured using known dye solution and TTC techniques. The following correlations were demonstrated using linear and logistic stepwise regression:

$$\begin{aligned} \text{AR} = & -0.6 \text{ CSP Diastolic, During Occlusion (Early Stages)} \\ & -0.4 \text{ CSP Systolic, Occlusion Interrupted (Early Stages)} \\ & +0.3 \text{ CSP Diastolic, During Occlusion (Later Stages)} \\ & +0.1 \text{ CSP Systolic, During Occlusion (Later Stages)} \\ & +34.5 \end{aligned}$$

$$r = 0.8 \quad p = 0.001$$

$$\begin{aligned} \text{IS} = & +1.4 \text{ CSP Diastolic, During Occlusion (Later Stages)} \\ & -0.6 \text{ CSP Systolic, During Occlusion (Middle Stages)} \\ & -0.9 \text{ CSP Systolic, Occlusion Interrupted (Middle Stages)} \\ & +43.8 \end{aligned}$$

$$r = 0.6 \quad p = 0.05$$

Referring to Fig. 20, the procedure for deriving IS and AR values is the same as the one shown in Fig. 18 up to the point of storing the local maxima and minima except that we now also store maxima and minima for the period after interruption of occlusion. Next IS and AR are calculated 210 and then displayed 212 for analysis. Similarly, referring to Fig. 21, the apparatus is similar to that of Fig. 19 but also includes an IS and AR calculator 214 that receives its input from the min and max storage 180 and a display 216 for displaying the AR and IS values.

Claims

1. **Apparatus** (10) for intermittently occluding a coronary sinus, comprising
 - means for occluding said sinus, and
 - a controller (28) having
 - means for providing trigger signals to said occluding means
 - to trigger an occlusion and
 - to interrupt said occlusion,

characterized by

 - a pressure transducer (50) for
 - sensing the fluid pressure within said sinus during said occlusion and

- providing corresponding fluid pressure signals, and
- said controller (28) being arranged
 - to trigger the initiation of the next said occlusion
 - at a time based on said fluid pressure signals.

5

2. Apparatus (10) of claim 1,
characterized in that

- said controller (28) triggers said initiation on the basis of
- successive pressure maxima of said fluid pressure signals.

10

3. Apparatus (10) of claim 1,
characterized in that

- said controller (28) triggers said initiation on the basis of
- successive pressure minima of said fluid pressure signals.

15

4. Apparatus (10) of claim 1,
characterized in that

- said controller (28) triggers said initiation on the basis of
- a combination of parameters derived from
- successive pressure maxima and minima of said fluid pressure signals.

20

5. Apparatus (10) of claim 4,
characterized in that

- said controller (28) triggers said initiation on the basis of
- fitting said pressure maxima and said pressure minima
- to exponential curves.

25

6. Apparatus (10) of claim 4,
characterized in that

- said parameters include
- heart rate.

30

7. Apparatus (10) of claim 5,
characterized in that

- said parameters include
- the asymptotic plateaus of said exponential curves.

35

8. Apparatus (10) of claim 5,
characterized in that

- said parameters include
- the time constants of said exponential curves.

40

Patentansprüche

1. Vorrichtung (10) für intermittierende Okklusion des Sinus coronarius, mit

- einer Okklusions-Einrichtung zur Okklusion des Sinus und
- einer Steuer-Einrichtung (28) mit
 - Mitteln zur Abgabe von Auslöse-Signalen an die Okklusions-Einrichtung
 - zum Auslösen einer Okklusion und
 - zum Unterbrechen der Okklusion,

45

50

gekennzeichnet durch

- einen Druck-Meßwertumformer (50) zur
- Erfassung des Flüssigkeits-Drucks im Sinus während der Okklusion und
- Abgabe entsprechender Flüssigkeits-Druck-Signale, und
- Ausbildung der Steuer-Einrichtung (28)
 - zum Auslösen der Einleitung der nächsten Okklusion
 - zu einem Zeitpunkt aufgrund der Flüssigkeits-Druck-Signale.

55

2. Vorrichtung (10) nach Anspruch 1,
gekennzeichnet dadurch, daß
 - die Steuer-Einrichtung (28) die Einleitung auslöst aufgrund
 - aufeinanderfolgender Druck-Maxima der Flüssigkeits-Druck-Signale.
- 5 3. Vorrichtung (10) nach Anspruch 1,
gekennzeichnet dadurch, daß
 - die Steuer-Einrichtung (28) die Einleitung auslöst aufgrund
 - aufeinanderfolgender Druck-Minima der Flüssigkeits-Druck-Signale.
- 10 4. Vorrichtung (10) nach Anspruch 1,
gekennzeichnet dadurch, daß
 - die Steuer-Einrichtung (28) die Einleitung auslöst aufgrund
 - einer Kombination von Parametern, abgeleitet aus
 - 15 - aufeinanderfolgenden Druck-Maxima und -Minima der Flüssigkeits-Druck-Signale.
5. Vorrichtung (10) nach Anspruch 4,
gekennzeichnet dadurch, daß
 - die Steuer-Einrichtung (28) die Einleitung auslöst aufgrund
 - 20 - Näherung der Druck-Maxima und -Minima
 - durch Exponential-Kurven.
6. Vorrichtung (10) nach Anspruch 4,
gekennzeichnet dadurch, daß
 - 25 - zu den Parametern gehört
 - der Herz-Schlag.
7. Vorrichtung (10) nach Anspruch 5,
gekennzeichnet dadurch, daß
 - 30 - zu den Parametern gehören
 - die asymptotischen Plateaus der Exponential-Kurven.
8. Vorrichtung (10) nach Anspruch 5,
gekennzeichnet dadurch, daß
 - 35 - zu den Parametern gehören
 - die Zeit-Konstanten der Exponential-Kurven.

Revendications

- 40 1. **Appareil** (10) pour occlusion intermittente du sinus coronaire, comprenant
 - des moyens pour occlusion dudit sinus, et
 - un controlleur (28) ayant
 - des moyens pour fournir des signaux de déclenchement aux dits moyens pour occlusion
 - pour déclencher une occlusion et
 - 45 - pour interrompre ladite occlusion,*caractérisé par*
 - un transducteur de pression (50) pour
 - detecter la pression du fluide à l'intérieur dudit sinus durant ladite occlusion et
 - fournir des signaux correspondants à la pression du fluide, et
 - 50 - ledit controlleur (28) étant arrangé
 - pour déclencher l'initiation de ladite prochaine occlusion
 - en un temps basé sur lesdits signaux de pression du fluide.
- 55 2. Appareil (10) selon la revendication 1,
caractérisé en ce que
 - ledit controlleur (28) déclenche ladite initiation sur la base de
 - maximums de pression successifs desdits signaux de pression du fluide.

3. Appareil (10) selon la revendication 1,

caractérisé en ce que

- ledit contrôleur (28) déclenche ladite initiation sur la base de
- minimums de pression successifs desdits signaux de pression du fluide.

5

4. Appareil (10) selon la revendication 1,

caractérisé en ce que

- ledit contrôleur (28) déclenche ladite initiation sur la base
- d'une combinaison de paramètres dérivés de
- maximums et minimums successifs de pression desdits signaux de pression de fluide.

10

5. Appareil (10) selon la revendication 4,

caractérisé en ce que

- ledit contrôleur (28) déclenche ladite initiation sur la base de
- l'ajustement desdits maximums et minimums de pression
- à des courbes exponentielles.

15

6. Appareil (10) selon la revendication 4,

caractérisé en ce que

- lesdits paramètres comprennent
- le rythme cardiaque.

20

7. Appareil (10) selon la revendication 5,

caractérisé en ce que

- lesdits paramètres comprennent
- les plateaux asymptotiques desdites courbes exponentielles.

25

8. Appareil (10) selon la revendication 5,

caractérisé en ce que

- lesdits paramètres comprennent
- les constantes de temps desdites courbes exponentielles.

30

35

40

45

50

55

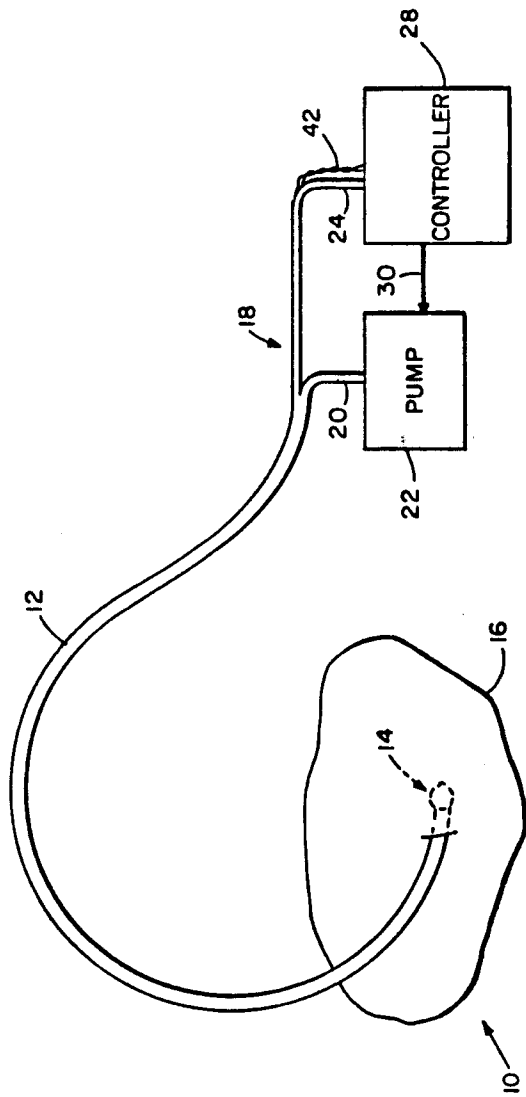


FIG. 1

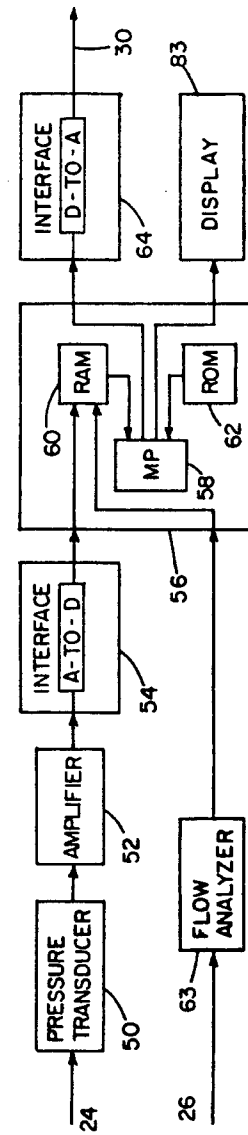
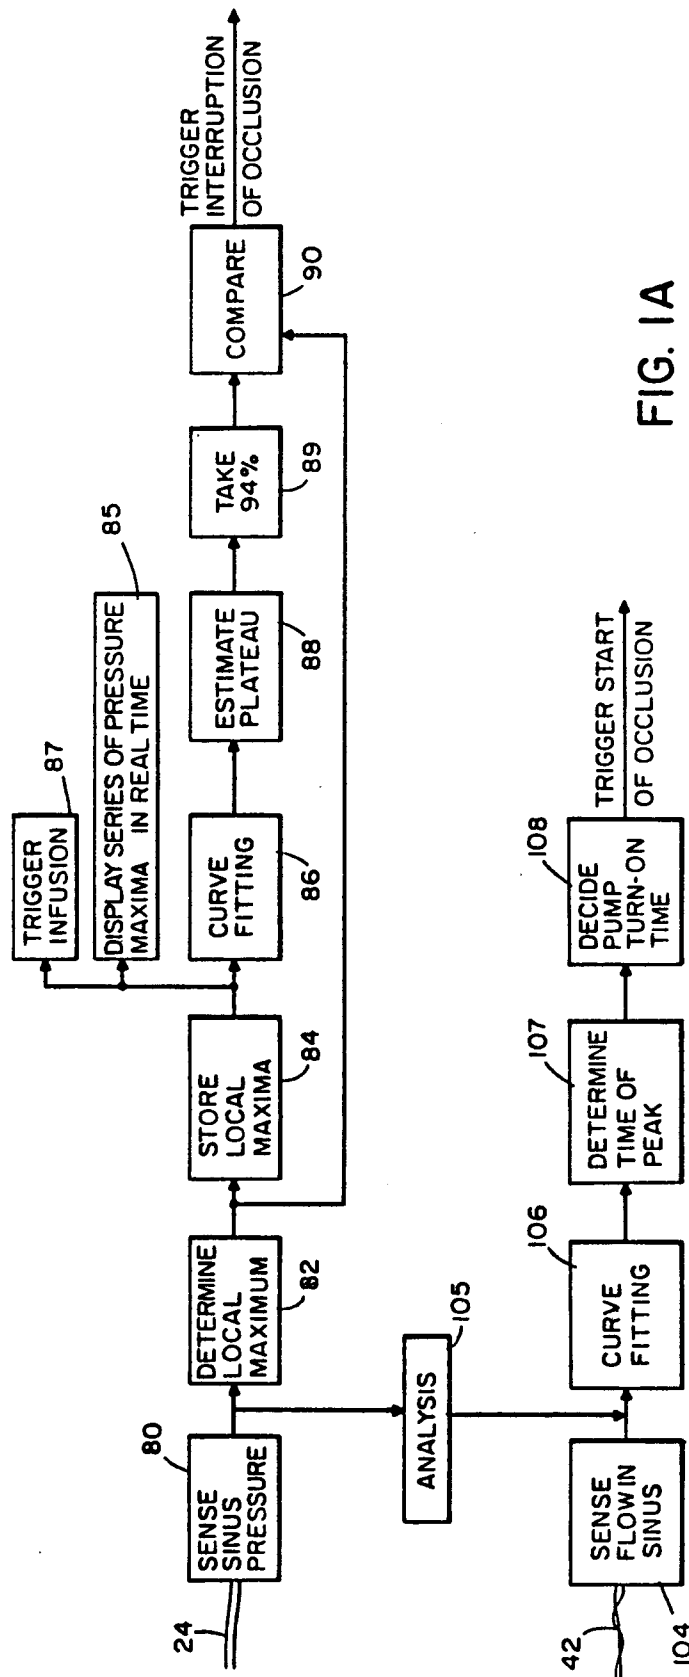


FIG. 3



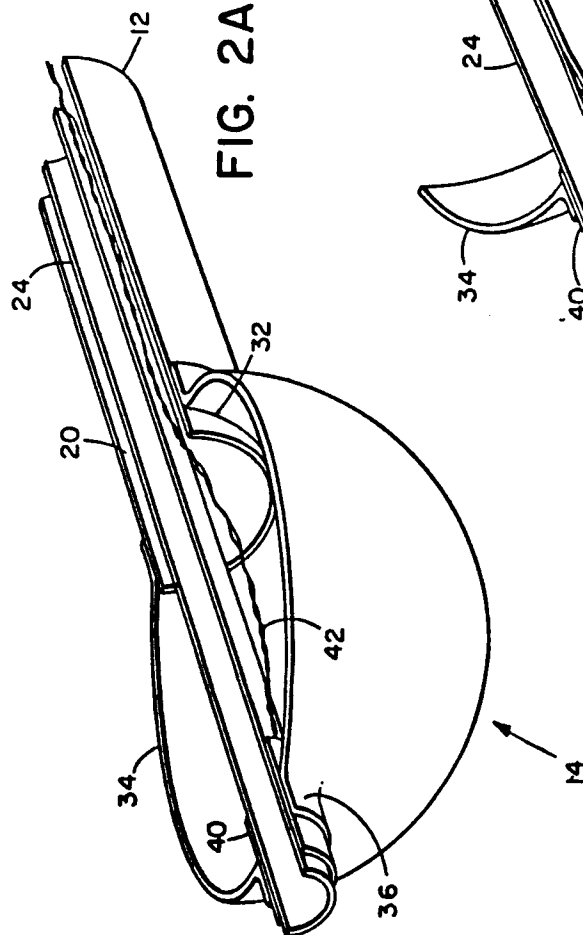


FIG. 2A

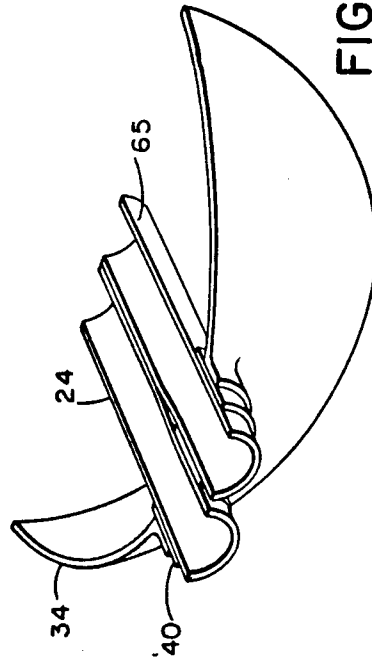
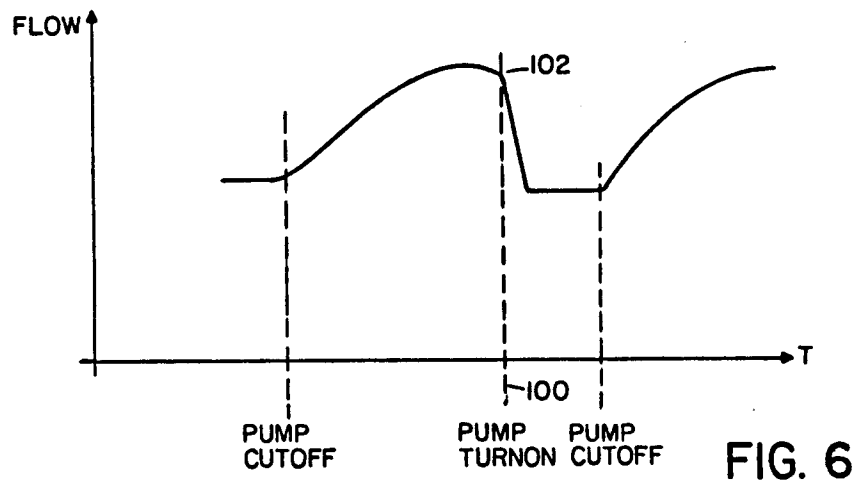
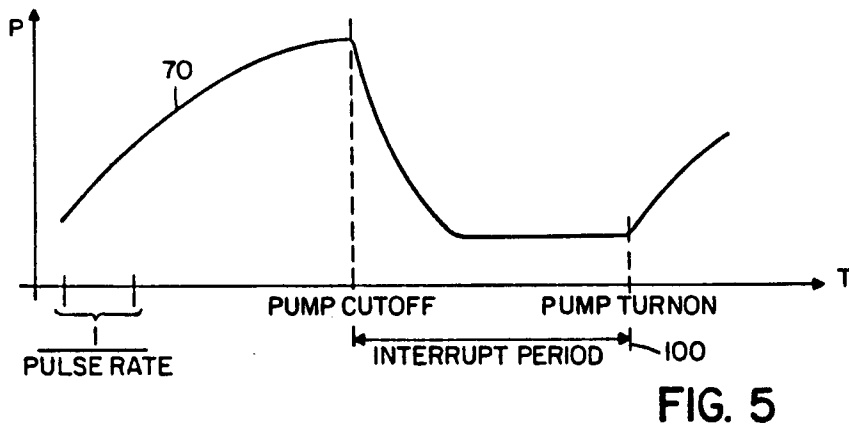
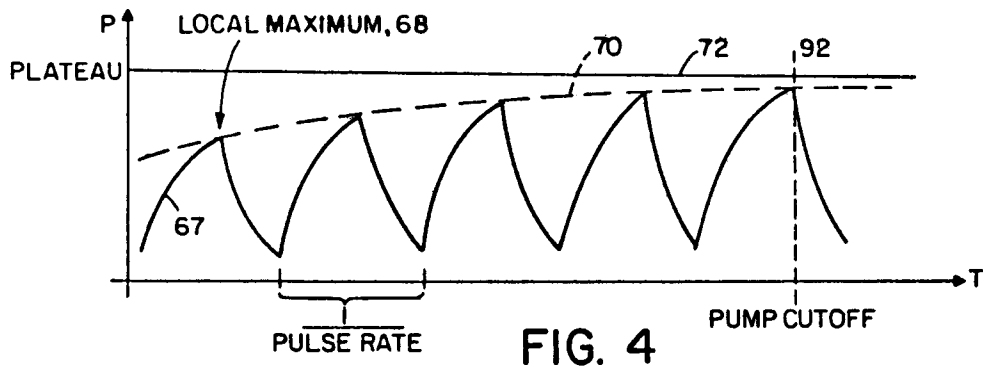


FIG. 2B



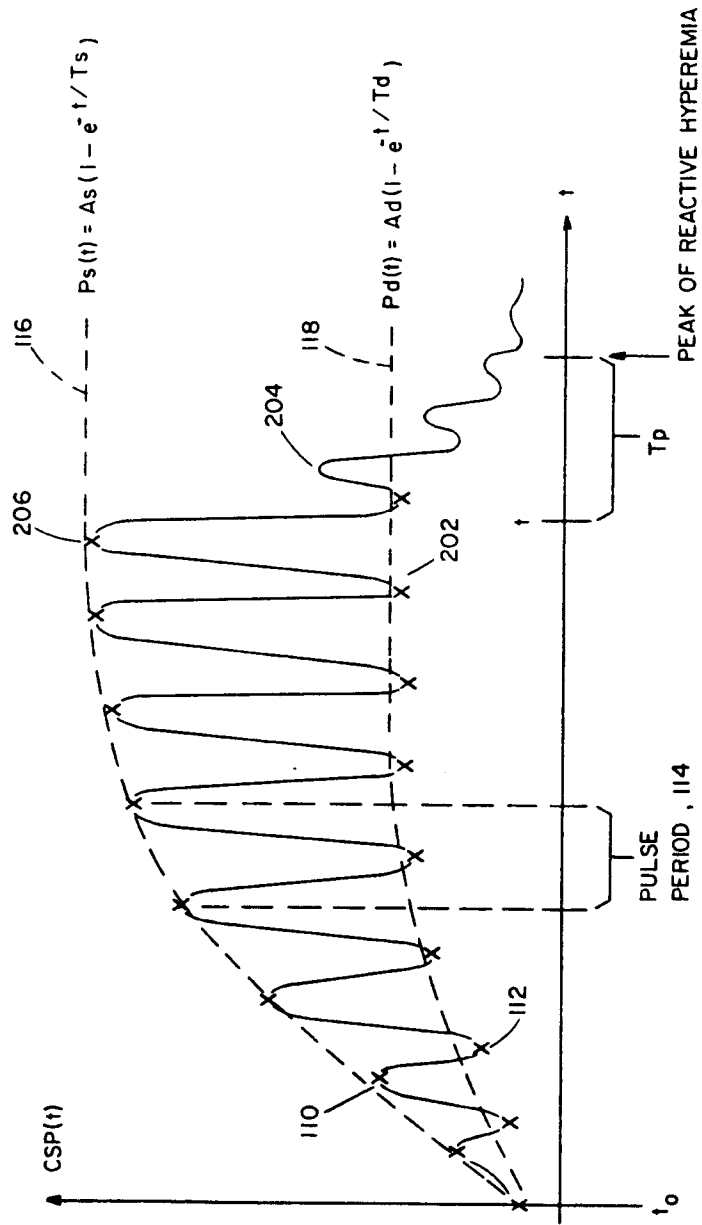


FIG 7

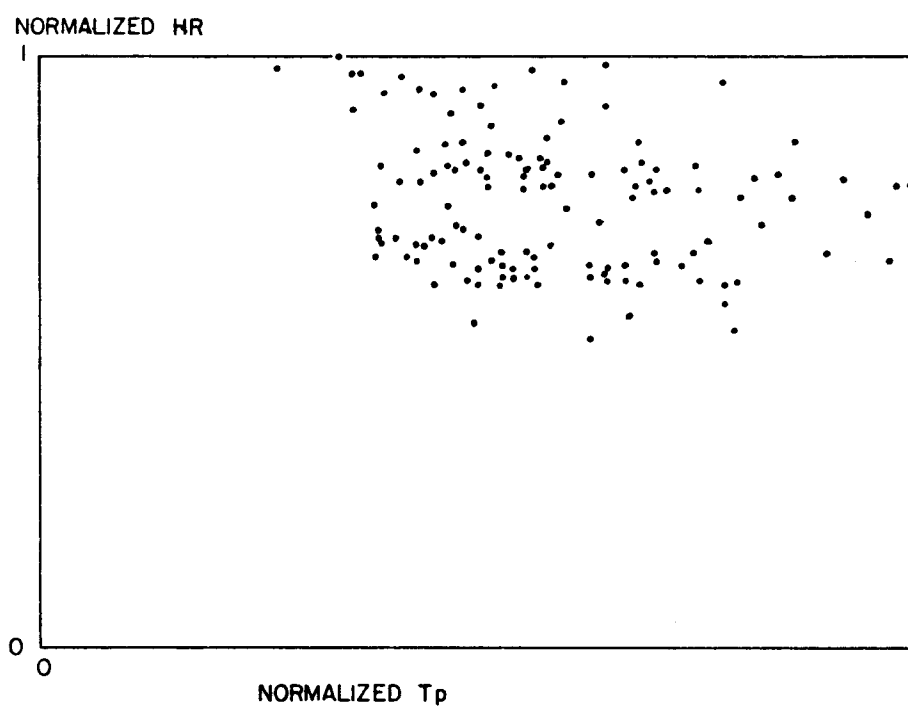


FIG 8

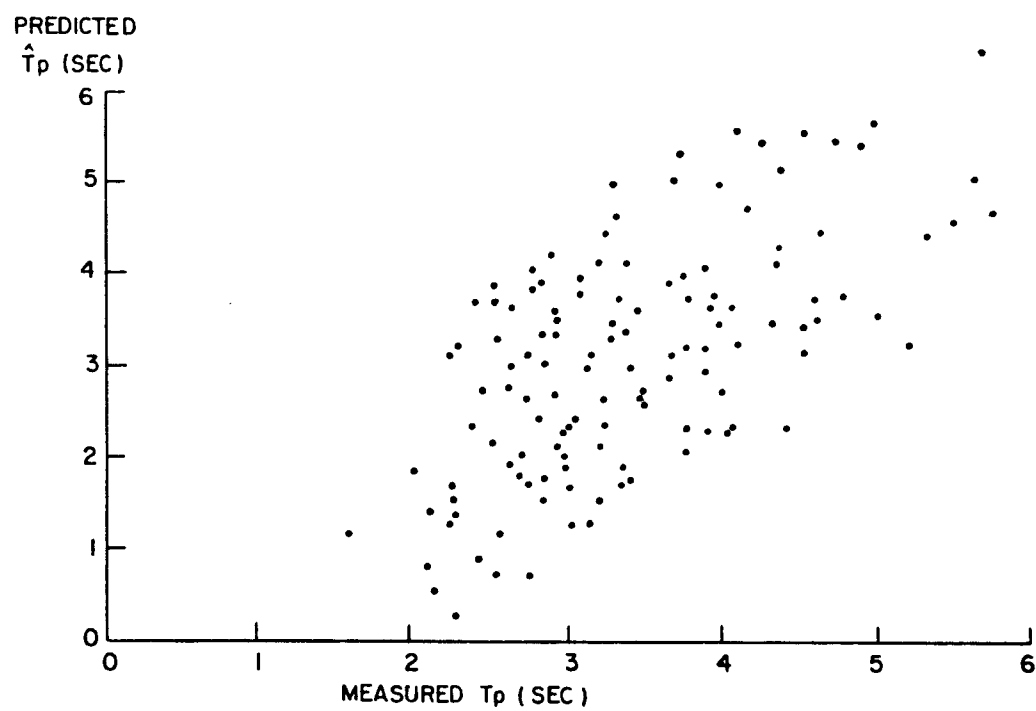


FIG 17

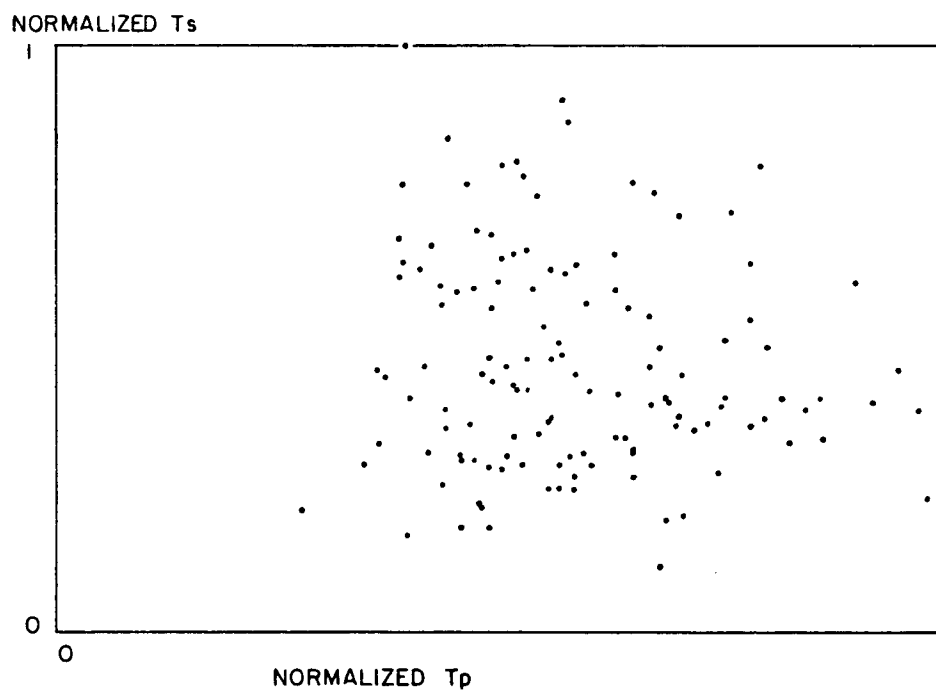


FIG 9

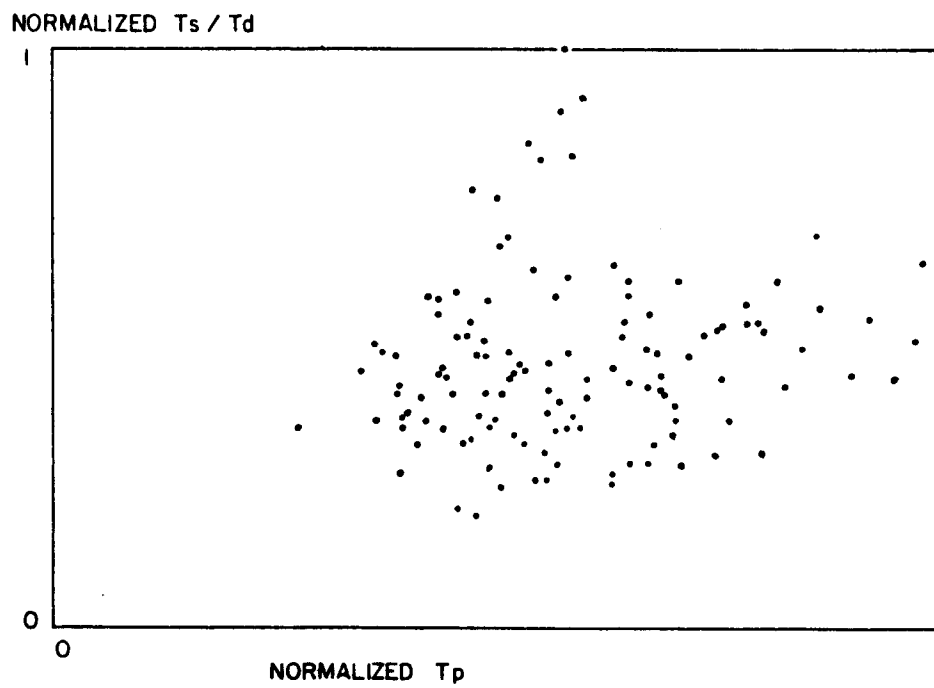


FIG 10

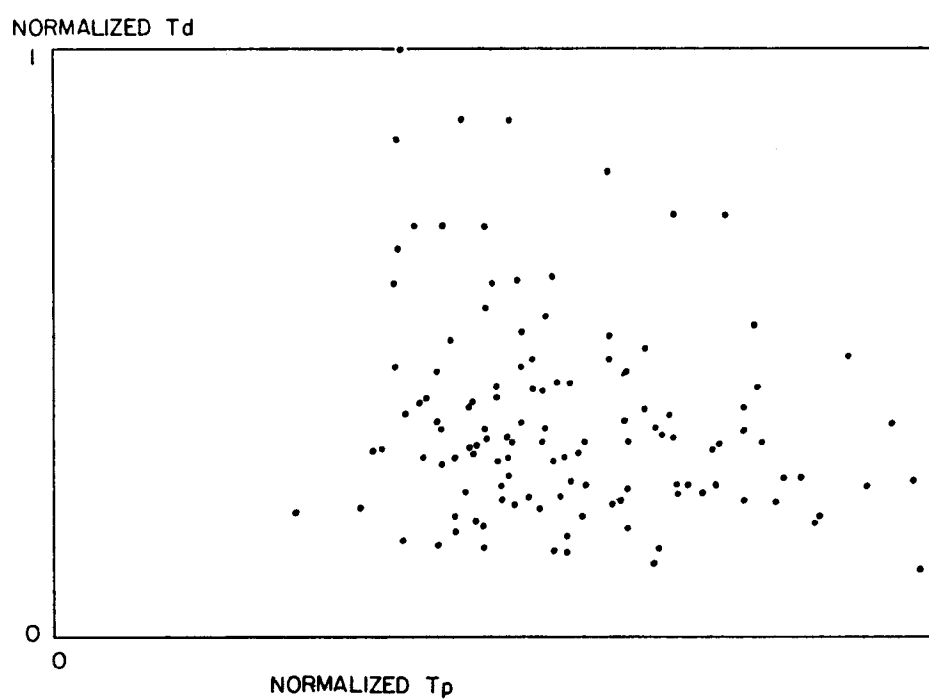


FIG 11

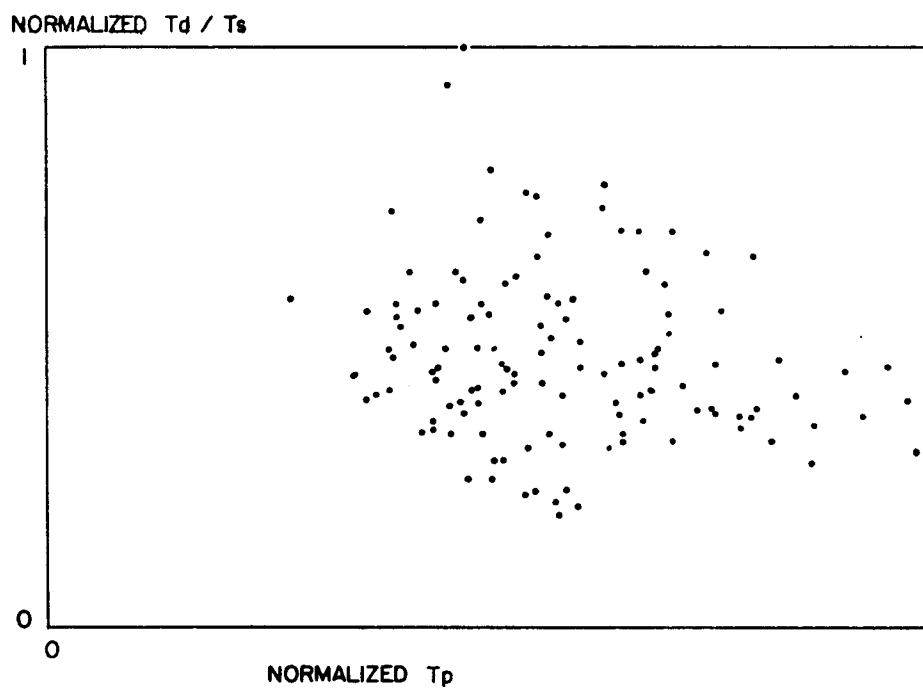


FIG 12

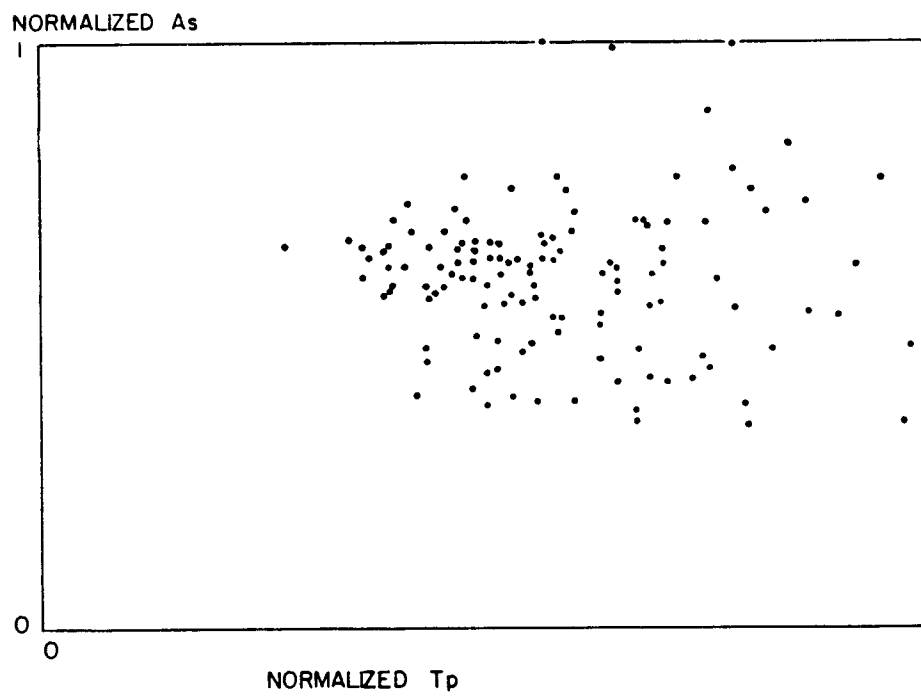


FIG 13

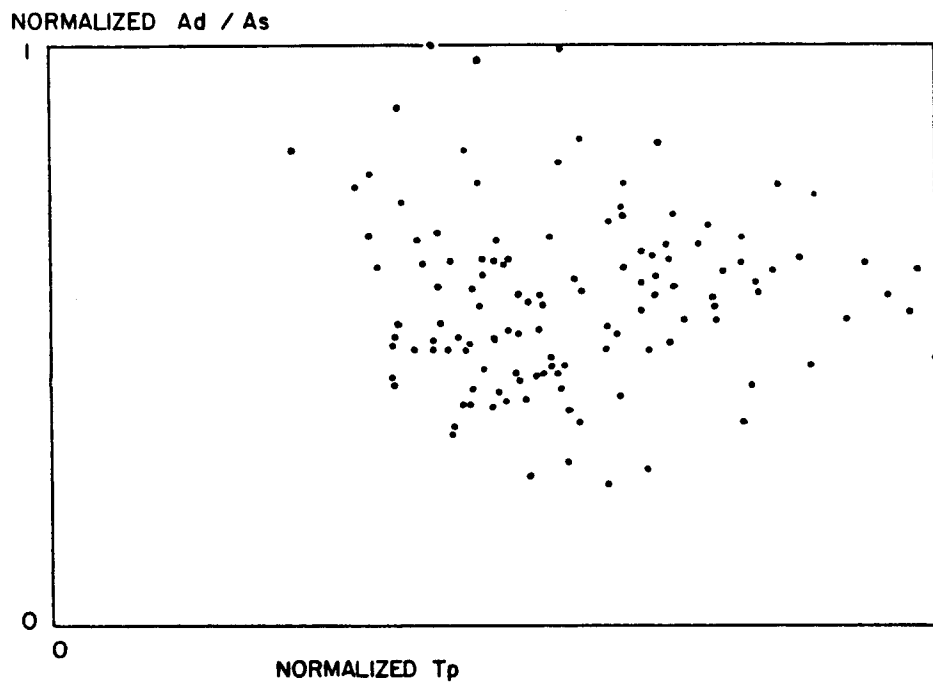


FIG 14

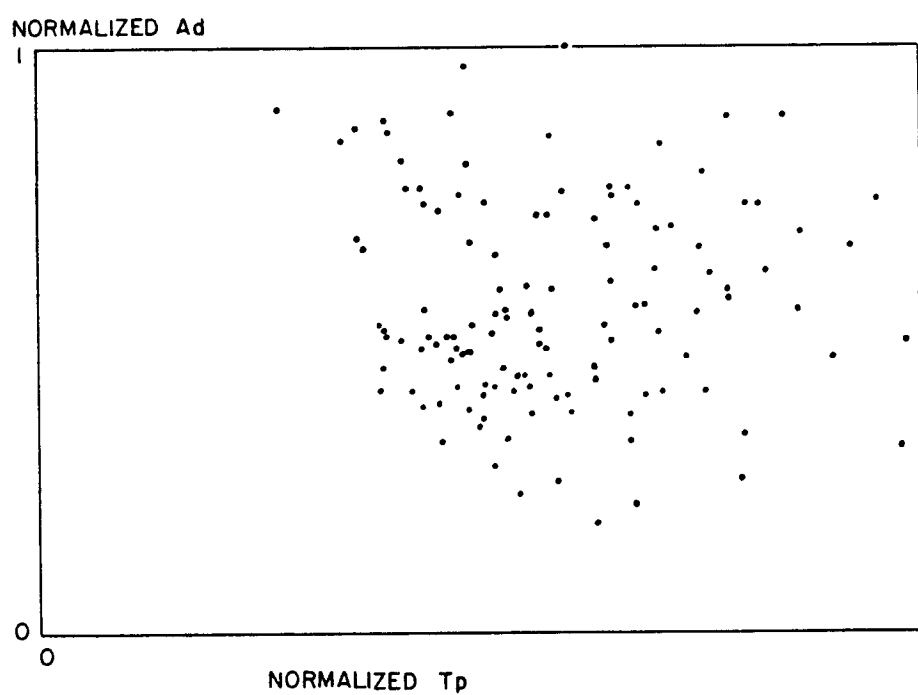


FIG 15

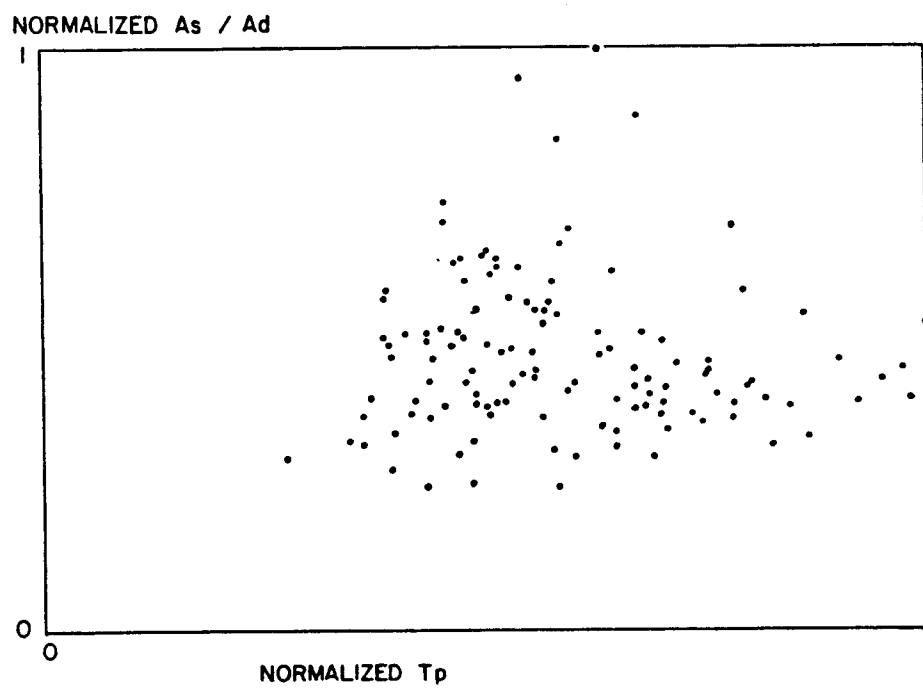


FIG 16

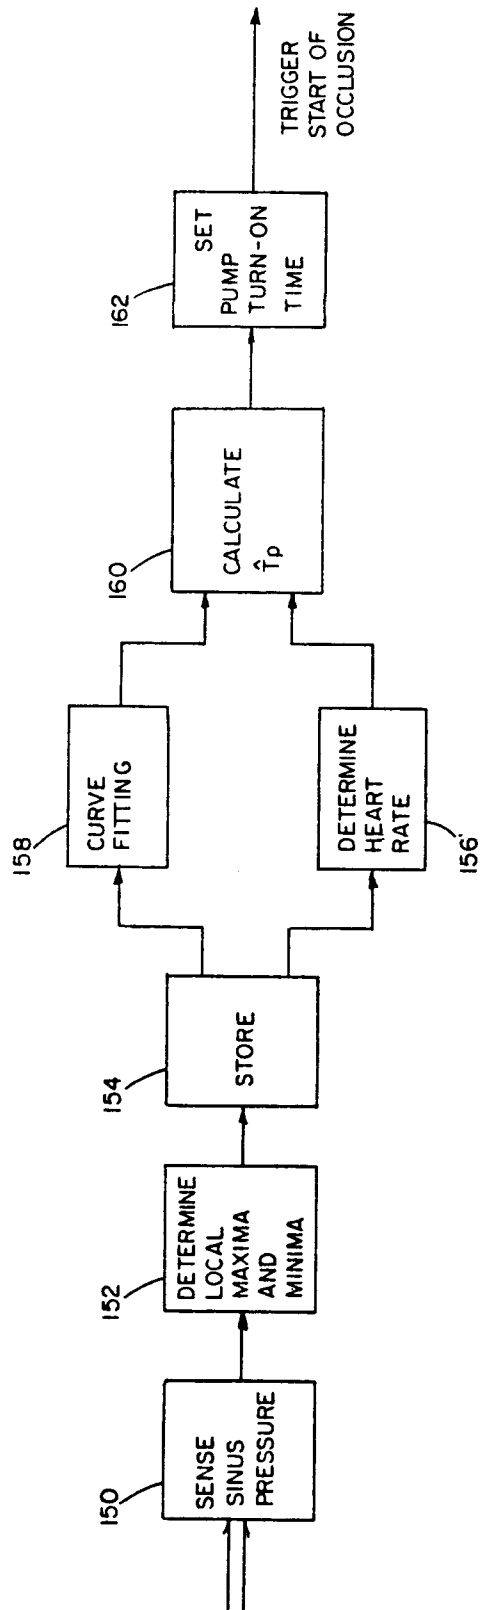


FIG 18

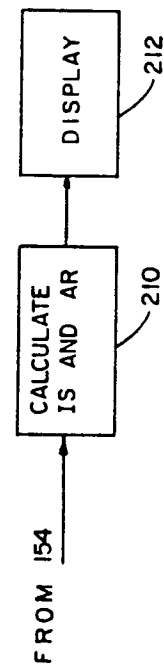


FIG 20

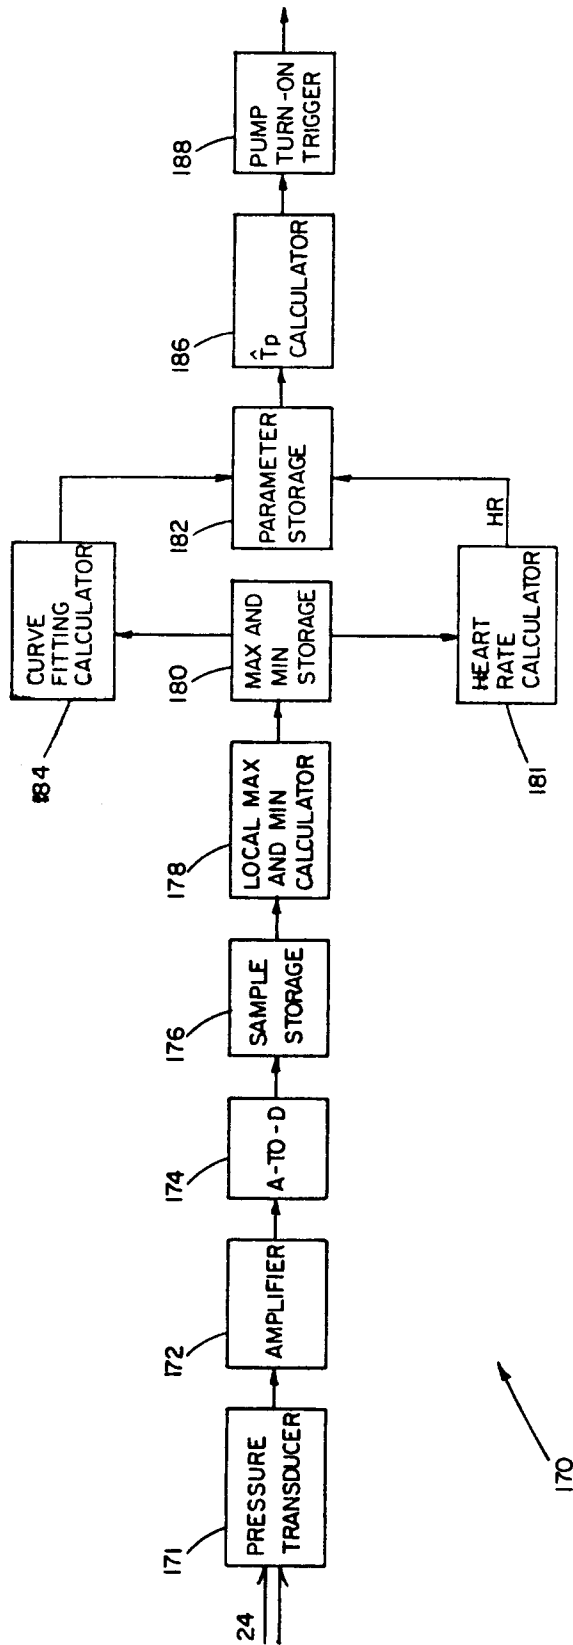


FIG 19

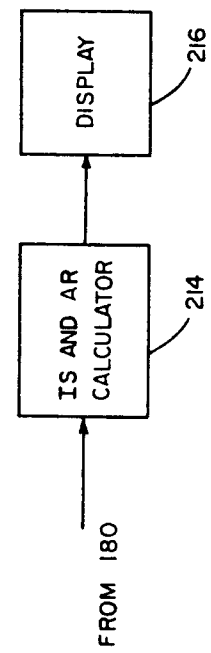


FIG 21