



(86) Date de dépôt PCT/PCT Filing Date: 2002/05/13
(87) Date publication PCT/PCT Publication Date: 2002/11/21
(45) Date de délivrance/Issue Date: 2011/07/05
(85) Entrée phase nationale/National Entry: 2003/11/13
(86) N° demande PCT/PCT Application No.: FR 2002/001595
(87) N° publication PCT/PCT Publication No.: 2002/091916
(30) Priorité/Priority: 2001/05/15 (FR01/06389)

(51) Cl.Int./Int.Cl. *A61B 1/267* (2006.01),
A61B 1/24 (2006.01), *A61B 5/103* (2006.01)


(72) Inventeurs/Inventors:
DEMATTEIS, MAURICE, FR;
PEPIN, JEAN-LOUIS, FR;
LEVY, PATRICK, FR

(73) Propriétaire/Owner:
UNIVERSITE JOSEPH FOURIER, FR

(74) Agent: ROBIC

(54) Titre : EMBOUT DESTINE A UN DISPOSITIF D'EVALUATION DE LA SENSIBILITE DU PHARYNX ET DISPOSITIF
LE COMPORTANT

(54) Title: MOUTHPIECE INTENDED FOR A DEVICE USED TO ASSESS THE SENSITIVITY OF THE PHARYNX AND A
DEVICE COMPRISING SAME

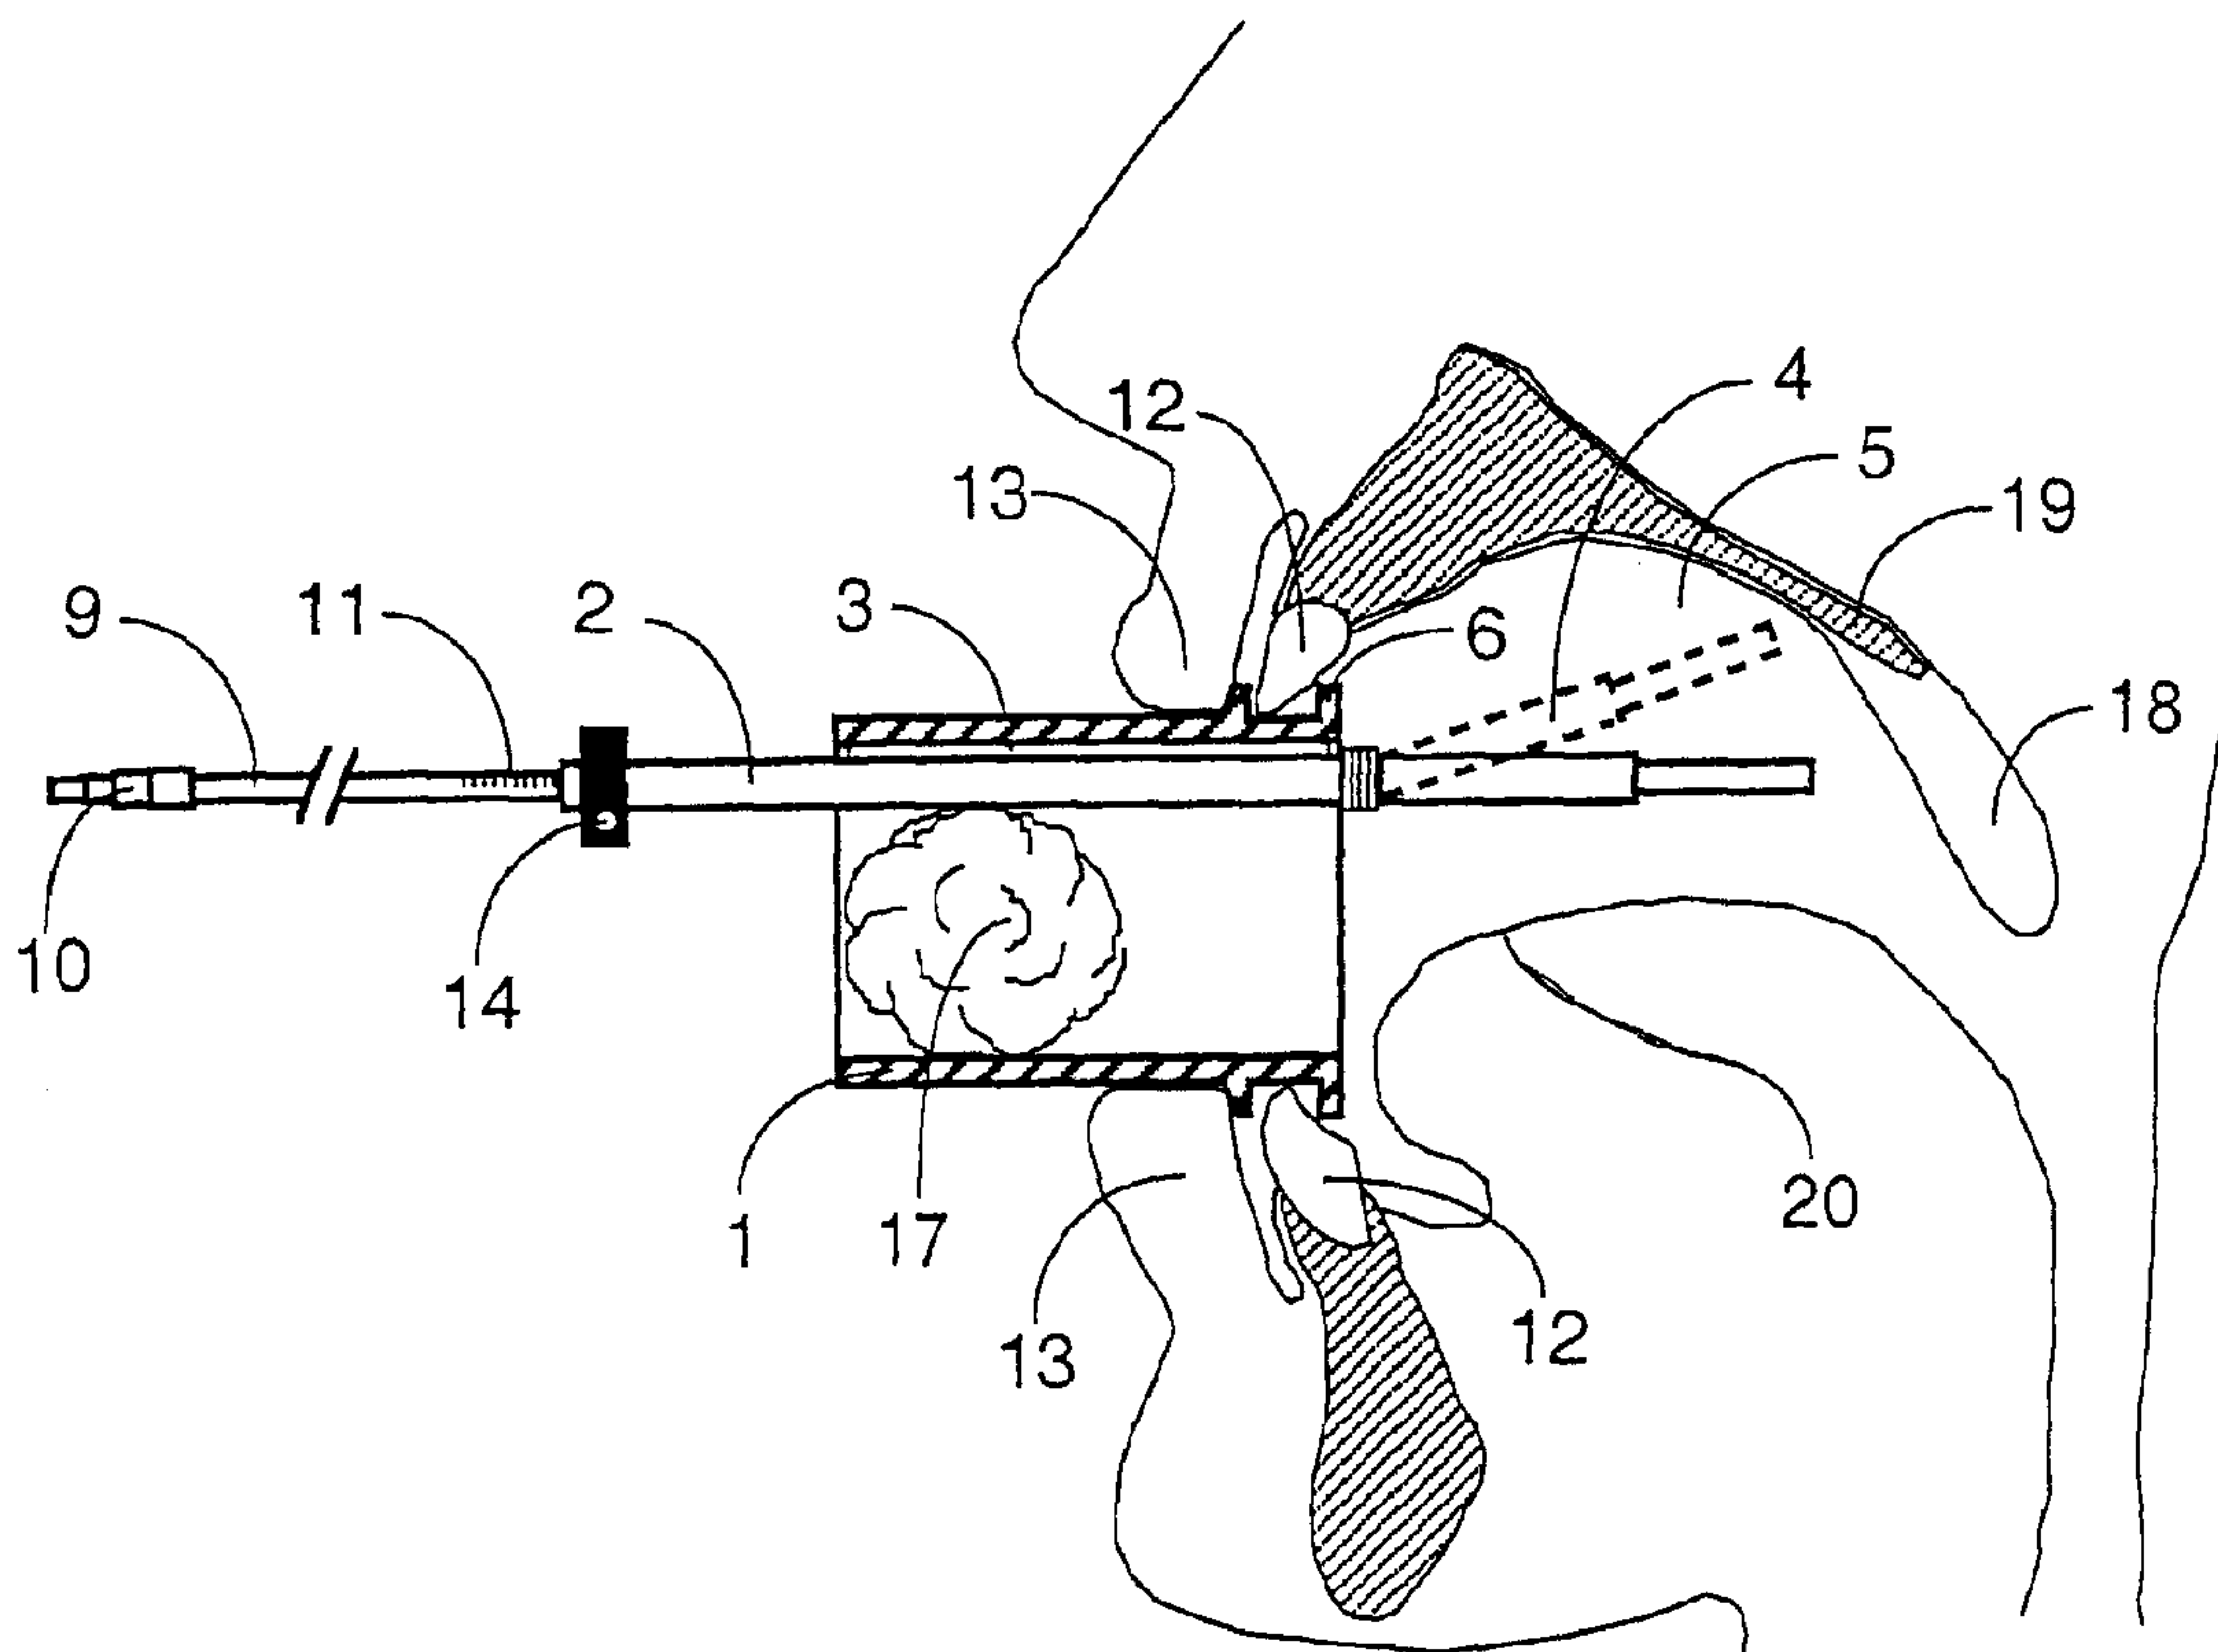

(57) **Abrégé(suite)/Abstract(continued):**

subject's mouth. A pipe (9) is introduced into the guide tube by means of the mouthpiece, under observation, until it touches the subject's palate. A measurement scale (1), which is disposed on the tube opposite the second end of the guide tube, is observed and the tube is subsequently withdrawn over a pre-determined distance, e.g. pulled out by 1 cm, and fixed in said position on the guide tube. A variable gas flow is injected into the pipe and reaches the pharyngeal mucous situated opposite the pipe. The sensitivity of the subject's pharynx, measured using the sensitive perception threshold, is determined using the lowest flow value perceived by the subject.

